



- (51) **International Patent Classification:**
A61B 17/072 (2006.01) *A61B 17/068* (2006.01)
- (21) **International Application Number:**
PCT/CN2014/093563
- (22) **International Filing Date:**
11 December 2014 (11.12.2014)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (71) **Applicant:** COVIDIEN LP [US/US]; 15 Hampshire Street, Mansfield, Massachusetts 02048 (US).
- (71) **Applicant (for MG only):** COVIDIEN (CHINA) MEDICAL DEVICES TECHNOLOGY CO., LTD. [CN/CN]; Rooms 501, No.3 Building, No. 2388, Chen Hang Road, Minhang District, Shanghai 201114 (CN).
- (72) **Inventors:** CAI, Longsheng; Room 502 No. 18, Building 359, Puxiu Road, Minhang District, Shanghai 201112 (CN). ZHANG, Xiliang; Room 601 No. 2, Lane 1122 Qinchun Road, Minhang District, Shanghai 201199 (CN). WANG, Zhaokai; Room 239 Mechanical Institute, #516 Jungong Road, Yangpu District, Shanghai 200093 (CN).
- (74) **Agent:** CCPIT PATENT AND TRADEMARK LAW OFFICE; 8th Floor, Vantone New World Plaza, 2

Fuchengmenwai Street, Xicheng District, Beijing 100037 (CN).

- (81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) **Title:** SURGICAL STAPLING LOADING UNIT

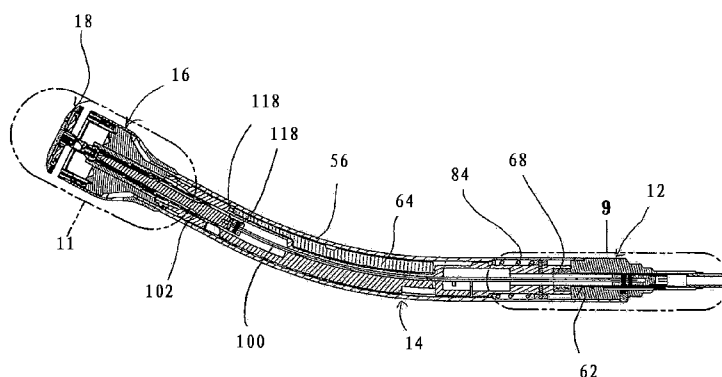


Fig. 8

(57) **Abstract:** A surgical loading unit (10) for use with a surgical handle assembly (1000) includes a handle mount (12) dimensioned for mounting to the handle assembly (1000), an outer member (56) extending from the handle mount (12), a staple cartridge assembly (16) mounted to the distal end of the outer member (56), and an anvil assembly (18) couplable relative to the staple cartridge assembly (16). A staple pusher (60) is at least partially disposed within the outer member (56) and operatively coupled to the staple cartridge assembly (16). The staple pusher (60) is adapted for longitudinal movement to eject staples from the staple cartridge assembly (16). An anvil approximator (94) is at least partially disposed within the outer member (56) and is operatively coupled to the anvil assembly (18). The anvil approximator (94) is adapted for movement between first and second positions corresponding to closed and open conditions of the anvil assembly (18) relative to the staple cartridge assembly (16). A lock member (24) is mounted to the handle mount (12). The lock member (12) is adapted to move from a lock position in secured engagement with the staple pusher (60) and the anvil approximator (94) to a release position releasing the staple pusher (60) and the anvil approximator (94) upon mounting of the handle mount (12) relative to the surgical handle assembly (1000).

SURGICAL STAPLING LOADING UNIT

BACKGROUND

1. Technical Field

[0001] The present disclosure relates to a surgical stapling loading unit for use with a surgical handle assembly. More particularly, the present disclosure relates to a stapling loading unit for use with a surgical handle assembly and having a lockout mechanism for retaining a staple pusher and an anvil approximator of the loading unit in their respective pre-fired positions until the loading unit is properly attached to the surgical handle assembly.

2. Background of Related Art

[0002] Surgical staplers for applying staples to tissue are well known. Such staplers include single use devices which are preloaded with one or more staples and are disposable after a single use. Multiple use devices are also available and are preloaded with a plurality of staples. These multiple use devices are disposable after the supply of staples has been exhausted or a surgical procedure has been completed. If the supply of staples is exhausted prior to completion of a surgical procedure, a new surgical stapler may be required to complete the surgical procedure. The use of additional surgical staplers for a single surgical procedure can be expensive.

[0003] In order to address the high expense of using multiple surgical staplers for a single procedure, surgical staplers with replaceable staple cartridges have been developed. In such surgical staplers, staples are housed within a cartridge. When the staples in the cartridge have been exhausted, the cartridge can be removed and replaced with a new cartridge having an additional supply of staples.

[0004] Covidien, LP, has manufactured and marketed stapling

systems having replaceable cartridges, such as the Multifire ENDO GIA™ 30 and Multifire ENDO GIA™ 60 systems, for a number of years. These systems include a surgical stapling handle assembly and a surgical loading unit. The loading unit may be a single use loading unit (SULU) or a multiple use loading unit (MULU). The loading unit includes a body and an end effector, and is attached to the handle assembly immediately prior to surgery. The end effector may include a cartridge which houses a plurality of staples. After use, the loading unit can be removed relative to the handle assembly and replaced with a new loading unit to perform additional stapling and/or cutting operations. A drive assembly is supported within the loading unit and is engagable with a control rod of the surgical handle assembly to control operation of the loading unit.

[0005] Although, these systems have provided significant clinical benefits, improvements are still possible. Accordingly, it would be desirable to provide an improved stapling loading unit for use in a surgical stapling system adapted to perform, e.g., a circular or end-to-end anastomosis, and which retains or locks the staple pusher assembly and/or the anvil approximator assembly in a pre-fired position until the loading unit is attached to the surgical handle assembly of the system.

SUMMARY

[0006] Accordingly, a surgical loading unit for use with a surgical handle assembly includes a handle mount dimensioned for mounting to the handle assembly, an outer member extending from the handle mount and having proximal and distal ends, a staple cartridge assembly mounted to the distal end of the outer member and having a plurality staples, and an anvil assembly couplable relative to the staple cartridge assembly. A staple pusher is at least

partially disposed within the outer member and is operatively coupled to the staple cartridge assembly. The staple pusher is adapted for longitudinal movement to eject the staples. An anvil approximator is at least partially disposed within the outer member and is operatively coupled to the anvil assembly. The anvil approximator is adapted for movement between first and second positions corresponding to closed and open conditions of the anvil assembly relative to the staple cartridge assembly. The loading unit further includes a lock member which is mounted to the handle mount. The lock member is adapted to move from a lock position in secured engagement with the staple pusher and the anvil approximator to a release position releasing the staple pusher and the anvil approximator upon mounting of the handle mount relative to the surgical handle assembly.

[0007] In embodiments, the lock member is adapted for rotational movement about the longitudinal axis to move from the lock position to the release position. In certain embodiments, a guide member having a guide channel arranged at an angle relative to the longitudinal axis is provided. The lock member may be at least partially received within the guide channel of the guide member and is adapted to traverse the channel during movement of the lock member from the lock position to the release position. In some embodiments, the lock member includes a lock tab and a channel tab. The lock tab is operatively engagable with the staple pusher and the anvil approximator when the lock member is in the lock position. The channel tab is received within the guide channel of the guide member and is adapted to traverse the channel.

[0008] In other embodiments, the guide member is adapted to move relative to the handle mount between a retracted position corresponding to the lock position of the lock member and an advanced position corresponding to the

release position of the lock member. The guide member may be normally biased toward the retracted position. A spring may be operatively engagable with the handle mount and the guide member, and dimensioned to normally bias the guide member to the retracted position. In some embodiments, the guide member is dimensioned to engage the handle assembly during mounting of the handle mount relative to the handle assembly causing movement of the guide member to the advanced position thereof.

[0009] In certain embodiments, the staple pusher includes a staple connector which is at least partially disposed within the handle mount, and incorporates a staple lock surface. The staple lock surface is engaged by the lock member when in the lock position of the lock member and released from the lock member when in the release position of the lock member. The staple pusher may be normally biased toward a proximal position thereof.

[0010] In other embodiments, the anvil approximator includes an anvil band which is at least partially disposed within the handle mount. The anvil band has an anvil lock surface which is engaged by the lock member when in the lock position of the lock member and released from the lock member when in the release position of the lock member.

[0011] In embodiments, the staple cartridge includes an annular array of staples and the anvil assembly includes an annular anvil head cooperable with the annular array of staples to perform a circular or an end-to-end anastomosis.

[0012] In another aspect of the present disclosure, a surgical system for performing a circular or an end-to-end anastomosis includes a handle assembly and a loading unit mountable to the handle assembly. The handle assembly includes a frame, a staple actuator and an anvil actuator each being at least partially disposed within the frame, and at least one manual member for actuating at least one of the staple actuator and the anvil actuator. The loading

unit includes a handle mount dimensioned for mounting to the frame of the handle assembly, an outer member extending from the handle mount and having proximal and distal ends, a staple cartridge assembly mounted to the distal end of the outer member, and an anvil assembly couplable relative to the staple cartridge assembly. The staple cartridge assembly includes a plurality of staples arranged in an annular array. The anvil assembly includes an anvil shaft and an anvil head. A staple pusher is at least partially disposed within the outer member and operatively coupled to the staple cartridge assembly. The staple pusher is adapted for longitudinal movement to eject the staples to be crimped by the anvil head. The staple pusher is couplable to the staple actuator of the handle assembly upon mounting of the handle mount to the frame whereby movement of the at least one manual member causes corresponding movement of the staple pusher. An anvil approximator is at least partially disposed within the outer member and operatively coupled to the anvil assembly. The anvil approximator is adapted for movement between first and second positions corresponding to closed and open conditions of the anvil assembly relative to the staple cartridge assembly. The anvil approximator is couplable to the anvil actuator of the handle assembly upon mounting of the handle mount to the frame whereby movement of the at least one manual member causes corresponding movement of the anvil approximator between the first and second positions. The loading unit further includes a lockout mechanism which is mounted to the handle mount. The lockout mechanism includes a lock member and a guide member. The guide member is engagable with the frame of the handle assembly upon mounting of the handle mount to the frame to cause the lock member to rotate about the longitudinal axis from a lock position where the lock member is in secured engagement with the staple pusher and the anvil approximator, to a release position where the lock member releases the staple pusher and the anvil

approximator.

[0013] In some embodiments, the guide member is adapted to move relative to the handle mount between a retracted position corresponding to the lock position of the lock member and an advanced position corresponding to the release position of the lock member. In certain embodiments, the lock member includes a channel tab and a locking tab. The locking tab is engagable with the staple pusher and with the anvil approximator when in the lock position of the lock member. The channel tab may be received within a guide channel defined within the guide member, and traverses the guide channel upon movement of the guide member between the retracted position and the advanced position. In some embodiments, the guide member is normally biased toward the retracted position thereof and the staple pusher is normally biased toward a proximal position thereof.

BRIEF DESCRIPTION OF THE DRAWINGS

[0014] Embodiments of the present disclosure will be readily appreciated by reference to the drawings wherein:

[0015] FIG.1 is a perspective view of a surgical loading unit for performing a surgical stapling procedure in accordance with the principles of the present disclosure;

[0016] FIG.2 is a side plan view of the surgical loading unit mounted to a surgical handle assembly;

[0017] FIG.3 is an exploded perspective view of the surgical loading unit;

[0018] FIG.4 is an isolated view of the area of detail identified in FIG.3 illustrating components of the handle mount of the surgical loading unit;

[0019] FIG.5 is a perspective view of the lock member of the handle

mount;

[0020] FIG.6 is a perspective view with portions removed of the handle mount of the surgical loading unit illustrating the lock member in a lock position;

[0021] FIG.7 is a perspective view of the handle mount illustrating the lock member in a release position;

[0022] FIG.8 is a side cross-sectional view of the surgical loading unit;

[0023] FIG.9 is an isolated view of the area of detail identified in FIG.8 illustrating a first side cross-sectional view of the handle mount with the lock member in the lock position;

[0024] FIG.10 is a second side cross-sectional view of the handle mount with the lock member in the lock position;

[0025] FIG.11 is an isolated view of the area of detail identified in FIG.8;

[0026] FIG.12 is an isolated view of the area of detail identified in FIG.3 illustrating the locking tabs of the anvil bands;

[0027] FIG.13 is a perspective view of the staple cartridge assembly;

[0028] FIG.14 is a cross-sectional view taken along the lines 14-14 of FIG.6 illustrating the lock member in the lock position in secured engagement with the staple pusher and the anvil approximator;

[0029] FIG.15A is a side plan view illustrating mounting of the handle mount of the loading unit to the handle assembly;

[0030] FIG.15B is an enlarged isolated view of the area of detail identified in FIG.15A;

[0031] FIG.15C is a view illustrating the handle mount mounted to the handle assembly and the guide member in the advanced position corresponding to the release position of the lock member;

[0032] FIG.16 is a cross-sectional view taken along the lines 16-16 of FIG.7 illustrating the lock member in the release position releasing the staple pusher and the anvil approximator;

[0033] FIG.17 is a perspective view of a portion of the handle mount illustrating the lock member in the release position;

[0034] FIG.18 is a side cross-sectional view of the loading unit with a segment of the surgical handle assembly in phantom, illustrating the anvil assembly in an open condition upon advancement of the anvil approximator;

[0035] FIG.19 is an isolated view of the area of detail of FIG.18; and

[0036] FIG.20 is a side cross-sectional view of the handle mount with a segment of the surgical handle assembly in phantom, illustrating the staple pusher advanced to fire the staples from the staple cartridge assembly.

DETAILED DESCRIPTION OF THE EMBODIMENT(S)

[0037] Particular embodiments of the present disclosure are described hereinbelow with reference to the accompanying drawings; however, it is to be understood that the disclosed embodiments are merely examples of the disclosure and may be embodied in various forms. Well-known functions or constructions are not described in detail to avoid obscuring the present disclosure in unnecessary detail. Therefore, specific structural and functional details disclosed herein are not to be interpreted as limiting, but merely as a basis for the claims and as a representative basis for teaching one skilled in the art to employ the present disclosure in virtually any appropriately detailed structure. Like reference numerals may refer to similar or identical elements throughout the description of the figures.

[0038] Referring now to the drawings where like reference numerals indicate similar components throughout the several views, FIGS.1-2 illustrate

the surgical loading unit in accordance with the principles of the present disclosure. In FIG.1, the surgical loading unit 10 is depicted in isolation while in FIG.2 the surgical loading unit 10 is depicted connected to a surgical handle assembly 1000. The surgical loading unit 10 and the surgical handle assembly 1000 form a surgical system adapted to perform a surgical procedure on tissue e.g., a circular or end-to-end anastomosis on tubular organs. The loading unit 10 may be a single use loading unit (SULU). It is also contemplated that the loading unit 10 may be a multi-use loading unit (MULU) adapted, e.g., for sequential firing of one or more staples.

[0039] The surgical handle assembly 1000 may be any handle assembly having at least one actuator, and in some embodiments, two actuators adapted to control operation of the loading unit 10. It is contemplated that the surgical handle assembly 1000 may be reusable, i.e., it can be reused with a plurality of loading units 10, and may be used with loading units having different stapling functions such as, e.g., linear stapling of tissue. Further details of the handle assembly 1000 and its interaction with the surgical loading unit 10 will be discussed in greater detail hereinbelow.

[0040] Referring now to FIGS.3-6, in conjunction with FIG.1, the surgical loading unit 10 will be discussed. The surgical loading unit 10 includes a handle mount 12 and an elongated segment 14 extending from the handle mount 12 and defining a longitudinal axis “k”. A staple cartridge assembly 16 and an anvil assembly 18 are each mounted relative to the elongated segment 14. The handle mount 12 includes a mount frame 20, a release or guide member 22 mounted to the mount frame 20 and a lock member 24 mounted relative to the guide member 22. The mount frame 20 defines a proximal mounting segment 26 of generally cylindrical configuration and a distal segment 28 also of general cylindrical configuration and defining a larger diameter than the proximal

mounting segment 26. The mount frame 20 defines a longitudinal passage 30 extending completely through the proximal mounting segment 26 and the distal segment 28. The proximal mounting segment 26 has diametrically opposed outer tabs 32 and an alignment tab 34 disposed at the proximal end of the mount frame 20. The opposed tabs 32 and the alignment tab 34 may cooperate with corresponding structure in the handle assembly 1000 to properly orient and secure the loading unit 10 relative to the handle assembly 1000, e.g., in a bayonet coupling relation. The mount frame 20 further includes a channeled groove 36 which receives the guide member 22. The channeled groove 36 terminates in a distal spring slot 38 defined within the distal segment 28 of the mount frame 20. The mount frame 20 also defines a keyed slot 40 extending through its distal face. A mount cover 42 is releasably couplable to the mount frame 20, and may be removed to permit assembly of the various components of the handle mount 12.

[0041] With reference to FIGS.3-7, the guide member 22 is adapted for reciprocal longitudinal movement relative to the mount frame 20 and within the channeled groove 36 between a retracted position (FIG.6) corresponding to a lock position of the lock member 24 and an advanced position (FIG.7) corresponding to a release position of the lock member 24. The guide member 22 includes a proximal guide tab 44, a cam slot 46 obliquely arranged with respect to the longitudinal axis “k” of the elongated segment 14 (FIG. 1) and a spring pin 48 extending from the distal end of the guide member 22. The proximal guide tab 44 engages corresponding structure within the handle assembly 1000 to move the guide member 22 in the direction of directional arrow “t” (FIG. 7) from the retracted position to the advanced position during linear insertion of the handle mount 12 within the handle assembly 1000. A coil spring 50 is at least partially mounted about the spring pin 48 and is disposed

within the distal spring slot 38 of the mount frame 20. The coil spring 50 biases the guide member 22 toward the retracted position depicted in FIG.6 thereby maintaining the lock member 24 in the lock position.

[0042] The lock member 24 is adapted for rotational movement about the longitudinal axis from the lock position (FIG.6) to the release position (FIG.7) to releasably secure the operating components in the elongated segment 14, i.e., the staple pusher and the anvil approximator, which respectively controls operation of the staple cartridge assembly 16 and the anvil assembly 18. As best depicted in FIGS.4 and 5, the lock member 24 includes a lock tab 52 and a channel boss 54. The lock tab 52 is operatively engagable with the operating components of the elongated segment 14 when the lock member 24 is in the lock position, e.g., prior to mounting the handle mount 12 to the handle assembly 1000, and releases the operating components when in the release position, e.g., when the handle mount 12 is mounted within the handle assembly 1000. The channel boss 54 is at least partially received within the cam slot 46 of the guide member 22. Upon movement of the guide member 22 from the retracted position (FIG.6) to the advanced position (FIG.7), the channel boss 54 traverses the cam slot 46 of the guide member 22, which causes the lock member 24 to rotate through a predetermined arc of rotation relative to the longitudinal axis “k” in the direction of directional arrow “b” (FIG.7) from its lock position to its release position. Further details of the operation of the lock member 24 will be discussed in greater detail hereinbelow.

[0043] With reference to FIGS.8-11, in conjunction with FIG.3, the elongated segment 14 includes an outer member 56, which in one embodiment, is in the form of an outer tube defining a longitudinal opening 56a (FIG. 3), and is mounted to the handle mount 12 through conventional arrangements. For example, the proximal end of the outer member 56 may be mounted about the

distal segment 28 of the handle mount 12 and secured via the use of adhesives, cements, fasteners, etc. The distal end of the outer member 56 may include a reduced diameter with opposed rectangular shaped windows 58 (FIG. 3) to assist in mounting the staple cartridge assembly 16 to the outer member 56.

[0044] Disposed within the outer member 56 is a staple pusher 60 including a staple connector 62 and a staple pusher tube 64 extending from the staple connector 62. The staple connector 62 is at least partially disposed within the longitudinal passage 30 of the handle mount 12 and incorporates a proximal cylindrical segment 66 and a distal collar segment 68. The proximal cylindrical segment 66 of the staple connector 62 includes a raised spline 70 (FIGS.3 and 10) which defines a staple lock surface in the form of a lock slot 72 through which the lock tab 52 of the lock member 24 extends when in the lock position of the lock member 24. During movement of the lock member 24 to the release position, the lock tab 52 traverses the lock slot 72 to be released from the spline 70 and permit distal longitudinal movement of the staple connector 62 and the staple pusher tube 64.

[0045] As best depicted in FIGS.9-10, the staple pusher tube 64 includes an alignment rod 74 which is received within the keyed slot 40 of the handle mount 12 to properly orient the staple pusher tube 64 relative to the handle mount 12. (see also FIG. 3) The proximal end of the staple pusher tube 64 defines a recess 76 which accommodates the distal collar segment 68 of the staple connector 62 to connect the two components. Adhesives and or cements may be used to securely fix the staple connector 62 and the staple pusher tube 64. The staple pusher tube 64 may include opposed wall segments or spacers 78 which couple to the main body 64a of the staple pusher tube 64 (FIG.3). In the alternative, the main body 64a and the wall spacers 78 may be monolithically formed. The staple pusher tube 64 further defines diametrically opposed locking tabs 80 at its

distal end which couple with the staple cartridge assembly 16 (see, e.g., FIGS.3 and 11).

[0046] Referring to FIGS.8-10, in conjunction with FIG.3, the stapler pusher 60 is normally spring biased toward a proximal position. In one embodiment, the outer member 56 includes a washer 82 residing in an internal shelf 83 of the outer member 56 and a coil spring 84 which engages the washer 82 at the distal end of the coil spring 84. The staple pusher 60 includes a lock ring 86 which is secured to the proximal cylindrical segment 66 of the staple connector 62 (FIG.3). The lock ring 86 includes lock pins 88 which extend through diametrically opposed openings 90 in the wall of the lock ring 86 and within aligned openings 92 in the wall of the staple connector 62 (FIG.3). The lock pins 88 may be secured within the openings 90, 92 with the use of adhesives, cements or the like. The coil spring 84 engages the lock ring 86 to normally bias the lock ring 86 and the staple pusher 60 in a proximal direction.

[0047] Referring to FIGS.8-11, an anvil approximator or drive 94 is at least partially disposed within the staple pusher 60 and the outer member 56. The anvil approximator 94 includes, from proximal to distal, an anvil sleeve 96, a connector 98 connected to the sleeve 96 and extending distally therefrom, a pair of elongate anvil bands 100 and an anvil retainer 102 coupled to the anvil bands 100. (see also FIG.3) The anvil sleeve 96 includes structure which operatively engages at least one actuator within the handle assembly 1000. As depicted in FIG.10, the structure may include a longitudinal opening 104 through which an anvil actuator of the handle assembly 1000 extends. The anvil sleeve 96 may define an internal shelf 105 or other coupling structure which engages with the anvil actuator of the handle assembly 1000. Other coupling mechanisms for coupling with the anvil actuator of the handle assembly 1000 are also envisioned.

[0048] The connector 98 defines first and second legs 98a, 98b with pairs of

opposed openings 106 extending through the walls of the legs 98a, 98b. (FIG. 3) The proximal ends of the anvil bands 100 are received within the legs 98a, 98b of the connector 98 and also define pairs of openings 108 which are in general alignment with the openings 106 of the connector 98. (See FIGS.3 and 12). A pair of pins 110 extends through the openings 106, 108 to couple the connector 98 with the anvil bands 100. At least one, e.g., both, of the anvil bands 100 include locking tabs 112 adjacent the proximal ends of the anvil bands 100. (FIG.12) The locking tabs 112 define anvil lock surfaces which are engaged by the lock tab 52 of the lock member 24 within the handle mount 12 to releasably secure the anvil approximator 94 in a first position which corresponds to a closed condition of the anvil assembly 18 relative to the staple cartridge assembly 16 (FIG.10). Upon movement of the lock member 24 to the release position, the lock tab 52 of the lock member 24 releases the locking tabs 112 of the anvil bands 100 to permit longitudinal movement of the anvil approximator 94 to a second position corresponding to an open condition of the anvil assembly 18.

[0049] With reference again to FIGS.3 and 8, the anvil retainer 102 includes a pair of retainer legs 114a, 114b with pairs of openings 116 extending through the retainer legs 114a, 114b. The distal ends of the anvil bands 100 are received within the retainer legs 114a, 114b and secured to the anvil retainer 102 via pins 118 which extend through the openings 116 in the legs 114a, 114b and the corresponding openings 120 defined within the anvil bands 100.

[0050] With reference now to FIGS.11 and 13, in conjunction with FIG. 3, the staple cartridge assembly 16 will be discussed. The staple cartridge assembly 16 includes an outer shell 122, an annular staple pusher ring 124, a cylindrical knife 126 and a staple guide 128. In FIG.13, the outer shell 122 is removed for illustrative purposes. The outer shell 122 is mounted to the outer

member 56 through cooperative engagement of shell locking detents 130 of the outer shell 122 with the rectangular shaped windows 58 of the outer member 56. (FIG.3) The outer member 56 may define a reduced diameter which receives the shell 122 to maintain a substantial constant diameter through most of the length of the elongated segment 14. The pusher ring 124 includes a pair of locking legs 132 at its proximal end. The locking legs 132 include openings 134 which receive the locking tabs 80 of the staple pusher tube 64 to couple the staple pusher 60 with the staple pusher ring 124. Thus, movement of the staple pusher 60 causes corresponding movement of the staple pusher ring 124. The staple pusher ring 124 defines a plurality of pusher elements 136 arranged in a circular or annular array. The cylindrical knife 126 is at least partially received within an annular groove or channel 138 within the interior of the staple pusher ring 124, and may be secured within the pusher ring 124 via the use of adhesives or other means (FIG.11). The staple guide 128 includes a plurality of staples 140 also arranged in an annular array. The staples 140 are ejected upon advancement of the staple pusher 60, the staple pusher ring 124 and the pusher elements 136.

[0051] The anvil assembly 18 includes an anvil shaft 142 and an anvil head 144 connected to the anvil shaft 142. (FIGS. 3 and 11) The anvil head 144 includes an annular anvil surface 146 which cooperates with the staples 140 to crimp the staples 140 during firing of the loading unit 10. The anvil shaft 142 is couplable to the anvil retainer 102. In one embodiment, the anvil shaft 142 includes one or more internal locking shelves 148 which cooperate with the outer locking ledge 150 on the anvil retainer 102 to releasably secure the anvil shaft 142 to the anvil retainer 102. The anvil shaft 142 may have sufficient resiliency or incorporate one or more deflectable components whereby the shaft 142 expands in diameter to receive the anvil retainer 102, and then returns towards its original diameter with the internal locking shelves 148 engaging the

outer ledge 150 on the anvil retainer 102. Removal of the anvil assembly 18 relative to the anvil retainer 102 may be effected by pulling on either or both the anvil assembly 18 and the anvil retainer 102 to cause the anvil shaft 142 to expand in diameter such that the locking shelves 148 clear the outer locking ledge 150 of the anvil retainer 102. The anvil head 144 may articulate about pivot pin 152.

[0052] The use and operation of the surgical loading unit 10 and the handle assembly 1000 will now be discussed. As best depicted in FIG.14, prior to mounting of the loading unit 10 to the handle assembly 1000, the lock member 24 is in the lock position in secured engagement with the staple pusher 60 and the anvil approximator 94. (see also FIG. 10) Specifically, the lock tab 52 of the lock member 24 is received within the lock slot 72 of the raised spline 70 of the staple connector 62, and also engages the locking tabs 112 of the anvil bands 100 of the anvil approximator 64. As discussed, the lock member 24 is normally biased to the lock position by the coil spring 50 which is engagement with the guide member 24 and normally biases the guide member 24 to its retracted position.

[0053] With reference now to FIGS.15A-15C, the loading unit 10 is advanced toward the handle frame 1002 of the handle assembly 1000 with the outer tabs 32 and the alignment tab 34 of the loading unit 10 in general alignment with respective grooves 1004, 1006 (shown in phantom) of the handle frame 1002. The handle mount 12 is inserted within the handle frame 1002 of the handle assembly 1000. The loading unit 10 may be secured to the handle frame 1002 through rotation of the loading unit 10 to establish a bayonet coupling with the outer tabs 32 of the loading unit 10 and cooperating grooves 1004, 1006 of the handle assembly 1000. Other mechanisms for securing the loading unit 10 and the handle assembly 1000 are also envisioned including, e.g.,

a snap-lock relationship.

[0054] Upon mounting of the handle mount 12 within the surgical handle assembly 1000, the proximal guide tab 44 of the guide member 22 is engaged by corresponding structure within the handle assembly 1000 and is driven against the bias of the coil spring 50 in the direction of directional arrow “t” (FIGS. 7 and 15C). The corresponding structure may be an internal shelf, detent or similar structure identified schematically (in phantom) as reference numeral 1008, within the interior of the handle frame 1002. Movement of the guide member 22 causes the lock member 24 to rotate through a predetermined arc of rotation from the lock position of FIG. 14 to the released position of FIGS. 16 and 17 such that the lock tab 52 of the lock member 24 releases the lock slot 72 of the staple connector 62 and also releases the locking tabs 112 of the anvil bands 100 of the anvil approximator 94. In this position of the lock member 24, the staple pusher 60 and the anvil approximator 94 are free for longitudinal movement.

[0055] In addition, during mounting of the handle mount 12, at least one, e.g. first and second actuators, within the handle frame 1002 of the handle assembly 1000 couple with the anvil approximator 94 and the staple pusher 60. Any mechanisms for coupling the actuators of the handle assembly 1000 with the anvil approximator 94 and staple pusher 60 are envisioned, including, e.g., a bayonet coupling, interference fit or any other keyed or non-keyed coupling mechanisms. For example, with reference to FIGS. 18 and 19, the first or anvil actuator of the handle assembly 1000, identified schematically (in phantom) as reference numeral 1010, may be coupled to the anvil sleeve 96 through insertion of the distal end of the first actuator 1010 through the longitudinal opening 104 of the anvil sleeve 96. (FIG. 10). The first actuator 1010 may have a spring-biased detent which flexes inwardly to be passed through the longitudinal opening 104, and then returns under the influence of its normal spring bias to

engage the internal shelf 105 of the anvil sleeve 96 to couple the components. The second or staple actuator of the handle assembly 1000, identified schematically (in phantom) as reference numeral 1012 in FIG. 20, may abut or engage the proximal end of the staple connector 62. Other arrangements are also envisioned.

[0056] The procedure may be continued by advancing the anvil actuator 1010 of the handle assembly 1000 via manual member 1014 (FIG. 2) connected to the anvil actuator 1010 (by conventional means) to move the anvil approximator 94 (including the anvil sleeve 96 and the anvil bands 100) in the distal direction from its first position to its second position to cause distal displacement of the anvil assembly 18 to its open condition relative to the staple cartridge assembly 16 (FIGS. 18 and 19). Prior or subsequent to advancement of the anvil approximator 94, the anvil retainer 102 may be mounted to the anvil shaft 142 of the anvil assembly 18 in the manner discussed hereinabove. The anvil assembly 18 may be positioned relative to a tubular organ or tissue and the anvil approximator 94 may be returned to its first position, as depicted in FIG. 20, by movement of the anvil actuator 1010 via manual member 1014 of the handle assembly 1000 in, e.g., a proximal direction, to position the anvil assembly 18 in its closed condition (FIG. 2) relative to the staple cartridge assembly 16. The staple cartridge assembly 16 is positioned relative to the tissue. Thereafter, the staple actuator 1012 of the handle assembly 1000 is actuated via manual member 1016 of the handle assembly 1000 (FIG. 2), which is connected to the staple actuator 1012 by conventional means, to advance the staple actuator 1012 and the staple connector 62 (and the staple pusher 60) as depicted in FIG. 20. Advancement of the staple connector 62 causes corresponding advancement of the staple pusher ring 124 and the cylindrical knife 126 of the staple cartridge assembly 16 to expel the staples 140 which are crimped by the anvil surface 146

of the anvil head 144 thereby joining the tissue or tubular organs and creating an opening therebetween with the cylindrical knife 146.

[0057] Subsequent to use of the loading unit 10, the loading unit 10 may be released from the handle assembly 1000 and disposed, or reloaded and sterilized for subsequent use. Alternatively, a second loading unit 10 can be mounted to the handle assembly 1000 to perform additional stapling or fastening functions and/or other procedures.

[0058] It will be understood that various modifications may be made to the embodiments disclosed herein. For example, the above described lockout mechanism may be incorporated into a variety of surgical instruments which include loading units and is not solely limited to use on staplers systems adapted to perform an end-to-end or circular anastomosis of tissue. For example, the loading unit may be adapted to fire clips or any other fastener dimensioned to attach tissue, including linear attachment of tissue. Therefore, the above description should not be construed as limiting, but merely as exemplifications of various embodiments. Those skilled in the art will envision other modifications within the scope and spirit of the claims appended hereto.

What is claimed is:

1. A surgical loading unit for use with a surgical handle assembly, which comprises:

a handle mount dimensioned for mounting to the handle assembly;

an outer member extending from the handle mount and defining a longitudinal axis and having proximal and distal ends;

a staple cartridge assembly mounted to the distal end of the outer member, the staple cartridge assembly including a plurality staples;

an anvil assembly couplable relative to the staple cartridge assembly;

a staple pusher at least partially disposed within the outer member and operatively coupled to the staple cartridge assembly, the staple pusher adapted for longitudinal movement to eject the staples;

an anvil approximator at least partially disposed within the outer member and operatively coupled to the anvil assembly, the anvil approximator adapted for movement between first and second positions corresponding to closed and open conditions of the anvil assembly relative to the staple cartridge assembly; and

a lock member mounted to the handle mount, the lock member adapted to move from a lock position in secured engagement with the staple pusher and the anvil approximator to a release position releasing the staple pusher and the anvil approximator upon mounting of the handle mount relative to the surgical handle assembly.

2. The surgical loading unit according to claim 1 wherein the lock member is adapted for rotational movement about the longitudinal axis to move from the lock position to the release position.

3. The surgical loading unit according to claim 2 including a guide member having a guide channel arranged at an angle relative to the longitudinal axis, the lock member at least partially received within the guide channel of the guide member and adapted to traverse the channel during movement of the lock member from the lock position to the release position.

4. The surgical loading unit according to claim 3 wherein the lock member includes a lock tab and a channel tab, the lock tab operatively engagable with the staple pusher and the anvil approximator when the lock member is in the lock position, the channel tab received within the guide channel and adapted to traverse the channel.

5. The surgical loading unit according to claim 3 wherein the guide member is adapted to move relative to the handle mount between a retracted position corresponding to the lock position of the lock member and an advanced position corresponding to the release position of the lock member.

6. The surgical loading unit according to claim 5 wherein the guide member is normally biased toward the retracted position.

7. The surgical loading unit according to claim 6 including a spring operatively engagable with the handle mount and the guide member, and dimensioned to normally bias the guide member to the retracted position.

8. The surgical loading unit according to claim 5 wherein the guide member is dimensioned to engage the handle assembly during mounting of the

handle mount relative to the handle assembly causing movement of the guide member to the advanced position thereof.

9. The surgical loading unit according to claim 2 wherein the staple pusher includes a staple connector at least partially disposed within the handle mount, the staple connector having a staple lock surface, the staple lock surface engaged by the lock member when in the lock position thereof and released from the lock member when in the release position thereof.

10. The surgical loading unit according to claim 9 wherein the staple pusher is normally biased toward a proximal position thereof.

11. The surgical loading unit according to claim 9 wherein the anvil approximator includes an anvil band at least partially disposed within the handle mount, the anvil band having an anvil lock surface, the anvil lock surface engaged by the lock member when in the lock position thereof and released from the lock member when in the release position thereof.

12. The surgical loading unit according to claim 1 wherein
the staple cartridge includes an annular array of staples and the anvil assembly includes an annular anvil head cooperable with the annular array of staples to perform a circular or an end-to-end anastomosis.

13. A surgical system for performing an anastomosis, which comprises:
a handle assembly including:
a frame;
a staple actuator and an anvil actuator at least partially disposed within the

frame; and

at least one manual member for actuating at least one of the staple actuator drive and the anvil actuator;

a loading unit including:

a handle mount dimensioned for mounting to the frame of the handle assembly;

an outer member extending from the handle mount and defining a longitudinal axis and having proximal and distal ends;

a staple cartridge assembly mounted to the distal end of the outer member, the staple cartridge assembly including a plurality of staples arranged in a circular array;

an anvil assembly couplable relative to the staple cartridge assembly, the anvil assembly including an anvil shaft and an anvil head;

a staple pusher at least partially disposed within the outer member and operatively coupled to the staple cartridge assembly, the staple pusher adapted for longitudinal movement to eject the staples, the staple pusher couplable to the staple actuator of the handle assembly upon mounting of the handle mount to the frame whereby movement of the at least one manual member causes corresponding movement of the staple pusher; and

an anvil approximator at least partially disposed within the outer member and operatively coupled to the anvil assembly, the anvil approximator adapted for movement between first and second positions corresponding to closed and open conditions of the anvil assembly relative to the staple cartridge, the anvil approximator couplable to the anvil actuator of the handle assembly upon mounting of the handle mount to the frame whereby movement of the at least one manual member causes corresponding movement of the anvil approximator between the first and second positions; and

a lockout mechanism mounted to the handle mount, the lockout mechanism including a lock member and a guide member, the guide member engageable with the frame of the handle assembly upon mounting of the handle mount to the frame of the handle assembly to cause the lock member to rotate about the longitudinal axis from a lock position where the lock member is in secured engagement with the staple pusher and the anvil approximator, to a release position where the lock member releases the staple pusher and the anvil approximator.

14. The surgical system according to claim 13 wherein the guide member is adapted to move relative to the handle mount between a retracted position corresponding to the lock position of the lock member and an advanced position corresponding to the release position of the lock member.

15. The surgical system according to claim 14 wherein the lock member includes a channel tab and a locking tab, the locking tab engageable with the staple pusher and the anvil approximator when in the lock position of the lock member, the channel tab received within a guide channel defined within the guide member, the channel tab traversing the guide channel upon movement of the guide member between the retracted position and the advanced position.

16. The surgical system according to claim 15 wherein the guide member is normally biased toward the retracted position thereof.

17. The surgical system according to claim 14 wherein the staple pusher is normally biased toward a proximal position thereof.

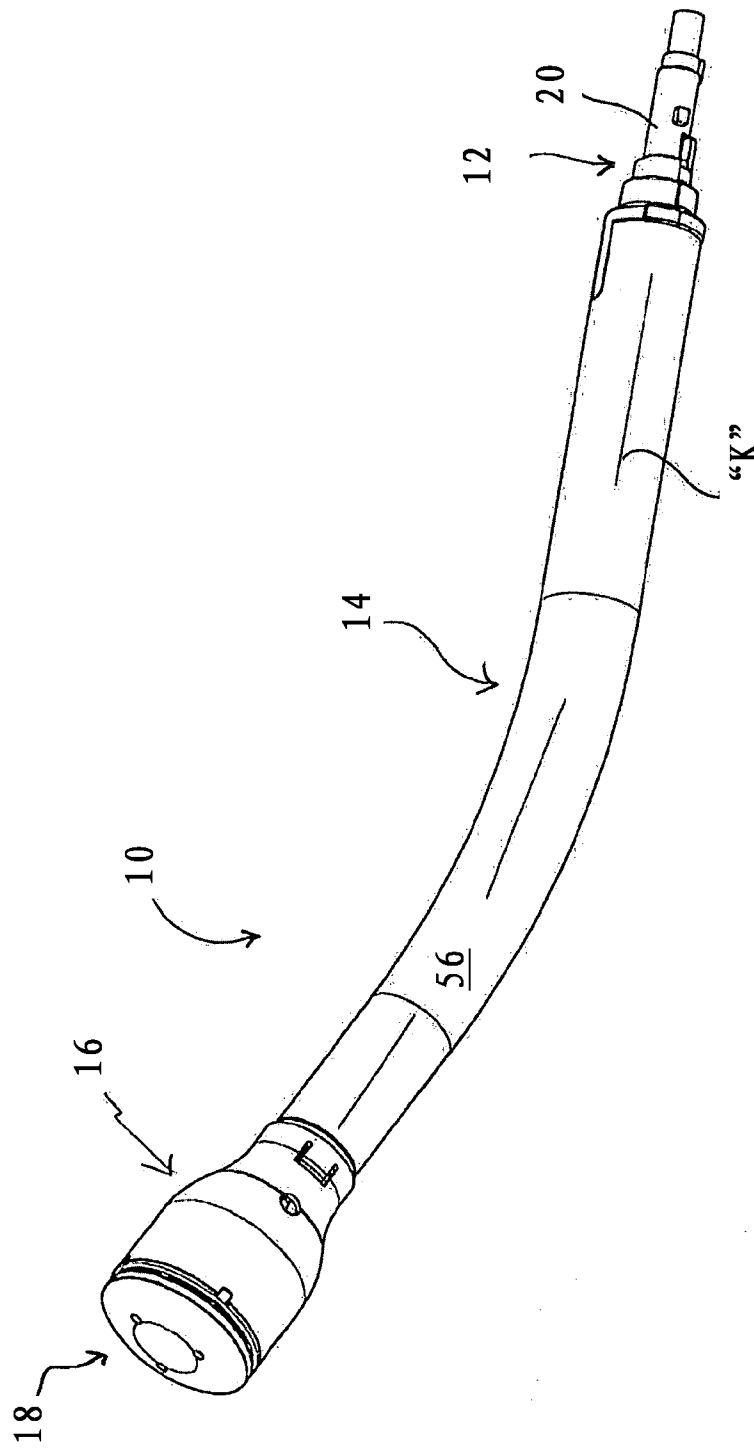


Fig. 1

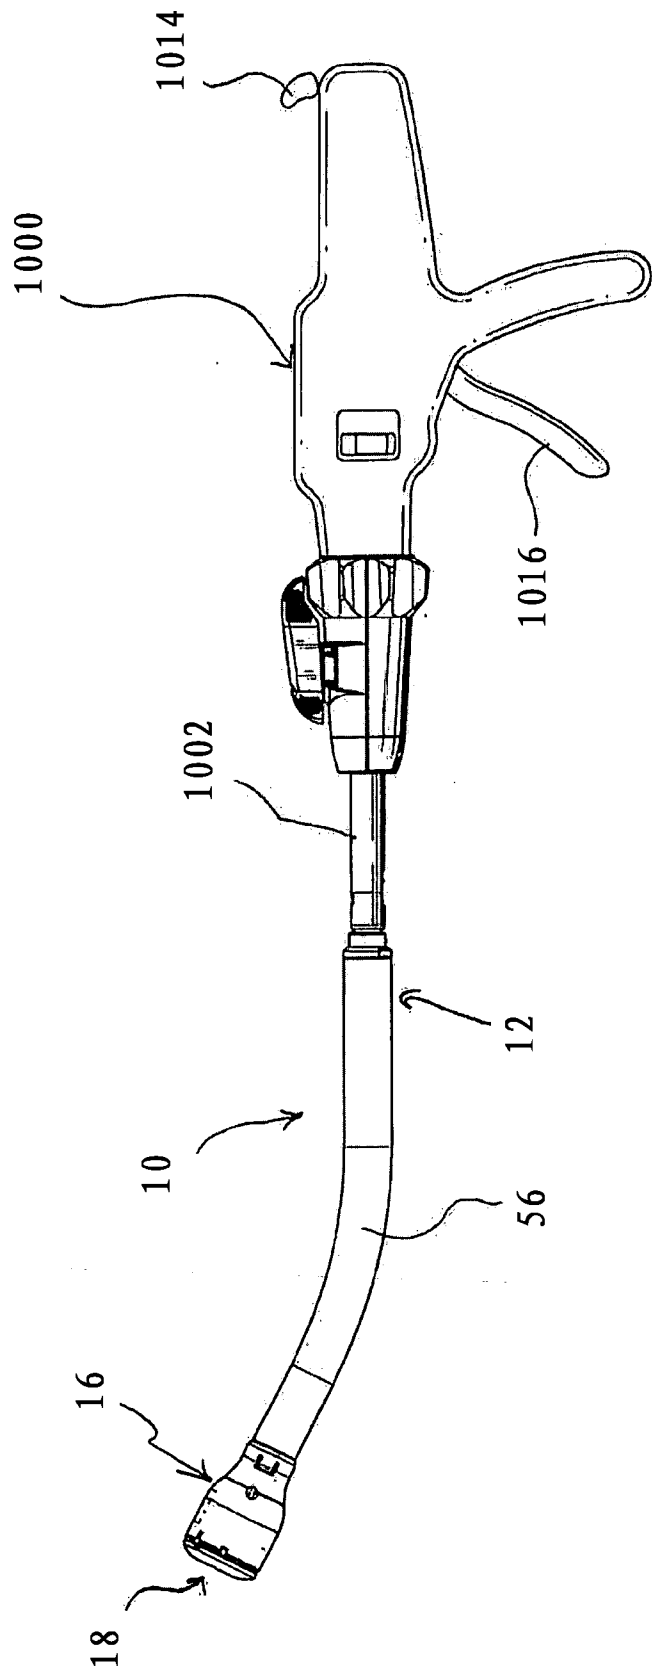


Fig. 2

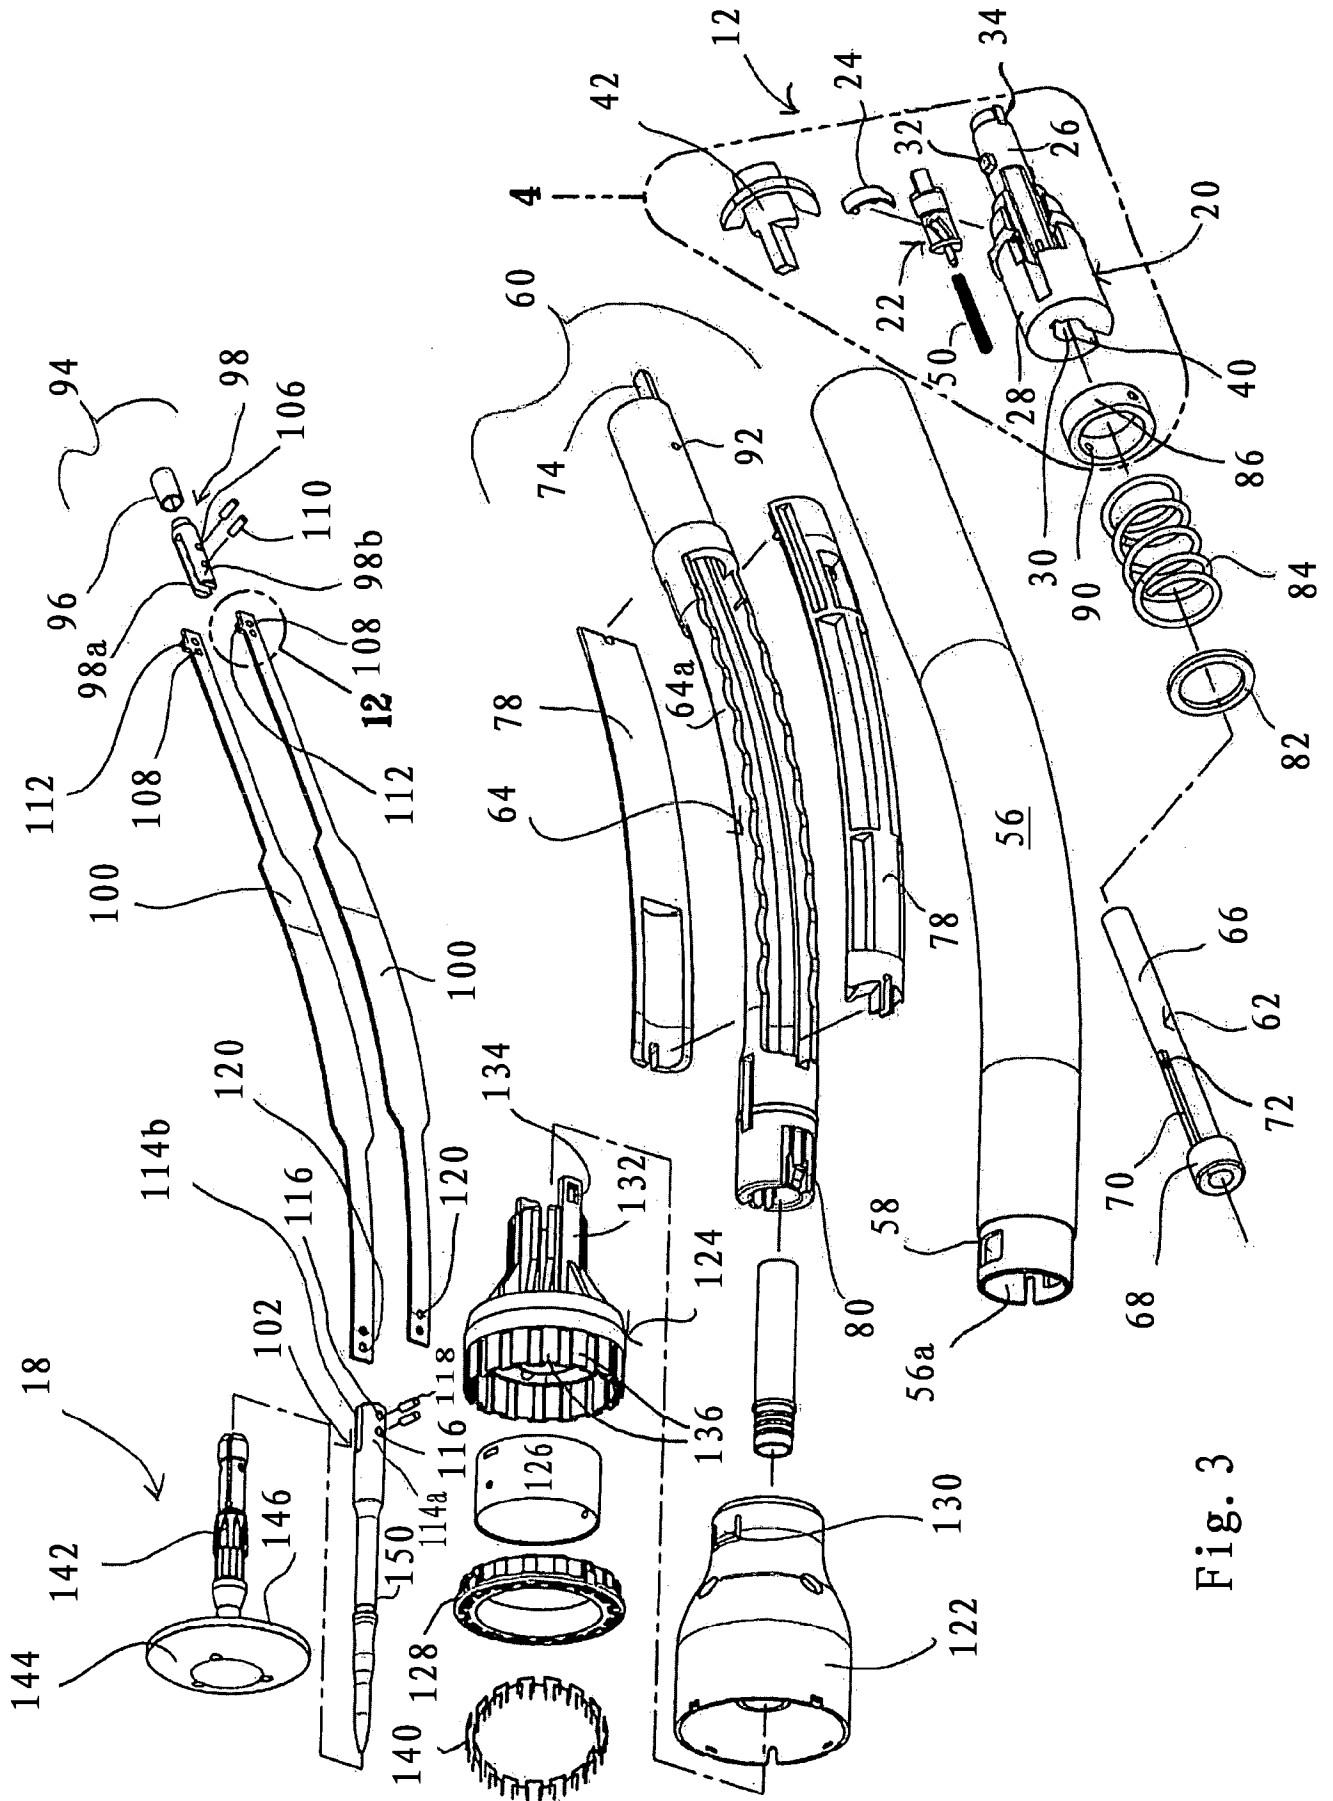
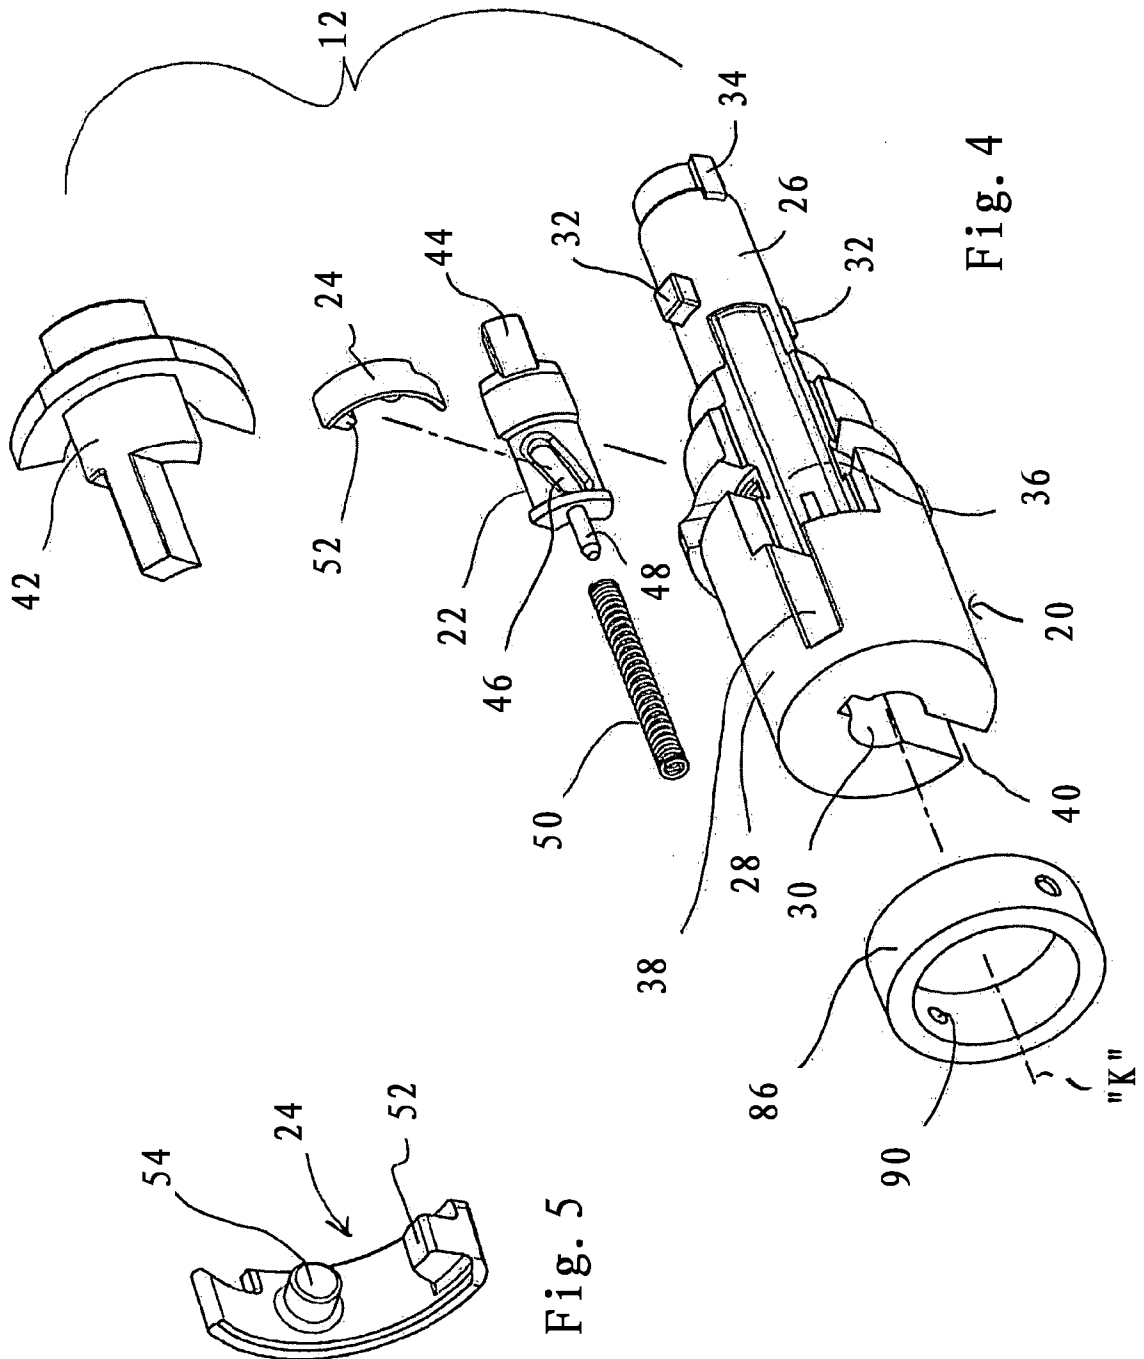
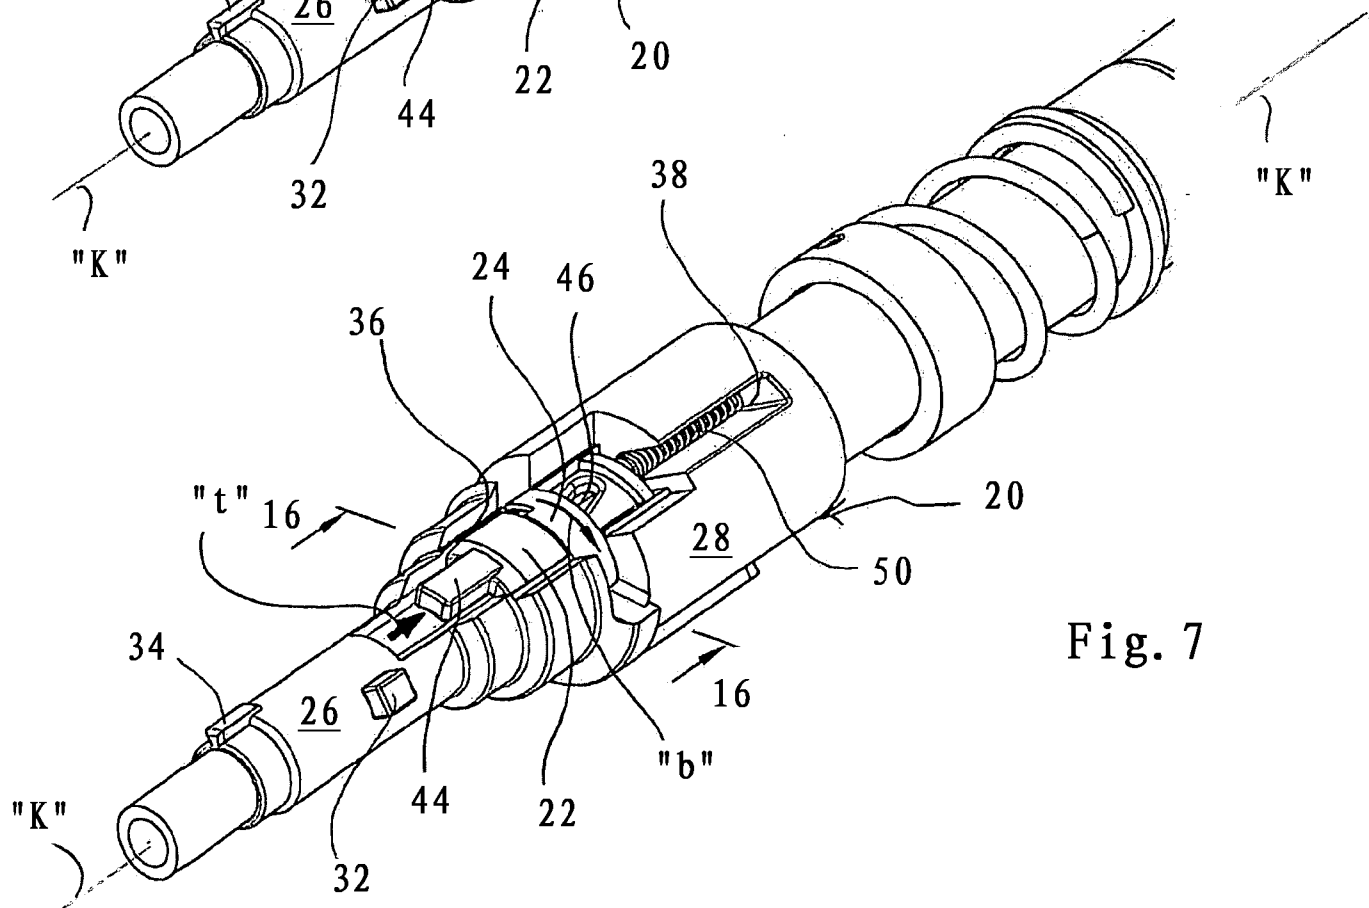
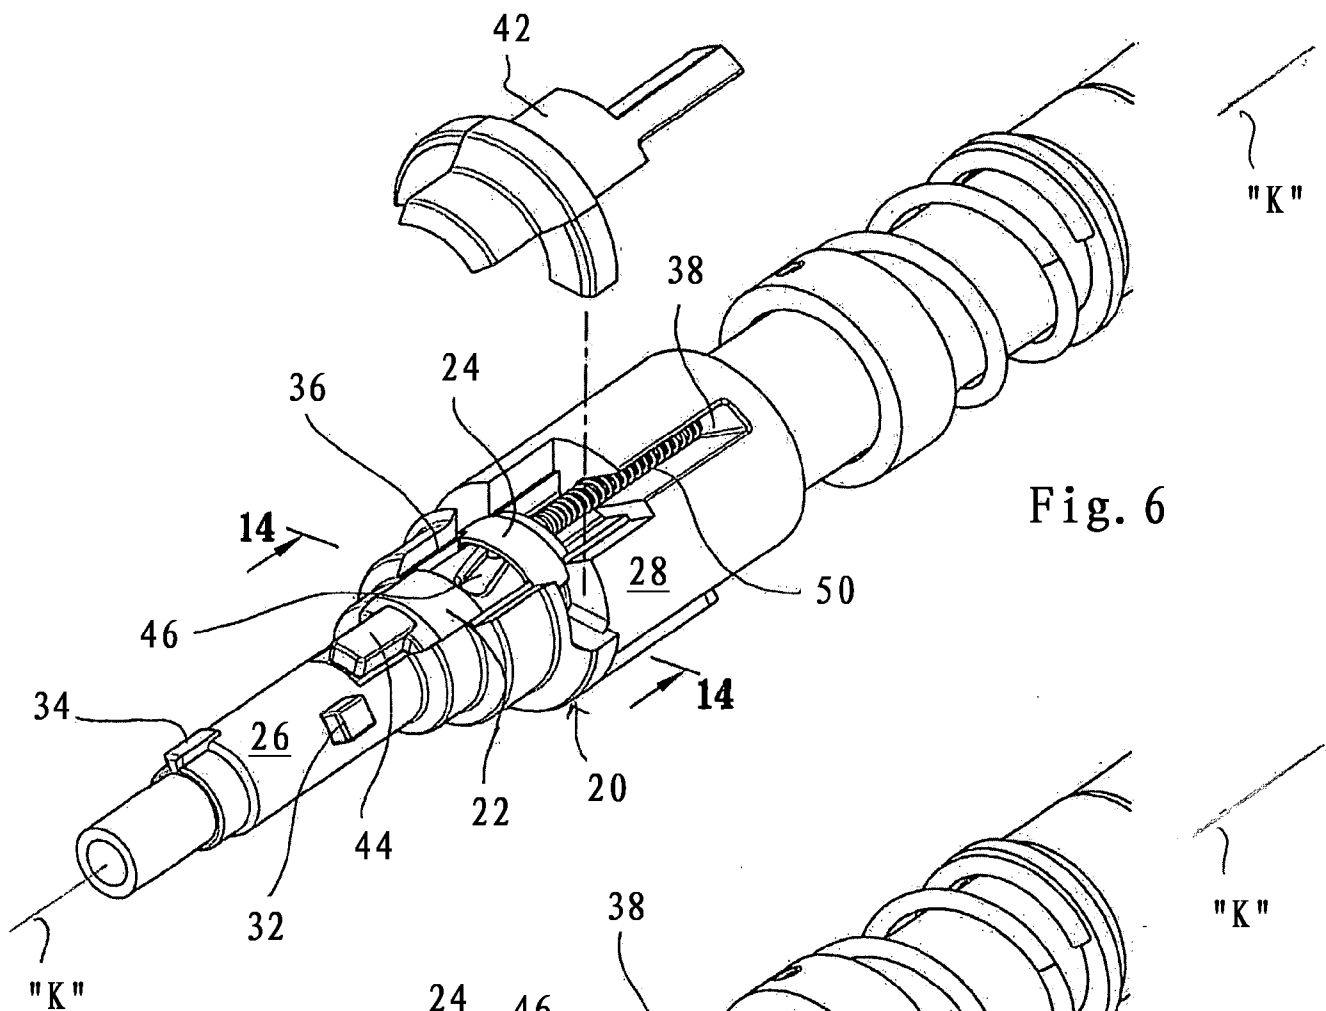


Fig. 3





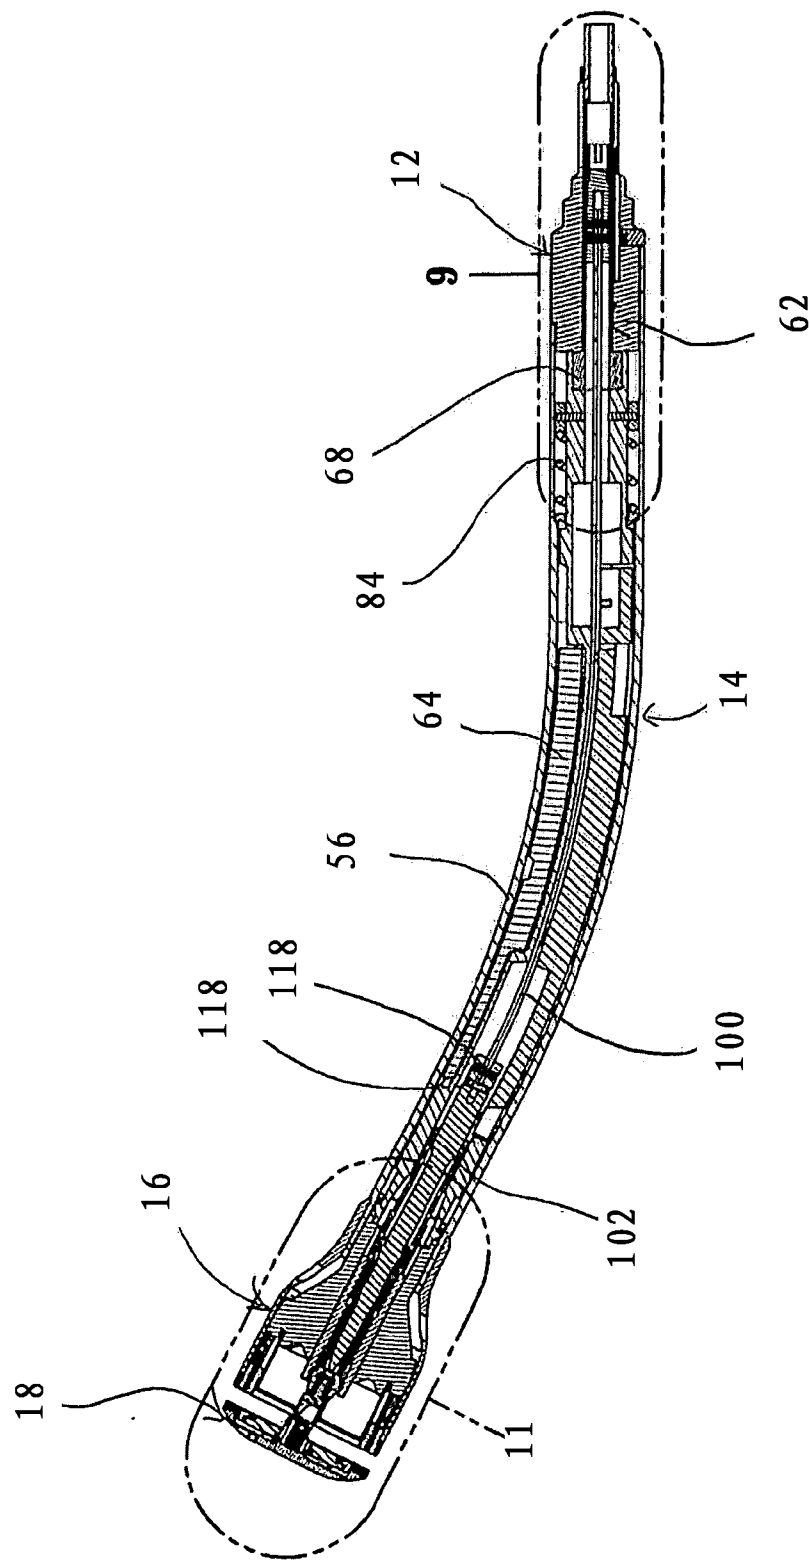
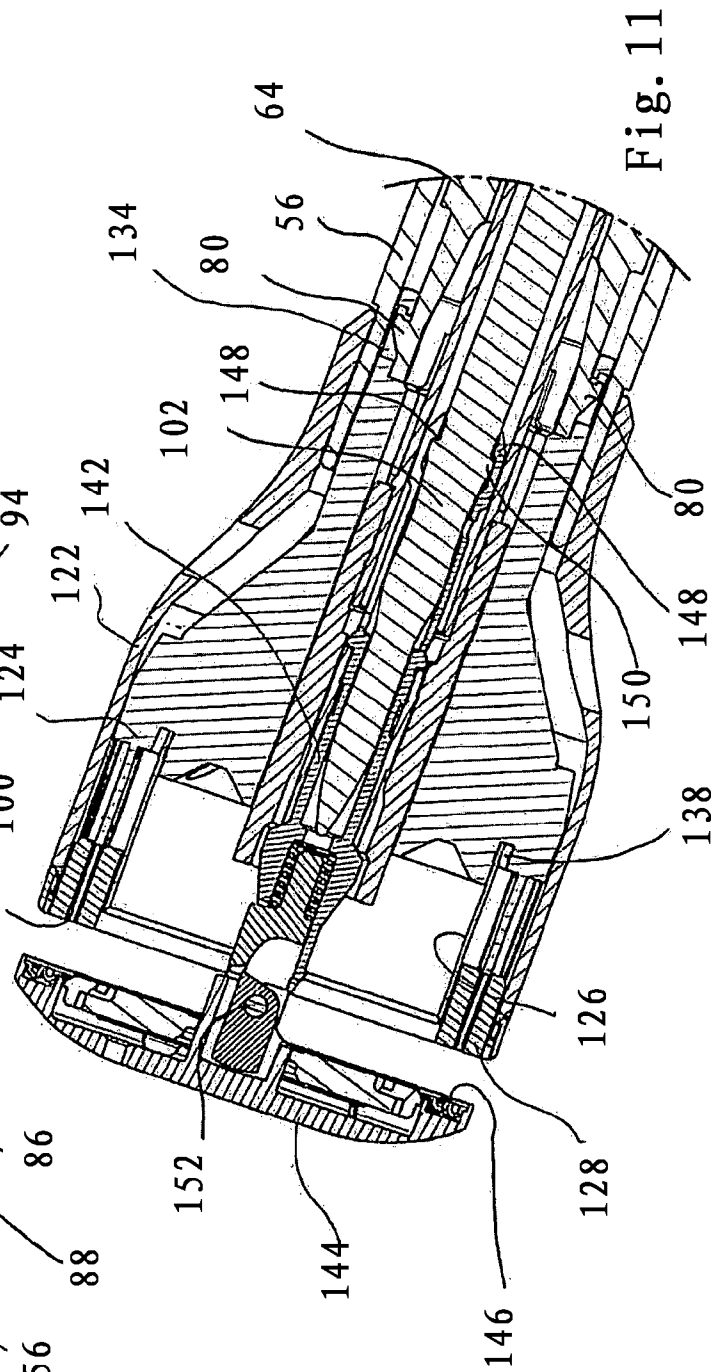
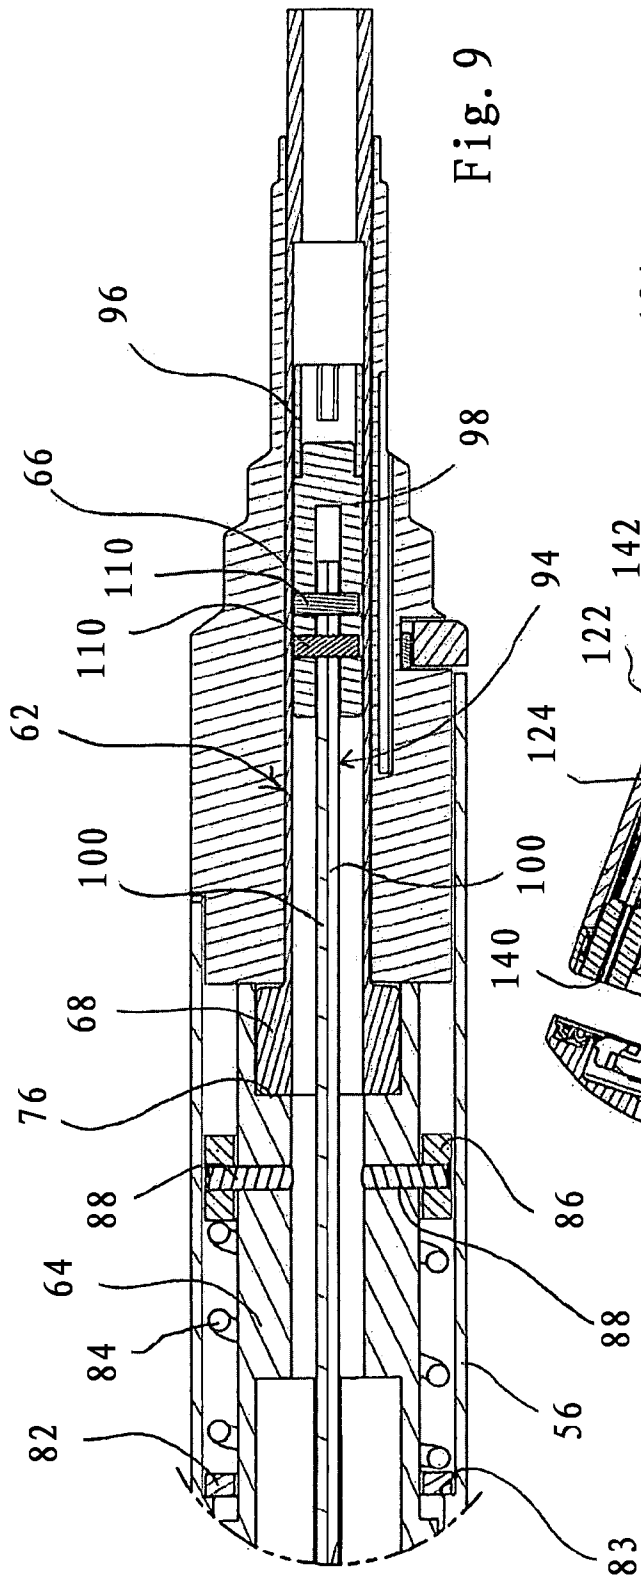


Fig. 8



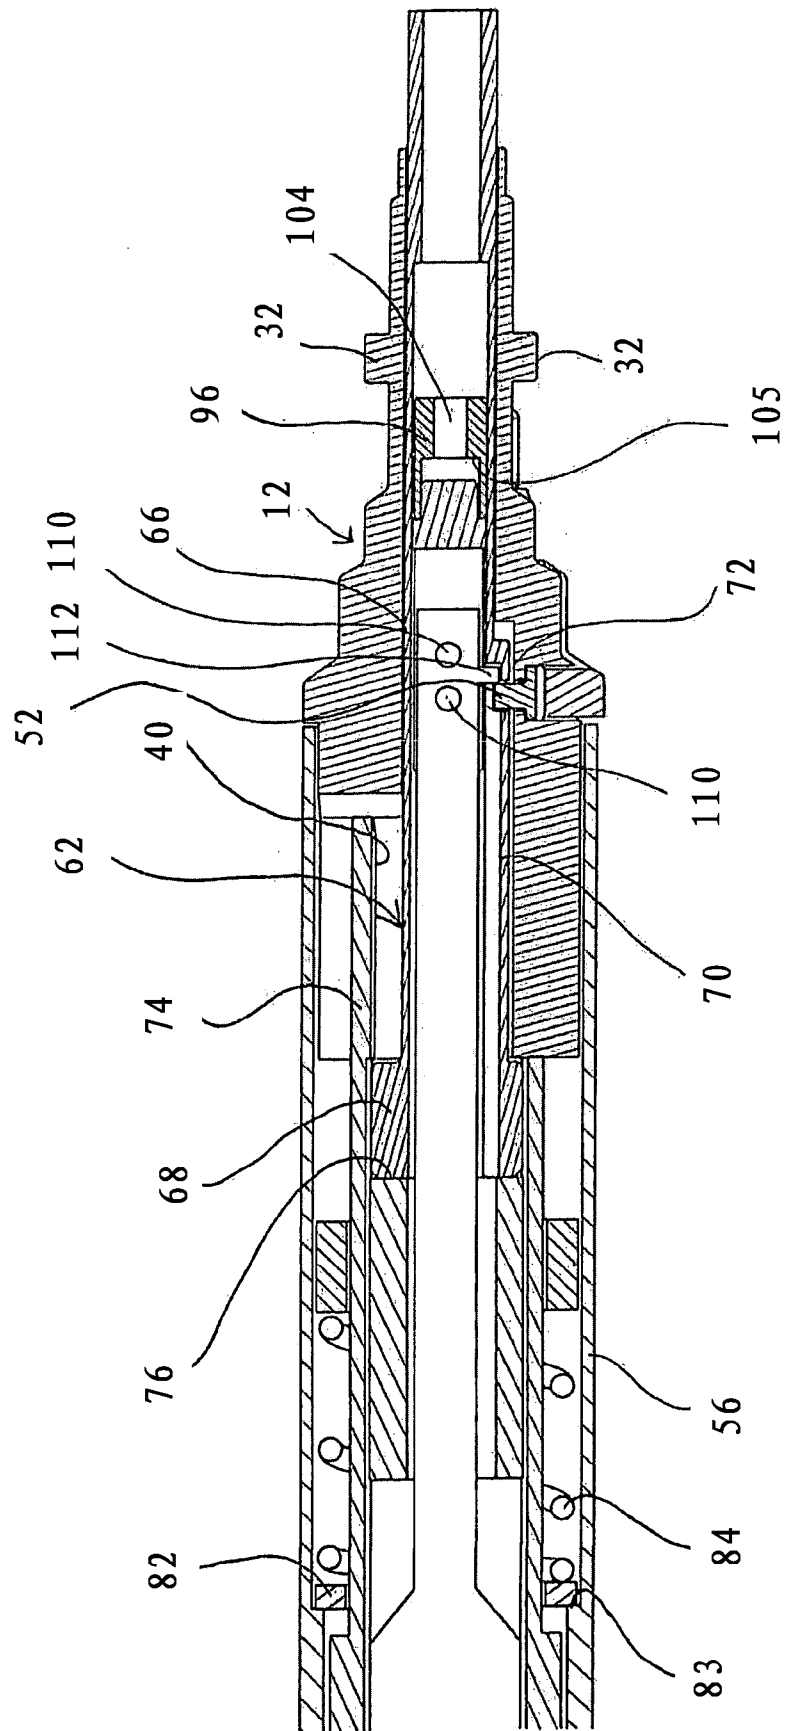


Fig. 10

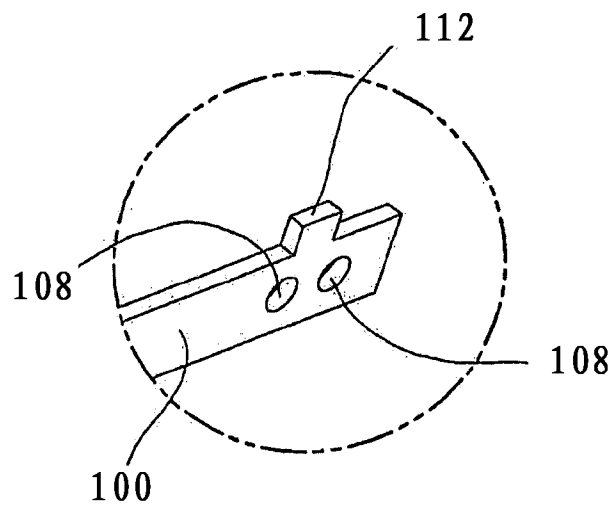


Fig. 12

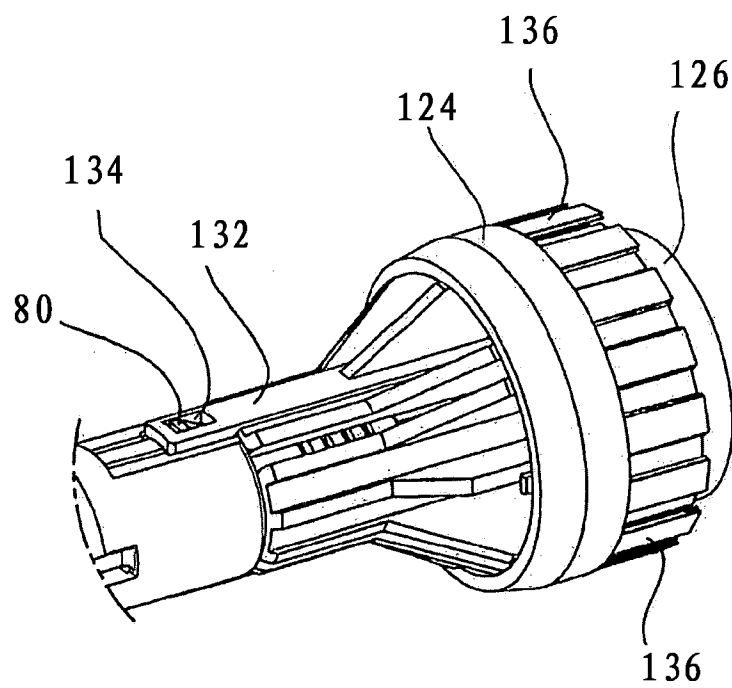
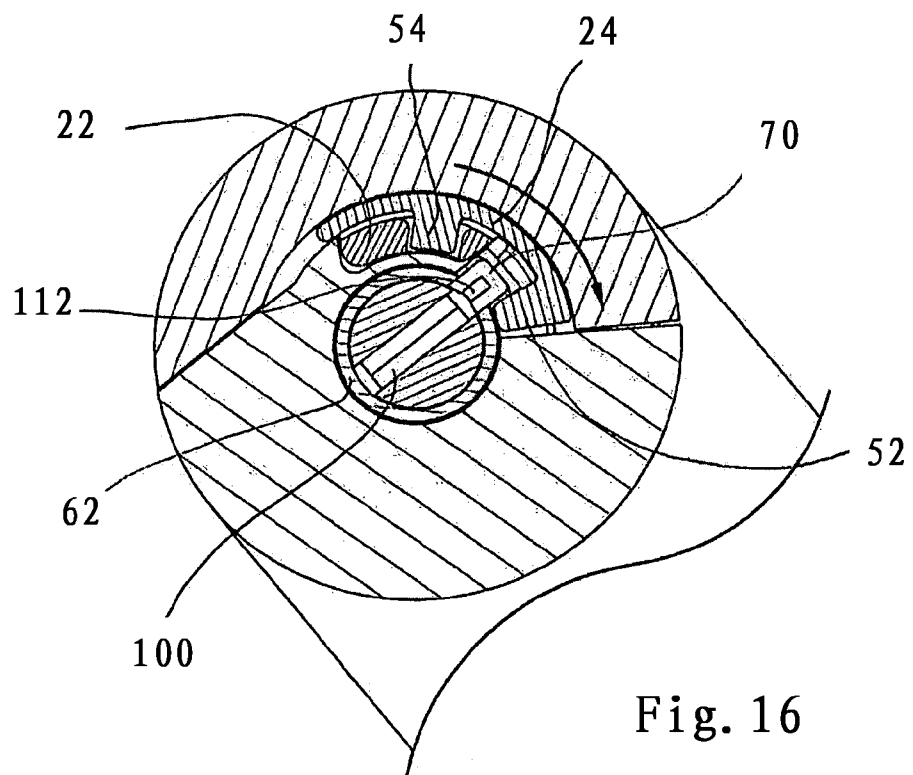
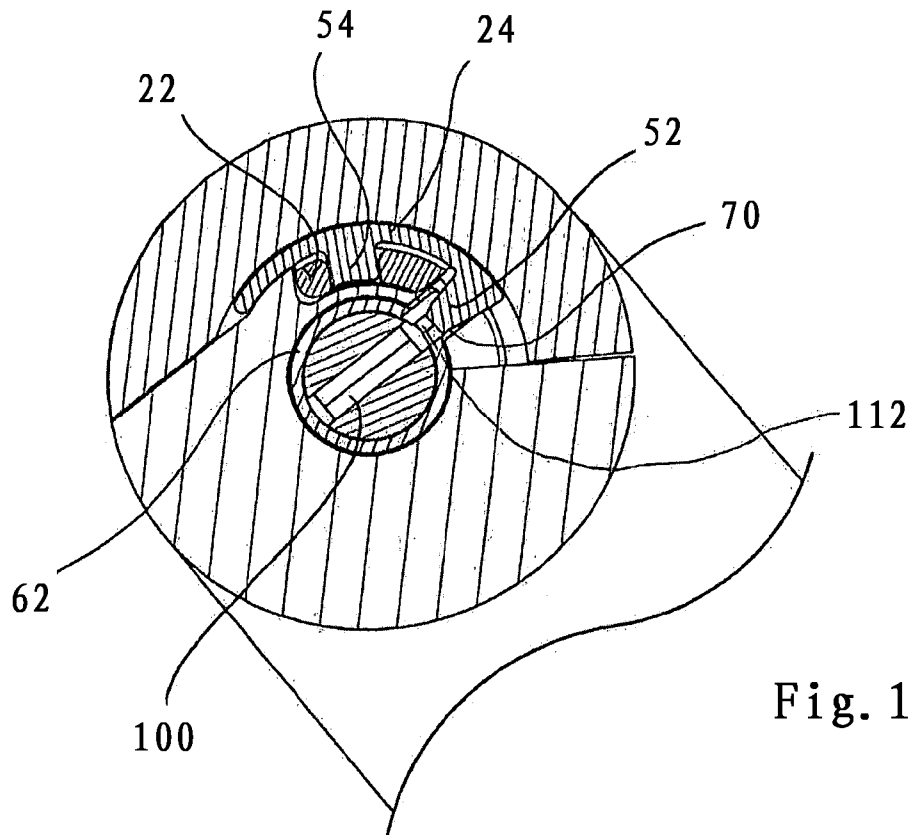
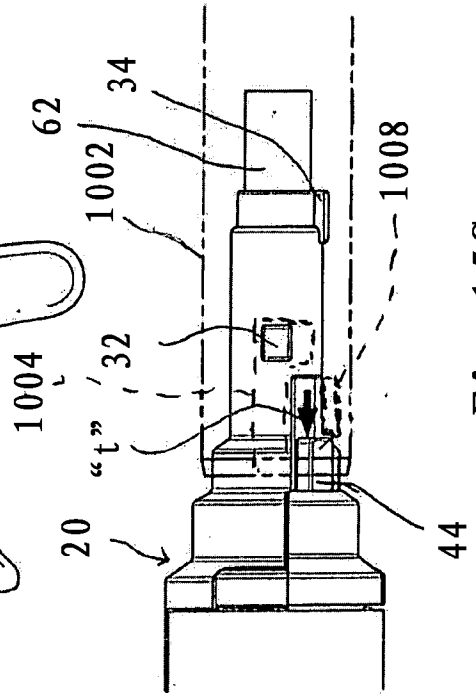
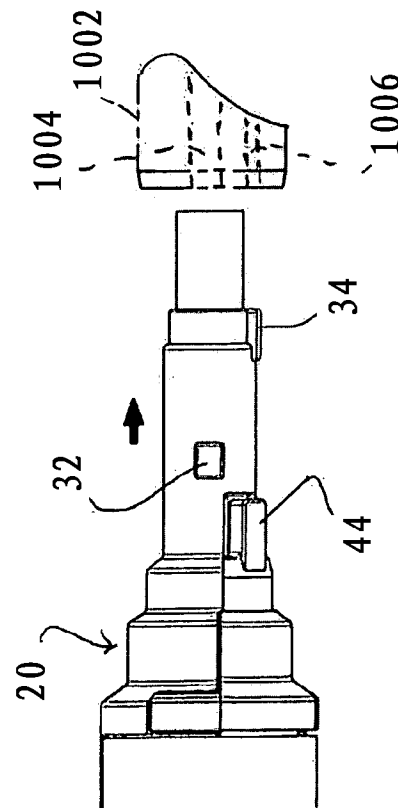
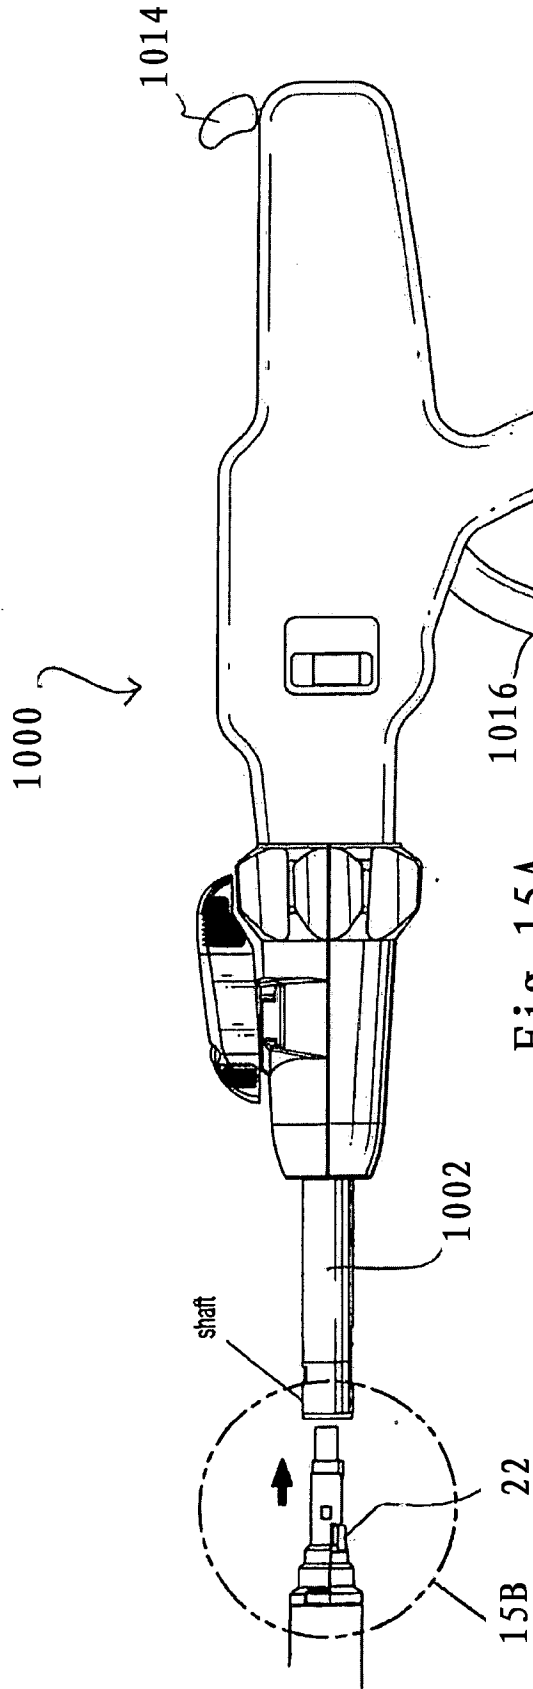


Fig. 13





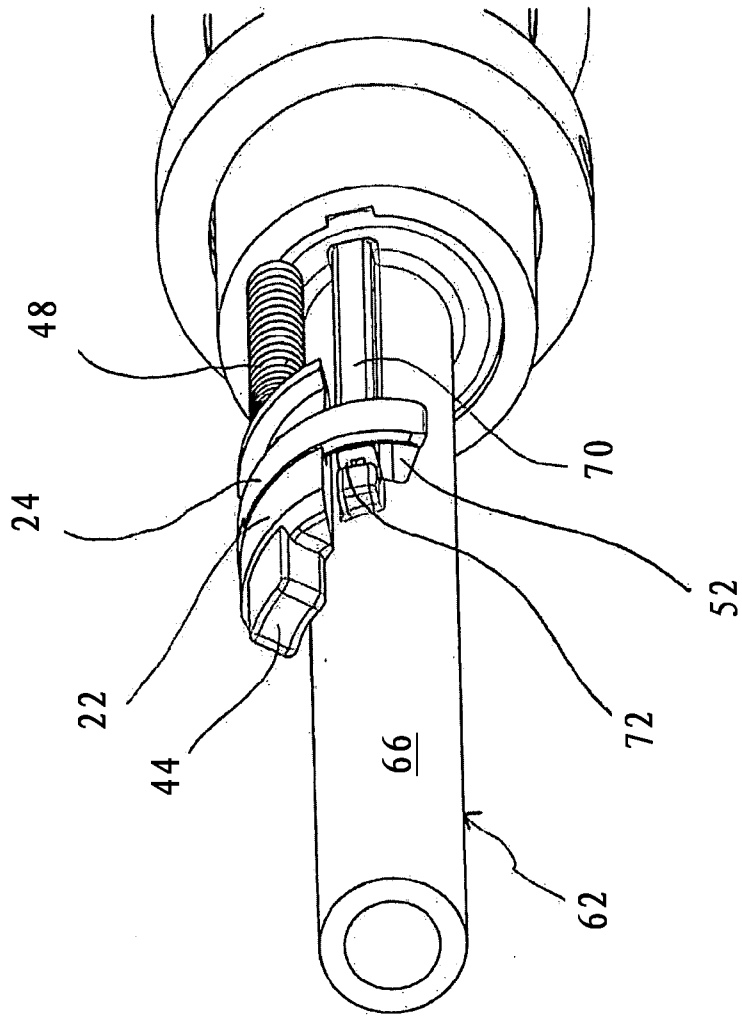


Fig. 17

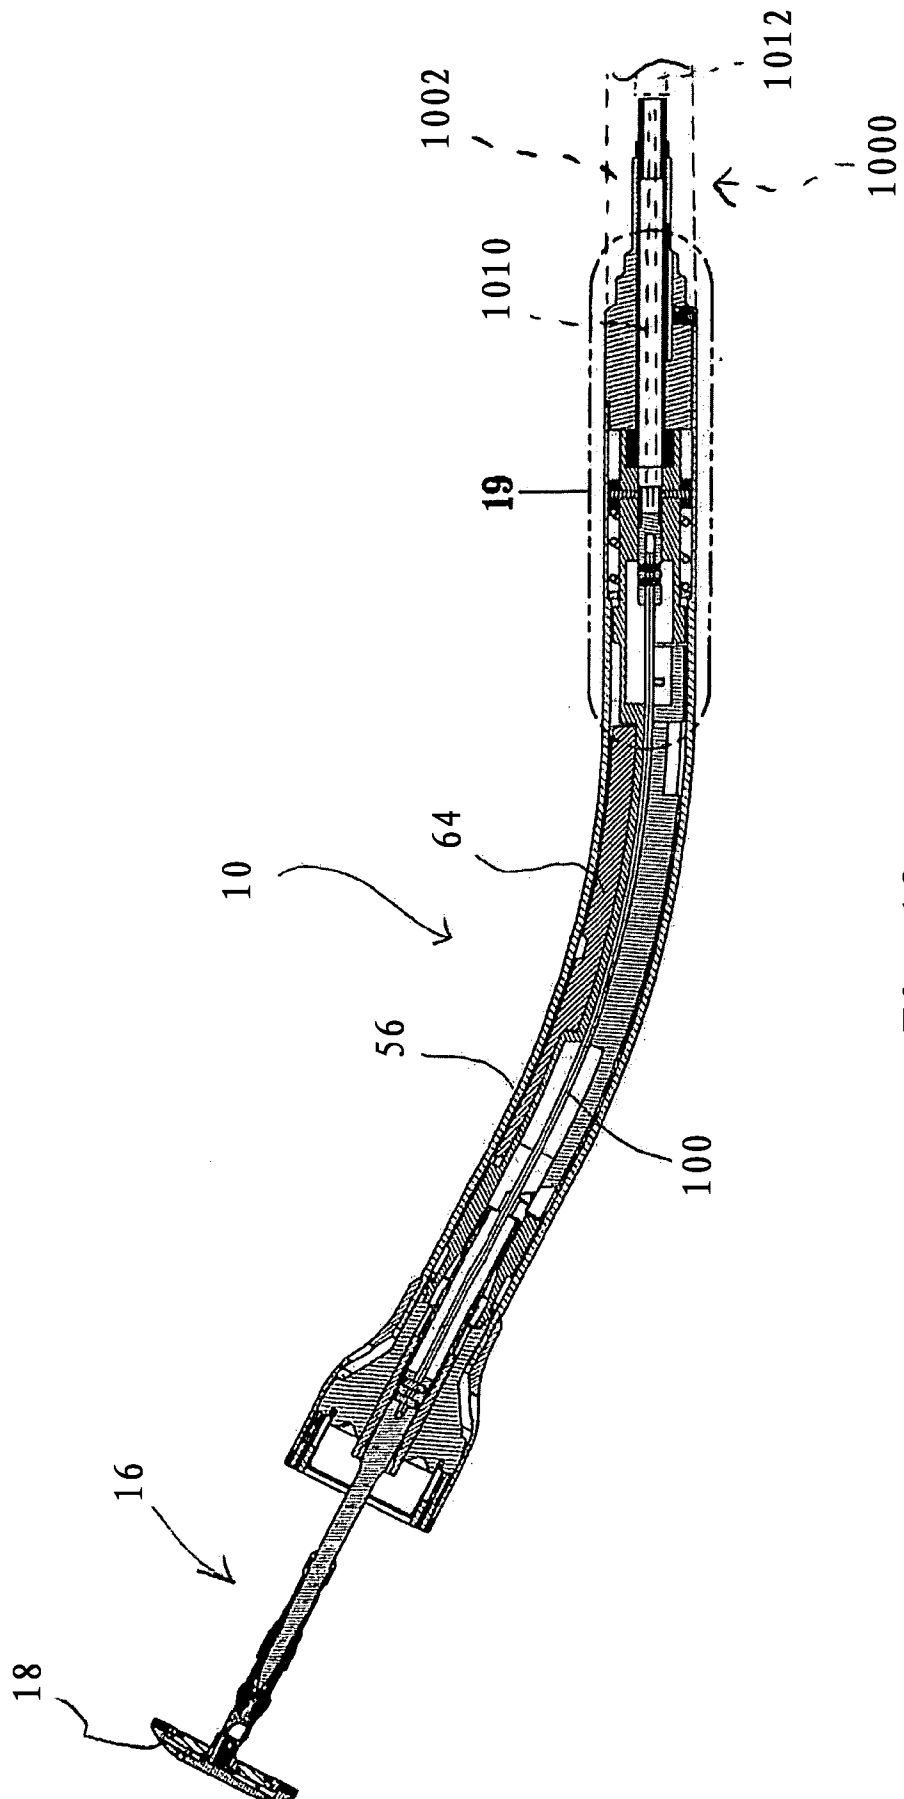


Fig. 18

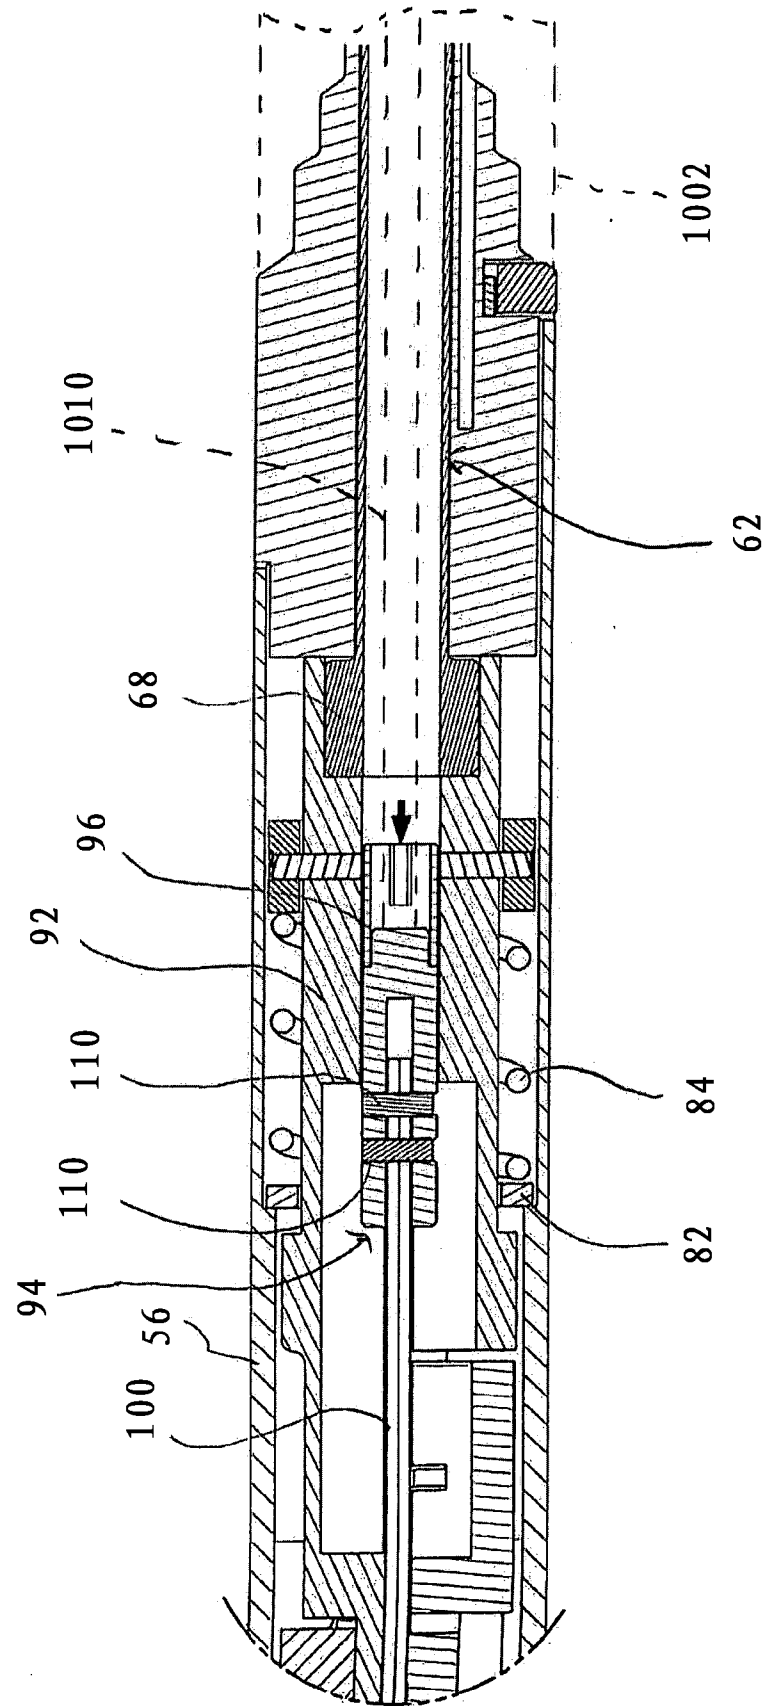


Fig. 19

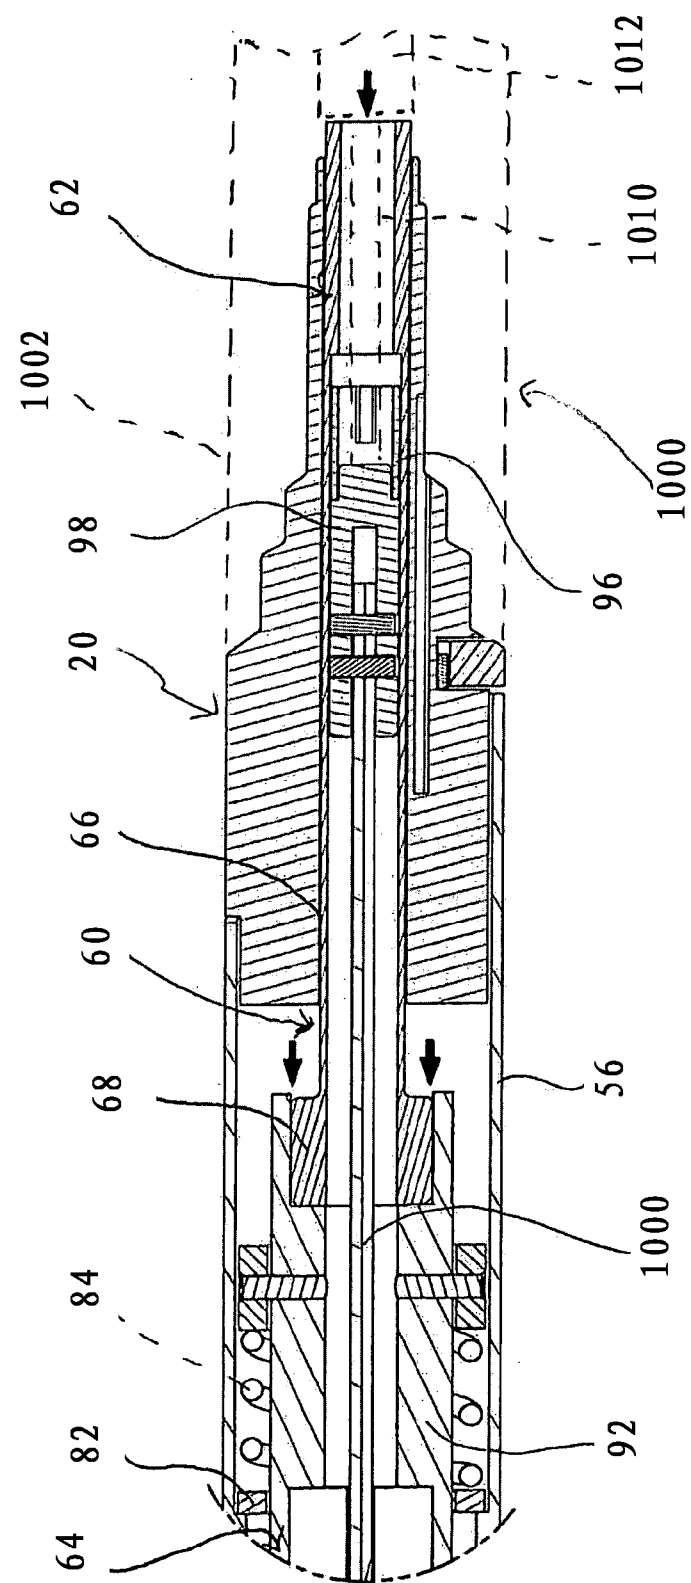


Fig. 20

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CN2014/093563

A. CLASSIFICATION OF SUBJECT MATTER

A61B 17/072(2006.01)i; A61B 17/068(2006.01)i

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 17

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

CNABS;VEN;CNKI: staple?, anastom+, lock+, stop+, prevent+, hanle?, shank?, rod?, pole?, load+, mount+

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 1709911 A1 (TYCO HEALTHCARE GROUP LP) 11 October 2006 (2006-10-11) the description, paragraphs 13-27, and figures 1-16	1-17
X	WO 03030743 A2 (TYCO HEALTHCARE GROUP LP) 17 April 2003 (2003-04-17) the description, page 18, line 4 to page 28, line 3, page 33, line 28 to page 34, line 20, and figures 5-12, 36-38, 72-80, 93-96	1-17
X	US 2012305627 A1 (TYCO HEALTHCARE GROUP LP) 06 December 2012 (2012-12-06) the description, paragraphs 89-113, and figures 1-39	1-17
A	CN 101843509 A (ETHICON ENDO SURGERY INC) 29 September 2010 (2010-09-29) the whole document	1-17
A	US 2009099566 A1 (MANESS MEGAN A ET AL.) 16 April 2009 (2009-04-16) the whole document	1-17



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

“A” document defining the general state of the art which is not considered to be of particular relevance

“E” earlier application or patent but published on or after the international filing date

“L” document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

“O” document referring to an oral disclosure, use, exhibition or other means

“P” document published prior to the international filing date but later than the priority date claimed

“T” later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

“X” document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

“Y” document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

“&” document member of the same patent family

Date of the actual completion of the international search

31 August 2015

Date of mailing of the international search report

14 September 2015

Name and mailing address of the ISA/CN

STATE INTELLECTUAL PROPERTY OFFICE OF THE
P.R.CHINA
6, Xitucheng Rd., Jimen Bridge, Haidian District, Beijing
100088, China

Authorized officer

GUI, Lin

Facsimile No. (86-10)62019451

Telephone No. (86-10)62085615

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.

PCT/CN2014/093563

Patent document cited in search report			Publication date (day/month/year)	Patent family member(s)			Publication date (day/month/year)
EP	1709911	A1	11 October 2006	US	2010301097	A1	02 December 2010
				ES	2329926	T3	02 December 2009
				CA	2541715	C	16 December 2014
				AU	2006201047	A1	26 October 2006
				EP	1709911	B1	29 July 2009
				AU	2006201047	B2	18 August 2011
				JP	4959209	B2	20 June 2012
				JP	2006289064	A	26 October 2006
				JP	2012130729	A	12 July 2012
				US	7780055	B2	24 August 2010
				US	2006226195	A1	12 October 2006
				CA	2541715	A1	06 October 2006
				DE	602006008056	E	10 September 2009
WO	03030743	A2	17 April 2003	AU	2008229931	A1	20 November 2008
				US	2012111921	A1	10 May 2012
				US	8418904	B2	16 April 2013
				US	2009266868	A1	29 October 2009
				ES	2514666	T3	28 October 2014
				CA	2695579	C	25 September 2012
				US	8033440	B2	11 October 2011
				JP	2009078168	A	16 April 2009
				EP	1432358	A2	30 June 2004
				US	8281973	B2	09 October 2012
				US	2012012639	A1	19 January 2012
				EP	2347722	A1	27 July 2011
				AU	2002362750	B2	10 July 2008
				US	2008283575	A1	20 November 2008
				US	2013200130	A1	08 August 2013
				US	2004232201	A1	25 November 2004
				US	7891534	B2	22 February 2011
				US	2011163148	A1	07 July 2011
				CA	2461956	C	04 January 2011
				AU	2008229931	B2	06 October 2011
				CA	2695579	A1	17 April 2003
				US	7934628	B2	03 May 2011
				CA	2461956	A1	17 April 2003
				JP	5068247	B2	07 November 2012
				JP	4252454	B2	08 April 2009
				JP	2011240148	A	01 December 2011
				US	8286848	B2	16 October 2012
				US	2010200639	A1	12 August 2010
				JP	2005505335	A	24 February 2005
				US	8113408	B2	14 February 2012
				EP	2623043	A1	07 August 2013
				EP	2347722	B1	17 September 2014
				DE	602006008056	E	10 September 2009
				EP	1432358	B1	12 August 2015
US	2012305627	A1	06 December 2012	US	2010237131	A1	23 September 2010
				EP	1021130	B1	15 November 2006
				US	8342377	B2	01 January 2013

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.

PCT/CN2014/093563

Patent document cited in search report				Publication date (day/month/year)		Patent family member(s)		Publication date (day/month/year)	
				US	2004108357	A1	10 June 2004		
				ES	2335523	T3	29 March 2010		
				CA	2666604	A1	01 April 1999		
				CA	2571579	A1	01 April 1999		
				ES	2399811	T3	03 April 2013		
				US	7565993	B2	28 July 2009		
				JP	2008086787	A	17 April 2008		
				CA	2304750	A1	01 April 1999		
				JP	4257029	B2	22 April 2009		
				US	8292152	B2	23 October 2012		
				US	2014110454	A1	24 April 2014		
				US	2013140342	A1	06 June 2013		
				JP	5084061	B2	28 November 2012		
				AU	750646	B2	25 July 2002		
				US	2005067460	A1	31 March 2005		
				US	8210416	B2	03 July 2012		
				EP	2316348	A1	04 May 2011		
				EP	2113207	A2	04 November 2009		
				JP	4500342	B2	14 July 2010		
				EP	2298186	A2	23 March 2011		
				US	8256656	B2	04 September 2012		
				EP	2298185	A2	23 March 2011		
				JP	4500343	B2	14 July 2010		
				US	8087563	B2	03 January 2012		
				EP	1762190	B8	23 December 2009		
				US	6669073	B2	30 December 2003		
				US	2012043368	A1	23 February 2012		
				US	2012055974	A1	08 March 2012		
				CA	2571468	A1	01 April 1999		
				US	2006255090	A1	16 November 2006		
				EP	1762190	A2	14 March 2007		
				CA	2552427	C	25 November 2008		
				CA	2571468	C	30 March 2010		
				JP	2010148890	A	08 July 2010		
EP	2286736	B1	07 November 2012						
JP	4500344	B2	14 July 2010						
ES	2275317	T3	01 June 2007						
US	6953139	B2	11 October 2005						
EP	2156796	B1	07 September 2011						
DE	69836436	D1	28 December 2006						
ES	2372662	T3	25 January 2012						
EP	2818124	A1	31 December 2014						
CN	101843509	A	29 September 2010	JP	2010221027	A	07 October 2010		
				US	8066167	B2	29 November 2011		
				JP	5528864	B2	25 June 2014		
				EP	2233084	A1	29 September 2010		
				CN	101843509	B	22 October 2014		
				US	2010237132	A1	23 September 2010		
US	2009099566	A1	16 April 2009	AU	2008229820	A1	30 April 2009		
				EP	2047826	A1	15 April 2009		

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.

PCT/CN2014/093563

Patent document cited in search report	Publication date (day/month/year)	Patent family member(s)	Publication date (day/month/year)
		JP 2009101152 A	14 May 2009
		CN 101507664 A	19 August 2009
<hr/>			