



(11) **EP 2 014 365 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
17.04.2013 Bulletin 2013/16

(51) Int Cl.:
B01L 1/00 ^(2006.01) **B08B 15/02** ^(2006.01)
F24F 3/16 ^(2006.01)

(21) Application number: **07123726.7**

(22) Date of filing: **19.12.2007**

(54) **Air curtain-isolated biosafety cabinet**

Luftvorhangisolierter Biosicherheitsschrank

Armoire de biosécurité isolée par rideau d'air

(84) Designated Contracting States:
DE FR GB IT NL

(30) Priority: **01.06.2007 TW 96209015 U**

(43) Date of publication of application:
14.01.2009 Bulletin 2009/03

(73) Proprietor: **Institute of Occupational Safety
and Health, Council of Labor Affairs
221 Shijr City, Taipei (TW)**

(72) Inventors:
• **Hung, Rong-Fung**
Taipei (TW)
• **Shih, Tung-Sheng,**
c/o Institute of Occupational Safety and Health
Shijr City 221 (TW)

- **Chang, Cheng-Ping,**
c/o Institute of Occupational Safety and Health
Shijr City 221 (TW)
- **Chen, Chun-Wan,**
c/o Institute of Occupational Safety and Health
Shijr City 221 (TW)
- **Hung, Chen-Hsiung**
Taipei 106 (TW)

(74) Representative: **Beck & Rössig**
European Patent Attorneys
Cuvilliesstrasse 14
81679 München (DE)

(56) References cited:
EP-A- 0 139 128 EP-A- 1 745 866
DE-A1- 3 811 780 US-A- 3 886 851
US-A- 4 098 174 US-A- 4 637 301
US-A1- 2006 079 164

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 014 365 B1

Description

Field of the invention

[0001] The present invention relates to a biosafety cabinet (BSC) comprising the features of the preamble portion of claim 1; more particularly, relates to forming an air-isolator at an opening of a door to isolate air flows inside and outside the BSC, to prevent circulations in the BSC, and to prevent contamination leakage from the BSC.

Description of the Related Art

[0002] In many microbiological experiments or procedures, biological dangers may do harm to operators. BSC is used to protect germs in the cabinet and to prevent contamination inside from leaking out.

[0003] Although BSC is used to protect germs in the cabinet and to protect the operator, events keep on happening that operators died because of contamination. It shows that BSC still has some problem. In an actual operation, there are two types of problems: (1) not obtaining the most proper design: They include insufficient suction amount, improper suction slot position, improper air supplier position, uneven flow rate at front opening, bad opening shape design, etc.; and (2) not operating in a best state: They include that the contamination is too much, the opening is too wide opened, that the suction amount is not well adjusted following an actual situation, etc.

[0004] According to NSF/ANSI 49, 2002, which is a newly revised standard for a level II BSC, the BSCs can be divided into four categories: A1, A2, B1 and B2.

[0005] Clark and Mullan, Rake, Kennedy, Kruse, etc. test BSCs for capabilities in exhausting contamination and found that the level II BSC can not resist a sudden change in indoor air pressure. Hence, the capability in exhausting contamination for a level II BSC has to be improved.

[0006] In the B2 BSC, waste gases are totally exhausted without recycling; all gases are flowed through HEPA filter; and the gases are exhausted to the exhausting system of a building. The BSC has a HEPA filter on top to supply air by an air blower. Thus, outer air is not allowed to enter the cabinet directly; and environments inside and outside the cabinet are separated. Then the air is exhausted by an air-suction device at a rate of 0.57 cubic meters per second for obtaining a negative pressure in the cabinet. And, if air supply is not enough, a sash may be opened to supply air into the BSC from outside. Yet, in such a situation, the contamination in the BSC may leak out at the opening by the interference of the outside flow and/or the action of the BSC door. Therefore, traditional BSC is weak in defending interferences of side flow and door operation.

[0007] EP 0 139 128 D1 discloses a BSC according to the preamble portion of claim 1.

[0008] Further bio safety cabinets are known from DE 38 11 780 A1 and EP 1 745 866 A1, and US 4,637,301 A1.

Summary of the invention

[0009] The object of the present invention is to provide a biosafety cabinet which prevents leakage and circulations in the biosafety cabinet.

[0010] To achieve the above purpose, the present invention provides a cabinet according to claim 1. Advantageous embodiments are laid down in further claims.

[0011] An air curtain-isolated BSC according to an embodiment of the invention comprises a main body, a door, an air blower, a suction box, a gas sucker, a plurality of cross flow fans and a high efficiency particulate air (HEPA) filter, where the main body has a space to contain a harmful gas to be exhausted and has an open space at a side. The door is movably assembled to the main body at the side to control an opening and has an air-pushing veil. The air blower is connected to an air inlet on top of the main body to supply fresh air. The suction box is set beneath the main body and has a suction slot at an edge of the main body corresponding to the air-pushing veil of the door. The gas sucker is set at an exit of the suction box for exhausting the harmful gas. The HEPA filter is set on top of the main body to supply air by the air blower and air flows inside and outside the BSC are isolated to prevent operators from damages owing to leakage of the contamination in the BSC, and to prevent contamination outside of the BSC from entering into the BSC to pollute a product in the BSC. Accordingly, a novel air curtain-isolated BSC is obtained.

Brief description of the drawings

[0012] The present invention will be better understood from the following detailed description of an embodiment according to the present invention, taken in conjunction with the accompanying drawings, in which present invention, taken in conjunction with the accompanying drawings, in which

- FIG.1 is the perspective view showing an embodiment according to the present invention;
- FIG.2 is the side view showing the embodiment;
- FIG.3 is the view showing the embodiment with the coordinated devices;
- FIG.4 is the view showing the straight curtain;
- FIG.5 is the view showing the slightly concave curtain;
- FIG.6 is the view showing the severely concave curtain; and
- FIG.7A to FIG.7C are view showing the changes of the oscillating curtain at different times.

Description of an embodiment

[0013] The following description is provided to under-

stand the features and the structures of the present invention.

[0014] FIG.1 to FIG.3 show a perspective view and a side view of an embodiment according to the present invention; and a view showing the embodiment with coordinated devices. As shown in the figures, the present invention is an air curtain-isolated biosafety cabinet (BSC), comprising a main body 11, a door 12, an air blower 13, a suction box 14, a gas sucker 15, a plurality of cross flow fans 20 and a high efficiency particulate air (HEPA) filter 16, where air flows inside and outside the BSC are isolated with no air circulation and dissipation and thus contamination in the cabinet is well prevented from leakage.

[0015] The main body 11 has a space to contain a harmful gas to be exhausted; and has an open space at a side.

[0016] The door 12 is movably assembled to the main body 11 at a side. The door 12 has a handle 121 to move the door for controlling an opening 125. A plurality of cross flow fans 20 is set on the door 12 and the door 12 is a telescopic sliding door to change opening size of the door 12. The door 12 blows air by setting a plurality of cross flow fans controlled by a cross-flow fan controller 2. Air is blown from upper side of the door 12 to a section of honeycombs 123. And then the air is continuously blown through a stabilizing passage 124 to dissipate turbulence energy to reach an opening 125 of the door 12.

[0017] Concerning supplying a down flow of air, the air blower 13 is controlled by an inverter 17a and is connected with the air inlet 111 on the top of the HEPA filter 16 to supply fresh air.

[0018] The suction box 14 is set beneath the main body 11; and has a suction slot 141 located at an edge of the main body 11 corresponding to the air-pushing veil 122 of the door 12.

[0019] The gas sucker 15 is set at an exit of the suction box 14 to suck the harmful gas. Another inverter 17b is used to change a rotation rate of the gas sucker 15 to control an average blowing rate of the air blower 13 and an average sectional sucking rate of the suction slot 141. A Venturi flow meter 18 is set between an exit of the gas sucker 15 and an exit of the suction box 14 to measure an air-blowing rate; and obtains a pressure difference between them with a coordination of a pressure transducer 19.

[0020] The HEPA filter 16 is deposited on top of the main body 11 to supply air in an average rate through the air blower 13. Thus, with the above structure, a novel air curtain-isolated BSC is obtained.

[0021] The present invention has the following characteristics: The door 12 is movably assembled at a side of the main body 11 and has an air-pushing veil 122. The inverter 17a is used to control the air blower 13 and the air blower 13 is connected to the air inlet 111 on the HEPA filter 16 through a flexible pipe. A plurality of cross flow fans 20 is set on the door 12; and the door is a telescopic sliding door to change a position of mouth for blowing

air. The cross flow fans 20 is controlled by a cross-flow fan controller 2 to provide a steady air flow to flow from the upper side of the door 12 and to flow through a section of honeycombs 123. Then, the air is flowed through a stabilizing passage 124 to dissipate turbulence energy to reach the opening of the door 12. The suction box 14 is set beneath the main body 11 and the suction slot 141 is located at an edge of the main body 11 corresponding to the air-pushing veil 122 of the door 12, where a push-pull air-isolator is thus obtained. The flow fields of the BSC are examined through a flow visualization and are effectively controlled to prevent contamination in the cabinet from leakage; and the position of the suction slot 141 can be changed to suck the contamination more effectively. Through the HEPA filter 16 on the main body 11, fresh air flow is supplied to meet a physical mechanism between air suction and air supply. Accordingly, the air curtain-isolated BSC obtains the physical mechanism between air suction and air supply; the air-isolator formed by the local air suction near the contamination source prevents the contamination from leakage; and, thus, energy is saved and contamination is prevented from leakage with practicality, convenience and safety.

[0022] Please further refer to FIG.4 to FIG.7C, which are views showing a straight curtain, a slightly concave curtain and a severely concave curtain; and views showing the changes of the oscillating curtain at different times. As shown in the figures, push-pull air-isolators are divided into four type, comprising a straight curtain 71, a slightly concave curtain 72, a severely concave curtain 73 and an oscillating curtain 74.

[0023] On using the present invention, flow fields in the main body 11 are described as follows:

(a) Slightly concave curtain 72: When an air-blowing velocity, an air-supplying velocity and an air-sucking velocity are adjusted to obtain a proper ratio, an air-isolator formed by the air from the door 12 is slightly concave inward the BSC. When the flow is close to the suction slot 141, the air flow is pulled down to be prevented from flowing outside or inside the BSC.

(b) Straight curtain 71: When the air-sucking velocity is smaller than the above one and thus is weak, the air isolator formed by the air from the door 12 is straight and not concave with no circulation formed in the cabinet.

(c) Severely concave curtain 73: When the air-sucking velocity is big, the air-isolator is moved inwardly and is severely concave; and, thus, obvious circulations are formed in the BSC.

(d) Oscillating curtain 74: Obvious circulations are generated inside and outside the BSC with the air-isolator swinging in and out of the BSC at different times.

[0024] With the above descriptions concerning the four types of flow fields, it is suggested to adjust push-pull velocities of air to obtain a slightly concave curtain 72 for

operations in the BSC.

[0025] To sum up, the present invention is an air curtain-isolated BSC, where an air-isolator is formed at an opening of a door for isolating air flows inside and outside the BSC to prevent operators from damages owing to contamination leakage from the BSC, and to prevent contamination outside of the BSC from entering into the BSC to pollute a product in the BSC.

Claims

1. An air curtain-isolated biosafety cabinet, comprising:

- a main body (11) having a space to contain a harmful gas to be exhausted and an open space at a side thereof;
 - a telescopic sliding door (12) movably mounted on the main body at the side of the main body (11) to control an opening of said firstmentioned space and having an opening (125) to produce an air-pushing veil (122);
 - a high efficiency particulate air (HEPA) filter (16) arranged on top of the main body (11);
 - an air blower (13) connected with an air inlet (111) to supply fresh air, the air inlet (111) being arranged on top of the HEPA filter (16) to supply air, so that the air blower (13) supplies air through said HEPA filter (16);
 - a suction box (14) located beneath the main body (11) and having a suction slot (141) located at an edge of the main body (11) corresponding to the air-pushing veil (122) of the door; and
 - a gas sucker (15) located at an exit of the suction box (14) to suck the harmful gas,
- characterized by**
- a plurality of cross flow fans set on the door (12),
 - a cross flow fan controller (2) controlling said cross flow fans on the door (12) to thereby control the air flow through the door (12) and its opening (125), wherein air is caused to flow from an upper side of the door (12) through a section of honeycombs (123) and then through a stabilizing passage (124) to dissipate turbulence energy to reach the opening (125),
 - a first inverter (17a) controlling air amount and flow velocity of said air blower (13),
 - a second inverter (17b) controlling gas amount and flow velocity of said gas sucker (15).

2. The air curtain-isolated biosafety cabinet according to claim 1, wherein said door (12) has a handle (121) to move said door (12) to further control an opening of said door.

Patentansprüche

1. Luftvorhangisolierter Biosicherheitsschrank, umfassend:

- einen Hauptkörper (11) mit einem Raum zur Aufnahme eines schädlichen Gases, das ausgestoßen werden soll, und einem offenen Raum an einer Seite;
 - eine Teleskopschiebetür (12), die beweglich an der Seite des Hauptkörpers (11) montiert ist, um die Öffnung des zuvor erwähnten Raums zu kontrollieren, und die eine Öffnung (125) aufweist, um einen luft-drückenden Vorhang (122) zu produzieren;
 - einen Schwebstofffilter (HEPA-Filter) (16), der oben auf dem Hauptkörper (11) angeordnet ist;
 - ein Luftgebläse (13), das mit einem Lufteintritt (111) verbunden ist, um Frischluft zuzuführen, wobei der Lufteintritt (111) oben auf dem HEPA-Filter (16) angeordnet ist, um die Luft so zuzuführen, dass die Luft vom Luftgebläse (13) durch den HEPA-Filter (16) geleitet wird;
 - einen Saugkasten (14), der unter dem Hauptkörper (11) angeordnet ist und einen Saugschlitz (141) aufweist, der an einem Rand des Hauptkörpers (11) angeordnet ist und mit dem luft-drückenden Vorhang (122) der Tür korrespondiert; und
 - einen Gassauger (15), der an einem Austritt des Saugkastens (14) angeordnet ist, um das schädliche Gas abzusaugen,
- gekennzeichnet durch**
- eine Vielzahl von Querstromlüftern, die an der Tür (12) angeordnet sind,
 - eine Querstromlüfter-Steuerung (2), welche die Querstromlüfter an der Tür (12) so steuert, dass der Luftstrom **durch** die Tür (12) und ihre Öffnung (125) kontrolliert wird, wobei die Luft dazu gebracht wird, von der oberen Seite der Tür (12) **durch** einen Abschnitt mit Wabenkörpern (123) und dann **durch** einen stabilisierenden Kanal (124) zu strömen, um die Turbulenzenergie abzuführen und die Öffnung (125) zu erreichen,
 - einen ersten Wechselrichter (17a), der die Luftmenge und Strömungsgeschwindigkeit des Luftgebläses (13) steuert,
 - einen zweiten Wechselrichter (17b), der die Gasmenge und Strömungsgeschwindigkeit des Gassaugers (15) steuert.

2. Luftvorhangisolierter Biosicherheitsschrank nach Anspruch 1, wobei die Tür (12) einen Griff (121) aufweist, damit die Tür (12) zur weiteren Regulierung der Türöffnung bewegt werden kann.

Revendications

1. Enceinte de sécurité biologique isolée par rideau d'air comprenant :

- un corps principal (11) ayant un espace pour contenir un gaz nocif à évacuer et un espace ouvert sur un côté de celui-ci ;
 - une porte coulissante télescopique (12) montée de manière mobile sur le corps principal sur le côté du corps principal (11) pour commander une ouverture de l'espace mentionné en premier et ayant une ouverture (125) pour produire un voile de poussée d'air (122) ;
 - un filtre à air à très haute efficacité (HEPA) (16) arrangé sur le dessus du corps principal (11) ;
 - une soufflante d'air (13) reliée à une entrée d'air (111) pour fournir de l'air frais, l'entrée d'air (111) étant arrangée sur le dessus du filtre HEPA (16) pour fournir de l'air si bien que la soufflante d'air (13) fournit de l'air par le filtre HEPA (16) ;
 - une boîte d'aspiration (14) située sous le corps principal (11) et ayant une fente d'aspiration (141) située sur un bord du corps principal (11) correspondant au voile de poussée d'air (122) de la porte et
 - une ventouse à gaz (15) située à une sortie de la boîte d'aspiration (14) pour aspirer le gaz nocif,
- caractérisée par**
- une pluralité de ventilateurs à flux transversal posés sur la porte (12),
 - un régulateur de ventilateur à flux transversal (2) qui commande lesdits ventilateurs à flux transversal sur la porte (12) pour ainsi commander le flux d'air à travers la porte (12) et son ouverture (125), l'air étant poussé à s'écouler d'un côté supérieur de la porte (12) à travers une section d'alvéoles en nid d'abeille (123) et ensuite à travers un passage de stabilisation (124) pour dissiper l'énergie de turbulence pour atteindre l'ouverture (125),
 - un premier inverseur (17a) commandant la quantité d'air et la vitesse du flux de ladite soufflante d'air (13),
 - un second inverseur (17b) commandant la quantité de gaz et la vitesse du flux à travers ladite ventouse à gaz (15).

2. Enceinte de sécurité biologique isolée par rideau d'air selon la revendication 1, ladite porte (12) ayant une poignée (121) pour déplacer ladite porte (12) pour mieux commander une ouverture de ladite porte.

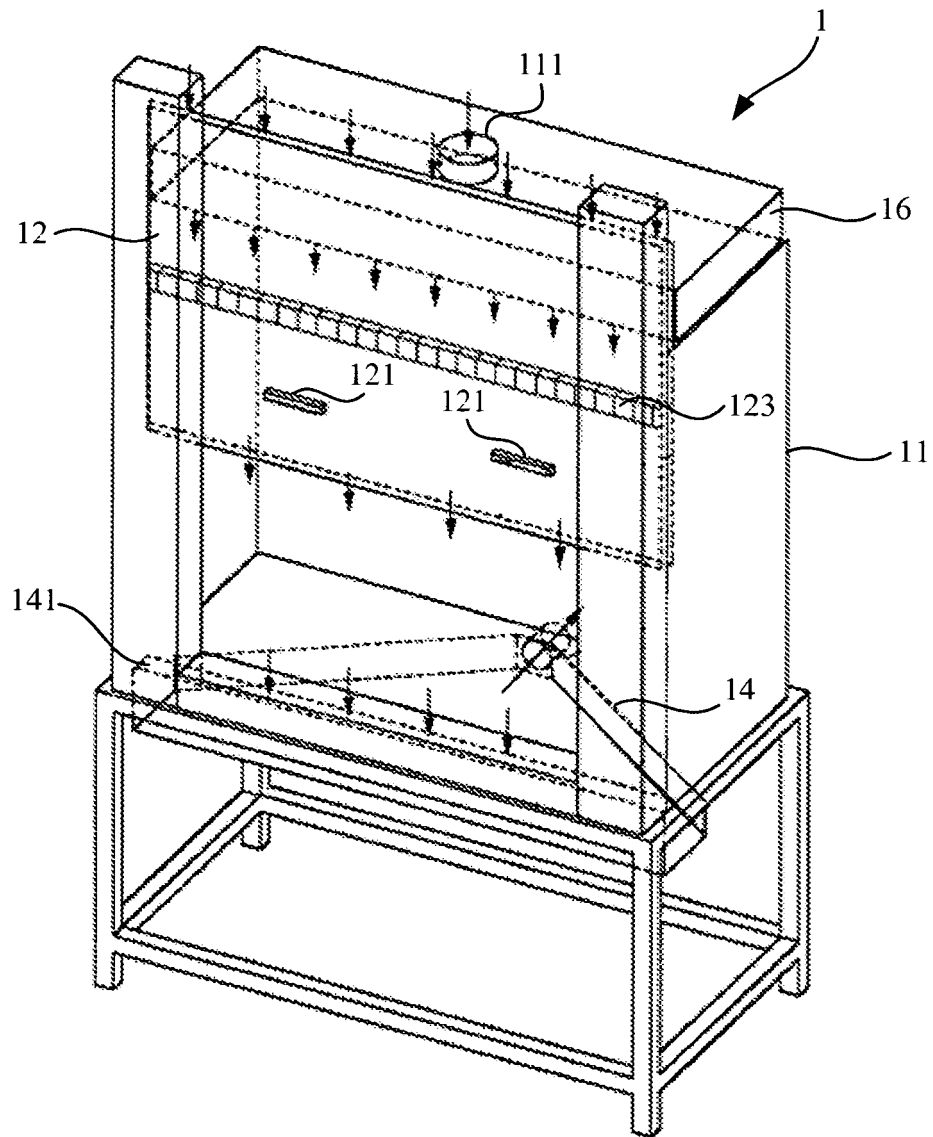


FIG.1

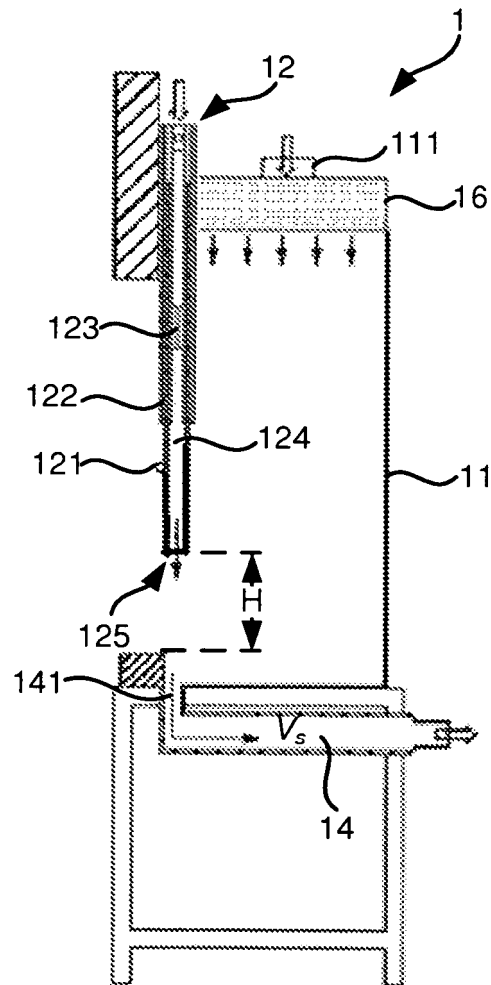


FIG.2

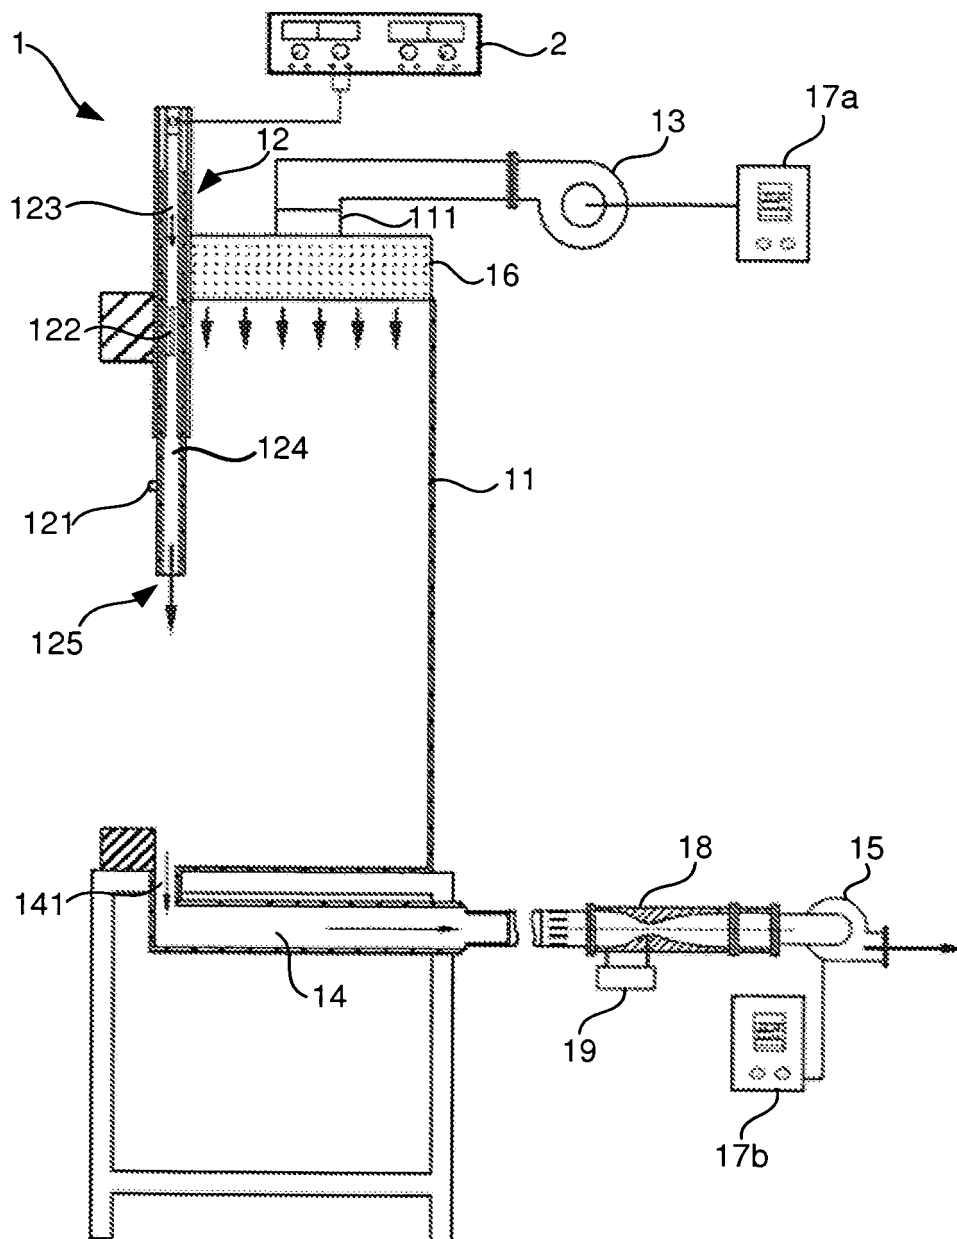


FIG.3

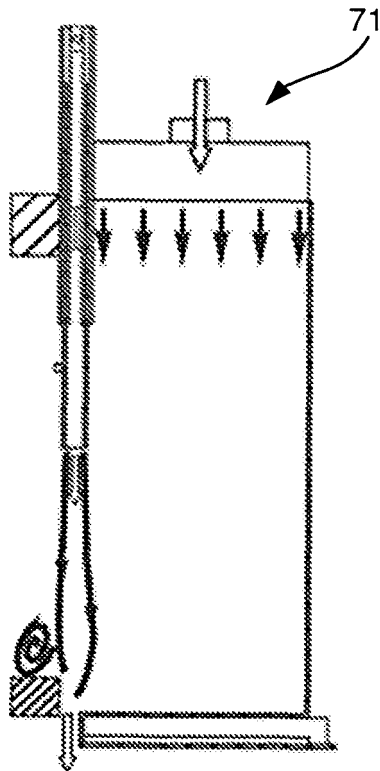


FIG.4

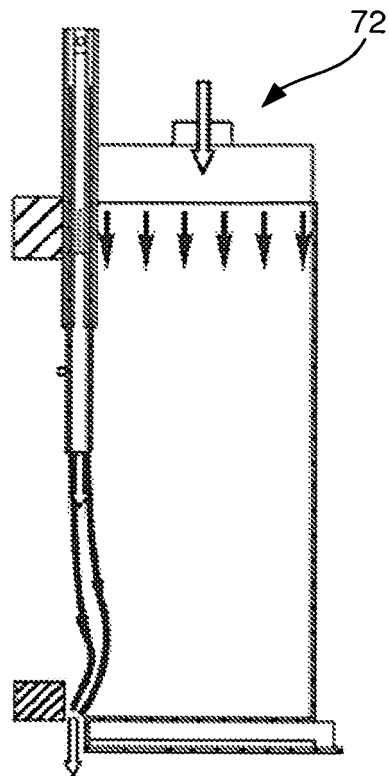


FIG.5

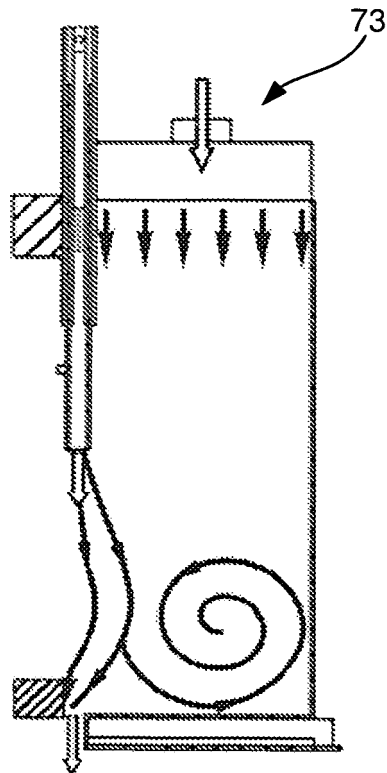


FIG.6

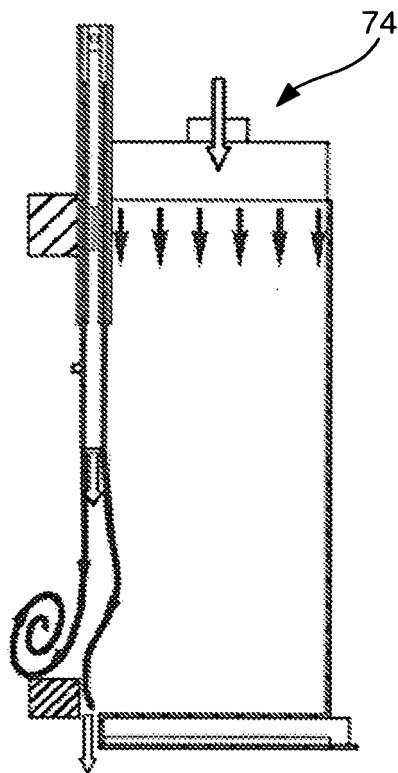


FIG.7A

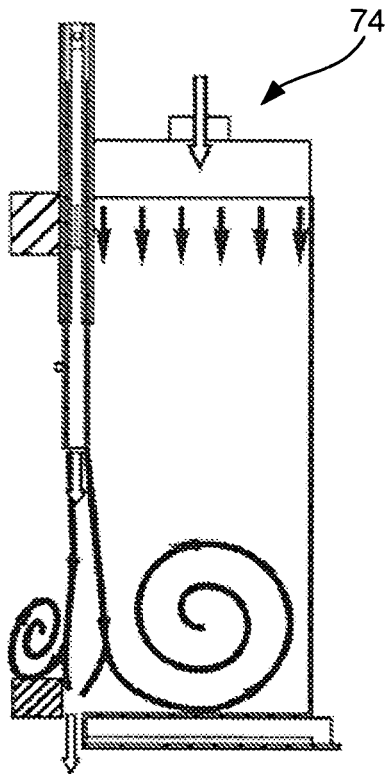


FIG.7B

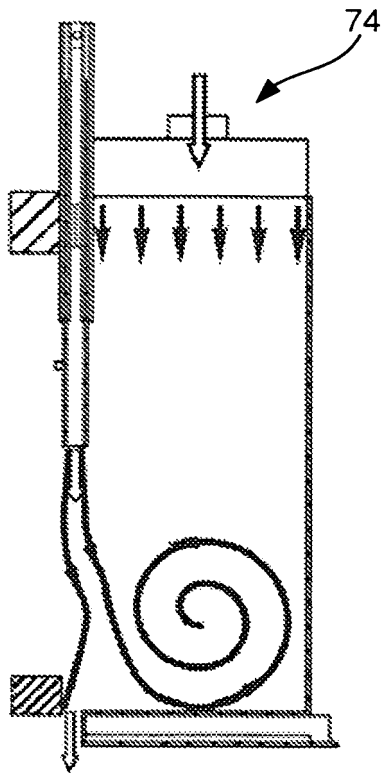


FIG.7C

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- EP 0139128 D1 [0007]
- DE 3811780 A1 [0008]
- EP 1745866 A1 [0008]
- US 4637301 A1 [0008]