

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. **AU 2014305676 B2**

(54) Title
Bone conduction hearing aid system

(51) International Patent Classification(s)
H04R 25/00 (2006.01)

(21) Application No: **2014305676**

(22) Date of Filing: **2014.07.10**

(87) WIPO No: **WO15/020753**

(30) Priority Data

(31) Number
13/963,186

(32) Date
2013.08.09

(33) Country
US

(43) Publication Date: **2015.02.12**

(44) Accepted Journal Date: **2016.12.22**

(71) Applicant(s)
Otorix USA Inc.;Patrik Westerkull

(72) Inventor(s)
Westerkull, Patrik

(74) Agent / Attorney
Griffith Hack, GPO Box 1285, Melbourne, VIC, 3001

(56) Related Art
US 2012/0294466 A1



- (51) International Patent Classification:
H04R 25/00 (2006.01)
- (21) International Application Number:
PCT/US2014/046146
- (22) International Filing Date:
10 July 2014 (10.07.2014)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
13/963,186 9 August 2013 (09.08.2013) US
- (71) Applicant: OTORIX USA INC. [US/US]; c/o Fasth Law Offices, 26 Pinecrest Plaza, Suite 2, Southern Pines, North Carolina 28387 (US).
- (72) Inventor; and
- (71) Applicant: WESTERKULL, Patrik [SE/SE]; Hovås hagstig 26A, S-436 54 Hovås (SE).
- (74) Agent: FASTH, Rolf; FASTH LAW OFFICES, 26 Pinecrest Plaza, Suite 2, Southern Pines, North Carolina 28387 (US).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CL, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

- *without international search report and to be republished upon receipt of that report (Rule 48.2(g))*

(54) Title: BONE CONDUCTION HEARING AID SYSTEM

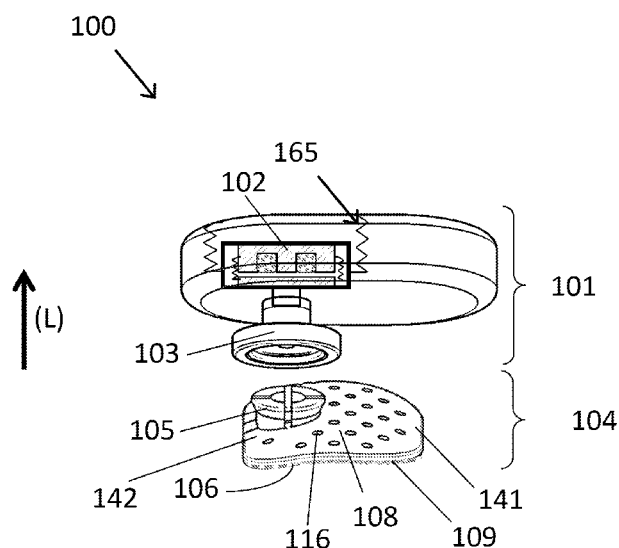


Fig 1.

(57) Abstract: A bone conduction hearing aid system (100) for generating bone conduction vibrations is disclosed. The bone conduction hearing aid system has a hearing aid (101) with a vibrator (102). The hearing aid system includes an interconnection unit (104) to connect the hearing aid to the user (138). The hearing aid (101) has a first connection portion (103) and the interconnection unit (104) has a second connection portion (105) so that there is a coupling between the interconnection unit (104) and the hearing aid (101) to connect and disconnect the hearing aid (101) to and from the interconnection unit (104). The interconnection unit (104) has an adhesive surface (106) facing the skin (113) so that it can be adhered to the skin (113) on the head (139) of the user (138). The sound vibrations are transmitted from the vibrator (102) to the hearing organ (137) as bone conduction sound vibrations.

BONE CONDUCTION HEARING AID SYSTEM

Technical field

The present invention relates to a hearing aid system providing bone conduction hearing.

Background of the invention

Bone conduction is the conduction of sound to the inner ear through the bones of the skull, and a bone conduction hearing aid, or bone conductor, is a device that stimulates through bone conduction. Other types of hearing aids may instead directly stimulate the tympanic membrane, the middle ear ossicles, the round window, the oval window or the cochlear fluid. Several different types of bone conduction hearing aids are available. A bone conduction hearing aid may amplify sound or it may also work as a tinnitus masker. A bone conductor may also be used in audiometry to determine bone conduction hearing thresholds. Current bone conductors include however several drawbacks, as described below.

The traditional bone conductor consists of a hearing aid with a vibrator that is pressed against the head behind the ear by a spring arrangement extending from the other side of the head. The steel spring arrangement is sometimes built into an eyeglass frame. The vibrations are transmitted through the skin and the skull bone into the inner ear. For the traditional bone conductors with a spring arrangement around the head, the constant pressure against the skull bone often causes headaches and skin irritation. The spring arrangement is also bulky and is not a practical or user friendly solution.

Another type of established bone conductor, which is sometimes called a direct bone conductor, includes a vibrator, which is directly and firmly connected to an anchoring component that is anchored to the skull bone through which the vibrations are directly transmitted from the vibrator to the skull bone. The vibrations do not pass through the skin on its way from the vibrator to the skull bone. This type of bone conductor may be designed with a permanent skin penetration which may lead to problems with skin infections. If this type of bone conductor is instead designed with an implanted vibrator and where energy are transmitted from an external hearing aid there is a significant energy loss when transmitting the energy with an inductive link through the skin. Another drawback is that the vibrator cannot easily be repaired if it breaks down.

Another type of bone conductor is a type where the vibrator is placed in an external unit outside the skin and where this external unit is kept in place through a magnetic attachment to a part that is anchored to the skull bone and implanted under the skin. In this arrangement, the signal from the external part is passing through the skin to the implanted part and the skull bone. For this type of bone conductor, surgery is still required and the magnetic force may cause skin necrosis due to the constant pressure against the skin and the hearing aid may also easily fall off.

JP 201 1087142 (A) presents a solution where a vibrator is attached to the skin of a user by means of an adhesive sheet. Although JP 201 1087142 (A) reduces the pressure against the head, it is still in need of further improvements in terms of functionality and comfort.

There is a need for a more effective bone conduction hearing aid system that is reliable and does not have the drawbacks discussed above.

Summary of the invention

The present invention provides a bone conduction hearing aid system, comprising,
a hearing aid device having a vibrator disposed in a hearing aid housing, the hearing aid device having a first connection portion;

an interconnection unit having a first side having a second connection portion (105) and a second side at least partly provided with an adhesive component, the second side being adhesively attachable to a skin of a user, and the first connection portion being removably connectable to the second connection portion,

wherein the second connection portion is non-centrally positioned on the first side of the interconnection unit .

The present invention also provides a method of operating a bone conduction hearing aid system, comprising,

providing a coupling between a first connection portion of a hearing aid device and a second connection portion at a first side of an interconnection unit , the coupling having a female coupling portion and a male coupling portion;

removably attaching an adhesive component of a second side of the interconnection unit onto a skin behind an outer ear on a head of a user;

connecting the hearing aid device to the interconnection unit so that at least a part of the interconnection unit is positioned between the hearing aid device and the skin of the user, by inserting at least a part of the male coupling portion into the female coupling portion to removably connect the hearing aid device to the interconnection unit;

transmitting bone conduction vibrations from the hearing aid device to the user; and

disconnecting the hearing aid device from the interconnection unit without removing the interconnection unit from the skin.

The bone conduction hearing aid system of the present invention has a hearing aid device with a vibrator disposed in a hearing aid housing. The hearing aid device has also a first connection portion. Furthermore, the bone conduction hearing aid system of the present invention has an interconnection unit that has a first side, having a second connection portion, and a second side at least partly provided with an adhesive component. The second side is configured to, when in use, face a skin of a user of the bone conduction hearing aid system. The first connection portion of the hearing aid device is connectable to the second connection portion of the interconnection unit so that these two portions form a coupling. The present invention allows the interconnection unit and the adhesive surface to be at least partly positioned between the

hearing aid device and the skin of the user to enable a practical and efficient use of the bone conduction hearing aid system. The present invention also allows the hearing device to be connected to and disconnected from the interconnection unit without having to, at the same time, connect or disconnect the interconnection unit to the skin of the user.

The bone conduction hearing aid system of the present invention is preferably configured so that the adhesive component is a separately arranged adhesive sheet having a first adhesive surface being connectable to the second surface of the interconnection unit, and a second adhesive surface configured to, when in use, being connectable to the skin of the user of the bone conduction hearing device. This is an efficient way to manufacture the adhesive component on the interconnection unit and may also enable changing a worn out adhesive component of the interconnection unit to a new adhesive component.

The bone conduction hearing aid system of the present invention is preferably configured with at least one through hole extending from the first side to the second side of the interconnecting unit. This allows for moisture and air transportation through the interconnection unit which is beneficial to the skin of the user to which the interconnection unit can be attached with the adhesive component. Preferably, the interconnection unit has several through-holes defined therein and the interconnection unit may also have a porous material for the same purpose.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the interconnection unit has a protective sheet disconnectably arranged on the adhesive component, such that the adhesive component is sandwiched between the protective sheet and the interconnection unit. The protective sheet protects the adhesive component during transportation.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the hearing aid device is rotatable about a rotation spot i.e. in relation to the interconnection unit about a geometric center axis extending through a respective center portion of the first and the second connection portions during use of the bone conduction hearing aid system. With the hearing aid device being rotatable to at least part of a turn, it is possible to somewhat adjust the orientation of the hearing aid device on the head of the user when the hearing aid device is connected to the interconnection unit that is adhesively attached to the skin of the user. This is practical since the orientation of the hearing aid device on the head of the user can then be adjusted without having to tear off the interconnection unit from the skin to reposition it or to attach a new interconnection unit at a new position on the skin.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the second connection portion is positioned non-centrally on the first side of the interconnection unit. The interconnection unit is preferably positioned on the naturally non-hair bearing area behind the ear of the user since the adhesive attachment of the interconnection unit would be less efficient on a hair bearing area. The hearing aid device should not touch the outer ear of the user since this may cause feedback and poor sound quality as well as discomfort. With

the second connection portion being non-centrally positioned on the first side, towards a rear portion of the interconnection unit when the interconnection unit is attached to the skin behind the ear of a user, the hearing aid device is positioned further back to the rear, i.e. further away from the outer ear which reduces the risk of the hearing aid device touching the outer ear. It is desirable not to have to shave off hair behind the naturally non-hair bearing area behind the ear, and the positioning of the second connection portion towards the rear portion of the interconnection unit increases the chances of the hearing aid not touching the outer ear and the interconnection unit still being adhesively attached to the naturally non-hair bearing area behind the ear of the user.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, one of the first and the second connection portion is a female connection portion and the other one of the first and the second connection portion is a male connection portion. Preferably, the male connection portion is at least partly insertable into the female connection portion. This is an efficient design that makes the coupling stable and robust and prevents the hearing aid device from sliding off sideways from the interconnection unit.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the second connection portion is defining a geometric plane. The geometric plane is perpendicular to a geometric center axis extending through a respective center portion of the first and the second connection portions during use of the bone conduction hearing aid system. Preferably, the first connection portion is configured to be tiltably disconnectable to the second connection portion in relation to the geometric plane. This design allows the first connection portion to be disconnected from the second connection portion by applying a tilting force on the hearing aid device when the hearing aid device is connected to the adhesively attached interconnection unit. This significantly reduces the risk of tearing the adhesively attached interconnection unit off from the skin of the user compared to if the hearing aid device would have been disconnected from the interconnection unit through a straight pulling force in a lateral direction. The lateral direction may be a direction pointing out from the head of a user when the bone conduction hearing aid system is worn by the user, and a contra-lateral direction may be an opposite direction to the lateral direction}. The coupling is preferably configured so that the hearing aid device can be disconnected from the interconnection unit without having to manually hold the interconnection unit to the skin to avoid the interconnection unit from inadvertently being torn off from the skin.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the hearing aid device is configured to be rotatably disconnectable from the interconnection unit about a geometric center axis extending through a respective center portion of the first and the second connection portions during use of the bone conduction hearing aid system. This configuration may comprise a disconnecting arrangement having a sloped contact surface in operative engagement with a rotational disconnection surface so that a manually applied rotational force is directed to overcome the connection force keeping the hearing aid device and the interconnection unit connected to each other. In this way, the hearing aid device may be

disconnected from the interconnection unit without having to pull the hearing aid device in the lateral direction to disconnect it from the interconnection unit which may then be undesirably torn off from the skin of the user.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, a portion of the first side is rigid in relation to the remaining portion of the first side, and the second connection portion is positioned on the rigid portion of the first side. It is desirable that at least a part of the interconnection unit is sufficiently rigid and that this part is in sufficiently rigid connection with the second connection portion so that the interconnection unit is not significantly deformed by the torque it is exposed to when, for example, tilting the hearing aid device to disconnect the hearing aid device from the interconnection unit, since significant deformation or bending of the interconnection unit might prevent disconnection of the hearing aid device through tilting. Deformation may also increase the risk of tearing off the interconnection unit from the skin. It may, however, be advantageous to still have part of the interconnection unit be more flexible since it can then more easily adapt to a curvature of the head of a user. A part of the interconnection unit may be transformable from a soft to a rigid state so that it can be more easily shaped to a curvature of the head of a user, but still be sufficiently rigid when in use. The interconnection unit may also be individually manufactured to fit the head curvature of a user by using any available technology for this.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, one of the first and the second connection portions has a permanent magnet, and the other of the first and the second connection portion has at least one of a permanent magnet and a ferromagnetic material so that the first and second connection portions are connectable to each other by magnetism. A magnetic coupling between the hearing aid device and the interconnection unit may be an efficient and durable connection. The coupling may alternatively be configured with, for example, one of the first connection portion and the second connection portion that is flexible in relation to the other of the first connection portion and the second connection portion which may be a more cost efficient solution than a magnetic coupling. The second connection portion may, for example, be a flexible polymer snap connection portion that is flexibly connectable to the first connection-portion. This is an efficient design because the second connection may then be less durable than the first connection portion, and because the interconnection unit is frequently replaced, it is acceptable if the durability of the second connection portion is shorter than the durability of the first connection portion on the hearing aid device which can then be made quite robust. In a preferred embodiment of the present invention, there is a first contact surface of the second connection portion and a second contact surface of the first connection- portion, where the first contact surface and the second contact surface face each other when the first connection portion is connected to the second connection portion. Preferably, the second contact surface is made of a material that has an increased resistance to wear in comparison to the material of the first contact surface.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the hearing aid device has a vibrator suspension device for acoustically isolating the vibrator

from the housing of the hearing aid device which is valuable to reduce the risk for acoustic feedback. The bone conduction hearing aid system of the present invention may also have a second high-frequency vibrator that has a resonance frequency higher than a resonance frequency of the vibrator above to further boost the acoustic high frequency performance.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the second connection portion of the interconnection unit is provided with an adhesive component so that the second connection portion is adhesively attachable to the first connection portion of the hearing aid device. The interconnection unit may then be a double sided adhesive sheet that is attached to the hearing aid device and the hearing aid with the double sided adhesive sheet can then be attached to the head of the user. When the hearing aid device is removed from the head also the interconnection unit, being a double sided adhesive sheet, is removed from the head. The double sided adhesive sheet may then be changed before attaching the hearing aid device to the head again. This alternative design may be efficient since it may offer a low profile and cost efficient design of the interconnection unit.

In a preferred embodiment of the bone conduction hearing aid system of the present invention, the bone conduction hearing aid system further has an implanted unit under the skin that includes an implanted magnetic material. Preferably, there is an external magnetic material in at least one of either the hearing aid device or the interconnection unit, and a permanent magnet in at least one of either the implanted magnetic material or the external magnetic material so that the implanted magnetic material is in operative engagement with the external magnetic material. With this design, the positioning of the adhesive interconnection unit on the head of the user is facilitated. This design may also contribute to improving sound transmission by creating a slight pressure on the skin. The bone conduction hearing aid system of the present invention may also comprise an ear hook to further ensure that the user does not drop the device.

The present invention has several advantages and allows a bone conductor to be retained on the user with an adhesive still allowing the user to take the hearing aid device on and off without having to tear the adhesive off the skin.

A substantial part of the interconnection unit can be located between the hearing aid device and the skin of the user. The bone conduction hearing aid system can then be considerably limited in size on the head of the user. It is in many cases possible to fully place the interconnection unit on the naturally non-hair bearing area behind the ear without requiring arrangements on other parts on the head of the user. The hearing aid device can be easily connected to and disconnected from the interconnection unit without the coupling being sensitive to water and dirt when, for example, connecting the hearing aid device to the interconnection unit after taking a shower (the hearing aid device may not be waterproof whereas the interconnection unit may stay attached to the skin of the user also during for example a shower).

Other advantages of the bone conduction hearing aid system of the present invention are that

the hearing aid device can be standardized since the coupling to the interconnection unit can be the same for more or less all patients which is important since the hearing aid is a quite expensive. The interconnection unit that is more frequently changed and fairly cost efficient to manufacture can, however, easily be manufactured in various shapes and sizes to fit different users.

Another advantage of the bone conduction hearing aid system of the present invention is that it enables the attachment of the interconnection unit to the skin to be a separate process from the connection procedure of the hearing aid device. With the bone conduction hearing aid system of the present invention, the attachment of the adhesive interconnection unit can be done accurately in a controlled situation, for example, in front of a mirror at home, and the interconnection unit will then stay in this position until it is removed after one or several days of usage. The hearing aid device may be connected to the interconnection unit in less controlled situations during the day, and as long as the interconnection unit is correctly placed, the hearing aid device will automatically be correctly positioned on the head, for example, when connecting the hearing aid device to the interconnection unit on the beach after a swim. The interconnection unit of the present invention which adheres to the skin can be changed at an interval that is suitable for the skin, which may be every night or it may, for example, be more seldom like every third day or once a week. The skin can then rest during a night when the interconnection unit is not attached.

The bone conduction hearing aid system of the present invention can be used as a long term treatment for patients with, for example, conductive hearing losses. The bone conduction hearing aid system of the present invention can also be efficient for the rehabilitation of temporary hearing losses due to various middle ear conditions, and it may also be used as a temporary hearing solution to evaluate bone conduction hearing for a patient to decide whether a surgical bone conduction bone conduction hearing aid should be applied on a patient.

The bone conduction hearing aid system of the present invention may also be a bone conduction tinnitus masker used to reduce the handicap of tinnitus, and it may also be applied as a bone conduction stimulator in audiometry to determine bone conduction hearing. In a preferred embodiment of the bone conduction hearing aid system of the present invention, the bone conduction hearing aid system has a signal generator for tinnitus masking.

As described above, the bone conduction hearing aid system of the present invention includes a unique combination of technologies and provides new solutions and several advantages to meet complex user requirements.

Brief description of the drawings

Fig. 1 is a perspective side view overviewing the bone conduction hearing aid system of the present invention when the hearing aid device is not connected to the interconnection unit, and where the vibrator of the hearing aid device has been visualized;

Fig. 2 is a perspective side view overviewing the bone conduction hearing aid system of the present invention when the bone conduction hearing aid system is connected to a user;

Fig. 3A is a side view of the interconnection unit of the present invention with an adhesive component and protective part separated from the interconnection unit;

Fig. 3B is a side view of the embodiment shown in Fig. 3A with the adhesive component and protective part attached to the interconnection unit;

Fig. 3C is a side view of the embodiment shown in Fig. 3B with the protective part partially removed;

Fig. 3D is a side view of the embodiment shown in Fig. 3C with the protective part fully removed and the embodiment attached to a skin portion of a user; Fig. 4 is a perspective side view of an embodiment of the bone conduction hearing aid system of the present invention with a flexible female connection portion of the hearing aid device and a corresponding male connection portion on the first side of the interconnection unit;

Fig. 5A is a side view of an alternative embodiment of the bone conduction hearing aid system of the present invention, and

Fig. 5B is a side view of the embodiment shown in Fig. 5A in a tilted position;

Fig. 6 is a cross-sectional side view of an embodiment of the bone conduction hearing aid system of the present invention including magnetic material in an implanted unit under the skin and a corresponding magnetic material in the interconnection unit;

Fig. 7 A is a perspective side view of an embodiment of the bone conduction hearing aid system of the present invention in a connected position;

Fig. 7B is a perspective side view of the embodiment shown in Fig. 7A in a disconnected position; and

Fig. 8 is a perspective side view of an embodiment of the bone conduction hearing aid system of the present invention with a flexible male connection portion of the hearing aid device and a corresponding female connection portion on a first side of the interconnection unit.

Detailed description

Fig. 1 is a perspective side overview of the bone conduction hearing aid system 100 of the present invention. A hearing aid device 101 has a vibrator 102 (shown as a cross-sectional view) disposed therein. The vibrator 102 is connected to a first connection portion 103 of the hearing

aid device 101. An interconnection unit 104 has a first side 108 and a second side (not shown) opposite to the first side 108. The first side 108 has a second connection portion 105. The first connection portion 103 and the second connection portion 105 form a coupling since they are connectable to each other. The second side has an adhesive component 109. The lateral direction (L) has been marked. A contra-lateral direction may be a direction opposite to the lateral direction (L) and a lateral side of a component may be a side facing the lateral direction and a contra-lateral side may be facing a contra-lateral direction. The first side 108 may, for example, be a lateral side of the interconnection unit 104. The adhesive component 109 has an adhesive surface 106 at the contra-lateral side of the adhesive component 109. The adhesive surface 106 can be removably connected to the skin on the head of a user (best shown in Fig. 2) and the first connection portion 103 can be removably connected to the second connection portion 105 of the interconnection unit 104 by inserting a portion of the second connection portion 103 into a cavity defined inside the portion 105. The hearing aid device 101 can then transmit bone conduction vibrations to the hearing organ of the user (see Fig. 2). The lateral direction (L) may be defined as the direction pointing out from the patient's head when the bone conduction hearing aid system 100 is connected to the skin of the patient. One useful feature is that the patient may simply remove the hearing aid device 101 by snapping the connection portion 103 from the second connection portion 105, and it may, preferably, require less force to remove the connection portion 103 from the connection portion 105 compared to removing the adhesive component 109 from the skin. In this way, the patient may easily remove the hearing aid device 101 from the interconnection unit 104 without inadvertently removing the interconnection unit 104 from the skin of the patient. To ensure this, the first connection portion 103 can be disconnected from the second connection portion 105 by tilting it in relation to the connection portion 105, thus generating significantly less pulling forces on the skin from the adhesive surface 106 when disconnecting the hearing aid device 101 from the interconnection unit 104 adhesively attached to a user. To enable disconnecting the hearing aid device 101 from the unit 104 with a tilting force, the unit 104 is sufficiently rigid so that the unit 104 is not deformed or bent when applying a tilting force since such deformation or bending may prevent the intended disconnection of the hearing aid device 101 from the interconnection unit 104 by using the above described tilting force. Preferably, the connection between connection portions 103 and 105 should have a female-male configuration such that the hearing aid device 101 cannot slide in a sideways direction relative to the interconnection unit 104 i.e. in a direction that is perpendicular to the lateral direction (L). The first connection portion 103 is, preferably, a substantially rigid female connection portion. The second connection portion 105 is, preferably, a male connection portion that consists of flexible and elastic protruding spring arms so that the portion 103 can be snapped onto the portion 105. It is also possible to make portion 105 rigid and portion 103 flexible and elastic. When the first connection portion 103 has been snapped onto the second connection portion 105, the flexible second connection portion 105 establishes a coupling force that keeps the hearing aid device 101 and the interconnection unit 104 together and allows sound vibrations to be transmitted from the vibrator 102 to the interconnection unit 104. The portions 103 and 105 may also include magnetic materials that adhere to one another so that the hearing aid device 101 is magnetically attached to the interconnection unit 104. If magnets are used, it is also preferable that the portions 103 and 105

are configured to have mechanisms to prevent sideways movement such as by using protruding parts that prevent sideways movement of portion 103 relative to portion 105.

The hearing aid device 101 may, in general, also include a microphone, electronics, battery and volume control which are not shown in the drawings. The hearing aid device 101 may include a signal generator to generate for example a noise signal for tinnitus masking or tones for audiometry. The hearing aid device 101 may also be connected with a cord to a conventional audiometer for audiometry.

Preferably, the interconnection unit 104 has a plurality of openings defined therethrough so that air and moisture may be transported through the interconnection unit 104 to reach portions of the patient's skin that is below the surface 106, and opening 116 is one such opening that has been marked.

The female first connection portion 103 can be turned about the center axis of the coupling relative to the male second connection portion 105 connected thereto. This is useful since it is then possible to adjust the orientation of the hearing aid device 101 when it is connected to the interconnection unit 104 attached to the user. Preferably, there should be sufficient friction between the first connection portion 103 and the second connection portion 105 to ensure that the hearing aid device 101 is still kept in an accurate position. The first side 108 has a front portion 141 and a rear portion 142. The front portion 141 is closer to the ear of the user than the rear portion 142 when the interconnection portion is adhered to the skin behind the ear (best shown in Fig. 2). The second connection portion 105 should be eccentrically positioned on the interconnection unit 104 so that the portion is off-center and closer to or at the rear portion 142. One advantage is that the hearing aid device 101 is also positioned further to the rear to avoid the hearing aid device 101 from touching the outer ear of a user. The hearing aid device 101 may also include a vibrator suspension device 165 that suspends the vibrator 102 from the housing of the hearing aid device 101 to minimize feedback problems.

The second connection portion 105 may be an elastic plastic snapping device and the first connection portion 103 may be a more durable female connection so that the wear is on the male connection portion 105 of the interconnection unit 104 which is frequently changed, instead of the wear being on the hearing aid device 101 which would need to be sent to repair when worn out. However, it is also possible to design the portions 103 and 105 so that the male portion 105 is more wear resistant than the female portion 103 and so that the female portion 103 is more flexible and elastic compared to the male portion 105. To achieve a stable and durable coupling, both the female 103 and male 105 connection portions include some substantially rigid mechanical components. The coupling of the bone conduction hearing aid system 100 of the present invention is, preferably, an arrangement between the hearing aid device 101 and the interconnection unit 104 that is quite stiff when these are connected to each other to ensure an efficient transmission of the vibrations from the vibrator 102 of the hearing aid device 101 to the interconnection unit 104 without damping or distortion of the signal. Fig. 2 is a perspective side overview of the bone conduction hearing aid system 100 of the present

invention when it is in position on and attached to a skin 113 on the head 139 of a user 138. The hearing aid device 101 is connected to the interconnection unit 104 which is connected with an adhesive surface to the skin behind the ear 107 of the user. Sound vibrations are transmitted from the hearing aid device 101 via the interconnection unit 104 to the head of the user to stimulate the hearing organ 137 in the head 139 through bone conduction.

Figs. 3A-3D are side views of the composition (Fig. 3A and Fig. 3B) and the application (Fig. 3C and Fig. 3D) of the interconnection unit 104 of the bone conduction hearing aid system of the present invention. A lateral direction (L) has been marked. In Fig. 3A the following separated parts are shown before assembly in manufacturing: the interconnection unit 104 has a first side 108, a second side 120 and an adhesive component 109 that may be a double-sided adhesive sheet, and a protective part 110 that is useful to protect a contra-lateral adhesive surface 106 of the adhesive component 109 during transportation and the protective part also prevents the adhesive from attaching to the skin of a user when trying out a suitable curvature version of the interconnection unit 104 for a specific user. A user-friendly feature is that the adhesive component (such as a double-sided adhesive sheet) 109 is adapted to be applied to the skin and that it allows oxygen to penetrate therethrough. It is also possible for the user to remove the interconnection unit 104 completely, for example, during a night so that the skin is not permanently interfered with and can "breathe" and function normally when the patient does not need to use the bone conduction hearing aid system 100. It may also be possible to configure the adhesive component 109 as an adhesive, such as glue, that is directly applied to the second side 120 instead of configuring it as a double-side adhesive sheet. However, the use of a double-sided adhesive sheet may be efficient in manufacturing when applying a contra-lateral adhesive surface 106 to the second side 120. The protective part may be a polymer sheet. The double-sided adhesive sheet or component 109 has a lateral adhesive surface 112 facing the first side 108. Instead of using an adhesive on the surface 112, it is also possible to use other removable attachment mechanisms such as Velcro or separate glue. Since the sheet 109 may be removably attached to the second side 120 it is also possible to change the sheet 109 on the interconnection unit 104 if this is more cost efficient than just to take a new complete interconnection unit 104 that includes a new sheet 109. In Fig. 3B, the parts shown in Fig. 3A have been assembled so that the double-sided adhesive sheet 109 has been adhered to the second side 120, and the protective part 110 has been attached to the other side 106 of the double-sided adhesive sheet 109 so that the unit is ready for transportation. In Fig. 3C, the protective part 110 is removed from the adhesive surface 106 of the double-sided adhesive sheet 109 by applying a force (F) to expose the contra-lateral adhesive surface 106. In Fig. 3D, the interconnection unit 104 with its double-sided adhesive sheet 109 has been adhesively attached to the skin 113 on the head of a user.

Fig. 4 is a perspective side view of the bone conduction hearing aid system 400 of the present invention. A hearing aid device 401 has a first connection portion 403. An interconnection unit 404 has a first side 408 and a conical-shaped connection portion 405 and an adhesive surface 406 at its contra-lateral side. The bone conduction hearing aid system 400 is similar to the

embodiment shown in Fig. 1, however, the first connection portion 403 and the second connection portion 405 are different, and the interconnection unit 404 has a flexible portion 415. The first connection portion 403 is a female coupling that has a flexible portion and a recess defined therein. The connection portion 405 may be a rigid male coupling so that the flexible female coupling of the connection portion 403 can be snapped onto the male coupling of the connection portion 405. Because an inner diameter of the recess of the flexible female coupling is slightly smaller than an outer diameter of the male coupling, the flexible and elastic female coupling of first connection portion 403 generates a coupling force about the male coupling of the connection portion 405 that keeps the hearing aid device 401 and the interconnection unit 404 together. The first connection portion 403 also acts as a member around the protruding second connection portion 405 that hinders the hearing aid device 401 from sliding off the interconnection unit 404 in a sideways direction (i.e. a direction perpendicular to a lateral direction (L)). The adhesive surface 406 on the contra-lateral side of the interconnection unit 404 is preferably attached to a skin surface behind the ear of the user (best shown in Fig. 2). The first side 408 has a rigid portion 414 and a softer flexible and bendable peripheral portion 415 to facilitate adhesion of the adhesive surface 406 to the skin surfaces of various curvatures. Because the rigid portion 414 is sufficiently rigid, it makes it easier for the user to separate connection 403 from connection 405, especially when disconnecting 401 is tilted in relation to 404. It is an important feature that the interconnection unit 404 both has a non-rigid or flexible portion 415 that is adaptable to the curvature of the skull of the patient while the rigid portion 414 makes it easier to remove the hearing aid device 401 from the interconnection unit 404. The interconnection unit 404 has through holes 416 for air and moisture transportation to and from the skin through the interconnection unit 404.

Figs. 5A and 5B are side views of the bone conduction hearing aid system 100 of the present invention having the hearing aid device 101 and the interconnection unit 104. Figs. 5A and 5B are intended to visualize the process when disconnecting the hearing aid device 101 from the interconnection unit 104 by applying a manual tilting force (F_m) on the hearing aid device 101. The interconnection unit 104 is attached with an adhesive to the skin 113 of the user. In Fig. 5A, the manual force (F_m) in contra-lateral direction is applied to a side end 167 of the hearing aid device 101. The side end 167 of the device 101 is located away from the first connection portion 103. The manual force (F_m) creates a torque that is counter-acted by a counter-acting force (F_c) in a rotation contact spot 160 in the interface between the first connection portion 103 and the second connection portion 105, and by a retention force (F_r). The retention force (F_r) is established by the flexible conical second connection portion 105 connected to or inserted into a recess in the rigid female first connection portion 103. In Fig. 5B, the retention force (F_r) has been overcome and the hearing aid device 101 is rotated or tilted off from the interconnection unit 104 about the rotation contact spot 160. As explained in more detail above, the first side 108 may, preferably, have a sufficiently rigid portion that partially or fully covers the side 108 so that the interconnection unit 104 can counteract the manual force (F_m) against the skin 113 and so that the interconnection unit 104 does not undesirably bend because a bending or deformation of the interconnection unit 104 may prevent the manual force 5 (F_m) from disconnecting the hearing aid device 101 from the interconnection unit 104 when the user is

applying the manual tilting force (F_m). With this configuration, the hearing aid device 101 may be disconnected from the unit 104 with manual forces that includes a force also in contra-lateral direction which minimizes the risk of the interconnection unit 104 being torn off from the skin 113 when the device 101 is disconnected from the unit 104.

Fig. 6 is a cross-sectional side view of a bone conduction hearing aid system 600 of the present invention. A hearing aid device 601 has a vibrator 602 and a first connection portion 603. An interconnection unit 604 has a second connection portion 605 and an adhesive component 609 being adhesively connectable to a skin 613 of a user. The interconnection unit 604 includes an external magnet material 628. An implanted unit 629 includes an implanted magnet material 630. One of the material 628 and the material 630 has a permanent magnet, and the other one of the material 628 and the material 630 has at least one of a permanent magnet and a ferromagnetic material so that unit 604 and unit 629 are connectable to each other by magnetism. The implanted unit 629 is located under the skin 613 and it is fixated to a skull bone 632 with a fixation device such as a fastener 633. The magnetic attraction between the external magnet 628 and the implanted magnet 630 presses the interconnection unit 604 towards the skin 613 to enhance sound transmission and to facilitate positioning of the interconnection unit 604 when attaching its adhesive component 609 to the skin 613. The interconnection unit 604 and the hearing aid device 601 are substantially retained on the user by the adhesive component 609 of the interconnection unit 604, although the magnetic interaction also contributes to the retention. The first connection portion 603 may be a permanent magnet and the second connection portion 605 may include a ferromagnetic material so that also the coupling between the interconnection unit 604 and the hearing aid device 601 is established by magnetic interaction.

Figs. 7 A and 7B are perspective side views of a bone conduction hearing aid system 700 of the present invention. In Fig. 7A, a hearing aid device 701 is connected to an interconnection unit 704 and in Fig. 7B, the hearing aid device 701 has been disconnected from the interconnection unit 704. The bone conduction hearing aid system 700 is similar to the embodiment of Fig. 1. However, the bone conduction hearing aid system 700 also includes a disconnecting arrangement to facilitate the disconnection of the hearing aid device 701 from the interconnection unit 704. In Fig. 7B, the hearing aid device 701 has been rotated 90 degrees in a clockwise direction about an axis parallel to the lateral direction (L) in relation to the interconnection unit 704 compared to the position of the hearing aid device 701 in Fig. 7A. The hearing aid device 701 has a first connection portion and a hearing aid disconnection portion 725 with a sloping contact surface 727. The interconnection unit 704 has a second connection portion 705 and a disconnection portion 724 with a sloping contact surface 726. The interconnection unit 704 an adhesive component 709 that can be attached to a skin of a user, as described earlier. The lateral direction (L) is marked and a contra-lateral direction is opposite to the lateral direction (L) .

Preferably, the first connection portion 703 is a rigid female connection portion. Preferably, the second connection portion 705 is a male connection portion that consists of flexible spring arms

so that the first connection portion 703 can be snapped on to it. The disconnection portion 724 extends further in the lateral direction than the most contra-lateral portion of the disconnection portion 725. When the hearing aid device 701 is rotated in the clockwise direction about a geometric center axis (parallel to the lateral direction) extending through a respective center portion of the first and the second connection in fig. 7A, the sloping contact surface 726 come in contact with the sloping contact surface 727 so that the rotational force creates an axial force parallel to the lateral direction (L) that urges the first connection portion 703 and the second connection portion 705 to disconnect from one another. In this way, the hearing aid device 701 can be rotated to disconnect it from the interconnection unit 704 instead of pulling it off with a force in lateral direction (L) which may cause the adhesive component 709 to be torn off from the skin of the user when the interconnection unit 704 is adhesively attached to the user. The disconnection arrangement may be designed in various ways depending on the design of the coupling. For example, the hearing aid device 701 may be disconnected from the interconnection unit 704 by turning the units in a counter-clockwise direction relative to one another. A disconnection arrangement may also be designed as a control handle so that a user can press a handle to counteract the coupling force to gently disconnect the hearing aid device 701.

Fig. 8 is a perspective side view of the bone conduction hearing aid system 800 of the present invention. The embodiment shown in Fig. 8 is very similar to the embodiment shown in Fig. 1 except that the positions of the male and female connections have been switched so that the female coupling is on the interconnection unit while the male coupling is on the hearing aid device. More particularly, a hearing aid device 801 has a first male connection portion 803. An interconnection unit 804 has a second connection portion 805 and an adhesive component 809. The first portion 803 is a flexible male coupling so that it can be removably snapped into the female portion 805. The female connection portion 805 has a recess 870 defined therein so that the first connection portion 803 can be retained to the portion 805. The way the male portion 803 connects to the female portion 805 is substantially similar to the embodiment of Fig. 1 except that the male and female portions have been switched. More particularly, the first connection portion 803 generates a coupling force that keeps the hearing aid device 801 and the interconnection unit 804 together. The female second connection portion 805 also acts as a member around the portion 805 to hinder the hearing aid device 801 to slide off from the unit 804 in a sidewise direction (i.e. a direction perpendicular to a lateral direction (L)). The adhesive segment 809 allows the interconnection unit 804 to be removably connected to a skin of the user. The hearing aid device 801 includes a tinnitus masking signal generator 881. The signal from the tinnitus masking signal generator 881 is transferred into vibrations by the vibrator 802 that is also located in the hearing aid device 801, and the vibrations is then transmitted to the hearing organ through bone conduction.

The vibrator of the present invention may be any suitable type of vibrator such as an electromagnetic vibrator or a piezoelectric vibrator. The amplifier of the hearing aid device may, for example, include digital processing, directional microphones, noise reduction, feedback suppression and other electronic and software features that are beneficial and used in any

suitable type of regular hearing aid. The hearing aid device may consist of one housing unit where all electronics are included, or it may consist of two or more separate housing units where different parts of the electronics are included in the different housings and where the separate housing units communicate with each other via wire or wireless communication. The interconnection unit may have a bulb or knob in part of the area facing the skin to create a local light pressure against the skin to further enhance sound transmission.

In the past, it has been assumed that it is necessary to apply a fairly high pressure to transmit bone conduction vibrations through the skin regardless of whether the bone conductor has been applied with an elastic or adhesive arrangement. In the present invention, it has been surprisingly realized that bone conduction work efficiently also without any pressure applied against the skin. In the prior art designs of hearing aid systems, it has also been assumed that an adhesively attached bone conductor requires an adhesive patch that extend over the hearing aid device so that the ends of the adhesive patch may be attached to the head. In other words, the prior art adhesive patch or band encloses the hearing aid device and the adhesive is therefore attached directly to the top of the hearing aid device to hold the entire hearing aid system in place on the head of the user. By stretching the prior art adhesive patch over the hearing aid device, the adhesive patch also provides an inwardly directed pressure onto the hearing aid system that, in turn, is pressed against the skin. The adhesive attachment area on the head of the user may then also have to be quite large. As indicated above, it was believed necessary in the past to apply a pressure on the skin to not only hold the hearing aid system in place but also to ensure proper conveyance of vibrations into the skull of the user. No one has realized that it is possible to place the adhesive in the area between the hearing aid system and the skin i.e. place the adhesive on the contact area of the hearing aid system that is directly applied to the skin to hold the hearing aid system in place on the skin behind the ear. More particularly, the hearing aid system of the present invention is preferably placed and adhered to the area of the skin behind the ear that does not have any hair growing thereon. It was unexpectedly realized that although no or very little pressure is being applied on the skin by the adhesive, the vibrations from the hearing aid system are properly and effectively being conveyed into the skull of the user while holding the hearing aid system in place so that the user can move without the hearing aid system undesirably moving or falling off. The adhesive carrier can at least partly be located between the bone conductor of the hearing aid device and the skin. In the present invention, it was also unexpectedly discovered that the adherence between the interconnection unit and the skin is sufficiently strong to make it possible to use a properly designed mechanically stable coupling between the interconnection unit and the hearing aid device so that the hearing aid device can conveniently be connected to and disconnected from the interconnection unit without undesirably moving or tearing off the interconnection unit from the skin. It was also surprisingly discovered that an adhesively attached bone conductor can be designed in one housing without feedback problems and without requiring a cord to a separate unit. An important feature of the present invention is thus that it is not necessary to apply a pressure on the skin in order to be able to properly and effectively convey the vibrations from the hearing aid unit into the skull of the user and to hold the hearing aid system in place while the user is moving. The fact that no or very little pressure is being applied on the skin is

more comfortable to the user and reduces the risk for not only discomfort in the area of attachment but also enhances the general comfort of the user because there is less strain on the skull. Another important feature is that the adherence is sufficiently strong so that the user can easily snap on and snap off the hearing aid device from the interconnection unit without tearing off the interconnection unit from the skin. This makes it possible for the user to only attach the hearing aid device to the interconnection unit when necessary but also the user can easily remove it without removing the interconnection unit when needed such as when sleeping or swimming.

For all of the above embodiments several alternative designs and combinations are possible and the invention is not limited to the preferred embodiments presented above. While the present invention has been described in accordance with preferred compositions and embodiments, it is to be understood that certain substitutions and alterations may be made thereto without departing from the spirit and scope of the following claims.

It is to be understood that, if any prior art is referred to herein, such reference does not constitute an admission that such prior art forms a part of the common general knowledge in the art, in Australia or any other country.

In the claims that follow and in the preceding description of the invention, except where the context requires otherwise due to express language or necessary implication, the word “comprise” or variations such as “comprises” or “comprising” is used in an inclusive sense, i.e. to specify the presence of the stated features but not to preclude the presence or addition of further features in various embodiments of the invention.

Claims

1. A bone conduction hearing aid system, comprising,
a hearing aid device having a vibrator disposed in a hearing aid housing, the hearing aid device having a first connection portion;
an interconnection unit having a first side having a second connection portion and a second side at least partly provided with an adhesive component, the second side being adhesively attachable to a skin of a user, and the first connection portion being removably connectable to the second connection portion,
wherein the second connection portion is non-centrally positioned on the first side of the interconnection unit .
2. The bone conduction hearing aid system according to claim 1 , wherein the adhesive component is a separately arranged adhesive sheet having a first adhesive surface being connectable to the second surface of the interconnection unit, and a second adhesive surface being connectable to the skin of the user.
3. The bone conduction hearing aid system according to claim 1 wherein the interconnection unit has at least one through hole defined therein extending from the first side to the second side of the interconnecting unit.
4. The bone conduction hearing aid system according to claim 1 , wherein the interconnection unit has a protective sheet being disconnectably arranged on the adhesive component, such that the adhesive component is sandwiched between the protective sheet and the interconnection unit.
5. The bone conduction hearing aid system according to any one of claims 1 to 4, wherein the hearing aid device is rotatable about a rotation contact spot.
6. The bone conduction hearing aid system according to any one of claims 1 to 5, wherein one of the first and the second connection portion is a female connection portion and the other of the first and the second connection portion is a male connection portion, and wherein the male connection portion is at least partly insertable into the female connection portion.
7. The bone conduction hearing aid system according to any one of claims 1 to 6 , wherein the first connection portion is tiltably disconnectable from the second connection portion .
8. The bone conduction hearing aid system according to any one of claims 1 to 7, wherein the first side has a rigid portion that is more rigid than a non-rigid portion of the first side, and the second connection portion is positioned on the rigid portion of the first side .
9. The bone conduction hearing aid system according to any one of claims 1 to 8, wherein the hearing aid device is rotatably disconnectable from the interconnection unit.

10. The bone conduction hearing aid system according to any one of claims 1 to 9 wherein one of the first and the second connection portions has a permanent magnet, and the other of the first and the second connection portion has at least one of a permanent magnet and a ferromagnetic material so that the first and second connection portions are connectable to each other by magnetism.
11. The bone conduction hearing aid system according to any one of claims 1 to 10 wherein the hearing aid device has a vibrator suspension device.
12. The bone conduction hearing aid system according to any one of claims 1 to 11 , wherein the bone conduction hearing aid system has an implanted unit under the skin having:
- an implanted magnetic material;
 - an external magnetic material in at least one of either the hearing aid device or the interconnection unit, and
 - a permanent magnet in at least one of either the implanted magnetic material or the external magnetic material, the implanted magnetic material is in operative engagement with the external magnetic material.
13. The bone conduction hearing aid system according to any one of claims 1 to 12 , wherein the bone conduction hearing aid system has a tinnitus masking signal generator.
14. A method of operating a bone conduction hearing aid system, comprising,
- providing a coupling between a first connection portion of a hearing aid device and a second connection portion at a first side of an interconnection unit , the coupling having a female coupling portion and a male coupling portion, and wherein the second connection portion is non-centrally positioned on the first side of the interconnection unit;
 - removably attaching an adhesive component of a second side of the interconnection unit onto a skin behind an outer ear on a head of a user;
 - connecting the hearing aid device to the interconnection unit so that at least a part of the interconnection unit is positioned between the hearing aid device and the skin of the user, by inserting at least a part of the male coupling portion into the female coupling portion to removably connect the hearing aid device to the interconnection unit;
 - transmitting bone conduction vibrations from the hearing aid device to the user; and
 - disconnecting the hearing aid device from the interconnection unit without removing the interconnection unit from the skin.
15. The method of claim 14 wherein the method further comprises the steps of:
- providing the interconnection unit with a rear portion having the second connection portion being positioned at the rear portion of the interconnection unit; and
 - removably attaching the interconnection unit onto a skin behind the outer ear of a user with the interconnection unit oriented so that the rear portion is positioned away from the outer ear.

1/8

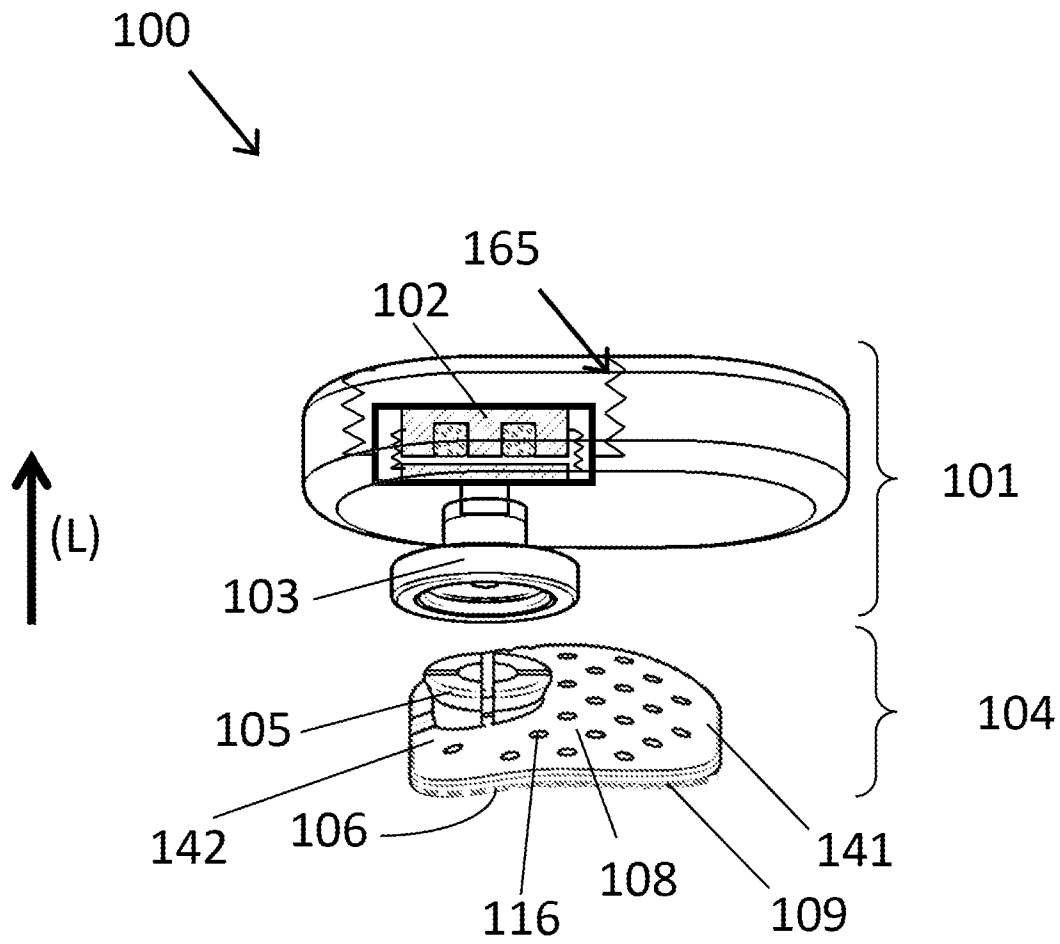


Fig 1.

2/8


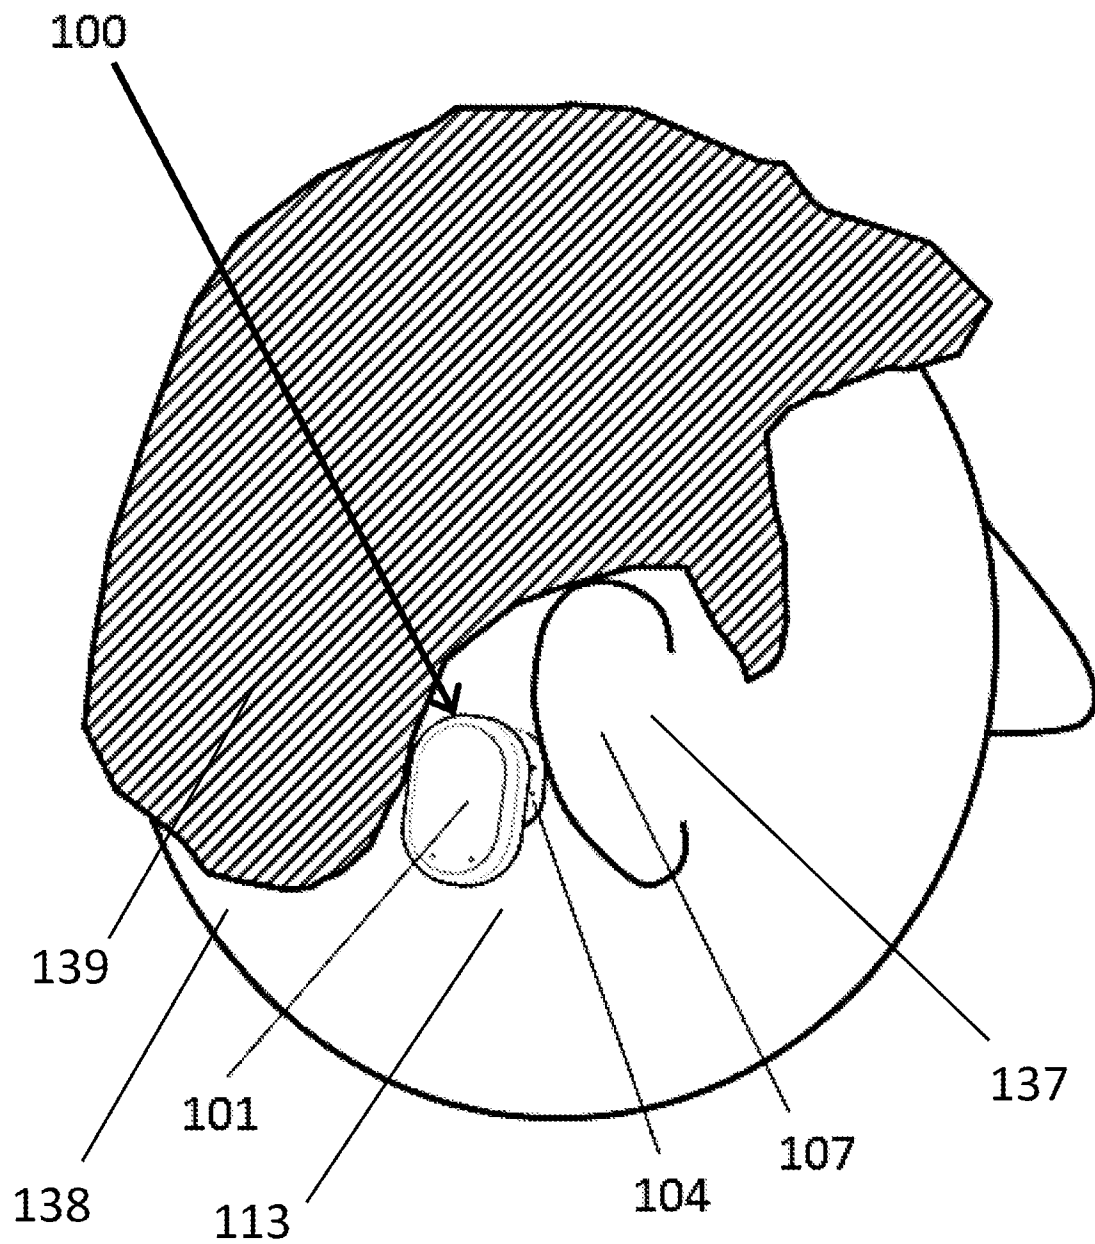


Fig 2.

3/8

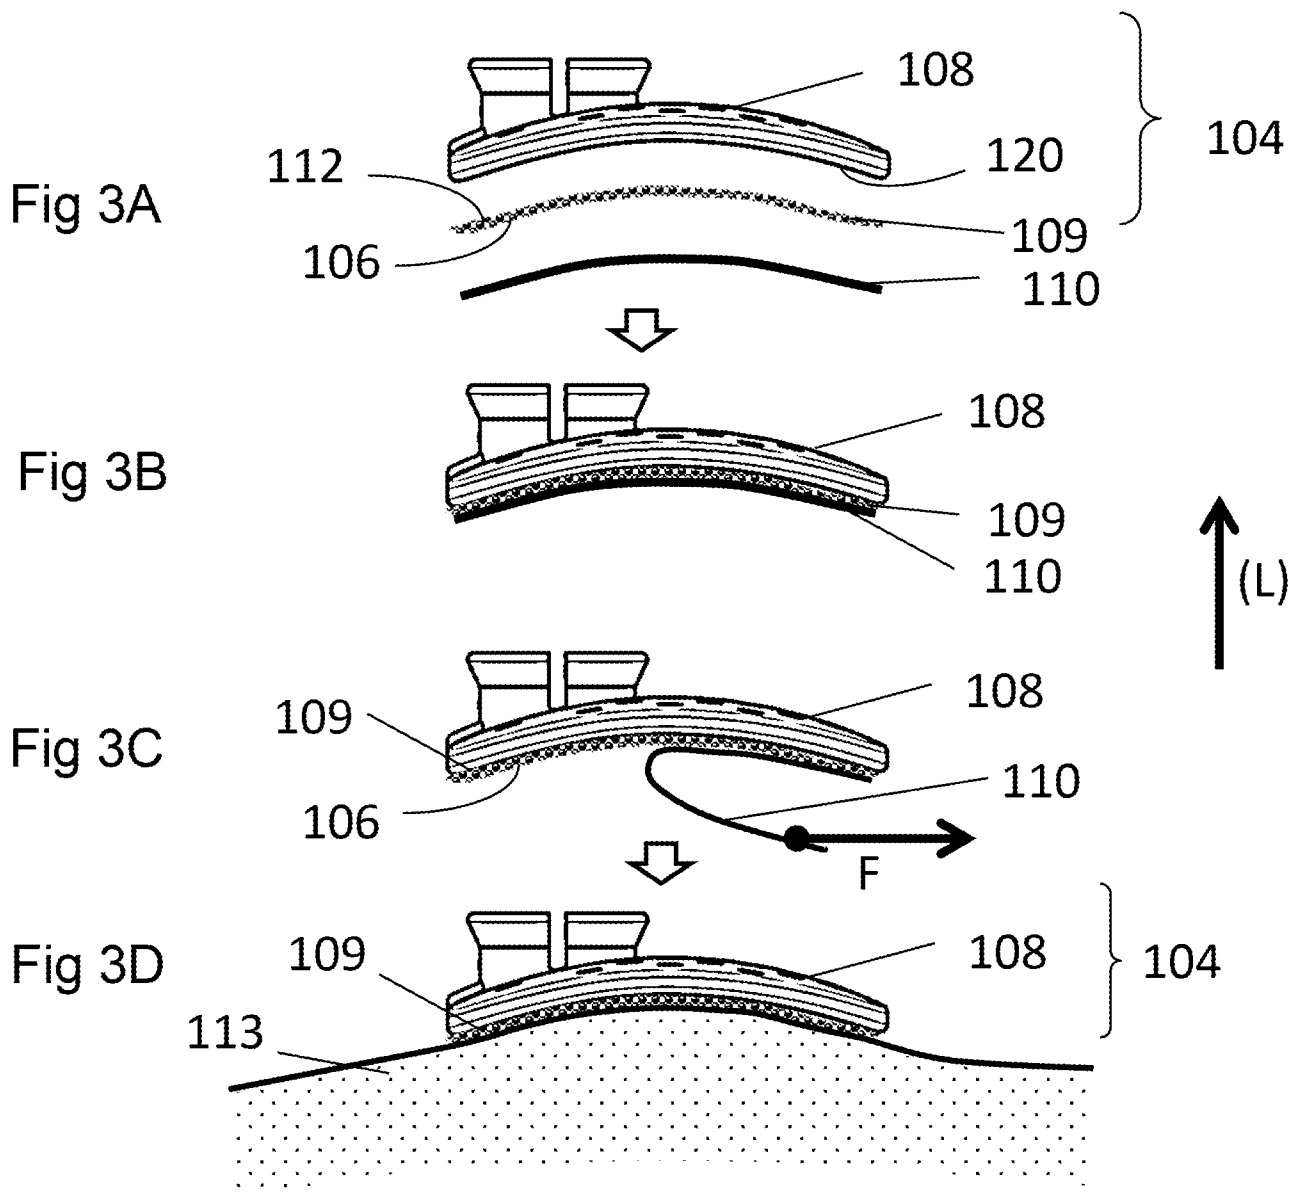

Figs 3 A – 3 D.

4/8



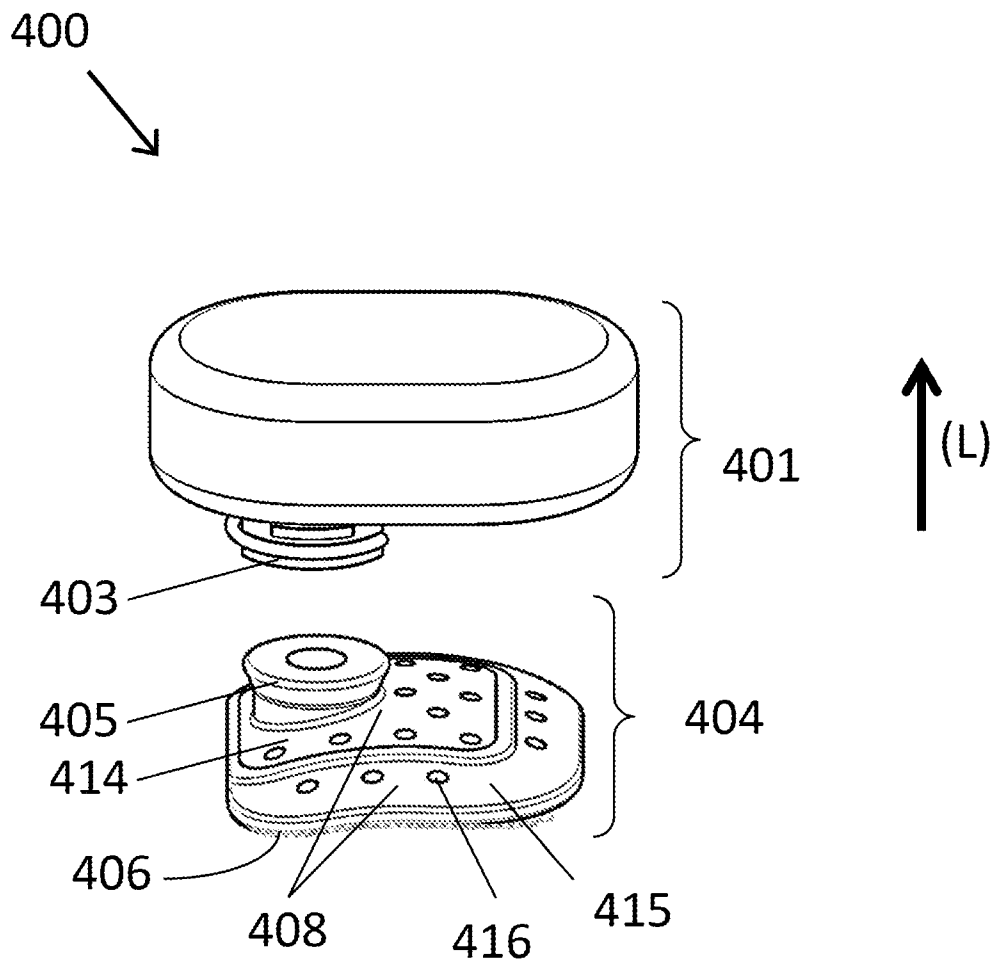


Fig 4.

5/8

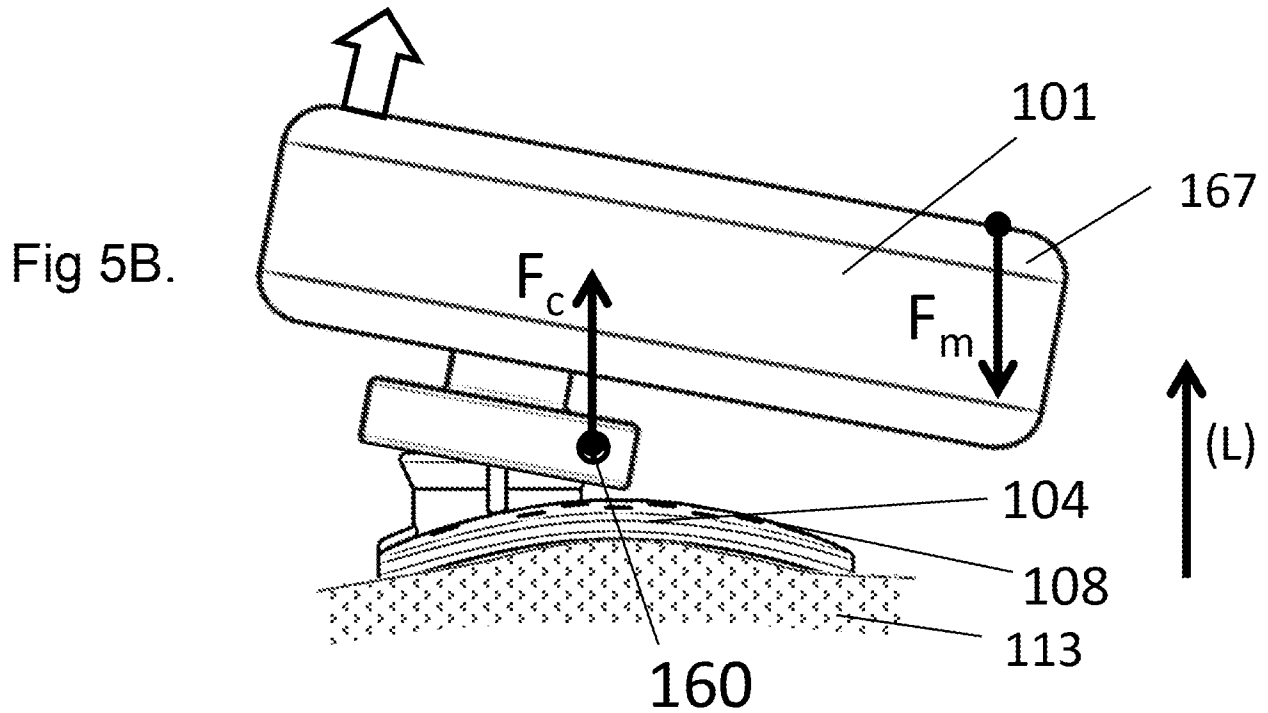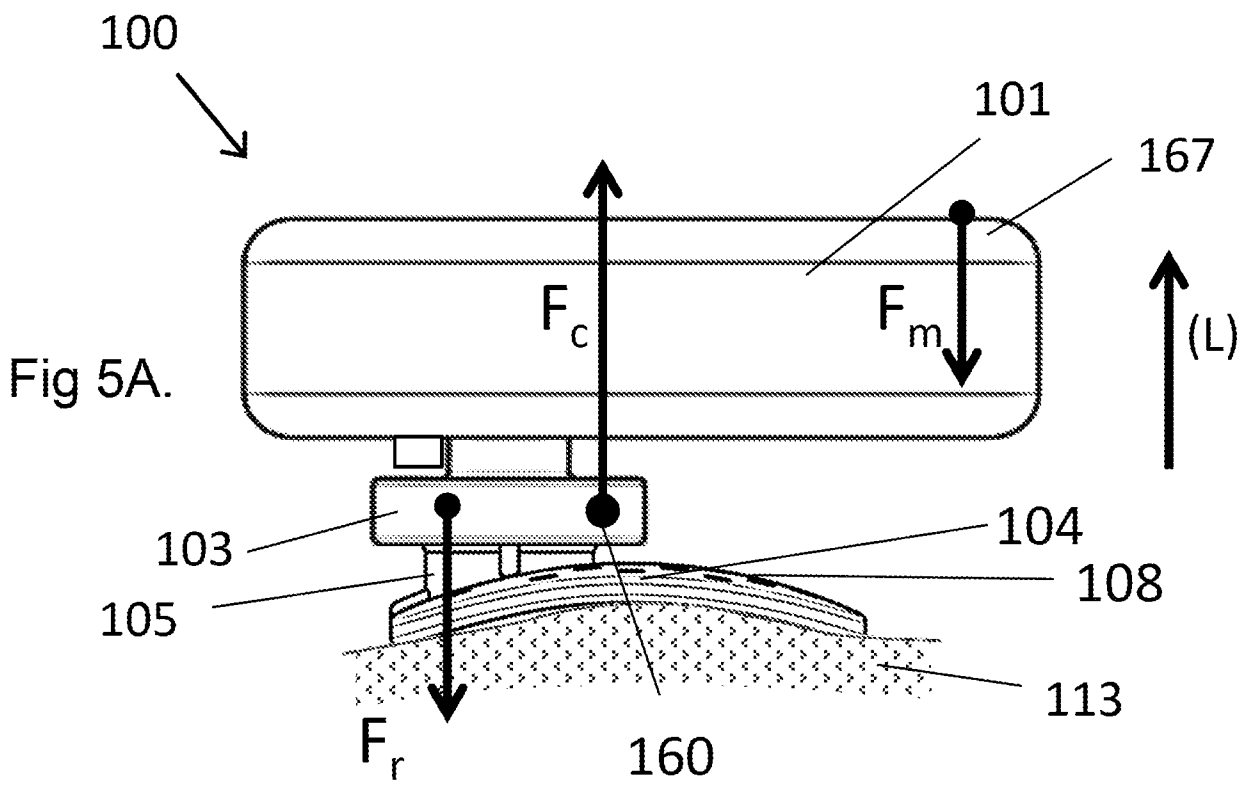

Figs 5A & 5B.

6/8

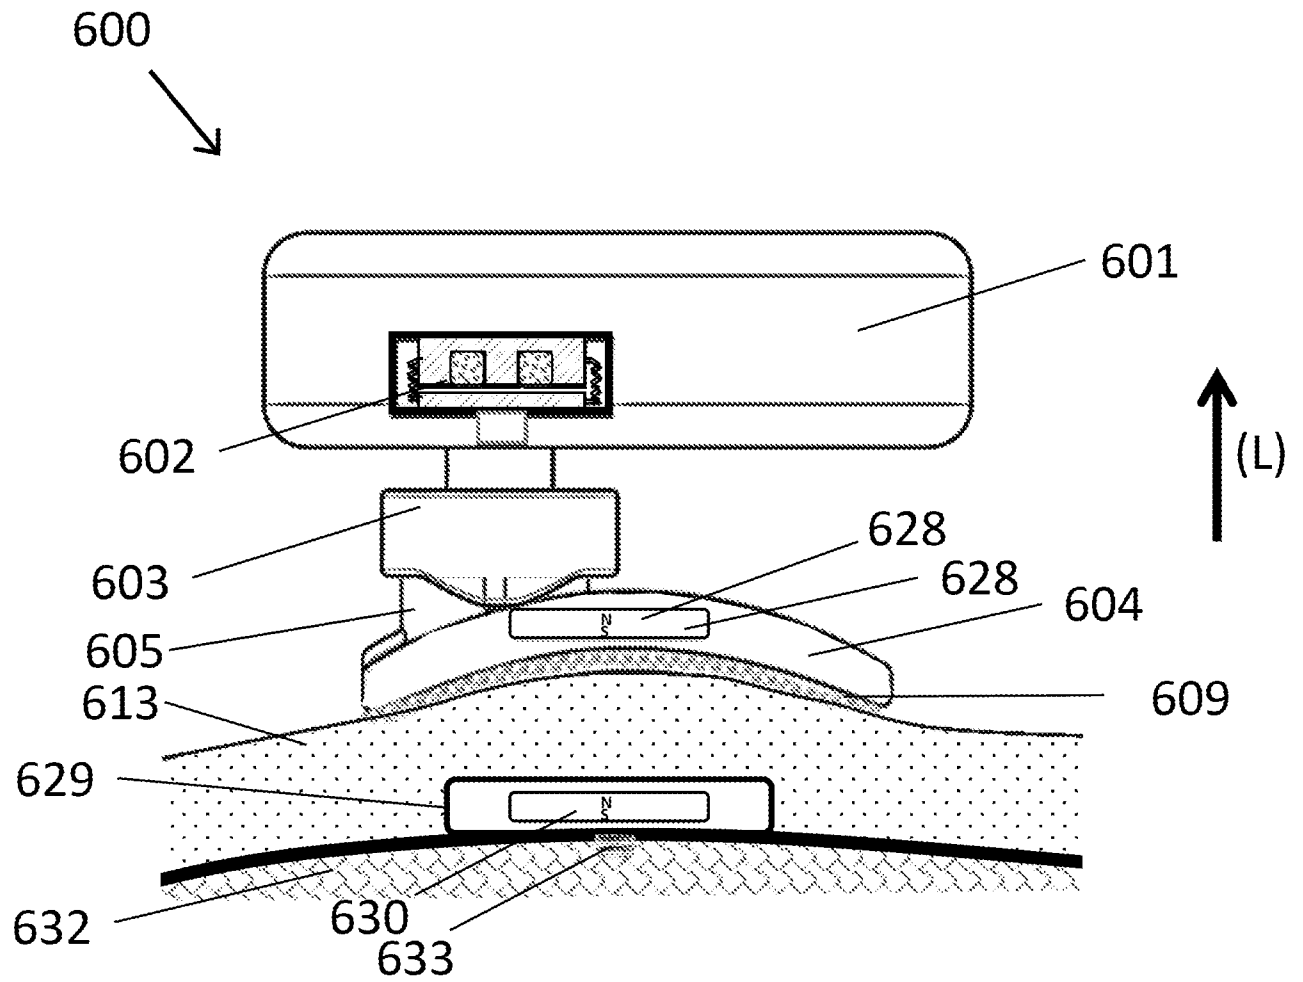


Fig 6.

7/8

700
↙

Fig 7A


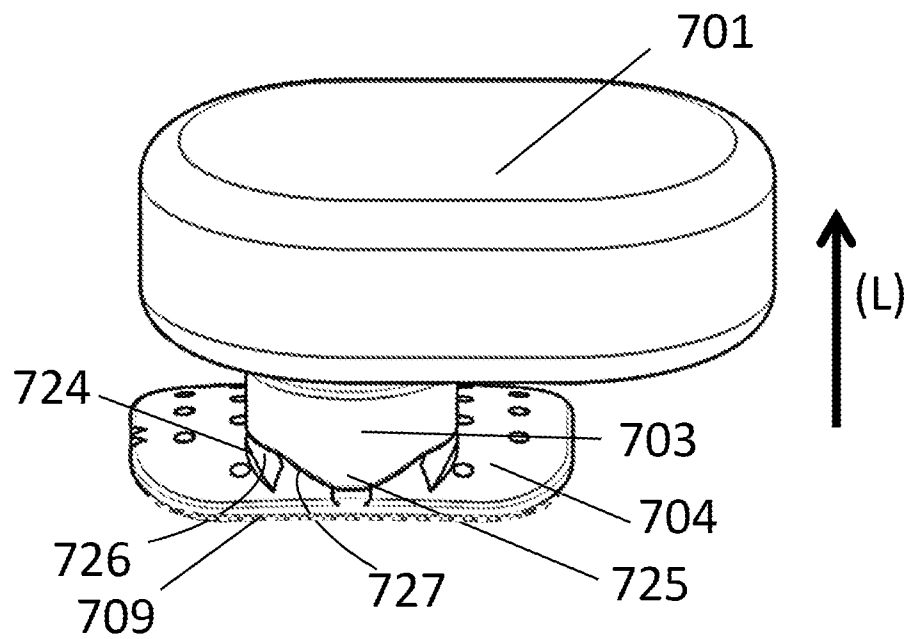


Fig 7B

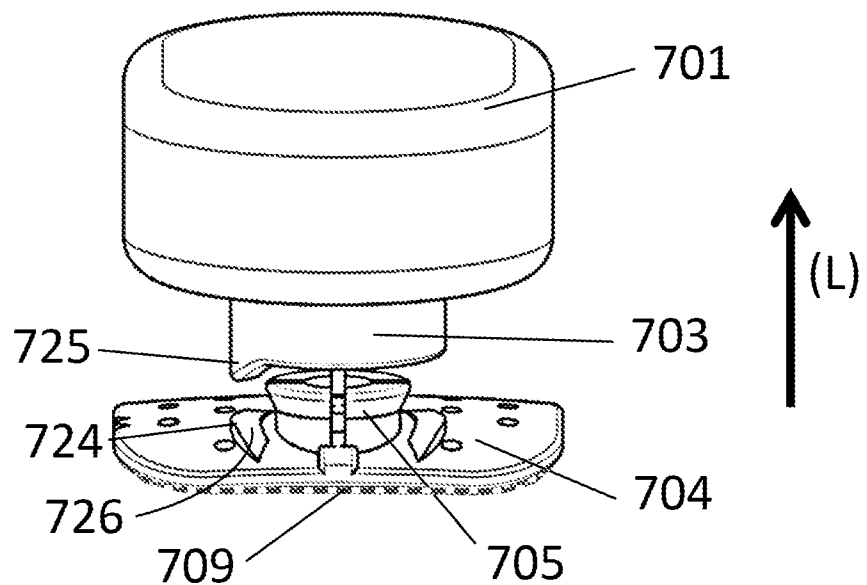

Figs 7A & 7B.

8/8

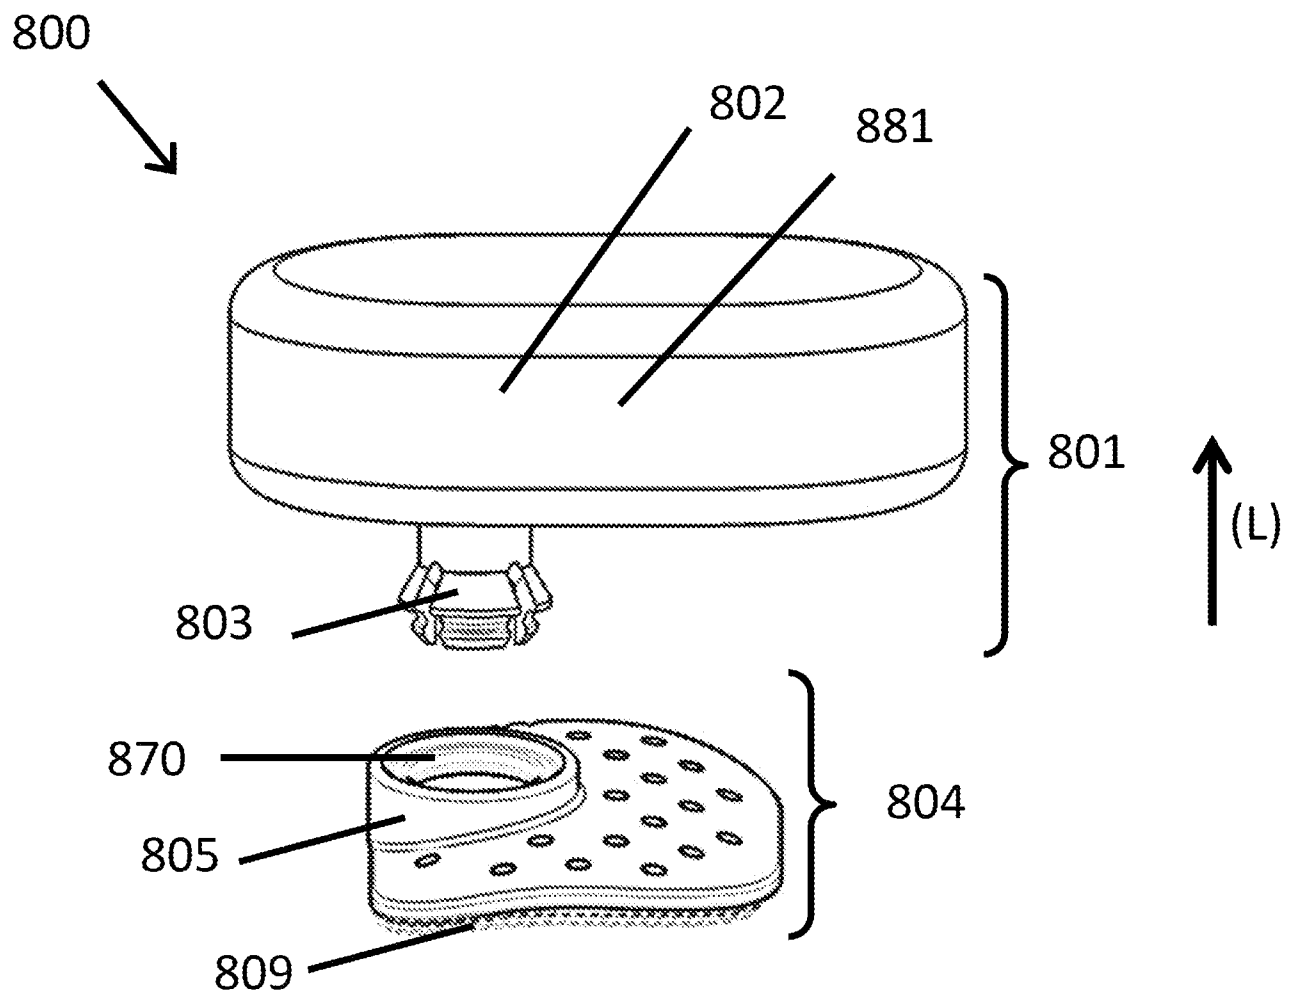


Fig 8.