



US00D938583S

(12) **United States Design Patent**
Yan et al.

(10) **Patent No.:** **US D938,583 S**

(45) **Date of Patent:** **** Dec. 14, 2021**

(54) **STENT DELIVERY DEVICE**

(71) Applicant: **Yipurun (Shanghai) Biotechnology Co., Ltd.**, Shanghai (CN)

(72) Inventors: **Wei Yan**, Shanghai (CN); **Peipei Xia**, Shanghai (CN); **Rui Yang**, Shanghai (CN); **Zheng Wei**, Shanghai (CN)

(73) Assignee: **Yipurun (Shanghai) Biotechnology Co., Ltd.**, Shanghai (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/701,459**

(22) Filed: **Aug. 12, 2019**

(30) **Foreign Application Priority Data**

Feb. 15, 2019 (CN) 201930065468.2

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**

USPC **D24/133**

(58) **Field of Classification Search**

USPC D24/133, 140, 146, 150, 155, 157, 113,
D24/127; D8/308, 315, 316, 318, 319,
D8/320

CPC A61F 9/0017; A61F 9/00781; A61F 9/008;
A61F 9/00709; A61F 9/00736; A61F 2/14

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,800,517 A * 9/1998 Anderson A61F 2/958
604/171
D402,030 S * 12/1998 Roberts D24/144
D402,031 S * 12/1998 Roberts D24/144
D439,336 S * 3/2001 Najmi D19/902
D463,555 S * 9/2002 Etter D24/143

D469,870 S * 2/2003 Niermann D24/112
D483,475 S * 12/2003 Kirwan D24/108
D490,152 S * 5/2004 Myall D24/133
D492,995 S * 7/2004 Rue D24/113
D496,730 S * 9/2004 Morawski A61B 17/3211
D24/133
D530,680 S * 10/2006 Fox D13/168
D535,026 S * 1/2007 Griffin A61B 17/3211
D24/146
D537,528 S * 2/2007 Christensen A61B 17/3211
D24/147
D568,475 S * 5/2008 Sandel D24/147
D571,010 S * 6/2008 Cote A61B 17/3211
D24/147
D586,916 S * 2/2009 Faulkner D24/146
D598,070 S * 8/2009 Sneddon D23/228
D612,051 S * 3/2010 Ruf D24/146

(Continued)

Primary Examiner — T Chase Nelson

Assistant Examiner — Kelly L Gross

(74) *Attorney, Agent, or Firm* — McCarter & English,
LLP; Jonathan C. Lovely

(57)

CLAIM

The ornamental design for a stent delivery device, as shown and described.

DESCRIPTION

FIG. 1 is a front side elevation view of a stent delivery device embodying my new design;

FIG. 2 is a rear side elevation view thereof;

FIG. 3 is a left side elevation view thereof;

FIG. 4 is a right side elevation view thereof;

FIG. 5 is a top plan view thereof;


FIG. 6 is a bottom plan view thereof;

FIG. 7 is a perspective view thereof; and,

FIG. 8 is another perspective view thereof.

The broken lines shown in the figures depict portions of the stent delivery device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

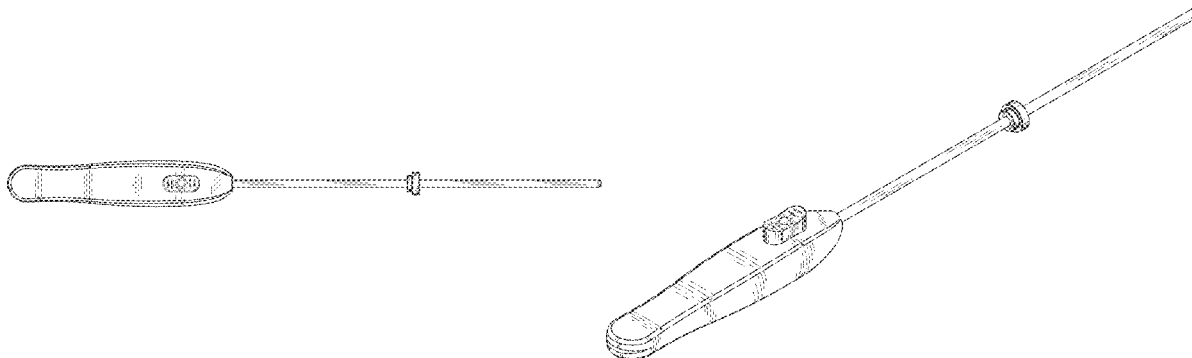

US D938,583 S

Page 2

(56)

References Cited

U.S. PATENT DOCUMENTS

D616,095 S *	5/2010	Kim	D24/140	D794,194 S *	8/2017	Schuerg	D24/144
D621,042 S *	8/2010	Ruf	D24/146	D794,790 S *	8/2017	Shi	D24/146
D628,293 S *	11/2010	Ruf	D24/146	D795,424 S *	8/2017	Sloss	D24/138
D628,695 S *	12/2010	Ruf	D24/146	9,717,627 B2 *	8/2017	Kuzma	A61F 9/0017
D634,843 S *	3/2011	Kim	D24/140	D799,040 S *	10/2017	Melnikoff	D24/152
D655,406 S *	3/2012	Ma	D24/112	D802,769 S *	11/2017	Robertson	D24/167
D665,909 S *	8/2012	Dodd	D24/146	D806,230 S *	12/2017	Johnson	A61B 17/3211
D677,380 S *	3/2013	Julian	D24/113				D24/112
D678,512 S *	3/2013	Bow	D24/112	D818,584 S *	5/2018	Lee	A61B 17/3211
D679,014 S *	3/2013	Jayaraj	D24/144				D24/133
D685,092 S *	6/2013	Morawski	A61B 17/3211	D828,548 S *	9/2018	Bow	D24/112
			D24/147	D834,702 S *	11/2018	Evans	D24/110
D703,707 S *	4/2014	Foster	D15/123	D837,975 S *	1/2019	Protasiewicz	D24/113
D719,255 S *	12/2014	Ohashi	D24/112	D838,360 S *	1/2019	Protasiewicz	D24/113
D719,651 S *	12/2014	Hoffmann	D24/133	D839,417 S *	1/2019	Funakoshi	D24/113
D736,923 S *	8/2015	Snow	D24/146	D841,164 S *	2/2019	Flowers	D24/150
D737,440 S *	8/2015	Shabaz	D24/146	D844,784 S *	4/2019	Swick	D24/147
D739,020 S *	9/2015	Kumar	D24/147	D846,738 S *	4/2019	Kalina, Jr	D24/133
D740,422 S *	10/2015	Herfort	D24/147	D847,334 S *	4/2019	Amano	D24/133
D740,630 S *	10/2015	Hasenmayer	D8/30	10,278,720 B2 *	5/2019	Marczyk	A61B 17/295
D741,483 S *	10/2015	Solingen	D24/146	D851,755 S *	6/2019	Nazzaro	D24/114
9,173,771 B2 *	11/2015	Keller	A61B 18/08	D855,181 S *	7/2019	Khan	D24/150
D744,638 S *	12/2015	Bow	D24/112	D861,864 S *	10/2019	Amano	D24/133
D749,717 S *	2/2016	Kobida	D24/108	D879,960 S *	3/2020	Melnikoff	D24/152
D753,301 S *	4/2016	Fiksen	D24/144	10,780,218 B2 *	9/2020	Novakovic	A61M 5/158
D755,383 S *	5/2016	Pfister	D24/144	D901,683 S *	11/2020	Kalina, Jr	D24/133
D759,246 S *	6/2016	Allen	D24/146	D903,100 S *	11/2020	Stats	D24/112
D765,841 S *	9/2016	Schuerg	D24/144	D910,836 S *	2/2021	Sandberg	A61F 2/966
D765,842 S *	9/2016	Schuerg	D24/144				D24/112
D766,432 S *	9/2016	Schuerg	D24/144	D911,521 S *	2/2021	Swift	D24/135
D767,760 S *	9/2016	Suwito	D24/141	D929,580 S *	8/2021	Bornhoft	D24/130
D770,044 S *	10/2016	Fiksen	D24/144	D929,586 S *	8/2021	Williams	D24/140
D770,618 S *	11/2016	Fiksen	D24/144	2011/0295354 A1 *	12/2011	Bueche	A61F 2/962
9,554,940 B2 *	1/2017	Haffner	A61F 2/14				623/1.11
D779,053 S *	2/2017	Kobida	D24/108	2012/0123516 A1 *	5/2012	Gerdt	A61F 2/966
D780,306 S *	2/2017	Bow	D24/112				623/1.12
9,592,151 B2 *	3/2017	Rangel-Friedman	A61F 9/00781	2014/0277564 A1 *	9/2014	Windheuser	A61M 25/01
			A61F 9/00781				623/23.7
D789,453 S *	6/2017	Walker	D19/180	2015/0081008 A1 *	3/2015	Sheldon	D06C 7/00
D791,318 S *	7/2017	Jutila	D24/141				623/1.12
D794,192 S *	8/2017	Schuerg	D24/144	2015/0297379 A1 *	10/2015	Green	A61F 2/95
D794,193 S *	8/2017	Schuerg	D24/144				623/1.12
				2015/0335452 A1 *	11/2015	Rao	A61F 2/95
							623/23.66

* cited by examiner




FIG. 1




FIG. 2




FIG.3




FIG.4




FIG.5




FIG.6

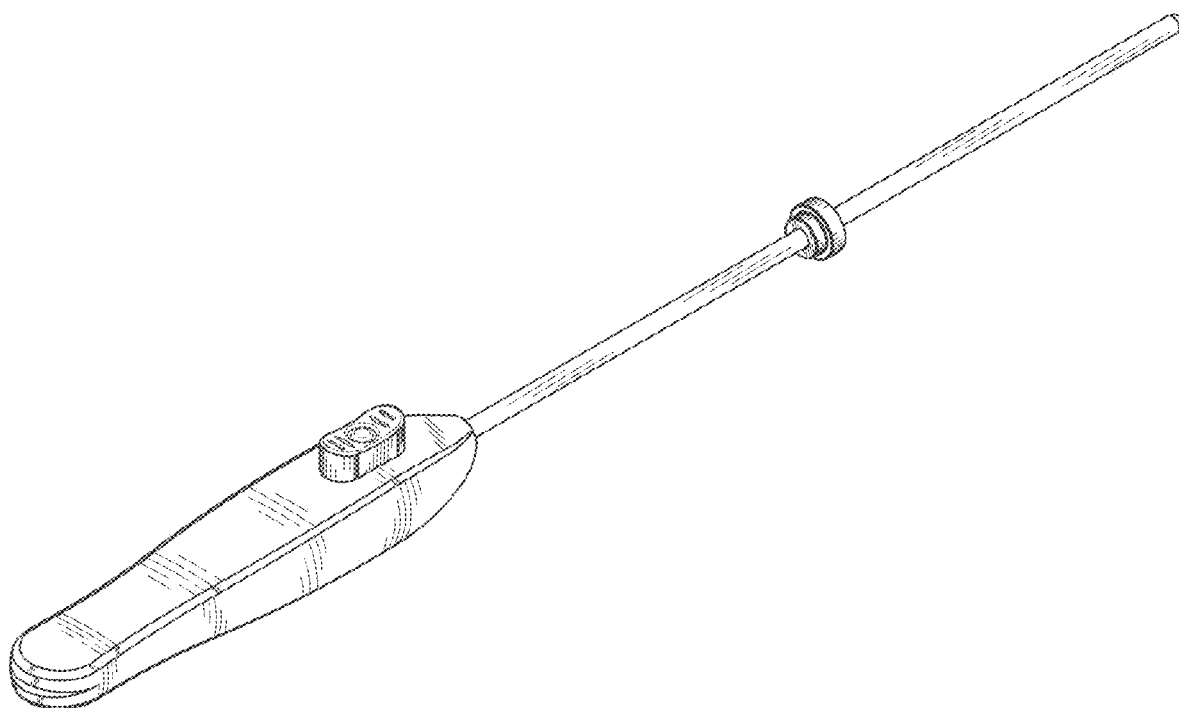


FIG.7

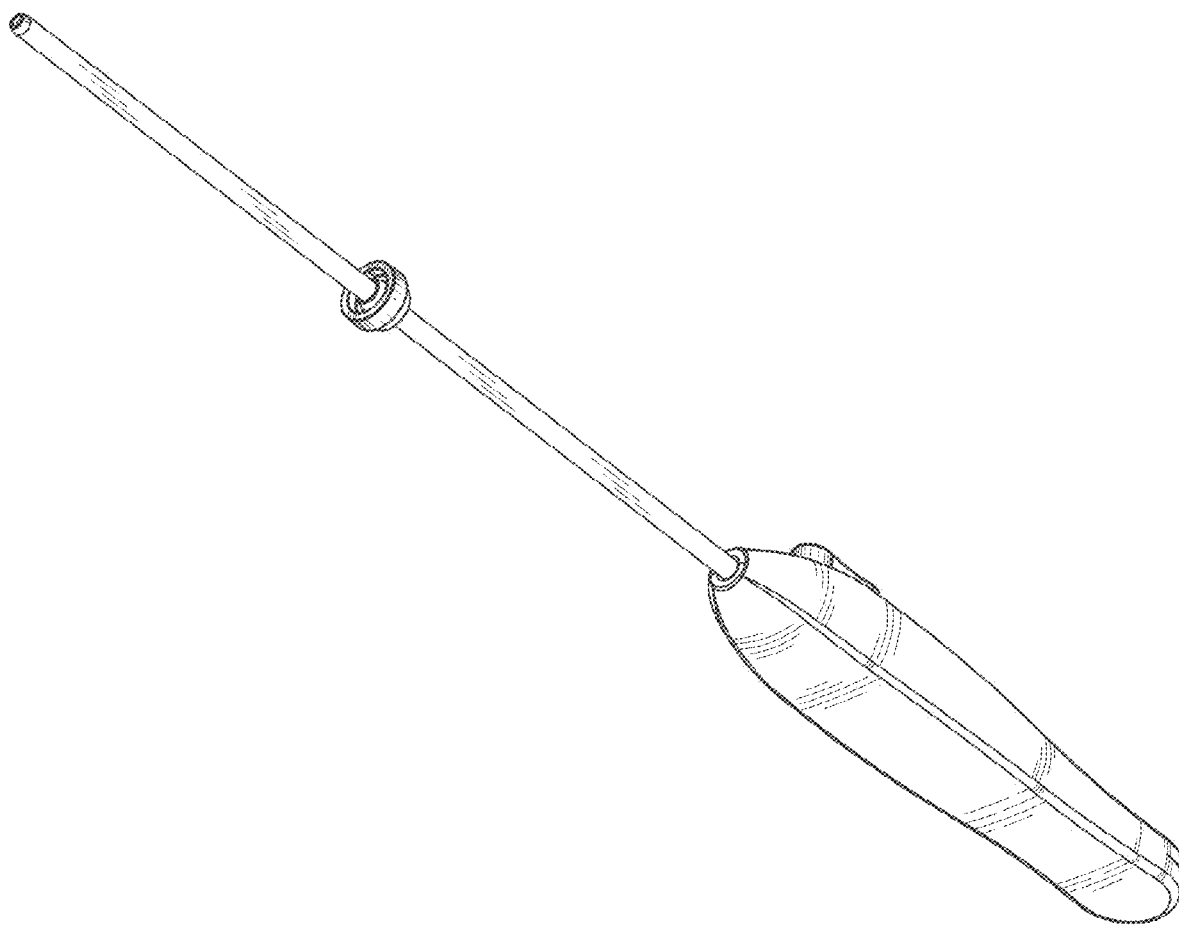


FIG.8