



US 20060122589A1


(19) **United States**(12) **Patent Application Publication****Abboud et al.**(10) **Pub. No.: US 2006/0122589 A1**(43) **Pub. Date:****Jun. 8, 2006**(54) **METHOD AND APPARATUS FOR
INFLATING AND DEFLATING BALLOON
CATHETERS**(52) **U.S. Cl.** 606/21; 606/41(75) **Inventors:** **Marwan Abboud**, Pierrefonds (CA);
Rachid Mahrouche, Anjou (CA);
Teresa Mihalik, Montreal (CA); **Chadi
Harmouche**, St-Laurent (CA); **Eric
Monger**, Ste-Genevieve (CA)(57) **ABSTRACT**


A system and method for controlling the inflation, ablation, and deflation of a balloon catheter. The system includes a balloon catheter, a console, having a pressurized gas or liquid inflation source, and an umbilical system to deliver pressurized coolant to the balloon catheter. The system comprises a PID (Proportional Integral Derivative) controller or other pressure-sensing device that monitors the amount of pressure and volume within the balloon catheter. During inflation, the pressure and/or volume of fluid within the balloon is maintained at a target amount in order to provide sufficient mechanized pressure against the desired target region. The system limits the inflation pressure such that a safe quantity of gas would be released should a leak occur. If the amount falls below a certain threshold level, gas or fluid egress is presumed and the inflation process is halted. In one embodiment, an intermediate console is placed between the console and the balloon catheter and coupled thereto. If a leak is detected, a shut off valve in the intermediate station is activated and the flow of pressurized coolant is interrupted. The balloon catheter can be re-inflated by a separate coolant source in the intermediate station or by a syringe. A further embodiment provides a second balloon to envelope the first balloon and in order to provide a safety vacuum between the two balloons.

Correspondence Address:

Christopher & Weisberg, P.A.**Suite 2040****200 East Las Olas Boulevard****Fort Lauderdale, FL 33301 (US)**(73) **Assignee:** **CryoCath Technologies Inc.**(21) **Appl. No.:** **11/301,768**(22) **Filed:** **Dec. 13, 2005****Related U.S. Application Data**

(62) Division of application No. 10/806,995, filed on Mar. 23, 2004.

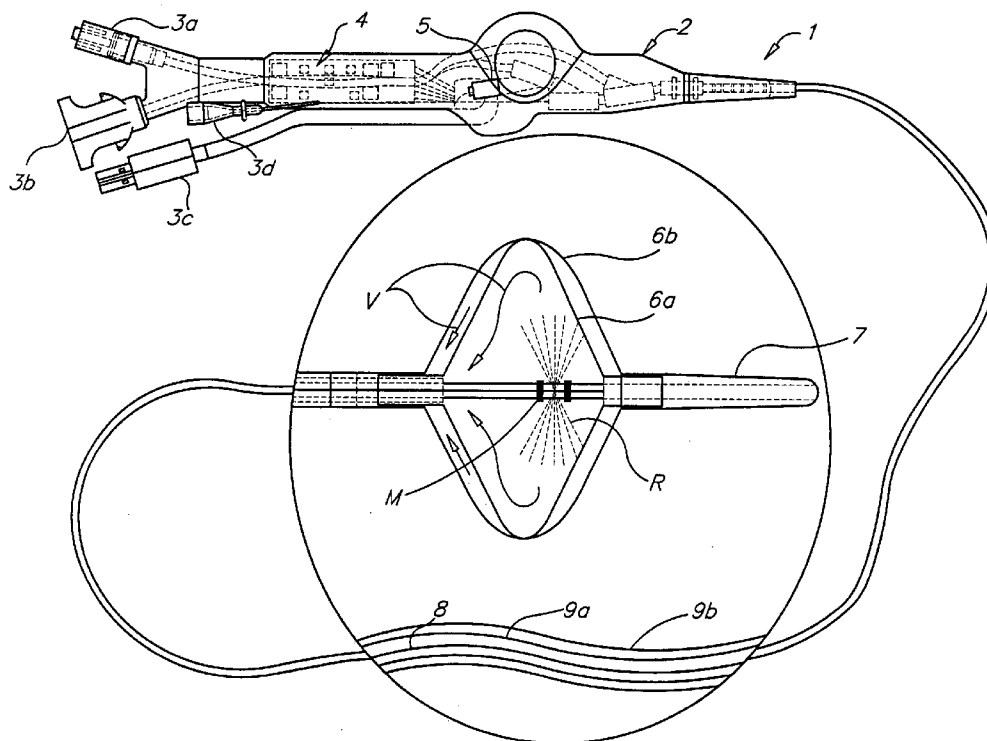Publication Classification(51) **Int. Cl.****A61B 18/02** (2006.01)**A61B 18/18** (2006.01)

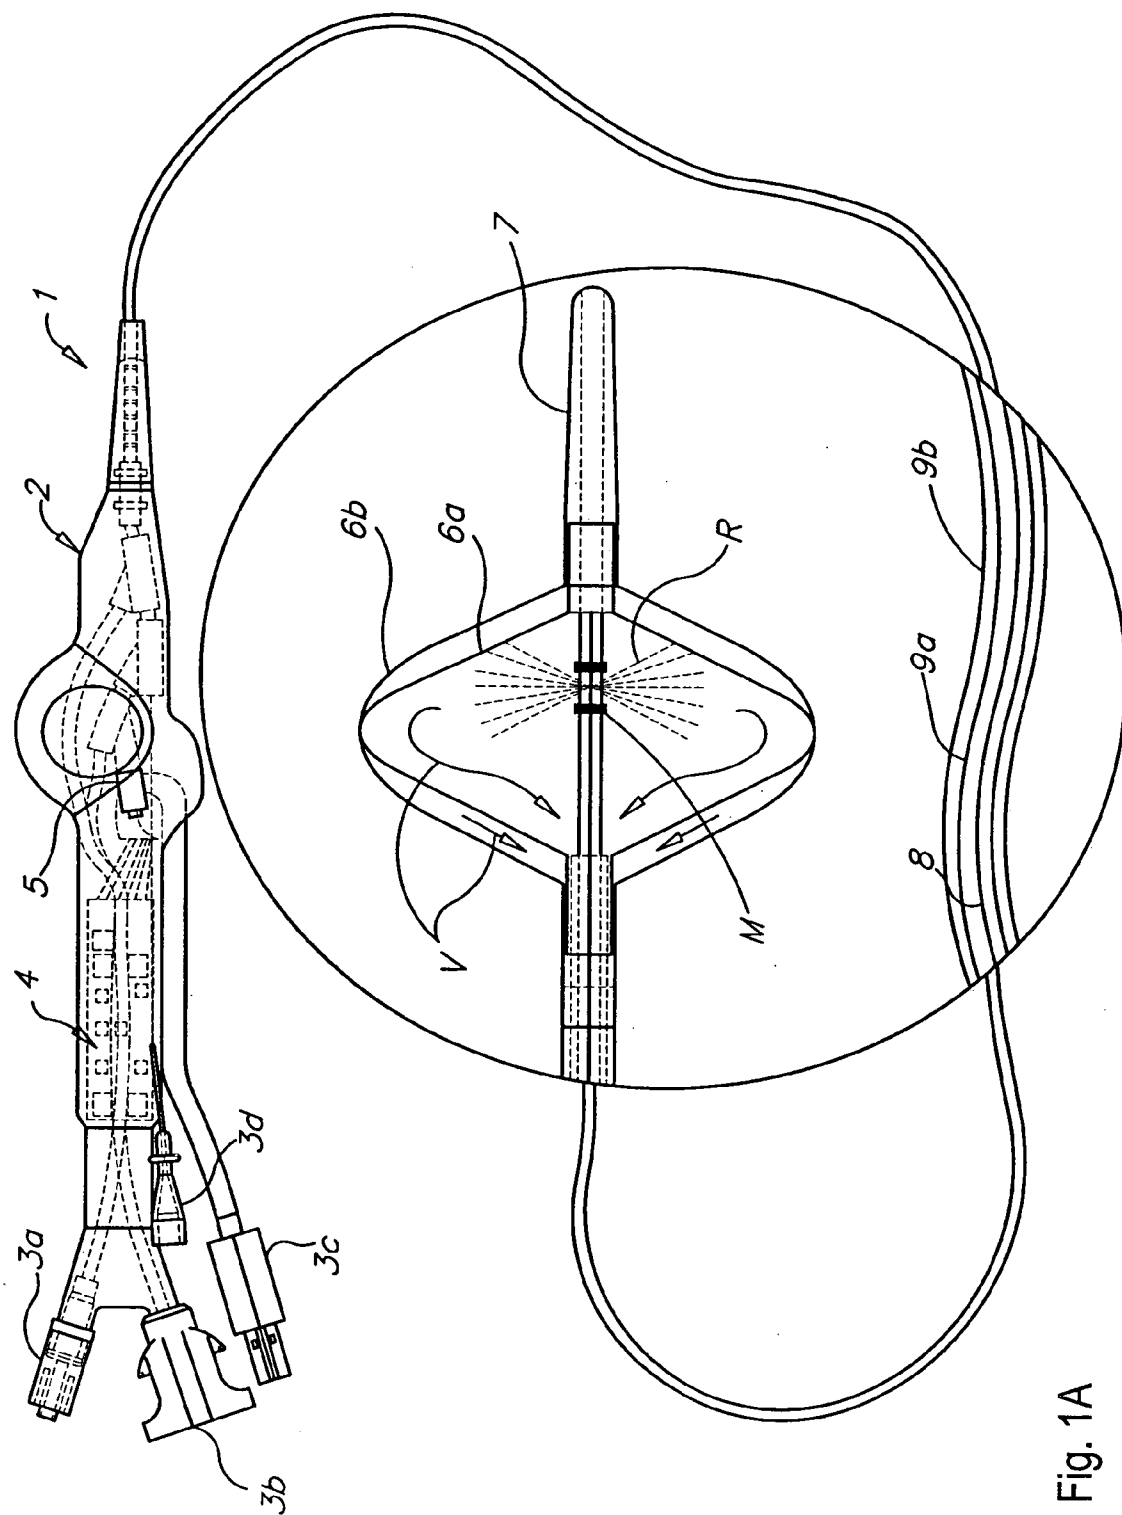

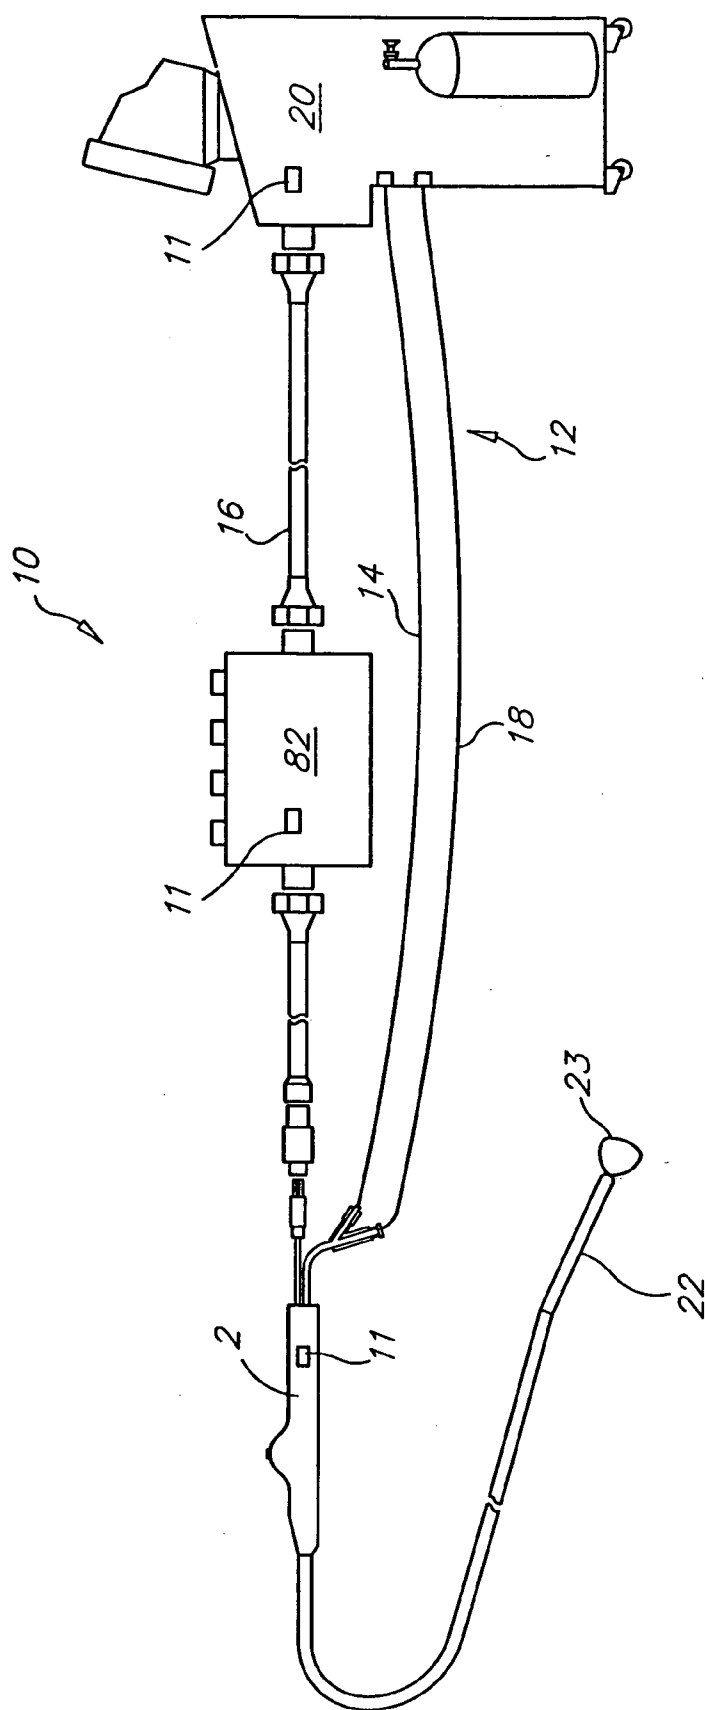


Fig. 1B

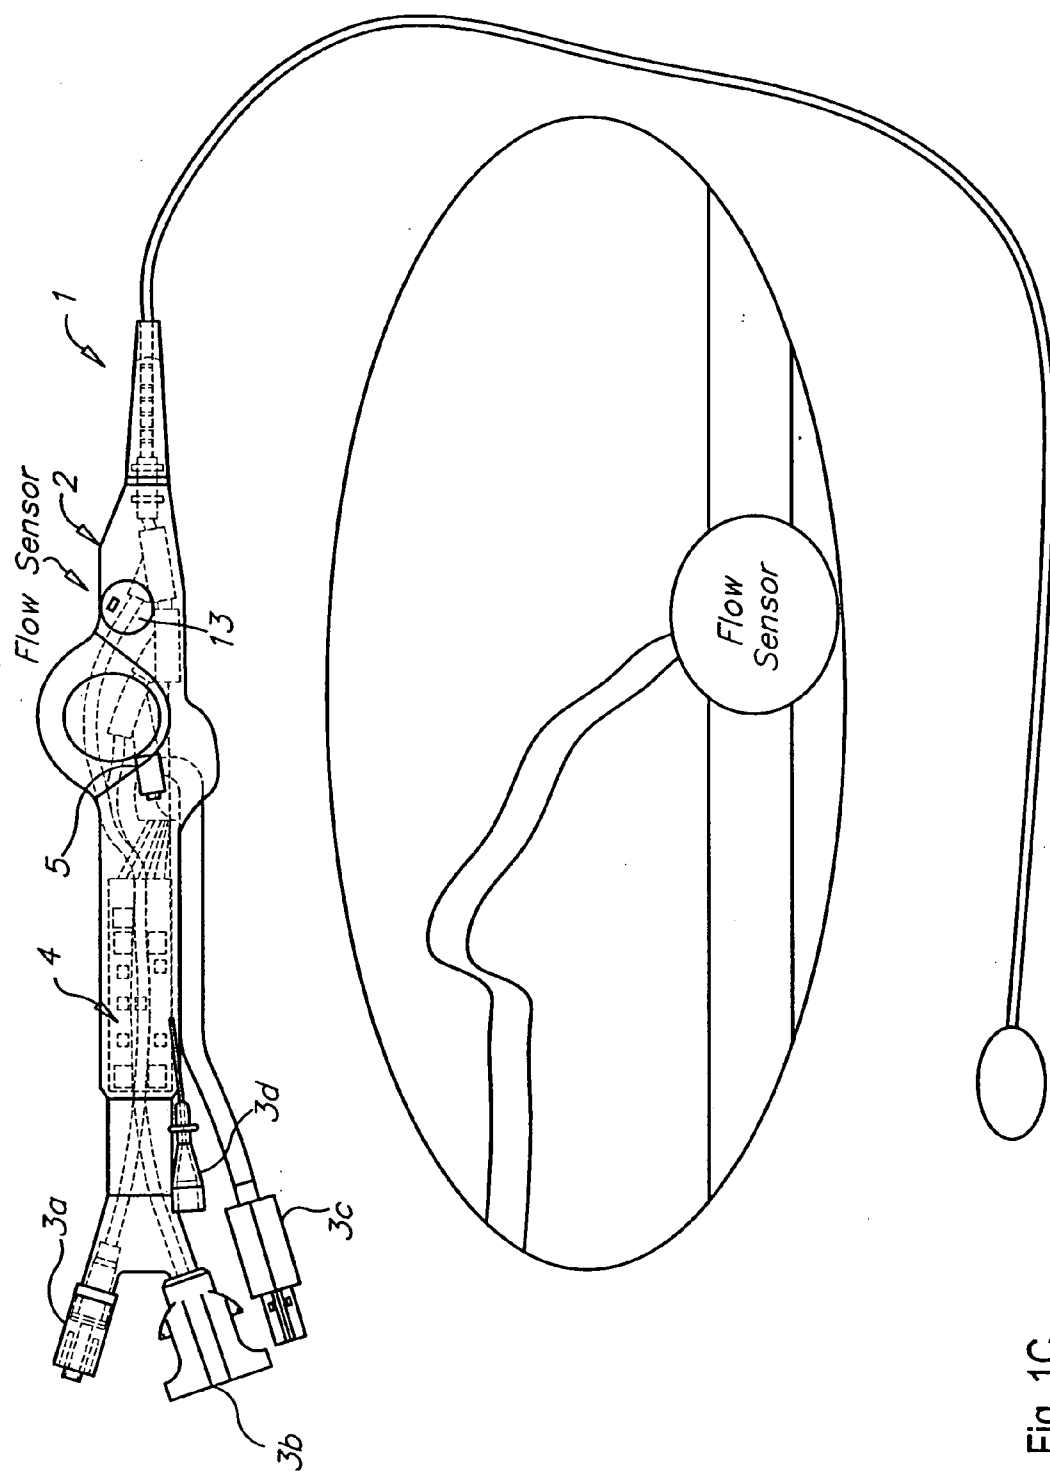
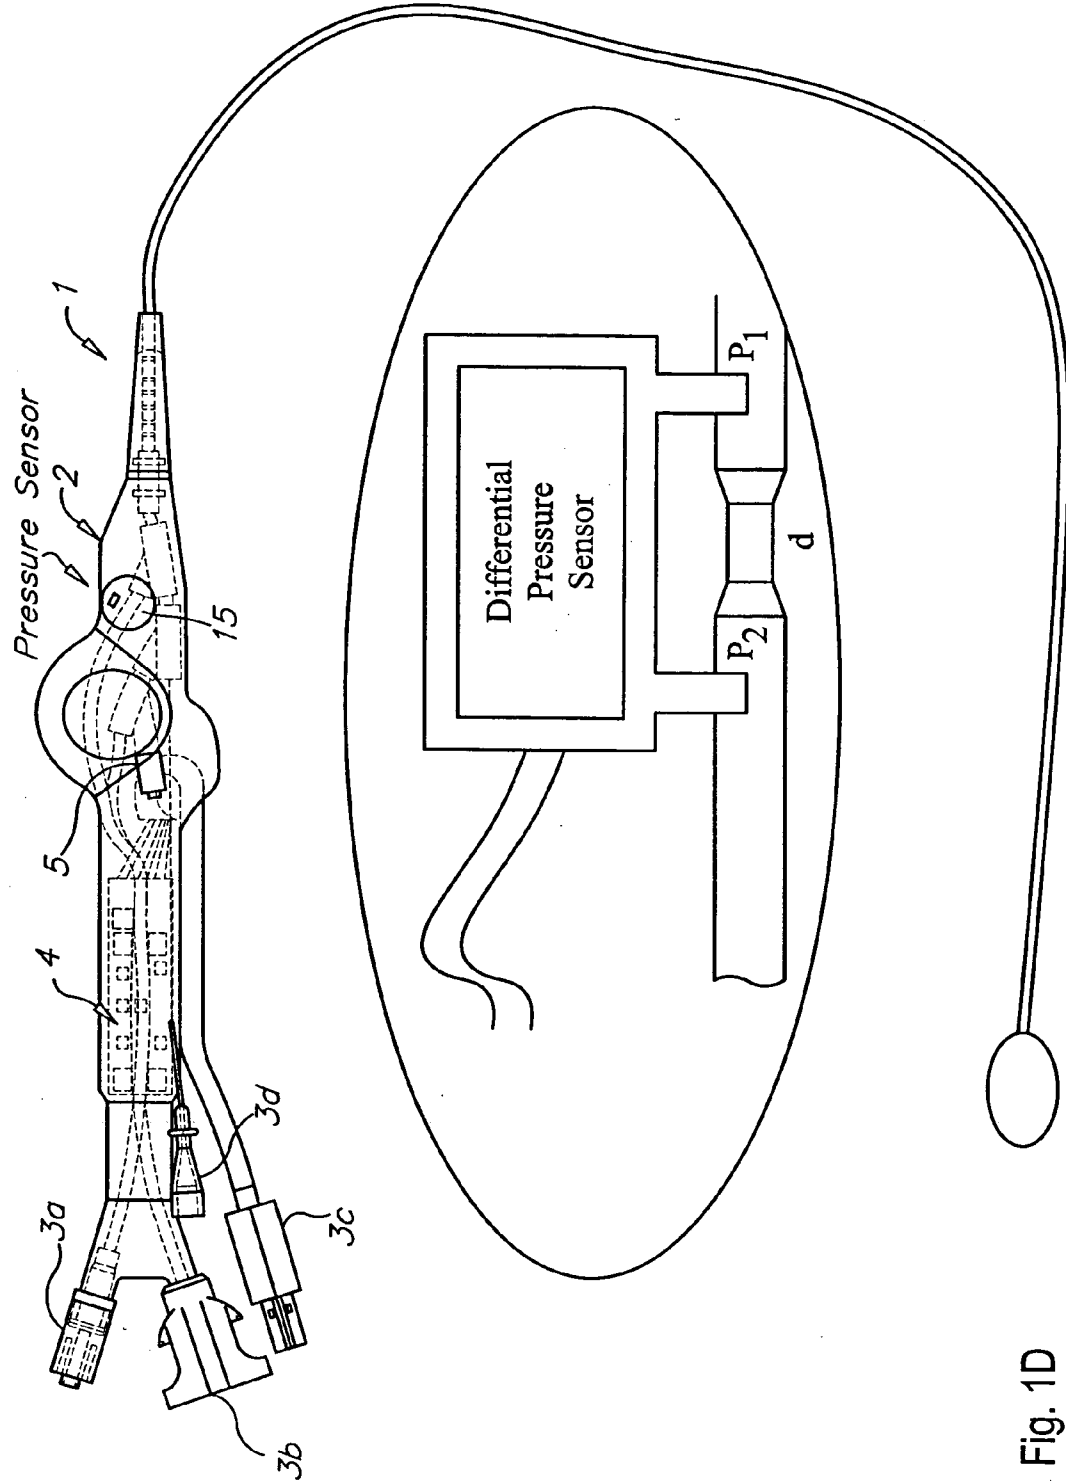
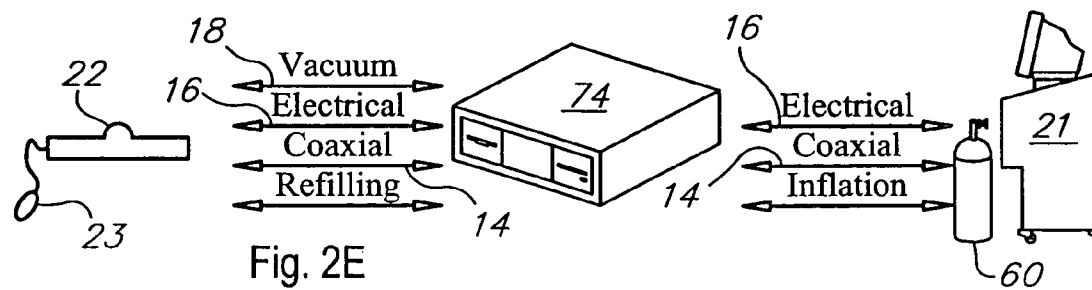
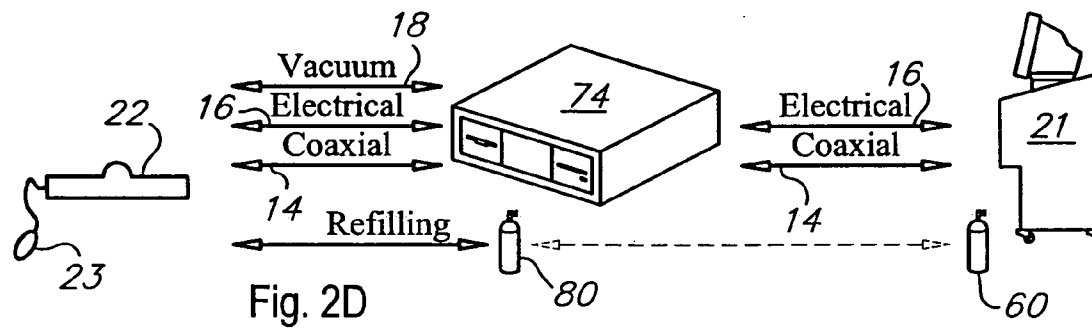
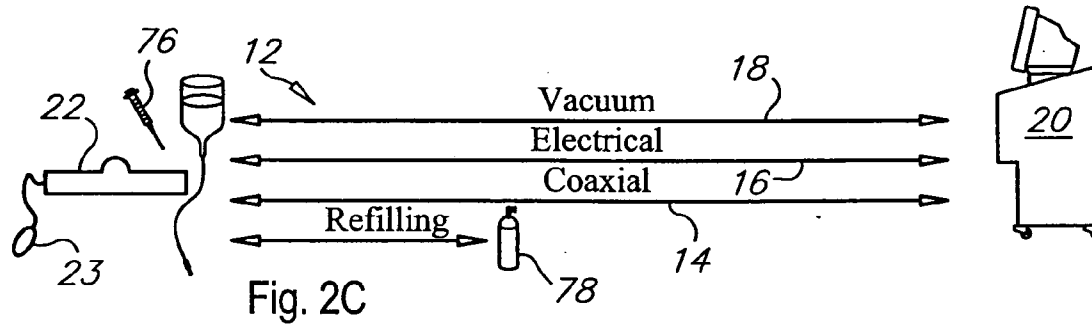
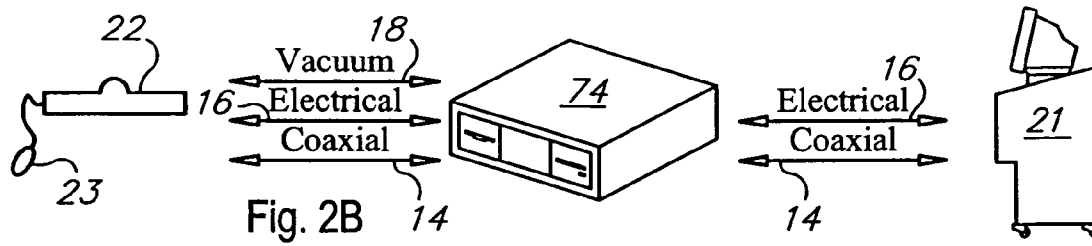
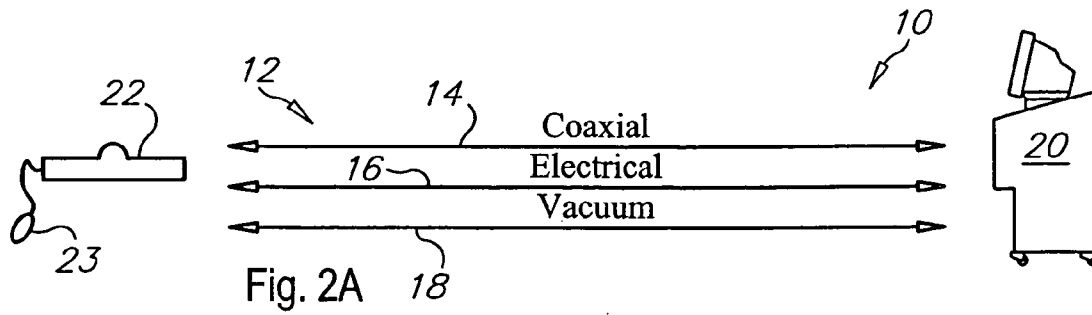


Fig. 1C





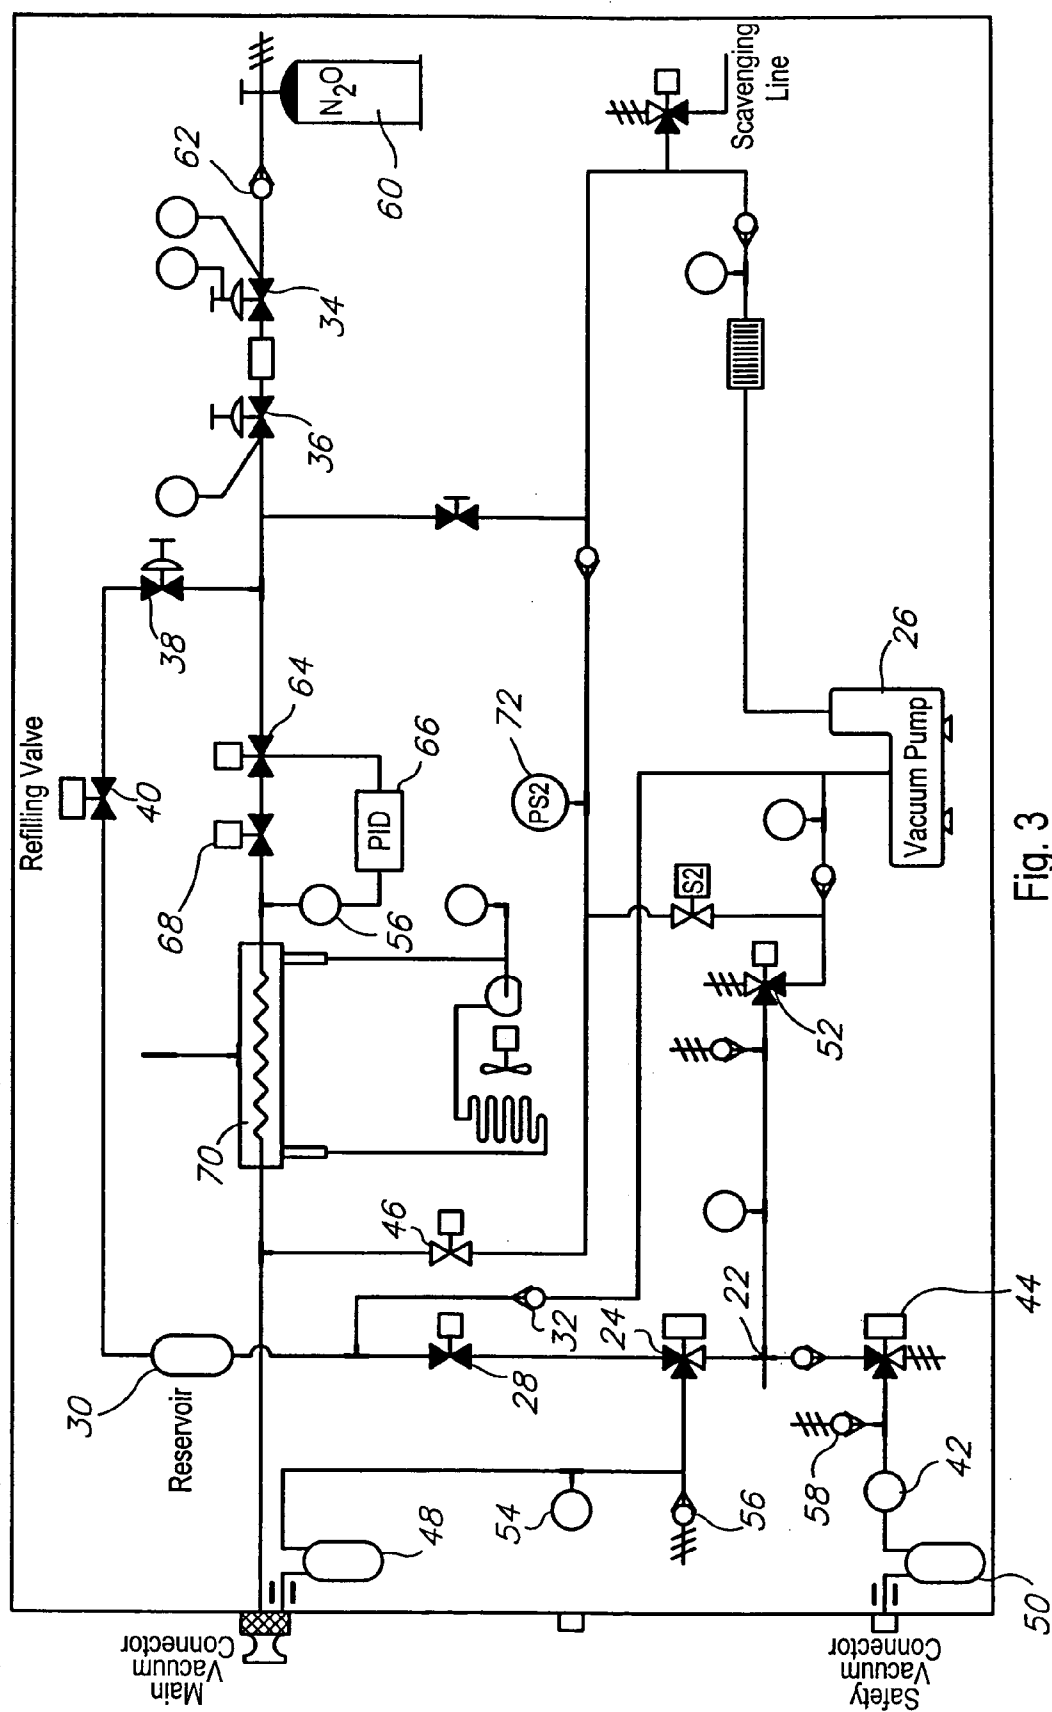


Fig. 3

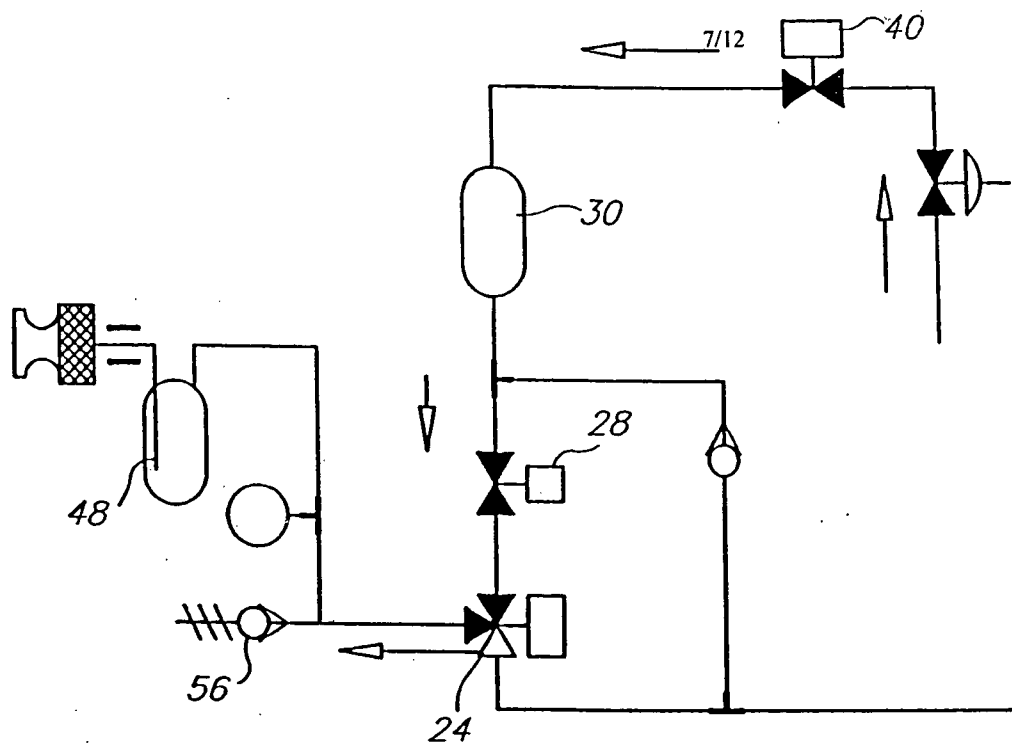


Fig. 4

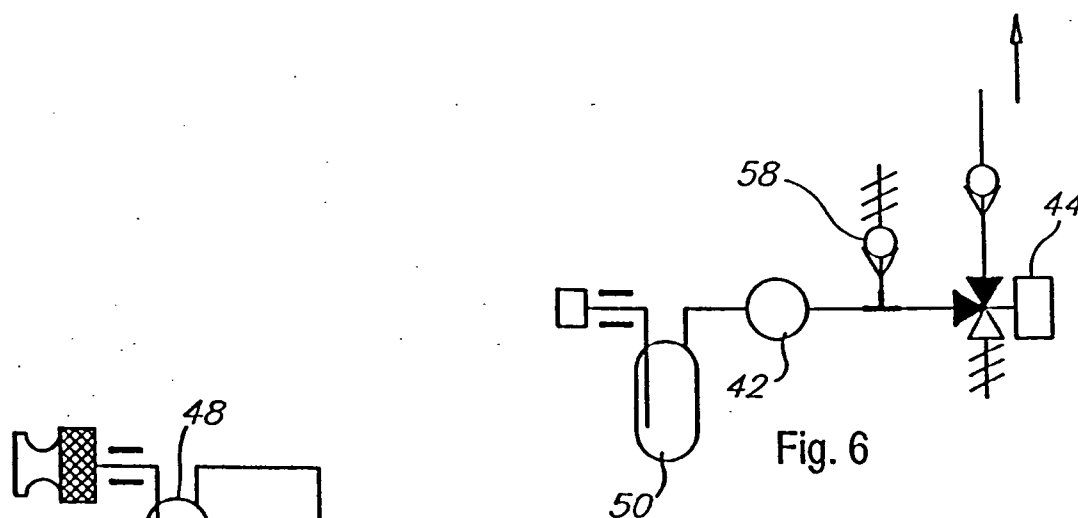


Fig. 6

Fig. 5

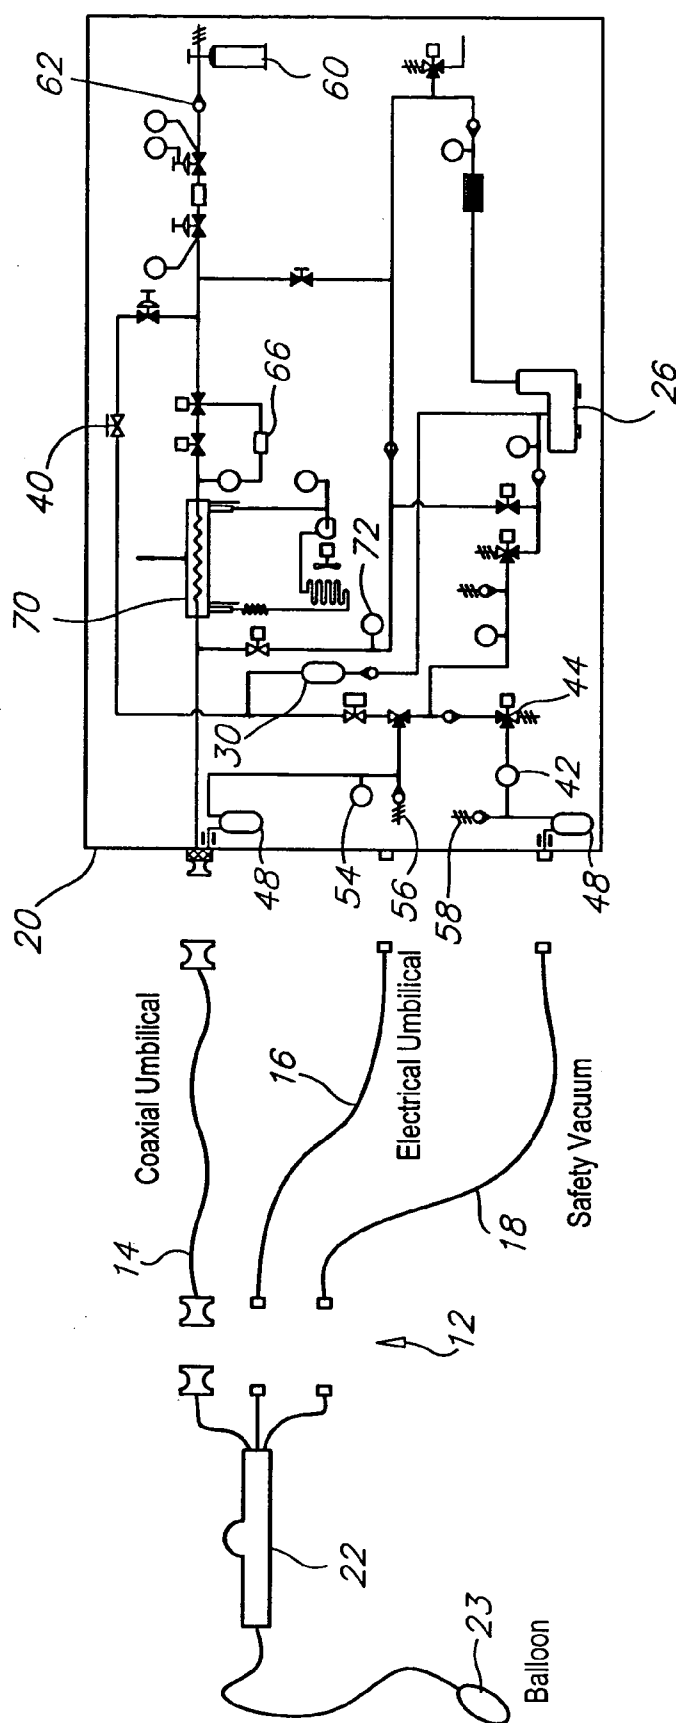


Fig. 7

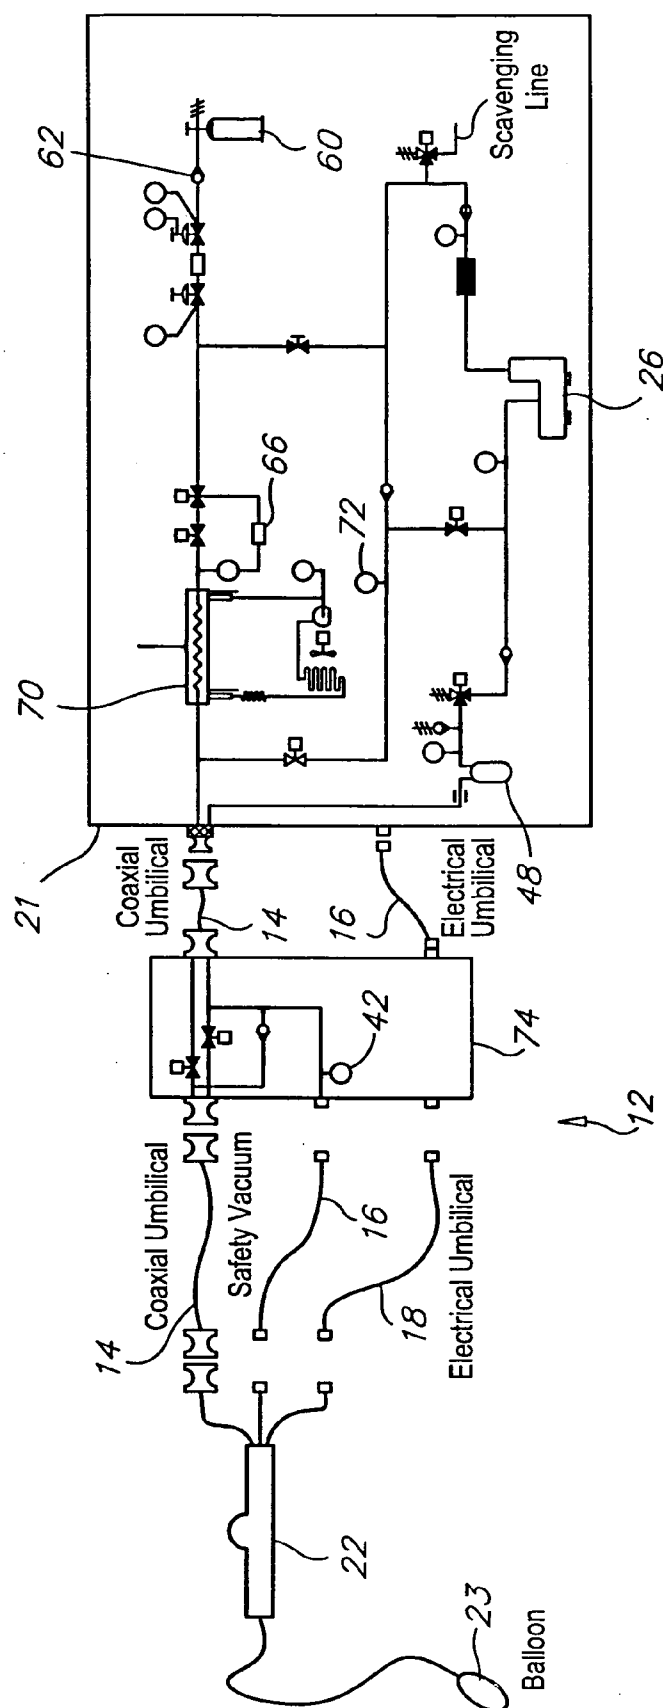


Fig. 8

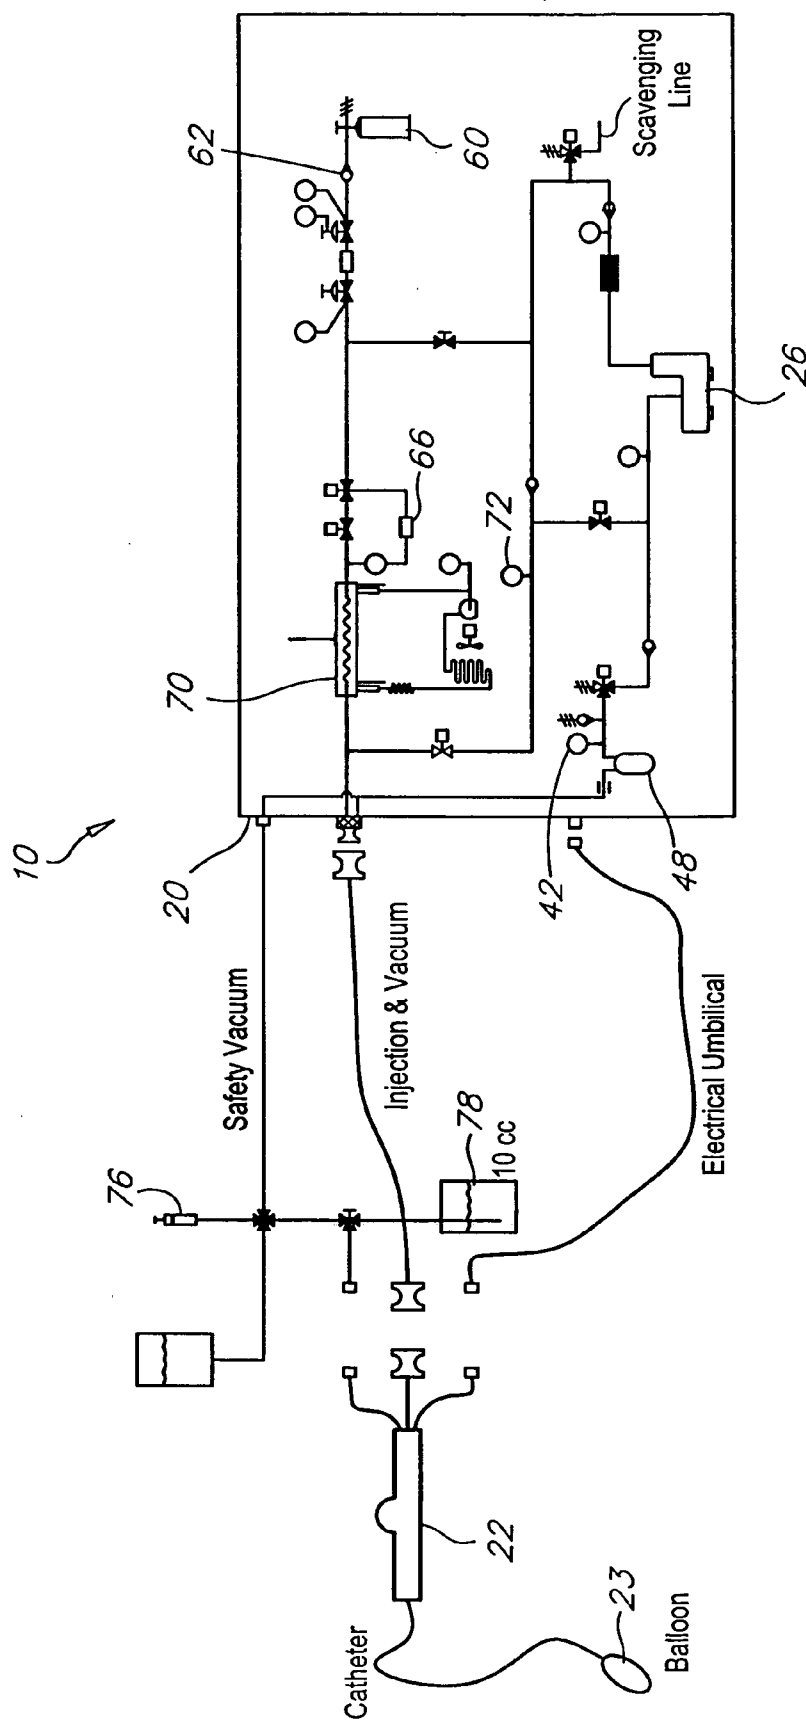


Fig. 9

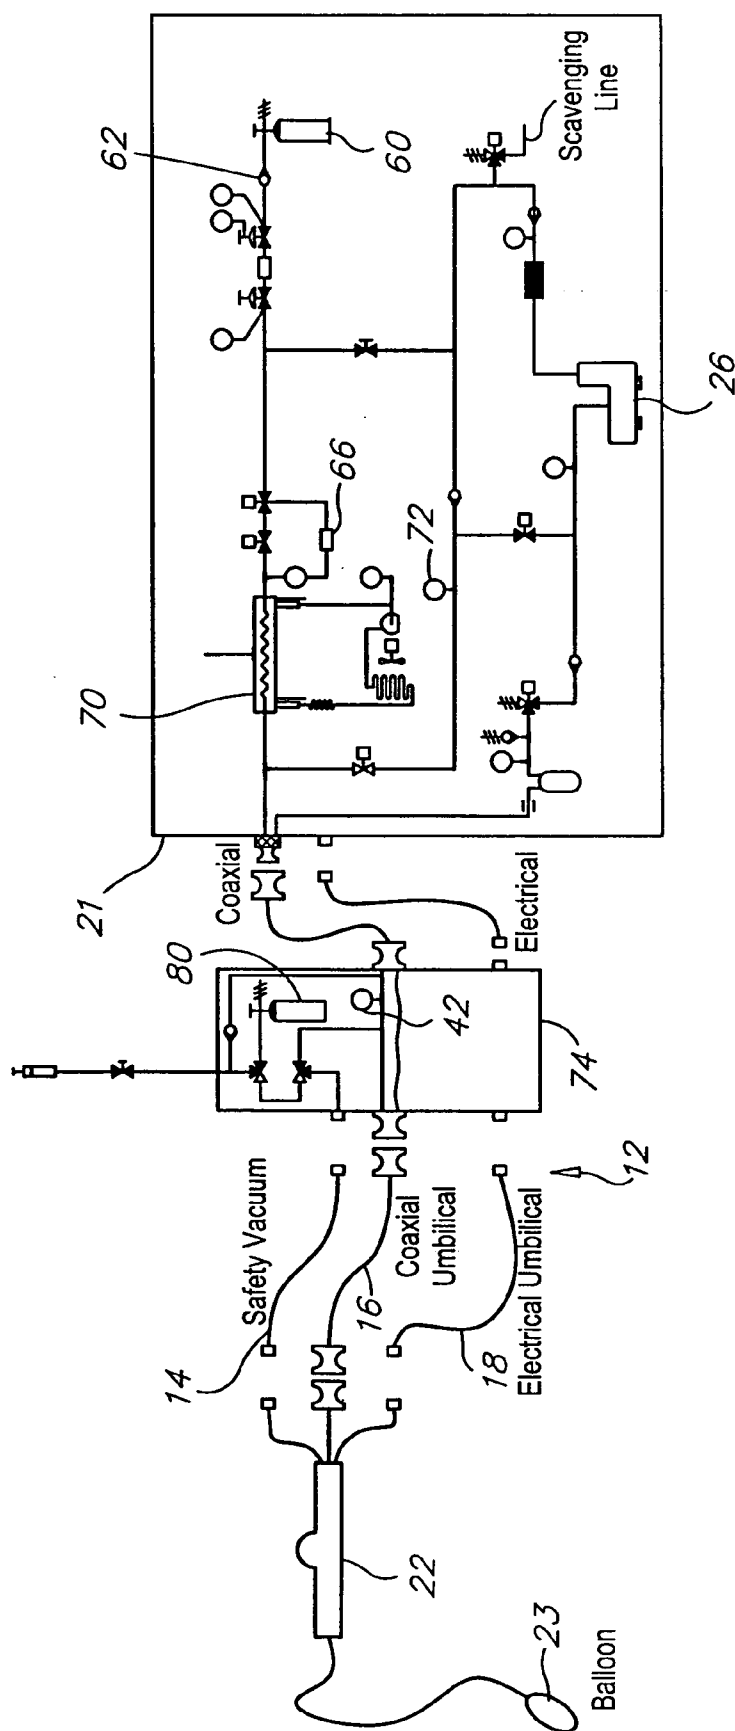


Fig. 10

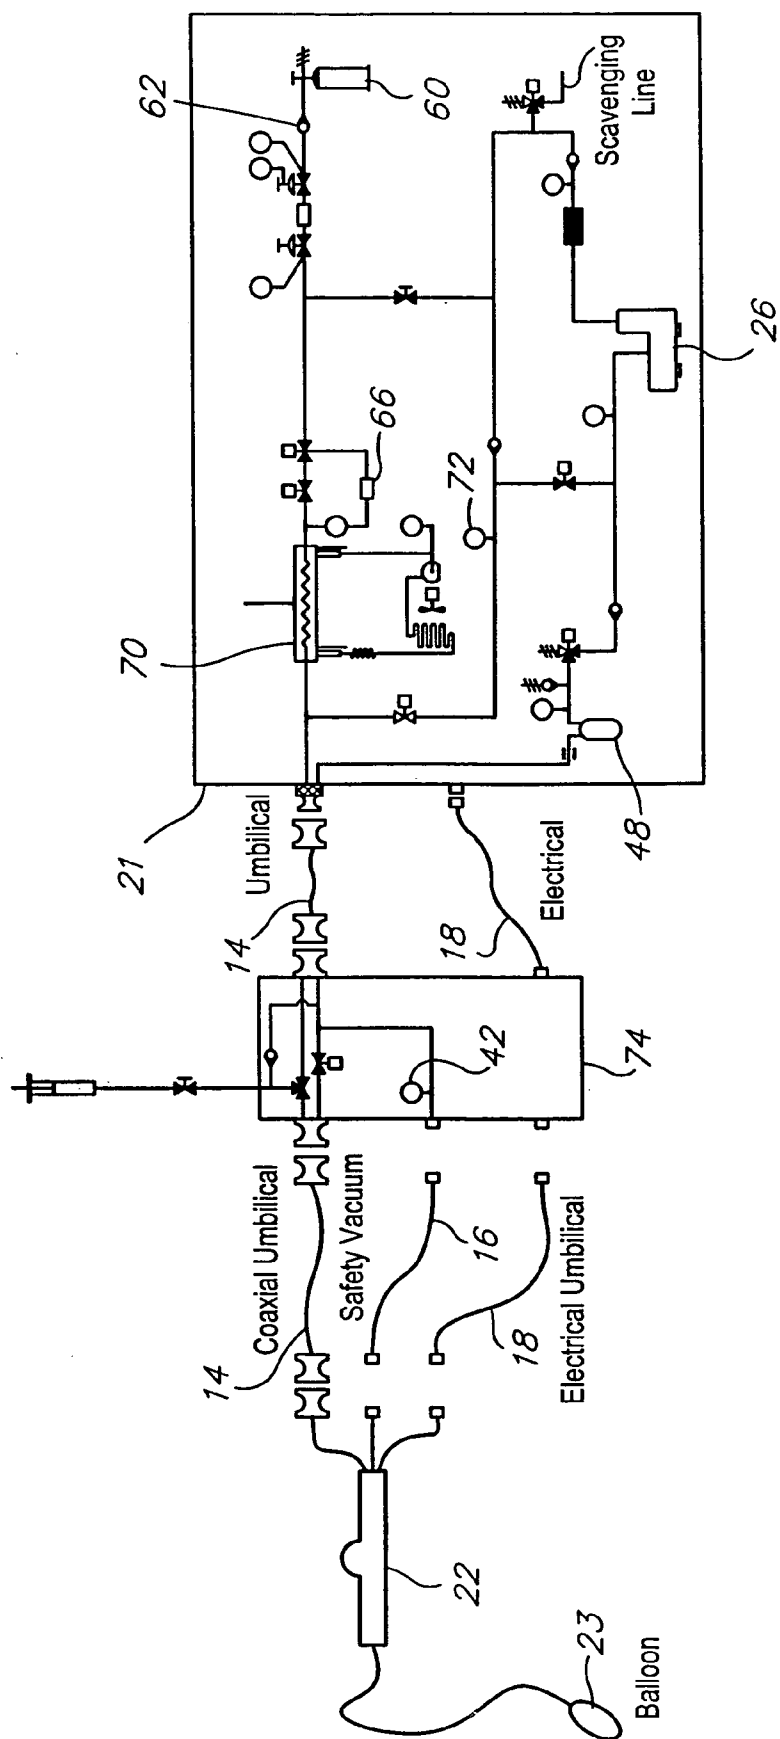


Fig. 11

METHOD AND APPARATUS FOR INFLATING AND DEFLATING BALLOON CATHETERS

CROSS-REFERENCE TO RELATED APPLICATION

[0001] n/a

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

[0002] n/a

FIELD OF THE INVENTION

[0003] The present invention relates to a method and system for inflating and deflating balloon catheters and more specifically to a method and system for controlling the inflation and deflation of balloon catheters in order to safely and effectively ablate a tissue region.

BACKGROUND OF THE INVENTION

[0004] The use of fluids with low operating temperatures, or cryogens, has begun to be explored in the medical and surgical field. Of particular interest are the potential use of catheter based devices, which employ the flow of cryogenic working fluids therein, to selectively freeze, or "cold-treat", targeted tissues within the body. Catheter based devices are desirable for various medical and surgical applications in that they are relatively non-invasive and allow for precise treatment of localized discrete tissues that are otherwise inaccessible. Catheters may be easily inserted and navigated through the blood vessels and arteries, allowing non-invasive access to areas of the body with relatively little trauma.

[0005] Catheter-based ablation systems are well known in the art. A cryogenic device uses the energy transfer derived from thermodynamic changes occurring in the flow of a cryogen therethrough to create a net transfer of heat flow from the target tissue to the device, typically achieved by cooling a portion of the device to very low temperature through conductive and convective heat transfer between the cryogen and target tissue. The quality and magnitude of heat transfer is regulated by the device configuration and control of the cryogen flow regime within the device.

[0006] A cryogenic device uses the energy transfer derived from thermodynamic changes occurring in the flow of a refrigerant through the device. This energy transfer is then utilized to create a net transfer of heat flow from the target tissue to the device, typically achieved by cooling a portion of the device to very low temperature through conductive and convective heat transfer between the refrigerant and target tissue. The quality and magnitude of heat transfer is regulated by device configuration and control of the refrigerant flow regime within the device.

[0007] Structurally, cooling can be achieved through injection of high pressure refrigerant through an orifice. Upon injection from the orifice, the refrigerant undergoes two primary thermodynamic changes: (i) expanding to low pressure and temperature through positive Joule-Thomson throttling, and (ii) undergoing a phase change from liquid to vapor, thereby absorbing heat of vaporization. The resultant flow of low temperature refrigerant through the device acts to absorb heat from the target tissue and thereby cool the tissue to the desired temperature.

[0008] Once refrigerant is injected through an orifice, it may be expanded inside of a closed expansion chamber, which is positioned proximal to the target tissue. Devices with an expandable membrane, such as a balloon, are employed as expansion chambers. In such a device, refrigerant is supplied through a catheter tube into an expandable balloon coupled to such catheter, wherein the refrigerant acts to both: (i) expand the balloon near the target tissue for the purpose of positioning the balloon, and (ii) cool the target tissue proximal to the balloon to cold-treat adjacent tissue.

[0009] One of the principal drawbacks to such a technique is that during the inflation phase coolant may seep out of the balloon and get into the bloodstream to cause significant harm. Therefore, if the balloon develops a crack, leak, rupture, or other critical structural integrity failure, coolant may quickly flow out of the catheter. Another situation that may occur during the balloon deflation phase is that the balloon may adhere to the ablated tissue causing severe damage. This may occur after cryoablation or cryomapping. Cryomapping is a procedure that chills conducting target tissue to create a transient electrical effect. By temporarily chilling the target tissue, it allows for precise site confirmation in order to prevent inadvertent ablation. During cryomapping, a procedure known as cryoadhesion takes place. Cryoadhesion is a procedure that ensures the catheter tip remains at the target cite for a seamless transition to cryoablation. In a cryoadhesion procedure, the tip of the catheter firmly attaches to the tissue when it freezes thereby reducing the risk of accidental slippage of the catheter tip. Therefore, during unmonitored balloon deflation, i.e. if the balloon deflates too quickly, the balloon, adhering to the tissue walls, may cause severe damage.

[0010] Accordingly, it would be desirable to provide an apparatus and method of monitoring and controlling the inflation and deflation phases of a balloon catheter that is adaptable and compatible with all types of balloon ablation catheters, and with all types of ablation procedures, for example RF ablation or cryoablation.

SUMMARY OF THE INVENTION

[0011] The present invention advantageously provides a method and system for controllably inflating and deflating a balloon catheter. The method and system allows for the monitoring of the inflation and deflation phases of a catheter system in order to allow ablation to take place, while detecting unwanted leaks of refrigerant into the bloodstream. Balloon leaks are identified, safety evacuation routes are provided, and a controlled deflation mechanism is presented that prevents damage to the interior blood vessel and tissue region, which may occur during unmonitored deflation due to the adherenace of the expandable membrane to the interior of the vessel.

[0012] In its preferred embodiment, a method of inflating and deflating a catheter during an ablation process, the catheter having an expandable membrane, is provided. The method comprises the steps of controllably inflating the expandable membrane to a target pressure or volume, ablating a desired tissue region while maintaining the target pressure or volume of the expandable membrane, and controllably deflating the expandable membrane so as not to damage desired tissue region.

[0013] In another aspect of the invention, a method for inflating and deflating a catheter having an expandable

membrane during an ablation process is provided. The catheter is part of a catheter system including a console, the catheter, and an umbilical system coupling the console to the catheter. The method comprises the steps of evacuating air from the expandable membrane by creating a vacuum in the expandable membrane, controllably inflating the expandable membrane proximate a desired tissue region, wherein the expandable membrane is inflated to a target pressure or volume in order to provide sufficient mechanical force against the desired tissue region, ablating the desired tissue region while maintaining the expandable membrane at the target pressure or volume, and controllably deflating the expandable membrane such that the desired tissue region is not damaged.

[0014] In still another aspect of the invention, an apparatus for inflating and deflating a catheter having an expandable membrane is provided. The apparatus comprises a console, the console including means for controlling the inflation and deflation of the expandable membrane and for determining if the expandable membrane maintains a target pressure or volume. The console also includes a pressurized inflation source. The apparatus further includes a catheter, and an umbilical system coupling the console to the expandable membrane and delivering pressurized media to the expandable membrane.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] A more complete understanding of the present invention, and the attendant advantages and features thereof, will be more readily understood by reference to the following detailed description when considered in conjunction with the accompanying drawings wherein:

[0016] **FIG. 1A** illustrates a first embodiment of a double balloon catheter used in conjunction with the present invention;

[0017] **FIG. 1B** illustrates a catheter system used in conjunction with the present invention;

[0018] **FIG. 1C** illustrates the double balloon catheter of **FIG. 1A** including a flow sensor located in the handle of the catheter;

[0019] **FIG. 1D** illustrates the double balloon catheter of **FIG. 1A** including a pressure sensor located in the handle of the catheter;

[0020] **FIGS. 2A-2E** illustrate a cryoablation system incorporating various embodiments of the apparatus and method of the present invention;

[0021] **FIG. 3** is a schematic representing the mechanical components of the control console of the present invention;

[0022] **FIG. 4** is a schematic representing the mechanical components of the inflation circuit portion of the control console of the present invention;

[0023] **FIG. 5** is a schematic representing the mechanical components of the deflation circuit and main vacuum path of the control console of the present invention; and

[0024] **FIG. 6** is a schematic representing the mechanical components of the safety vacuum path of the control console of the present invention;

[0025] **FIG. 7** is a schematic representation of the embodiment illustrated in **FIG. 2A**;

[0026] **FIG. 8** is a schematic representation of the embodiment illustrated in **FIG. 2B**;

[0027] **FIG. 9** is a schematic representation of the embodiment illustrated in **FIG. 2C**;

[0028] **FIG. 10** is a schematic representation of the embodiment illustrated in **FIG. 2D**; and

[0029] **FIG. 11** is a schematic representation of the embodiment illustrated in **FIG. 2E**.

DETAILED DESCRIPTION OF THE INVENTION

[0030] The present invention is an apparatus and method for controlling the inflation and deflation of balloon catheters. In its preferred embodiment, the invention requires four steps to properly control the inflation and deflation of the balloon catheter. However, the invention allows for a variety of different implementations in order to accomplish this task. An intermediary control station containing a shut off valve and/or a coolant source may be implemented to assist in properly monitoring, controlling and maintaining the target balloon pressure and/or volume.

[0031] Referring now to the drawing figures in which like reference designations refer to like elements, a first embodiment of a double balloon catheter used in conjunction with the present invention is shown in **FIG. 1A**. The catheter **1** includes a handle **2** having a number of proximal connector ports **3a-3d**. Port **3a** may be a first vacuum connector, having a first vacuum lumen therein, such as a 10 French lumen. Port **3b** may be a coaxial connector having both a vacuum lumen and injection therein, the vacuum lumen being a second vacuum lumen, such as a 8 French lumen. Port **3c** may be an electrical connector. Port **3d** may be a guidewire luer hub.

[0032] The handle **2** further includes a blood detection board **4** and pressure relief valve **5**. The distal end portion of the catheter **1** includes two balloons: an inner balloon **6a** and an outer balloon **6b** surrounding inner balloon **6a**. A soft distal tip **7** is located just distal to the two balloons **6a** and **6b**. When refrigerant is injected into the balloons along lines **R** as shown, vacuum applied through the ports **3a** and **3b** will serve to draw any fluid within balloons **6a** and **6b** along arrows **V** out of the balloons and the catheter. Radiopaque marker bands **M** are located proximate the exit point of the refrigerant injected into balloon **6a** to aid in the positioning and tracking of the device.

[0033] Catheter **1** includes an elongate shaft having a guidewire **8** and an inner shaft **9a** and outer shaft **9b**. Exemplary embodiments of the inner shaft **9a** include an 8 French shaft, while exemplary embodiments of the outer shaft **9b** include a 10 French shaft.

[0034] A typical catheter system **10** is shown in **FIG. 1B**. The system includes a console **20** coupled to one end of an umbilical system **12**. The opposing end of umbilical system **12** is coupled to an energy treatment device **22**. Energy treatment device **22** may be a medical probe, a catheter, a balloon-catheter, as well as other devices commonly known in the art that are smooth enough to pass easily through blood vessels and heart valves. As shown in **FIG. 1A**, the

energy treatment device **22** includes a balloon structure **23** that can be a single wall or a double wall configuration, wherein the double wall configuration places the space between balloon walls in communication with a vacuum source.

[0035] Umbilical system **12** is comprised of three separate umbilicals: a coaxial cable umbilical **14**, an electrical umbilical **16** and a vacuum umbilical **18**. An outer vacuum umbilical is used in the case of a double balloon system; it is not necessary for a single balloon system having only one vacuum lumen. If the user wishes to perform an RF ablation procedure, radiofrequency energy can be provided to electrodes on device **22** via electrical umbilical **16** to perform an RF ablation technique as is common in the art. Electrical umbilical **16** can include an ECG box **82** to facilitate a connection from electrodes on catheter **22** (not shown) to an ECG monitor. Coaxial umbilical **14** includes both a cooling injection umbilical and a vacuum umbilical that provide respective inlet and return paths for a refrigerant or coolant used to cool a tissue-treating end of device **22**. The vacuum umbilical **18** is used as safety conduit to allow excess coolant or gas to escape from device **22** if the pressure within the balloon on device **22** exceeds a predefined limit. The vacuum umbilical **18** can also be used to capture air through a leak of the outer vacuum system where it is outside the patient and as a lumen to ingress blood when in the patient.

[0036] Referring once again to **FIG. 1B**, catheter system **10** may include one or more sensors **11**, which are used to monitor the amount of fluid or gas refrigerant injected through the umbilical system and into the balloons. It is contemplated that the sensors may be located in one of several locations throughout catheter system **10**. For example, sensor **11** may be located in console **20**, ECG Box **82**, and/or handle **2**.

[0037] Two different types of sensors are contemplated for use with the present invention in order to monitor how much coolant is flowing into the balloons. A flow sensor **13** shown in **FIG. 1C**, measures the rate or speed of fluid or gas at a certain location. An exemplary embodiment of flow sensor **13** is the Microbridge Mass Air Flow Sensor by Honeywell®.

[0038] Alternately, one or more sensors **11** may be a pressure sensor **15** as shown in **FIG. 1D**. Pressure sensor **15** in **FIG. 1D** is a differential pressure sensor that can determine the amount of pressure in the balloons by determining the difference in pressure between points p_1 and p_2 and the velocity through the restriction point d . An exemplary embodiment of pressure sensor **15** is the 26PC SMT Pressure Sensor by Honeywell®.

[0039] **FIGS. 2A-2E** illustrate different embodiments of the catheter system **10** of the present invention. In general, the inflation/deflation system described herein can be used with both single and double balloon systems. For a single balloon system, the refrigerant is sprayed into the balloon and creates a circumferential region of cooling around the balloon's perimeter. The refrigerant expands and the vapor is drawn back into the console via the return vacuum lumen. With respect to a double balloon system, a second balloon and second vacuum lumen envelop the single balloon system and are always maintained under vacuum for safety reasons. The vacuum of the outer balloon will capture refrigerant

escaping through any breach of the inner balloon system. A flow switch mounted on the outer vacuum system is used to monitor any flow activity. Under normal operation, no fluid should pass through the outer vacuum system. Any discussion of a "flow switch" herein implies a double balloon system. Otherwise, all inflation/deflation methods also apply to a single balloon catheter.

[0040] Each embodiment includes a console **20** or console **21**, an umbilical system comprised of varying combinations of separate umbilicals, and an ablation device **22**. Each of the embodiments shown in **FIGS. 2A-2E** is represented by more detailed corresponding schematics in **FIGS. 7-11**, respectively, and are discussed in greater detail below.

[0041] **FIG. 2A** represents a typical catheter ablation system **10**. Console **20** is coupled to a catheter **22** via an umbilical system **12**, comprised of coaxial umbilical **14**, which transfers coolant from console **20** to catheter **22** and provides a return conduit for the coolant, electrical umbilical **16**, which transfers RF energy from console **20** to catheter **22** during an RF ablation procedure or electrical signals during a cryoablation procedure, and safety vacuum umbilical **18**, to allow for quick evacuation of coolant if needed.

[0042] Coolant is provided by a coolant source within console **20**. Coolant, typically N_2O , passes through the internal piping of console **20** before being transferred to catheter **22** via the coaxial umbilical **14**. At the distal end of the umbilical, inside catheter **22**, the coolant is released inside the catheter tip cavity, which is under vacuum. Both the phase change from liquid to gas and the sudden expansion of the coolant are endothermic reactions, causing a temperature differential which results in the catheter tip or balloon freezing. The coolant vapor is then returned through the vacuum path via umbilical **14** and into console **20**, where it is evacuated through a scavenging line.

[0043] **FIG. 2B** represents another catheter ablation system. However, in this embodiment, an intermediary station **74** is inserted into the catheter system. As explained in greater detail below, station **74** contains detection valves to detect a drop in balloon pressure which might indicate a leak, and shut off valves to terminate balloon inflation if necessary. Station **74** is coupled to console **21** and catheter **22** via electrical umbilical **16** and coaxial umbilical **14**. Vacuum umbilical **18** provides an emergency evacuation path for coolant from the catheter.

[0044] **FIG. 2C** represents the catheter ablation system of **FIG. 2A** including a secondary coolant source **78** used to re-inflate the expandable membrane, or balloon **23** of catheter **22** via syringe **76**.

[0045] **FIG. 2D** illustrates two possible configurations for the ablation system. In a first configuration, a secondary coolant source includes a small tank or canister **80** located within an intermediary station **74**. In a second configuration, the secondary coolant source includes a small tank or canister **60** located inside the console **21**. In both configurations, the secondary coolant source is independent from the source of cooling provided by other components within the console **21** (the primary coolant source), and it does not require the same type of refrigerant that is provided by the primary coolant source.

[0046] **FIG. 2E** illustrates a configuration where the secondary cooling source and the primary cooling source are unified and thus share the same source of refrigerant.

[0047] **FIG. 3** refers to a schematic representing the console **20** portrayed in **FIGS. 2A and 2C**. The schematic shown is designed specially for balloon catheters and contains a series of two and three-way solenoid valves and regulators that assist in monitoring the pressure of the balloon catheter **23**, which may drop quickly if a leak of fluid occurs. Device **22** (shown in **FIGS. 2A-2E**) is a catheter with an expandable membrane **23** at its distal end. Console **20** is represented by the schematic in **FIG. 3** that shows the layout of the internal mechanical components of console **20**.

[0048] In an exemplary embodiment, the system is operated in four phases. The first phase is the evacuation/flushing phase. When the catheter **22** is inserted inside the patient it is first necessary to evacuate air molecules from within the catheter, air contained inside the umbilical connecting the catheter **22** to the console **20**, as well as from the catheter shaft itself. Although it is not theoretically possible to evacuate 100% of the air molecules, by minimizing the amount of air within the umbilical and catheter shaft, the catheter is prepared for inflation and then ablation, while minimizing the dangers associated with fluid egress.

[0049] During the evacuation/flushing phase, a 3-way solenoid valve **24** is open toward vacuum pump **26**, which ensures that there is a vacuum in catheter **22**. The 3-way solenoid valve **24** can be replaced by a PID-driven proportional valve. In either configuration, the 2-way solenoid **28** that supports high pressure is closed to prevent any high-pressure gas from reservoir **30** from entering the inner vacuum system/balloon catheter during the refilling process. Reservoir **30** could be a tube or reservoir containing enough fluid volume to fill the umbilical tubes and catheter **22** to a predefined pressure. If the pressure within reservoir **30** exceeds a predetermined pressure setpoint, a check valve **32** will open to evacuate the exceeded amount of coolant such as, for example, nitrous oxide (N_2O) in the system in order to keep a fixed amount of nitrous oxide in reservoir **30**. During this phase, reservoir **30** is filled with N_2O received from N_2O source **60**. The N_2O is received from a high pressure line after leaves tank **60** and passes through a series of regulators, namely, a first regulator **34**, a second regulator **36** and then into either a third regulator **38** or a proportional valve, that are adjusted to the predetermined pressure. The reservoir pressure can be controlled through a pressure regulator **38** or through a proportional valve that would refill the tank with different pressure setpoints for different balloon sizes or different inflation pressures. The pressure setpoint can be programmed into a circuit, chip or other memory device that can be located in the handle.

[0050] Refilling valve **40** opens for a period of time and fills reservoir **30**. During this phase, the 2-way solenoid valve **28** remains closed. Also, during this phase, the system is under vacuum and provides verification for any leaks that occur.

[0051] Thus, when the catheter is outside the patient, any breach of the inner or outer vacuum systems will be detected by a high baseline flow through the console flow meter. In addition, a flow switch located in the console or in the catheter handle and mounted on the outer vacuum system will also detect a leak of air through a breach of the outer balloon or vacuum lumen. The flow switch is capable of detecting volumes of gas as little as 1 cc of vapor, and flow rates as little as 20 sccm. When the catheter is inserted

into the patient, blood ingress through either the inner or outer vacuum lumens or both will be detected by the leak and blood detection systems. In the case of a constant pressure inflation with circulating flow, the balloon pressure can also be controlled with a PID-driven proportional valve located on the return vacuum lumen or a three-way solenoid valve in series with a pressure switch or pressure transducer.

[0052] Referring to **FIG. 4**, the inflation phase of the invention will now be discussed. Prior to positioning catheter **22** on the ablation site, the physician must first inflate the expandable membrane **23** inside the heart chamber and then position the balloon **23** proximate the ablation site. During this phase, the system is under vacuum and provides verification for leaks between balloon **23** and the blood. In one embodiment, balloon **23** is inflated by injecting fluid or gas through the umbilical under a fixed flow pressure. This insures a defined and constant pressure inside the balloon in order to provide a mechanical force for inflation. An alternate way to inflate balloon **23** is to use a fixed volume of inflation. This volume would be minimized in order to meet the constraints related to gas egress within the blood stream (maximum of 20 cc within 10 minutes) and meet the requirement for pressure needed to inflate the balloon under the harshest room conditions.

[0053] **FIG. 3** illustrates the inflation portion of the console mechanics of **FIG. 2**. During the inflation phase, valve **24** is open toward reservoir **30** and valve **28** opens, while refilling valve **40** remains closed. A fixed amount of N_2O is injected to inflate balloon **23** in order to provide sufficient mechanical force for inflation. If a leak occurs in the balloon, the released volume of N_2O would be no more than 20 cc. The solenoid valve **44** (shown in **FIG. 33**) remains open during this phase in order to ensure a vacuum in the safety line. If a leak occurs in the inner balloon of the catheter, the flow switch **42** (**FIG. 3**), detects leaks as small as 1 cc of vapor. Flow switch **42** is active during all phases to prevent any leak of the inner balloon system in catheter **22**. The leak and blood detection systems are still active and monitoring any blood ingress through the outer vacuum lumen. After air has been flushed from catheter **22** and the umbilicals connecting catheter **22** to console **20**, and balloon **23** has been inflated, ablation may now take place.

[0054] A transition mode follows inflation but precedes ablation. In the case of cryogenic ablation systems, a transition method is needed to transition from closed pressurized volume to an open circuit, which allows the flow of refrigerant to enter and exit the catheter tip while at the same time controlling the balloon pressure in order to keep the balloon inflated and in place. During the transition, a pressure switch, which is adjusted to a pressure higher than atmospheric pressure but preferably lower than 20 psia, monitors the pressure inside the balloon catheter **22**. The solenoid valve **24** remains closed until the pressure in the catheter is higher than the preset switch value after which the solenoid valve opens to allow evacuation of excess refrigerant. When the pressure falls below the reset switch value, the solenoid valve **24** closes to keep the balloon inflated and above atmospheric pressure. During the transition, ablation is already initiated but the pressure switch controls the balloon pressure until refrigerant flow alone maintains the balloon open and above atmospheric pressure. The transition phase is considered complete when certain conditions are met: 1) when the pressure switch commands the solenoid valve **24**

to open to vacuum and the balloon pressure remains above the present switch value; 2) the duration of the transition phase exceeds a predetermined time; and 3) the injection pressure reaches a predetermined value that is adequate to generate enough flow to maintain the balloon open. Check valve **56** is used to prevent any abnormal rise in the pressure in the catheter tip. Another check valve **58**, shown also in **FIG. 6**, prevents any excessive pressure in the safety vacuum line and in the event the solenoid valve **44** is blocked.

[0055] During the ablation phase, refrigerant is injected through the umbilical system into the ablation device **22**. When injection of refrigerant is desired, N₂O gas is released from source **60** and provides high pressure liquid through a check valve **62** and a series of pressure regulators **34** and **36**. Regulators **34** and **36** are primary and secondary pressure regulators respectively, which serve to bring the gas pressure down to between 810 and approximately 840 psig. The liquid nitrous oxide goes through a proportional valve **64** driven by a Proportional Integral Derivative (PID) controller **66** so that the refrigerant pressure can be varied from 0 psig to approximately 760 psig, and through an injection solenoid valve **68** which remains open. The N₂O then passes through a sub-cooler **70** with various refrigeration components such as a compressor, a condenser, a capillary tube and a heat exchanger, which insures its liquid state through the umbilical and into the small diameter catheter injection tubing. During injection, solenoid vent valve **46** is closed. To detect a failure of this valve, the pressure switch **72** will close when detecting a pressure higher than 15 psig, creating a failure signal.

[0056] During the injection phase, proportional valve **64** is used to vary the pressure inside the injection line. This in turn will vary the flow rate of refrigerant to the catheter tip. An increase in the flow rate (less restriction by the regulator) lowers the temperature of the catheter tip. Conversely, decreasing the flow rate allows the catheter tip to be warmed by its surroundings.

[0057] **FIG. 5** illustrates the deflation and main path circuitry of the present invention. At the end of the ablation phase, the system provides a method to insure a controlled/slow deflation in order to prevent damaging the ablated tissue during balloon deflation. This can be a hazard due to cryoadhesion, which may occur when the catheter attaches to the tissue during freezing. Referring to both **FIGS. 3 and 5**, during deflation, the solenoid valve **24** (**FIG. 3**) remains closed until the temperature in the balloon is higher than a predetermined temperature (usually above freezing to ensure that surrounding tissue has thawed). When the temperature increases to greater than the predetermined temperature, the solenoid valve **24** opens to vacuum and collapses the balloon. On both vacuum paths, liquid sensors and insulated liquid spargers **48** and **50** (**FIG. 3**) are installed to prevent any liquid from entering the vacuum pump **26**. If this occurs, injection and/or inflation will be stopped and both valves **52** (**FIG. 3**) and **44** (**FIG. 3**) will switch to atmosphere.

[0058] **FIG. 6** illustrates the safety vacuum portion of the console circuitry of **FIG. 3**. If a leak occurs in the catheter during inflation or ablation, flow switch **42** can detect such a leak in amounts as small as 1 cc of vapor. Upon detection of the leak, inflation of the balloon catheter is stopped. Prior

to inflation, the flow switch can detect leaks of the outer balloon or guide wire lumen when the catheter is in the air. In case of pressurization of the safety vacuum line 1/3 psi above atmosphere, a pressure relief valve **58** located distal to the flow switch will vent excess pressure.

[0059] Referring now to **FIG. 7**, one embodiment of the present invention is shown. The schematic in **FIG. 7** illustrates the mechanical connection of the console **20**, umbilical system **12** and catheter **22**. The representation in **FIG. 7** corresponds to the embodiment shown in **FIG. 2A**. The internal components of console **20** are similar and correspond to those shown in greater detail in **FIG. 3** explained above. In this embodiment, the balloon **23** is inflated by receiving gas or fluid from source **60** via coaxial umbilical **14**. PID controller **66** controls the flow of pressurized fluid/gas from console **20** through umbilical system **12** to balloon **23**.

[0060] **FIG. 8** shows an alternate embodiment of the invention in which an intermediary station **74** containing all components and circuits to operate the balloon catheter is coupled to console **10**, between the console and balloon catheter **23**. Station **74** includes a series of shut-off valves and detection switches. Detection circuitry within station **74** can detect if the volume of gas within balloon catheter **23** has exceeded a certain predetermined amount (i.e. 20 cc within the catheter and the umbilical system), and shut-off valves within station **74** are activated, preventing any further inflation. Station **74** advantageously provides a quicker and more effective way of detecting leakage of gas or liquid into the blood stream. If the pressure within balloon catheter **23** drops, this could be an indication that fluid within the balloon has escaped. By inserting station **74** within system **10**, a quicker and more efficient way of detecting leaks and preventing unwanted balloon inflation is provided.

[0061] **FIG. 9** shows yet another embodiment of the invention. Here, balloon inflation can be performed by a syringe **76** coupled to a saline water source **78** or any other fluid media including gasses or liquids. This embodiment becomes practical when manual balloon inflation is required.

[0062] In **FIG. 10**, intermediary station **74** includes a second inflation source **80**. As in the embodiment depicted in **FIG. 8**, leak detection circuitry and shut-off valves located in station **74** provide an efficient way of detecting leaks and quickly prohibiting the further inflation of balloon catheter **23**. Should further inflation be required, a separate pressurized N₂O source **80** is provided in station **74**, which is at a closer and more convenient location, i.e. nearer the catheter and not in a remote location such as console **20**.

[0063] In **FIG. 10**, the refilling source **80** is located in the intermediate box **74** and inflation occurs through the outer vacuum umbilical. In **FIG. 11**, the refilling source is the coolant tank **60** located in the cryoablation console and inflation occurs through the inner vacuum umbilical.

[0064] It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described herein above. In addition, unless mention was made above to the contrary, it should be noted that all of the accompanying drawings are not to scale. A variety of modifications and variations are possible in light of the above teachings without departing from the scope and spirit of the invention, which is limited only by the following claims.

1-11. (canceled)

12. An apparatus for inflating and deflating a catheter having a first expandable membrane, the apparatus comprising:

a first console including means for controlling the inflation and deflation of the first expandable membrane in order to reach a target pressure or volume;

a catheter; and

an umbilical system coupling the console to the catheter and delivering pressurized coolant to the first expandable membrane.

13. The apparatus of claim 12, wherein the first console includes means for determining if the first expandable membrane has reached its target pressure or volume.

14. The apparatus of claim 13, wherein the means for determining if the first expandable membrane has reached its target pressure or volume is a Proportional Integral Derivative controller.

15. The apparatus of claim 12, further comprising an intermediary console located between the first console and the catheter.

16. The apparatus of claim 15, wherein the intermediary console includes means for interrupting the flow of pressurized coolant from the first console to the catheter if the target pressure or volume has been exceeded.

17. The apparatus of claim 16, wherein the means for interrupting the flow of pressurized coolant from the first console to the catheter is a shut-off valve located within the intermediary console.

18. The apparatus of claim 15, wherein the intermediary console includes means for re-inflating the first expandable membrane.

19. The apparatus of claim 18, wherein the means for re-inflating the first expandable membrane is a source of pressurized coolant within the intermediary console.

20. The apparatus of claim 12, wherein the catheter further comprises a second expandable membrane, the first

and second expandable membranes defining a safety vacuum space disposed between the first and second expandable membranes.

21. The apparatus of claim 20, further comprising a vacuum umbilical in communication with the safety vacuum space.

22. The apparatus of claim 21, further comprising a flow switch.

23. The apparatus of claim 22, further comprising a flow detector, the flow switch and flow detector being in fluid communication with the safety vacuum space.

24. The apparatus of claim 20, further comprising a pressure sensing element in communication with the safety vacuum space.

25. The apparatus of claim 20, further comprising a leak detection element in communication with the safety vacuum space.

26. The apparatus of claim 20, further comprising a blood detection element in communication with the safety vacuum space.

27. The apparatus of claim 20, further comprising a fluid detection element in communication with the safety vacuum space.

28. The apparatus of claim 12, further comprising a pressure sensing element in communication with a volume within the first expandable membrane.

29. The apparatus of claim 12, further comprising a leak detection element in communication with a volume within the first expandable membrane.

30. The apparatus of claim 12, further comprising a blood detection element in communication with a volume within the first expandable membrane.

31. The apparatus of claim 12, further comprising a fluid detection element in communication with a volume within the first expandable membrane.

* * * * *