



(22) Date de dépôt/Filing Date: 2009/10/09

(41) Mise à la disp. pub./Open to Public Insp.: 2010/04/15

(45) Date de délivrance/Issue Date: 2021/08/03

(62) Demande originale/Original Application: 2 776 425

(30) Priorité/Priority: 2008/10/10 (US61/136885)

(51) Cl.Int./Int.Cl. *A61F 2/26* (2006.01),
A61F 5/41 (2006.01), *A61M 5/142* (2006.01),
A61M 5/158 (2006.01)


(72) Inventeur/Inventor:
FORSELL, PETER, CH

(73) Propriétaire/Owner:
MEDICALTREE PATENT LTD., MT

(74) Agent: SMART & BIGGAR IP AGENCY CO.

(54) Titre : INFUSION DE MEDICAMENTS

(54) Title: INFUSION OF DRUGS

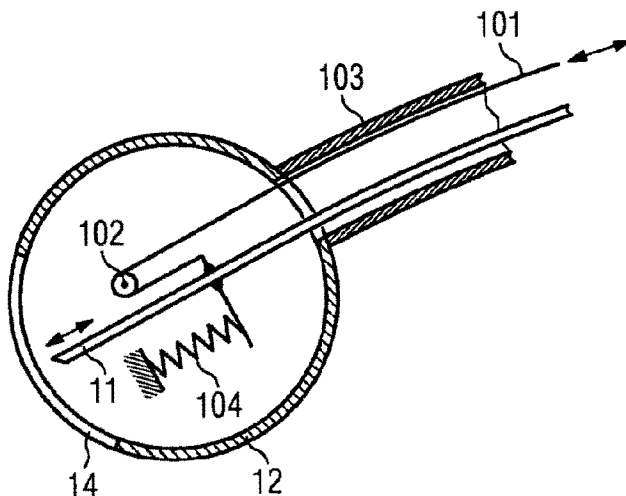

(57) **Abrégé/Abstract:**

An at least partly implantable system for injecting a substance into a patient's body, in particular a penis erection stimulation system, comprises one or more long, flexibly bendable infusion needles, the tip ends of which are disposed within and implanted along with at least one first housing, in particular adjacent the patient's left and right corpora cavernosa. The respective other end or ends of the infusion needles are disposed and implanted along with at least one second housing remote from the first housing. A reservoir and a pump are also implanted inside the patient's body to supply the infusion needle with infusion liquid. A drive unit also adapted for implantation inside the patient's body is arranged for advancing and retracting the infusion needle such that its tip end penetrates the at least one first housing's outer wall in at least one penetration area, more specifically at least in two different penetration areas either simultaneously or in immediate time succession, thereby injecting the substance into the patient's body.

Abstract

An at least partly implantable system for injecting a substance into a patient's body, in particular a penis erection stimulation system, comprises one or more long, flexibly bendable infusion needles, the tip ends of which are disposed within and implanted
5 along with at least one first housing, in particular adjacent the patient's left and right corpora cavernosa. The respective other end or ends of the infusion needles are disposed and implanted along with at least one second housing remote from the first housing. A reservoir and a pump are also implanted inside the patient's body to supply the infusion needle with infusion liquid. A drive unit also adapted for
10 implantation inside the patient's body is arranged for advancing and retracting the infusion needle such that its tip end penetrates the at least one first housing's outer wall in at least one penetration area, more specifically at least in two different penetration areas either simultaneously or in immediate time succession, thereby injecting the substance into the patient's body.

INFUSION OF DRUGS

This application is a divisional of Canadian Patent Application Number 2,776,425 filed on October 9, 2009.

Background of the Invention

- 5 The present invention relates generally to the infusion of a substance, in particular drugs, into a patient's body, and, more specifically, to the stimulation of penis erection.

When a male is stimulated erotically, connections between arteries and veins are closed (arteriovenous anastomoses) so that blood which is normally able to bypass the empty spaces or sinuses of the corpora cavernosa is retained in the penis.

- 10 The main vessels supplying the blood to the cavernous spaces in the erectile tissue of the corpora cavernosa are the deep arteries of the penis. They are therefore heavily involved in the erection of the penis. They give off numerous branches - the helicine arteries - that open directly into the cavernous spaces. When the penis is flaccid, these arteries are coiled, restricting blood flow. However, the smooth muscle in the coiled
15 helicine arteries relaxes as a result of parasympathetic stimulation. In their relaxed state, the helicine arteries straighten, enlarging their lumina and allowing blood to flow into and dilate the cavernous spaces in the corpora of the penis at arterial pressure. In combination with the bulbospongiosus and ischiocavernosus muscles compressing the veins egressing from the corpora cavernosa, the erectile bodies of the penis become
20 enlarged and rigid, and an erection occurs.

- Patients suffering from erectile dysfunction can cause the penis to become turgid by injecting into the corpora cavernosa a medicament, such as papaverine or prostaglandin E1, causing the smooth muscles to relax. The patients have to learn a certain technique under doctor's supervision in order to be able to properly inject the medicament in each
25 of the corpora cavernosa. Only after about 15 minutes after administration of the medicament will the medicament become effective. The entire procedure is inconvenient, the more so as the medicament must usually first

be mixed together from a dry substance and a saline solution. Only as a dry substance (and typically cooled) are the available medicaments stable.

Furthermore, proper administration and dosing is critical since the medicament
5 may be transported with the blood into other regions of the patient's body if the injection is not done properly.

Recently, a different method has become known under the brand Muse®. In this method, a plastic rod comprising the medicament alprostadil is inserted into the
10 urethra. Upon pressing a button, the alprostadil is released from the rod into the urethra. After removal of the plastic rod, the penis is rolled between the palms of the hands so that the medicament dissolves, distributes and is absorbed through the urethra wall. However, proper dosage and administration is also critical in this method.

15 The afore-mentioned problems are not limited to the administration of drugs stimulating penis erection. Similar problems can also occur in other applications where a substance is to be injected frequently.

20 It is therefore the object of the present invention to improve the administration of a drug into a patient's body, and more specifically to improve the stimulation of a penis erection so that the entire process is more reliable and more convenient for the patient.

25 **Summary of the Invention**

The essence of the invention lies in injecting a substance into the patient's body using at least one implantable infusion needle. This will greatly improve the patient's comfort as he no longer needs to pierce himself with the infusion needle,
30 which for many people is not an easy task. Furthermore, due to the permanent implantation of the infusion needle, the injection will always occur at the proper location, said location being selected such that the drug is most effective. While there are many conceivable technical variations for injecting the drug through the infusion needle into the patient's body, such injections are definitely more
35 convenient for the patient once the infusion needle has been implanted as

compared to the alternative of injecting the drug manually from outside the patient's body.

- According to the invention, the at least one implantable infusion needle is long and flexibly bendable, with the respective tip end or ends being disposed within (at least one) first housing so as to penetrate the first housing's outer wall or walls in at least one penetration area, preferably in two or more different penetration areas. As will be described below, two or more infusion needles may be provided in order to inject the drug in the two or more different penetration areas, or a single infusion needle may be provided along with an appropriate drive unit for displacing the tip end of the infusion needle so as to penetrate the first housing's outer wall in the respective different penetration areas. Arranging the infusion needle's tip end in said first housing prevents any fibrosis from growing into the infusion needle.
- The use of one or more long flexible needles is chosen for reasons of space constraints in the area where the injection of the drugs has to occur. The at least one first housing accommodating the tip end of such long infusion needle or needles can be kept small and, therefore, can be arranged conveniently in close proximity to a constrained injection area, where the tip end can penetrate the outer wall of the first housing upon advancement of the long infusion needle. The respective other end of the long, flexibly bendable infusion needle or needles, i.e. the infusion needle's rear end, is arranged in a second housing which can be implanted inside the patient's body remote from the first housing in an area with fewer space constraints. The injection needle is sufficiently long to bridge the distance from the second housing for remote implantation to the first housing and further through the first housing up to the outer wall of the first housing to be penetrated by the needle. Thus, since the respective other end of the infusion needle or needles is remotely implanted within the patient's body, other components of the system cooperating with the rear end of the infusion needle may also be implanted remote from the injection area, such as a reservoir for storing the substance to be injected, a pump for advancing the substance from the reservoir to the infusion needle and further through the needle into the patient's body, a motor for actuating the system's active parts, at least one drive unit for – at least – advancing (and possibly retracting) the infusion needle or needles in such a way that it penetrates at least one penetration area - preferably two or more different penetration areas - so as to allow for injecting the substance

through said penetration area or areas via the at least one infusion needle, and so forth. In a particularly preferred embodiment, the tip end of the infusion needle is advanced by advancing the entire needle from the infusion needle's rear end. It is particularly advantageous to arrange at least a part of the drive unit, preferably the entire drive unit, for advancing the infusion needle within the second housing. More preferably, a reservoir and/or most or all of the active parts, such as a motor, a pump and the like, may also be implanted remotely within the patient's body and, more preferably, may be accommodated in the remotely implanted second housing, whereas the first housing only includes passive elements, possibly including passive elements of the drive unit. In this context it is to be understood that a drive unit according to the present invention includes not only the drive itself, such as an electric motor, but also those components which are involved in transforming the driving energy provided by the drive into movement of the at least one needle, such as transmission gears and the like. Other components such as an energy source, a control unit and/or a data processing device may be extracorporal to complete the system. However, it is preferred that the aforementioned components be implanted as well, preferably forming an integral part with the remaining components of the system so as to be implantable as a unitary piece with the second housing.

The infusion needle or needles may rest at the implantation site over a long time either for single use or for multiple use. For instance, where it is likely that a patient will suffer an allergic attack, such as severe allergic reactions affecting e.g. the respiratory tract, in the near future or possibly only within a year or two, the infusion needle and possibly the entire system may be implanted in the patient's body for single use at the appropriate time. Over time, fibrosis will grow on the system. However, at the time of use, the infusion needle may be advanced by the drive unit so as to penetrate any fibrosis, thereby allowing immediate drug delivery from the reservoir through the tip end of the infusion needle into the patient's body. Where the infusion needle is implanted adjacent a blood vessel, the tip end of the infusion needle may be advanced into the blood vessel without any risk of formation of thrombosis (nicht fibrosis?) prior to use.

Where the system is implanted for multiple use, the drive unit is preferably configured for advancing and retracting the tip end of the infusion needle. Thus,

each time when the drug is delivered to the patient, the infusion needle will be advanced, the drug injected and the infusion needle retracted again.

5 More specifically, in the case of multiple use, it is even preferred when the at least one drive unit is coupled to the at least one infusion needle so as to advance and retract the tip end of the at least one infusion needle in such a way that it penetrates at least two different penetration areas within the housing's outer wall, so as to allow for injecting the substance through said at least two different penetration areas via the at least one infusion needle. The distance between the
10 two different penetration areas to be penetrated by the at least one infusion needle is selected such that the respective parts of the patient's body are pierced whenever the drug is to be injected.

15 This structure can advantageously be used for stimulating penis erection, in which case the first housing or housings are adapted for implantation inside the patient's body adjacent to both the right and left corpus cavernosum of the patient's penis and/or the two deep arteries of the right and left corpus cavernosum and/or adjacent to muscle tissue regulating blood flow through the patient's left and right corpus cavernosum and/or in sufficiently close proximity to another type of tissue
20 allowing both the first and second corpus cavernosum to become turgid when the particular drug is injected therein. The at least one infusion needle then penetrates the at least two different penetration areas either simultaneously (e.g. where a plurality of needles, i.e. at least two needles, are provided) or in immediate time succession (e.g. where a single needle is provided).
25 Preferably, a single command or single action from the patient is sufficient for injecting the substance through the at least two penetration areas, either due to a corresponding mechanical structure of the drive unit or due to a suitably configured control unit controlling the drive unit. This will make the handling of the system easy for the patient.

30 Where two different penetration areas are pierced in immediate time succession, the time delay between the penetration of the first and the second of the penetration areas is preferably as short as possible, more preferably less than 120 seconds, and most preferably less than 60 seconds. This can be achieved by
35 means of a properly controlled drive unit. A longer time delay would be inconvenient for the patient. Therefore, it is preferred that, once the infusion

needle has been retracted from a first of the two penetration areas, it is immediately advanced to the second of the penetration areas.

While it is possible according to one aspect of the invention to actively open the
5 outer wall or walls of the at least one first housing for allowing the infusion needle
to penetrate the outer wall, it is preferred according to another aspect of the
invention to arrange the needle so as to penetrate the outer wall by piercing
through the outer wall. For that purpose, the outer wall may either comprise flaps
10 to be pushed aside by the infusion needle as the infusion needle is advanced, or
the outer wall may be made at least in the penetration areas from a material which
is self-sealing in respect of penetrations resulting from the at least one infusion
needle. This is generally known from WO 2007/051563 disclosing an implantable
infusion device with a single infusion needle entirely contained in a housing to be
15 implanted adjacent an injection area, the needle being laterally displaceable within
the housing and both advanceable and retractable through the housing's outer
wall. While the entire first housing may be made from the self-sealing material, it is
advantageous for stability reasons if the self-sealing material forms at least one
window area in the outer wall, the window area being positioned for penetration by
20 the tip end of the at least one infusion needle. The window area may be formed by
a self-sealing penetration membrane which is preferably integrated in the outer
wall by press fitting it into the outer wall. Typically, the self-sealing material would
be made from a polymer material which preferably comprises silicone. Other
biocompatible polymer materials, such as polyurethane and the like, may be
employed as well. The self-sealing material may also be a composite material. A
25 particularly preferred embodiment of such composite material comprises at least
one outer shape-giving layer and a self-sealing soft material contained within the
outer layer. Thus, the outer layer forms a shell for the soft material. The outer
layer may be made from a biocompatible polymer, such as one of those polymers
mentioned above, and preferably the self-sealing soft material may be a gel.

30 Instead of a self-sealing material, the part of the outer wall of the first housing to
be penetrated by the infusion needle may comprise one or more flaps in the
penetration areas through which the infusion needle or needles can pass. This can
reduce the force needed for the infusion needle to penetrate the outer wall, as
35 compared to the penetration of a self-sealing membrane. The flap is preferably

arranged to be pushed aside by the infusion needle upon advancement of the infusion needle.

Alternatively, the outer wall may comprise at least one door in the penetration areas. A drive is connected to the door for actively opening the door so as to allow for the infusion needle to be advanced through the opened door. Again, the door may comprise a flap, such as a resilient, normally closed flap. It is particularly preferred if the drive connected to the door forms part of the drive unit coupled to the infusion needle. More specifically, the arrangement may be such that advancement of the infusion needle by means of the drive unit simultaneously causes the drive to open the door.

The at least one infusion needle preferably has a tube-like body closed at the tip end and provided with a laterally arranged delivery exit port for delivery of the drug into the particular body part. Therefore, the needle will not cut out any material but will simply divide it during penetration. Thus, when the needle penetrates any material, such as fibrosis and/or the self-sealing penetration membrane, there will be no material entering and blocking the drug delivery passageway.

As mentioned above, a separate infusion needle may be provided for each of the two or more penetration areas. Thus, where injection is desired to occur in two or more different areas, such as for provoking penis erection, two or more separate infusion needles may be advanced through the corresponding penetration area of the respective first housing or housings – preferably simultaneously – and retracted again after injection.

According to a preferred embodiment of the invention, a plurality of two or more infusion needles is provided for each of the different penetration areas and arranged for penetrating different penetration sites within each of said different penetration areas. This allows for penetrating different sites within each penetration area at different times, thereby giving the human tissue time to recover from the piercing by the infusion needle. This can be achieved with a drive unit suitably configured to advance and retract one infusion needle in each of said different penetration areas at one time, and to advance and retract a different infusion needle in each of said different penetration areas at a different time.

The drive unit may be such that the infusion needle is advanced and/or retracted by turning the infusion needle or by turning an element cooperating with the infusion needle. More specifically, the drive unit for advancing and retracting the infusion needle may comprise a screw drive connection. For instance, the drive of
5 the drive unit may turn a screw threadingly engaged with a rack coupled to the infusion needle so that rotation of the screw will cause the infusion needle to be advanced or retracted. The screw and rack of the screw drive connection are preferably accommodated in the remotely implanted second housing but may also be arranged in the housing accommodating the tip end of the needle. Instead of
10 the screw, the infusion needle itself may be rotated by means of a suitable drive so that threading on the needle engaging a fixedly mounted rack causes the infusion needle to advance or retract upon rotation of the infusion needle. Between the first and second housings, the infusion needle is preferably guided in a sheath, so as to reduce friction and prevent growth of fibrosis that might hinder movement
15 of the needle.

The tip ends of a plurality of infusion needles may be contained in a common housing in spaced apart relationship, with the drive unit being configured to advance and retract the tip ends of the infusion needles so as to penetrate the
20 outer wall of the common housing in said at least two different penetration areas, again preferably simultaneously. Placing the tip ends in a common housing simplifies the procedure for fixing the needles in place close to the injection areas. Furthermore, a single drive unit may be used for advancing and retracting the tip ends of the plurality of infusion needles, this making the entire system less
25 voluminous.

According to a particularly preferred aspect of the invention, the tip end or ends of the at least one infusion needle are laterally movable, so as to vary the penetration sites within the particular penetration areas of the first housing's outer wall,
30 thereby varying the injection site within the particular injection area in the patient's body. As set out above, frequent piercing of the same body part may cause irritation, eventually making further piercing difficult or even impossible. Variation of the injection site by laterally displacing the needle upon each injection cycle may overcome such problems. Accordingly, the at least one drive unit is preferably
35 configured to laterally displace the tip end or ends of the at least one infusion needle to different penetration sites within each of said different penetration areas.

More specifically, the drive unit is preferably configured to laterally displace the tip ends of two or more infusion needles simultaneously. This can be achieved e.g. by jointly mounting the tip ends of the infusion needles on a movable carriage of the drive unit, such as a turntable and/or a shuttle, possibly in the form of a slide.

- 5 Thus, the drive unit for advancing and retracting the tip ends of the infusion needles is preferably configured so as to also laterally displace the tip ends of the infusion needles each time the tip ends are advanced or retracted.

- 10 Thus, the lateral displacement and the advancement/retraction of the tip end or ends of the at least one infusion needle are coordinated. The lateral displacement of the tip end may take place before and/or after an injection. The mechanism may be such that after a certain number of lateral displacements or after lateral displacement over a predefined distance, the tip end of the infusion needle is laterally returned to its initial position so that the next number of infusions will take place again at locations that have previously been penetrated by the needle. It is even preferred to configure the drive unit such that the tip end or ends of the at least one infusion needle are displaced in at least two different lateral directions. For instance, when the infusion needle has laterally returned to its initial position, the next number of infusions may take place somewhat laterally offset above or below the first number of penetration sites. This permits a two-dimensional array of penetration sites to be obtained.

- 25 The tip ends of two or more infusion needles may be arranged one above the other within a common first housing. Generally speaking, it is preferable in such a situation that the direction of lateral displacement of the tip ends of the infusion needles within the different penetration areas is different from, in particular perpendicular to, the direction of distance between the different penetration areas. Alternatively, where the infusion needles are arranged with great lateral distance between each other, the direction of lateral displacement of the tip ends of the infusion needles within each of the two different penetration areas may generally be the same as the direction of distance between the different penetration areas.

- 35 It is likewise possible to provide the tip end of a single infusion needle within the first housing and to implant the first housing within the patient's body adjacent the two or more injection areas. In this case, the drive unit may be configured so as to laterally displace the tip end of the one infusion needle between various lateral

positions such that the infusion needle can penetrate the first housing's outer wall in the different penetration areas. The distance of lateral displacement of the single infusion needle between the different penetration areas would amount to 3 mm, 4 mm, 5 mm or even more upon each successive injection. Such successive
5 injections are preferably in immediate time succession, preferably not exceeding 120 seconds between two injections, more preferably not exceeding 60 seconds. Most preferably, the drive unit will be adapted to initiate advancement of the one infusion needle to a second one of the plurality of penetration areas once it has been retracted from a first one of the penetration areas.

10

An implantable infusion device comprising a single, laterally displaceable infusion needle contained within a housing so as to penetrate the housing's outer wall at different penetration sites is generally known from previously mentioned WO 2007/051563. However, this prior art device is neither intended nor configured for
15 injecting drugs simultaneously or quasi-simultaneously in immediate time succession in two or more different injection areas. The drive unit of the prior art device is instead configured to administer the drug at a different penetration site of a single injection area at each time of operation. For instance, the prior art device may be placed along a blood vessel so as to inject drugs at different injection sites
20 within a single injection area of the blood vessel. Thus, the distance of lateral displacement of the tip end of the infusion needle between one injection and a next following injection is not configured in the prior art device such that different injection areas within the patient's body could be reached. Also, the prior art infusion device is not aimed at being used for the stimulation of penis erection. In
25 addition, in the prior art infusion device the entire infusion needle is accommodated in the housing which is to be implanted next to the constrained injection area, thereby requiring that the drive unit for advancing and retracting the tip end of the infusion needle is also implanted in the same constrained area.

30 Turning back to the present invention, it is again preferable, when the patient desires to perform another injection at a later point of time, that the single infusion needle does not penetrate the same penetration site within the particular penetration area of the housing's outer wall, but that the drive unit is configured to laterally displace the tip end of the one infusion needle to different penetration
35 sites within each of the different penetration areas. Again, the direction of lateral displacement of the tip end of the one infusion needle within each of the different

penetration areas may either be the same as the direction of lateral displacement of the tip end of the infusion needle between the different penetration areas, or may be different from, in particular perpendicular to, the direction of lateral displacement of the tip end of the infusion needle between the different

5 penetration areas. Depending upon the particular configuration of the system, this may be achieved with a single, multifunctional drive unit or with a plurality of different drive units suitably arranged to work in coordinated fashion. Even a combination of these alternatives is possible. For instance, when after a number of infusion cycles an infusion needle has laterally returned to its initial position, the

10 next number of infusions within the same penetration area may take place somewhat laterally offset above or below the first number of penetration sites. Thus, a two-dimensional array of penetration sites can be obtained in each penetration area, thereby keeping the maximum dimensions of the penetration areas at a minimum.

15 Where the first housing or at least the window area thereof is formed spherically, even a three-dimensional array of penetration sites through the first housing's outer wall can be obtained by means of a suitably adapted drive unit for the needle displacement. This greatly increases the system's flexibility of use.

20 Regardless of the number of needles involved and regardless of the particular penetration site array to be achieved, it is preferable to configure the drive unit such that the lateral displacement of the tip end of the infusion needle or needles is achieved automatically during advancement and/or retraction of the tip end of the needle or needles. For instance, where the infusion needle is mounted on a

25 movable carriage for the lateral displacement of the tip end of the needle, such as on a turntable or a shuttle, e.g. in the form of a slide, the drive unit may comprise a stepper which is adapted to automatically advance the movable carriage a predefined distance upon each advancement and/or retraction of the infusion needle.

30

Now, turning to the reservoir, it should be considered that long term storage is not possible with many currently available drugs, this being particularly true of drugs stimulating penis erection. Where long term storage is desired, the drug to be injected would typically be provided as a first substance and mixed with a second

35 substance for injection shortly before the injection is performed. Therefore, according to a preferred embodiment of the present invention, the reservoir of the

- system comprises at least one first compartment, e.g. for accommodating an infusion liquid such as a saline solution, and at least one second compartment, e.g. containing a drug, in particular a drug in dry form, for mixing with the infusion liquid of the first compartment. The drug may be in powder form and, more specifically, may be a freeze-dried drug. In particular, the drug contained in the second compartment would be a drug for stimulating penis erection. A mixing chamber may be provided for mixing the substance from the first compartment with the substance from one or more of the at least one second compartment.
- 10 The number of the second compartments may be huge, such as 50 or more, in particular 100 or more. This would not constitute a particular problem in terms of space constraints since the amount of drugs required for each stimulation of penis erection is extremely little and would amount to a few micrograms. Furthermore, the reservoir may be adapted for implantation within the patient's body remote from the housing containing the needle, such as close to the symphyseal bone. There is a lot of space available above the patient's symphyseal bone, and the drugs could be delivered to the tip end of the needle through an appropriate conduit. If desired, one can inject pure saline solution after the drug injection has been completed so as to clean the conduit and needle from any drug residue.
- 15 20 Such cleaning injection could be done through a different penetration area of the housing's outer wall into tissue of the patient which would not affect penis stimulation.
- Preferably, the second compartments containing the drug are liquid-tightly sealed against the first compartment, with a mechanism being provided for individually opening a connection between the second compartments and the first compartment.
- 25 According to a preferred embodiment, the second compartments are mounted in a plate so as to open towards a first side of the plate and the opening mechanism is adapted to act on the second compartments from a second side of the plate opposite the first side of the plate so that the compartments open to the first side of the plate. Thus, the second compartments may be pushed from their rear side (second side of the plate) so as to open frontward into e.g. a mixing chamber in which the content of the opened second compartments mixes with the content of the first compartment of the reservoir, such as with saline solution. More
- 30 35

specifically, the second compartments may be mounted in the plate as displaceable drug containers and the opening mechanism may be adapted to displace the drug containers such that they deliver their drug contents in the manner described.

5

Alternatively, the plate may be rotatable so as to allow the drug containers to be brought into alignment with a conduit upon rotation of the plate. Thus, when the drug is brought into alignment with such conduit, it may be mixed with e.g. saline solution pumped through the conduit towards the infusion needle.

10

According to another preferred embodiment, the second compartments are mounted on a tape wound up on a reel. A plurality of rows of the second compartments may be arranged on the tape in side-by-side relationship in a direction different to the winding direction of the tape. This way, the length of the tape can be reduced. It is particularly preferable if the tape is contained in a replaceable cassette. Thus, when all of the second compartments of the tape are emptied, the tape can be easily replaced by replacing the cassette.

15

As mentioned above, while the reservoir may generally be part of the housing accommodating the at least one infusion needle, it is preferred to arrange the reservoir separate from the housing for remote implantation within the patient's body.

20

At least a section of a periphery of the first compartment of the reservoir may be made from a flexible material permitting volume changes of the first compartment by deformation of the flexible material as infusion liquid is filled into or drawn out of the reservoir. Thus, the reservoir may be of balloon type. The flexible material may comprise a polymer membrane. A bellows construction is preferable having pre-bent creases to reduce long term degradation.

25

30

According to a particular embodiment, drawing liquid from the reservoir may cause a pressure decrease in at least part of the reservoir so that a negative pressure is attained as compared to the pressure in front of the infusion needle. For instance, the first compartment of the reservoir may comprise a gas chamber and a liquid chamber, said chambers being separated by a membrane, e.g. the polymer

35

membrane. When liquid is drawn from the liquid chamber, the pressure in the gas chamber will decrease accordingly.

5 The reservoir may have an injection port for injecting liquid from outside the human body into the implanted reservoir. That way, the reservoir implanted in the patient's body along with the infusion device may be kept relatively small since the reservoir can be refilled easily at appropriate time intervals, possibly with a doctor's aid.

10 Preferably, the injection port comprises a self-sealing material in respect of penetrations caused by a replenishing syringe that would be typically used to refill the reservoir through the patient's skin. It is preferable to implant the self-sealing injection port of the reservoir subcutaneously in the patient's body so that it is easily accessible for refill by means of the syringe.

15 While it has already been pointed out that drugs, in particular the drugs for stimulating penis erection, may degrade upon long term storage, another important influence on drug degradation is the storage temperature. Some drugs have to be stored in a refrigerator at low or at least moderate temperature. A
20 preferred embodiment of the invention therefore provides for a cooling device for keeping the content within at least one compartment of the reservoir at a temperature below 37°C. This can be achieved with relatively little energy supply if the amount of drugs to be cooled is extremely little, as explained above, and if furthermore the drug compartment within the reservoir is thermally insulated. For
25 instance, the reservoir may be comprised in an insulation chamber.

It is preferred to provide the cooling device with a heat exchanger for exchanging with the patient's body heat generated by the cooling device. Such heat exchanger may be implanted within the patient's body remote from the cooling device to
30 safely dissipate the heat energy in an area where it cannot adversely affect the content of the reservoir.

The cooling device can be of a variety of different types. According to a first embodiment, the cooling device may contain at least two different chemicals
35 reacting with each other, thereby consuming thermal energy which energy is drawn from the contents within the reservoir so that a cooling effect on the

contents is achieved. The two chemicals may be provided in separate chambers and a flow control device may be provided to bring together certain amounts of the two different chemicals so as to control the amount of thermal energy drawn from the contents within the reservoir.

5

According to a second embodiment, the cooling device may comprise at least one Peltier element. A Peltier element is an electrothermal converter causing a temperature difference to occur when an electric current is flowing through the element, based on the Peltier effect. While one part of the Peltier element cools
10 down, a different part thereof heats up. Such heat may again be removed by means of a heat exchanger or simply by providing the particular part generating the heat with an enlarged surface so that the heat is directly dissipated into the adjacent body part of the patient.

15 According to a third embodiment, the cooling device may be of a refrigerator-type construction. That is, heat exchanging pipes within a chamber to be cooled and heat exchanging pipes outside the chamber for dissipating the heat energy absorbed in the cooling chamber are provided along with a compressor for compressing the refrigerant gas when it exits the cooling chamber and an
20 expansion valve for expanding the refrigerant gas before it re-enters the cooling chamber.

Turning now to the pump for advancing the infusion liquid from the reservoir to the infusion needle or needles, such pump may be a manually driven pump or an
25 automatically driven pump. The manually driven pump may be formed from a balloon which may be manually compressed if suitably arranged under the patient's skin. The balloon type pump may at the same time serve as a reservoir for the infusion liquid, in particular for the saline solution. Preferably, however, an automatically driven pump is used. While the type of pump is not critical, one
30 specific type of pump is particularly preferred. More particularly, an implantable pump preferably comprises a valve device having a first and a second valve member, each having a smooth surface facing each other so as to form a sealing contact between the first and second valve members and further having different liquid channels that can be brought into alignment by displacement of the two
35 smooth surfaces relative to one another while maintaining the sealing contact. This type of pump is described in great detail in WO 2004/012806 A1. The first

and second valve members are preferably made from a ceramic material for its excellent sealing capabilities over a long period of time and its inertness to many substances.

- 5 The pump may be a membrane type pump, as also described in WO 2004/012806 A1, but is not restricted to this type of pump. The membrane type pump may comprise a membrane displaceable by a piston as the piston moves, the piston being coupled to the valve device so as to slidably displace the first and second valve members relative to one another as the piston moves. Preferably, the pump
10 will be implanted separate from the housing accommodating the needle or needles for remote implantation within the patient's body.

- Due to the space constraints within the patient's body in the area where injection is to take place, it is advantageous to implant as many components of the system as
15 possible remote from the first housing accommodating the tip end of the infusion needle or needles. In this context, the drive unit may comprise a mechanical drive for transmitting kinetic energy from a remote location within the patient's body to the at least one infusion needle. The mechanical drive element may comprise a rotating shaft by which a considerable distance can be bridged within the patient's
20 body. The rotating shaft may, upon rotation about its axis of rotation, cause movement of the infusion needle either directly or indirectly. More specifically, the rotating shaft may be in the form of a worm screw which, when turned, causes the infusion needle or needles to advance and retract and/or causes the infusion needle or needles to move laterally upon each advancement/retraction. Individual
25 rotating shafts or worm screws may be provided for each individual infusion needle and/or for advancing and retracting the tip end of the infusion needle or needles on the one hand and laterally displacing the tip end of the infusion needle or needles on the other hand. Most preferably, the rotating shaft or worm screw is flexibly bendable, so that it can be freely arranged within the patient's body.

- 30 Alternatively or in addition, the drive unit may comprise at least one wire directly or indirectly cooperating with the infusion needle so as to cause movement of the infusion needle upon actuation of the wire. Thus, the wire may be pulled at one end thereof which is located within the patient's body remote from the injection
35 sites. Preferably, the wire extends through the same conduit which connects the infusion needle or needles with the reservoir. More specifically, pulling the wire

may cause the tip end of the infusion needle or needles to displace laterally from a first to a second of the different penetration areas or from a first penetration site to a second penetration site within a single one of the different penetration areas. A single pulling wire may be sufficient to cause movement of the infusion needle in one direction, whereas a spring element or any other pretensioning means may be provided to urge the infusion needle back to the initial starting position or to a different starting position. Alternatively, two pulling wires may be provided to move the infusion needle back and forth in a single dimension.

According to a preferred embodiment, the tip end of the at least one infusion needle is arranged for two-dimensional lateral displacement. This can be achieved by means of two pulling wires, preferably cooperating again with spring elements or other pretensioning means to provide a counterforce to be overcome by pulling the wires. Alternatively, three pulling wires may be provided to laterally displace the tip end of the infusion needle back and forth along at least two directions within a two-dimensional plane.

A pulling wire may also be arranged to advance or retract the infusion needle by pulling the wire. Again, a spring element or other pretensioning means may be provided to urge the infusion needle back to its initial starting position or to a different starting position.

Alternatively, the drive unit may comprise a hydraulic drive for transmitting hydraulic energy to the at least one infusion needle for advancing the tip end thereof and/or for laterally displacing the tip end thereof. The infusion liquid itself may be used as the hydraulic medium providing the hydraulic energy, or a secondary liquid different from the infusion liquid may be used.

Further alternatively, the drive unit may comprise one or more electric motors preferably inside the second housing accommodating the respective other end of the at least one infusion needle. In this case, energy may be transmitted from a remote location within the patient's body to the at least one motor by means of appropriate wiring. Again, as in the two afore-described alternatives, a single motor may be provided for advancing and retracting the tip end of the infusion needle or needles and for laterally displacing the tip end of the infusion needle or needles, or individual motors may be provided for each individual infusion needle

and/or for advancing the tip ends of the infusion needle or needles on the one hand and laterally displacing the infusion needle or needles on the other hand.

Even further alternatively, the drive unit may comprise an electromagnetic drive for
5 laterally displacing and/or for advancing and retracting the tip end of the infusion
needle or needles. For instance, the electromagnetic drive may comprise a group
of electromagnets composed of a plurality of laterally spaced apart electromagnet
first parts and at least one electromagnet second part, the electromagnet second
10 part cooperating with an energized one of the electromagnet first parts. The
electromagnet second part is fixedly connected to the infusion needle or needles
either directly or indirectly so that upon energization of one or more of the
electromagnet first parts the electromagnet second part and, thus, the infusion
15 needle or needles will be caused to move. The arrangement of the electromagnet
first parts and second part may be such that the electromagnet first parts are
arranged in a first plane and the electromagnet second part is movable in front of
or behind the first plane. Alternatively, the electromagnet first parts may face each
other, thereby defining a first plane between them, and the electromagnet second
20 part may be movable within the first plane. Depending on which one or ones of the
electromagnet first parts are energized, the electromagnet second part with the
infusion needle or needles fixed thereto will move accordingly. The electromagnet
first parts preferably each include a magnetic coil.

In either one of the aforementioned alternatives, it is advantageous to transmit the
driving energy through the conduit that connects the first and second housings.
25 That is, in the case of a mechanical drive element in the form of a wire or rotating
shaft, the wire/shaft and the infusion liquid may be guided through a common
conduit. The common conduit may comprise two separate paths, one for the shaft
or wire and one for the at least one infusion needle. Such a common conduit
facilitates the handling and arrangement of the system during implantation.
30 Similarly, the wiring for transmitting electric energy to the motor or to the
electromagnetic drive may be guided through a conduit connecting the infusion
needle or needles with the reservoir.

Where the pump and/or drive unit is not actuated manually, a drive in the form of a
35 motor may be arranged e.g. for electrically, magnetically or electromagnetically
actuating the pump and/or drive unit or for hydraulically actuating the pump and/or

- drive unit. The motor is preferably arranged for actuating either the pump or the drive unit, thereby causing simultaneous actuation of the other, e.g. the drive unit or the pump. A motor may also be provided for actuation of any other energy consuming part of the infusion device. More specifically, a plurality of motors may
- 5 be provided, e.g. an individual motor for each infusion needle and/or an individual motor for displacing the tip end of the infusion needle in a lateral direction on the one hand and for advancing the tip end of the infusion needle through the housing's outer wall on the other hand.
- 10 Again, for reasons of space constraints in the area of implantation of the first housing or housings accommodating the tip end or ends of the at least one infusion needle, it is advantageous to remotely implant the motor within the patient's body separate from the first housing, preferably close to or within the second housing. Again, actuating means may be provided for manual activation of
- 15 the motor or motors, such actuating means preferably being adapted for subcutaneous implantation.

The term "motor" according to the present invention includes anything that employs energy other than manual power and either automatically transforms

20 such energy into kinetic or hydraulic or another type of energy or directly uses such energy to activate the pump, drive unit and/or other part of the overall system. As such, it is possible that part of the drive unit also forms part of the motor, e.g. in the case of an electromagnetically actuated drive unit.

- 25 Coupling elements may be provided either for conductive or for wireless energy transfer from outside the patient's body to the motor. For instance, the motor may be arranged for being wirelessly driven by an external electromagnetic field.

- An energy source for providing energy to at least one of the pump, the drive unit
- 30 and the drive (motor) for driving the drive unit, and any other energy consuming part of the system may be provided. For instance, an external energy source for use outside the patient's body, such as a primary energy source or a battery, in particular a rechargeable battery, that may be mounted on the patient's skin, may be used to provide energy to the pump and/or drive unit and/or any other energy
- 35 consuming part of the system. The energy source may in particular be connected to the at least one motor for actuating these components. An external energy

source for wireless energy transfer may be adapted to create an external field, such as an electromagnetic field, magnetic field or electrical field, or create a wave signal, such as an electromagnetic wave or sound wave signal.

- 5 Where the energy is wirelessly transferred to the implanted components, a transforming device for transforming the wirelessly transferred energy into electric energy may be provided. Such transforming device is preferably adapted to be placed directly under the patient's skin so as to minimize the distance and the amount of tissue between the transforming device and the energy supply means
10 outside the patient's body.

- Instead of or in addition to an external energy source, the system may comprise an implantable energy source. While such implantable energy source may be part of or may be contained within the housing accommodating the infusion needle or
15 needles, it is preferred to provide the implantable energy source separate from the housing for remote implantation within the patient's body. Such implantable energy source preferably comprises energy storage means, such as a long-life battery or, more preferably, an accumulator. The accumulator has the advantage of being rechargeable. Preferably, the accumulator comprises a rechargeable battery
20 and/or a capacitor.

- Again, coupling elements for conductive or wireless energy transfer from a primary energy source outside the patient's body to the accumulator may be provided for charging the accumulator from outside the patient's body when the device is
25 implanted in the patient's body. Similarly, the accumulator may comprise coupling elements for conductive and/or wireless energy supply to the at least one motor of the infusion device.

- A feedback subsystem, which may be part of a control unit described below, can
30 advantageously be provided to wirelessly send feedback information relating to the energy to be stored in the energy storage means from inside the human body to the outside thereof. The feedback information is then used for adjusting the amount of wireless energy transmitted by the energy transmitter. Such feedback information may relate to an energy balance which is defined as the balance
35 between an amount of wireless energy received inside the human body and an amount of energy consumed by the at least one energy consuming part.

Alternatively, the feedback information may relate to an energy balance which is defined as the balance between a rate of wireless energy received inside the human body and a rate of energy consumed by the at least one energy consuming part.

5

Preferably, a control unit is provided for controlling an amount of infusion liquid to be administered through the at least one injection needle. A single command from the patient to the control unit, such as a single actuation of a press button or other type of switch, is sufficient for causing the control unit to control the injection of the
10 drugs at two different locations within the patient's body. The control unit may be provided for controlling at least one of the pump, the drive unit and the motor and any other energy consuming part of the system and, where the system includes an internal or external energy source, said energy source. Again, the control unit is preferably separate from the housing accommodating the infusion needle or
15 needles so as to be implantable within the patient's body. The control unit may be adjusted such that the appropriate amount of drugs will be administered at the appropriate time to the particular one of the injection sites. Automatic administration will substantially relieve the patient.

20 Preferably, the control unit has a data transfer port for data transfer between an external data processing device outside the patient's body and the control unit implanted in the patient's body, regardless of whether the control unit is contained in the housing accommodating the infusion needle or needles or whether it is implanted within the patient's body remote from said housing. The data transfer
25 port allows for monitoring the control unit to adapt the system to changing needs of the patient. Preferably, the data transfer port is a wireless transfer port for the data transfer, so as to provide easy data exchange between the control unit and the external data processing device, e.g. during a visit to the doctor. Most preferably, the control unit is programmable to further increase its adaption
30 flexibility. Instead of or in addition to the external data processing device, the control unit may comprise an external component for manual operation by the patient for setting into operation the control unit.

Apart from or as a part of the control unit, feedback may be provided on
35 parameters relevant for the treatment. Such parameters may be either physical parameters of the patient and/or process parameters of the system. For this

purpose, at least one feedback sensor is provided for detecting such parameters. For instance, the feedback sensor may be adapted to detect one or more parameters relating to any of the following: drug level, flow volume in blood vessel, pressure, electrical parameters, distension, distance, etc.

5

The feedback sensors may be connected to the control unit and the control unit may comprise a control program for controlling drug delivery in response to one or more signals from the feedback sensors. In addition or alternatively, feedback data may be transferred from the control unit to the external data processing device. Such feedback data may be useful for the doctor's diagnosis.

10

The penetration areas of the wall or walls of the first housing or housings within which the tip end of the infusion needle or needles are disposed may be arranged in the patient's body at various locations. For instance, they may be arranged adjacent the left and right corpora cavernosa and/or the two deep arteries running through the left and right corpora cavernosa and/or muscle tissue regulating blood flow through the patient's left and right corpora cavernosa and/or another kind of tissue in close proximity to the left and right corpora cavernosa.

15

20 A holder may be used to secure the corpora cavernosa to the first housing or housings so that the housing rests in place.

Other components of the system are preferably remotely implanted, such as adjacent the patient's symphyseal bone. As discussed above, some components of the system may be implanted subcutaneously. Subcutaneous implantation increases the possibilities of wireless energy and/or data transfer between the implanted and the extracorporal parts of the system. Also, refilling the reservoir through an injection port by means of a replenishing needle penetrating through the patient's skin is substantially facilitated when an injection port of the reservoir is implanted subcutaneously. In particular, the compartment of the reservoir containing the saline solution might need to be refilled frequently, whereas the other compartments comprising individual small doses of the drug would need no refill. It should be understood, however, that depending upon the circumstances any implantable component of the system may be placed in the abdomen or even in the thorax. Activating means for direct manual operation by the patient may also be provided to be implanted subcutaneously, e.g. for setting into operation one or

25

30

35

more of the aforementioned motors or for simply setting into operation the control unit of the system. Such activating means may be in the form of a subcutaneously implantable switch manually operable by the patient from outside the patient's body.

According to one aspect of the present invention, there is provided an at least partly
5 implantable system for injecting a substance into a patient's body, comprising at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one housing's outer wall in at least one penetration area, and at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of
10 the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein the at least one drive unit comprises a hydraulic drive for transmitting hydraulic energy to the at least one infusion needle.

According to another aspect of the present invention, there is provided an at least
15 partly implantable system for injecting a substance into a patient's body, comprising at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer wall in at least one penetration area, and at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip
20 end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein at least in the at least one penetration area the at least one housing's outer wall is made from a material which is self-sealing in respect of penetrations resulting from said at least one infusion needle.

25 According to still another aspect of the present invention, there is provided an at least partly implantable system for injecting a substance into a patient's body, comprising at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer

wall in at least one penetration area, and at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in

5 said at least one penetration area, wherein the at least one housing's outer wall comprises at least one flap in the at least one penetration area through which the tip end or ends of the at least one infusion needle can pass, said at least one flap being arranged to be pushed aside by the tip end or ends of the at least one infusion needle upon advancement of said at least one infusion needle.

- 10 According to yet another aspect of the present invention, there is provided an at least partly implantable system for injecting a substance into a patient's body, comprising at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer wall in at least one penetration area, and at least one drive unit adapted for being
- 15 coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein the at least one housing's outer wall comprises at least one door in the at least one penetration area, wherein a drive is
- 20 connected to the at least one door for actively opening the at least one door so as to allow for the tip end or ends of the at least one infusion needle to be advanced through the opened at least one door.

- According to a further aspect of the present invention, there is provided an at least partly implantable system for injecting a substance into a patient's body, comprising
- 25 at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer wall in at least one penetration area, and at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle

penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, further comprising at least one reservoir adapted for implantation inside the patient's body in fluid connection with the at least one infusion needle to supply to the infusion needle the substance to be injected into the

5 patient's body.

According to yet a further aspect of the present invention, there is provided an at least partly implantable system for injecting a substance into a patient's body, comprising at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first

10 housing's outer wall in at least one penetration area, and at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein at least one feedback sensor

15 (F) is provided and adapted to sense at least one parameter out of the group comprising a) one or more physical parameters of the patient and b) one or more process parameters of the system.

The various aforementioned features of the invention may be combined in any way if such combination is not clearly contradictory. The invention will now be described in

20 more detail in respect of preferred embodiments and with reference to the accompanying drawings. Again, individual features of the various embodiments may be combined or exchanged unless such combination or exchange is clearly contradictory to the overall function of the device. In particular, while the following description of preferred embodiments specifically relates to the stimulation of penis

25 erection and, more specifically, to systems for the drug delivery at two or more different injection sites, it is to be understood that other uses, in particular with a single needle adapted for drug delivery at a single injection site, are also encompassed by this invention.

Brief Description of the Drawings

Figure 1 shows the muscles of the perineum,

Figure 2 shows a cross-section through the penis,

Figure 3 shows a first embodiment including a single long and flexible infusion
5 needle,

Figure 4 shows a second embodiment including a single infusion needle and a motor
accommodated in a common housing,

Figure 5 shows a third embodiment including the tip ends of two long and flexible
infusion needles in a common housing,

10 Figure 6 shows a plan view of a part of the infusion device of Figures 4 and 5,

Figure 7 shows a cross-sectional view through a penetration membrane made from a
composite material,

Figure 8 shows a cross-sectional view through the outer wall with flaps in the penetration area,

- 5 Figure 9 shows a cross-sectional view through the outer wall with an actively openable door in the penetration area,

Figure 10 shows a cross-sectional view through the outer wall with an actively openable door according to another embodiment,

10

Figure 11 shows a fourth embodiment including the tip ends of a plurality of infusion needles within a common housing,

- 15 Figure 12 shows a fifth embodiment comprising a single infusion needle, the tip end of which is laterally and vertically displaceable,

Figure 13 shows a sixth embodiment similar to the fifth embodiment, but with more steps for laterally displacing the tip end of the infusion needle,

- 20 Figure 14 shows a seventh, spherical embodiment for obtaining a three-dimensional array of penetration sites,

Figure 15 shows an eighth embodiment comprising the tip ends of two infusion needles in a common housing which are laterally and vertically displaceable,

25

Figure 16 shows a ninth embodiment with a principle of advancing and retracting an infusion needle by means of a pull wire,

- 30 Figure 17 shows a tenth embodiment with a principle of laterally displacing an infusion needle by means of pull wires,

Figure 18 shows an eleventh embodiment with a principle of advancing and retracting an infusion needle and laterally displacing an infusion needle by means of rotating shafts,

35

Figure 19 shows the overall system of the invention implanted in a patient's body according to a first variation,

5 Figure 20 shows the overall system of the invention implanted in the patient's body according to a second variation,

Figure 21 shows the overall system of the invention implanted in the patient's body according to a third variation,

10 Figure 22 shows drug compartments as part of the reservoir of the system according to a first principle,

15 Figure 23 shows drug compartments mounted on a tape wound on a reel in a replaceable cassette as part of the reservoir of the system according to a second principle,

Figure 24 shows a part of the tape of Figure 19 in greater detail,

20 Figure 25 shows the principle of operation of the replaceable cassette of Figure 23,

Figure 26 shows drug compartments as part of the reservoir of the system according to a third principle,

25 Figure 27 shows a cross-sectional view through the drug compartments of Figure 26 including an insulation chamber and cooling device,

Figure 28 shows the principle of the cooling device of Figure 27 in combination with a heat exchanger,

30 Figure 29 shows a specific embodiment for the cooling device of Figure 27,

Figure 30 shows a part of the system implanted in the patient's body comprising separate infusion needles for the right and the left corpus cavernosum,

35 Figure 31 diagrammatically shows the system of Figure 30,

Figure 32 shows a part of the system of Figure 31, including a tube into which the tip end of the infusion needle can be advanced,

- 5 Figures 33A to 33C show a first and second embodiment for electromagnetically displacing the tip end of the infusion needle in a plurality of lateral directions, and

Figures 34A and 34B show a third embodiment for electromagnetically displacing the tip end of the infusion needle in a plurality of lateral directions.

10

Detailed Description of the Drawings

- Figure 1 shows the muscles of the perineum of a male. Reference numerals 1, 2
15 and 3 designate the ischiocavernosus muscles, bulbospongiosus muscles and superficial transverse perineal muscles, respectively. The bulbospongiosus muscle surrounds lateral aspects of the bulb of the penis at the most proximal part of the body of the penis inserting into the perineal membrane, and further surrounds the dorsal aspect of the corpus spongiosum 4 surrounding the urethra 5 and the left
20 and right corpora cavernosa 6, 7. The ischiocavernosus 1 embraces the crus of the penis, inserting onto the inferior and medial aspects of the crus and to the perineal membrane medial to the crus. While the bulbospongiosus muscle assists the erection by compressing outflow via the deep perineal vein and by pushing blood from the bulb into the body of the penis, the ischiocavernosus muscle 1
25 maintains erection of the penis by compressing outflow veins and pushing blood from the root of the penis into the body of the penis. Figure 2 is a cross-sectional view through the penis. As can be seen, the penis is composed of three cylindrical bodies of erectile cavernous tissue: the paired corpora cavernosa 6, 7 dorsally and the single corpus spongiosum ventrally. Deep arteries 9, 10 run distally near the
30 center of the corpora cavernosa, supplying the erectile tissue in these structures. The deep arteries of the penis are the main vessels of the cavernous spaces in the erectile tissue of the corpora cavernosa and are therefore involved in the erection of the penis. They give off numerous branches that open directly into the cavernous spaces. When the penis is flaccid, these arteries are coiled, restricting
35 blood flow.

For reasons of simplification, the following figures only display the corpora cavernosa 6, 7. Figure 3 shows a part of the system according to a first embodiment. More specifically, a single long and flexibly bendable infusion needle 11 is arranged with its tip end 13 in a first housing 12, wherein the tip end 13 of the needle 11 is positioned such that it can be advanced and retracted through a self-sealing window area 14 in the housing's 12 outer wall 15 in a longitudinal direction 16, so as to pierce the corpus cavernosum 6 or 7 located adjacent the window area 14.

- Two window areas 14 are provided in the outer wall 15 of the first housing 12, one adjacent each of the two corpora cavernosa 6, 7. The infusion needle is displaceable in a lateral direction 17 between the two window areas 14 by means of a drive unit D. The same drive unit D or a different drive unit may cause the infusion needle 11 to be advanced and retracted. It is preferred that the drive unit for advancing and/or retracting the infusion needle, or at least the drive thereof, is disposed in a second housing which accommodates the respective other end of the infusion needle 11 and which is remotely implanted in the patient's body. For the purpose of enabling the tip end of the infusion needle to be advanced and retracted, the infusion needle 11 is mounted on a slide 18 for longitudinal movement. A conduit 19 is connected to the first housing 12 guiding the infusion needle 11 therein and, thus, protecting the infusion needle 11 against overgrowth with fibrosis. The conduit 19 continues to guide the infusion needle within the first housing up to the slide 18 and is fixed to the slide so as to perform the function of a Bowden cable system, i.e. preventing the front part of the infusion needle 11 from flexing away when the tip end 13 of the needle is advanced through the window area 14.

- In operation, the infusion needle 11 will first be advanced with the tip end 13 thereof to penetrate one of the two self-sealing penetration windows 14, injection fluid containing a drug for stimulation of penis erection will be injected into the corpus cavernosum 7 through the infusion needle 11 and, thereafter, the infusion needle 11 will be retracted again. Upon retraction of the infusion needle, the infusion needle will be laterally displaced along the direction 17 so that the tip end 13 thereof comes to lie in front of the other of the two self-sealing window areas 14, the infusion needle 11 will be advanced again so that infusion liquid can be injected through the tip end 13 thereof into the other corpus cavernosum 7 and

then the infusion needle 11 will be retracted again. At the end of this procedure, the infusion needle 11 will return to its initial position shown in Figure 3.

5 The structure of the system shown in Figure 3 may be purely mechanical. For instance, as will be described in more detail below, the pressure with which the infusion liquid is advanced through the needle 11 may in cooperation with spring elements cause the needle 11 to be advanced, retracted and laterally displaced to the other window area 14. Thus, after two pulses of injection fluid advanced through the conduit 19 towards the needle 11, the needle 11 will automatically
10 return to its starting position shown in Figure 3.

However, it is likewise possible to incorporate a motor M or a plurality of motors M within the first housing 12 in order to achieve the desired needle displacement by means of the drive unit D. This is schematically shown in Figure 4. Of course, the
15 motor M will have to be provided with energy and will need to be controlled in an appropriate manner so as to obtain the desired effect. This is not specifically shown in Figure 4. The energy is preferably transmitted to the motor M from an energy source either remotely implanted inside the patient's body or provided externally of the patient's body. The number and size of the motors M in the first
20 housing 12 should be kept at a minimum for reason of space constraints. Instead, the motors are preferably arranged remote from the first housing 12 in proximity to or within the afore-mentioned second housing.

The drive D may be configured such that after each penetration cycle (consisting
25 of two injections) the infusion needle 11 stops at a position different from the starting position so that the tip end 13 thereof penetrates the window areas 14 in the next following injection cycle at different sites as compared to the foregoing injection cycle.

30 Figure 5 shows a third embodiment which differs from the first and second embodiments in that it comprises two infusion needles 11 guided within a common sheath or conduit 19 up to the first housing's outer wall 15 and guided within the first housing in separate sheaths. Thus, when both infusion needles 11 are advanced and retracted simultaneously along the direction 16, injection of infusion
35 liquid occurs at exactly the same time. The drive unit D or a different drive unit may be used to turn the turntable 20 on which the tip ends of the infusion needles

11 are mounted, stepwise in the direction 17 so that the window areas 14 will be penetrated by the tip ends of the infusion needles 11 at different penetration sites during the next following injection cycle. Again, one or more motors M, not shown in Figure 5, may be used for driving one or more of the components of the drive
5 unit D.

The principle of a guide structure for laterally displacing the tip end of the infusion needle will now be described in context with Figure 6. Such guide structure may be used e.g. for each of the two infusion needles 11 shown in Figure 5 or may also be
10 used slightly modified for the lateral displacement of the infusion needle 11 shown in Figures 3 and 4.

The guide structure 28 is securely fixed adjacent the self-sealing window area 14 which itself is implanted adjacent the patient's corpus cavernosum 7. The guide
15 structure 28 comprises a guide pin 27 securely connected to the tip end of the infusion needle 11 (not shown) such that the infusion needle 11 cooperates with the guide structure 28. Upon advancement or retraction of the infusion needle 11, the guide pin 27 will be guided in the guide structure 28 and thereby laterally
20 displace the tip end of the infusion needle 11, which lateral displacement causes rotation of the turntable 20 (not shown in Figure 6). Resilient flaps 28a, 28b within the guide structure 28 serve to guide the guide pin 27 through the entire guide structure 28 upon repeated advancement and retraction of the infusion needle 11. The guide structure 28 is designed to provide different penetration sites through the self-sealing window area 14 into the corpus cavernosum 7. Where it is desired,
25 the trajectory of guide structure 28 may include a return path 28c for the guide pin 27 to return to its starting position shown in Figure 6. Such return action will be caused by a return spring 29 which is permanently fixed to a rigid part of the first housing.

30 The same structure can likewise be used in the embodiments shown in Figures 3 and 4 to displace the tip end of the single infusion needle 11 laterally between the two window areas 14. Of course, the structure would have to be slightly adapted to accommodate for the larger distance to be overcome between the two window areas 14.

35

Figure 7 shows a preferred embodiment of a penetration membrane to be used as the self-sealing window area 14 in the outer wall 15 of the housing 12. The penetration membrane 30 is made from a composite material. The same material can also be used for other flexible wall portions or for an infusion port that will be described below in connection with another embodiment. The composite material of penetration membrane 30 shown in Figure 7 comprises an outer shape-giving layer 30a defining a volume in which a self-sealing soft material 30b is contained. Self-sealing soft material 30b can be of gel type having a viscosity such that it does not flow through any penetrations caused by the infusion needle 11 during penetration of the outer shape-giving layer 30a. Instead of a single outer shape-giving layer 30a, the shape-giving layer 30a may comprise a plurality of layers. The outer shape-giving layer 30a preferably comprises silicone and/or polyurethane, since such materials can be produced to have self-sealing properties in respect of penetrations resulting from the infusion needle 11.

Instead of a self-sealing membrane, the window area 14 in the outer wall 15 of the housing 12 may be formed by one or more flaps, as shown in Figure 8. Two flaps 30' being made from a resilient, biocompatible material are arranged so as to form a slit which is normally closed and through which the infusion needle 11 can pass when it is advanced. Upon advancement of the infusion needle 11, the needle's tip end will push aside the normally closed flaps 30', and when the needle 11 is retracted again, the flaps 30' will return to their normally closed position so as to form a seal against ingress of body liquid.

Figure 9 shows a different embodiment. In this case, the self-sealing window 14 in the outer wall 15 comprises a door 30" which can be opened by mechanical action. In the embodiment shown, the door is formed by a flap made from a resilient, biocompatible material which keeps the window area 14 closed in its normal position. A pull wire 300 is attached to one end of the door 30" in order to allow for opening the door by pulling the pull wire 300. The pull wire 300 or any other drive connected to the door 30" forms part of the drive unit coupled to the front part of the infusion needle 11. For instance, as is shown in Figure 10, the pull wire 300 may be attached directly to the infusion needle 11 so that advancement of the infusion needle 11 will simultaneously cause the door 30" to be lifted up so that the infusion needle 11 can pass underneath the door 30" and, thus, penetrate the outer wall 15 easily. Due to the resiliency of the door material, the door 30" will

automatically close when the force, such as the pulling force exerted via the pull wire 300, is released. Instead or in addition, the closing action may be supported by at least one spring element urging the door into its closed position.

- 5 Figure 11 shows a fourth embodiment comprising a plurality of infusion needles for each of the two window areas 14. In this embodiment it is not necessary to provide a turntable by which the needles can be pivoted stepwise in order to laterally displace the needles from one penetration site to a different penetration site within the same window area 14. Instead, upon successive injection cycles a different
- 10 one of the plurality of injection needles will be advanced and retracted for each of the two window areas 14. Thus, the effect achieved is the same as in the embodiment shown in Figure 5.

- Figure 12 shows a fifth embodiment which differs from the first and second
- 15 embodiments shown in Figures 3 and 4 in that the tip end of the single infusion needle 11 is not only laterally displaceable in the direction 17 between the two window areas 14 but also laterally displaceable between different penetration sites 21 within the same penetration area 14. More specifically, the direction of lateral displacement of the tip end of the infusion needle 11 within each of said different
- 20 penetration areas 14 is perpendicular to the direction of lateral displacement between the different penetration areas 14. To achieve this result, the drive unit D is configured to longitudinally advance and retract the infusion needle 11 along a direction 16, to pivot the tip end of the infusion needle 11 by means of a turntable 20 between the two penetration areas 14 along a pivoting direction 17 and to raise
- 25 or lower the tip end of the infusion needle 11 along a third direction 22 perpendicular to the longitudinal direction 16. A suitable purely mechanical construction may perform this function. However, one or more motors may also be provided to perform one and/or the other of these functions. The motor or motors and, in particular, the drive unit for advancing and retracting the infusion needle
- 30 are preferably provided remote from the first housing, as already mentioned previously.

- Figure 13 shows a sixth embodiment similar to the fifth embodiment shown in Figure 12. In contrast to Figure 12, the tip end of the infusion needle 11 is not only
- 35 laterally displaceable between different penetration sites 21 within the same penetration area 14 in a direction perpendicular to the direction of lateral

displacement between the two penetration areas 14, but is also laterally displaceable within the same penetration area 14 in a direction parallel to the direction of lateral displacement between the different penetration areas 14. In other words, the tip end of the infusion needle 11 is laterally displaceable in two dimensions within the same penetration area 14.

Figure 14 shows a seventh embodiment which enables the tip end of the infusion needle 11 to be moved along a three-dimensional, spherically curved array of penetration sites. In this embodiment, a part of the first housing 12, more specifically the window area 14, is spherically curved and the front part of the infusion needle 11 is mounted in a sphere so that upon rotation of the sphere along the directions 17a and 17b the tip end 13 of the needle 11 can be moved to any position in front of the window area 14. Once an appropriate position has been adjusted for the tip end 13, the needle 11 can be advanced on the slide 18 so as to penetrate the window area 14. Instead of accommodating the slide inside the sphere, it may likewise be mounted on the outer surface of the sphere. Similarly, the infusion needle 11 itself can be mounted on the outer surface of the sphere. The mechanism for moving the sphere along the directions 17a, 17b can be of many different types, such as mechanical by means of rollers or magnetic.

Figure 15 shows an eighth embodiment similar to the third embodiment shown in Figure 5. That is, tip ends of two needles 11 are provided in a common first housing so as to be longitudinally movable in order to advance and retract the tip ends through the penetration areas 14. Instead of mounting the front part of the infusion needles 11 on a turntable 20, as in the embodiment of Figure 5, so as to change the injection sites 22 within a penetration area 14 upon each injection cycle, the eighth embodiment of Figure 15 achieves the same result by raising and lowering the tip ends of the two injection needles along a direction 22, similar to the fifth embodiment described above in relation to Figure 12. Again, the result is that the direction of lateral displacement of the tip ends of the two infusion needles 11 within each of the two different penetration areas 14 is perpendicular to the direction of distance between the two different penetration areas 14. Of course, this embodiment, like the sixth embodiment shown in Figure 13, can also be modified such that the tip ends of the two infusion needles 11 are laterally displaceable in two dimensions within the same penetration area 14.

Figure 16 shows a ninth embodiment with a principle of advancing and retracting the infusion needle 11 by means of a pull wire 101. The pull wire 101 is redirected about a pin 102 such that by pulling the wire 101 at an end remotely located somewhere in the patient's body the tip end of the infusion needle 11 will be
5 advanced through the window of the housing 12. A helical spring provides a counterforce so that the infusion needle 11 will be retracted once the pulling force on the pull wire 101 is released. This principle can be combined with other embodiments described hereinbefore and hereinafter. Instead of the helical spring 104, a second pull wire may be provided to retract the infusion needle 11. It
10 even possible to use a single pull wire 101 running around two pins 102 in a loop, so that pulling the wire 101 in the one direction or in the other direction will cause advancement or retraction of the infusion needle 11.

The pull wire 101 and the infusion needle are guided in a common sheath 103.
15 The common sheath 103 has various functions. First, it gives support to the pull wire 101 in bending sections. Second, it facilitates implantation of the infusion needle 11 along with the pull wire 101. Third, it protects the pull wire 101 against any build-up of fibrosis.

20 Figure 17 shows a tenth embodiment which involves remotely actuated pull wires 105, 106 guided within a common sheath 103 along with the infusion needle 11. The pull wires 105 and 106 are directly attached to the front end of the infusion needle 11 on opposite sides thereof so that the tip end of the infusion needle 11 which is mounted on a turntable 20 will be laterally displaced in the one direction
25 or in the other direction depending on whether the wire 105 or the wire 106 is pulled. Instead of using two wires 105, 106, one of the wires may be replaced with a pretensioning means, such as the helical spring 104 in Figure 16. In addition, a further wire, in particular third wire (not shown), may be provided for lateral displacement of the infusion needle 11 in a further direction, so that a two-
30 dimensional lateral displacement can be achieved by pulling the appropriate wires. In particular, due to the fact that the infusion needle 11 is long and flexibly bendable, one can dispense with the turntable 20 and achieve accurate lateral displacement of the tip end of the infusion needle 11 by pulling the appropriate one of three pull wires which are attached either directly or indirectly to the
35 circumference of the front end of the infusion needle at regularly spaced intervals.

The pull wires may alternatively be attached to an element other than the infusion needle 11, provided that the infusion needle 11 is connected to such other element, so that when the other element is moved or turned by pulling one or more of the wires the tip end of the infusion needle 11 will be displaced accordingly.

Figure 18 shows an eleventh embodiment with a different principle of advancing and retracting the tip end of the infusion needle, on the one hand, and laterally displacing the tip end of the infusion needle 11, on the other hand. Instead of pull wires, rotating shafts 107, 108 are provided. The drive for driving the rotating shafts 107, 108 is remotely located somewhere in the patient's body. The front ends of the rotating shafts have a threading 109, 110, e.g. in the form of a worm screw, meshing with the teeth of a rack 111, 112 formed either directly or indirectly on the infusion needle 11 and on the turntable 20, respectively. Thus, by turning the rotating shaft 107, the infusion needle 11 will advance or retract, as the case may be, due to the cooperation of the worm screw 109 and the rack 111. The gearing 109, 111 may likewise be arranged remote from the first housing, i.e. within the second housing accommodating the respective other end of the needle. Similarly, by turning the rotating shaft 108, the infusion needle 11 will be displaced laterally in the one or the other direction due to the cooperation of the worm screw 110 and the rack 112 of the turntable 20. Again, the rotating shafts 107, 108 are guided in a common sheath 103 along with the infusion needle 11.

In Figures 17 and 18, the action of the pull wires 105, 106 and the rotating shaft 108 make it possible to laterally displace the tip end of the infusion needle 11 between two different penetration areas and/or from a first penetration site to a second penetration site within a single penetration area.

Figure 19 shows a first variation of an overall system comprising any one of the first to eleventh embodiment described above. Specifically shown in the variation shown in Figure 19 is a first housing 12 accommodating the tip end of a single infusion needle 11 and a drive unit D as described in relation to Figure 12. The housing 12 is implanted with its window areas 14 positioned adjacent the corpora cavernosa 6, 7, of which window areas 14 only one is shown in Figure 19. A motor M is contained in the housing 12 for driving the drive unit D. While the motor M in the housing 12 may be designed to move the front end of the infusion needle 11 in

all directions as indicated in Figure 19, it is possible and even preferable to cause advancement and retraction of the front end of the infusion needle by advancing and retracting the entire infusion needle from its rear end using an additional motor, so as to minimize the motor size in the housing 12 for reasons of space constraints in the injection area. The additional motor may be accommodated in a separate second housing – not shown in Figure 19 – along with the rear end of the infusion needle and possibly along with further components remotely implanted in the patient's body. The motor M within the housing 12 (and likewise the aforementioned additional motor) is controlled by means of a control unit C₂ constituting the implantable part of a control system which further comprises an external data processing device C₁ by which commands and any other kind of data can be sent to the control unit C₂. For instance, the external data processing device C₁ may be used to initiate an injection cycle from outside the patient's body, this being done wirelessly as indicated by arrow 23. The implanted control unit C₂ not only controls the motor M inside the housing 12 but also controls the energy supply from an accumulator A to the motor M inside the housing 12.

The external data processing device C₁ may likewise be used to program the implanted control unit C₂. Also, a data transfer port for transferring data between the external data processing device C₁ and the implanted control unit C₂ may be adapted to transfer data in both directions.

A feedback sensor F implanted inside the patient's penis is shown here as being connected to the motor M inside the housing 12 and may likewise be connected to the implantable control unit C₂. The feedback sensor F can sense one or more physical parameters of the patient, such as the drug level inside the corpora cavernosa, the flow volume through the corpora cavernosa, the pressure inside the corpora cavernosa and the like. Other feedback sensors may be provided at a different location so as to sense process parameters of the system, such as electrical parameters, distention, distance and the like.

The conduit 19 guides the infusion needle 11 from a reservoir comprising compartments R₁ and R₂ and accommodates the wiring 24 for transmitting electric energy from the energy source A to the motor M inside the housing 12.

35

In the variation of the entire system shown in Figure 19, the reservoir comprises a first compartment R_1 with e.g. a saline solution included therein, and a second compartment R_2 with e.g. a drug in powder form or freeze-dried form included therein. A pump P driven by a second motor M_2 is arranged to pump infusion liquid from the reservoir R_1 to the infusion needle 11. The infusion liquid pumped by the pump P will pass through a mixing chamber 26 into which drugs will be released from the reservoir R_2 in appropriate time coordination. The motor M_2 or a different motor may cause the drugs to be released from the second reservoir R_2 . The motor M_2 is also controlled by the control unit C_2 . Thus, infusion liquid pumped via the pump P from the relatively large first reservoir R_1 through the mixing chamber 26, in which it is mixed with the drugs released from the second reservoir R_2 , will reach the infusion needle 11 which has meanwhile penetrated the self-sealing window area 14 of the housing 12 and will flow into the corpus cavernosum 7.

In addition to or instead of the control unit C_2 , a pressure sensitive switch for activating the motor M inside the housing 12 and/or the motor M_2 may be arranged subcutaneously.

Although the embodiment shown in Figure 19 may comprise one of a great variety of reservoir types, a particular reservoir type will now be described. The volume of the reservoir R_1 is divided into two sections by means of a membrane 31. One section is filled with gas whereas the other section is filled with the infusion liquid (saline solution). An infusion port 32 allows for refilling the reservoir R_1 with infusion liquid by means of a replenishing needle. When the reservoir R_1 is in its full state, the gas section is at ambient pressure or over-pressurized. As infusion liquid is drawn from the reservoir R_1 by means of the pump P upon each infusion cycle, the pressure in the gas section will decrease below ambient pressure, i.e. to a negative relative value. Depending upon the particular type of pump P, it may be advantageous to provide a single acting ball valve to prevent any backflow from the pump P to the reservoir R_1 .

There are various ways of providing the motors M and M_2 with energy. In the variation shown in Figure 19, energy is supplied from outside the patient's body either for direct use by the motors and/or for charging the accumulator A, which may be in the form of a rechargeable battery and/or a capacitor. An extracorporal primary energy source E transmits energy of a first form through the patient's skin

100 to an energy transforming device T which transforms the energy of the first form into energy of a second form, such as electric energy. The electric energy is used to recharge the accumulator A which provides secondary energy to the motor M upon demand.

5

The external primary energy source E may be adapted to create an external field, such as an electromagnetic field, magnetic field or electrical field, or create a wave signal, such as an electromagnetic wave or sound wave signal. For instance, the energy transforming device T as shown in Figure 19 may act as a solar cell, but adapted to the particular type of wave signal of the primary energy source E. The energy transforming device T may also be adapted to transform temperature changes into electrical energy.

10

Instead of the external primary energy source E, an implantable primary energy source E may be used, such as a regular long-life battery instead of the accumulator A.

15

The energy signal may also be used to transmit signals from the external data processing device C₁ by appropriate modulation of the energy signal, regardless of whether the energy is transmitted wirelessly or by wire, the energy signal thereby serving as a carrier wave signal for the digital or analog control signal. More particularly, the control signal may be a frequency, phase and/or amplitude modulated signal.

20

Figure 20 shows a second variation of the entire system which basically differs from the system of Figure 19 only in that the motor M inside the housing 12 is dispensed with. Instead, the motor M₂ is used to drive the drive unit D. This is achieved by means of a rotating shaft 33 in the form of an elastically bendable worm screw, the rotating shaft 30 replacing the wiring 24 of the system shown in Figure 19. Alternatively, since the infusion needle 11 is long and flexible, the infusion needle may be advanced by engagement of two helical gears, one of which is formed on the rear end of the infusion needle, or by a similar gearing cooperating with the infusion needle's rear end.

30

Figure 21 shows a third variation of the entire system which operates purely mechanically. The reservoir R₁ containing the infusion liquid, i.e. the saline

35

solution, is of balloon type, thereby functioning both as a reservoir and as a pump if it is compressed manually from outside the patient's body. The pressure generated in the reservoir R_1 will act on the reservoir R_2 containing the drug. Upon a certain pressure, the drug will be released from the reservoir R_2 into the mixing
5 chamber 26 and upon further increase of the pressure the infusion liquid will be allowed to enter the mixing chamber 26, mix with the drug released from the reservoir R_2 , flow towards the infusion needle 11, and build up pressure on the infusion needle 11 such that the drive unit D is caused to advance the infusion
10 needle 11 through the self-sealing window area 14 into the patient's corpus cavernosum. Once the pressure is released, the infusion needle 11 will retract automatically due to mechanical spring forces or the like and move into a different position in which it can penetrate the second of the two self-sealing window areas 14 when the reservoir R_1 is compressed again. Where two infusion needles 11 are provided, a single compressing action on the reservoir R_1 would be sufficient to
15 inject the drug into both the left and right corpora cavernosa.

Figure 22 shows a first principle of how drugs within a plurality of compartments 34 of the reservoir R_2 can be released one at a time by a purely hydromechanical solution. As the infusion liquid is urged from the reservoir R_1 towards the conduit
20 25 leading to the infusion needle or needles, it is first blocked by a spring-loaded ball valve 34 which opens only when a certain pressure is exceeded. The pressure building up in front of the ball valve 34 is guided by means of a stepper valve V sequentially onto one of a plurality of compartments 35. The compartments are each formed as a cavity 35 within a piston 36. Once a certain pressure is
25 exceeded, the piston 36 will be pushed into a position where the compartment 35 is in flow communication with a mixing chamber 26. In the state shown in Figure 22, three pistons 36 have already been pushed into such position. When the pressure in the reservoir R_1 is further increased, the spring force of the ball valve 34 will be overcome and the infusion liquid urged from the reservoir R_1 towards the
30 conduit 25 will take with it the drug that has been released into the mixing chamber 26.

Figures 23 to 25 show a second principle of realizing the reservoir R_2 comprising a plurality of small drug compartments 35, 35a, 35b. The drug compartments are
35 integrally formed in a tape 201 which is wound on a first reel 202 and can be unwound from said first reel 202 onto a second reel 203. The reels 202, 203 and

the tape 201 are contained in a cassette 200 which may be inserted in the entire system so as to form part of the reservoir. The cassette 200 is preferably replaceable.

- 5 As can be seen in Figure 24, the compartments 35, 35a, 35b containing the drug e.g. in powder form or freeze-dried form are arranged in a plurality of rows as seen in the transporting direction (indicated by the arrow). However, the compartments 35 of one row are a certain distance offset in the transporting direction from the compartments 35a and 35b of the other rows. Thus, when the
- 10 tape 201 is wound from reel 202 to reel 203, it is guided through a conduit 204 forming part of the cassette 200 through which the infusion liquid is pumped from the reservoir R₁ to the infusion needle or needles, and the compartments 35, 35a, 35b will enter the conduit 204 one after the other.
- 15 While it is conceivable to open one of the compartments 35, 35a, 35b that has entered the conduit 204 by mechanical action, such as a hammer or piercing element, the opening of the compartments 35 in the embodiment shown in Figures 23 to 25 needs no further action other than winding the tape 201 onto the reel 203. That is, as can be seen from Figure 25, when the tape 201 enters the conduit 204
- 20 through a first slit 205, the compartments 35 will not be damaged due to the fact that the slit 205 is relatively wide and is closed by two soft sealing lips 206. However, when the tape 201 exits the conduit 204 on the other side thereof, it will have to pass a narrower second slit 207 with front edges 208 that are not resilient. The compartments 35 will therefore burst on their way out of the conduit 204 when
- 25 they slip between the edges 208 of the narrow slit 207. Soft seals 209 in the slit 207 prevent liquid from leaking from the conduit 204.

The entry 210 and the exit 211 of the conduit 204 within the cassette 200 each include a valve that automatically closes when the cassette 200 is removed from

30 the system and automatically opens when the cassette 200 is installed in the system. This allows for replacement of the cassette 200 without adversely affecting the remaining components of the overall system.

Figures 26 and 27 show a third principle of realizing the reservoir R₂ comprising a

35 plurality of small drug compartments 35. While Figure 26 shows a cross-sectional plan view according to section BB in Figure 27, Figure 27 shows a cross-sectional

side view thereof according to section AA in Figure 26. The compartments 35 containing the drug in powder form or freeze-dried form are arranged in a rotatable plate 37. A motor M_2 is provided to rotate the plate 37 about an axis 38. The motor M_2 is controlled to advance the plate 37 stepwise so as to bring one
5 compartment 35 at a time in line with the conduit 39 connecting the reservoir R_1 containing the saline solution with the infusion needle or needles. Energy is supplied to the motor M_2 from the accumulator A via the control unit C_1 .

The rotatable plate 37 is mounted in a fixed base plate 39 which itself is fixedly
10 mounted in a housing 40 insulating the base plate 39 and the rotatable plate 37 thermally against an outer housing 42. A cooling device 41 is provided to cool a liquid surrounding the base plate 39 and rotatable plate 37 down to a temperature below 37°C . This serves to protect the drugs inside the compartment 36 from degrading too quickly. The accumulator A supplies the cooling device 41 with
15 energy.

Figure 28 shows a general principle of cooling the reservoir R_2 containing the drug to be cooled. The cooling device 41 may be an electrothermal cooler, i.e. based on the Peltier effect consuming electric energy, or may be of the refrigerator type.
20 Accordingly, the cold part of the cooler 41 is placed on the side to be cooled whereas the warm part of the cooling device 41 is placed on the other side so that the heat energy can be dissipated to the outside. An increased surface 41a on the warm side of the cooling device 41 serves to increase heat dissipation. Furthermore, a heat exchanging fluid may be passed through a conduit 41b along
25 the increased surface 41a to transfer the dissipated heat energy to a remote location within the patient's body where the heat is dissipated into the patient's body through a specific heat exchanging surface 41c.

Figure 29 shows a different principle of cooling the drugs contained in the
30 reservoir R_2 . In this embodiment, two chemicals X1 and X2 are contained separate from each other in respective compartments of the cooling device 41. When the chemicals X1 and X2 are brought together, they will react with each other and such reaction will consume energy which is absorbed as thermal energy from the surroundings. By means of two pistons 41d, 41e, the chemicals X1, X2 are
35 dispensed into a cooling line 41f in a controlled manner, which cooling line is preferably in contact with the housing 40 containing the reservoir R_2 . The chemical

mixture X1-X2 displaced within the cooling line 41f will flow back into the chamber containing the chemicals X1, X2, but onto the other side of the pistons 41d, 41e.

5 A further embodiment is shown in Figure 30. In this embodiment, again, two separate long and flexible infusion needles 11 are provided with their respective front ends accommodated in a housing 12, one infusion needle for each of the left and right corpora cavernosa. However, unlike the previously discussed
10 embodiments, the two needles each have their own housing 12 implanted in the patient's body with their respective self-sealing window area 14 adjacent the left and right corpora cavernosa, respectively. This principle is shown in Figure 31 in more detail with respect to one of the two needles. The drive unit D comprises a piston 50, to which the hollow infusion needle 11 is attached. The piston 50 separates a first chamber 51a in front of the piston 50 and a second chamber 51b behind the piston 50. While the pressure in the first chamber 51a corresponds to
15 the pressure exerted by the pump P via the conduit 25, the pressure in the second chamber 51b can be kept at a lower value. The second chamber 51b may be filled with a liquid, such as the infusion liquid, and the liquid may be urged into a flexible volume 52. The flexible volume 52 could be of simple balloon type so as to fill up without exerting any strong counterforce.

20 Instead of the flexible volume 52, a conduit 53 may connect the second chamber 51b with the reservoir R₁. Thus, when the needle 11 is advanced, liquid will be dispelled from the second chamber 51b through the conduit 53 into the reservoir R₁, and as the needle 11 is retracted by means of a return spring 55, liquid will be
25 drawn from the reservoir R₁ through the conduit 53 back into the second chamber 51b.

The injection process is carried out as follows. As the pressure is increased in the first chamber 51a by means of the pump P remote from the housing 12
30 accommodating the tip end 13 of the infusion needle 11, the entire infusion needle 11 which is guided in the conduit 19 will be displaced against the force of the spring 55 of the drive unit B. Thus, the tip end 13 of the infusion needle 11 will penetrate through the self-sealing window area 14 press-fitted into the wall 15 of the housing 12 and will further penetrate any fibrosis having built up in front of the
35 housing. When the return spring 55 is completely compressed and the pressure built up by the pump P is further increased, a ball valve 56 will be displaced

against a second return spring 57 which is stronger than the first return spring 55. That way, as long as the pressure is held at a sufficiently high level, infusion liquid will be pumped from the reservoir R₁ through the conduit 25, the hollow infusion needle 11 and the needle's laterally arranged exit port into the patient's body.

- 5 Upon pressure release, the ball valve 56 will close due to the return springs 55 and 57, and then the needle 11 will be retracted to its initial position shown in Figure 22.

- 10 It may be advantageous not to pierce any living tissue by means of the injection needle 11 once it is advanced through the outer wall 15 of the housing 12. Therefore, as shown in Figure 32, a tube 58 may be placed in front of the window area 14. The cross-sectional form of the tube 58 may be adapted to the cross-sectional form of the window area 14, i.e. where the window area 14 is rectangular, the tube 58 likewise has a rectangular cross-section.

- 15 The exit end of the tube 58 has an open area 59 sufficiently large to prevent growth of fibrosis from spanning over the open area. Fibrosis will slowly grow into the tube along the tube's inner surface, before it reaches the window area 14 after a relatively long time. The tip end 13 of the needle 11 will therefore not have to
20 penetrate any fibrosis during the first while after implantation of the system. Preferably, the open area 59 has an opening width of at least 3 mm. The length of the tube 58 may be in the range of 4 mm to 30 mm. The opening width 59 and the length of the tube 58 should be adjusted such that the substance injected into the tube 58 can safely seep into the patient's body. Thus, the longer the tube is, the
25 larger the opening width thereof should be.

- Figures 33A and 33B show a first embodiment for displacing the tip end of the infusion needle 11 in two or more different directions, i.e. a two-dimensional displacement. More specifically, Figure 33A shows a plan view, whereas Figure
30 33B shows a side elevational view schematically. As can be seen, a plate 60 to which the infusion needle 11 is fixedly mounted has a projection 61 extending into a frame 62 within which the projection 61 is free to move in any direction. Electromagnetic coils 63 are mounted on the sides of the frame 62 and are individually energizable. The electromagnetic coils 63 constitute the first part of an
35 electromagnetic drive whereas the projection 61 is configured to constitute the second part of the electromagnetic drive. Thus, when one or more of the

electromagnetic coils are energized, an electromagnetic field is created in the frame 62 and the electromagnet second part, i.e. the projection 61, will adjust its position within such field accordingly. Due to the fact that the front end of the infusion needle 11 is fixedly mounted to the plate 60, the infusion needle 11 will
5 move along with the projection 61. This way, the tip end of the infusion needle 11 can be displaced laterally and can also be advanced and retracted.

More preferably, however, the infusion needle 11 is attached to the electromagnetic drive in a different manner, namely perpendicular to the plane
10 defined by the electromagnetic coils 63 (rather than in parallel as in Figure 33B). As a result, the tip end of the infusion needle will be displaceable in a plurality of lateral directions rather than being advanceable and retractable. The drive unit for advancing and retracting the infusion needle 11 is instead preferably connected to the rear end of the long and flexibly needle.

15 Alternatively, the electromagnetic drive may be such as to displace the tip end of the infusion needle in any lateral direction and, in addition, to advance and retract the infusion needle. This can be achieved e.g. with a structure as schematically shown in Figure 33C relating to a second embodiment for displacing the tip end of
20 the infusion needle 11. Figure 33C shows an elevational side view similar to Figure 33B, but the electromagnetic coils 63 do not define a single plane, but rather a plurality of planes is defined one above the other by providing additional electromagnetic coils 63 in a vertical direction. The top plan view would be similar to Figure 33A. This way, the electromagnet second part 61 fixedly connected to
25 the needle 11 moves within a three-dimensional frame 62 depending on the energization of respective ones of the magnetic coils 63.

Figure 34A and 34B shows a plan view and a side view of a third embodiment of an electromagnetic drive for moving the tip end of the infusion needle 11 in a
30 plurality of directions. In this embodiment, the electromagnetic coils 63 constituting the electromagnet first parts are arranged in a first plane and the electromagnet second part constituted by the protrusion 61 fixedly connected to the infusion needle 11 via the plate 60 is movable in a plane in front of or behind the plane defined by the electromagnet first parts. However, the electromagnetic coils 63 are
35 oriented differently in this third embodiment. Again, depending upon the energization of the individual electromagnetic coils, the electromagnet second

part, i.e. the protrusion 61, will adjust its position in the created electromagnetic field within the frame 62.

A method of treating a human being (or an animal) by implanting at least part of the system in the patient's body comprises the steps of cutting the skin, dissecting free a first area near the left and right corpus cavernosum, placing the at least one first housing accommodating the tip end or ends of the at least one infusion needle within said dissected area such that the tip end, when penetrating the housing's outer wall, can penetrate into the left and right corpus cavernosum and/or the two deep arteries of the right and left corpus cavernosum and/or into muscle tissue regulating blood flow to the patient's left and right corpus cavernosum and/or into another kind of tissue in close proximity to the patient's left and right corpus cavernosum allowing stimulation of erection of the two corpora cavernosa, placing at least one second housing accommodating the respective other end or ends of the at least one infusion needle within the patient's body remote from the at least one first housing, and finally closing at least the skin after implantation of at least parts of the system.

Where parts of the system are implanted remote from the corpora cavernosa, a second area remote from the first area may be dissected free in order to place e.g. the at least one reservoir in the patient's body at the remote second area, with a conduit connecting the reservoir with the rear end of the at least one infusion needle accommodated in the at least one second housing. In this case, it is preferable to place the second housing and/or the reservoir adjacent the patient's symphyseal bone.

One or more of the following elements may be placed within the patient's body remote from the housing or housings accommodating the at least one needle:

- at least one drive unit for advancing and retracting the tip end of the infusion needle,
- a reservoir for supplying to the infusion needle a substance to be injected into the patient's body,
- a pump (P) for advancing the substance from the reservoir to the at least one infusion needle,

- at least one motor (M, M₂) for actuation of the drive unit (D) or a drive driving the drive unit, and/or the pump (P) or any other energy consuming part of the system,
- energy storage means (A) for providing the at least one motor with energy,
- 5 - galvanic coupling elements between either an external energy source (E) or the energy storage means (A) and the motor (M, M₂) for transmitting energy to the motor in contacting fashion,
- wireless coupling elements adapted to connect either the motor (M, M₂) or the energy storage means (A) or both to an extracorporal primary energy
- 10 source for transmitting energy to either the motor or the energy storage means or both in non-contacting fashion,
- control unit (C1) for controlling the motor (M, M₂),
- a data transmission interface for wirelessly transmitting data from an external data processing device (C₂) to the control unit (C₁),
- 15 - the feedback sensor (F),
- wireless energy transforming means, and
- the injection port (32) for refilling the reservoir (R₁).

CLAIMS:

1. An at least partly implantable system for injecting a substance into a patient's body, comprising
at least one infusion needle with a tip end of each of said at least one
5 infusion needle arranged in at least one housing for penetrating the at least one housing's outer wall in at least one penetration area, and
at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or
10 ends thereof said at least one housing's outer wall in said at least one penetration area, wherein the at least one drive unit comprises a hydraulic drive for transmitting hydraulic energy to the at least one infusion needle.
2. The system according to claim 1, wherein the hydraulic drive transmits hydraulic energy to the at least one infusion needle for advancing the tip end of the at
15 least one infusion needle.
3. The system according to claim 1 or 2, wherein hydraulic fluid of the hydraulic drive is guided through a conduit connecting the at least one infusion needle with at least one reservoir.
4. The system according to claim 3, wherein the system is adapted to use
20 as the hydraulic fluid infusion liquid to be injected into the patient's body.
5. The system according to claim 3, wherein the system is adapted to use as the hydraulic fluid a secondary liquid different from an infusion liquid to be injected into the patient's body.
6. The system according to any one of claims 1 to 5, wherein the at least
25 one drive unit comprises as a drive at least one electric motor.

7. The system according to claim 6, further comprising wiring for transmitting electric energy from a remote location within the patient's body to the at least one electric motor.

8. The system according to claim 7, wherein the wiring is guided through a
5 conduit connecting the at least one infusion needle with the at least one reservoir.

9. The system according to any one of claims 1 to 8, wherein the at least one drive unit comprises an electromagnetic drive.

10. An at least partly implantable system for injecting a substance into a patient's body, comprising

10 at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer wall in at least one penetration area, and

at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one
15 infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein at least in the at least one penetration area the at least one housing's outer wall is made from a material which is self-sealing in respect of penetrations resulting from said at least one infusion needle.

20 11. The system according to claim 10, wherein the self-sealing material forms at least two window areas in said at least one housing's outer wall, said at least two window areas being positioned for penetration by the tip end or ends of the at least one infusion needle.

12. The system according to claim 10 or 11, wherein the self-sealing
25 material comprises a penetration membrane integrated in the at least one housing's outer wall.

13. The system according to claim 12, wherein the penetration membrane is sealingly press-fitted into the at least one housing's outer wall.

14. The system according to any one of claims 10 to 13, wherein the self-sealing material comprises at least one polymer selected from the group of materials
5 comprising silicon and polyurethane.

15. The system according to any one of claims 10 to 14, wherein the self-sealing material is made from a composite material.

16. The system according to claim 15, wherein the composite material comprises at least one outer shape-giving layer and a self-sealing soft material
10 contained within the outer layer.

17. The system according to claim 16, wherein the self-sealing soft material is a gel.

18. An at least partly implantable system for injecting a substance into a patient's body, comprising

15 at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer wall in at least one penetration area, and

at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one
20 infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein the at least one housing's outer wall comprises at least one flap in the at least one penetration area through which the tip end or ends of the at least one infusion needle can pass, said at least one flap being arranged to be pushed aside by
25 the tip end or ends of the at least one infusion needle upon advancement of said at least one infusion needle.

19. An at least partly implantable system for injecting a substance into a patient's body, comprising

at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first
5 housing's outer wall in at least one penetration area, and

at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration
10 area, wherein the at least one housing's outer wall comprises at least one door in the at least one penetration area, wherein a drive is connected to the at least one door for actively opening the at least one door so as to allow for the tip end or ends of the at least one infusion needle to be advanced through the opened at least one door.

20. The system according to claim 19, wherein the drive connected to the at
15 least one door forms part of the at least one drive unit coupled to the at least one infusion needle.

21. The system according to claim 19 or 20, wherein the at least one door comprises a normally closed, resilient flap.

22. The system according to any one of claims 19 to 21, comprising at least
20 one spring element urging the at least one door into its closed position.

23. An at least partly implantable system for injecting a substance into a patient's body, comprising

at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first
25 housing's outer wall in at least one penetration area, and

at least one drive unit adapted for being coupled to the at least one infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, further comprising at least one reservoir adapted for implantation inside the patient's body in fluid connection with the at least one infusion needle to supply to the infusion needle the substance to be injected into the patient's body.

5

10

24. The system according to claim 23, wherein the at least one reservoir is adapted for implantation inside the patient's body remote from the at least one first housing.

25. The system according to claim 24, wherein the at least one reservoir is contained in at least one second housing.

15

26. The system according to any one of claims 23 to 25, wherein the at least one reservoir has an injection port for refilling the at least one reservoir with infusion liquid.

27. The system according to claim 26, wherein the injection port comprises a material which is self-sealing in respect of penetrations caused by a replenishing needle.

20

28. The system according to claim 26 or 27, wherein the injection port is adapted for subcutaneous implantation.

29. The system according to any one of claims 26 to 28, wherein the at least one reservoir is adapted for implantation inside the patient's body remote from the at least one housing.

25

30. The system according to claim 29, comprising at least one conduit for connecting the at least one reservoir with the at least one infusion needle.

31. The system according to claim 30, wherein the at least one conduit has a length sufficient to bridge the distance between the patient's symphyseal bone and the inferior fascia of the patient's urogenital diaphragm.

5 32. The system according to claim 30, wherein the at least one conduit has a length of 10 cm or more.

33. The system according to any one of claims 29 to 32, wherein, where a plurality of infusion needles is provided, separate conduits are provided between each of the infusion needles and the at least one reservoir.

10 34. The system according to any one of claims 23 to 33, further comprising a cooling device for keeping the content within at least one compartment of the reservoir at a temperature below 37°C.

35. The system of claim 34, wherein the reservoir or the at least one compartment thereof is comprised in an insulation chamber.

15 36. The system according to claim 34 or 35, further comprising a heat exchanger for exchanging heat generated by the cooling device with the patient's body.

37. The system of claim 36, wherein the heat exchanger is adapted for implantation within the patient's body remote from the cooling device and is connected to the cooling device via fluid lines for conducting a heat exchange fluid.

20 38. The system according to any one of claims 34 to 37, wherein the cooling device contains at least two different chemicals reacting with each other, thereby consuming thermal energy.

25 39. The system according to claim 38, wherein the at least two chemicals are provided in separate chambers, the system further comprising a flow control device for bringing together certain amounts of the different chemicals.

40. The system according to any one of claims 34 to 39, wherein the cooling device comprises at least one Peltier element.
41. The system according to any one of claims 34 to 39, wherein the cooling device is of a refrigerator-type construction.
- 5 42. The system according to any one of claims 23 to 41, further comprising at least one pump adapted for implantation inside the patient's body to advance the substance from the at least one reservoir to the at least one infusion needle.
43. The system according to claim 42, wherein the at least one pump is adapted for implantation inside the patient's body remote from the at least one first
10 housing.
44. The system according to claim 39, wherein the at least one pump is contained in at least one second housing.
45. The system according to any one of claims 42 to 44, wherein the at least one pump is adapted for remote implantation within the patient's body separate
15 from the at least one first housing within which the tip end or ends of the at least one infusion needle is contained.
46. The system according to any one of claims 42 to 45, wherein actuating means are provided for direct manual operation of at least one out of the group comprising the at least one drive unit and the at least one pump.
- 20 47. The system according to claim 46, wherein the actuating means are arranged for directly actuating either the at least one pump or the at least one drive unit, thereby simultaneously indirectly actuating the other, i.e. the at least one drive unit or the at least one pump.
48. An at least partly implantable system for injecting a substance into a
25 patient's body, comprising

at least one infusion needle with a tip end of each of said at least one infusion needle arranged in at least one housing for penetrating the at least one first housing's outer wall in at least one penetration area, and

at least one drive unit adapted for being coupled to the at least one
5 infusion needle and arranged at least for advancing the tip end of the at least one infusion needle so that the at least one infusion needle penetrates with the tip end or ends thereof said at least one housing's outer wall in said at least one penetration area, wherein at least one feedback sensor (F) is provided and adapted to sense at
10 least one parameter out of the group comprising a) one or more physical parameters of the patient and b) one or more process parameters of the system.

49. The system according to claim 48, wherein the at least one feedback sensor is adapted to sense one or more parameters of a group of parameters relating to: drug level, flow volume in a blood vessel.

50. The system according to claim 48 or 49, wherein the at least one
15 feedback sensor is adapted to sense one or more parameters of the group of parameters comprising: pressure, electrical parameters, distension, and distance.

51. The system according to any one of claims 48 to 50, wherein the at least one feedback sensor is connected to a control.

52. The system according to claim 51, further comprising a control program
20 for controlling at least one motor in response to one or more signals from the at least one feedback sensor.

53. The system according to claim 51 or 52, comprising a feedback
subsystem adapted to wirelessly send feedback information relating to the energy to be stored in energy storage means from inside the human body to the outside
25 thereof, wherein the system is adapted to use the feedback information for adjusting the amount of wireless energy transmitted by the energy transmitter.

54. The system according to claim 53, wherein the feedback information relates to an energy balance which is defined as the balance between an amount of wireless energy received inside the human body and an amount of energy consumed by the at least one energy consuming part.

- 5 55. The system according to claim 54, wherein the feedback information relates to an energy balance which is defined as the balance between a rate of wireless energy received inside the human body and a rate of energy consumed by the at least one energy consuming part.

1/24

FIG 1



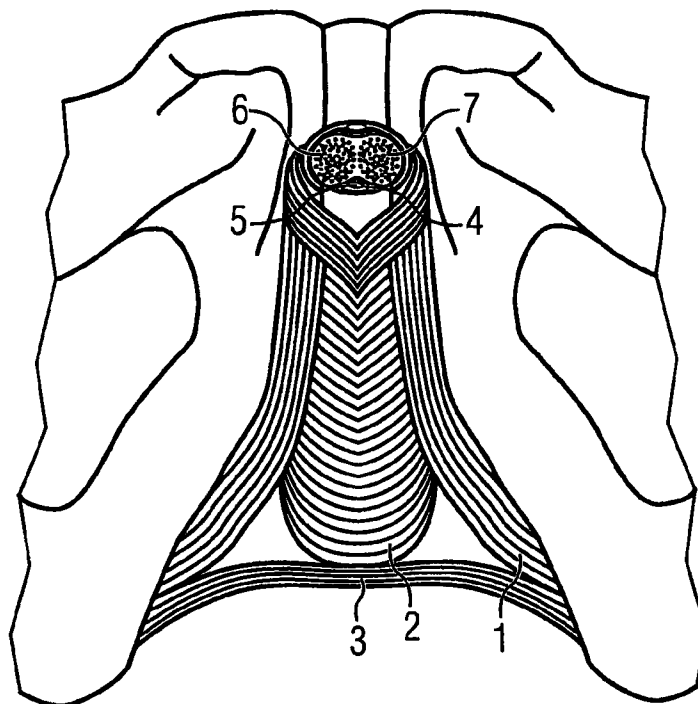


FIG 2

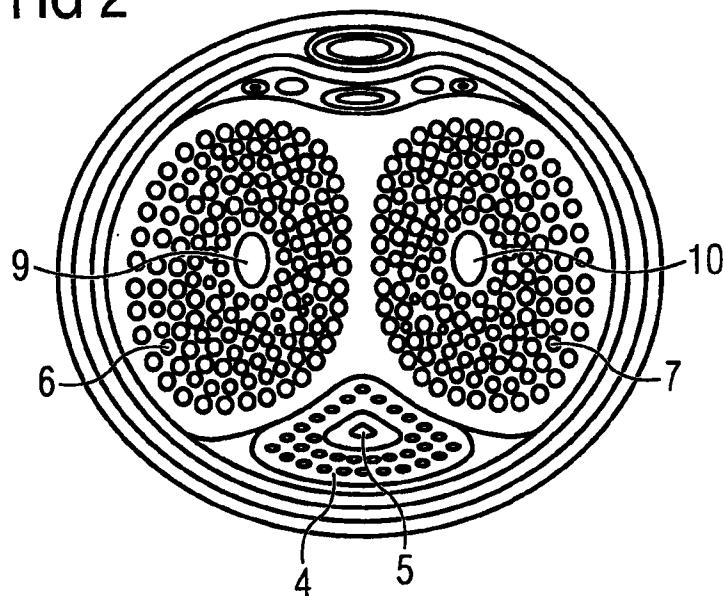


2/24

FIG 3

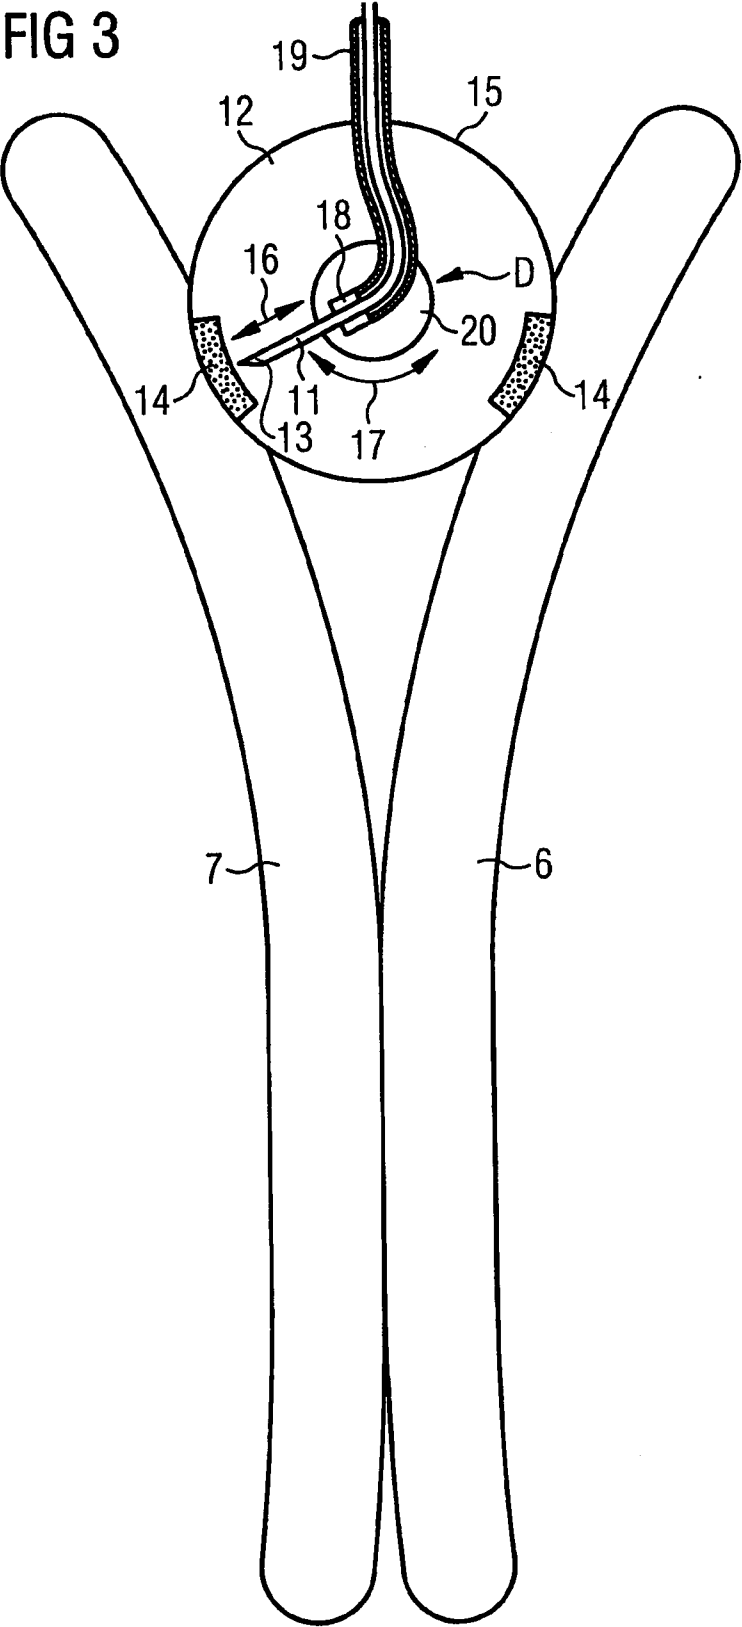


3/24

FIG 4

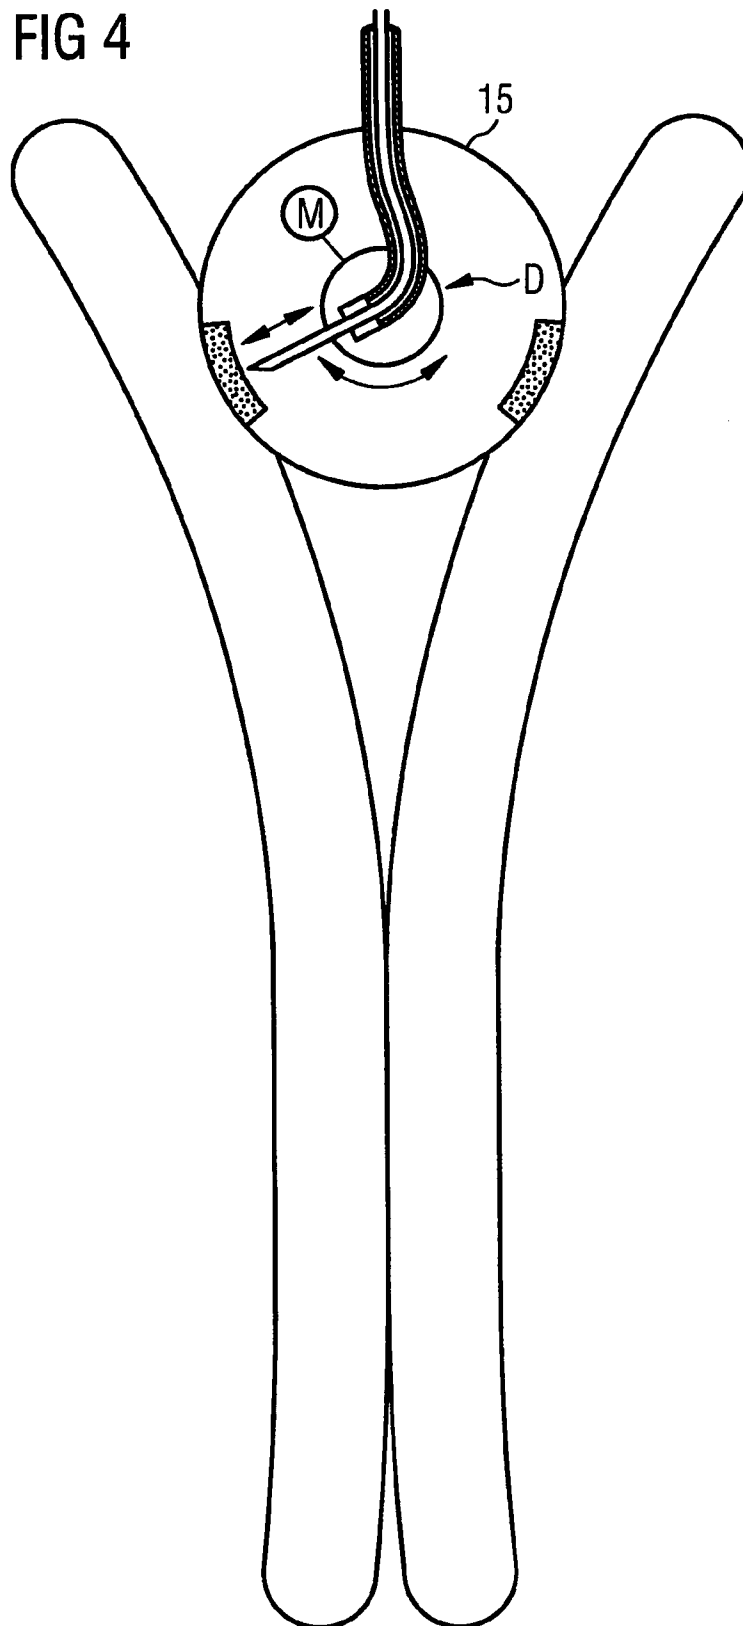

4/24

FIG 5

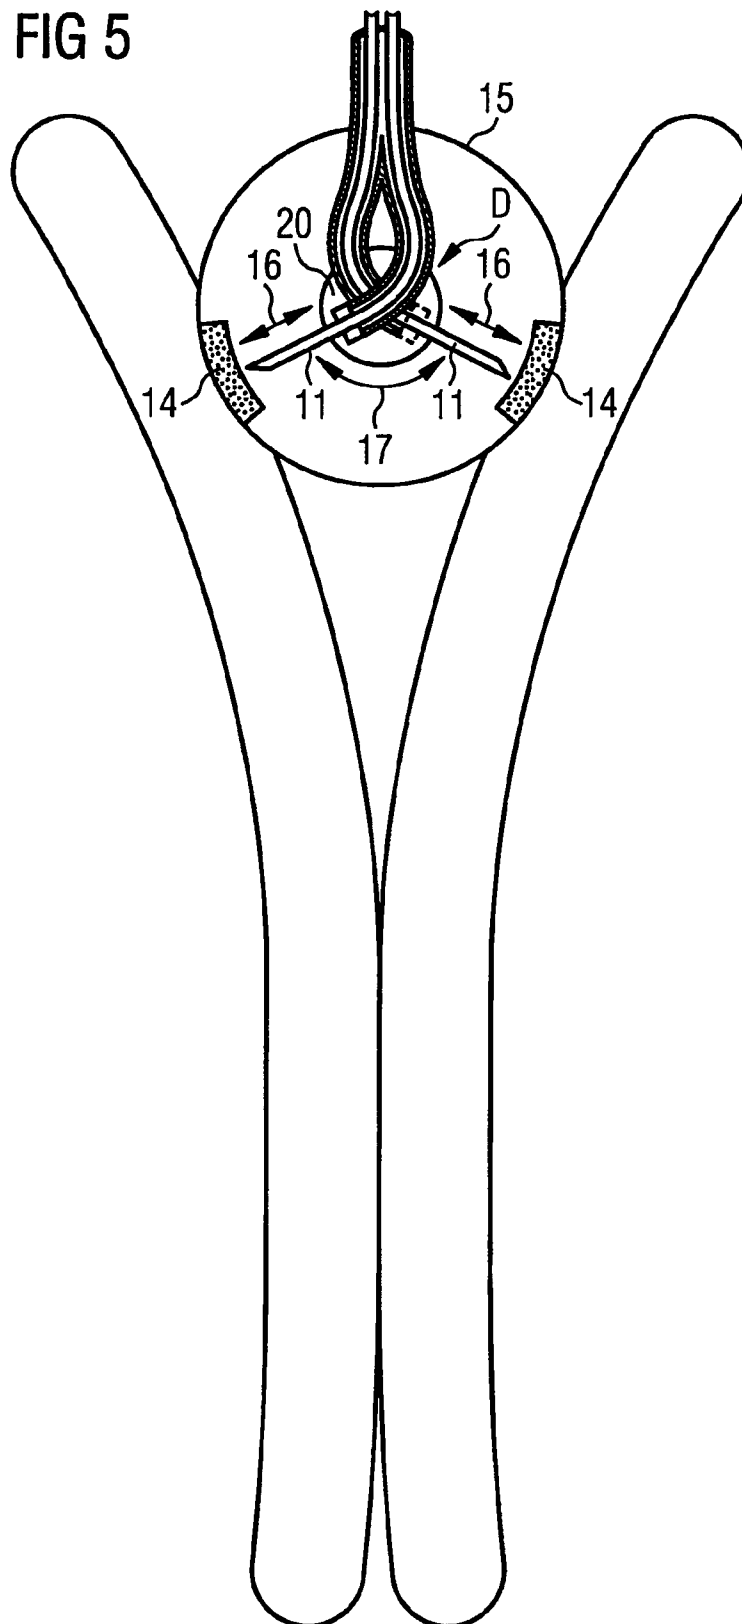

5/24

FIG 6



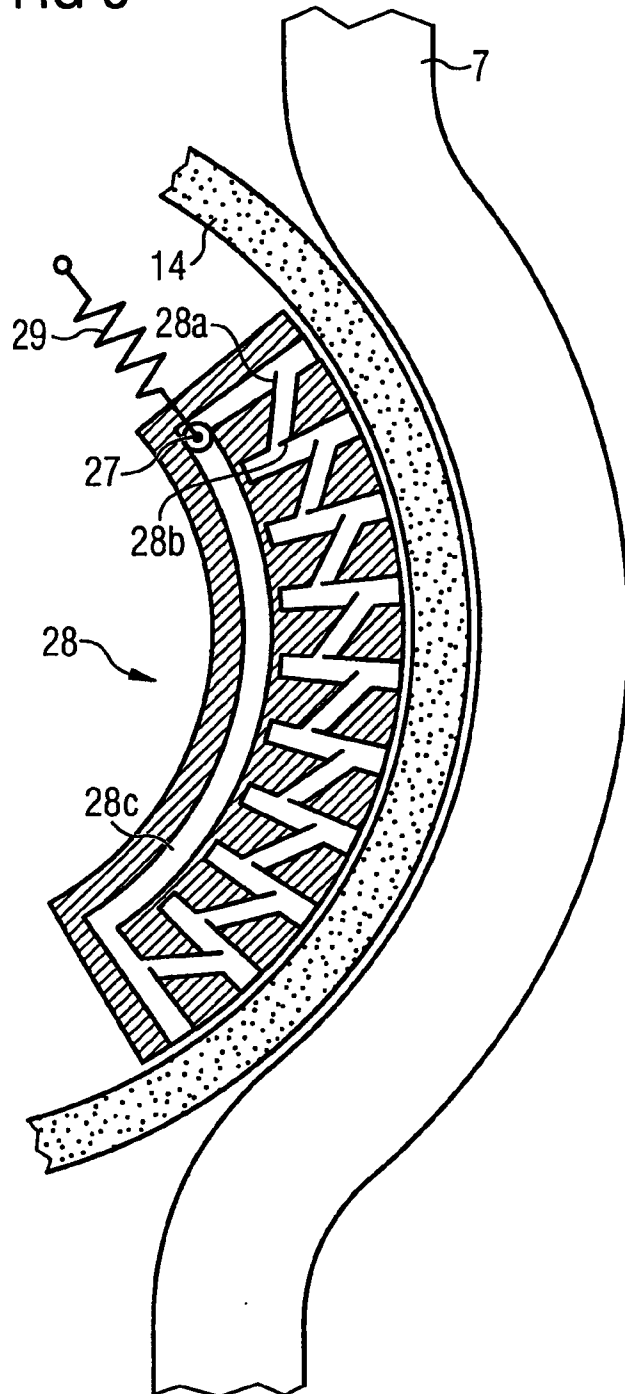


FIG 7

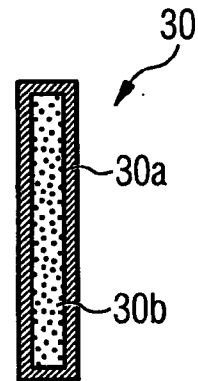

6/24

FIG 8

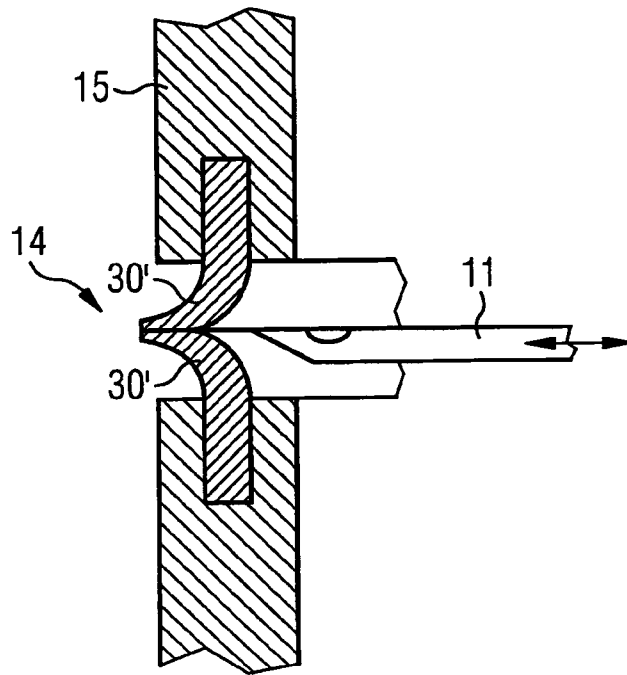

7/24

FIG 9



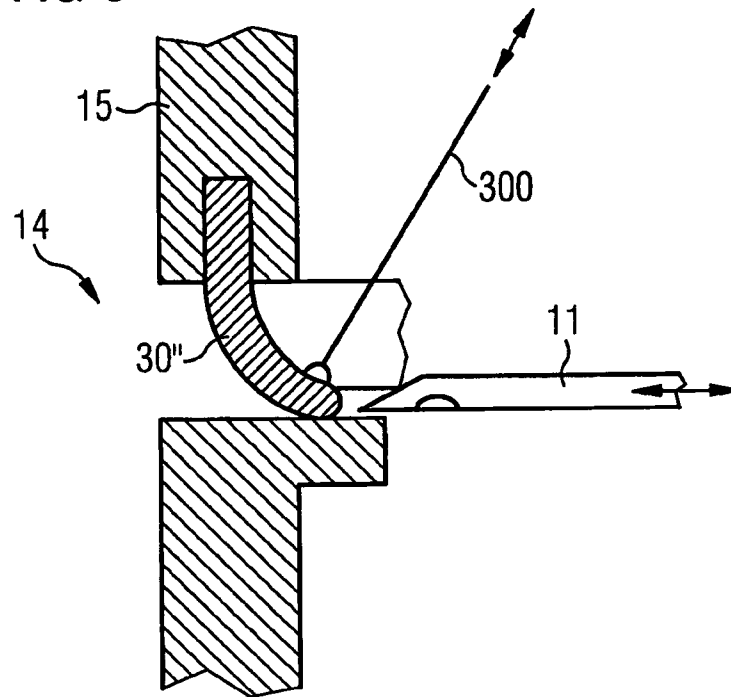


FIG 10

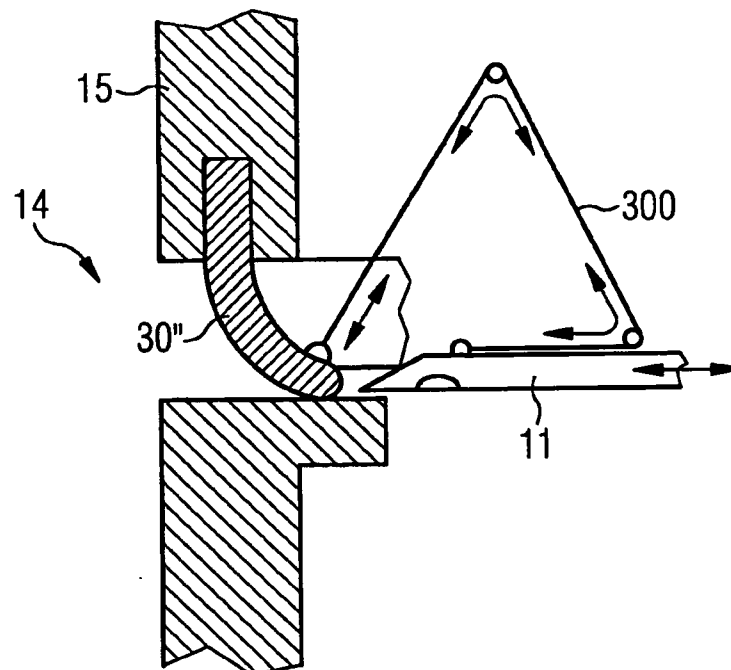


8/24

FIG 11

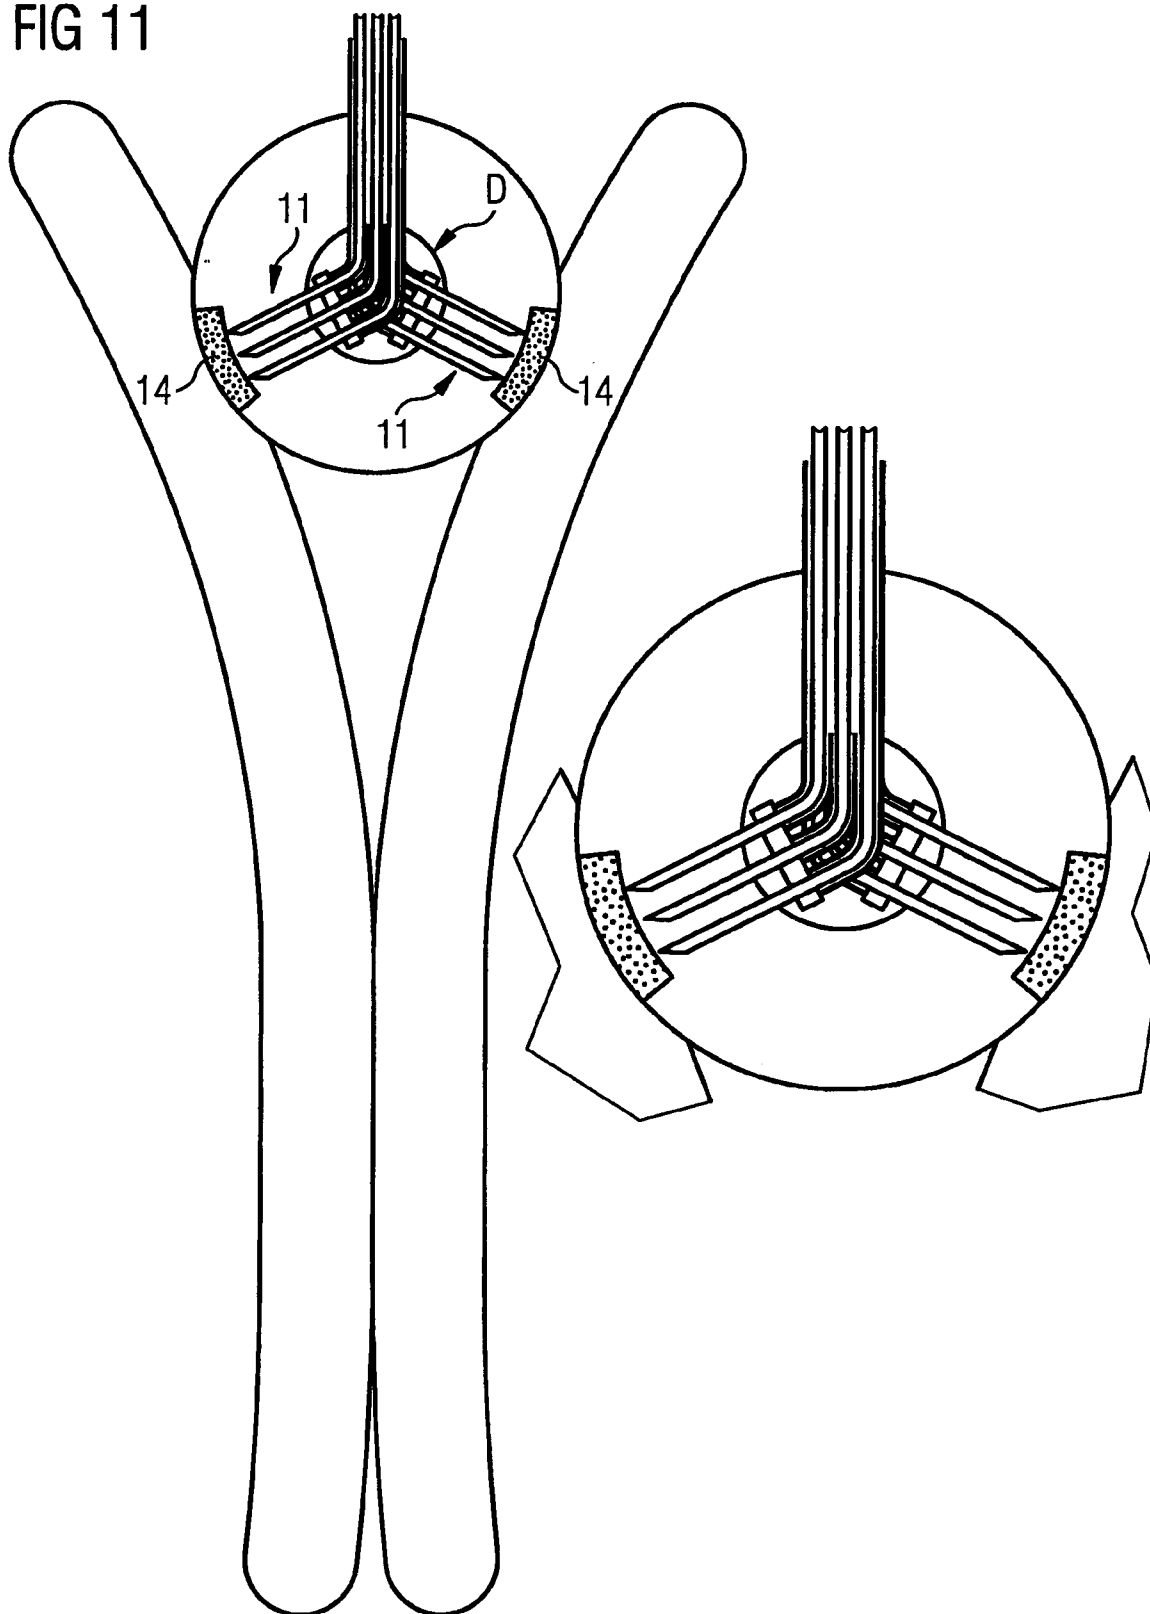

9/24

FIG 12

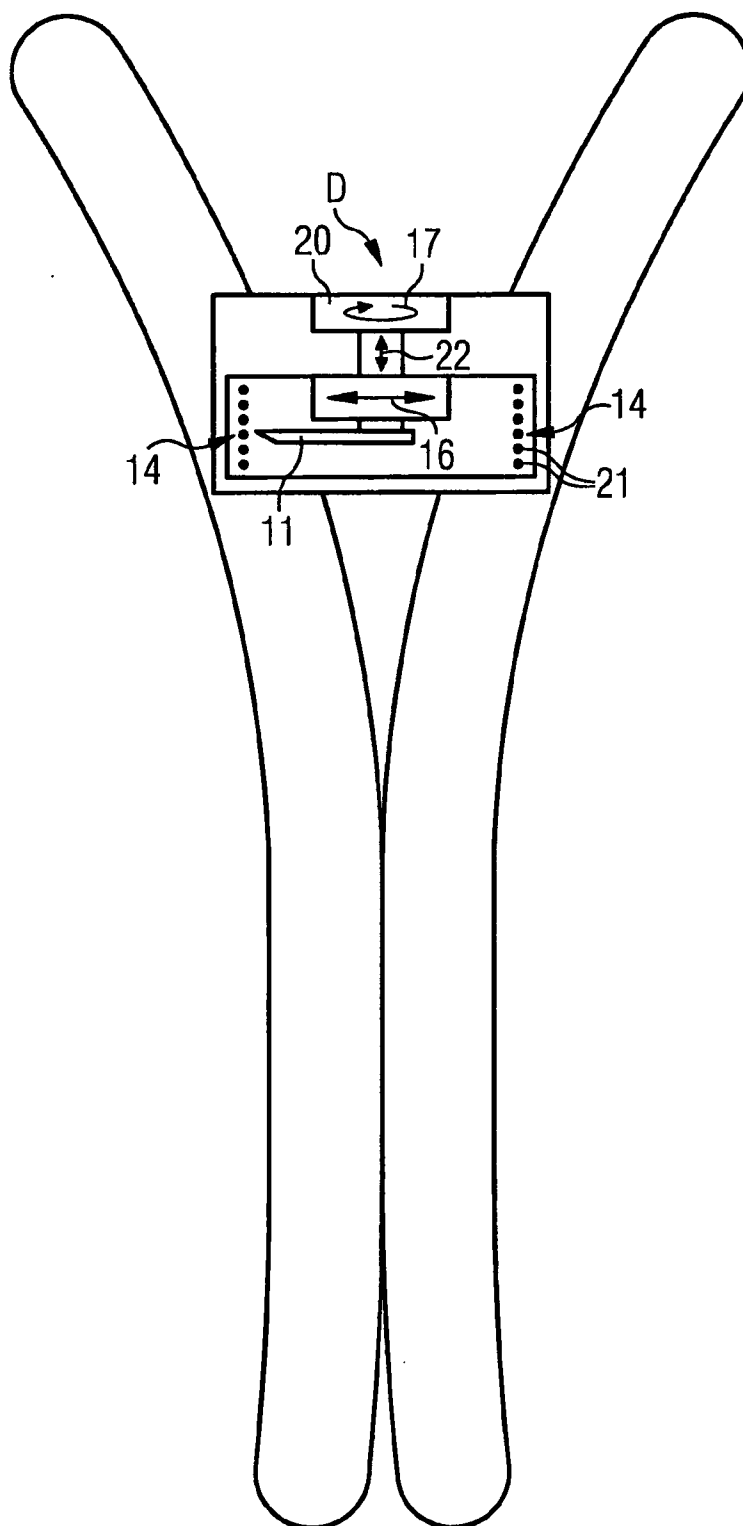

10/24

FIG 13



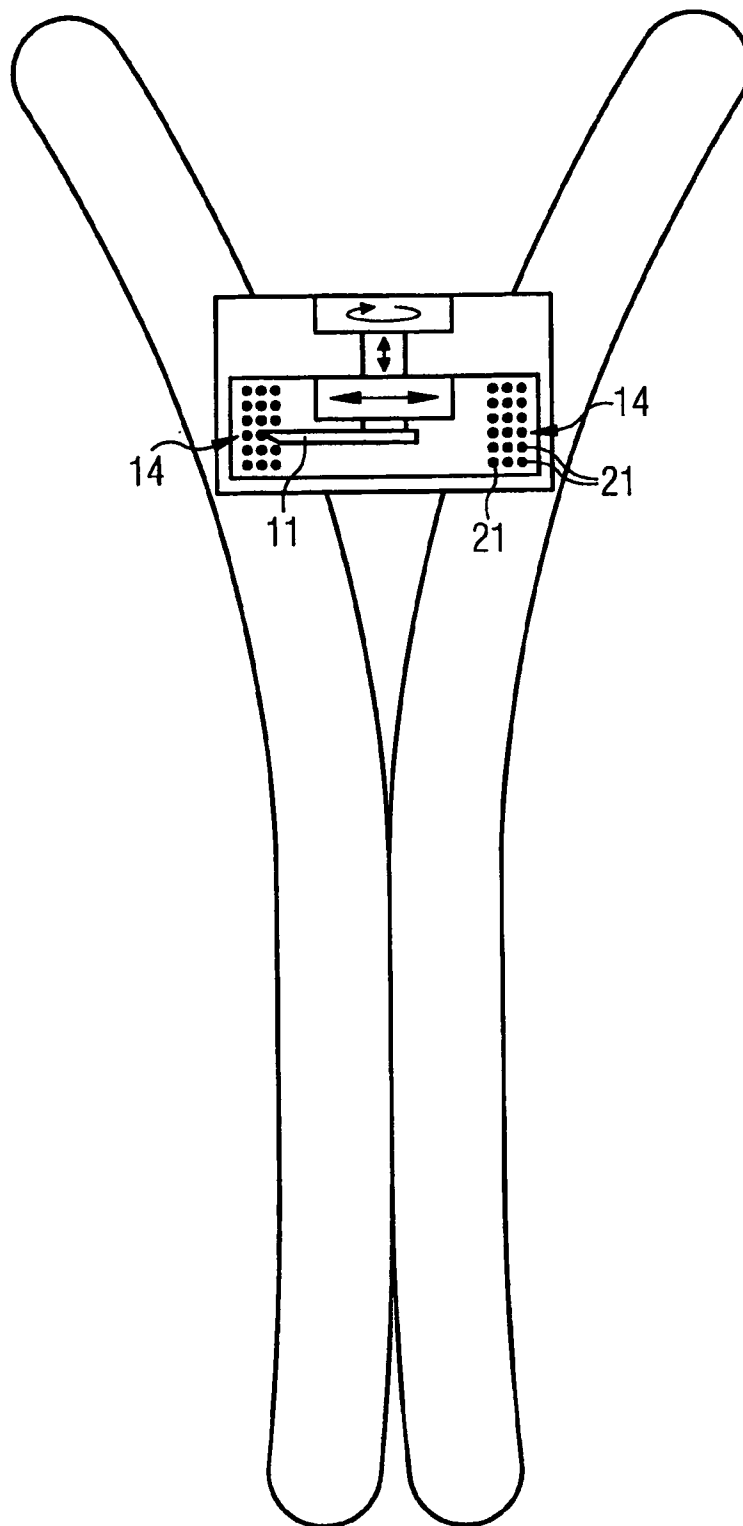


FIG 14

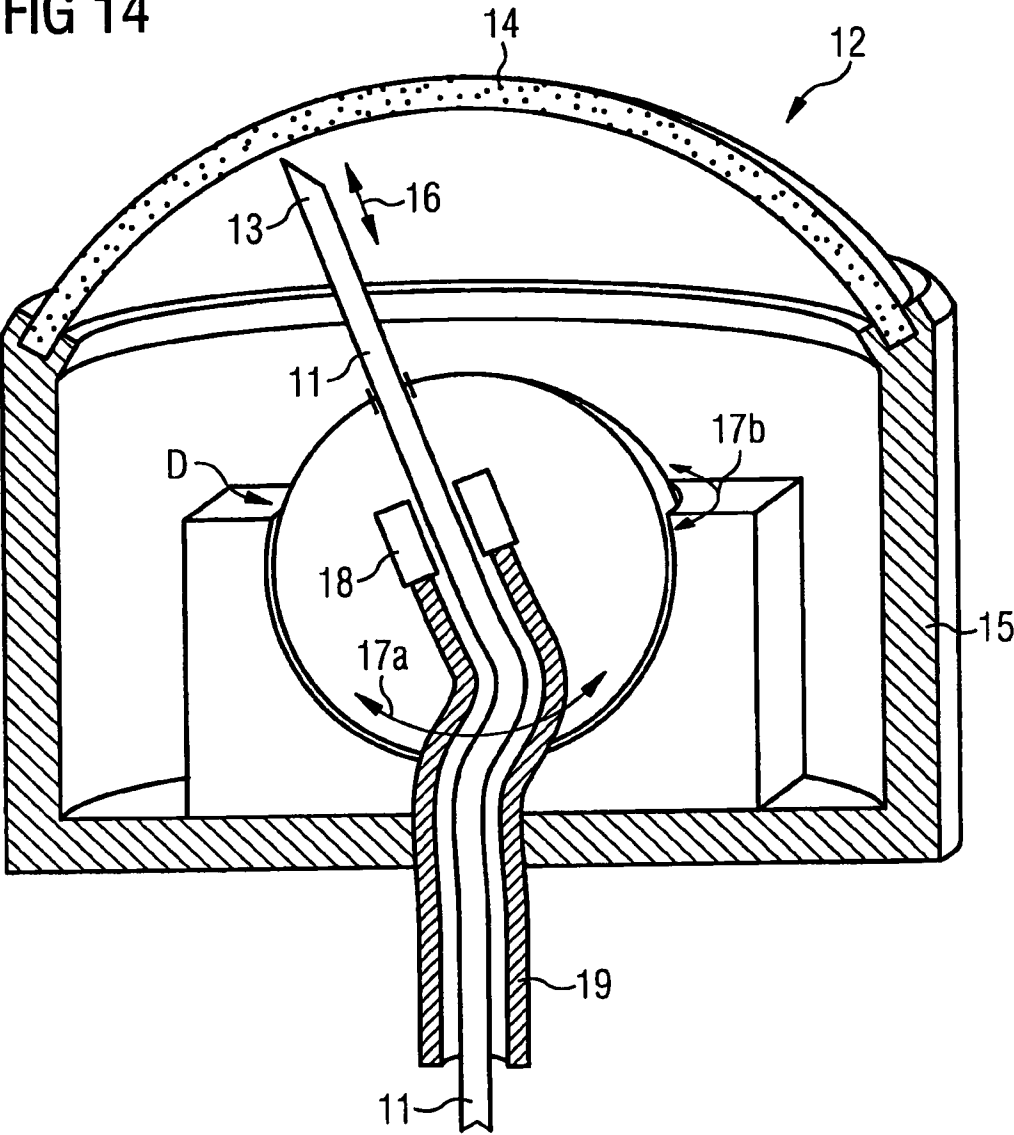

12/24

FIG 15

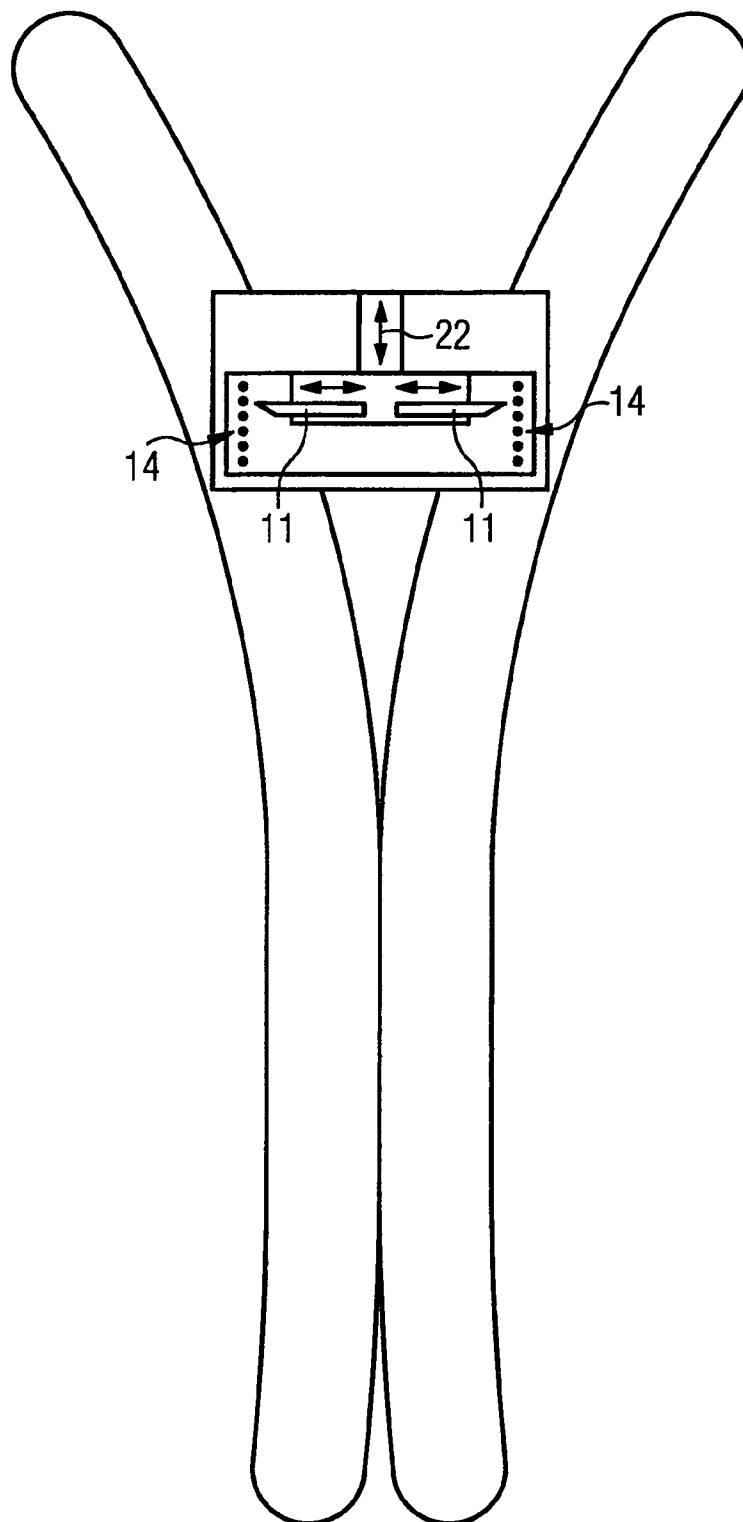

13/24

FIG 16

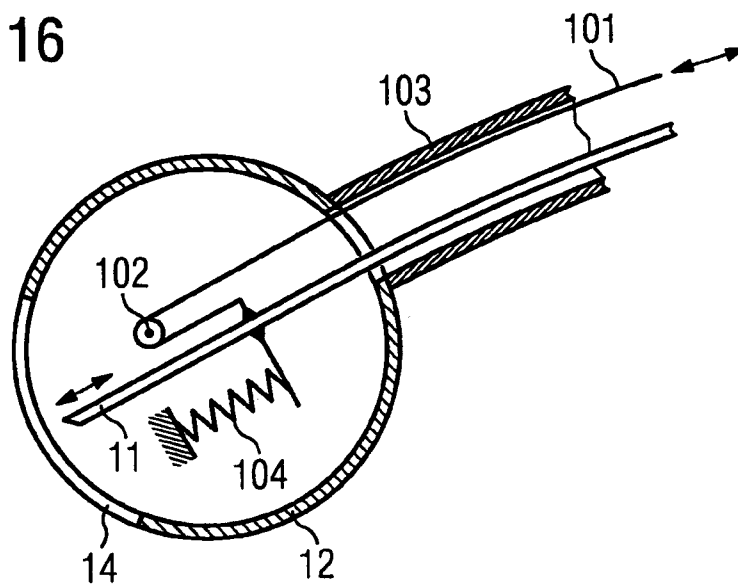


FIG 17



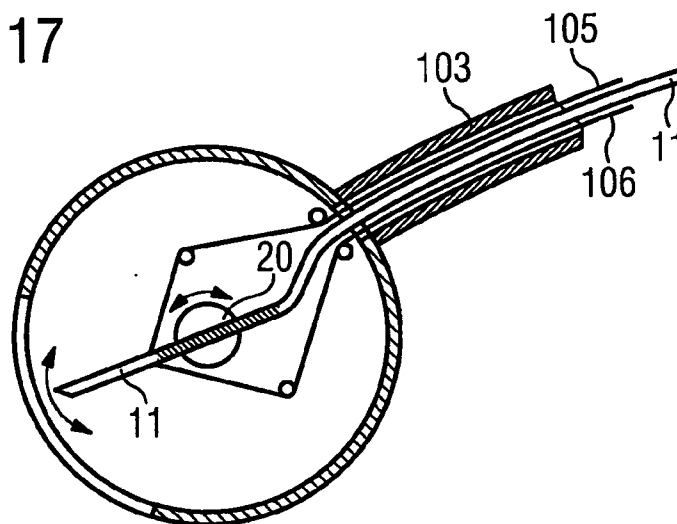


FIG 18

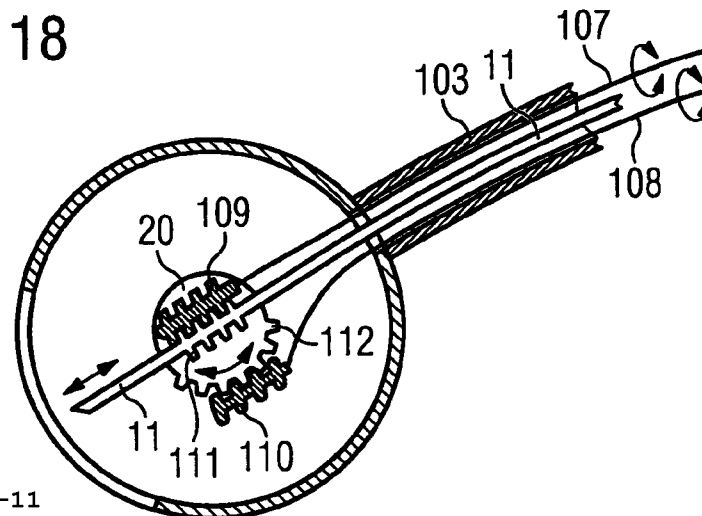

14/24

FIG 19

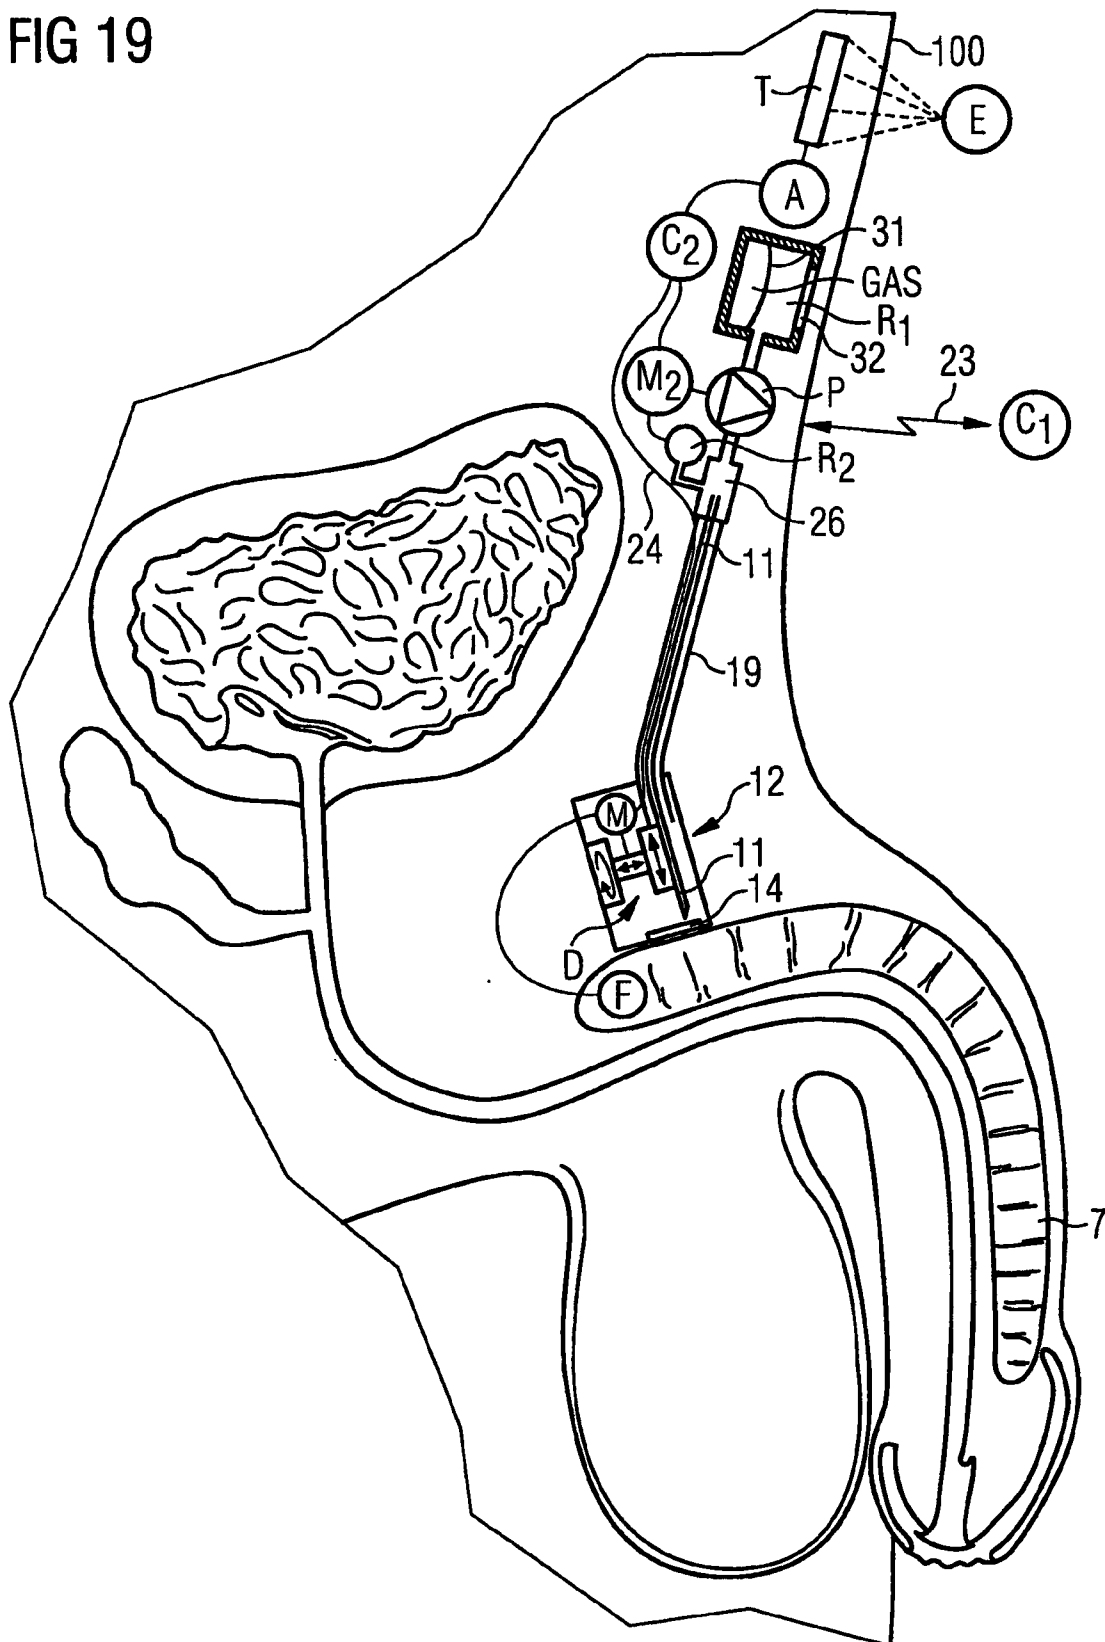

16/24

FIG 21


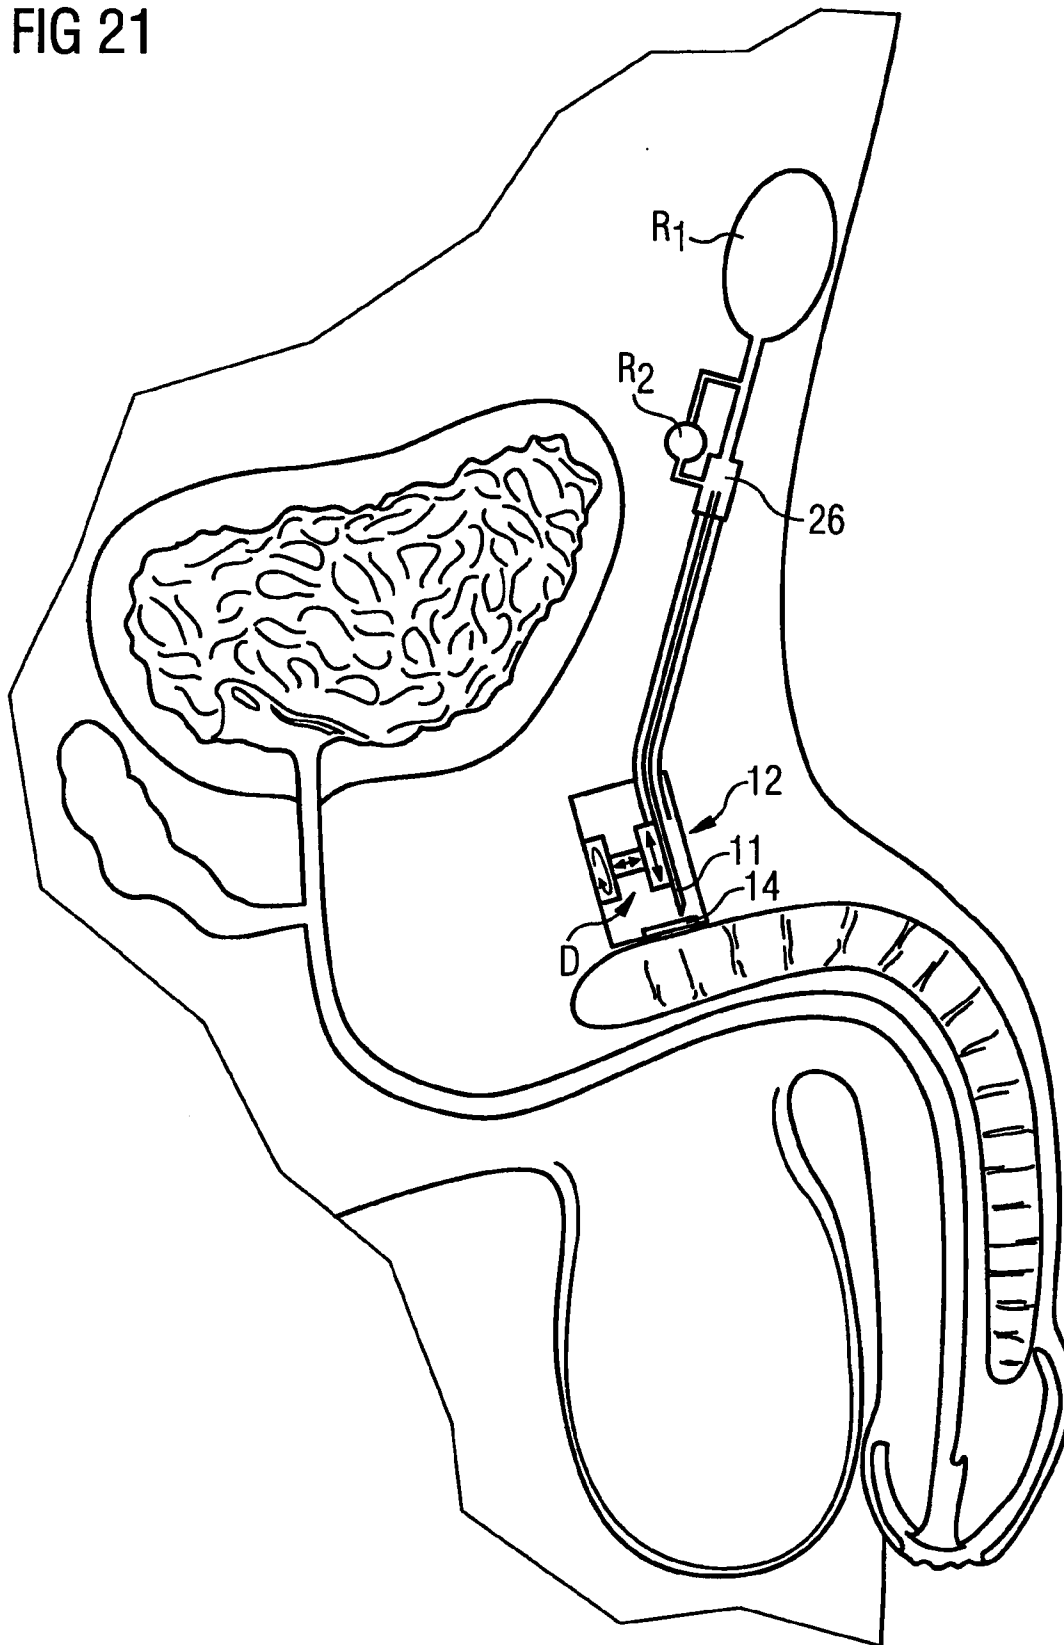


FIG 22

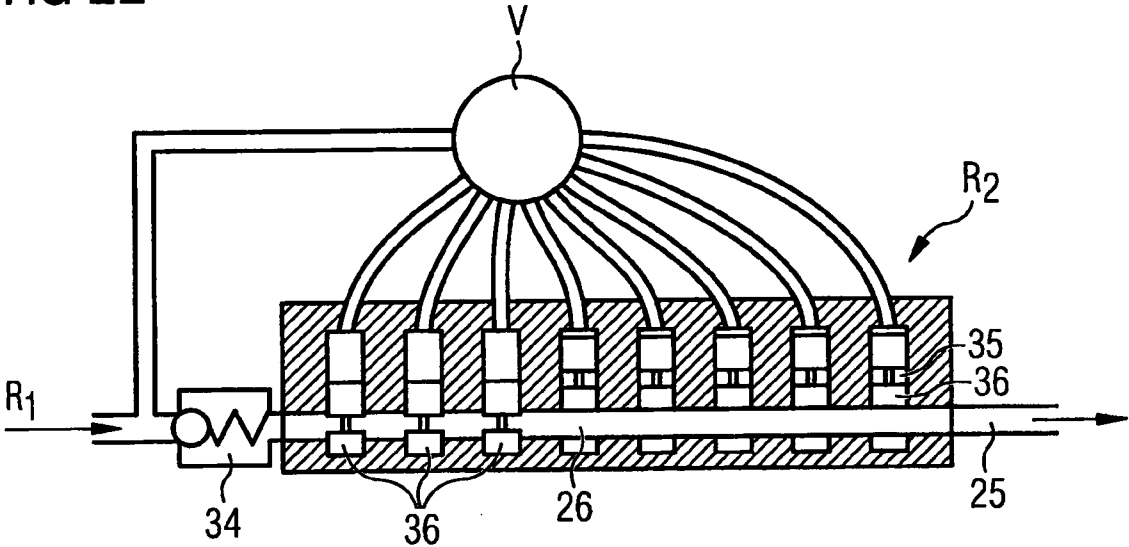

18/24

FIG 23

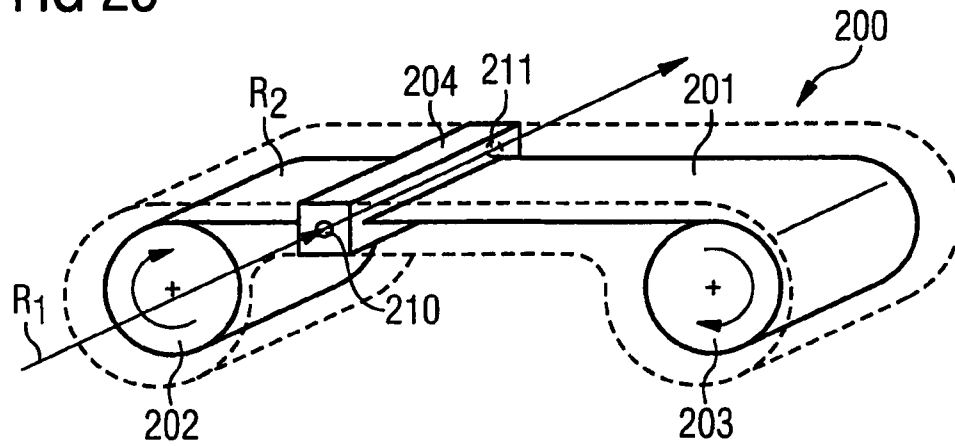


FIG 24


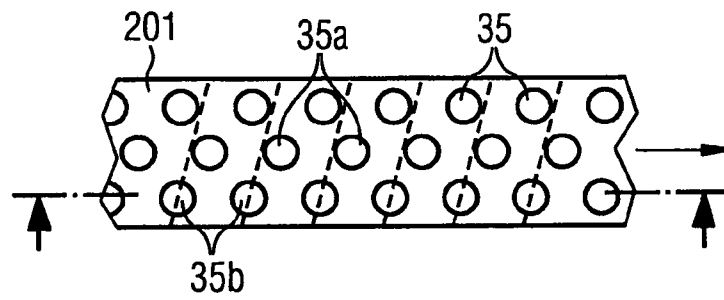


FIG 25

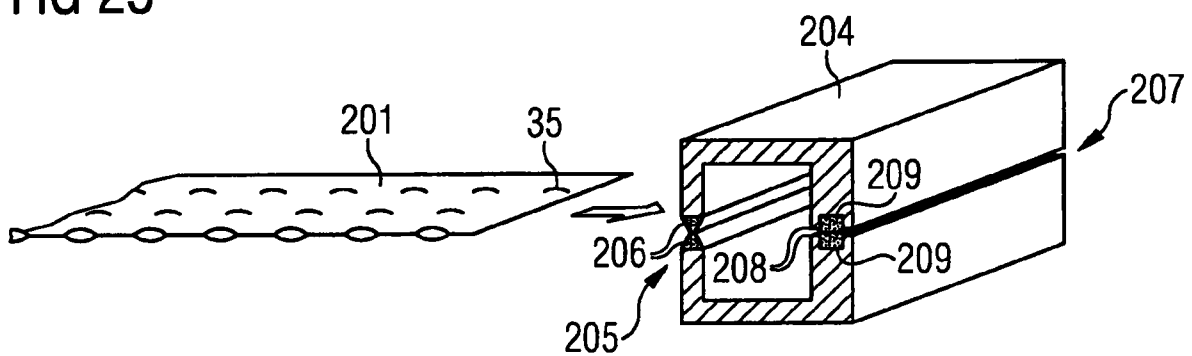

19/24

FIG 26


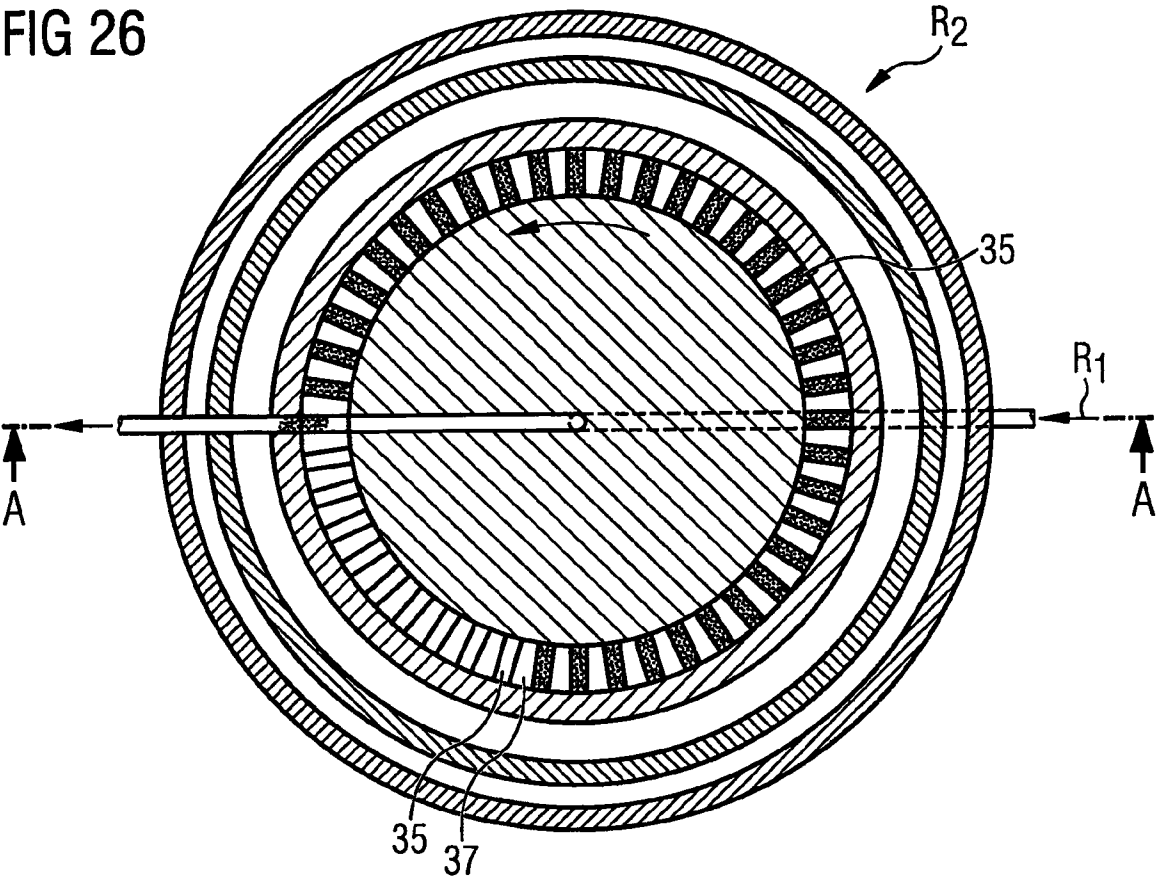


FIG 27

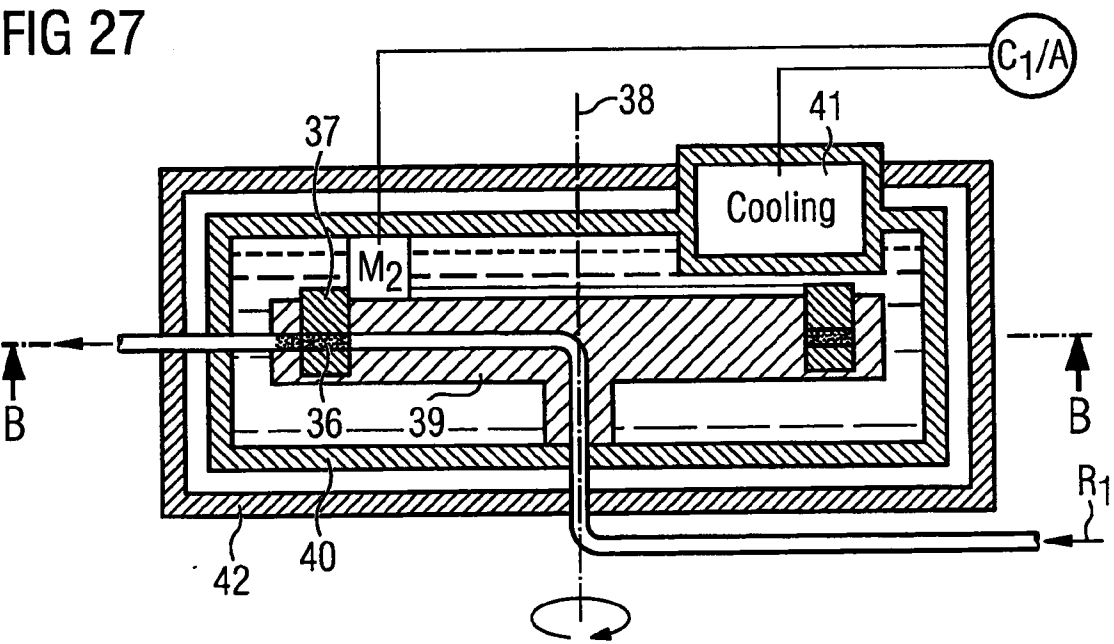

20/24

FIG 28



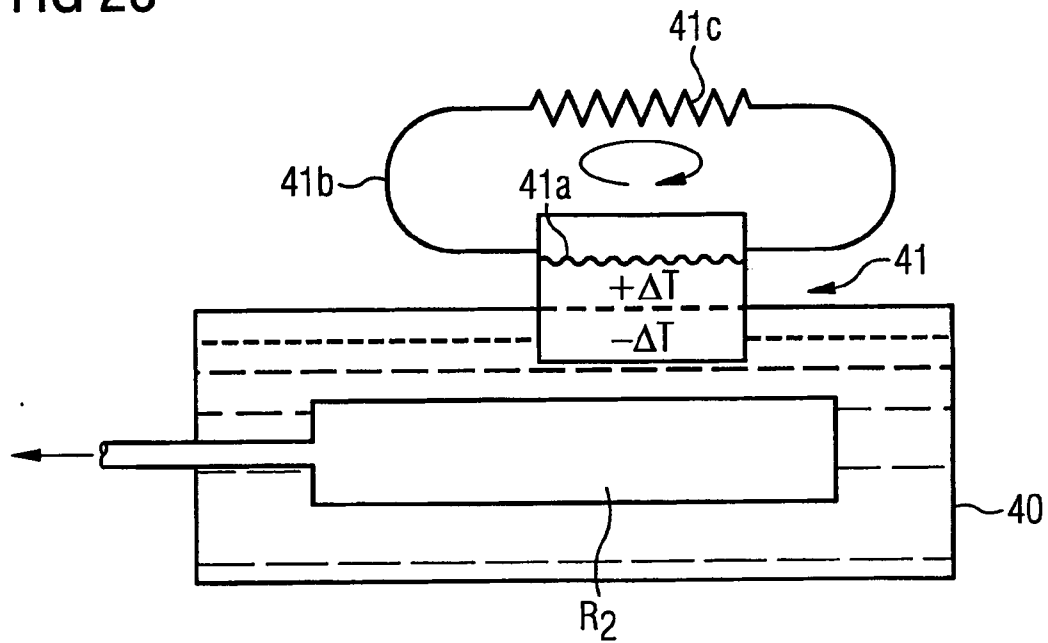


FIG 29

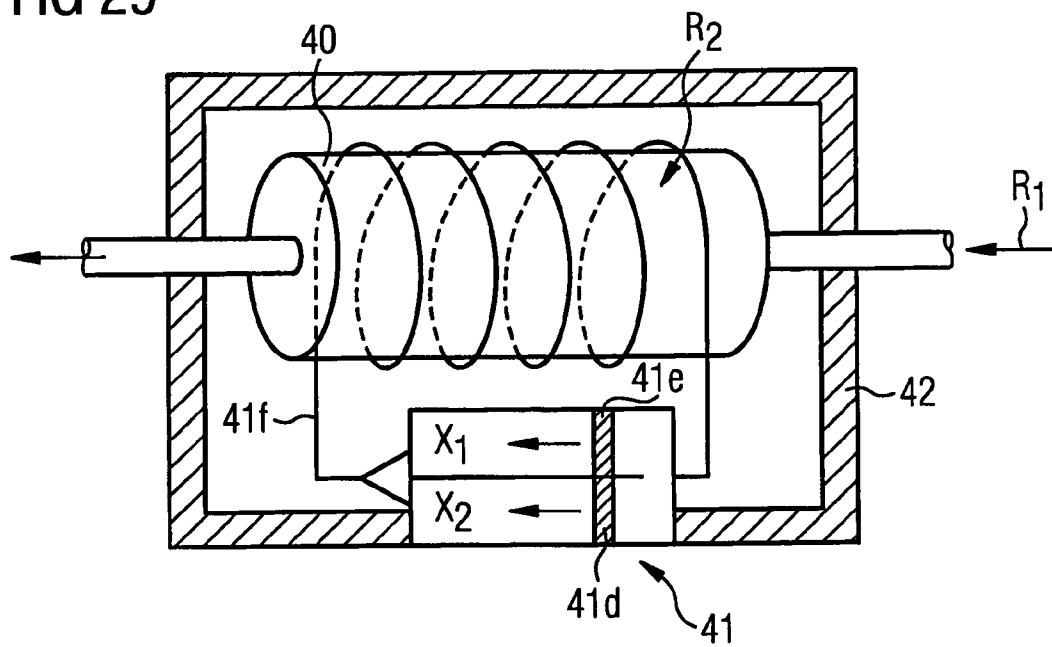

21/24

FIG 30

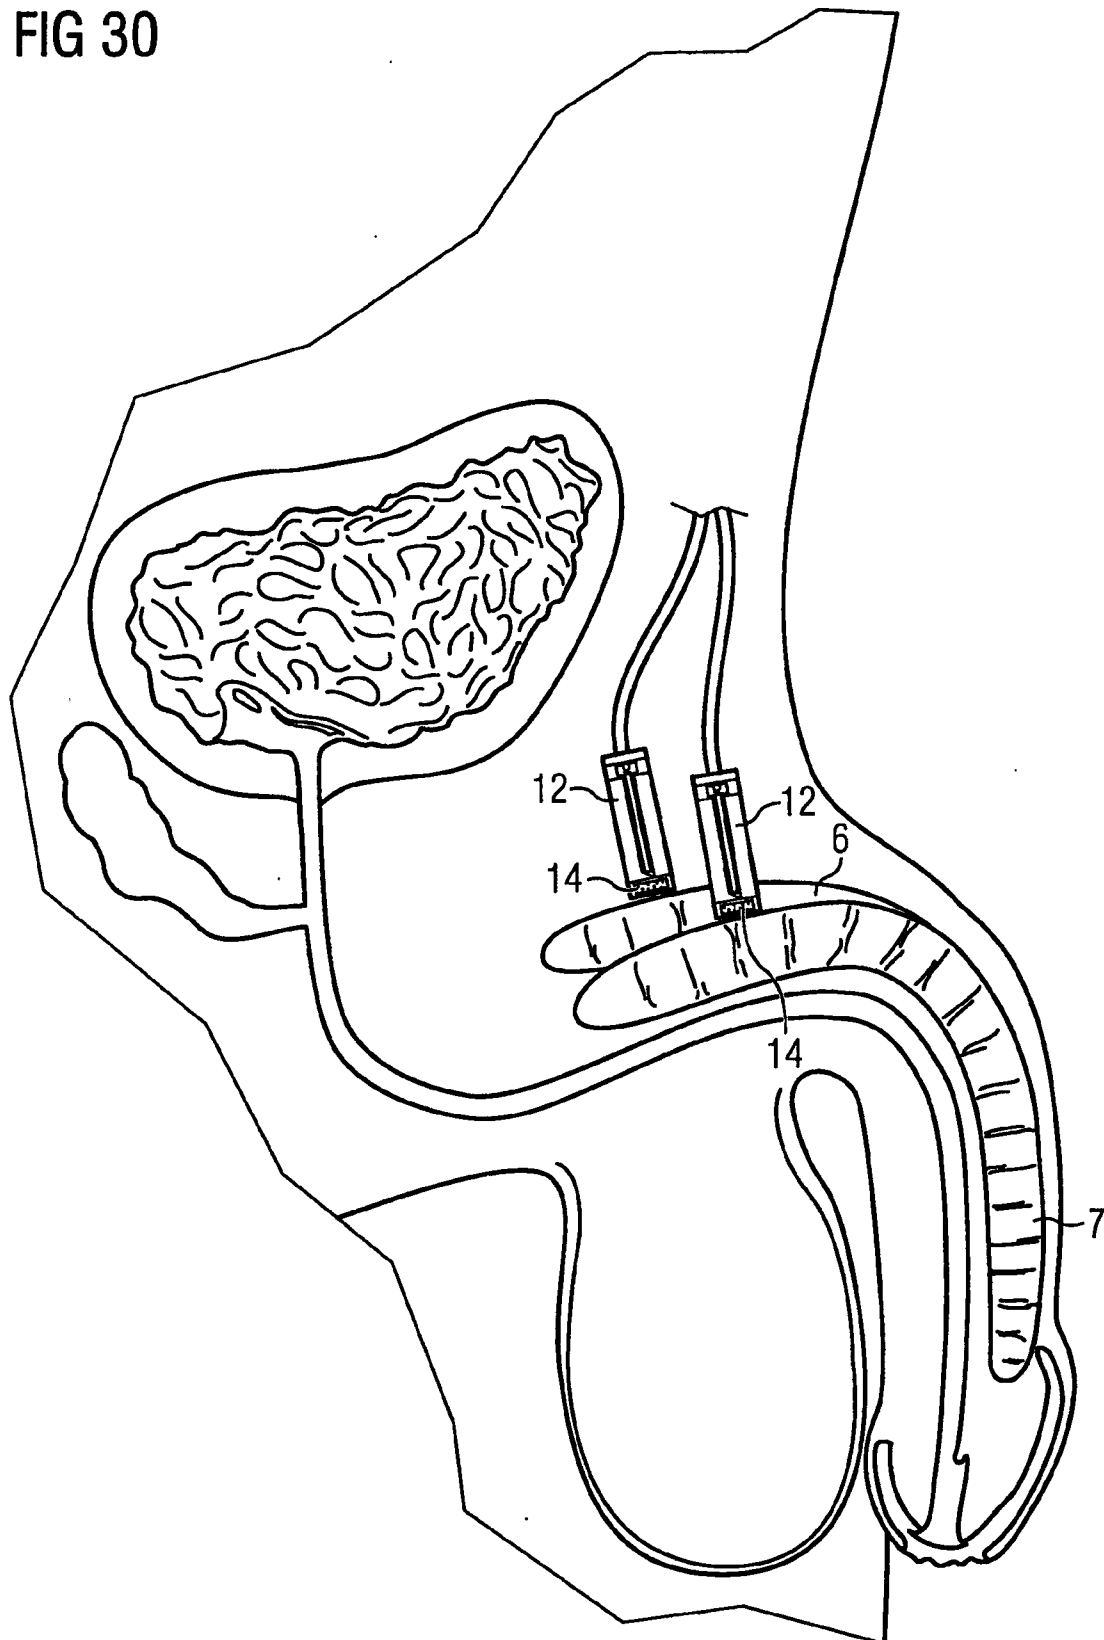

22/24

FIG 31


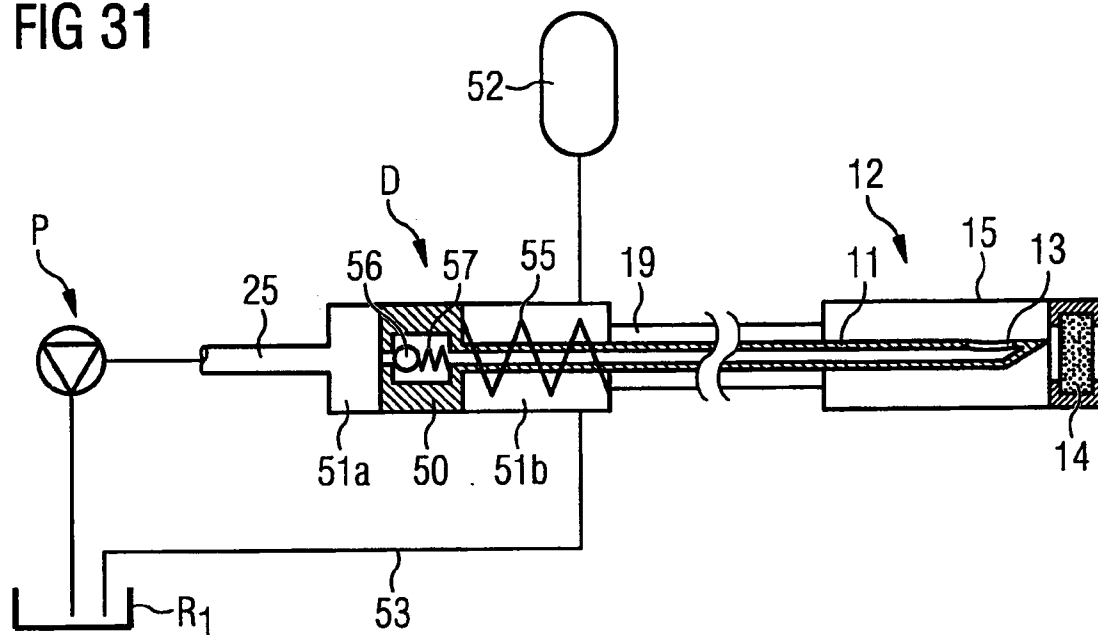


FIG 32

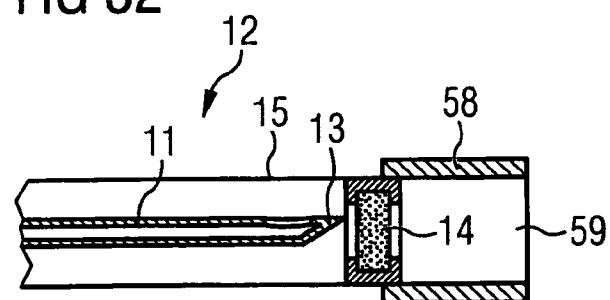

23/24

FIG 33A

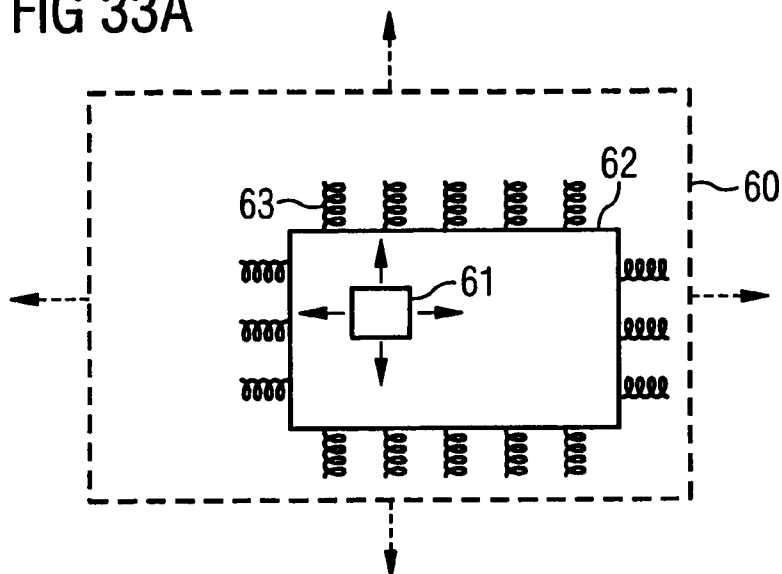


FIG 33B


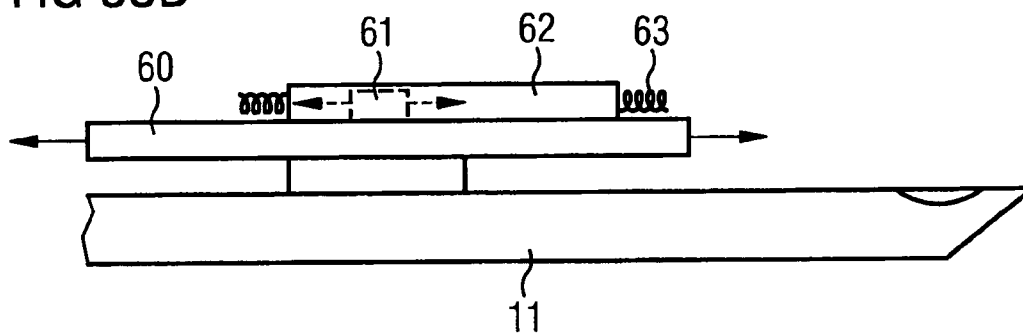


FIG 33C

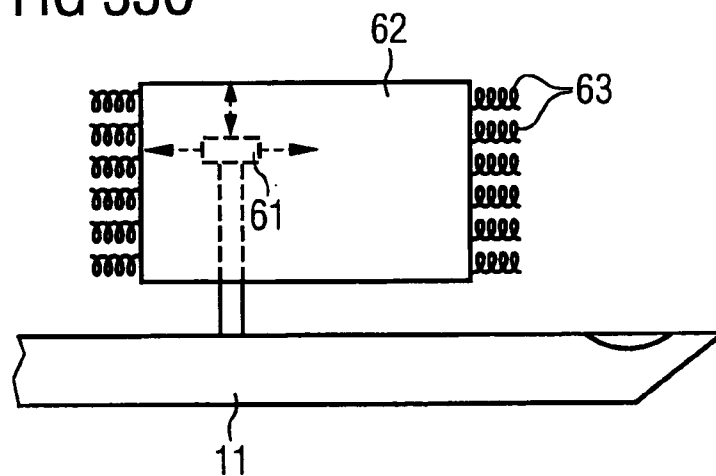

24/24

FIG 34A

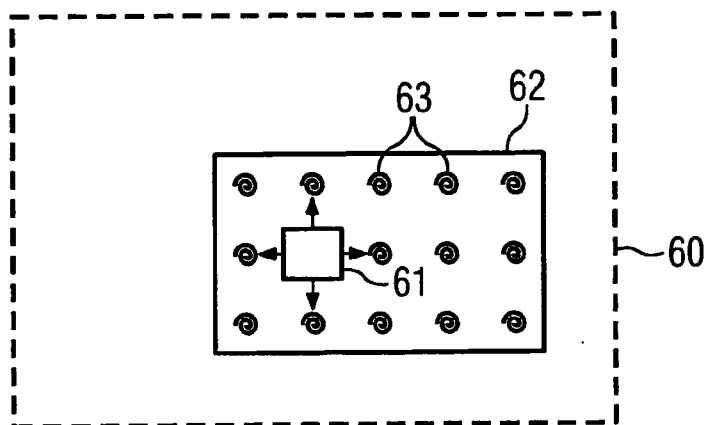


FIG 34B

