

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. AU 2016291677 B2

(54) Title
Earplug assembly for iontophoresis system

(51) International Patent Classification(s)
A61F 11/00 (2006.01) **A61N 1/30** (2006.01)
A61M 31/00 (2006.01) **A61N 1/32** (2006.01)
A61N 1/04 (2006.01)

(21) Application No: **2016291677** (22) Date of Filing: **2016.07.15**

(87) WIPO No: **WO17/011777**

(30) Priority Data

(31) Number (32) Date (33) Country
14/800,869 **2015.07.16** **US**

(43) Publication Date: **2017.01.19**
(44) Accepted Journal Date: **2021.07.15**

(71) Applicant(s)
Tusker Medical, Inc.

(72) Inventor(s)
Ray, Miranda M.;Girotra, Rohit;Truong, Anh Quoc;Patel, Radhika;Gross, Thomas D.;Cantu, Alfredo

(74) Agent / Attorney
Davies Collison Cave Pty Ltd, Att: Scott Sonneman Level 15 1 Nicholson Street, Melbourne, VIC, 3000, AU

(56) Related Art
US 2010/0198135 A1
US 2010/0030131 A1

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2017/011777 A1

(43) International Publication Date

19 January 2017 (19.01.2017)

WIPO | PCT

(51) International Patent Classification:

A61F 11/00 (2006.01) A61N 1/32 (2006.01)
A61M 31/00 (2006.01) A61N 1/04 (2006.01)
A61N 1/30 (2006.01)

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(21) International Application Number:

PCT/US2016/042577

(22) International Filing Date:

15 July 2016 (15.07.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

14/800,869 16 July 2015 (16.07.2015) US

(71) Applicant: **TUSKER MEDICAL, INC.** [US/US]; 4970 El Camino Real, Suite 220, Los Altos, California 94022 (US).

(72) Inventors: **RAY, Miranda M.**; 709 N. 2nd Street, San Jose, California 95112 (US). **GIROTRA, Rohit**; 2225 West Middlefield Road, Mountain View, California 94043 (US). **TRUONG, Anh Quoc**; 4068 Emerald Isle Lane, San Jose, California 95135 (US). **PATEL, Radhika**; 800 Foot-hill Ranch Road, Santa Rosa, California 95049 (US). **GROSS, Thomas D.**; 200 Kimble Avenue, Los Gatos, California 95030 (US). **CANTU, Alfredo**; 4035 School Street, Pleasanton, California 94566 (US).

(74) Agents: **TALBOT, C. Scott** et al.; Cooley LLP, 1299 Pennsylvania Ave., Suite 700, Washington, District of Columbia 20004 (US).

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:


— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))

Published:

— with international search report (Art. 21(3))

— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) Title: EARPLUG ASSEMBLY FOR IONTOPHORESIS SYSTEM

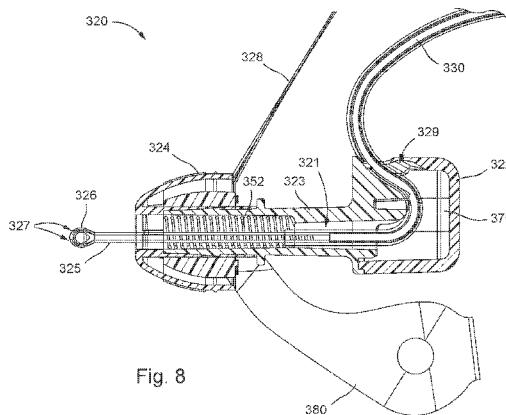

(57) Abstract: Systems, apparatus, and methods are disclosed for gripping and/or positioning a plug (320) in an ear canal outside a tympanic membrane, performing iontophoresis, and/or delivering a pressure equalization tube to the tympanic membrane, including a rigid body (323), an electrode (352), and/or a liner strip (380). The rigid body may define a channel (321), a vent path (329), and a reservoir (370) in fluid communication with the channel and vent path. The reservoir may be configured to increase the volume of the channel, thereby tolerating volumetric changes in the ear without exposing the electrode disposed within the channel to air. The electrode may define a longitudinal axis from which the reservoir extends laterally and proximally to increase a spacing between the electrode and the vent path. The liner strip may include a plurality of gripping portions and attachment portions to cover at least some of a pressure sensitive adhesive on the plug.

WO 2017/011777 A1

EARPLUG ASSEMBLY FOR IONTOPHORESIS SYSTEM

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of and claims priority to U.S. Patent Application No. 14/800,869, filed July 16, 2015, entitled “Earplug Assembly for Iontophoresis System,” the contents of which are incorporated herein by reference in their entirety.

BACKGROUND

[0002] Some children may exhibit recurrent episodes of otitis media and/or -otitis media with effusion. Treatment of severe cases may involve the placement of a pressure equalization tube or tympanostomy tube through the tympanic membrane to provide adequate drainage of the middle ear by providing fluid communication between the middle and outer ear. In particular, such a tube may provide a vent path that promotes drainage of fluid from the middle ear via the Eustachian tube and may thus reduce stress imposed on the tympanic membrane from pressure within the middle ear. This may further reduce the likelihood of future infections and pressure induced ruptures of the tympanic membrane. Pressure equalization tubes may fall out spontaneously within about a year of placement. Exemplary pressure equalization tube delivery systems are disclosed in U.S. Patent No. 8,052,693, entitled “System and Method for the Simultaneous Automated Bilateral Delivery of Pressure Equalization Tubes,” issued November 8, 2011, the disclosure of which is incorporated by reference herein. Additional exemplary pressure equalization tube delivery systems are disclosed in U.S. Patent No. 8,249,700, entitled “System and Method for the Simultaneous Bilateral Integrated Tympanic Drug Delivery and Guided Treatment of Target Tissues within the Ears,” issued August 21, 2012, the disclosure of which is incorporated by reference herein. Still additional exemplary pressure equalization tube delivery systems are disclosed in U.S. Pub. No. 2011/0015645, entitled “Tympanic Membrane Pressure Equalization Tube Delivery System,” published January 20, 2011, the disclosure of which is incorporated by reference herein.

[0003] Insertion of a pressure equalization tube may be performed using general anesthesia in some cases, which may require additional resources such as an operating room, the presence of an anesthesiologist, and time in a recovery room. Furthermore, the use of general anesthesia may include certain risks that a patient may or may not be comfortable with

undertaking. Some pressure equalization tube delivery systems and methods provide a local anesthetic through iontophoresis. Examples of such systems and methods are disclosed in U.S. Pub. No. 2010/0198135, entitled "Systems and Methods for Anesthetizing Ear Tissue," published August 5, 2010, the disclosure of which is incorporated by reference herein. Additional examples of such systems and methods are disclosed in U.S. Patent No. 8,192,420, entitled "Iontophoresis Methods," issued June 5, 2012, the disclosure of which is incorporated by reference herein.

[0004] While a variety of pressure equalization tube delivery systems and methods have been made and used, it is believed that no one prior to the inventor(s) has made or used an invention as described herein.

[0004A] The present invention provides an apparatus comprising:

- (a) a rigid body defining:
 - (i) a channel;
 - (ii) a reservoir in fluid communication with the channel, the reservoir and the channel providing a combined volume greater than a volume of the channel; and
 - (iii) a vent path in fluid communication with the reservoir; and
 - (iv) a conduit opening;
- (b) an electrode defining a longitudinal axis and disposed within the channel of the rigid body, the reservoir extending laterally and proximally from the longitudinal axis defined by the electrode;
- (c) a sealing element configured to bear against a wall of an ear canal to thereby define a closed volume outside of a tympanic membrane in the ear canal; and
- (d) a fluid conduit in fluid communication with the channel to fill at least one of the closed volume, the channel, and the reservoir with fluid, the fluid conduit extending through the conduit opening defined by the rigid body.

SUMMARY

[0005] In one embodiment, an apparatus includes a rigid body defining a channel, a reservoir in fluid communication with the channel, the reservoir configured to increase the volume of the channel, and a vent path in fluid communication with the reservoir. The apparatus further includes an electrode defining a longitudinal axis and disposed within the

channel of the rigid body, the reservoir extending laterally and proximally from the longitudinal axis defined by the electrode to increase a spacing between the electrode and the vent path.

[0006] In another embodiment, an apparatus includes a fluid reservoir defining a first volume, a plug to define a closed volume in an ear canal outside a tympanic membrane, a working conduit to connect the fluid reservoir with the closed volume, and a drainage conduit to extend from the fluid reservoir to a region outside the closed volume and the plug. The working conduit defines a second volume, and the first volume of the fluid reservoir is greater than the second volume of the working conduit. The fluid reservoir, the plug, the working conduit, and the drainage conduit are configured to supply fluid from the fluid reservoir through the working conduit to the closed volume.

[0007] In some embodiments, an apparatus includes a liner strip to facilitate gripping and/or positioning a plug in an ear canal outside a tympanic membrane. The plug includes a sealing element with a pressure sensitive adhesive thereon. The liner strip includes a plurality of attachment portions and a plurality of gripping portions. Each attachment portion is defined by a corresponding fold in the liner strip and configured to cover a discrete portion of the pressure sensitive adhesive on the sealing element. Each gripping portion is defined by a corresponding fold in the liner strip and configured to extend proximally away from the plug. Each attachment portion is connected to a distal end of a corresponding gripping portion.

[0008] It should be appreciated that all combinations of the foregoing concepts and additional concepts discussed in greater detail below (provided such concepts are not mutually inconsistent) are contemplated as being part of the inventive subject matter disclosed herein. In particular, all combinations of claimed subject matter appearing at the end of this disclosure are contemplated as being part of the inventive subject matter disclosed herein. It should also be appreciated that terminology explicitly employed herein that also may appear in any disclosure incorporated by reference should be accorded a meaning most consistent with the particular concepts disclosed herein.

[0009] In the description in this specification reference may be made to subject matter which is not within the scope of the appended claims. That subject matter should be readily

identifiable by a person skilled in the art and may assist in putting into practice the invention as defined in the presently appended claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The skilled artisan will understand that the drawings primarily are for illustrative purposes and are not intended to limit the scope of the inventive subject matter described herein. The drawings are not necessarily to scale; in some instances, various aspects of the inventive subject matter disclosed herein may be shown exaggerated or enlarged in the drawings to facilitate an understanding of different features. In the drawings, like reference characters generally refer to like features (e.g., functionally similar and/or structurally similar elements).

[0011] FIG. 1 depicts a perspective view of an exemplary pressure equalization tube delivery device (PETDD) in accordance with some embodiments.

[0012] FIG. 2 depicts a perspective view of an exemplary pressure equalization (PE) tube suitable for delivery by the PETDD of FIG. 1 in accordance with some embodiments.

[0013] FIG. 3 depicts a side elevational view of the PE tube of FIG. 2, positioned within a tympanic membrane in accordance with some embodiments.

[0014] FIG. 4 depicts an exemplary iontophoresis system incorporating an earplug in accordance with some embodiments.

[0015] FIG. 5 depicts a cross-sectional side view of the earplug of FIG. 4 in accordance with some embodiments.

[0016] FIG. 6 depicts a perspective view of another exemplary iontophoresis system incorporating an earplug in accordance with some embodiments.

[0017] FIG. 7 depicts a perspective view of the earplug of FIG. 6 in accordance with some embodiments.

[0018] FIG. 8 depicts a side cross-sectional view of the earplug of FIG. 6, with the cross-section taken along line 8-8 of FIG. 7 in accordance with some embodiments.

[0019] FIG. 9 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned adjacent to a patient's ear at a horizontal orientation in accordance with some embodiments.

[0020] FIG. 10 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned within a patient's ear canal at a horizontal orientation in accordance with some embodiments.

[0021] FIG. 11 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned within a patient's ear canal at a horizontal orientation, and with the earplug filling a patient's ear canal with iontophoresis fluid in accordance with some embodiments.

[0022] FIG. 12 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned within a patient's ear canal at a horizontal orientation, and with a patient's ear canal fully filled with iontophoresis fluid and excess fluid escaping through a vent path of the earplug in accordance with some embodiments.

[0023] FIG. 13 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned within a patient's ear canal at a horizontal orientation, and with the earplug in a state ready for activation of an electrode of the earplug in accordance with some embodiments.

[0024] FIG. 14 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned within a patient's ear canal at a horizontal orientation, and with the patient's ear canal exhibiting volumetric changes, thereby expelling iontophoresis fluid through the vent path in accordance with some embodiments.

[0025] FIG. 15 depicts another side cross-sectional view of the earplug of FIG. 6, with the earplug positioned within a patient's ear canal at a horizontal orientation, and with at least some fluid expelled from a reservoir of the earplug in accordance with some embodiments.

[0026] FIG. 16 depicts yet another side cross-sectional view of the earplug of FIG. 6 with the earplug positioned within a patient's ear canal at a vertical orientation in accordance with some embodiments.

[0027] FIG. 17 depicts a front elevational view of a liner strip that may be used with the earplug of FIG. 6, with the liner strip in a flat and unfolded configuration in accordance with some embodiments.

[0028] FIG. 18 depicts a perspective view of the liner strip of FIG. 17 in a folded configuration in accordance with some embodiments.

[0029] FIG. 19 depicts detailed perspective view of the liner strip of FIG. 17 attached to the earplug of FIG. 6 in the folded configuration of FIG. 18 in accordance with some embodiments.

DETAILED DESCRIPTION

[0030] The following description of certain examples of the technology should not be used to limit its scope. Other examples, features, aspects, embodiments, and advantages of the technology will become apparent to those skilled in the art from the following description, which is by way of illustration, one of the best modes contemplated for carrying out the technology. As will be realized, the technology described herein is capable of other different and obvious aspects, all without departing from the technology. Accordingly, the drawings and descriptions should be regarded as illustrative in nature and not restrictive.

[0031] It is further understood that any one or more of the teachings, expressions, embodiments, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, embodiments, examples, etc. that are described herein. The

following-described teachings, expressions, embodiments, examples, etc. should therefore not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

I. Exemplary Pressure Equalization Tube Delivery Device (PETDD)

[0032] As noted above, a pressure equalization (PE) tube may be delivered to the tympanic membrane (TM) of a patient as a way of treating, for example, otitis media. In some instances, a delivery instrument may be used to insert PE tubes in the tympanic membrane (TM) without the use of general anesthesia. FIG. 1 shows an exemplary equalization tube delivery device (PETDD) (10) that may be used in such procedures. It should be understood that PETDD (10) may be used with an endoscope to provide visualization of the tympanic membrane (TM) during use of PETDD (10). It should also be understood that a patient may receive local anesthesia at the tympanic membrane (TM) through a process of iontophoresis before PETDD (10) is actuated to deploy a PE tube. Various examples of devices and methods that may be used to provide iontophoresis will be described in greater detail below. It should also be understood that iontophoresis may be provided in accordance with at least some of the teachings of U.S. Pub. No. 2010/0198135, the disclosure of which is incorporated by reference herein; and/or in accordance with at least some of the teachings of U.S. Patent No. 8,192,420, the disclosure of which is incorporated by reference herein.

[0033] As shown in FIG. 1, PETDD (10) of this example includes a handpiece (12) and a cannula (14) extending distally from handpiece (12). Cannula (14) is sized for insertion in a patient's ear canal, such that the tip (16) of cannula may directly engage the patient's tympanic membrane (TM). As soon as the tip (16) achieves apposition with the tympanic membrane (TM), the operator may depress button (18), which may trigger a firing sequence whereby PETDD (10) creates a myringotomy incision, dilates the myringotomy incision, and inserts a PE tube in the myringotomy incision nearly instantly. A pin (19) selectively locks button (18) to avoid premature firing of PETDD (10), such that the operator must remove pin (19) before intentionally firing PETDD (10).

[0034] By way of example only, PETDD (10) may be constructed and operable in accordance with at least some of the teachings of U.S. Patent No. 8,052,693, the disclosure of

which is incorporated by reference herein; U.S. Patent No. 8,249,700, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2011/0015645, the disclosure of which is incorporated by reference herein; and/or U.S. Pub. No. 2014/0276906, entitled “Features to Improve and Sense Tympanic Membrane Apposition by Tympanostomy Tube Delivery Instrument,” filed on even date herewith, the disclosure of which is incorporated by reference herein. Other suitable forms that PETDD (10) may take will be apparent to those of ordinary skill in the art in view of the teachings herein. It should also be understood that a PE tube may be inserted in a tympanic membrane (TM) manually, such as by creating the myringotomy incision with a knife and inserting the PE tube using forceps, etc.

[0035] FIGS. 2-3 show an exemplary PE tube (20) that may be delivered to the tympanic membrane (TM) using PETDD (10). PE tube (20) of this example comprises a cylindraceous body (22) that defines a passageway (24). A flange (26) is located at one end of body (22) while a set of petals (28) are located at the other end of body (22). PE tube (20) is formed of a resilient material that is biased to assume the rivet like configuration shown in FIGS. 2-3. However, flange (26) and petals (28) may be flexed inwardly toward the longitudinal axis of body (22) to provide PE tube (20) with a cylindraceous configuration. In particular, flange (26) and petals (28) may be flexed such that their outer surfaces are at the same radial distance from the longitudinal axis as the outer perimeter of body (22). This may enable PE tube (200) to collapse to fit within cannula (14). When PE tube (20) is disposed in a tympanic membrane (TM), petals (28) are located medially (i.e., on the middle ear side) while flange (26) is located laterally (i.e., on the outer ear side).

[0036] By way of example only, PE tube (20) may also be configured in accordance with at least some of the teachings of U.S. Pat. No. 9,011,363, entitled “Tympanic Membrane Pressure Equalization Tube,” issued April 21, 2015, the disclosure of which is incorporated by reference herein; and/or at least some of the teachings U.S. Pub. No. 2014/0276906, the disclosure of which is incorporated by reference herein. Other suitable forms that PE tube (20) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

II. Exemplary Iontophoresis System

[0037] As noted above, PETDD (10) may be used in conjunction with an iontophoresis system, which may be used to anesthetize the patient’s ear before PETDD (10) is inserted

into the patient's ear canal to deliver PE tube (20) in the tympanic membrane (TM). By way of example only, iontophoresis may be provided in accordance with at least some of the teachings of U.S. Pub. No. 2010/0198135, the disclosure of which is incorporated by reference herein; and/or in accordance with at least some of the teachings of U.S. Patent No. 8,192,420, the disclosure of which is incorporated by reference herein. In addition or in the alternative, iontophoresis may be provided in accordance with any of the various teachings below. It should be understood that any of the below teachings may be readily combined with at least some of the teachings of U.S. Pub. No. 2010/0198135, the disclosure of which is incorporated by reference herein; and/or at least some of the teachings of U.S. Patent No. 8,192,420, the disclosure of which is incorporated by reference herein.

[0038] FIG. 4 shows one merely illustrative iontophoresis system (200). Iontophoresis system (200) of this example comprises an earplug (220), fluid source (140), control unit (170), and ground pad (180). Earplug (220) is configured to be inserted into a patient's ear and remain there without needing a separate component like a headframe to hold it in place. By way of example only, a biocompatible adhesive may be used to assist in holding earplug (220) in place within a patient's ear canal. Earplug (220) includes a pair of gripping features (222) that are configured to be gripped and thereby serve as a handle during insertion of earplug (220) in a patient's ear. Earplug (220) also includes a pull-tab (228) that may be gripped and pulled to assist in removing earplug (220) from the patient's ear. Of course, these features are mere examples, and any other suitable kinds of gripping features may be incorporated into earplug (220). While only one earplug (220) is shown, it should be understood that iontophoresis system (200) may have two earplugs (220) that may be used simultaneously.

[0039] In some versions, earplug (220) is configured and operable in accordance with at least some of the teachings of U.S. Pub. No. 2014/0102461, entitled "Adhesive Earplugs Useful for Sealing the Ear Canal," published April 17, 2014, the disclosure of which is incorporated by reference herein. As best seen in FIG. 5, earplug (220) of the present example includes a flexible sealing element (224) and a distally projecting nozzle (226). Sealing element (224) is configured to provide a fluid tight seal against the patient's ear canal when earplug (220) is inserted in the patient's ear canal. In some instances, and as noted above, a biocompatible pressure sensitive adhesive is applied to the outer surface of sealing element (224) to promote a fluid tight seal against the patient's ear canal. Nozzle (226) is positioned to project into the

patient's ear canal when earplug (220) is inserted in the patient's ear canal, such that nozzle (226) is spaced lateral to the tympanic membrane (TM). Nozzle (226) has spray apertures (227) and is secured to the distal end of a semi-rigid post (225). Post (225) provides a path for fluid communication from conduit (230) to spray apertures (227). Spray apertures (227) are thus in fluid communication with fluid source (140) via post (225) and conduit (230).

[0040] Sealing element (224) is secured to a rigid frame (223), which defines gripping features (222). Sealing element (224) and frame (223) also together define a working channel (221). Frame (223) defines a plurality of vent paths (229) in fluid communication with working channel (221). Vent paths (229) are configured to allow air to escape working channel (221) while working channel (221) fills with iontophoresis solution; yet are further configured prevent iontophoresis solution from escaping working channel (221) via vent paths (229) once working channel (221) is filled with iontophoresis solution. An iontophoresis electrode (252) in the form of a coil extends along at least part of the length of working channel (221). It should be understood that iontophoresis electrode (252) may have any other suitable configuration. Iontophoresis electrode (252) is coupled with control unit (170) via a cable (250) and is thereby operable to be activated with a positive voltage as described above. Thus, control unit (170) may activate iontophoresis electrode (252) to provide an electrorepulsive force to the iontophoresis solution ions delivered through apertures (227), to drive the anesthetic of the iontophoresis solution ions into the tympanic membrane (TM) for anesthetization of the tympanic membrane (TM) as described above.

[0041] It should be understood that the above described iontophoresis system (200) may be varied in numerous ways. Several examples of how iontophoresis system (200) may be varied will be described in greater detail below, while still other examples will be apparent to those of ordinary skill in the art in view of the teachings herein. While the various iontophoresis systems described herein have been mentioned in relation to PETDD (10) and PE tube (20) delivery, it should be understood that any of the iontophoresis systems described herein may be used before a manual delivery of a PE tube (20), such that the iontophoresis systems described herein do not necessarily need to be used in conjunction with a PETDD (10). It should also be understood that iontophoresis systems may be used in various other clinical contexts, such that the iontophoresis systems described herein do not necessarily need to be used in the context of a PE tube (20) delivery or in other procedures in a patient's ear. The teachings herein may be readily applied to iontophoresis systems that are used in various

other procedures and in various other parts of the human anatomy. Alternative systems and settings in which the teachings herein may be applied will be apparent to those of ordinary skill in the art.

III. Exemplary Fluid Flow Variations for Iontophoresis System

[0042] As noted above, vent paths (229) of earplug (220) are configured to allow air to escape working channel (221) while working channel (221) and the patient's ear canal fills with iontophoresis solution. In some instances, it may be desirable to relocate and/or modify the structure associated with vent paths (229). In particular, there may be instances during use of earplug (220) where iontophoresis solution escapes through vent paths (229) and leaves a proximal portion of iontophoresis electrode (252) exposed to air. For instance, if the patient talks, coughs, swallows, cries, yawns, or otherwise moves their lower jaw, the motion associated with such activity may cause variation in the effective volume of the patient's ear canal. This variation of the effective volume of the patient's ear canal may in turn drive at least some iontophoresis solution through vent paths (229). The resulting exposure of even just a portion of iontophoresis electrode (252) to air may adversely affect the iontophoretic performance of earplug (220). In instances where the entire iontophoresis electrode (252) is left exposed to air, the iontophoresis procedure may be completely interrupted until the physician injects more iontophoresis solution into earplug (220).

[0043] It may therefore be desirable to relocate and/or modify the structure associated with vent paths (229) in order to provide greater tolerance to variations in the effective volume of the patient's ear canal, to thereby reduce the risk of even a portion of iontophoresis electrode (252) being exposed to air during an iontophoresis procedure. The following example includes a variation of earplug (220) where the vent path is relocated. However, it should be understood that the following example is merely illustrative. Other suitable variations will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0044] FIG. 6 depicts another exemplary iontophoresis system (300) that may be used to anesthetize a patient's tympanic membrane (TM), such as before a inserting a PE tube (20) into the tympanic membrane (TM) as described above. Iontophoresis system (300) of this example is substantially similar to iontophoresis system (200) described above, except where otherwise noted herein. Iontophoresis system (300) comprises an earplug (320), which is substantially similar to earplug (220) described above, except earplug (320) is generally

configured to provide improved management of fluid flow in response to volumetric changes in a patient's ear during an iontophoresis procedure. Like with earplug (220), earplug (320) is in communication with fluid source (140) via a conduit (330) that is in the form of flexible tubing. Also like with earplug (220), earplug (320) is in communication with control unit (170) and ground pad (180) via a cable (350). Conduit (330) and cable (350) are coupled together along a shared length extending between a clip (340) and earplug (320). Clip (340) is operable to selectively secure the combination of conduit (330) and cable (350) to the patient's clothing and/or to any other suitable structure.

[0045] Earplug (320) is configured to be inserted into a patient's ear and remain there without needing a separate component like a headframe to hold it in place. As will be described in greater detail below, a biocompatible pressure sensitive adhesive is be used to assist in holding earplug (320) in place within a patient's ear canal. Earplug (320) includes a gripping feature (322) that is configured to be gripped and thereby serve as a handle during insertion of earplug (320) in a patient's ear. Earplug (320) also includes a pull-tab (328) that may be gripped and pulled to assist in removing earplug (320) from the patient's ear. Of course, these features are merely illustrative examples, and any other suitable kinds of gripping features may be incorporated into earplug (320). While only one earplug (320) is shown, it should be understood that iontophoresis system (300) may have two earplugs (320) that may be used in both of the patient's ears simultaneously or in a sequence.

[0046] As best seen in FIGS. 7-8, earplug (320) of the present example includes a flexible sealing element (324) and a distally projecting nozzle (326). Sealing element (324) is configured to provide a fluid tight seal against the patient's ear canal when earplug (320) is inserted in the patient's ear canal. In the present example, a pressure sensitive adhesive is applied to the outer surface of sealing element (324) to promote a fluid tight seal against the patient's ear canal. Nozzle (326) is positioned to project into the patient's ear canal when earplug (320) is inserted in the patient's ear canal, such that nozzle (326) is spaced lateral to the tympanic membrane (TM). Nozzle (326) has a plurality of spray apertures (327) and is secured to the distal end of a semi-rigid post (325). Post (325) defines a lumen providing a path for communication of fluid from conduit (330) to spray apertures (327). Spray apertures (327) are thus in fluid communication with fluid source (140) via post (325) and conduit (330). Sealing element (324) is secured to a rigid frame (323). Sealing element (324) and

frame (323) together define a working channel (321), as will be described in greater detail below.

[0047] Gripping feature (322) is fixedly secured to rigid frame (323). Gripping feature (322) and frame (323) cooperate to define a reservoir (370). Reservoir (370) is in fluid communication with working channel (321). Reservoir (370) extends laterally relative to a longitudinal axis defined by post (325). Thus, reservoir (370) and working channel (321) together form an L-shaped cavity. As will be described in greater detail below, this L-shaped cavity operates to maintain fluid contact with iontophoresis electrode (352) even when a patient's ear canal experiences volumetric changes throughout the iontophoresis procedure. Frame (323) also defines at least one vent path (329), which is also in fluid communication with reservoir (370). Vent path (329) is configured to allow air to escape reservoir (370) when reservoir (370) fills with iontophoresis solution, as will be described in greater detail below. In the present example, vent path (329) is formed as a circular opening with a diameter of approximately 0.025 inches. Alternatively, vent path (329) may have any other suitable size or configuration.

[0048] An iontophoresis electrode (352) in the form of a coil extends along at least part of the length of working channel (321). It should be understood that iontophoresis electrode (352) may have any other suitable configuration. Iontophoresis electrode (352) is coupled with control unit (170) via cable (350) and is thereby operable to be activated with a positive voltage as described above. Thus, control unit (170) may activate iontophoresis electrode (352) to provide an electrorepulsive force to the iontophoresis solution ions delivered through apertures (327), to drive the anesthetic of the iontophoresis solution ions into the tympanic membrane (TM) for anesthetization of the tympanic membrane (TM) as described above.

[0049] Unlike earplug (220) described above, earplug (320) of the present example is configured to tolerate volumetric changes in a patient's ear during an iontophoresis procedure without letting iontophoresis electrode (352) become exposed to air. In particular, reservoir (370) of the present example is configured to effectively increase the volume of working channel (321), thereby providing a spacing between vent path (329) and iontophoresis electrode (352) that is greater than the spacing between vent paths (229) and iontophoresis electrode (252). In the present example, reservoir (370) and working channel (321) provide a combined volume that is about three times that of working channel (221) described above. In some other examples, reservoir (370) and working channel (321) provide a combined volume

that is between about two times and about four times that of working channel (221). Of course, reservoir (370) and working channel (321) may instead provide any other suitable combined volume in relation to the volume of working channel (221).

[0050] Unlike earplug (220) described above, earplug (320) of the present example is configured such that vent path (329) is repositioned for management of fluid flow in response to volumetric changes in a patient's ear canal. As can be seen, vent path (329) of the present example is positioned adjacent to reservoir (370) at the furthest lateral point of reservoir (370). As will be described in greater detail below, the above described positioning of vent path (329) directs fluid out of reservoir (370) such that any open space created by displaced fluid remains within reservoir (370). Although vent path (329) of the present example is shown as being integral with an opening for conduit (330), it should be understood that in other examples vent path (329) is a discrete opening in gripping feature (322), spaced away from the point at which conduit (330) enters gripping feature (322).

[0051] FIGS. 9-15 show a merely illustrative use of earplug (320). As can be seen in FIG. 9, earplug (320) is initially positioned outside of a patient's ear. At this stage, fluid has not yet been injected into earplug (320). The operator may begin the iontophoresis procedure by inserting sealing element (324) of earplug (320) into a patient's ear canal (EC). As can be seen in FIG. 10, sealing element (324) is positioned to bear against the walls of the ear canal (EC), simultaneously securing earplug (320) and creating a fluid seal between sealing element (324) and the wall of the ear canal (EC). The sealing of the ear canal (EC) creates a fluid tight cavity between tympanic membrane (TM) and earplug (320) that may be used to contain iontophoresis fluid. While not shown in FIGS. 9-10, a liner strip (380) as described below may be used to assist the operator in positioning earplug (320) in the ear canal (EC) without the operator's fingers getting stuck to the pressure sensitive adhesive on sealing element (324).

[0052] Once earplug (320) is secured in the patient's ear canal (EC), the operator may begin administration of iontophoresis fluid (390) to the ear canal (EC) via conduit (330) and nozzle (326), as can be seen in FIG. 11. As fluid (390) is administered, the ear canal (EC), working channel (321) and reservoir (370) will fill with fluid (390); and the air displaced from the ear canal (EC), working channel (321) and reservoir (370) will flow out to the atmosphere through vent path (329). The operator may continue administering fluid (390) until fluid (390) is observed flowing out through vent path (329) as shown in FIG. 12. Once fluid flows

through vent path (329), the ear canal (EC), working channel (321), reservoir (370) are full of fluid (390) and earplug (320) is ready to activate iontophoresis electrode (352) to thereby provide an electrorepulsive force to the iontophoresis fluid ions. In some versions, gripping feature (322) is transparent, enabling the operator to visually observe reservoir (370) filling with fluid (390). This may enable the operator to be more ready to cease injecting fluid (390) via conduit (330) when the level of fluid (390) reaches vent path (329).

[0053] Prior to activation of electrode (352), the operator may remove a fluid delivery device (not shown) such as a syringe from conduit (330). It should be understood that in some circumstances removal of such a device may result in some loss of fluid (390) from working channel (321). By way of example only, in some examples this may result in a loss of about 0.04 cc of fluid (390). As a result, an air pocket (392) of a corresponding volume may form adjacent to vent path (329) in reservoir (370), as shown in FIG. 13. It should be understood that this air pocket (392) is substantially spaced away from iontophoresis electrode (352), such that iontophoresis electrode (352) remains fully submerged in fluid (390) with no meaningful risk of any portion of electrode (352) being exposed to air.

[0054] During the iontophoresis procedure, the patient may talk, cough, swallow, cry, yawn, or otherwise move their lower jaw, and the motion associated with such activity may cause variation in the effective volume of the patient's ear canal (EC). Such volumetric changes may cause a pumping action, which will vary the level of fluid (390) in reservoir (370). In some instances, this variation of the level of fluid (390) may displace fluid (390) out of vent path (329), as shown in FIG. 14. As fluid (390) is displaced out of vent path (329) the volume of fluid (390) disposed in the ear canal (EC), working channel (321), reservoir (370) is reduced by a corresponding amount. As can be seen in FIG. 15, such a reduction in fluid (390) will correspondingly cause the air pocket (392) in reservoir (370) to expand and contract. Even with further volumetric changes in the patient's ear canal (EC), the air pocket (392) may eventually reach a point where fluid (390) stops leaking from vent path (329) and the size of air pocket (392) simply expands and contracts in response to the volumetric changes in the patient's ear canal (EC). Because of the volume and L-shape provided by reservoir (370), the air pocket (392) will remain positioned exclusively in reservoir (370) instead of extending to the remainder of working channel (321) or the ear canal (EC). Thus, reservoir (370) maintains complete contact between fluid (390) and electrode (352),

preventing exposure of electrode (352) to air, thereby maintaining full electrical conductivity between fluid (390) and electrode (352).

[0055] In some instances earplug (320) may be used in an inverted position (i.e., at a vertical orientation). In particular, the operator may wish to insert earplug (320) in a patient's ear while the patient's head is oriented toward the ground. During such an operation, reservoir (370) and vent path (329) may generally provide the same function as described above but with different positioning of the air in reservoir (370). As can be seen in FIG. 16, with earplug (320) positioned vertically, an air bubble (394) is disposed within reservoir (370) away from vent path (329). Surface tension at the interface between the air bubble (394) and the fluid (390) keeps the air bubble (394) within reservoir (370) and away from the rest of working channel (321). Similarly, surface tension between fluid (390) and vent path (329) maintains fluid (390) within reservoir (370), while permitting some fluid (390) to be released in response to volumetric changes in the ear canal (EC). It should be understood that to maintain the air bubble (394) in the position shown the interface between reservoir (370) and the remainder of working channel (321) is sized to correspond to the size of the air bubble (394). Additionally, the extension of post (325) though working channel (321) further reduces the size of working channel (321) to further prevent any travel of the air bubble (394).

IV. Exemplary Liner Strip for Use with Earplug

[0056] As noted above, a pressure sensitive adhesive may be provided on sealing element (324) in order to provide a more secure and fluid tight fit between sealing element (324) and the wall of the patient's ear canal (EC). It may be desirable to provide a feature that facilitates gripping and positioning of earplug (320) without the operator's fingers getting stuck to the pressure sensitive adhesive on sealing element (324). To that end, earplug (320) of the present example includes a liner strip (380).

[0057] FIGS. 17-19 show liner strip (380) in greater detail. As can be seen, liner strip (380) of the present example is constructed as a single generally flat part having a shape generally resembling an imperial moustache, or (when turned 180° from the view in FIG. 17) a handlebar mustache. At least a portion of liner strip (380) is coated with fluoro-silicone, providing a low-tack release surface that facilitates peeling of liner strip (380) away from the pressure sensitive adhesive on sealing element (324). Liner strip (380) itself comprises a

generally flexible 0.0009 inch thick polyethylene terephthalate (PET) film. Alternatively, liner strip (380) may comprise a variety of other suitable materials having a range of thicknesses.

[0058] The shape of liner strip (380) divides liner strip (380) into four discrete portions (382, 383, 384, 385). In particular, liner strip (380) may be folded along three fold lines (shown in broken lines in FIG. 17) to more readily define each portion (382, 383, 384, 385). When folded, liner strip (380) defines two attachment portions (382, 383) and two gripping portions (384, 385). As can best be seen in FIG. 18, attachment portions (382, 383) are folded in a reverse direction to define a surface suitable for attachment of liner strip (380) to opposing sides of sealing element (324). In the present example, each attachment portion (382, 383) is also heat formed to define a slight curvature in each attachment portion (382, 383). The curvature of each attachment portion (382, 383) is entirely optional and may be omitted in some examples. However, where used, the curvature of attachment portions (382, 383) corresponds to the curvature of flexible sealing element (324) of earplug (320) to promote full apposition between attachment portions (382, 383) and sealing element (324).

[0059] As seen in FIG. 18 and 19, each gripping portion (384, 385) extends proximally away from each respective attachment portion (382, 383). In particular, each gripping portion comprises a corresponding thin portion (386, 387) and thick portion (388, 389). Each thin portion (386, 387) curves laterally away from each attachment portion (382, 383) to orient each respective thick portion (388, 389) away from earplug (320). This feature permits thick portions (388, 389) to be used for grasping by a user to manipulate earplug (320) by grasping liner strip (380).

[0060] As can be seen in FIG. 19, liner strip (380) is placed on earplug (320) such that attachment portions (382, 383) are positioned about sealing element (324) at angular locations corresponding to the posterior and anterior walls of a patient's ear canal (EC). In some instances, this positioning corresponds to the areas of flexible sealing element (324) that will encounter the most resistance from a patient's ear canal (EC) during insertion of earplug (320). Such positioning may be desirable to ensure that the pressure sensitive adhesive on sealing element (324) fully engages the superior and inferior walls of the patient's ear canal (EC) before the pressure sensitive adhesive on sealing element (324) contacts the posterior and anterior walls of the patient's ear canal (EC). Once earplug (320) is inserted into the ear canal (EC) far enough for sealing element (324) to fully engage the

posterior and anterior walls of the patient's ear canal (EC), the operator may peel away liner strip (380) to allow the pressure sensitive adhesive on sealing element (324) to contact the posterior and anterior walls of the patient's ear canal (EC). At this stage, the pressure sensitive adhesive on sealing element (324) may contact the walls of the ear canal (EC) about the entire angular perimeter of sealing element (324). Liner strip (380) may then be disposed of.

[0061] In the present example, the pressure sensitive adhesive is provided about the entire angular perimeter of sealing element (324). Also in the present example, attachment portions (382, 383) are together sized to contact approximately 40% of the surface of sealing element (324) that is coated with pressure sensitive adhesive. Alternatively, attachment portions (382, 383) may cover any other suitable portion of the surface of sealing element (324) that is coated with pressure sensitive adhesive. It should also be understood that pressure sensitive adhesive may be provided about only a portion of the angular perimeter of sealing element (324). For instance, earplug (320) may be configured such that pressure sensitive adhesive is only provided on the zones of sealing element (324) that will contact posterior and anterior walls of the patient's ear canal (EC); but not on the zones of sealing element (324) that will contact posterior and anterior walls of the patient's ear canal (EC).

[0062] As another merely illustrative example, a lubricious material (e.g., alcohol, etc.), may be applied to the pressure sensitive adhesive on sealing element (324) to aid in insertion of sealing element (324) in the ear canal (EC); with the lubricious material being configured to evaporate or otherwise dissipate to enable the pressure sensitive adhesive to adhere to the walls of the ear canal (EC) shortly after sealing element (324) is inserted in the ear canal (EC). Still other suitable variations will be apparent to those of ordinary skill in the art in view of the teachings herein.

V. Exemplary Combinations

[0063] The following examples relate to various non-exhaustive ways in which the teachings herein may be combined or applied. It should be understood that the following examples are not intended to restrict the coverage of any claims that may be presented at any time in this application or in subsequent filings of this application. No disclaimer is intended. The following examples are being provided for nothing more than merely illustrative purposes. It is contemplated that the various teachings herein may be arranged and applied in numerous

other ways. It is also contemplated that some variations may omit certain features referred to in the below examples. Therefore, none of the aspects or features referred to below should be deemed critical unless otherwise explicitly indicated as such at a later date by the inventors or by a successor in interest to the inventors. If any claims are presented in this application or in subsequent filings related to this application that include additional features beyond those referred to below, those additional features shall not be presumed to have been added for any reason relating to patentability.

Example 1

[0064] An apparatus comprising: (a) a rigid body, wherein the rigid body defines: (i) a channel, (ii) reservoir in fluid communication with the channel, and (ii) vent path in fluid communication with the reservoir, wherein the reservoir is configured to provide spacing between the channel and the vent path; (b) a flexible sealing element, wherein the sealing element is positioned distal to the rigid body; (c) a nozzle assembly, wherein the nozzle assembly comprises: (i) a nozzle head, and (ii) a post, wherein the post extends distally through the channel of the rigid body, wherein the nozzle head projects distally from a distal end of the post; and (d) an electrode, wherein the electrode is disposed within the channel of the rigid body, wherein the reservoir extends laterally from a longitudinal axis defined by the electrode.

Example 2

[0065] The apparatus of Example 1, wherein the electrode terminates at a proximal end, wherein the proximal end of the electrode is distal to the reservoir.

Example 3

[0066] The apparatus of any one or more of Examples 1 through 2, wherein the channel and the reservoir together define an L-shape.

Example 4

[0067] The apparatus of any one or more of Examples 1 through 3, wherein the channel extends distally relative to the reservoir, wherein the vent path extends laterally relative to the reservoir.

Example 5

[0068] The apparatus of any one or more of Examples 1 through 4, wherein the sealing element is configured to bear against a wall of an ear canal to thereby define a closed volume outside of a tympanic membrane in the ear canal.

Example 6

[0069] The apparatus of Example 5, wherein the reservoir is in configured to communicate with the closed volume through the channel.

Example 7

[0070] The apparatus of Example 6, wherein the vent path is configured to release excess fluid from the reservoir in response to filling of the closed volume, the channel, and the reservoir with fluid.

Example 8

[0071] The apparatus of any one or more of Examples 6 through 7, wherein the reservoir is configured to provide an air pocket between fluid and the vent path as the closed volume, the channel, and the reservoir are filled with fluid, wherein the channel is configured to maintain submersion of the electrode in the fluid while the air pocket resides in the reservoir.

Example 9

[0072] The apparatus of any one or more of Examples 5 through 8, further comprising a fluid conduit, wherein the fluid conduit is in communication with the channel, wherein the fluid conduit is configured to fill the closed volume, the channel, and the reservoir with fluid.

Example 10

[0073] The apparatus of Example 9, wherein the fluid conduit extends through a conduit opening disposed in the rigid body.

Example 11

[0074] The apparatus of Example 10, wherein the conduit opening and vent path are integral with each other.

Example 12

[0075] The apparatus of any one or more of Examples 10 through 11, wherein the conduit opening and the vent path are separately formed as discrete openings in the rigid body.

Example 13

[0076] The apparatus of any one or more of Examples 1 through 12, further comprising a flexible fluid conduit fluidly coupled with the post, wherein the post is configured to communicate fluid from the fluid conduit to the nozzle head.

Example 14

[0077] The apparatus of any one or more of Examples 1 through 13, further comprising a pressure sensitive adhesive applied to the sealing element.

Example 15

[0078] The apparatus of Example 14, further comprising a liner strip, wherein the liner strip comprises a pair of attachment portions secured to the pressure sensitive adhesive on the sealing element.

Example 16

[0079] The apparatus of Example 15, wherein the sealing element defines an anterior zone, a posterior zone, a superior zone, and an inferior zone, wherein the attachment portions are configured to engage only the anterior and posterior zones of the sealing element, wherein the attachment portions are configured to not engage the superior and inferior zones of the sealing element.

Example 17

[0080] An apparatus, comprising: (a) an iontophoresis fluid reservoir, wherein the fluid reservoir defines a first volume; (b) a plug configured to define a closed volume in a patient's ear canal outside a tympanic membrane of the patient; (c) a working conduit configured to connect the iontophoresis fluid reservoir with the closed volume, wherein the working conduit defines a second volume; and (d) a drainage conduit passing from the fluid reservoir to a region outside the closed volume and plug; wherein the reservoir, plug, working conduit,

and drainage conduit are configured to supply iontophoresis fluid through the working conduit, wherein the first volume of the fluid reservoir is greater than the second volume of the working conduit.

Example 18

[0081] An apparatus, comprising: (a) a plug configured to define a closed volume in a patient's ear canal outside a tympanic membrane of the patient, wherein the plug defines a channel configured to communicate with the closed volume, wherein the plug further includes a sealing element having a pressure sensitive adhesive thereon; (b) an iontophoresis electrode situated in the channel; and (c) a liner strip, wherein the liner strip comprises: (i) a pair of attachment portions, wherein each attachment portion is defined by a corresponding fold in the liner strip, wherein each attachment portion is configured cover two discrete portions the pressure sensitive adhesive on the sealing element, and (ii) a pair of gripping portions, wherein each gripping portion is defined by a fold in the liner strip, wherein each attachment portion is disposed on a distal end of a respective gripping portion.

Example 19

[0082] The apparatus of Example 18, wherein the attachment portions extend proximally from corresponding distal ends of the gripping portions.

Example 20

[0083] The iontophoresis apparatus of any one or more of Examples 18 through 19, wherein each attachment portion comprises a generally curved shape contoured to complement a curvature of the sealing element.

VI. Miscellaneous

[0084] It should be understood that any of the examples described herein may include various other features in addition to or in lieu of those described above. By way of example only, any of the devices herein may also include one or more of the various features disclosed in any of the various references that are incorporated by reference herein. It should also be understood that any one or more of the teachings, expressions, embodiments, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, embodiments, examples, etc. that are described herein. The above-described teachings,

expressions, embodiments, examples, etc. should therefore not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

[0085] It should be appreciated that any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated material does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

[0086] Versions described above may be designed to be disposed of after a single use, or they can be designed to be used multiple times. Versions may, in either or both cases, be reconditioned for reuse after at least one use. Reconditioning may include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, some versions of the device may be disassembled, and any number of the particular pieces or parts of the device may be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, some versions of the device may be reassembled for subsequent use either at a reconditioning facility, or by a user immediately prior to a procedure. Those skilled in the art will appreciate that reconditioning of a device may utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

[0087] By way of example only, versions described herein may be sterilized before and/or after a procedure. In one sterilization technique, the device is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and device may then be placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation may kill bacteria on the device and in the container. The sterilized device may then be stored in the sterile container for later use. A device may also

be sterilized using any other technique known in the art, including but not limited to beta or gamma radiation, ethylene oxide, or steam.

[0088] While various inventive embodiments have been described and illustrated herein, those of ordinary skill in the art will readily envision a variety of other means and/or structures for performing the function and/or obtaining the results and/or one or more of the advantages described herein, and each of such variations and/or modifications is deemed to be within the scope of the inventive embodiments described herein. More generally, those skilled in the art will readily appreciate that all parameters, dimensions, materials, and configurations described herein are meant to be exemplary and that the actual parameters, dimensions, materials, and/or configurations will depend upon the specific application or applications for which the inventive teachings is/are used. Those skilled in the art will recognize, or be able to ascertain using no more than routine experimentation, many equivalents to the specific inventive embodiments described herein. It is, therefore, to be understood that the foregoing embodiments are presented by way of example only and that, within the scope of the appended claims and equivalents thereto; inventive embodiments may be practiced otherwise than as specifically described and claimed. Inventive embodiments of the present disclosure are directed to each individual feature, system, article, material, kit, and/or method described herein. In addition, any combination of two or more such features, systems, articles, materials, kits, and/or methods, if such features, systems, articles, materials, kits, and/or methods are not mutually inconsistent, is included within the inventive scope of the present disclosure.

[0089] Also, various inventive concepts may be embodied as one or more methods, of which an example has been provided. The acts performed as part of the method may be ordered in any suitable way. Accordingly, embodiments may be constructed in which acts are performed in an order different than illustrated, which may include performing some acts simultaneously, even though shown as sequential acts in illustrative embodiments.

[0090] All definitions, as defined and used herein, should be understood to control over dictionary definitions, definitions in documents incorporated by reference, and/or ordinary meanings of the defined terms.

[0091] The indefinite articles “a” and “an,” as used herein in the specification and in the claims, unless clearly indicated to the contrary, should be understood to mean “at least one.”

[0092] The phrase “and/or,” as used herein in the specification and in the claims, should be understood to mean “either or both” of the elements so conjoined, i.e., elements that are conjunctively present in some cases and disjunctively present in other cases. Multiple elements listed with “and/or” should be construed in the same fashion, i.e., “one or more” of the elements so conjoined. Other elements may optionally be present other than the elements specifically identified by the “and/or” clause, whether related or unrelated to those elements specifically identified. Thus, as a non-limiting example, a reference to “A and/or B”, when used in conjunction with open-ended language such as “comprising” can refer, in one embodiment, to A only (optionally including elements other than B); in another embodiment, to B only (optionally including elements other than A); in yet another embodiment, to both A and B (optionally including other elements); etc.

[0093] As used herein in the specification and in the claims, “or” should be understood to have the same meaning as “and/or” as defined above. For example, when separating items in a list, “or” or “and/or” shall be interpreted as being inclusive, i.e., the inclusion of at least one, but also including more than one, of a number or list of elements, and, optionally, additional unlisted items. Only terms clearly indicated to the contrary, such as “only one of” or “exactly one of,” or, when used in the claims, “consisting of,” will refer to the inclusion of exactly one element of a number or list of elements. In general, the term “or” as used herein shall only be interpreted as indicating exclusive alternatives (i.e. “one or the other but not both”) when preceded by terms of exclusivity, such as “either,” “one of,” “only one of,” or “exactly one of.” “Consisting essentially of,” when used in the claims, shall have its ordinary meaning as used in the field of patent law.

[0094] As used herein in the specification and in the claims, the phrase “at least one,” in reference to a list of one or more elements, should be understood to mean at least one element selected from any one or more of the elements in the list of elements, but not necessarily including at least one of each and every element specifically listed within the list of elements and not excluding any combinations of elements in the list of elements. This definition also allows that elements may optionally be present other than the elements specifically identified within the list of elements to which the phrase “at least one” refers, whether related or unrelated to those elements specifically identified. Thus, as a non-limiting example, “at least one of A and B” (or, equivalently, “at least one of A or B,” or, equivalently “at least one of A and/or B”) can refer, in one embodiment, to at least one, optionally including more than one,

A, with no B present (and optionally including elements other than B); in another embodiment, to at least one, optionally including more than one, B, with no A present (and optionally including elements other than A); in yet another embodiment, to at least one, optionally including more than one, A, and at least one, optionally including more than one, B (and optionally including other elements); etc.

[0095] In the claims, as well as in the specification above, all transitional phrases such as "comprising," "including," "carrying," "having," "containing," "involving," "holding," "composed of," and the like are to be understood to be open-ended, i.e., to mean including but not limited to. Only the transitional phrases "consisting of and "consisting essentially of shall be closed or semi-closed transitional phrases, respectively, as set forth in the United States Patent Office Manual of Patent Examining Procedures, Section 2111.03.

[0096] Having shown and described various embodiments of the present invention, further adaptations of the methods and systems described herein may be accomplished by appropriate modifications by one of ordinary skill in the art without departing from the scope of the present invention. Several of such potential modifications have been mentioned, and others will be apparent to those skilled in the art. For instance, the examples, embodiments, geometries, materials, dimensions, ratios, steps, and the like discussed above are illustrative and are not required. Accordingly, the scope of the present invention should be considered in terms of the following claims and is understood not to be limited to the details of structure and operation shown and described in the specification and drawings.

[0097] The reference in this specification to any prior publication (or information derived from it), or to any matter which is known, is not, and should not be taken as an acknowledgment or admission or any form of suggestion that that prior publication (or information derived from it) or known matter forms part of the common general knowledge in the field of endeavour to which this specification relates.

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. An apparatus comprising:
 - (a) a rigid body defining:
 - (i) a channel;
 - (ii) a reservoir in fluid communication with the channel, the reservoir and the channel providing a combined volume greater than a volume of the channel; and
 - (iii) a vent path in fluid communication with the reservoir; and
 - (iv) a conduit opening;
 - (b) an electrode defining a longitudinal axis and disposed within the channel of the rigid body, the reservoir extending laterally and proximally from the longitudinal axis defined by the electrode;
 - (c) a sealing element configured to bear against a wall of an ear canal to thereby define a closed volume outside of a tympanic membrane in the ear canal; and
 - (d) a fluid conduit in fluid communication with the channel to fill at least one of the closed volume, the channel, and the reservoir with fluid, the fluid conduit extending through the conduit opening defined by the rigid body.
2. The apparatus of claim 1, wherein the electrode terminates at a proximal end positioned distal to the reservoir.
3. The apparatus of claim 1 or claim 2, wherein the channel and the reservoir together define an L-shape.
4. The apparatus of any one of claims 1 to 3, wherein the channel extends distally from the reservoir, and the vent path extends laterally and proximally from the reservoir.

5. The apparatus of any one of claims 1 to 4, wherein the sealing element is positioned distal to the rigid body.
6. The apparatus of any one of claims 1 to 5, wherein the reservoir is configured to be in fluid communication with the closed volume through the channel.
7. The apparatus of claim 6, wherein the vent path is configured to release excess fluid from the reservoir when at least one of the closed volume, the channel, and the reservoir are filled with fluid.
8. The apparatus of claim 6 or claim 7, wherein the reservoir is configured to provide an air pocket between fluid and the vent path as at least one of the closed volume, the channel, and the reservoir are filled with fluid, and wherein the channel is configured to maintain submersion of the electrode in the fluid while the air pocket resides in the reservoir.
9. The apparatus of any one of claims 1 to 8, wherein the conduit opening and the vent path are integrally formed with each other in the rigid body.
10. The apparatus of any one of claims 1 to 8, wherein the conduit opening and the vent path are separately formed as discrete openings in the rigid body.
11. The apparatus of any one of claims 1 to 10, further comprising:
 - a nozzle assembly including a post extending through at least a portion of the channel and a nozzle head projecting distally from a distal end of the post; and
 - the fluid conduit fluidly coupled with the post to communicate fluid from a fluid source to the nozzle head.

12. The apparatus of any one of claims 1 to 11, further comprising a pressure sensitive adhesive provided on the sealing element.
13. The apparatus of claim 12, further comprising a liner strip including a plurality of attachment portions secured to the pressure sensitive adhesive on the sealing element.
14. The apparatus of any one of claims 1 to 13, further comprising a plug including the sealing element.
15. The apparatus of claim 12, further comprising:
 - a plug including the sealing element;
 - a liner strip positionable over the pressure sensitive adhesive to facilitate at least one of gripping and positioning the plug in the ear canal, the liner strip configured to be peeled away to allow the pressure sensitive adhesive to contact a wall surface of the wall of the ear canal after the plug is inserted into the ear canal and the sealing element is engaged with the wall surface of the ear canal.
16. The apparatus of claim 15, wherein the liner strip includes:
 - (i) a plurality of gripping portions, each gripping portion (1) defined by a different fold from a plurality of folds in the liner strip and (2) configured to extend proximally away from the plug; and
 - (ii) a plurality of attachment portions, each attachment portion (1) connected to a distal end of a gripping portion from the plurality of gripping portions, (2) defined by the fold in the liner strip that defines that gripping portion, and (3) configured to cover a discrete portion of the pressure sensitive adhesive disposed on the sealing element.

17. The apparatus of claim 16, wherein each attachment portion (4) extends proximally from the distal end of that gripping portion.
18. The apparatus of any one of claims 13, 16, 17, and claim 14 when dependent on claim 13, wherein the sealing element defines an anterior zone, a posterior zone, a superior zone, and an inferior zone, and wherein the attachment portions are configured to engage at least the anterior zone and the posterior zone of the sealing element.
19. The apparatus of any one of claims 1 to 18, wherein the reservoir and the channel provide a combined volume that is between about two times and about four times that of the channel.
20. The apparatus of any one of claims 1 to 19, wherein the fluid conduit is configured to supply the fluid through the reservoir and through the channel to the closed volume.

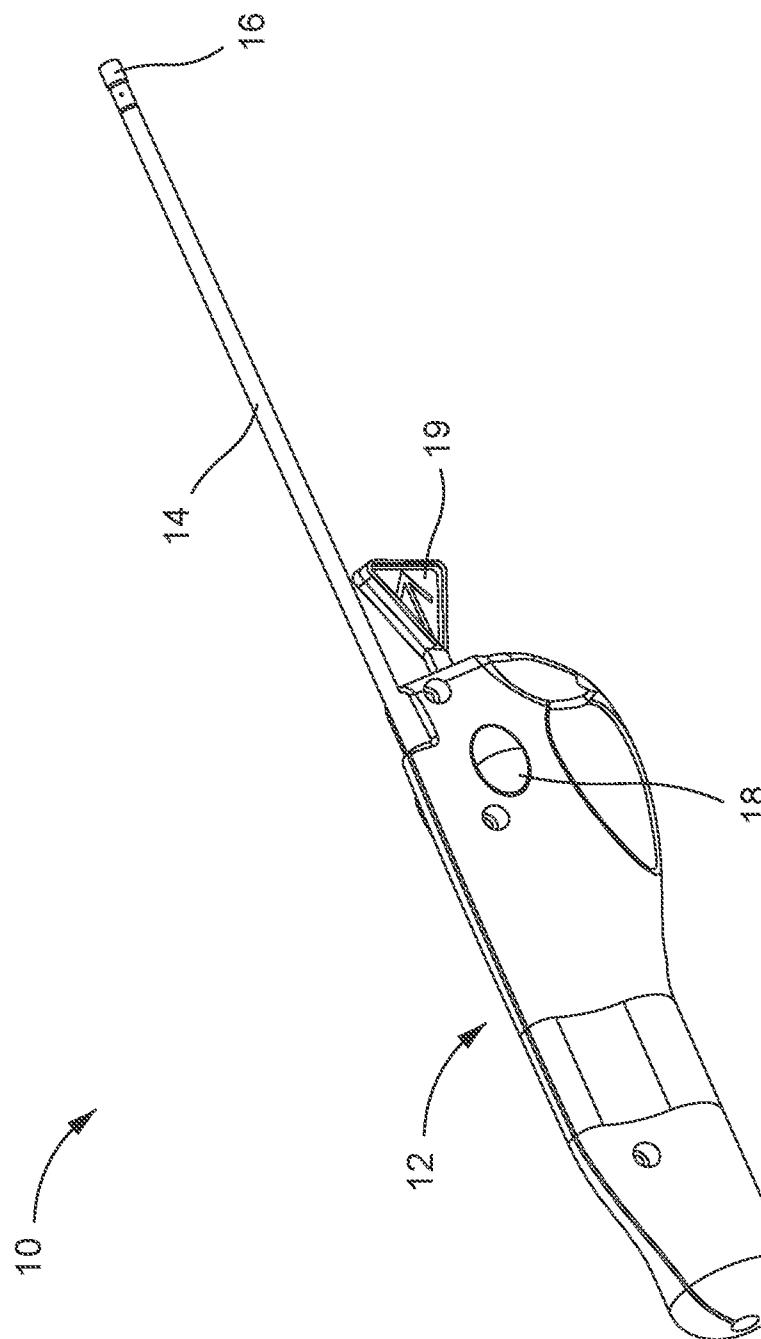


Fig. 1

2/18

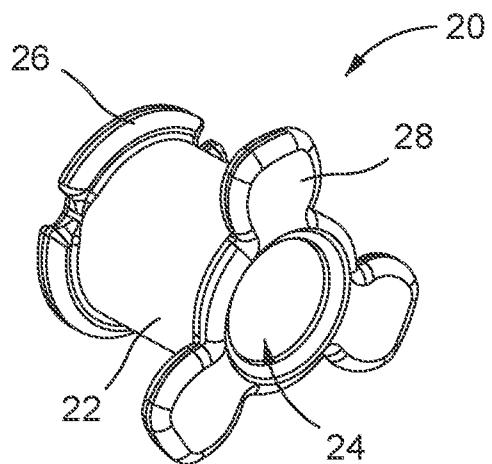


Fig. 2

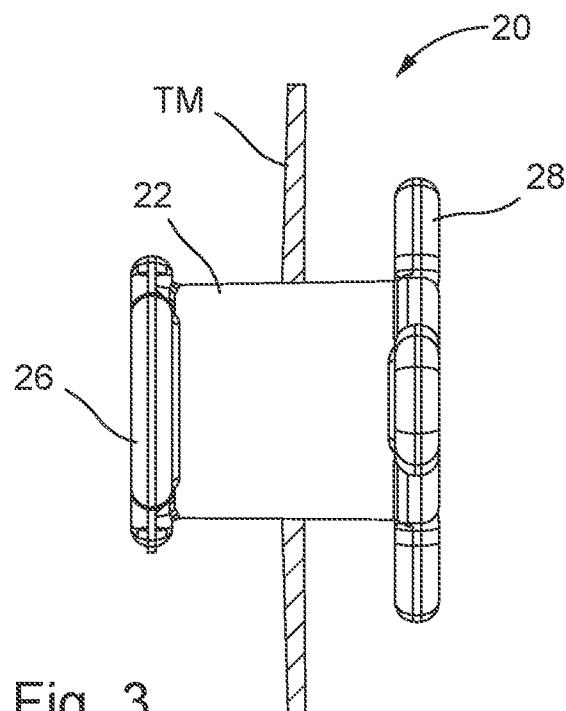
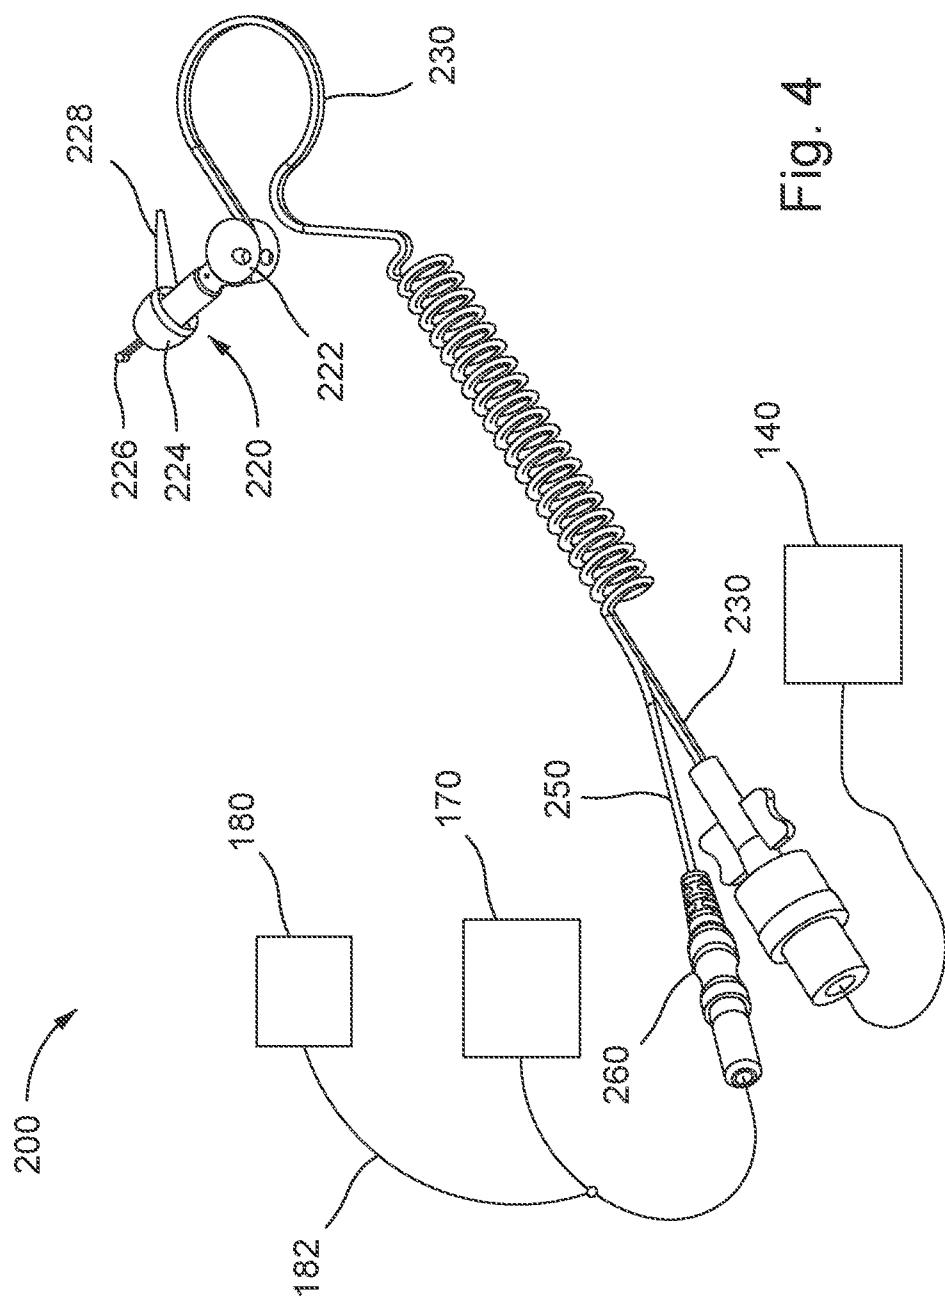


Fig. 3



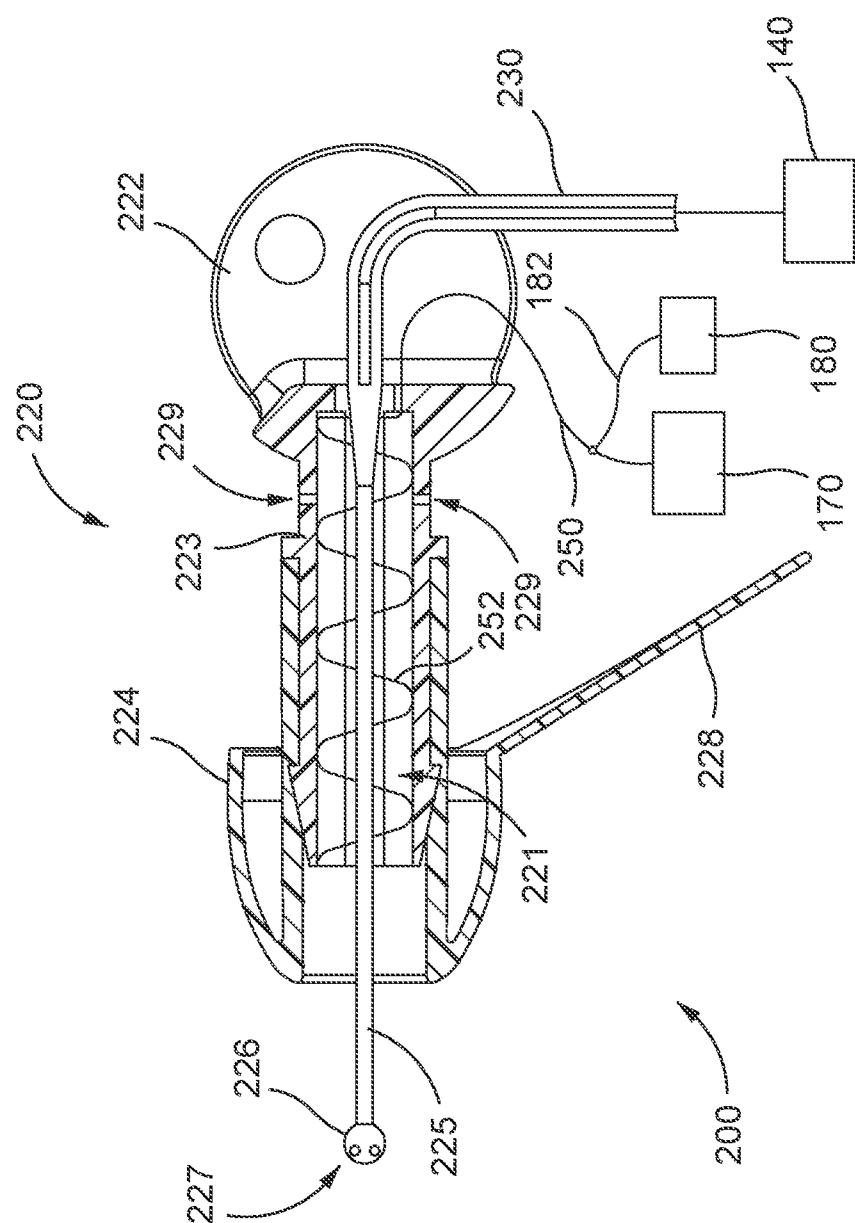


Fig. 5

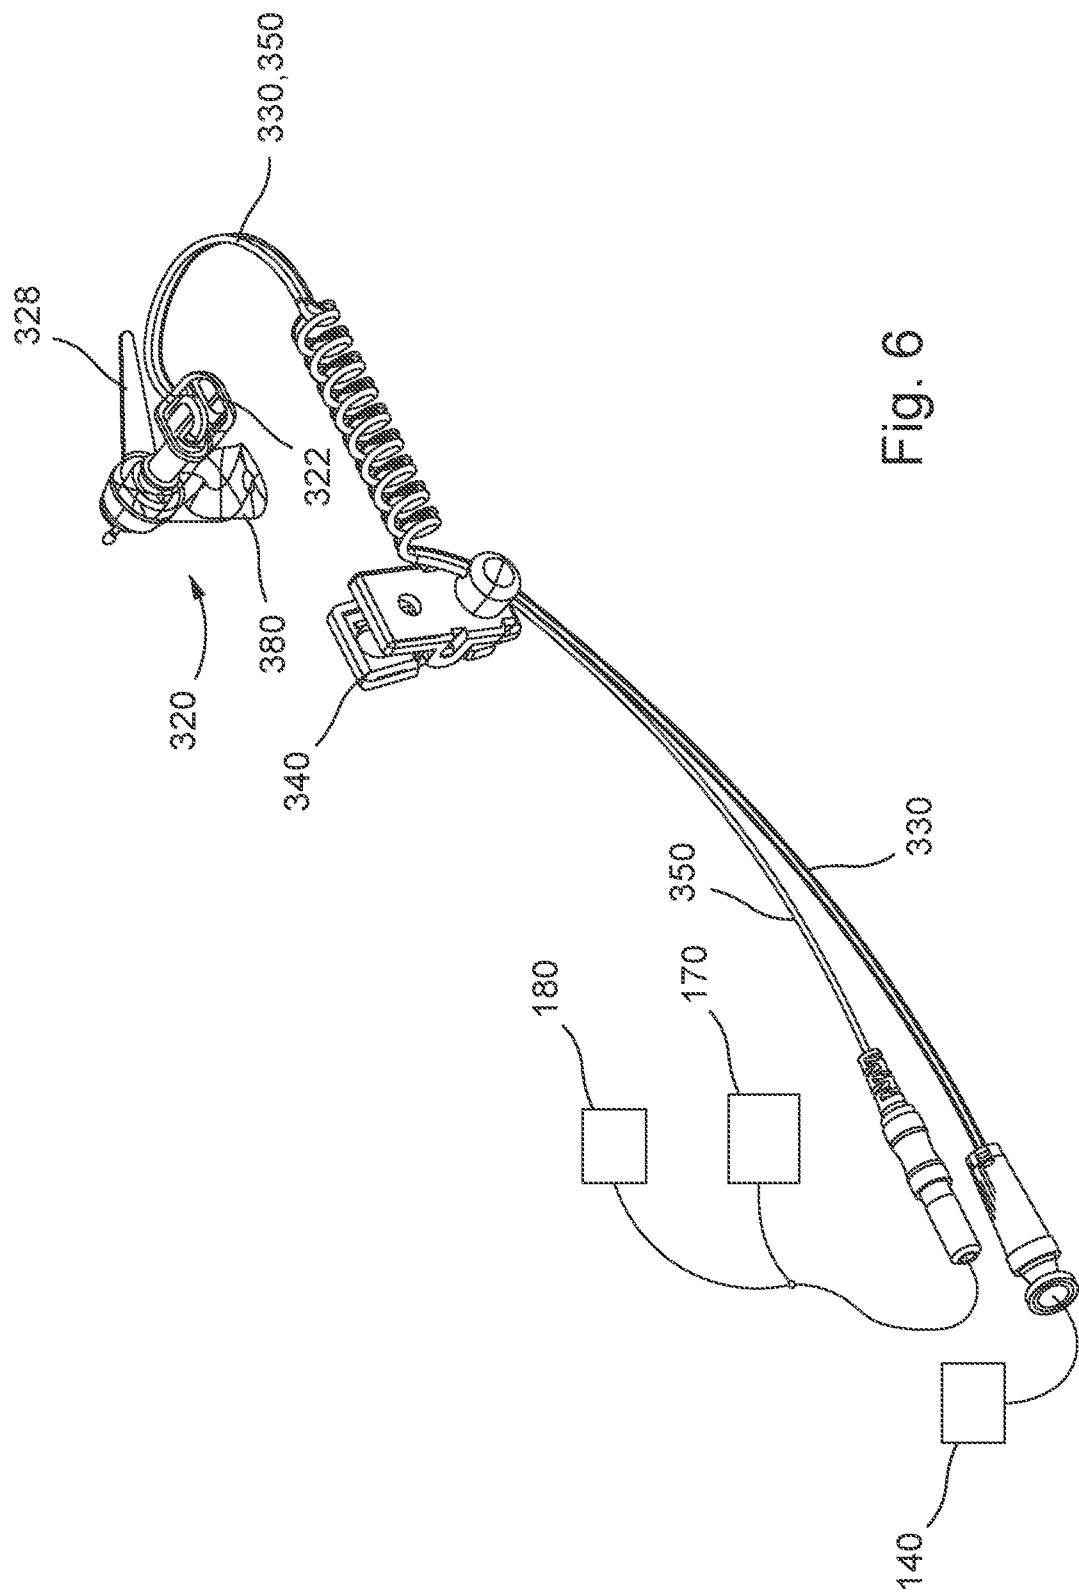
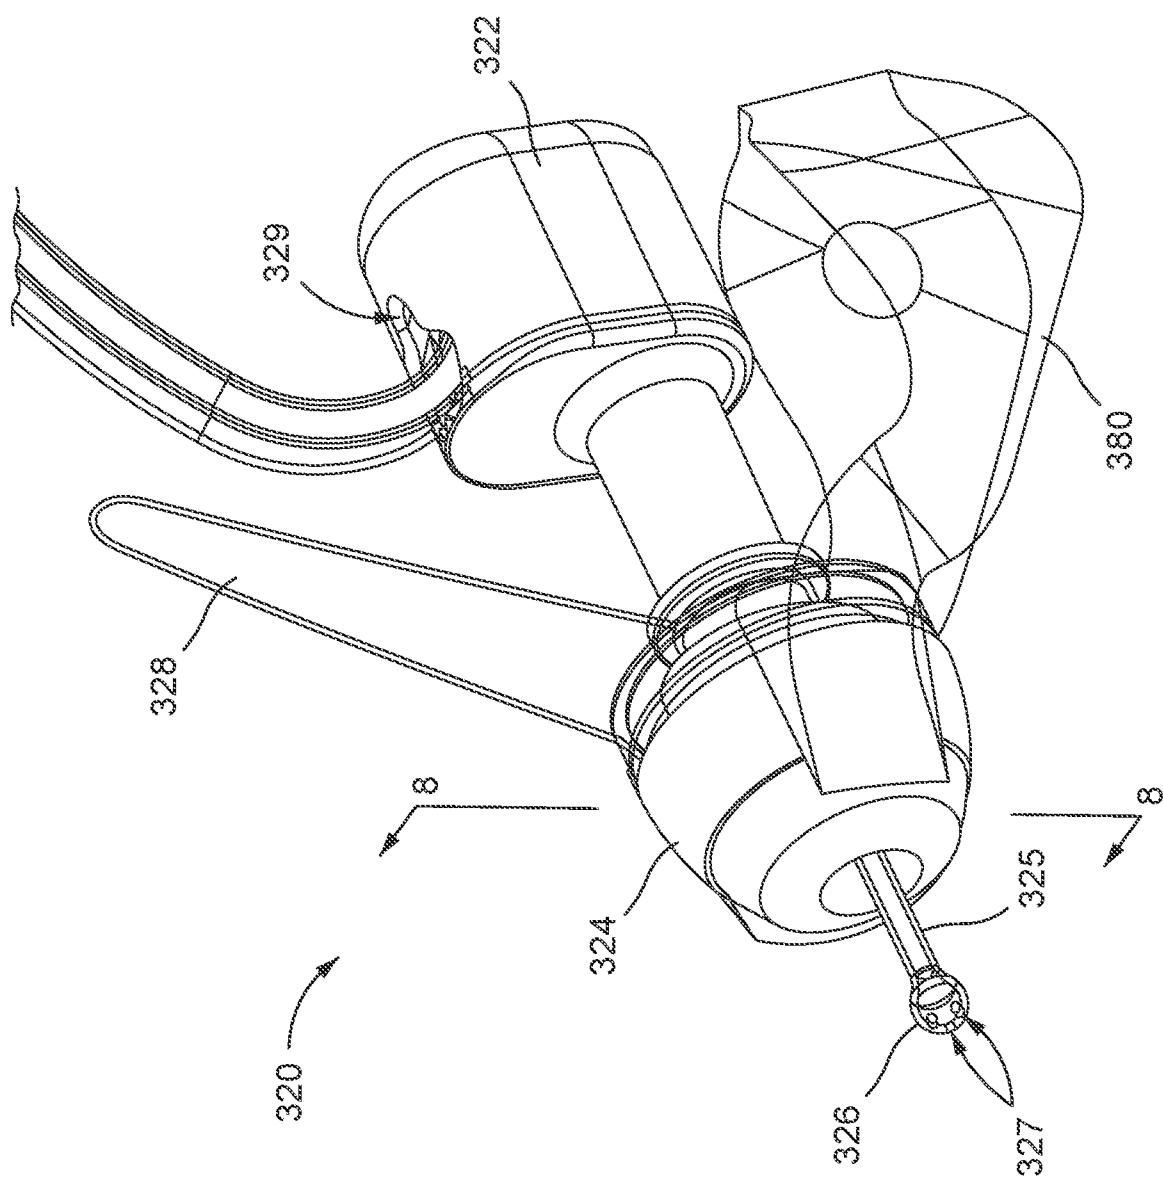


Fig. 7



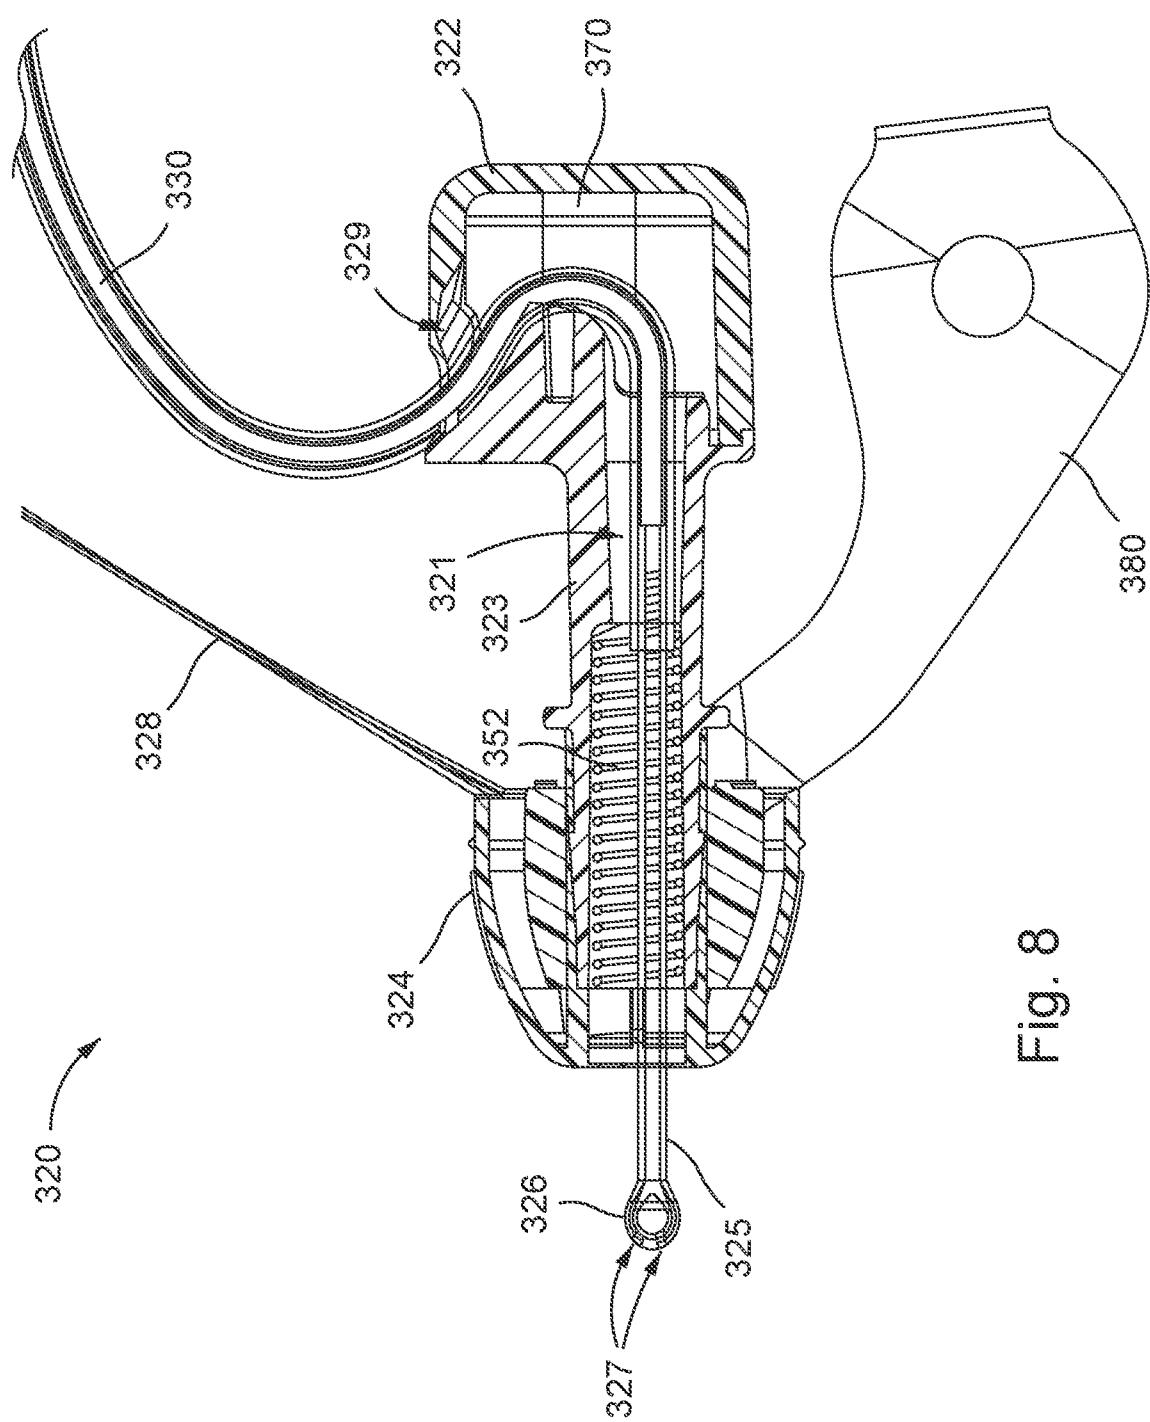


Fig. 8

8/18

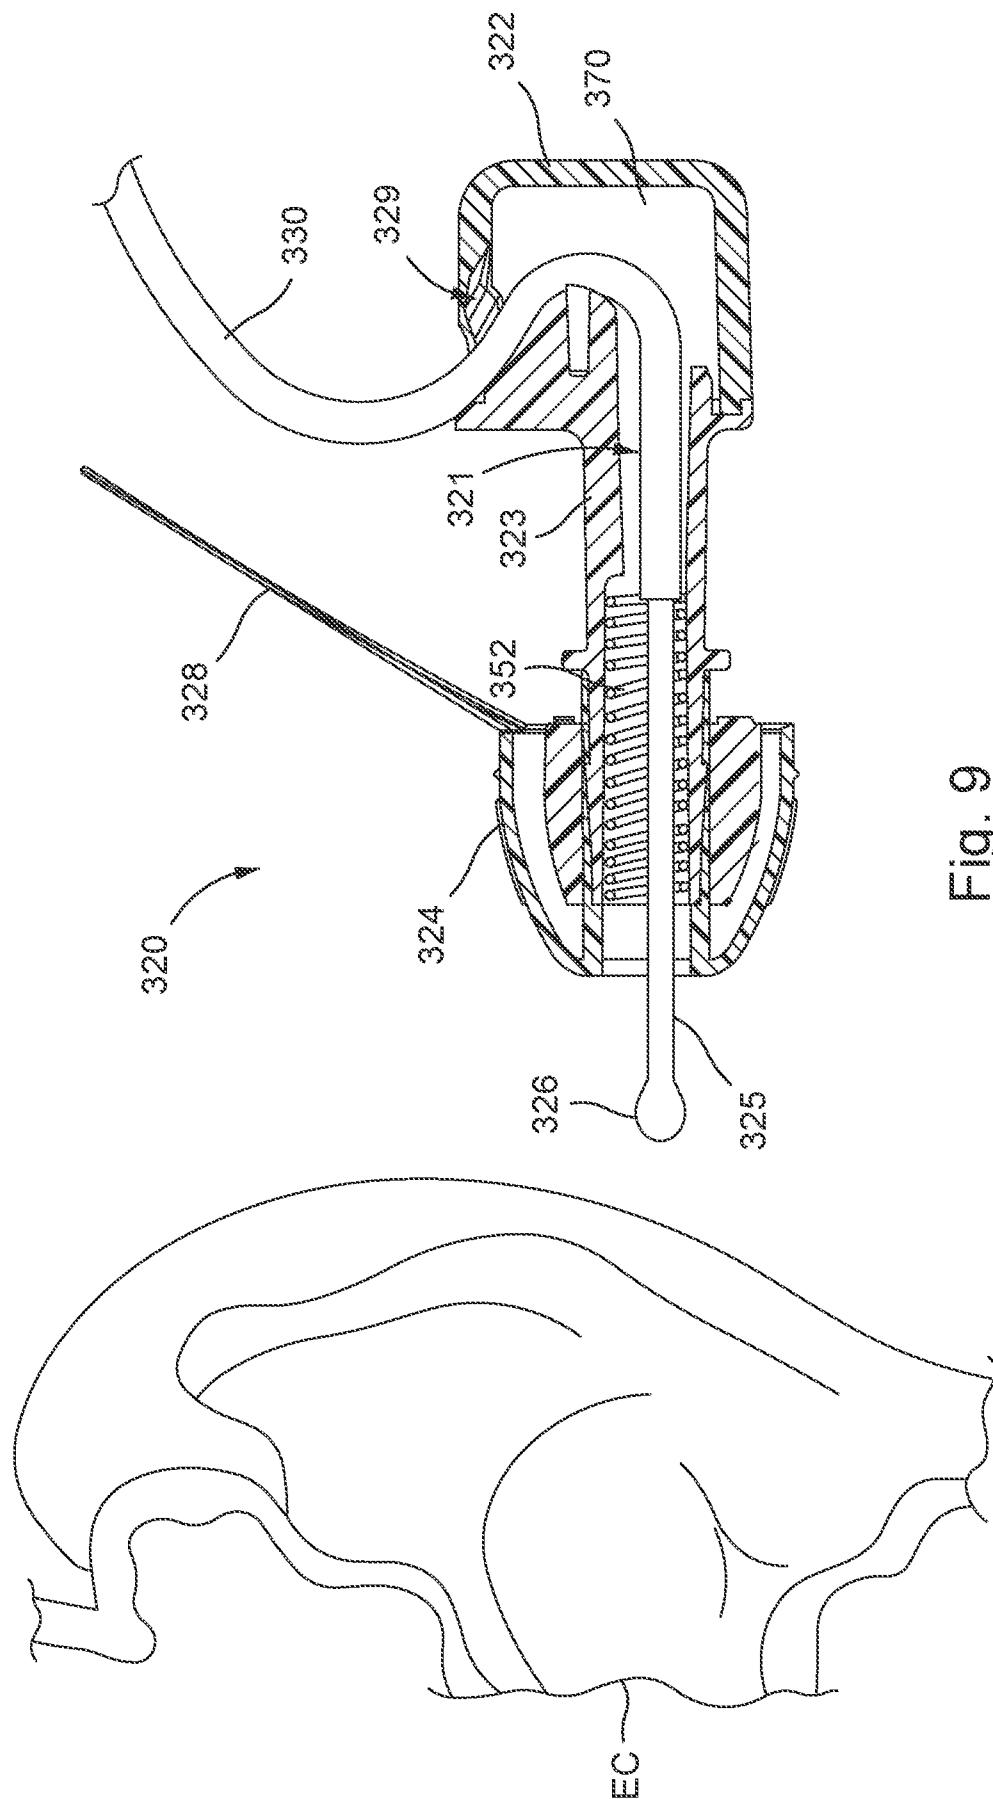


Fig. 9

9/18

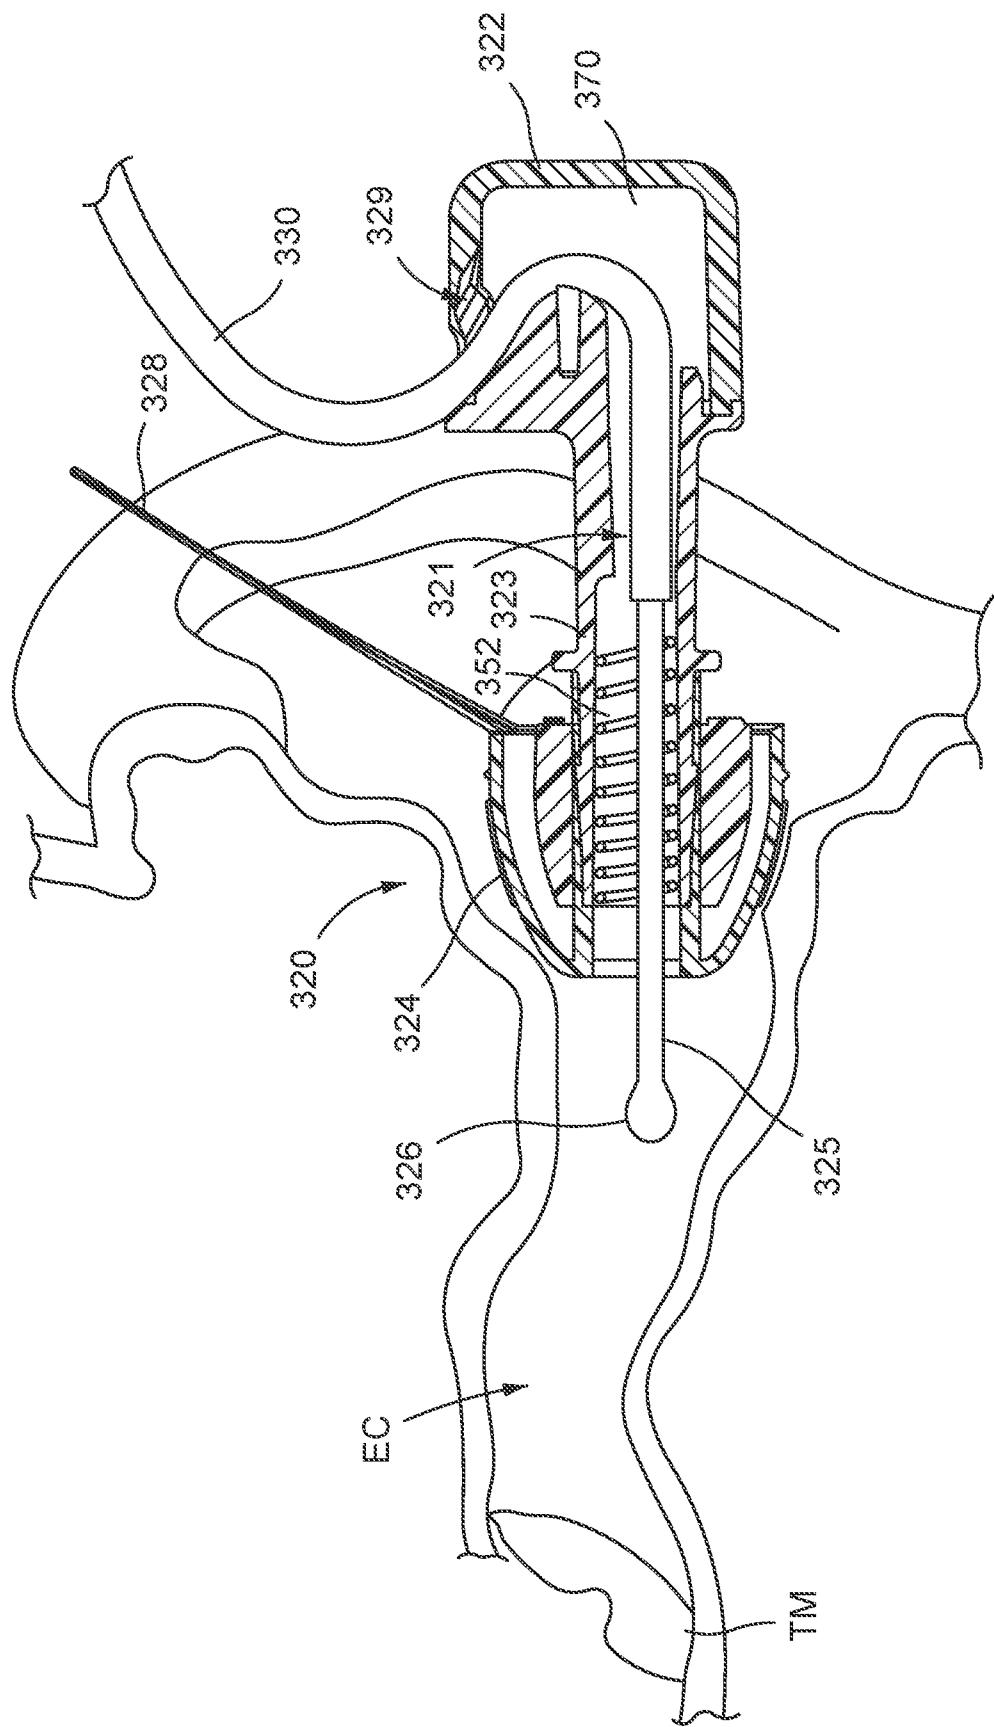


Fig. 10

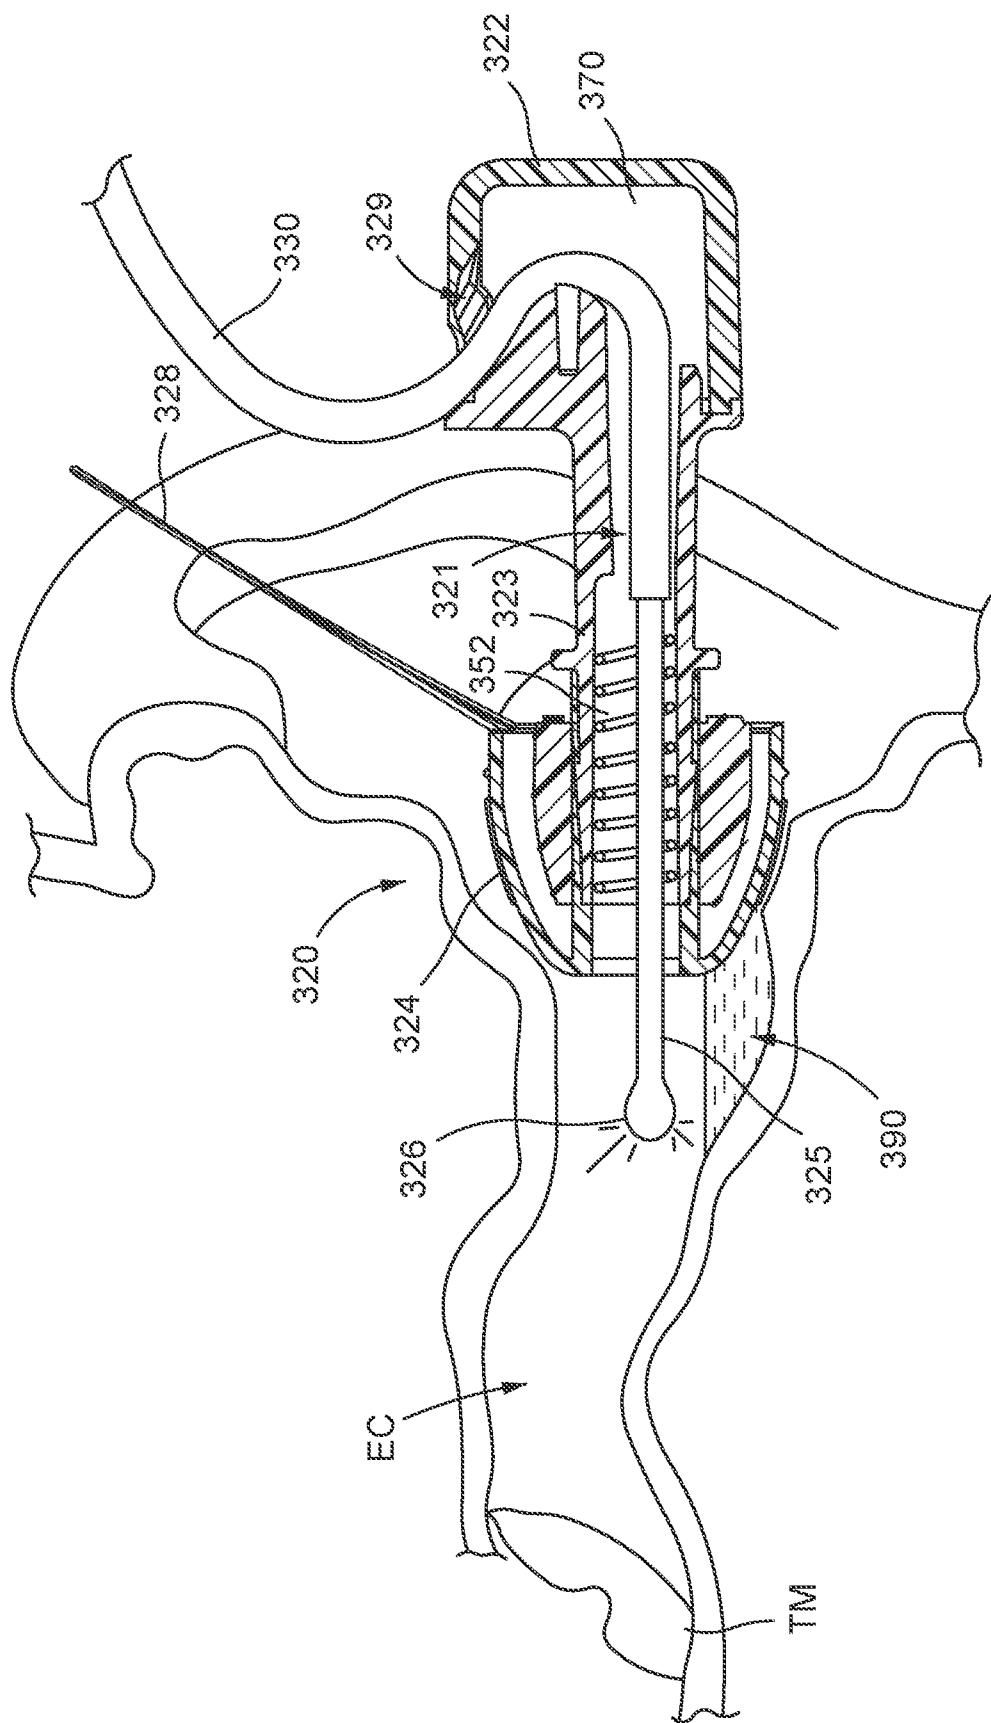


Fig. 11

11/18


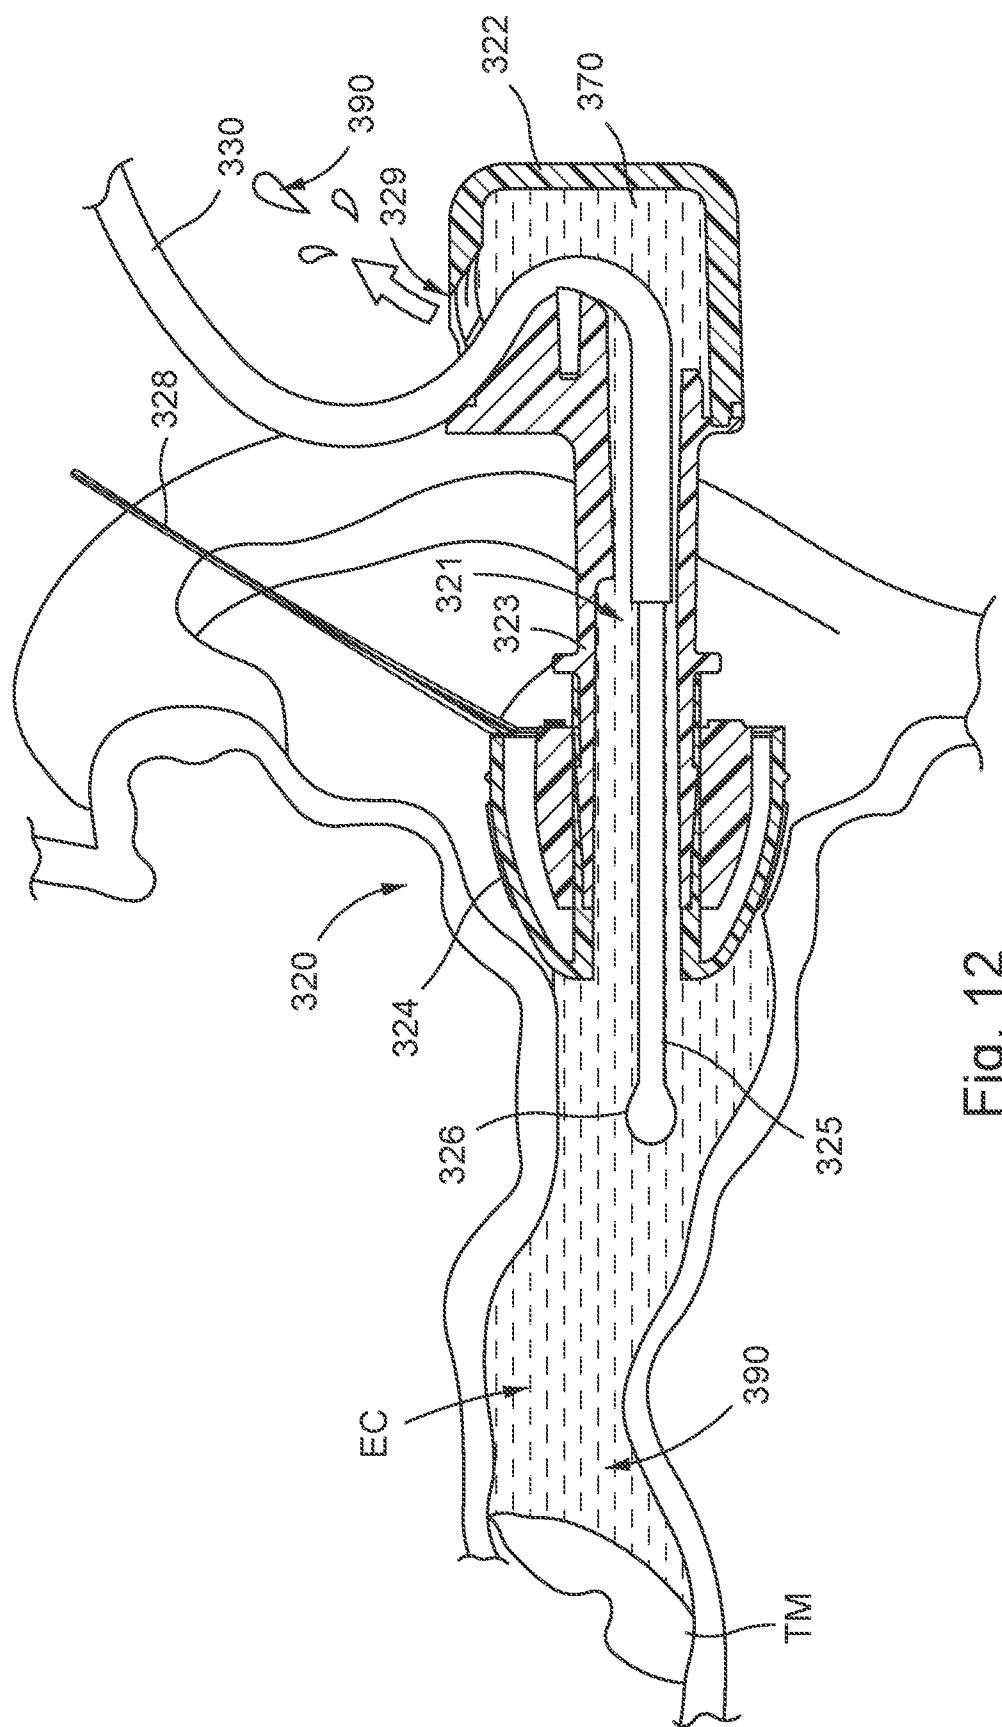


Fig. 12

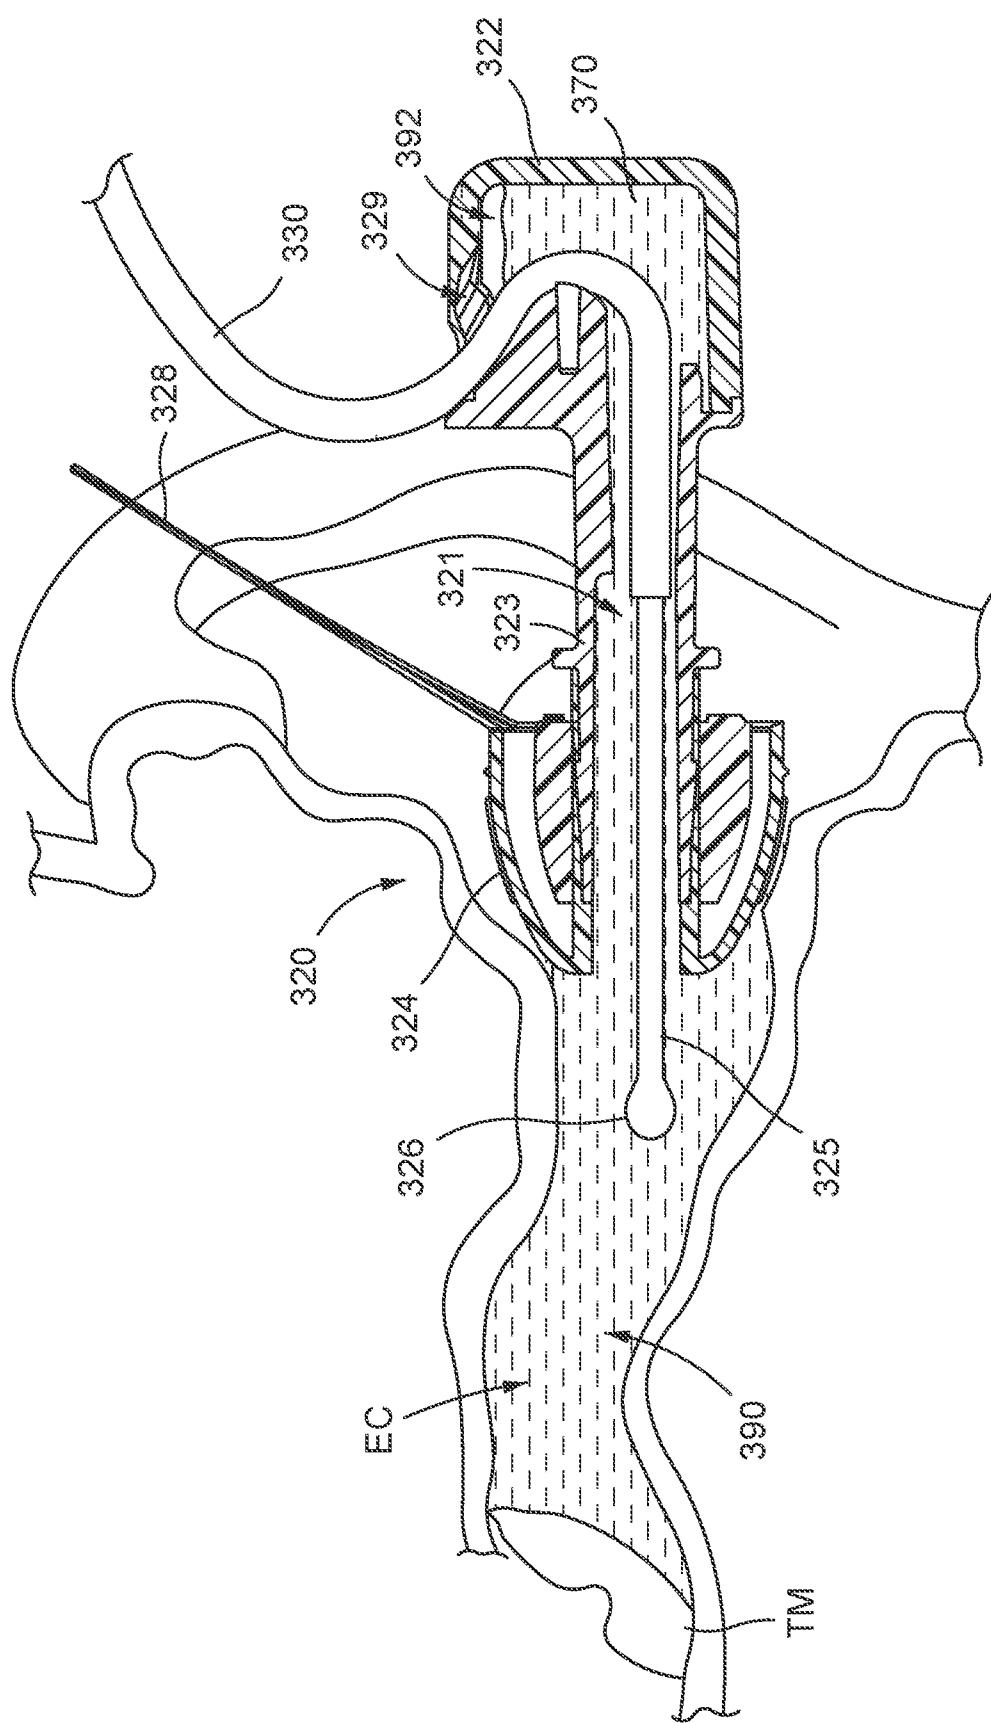

38

13/18

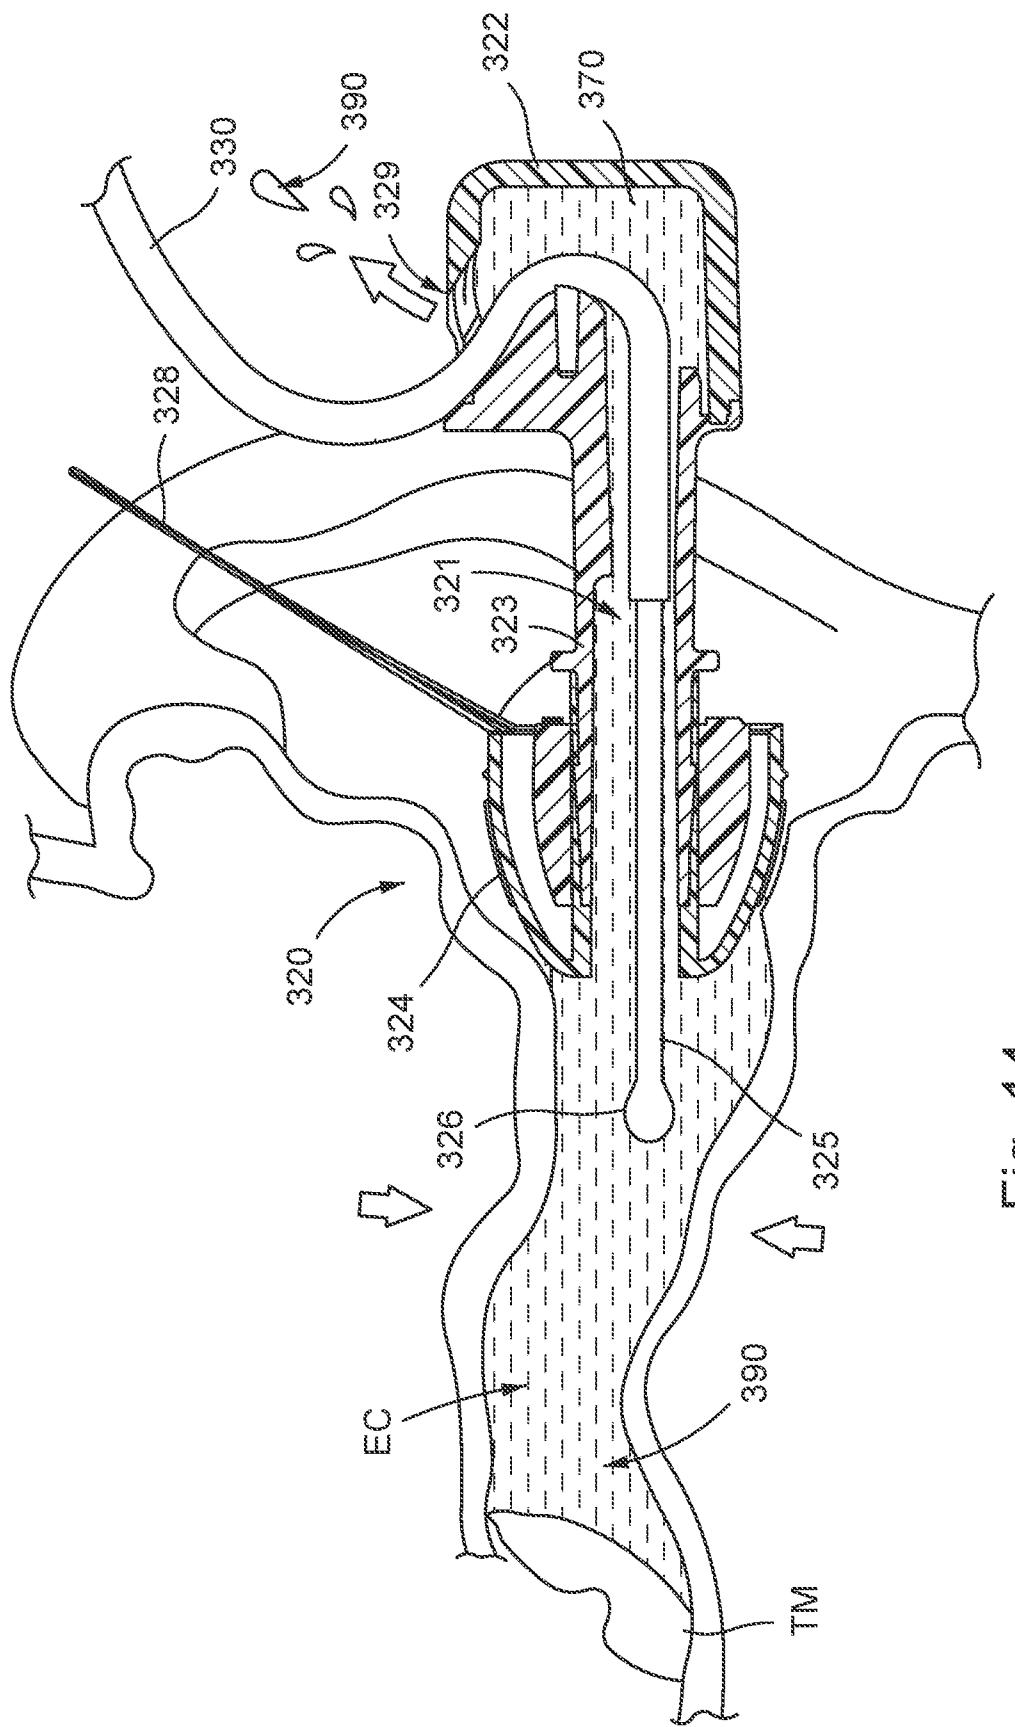


Fig. 14

14/18

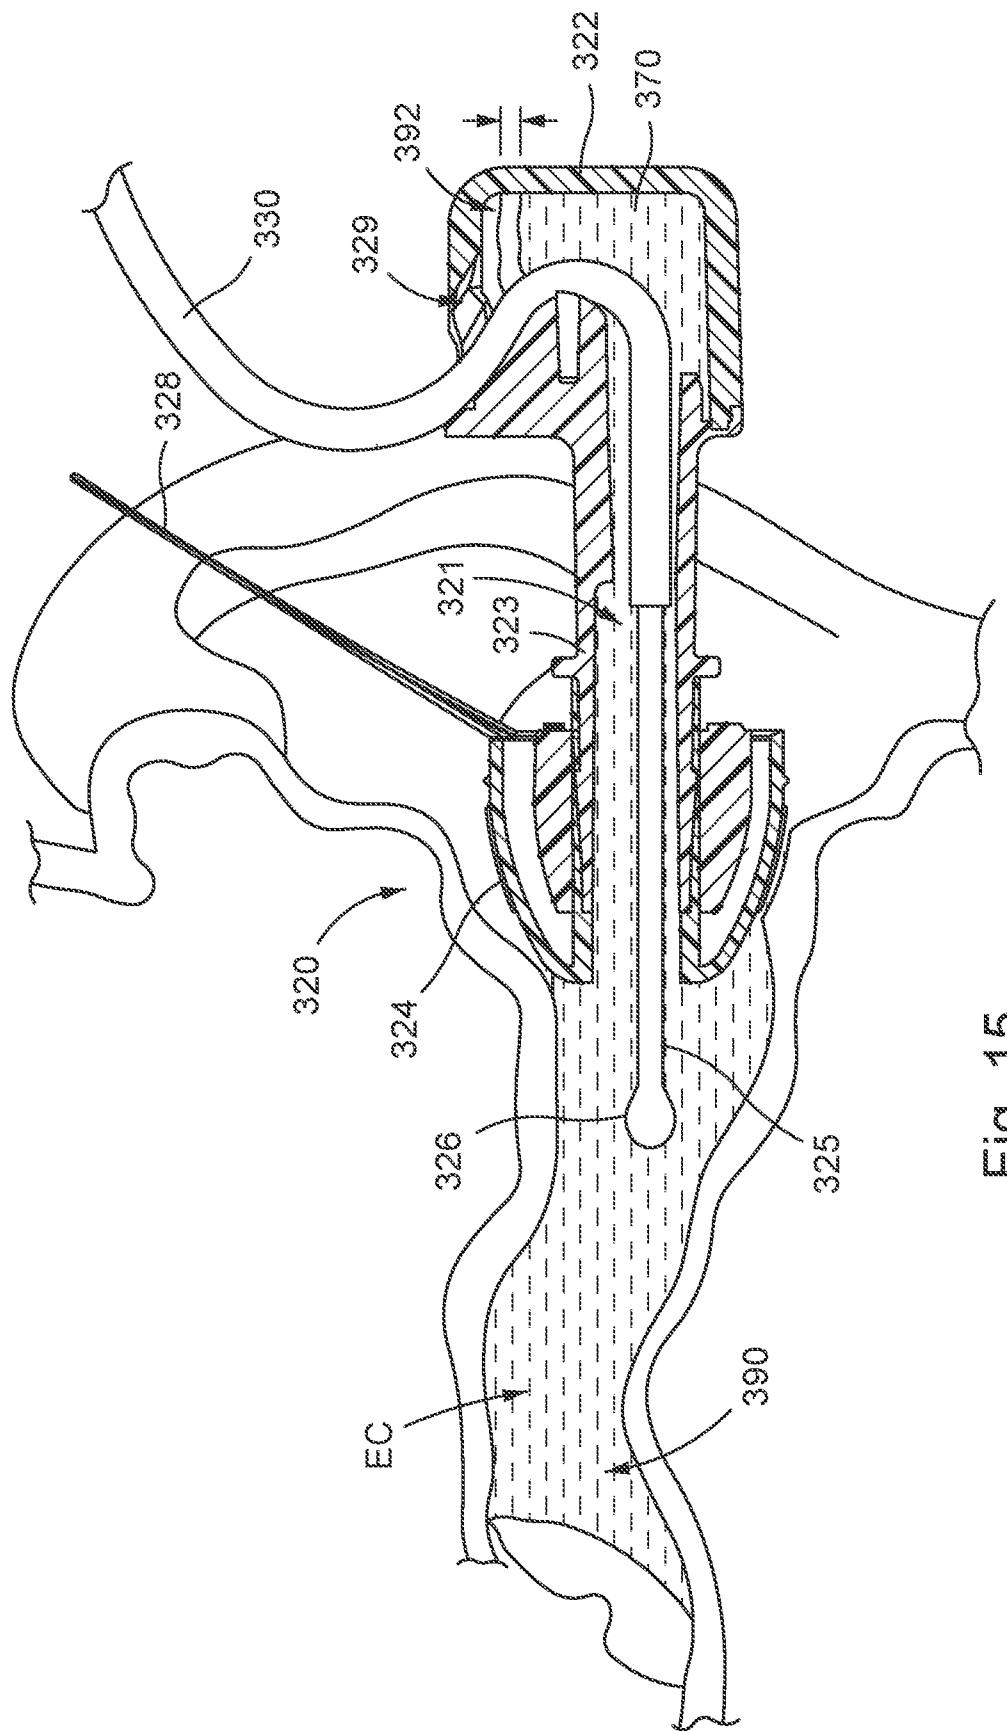


Fig. 15

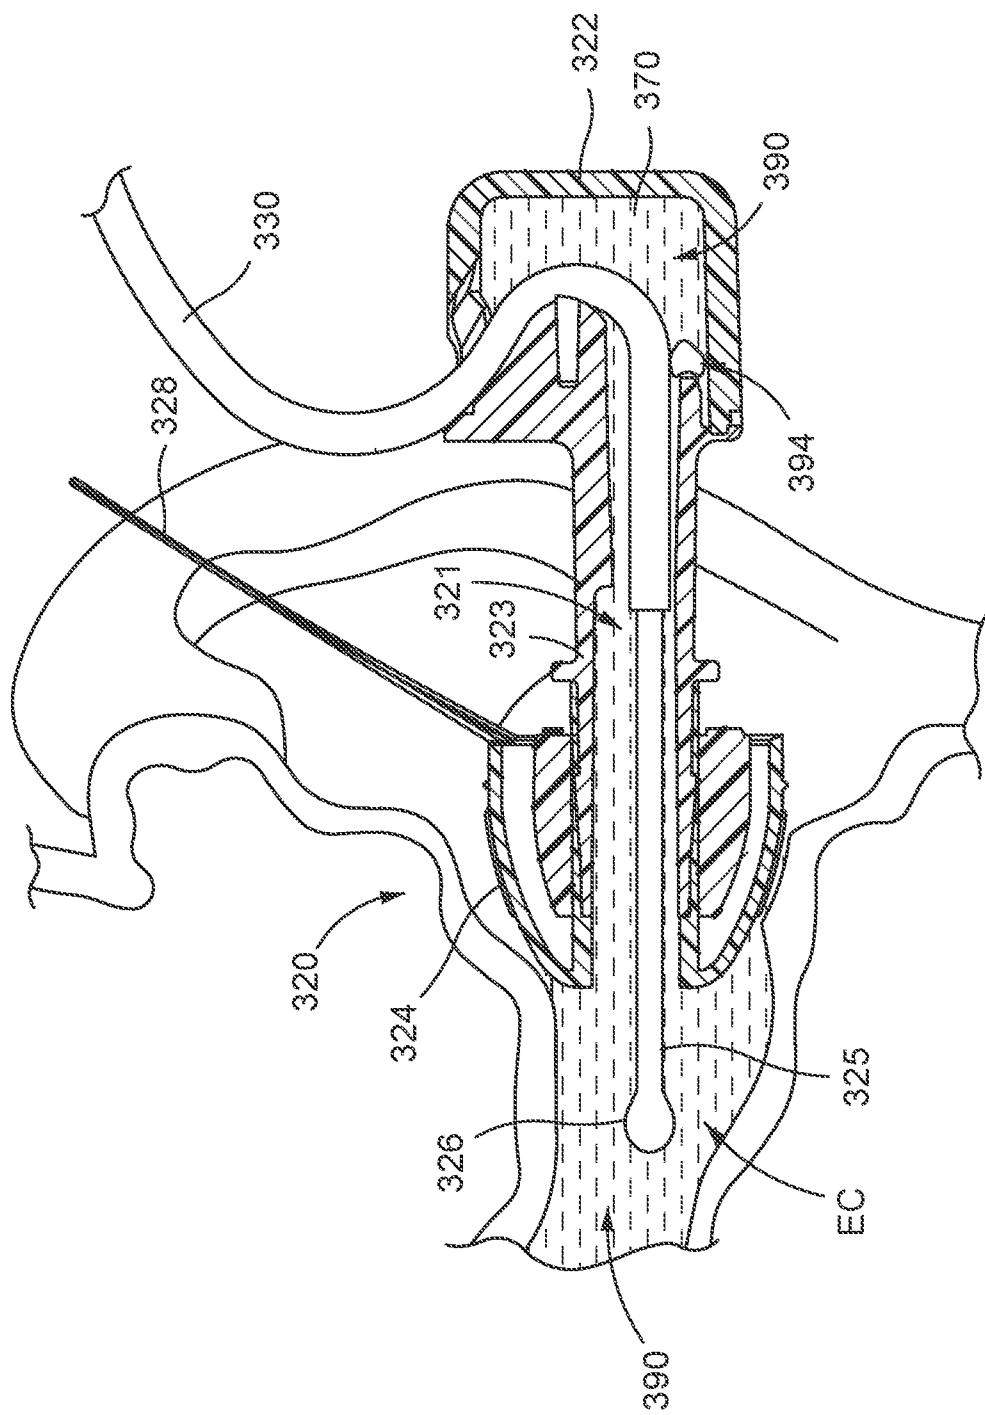


Fig. 16

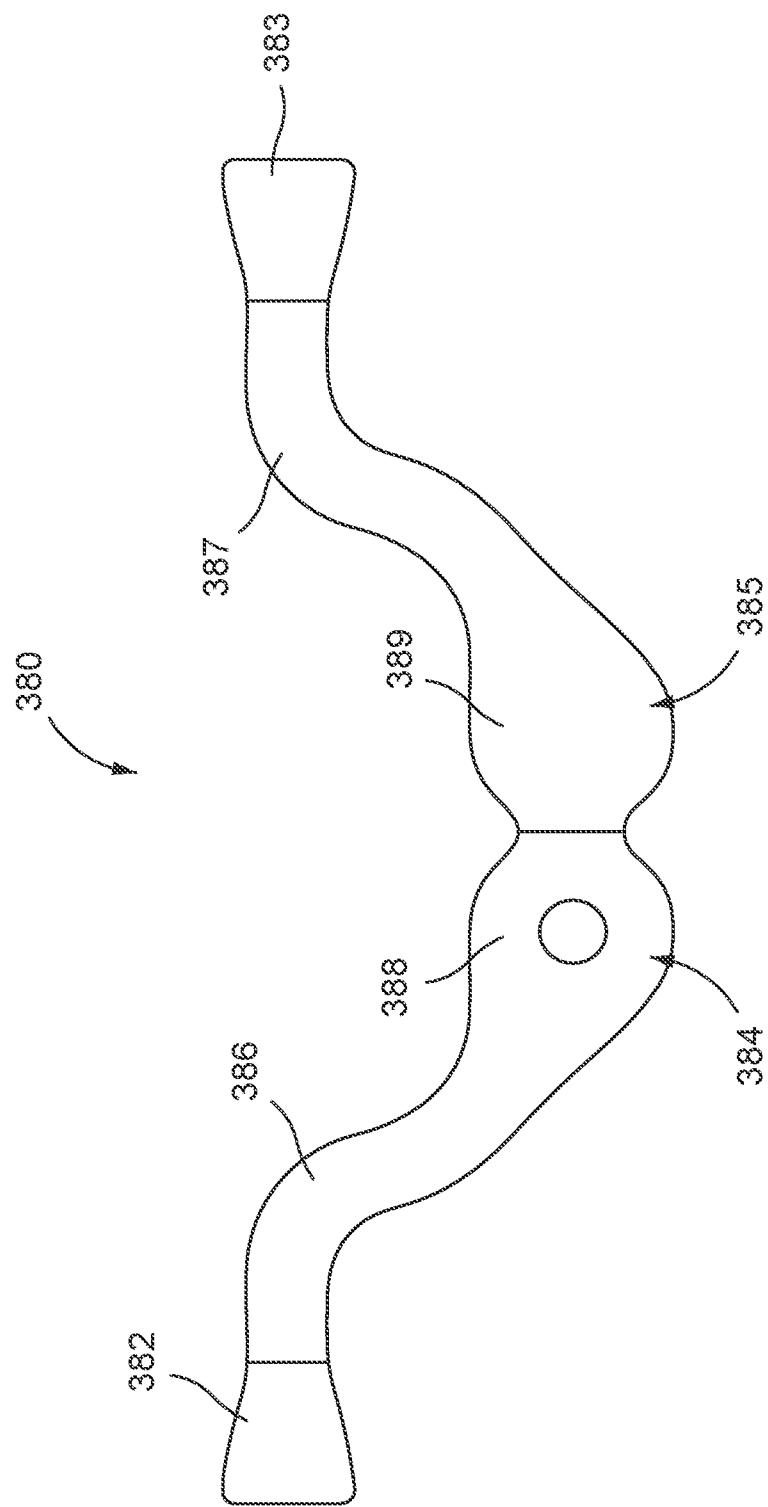


Fig. 17

17/18

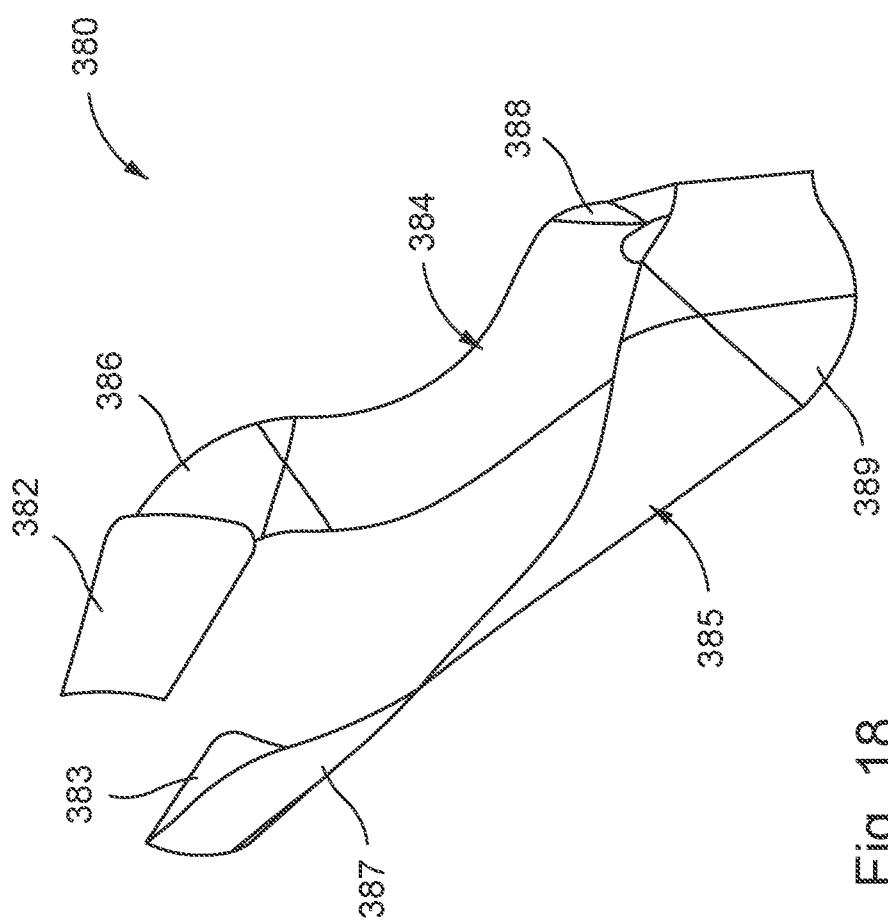


Fig. 18

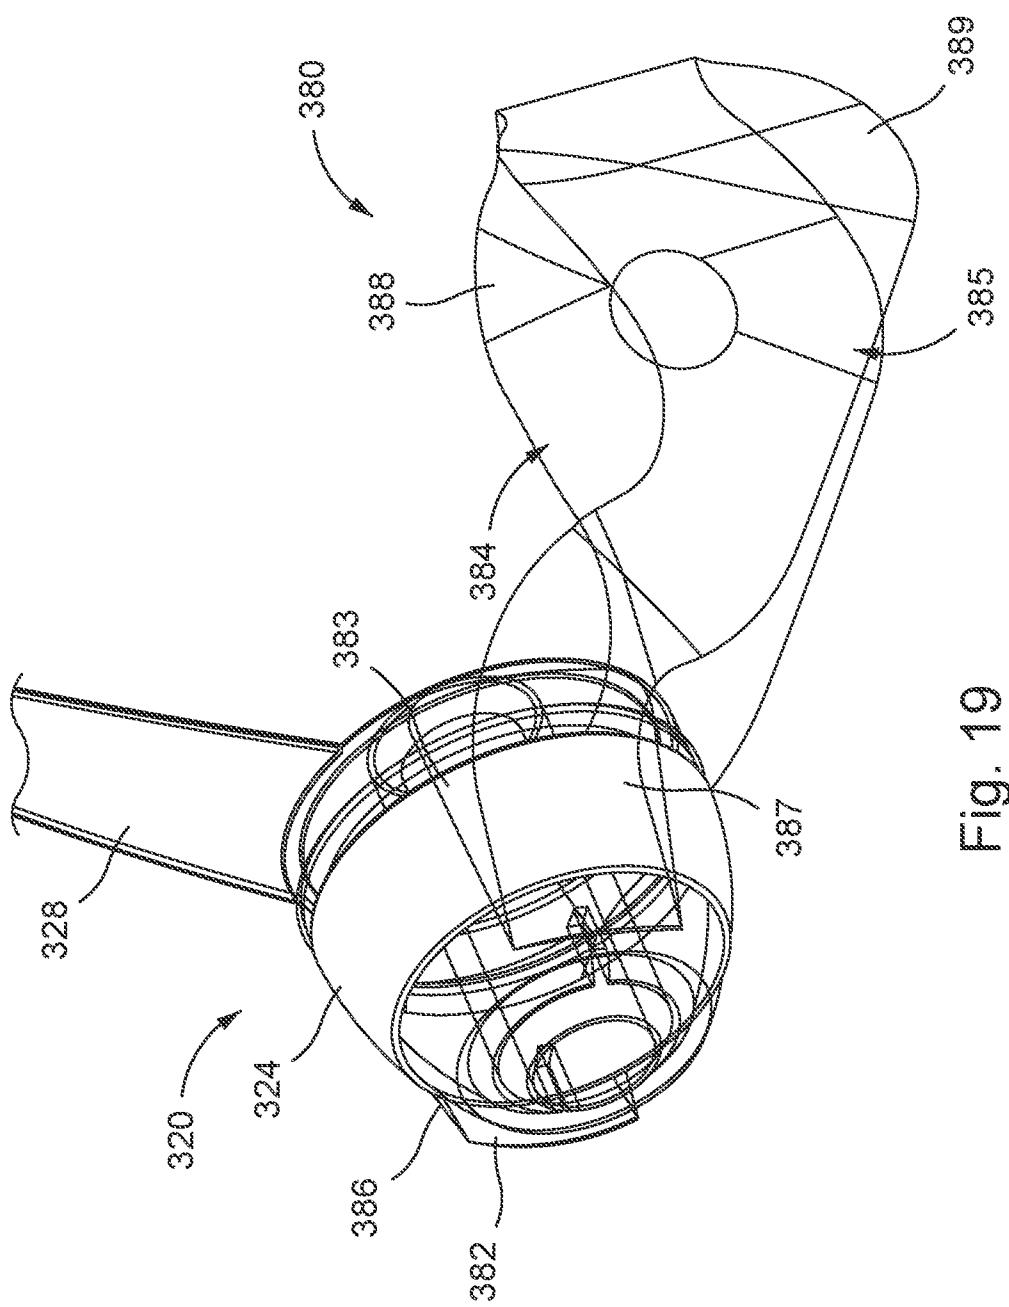


Fig. 19