

**(19) AUSTRALIAN PATENT OFFICE**

(54) Title  
Packaged antimicrobial medical device and method of preparing same

(51)<sup>6</sup> International Patent Classification(s)  
**A61B** 17/06 (2006.01) <sup>8BMEP</sup> **A61L**  
**A61L** 17/00 (2006.01) 17/00  
A61B 17/06 20060101ALI2005100  
20060101AFI2005100 <sup>8BMEP</sup>  
PCT/US2003/030600

(21) Application No: 2003277018 (22) Application Date: 2003 .09 .25

(87) WIPO No: W004/032704

(30) Priority Data

(31) Number	(32) Date	(33) Country
10/367,565	2003 .02 .15	US
10/367,497	2003 .02 .15	US
60/416,114	2002 .10 .04	US

(43) Publication Date : 2004 .05 .04

(43) Publication Journal Date : 2004 .06 .03

(71) Applicant(s)  
Ethicon, Inc.

(72) Inventor(s)  
Fischer, Jerome A., Rothenburger, Stephen, Cerwin, Robert, Scalzo, Howard, McDivitt, James R.

(74) Agent/Attorney  
Callinans, 1193 Toorak Road, Camberwell, VIC, 3124

(56) Related Art  
EP 761243  
US 3629477  
WO 01/28601

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
22 April 2004 (22.04.2004)

PCT

(10) International Publication Number  
WO 2004/032704 A3

- (51) International Patent Classification<sup>7</sup>: A61B 17/00, 17/04, 17/06, A61K 31/665, 31/075
- (21) International Application Number: PCT/US2003/030600
- (22) International Filing Date: 25 September 2003 (25.09.2003)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
60/416,114 4 October 2002 (04.10.2002) US  
10/367,497 15 February 2003 (15.02.2003) US  
10/367,565 15 February 2003 (15.02.2003) US
- (71) Applicant: ETHICON, INC. [US/US]; U. S. Route #22, Somerville, NJ 08876 (US).
- (72) Inventors: SCALZO, Howard; 16 North 11th Street, Kenilworth, NJ 07033 (US). FISCHER, Jerome, A.; 5 Mattben Drive, Warren, NJ 07059 (US). MCDIVITT, James, R.; 12 Monsey Road, Flemington, NJ 08822 (US). ROTHENBURGER, Stephen; 729 Ridge Road, Phillipsburg, NJ 08865 (US). CERWIN, Robert; 404 Cafferty Road, Pipersville, PA 18947 (US).
- (74) Agents: JOHNSON, Philip, S. et al.; JOHNSON & JOHNSON, One Johnson & Johnson Plaza, New Brunswick, NJ 08933 (US).
- (81) Designated States (national): AL, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:  
— with international search report  
— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments
- (88) Date of publication of the international search report: 10 June 2004
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

WO 2004/032704 A3

(54) Title: PACKAGED ANTIMICROBIAL MEDICAL DEVICE AND METHOD OF PREPARING SAME

(57) Abstract: An antimicrobial suture assembly comprising a containment compartment comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said containment compartment; and a suture positioned within the containment compartment, the suture comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the suture; a method for making the antimicrobial suture assembly; and a braided suture having antimicrobial properties comprising an elongate braided structure formed from a plurality of polymeric filaments, said filaments being formed from a polymeric material that is absorbable under physiological conditions, and a coating material disposed on said elongate braided structure, said coating comprising a film forming absorbable polymer, a substantially water-insoluble salt of a fatty acid and an effective amount of an antimicrobial agent selected from the group consisting of halogenated hydroxyl ethers, halogen-o-hydroxy-Biphenyl ethers, acyloxydiphenyl ethers and combinations thereof, said effective amount being sufficient to substantially inhibit microbial growth on or adjacent said suture when said suture is implanted in a patient's body.

**PACKAGED ANTIMICROBIAL MEDICAL DEVICE  
AND METHOD OF PREPARING SAME**

**CROSS-REFERENCE TO RELATED APPLICATIONS**

- 5 This application claims the benefit of U.S. Provisional Application No. 60/416,114, filed on October 04, 2002, U.S. Application No. 10/367,497, filed on February 15, 2003, and U.S. Application No. 10/367,565, filed on February 15, 2003, the contents of which are incorporated herein by reference.

10 **FIELD OF THE INVENTION**

The present invention relates to a packaged antimicrobial medical device and its methods of making.

**BACKGROUND OF THE INVENTION**

- 15 Each year, patients undergo a vast number of surgical procedures in the United States. Current data shows about twenty-seven million procedures are performed per year. Post-operative or surgical site infections ("SSIs") occur in approximately two to three percent of all cases. This amounts to more than 675,000 SSIs each year.
- 20 The occurrence of SSIs is often associated with bacteria that can colonize on implantable medical devices used in surgery. During a surgical procedure, bacteria from the surrounding atmosphere may enter the surgical site and attach to the medical device. Specifically, bacteria can spread by using the implanted medical device as a pathway to surrounding tissue. Such bacterial colonization on the medical device may lead to

infection and trauma to the patient. Accordingly, SSIs may significantly increase the cost of treatment to patients.

- Implantable medical devices that contain antimicrobial agents applied to or incorporated within have been disclosed and/or exemplified in the art. Examples of such devices are disclosed in European Patent Application No. EP 0 761 243. Actual devices exemplified in the application include French Percuflex catheters. The catheters were dip-coated in a coating bath containing 2,4,4'-trichloro-2-hydroxydiphenyl ether (Ciba Geigy Irgasan (DP300)) and other additives. The catheters then were sterilized with ethylene oxide and stored for thirty days. Catheters coated with such solutions exhibited antimicrobial properties, i.e., they produced a zone of inhibition when placed in a growth medium and challenged with microorganism, for thirty days after being coated. It is not apparent from the application at what temperature the sterilized, coated catheters were stored.
- Most implantable medical devices are manufactured, sterilized and contained in packages until opened for use in a surgical procedure. During surgery, the opened package containing the medical device, packaging components contained therein, and the medical device, are exposed to the operating room atmosphere, where bacteria from the air may be introduced. Incorporating antimicrobial properties into the package and/or the packaging components contained therein substantially prevents bacterial colonization on the package and components once the package has been opened. The antimicrobial package and/or packaging components in combination with the incorporation of antimicrobial properties

onto the medical device itself would substantially ensure an antimicrobial environment about the sterilized medical device.

#### **SUMMARY OF THE INVENTION**

The present invention relates to packaged antimicrobial medical devices and methods for  
5 preparing such packaged medical devices. In accordance with embodiments of the present invention, an antimicrobial agent is disposed on the surfaces of the medical device. The medical device is positioned within a package or within a packaging component such as a containment compartment within a package, and upon being subjected to sufficient conditions, a portion of the antimicrobial agent transfers from the medical device to the  
10 package and/or the containment compartment. The transfer of the antimicrobial agent is in an amount sufficient to inhibit bacterial growth on and about the medical device, the package and/or the containment compartment.

An embodiment of the packaged antimicrobial medical device includes at least one  
15 package having an inner surface with an antimicrobial agent disposed thereon, the antimicrobial agent being selected from halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the package; and at least one medical device positioned within the package, the medical device having one or more surfaces having an antimicrobial agent  
20 disposed thereon, the antimicrobial agent being selected from halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the medical device.

Another embodiment of the packaged antimicrobial medical device includes a package having an inner surface and a containment compartment for securing the medical device and that resides within the package. In this embodiment, at least one surface of the containment compartment includes an antimicrobial agent disposed thereon, present in an amount sufficient to substantially inhibit bacterial colonization on the containment compartment. In an alternate embodiment, the inner surface of the package and at least one surface of the containment compartment include an antimicrobial agent disposed thereon, present in an amount sufficient to substantially inhibit bacterial colonization on the package and the containment compartment. The packaged medical device also includes at least one medical device positioned within the containment compartment. The medical device also has one or more surfaces having an antimicrobial agent disposed thereon. The antimicrobial agent is present on the medical device in an amount sufficient to substantially inhibit bacterial colonization on the medical device. The antimicrobial agent disposed on the package, the containment compartment and medical device may be selected from antimicrobial compounds which include halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof.

Another embodiment is an antimicrobial suture assembly comprising a containment compartment comprising one or more surfaces having an antimicrobial agent disposed thereon, the antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the containment compartment; and a suture positioned within the containment compartment, the suture comprising one or more

surfaces having an antimicrobial agent disposed thereon, the antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the suture.

5

The present invention is also directed to a method for preparing a packaged antimicrobial medical device, which includes the steps of providing a package and/or a containment compartment that is substantially free of an antimicrobial agent; positioning a medical device within the package or the containment compartment, the medical device including

10 one or more surfaces having an antimicrobial agent disposed thereon, the antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof; subjecting the package and/or the containment compartment and the medical device to conditions sufficient to transfer a first portion of the antimicrobial agent from the medical device to the package and/or the  
15 containment compartment, while retaining a second portion of the antimicrobial agent on the surface of the medical device, thereby substantially inhibiting bacterial colonization on the medical device, the package and/or the containment compartment.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

20 Fig. 1 is a graph illustrating the transfer of an antimicrobial agent from the medical device to a containment compartment at 55C as a function of time.

Fig. 2 is a photographic representation of a containment compartment on a TSA plate challenged *Staphylococcus aureus*.

Fig. 3 is a photographic representation of a suture on a TSA plate challenged Staphylococcus epidermidis.

Fig. 4 is a scanning electron microscope ("SEM") image of suture strands coated with an antimicrobial composition and exposed to methicillin-resistant Staphylococcus epidermidis.

Fig. 5 is a scanning electron microscope ("SEM") image of suture strands, which are not coated with an antimicrobial composition, exposed to methicillin-resistant Staphylococcus epidermidis.

## 10 DETAILED DESCRIPTION OF EMBODIMENTS OF THE INVENTION

### Packaged Antimicrobial Medical Device

One embodiment of the packaged antimicrobial medical device includes at least one package having an inner surface. The inner surface includes an antimicrobial agent disposed thereon, present in an amount sufficient to substantially inhibit bacterial colonization on the package. The packaged medical device also includes at least one medical device positioned within the package. The medical device also has one or more surfaces having an antimicrobial agent disposed thereon. The antimicrobial agent is present on the medical device, in an amount sufficient to substantially inhibit bacterial colonization on the medical device. The antimicrobial agent disposed on the package and medical device may be selected from antimicrobial compounds which include halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof.



In another embodiment, the packaged medical device includes a package having an inner surface and a containment compartment for securing the medical device and that resides within the package. In this embodiment, at least one surface of the containment compartment includes an antimicrobial agent disposed thereon, present in an amount

5 sufficient to substantially inhibit bacterial colonization on the containment compartment.

In an alternate embodiment, the inner surface of the package and at least one surface of the containment compartment include an antimicrobial agent disposed thereon, present in an amount sufficient to substantially inhibit bacterial colonization on the package and the containment compartment. The packaged medical device also includes at least one

10 medical device positioned within the containment compartment. The medical device also has one or more surfaces having an antimicrobial agent disposed thereon. The antimicrobial agent is present on the medical device, in an amount sufficient to substantially inhibit bacterial colonization on the medical device. The antimicrobial agent disposed on the package, the containment compartment and medical device may be

15 selected from antimicrobial compounds which include halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof.

Another embodiment is an antimicrobial suture assembly comprising a containment compartment comprising one or more surfaces having an antimicrobial agent disposed

20 thereon, the antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the containment compartment; and a suture positioned within the containment compartment, the suture comprising one or more

surfaces having an antimicrobial agent disposed thereon, the antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the suture.

5

The medical devices described herein are generally implantable medical devices, including but not limited to mono and multifilament sutures, surgical meshes such as hernia repair mesh, hernia plugs, brachy seed spacers, suture clips, suture anchors, adhesion prevention meshes and films, and suture knot clips. Also included are implantable medical devices that are absorbable and non-absorbable. An absorbable polymer is defined as a polymer that, when exposed to physiological conditions, will degrade and be absorbed by the body over a period of time. Absorbable medical devices typically are formed from generally known, conventional absorbable polymers including, but not limited to, glycolide, lactide, co-polymers of glycolide, or mixtures of polymers, such as polydioxanone,

10


15

polycaprolactone and equivalents thereof. Preferably, the polymers include polymeric materials selected from the group consisting of greater than about 70% polymerized glycolide, greater than about 70% polymerized lactide, polymerized 1,4-dioxan-2-one, greater than about 70% polypeptide, copolymers of glycolide and lactide, greater than about 70% cellulose and cellulosic derivatives. Examples of absorbable medical device include mono and multifilament sutures. The multifilament suture includes sutures wherein a plurality of filaments are formed into a braided structure. Examples of non-absorbable medical devices include mono and multifilament sutures, surgical meshes such

20

as hernia repair mesh, hernia plugs and brachy seed spacers, which may be polymeric or nonpolymeric.

Suitable antimicrobial agents may be selected from, but are not limited to, halogenated hydroxyl ethers, acyloxydiphenyl ethers, or combinations thereof. In particular, the antimicrobial agent may be a halogenated 2-hydroxy diphenyl ether and/or a halogenated 2-acyloxy diphenyl ether, as described in U.S. Patent No. 3,629,477, and represented by the following formula:

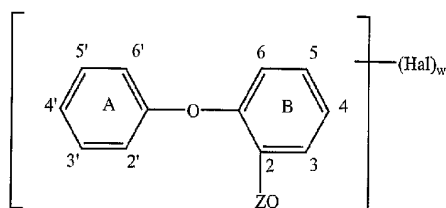

10

In the above formula, each Hal represents identical or different halogen atoms, Z represents hydrogen or an acyl group, and w represents a positive whole number ranging from 1 to 5, and each of the benzene rings, but preferably ring A can also contain one or several lower alkyl groups which may be halogenated, a lower alkoxy group, the allyl group, the cyano group, the amino group, or lower alkanoyl group. Preferably, methyl or methoxy groups are among the useful lower alkyl and lower alkoxy groups, respectively, as substituents in the benzene rings. A halogenated lower alkyl group, trifluoromethyl group is preferred.

15

Antimicrobial activity similar to that of the halogen-o-hydroxy-diphenyl ethers of the above formula is also attained using the O-acyl derivatives thereof which partially or completely hydrolyze under the conditions for use in practice. The esters of acetic acid, chloroacetic acid, methyl or dimethyl carbamic acid, benzoic acid, chlorobenzoic acid, 5 methylsulfonic acid and chloromethylsulfonic acid are particularly suitable.

One particularly preferred antimicrobial agent within the scope of the above formula is 2,4,4'-trichloro-2'-hydroxydiphenyl ether, commonly referred to as triclosan (manufactured by Ciba Geigy under the trade name Irgasan DP300 or Irgacare MP).

10 Triclosan is a broad-spectrum antimicrobial agent that has been used in a variety of products, and is effective against a number of organisms commonly associated with SSIs. Such microorganisms include, but are not limited to, genus *Staphylococcus*, *Staphylococcus epidermidis*, *Staphylococcus aureus*, methicillin-resistant *Staphylococcus epidermidis*, methicillin-resistant *Staphylococcus aureus*, and combinations thereof.

15

It is advantageous to use a coating composition as a vehicle for delivering the antimicrobial agent to the surface of the device where such coating already is used conventionally in the manufacture of the device, such as, for example, absorbable and non-absorbable multifilament sutures. Examples of medical devices, as well as coatings that 20 may be applied thereto, may be found in U.S. Patent Nos. 4,201,216, 4,027,676, 4,105,034, 4,126,221, 4,185,637, 3,839,297, 6,260,699, 5,230,424, 5,555,976, 5,868,244, and 5,972,008, each of which is hereby incorporated herein in its entirety. As disclosed in U.S. Patent No. 4,201,216, the coating composition may include a film-forming polymer and a

substantially water-insoluble salt of a C<sub>6</sub> or higher fatty acid. As another example, an absorbable coating composition that may be used for an absorbable medical device may include poly(alkylene oxylates) wherein the alkylene moieties are derived from C<sub>6</sub> or mixtures of C<sub>4</sub> to C<sub>12</sub> diols, which is applied to a medical device from a solvent solution, as  
5 disclosed in U.S. Patent No. 4,105,034. The coating compositions of the present invention may include a polymer or co-polymer, which may include lactide and glycolide, as a binding agent. The compositions may also include calcium stearate, as a lubricant, and an antimicrobial agent. Medical devices not conventionally employing a coating in the manufacturing process, however, also may be coated with a composition comprising an  
10 antimicrobial agent. The coating may be applied to the device by, for example, dip coating, spray coating, suspended drop coating, or any other conventional coating means.

Absorbable medical devices are moisture sensitive, that is, they are devices that will degrade if exposed to moisture in the atmosphere or in the body. It is known by those of  
15 ordinary skill in the art that medical devices made from absorbable polymers may deteriorate and lose their strength if they come into contact with water vapor prior to use during surgery. For instance, the desirable property of in vivo tensile strength retention for sutures will be rapidly lost if the sutures are exposed to moisture for any significant period of time prior to use. Therefore, it is desirable to use a hermetically sealed package for  
20 absorbable medical devices. A hermetically sealed package is defined herein to mean a package made of a material that serves as both a sterile barrier and a gas barrier, i.e., prevents or substantially inhibits moisture and gas permeation.

Materials useful for constructing the package for absorbable medical devices, for example, include single and multilayered conventional metal foil products, often referred to as heat-sealable foils. These types of foil products are disclosed in U.S. Patent No. 3,815,315, which is hereby incorporated by reference in its entirety. Another type of foil product that  
5 may be utilized is a foil laminate referred to in the field of art as a peelable foil. Examples of such peelable foil and substrates are disclosed in U.S. Patent No. 5,623,810, which is hereby incorporated by reference in its entirety. If desired, conventional non-metallic polymer films in addition to or in lieu of metal foil may be used to form the package for absorbable medical devices. Such films are polymeric and may include conventional  
10 polyolefins, polyesters, acrylics and the like, combinations thereof and laminates. These polymeric films substantially inhibit moisture and oxygen permeation and may be coated with conventional coatings, such as, for example, mineral coatings that decrease or reduce gas intrusion. The package may comprise a combination of polymer and metal foils, particularly a multi-layer polymer/metal-foil composite.

15 Nonabsorbable medical devices may be packaged in any of the materials described above. In addition, it is desirable to package nonabsorbable medical devices in a package made of a material that serves as a sterile barrier, such as a porous material, i.e., medical grade paper, or a polymeric film that is permeable to moisture and gas, i.e., TYVEK film,  
20 manufactured by DuPont and made from high-density polyethylene fibers.

Packages for surgical needles, sutures and combinations including the suture and a surgical needle typically comprise a suture tray as the containment compartment, for securely

holding the suture and/or surgical needle in place. One type of containment compartment typically used for surgical needles and/or sutures is a folder package made from a stiff, medical grade paper. A folder package will typically have a plurality of foldable panels and cut-out tabs and tab pockets. Folder packages for surgical needles and sutures are

5 illustrated and disclosed in the following patents, each of which is hereby incorporated by reference in its entirety: U.S. Pat. Nos. 4,126,221, 4,120,395 and 5,555,976. Another conventionally used containment compartment for surgical needles and/or sutures is a molded plastic tray having a central floor surrounded by an outer winding channel for receiving and retaining a suture, e.g., an oval channel. The containment compartment may

10 further include a medical grade paper or plastic cover that may be mounted to the top of the winding channel, or the molded plastic tray may have molded retainer elements, in order to maintain the suture in the channel. The molded plastic tray may be made from a thermoplastic material selected from the group consisting of polyester, polyvinyl chloride, polypropylene, polystyrene, and polyethylene. Containment compartments having

15 winding channels are illustrated in the following, each of which is hereby incorporated by reference in its entirety: U.S. Pat. Nos. 4,967,902, 5,213,210 and 5,230,424.

Microorganisms of the genus *Staphylococcus* are the most prevalent of all of the organisms associated with device-related surgical site infection. *S. aureus* and *S. epidermidis* are

20 commonly present on patients' skin and as such are introduced easily into wounds. One of the most efficacious antimicrobial agents against *Staphylococcus* is 2,4,4'-trichloro-2'-hydroxydiphenyl ether. This compound has a minimum inhibitory concentration (MIC) against *S. aureus* of 0.01 ppm, as measured in a suitable growth medium and as described

- by Bhargava, H. et al in the American Journal of Infection Control, June 1996, pages 209-218. The MIC for a particular antimicrobial agent and a particular microorganism is defined as the minimum concentration of that antimicrobial agent that must be present in an otherwise suitable growth medium for that microorganism, in order to render the growth medium unsuitable for that microorganism, i.e., the minimum concentration to inhibit growth of that microorganism. The phrase "an amount sufficient to substantially inhibit bacterial colonization" as used herein is defined as the minimum inhibitory concentration for *S. aureus* or greater.
- 10 A demonstration of this MIC is seen in the disk diffusion method of susceptibility. A filter paper disk, or other object, impregnated with a particular antimicrobial agent is applied to an agar medium that is inoculated with the test organism. Where the anti-microbial agent diffuses through the medium, and as long as the concentration of the antimicrobial agent is above the minimum inhibitory concentration (MIC), none of the susceptible organism will
- 15 grow on or around the disk for some distance. This distance is called a zone of inhibition. Assuming the antimicrobial agent has a diffusion rate in the medium, the presence of a zone of inhibition around a disk impregnated with an antimicrobial agent indicates that the organism is inhibited by the presence of the antimicrobial agent in the otherwise satisfactory growth medium. The diameter of the zone of inhibition is inversely
- 20 proportional to the MIC.

Alternatively, the concentration of triclosan on the surface of a medical device such as a coated suture may be greater than about 0.01 ppm (wt./wt. coating) or between about 30 ppm to 5,000 ppm (wt./wt. suture). The concentration of triclosan on the surface of



package or containment compartment may be between about 5 ppm to 5,000 ppm (wt./wt. package or compartment). For other particular applications, however, higher amounts of antimicrobial agent may be useful and should be considered well within the scope of the present invention.

5

**Method for Making a Packaged Antimicrobial Medical Device**

In accordance with various methods of the present invention, a package and containment compartment that are initially substantially free of an antimicrobial agent, *i.e.*, no antimicrobial agent is intended to be present on the package or containment compartment  
10 surfaces, may be provided. A medical device, which has an antimicrobial agent disposed thereon, is positioned within the package or containment compartment. Subsequently, the package, the containment compartment if utilized and the medical device are subjected to time, temperature and pressure conditions sufficient to vapor transfer a portion of the antimicrobial agent from the medical device to the package and/or the containment  
15 compartment.

The rate of transfer of an antimicrobial agent such as triclosan from the medical device to the package and/or containment compartment is substantially dependent upon the time, temperature and pressure conditions under which the package with the containment  
20 compartment and the medical device is processed, stored and handled. For example, Figure 1 illustrates that triclosan is capable of transferring from a suture to a containment compartment (in a closed vial at atmospheric pressure) when the temperature is maintained at 55C over a period of time. The conditions to effectively vapor transfer an antimicrobial

agent such as triclosan include a closed environment, atmospheric pressure, a temperature of greater than 40C, for a period of time ranging from 4 to 8 hours. Also included are any combinations of pressure and temperature to render a partial pressure for the antimicrobial agent that is the same as the partial pressure rendered under the conditions described

5 above, in combination with a period of time sufficient to render an effective amount or concentration of the antimicrobial agent on the package and/or containment compartment, i.e., the minimum inhibitory concentration (MIC) or greater. Specifically, it is known to one of ordinary skill that if the pressure is reduced, the temperature may be reduced to effect the same partial pressure. Alternatively, if the pressure is reduced, and the

10 temperature is held constant, the time required to render an effective amount or concentration of the antimicrobial agent on the package and/or containment compartment may be shortened. While a portion of the antimicrobial agent is transferred to the package and/or containment compartment during this process, a second portion is retained on the surface of the medical device. Accordingly, after the transfer, the medical device

15 and the package and/or the containment compartment contain the antimicrobial agent in an amount effective to substantially inhibit bacterial colonization thereon and thereabout.

Medical devices typically are sterilized to render microorganisms located thereon non-viable. In particular, sterile is understood in the field of art to mean a minimum sterility

20 assurance level of  $10^{-6}$ . Examples of sterilization processes are described in U.S. Patent Nos. 3,815,315, 3,068,864, 3,767,362, 5,464,580, 5,128,101 and 5,868,244, each of which is incorporated herein in its entirety. Specifically, absorbable medical devices may be

sensitive to radiation and heat. Accordingly, it may be desirable to sterilize such devices using conventional sterilant gases or agents, such as, for example, ethylene oxide gas.

An ethylene oxide sterilization process is described below, since the time, temperature and pressure conditions sufficient to vapor transfer a portion of the antimicrobial agent from the medical device to the package and/or containment compartment, are present in an ethylene oxide sterilization process. However the time, temperature and pressure conditions sufficient to vapor transfer the antimicrobial agent from the medical device to the package and/or containment compartment may be effected alone or in other types of sterilization processes, and are not limited to an ethylene oxide sterilization process or to sterilization processes in general.

As discussed above, absorbable medical devices are sensitive to moisture and are therefore often packaged in hermetically sealed packages, such as sealed foil packages. However, sealed foil packages are also impervious to sterilant gas. In order to compensate for this and utilize foil packages in ethylene oxide gas sterilization processes, processes have been developed using foil packages having gas permeable or pervious vents (e.g., TYVEK polymer). The gas permeable vents are mounted to an open end of the package and allow the passage of air, water vapor and ethylene oxide into the interior of the package. After the sterilization process is complete, the package is sealed adjacent to the vent, and the vent is cut away or otherwise removed, thereby producing a gas impervious hermetically sealed package. Another type of foil package having a vent is a pouch-type package having a vent mounted adjacent to an end of the package, wherein the vent is

sealed to one side of the package creating a vented section. After the sterilization process is complete the package is sealed adjacent to the vent, and the package is cut away for the vented section.

- 5 The package and containment compartment are substantially free of, and preferably completely free of, antimicrobial agent prior to the transfer of the antimicrobial agent from the medical device to the package and/or the containment compartment. The medical device may first be placed within the containment compartment, if necessary, and then within the package. After the peripheral seal and side seals have been formed in the
- 10 package, the packaged medical device may be placed into a conventional ethylene oxide sterilization unit. If the package is a foil package, the gas permeable vents described above may be used. Prior to the start of the cycle, the sterilization unit may be heated to an internal temperature of about 25°C. The sterilization unit is maintained about 22 to 37°C throughout the humidification and sterilization cycles. Next, a vacuum may be drawn on
- 15 the sterilization unit to achieve a vacuum of approximately 1.8 to 6.0 kPa. In a humidification cycle, steam then may be injected to provide a source of water vapor for the product to be sterilized. The packaged medical devices may be exposed to water vapor in the sterilization unit for a period of time of about 60 to 90 minutes. Times may vary, however, depending upon the medical device being sterilized.

20

Following this humidification portion of the cycle, the sterilization unit may be pressurized by the introduction of dry inert gas, such as nitrogen gas, to a pressure of between about 42 and 48 kPa. Once the desired pressure is reached, pure ethylene oxide may be introduced

into the sterilization unit until the pressure reaches about 95 kPa. The ethylene oxide may be maintained for a period of time effective to sterilize the packaged medical device. For example, the ethylene oxide may be maintained in the sterilization unit for about 360 to about 600 minutes for surgical sutures. The time required to sterilize other medical devices may vary depending upon the type of product and the packaging. The ethylene oxide then may be evacuated from the sterilization unit and the unit may be maintained under vacuum at a pressure of approximately 0.07 kPa for approximately 150 to 300 minutes in order to remove residual moisture and ethylene oxide from the sterilized packaged medical devices. The pressure in the sterilization unit may be returned to atmospheric pressure.

The following stage of the process is a drying cycle. The packaged medical device may be dried by exposure to dry nitrogen and vacuum over a number of cycles sufficient to effectively remove residual moisture and water vapor from the packaged medical device to a preselected level. During these cycles, the packaged medical device may be subjected to a number of pressure increases and decreases, at temperatures greater than room temperature. Specifically, the jacket temperature of the drying chamber may be maintained at a temperature of between approximately 53°C to 57°C throughout the drying cycle. Higher temperatures, however, may be employed, such as about 65°C to 70°C for sutures, and higher depending upon the medical device being sterilized. A typical drying cycle includes the steps of increasing the pressure with nitrogen to approximately 100 kPa, evacuating the chamber to a pressure of approximately 0.07kPa over a period of 180 to 240 minutes, reintroducing nitrogen to a pressure of 100 kPa and circulating the nitrogen for

approximately 90 minutes, evacuating the chamber to a pressure of approximately 0.01 kPa over a period of approximately 240 to 360 minutes and maintaining a pressure of not more than 0.005 kPa for an additional 4 to 96 hours. At the end of the humidification, sterilization and drying cycles, which takes typically about 24 hours, the vessel is returned  
5 to ambient pressure with dry nitrogen gas. Once drying to the preselected moisture level is complete, the packaged medical device may be removed from the drying chamber and stored in a humidity controlled storage area.

Upon completion of the sterilization process, the antimicrobial medical device, the  
10 package and/or the containment compartment have thereon an amount of the antimicrobial agent effective to substantially inhibit colonization of bacteria on or adjacent the antimicrobial device, the package and/or the containment compartment.

#### **Example 1**

15 A series of USP standard size 5-0 coated polyglactin 910 sutures were coated with a 2% triclosan coating composition so that each suture contained about a total of 23.2 µg triclosan before sterilization. The coated sutures each were placed in a package as described herein above including a containment component, *i.e.*, a tray, for holding the suture and a paper component for covering the suture in the tray. The suture in the  
20 containment component and packaging were sterilized as described herein above. After sterilization, it was determined that that suture contained about 5.5 µg triclosan, the tray about 0.2 µg triclosan, the paper component about 2.3 µg triclosan, and the package heat seal coating about 1.5 µg triclosan. Triclosan not recovered after sterilization was about

13.7 µg triclosan. Fig. 1 indicates triclosan transfer from the antimicrobial suture to the tray of the package as a function of time at 55°C.

After sterilization, the paper component and tray of the sterilized package were  
5 tested for antimicrobial properties utilizing a zone of inhibition test as indicated herein  
below. Zone of inhibition testing is a conventional method for estimating the inhibitory  
effects of antimicrobial substances against specific bacterial strains of interest. Zone of  
inhibition assays are useful for testing diffusible agents. As the agent diffuses away from  
the disk, the concentration decreases logarithmically. The sensitivity of the organism to  
10 the agent is judged by the appearance and size of a zone where no growth occurs, *i.e.*, the  
zone of inhibition.

A comparative example of a package that contained a conventional commercially  
available suture, *i.e.*, not having triclosan applied thereto, also was prepared and tested for  
15 antimicrobial properties.

Fig. 2 is a photographic representation of the zone of inhibition with respect to a  
tray of the antimicrobial package on a TSA plate challenged with *Staphylococcus aureus*.

20 The results of the zone of inhibition assays for the paper component and tray are  
listed in Table 1. The zones were measured for both treated and untreated tray and paper  
component. As shown in Table 1, zones of inhibition were present for all treated c

omponents against both *Staphylococcus aureus* and *Staphylococcus epidermidis*. The untreated components exhibited no zones of inhibition.

Table 1. Zone of Inhibition Assay for Package Components

<i>Staphylococcus epidermidis</i>			
Treated Package Component	Zone size	Untreated Package Component	Zone size
Tray	18 mm	Tray	0
Paper	13 mm	Paper	0
<i>Staphylococcus aureus</i>			
Treated Package Component	Zone size	Untreated Package Component	Zone size
Tray	12 mm	Tray	0
Paper	13 mm	Paper	0

5

### Example 2

This example is a 24-hour aqueous immersion assay. The purpose of this assay was to determine the effect of aqueous exposure on the antimicrobial properties of suture material for a range of suture diameters. Sterile sutures in USP sizes 2-0, 3-0, 4-0, and 5-0, with and without a 1% triclosan coating applied thereto, were aseptically cut into 5-cm pieces. One half of the cut pieces were stored in a sterile Petri dish and kept under a dry nitrogen atmosphere for 24 hours (dry suture). One half of the cut pieces were aseptically transferred to sterile 0.85% saline and incubated at 37°C for 24 hours (wet sutures).

15 The dry and wet sutures were then aseptically placed in individual sterile Petri dishes and challenged with 100 microliters of inoculum containing  $10^5$  colony-forming units (CFU) of *Staphylococcus aureus* or *Staphylococcus epidermidis*. Ten replicates of each suture size were used for each organism and for both the dry and wet sample groups. TSA was poured into each dish and allowed to solidify. The plates were incubated at 37°C



for 48 hours. After incubation, the plates were examined under a darkfield colony counter and the zones of inhibition were measured.

The results of the zone of inhibition assays are listed in Table 2. Zones of inhibition were present for all sizes of coated polyglactin 910 suture having triclosan applied thereto. Both the dry and wet samples exhibited significant zones of inhibition. The coated polyglactin 910 suture controls had no zones of inhibition. A typical zone of inhibition is depicted in Fig. 3.

Table 2. 24 Hour Aqueous Immersion Assay: Zone of Inhibition Diameter

	Zone Diameter Average (mm)			
	<i>S aureus</i>		<i>S epidermidis</i>	
	<i>Dry</i>	<i>Wet</i>	<i>Dry</i>	<i>Wet</i>
<i>Suture Material</i>				
Size 2-0				
+ Triclosan	10	9	10	9
Control	0	0	0	0
Size 3-0				
+ Triclosan	10	10	10	8
Control	0	0	0	0
Size 4-0				
+ Triclosan	10	3	10	2
Control	0	0	0	0

Size 5-0				
+ Triclosan	10	3	10	2
Control	0	0	0	0

All suture samples were from different lots. Average zone diameter is based on triplicate plates.

As shown in Fig. 3, areas of inhibited bacterial growth were observed around coated polyglactin 910 suture containing triclosan, while the control suture without triclosan had confluent bacterial growth. The response was similar for *Staphylococcus epidermidis* (shown), *Staphylococcus aureus*, MRSA, and MRSE, and was consistent for a variety of suture sizes.

10

#### Example 4

This example is directed to a 7-day aqueous immersion assay. The purpose of this assay was to determine if the antimicrobial effect of triclosan treatment would endure for 7 days in a buffered aqueous environment.

15 Sterile USP size 2-0 coated polyglactin 910 suture coated with a 1%, 2%, and 3% triclosan coating solution, respectively, and ethylene oxide sterilized USP size 2-0 coated polyglactin suture were aseptically cut into 5-cm pieces. Samples were tested on each of 7 days in triplicate.

On day 1, 3 pieces of each suture material were placed into individual sterile Petri dishes and inoculated with 0.1 mL of challenge organism containing approximately  $10^4$  CFU. TSA was poured into each dish and allowed to solidify. All remaining pieces of  
20 suture material were placed into 100 mL of sterile phosphate buffered 0.85% saline (PBS).

Every 24 hours for the next 6 days, 3 pieces of each suture material were removed from the PBS, inoculated, and pour plated in tryptic/soy/agar (TSA). All plates were incubated at 37°C for 48 hours and the plates examined for the presence or absence of a zone of inhibition.

- 5 The results for the 7-day assay are presented in Table 4. The coated polyglactin 910 suture with triclosan produced zones of inhibition after every challenge. The control coated polyglactin 910 suture without triclosan produced no growth inhibition.

Table 4. 7-Day Aqueous Immersion Assay: Zone of Inhibition Diameter

		Zone Diameter Average (mm)						
	Day	1	2	3	4	5	6	7
Triclosan coating								
1%		20	18	20	20	19	21	20
2%		24	20	22	21	24	24	23
3%		27	25	15	25	27	30	27
Control (0%)		0	0	0	0	0	0	0

10

All suture samples were from different lots. Average diameter is based on triplicate plates.

- This example is a demonstration of the efficacy of the antimicrobial suture where samples of the antimicrobial suture and a conventional suture were each separately exposed by immersion in aqueous buffer as a model of physiological conditions for up to seven days. On each day, samples of both the conventional and the antimicrobial suture of the invention were removed and placed on tryptic/soy/agar (TSA) plates that had been
- 15

inoculated with a  $10^4$  colony forming unit (CFU) Staphylococcus challenge. As is shown in Table 4, the antimicrobial suture of the invention developed a zone of inhibition around it on the plate, even after seven days of immersion, providing evidence that the concentration of the antimicrobial agent on and around the antimicrobial suture of the invention was still above the MIC, while the conventional sutures, treated similarly, developed no zone of inhibition, i.e. the microorganisms freely grew on and around the conventional suture.

#### **Example 6**

This example relates to scanning electron microscopy. Scanning electron microscope (SEM) images were prepared using sutures that had been exposed to MRSE in broth culture. Single 6-inch strands of USP size 2-0 coated polyglactin 910 suture coated with 0.5% triclosan coating solution were placed in separate tubes containing 30 mL of sterile TSB and inoculated with 0.1 mL of a 24-hour culture of the challenge organism in TSB. Single 6-inch strands of USP size 2-0 Polysorb® (braided lactomer 9-1) suture, available from United States Surgical Corporation, and which did not contain triclosan, were also prepared in the same fashion. The tubes were incubated for 24 hours at 37°C. After incubation, the sutures were prepared for SEM as follows.

Each strand of the suture was removed from the broth and rinsed by vortexing in 100 mL of sterile saline for 10 seconds. The rinsed strands were fixed in 10% buffered formalin for 5 minutes. The fixed strands were dehydrated in ethanol using sequential 5-minute exposures of 50%, 70%, 85%, 95%, and 100% ethanol. A final dehydration was performed using a 5-minute exposure in hexamethylenedisilazane. The samples were air

dried prior to SEM. The SEM used for imaging the bacteria was a JEOL (Japan Electronics and Optics Laboratory) JSM-5900LV scanning electron microscope.

Figs. 4 and 5 illustrate the differences between the triclosan-treated suture (a) and the untreated suture (b). The triclosan-treated suture had very few bacteria associated with it anywhere on the surface, while the untreated suture was uniformly and heavily coated with bacteria.

The data presented above indicate that coated polyglactin 910 suture with triclosan exhibits antimicrobial activity in vitro against *Staphylococcus aureus* and *Staphylococcus epidermidis* compared to untreated controls. This activity is evident on a range of suture diameters. The antimicrobial activity endures despite extended exposure to a buffered aqueous environment. Methicillin-resistant strains of *Staphylococcus aureus* and *Staphylococcus epidermidis* were inhibited after 24 hours of aqueous extraction by polyglactin 910 with triclosan at low triclosan concentrations. Low levels of triclosan on the suture are sufficient to greatly reduce colonization of the suture compared to controls as illustrated by scanning electron microscopy. These data support the conclusion that coated polyglactin 910 suture with triclosan provides an antimicrobial effect sufficient to prevent in vitro colonization of the suture by *Staphylococcus aureus* and *Staphylococcus epidermidis*.

Moreover, coated medical devices may be stable for extended periods of time. During storage, coated devices may maintain a sufficient amount of triclosan to exhibit desired antimicrobial effects. Standard accelerated aging tests may be used to estimate antimicrobial properties after exposure to typical storage conditions.

Upon exposure to accelerated aging tests, triclosan coated sutures exhibited zones of inhibition against *Staphylococcus aureus* and *Staphylococcus epidermidis*. In particular, triclosan coated sutures were exposed to 50°C for 157 days. Table 6 indicates triclosan loss from various USP size 2-0 coated dyed polyglactin 910 sutures with varying levels of triclosan upon exposure of the sutures to 50°C for 157 days. The exposure took place after the sutures had been ethylene oxide sterilized and placed in a hot room for three days. Table 7 exhibits antimicrobial properties of those sutures after such exposure. As indicated in Table 7, zones of inhibition were exhibited against both *Staphylococcus aureus* and *Staphylococcus epidermidis* after exposure. Although no zones of inhibition were exhibited against *Streptococcus agalactiae* under these testing conditions, higher concentrations of triclosan are known to inhibit growth of *Streptococcus agalactiae*. It is important to note that standard accelerated aging tests do not employ true hospital storage conditions, and thus, typically demonstrate worst-case scenarios. As such, the stability of triclosan coated sutures is believed to be significantly longer under normal shelf-storage conditions.

Table 6. Triclosan Loss at 50°C for 2-0 Dyed Vicryl Suture After Ethylene Oxide Sterilization and 3 Days in Hot Room

<i>1% Solution</i>		<i>2% Solution</i>		<i>3% Solution</i>	
at 50°C	Irgacare	at 50°C	Irgacare	at 50°C	Irgacare
<u>Days</u>	<u>ppm</u>	<u>Days</u>	<u>ppm</u>	<u>Days</u>	<u>ppm</u>
0	200	0	295	0	333
3	127	3	216	3	266
3	132	3	235	3	291
3	156	3	230	3	291
11	94	11	163	11	227
11	91	11	163	11	213
18	89	18	140	18	189
32	69	32	120	32	155
58	58	58	108	58	164

157	59	157	118	157	130
157	39	157	79	157	101

Table 7: Zones of Inhibition for 2-0 Dyed Vicryl Suture After Exposure to 50°C for 157 Days

Triclosan Coating Conc. (%)	Triclosan on Suture (ppm)	Storage Conditions/ Sterilization Cycle	Zone of Inhibition (Yes/No)					
			S. aureus		Strep agalacticae		S. epidermidis	
			24 hr.	48 hr.	24 hr.	48 hr.	24 hr.	48 hr.
			No	No	No	No	No	No
1.0	39	50C for 157 days / N cycle	Yes	No	No	No	Yes	Yes
2.0	79	50C for 157 days / N cycle	Yes	Yes	No	No	Yes	Yes
3.0	101	50C for 157 days / N cycle	Yes	Yes	No	No	Yes	Yes
1.0	59	50C for 157 days / N cycle	Yes	No	No	No	Yes	Yes
2.0	118	50C for 157 days / N cycle	Yes	Yes	No	No	Yes	Yes
3.0	130	50C for 157 days / N cycle	Yes	Yes	No	No	Yes	Yes

**WHAT IS CLAIMED IS:**

1. An antimicrobial suture assembly comprising:  
a containment compartment comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the  
5 group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said containment compartment; and  
a suture positioned within the containment compartment, the suture comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent  
10 being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the suture.
2. The suture assembly according to Claim 1, wherein the suture has a polymeric coating containing the antimicrobial agent.
- 15 3. The suture assembly according to Claim 2, wherein the suture is formed from a plurality of polymeric filaments.
4. The suture assembly according to Claim 1, wherein the suture is a monofilament suture.
5. The suture assembly according to Claim 3, wherein the plurality of  
20 filaments is formed into a braided structure
6. The suture assembly according to Claim 5, wherein the plurality of filaments is formed from a material that is absorbable under physiological conditions.
7. The suture assembly according to Claim 6, further comprising a needle.



8. The suture assembly according to Claim 1, wherein the containment compartment further comprises a winding channel or retaining members for securing the suture.

9. The suture assembly according to Claim 8, further comprising a paper or plastic cover positioned over the winding channel or retaining members, wherein the cover comprises one or more surfaces having said antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said cover.

10. A packaged suture having antimicrobial properties comprising:  
an outer package comprising an inner surface having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said inner surface of said outer package; and

a suture assembly comprising:

a containment compartment comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said containment compartment; and

a suture positioned within the containment compartment, the suture comprising one or more surfaces having an antimicrobial agent disposed thereon, said

antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on the suture.

11. An antimicrobial suture assembly comprising:
  - 5 a containment compartment comprising one or more surfaces having between about 5 ppm and 5000 ppm of 2,4,4'-trichloro-2'-hydroxydiphenyl ether disposed thereon, to substantially inhibit bacterial colonization on said containment compartment; and
  - an elongate braided suture positioned within the containment compartment, said elongate braided suture formed from a plurality of filaments of a polymeric material
  - 10 comprising greater than about 70% polymerized glycolide and comprising one or more surfaces having a coating disposed thereon, said coating comprising a film-forming absorbable polymer, a substantially water-insoluble salt of a fatty acid and between about 30 ppm and 5000 ppm of 2,4,4'-trichloro-2'-hydroxydiphenyl ether to substantially inhibit bacterial colonization on said braided suture.
- 15 12. A packaged antimicrobial suture produced according to the process of:
  - providing a containment compartment that is substantially free of an antimicrobial agent;
  - positioning a suture within the containment compartment, said suture comprising
  - one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial
  - 20 agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof;
  - placing the containment compartment having the suture in an outer package; and

subjecting the outer package, the containment compartment and the suture to time, temperature and pressure conditions sufficient to vapor transfer an effective amount of the antimicrobial agent from the suture to the containment compartment, while retaining an effective amount of said antimicrobial agent on the suture, thereby substantially inhibiting bacterial colonization on the suture and the containment compartment.

13. A method of making a packaged antimicrobial suture comprising the steps of:

providing a containment compartment that is substantially free of an antimicrobial agent;

10 positioning a suture within the containment compartment, said suture comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof;

placing the containment compartment having the suture in an outer package; and

15 subjecting the outer package, the containment compartment and the suture to time, temperature and pressure conditions sufficient to vapor transfer an effective amount of the antimicrobial agent from the suture to the containment compartment, while retaining an effective amount of said antimicrobial agent on the suture, thereby substantially inhibiting bacterial colonization on the suture and the containment compartment.

20 14. The method for making a packaged antimicrobial suture according to Claim 13, wherein the effective amount of the antimicrobial agent is vapor transferred to the containment compartment during an ethylene oxide sterilization process.

15. The method for making a packaged antimicrobial suture according to Claim 13, wherein the step of subjecting the outer package, the containment compartment and the suture to conditions sufficient to vapor transfer an effective amount of the antimicrobial agent comprises the steps of:
- 5 placing the outer package having the containment compartment and the suture therein in a sterilization unit;
- heating the sterilization unit to a first temperature;
- adjusting the pressure in the sterilization unit to a first pressure value;
- injecting steam into the sterilization unit to expose the outer package, the
- 10 containment compartment and the suture to water vapor for a first period of time;
- adjusting the pressure within the sterilization unit to a second pressure value;
- introducing a chemical sterilization agent into the sterilization unit;
- maintaining the chemical sterilization agent in the sterilization unit for a second
- period of time to render a sufficient amount of microorganisms within the package non-
- 15 viable;
- removing residual moisture and chemical sterilization agent from the suture;
- and
- drying the packaged antimicrobial suture to a desired moisture level.
16. The method for making a packaged antimicrobial suture according to Claim
- 20 15, wherein the step of introducing a chemical sterilization agent comprises introducing ethylene oxide gas into the sterilization unit.
17. A packaged medical device having antimicrobial properties, comprising:

at least one hermetically sealed package comprising an inner surface having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization  
5 on said package; and

at least one implantable medical device positioned within said at least one hermetically sealed package, said medical device comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and  
10 combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said medical device.

18. The packaged medical device according to Claim 17, wherein said medical device has a polymeric coating containing the antimicrobial agent.

19. The packaged medical device according to Claim 18, wherein said medical  
15 device is formed from a plurality of filaments.

20. The packaged medical device according to Claim 19, wherein the medical device formed from a plurality of filaments is a braided suture.

21. The packaged medical device according to Claim 20, wherein the braided suture is absorbable under physiological conditions.

20 22. The packaged medical device according to claim 17, wherein the device is a monofilament suture

23. The packaged medical device according to claim 22, wherein the monofilament suture is formed from a polymeric material that is absorbable under physiological conditions.

24. The packaged medical device according to Claim 17, wherein the medical  
5 device is selected from the group consisting of surgical meshes and films, hernia plugs, brachy seed spacers and surgical knot clips.

25. A packaged medical device having antimicrobial properties, comprising:  
at least one package comprising an inner surface having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of  
10 halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said package; and  
at least one implantable medical device positioned within said at least one package, said medical device being selected from the group consisting of sutures, surgical meshes, hernia plugs, brachy seed spacers, suture clips, suture anchors, adhesion prevention meshes  
15 and films, and suture knot clips; and said medical device comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof, in an amount sufficient to substantially inhibit bacterial colonization on said medical device.

20 26. The packaged medical device according to Claim 25, wherein the medical device is selected from the group consisting of surgical meshes and films, hernia plugs, brachy seed spacers and surgical knot clips.

27. A packaged medical device produced according to the process of:

providing a package comprising an inner surface that is substantially free of an antimicrobial agent;

positioning a medical device within the package, said medical device comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof; and

subjecting the package and the medical device to time, temperature and pressure conditions sufficient to vapor transfer an effective amount of the antimicrobial agent from the medical device to the inner surface of the package, while retaining an effective amount of said antimicrobial agent on the medical device, thereby substantially inhibiting bacterial colonization on the medical device and the inner surface of the package.

28. A method of making a packaged medical device comprising the steps of:


providing a package comprising an inner surface that is substantially free of an antimicrobial agent;

positioning a medical device within the package, said medical device comprising one or more surfaces having an antimicrobial agent disposed thereon, said antimicrobial agent being selected from the group consisting of halogenated hydroxyl ethers, acyloxydiphenyl ethers, and combinations thereof; and

subjecting the package and the medical device to time, temperature and pressure conditions sufficient to vapor transfer an effective amount of the antimicrobial agent from the medical device to the inner surface of the package, while retaining an effective amount of said antimicrobial agent on the medical device, thereby substantially inhibiting bacterial colonization on the medical device and the inner surface of the package.

1/5


**FIG. 1**  
Triclosan Transfer from Suture to Tray

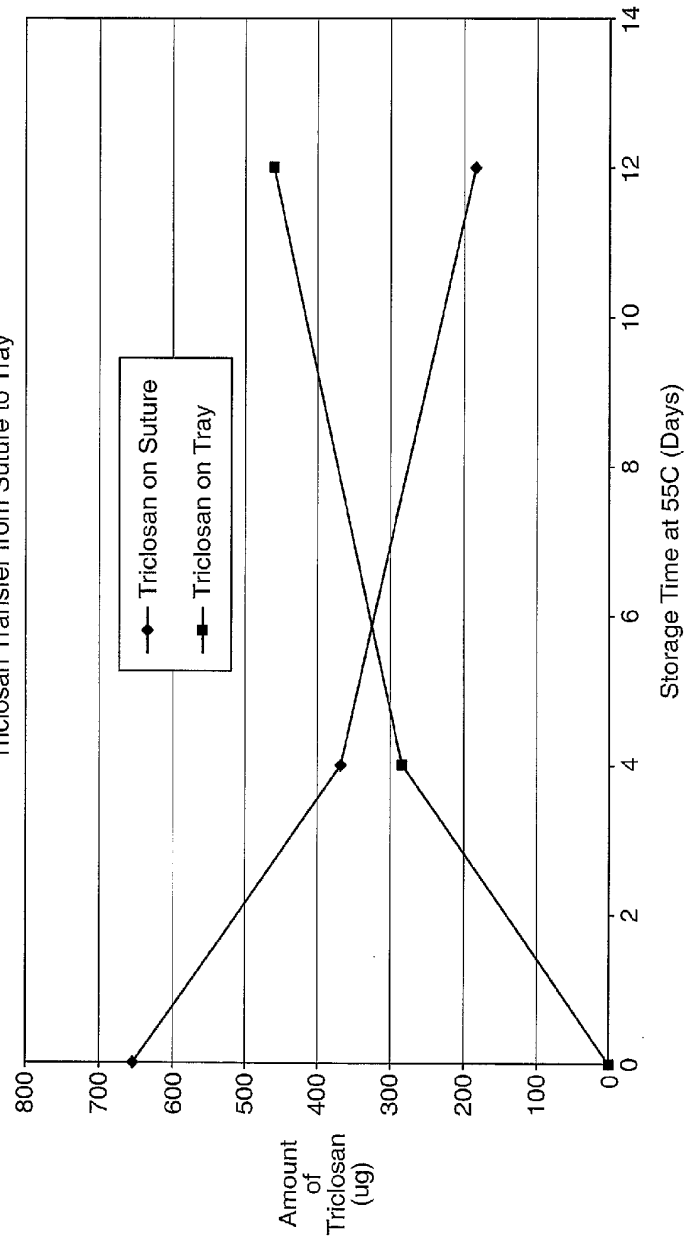




2/5

**FIG. 2**

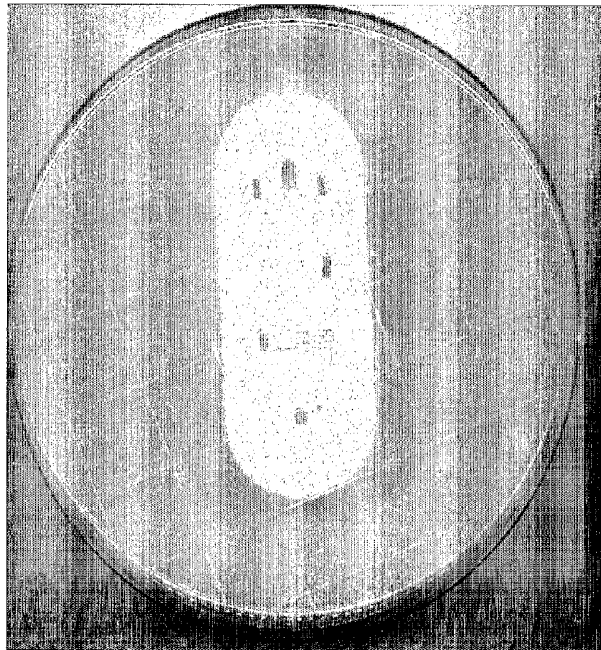


3/5

**FIG. 3**

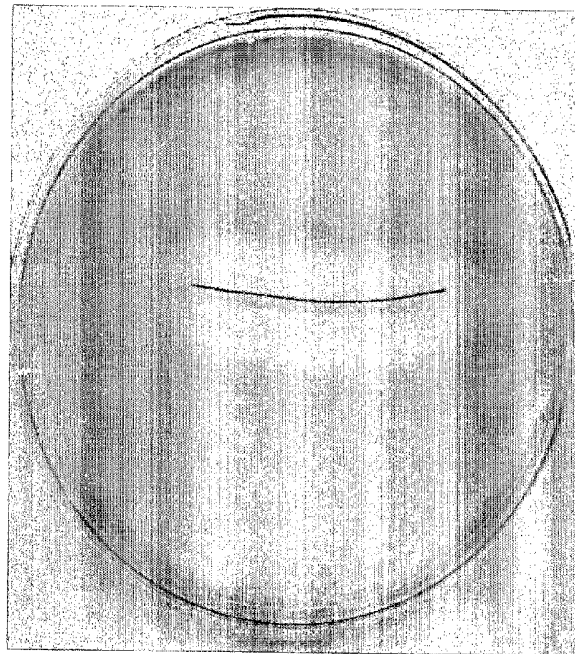

4/5

**FIG. 4**

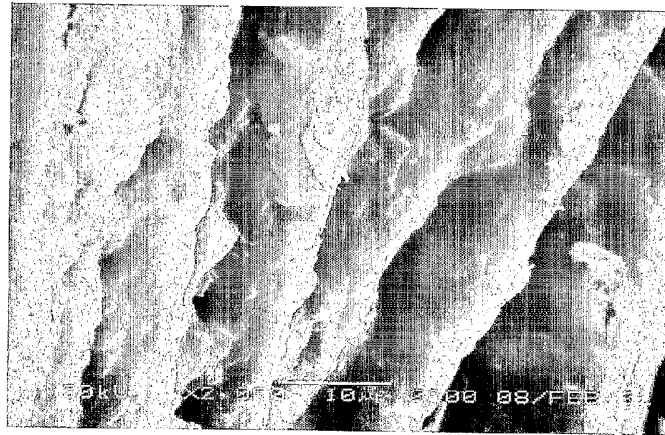

5/5

**FIG. 5**

