



(51) International Patent Classification:

A61M 16/06 (2006.01) A62B 7/04 (2006.01)

A61M 16/00 (2006.01)

(21) International Application Number:

PCT/US2022/025668

(22) International Filing Date:

21 April 2022 (21.04.2022)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

63/185,053 06 May 2021 (06.05.2021) US

(71) Applicant: **DUKE UNIVERSITY** [US/US]; 2812 Erwin Road, Suite 306, Durham, North Carolina 27705 (US).

(72) Inventors: **DRIEHUYS, Bastiaan**; 111 Graylyn Drive, Chapel Hill, North Carolina 27101 (US). **CHURCH, Alexander**; 3806 University Dr., Apt. 259, Durham, North Carolina 27707 (US).

(74) Agent: **RICHARDSON, Julie H.**; MYERS BIGEL, P.A., PO Box 37428, Raleigh, North Carolina 27627 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,

DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, IT, JM, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

— of inventorship (Rule 4.17(iv))

Published:

— with international search report (Art. 21(3))

(54) Title: GAS INHALATION DELIVERY DEVICES AND RELATED METHODS

(57) Abstract: Devices that allow serially controlled delivery of room air for practice inhalation and breath-hold procedures and a different (image contrast) gas for inhalation for a medical procedure include an actuator that is controllably, pneumatically operated by a user via a length of conduit.

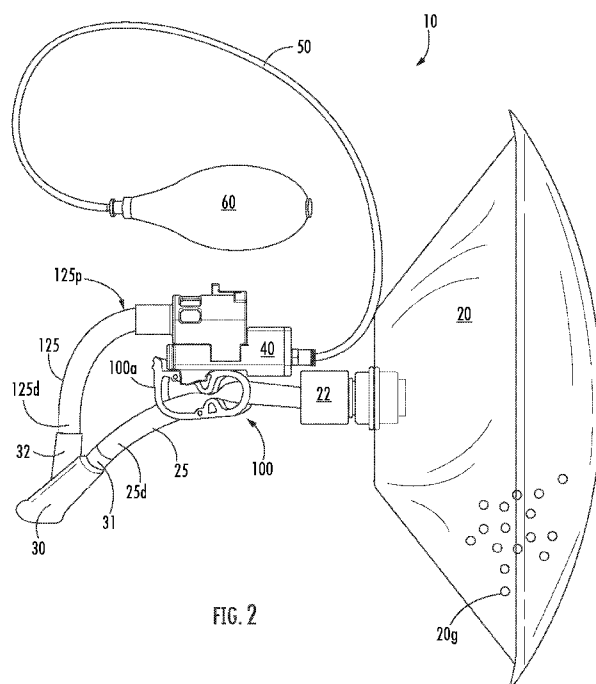


FIG. 2

GAS INHALATION DELIVERY DEVICES AND RELATED METHODS

RELATED APPLICATIONS

[0001] This application claims the benefit of and priority to U.S. Provisional Application Serial Number 63/185,053, filed May 6, 2021, the contents of which are hereby incorporated by reference as if recited in full herein.

GOVERNMENT GRANTS

[0002] The invention was made with government support under Grant Numbers R01HL126771 and R01HL105643 awarded by the National Institutes of Health/National Heart, Lung & Blood Institute. The United States government has certain rights in the invention.

FIELD OF THE INVENTION

[0003] The invention relates to gas delivery devices that are particularly suitable for inhalation delivery of gases for use in imaging, such as for MRI evaluations.

BACKGROUND

[0004] Hyperpolarized (which may also be referred to in an abbreviated form “HP”) ^{129}Xe MRI is emerging as a valuable means of imaging lung structure and function. *See* Kruger et al. Functional imaging of the lungs with gas agents. *Journal of Magnetic Resonance Imaging*. 2016;43(2):295-315; Matin et al. Chronic obstructive pulmonary disease: lobar analysis with hyperpolarized ^{129}Xe MR imaging. *Radiology*. 2016;282(3):857-868, the contents of which are hereby incorporated by reference as if recited in full herein. Hyperpolarized ^{129}Xe MRI is used for high-resolution, non-invasive 3D imaging of pulmonary function and to obtain dynamic and static spectral parameters for assessing lung function. *See, e.g.*, U.S. Patent No. 8,911,709 and U.S. Patent Application Publication Number 2020/0022616, the contents of which are also incorporated by reference as if recited in full herein.

[0005] It can be important to ensure that image or spectroscopy data are highly repeatable for clinical evaluations. Thus, ensuring that patients begin their inhalation of HP gas from a well-defined lung volume, quickly and comfortably within the confines of the MRI scanner can facilitate such an outcome.

[0006] Conventionally, a single-use dose delivery bag with a pinch valve as shown in **FIGs. 1A** and **1B** has been used for providing HP gas to a patient for inhalation during an MRI imaging session. The HP gas in the dose delivery bag can comprise about a liter of about 1% enriched ^{129}Xe , about 10% nitrogen and about 89% helium as a drug component of a drug-device combination product provided by Polarean, Inc., Durham, NC. Current methods of dose administration involve a technician such as a Clinical Research Coordinator (CRC) coaching the patient to take some preparatory room air breaths and then to exhale fully before inhaling the gas from the dose delivery bag. Once the preparatory room air breathing is completed, the technician then places the mouthpiece of the dose delivery bag in the patient's mouth, opens the pinch valve, and rapidly releases the contents of the bag, squeezing the bag to facilitate the entire content is inhaled while coaching the patient to breathe in rapidly, e.g., saying “breathe in... breathe in...breathe in” and after about 6-8 seconds of inhalation, say “hold it” which can be used to signal the MRI operator to initiate the scan. However, as shown in **FIG. 1B**, the delivery procedure is challenged by the confined space of the MRI machine, often requiring a coordinator to reach into the bore of the magnet to reach the patient's mouth and/or to release the pinch valve using a hand that is adjacent the mouth and nose of the patient. This can lead to significant delays and confusion, undesirably causing a patient to inhale some air before the dose, and/or change their lung inflation level.

[0007] There is a need for alternate devices that can deliver gas for inhalation for a medical procedure, such as an MRI imaging session.

SUMMARY

[0008] Embodiments of the present invention provide a compact inhalation delivery device that can serially administer either room air (and vent to room) or image contrast gas in a controlled manner.

[0009] The dose delivery device includes a pneumatic actuator assembly. The actuator controls at least one valve that allows the patient to inhale room air during practice inhalation procedures and to inhale gas from a dose delivery bag for a “breath-hold” inhalation for an imaging session.

[0010] This device can allow a clinician or technical assistant such as an MRI technologist to remain outside of a magnet bore during imaging (potentially in a position to initiate an image scan and actuate the actuation assembly of the device) as well as allows the

patient to keep the mouthpiece in their mouth or face mask on their face during practice inhalations of room air then actual dose administration.

[0011] Embodiments of the present invention are directed to an inhalation gas delivery device that includes: an inhalation delivery output member; a bag of gas for inhalation in fluid communication with the inhalation delivery output member; and an actuator assembly with an actuator member. The actuator member has a first position which allows room air to flow along a first (optionally enclosed) flow path to the inhalation gas output member and the actuator member has a second position which allows gas from the bag to flow along a second enclosed flow path to the inhalation gas output member.

[0012] The device can also include a conduit in fluid communication with the actuator assembly whereby a user pneumatically actuates the actuator member via the conduit to move from the first position to the second position.

[0013] The inhalation gas delivery device can be non-ferromagnetic and can be configured for use in an MRI scanner room.

[0014] The inhalation gas delivery device can vent expiration breaths of inhaled air and inhaled gas to atmosphere.

[0015] The actuator member can have a piston that travels a stroke distance in a range of about 5 mm and about 10 mm between the first and second positions.

[0016] The actuator assembly can have a housing that encloses at least part of a piston. The housing can have at least one air inlet (vent) downstream of the piston and the actuator assembly can close the at least one air inlet when the actuator member is in the second position.

[0017] The inhalation gas delivery device can further include a housing having an air vent closure member that is coupled to the actuator member. The air vent closure member can slide linearly in concert with the actuator member as the actuator member moves from the first position to the second position.

[0018] The gas in the bag can include hyperpolarized noble gas. The inhalation gas delivery device can be non-ferromagnetic.

[0019] The hyperpolarized noble gas can be ^{129}Xe .

[0020] The bag and the actuator assembly can reside a (short) distance in a range of about 0.1 inches (2.54 mm)-12 inches (30.4 cm) from the inhalation delivery output member.

[0021] The actuator assembly can have a housing with an internal chamber. The housing can have an outer wall with at least one air inlet (or vent). The actuator member can include a piston with a first segment having a first outer diameter and a second segment

having a second outer diameter. The first segment can have a face with a seal or the face can cooperate with a component that has a seal that seals the gas from the bag from flowing through the piston when the piston is in the first position.

[0022] The first segment can have at least one gas intake inlet adjacent the face seal surface. The second segment can block the at least one air inlet when the actuator member is in the second position.

[0023] The second segment can have first and second seals axially spaced apart and extending about the outer diameter thereof,

[0024] At least one air inlet can reside between the first and second seals when the actuator member is in the second position.

[0025] The piston can have a flat circumferentially extending working surface that projects radially outward and extends between the first and second segments.

[0026] The inhalation gas delivery device can further include a length of conduit coupled to the housing and in fluid communication with a pressurized fluid source and in fluid communication with the working surface of the piston whereby pressurized fluid input into the housing from the conduit actuates the piston to move to the second position.

[0027] The actuator assembly can have a housing and the housing can have an outer wall with at least one air inlet. The piston resides in the housing and the piston comprises a proximal end that comprises a plurality of gas intake inlets that merge into an open channel downstream of the gas intake inlets and forming part of the second flow path.

[0028] The actuation assembly can have a housing with an internal chamber and a piston as the actuation member inside the internal chamber. The housing can have air inlets providing intake of room air for the first flow path. The piston can have gas intake inlets upstream of the air inlets and the piston can block the air inlets in the second position and the piston can seal the gas intake inlets when the piston is in the first position.

[0029] The inhalation delivery device can further include a pressurized fluid source comprising a syringe coupled to a length of conduit and to the actuator assembly or a compressible bulb coupled to a length of conduit and to the actuator assembly.

[0030] The inhalation delivery output member can have a single branch that serially defines part of the first flow path and part of the second flow path.

[0031] The inhalation delivery output member comprises a first branch that defines part of the first flow path and a separate second branch that defines part of the second flow path.

[0032] Other embodiments are directed to methods of providing inhalable gas for a medical procedure. The methods can include: providing a bag of inhalable gas; providing an inhalation delivery output member such as a face mask or mouthpiece; and connecting an actuator assembly to the bag and to the inhalation delivery output member. The actuator assembly and the bag reside within 0.1-12 inches (2.54 mm-30.48 cm) from a face of the patient. The method also includes; placing the inhalation delivery output member on a face over a nose and mouth or in a mouth of a patient; directing the patient to inhale practice room air breaths with the inhalation delivery output member on the face or in the mouth while an actuator member of the actuator assembly is in a first position providing open air inlets; and then actuating the actuating assembly to move the actuator member to a second position to close the air inlets and open gas intake inlets to provide a flow path that directs gas from the bag of inhalable gas to flow to the inhalation delivery output member for inhalation by the patient.

[0033] The medical procedure can be an MRI imaging session.

[0034] The actuator assembly can be manually actuated via a pressurized fluid source in communication with the actuator assembly via a conduit that can optionally have a length in a range of 1-12 feet or 1-10 feet.

[0035] The inhalable gas can include hyperpolarized ^{129}Xe gas.

[0036] Other devices and/or methods according to embodiments of the invention will be or become apparent to one with skill in the art upon review of the following drawings and detailed description. It is intended that all such additional devices and methods be included within this description, be within the scope of the present invention, and be protected by the accompanying claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0037] Features of the present invention will be more readily understood from the following detailed description of exemplary embodiments thereof when read in conjunction with the accompanying drawings.

[0038] **FIG. 1A** is a digital photograph of a prior art dose delivery device.

[0039] **FIG. 1B** shows the dose delivery device of **FIG. 1A** in use with a patient in a bore of a magnet of an MRI scanner.

[0040] **FIG. 2** is a top view of a dose delivery device according to embodiments of the present invention.

[0041] FIG. 3 is a top view of the dose delivery device shown in FIG. 2 illustrating alternate flow paths according to embodiments of the present invention.

[0042] FIG. 4 illustrates the dose delivery device in use with a patient and a technician according to embodiments of the present invention.

[0043] FIG. 5A is an enlarged side view of an example actuator assembly of the dose delivery device shown in FIG. 2 according to embodiments of the present invention.

[0044] FIG. 5B is an enlarged side view of the example actuator assembly of the dose delivery device shown in FIG. 5A with the air vents/inlets closed according to embodiments of the present invention.

[0045] FIG. 6 is a top view of another embodiment of a dose delivery system according to embodiments of the present invention.

[0046] FIG. 7A is a side perspective, section view of the actuator assembly shown in FIG. 5A, illustrating the air closure member and actuator member in respective first positions according to embodiments of the present invention.

[0047] FIG. 7B is a side view of the section view shown in FIG. 7A.

[0048] FIG. 7C is another side perspective, section view of the actuator assembly shown in FIG. 5A illustrating the air closure member and actuator member in a second operative position from the first operative position shown in FIG. 7A according to embodiments of the present invention.

[0049] FIG. 7D is a side view of the section view shown in FIG. 7C.

[0050] FIG. 8 is a schematic side view of another embodiment of a dose delivery system according to embodiments of the present invention.

[0051] FIG. 9A is a partial section view of a part of a dose delivery system with a piston in a first, home position according to embodiments of the present invention.

[0052] FIG. 9B is a partial section view of the part of the dose delivery system shown in FIG. 9A but with the piston in a second, extended position according to embodiments of the present invention.

[0053] FIG. 10 is an enlarged front, side perspective view of the piston shown in FIGs. 8, 9A and 9B according to embodiments of the present invention.

[0054] FIG. 11 is a rear view of the piston shown in FIG. 10.

[0055] FIG. 12 is an enlarged front, side perspective view of another embodiment of the piston shown in FIG. 10 according to embodiments of the present invention.

[0056] FIGs. 13A and 13B are side perspective view of a dose delivery system similar to the system shown in FIG. 8 but with the actuator assembly comprising a fluid port

connected to a conduit and a pressurized fluid source according to embodiments of the present invention.

[0057] FIGs. 14A and 14B illustrate the conduit and user input providing part of the actuator control shown in FIGs. 13A and 13B, respectively.

[0058] FIG. 15 is an enlarged side perspective view of a part of the dose delivery system shown in FIGs. 13A and 13B.

[0059] FIG. 16 is a top view of another embodiment of a dose delivery system according to embodiments of the present invention.

[0060] FIG. 17 is a partially exploded side, perspective view of the dose delivery system shown in FIG. 16.

[0061] FIG. 18A is an enlarged top, perspective view of the actuator assembly and part of the bag conduit shown in FIG. 16.

[0062] FIG. 18B is an enlarged side view of the actuator assembly and part of the bag conduit shown in FIG. 18A.

[0063] FIG. 19A illustrates the air flow path when the piston of the actuator assembly is in a first position.

[0064] FIG. 19B illustrates a gas flow path when the piston of the actuator assembly is in a second position.

[0065] FIG. 20 is an enlarged, side perspective view of the actuator assembly shown in FIG. 16.

[0066] FIG. 21 is a disassembled view of the actuator assembly shown in FIG. 20.

[0067] FIG. 22A is an enlarged cross-sectional view of the actuator assembly shown in FIG. 20 with the internal piston in a first position allowing room air to flow therethrough according to embodiments of the present invention.

[0068] FIG. 22B is an enlarged cross-sectional view of the actuator assembly shown in FIG. 22A with the internal piston in a second position blocking room air and allowing (hyperpolarized) gas to flow therethrough according to embodiments of the present invention.

[0069] FIG. 23 is an enlarged, side perspective cross-sectional view of the actuator assembly shown with the piston in the position shown in FIG. 22A.

[0070] FIG. 24A is a side, end perspective view of the example piston of the actuator assembly shown in FIG. 23.

[0071] FIG. 24B is an opposing end perspective view of the example piston shown in FIG 24A.

[0072] **FIGs. 25A-FIG. 25C** are illustrations of a sequence of actions that can be used to position the dose delivery device, then deliver the gas from a bag while a patient is inside the scanner according to embodiments of the present invention.

[0073] **FIG. 26** is a flow chart of example actions that can be used to deliver a dose of gas to a patient for a medical procedure according to embodiments of the present invention.

DETAILED DESCRIPTION

[0074] While the invention may be made in modified and alternative forms, specific embodiments thereof are shown by way of example in the drawings and will be described in detail. It should be understood, however, that there is no intent to limit the invention to the particular forms disclosed, but on the contrary, the invention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention. Like reference numbers signify like elements throughout the description of the figures.

[0075] In the figures, the thickness of certain lines, layers, components, elements or features may be exaggerated for clarity. Broken lines illustrate optional features or operations unless specified otherwise. The sequence of operations (or steps) is not limited to the order presented in the claims or figures unless specifically indicated otherwise.

[0076] The terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting of the invention. As used herein, the singular forms "a", "an" and "the" are intended to include the plural forms as well, unless the context clearly indicates otherwise. It will be further understood that the terms "comprises" and/or "comprising," when used in this specification, specify the presence of stated features, integers, steps, operations, elements, and/or components, but do not preclude the presence or addition of one or more other features, integers, steps, operations, elements, components, and/or groups thereof. As used herein, the term "and/or" includes any and all combinations of one or more of the associated listed items. As used herein, phrases such as "between X and Y" and "between about X and Y" should be interpreted to include X and Y. As used herein, phrases such as "between about X and Y" mean "between about X and about Y." As used herein, phrases such as "from about X to Y" mean "from about X to about Y."

[0077] Unless otherwise defined, all terms (including technical and scientific terms) used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. It will be further understood that terms, such as those defined in commonly used dictionaries, should be interpreted as having a meaning that is consistent with their meaning in the context of the specification and relevant art and should

not be interpreted in an idealized or overly formal sense unless expressly so defined herein. Well-known functions or constructions may not be described in detail for brevity and/or clarity.

[0078] It will be understood that, although the terms first, second, etc. may be used herein to describe various elements, components, regions, layers and/or sections, these elements, components, regions, layers and/or sections should not be limited by these terms. These terms are only used to distinguish one element, component, region, layer or section from another region, layer or section. Thus, a first element, component, region, layer or section discussed below could be termed a second element, component, region, layer or section without departing from the teachings of the present invention.

[0079] The term "MRI scanner" refers to a magnetic resonance imaging and/or NMR spectroscopy system. As is well known, the MRI scanners include a low field strength magnet (typically between about .1T to about .5T), a medium or a high-field strength superconducting magnet, an RF pulse excitation system, and a gradient field system. MRI scanners are well known to those of skill in the art. Examples of commercially available clinical MRI scanners include, for example, those provided by General Electric Medical Systems, Siemens, Philips, Varian, Bruker, Marconi, Hitachi and Toshiba. The MRI systems can be any suitable magnetic field strength, such as, for example, about 1.5T or higher field systems of between about 2.0T-10.0T.

[0080] The term "high-field strength" refers to magnetic field strengths above 1.0T, typically above 1.5T, such as 2.0T or 3.0T. However, the present invention is not limited to these field strengths and may be suitable for use with lower or higher field strength magnets, such as, for example, 3.0T or even greater or even with other imaging modalities.

[0081] The term "hyperpolarized" refers to a noble gas such as ^3He or ^{129}Xe that has increased polarization over natural or equilibrium levels. As is known by those of skill in the art, hyperpolarization can be induced by spin-exchange with an optically pumped alkali-metal vapor. *See* Albert et al., U.S. Patent No. 5,545,396; and Cates et al, U.S. Patent Nos. 5,642,625 and U.S. Patent No. 5,809,801. These references are hereby incorporated by reference as if recited in full herein. One polarizer that is suitable for generating the hyperpolarized ^{129}Xe is the 9800, 9810 or 9820 polarizer models made by Polarean, Imaging, plc, Durham, NC. Thus, as used herein, the terms "hyperpolarize", "polarize", and the like mean to artificially enhance the polarization of certain noble gas nuclei over the natural or equilibrium levels.

[0082] Embodiments of the invention may be particularly suitable for use with human patients but may also be used with animals or other mammalian subjects.

[0083] Turning now to **FIGs. 2-4, 5A and 5B**, an example dose delivery device **10** is shown. In the embodiment shown, the dose delivery device includes a bag **20** and a tube **25** sealably coupled to the bag **20** via a connector **22**. The dose delivery device **10** also includes an inhalation delivery output member **30** sealably coupled to the tube **25** and an actuator assembly **40** in communication with a valve **100** that can controllably open and close the flow path **25f** provided by the tube **25** between the gas **20g** in the bag **20** and the inhalation delivery output member **30**.

[0084] The bag **20** can be a medical grade Tedlar® film bag (from the polyvinyl fluoride family). *See also*, U.S. Patent No. 6,128,918, the contents of which are hereby incorporated by reference as if recited in full herein.

[0085] The valve **100** can be a clamp or pinch valve that externally clamps/pinches the tube **25** to close the associated flow path **25f**.

[0086] The inhalation delivery output member **30** can comprise a first branch **31** that couples to a distal end portion **25d** of the tube **25** and a second branch **32** that couples to a distal end portion **125d** of a secondary tube **125**. The secondary tube **125** can define an airflow path **125f** between room air and the inhalation delivery output member **30**.

[0087] The conduit **50** can have a smaller inner and outer diameter than the tube **25** and/or tube **125** and can have a length that is longer than either of the tubes **25**, **125**. In some embodiments, the conduit **50** can have a (loose) length that is in a range of about 1 foot and about 12 feet, preferably 2-10 feet, more preferably 3-8 feet, such as about 3 feet, about 4 feet, about 5 feet and about 6 feet, about 7 feet and about 8 feet thereby allowing the user/technician to reside relatively close to the patient for “coaching” the breath hold procedure while the inhalation delivery output member **30** is in/on the patient with the bag **20** adjacent thereto and in operative position. The loose length of conduit **50** can allow the technician to reside a distance away from/outside the bore **200b** of the magnet **200** and inside the scanner room **205** (**FIG. 4**) of an MRI suite.

[0088] The delivery device **10** can be configured to allow a single technologist to perform the procedure with a respective patient, including both actuating the actuator assembly **40** to deliver the dose of gas from the bag **20** for breath hold and initiating a scan during an MRI imaging session.

[0089] The conduit **50** can be flexible and extend down from a face of a user as it exits the magnet bore **200b**. The bag **20** and actuator assembly **40** can reside within 0.1-12

inches of a face of a patient and/or from the inhalation delivery output member **30**, e.g., close to the face of a patient, and adjacent to or partially or totally within the bore **200b** as shown in **FIG. 4**.

[0090] The conduit **50** can be in fluid communication with a pressurized gas source **60** such as a bulb **60b** (**FIGs. 2-4**) or syringe **60s** (**FIG. 6**).

[0091] The actuator assembly **40** can have a first connector **50c** that couples to a conduit **50** that connects to a pressurized gas source **60** that provides pneumatic input to the actuator assembly **40**. The actuator assembly **40** can have a second connector **125c** that connects to a proximal end portion **125p** of the secondary tube **125** providing the air input/output paths. The second connector **125c** can reside in-line with and proximate to at least one air inlet **43** (interchangeably referred to as “air vent” herein), shown as a plurality of adjacent air inlets **43**.

[0092] Referring to **FIGs. 5A** and **5B**, the actuator assembly **40** can comprise a housing **40h** and an actuator member **45** that has a linear stroke distance **L**. The actuator member **45** can be configured as and/or comprise a piston **45p** (**FIG. 7A**) in fluid communication with the conduit **50**. The stroke distance **L** can be relatively small such as a range of about 4-30 mm, more typically a range of about 5-10 mm such as about 8.5 mm, in some embodiments, for example. The actuator member **45** can have a first (home) position which is a retracted position whereby the valve **100** is pinched to close the flow path **25p**. The actuator member **45** can have a second extended position (**FIG. 5B**) whereby the valve **100** is un-pinched and opens the flow path **25**. Thus, when extended, the actuator member **45** pushes against an arm **100a** of the valve **100** to decompress the tube **25** sufficiently to open the flow path **25f**.

[0093] In some embodiments, the actuator assembly **40** can be configured, simultaneous with the extension of the actuator member **45**, to direct an air (inlet) closure member **48** to move to close the air inlets **43** thereby preventing the patient from inhaling air through the inhalation delivery output member **30**. The air closure member **48** can be coupled to the actuator member **45** and may slidably move axially parallel to and in concert with the actuator member **45**.

[0094] Referring to **FIGs. 7A, 7B, 7C** and **7D**, the actuator assembly **40** has first and second internal chambers **47₁**, **47₂**, one, above the other, the first chamber **47₁** enclosing the air closure member **48** and the second chamber **47₂** enclosing the piston **45p**. The piston **45p** can be sealably coupled to the second chamber **47₂** via a seal **49**, such an O-ring, on the piston **45p** adjacent the connector **50c** for the conduit **50**.

[0095] The actuator assembly 40 can also include a seal 42 configured as a face seal for closing/sealing the air closure member 48 against the distal end 47d of the chamber 47₁.

[0096] Still referring to FIGs. 7A-7D, the actuator assembly 40 can include a locking pawl 41 that locks the air closure member 48 in the closed position (FIGs. 7C, 7D) once the actuator assembly 40 is actuated to open the valve 100. The locking pawl 41 can be configured to block a proximal end of the air closure member 48 to keep the air closure member 48 from retracting.

[0097] The air closure member 48 can include a coupler segment 48c that is coupled to the actuator member 45. The coupler segment 48c can slidably reside inside the second chamber 47₂, inside a slot 45s formed in the actuator member 45.

[0098] Referring to FIG. 3, the example alternate flow paths 25f, 125f are shown with the appended arrows. The preparatory air flow breaths are allowed via tube 125 for air flow path 125 with air in-taken into the flow path 125f via the air inlets 43 (FIG. 5A) while the valve 100 closes the flow path 25f. When the actuator assembly 40 opens the valve 100, it closes the air inlets 43 so that the patient inhales the gas from the bag 20 via flow path 25f. Thus, the actuation assembly 40 of the inhalation delivery device 10 is actuated to close the air inlets (vents) 43 when positive pressure is applied.

[0099] In some embodiments, pressure can be (manually) applied externally to compress the bulb 60b (FIG. 2) or move a plunger of a syringe 60s (FIG. 6) to provide positive pressure to keep air inlets 43 (FIG. 5A) open to room air while the actuator member 45 is in the home or retracted (first) position.

[00100] Releasing or decreasing external pressure on the bulb 60b or retracting the plunger in the syringe 60s can reduce air pressure applied to the actuator assembly 40 which can cause the actuator assembly 40 to move an air inlet closure member 48 to close the air inlets 43 and concurrently extend the actuator member 45 (FIG. 5B).

[00101] The actuator assembly 40 can be configured to operate in the reverse whereby positive air pressure can be increased to move the actuator member 45 to the second position and close the air inlets 43.

[00102] In some embodiments, the device 10 can be configured to have the technician retract the syringe 60s or squeeze/compress the bulb 60b in order to close the flow path 25f at the bag outlet to the flow path 25f and open the air vents 43 once the scan is complete. This can allow the patient to exhale through the output member 30 of an intact device 10 once again after the scan. Also, or alternatively, negative pressure may be controllably applied to

the actuator assembly **10** and used for redundancy at defined times/actions before or after the positive pressure is applied.

[00103] Typically, the technician squeezes the bulb **60b** or extends a plunger the syringe **60s** to administer the dose or actuate the device to close the air inlets **43** and open the flow path **25f** from the bag **20** to the output member **30** when the patient is ready for the breath-hold inhalation of the gas after practice inhalations with room air, all the while the output member **30** is in position on/in the patient.

[00104] The inhalation delivery output member **30** can alternatively be configured as a face mask **30m** (**FIG. 6**), which may be particularly suitable for pediatric use.

[00105] The actuator assembly **40** can be configured to provide linear motion of the actuator member **45** and the air closure member **48** in response to pneumatic input to open the valve **100** and concurrently seal the air inlets **43**. The actuator assembly **40** is configured to allow the patient to inhale room air during practice inhalation procedures using the inhalation delivery output member **30**, then close the air flow path off and open the gas path from the bag **20** to inhale the gas.

[00106] The dose delivery device **10** can be configured to be a compact, MRI-safe device that can administer hyperpolarized gas in a controlled manner. As shown in **FIG. 3**, this device **10** allows for the technologist to remain outside of the bore **200b** of a superconducting magnet **200** during imaging. The dose delivery device **10** is configured so that the inhalation delivery output member **30** can remain in position on/in the patient both when practicing inhalation procedures using room air and during dose administration thereby facilitating imaging repeatability and proper dose inhalation.

[00107] Turning now to **FIGs. 8-13A, 13B**, another embodiment of a dose delivery device **10'** is shown. As shown, the dose delivery device **10'** comprises an actuator assembly **40'** that is configured to combine functions of the actuator assembly **40** and valve **100** described above into a single multi-functional piston **140** inside a piston housing **140h**.

[00108] The piston housing **140h** comprises a piston chamber **240** that encloses the piston **140**. The piston housing **140h** comprises at least one (room) air inlet **43**, shown as a plurality of circumferentially spaced apart and circumferentially extending inlets **43** that are closer to the distal end portion **140d** of the housing **140h** than the proximal end portion **140p** of the housing **140h**.

[00109] The piston housing **140h** has an attachment segment or member (connector) **245** that is directly or indirectly coupled to the connector **22** of the bag **20**. The attachment segment **245** may be located on a proximal end portion **140p** of the piston housing **140h**.

[00110] The piston housing **140h** can have a distal end portion **140d** with a connector **247** that is directly or indirectly coupled to the inhalation delivery output member **30'**. The output member **30'** can be formed to be integral with the connector **247** or even the piston housing **140h**. As shown, the output member **30'** is a mouthpiece **30m**.

[00111] The inhalation delivery output member **30'** can have a single branch **33** that is connected to the connector **247** of the piston housing.

[00112] Referring to **FIG. 8**, the dose delivery device **10'** can have a first tube segment **25₁** that is coupled to the proximal end portion **140p** of the piston housing **140h**. The first tube segment **25₁** can be in-line with the connector **245** and/or axially extending centerline of the piston **140**. The first tube segment **25₁** can receive the connector **245** and couple to the connector **22** of the bag **20**.

[00113] The dose delivery device **10'** can have a second tube segment **25₂** that is coupled to the distal end portion **140d** of the piston housing **140h**. The second tube segment **25₂** can be spaced apart from but in-line with the first tube segment **25₁**. The second tube segment **25₂** receives the connector **247** and the single branch **33** of the inhalation delivery output member **30'**.

[00114] **FIG. 9A** illustrates the piston **140** in a home position, sealed against the proximal end portion **140p** of the piston housing **140h**, exposing the air inlets **43** allowing (room) air flow **25f** between the room and the patient inhalation delivery member **30'**. **FIG. 9B** illustrates the piston **140** in a second operative position, whereby the piston **140** sealably closes (blocks) the air inlets **43** and directs gas flow **25f** from the bag **20** through gas inlets **143** in the piston **140** (**FIG. 10**) to the patient inhalation delivery member **30'**.

[00115] **FIGs. 9A** and **9B** also show the piston housing **140h** and the patient inhalation delivery output member **30'** can be directly attached or integrated into a single monolithic body without requiring a segment of tubing to couple the two features. The branch segment **33'** can have an outer wall that is angled at an angle in a range of 30-60 degree from a centerline axis A-A of the piston **140**, typically about 45 degrees.

[00116] The piston **140** can be configured to move axially a relatively short stroke distance between the first and second positions. The stroke distance **L** can be in a range of about 4-30 mm, more typically a range of about 5-10 mm, such as about 8.5 mm, in some embodiments. This stroke distance of the piston **140** controllably directs either air (**FIG. 9A**) or gas from the bag **20** (**FIG. 9B**) to the patient.

[00117] In the first (home or start) position (**FIG. 9A**), the piston **140** seals the gas from the bag **20** from entering the actuator assembly **40'** while the air inlet(s) **43** are open.

[00118] Referring to **FIG. 10**, a face seal surface **144** can be provided on a distal or proximal end of the piston **140**. The face seal surface **144** can be a closed surface, forming a seal surface, optionally surrounded by a seal **146** such as an O-ring. The face seal surface **144** can be configured to keep the contents of the bag **20** closed off from flow path **25f** prior to the actuator member being actuated, typically by a technician. **FIG. 12** illustrates that no face seal **146** is required on the piston **140**. The seal **146**, whether an O-ring or other suitable seal configuration can be provided in the connector **245** or other mating component of the face seal surface **144** of the actuator assembly **40'** of the device **10'**, rather than on the face **144** of the piston **140**. An example of another configuration of a seal **146** is an extruded and cut seal profile, for example, optionally held by a groove.

[00119] Referring to **FIGs. 10-12**, the gas intake apertures **143** can be circumferentially spaced apart and positioned about the medially located seal surface **144**. The gas intake apertures **143** are configured to allow gas from the bag **20** to flow through the piston **140** and into the inhalation delivery output member **30'** when the piston **140** is in the second (actuated) position (**FIG. 9B**).

[00120] Referring to **FIGs. 9A, 9B, 10** and **12**, that the piston **140** can include first and second concentric body segments **140₁**, **140₂**. The first segment **140₁** can reside closer to the proximal end of the housing **140h** than the second segment **140₂**. The first and second concentric body segments **140₁**, **140₂** can reside in a chamber **240** in the piston housing **140h** that has corresponding first and second concentric body segments **240₁**, **240₂**. The first segment **140₁** of the piston can provide the gas intake apertures **143** and seal surface **144** and can provide an outer diameter seal **147**. The second segment **140₂** of the piston **140** can have a larger outer diameter than the first segment **140₁**. The second segment **140₂** of the piston **140** can define a piston working face segment **140f** and support first and second outer perimeter axially spaced apart seals **148**, **149**. The second segment **240₂** of the chamber **240** of the housing **140h** can provide the air inlets **43**. The second segment **140₂** of the piston **140** can block the air inlets **43** when the piston **140** is in the second position (**FIG. 9B**) with the air inlets between seals **148**, **149**.

[00121] **FIG. 11** illustrates a rear view of the piston **140** shown in **FIG. 10**. The piston housing **140h** can include an internal (annular) cavity or chamber **140a** extending rearward of the gas intake apertures **143** and/or about a length of the second segment **140₂** of the piston **140**. The inner wall **141** of the annular chamber **140a** can bound an axially extending open channel **142**. The gas intake apertures **143** can merge into the open channel **142**. A closed

end **140e** of the annular chamber **140a** can reside radially outward from the open channel **142**.

[00122] Referring to **FIGs. 13A, 13B, 14A, 14B** and **15**, the inhalation (e.g., dose) delivery device **10'** can include an attachment segment/connector **250** coupled to the piston housing **140h** and in fluid communication with a port **150** in an outer wall **140w** of the piston housing **140h** and to the piston working face **140f** (**FIG. 10**) of the piston **140** inside the housing **140h**. The attachment segment/connector **250** can be connected to a length of tubing **50** that is connected to a pressurized fluid source (typically a gas such as air) **60** such as a bulb **60b** or syringe **60s** as discussed above with respect to the embodiment of **FIGs. 2** and **6**. A first end portion **51** of the conduit **50** can include a first connector **1250** and a second end portion **52** of the conduit **50** can include a second connector **1350**. The first connector **1250** can connect to the connector **250** provided by the piston housing **140h**. The second connector **1350** can connect to the user input for the pressurized input for the actuator assembly **40, 40'**. One or more of the connectors **250, 1250** and/or **1350** can be luer-lock connectors.

[00123] As shown, the conduit **50** can have a smaller inner diameter and outer diameter and a longer length than a sum of the first and/or second segments **25₁, 25₂** providing part of the inhalation flow path **25f** between the bag **20** and the inhalation delivery output member **30, 30'**.

[00124] A pinch valve **100p** can be placed externally along the first segment **25₁** between the bag **20** and the piston housing **140h** and used in combination with the actuator assembly **40'** for redundant control of the flow path **25f**.

[00125] The branch **33'** of the inhalation delivery output member **30'** can extend into the second segment **25₂** of the flow path conduit **25** and can be in-line with the axially extending centerline of the piston **140**.

[00126] Referring now to **FIGs. 16-24B**, another embodiment of the dose delivery device **10''** with another example actuator assembly **40''** is shown. In this embodiment, the actuator assembly **40''** comprises a piston **140'** in a piston chamber **247'** in the piston housing **140h'**. The piston chamber **247'** can have a straight linear configuration and the inhalation delivery device **30''** (shown as mouthpiece **30m**) can be in-line with the piston chamber **247'** and the piston housing **140h'**. As shown, the piston housing **140h'** defines a single branch **33** that connects to the inhalation delivery device **30'** and that can enclose the piston **140'**. The piston **140'** can have an open channel **142** and the piston **140'** can travel between first and second operative positions in the piston housing **140h'**.

[00127] Referring to **FIGs. 19A, 22A and 19B, 22B**, the piston **140'** can move in the housing **140h'** between a first (home) position (**FIG. 22A**) to a second position (**FIG. 22B**). The piston **140'** is configured to cooperate with the housing **140h'** to allow (ambient) room air to flow through the piston **140'** to the inhalation gas output member **30'** (and flow the opposite direction to vent) when the piston **140'** is in the first position (**FIGs. 19A, 22A**). The piston **140'** is configured to cooperate with the housing **140h'** to block room air in the second position (**FIGs. 19B, 22B**) while also allowing gas from the bag **20** to flow in the flow path **25f** provided by the housing **140h'** downstream of the piston **140'** to the inhalation gas output member **30'**.

[00128] The housing **140h'** can have an outer wall **140w** with first and second ports **150'**, **245p** extending therethrough. The first and second ports **150'**, **245p** can be provided as parallel projecting segments, connecting to conduits **50, 25**, respectively. The piston housing **140h'** can have a first end portion **140e₁** that is axially spaced apart from a second end portion **140e₂**. The second end portion **140e₂** faces the output device **30''**, e.g., mouthpiece **30m**. The first end portion **140e₁** intakes air and vents to atmosphere. The first end portion **140e₂** can include or be coupled to an end cap **2000**.

[00129] The second end portion **140e₂** can be coupled to the inhalation delivery output device **30''** via connector or adapter member **247** (**FIG. 18B**) that can attach the piston housing **140h** and the mouthpiece **30m**. The connector or adapter member **247** can be integral to the piston housing **140h**, the mouthpiece **30m** or provided as a separate connecting member.

[00130] The first port **150'** can be an actuator input port **150'** in fluid communication with the piston **140'**. As shown, the first port **150'** is located further away from the gas inhalation output member **30''** than the conduit **25** attached to the bag **20**. In operation, pressurized input forces the piston **140'** to move toward the first end portion **140e₁** of the housing **140h'** which closes air intake ports at the first end portion **140e₁** of the housing **140h** and concurrently opens the port **245'** to the conduit **25** attached to the bag **20** (**FIG. 16**).

[00131] Referring to **FIGs. 21, 22A, 22B, 23, 24A and 24B**, the piston **140'** can have a plurality of circumferentially extending, axially spaced apart, seals **147, 148, 149**. The seals **147, 148, 149** can be provided as elastomeric outer wall segments formed/injection molded/3-D printed/overmolded onto/into the wall **140w** or body of the piston **140'**. The seals **147, 148, 149** may alternatively be provided as separate seal members such as O-rings or gaskets.

[00132] Referring again to **FIG. 22A**, the housing **140h'** can have a flat surface and/or ledge **145** that defines a seating surface for the piston **140'** when the piston **140'** is in the first position that blocks the port **245p**.

[00133] The piston **140'** can have first and second longitudinally extending segments **140₁**, **140₂**, each with different outer diameters. The first segment **140₁** can have a greater outer diameter than the second segment **140₂**. The flat surface **140f** can define a step between the first and second segments **140₁**, **140₂**. The first segment **140₁** can reside further away from the inhalation delivery output member **30'** than the second segment **140₂** and can have a length that is less than 50% of the length of the second segment **140₂**.

[00134] At least two of the seals, shown as first and second seals **147**, **148**, can be axially (longitudinally) spaced apart and extend circumferentially about the outer wall of the piston **140'**. With the piston **140'** in the first position (**FIG. 22A**) one seal **148** resides on one side of the port **245p** and the other seal **147** resides on the other side to thereby seal off the port **245p** from the flow path **25f**.

[00135] The piston **140'** can include at least one additional seal, shown as a third seal **149**, that also extends circumferentially about the outer wall of the piston **140'**, at a location closer to the first end **140e₁** of the housing **140h**. The seal **149** can reside on the first segment **140₁**.

[00136] The piston **140'** can have a flat circumferentially extending working surface **140f** that projects radially outward and cooperates with an internal flat surface **145** of the housing **140h** when the piston **140'** is in the first position (**FIG. 22A**).

[00137] Referring to **FIGs. 22A, 22B, 24A, 24B**, the piston **140'** can have longitudinally extending legs **1149** that extend a sub-distance of the overall length of the piston **140'** to define a stop position against the ledge **145** for the piston **140'** in the piston chamber **240'**. The legs **1149** can also provide structural rigidity to the piston **140'**.

[00138] The top of the piston **140'** can also include an annular surface **1144** that resides in front of the legs **1149** and circumferentially extends about the opening for the channel **142**.

[00139] Still referring to **FIGs. 24A, 24B**, the piston **140'** can have an open medial through channel **142**. The first end **1140e₁** of the piston **140** can have a surface with a seal **146** that surrounds an outer diameter of the open channel **142** and projects outward from a seal face **1144**. The first end **1140e₁** can also provide the seal **149**. The seal **149** can extend circumferentially about the outer wall of the piston **140'**. The seal **149** can reside in front of the legs **1149**. The second end **1140e₂** can provide the circumferentially extending seal **147**.

[00140] The seal **146** can seal against a cap **2000** providing a seal surface **2144** that faces the seal **146** and abuts the seal **146** when the piston **140'** is in the second position (FIGs. **19B**, **22B**). The cap **2000** also comprises at least one air intake/outlet aperture **2143** that allows air to enter and exit from the channel **142** of the piston **140'** when the piston **140'** is in the first position (FIGs. **19A**, **22A**). The gas from the bag **20** can flow through the piston housing **140h'** in the flow path **25f**, downstream of the piston **140'**, when the piston **140'** is in the second position (FIGs. **19B**, **22B**).

[00141] FIGs. **25A-25C** illustrate a series of actions that can be used to dispense the gas from the bag **20** when the patient is in a bore **200b** of a scanner **200** according to embodiments of the present invention.

[00142] FIGs. **25A-25C** also illustrate the bag **20** can be at least partially supported by a bag holder **2500** to reduce any torque that may be applied to the mouthpiece **30m** by the torque arm that may be generated by the conduit **25** and bag connector **22**, for example. The bag holder **2500** is sized and configured to be able to move with the scanner bed without contacting the wall of the bore of the magnet.

[00143] The bag holder **2500** can be non-ferromagnetic and may have a pair of arms **2501** spaced apart to define a support space **2502** that receives a bottom portion of the bag **20**. The bag holder **2500** can be configured to hold at least part of the bag **20** a distance above a table or bed of a scanner when the inhalation delivery output member is inserted into a patient to thereby reduce or remove any torque arm generated onto the inhalation delivery output member to reduce any retention force needed to be applied by the patient to retain the inhalation delivery output member in a mouth of the patient.

[00144] A clinician/technician can attach the length of tubing **50** and pressurized fluid source /syringe and then actuate the piston **140**, **140'** once the patient is in position, e.g., within the MRI bore **200b** and a patient has completed the preparatory breathing procedure using room air. The same clinician/technician can also initiate an MRI scan for obtaining MRI signal data of the patient using the inhaled gas such as image data and/or spectroscopic data of cardiac and/or lung function.

[00145] Where the device **10**, **10'**, **10''** is used to dispense hyperpolarized noble gas, the material(s)/components in communication with the gas should be medical grade and formulated to not negatively impact polarization decay and can also be non-ferromagnetic for MRI-compatibility.

[00146] The dose delivery device **10**, **10'**, **10''** can be a manually operated pneumatic control that is open loop and vents to atmosphere.

[00147] FIG. 26 is a flow chart of example actions that can be used to deliver an inhalation dose of a gas to a patient during an imaging procedure according to embodiments of the present invention. Inhalable gas is provided in a bag (block 300). An actuator assembly comprising an inhalation delivery output member is attached or attachable to the bag (block 310). The inhalation delivery output member is placed on/in a patient (block 315). The patient is directed to take practice inhalation breaths of room air with the inhalation delivery output member on/in position for a subsequent inhalation of a gas from the bag for a breath hold delivery (block 320). The actuation assembly is actuated to cause a piston thereof to move from a first position to a second position to close air inlets and provide an inhalation flow path for gas from the bag to the patient using the inhalation delivery output member (block 325).

[00148] The actuation assembly can comprise a linear actuator that is configured to have a short stroke distance that concurrently opens gas inlets to release the gas from the bag and closes air inlets to block room air from flowing to the patient (block 312).

[00149] The actuator assembly can be connected to a length of tubing typically in a range of 1-12 feet or 1-10 feet, such as in a range of 2-10 feet, 2-8 feet or 2-6 feet, for example, that is connected to a pressurized gas source whereby a user provides gas or pneumatic control to actuate the actuator assembly (block 314).

[00150] The gas can be HP gas and the actuating can be carried out manually while the patient is in a bore of a magnet of an MRI scanner with a technician residing in the scanner room with the magnet but outside the bore a distance of 1-10 feet (optionally 2-8 feet, such as 2-6 feet) to pneumatically control the actuation (block 327).

[00151] In some embodiments of the present invention have been illustrated herein by way of example. Many variations and modifications can be made to the embodiments without substantially departing from the principles of the present invention. All such variations and modifications are intended to be included herein within the scope of the present invention, as set forth in the following claims.

THAT WHICH IS CLAIMED:

1. An inhalation gas delivery device, comprising:
an inhalation delivery output member;
a bag of gas in fluid configured for inhalation in fluid communication with the inhalation delivery output member; and
an actuator assembly comprising an actuator member coupled to the inhalation delivery output member, wherein the actuator member has a first position which allows room air to flow along a first flow path to the inhalation gas output member, and wherein the actuator member has a second position which allows gas from the bag to flow along a second enclosed flow path to the inhalation gas output member thereby blocking air from entering the second enclosed flow path.
2. The inhalation delivery device of Claim 1, further comprising a conduit in fluid communication with the actuator assembly and a pressurized gas source whereby a user pneumatically actuates the actuator member, via the conduit, to move from the first position to the second position.
3. The inhalation gas delivery device of Claim 1, wherein the inhalation gas delivery device is non-ferromagnetic and configured for use in an MRI scanner room.
4. The inhalation gas delivery device of Claim 1, wherein the inhalation gas delivery device is configured to vent expiration breaths of inhaled air and inhaled gas to atmosphere.
5. The inhalation gas delivery device of Claim 1, wherein the actuator member comprises a piston that travels a stroke distance in a range of 3 mm and 30 mm between the first and second positions.
6. The inhalation gas delivery device of Claim 5, wherein the stroke distance is in a range of about 5 mm and about 10 mm.
7. The inhalation gas delivery device of Claim 5, wherein the actuator assembly comprises a housing that encloses at least part of the piston, wherein the housing comprises at

least one air inlet, and wherein the actuator assembly closes the at least one air inlet when the actuator member is in the second position.

8. The inhalation gas delivery device of Claim 1, further an air vent closure member that is coupled to the actuator member, wherein the air vent closure member slides linearly in concert with the actuator member as the actuator member moves from the first position to the second position.

9. The inhalation gas delivery device of Claim 1, wherein the gas in the bag comprises hyperpolarized noble gas, and wherein the inhalation gas delivery device is non-ferromagnetic.

10. The inhalation gas delivery device of Claim 7, wherein the hyperpolarized noble gas is ^{129}Xe .

11. The inhalation gas delivery device of Claim 1, wherein the bag and the actuator assembly reside a distance in a range of about 0.1 inches (2.54 mm)-12 inches (30.4 cm) from the inhalation delivery output member.

12. The inhalation gas delivery device of Claim 1, wherein the actuator assembly comprises a housing with an internal chamber, wherein the housing comprises an outer wall with at least one fluid port, wherein the actuator member is a piston in the internal chamber of the housing, wherein the piston comprises a first segment having a first outer diameter and a second segment having a second outer diameter in the internal chamber of the housing, wherein the piston comprises an open channel extending therethrough, wherein the piston is configured to cooperate with the housing to (i) allow room air to flow through the piston to the inhalation gas output member when the piston is in the first position and (2) block room air while also allowing gas from the bag to flow to the inhalation gas output member when the piston is in the second position.

13. The inhalation gas delivery device of Claim 12, wherein the second segment comprises first and second seals axially spaced apart and extending circumferentially thereabout, wherein the first segment comprises at least one seal extending circumferentially thereabout.

14. The inhalation gas delivery device of Claim 12, further comprising a conduit attached to the bag and to the housing, wherein the at least one fluid port comprises an actuator input port in fluid communication with the piston.

15. The inhalation gas delivery device of Claim 12, further comprising a length of conduit coupled to the housing and in fluid communication with a pressurized fluid source, wherein the length of conduit cooperates with the housing to direct pressurized fluid from the fluid source toward a working surface of the piston whereby pressurized fluid input into the housing from the conduit actuates the piston to move to the second position.

16. The inhalation delivery device of Claim 1, wherein the actuator assembly comprises a housing, wherein the housing comprises an outer wall with first and second fluid ports, the first fluid port in fluid communication with the bag via a length of conduit and the second fluid port in fluid communication with a pressurized fluid source configured to actuate the actuator member to move to the second position.

17. The inhalation delivery device of Claim 1, wherein the actuator assembly comprises a piston as the actuator member inside an internal chamber of a piston housing, wherein the piston seals air inlets of the inhalation delivery device in the second position and the piston seals an inhalation gas inlet of the inhalation delivery device when the piston is in the first position.

18. The inhalation delivery device of Claim 1, further comprising a pressurized fluid source comprising a syringe coupled to a length of conduit and to the actuator assembly or a compressible bulb coupled to a length of conduit and to the actuator assembly.

19. The inhalation delivery device of Claim 1, wherein the inhalation delivery output member comprises a single branch that serially defines part of the first flow path and part of the second flow path.

20. The inhalation delivery device of Claim 1, wherein the inhalation delivery output member comprises a first branch that defines part of the first flow path and a separate second branch that defines part of the second flow path.

21. The inhalation delivery device of Claim 1, wherein the actuator member comprises a piston with a plurality of longitudinally spaced apart seals that extend circumferentially about the piston, and wherein the actuator assembly is configured to allow air to flow into and/or out of the first enclosed flow path when the piston is in the first position and is configured to allow only gas from the bag to flow into the second enclosed flow path when the piston is in the second position.

22. The inhalation delivery device of Claim 1, further comprising a bag holder configured to hold at least part of the bag a distance above a table or bed of a scanner when the inhalation delivery output member is inserted into a patient to thereby reduce or remove any torque arm generated onto the inhalation delivery output member to reduce any retention force needed to be applied by the patient to retain the inhalation delivery output member in a mouth of the patient.

23. A method of providing inhalable gas for a medical procedure, comprising:
providing a bag of inhalable gas;
providing an inhalation delivery output member such as a face mask or mouthpiece;

connecting an actuator assembly to the bag and to the inhalation delivery output member, wherein the actuator assembly and the bag reside within 0.1-12 inches (2.54 mm-30.48 cm) from a face of the patient;

placing the inhalation delivery output member on a face over a nose and mouth or in a mouth of a patient;

directing the patient to inhale practice room air breaths with the inhalation delivery output member on the face or in the mouth while an actuator member of the actuator assembly is in a first position providing open air inlets; and then

actuating the actuating assembly to move the actuator member to a second position to close the air inlets and open gas intake inlets to provide a flow path that directs gas from the bag of inhalable gas to flow to the inhalation delivery output member for inhalation by the patient.

24. The method of Claim 23, wherein the medical procedure is an MRI imaging session, wherein the actuator assembly is manually actuated via a pressurized

fluid source in communication with the actuator assembly via a conduit that has a length of 1-10 feet, and wherein the inhalable gas comprises hyperpolarized ^{129}Xe .

25. The method of Claim 23, further comprising placing the bag of inhalable gas into a bag holder.

26. The method of Claim 25, wherein the bag holder is non-ferromagnetic.

1/37

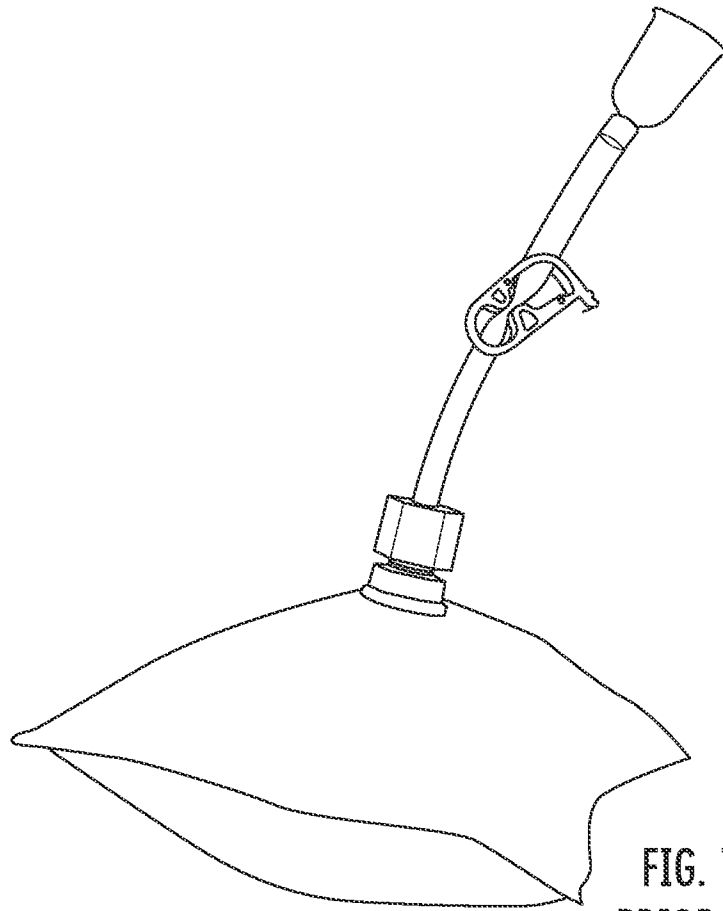


FIG. 1A
PRIOR ART

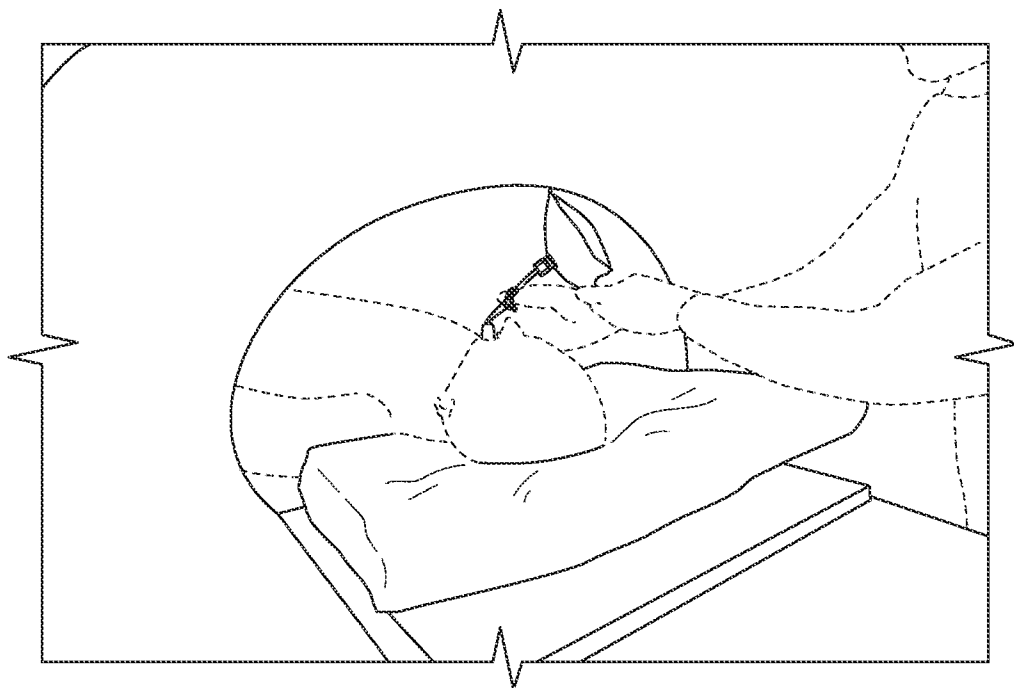


FIG. 1B
PRIOR ART

2/37

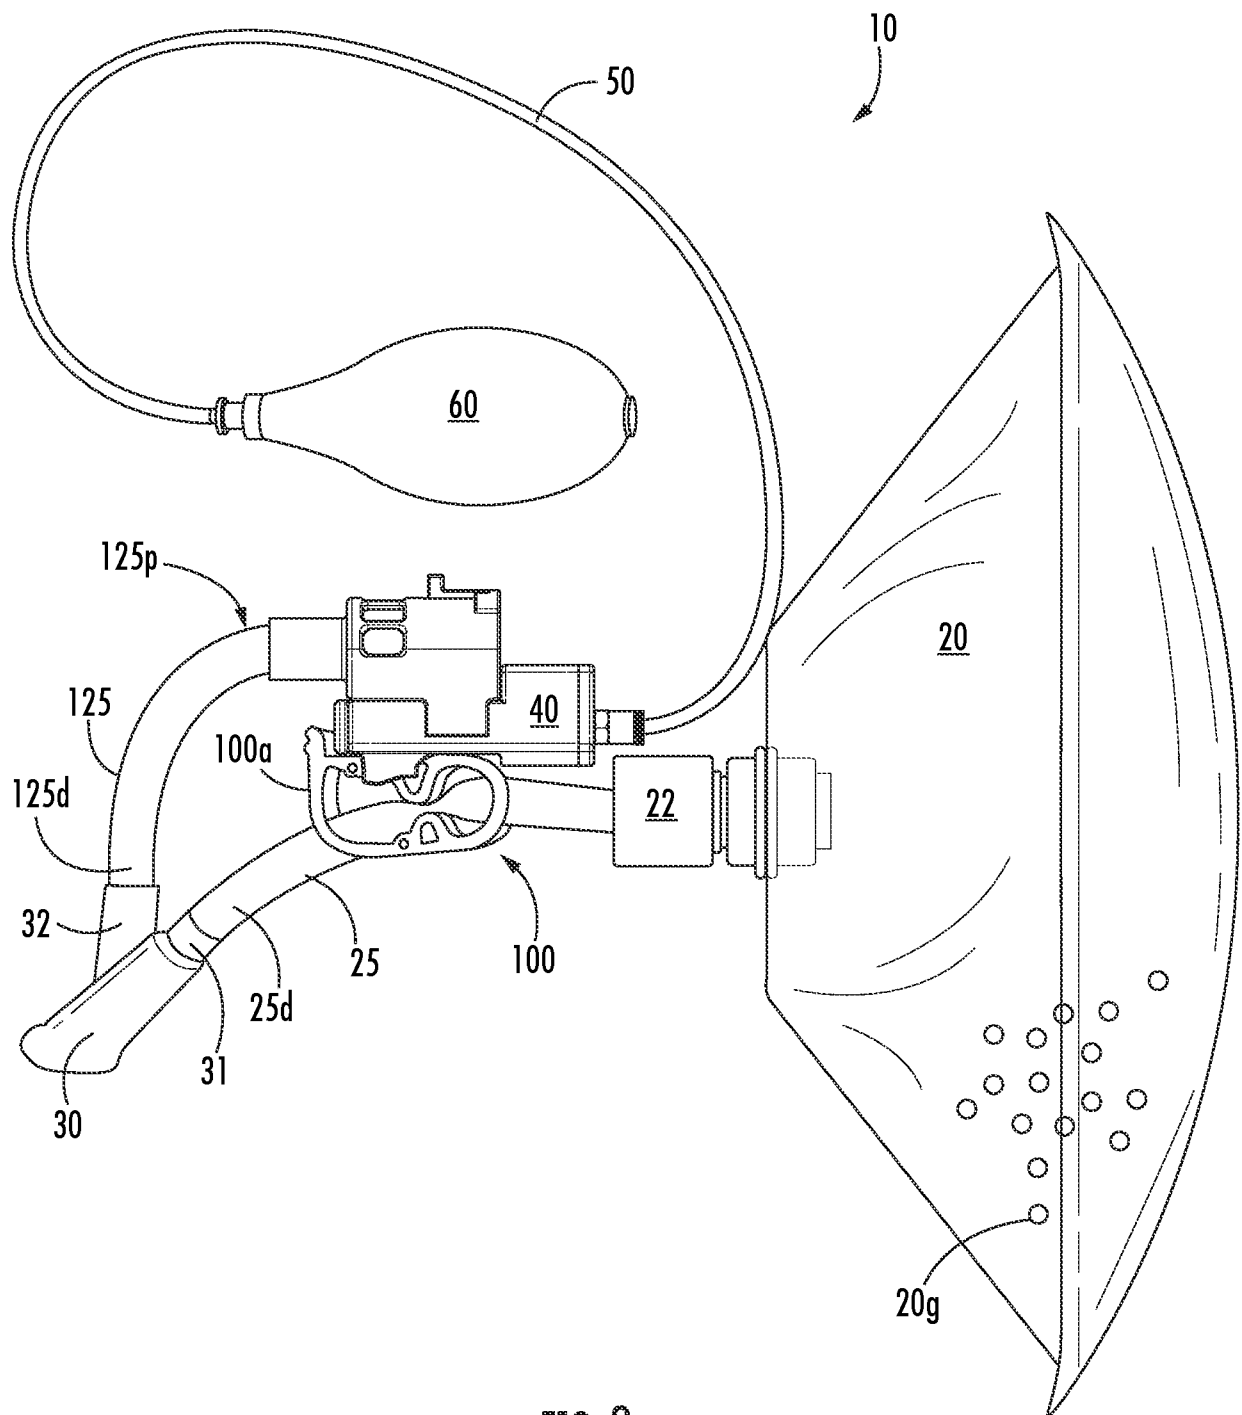


FIG. 2

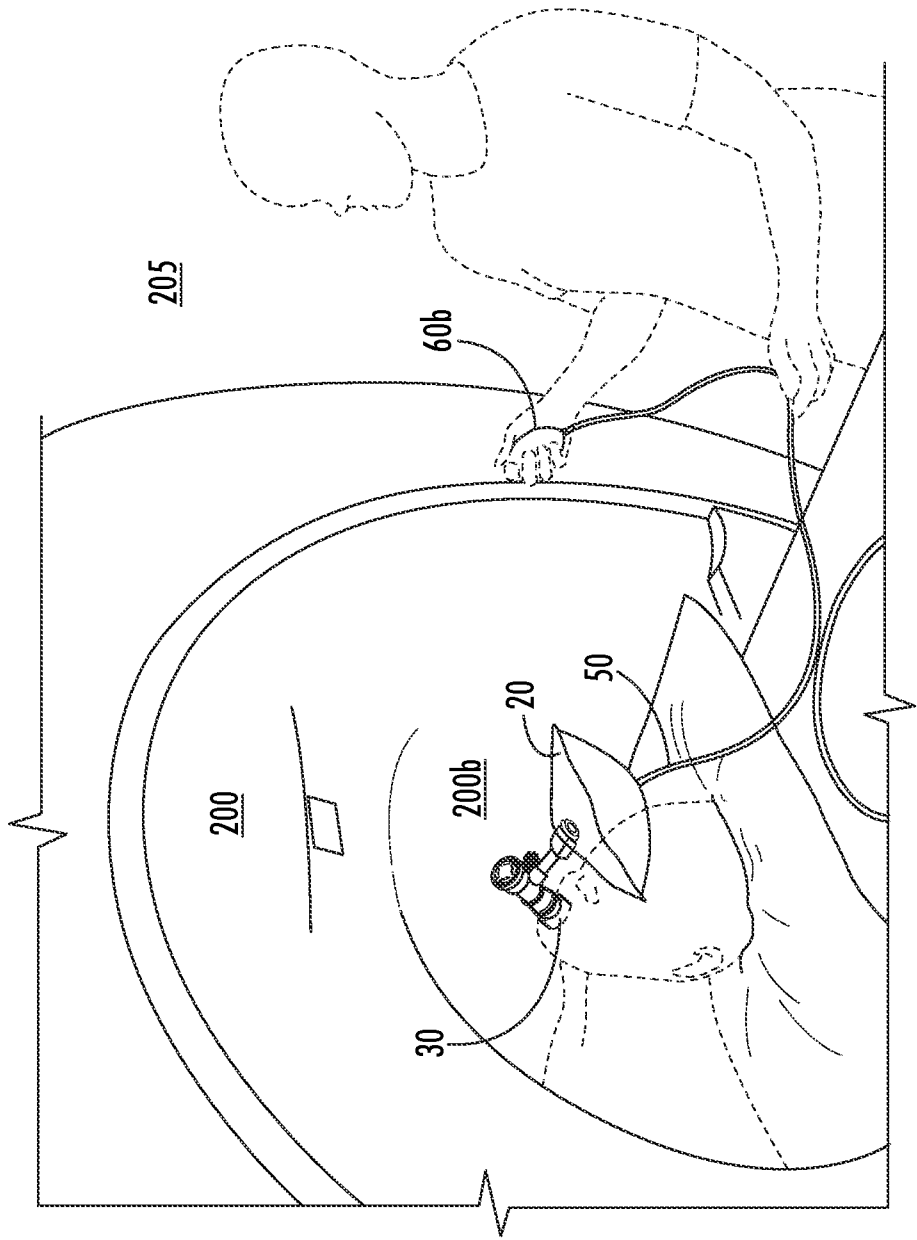


FIG. 4

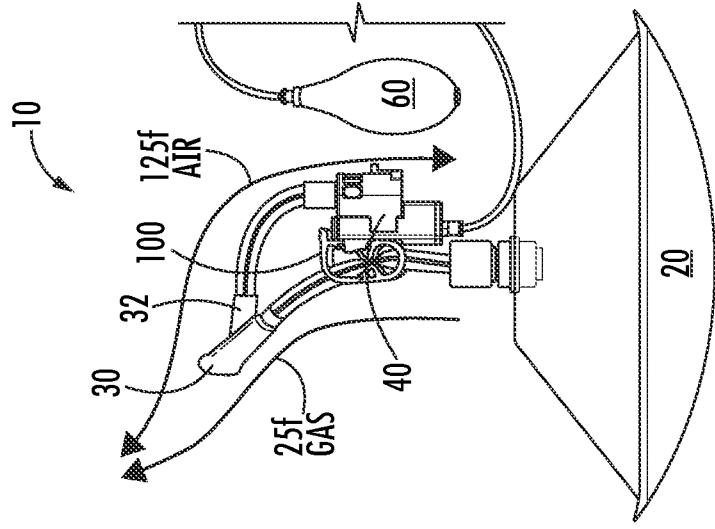


FIG. 3

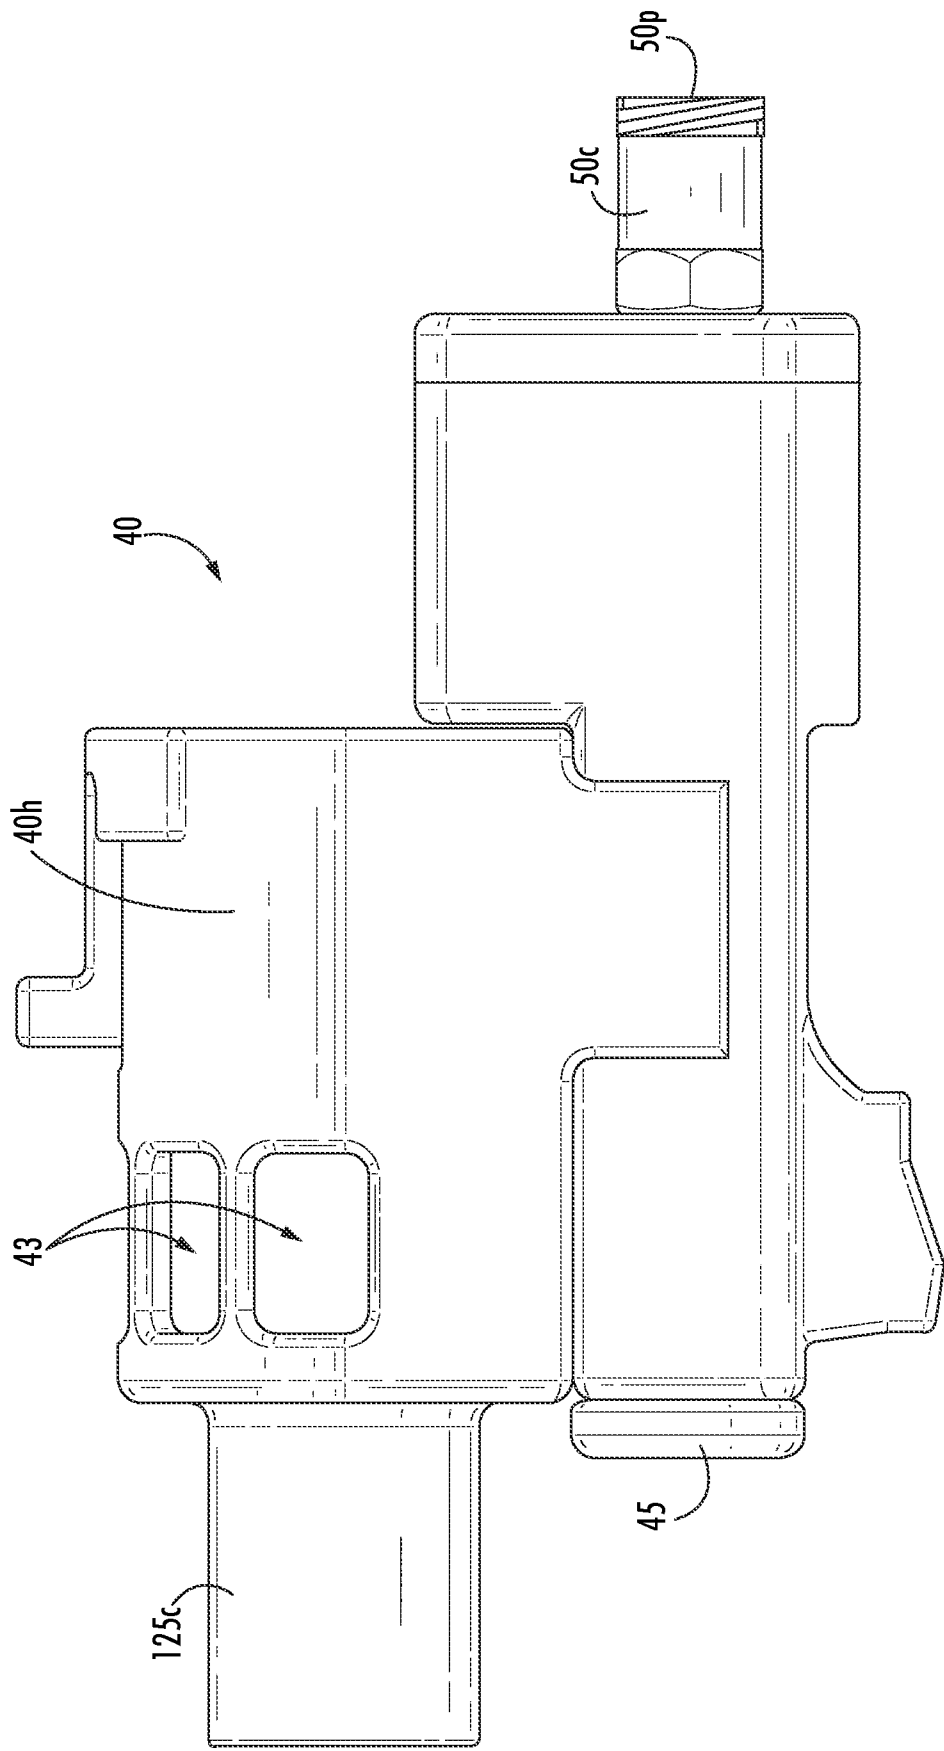


FIG. 5A

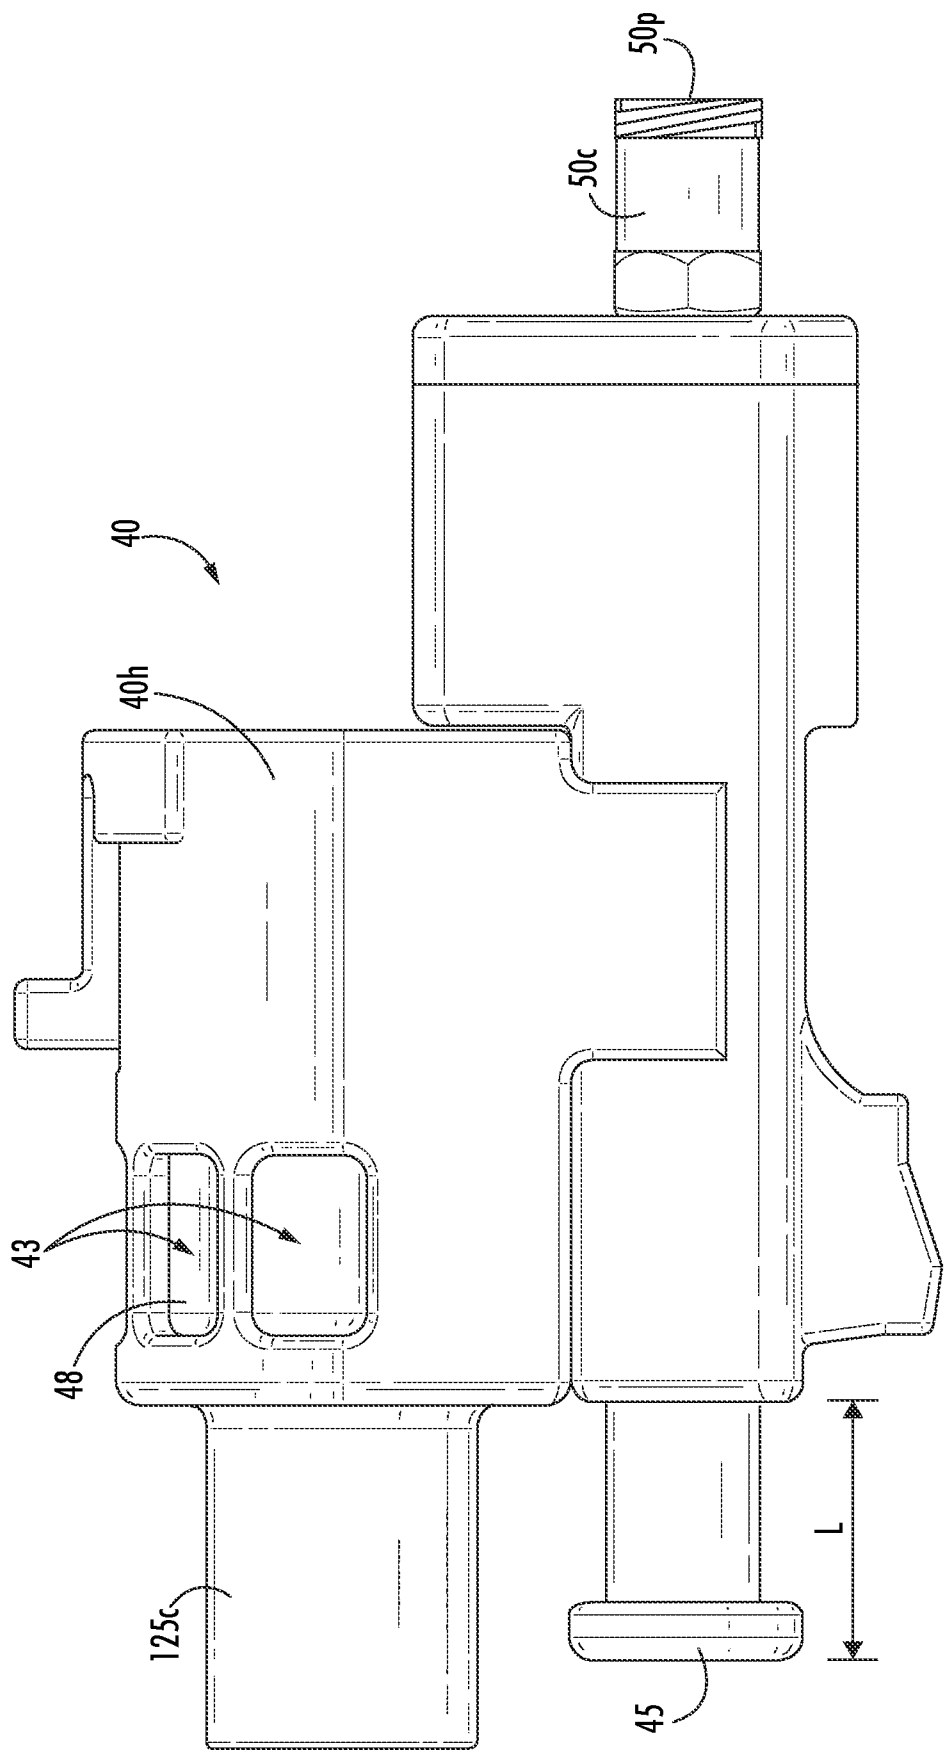


FIG. 5B

6/37



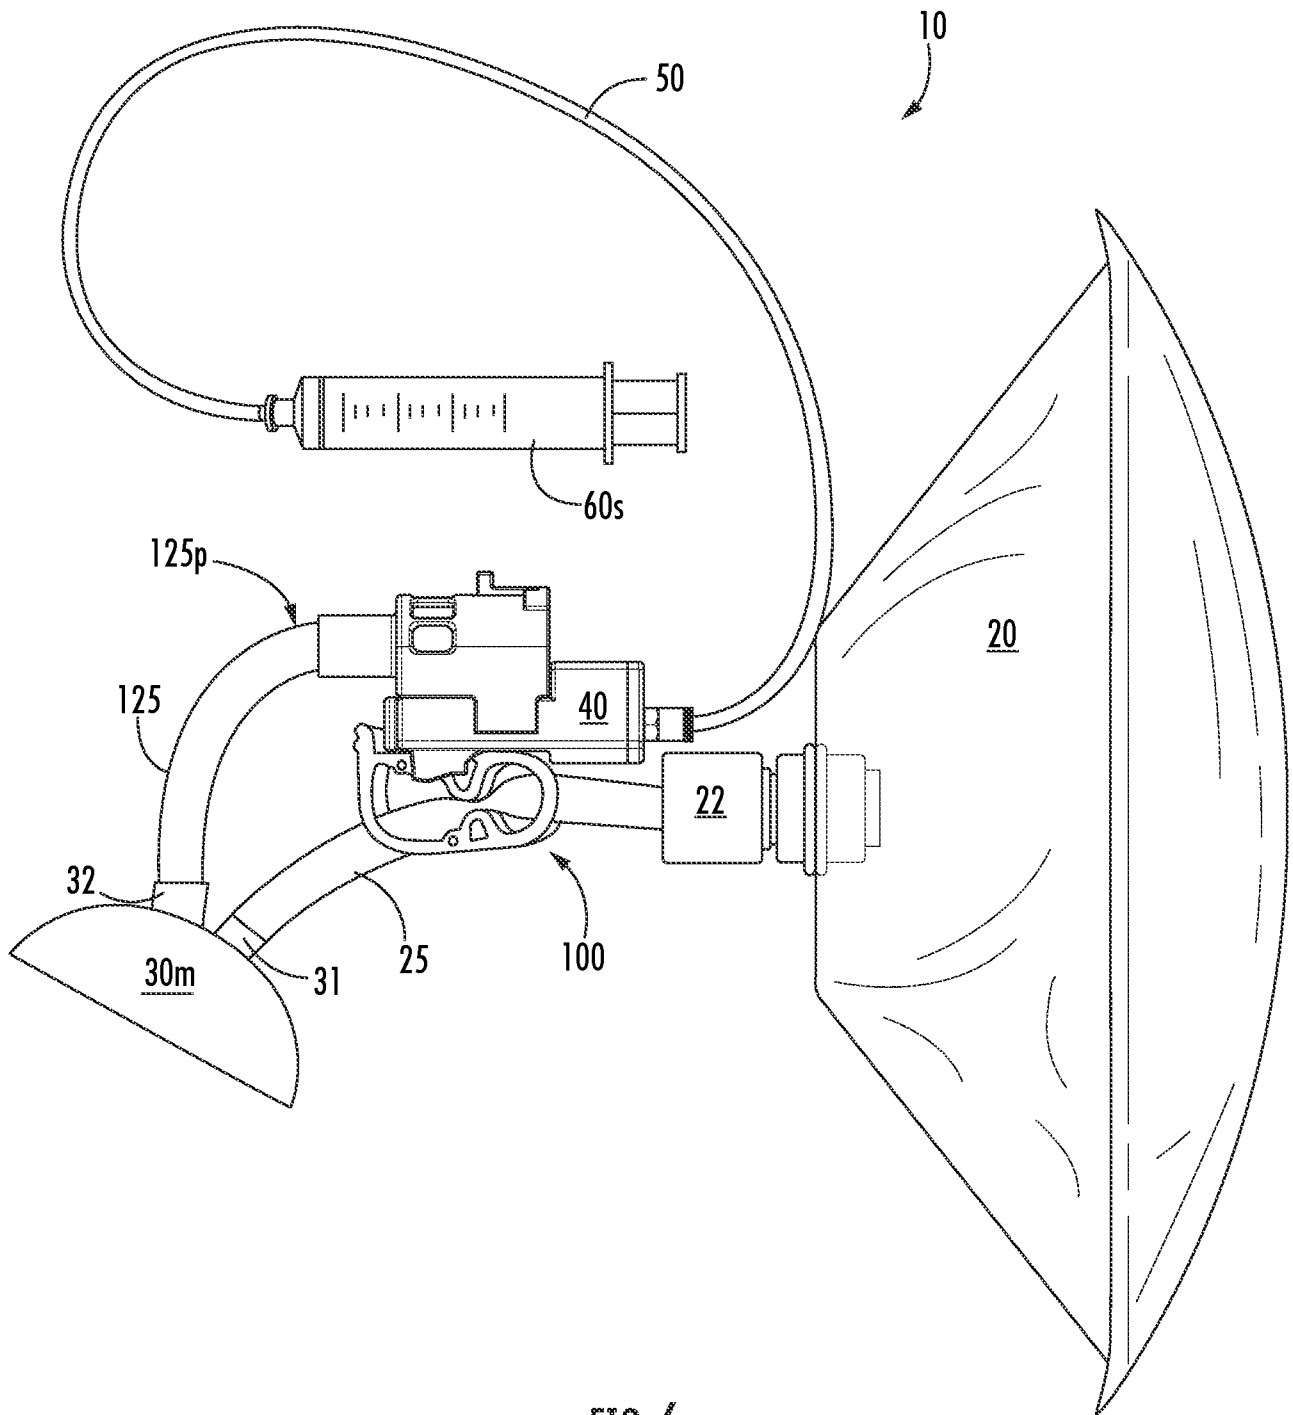


FIG. 6

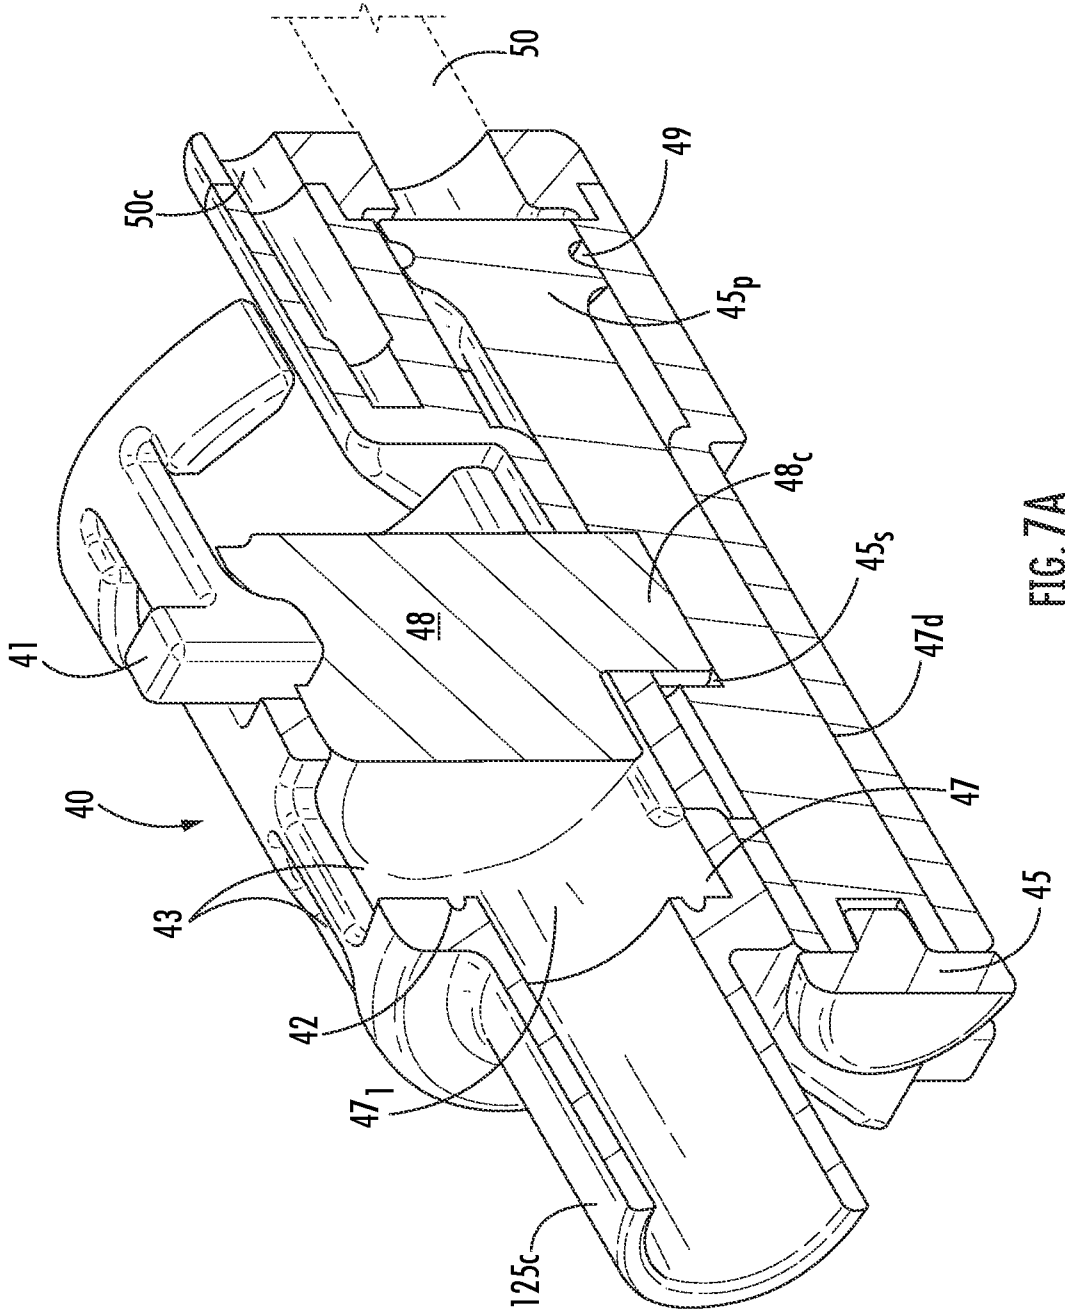

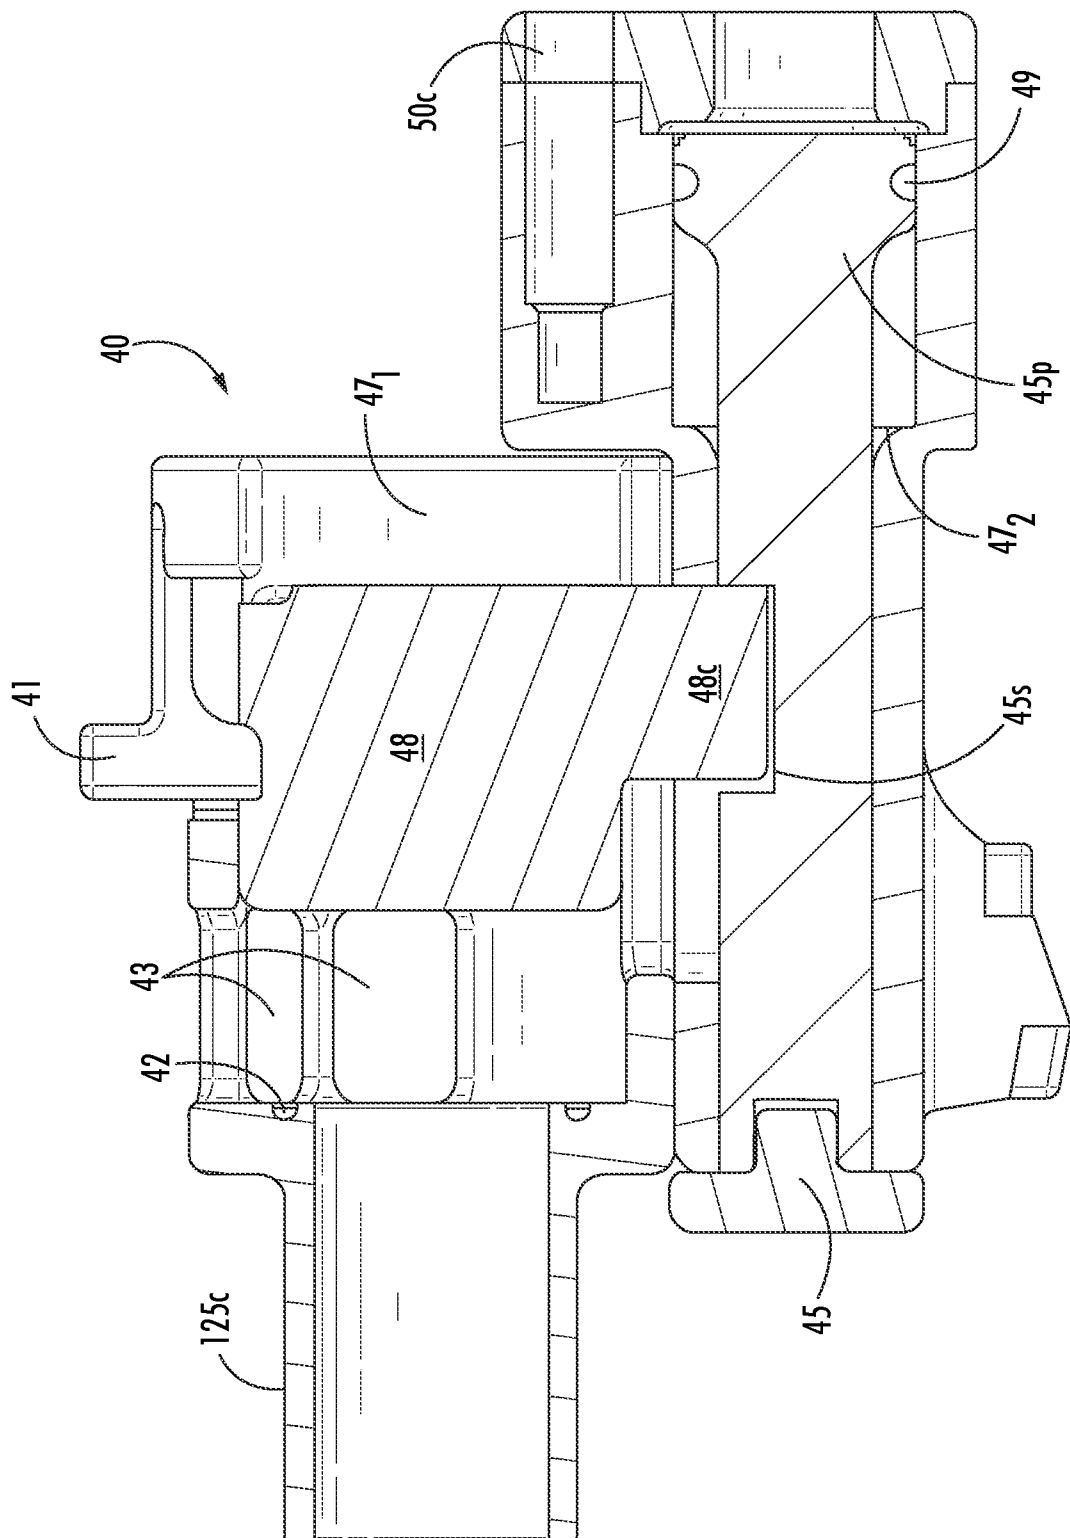

3764

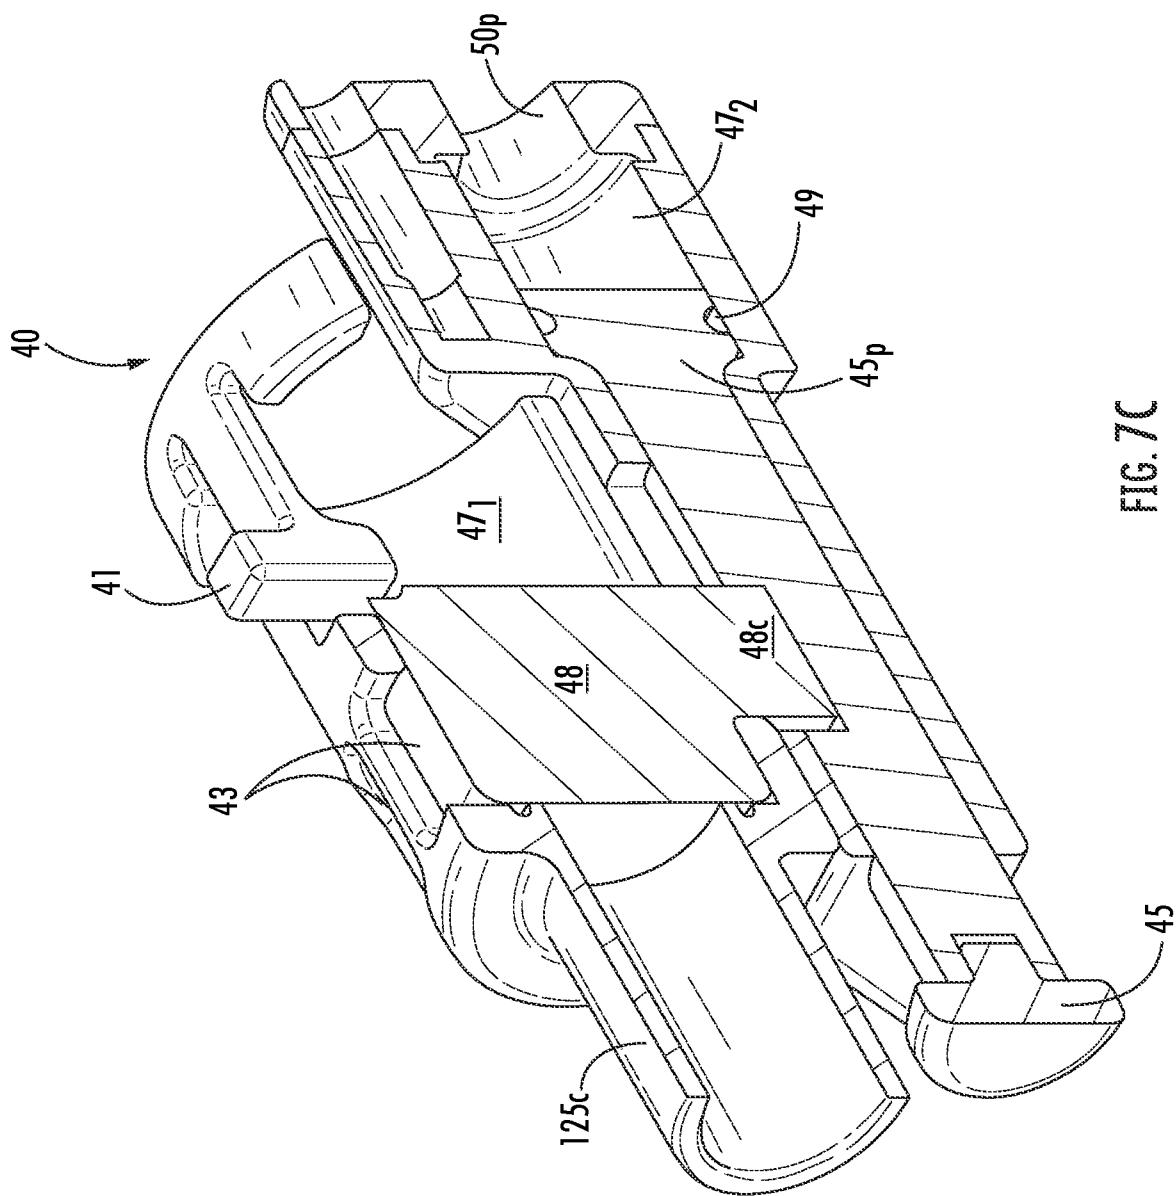


FIG. 7C

10/37

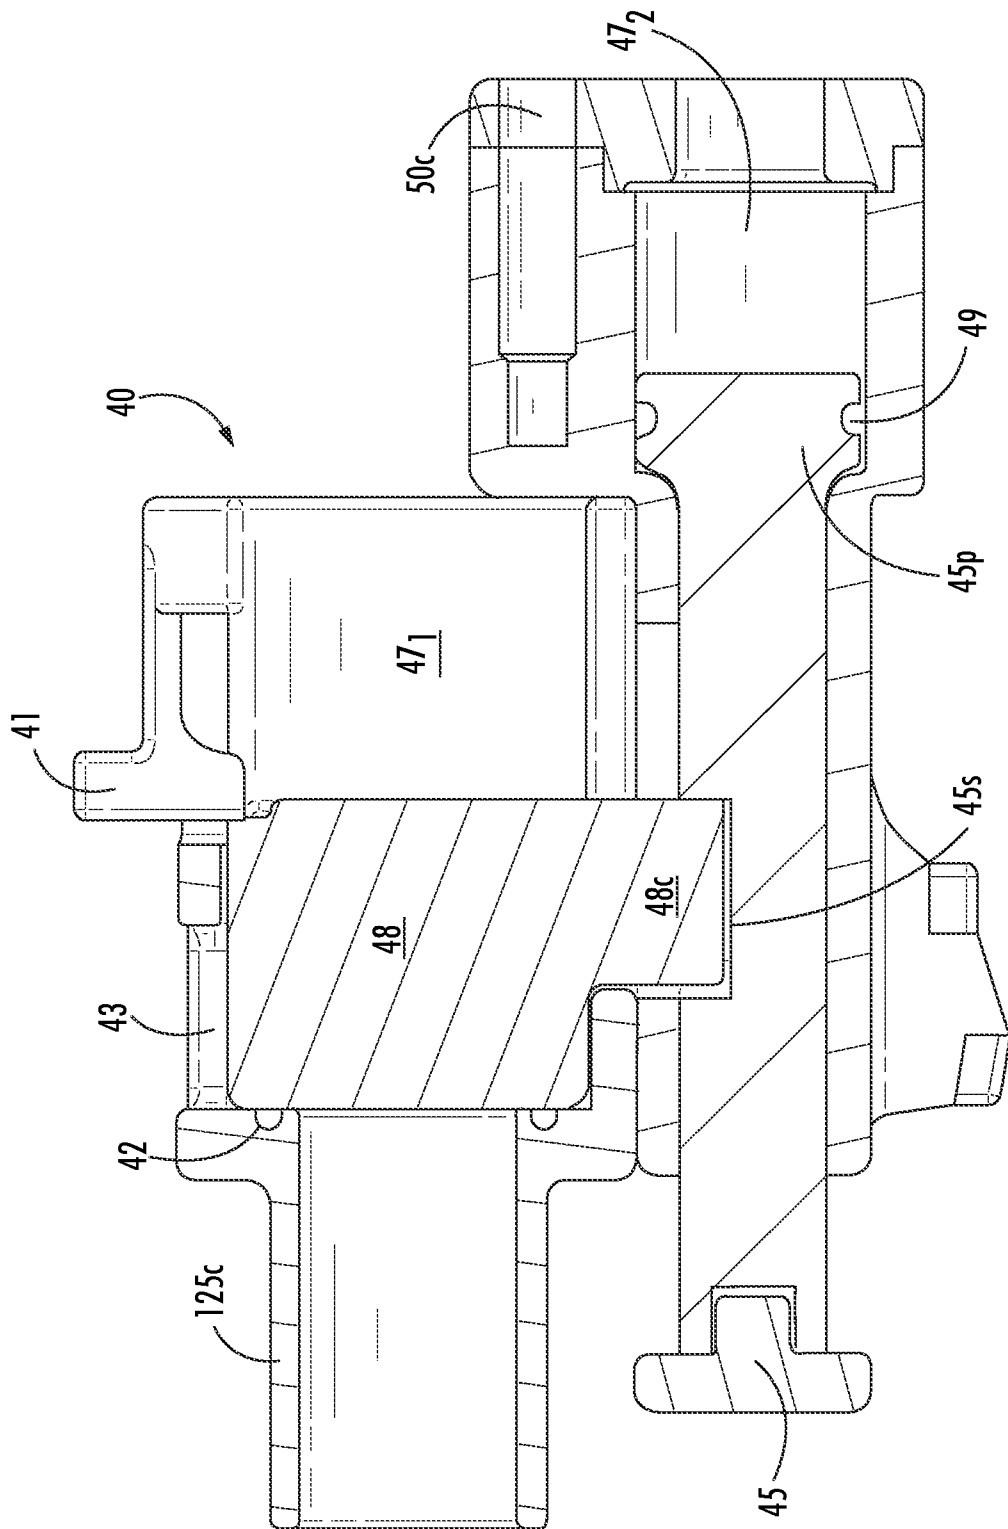


Fig. 7

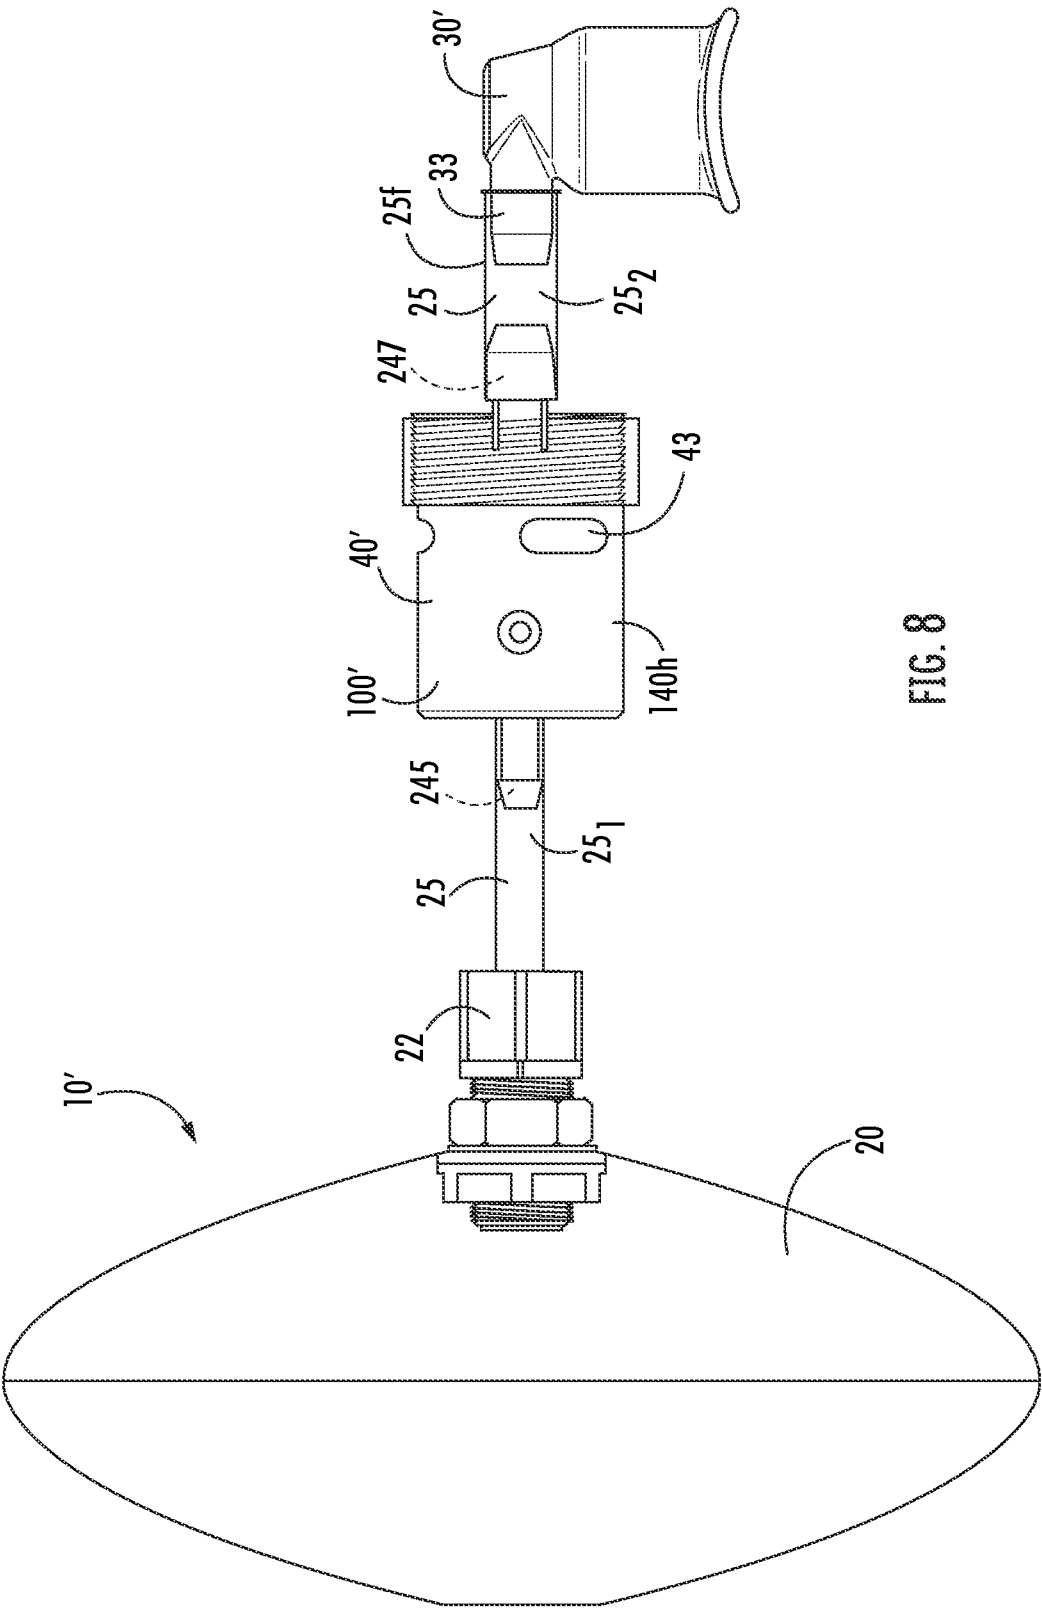


FIG. 8

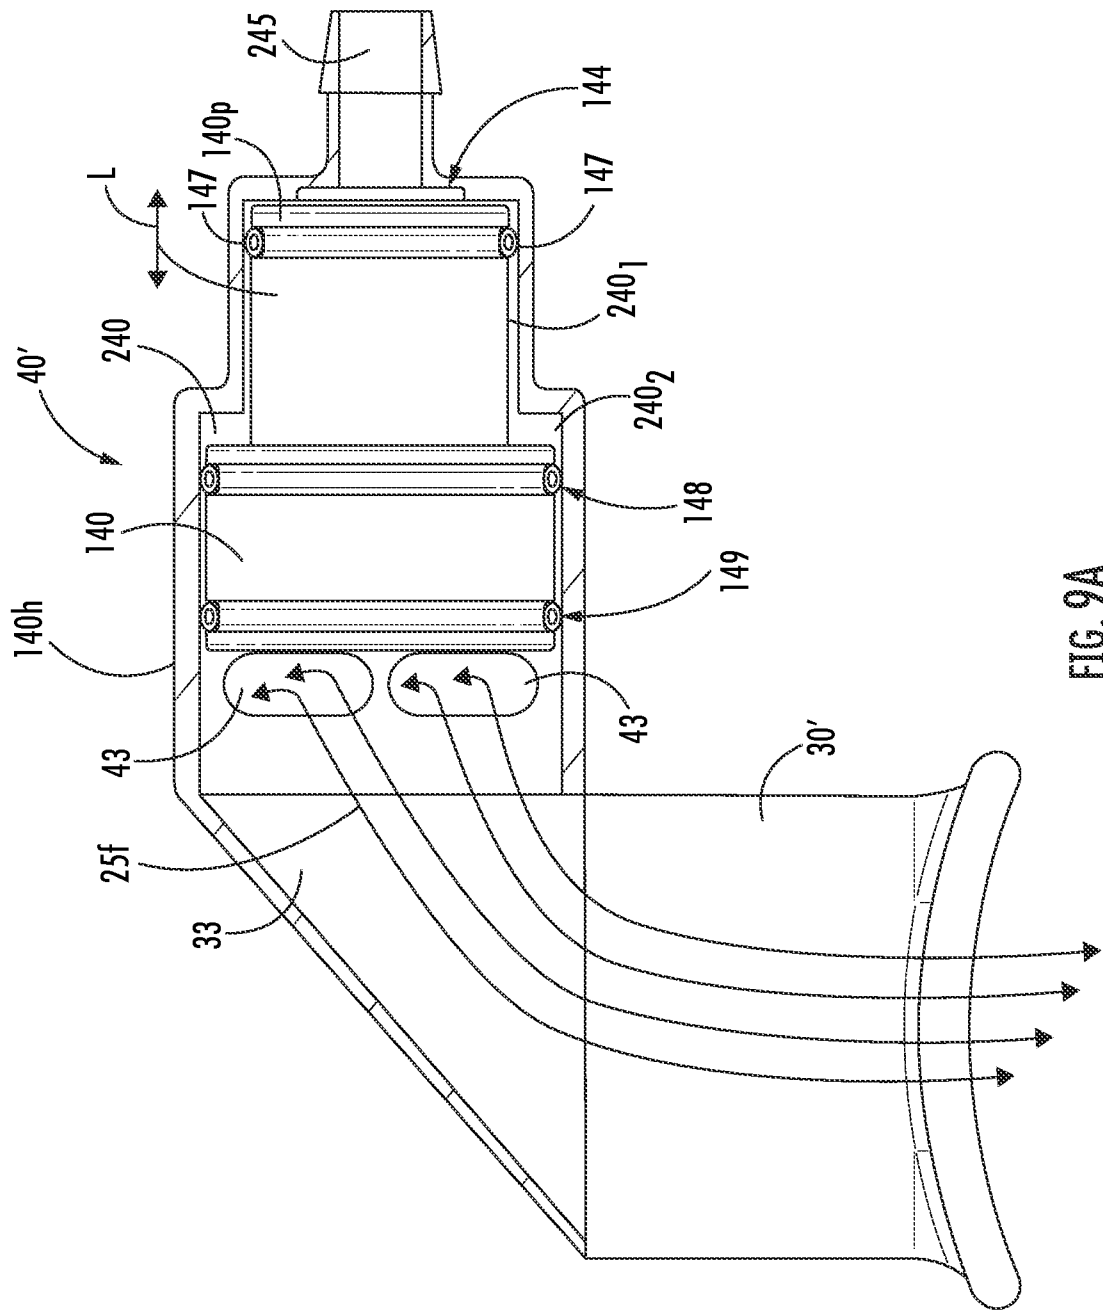


FIG. 9A

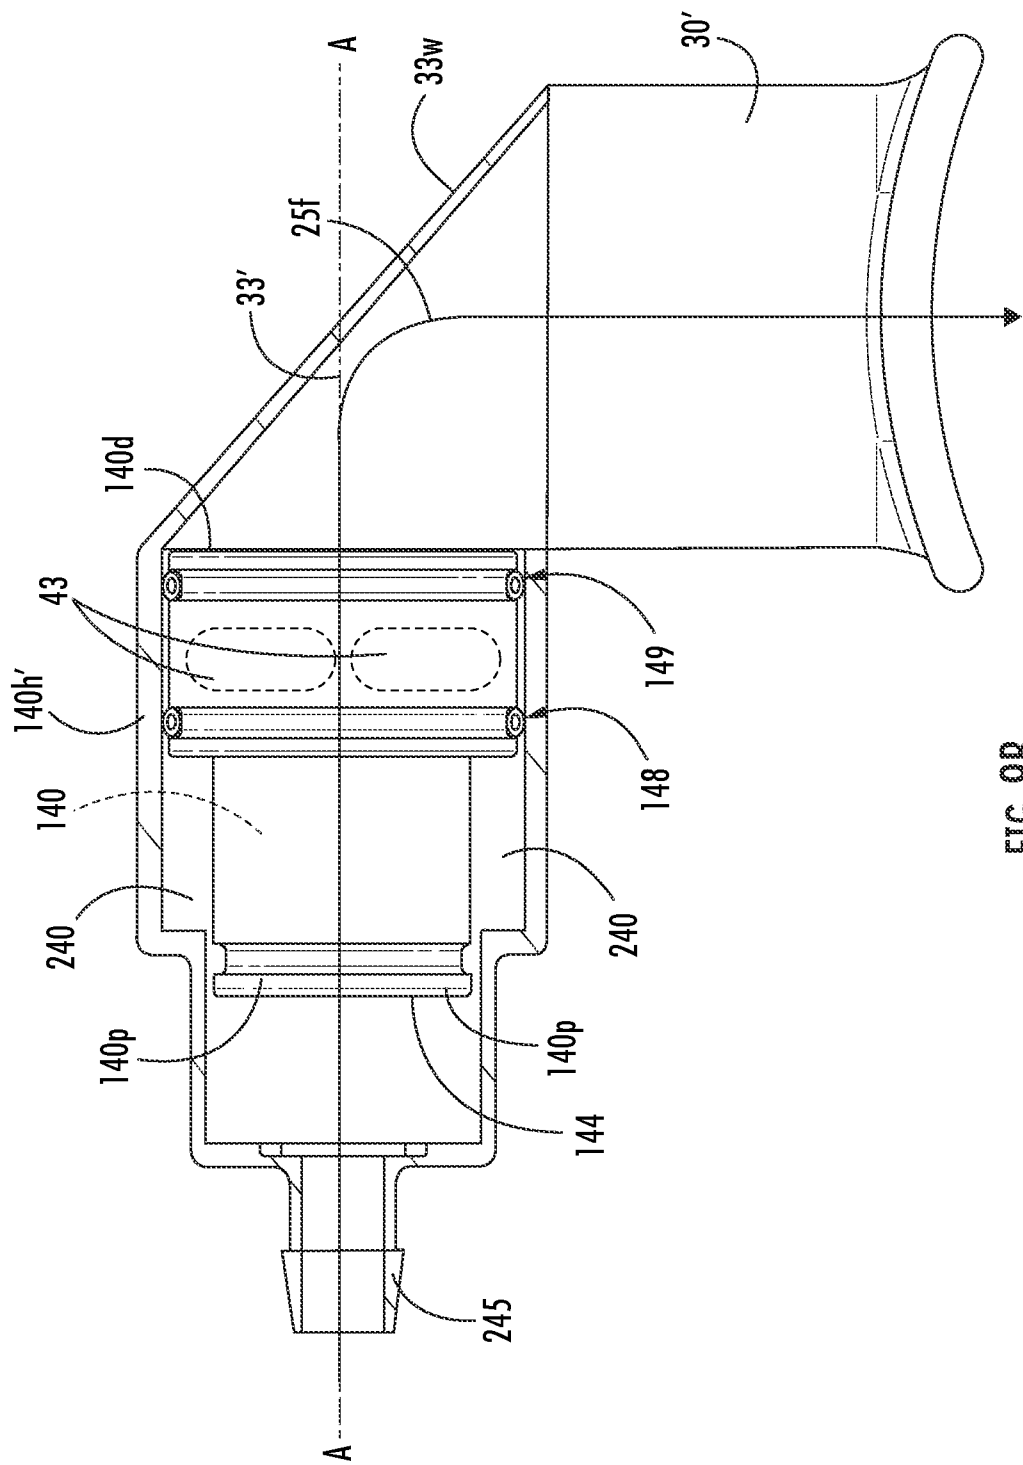


FIG. 9B

14/37

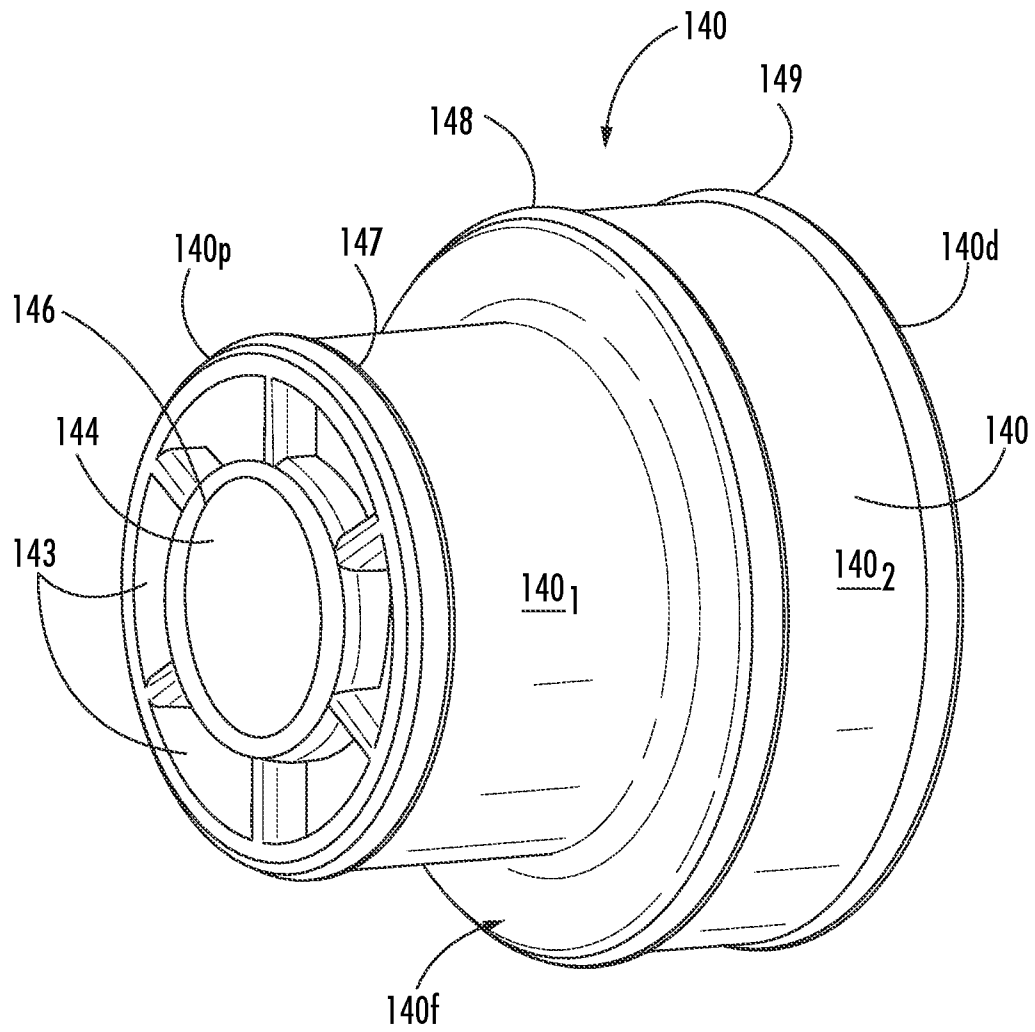


FIG. 10


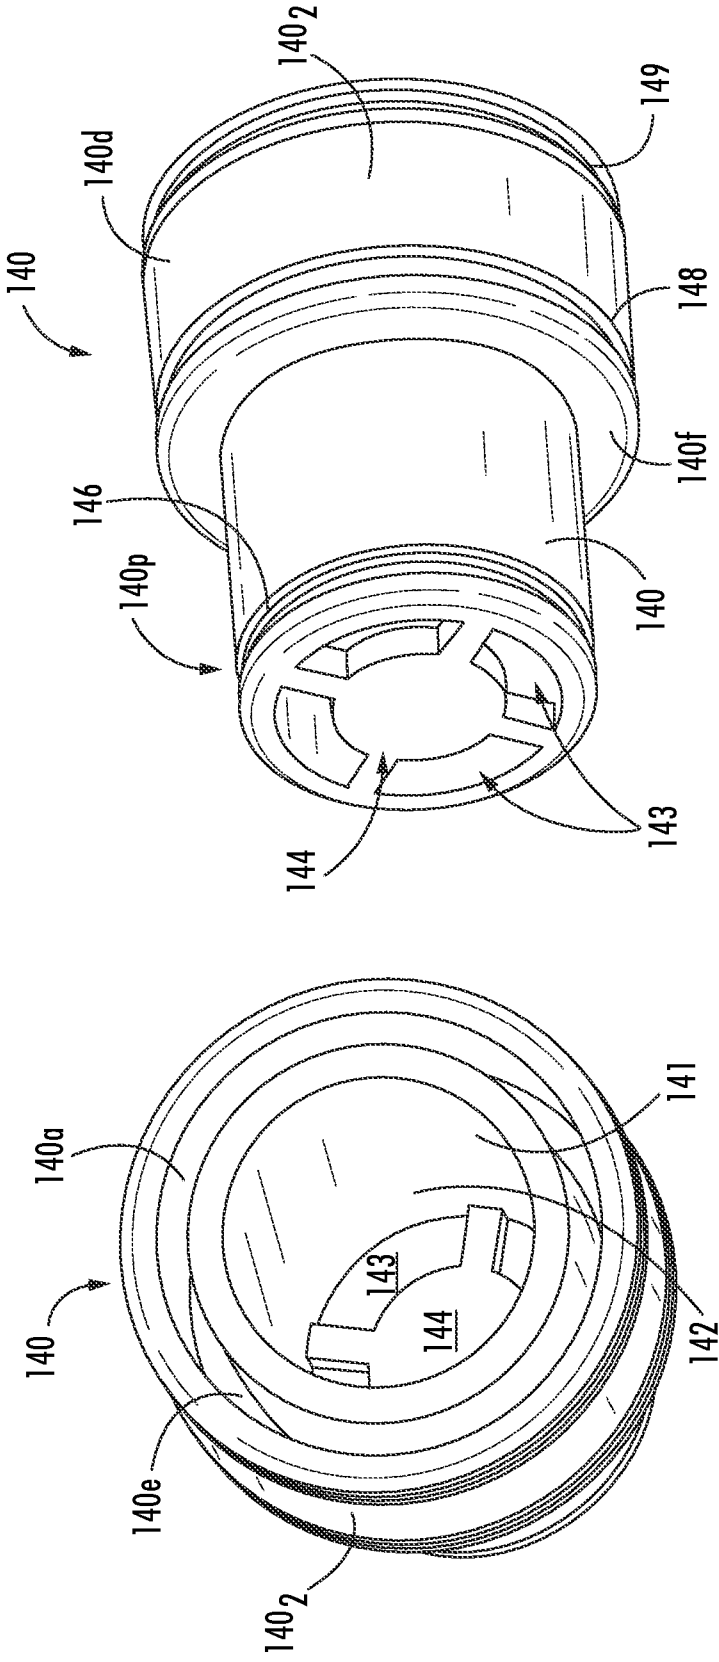


FIG. 12

FIG. 11

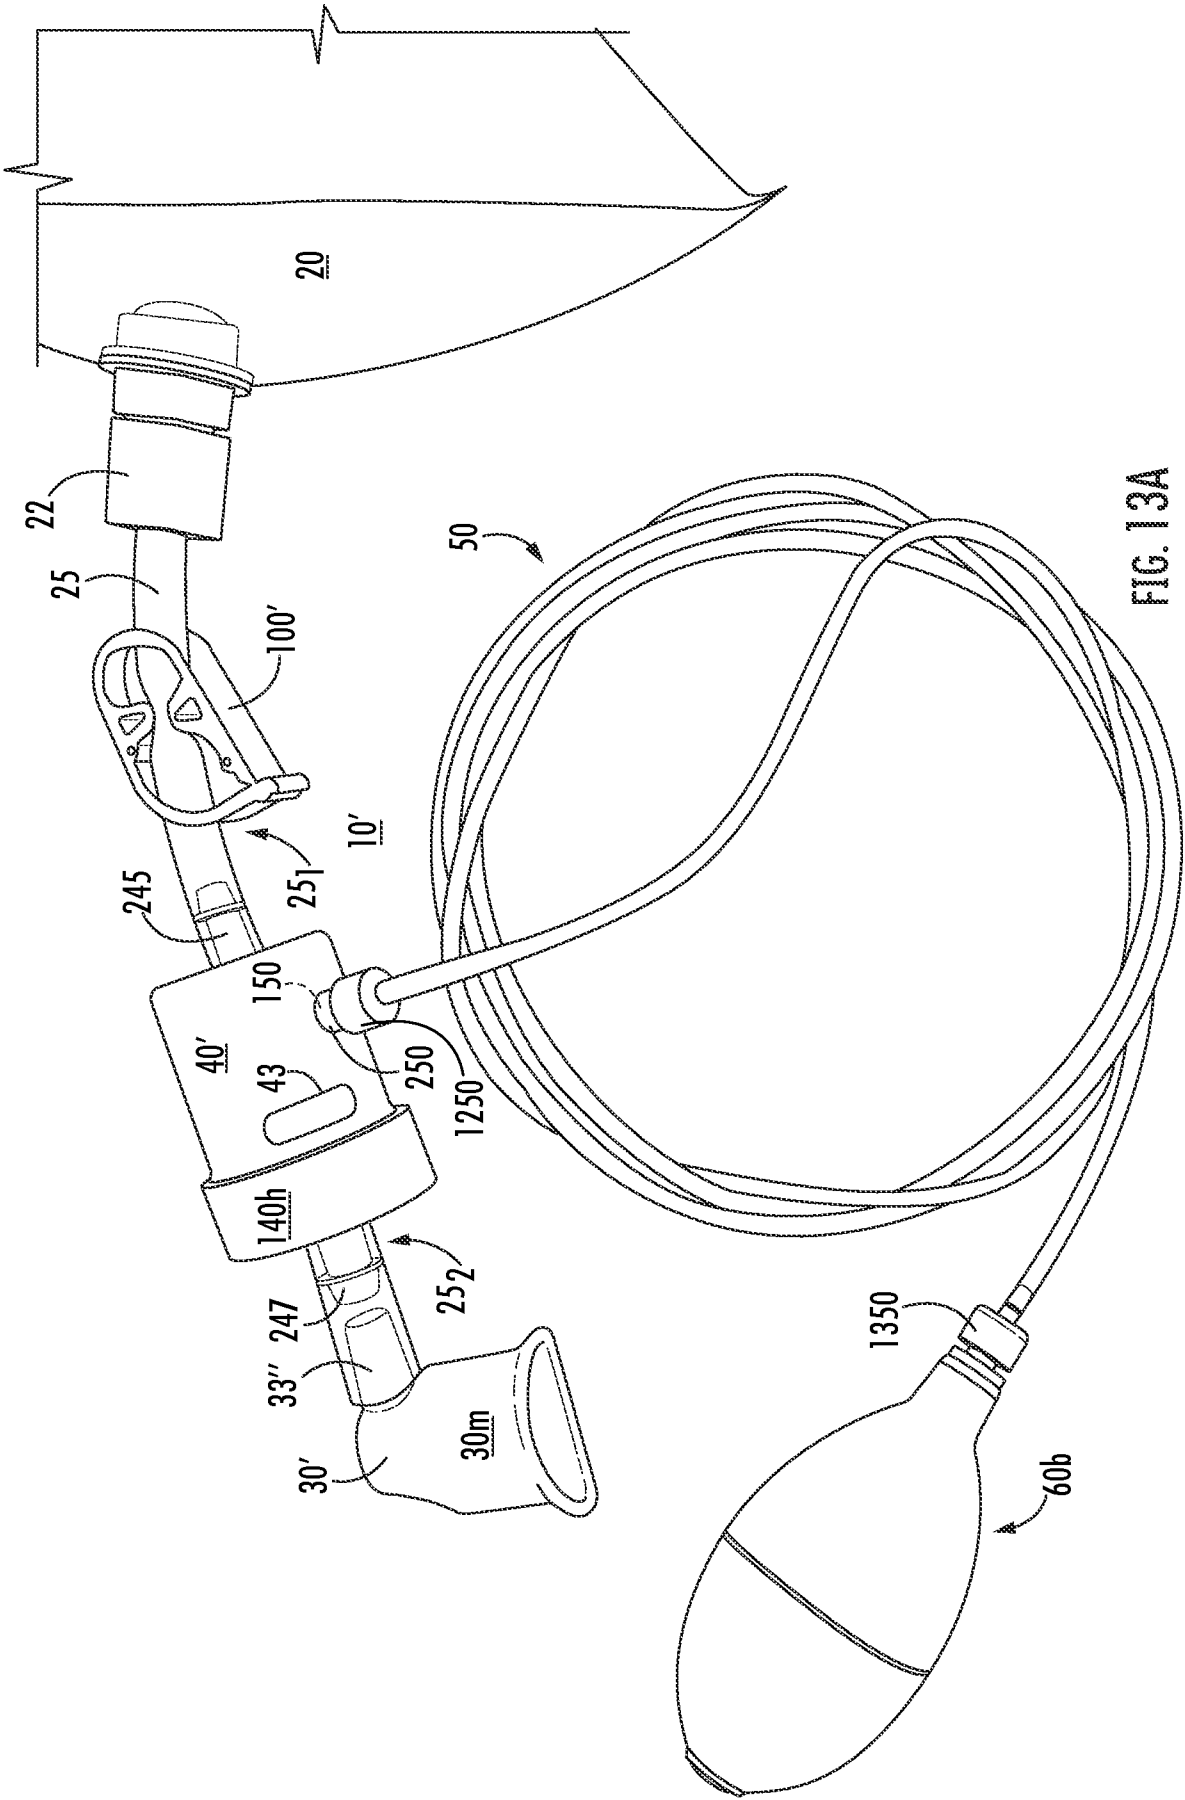

17/37

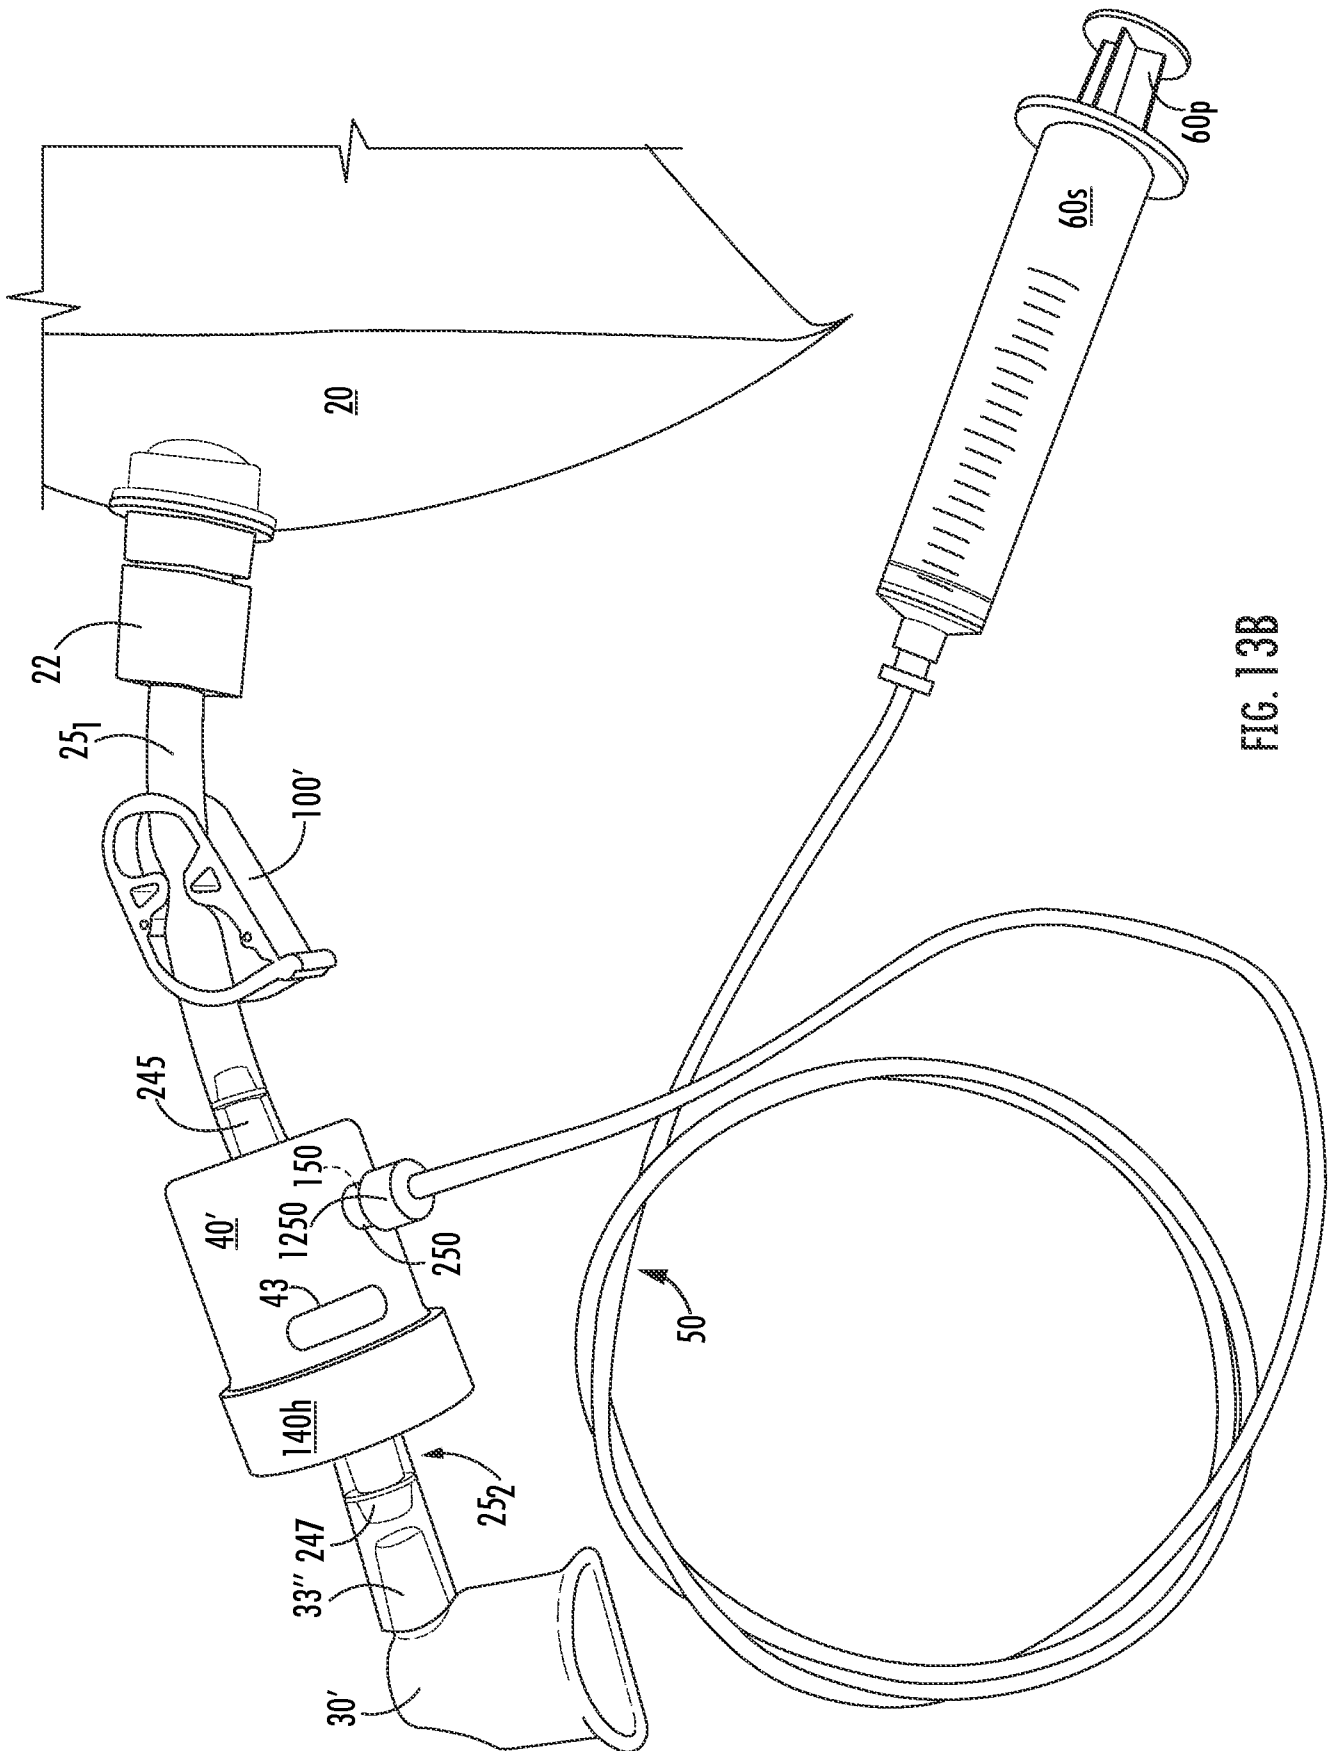


FIG. 13B

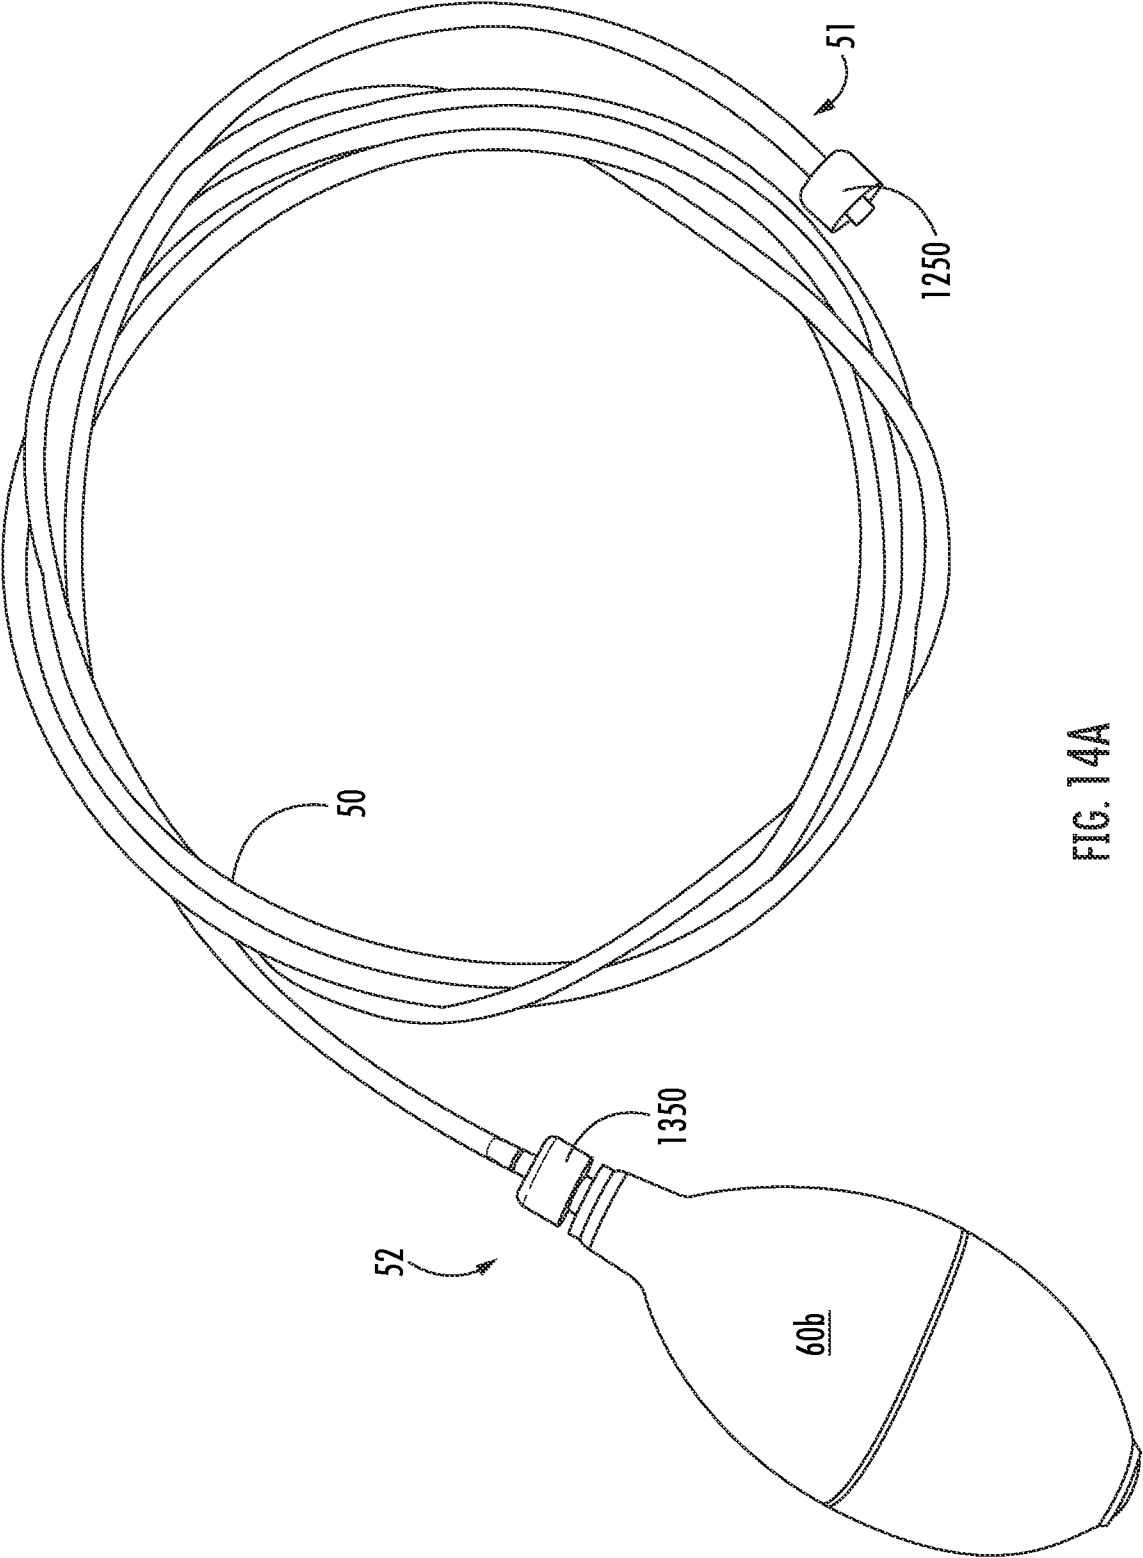


FIG. 14A

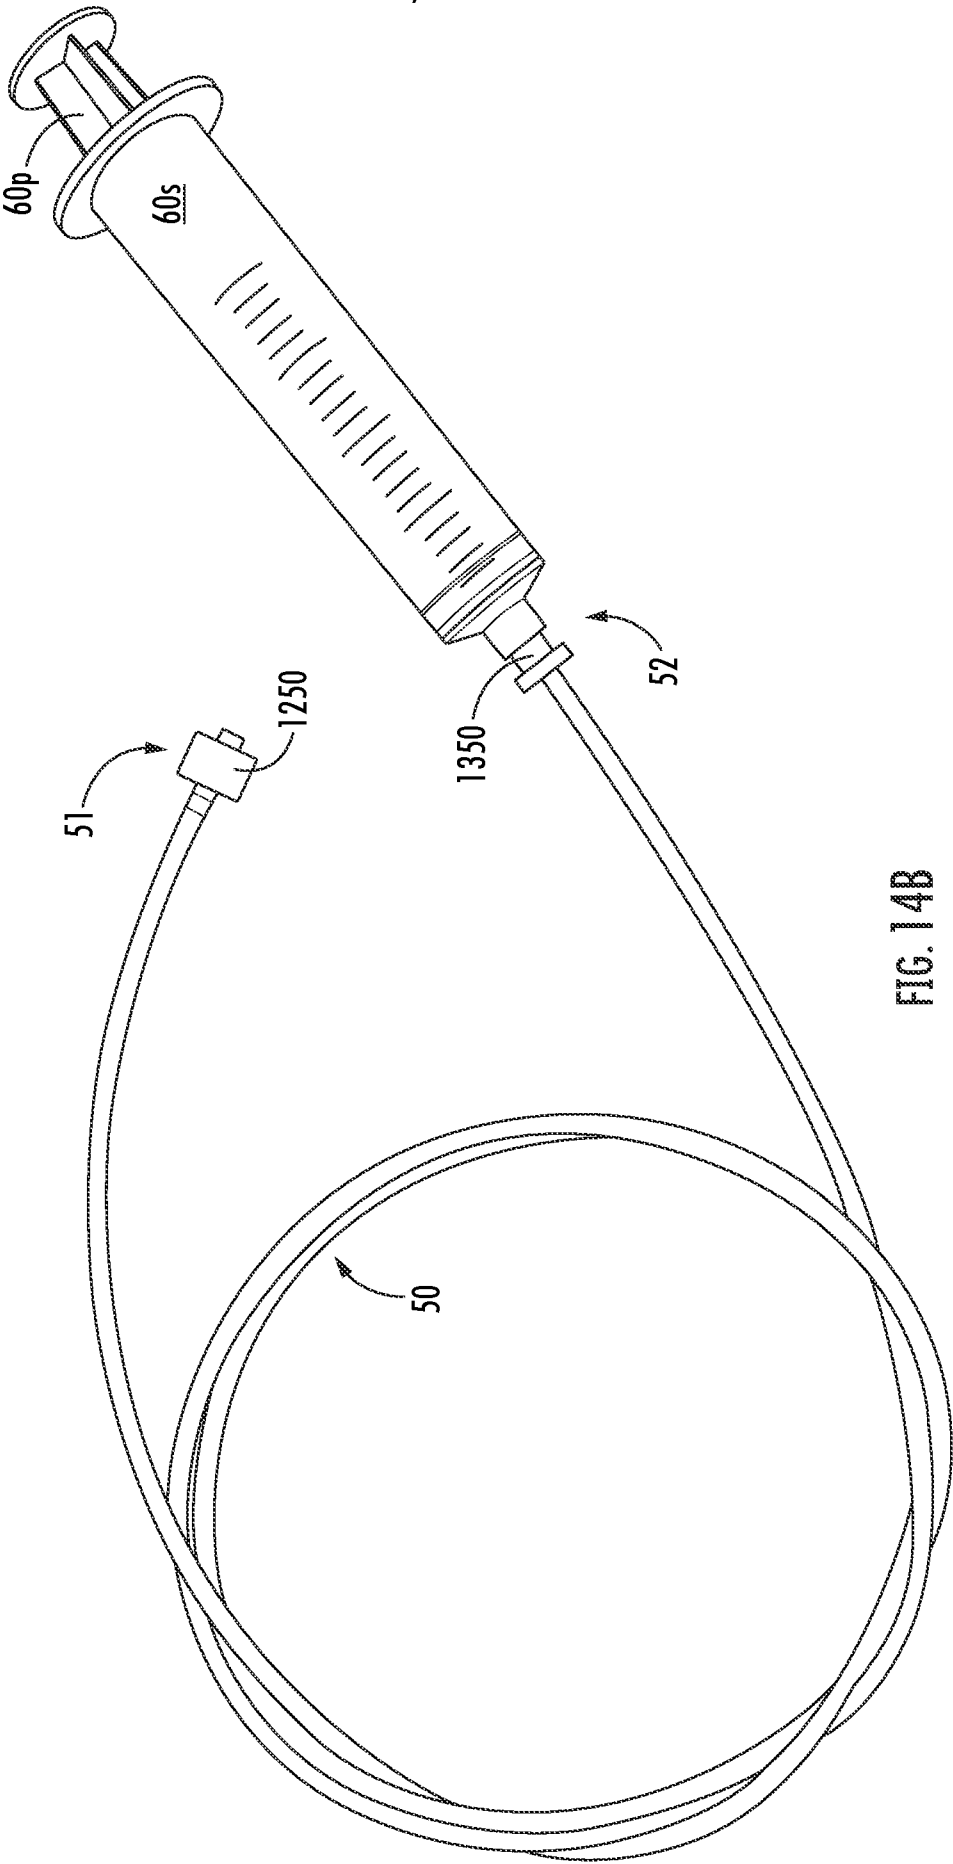


FIG. 14B

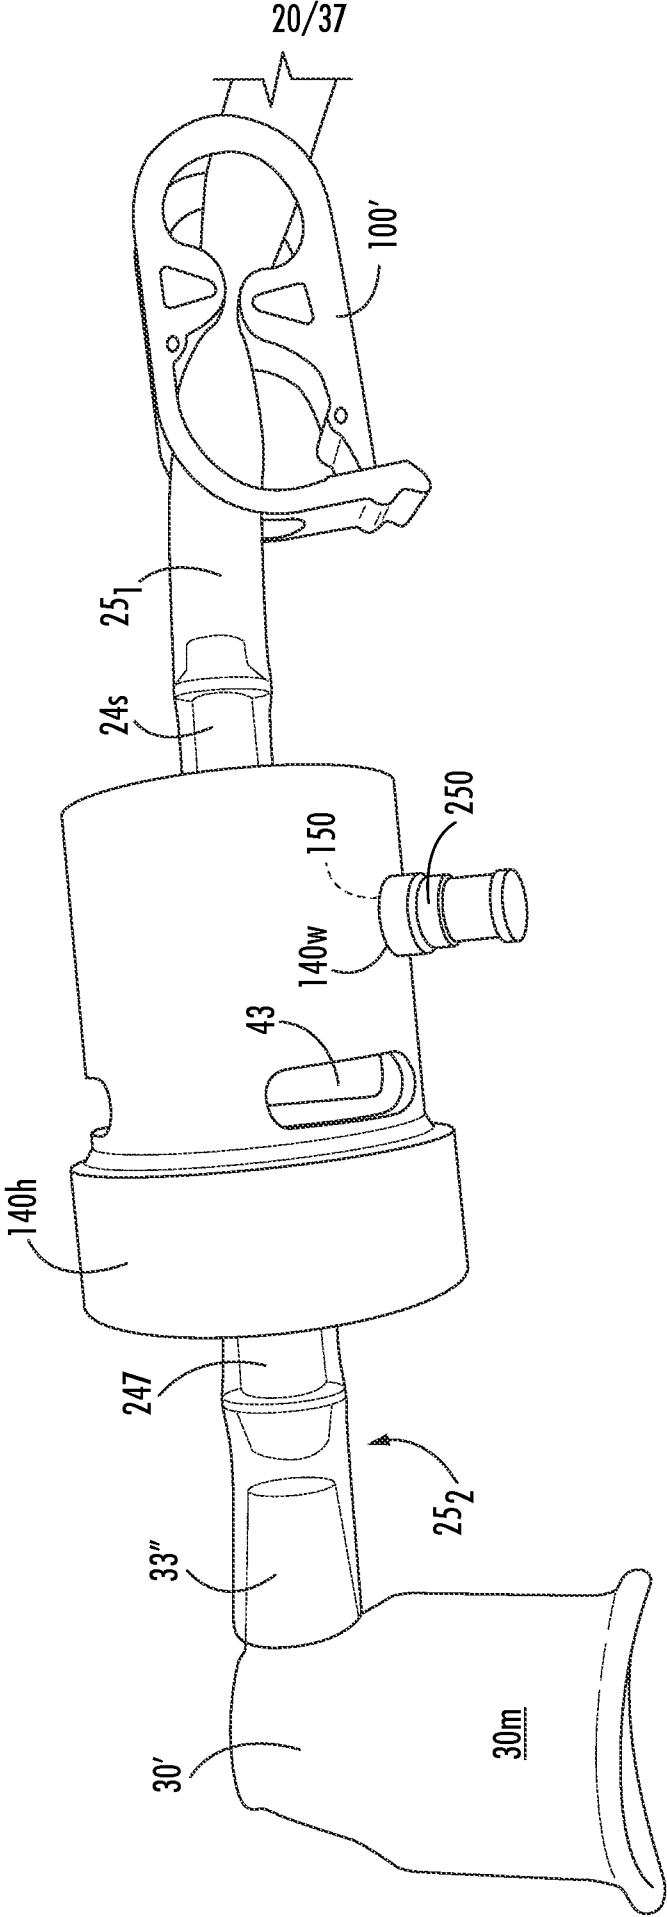


FIG. 15



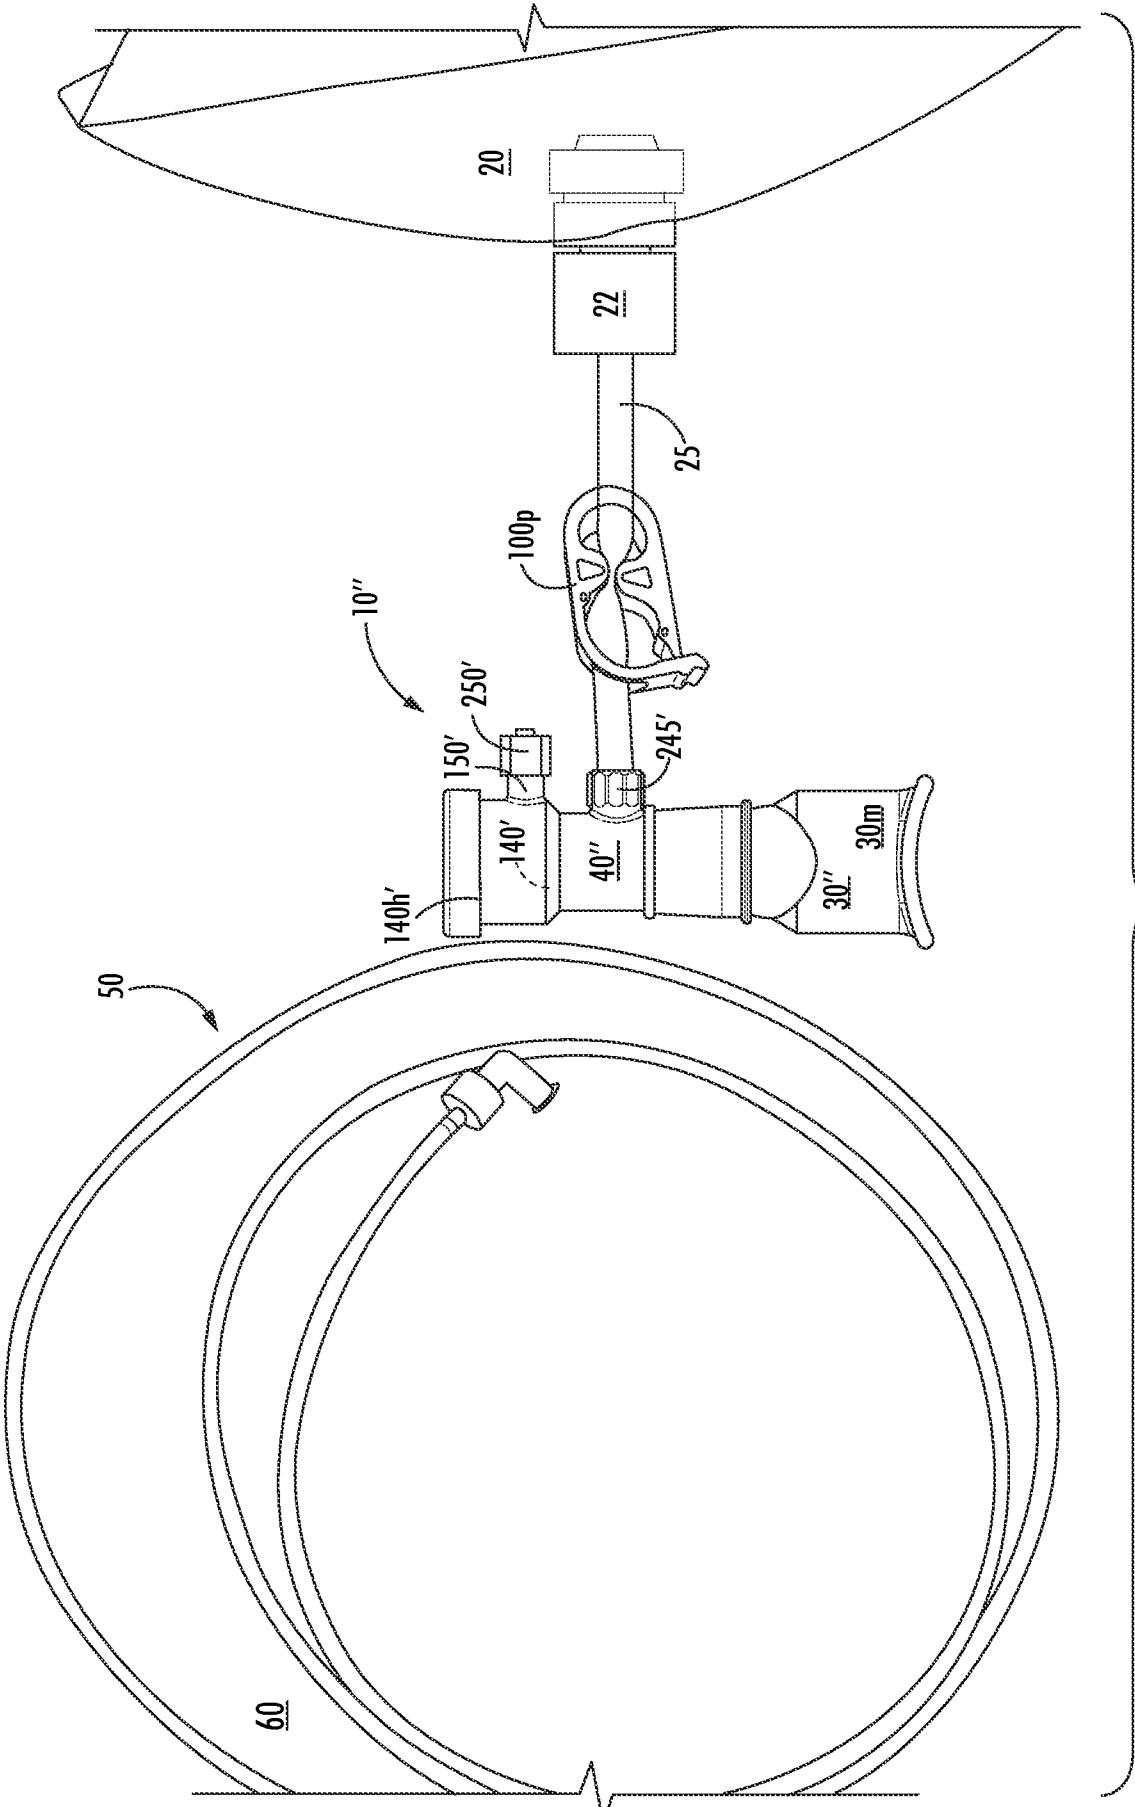


FIG. 16

22/37

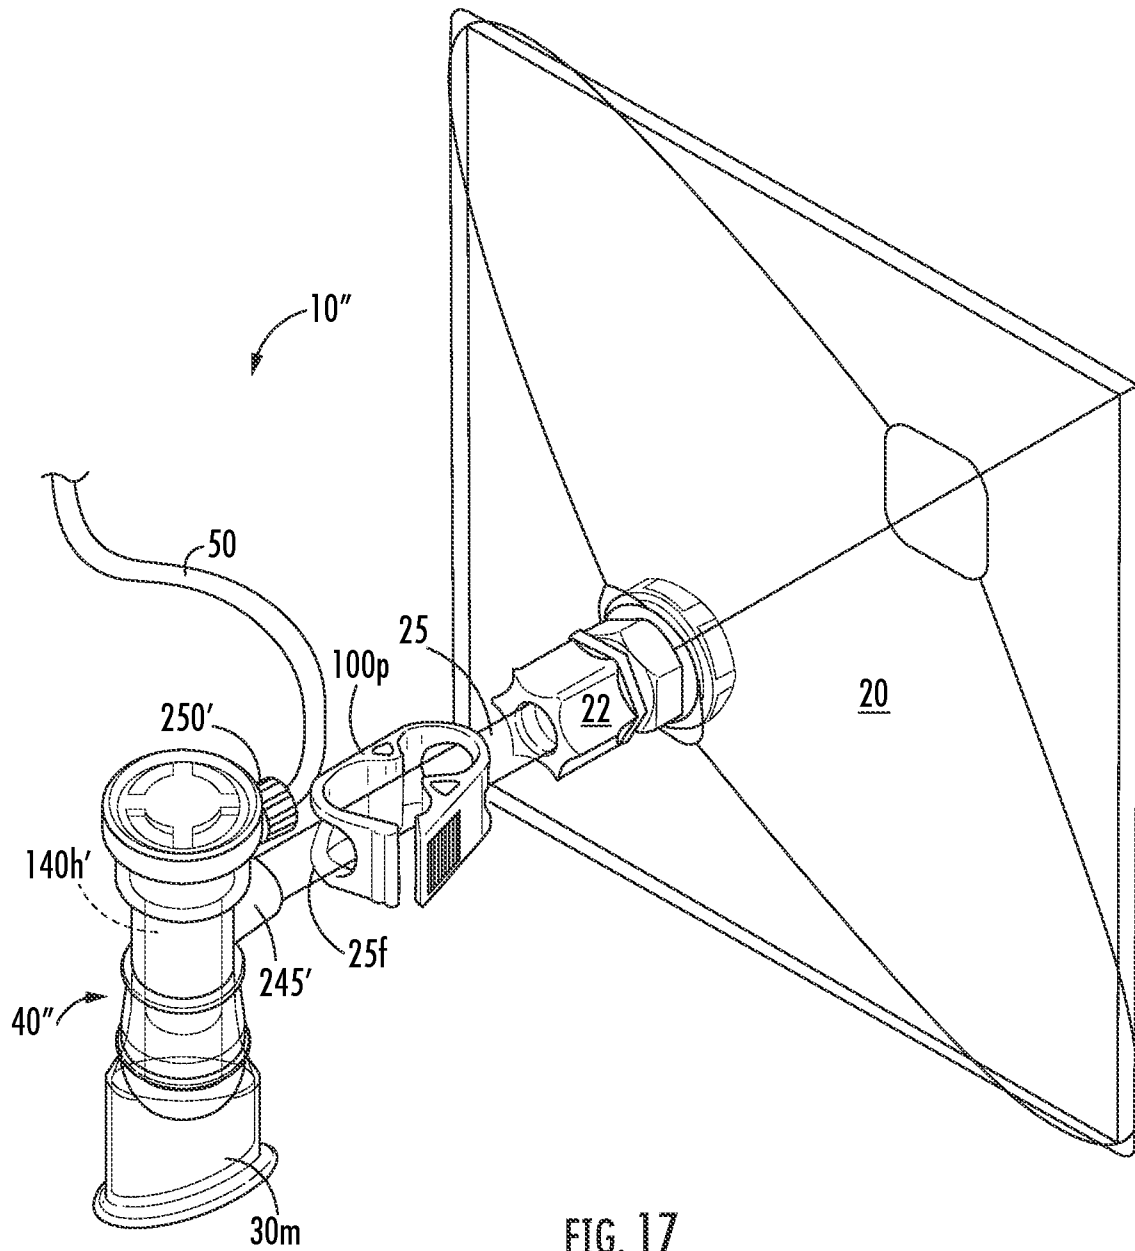

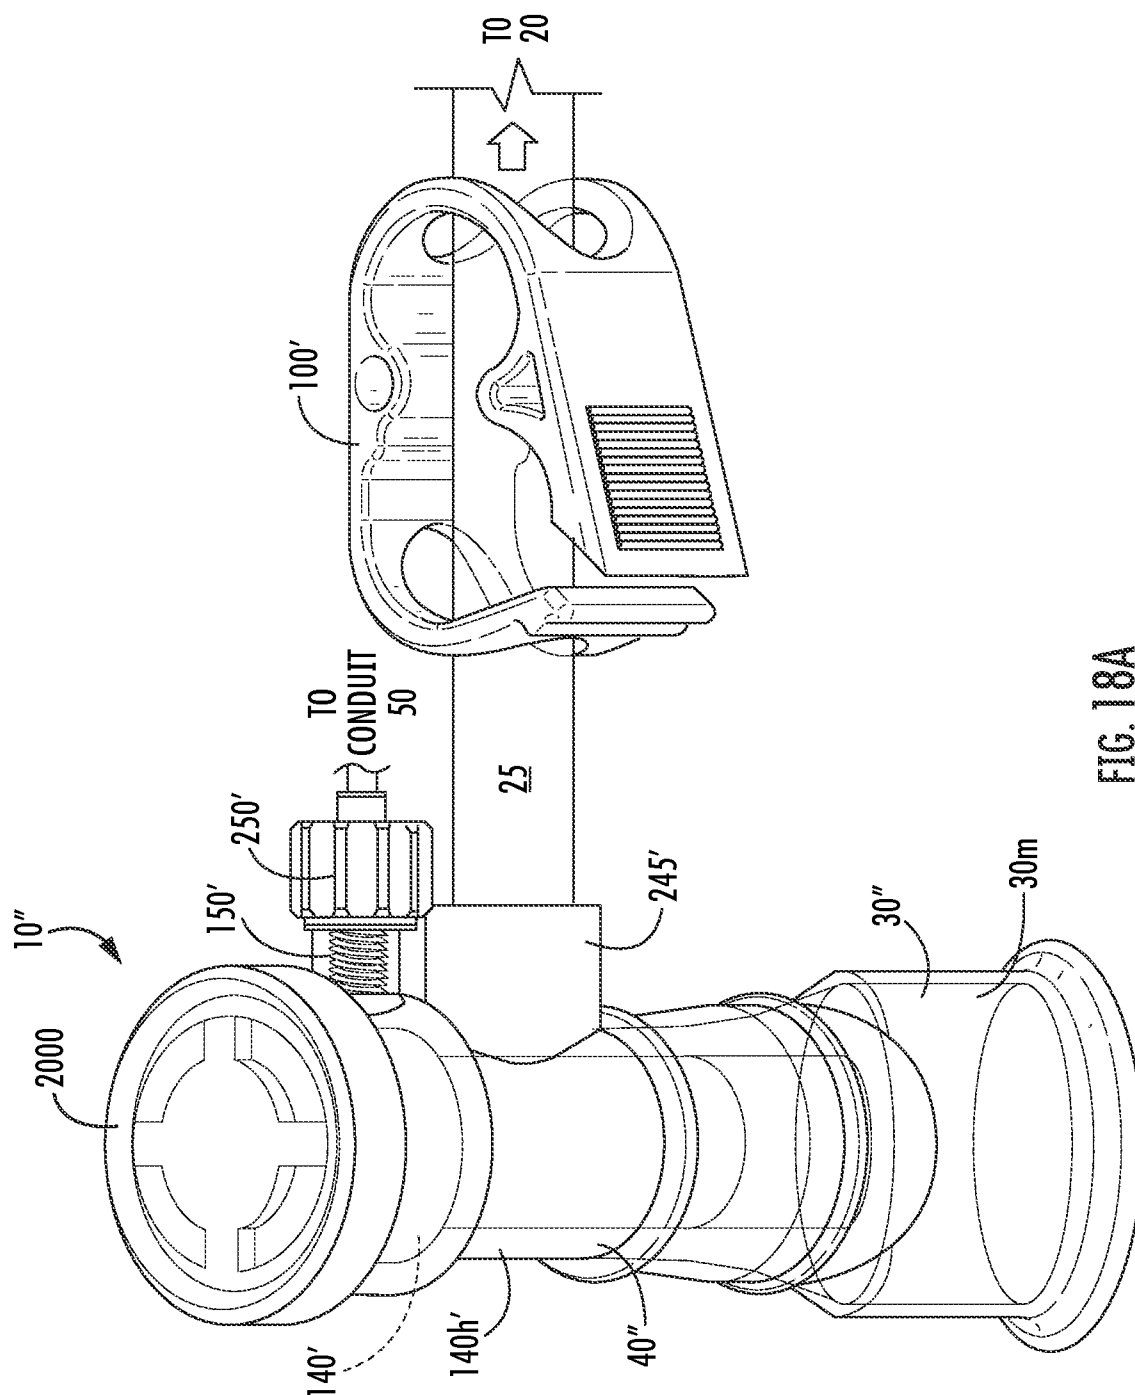

24/37

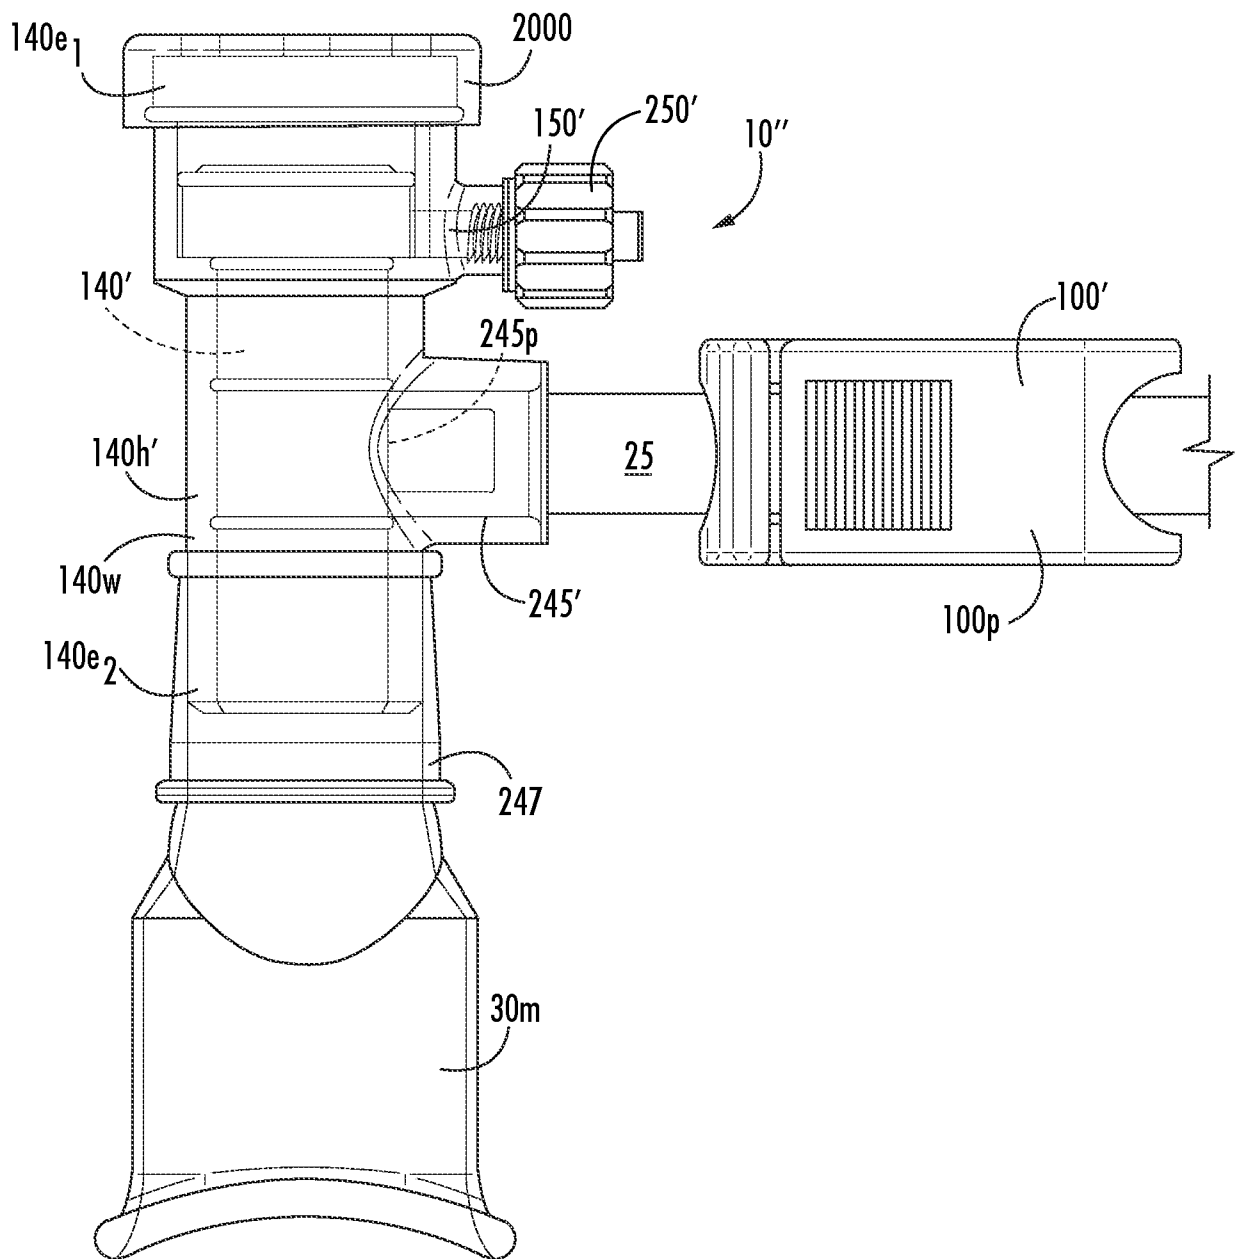


FIG. 18B

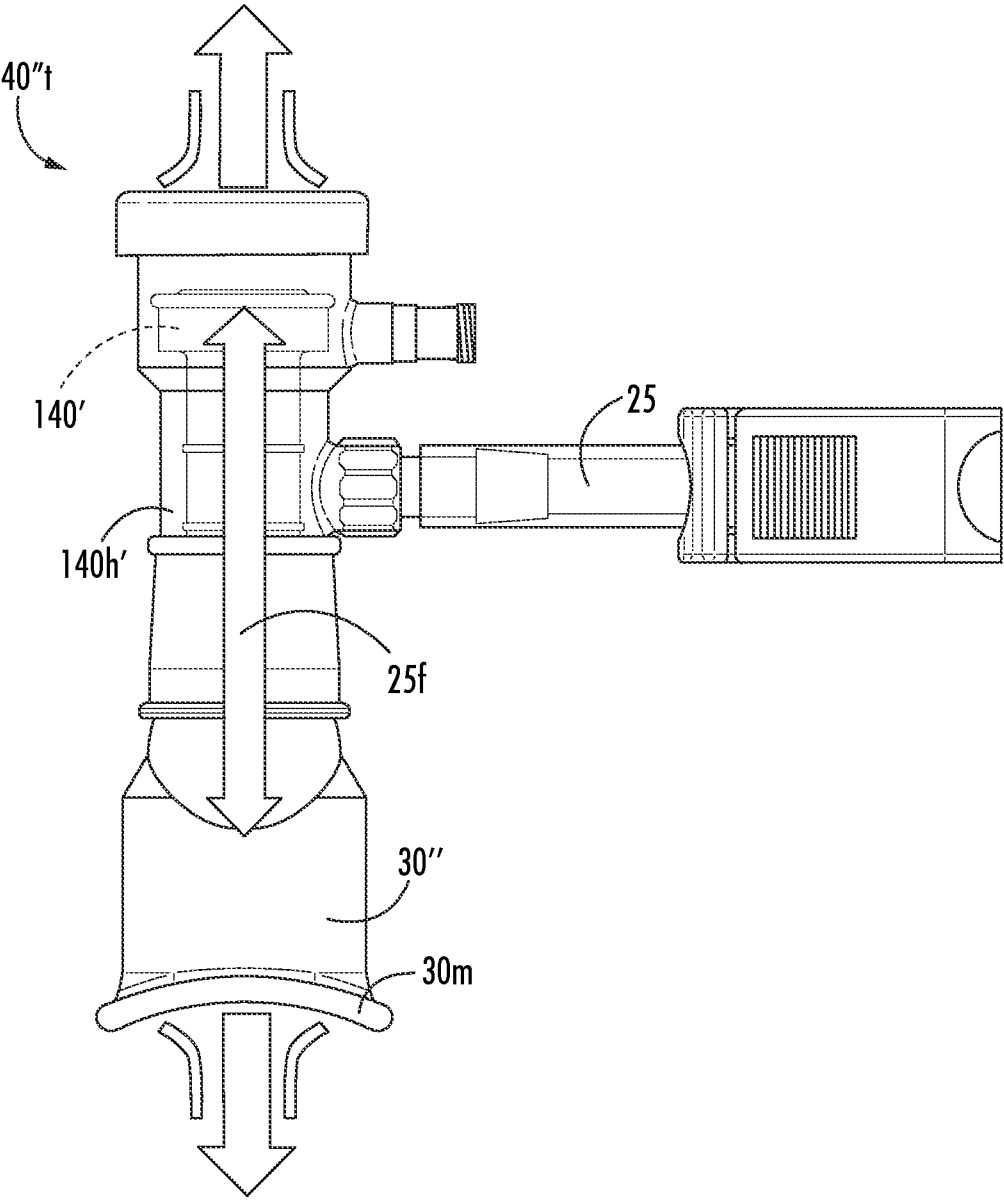


FIG. 19A

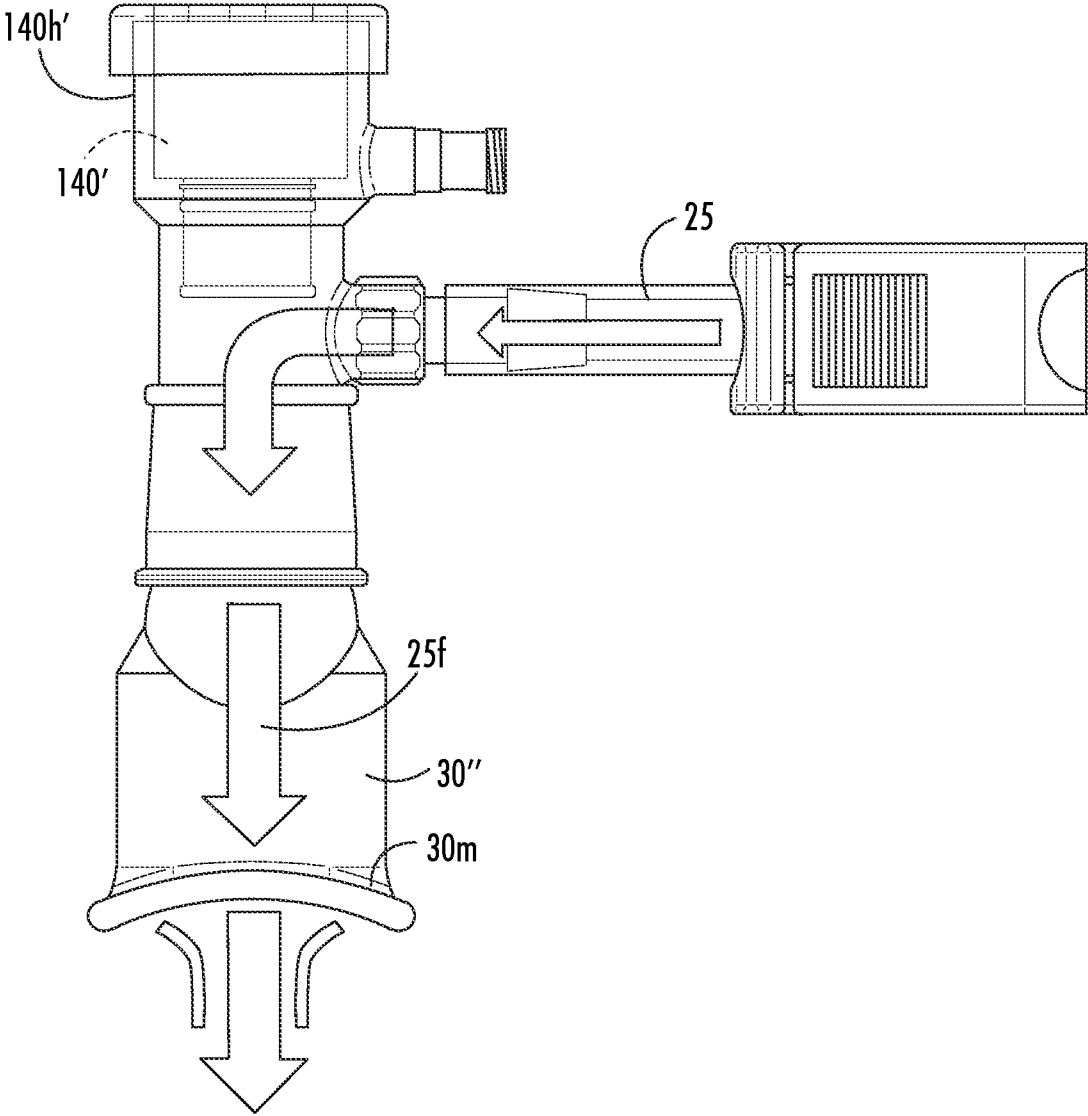


FIG. 19B

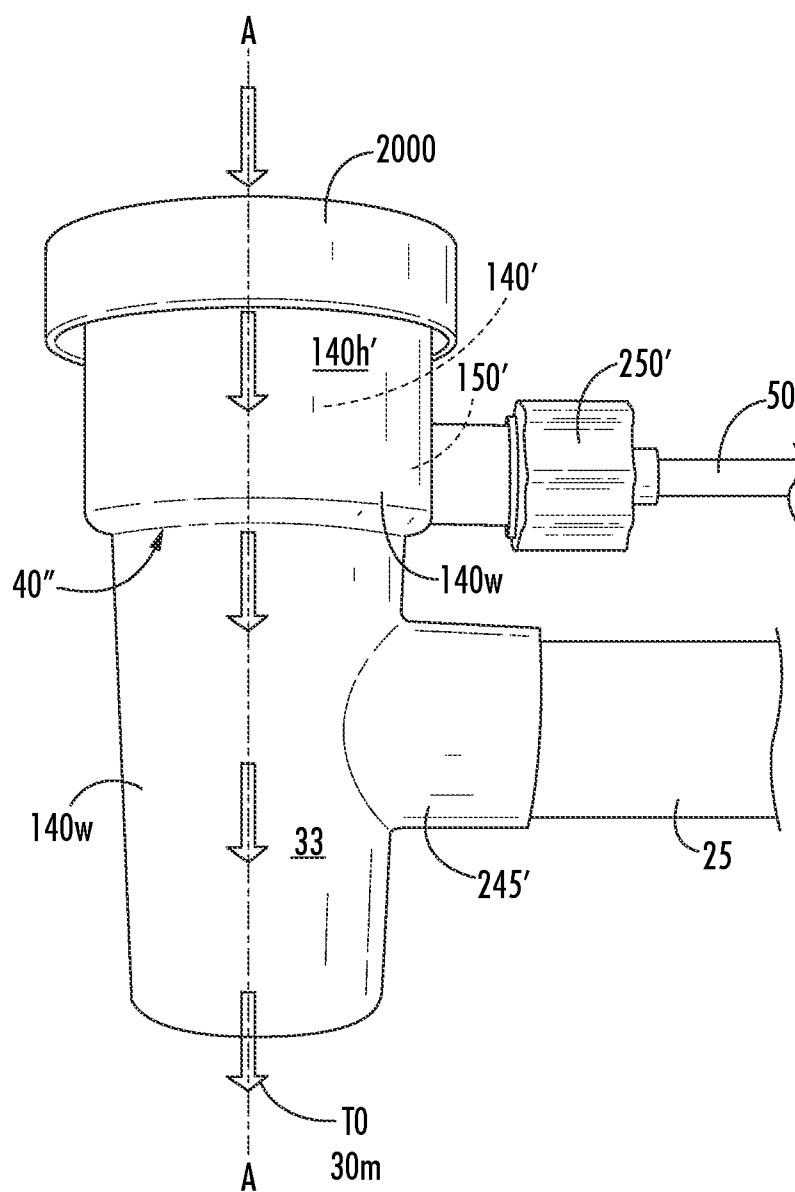


FIG. 20

28/37

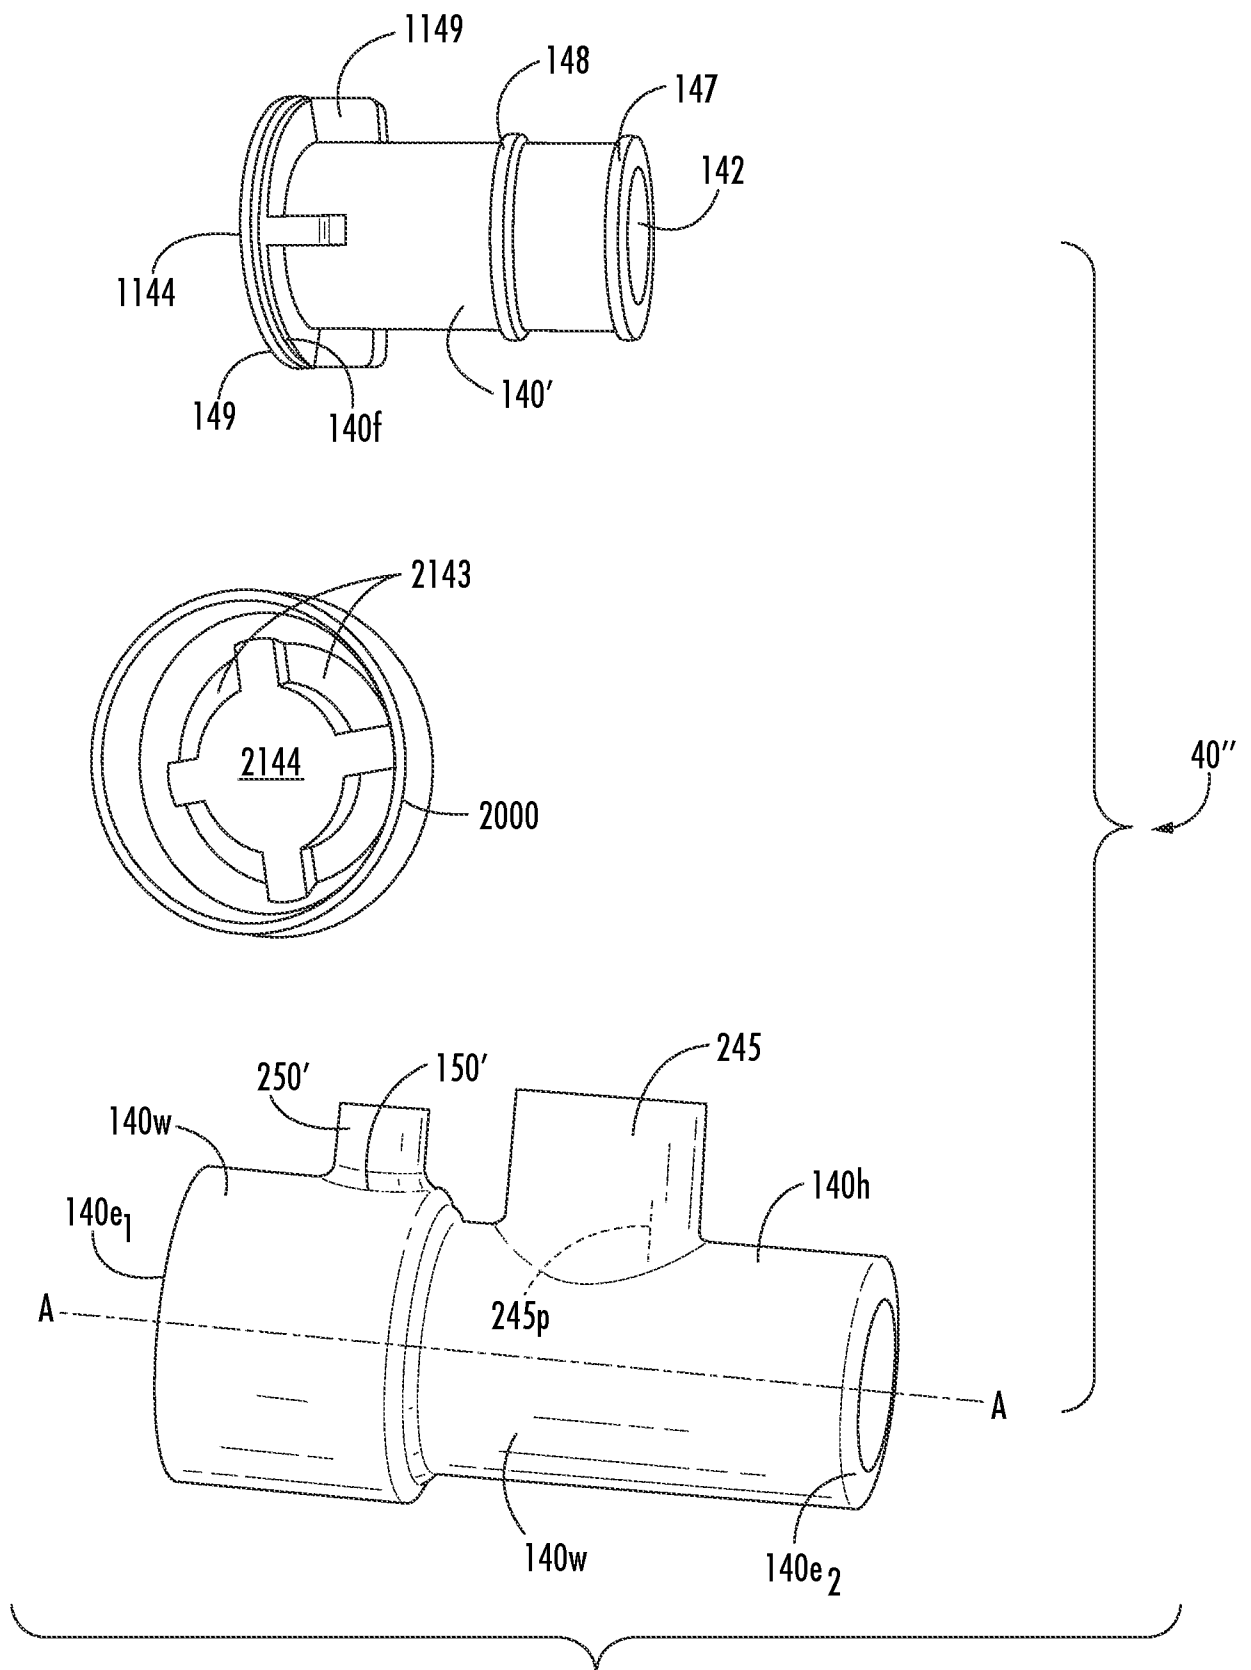


FIG. 21

29/37

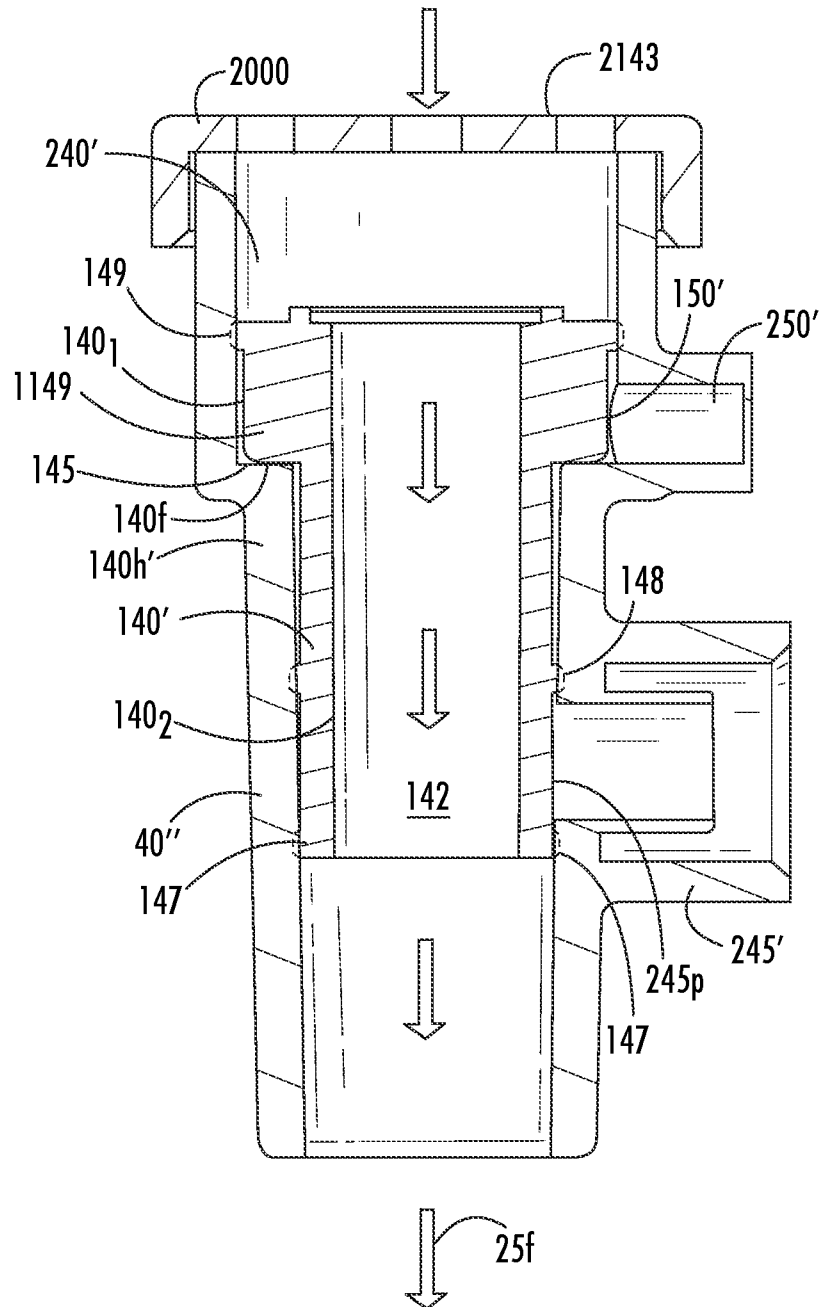


FIG. 22A

30/37

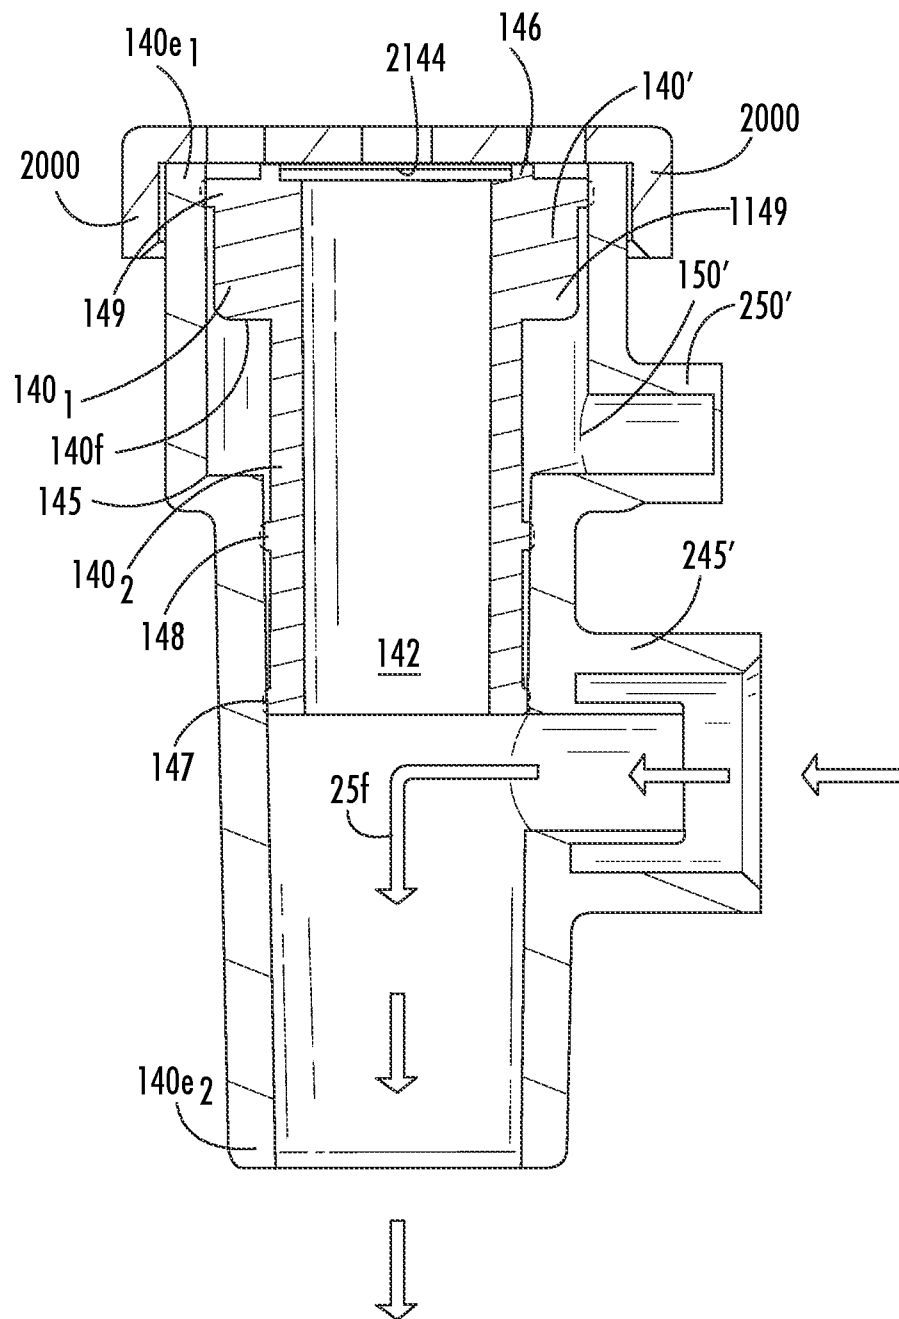


FIG. 22B

31/37

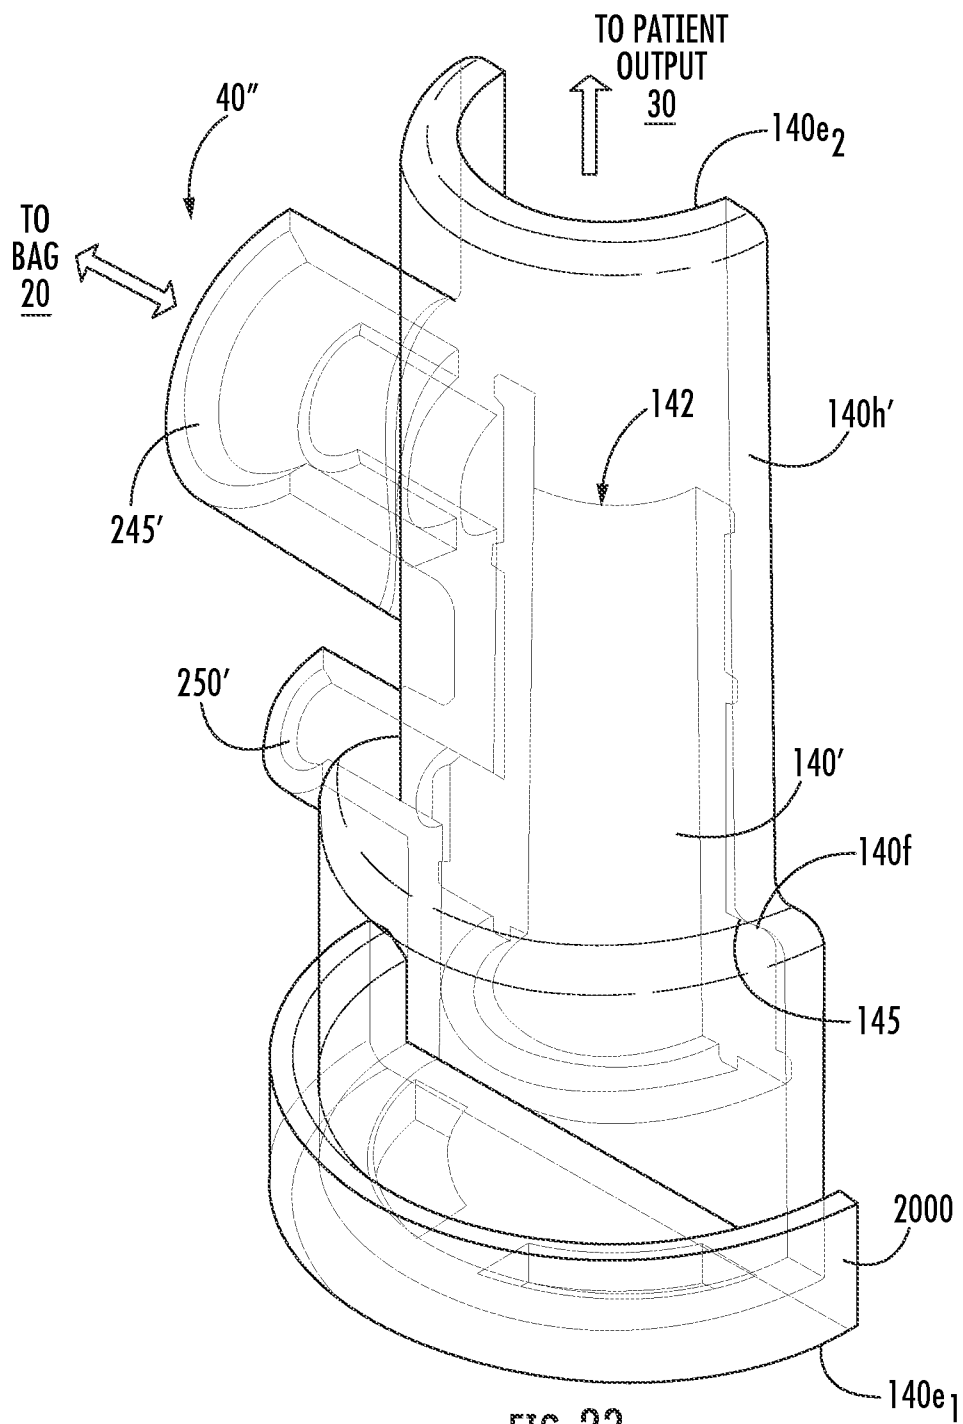


FIG. 23

32/37

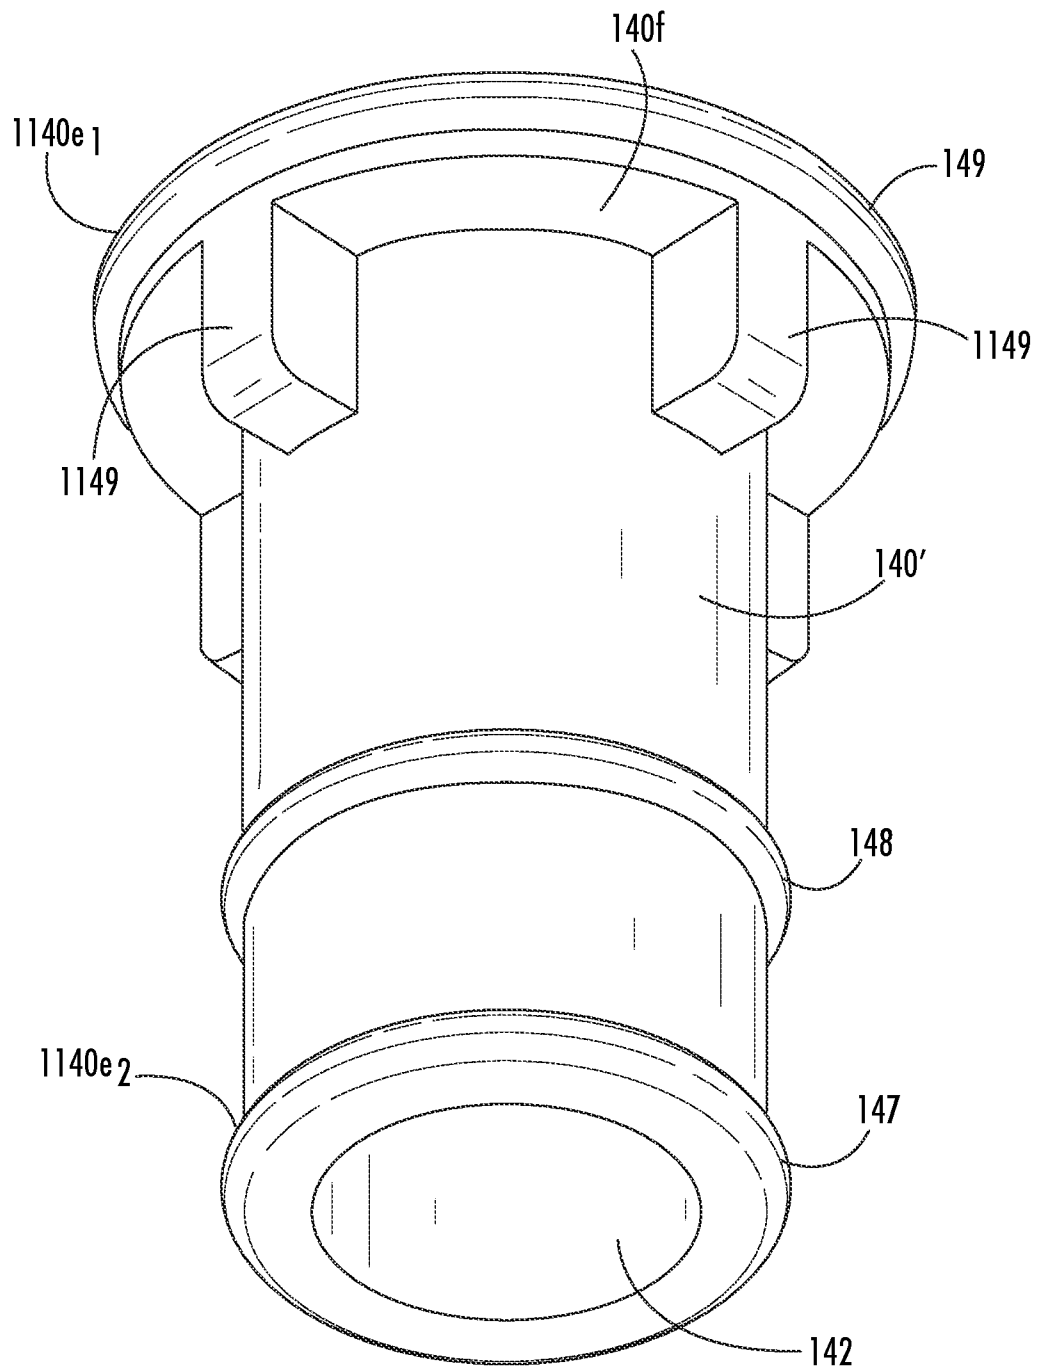


FIG. 24A

33/37

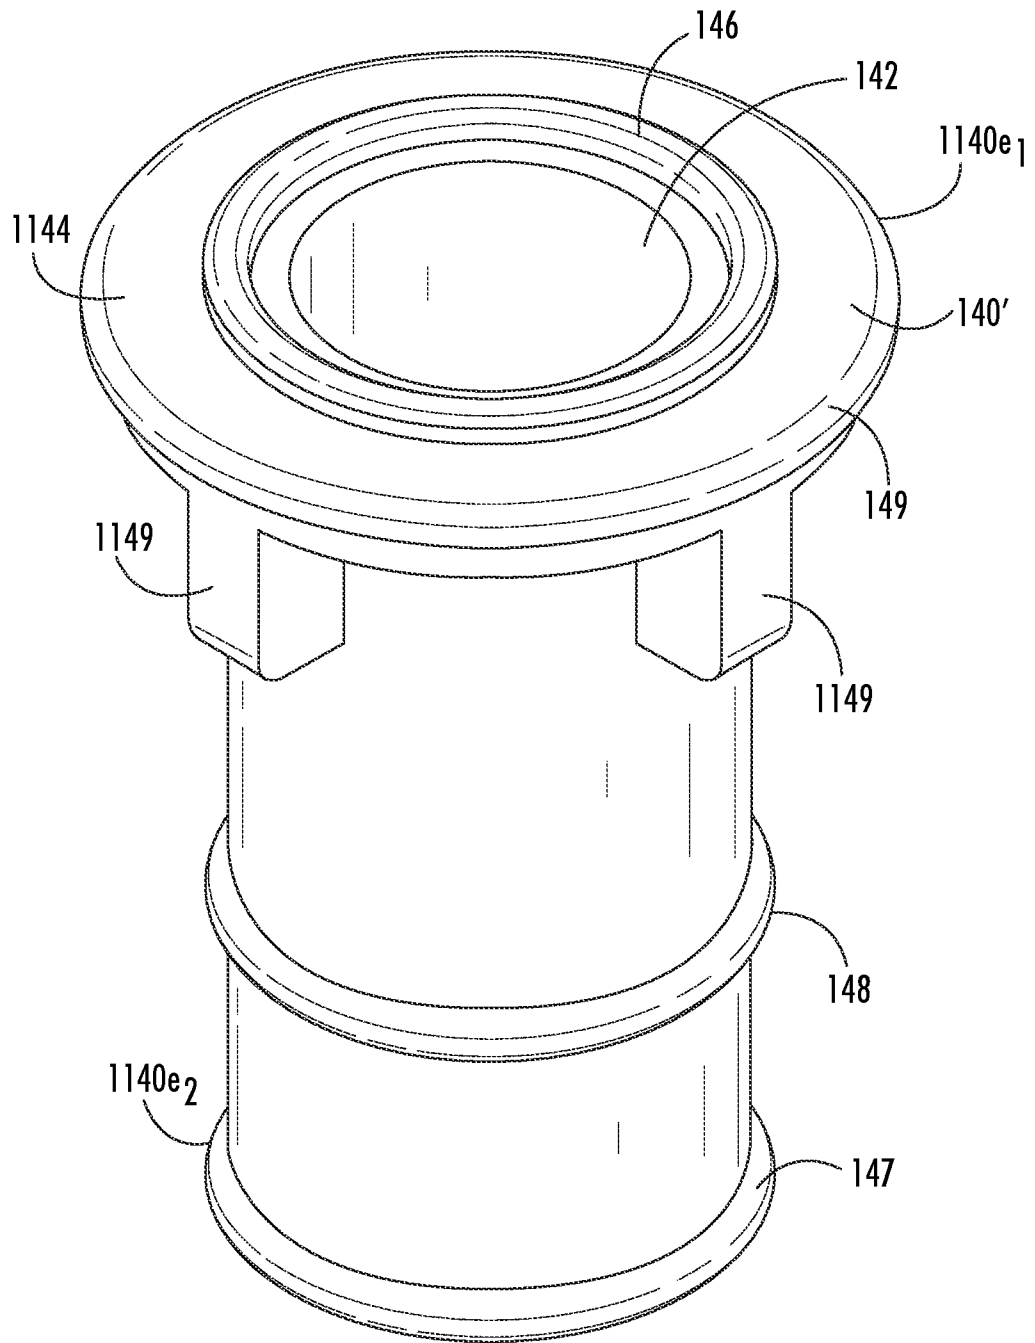


FIG. 24B

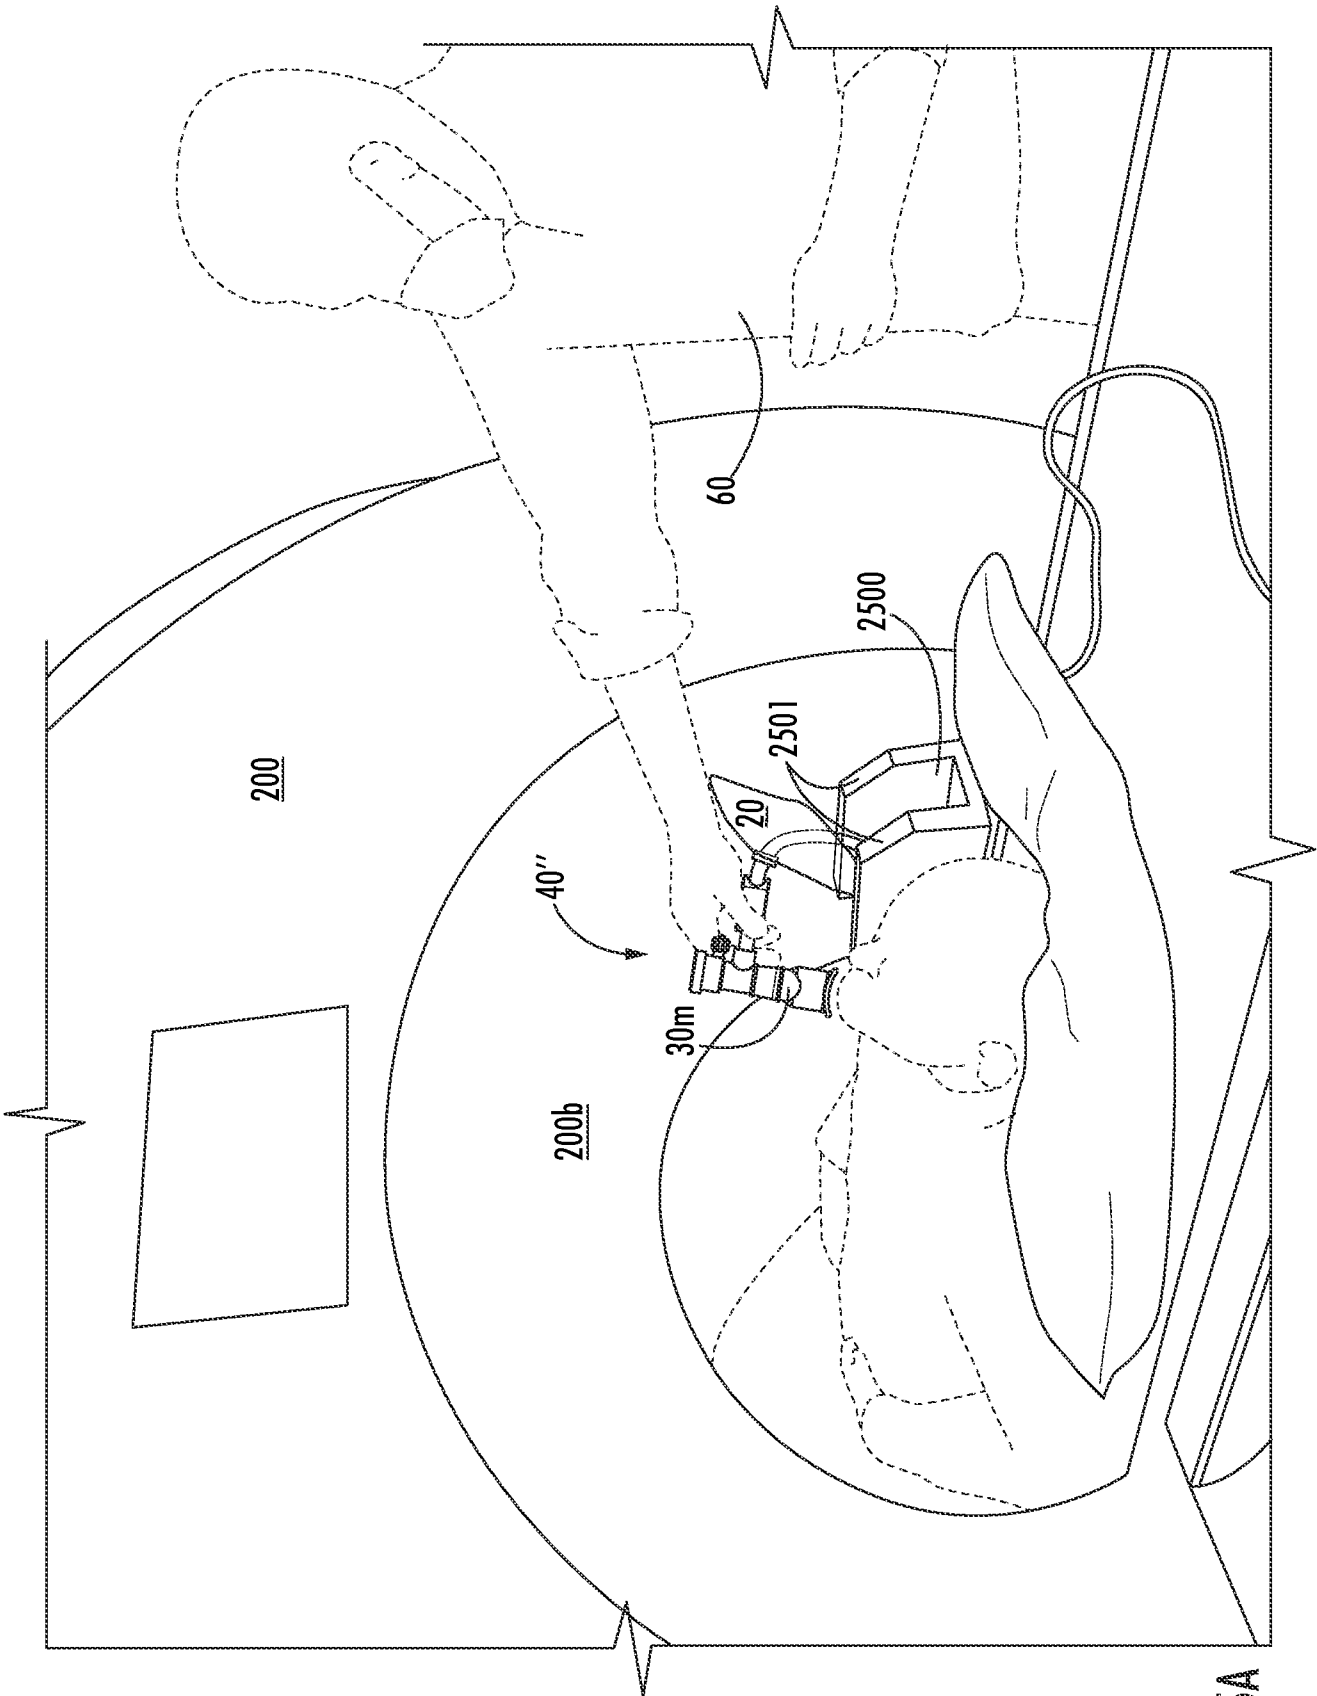
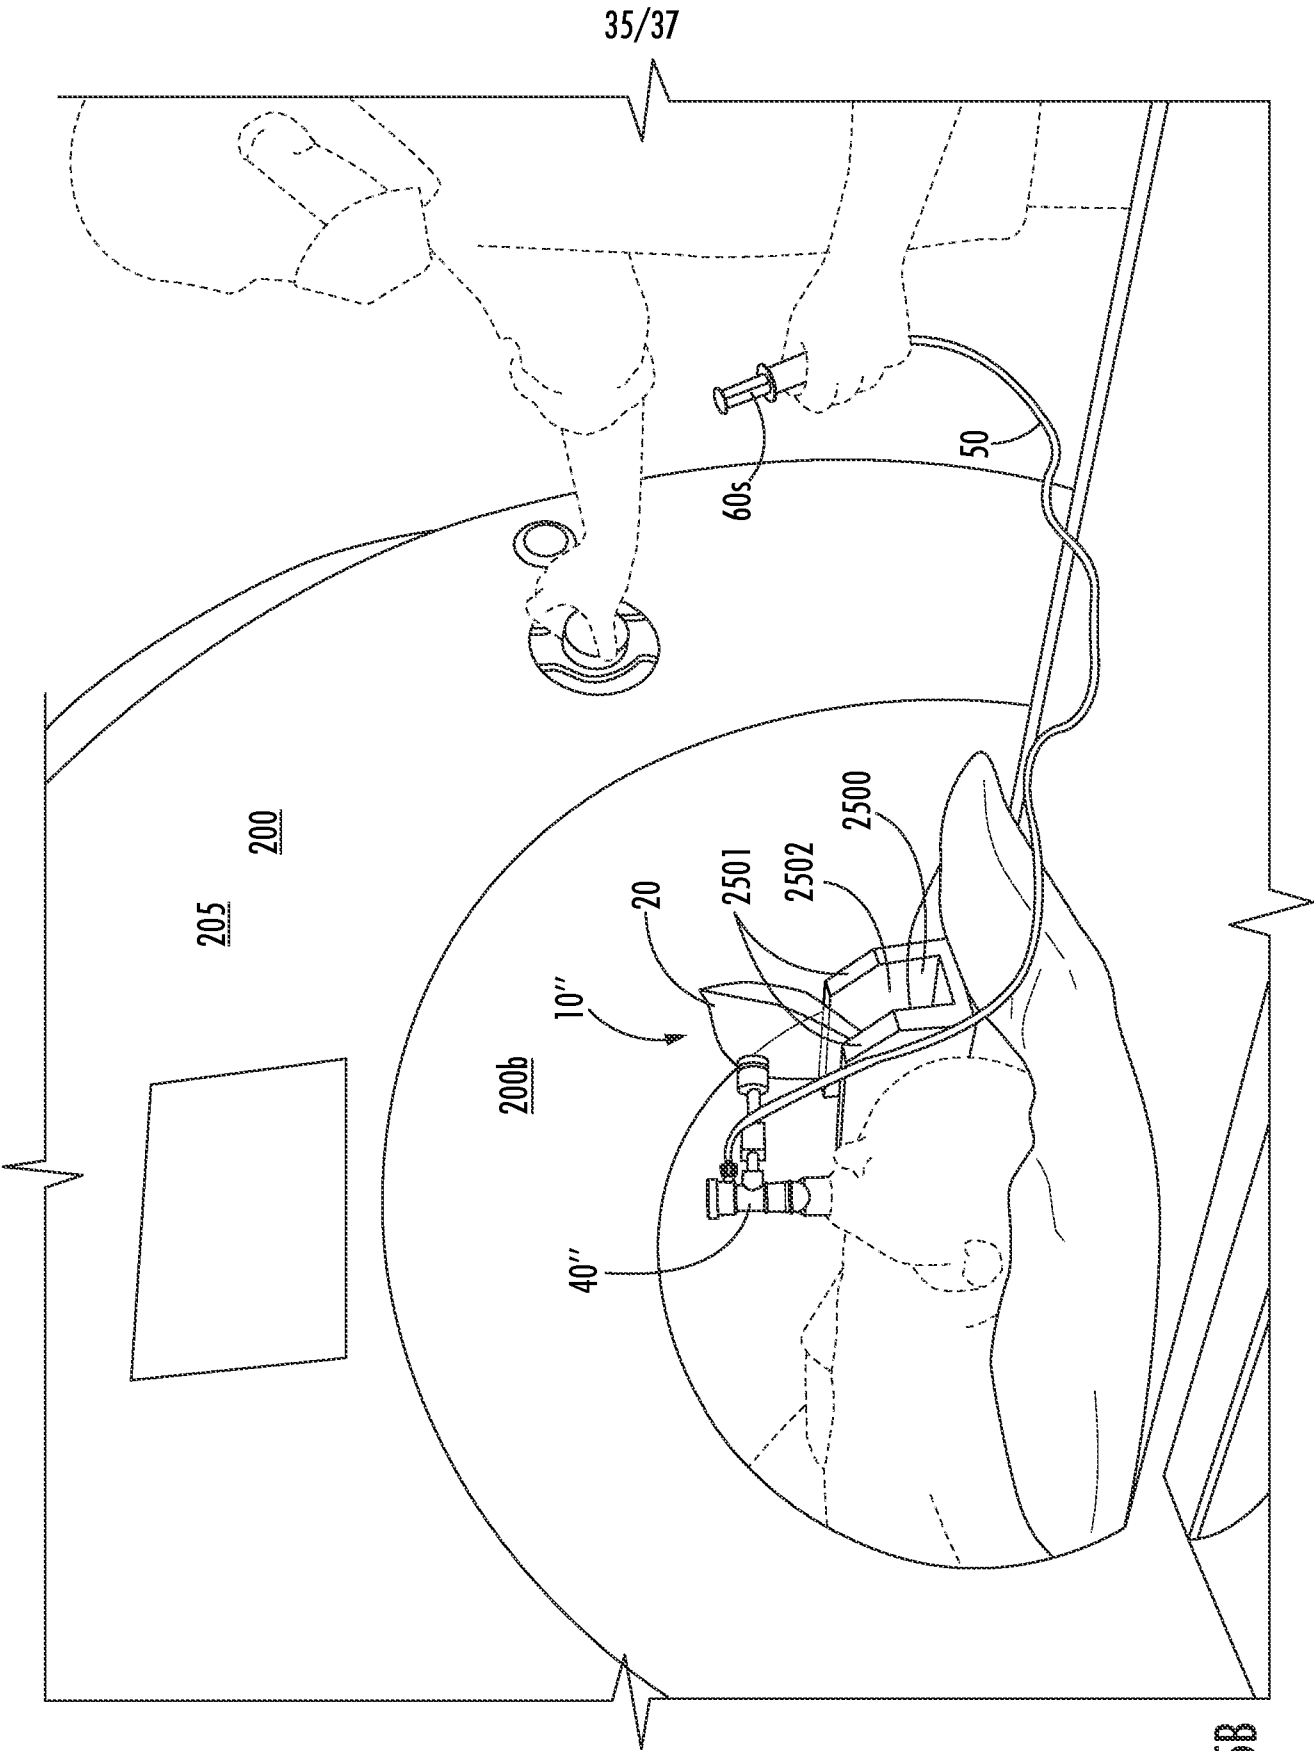


FIG. 25A



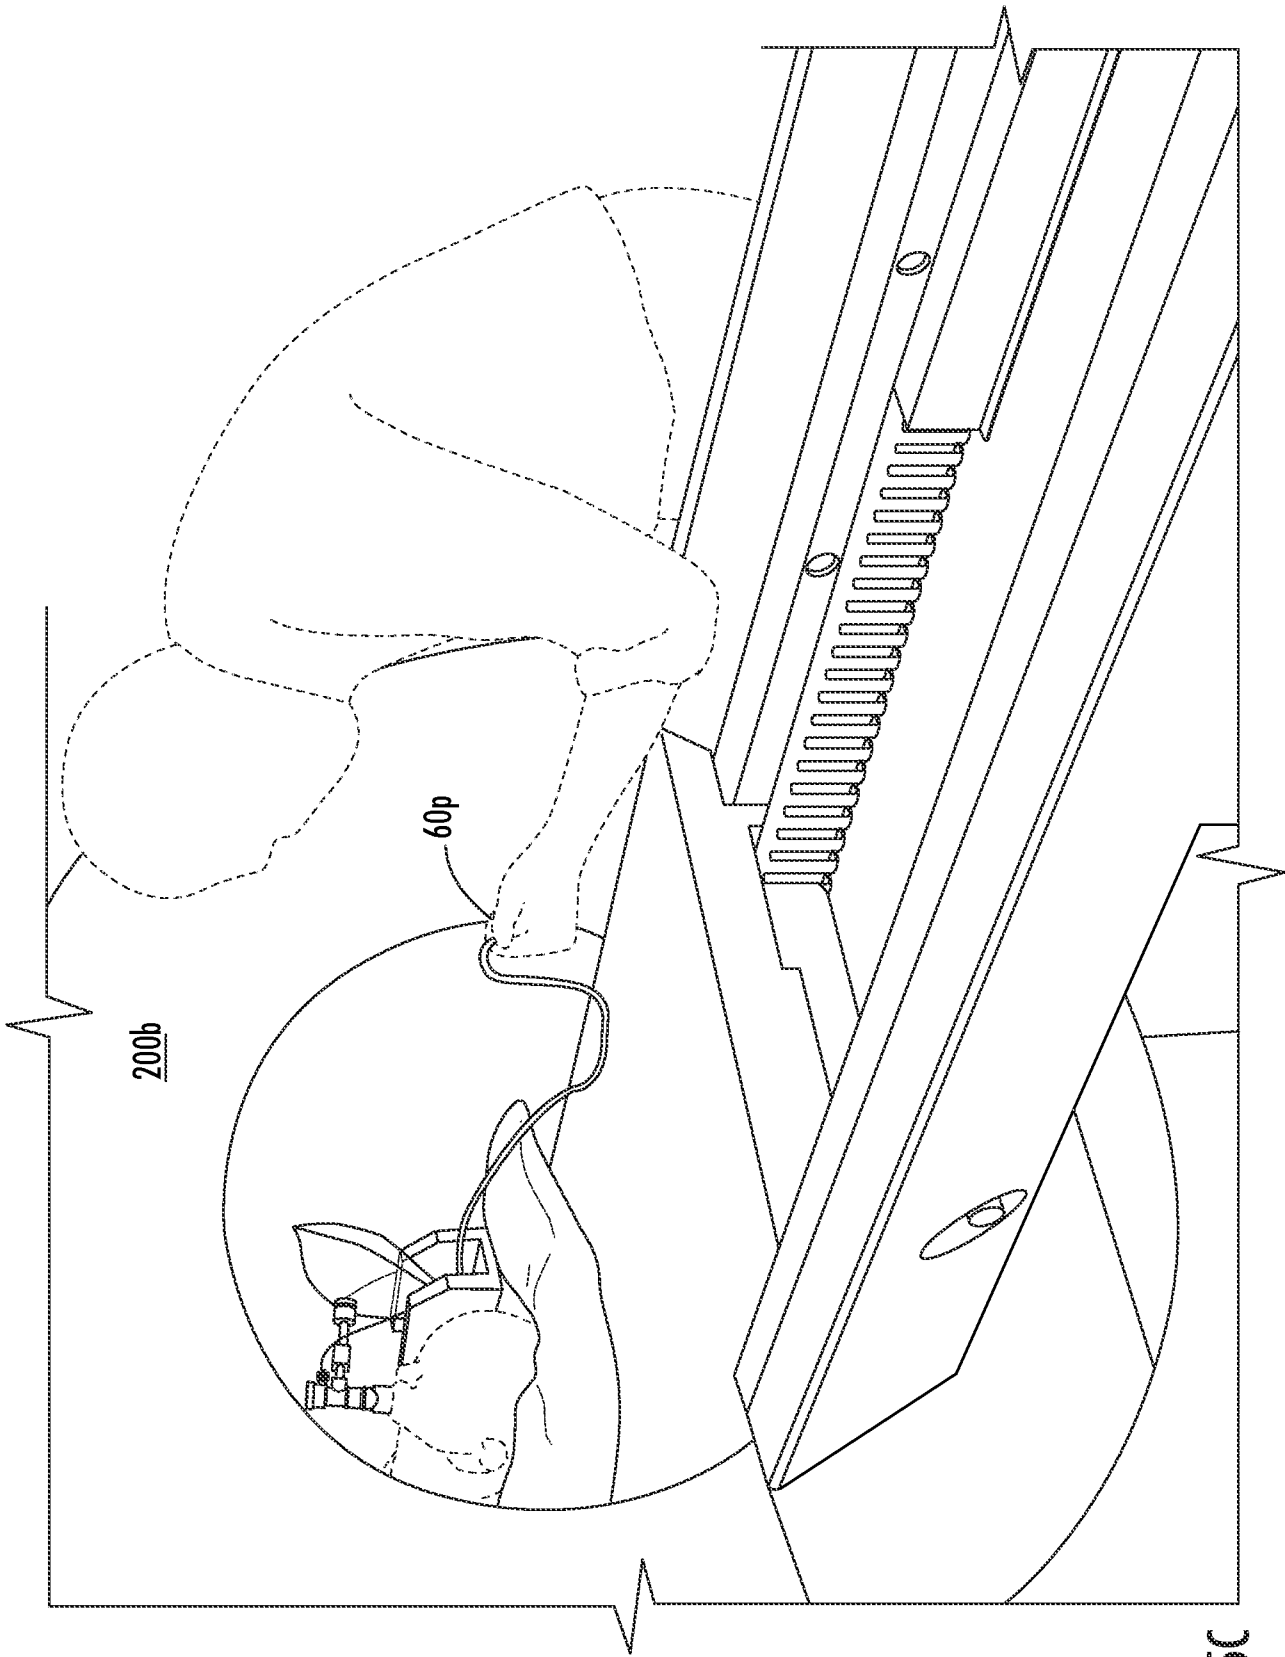


FIG. 25C

37/37

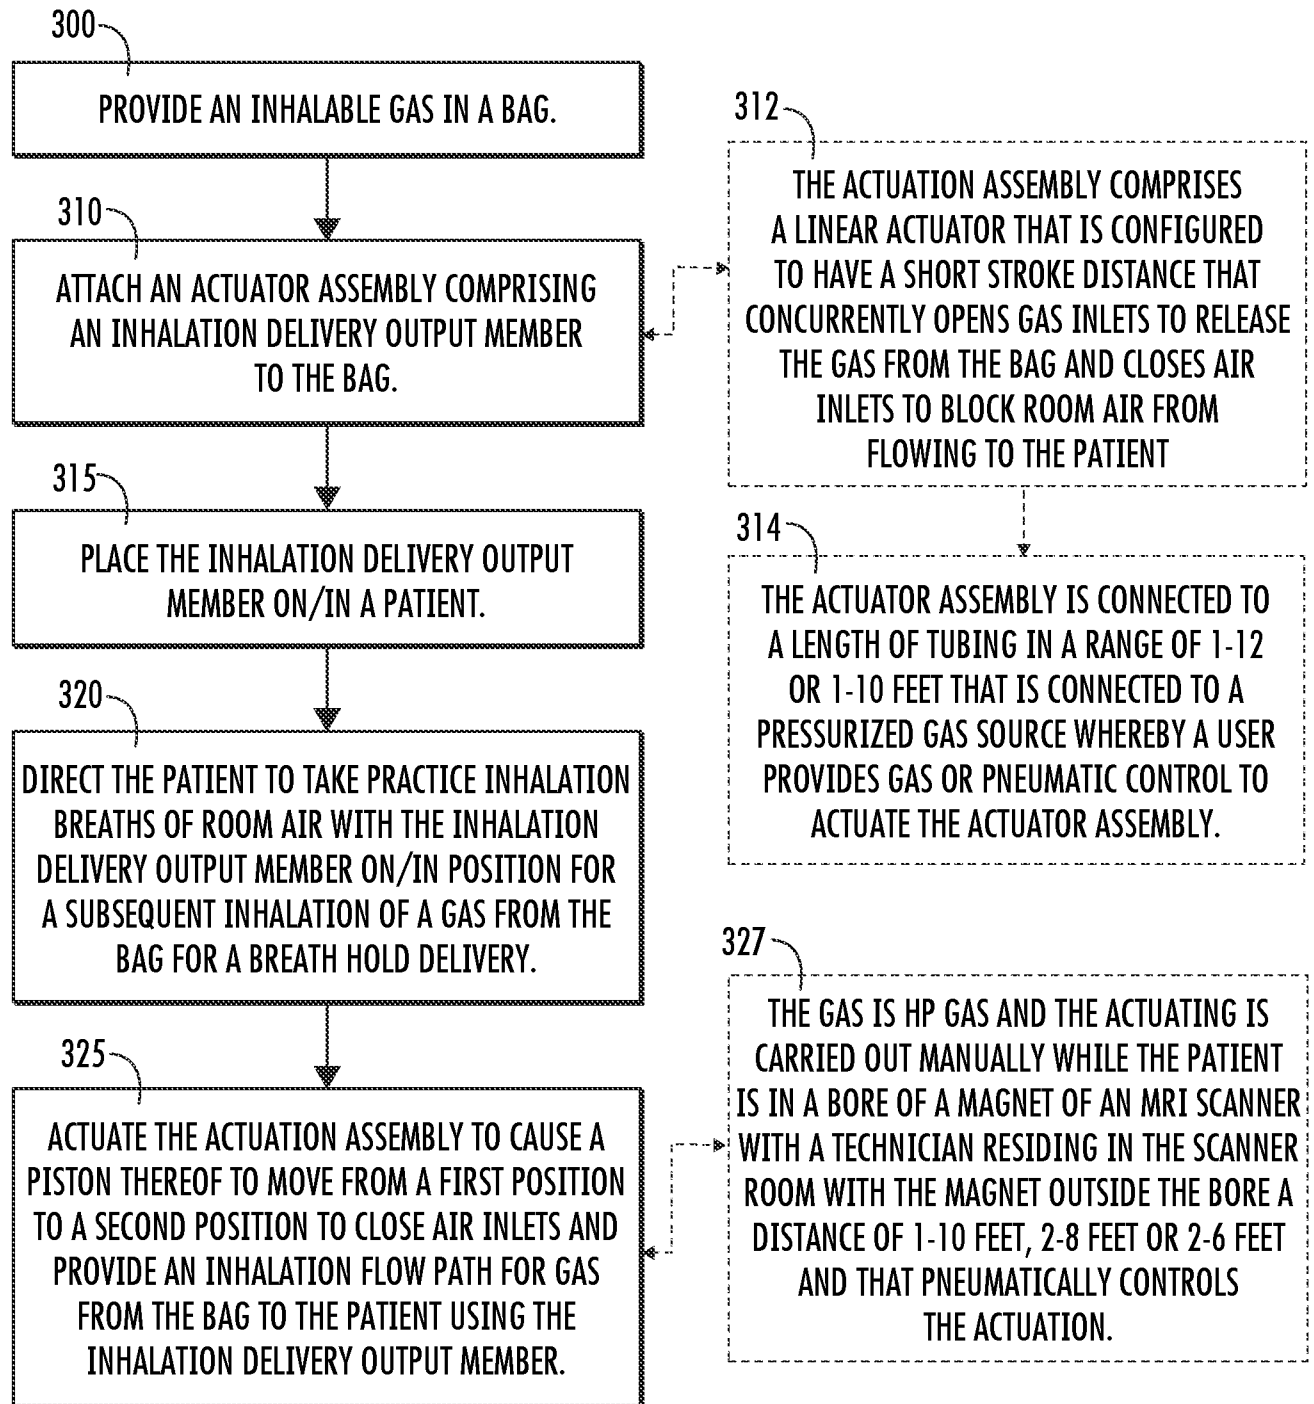


FIG. 26

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US22/25668

A. CLASSIFICATION OF SUBJECT MATTER

IPC - A61M 16/06; A61M 16/00; A62B 7/04 (2022.01)

CPC - A62B 17/04; A61M 16/06; A61M 16/00; A62B 7/04; A61M 16/0605; A61M 16/12

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X --- Y --- A	US 2006/0048777 A1 (BROOKMAN, M) 09 March 2006; Figures 1A, 2b, 3 & 4; paragraphs [0013 & 0033 & 0035 & 0036 & 0038 & 0041 & 0047 & 0048]	1,2,4,19,20 --- 3, 9,11,18 --- 5-8,10,12-17,21-26
Y --- A	US 2006/0201504 A1 (SINGHAL, A ET AL) 14 September 2006; Figure 1; paragraph [0010]	3 --- 1-2,4-26
Y --- A	US 2008/0000471 A1 (BOLAM, K ET AL) 03 January 2008; Paragraphs [0046 & 0047 & 0049 & 0050 & 0057]	9 --- 1-8,10-26
Y --- A	KR 200234760 Y1 (VIRTUALMEDI) 25 September 2001; Figure 2; page 3; paragraphs [0003 & 0006]	11 --- 1-10,12-26
Y --- A	CN 112190809 A (LI JINGJING) 08 January 2021; Figures 1 & 2; paragraphs [0036 & 0048-0050]	18 --- 1-17,19-26
A	US 4,644,947 A (WHITWAM, J ET AL) 24 February 1987; column 3, lines 12-50; column 10, lines 5-20	1-26

☒ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"D" document cited by the applicant in the international application

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

20 June 2022 (20.06.2022)

Date of mailing of the international search report

JUL 25 2022

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450
Facsimile No. 571-273-8300

Authorized officer

Shane Thomas

Telephone No. PCT Helpdesk: 571-272-4300

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US22/25668

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4,378,011 A (WARNCKE, E ET AL) 29 March 1983; Figure 1; column 3, lines 39-50; column 3, lines 65-68; column 4, lines 1-8	1-26