



(51) International Patent Classification:

A61B 17/17 (2006.01) A61B 17/70 (2006.01)
A61B 17/34 (2006.01) A61B 17/88 (2006.01)

(21) International Application Number:

PCT/US2017/062631

(22) International Filing Date:

20 November 2017 (20.11.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/426,027 23 November 2016 (23.11.2016) US

(71) Applicant: ECA MEDICAL INSTRUMENTS [US/US];
1107 Tourmaline Drive, Newbury Park, CA 91320 (US).

(72) Inventors: NINO, John; 1107 Tourmaline Drive, Newbury
Park, CA 91320 (US). IVINSON, David; 1107 Tourmaline
Drive, Newbury Park, CA 91320 (US).

(74) Agent: KRIETZMAN, Mark H.; Washington Square,
1050 Connecticut Avenue, N.W., Suite 1100, Washington,
D.C. (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,
HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP,
KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: ORBITAL TROCAR DEVICE WITH DETACHABLE HANDLE AND ASSOCIATED METHODS

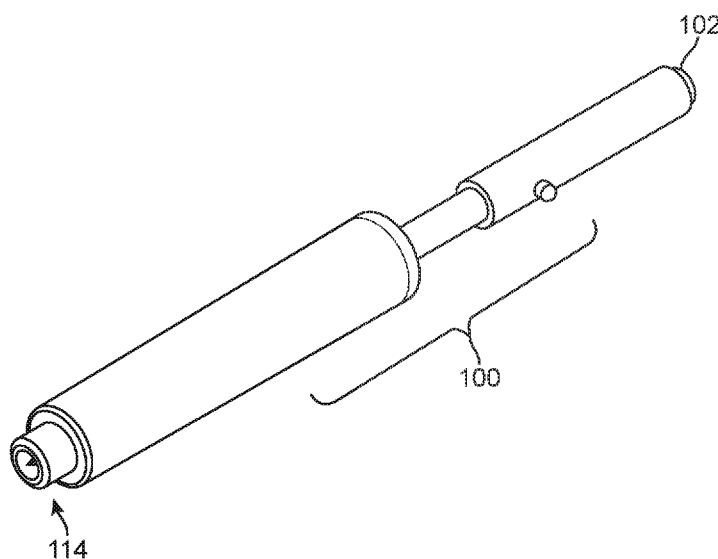


FIG. 2

(57) Abstract: The present disclosure provides methods for forming or enlarging holes in bone tissue and methods for fixing matched medical plates to bodies. The present disclosure also provides for products produced by the methods of the present disclosure and for apparatuses used to perform the methods of the present disclosure.



INTERNATIONAL PATENT APPLICATION**ORBITAL TROCAR DEVICE WITH DETACHABLE HANDLE
AND ASSOCIATED METHODS****PRIORITY**

[0001] This is an International Patent Application claiming priority to United States Provisional Patent Application 62/426,027, filed November 23, 2016, the disclosure of which is incorporated by reference in its entirety.

FIELD OF THE DISCLOSURE

[0002] This disclosure is in the field medical treatment devices and methods. In particular, the disclosure relates to devices and methods for use in medical procedures including devices incorporating cutting tips for creating or enlarging holes in bone.

BACKGROUND

[0003] Orthopedic surgical procedures can require the creation or enlargement of holes in bones. In vertebral surgery, for example, precise alignment of holes is desirable, and in some instances alignment of holes is necessary for proper placement of medical devices, such as matched medical plates.

[0004] Thus, there is a need for medical devices that allow for precise alignment of holes in bone, including alignment of holes for use with other medical devices. The disclosure is directed to these and other important needs.

DISCLOSURE

[0005] The present disclosure provides aspects of trocar insertion systems comprising a driver handle with a driving shaft affixed thereto, a first mating feature on the end of the driving shaft opposite the driver handle, an elongated blade fixture having proximal and distal ends with a second mating feature on the distal end, a spring retention feature located on the elongated blade fixture between the proximal and distal ends, a collar feature located on the elongated blade fixture between the spring retention feature and the distal end, a spring housing cap slidably fitted around the elongated blade fixture between the spring retention feature and the collar feature, a trocar compression spring slidably fitted around the elongated blade fixture

between proximal end and the spring retention feature, a spring housing comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap, wherein the trocar compression spring and spring retention feature are enclosed within the interior volume of the spring housing, wherein the trocar compression spring is configured to be compressed between the spring retention feature and a spring catching feature located at the proximal end of the spring housing, and wherein at least a portion of the elongated blade fixture is slidably disposed within the spring housing with the central longitudinal axes of the elongated blade fixture and the spring housing being coaxially aligned, and wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft and the elongated blade fixture are detachably connected in coaxial alignment.

[0006] The present disclosure provides kits comprising a driver handle with a driving shaft affixed thereto, wherein the driving shaft comprises a first mating feature on the end of the driving shaft opposite the driver handle, and one or more trocar assemblies, wherein each of the one or more trocar assemblies comprises an elongated blade fixture having proximal and distal ends with a second mating feature on the distal end, a spring retention feature located on the elongated blade fixture between the proximal and distal ends, a collar feature located on the elongated blade fixture between the spring retention feature and the distal end, a spring housing cap slidably fitted around the elongated blade fixture between the spring retention feature and the collar feature, a trocar compression spring slidably fitted around the elongated blade fixture between proximal end and the spring retention feature, and a spring housing comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap, wherein the trocar compression spring and spring retention feature are enclosed within the interior volume of the spring housing, wherein the trocar compression spring is configured to be compressed between the spring retention feature and a spring catching feature located at the proximal end of the spring housing, wherein at least a portion of the elongated blade fixture is slidably disposed within the spring housing with the central longitudinal axes of the elongated blade fixture and the spring housing being coaxially aligned, and wherein the first mating feature and second mating features are configured for detachable engagement such that the driving shaft and the elongated blade fixture are detachably connected in coaxial alignment.

[0007] The present disclosure provides aspects of devices comprising an elongated blade fixture having proximal and distal ends with a mating feature on the distal end, a spring retention feature located on the elongated blade fixture between the proximal and distal ends, a collar feature located on the elongated blade fixture between the spring retention feature and the distal end, a spring housing cap slidably fitted around the elongated blade fixture between the

spring retention feature and the collar feature, a trocar compression spring slidably fitted around the elongated blade fixture between proximal end and the spring retention feature, and a spring housing comprising a hollow body configured to slidably fit around the elongated blade fixture and attach to the spring housing cap.

[0008] The present disclosure provides methods of fixing a matched medical plate having one or more apertures to a body, the methods comprising positioning the matched medical plate adjacent to the body such that at least one of the one or more apertures is oriented towards the body, inserting a first trocar insertion system into a first one of the apertures oriented towards the body, wherein the first trocar insertion system comprises a driver handle with a driving shaft affixed thereto, a first mating feature on the end of the driving shaft opposite the driver handle, an elongated blade fixture having proximal and distal ends with a second mating feature on the distal end, a spring retention feature located on the elongated blade fixture between the proximal and distal ends, a collar feature located on the elongated blade fixture between the spring retention feature and the distal end, a spring housing cap slidably fitted around the elongated blade fixture between the spring retention feature and the collar feature, a trocar compression spring slidably fitted around the elongated blade fixture between proximal end and the spring retention feature, a spring housing comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap, wherein the trocar compression spring and spring retention feature are enclosed within the interior volume of the spring housing, wherein the trocar compression spring is configured to be compressed between the spring retention feature and a spring catching feature located at the proximal end of the spring housing, wherein at least a portion of the elongated blade fixture is slidably disposed within the spring housing with the central longitudinal axes of the elongated blade fixture and the spring housing being coaxially aligned, and wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft and the elongated blade fixture are detachably connected in coaxial alignment, the methods further comprising engaging the exterior of the first trocar insertion system spring housing with the first aperture oriented towards the body, applying a force to the driver handle relative to the matched medical plate to move the proximal end of the elongated blade fixture through the first aperture oriented towards the body, fixing the proximal end of the elongated blade fixture to the body, detaching the driving shaft from the elongated blade fixture by disengaging the first mating feature and second mating feature, and removing the driver handle with the driving shaft affixed thereto while leaving the proximal end of the elongated blade fixture fixed to the body.

[0009] The present disclosure provides methods of forming a pilot hole in bone tissue, the methods comprising positioning a matched medical plate having one or more apertures adjacent to the bone tissue such that at least one of the one or more apertures is oriented towards the bone tissue, inserting a first trocar insertion system into a first one of the apertures oriented towards the body, wherein the first trocar insertion system comprises a driver handle with a driving shaft affixed thereto, a first mating feature on the end of the driving shaft opposite the driver handle, an elongated blade fixture having proximal and distal ends with a second mating feature on the distal end, a spring retention feature located on the elongated blade fixture between the proximal and distal ends, a collar feature located on the elongated blade fixture between the spring retention feature and the distal end, a spring housing cap slidably fitted around the elongated blade fixture between the spring retention feature and the collar feature, a trocar compression spring slidably fitted around the elongated blade fixture between proximal end and the spring retention feature, a spring housing comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap, wherein the trocar compression spring and spring retention feature are enclosed within the interior volume of the spring housing, wherein the trocar compression spring is configured to be compressed between the spring retention feature and a spring catching feature located at the proximal end of the spring housing, wherein at least a portion of the elongated blade fixture is slidably disposed within the spring housing with the central longitudinal axes of the elongated blade fixture and the spring housing being coaxially aligned, and wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft and the elongated blade fixture are detachably connected in coaxial alignment, the methods further comprising engaging the exterior of the trocar insertion system spring housing with the aperture oriented towards the body, applying a force to the driver handle relative to the matched medical plate to move the proximal end of the elongated blade fixture through the aperture oriented towards the body, forming the pilot hole in the bone tissue with the proximal end of the elongated blade fixture, and removing the trocar insertion system from the matched medical plate aperture.

[0010] The present disclosure provides methods of forming a pilot hole in bone tissue, the methods including positioning a matched medical plate having one or more apertures having first guide of the toroidal interface on one side and a second guide of the toroidal interface on the opposite side; aligning a trocar insertion system having a drive handle and an elongated blade, with a spring in a movable spring housing having a toroid forming an extended curved annular wall surface at its proximal end with a toroidal covering the blade in an unactuated position; engaging the toroidal interface with the toroid at the first guide of the toroidal interface

of the aperture oriented towards the body; adjusting the cone of operation of the trocar insertion system via movement within the cone of operation; applying force to the driver handle relative to the matched medical plate to move the proximal end of the elongated blade fixture and at least a portion of the shaft through the toroidal interface and aperture; forming the pilot hole in the bone tissue with the proximal end of the elongated blade fixture within the limits of a control cone of operation ; and, removing the trocar insertion system from the matched medical plate aperture.

[0011] The general description and the following detailed description are exemplary and explanatory only and are not restrictive of the disclosure, as defined in the appended claims. Other aspects of the present disclosure will be apparent to those skilled in the art in view of the detailed description of the disclosure as provided herein.

DRAWINGS

[0012] The summary, as well as the following detailed description, is further understood when read in conjunction with the appended drawings. For the purpose of illustrating the disclosure, there are shown in the drawings exemplary implementations of the disclosure; however, the disclosure is not limited to the specific methods, compositions, and devices disclosed. In addition, the drawings are not necessarily drawn to scale. In the drawings:

- [0013] FIG 1 illustrates aspects of a trocar insertion device;
- [0014] FIG 2 illustrates aspects of a portion of a trocar insertion device;
- [0015] FIG 3 illustrates an assembly view of aspects of a trocar insertion device;
- [0016] FIG 4 illustrates an assembly view of aspects of a trocar insertion device;
- [0017] FIGS 5A-5C illustrate an assembly view of aspects of catches and latches for a trocar device;
- [0018] FIGS 6A-D illustrate cut-away views of aspects of a trocar insertion devices;
- [0019] FIGS 7A-8E illustrate aspects of trocar insertion systems;
- [0020] FIG 9 illustrates a trocar insertion system kit; and
- [0021] FIG 10A-10B illustrate a cut-away view of a portion of a trocar insertion devices.

FURTHER DISCLOSURE

[0022] The present disclosure may be understood more readily by reference to the following detailed description taken in connection with the accompanying figures and examples, which form a part of this disclosure. It is to be understood that this disclosure is not limited to

the specific devices, methods, applications, conditions or parameters described and/or shown herein, and that the terminology used herein is for the purpose of describing particular exemplars by way of example only and is not intended to be limiting of the claimed disclosure. Also, as used in the specification including the appended claims, the singular forms “a,” “an,” and “the” include the plural, and reference to a particular numerical value includes at least that particular value, unless the context clearly dictates otherwise. The term “plurality”, as used herein, means more than one. When a range of values is expressed, another exemplar includes from the one particular value and/or to the other particular value. Similarly, when values are expressed as approximations, by use of the antecedent “about,” it will be understood that the particular value forms another exemplar. All ranges are inclusive and combinable.

[0023] It is to be appreciated that certain features of the disclosure which are, for clarity, described herein in the context of separate exemplar, may also be provided in combination in a single exemplary implementation. Conversely, various features of the disclosure that are, for brevity, described in the context of a single exemplary implementation, may also be provided separately or in any subcombination. Further, reference to values stated in ranges include each and every value within that range.

[0024] In one aspect, the present disclosure provides trocar insertion systems. As depicted in FIG 1, the trocar insertion system may comprise a trocar assembly 100, which can be detachably connected to a handle assembly 200 using mating features provided thereon. Exemplary implementations of the handle assemblies 200 and trocar assemblies 100 are depicted in FIGs 3 and 4. In some exemplars, the trocar insertion systems may comprise a driver handle (202) with a driving shaft (206) affixed thereto, a first mating feature on the proximal end (220) of the driving shaft (206) opposite the driver handle (202), an elongated blade fixture (112) having a proximal end (114) and a distal end (102). Between the proximal end (114) and the distal end (102) is an elongated region of shaft (115). A spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends (114/102), a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the proximal end (102), a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116), a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between the proximal end (102) and the spring retention feature (119), a spring housing (106) comprising a hollow body with proximal and distal ends 106'/106'', wherein the distal end 106'' is fixedly attached to the spring housing cap (110), the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing

(106), the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), and at least a portion of the elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned. The first mating feature and second mating feature can be detachably engaged such that the driving shaft (206) and the elongated blade fixture (112) are detachably connected in coaxial alignment. The spring retention feature (119) may comprise any feature present on the elongated blade fixture (112) that is capable of retaining one end of a compression spring in a fixed position as the spring is compressed against the feature. In some instances the spring retention feature (119) comprises a retaining ring or clip (120) that is positioned within a slot or groove (118) on the elongated blade fixture (112). In some instances, self-locking retaining rings can be used without a slot or groove on the shaft of the elongated blade fixture. Driver handle (202) can be a suitable shape to be gripped in a human hand. In some instances, the driver handle can be a welled handle suitable for medical waste collection during use, as described in U.S. Patent Application No. 13/983,535. Driving shaft (206) can be affixed within driver handle (202) such that rotation of the driver handle (202) creates rotation of the driver shaft (206) with no slippage. In some instances, the distal end (208) of the driving shaft (206) is affixed within an aperture (204) of driver handle (202).

[0025] Spring housing (106) can be formed with any suitable external profile. A cylindrical cross-section is suitable for some applications, while other polygonal, star-shaped, keyed, flanged, or grooved cross-sections may be also suitable in other exemplary implementations. The proximal end (114) of the elongated blade fixture (112) can be located at the center of the cross-section of spring housing (106) or at other positions as desired, provided the proximal end (114) can slide through the end of spring housing (106) during operation.

[0026] The trocar assembly (100) and handle assembly (200) can be detachably connected using any suitable pair of first and second mating features that allow for connection and disconnection with coaxial alignment between the driving shaft (206) and elongated blade fixture (112). In some instances, the first mating feature and second mating feature comprise a pair of helical threads that can detachably engage together. In some instances, the first and second mating features comprise a ball detent mechanism arrangement wherein one of the driving shaft (206) and elongated blade fixture (112) can be received within the other such that a spring-loaded ball falls partially into an aperture in order to detachably connect the driving shaft (206) and elongated blade fixture (112). In some instances, the second mating feature comprises

a protruding part and the first mating feature comprises a depression adapted to receive the protruding part in a snap joint configuration. Trocar assembly (100) can include an area suitable for grasping by a user, such as the area of the elongated blade fixture (112) between trocar locator pin (124) and spring housing cap (110). The grasping area can be configured for enhanced grip by methods known in the art including incorporating coated or textured surfaces, depressions, grooves, or cut-outs that allow for improved grasping and controlled twisting of the trocar assembly (100) as it is engaged with the handle assembly (200), provided the features do not interfere with the slidable engagement of the spring housing cap (110) and spring housing (106) around the elongated blade fixture (112) as trocar compression spring (108) is compressed.

[0027] In some exemplars, trocar assembly (100) and handle assembly (200) can be detachably connected with spring-loaded configurations. In some exemplars, the driving shaft (206) comprises a hollow tube with a first aperture (210) and a second aperture (212) through the walls of the hollow tube on opposite sides of the central longitudinal axis of the hollow tube, a third aperture (214) through the wall of the hollow tube in a position between the location of the first and second apertures and the proximal end of the hollow tube, and a groove (222) through the wall of the hollow tube at the proximal end. In the spring-loaded configurations, the trocar insertion systems further comprise a spring stop pin (216) fixed within the first and second apertures (210/212) and passing through the central longitudinal axis of the hollow tube, a control pin (218) fixed within the third aperture (214) and partially extending into the interior volume of the hollow tube, and a spring pressure pin (226) comprising a cylinder configured to slide within the interior of the hollow tube, positioned within the interior volume of the hollow tube with the longitudinal axis of the cylinder aligned with the hollow tube longitudinal axis. In the spring-loaded configurations the spring pressure pin (226) can have a reduced diameter in a portion of the middle of the side walls, the reduction in diameter can be at least as large as the portion of the control pin that partially extends into the interior volume of the hollow tube, and the spring pressure pin (226) can be positioned such that the portion of the control pin that partially extends into the interior volume of the hollow tube is slidably contained within the volume of the reduced diameter portion of the spring pressure pin (226) between the two non-reduced-diameter end regions of the spring pressure pin (226). In these instances, a handle compression spring (224) can be positioned within the interior volume of the hollow tube between the spring stop pin and the spring pressure pin (226), and a fourth aperture can be located on the elongated blade fixture (112) between the collar feature (116) and the distal end, the distal end of the elongated blade fixture can be configured to slidably fit within the interior of the proximal end of the hollow tube, a trocar locator pin (124) can be fixed within the fourth

aperture (122) and partially extending outward from the elongated blade fixture (112) surface. For connection of the trocar assembly (100) to the handle assembly (200), the driving shaft (206) and elongated blade fixture (112) can be detachably connected by the detachable engagement of the trocar locator pin (124) within the groove (222) of the driving shaft (206), and the handle compression spring (224) can be at least partially compressed by the spring pressure pin (226), which can be slidably contained between the distal end of the elongated blade fixture (112) and the handle compression spring (224). Aspects of some exemplars of such engagement are depicted in FIGs 6A-6D.

[0028] In some exemplary implementations of the trocar insertion systems the exterior of the spring housing (106) can be configured to engage with an aperture (302) of a matched medical plate (300) such that the spring housing (106) is retained within the aperture (302) and the proximal end of the elongated blade fixture (112) passes through the aperture (302) when a force is applied to the distal end of the elongated blade fixture (112) relative to the matched medical plate (300). FIGs 7A and 8A depict one implementation of such a system. FIG 6A depicts a cut-away view of an implementation of a trocar insertion system when the trocar compression spring (108) is compressed by the force against a matched medical plate (300), having an aperture 302 which is not shown in FIG 6A, and the proximal end (114) of the elongated blade fixture (112) is exposed. In one aspect, the present disclosure provides a trocar insertion systems as depicted in FIG 6D, the trocar insertion system comprises a trocar assembly (101), which can be detachably connected to a handle assembly 200 using mating features provided thereon. The exterior of the spring housing (106) comprises a cylinder with a tapered diameter proximal end (109) having at its end 109' a toroid (128) forming an extended curved annular wall surface (129).

[0029] FIGs 7B and 8B depict aspects of implementations of a trocar insertion system with toroid end to allow the user to position a blade deployment in a cone of operation. FIGs 7B and 6D depicts a view of an implementation of a trocar insertion system when the trocar compression spring is in an un-actuated state whereby the spring housing covers the elongated blade. When actuated via compression by the force against a matched medical plate (350), as is shown in FIG 8B, and the proximal end (114) of the elongated blade fixture is exposed.

[0030] FIG 8B further illustrates aspects of a trocar with spring housing with matched medical plate 350 and toroidal interface 400. A matched medical plate refers to a medical plate that matches the distal end of the spring housing (106) with tapered diameter proximal end (109). In this exemplar the toroid (128) portion at the end (109') forms an extended curved annular wall surface (129). The annular wall surface mates reversible with the curved guide (401) which

provides for movement of the device and the exposed proximal end (114) which protrudes through the matched medical plate (350) thereby allowing for operation, resection and tool usage at angles other than perpendicular to the matched medical plate. Those of ordinary skill in the art will recognize that the toroid (128) may be positioned at a non-tapered distal end if the spring housing does not include a tapered end and such an arrangement is within the scope of this disclosure.

[0031] FIGs 8C-8E illustrates aspects of a trocar with spring housing with matched medical plate 355 and toroidal interface 400. In this exemplar the toroid (128) portion again covers the end (109') forming an extended curved annular wall surface (129) and it mates reversibly with the first guide (402) of the toroidal interface (400) which provides for movement of the device and the exposed proximal end (114) in the first guide (402) which is placed away from a body being operated on. During operation the elongated shaft (115) of an exposed proximal end (114) of the elongated blade fixture (112) is limited to movement within the second guide (404). Which faces the body being operated on, of the toroidal interface. The maximum area of operation for the exposed proximal end (114) is set by a control cone of operation (406) in the toroidal interface which is defined by the angle theta " θ " of the second guide (404). FIG 8C illustrates operation when the position of the shaft (115) is at theta " θ " of about 10 degrees. FIG 8D illustrates operation when the position of the shaft (115) is at theta " θ " of about 20 degrees. FIG 8E illustrates operation when the position of the shaft (115) is at theta " θ " of about 30 degrees.

[0032] In some exemplary implementations of the trocar insertion systems the exterior of the spring housing (106) comprises a cylinder with a tapered diameter proximal end (109) near the proximal end of the elongated blade fixture (112). One such exemplar is depicted in FIG 10.

[0033] The proximal end of the elongated blade fixture can be any shape desired by a user. Suitable shapes can include drivers, screwdrivers, wrenches, cutters, probes, retractors, resectors, awls, prods, or other shapes useful for surgical applications. In some instances of the trocar insertion systems the proximal end of the elongated blade fixture (112) comprises a shape suitable for anchoring into body tissue. In some instances the trocar insertion systems the proximal end of the elongated blade fixture (112) comprises a bone awl. In some instances the trocar insertion systems the proximal end of the elongated blade fixture (112) comprises a shape suitable for forming pilot holes in bone. In some instances the trocar insertion systems the elongated blade fixture (112) further comprises a lumen. In some instances a portion of the elongated blade fixture shaft comprises a cutting or filing zone.

[0034] FIGs 5A-5C depict groove (222) of the driving shaft (206) that is included in some instances of the trocar insertion systems. During detachable engagement, trocar locator pin (124) slides into groove (222) and is held in place in a resting position (223) of the groove by the force exerted by the handle compression spring (224) when the spring is in a compressed state, as depicted in FIGs 6A and 6B. Groove (222) can be formed in a variety of shapes, provided that the groove (222) allows for insertion of trocar locator pin (124) and provides a resting position (223). In some exemplars, the force applied to the elongated blade fixture (112) during methods of use will compress the handle compression spring (224) such that the trocar locator pin (124) is driven into a working position (225). Working position (225) can be provided in various positions of the groove (222) and preferably allows for the elongated blade fixture (112) to be rotated with the rotation of the driver handle (202) and driving shaft (206). In some exemplars, the force applied to the elongated blade fixture (112) during methods of use will not compress the handle compression spring (224), and the elongated blade fixture (112) can be rotated with the rotation of the driver handle (202) and driving shaft (206) with trocar locator pin (124) remaining in the resting position (223).

[0035] The present disclosure also provides kits comprising one or more trocar assemblies (100) and one or more handle assemblies (200). In some exemplary implementations the kits comprise a driver handle (202) with a driving shaft (206) affixed thereto, wherein the driving shaft (206) comprises a first mating feature on the end of the driving shaft (206) opposite the driver handle (202) and one or more trocar assemblies (100). In some instances the one or more trocar assemblies 100 comprise an elongated blade fixture (112) having proximal and distal ends with a second mating feature on the distal end, a spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends, a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end, a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116), a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119), a spring housing (106) comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap (110), wherein the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106), wherein the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), and wherein at least a portion of the elongated blade fixture (112) is slidably disposed within the

spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned, and wherein the first mating feature and second mating features are configured for detachable engagement such that the driving shaft (206) and the elongated blade fixture (112) are detachably connected in coaxial alignment. In some instances, kits can further comprise a tool configured for connecting a trocar assembly to the driving shaft (206), detaching a trocar assembly from the driving shaft (206), or both. One exemplar of a kit is depicted in FIG 9, which can include one or more trocar assemblies 100/101, one or more handle assemblies 200, one or more fixed drivers 400, one or more torque-limiting drivers 500, one or more matched medical plates 300/350/355, and one or more plate holding forceps 600 contained in a sterile-packed instrument tray 700. In some exemplary implementations, as many of the components in the kits are designed for single-use and are disposable. In some instances, the entire kit is compatible with medical-grade sterilization procedures, including but not limited to ethylene oxide (EtO) and gamma ray sterilization.

[0036] The present disclosure also provides devices comprising an elongated blade fixture (112) having proximal and distal ends with a mating feature on the distal end, a spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends, a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end, a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116), a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119), and a spring housing (106) comprising a hollow body configured to slidably fit around the elongated blade fixture (112) and attach to the spring housing cap (110). In some instances, the devices may comprise a spring housing (106) that further comprises proximal and distal ends, wherein the distal end is attached to the spring housing cap (110), the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106), the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), and at least a portion of the elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned. In some instances the exterior of the spring housing (106) can be configured to engage with an aperture (302) of a matched medical plate (300) or the toroidal interface (400) in matched medical plates (350/355) such that the spring housing (106) is retained within the aperture (302) and the proximal end of the elongated blade fixture (112)

passes through the aperture (302) when a force is applied to the distal end of the elongated blade fixture (112) relative to the matched medical plate (350/355). In some instances of the devices the exterior of the spring housing (106) comprises a cylinder with a tapered diameter at its proximal end (109). The proximal end of the elongated blade fixture can be any shape desired by a user. Suitable shapes can include drivers, screwdrivers, wrenches, cutters, probes, retractors, resectors, awls, prods, or other shapes useful for surgical applications. In some instances of the devices the proximal end of the elongated blade fixture (112) comprises a shape suitable for anchoring into body tissue. In some instances of the trocar insertion systems the proximal end of the elongated blade fixture (112) comprises a bone awl. In some instances of the devices the proximal end of the elongated blade fixture (112) comprises a shape suitable for forming pilot holes in bone. In some instances of the devices the elongated blade fixture (112) further comprises a lumen. In some instances of the devices a portion of the elongated blade fixture shaft comprises a cutting or filing zone.

[0037] The present disclosure provides methods of using one or more trocar assemblies (100) and one or more handle assemblies (200) disclosed herein. In some aspects, the methods of use include methods of fixing matched medical plates (300/350/355) to a body. In other aspects, the methods of use include methods of forming pilot holes in bone tissue. In some exemplary implementations the methods of forming pilot holes in bone tissue can include the use of matched medical plates (300/350/355), and can be used to form pilot holes aligned with apertures (302) of the matched medical plates (300/350/355).

[0038] The present disclosure provides methods of fixing a matched medical plate (300) having one or more apertures (302) to a body, the methods comprising positioning the matched medical plate (300/3510/355) adjacent to the body such that at least one of the one or more apertures (302) is oriented towards the body, inserting a first trocar insertion system into a first one of the apertures (302) oriented towards the body, wherein the first trocar insertion system comprises (i) a driver handle (202) with a driving shaft (206) affixed thereto, (ii) a first mating feature on the end of the driving shaft (206) opposite the driver handle (202), (iii) an elongated blade fixture (112) having proximal and distal ends with a second mating feature on the distal end, (iv) a spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends, (v) a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end, (vi) a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116), (vi) a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature

(119), and (vii) a spring housing (106) comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap (110), wherein the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106), wherein the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), wherein at least a portion of the elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned, and wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft (206) and the elongated blade fixture (112) are detachably connected in coaxial alignment, the method further comprising engaging the exterior of the first trocar insertion system spring housing (106) with the first aperture (302) oriented towards the body, applying a force to the driver handle (202) relative to the matched medical plate (300/350/355) to move the proximal end of the elongated blade fixture (112) through the first aperture (302) oriented towards the body, fixing the proximal end of the elongated blade fixture (112) to the body, detaching the driving shaft (206) from the elongated blade fixture (112) by disengaging the first mating feature and second mating feature, and removing the driver handle (202) with the driving shaft (206) affixed thereto while leaving the proximal end of the elongated blade fixture (112) fixed to the body. In some exemplary implementations, the methods further comprise positioning the matched medical plate (300) adjacent to the body such that a second aperture of the one or more apertures (302) is oriented towards the body, and the methods further comprise engaging the first mating feature on the end of the driving shaft (206) with a third mating feature of a trocar device to form a second trocar insertion system, wherein the trocar device comprises (i) an elongated blade fixture (112) having proximal and distal ends with a third mating feature on the distal end, (ii) a spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends, (iii) a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end, (iv) a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116), (v) a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119), and (vi) a spring housing (106) comprising a hollow body configured to slidably fit around the elongated blade fixture (112) and attach to the spring housing cap (110), the methods further comprising inserting the second trocar insertion system into the second aperture oriented towards the body, engaging the exterior of the spring housing

(106) of the second trocar insertion system with the aperture, applying a force to the driver handle (202) relative to the matched medical plate (300) to move the proximal end of the elongated blade fixture (112) of the second trocar insertion system through the aperture, fixing the proximal end of the elongated blade fixture (112) of the second trocar insertion system to the body, detaching the driving shaft (206) from the trocar device by disengaging the first mating feature and the third mating feature, and removing the driver handle (202) with the driving shaft (206) affixed thereto while leaving the proximal end of the elongated blade fixture (112) of the trocar device fixed to the body.

[0039] The present disclosure provides methods of forming a pilot hole in bone tissue, the methods comprising positioning a matched medical plate (300) having one or more apertures (302) adjacent to the bone tissue such that at least one of the one or more apertures (302) is oriented towards the bone tissue, inserting a trocar insertion system into one of the apertures (302) oriented towards the body, wherein the trocar insertion system comprises (i) a driver handle (202) with a driving shaft (206) affixed thereto, (ii) a first mating feature on the end of the driving shaft (206) opposite the driver handle (202), (iii) an elongated blade fixture (112) having proximal and distal ends with a second mating feature on the distal end, (iv) a spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends, (v) a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end, (vi) a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116), (vii) a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119), and (viii) a spring housing (106) comprising a hollow body with proximal and distal ends, wherein the distal end is fixedly attached to the spring housing cap (110), wherein the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106), wherein the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), wherein at least a portion of the elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned, and wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft (206) and the elongated blade fixture (112) are detachably connected in coaxial alignment, the methods further comprising engaging the exterior of the trocar insertion system spring housing (106) with the aperture (302) oriented towards the body, applying a force to the driver handle

(202) relative to the matched medical plate (300/350/355) to move the proximal end of the elongated blade fixture (112) through the aperture (302) oriented towards the body, forming the pilot hole in the bone tissue with the proximal end of the elongated blade fixture (112), and removing the trocar insertion system from the matched medical plate (300) aperture (302).

[0040] In any of the above exemplary implementations when utilizing a matched medical plate (350/355) with a toroidal interface (400) the elongated blade fixture (112) can be utilized along any portion of the control cone of operation (406). Accordingly, the angle theta “ θ ” which defines the maximum cone of operation may be preset. In some instance the kit may contain several matched medical plate (which may be marked to show their aspects of cones of operation) and some maybe preset at theta “ θ ” less or greater than others thereby providing the user a choice on who to limit the cone of operation.

[0041] Those of ordinary skill in the art will appreciate that a variety of materials can be used in the manufacturing of the components in the devices and systems disclosed herein. Any suitable structure and/or material can be used for the various features described herein, and a skilled artisan will be able to select an appropriate structures and materials based on various considerations, including the intended use of the systems disclosed herein, the intended arena within which they will be used, the sterilization parameters and/or sterilants to which they are intended to be exposed, and the equipment and/or accessories with which they are intended to be used, among other considerations. Conventional polymeric, metal-polymer composites, ceramics, and metal materials are suitable for use in the various components. Examples of suitable polymer materials include polyetherimide (Ultem®), polyacrylamide (Ixef®), and other medical grade engineered polymeric (plastic) materials, extruded, injection-molded, or otherwise formed into the desired structures. In some instances, the number of polymer components is maximized in order to provide systems most suitable as single-use disposables. For uses requiring stronger systems, particular components such as the elongated blade fixture (112) and driving shaft (206) can be machined or ground stainless steel, including 302, 316, 416, 420, 440c, 455, 465, 17-4, 17-7, and other grades. In some instances the spring housing (106), trocar locator pin (124), spring stop pin (216), control pin (218), and spring pressure pin (226) can be made from stainless steel, including 302, 316, 416, 420, 440c, 455, 465, 17-4, 17-7, and other grades. Trocar compression spring (108) and handle compression spring (224) can be stainless steel or medical grade engineered polymer, provided they are selected to provide suitable spring rates and cycle life for the desired use. Matched medical plates (300/350/355) can be radiopaque in some instances. Materials hereinafter discovered and/or developed that are determined to be

suitable for use in the features and elements described herein would also be considered acceptable.

[0042] When ranges are used herein for physical properties, such as molecular weight, or chemical properties, such as chemical formulae, all combinations, and subcombinations of ranges for specific exemplar therein are intended to be included.

[0043] The disclosures of each patent, patent application, and publication cited or described in this document are hereby incorporated herein by reference, in its entirety.

[0044] Those of ordinary skill in the art will appreciate that numerous changes and modifications can be made to the exemplars of the disclosure and that such changes and modifications can be made without departing from the spirit of the disclosure. It is, therefore, intended that the appended claims cover all such equivalent variations as fall within the true spirit and scope of the disclosure.

What is Claimed:

1. A spring housing mated to a trocar assembly comprising:
a hollow body (106) with proximal end (106'') and distal end (106');
wherein
the distal end is fixedly attached to a spring housing cap (110),
a trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106),
the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end (109) of the spring housing (106), and;
at least a portion of an elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned.
2. The spring housing assembly of claim 1 further comprising:
a driver handle (202) with an at least partially hollow driving shaft (206) affixed thereto;
a first mating feature on an open proximal end (220) of the driving shaft (206) opposite the driver handle (202); and,
wherein the hollow body fits movably into the proximal end.
3. The spring housing assembly of claim 2 further comprising:
the elongated blade fixture (112) has a proximal and distal ends with a second mating feature on its distal end; and,
the spring retention feature (119) is located on the elongated blade fixture (112) between the proximal and distal ends.
4. The spring housing assembly of claim 3 further comprising:
a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end; and,
a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116).

5. The spring housing assembly of claim 3 or 4 further comprising a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119).
6. The spring housing assembly of claim 1 further comprising a toroid (128) at the proximal end of the hollow body (106) forming an extended curved annular wall surface (129).
7. A method of forming a pilot hole in bone tissue, the method comprising:
 - positioning a matched medical plate (350) having one or more apertures (302) with curved guides (401) adjacent to the bone tissue such that at least one of the one or more apertures (302) is oriented towards the bone tissue;
 - inserting a trocar insertion system into one of the apertures (302) oriented towards the body;
 - a spring housing (106) having a hollow body with a proximal end and a distal end;
 - wherein the distal end is fixedly attached to the spring housing cap (110), the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106), the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), at least a portion of the elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned; wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft (206) and the elongated blade fixture (112) are detachably connected in coaxial alignment;
 - engaging the proximal end (109) of the spring housing (106) with the aperture (302) oriented towards the body;
 - applying a force to the driver handle (202) relative to the matched medical plate (350) to move the proximal end of the elongated blade fixture (112) through the aperture (302) oriented towards the body;
 - forming the pilot hole in the bone tissue with the proximal end of the elongated blade fixture (112); and,
 - removing the trocar insertion system from the matched medical plate (350) aperture (302).

8. The method of forming a pilot hole of claim 7 further comprising placing the spring housing within the open proximal end (220) of a driving shaft attached to a driver handle (202).

9. The method of forming a pilot hole of claim 8 wherein the elongated blade fixture (112) has a proximal and distal ends with a second mating feature on its distal end; and, the spring retention feature (119) is located on the elongated blade fixture (112) between the proximal and distal ends.

10. The method of forming a pilot hole of claim 9 wherein a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end; and, a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116).

12. The method of forming a pilot hole of claim 11 wherein a trocar compression spring (108) is slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119).

13. A method of forming a pilot hole in bone tissue, the method comprising:
positioning a matched medical plate (355) having one or more apertures (302) having first guides on one side and a second guide,
inserting a trocar insertion system into one of the apertures (302) oriented towards the body, wherein the trocar insertion system includes an interface (400) which comprises;
a driver handle (202) with a driving shaft (206) affixed thereto;
a first mating feature on the end of the driving shaft (206) opposite the driver handle (202);
a shaft (115) with an elongated blade fixture (112) at one end having proximal and distal ends with a second mating feature on the distal end;
a spring retention feature (119) located on the elongated blade fixture (112) between the proximal and distal ends;
a collar feature (116) located on the elongated blade fixture (112) between the spring retention feature (119) and the distal end;
a spring housing cap (110) slidably fitted around the elongated blade fixture (112) between the spring retention feature (119) and the collar feature (116);

a trocar compression spring (108) slidably fitted around the elongated blade fixture (112) between proximal end and the spring retention feature (119);

a spring housing (106) comprising a hollow body with a proximal end and distal end, wherein the distal end is fixedly attached to the spring housing cap (110), the trocar compression spring (108) and spring retention feature (119) are enclosed within the interior volume of the spring housing (106),

the trocar compression spring (108) is configured to be compressed between the spring retention feature (119) and a spring catching feature (107) located at the proximal end of the spring housing (106), and,

at least a portion of the elongated blade fixture (112) is slidably disposed within the spring housing (106) with the central longitudinal axes of the elongated blade fixture (112) and the spring housing (106) being coaxially aligned,

wherein the first mating feature and second mating feature are detachably engaged such that the driving shaft (206) and the elongated blade fixture (112) are detachably connected in coaxial alignment;

engaging the aperture with the trocar insertion system spring housing (106) with the first guide of the aperture (302) oriented towards the body;

applying a force to the driver handle (202) relative to the matched medical plate (355) to move the proximal end of the elongated blade fixture (112) and at least a portion of the shaft (115) through the aperture (302) oriented towards the body;

forming the pilot hole in the bone tissue with the proximal end of the elongated blade fixture (112).

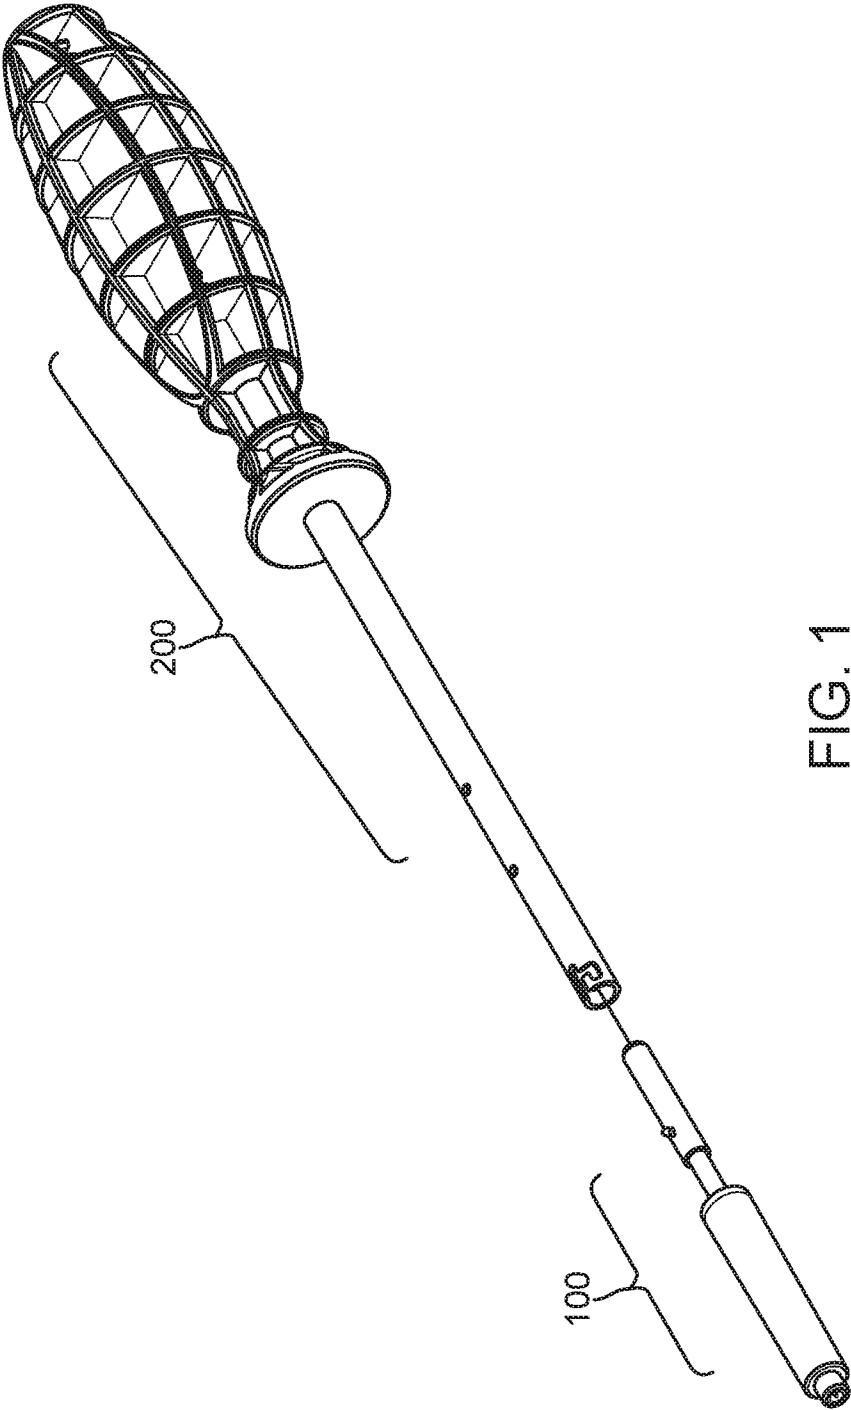


FIG. 1

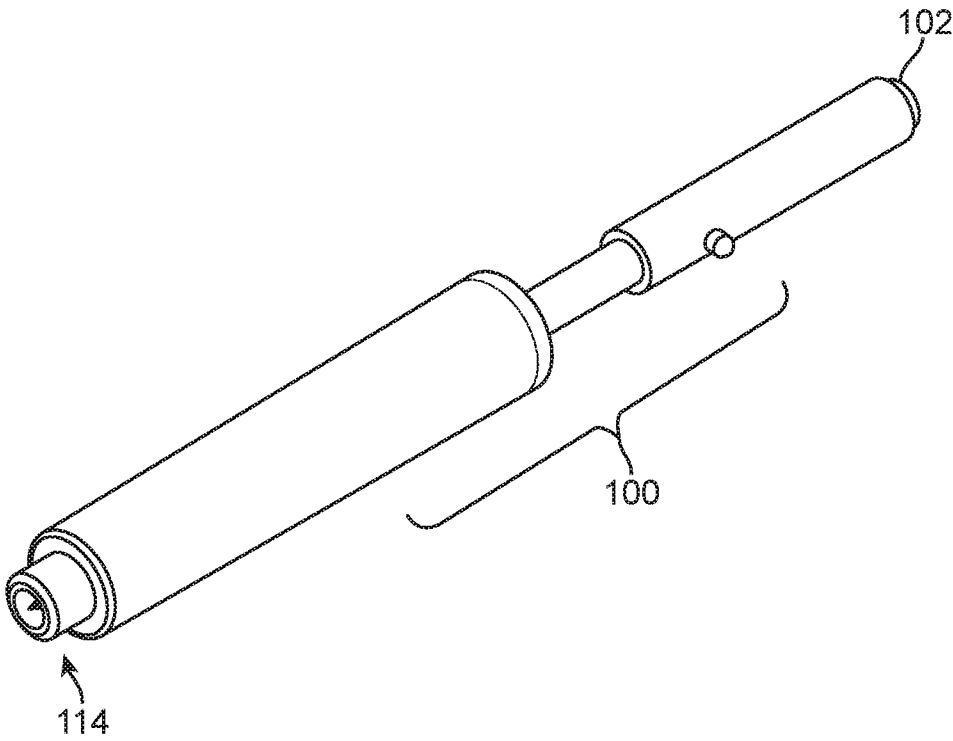


FIG. 2

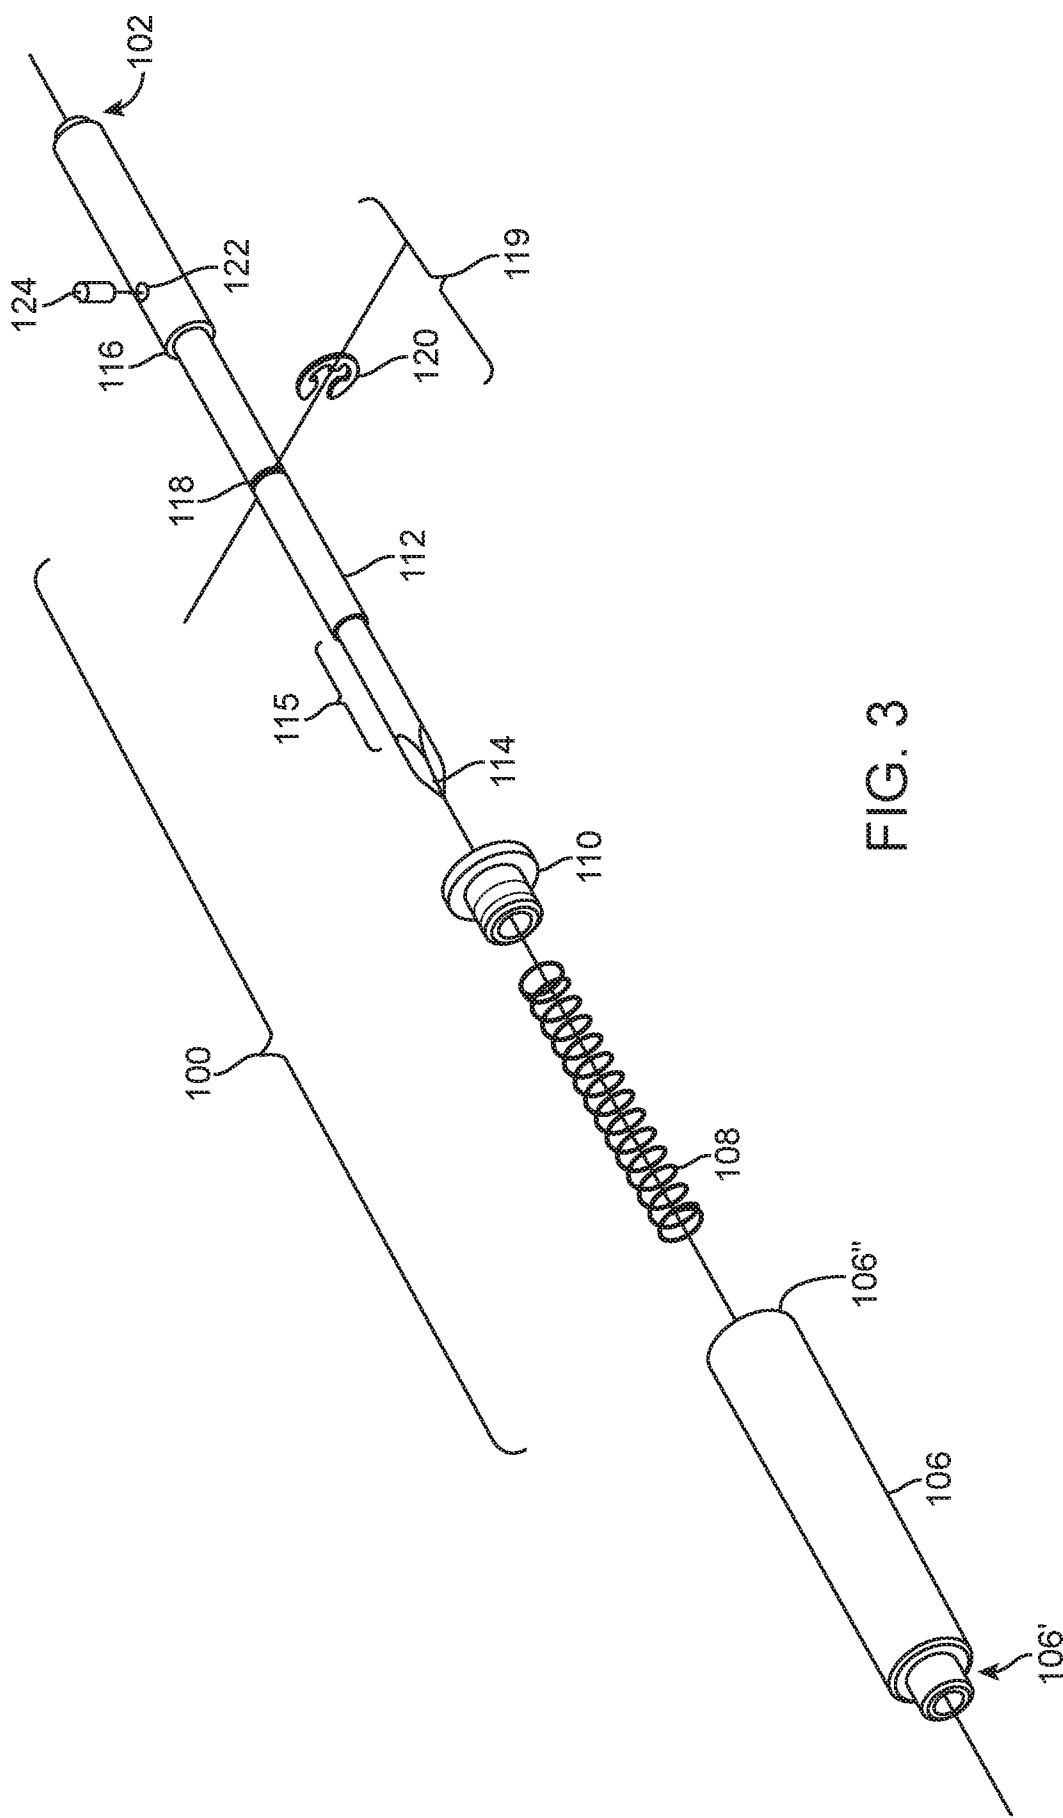


FIG. 3

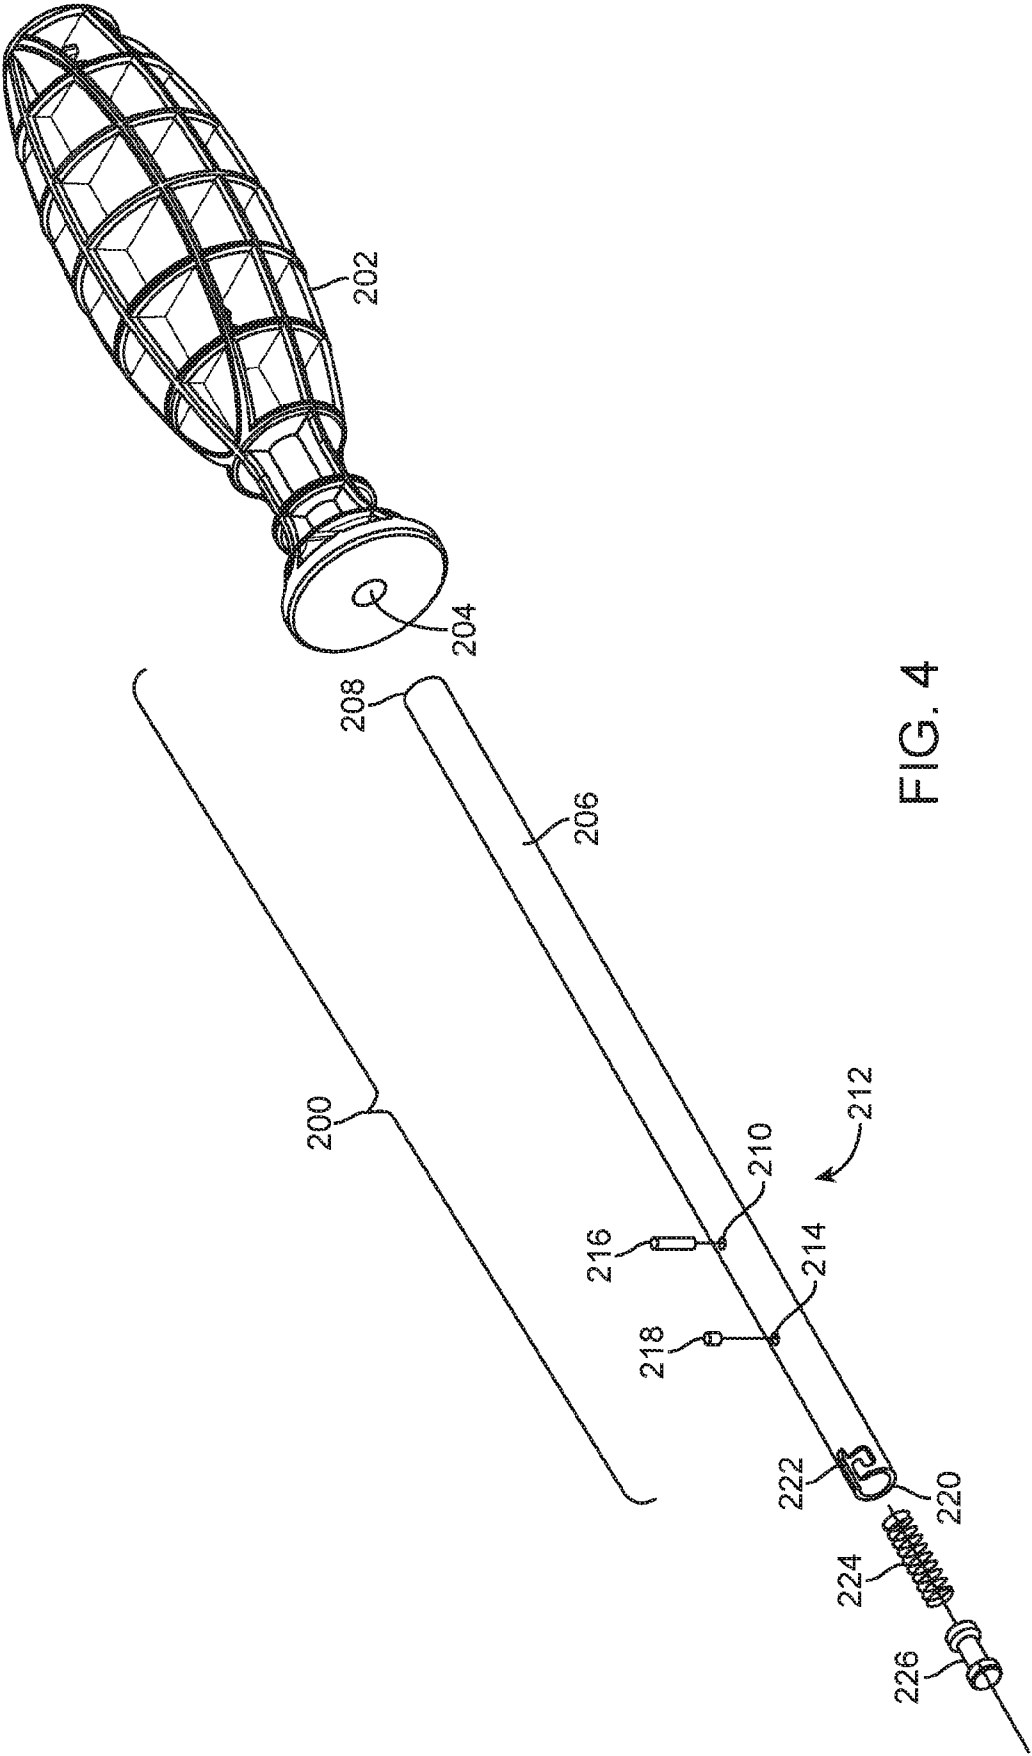


FIG. 4

5 / 17

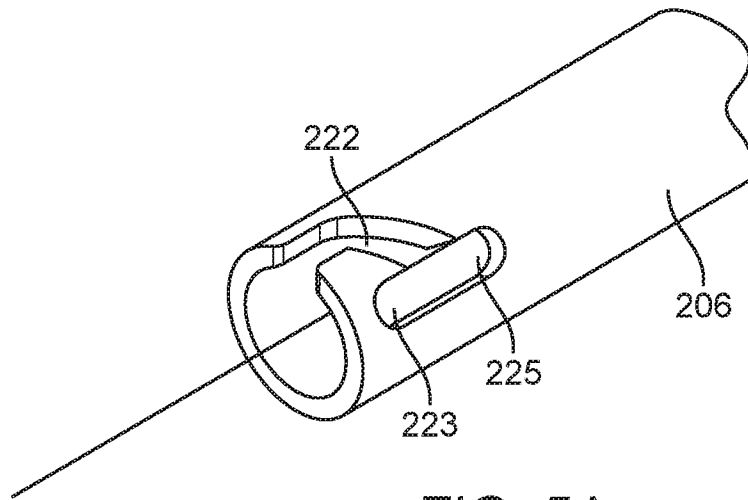


FIG. 5A

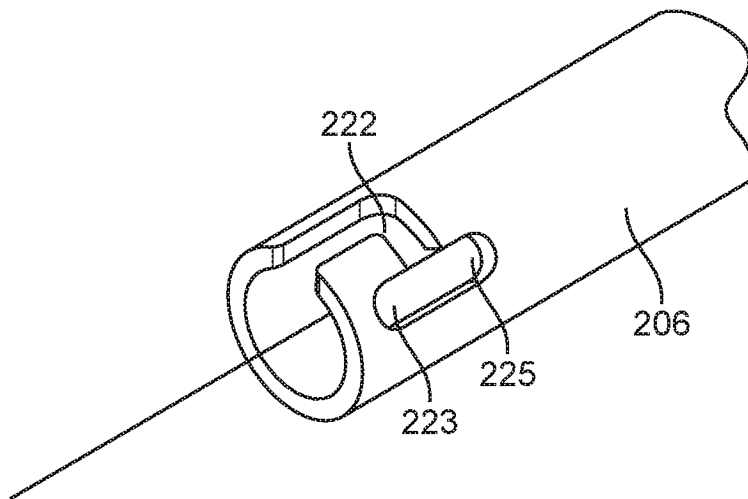


FIG. 5B

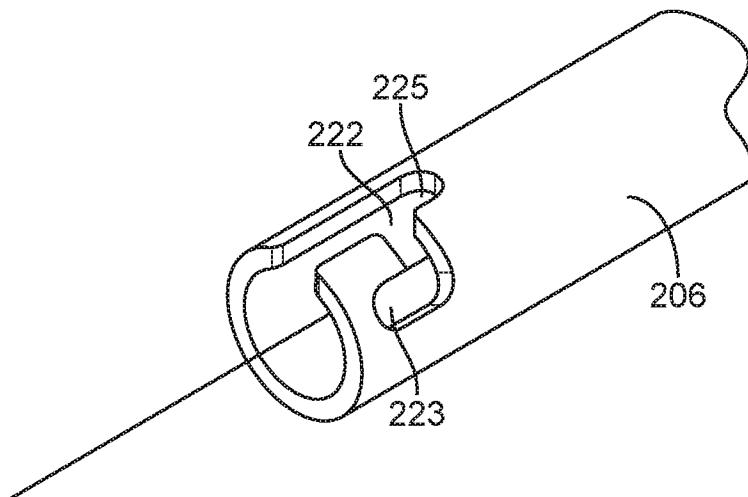


FIG. 5C

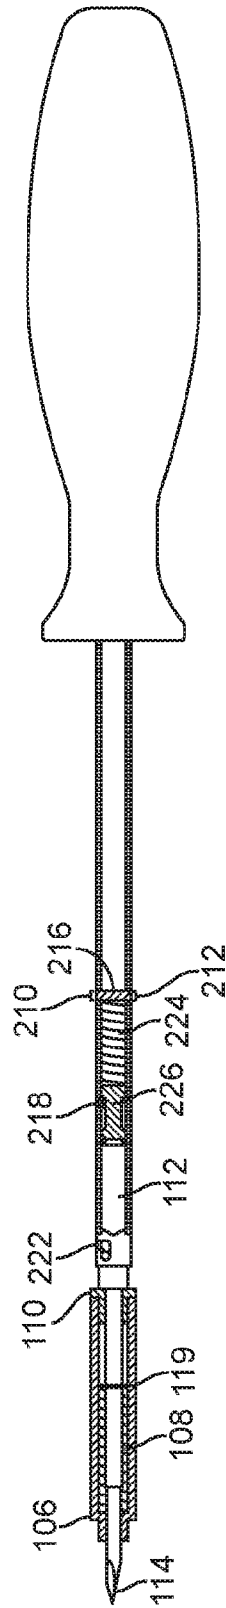


FIG. 6A

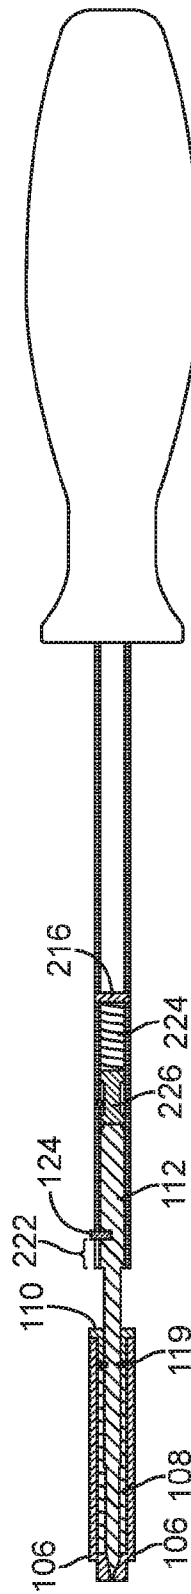


FIG. 6B


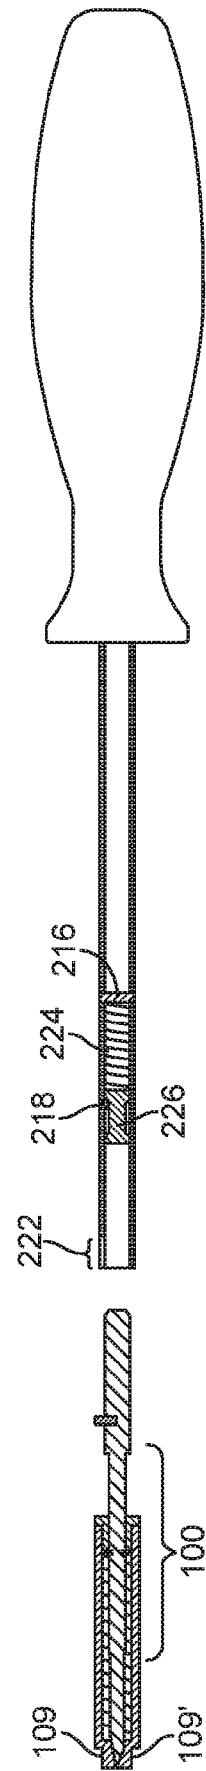


FIG. 6C

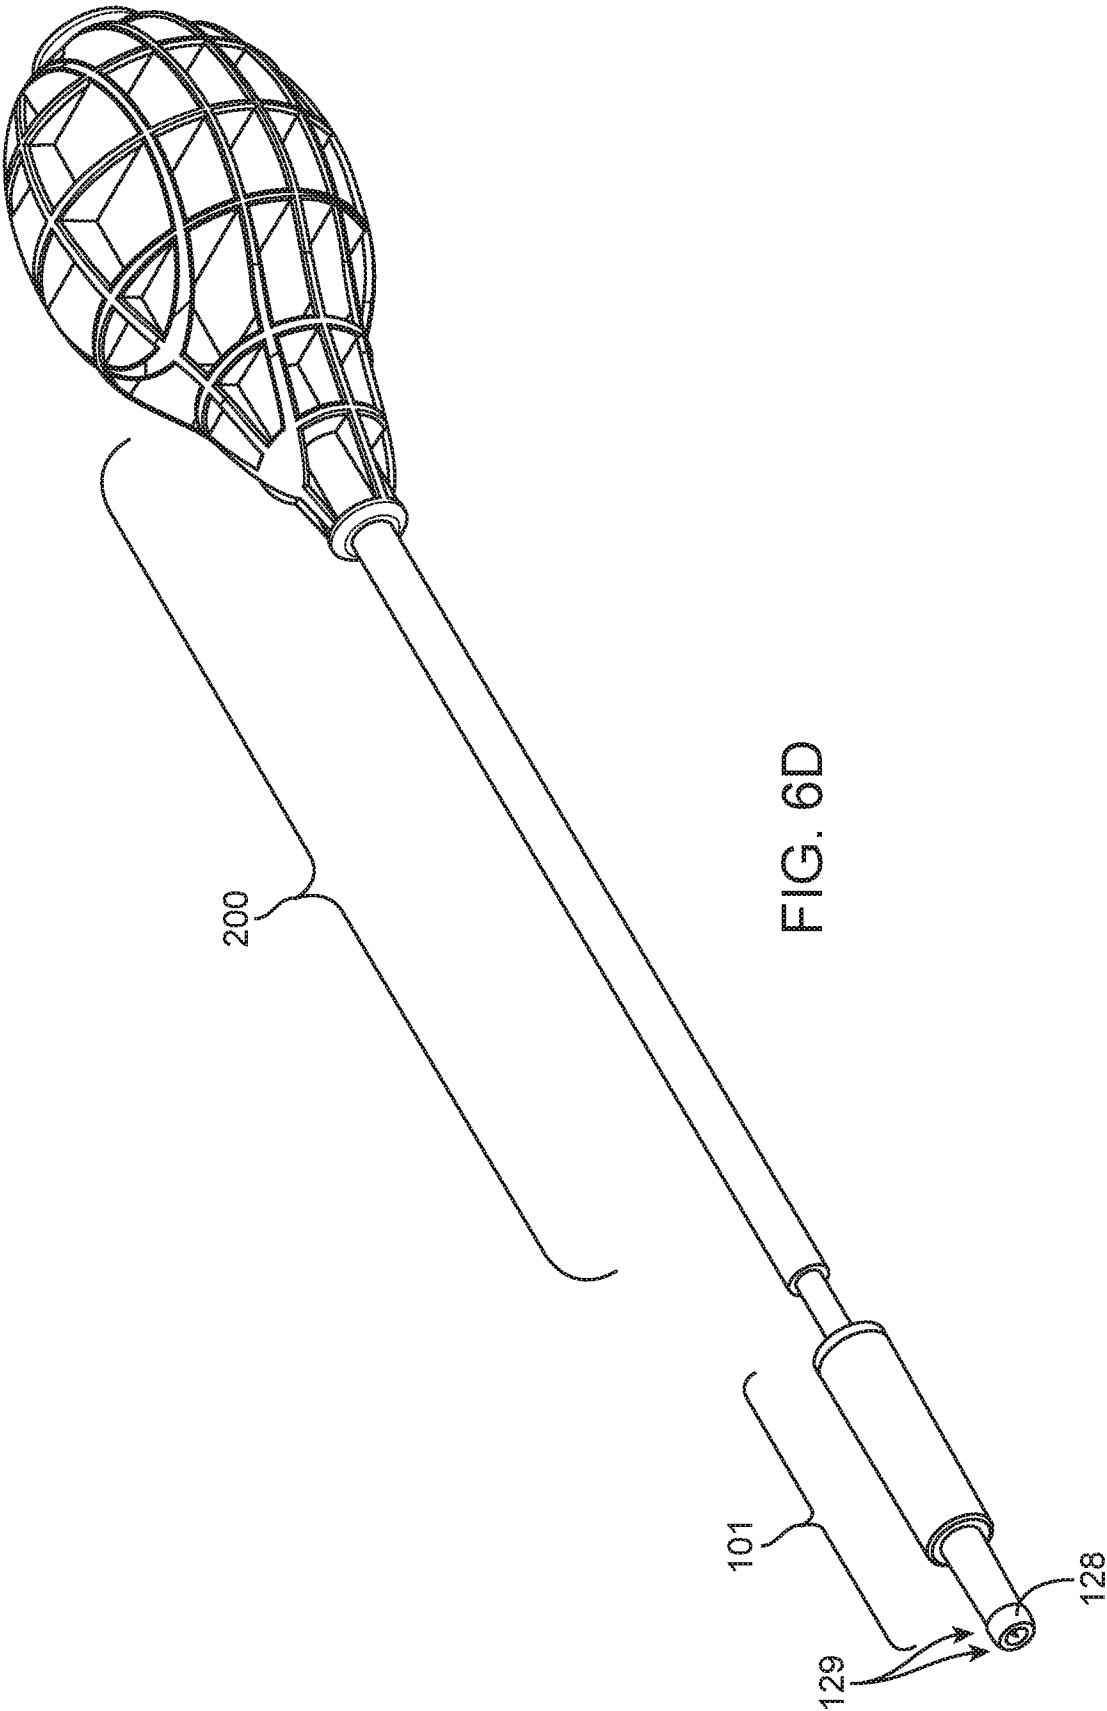

8 / 17

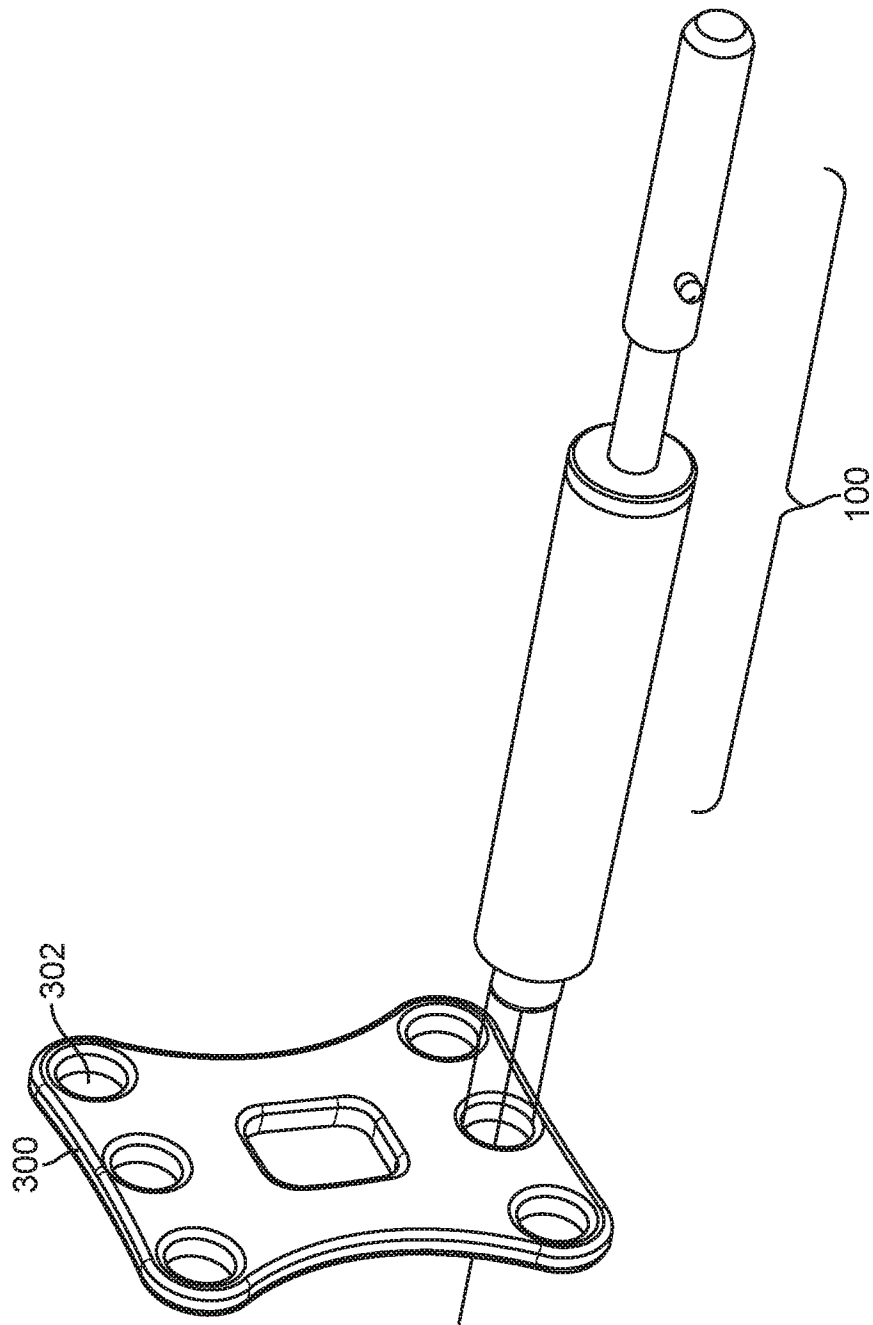
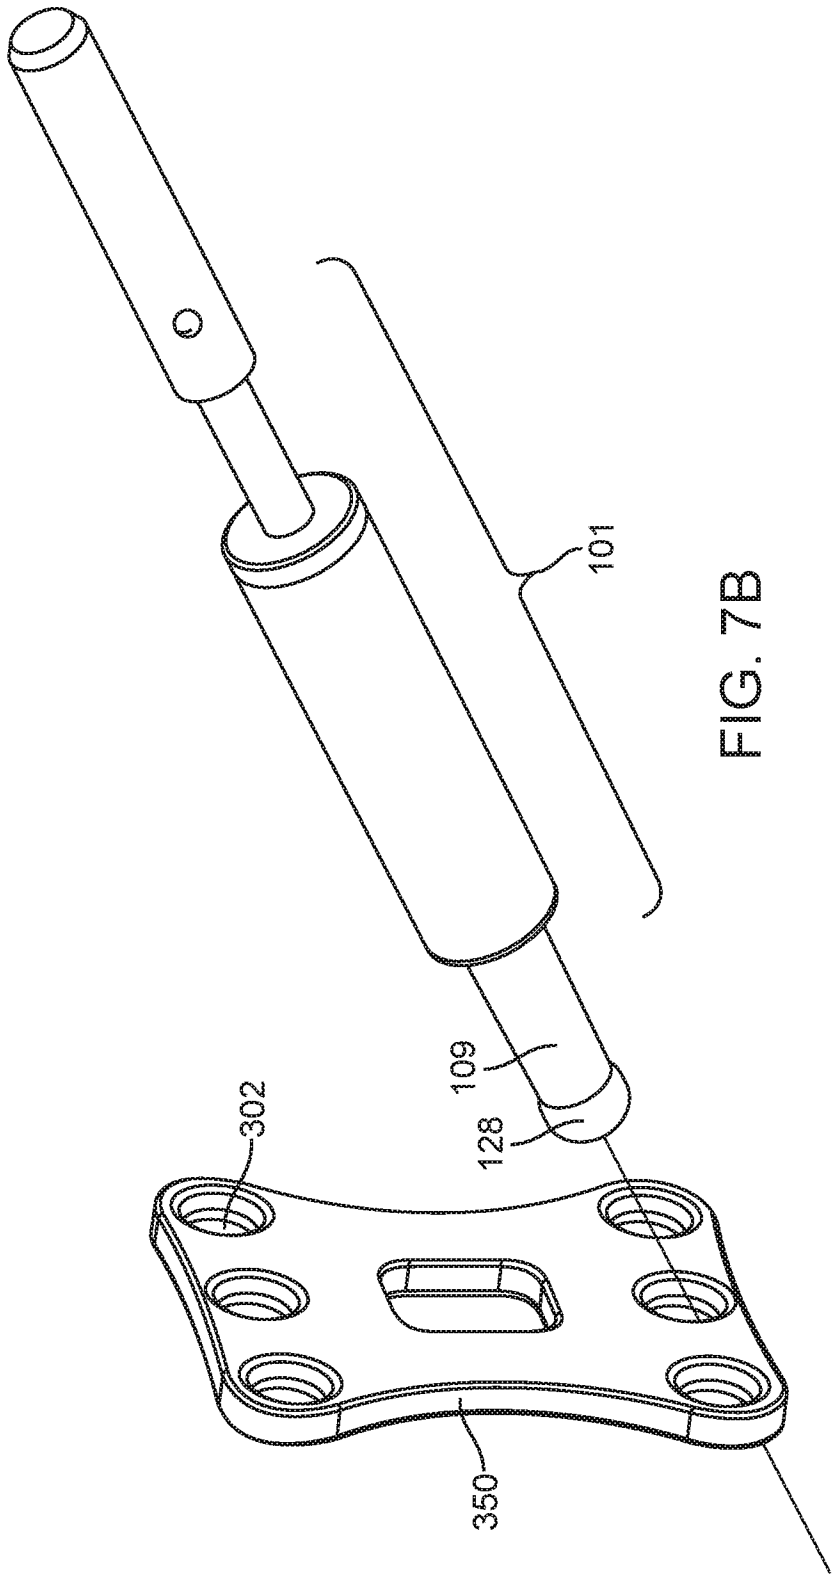


FIG. 7A



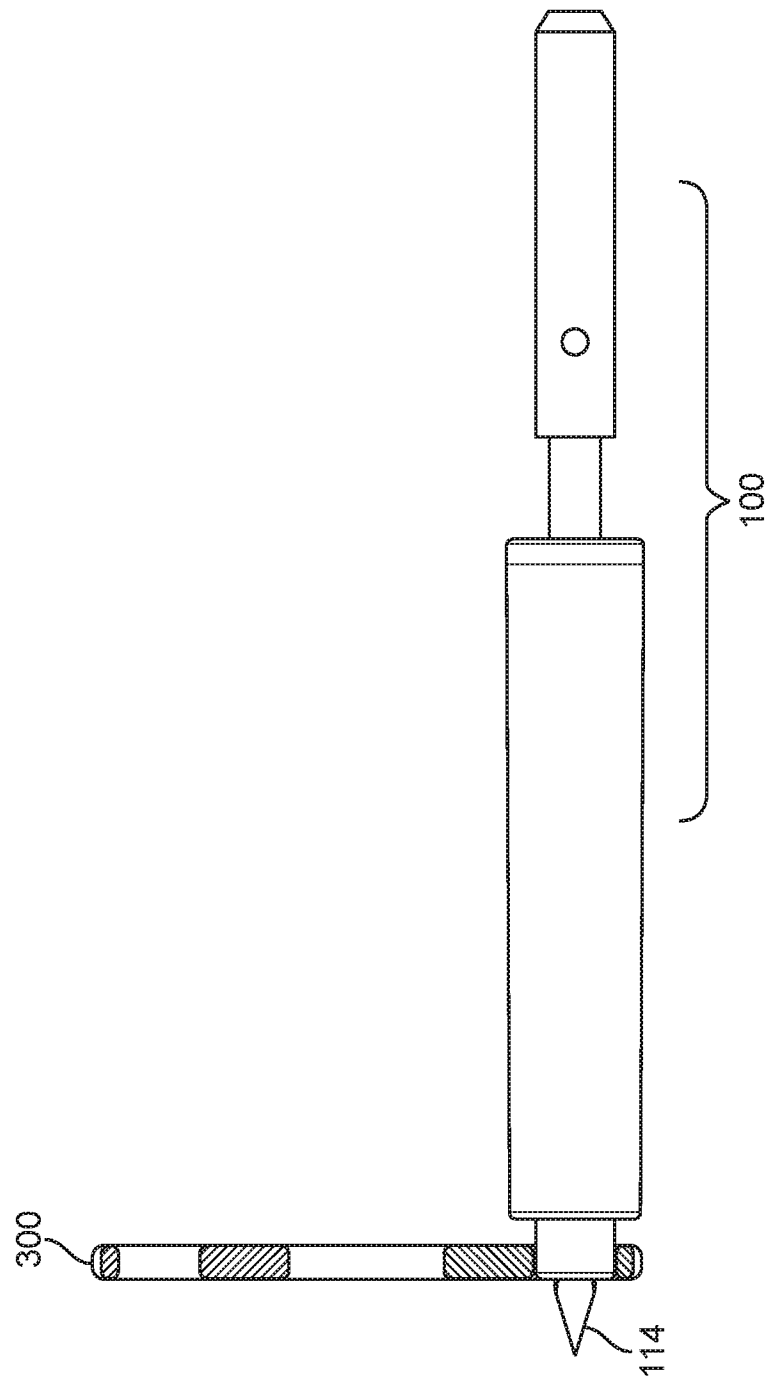
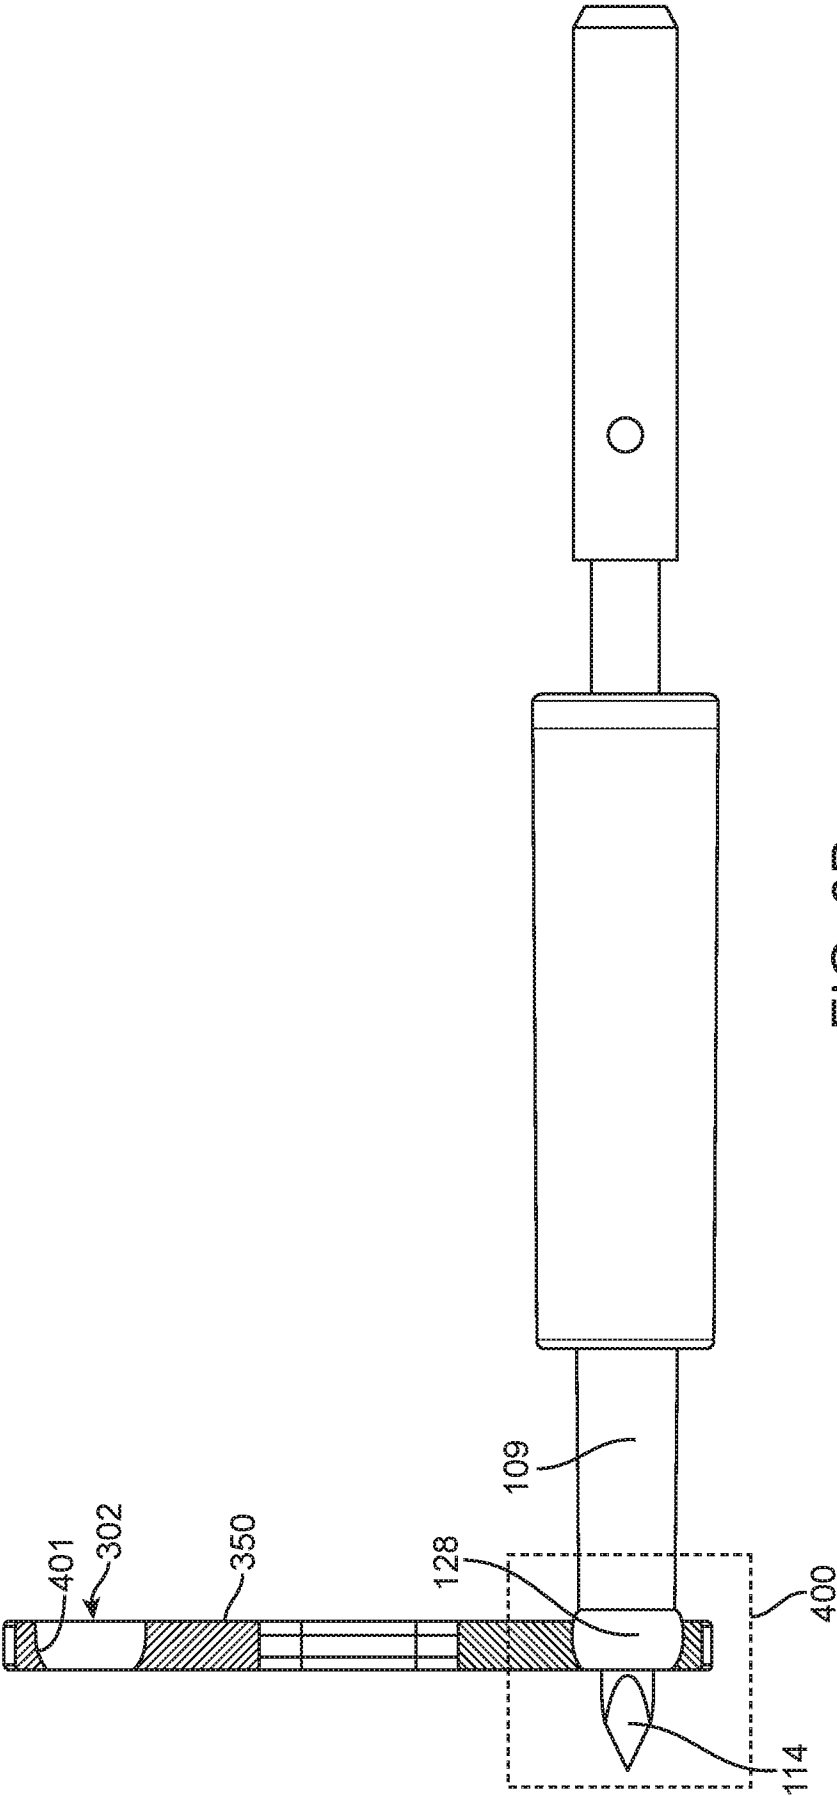


FIG. 8A



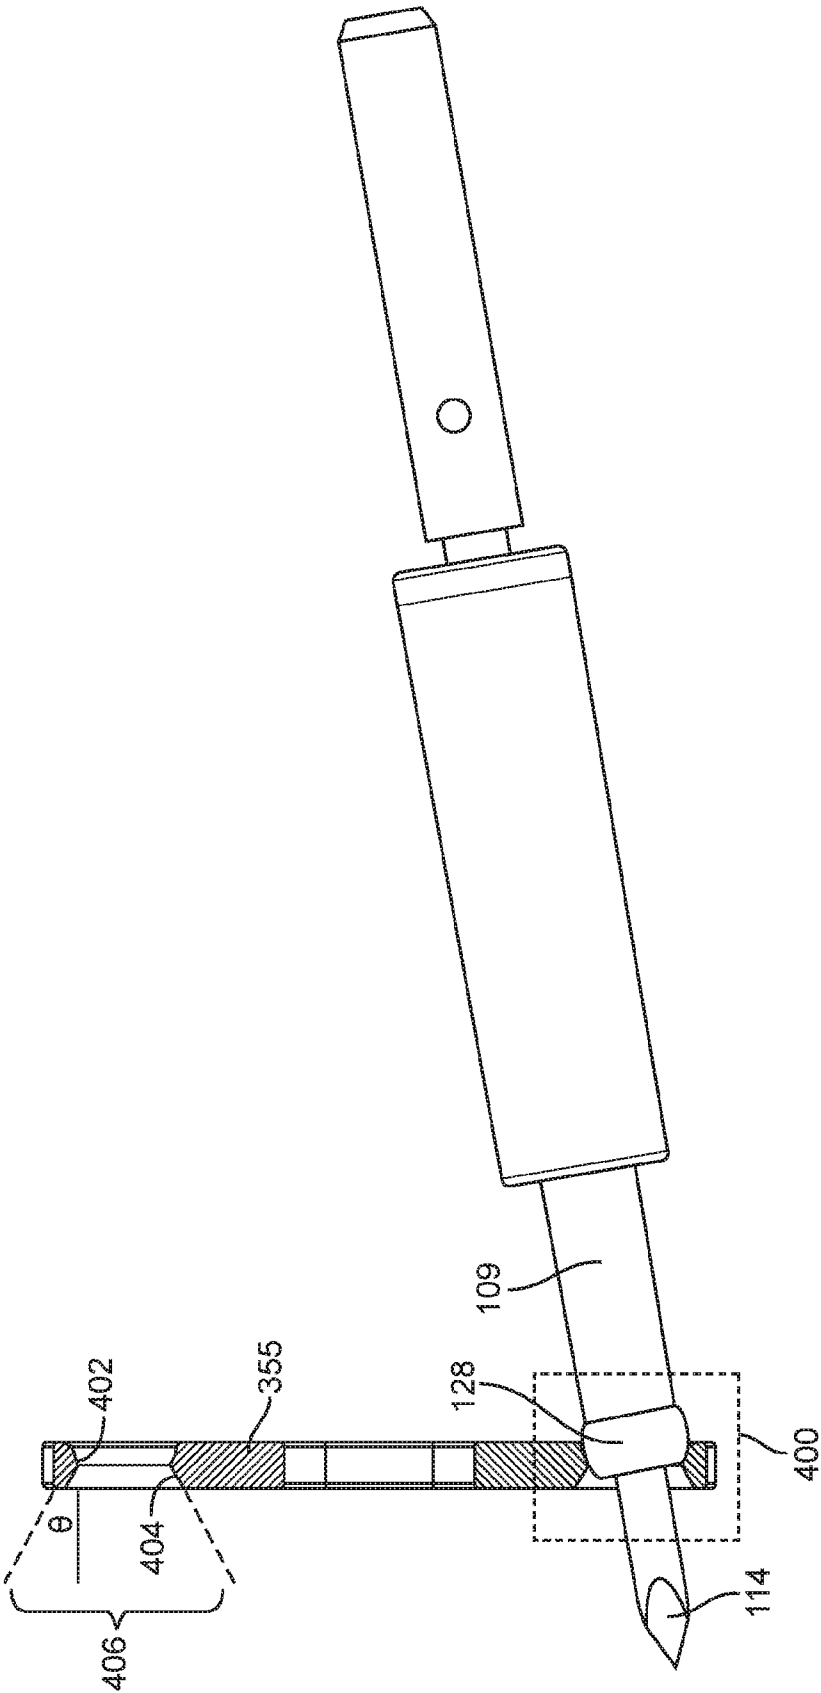


FIG. 8C

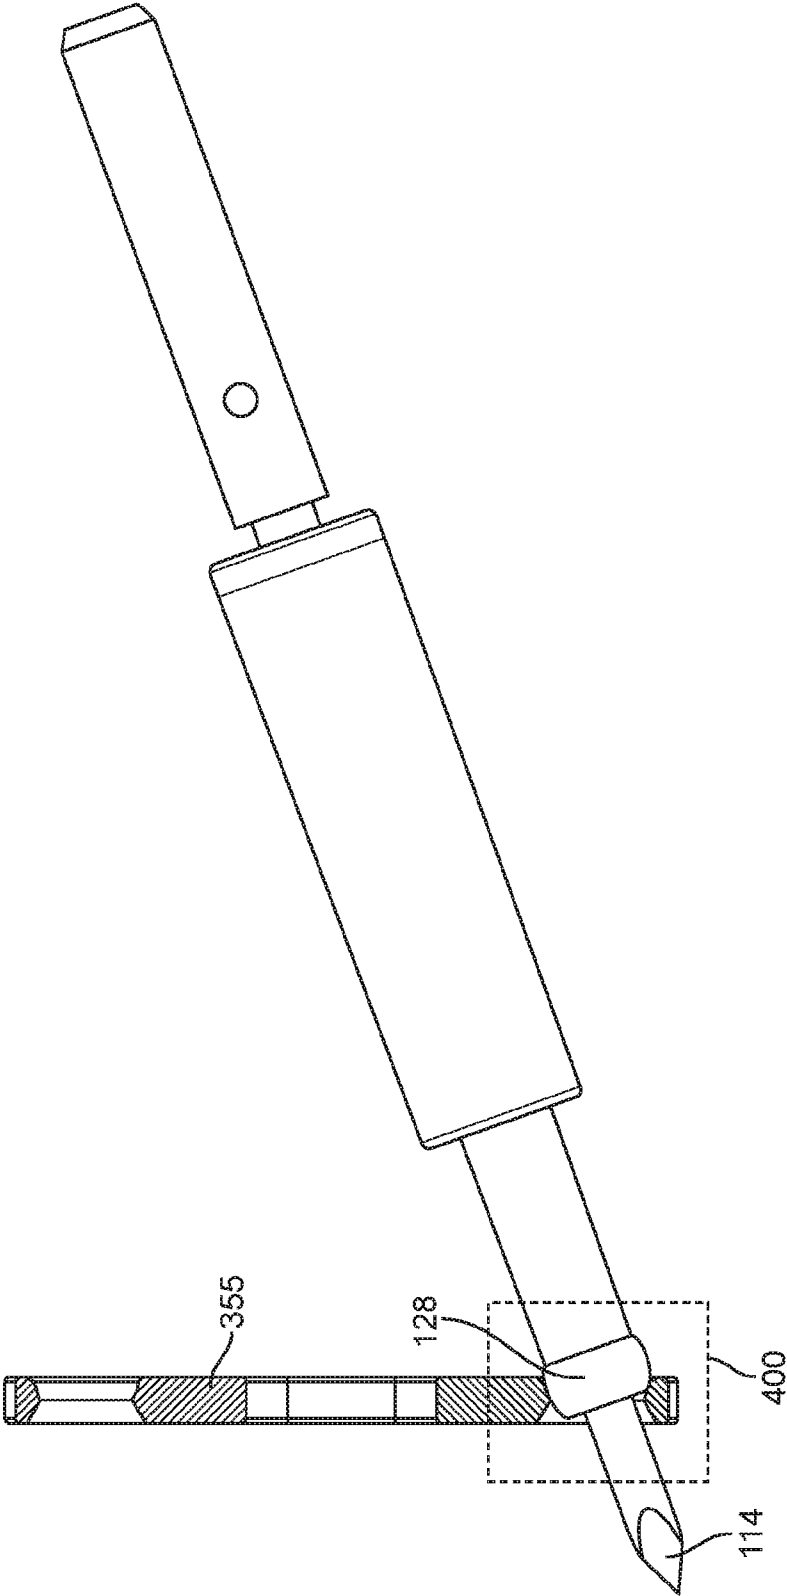


FIG. 8D

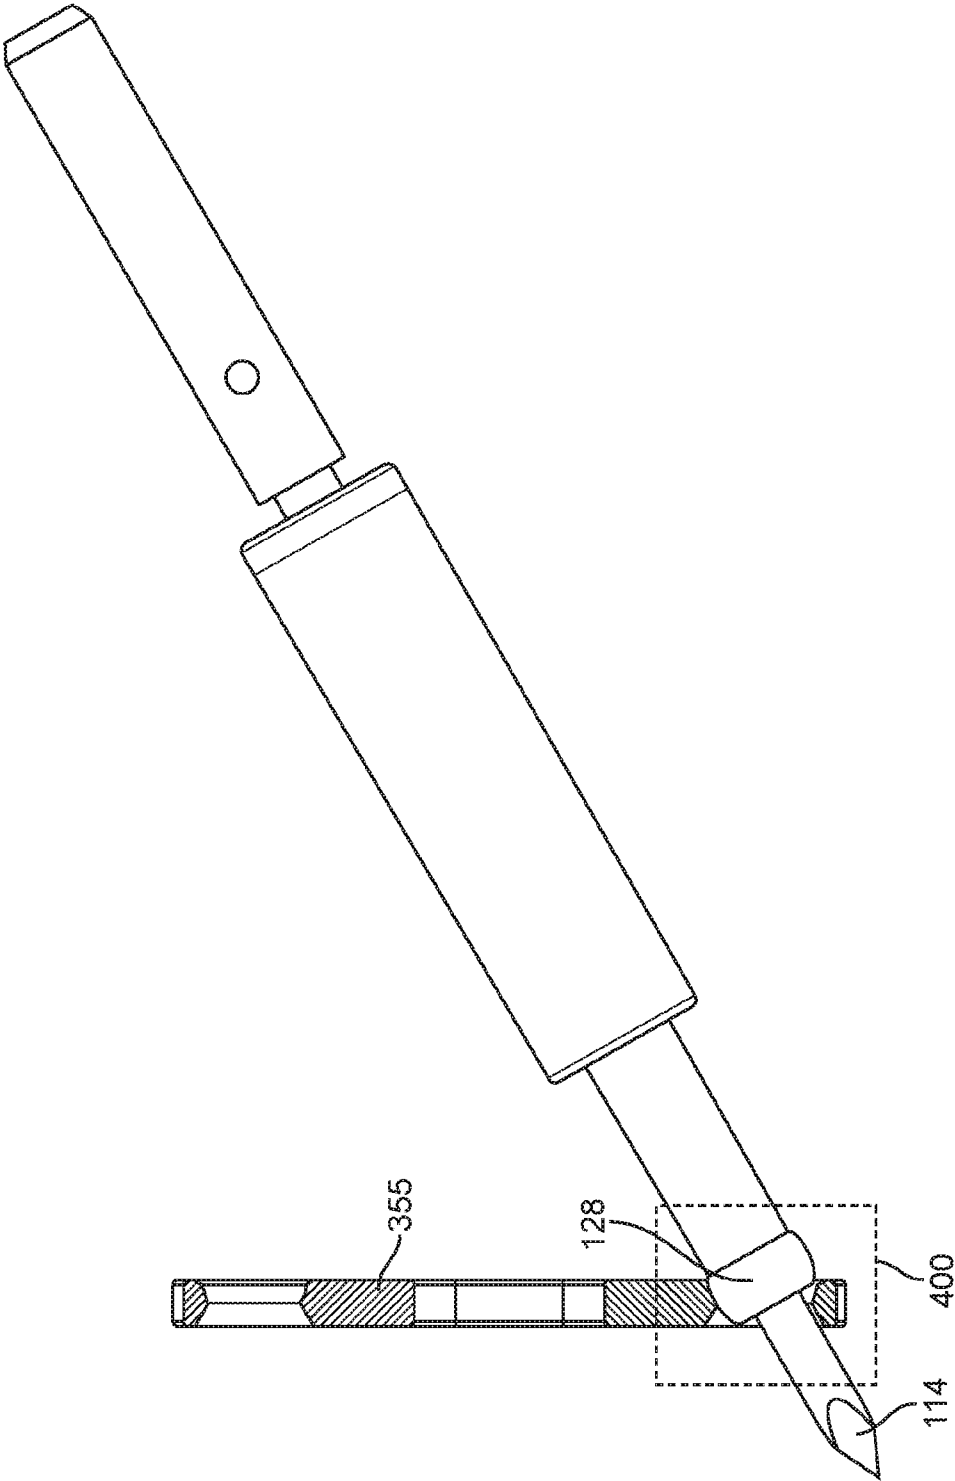


FIG. 8E

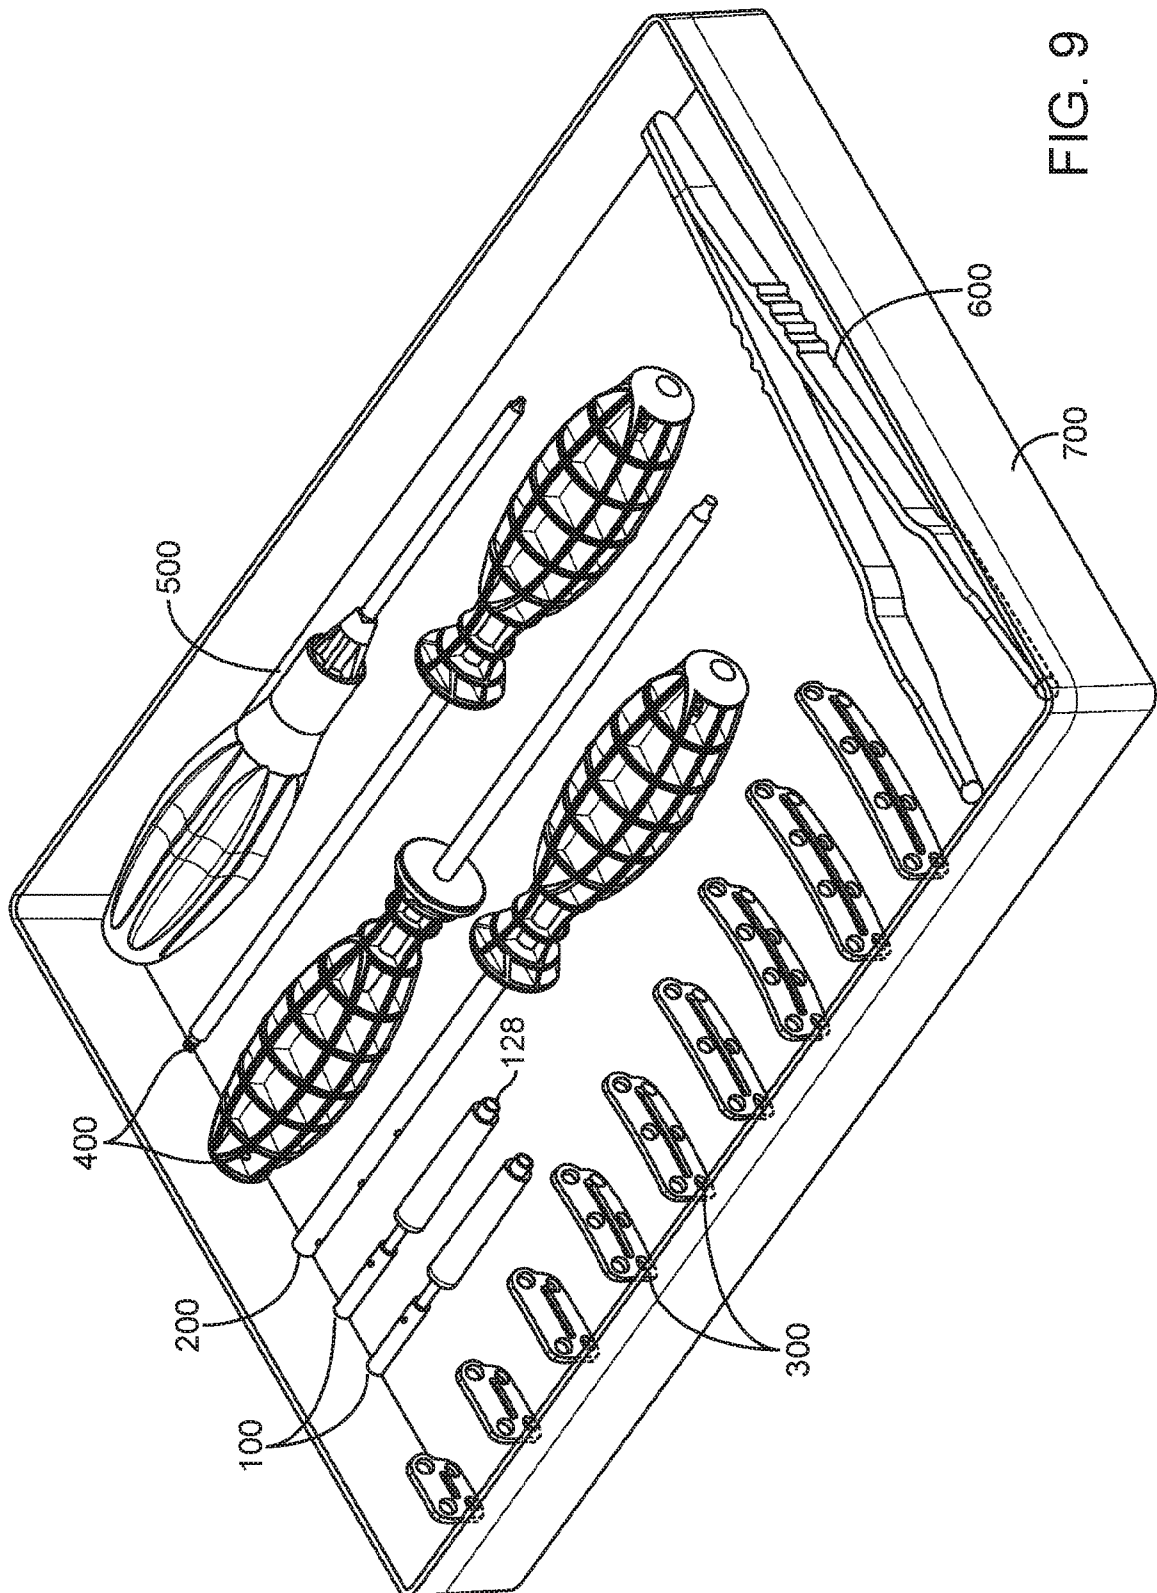


FIG. 9

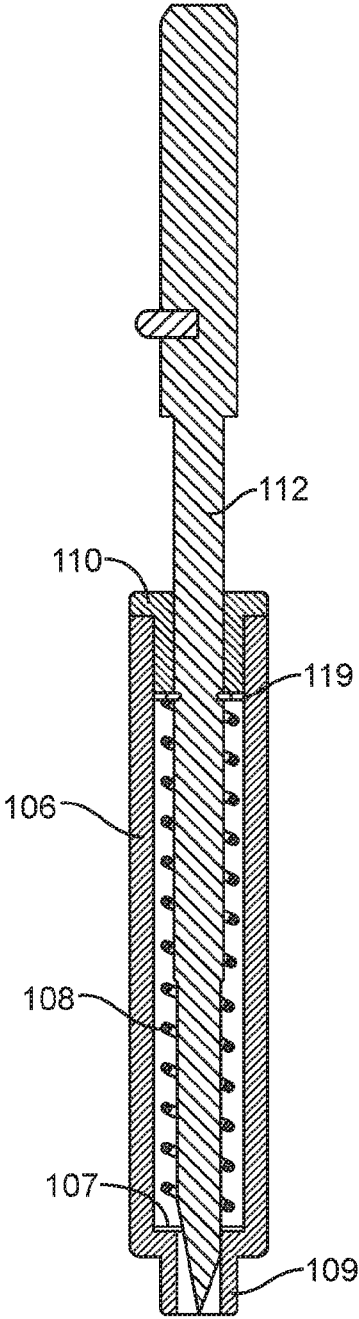


FIG. 10A

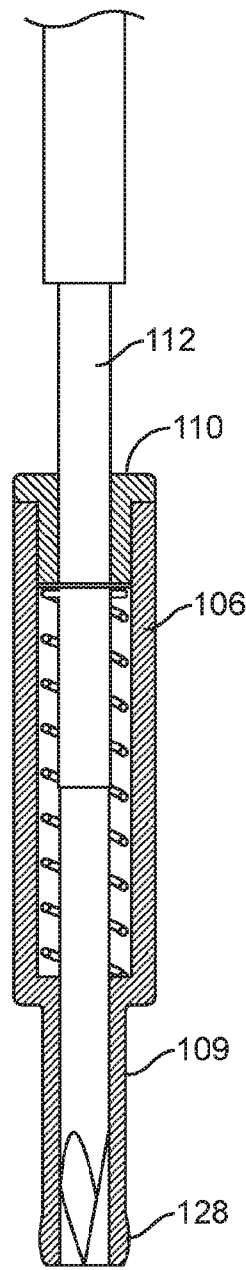


FIG. 10B

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US17/62631

A. CLASSIFICATION OF SUBJECT MATTER

IPC - A61B 17/17, 17/34, 17/70, 17/88 (2018.01)

CPC - A61B 17/34, 17/1604, 17/1633, 17/1728, 17/3403

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 2016/114769 A1 (ECA MEDICAL INSTRUMENTS) July 21, 2016; paragraphs [0022], [0024]-[0026], [0028], claim 24, figures 1- 4, 5A, 6A-6C, 7-8	1-10 & 12-13
A	US 7,540,875 B2 (JESSEN, J) June 2, 2009; abstract, column 10, lines 1-30, column 11, lines 5-15	1-10 & 12-13
A	US 2001/0029387 A1 (WOLF, P et al.) October 11, 2001; abstract, paragraph [0021], claim 1	1-10 & 12-13

☐ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

09 January 2018 (09.01.2018)

Date of mailing of the international search report

05 FEB 2018

Name and mailing address of the ISA/

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Shane Thomas

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774