




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification⁵ : A61F 2/08</p>	<p>A1</p>	<p>(11) International Publication Number: WO 94/15550 (43) International Publication Date: 21 July 1994 (21.07.94)</p>
<p>(21) International Application Number: PCT/US94/00191 (22) International Filing Date: 6 January 1994 (06.01.94) (30) Priority Data: 08/001,065 6 January 1993 (06.01.93) US 08/100,458 30 July 1993 (30.07.93) US (71) Applicant: SMITH & NEPHEW RICHARDS INC. [US/US]; 1450 Brooks Road, Memphis, TN 38116 (US). (72) Inventors: CASSIDY, James, J.; 9166 Valkrie Lane, Memphis, TN 38133 (US). MCLEOD, William, D.; 4756 Mallard Nest Drive, Memphis, TN 38141 (US). (74) Agents: KRIEGER, Paul, E. et al.; Pravel, Hewitt, Kimball & Krieger, 10th floor, 1177 West Loop South, Houston, TX 77027-9095 (US).</p>		<p>(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>With international search report.</i></p>

(54) Title: LOAD BEARING POLYMERIC CABLE

(57) Abstract

A surgical cable (10) for use in the repair of fractures or fusions of small bones (50), and to assist in the repair of torn ligaments and tendons. The surgical cable has unique characteristics of high tensile strength, flexibility and inelasticity or stiffness.

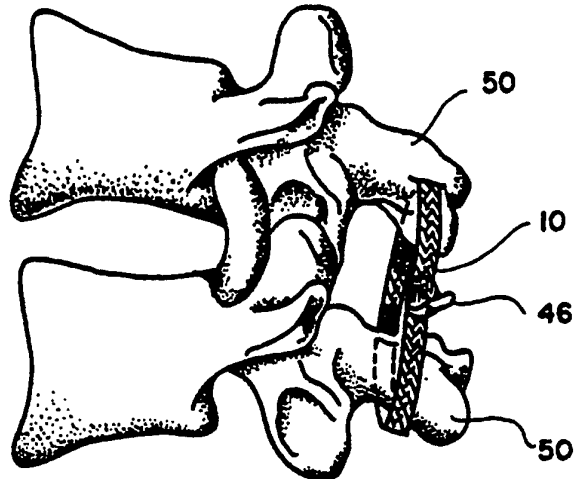

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgystan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

LOAD BEARING POLYMERIC CABLE

The present invention relates to a load bearing polymeric surgical cable, more specifically to a stress-sharing/shielding cable or suture for use in the repair of small bone fractures and fusions and in the repair of ligaments and tendons.

Surgical procedures for the repair or fusion of small bones, ligaments and tendons, require use of a prosthetic or orthotic device or suture which can bear a heavy load caused by the unique anatomical features of the compromised bone or tendon. For example, fractures of the patella are exposed to high stresses during flexion and extension of the knee joint; fusions of the spinal vertebrae are exposed to high gravitational forces and movements of the spinal column; and torn ligaments and tendons are exposed to high stresses due to contraction of the associated muscles or flexion and extension of the bony structures.

An orthotic, prosthetic device or suture used in such fashion must be able to bear heavy stress loads, be flexible enough to achieve the desired repair, and be sufficiently inelastic to maintain alignment of the anatomical structures for proper fusion and repair.

Materials currently available for such surgical procedures include synthetic or wire sutures, metal cable and various specialised prosthetic or orthotic devices. Synthetic and metal sutures are susceptible to fatigue and breakage during application and use. The currently available synthetic suture materials have insufficient strength and stiffness to provide the

- 2 -

stress sharing and strain-limiting capabilities required. Metal cable or wire sutures, while providing additional strength, lack the flexibility required for many fusion and/or repair procedures.

Satisfactory repair or fusion requires that the bones or bone fragments remain sufficiently immobilised to permit healing. Current procedures for the repair or fusion of small bones including vertebrae and the patella, restrict motion of the bones or bone fragments by wiring the elements into the appropriate position. The applied surgical wire is generally bent tightly around the bone fragments and two ends of the wire are generally twisted together to provide compressive force.

Breakage of wire sutures or cables may occur with bending during implantation of the device or post-implantation movement generating repetitive bending stresses. Failure of the wire to supply sufficient compressive force and apposition of bone fragments results in reduced or failed healing of the bones. Sharp wire points caused by wire breakage in situ can result in significant damage to surrounding tissues and/or joint capsules.

Metal suture material is radiopaque, and interferes with efficient x-ray monitoring of bone fusion and repair. Metal sutures also interfere with the use of magnetic resonance imaging diagnostic procedures which require that no metal be present in the vicinity of use.

- 3 -

It would be highly desirable to provide a small diameter, flexible, load bearing suture to replace low strength polymeric or synthetic sutures and metal sutures for use in the fusion, repair, and augmentation of small bones, ligaments and tendons.

It has been found that a braided cable formed of strong polymeric fibres produces a load bearing suture of sufficient tensile strength, flexibility and stiffness to be useful in the repair and fusion of small bones, ligaments and tendons.

The polymeric braided cable of the present invention has strength at least equivalent to that of a metal suture, and much greater flexibility. The present invention does not exhibit the problems associated with metal fatigue and breakage of wire, and may be formed with a much smaller diameter.

The polymeric braided cable of the present invention may also be formed of a bioresorbable polymer, eliminating the necessity of removing the cable and allowing gradual transfer of stress to the tissue or bone over time.

The load bearing cable of the present invention has the following characteristics: greater tensile strength than available polymeric suture materials; greater stiffness than available suture materials; greater flexibility and fatigue lifetime than metal sutures; transparent to x-rays and does not interfere with magnetic resonance imaging; tightly woven to discourage tissue ingrowth.

- 4 -

The load bearing cable of the present invention is formed of a plurality of high tensile strength polymeric fibres, each of which is less than 100 microns in diameter and has a tensile strength of greater than or equal to about 300,000 psi, suitably greater than or equal to about 350,000 psi and preferably greater than 500,000 psi. To form the load-bearing cable, a plurality of such fibres are formed into a hollow braid having a longitudinal bore extending through the centre. The load bearing cable may comprise a braid formed from as few as one ply or as many as six ply bundles of approximately 120 individual fibres per ply.

According to the present invention there is provided a load bearing cable comprising a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs.

The cable of the present invention is aptly formed of from one to 6 ply of polymeric fibres. Aptly the cable is a two-ply, eight strand braided cable, preferably less than 3mm in diameter. Preferably the cable is a one ply, eight strand braided cable less than 1mm in diameter.

In rope terminology, a plain braid is defined according to the number of picks per inch. A "pick" is

- 5 -

defined as a crossing of one yarn bundle over another, with the number of picks counted across the longitudinal axis. The greater number of picks per inch, the tighter the braid.

Suitably the cable is such that the braid has a weave angle that provides 5 to 7 picks/inch. In the preferred embodiment the braid has approximately 4 to 8 picks/inch providing a flexible cable having a desired diameter of less than 3mm.

The fibres are formed of a high strength, biocompatible, organic polymer, preferably polyolefines such as high strength polypropylene or ultra-high molecular weight polyethylene. US patent 4,413,110, to Kavesh et al, describes one process for the production of ultra-high molecular weight polyethylene (UHMWPE) fibres which have a high tenacity and a high tensile modulus. Any suitable means for providing UHMWPE will suffice.

Commercial embodiments of the polyethylene fibres described in the Kavesh patent are known by the Trade Marks **SPECTRA-900** and **SPECTRA-1000** and are sold by Allied-Signal Inc. These commercially available fibres have a tensile strength of about 375,000 - 425,000 psi per individual monofilament. The density of each monofilament is between 0.5 and 1.5 g/cm³, preferably about 0.97. Fibres of **SPECTRA-1000** have a tenacity of approximately 35 g/denier, a specific gravity of 0.97 and an average diameter of 27 microns (0.0011 inch). Each monofilament is less than 100 microns in diameter.

- 6 -

Fibres are assembled to form a tight weave which discourages fibrous ingrowth. Preferably, pore sizes are less than 30 microns. For UHMWPE, the cable 10 is optimally formed of 8 strands, each strand having from one to six ply. Each single ply strand contains approximately 120 fibres of UHMWPE. Thus, the preferred embodiment of the braided load-bearing cable 10 has from 960 individual fibres for a one ply braid to 1920 individual fibres for a two ply braid.

Preferably the load bearing cables of the present invention have a diameter of approximately less than three millimetres and can carry loads of up to 550 pounds. For example, a single ply 8-strand diamond braid can withstand a load of approximately 320 lbs and a double ply can withstand a load of approximately 320 lbs..

The cables of the present invention are formed with the strongest available biocompatible polymer and optionally with a biocompatible resorbable polymer. The upper limit imposed on the strength of the polymer is the flexibility required.

In one embodiment, the polymeric fibres of the present invention are bioresorbable. Suitable fibres are, for example, those formed of polylactic acid or polyglycolic acid.

Examples of material useful in the present invention are ultra-high molecular weight polyethylene fibres, each having a tensile strength of aptly at least 300,000 psi. Suitably each fibre has a tensile

- 7 -

strength of at least 350,000 psi. Especially preferred is the ultra-high molecular weight polyethylene, eg. **SPECTRA-1000**.

The surface of the fibres may be modified, for example roughened, for ease of fixation of the cable.

The load bearing cable of the present invention may be utilised in a variety of surgical procedures to fuse or repair small bones and ligaments and tendons. For example, the cable may be used as an orthosis and shield the torn ligament or tendon from the normal stress and strain until the tissue has healed, eg. by sewing the cable through remnants of a ligament and bringing the torn ends into opposition. Accordingly to facilitate such use, the cable 10 may be attached to a needle 60 as shown in Figure 6, or similar device for threading the cable 10 through tissues.

Accordingly the present invention further provides the cable of the present invention having a needle attached to at least one end of the longitudinal axis of the cable. Suitably the needle is attached to one end only of the longitudinal axis of the cable.

Alternatively, the cable may be used to shield normal stress and strain until the tissue has become strong enough to carry the full amount of stress, eg. by sewing the cable through a replacement tissue graft. The load bearing cable of the present invention may also be substituted for surgical wire or cable in the repair of small bone fractures such as the patella or bone fusions such as vertebral fusions. The cable has

- 8 -

sufficient tensile strength to maintain bone fragments in close approximation to promote active healing and is sufficiently inelastic to prevent separation of fragments under tensile loading. The load bearing cable is less susceptible to fatigue failure than surgical wire. In the event the cable does fail, no threat of damage to surrounding tissue is posed.

The present invention further provides a method for the repair of torn ligaments and tendons comprising opposing torn ends of a ligament or a tendon with a load bearing cable comprising a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs.

In the method of the present invention, the cable may additionally be sewn through a tissue graft.

In a further embodiment of the present invention there is provided a method for the repair of fractures or fusions of small bones comprising bringing bone fragments or bone elements into close approximation and applying compressive force thereon by winding a load bearing cable comprising a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can

- 9 -

withstand approximately 300 to 550 lbs, about or through opposed bone fragments or bone elements and tightly securing together the ends of the cable.

The securing together of the ends of the cable may be by any suitable means, eg. by knotting. Alternatively the securing together of the ends may be by fusing the ends by using heat.

According to the method of the present invention the cable may be applied to fragments of the patella. Alternatively the cable may be applied to the fusion of adjacent vertebrae of the spinal column.

In a yet further embodiment of the present invention there is provided a method for the repair of opposed fractures of small bones or for enabling fusions of small bones, comprising the steps of:

- a) positioning opposed bone fragments or elements into close approximation with each other;
- b) applying a compressive force between the opposed bone fragments or elements toward each other, the polymeric cable being flexible and capable of bearing sufficient stress loads to repair or fuse the opposing bone fragments or elements, and to be sufficiently inelastic for maintaining continuous pressure on the bone fragments or elements; and
- c) securing the cable in place relative to the bone fragments or elements.

The positioning of the bone fragments or elements may further include the positioning of adjacent vertebrae of the spinal column or the patella. The

- 10 -

surgical cable employed in the above disclosed method suitably has a diameter of less than or equal to 3mm, is capable of withstanding a load of up to 550 lbs and the tensile strength of each polymeric fibre is greater than or equal to 500,000 psi.

Suitably the cable employed in the method of the present invention is formed of braided strands of polymeric fibre. Suitably the fibres are bioresorbable. Preferably the fibres comprise ultra high molecular weight polyethylene, eg. **SPECTRA 1000** fibres.

In the method of the present invention, the step of applying a compressive force may further include wrapping the polymeric cable around the adjacent vertebrae or fragments to fuse them together.

The method of the present invention may further include attachment of the cable to bone with an attachment means. The attachment means may be any suitable attachment means, eg. surgical staples, pins and screws.

The present invention can be better understood by reference to the drawings in which:

Figure 1 is a pictorial view of the load bearing cable of the present invention as applied to adjacent vertebrae in a spinal column fusion.

Figure 2 is a pictorial view of the load bearing cable of the present invention as applied to repair of

- 11 -

a fractured patella.

Figure 3 is a pictorial view of the load bearing cable of the present invention as applied to the repair of a torn ligament.

Figure 4 is a pictorial view of the load bearing cable of the present invention as applied to the repair of a clavicular ligament.

Figure 5 is a longitudinal view of a braided load bearing cable of the present invention.

Figure 6 is a pictorial view of a load bearing cable of the present invention swaged to a needle.

Figures 1 through 6 illustrate the exemplary embodiments of a load bearing cable 10 of the present invention. Although the cable of the present invention is shown as connecting specific small bones and/or ligaments, the cable can also be used in the repair of other small bones and soft tissues.

As shown in Figure 5, the load bearing, braided cable 10 is formed of a plurality of biocompatible polymeric fibres wound as bundles of parallel fibres into yarns 22. Yarns of from one to six ply are then wound into strands 24. The strands are then intertwined to form the braided cable 10, for example, an eight-strand diamond braid. In a preferred embodiment, the polymeric fibres are bundled into yarns of approximately 650 denier, the yarns are wound into 1 to 6 ply, and more preferably one or two-ply strands,

- 12 -

and the strands are braided into a single, hollow, plain 8-strand diamond braid. The braided construction allows utilisation of high strength fibres as individual units while providing negligible bending resistance. Preferably, the resulting braid contains approximately 4 to 8 picks per inch.

Characteristics of the structure of the present invention and its application may be better understood by reference to the examples which follow:

Example 1

Fatigue Testing of Metal Surgical Sutures

Titanium orthopaedic cable having a diameter of 0.045 inch and cobalt chromium orthopaedic cable having a diameter of 0.045 inch were tested for bending fatigue. A 15 inch length of the metal cable was installed on a bending fixture for fatigue testing. A loading rod was fixed to a load cell and the fatigue test fixture was positioned so that the loading rod was directly above the cable. Operating in stroke control the loading rod was moved downward against the cable until a load of two pounds was read. The displacement of the crosshead at this two pound load was recorded. The rod was then advanced until a load of 20 pounds was indicated, and this displacement was recorded. Still in stroke control, a sinusoidal function varying between the two previously recorded displacements was established at a rate of 0.5 Hz. This created a load variation on from 2 to 20 pounds on the cable, with resultant bending around the rod. Testing continued

- 13 -

until the cable broke. This testing was performed on six titanium cables and six cobalt chromium cables. The results are shown in Table 1.

Table 1

<u>Cable Material</u>	<u>Average Cycles to Failure</u>
Cobalt Chromium	18,408 (S D 4854)
Titanium	8,042 (S D 1161)

Example 2

Fatigue Testing of a Cobalt-Chrome Surgical Cable

Testing was performed on a cobalt-chrome surgical cable (Richards MP35N), 0.044 inches in diameter in a bending fixture as described for Example 1. The pulley system was cycled at a rate of 0.7 Hz at displacements that resulted in the plunger seeing an axial load that varied between 2 to 20 pounds. Cycling was halted upon failure. The average fatigue life was 56,700 cycles.

Example 3

Fatigue Testing of Braided UHMWPE Surgical Cable

An ultra-high molecular weight polyethylene braided cable was fabricated from **SPECTRA-1000** fibre. Yarns of approximately 650 denier were arranged as single ply and two-ply strands, and braided into an 8-strand hollow diamond braid.

- 14 -

The braided cable was fatigue tested in a bending fixture as described in Example 1. The springs had a spring constant of 6 lbs/in. The pulley radius was one inch. The distance between pulley centres was three inches. The load plunger had a radius of 0.2 inches. Each test was conducted at 1 Hz.

During fatigue testing, the surgical cable or metal suture was subjected to a sinusoidal plunger load of from 2 to 20 pounds-force (lbf). The springs provided resistance to the plunger load. The material was also subjected to a pre-load of approximately 7.5 lbf due to the tensioning of the springs.

The polymeric ultra high molecular weight polyethylene cable of the present invention was attached to the springs by tying a knot in both ends of the braid and searing the knot with heat. The knot was then passed through a ring and set screw and a set screw was tightened down to secure the braid to the spring.

Because the cable was flexible, the loading was considered a purely tensile load. Therefore, a static analysis was used to determine the tension in the cable. A single ply braid having a cross-sectional diameter of approximately 0.040 inches (1 mm) and a two-ply braid having a cross-sectional diameter of approximately 0.060 inches (1.52 mm) were tested. The maximum stress in each cable was 401 psi for the single ply and 267 psi for the two ply cables.

Before testing, half of the ultra high molecular

- 15 -

weight polyethylene braids were treated to roughen the surface of the braid for enhancement of knot holding capability of the braid by application of a charged plasma to the surface of the braid.

Five tests were run for each of the single ply and two ply braids in both treated and untreated conditions. The results are shown in Table 2. The single ply and two ply braided ultra high molecular weight polyethylene surgical cable in both treated and untreated conditions survived 100,000 cycles in the bending fixture described above. There were no braid failures or knot failures in any of the tests taken to 100,000 cycles.

Fatigue testing of metal surgical cables using the same procedure and protocol indicated that MP35N cables (cobalt-chrome) had a fatigue life of 56,700 cycles as discussed in Example 2. Testing of titanium and Co-Cr surgical cable using the same protocol and procedures determined the fatigue life to be 8,042 cycles and 18,408 cycles, respectively, as discussed in Example 1.

These results indicate the braided polymeric cable of the present invention has a better fatigue life than the metal cables formed of cobalt-chrome, or titanium. The charged plasma surface roughening treatment did not effect the fatigue life of the braid.

- 16 -

Table 2Fatigue Strength of UHMWPE Braided Cable

<u>Ply</u>	<u>Roughening Treatment</u>	<u>Cycles</u>
Single	Untreated	100,000
Single	Untreated	100,000
Single	Untreated	100,000
Single	Untreated	100,000
Single	Untreated	100,000
Single	Treated	100,000
Single	Treated	100,000
Single	Treated	100,000
Single	Treated	100,000
Single	Treated	100,000
Two-Ply	Untreated	100,000
Two-Ply	Untreated	100,000
Two-Ply	Untreated	100,000
Two-Ply	Untreated	100,000
Two-Ply	Untreated	100,000
Two-Ply	Treated	100,000
Two-Ply	Treated	100,000
Two-Ply	Treated	100,000
Two-Ply	Treated	100,000
Two-Ply	Treated	100,000

Example 4Repair of Anterior Cruciate Ligament

The anterior cruciate ligament of the knee connects the femur to the tibia, preventing the tibia from sliding anteriorly beneath the femur. As shown,

- 17 -

for example in Figure 3, to repair or reconstruct a torn anterior cruciate ligament, the load bearing cable 10 of the present invention is anchored to both the femur 30 and the tibia 32. Anchorage to bone may be via surgical staple, pins, or screws 34. The cable 10 is sewn along the axis of the normal ligament, and thus bears all or part of the tensile load normally borne by the native ligament. The cable replaces a cast, cast-brace or brace normally required to immobilise the joint after surgery and permits healing of the tissue graft by acting as an internal splint to shield the tissue from stress while permitting some joint motion during the post-operative period. This procedure alleviates loss of tensile strength in the tissue graft normally associated with joint immobilisation following surgery. Once satisfactory tissue strength is achieved in the graft, the cable may be removed.

When a bioresorbable cable is used to augment the ligament, the cable will resorb over a suitable time for healing, gradually transferring load to the tissue graft.

Example 5

Repair of Patella Fracture

As shown in Figure 2, the patella 40 is a small bone which covers the anterior compartment of the knee joint. Superiorly it is attached to the tendon of the quadriceps muscle group and inferiorly, it is attached to the patellar ligament 42, which inserts into the anterior surface of the tibia 44. The patella

- 18 -

functions to enhance the lever arm of the muscles which extend the leg. As such, the patella is loaded in tension, having an approximate superior-inferior direction.

When the patella is fractured in a transverse direction, perpendicular to the line of force, apposition of the patella fragments and compressive force is required to keep the fragments in close approximation for healing. Generally, surgical wire has been used to bend tightly around the patella, twisting two ends of a wire together to provide compressive force. This application method often results in wire breakage. In addition, post implantation wire fatigue caused by high tensile stresses from the quadriceps muscle group during extension of the leg often causes surgical wire to fail. Failure of the wire to supply sufficient compressive force or failure or intimate apposition of patella fragments due to wire breakages results in a reduced or failed healing of the bone. Sharp wire points caused by wire breakage in situ can result in significant damage to surrounding tissues and may even penetrate the knee joint capsule.

The load bearing cable 10 of the present invention is substituted for surgical wire in repair of patella fractures. The cable material is wrapped tightly around the patella 40 with two ends 46 tied together tightly to provide compressive force. The cable has sufficient tensile strength to maintain the patella fragments in close approximation and promote active healing, and is sufficiently inelastic to

- 19 -

prevent separation of the patella fragments under tensile loading. The load bearing cable is less susceptible to fatigue failure than surgical wire. In the event the cable does fail, no threat of damage to surrounding tissues is posed.

When the cable is formed of a bioresorbable polymeric fibre, stress will gradually be transferred to the patella in a controlled manner, as the cable is resorbed, enhancing healing per Wolff's law, bone remodels in response to applied stress.

Example 6

Fusion of Spinal Vertebrae

Current procedures for repair or fusion of the spinal column restrict motion of vertebral bodies by fixing posterior elements of the vertebrae, transverse processes and pedicles, together, inserting a bone graft along the posterior surface of the spinal column, and then fixing the graft into position. Satisfactory fusion requires that the vertebrae remain sufficiently immobilised to permit healing of the bone graft to the vertebrae.

In general, surgical wire has been used in this procedure. Problems with the use of surgical wire in spinal fusions are similar to those encountered with the patella fusion described for Example 5, including wire breakage during insertion or tensioning, failure to maintain adequate compressive force, and fatigue of wire over time. In addition the proximity of the

- 20 -

spinal cord to the fusion site makes the consequences of wire breakage life threatening.

These problems are circumvented by use of the load bearing cable of the present invention as described in Example 5. As shown, for example in Figure 1, the surgical cable 10 of the present invention is substituted for surgical wire in the fixation of the posterior elements 50 of the vertebrae and fixation of the graft into position. The surgical cable of the present invention provides sufficient compression and tensile strength to maintain the vertebral processes and/or graft in close approximation for fusion and healing.

When a bioresorbable fibre cable is used, stresses transferred to the bone graft in a controlled manner as the cable is resorbed, resulting in enhanced healing and greater success rate.

Having described the invention above, various modifications of the techniques, procedures, material and equipment will be apparent to those in the art. It is intended that all such variations within the scope and spirit of the appended claims be embraced thereby.

- 21 -

CLAIMS

1. A load bearing cable comprising:
a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs.
2. A cable as claimed in claim 1, wherein the tensile strength of each polymeric fibre is greater than or equal to 500,000 psi.
3. A cable as claimed in either claims 1 or 2, wherein the braid diameter is less than or equal to 1mm.
4. A cable as claimed in any one of the preceding claims, wherein the polymeric fibre is formed of ultra-high molecular weight polyethylene.
5. A cable as claimed in any one of the preceding claims, wherein the polymeric fibres are formed of **SPECTRA-1000**.
6. A cable as claimed in any one of the preceding claims, comprising bioresorbable polymeric fibres.
7. A cable as claimed in any one of the preceding claims, wherein the braid is formed of from 1 to 6 ply at 650 denier per ply, of polymeric fibres.
8. A cable as claimed in claim 7, wherein the braid

- 22 -

is formed of a single ply of polymeric fibres.

9. A cable as claimed in claim 7, wherein the braid is formed of two ply polymeric fibres.

10. A cable as claimed in any one of the preceding claims, wherein the braid has a weave angle that will provide 5 to 7 picks per inch.

11. A cable as claimed in any one of the preceding claims, further comprising:

a needle attached to at least one end of the longitudinal axis of the cable.

12. A cable as claimed in any one of the preceding claims, wherein the needle is attached to only one end of the cable.

13. A method for the repair of torn ligaments and tendons comprising:

opposing torn ends of a ligament or a tendon with a load bearing cable comprising:

a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs.

14. A method as claimed in claim 13 wherein the cable is additionally sewn through a tissue graft.

- 23 -

15. A method for the repair of fractures or fusions of small bones comprising:

bringing bone fragments or bone elements into close approximation and applying compressive force thereon by winding a load bearing cable comprising:

a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs,

about or through opposed bone fragments or bone elements and tightly securing together the ends of the cable.

16. A method as claimed in claim 15 wherein the securing together of the ends of the cable is by knotting.

17. A method as claimed in claim 15 wherein the securing together of the ends of the cable is by fusing using heat.

18. A method as claimed in claim 17 wherein a load bearing cable comprising:

a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs, has been treated to

- 24 -

roughen the surface of the cable.

19. A method as claimed in any one of claims 13 to 18 wherein a load bearing cable comprising:

a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs, is applied to fragments of the patella.

20. A method as claimed in any one of claims 13 to 18 wherein a load bearing cable comprising:

a hollow braid having a longitudinal axis, the hollow braid being formed of a plurality of polymeric fibres, each polymeric fibre having a tensile strength greater than or equal to 300,000 psi, wherein the braid has a diameter of less than or equal to 3mm and wherein said braided cable can withstand a load of approximately 300 to 550 lbs, is applied to the fusion of adjacent vertebrae of the spinal column.

21. A method for the repair of opposed fractures of small bones or for enabling fusions of small bones, comprising the steps of:

- a) positioning opposed bone fragments or elements into close approximation with each other;
- b) applying a compressive force between the opposed bone fragments or elements by utilizing a surgical cable formed of polymeric material to force the opposed bone fragments or elements toward each

- 25 -

other, the polymeric cable being flexible and capable of bearing sufficient stress loads to repair or fuse the opposing bone fragments or elements, and to be sufficiently inelastic for maintaining continuous pressure on the bone fragments or elements; and

c) securing the cable in place relative to the bone fragments or elements.

22. A method as claimed in claim 21, wherein the step of positioning bone fragments or elements further includes positioning adjacent vertebrae of the spinal column.

23. A method as claimed in claim 21, wherein the step of positioning bone fragments or elements further includes positioning fragments of the patella.

24. A method as claimed in any of claims 21 to 23, wherein the polymeric cable has a diameter of less than or equal to 3mm, is capable of withstanding a load of up to 550 lbs, and the tensile strength of each polymeric fibre is greater than or equal to 500,000 psi.

25. A method as claimed in any of claims 21 to 24, wherein the polymeric cable is formed of braided strands of polymeric fibre.

26. A method as claimed in any one of claims 21 to 25, wherein the polymeric material is formed of ultra high molecular weight polyethylene fibres.

27. A method as claimed in claim 26 wherein the

- 26 -

polymeric fibres are formed of **SPECTRA 1000**.

28. A method as claimed in any of claims 21 to 26, wherein the polymeric material is bioresorbable.

29. A method as claimed in any one of claims 21 to 28, wherein the step of applying a compressive force further includes wrapping the polymeric cable around the opposed bone fragments or elements to fuse them together.

30. A method as claimed in any one of claims 21 to 29, wherein the step of securing the cable further includes knotting the ends of the cable together.

31. A method as claimed in any one of claims 21 to 29, wherein the step of securing the cable further includes fusing the ends of the cable together with heat.

32. A method as claimed in any one of claims 21 to 29, wherein the step of securing the cable further includes attachment to bone with an attachment means, the attachment means including surgical staples, pins and screws.

33. A method for the repair of fractures of the vertebrae or for enabling fusions of adjacent vertebrae, comprising the steps of:

a) positioning the adjacent vertebrae or vertebrae fragments into close approximation with each other;

b) applying a compressive force between the

- 27 -

adjacent vertebrae or fragments by utilizing a surgical cable formed of polymeric material to force the adjacent vertebrae or fragments toward each other, the polymeric cable being flexible and capable of bearing sufficient stress loads to repair or fuse the adjacent vertebrae or fragments, and to be sufficiently inelastic for maintaining continuous pressure on the vertebrae or fragments; and

c) securing the cable in place relative to the vertebrae or fragments.

34. A method as claimed in claim 33, wherein the polymeric cable has a diameter of less than or equal to 3mm, is capable of withstanding a load of up to 550 lbs, and the tensile strength of each polymeric fibre is greater than or equal to 500,000 psi.

35. A method as claimed in either claim 33 or 34, wherein the polymeric material is formed of braided strands of polymeric fibre.

36. A method as claimed in any one of claims 33 to 35, wherein the polymeric material is formed of ultra high molecular weight polyethylene fibres.

37. A method as claimed in claim 36, wherein the polymeric fibres are formed of **SPECTRA 1000**.

38. A method as claimed in any one of claims 33 to 35, wherein the polymeric material is bioresorbable.

39. A method as claimed in any one of claims 33 to 38, wherein the step of applying a compressive force

- 28 -

further includes wrapping the polymeric cable around the adjacent vertebrae or fragments to fuse them together.

40. A method as claimed in claim 33, wherein the step of securing the cable further includes knotting the ends of the cable together.

41. A method as claimed in any of claims 33 to 39, wherein the step of securing the cable further includes fusing the ends of the cable together with heat.

42. A method as claimed in any of claims 33 to 39, wherein the step of securing the cable further includes attachment to bone with an attachment means, the attachment means including surgical staples, pins and screws.

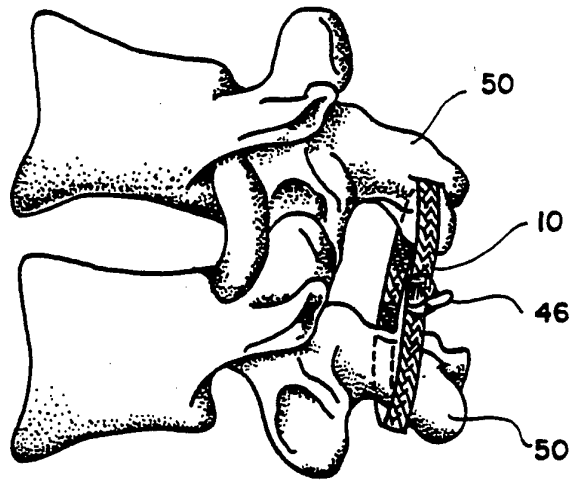


FIG. 1

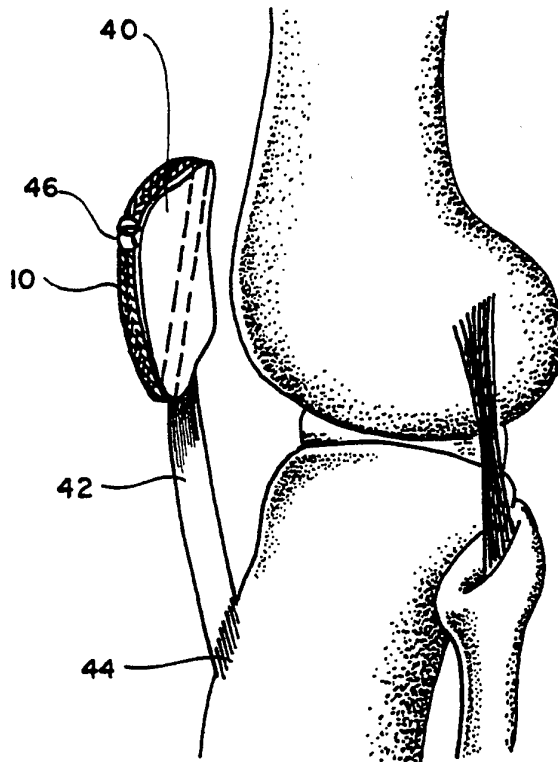


FIG. 2

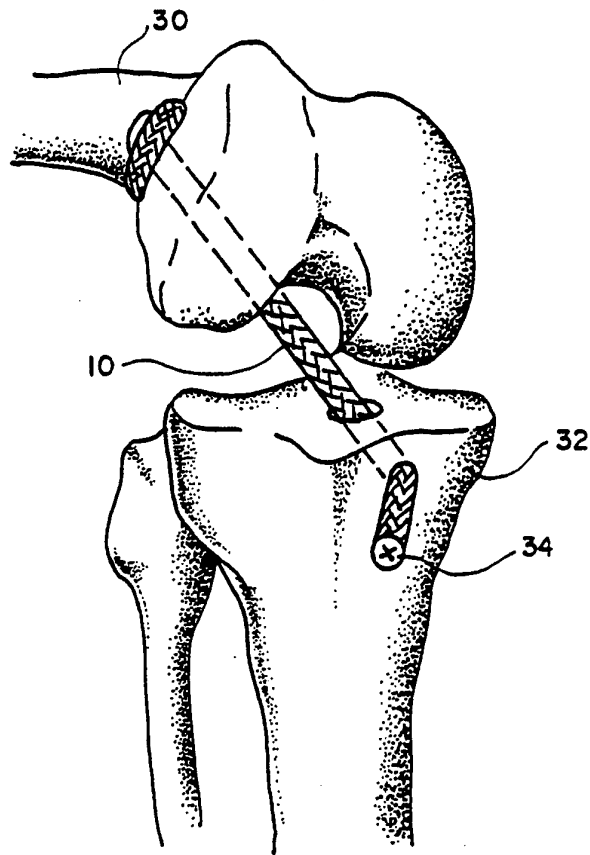


FIG. 3

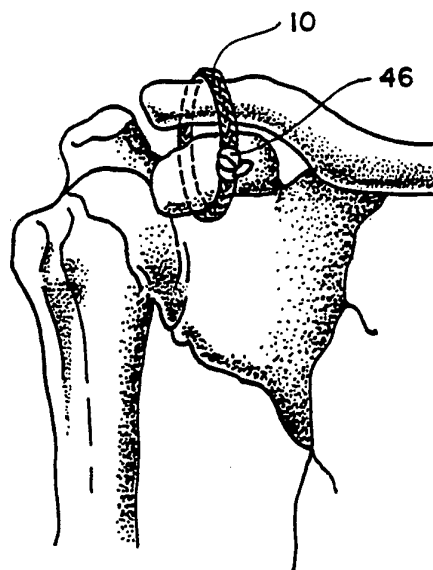


FIG. 4

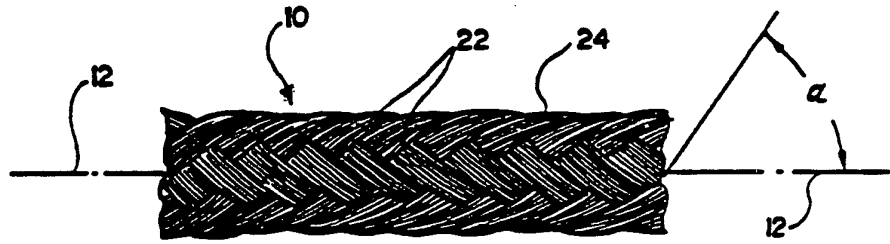


FIG. 5

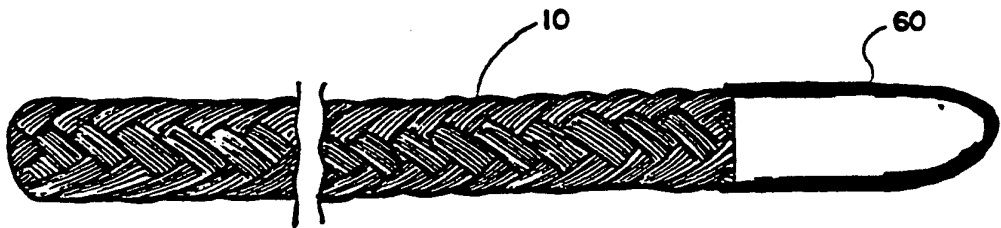


FIG. 6

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US94/00191

A. CLASSIFICATION OF SUBJECT MATTER
 IPC(S) :A61F 2/08
 US CL :623/13, 17
 According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
 Minimum documentation searched (classification system followed by classification symbols)
 U.S. : 623/1, 13, 17, 66; 87/6, 8; 606/224-228

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
 None

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
 None

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US, A, 4,932,972, (Dunn et al.), 12 June 1990. See column 6, lines 7-44	1-10, 21, 23, 25-28, 32
Y	US, A, 4,942,875, (Hlavacek et al.), 24 July 1990. See Abstract of Disclosure.	11-20, 22, 24, 29-31, 33-42
Y	US, A, 5,061,283, (Silvestrini), 29 October 1991. See Abstract of Disclosure.	11-20
A	US, A, 4,790,850, (Dunn et al.), 13 December 1988. See Abstract of Disclosure.	1-42

Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be part of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search 16 MARCH 1994	Date of mailing of the international search report 05 MAY 1994
--	---

Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. (703) 305-3230	Authorized officer <i>Gary Jackson</i> FOR GARY JACKSON Telephone No. (703) 308-4302
---	--