



US 20030229391A1

(19) **United States**
(12) **Patent Application Publication** (10) **Pub. No.: US 2003/0229391 A1**
Thompson (43) **Pub. Date: Dec. 11, 2003**

(54) **STENT**

is a continuation of application No. 09/049,486, filed on Mar. 27, 1998, now Pat. No. 6,132,460.

(76) Inventor: **Paul J. Thompson, New Hope, MN (US)**

Publication Classification

Correspondence Address:
MERCHANT & GOULD PC
P.O. BOX 2903
MINNEAPOLIS, MN 55402-0903 (US)

(51) **Int. Cl.⁷** **A61F 2/06**
(52) **U.S. Cl.** **623/1.17**

(57) **ABSTRACT**


(21) Appl. No.: **10/389,273**

(22) Filed: **Aug. 14, 2003**

Related U.S. Application Data

(63) Continuation of application No. 09/765,725, filed on Jan. 18, 2001, now Pat. No. 6,558,415, which is a continuation-in-part of application No. 09/545,810, filed on Apr. 7, 2000, now Pat. No. 6,358,274, which

The present disclosure relates to a stent including a stent body having a stent axis. The stent body includes structural members defining openings through the stent body. The structural members are provided with regions having different widths. The relative sizes of the widths are selected to control the length of the stent body as the stent body is radially expanded from an un-deployed orientation to a deployed orientation. In one embodiment, the regions having different widths are provided by tapering the widths of selected segments of the structural member.

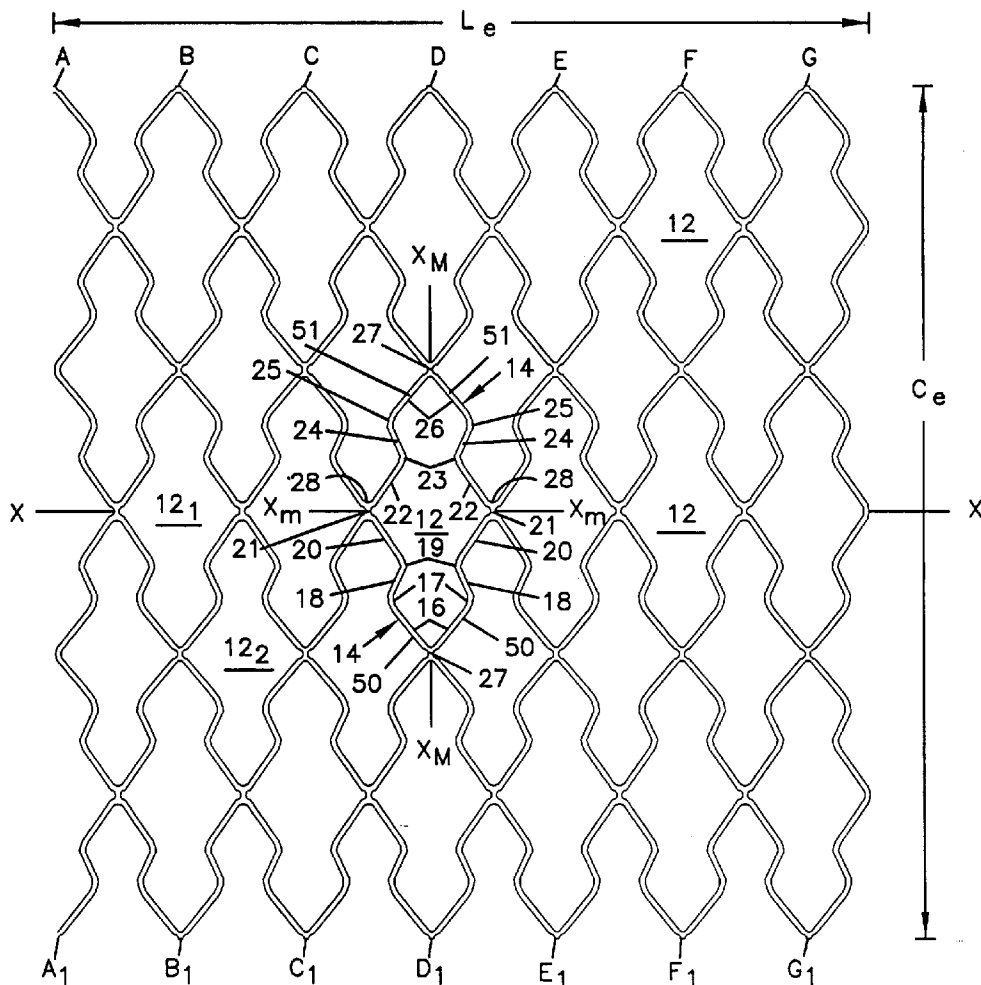

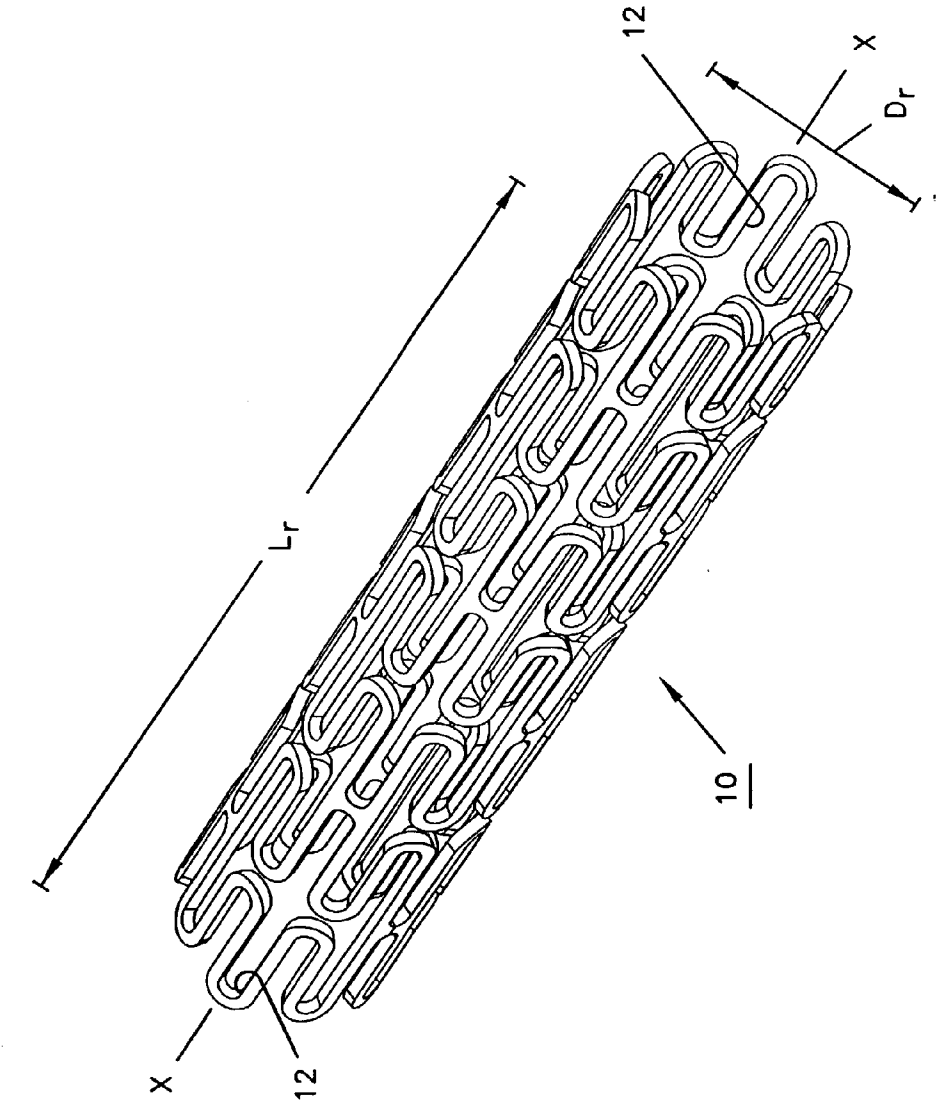
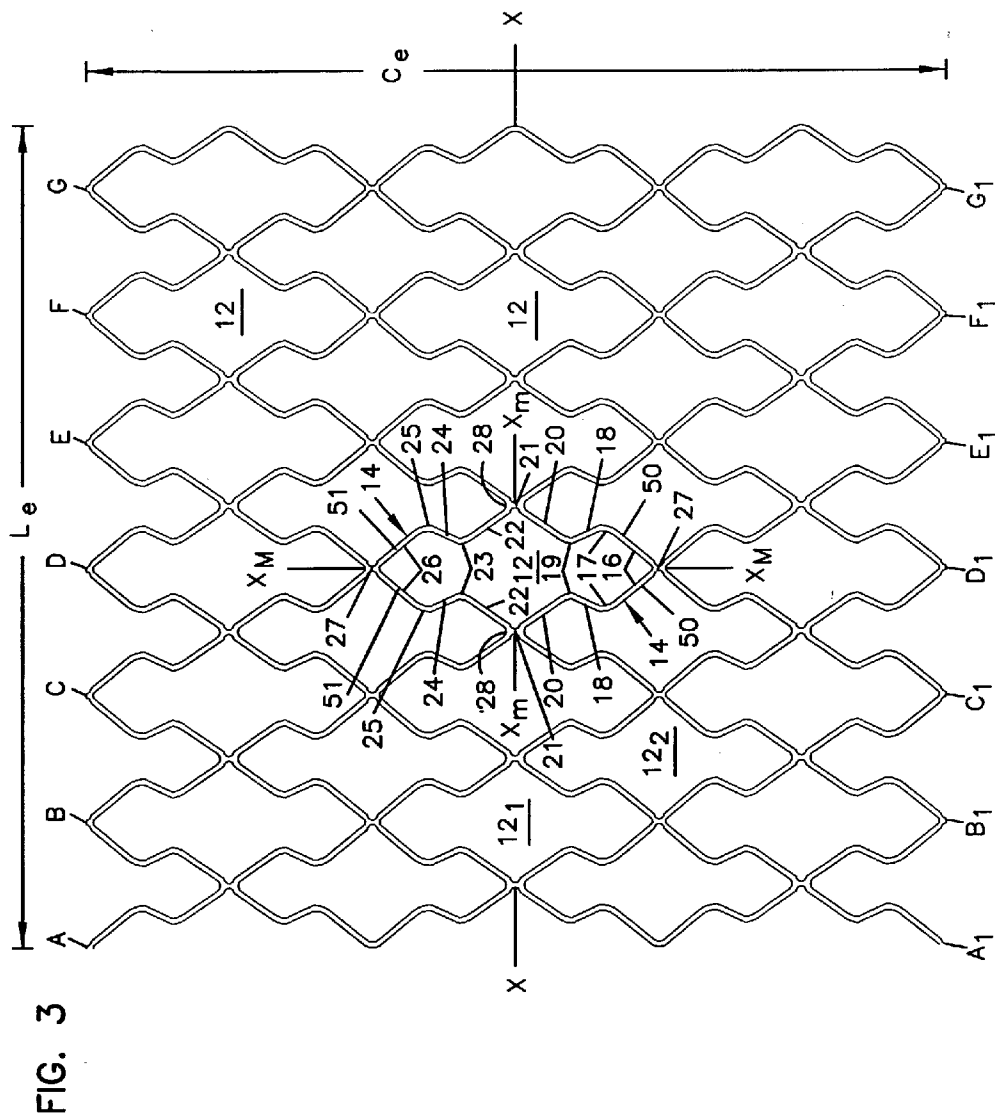


FIG. 1



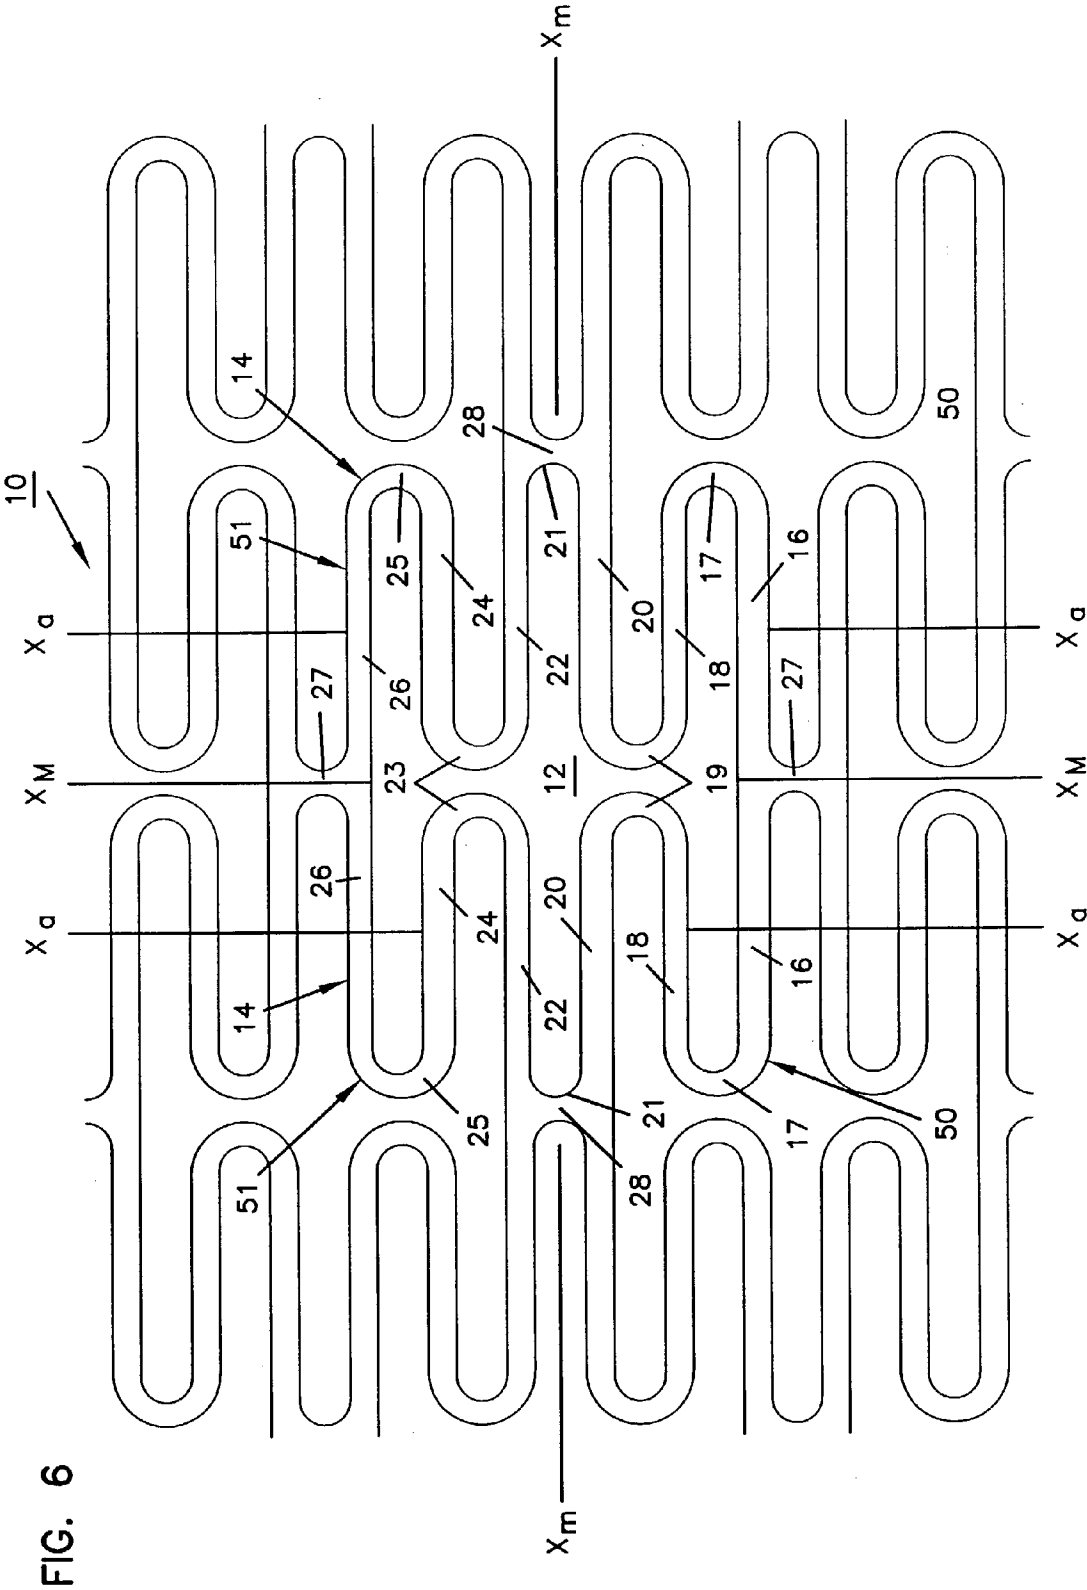


FIG. 7

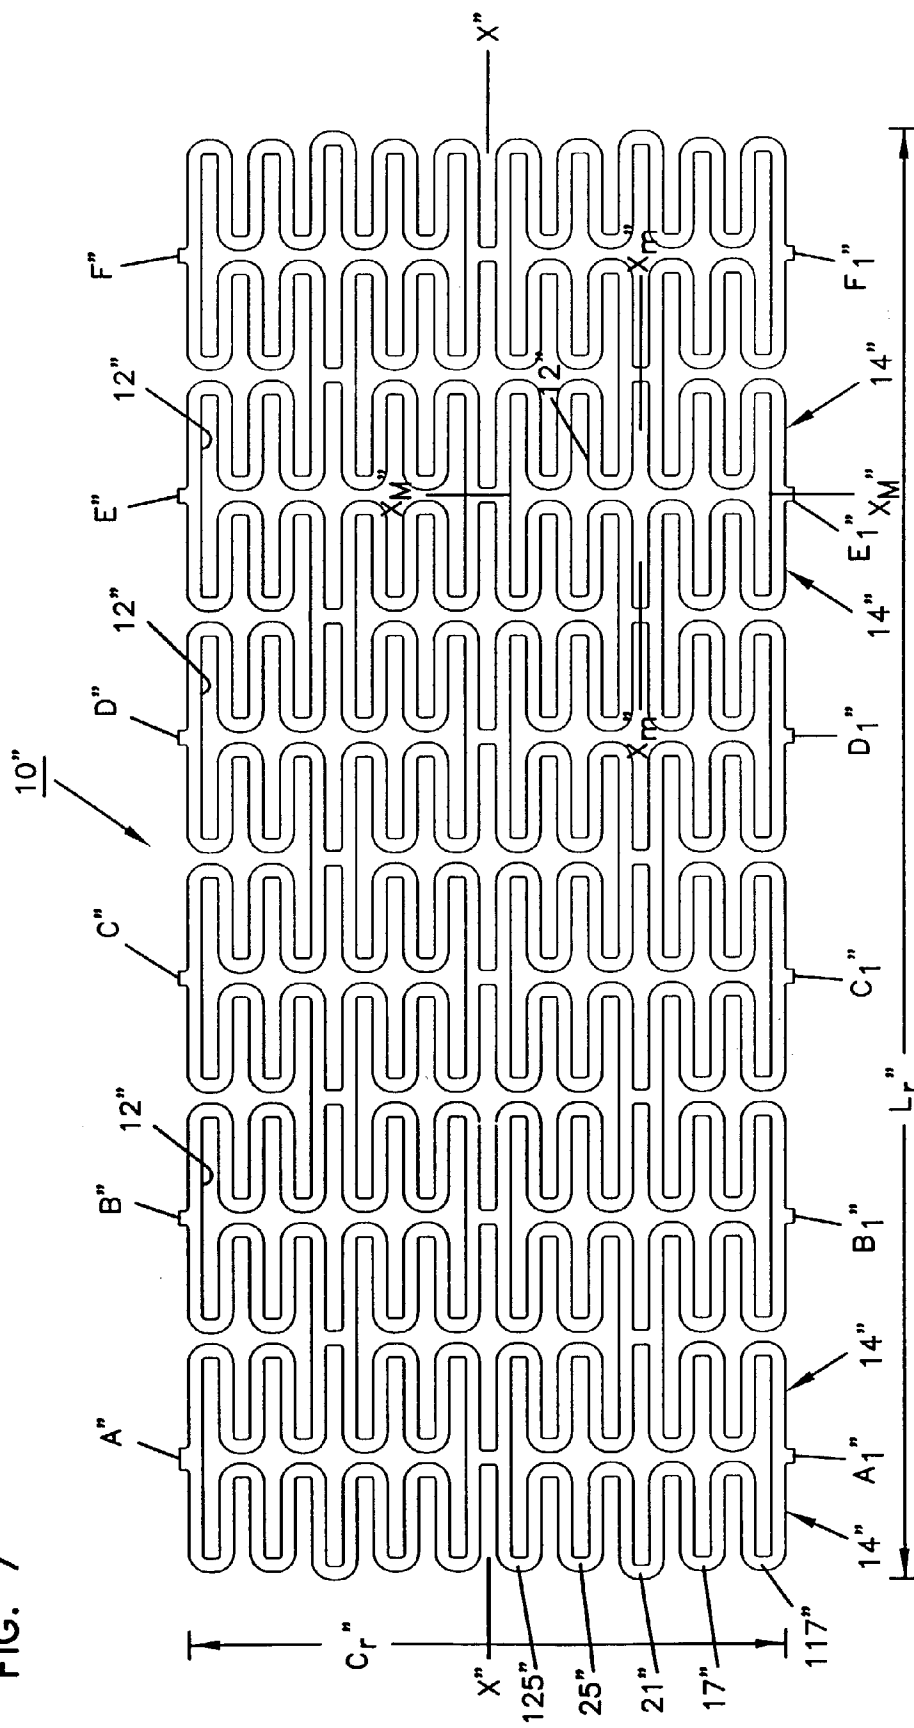


FIG. 9



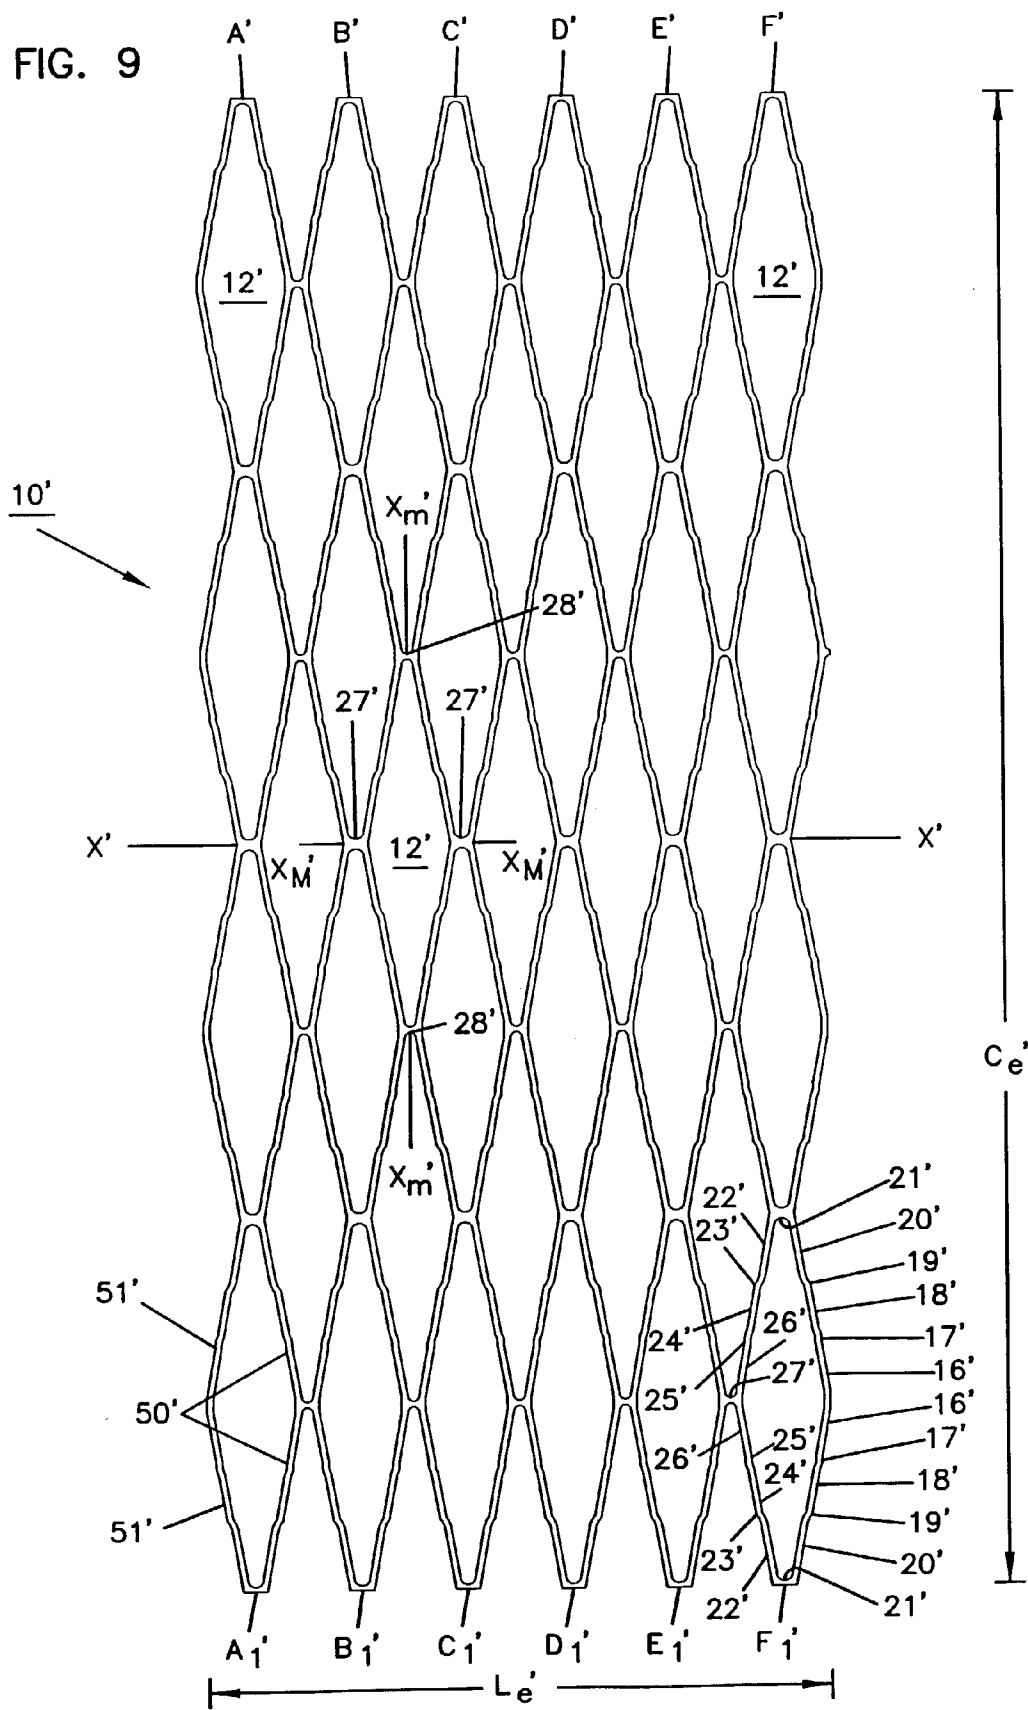


FIG.10

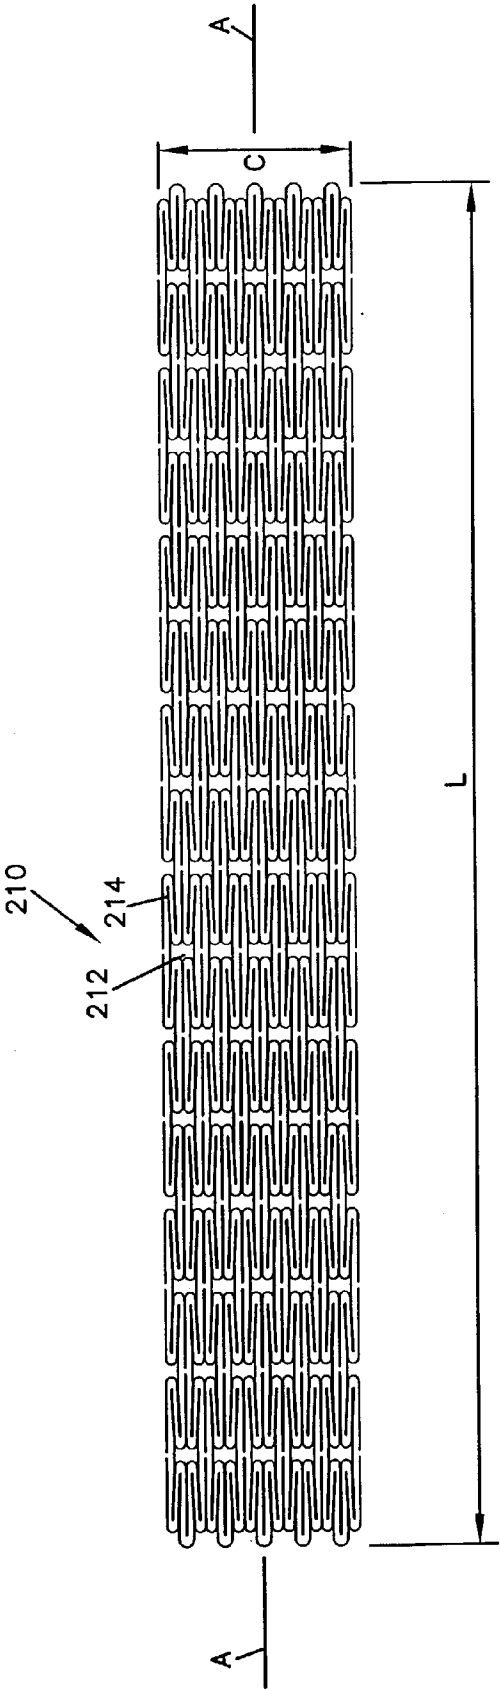

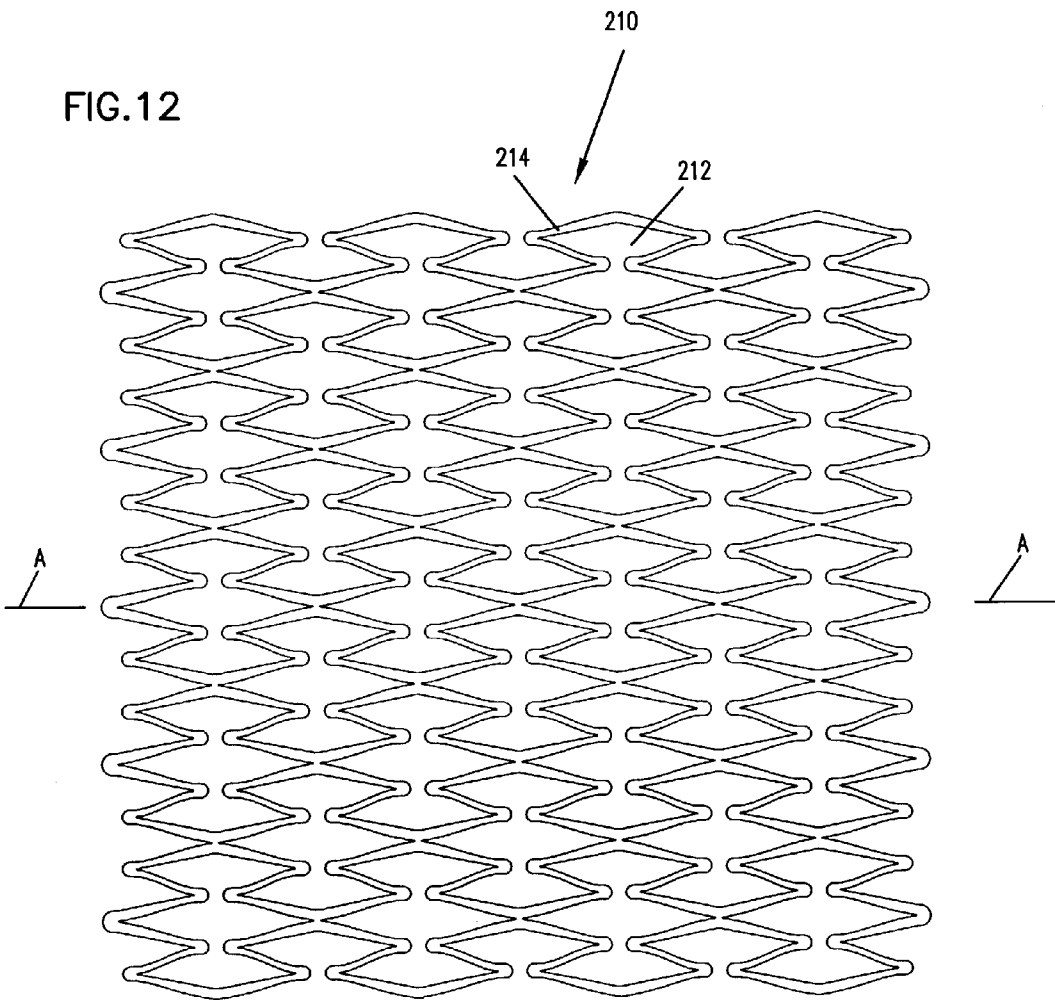

STENT

I.

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation-in-part of co-pending and commonly assigned U.S. patent application Ser. No. 09/545,810 which is a continuation of commonly assigned U.S. patent application Ser. No. 09/049,486 filed Mar. 27, 1998, now U.S. Pat. No. 6,132,460.

II.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] This invention pertains to stents for use in intraluminal applications. More particularly, this invention pertains to a novel structure for such stents.

[0004] 2. Description of the Prior Art

[0005] Stents are widely used for numerous applications where the stent is placed in the lumen of a patient and expanded. Such stents may be used in coronary or other vasculature, as well as other body lumens.

[0006] Commonly, stents are cylindrical members. The stents expand from reduced diameters to enlarged diameters. Frequently, such stents are placed on a balloon catheter with the stent in the reduced-diameter state. So placed, the stent is advanced on the catheter to a placement site. At the site, the balloon is inflated to expand the stent to the enlarged diameter. The balloon is deflated and removed, leaving the enlarged diameter stent in place. So used, such stents are used to expand occluded sites within a patient's vasculature or other lumen.

[0007] Examples of prior art stents are numerous. For example, U.S. Pat. No. 5,449,373 to Pinchasik et al. teaches a stent with at least two rigid segments joined by a flexible connector. U.S. Pat. No. 5,695,516 to Fischell teaches a stent with a cell having a butterfly shape when the stent is in a reduced-diameter state. Upon expansion of the stent, the cell assumes a hexagonal shape.

[0008] In stent design, it is desirable for the stent to be flexible along its longitudinal axis to permit passage of the stent through arcuate segments of a patient's vasculature or other body lumen. Preferably, the stent will have at most minimal longitudinal shrinkage when expanded and will resist compressive forces once expanded.

III.

SUMMARY OF THE INVENTION

[0009] The present disclosure relates to a stent including a stent body having a stent axis. The stent body includes structural members that define openings through the stent body. The structural members are provided with regions having different widths. The relative sizes of the widths are selected to control the length of the stent body as the stent body is radially expanded from an un-deployed orientation to a deployed orientation. In one embodiment, the regions having different widths are provided by tapering the widths

of selected segments of the structural member. In a preferred embodiment, the relative sizes of the widths are selected to minimize or eliminate length changes as the stent body is expanded from the un-deployed orientation to the expanded orientation.

IV.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] FIG. 1 is a perspective view of a first embodiment of a stent according to the present invention shown in a rest diameter state and showing a plurality of stent cells each having a major axis perpendicular to an axis of the stent;

[0011] FIG. 2 is a plan view of the stent of FIG. 1 as it would appear if it were longitudinally split and laid out flat;

[0012] FIG. 3 is the view of FIG. 2 following expansion of the stent to an enlarged diameter;

[0013] FIG. 4 is a view taken along line 4-4 in FIG. 2;

[0014] FIG. 5 is a view taken along line 5-5 in FIG. 2;

[0015] FIG. 6 is an enlarged view of a portion of FIG. 2 illustrating a cell structure with material of the stent surrounding adjacent cells shown in phantom lines;

[0016] FIG. 7 is the view of FIG. 2 showing an alternative embodiment of the present invention with a cell having five peaks per longitudinal segment;

[0017] FIG. 8 is the view of FIG. 2 showing an alternative embodiment of the present invention with a major axis of the cell being parallel to an axis of the stent; and

[0018] FIG. 9 is the view of FIG. 8 following expansion of the stent to an enlarged diameter;

[0019] FIG. 10 is a plan view of another stent as it would appear if it were longitudinally split and laid out flat;

[0020] FIG. 11 is an enlarged view of a portion of the stent of FIG. 10; and

[0021] FIG. 12 is a plan view of a portion of the stent of FIG. 10 in a deployed/expanded orientation, the stent has been longitudinally cut and laid flat.

V.

DESCRIPTION OF THE PREFERRED EMBODIMENT

[0022] Referring now to the several drawing figures in which identical elements are numbered identically, a description of the preferred embodiment of the present invention will now be provided. Where several embodiments are shown, common elements are similarly numbered and not separately described with the addition of apostrophes to distinguish the embodiments.

[0023] FIG. 1 illustrates a stent 10 having a rest length L_r and an un-deployed or reduced diameter D_r . For ease of illustration, the stent 10 is shown flat in FIG. 2 which illustrates a rest circumference C_r ($C_r = \pi D_r$). In FIG. 2, locations A, B, C, D, E, F and G are shown severed from their normally integrally formed locations A_1 , B_1 , C_1 , D_1 , E_1 , F_1 and G_1 . This permits the stent 10 to be shown as if it were severed at normally integrally formed locations A- A_1 , B- B_1 , C- C_1 , D- D_1 , E- E_1 , F- F_1 and G- G_1 and laid flat. FIG.

6 is an enlarged portion of the view of FIG. 2 to better illustrate a novel cell structure as will be described. The stent 10 is a reticulated, hollow tube. The stent 10 may be expanded from the rest diameter D_r (and corresponding rest circumference C_r) to an expanded or enlarged diameter. FIG. 3 is a view similar to FIG. 2 (i.e., illustrating the expanded stent 10 as it would appear if longitudinally split and laid flat). Since FIG. 3 is a two-dimensional representation, the enlarged diameter is not shown. However, the enlarged circumference C_e is shown as well as a length L_e following expansion. The expanded diameter is equal to C_e/π .

[0024] As will be discussed length L_e is preferably not more than minimally smaller (e.g., less than 10% smaller) than length L_r . Ideally, L_e equals L_r .

[0025] The material of the stent 10 defines a plurality of cells 12. The cells 12 are bounded areas which are open (i.e., extend through the wall thickness of the stent 10). The stent 10 may be formed through any suitable means including laser or chemical milling. In such processes, a hollow cylindrical tube is milled to remove material and form the open cells 12.

[0026] The cells 12 have a longitudinal or major axis X_M-X_M and a transverse or minor axis X_m-X_m . In the embodiments of FIGS. 1-3, the major axis X_M-X_M is perpendicular to the longitudinal cylindrical axis $X-X$ of the stent 10. In the embodiments of FIGS. 8 and 9, the major axis X_M-X_M is parallel to the longitudinal cylindrical axis $X-X$ of the stent 10. The cell 12 is symmetrical about axes X_M-X_M and X_m-X_m .

[0027] The cell 12 is defined by portions of the tube material including first and second longitudinal segments 14. The segments 14 each have a longitudinal axis X_a-X_a as shown in FIG. 6. The segments' longitudinal axes X_a-X_a are parallel to and positioned on opposite sides of the cell major axis X_M-X_M .

[0028] Each of longitudinal segments 14 has an undulating pattern to define a plurality of peaks 17, 21, 25 and valleys 19, 23. The peaks 17, 21, 25 are spaced outwardly from the longitudinal axes X_a-X_a and the valleys 19, 23 are spaced inwardly from the longitudinal axes X_a-X_a . As used in this context, "inward" and "outward" mean toward and away from, respectively, the cell's major axis X_M-X_M .

[0029] Each of the peaks 17, 21, 25 and valleys 19, 23 is a generally semi-circular arcuate segment. The peaks 17, 21, 25 and valleys 19, 23 are joined by parallel and spaced-apart straight segments 16, 18, 20, 22, 24 and 26 which extend perpendicular to the major axis X_M-X_M . Linearly aligned straight end portions 16, 26 of opposing segments 14 are joined at first and second longitudinal connection locations 27 spaced apart on the major axis X_M-X_M . First and second transverse connection locations 28 are spaced apart on the minor axis X_m-X_m . The first and second transverse connection locations 28 are positioned at the apices of the center peaks 21 of the longitudinal segments 14.

[0030] Except as will be described, the segments 14 have uniform cross-sectional dimensions throughout their length as illustrated in FIG. 4. By way of non-limiting example, the width W and thickness T of the straight line segments 16, 18, 20, 22, 24 and 26 are about 0.0065 inch (about 0.16 mm) and about 0.0057 inch (about 0.14 mm), respectively.

[0031] For reasons that will be described, the width W' (FIG. 5) at the apices of the peaks 17, 21, 25 and valleys 19, 23 is narrower than width W (in the example given, narrow width W' is about 0.0055 inch or about 0.13 mm). The width of the peaks 17, 21, 25 and valleys 19, 23 gradually increases from width W' at the apices to width W at the straight segments 16, 18, 20, 22, 24 and 26. At the longitudinal and transverse connection locations 27, 28, the width W_c (shown in FIG. 2) is preferably equal to or less than the common width W .

[0032] The combined lengths of segments 16-20 to the apex of peak 21 represent a path length 50 from longitudinal connection location 27 to transverse connection location 28. Similarly the combined lengths of the other arcuate and straight segments 22-26 to the apex of peak 21 represent identical length path lengths 51 of identical geometry from longitudinal connection locations 27 to transverse connection locations 28. Each of the path lengths 50, 51 is longer than a straight-line distance between the transverse and longitudinal connection locations 27, 28. As will be described, the straight-line distance between the transverse and longitudinal connection locations 27, 28 increases as the diameter of the stent 10 is expanded. The path lengths 50, 51 are sized to be not less than the expanded straight-line distance.

[0033] The stent 10 includes a plurality of identical cells 12. Opposite edges of the segments 14 define obliquely adjacent cells (such as cells 12₁, 12₂ in FIG. 2). Cells 12 having major axes X_M-X_M collinear with the major axis X_M-X_M of cell 12 are interconnected at the longitudinal connection locations 27. Cells having minor axes collinear with the minor axis X_m-X_m of cell 12 are interconnected at the transverse connection locations 28.

[0034] As mentioned, the stent 10 in the reduced diameter of FIG. 1 is advanced to a site in a lumen. The stent 10 is then expanded at the site. The stent 10 may be expanded through any conventional means. For example, the stent 10 in the reduced diameter may be placed on the balloon tip of a catheter. At the site, the balloon is expanded to generate radial forces on the interior of the stent 10. The radial forces urge the stent 10 to radially expand without appreciable longitudinal expansion or contraction. Plastic deformation of the material of the stent 10 (e.g., stainless steel) results in the stent 10 retaining the expanded shape following subsequent deflation of the balloon. Alternatively, the stent 10 may be formed of a super-elastic or shape memory material (such as nitinol—a well-known stent material which is an alloy of nickel and titanium).

[0035] As the stent 10 expands, the path lengths 50, 51 straighten to accommodate the expansion. FIG. 3 illustrates the straightening of the path lengths 50, 51. In FIG. 3, the stent 10 has been only partially expanded to an expanded diameter less than a maximum expanded diameter. At a maximum expanded size, the path lengths 50, 51 are fully straight. Further expansion of the stent 10 beyond the maximum expanded size would result in narrowing of the minor axis X_m-X_m (i.e., a narrowing of a separation between the transverse connection locations and a resulting narrowing of the length L_r of the stent) or would require stretching and thinning of the stent material.

[0036] As shown in FIG. 3, during expansion of the stent 10, the straight segments 16, 18, 20, 22, 24 and 26 are substantially unchanged. The straightening of the path lengths 50, 51 results in bending of the arcuate peaks 17, 21, 25 and valleys 19, 23. Since the width W' of the peaks 17, 21, 25 and valleys 19, 23 is less than the width W of the straight segments 16, 18, 20, 22, 24 and 26, the arcuate peaks 17, 21, 25 and valleys 19, 23 are less stiff than the straight segments 16, 18, 20, 22, 24 and 26 and, therefore, more likely to deform during expansion.

[0037] As the stent 10 expands, the cells 12 assume a diamond shape shown in FIG. 3. Since the expansion forces are radial, the length of the major axis X_M-X_M (i.e., the distance between the longitudinal connection locations 27) increases. The length of the minor axis X_m-X_m (and hence the length of the stent 10) remains unchanged.

[0038] The stent 10 is highly flexible. To advance to a site, the axis X-X of the stent 10 must bend to navigate through a curved lumen. Further, for placement at a curved site in a lumen, the stent 10 must be sufficiently flexible to retain a curved shape following expansion and to bend as the lumen bends over time. The stent 10, as described above, achieves these objections.

[0039] When bending on its axis X-X, the stent 10 tends to axially compress on the inside of the bend and axially expand on the outside of the bend. The present design permits such axial expansion and contraction. The novel cell geometry 12 results in an accordion-like structure which is highly flexible before and after radial expansion. Further, the diamond shape of the cells 12 after radial expansion resists constricting forces otherwise tending to collapse the stent 10.

[0040] Numerous modifications are possible. For example the stent 10 may be lined with either an inner or outer sleeve (such as polyester fabric or ePTFE) for tissue growth. Also, the stent may be coated with radiopaque coatings such as platinum, gold, tungsten or tantalum. In addition to materials previously discussed, the stent may be formed of any one of a wide variety of previous known materials including, without limitation, MP35N, tantalum, platinum, gold, Elgiloy and Phynox.

[0041] While three cells 12 are shown in FIG. 2 longitudinally connected surrounding the circumference C_r of the stent, a different number could be so connected to vary the properties of the stent 10 as a designer may elect. Likewise, while each column of cells 12 in FIG. 2 is shown as having three longitudinally connected cells 12, the number of longitudinally connected cells 12 could vary to adjust the properties of the stent. Also, while each longitudinal segment 14 is shown as having three peaks 17, 21, 25 per longitudinal segment 14, the number of peaks could vary. FIG. 7 illustrates a stent 10' with a cell 12' having five peaks 17', 21', 25' and 125' per longitudinal segment 14'. Preferably, the longitudinal segment will have an odd number of peaks so that the transverse connection points are at an apex of a center peak.

[0042] FIGS. 8 and 9 illustrate an alternative embodiment where the major axis $X_M'-X_M'$ of the cells 12' are parallel with the cylindrical axis X'-X' of the stent 10'. In FIG. 9, the expanded stent 10' is shown at a near fully expanded state where the path lengths 50', 51' are substantially linear.

[0043] When forming the stent from shape memory metal such as nitinol, the stent can be laser cut from a nitinol tube. Thereafter, the stent can be subjected to a shape-setting process in which the cut tube is expanded on a mandrel and then heated. Multiple expansion and heating cycles can be used to shape-set the stent to the final expanded diameter. Preferably, the final expanded diameter is equal to the desired deployed diameter of the stent. During expansion, the stent is preferably axially restrained such that the length of the stent does not change during expansion. The finished stent preferably has an austenite finish temperature less than body temperature. Thus, at body temperature, the stent will self-expand to the desired deployed diameter due to the shape memory characteristic of the metal forming the stent.

[0044] In use, the finished stent can be mounted on a delivery catheter. As is conventionally known in the art, the stent can be held in a compressed orientation on the delivery catheter by a retractable sheath. As is also known in the art, the delivery catheter can be used to advance the stent to a deployment location (e.g., a constricted region of a vessel). At the deployment site, the sheath is retracted thereby releasing the stent. Once released, the stent self-expands to the deployed diameter.

[0045] It has been noted that the lengths of prior art stents when mounted on a delivery catheter can be different from the deployed lengths of such stents. For example, it has been determined that the deployed lengths of the prior art stents are often shorter than the compressed orientation lengths (i.e., the lengths of the stents when mounted on a delivery catheter). Shortening can be problematic because shortening makes it more difficult for a physician to accurately place a stent at a desired position in a vessel.

[0046] An important aspect of the present invention relates to a stent design that reduces or eliminates shortening of a stent. For example, one embodiment of the present invention relates to a stent having the same length or substantially the same length at each of the following stages: 1) when the stent is initially cut from a tube of shape-memory alloy; 2) when the stent is shape-set to the desired expanded diameter; 3) when the stent is compressed on the delivery catheter; and 4) when the stent is deployed at a deployment location.

[0047] With respect to shape memory stents, it has been found that varying the width of the segments 16, 18, 20, 22, 24 and 26 controls whether the stent shortens, lengthens, or remains the same length during expansion from the compressed orientation (i.e., the reduced diameter orientation) to the deployed orientation. For example, the segments 26 and 16 are preferably constructed with enlarged widths adjacent the connection locations 27, and reduced widths adjacent their corresponding peaks 25 and 17. Similarly, the segments 22 and 20 are preferably constructed with enlarged widths adjacent the connection locations 28, and reduced widths adjacent their corresponding valleys 23 and 19. The relative sizes between the enlarged widths and the reduced widths controls whether the stent shortens, lengthens, or remains the same during expansion.

[0048] FIGS. 10-12 show a stent 210 having a cell structure adapted to limit any length changes that may occur as the stent is expanded from the compressed orientation to the deployed orientation. Preferably the length change between the compressed orientation and the deployed orientation is less than 5 percent. More preferably, the length change

between the compressed orientation and the deployed orientation is less than 2 percent. Most preferably, the stent **210** experiences substantially no length change as it is released from a delivery catheter and expanded from the compressed orientation to the deployed orientation.

[0049] FIG. 10 shows the stent **210** cut longitudinally along its length and laid flat. The stent **210** has a length L and a circumference C . FIG. 10 is representative of the stent **210** after the stent **210** has been laser cut from a shape-memory tube, but before the stent **210** has been shape-set to the expanded diameter. FIG. 12 shows a portion of the stent **210** after the stent has been shape-set to the desired expanded diameter. In both FIGS. 10 and 12, the stent **210** is elongated along axis A-A and includes a stent body (i.e., a three-dimensional structure) having cell defining portions that define plurality of cells **212**. After the stent **210** has been shape-set to the expanded diameter as shown in FIG. 12, the cells **212** are preferably more open than the cells **212** depicted in FIG. 10. However, while the circumference C increases, the length L preferably remains substantially the same at both diameters.

[0050] Referring to FIG. 11, the cell defining portions of the stent body include circumferential connection locations **227** and longitudinal connection locations **228**. "Circumferential connection locations" are locations where circumferentially adjacent cell defining structures, as defined relative to axis A-A, are connected together. "Longitudinal connection locations" are locations where longitudinally adjacent cell defining portions, as defined relative to the axis A-A, are connected together.

[0051] Referring still to FIG. 11, each cell defining portion includes two axially spaced-apart members **214** (i.e., members that are spaced-apart from one another along the axis A-A) that extend circumferentially about the axis A-A in an undulating pattern. The members **214** extend in the undulating pattern between the circumferential connection locations **227**. Adjacent the circumferential connection locations **227**, the ends of the undulating members **214** are connected to one another. At the longitudinal connection locations **228**, the undulating members **214** merge with the undulating members **214** of longitudinally adjacent cell defining portions.

[0052] Still referring to FIG. 11, each undulating member **214** is shown including: 1) a segment **226** that extends from connection location **227** to peak **225**; 2) a segment **224** that extends from peak **225** to valley **223**; 3) a segment **222** that extends from valley **223** to connection location **228**; 4) a segment **220** that extends from connection location **228** to valley **219**; 5) a segment **218** that extends from valley **219** to peak **217**; and 6) a segment **216** that extends from peak **217** to connection location **227**. The segments **216-226** preferably extend generally longitudinally along the stent **210**. The term "generally longitudinally" will be understood to mean that the segments **216-226** are closer to a parallel relationship relative to the axis A-A of the stent **210** than to a transverse relationship relative to the axis A-A of the stent **210**.

[0053] To prevent length changes during deployment of the stent, the segments **226** and **216** preferably include enlarged widths W_1 adjacent the connection locations **227**, and reduced widths W_2 adjacent their corresponding peaks **225** and **217**. Similarly, the segments **222** and **220** are

preferably constructed with enlarged widths W_1 adjacent the connection locations **228**, and reduced widths W_2 adjacent their corresponding valleys **223** and **219**. Preferably, widths of the segments **226**, **222**, **220** and **216** taper (i.e., narrow) continuously along their lengths. As is clear from FIG. 11, the widths of the segments are measured in a circumferential direction relative to the axis A-A.

[0054] Referring once again to FIG. 11, pairs of tapered segments **226** and **216** are provided at each circumferential connection location **227**, and pairs of tapered segments **222** and **220** are provided at each longitudinal connection location **228**. Each pair of tapered segments is defined by an inner cut **250** that is parallel to the axis A-A of the stent **210**, and two outer cuts **252** that are angled relative to the axis A-A of the stent **210**. Preferably, the outer cuts **252** diverge from one another as the cuts **252** extend toward their corresponding connection location **227** or **228**. The angled orientation of the cuts **252** causes the segments **224** and **218** which interconnect the pairs of tapered segments **226**, **216**, **222** and **220** to have a non-tapered configuration. Additionally, the angled orientation of the cuts **252** causes the segments **224** and **218** to be angled (i.e., skewed) relative to the axis A-A of the stent **210**.

[0055] The narrowing from width W_1 to W_2 results in a taper along the lengths of the segments **226**, **222**, **220** and **216**. Preferably, the taper has an angle B in the range of 0.5-5 degrees relative to the axis A-A of the stent **210**. More preferably, the taper angle B is in the range of 1-3 percent. It has been found that the relative sizes of W_1 and W_2 have an effect on the deployed length of the stent **210** (i.e., the length of the stent after deployment in a vessel) as compared to the compressed length of the stent **210** (i.e., the length of the stent when mounted on a delivery catheter). As a result, in the design of the stent, the widths W_1 and W_2 can be selected to effect a desired change in length including no change in length if so desired. For example, a stent having a 5 millimeter cell length L_c (labeled on FIG. 11), a first width W_1 of 0.0065 inch and a second width W_2 of 0.0059 inch, has been found to lengthen about 10% during expansion from the compressed orientation to the deployed orientation. Alternatively, a stent having a 5 millimeter cell length L_c (labeled on FIG. 11), a first width W_1 of 0.009 and a second width W_2 of 0.0047, has been found to shorten about 10% during expansion from the compressed orientation to the deployed orientation. Further, a stent with a 5 millimeter cell length L_c (labeled on FIG. 11), a first width W_1 of 0.008 inches, a second width W_2 of 0.0052 inches and an angle B of two degrees has been found to experience no lengthening and no shortening when expanded from the compressed orientation and the deployed orientation.

[0056] While a preferred use for the inventive features disclosed in FIGS. 10-12 is in a self-expanding stent, the features also have benefits when used with non-self-expanding stents (e.g., balloon expandable stents made of a material such as stainless steel). Also, while FIGS. 10-12 illustrate a preferred geometry for practicing the present invention, the technique for controlling length variations by varying the widths of selected portions of a stent is also applicable to stents having other geometries, shapes, or strut patterns. Further, the various aspects of the present invention can also be used to cause a desired shortening or lengthening of a stent during deployment.

[0057] From the foregoing, the present invention has been shown in a preferred embodiment. Modifications and equivalents are intended to be included within the scope of the appended claims.

What is claimed is:

1. A stent comprising:
 - a stent body having a stent axis;
 - the stent body including a structural member extending in an undulating pattern about a circumference of the stent body;
 - the structural member including a plurality of segments that extend generally longitudinally along the stent axis; and
 - at least some of the segments having widths that taper as the at least some segments extend longitudinally along the stent axis.
2. The stent of claim 1, wherein a taper angle of the widths is selected to minimize a length change of the stent body as the stent body is radially expanded from an un-deployed orientation to a deployed orientation.
3. The stent of claim 1, wherein the at least some segments include pairs of tapered segments, the pairs of tapered segments being interconnected by non-tapered segments.
4. The stent of claim 3, wherein the non-tapered segments are skewed relative to the stent axis.
5. The stent of claim 1, wherein the segments are substantially straight.
6. The stent of claim 1, wherein the stent body is made of a shape-memory metal.
7. A stent comprising:
 - a stent body having a stent axis;
 - the stent body including a plurality of cell structures defining a plurality of cells;
 - the cell structures including structural members that extend in an undulating pattern about a circumference of the stent body;
 - the structural members including segments that extend generally longitudinally along the stent axis;
 - the structural members including peaks and valleys;
 - the cell structures being interconnected at connection locations;
 - at least some of the segments extending from the connection locations to the peaks and valleys; and
 - the at least some segments having enlarged first widths adjacent the connection locations as compared to smaller second widths located adjacent the peaks and valleys.
8. The stent of claim 7, wherein the at least some of the segments are provided with a narrowing width taper that extends between the first and second widths.
9. The stent of claim 7, wherein the relative sizes of the first and second widths are selected to minimize a length change of the stent body as the stent body is radially expanded from an un-deployed orientation to a deployed orientation.

10. The stent of claim 7, wherein the at least some segments include pairs of tapered segments positioned at the connection locations, the pairs of tapered segments being interconnected by non-tapered segments.

11. The stent of claim 10, wherein the non-tapered segments are skewed relative to the stent axis.

12. The stent of claim 7, wherein the segments are straight.

13. The stent of claim 7, wherein the connection locations include longitudinal connection locations and circumferential connection locations.

14. The stent of claim 13, wherein the cells are symmetrical about first axes extending through the circumferential connection locations, and the cells are also symmetrical about second axes extending through the longitudinal connection locations.

15. A stent comprising:

a stent body having a stent axis;

the stent body including a structural member extending in an undulating pattern about a circumference of the stent body;

the structural member including peaks and valleys, and also including segments that interconnect the peaks and valleys; and

at least some of the segments having widths that taper along lengths of the at least some segments.

16. The stent of claim 15, wherein the segments are substantially straight.

17. The stent of claim 15, wherein the structural members form cell structures that are interconnected at connection locations, and wherein the at least some segments have larger widths adjacent the connection locations than adjacent the peaks and valleys.

18. The stent of claim 15, wherein a taper angle of the widths is selected to control a length change of the stent body as the stent body is radially expanded from an un-deployed orientation to a deployed orientation.

19. The stent of claim 18, wherein the taper angle is selected to minimize a length change of the stent body as the stent body is expanded from the un-deployed orientation to the deployed orientation.

20. A stent comprising:

a stent body having a stent axis, the stent body being radially expandable from a non-deployed orientation having a first length to a deployed orientation having a second length;

the stent body including a structural member extending in an undulating pattern about a circumference of the stent body; and

the first length being substantially equal to the second length.

21. A method for making a stent, the method comprising:

constructing a stent body having a stent axis, the stent body including structural members defining openings through the stent body; and

during construction of the stent body, providing at least some of the structural members with regions having first and second different widths, the relative sizes of the first and second widths being selected to control a

length of the stent body as the stent body is radially expanded from an un-deployed orientation to a deployed orientation.

22. The method of claim 21, wherein the relative sizes of the widths are selected to minimize a length variation when the stent body is radially expanded from the un-deployed orientation to the deployed orientation.

23. The method of claim 21, further comprising providing the structural members with a gradual taper in width between the first and second widths.

24. The method of claim 23, wherein the segments are substantially straight.

25. The method of claim 21, further comprising shape-setting the stent body to an expanded diameter corresponding to the deployed orientation after the stent body has been constructed.

26. The method of claim 21, wherein the structural members extend in undulating patterns.

27. A stent comprising:

a stent body that is radially expandable from an un-deployed orientation to a deployed orientation;

the stent body including structural members defining openings through the stent body;

the structural members including segments having first regions with enlarged widths and second regions with more narrow widths; and

the relative sizes of the enlarged widths and the more narrow widths are selected to control a length of the stent body as the stent body is expanded from the un-deployed orientation to the deployed orientation.

28. The stent of claim 27, wherein the relative sizes of widths are selected to minimize a change in the length of the stent body as the stent body is expanded from the un-deployed orientation to the deployed orientation.

29. The stent of claim 27, wherein widths of the segments gradually taper between the enlarged widths and the more narrow widths.

30. The stent of claim 29, wherein the segments are substantially straight between the first regions and the second regions.

31. The stent of claim 30, wherein between the first and second regions, the segments extend in a generally longitudinal direction relative to an axis of the stent.

* * * * *