



US00D985773S

(12) **United States Design Patent**
Limem et al.

(10) **Patent No.:** **US D985,773 S**

(45) **Date of Patent:** **** May 9, 2023**

(54) **THREE DIMENSIONAL MASTOPEXY IMPLANT**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Tepha, Inc.**, Lexington, MA (US)

WO WO 2004/096098 A1 11/2004
WO WO 2006/117622 A1 11/2006

(Continued)

(72) Inventors: **Skander Limem**, Melrose, MA (US);
Emily Stires, Boston, MA (US);
Rebecca Marciante, North Reading,
MA (US); **Said Rizk**, Windham, NH
(US); **Arikha Moses**, Summit, NJ (US);
Fabio Felix, Foxborough, MA (US);
Bruce Van Natta, Westfield, IN (US)

OTHER PUBLICATIONS

European Search Report and Written Opinion dated Jul. 3, 2017 for
European Application No. 12754773.5.

(Continued)

(73) Assignee: **Tepha, Inc.**, Lexington, MA (US)

Primary Examiner — Charles D Hanson

(74) *Attorney, Agent, or Firm* — Wolf, Greenfield &
Sacks, P.C.

(**) Term: **15 Years**

(21) Appl. No.: **29/798,824**

(57) **CLAIM**

(22) Filed: **Jul. 10, 2021**

The ornamental design for a three dimensional mastopexy
implant, as shown and described.

Related U.S. Application Data

(62) Division of application No. 29/735,098, filed on May
18, 2020, now Pat. No. Des. 927,689, which is a
division of application No. 29/668,175, filed on Oct.
29, 2018, now Pat. No. Des. 888,244, which is a
division of application No. 29/542,048, filed on Oct.
9, 2015, now Pat. No. Des. 836,778.

DESCRIPTION

FIG. 1 is a front view of a three dimensional mastopexy
implant showing our new design;
FIG. 2 is a top view of the three dimensional mastopexy
implant shown in FIG. 1;
FIG. 3 is a side view of the three dimensional mastopexy
implant shown in FIG. 1;
FIG. 4 is a bottom view of the three dimensional mastopexy
implant shown in FIG. 1;
FIG. 5 is another side view of the three dimensional mas-
topexy implant shown in FIG. 1;
FIG. 6 is a rear view of the three dimensional mastopexy
implant shown in FIG. 1; and,
FIG. 7 is a top, front, side perspective view of the three
dimensional mastopexy implant shown in FIG. 1.
The broken lines shown in the figures form no part of the
claimed design.


(51) **LOC (14) Cl.** **24-03**
(52) **U.S. Cl.**
USPC **D24/155**
(58) **Field of Classification Search**
USPC D24/155
CPC A61F 2/12
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,701,879 A 2/1955 Bennett
3,280,818 A 10/1966 Pankey et al.
(Continued)

1 Claim, 7 Drawing Sheets

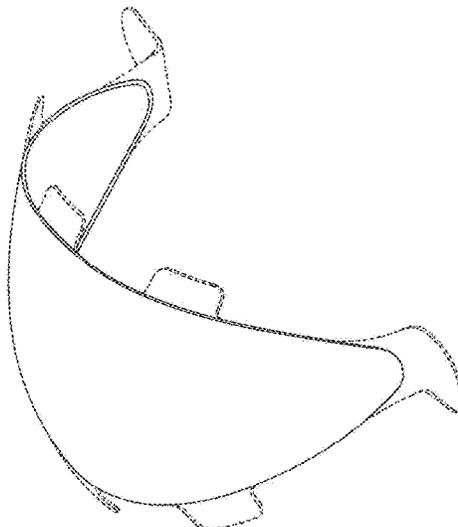

(56)

References Cited

OTHER PUBLICATIONS

International Search Report and Written Opinion dated Nov. 5, 2012 for International Application No. PCT/US2012/027975.

International Search Report and Written Opinion dated Apr. 23, 2019 for International Application No. PCT/US2019/015849.

International Written Opinion dated Feb. 12, 2015 for International Application No. PCT/US2014/046420.

[No Author Listed], "GalaFLEX Mesh . . . Supporting Your Quest for Timeless Beauty," Tepha, Inc. 400109 Rev.B, Oct. 2012.

[No Author Listed], "GalaFLEX Mesh," Tepha, Inc., Website, P/N 400124, Rev.A, Oct. 2013.

Auclair et al., Repair of mammary ptosis by insertion of an internal absorbable support and periareolar scar. *Ann Chir Plast Esthet.* 1993;38(1):107-13.

Debruijn et al., Mastopexy with 3D Preshaped Mesh for Long Term Results: Development of the Internal Bra System. *Aesth Plast Surg.* 2008;32:757-65. doi: 10.1007/s00266-008-9186-y.

Debruijn et al., Mastopexy with Mesh Reinforcement: the Mechanical Characteristics of Polyester Mesh in the Female Breast. *Plast Reconstr Surg.* 2009;124:364.

Goes, Periareolar mammoplasty: double skin technique with application of polyglactine or mixed mesh. *Plast Reconstr Surg.* 1996;97:959-68.

Goes, Periareolar mammoplasty: double-skin technique with application of mesh support. *Clin Plastic Surg.* 2002;29:349-64.

Goes, Periareolar Mastopexy with FortaPerm. *Aesth Plast Surg.* 2010;34:350-58.

Johnson, Central core reduction mammoplasties and Marlex suspension of breast tissue. *Aesth Plast Surg.* 1981;5:77-84.

Malluci, Concepts in aesthetic breast dimensions: Analysis of the ideal breast. *J Plast Reconstr Aesth Surg.* 2012;65:8-16.

Malluci, Design for Natural Breast Augmentation: The ICE Principle, *Plastic and Reconstructive Surgery.* Jun. 2016;137(6):1728-37.

Malluci, Population Analysis of the Perfect Breast: A Morphometric Analysis. *J Plast Reconstr Surg.* 2014;134(3):436-47.

Ray et al., Polydioxanone (PDS), A Novel Monofilament Synthetic Absorbable Suture. *Surg Gynecol Obst.* Oct. 1981;153:497-507.

Van Deventer, Improving the Longevity and Results of Mastopexy and Breast Reduction Procedures: Reconstructing an Internal Breast Support System with Biocompatible Mesh to Replace the Supporting Function of the Ligamentous Suspension. *Aesth Plast Surg.* 2012;36:578-89. doi: 10.1007/s00266-011-9845-2.

Williams, Poly-4-hydroxybutyrate (P4HB): a new generation of resorbable medical devices for tissue repair and regeneration. *Biomed Tech.* 2013;58(5):439-52. doi: 10.1515/bmt-2013-0009.

* cited by examiner

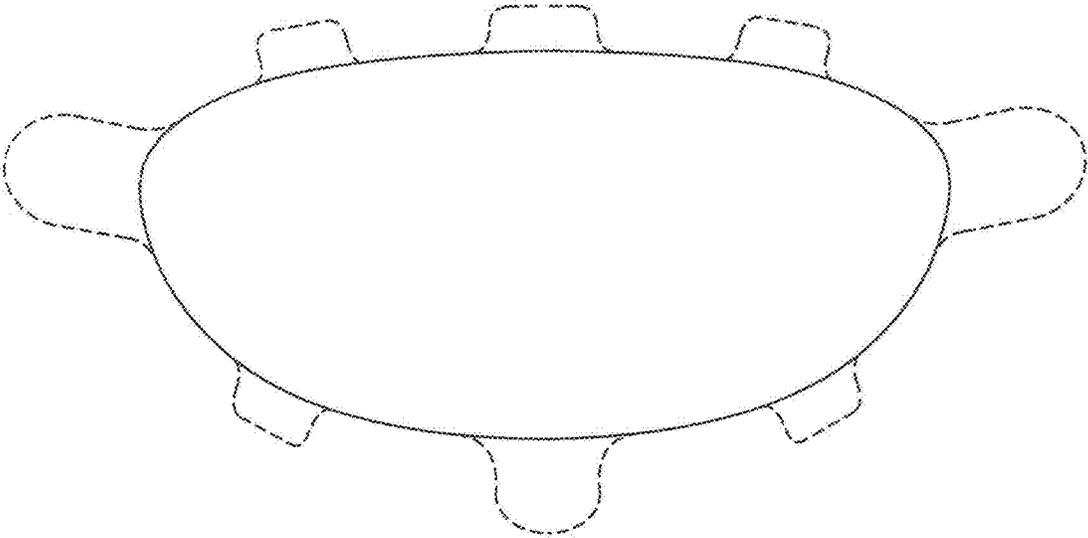


Figure 1

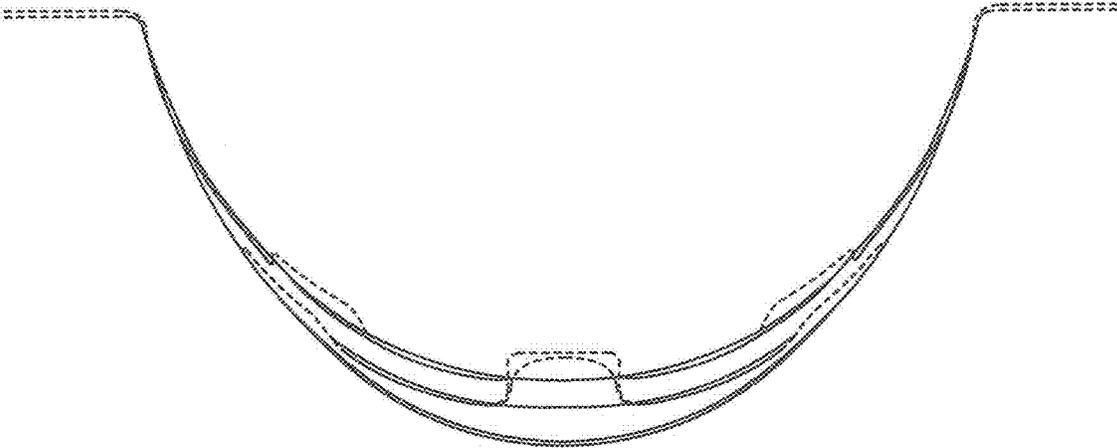


Figure 2

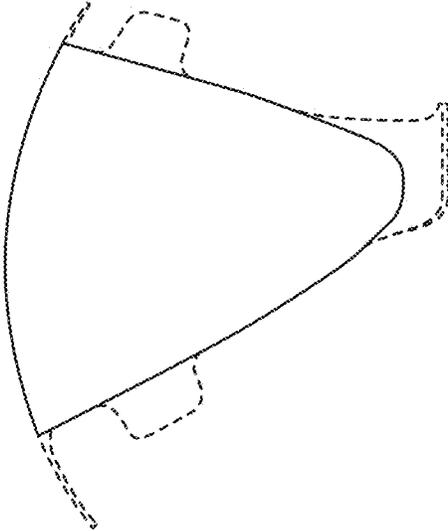


Figure 3

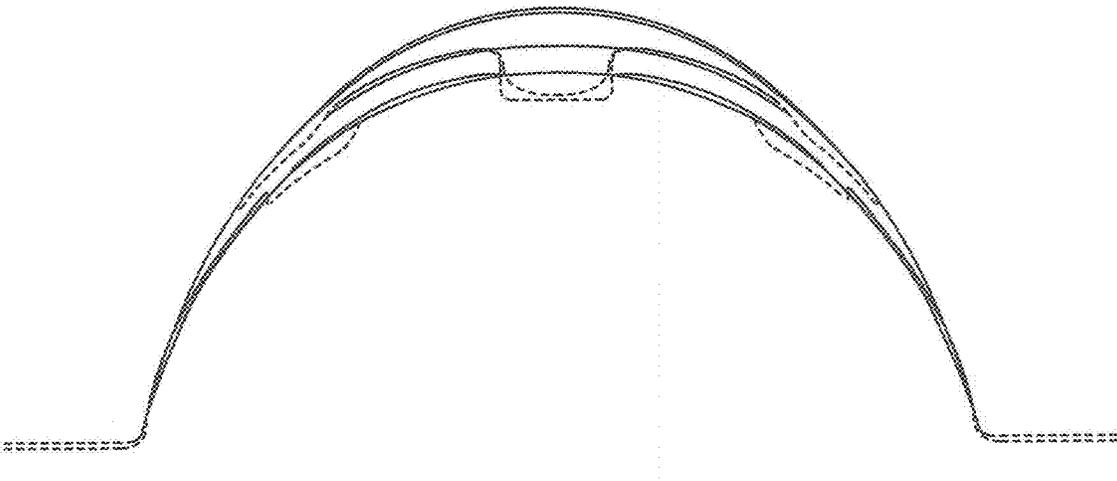


Figure 4

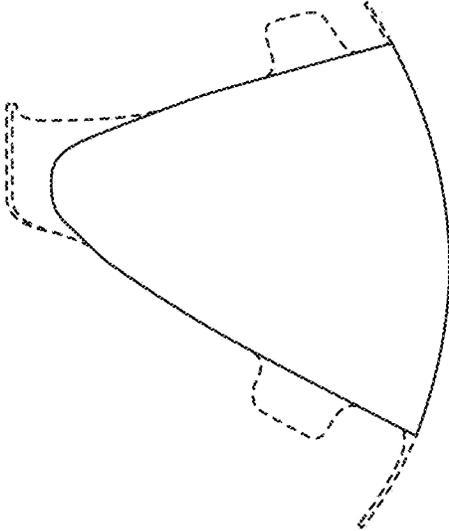


Figure 5

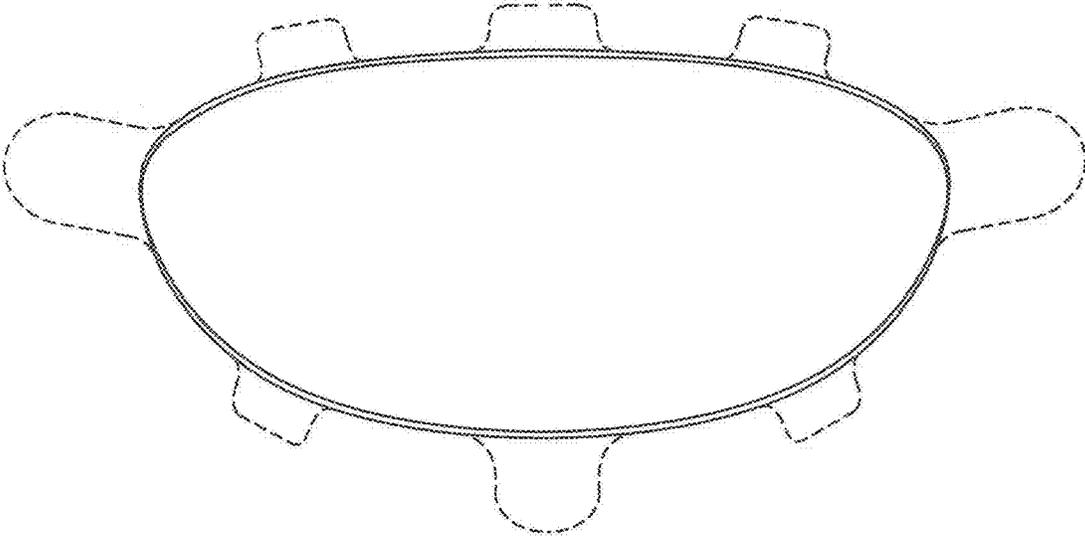


Figure 6

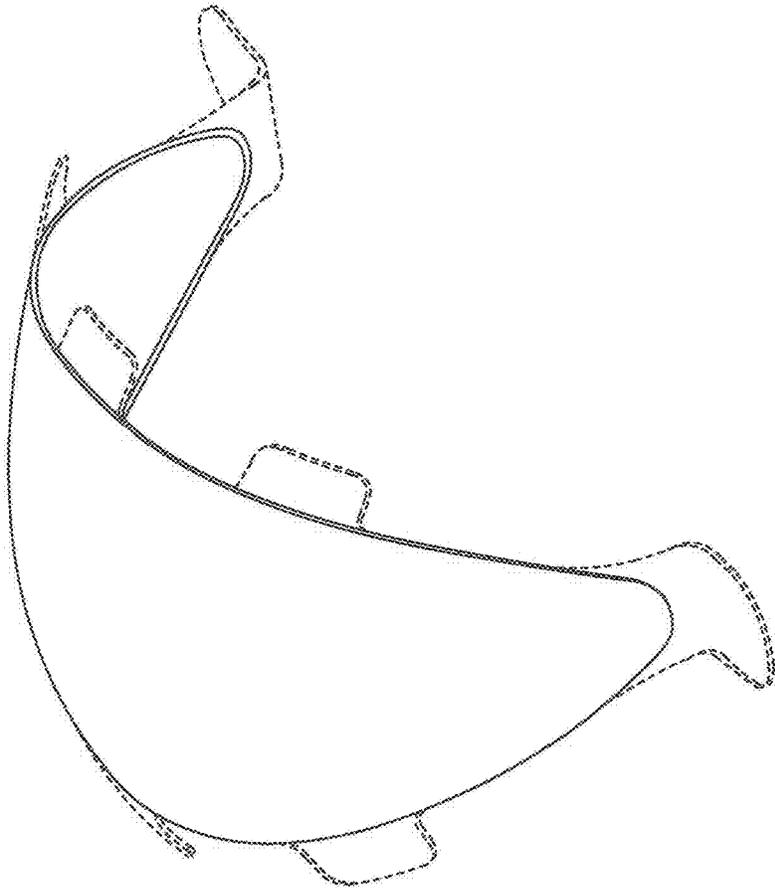


Figure 7