



(51) International Patent Classification:
A61B 17/072 (2006.01) H02J 7/00 (2006.01)
H01M 10/44 (2006.01)

(21) International Application Number:
PCT/US2011/053393

(22) International Filing Date:
27 September 2011 (27.09.2011)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
12/896,381 1 October 2010 (01.10.2010) US

(71) Applicant (for all designated States except US):
ETHICON ENDO-SURGERY, INC. [US/US]; 4545
Creek Road, Cincinnati, OH 45242 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **LEIMBACH, Richard, L.** [US/US]; 2901 Markbreit Avenue, Cincinnati, OH 45209 (US). **SCHWEMBERGER, Richard, F.** [US/US]; 8250 Eagle Creek Road, Cincinnati, OH 45247 (US). **SWENSGARD, Brett, E.** [US/US]; 7936 Orchard Court, West Chester, OH 45069 (US).

(74) Agents: **JOHNSON, Philip, S.** et al.; Johnson & Johnson, One Johnson & Johnson Plaza, New Brunswick, NJ 08933 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: SURGICAL INSTRUMENT HAVING A POWER CONTROL CIRCUIT

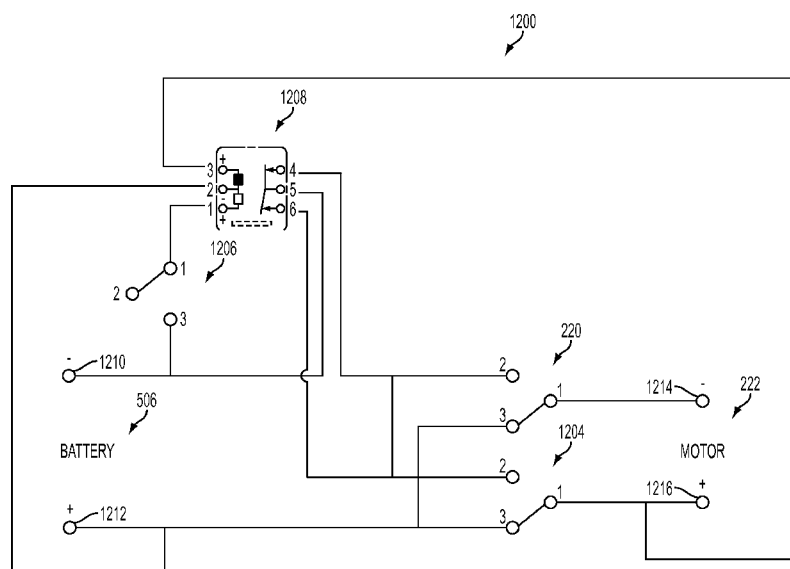


FIG. 52

device (1208) and an end-of-stroke sensor (1204). The firing switch may be configured to be in electrical communication with a power supply (506) for powering the drive device and in electrical communication with the drive device. The clamp switch may be in mechanical communication with the clamping trigger. The latching device may be in electrical communication with the clamp switch, the power supply and the drive device. The end-of-stroke switch may be in electrical communication with the latching device. Additionally, the firing switch may be electrically connected to, upon actuation, connect the power supply to the drive device via a first connection comprising the latching device and the firing switch. Further, the end-of-stroke switch may be electrically connected to, upon sensing an end of a stroke of the firing bar, cause a change in a state of the latching device to break the first connection between the power supply and the drive device.

(57) Abstract: Various embodiments are directed to a powered surgical instrument for cutting and fastening tissue. The instrument may comprise an end effector (104) comprising a first jaw member and a second jaw member (112). The second jaw member may be coupled to move relative to the first jaw member from an open position, where the jaw members are apart from one another, to a closed position. The end effector may also comprise a firing bar (108) positioned to fire by translating within the end effector when the first and second jaw members are in the closed position. Additionally, the surgical instrument may comprise a drive device (130), a clamping trigger (120) and a control circuit. The drive device may be mechanically coupled to the firing bar. The clamping trigger may be mechanically coupled to the end effector such that actuation of the clamping trigger causes the second jaw member to pivot towards the first jaw member. The control circuit (1200) may comprise a firing switch (220), a clamp switch (1206), a latching

**Declarations under Rule 4.17:**

— as to the identity of the inventor (Rule 4.17(i))

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))

— as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

Published:

— with international search report (Art. 21(3))

TITLE

SURGICAL INSTRUMENT HAVING A POWER CONTROL CIRCUIT

BACKGROUND

[0001] Traditionally, surgical devices have been hand operated, with the force to fire and/or manipulate the instruments provided directly by the clinician. A growing number of surgical instruments, however, are powered surgical instruments where the force to fire and/or manipulate the instrument are provided by an automated device, such as an electric motor, pneumatic or hydraulic device, *etc.* Examples of powered surgical instruments may include such as cutters, graspers, and/or staplers, for example. Such powered instruments free instrument designers from the need to limit the amount of force required to fire to that which can reasonably be provided by a human clinician. Powered instruments may also be more easily used by smaller clinicians and/or clinicians with less physical strength.

[0002] One significant challenge of powered instruments, however, is lack of feedback to the clinician. When a clinician uses a manually powered surgical instrument, the clinician is able to know the state of the instrument based on the amount of force that the clinician has already provided to the instrument, the position of the handle trigger or other device for receiving clinician force, *etc.* In a powered instrument, however, such feedback may be absent. Accordingly, there is a need to compensate for the lack of feedback from powered surgical instruments.

DRAWINGS

[0003] The features of the various embodiments are set forth with particularity in the appended claims. The various embodiments, however, both as to organization and methods of

operation, together with advantages thereof, may best be understood by reference to the following description, taken in conjunction with the accompanying drawings as follows:

[0004] Figure 1 shows one embodiment of a surgical stapling and cutting instrument with an electrically powered firing feature.

[0005] Figure 2 shows one embodiment of an end effector of the instrument of Figure 1.

[0006] Figures 3 and 4 show additional views of one embodiment of a firing bar of the instrument of Figure 1.

[0007] Figure 5 illustrates an alternative embodiment of an end effector having a firing bar lacking a middle pin.

[0008] Figure 6 illustrates a cut-away side view of one embodiment of the surgical instrument of Figure 1.

[0009] Figure 7 illustrates an exploded view of one embodiment of the surgical instrument showing various components thereof.

[0010] Figure 8 illustrates a shallower cut-away side view of one embodiment of the surgical instrument of Figure 1 to show component features not shown in the cut-away side view of Figure 6.

[0011] Figure 9 illustrates an internal view of one embodiment of the surgical instrument of Figure 1.

[0012] Figure 10 illustrates a partial cross-sectional view of one embodiment of the surgical instrument of Figure 1 with various components removed for clarity showing the operation of the retraction lever.

[0013] Figures 11 and 12 illustrate one embodiment of a locking cam of the surgical instrument of Figure 1 during various states of operation.

[0014] Figures 13-15 show various embodiments of the locking cam of Figures 11 and 12 and an intermediate gear during three stages of operation.

[0015] Figure 16 depicts one embodiment of the end effector of the instrument of Figure 1 in an open position, as a result of a retracted closure sleeve, with a staple cartridge installed in the elongate channel.

[0016] Figure 17 shows one embodiment of the implement portion of the surgical stapling and severing instrument of Figure 1 in disassembled form.

[0017] Figure 18 shows one embodiment of the end effector of the instrument of Figure 1 with a portion of the staple cartridge removed.

[0018] Figure 19 depicts the end effector of Figure 18 with all of the staple cartridge removed.

[0019] Figure 20 depicts one embodiment of the end effector of the instrument of Figure 1 closed in a tissue clamping position with the firing bar unfired.

[0020] Figure 21 depicts one embodiment of the upper surface of the staple cartridge shown in Figure 16 with the firing bar in its unfired, proximal position.

[0021] Figure 22 depicts one embodiment of the end effector of the instrument of Figure 1 near the pivot showing that the elongate channel has opposing ramp portions to thereby cooperate with the anvil to prevent tissue from jamming the end effector.

[0022] Figure 23 illustrates one embodiment of the end effector of the instrument of Figure 1 with tissue present between the staple cartridge and the anvil.

[0023] Figures 24-26 illustrate one embodiment of the end effector of the instrument of Figure 1 at various stages of firing.

[0024] Figures 27-29 schematically illustrate one embodiment of a battery unit and a portion of the instrument of Figure 1 showing the attachment and detachment of the battery unit to the instrument.

[0025] Figure 30 illustrates a graph of the voltage level of one embodiment of the battery unit of Figures 27, 28 and 29 over time, as measured from the time of attachment to the instrument of Figure 1.

[0026] Figure 31 shows one embodiment of a simplified circuit diagram of one embodiment of a battery unit comprising a drain.

[0027] Figure 32 is one embodiment of a simplified circuit diagram of one embodiment of a battery unit comprising a first drain and a second drain.

[0028] Figures 33-36 are perspective views of one embodiment of a battery unit.

[0029] Figures 37 and 38 illustrate cross-sectional views of one embodiment of the battery unit of Figures 33-36 including a translatable drain.

[0030] Figures 39-42 show multiple views of one embodiment of a battery dock.

[0031] Figure 43 is a perspective view of one embodiment of the translatable drain of Figures 37 and 38.

[0032] Figure 44 illustrates one embodiment of the battery unit of Figures 33-36 attached to a battery dock with various components omitted for clarity.

[0033] Figures 45 and 46 illustrate one embodiment of a battery unit with various components omitted for clarity.

[0034] Figures 47 and 48 illustrate one embodiment of a battery unit with various components omitted for clarity.

[0035] Figure 49 is a perspective view of one embodiment of single cell battery unit.

[0036] Figures 50 and 51 show internal views of the battery unit of Figure 49 during various stages of operation with various components omitted for clarity.

[0037] Figure 52 illustrates one embodiment of a control circuit that may control a connection between the battery unit or other power supply and the motor or other drive device for firing the instrument of Figure 1.

[0038] Figure 53 illustrates one embodiment of the control circuit of Figure 52 with additional switches and features.

[0039] Figure 54 is a flowchart showing one embodiment of a process flow showing the firing of the instrument of Figure 1 utilizing the control circuit as illustrated in Figure 53.

[0040] Figure 55 illustrates a perspective view of one embodiment of circuit board for implementing the control circuit of Figure 52 or 53, coupled to the battery dock of Figure 36.

[0041] Figure 56 illustrates a cut away view of one embodiment of the instrument of Figure 1 showing the emergency access door switch.

[0042] Figure 57 illustrates another cut away view of one embodiment of the instrument of Figure 1 showing the clamp switch.

[0043] Figure 58 illustrates another cut away view of one embodiment of the instrument of Figure 1 showing the stroke position switch.

[0044] Figure 59 illustrates another cut away view of one embodiment of the instrument of Figure 1 showing the end-of-stroke/motor reverse switch.

DESCRIPTION

[0045] Various embodiments are directed to surgical instruments having control circuits for implementing an electronic lock-out. For example, the control circuit may comprise one or more latching devices such as, for example, a latching relay, a transistor, *etc.* The surgical devices may comprise an end effector having first and second jaw members, where at least one of the jaw members is translatable (*e.g.*, pivotally or otherwise) towards the other. The surgical instruments may also have a firing bar that is translatable through the end effector when the jaw members are closed (*e.g.*, pivoted towards one another). The jaw members of the end effector may serve to clamp tissue. Once tissue is clamped, the firing bar may act upon the tissue. In various embodiments, distal motion of the firing bar may cause cutting and/or fastening of tissue. For example, the firing bar may define a cutting edge or knife to cut tissue clamped between the jaw members. Also, for example, the firing bar may drive a wedge or other mechanism to drive staples through the tissue clamped between the jaw members. According to various embodiments, the firing bar may be driven by a drive device such as, for example, an electric motor, a pneumatic or hydraulic device, *etc.* The drive device may be powered by a power

supply such as, for example, a battery and/or a connection to an external source of electrical power, such as a wall outlet.

[0046] Figure 1 shows one embodiment of a surgical stapling and cutting instrument 102 with an electrically powered firing feature. The illustrated embodiment is an endoscopic instrument and, in general, the embodiments of the instrument 102 described herein are endoscopic surgical cutting and fastening instruments. It should be noted, however, that according to other embodiments, the instrument may be a non-endoscopic surgical cutting and fastening instrument, such as a laparoscopic or open surgical instrument. The instrument 102 may comprise an end effector 104 that may be operative to staple and cut tissue in response to control operations executed by a clinician grasping a handle portion 106. Figure 2 shows one embodiment of the end effector 104 of the instrument 102. According to various embodiments, the instrument 102 may utilize an E-beam firing mechanism or firing bar 108 that may control the spacing of the end effector 104. For example, a first jaw member, or elongate channel 110 and a pivotally translatable second jaw member or anvil 112 may be maintained at a spacing that assures effective stapling and severing.

[0047] The instrument 102 may comprise the handle portion 106 and an implement portion 114. The implement portion 114 may be connected to the handle portion 106 and may comprise a shaft 116 distally terminating in the end effector 104. The handle portion 106 may comprise a pistol grip 118. A closure trigger 120 may be positioned such that a clinician may pivotally draw the closure trigger 120 towards the pistol grip 118 to cause clamping, or closing, of the anvil 112 toward the elongate channel 110 of the end effector 104. A firing trigger 122 may be positioned farther outboard of the closure trigger 120 and may be pivotally drawn by the clinician to cause the stapling and severing of clamped tissue in the end effector 104. As described below, the stapling and severing of the clamped tissue by the end effector 104 may be powered by an electric motor.

[0048] It will be appreciated that the terms “proximal” and “distal” are used herein with reference to a clinician gripping a handle of an instrument. Thus, the end effector 104 is distal

with respect to the more proximal handle portion 106. It will be further appreciated that for convenience and clarity, spatial terms such as “vertical” and “horizontal” are used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

[0049] In use, the clinician may actuate the closure trigger 120 first. For example, once the clinician is satisfied with the positioning of the end effector 104, the clinician may draw back the closure trigger 120 to its fully closed, locked position proximate to the pistol grip 118. Then, the clinician may actuate the firing trigger 122 to initiate powered cutting and stapling of tissue held between the anvil 112 and elongate channel 110. For example, the firing bar 108 may be powered forward to cut tissue and drive staples, for example, as described herein below. When the clinician removes pressure from the firing trigger 122, the firing bar 108 may be returned to the pre-firing position shown in Figure 2. The clinician may actuate a release button 124 on the handle portion 106 to release the closure trigger 120. The clinician may then release the closure trigger, in turn releasing the anvil 112 and elongate channel 110 to pivot away from one another back to the position shown in Figure 2.

[0050] Referring again to Figure 1, the shaft 116 may comprise a frame 126 enclosed by a closure sleeve 128. A firing drive member 130 may be positioned within the frame 126 and may extend from the handle portion 106 to the firing bar 108. The drive member 130 may comprise a single component, or may be made up of multiple components. The frame 126 may connect the handle portion 106 to the end effector 104. With the closure sleeve 128 withdrawn proximally by the closure trigger 120 as depicted in Figures 1 and 2, the anvil 112 may springedly open, pivoting away from the elongate channel 110 and translating proximally with the closure sleeve 128.

[0051] The elongate channel 110 may receive a staple cartridge 132 that may be responsive to the firing bar 108 to drive staples into forming contact with the anvil 112. It will be appreciated that although a readily replaceable staple cartridge 132 is advantageously described herein, a staple cartridge 132 consistent with various embodiments may be permanently affixed

or integral to the elongate channel 110, for instance when a larger portion of the end effector 104 is replaced after each firing.

[0052] Figures 3 and 4 show additional views of one embodiment of the firing bar 108. As illustrated in Figures 2-4, the firing bar 108 may include three vertically spaced pins that control the spacing of the end effector 104 during firing. An upper pin 134 may be staged to enter an anvil pocket 136 near the pivot between the anvil 112 and elongate channel 110. When fired with the anvil 112 closed, the upper pin 134 may advance distally within a longitudinal anvil slot 138 extending distally through anvil 112. According to various embodiments, minor upward deflections of the anvil 112 may be overcome by a downward force imparted on the anvil 112 by the upper pin 134. The firing bar 108 may also include a lower pin, or firing bar cap, 140 that may upwardly engage a channel slot 142 in the elongate channel 110, thereby cooperating with the upper pin 134 to draw the anvil 112 and the elongate channel 110 together in the event of excess tissue clamped therebetween.

[0053] The firing bar 108 may also comprise a middle pin 144 that may pass through a firing drive slot 146 formed in a lower surface of the cartridge 132 and an upward surface of the elongate channel 110. In this way, the middle pin 144 may initiate the driving of the staples, as described below. The middle pin 144, by sliding against the elongate channel 110, may resist a tendency for the end effector 104 to be pinched shut at its distal end. To illustrate an advantage of the middle pin 144, Figure 5 illustrates an alternative embodiment of an end effector 148 having a firing bar 150 lacking a middle pin. As shown in Figure 5, the end effector 148 is allowed to pinch shut at its distal end, which may tend to impair desired staple formation.

[0054] Returning to Figures 2-4, the firing bar 108 may comprise a distally presented cutting edge 152 between the upper and middle pins 134, 144. When the end effector 104 is fired, the cutting edge 152 may traverse through a proximally presented, vertical slot 154 in the cartridge 132 to sever clamped tissue present between the anvil 112 and the elongate channel 110. The affirmative positioning of the firing bar 108 with regard to the elongate channel 110 and anvil 112 may make it more likely that an effective cut is performed.

[0055] The affirmative vertical spacing provided by the E-Beam firing bar 108 may be suitable for the limited size available for endoscopic devices. Moreover, the E-Beam firing bar 108 may enable fabrication of an anvil 112 with a camber imparting a vertical deflection at its distal end, similar to the position depicted in Figure 5. This cambered anvil 112 may assist in achieving a desirable gap in the end effector 104 even with an anvil 112 having reduced thickness, which may be thus more suited to the size limitations of an endoscopic device. The E-Beam firing bar 108 may further enable increased applications, especially in combination with a range of configurations of staple cartridges. For instance, a clinician may select a gray staple cartridge yielding a 0.02 mm tissue gap, a white staple cartridge yielding a 0.04 mm tissue gap, a blue cartridge yielding a 0.06 mm tissue gap, or a green cartridge yielding a 0.102 mm tissue gap. The vertical height of each respective staple cartridge in combination with the length of staples and an integral wedge sled (described in more detail below) may predetermine this desired tissue thickness with the anvil 112 appropriately vertically spaced by the E-Beam firing bar 108.

[0056] Figures 6-9 illustrate various internal components of the handle portion 106 of one embodiment of the surgical instrument 102. For example, Figure 6 illustrates a cut-away side view of one embodiment of the surgical instrument 102. Figure 7 illustrates an exploded view of one embodiment of the surgical instrument 102 showing a portion of the components thereof. Figure 8 illustrates a cut-away side view of one embodiment of the surgical instrument of 102 that is shallower than the cut-away of Figure 6 in order to show component features not shown in the cut-away side view of Figure 6. Figure 9 illustrates an internal view of one embodiment of the surgical instrument 102.

[0057] With reference to Figures 6-9, the handle portion 106 may be comprised of first and second base sections 156 and 158, which may be molded from a polymeric material such as a glass-filled polycarbonate. Within the first and second base sections 156, 158 may be first and second frame sections 160, 162. A rotating knob 164 may have a bore 166 extending completely through it for engaging and rotating the implement portion 114 about its longitudinal axis. The

rotating knob 164 may include an inwardly protruding boss 168 extending along at least a portion of the bore 166. The protruding boss 168 is received within a longitudinal slot 170 formed at a proximal portion of the closure sleeve 128 such that rotation of the rotating knob 164 effects rotation of the closure sleeve 128. It will be appreciated that the boss 168 may further extend through frame 126 and into contact with a portion of the firing drive member 130 to effect its rotation as well. Thus, the end effector 104 may rotate with the rotating knob 164.

[0058] A proximal end 172 of the frame 126 may pass proximally through the rotating knob 164 and may be provided with a circumferential notch 174 that is engaged by opposing channel securement members 176 extending respectively from the frame sections 160 and 162. The channel securement members 176 extending from the frame sections 160, 162 may serve to secure the frame 126 to the handle portion 106 such that the frame 126 does not move longitudinally relative to the handle portion 106.

[0059] The closure trigger 120 may have a handle section 178, a lever section 180, and an intermediate section 182. A bore 184 may extend through the intermediate section 182. A cylindrical support member 186 may pass through the bore 184 for pivotally mounting the closure trigger 120 on the handle portion 106 (e.g., via the frame sections 160, 162). A second cylindrical support member 188 may pass through a bore 190 of firing trigger 122 for pivotally mounting the firing trigger 122 on the handle portion 106.

[0060] A closure yoke 192 may be housed within the handle portion 106 for reciprocating movement therein and serves to transfer motion from the closure trigger 120 to the closure sleeve 128. The closure yoke 192 may be coupled to the handle portion 106 via the respective frame portions 160, 162. A proximal end 194 of the closure sleeve 128 is provided with a flange 196 that is snap-fitted into a receiving recess 198 formed in the yoke 192. A distal end of the yoke 192 may be coupled to a secondary yoke 200 via a biasing member such as a spring 202. A proximal end of the yoke 192 may define a bore 204 for receiving a linkage 206. A proximal end of the linkage 206 may be coupled to the closure trigger 120. For example, the linkage 206 may comprise a bore for receiving the pin 188. In this way, when the clinician

moves the handle section 178 of the closure trigger 120 proximally toward the pistol grip 118, the linkage 206 may be pushed distally, causing corresponding distal motion of the secondary yoke 200, compressing the spring 202 biases the yoke proximally and, in turn, pushing the yoke 192 and closure sleeve 128 distally. Distal movement of the closure sleeve 128 may cause pivotal translation movement of the anvil 112 distally and toward the elongate channel 110 of the end effector 104 and proximal movement effects closing, as described below.

[0061] As the closure trigger 120 is pulled towards the pistol grip 118, the lever portion 180 of the trigger 120 may translate distally. When the closure trigger 120 is fully pulled against the pistol grip 118, a clamp lock switch 124 may pivot about a clamp lock pin 208 to lock the closure trigger 120 into the clamped position. For example, the clamp lock switch 124 may be biased by a spring (not shown) to pivot about the pin 208. The clinician may unlock the closure trigger 120, for example, by actuating the clamp lock switch 124, causing it to pivot about the clamp lock pin 208 (clockwise as shown in Figures 6 and 8). This may allow the closure trigger 120 to return to the open position, causing proximal motion of the closure sleeve and pivoting the anvil 112 proximally and away from the elongate channel 110 of the end effector 104, as described below.

[0062] As the closure trigger 120 is moved toward the pistol grip 118, its intermediate section 182 may be pulled proximally, causing the firing trigger 122 to also move proximally to its “firing” position. When in its firing position, the firing trigger 122 may be located at an angle of approximately 45° to the pistol grip 118. To fire the instrument 102, the clinician may first deactivate a firing trigger safety 210. For example, the safety 210 may be pivotally coupled to the closure trigger 120 about a pin 212. A distal portion of the safety 210 may be received into a cavity 214 of the firing trigger 122, preventing the firing trigger 122 from being actuated. The clinician may deactivate the safety 210 by removing it from the cavity 214 and pivoting the safety 210 proximally. This may allow the clinician to actuate the firing trigger 122.

[0063] The firing trigger 122 may be biased to an “off” position by a biasing member such as a spring 216 (Figure 9). When actuated (*e.g.*, against the force of the spring 216), the

firing trigger 122 may be rotated clockwise, as shown in Figure 9. A contactor portion 218 of the trigger may activate a trigger switch 220, *e.g.*, via an actuator 221, which may initiate firing of the instrument 102. Actuation of the trigger switch 220 may activate a motor 222. The motor 222 may be coupled to a gearbox 224 comprising an enclosure 226 and gear cluster 228. The gearbox 224 may gear down the motor 222. In one example embodiment, the motor 222 may rotate at 106,000 RPM, while the gearbox 224 may have a ratio of 509-to-1.

[0064] An intermediate gear 230 may be coupled to the output of the gearbox 224. The intermediate gear 230 may be in mechanical communication with a drive gear 232. The drive gear 232 may be rotatable about a drive shaft 234. A biasing member such as a spring 236 may bias the drive gear 232 and/or drive shaft 234 such that the drive gear 232 is in mechanical communication with a geared face 240 of a rack 238. The rack 238 may be coupled to the firing drive member 130 which may, ultimately, be in mechanical communication with the firing bar 108. Accordingly, rotation of the motor 222 may cause rotation of the gearbox 224, leading to rotation of the intermediate 230 and drive 232 gears. Rotation of the drive gear 232 may result in distal or proximal motion of the rack 238, drive member 130, and drive bar 108. Distal and proximal motion of the drive bar 108 may cause the instrument 102 to fire, for example, as described herein below.

[0065] When the instrument is fired, the rack 238 may translate distally. A top geared face 242 of the rack 238 may be coupled to a clamp lock 244, causing the clamp lock 244 to translate distally about a pivot pin 246. In its distal position, the clamp lock 244 may contact the clamp switch 124, preventing it from disengaging as described above. In this way, the clinician may be mechanically prevented from releasing the clamp switch 124 while the instrument 102 is in a fired position (*e.g.*, the drive bar 108 is extended distally).

[0066] According to various embodiments, the surgical instrument 102 may comprise mechanisms allowing a clinician to disable the motor 222 and manually disengage the firing bar 108. For example, the instrument 102 may comprise an emergency access door 248. The access door 248 may be coupled to a switch, as described below, such that when the clinician opens the

access door 248, electric power to the motor 222 may be cut. Below the access door 248, the device 102 may comprise a manual retraction lever 250. The retraction lever 250 may be rotatable about a pivot a pin 252. A locking cam 254 may also be pivotable about the pin 252. After the clinician has opened and/or removed the access door 248, the clinician may pull up on the retraction lever 250. This may cause the lever 250 to rotate about the pin 252 (clockwise as shown in Figure 9 and counter clockwise as shown in Figure 6). Initially, the locking cam 254 may rotate with the retraction lever 250. As the locking cam 254 rotates, a locking arm 256 of the cam 254 may contact a top surface 258 the drive gear 232, working against the bias of the spring 236 to push the drive gear 232 down and out of contact with the geared face 240 of the rack 238. This may disengage the motor 222 from the rack 238, drive member 130 and drive bar 108. When the locking cam 254 is rotated by a predetermined amount, the locking arm 256 may lock against the drive gear 232, preventing reverse rotation of the locking cam 254.

[0067] Figures 10-15 illustrate additional details of the operation of the locking cam 254. Figure 10 illustrates a partial cross-sectional view of one embodiment of the surgical instrument 102 with various components removed for clarity showing the operation of the retraction lever 250. In Figure 10, the rack 238 is shown in cross-section. Figures 11 and 12 illustrate one embodiment of the locking cam 254 during various states of operation. The locking cam 254 may comprise a body portion 260. The locking arm 256 that may pivot, or otherwise flex, with respect to the body portion 260 about a hinge portion 262. The hinge portion 262 may comprise, for example, a living hinge. In one embodiment, the body portion 260 and the locking arm 256 may be unitary and formed from a single piece of material. The locking cam 254 may define a clearance 264 that allows the locking arm 256 to pivot toward the body portion 260. The locking arm 256 may have a tooth 266 that is received by a notch 268 in the body portion 260. On their respective outer peripheries, the body portion 260 may have a first contacting surface 270 and the locking arm 256 may have a second contacting surface 272. In the closed position (Figure 11), the first contacting surface 270 may be generally aligned with the second contacting surface 272 such that the outer periphery of the locking cam 254 has a

generally continuous cammed surface. In the open position (Figure 12), the locking arm 256 pivots away from the body portion 260 to increase the clearance 264. A gap 258 is created between the first contacting surface 270 and the second contacting surface 272.

[0068] Referring now to Figures 10, 11, and 12, upon rotation of the lever 250 in the direction indicated by arrow 274, the locking cam 254 is rotated and the second outer surface 272 of the locking arm 256 first contacts a top surface 258 of the intermediate gear 230. As a result of this contact, the locking arm 256 may be pivoted toward the body portion 260 to create a generally continuous periphery. As the locking cam 254 continues to rotate, the second contacting surface 272 and then the first contacting surface 270 exerts force on the intermediate gear 230 to overcome the biasing force applied by the spring 236. As a result, the intermediate gear 230 is pushed in the direction indicated by arrow 275 as the lever 250 is rotated in the direction indicated by arrow 274. The movement of the intermediate gear 230 may decouple it from the geared face 240 of the rack 260 allowing the rack 260 to translate freely. Once the locking arm 256 clears the top surface 258 of the intermediate gear 230, it may pivot to the open position (FIG. 12) to lock the locking cam 254 into place. Once in the open position, the locking cam 254 may be impeded from rotating in the direction indicated by arrow 276 (Figure 10) due to the engagement of the locking arm 256 with the intermediate gear 230.

[0069] Figures 13-15 show various embodiments of the locking cam 254 and a intermediate gear 230 during three stages of operation. Various components have been removed and/or simplified for clarity. As illustrated, the locking cam 254 may be manufactured from a single piece of material. The locking cam 254 comprises a locking arm 256 that is pivotable with respect to a body portion 260. Figure 13 shows one embodiment of the locking cam 254 in a non-engaged position. In this position, a distal portion 278 of the locking arm 256 is separated from the body portion 260. As illustrated in Figure 14, when the locking cam 254 is rotated in the direction indicated by arrow 274, the locking arm 256 is drawn toward the body portion 260 to create a generally continuous periphery spanning the locking arm 256 and the body portion 260. As the locking cam 254 contacts a top face 258 of the intermediate gear 230, the gear 230

may move in the direction indicated by arrow 280. As the locking cam 254 continues to rotate in the direction indicated by arrow 274, eventually the locking arm 256 passes over the drive shaft 234. As shown in Figure 15, when the distal portion 278 of the locking arm 256 separates from the body portion 260, it engages the teeth of the intermediate gear 230 to lock the locking cam 254 into an engaged position. Accordingly, in various embodiments, while the locking cam 254 may be made from a single piece of material, it may function as two parts (e.g., a cam and a locking mechanism).

[0070] Referring now to Figure 6, the retraction lever 250 may also comprise a ratchet arm 282 rotatable about a ratchet pin 284. As the retraction lever 250 is pulled up, a tooth portion 286 of the ratchet arm 282 may come into contact with the top geared face 242 of the rack 238. Further rotation of the ratchet lever 250 may cause the tooth 286 to exert a proximally directed force on the rack 238, causing the drive member 130 and drive bar 108 to translate proximally. Further lifting of the retraction lever 250 may disengage the tooth portion 286 from the top geared face 242, allowing the clinician to replace the retraction lever 250 towards its original position without causing corresponding distal motion of the rack 238. Additional proximal motion of the rack 126, drive member 130 and drive bar 108 may be achieved by additional lifting of the retraction lever 250, repeating the process described above.

[0071] Figure 17 shows one embodiment of the implement portion 114 of the surgical stapling and severing instrument 102 in disassembled form. The staple cartridge 132 is shown as being comprised of a cartridge body 304, a wedge sled 306, single and double drivers 308, staples 310, and a cartridge tray 312. When assembled, the cartridge tray 312 holds the wedge sled 306, single and double drivers 308, and staples 310 inside the cartridge body 304.

[0072] The elongate channel 110 may have a proximally placed attachment cavity 314 that receives a channel anchoring member 316 on the distal end of the frame 126 for attaching the end effector 104 to the handle portion 106. The elongate channel 110 may also have an anvil cam slot 316 that pivotally receives an anvil pivot 318 of the anvil 112. The closure sleeve 128 that encompasses the frame 126 may include a distally presented tab 320 that engages an anvil

feature 324 proximate but distal to the anvil pivot 318 on the anvil 112 to thereby effect opening and closing of the anvil 112. The firing drive member 130 is shown as being assembled from the firing bar 108 attached to a firing connector 326 by pins 328, which in turn is rotatably and proximally attached to the metal drive rod 330. The firing bar 108 is guided at a distal end of the frame by a slotted guide 332 inserted therein.

[0073] With particular reference to Figure 18, a portion of the staple cartridge 132 is removed to expose portions of the elongate channel 110, such as recesses 300, 302 and to expose some components of the staple cartridge 132 in their unfired position. In particular, the cartridge body 304 (shown in Figure 17) has been removed. The wedge sled 306 is shown at its proximal, unfired position with a pusher block 334 contacting the middle pin 144 (not shown in Figure 18) of the firing bar 108. The wedge sled 306 is in longitudinal sliding contact upon the cartridge tray 312 and includes wedges 308 that force upward the single and double drivers 308 as the wedge sled 306 moves distally. Staples 310 (not shown in Figure 18) resting upon the drivers 308 are thus also forced upward into contact with the anvil forming pockets 290 on the anvil 112 to form closed staples. Also depicted is the channel slot 142 in the elongate channel 110 that is aligned with the vertical slot 154 in the staple cartridge 132.

[0074] Figure 19 depicts the end effector 104 of Figure 18 with all of the staple cartridge 132 removed to show the middle pin 144 of the firing bar 108 as well as portion of the elongate channel 110 removed adjacent to the channel slot 142 to expose the firing bar cap 140. In addition, portions of the shaft 116 are removed to expose a proximal portion of the firing bar 108. Projecting downward from the anvil 112 near the pivot, a pair of opposing tissue stops 346 may prevent tissue being positioned too far up into the end effector 104 during clamping.

[0075] Figure 20 depicts one embodiment of the end effector 104 closed in a tissue clamping position with the firing bar 108 unfired. The upper pin 134 is shown in the anvil pocket 136, vertically aligned with the anvil slot 138 for distal longitudinal movement of the firing bar 108 during firing. The middle pin 144 may be positioned to push the wedge sled 306 distally so that wedge 308 sequentially contacts and lifts double drivers 308 and the respective staples 310

into forming contact with staple forming pockets 290 in the lower surface 288 of the anvil 112. According to various embodiments, the end effector 104 may implement a mechanical lock-out mechanism. The mechanical lock-out mechanism may prevent the instrument 102 from being fired twice without reloading a new staple cartridge 132. For example, it will be appreciated that firing the instrument 102 without a loaded staple cartridge present may cause tissue to be cut, but not fastened. The lock-out may be implemented in any suitable manner. For example, the firing bar 108, upon retraction in the proximal direction, may be shifted by the elongate channel 110, or other component, such that the upper pin 134 is no longer in alignment with the anvil slot 138, preventing the firing bar 108 from moving distally (*e.g.*, re-firing). Installation of a new staple cartridge 132 to the elongate channel 110 may snap the firing bar 108 back, aligning the upper pin 134 with the anvil slot 138 and allowing re-firing. It will be appreciated that any suitable mechanism in the end effector or the handle 106 may be utilized to implement a mechanical lock-out.

[0076] Figure 21 depicts one embodiment of the upper surface 294 of the staple cartridge 132 with the firing bar 108 in its unfired, proximal position. The stapler apertures 292 are arrayed on each side of the vertical slot 154 in the staple cartridge 132. Figure 22 depicts one embodiment of the end effector 104 near the pivot showing that the elongate channel 110 has opposing ramp portions 348 to thereby cooperate with the tissue stops 346 of the anvil 112 to prevent tissue from jamming the end effector 104. Also depicted in greater detail are the double drivers 308 and their relation to the staples 310.

[0077] Figures 24-26 illustrate one embodiment of the end effector 104 at various stages of firing. In use, the surgical stapling and severing instrument 102 may be used to cut and staple tissue. In Figures 1-2, the instrument 102 is shown in its start position, having had an unfired, fully loaded staple cartridge 132 snap-fitted into the distal end of the elongate channel 110. Both triggers 120, 122 are forward and the end effector 104 is open, such as would be typical after inserting the end effector 104 through a trocar or other opening into a body cavity. The instrument 102 may then be manipulated by the clinician such that tissue 340 to be stapled

and severed is positioned between the staple cartridge 132 and the anvil 112. Figure 23 illustrates the end effector 104, according to one embodiment, with tissue 340 present between the staple cartridge 132 and the anvil 112.

[0078] Next, the clinician moves the closure trigger 120 proximally until positioned directly adjacent to the pistol grip 118, locking the handle portion 106 into the closed and clamped position. The retracted firing bar 108, shown in Figure 24 in the end effector 104 may not impede the selective opening and closing of the end effector 104, but rather may reside within the anvil pocket 136. With the anvil 112 closed and clamped, the firing bar 108 may be aligned for firing through the end effector 104. In particular, the upper pin 134 may be aligned with the anvil slot 138 and the elongate channel 110 may be affirmatively engaged about the channel slot 142 by the middle pin 144 and the firing bar cap 140.

[0079] After tissue clamping has occurred, the clinician may move the firing trigger 122 proximally causing the firing bar 108 to move distally into the end effector 104, shown in Figure 25. In particular, the middle pin 144 enters the staple cartridge 132 through the firing drive slot 146 to cause the firing of the staples 310 via wedge sled 306 toward the anvil 112. The lower most pin, or firing bar cap 140, cooperates with the middle pin 144 to slidably position cutting edge 152 of the firing bar 108 to sever tissue. The two pins 140, 144 also position the upper pin 134 of the firing bar 108 within longitudinal anvil slot 138 of the anvil 112, affirmatively maintaining the spacing between the anvil 112 and the elongate channel 110 throughout its distal firing movement.

[0080] The clinician may continue moving the firing trigger 122 until brought proximal to the closure trigger 120 and pistol grip 118. Thereby, all of the ends of the staples 310 may be bent over as a result of their engagement with the anvil 112, as shown in Figure 26. The firing bar cap 140 may be arrested against a firing bar stop 342 projecting toward the distal end of the channel slot 142. The cutting edge 152 may have traversed completely through the tissue. The process is complete by releasing the firing trigger 122. Releasing the firing trigger 122 may, as described herein below, cause the motor 222 to reverse its rotation, causing retraction of the

firing bar 108. Upon retraction of the firing bar 108, the clinician may depress the clamp switch 124. (e.g., while simultaneously squeezing the closure trigger 120) This may open the end effector 104.

[0081] Referring back to Figure 1, the handle 106 of the instrument 102 may house at least one battery unit 506. The battery unit 506 may comprise a single battery or a plurality of batteries arranged in a series and/or parallel configuration. The handle 502 may comprise a battery dock 508 to which the battery unit 506 may be attached. The battery dock 508 may be any suitable structure for coupling the battery unit 506 to the instrument 102. For example, the battery dock 508 may be or comprise a cavity in the handle 106 configured to receive at least a portion of the battery unit 506, as illustrated. In other embodiments, the battery dock 508 may be implemented using a variety of other structures. In one embodiment, the battery dock 508 may comprise a post that is received by the battery unit 506. In one embodiment, the pistol grip 120 may comprise the battery dock 508. In any event, as discussed in more detail below, the battery dock 508 may comprise a protruding portion to interact with the battery unit 506 upon attachment of the battery unit 506 to the handle 502. Once attached, the battery unit 506 may be electrically connected to and may provide power to the motor 222 of the instrument 102.

[0082] Figures 27-29 schematically illustrate one embodiment of the battery unit 506 and a portion of the instrument 102 showing the attachment and detachment of the battery unit 506 to the instrument 102. The battery unit 506 may comprise a drain 512 that automatically completes a circuit within the battery unit 506 upon attachment to the instrument 102. The drain may serve to slowly reduce the charge of the battery unit 506 over time. Once the battery unit 506 has been sufficiently drained it may be disposed as non-hazardous waste, for example. The battery unit 506 may comprise a voltage source 510. In one embodiment, the voltage source 510 is a lithium battery and comprises at least one cell selected from the group consisting of a CR123 cell and a CR2 cell. As is to be appreciated, any suitable voltage source may be used. The battery unit 506 may also comprise a drain 512 that may be electrically coupled to the voltage source 510 when a switch 516 is closed. The battery unit 506 and the instrument 102 each

comprise electrically conductive contacts 518, 520, respectively, that are placed into contact upon attachment of the battery unit 506 to the instrument 102. Figure 27 illustrates the battery in a non-attached position. The switch 516 is in an open position and the voltage source 510 may be in a fully charged condition. Figure 28 illustrates that battery unit 506 in an attached position. The conductive contacts 518 of the battery unit 506 are in electrical communication with the contacts 520 of the instrument thereby allowing the battery unit 506 to supply energy to the circuit 514 (Figure 46). In the attached position, the switch 516 may transition to the closed position to electrically couple the voltage source 510 to the drain 512. Energy will flow from the voltage source 510 through the drain 512 during operation of the instrument. In other words, the drain 512 will be draining the charge from the voltage source 510 concurrently as the battery unit 506 is supplying operational power to the instrument 102. As discussed in more detail below, a portion of the instrument 102 may physically interact with the drain 512 during attachment of the battery unit 506 to the instrument 102 to transition the switch 516 from the open to the closed state. Figure 29 illustrates the battery unit 506 in a non-attached position. In one embodiment, the switch 516 remains in the closed position to continue to drain the voltage source 510 even after the battery unit 506 has been detached from the instrument 102.

[0083] Figure 30 illustrates a graph 600 of the voltage level of one embodiment of the battery unit 506 over time, as measured from the time of attachment to the instrument 102. The graph 600 includes three example discharge curves 602, 604, 606. As illustrated by the first discharge curve 602, the voltage of the power source 510 may drop below 2.0 volts after around 28 hours. As illustrated by the second discharge curve 604, the voltage of the power source 510 may drop below 2.0 volts after around 30 hours. As illustrated by the third discharge curve 606, the voltage of the power source 510 may drop below 2.0 volts after around 33 hours. The overall shape of the discharge curve may depend upon, for example, the level of activity of the instrument 102 during the surgical procedure. For example, the instrument associated with the first discharge curve 602 was more heavily used during the surgical procedure than the instrument associated with discharge curve 606. In any event, the drain 512 may maintain the

voltage level of the battery unit 506 at a satisfactory level for a certain time period to ensure that the instrument can be used for its intended purpose during the course of the surgical procedure. For example, in one embodiment, the voltage level of the battery unit 506 may be maintained around 6 volts for approximately 12 hours. After 12 hours, the voltage level gradually decreases to a non-hazardous level. As is to be appreciated, the drain 512 may be calibrated to deplete the voltage source faster or slower.

[0084] In one embodiment, a resistive element may be used to reduce the energy level of the voltage source. Figure 31 shows a simplified circuit diagram of one embodiment of a battery unit 616 comprising a drain 612. The battery unit 616 may be attached to an instrument 102, for example, via its contacts 618. In this embodiment, the battery unit 616 may comprise a first grouping of cells 610 and a second grouping of cells 611. In one embodiment, the first and second grouping of cells 610, 611 may be lithium batteries. The first and second grouping of cells 610, 611 may each have a plurality of separate cells 610a, 610b, 611a, 611b arranged in a parallel formation. For example, the first and second grouping of cells 610, 611 may each be 6 VDC and arranged in a series configuration to produce 12 VDC at the contacts 618 of the battery unit 616 when fully charged. The cells 610a, 610b, 611a, 611b, however, may be electrically connected to one another in series or parallel or any other combination thereof. The number of cells 610a, 610b, 611a, 611b may be chosen to reduce the fire hazard resulting from the battery unit 616. For example, the number of connected cells may be selected such that the cumulative energy available to an arc or short is less than the energy required to ignite common shipping and/or packing materials. According to various embodiments, this value may be defined by appropriate government regulations.

[0085] In one embodiment, the drain 612 may comprise a first resistive element 622 and a second resistive element 624. As is to be appreciated, in some embodiments, the battery unit 616 may comprise, for example, multiple drains 612 each having more or less than two resistive elements or other circuitry. In the illustrated embodiment, the first resistive element 622 is coupled across a first anode 626 and a first cathode 628 of the first grouping of cells 610

through a first switch 630. The first resistive element 624 may be coupled across a second anode 632 and a second cathode 634 of the second grouping of cells 611 through a second switch 636. The first and second switches 630, 636 may be closed upon attachment of the battery unit 616 to the surgical instrument 102 in order to initiate the draining of the first and second grouping of cells 610, 611.

[0086] The value of the resistive elements utilized by the drain 612 may vary based on implementation. In one embodiment, the first resistive element 622 has a resistance in the range of about 90 ohms to about 110 ohms. In one embodiment, the first resistive element 622 has a resistance in the range of about 97 ohms to about 104 ohms. In one embodiment, the resistive element 622 is 102.9 ohms and has a power rating of 1 watt. The determination of the necessary resistance is based at least partially on the capacity of the voltage source, the voltage level of the voltage source, and the desired temporal length of the drainage curve. For example, in one embodiment the battery capacity of the first grouping of cells 610 is 1400 mAh, the voltage level is 6 VDC, and the target drain time is 24 hours. Dividing 1400 mAh by 24 hours yields a current of 0.0582 A. Using Ohm's law, 6 V divided by 0.0582A yields a resistance of 102.9 ohms. With a current of 0.0582 and a resistance of 102.9 ohms, the power dissipated by the resistor is 350W. As is to be appreciated, different voltage levels, battery capacities, and desired time of discharge will result in different resistance values.

[0087] Figure 32 is a simplified circuit diagram of one embodiment of a battery unit 716 comprising a first drain 712 and a second drain 713. The battery unit 716 may be attached to an instrument 102, for example, via its contacts 718. In this embodiment, the battery unit 716 comprises a first grouping of cells 710, a second grouping of cells 711, and a third cell 714. The first drain 712 comprises a first resistive element 722 and a second resistive element 724. The second drain 713 comprises a third resistive element 726. The resistive elements 722, 724, 726 are coupled to respective cells through switches 730, 736, and 738. The switches 730, 736, and 738 may be closed upon attachment of the battery unit 716 to the surgical instrument 102 in order to initiate the draining of the first and second grouping of cells 610, 611 and the third cell

716. The resistance of the third resistive element 726 may be similar or different from the resistances of the first and second resistive element 722, 724. As described above, the resistance of the third resistive element 726 may at least partially depend on the voltage of the third cell 714 and the desired characteristics of the drainage curve.

[0088] Figures 33-36 are perspective views of one embodiment of a battery unit 506 implementing the schematic of the battery unit 616 shown in Figure 31. The battery unit 506 may comprise a casing 802 defining an interior cavity 810. While the interior cavity 810 is illustrated in a central portion of the casing 802, it is to be appreciated that the internal cavity 810 may be positioned in any suitable location. The casing 802 may be covered by a cap 804 that may be secured to the casing 802 utilizing one or more mechanical latches 806, 808. Figure 34 illustrates one embodiment of the battery unit 506 with the cap 804 removed to show a plurality of cells 812 within. Any suitable number and/or type of cells 812 may be used. For example, CR123 and/or CR2 cells may be used. Figure 35 illustrates one embodiment of the battery unit 506 with a portion of the casing 802 removed to reveal the cells 812. Figure 36 illustrates one embodiment of the battery unit, with a portion of the casing 802 missing as in Figure 35. Figure 36 shows the battery pack 506 from a side 890 positioned to face distally when the battery pack 506 is installed on the surgical device 102. The interior cavity 810 is visible as well as a pair of contacts 886, 888 in electrical communication with the various cells 812.

[0089] Figures 37 and 38 illustrate cross-sectional views of one embodiment of the battery unit 506 including a translatable drain 812. The drain 812 may be positioned within the interior cavity 810 and may be translatable within the interior cavity 810 in the directions of arrow 815. Figures 37 shows the drain 812 in an open position and Figure 38 shows the drain 812 in a closed position. The drain 812 may comprise at least two contacts 816, 818. When the drain 812 is in the open position, a portion of the contacts 816, 818 may touch a non-conductive portion of the casing 802, such as fingers 820, 822. According to various embodiments, the contacts 816, 818 may be biased to exert a force against the fingers 820, 822 in order to resist movement of the drain 812 in the direction of the arrows 815. Also, in some embodiments, the

fingers 820, 822 may define one or more protrusions or stepped down portions, as shown in Figures 37 and 38. The battery unit 506 may also comprise one or more electrodes, such as first electrode 824 and second electrode 826. The first and second electrodes 824 and 826 may each be electrically coupled to a cathode or an anode of cells contained within the battery unit 506. In the closed position (Figure 38), the contacts 816, 818 are in electrical connection with the electrodes 824, 826, thereby allowing the voltage source to discharge through the drain 812. As discussed in more detail below, the drain 812 may be translated from the open position to the closed position upon attachment of the battery unit 506 to a surgical instrument.

[0090] Figure 43 is a perspective view of one embodiment of the drain 812 in accordance with one non-limiting embodiment. The contacts 816, 818 of the drain 812 may be coupled to a base portion 830 of the drain 812. Similarly contacts 836, 838 of the drain 812 may be coupled to the base portion 830 of the drain 812. According to various embodiments, the contacts 816, 818 may be electrically connected to one another via a resistive element (not shown) mounted to a circuit board 832. Similarly, the contacts 836, 838 may be electrically connected to one another via a resistive element mounted to the circuit board 832. As illustrated, the contacts 816, 818, 836, 838 may have a bend or curvature to bias the contacts towards an outward position when they are inwardly compressed. Additionally, in one embodiment, the distal end of each of the contacts 816, 818, 836, 838 may have an inwardly turned section. The base portion 830 may comprise a contacting surface 840 that engages the instrument when the battery unit 506 is attached to the instrument. Through this engagement, the drain 812 may be translated relative to the casing 802.

[0091] Figures 39-42 illustrate multiple views of a one embodiment of a battery dock 850. The battery dock 850 may be positioned within the handle 106 of the instrument 102 and may receive the battery unit 506. For example, the battery dock 850 may comprise a protruding member or bulkhead 858. The battery dock 850 may be positioned within the base sections 156, 158 and, in some embodiments, may be coupled to the frame sections 160, 162 such that the protruding member 858 extends proximally. The battery unit 506 may be installed into the

device 102 by pushing it distally against the battery dock 850. The protruding member 858 of the battery dock 850 may extend into the exterior cavity 810 of the battery unit 506. Contacts 882, 884 of the battery dock 850 may also extend into the interior cavity 810 of the battery unit 506. Within the cavity, the contacts 882, 884 of the battery dock 850 may be in electrical communication with the contact 886, 888 of the battery unit 506 (Figure 36). When the contacts 886, 888 of the battery unit 506 come into contact with the contacts 882, 884 of the battery dock 850, the battery unit 506 may be in electrical communication with the instrument 102.

[0092] Figure 44 illustrates one embodiment of the battery unit 506 attached to the battery dock 850. For clarity, various components have been removed. Referring now to Figures 37, 38, 43 and 44 as well as to Figures 39-42, the battery dock 850 is shown with its protruding member 858 sized to be received by the cavity 810 (Figure 33) of the battery unit 506. Prior to attachment, the drain 812 may be in the open position (Figure 37). During attachment of the battery unit 506 to the battery dock 850, the protruding member 858 is inserted into the cavity 810 and the battery unit 506 is moved relative to the battery dock 850 in the direction indicated by arrow 862. Eventually the distal end 860 of the protruding member 858 contacts the contacting surface 840 of the drain 812. As the user continues to attach the battery unit 506, the drain 812 is translated relative to the casing 802 in the direction indicated by arrow 864 and moves into the closed position (Figure 38). In this position, the battery unit 506 commences to slowly drain. When the battery unit 506 is removed from the battery dock 850, the drain 812 may remain in the position shown in Figure 38. In this way, the cells (not shown) of the battery unit 506 may drain any remaining charge across a resistive element either before or during disposal.

[0093] As is to be appreciated, the translatable discharge drain of the battery unit is not limited to the implementation illustrated in Figure 44. Figures 45 and 46, for example, illustrate one embodiment of a battery unit 900 and drain 912 with various components removed for clarity. The drain 912 that is translatable between an open position (Figure 45) and a closed position (Figure 46). In the open position, contacts 916, 918 are engaged with non-conductive

portions of a casing 920, 922, respectively. The drain 912 may ride in a track 914 when translating between the open position and the closed position. Figure 46 shows the battery unit 900 in a closed position after a ram 958 has translated the drain 912 in the direction indicated by arrow 964. The ram 958 may be a component of a battery dock of a surgical instrument, for example. In one embodiment, the battery dock comprises a cavity that is dimensioned to receive the battery unit 900, and the ram 958 is positioned within the cavity. In the closed position, the contacts 916, 918 are in electrical contact with electrodes 924, 926. The drain 912 may comprise a printed circuit board 932 to which at least one resistive element is mounted using a surface mount or a through-hole connection, for example.

[0094] Figures 47 and 48 illustrate a battery unit 1000 in accordance with another non-limiting embodiment. Various components have been omitted for clarity. The battery unit 1000 may comprise a drain 1012 that may be translatable between an open position (Figure 47) and a closed position (Figure 48). The battery unit 1000 may also comprise a first electrode 1024 with a contact 1025 and a second electrode 1026 with a contact 1027. The electrodes 1024, 1026 may be in contact with cells (not shown) of the battery unit 1000. In the open position, contacts 1016, 1018 of the drain 1012 are not engaged with contacts 1025, 1027 of the electrodes 1024, 1026. The drain 1012 may ride in a track 1014 when translating between the open position and the closed position. Figure 48 shows the battery unit 1000 in a closed position after a ram 1058 has translated the drain 1012 in the direction indicated by arrow 1064. The ram 1058 may be a component of a battery dock of a surgical instrument, for example. In the closed position, the contacts 1016, 1018 of the drain 1012 are in electrical contact with the contacts 1025, 1027 of the electrodes 1024, 1026. The drain 1012 may comprise a printed circuit board 1032 that includes at least one resistive element. In some embodiments, the contacts 1016, 1018 themselves may comprise the resistive elements. In fact, the resistive elements may be elements of any suitable resistance value and any suitable mechanical configuration.

[0095] Figure 49 is a perspective view of one embodiment of a battery unit 1100. Figures 50 and 51 show internal views of the battery unit 1100 during various stages of operation

with various components removed for clarity. The battery unit 1100 has one cell 1102 and an outer casing 1104 that defines a cavity 1110. The outer casing 1104 may be non-conductive and have conductive contacts for supplying energy to circuitry of a surgical instrument when the battery unit 1100 is attached to a surgical instrument. In one embodiment, the battery unit 1100 is received by a cavity in a pistol grip portion of a surgical instrument. The battery unit 1100 comprises a drain 1112 that is translatable between an open position (Figure 50) and a closed position (Figure 51). In one embodiment the drain 1112 has first and second contacts 1116, 1118 that are coupled to a circuit board 1132. The circuit board 1132 may include, for example, at least one resistive element. In some embodiments, the circuit board 1132 includes additional circuitry. The battery unit 1100 comprises a first electrode 1124 coupled to an anode of the cell 1102 and a second electrode coupled to a cathode of the cell 1102. Before the battery unit 1100 is attached to an instrument, the drain 1112 is in the open position (Figure 50). In the illustrated embodiment, the first contact 1116 is electrically coupled to the first electrode 1124 and the second contact 1118 is resting on, or otherwise contacting, a non-conductive finger 1120. As the battery unit 1100 is attached to an instrument, a protruding portion 1158 of the instrument may be received by the cavity 1110 and contact the drain 1112 to drive the drain 1112 in the direction indicated by the arrow 1164. In the closed position (Figure 51) the first contact 1116 is electrically coupled to the first electrode 1124 and the second contact 1118 is electrically coupled to the second electrode 1126. In this position, a closed circuit is created that allows the cell 1102 to discharge energy through the drain 1112. Additional embodiments of battery units are disclosed in commonly owned U.S. Patent Application Serial No. 12/884,995 entitled, "POWER CONTROL ARRANGEMENTS FOR SURGICAL INSTRUMENTS AND BATTERIES," filed on September 17, 2010 and incorporated herein by reference in its entirety. Still other embodiments of battery units are disclosed in commonly owned U.S. Patent Application Serial No. 12/884,838, entitled "SURGICAL INSTRUMENTS AND BATTERIES FOR SURGICAL INSTRUMENTS," filed on September 17, 2010 and also incorporated herein by reference in its entirety.

[0096] According to various embodiments, electrical connection of the battery unit 506 or other power supply to the motor 222 may initiate a firing of the instrument 102. Figure 52 illustrates one embodiment of a control circuit 1200 that may control a connection between the battery unit 506 or other power supply and the motor 222 or other drive device for firing the instrument 102. According to various embodiments, the control circuit 1200 may be implemented with components on a PC board 1202 shown in Figure 7. The control circuit 1200 may comprise various switches and other components for controlling the connection between the battery unit 506 and the motor 222. The battery unit 506 is shown with a positive electrode 1212 and a negative electrode 1210. Similarly, the motor 222 is shown with a positive terminal 1216 and a negative terminal 1214. It will be appreciated that the polarity of the circuit 1200 could be reversed, for example, based on other design considerations.

[0097] The control circuit 1200 may comprise a firing switch 220 (also shown in Figure 9), which may be in mechanical communication with the firing trigger 120 (*e.g.*, via an actuator 221). The control circuit 1200 may also comprise an end-of-stroke/reverse motor switch 1204 and a clamp switch 1206. The end-of-stroke/reverse motor switch 1204 may be actuated when the firing bar 108 reaches the end of its stroke (*e.g.*, at or near its distal-most position). Also, according to various embodiments, the end-of-stroke/reverse motor switch 1204 may be actuated manually by the clinician prior to the end of the stroke of the firing bar 108 to abort and/or reverse the firing of the instrument 102. A clamp switch 1206 may be actuated when the end effector 104 is closed (*e.g.*, the anvil 112 and elongate channel 110 are brought into contact with one another) and also when the end effector 104 is opened. A clamping relay 1208 may also be a component of the circuit 1200. According to various embodiments, the relay 1208 may be a non-solid state relay (*e.g.*, a mechanical relay, an electromagnetic relay, *etc.*). This may allow the instrument 102 to be subjected to gamma sterilization as well as other sterilization techniques that have the potential to damage solid state components. It will be appreciated, however, that the clamping relay 1208 may, in various embodiments, be replaced with any sort of switching

device including, for example, a field effect transistor (FET), bipolar junction transistor (BJT), *etc.* Also, in some embodiments, the relay 1208 may be replaced with a microprocessor.

[0098] When the instrument is ready for use (*e.g.*, a staple cartridge 132 is loaded to the elongate channel 110), the control circuit 1200 may be configured as shown in Figure 52. The end-of-stroke/reverse motor switch 1204 may be connected between 1 and 3, creating an electrical connection between the positive electrode 1212 of the battery and the positive terminal 1216 of the motor 222. The relay 1208 may be in a closed state. For example, an electrical connection may be made between pins 4 and 5 of the relay 1208. The firing switch 220 may be connected between points 1 and 3, creating an electrical connection between the positive electrode 1212 of the battery 506 and the negative terminal 1214 of the motor 222. Because both terminals 1214, 1216 of the motor 222 are connected to a single electrode 1212 of the battery 506, the motor 222 may not operate.

[0099] The clinician may initiate a firing operation by actuating the firing trigger 122, which, via the actuator 221, may cause the firing switch 220 to transition to a second state where the points 1 and 3 are connected. This may create an electrical connection between the negative terminal 1214 of the motor 222 and the negative electrode 1210 of the battery 506 (*e.g.*, via pints 1 and 2 of the firing switch 220 and pins 4 and 5 of the relay 1208. This may cause the motor 222 to rotate in a forward direction. For example, the motor may rotate the gearbox 224, intermediate gear 230, drive gear 232 and rack 238 to ultimately push the firing bar 108 distally.

[0100] When the firing bar 108 reaches the end of its stroke, the end-of-stroke switch 1204 may transition from the position shown in Figure 52 to a position where the points 1 and 2 of the switch 1204 are connected. This may connect pin 3 of the relay 1208 to the negative electrode 1210 of the battery 506 (*e.g.*, via the pin 4-5 connection of the relay 1208). In turn, this may energize the relay 1208 causing removal of the electrical connection between pins 4 and 5 and generation of an electrical connection between pins 5 and 6. When the clinician releases the firing trigger 122, the firing switch may revert to the state shown in Figure 52. This may cause the motor 222 to be connected to the battery 506 with a reverse polarity. For example, the

positive terminal 1216 of the motor 222 may be connected to the negative electrode 1210 of the battery 506 via the switch 1204 and the relay 1208 (*e.g.*, via pins 5 and 6). The negative terminal 1214 of the motor 222 may be connected to the positive electrode 1212 of the battery 506 via the firing switch 220. As a result, the motor 222 may rotate in reverse, pulling the firing bar 108 proximally, via the gearbox 224, intermediate gear 230, drive gear 232 and rack 238.

[0101] At the conclusion of the firing operation, the relay 1208 may be in a state where there is no electrical connection between pins 4 and 5. In this state, the instrument 102 may not be re-fired (*e.g.*, the motor 222 may not be connected to the batter 506 with the correct polarity to cause forward rotation). According to various embodiments, a clamp switch 1206 may be positioned to energize the relay 1208 (*e.g.*, pulling pin 1 low) in order to transition the relay 1208 back to the initial state having an electrical connection between pins 4 and 5. This may allow the instrument 102 to fire again. The clamp switch 1206 may be in mechanical communication with a portion of the drive train actuated by the closure trigger 120 to close the anvil 114 against the elongate channel 110. For example, the clamp switch 1206 may be in mechanical communication with the clamp lock 244 described herein above. When the anvil 114 is closed against the elongate channel 110 (*e.g.*, when the clamp lock 244 is engaged), the switch 1206 may be in the position shown in Figure 52, resulting in an electrical connection between points 1 and 3 of the switch 1206. When the clamp lock 244 is disengaged, the clamp switch 1206 may be configured to create an electrical connection between points 1 and 2, energizing the relay 1208 as described. Accordingly, after the instrument 102 is fired, the circuit 1200 may be configured to prevent the motor 222 from operating in the forward direction until the end effector 104 is re-opened. This may prevent the clinician from accidentally re-firing the instrument 102 before the end effector 104 is opened to install a new staple cartridge 132. According to various embodiments, the instrument 102 may comprise a mechanical lock-out device in addition to the relay lock-out implemented by the circuit 1200. The circuit 1200, as described herein, however, may prevent the clinician from driving the instrument 102 into the

mechanical lock-out. This may save wear and tear on the instrument 102 and may also prevent clinician confusion that may occur when the device is in a mechanical lock-out state.

[0102] Figure 53 illustrates one embodiment of the control circuit 1200 with additional switches and features. For example, the circuit 1200, as shown in Figure 53, may additionally comprise an emergency access or bailout door switch 1218. The emergency access door switch 1218 may be in mechanical communication with the emergency access door 248. For example, when the emergency access door 248 is in place, the switch 1204 may be closed, as shown in Figure 53. When the emergency access door 248 is removed, the switch 1204 may be opened, creating an open circuit relative to the negative terminal of the battery 506. A stroke position switch 1220 may be connected to switch a resistive element 1222 into and out of the circuit 1200 based on the position of the firing bar 108. The resistive element may be a single resistor and/or a resistor network connected in series, parallel (as shown) or any other suitable configuration. When the resistive element 1222 is switched into the circuit 1200, the current provided to the motor 222 may be reduced. This may reduce the speed and torque provided by the motor 222. Additionally, the control circuit 1200, as illustrated in Figure 53 may comprise a PTC or other thermal fuse element 1224 to break a connection between the motor 222 and the battery 506 in the event that too much heat is generated (*e.g.*, by the resistive element 1222).

[0103] Figure 54 is a flowchart showing one embodiment of a process flow 1301 showing the firing of the instrument 102 utilizing the control circuit 1200 as illustrated in Figure 53. At 1300, the instrument 102 may be ready to fire. For example, the switches 1218, 1206, 1220, 220, 1204 and relay 1208 may be configured as illustrated in Table 1 below:

Table 1

Switch	Pin/Point Connection
Emergency Access Door (1218)	1-2
Clamp (1206)	1-2
Stroke Position (1220)	1-2
Fire (220)	1-3
End-of-stroke/Motor Direction (1204)	1-3

Relay (1208)	4-5
--------------	-----

At 1302, the clinician may actuate the firing trigger 122. This may cause the fire switch 220 to close, creating a connection between points 1 and 2 of the switch 220. Accordingly, the positive terminal of the motor 222 may be connected to the positive electrode 1212 of the battery 506 via the end-of-stroke/motor direction switch 1204. The negative terminal 1214 of the motor 222 may be connected to the negative electrode 1210 of the battery 506 via the thermal fuse element 1224, the resistive element 1222, and the connection between pins 4 and 5 of the relay. This may cause rotation of the motor 222 resulting in distal movement of the firing bar 108 (*e.g.*, via the gearbox 224, intermediate gear 230, drive gear 232 and rack 238). Because the resistive element 1222 is electrically connected between the motor 222 and the battery 506, the current provided to the motor 222 may be reduced. This may, in turn, reduce the speed and/or torque provided by the motor 222 while the resistive element 1222 is active.

[0104] At 1304, the firing bar 108 may pass a predetermined position in its firing stroke. This may cause the stroke position switch 1220 to be opened, causing a connection between points 1 and 2 of the switch 1220. This may, in turn, switch the resistive element 1222, thermal fuse 1224, and relay 1208 out of circuit, allowing full current to be provided to the motor 222. The predetermined position in the firing stroke, in various embodiments, may be a point past which a mechanical lockout is no longer possible and/or likely. For example, the resistive element 1222 may be utilized to limit the current to the motor 222 during the portion of the firing stroke where the firing bar 108 or other drive train element may encounter a mechanical lock-out. This may limit damage to the drive train or other component of the device 102 if the mechanical lock-out is encountered. When the possibility of encountering a mechanical lock-out has passed, the stroke position switch 1220 may be actuated to switch out the resistive element 1222, allowing full power to be provided to the motor 222 (*e.g.*, for cutting tissue).

[0105] The firing bar 108 may reach the end of its stroke (*e.g.*, at or near its distal-most position) at 1306. At this point, the end-of-stroke/motor direction switch 1204 may be actuated, causing it to be connected between points 1 and 2. In this way, the positive terminal 1216 of the

motor 222 may be electrically connected to the negative electrode 1210 of the battery 506. The pin 3 of the relay 1208 may also be electrically connected to the negative electrode 1210 of the battery 506, energizing the relay 1208 and breaking the connection between relay pins 4 and 5. When the clinician releases the trigger 122 at 1308, the firing switch 220 may also be actuated, causing it to be connected between points 1 and 2. This may cause the negative terminal 1214 of the motor to be electrically connected to the positive electrode 1212 of the battery 506. In this way, the rotation direction of the motor 222 may be reversed, causing the motor 222 to return the firing bar to its initial, proximal position (*e.g.*, via the via the gearbox 224, drive gear 232 and rack 238).

[0106] Similar to embodiment described above, when the relay 1208 is opened (*e.g.*, the connection between pins 4 and 5 is broken), it may not be possible to rotate the motor 222 in a forward direction to fire the firing bar 108 until the clamp switch 1206 is actuated (*e.g.*, by opening the end effector 104). In this way, the clinician may be prevented from re-firing the instrument 102 prior to opening the end effector 104, for example, to load a new staple cartridge 132. Also, similar to the embodiment described above, the clinician may abort a firing stroke by manually switching the end-of-stroke/motor direction switch 1204 to the state where points 1 and 2 are connected, causing the circuit 1200 and instrument 102 to behave as described above with respect to 1306 and 1308.

[0107] Figures 55-59 show the orientation and operation of various embodiments of the switches 1218, 1206, 1220, 220, and 1204 described above. Figure 55 illustrates a perspective view of one embodiment of the circuit board 1202 coupled to the battery dock 850. The circuit board 1202 and battery dock 850, as shown, may be positioned within the handle 106 of the instrument 102, for example, as illustrated in Figure 7. Figure 55 shows, on the circuit board 1202, the emergency access door switch 1218, the clamp switch 1206, the stroke position switch 1220, the trigger switch 220 and the end-of-stroke/motor direction switch 1204. Figure 56 illustrates a cut away view of one embodiment of the instrument 102 showing the emergency access door switch 1218. The switch 1218 may comprise an actuator 1304, which may be spring

biased. The emergency access door 248, as shown, may comprise an arm 1302. The arm 1302 may be positioned under the actuator 1304 of the switch 1218. When the emergency access door 248 is removed, the arm 1302 may be removed from under the actuator 1304, changing the state of the switch 1218.

[0108] Figure 57 illustrates another cut away view of one embodiment of the instrument 102 showing the clamp switch 1206. The clamp switch 1206 may comprise an actuator 1306. The actuator 1306 may be positioned such that the state of the switch 1206 is changed when the clamp release button 124 is actuated to unclamp the end effector 104.

[0109] Figure 58 shows another cut away view of one embodiment of the instrument 102 showing the stroke position switch 1220. The stroke position switch 1220 may comprise an actuator 1308 and an actuator lever 1310. The actuator lever 1310 may ride along a top surface of the rack 238. According to various embodiments, the rack 238 may define an indentation 1312 along its top surface. The indentation 1312 may be positioned longitudinally on the rack such that the actuator lever 1310 of the switch 1220 falls into the indentation 1312 at the predetermined position of the firing stroke referred to with respect to Figure 54. Alternatively, it will be appreciated that the rack 238 may comprise a protrusion positioned to contact the actuator at the predetermined part of the firing stroke.

[0110] Figure 59 illustrates another cut away view of one embodiment of the instrument 102 showing the end-of-stroke/motor reverse switch 1204. The switch 1204 may comprise an actuator 1322. The actuator 1322 may be activated by an external reverse motor button 1320 or by the rack 238 as it reaches the distal end of its travel (*e.g.*, indicating an end of the stroke of the firing bar 108). For example, the rack 238 may comprise a protrusion 1324 that contacts the actuator 1322 of the switch 1204. Also, for example, the rack 238 may comprise an indentation or cavity (not shown) positioned to contact the actuator 1322 at the distal end of the travel of the track 238.

[0111] Although the device described herein shows the rotational movement of the motor 222 being translated into longitudinal motion in the handle 106 (*e.g.*, via the rack 238 and

firing bar 108), it will be appreciated that instruments according to various embodiments may perform this translation outside of the handle, for example, in the shaft, or at the end effector itself. For example, in some embodiments, a rotating drive shaft (not shown) may extend some or all of the way through the shaft 114 from the handle 106 to the end effector 104. The various switches described herein may be utilized in such an embodiment. For example, the various switches described herein may be positioned to be actuated in the same relationship to the position of the firing bar 108 as described herein.

[0112] While the present invention has been illustrated by description of several embodiments and while the illustrative embodiments have been described in considerable detail, it is not the intention of the applicant to restrict or in any way limit the scope of the appended claims to such detail. Additional advantages and modifications may readily appear to those skilled in the art. For another example, although the E-beam firing beam 108 has advantages for an endoscopically employed surgical severing and stapling instrument 102, a similar E-Beam may be used in other clinical procedures. It is generally accepted that endoscopic procedures are more common than laparoscopic procedures. Accordingly, the present invention has been discussed in terms of endoscopic procedures and apparatus. However, use herein of terms such as “endoscopic”, should not be construed to limit the present invention to a surgical stapling and severing instrument for use only in conjunction with an endoscopic tube (i.e., trocar). On the contrary, it is believed that the present invention may find use in any procedure where access is limited to a small incision, including but not limited to laparoscopic procedures, as well as open procedures. For yet another example, although an illustrative handle portion 106 described herein is manually operated by a clinician, it is consistent with aspects of the invention for some or all of the functions of a handle portion to be powered (e.g., pneumatic, hydraulic, electromechanical, ultrasonic, etc.). Furthermore, controls of each of these functions may be manually presented on a handle portion or be remotely controlled (e.g., wireless remote, automated remote console, etc.).

[0113] It is to be understood that at least some of the figures and descriptions herein have been simplified to illustrate elements that are relevant for a clear understanding of the disclosure, while eliminating, for purposes of clarity, other elements. Those of ordinary skill in the art will recognize, however, that these and other elements may be desirable. However, because such elements are well known in the art, and because they do not facilitate a better understanding of the disclosure, a discussion of such elements is not provided herein.

[0114] While several embodiments have been described, it should be apparent, however, that various modifications, alterations and adaptations to those embodiments may occur to persons skilled in the art with the attainment of some or all of the advantages of the disclosure. For example, according to various embodiments, a single component may be replaced by multiple components, and multiple components may be replaced by a single component, to perform a given function or functions. This application is therefore intended to cover all such modifications, alterations and adaptations without departing from the scope and spirit of the disclosure as defined by the appended claims.

[0115] Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

CLAIMS

What is claimed is:

1. A powered surgical instrument for cutting and fastening tissue, the instrument comprising:
 - an end effector comprising:
 - a first jaw member;
 - a second jaw member coupled to move relative to the first jaw member from an open position, where the jaw members are apart from one another, to a closed position; and
 - a firing bar positioned to fire by translating within the end effector when the first and second jaw members are in the closed position; and
 - a drive device mechanically coupled to the firing bar; and
 - a clamping trigger mechanically coupled to the end effector such that actuation of the clamping trigger causes the second jaw member to pivot towards the first jaw member;
 - a control circuit, wherein the control circuit comprises:
 - a firing switch configured to be in electrical communication with a power supply for powering the drive device and in electrical communication with the drive device;
 - a clamp switch in mechanical communication with the clamping trigger;
 - a latching device in electrical communication with the clamp switch, the power supply and the drive device; and
 - an end-of-stroke switch in electrical communication with the latching device; and
 - wherein the firing switch is electrically connected to, upon actuation, connect the power supply to the drive device via a first connection comprising the latching device and the firing switch;
 - wherein the end-of-stroke switch is electrically connected to, upon sensing an end of a stroke of the firing bar, cause a change in a state of the latching device to break the first connection between the power supply and the drive device.
2. The surgical instrument of claim 1, wherein the clamp switch is electrically and mechanically connected, upon release of the clamping trigger, to energize the relay to reestablish the connection between the power supply and the drive device.

3. The surgical instrument of claim 1, wherein the first jaw member is shaped to receive a staple cartridge and the second jaw member defines at least one staple pocket for receiving and forming a staple.

4. The surgical instrument of claim 3, wherein the firing bar is in mechanical communication with a staple driver to push the staple driver distally upon firing.

5. The surgical instrument of claim 1, wherein the firing bar comprises a cutting edge.

6. The surgical instrument of claim 1, further comprising a rack translatable distally and proximally within the handle, wherein the rack is in mechanical communication with the firing bar, wherein the rack defines at least one geared face.

7. The surgical instrument of claim 6, wherein the drive device is positioned to rotate a gear in mechanical communication with the rack.

8. The surgical instrument of claim 7, wherein rotational motion of the drive device and gear in a first direction causes the rack and the firing bar to translate distally, and wherein rotational motion of the drive device and gear in a second direction causes the rack and the firing bar to translate proximally.

9. The surgical instrument of claim 6, wherein the rack defines a protrusion, and wherein the end-of-stroke switch comprises an actuator positioned to contact the protrusion to actuate the end-of-stroke switch when the rack reaches a position indicating the end of the firing bar stroke.

10. The surgical instrument of claim 6, wherein the control circuit further comprises a stroke position switch positioned to actuate when the firing bar reaches a predetermined position; and a resistive element in electrical communication with the stroke position switch, wherein the stroke position switch is electrically connected to electrically switch the resistive element

between the power supply and the drive device until actuated in response to the firing bar reaching the predetermined position.

11. The surgical instrument of claim 10, wherein the stroke position switch comprises an actuator, and wherein the rack defines a cavity positioned to receive the actuator of the stroke position switch to actuate the stroke position switch when the firing bar reaches the predetermined position.

12. The surgical instrument of claim 1, wherein the handle further comprises a clamp lock mechanically positioned to lock the second jaw member against the first jaw member.

13. The surgical instrument of claim 12, wherein the clamp switch comprises an actuator positioned to be actuated upon release of the clamp lock.

14. The surgical instrument of claim 1, wherein the control circuit further comprises an emergency access door switch coupled to an emergency access door of the handle such that opening of the emergency access door actuates the emergency access door switch to break an electrical connection to the power supply.

15. The surgical instrument of claim 1, wherein the latching device is a relay.

16. The surgical instrument of claim 15, wherein the relay is a latching relay.

17. The surgical instrument of claim 1, wherein the relay is at least one of a mechanical relay and an electromagnetic relay.

18. A powered surgical instrument for cutting and fastening tissue, the instrument comprising:

an end effector comprising:

a first jaw member;

a second jaw coupled to pivot relative to the first jaw member; and

a firing bar positioned to fire by translating distally within the end effector when the first and second jaw members are pivoted to a closed position; and

a handle, wherein the handle comprises:

a clamping trigger mechanically coupled to the end effector such that actuation of the clamping trigger causes the second jaw member to pivot towards the first jaw member;

a firing trigger;

a drive device mechanically coupled to the firing bar at least distally; and

a control circuit, wherein the control circuit comprises:

a firing switch in electrical communication with a power supply for powering the drive device and in electrical communication with the drive device, and in mechanical communication with the firing trigger;

a clamp switch in mechanical communication with the clamping trigger;

a stroke position switch positioned to actuate when the firing bar reaches a predetermined position;

a resistive element in electrical communication with the stroke position switch;

a relay in electrical communication with the clamp switch, the power supply and the drive device; and

an end-of-stroke switch in electrical communication with the relay; and

wherein the firing switch is electrically connected such that actuation of the firing trigger connects the power supply to the drive device via a first connection comprising the relay and the firing switch;

wherein the end-of-stroke switch is electrically connected to, upon sensing an end of the firing bar stroke, energize the relay and break the first connection between the power supply and the drive device; and

wherein actuation of stroke position switch causes the resistive element to be electrically isolated from at least one of the power supply and the drive device.

19. The surgical instrument of claim 18, wherein the control circuit further comprises an emergency access door switch coupled to an emergency access door of the handle such that opening of the emergency access door actuates the emergency access door switch to break an electrical connection to the power supply.

20. The surgical instrument of claim 18, further comprising a rack translatable distally and proximally within the handle, wherein the rack is in mechanical communication with the firing bar, wherein the rack defines at least one geared face.

21. The surgical instrument of claim 20, wherein the drive device is positioned to rotate a gear in mechanical communication with the rack.

22. The surgical instrument of claim 20, wherein the stroke position switch comprises an actuator, and wherein the rack defines a cavity positioned to receive the actuator of the stroke position switch to actuate the stroke position switch when the firing bar reaches the predetermined position.

23. The surgical instrument of 18, wherein the control circuit further comprises a thermal fuse electrically connected between the power supply and the drive device when the resistive element is electrically connected between the power supply and the drive device.

24. The surgical instrument of claim 18, wherein the relay is a latching relay.

25. The surgical instrument of claim 18, wherein the relay is at least one of a mechanical relay and an electromagnetic relay.

1/43

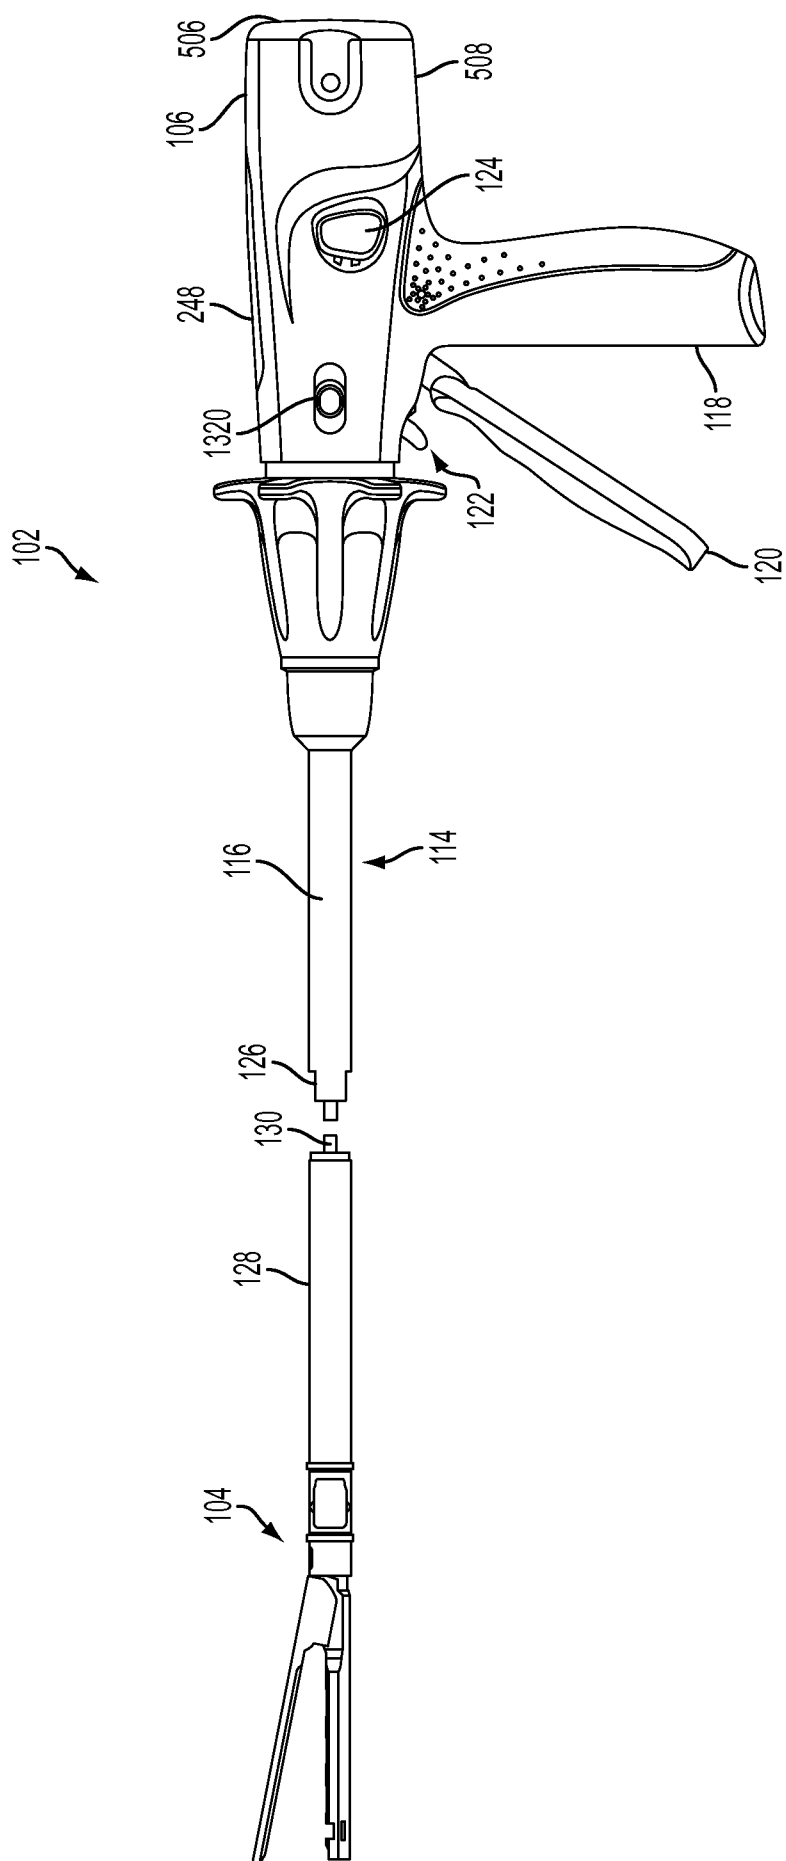


FIG. 1

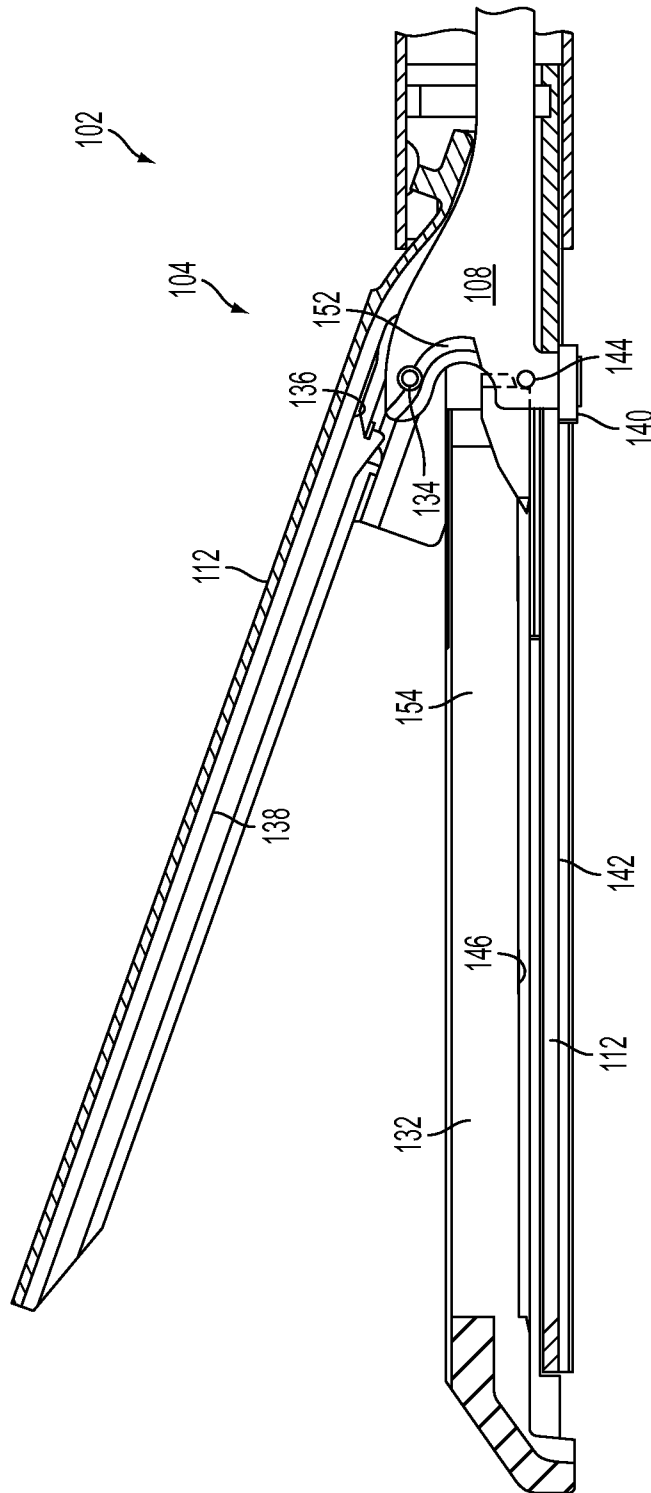


FIG. 2

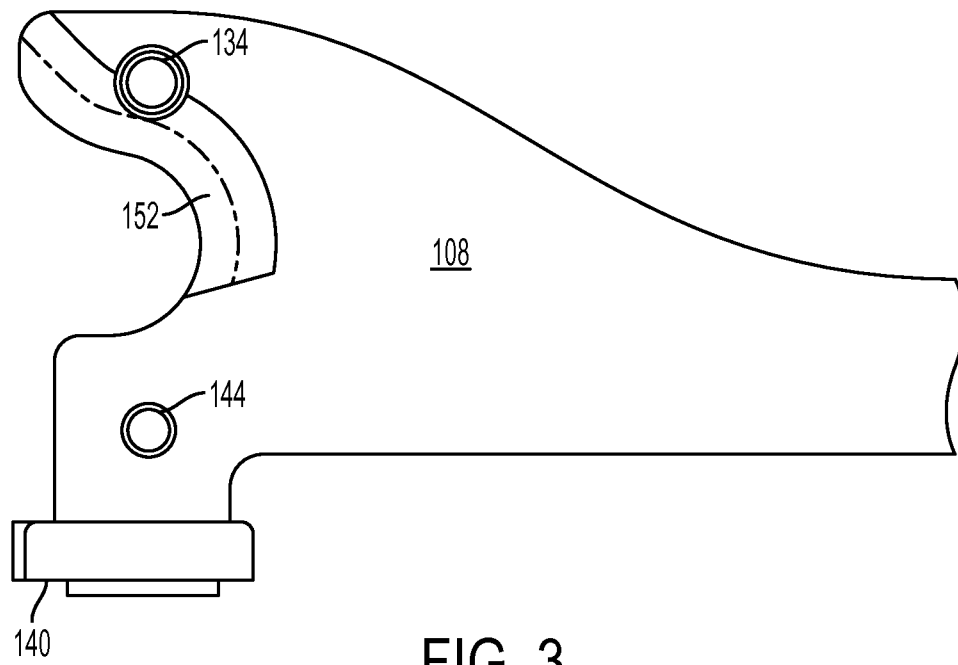


FIG. 3

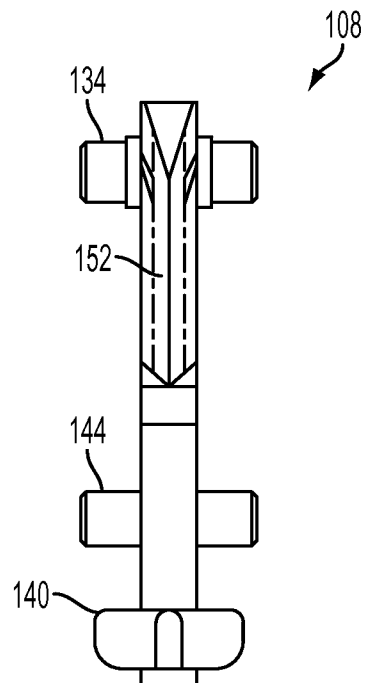


FIG. 4

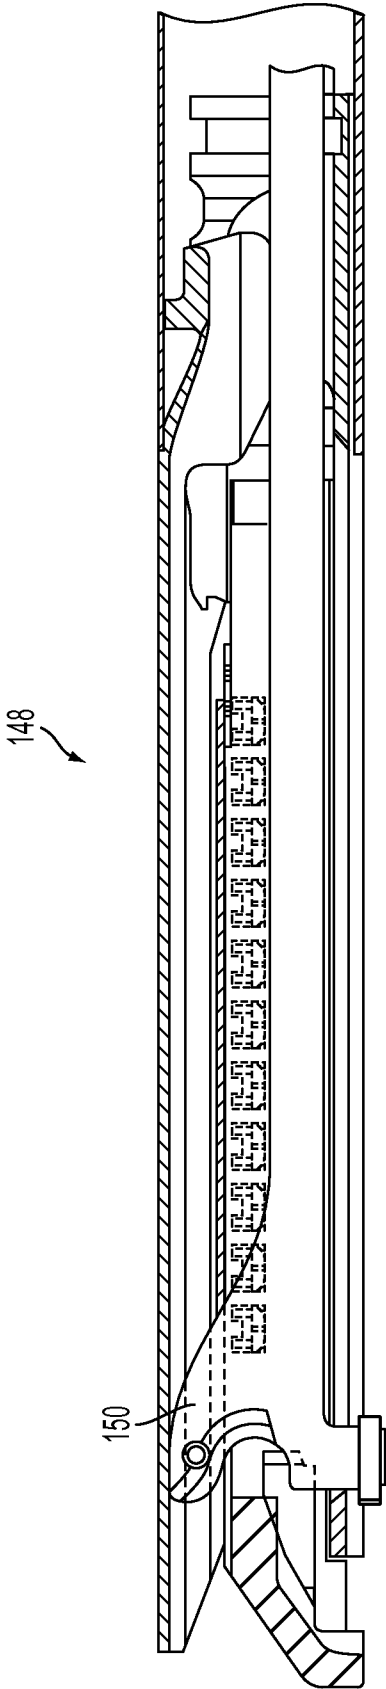


FIG. 5

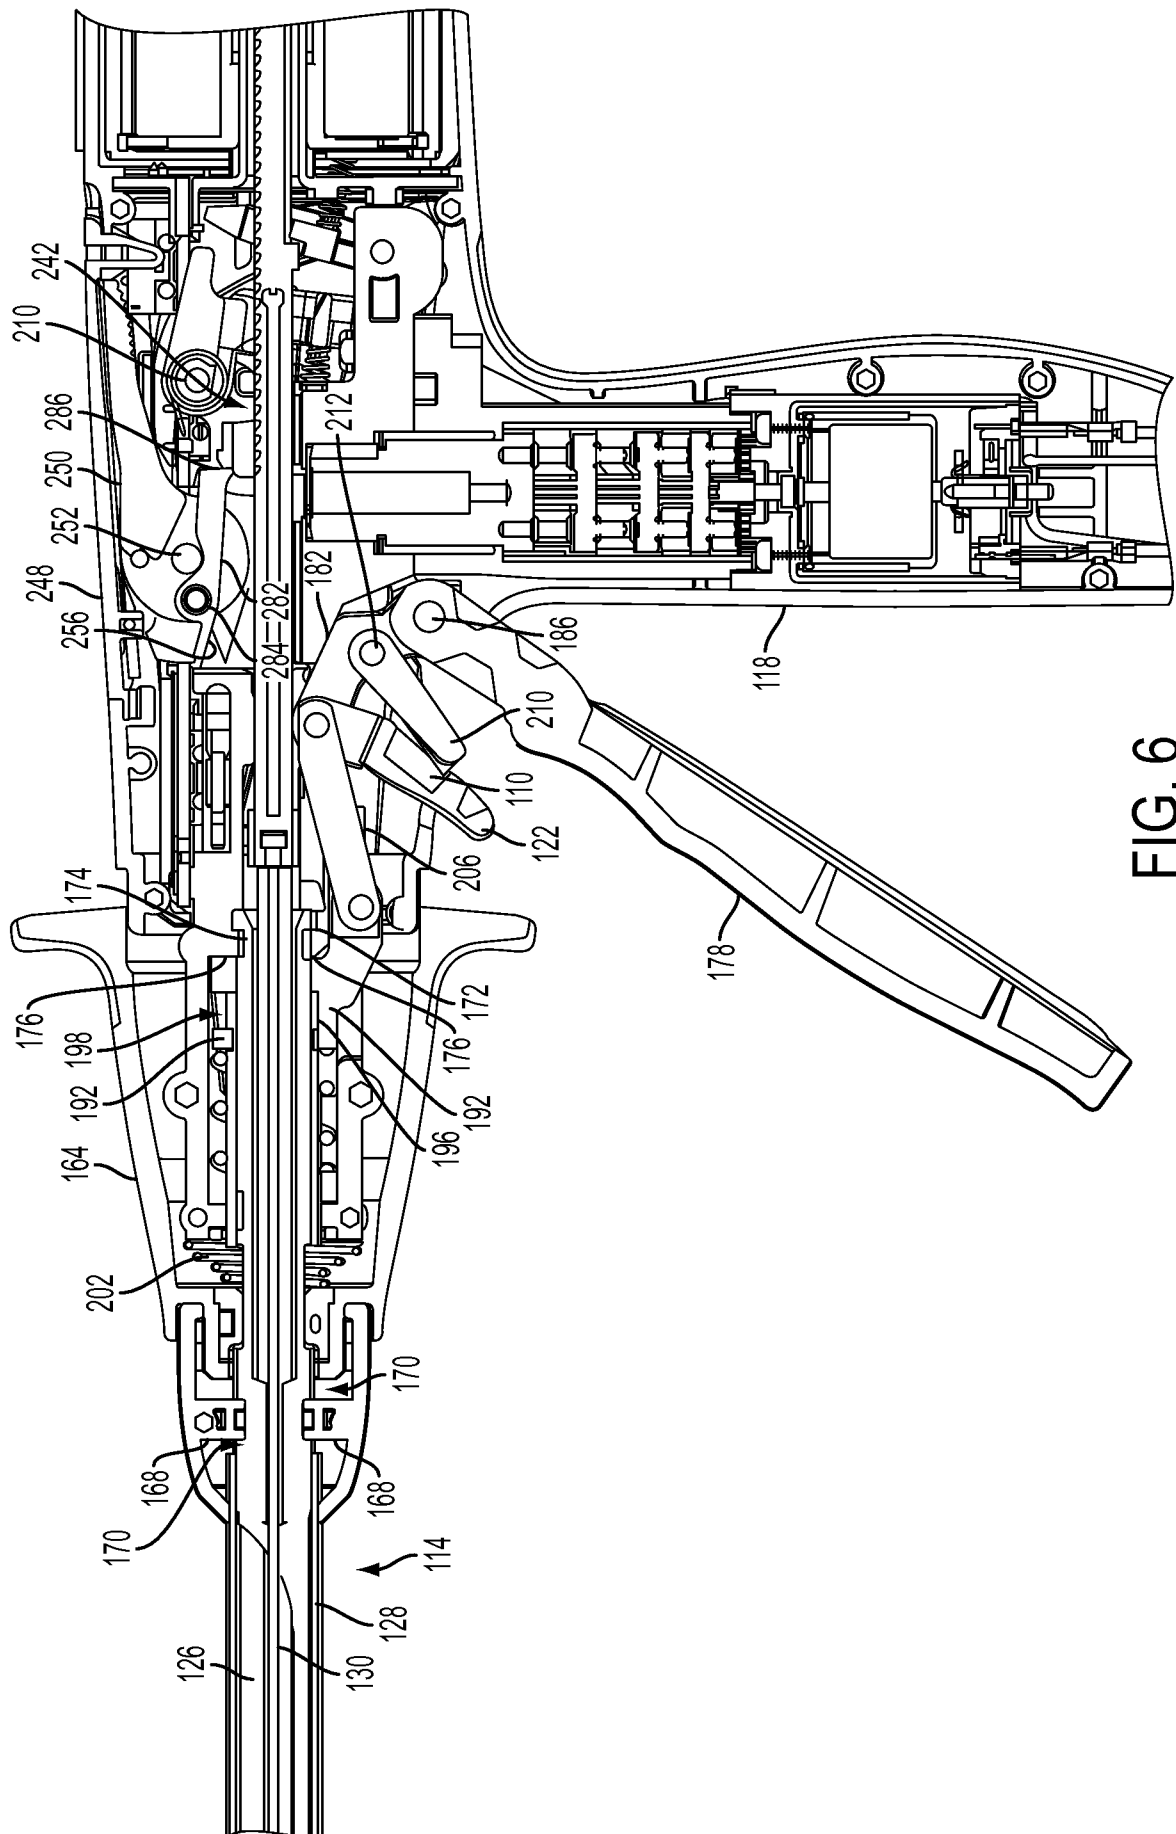


Fig. 6

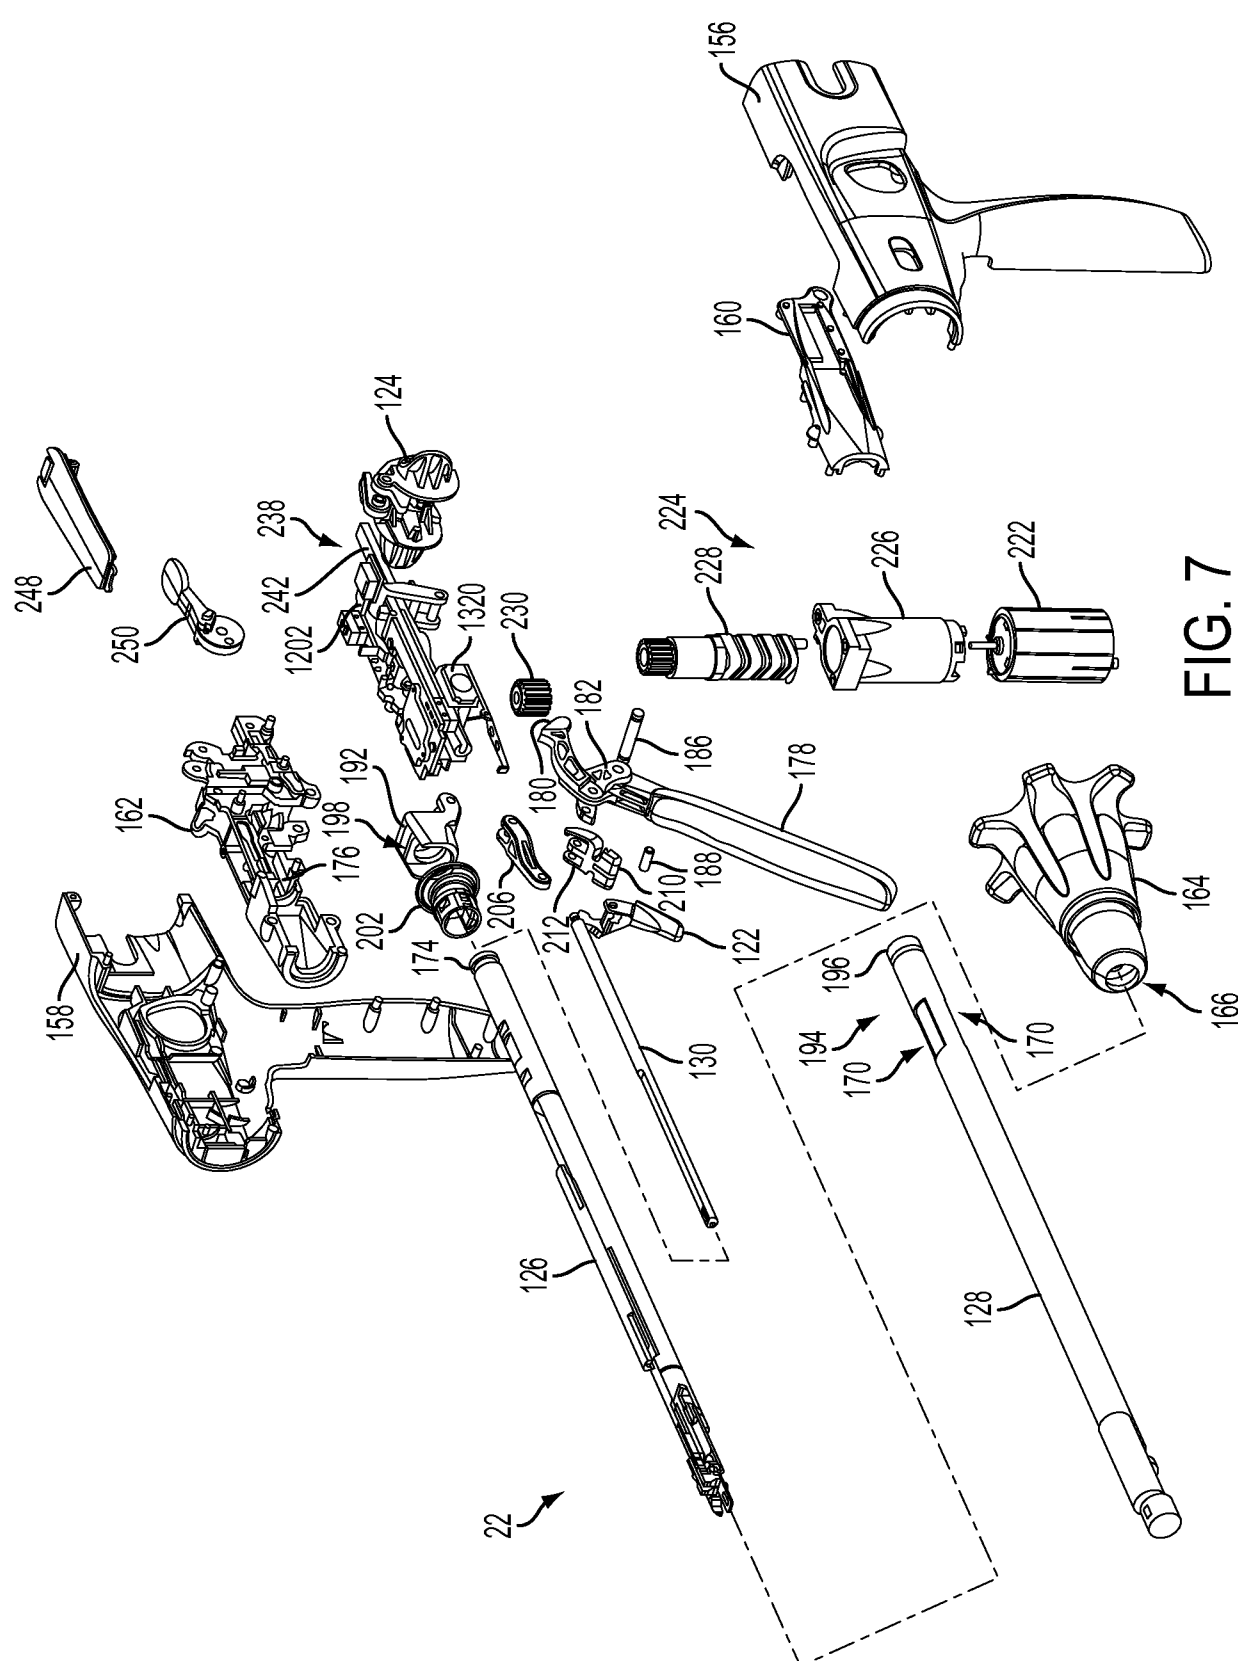


FIG. 7

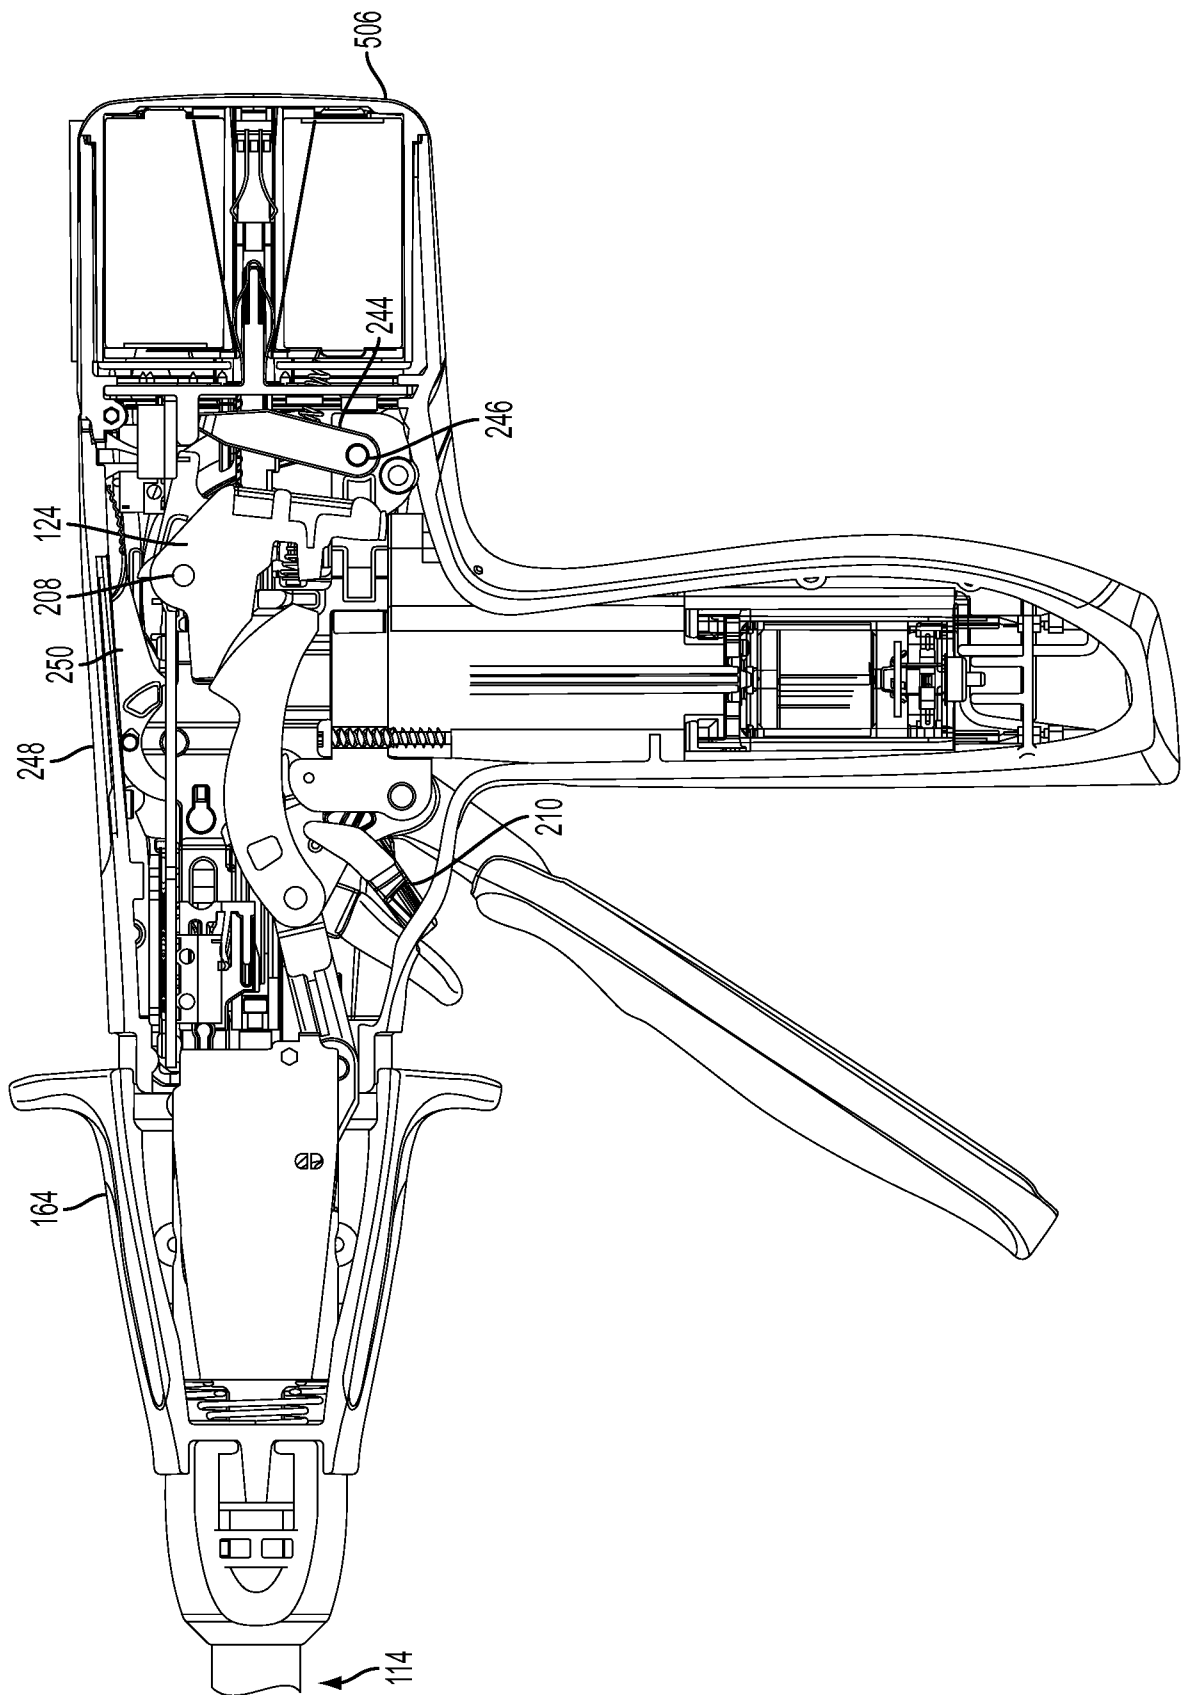


FIG. 8

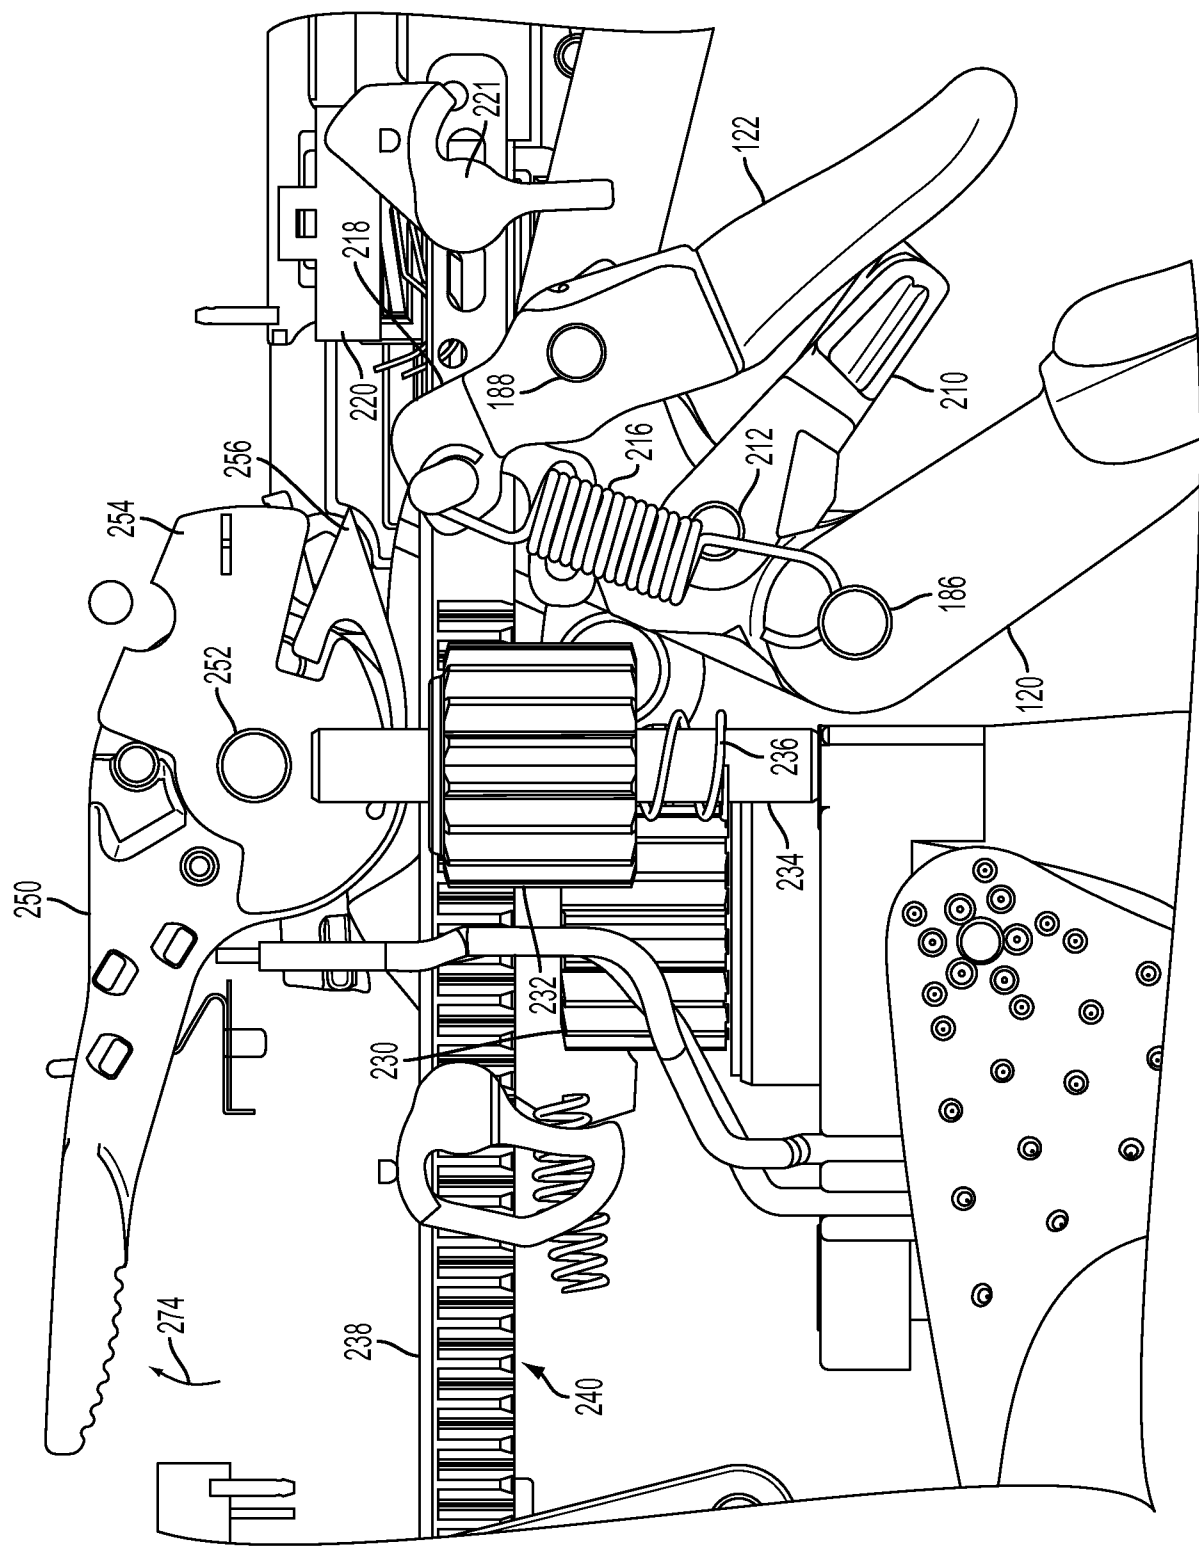


FIG. 9

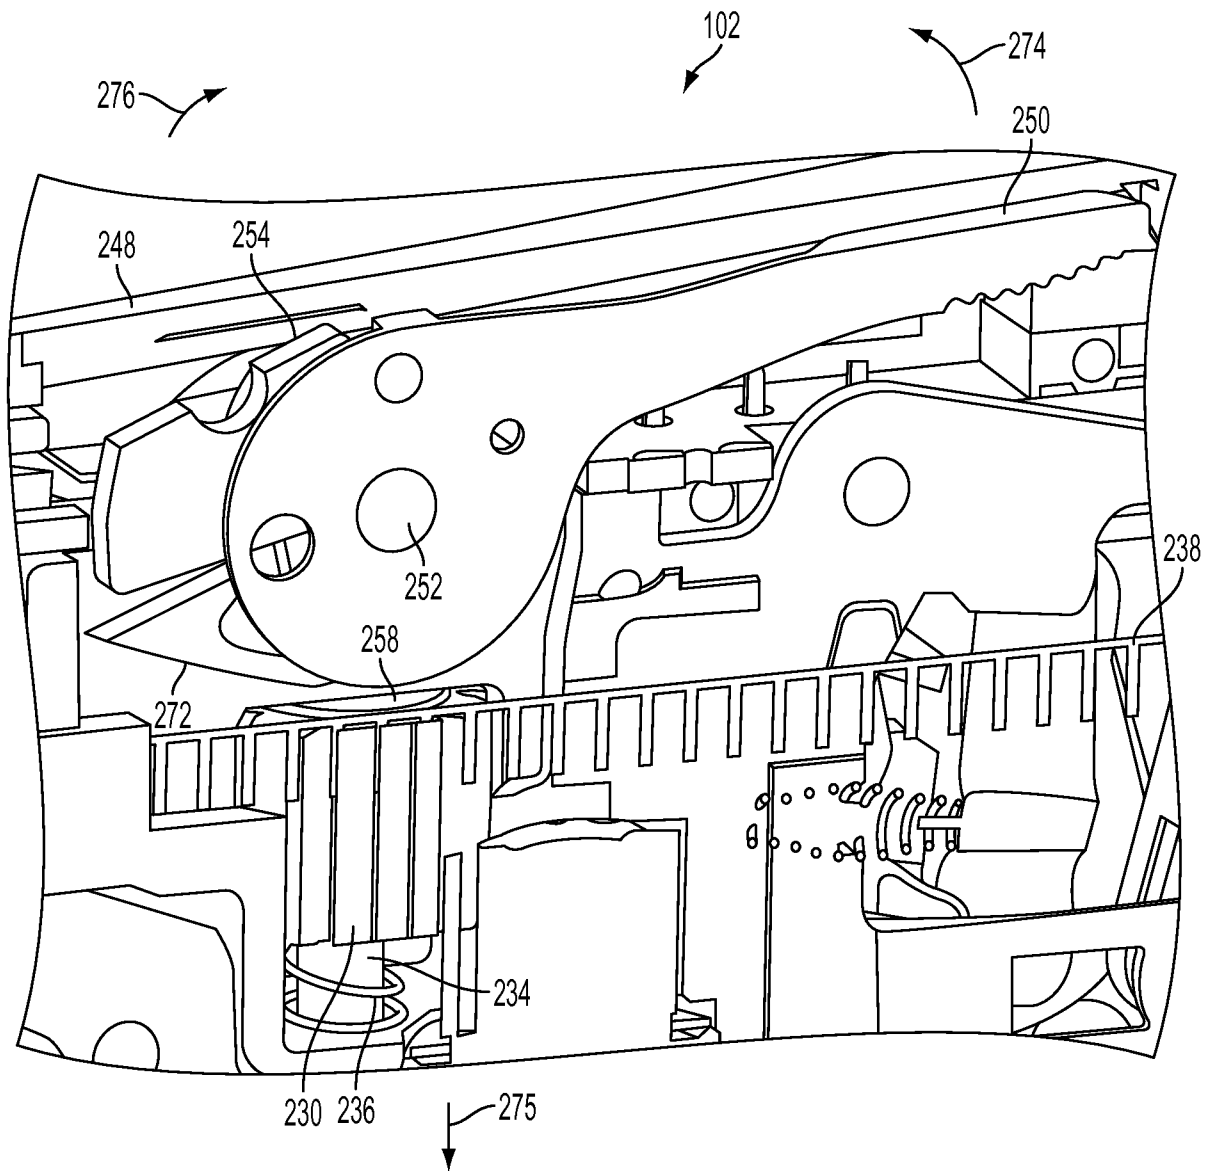


FIG. 10

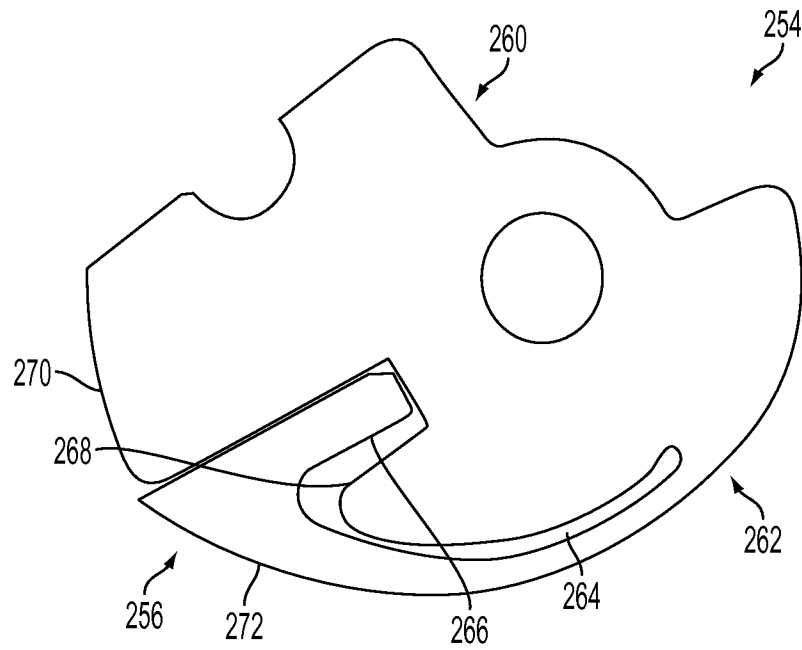


FIG. 11

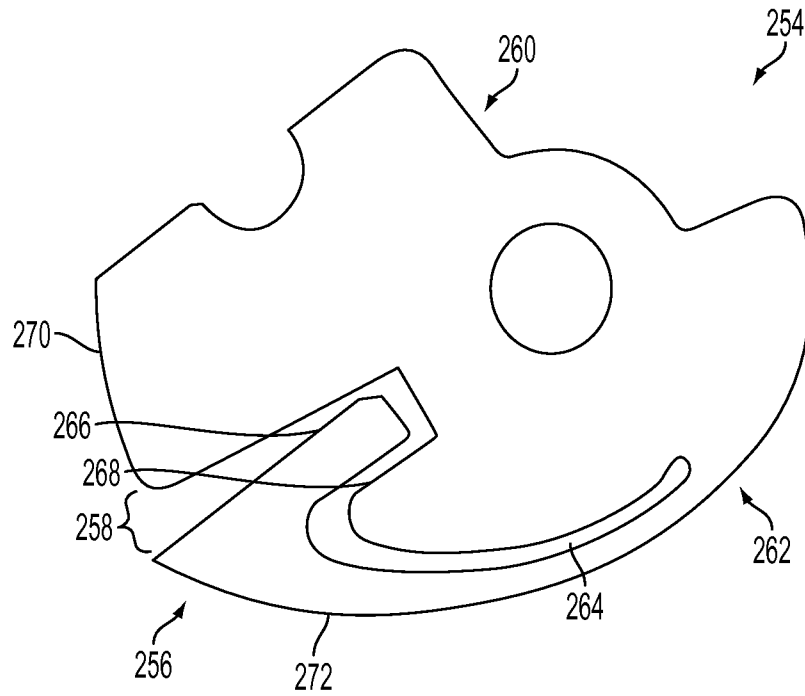


FIG. 12

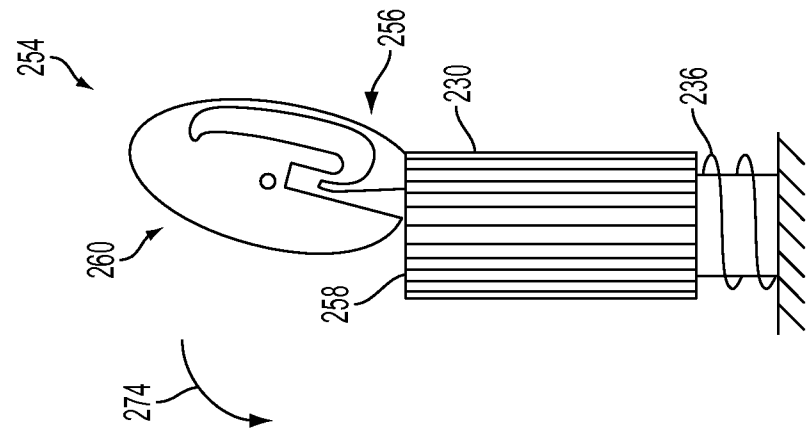


FIG. 13

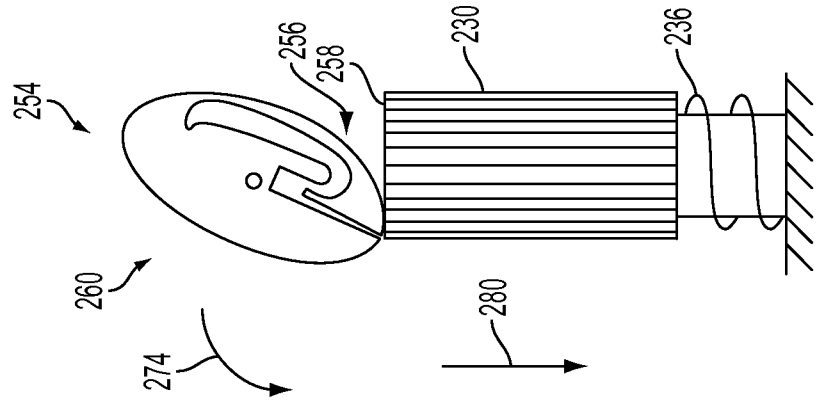


FIG. 14

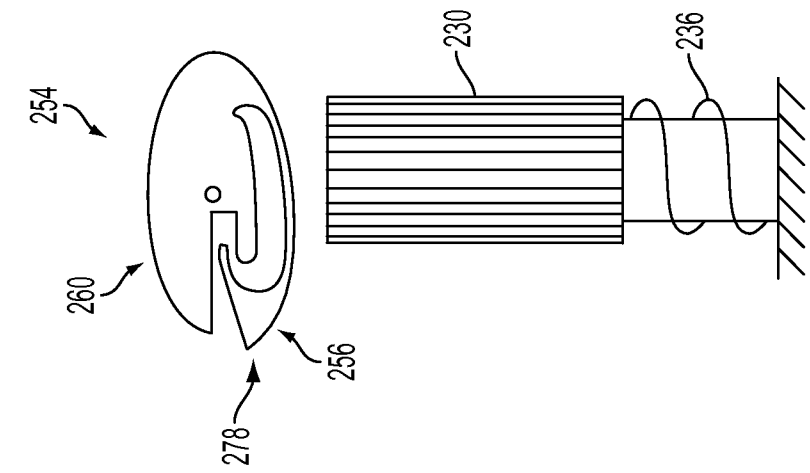


FIG. 15

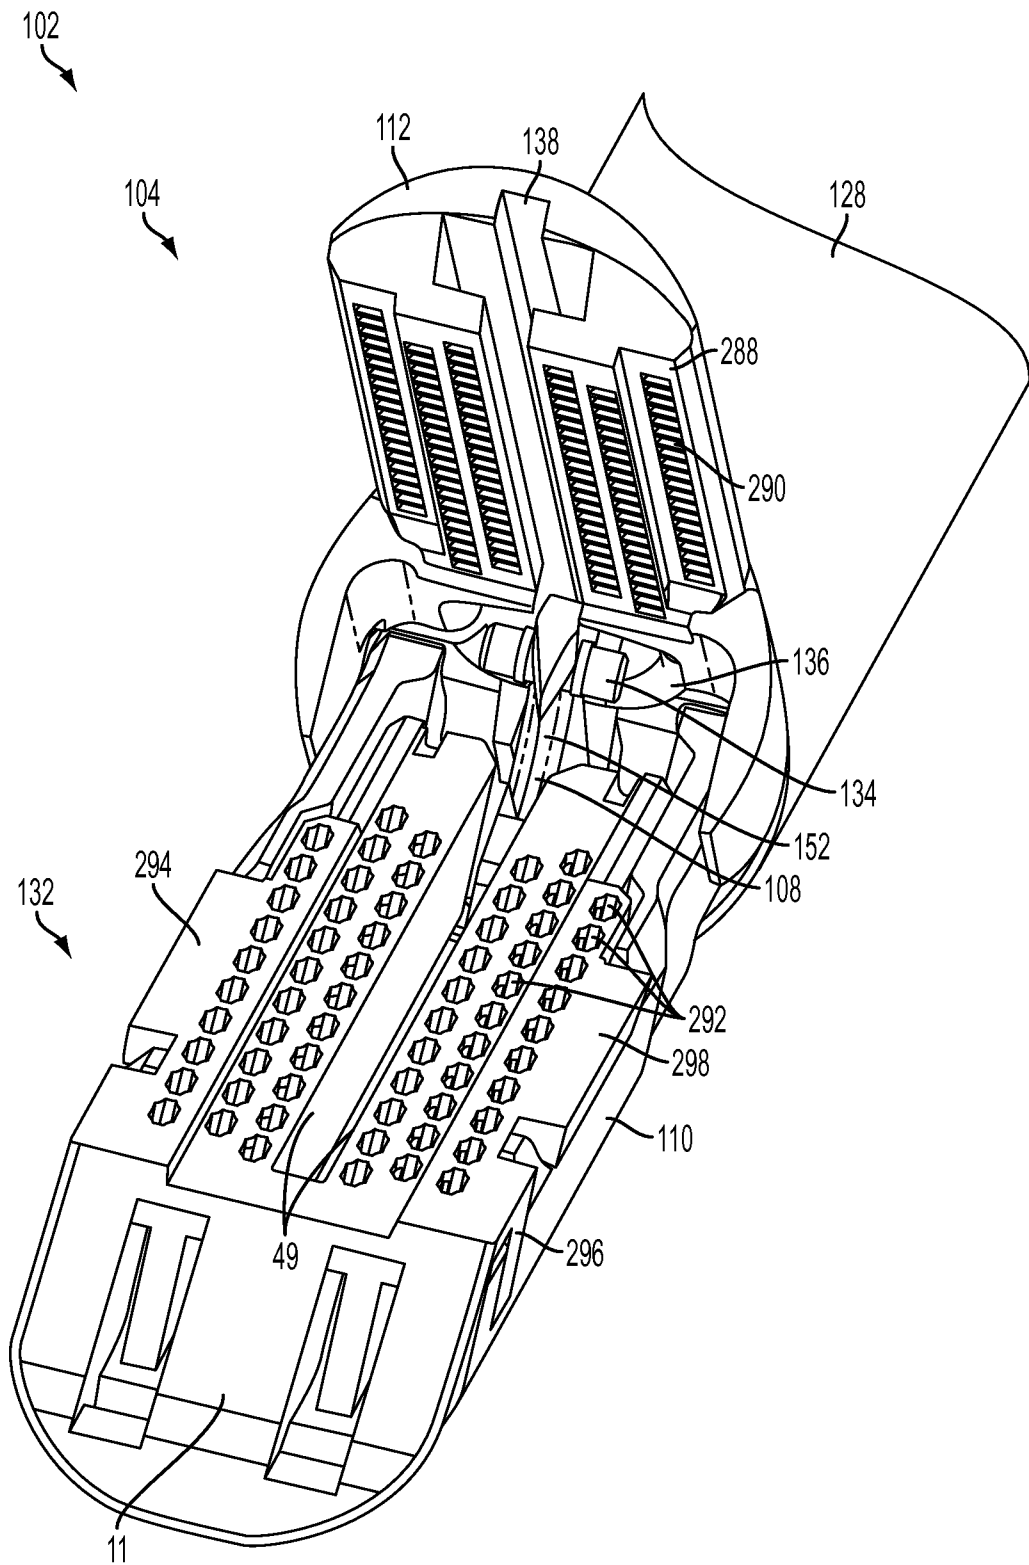


FIG. 16

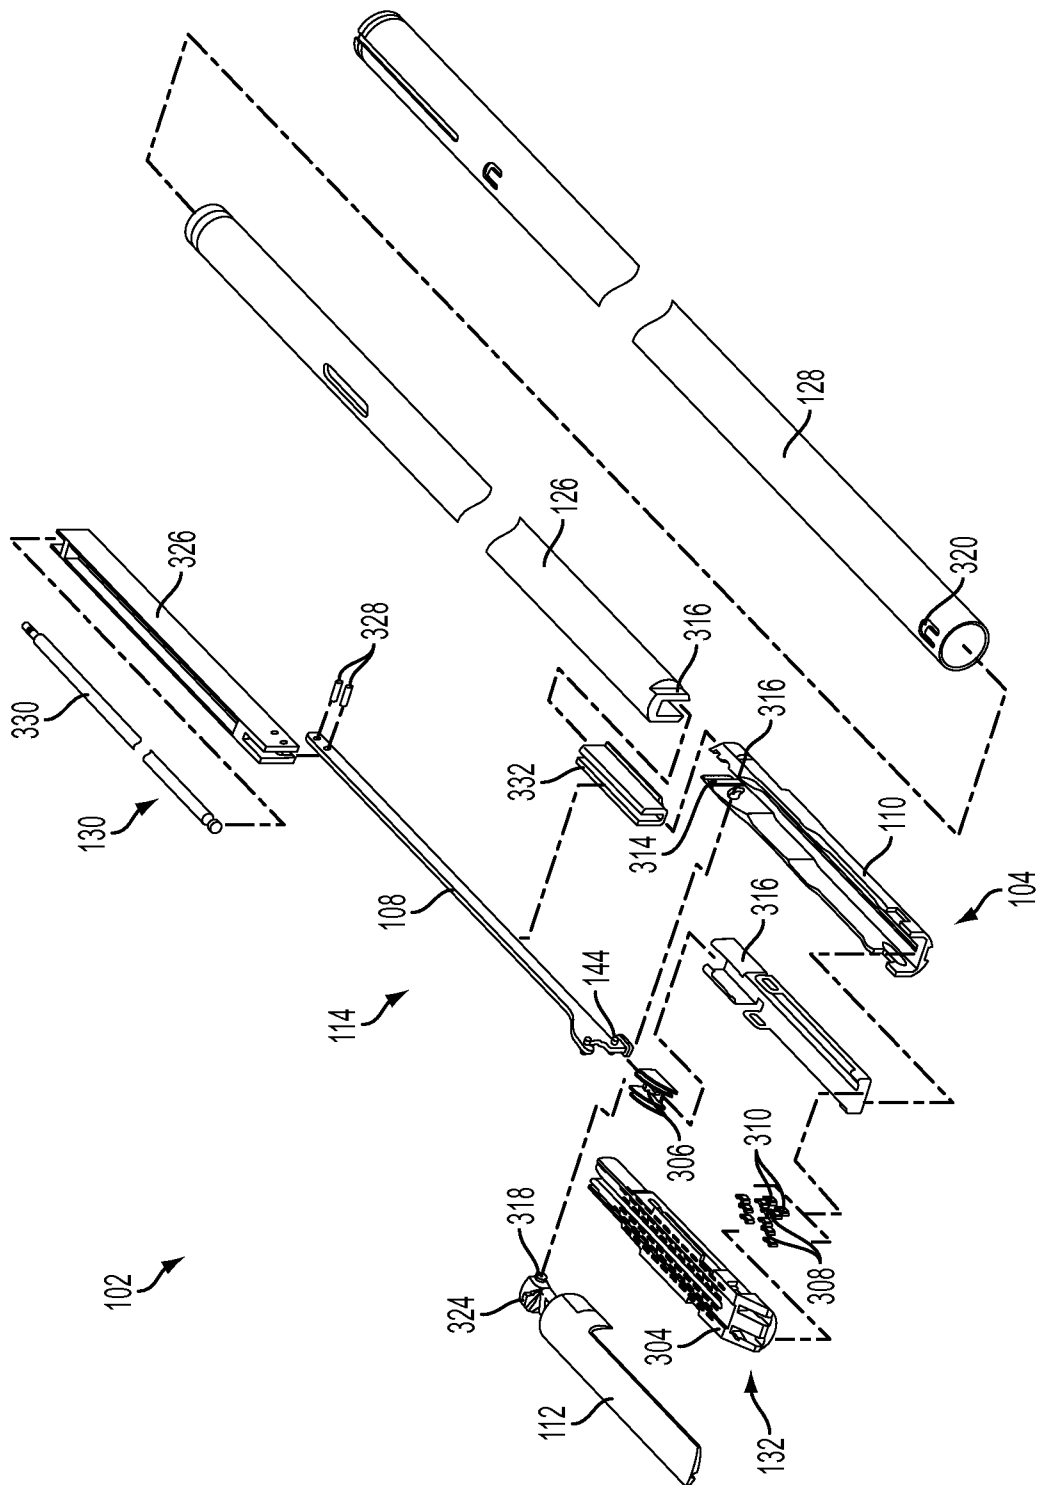


FIG. 17

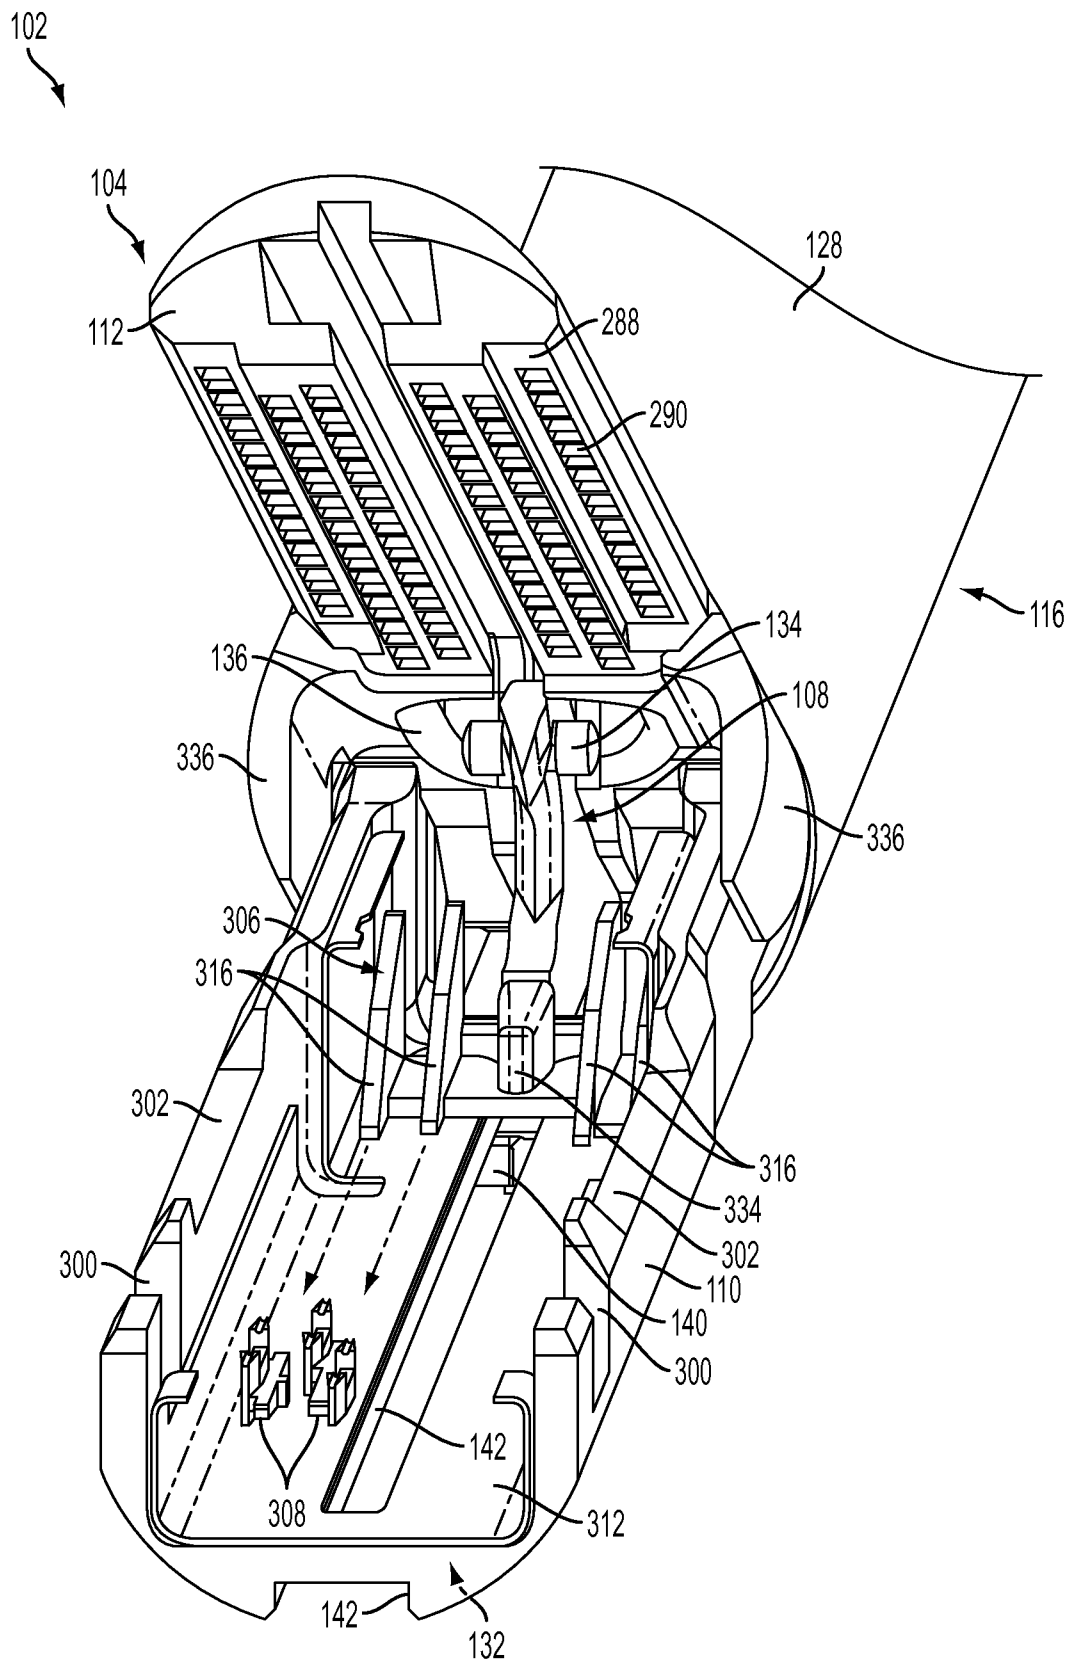


FIG. 18

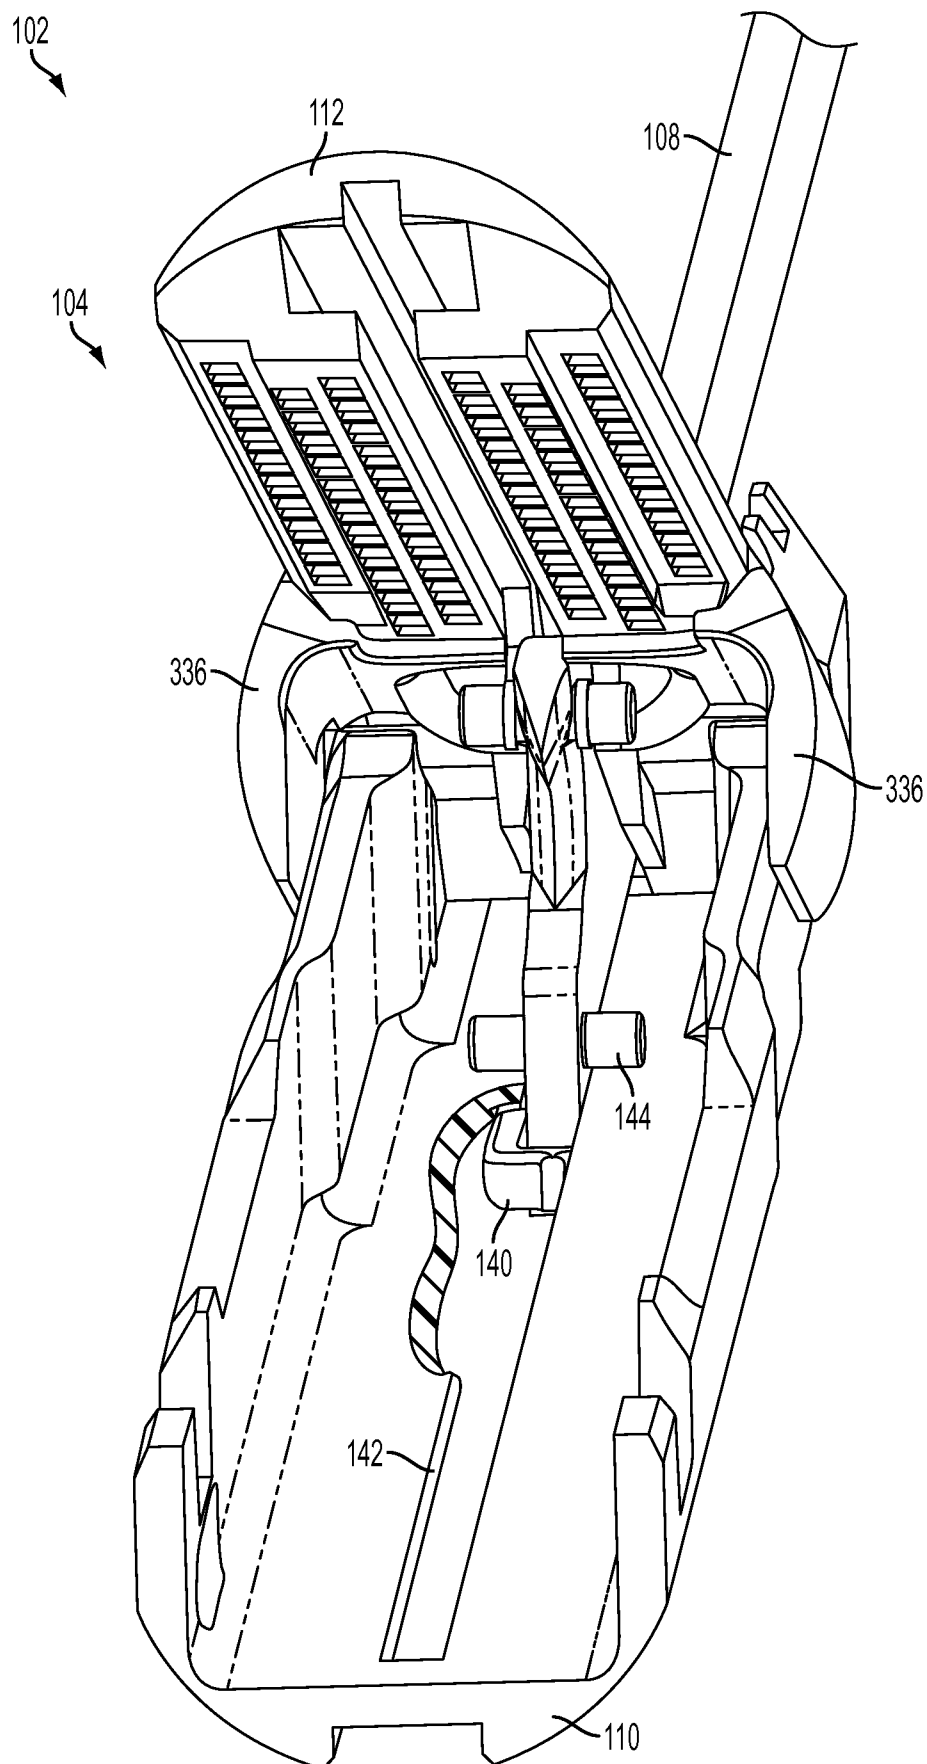


FIG. 19

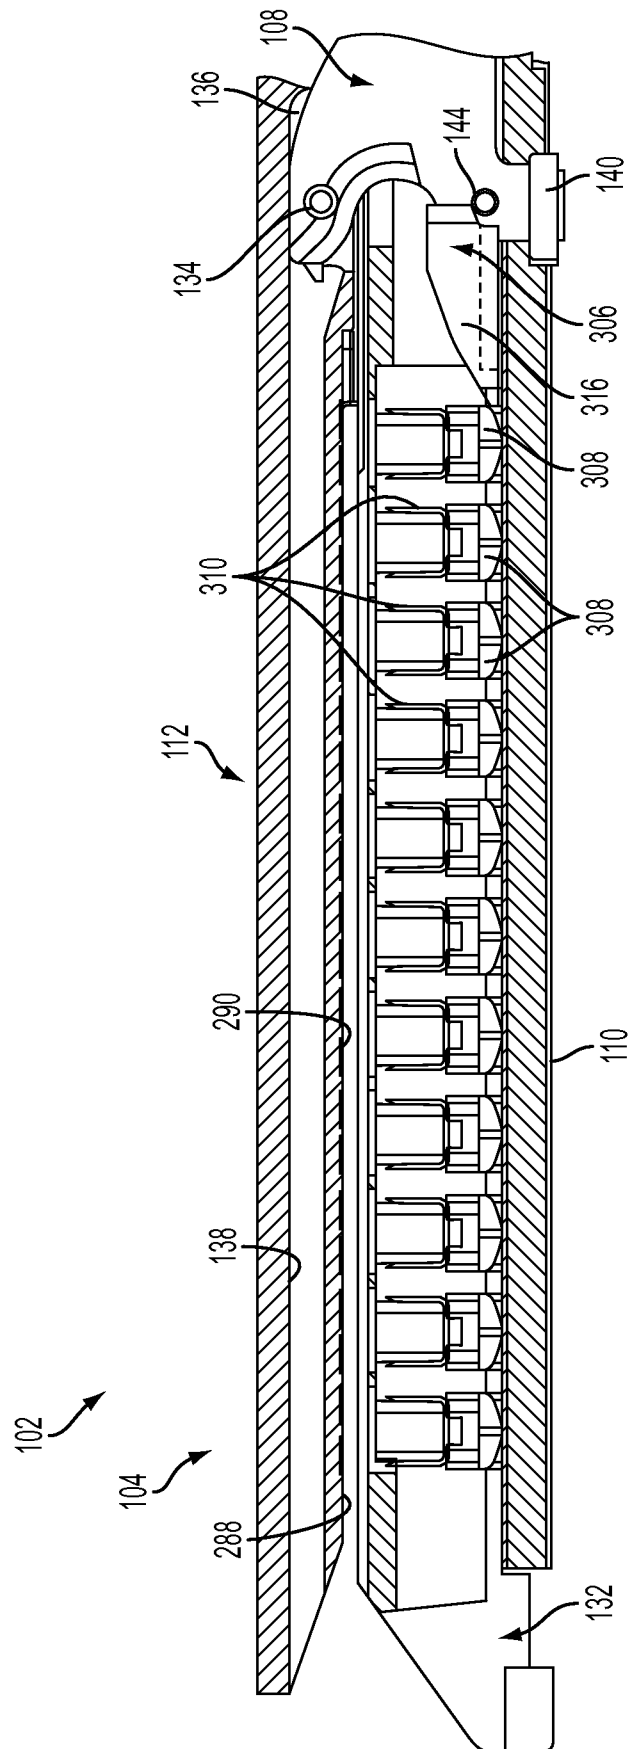


FIG. 20

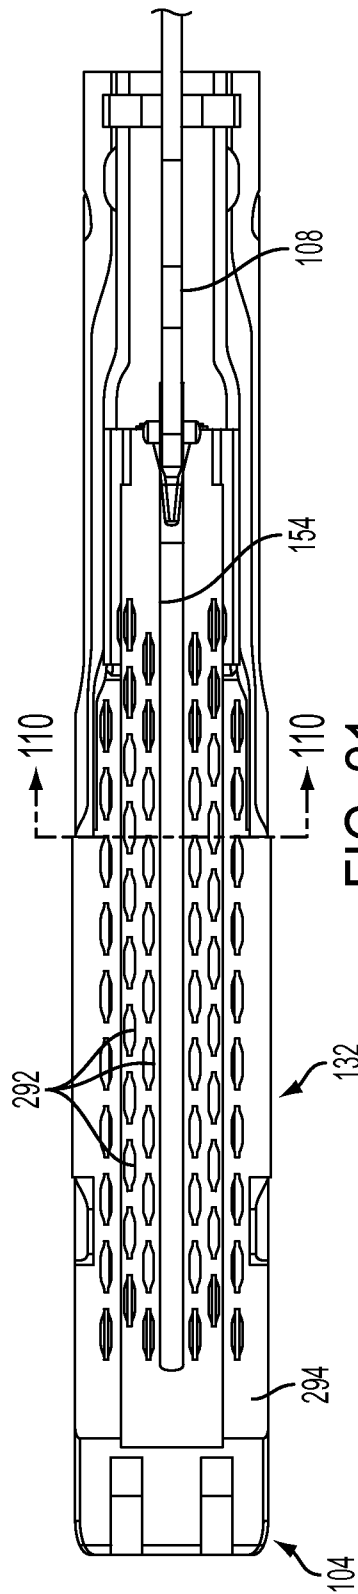


FIG. 21

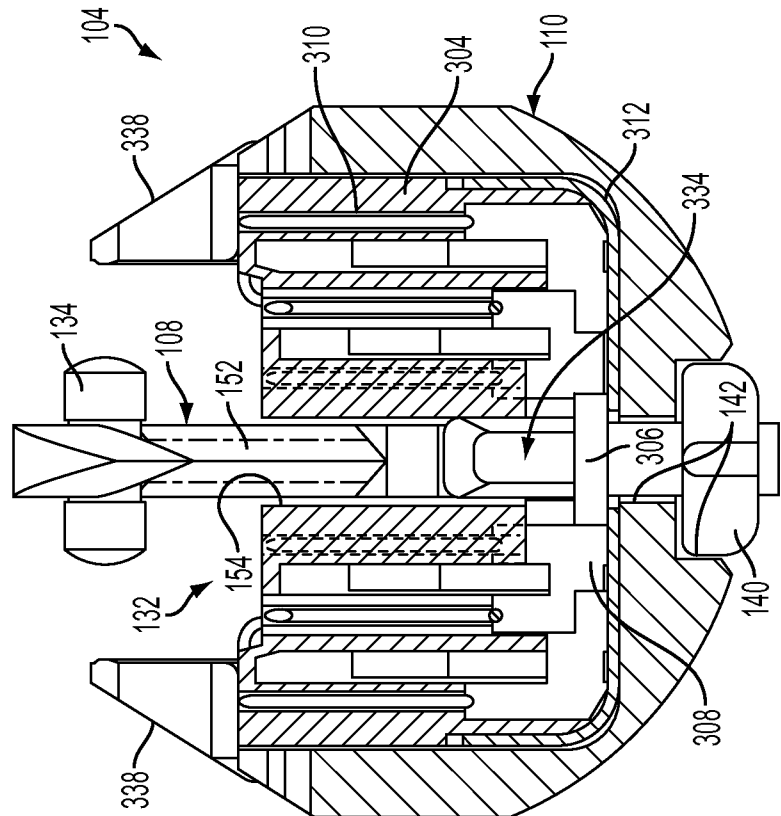


FIG. 22

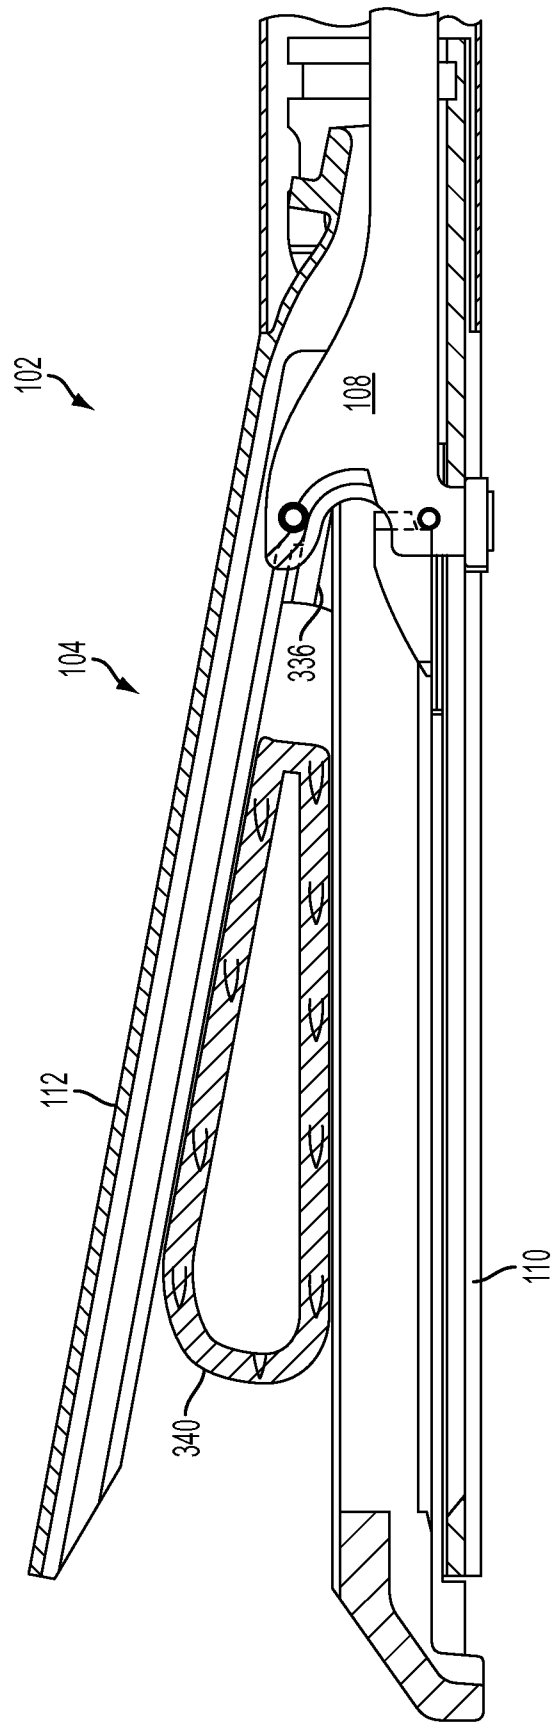


FIG. 23

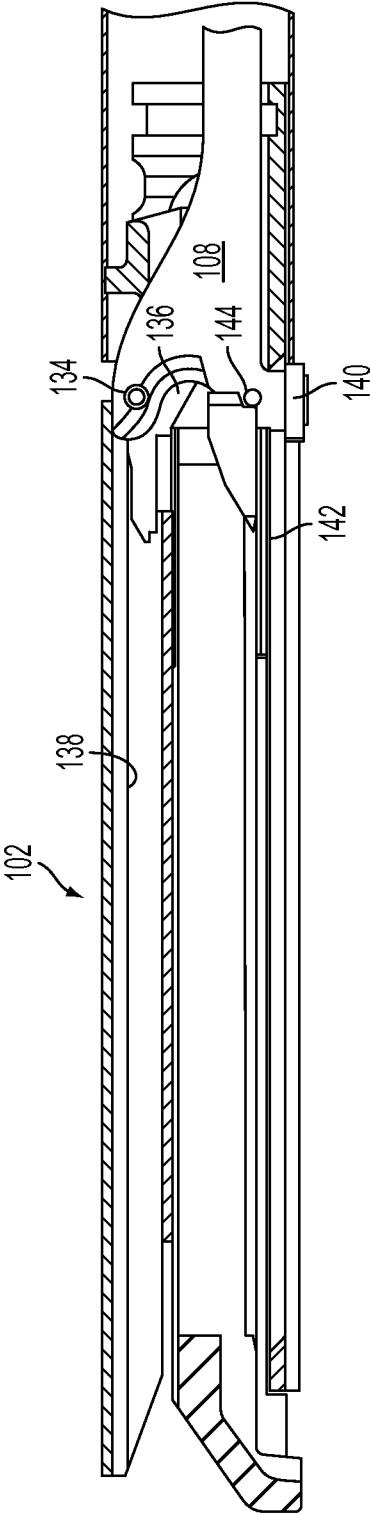


FIG. 24

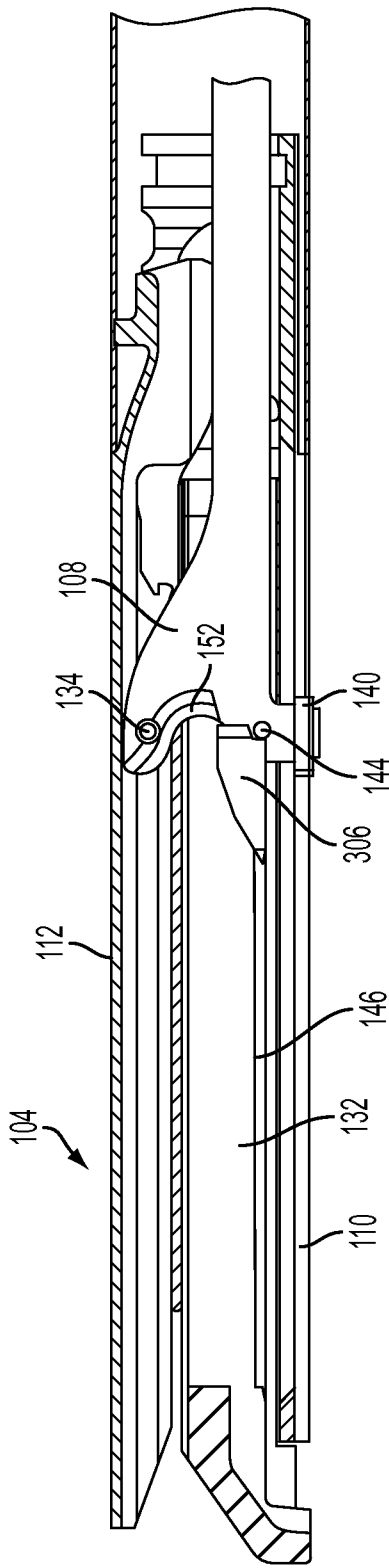


FIG. 25

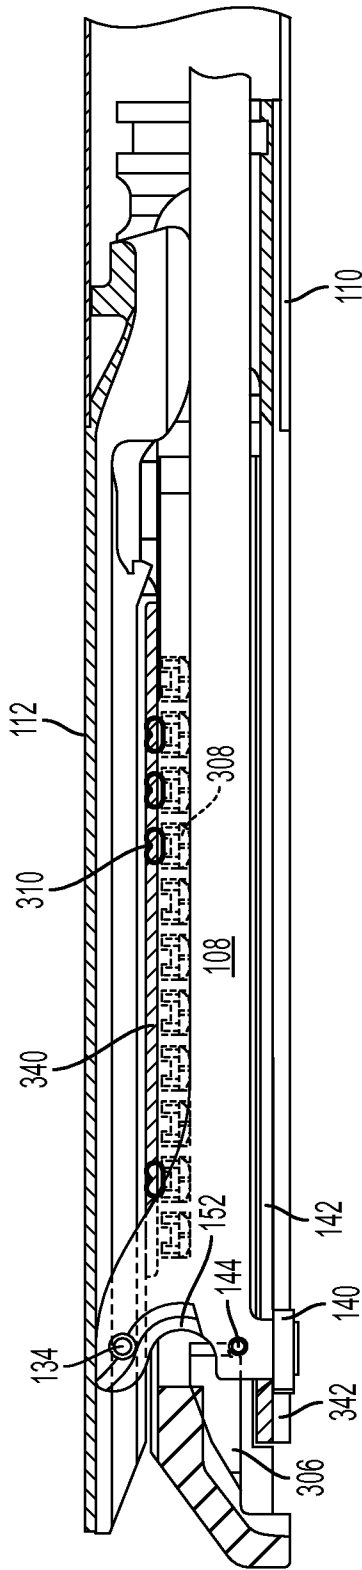


FIG. 26

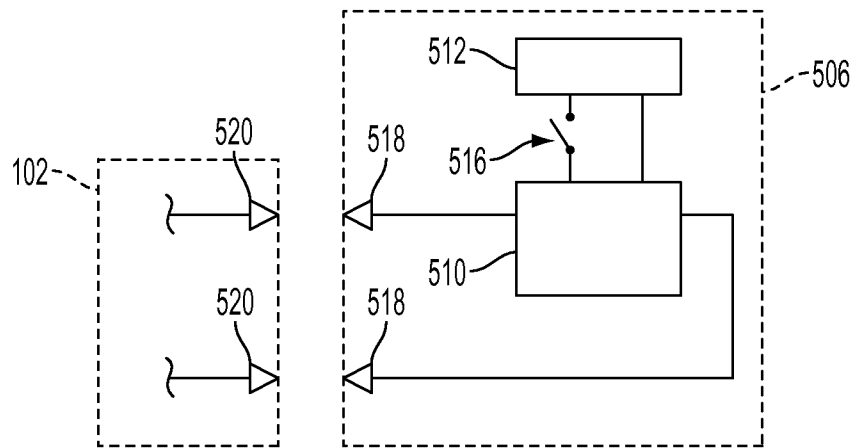


FIG. 27

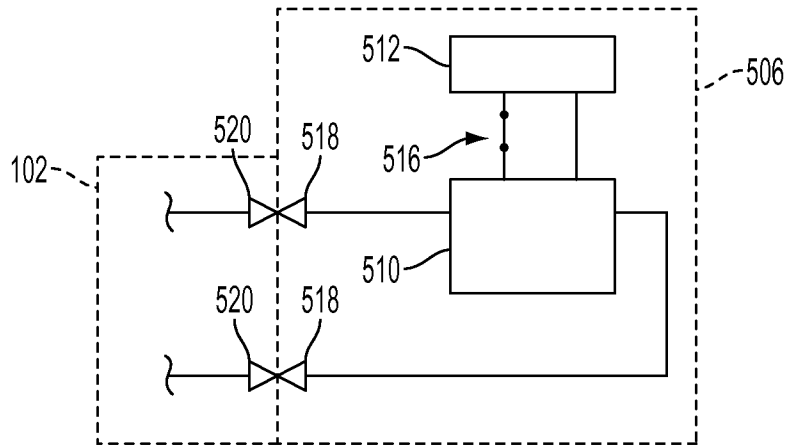


FIG. 28

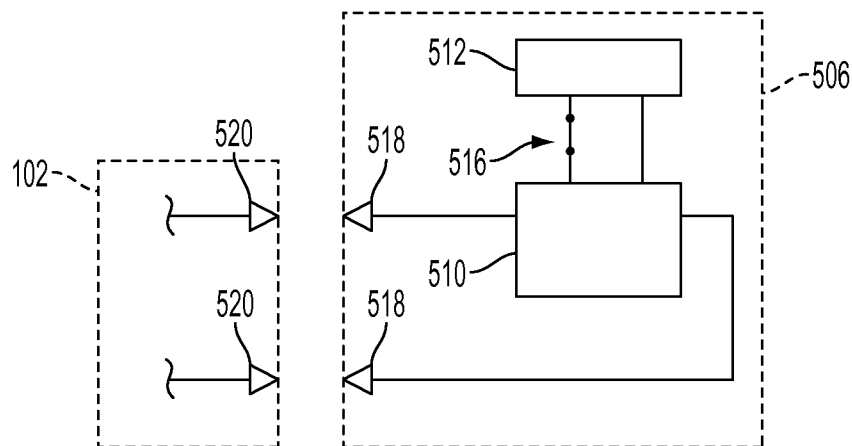


FIG. 29

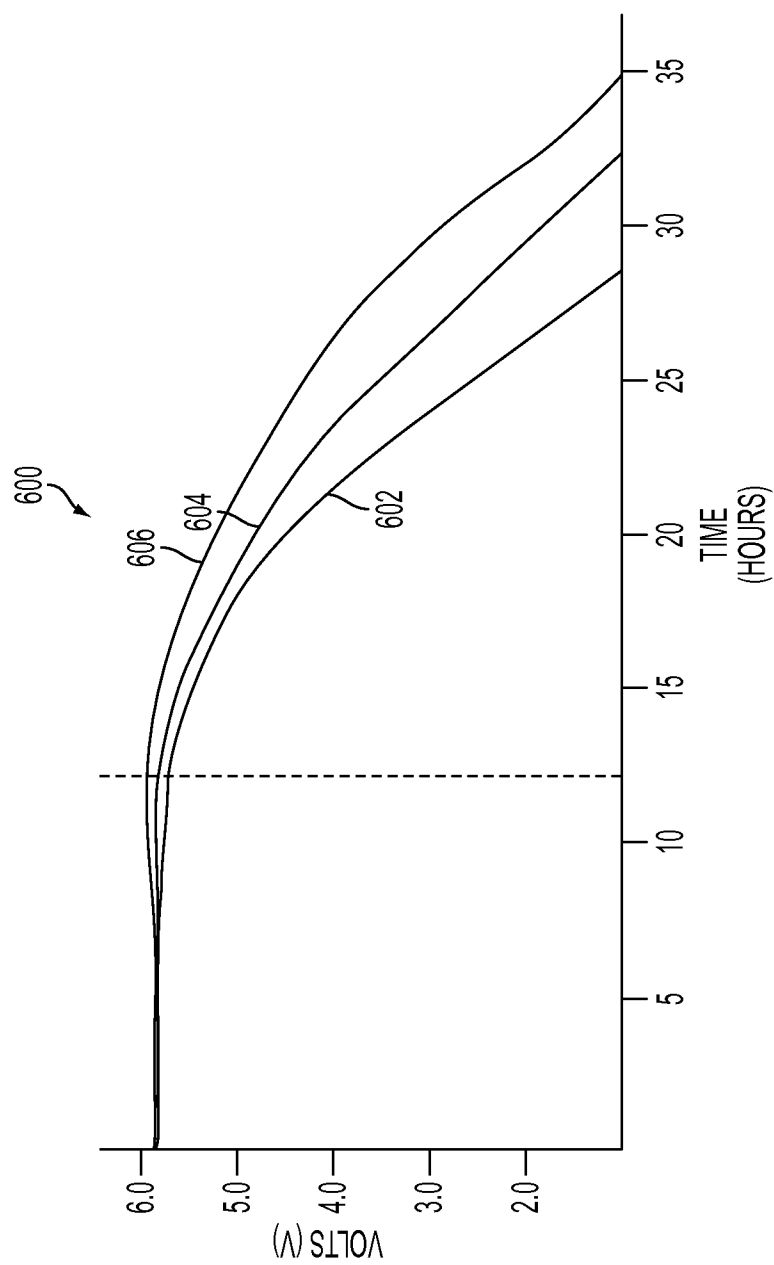


FIG. 30

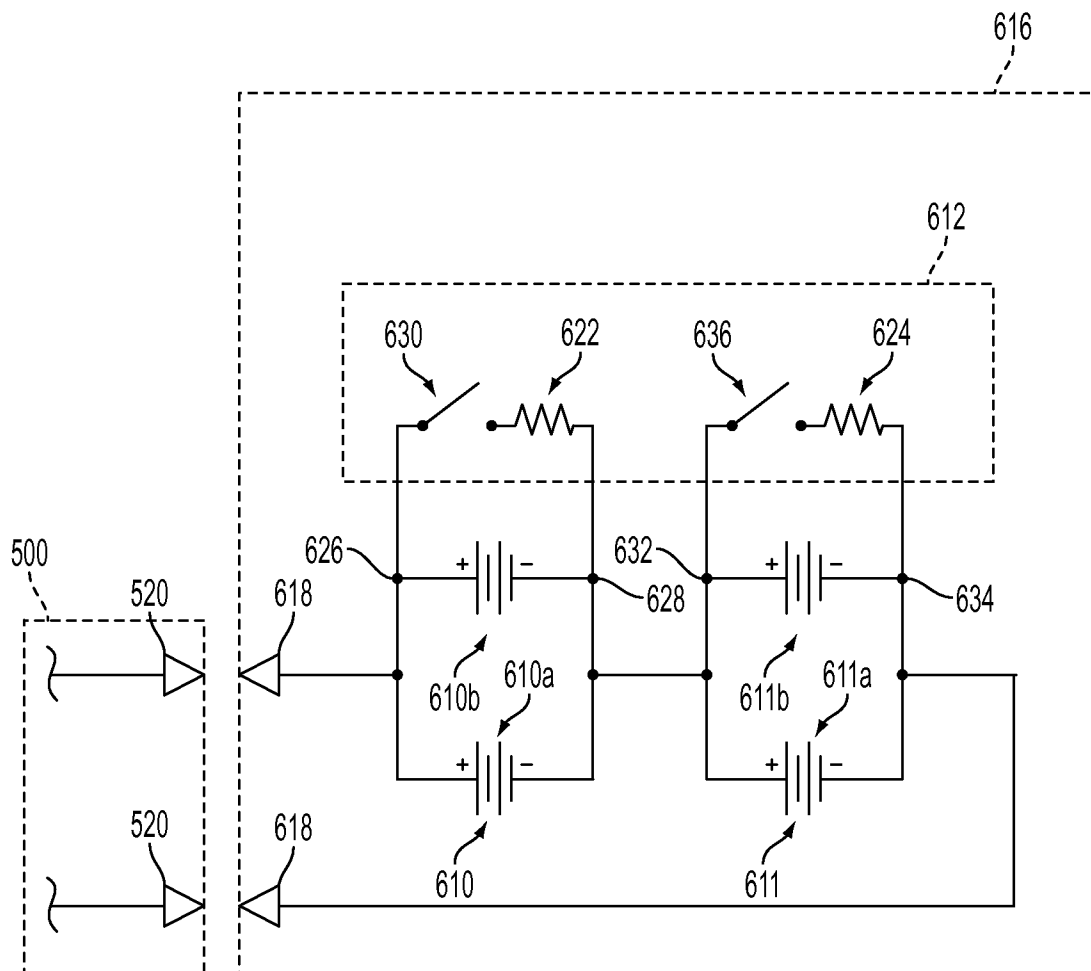


FIG. 31

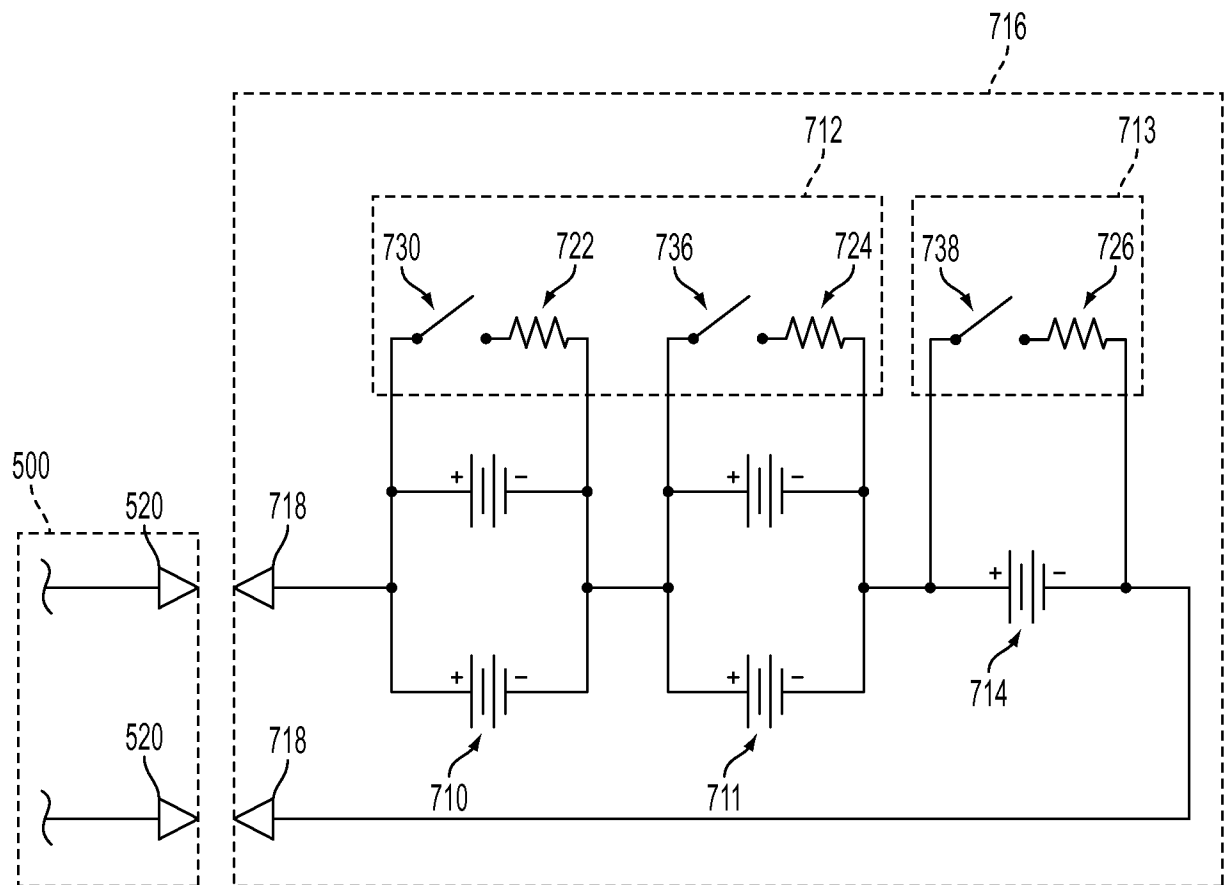


FIG. 32

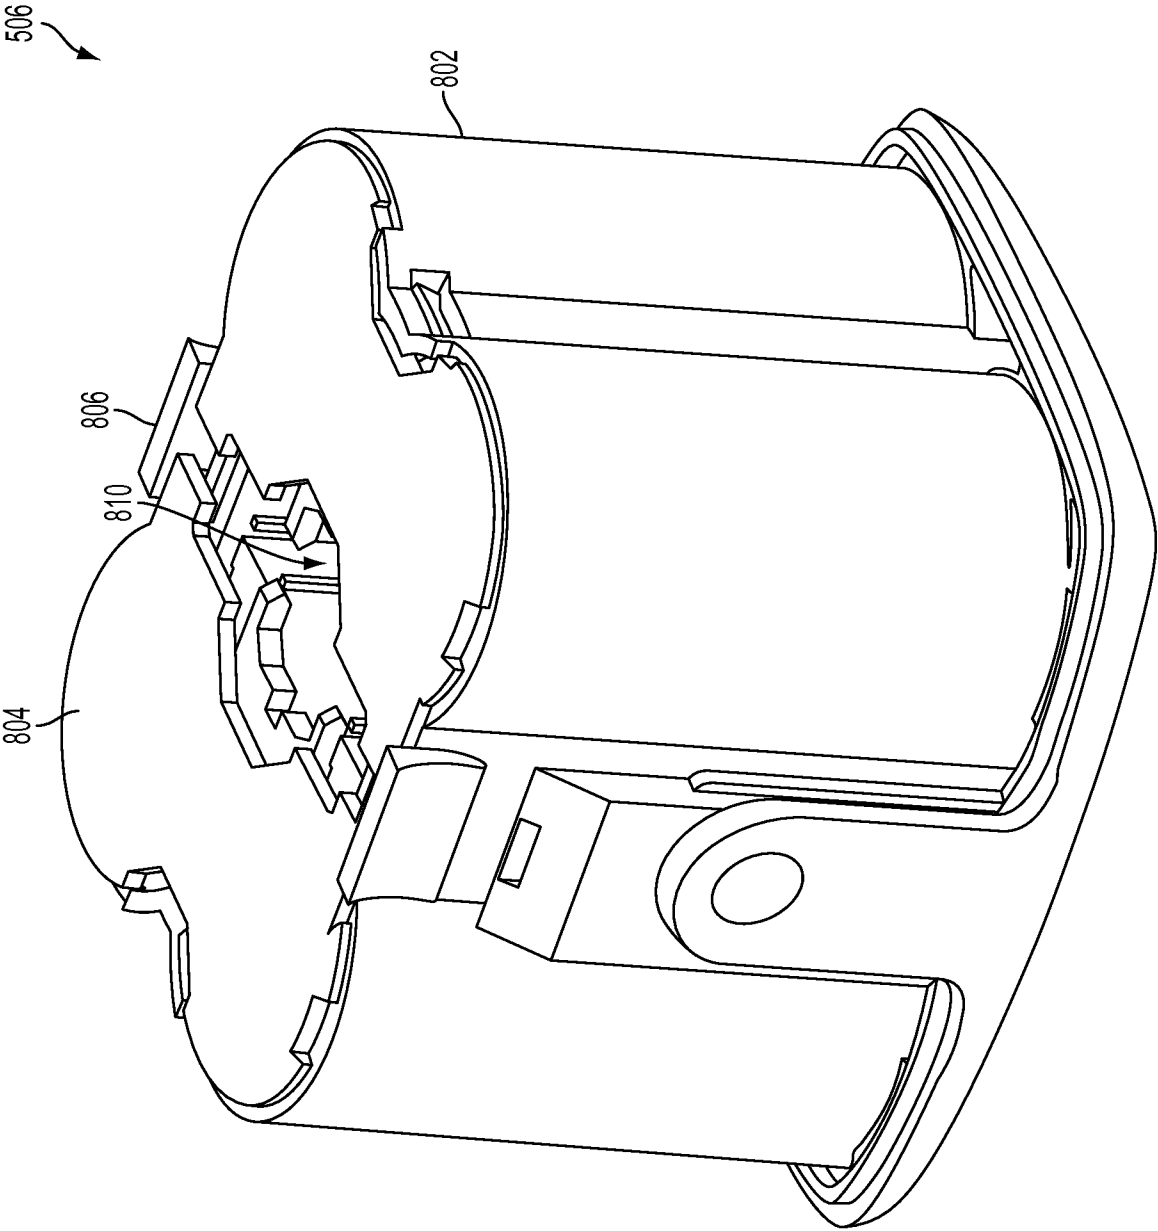


FIG. 33

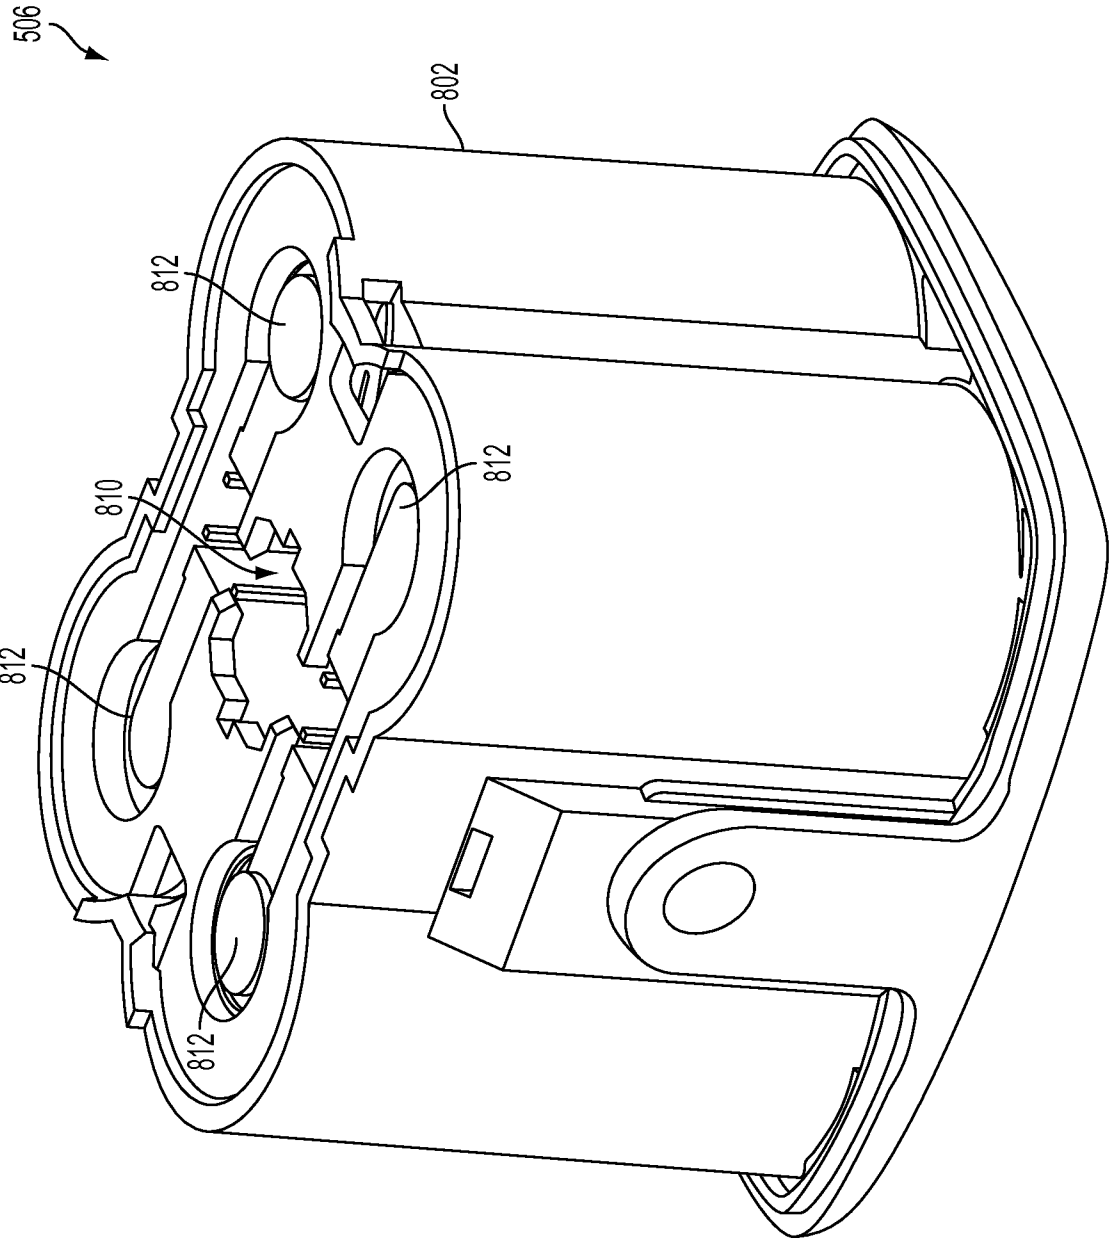


FIG. 34

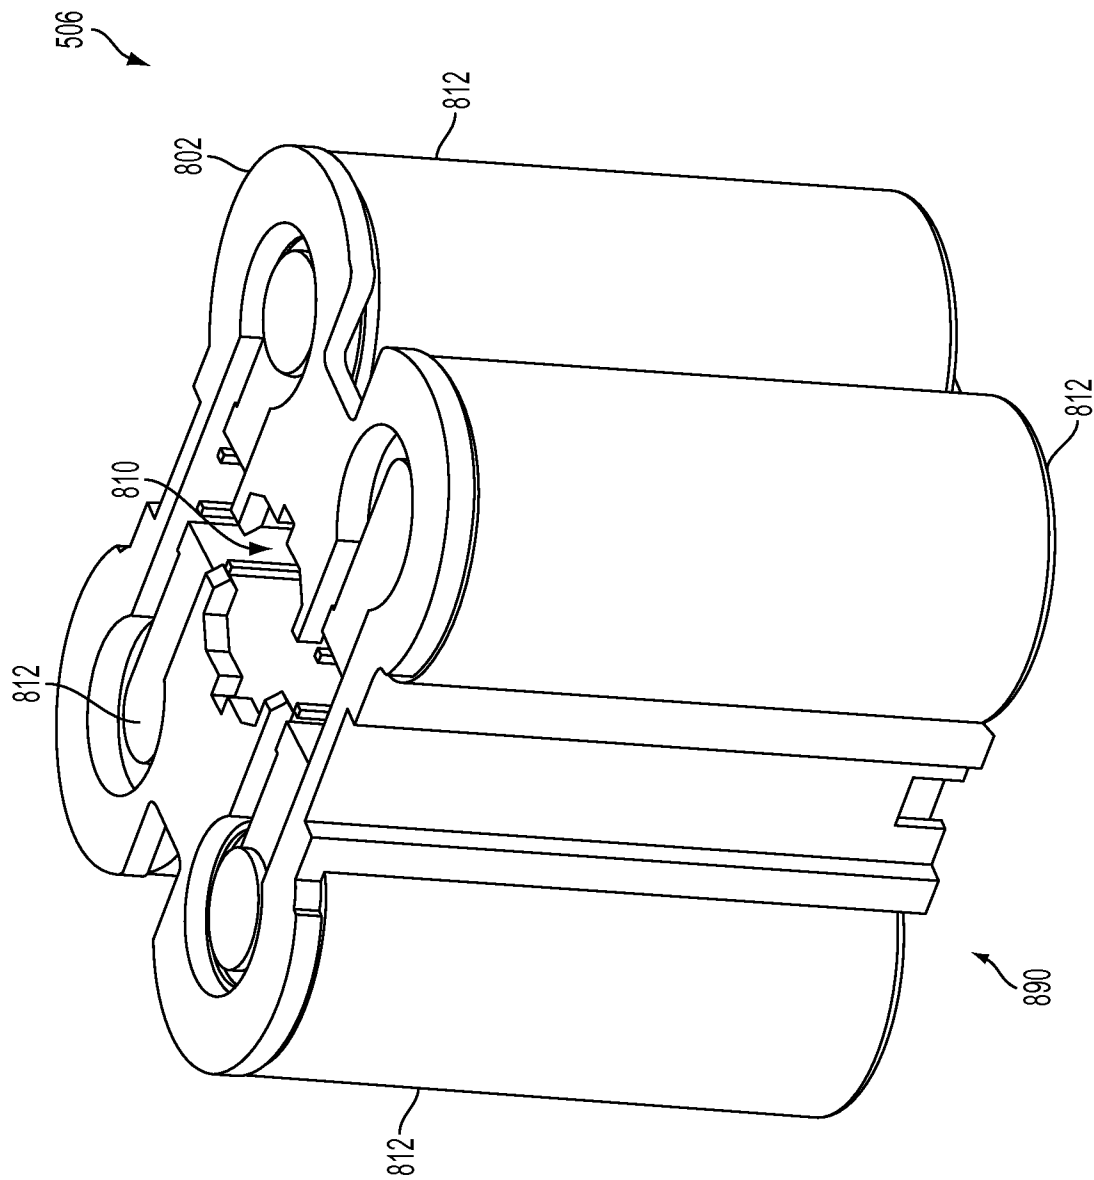


FIG. 35

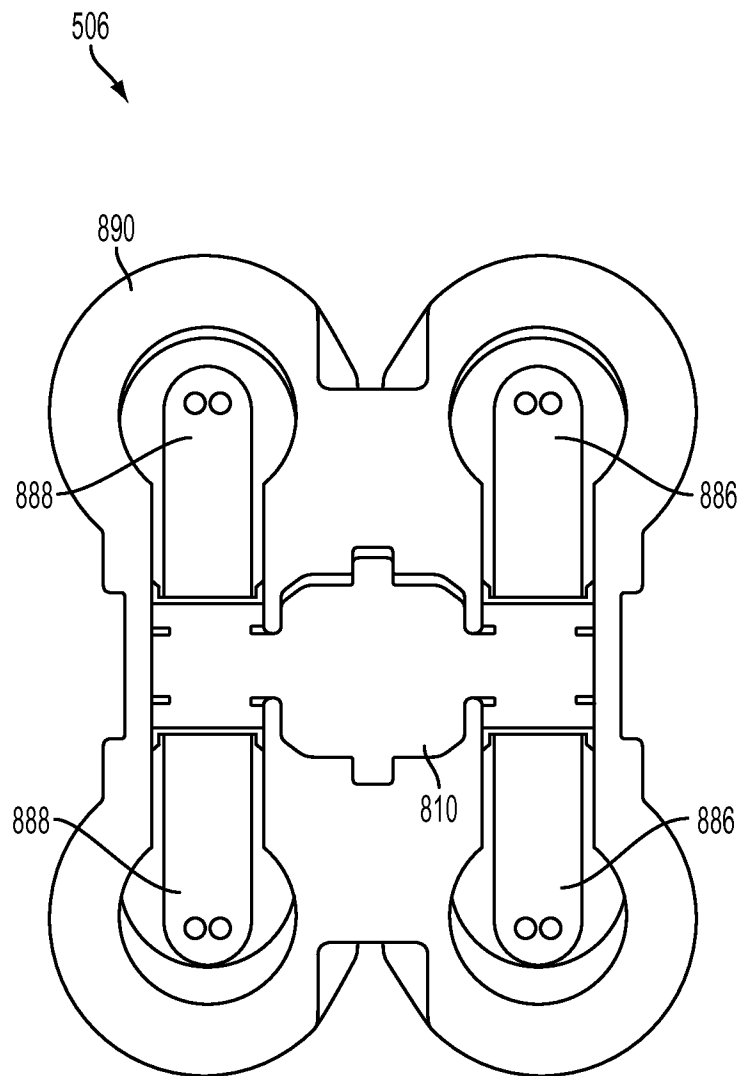


FIG. 36

30/43

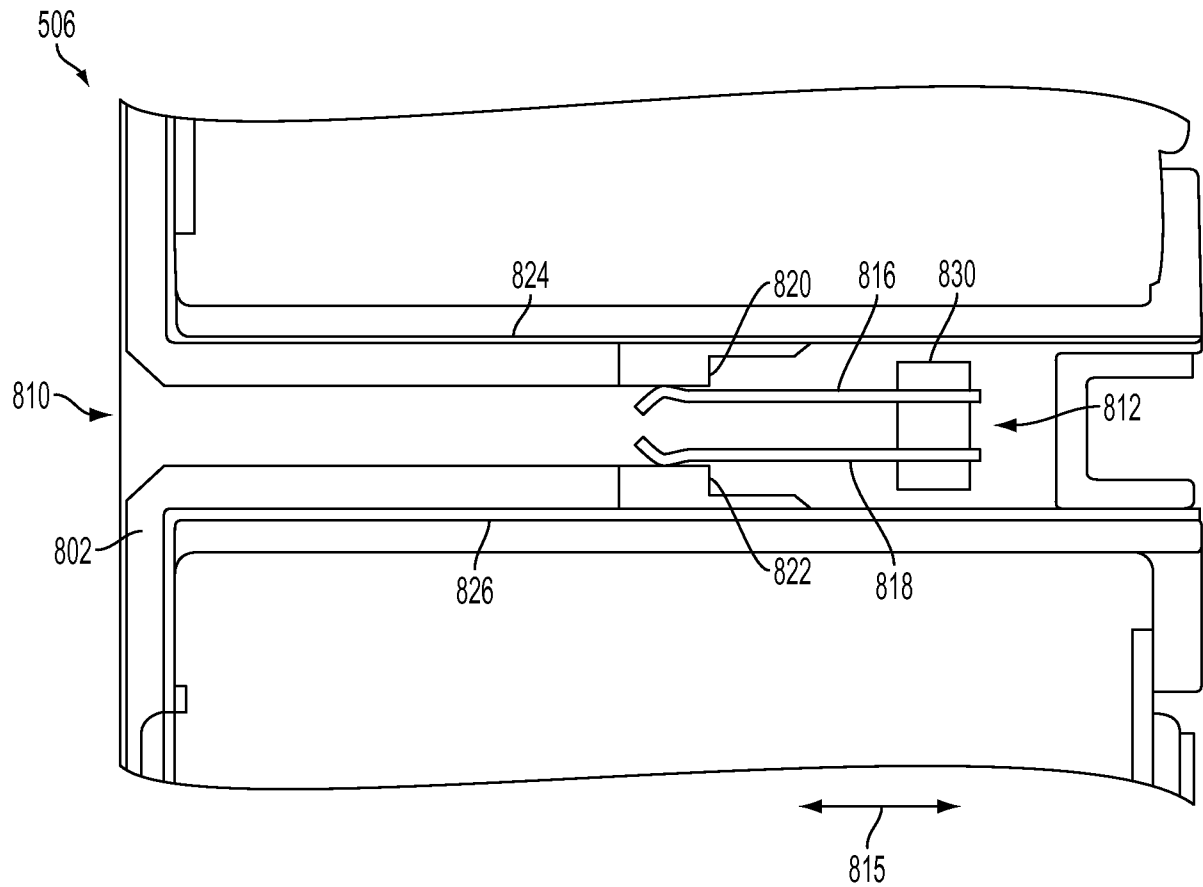


FIG. 37

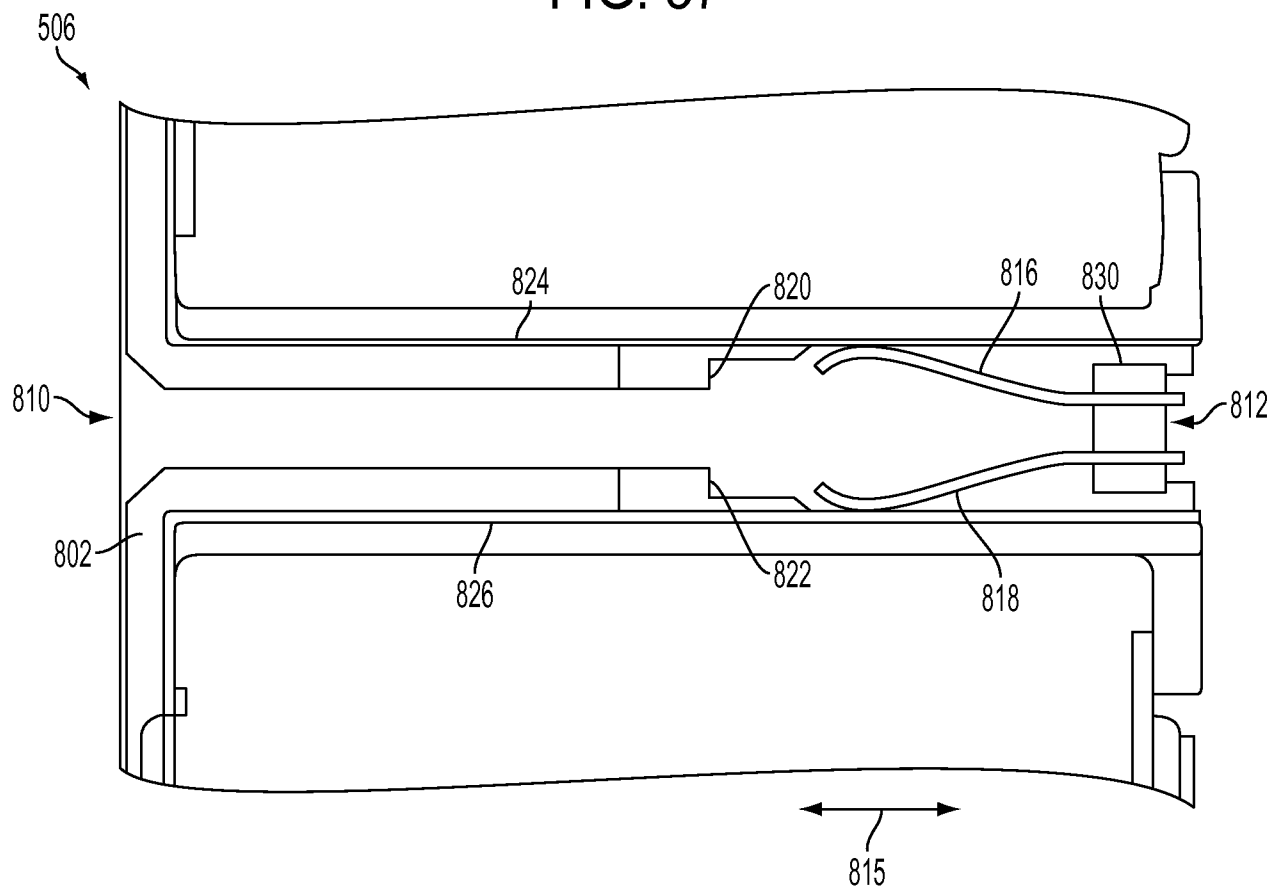


FIG. 38

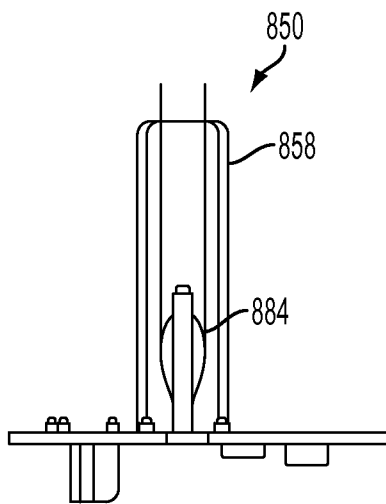


FIG. 39

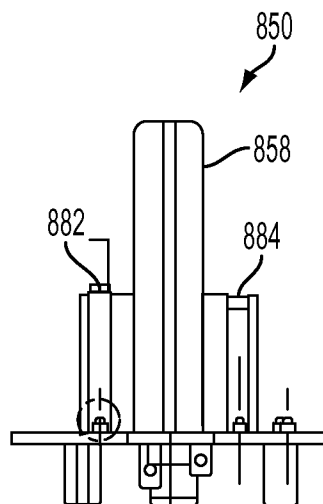


FIG. 40

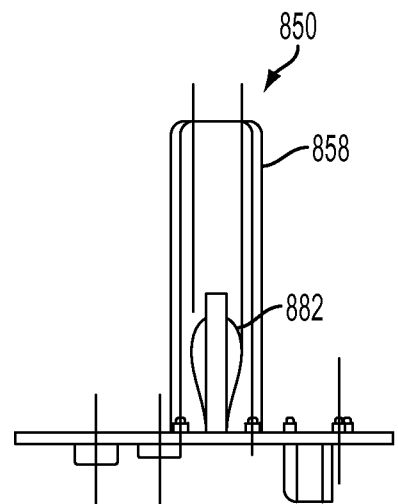


FIG. 41

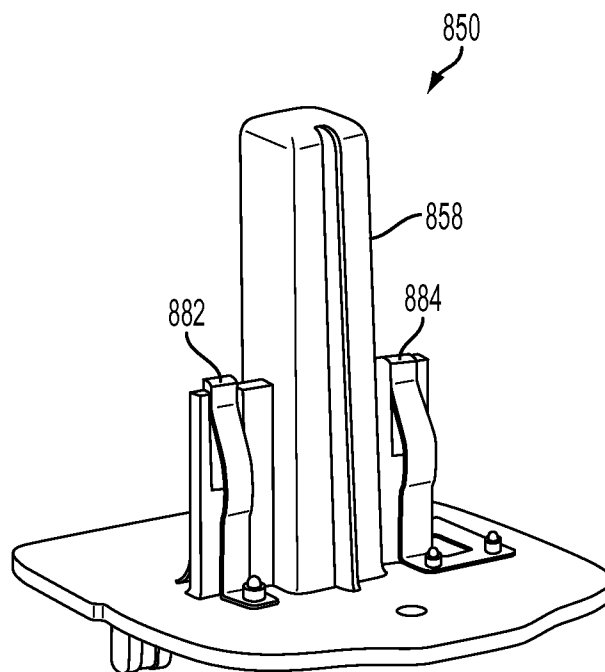


FIG. 42

32/43

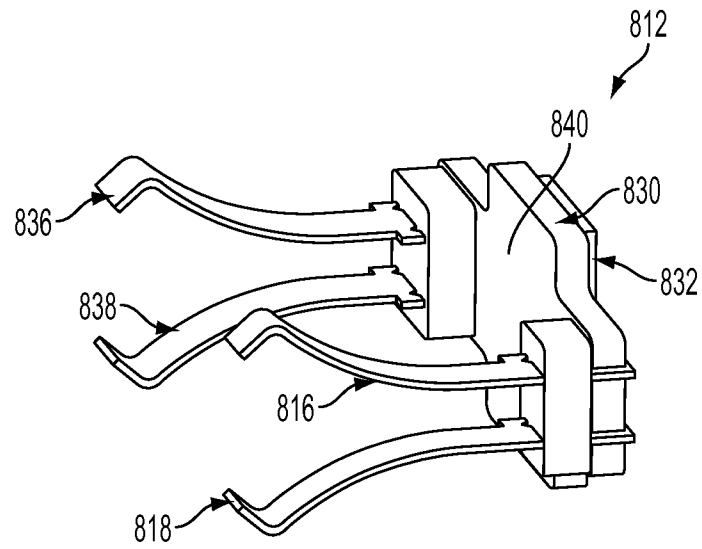


FIG. 43

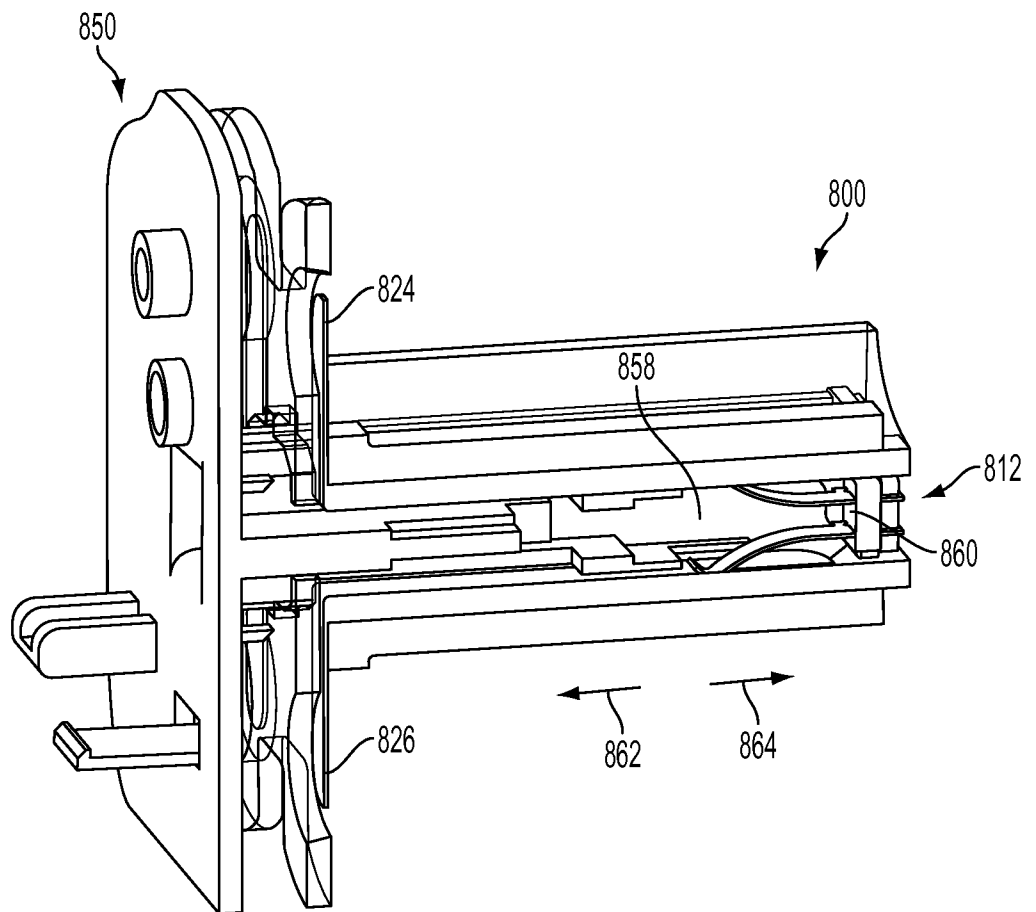


FIG. 44

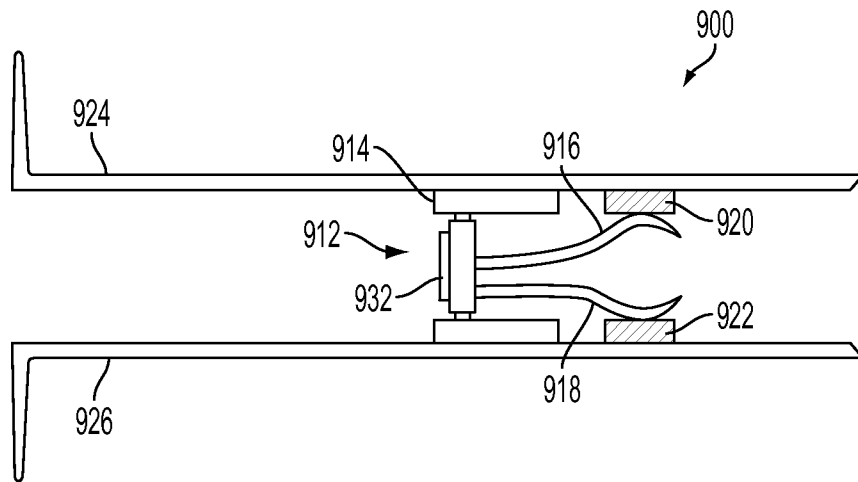


FIG. 45

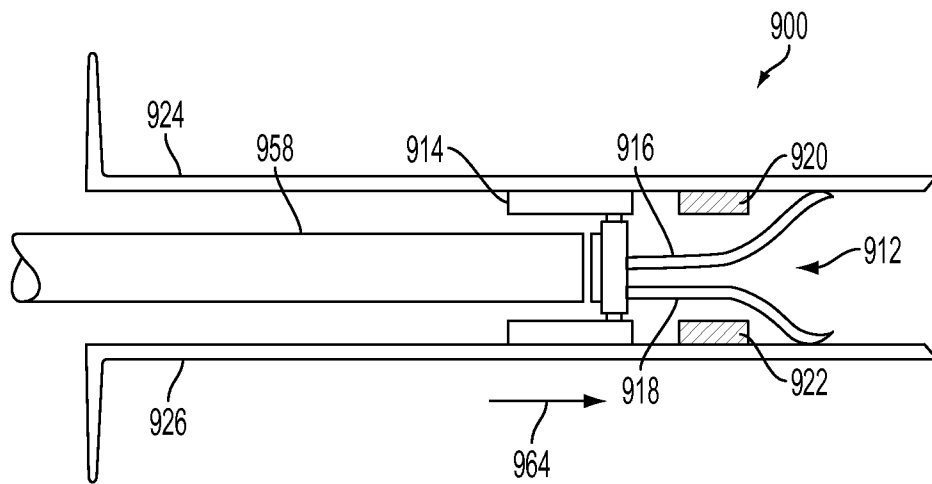


FIG. 46

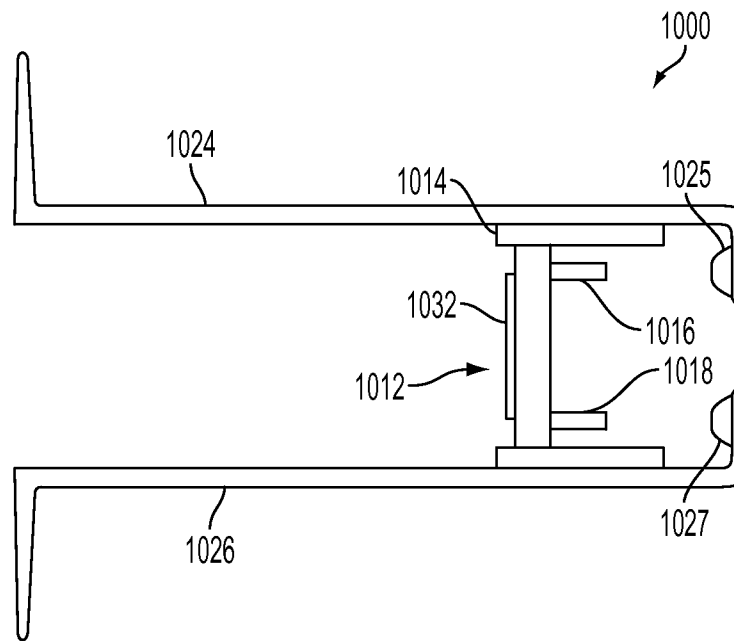


FIG. 47

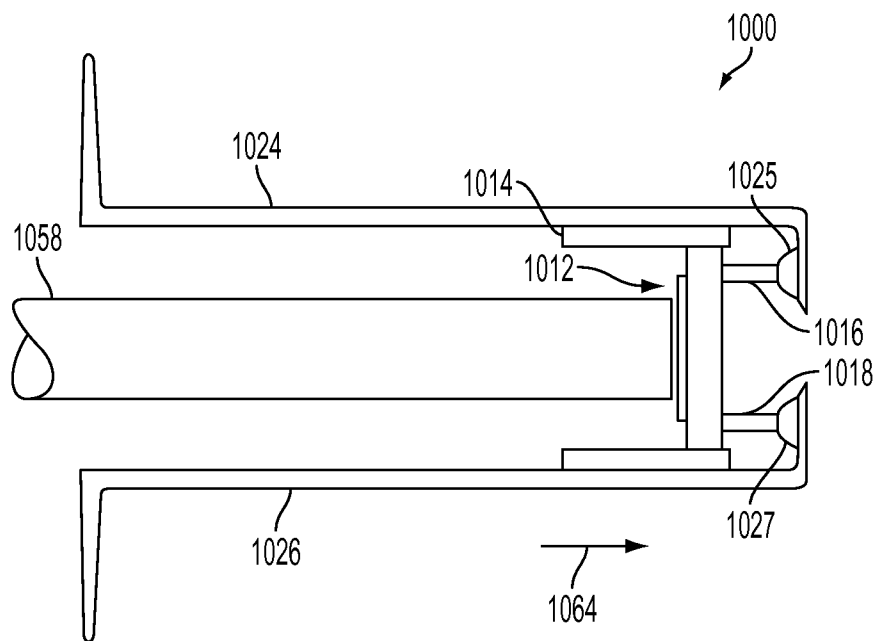


FIG. 48

35/43

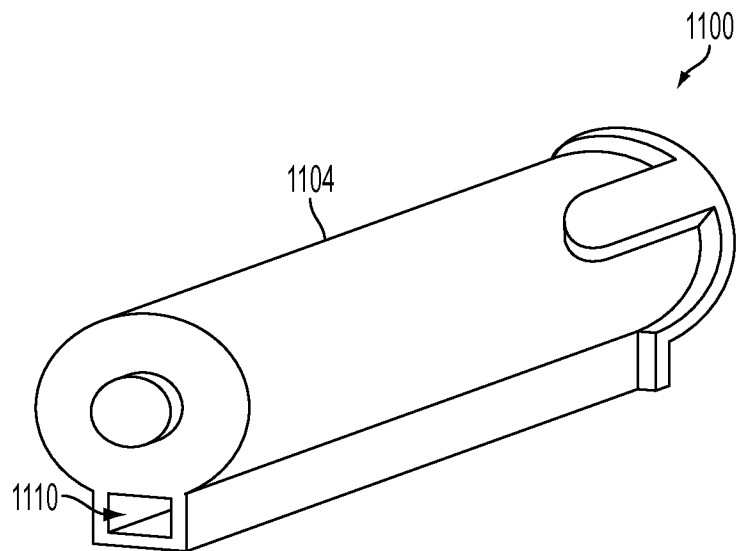


FIG. 49

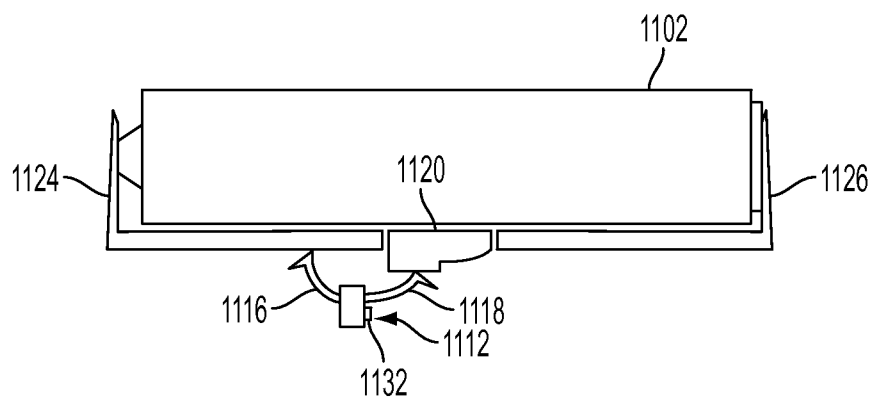


FIG. 50

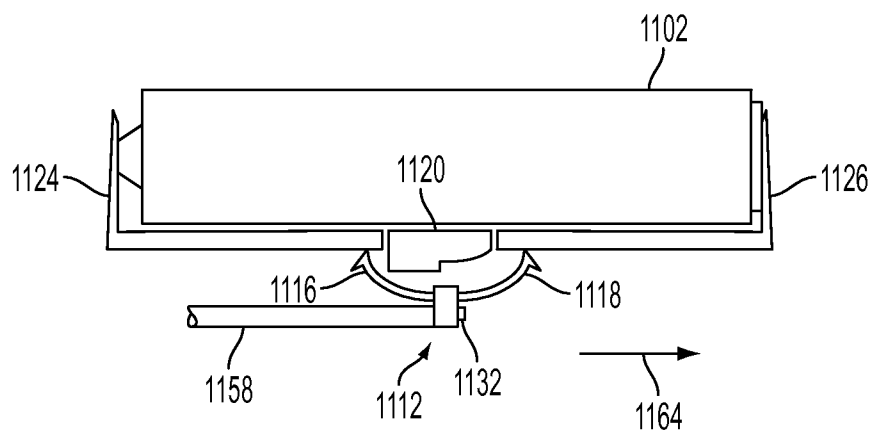


FIG. 51

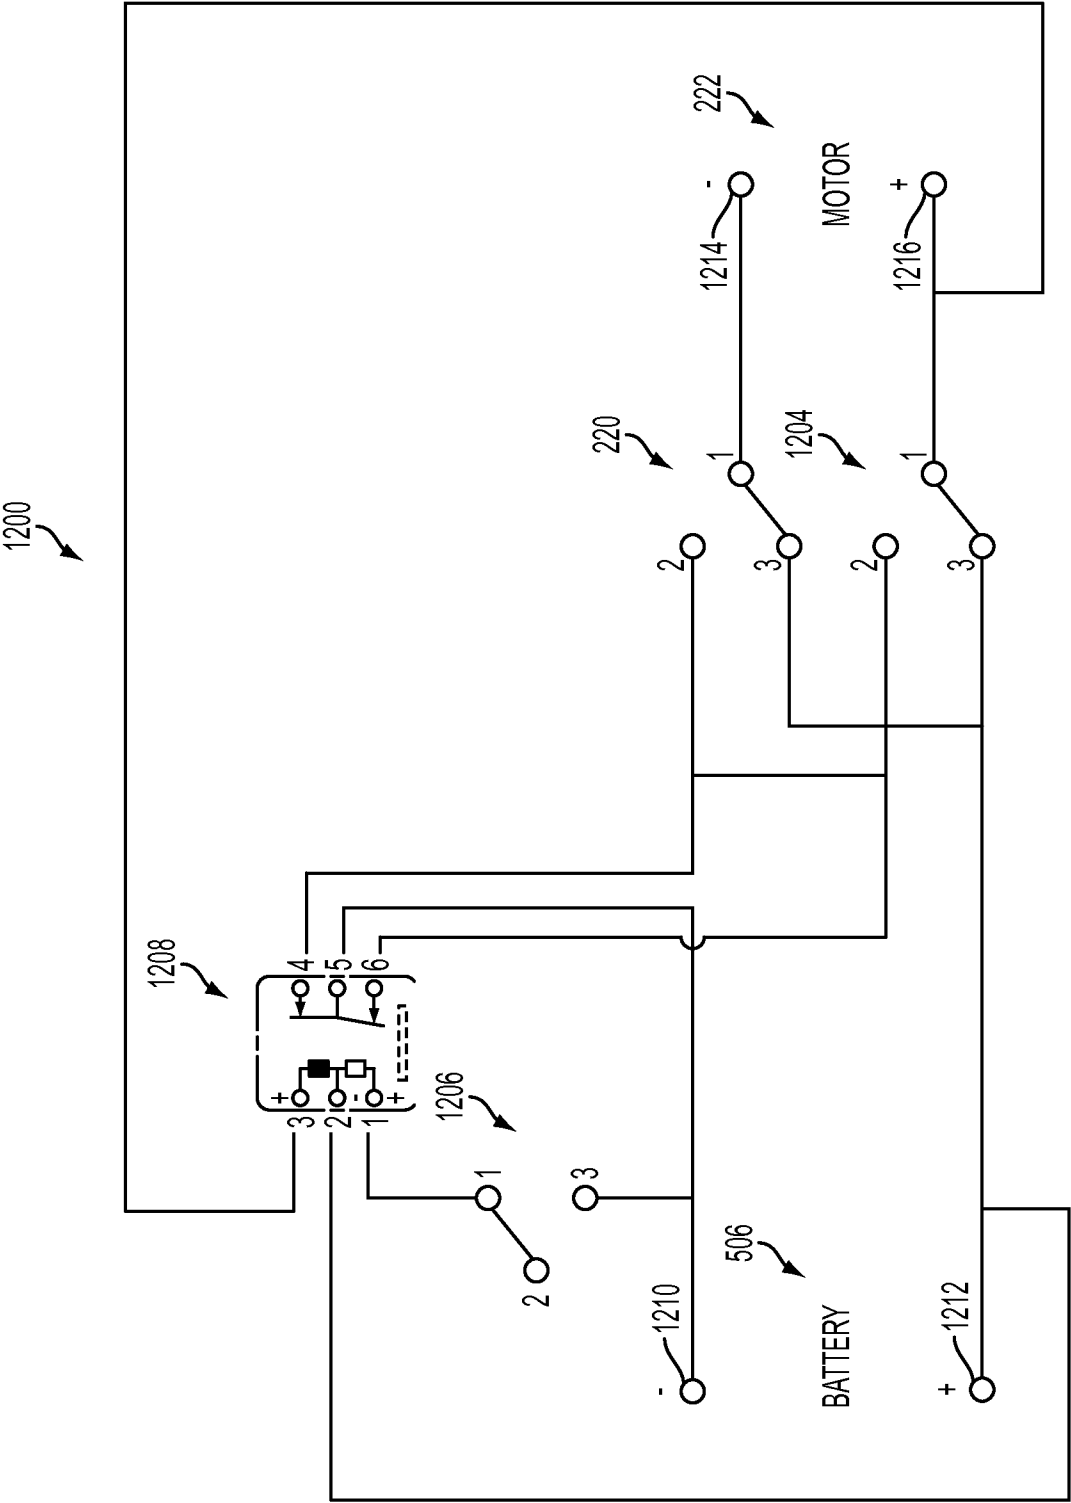


FIG. 52

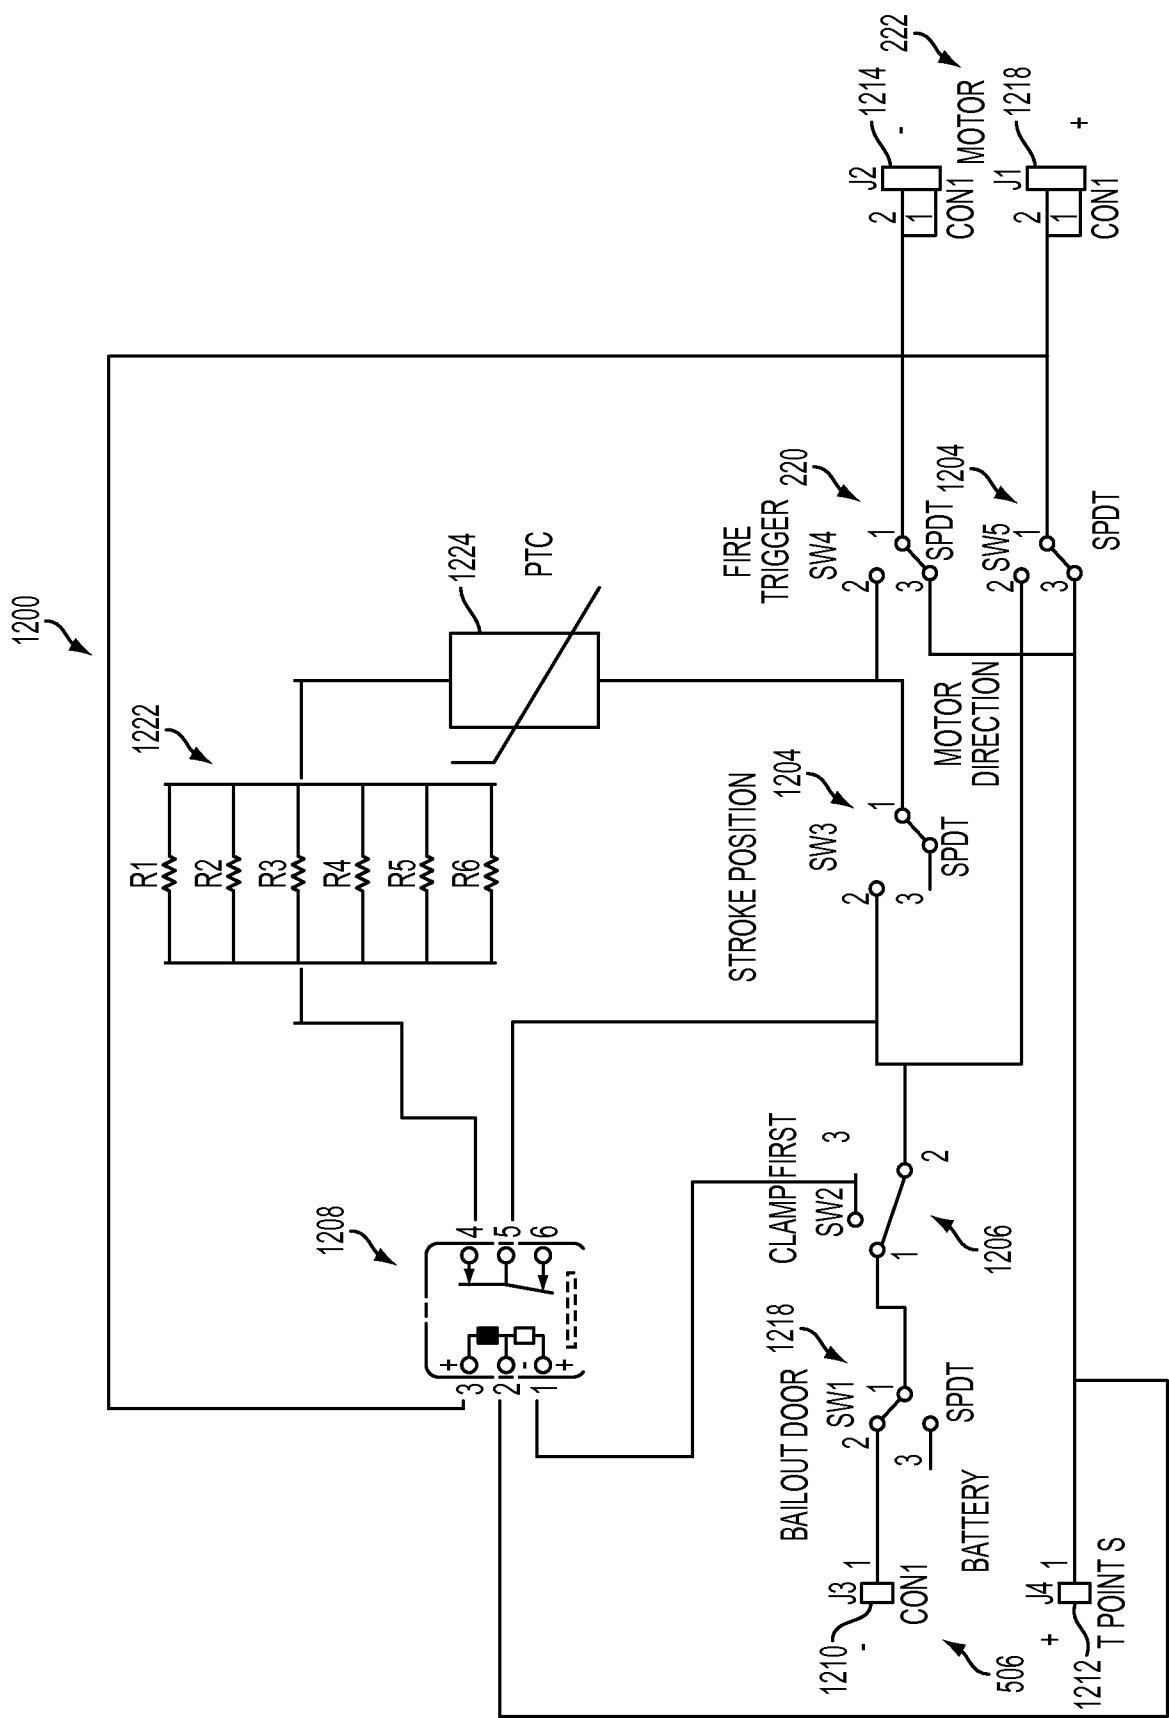


FIG. 53

38/43

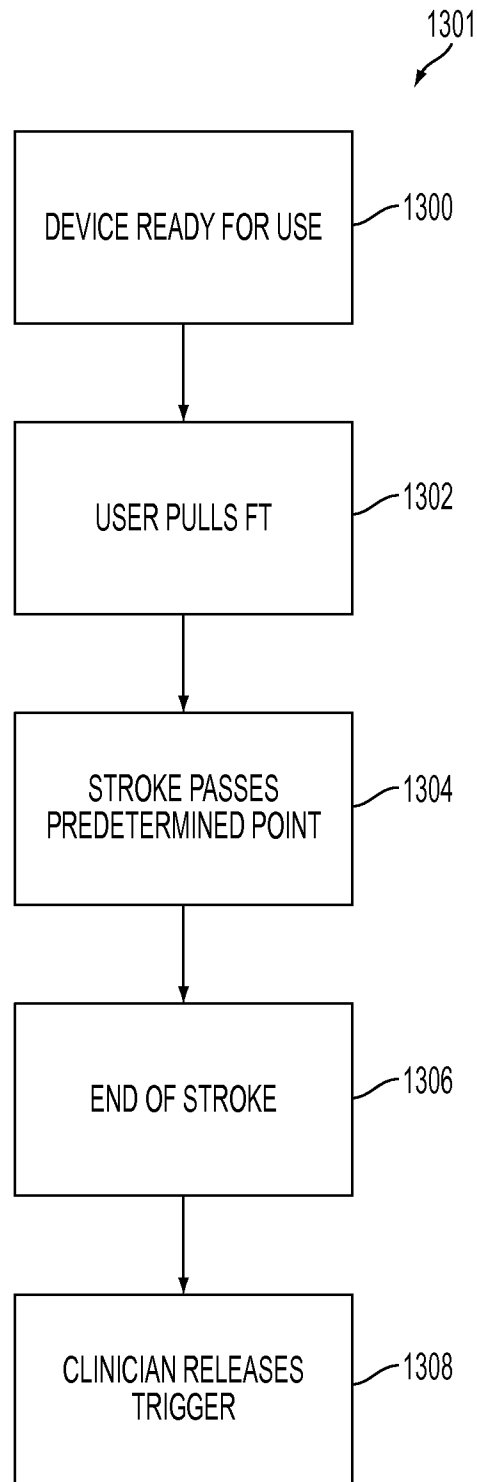


FIG. 54

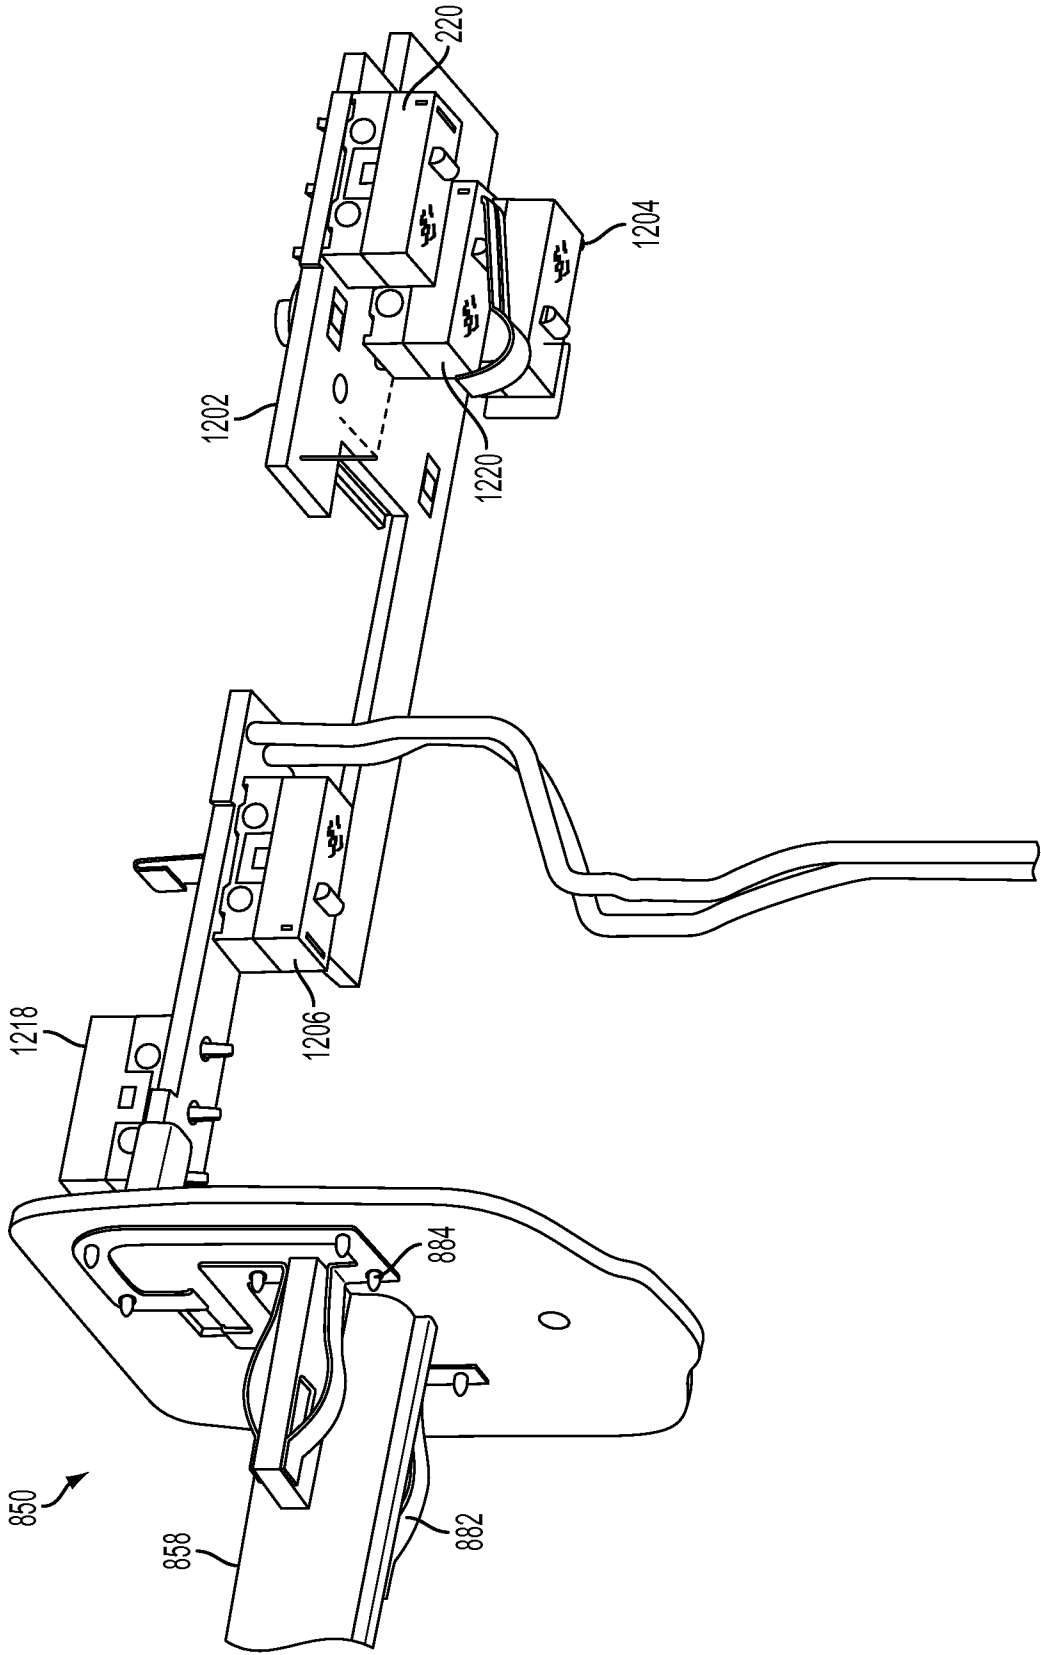


FIG. 55

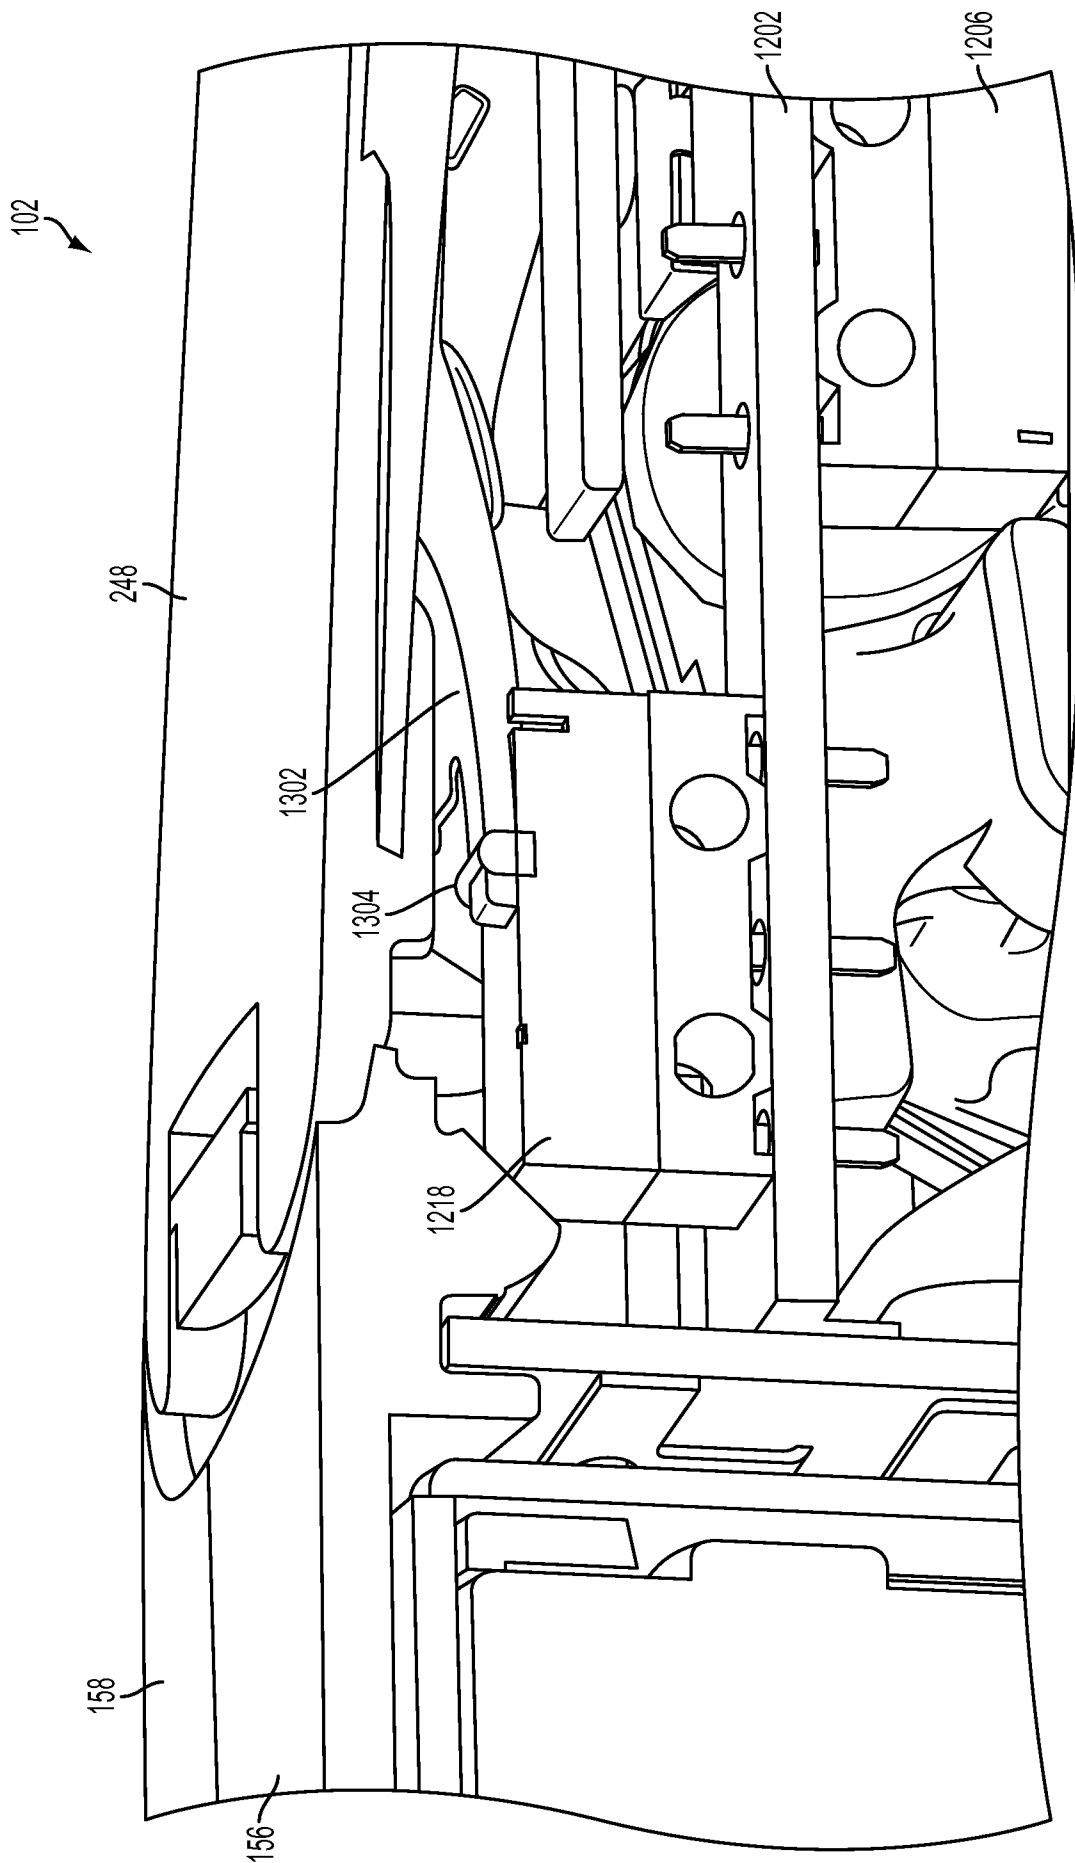


FIG. 56

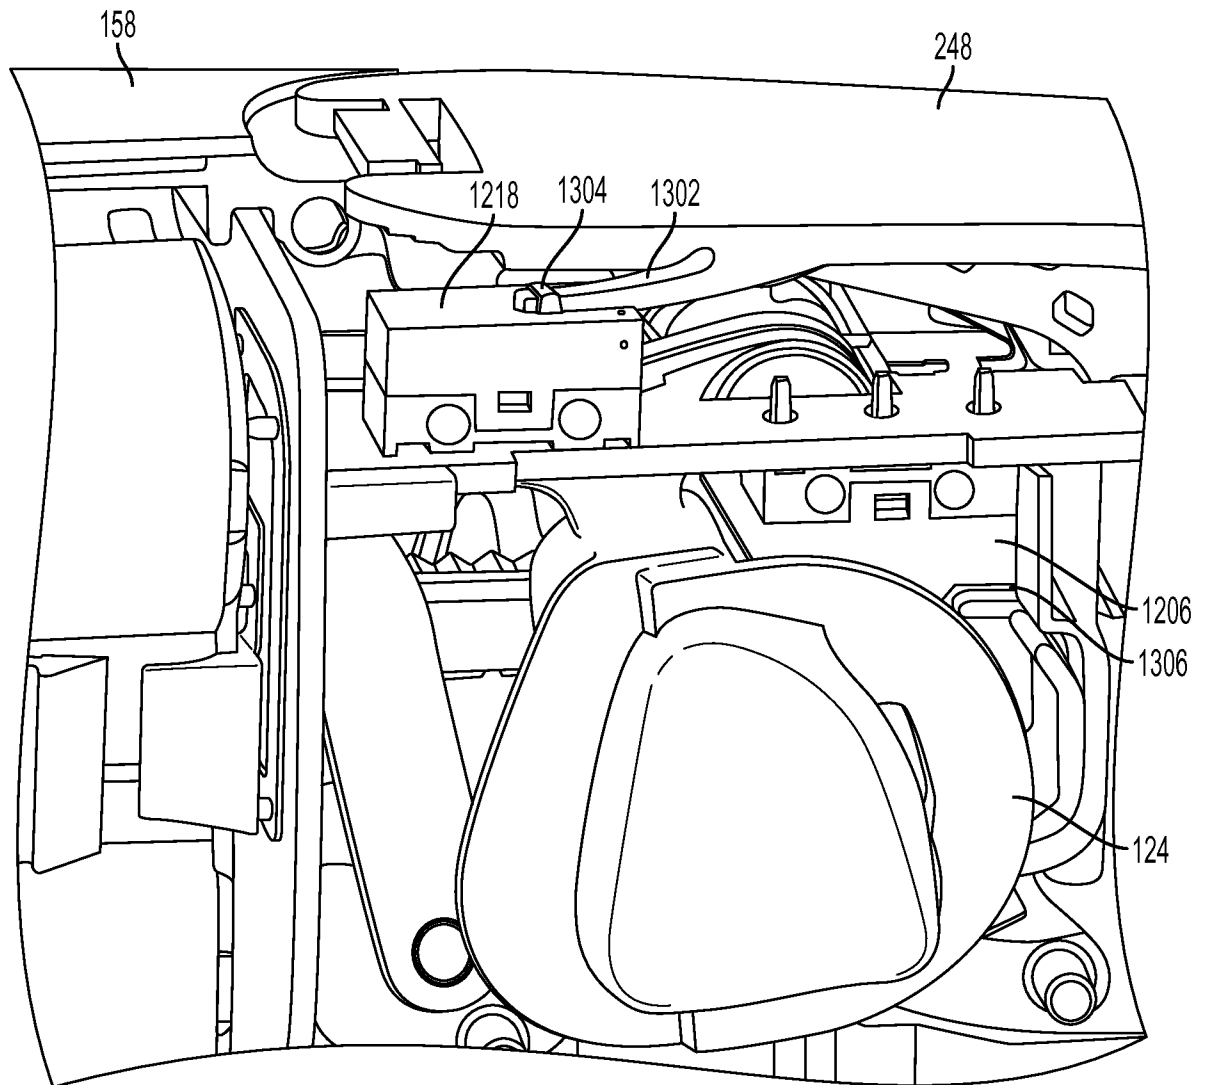


FIG. 57

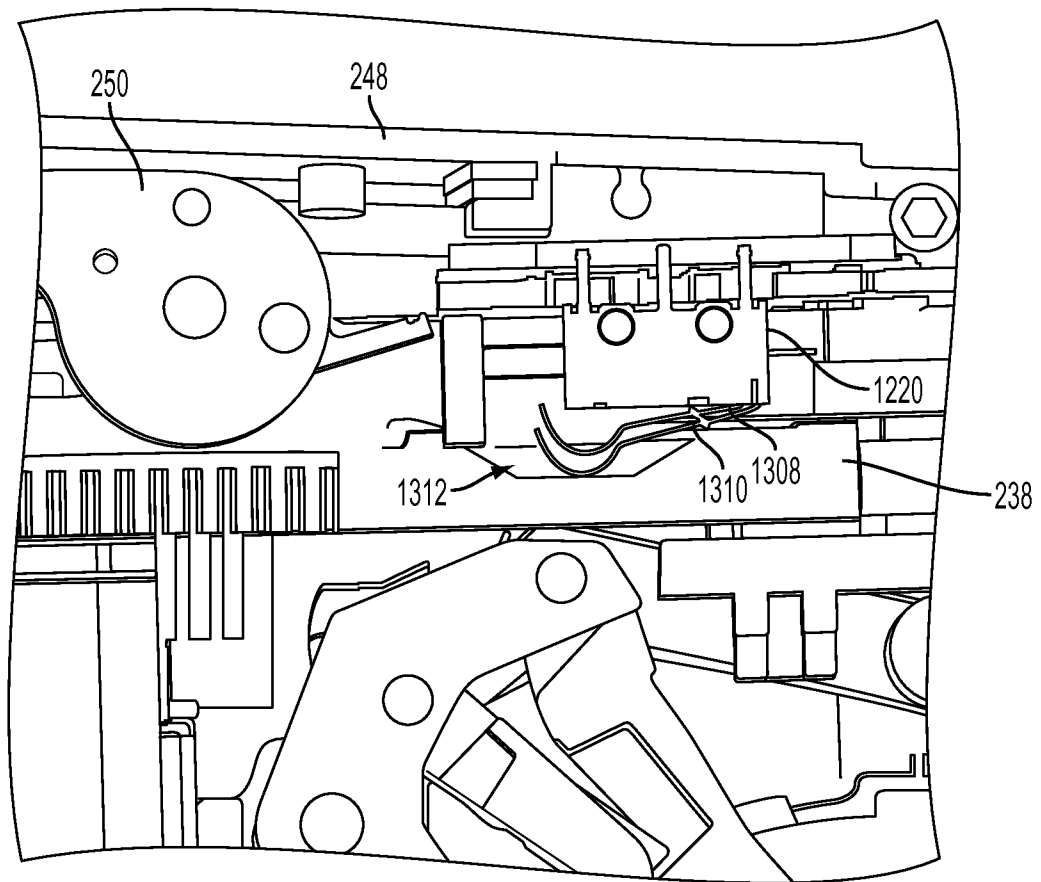


FIG. 58

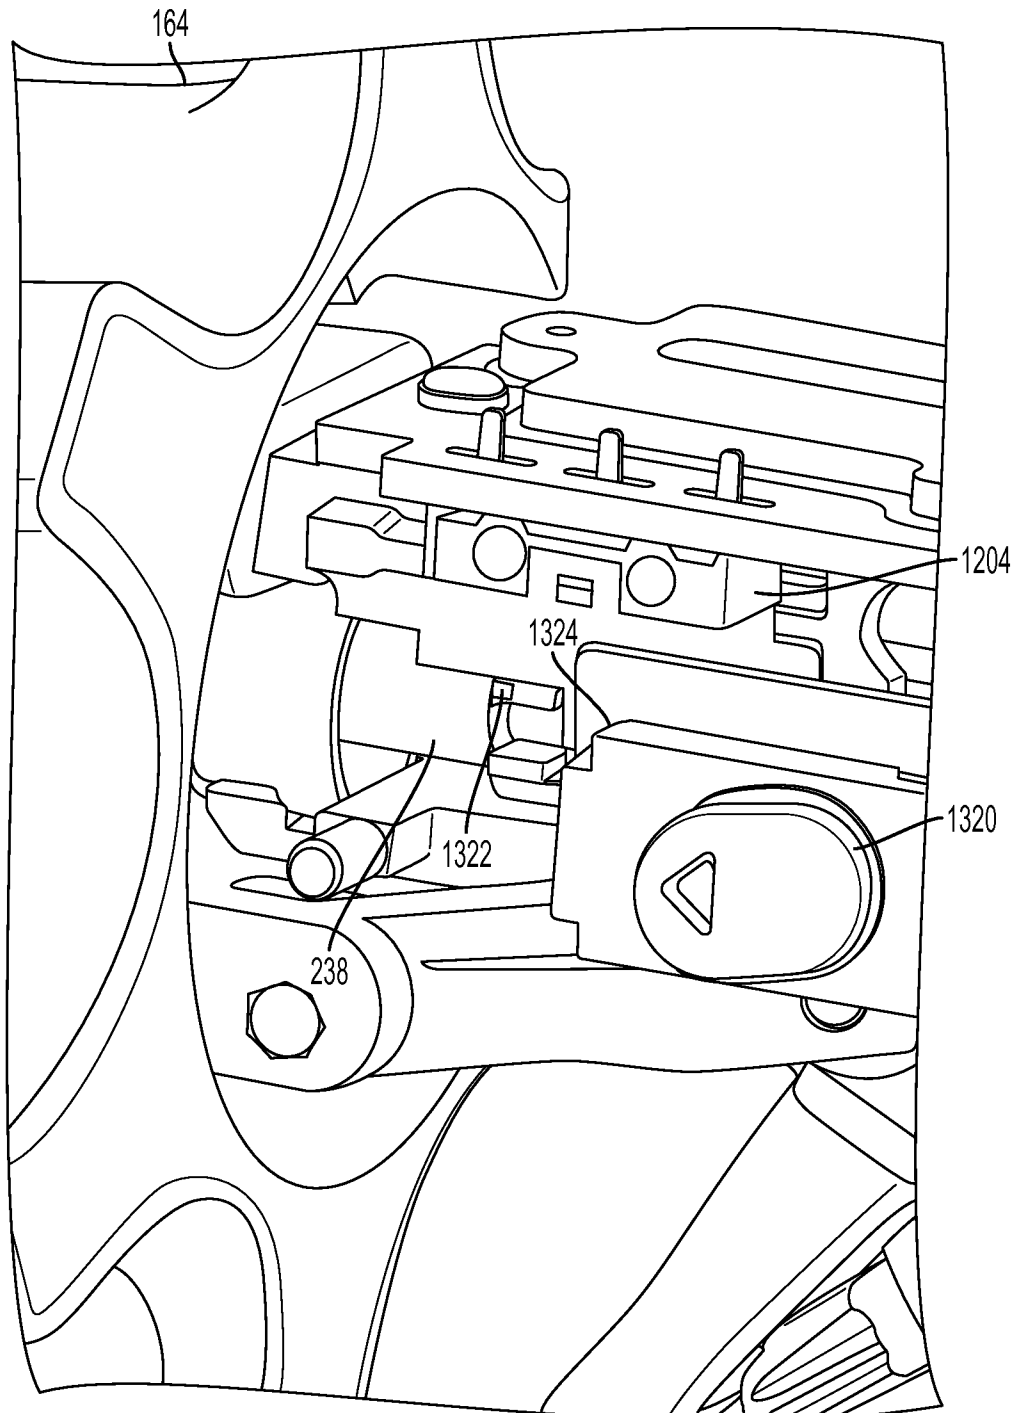


FIG. 59

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2011/053393

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61B17/072 H01M10/44 H02J7/00
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B H01M H02J

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EP0-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 1 813 207 A1 (ETHICON ENDO SURGERY INC [US]) 1 August 2007 (2007-08-01)	1-17
A	paragraph [0061] paragraph [0053] - paragraph [0056] paragraph [0065] - paragraph [0071]; figure 11	18-25
X	US 2010/089970 A1 (SMITH BRET W [US] ET AL) 15 April 2010 (2010-04-15)	1-14
A	paragraph [0138] - paragraph [0141]; figure 60	18-25
A	EP 2 090 240 A1 (ETHICON ENDO SURGERY INC [US]) 19 August 2009 (2009-08-19) paragraph [0029] - paragraph [0036]; figures	1,18
	----- -/--	

☒ Further documents are listed in the continuation of Box C.

☒ See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

24 November 2011

Date of mailing of the international search report

30/11/2011

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Nistor, Loredana

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2011/053393

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 2009/046394 A1 (ETHICON ENDO SURGERY INC [US]; SMITH KEVIN W [US]; BALES THOMAS [US];) 9 April 2009 (2009-04-09) page 63, line 21 - page 65, line 30; figures 35-36	1,18
A	----- EP 2 090 238 A1 (ETHICON ENDO SURGERY INC [US]) 19 August 2009 (2009-08-19) paragraph [0037] - paragraph [0045]; figure 11 -----	1,18

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2011/053393

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 1813207	A1	01-08-2007	AT 506015 T	15-05-2011
			AU 2007200357 A1	16-08-2007
			BR PI0701393 A	11-12-2007
			CA 2576470 A1	31-07-2007
			CN 101133972 A	05-03-2008
			EP 1813207 A1	01-08-2007
			EP 2272441 A1	12-01-2011
			JP 2007203057 A	16-08-2007
			KR 20070079050 A	03-08-2007
			SG 134314 A1	29-08-2007
			US 2007175956 A1	02-08-2007

US 2010089970	A1	15-04-2010	CN 102176869 A	07-09-2011
			EP 2349022 A2	03-08-2011
			US 2010089970 A1	15-04-2010
			WO 2010042786 A2	15-04-2010

EP 2090240	A1	19-08-2009	AT 505138 T	15-04-2011
			BR PI0901477 A2	06-04-2010
			CN 101507625 A	19-08-2009
			EP 2090240 A1	19-08-2009
			JP 2009189821 A	27-08-2009
			US 2009206136 A1	20-08-2009
			US 2010301096 A1	02-12-2010
			US 2011132965 A1	09-06-2011

WO 2009046394	A1	09-04-2009	AU 2008308496 A1	09-04-2009
			CA 2699481 A1	09-04-2009
			CN 102083373 A	01-06-2011
			EP 2197361 A1	23-06-2010
			JP 2010540192 A	24-12-2010
			WO 2009046394 A1	09-04-2009

EP 2090238	A1	19-08-2009	EP 2090238 A1	19-08-2009
			EP 2090249 A1	19-08-2009
			EP 2090250 A1	19-08-2009
			US 2009209979 A1	20-08-2009
