

(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
21 August 2008 (21.08.2008)

PCT

(10) International Publication Number
WO 2008/100437 A1

(51) International Patent Classification:

A61F 13/00 (2006.01)

(21) International Application Number:

PCT/US2008/001726

(22) International Filing Date: 8 February 2008 (08.02.2008)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

60/900,463 9 February 2007 (09.02.2007) US

(71) Applicant (for all designated States except US): KCI LICENSING INC. [US/US]; Legal Department - Intellectual Property, P.O. Box 659508, San Antonio, TX 78265-9508 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): ROBINSON, Timothy, Mark [GB/GB]; 27 Wellington Terrace, Basingstoke, Hampshire RG23 8HH (GB). LOCKE, Christopher, Brian [GB/GB]; 6 Bosworth Mews, Bournemouth, Dorset BH9 3SD (GB).

(74) Agents: MASON, Robert, W. et al.; Kinetic Concepts, Inc., P.O. Box 659508, San Antonio, TX 78265-9508 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).


Declaration under Rule 4.17:

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))

Published:

— with international search report
— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

(54) Title: A BREATHABLE INTERFACE SYSTEM FOR TOPICAL REDUCED PRESSURE

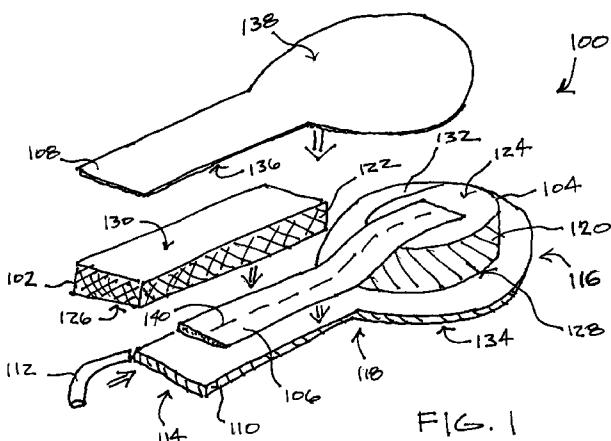

WO 2008/100437 A1

(57) Abstract: A breathable interface system including an applicator having an aperture therethrough; a drape substantially covering the applicator; a first pad section located between the drape and the applicator; a second pad section substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and a fabric layer located at least partially between the second pad section and the drape; and a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture; wherein the drape is secured to the applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.

A BREATHABLE INTERFACE SYSTEM FOR TOPICAL REDUCED PRESSURE**BACKGROUND OF THE INVENTION**5 **1. Field of the Invention**

The present application relates generally to systems and methods for providing reduced pressure tissue treatment to open wounds and other tissue sites. More particularly, the present application relates to a breathable interface systems for topical reduced pressure.

10 **2. Description of Related Art**

Clinical studies and practice have shown that providing a reduced pressure in proximity to a tissue site augments and accelerates the growth of new tissue at the tissue site. The applications of this phenomenon are numerous, but application of reduced pressure has been particularly successful in treating wounds and tissue sites. This treatment (frequently referred to in the medical community as “negative pressure wound therapy,” “reduced pressure therapy,” or “vacuum therapy”) provides a number of benefits, including faster healing, and increased formulation of granulation tissue.

Reduced pressure tissue treatment has recently been popularized by Kinetic Concepts, Inc. of San Antonio, Texas, through its commercially available VAC reduced pressure tissue treatment systems product line. In general, such reduced pressure tissue treatment systems 20 comprise a pad-based dressing, which is applied to the tissue and is sometimes referred to as the “tissue interface” or the “wound interface.”

Current dressings, however, have several disadvantages. They are difficult to apply to small wounds, and often lead to maceration of the wound periphery. Traditionally, dressings have been rather cumbersome, limiting many patient activities. Simply sitting on or rolling 25 onto a dressing may cause significant patient discomfort. Moreover, these actions may

compress the dressing and interfere with the application of reduced pressure to a manifold at the tissue site.

SUMMARY

The problems presented with these conventional dressings are solved by an improved breathable interface system for topical reduced pressure. One illustrative embodiment of the breathable interface system includes a first pad section, a second pad section, and a fabric layer, all positioned between a drape and an applicator. In addition, the dressing may include an interface component to facilitate fluid connection of a conduit to the dressing. Alternatively, a conduit may be placed in direct contact with or inserted directly into the dressing to deliver reduced pressure that is then distributed to a tissue site through the fabric layer and the pad sections.

In another illustrative embodiment, the breathable interface system may include a layer having a high moisture vapor transmission rate, which rapidly removes moisture from the periphery of the tissue site and insulates the periphery from exudate removed from the tissue site. Thus, these illustrative embodiments substantially eliminate or reduce maceration around a tissue site during reduced pressure tissue treatment, particularly around small tissue sites.

These and other illustrative embodiments also may include a fabric layer that provides additional fluid pathways that are less susceptible to collapsing under higher compressive loads, thereby improving the performance of reduced pressure tissue treatment in active patients. These additional fluid pathways also reduce the time to distribute reduced pressure to a tissue site, which enhances the effectiveness of intermittent reduced pressure tissue treatment.

One illustrative embodiment includes a breathable interface system including an applicator having an aperture therethrough; a drape substantially covering the applicator; a first pad section located between the drape and the applicator; a second pad section

substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and a fabric layer located at least partially between the second pad section and the drape; and a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced 5 pressure to the aperture; wherein the drape is secured to the applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.

Another illustrative embodiment includes a breathable interface system including an applicator having an aperture therethrough; a drape substantially covering the applicator; a first pad section located between the drape and the applicator; a second pad section 10 substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and a fabric layer located at least partially between the first pad section and the second pad section and the applicator; and a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture; wherein the drape is secured to the 15 applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.

Yet another illustrative embodiment includes a breathable interface system including an applicator having an aperture therethrough; a drape substantially covering the applicator; a first pad section located between the drape and the applicator; a second pad section 20 substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and a fabric layer located at least partially between the first pad section and the second pad section and the drape; and a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture; wherein the drape is secured to the 25 applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.

Still yet another illustrative embodiment includes a reduced pressure tissue treatment apparatus for applying reduced pressure tissue treatment to a tissue site including an applicator having an aperture therethrough; a drape substantially covering the applicator; a first pad section located between the drape and the applicator; a second pad section substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; a fabric layer located at least partially between the second pad section and the drape, wherein the drape is secured to the applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment; a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture; and a reduced pressure source in communication with the reduced pressure conduit to deliver reduced pressure to the tissue site.

Other objects, features, and advantages of the illustrative embodiments will become apparent with reference to the drawings and the detailed description that follow.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an exploded view of the breathable interface system according to an illustrative embodiment of the invention;

5 FIG. 2 is a perspective view of the breathable interface system without a drape according to an illustrative embodiment of the invention;

FIG. 3 is a bottom view of an applicator of a breathable interface system of FIGS. 1 and 2 according to an illustrative embodiment of the invention;

FIG. 4 is cross-sectional view of the breathable interface system along lines 4-4 of FIG. 2 according to an illustrative embodiment of the invention;

10 FIG. 5 is cross-sectional view of the breathable interface system according to another illustrative embodiment of the invention;

FIG. 6 is cross-sectional view of the breathable interface system according to another illustrative embodiment of the invention;

15 FIG. 7 is a schematic diagram of a reduced pressure tissue treatment system having a breathable interface system according to an illustrative embodiment of the invention;

FIG. 8 is a chart that compares the results of pressure transmission experiments on a conventional dressing and a breathable interface system according to an illustrative embodiment of the present invention; and

20 FIG. 9 is a chart that compares response times when subjected to intermittent application of reduced pressure under dry conditions of a conventional dressing and a breathable interface system according to an illustrative embodiment of the present invention.

DETAILED DESCRIPTION OF A PREFERRED EMBODIMENT

In the following detailed description of the preferred embodiments, reference is made to the accompanying drawings that form a part hereof, and in which is shown by way of illustration specific preferred embodiments in which the invention may be practiced. These 5 embodiments are described in sufficient detail to enable those skilled in the art to practice the invention, and it is understood that other embodiments may be utilized and that logical, structural, mechanical, electrical, and chemical changes may be made without departing from the spirit or scope of the invention. To avoid detail not necessary to enable those skilled in the art to practice the invention, the description may omit certain information known to those 10 skilled in the art. The following detailed description is, therefore, not to be taken in a limiting sense, and the scope of the present invention is defined only by the appended claims.

The term "reduced pressure" as used herein generally refers to a pressure less than the ambient pressure at a tissue site that is being subjected to treatment. In most cases, this reduced pressure will be less than the atmospheric pressure at which the patient is located. 15 Alternatively, the reduced pressure may be less than a hydrostatic pressure of tissue at the tissue site. Although the terms "vacuum" and "negative pressure" may be used to describe the pressure applied to the tissue site, the actual pressure applied to the tissue site may be significantly less than the pressure normally associated with a complete vacuum. Reduced pressure may initially generate fluid flow in the tube in the area of the tissue site. As the 20 hydrostatic pressure around the tissue site approaches the desired reduced pressure, the flow may subside, and the reduced pressure is then maintained. Unless otherwise indicated, values of pressure stated herein are gauge pressures.

The term "tissue site" as used herein refers to a wound or defect located on or within any tissue, including but not limited to, bone tissue, adipose tissue, muscle tissue, neural 25 tissue, dermal tissue, vascular tissue, connective tissue, cartilage, tendons, or ligaments. The

term "tissue site" may further refer to areas of any tissue that are not necessarily wounded or defective, but are instead areas in which it is desired to add or promote the growth of additional tissue. For example, reduced pressure tissue treatment may be used in certain tissue areas to grow additional tissue that may be harvested and transplanted to another tissue

5 location.

Referring to FIGS. 1-3, an illustrative embodiment of a breathable interface system 100 is shown. In this embodiment, the breathable interface system 100 includes a first pad section 102, a second pad section 104, and a fabric layer 106, all positioned between a drape 108 and an applicator 110. The breathable interface system 100 generally has one end 116 that is located substantially adjacent to or over a tissue site and another end 114 that is located distally away from end 116, in one example. Nearer to end 114, the fabric layer 106 may be positioned or located at least partially between the applicator 110 and the first pad section 102. Nearer to end 116, the fabric layer 106 may be positioned or located at least partially between the second pad section 104 and the drape 108. The fabric layer 106 extends along a portion of a top surface 124 of the second pad section 104 between the second pad section 104 and the drape 108. Once the fabric layer 106 reaches a side 120 of the second pad section 104 it transitions near the area 118 between the side 120 of the second pad section 104 and the side 122 of the first pad section 102 to extend along a portion of the bottom surface 126 of the first pad section 102 between the first pad section 102 and the applicator 110.

15

FIG. 2 is an illustrative embodiment of a breathable interface system 200 without the drape 108 placed on top of the first pad section 102, second pad section 104, and fabric layer 106 for illustration purposes. The fabric layer 106 can be seen extending over the top surface 124 of the second pad section 104 and beneath the bottom surface 126 of the first pad section 102. FIG. 3 is an illustrative embodiment of the applicator 110 including an aperture 302 that extends through the applicator 110 substantially near the end 116 of the applicator 110. The aperture 302 preferably is located near a tissue site to enable fluid to flow from the tissue site

20

25

to the first pad section 102, second pad section 104, fabric layer 106, and reduced pressure conduit 112 of the breathable interface systems herein described.

In an illustrative embodiment, any hydrogel or bonding agent may be applied to the aperture 302 and the applicator 110 for sealing or contact purposes with a tissue site. The 5 second pad section 104 is generally positioned to substantially cover the aperture 302, between the drape 108 and the applicator 110 as shown in FIGS. 4 and 6. In FIG. 5, the aperture 302 may be substantially covered by the fabric layer 106 as described herein. The size of the aperture 302 may vary to accommodate larger wounds, but in one embodiment, a size of about 10 to about 20 mm is advantageous for small wounds.

10 Referring to FIG. 4, an illustrative embodiment of the breathable interface system 100 is shown. The aperture 302 is shown disposed through the applicator 110. In addition, the breathable interface system 100 may further include an interface 402 that facilitates fluid communication between the first pad section 102 and/or fabric layer 106 and the reduced pressure conduit 112. Referring to FIG. 5, another illustrative embodiment of the breathable 15 interface system 500 is shown. The breathable interface system 500 may include a different arrangement of the first pad section 102, second pad section 104, and fabric layer 106 between the drape 108 and the applicator 110. In this illustrative embodiment, the fabric layer 106 is located between the bottom surface 126 of the first pad section 102 and the bottom surface 128 of the second pad section 104 and the top surface 132 of the applicator 110. The first pad 20 section 102 and second pad section 104 are located or positioned on top of the fabric layer 106. In this illustrative embodiment, the fabric layer 106 substantially covers the aperture 302. Referring to FIG. 6, yet another illustrative embodiment of the breathable interface system 600 is shown. In this illustrative embodiment, the fabric layer 106 is located between the top surface 124 of the second pad section 104 and the top surface 130 of the first pad section 102 25 and the bottom surface 136 of the drape 108.

In any of the breathable interface systems 100, 200, 500, and 600, the reduced pressure conduit 112 may be located in direct contact with the first pad section 102 and/or the fabric layer 106. The reduced pressure conduit 112 may be placed in direct contact with the first pad section 102 or the fabric layer 106 by directly inserting it into either of the first pad section 102 or the fabric layer 106 near the end 114 of the breathable interface system 100. In another 5 illustrative embodiment, the breathable interface systems 100, 200, 500, and 600 may further include the interface 402 as shown in FIG. 4 for facilitating the fluid communication and flow between the first pad section 102 and/or fabric layer 106 and the reduced pressure conduit 112. In yet another illustrative embodiment, the reduced pressure conduit 112 may not be in direct 10 contact with the first pad section 102 and/or fabric layer 106, but may otherwise be in fluid communication with the first pad section 102 and/or fabric layer 106.

In one illustrative embodiment, the side 120 of the second pad section 104 extends between the top surface 124 and a bottom surface 128 of the second pad section 104. The bottom surface 128 of the second pad section 104 may have a surface area that may cover 15 substantially all or a portion of the top surface 132 of the end 116 of the applicator 110. Additionally, the side 122 of the first pad section 102 extends between the top surface 130 and the bottom surface 126 of the first pad section 102. The bottom surface 126 of the first pad section 102 may have a surface area that may cover substantially all or a portion of the end 114 of the top surface 132 of the applicator 110.

20 The applicator 110 may be any size desirable to adequately provide effective covering and functionality to a tissue site as described herein. In one aspect, the applicator 110 includes a bottom surface 134 that may preferably contact the tissue site. The end 116 of the applicator 110 may have a surface area of a different shape than the end 114 of the applicator 110. For example, the surface area of the end 116 as shown in FIG. 1 shows a surface area of a 25 substantially circular shape. Nevertheless, the shape of the end 116 of the applicator 110 may any desirable shape, symmetric, asymmetric, or otherwise, to provide the covering of a tissue

site and functionality as herein described. In one illustrative embodiment, the end 114 of the applicator 110 may have a surface area that approximates a rectangular shape; however, the end 114 of the applicator 110 may also be any desirable shape, symmetric, asymmetric, or otherwise, to provide the covering and functionality as herein described.

5 Preferably, the bottom surface 136 of the drape 108 covers and secures the first pad section 102, fabric layer 106, and second pad section 104 to the top surface 132 of the applicator 110. In one aspect, the applicator 110 and drape 108 are sealed together substantially around the perimeter or periphery of their respective shapes. Preferably, the applicator 110 and drape 108 isolate the tissue site from its surrounding environment and
10 maintain a reduced pressure at the tissue site when reduced pressure is applied as described herein. The applicator 110 may be secured to drape 108 with any suitable bonding agent, such as an acrylic adhesive or hydrogel. In addition, the applicator 110 may be joined to the drape 108 by other commonly known means, such as bonding, adhesives, welding, fastening, and sintering, for example. Typically, a hydrogel or other tissue-friendly bonding agent may be
15 applied to the tissue side or bottom surface 134 of the applicator 110, which is then placed into the tissue site or in contact with the perimeter of the tissue site to secure the dressing to the tissue site.

In an illustrative embodiment, the first pad section 102 and second pad section 104 may be a material known in the art to be suitable for reduced pressure tissue treatment, the size
20 and shape of which may be varied to accommodate tissue sites of various size and shape as described herein. Preferably, the first pad section 102 and second pad section 104 include a plurality of flow channels or pathways to facilitate the distribution of reduced pressure or fluids to or from the tissue site. In one illustrative embodiment, the first pad section 102 and second pad section 104 are porous foam that includes interconnected cells or pores that act as
25 flow channels. In addition to the above, the first pad section 102 and second pad section 104 may be a material such as an open cell, reticulated foam that is formed from a range of

polymers, including without limitation polyurethane, polyolefin, vinyl acetate, polyvinyl alcohol, and their copolymers. Additionally, the first and second pad section 102, 104 may be woven or non-woven materials, including 3-dimensional fabric structures. The pads may also be made from a sintered polymer, including materials such as sintered polyolefin, ethylene 5 vinyl acetate, and fluoropolymer. The first pad section 102 and second pad section 104 may also be any other type of open-cell, reticulated foam, such as GranuFoam® and Whitefoam™ that are manufactured by Kinetic Concepts, Inc. of San Antonio, Texas. If open-cell foam is used, the porosity may vary, but is preferably about 400 to 600 microns. Alternatively, gauze or any other material suited to a particular biological application may be used to construct first 10 pad section 102 and second pad section 104. In a certain illustrative embodiment, first pad section 102 and second pad section 104 may be constructed as a single, unitary pad. In another illustrative embodiment, first pad section 102 and second pad section 104 may be a multi-component or multi-layered pad section. Preferably, the thicknesses of the first pad section 102 and second pad section 104 is from about 1 mm to about 50 mm, and in one 15 implementation from about 5 mm to about 20 mm, although any thicknesses may be used.

In an illustrative embodiment, the fabric layer 106 may be a woven or non-woven fabric material known in the art, the size and shape of which may be varied to accommodate tissue sites of various size and shape as described herein. It may be constructed from any fiber material that maintains its structural integrity when exposed to fluids, such as polyamide, 20 polyolefin, nylon, polyester, a polyamide coated with polyurethane, any polymeric mesh, a non-woven (air layed) melt blown polymer, or flexible sintered polymer. The fabric layer 106 may also be a fabric covered with adhesive or hydrogel to facilitate bonding to the tissue site, where the fabric layer 106 extends beyond the applicator 110. The material may be woven together to form a layer of appropriate dimensions, or it may be any type of open cell mesh 25 construction of appropriate dimensions. As illustrated in FIG. 1, the fabric layer 106 may also be folded and include stitching 140 to provide additional channels and structural support. A

folded fabric layer may be stitched lengthwise down the middle, as depicted in Figure 2, around the edges, or any combination thereof. As an alternative to stitching, a folded fabric layer may be secured with an acrylic adhesive or any other suitable bonding agent. The fabric layer 106 may also include several overlapping layers joined together by any known means.

5 The thicknesses of the fabric layer 106 may be from about 1 mm to about 50 mm, or alternatively about 5 mm to about 20 mm, although any thicknesses may be used.

The drape 108 may be a flexible material having a sufficiently high moisture vapor transmission rate (“MTVR”) to preclude tissue maceration, typically greater than 600 mg/m²/day. In one aspect, plastics and thermoplastics are an example of suitable materials for 10 the drape 108. And like the drape 108, the applicator 110 generally is constructed from any flexible material having a sufficiently high MTVR to preclude maceration of the tissue site, such as plastics and thermoplastics.

The reduced pressure conduit 112 may represent any conduit tubing, line, or path through which a gas, liquid, gel, or other fluid may be carried, and may have more than one 15 internal lumen. While the reduced pressure conduit 112 may be inflexible, it is preferred that it be flexible enough for ease of use and comfort for a patient. The reduced pressure conduit is configured for connection to a reduced pressure source to provide delivery of reduced pressure.

In an illustrative embodiment, the breathable interface systems 100, 200, 500, and 600 20 may be lightweight, low-profile interface systems for low-severity, small tissue sites, but the principles are readily extendable by a person of ordinary skill in the art to larger, more extensive tissue sites, as well as numerous other types of tissue treatments.

Referring again to FIGS. 1-6, the aperture 302 is placed over a tissue site and the 25 reduced pressure source 704 delivers a reduced pressure through the reduced pressure conduit 112 to the breathable interface systems 100, 200, 500, and 600. The aperture 302 may be a single aperture as shown, or any number or plurality of holes, openings, apertures, slits, or the

like desirable for providing distribution of reduced pressure and fluid transmission between the tissue site and the first pad section 102, second pad section 104, and fabric layer 106. As described above, the first pad section 102 and second pad section 104 may include pathways or channels that permit the reduced pressure to be distributed throughout the breathable 5 interface systems 100, 200, 500, and 600, and that permit fluids to be removed from a tissue site through the aperture 302. The weave or mesh structure of the fabric layer 106 provides additional fluid pathways that are less susceptible to collapsing under compressive loads that may be applied to the breathable interface systems 100, 200, 500, and 600, such as those encountered when a patient rolls in bed or otherwise moves causing compression of the 10 dressing. The additional fluid pathways also reduce the time required to distribute reduced pressure to a tissue site. As detailed below, testing has shown that pressure changes by a reduced pressure source are communicated to the tissue site much more quickly with a dressing configured like that of the breathable interface systems 100, 200, 500, and 600.

Referring to FIG. 7, an illustrative embodiment of a reduced pressure tissue treatment 15 system 700 incorporating the novel features of the breathable interface system is shown. The reduced pressure tissue treatment system 700 includes a breathable interface system 701 similar to the other breathable interface system described herein, which is applied to a tissue site 702 for treatment. Breathable interface system 100 is fluidly connected to a reduced pressure source 704 by a reduced pressure conduit 112. In certain embodiments, the reduced 20 pressure tissue treatment system 700 may also include a canister 706 for collecting fluid and other non-gaseous exudates extracted from the 702.

Referring to FIG. 8, a chart that compares the results of pressure transmission tests on a conventional dressing and a breathable interface system 100 as substantially described above is shown. In the tests, reduced pressure was applied to and water was pumped through each 25 breathable interface system 100 while the breathable interface system 100 was subjected to a range of compressive forces. Pressure measurements were taken on both sides of the

compressive forces to determine the performance of each specimen. The results, as shown in FIG. 8, demonstrate that a breathable interface system 100 as described above enables pressure communication across the compressive load to a much greater extent than a conventional dressing.

5 The flow of water was set to approximately 20 mls/hr and a compressive force from approximately 0 N to about 500 – 930 N was applied to the conventional dressing and the breathable interface system 100. The y-axis 802 represents the amount of reduced pressure or vacuum measured at either the pump or the dressing/breathable interface system 100. The x-axis 804 represents the duration of time expired from the start of the tests. Line 806 represents
10 the magnitude of the reduced pressure at the pump for the conventional dressing and the line 808 represents the magnitude of the reduced pressure at the opposite side of the dressing. As can be seen from FIG. 8, a compressive force of approximately 900 N was applied to the conventional dressing and the amount of measurable reduced pressure was approximately 0 mm Hg. at the dressing, as shown by line 808. At the start of event 814, the compressive force
15 was released, thus the amount of measurable reduced pressure at the dressing increased to approximately 120 mm Hg. At the end of event 814, a compressive force was applied at a magnitude of 525 N and the amount of measurable reduced pressure dropped back to approximately 0 mm Hg. During this same event, the measurable reduced pressure at the pump side of the dressing, as shown by line 806, stayed at approximately 125 mm Hg. This
20 shows that with a conventional dressing under compressive force, the amount of reduced pressure through the dressing is approximately 0 mm Hg. Similarly, at events 816, 818, and 820, compressive forces were released and reapplied at approximately 250 N. It can be seen
25 from FIG. 8, that essentially the same results followed. Namely, as soon as a compressive force was applied, the measurable amount of reduced pressure through the conventional dressing dropped to 0 mm Hg, or near 0 mm Hg.

Conversely, line 810 represents the magnitude of the reduced pressure at the pump for the breathable interface system 100 and the line 812 represents the magnitude of the reduced pressure at the opposite side of the dressing. As described above, a compressive force of approximately 900 N was applied to the conventional dressing and the amount of measurable 5 reduced pressure was approximately 50 mm Hg at the dressing, as shown by line 812. At the start of event 814, the compressive force was released, thus the amount of measurable reduced pressure at the dressing increased to approximately 120 mm Hg. At the end of event 814, a compressive force was applied at a magnitude of 525 N and the amount of measurable reduced 10 pressure was reduced to approximately 50 mm Hg. During this same event, the measurable reduced pressure at the pump side of the dressing, as shown by line 810, stayed at approximately 125 mm Hg. This shows that with a breathable interface system 100 under compressive force, the amount of reduced pressure is still substantial. Similarly, at events 15 816, 818, and 820, compressive forces were released and reapplied at approximately 250 N. It can be seen from FIG. 8, that even better results followed. Namely, as soon as a compressive force of approximately 250 N was applied, the measurable amount of reduced pressure through the conventional dressing increased to between approximately 70 mm Hg. and 100 20 mm Hg.

Referring to FIG. 9, another chart is shown that compares response times of a conventional dressing and a breathable interface system 100 as substantially described above 25 in FIG. 8 when subjected to intermittent application of reduced pressure under dry conditions. The response times illustrated in FIG. 9 demonstrate that a conventional dressing responds much more slowly than the breathable interface system 100 described above when subjected to these conditions.

Pressure measurements were taken on both sides of the compressive forces to 25 determine the response times of a conventional dressing compared with the breathable interface system 100 described above. The results, as shown in FIG. 9, demonstrate that a

breathable interface system 100 as described above enables faster response times to the intermittent application and release of reduced pressure. The y-axis 902 represents the amount of reduced pressure or vacuum measured at either the pump or the dressing/breathable interface system 100. The x-axis 904 represents the duration of time expired from the start of 5 the tests. Line 906 represents the magnitude of the reduced pressure measured at the pump for the conventional dressing and the line 908 represents the magnitude of the reduced pressure at the opposite side of the dressing. Line 910 represents the magnitude of the reduced pressure measured at the pump for the breathable interface system 100 and the line 912 represents the magnitude of the reduced pressure measured at the opposite side of the breathable interface 10 system 100.

As can be seen from FIG. 9, a reduced pressure is cycled on and off between approximately 0 mm Hg and 125 mm Hg. The lines 906 and 910 fairly closely match each other showing that there is little difference of measurable reduced pressure during the tests at the pump side of the dressing/breathable interface system 100 during the cycling of the 15 reduced pressure. At the other side of the dressing, line 908 shows a lag time in achieving the applied reduced pressure at the conventional dressing. This can be seen as line 908 has an arc to its shape representing the gradual building of reduced pressure before it attains full reduced pressure. Conversely, line 912 shows sharp transitions when the reduced pressure is cycled on and off, thus representing that the breathable interface system 100 provides for improved fluid 20 transmission and response to reduced pressure than conventional dressings.

It should be apparent from the foregoing that an invention having significant advantages has been provided. While the invention is shown in only a few of its forms, it is not just limited but is susceptible to various changes and modifications without departing from the spirit thereof.

We claim:

1. A breathable interface system comprising:
 - an applicator having an aperture therethrough;
 - 5 a drape substantially covering the applicator;
 - a first pad section located between the drape and the applicator;
 - a second pad section substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and
 - 10 a fabric layer located at least partially between the second pad section and the drape; and
 - a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture;
 - 15 wherein the drape is secured to the applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.
2. The breathable interface system of claim 1, wherein the fabric layer is located at least partially between the first pad section and the applicator.
- 20 3. The breathable interface system of claim 1 further comprising an interface located between the reduced pressure conduit and at least one of the first pad section and the fabric layer.
- 25 4. The breathable interface system of claim 1, wherein the first pad section and the second pad section are selected from the group consisting of open-cell reticulated foam, sintered polymers, ethylene vinyl acetate, fluoropolymers, polyurethane, polyolefin, vinyl acetate, polyvinyl alcohol, and their copolymers.

5. The breathable interface system of claim 1, wherein the fabric layer is selected from the group consisting of woven fabric, non-woven fabric, polyamide, nylon, polyamide coated with polyurethane, polymeric meshes, non-woven melt blown polymers, and flexible sintered polymers.
- 10 6. The breathable interface system of claim 1, wherein the first pad section, the second pad section, and the fabric layer have a thickness of from about 5 mm to about 20 mm.
- 15 7. The breathable interface system of claim 1, wherein the fabric layer includes several overlapping layers joined together.
- 20 8. A breathable interface system comprising:
an applicator having an aperture therethrough;
a drape substantially covering the applicator;
a first pad section located between the drape and the applicator;
a second pad section substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and
a fabric layer located at least partially between the first pad section and the second pad section and the applicator; and
a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture;
wherein the drape is secured to the applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.
- 25 9. The breathable interface system of claim 9 further comprising an interface located between the reduced pressure conduit and at least one of the first pad section and the fabric layer.
- 30 10. The breathable interface system of claim 8, wherein the first pad section and the second pad section are selected from the group consisting of open-cell reticulated foam, GranuFoam[®], WhitefoamTM, sintered polymers, ethylene

vinyl acetate, fluoropolymers, polyurethane, polyolefin, vinyl acetate, polyvinyl alcohol, and their copolymers.

11. The breathable interface system of claim 8, wherein the fabric layer is selected from the group consisting of woven fabric, non-woven fabric, polyamide, nylon, polyamide coated with polyurethane, polymeric meshes, non-woven melt-blown polymers, and flexible sintered polymers.
12. The breathable interface system of claim 8, wherein the first pad section, the second pad section, and the fabric layer have a thickness of from about 5 mm to about 20 mm.
13. The breathable interface system of claim 8, wherein the fabric layer includes several overlapping layers joined together.
14. A breathable interface system comprising:
 - an applicator having an aperture therethrough;
 - a drape substantially covering the applicator;
 - a first pad section located between the drape and the applicator;
 - a second pad section substantially covering the aperture and located between the drape and the applicator, the second pad section substantially adjacent to the first pad section; and
 - a fabric layer located at least partially between the first pad section and the second pad section and the drape; and

a reduced pressure conduit in communication with one of the first pad section and the fabric layer for providing reduced pressure to the aperture; wherein the drape is secured to the applicator, covering the first pad section, the second pad section, and the fabric layer in a substantially sealed environment.
15. The breathable interface system of claim 14 further comprising an interface located between the reduced pressure conduit and at least one of the first pad section and the fabric layer.

16. The breathable interface system of claim 14, wherein the first pad section and the second pad section are selected from the group consisting of open-cell reticulated foam, GranuFoam®, Whitefoam™, sintered polymers, ethylene vinyl acetate, fluoropolymers, polyurethane, polyolefin, vinyl acetate, polyvinyl alcohol, and their copolymers.

5

17. The breathable interface system of claim 14, wherein the fabric layer is selected from the group consisting of woven fabric, non-woven fabric, polyamide, nylon, polyamide coated with polyurethane, polymeric meshes, non-woven melt blown polymers, and flexible sintered polymers.

10



18. The breathable interface system of claim 14, wherein the first pad section, the second pad section, and the fabric layer have a thickness of from about 5 mm to about 20 mm.

15

19. The breathable interface system of claim 14, wherein the fabric layer includes several overlapping layers joined together.

20. A reduced pressure tissue treatment apparatus for applying reduced pressure tissue treatment to a tissue site comprising:
20 an applicator having an aperture therethrough;
an drape substantially covering the applicator;
a first pad section located between the drape and the applicator;
a second pad section substantially covering the aperture and located between
25 the drape and the applicator, the second pad section substantially adjacent to
the first pad section;
a fabric layer located at least partially between the second pad section and the
drape, wherein the drape is secured to the applicator, covering the first pad
section, the second pad section, and the fabric layer in a substantially sealed
30 environment;
a reduced pressure conduit in communication with one of the first pad section
and the fabric layer for providing reduced pressure to the aperture; and
a reduced pressure source in communication with the reduced pressure conduit
to deliver reduced pressure to the tissue site.

21. The reduced pressure tissue treatment apparatus of claim 20, wherein the fabric layer is located at least partially between the first pad section and the applicator.
- 5
22. The reduced pressure tissue treatment apparatus of claim 20, wherein the first pad section and the second pad section are selected from the group consisting of open-cell reticulated foam, GranuFoam®, Whitefoam™, sintered polymers, ethylene vinyl acetate, fluoropolymers, polyurethane, polyolefin, vinyl acetate, polyvinyl alcohol, and their copolymers.
- 10
23. The reduced pressure tissue treatment apparatus of claim 20, wherein the fabric layer is selected from the group consisting of woven fabric, non-woven fabric, polyamide, nylon, polyamide coated with polyurethane, polymeric meshes, non-woven melt blown polymers, and flexible sintered polymers.
- 15
24. The reduced pressure tissue treatment apparatus of claim 20, wherein the first pad section, the second pad section, and the fabric layer have a thickness of from about 5 mm to about 20 mm.
- 20
25. The reduced pressure tissue treatment apparatus of claim 20, wherein the fabric layer includes several overlapping layers joined together.

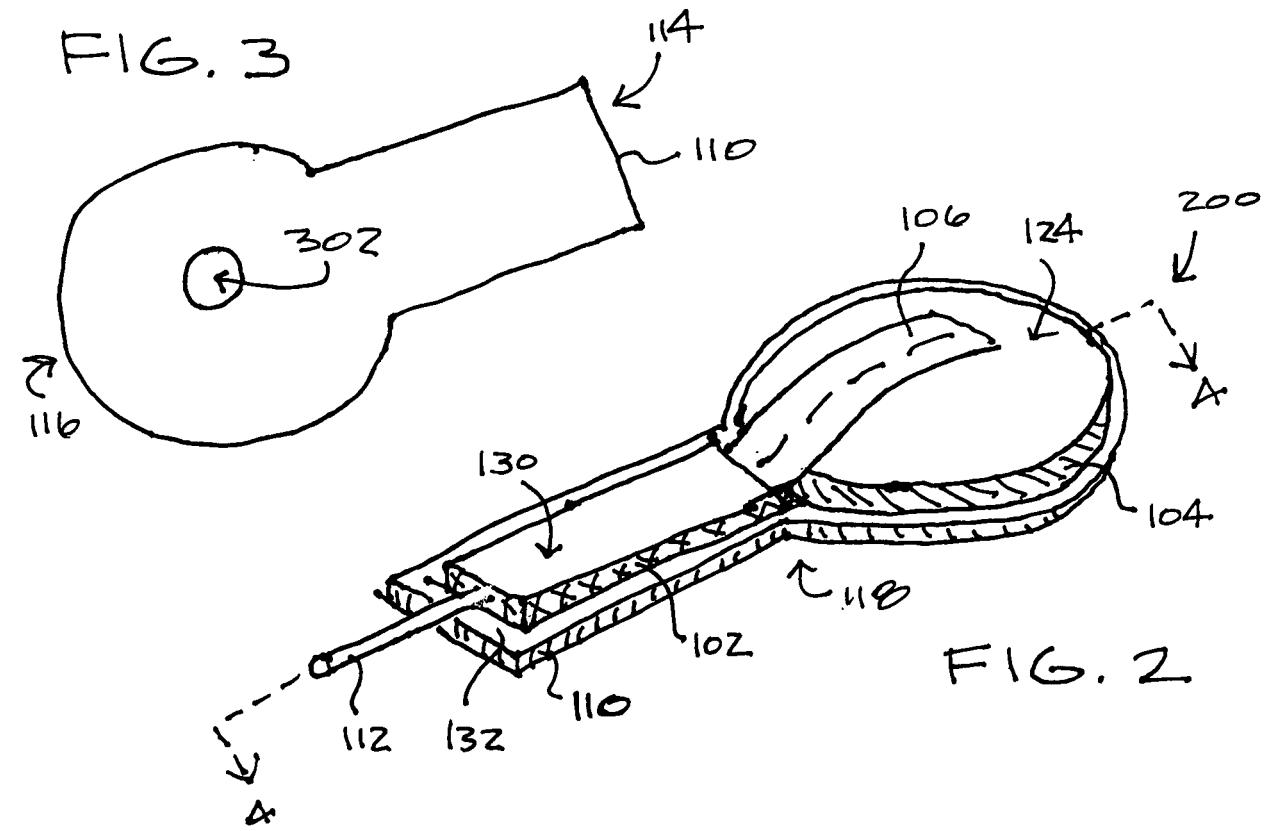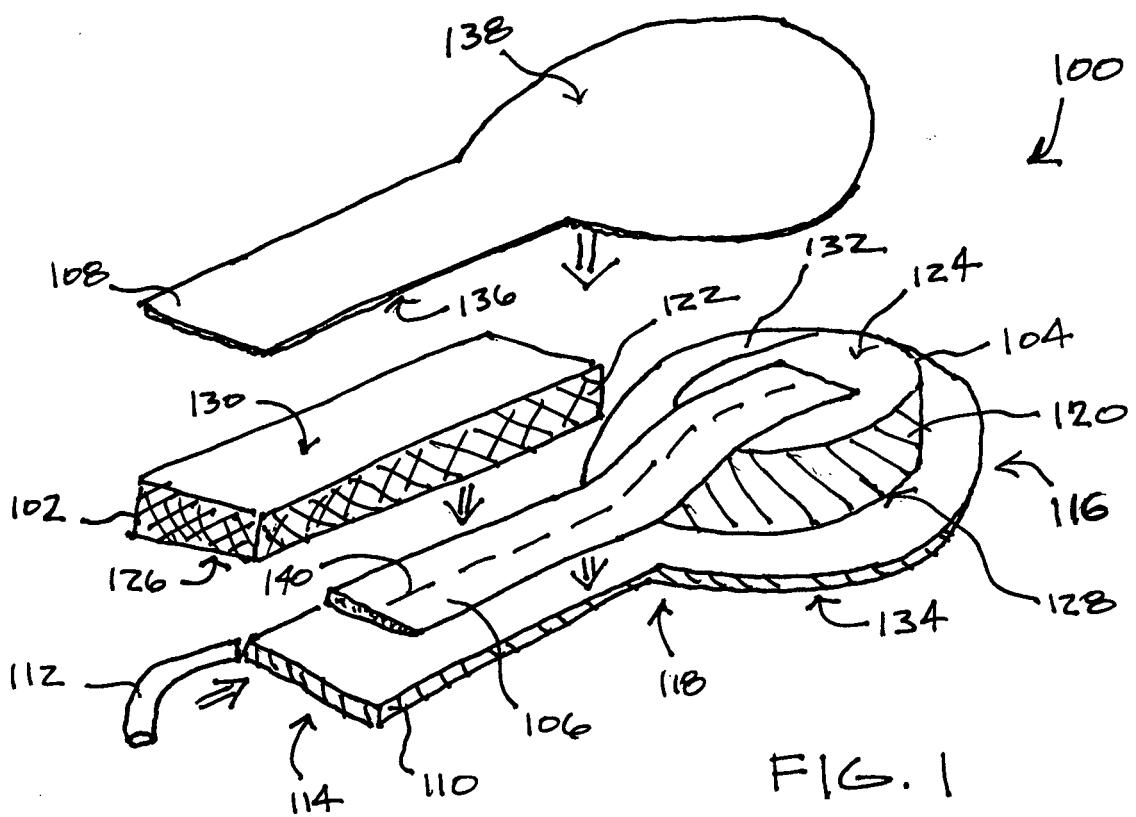

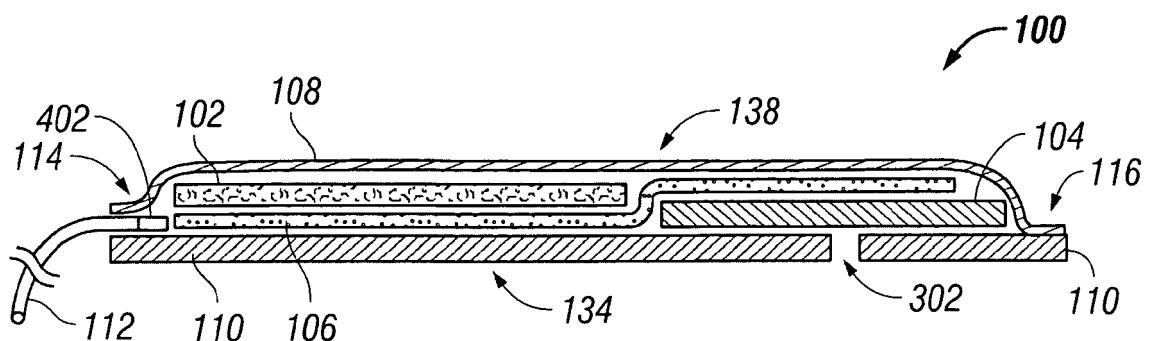


FIG. 4

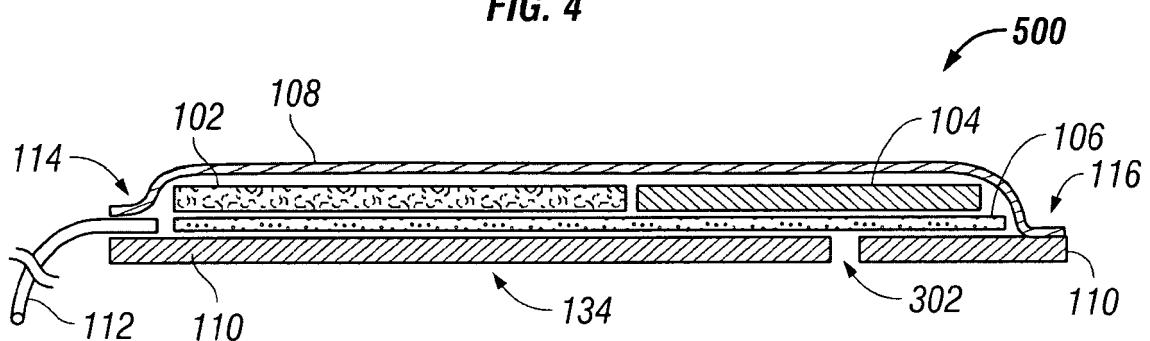


FIG. 5

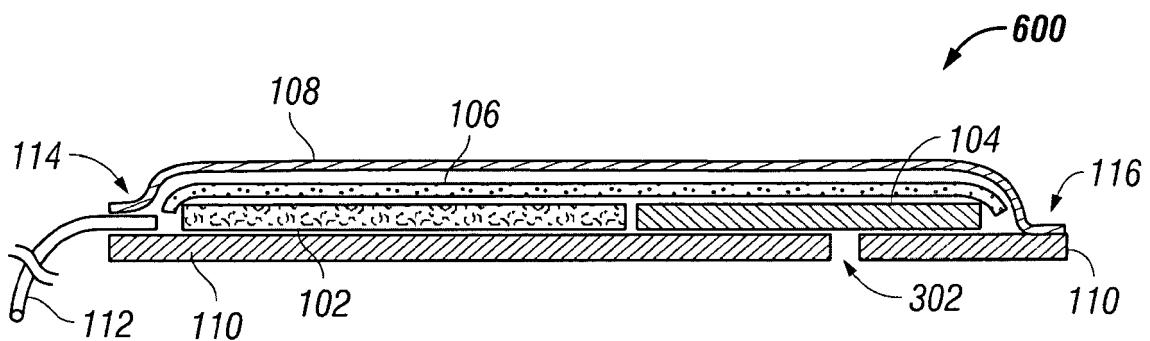


FIG. 6

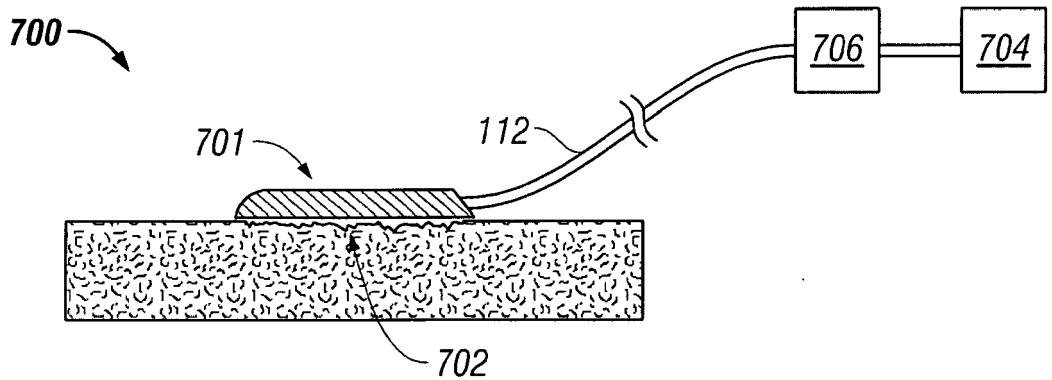


FIG. 7

Pressure Transmission in Compressed Foam & Foam/Fabric Strips under 500 -
930N compression 20ml/hr water flow

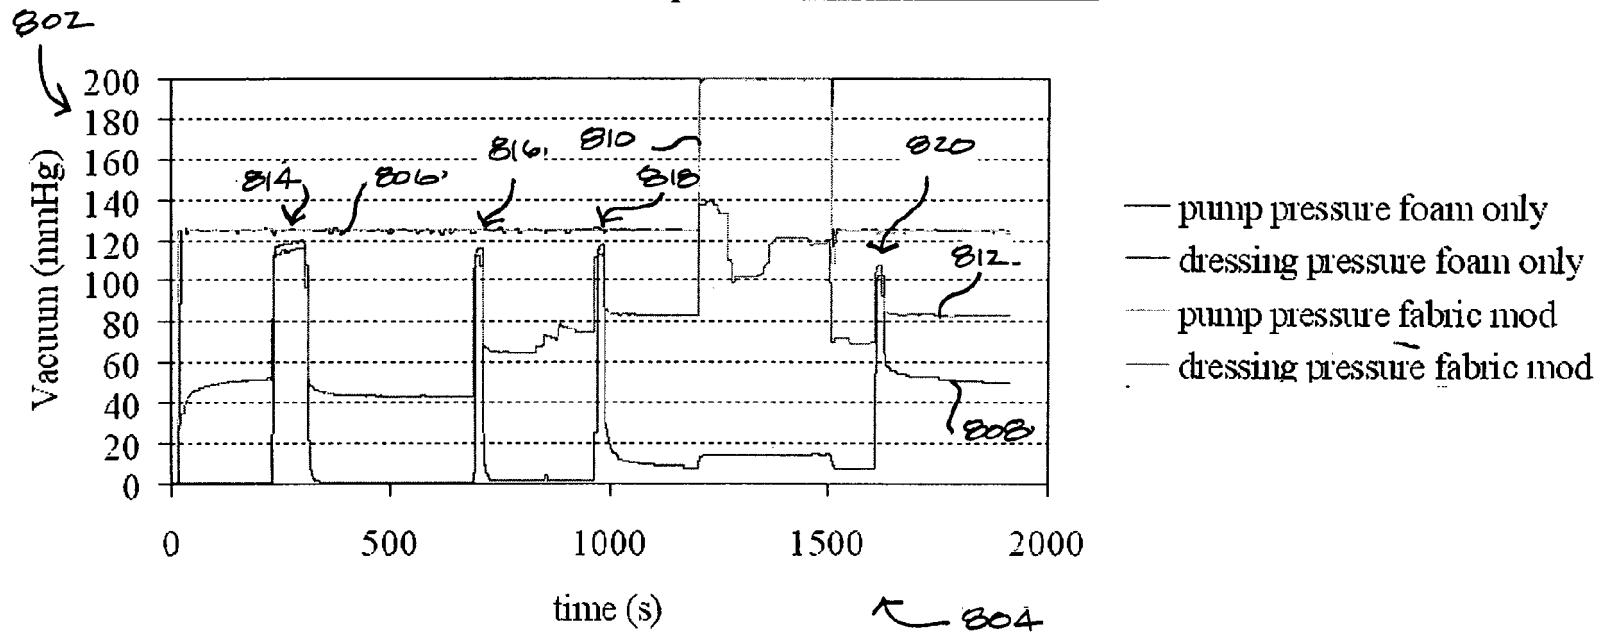


FIG. 8

Pressure Transmission in Compressed Foam & Foam/Fabric Strips under 930N compression

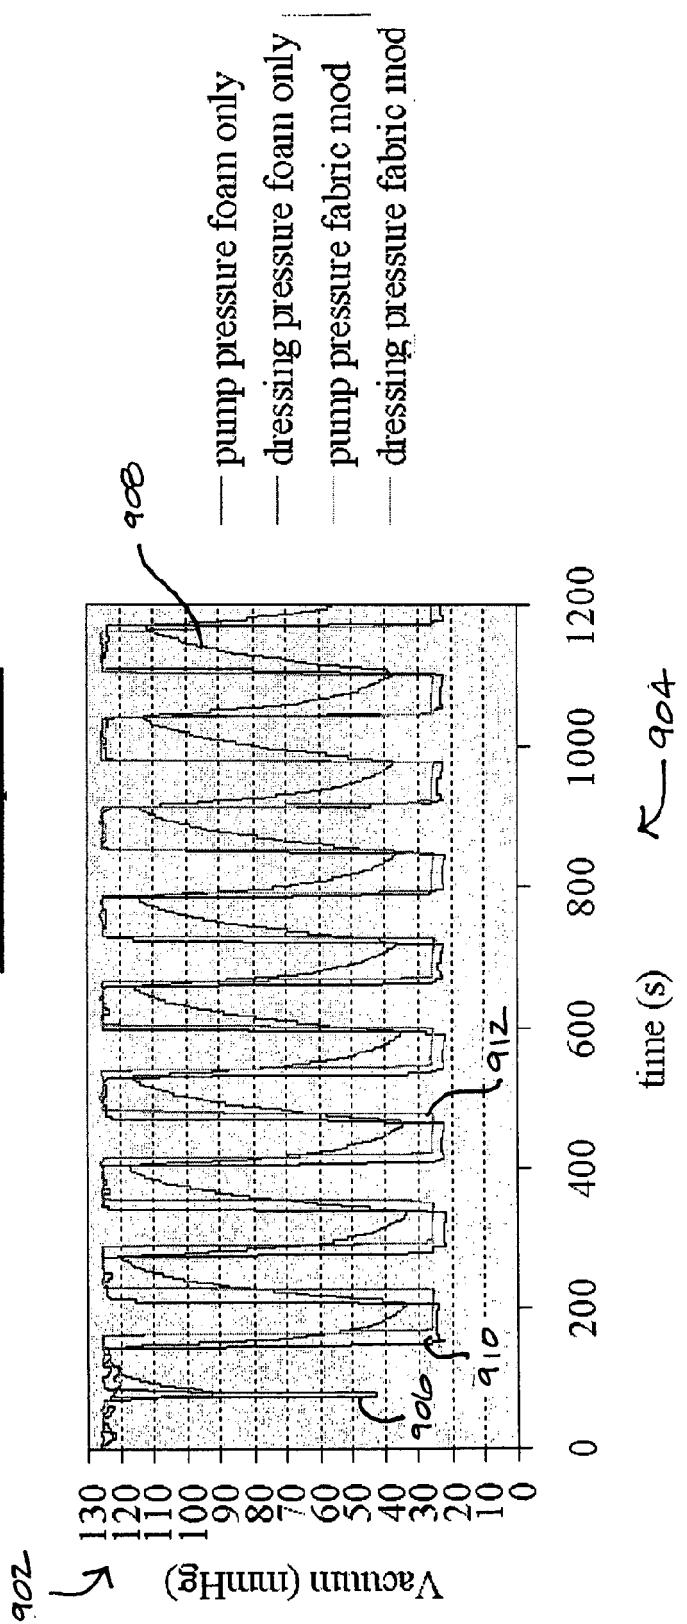


Fig. 9

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2008/001726

A. CLASSIFICATION OF SUBJECT MATTER
 IPC(8) - A61F 13/00 (2008.04)
 USPC - 602/42

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
 IPC(8) - A61F 5/00, 5/44, 13/00 (2008.04)
 USPC - 602/42

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

Patbase

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2004/0030304 A1 (HUNT et al) 12 February 2004 (12.02.2004) entire document	1-25
Y	WO 2005/123170 A1 (WATT et al) 29 December 2005 (29.12.2005) entire document	1-25

Further documents are listed in the continuation of Box C.

* Special categories of cited documents:	
"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"E" earlier application or patent but published on or after the international filing date	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"O" document referring to an oral disclosure, use, exhibition or other means	"&" document member of the same patent family
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search	Date of mailing of the international search report
28 May 2008	11 JUN 2008
Name and mailing address of the ISA/US Mail Stop PCT, Attn: ISA/US, Commissioner for Patents P.O. Box 1450, Alexandria, Virginia 22313-1450 Facsimile No. 571-273-3201	Authorized officer: Blaine R. Copenheaver PCT Helpdesk: 571-272-4300 PCT OSP: 571-272-7774