



- (51) International Patent Classification:
H01J 49/40 (2006.01)
- (21) International Application Number:
PCT/US2013/031506
- (22) International Filing Date:
14 March 2013 (14.03.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (71) Applicant: LECO CORPORATION [US/US]; 3000 Lakeview Avenue, St. Joseph, MI 49085-2319 (US).
- (72) Inventors: VERENCHIKOV, Anatoly; 20 Kavalergardskaya, Apt. 16, St. Petersburg, 193124 (RU). YAVOR, Mikhail; Aviakonstruktorov Avenue, Apt. 389, St. Petersburg, 197372 (RU).
- (74) Agents: O'BRIEN, Jonathan, P. et al.; Honigman Miller Schwartz and Cohn LLP, 350 East Michigan Avenue, Suite 300, Kalamazoo, MI 49007-3800 (US).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published: — with international search report (Art. 21(3))

(54) Title: MULTI-REFLECTING MASS SPECTROMETER

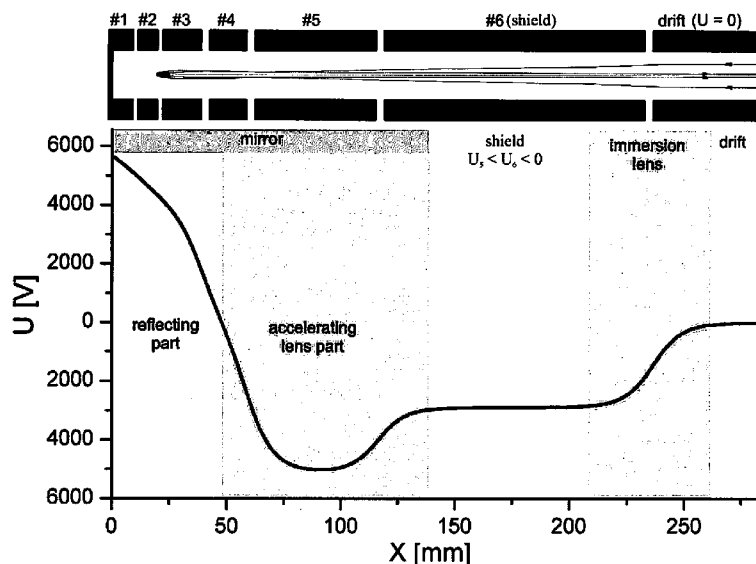


Fig. 8

(57) Abstract: To improve spatial and energy acceptance of multi-reflecting time-of-flight, open traps, and electrostatic trap analyzers, a novel ion mirror is disclosed. Incorporation of immersion lens between ion mirrors allows reaching the fifth order time per energy focusing simultaneously with the third order time per spatial focusing including energy-spatial cross terms. Preferably the analyzer has hollow cylindrical geometry for extended flight path. The time-of-flight analyzer preferably incorporates spatially modulated ion mirror field for isochronous ion focusing in the tangential direction.

WO 2014/142897 A1

MULTI-REFLECTING MASS SPECTROMETER**TECHNICAL FIELD**

5 [001] This disclosure relates to the area of mass spectroscopic analysis, multi-reflecting time-of-flight mass spectrometers and electrostatic traps and to the related apparatus, including electrostatic ion mirrors.

BACKGROUND

10 [002] Multi-reflecting mass spectrometers, either time-of-flight (MR-TOF MS), open traps, or electrostatic traps (E-trap), comprise gridless ion mirrors to arrange isochronous motion of ion packets, essentially independent of ion energy and spatial spreads.

[003] An important class of ion mirrors for multi-reflecting mass spectrometers is represented by mirrors which are substantially elongated in one transverse direction Z to form a two-dimensional electrostatic field. This field can have either planar or hollow cylindrical symmetry. SU1725289, incorporated herein by reference, introduces an MR TOF MS with ion mirrors of planar symmetry. Except Z -edges, the electrostatic field is two-dimensional $E(X,Y)$, i.e. essentially independent of the Cartesian coordinate Z . Ions move along zigzag trajectories, being injected at small angle to X -axis, periodically reflected from the mirrors in the X -direction, spatially focused in the Y -direction, and slowly drifting in the Z -direction. US7196324, GB2476964, GB2477007, WO2011086430, and co-pending application 223322-313911, incorporated herein by reference, disclose multi-reflecting analyzers with hollow cylindrical mirrors formed by two sets of coaxial ring electrodes. Contrary to planar mirrors, cylindrical mirrors eliminate Z -edges, thus forming electrostatic field completely independent on the azimuthal Z -direction. The analyzer provides a compact folding of ion path per instrument size. However, when arranging zigzag ion trajectories, the ion path deviates from a cylindrical surface, which demands for ion mirrors being highly isochronous relative to radial Y -displacements.

25 [004] Electrostatic multi-reflecting analyzers with two-dimensional ion mirrors of both - planar and hollow cylindrical geometry are disclosed for use as time-of-flight analyzers (SU1725289, US7385187), open traps (GB2478300, WO2011107836), and electrostatic traps (GB2476964, GB2477007, WO2011086430). While in time-of-flight (TOF) analyzers ion packets travel towards a fast response detector along a fixed path, in electrostatic traps, the ion packets are trapped indefinitely. They keep reflecting while being detected by image current

detector. Open electrostatic traps could be considered as a hybrid between TOF and traps. Ions reach a detector after a loosely defined number of reflections within some span in the number of reflections.

[005] Multi-reflecting time-of-flight mass spectrometers can be combined with a set of periodic lenses to confine ions in the Z -direction, as disclosed in GB2403063 and US7385187, incorporated herein by references. US2011186729, incorporated herein by reference, discloses quasi-planar ion mirrors, in which the electrostatic field of planar symmetry is superimposed with a weak field spatially periodic in the Z -direction to provide ion confinement in this direction. Such periodic field, by itself or in combination with periodic lenses, allows significant reducing of flight time distortions due to the spatial Z -spread in ion bunches. GB2476964, GB2477007, WO2011086430, incorporated by reference, disclose periodic lens in the tangential direction within cylindrical hollow analyzers.

[006] The general trend in design of multi-reflecting mass spectrometers is to minimize the effect of ion packet broadening during periodic ion motion between the mirrors in order to increase the mass resolving power of the spectrometer at given energy tolerance and phase space acceptance, i.e. acceptance of initial spatial, angular, and energy spreads of ion packets. In order to improve the energy tolerance of the mass analyzer, US4731532, incorporated herein by reference, discloses a gridless ion mirror with a purely retarding field which provides for second-order focusing of the flight time T with respect to kinetic energy K , i.e. $dT/dK = d^2T/dK^2 = 0$. Since present invention is primarily concerned with analyzer isochronicity we will be referring time-per-energy focusing as “energy focusing”. In the paper by A. Verenchikov et al., Technical Physics, v.50, N1, 2005, p.73-81, incorporated herein by references, planar ion mirrors are described with an accelerating potential at one of the mirror electrodes, which provide for third-order energy focusing, i.e. for $dT/dK = d^2T/dK^2 = d^3T/dK^3 = 0$. Co-pending application 223322-318705, incorporated herein by reference, discloses gridless ion mirrors of either planar or hollow cylindrical geometry, possessing fourth ($d^4T/dK^4=0$) and fifth ($d^5T/dK^5=0$) order energy focusing. Achieving high order of energy focusing allows increasing the energy tolerance of the mass analyzer to >10% at mass resolving power above 100,000.

[007] Since in gridless ion mirrors due to an inhomogeneous field structure ion flight time in general depends not only on ion energy but also on ion initial coordinate and direction of motion, it is important to design ion mirrors such to provide for periodic focusing of the flight time with respect to the spatial spread of ion packets. In general, for two dimensional and Z -independent fields with X -direction for ion reflections, the flight time T through the analyzer

depends on ion kinetic energy K , initial spatial coordinate Y_0 and angular coordinate b_0 ($b = dY/dX$). At small deviations of initial ion parameters the time-of-flight deviations can be represented by the Taylor expansion:

$$t = (T|\delta)\delta + (T|\delta\delta)\delta^2 + (T|\delta\delta\delta)\delta^3 + (T|\delta\delta\delta\delta)\delta^4 + (T|\delta\delta\delta\delta\delta)\delta^5 + \dots \\ + (T|yy)y_0^2 + (T|yb)y_0b_0 + (T|bb)b_0^2 \\ + (T|yy\delta)y_0^2\delta + (T|yb\delta)y_0b_0\delta + (T|bb\delta)b_0^2\delta + \dots$$

where $t = (T - T_0)/T_0$ is the relative flight time deviation, T_0 is the flight time corresponding to an ion with zero initial coordinates $Y_0 = B_0 = 0$ and with the mean kinetic energy value K_0 , $\delta = (K - K_0)/K_0$ is the relative energy deviation, and $y = Y/H$ is the coordinate normalized to the window height H of the ion mirror. The expansion (aberration) coefficients (...|...) are normalized derivatives: $(t|\delta) = dt/d\delta$, $(t|\delta\delta) = (1/2)d^2t/d\delta^2$ etc. N -th order energy focusing means that all coefficients at the pure powers of δ up to N -th power inclusively are zeroes. The second order spatial focusing (i.e. time-of-flight focusing with respect to spatial and energy spreads) means that $(t|yy) = (t|yb) = (t|bb) = 0$, because the mixed second order terms $(t|y\delta)$ and $(t|b\delta)$ vanish due to the system symmetry with respect to the plane $Y = 0$.

[008] The paper by M. Yavor et al., Physics Procedia, v.1 N1, 2008, p.391-400, incorporated herein by reference, provides details of geometry and potentials for planar ion mirrors which simultaneously provide the third order energy focusing, second order spatial focusing and geometrical focusing in Y -direction. In such analyzers, the broadening of ion packets in the mirror fields is dominated by so-called "mixed" third order aberrations due to both spatial and energy spreads, i.e. terms $(t|yy\delta)y_0^2\delta$, $(t|yb\delta)y_0b_0\delta$ and $(t|bb\delta)b_0^2\delta$, because the rest third order aberrations vanish due to the system symmetry with respect to the plane $Y = 0$. These terms are responsible for deterioration of the resolving power of multi-reflection mass spectrometers at both FWHM level and even more severely at the 10% peak height level. This deterioration is especially noticeable in hollow cylindrical analyzers in which ions are periodically shifted in radial Y -direction from the "ideal" cylindrical surface of ion motion, as well as in planar mass analyzers with periodic lenses, in which ions are injected with a large enough Y -spread through a "double orthogonal" accelerator described in US2007176090, incorporated herein by reference.

[009] As described in the co-pending application 223322-318705, incorporated herein by reference, the order of energy focusing can be increased by optimizing the electrostatic potential distribution in the region of ion reflection. The improvement is reached by increasing the number of mirror electrodes with different electrode potentials and choosing sufficiently thin

electrodes in the region of ion reflection. This strategy of design, however, fails in case one wants to achieve high order energy focusing simultaneously with high order spatial focusing. Up to fifth-order energy focusing may be achieved in combination with the second-order spatial focusing. To obtain third-order energy focusing in combination with the third-order spatial focusing one has to increase the width of the mirror electrode with accelerating potential, though such geometry modification causes a negative consequence of reducing the spatial acceptance of the ion mirror. However, our own thorough numerical simulations of gridless ion mirrors show that no straightforward steps like increasing the number of mirror electrodes, splitting them into parts with introducing more independent electrode voltages, varying their widths and shapes and other similar means do not lead to elimination of the mixed (energy-spatial) third order aberrations in ion mirrors with the fourth and higher order of energy focusing. Using the above mentioned optimization procedures one can reach high-order energy isochronicity, however, at a cost of increasing mixed third order aberrations. In other words, increasing the energy acceptance leads to reduction of the spatial acceptance.

[010] Thus, prior art ion mirrors possess either high energy acceptance or high spatial acceptance but not both at the same time. Therefore, there is a need for improving the spatial phase space acceptance of ion mirrors possessing high energy tolerance, i.e. flight time focusing with respect to energy of fourth and higher orders.

SUMMARY

[011] The inventors have realized that the spatial acceptance of planar time-of-flight mass analyzers can be increased while maintaining high order time per energy focusing by adding a planar lens between prior art ion mirrors, which may include the following:

- (a) said mirrors have accelerating and reflecting electrostatic field regions;
- (b) said planar lens focuses ions in the same *Y*-direction as the mirrors do;
- (c) the lens pre-focuses ions to the region of the retarding mirror field;
- (d) the mirror and lens fields are separated by a field-free space; and
- (e) said lens is immersion, that is, ions are accelerated by the lens in the direction towards the mirror and decelerated on the way back. This also means that ions pass the field-free space between the lens and the mirror at an increased energy as compared to ion energy outside the “mirror plus lens” pair.

[012] Therefore, in the invented configuration there are in general two lens regions formed in each mirror-lens combination: the pre-focusing lens and the “internal” lens formed by the accelerating electrode of ion mirror. So, on the way to the ion mirror ions are accelerated twice:

first, by the pre-focusing lens and then by the field of the mirror accelerating electrode. After passing the latter field ions are reflected by the retarding field of the mirror.

[013] The reduction of the flight time aberrations due to spatial ion spreads in *Y*-direction by providing means of shrinking *Y*-widths of ion bunches inside the mirror reflecting field could be expected by those experienced in the art. It is important to emphasize, however, that the pre-focusing lens itself introduces additional aberrations, and numerous calculations show that the positive effect of focusing is modest and expectations are not met if using just an arbitrary pre-focusing lens. The principal and unobvious point of the invention is that an efficient reduction of mixed third order aberrations in the mirror-lens combinations occurs only in case when the pre-focusing lens is immersion (accelerating ions on the way to the mirror). Though inventors do not know a strict mathematical proof, thorough numerical simulation of various mirror-lens combinations confirm this conclusion.

[014] In an embodiment, there is provided isochronous time-of-flight or electrostatic trap analyzer comprising:

(a) Two parallel and aligned grid-free ion mirrors separated by a field free region, said mirrors being arranged to reflect ions in a first *X*-direction, said mirrors being substantially elongated in the transverse drift *Z*-direction to form a two-dimensional electrostatic field either of planar symmetry or of a hollow cylindrical symmetry;

(b) Said mirrors having at least one electrode with an accelerating potential compared to the field-free space potential, arranged to geometrically focus ions in the *Y*-direction; and

(c) At least one planar electrostatic lens, arranged to geometrically focus ions in the *Y*-direction, said lens being elongated in said transverse *Z*-direction and placed between said ion mirrors.

[015] Preferably, said lenses are immersion. In an implementation, said mirrors are preferably symmetric with respect to the median plane $X=0$ of the analyzer. In an implementation, there are preferably two said planar lenses, identical and located symmetric with respect to the median plane of the analyzer, one at each side of said median plane. In this case, three field-free regions are formed: one between said pre-focusing lenses and two between said lens and said mirror. In an implementation, said two field free regions between lens and ion mirror have higher accelerating potential as compared to the field free region between said lenses.

[016] In an implementation, a single pre-focusing lens field can be superimposed with the fields of periodic lenses placed between ion mirrors and arranged for confining ions in the drift

Z-direction. In this case, instead of planar lenses, the array of periodic lenses is composed of lenses with 3D field, focusing ions in both transversal directions Y and Z .

[017] In an implementation, electrostatic field of one or both mirrors of planar or hollow cylindrical symmetry can be superimposed with a weak field being periodic in the direction Z of elongation of the mirrors to provide ion confinement in the Z -direction. Preferably, said spatially modulated electrostatic field by itself or in combination with a periodic lens is such that it eliminates time per spatial aberrations in the Z -direction.

BRIEF DESCRIPTION OF THE DRAWINGS

[018] Various embodiments of the present invention together with arrangement given illustrative purposes only will now be described, by way of example only, and with reference to the accompanying drawings in which:

[019] Fig.1 depicts a four-electrode planar ion mirror of prior art (MPA-1) with the third order energy focusing, the second order spatial focusing, and compensated second order mixed aberrations. Sample ion trajectories and electrostatic potential $U(X)$ distribution in the middle plane ($Y = 0$) are drawn for mean kinetic ion energy per charge ratio $K_0/Q = 4500$ V.

[020] Fig. 2 shows typical flight time broadening in prior art ion mirrors MPA-1 of Fig.1 as a function of ion energy in case of finite energy K - and spatial Y -spreads of ion bunches.

[021] Fig. 3 depicts an ion mirror of prior art (MPA-2) capable of reaching the fifth order energy focusing. The electrostatic potential $U(X, Y=0)$ distributions for $K_0/Q = 4500$ V are presented for three tuning modes MPA-2-3, MPA-2-4 and MPA-2-5, corresponding to the third, fourth and fifth-order energy focusing. Between tuning modes, lower order energy-focusing allows better compensation of spatial and mixed term aberrations.

[022] Fig. 4 plots ion flight time Vs ion energy at $Y = 0$ for prior art ion mirrors MPA-2 of Fig. 3 at three above mentioned tuning modes.

[023] Fig. 5 shows typical flight time broadening as a function of ion energy at finite ionic Y -spatial spread in MPA-2 mirror at the MPA-2-3 tuning mode providing 3rd order energy focusing.

[024] Fig. 6 shows typical flight time broadening as a function of ion energy at finite ionic Y -spatial spread in MPA-2 mirror at the MPA-2-4 tuning mode providing 4th order energy focusing.

[025] Fig. 7 shows typical flight time broadening as a function of ion energy at finite ionic Y -spatial spread in MPA-2 mirror at the MPA-2-5 tuning mode providing 5th order energy focusing.

[026] **Fig. 8** depicts an ion mirror-lens combination (ML-1) of the present invention. The fourth order energy focusing is reached simultaneously with much smaller (compared to MPA-1 and MPA-2) mixed third order aberrations. Sample ion trajectories and electrostatic potential $U(X, Y=0)$ distribution corresponds to $K_0/Q=4500$ V.

[027] **Fig. 9** shows typical flight time broadening as a function of ion energy at finite ionic Y -spatial spread in mirror-lens combination ML-1 of Fig. 8, tuned to compensate first trough fourth energy derivatives ($dT/dK = d^2T/dK^2 = d^3T/dK^3 = d^4T/dK^4 = 0$).

[028] **Fig. 10** shows typical flight time broadening as a function of ion energy at finite ionic Y -spatial spread in mirror-lens combination ML-1, at an alternative analyzer tuning corresponding to non-zero but partly mutually compensating first and third energy derivatives ($d^2T/dK^2 = d^4T/dK^4 = 0$, $dT/dK \neq 0$, $d^3T/dK^3 \neq 0$) to minimize the overall time broadening.

[029] **Fig. 11** depicts an ion mirror-lens combination (ML-2) of the present invention providing the fifth-order energy focusing and simultaneously eliminating mixed third order aberrations. Electrostatic potential $U(X, Y=0)$ distribution are drawn for $K_0/Q=4500$ V.

[030] **Fig. 12** shows typical flight time broadening as a function of ion energy at finite ionic Y -spatial spread in mirror-lens combination ML-2 of Fig. 11.

[031] **Fig. 13** presents a comparison of peak shapes for mass analyzers with different ion mirrors:

- A – “ideal” analyzer possessing no time-of-flight aberrations;
- B – mass analyzer with the mirrors MPA-1;
- C – mass analyzer with the mirrors MPA-2 in the 3rd order focusing mode MPA-2-3;
- D – mass analyzer with the mirrors MPA-2 in the 5th order focusing mode MPA-2-5;
- E – mass analyzer with the mirror-lens combinations ML-2.

Peak shapes are calculated at time focus positions. Analyzers are scaled such that to maintain the same flight time T_0 . In all cases ion packets have the same relative initial spreads: Gaussian energy distribution at $\sigma_K = 0.011K_0$, uniform Y -distribution at full height of $2Y_0 = 0.133H$, and Gaussian distribution of ion start times, corresponding to the mass resolving power of $R_m = T_0 / (2\Delta T_i) = 300\,000$ at FWHM.

[032] **Fig. 14** presents a block schematic view of mirror-lens combinations of the present invention.

DETAILED DESCRIPTION

[033] As disclosed in GB2403063 and US7385187, incorporated herein by references, a multi-reflecting time-of-flight analyzer of prior art comprises two ion mirrors, elongated in a drift Z -direction, turned face-to-face and separated by a drift space. The ion packets move along zigzag trajectories, being periodically reflected in the X -direction between the mirrors. Zigzag trajectories are arranged by injecting ions at small angle to the X -axis and by spatial ion confinement in a periodic lens.

[034] Referring to Fig. 1, a planar mirror of US7385187 (MPA-1) is shown at XY plane which is orthogonal to the Z -direction of mirror elongation. The electrostatic field is formed by applying voltages to four electrodes (#1 – #4). The distance between outer cap electrodes (electrodes #1) is $2X_0$. The Table 1 presents electrode X -widths L , normalized to the Y -height H of the mirror window, so as electrode potentials normalized to K_0/Q , where Q is the ion charge and K_0 is the mean ion kinetic energy in field-free space. The electrostatic potentials are retarding at the electrodes #1 and #2, nearly drift potential at the electrode #3, and accelerating at the electrode #4 (see Table 1). Though prior art analyzers operate at floated drift space, for simulation purposes the drift potential is set to zero ($U = 0$ in Fig. 1) and mirror potentials are shifted by K_0/Q , i.e. experimentally used normalized potentials are less by 1 as compared to simulated ones.

[035] Table 1: Geometry and electrode potentials for the prior art mirror MPA-1

Electrode	#1	#2	#3	#4
Normalized width, L/H	0.917	0.917	0.917	0.917
Normalized potential, UQ/K_0	1.361	0.969	-0.139	-1.898

[036] Again referring to Fig. 1, axial electrostatic potential distribution $U(X, Y=0)$ for MPA-1 shows that the mirror field consists of two regions – the region of accelerating field ($U < 0$ for positive ions) and the region of the reflecting field ($U > 0$ for positive ions) for a particular ion mirror with $X_0 = 308$ mm and $H = 30$ mm. The region of the accelerating field performs a geometrical ion focusing in the Y -direction, as seen from sample ion trajectories. The focusing strength is tuned by adjusting potential #4 such that parallel ion beam entering the mirror is focused such that it returns into a point (in paraxial approximation) at the middle plane of the analyzer. Such geometrical focusing provides transformation of an ion trajectory to itself after four mirror reflections. The ion-optical and isochronous properties of the time-of-flight analyzers with MPA-1 mirrors, have been described in detail, e.g. in the paper by M. Yavor et al., Physics Procedia, v.1 N1, 2008, p.391-400, incorporated herein by reference. The proper

tuning of the mirrors simultaneously provides the following properties at the middle plane of the analyzer: the above mentioned geometric focusing in the Y-direction; the third order energy focusing $(t|\delta) = (t|\delta\delta) = (t|\delta\delta\delta) = 0$ after each ion reflection; and second order spatial focusing $(t|y) = (t|b) = (t|y\delta) = (t|b\delta) = (t|yy) = (t|yb) = (t|bb) = 0$ after two mirror reflections.

[037] Referring to Fig. 2, a simulated plot of ion distribution in the normalized time-energy plane is shown at a time focal plane (located at the middle plane of the analyzer) after even number of mirror reflections in MPA-1 analyzer of Fig. 1. Initial ion bunch has Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform Y-distribution at full height of $2Y_0 = 0.133H$. The plot characterizes maximal $\Delta T/T_0 \sim 2.5 \times 10^{-5}$ ion bunch broadening due to analyzer aberrations. The points corresponding to individual “probe” ions are mostly enclosed between two curves: $(T - T_0)/T_0 = (t|\delta\delta\delta\delta)\delta^4$ and $(T - T_0)/T_0 = (t|\delta\delta\delta\delta)\delta^4 + (t|yy\delta)y_0^2\delta$, composed of energy and third order mixed aberrations. With good accuracy, the aberrations $(t|\delta\delta\delta\delta)\delta^4$ and $(t|yy\delta)y_0^2\delta$ dominate in broadening of time-of-flight peaks. The values of the corresponding and some higher (5th and 6th) order energy aberration coefficients are presented in Table 2.

[038] **Table 2.** Aberration coefficients of the mass analyzer with the mirrors MPA-1

Aberration coefficient	Value
$(t \delta\delta\delta\delta)$	11.5
$(t \delta\delta\delta\delta\delta)$	8.50
$(t \delta\delta\delta\delta\delta\delta)$	-115.3
$(t yy\delta)$	0.0727

[039] Based on aberration coefficient values one can calculate magnitudes of time spread induced by aberrations for given values of energy and coordinate spreads. For example, let the total flight time be $T_0 = 1$ ms and consider an ion bunch of Fig.2 with Gaussian energy distribution at $\sigma_K = 0.011$ and with the uniform coordinate spread of $Y_0/H = \pm 0.067$. Then, about 95% ions deviate from the mean energy by less than $\delta = 2\sigma_K = \pm 0.022$, i.e. stay within the total energy spread of 4.4%. Due to the fourth order aberration $(t|\delta\delta\delta\delta)\delta^4$ the maximum deviation of the normalized flight time equals $11.5 \cdot 0.022^4 \approx 2.6E-6$ and the absolute time spread is 2.6 ns. Similarly, the 5th order aberration $(t|\delta\delta\delta\delta\delta)\delta^5$ contributes $8.5 \cdot 2 \cdot 0.022^5 \approx 9E-8$, corresponding to 0.09 ns. Additional factor of 2 appears since deviations of opposite signs are summed for odd

order aberrations. The coordinate spread contributes to the flight time spread mainly due to the mixed aberration $(t|yy\delta)y_0^2\delta$ as $0.0727*0.067^2*2*0.022 \approx 1.4E-5$ and absolute value 14 ns.

[040] Referring to Fig. 3, another ion mirror of prior art (MPA-2) is shown, wherein the corresponding time-of-flight mass analyzer is composed of two such mirrors, placed face-to-face and separated by a drift space. The mirror is described in a co-pending application 223322-318705, incorporated herein by reference. The mirror provides for the fifth order energy focusing $(t|\delta) = (t|\delta\delta) = (t|\delta\delta\delta) = (t|\delta\delta\delta\delta) = (t|\delta\delta\delta\delta\delta) = 0$. To this goal, the mirror cap is separated from the electrode #1 and forms a separate electrode #0, retarding voltages are applied to the electrodes #1, #2 and #3, the field-free potential ($U = 0$ in Fig. 3) is applied to the electrode #4, and an accelerating potential is applied to the electrode #5. The mirror sizes and the electric tuning of the mirror electrodes in the fifth order energy focusing mode (MPA-2-5) are presented in Table 3, in which the cap-to-cap separation is $2X_0 = 908$ mm and the height of the mirror window is $H = 30$ mm.

[041] **Table 3.** Geometry and electrode potentials for the prior art mirror MPA-2

Electrode		#0	#1	#2	#3	#4	#5
Normalized width, L/H		–	0.433	0.484	0.933	0.883	3.342
Normalized potential, UQ/K_0	5 order energy focusing (MPA-2-5)	1.222	1.387	1.059	0.919	0	–0.977
	4 order energy focusing (MPA-2-4)	1.539	1.116		0.943	0	–1.009
	3 order energy focusing (MPA-2-3)	1.267			0.981	0	–1.046

[042] By electrically connecting adjacent electrodes, the number of independently adjusted voltages can be reduced, and the mirror MPA-2 can be tuned such that the order of energy focusing can be decreased to the fourth one $(t|\delta) = (t|\delta\delta) = (t|\delta\delta\delta) = (t|\delta\delta\delta\delta) = 0$ (mode MPA-2-4) or to the third one $(t|\delta) = (t|\delta\delta) = (t|\delta\delta\delta) = 0$ (mode MPA-2-3). The corresponding modes of electric tuning are shown in Table 3 and the potential distributions $U(X, Y=0)$ are shown in Fig. 3.

[043] Referring to Table 4, in our own simulations we found that sacrificing the energy focusing allows simultaneous reduction of the mixed third order aberrations. As an example, the geometry and potentials of mirror MPA-2 are optimized such that in the third order energy focusing mode MPA-2-3 there are reached: second order spatial focusing $(t|y) = (t|b) = (t|yy) = (t|yb) = (t|bb) = 0$; and mixed third order aberrations are eliminated:

$(t | yy\delta) = (t | yb\delta) = (t | bb\delta) = 0$. This means the full third order focusing of the flight time, because all the remaining third order aberration coefficients in the analyzer vanish automatically because of the system symmetry with respect to the $Y = 0$ plane. The dominating non-vanishing aberration in this case remains the fourth order aberration $(t | \delta\delta\delta\delta)\delta^4$.

[044] **Table 4.** Aberration coefficients of the mass analyzer with the mirrors MPA-2

Aberration coefficient	Value		
	5 order energy focusing (MPA-2-5)	4 order energy focusing (MPA-2-4)	3 order energy focusing (MPA-2-3)
$(t \delta\delta\delta\delta)$	0	0	26.0
$(t \delta\delta\delta\delta\delta)$	0	-118.0	42.7
$(t \delta\delta\delta\delta\delta\delta)$	646.2	-186.8	-437.6
$(t yy\delta)$	0.0270	0.0165	0

[045] Referring to Fig.4, the dependencies of the flight time on ion energy are plotted in the three above discussed modes. These dependencies show that if the mixed third order aberrations could be neglected, increasing the order of energy focusing would lead to significant reduction of the time peak broadening. For an exemplar 7 % energy spread, proceeding from the third to fourth and then to fifth order energy focusing drops the time spread 3 and 30 times correspondingly. However, as shown in Table 4, increasing the energy focusing order causes growth of the third order mixed aberration $(t | yy\delta)$, which reduces improvement of the overall time peak broadening and thus limits the energy tolerance of the analyzer.

[046] Referring to Fig. 5, a plot of the flight time distribution in the time-energy plane is shown at a time focal plane after an even number of ion reflections by mirrors MPA-2 of Fig. 3, tuned to the third order energy focusing mode MPA-2-3, also providing complete third order focusing. Initial ion bunch has Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform Y -distribution at full height of $2Y_0 = 0.133H$, same as used for plotting Fig. 2. Due to elimination of the mixed third order aberrations, the points at the plot approximately follow the curve $(T - T_0)/T_0 = (t | \delta\delta\delta\delta)\delta^4$, which means that the fourth order aberration $(t | \delta\delta\delta\delta)\delta^4$ dominates in flight time broadening. Comparing Tables 2 and 4, the mirror MPA-2 in the MPA-2-3 tuning mode has more than twice larger aberration coefficient $(t | \delta\delta\delta\delta)$ as compared to the mirror MPA-1, which again reflects the general trend: energy aberrations increase when tuning for lower third order mixed aberrations. Comparing Fig. 2 and Fig. 5, the time broadening is somewhat higher in Fig. 5 in spite of formally higher order overall focusing.

[047] Referring to Fig. 6, a plot of the flight time distribution in the time-energy plane is shown at a time focal plane after an even number of ion reflections by mirrors MPA-2 of Fig. 3, tuned to the fourth order energy focusing mode MPA-2-4. Initial ion bunch has Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform Y -distribution at full height of $2Y_0 = 0.133H$, same as used for plotting Fig. 2 and Fig. 5. The plot evidently demonstrates some contribution of the non-vanishing aberration $(t|yy\delta)y_0^2\delta$. Similarly to Fig. 2, the points corresponding to individual ions are mostly enclosed between two curves: symmetric and tilted curves corresponding to $(T-T_0)/T_0 = (t|\delta\delta\delta\delta\delta)\delta^5$ and $(T-T_0)/T_0 = (t|\delta\delta\delta\delta\delta)\delta^5 + (t|yy\delta)y_0^2\delta$. As seen from the plot, the $(t|\delta\delta\delta\delta\delta)\delta^5$ aberration dominates over $(t|yy\delta)y_0^2\delta$ aberration (subject to initial δ - and y -spreads). Thus, fourth order energy focusing allows 3 times smaller time spread compared to the third order energy focusing, being consistent with the plot of Fig. 4.

[048] Referring to Fig. 7, a plot of the flight time distribution in the time-energy plane is shown at a time focal plane after an even number of ion reflections by the mirrors MPA-2 of Fig. 3, tuned to the fifth order energy focusing mode MPA-2-5. Initial ion bunch has Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform Y -distribution at full height of $2Y_0 = 0.133H$, same as used for plotting Fig. 2, Fig.5 and Fig.6. Similarly to Fig. 6, in Fig.7 the points corresponding to individual ions are enclosed between two curves: symmetric and tilted curves corresponding to $(T-T_0)/T_0 = (t|\delta\delta\delta\delta\delta\delta)\delta^6$ and $(T-T_0)/T_0 = (t|\delta\delta\delta\delta\delta\delta)\delta^6 + (t|yy\delta)y_0^2\delta$. However (unlike in Fig. 6), the contribution of the non-vanishing aberration $(t|yy\delta)y_0^2\delta$ becomes absolutely dominating. Switching between MPA-2-4 and MPA-2-5 modes improves time spread 1.5 times only, instead of ten-fold predicted by Fig. 4.

[049] Therefore, in “typical” prior art ion mirrors consisting of two regions with reflecting and accelerating fields, improvement of time per energy focusing has limited effect on the resolving power and on the energy tolerance because of the inevitable and dominating third order mixed aberrations.

[050] Mirror-lens combinations of present invention

[051] Referring to Fig. 8, a combination of a planar mirror and of a planar lens is shown in the XY -plane and denoted as ML-1. Both the ion mirror and the planar lens are substantially elongated in the Z -direction such that to form substantially two dimensional electrostatic fields in the XY -plane orthogonal to the Z -direction. A multi-reflecting time-of-flight analyzer comprises two such mirror-lens combinations, turned face-to-face and separated by a field-free drift space. For simulation purposes, drift potential is set to zero $U_D = 0$. The mirror electrostatic field is formed by electrodes #1 to #5. Retarding voltages are applied to electrodes

#1, #2 and #3, thus forming the reflecting mirror field. The electrode #4 is at drift potential ($U_4 = U_D = 0$). The highest accelerating voltage is applied to the electrode #5 for geometric ion focusing ($U_5 < U_6$ for positive ions). The electrode #6 plays a role of the field-free shield for the mirror. This electrode is long enough such a field-free region of electrode #6 separates the mirror from the pre-focusing lens formed by applying $U_6 < U_D$ (for positive ions). The potential at the electrode #6 is biased lower than the drift potential $U_D = 0$, such that to form an immersion lens between the shield electrode #6 and the drift at the potential $U = 0$. Such immersion lens accelerates ions moving towards the mirror. The sample ion trajectories shown in Fig. 8 demonstrate that on the way to the mirror ions are geometrically focused first by the immersion lens and then additionally by the lens formed in the accelerating field region of the ion mirror. The electrode widths and options of electric tuning are presented in Table 5. For the particular mirror-lens combination ML-1, the cap-to cap distance is $2X_0 = 836$ mm and the height of the mirror window is $H = 24$ mm.

[052] **Table 5.** Geometry and electrode potentials for the mirror-lens combination ML-1

Electrode		#1	#2	#3	#4	#5	#6
Normalized width, L/H		0.375	0.350	0.750	0.750	2.333	4.958
Normalized potential, UQ/K_0	$(t \delta)=(t \delta\delta)=(t \delta\delta\delta)=(t \delta\delta\delta\delta)=0$	1.296	1.077	0.924	0	-1.155	-0.639
	$(t \delta)\neq 0, (t \delta\delta\delta)\neq 0$	1.293	1.076	0.924	0	-1.152	-0.638

[053] The mirror-lens combination ML-1 is designed such that the fourth order energy focusing $(t|\delta)=(t|\delta\delta)=(t|\delta\delta\delta)=(t|\delta\delta\delta\delta)=0$ is achieved together with negligibly small third order mixed aberrations, thus reaching the object of the invention.

[054] Referring to Fig. 9, a plot of the flight time distribution in the time-energy plane is shown at a time focal plane (located in the middle plane of the analyzer) after an even number of ion reflections from the mirror ML-1 of Fig. 8, for a bunch of ions with the same relative energy and Y -coordinate initial spreads as used for plotting Figs. 2, 5-7 (Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform Y -distribution at full height of $2Y_0 = 0.133H$). The third order mixed aberration is nearly cancelled and the fifth order aberration $(t|\delta\delta\delta\delta\delta)\delta^5$ becomes dominating. As a result, the amplitude of flight time broadening becomes 3 times smaller compared to prior art analyzer with the fourth order energy focusing MPA-2-4 in Fig. 6.

[055] Referring to Fig. 10, a plot of the flight time distribution in the time-energy plane is shown at a time focal plane after an even number of ion reflections by the mirror ML-1, for a bunch of ions with the same energy and Y -coordinate initial spreads as used for plotting Figs. 9,

but in case of a slightly different electric tune. With this “shifted” tune, the first and third order aberration coefficients $(t|\delta)$ and $(t|\delta\delta\delta)$ are not eliminated completely but tuned to some small values such that the amplitude of the flight time broadening is minimized for given energy spread. One possible option for such tune is to represent the dependence $t(\delta)$ by a fifth order Chebychev polynomial. For the plots of Figs. 9 and 10, the corresponding electric tunes are presented in Table 5 and the values of relevant aberration coefficients are shown in Table 6. Comparing Fig. 9 and Fig. 10, the amplitude of the flight time broadening is twice smaller in the “shifted” tune.

[056] Table 6. Relevant aberration coefficients for two tunes of the mirror-lens combination ML-1

Aberration coefficient	Value	
	$(t \delta)=(t \delta\delta)=$ $(t \delta\delta\delta)=(t \delta\delta\delta\delta)=0$	$(t \delta)\neq 0, (t \delta\delta\delta)\neq 0$
$(t \delta)$	0	-1.3×10^{-5}
$(t \delta\delta)$	0	0
$(t \delta\delta\delta)$	0	0.051
$(t \delta\delta\delta\delta)$	0	0
$(t \delta\delta\delta\delta\delta)$	-37.1	-37.1
$(t \delta\delta\delta\delta\delta\delta)$	251.1	259.1
$(t \gamma\gamma\delta)$	0.00297	0.00270

[057] Referring to Fig. 11, yet another geometry (ML-2) of a planar mirror combined with a planar lens is shown. In this combination, the separation distance from the mirror and the lens is considerably increased as compared to the geometry ML-1 (electrode #6 width normalized by the window height H is 8.10 in ML-2 as compared to 4.96 in ML-1), which allowed eliminating of third order mixed aberrations simultaneously with the fifth order energy focusing. The widths of all electrodes and the mode of electric tuning are given in Table 7. The absolute values of the cap-to-cap distance and of the mirror window height are $2X_0 = 1080$ mm and $H = 30$ mm.

[058] Table 7. Geometry and electrode potentials for the mirror-lens combination ML-2

Electrode	#1	#2	#3	#4	#5	#6
Normalized width, L/H	0.458	0.423	0.82	0.917	0.917	8.100
Normalized potential, UQ/K_0	1.265	1.054	0.918	0	-1.313	-0.581

[059] Referring to Fig. 12, a plot of the flight time distribution in the time-energy plane is shown at a time focal plane after an even number of ion reflections by the mirror ML-2 of Fig. 11, for a bunch of ions with the same energy and *Y*-coordinate initial spreads as used for plotting Figs. 2, 5-7, 9 and 10 (Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform *Y*-distribution at full height of $2Y_0 = 0.133H$). As clearly seen the object of the invention is reached, i.e. normalized time spread amplitude is reduced down to $\Delta T/T_0 < 10^{-6}$. The amplitude of the flight time broadening became almost an order of magnitude smaller than in the prior art analyzer with the fifth order energy focusing mirror at MPA-2-5 tuning mode in (Fig. 7). As shown in Table 8, after eliminating the third order spatial aberration, third order mixed aberrations together with the fifth order energy aberrations, the time spread becomes dominated by higher order aberrations – the sixth order aberration $(t|\delta\delta\delta\delta\delta\delta)\delta^6$ and fourth order spatial aberrations.

[060] **Table 8.** Relevant aberrations of the analyzer with the mirror-lens combination ML-2

Aberration coefficient	Value
$(t \delta\delta\delta\delta)$	0
$(t \delta\delta\delta\delta\delta)$	0
$(t \delta\delta\delta\delta\delta\delta)$	466.0
$(t y\gamma\delta)$	0
$(t y\gamma\gamma\gamma)$	0.00408
$(t y\gamma\delta\delta)$	0.13

[061] Referring to Fig. 13, influence of flight time aberrations on the shape of time-of-flight peaks is compared for different ion mirror designs. The peaks are simulated assuming initial time spread ΔT_i (usually defined by turn-around time in the ion source) with Gaussian distribution corresponding to mass resolving power $R_m = T_0 / (2\Delta T_i) = 300\,000$ at FWHM at the absence of flight time aberrations in the analyzer. The initial energy and spatial spreads in ion bunches are the same as used for plotting Figs. 2, 5-7, 9, 10 and 12 (Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform *Y*-distribution at full height of $2Y_0 = 0.133H$). The horizontal scale is equal in all plots. Fig. 13-A shows the peak shape for an “ideal” analyzer possessing no time-of-flight aberrations (i.e. the mass peak shape is the same one as at the analyzer entrance). Fig. 13-B shows the peak shape for the MPA-1 prior art mass analyzer, possessing the third order energy focusing and the second-order spatial focusing. Ion mirror aberrations in this case contribute to both FWHM peak width and to the long peak tails. Fig. 13-C shows the peak

shape for the MPA-2 prior art mass analyzer in the 3rd order full focusing mode MPA-2-3. Elimination of the third order mixed aberrations in this case reduces the FWHM peak width practically to the width of the “ideal” peak, but the fourth order energy aberration contributes to a very long tail on the right peak side. Fig. 13-D shows the peak shape for the MPA-2 prior art mass analyzer in the fifth order energy focusing mode MPA-2-5. As compared to Fig. 13-C, the long tail due to the energy spread disappears, but the non-vanishing third order mixed aberration still deteriorates the mass resolving power at small peak height. Finally, Fig. 13-E shows the peak shape in the mass analyzer with the mirror-lens combinations ML-2 of the present invention. In this analyzer, for given energy and spatial ion spreads the contribution of flight time aberrations is negligible and the peak shape is practically the “ideal” one.

[062] Thus, the novel mirror-immersion lens combination allows reaching a super-high level of the mass resolving power in multi-reflecting time-of-flight analyzer both at FWHM and at low peak height levels, which has not been possible using prior art designs of gridless ion mirrors, which demonstrates reaching the goal of the invention.

[063] Alternative and supplementary designs

[064] Referring to Fig.14, several geometric configurations 1 to 3 of the TOF analyzer of the present invention are shown at the level of block schematics. Basic symmetric configuration 1 employs mirror-lens combinations of Figs. 8 and 11. The configuration 1 comprises two ion mirrors, each including a reflecting part 11 and the accelerating lens part 12, and two immersion lenses 13. Each lens 13 is separated from the corresponding accelerating mirror part 12 by a shield 14 creating a field-free space with the potential U_S different from the drift potential U_D in the space 15 between the immersion lenses 13. Another analyzer configuration 2 employs only one immersion lens 13, so that the analyzer comprises one ion mirror and one mirror-lens combination. Yet another analyzer configuration 3 employs one lens 16 such that the potentials U_D at both sides of this lens are equal. In a sense the configuration 3 may be considered as a configuration 1 with a zero drift space length.

[065] Again referring to Fig.14, mirror-lens combinations can be further combined with an array of planar lenses as disclosed for a planar MR-TOF MS in GB2403063 and US5017780 by the authors, incorporated herein by references. In configuration 4 a periodic lens 17 focuses ions in the Z-direction. The lens 17 is located in the space 15 with the drift potential U_D . Note, that the periodic lens focuses ions in the direction which is perpendicular to the Y-direction of focusing by immersion lenses and by ion mirrors. In another configuration 5, electrostatic fields are superimposed for the planar lens 16 (focusing ions in Y-direction) and for periodic lens 17

(focusing ions in the Z-direction). Such superposition can form periodic lenses with 3D field, focusing ions in both transversal directions *Y* and *Z*.

[066] In yet another embodiment (not shown), electrostatic field of one or both mirrors can be superimposed with a weak field being periodic in the Z-direction (direction of mirror elongation). Such spatial (not time) modulation of the ion mirror field in the Z-direction provides for ion confinement in the Z-direction as disclosed in US2011186729 by the authors, incorporated herein by reference. In another embodiment, such spatial periodic modulation of the ion mirror field is combined with the above described focusing by a periodic lens or by a spatially Z-modulated immersion lens, such that a combined Z-focusing allows mutual cancellation of major time-of-flight aberrations related to ion packet width in the Z-direction. The improved isochronicity of spatial focusing in the Z-direction is expected based on the analogy with the presently described spatial and time-of-flight focusing in the *Y*-direction.

[067] The novel mirror-immersion lens combination substantially reduces analyzer aberrations. The above described isochronous geometrical focusing in the Z-direction is expected to further decrease the analyzer aberrations. Then the initial turn-around time is expected to define peak width. This makes practical the further extension of the flight path. In another embodiment, a mirror-lens combination may be implemented in a hollow cylindrical mass analyzer which provides an efficient trajectory folding relative to the analyzer size, as disclosed in co-pending applications US7196324, GB2476964, GB2477007, WO2011086430, and co-pending application 223322-313911 by the authors, incorporated herein by references. In this case, electrodes of the mirror-lens combination have a small (compared to the mirror window height) curvature in the drift direction *Z*. Combining hollow cylindrical symmetry with the novel mirror-immersion lens combination provides an additional effect, since the novel ion mirror has much higher tolerance to radial ion displacement, thus opening the way for high (half million to million range) of resolving power in cylindrical time-of-flight and electrostatic trap analyzers.

[068] In yet another embodiment, electrostatic field of one or both mirrors of hollow cylindrical symmetry can be periodically (spatially and not in time) modulated in the tangential Z-direction in combination with either tangentially periodic lens in the field free space or with the tangentially periodically modulated immersion lens.

[069] To further improve resolving power *R* with a target of $R \sim 1,000,000$ one may reduce the turn round time by improved ion confinement within small ($d = 2-3$ mm) bore gaseous ion guides, and by using higher acceleration energy in the analyzer, accompanied with the proportional increase in the acceleration field strength.

[070] Let us make numerical estimates for a particular hollow cylindrical MR-TOF analyzer with ion mirrors of Fig.11 at $2X_0 = 1080$ mm, window height $H = 30$ mm, $2R = 320$ mm diameter of median surface and with a periodic lens at $p = 10$ mm pitch. Such analyzer has 100 m flight path. The chosen parameters minimize effects of radial ion path deviation and satisfy criteria $R > 2X_0/3$ and $R > 50 * 2X_0 * \alpha^2$, where $\alpha \sim p/2X_0$ is the ion trajectory inclination angle in the analyzer, as disclosed in WO2011086430 and co-pending application 223322-313911, incorporated by the reference. Preferably, the hollow cylindrical analyzer has at least one radial steering electrode for steering ions to the mean cylindrical surface at ion reflection point, as disclosed in the same applications. Those precautions in combination with the third order spatial focusing of the present invention would ensure minimal spatial aberrations of the cylindrical MR-TOF analyzer, assessed in our simulations being under $2\Delta T/T_0 < 1E-6$ for the earlier assumed ion packet spreads (Gaussian energy distribution at $\sigma_K = 0.011K_0$ and uniform Y -distribution at full height of $2Y_0 = 0.133H$).

[071] Let us estimate resolution limit which is set by the turn around time in the proposed cylindrical analyzer. At preferred acceleration energy of 8 kV, the maximal voltage (on fifth electrode) is about 18.5 kV, i.e. sufficiently small (< 20 kV) to avoid electrical breakdown. Typical flight time of $m/z = 1000$ amu ions is then calculated as $T_0 = 2.5$ ms. Accounting $\Delta K/K_0 \sim 7\%$ limit onto relative energy spread, set by the analyzer aberrations at $R \sim 1,000,000$, the field strength in the orthogonal accelerator can be brought to $E = 400$ V/mm at $\Delta X = 1.5$ mm continuous ion beam size. If using small bore quadrupole ion guides, the output beam diameter can be brought to approximately 0.3 mm for 1000 amu ions. The beam diameter past the ion guide can be estimated as $d \sqrt{4kT/qV_{RF}}$ for thermal energy $kT = 0.026$ eV, $V_{RF} = 1000$ V and parameter $q = 0.01$ at 1000amu which allows low mass cut off in quadrupole at 50 amu. At proper telescopic refocusing of continuous ion beam in front of the accelerator, and accounting conservation of phase space $\Delta X * \Delta V_x$ in electrostatic lens (between quadrupole and accelerator), the transverse velocity spread ΔV_x of 1000 amu ions in the orthogonal accelerator can be reduced about 5 fold (1.5 mm /0.3 mm) relative to thermal velocity and (accounting velocity in opposite directions) can be brought down to 24 m/s. Then the turnaround time in 400 V/mm pulsed field corresponding to $A = 4E+10$ m²/s acceleration would induce turn around time $\Delta T_i = \Delta V_x/A = 0.6$ ns. Accounting 2.5 ms flight time for 1000 amu ions in $L = 100$ m MR-TOF, such turn around time is expected to limit the resolving power at about $2E+6$ level. In other words, extension of flight path and increasing acceleration voltage in the cylindrical hollow analyzer

does soften turn around time limitation and opens the opportunity of $R > 1E+6$ in MR-TOF analyzers.

[072] However, due to prolonged flight times in cylindrical MR-TOF, the expected duty cycle of the orthogonal accelerator becomes very low – between 0.1 and 0.2%, even with the method of double orthogonal extraction, disclosed in US2007176090, incorporated herein by reference. To remove the limiting link between the resolving power and the sensitivity of MR-TOF analyzers, preferably, the orthogonal accelerator should employ a method of frequent encoded pulsing disclosed in WO2011135477, incorporated herein by reference. Alternatively, in case of using the MR-TOF analyzer as a second stage of MS-MS tandem, the orthogonal accelerator may be preferably replaced by a linear ion trap with a pulsed radial ejection. The replacement becomes possible because of small intensity of parent ion beam which avoids space charge saturation in the pulsed trap and in the MR-TOF analyzer. Such trap should be oriented along the Z-axis, tilted by angle $\alpha/2$ and followed by a deflector for ion steering at angle $\alpha/2$, where the ion trajectory inclination angle in the analyzer is $\alpha \sim p/2X_0$, equal to 1/100 in the numerical example. Preferably, to avoid interference with ion trajectories and to reduce gas load onto the MR-TOF, the trap is followed by an isochronous curved inlet formed by electrostatic sectors as described in US7326925 by authors, incorporated herein by reference.

[073] Coaxial ion mirrors

[074] The improved ion mirrors scheme is applicable to coaxial multi-reflecting analyzers with a time-of-flight or image current detectors, disclosed in GB2080021, US5017780, US6013913A, US5880466, and US6744042, incorporated herein by reference. The cylindrical two-dimensional electrostatic field is known to provide very similar properties as planar two-dimensional field. Based on the above described ion optical studies it becomes obvious that at least a single focusing lens, and preferably an immersion lens is expected to improve spatial and energy acceptance of coaxial multi-reflecting analyzers. Such time-of-flight, or electrostatic trap analyzer should comprise: (a) two parallel and aligned grid-free coaxial ion mirrors separated by a field free region, said mirrors being arranged to reflect ions in the coaxial direction; (b) said mirrors having at least one electrode with an accelerating potential compared to the field-free space potential; and (c) at least one electrostatic lens, arranged to focus ions in the radial direction and placed between said ion mirrors. Preferably, said at least one lens is immersion. Preferably, the mirror-immersion lens arrangement is symmetric.

[075] Although the present invention has been describing with reference to preferred embodiments, it will be apparent to those skilled in the art that various modifications in form

and detail may be made without departing from the scope of the present invention as set forth in the accompanying claims.

CLAIMS**WHAT IS CLAIMED IS:**

1. An isochronous time-of-flight, open trap, or electrostatic trap analyzer comprising:
two parallel and aligned grid-free ion mirrors separated by a field free region, said mirrors being arranged to reflect ions in a first X -direction, said mirrors being substantially elongated in the transverse drift Z -direction to form a two-dimensional electrostatic field $E(X,Y)$ either of planar symmetry or of a hollow cylindrical symmetry, wherein said mirrors have at least one electrode with an accelerating potential as compared to the field-free space potential;
and
at least one electrostatic lens, arranged to focus ions in the Y -direction, said lens being elongated in said transverse Z -direction and placed between said ion mirrors.
2. An apparatus as set forth in claim 1, wherein said at least one lens is of (i) planar symmetry; (ii) hollow cylindrical symmetry.
3. An apparatus as set forth in claims 1 or 2, wherein said at least one lens is formed by a (i) set of pairs of flat electrodes with parallel surfaces; (ii) set of planar aperture slit electrodes; (iii) set of pairs of coaxial ring electrodes; (iv) set of coaxial ring-shaped aperture slits.
4. An apparatus as set forth in claims 1 to 3, wherein the number of said lens is two.
5. An apparatus as set forth in claims 1 to 4, wherein said lenses are separated from said mirror fields as well as from each other by field-free space (shield).
6. An apparatus as set forth in claims 1 to 5, wherein said lenses are immersion.
7. An apparatus as set forth in claims 1 to 6, wherein ions pass the field-free space separating said lenses and said mirrors at higher kinetic energies than the field-free space between said lenses.
8. An apparatus as set forth in claims 1 to 7, wherein a set of periodic lenses is placed between said mirrors for confining ions in said direction of elongation.

9. An apparatus as set forth in claims 1 to 8, wherein said lens is superimposed with said periodic lenses forming a set of lenses focusing ions in two transversal directions.
10. An apparatus as set forth in claims 1 to 9, wherein at least one mirror has a feature providing weak field being periodic in the direction Z of elongation of the mirror.
11. An apparatus as set forth in claims 1 to 10, further comprising an orthogonal accelerator with encoded frequent pulsing.
12. An apparatus as set forth in claim 1 to 10, further comprising a radial pulsed linear ion trap and a curved electrostatic sector inlet.
13. An isochronous time-of-flight or electrostatic trap analyzer comprising:
 - (a) Two parallel and aligned grid-free coaxial ion mirrors separated by a field free region, said mirrors being arranged to reflect ions in the coaxial direction;
 - (b) Said mirrors having at least one electrode with an accelerating potential compared to the field-free space potential; and
 - (c) At least one electrostatic lens, arranged to focus ions in the radial direction and placed between said ion mirrors.
14. An apparatus as set forth in claim 13, wherein said at least one lens is immersion.

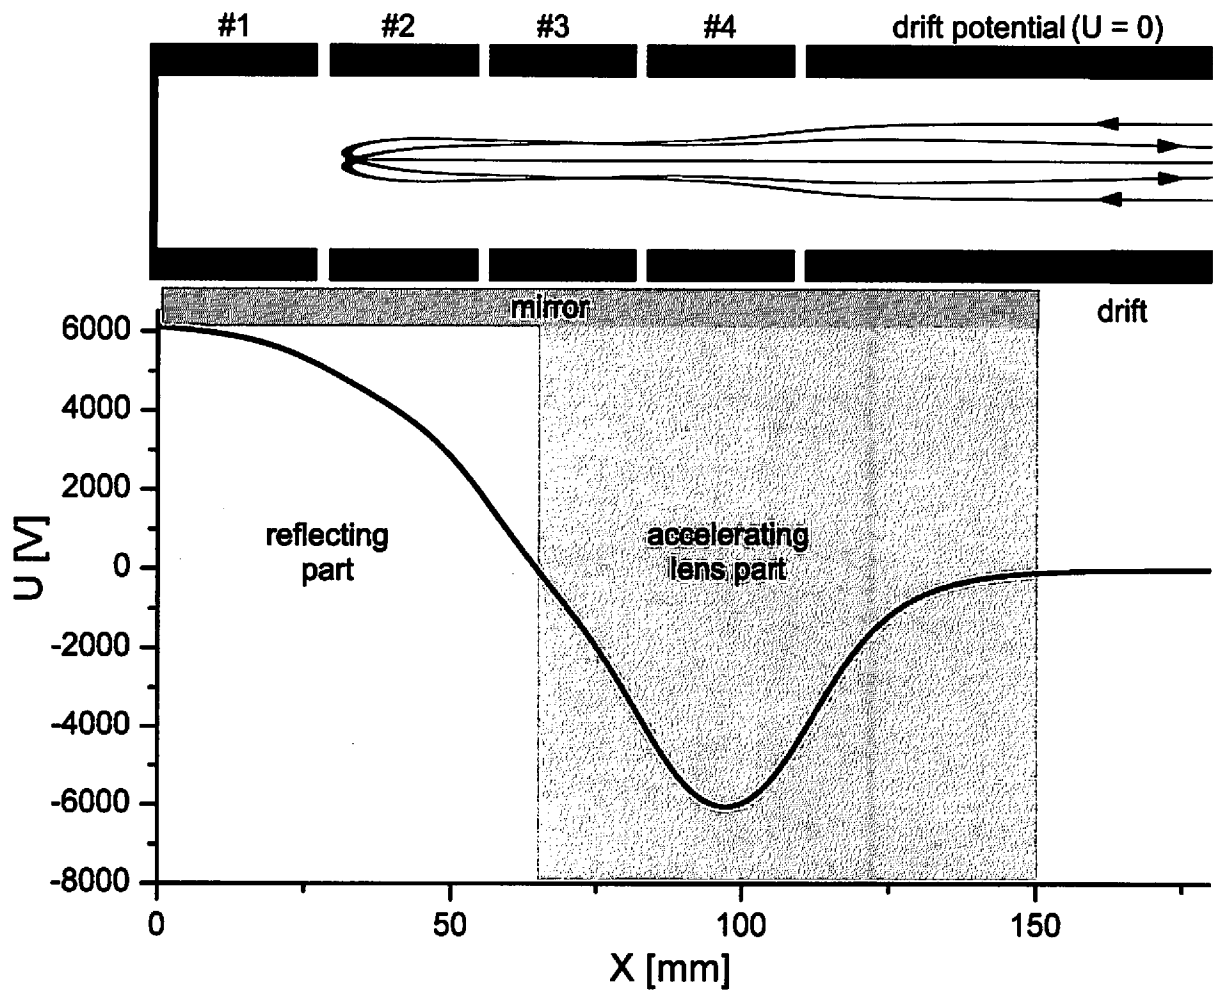


Fig. 1; Prior Art MPA-1

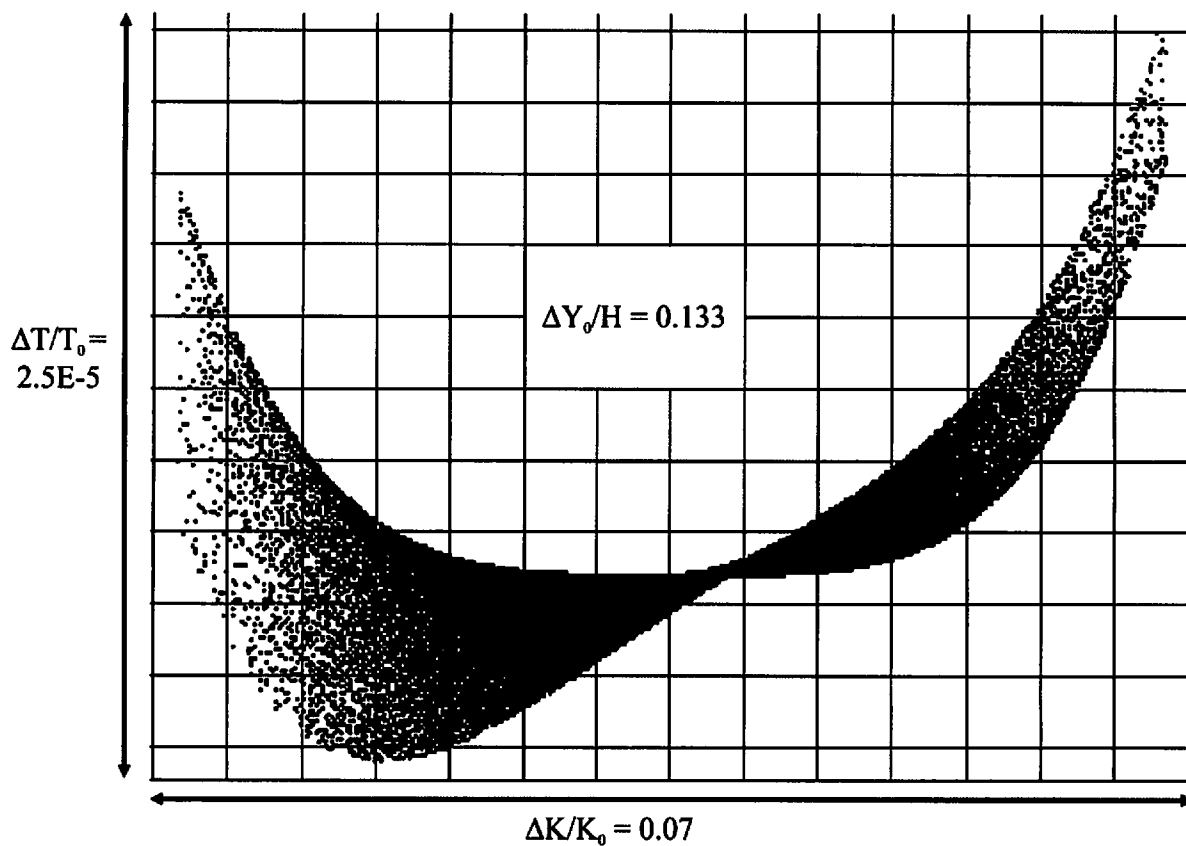


Fig. 2; Prior Art MPA-1

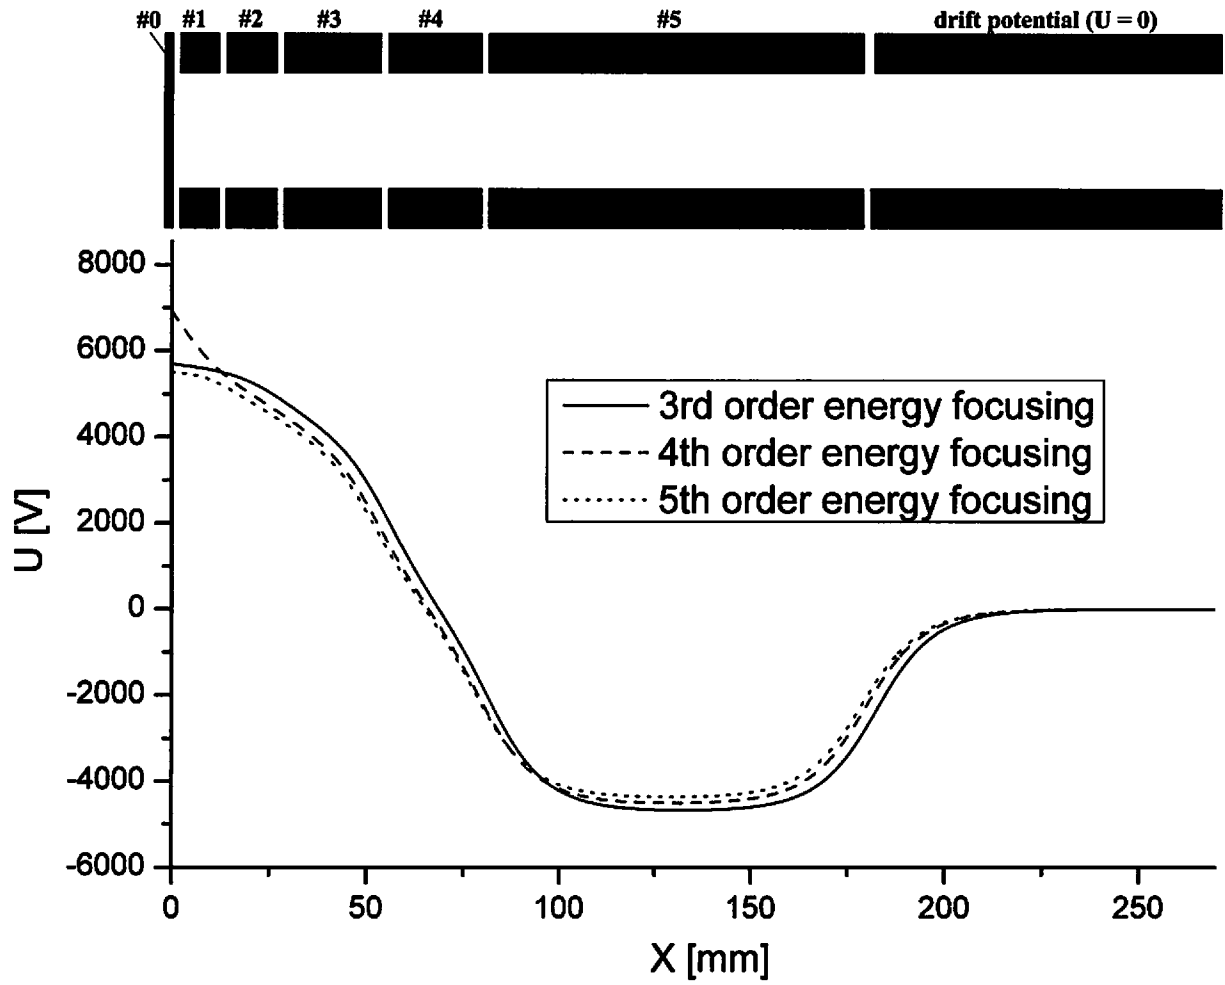


Fig. 3; Prior Art MPA-2

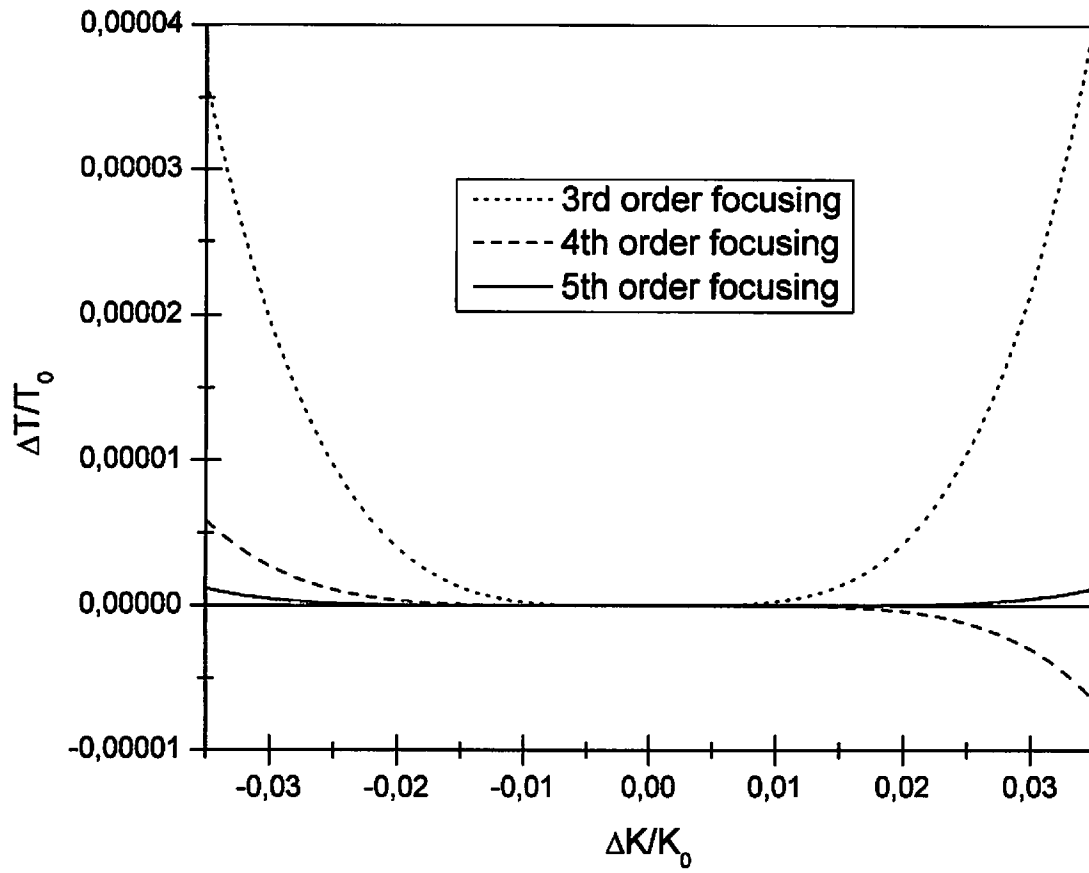


Fig. 4; Prior Art MPA-2

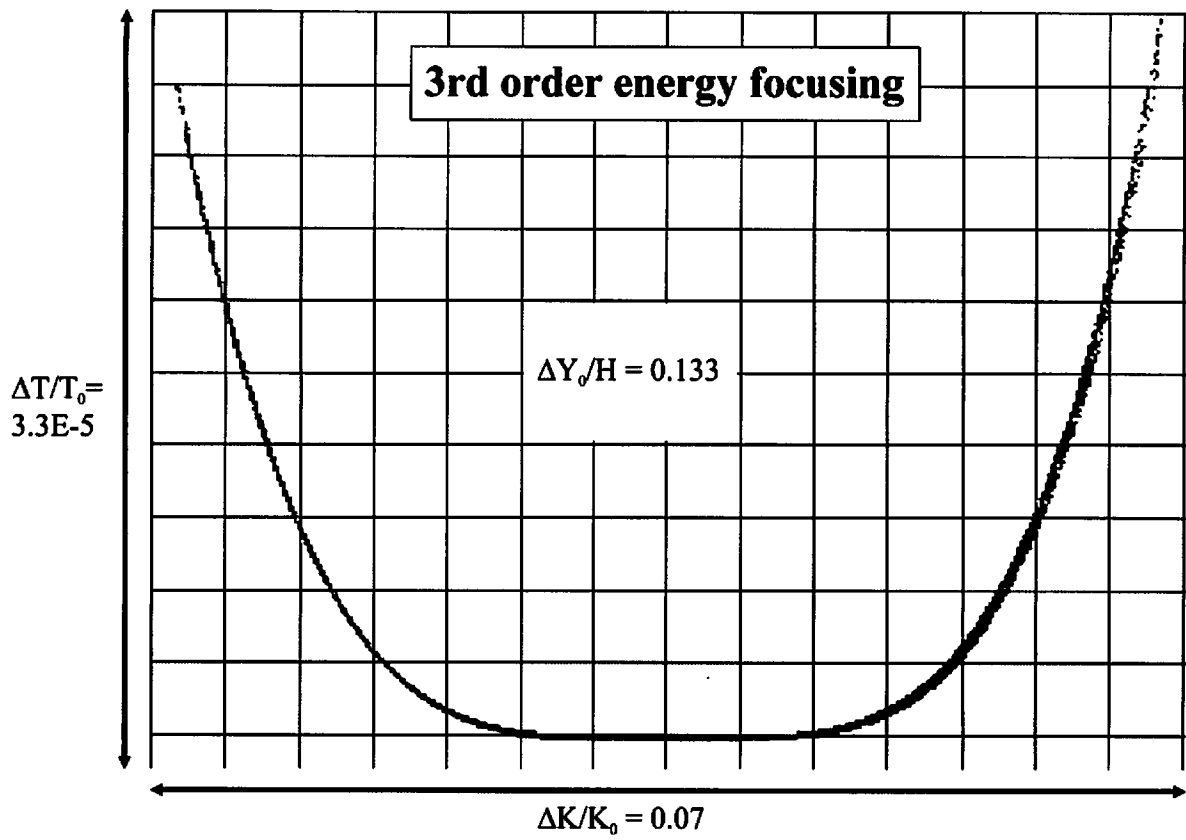


Fig. 5; Prior Art MPA-2-3

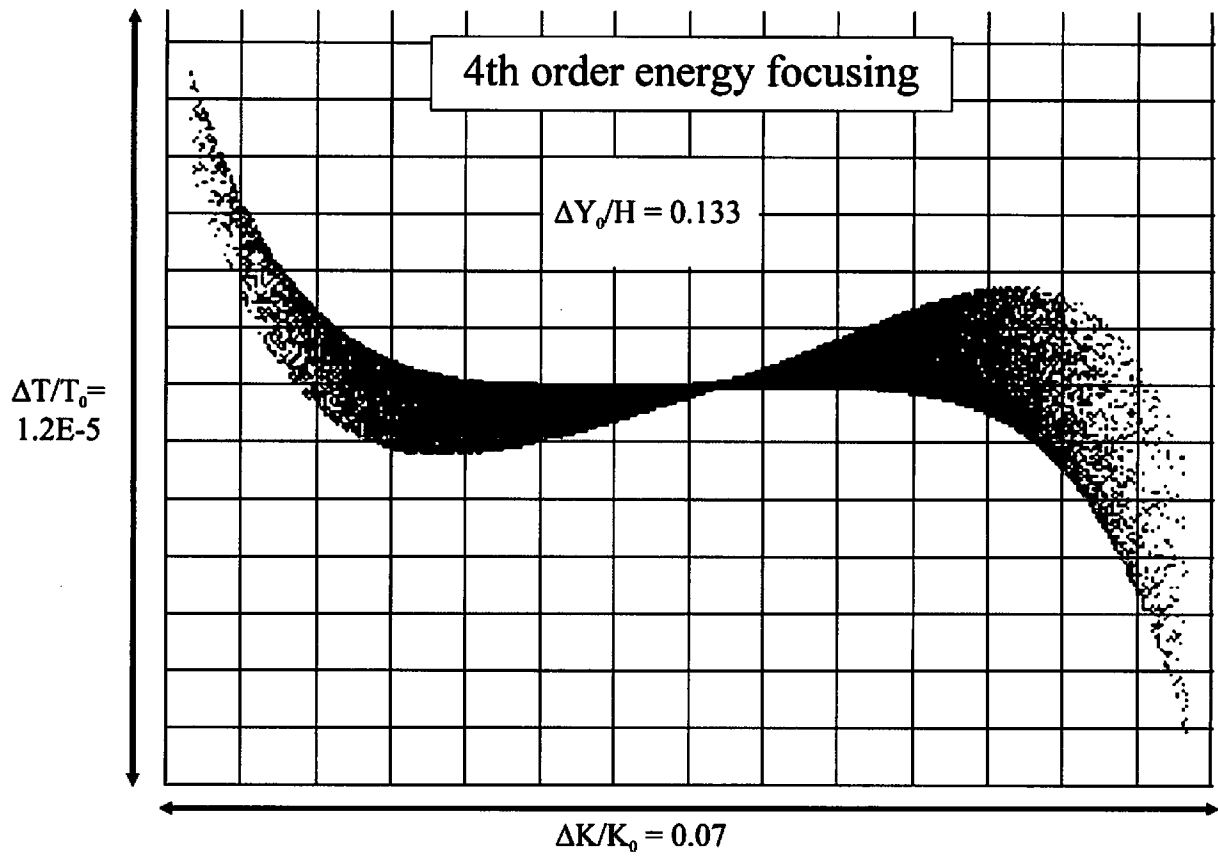


Fig. 6; Prior Art MPA-2-4

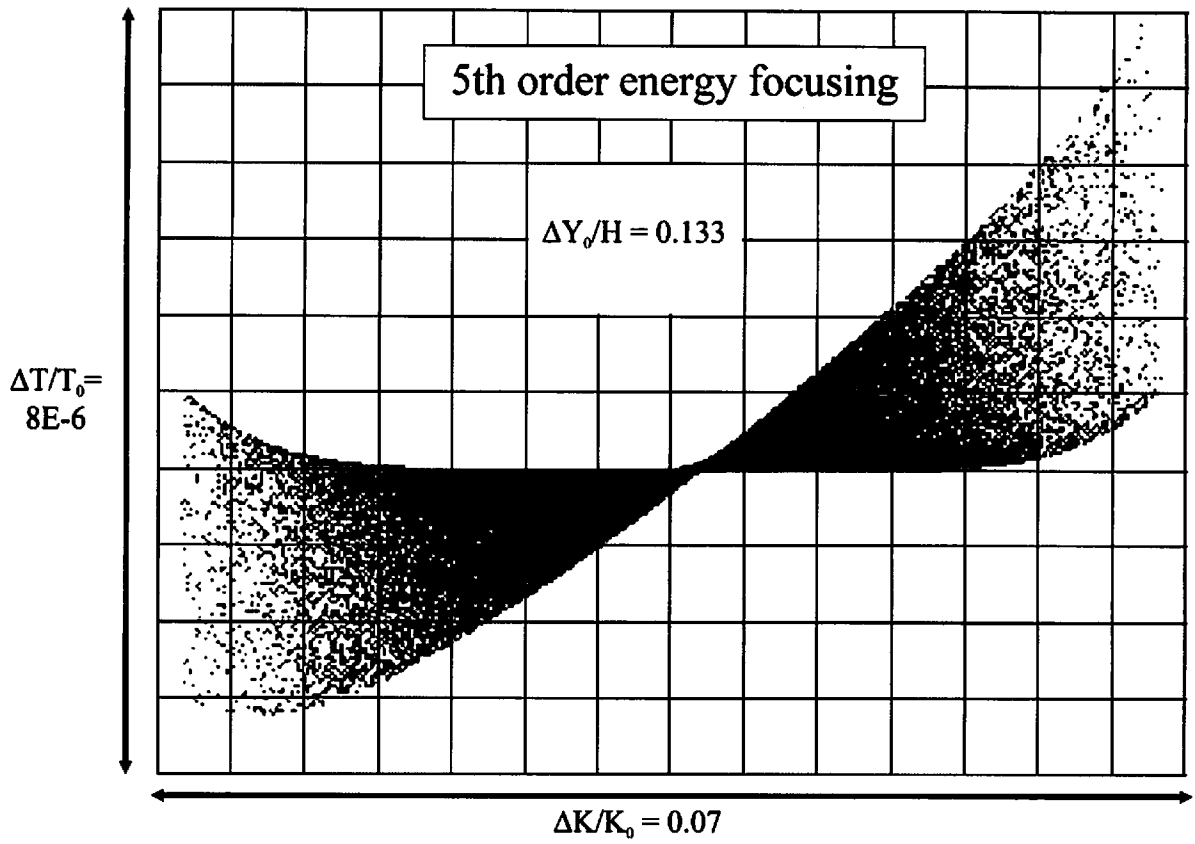


Fig. 7; Prior Art MPA-2-5

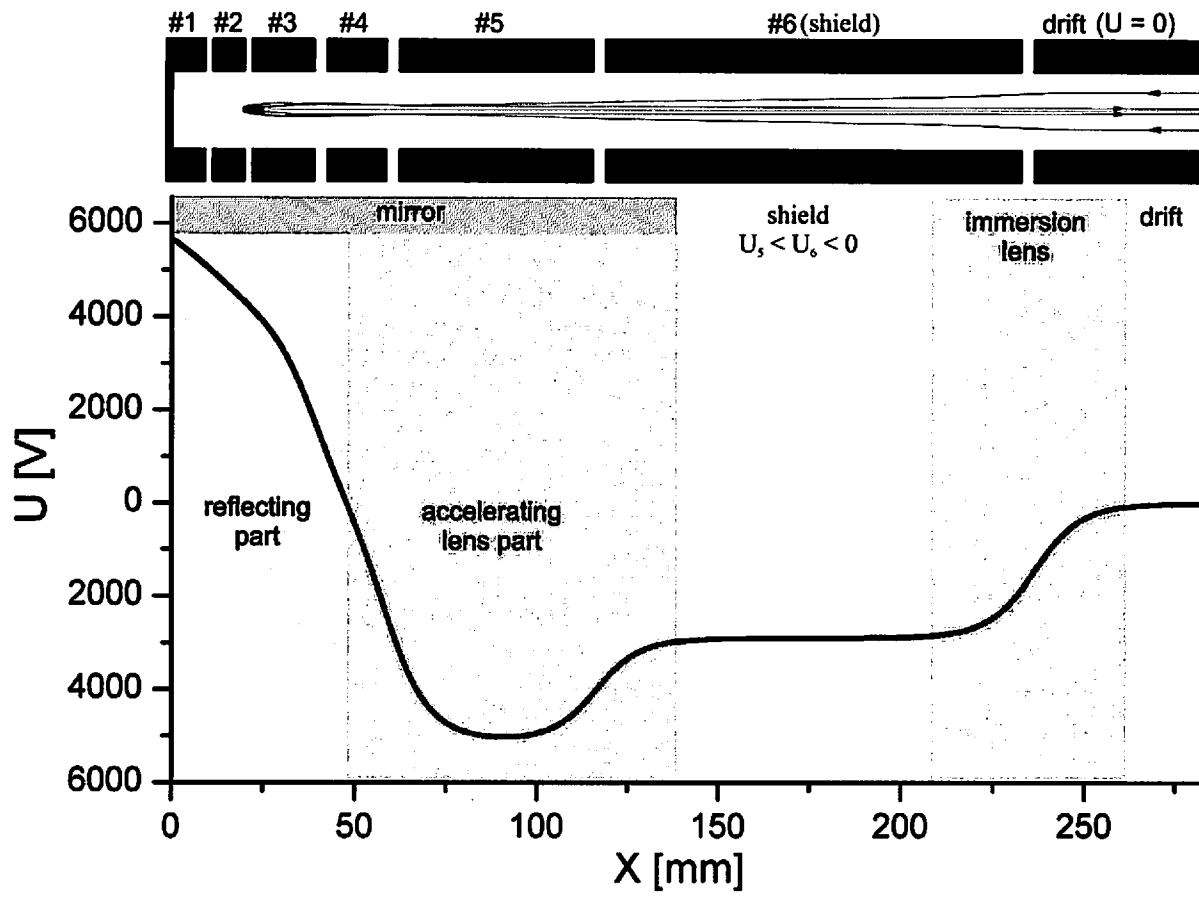


Fig. 8

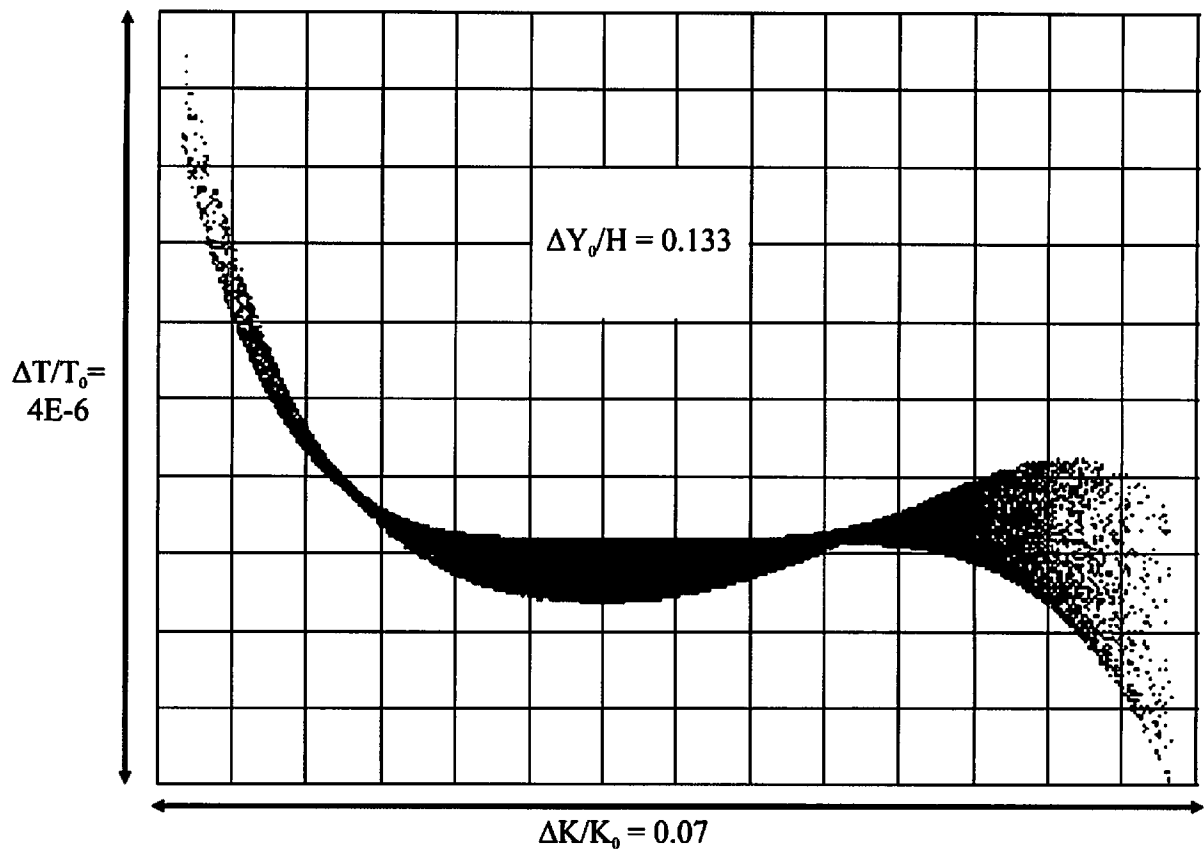


Fig. 9

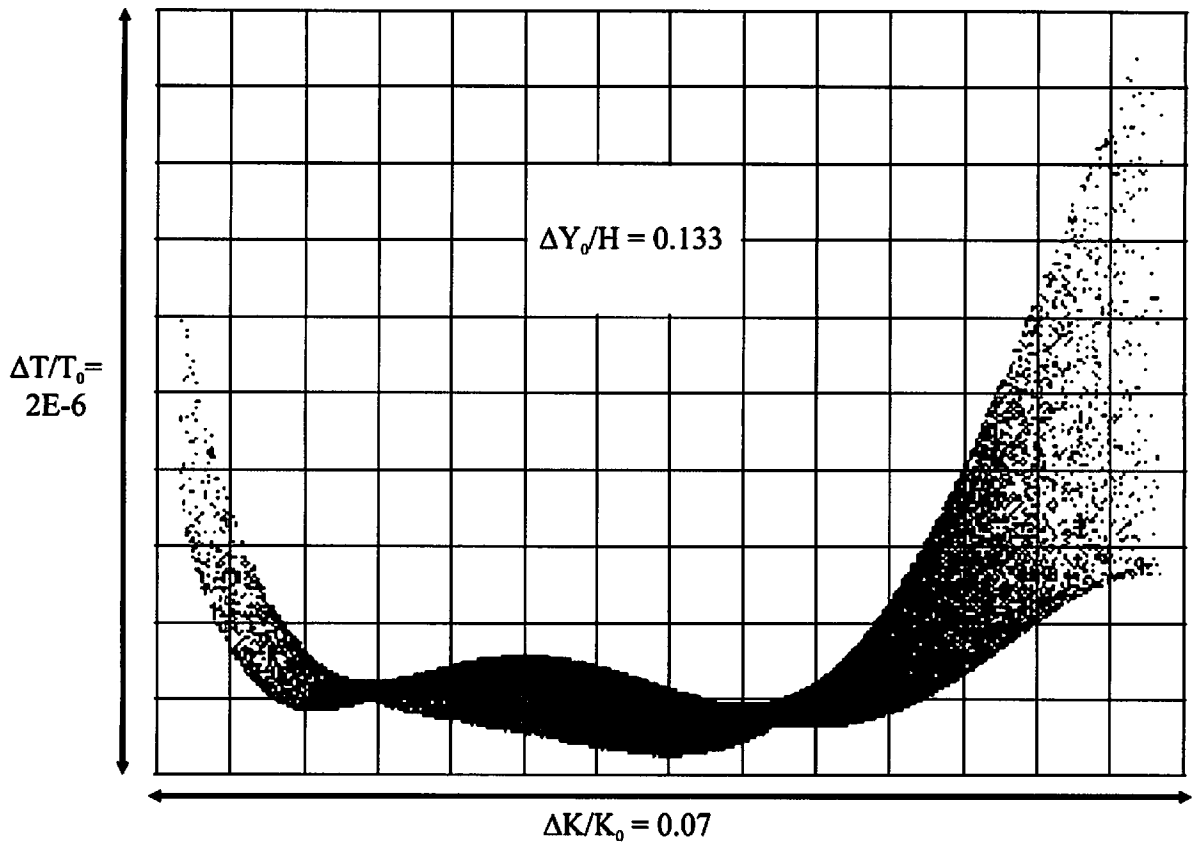


Fig. 10

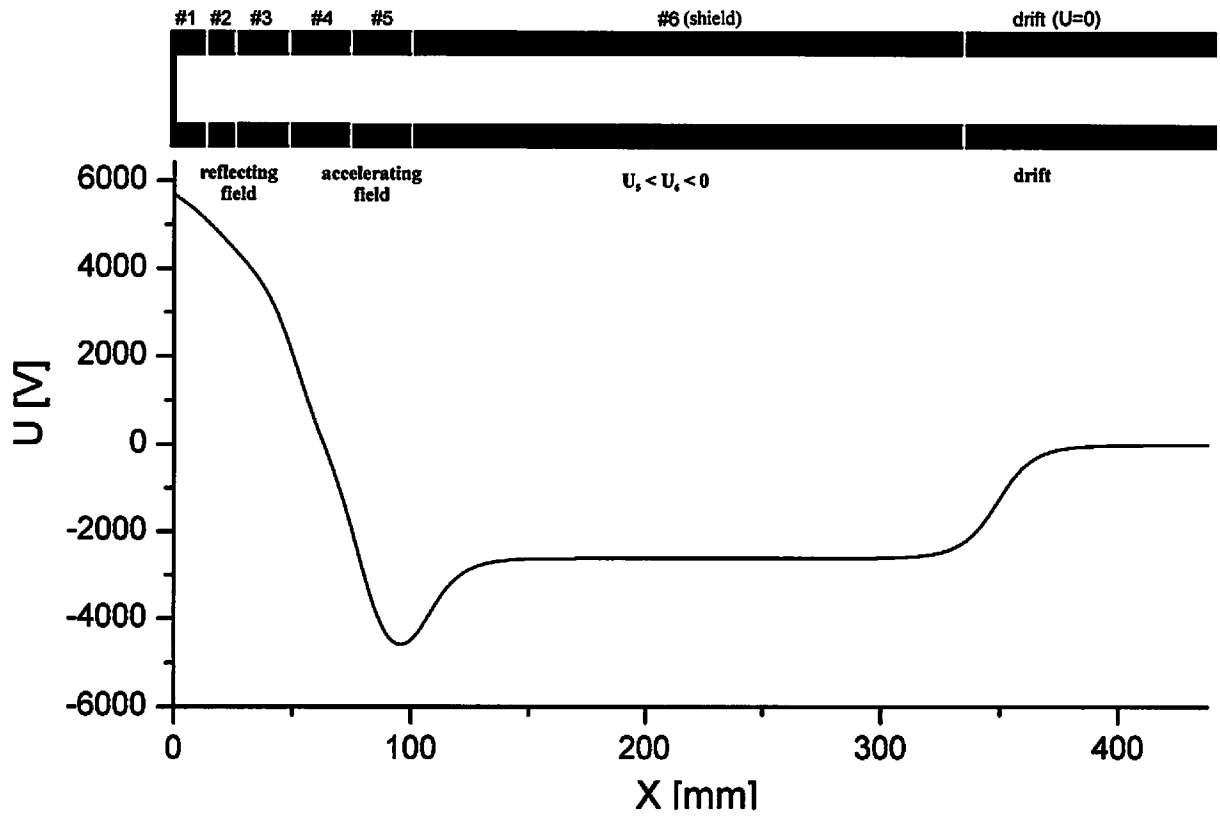


Fig. 11

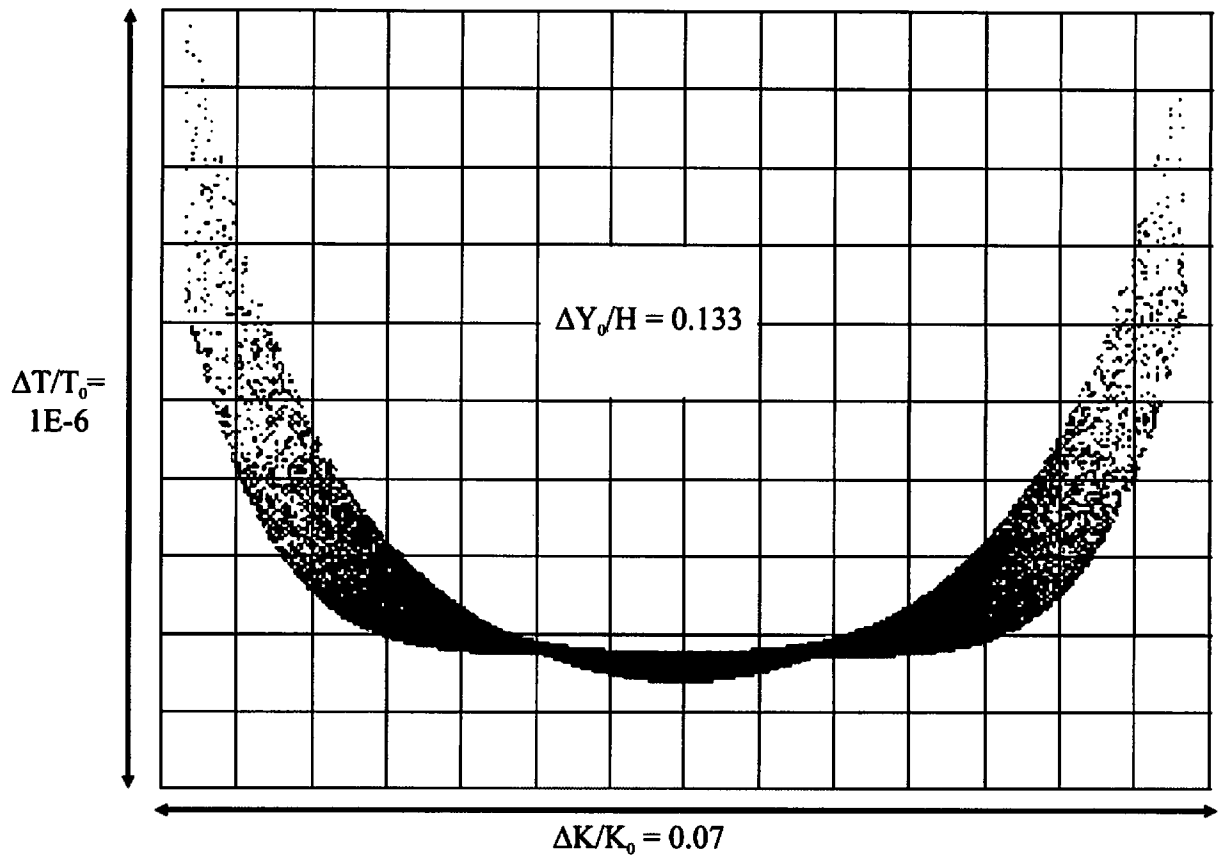


Fig. 12

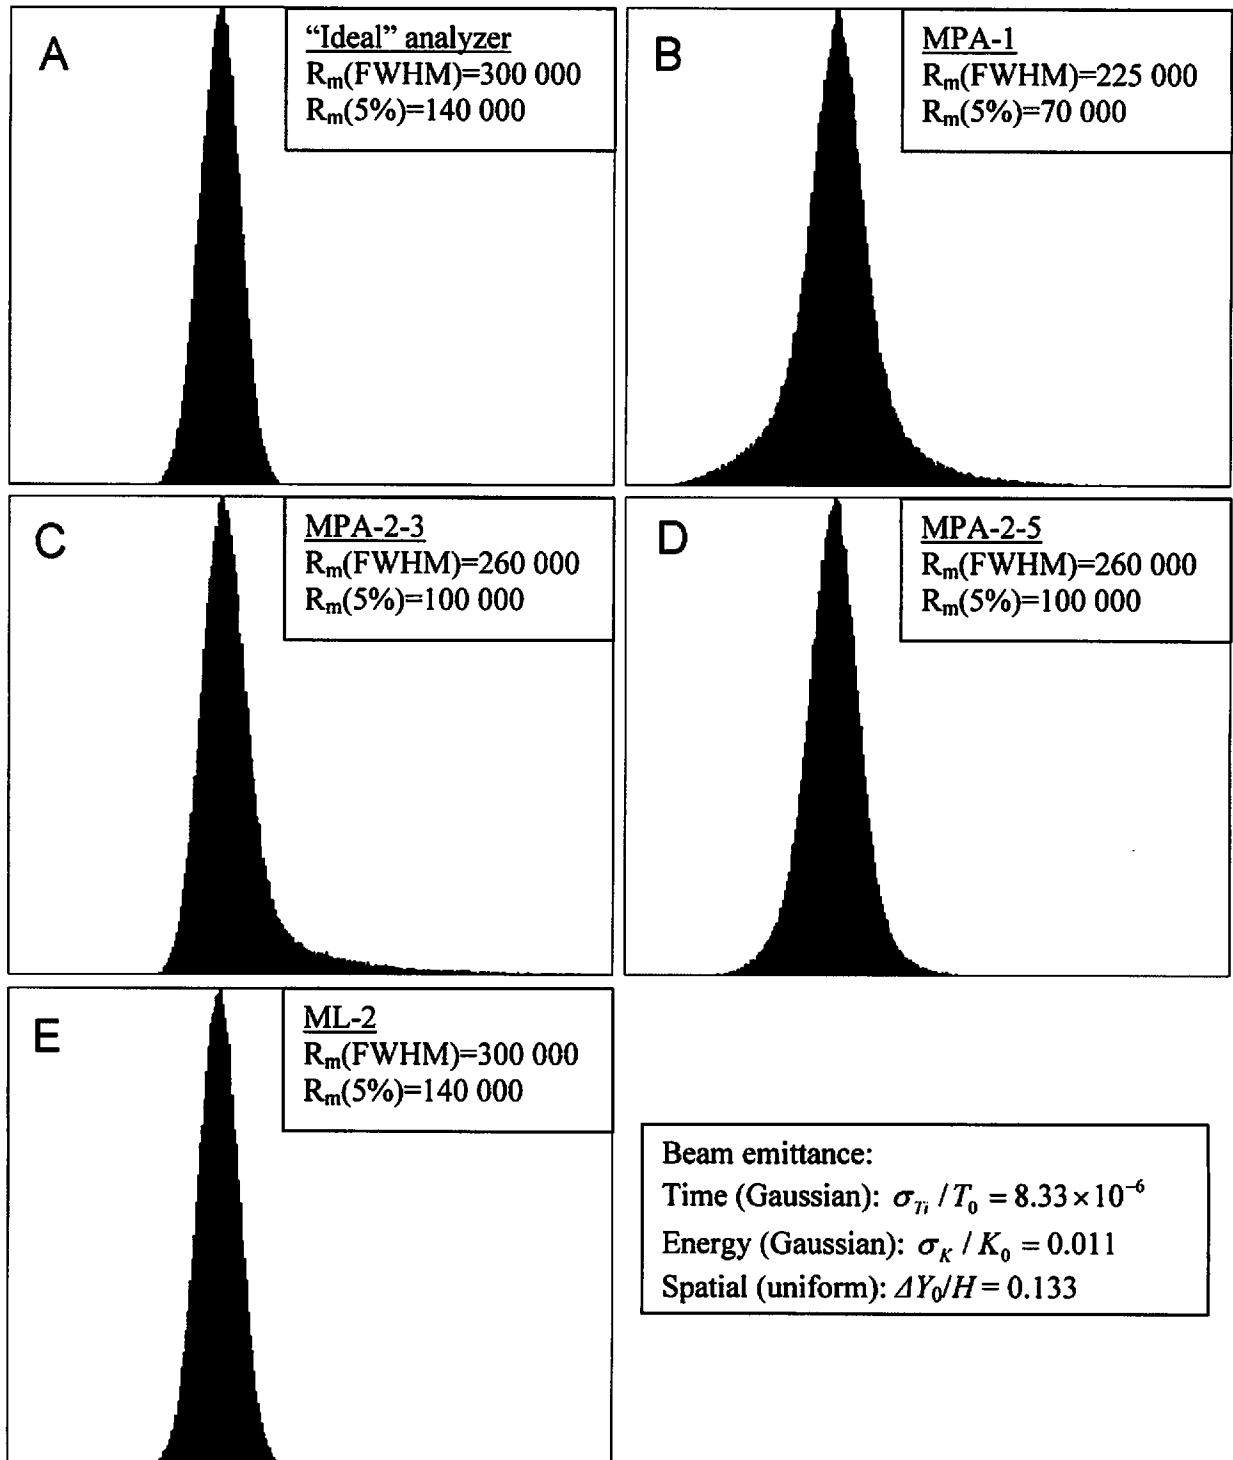


Fig. 13

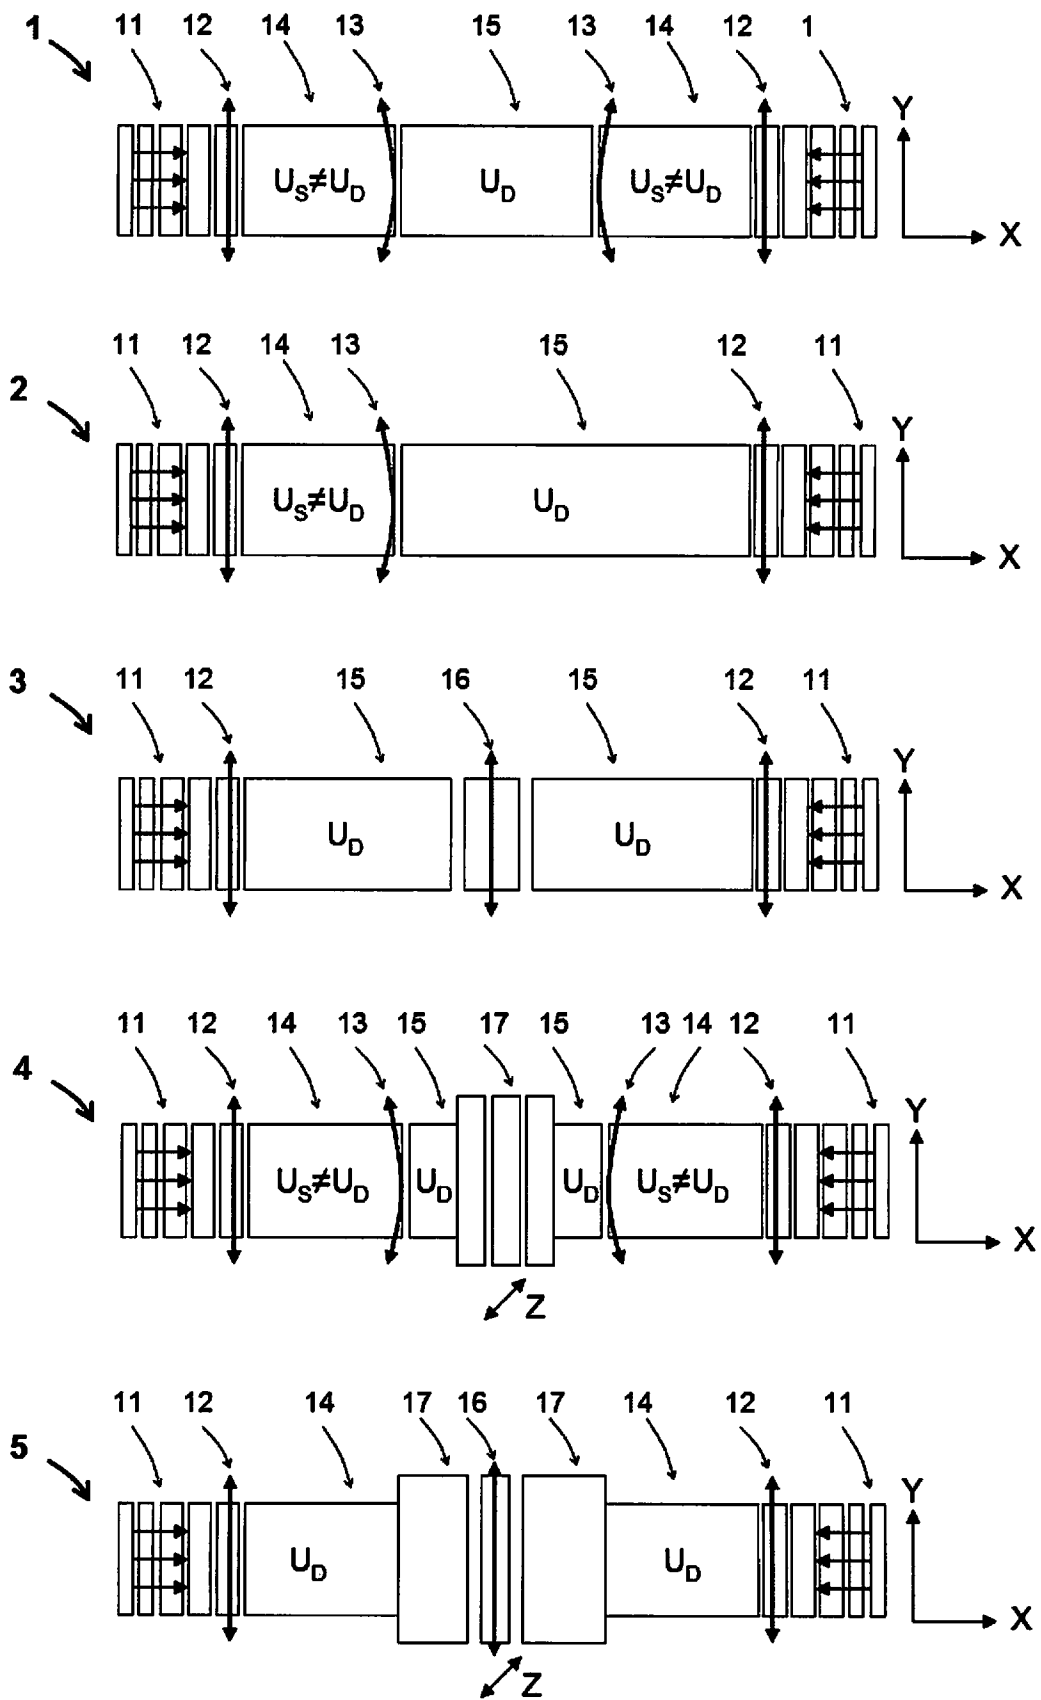


Fig. 14

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2013/031506

A. CLASSIFICATION OF SUBJECT MATTER
INV. H01J49/40
ADD.
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
Minimum documentation searched (classification system followed by classification symbols)
H01J
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
E	WO 2013/063587 A2 (LECO CORP [US]) 2 May 2013 (2013-05-02) figures 6,7 paragraph [0082] - paragraph [0086] -----	1-7
X	US 2007/029473 A1 (VERENTCHIKOV ANATOLI N [RU] VERENTCHIKOV ANATOLI [RU] ET AL) 8 February 2007 (2007-02-08) cited in the application	1-3,6,8, 9
Y	figures 4,5 paragraph [0075] - paragraph [0088] ----- -/--	4,5,7

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search 29 October 2013	Date of mailing of the international search report 16/01/2014
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer Cornelussen, Ronald

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2013/031506

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	YAVOR M ET AL: "Planar multi-reflecting time-of-flight mass analyzer with a jig-saw ion path", PHYSICS PROCEDIA, ELSEVIER, AMSTERDAM, NL, vol. 1, no. 1, 1 August 2008 (2008-08-01), pages 391-400, XP025818210, ISSN: 1875-3892, DOI: 10.1016/J.PHPRO.2008.07.120 [retrieved on 2008-08-01]	1-3,6,8,9
A	page 392, last paragraph page 393, last paragraph - page 394, paragraph 1 page 395, paragraph under figure 4 figures 2,3,6,7 the whole document	4,5,7
X	----- GB 2 403 063 A (VERENTCHIKOV ANATOLI NICOLAI [RU]) 22 December 2004 (2004-12-22) cited in the application	1-3,6,8,9
A	figure 5	4,5,7
Y	----- US 2011/017907 A1 (MAKAROV ALEXANDER A [DE] ET AL) 27 January 2011 (2011-01-27) figures 4,9 paragraph [0104]	4,5,7
A	----- SU 1 725 289 A1 (INST YADERNOJ FIZ AN KAZSSR [SU]) 7 April 1992 (1992-04-07) cited in the application figure 1 the whole document	1-9
A	----- US 2006/214100 A1 (VERENTCHIKOV ANATOLI N [RU] ET AL) 28 September 2006 (2006-09-28) the whole document	1-9
A	----- F Hinterberger: "Ion optics with electrostatic lenses", 1 January 2005 (2005-01-01), XP055085820, Retrieved from the Internet: URL: http://cds.cern.ch/record/1005034/files/p27.pdf [retrieved on 2013-10-29] the whole document	1-9

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2013/031506

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.

2. As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.

3. As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-9

Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-9

An isochronous time-of-flight analyzer comprising ion mirrors that are elongated in a drift direction. Each ion mirror comprises two lenses.

2. claim: 10

At least one mirror of the time-of-flight analyzer has a feature providing weak field being periodic in the direction Z of elongation of the ion mirror.

3. claim: 11

The time-of-flight analyzer further comprises an orthogonal accelerator with encoded frequency pulsing.

4. claim: 12

The time-of-flight analyzer further comprising a radial pulsed linear ion trap and a curved electrostatic sector inlet.

5. claims: 13, 14

The electrodes of the ion mirrors are not planar, but coaxial.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2013/031506

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2013063587	A2	02-05-2013	NONE
US 2007029473	A1	08-02-2007	NONE
GB 2403063	A	22-12-2004	AT 464648 T 15-04-2010 CN 1853255 A 25-10-2006 EP 1665326 A2 07-06-2006 GB 2403063 A 22-12-2004 JP 4763601 B2 31-08-2011 JP 2007526596 A 13-09-2007 KR 20060026053 A 22-03-2006 WO 2005001878 A2 06-01-2005
US 2011017907	A1	27-01-2011	CA 2710148 A1 02-07-2009 EP 2232525 A2 29-09-2010 EP 2610893 A2 03-07-2013 EP 2610894 A2 03-07-2013 EP 2613339 A1 10-07-2013 GB 2455977 A 01-07-2009 JP 5282102 B2 04-09-2013 JP 2011507205 A 03-03-2011 JP 2013175481 A 05-09-2013 JP 2013179083 A 09-09-2013 JP 2013179084 A 09-09-2013 US 2011017907 A1 27-01-2011 US 2013187043 A1 25-07-2013 US 2013313424 A1 28-11-2013 WO 2009081143 A2 02-07-2009
SU 1725289	A1	07-04-1992	NONE
US 2006214100	A1	28-09-2006	CN 101171660 A 30-04-2008 EP 1866951 A2 19-12-2007 JP 5357538 B2 04-12-2013 JP 2008535164 A 28-08-2008 US 2006214100 A1 28-09-2006 WO 2006102430 A2 28-09-2006