

(19) World Intellectual Property
Organization
International Bureau




(43) International Publication Date
23 December 2004 (23.12.2004)

PCT

(10) International Publication Number
WO 2004/110242 A2

- (51) International Patent Classification⁷: **A61B**
- (21) International Application Number:
PCT/IB2004/002020
- (22) International Filing Date: 17 June 2004 (17.06.2004)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
60/479,576 18 June 2003 (18.06.2003) US
60/512,491 18 October 2003 (18.10.2003) US
- (71) Applicant (for all designated States except US): **KONINKLIJKE PHILIPS ELECTRONICS N.V.** [NL/NL];
Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **YANOF, Jeffrey, H.** [US/US]; 595 Miner Road, Cleveland, OH 44143 (US).
BAUER, Chris [US/US]; 595 Miner Road, Cleveland, OH 44143 (US).
- (74) Common Representative: **KONINKLIJKE PHILIPS ELECTRONICS N.V.**; c/o LUNDIN, Thomas, M., 595 Miner Road, Cleveland, OH 44143 (US).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
— without international search report and to be republished upon receipt of that report
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: REMOTELY HELD NEEDLE GUIDE FOR CT FLUOROSCOPY

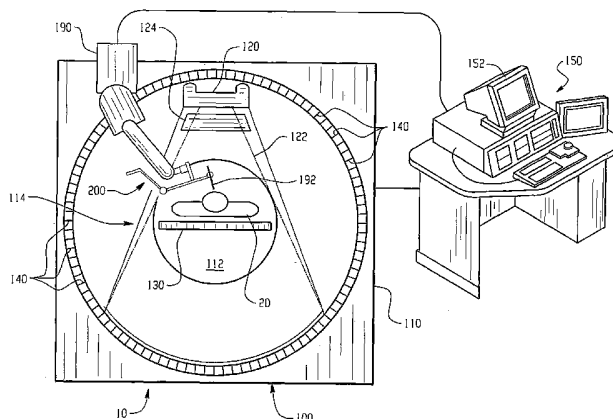

(57) Abstract: A guide apparatus (200) is provided for use with an associated imaging device (100) to direct movement of an associated interventional implement (192) relative to a patient (20) disposed on the imaging device (100). The guide apparatus includes a connector portion (210) coupling the guide apparatus with the associated imaging device (100). A main body portion (220) of the apparatus is supported relative to the associated imaging device by the connector portion (210). A gripping area (230) is formed at a first end (222) of the main body portion (220), the gripping area (230) being adapted to the guide apparatus (200) for manual gripping by an associated operator. A holding area (240) is formed at a second end (224) of the main body portion (220). The holding area (240) is adapted to hold the associated interventional implement (192) in an orientation suitable for motion relative to said patient (20) along a selected linear path (P) and also operative to translate the associated interventional implement (192) along said selected linear path (P) in response to manual force applied by the associated human operator at said gripping area (230). A robot arm (190) positions the apparatus to hold a biopsy needle relative to the patient based on a virtual planned trajectory. A linear slider joint constrains movement of the needle to the path (P) and permits manual insertion of the needle and attendant tactile feedback.



WO 2004/110242 A2

REMOTELY HELD NEEDLE GUIDE FOR CT FLUOROSCOPY

The present invention relates to the art of interactive intra-procedural image-guided surgery and interactive pre-procedural surgical planning. It finds particular application in conjunction with the planning and implementation stages of minimally invasive stereotactic surgical procedures performed in CT imaging systems using a robotic localization device to
5 orient an interventional implement such as a biopsy needle, ablation probe, or the like for planning and placement of objects or extraction of tissue from within the body of a patient, and will be described with particular reference thereto. It is to be appreciated, however, that the invention is also applicable to a wide range of imaging equipment and techniques, for example ultrasonic and magnetic resonance devices, and to a broad range of minimally
10 invasive surgical procedures including many forms of surgery for placing objects at precise points within a patient such as interventional radiology procedures and for removing tissue from precise locations within the patient during ablation procedures and biopsies.

It is often desired that interventional medical procedures be as minimally invasive as possible. However, it is also desirable to be able to visualize or otherwise know the relative
15 positions and/or orientations of surgical tools or devices with respect to surrounding anatomy. The latter goal may be achieved by a direct inspection of the anatomy. However, in the case of interior anatomy, direct inspection may be more invasive than desired inasmuch as additional or larger incisions may have to be made to expose or access the interior anatomy for direct inspection.

For example, it is often desirable to sample or test a portion of tissue from human or
20 animal subjects, particularly in the diagnosis and treatment of potentially cancerous tumors, pre-malignant conditions, and other diseases or disorders. Typically, in the case of tumors, when the physician suspects that cancer or an otherwise diseased condition exists, a biopsy is performed to determine if in fact cells from the tumor are cancerous or otherwise diseased.
25 Many biopsies, such as percutaneous biopsies, are performed with a needle-like instrument used to collect the cells for analysis.

In recent years, the performance of interventional medical procedures such as needle biopsies has been enhanced by the use of x-ray imaging, CT scans, continuous CT (CCT), magnetic resonance imaging (MRI), fluoroscopy, single photon emission CT (SPECT),
30 positron emission tomography (PET), and the like. The imaging equipment allows an

interventionalist, such as a radiologist, surgeon, physician, or other medical personnel, to track the insertion of interventional devices, such as biopsy needles, in a subject during diagnostic and therapeutic procedures. While such imaging modalities allow procedures to be performed with minimal invasiveness and are helpful to the interventionalist and the patient, they have
5 certain drawbacks.

For example, with some image-guided procedures, e.g., those using CT imaging, the tracking of the needle position is not done in real-time. That is to say, a static image is obtained and the needle position noted therein. Subsequently, the needle is advanced or retracted by a small amount and another static image obtained to verify the new needle
10 position. This sequence is repeated as many times as necessary to track the needle's progression. Such a procedure tends to be time consuming inasmuch as the needle progresses by only a short distance or increment between imaging, and needle progression is halted during imaging. Moreover, accuracy suffers to the extent that in the interim, i.e., between images, the needle's position cannot be visualized.

With the development of CCT imaging and fluoroscopy, real-time imaging has been made possible. In CCT scanning, a rotating x-ray source irradiates the subject continuously, generating images at a rate of approximately six frames per second. The use of CCT or fluoroscopy by the interventionalist for real-time guidance and/or tracking of the needle during
15 biopsies is gaining popularity. As a result, biopsies have become not only more accurate, but also shorter in duration. However, because the imaging proceeds continuously, the patient and potentially the interventionalist are both exposed to a greater dose of radiation as compared to, e.g., non-continuous CT.
20

Accordingly, there exists in the prior art a trade-off between the level of radiation exposure experienced and real-time visualization of the procedure. That is to say, lower
25 radiation exposure is conventionally achieved at the cost of real-time visualization, and conversely, real-time visualization is conventionally achieved at the cost of higher radiation exposure.

One problem resides in protecting the interventionalist from radiation exposure. In needle biopsies, for example, often the biopsy needle and guide are held within or close to the
30 plane of the x-ray radiation so that the needle-tip will reside in the image plane thereby permitting continuous tracking. Staying close to the plane of imaging also, more often than not, allows for the distance the needle passes through the subject to be minimized.

Consequently, this typically results in the interventionalist placing his/her hands in the x-ray beam. The hands of an interventionalist who performs several such procedures per day can easily receive a toxic dose of radiation. Therefore, it is desirable to provide interventionalists with a way to perform needle biopsies without the risk of radiation exposure.

5 A proposed approach to solving the aforementioned problem involves the use of automated robot-like mechanical systems which allow the interventionalist to manipulate the biopsy needle remotely while keeping hands clear of the x-ray beam. However, such systems typically reduce or eliminate the tactile sensations (e.g., pressure and tension forces, shear, and/or moment on the needle) otherwise available to an interventionalist directly manipulating
10 the needle. This is disadvantageous in that interventionalists typically obtain useful information from these tactile sensations and rely upon it regarding the procedure. For example, they are often able to feel the progress of the needle as it transitions between different tissue types, makes contact with bones, punches through skin, etc. The interventionalists generally desire this "feel" as they perform biopsies. To trained personnel, it
15 serves as an additional indication of the needle's location.

Commonly owned U.S. Patent No. 6,245,028 to Furst, et al. addresses the lack of feel and interventionalist radiation exposure issues in part. However, the tubular curved needle guide disclosed there encloses the biopsy needle and does not provide a means of lateral release. It is also not clear if the needle could be driven on a straight path or how the
20 interventionist could make manual adjustments to steer the needle such as, for example, by beveling the tip of the needle should the need arise. In some embodiments of the needle biopsy system disclosed there, a master-slave system is used wherein a joystick controlled motorized device drives the needle. Failure modes or mechanisms are not discussed in either the drive mechanism or in the simulated force feedback system.

25 The present invention contemplates a new and improved interactive image-guided interventional method and system including a remotely held needle guide apparatus for enabling radiologists to safely extend their reach into the active region of a CT aperture during needle insertion under real-time x-ray CT fluoroscopy. The present invention overcomes the above-referenced problems arising in the prior art techniques and others as will become
30 apparent to those skilled in the art.

In accordance with one aspect of the present invention, a guide apparatus is provided for use with an associated imaging device to direct movement of an associated interventional implement relative to a patient disposed on the imaging device. The guide apparatus includes a connector portion for coupling the guide apparatus with the associated imaging device, a main body portion, a gripping area, and a holding area. The main body portion is supported relative to the associated imaging device by the connector portion. The gripping area is formed at a first end of the main body portion and is adapted for manual gripping by an associated human operator of the subject guide apparatus. The holding area is formed at the second end of the main body portion and is adapted to hold the associated interventional implement in an orientation suitable for motion relative to the patient along a selected linear path. The holding area is operative to translate the associated interventional implement along the selected linear path in response to manual force applied by the associated human operator at the gripping area.

In accordance with another aspect of the invention, a system is provided for inserting a medical device into a patient. The system includes an imaging device scanning the patient to generate a volumetric image data set of the patient. A human readable display device is provided for displaying an image of the patient derived from the volumetric image data set. Means are provided for selecting a virtual trajectory defining a path for inserting the medical device into the patient. Robotic means are provided on the imaging device, the robotic means being movable into selected positions relative to the imaging device. A guide apparatus is disposed on the robotic means, the guide apparatus being adapted to direct movement of the medical device relative to the patient.

In accordance with yet a further aspect of the invention, the imaging device is a CT scanner, an MRI scanner, a CCT scanner, a fluoroscope, a SPECT scanner, a PET scanner, or a combination of the foregoing.

In accordance with yet a further aspect of the invention, the medical device is a tissue ablation probe or a biopsy needle.

In accordance with a still further aspect of the invention, the guide apparatus includes a connector portion having a linear slide joint for movement of the guide apparatus along a single linear trajectory.

One advantage of the present invention is that it guards against excessive radiation exposure to both the interventionist and the patient.

Another advantage of the present invention is that it provides tactile feedback to the interventionist.

Yet another advantage of the present invention is that it permits the interventionist to continually monitor and/or visualize the progression of the procedure via a virtual view of the same while continuously obtaining real-time images of the actual procedure for verification.

Still further advantages and benefits of the present invention will become apparent to those of ordinary skill in the art upon reading and understanding the following detailed description of the preferred embodiments.

The invention may take form in various components and arrangements of components, and in various steps and arrangements of steps. The drawings are only for purposes of illustrating preferred embodiments and are not to be construed as limiting the invention.

FIGURE 1 is a diagrammatic illustration of an image-guided interventional medical procedure system in accordance with aspects of the present invention;

FIGURE 2 shows a robotic arm supporting a remotely held needle guide apparatus carrying a biopsy needle in accordance with aspects of the present invention;

FIGURE 3 is a perspective view showing the remotely held needle guide apparatus formed in accordance with aspects of the present invention;

FIGURES 3A and 3B are elevational views showing a preferred embodiment of a needle holder portion of the needle guide device of FIGURE 3;

FIGURES 4A and 4B are partial cross-sectional views of a linear guide mechanism of the remotely held needle guide apparatus of FIGURE 3;

FIGURE 5 is a virtual planning view in accordance with aspects of the present invention for interventional medical procedures; and,

FIGURE 6 is a block diagram showing the preferred operation of the image-guided interventional medical procedure system in accordance with aspects of the present invention.

With reference to FIGURE 1, an image-guided interventional medical procedure system **10** includes a diagnostic imaging apparatus **100** capable of generating medical diagnostic images of a subject **20**. Optionally, the imaging apparatus **100** is an x-ray

imaging device, CT scanner, CCT scanner, MRI scanner, fluoroscope, SPECT scanner, PET scanner, a combination of the foregoing or the like.

In the illustrated preferred embodiment, the diagnostic imaging apparatus **100** is a CT scanner having a stationary gantry **110** which defines a central examination region **112**. A rotating gantry **114** is mounted on the stationary gantry **110** for rotation about the examination region **112**. A source of penetrating radiation **120**, such as an x-ray tube, is arranged on the rotating gantry **114** for rotation therewith. The source of penetrating radiation produces a beam of radiation **122** that passes through the examination region **112** as the rotating gantry **114** rotates. A collimator and shutter assembly **124** forms the beam of radiation **122** into a thin fan-shape and selectively gates the beam **122** on and off. Alternately, the radiation beam **122** is gated on and off electronically at the source **120**. Using an appropriate reconstruction algorithm in conjunction with the data acquired from the CT scanner, images of the subject **20** therein are selectively reconstructed.

A subject support **130**, such as an operating table, couch or the like, suspends or otherwise holds the subject **20** received thereon, such as a human or animal patient, at least partially within the examination region **112** such that the thin fan-shaped beam of radiation **122** cuts a cross-sectional slice through the region of interest of the subject **20**.

In the illustrated fourth generation CT scanner, a ring of radiation detectors **140** is mounted peripherally around the examination region **112** on the stationary gantry **110**. Alternately, a third generation CT scanner is employed with an arc of radiation detectors **140** mounted on the rotating gantry **114** on a side of the examination region **112** opposite the source **120** such that they span the arc defined by the thin fan-shaped beam of radiation **122**. Regardless of the configuration, the radiation detectors **140** are arranged to receive the radiation emitted from the source **120** after it has traversed the examination region **112**.

In a source fan geometry, an arc of detectors which span the radiation emanating from the source **120** are sampled concurrently at short time intervals as the source **120** rotates behind the examination region **112** to generate a source fan view. In a detector fan geometry, each detector is sampled a multiplicity of times as the source **120** rotates behind the examination region **112** to generate a detector fan view. The paths between the source **120** and each of the radiation detectors **140** are denoted as rays.

The radiation detectors **140** convert the detected radiation into electronic projection data. That is to say, each of the radiation detectors **140** produces an output signal which is

proportional to an intensity of received radiation. Optionally, a reference detector may detect radiation which has not traversed the examination region **112**. A difference between the magnitude of radiation received by the reference detector and each radiation detector **140** provides an indication of the amount of radiation attenuation along a corresponding ray of a sampled fan of radiation. In either case, each radiation detector **140** generates data elements which correspond to projections along each ray within the view. Each element of data in the data line is related to a line integral taken along its corresponding ray passing through the subject being reconstructed.

With each scan by the CT scanner, the image data from the radiation detectors **140** is collected and reconstructed into image representations of the subject **20** in the usual manner. For example, a data processing unit incorporated in a workstation and/or control console **150** collects the image data and reconstructs the image representation therefrom using rebinning techniques, convolution/backprojection algorithms, and/or other appropriate reconstruction techniques. In a preferred embodiment, the image representations corresponding to the cross-sectional slice traversed by the thin fan-shaped beam of radiation **122** through the region of interest of the subject **20**, are displayed on a human viewable display, such as a video monitor **152** or the like, which is also part of the console **150**. Several preferred views are illustrated in FIGURE 5 and will be described in greater detail below. The control console **150** is optionally remotely located with respect to the imaging apparatus **100** (e.g., in a shielded room adjacent the scanning room containing the imaging apparatus **100**) and typically it includes one or more monitors **152**, a computer or data processing hardware and/or software, one or more memories or other data storage devices, and one or more standard input devices (e.g., keyboard, mouse, trackball, etc.).

With reference to FIGURE 2-4B, and continuing reference to FIGURE 1, in a preferred embodiment, the image-guided interventional medical procedure system **10** also includes a robotic arm **190** preferably carried on the stationary gantry **110**. The robotic arm **190** supports a remotely held needle guide apparatus **200** carrying an interventional implement or other like medical device **191** e.g., an ablation probe or a biopsy needle **192** at a desired location and trajectory. The medical device **191** is supported within the examination region **112** as shown. The robotic arm **190** is preferably a fully adjustable multi-jointed multi-segmented arm with each joint having at least one degree of freedom. As will be described in greater detail later herein, a medical device **191**, preferably the ablation probe or biopsy needle

192, is held by the needle guide apparatus 200 (as best seen in FIGURE 3). Accordingly, by appropriately arranging the robotic arm 190 (i.e., flexing or otherwise adjusting the multiple joints and/or segments, but preferably by executing a program which aligns the arm to the planned trajectory and by appropriately positioning the subject 20 and the robotic arm 190 relative to one another, any arbitrary position and/or orientation of the biopsy needle 192 relative to the subject 20 is achieved as desired. Preferably, the position and/or orientation of the medical device 191 defines a physical path coincident with the virtual planned trajectory.

With particular reference to FIGURE 3, the remotely held needle guide apparatus 200 includes a connector portion 210 for coupling the guide apparatus 200 with the associated imaging device 100, preferably to the distal end 194 of the robotic arm 190. In its preferred form, the connector portion 210 includes a prism joint linear slider mechanism 212 having a single degree of freedom.

A main body portion 220 of the needle guide apparatus 200 is supported relative to the associated imaging device 100 by the connector portion 210. A gripping area 230 is formed at a first end 222 of the main body portion 220. The gripping area 230 is provided to adapt the needle guide apparatus 200 for manual gripping by an associated interventionist. A medical device holding area 240 is formed at a second end 224 of the main body portion 220 as illustrated. The holding area 240 is adapted to hold an associated interventional implement such as a biopsy needle 192 in an orientation suitable for motion relative to the patient 20 along a selected linear path P. The implement holding area 240 is operative to translate the associated interventional tool 192 such as an ablation probe or a biopsy needle 192 along a linear path, selected in a manner to be described in greater detail below, in response to manual force provided by the associated interventionist at the gripping area 230. In that manner, force applied by the interventionist at the gripping area 230 in the direction A urges the main body portion 220 to translate along a linear path B as constrained by the single degree of freedom connector portion 210. This in turn causes the holding area 240 to similarly move in a linear path C. It is to be appreciated that each of the linear paths A, B, and C traversed by portions of the needle guide apparatus 200 lie or extend in parallel with the path defined by the single degree of freedom connector portion 210. The connector portion 210 is preferably a linear slider prism joint although any suitable mechanism which restrict movement to a single linear path could be used as well.

In connection with the above, it is further to be appreciated that, preferably, the associated interventional implement **192** is held in a relationship relative to the patient disposed on the patient support along a linear path **P** which lies identically parallel with the linear paths **A**, **B**, and **C** traversed by the needle guide apparatus **200** as constrained by the linear slider prism joint **212**. To that end, the holding area **240** includes a needle holder portion **250** which is adapted to hold the implement **192** in an orientation suitable for motion relative to the patient **20** along the planned trajectory **P**. Preferably, the needle holder portion **250** is biased in an open position by the gripping area **230** or through other means so that the needle **192** is held firmly in place only through the active participation of the interventionist. In that sense, the needle holder **250** formed in the holding area **240** is "failsafe" and preferably releases from the grip of the guide apparatus **200** when active physical control over the apparatus is discontinued by the interventionist. Prior art systems such as robotic or other direct mechanical needle feeding apparatus do not enjoy this benefit and therefore pose a potential risk to the patient. At least a substantial portion of the needle holder **250**, and part of the second end **224** as desired, is preferably formed of an x-ray transmissive material to prevent scattering for easier visualization of the interventional process. An acrylic material is preferred for use in the needle holder area of the subject apparatus. However, any other suitable easily sterilizable x-ray transmissive material can be used as desired. Also, the needle holder **250** may be coated with an x-ray transmissive material to enhance the grip of the holder on the tool **192** as desired.

FIGURES **3A** and **3B** show an alternative preferred embodiment of the subject needle holder **250'** including a set of tweezers-like arm portions **251**, **252**, and **253** adapted to grip the needle portion **193** of the biopsy needle **122** in a V-shaped groove **254** formed thereby. It is to be appreciated that the V-shaped groove enables needles or probes having a variety of diameters to be held by the holder while maintaining a single common central axis line relative to the needle guide apparatus **200**. Although three arm portions are shown, more arms having a similar configuration can be used as well for added precision and stability. In the form shown, the uppermost arm portion **251** and the lowermost arm portion **253** are adapted to engage the needle **193** on an opposite side from the central arm portion **252**. Each of the arm portions overlies each other in the vertical, or needle, direction so that the confronting arm portions can overlap in the vertical direction without mechanically interfering with each other for grasping needles having a small diameter. For larger needles, the arm

portions **251-253** do not overlap while in the grasped orientation, but rather engage the needle **193** at linear contact points established by the V-groove areas **254** such as illustrated in FIGURE **3B**.

FIGURE **4A** illustrates a cross-sectional view of the connector portion **210** of the subject guide apparatus **200**. In the embodiment illustrated, the connector portion **210** includes a linear slider **260** including an internal spring mechanism **262** to bias a lower end **264** of the connector portion supporting the main body **220** of the apparatus **200** against gravity relative to the distal end of the robot arm **190**. In its preferred form, the spring mechanism **262** has adequate spring force to compensate for the overall weight of the guide apparatus **200**. In that way, the guide apparatus is held in an unextended position until the interventionist actively pushes downwardly on the holding area **230**. Preferably, as illustrated in FIGURE **3**, the holding area **230** includes a set of stirrup-like handles **266** held in a selectable angular relationship relative to the first end **222** of the main body portion **220**. A set of large wing-nuts **268** or the like are provided for adjustment for ease and convenience of use.

FIGURE **4B** shows a cross-sectional view of another embodiment of the subject connector portion **210** in the form of a prism joint **270**. As with the linear slide joint **260** discussed above, the prism joint **270** permits only single degree of freedom movement. Thus, the joint provides for translation of the apparatus **200** and of the interventional biopsy needle **192** only along the planned trajectory **P**.

Preferably, in each of the connector areas **210** described above, a position feedback device **280** is provided for deriving a virtual display of the location of the biopsy needle **192** relative to the patient during an interventional procedure such as shown in FIGURE **5**. To that end, as the surgeon exerts manual force against the holding area of the apparatus, the needle is driven into the patient and feedback of needle movement relative to the distal end of the robot arm is provided to the scanner by the feedback device. Preferably, a resolver is provided using a gear connection or the like disposed between the fixed and movable parts of the apparatus **200**. However, a slide scale, linear wiper, or other such device can be used as well.

In accordance with a preferred embodiment, a diagnostic medical image or images of the region of interest of the subject **20** are obtained prior to conducting the interventional medical procedure. For example, where the procedure of interest is a tissue ablation procedure or a biopsy, pre-procedural or pre-operative images are obtained including axial slices or views which contain or are near the tumor or diseased anatomy. Optionally, the pre-operative

images or image data is obtained with the imaging apparatus **100**, or another diagnostic medical imaging device. Using the pre-operative image data, the interventionalist or other medical personnel plan the procedure via a virtual procedure planning system and/or method. The preferred example of virtual procedure planning is found in commonly owned U.S. Patent
5 No. 6,064,904 to Yanof, et al. which is included herein.

With reference to FIGURE **5**, the virtual procedure planning results in an image or images of the region of interest including superimposed therein a virtual surgical instrument, e.g., a virtual ablation probe or a virtual biopsy needle **300**, which is moved on the screen using a mouse pointer or the like to desired orientation and position relative to the pre-
10 operative images obtained. That is to say, the pre-operative images visualize the anatomy of interest **310**, and via the virtual planning, a virtual needle **300** or other medical instrument is superimposed or otherwise incorporated therein at the desired position and trajectory for carrying out the procedure. In the illustrated embodiment, the virtual needle **300** is defined by an entry or percutaneous insertion point **302**, a target point **304** and/or depth-to-target reading
15 **305**, and a needle trajectory **306** connecting the two points and/or an angulation reading. Collectively, the pre-operative or pre-procedural images with the virtual surgical or medical instrument depicted therein are referred to herein as the virtual and/or planning views **290-294**. In a preferred embodiment, the virtual planning views include the virtual needle **300** superimposed on a transverse axial slices or oblique plane containing the needle's trajectory. Using multi-planar reformatted (MPR) views, the needle's trajectory **306** is tracked in the
20 virtual planning view regardless of whether or not it is in the transverse axial plane. That is to say, the virtual planning view is optionally generated from volumetric data and it can therefore show the complete trajectory of the virtual needle **300** for any arbitrary orientation, unlike the actual images generated by the CT scanner which can for the most part only readily obtain
25 images of the transverse axial view. Accordingly, where the needle trajectory is not co-planar with the transverse axial view, visualization of the complete needle trajectory is not lost.

The virtual planning views are preferably loaded and/or maintained on the workstation or control console **150**, or alternately, it is maintained on a separate computer, workstation or console from which it may be displayed and/or viewed by the interventionalist.

30 With reference to FIGURE **6** and continuing reference to the preceding figures, an exemplary intra-operative procedure employing the system **10** will now be described. For purposes of this example, the procedure is a biopsy. Having appropriately positioned the

subject or patient **20** within the examination region **112** of the imaging apparatus **100**, the robotic arm **190** holding the biopsy needle **192** in the needle holder portion **250** of its gripper **240** is initially positioned and/or arranged such that the needle **192** corresponds to the virtual needle **300** in the virtual planning view, i.e., such that the actual needle's tip registers with the entry point **302** and the actual needle's orientation matches the planned trajectory **306**. Preferably, the robotic arm **190** automatically moves to its initial positioning and/or arrangement based upon position and orientation command signals generated by a program and derived from the virtual planning view constructed by the operator and maintained in the control console **150**. That is to say, the interventionalist or other operator sends (from the control console or otherwise) the virtual planning view or data to a robot controller **400** which controls the movement of the robotic arm **190** into the desired position and orientation accordingly. The robot controller **400** is optionally a dedicated processor or processing unit, incorporated in the control console, or otherwise.

The interventionalist then physically uses the needle guide apparatus **200** to drive the actual needle **192**, i.e., selectively advance and/or retract the needle **192** along its (the planned) trajectory during active CT fluoroscopy. That is to say, by manipulating the handle **266** of the guide apparatus **200**, the interventionalist imparts a desired amount or degree of movement of the needle **192**. This movement is measure by the feedback device **280** which generates a signal responsive or proportional thereto. The signal is communicated to a virtual view processing unit **410**. The virtual view processing unit **410** updates the position of the virtual needle **300** in the virtual planning view display on the monitor **152** by advancing and/or retracting the virtual needle **300** along the planned trajectory **306** in accordance with the amount indicated by the feedback signal **281**. Preferably, the virtual processing unit **410** continually updates the virtual planning view in this manner as the feedback signal varies due to manipulations of the needle guide apparatus **200**. Additionally, the feedback signal may be used to update the real-time CT fluoroscopy image/view (not shown) as desired. This would be useful when the real-time view update period is large. The attenuated needle image would be shown with a virtual needle appendage, the size of which is representative of a difference between the needle depth from the prior CT fluoroscopy update and the position signal derived from the feedback device **280**.

As with the robot controller **400**, the virtual processing unit **410** is optionally a dedicated processor or processing unit, incorporated in the control console **150**, or otherwise.

Optionally, the advancement and/or retraction of the virtual needle **300** is indicated in the virtual view by: adjusting the depth-to-target reading; selectively switching portions of a line between a dashed, dotted or otherwise broken line which represents the remaining trajectory **306** not occupied by the needle, and a solid line representing the virtual needle **300**; both of
5 the foregoing; or otherwise as appropriate. In this manner, the interventionalist can visualize the progression of the procedure without having to continually image the patient **20**, and hence, expose the patient **20** continually to the radiation beam **122**.

As described, in addition to monitoring the progress of the procedure via the virtual view, the interventionalist may intermittently, as desired or upon demand, conduct an intra-
10 operative imaging experiment **900** with the imaging apparatus **100** to obtain a real-time image which visualizes the actual procedure. Herein, these intra-operative images are referred to as the actual view. Inasmuch as the imaging is intermittent, the radiation exposure to the patient **20** is less than the exposure that would otherwise be experienced if the patient **20** were being continually imaged. Preferably, the actual view is displayed on the monitor **152** alongside the
15 virtual view. Accordingly, the interventionalist may consult the periodically updated actual view and reference it against the continually updated virtual view to ensure that the actual procedure is in fact progressing as indicated in the virtual view.

Having thus described the preferred embodiment(s), the invention is now claimed to be:

1. A system (10) for inserting a medical device (191) into a patient, the system including an imaging device (100) scanning the patient to generate a volumetric image data set of the patient, a human readable device (152) for displaying an image of the patient derived from said volumetric image data set, means for selecting a virtual trajectory (300, P) defining a path for inserting the medical device (191) into said patient, robotic means (190) on said imaging device and movable into selected positions relative to the imaging device, and a guide apparatus (200) to direct movement of the medical device (191) relative to the patient (20) disposed on the robotic means (100), the guide apparatus (200) comprising:

a connector portion (210) coupling the guide apparatus with the associated imaging device (100) at a distal end of the robotic means (190);

a main body portion (220) supported relative to the associated imaging device by the connector portion (210);

a gripping area (230) formed at a first end (222) of the main body portion (220), the gripping area (230) adapting the guide apparatus (200) for manual gripping by an associated operator; and,

a holding area (240) formed at a second end (224) of the main body portion (220), the holding area (240) being adapted to hold the medical device (191) in an orientation suitable for motion relative to said patient (20) along a selected linear path (P), the holding area (240) being operative to translate the medical device (191) along said selected linear path (P) in response to manual force applied by the associated human operator at said gripping area (230).

2. The system (10) according to claim 1, wherein the imaging device (100) is a CT scanner, an MRI scanner, a CCT scanner, a fluoroscope, a SPECT scanner, a PET scanner, or a combination of the foregoing.

3. The system (10) according to either of claims 1 and 2, wherein the medical device (191) is an ablation probe or a biopsy needle (192).

4. The system (10) according to any one of claims 1-3, wherein said means for selecting said virtual trajectory includes means for selecting a virtual target point (304) in said image of the patient by identifying a first coordinate in said image of the patient, and means for identifying a virtual path (306) extending from said selected virtual target point (304) and out from the body of the patient.

5. The system (10) according to any one of claims 1-4, wherein said robotic means (190) is adapted to move said guide apparatus (200) into a position whereat said medical device (191) is in an orientation suitable for motion relative to said patient (20) along said selected linear path (P) coincident with said virtual path (306) extending from said virtual target point (304) and out from the body of the patient.

6. The system (10) according to any of the previous claims, wherein said connector portion (210) of the guide apparatus (200) includes a one of a linear slide joint (260) and a prism joint (270).

7. The system according to any of the previous claims, further including:
a position feedback device (280) provided on said connector portion (210) of the guide apparatus (200) for providing a feedback signal indicating a position of the guide apparatus relative to the patient; and,

means for displaying an image of the medical device (190) as it is physically moved relative to the patient based upon said feedback signal, together with said image of the patient and said virtual path.

8. The system according to any of the previous claims, wherein the holding area (240) is formed of an x-ray transmissive material.

9. The system according to any of the previous claims, wherein the holding area (240) includes a set of tweezers-like arm portions (251, 252, 253) adapted to grip the medical device (191) in a V-shaped groove (254) formed by the arm portions.

10. A method of inserting a medical device (191) into a patient, the method comprising:

providing an imaging device (100) scanning the patient to generate a volumetric image data set of the patient;

providing a human readable device (152) for displaying an image of the patient derived from said volumetric image data set;

providing means for selecting a virtual trajectory (300, P) defining a path for inserting the medical device (191) into said patient;

providing robotic means (190) on said imaging device and movable into selected positions relative to the imaging device;

providing a guide apparatus (200) to direct movement of the medical device (191) relative to the patient (20) disposed on the robotic means (190), the guide apparatus (200) including a connector portion (210) coupling the guide apparatus with the associated imaging device (100) at a distal end of the robotic means (190); a main body portion (220) supported relative to the associated imaging device by the connector portion (210); a gripping area (230) formed at a first end (222) of the main body portion (220), the gripping area (230) adapting the guide apparatus (200) for manual gripping by an associated operator; and, a holding area (240) formed at a second end (224) of the main body portion (220), the holding area (240) holding the medical device (191) in an orientation suitable for motion relative to said patient (20) along a selected linear path (P), the holding area (240) being operative to translate the medical device (191) along said selected linear path (P) in response to manual force applied by the associated human operator at said gripping area (230); and,

inserting the medical device (191) into the patient by manually urging the guide apparatus (200) towards said patient.

11. The system (10) according to claim 1, wherein providing the imaging device (100) includes providing a CT scanner, an MRI scanner, a CCT scanner, a fluoroscope, a SPECT scanner, a PET scanner, or a combination of the foregoing.

12. The method according to either of claims 1 and 2, wherein the providing step includes providing an ablation probe or a biopsy needle (192).

13. The method according to any one of claims 1-3, wherein said providing means for selecting said virtual trajectory includes providing means for selecting a virtual target point (304) in said image of the patient by identifying a first coordinate in said image of the patient, and providing means for identifying a virtual path (306) extending from said selected virtual target point (304) and out from the body of the patient, and moving the medical device and apparatus (200) while performing said scanning of the patient.

14. The method according to any one of claims 1-4, further including, using said robotic means (190), moving said guide apparatus (200) into a position whereat said medical device (191) is in an orientation suitable for motion relative to said patient (20) along said selected linear path (P) coincident with said virtual path (306) extending from said virtual target point (304) and out from the body of the patient.


15. The method according to any of the previous claims, wherein providing said connector portion (210) of the guide apparatus (200) includes providing a one of a linear slide joint (260) and a prism joint (270).

16. The method according to any of the previous claims, further including:
providing a position feedback device (280) on said connector portion (210) of the guide apparatus (200) for generating a feedback signal indicating a position of the guide apparatus relative to the patient; and,


displaying an image of the medical device (190) as it is physically moved relative to the patient based upon said feedback signal, together with said image of the patient and said virtual path.

17. The method according to any of the previous claims, including forming the holding area (240) of an x-ray transmissive material.

18. The method according to any of the previous claims, wherein providing the holding area (240) includes providing a set of tweezers-like arm portions (251, 252, 253) adapted to grip the medical device (191) in a V-shaped groove (254) formed by the arm portions.

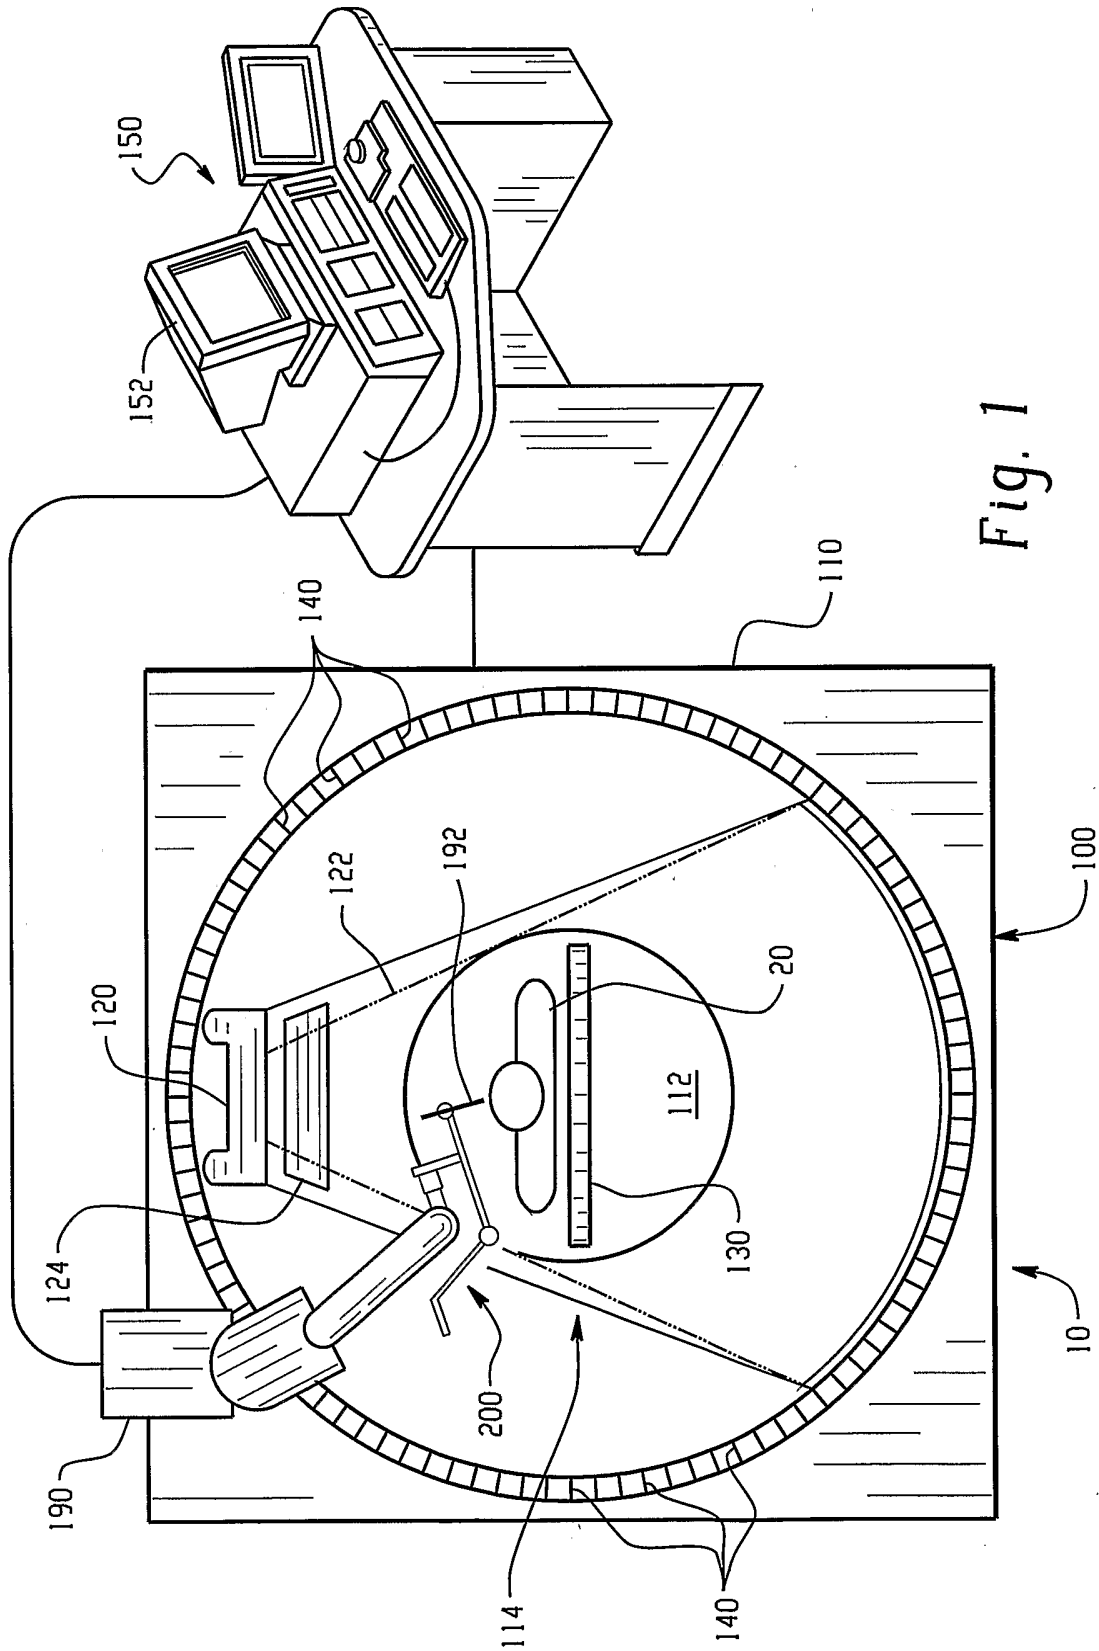

2/8

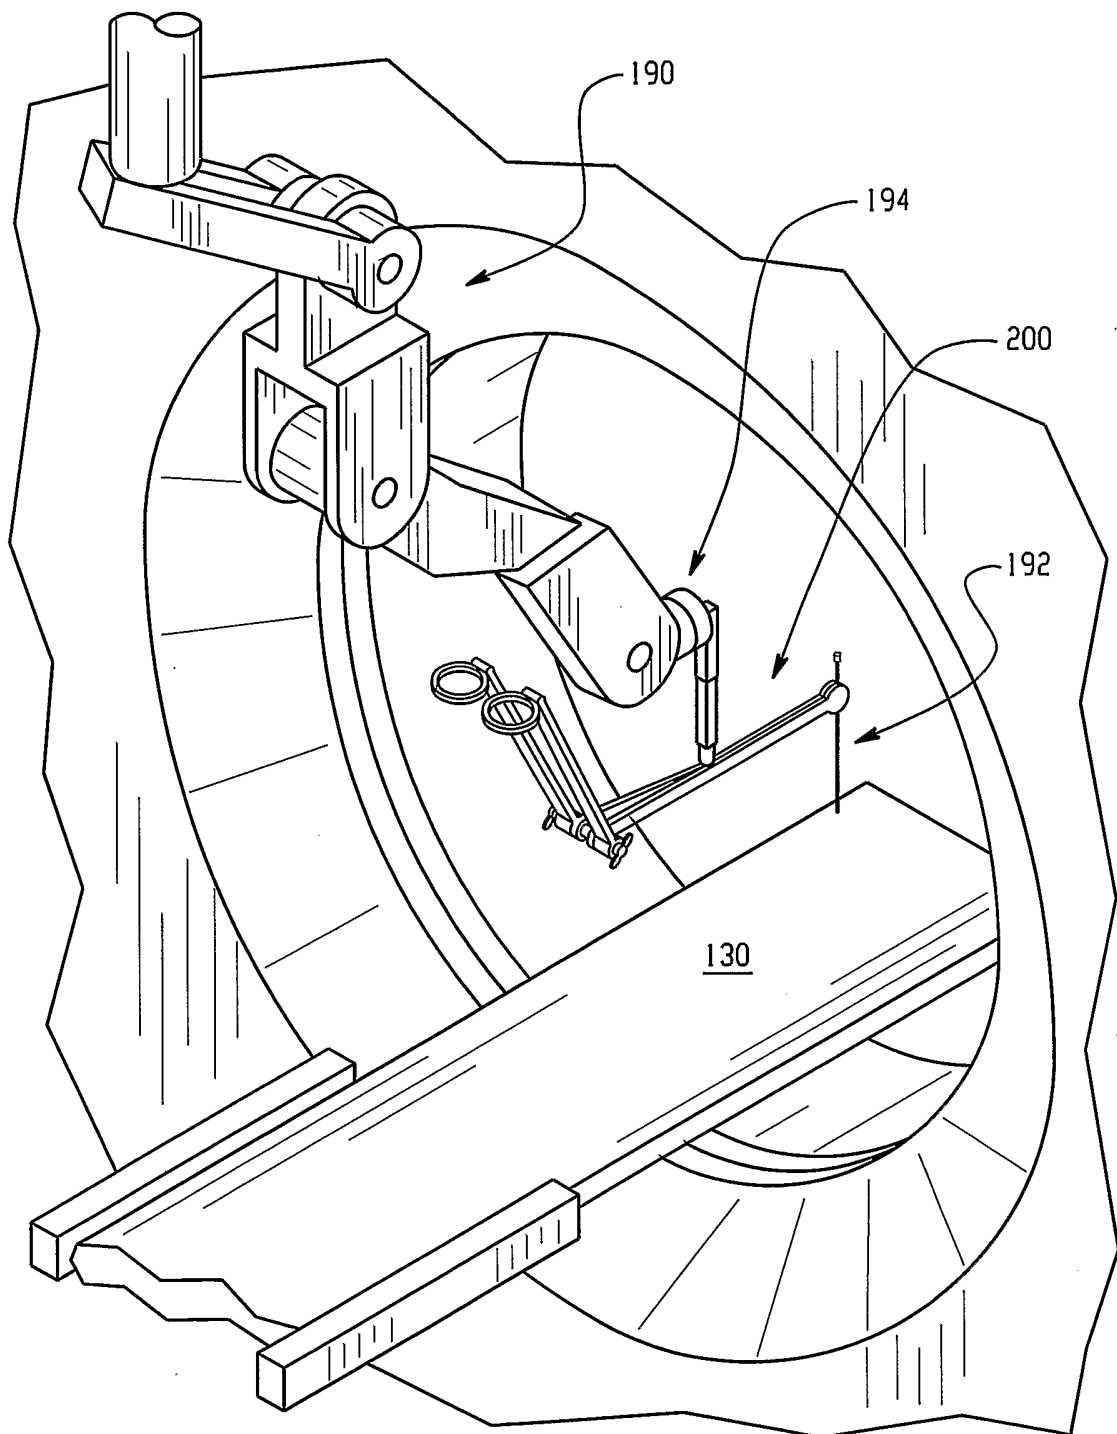*Fig. 2*

3/8

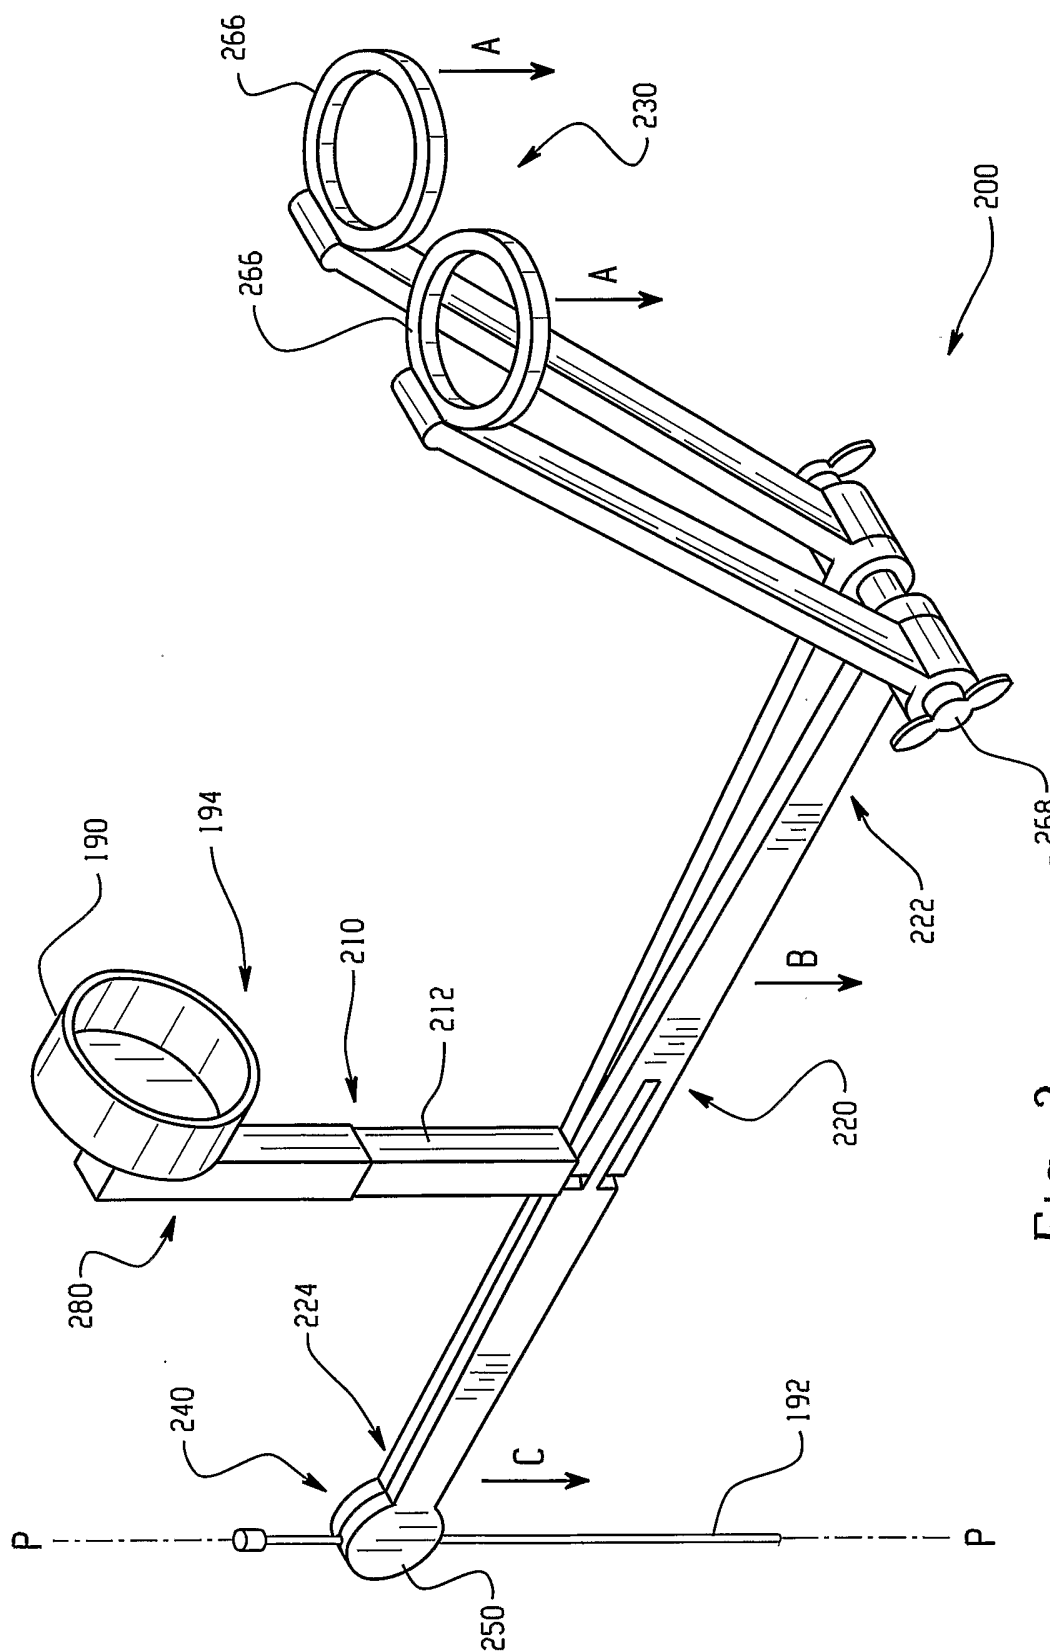


Fig. 3

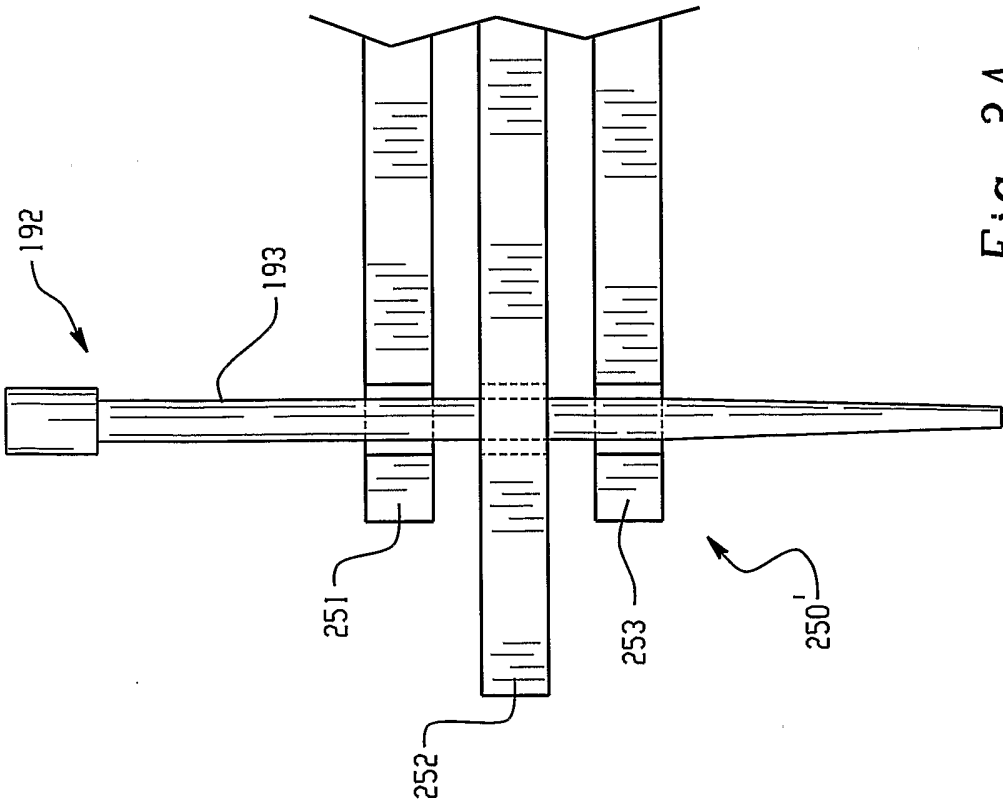


Fig. 3A

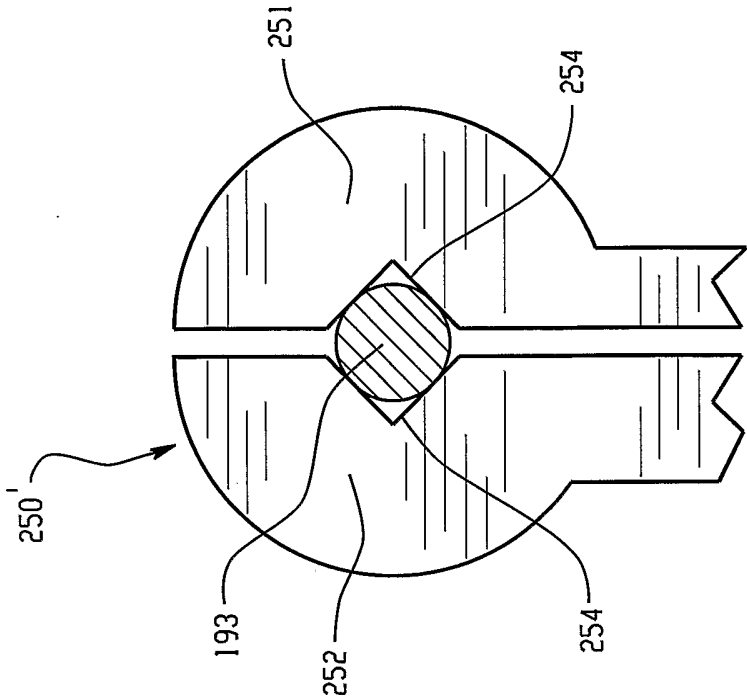
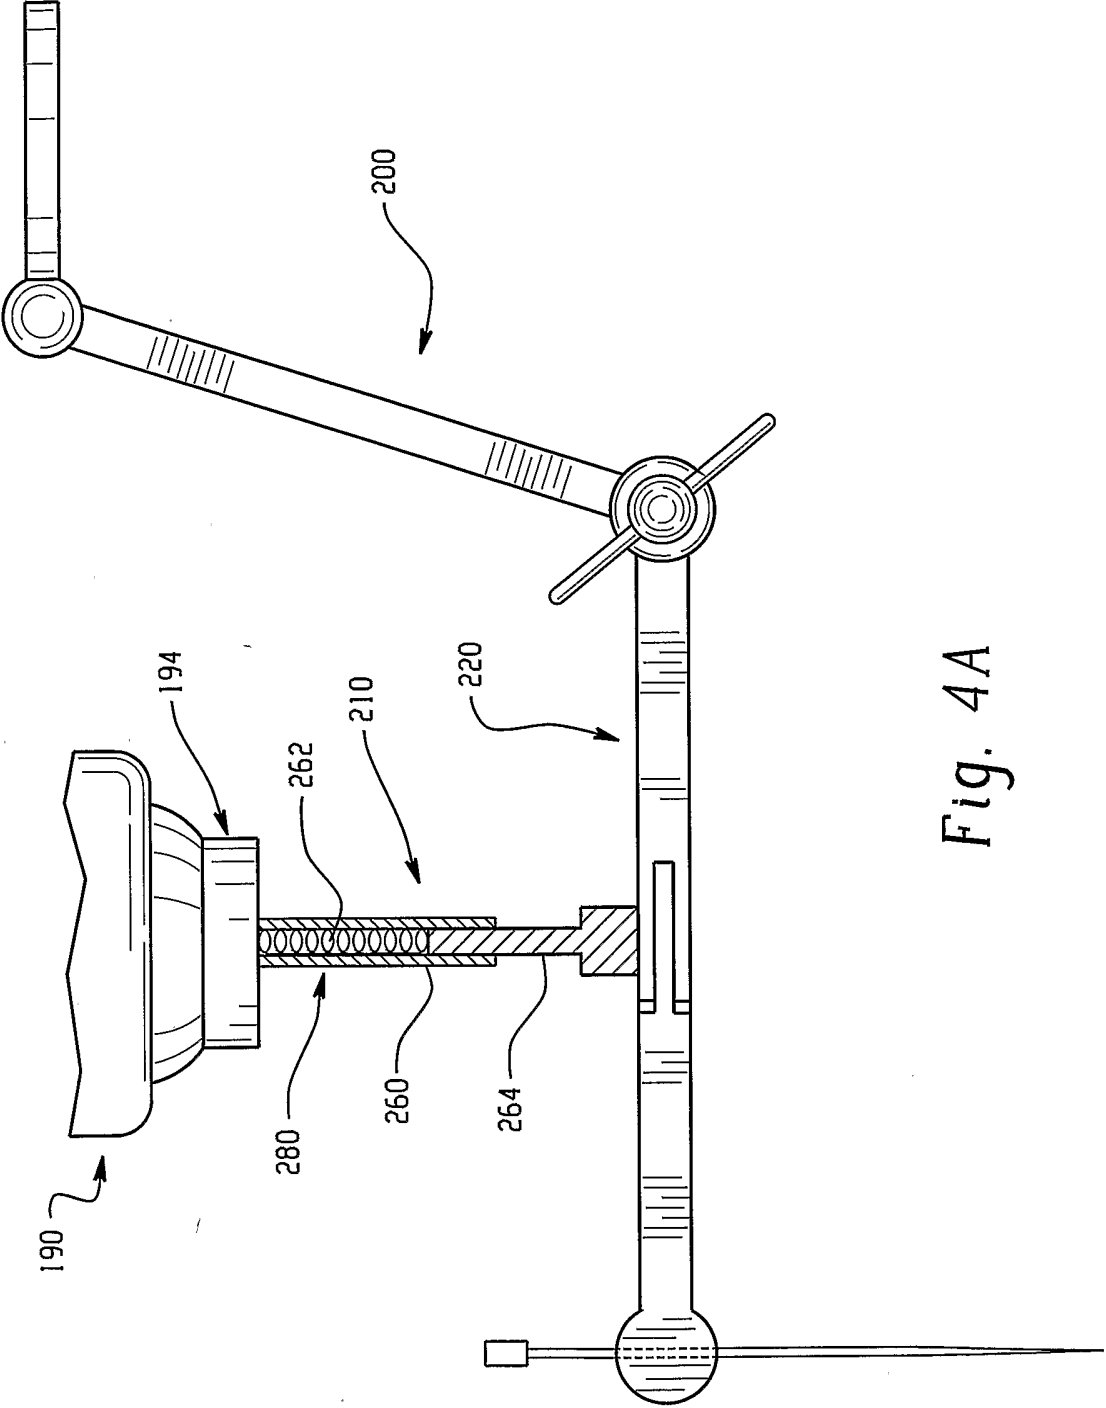


Fig. 3B



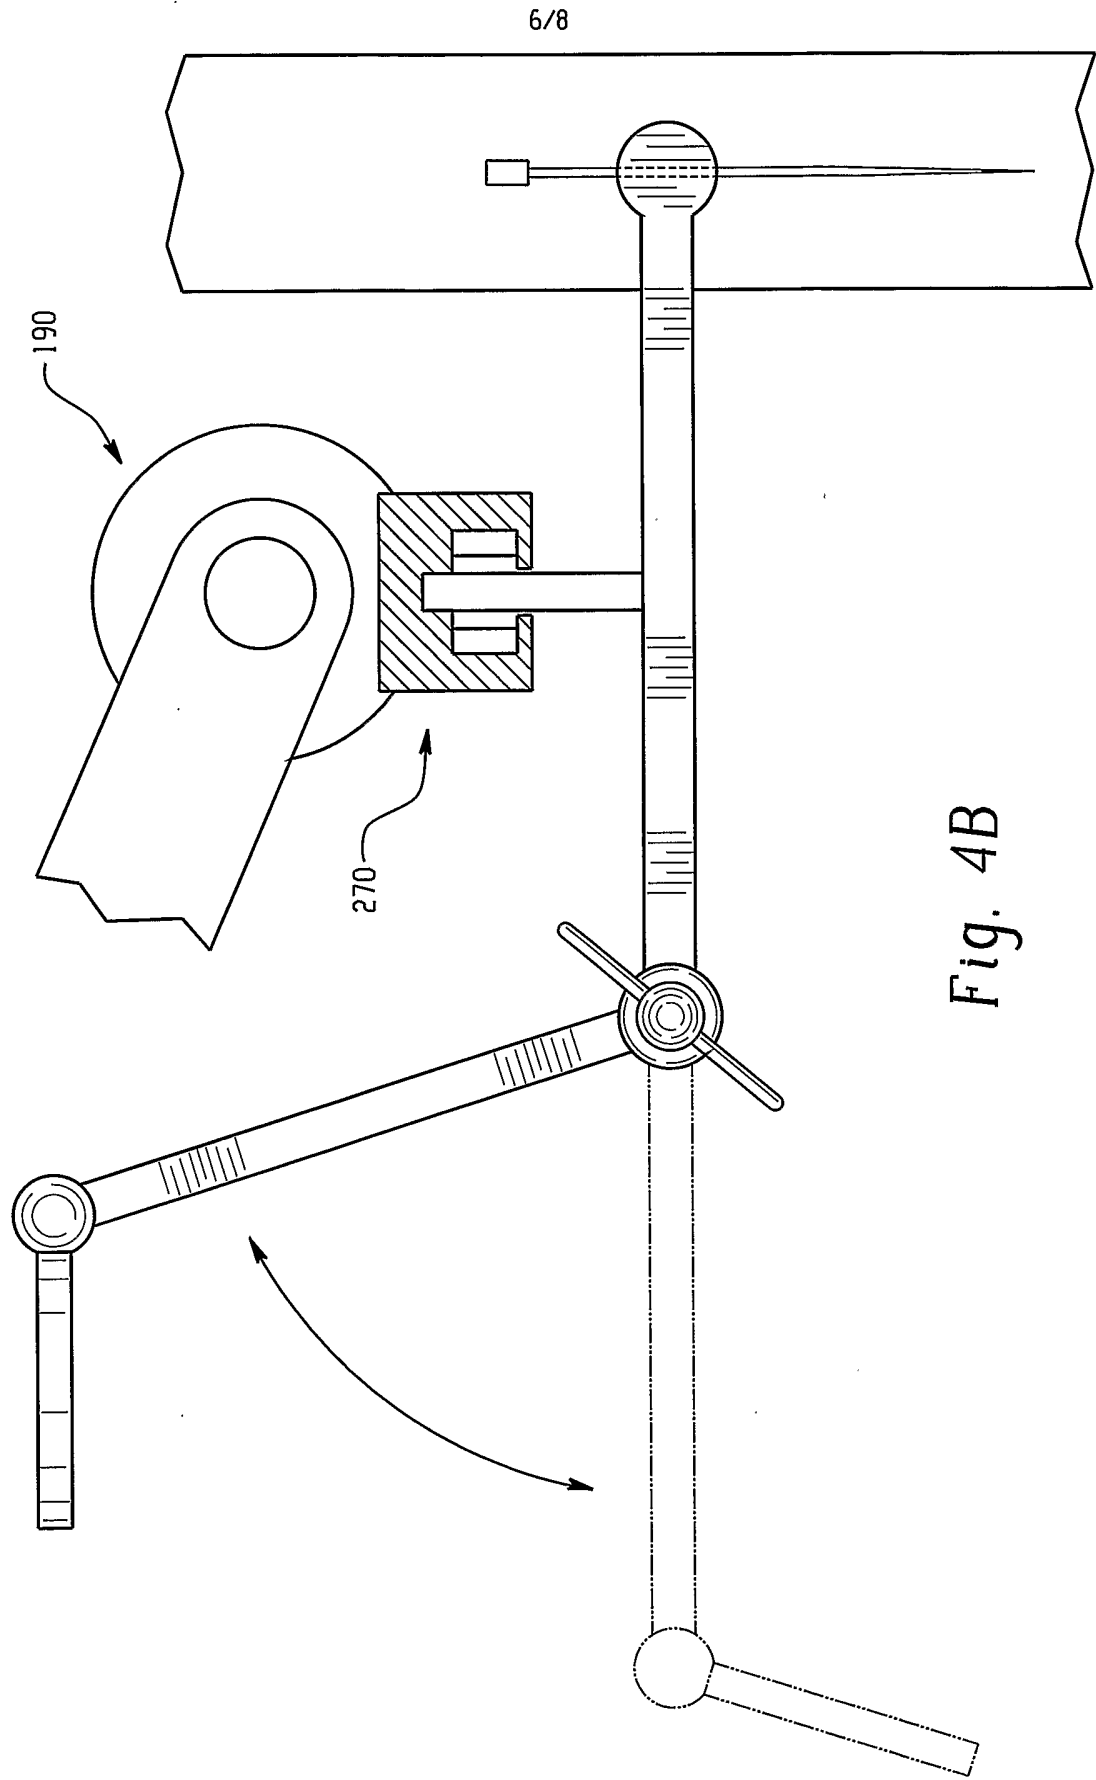
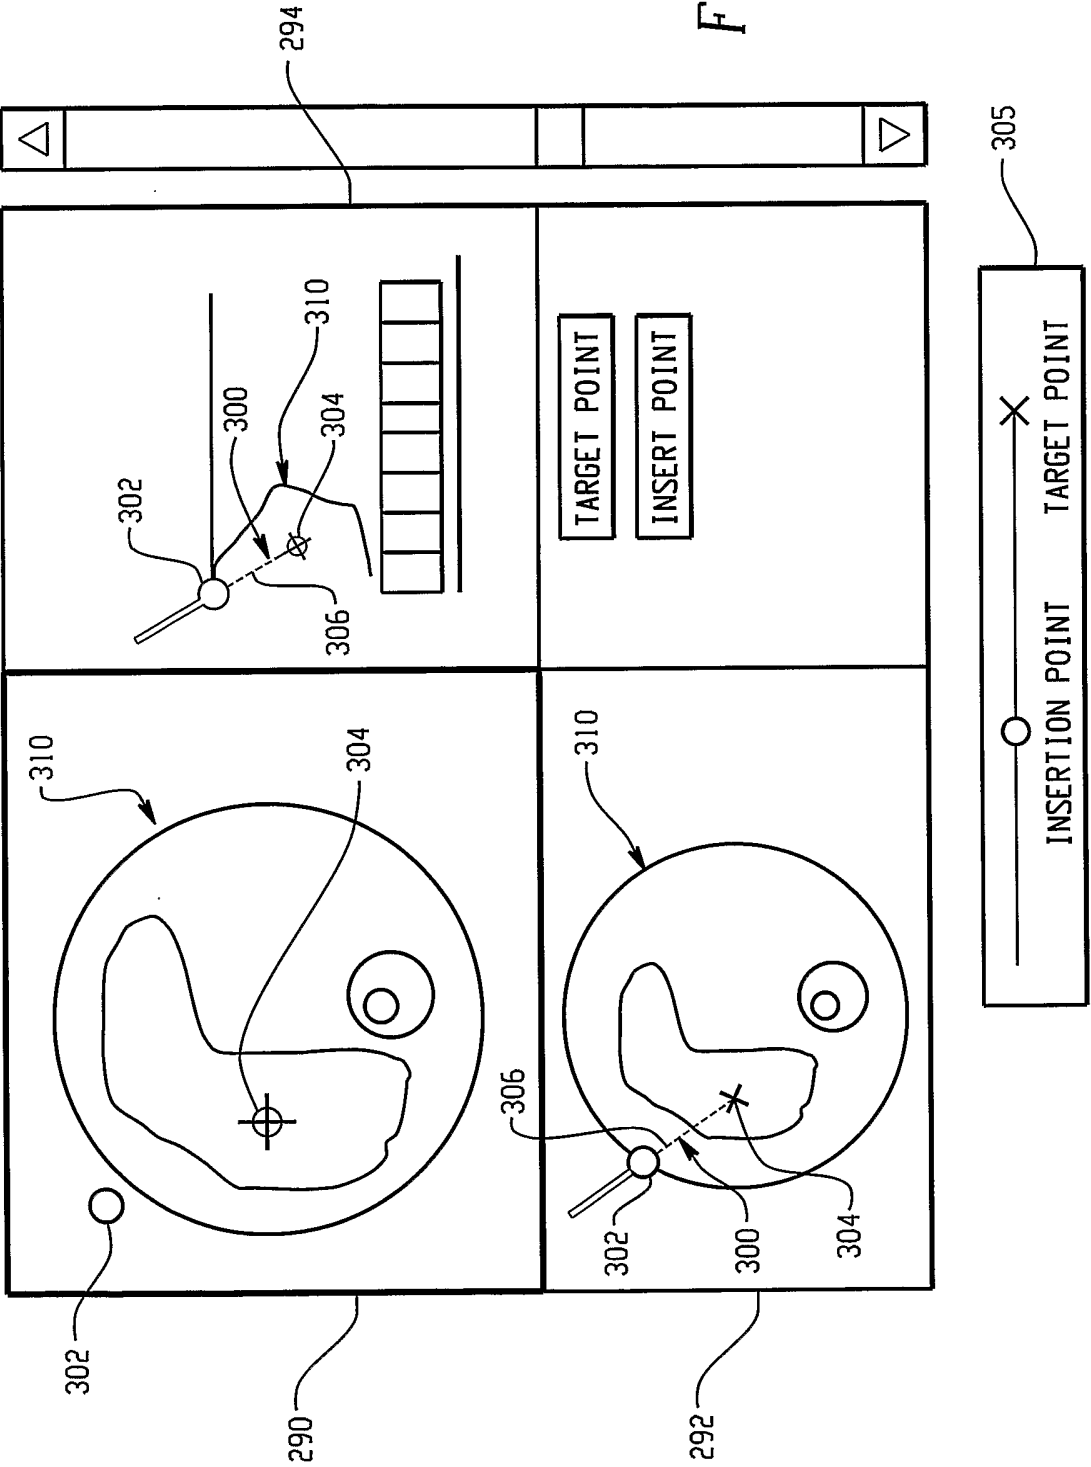


Fig. 4B



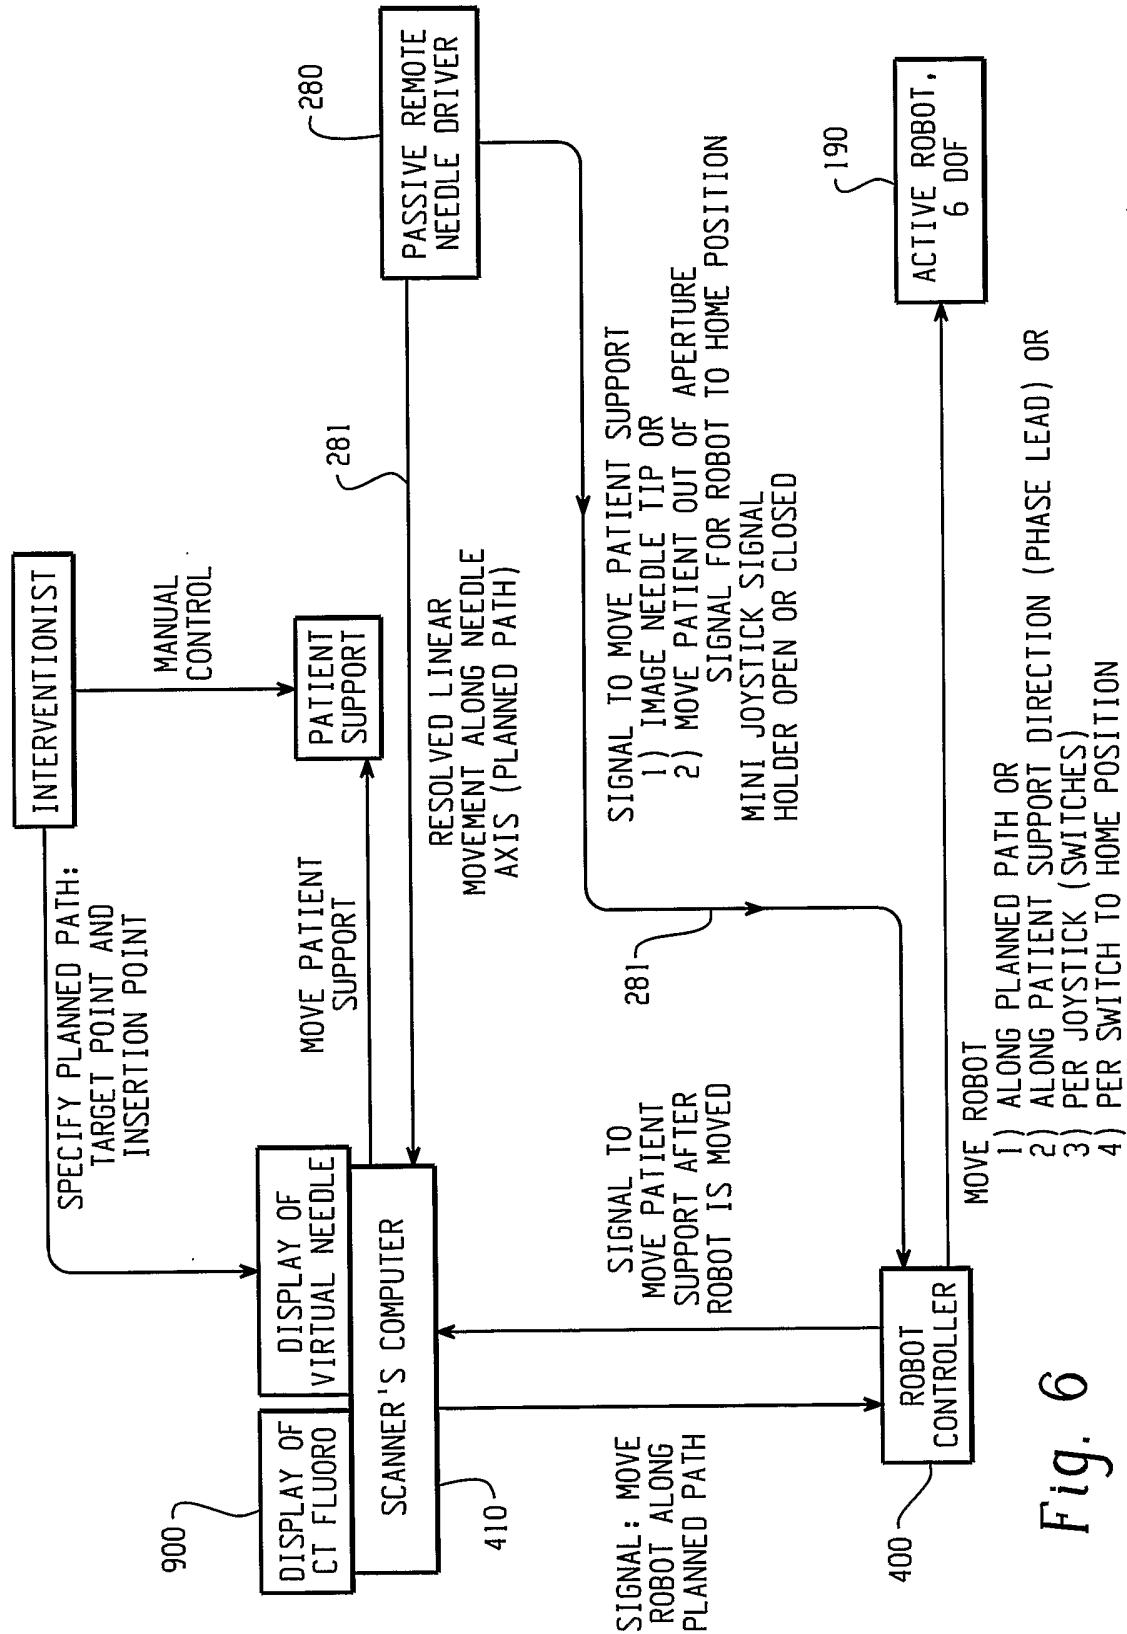


Fig. 6