



(22) Date de dépôt/Filing Date: 2006/06/29

(41) Mise à la disp. pub./Open to Public Insp.: 2006/12/30

(30) Priorité/Priority: 2005/06/30 (US11/171,679)

(51) Cl.Int./Int.Cl. *A61B 17/00* (2006.01),
A61F 2/84 (2006.01), *A61F 2/02* (2006.01),
A61F 2/88 (2006.01)


(71) Demandeur/Applicant:
CORDIS NEUROVASCULAR, INC., US

(72) Inventeurs/Inventors:
MITELBERG, VLADIMIR, US;
JONES, DONALD K., US;
LORENZO, JUAN A., US

(74) Agent: SIM & MCBURNEY

(54) Titre : DISPOSITIF DE MISE EN PLACE D'UNE SPIRE METALLIQUE POUR EMBOLISATION RESISTANTE A L'ETIREMENT AVEC MECANISME DE LIBERATION MECANIQUE

(54) Title: STRETCH RESISTANT EMBOLIC COIL DELIVERY SYSTEM WITH MECHANICAL RELEASE MECHANISM

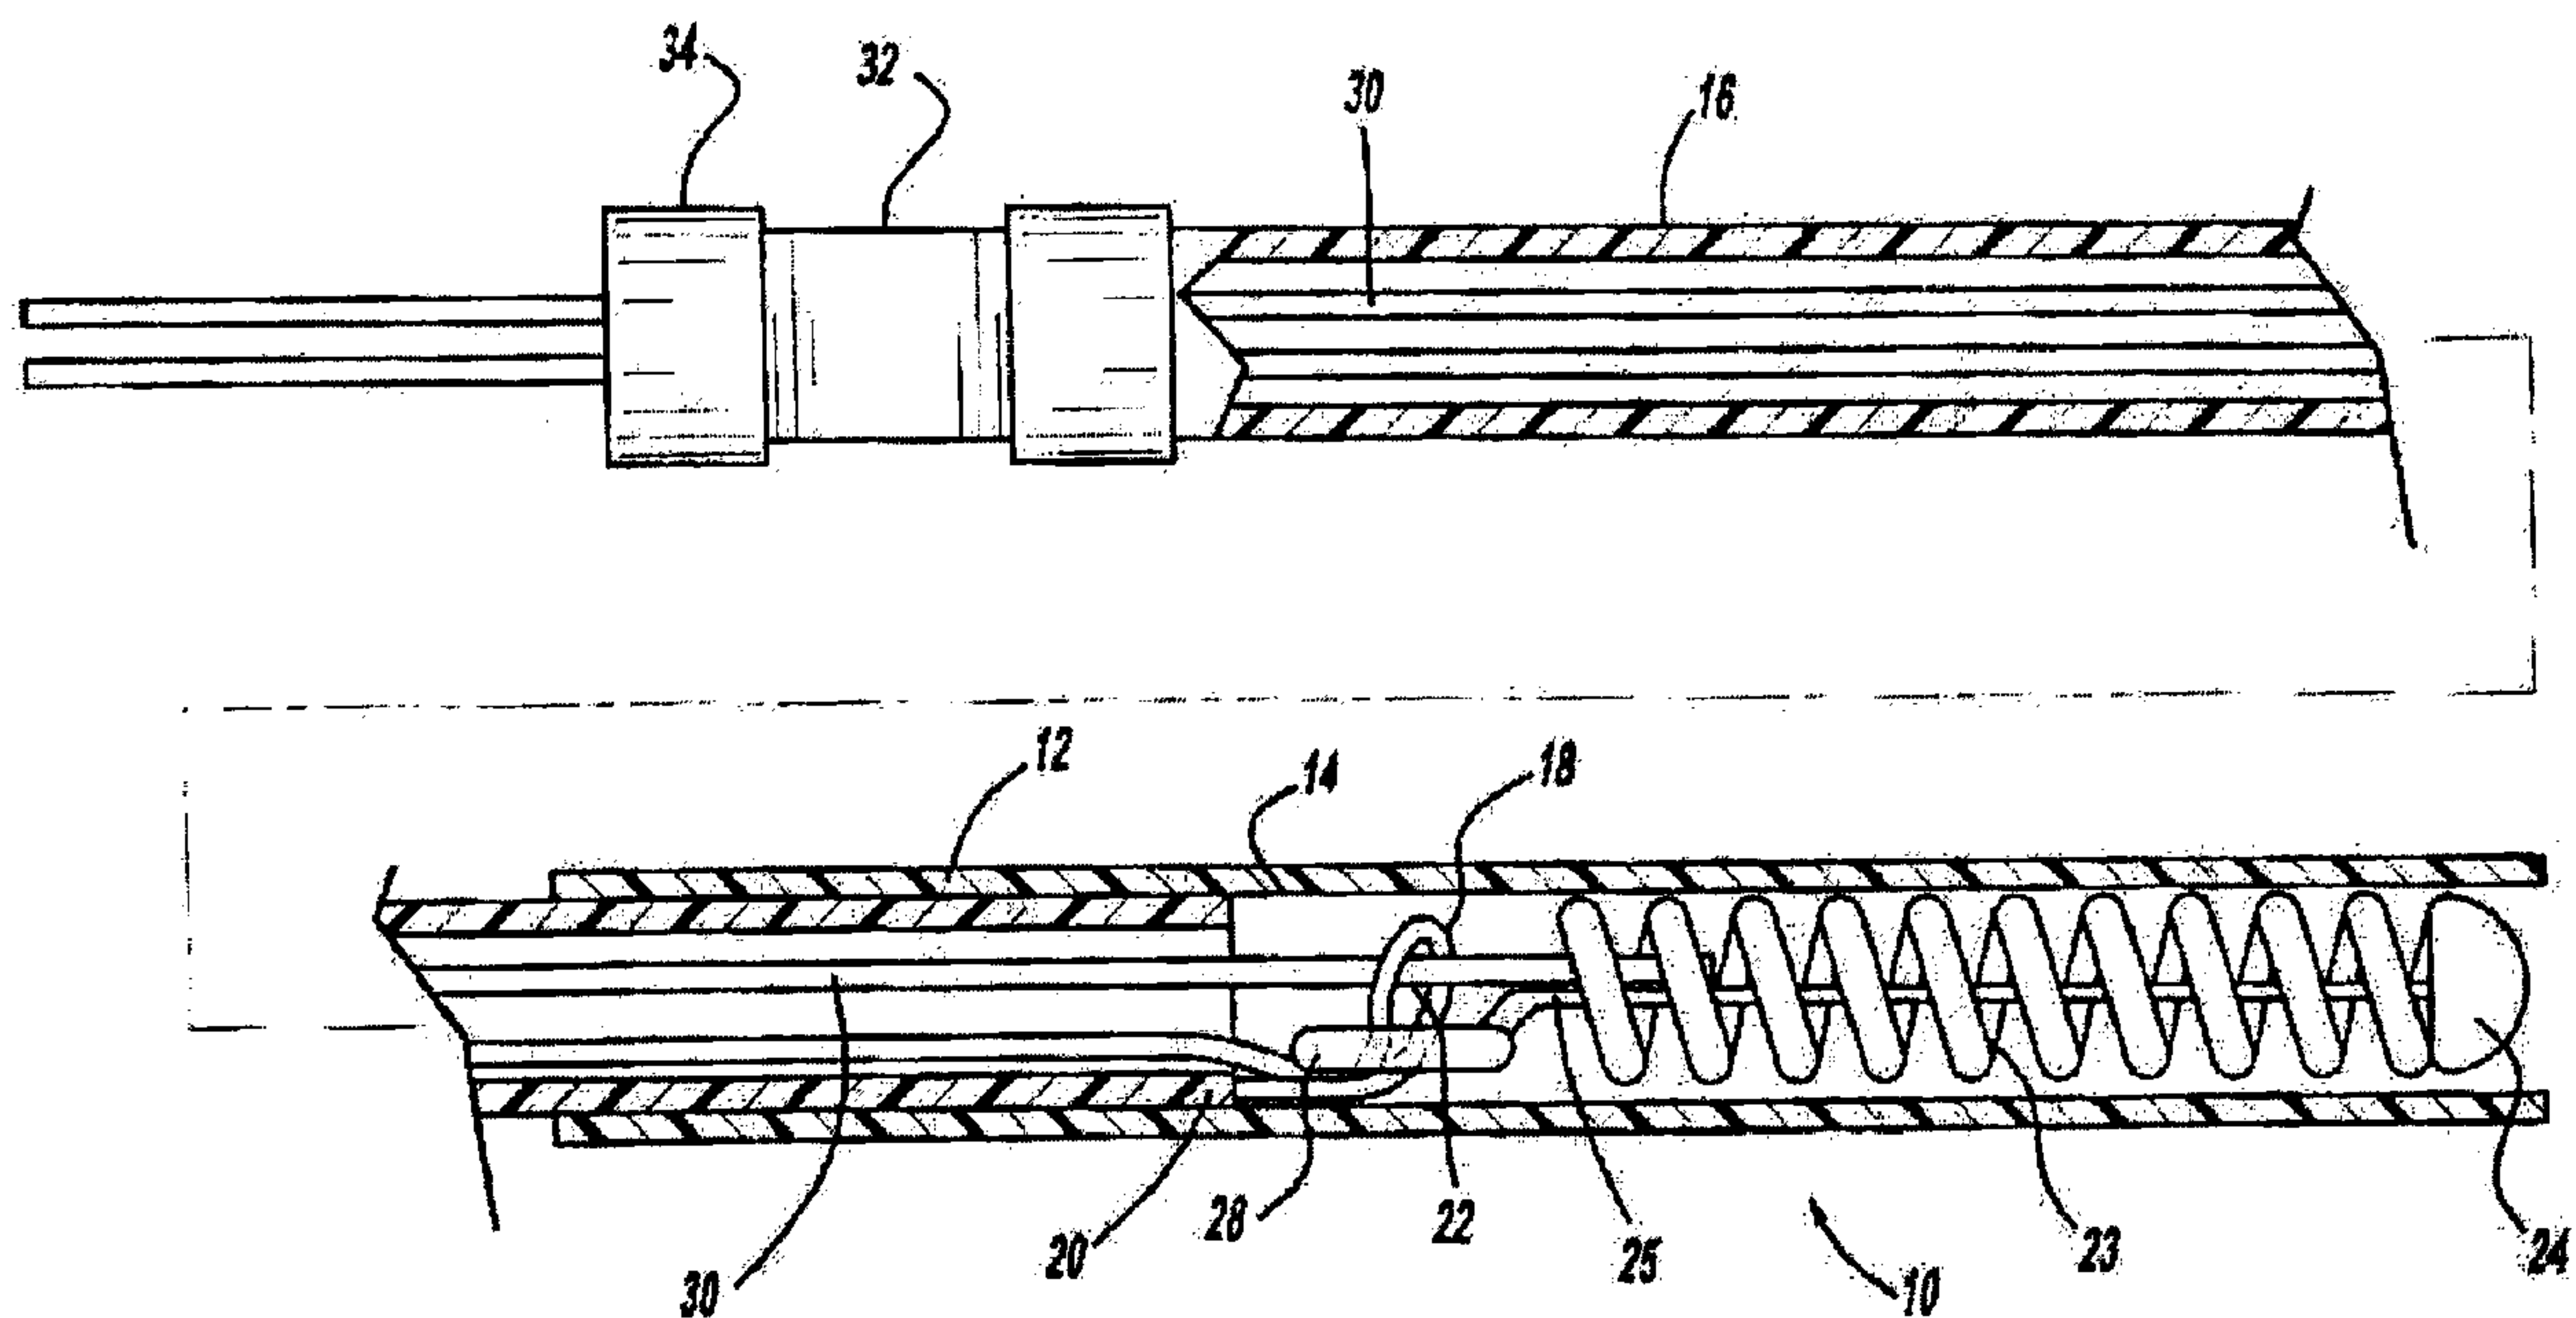

(57) Abrégé/Abstract:

A medical device for placing an embolic device at a predetermined site within a vessel of the body including a delivery catheter and a flexible pusher member having a lumen therethrough and being slidably disposed within the lumen of the catheter. A stretch resistant embolic device is retained within the delivery catheter by a mechanical interlocking mechanism which includes an engagement member which is attached to the distal end of the pusher member and extends through a retaining ring at the proximal end of the embolic device. A detachment member extends through an aperture at the distal end of the engagement member thereby locking the embolic device onto the pusher member. The engagement member engages a retaining ring on the embolic device. When the embolic device is advanced to the predetermined site within the vessel, the detachment member is withdrawn from the aperture to thereby release the embolic device at the treatment site.



**STRETCH RESISTANT EMBOLIC COIL DELIVERY
SYSTEM WITH MECHANICAL RELEASE MECHANISM**

Abstract

5 A medical device for placing an embolic device at a predetermined site within a vessel of the body including a delivery catheter and a flexible pusher member having a lumen therethrough and being slidably disposed within the lumen of the catheter. A stretch resistant embolic device is retained within the delivery catheter by a mechanical interlocking mechanism which includes an engagement member which is attached to the
10 distal end of the pusher member and extends through a retaining ring at the proximal end of the embolic device. A detachment member extends through an aperture at the distal end of the engagement member thereby locking the embolic device onto the pusher member. The engagement member engages a retaining ring on the embolic device. When the embolic device is advanced to the predetermined site within the vessel, the
15 detachment member is withdrawn from the aperture to thereby release the embolic device at the treatment site.

STRETCH RESISTANT EMBOLIC COIL DELIVERY SYSTEM WITH MECHANICAL RELEASE MECHANISM

BACKGROUND OF INVENTION

Cross-Reference to Related Applications(s)

This patent application is a continuation-in-part of U.S. patent application Serial No. 11/143,052 (Attorney Docket No. CRD5195USNPO), filed on June 2, 2005, entitled,
5 “Stretch Resistant Embolic Coil Delivery System With Mechanical Release Mechanism.”

Field of the Invention

The present invention relates to a medical device for placing a stretch resistant embolic device at a predetermined site within a vessel of the human body, and more
10 particularly, relates to a catheter-based deployment system for delivering an embolic device. This device is particularly suited to transport an embolic device, such as a stretch resistant embolic coil, through the tortious vasculature of the human brain to a selected site within the vessel or within an aneurysm.

15 Description of the Prior Art

For many years, flexible catheters have been used to place various devices within the vessels of the human body. Such devices include dilation balloons, radiopaque fluids, liquid medications, and various types of occlusion devices such as balloons and embolic

coils. Examples of such catheter-based devices are disclosed in U.S. Patent No. 5,108,407, entitled, "Method and Apparatus for Placement of an Embolic Coil" and U.S. Patent No. 5,122,136, entitled, "Endovascular Electrolytically Detachable Guidewire Tip For The Electroformation Of Thrombus In Arteries, Veins, Aneurysms, Vascular Malformations And Arteriovenous Fistulas." These patents disclose catheter-based devices for delivering embolic coils to preselected positions within vessels of the human body in order to treat aneurysms, or alternatively, to occlude blood vessels at a particular location.

Coils which are placed in vessels may take the form of helically wound coils, or alternatively, may take the form of randomly wound coils, coils wound within coils or other such coil configurations. Examples of various coil configurations are disclosed in U.S. Patent No. 5,334,210, entitled, "Vascular Occlusion Assembly" and U.S. Patent No. 5,382,259 entitled, "Vasoocclusion Coil with Attached Tubular Woven or Braided Fibrous Covering." Embolic coils are generally formed of a radiopaque metallic material, such as platinum, gold, tungsten, or alloys of these metals. Often, several coils are placed at a given location to occlude the flow of blood through the vessel, or aneurysm, by promoting thrombus formation at the particular site.

In the past, embolic coils have been placed within the distal end of a catheter. When the distal end of the catheter is properly positioned, the coil may then be pushed out of the end of the catheter with a pusher member to release the coil at the desired location. This procedure for placement of an embolic coil is conducted under fluoroscopic visualization such that the movement of the coil through the vasculature of the body may be monitored and the coil placed at the desired location.

Another procedure involves the use of glue or solder for attaching the coil to a guidewire, which in turn, is placed within a flexible catheter for positioning the coil within the vessel at a preselected position. Once the coil is in the desired position, the coil is held in position by the catheter and the guidewire is pulled proximally to thereby
5 cause the coil to become detached from the guidewire and released from the catheter. Such a coil positioning system is disclosed in U.S. Patent 5,263,964 entitled, "Coaxial Traction Detachment Apparatus and Method."

Still another coil positioning procedure is that of having a catheter with a socket at the distal end of the catheter for retaining a ball which is, in turn, bonded to the proximal
10 end of the coil. The ball, which is generally larger in diameter than the outside diameter of the coil, is placed in the socket within the lumen at the distal end of the catheter and the catheter is then moved into a vessel in order to place the coil at a desired position. Once the position is reached, a pusher wire with a piston at the end thereof is pushed distally from the proximal end of the catheter to push the ball out of the socket in order to
15 release the coil at the desired position. Such a system is disclosed in U.S. Patent No. 5,350,397, entitled, "Axially Detachable Embolic Coil Assembly."

Another procedure for placing an embolic coil within a vessel is that of using a heat releasable adhesive bond for retaining the coil at the distal end of the catheter. One such system uses laser energy transmitted through a fiber optic cable to apply heat to the
20 adhesive bond in order to release the coil from the end of the catheter. Such a procedure is disclosed in U.S. Patent No. 5,108,407, entitled "Method and Apparatus for Placement of an Embolic Coil."

Yet another coil deployment system incorporates a catheter having a lumen throughout the length of the catheter and a distal tip for retaining the coil for positioning the coil at a preselected site. The distal tip of the catheter is formed of a material which exhibits the characteristic that when the lumen of the catheter is pressurized the distal tip expands radially to release the coil at the preselected site. Such a deployment system is disclosed in U.S. Patent No. 6,113,622, entitled, "Embolic Coil Hydraulic Deployment System."

Still another coil deployment system incorporates an interlocking mechanism on the coil. The interlocking end on the embolic coil couples with a similar interlocking mechanism on a pusher assembly. A control wire which extends through the locking mechanism secures the coil to the pusher assembly. The pusher assembly and embolic coil are initially disposed within the lumen of a catheter. When the embolic coil is pushed out of the end of the catheter for placement, the control wire is retracted and the coil disengages from the pusher assembly. Such a deployment system is disclosed in U.S. Patent No. 5,925,059, entitled, "Detachable Embolic Coil Assembly."

Yet another coil deployment system incorporates an embolic device detachably mounted on the distal portion of a pusher member and held in place with a connector thread or fiber. The fiber passes through a cutter member that may be activated to cut the connector fiber. Once the connector fiber is cut, the embolic device is released. Such a deployment system is disclosed in Published U.S. Patent Application No. 2002/0165569, entitled, "Intravascular Device Deployment Mechanism Incorporating Mechanical Detachment."

Still another coil deployment system incorporates an embolic device with a stretch resistant member therethrough. The distal end of the stretch resistant member attaches to the embolic coil and the proximal end of the stretch resistant member is detachably mounted on the pusher member through various means such as adhesive, or
5 by a connector fiber adhered to or tied to the pusher member, and is detachable by the application of heat. Such a deployment system is disclosed in Published U.S. Patent Application No. 2004/0034363, entitled, "Stretch Resistant Therapeutic Device."

Still another coil deployment system incorporates a pusher wire with a stiff wavy-shaped end segment which is coupled to the embolic coil and is placed in the lumen of
10 the catheter. The coil is advanced through the catheter until it reaches a predetermined site in the vessel at which time the pusher wire is retracted and the embolic coil is released. Such a system is disclosed in U.S. Patent No. 6,203,547, entitled, "Vaso-occlusion Apparatus Having A Manipulable Mechanical Detachment Joint And A Method For Using The Apparatus."

15 A still further embolic device deployment system for placement of an embolic device, or coil, includes a delivery catheter and a flexible pusher member. The embolic device is retained by an interlocking mechanism which includes a detachment member which extends through an aperture in an engagement member which is attached to a pusher member. The engagement member engages a ring on the embolic device. When
20 the detachment member is withdrawn from the aperture of the engagement member, the embolic device is released. One such deployment system is disclosed in a United States patent application U.S. Serial No. 11/143,052, entitled, "Stretch Resistant Embolic Coil Delivery System With Mechanical Release Mechanism," filed on June 2, 2005 (Attorney

Docket No. CRD5195USNP0), and assigned to the same assignee as the present application.

SUMMARY OF THE INVENTION

5 The present invention is directed toward a vascular occlusive embolic device deployment system for use in placing a stretch-resistant embolic device at a predetermined site within a vessel which includes an elongated flexible deployment catheter, an elongated pusher member having a lumen extending therethrough and being slidably disposed within the lumen of the catheter. The embolic device takes the form of

10 an embolic coil defining a central lumen extending between the proximal and distal ends of the coil. A stretch resistant member, such as a platinum wire, having first and second ends in which the first end of the stretch resistant member is attached to the distal section of the coil and the second end of the stretch resistant member is attached to a retaining ring. An elongated engagement member, preferably comprising a fiber or filament

15 extending from a position proximal the pusher member, through the lumen in the pusher member to a position distal of the pusher member and looping back for attachment to the distal end of the pusher member to form a loop portion defining an aperture. The loop portion of the engagement member extends through the retaining ring of the embolic device. In addition, the deployment system includes an elongated detachment member

20 which extends from the proximal end of the pusher member, through the lumen of the pusher member and through the aperture of the engagement member such that when the detachment member is pulled proximally the distal end of the detachment member is

withdrawn from the aperture of the engagement member to thereby release the embolic device.

In accordance with another aspect of the present invention, there is provided a deployment system for use in placing an embolic device at a predetermined site within a vessel which includes an elongated flexible deployment catheter, an elongated pusher member being slidably disposed within the lumen of the catheter. The embolic device takes the form of an embolic coil defining a central lumen extending between the proximal and distal ends of the coil. A stretch resistant member having first and second ends in which the first end of the stretch resistant member is attached to the distal section of the coil and the second end of the stretch resistant member is attached to a retaining ring. An elongated engagement member preferably comprising a fiber or filament extending from a position proximal the deployment catheter, through the lumen in the deployment catheter to a position distal of the pusher member and looping back for attachment to the distal end of the pusher member to form a loop portion defining an aperture. The loop portion of the engagement member extends through the retaining ring of the stretch-resistant embolic device. In addition, the deployment system includes an elongated detachment member which extends from the proximal end of the catheter through the lumen of the catheter and through the aperture of the engagement member such that when the detachment member is pulled proximally the distal end of the detachment member is withdrawn from the aperture of the engagement member to thereby release the embolic device.

In accordance with another aspect of the present invention, the second end of the stretch-resistant member is attached to the proximal section of the coil, as opposed to the

retaining ring, to prevent the coil from stretching, and the proximal end of the coil is attached to the retaining ring.

In accordance with another aspect of the present invention, the loop portion of the engagement member extends through the retaining ring Such that the aperture formed by
5 the loop portion extends through the retaining ring with the result that when the detachment member extends through the aperture the retaining ring of the embolic device is interlocked onto the engagement member until the detachment member is withdrawn from the aperture.

In accordance with another aspect of the present invention, the aperture has a
10 central axis which extends substantially at a right angle to the central axis of the retaining ring. In addition, the embolic device takes the form of a helically wound embolic coil having a central axis which extends at a right angle to the central axis of the retaining ring. The stretch resistant member is attached to and extends from a distal section to a proximal section of the helically wound coil.

15 In accordance with still another aspect of the present invention, the embolic device takes the form of a helically wound coil formed of a plurality of turns of which one turn has a central axis which extends at a right angle to the central axis of the other turns to thereby form the retaining ring.

In addition, the vascular embolic device deployment system preferably includes a
20 retaining clamp mounted on the proximal end of the pusher member, and the detachment member and engagement member extend from a position proximal of the retaining clamp and through a lumen in the clamp in order that the detachment member and engagement member may be clamped in a fixed position prior to the release of the embolic device.

Upon release of the clamp, the detachment member may be withdrawn from the aperture of the engagement member to thereby release the embolic device.

BRIEF DESCRIPTION OF THE DRAWINGS

5 Figure 1 is an enlarged, partially sectional view of an embodiment of an embolic device deployment system in accordance with the present invention;

 Figure 1A is an enlarged, partially sectional view of a second embodiment of an embolic device deployment system in accordance with the present invention;

 Figures 2A, 2B and 2C are enlarged, sectional views, illustrating in more detail
10 the coil deployment system of Figure 1;

 Figures 3, 3A, 3B, and 3C are enlarged, sectional views of the coil deployment system shown in Figures 1 and 2 illustrating the sequential steps in the advancement of the embolic device, removal of a detachment member, and release of the embolic device.

DESCRIPTION OF THE PREFERRED EMBODIMENT

15 Figure 1 generally illustrates one embodiment of a vascular occlusive embolic device deployment system 10 which includes a sheath introducer 12 having a lumen 14 extending therethrough and having an elongated pusher member 16 slidably disposed within the lumen 14 of the sheath introducer 12. An elongated engagement member 18,
20 preferably comprising a fiber or filament extending from a position proximal the pusher member 16, through the lumen in the pusher member 16 to a position distal of the pusher member 16 and looping back for attachment to the distal end of the pusher member 16 to form a loop portion defining an aperture 22. The central axis of the aperture 22 extends

generally parallel to the axis of the pusher member 16. The engagement member 18 is preferably formed of a small diameter resilient wire, such as Nitinol, however, it may be formed from any flexible polymer, such as PTFE, or metallic fiber or wire.

The deployment system 10 also includes an embolic device 23, which as
5 illustrated, preferably takes the form of a helically wound embolic coil, which is disposed in the distal section of the sheath introducer 12. While the embolic device as illustrated is shown as a helically wound coil various other types of embolic devices, such as filaments, braids, foams, expandable meshes and stents, could be delivered using the present deployment system and various other coil configurations could be delivered using
10 this system. A weld, or solder, bead 24 is formed at the distal end of the embolic device 23 to provide an atraumatic tip for the embolic device. In addition, the distal end of a stretch-resistant member 25, which preferably takes the form of a platinum wire, is attached to the distal bead 24 and extends proximally through the central lumen of the coil. While the stretch-resistant member preferably takes the form of a platinum wire,
15 other materials or composites such as polymers, metals and ceramics, having a low elongation relative to the coil elongation may also be suitable. Alternatively, the distal end of the stretch-resistant member could be attached to the coil at a more proximal location in the distal section of the coil. The proximal end of the stretch resistant member is then attached to the edge of the retaining ring 28. Preferably, the retaining ring 28 has
20 a central axis which extends at right angles to the central axis of the sheath introducer 12 and also extends at right angles to the central axis of the helically wound embolic coil.

Figure 1A illustrates another variation of the stretch-resistant embolic device 23 in which the distal end of a stretch-resistant member 27 is attached to the bead 24 at the

distal end of the coil and the proximal end of the stretch-resistant coil is attached to the turns in the proximal section of the coil by use of a weld, or solder, bead 29. With this embodiment, the most proximal end of the coil is attached to the retaining ring 28.

As illustrated in Figures 1, 1A, 2A and 2B, the engagement member 18 extends in
5 a direction parallel to the central axis of the pusher member 16 and extends through the retaining ring 28 and is constrained in a generally L-shaped configuration by a detachment member 30. The elongated detachment member 30 extends from the proximal end of the deployment system 10 and through a lumen in the pusher member and then through the aperture 22 of the engagement member 18 and serves the function
10 of interlocking the embolic device 23 to the pusher member 16 until such time as the detachment member 30 is withdrawn proximally. Alternatively, the configuration of the pusher member 16 may include two or more lumens through which the engagement member 18 and the detachment member 30 are disposed within separate lumens. When the detachment member 30 is withdrawn from the aperture 22, the engagement member
15 18 returns to its normal configuration thereby releasing the retaining ring 28. The detachment member 30 preferably takes the form of a small diameter elongate filament, however, other forms such as wires or tubular structures are also suitable. While the detachment member 30 is preferably formed of nitinol, other metals and materials such as, stainless steel, PTFE, nylon, ceramic or glass fiber and composites may also be
20 suitable.

A Tuohy-Borst type of clamp 32 is mounted on the proximal end of the pusher member 16 and when tightened onto the detachment member 30 and onto the engagement member 18 and serves to prevent movement of the detachment member and

the engagement member 18 until such time as the clamping cap 34 is loosened to release the grip onto these members. Figure 2A and 2B illustrate the interlocking arrangement between the embolic device 23 and the pusher member 16 as shown in Figure 1, however, these latter figures illustrate the operation of the deployment system once the pusher member 16 has been moved distally to a position so that the distal end of the pusher member 16 extends slightly out of the distal end of the sheath introducer 12 or a delivery catheter thereby exposing the embolic device 23. As illustrated in Figure 2C, once the embolic device 23 has been moved out of the end of the sheath introducer 12 the detachment member 30 may be pulled proximally to withdraw the detachment member from the aperture 22 of the engagement member 18 to thereby cause the engagement member to disengage from the retaining ring 28 of the embolic device thereby releasing the embolic device 23 at a preselected position. In operation, once the embolic device 23 is properly positioned, cap 34 of the Touhy-Borst clamp 32 is loosened and the detachment member 30 is withdrawn proximally while holding the engagement member in a fixed position relative to clamp 32 thereby unsecuring the embolic device 23 for release. To enhance the release of the embolic device, the engagement member 18 may be subsequently withdrawn proximally. Alternatively, if desired, the detachment sequence described above and illustrated in Figures 2A, 2B and 2C may be executed while the embolic device 23 is still within the lumen of sheath introducer 12 or a delivery catheter.

One of the important advantages of the present invention is that the embolic device may be placed at a desired location within a vessel, or within an aneurysm, with the configuration of the device deployment system as shown in Figures 2A and 2B. If it is

determined that the embolic device is improperly positioned, the embolic device 23 may then be withdrawn from that location and placed at another location, or even removed from the body by first withdrawing the pusher member 16 and the embolic device totally back into the delivery catheter. Once the embolic device has been entirely withdrawn
5 back into the delivery catheter, the catheter may then be moved to a more desirable location and the embolic device may then be released at the new location. With the addition of the stretch resistant member 25, the embolic device may be withdrawn without concern that the coil will stretch and become very difficult to remove.

Figures 3, 3A and 3B generally illustrate the sequence of placing an embolic
10 device, such as a helical wound coil into an aneurysm 36 which extends from a vessel wall 38. More particularly, Figure 3 illustrates the vascular occlusive embolic device deployment system 10 in the same configuration as shown in Figure 1 after the pusher member and associated embolic device have been inserted into a delivery catheter 35 and advanced into a position for deployment of the embolic device 23, shown as a helical
15 embolic coil, into the aneurysm 36. Figure 3A illustrates the deployment device having a configuration similar to Figure 2A with the embolic device 23 being placed within the aneurysm 36 but prior to withdrawal of the detachment member 30. At this point, prior to the withdrawal of the detachment member 30, as previously mentioned, if it is determined that the embolic device has been improperly placed, the pusher member may
20 be withdrawn thereby withdrawing the embolic device back into the delivery catheter 35 for repositioning to a different location, or alternatively, to remove the embolic coil entirely from the body.

Figure 3B illustrates the deployment device after the detachment member 30 has been removed from the engagement member 18 thereby releasing the embolic device within the aneurysm 36, and Figure 3C illustrates the deployment device after the pusher member 16 has been withdrawn back into the delivery catheter 35 at the completion of
5 the procedure or alternatively in order to insert a second coil through the delivery catheter 35 and into the same aneurysm.

As is apparent, there are numerous modifications of the preferred embodiment described above which will be readily apparent to one skilled in the art, such as many variations and modifications of the embolic device including numerous coil winding
10 configurations, or alternatively other types of embolic devices. Also, there are many possible variations in the materials and configurations of the release mechanism. These modifications would be apparent to those having ordinary skill in the art to which this invention relates and are intended to be within the scope of the claims which follow.

CLAIMS

That which is claimed is:

1. A vasoocclusive embolic device deployment system for use in placing an embolic device at a predetermined site within a vessel comprising:

5 an elongated flexible deployment catheter having a lumen extending therethrough and having proximal and distal ends;

an elongated pusher member having a lumen extending therethrough and having proximal and distal ends and being slidably disposed within the lumen of the deployment catheter;

10 an embolic device which takes the form of an embolic coil being coupled to a retaining ring;

an elongated engagement member comprising a fiber extending from a position proximal the pusher member, through the lumen in the pusher member to a position distal of the pusher member and looping back for attachment to the distal end of the pusher member to form a loop portion defining an aperture, said loop portion of said engagement member extending through said retaining ring; and,

15

an elongated detachment member extending from a position proximal of the proximal end of the pusher member, through the lumen of the pusher member and through the aperture of the engagement member such that when the detachment member is pulled proximally the distal end of the detachment member is withdrawn from the aperture of the engagement member to thereby release the embolic device.

20

2. A vasoocclusive embolic device deployment system as defined in Claim 1, wherein
said embolic coil includes a central lumen extending between proximal and distal
sections of the coil, a stretch resistant member having first and second ends, said first end
of the stretch resistant member is attached to the distal section of the coil and the second
5 end of the stretch resistant member is attached to said retaining ring.

3. A vasoocclusive embolic device deployment system as defined in Claim 2, wherein
said fiber of the engagement member is formed of a wire.

10 4. A vasoocclusive embolic device deployment system as defined in Claim 3, wherein
said fiber of the engagement member is formed of a polymer.

5. A vasoocclusive embolic device deployment system as defined in Claim 1, wherein
said engagement member is formed of a nitinol wire.

15

6. A vasoocclusive embolic device deployment system as defined in Claim 5, wherein
said loop portion of said engagement member extends through the retaining ring of said
embolic device such that when said detachment member extends through said aperture,
said retaining ring of said embolic device is interlocked onto said engagement member
20 until the detachment member is withdrawn from said aperture.

7. A vasoocclusive embolic device deployment system as defined in Claim 2, wherein
said stretch resistant member is formed of a wire.

8. A vasoocclusive embolic device deployment system as defined in Claim 2, wherein said stretch resistant member is formed of a fiber.

9. A vasoocclusive embolic device deployment system as defined in Claim 2, wherein
5 the first end of said stretch-resistant member is attached to the distal end of the embolic coil.

10. A vasoocclusive embolic device deployment system for use in placing an embolic device at a predetermined site within a vessel comprising:

10 an elongated flexible deployment catheter having a lumen extending therethrough and having proximal and distal ends;

an elongated pusher member having proximal and distal ends and being slidably disposed within the lumen of the deployment catheter;

15 an embolic device which takes the form of an embolic coil being coupled to a retaining ring;

an elongated engagement member comprising a fiber extending from a position proximal the deployment catheter, through the lumen in the deployment catheter to a position distal of the pusher member and looping back for attachment to the distal end of the pusher member to form a loop portion defining an aperture, said loop portion of said
20 engagement member extending through said retaining ring; and,

an elongated detachment member extending from a position proximal of the deployment catheter, through the lumen of the catheter and through the aperture of the engagement member such that when the detachment member is pulled proximally the

distal end of the detachment member is withdrawn from the aperture of the engagement member to thereby release the embolic device.

11. A vasoocclusive embolic device deployment system as defined in Claim 10,
5 wherein said engagement member is formed of a nitinol wire.

12. A vasoocclusive embolic device deployment system as defined in Claim 11,
wherein said loop portion of said engagement member extends through the retaining ring
of said embolic device such that when said detachment member extends through said
10 aperture, said retaining ring of said embolic device is interlocked onto said engagement
member until the detachment member is withdrawn from said aperture.

13. A vasoocclusive embolic device deployment system as defined in Claim 12,
wherein a central axis of said aperture extends substantially at a right angle to a central
15 axis of said retaining ring.

14. A vasoocclusive embolic device deployment system as defined in Claim 13,
wherein said embolic coil includes a central lumen extending between proximal and
distal sections of the coil, a stretch resistant member having first and second ends, said
20 first end of the stretch resistant member is attached to the distal section of the coil and the
second end of the stretch resistant member is attached to said retaining ring.

15. A vasoocclusive embolic device deployment system as defined in Claim 14,
wherein said embolic device takes the form of a helically wound embolic coil.

16. A vasoocclusive embolic device deployment system as defined in Claim 15,
5 wherein said central axis of said retaining ring extends substantially at a right angle to a
central axis of said helically wound embolic coil.

17. A vasoocclusive embolic device deployment system as defined in Claim 16,
wherein said helically wound embolic coil is comprised of a plurality of turns of which
10 one of said plurality of turns has a central axis which extends substantially at a right angle
to a central axis of the other turns and forms the retaining ring.

18. A vasoocclusive embolic device deployment system as defined in Claim 10,
including a retaining clamp having a lumen extending therethrough and being mounted
15 on the proximal end of the pusher member, and wherein said detachment member extends
from a position proximal of said clamp and through the lumen of the clamp so that said
detachment member may be clamped into a fixed position prior to the release of the
clamp and withdrawal of the detachment member from the aperture of the engagement
member.

20

19. A vasoocclusive embolic device deployment system for use in placing an embolic
device at a predetermined site within a vessel comprising:

an elongated flexible deployment catheter having a lumen extending therethrough and having proximal and distal ends;

an elongated pusher member having a lumen extending therethrough and having proximal and distal ends and being slidably disposed within the lumen of the deployment
5 catheter;

an embolic device which takes the form of an embolic coil being coupled to a retaining ring;

an engagement member comprising a fiber having first and second ends attached to the distal end of the pusher member so as to form a loop portion having an aperture,
10 said loop portion of said engagement member extending through said retaining ring; and,

an elongated detachment member extending from a position proximal of the proximal end of the pusher member, through the lumen of the pusher member and through the aperture of the engagement member such that when the detachment member is pulled proximally the distal end of the detachment member is withdrawn from the
15 aperture of the engagement member to thereby release the embolic device.

20. A vasoocclusive embolic device deployment system as defined in Claim 19, wherein said embolic device takes the form of an embolic coil.

20 21. A vasoocclusive embolic device deployment system as defined in Claim 20, wherein said embolic device takes the form of a helically wound embolic coil.

22. A vasoocclusive embolic device deployment system as defined in Claim 19, wherein said engagement member is of an L-shaped configuration so as to form first and second legs, said first leg being attached to said pusher member and said second leg extending through said retaining ring.

5

23. A vasoocclusive embolic device deployment system as defined in Claim 22, wherein said aperture extends through the distal end of said second leg such that when said detachment member extends through said aperture said retaining ring of said embolic device is interlocked onto said engagement member until the detachment member is withdrawn from said aperture.

10

24. A vasoocclusive embolic device deployment system for use in placing an embolic device at a predetermined site within a vessel comprising:

an elongated flexible deployment catheter having a lumen extending therethrough

15 and having proximal and distal ends;

an elongated pusher member having proximal and distal ends and being slidably disposed within the lumen of the deployment catheter;

an embolic device which takes the form of an embolic coil defining a central lumen extending between the proximal and distal sections of the coil, a stretch-resistant member having first and second ends, said first end of the stretch resistant member is attached to the distal section of the coil and the second end of the stretch resistant member is attached to a retaining ring;

20

an engagement member fixedly attached to the distal end of the pusher member and having an aperture extending through the distal end thereof; said engagement member extending through said retaining ring of the embolic device; and,

an elongated detachment member extending from a position proximal of the deployment catheter, through the lumen of the catheter and through the aperture of the engagement member such that when the detachment member is pulled proximally the distal end of the detachment member is withdrawn from the aperture of the engagement member to thereby release the embolic device.

25. A vasoocclusive embolic device deployment system as defined in Claim 24, wherein said engagement member is of an L-shaped configuration so as to form first and second legs, said first leg being attached to said pusher member and said second leg extending through said retaining ring.

26. A vasoocclusive embolic device deployment system as defined in Claim 25, wherein said aperture extends through the distal end of said second leg such that when said detachment member extends through said aperture said retaining ring of said embolic device is interlocked onto said engagement member until the detachment member is withdrawn from said aperture.

27. A vasoocclusive embolic device deployment system as defined in Claim 26, wherein a central axis of said aperture extends substantially at a right angle to a central axis of said retaining ring.

28. A vasoocclusive embolic device deployment system as defined in Claim 27,
wherein said embolic device takes the form of an embolic coil.

29. A vasoocclusive embolic device deployment system as defined in Claim 28,
5 wherein said embolic device takes the form of a helically wound embolic coil.


30. A vasoocclusive embolic device deployment system as defined in Claim 29,
wherein said central axis of said retaining ring extends substantially at a right angle to a
central axis of said helically wound embolic coil.


10

31. A vasoocclusive embolic device deployment system as defined in Claim 30,
wherein said helically wound embolic coil is comprised of a plurality of turns of which
one of said plurality of turns has a central axis which extends substantially at a right angle
to a central axis of the other turns and forms the retaining ring.

15

32. A vasoocclusive embolic device deployment system as defined in Claim 24,
including a retaining clamp having a lumen extending therethrough and being mounted
on the proximal end of the pusher member, and wherein said detachment member extends
from a position proximal of said clamp and through the lumen of the clamp so that said
20 detachment member may be clamped into a fixed position prior to the release of the
clamp and withdrawal of the detachment member from the aperture of the engagement
member.

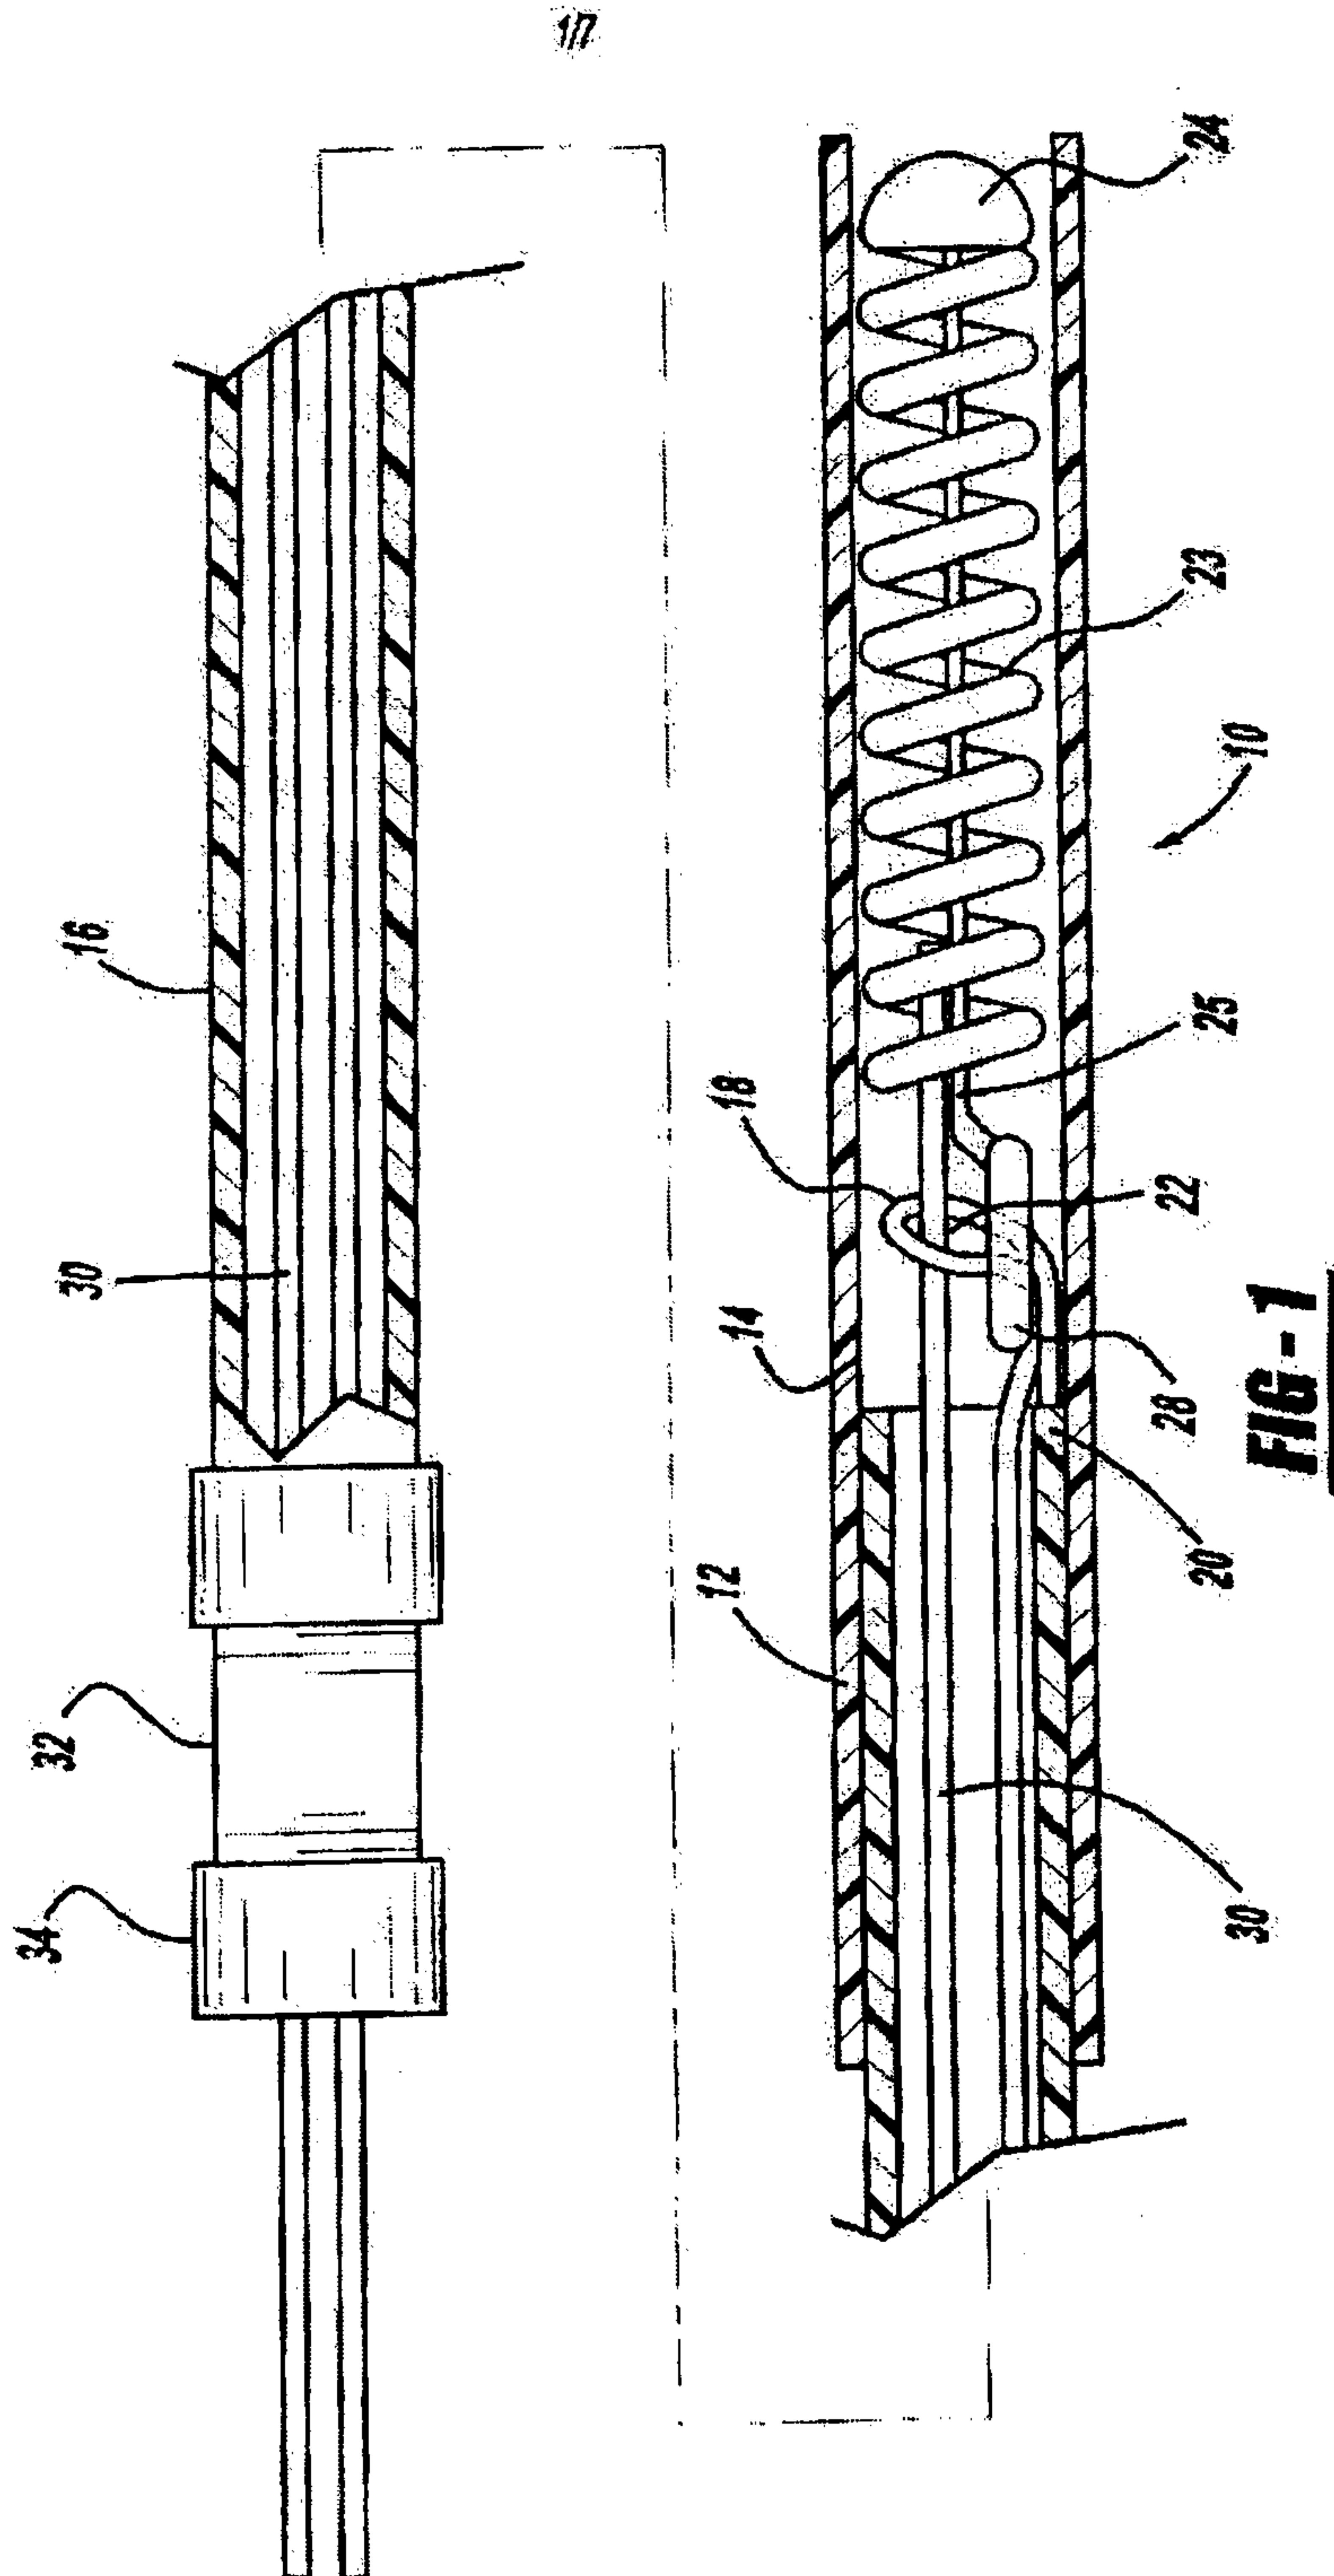

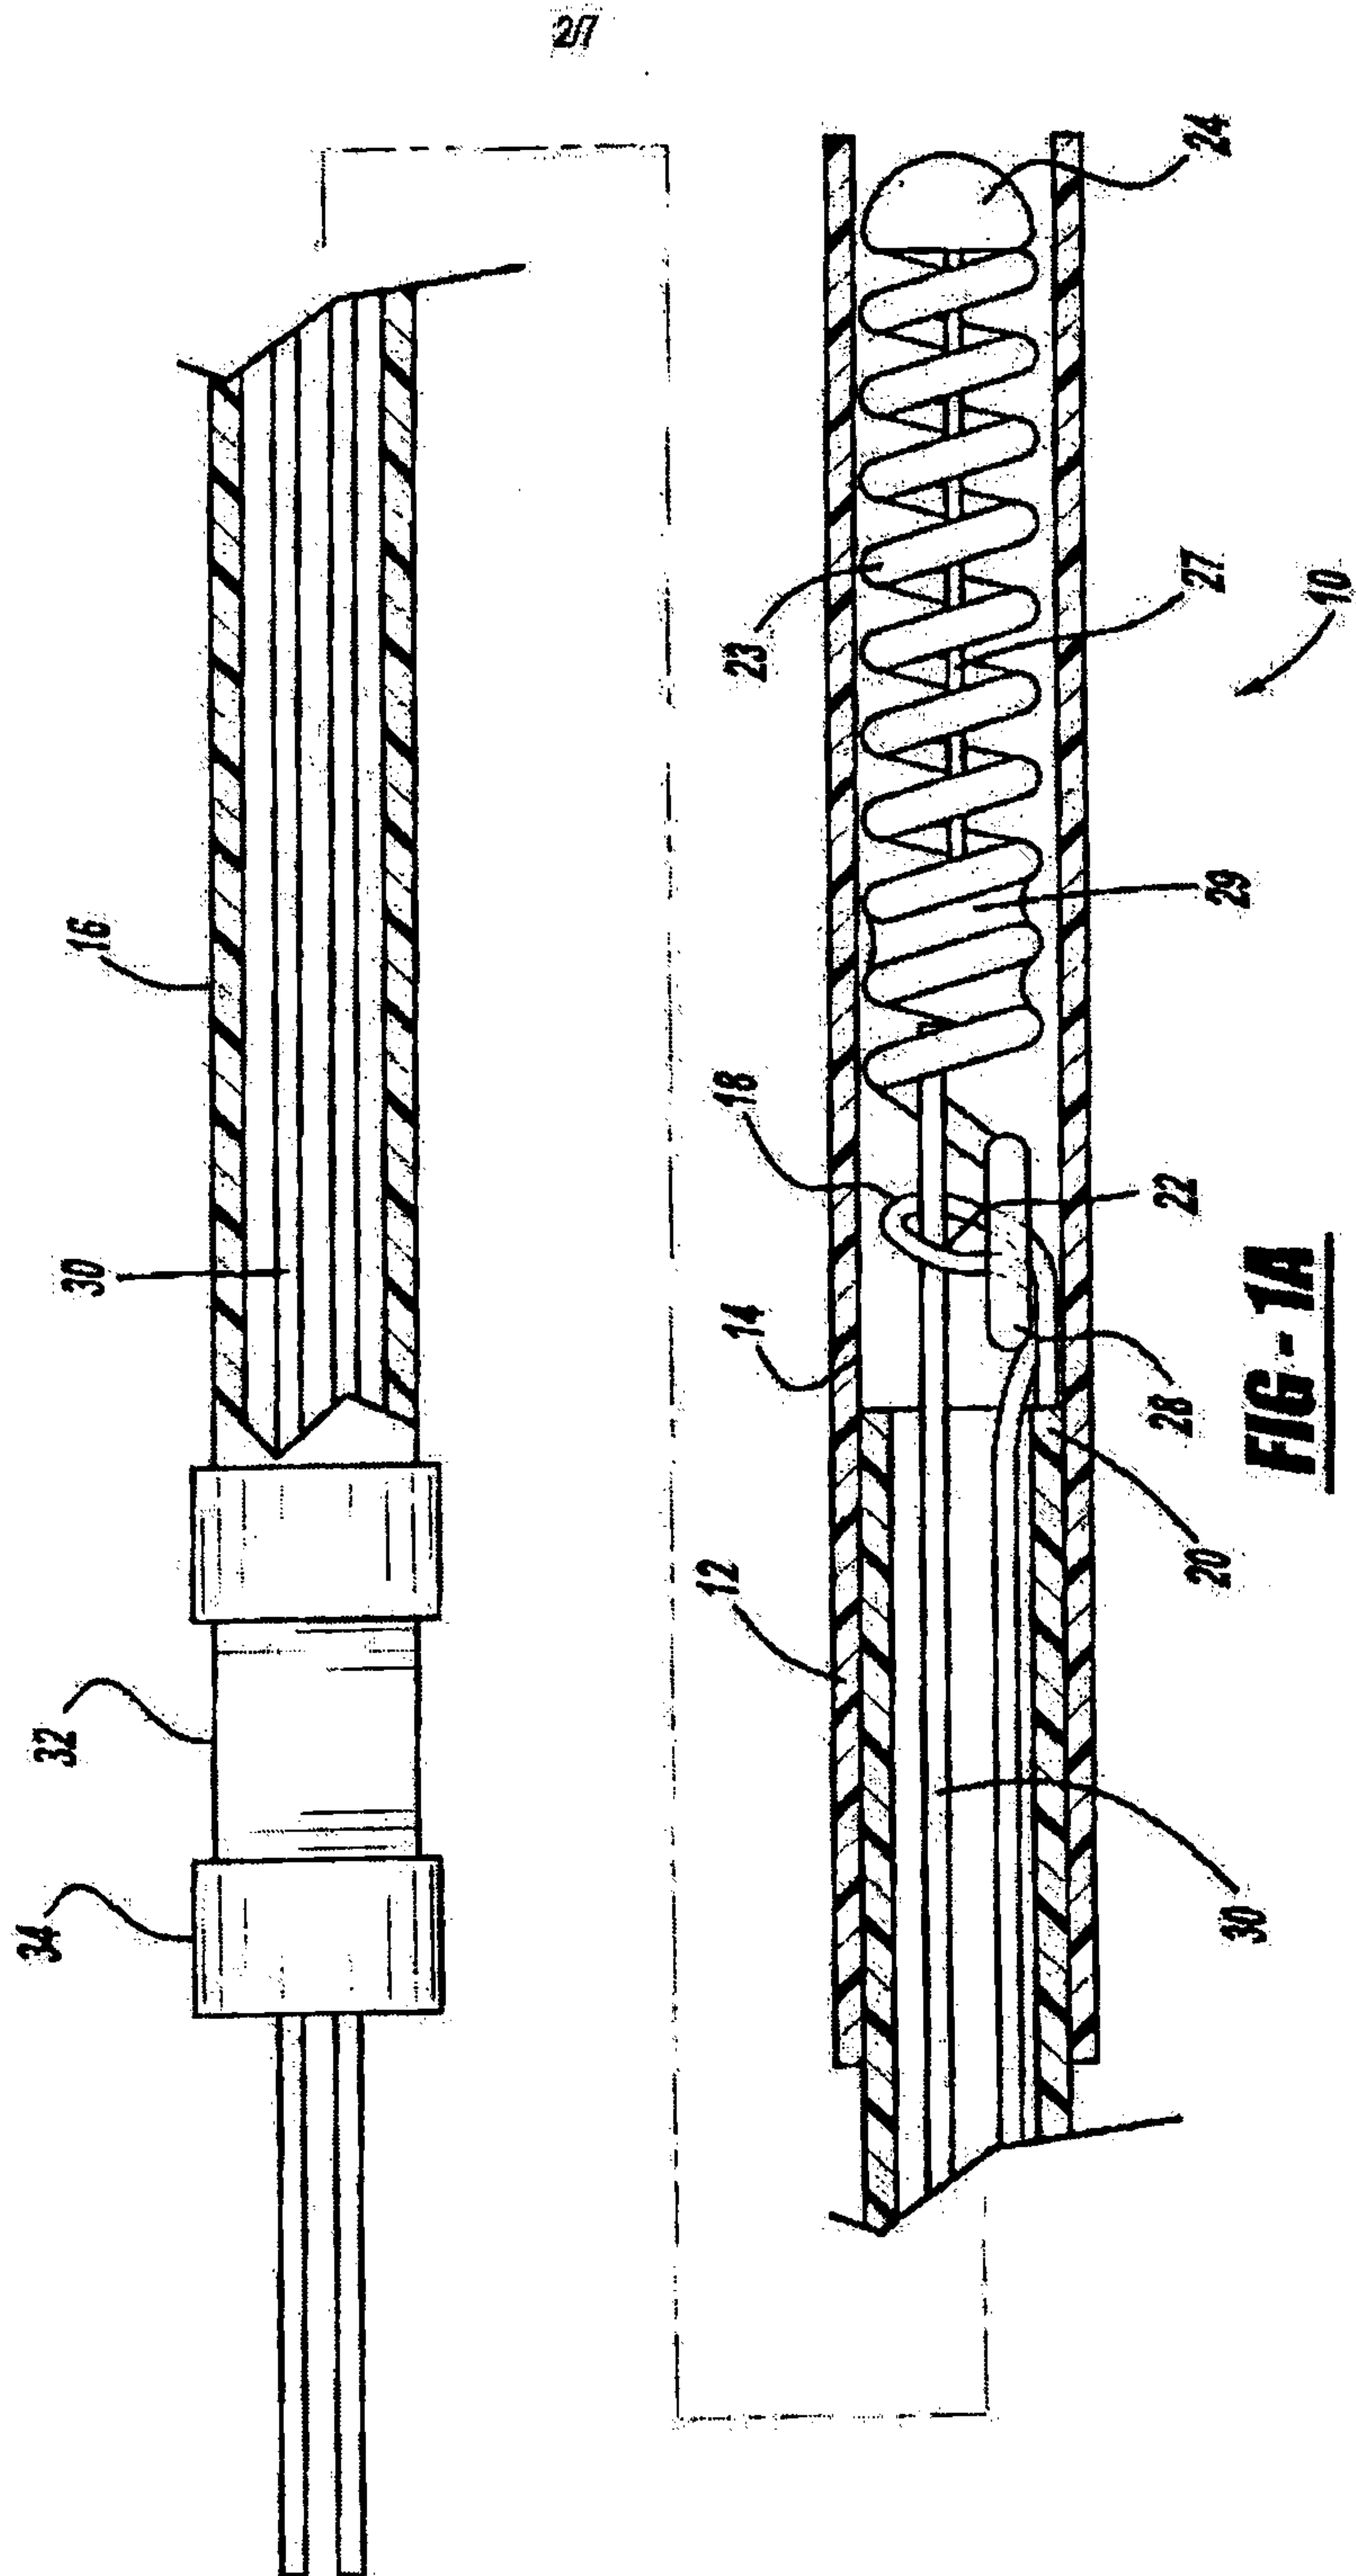

37

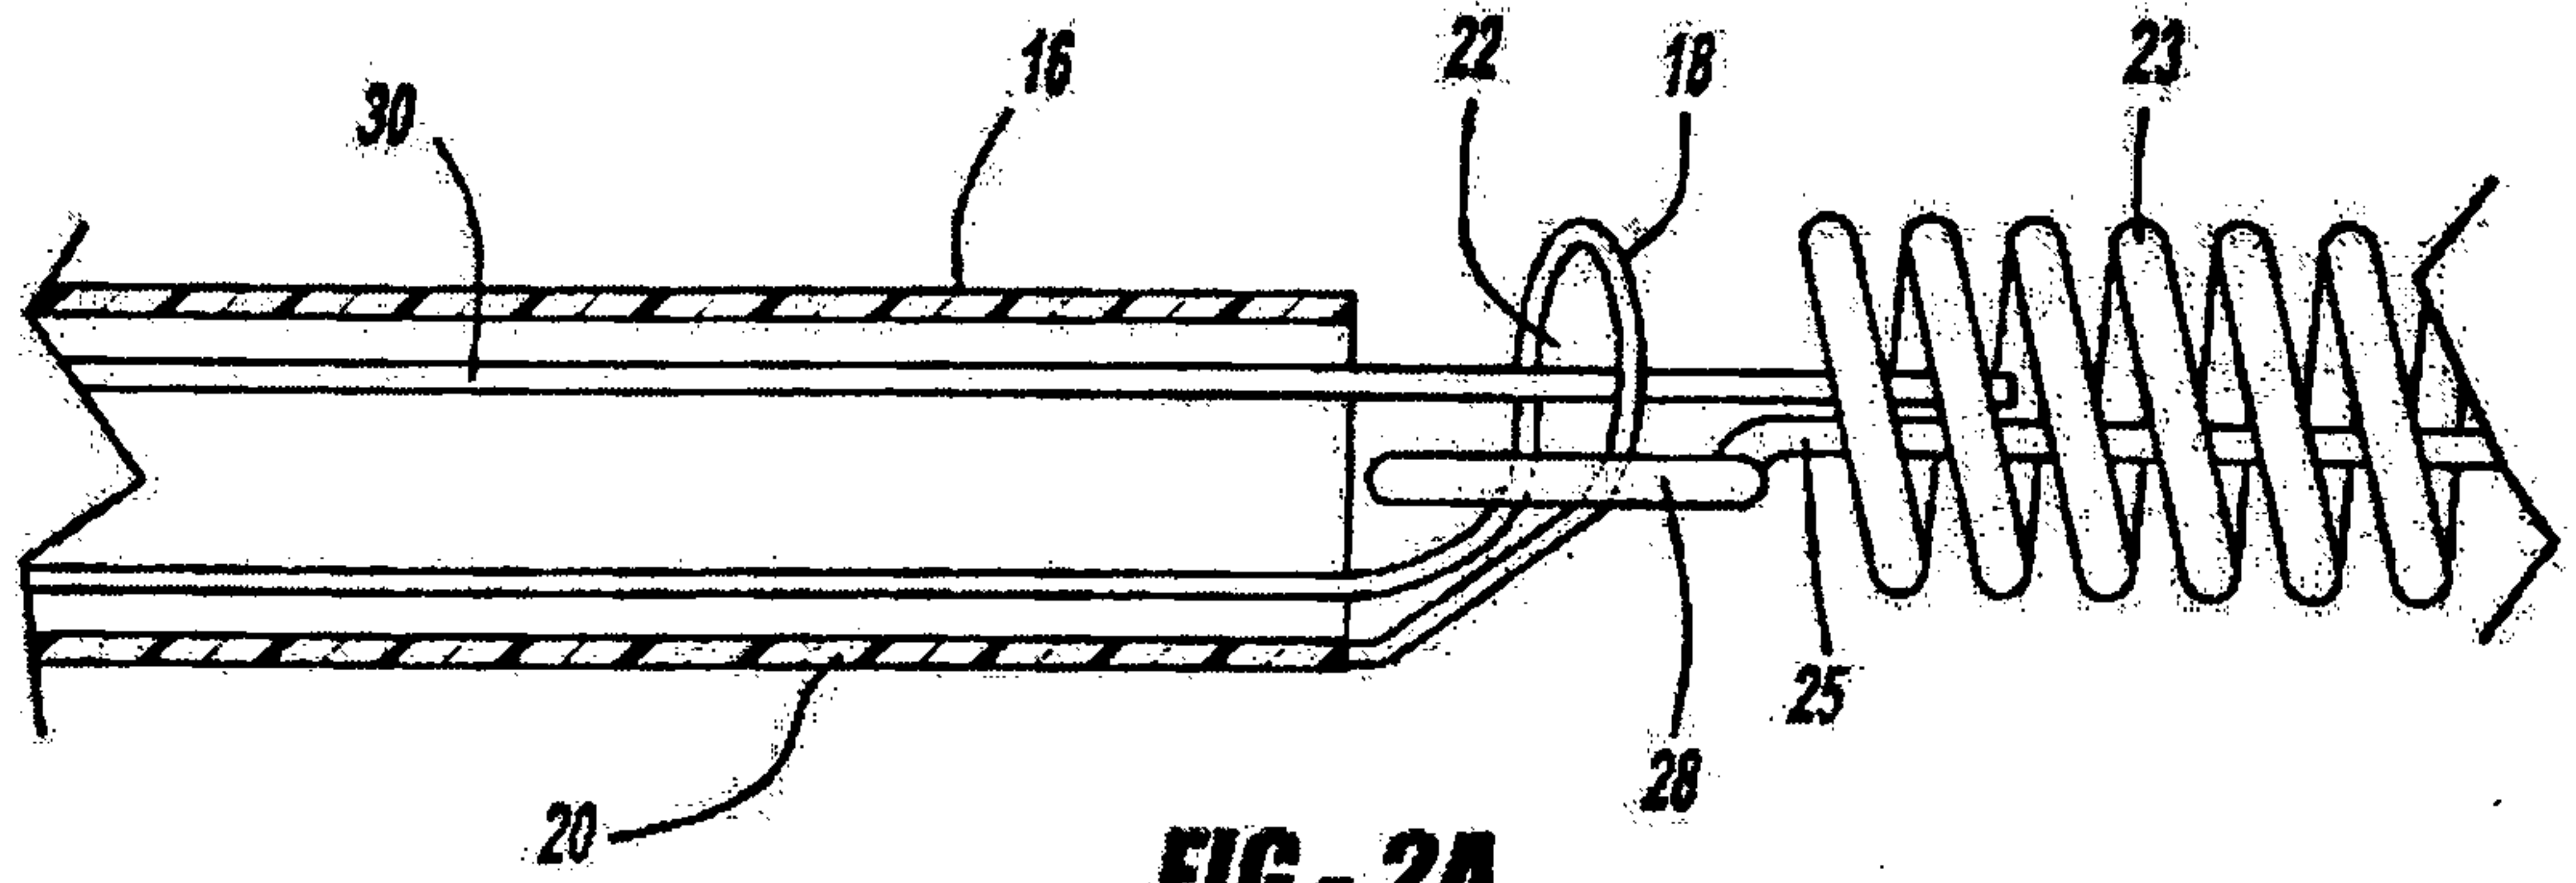


FIG - 2A

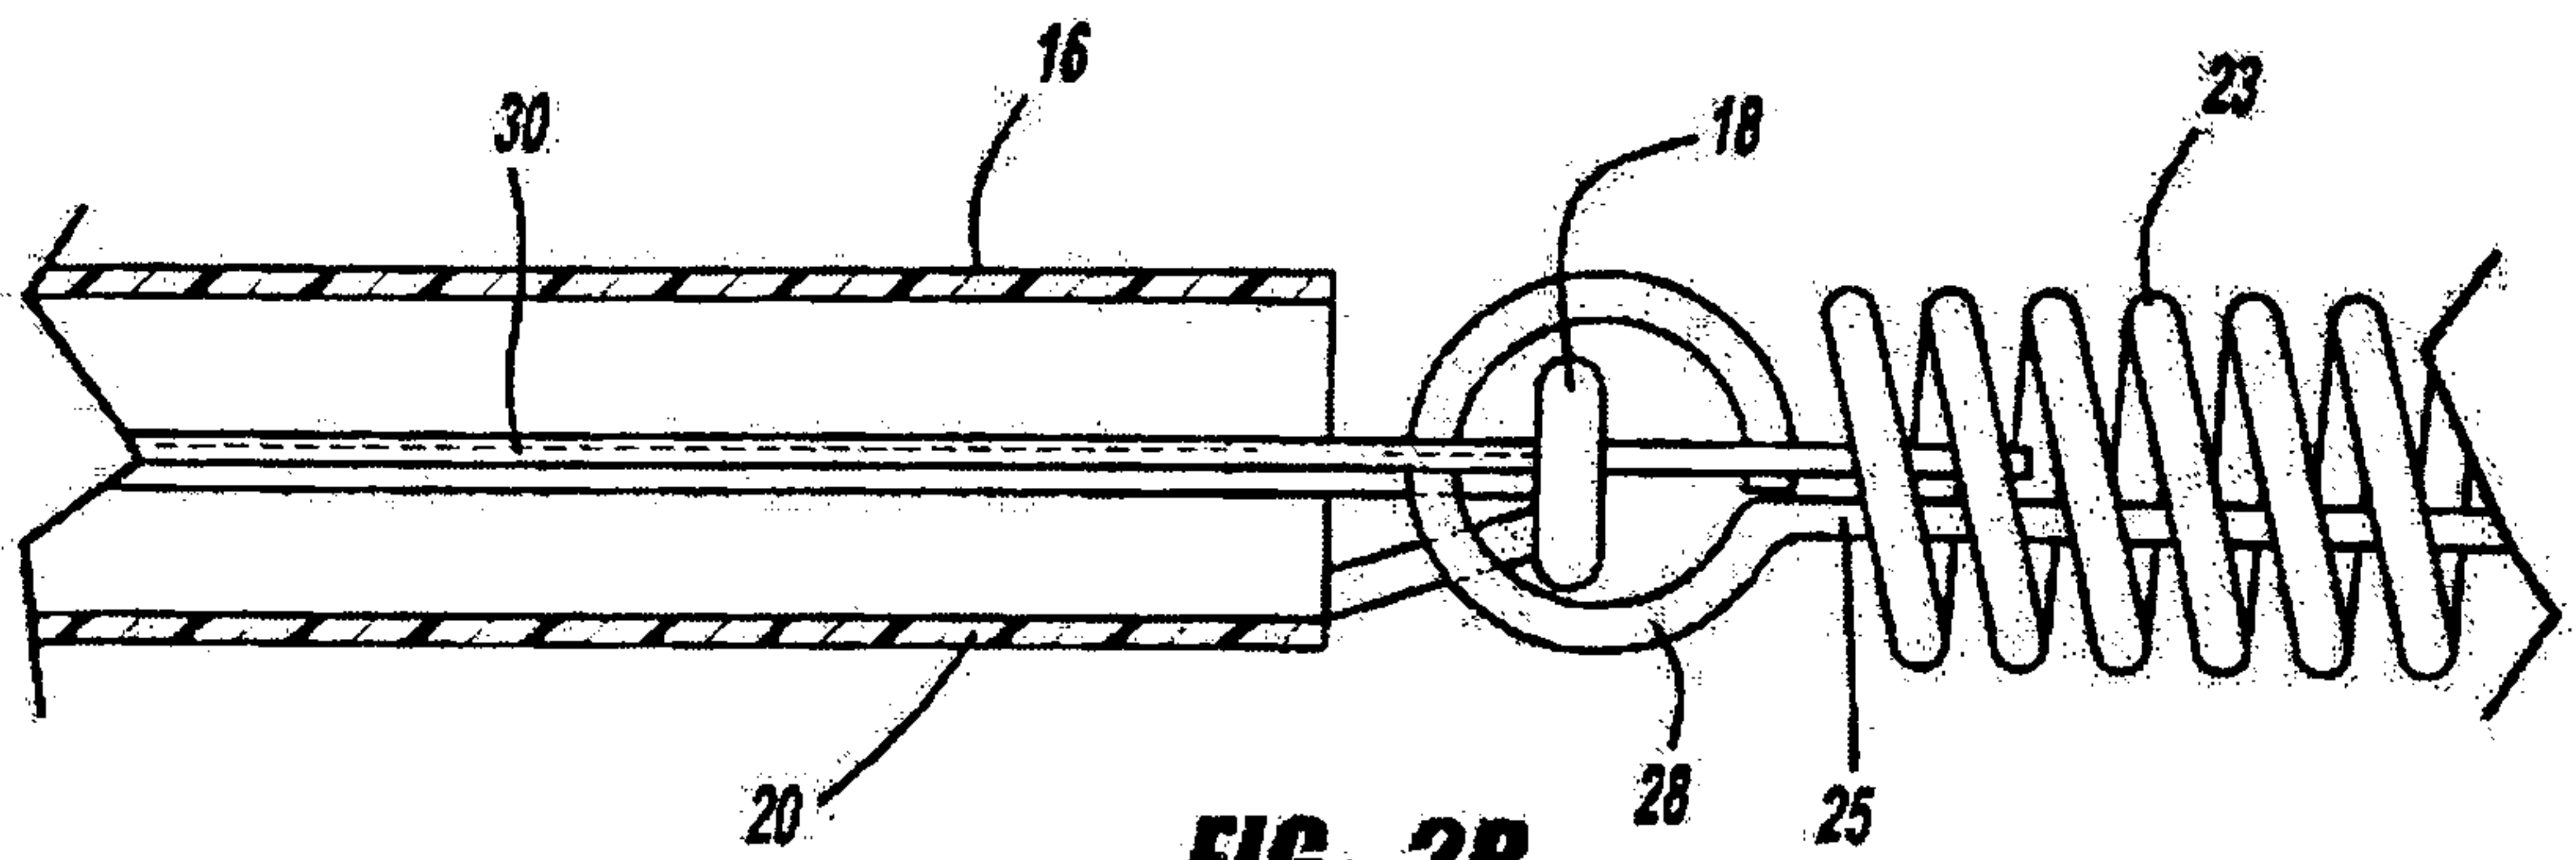


FIG - 2B

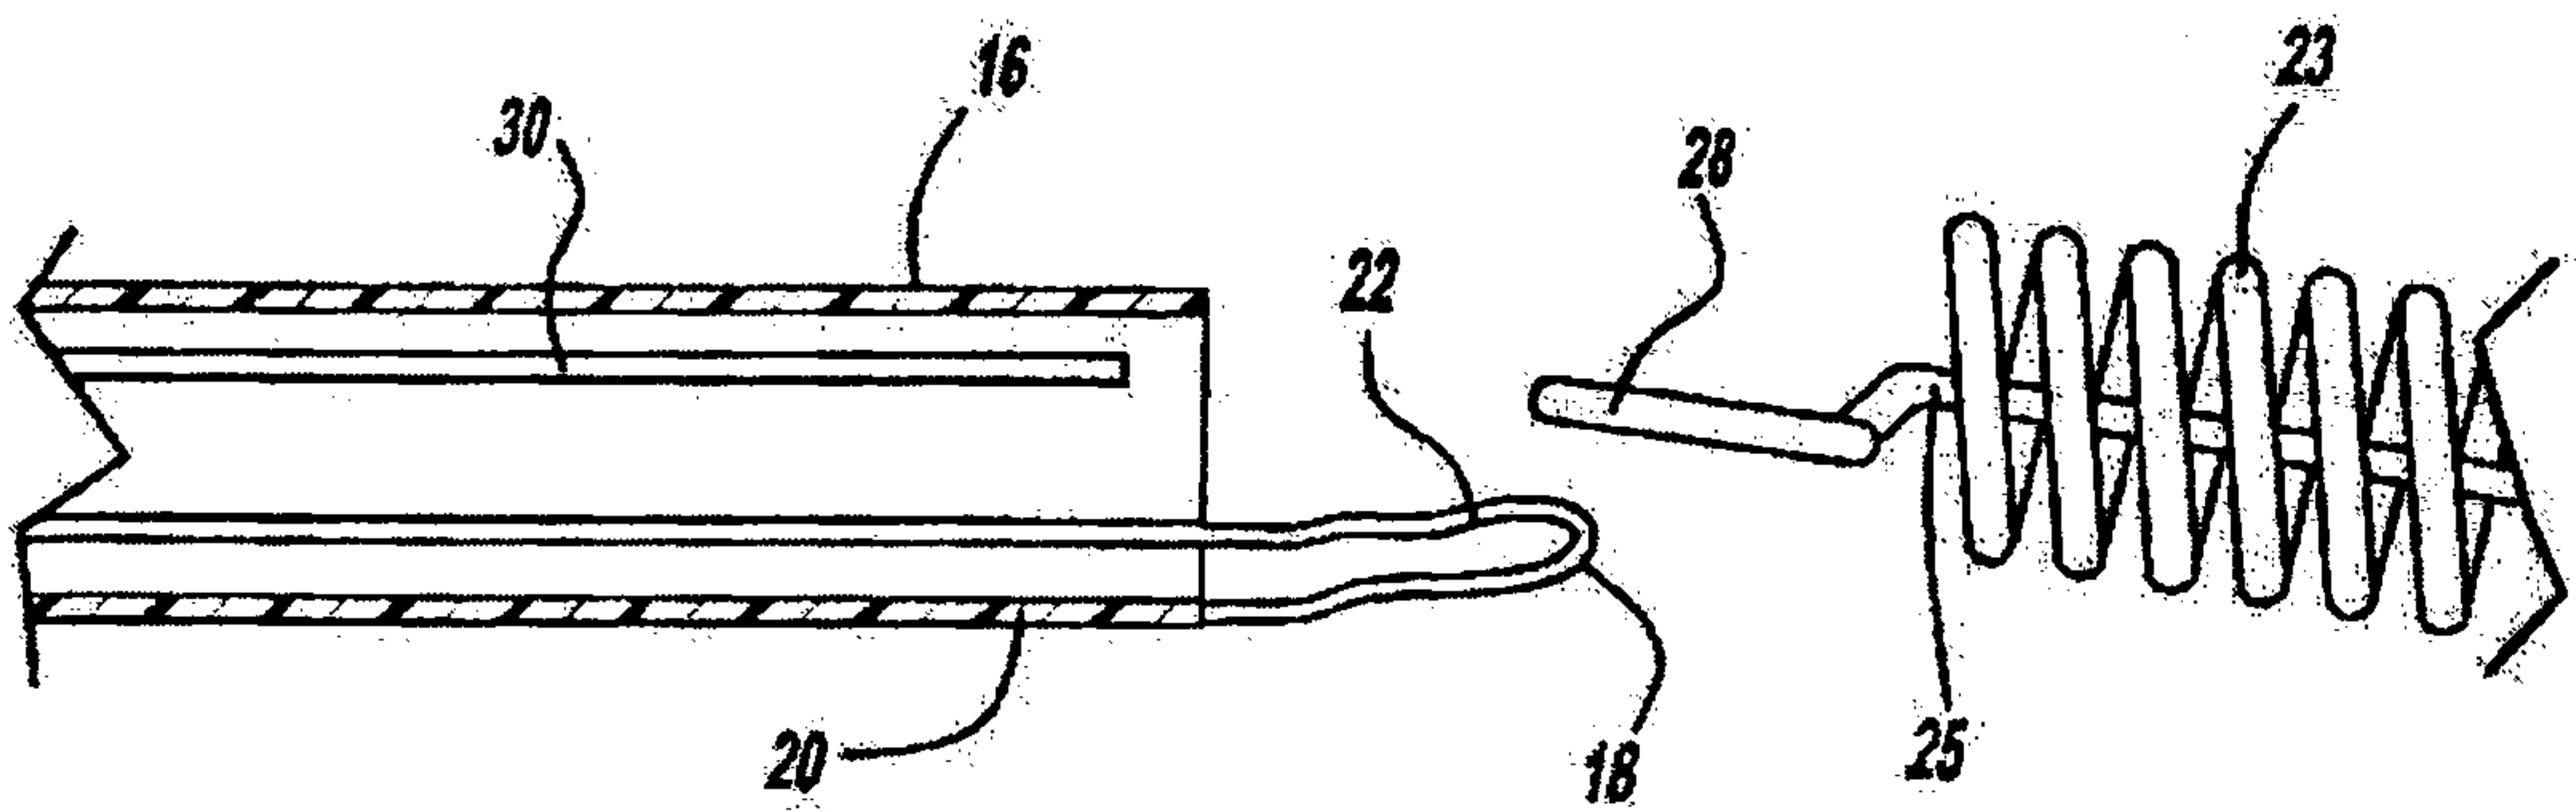


FIG - 2C

4/7

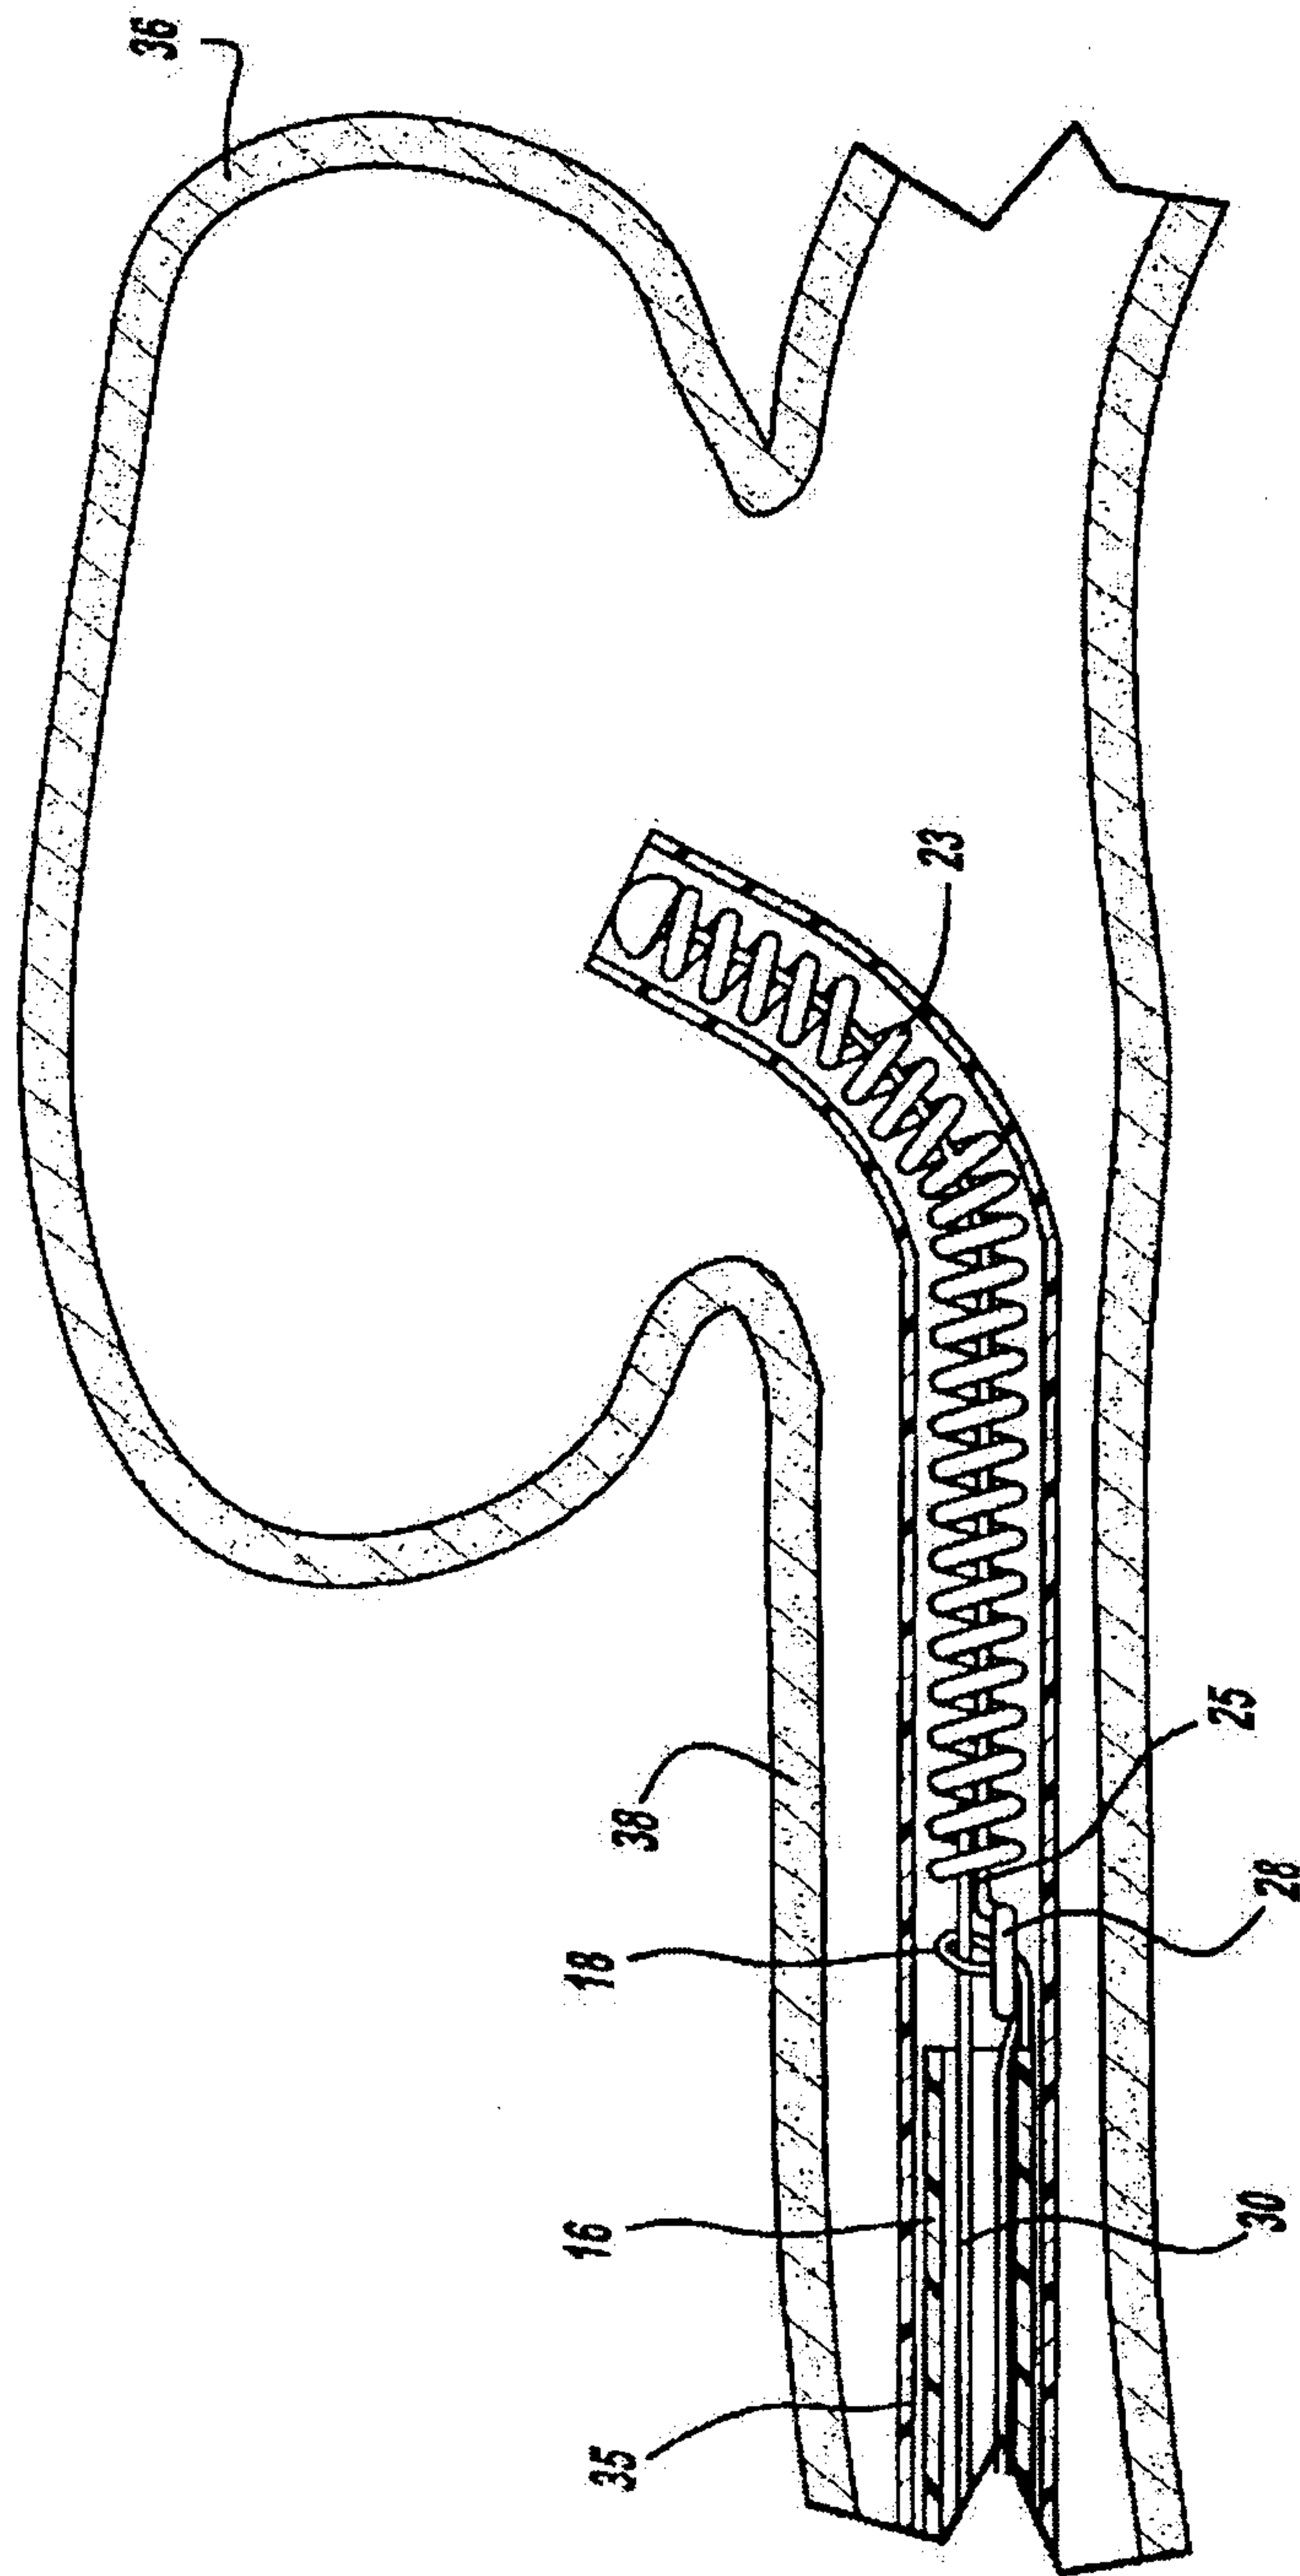


FIG - 3

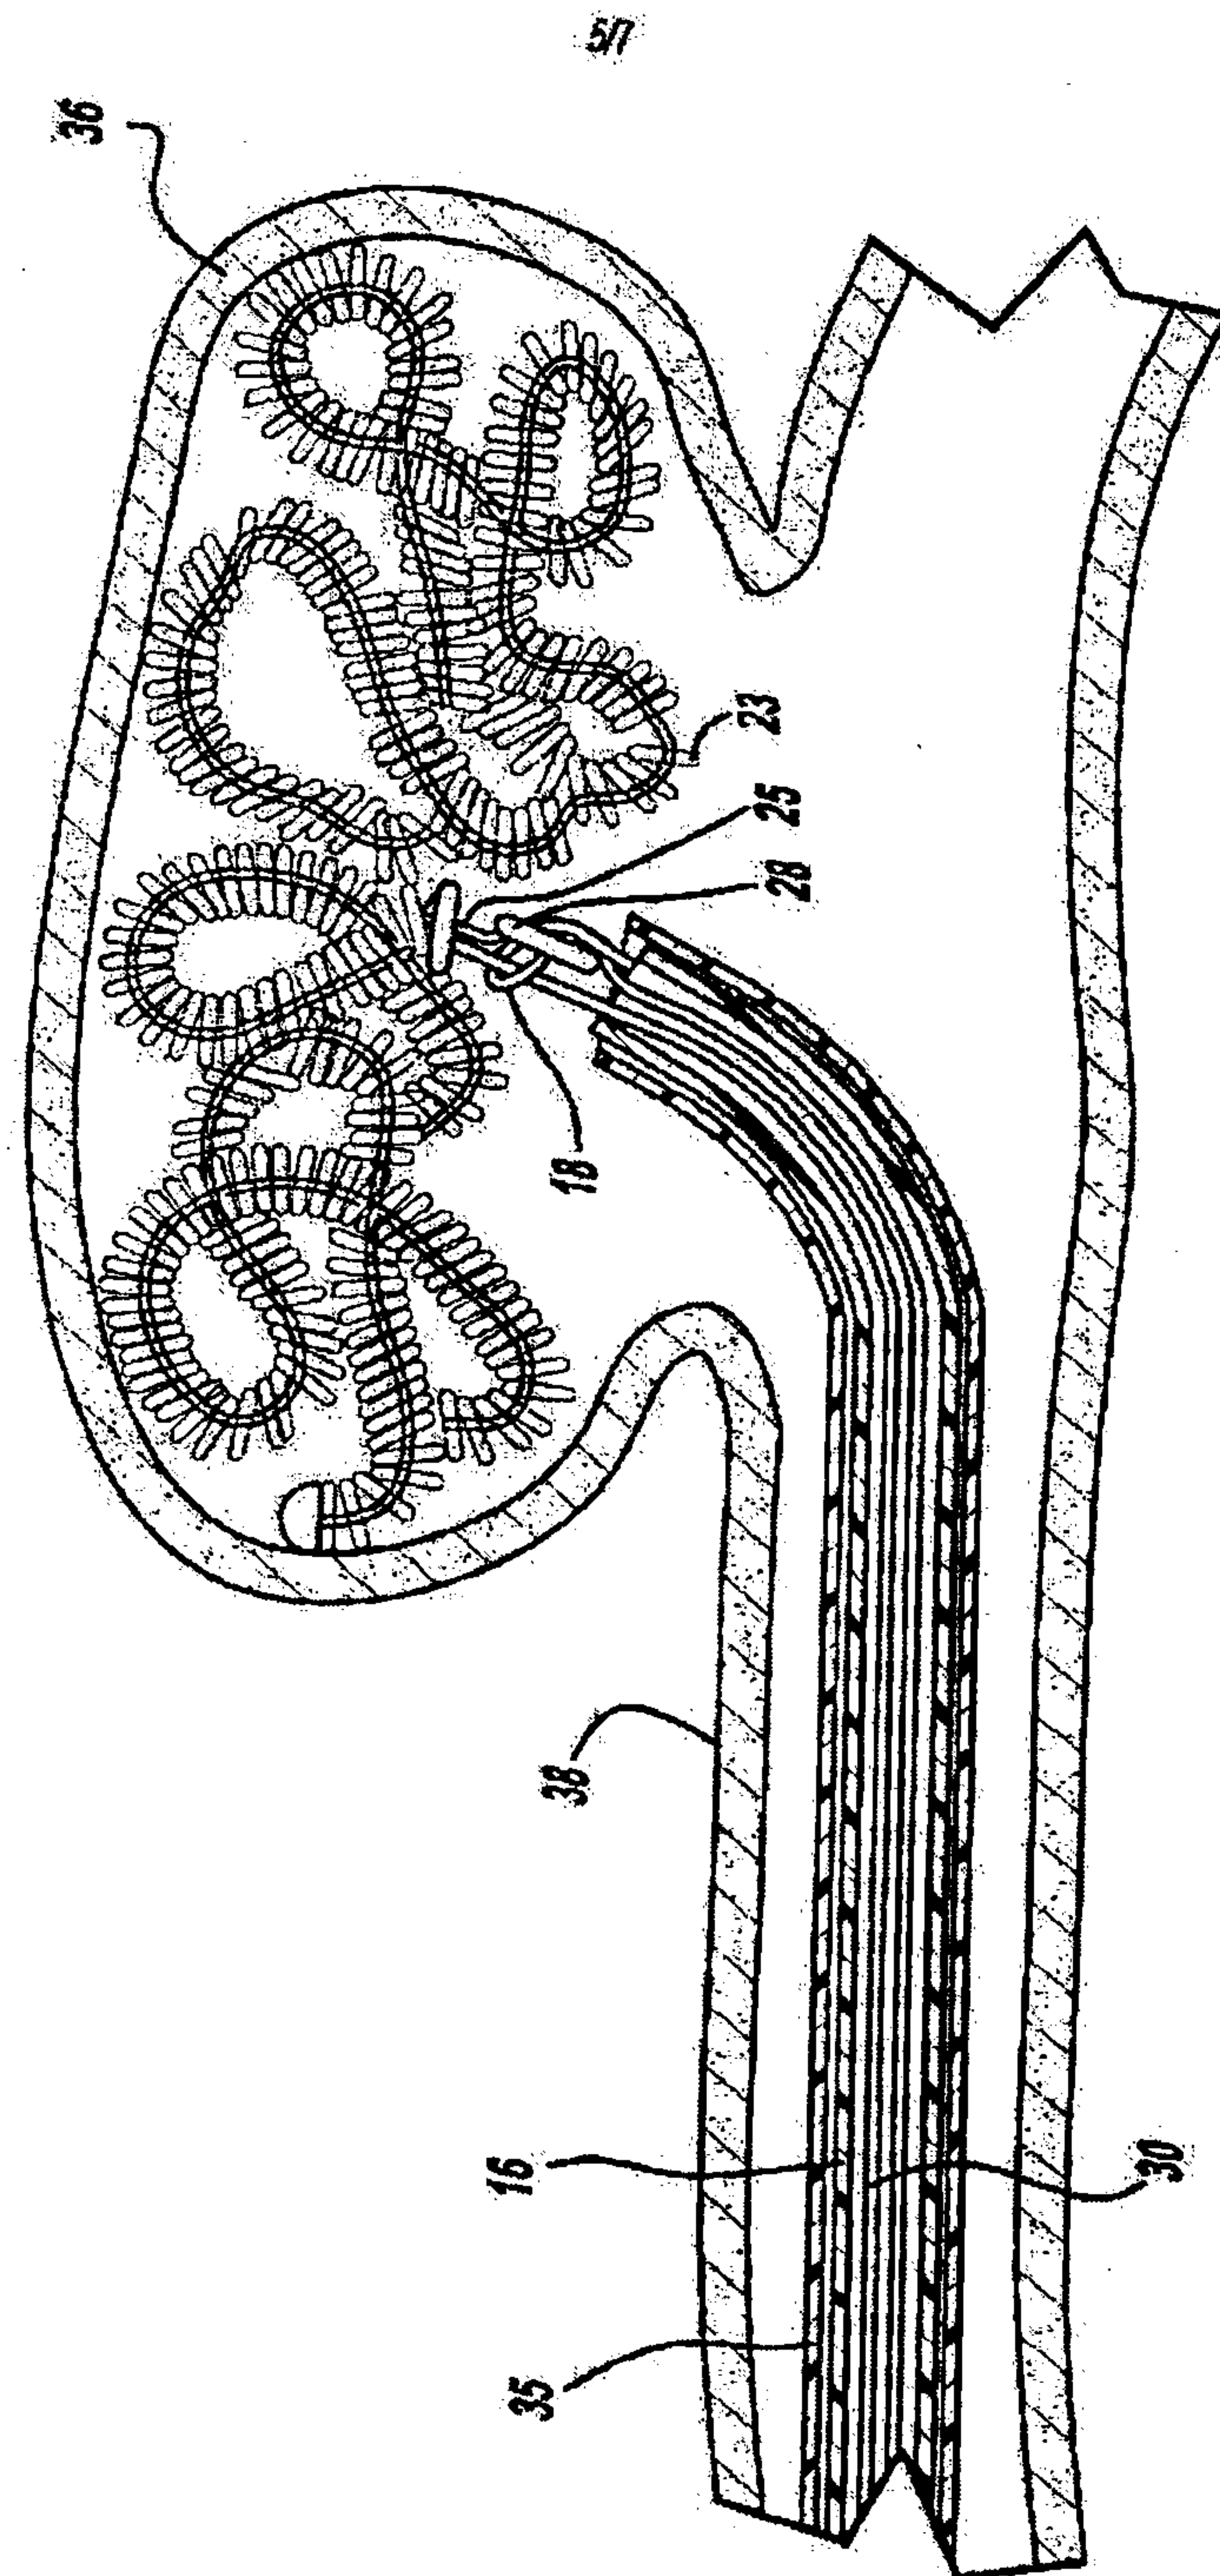


FIG-3A

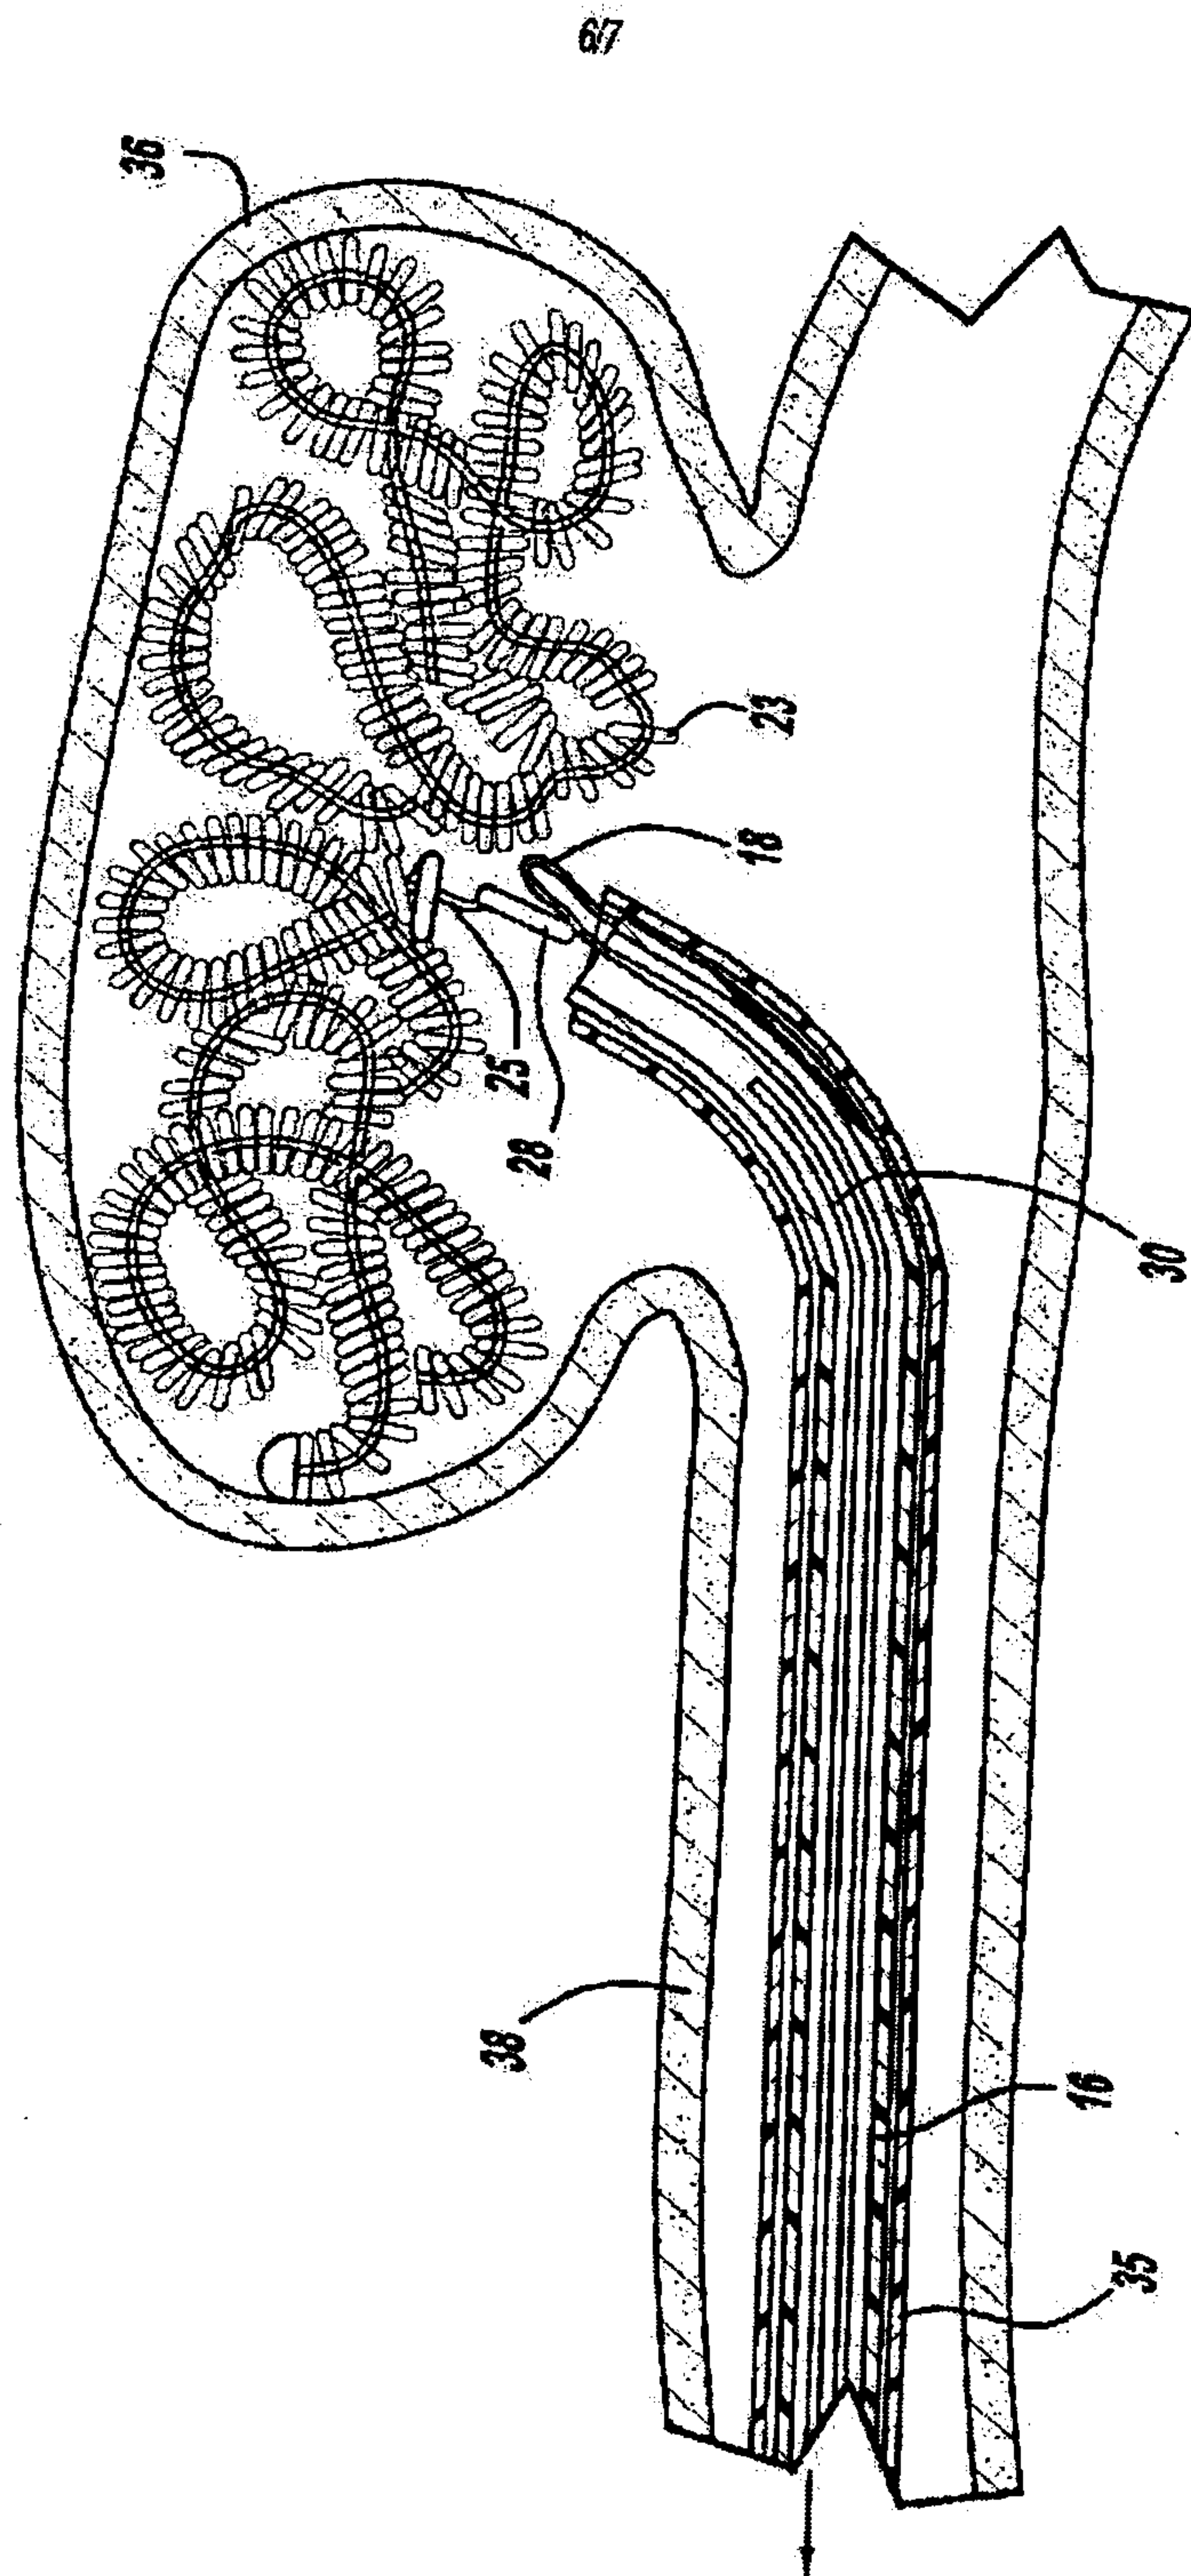


FIG - 3B

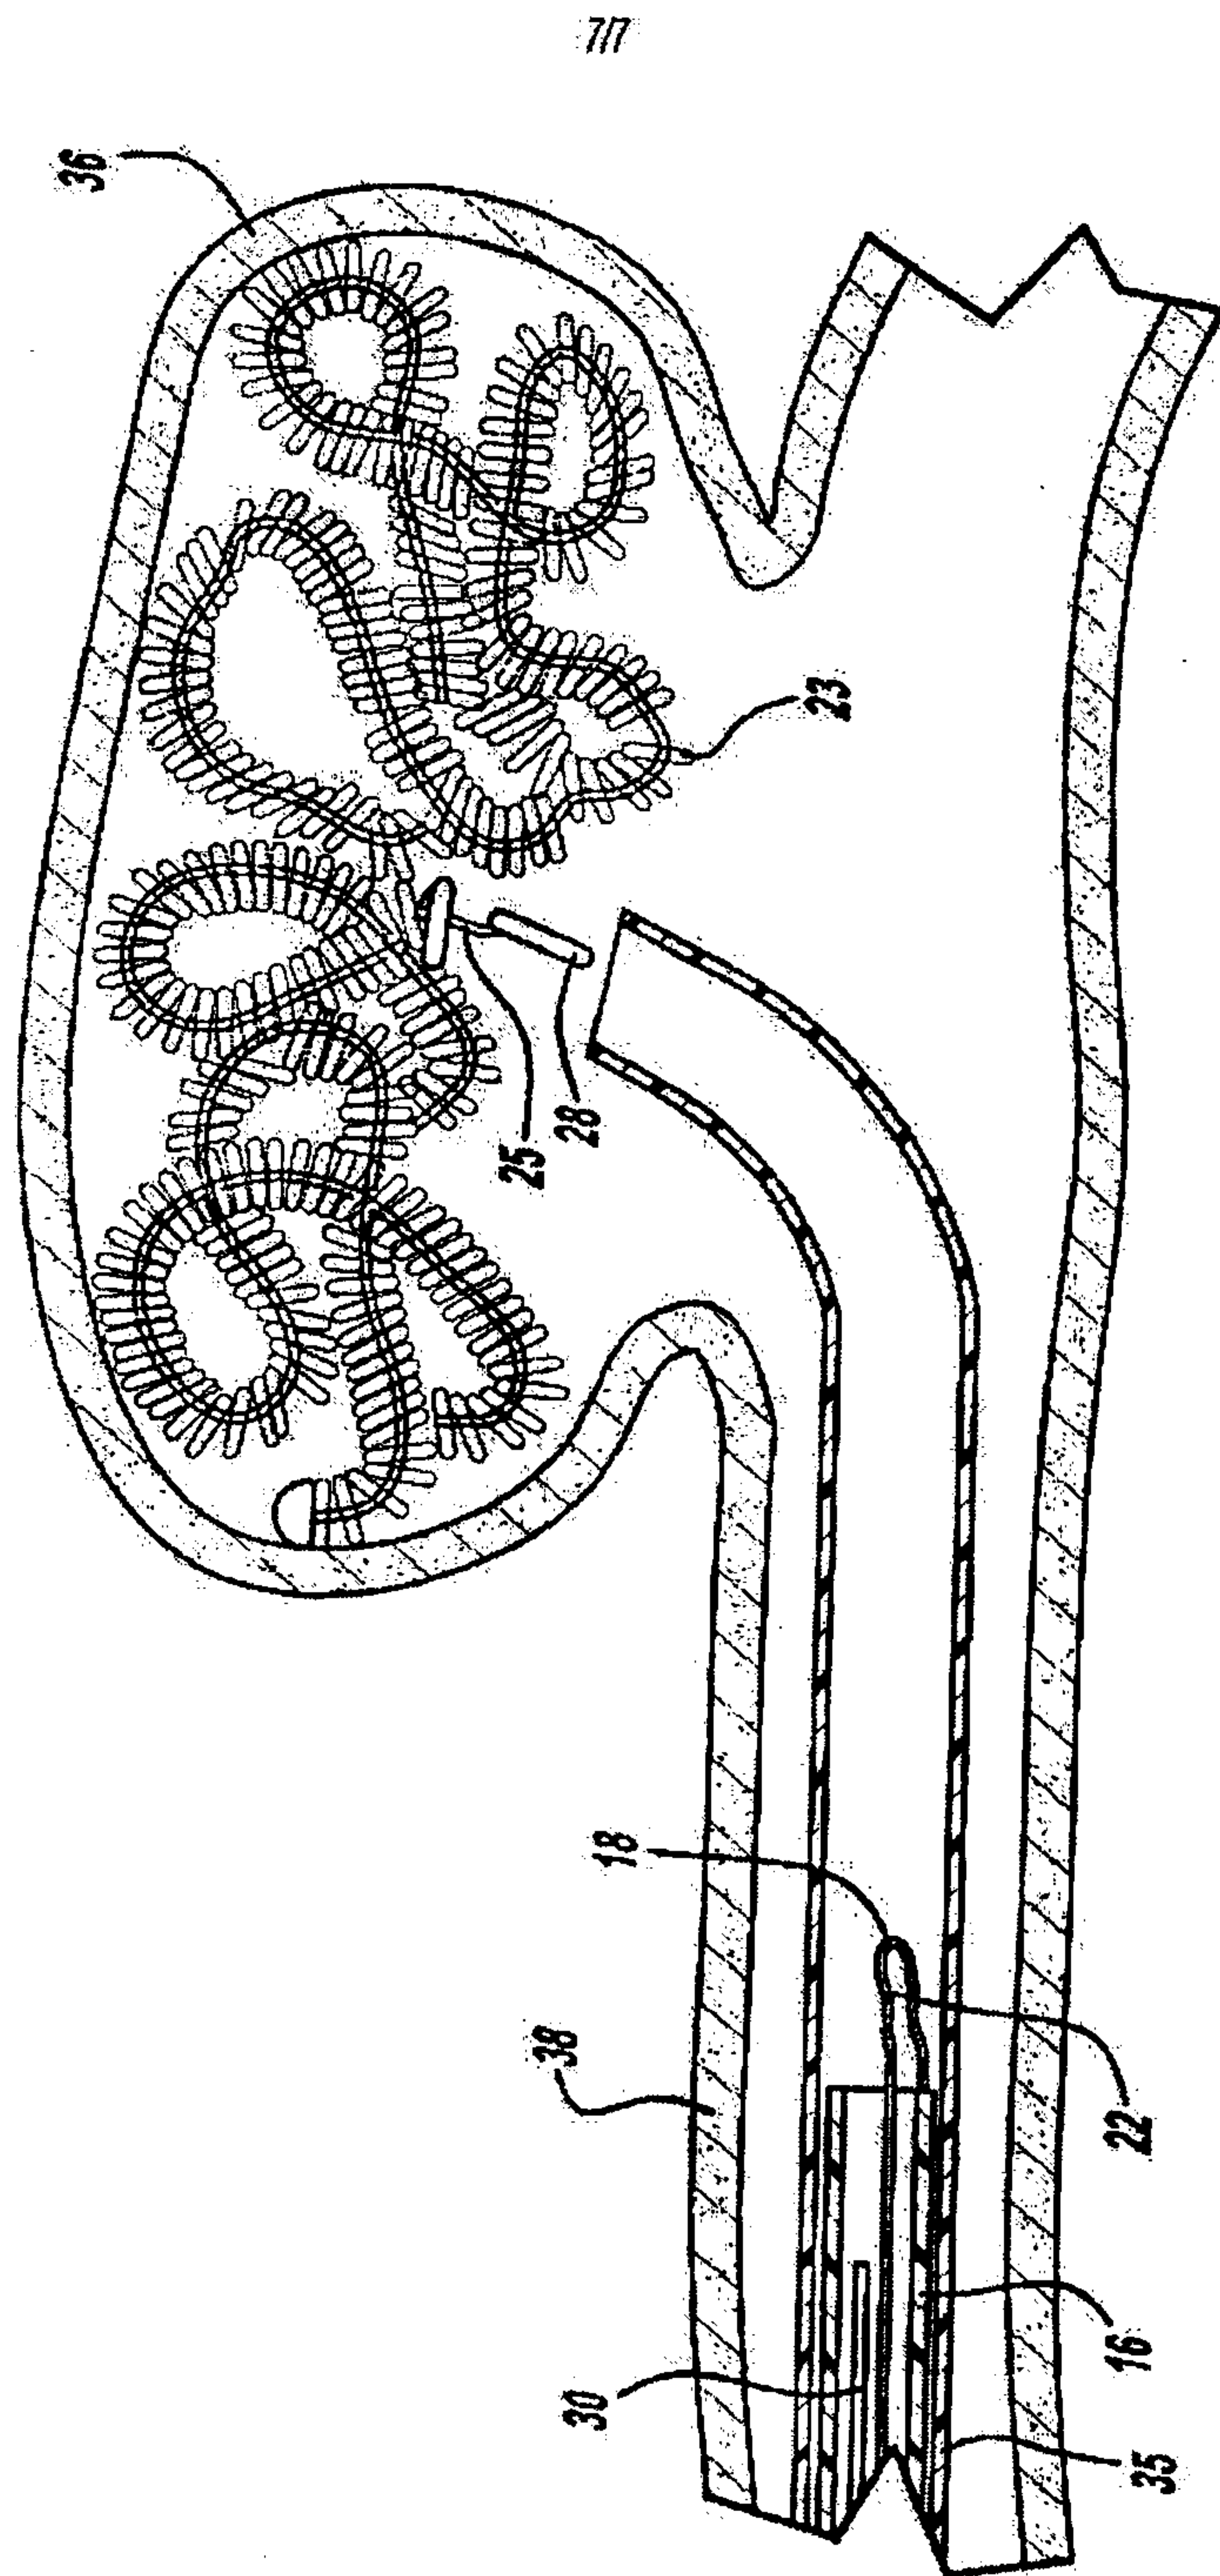


FIG-3C

