



(12) **United States Design Patent**
Barbu-Roth et al.

(10) **Patent No.:** **US D899,694 S**
(45) **Date of Patent:** **** Oct. 20, 2020**

(54) **LOCOMOTION TRAINING DEVICE FOR INFANTS**

(71) Applicant: **Université Paris Descartes**, Paris (FR)

(72) Inventors: **Marianne Barbu-Roth**, Paris (FR);
Vincent Forma, Paris (FR); **Joëlle Provasi**, Massy (FR); **Caroline Teulier**, Gif-sur-Yvette (FR)

(73) Assignee: **UNIVERSITE PARIS DESCARTES**, Paris (FR)

(**) Term: **15 Years**

(21) Appl. No.: **29/636,402**

(22) Filed: **Feb. 8, 2018**

(30) **Foreign Application Priority Data**

Aug. 9, 2017 (EM) 004140416-0001
Aug. 9, 2017 (EM) 004140416-0002

(51) **LOC (12) Cl.** **29-02**
(52) **U.S. Cl.**

USPC **D29/101.1**

(58) **Field of Classification Search**

USPC D29/100, 101.1, 101.5, 103; 128/875;
D24/193; D6/333; D12/128
CPC A47D 13/04; A47D 13/046; A47D 13/08;
A47D 15/00; A47D 15/003; A47D
15/005; A47D 15/008; G09B 19/003;
A62B 35/00; A63H 33/006; A61G
2200/14

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,572,273 A * 2/1926 Elton A47D 13/08
280/87.051
2,102,281 A * 12/1937 Pringle A47D 15/008
128/875

3,027,058 A * 3/1962 Huber A47D 13/025
224/155
D261,378 S * 10/1981 Bergeron D12/128
4,911,105 A * 3/1990 Hocum A47D 15/008
128/875

(Continued)

OTHER PUBLICATIONS

Medical Device Enables CP Infants to Crawl (on-line), dated Oct. 13, 2011. Retrieved from Internet May 13, 2020, URL: <https://www.todaymedicaldevelopments.com/article/medical-device-design-engineering-manufacturing-101311/> (2 pages) (Year: 2011).*

Primary Examiner — Kimberly Barnes

(74) *Attorney, Agent, or Firm* — Pearne & Gordon LLP

(57) **CLAIM**

We claim the ornamental design for a locomotion training device for infants, as shown and described.

DESCRIPTION

FIG. 1 is a top, front perspective view of a locomotion training device for infants showing our new design.

FIG. 2 is a top perspective view thereof;

FIG. 3 is a top plan view thereof;

FIG. 4 is a front view thereof;

FIG. 5 is a left side view thereof;

FIG. 6 is a rear view thereof;

FIG. 7 is another top view thereof, shown at a point in rotation half way between the views illustrated in FIGS. 2 and 3;



FIG. 8 is a top view thereof as in FIG. 7, but with outer securing straps opened;

FIG. 9 is a top view thereof as in FIGS. 7 and 8, but with harness thereof (including inner securing straps) completely opened; and,

FIG. 10 is a bottom view thereof.

The broken lines in the drawings depict stitching and other features of the locomotion training device for infants that form no part of the claimed design.

1 Claim, 10 Drawing Sheets

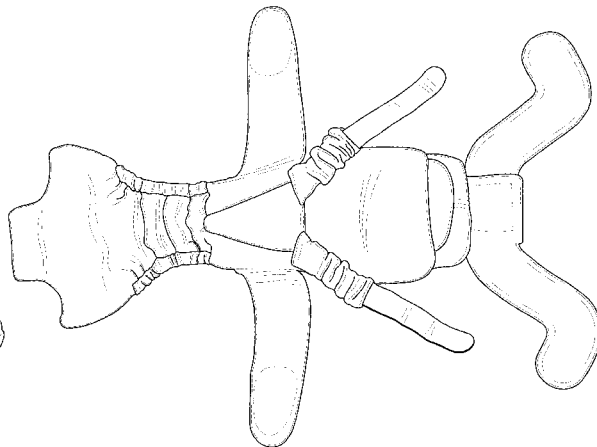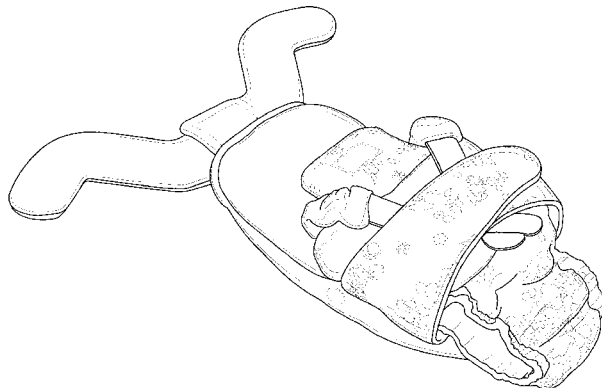

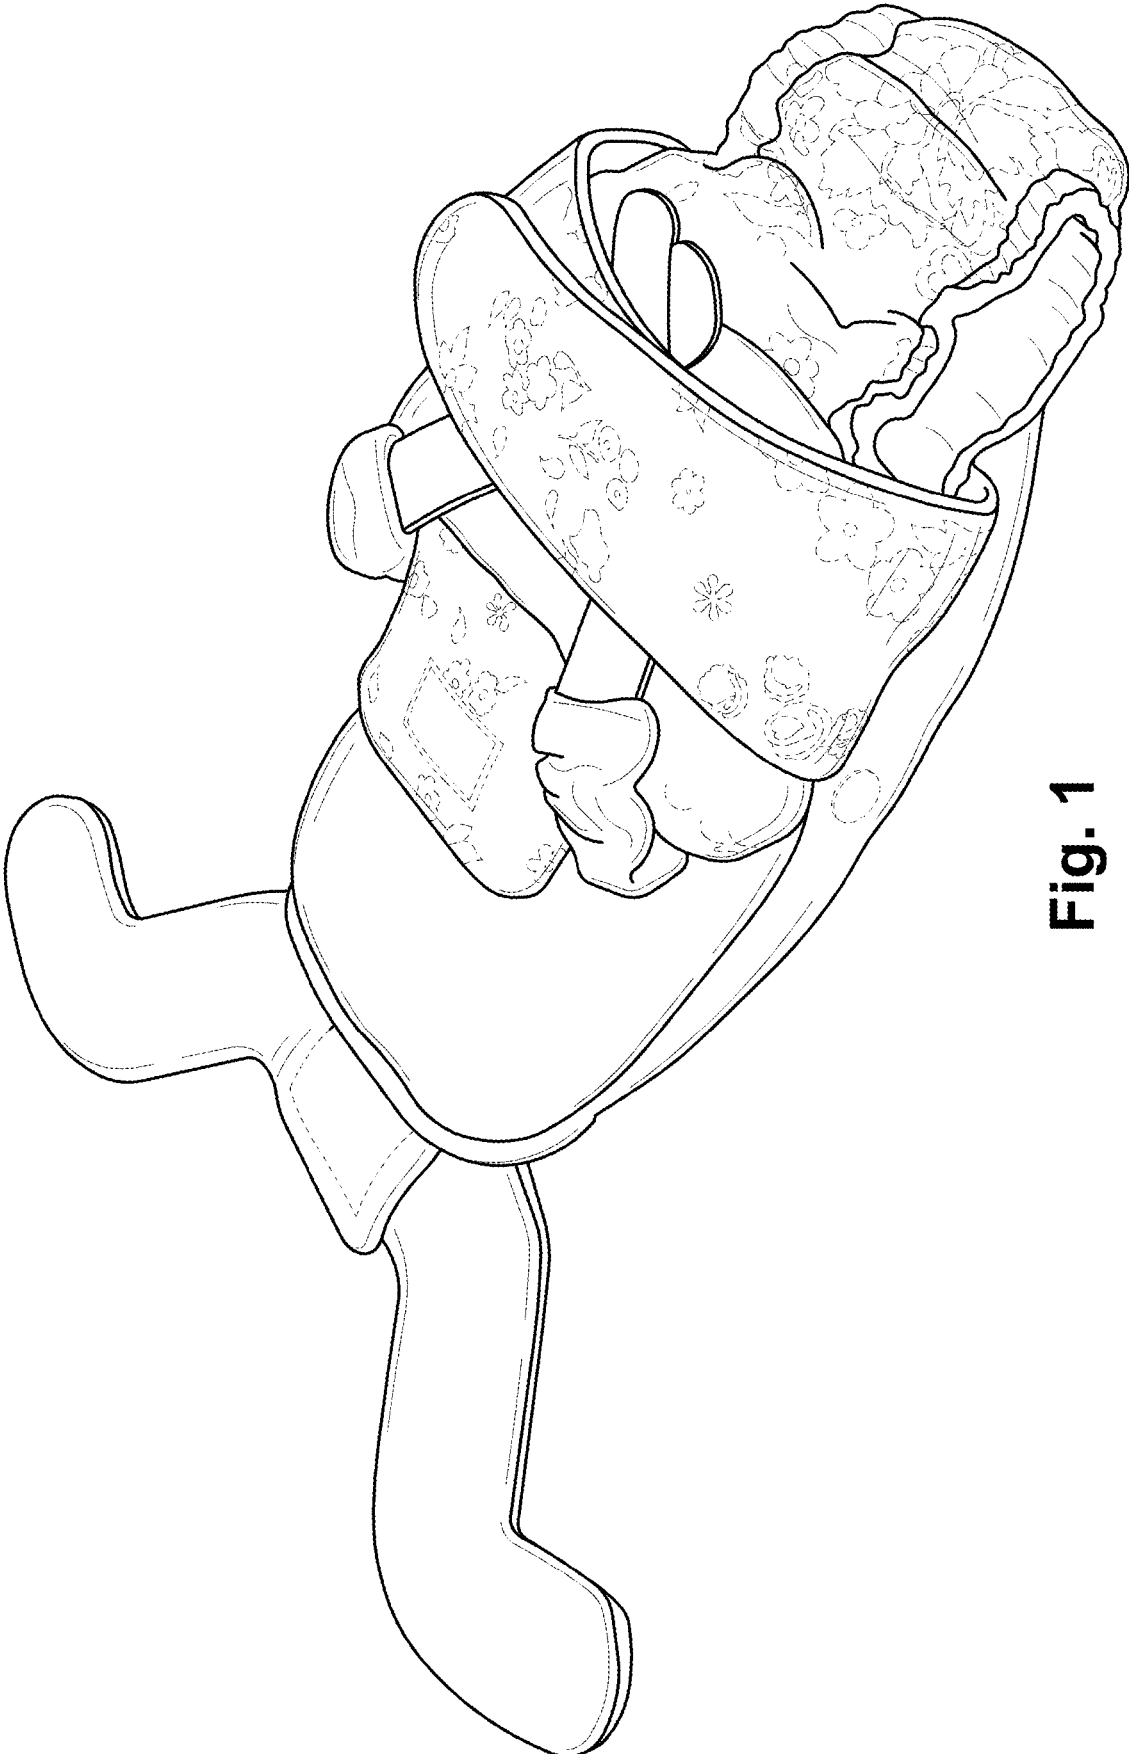


Fig. 1

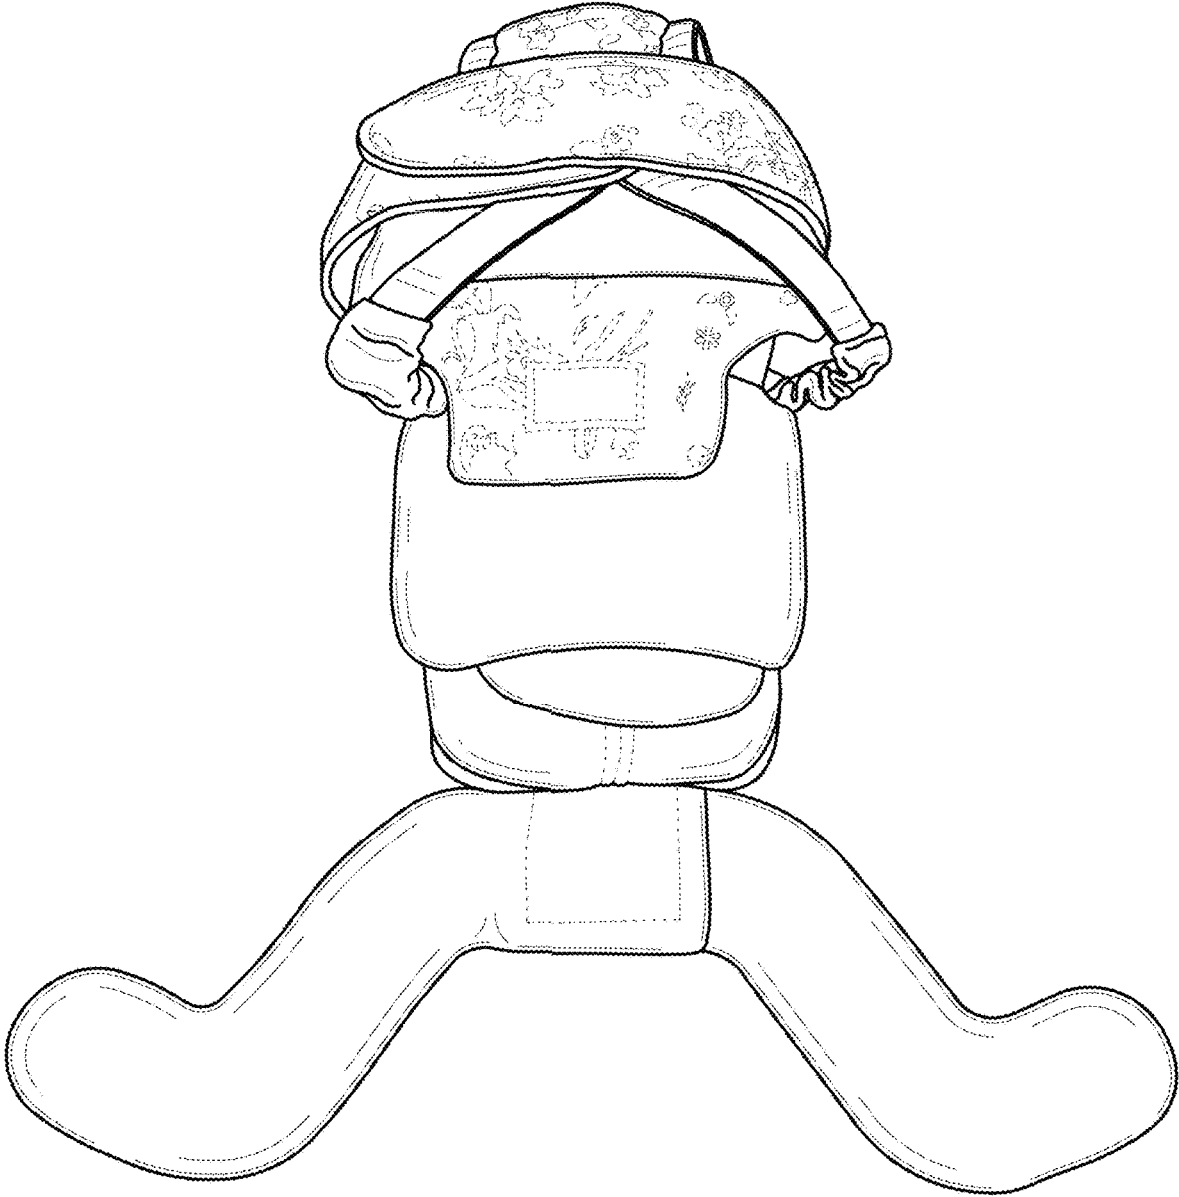


Fig. 2

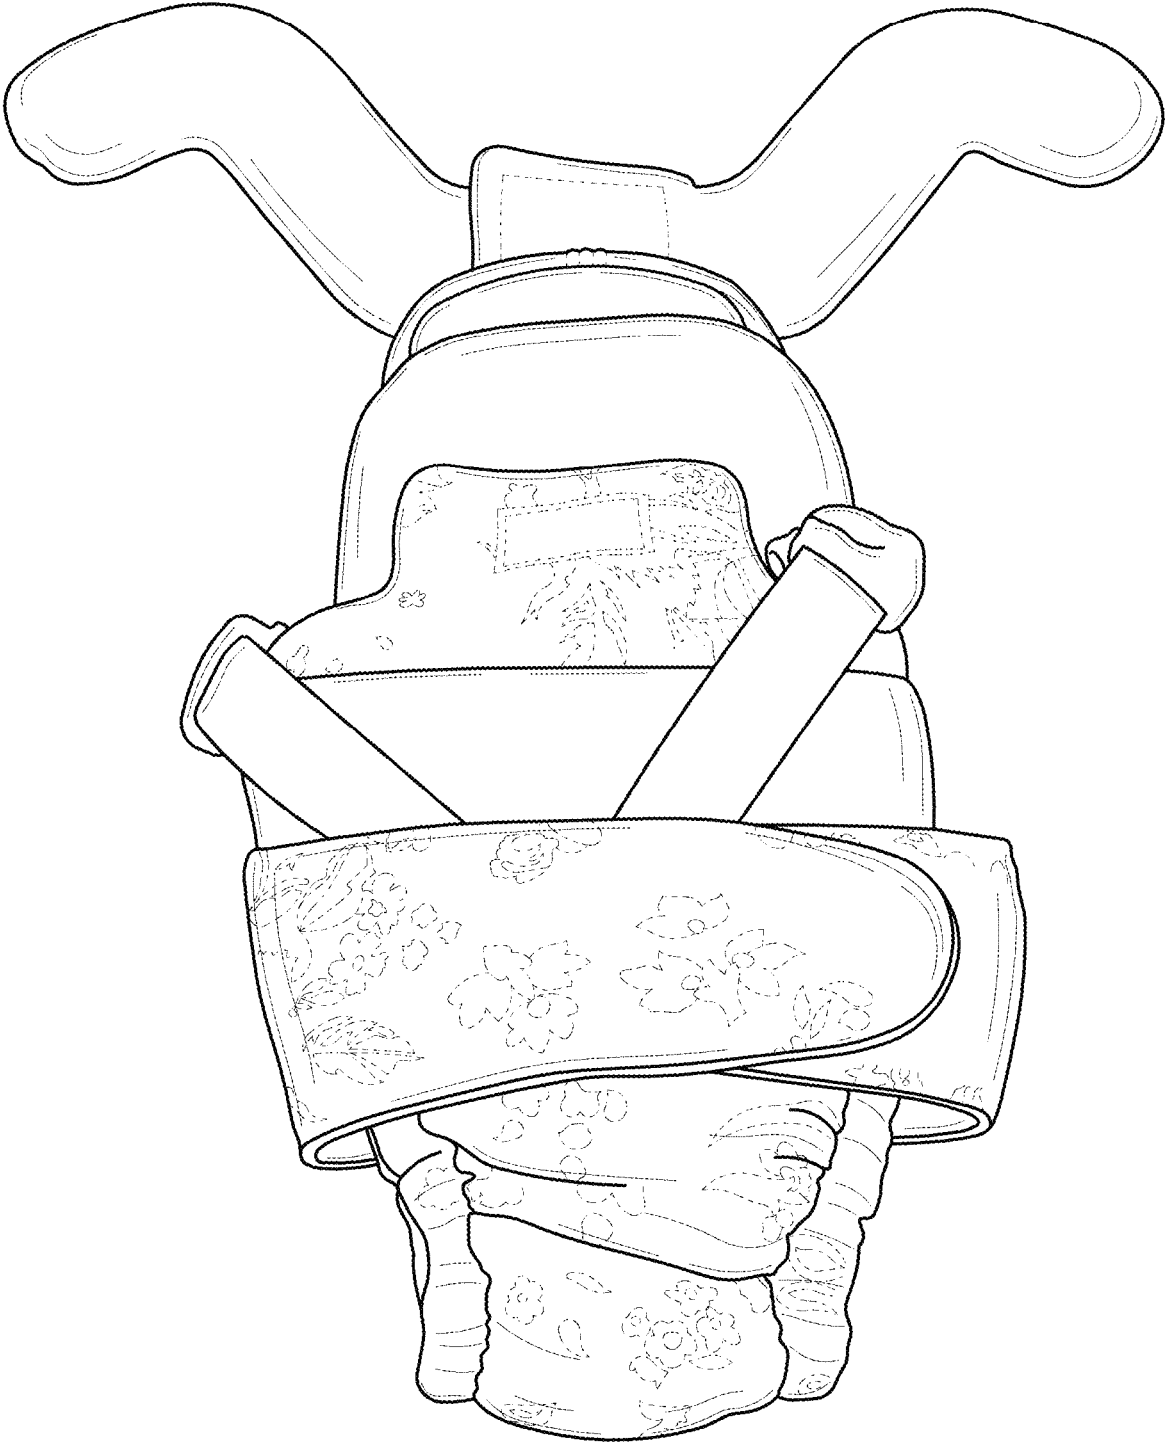


Fig. 3

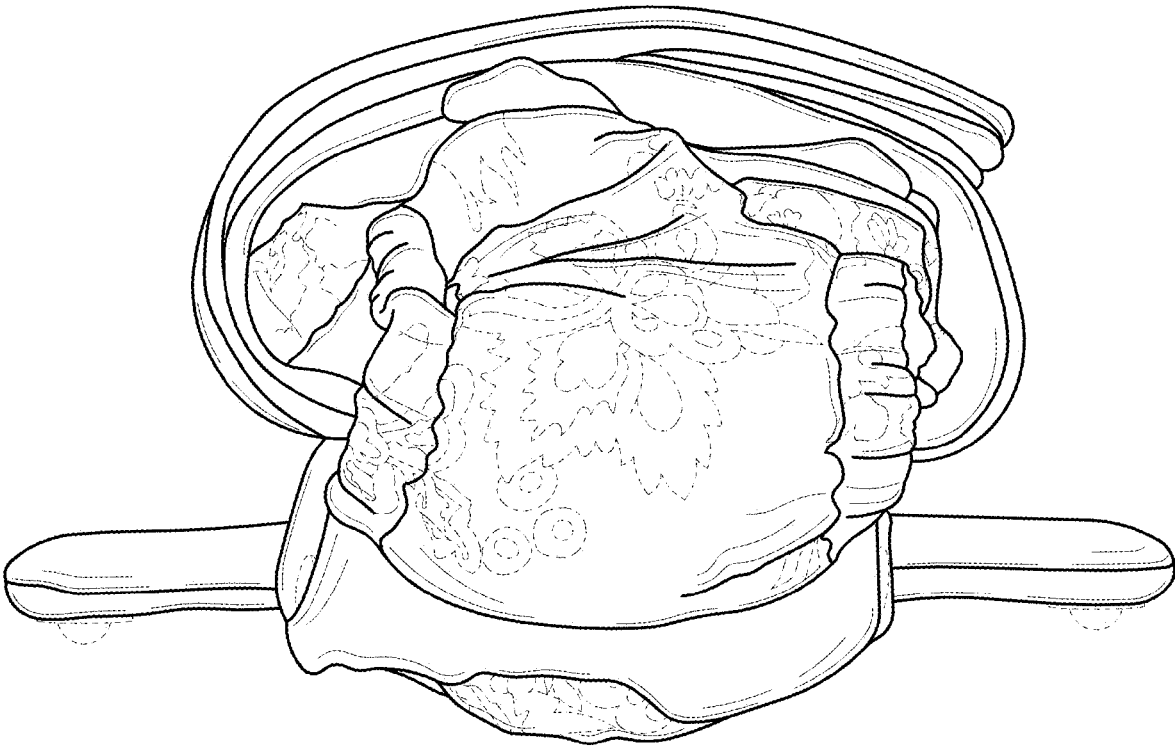


Fig. 4

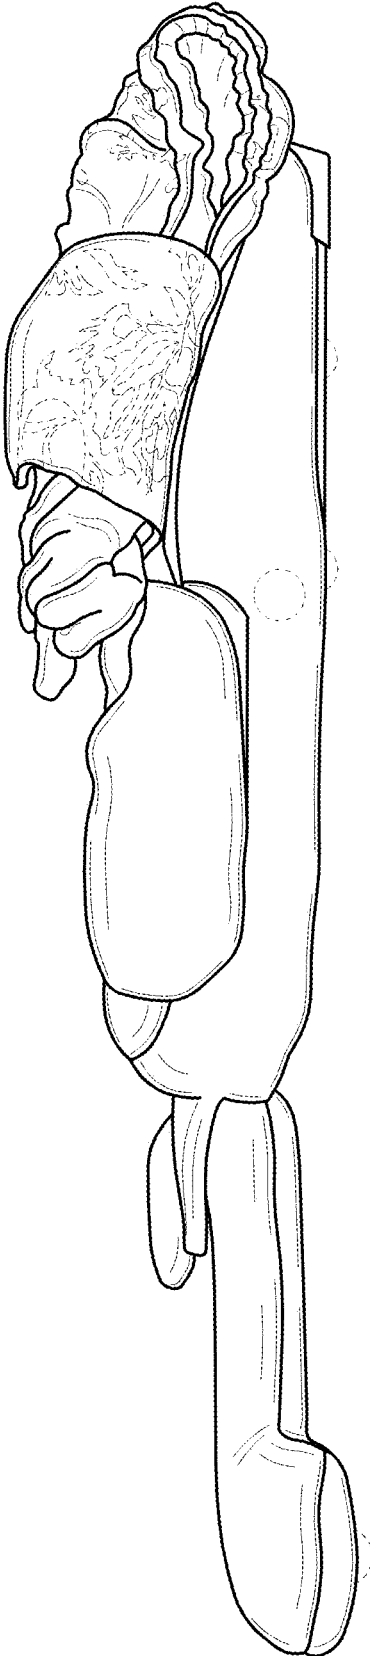


Fig. 5

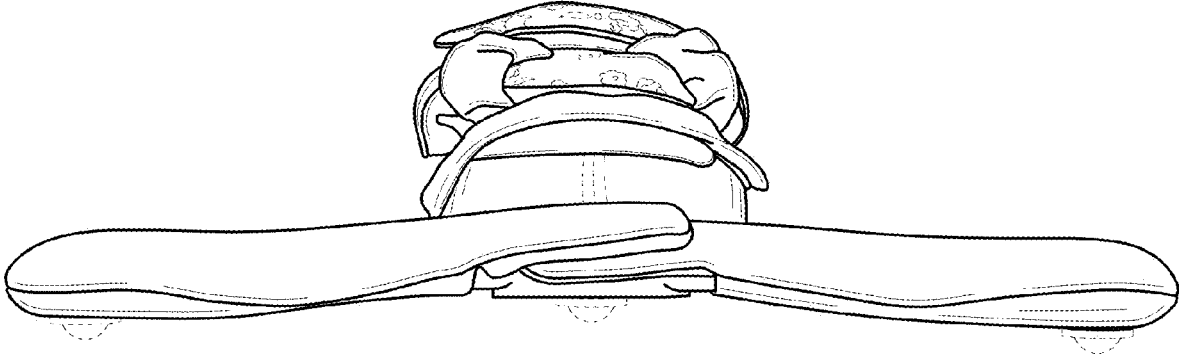


Fig. 6

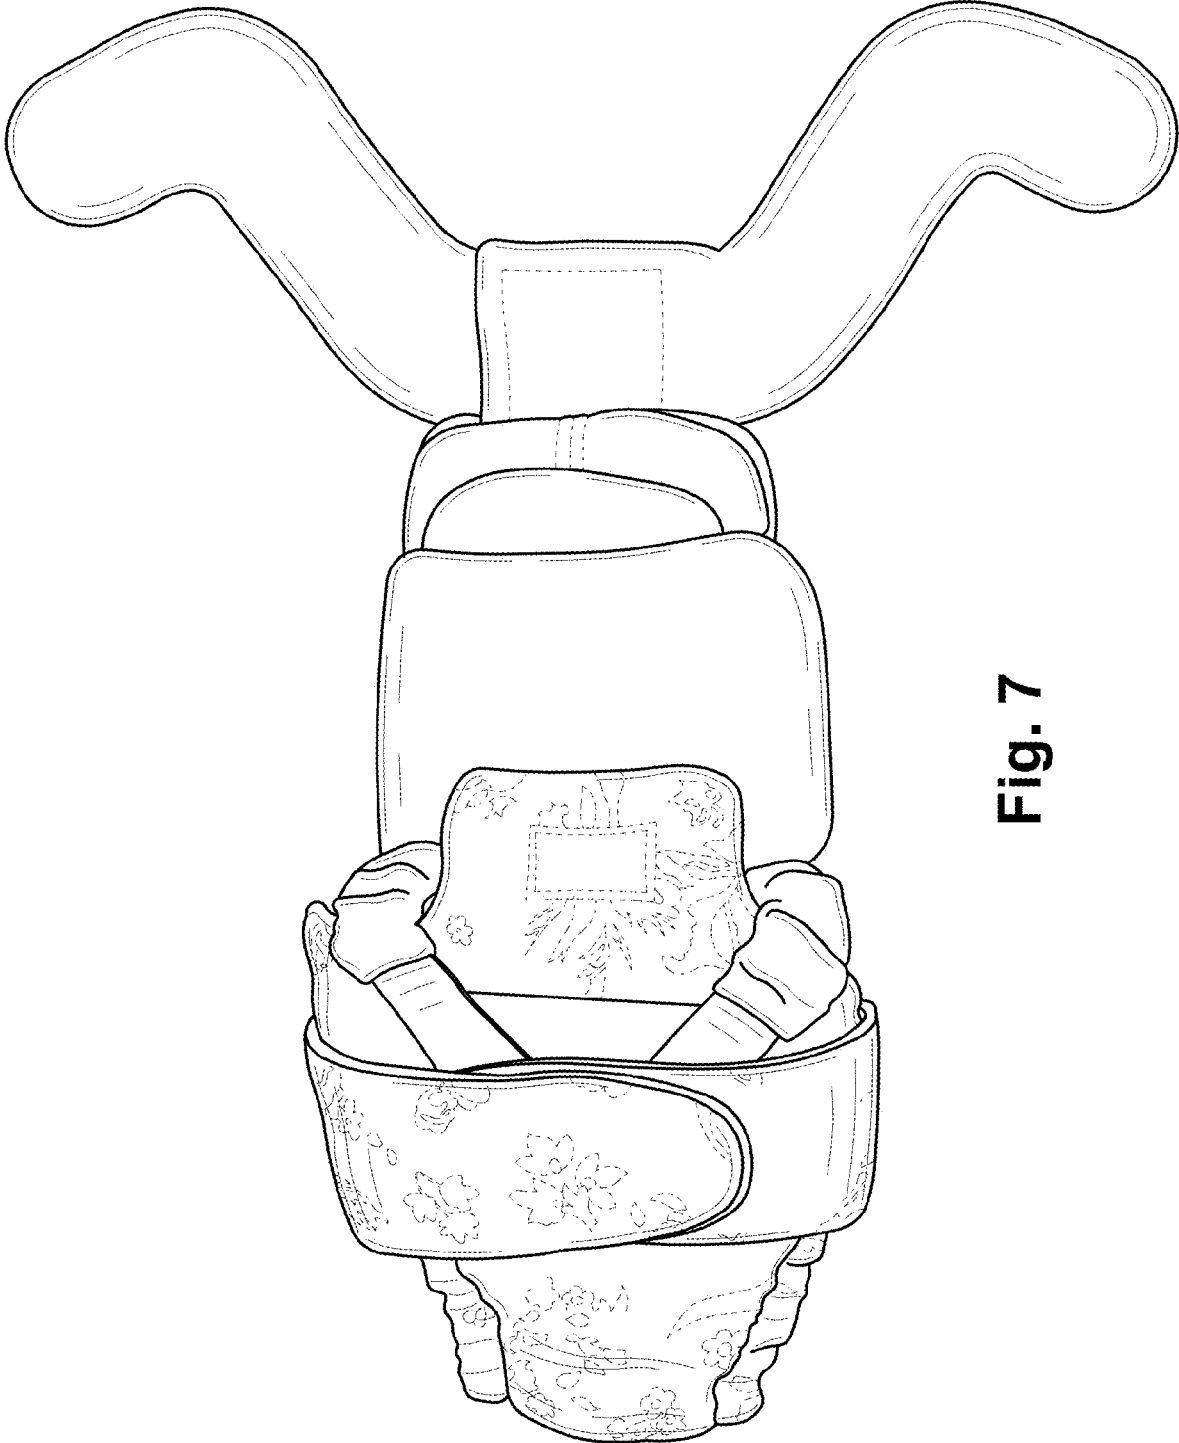


Fig. 7

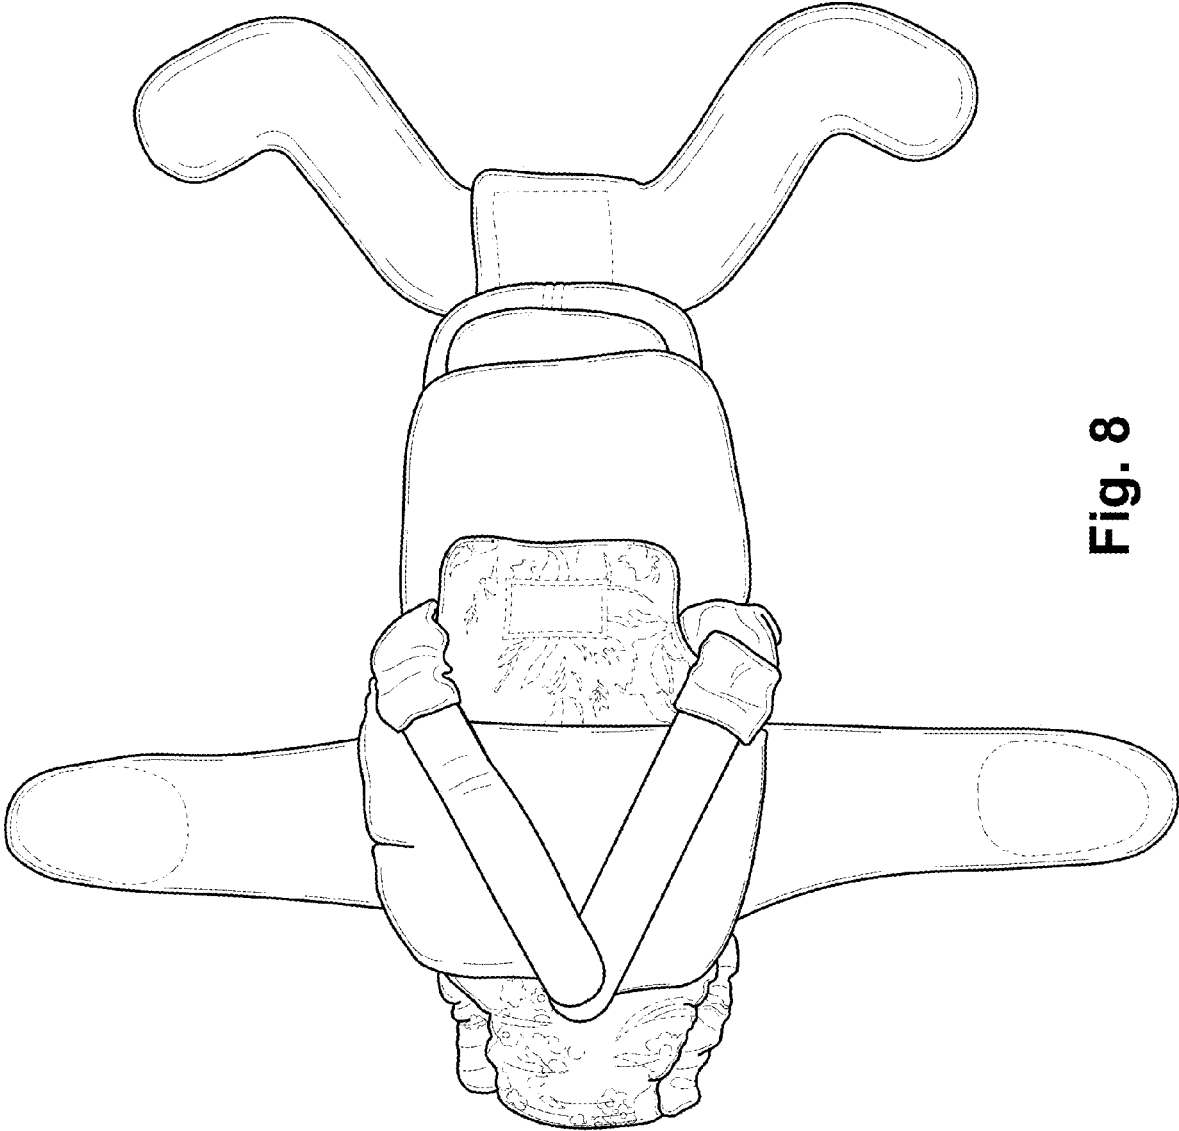


Fig. 8

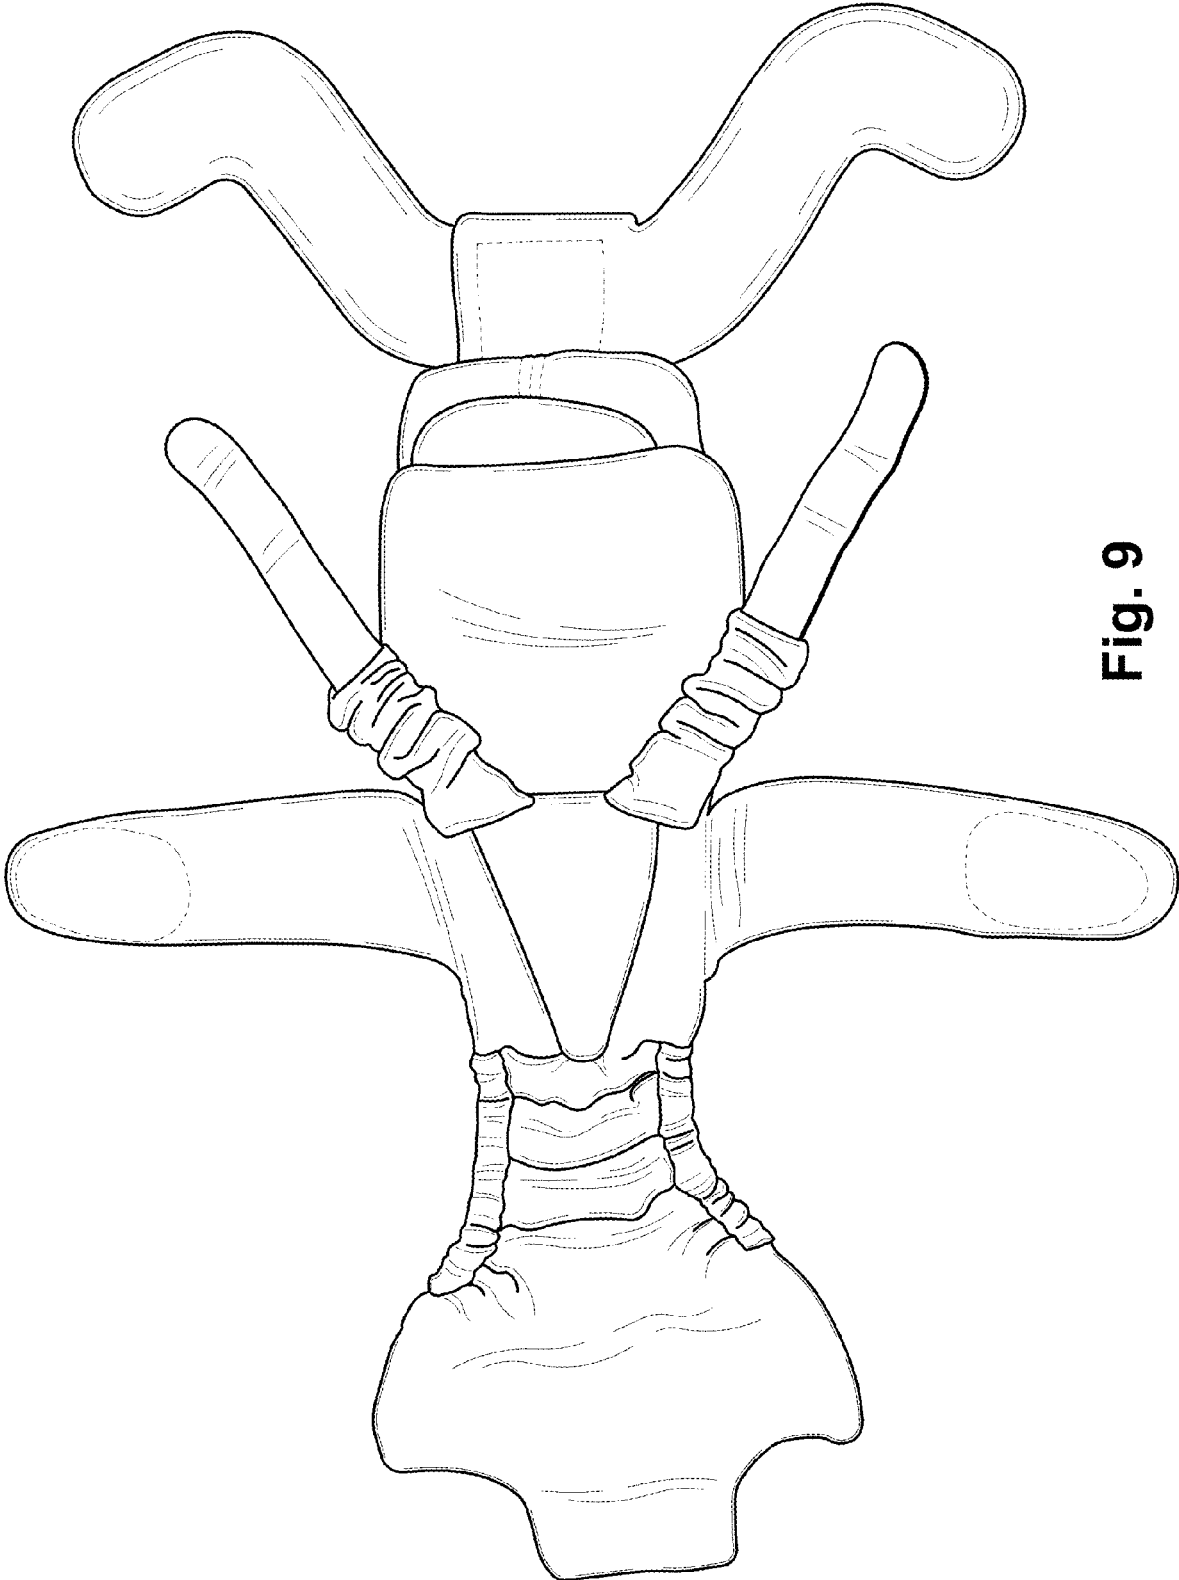


Fig. 9

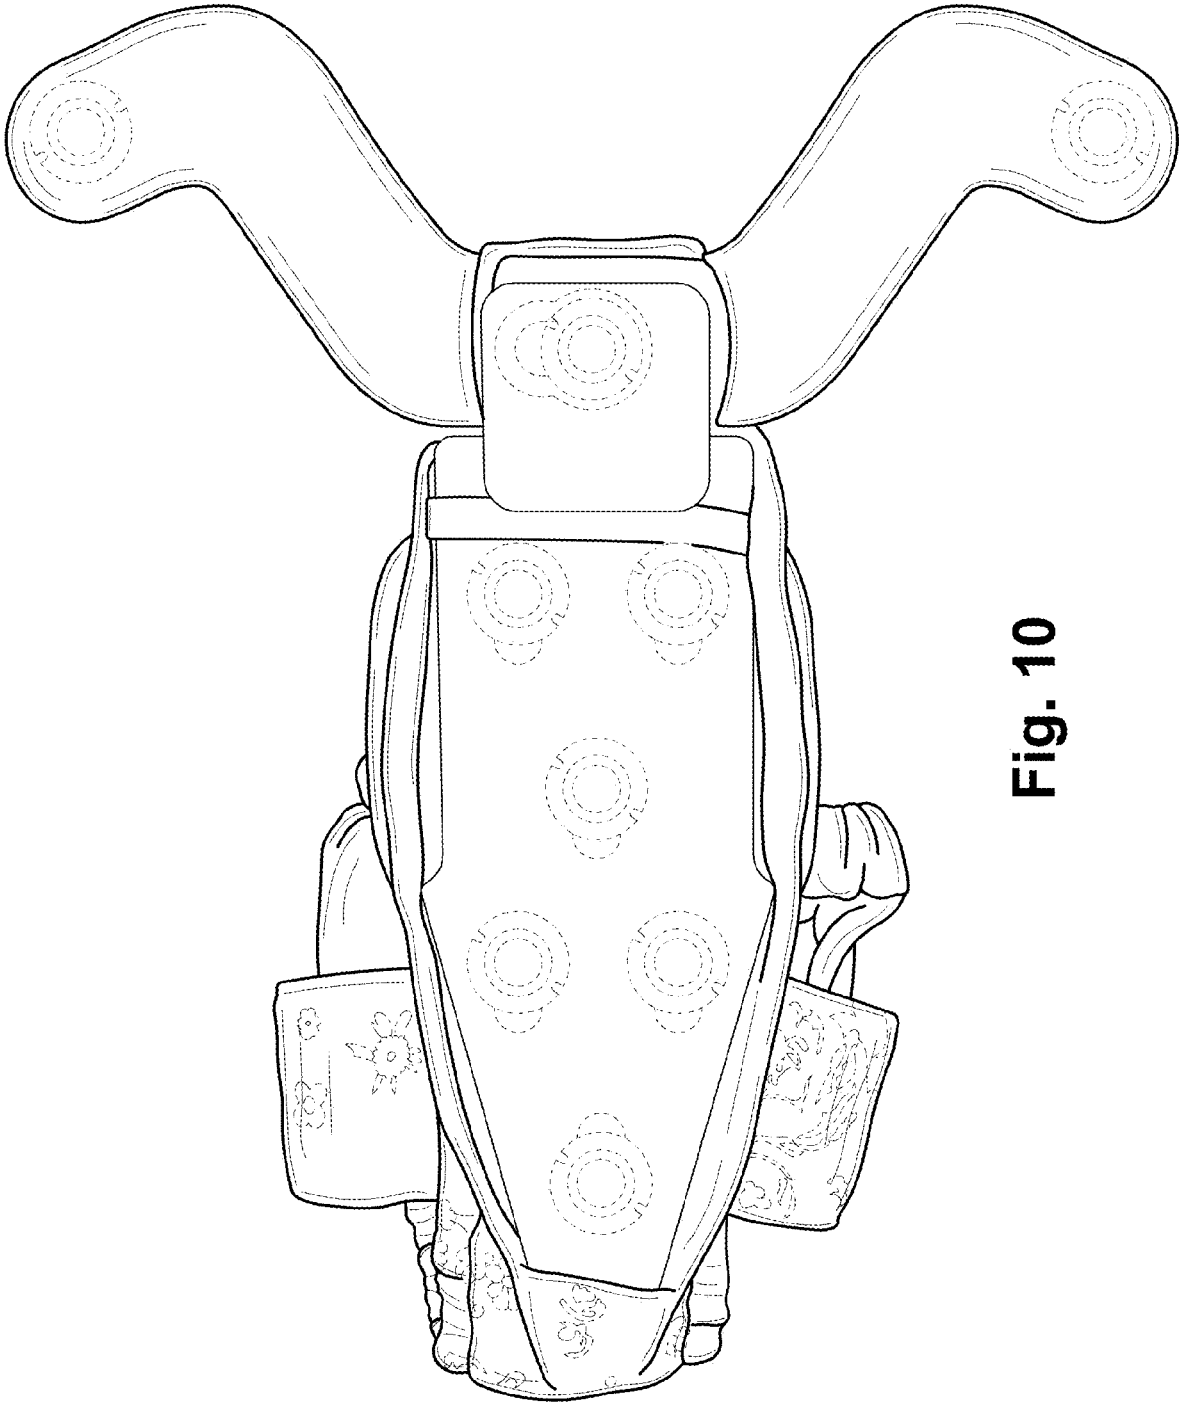


Fig. 10