



US009113884B2

(12) **United States Patent**
Shelton, IV et al.

(10) **Patent No.:** **US 9,113,884 B2**
(45) **Date of Patent:** **Aug. 25, 2015**

(54) **MODULAR SURGICAL TOOL SYSTEMS**

(75) Inventors: **Frederick E. Shelton, IV**, Hillsboro, OH (US); **Jerome R. Morgan**, Cincinnati, OH (US); **Taylor W. Aronhalt**, Loveland, OH (US); **Gregory W. Johnson**, Milford, OH (US); **Chester O. Baxter, III**, Loveland, OH (US); **Joseph E. Young**, Loveland, OH (US); **Barry C. Worrell**, Centerville, OH (US); **Christopher J. Schall**, Cincinnati, OH (US); **Mark S. Ortiz**, Milford, OH (US); **Jason K. Rupert**, Columbia Township, OH (US); **Steven G. Hall**, Cincinnati, OH (US); **Daniel J. Mumaw**, Johannesburg, OH (US); **Aron O. Zingman**, Cambridge, MA (US); **Katherine J. Schmid**, Cincinnati, OH (US); **Jacob S. Gee**, Cincinnati, OH (US); **Richard W. Timm**, Cincinnati, OH (US)

(73) Assignee: **Ethicon Endo-Surgery, Inc.**, Cincinnati, OH (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 843 days.

(21) Appl. No.: **13/181,798**

(22) Filed: **Jul. 13, 2011**

(65) **Prior Publication Data**

US 2012/0239010 A1 Sep. 20, 2012

Related U.S. Application Data

(60) Provisional application No. 61/452,432, filed on Mar. 14, 2011.

(51) **Int. Cl.**

A61B 17/072 (2006.01)

A61B 17/115 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 17/1155** (2013.01); **A61B 17/00234** (2013.01); **A61B 17/3417** (2013.01); **A61B 2017/00287** (2013.01); **A61B 2017/00477** (2013.01); **A61B 2017/07257** (2013.01)

(58) **Field of Classification Search**

CPC . A61B 17/115; A61B 17/1155; A61B 17/105
USPC 227/176.1, 178.1, 179.1, 180.1, 181.1
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,224,882 A 12/1940 Peck
2,742,955 A 4/1956 Dominguez
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2008207624 A1 3/2009
AU 2012200178 B2 7/2013
(Continued)

OTHER PUBLICATIONS

International Search Report for PCT/US2012/028886, dated Nov. 23, 2012 (6 pages).


(Continued)

Primary Examiner — Nathaniel Chukwurah

(57) **ABSTRACT**

Modular surgical instruments are disclosed. In various embodiments, a modular surgical instrument is disclosed for use with a plurality of interchangeable surgical tool heads that are configured to perform different surgical actions. The instrument is configured to apply a plurality of different rotary drive motions and axial drive motions depending upon the type of surgical tool head attached thereto.

14 Claims, 52 Drawing Sheets

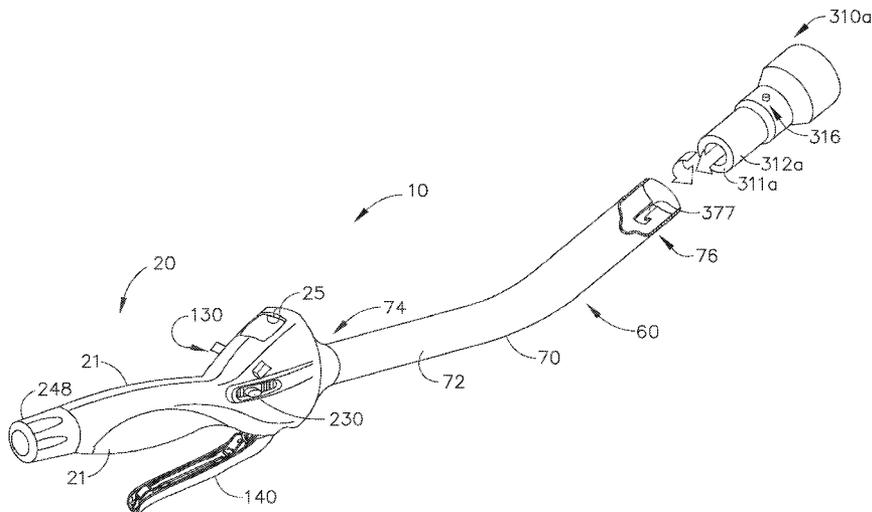

| | | | | | | | | | |
|------|-------------------------|-----------|--|-----------|-----|---------|--------------------------------|--|--|
| (51) | Int. Cl. | | | | | | | | |
| | <i>A61B 17/34</i> | (2006.01) | | 5,366,479 | A | 11/1994 | McGarry et al. | | |
| | <i>A61B 17/00</i> | (2006.01) | | 5,374,277 | A | 12/1994 | Hassler | | |
| | | | | 5,375,588 | A | 12/1994 | Yoon | | |
| | | | | 5,383,880 | A | 1/1995 | Hooven | | |
| | | | | 5,383,888 | A | 1/1995 | Zvenyatsky et al. | | |
| | | | | 5,383,895 | A | 1/1995 | Holmes et al. | | |
| | | | | 5,391,180 | A | 2/1995 | Tovey et al. | | |
| (56) | References Cited | | | 5,395,030 | A * | 3/1995 | Kuramoto et al. 227/179.1 | | |
| | U.S. PATENT DOCUMENTS | | | 5,395,384 | A | 3/1995 | Duthoit | | |
| | | | | 5,404,870 | A | 4/1995 | Brinkerhoff et al. | | |
| | | | | 5,405,072 | A | 4/1995 | Zlock et al. | | |
| | | | | 5,405,344 | A | 4/1995 | Williamson et al. | | |
| | | | | 5,405,360 | A | 4/1995 | Tovey | | |
| | | | | 5,411,508 | A | 5/1995 | Bessler et al. | | |
| | | | | 5,413,272 | A | 5/1995 | Green et al. | | |
| | | | | 5,413,573 | A | 5/1995 | Koivukangas | | |
| | | | | 5,415,334 | A | 5/1995 | Williamson, IV et al. | | |
| | | | | 5,417,361 | A | 5/1995 | Williamson, IV | | |
| | | | | 5,425,745 | A | 6/1995 | Green et al. | | |
| | | | | 5,441,494 | A | 8/1995 | Ortiz | | |
| | | | | 5,445,644 | A | 8/1995 | Pietrafitta et al. | | |
| | | | | 5,449,365 | A | 9/1995 | Green et al. | | |
| | | | | 5,452,837 | A | 9/1995 | Williamson, IV et al. | | |
| | | | | 5,474,057 | A | 12/1995 | Makower et al. | | |
| | | | | 5,476,479 | A | 12/1995 | Green et al. | | |
| | | | | 5,478,354 | A | 12/1995 | Tovey et al. | | |
| | | | | 5,480,089 | A | 1/1996 | Blewett | | |
| | | | | 5,480,409 | A | 1/1996 | Riza | | |
| | | | | 5,482,197 | A | 1/1996 | Green et al. | | |
| | | | | 5,484,095 | A | 1/1996 | Green et al. | | |
| | | | | 5,485,947 | A | 1/1996 | Olson et al. | | |
| | | | | 5,485,952 | A | 1/1996 | Fontayne | | |
| | | | | 5,487,499 | A | 1/1996 | Sorrentino et al. | | |
| | | | | 5,487,500 | A | 1/1996 | Knodel et al. | | |
| | | | | 5,489,058 | A | 2/1996 | Plyley et al. | | |
| | | | | 5,490,819 | A | 2/1996 | Nicholas et al. | | |
| | | | | 5,497,933 | A | 3/1996 | DeFonzo et al. | | |
| | | | | 5,503,320 | A | 4/1996 | Webster et al. | | |
| | | | | 5,503,635 | A | 4/1996 | Sauer et al. | | |
| | | | | 5,505,363 | A | 4/1996 | Green et al. | | |
| | | | | 5,507,426 | A | 4/1996 | Young et al. | | |
| | | | | 5,509,596 | A | 4/1996 | Green et al. | | |
| | | | | 5,511,564 | A | 4/1996 | Wilk | | |
| | | | | 5,514,157 | A | 5/1996 | Nicholas et al. | | |
| | | | | 5,520,609 | A | 5/1996 | Moll et al. | | |
| | | | | 5,520,678 | A | 5/1996 | Heckele et al. | | |
| | | | | 5,527,264 | A | 6/1996 | Moll et al. | | |
| | | | | 5,529,235 | A | 6/1996 | Boiarski et al. | | |
| | | | | 5,531,856 | A | 7/1996 | Moll et al. | | |
| | | | | 5,533,661 | A | 7/1996 | Main et al. | | |
| | | | | 5,535,934 | A | 7/1996 | Boiarski et al. | | |
| | | | | 5,540,375 | A | 7/1996 | Bolanos et al. | | |
| | | | | 5,542,594 | A | 8/1996 | McKean et al. | | |
| | | | | 5,549,621 | A | 8/1996 | Bessler et al. | | |
| | | | | 5,549,637 | A | 8/1996 | Crainich | | |
| | | | | 5,551,622 | A | 9/1996 | Yoon | | |
| | | | | 5,553,765 | A | 9/1996 | Knodel et al. | | |
| | | | | 5,554,169 | A | 9/1996 | Green et al. | | |
| | | | | 5,556,416 | A | 9/1996 | Clark et al. | | |
| | | | | 5,558,665 | A | 9/1996 | Kieturakis | | |
| | | | | 5,560,530 | A | 10/1996 | Bolanos et al. | | |
| | | | | 5,560,532 | A | 10/1996 | DeFonzo et al. | | |
| | | | | 5,562,241 | A | 10/1996 | Knodel et al. | | |
| | | | | 5,562,690 | A | 10/1996 | Green et al. | | |
| | | | | 5,562,701 | A | 10/1996 | Huitema et al. | | |
| | | | | 5,562,702 | A | 10/1996 | Huitema et al. | | |
| | | | | 5,564,615 | A | 10/1996 | Bishop et al. | | |
| | | | | 5,571,285 | A | 11/1996 | Chow et al. | | |
| | | | | 5,575,803 | A | 11/1996 | Cooper et al. | | |
| | | | | 5,575,805 | A | 11/1996 | Li | | |
| | | | | 5,577,654 | A | 11/1996 | Bishop | | |
| | | | | 5,580,067 | A | 12/1996 | Hamblin et al. | | |
| | | | | 5,586,711 | A | 12/1996 | Plyley et al. | | |
| | | | | 5,588,579 | A | 12/1996 | Schnut et al. | | |
| | | | | 5,588,580 | A | 12/1996 | Paul et al. | | |
| | | | | 5,588,581 | A | 12/1996 | Conlon et al. | | |
| | | | | 5,601,224 | A | 2/1997 | Bishop et al. | | |
| | | | | 5,603,443 | A | 2/1997 | Clark et al. | | |
| | | | | 5,605,273 | A | 2/1997 | Hamblin et al. | | |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|-------------|---------|---------------------|--------------|---------|-----------------------|
| 5,607,094 A | 3/1997 | Clark et al. | 5,782,859 A | 7/1998 | Nicholas et al. |
| 5,607,450 A | 3/1997 | Zvenyatsky et al. | 5,785,232 A | 7/1998 | Vidal et al. |
| 5,609,285 A | 3/1997 | Grant et al. | 5,785,647 A | 7/1998 | Tompkins et al. |
| 5,613,937 A | 3/1997 | Garrison et al. | 5,787,897 A | 8/1998 | Kieturakis |
| 5,615,820 A | 4/1997 | Viola | 5,792,135 A | 8/1998 | Madhani et al. |
| 5,618,303 A | 4/1997 | Marlow et al. | 5,797,536 A | 8/1998 | Smith et al. |
| 5,618,307 A | 4/1997 | Donlon et al. | 5,797,537 A | 8/1998 | Oberlin et al. |
| 5,620,452 A | 4/1997 | Yoon | 5,797,538 A | 8/1998 | Heaton et al. |
| 5,628,446 A | 5/1997 | Geiste et al. | 5,797,959 A | 8/1998 | Castro et al. |
| 5,628,743 A | 5/1997 | Cimino | 5,799,857 A | 9/1998 | Robertson et al. |
| 5,630,539 A | 5/1997 | Plyley et al. | 5,807,376 A | 9/1998 | Viola et al. |
| 5,630,540 A | 5/1997 | Blewett | 5,807,378 A | 9/1998 | Jensen et al. |
| 5,632,432 A | 5/1997 | Schulze et al. | 5,810,721 A | 9/1998 | Mueller et al. |
| 5,632,433 A | 5/1997 | Grant et al. | 5,810,855 A | 9/1998 | Rayburn et al. |
| 5,634,584 A | 6/1997 | Okorocho et al. | 5,814,055 A | 9/1998 | Knodel et al. |
| 5,636,780 A | 6/1997 | Green et al. | 5,814,057 A | 9/1998 | Oi et al. |
| 5,639,008 A | 6/1997 | Gallagher et al. | 5,817,084 A | 10/1998 | Jensen |
| 5,651,491 A | 7/1997 | Heaton et al. | 5,820,009 A | 10/1998 | Melling et al. |
| 5,651,762 A | 7/1997 | Bridges | 5,826,776 A | 10/1998 | Schulze et al. |
| 5,653,373 A | 8/1997 | Green et al. | 5,836,503 A | 11/1998 | Ehrenfels et al. |
| 5,653,374 A | 8/1997 | Young et al. | 5,839,369 A | 11/1998 | Chatterjee et al. |
| 5,653,721 A | 8/1997 | Knodel et al. | 5,839,639 A | 11/1998 | Sauer et al. |
| 5,655,698 A | 8/1997 | Yoon | 5,843,096 A | 12/1998 | Igaki et al. |
| 5,657,921 A | 8/1997 | Young et al. | 5,855,311 A | 1/1999 | Hamblin et al. |
| 5,662,258 A | 9/1997 | Knodel et al. | 5,860,581 A | 1/1999 | Robertson et al. |
| 5,662,260 A | 9/1997 | Yoon | 5,865,361 A | 2/1999 | Milliman et al. |
| 5,667,517 A | 9/1997 | Hooven | 5,871,135 A | 2/1999 | Williamson, IV et al. |
| 5,667,526 A | 9/1997 | Levin | 5,901,895 A | 5/1999 | Heaton et al. |
| 5,667,527 A | 9/1997 | Cook | 5,906,577 A | 5/1999 | Beane et al. |
| 5,669,544 A | 9/1997 | Schulze et al. | 5,906,625 A | 5/1999 | Bitto et al. |
| 5,673,840 A | 10/1997 | Schulze et al. | 5,911,353 A | 6/1999 | Bolanos et al. |
| 5,673,841 A | 10/1997 | Schulze et al. | 5,915,616 A | 6/1999 | Viola et al. |
| 5,680,981 A | 10/1997 | Mililli et al. | 5,931,853 A | 8/1999 | McEwen et al. |
| 5,680,982 A | 10/1997 | Schulze et al. | 5,937,951 A | 8/1999 | Izchukwu et al. |
| 5,681,341 A | 10/1997 | Lunsford et al. | 5,938,667 A | 8/1999 | Peysner et al. |
| 5,683,349 A | 11/1997 | Makower et al. | 5,941,442 A | 8/1999 | Geiste et al. |
| 5,685,474 A | 11/1997 | Seeber | 5,947,984 A | 9/1999 | Whipple |
| 5,690,269 A | 11/1997 | Bolanos et al. | 5,954,259 A | 9/1999 | Viola et al. |
| 5,692,668 A | 12/1997 | Schulze et al. | 5,964,774 A | 10/1999 | McKean et al. |
| 5,695,504 A | 12/1997 | Gifford, III et al. | 5,997,528 A | 12/1999 | Bisch et al. |
| 5,695,524 A | 12/1997 | Kelley et al. | 6,003,517 A | 12/1999 | Sheffield et al. |
| 5,697,543 A | 12/1997 | Burdorff | 6,010,054 A | 1/2000 | Johnson et al. |
| 5,697,943 A | 12/1997 | Sauer et al. | 6,017,356 A | 1/2000 | Frederick et al. |
| 5,700,270 A | 12/1997 | Peysner et al. | 6,024,748 A | 2/2000 | Manzo et al. |
| 5,702,409 A | 12/1997 | Rayburn et al. | 6,032,849 A | 3/2000 | Mastri et al. |
| 5,704,534 A | 1/1998 | Huitema et al. | 6,053,390 A | 4/2000 | Green et al. |
| 5,707,392 A | 1/1998 | Kortenbach | RE36,720 E | 5/2000 | Green et al. |
| 5,709,706 A | 1/1998 | Kienzle et al. | 6,056,735 A | 5/2000 | Okada et al. |
| 5,711,472 A | 1/1998 | Bryan | 6,063,025 A | 5/2000 | Bridges et al. |
| 5,713,505 A | 2/1998 | Huitema | 6,063,097 A | 5/2000 | Oi et al. |
| 5,715,987 A | 2/1998 | Kelley et al. | 6,083,234 A | 7/2000 | Nicholas et al. |
| 5,718,360 A | 2/1998 | Green et al. | 6,083,242 A | 7/2000 | Cook |
| 5,725,554 A | 3/1998 | Simon et al. | 6,099,551 A | 8/2000 | Gabbay |
| 5,728,121 A | 3/1998 | Bimbo et al. | 6,102,271 A | 8/2000 | Longo et al. |
| 5,730,758 A | 3/1998 | Allgeyer | 6,117,158 A | 9/2000 | Measamer et al. |
| 5,732,871 A | 3/1998 | Clark et al. | 6,119,913 A | 9/2000 | Adams et al. |
| 5,732,872 A | 3/1998 | Bolduc et al. | 6,126,058 A | 10/2000 | Adams et al. |
| 5,735,874 A | 4/1998 | Measamer et al. | 6,142,933 A | 11/2000 | Longo et al. |
| 5,738,629 A | 4/1998 | Moll et al. | 6,159,146 A | 12/2000 | El Gazayerli |
| 5,741,271 A | 4/1998 | Nakao et al. | 6,159,200 A | 12/2000 | Verdura et al. |
| 5,743,456 A | 4/1998 | Jones et al. | 6,162,208 A | 12/2000 | Hipps |
| 5,749,889 A | 5/1998 | Bacich et al. | 6,165,188 A | 12/2000 | Saadat et al. |
| 5,749,893 A | 5/1998 | Vidal et al. | 6,171,330 B1 | 1/2001 | Benchetrit |
| 5,752,644 A | 5/1998 | Bolanos et al. | 6,174,318 B1 | 1/2001 | Bates et al. |
| 5,752,965 A | 5/1998 | Francis et al. | 6,193,129 B1 | 2/2001 | Bittner et al. |
| 5,752,970 A | 5/1998 | Yoon | 6,202,914 B1 | 3/2001 | Geiste et al. |
| 5,758,814 A | 6/1998 | Gallagher et al. | 6,214,028 B1 | 4/2001 | Yoon et al. |
| 5,762,256 A | 6/1998 | Mastri et al. | 6,221,007 B1 | 4/2001 | Green |
| 5,766,188 A | 6/1998 | Igaki | 6,231,565 B1 | 5/2001 | Tovey et al. |
| 5,766,205 A | 6/1998 | Zvenyatsky et al. | 6,234,178 B1 | 5/2001 | Goble et al. |
| 5,769,892 A | 6/1998 | Kingwell | 6,241,139 B1 | 6/2001 | Milliman et al. |
| 5,779,130 A | 7/1998 | Alesi et al. | 6,248,117 B1 | 6/2001 | Blatter |
| 5,779,131 A | 7/1998 | Knodel et al. | 6,250,532 B1 | 6/2001 | Green et al. |
| 5,779,132 A | 7/1998 | Knodel et al. | 6,254,534 B1 | 7/2001 | Butler et al. |
| 5,782,397 A | 7/1998 | Koukline | 6,258,107 B1 | 7/2001 | Balazs et al. |
| | | | 6,264,086 B1 | 7/2001 | McGuckin, Jr. |
| | | | 6,264,087 B1 | 7/2001 | Whitman |
| | | | 6,302,311 B1 | 10/2001 | Adams et al. |
| | | | 6,309,403 B1 | 10/2001 | Minor et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|----------------|---------|-----------------------|----------------|---------|---------------------------|
| 6,315,184 B1 | 11/2001 | Whitman | 6,827,712 B2 | 12/2004 | Tovey et al. |
| 6,325,810 B1 | 12/2001 | Hamilton et al. | 6,830,174 B2 | 12/2004 | Hillstead et al. |
| 6,330,965 B1 | 12/2001 | Milliman et al. | 6,835,199 B2 | 12/2004 | McGuckin, Jr. et al. |
| 6,331,181 B1 | 12/2001 | Tierney et al. | 6,843,403 B2 | 1/2005 | Whitman |
| 6,338,737 B1 | 1/2002 | Toledano | 6,846,307 B2 * | 1/2005 | Whitman et al. 606/1 |
| 6,346,077 B1 | 2/2002 | Taylor et al. | 6,846,308 B2 | 1/2005 | Whitman et al. |
| 6,352,503 B1 | 3/2002 | Matsui et al. | 6,846,309 B2 | 1/2005 | Whitman et al. |
| 6,364,888 B1 | 4/2002 | Niemeyer et al. | 6,849,071 B2 | 2/2005 | Whitman et al. |
| 6,387,113 B1 | 5/2002 | Hawkins et al. | RE38,708 E | 3/2005 | Bolanos et al. |
| 6,391,038 B2 | 5/2002 | Vargas et al. | 6,866,178 B2 | 3/2005 | Adams et al. |
| 6,398,797 B2 | 6/2002 | Bombard et al. | 6,866,671 B2 | 3/2005 | Tierney et al. |
| 6,402,766 B2 | 6/2002 | Bowman et al. | 6,872,214 B2 | 3/2005 | Sonnenschein et al. |
| RE37,814 E | 8/2002 | Allgeyer | 6,874,669 B2 | 4/2005 | Adams et al. |
| 6,436,110 B2 | 8/2002 | Bowman et al. | 6,877,647 B2 | 4/2005 | Green et al. |
| 6,436,122 B1 | 8/2002 | Frank et al. | 6,905,057 B2 | 6/2005 | Swayze et al. |
| 6,440,146 B2 | 8/2002 | Nicholas et al. | 6,913,608 B2 | 7/2005 | Liddicoat et al. |
| 6,443,973 B1 * | 9/2002 | Whitman 606/219 | 6,913,613 B2 | 7/2005 | Schwarz et al. |
| 6,447,523 B1 | 9/2002 | Middleman et al. | 6,936,042 B2 | 8/2005 | Wallace et al. |
| 6,450,391 B1 | 9/2002 | Kayan et al. | 6,939,358 B2 | 9/2005 | Palacios et al. |
| 6,458,077 B1 | 10/2002 | Boebel et al. | 6,945,444 B2 | 9/2005 | Gresham et al. |
| 6,488,196 B1 | 12/2002 | Fenton, Jr. | 6,953,138 B1 | 10/2005 | Dworak et al. |
| 6,488,197 B1 | 12/2002 | Whitman | 6,953,139 B2 | 10/2005 | Milliman et al. |
| 6,491,201 B1 | 12/2002 | Whitman | 6,959,851 B2 | 11/2005 | Heinrich |
| 6,491,701 B2 | 12/2002 | Tierney et al. | 6,960,220 B2 | 11/2005 | Marino et al. |
| 6,494,885 B1 | 12/2002 | Dhindsa | 6,964,363 B2 | 11/2005 | Wales et al. |
| 6,503,257 B2 | 1/2003 | Grant et al. | 6,971,988 B2 | 12/2005 | Orban, III |
| 6,503,259 B2 | 1/2003 | Huxel et al. | 6,978,921 B2 | 12/2005 | Shelton, IV et al. |
| 6,505,768 B2 | 1/2003 | Whitman | 6,978,922 B2 | 12/2005 | Bilotti et al. |
| 6,510,854 B2 | 1/2003 | Goble | 6,981,628 B2 | 1/2006 | Wales |
| 6,517,528 B1 | 2/2003 | Pantages et al. | 6,981,978 B2 | 1/2006 | Gannoe |
| 6,517,565 B1 | 2/2003 | Whitman et al. | 6,986,451 B1 | 1/2006 | Mastri et al. |
| 6,517,566 B1 | 2/2003 | Hovland et al. | 6,988,650 B2 | 1/2006 | Schwemberger et al. |
| 6,533,157 B1 | 3/2003 | Whitman | 7,000,818 B2 | 2/2006 | Shelton, IV et al. |
| 6,543,456 B1 | 4/2003 | Freeman | 7,000,819 B2 | 2/2006 | Swayze et al. |
| 6,551,333 B2 | 4/2003 | Kuhns et al. | 7,001,408 B2 | 2/2006 | Knodel et al. |
| 6,569,171 B2 | 5/2003 | DeGuillebon et al. | 7,032,798 B2 | 4/2006 | Whitman et al. |
| 6,578,751 B2 | 6/2003 | Hartwick | 7,032,799 B2 | 4/2006 | Viola et al. |
| 6,582,364 B2 | 6/2003 | Butler et al. | 7,044,352 B2 | 5/2006 | Shelton, IV et al. |
| 6,588,643 B2 | 7/2003 | Bolduc et al. | 7,044,353 B2 | 5/2006 | Mastri et al. |
| 6,592,597 B2 | 7/2003 | Grant et al. | 7,052,454 B2 | 5/2006 | Taylor |
| 6,601,749 B2 | 8/2003 | Sullivan et al. | 7,055,731 B2 | 6/2006 | Shelton, IV et al. |
| 6,605,078 B2 | 8/2003 | Adams | 7,056,330 B2 | 6/2006 | Gayton |
| 6,616,686 B2 | 9/2003 | Coleman et al. | 7,059,331 B2 | 6/2006 | Adams et al. |
| 6,619,529 B2 | 9/2003 | Green et al. | 7,063,712 B2 | 6/2006 | Vargas et al. |
| 6,629,630 B2 | 10/2003 | Adams | 7,066,944 B2 | 6/2006 | Laufer et al. |
| 6,629,988 B2 | 10/2003 | Weadock | 7,070,083 B2 | 7/2006 | Jankowski |
| 6,638,285 B2 | 10/2003 | Gabbay | 7,077,856 B2 | 7/2006 | Whitman |
| 6,638,297 B1 | 10/2003 | Huitema | 7,080,769 B2 | 7/2006 | Vresh et al. |
| 6,644,532 B2 | 11/2003 | Green et al. | 7,083,075 B2 | 8/2006 | Swayze et al. |
| 6,645,201 B1 | 11/2003 | Utley et al. | 7,083,626 B2 | 8/2006 | Hart et al. |
| 6,656,193 B2 | 12/2003 | Grant et al. | 7,087,071 B2 | 8/2006 | Nicholas et al. |
| 6,666,854 B1 | 12/2003 | Lange | 7,090,683 B2 | 8/2006 | Brock et al. |
| 6,681,978 B2 | 1/2004 | Geiste et al. | 7,094,247 B2 | 8/2006 | Monassevitch et al. |
| 6,681,979 B2 | 1/2004 | Whitman | 7,108,701 B2 | 9/2006 | Evens et al. |
| 6,692,507 B2 | 2/2004 | Pugsley et al. | 7,108,709 B2 | 9/2006 | Cummins |
| 6,695,199 B2 | 2/2004 | Whitman | 7,111,769 B2 | 9/2006 | Wales et al. |
| 6,698,643 B2 | 3/2004 | Whitman | 7,114,642 B2 | 10/2006 | Whitman |
| 6,699,235 B2 | 3/2004 | Wallace et al. | 7,121,446 B2 | 10/2006 | Arad et al. |
| 6,716,232 B1 | 4/2004 | Vidal et al. | 7,122,028 B2 | 10/2006 | Looper et al. |
| 6,716,233 B1 | 4/2004 | Whitman | 7,128,253 B2 | 10/2006 | Mastri et al. |
| 6,722,552 B2 | 4/2004 | Fenton, Jr. | 7,128,254 B2 | 10/2006 | Shelton, IV et al. |
| 6,723,087 B2 | 4/2004 | O'Neill et al. | 7,128,748 B2 | 10/2006 | Mooradian et al. |
| 6,726,697 B2 | 4/2004 | Nicholas et al. | 7,131,445 B2 | 11/2006 | Amoah |
| 6,736,825 B2 | 5/2004 | Blatter et al. | 7,134,587 B2 | 11/2006 | Schwemberger et al. |
| 6,755,338 B2 | 6/2004 | Hahnen et al. | 7,140,527 B2 | 11/2006 | Ehrenfels et al. |
| 6,769,590 B2 | 8/2004 | Vresh et al. | 7,147,138 B2 | 12/2006 | Shelton, IV |
| 6,769,594 B2 | 8/2004 | Orban, III | 7,147,139 B2 | 12/2006 | Schwemberger et al. |
| 6,780,151 B2 | 8/2004 | Grabover et al. | 7,147,650 B2 | 12/2006 | Lee |
| 6,786,382 B1 | 9/2004 | Hoffman | 7,156,863 B2 | 1/2007 | Sonnenschein et al. |
| 6,786,896 B1 | 9/2004 | Madhani et al. | 7,159,750 B2 | 1/2007 | Racenet et al. |
| 6,793,652 B1 | 9/2004 | Whitman et al. | 7,168,604 B2 | 1/2007 | Milliman et al. |
| 6,805,273 B2 | 10/2004 | Bilotti et al. | 7,179,267 B2 | 2/2007 | Nolan et al. |
| 6,817,508 B1 | 11/2004 | Racenet et al. | 7,182,239 B1 | 2/2007 | Myers |
| 6,817,509 B2 | 11/2004 | Geiste et al. | 7,188,758 B2 | 3/2007 | Viola et al. |
| 6,821,284 B2 | 11/2004 | Sturtz et al. | 7,207,471 B2 | 4/2007 | Heinrich et al. |
| | | | 7,207,472 B2 | 4/2007 | Wukusick et al. |
| | | | 7,208,005 B2 | 4/2007 | Frecker et al. |
| | | | 7,210,609 B2 | 5/2007 | Leiboff et al. |
| | | | 7,213,736 B2 | 5/2007 | Wales et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|---------|----------------------|--------------|---------|------------------------|
| 7,220,272 B2 | 5/2007 | Weadock | 7,494,499 B2 | 2/2009 | Nagase et al. |
| 7,225,964 B2 | 6/2007 | Mastri et al. | 7,500,979 B2 | 3/2009 | Hueil et al. |
| 7,229,408 B2 | 6/2007 | Douglas et al. | 7,503,474 B2 | 3/2009 | Hillstead et al. |
| 7,234,624 B2 | 6/2007 | Gresham et al. | 7,506,790 B2 | 3/2009 | Shelton, IV |
| 7,237,708 B1 | 7/2007 | Guy et al. | 7,506,791 B2 | 3/2009 | Omaits et al. |
| 7,238,195 B2 | 7/2007 | Viola | 7,510,107 B2 | 3/2009 | Timm et al. |
| 7,241,288 B2 | 7/2007 | Braun | 7,517,356 B2 | 4/2009 | Heinrich |
| 7,246,734 B2 | 7/2007 | Shelton, IV | 7,524,320 B2 | 4/2009 | Tierney et al. |
| 7,252,660 B2 | 8/2007 | Kunz | 7,546,940 B2 | 6/2009 | Milliman et al. |
| 7,258,262 B2 | 8/2007 | Mastri et al. | 7,547,312 B2 | 6/2009 | Bauman et al. |
| 7,267,679 B2 | 9/2007 | McGuckin, Jr. et al. | 7,549,563 B2 | 6/2009 | Mather et al. |
| 7,278,562 B2 | 10/2007 | Mastri et al. | 7,549,564 B2 | 6/2009 | Boudreaux |
| 7,278,563 B1 | 10/2007 | Green | 7,549,998 B2 | 6/2009 | Braun |
| 7,296,722 B2 | 11/2007 | Ivanko | 7,556,185 B2 | 7/2009 | Viola |
| 7,296,724 B2 | 11/2007 | Green et al. | 7,559,449 B2 | 7/2009 | Viola |
| 7,297,149 B2 | 11/2007 | Vitali et al. | 7,559,450 B2 | 7/2009 | Wales et al. |
| 7,300,450 B2 | 11/2007 | Vleugels et al. | 7,559,452 B2 | 7/2009 | Wales et al. |
| 7,303,106 B2 | 12/2007 | Milliman et al. | 7,565,993 B2 | 7/2009 | Milliman et al. |
| 7,303,107 B2 | 12/2007 | Milliman et al. | 7,568,603 B2 | 8/2009 | Shelton, IV et al. |
| 7,303,108 B2 | 12/2007 | Shelton, IV | 7,568,604 B2 | 8/2009 | Ehrenfels et al. |
| 7,308,998 B2 | 12/2007 | Mastri et al. | 7,575,144 B2 | 8/2009 | Ortiz et al. |
| 7,328,828 B2 | 2/2008 | Ortiz et al. | 7,588,174 B2 | 9/2009 | Holsten et al. |
| 7,328,829 B2 | 2/2008 | Arad et al. | 7,588,175 B2 | 9/2009 | Timm et al. |
| 7,334,717 B2 | 2/2008 | Rethy et al. | 7,588,176 B2 | 9/2009 | Timm et al. |
| 7,334,718 B2 | 2/2008 | McAlister et al. | 7,588,177 B2 | 9/2009 | Racenet |
| 7,338,505 B2 | 3/2008 | Belson | 7,597,229 B2 | 10/2009 | Boudreaux et al. |
| 7,338,513 B2 | 3/2008 | Lee et al. | 7,597,230 B2 | 10/2009 | Racenet et al. |
| 7,343,920 B2 | 3/2008 | Toby et al. | 7,604,150 B2 | 10/2009 | Boudreaux |
| RE40,237 E | 4/2008 | Bilotti et al. | 7,604,151 B2 | 10/2009 | Hess et al. |
| 7,354,447 B2 | 4/2008 | Shelton, IV et al. | 7,607,557 B2 | 10/2009 | Shelton, IV et al. |
| 7,357,287 B2 | 4/2008 | Shelton, IV et al. | 7,611,038 B2 | 11/2009 | Racenet et al. |
| 7,364,060 B2 | 4/2008 | Milliman | 7,624,902 B2 | 12/2009 | Marczyk et al. |
| 7,364,061 B2 | 4/2008 | Swayze et al. | 7,624,903 B2 | 12/2009 | Green et al. |
| 7,377,928 B2 | 5/2008 | Zubik et al. | 7,631,793 B2 | 12/2009 | Rethy et al. |
| 7,380,695 B2 | 6/2008 | Doll et al. | 7,635,074 B2 | 12/2009 | Olson et al. |
| 7,380,696 B2 | 6/2008 | Shelton, IV et al. | 7,637,409 B2 | 12/2009 | Marczyk |
| 7,398,907 B2 | 7/2008 | Racenet et al. | 7,641,095 B2 | 1/2010 | Viola |
| 7,398,908 B2 | 7/2008 | Holsten et al. | 7,644,848 B2 | 1/2010 | Swayze et al. |
| 7,401,721 B2 | 7/2008 | Holsten et al. | 7,648,519 B2 | 1/2010 | Lee et al. |
| 7,404,508 B2 | 7/2008 | Smith et al. | 7,651,017 B2 | 1/2010 | Ortiz et al. |
| 7,404,509 B2 | 7/2008 | Ortiz et al. | 7,654,431 B2 | 2/2010 | Hueil et al. |
| 7,404,822 B2 | 7/2008 | Viart et al. | 7,658,311 B2 | 2/2010 | Boudreaux |
| 7,407,075 B2 | 8/2008 | Holsten et al. | 7,658,312 B2 | 2/2010 | Vidal et al. |
| 7,407,076 B2 | 8/2008 | Racenet et al. | 7,662,161 B2 | 2/2010 | Briganti et al. |
| 7,407,078 B2 | 8/2008 | Shelton, IV et al. | 7,665,646 B2 | 2/2010 | Prommersberger |
| 7,410,086 B2 | 8/2008 | Ortiz et al. | 7,665,647 B2 | 2/2010 | Shelton, IV et al. |
| 7,416,101 B2 | 8/2008 | Shelton, IV et al. | 7,669,746 B2 | 3/2010 | Shelton, IV |
| RE40,514 E | 9/2008 | Mastri et al. | 7,669,747 B2 | 3/2010 | Weisenburgh, II et al. |
| 7,419,080 B2 | 9/2008 | Smith et al. | 7,670,334 B2 | 3/2010 | Hueil et al. |
| 7,419,081 B2 | 9/2008 | Ehrenfels et al. | 7,673,780 B2 | 3/2010 | Shelton, IV et al. |
| 7,422,136 B1 | 9/2008 | Marczyk | 7,673,781 B2 | 3/2010 | Swayze et al. |
| 7,422,139 B2 | 9/2008 | Shelton, IV et al. | 7,673,782 B2 | 3/2010 | Hess et al. |
| 7,424,965 B2 | 9/2008 | Racenet et al. | 7,673,783 B2 | 3/2010 | Morgan et al. |
| 7,431,188 B1 | 10/2008 | Marczyk | 7,674,255 B2 | 3/2010 | Braun |
| 7,431,189 B2 | 10/2008 | Shelton, IV et al. | 7,682,686 B2 | 3/2010 | Curro et al. |
| 7,431,730 B2 | 10/2008 | Viola | 7,686,201 B2 | 3/2010 | Csiky |
| 7,434,717 B2 | 10/2008 | Shelton, IV et al. | 7,686,826 B2 | 3/2010 | Lee et al. |
| 7,438,209 B1 | 10/2008 | Hess et al. | 7,691,098 B2 | 4/2010 | Wallace et al. |
| 7,438,718 B2 | 10/2008 | Milliman et al. | 7,699,204 B2 | 4/2010 | Viola |
| 7,441,684 B2 | 10/2008 | Shelton, IV et al. | 7,699,844 B2 | 4/2010 | Utley et al. |
| 7,441,685 B1 | 10/2008 | Boudreaux | 7,699,859 B2 | 4/2010 | Bombard et al. |
| 7,448,525 B2 | 11/2008 | Shelton, IV et al. | 7,708,180 B2 | 5/2010 | Murray et al. |
| 7,455,208 B2 | 11/2008 | Wales et al. | 7,708,181 B2 | 5/2010 | Cole et al. |
| 7,455,682 B2 | 11/2008 | Viola | 7,708,758 B2 | 5/2010 | Lee et al. |
| 7,464,846 B2 | 12/2008 | Shelton, IV et al. | 7,717,312 B2 | 5/2010 | Beetel |
| 7,464,849 B2 | 12/2008 | Shelton, IV et al. | 7,717,313 B2 | 5/2010 | Crisuolo et al. |
| 7,467,740 B2 | 12/2008 | Shelton, IV et al. | 7,721,930 B2 | 5/2010 | McKenna et al. |
| 7,472,815 B2 | 1/2009 | Shelton, IV et al. | 7,721,931 B2 | 5/2010 | Shelton, IV et al. |
| 7,473,221 B2 | 1/2009 | Ewers et al. | 7,721,933 B2 | 5/2010 | Ehrenfels et al. |
| 7,481,347 B2 | 1/2009 | Roy | 7,721,934 B2 | 5/2010 | Shelton, IV et al. |
| 7,481,349 B2 | 1/2009 | Holsten et al. | 7,721,936 B2 | 5/2010 | Shelton, IV et al. |
| 7,481,824 B2 | 1/2009 | Boudreaux et al. | 7,726,537 B2 | 6/2010 | Olson et al. |
| 7,490,749 B2 | 2/2009 | Schall et al. | 7,726,538 B2 | 6/2010 | Holsten et al. |
| 7,491,232 B2 | 2/2009 | Bolduc et al. | 7,731,072 B2 | 6/2010 | Timm et al. |
| 7,494,039 B2 | 2/2009 | Racenet et al. | 7,735,703 B2 | 6/2010 | Morgan et al. |
| | | | 7,736,306 B2 | 6/2010 | Brustad et al. |
| | | | 7,738,971 B2 | 6/2010 | Swayze et al. |
| | | | 7,740,159 B2 | 6/2010 | Shelton, IV et al. |
| | | | 7,743,960 B2 | 6/2010 | Whitman et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|---------|--------------------|--------------|---------|---------------------|
| 7,744,624 B2 | 6/2010 | Bettuchi | 7,934,630 B2 | 5/2011 | Shelton, IV et al. |
| 7,744,628 B2 | 6/2010 | Viola | 7,934,631 B2 | 5/2011 | Balbierz et al. |
| 7,753,245 B2 | 7/2010 | Boudreaux et al. | 7,938,307 B2 | 5/2011 | Bettuchi |
| 7,753,904 B2 | 7/2010 | Shelton, IV et al. | 7,942,890 B2 | 5/2011 | D'Agostino et al. |
| 7,758,612 B2 | 7/2010 | Shipp | 7,950,560 B2 | 5/2011 | Zemlok et al. |
| 7,766,209 B2 | 8/2010 | Baxter, III et al. | 7,950,561 B2 | 5/2011 | Aranyi |
| 7,766,210 B2 | 8/2010 | Shelton, IV et al. | 7,954,682 B2 | 6/2011 | Giordano et al. |
| 7,766,821 B2 | 8/2010 | Brunnen et al. | 7,954,684 B2 | 6/2011 | Boudreaux |
| 7,770,773 B2 | 8/2010 | Whitman et al. | 7,954,686 B2 | 6/2011 | Baxter, III et al. |
| 7,770,774 B2 | 8/2010 | Mastri et al. | 7,954,687 B2 | 6/2011 | Zemlok et al. |
| 7,770,775 B2 | 8/2010 | Shelton, IV et al. | 7,955,253 B2 | 6/2011 | Ewers et al. |
| 7,770,776 B2 | 8/2010 | Chen et al. | 7,955,257 B2 | 6/2011 | Frasier et al. |
| 7,776,060 B2 | 8/2010 | Mooradian et al. | 7,959,051 B2 | 6/2011 | Smith et al. |
| 7,780,054 B2 | 8/2010 | Wales | 7,963,432 B2 | 6/2011 | Knodel et al. |
| 7,780,685 B2 | 8/2010 | Hunt et al. | 7,966,799 B2 | 6/2011 | Morgan et al. |
| 7,784,662 B2 | 8/2010 | Wales et al. | 7,967,180 B2 | 6/2011 | Scirica |
| 7,784,663 B2 | 8/2010 | Shelton, IV | 7,967,181 B2 | 6/2011 | Viola et al. |
| 7,789,889 B2 | 9/2010 | Zubik et al. | 7,967,791 B2 | 6/2011 | Franer et al. |
| 7,793,812 B2 | 9/2010 | Moore et al. | 7,980,443 B2 | 7/2011 | Scheib et al. |
| 7,794,475 B2 | 9/2010 | Hess et al. | 7,981,132 B2 | 7/2011 | Dubrul et al. |
| 7,798,386 B2 | 9/2010 | Schall et al. | 7,988,026 B2 | 8/2011 | Knodel et al. |
| 7,799,039 B2 | 9/2010 | Shelton, IV et al. | 7,988,027 B2 | 8/2011 | Olson et al. |
| 7,803,151 B2 | 9/2010 | Whitman | 7,992,757 B2 | 8/2011 | Wheeler et al. |
| 7,806,891 B2 | 10/2010 | Nowlin et al. | 7,997,469 B2 | 8/2011 | Olson et al. |
| 7,810,690 B2 | 10/2010 | Bilotti et al. | 8,002,696 B2 | 8/2011 | Suzuki |
| 7,810,691 B2 | 10/2010 | Boyden et al. | 8,002,795 B2 | 8/2011 | Beetel |
| 7,810,692 B2 | 10/2010 | Hall et al. | 8,006,885 B2 | 8/2011 | Marczyk |
| 7,810,693 B2 | 10/2010 | Broehl et al. | 8,006,889 B2 | 8/2011 | Adams et al. |
| 7,815,092 B2 | 10/2010 | Whitman et al. | 8,011,550 B2 | 9/2011 | Aranyi et al. |
| 7,819,296 B2 | 10/2010 | Hueil et al. | 8,011,551 B2 | 9/2011 | Marczyk et al. |
| 7,819,297 B2 | 10/2010 | Doll et al. | 8,011,553 B2 | 9/2011 | Mastri et al. |
| 7,819,298 B2 | 10/2010 | Hall et al. | 8,011,555 B2 | 9/2011 | Tarinelli et al. |
| 7,819,299 B2 | 10/2010 | Shelton, IV et al. | 8,016,176 B2 | 9/2011 | Kasvikis et al. |
| 7,823,592 B2 | 11/2010 | Bettuchi et al. | 8,016,177 B2 | 9/2011 | Bettuchi et al. |
| 7,824,426 B2 | 11/2010 | Racenet et al. | 8,016,178 B2 | 9/2011 | Olson et al. |
| 7,828,189 B2 | 11/2010 | Holsten et al. | 8,016,855 B2 | 9/2011 | Whitman et al. |
| 7,828,808 B2 | 11/2010 | Hinman et al. | 8,016,858 B2 | 9/2011 | Whitman |
| 7,832,408 B2 | 11/2010 | Shelton, IV et al. | 8,020,742 B2 | 9/2011 | Marczyk |
| 7,832,611 B2 | 11/2010 | Boyden et al. | 8,020,743 B2 | 9/2011 | Shelton, IV |
| 7,832,612 B2 | 11/2010 | Baxter, III et al. | 8,025,199 B2 | 9/2011 | Whitman et al. |
| 7,837,079 B2 | 11/2010 | Holsten et al. | 8,028,883 B2 | 10/2011 | Stopek |
| 7,837,080 B2 | 11/2010 | Schwemberger | 8,028,885 B2 | 10/2011 | Smith et al. |
| 7,837,081 B2 | 11/2010 | Holsten et al. | 8,034,077 B2 | 10/2011 | Smith et al. |
| 7,837,694 B2 | 11/2010 | Tethrake et al. | 8,038,045 B2 | 10/2011 | Bettuchi et al. |
| 7,842,028 B2 | 11/2010 | Lee | 8,038,046 B2 | 10/2011 | Smith et al. |
| 7,845,533 B2 | 12/2010 | Marczyk et al. | 8,043,328 B2 | 10/2011 | Hahnen et al. |
| 7,845,535 B2 | 12/2010 | Scircia | 8,056,787 B2 | 11/2011 | Boudreaux et al. |
| 7,845,536 B2 | 12/2010 | Viola et al. | 8,056,788 B2 | 11/2011 | Mastri et al. |
| 7,845,537 B2 | 12/2010 | Shelton, IV et al. | 8,066,167 B2 | 11/2011 | Measamer et al. |
| 7,846,149 B2 | 12/2010 | Jankowski | D650,074 S | 12/2011 | Hunt et al. |
| 7,857,183 B2 | 12/2010 | Shelton, IV | 8,075,476 B2 | 12/2011 | Vargas |
| 7,857,185 B2 | 12/2010 | Swayze et al. | 8,083,119 B2 | 12/2011 | Prommersberger |
| 7,857,186 B2 | 12/2010 | Baxter, III et al. | 8,083,120 B2 | 12/2011 | Shelton, IV et al. |
| 7,861,906 B2 | 1/2011 | Doll et al. | 8,091,756 B2 | 1/2012 | Viola |
| 7,862,502 B2 | 1/2011 | Pool et al. | 8,097,017 B2 | 1/2012 | Viola |
| 7,866,527 B2 | 1/2011 | Hall et al. | 8,100,310 B2 | 1/2012 | Zemlok |
| 7,871,418 B2 | 1/2011 | Thompson et al. | 8,105,350 B2 | 1/2012 | Lee et al. |
| 7,879,070 B2 | 2/2011 | Ortiz et al. | 8,109,426 B2 | 2/2012 | Milliman et al. |
| 7,883,461 B2 | 2/2011 | Albrecht et al. | 8,113,410 B2 | 2/2012 | Hall et al. |
| 7,891,531 B1 | 2/2011 | Ward | 8,114,100 B2 | 2/2012 | Smith et al. |
| 7,891,532 B2 | 2/2011 | Mastri et al. | 8,123,103 B2 | 2/2012 | Milliman |
| 7,900,805 B2 | 3/2011 | Shelton, IV et al. | 8,123,767 B2 | 2/2012 | Bauman et al. |
| 7,905,380 B2 | 3/2011 | Shelton, IV et al. | 8,128,645 B2 | 3/2012 | Sonnenschein et al. |
| 7,905,381 B2 | 3/2011 | Baxter, III et al. | 8,136,712 B2 | 3/2012 | Zingman |
| 7,909,220 B2 | 3/2011 | Viola | 8,141,762 B2 | 3/2012 | Bedi et al. |
| 7,909,221 B2 | 3/2011 | Viola et al. | 8,141,763 B2 | 3/2012 | Milliman |
| 7,913,891 B2 | 3/2011 | Doll et al. | 8,152,041 B2 | 4/2012 | Kostrzewski |
| 7,913,893 B2 | 3/2011 | Mastri et al. | 8,157,145 B2 | 4/2012 | Shelton, IV et al. |
| 7,914,543 B2 | 3/2011 | Roth et al. | 8,157,152 B2 | 4/2012 | Holsten et al. |
| 7,918,376 B1 | 4/2011 | Knodel et al. | 8,157,153 B2 | 4/2012 | Shelton, IV et al. |
| 7,918,377 B2 | 4/2011 | Measamer et al. | 8,161,977 B2 | 4/2012 | Shelton, IV et al. |
| 7,922,061 B2 | 4/2011 | Shelton, IV et al. | 8,162,197 B2 | 4/2012 | Mastri et al. |
| 7,922,063 B2 | 4/2011 | Zemlok et al. | 8,167,185 B2 | 5/2012 | Shelton, IV et al. |
| 7,922,743 B2 | 4/2011 | Heinrich et al. | 8,172,120 B2 | 5/2012 | Boyden et al. |
| 7,926,691 B2 | 4/2011 | Viola et al. | 8,172,122 B2 | 5/2012 | Kasvikis et al. |
| | | | 8,172,124 B2 | 5/2012 | Shelton, IV et al. |
| | | | 8,177,797 B2 | 5/2012 | Shimoji et al. |
| | | | 8,186,555 B2 | 5/2012 | Shelton, IV et al. |
| | | | 8,186,560 B2 | 5/2012 | Hess et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|---------|--------------------|-----------------|---------|----------------------|
| 8,191,752 B2 | 6/2012 | Scirica | 8,413,870 B2 | 4/2013 | Pastorelli et al. |
| 8,196,795 B2 | 6/2012 | Moore et al. | 8,413,871 B2 | 4/2013 | Racenet et al. |
| 8,196,796 B2 | 6/2012 | Shelton, IV et al. | 8,413,872 B2 | 4/2013 | Patel |
| 8,201,721 B2 | 6/2012 | Zemlok et al. | 8,414,577 B2 | 4/2013 | Boudreaux et al. |
| 8,205,781 B2 | 6/2012 | Baxter, III et al. | 8,424,740 B2 | 4/2013 | Shelton, IV et al. |
| 8,210,411 B2 | 7/2012 | Yates et al. | 8,424,741 B2 | 4/2013 | Mcguckin, Jr. et al. |
| 8,210,414 B2 | 7/2012 | Bettuchi et al. | 8,444,036 B2 | 5/2013 | Shelton, IV |
| 8,210,415 B2 | 7/2012 | Ward | 8,453,904 B2 | 6/2013 | Eskaros et al. |
| 8,211,125 B2 | 7/2012 | Spivey | 8,453,907 B2 | 6/2013 | Laurent et al. |
| 8,215,531 B2 | 7/2012 | Shelton, IV et al. | 8,453,908 B2 | 6/2013 | Bedi et al. |
| 8,215,533 B2 | 7/2012 | Viola et al. | 8,453,912 B2 | 6/2013 | Mastri et al. |
| 8,220,688 B2 | 7/2012 | Laurent et al. | 8,453,914 B2 | 6/2013 | Laurent et al. |
| 8,220,690 B2 | 7/2012 | Hess et al. | 8,459,520 B2 | 6/2013 | Giordano et al. |
| 8,225,799 B2 | 7/2012 | Bettuchi | 8,459,525 B2 | 6/2013 | Yates et al. |
| 8,226,553 B2 | 7/2012 | Shelton, IV et al. | 8,464,922 B2 | 6/2013 | Marczyk |
| 8,231,040 B2 | 7/2012 | Zemlok et al. | 8,464,923 B2 | 6/2013 | Shelton, IV |
| 8,231,041 B2 | 7/2012 | Marczyk et al. | 8,464,925 B2 | 6/2013 | Hull et al. |
| 8,231,042 B2 | 7/2012 | Hessler et al. | 8,465,515 B2 | 6/2013 | Drew et al. |
| 8,231,043 B2 | 7/2012 | Tarinelli et al. | 8,474,677 B2 | 7/2013 | Woodard, Jr. et al. |
| 8,236,010 B2 | 8/2012 | Ortiz et al. | 8,479,969 B2 | 7/2013 | Shelton, IV |
| 8,241,271 B2 | 8/2012 | Millman et al. | 8,485,412 B2 | 7/2013 | Shelton, IV et al. |
| 8,241,308 B2 | 8/2012 | Kortenbach et al. | 8,485,413 B2 | 7/2013 | Scheib et al. |
| 8,241,322 B2 | 8/2012 | Whitman et al. | 8,485,970 B2 | 7/2013 | Widenhouse et al. |
| 8,245,899 B2 | 8/2012 | Swensgard et al. | 8,490,853 B2 | 7/2013 | Criscuolo et al. |
| 8,245,901 B2 | 8/2012 | Stopek | 8,496,156 B2 | 7/2013 | Sniffin et al. |
| 8,256,654 B2 | 9/2012 | Bettuchi et al. | 8,499,993 B2 | 8/2013 | Shelton, IV et al. |
| 8,256,655 B2 | 9/2012 | Sniffin et al. | 8,517,239 B2 | 8/2013 | Scheib et al. |
| 8,257,251 B2 | 9/2012 | Shelton, IV et al. | 8,517,243 B2 | 8/2013 | Giordano et al. |
| 8,267,300 B2 | 9/2012 | Boudreaux | 8,517,244 B2 | 8/2013 | Shelton, IV et al. |
| 8,272,553 B2 | 9/2012 | Mastri et al. | 8,529,600 B2 | 9/2013 | Woodard, Jr. et al. |
| 8,276,801 B2 | 10/2012 | Zemlok et al. | 8,534,528 B2 | 9/2013 | Shelton, IV |
| 8,276,802 B2 | 10/2012 | Kostrzewski | 8,540,128 B2 | 9/2013 | Shelton, IV et al. |
| 8,281,973 B2 | 10/2012 | Wenchell et al. | 8,540,129 B2 | 9/2013 | Baxter, III et al. |
| 8,286,845 B2 | 10/2012 | Perry et al. | 8,540,130 B2 | 9/2013 | Moore et al. |
| 8,287,561 B2 | 10/2012 | Nunez et al. | 8,540,131 B2 | 9/2013 | Swayze |
| 8,292,151 B2 | 10/2012 | Viola | 8,540,133 B2 | 9/2013 | Bedi et al. |
| 8,292,155 B2 | 10/2012 | Shelton, IV et al. | 8,561,870 B2 | 10/2013 | Baxter, III et al. |
| 8,292,157 B2 | 10/2012 | Smith et al. | 8,567,656 B2 | 10/2013 | Shelton, IV et al. |
| 8,308,040 B2 | 11/2012 | Huang et al. | 8,573,461 B2 | 11/2013 | Shelton, IV et al. |
| 8,308,042 B2 | 11/2012 | Aranyi | 8,573,465 B2 | 11/2013 | Shelton, IV et al. |
| 8,308,046 B2 | 11/2012 | Prommersberger | 8,579,937 B2 | 11/2013 | Gresham |
| 8,317,070 B2 | 11/2012 | Hueil et al. | 8,584,919 B2 | 11/2013 | Hueil et al. |
| 8,317,074 B2 | 11/2012 | Ortiz et al. | 8,590,762 B2 | 11/2013 | Hess et al. |
| 8,322,455 B2 | 12/2012 | Shelton, IV et al. | 8,602,287 B2 | 12/2013 | Yates et al. |
| 8,322,589 B2 | 12/2012 | Boudreaux | 8,602,288 B2 | 12/2013 | Shelton, IV et al. |
| 8,328,062 B2 | 12/2012 | Viola | 8,608,044 B2 | 12/2013 | Hueil et al. |
| 8,328,063 B2 | 12/2012 | Milliman et al. | 8,608,045 B2 | 12/2013 | Smith et al. |
| 8,328,064 B2 | 12/2012 | Racenet et al. | 8,608,046 B2 | 12/2013 | Laurent et al. |
| 8,333,313 B2 | 12/2012 | Boudreaux et al. | 8,616,431 B2 | 12/2013 | Timm et al. |
| 8,348,123 B2 | 1/2013 | Scirica et al. | 8,622,274 B2 | 1/2014 | Yates et al. |
| 8,348,129 B2 | 1/2013 | Bedi et al. | 8,622,275 B2 | 1/2014 | Baxter, III et al. |
| 8,348,131 B2 | 1/2013 | Omaits et al. | 8,631,987 B2 | 1/2014 | Shelton, IV et al. |
| 8,348,837 B2 | 1/2013 | Wenchell | 8,632,525 B2 | 1/2014 | Kerr et al. |
| 8,348,972 B2 | 1/2013 | Soltz et al. | 8,632,535 B2 | 1/2014 | Shelton, IV et al. |
| 8,353,437 B2 | 1/2013 | Boudreaux | 8,632,563 B2 | 1/2014 | Nagase et al. |
| 8,353,438 B2 | 1/2013 | Baxter, III et al. | 8,636,187 B2 | 1/2014 | Hueil et al. |
| 8,353,439 B2 | 1/2013 | Baxter, III et al. | 8,636,736 B2 | 1/2014 | Yates et al. |
| 8,357,144 B2 | 1/2013 | Whitman et al. | 8,652,120 B2 | 2/2014 | Giordano et al. |
| 8,360,296 B2 | 1/2013 | Zingman | 8,657,174 B2 | 2/2014 | Yates et al. |
| 8,360,297 B2 | 1/2013 | Shelton, IV et al. | 8,657,176 B2 | 2/2014 | Shelton, IV et al. |
| 8,360,299 B2 | 1/2013 | Zemlok et al. | 8,657,178 B2 | 2/2014 | Hueil et al. |
| 8,365,973 B1 | 2/2013 | White et al. | 8,668,130 B2 | 3/2014 | Hess et al. |
| 8,365,976 B2 | 2/2013 | Hess et al. | 8,672,207 B2 | 3/2014 | Shelton, IV et al. |
| 8,371,491 B2 | 2/2013 | Huitema et al. | 8,672,208 B2 | 3/2014 | Hess et al. |
| 8,371,492 B2 | 2/2013 | Aranyi et al. | 8,684,253 B2 | 4/2014 | Giordano et al. |
| 8,371,493 B2 | 2/2013 | Aranyi et al. | 8,695,866 B2 | 4/2014 | Leimbach et al. |
| 8,372,094 B2 | 2/2013 | Bettuchi et al. | 8,701,958 B2 | 4/2014 | Shelton, IV et al. |
| 8,393,513 B2 | 3/2013 | Jankowski | 8,708,213 B2 | 4/2014 | Shelton, IV et al. |
| 8,393,514 B2 | 3/2013 | Shelton, IV et al. | 8,720,766 B2 | 5/2014 | Hess et al. |
| 8,397,971 B2 | 3/2013 | Yates et al. | 8,727,197 B2 | 5/2014 | Hess et al. |
| 8,398,669 B2 | 3/2013 | Kim | 8,727,961 B2 | 5/2014 | Ziv |
| 8,403,198 B2 | 3/2013 | Sorrentino et al. | 8,758,235 B2 | 6/2014 | Jaworek |
| 8,408,439 B2 | 4/2013 | Huang et al. | 2001/0025183 A1 | 9/2001 | Shahidi |
| 8,408,442 B2 | 4/2013 | Racenet et al. | 2002/0095175 A1 | 7/2002 | Brock et al. |
| 8,409,079 B2 | 4/2013 | Okamoto et al. | 2002/0103494 A1 | 8/2002 | Pacey |
| | | | 2002/0117534 A1 | 8/2002 | Green et al. |
| | | | 2003/0190584 A1 | 10/2003 | Heasley |
| | | | 2003/0220660 A1 | 11/2003 | Kortenbach et al. |
| | | | 2004/0006372 A1 | 1/2004 | Racenet et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | | | |
|--------------|-----|---------|-----------------------------|--------------|----|---------|-----------------------|
| 2004/0094597 | A1 | 5/2004 | Whitman et al. | 2007/0023477 | A1 | 2/2007 | Whitman et al. |
| 2004/0097987 | A1 | 5/2004 | Pugsley et al. | 2007/0027468 | A1 | 2/2007 | Wales et al. |
| 2004/0098040 | A1 | 5/2004 | Taniguchi et al. | 2007/0027469 | A1 | 2/2007 | Smith et al. |
| 2004/0108357 | A1 | 6/2004 | Milliman et al. | 2007/0034668 | A1 | 2/2007 | Holsten et al. |
| 2004/0111081 | A1 | 6/2004 | Whitman et al. | 2007/0043387 | A1 | 2/2007 | Vargas et al. |
| 2004/0147909 | A1 | 7/2004 | Johnston et al. | 2007/0055219 | A1 | 3/2007 | Whitman et al. |
| 2004/0158261 | A1 | 8/2004 | Vu | 2007/0066981 | A1 | 3/2007 | Meagher |
| 2004/0164123 | A1 | 8/2004 | Racenet et al. | 2007/0073341 | A1 | 3/2007 | Smith et al. |
| 2004/0167572 | A1 | 8/2004 | Roth et al. | 2007/0078484 | A1 | 4/2007 | Talarico et al. |
| 2004/0173659 | A1 | 9/2004 | Green et al. | 2007/0084897 | A1 | 4/2007 | Shelton, Jr. et al. |
| 2004/0193177 | A1 | 9/2004 | Houghton et al. | 2007/0093869 | A1 | 4/2007 | Bloom et al. |
| 2004/0193189 | A1 | 9/2004 | Kortenbach et al. | 2007/0102472 | A1 | 5/2007 | Shelton, IV |
| 2004/0222268 | A1 | 11/2004 | Bilotti et al. | 2007/0106317 | A1 | 5/2007 | Shelton, IV et al. |
| 2004/0232201 | A1 | 11/2004 | Wenchell et al. | 2007/0118175 | A1 | 5/2007 | Butler et al. |
| 2004/0243147 | A1 | 12/2004 | Lipow | 2007/0129605 | A1 | 6/2007 | Schaaf |
| 2004/0243176 | A1 | 12/2004 | Hahnen et al. | 2007/0135803 | A1 | 6/2007 | Belson |
| 2004/0254566 | A1 | 12/2004 | Plicchi et al. | 2007/0170225 | A1 | 7/2007 | Shelton, IV et al. |
| 2004/0254608 | A1 | 12/2004 | Huitema et al. | 2007/0173687 | A1 | 7/2007 | Shima et al. |
| 2004/0260315 | A1 | 12/2004 | Dell et al. | 2007/0175950 | A1 | 8/2007 | Shelton, IV et al. |
| 2004/0267310 | A1 | 12/2004 | Racenet et al. | 2007/0175951 | A1 | 8/2007 | Shelton, IV et al. |
| 2005/0033357 | A1 | 2/2005 | Braun | 2007/0175955 | A1 | 8/2007 | Shelton, IV et al. |
| 2005/0059997 | A1 | 3/2005 | Bauman et al. | 2007/0179528 | A1 | 8/2007 | Soltz et al. |
| 2005/0070929 | A1 | 3/2005 | Dalessandro et al. | 2007/0181632 | A1 | 8/2007 | Milliman |
| 2005/0085693 | A1 | 4/2005 | Belson et al. | 2007/0194079 | A1 | 8/2007 | Hueil et al. |
| 2005/0103819 | A1 | 5/2005 | Racenet et al. | 2007/0194082 | A1 | 8/2007 | Morgan et al. |
| 2005/0107824 | A1 | 5/2005 | Hillstead et al. | 2007/0203510 | A1 | 8/2007 | Bettuchi |
| 2005/0131390 | A1 | 6/2005 | Heinrich et al. | 2007/0219571 | A1 | 9/2007 | Balbierz et al. |
| 2005/0131457 | A1 | 6/2005 | Douglas et al. | 2007/0221700 | A1 | 9/2007 | Ortiz et al. |
| 2005/0145675 | A1 | 7/2005 | Hartwick et al. | 2007/0225562 | A1 | 9/2007 | Spivey et al. |
| 2005/0154406 | A1 | 7/2005 | Bombard et al. | 2007/0239028 | A1 | 10/2007 | Houser et al. |
| 2005/0177181 | A1 | 8/2005 | Kagan et al. | 2007/0244471 | A1 | 10/2007 | Malackowski |
| 2005/0182298 | A1 | 8/2005 | Ikeda et al. | 2007/0246505 | A1 | 10/2007 | Pace-Florida et al. |
| 2005/0187576 | A1* | 8/2005 | Whitman et al. 606/219 | 2007/0270784 | A1 | 11/2007 | Smith et al. |
| 2005/0189397 | A1 | 9/2005 | Jankowski | 2007/0276189 | A1 | 11/2007 | Abel et al. |
| 2005/0192628 | A1 | 9/2005 | Viola | 2007/0287993 | A1 | 12/2007 | Hinman et al. |
| 2005/0203550 | A1 | 9/2005 | Laufer et al. | 2007/0299427 | A1 | 12/2007 | Yeung et al. |
| 2005/0216055 | A1 | 9/2005 | Scirica et al. | 2008/0029570 | A1 | 2/2008 | Shelton et al. |
| 2005/0240222 | A1 | 10/2005 | Shipp | 2008/0029573 | A1 | 2/2008 | Shelton et al. |
| 2005/0256452 | A1 | 11/2005 | DeMarchi et al. | 2008/0029574 | A1 | 2/2008 | Shelton et al. |
| 2005/0263563 | A1 | 12/2005 | Racenet et al. | 2008/0029575 | A1 | 2/2008 | Shelton et al. |
| 2005/0274768 | A1 | 12/2005 | Cummins et al. | 2008/0035701 | A1 | 2/2008 | Racenet et al. |
| 2005/0283188 | A1 | 12/2005 | Loshakove et al. | 2008/0041917 | A1 | 2/2008 | Racenet et al. |
| 2006/0011699 | A1 | 1/2006 | Olson et al. | 2008/0078802 | A1 | 4/2008 | Hess et al. |
| 2006/0020258 | A1 | 1/2006 | Strauss et al. | 2008/0082114 | A1 | 4/2008 | McKenna et al. |
| 2006/0025811 | A1 | 2/2006 | Shelton, IV | 2008/0082125 | A1 | 4/2008 | Murray et al. |
| 2006/0025812 | A1 | 2/2006 | Shelton, IV | 2008/0083808 | A1 | 4/2008 | Scirica |
| 2006/0025813 | A1 | 2/2006 | Shelton et al. | 2008/0083813 | A1 | 4/2008 | Zemlok et al. |
| 2006/0041188 | A1 | 2/2006 | Dirusso et al. | 2008/0140115 | A1 | 6/2008 | Stopek |
| 2006/0047303 | A1 | 3/2006 | Ortiz et al. | 2008/0154299 | A1 | 6/2008 | Livneh |
| 2006/0047307 | A1 | 3/2006 | Ortiz et al. | 2008/0169328 | A1 | 7/2008 | Shelton |
| 2006/0049229 | A1 | 3/2006 | Milliman et al. | 2008/0169331 | A1 | 7/2008 | Shelton et al. |
| 2006/0052825 | A1 | 3/2006 | Ransick et al. | 2008/0169332 | A1 | 7/2008 | Shelton et al. |
| 2006/0085033 | A1 | 4/2006 | Crisuolo et al. | 2008/0169333 | A1 | 7/2008 | Shelton et al. |
| 2006/0108393 | A1 | 5/2006 | Heinrich et al. | 2008/0169333 | A1 | 7/2008 | Shelton et al. |
| 2006/0122636 | A1 | 6/2006 | Bailly et al. | 2008/0172088 | A1 | 7/2008 | Smith et al. |
| 2006/0161050 | A1 | 7/2006 | Butler et al. | 2008/0183193 | A1 | 7/2008 | Omori et al. |
| 2006/0161185 | A1 | 7/2006 | Saadat et al. | 2008/0185419 | A1 | 8/2008 | Smith et al. |
| 2006/0173470 | A1 | 8/2006 | Oray et al. | 2008/0197167 | A1 | 8/2008 | Viola et al. |
| 2006/0180634 | A1 | 8/2006 | Shelton, IV et al. | 2008/0200933 | A1 | 8/2008 | Bakos et al. |
| 2006/0185682 | A1 | 8/2006 | Marczyk | 2008/0242939 | A1 | 10/2008 | Johnston |
| 2006/0201989 | A1 | 9/2006 | Ojeda | 2008/0251568 | A1 | 10/2008 | Zemlok et al. |
| 2006/0212069 | A1 | 9/2006 | Shelton, IV | 2008/0251569 | A1 | 10/2008 | Smith et al. |
| 2006/0226196 | A1 | 10/2006 | Hueil et al. | 2008/0255413 | A1 | 10/2008 | Zemlok et al. |
| 2006/0235368 | A1 | 10/2006 | Oz | 2008/0255519 | A1 | 10/2008 | Piskun et al. |
| 2006/0235469 | A1 | 10/2006 | Viola | 2008/0283570 | A1 | 11/2008 | Boyden et al. |
| 2006/0241655 | A1 | 10/2006 | Viola | 2008/0290134 | A1 | 11/2008 | Bettuchi et al. |
| 2006/0241692 | A1 | 10/2006 | McGuckin, Jr. et al. | 2008/0294179 | A1 | 11/2008 | Balbierz et al. |
| 2006/0252993 | A1 | 11/2006 | Freed et al. | 2008/0296346 | A1 | 12/2008 | Shelton, IV et al. |
| 2006/0258904 | A1 | 11/2006 | Stefanchik et al. | 2008/0308602 | A1 | 12/2008 | Timm et al. |
| 2006/0259073 | A1 | 11/2006 | Miyamoto et al. | 2008/0308603 | A1 | 12/2008 | Shelton, IV et al. |
| 2006/0271102 | A1 | 11/2006 | Bosshard et al. | 2008/0308608 | A1 | 12/2008 | Prommersberger |
| 2006/0278680 | A1 | 12/2006 | Viola et al. | 2008/0314960 | A1 | 12/2008 | Marczyk et al. |
| 2006/0278681 | A1 | 12/2006 | Viola et al. | 2009/0001121 | A1 | 1/2009 | Hess et al. |
| 2006/0289602 | A1 | 12/2006 | Wales et al. | 2009/0001122 | A1 | 1/2009 | Prommersberger et al. |
| 2007/0023476 | A1 | 2/2007 | Whitman et al. | 2009/0001130 | A1 | 1/2009 | Hess et al. |
| | | | | 2009/0005807 | A1 | 1/2009 | Hess et al. |
| | | | | 2009/0005809 | A1 | 1/2009 | Hess et al. |
| | | | | 2009/0012534 | A1 | 1/2009 | Madhani et al. |
| | | | | 2009/0012556 | A1 | 1/2009 | Boudreaux et al. |
| | | | | 2009/0048612 | A1 | 2/2009 | Farritor et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|-----------------|---------|--------------------------|-----------------|---------|------------------------|
| 2009/0054908 A1 | 2/2009 | Zand et al. | 2011/0114700 A1 | 5/2011 | Baxter, III et al. |
| 2009/0078736 A1 | 3/2009 | Van Lue | 2011/0118754 A1 | 5/2011 | Dachs, II et al. |
| 2009/0088774 A1 | 4/2009 | Swarup et al. | 2011/0118778 A1 | 5/2011 | Burbank |
| 2009/0108048 A1 | 4/2009 | Zemlok et al. | 2011/0125176 A1 | 5/2011 | Yates et al. |
| 2009/0112229 A1 | 4/2009 | Omori et al. | 2011/0125177 A1 | 5/2011 | Yates et al. |
| 2009/0114701 A1 | 5/2009 | Zemlok et al. | 2011/0132964 A1 | 6/2011 | Weisenburgh, II et al. |
| 2009/0149871 A9 | 6/2009 | Kagan et al. | 2011/0144430 A1 | 6/2011 | Spivey et al. |
| 2009/0157087 A1 | 6/2009 | Wei et al. | 2011/0147433 A1 | 6/2011 | Shelton, IV et al. |
| 2009/0198272 A1 | 8/2009 | Kerver et al. | 2011/0155781 A1 | 6/2011 | Swensgard et al. |
| 2009/0204108 A1 | 8/2009 | Steffen | 2011/0155784 A1 | 6/2011 | Shelton, IV et al. |
| 2009/0206125 A1 | 8/2009 | Huitema et al. | 2011/0155786 A1 | 6/2011 | Shelton, IV |
| 2009/0206126 A1 | 8/2009 | Huitema et al. | 2011/0155787 A1 | 6/2011 | Baxter, III et al. |
| 2009/0206131 A1 | 8/2009 | Weisenburgh, II et al. | 2011/0163146 A1 | 7/2011 | Ortiz et al. |
| 2009/0206133 A1 | 8/2009 | Morgan et al. | 2011/0172495 A1 | 7/2011 | Armstrong |
| 2009/0206137 A1 | 8/2009 | Hall et al. | 2011/0174861 A1 | 7/2011 | Shelton, IV et al. |
| 2009/0206139 A1 | 8/2009 | Hall et al. | 2011/0174862 A1 | 7/2011 | Shelton, IV et al. |
| 2009/0206141 A1 | 8/2009 | Huitema et al. | 2011/0192882 A1 | 8/2011 | Hess et al. |
| 2009/0206142 A1 | 8/2009 | Huitema et al. | 2011/0210156 A1 | 9/2011 | Smith et al. |
| 2009/0209946 A1 | 8/2009 | Swayze et al. | 2011/0253765 A1 | 10/2011 | Nicholas et al. |
| 2009/0218384 A1 | 9/2009 | Aranyi | 2011/0275901 A1 | 11/2011 | Shelton, IV |
| 2009/0242610 A1 | 10/2009 | Shelton, IV et al. | 2011/0276083 A1 | 11/2011 | Shelton, IV et al. |
| 2009/0255974 A1 | 10/2009 | Viola | 2011/0278343 A1 | 11/2011 | Knodel et al. |
| 2009/0255975 A1 | 10/2009 | Zemlok et al. | 2011/0288573 A1 | 11/2011 | Yates et al. |
| 2009/0255976 A1 | 10/2009 | Marczyk et al. | 2011/0290851 A1 | 12/2011 | Shelton, IV |
| 2009/0255977 A1 | 10/2009 | Zemlok | 2011/0290853 A1 | 12/2011 | Shelton, IV et al. |
| 2009/0255978 A1 | 10/2009 | Viola et al. | 2011/0290854 A1 | 12/2011 | Timm et al. |
| 2009/0277949 A1 | 11/2009 | Viola et al. | 2011/0290855 A1 | 12/2011 | Moore et al. |
| 2009/0292176 A1 | 11/2009 | Bonadio et al. | 2011/0290856 A1 | 12/2011 | Shelton, IV et al. |
| 2010/0012704 A1 | 1/2010 | Tarinelli Racenet et al. | 2011/0295242 A1 | 12/2011 | Spivey et al. |
| 2010/0069942 A1 | 3/2010 | Shelton, IV | 2011/0295269 A1 | 12/2011 | Swensgard et al. |
| 2010/0072254 A1 | 3/2010 | Aranyi et al. | 2011/0295295 A1 | 12/2011 | Shelton, IV et al. |
| 2010/0076475 A1 | 3/2010 | Yates et al. | 2012/0024935 A1 | 2/2012 | Shelton, IV et al. |
| 2010/0087840 A1 | 4/2010 | Ebersole et al. | 2012/0024936 A1 | 2/2012 | Baxter, III et al. |
| 2010/0108740 A1 | 5/2010 | Pastorelli et al. | 2012/0029272 A1 | 2/2012 | Shelton, IV et al. |
| 2010/0108741 A1 | 5/2010 | Hessler et al. | 2012/0029544 A1 | 2/2012 | Shelton, IV et al. |
| 2010/0133317 A1 | 6/2010 | Shelton, IV et al. | 2012/0029547 A1 | 2/2012 | Shelton, IV et al. |
| 2010/0147921 A1 | 6/2010 | Olson | 2012/0046692 A1 | 2/2012 | Smith et al. |
| 2010/0147922 A1 | 6/2010 | Olson | 2012/0071711 A1 | 3/2012 | Shelton, IV et al. |
| 2010/0163598 A1 | 7/2010 | Belzer | 2012/0074196 A1 | 3/2012 | Shelton, IV et al. |
| 2010/0179382 A1 | 7/2010 | Shelton, IV et al. | 2012/0074198 A1 | 3/2012 | Huitema et al. |
| 2010/0193566 A1 | 8/2010 | Scheib et al. | 2012/0074200 A1 | 3/2012 | Schmid et al. |
| 2010/0200637 A1 | 8/2010 | Beetel | 2012/0074201 A1 | 3/2012 | Baxter, III et al. |
| 2010/0222901 A1 | 9/2010 | Swayze et al. | 2012/0080332 A1 | 4/2012 | Shelton, IV et al. |
| 2010/0228091 A1 | 9/2010 | Widenhouse et al. | 2012/0080335 A1 | 4/2012 | Shelton, IV et al. |
| 2010/0230465 A1 | 9/2010 | Smith et al. | 2012/0080336 A1 | 4/2012 | Shelton, IV et al. |
| 2010/0243707 A1 | 9/2010 | Olson et al. | 2012/0080337 A1 | 4/2012 | Shelton, IV et al. |
| 2010/0243708 A1 | 9/2010 | Aranyi et al. | 2012/0080338 A1 | 4/2012 | Shelton, IV et al. |
| 2010/0249519 A1 | 9/2010 | Park et al. | 2012/0080340 A1 | 4/2012 | Shelton, IV et al. |
| 2010/0258611 A1 | 10/2010 | Smith et al. | 2012/0080344 A1 | 4/2012 | Shelton, IV |
| 2010/0276471 A1 | 11/2010 | Whitman | 2012/0080345 A1 | 4/2012 | Morgan et al. |
| 2010/0292540 A1 | 11/2010 | Hess et al. | 2012/0080475 A1 | 4/2012 | Smith et al. |
| 2010/0294827 A1 | 11/2010 | Boyden et al. | 2012/0080478 A1 | 4/2012 | Morgan et al. |
| 2010/0294829 A1 | 11/2010 | Giordano et al. | 2012/0080479 A1 | 4/2012 | Shelton, IV |
| 2010/0305552 A1 | 12/2010 | Shelton, IV et al. | 2012/0080480 A1 | 4/2012 | Woodard, Jr. et al. |
| 2010/0312261 A1 | 12/2010 | Suzuki et al. | 2012/0080481 A1 | 4/2012 | Widenhouse et al. |
| 2010/0320252 A1 | 12/2010 | Viola et al. | 2012/0080482 A1 | 4/2012 | Schall et al. |
| 2010/0331880 A1 | 12/2010 | Stopek | 2012/0080483 A1 | 4/2012 | Riesterberg et al. |
| 2011/0006099 A1 | 1/2011 | Hall et al. | 2012/0080484 A1 | 4/2012 | Morgan et al. |
| 2011/0006101 A1 | 1/2011 | Hall et al. | 2012/0080485 A1 | 4/2012 | Woodard, Jr. et al. |
| 2011/0011916 A1 | 1/2011 | Levine | 2012/0080486 A1 | 4/2012 | Woodard, Jr. et al. |
| 2011/0017801 A1 | 1/2011 | Zemlok et al. | 2012/0080488 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0022032 A1 | 1/2011 | Zemlok et al. | 2012/0080489 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0024477 A1 | 2/2011 | Hall | 2012/0080490 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0024478 A1 | 2/2011 | Shelton, IV | 2012/0080491 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0024479 A1 | 2/2011 | Swensgard et al. | 2012/0080493 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0036887 A1 | 2/2011 | Zemlok et al. | 2012/0080496 A1 | 4/2012 | Schall et al. |
| 2011/0036891 A1 | 2/2011 | Zemlok et al. | 2012/0080498 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0060363 A1 | 3/2011 | Hess et al. | 2012/0080499 A1 | 4/2012 | Schall et al. |
| 2011/0068148 A1 | 3/2011 | Hall et al. | 2012/0080500 A1 | 4/2012 | Morgan et al. |
| 2011/0084112 A1 | 4/2011 | Kostrzewski | 2012/0080501 A1 | 4/2012 | Morgan et al. |
| 2011/0087276 A1 | 4/2011 | Bedi et al. | 2012/0080502 A1 | 4/2012 | Morgan et al. |
| 2011/0087279 A1 | 4/2011 | Shah et al. | 2012/0080503 A1 | 4/2012 | Woodard, Jr. et al. |
| 2011/0095068 A1 | 4/2011 | Patel | 2012/0083833 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0101065 A1 | 5/2011 | Milliman | 2012/0083834 A1 | 4/2012 | Shelton, IV et al. |
| 2011/0114697 A1 | 5/2011 | Baxter, III et al. | 2012/0083835 A1 | 4/2012 | Shelton, IV et al. |
| | | | 2012/0083836 A1 | 4/2012 | Shelton, IV et al. |
| | | | 2012/0138658 A1 | 6/2012 | Ullrich et al. |
| | | | 2012/0138660 A1 | 6/2012 | Shelton, IV |
| | | | 2012/0150192 A1 | 6/2012 | Dachs, II et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|-----------------|---------|--------------------------------|-----------------|---------|---------------------------------------|
| 2012/0160721 A1 | 6/2012 | Shelton, IV et al. | 2013/0126581 A1 | 5/2013 | Yates et al. |
| 2012/0175398 A1 | 7/2012 | Sandborn et al. | 2013/0126582 A1 | 5/2013 | Shelton, IV et al. |
| 2012/0175399 A1 | 7/2012 | Shelton et al. | 2013/0146641 A1 | 6/2013 | Shelton, IV et al. |
| 2012/0187179 A1 | 7/2012 | Gleiman | 2013/0146642 A1 | 6/2013 | Shelton, IV et al. |
| 2012/0199630 A1 | 8/2012 | Shelton, IV | 2013/0146643 A1 | 6/2013 | Schmid et al. |
| 2012/0199632 A1 | 8/2012 | Spivey et al. | 2013/0150832 A1 | 6/2013 | Belson et al. |
| 2012/0203247 A1 | 8/2012 | Shelton, IV et al. | 2013/0153634 A1 | 6/2013 | Carter et al. |
| 2012/0223123 A1 | 9/2012 | Baxter, III et al. | 2013/0153636 A1 | 6/2013 | Shelton, IV et al. |
| 2012/0234890 A1 | 9/2012 | Aronhalt et al. | 2013/0153641 A1 | 6/2013 | Shelton, IV et al. |
| 2012/0234891 A1 | 9/2012 | Aronhalt et al. | 2013/0161375 A1 | 6/2013 | Huitema et al. |
| 2012/0234892 A1 | 9/2012 | Aronhalt et al. | 2013/0168435 A1 | 7/2013 | Huang et al. |
| 2012/0234893 A1 | 9/2012 | Schuckmann et al. | 2013/0172929 A1 | 7/2013 | Hess et al. |
| 2012/0234895 A1 | 9/2012 | O'Connor et al. | 2013/0175317 A1 | 7/2013 | Yates et al. |
| 2012/0234896 A1 | 9/2012 | Ellerhorst et al. | 2013/0175321 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0234897 A1 | 9/2012 | Shelton, IV et al. | 2013/0175322 A1 | 7/2013 | Yates et al. |
| 2012/0234898 A1 | 9/2012 | Shelton, IV et al. | 2013/0181030 A1 | 7/2013 | Hess et al. |
| 2012/0234899 A1 | 9/2012 | Scheib et al. | 2013/0181033 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0238823 A1 | 9/2012 | Hagerty et al. | 2013/0181034 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0238824 A1 | 9/2012 | Widenhouse et al. | 2013/0184718 A1 | 7/2013 | Smith et al. |
| 2012/0238826 A1 | 9/2012 | Yoo et al. | 2013/0184719 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0238829 A1 | 9/2012 | Shelton, IV et al. | 2013/0186932 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0239009 A1 | 9/2012 | Mollere et al. | 2013/0186933 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0239075 A1 | 9/2012 | Widenhouse et al. | 2013/0186934 A1 | 7/2013 | Shelton, IV et al. |
| 2012/0239082 A1 | 9/2012 | Shelton, IV et al. | 2013/0186936 A1 | 7/2013 | Shelton, IV |
| 2012/0241491 A1 | 9/2012 | Aldridge et al. | 2013/0190733 A1 | 7/2013 | Giordano et al. |
| 2012/0241492 A1 | 9/2012 | Shelton, IV et al. | 2013/0190757 A1 | 7/2013 | Yates et al. |
| 2012/0241493 A1 | 9/2012 | Baxter, III et al. | 2013/0193188 A1 | 8/2013 | Shelton, IV et al. |
| 2012/0241496 A1 | 9/2012 | Mandakolathur Vasudevan et al. | 2013/0193189 A1 | 8/2013 | Swensgard et al. |
| 2012/0241497 A1 | 9/2012 | Mandakolathur Vasudevan et al. | 2013/0197556 A1 | 8/2013 | Shelton, IV et al. |
| 2012/0241498 A1 | 9/2012 | Gonzalez et al. | 2013/0200132 A1 | 8/2013 | Moore et al. |
| 2012/0241499 A1 | 9/2012 | Baxter, III et al. | 2013/0206814 A1 | 8/2013 | Morgan et al. |
| 2012/0241500 A1 | 9/2012 | Timmer et al. | 2013/0214030 A1 | 8/2013 | Aronhalt et al. |
| 2012/0241501 A1 | 9/2012 | Swayze et al. | 2013/0221063 A1 | 8/2013 | Aronhalt et al. |
| 2012/0241502 A1 | 9/2012 | Aldridge et al. | 2013/0221064 A1 | 8/2013 | Aronhalt et al. |
| 2012/0241503 A1 | 9/2012 | Baxter, III et al. | 2013/0221065 A1 | 8/2013 | Aronhalt et al. |
| 2012/0241505 A1 | 9/2012 | Alexander, III et al. | 2013/0233906 A1 | 9/2013 | Hess et al. |
| 2012/0248169 A1 | 10/2012 | Widenhouse et al. | 2013/0248576 A1 | 9/2013 | Laurent et al. |
| 2012/0253298 A1 | 10/2012 | Henderson et al. | 2013/0248577 A1 | 9/2013 | Leimbach et al. |
| 2012/0273550 A1 | 11/2012 | Scirica | 2013/0256365 A1 | 10/2013 | Shelton, IV et al. |
| 2012/0283707 A1 | 11/2012 | Giordano et al. | 2013/0256366 A1 | 10/2013 | Shelton, IV et al. |
| 2012/0283748 A1 | 11/2012 | Ortiz et al. | 2013/0256367 A1 | 10/2013 | Scheib et al. |
| 2012/0289979 A1 | 11/2012 | Eskaros et al. | 2013/0256368 A1 | 10/2013 | Timm et al. |
| 2012/0292367 A1 | 11/2012 | Morgan et al. | 2013/0256369 A1 | 10/2013 | Schmid et al. |
| 2012/0298719 A1 | 11/2012 | Shelton, IV et al. | 2013/0256371 A1 | 10/2013 | Shelton, IV et al. |
| 2012/0298722 A1 | 11/2012 | Hess et al. | 2013/0256372 A1 | 10/2013 | Baxter, III et al. |
| 2012/0312860 A1 | 12/2012 | Ming et al. | 2013/0256373 A1 | 10/2013 | Schmid et al. |
| 2012/0318842 A1 | 12/2012 | Anim et al. | 2013/0256374 A1 | 10/2013 | Shelton, IV et al. |
| 2012/0318843 A1 | 12/2012 | Henderson et al. | 2013/0256375 A1 | 10/2013 | Shelton, IV et al. |
| 2012/0318844 A1 | 12/2012 | Shelton, IV et al. | 2013/0256376 A1 | 10/2013 | Barton et al. |
| 2012/0325892 A1 | 12/2012 | Kostrzewski | 2013/0256377 A1 | 10/2013 | Schmid et al. |
| 2013/0012931 A1 | 1/2013 | Spivey et al. | 2013/0256378 A1 | 10/2013 | Schmid et al. |
| 2013/0012957 A1 | 1/2013 | Shelton, IV et al. | 2013/0256379 A1 | 10/2013 | Schmid et al. |
| 2013/0018228 A1 | 1/2013 | Armstrong | 2013/0256380 A1 | 10/2013 | Schmid et al. |
| 2013/0018361 A1 | 1/2013 | Bryant | 2013/0256382 A1 | 10/2013 | Swayze et al. |
| 2013/0020375 A1 | 1/2013 | Shelton, IV et al. | 2013/0256383 A1 | 10/2013 | Aronhalt et al. |
| 2013/0020376 A1 | 1/2013 | Shelton, IV et al. | 2013/0261648 A1 | 10/2013 | Laurent et al. |
| 2013/0023861 A1 | 1/2013 | Shelton, IV et al. | 2013/0270322 A1 | 10/2013 | Scheib et al. |
| 2013/0026208 A1 | 1/2013 | Shelton, IV et al. | 2013/0277412 A1 | 10/2013 | Gresham et al. |
| 2013/0026210 A1 | 1/2013 | Shelton, IV et al. | 2013/0310873 A1 | 11/2013 | Stopek (nee Prommersberger) et al. |
| 2013/0037596 A1 | 2/2013 | Bear et al. | 2013/0313303 A1 | 11/2013 | Shelton, IV et al. |
| 2013/0048697 A1 | 2/2013 | Shelton, IV et al. | 2013/0313304 A1 | 11/2013 | Shelton, IV et al. |
| 2013/0056518 A1 | 3/2013 | Swensgard | 2013/0313306 A1 | 11/2013 | Shelton, IV et al. |
| 2013/0056520 A1 | 3/2013 | Swensgard | 2013/0317310 A1 | 11/2013 | Widenhouse et al. |
| 2013/0056521 A1 | 3/2013 | Swensgard | 2013/0327809 A1 | 12/2013 | Shelton, IV et al. |
| 2013/0056522 A1 | 3/2013 | Swensgard | 2013/0327810 A1 | 12/2013 | Swayze et al. |
| 2013/0062391 A1 | 3/2013 | Boudreaux et al. | 2013/0334278 A1 | 12/2013 | Kerr et al. |
| 2013/0075443 A1 | 3/2013 | Giordano et al. | 2013/0334283 A1 | 12/2013 | Swayze et al. |
| 2013/0075448 A1 | 3/2013 | Schmid et al. | 2013/0334284 A1 | 12/2013 | Swayze et al. |
| 2013/0075449 A1 | 3/2013 | Schmid et al. | 2013/0334285 A1 | 12/2013 | Swayze et al. |
| 2013/0075450 A1 | 3/2013 | Schmid et al. | 2013/0334286 A1 | 12/2013 | Swayze et al. |
| 2013/0079814 A1 | 3/2013 | Hess et al. | 2013/0334287 A1 | 12/2013 | Shelton, IV |
| 2013/0087597 A1 | 4/2013 | Shelton, IV et al. | 2013/0334288 A1 | 12/2013 | Shelton, IV |
| 2013/0105551 A1 | 5/2013 | Zingman | 2013/0341374 A1 | 12/2013 | Shelton, IV et al. |
| 2013/0116668 A1 | 5/2013 | Shelton, IV et al. | 2014/0000411 A1 | 1/2014 | Shelton, IV et al. |
| 2013/0116669 A1 | 5/2013 | Shelton, IV et al. | 2014/0001231 A1 | 1/2014 | Shelton, IV et al. |
| | | | 2014/0001234 A1 | 1/2014 | Shelton, IV et al. |
| | | | 2014/0001235 A1 | 1/2014 | Shelton, IV |
| | | | 2014/0001236 A1 | 1/2014 | Shelton, IV et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

2014/0001237 A1 1/2014 Shelton, IV et al.
 2014/0001238 A1 1/2014 Shelton, IV et al.
 2014/0001239 A1 1/2014 Shelton, IV et al.
 2014/0001240 A1 1/2014 Shelton, IV et al.
 2014/0005640 A1 1/2014 Shelton, IV et al.
 2014/0005653 A1 1/2014 Shelton, IV et al.
 2014/0005661 A1 1/2014 Shelton, IV et al.
 2014/0005662 A1 1/2014 Shelton, IV
 2014/0005676 A1 1/2014 Shelton, IV et al.
 2014/0005677 A1 1/2014 Shelton, IV et al.
 2014/0005678 A1 1/2014 Shelton, IV et al.
 2014/0005679 A1 1/2014 Shelton, IV et al.
 2014/0005680 A1 1/2014 Shelton, IV et al.
 2014/0005693 A1 1/2014 Shelton, IV et al.
 2014/0005694 A1 1/2014 Shelton, IV et al.
 2014/0005695 A1 1/2014 Shelton, IV
 2014/0005708 A1 1/2014 Shelton, IV
 2014/0005718 A1 1/2014 Shelton, IV et al.
 2014/0008414 A1 1/2014 Shelton, IV et al.
 2014/0014705 A1 1/2014 Baxter, III
 2014/0042205 A1 2/2014 Baxter, III et al.
 2014/0048582 A1 2/2014 Shelton, IV et al.
 2014/0061279 A1 3/2014 Laurent et al.
 2014/0097227 A1 4/2014 Aronhalt et al.
 2014/0128850 A1 5/2014 Kerr et al.

FOREIGN PATENT DOCUMENTS

CA 2458946 A1 3/2003
 CA 2512960 A1 1/2006
 CA 2514274 A1 1/2006
 CA 2639177 A1 2/2009
 CN 2488482 Y 5/2002
 CN 1523725 A 8/2004
 CN 1634601 A 7/2005
 CN 1868411 A 11/2006
 CN 1915180 A 2/2007
 CN 101011286 A 8/2007
 CN 101095621 A 1/2008
 CN 101023879 B 3/2013
 DE 273689 C 5/1914
 DE 1775926 A 1/1972
 DE 3036217 A1 4/1982
 DE 3212828 A1 11/1982
 DE 3210466 A1 9/1983
 DE 3709067 A1 9/1988
 DE 9412228 U 9/1994
 DE 19509116 A1 9/1996
 DE 19851291 A1 1/2000
 DE 19924311 A1 11/2000
 DE 69328576 T2 1/2001
 DE 20016423 U1 2/2001
 DE 10052679 A1 5/2001
 DE 20112837 U1 10/2001
 DE 20121753 U1 4/2003
 DE 10314072 A1 10/2004
 DE 202007003114 U1 6/2007
 EP 0000756 A1 2/1979
 EP 0122046 A1 10/1984
 EP 0070230 B1 10/1985
 EP 0156774 A2 10/1985
 EP 0387980 B1 10/1985
 EP 0033548 B1 5/1986
 EP 0077262 B1 8/1986
 EP 0129442 B1 11/1987
 EP 0276104 A2 7/1988
 EP 0178940 B1 1/1991
 EP 0178941 B1 1/1991
 EP 0169044 B1 6/1991
 EP 0248844 B1 1/1993
 EP 0545029 A1 6/1993
 EP 0277959 B1 10/1993
 EP 0233940 B1 11/1993
 EP 0261230 B1 11/1993

EP 0639349 A2 2/1994
 EP 0324636 B1 3/1994
 EP 0593920 A1 4/1994
 EP 0594148 A1 4/1994
 EP 0427949 B1 6/1994
 EP 0523174 B1 6/1994
 EP 0600182 A2 6/1994
 EP 0310431 B1 11/1994
 EP 0375302 B1 11/1994
 EP 0376562 B1 11/1994
 EP 0630612 A1 12/1994
 EP 0634144 A1 1/1995
 EP 0646356 A2 4/1995
 EP 0646357 A1 4/1995
 EP 0505036 B1 5/1995
 EP 0653189 A2 5/1995
 EP 0669104 A1 8/1995
 EP 0511470 B1 10/1995
 EP 0674876 A2 10/1995
 EP 0679367 A2 11/1995
 EP 0392547 B1 12/1995
 EP 0685204 A1 12/1995
 EP 0364216 B1 1/1996
 EP 0699418 A1 3/1996
 EP 0702937 A1 3/1996
 EP 0705571 A1 4/1996
 EP 0711611 A2 5/1996
 EP 0484677 B2 6/1996
 EP 0541987 B1 7/1996
 EP 0667119 B1 7/1996
 EP 0748614 A1 12/1996
 EP 0708618 B1 3/1997
 EP 0770355 A1 5/1997
 EP 0503662 B1 6/1997
 EP 0447121 B1 7/1997
 EP 0621009 B1 7/1997
 EP 0625077 B1 7/1997
 EP 0633749 B1 8/1997
 EP 0710090 B1 8/1997
 EP 0578425 B1 9/1997
 EP 0625335 B1 11/1997
 EP 0552423 B1 1/1998
 EP 0592244 B1 1/1998
 EP 0648476 B1 1/1998
 EP 0649290 B1 3/1998
 EP 0598618 B1 9/1998
 EP 0676173 B1 9/1998
 EP 0678007 B1 9/1998
 EP 0603472 B1 11/1998
 EP 0605351 B1 11/1998
 EP 0878169 A1 11/1998
 EP 0879742 A1 11/1998
 EP 0695144 B1 12/1998
 EP 0722296 B1 12/1998
 EP 0760230 B1 2/1999
 EP 0623316 B1 3/1999
 EP 0650701 B1 3/1999
 EP 0537572 B1 6/1999
 EP 0923907 A1 6/1999
 EP 0640317 A1 9/1999
 EP 0843906 B1 3/2000
 EP 0552050 B1 5/2000
 EP 0833592 B1 5/2000
 EP 0832605 B1 6/2000
 EP 0830094 B1 9/2000
 EP 1034747 A1 9/2000
 EP 1034748 A1 9/2000
 EP 0694290 B1 11/2000
 EP 1050278 A1 11/2000
 EP 1053719 A1 11/2000
 EP 1053720 A1 11/2000
 EP 1055399 A1 11/2000
 EP 1055400 A1 11/2000
 EP 1080694 A1 3/2001
 EP 1090592 A1 4/2001
 EP 1095627 A1 5/2001
 EP 1256318 B1 5/2001
 EP 0806914 B1 9/2001
 EP 0768840 B1 12/2001

(56)

References Cited

FOREIGN PATENT DOCUMENTS

| | | | | | | | |
|----|---------|----|---------|----|---------|----|---------|
| EP | 0908152 | B1 | 1/2002 | EP | 1032318 | B1 | 8/2006 |
| EP | 0872213 | B1 | 5/2002 | EP | 1045672 | B1 | 8/2006 |
| EP | 0862386 | B1 | 6/2002 | EP | 1617768 | B1 | 8/2006 |
| EP | 0949886 | B1 | 9/2002 | EP | 1693015 | A2 | 8/2006 |
| EP | 1238634 | A2 | 9/2002 | EP | 1400214 | B1 | 9/2006 |
| EP | 0858295 | B1 | 12/2002 | EP | 1702567 | A2 | 9/2006 |
| EP | 0656188 | B1 | 1/2003 | EP | 1129665 | B1 | 11/2006 |
| EP | 0717960 | B1 | 2/2003 | EP | 1400206 | B1 | 11/2006 |
| EP | 1284120 | A1 | 2/2003 | EP | 1721568 | A1 | 11/2006 |
| EP | 1287788 | A1 | 3/2003 | EP | 1256317 | B1 | 12/2006 |
| EP | 0717966 | B1 | 4/2003 | EP | 1285633 | B1 | 12/2006 |
| EP | 0869742 | B1 | 5/2003 | EP | 1728473 | A1 | 12/2006 |
| EP | 0829235 | B1 | 6/2003 | EP | 1728475 | A2 | 12/2006 |
| EP | 0887046 | B1 | 7/2003 | EP | 1736105 | A1 | 12/2006 |
| EP | 0852480 | B1 | 8/2003 | EP | 1011494 | B1 | 1/2007 |
| EP | 0891154 | B1 | 9/2003 | EP | 1479346 | B1 | 1/2007 |
| EP | 0813843 | B1 | 10/2003 | EP | 1484024 | B1 | 1/2007 |
| EP | 0873089 | B1 | 10/2003 | EP | 1749485 | A1 | 2/2007 |
| EP | 0856326 | B1 | 11/2003 | EP | 1754445 | A2 | 2/2007 |
| EP | 1374788 | A1 | 1/2004 | EP | 1759812 | A1 | 3/2007 |
| EP | 0741996 | B1 | 2/2004 | EP | 1767157 | A1 | 3/2007 |
| EP | 0814712 | B1 | 2/2004 | EP | 1767163 | A1 | 3/2007 |
| EP | 1402837 | A1 | 3/2004 | EP | 1769756 | A1 | 4/2007 |
| EP | 0705570 | B1 | 4/2004 | EP | 1769758 | A1 | 4/2007 |
| EP | 0959784 | B1 | 4/2004 | EP | 1581128 | B1 | 5/2007 |
| EP | 1407719 | A2 | 4/2004 | EP | 1780825 | A1 | 5/2007 |
| EP | 1086713 | B1 | 5/2004 | EP | 1785097 | A2 | 5/2007 |
| EP | 0996378 | B1 | 6/2004 | EP | 1790293 | A2 | 5/2007 |
| EP | 1426012 | A1 | 6/2004 | EP | 1790294 | A1 | 5/2007 |
| EP | 0833593 | B2 | 7/2004 | EP | 1800610 | A1 | 6/2007 |
| EP | 1442694 | A1 | 8/2004 | EP | 1300117 | B1 | 8/2007 |
| EP | 0888749 | B1 | 9/2004 | EP | 1813199 | A1 | 8/2007 |
| EP | 0959786 | B1 | 9/2004 | EP | 1813200 | A2 | 8/2007 |
| EP | 1459695 | A1 | 9/2004 | EP | 1813201 | A1 | 8/2007 |
| EP | 1254636 | B1 | 10/2004 | EP | 1813202 | A1 | 8/2007 |
| EP | 1473819 | A1 | 11/2004 | EP | 1813203 | A2 | 8/2007 |
| EP | 1477119 | A1 | 11/2004 | EP | 1813207 | A1 | 8/2007 |
| EP | 1479345 | A1 | 11/2004 | EP | 1813209 | A1 | 8/2007 |
| EP | 1479347 | A1 | 11/2004 | EP | 1837041 | A1 | 9/2007 |
| EP | 1479348 | A1 | 11/2004 | EP | 0922435 | B1 | 10/2007 |
| EP | 0754437 | B2 | 12/2004 | EP | 1487359 | B1 | 10/2007 |
| EP | 1025807 | B1 | 12/2004 | EP | 1599146 | B1 | 10/2007 |
| EP | 1001710 | B1 | 1/2005 | EP | 1839596 | A1 | 10/2007 |
| EP | 1520521 | A1 | 4/2005 | EP | 2110083 | A2 | 10/2007 |
| EP | 1520522 | A1 | 4/2005 | EP | 1679096 | B1 | 11/2007 |
| EP | 1520523 | A1 | 4/2005 | EP | 1857057 | A2 | 11/2007 |
| EP | 1520525 | A1 | 4/2005 | EP | 1402821 | B1 | 12/2007 |
| EP | 1522264 | A1 | 4/2005 | EP | 1872727 | A1 | 1/2008 |
| EP | 1523942 | A2 | 4/2005 | EP | 1550410 | B1 | 2/2008 |
| EP | 1550408 | A1 | 7/2005 | EP | 1671593 | B1 | 2/2008 |
| EP | 1557129 | A1 | 7/2005 | EP | 1897502 | A1 | 3/2008 |
| EP | 1064883 | B1 | 8/2005 | EP | 1611856 | B1 | 4/2008 |
| EP | 1067876 | B1 | 8/2005 | EP | 1908417 | A2 | 4/2008 |
| EP | 0870473 | B1 | 9/2005 | EP | 1330201 | B1 | 6/2008 |
| EP | 1157666 | B1 | 9/2005 | EP | 1702568 | B1 | 7/2008 |
| EP | 0880338 | B1 | 10/2005 | EP | 1943955 | A2 | 7/2008 |
| EP | 1158917 | B1 | 11/2005 | EP | 1943957 | A2 | 7/2008 |
| EP | 1344498 | B1 | 11/2005 | EP | 1943962 | A2 | 7/2008 |
| EP | 0906764 | B1 | 12/2005 | EP | 1943964 | A1 | 7/2008 |
| EP | 1330989 | B1 | 12/2005 | EP | 1943976 | A2 | 7/2008 |
| EP | 0771176 | B2 | 1/2006 | EP | 1593337 | B1 | 8/2008 |
| EP | 1621138 | A2 | 2/2006 | EP | 1970014 | A1 | 9/2008 |
| EP | 1621139 | A2 | 2/2006 | EP | 1980213 | A2 | 10/2008 |
| EP | 1621141 | A2 | 2/2006 | EP | 1759645 | B1 | 11/2008 |
| EP | 1621145 | A2 | 2/2006 | EP | 1990014 | A2 | 11/2008 |
| EP | 1621151 | A2 | 2/2006 | EP | 1552795 | B1 | 12/2008 |
| EP | 1034746 | B1 | 3/2006 | EP | 1693008 | B1 | 12/2008 |
| EP | 1201196 | B1 | 3/2006 | EP | 1759640 | B1 | 12/2008 |
| EP | 1632191 | A2 | 3/2006 | EP | 1997439 | A2 | 12/2008 |
| EP | 1647231 | A1 | 4/2006 | EP | 2000102 | A2 | 12/2008 |
| EP | 1065981 | B1 | 5/2006 | EP | 2005894 | A2 | 12/2008 |
| EP | 1082944 | B1 | 5/2006 | EP | 2005901 | A1 | 12/2008 |
| EP | 1652481 | A2 | 5/2006 | EP | 2008595 | A2 | 12/2008 |
| EP | 1382303 | B1 | 6/2006 | EP | 1736104 | B1 | 3/2009 |
| EP | 1253866 | B1 | 7/2006 | EP | 1749486 | B1 | 3/2009 |
| | | | | EP | 1782743 | B1 | 3/2009 |
| | | | | EP | 2039302 | A2 | 3/2009 |
| | | | | EP | 2039308 | A2 | 3/2009 |
| | | | | EP | 2039316 | A2 | 3/2009 |

(56)

References Cited

FOREIGN PATENT DOCUMENTS

| | | | | | | | |
|----|---------|----|---------|----|-------------|----|---------|
| EP | 1721576 | B1 | 4/2009 | EP | 2517651 | A2 | 10/2012 |
| EP | 1733686 | B1 | 4/2009 | EP | 1884206 | B1 | 3/2013 |
| EP | 2044890 | A1 | 4/2009 | EP | 2090238 | B1 | 4/2013 |
| EP | 1550409 | A1 | 6/2009 | EP | 2090234 | B1 | 9/2013 |
| EP | 1550413 | B1 | 6/2009 | EP | 2644124 | A1 | 10/2013 |
| EP | 1719461 | B1 | 6/2009 | EP | 2644209 | A2 | 10/2013 |
| EP | 1834594 | B1 | 6/2009 | ES | 2396594 | T3 | 2/2013 |
| EP | 2077093 | A2 | 7/2009 | FR | 459743 | A | 11/1913 |
| EP | 1745748 | B1 | 8/2009 | FR | 999646 | A | 2/1952 |
| EP | 2090237 | A1 | 8/2009 | FR | 1112936 | A | 3/1956 |
| EP | 2090241 | A1 | 8/2009 | FR | 2598905 | A1 | 11/1987 |
| EP | 2090244 | A2 | 8/2009 | FR | 2765794 | A | 1/1999 |
| EP | 2090245 | A1 | 8/2009 | FR | 2815842 | | 10/2000 |
| EP | 2090254 | A1 | 8/2009 | GB | 939929 | A | 10/1963 |
| EP | 2090256 | A2 | 8/2009 | GB | 1210522 | A | 10/1970 |
| EP | 2095777 | A2 | 9/2009 | GB | 1217159 | A | 12/1970 |
| EP | 2098170 | A2 | 9/2009 | GB | 1339394 | A | 12/1973 |
| EP | 2110082 | A1 | 10/2009 | GB | 2024012 | A | 1/1980 |
| EP | 2111803 | A2 | 10/2009 | GB | 2109241 | A | 6/1983 |
| EP | 1813208 | B1 | 11/2009 | GB | 2272159 | A | 5/1994 |
| EP | 1908426 | B1 | 11/2009 | GB | 2284242 | A | 5/1995 |
| EP | 2116195 | A1 | 11/2009 | GB | 2336214 | A | 10/1999 |
| EP | 1607050 | B1 | 12/2009 | GB | 2425903 | A | 11/2006 |
| EP | 1815804 | B1 | 12/2009 | GR | 93100110 | A | 11/1993 |
| EP | 1875870 | B1 | 12/2009 | GR | 930100110 | A | 11/1993 |
| EP | 1878395 | B1 | 1/2010 | JP | 50-33988 | U | 4/1975 |
| EP | 2151204 | A1 | 2/2010 | JP | S 58500053 | A | 1/1983 |
| EP | 2165656 | A2 | 3/2010 | JP | 60-100955 | A | 4/1985 |
| EP | 2165660 | A2 | 3/2010 | JP | 61-98249 | A | 5/1986 |
| EP | 1566150 | B1 | 4/2010 | JP | S 61502036 | A | 9/1986 |
| EP | 1813206 | B1 | 4/2010 | JP | S 63-59764 | A | 3/1988 |
| EP | 1769754 | B1 | 6/2010 | JP | S 63-147449 | A | 6/1988 |
| EP | 1854416 | B1 | 6/2010 | JP | 63-203149 | | 8/1988 |
| EP | 2198787 | A1 | 6/2010 | JP | H 02-279149 | A | 11/1990 |
| EP | 1647286 | B1 | 9/2010 | JP | 3-12126 | A | 1/1991 |
| EP | 1825821 | B1 | 9/2010 | JP | H 05-084252 | A | 4/1993 |
| EP | 1535565 | B1 | 10/2010 | JP | 5-212039 | A | 8/1993 |
| EP | 1702570 | B1 | 10/2010 | JP | 6007357 | A | 1/1994 |
| EP | 1785098 | B1 | 10/2010 | JP | H 6-30945 | | 2/1994 |
| EP | 2005896 | B1 | 10/2010 | JP | H 06-26812 | U | 4/1994 |
| EP | 2030578 | B1 | 11/2010 | JP | H 6-121798 | A | 5/1994 |
| EP | 1627605 | B1 | 12/2010 | JP | H 06-197901 | A | 7/1994 |
| EP | 2027811 | B1 | 12/2010 | JP | H 06-237937 | A | 8/1994 |
| EP | 2130498 | B1 | 12/2010 | JP | 7051273 | A | 2/1995 |
| EP | 1994890 | B1 | 1/2011 | JP | 7-124166 | A | 5/1995 |
| EP | 2005900 | B1 | 1/2011 | JP | 07-171163 | | 7/1995 |
| EP | 2286738 | A2 | 2/2011 | JP | 7-255735 | A | 10/1995 |
| EP | 1690502 | B1 | 3/2011 | JP | 8-33642 | A | 2/1996 |
| EP | 2292153 | A1 | 3/2011 | JP | 8033641 | A | 2/1996 |
| EP | 1769755 | B1 | 4/2011 | JP | 8-164141 | A | 6/1996 |
| EP | 2090240 | B1 | 4/2011 | JP | H 08-182684 | A | 7/1996 |
| EP | 2305135 | A1 | 4/2011 | JP | H 08-507708 | A | 8/1996 |
| EP | 2314254 | A2 | 4/2011 | JP | 8229050 | A | 9/1996 |
| EP | 1813205 | B1 | 6/2011 | JP | H 09-501081 | A | 2/1997 |
| EP | 2090243 | B1 | 6/2011 | JP | H 09-501577 | A | 2/1997 |
| EP | 2329773 | A1 | 6/2011 | JP | H 09-164144 | A | 6/1997 |
| EP | 1908414 | B1 | 11/2011 | JP | H 10-118090 | A | 5/1998 |
| EP | 2153781 | B1 | 11/2011 | JP | H 10-512469 | A | 12/1998 |
| EP | 2389928 | A2 | 11/2011 | JP | 2000-14632 | | 1/2000 |
| EP | 1847225 | B1 | 12/2011 | JP | 2000033071 | A | 2/2000 |
| EP | 1785102 | B1 | 1/2012 | JP | 2000-112002 | A | 4/2000 |
| EP | 2090253 | B1 | 3/2012 | JP | 2000171730 | A | 6/2000 |
| EP | 2457519 | A1 | 5/2012 | JP | 2000287987 | A | 10/2000 |
| EP | 2462880 | A2 | 6/2012 | JP | 2000325303 | A | 11/2000 |
| EP | 1813204 | B1 | 7/2012 | JP | 2001-046384 | A | 2/2001 |
| EP | 2189121 | B1 | 7/2012 | JP | 2001-514541 | A | 9/2001 |
| EP | 2005895 | B1 | 8/2012 | JP | 2001-517473 | A | 10/2001 |
| EP | 2090248 | B1 | 8/2012 | JP | 2001286477 | A | 10/2001 |
| EP | 2481359 | A1 | 8/2012 | JP | 2002143078 | A | 5/2002 |
| EP | 1616549 | B1 | 10/2012 | JP | 2002-528161 | A | 9/2002 |
| EP | 2030579 | B1 | 10/2012 | JP | 2002369820 | A | 12/2002 |
| EP | 2090252 | B1 | 10/2012 | JP | 2003-500153 | A | 1/2003 |
| EP | 2517637 | A1 | 10/2012 | JP | 2003-164066 | | 6/2003 |
| EP | 2517645 | A2 | 10/2012 | JP | 2003-521301 | A | 7/2003 |
| EP | 2517649 | A2 | 10/2012 | JP | 2004-162035 | A | 6/2004 |
| | | | | JP | 2004-229976 | A | 8/2004 |
| | | | | JP | 2004-531280 | A | 10/2004 |
| | | | | JP | 2004-532084 | A | 10/2004 |
| | | | | JP | 2004-532676 | A | 10/2004 |

(56)

References Cited

| FOREIGN PATENT DOCUMENTS | | | RU | | U1 | |
|--------------------------|--------------|----|---------|----|-------------|------------|
| JP | 2004-4532676 | A | 10/2004 | RU | 42750 | 12/2004 |
| JP | 2004-329624 | A | 11/2004 | RU | 61114 | 2/2007 |
| JP | 2004-344663 | | 12/2004 | SU | 189517 | A 1/1967 |
| JP | 2005-028147 | A | 2/2005 | SU | 328636 | A 9/1972 |
| JP | 2005-28148 | A | 2/2005 | SU | 674747 | A1 7/1979 |
| JP | 2005-028149 | A | 2/2005 | SU | 886900 | A1 12/1981 |
| JP | 2005-505309 | A | 2/2005 | SU | 1009439 | A 4/1983 |
| JP | 2005505322 | T | 2/2005 | SU | 1022703 | A1 6/1983 |
| JP | 2005-103280 | A | 4/2005 | SU | 1333319 | A2 8/1987 |
| JP | 2005-103281 | A | 4/2005 | SU | 1377053 | A1 2/1988 |
| JP | 2005-511131 | A | 4/2005 | SU | 1509051 | A1 9/1989 |
| JP | 2005103293 | A | 4/2005 | SU | 1561964 | A1 5/1990 |
| JP | 2005131163 | A | 5/2005 | SU | 1708312 | A1 1/1992 |
| JP | 2005131164 | A | 5/2005 | SU | 1722476 | A1 3/1992 |
| JP | 2005131173 | A | 5/2005 | SU | 1752361 | A1 8/1992 |
| JP | 2005131211 | A | 5/2005 | SU | 1814161 | A1 5/1993 |
| JP | 2005131212 | A | 5/2005 | WO | WO 82/02824 | A1 9/1982 |
| JP | 2005-144183 | A | 6/2005 | WO | WO 86/02254 | A1 4/1986 |
| JP | 2005-516714 | A | 6/2005 | WO | WO 91/15157 | A1 10/1991 |
| JP | 2005137423 | A | 6/2005 | WO | WO 92/20295 | A1 11/1992 |
| JP | 2005152416 | A | 6/2005 | WO | WO 92/21300 | A1 12/1992 |
| JP | 2005-523105 | A | 8/2005 | WO | WO 93/08755 | A1 5/1993 |
| JP | 4461008 | B2 | 8/2005 | WO | WO 93/13718 | A1 7/1993 |
| JP | 2005524474 | A | 8/2005 | WO | WO 93/14690 | A1 8/1993 |
| JP | 2005-335432 | A | 12/2005 | WO | WO 93/15648 | A1 8/1993 |
| JP | 2005-342267 | A | 12/2005 | WO | WO 93/15850 | A1 8/1993 |
| JP | 2006-034975 | A | 2/2006 | WO | WO 93/19681 | A1 10/1993 |
| JP | 2006-34977 | A | 2/2006 | WO | WO 94/00060 | A1 1/1994 |
| JP | 2006-034980 | A | 2/2006 | WO | WO 94/11057 | A1 5/1994 |
| JP | 2006-506106 | A | 2/2006 | WO | WO 94/12108 | A1 6/1994 |
| JP | 2006-187649 | A | 7/2006 | WO | WO 94/18893 | A1 9/1994 |
| JP | 2006-218297 | A | 8/2006 | WO | WO 94/20030 | A1 9/1994 |
| JP | 2006-223872 | A | 8/2006 | WO | WO 94/22378 | A1 10/1994 |
| JP | 2006-281405 | A | 10/2006 | WO | WO 94/23659 | A1 10/1994 |
| JP | 2006-334417 | A | 12/2006 | WO | WO 94/24943 | A1 11/1994 |
| JP | 2006-346445 | A | 12/2006 | WO | WO 94-24947 | A1 11/1994 |
| JP | 2007-61628 | A | 3/2007 | WO | WO 95/02369 | A1 1/1995 |
| JP | 2007-098130 | A | 4/2007 | WO | WO 95/03743 | A1 2/1995 |
| JP | 2007-105481 | A | 4/2007 | WO | WO 95/06817 | A1 3/1995 |
| JP | 3906843 | B2 | 4/2007 | WO | WO 95/09576 | A1 4/1995 |
| JP | 2007-117725 | A | 5/2007 | WO | WO 95/09577 | A1 4/1995 |
| JP | 2007-130471 | A | 5/2007 | WO | WO 95/14436 | A1 6/1995 |
| JP | 2007-222615 | A | 6/2007 | WO | WO 95/17855 | A1 7/1995 |
| JP | 2007-203051 | A | 8/2007 | WO | WO 95/18383 | A1 7/1995 |
| JP | 2007-203057 | A | 8/2007 | WO | WO 95/18572 | A1 7/1995 |
| JP | 2007/524435 | A | 8/2007 | WO | WO 95/19739 | A1 7/1995 |
| JP | 2007-229448 | A | 9/2007 | WO | WO 95/20360 | A1 8/1995 |
| JP | 4001860 | B2 | 10/2007 | WO | WO 95/23557 | A1 9/1995 |
| JP | 2007-325922 | A | 12/2007 | WO | WO 95/24865 | A1 9/1995 |
| JP | 2008-68073 | A | 3/2008 | WO | WO 95/25471 | A3 9/1995 |
| JP | 2008-259860 | A | 10/2008 | WO | WO 95/26562 | A1 10/1995 |
| JP | 2008-264535 | A | 11/2008 | WO | WO 95/29639 | A1 11/1995 |
| JP | 2008-283459 | A | 11/2008 | WO | WO 96/04858 | A1 2/1996 |
| JP | 2009-502351 | A | 1/2009 | WO | WO 96/18344 | A2 6/1996 |
| JP | 2009-506799 | A | 2/2009 | WO | WO 96/19151 | A1 6/1996 |
| JP | 2009-106752 | A | 5/2009 | WO | WO 96/19152 | A1 6/1996 |
| JP | 2009-189836 | A | 8/2009 | WO | WO 96/20652 | A1 7/1996 |
| JP | 2009-539420 | A | 11/2009 | WO | WO 96/21119 | A1 7/1996 |
| JP | 2010-098844 | A | 4/2010 | WO | WO 96/22055 | A1 7/1996 |
| JP | 4549018 | B2 | 9/2010 | WO | WO 96/23448 | A1 8/1996 |
| JP | 4783373 | B2 | 7/2011 | WO | WO 96/24301 | A1 8/1996 |
| JP | 5410421 | B2 | 11/2012 | WO | WO 96/24301 | A1 8/1996 |
| JP | 5140421 | B2 | 6/2013 | WO | WO 96/27337 | A1 9/1996 |
| JP | 2013-128791 | A | 7/2013 | WO | WO 96/31155 | A1 10/1996 |
| JP | 5333899 | B2 | 11/2013 | WO | WO 96/35464 | A1 11/1996 |
| RU | 2008830 | C1 | 3/1994 | WO | WO 96/39085 | A1 12/1996 |
| RU | 2052979 | C1 | 1/1996 | WO | WO 96/39086 | A1 12/1996 |
| RU | 2098025 | C1 | 12/1997 | WO | WO 96/39087 | A1 12/1996 |
| RU | 2141279 | C1 | 11/1999 | WO | WO 96/39088 | A1 12/1996 |
| RU | 2144791 | C1 | 1/2000 | WO | WO 96/39089 | A1 12/1996 |
| RU | 2181566 | C2 | 4/2002 | WO | WO 97/00646 | A1 1/1997 |
| RU | 2187249 | C2 | 8/2002 | WO | WO 97/00647 | A1 1/1997 |
| RU | 2189091 | C2 | 9/2002 | WO | WO 97/01989 | A1 1/1997 |
| RU | 32984 | U1 | 10/2003 | WO | WO 97/06582 | A1 2/1997 |
| RU | 2225170 | C2 | 3/2004 | WO | WO 97/10763 | A1 3/1997 |
| | | | | WO | WO 97/10764 | A1 3/1997 |
| | | | | WO | WO 97/11648 | A2 4/1997 |
| | | | | WO | WO 97/11649 | A1 4/1997 |
| | | | | WO | WO 97/15237 | A1 5/1997 |
| | | | | WO | WO 97/24073 | A1 7/1997 |

(56)

References Cited

FOREIGN PATENT DOCUMENTS

| | | | | | | | |
|----|--------------|----|---------|----|----------------|----|---------|
| WO | WO 97/24993 | A1 | 7/1997 | WO | WO 03/037193 | A1 | 5/2003 |
| WO | WO 97/30644 | A1 | 8/1997 | WO | WO 03/047436 | A3 | 6/2003 |
| WO | WO 97/34533 | A1 | 9/1997 | WO | WO 03/055402 | A1 | 7/2003 |
| WO | WO 97/37598 | A1 | 10/1997 | WO | WO 03/057048 | A1 | 7/2003 |
| WO | WO 97/39688 | A2 | 10/1997 | WO | WO 03/057058 | A1 | 7/2003 |
| WO | WO 98/01080 | A1 | 1/1998 | WO | WO 03/063694 | A1 | 8/2003 |
| WO | WO 98/17180 | A1 | 4/1998 | WO | WO 03/077769 | A1 | 9/2003 |
| WO | WO 98/27880 | A1 | 7/1998 | WO | WO 03/079911 | A1 | 10/2003 |
| WO | WO 98/30153 | A1 | 7/1998 | WO | WO 03/082126 | A1 | 10/2003 |
| WO | WO 98/47436 | A1 | 10/1998 | WO | WO 03/086206 | A1 | 10/2003 |
| WO | WO 99/03407 | A1 | 1/1999 | WO | WO 03/088845 | A2 | 10/2003 |
| WO | WO 99/03408 | A1 | 1/1999 | WO | WO 03/090630 | A2 | 11/2003 |
| WO | WO 99/03409 | A1 | 1/1999 | WO | WO 03/094743 | A1 | 11/2003 |
| WO | WO 99/12483 | A1 | 3/1999 | WO | WO 03/094745 | A1 | 11/2003 |
| WO | WO 99/12487 | A1 | 3/1999 | WO | WO 03/094746 | A1 | 11/2003 |
| WO | WO 99/12488 | A1 | 3/1999 | WO | WO 03/094747 | A1 | 11/2003 |
| WO | WO 99/15086 | A1 | 4/1999 | WO | WO 03/101313 | A1 | 12/2003 |
| WO | WO 99/15091 | A1 | 4/1999 | WO | WO 03/105698 | A2 | 12/2003 |
| WO | WO 99/23933 | A2 | 5/1999 | WO | WO 03/105702 | A2 | 12/2003 |
| WO | WO 99/23959 | A1 | 5/1999 | WO | WO 2004/006980 | A2 | 1/2004 |
| WO | WO 99/25261 | A1 | 5/1999 | WO | WO 2004/011037 | A2 | 2/2004 |
| WO | WO 99/29244 | A1 | 6/1999 | WO | WO 2004/019769 | A1 | 3/2004 |
| WO | WO 99/34744 | A1 | 7/1999 | WO | WO 2004/019803 | A1 | 3/2004 |
| WO | WO 99/45849 | A1 | 9/1999 | WO | WO 2004/021868 | A2 | 3/2004 |
| WO | WO 99/48430 | A1 | 9/1999 | WO | WO 2004/028585 | A2 | 4/2004 |
| WO | WO 99/51158 | A1 | 10/1999 | WO | WO 2004/032754 | A2 | 4/2004 |
| WO | WO 00/24322 | A1 | 5/2000 | WO | WO 2004/032760 | A2 | 4/2004 |
| WO | WO 00/24330 | A1 | 5/2000 | WO | WO 2004/032762 | A1 | 4/2004 |
| WO | WO 00/41638 | A1 | 7/2000 | WO | WO 2004/032763 | A2 | 4/2004 |
| WO | WO 00/48506 | A1 | 8/2000 | WO | WO 2004/034875 | A2 | 4/2004 |
| WO | WO 00/53112 | A2 | 9/2000 | WO | WO 2004/047626 | A1 | 6/2004 |
| WO | WO 00/54653 | A1 | 9/2000 | WO | WO 2004/047653 | A2 | 6/2004 |
| WO | WO 00/57796 | A1 | 10/2000 | WO | WO 2004/049956 | A2 | 6/2004 |
| WO | WO 00/64365 | A1 | 11/2000 | WO | WO 2004/052426 | A2 | 6/2004 |
| WO | WO 00/72762 | A1 | 12/2000 | WO | WO 2004/056276 | A1 | 7/2004 |
| WO | WO 00/72765 | A1 | 12/2000 | WO | WO 2004/056277 | A1 | 7/2004 |
| WO | WO 01/03587 | A1 | 1/2001 | WO | WO 2004/062516 | A1 | 7/2004 |
| WO | WO 01/05702 | A1 | 1/2001 | WO | WO 2004/078050 | A2 | 9/2004 |
| WO | WO 01/10482 | A1 | 2/2001 | WO | WO 2004/078051 | A2 | 9/2004 |
| WO | WO 01/35845 | A1 | 5/2001 | WO | WO 2004/078236 | A2 | 9/2004 |
| WO | WO 01/54594 | A1 | 8/2001 | WO | WO 2004/086987 | A1 | 10/2004 |
| WO | WO 01/58371 | A1 | 8/2001 | WO | WO 2004/096015 | A2 | 11/2004 |
| WO | WO 01/62158 | A2 | 8/2001 | WO | WO 2004/096057 | A2 | 11/2004 |
| WO | WO 01/62161 | A1 | 8/2001 | WO | WO 2004/103157 | A2 | 12/2004 |
| WO | WO 01/62162 | A1 | 8/2001 | WO | WO 2004/105593 | A1 | 12/2004 |
| WO | WO 01/62164 | A2 | 8/2001 | WO | WO 2004/105621 | A1 | 12/2004 |
| WO | WO 01/62169 | A2 | 8/2001 | WO | WO 2004/112618 | A2 | 12/2004 |
| WO | WO 01/78605 | A2 | 10/2001 | WO | WO 2004/112652 | A2 | 12/2004 |
| WO | WO 01/80757 | A2 | 11/2001 | WO | WO 2005/027983 | A2 | 3/2005 |
| WO | WO 01/91646 | A1 | 12/2001 | WO | WO 2005/037329 | A2 | 4/2005 |
| WO | WO 02/00121 | A1 | 1/2002 | WO | WO 2005/042041 | A1 | 5/2005 |
| WO | WO 02/07608 | A2 | 1/2002 | WO | WO 2005/044078 | A2 | 5/2005 |
| WO | WO 02/07618 | A1 | 1/2002 | WO | WO 2005/055846 | A1 | 6/2005 |
| WO | WO 02/17799 | A1 | 3/2002 | WO | WO 2005/072634 | A2 | 8/2005 |
| WO | WO 02/19920 | A1 | 3/2002 | WO | WO 2005/078892 | A1 | 8/2005 |
| WO | WO 02/19932 | A1 | 3/2002 | WO | WO 2005/079675 | A2 | 9/2005 |
| WO | WO 02/30297 | A2 | 4/2002 | WO | WO 2005/096954 | A2 | 10/2005 |
| WO | WO 02/32322 | A2 | 4/2002 | WO | WO 2005/112806 | A2 | 12/2005 |
| WO | WO 02/36028 | A1 | 5/2002 | WO | WO 2005/112808 | A1 | 12/2005 |
| WO | WO 02/43571 | A2 | 6/2002 | WO | WO 2005/115251 | A2 | 12/2005 |
| WO | WO 02/058568 | A1 | 8/2002 | WO | WO 2005/115253 | A2 | 12/2005 |
| WO | WO 02/060328 | A1 | 8/2002 | WO | WO 2005/117735 | A1 | 12/2005 |
| WO | WO 02/067785 | A2 | 9/2002 | WO | WO 2005/122936 | A1 | 12/2005 |
| WO | WO 02/087586 | A1 | 11/2002 | WO | WO 2006/023486 | A1 | 3/2006 |
| WO | WO 02/098302 | A1 | 12/2002 | WO | WO 2006/023578 | A2 | 3/2006 |
| WO | WO 03/000138 | A2 | 1/2003 | WO | WO 2006/027014 | A1 | 3/2006 |
| WO | WO 03/001329 | A2 | 1/2003 | WO | WO 2006/028314 | A1 | 3/2006 |
| WO | WO 03/013363 | A1 | 2/2003 | WO | WO 2006/044490 | A2 | 4/2006 |
| WO | WO 03/013372 | A2 | 2/2003 | WO | WO 2006/044581 | A2 | 4/2006 |
| WO | WO 03/015604 | A2 | 2/2003 | WO | WO 2006/044810 | A2 | 4/2006 |
| WO | WO 03/020106 | A2 | 3/2003 | WO | WO 2006/051252 | A1 | 5/2006 |
| WO | WO 03/020139 | A2 | 3/2003 | WO | WO 2006/059067 | A1 | 6/2006 |
| WO | WO 03/024339 | A1 | 3/2003 | WO | WO 2006/083748 | A1 | 8/2006 |
| WO | WO 03/079909 | A3 | 3/2003 | WO | WO 2006/092563 | A1 | 9/2006 |
| WO | WO 03/030743 | A2 | 4/2003 | WO | WO 2006/092565 | A1 | 9/2006 |
| | | | | WO | WO 2006/115958 | A1 | 11/2006 |
| | | | | WO | WO 2006/125940 | A1 | 11/2006 |
| | | | | WO | WO 2006/132992 | A1 | 12/2006 |
| | | | | WO | WO 2007/002180 | A2 | 1/2007 |

(56)

References Cited

FOREIGN PATENT DOCUMENTS

| | | | |
|----|----------------|----|---------|
| WO | WO 2007/016290 | A2 | 2/2007 |
| WO | WO 2007/018898 | A2 | 2/2007 |
| WO | WO 2007/089603 | A2 | 8/2007 |
| WO | WO 2007/098220 | A2 | 8/2007 |
| WO | WO 2007/121579 | A1 | 11/2007 |
| WO | WO 2007/131110 | A2 | 11/2007 |
| WO | WO 2007/137304 | A2 | 11/2007 |
| WO | WO 2007/139734 | A2 | 12/2007 |
| WO | WO 2007/142625 | A2 | 12/2007 |
| WO | WO 2007/145825 | A2 | 12/2007 |
| WO | WO 2007/147439 | A1 | 12/2007 |
| WO | WO 2008/020964 | A2 | 2/2008 |
| WO | WO 2008/021969 | A2 | 2/2008 |
| WO | WO 2008/039249 | A1 | 4/2008 |
| WO | WO 2008/039270 | A1 | 4/2008 |
| WO | WO 2008/045383 | A2 | 4/2008 |
| WO | WO 2008/057281 | A2 | 5/2008 |
| WO | WO 2008/070763 | A1 | 6/2008 |
| WO | WO 2008/089404 | A2 | 7/2008 |
| WO | WO 2008/101080 | A1 | 8/2008 |
| WO | WO 2008/109125 | A1 | 9/2008 |
| WO | WO 2008/124748 | A1 | 10/2008 |
| WO | WO 2009/023851 | A1 | 2/2009 |
| WO | WO 2009/033057 | A2 | 3/2009 |
| WO | WO 2009/046394 | A1 | 4/2009 |
| WO | WO 2009/137761 | A2 | 11/2009 |
| WO | WO 2009/143092 | A1 | 11/2009 |
| WO | WO 2009/143331 | A1 | 11/2009 |
| WO | WO 2010/028332 | A2 | 3/2010 |
| WO | WO 2010/030434 | A1 | 3/2010 |
| WO | WO 2010/054404 | A1 | 5/2010 |
| WO | WO 2010/063795 | A1 | 6/2010 |
| WO | WO 2010/098871 | A2 | 9/2010 |
| WO | WO 2011/044343 | A2 | 4/2011 |
| WO | WO 2012/021671 | A1 | 2/2012 |
| WO | WO 2012/044551 | A1 | 4/2012 |
| WO | WO 2012/044554 | A1 | 4/2012 |
| WO | WO 2012/044820 | A1 | 4/2012 |
| WO | WO 2012/044844 | A2 | 4/2012 |
| WO | WO 2013/043717 | A1 | 3/2013 |

OTHER PUBLICATIONS

Disclosed Anonymously, "Motor-Driven Surgical Stapler Improvements," Research Disclosure Database No. 526041, Published: Feb. 2008.

C.C. Thompson et al., "Peroral Endoscopic Reduction of Dilated Gastrojejunal Anastomosis After Roux-en-Y Gastric Bypass: A Possible New Option for Patients with Weight Regain," *Surg Endosc* (2006) vol. 20, pp. 1744-1748.

B.R. Coolman, DVM, MS et al., "Comparison of Skin Staples With Sutures for Anastomosis of the Small Intestine in Dogs," Abstract; <http://www.blackwell-synergy.com/doi/abs/10.1053/jvet.2000.7539?cookieSet=1&journalCode=vsu> which redirects to <http://www3.interscience.wiley.com/journal/119040681/abstract?CRETRY=1&SRETRY=0>; [online] accessed: Sep. 22, 2008 (2 pages).

The Sodem Aseptic Battery Transfer Kit, Sodem Systems, (2000), 3 pages.

"Biomedical Coatings," Fort Wayne Metals, Research Products Corporation, obtained online at www.fwmetals.com on Jun. 21, 2010 (1 page).

Van Meer et al., "A Disposable Plastic Compact Wrist for Smart Minimally Invasive Surgical Tools," LAAS/CNRS (Aug. 2005).

Breedveld et al., "A New, Easily Miniaturized Sterrable Endoscope," *IEEE Engineering in Medicine and Biology Magazine* (Nov./Dec. 2005).

D. Tuite, Ed., "Get the Lowdown on Ultracapacitors," Nov. 15, 2007; [online] URL: <http://electronicdesign.com/Articles/Print.cfm?ArticleID=17465>, accessed Jan. 15, 2008 (5 pages).

Datasheet for Panasonic TK Relays Ultra Low Profile 2 A Polarized Relay, Copyright Matsushita Electric Works, Ltd. (Known of at least as early as Aug. 17, 2010), 5 pages.

ASTM procedure D2240-00, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Aug. 2000).

ASTM procedure D2240-05, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Apr. 2010).

Covidien Brochure, "Endo GIA™ Reloads with Tri-Staple™ Technology," (2010), 1 page.

Covidien Brochure, "Endo GIA™ Reloads with Tri-Staple™ Technology and Endo GIA™ Ultra Universal Staplers," (2010), 2 pages.

Covidien Brochure, "Endo GIA™ Black Reload with Tri-Staple™ Technology," (2012), 2 pages.

Covidien Brochure, "Endo GIA™ Curved Tip Reload with Tri-Staple™ Technology," (2012), 2 pages.

Covidien Brochure, "Endo GIA™ Reloads with Tri-Staple™ Technology," (2010), 2 pages.

Covidien Brochure, "Endo GIA™ Ultra Universal Stapler," (2010), 2 pages.

Miyata et al., "Biomolecule-Sensitive Hydrogels," *Advanced Drug Delivery Reviews*, 54 (2002) pp. 79-98.

Jeong et al., "Thermosensitive Sol-Gel Reversible Hydrogels," *Advanced Drug Delivery Reviews*, 54 (2002) pp. 37-51.

Byrne et al., "Molecular Imprinting Within Hydrogels," *Advanced Drug Delivery Reviews*, 54 (2002) pp. 149-161.

Qiu et al., "Environment-Sensitive Hydrogels for Drug Delivery," *Advanced Drug Delivery Reviews*, 53 (2001) pp. 321-339.

Hoffman, "Hydrogels for Biomedical Applications," *Advanced Drug Delivery Reviews*, 43 (2002) pp. 30-12.

Hoffman, "Hydrogels for Biomedical Applications," *Advanced Drug Delivery Reviews*, 54 (2002) pp. 30-12.

Peppas, "Physiologically Responsive Hydrogels," *Journal of Bioactive and Compatible Polymers*, vol. 6 (Jul. 1991) pp. 241-246.

Ebara, "Carbohydrate-Derived Hydrogels and Microgels," *Engineered Carbohydrate-Based Materials for Biomedical Applications: Polymers, Surfaces, Dendrimers, Nanoparticles, and Hydrogels*, Edited by Ravin Narain, 2011, pp. 337-345.

Peppas, Editor "Hydrogels in Medicine and Pharmacy," vol. I, Fundamentals, CRC Press, 1986.

Matsuda, "Thermodynamics of Formation of Porous Polymeric Membrane from Solutions," *Polymer Journal*, vol. 23, No. 5, pp. 435-444 (1991).

Young, "Microcellular foams via phase separation," *Journal of Vacuum Science & Technology A* 4(3), (May/June. 1986).

International Preliminary Report on Patentability for PCT/US2012/028886, Sep. 17, 2013 (12 pages).

* cited by examiner

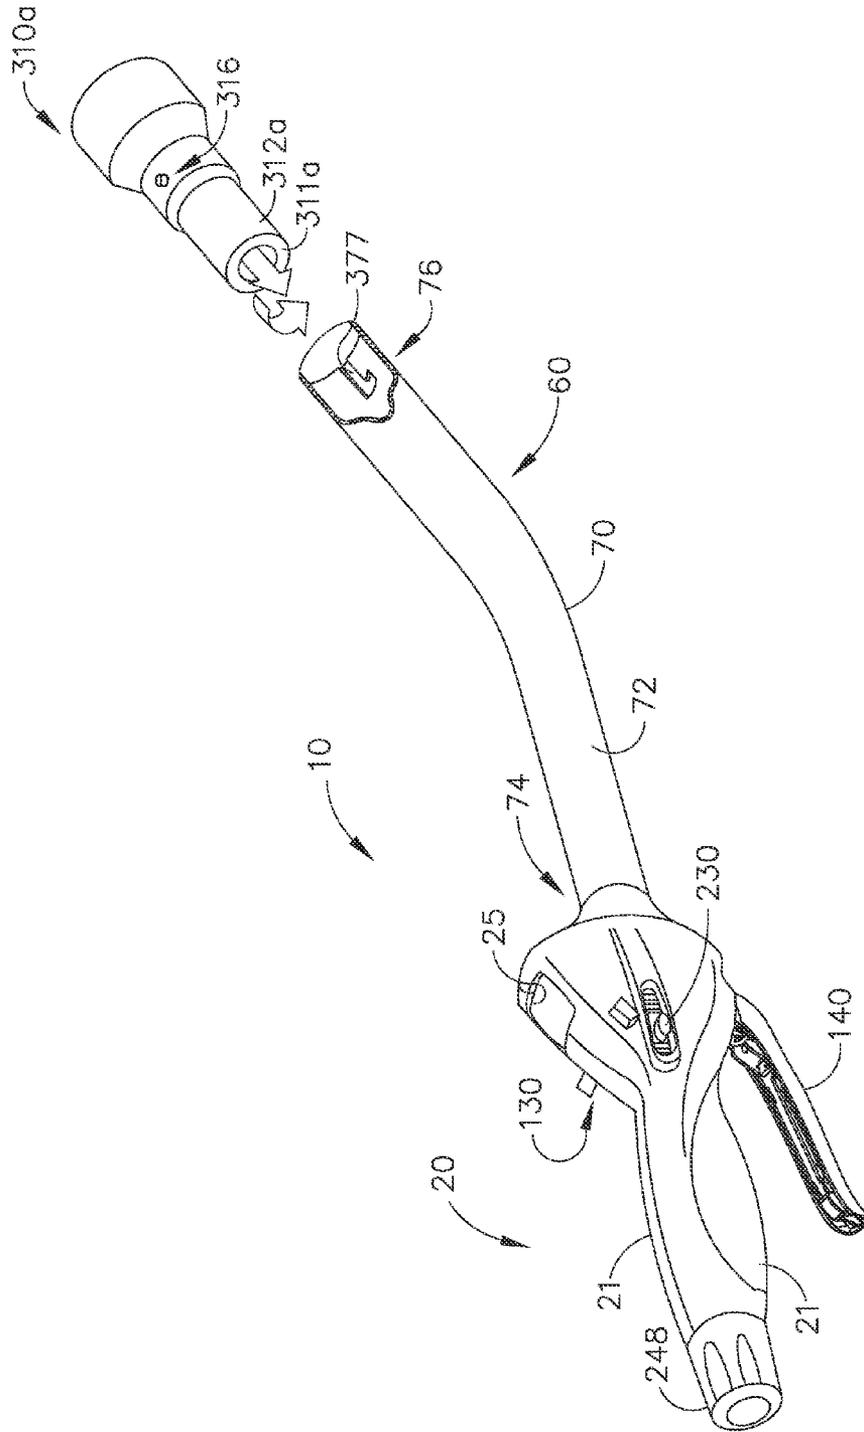


FIG. 1

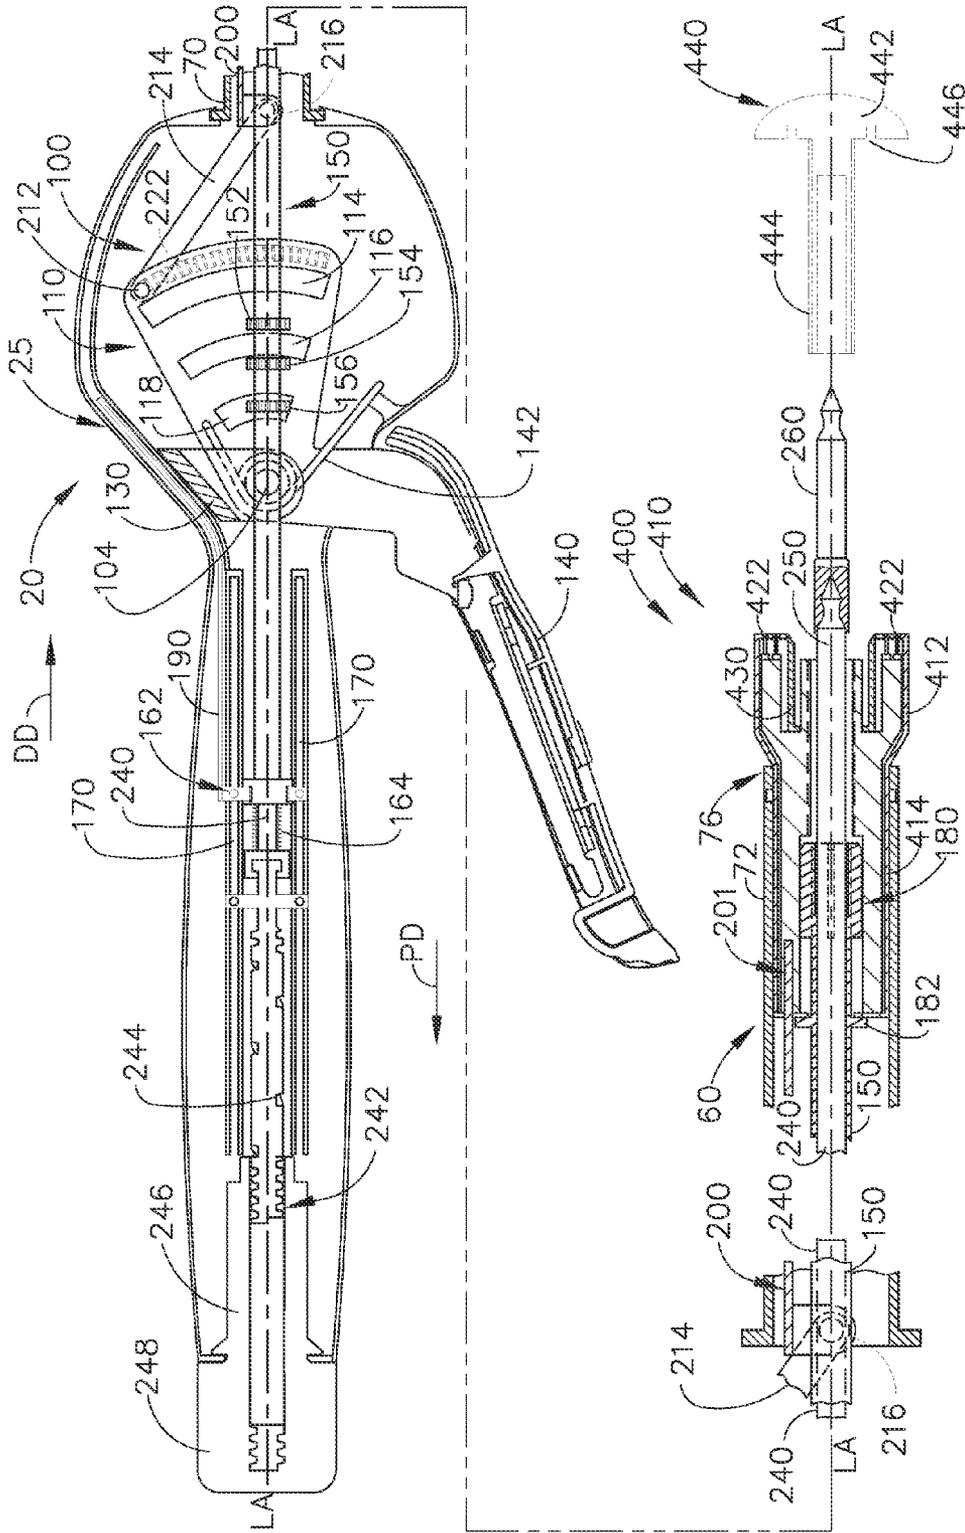


FIG. 2

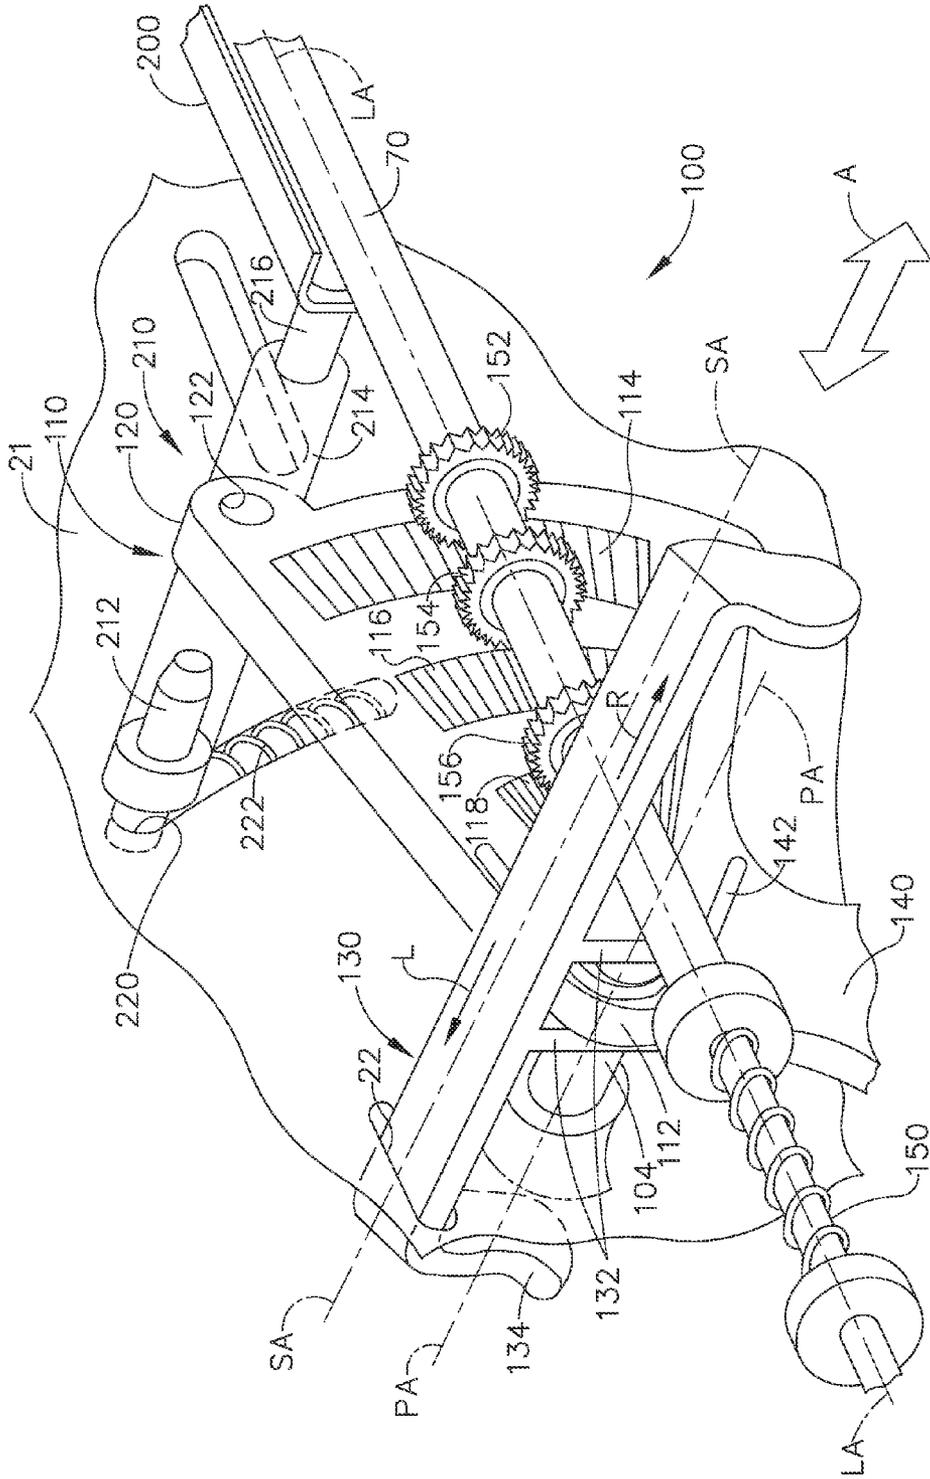


FIG. 3

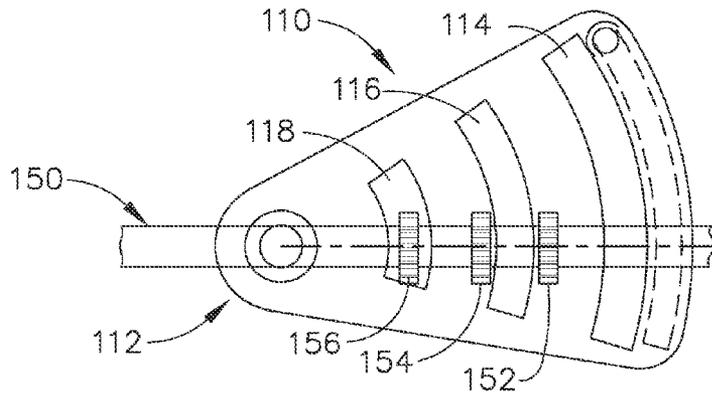


FIG. 3A

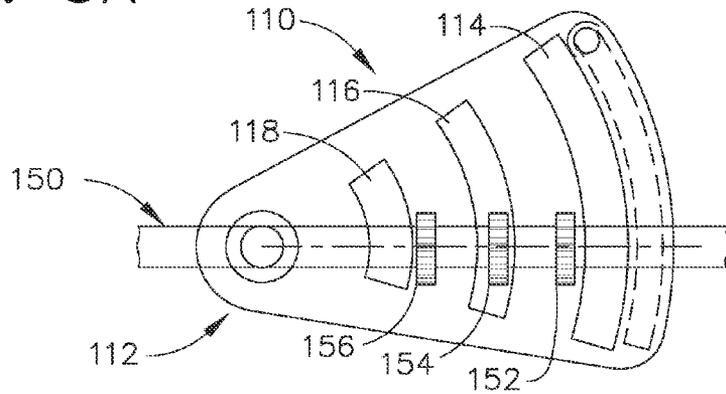


FIG. 3B

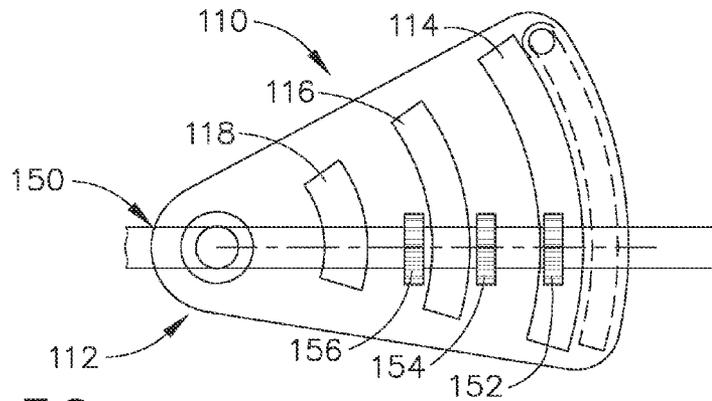


FIG. 3C

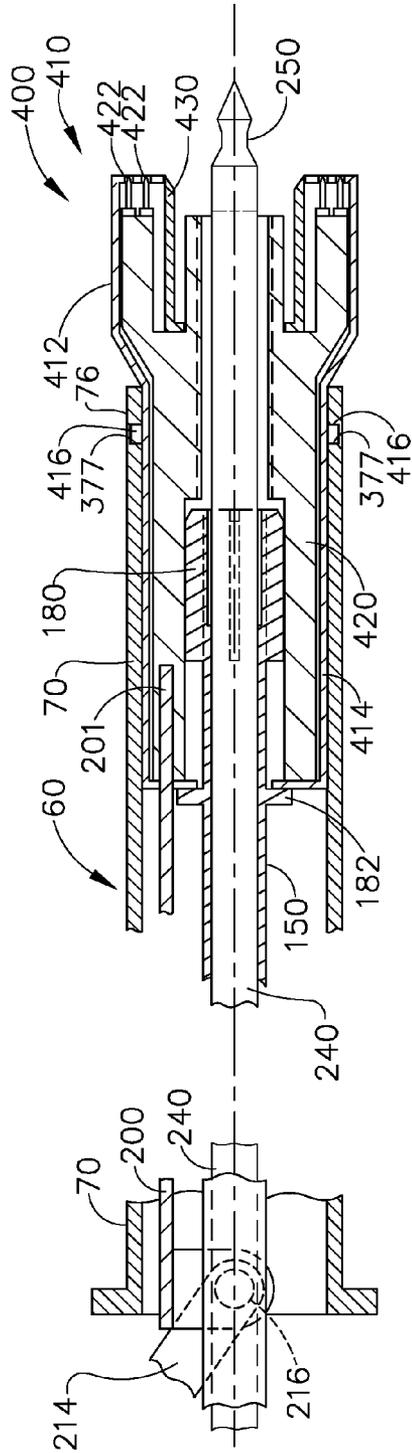


FIG. 5

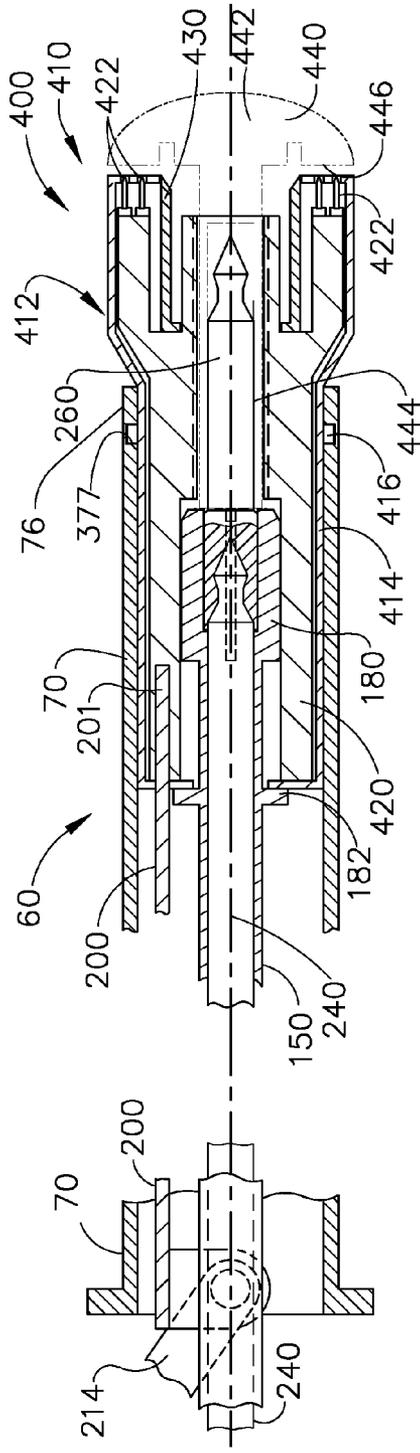


FIG. 5A

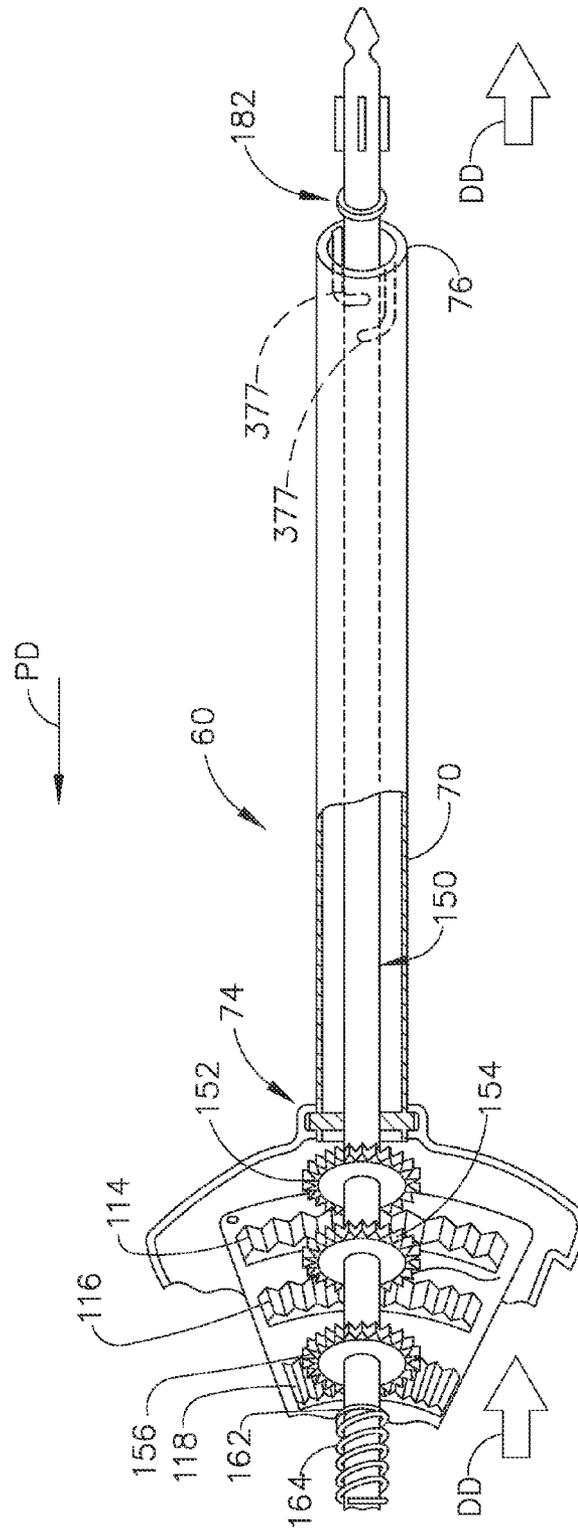


FIG. 6

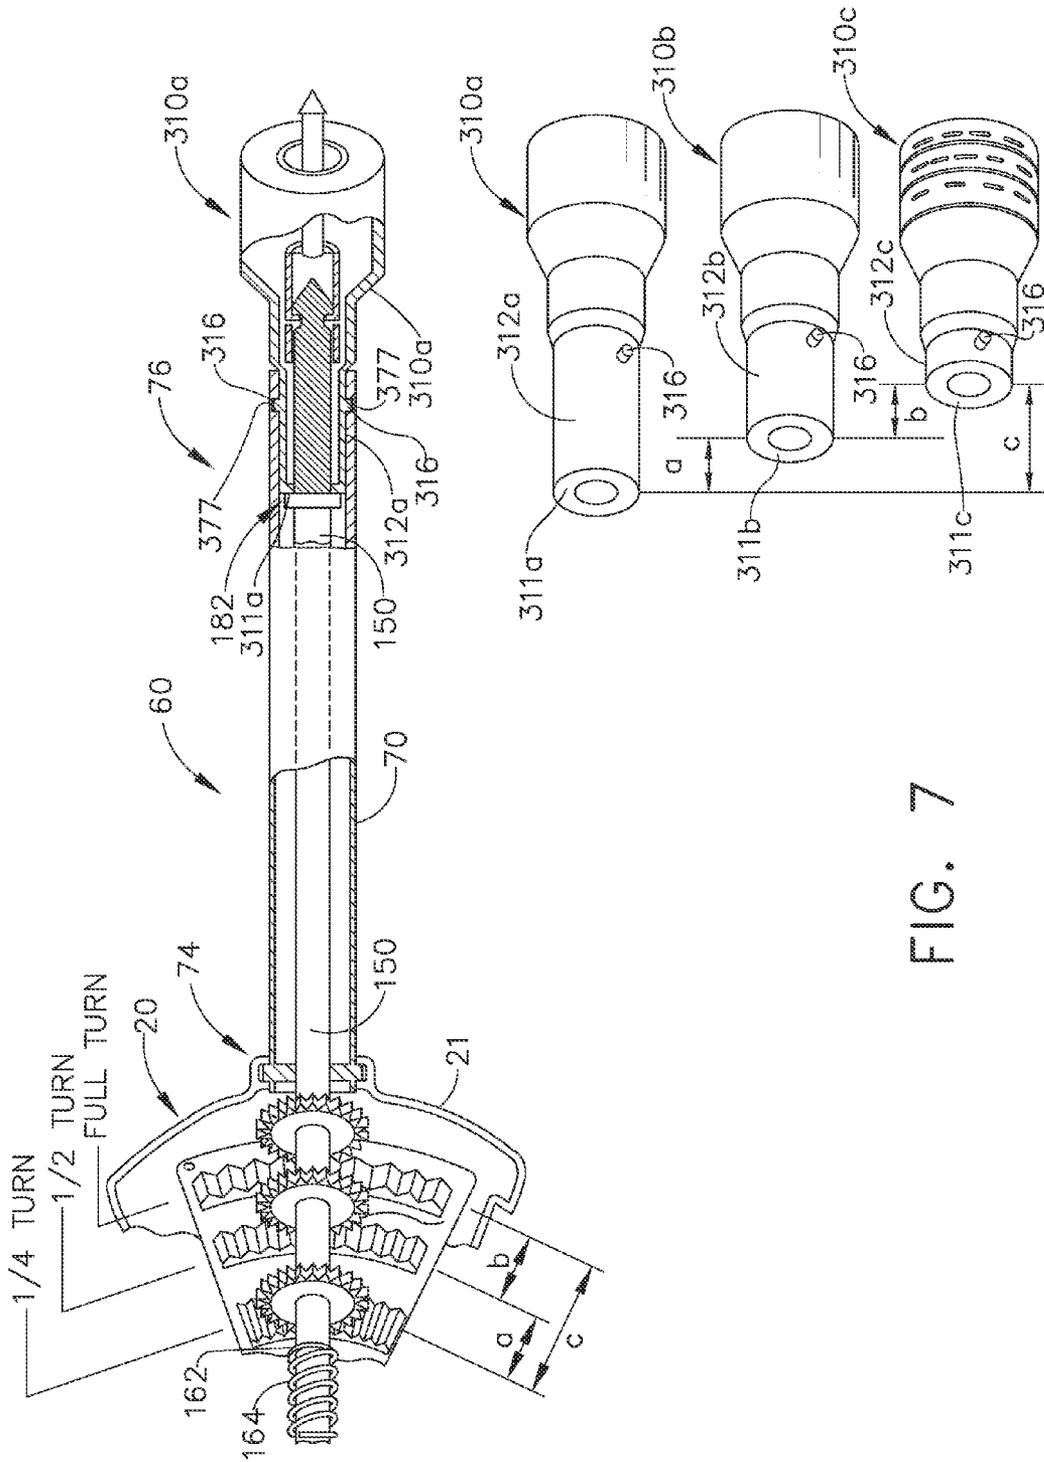


FIG. 7

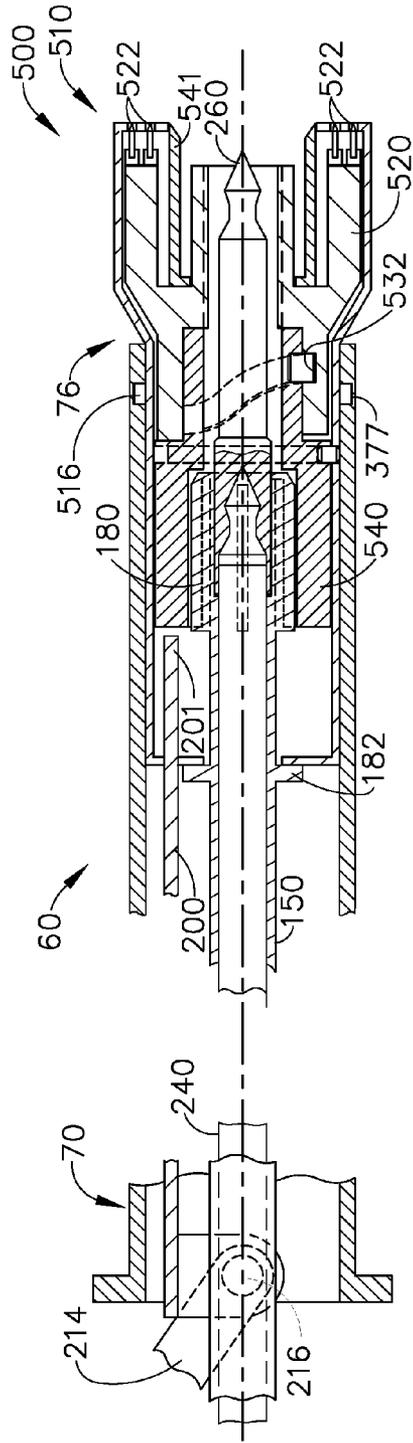


FIG. 9

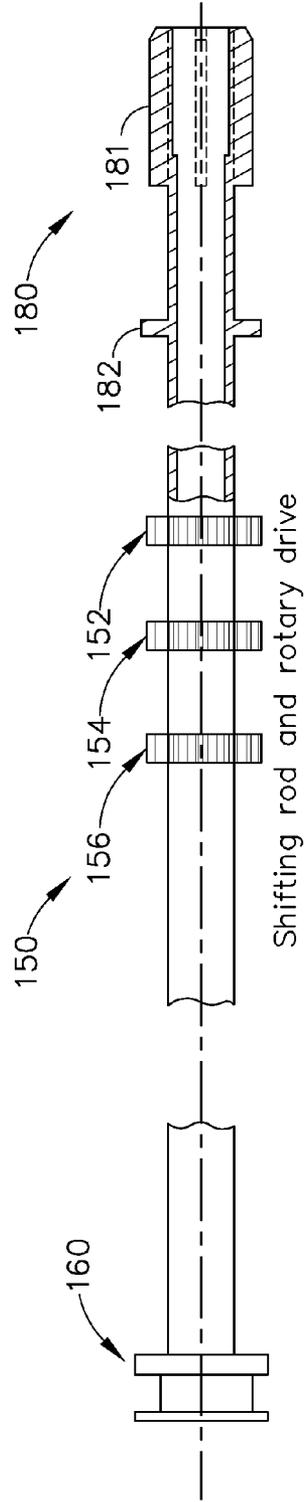


FIG. 10

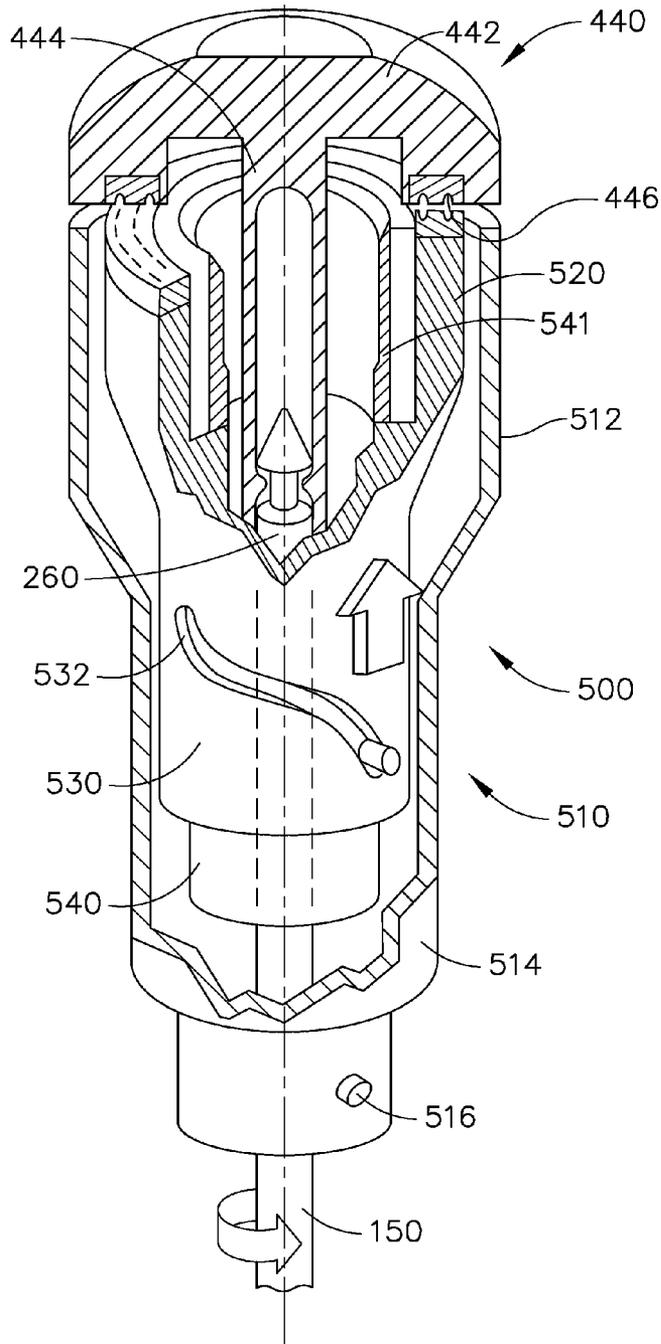


FIG. 11

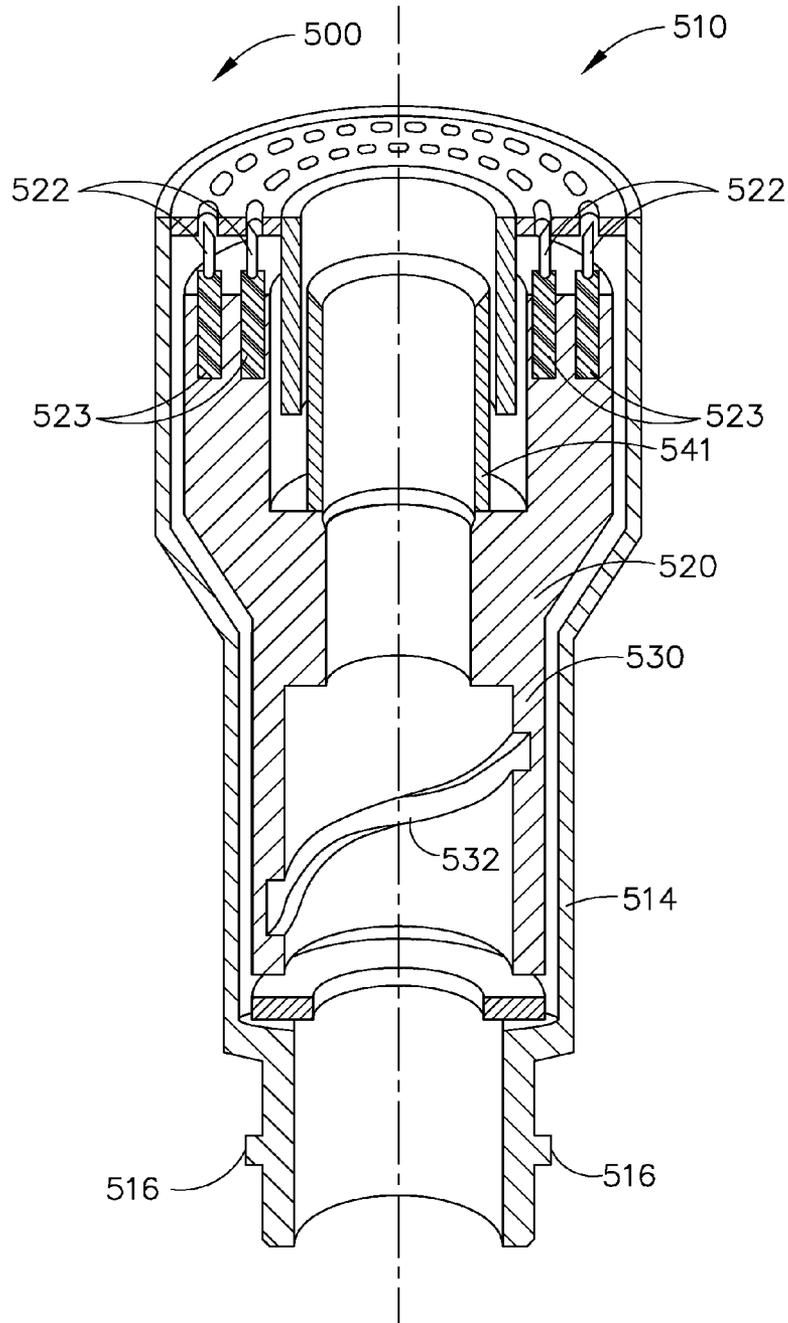


FIG. 12

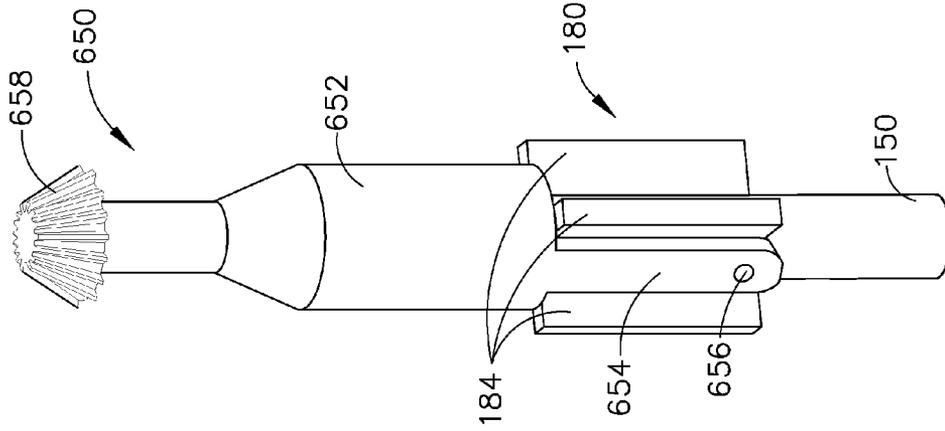


FIG. 15

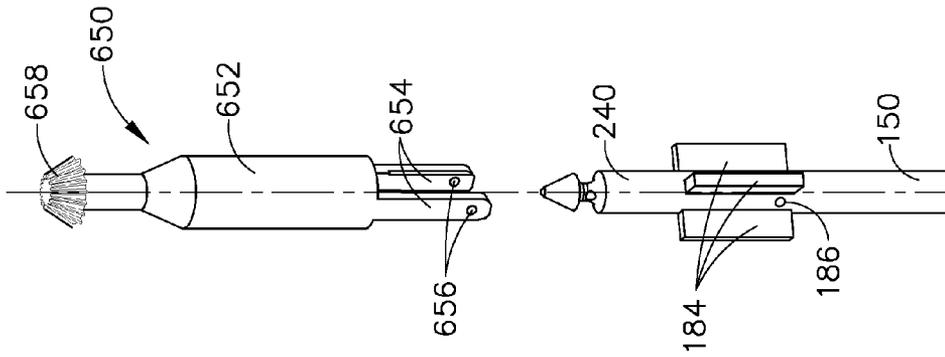


FIG. 14

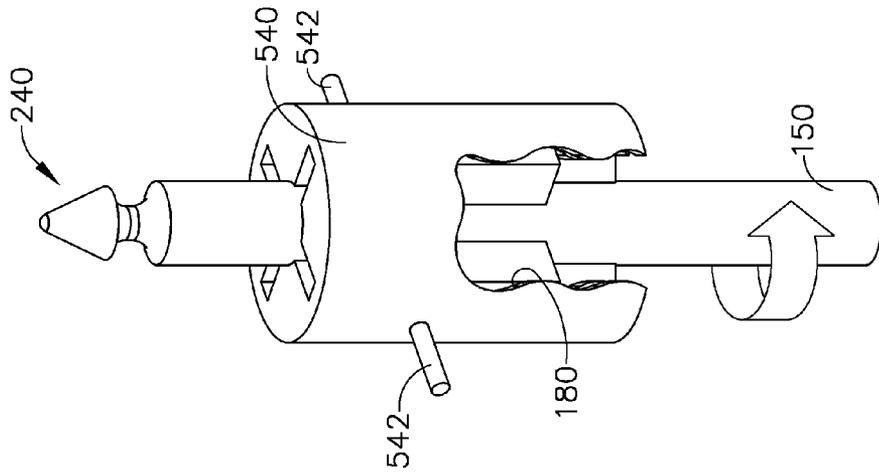


FIG. 13

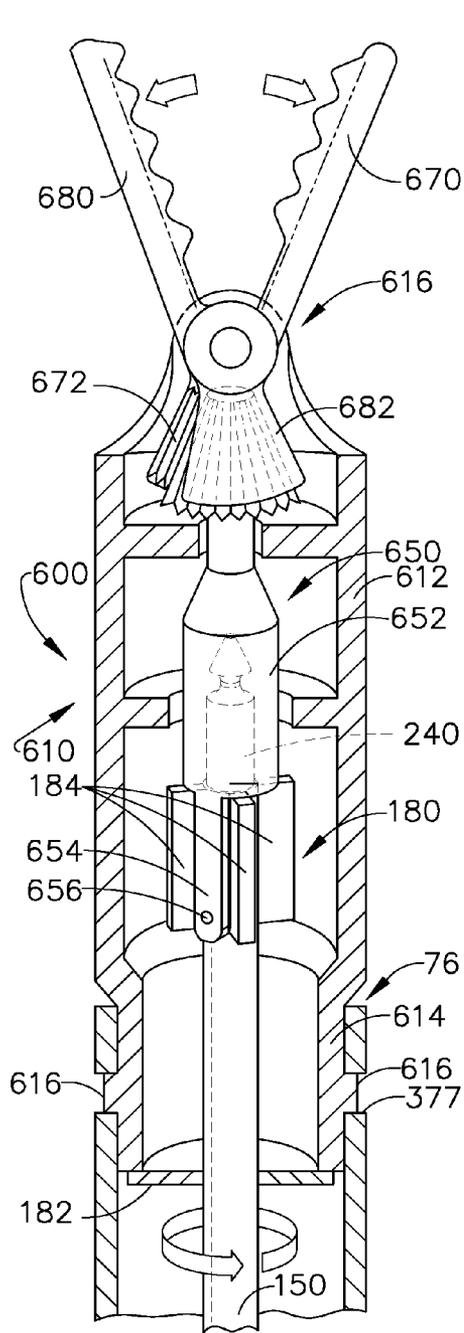


FIG. 16

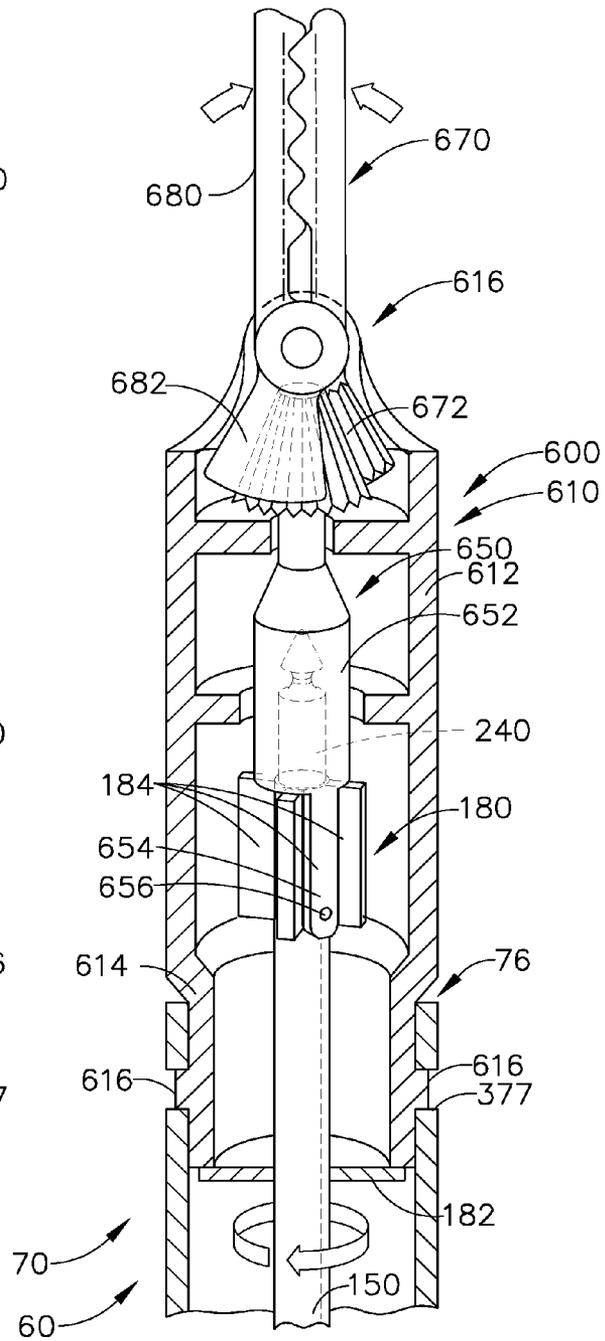


FIG. 17

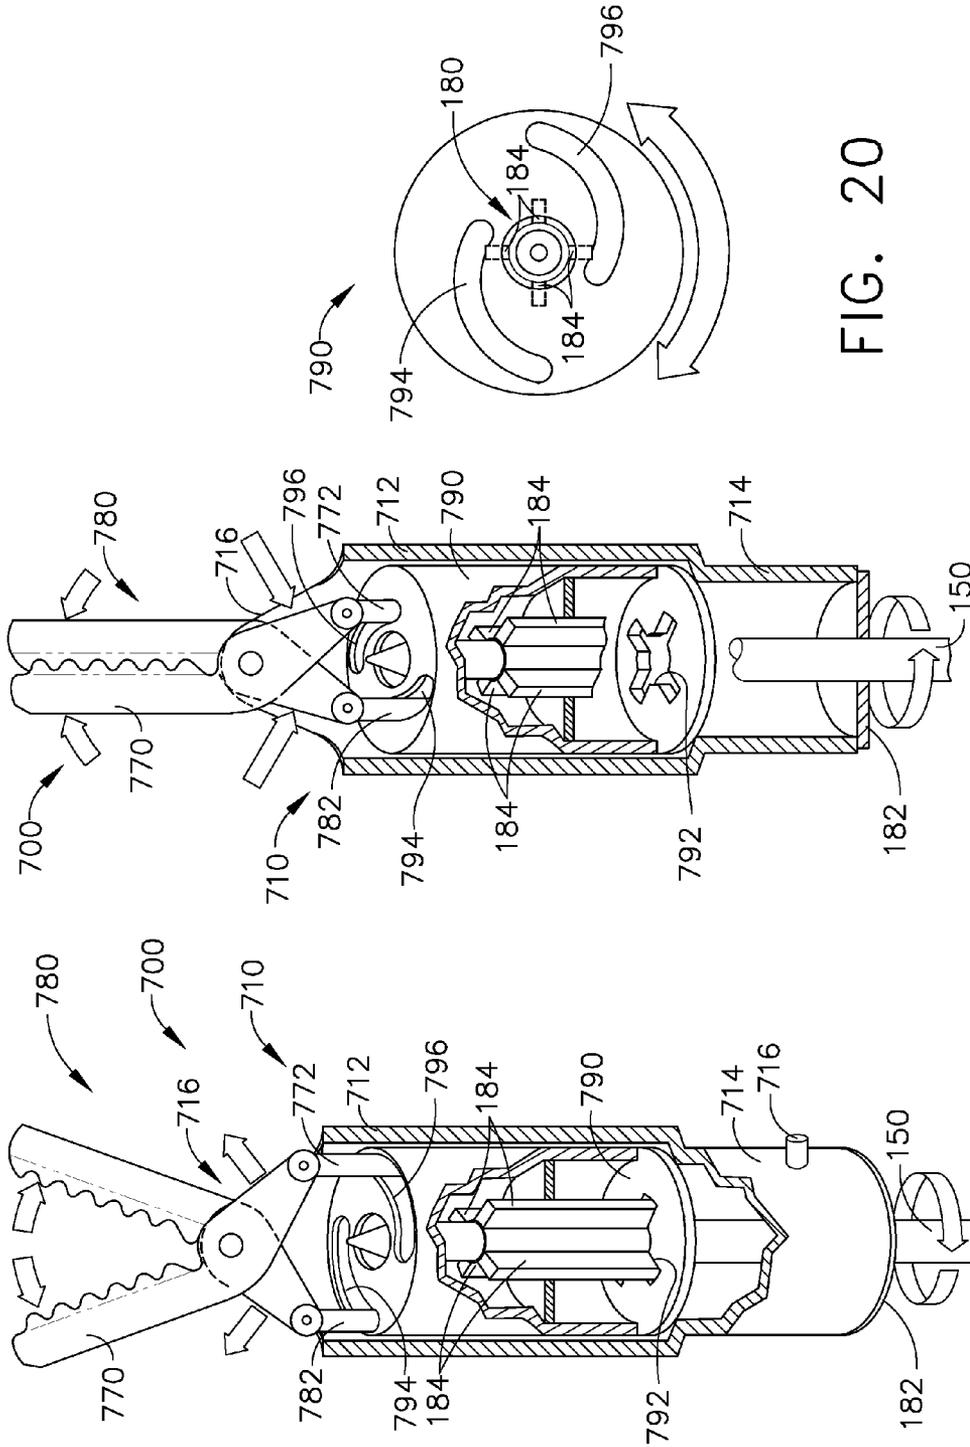


FIG. 20

FIG. 19

FIG. 18

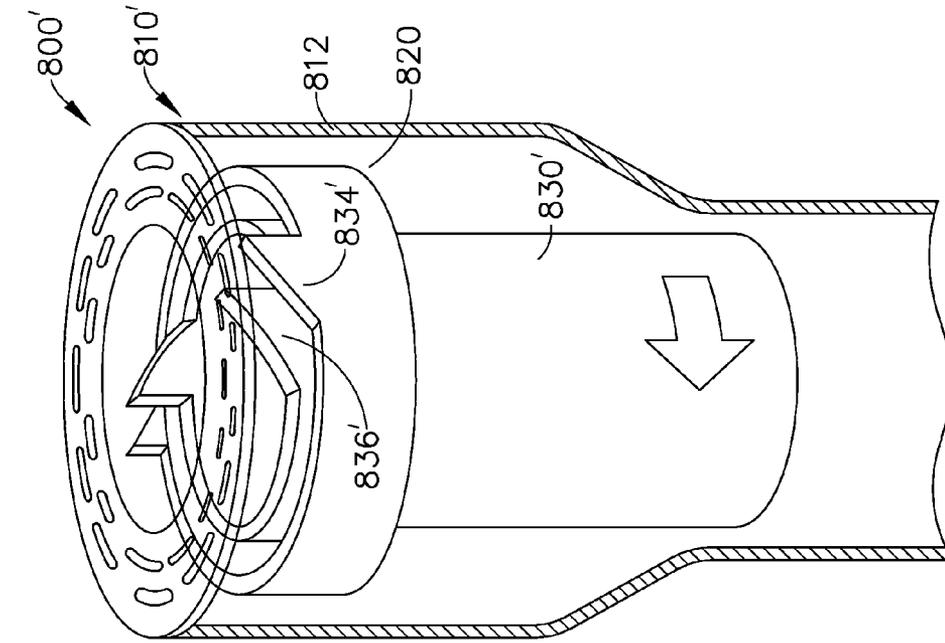


FIG. 21

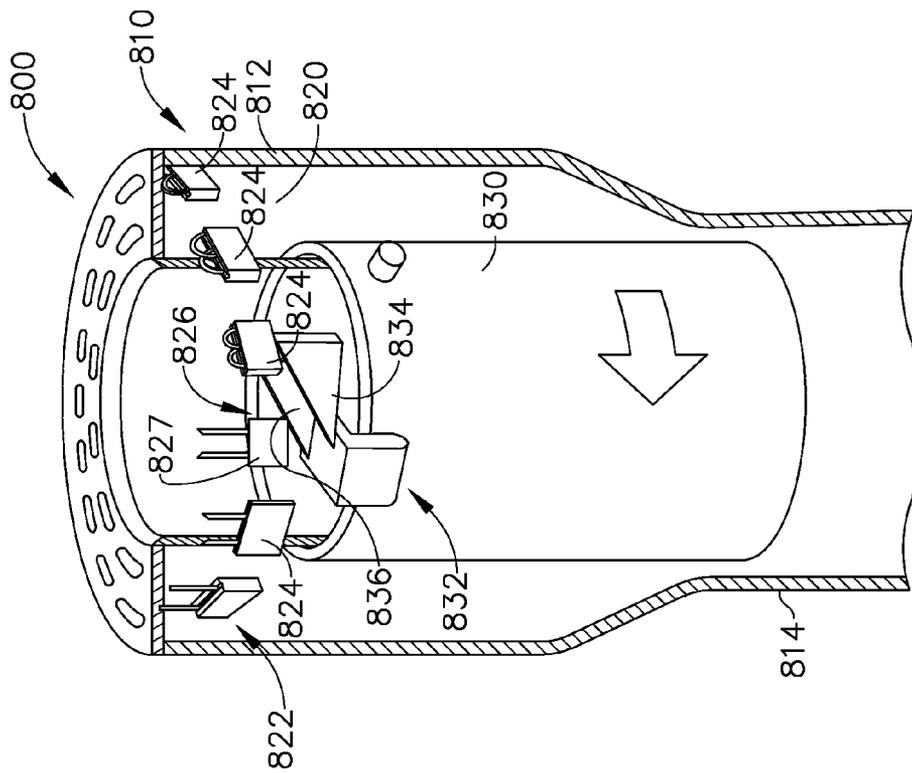


FIG. 22

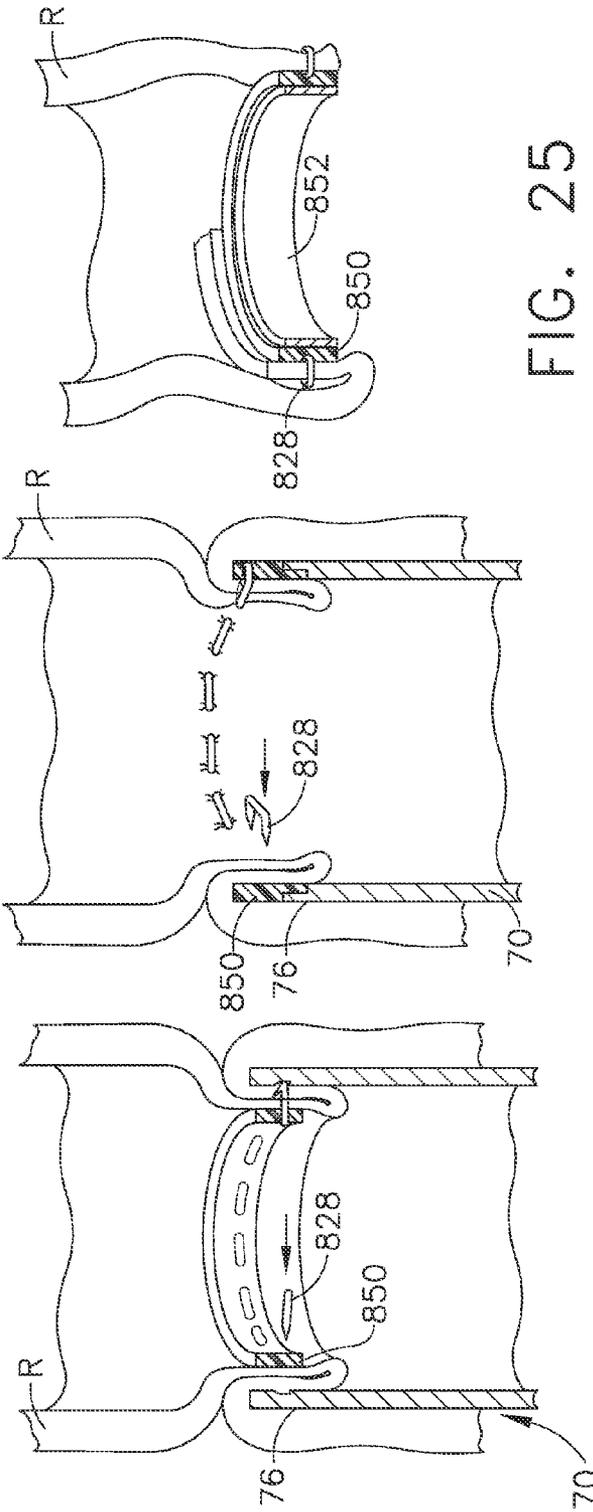


FIG. 23

FIG. 24

FIG. 25

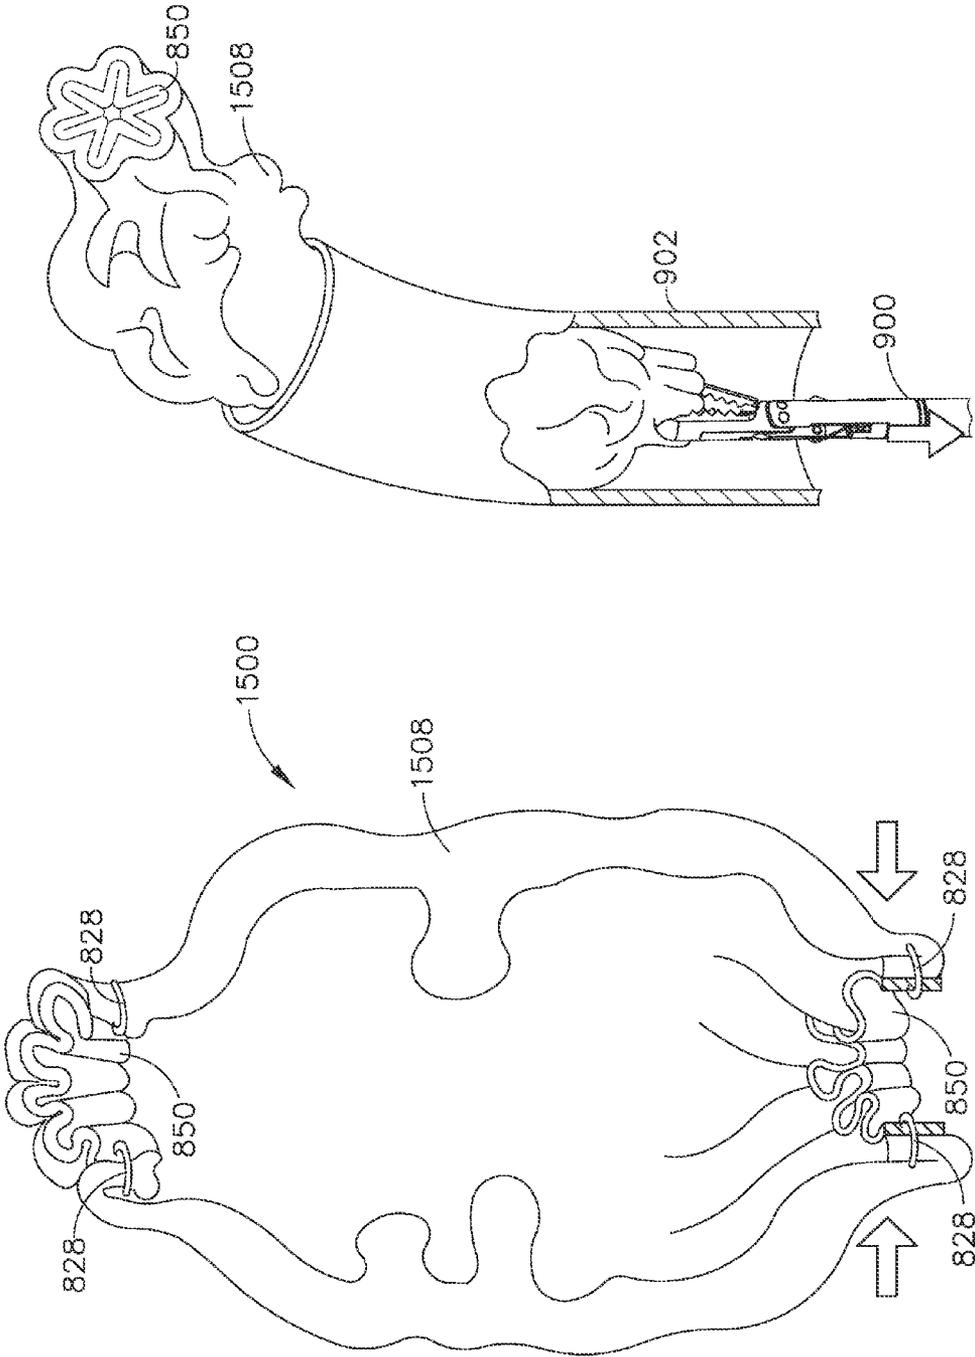


FIG. 27

FIG. 26

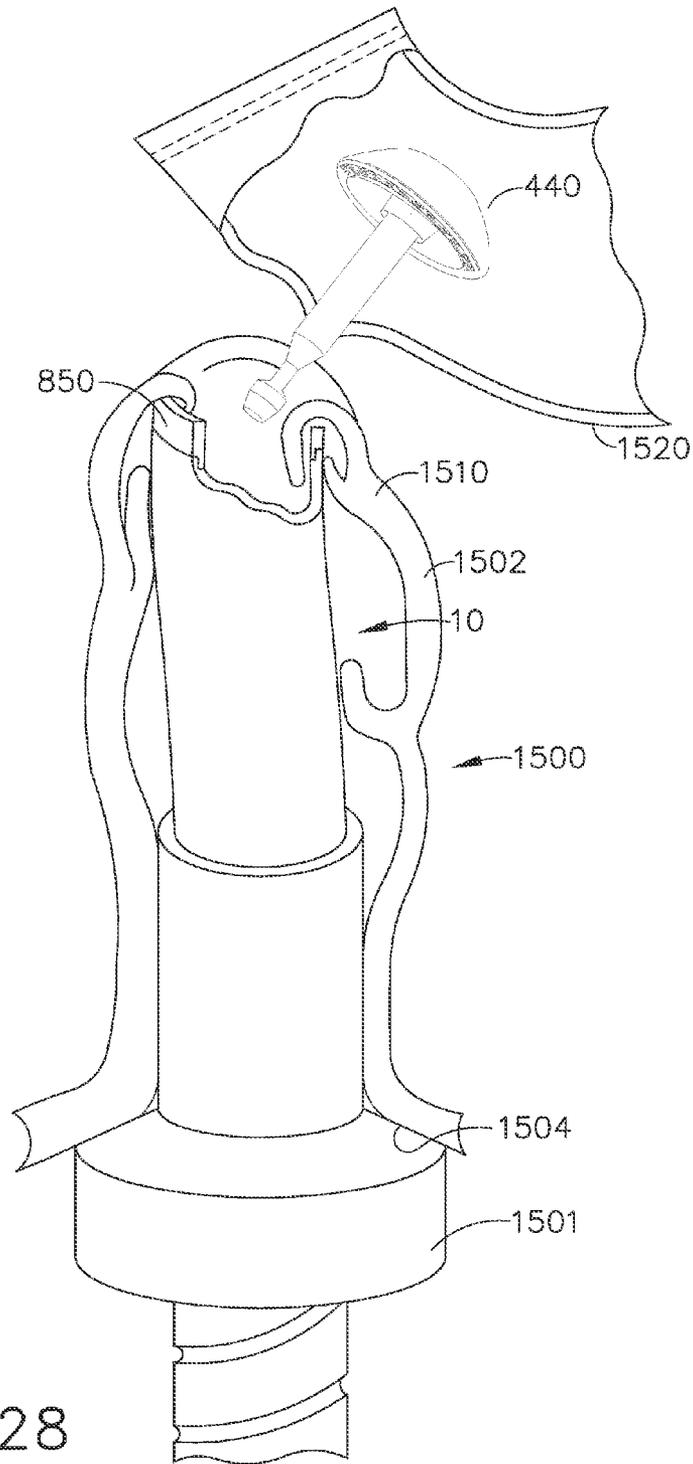
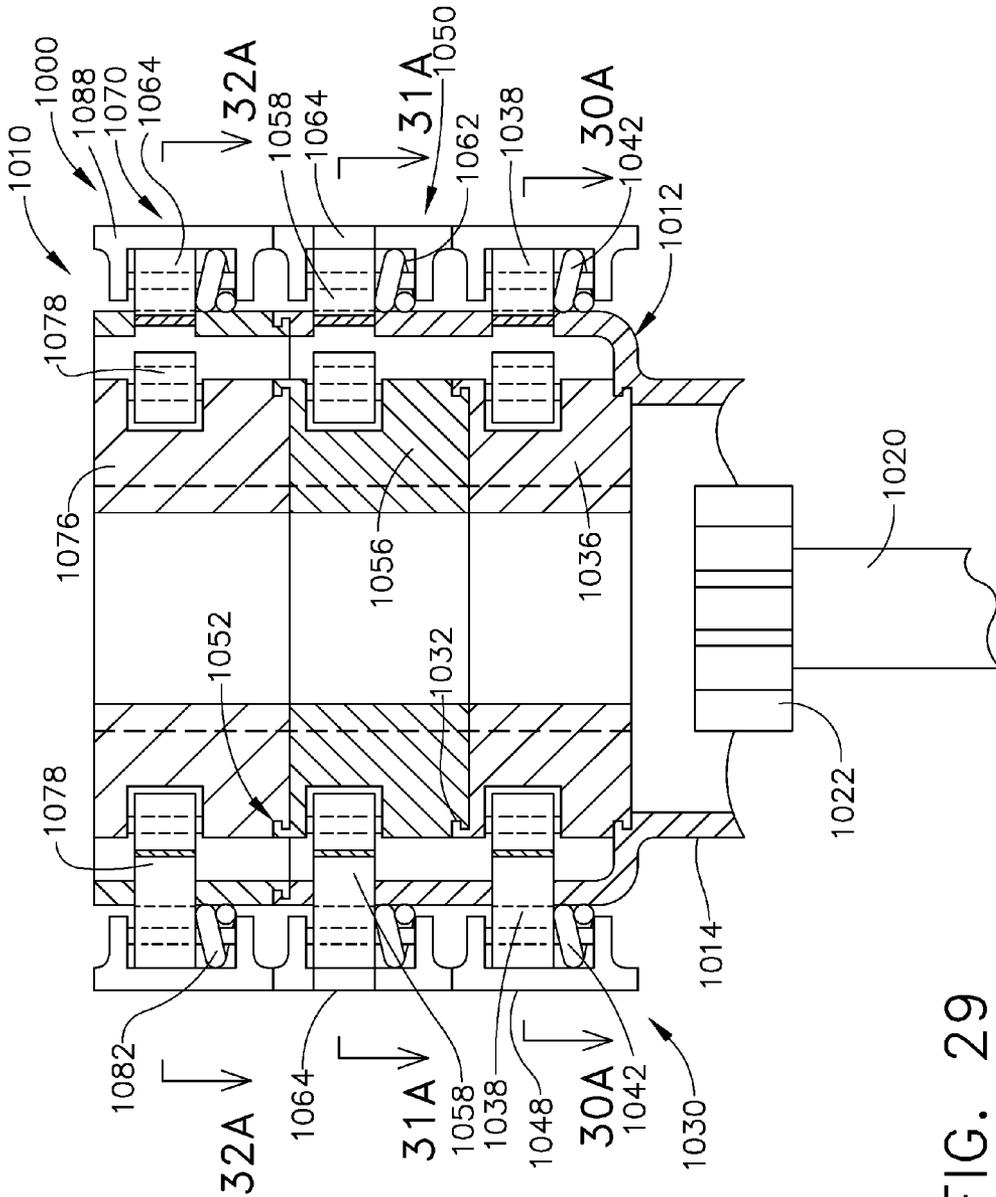


FIG. 28



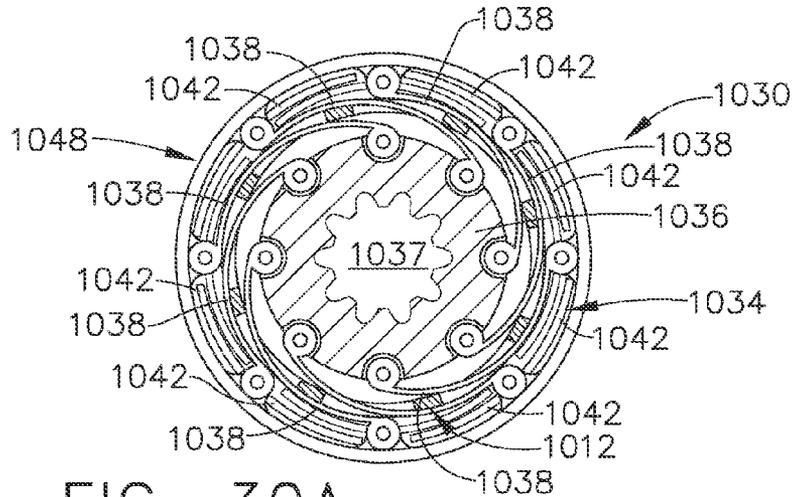


FIG. 30A

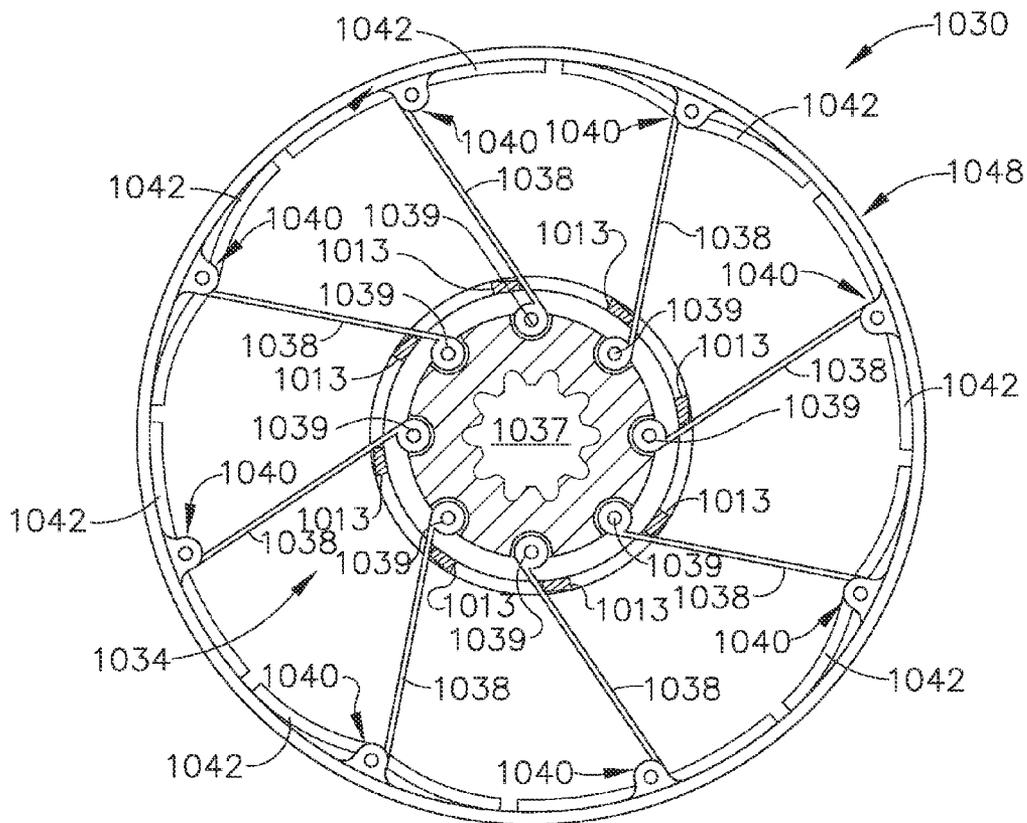


FIG. 30B

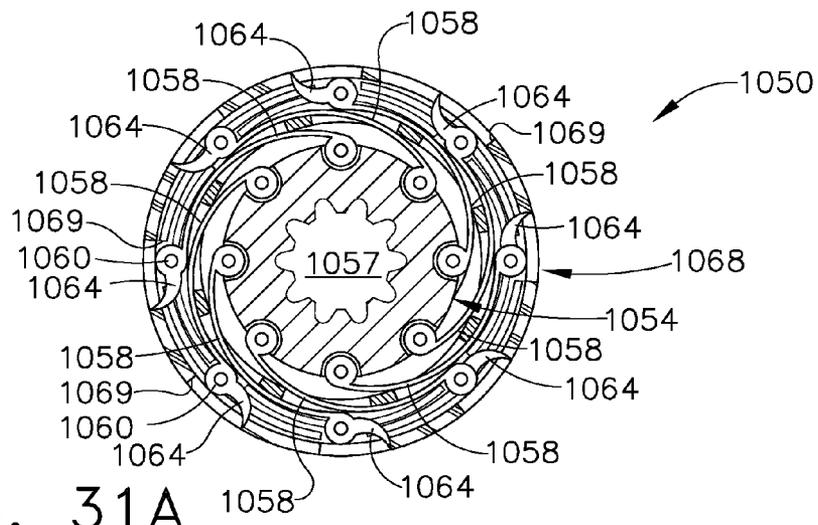


FIG. 31A

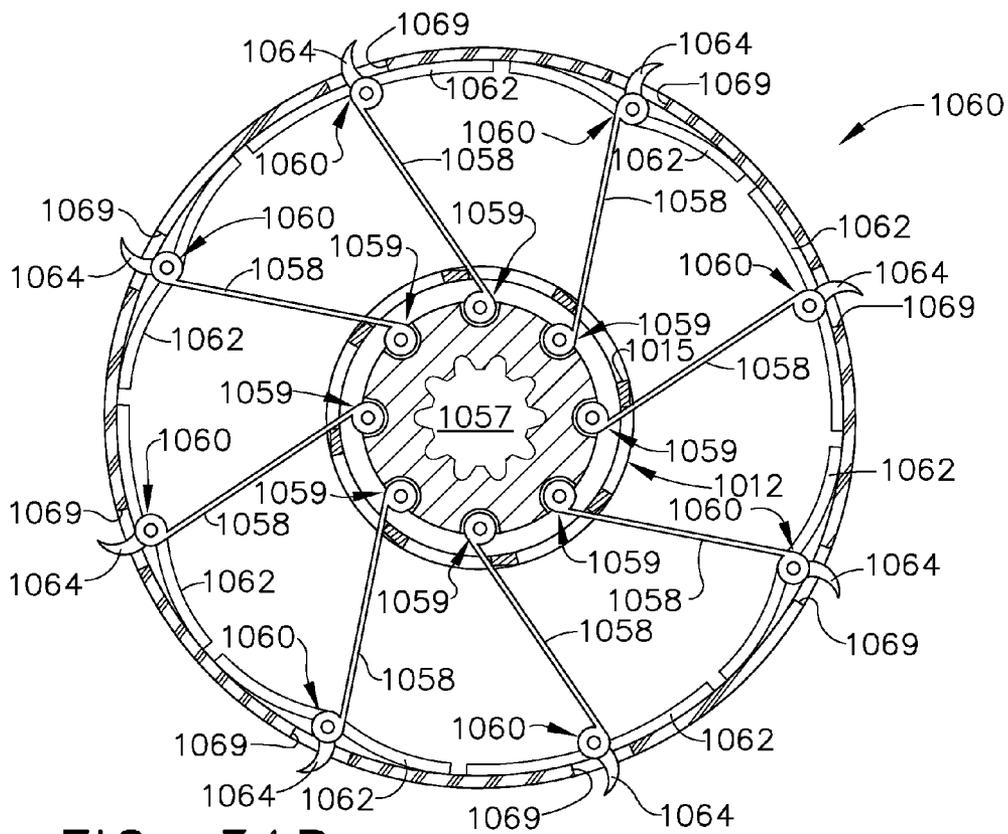


FIG. 31B

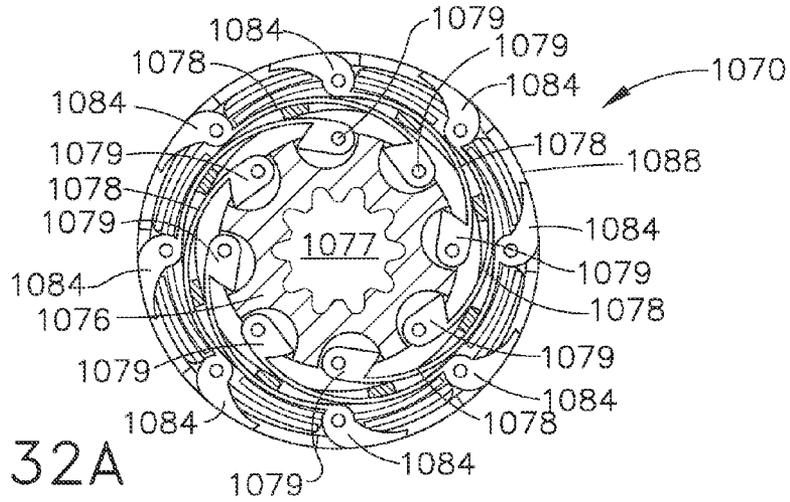


FIG. 32A

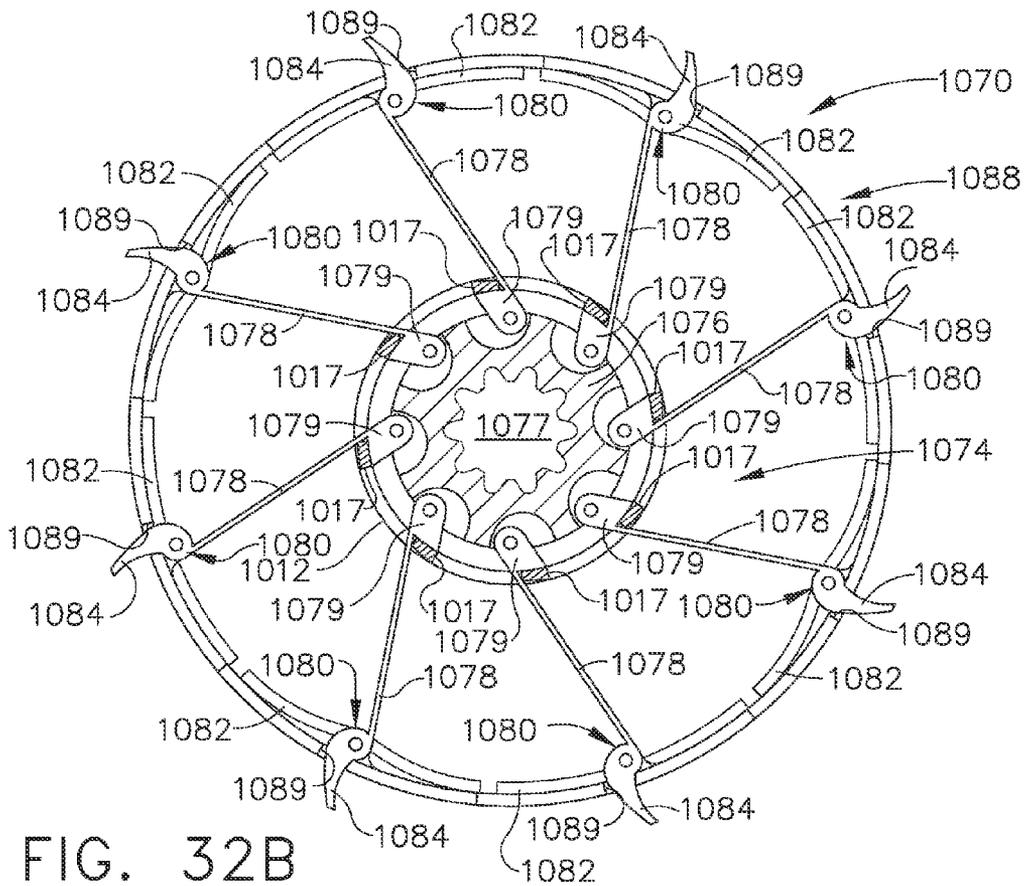


FIG. 32B

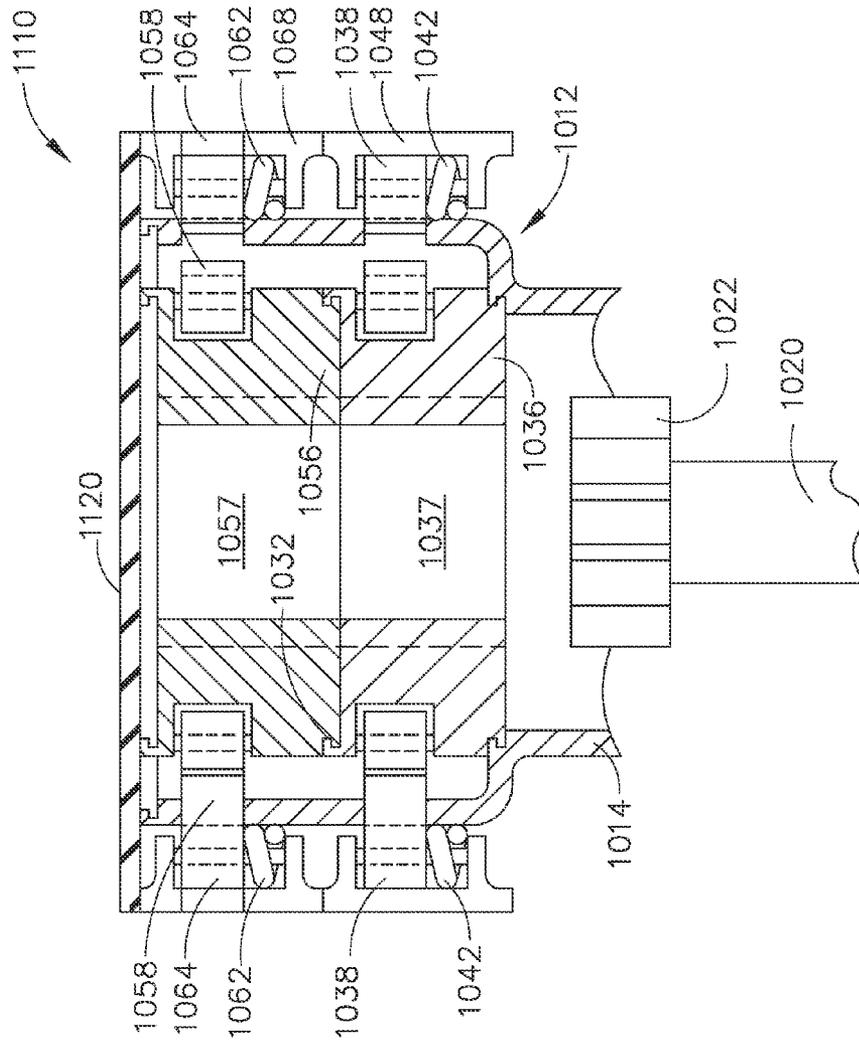


FIG. 33

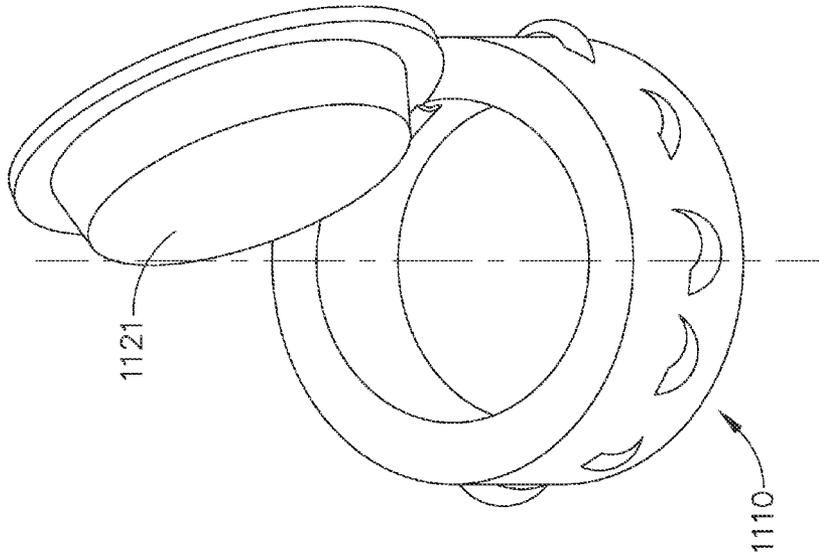


FIG. 33B

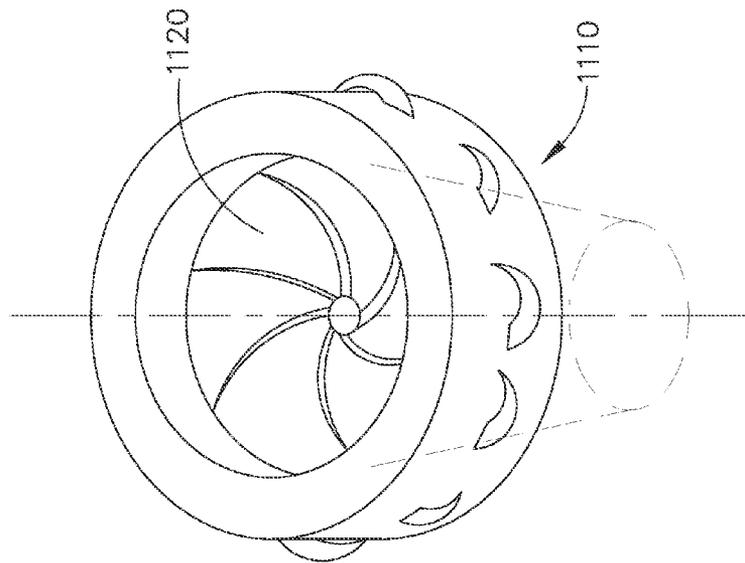
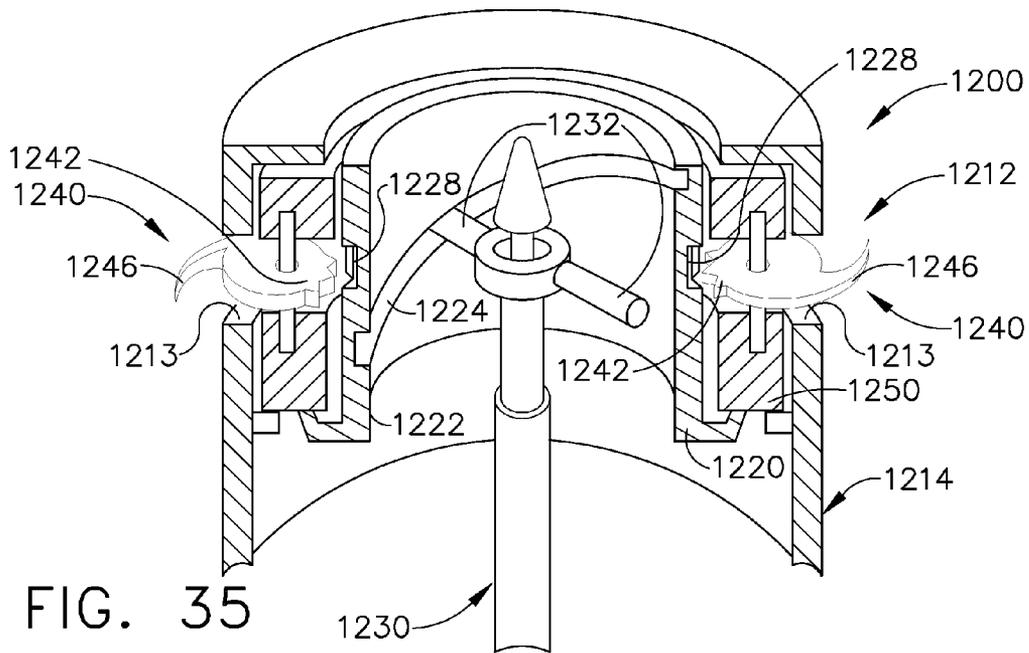
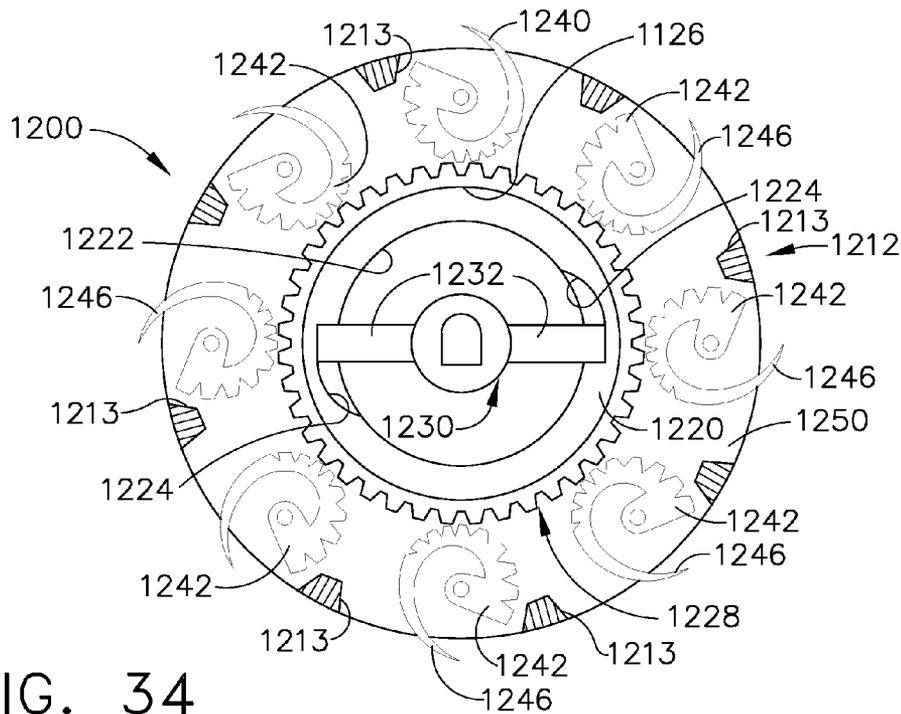


FIG. 33A



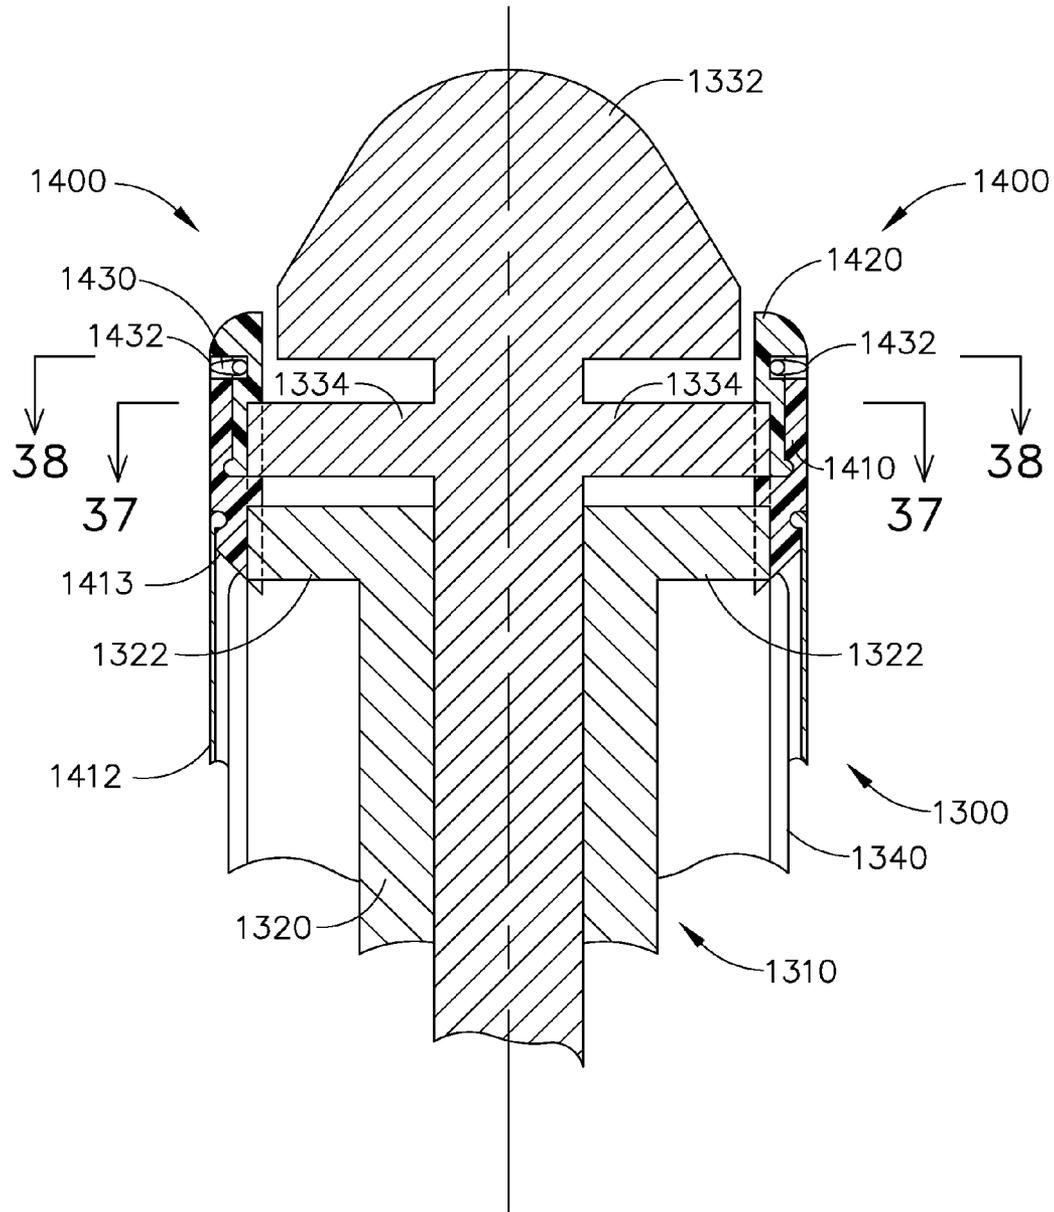


FIG. 36

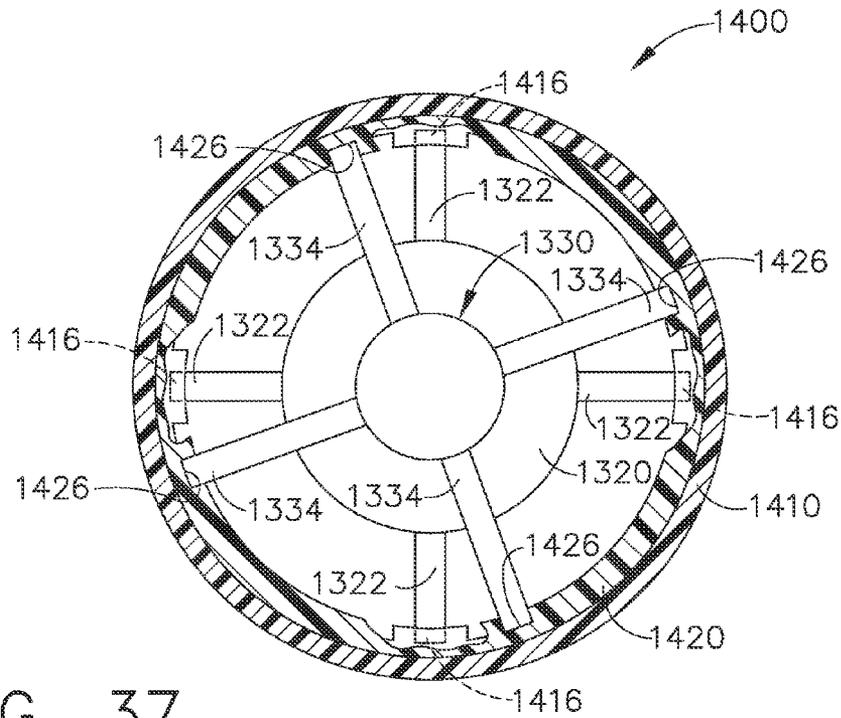


FIG. 37

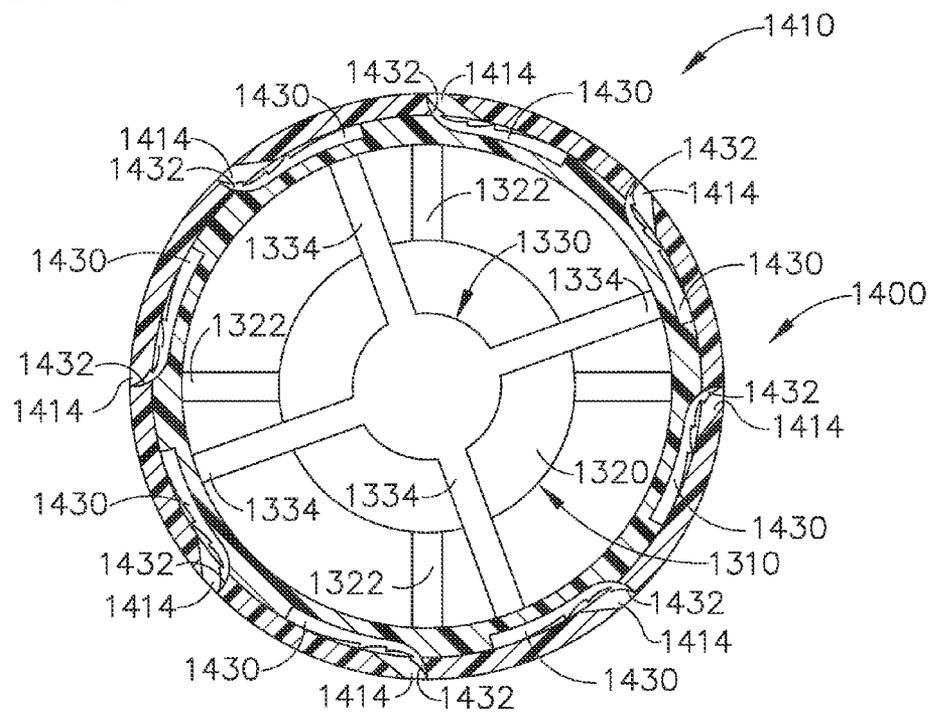


FIG. 38

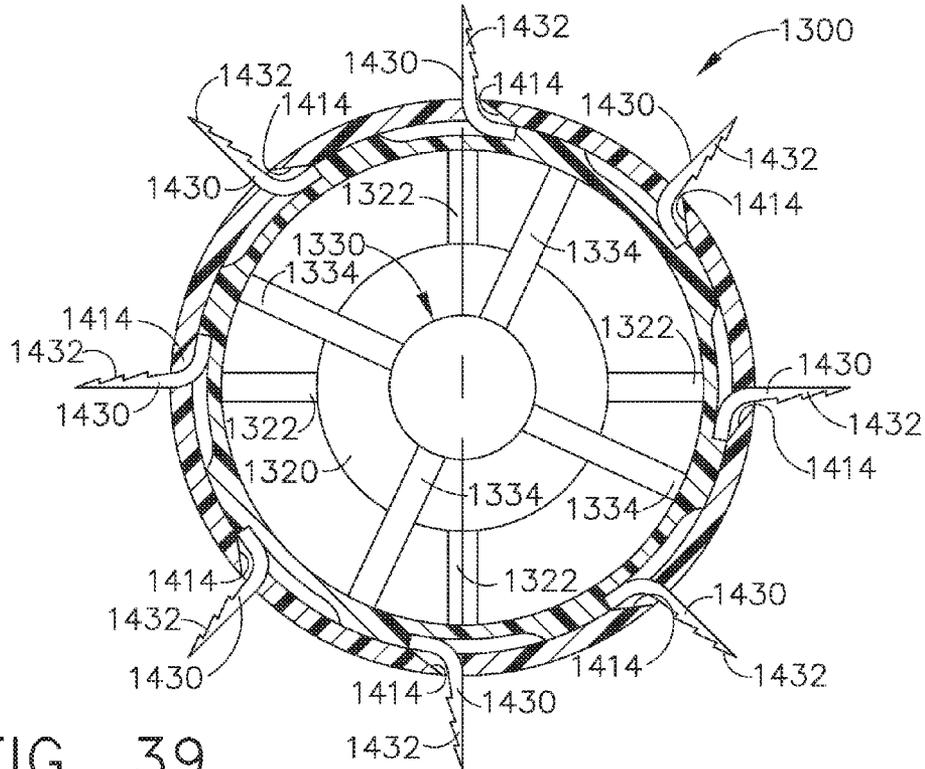


FIG. 39

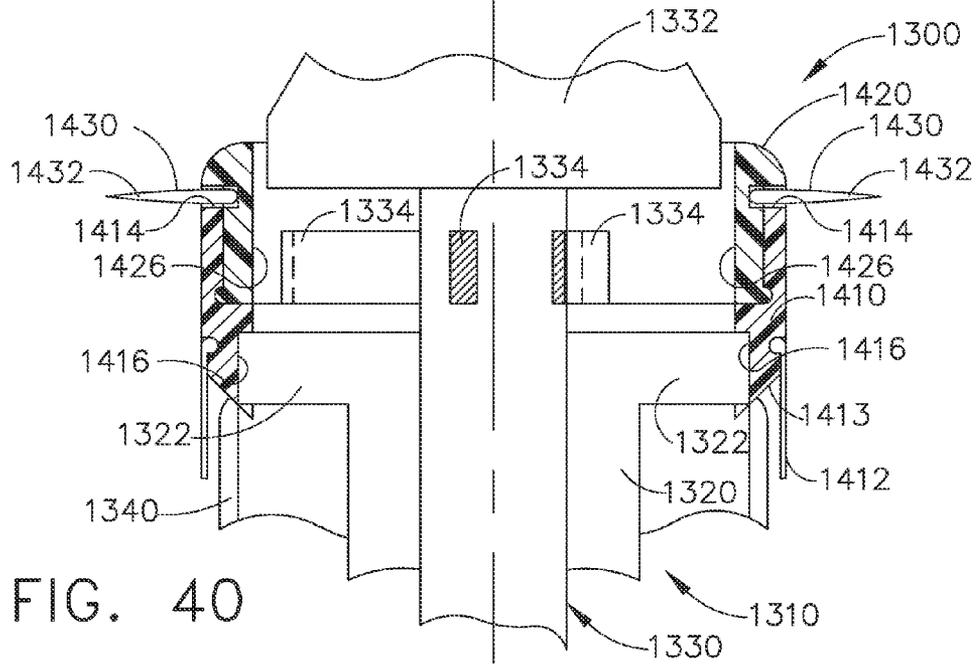


FIG. 40

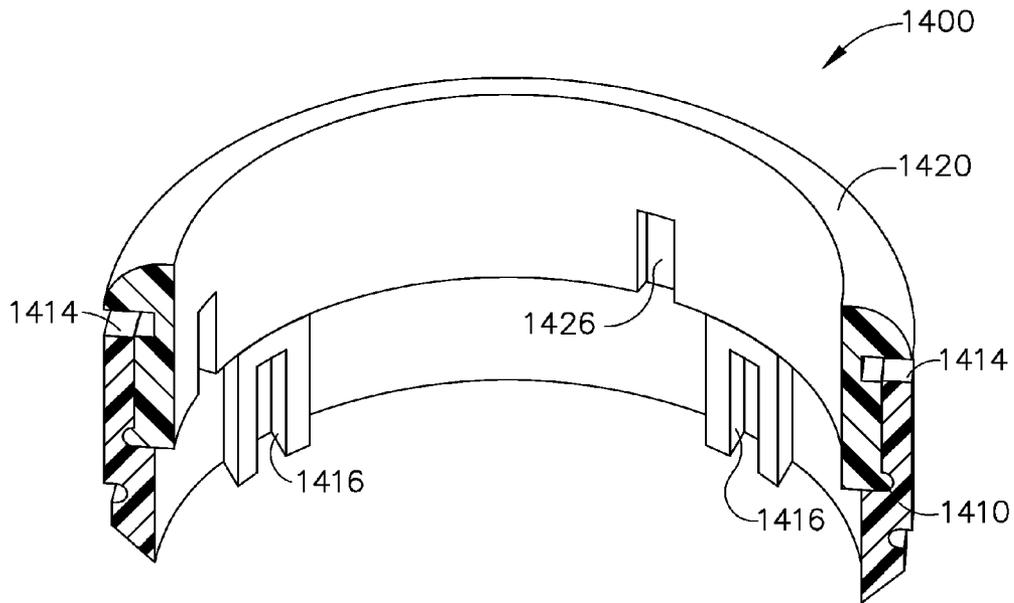


FIG. 41A

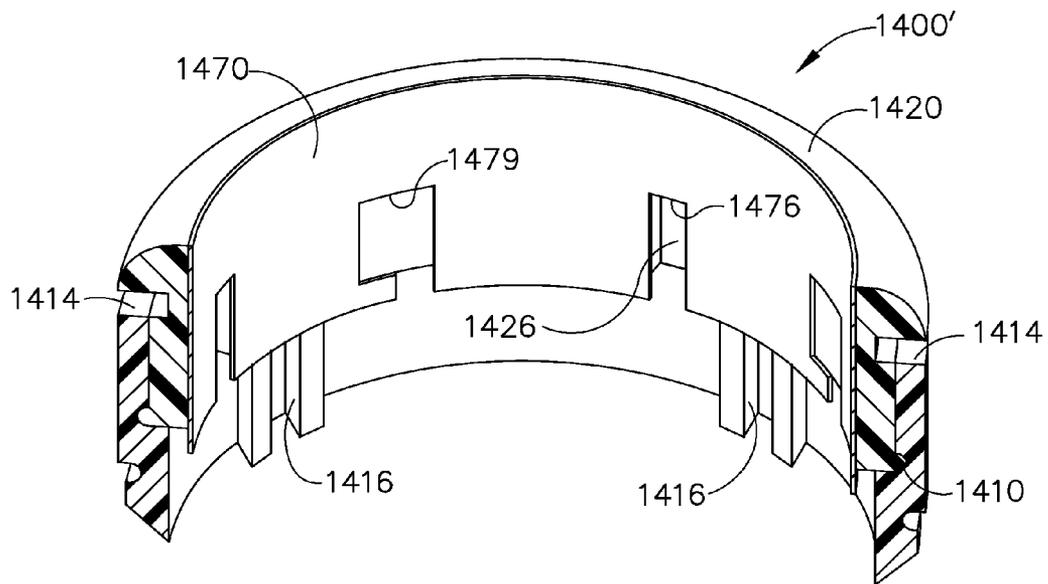


FIG. 41B

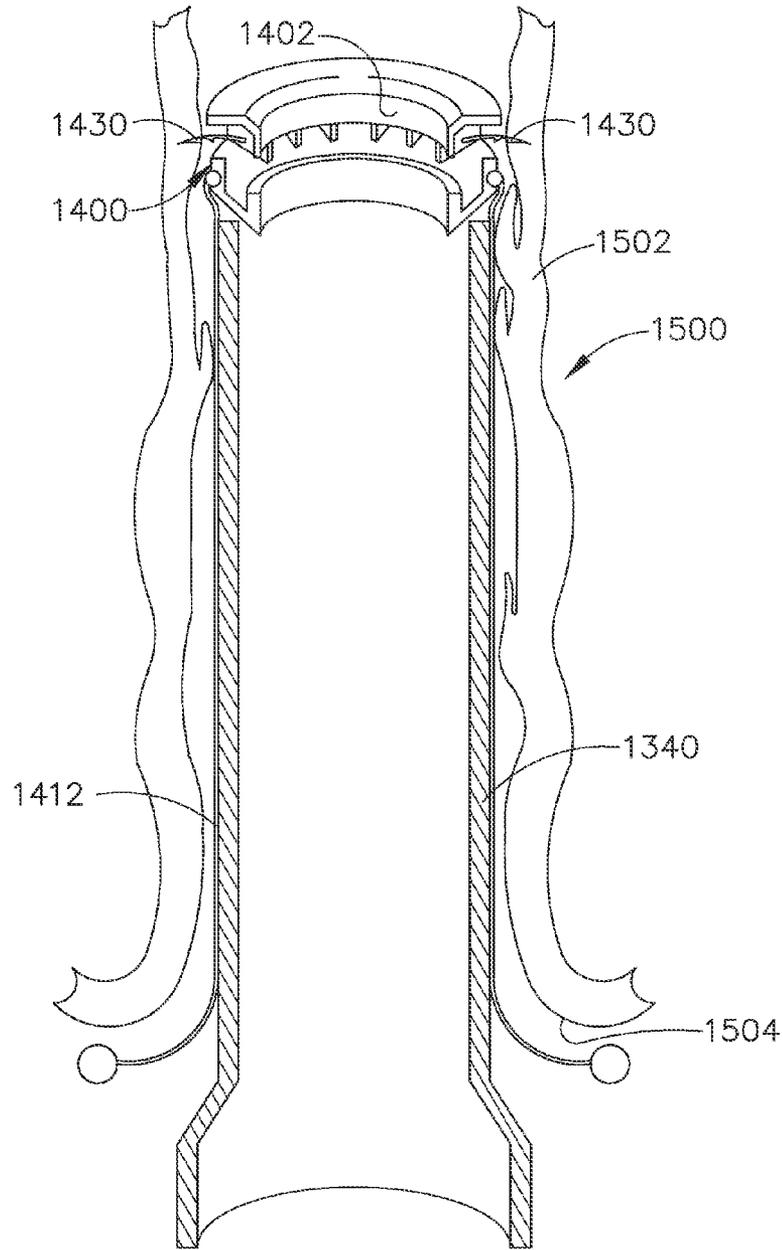


FIG. 42

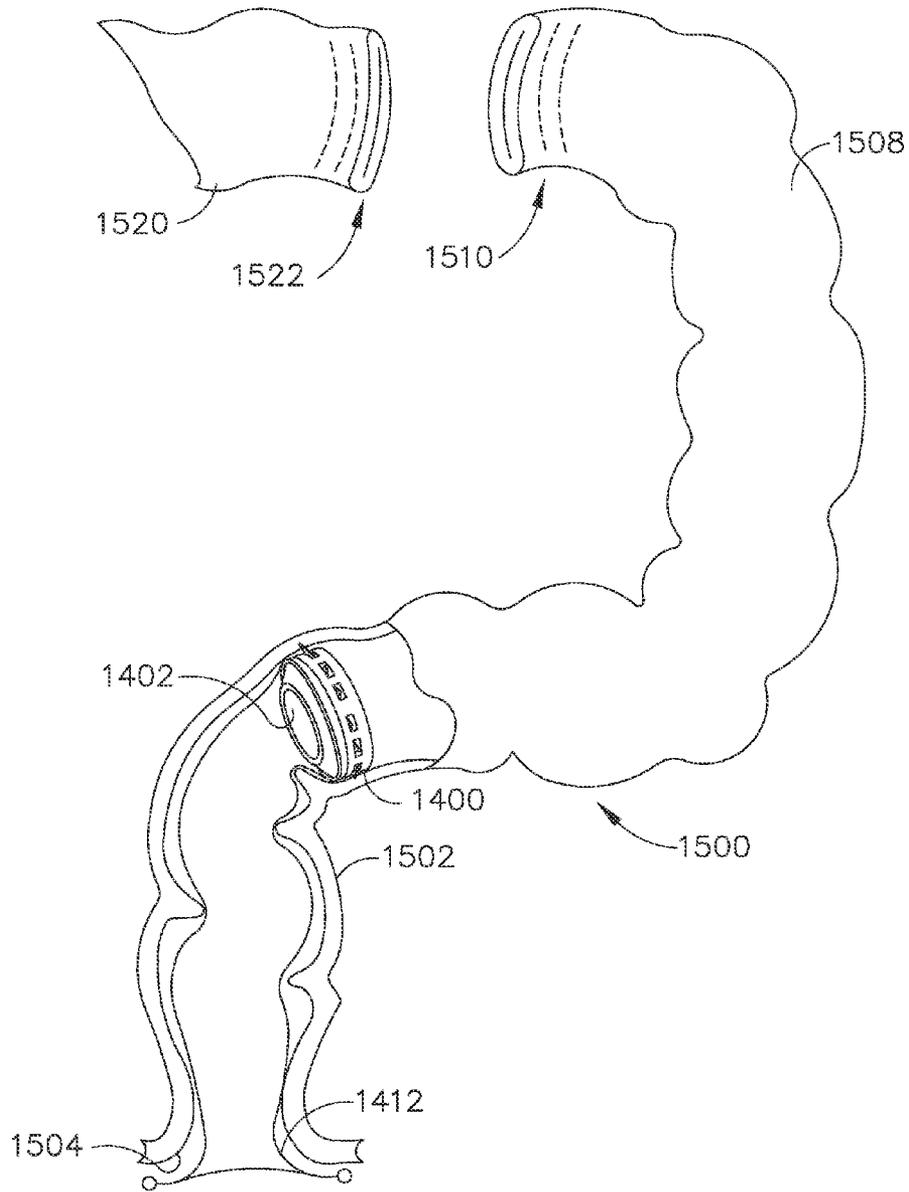


FIG. 43

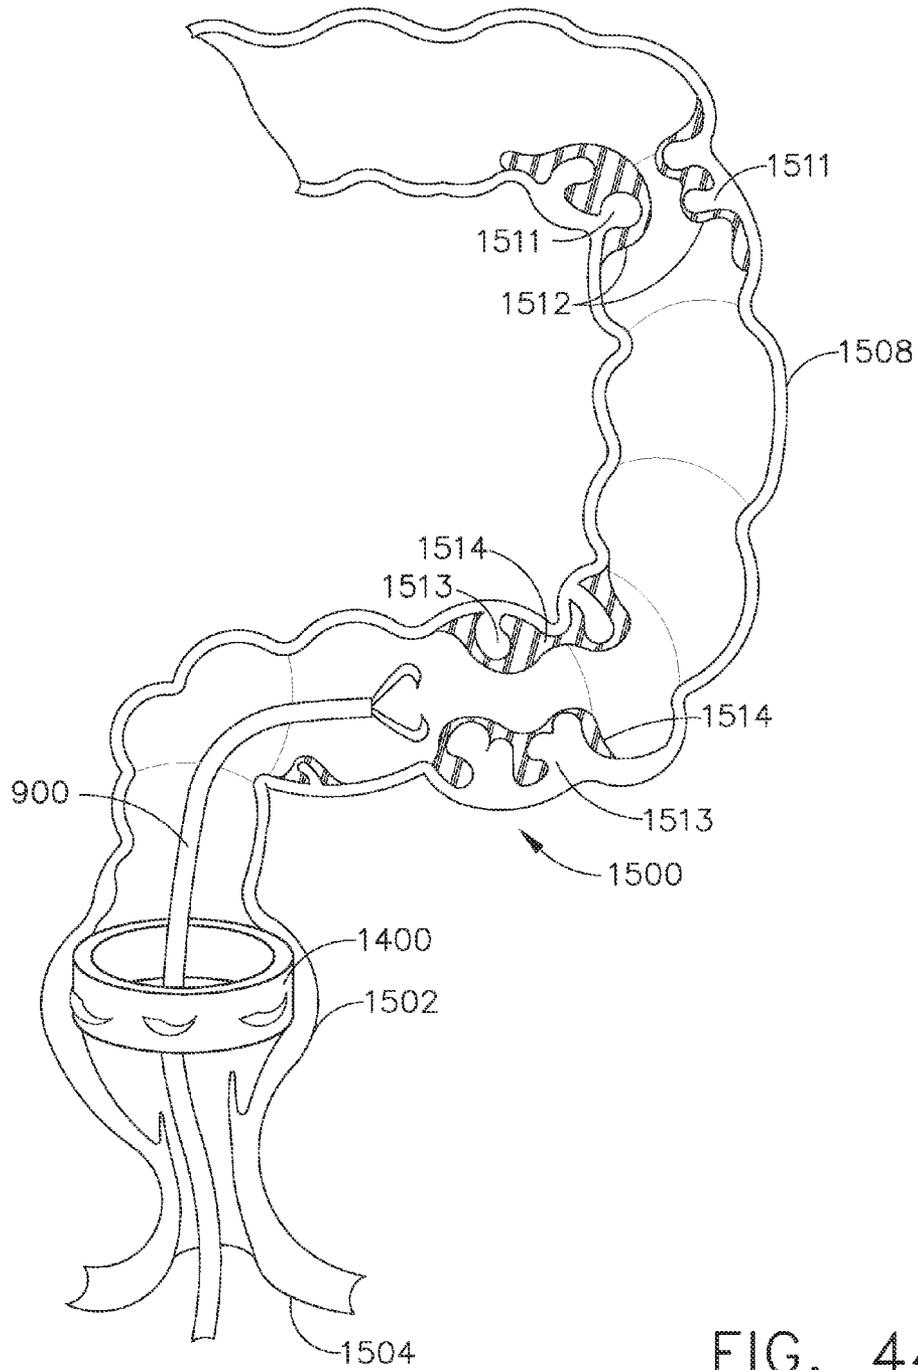


FIG. 44

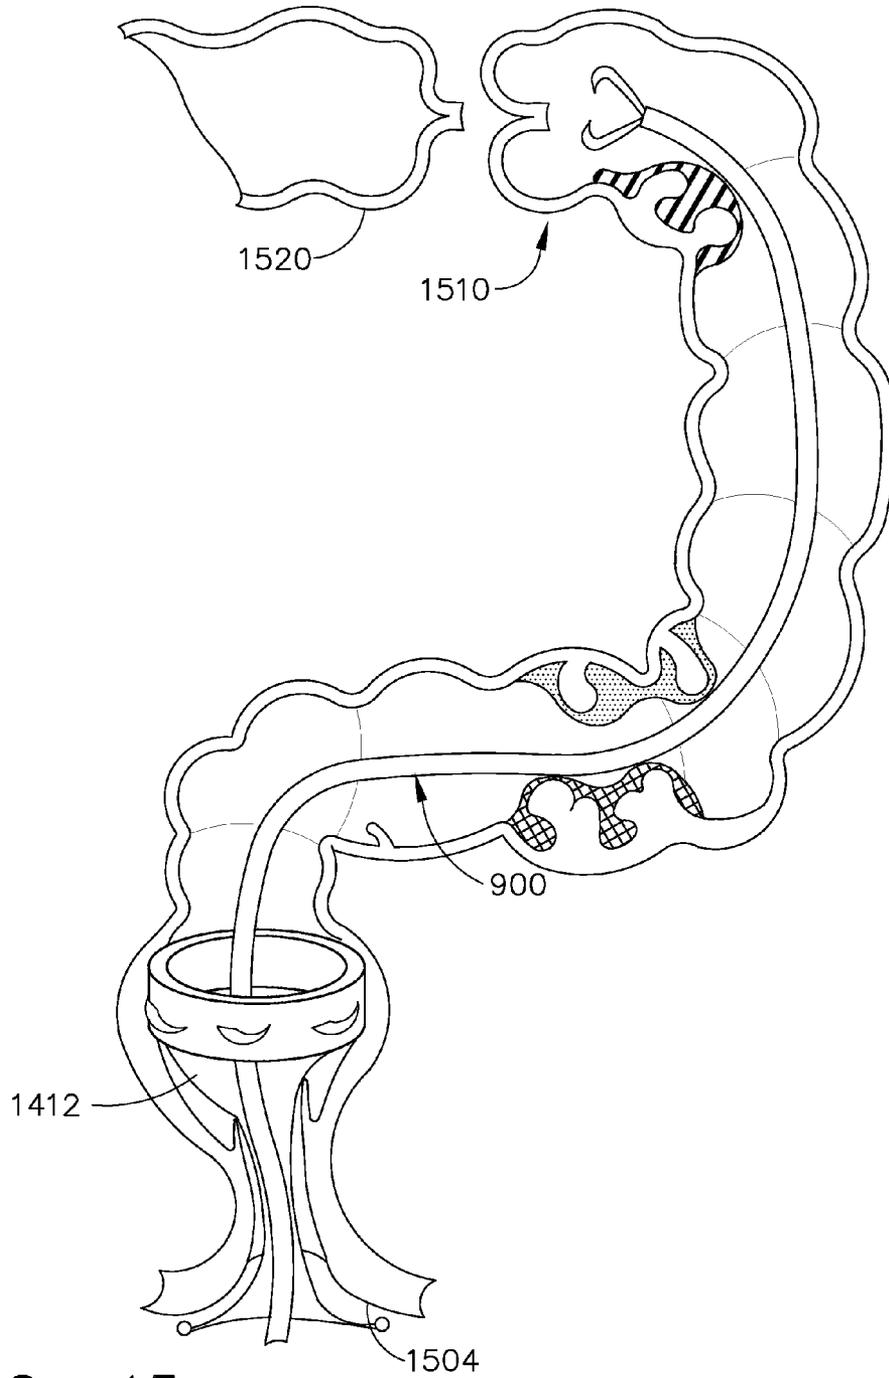


FIG. 45

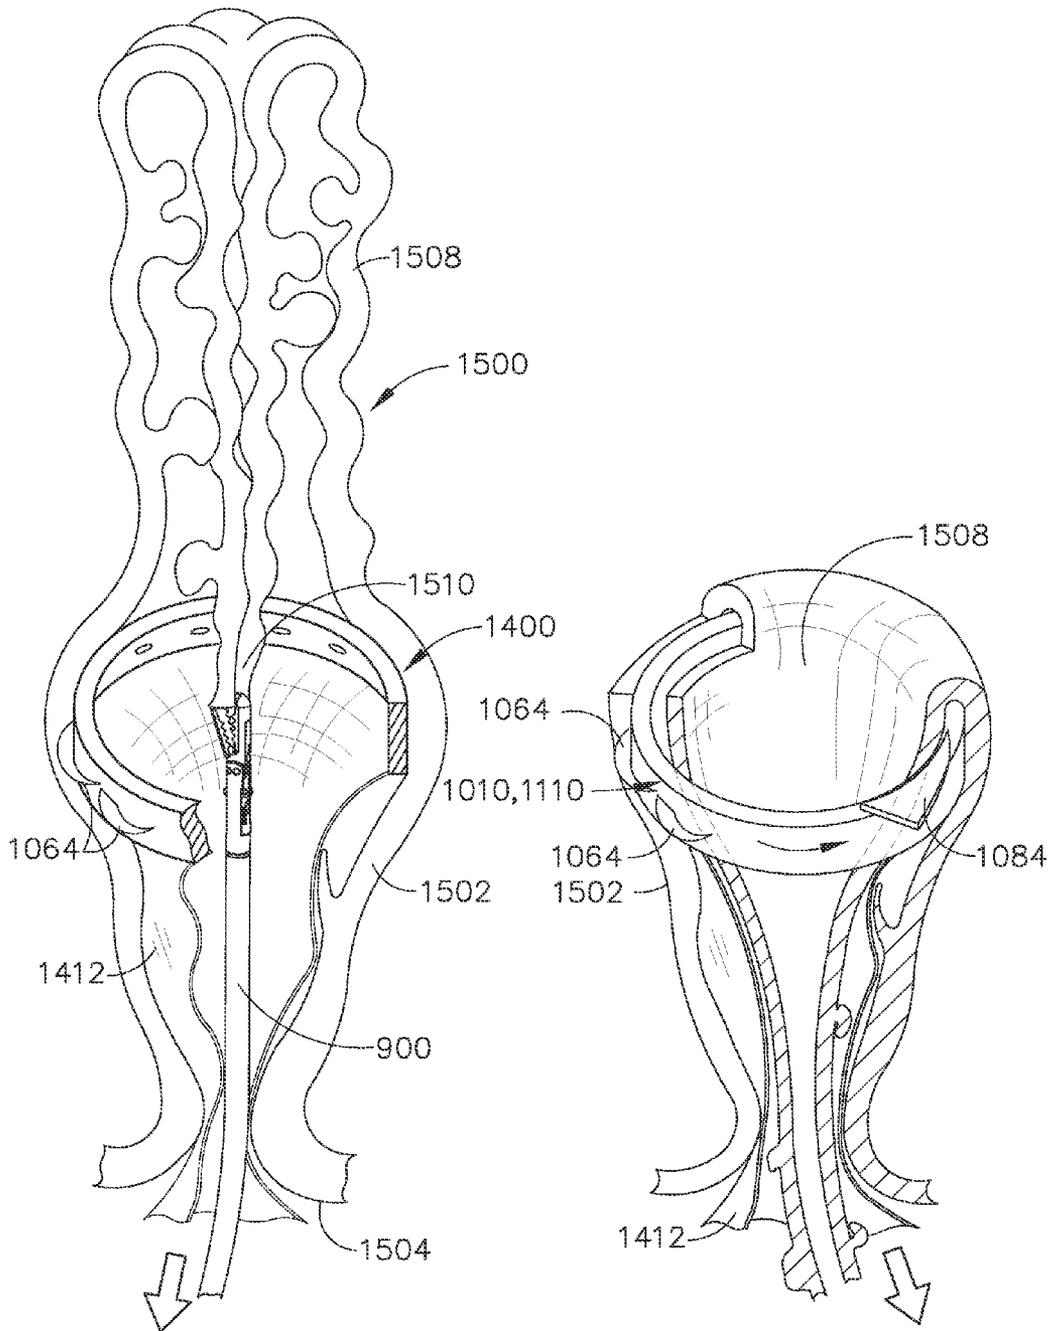


FIG. 46

FIG. 47

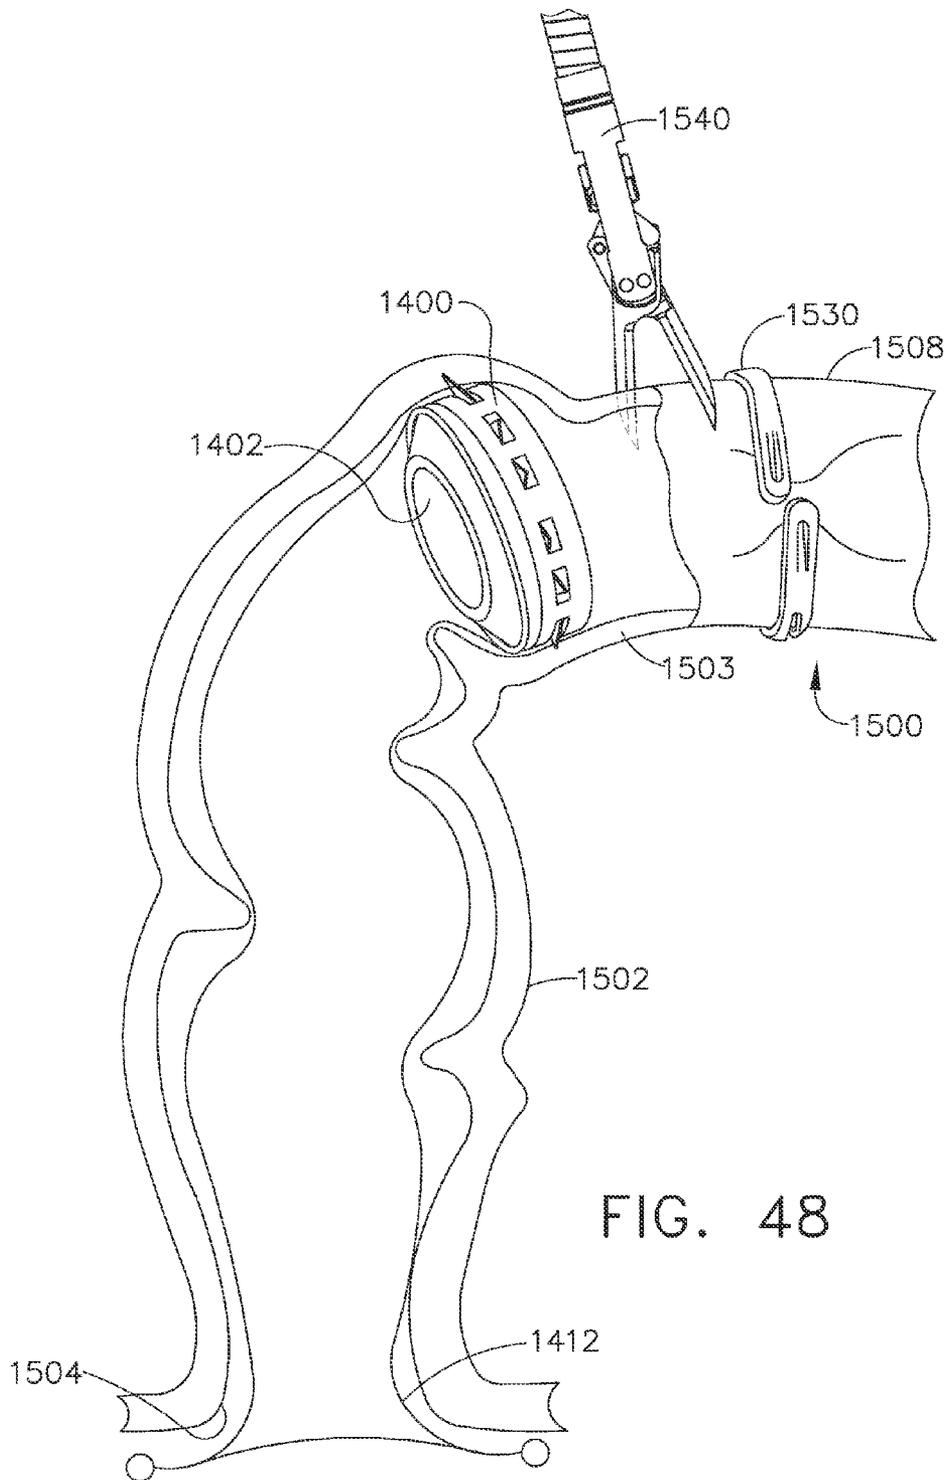


FIG. 48

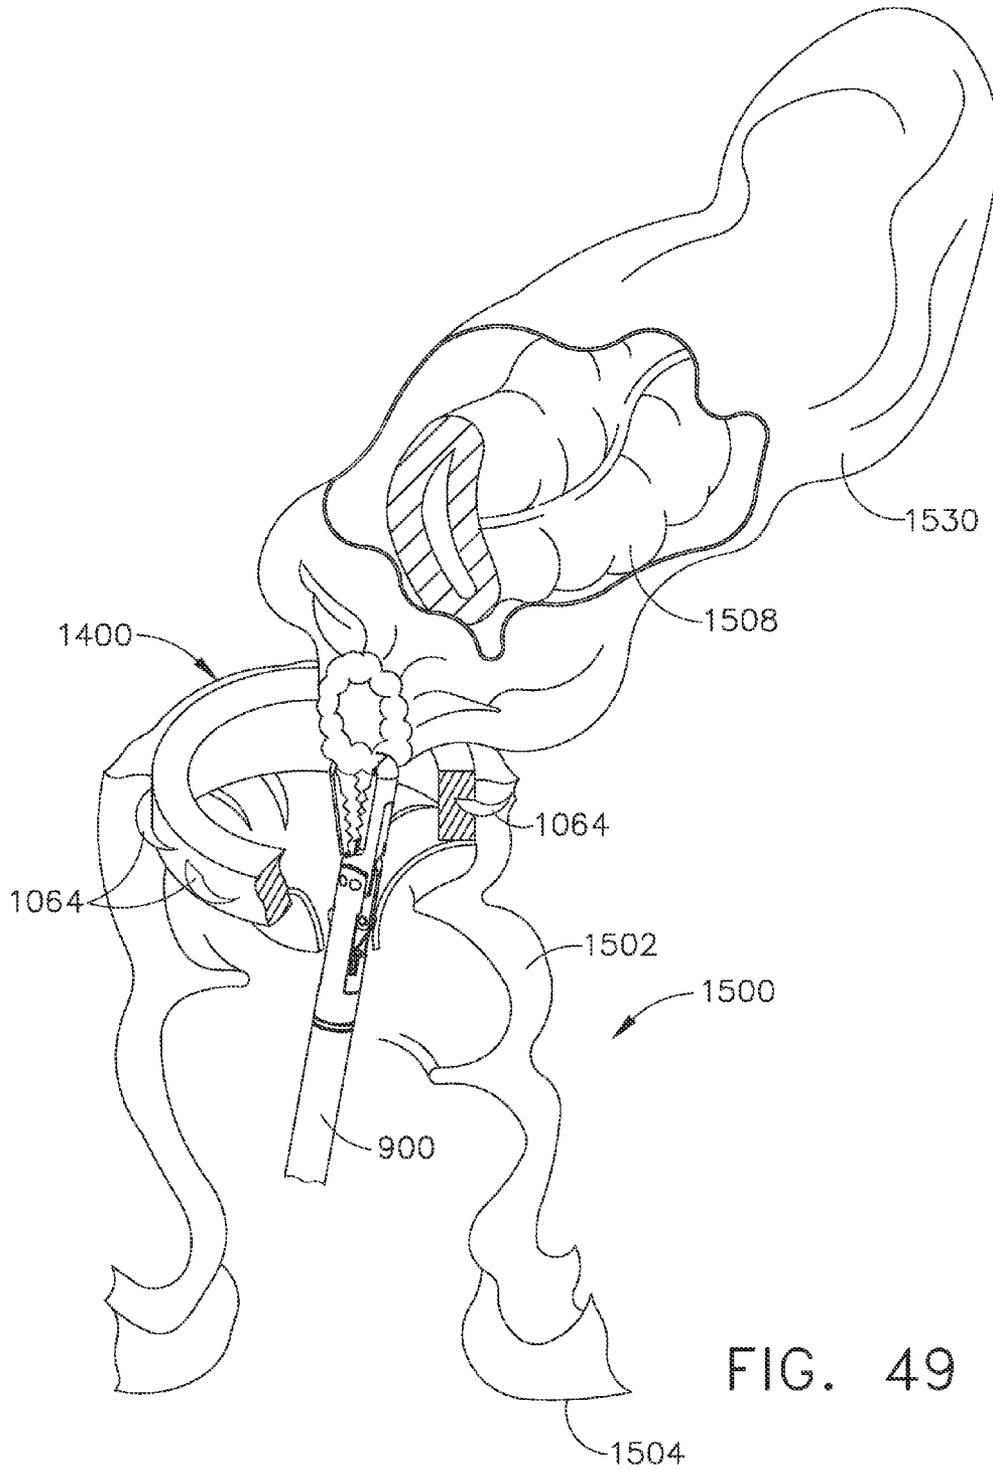


FIG. 49

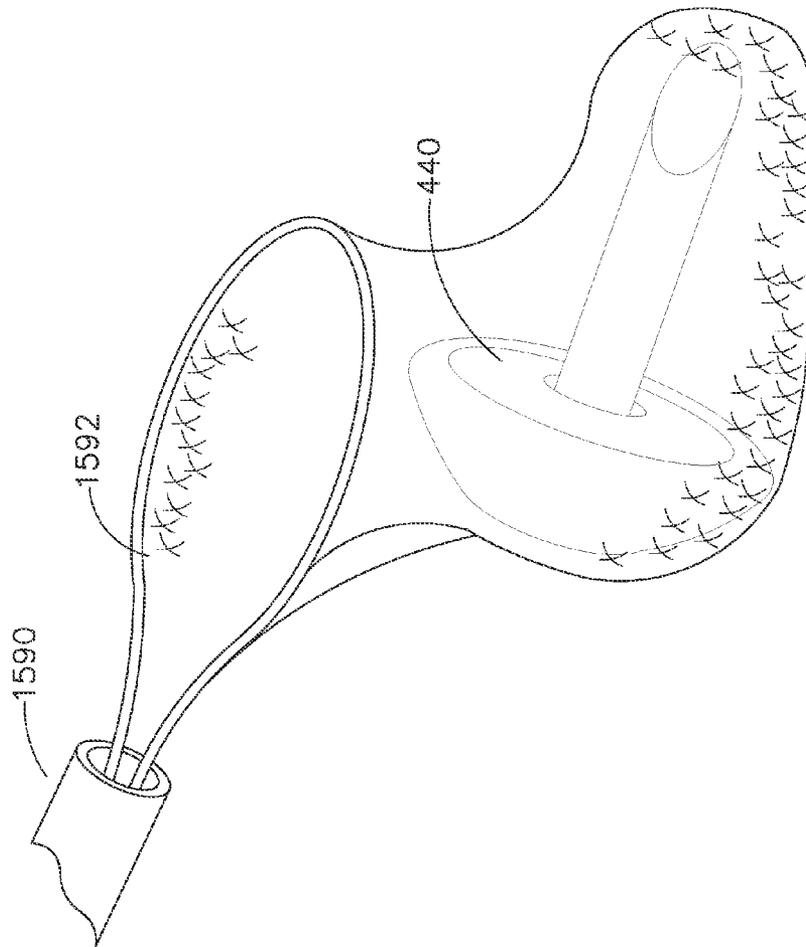


FIG. 50

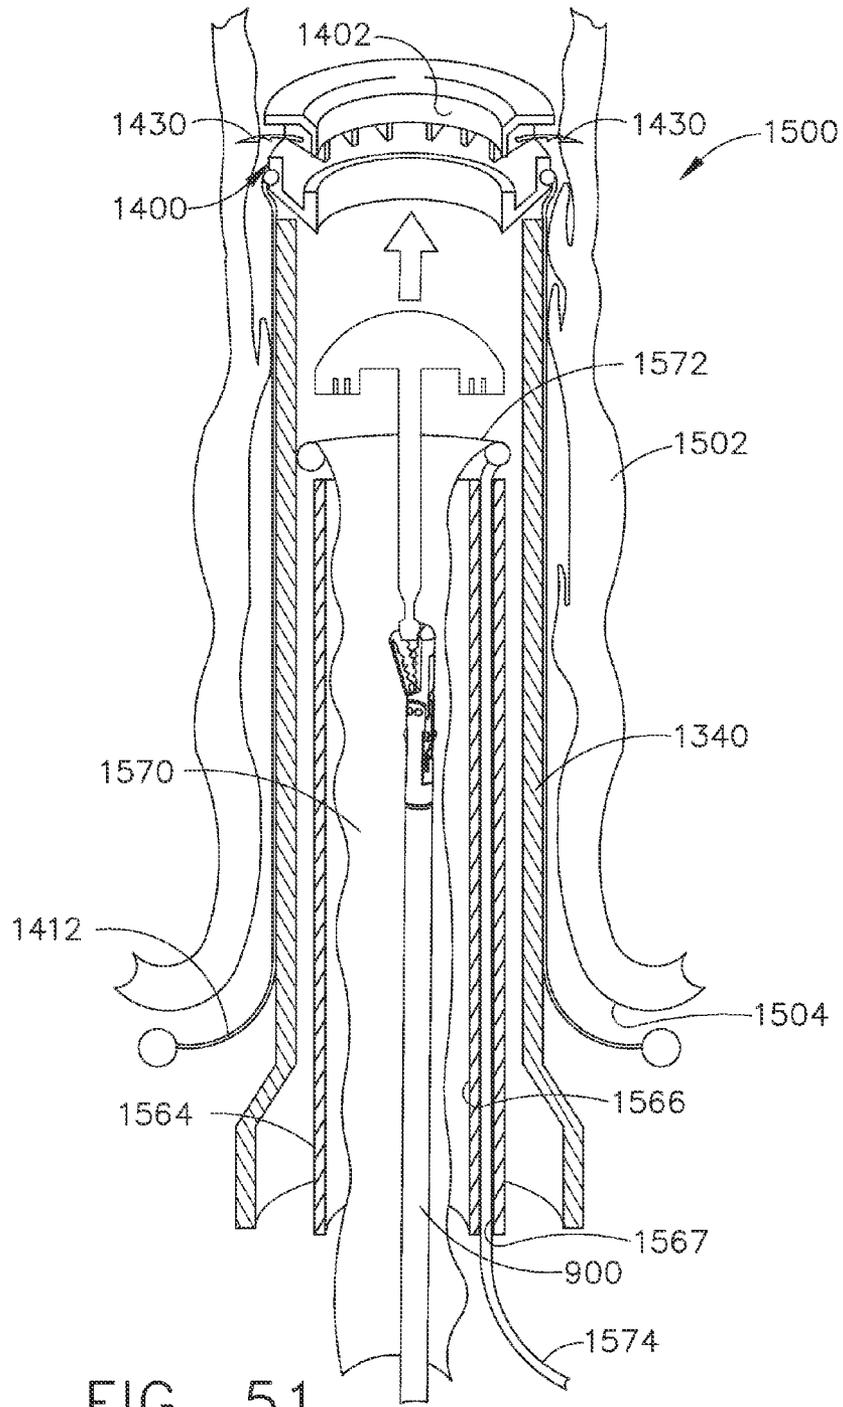


FIG. 51

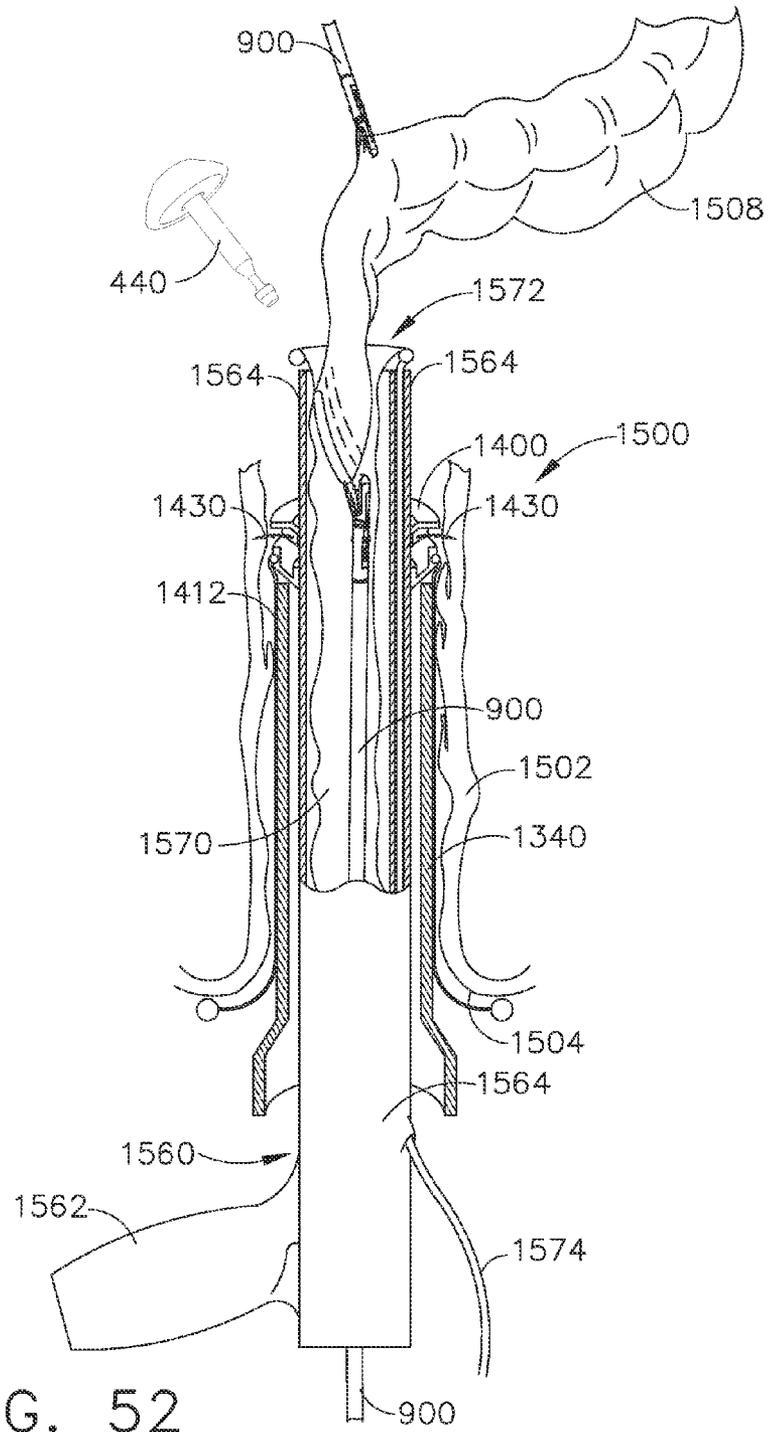


FIG. 52

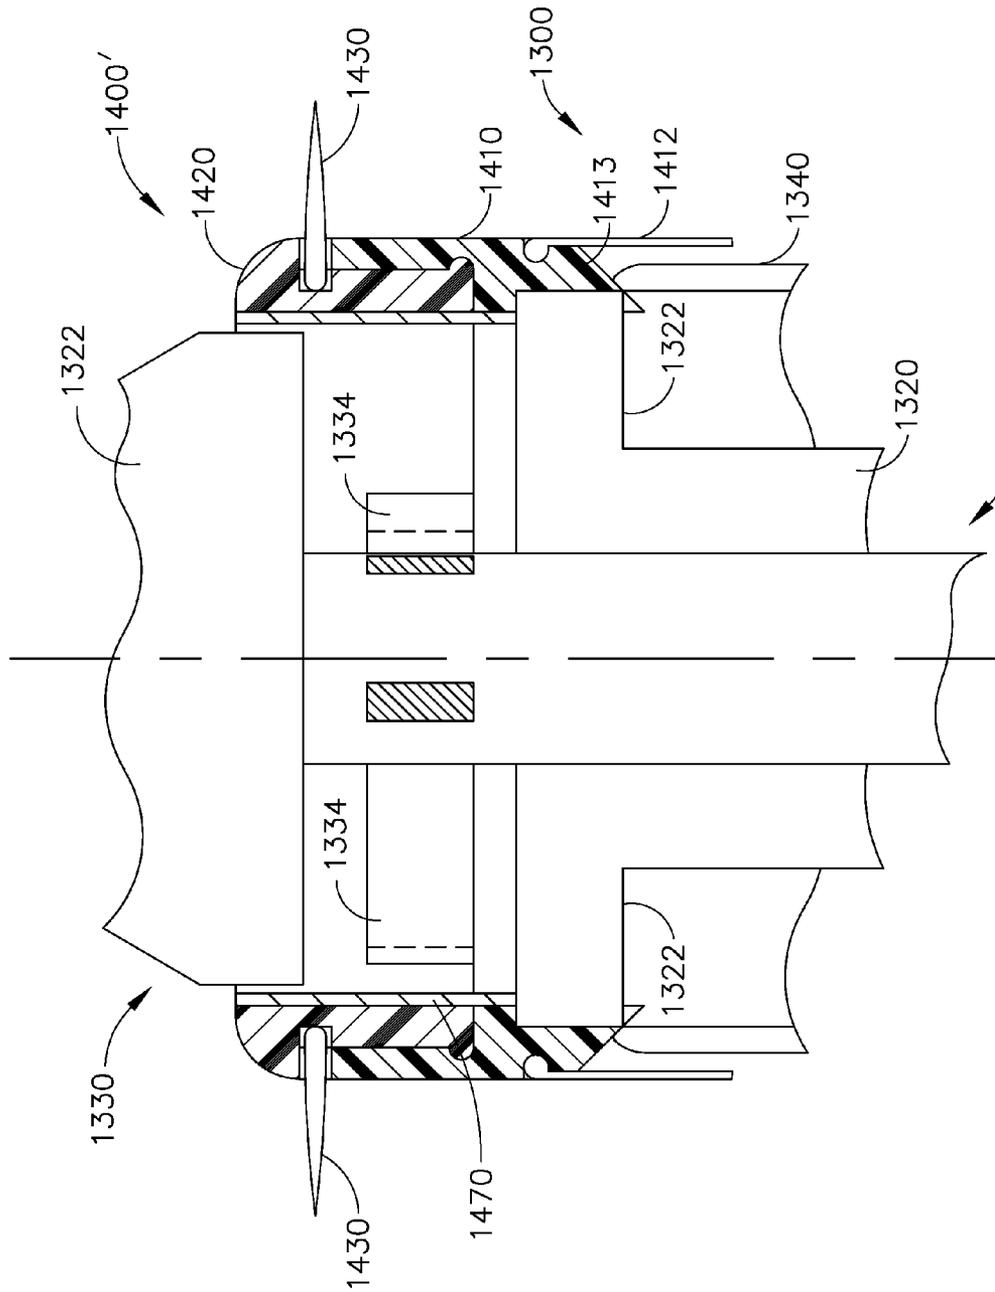


FIG. 53

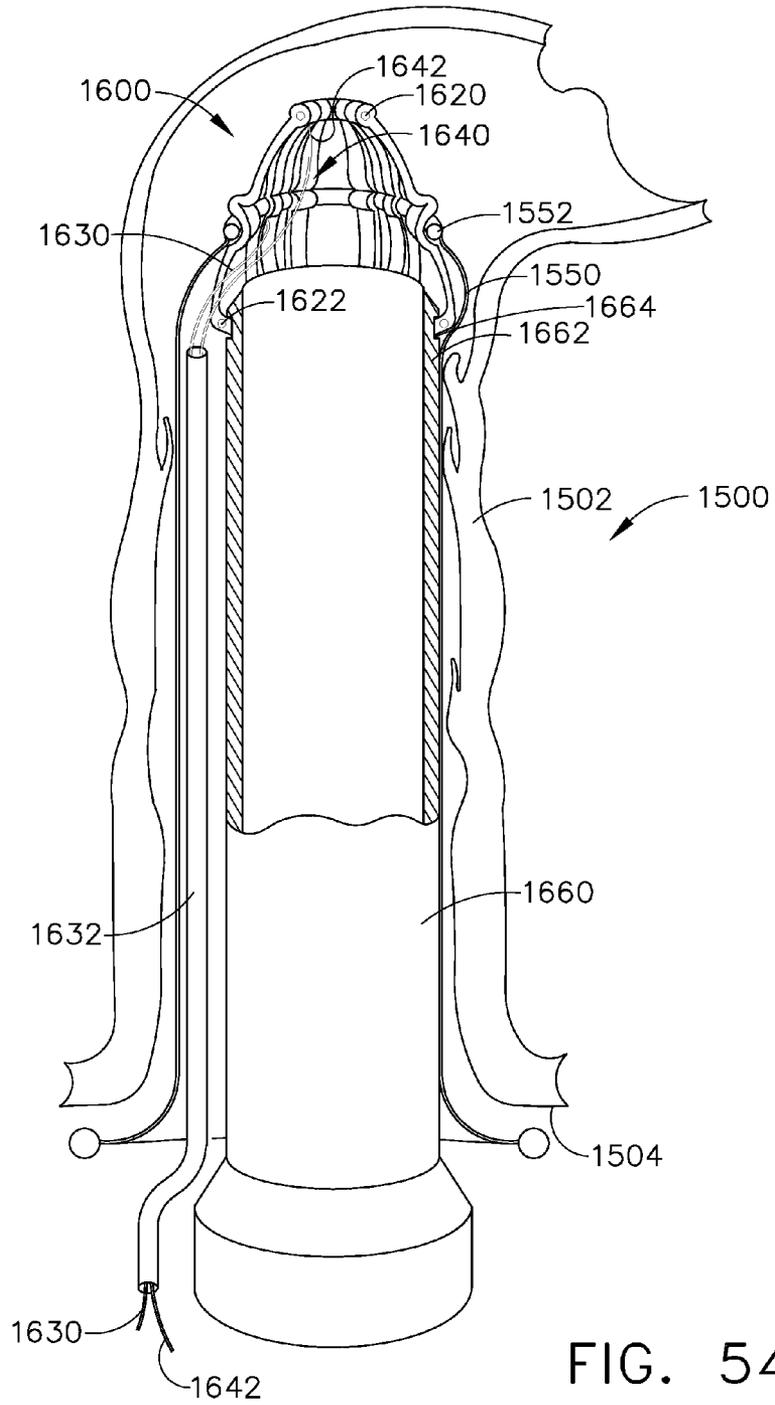


FIG. 54

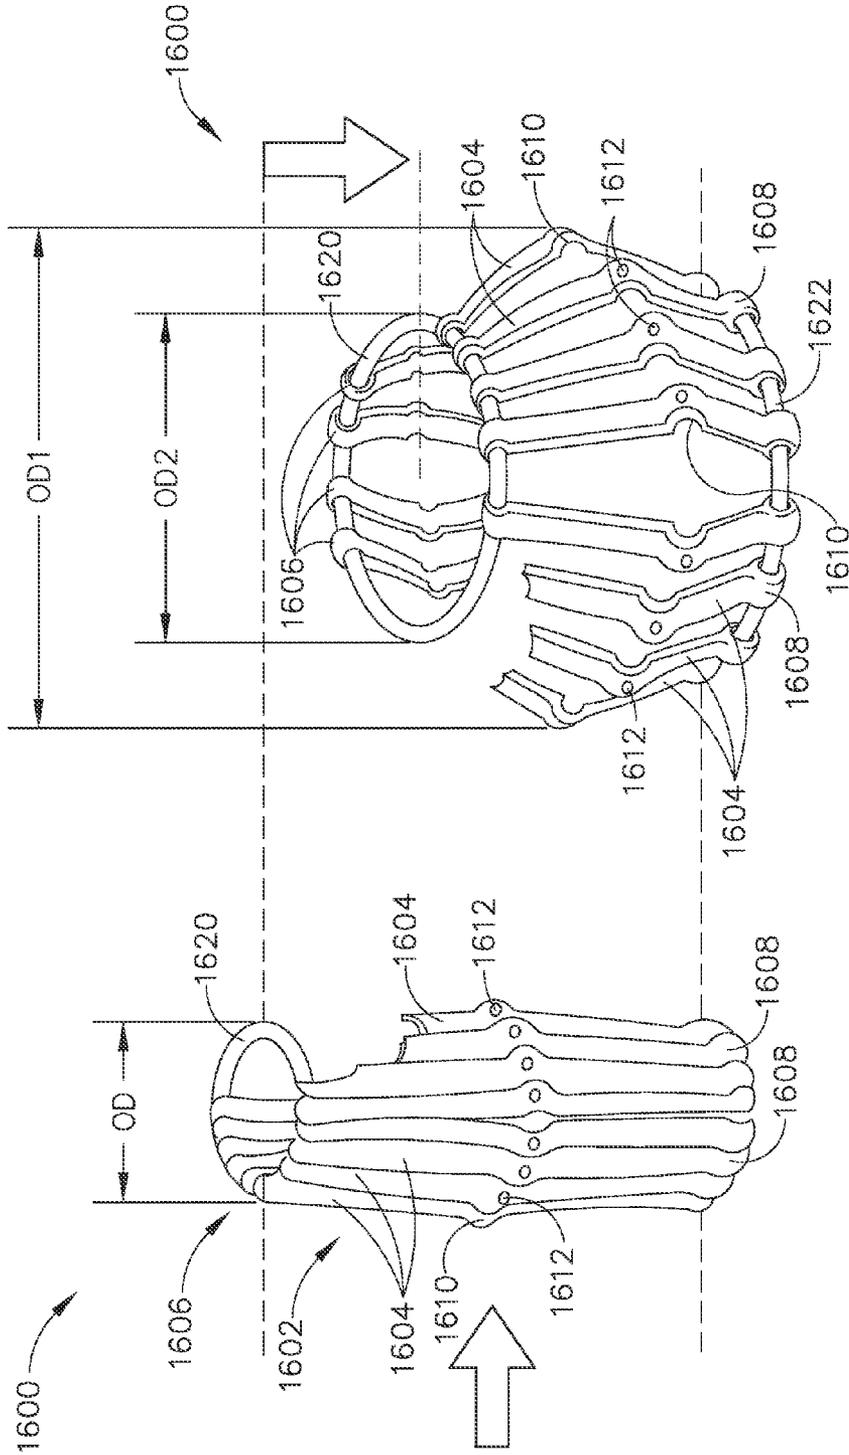


FIG. 55

FIG. 56

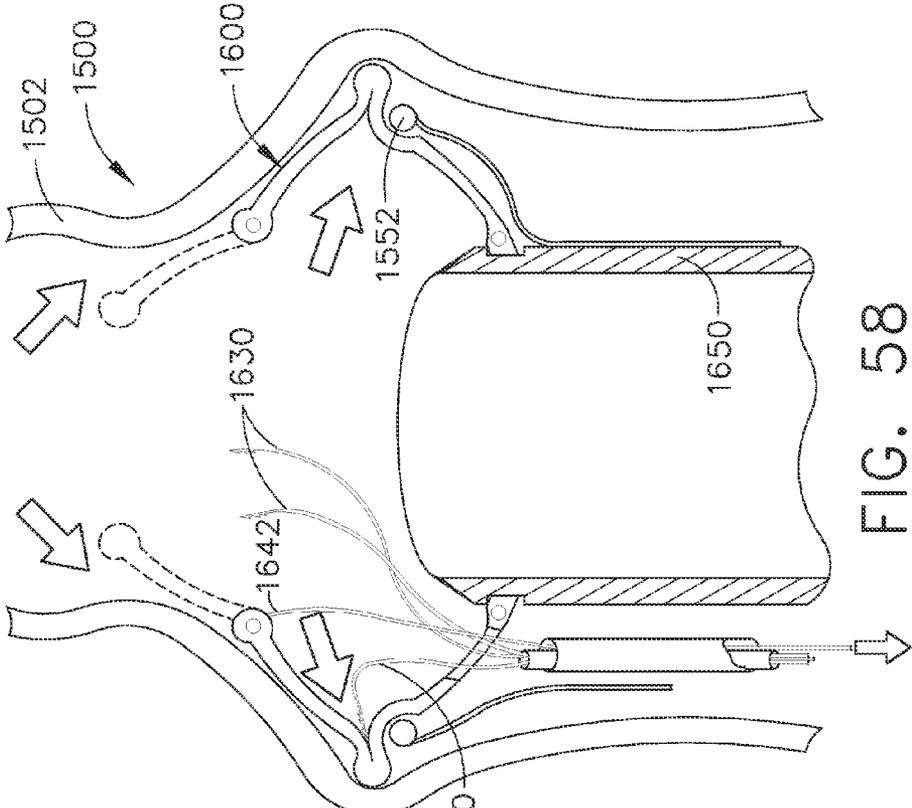


FIG. 57

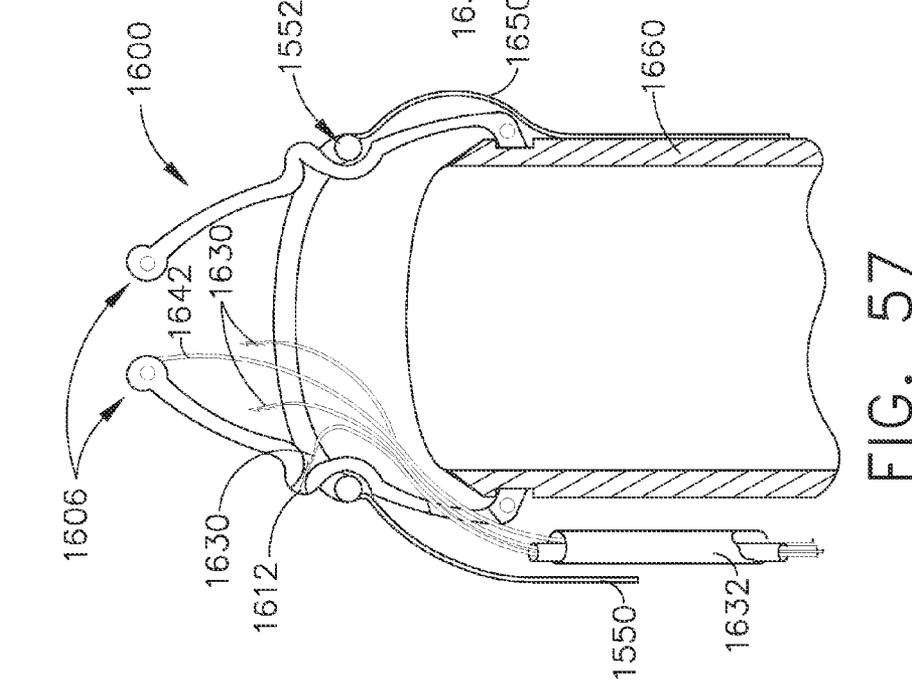


FIG. 58

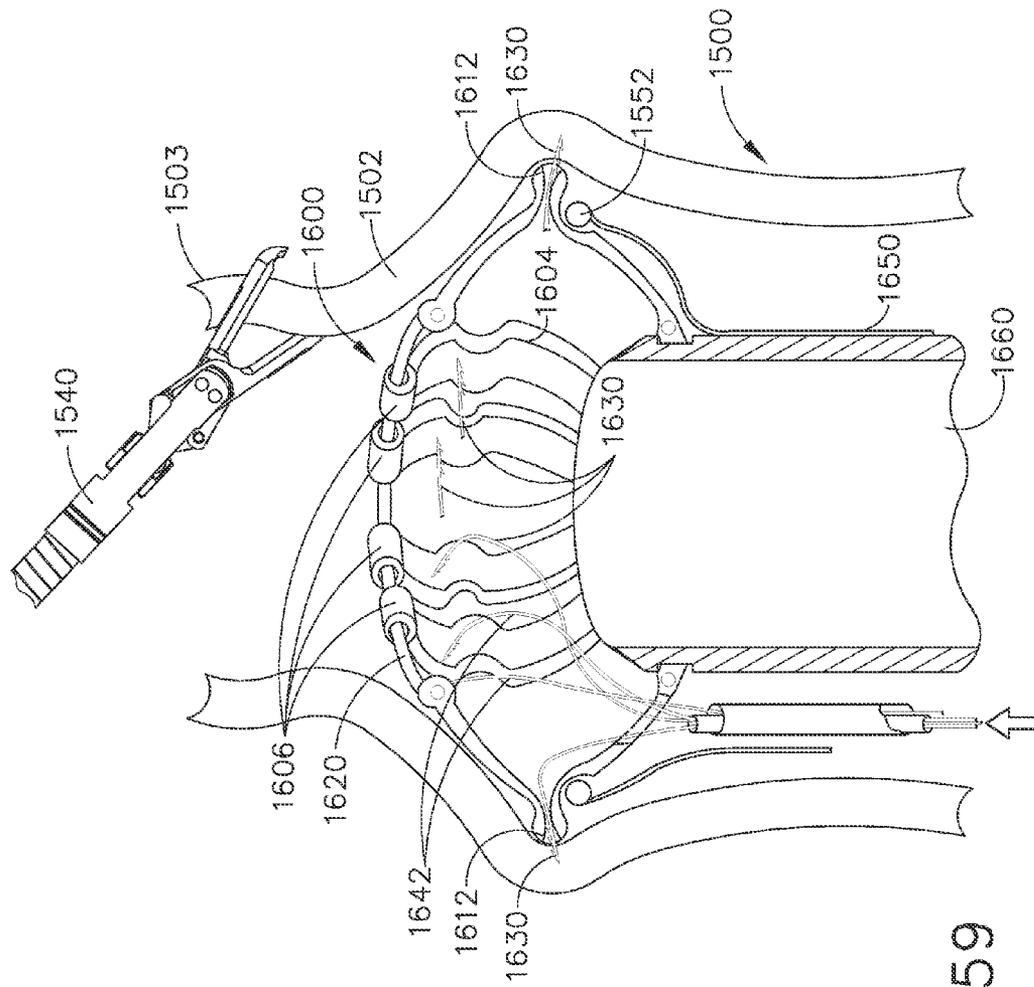


FIG. 59

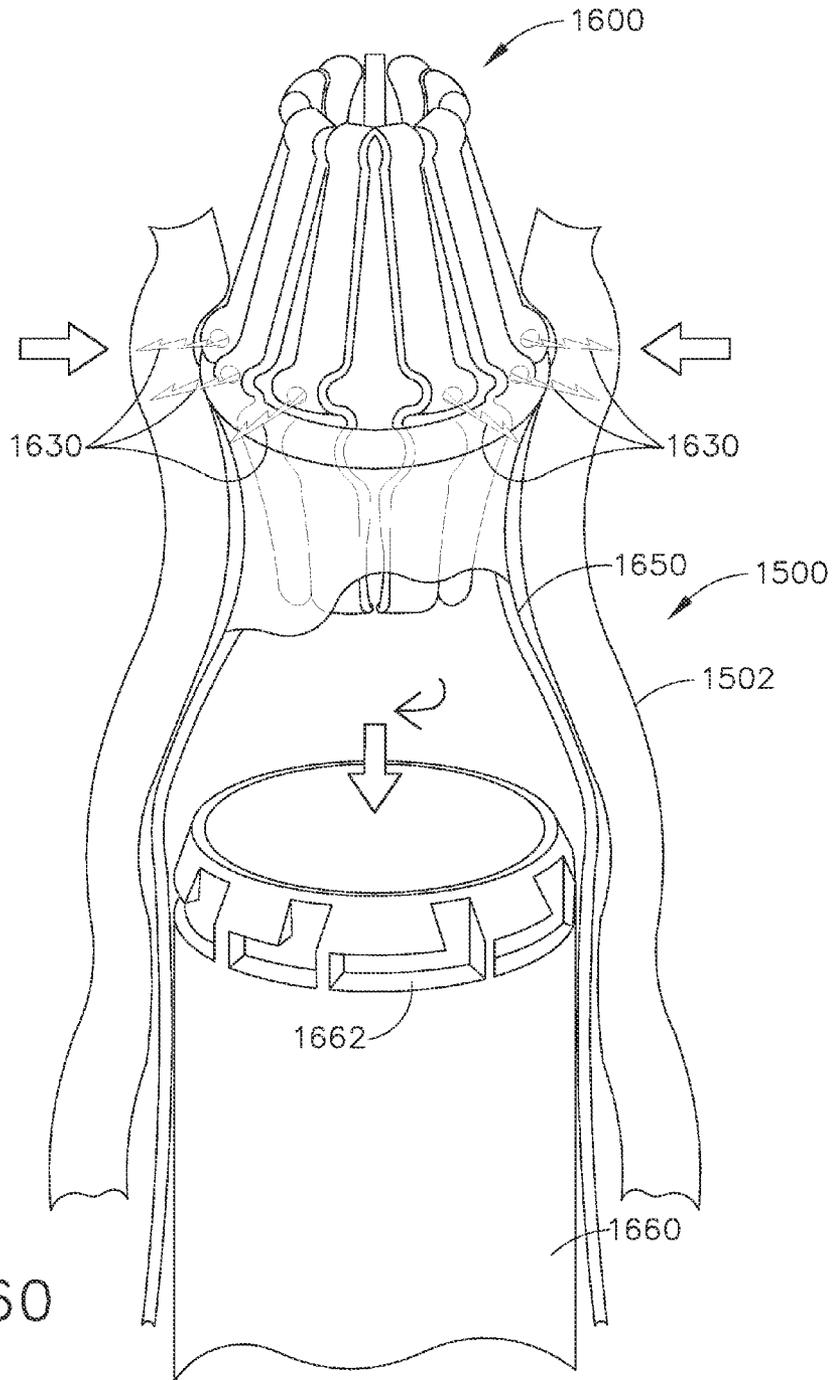


FIG. 60

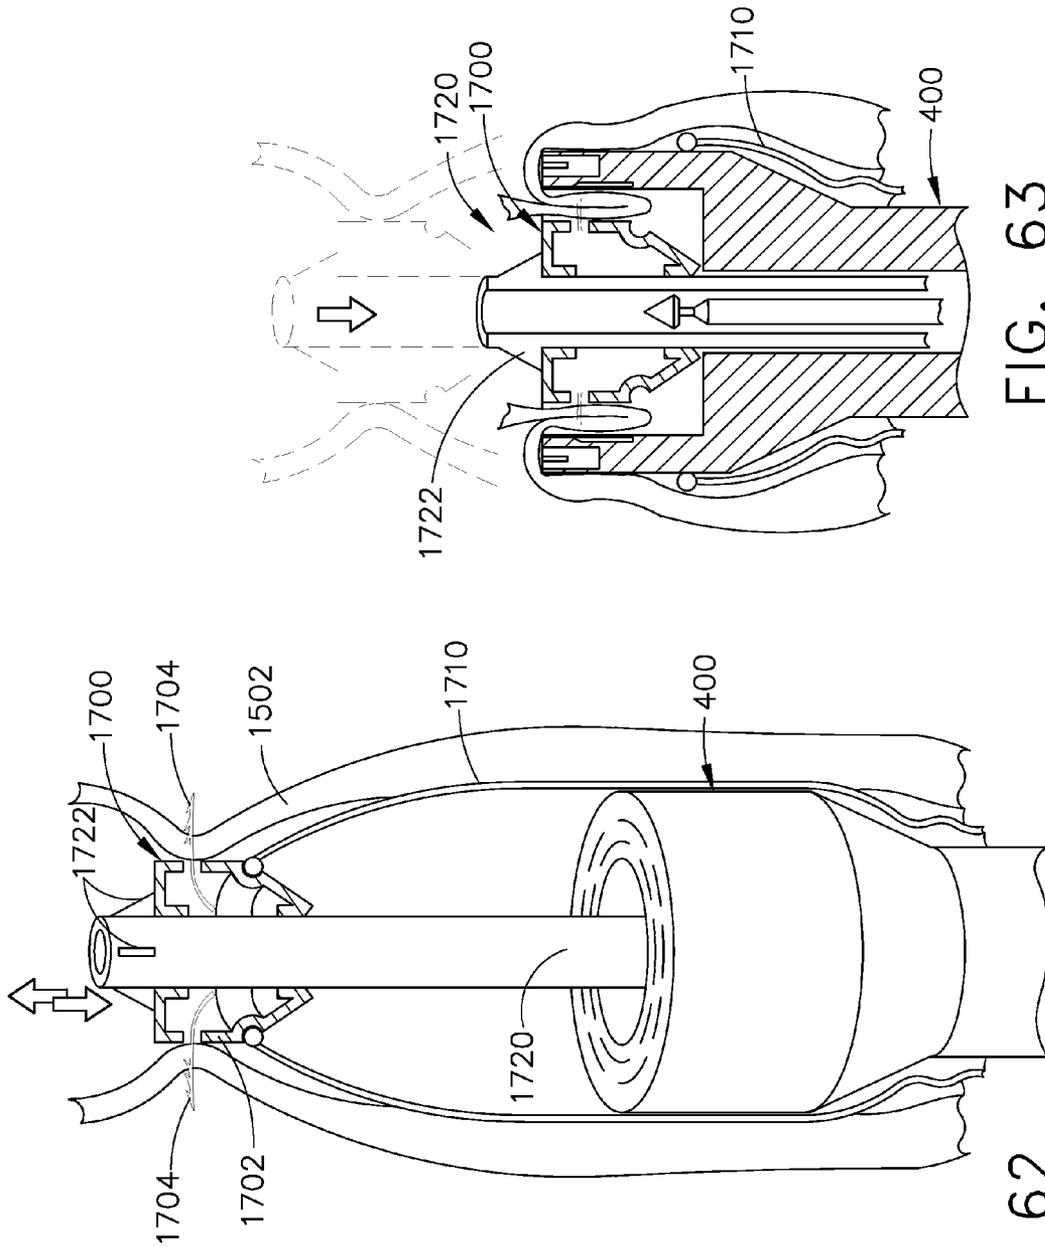


FIG. 63

FIG. 62

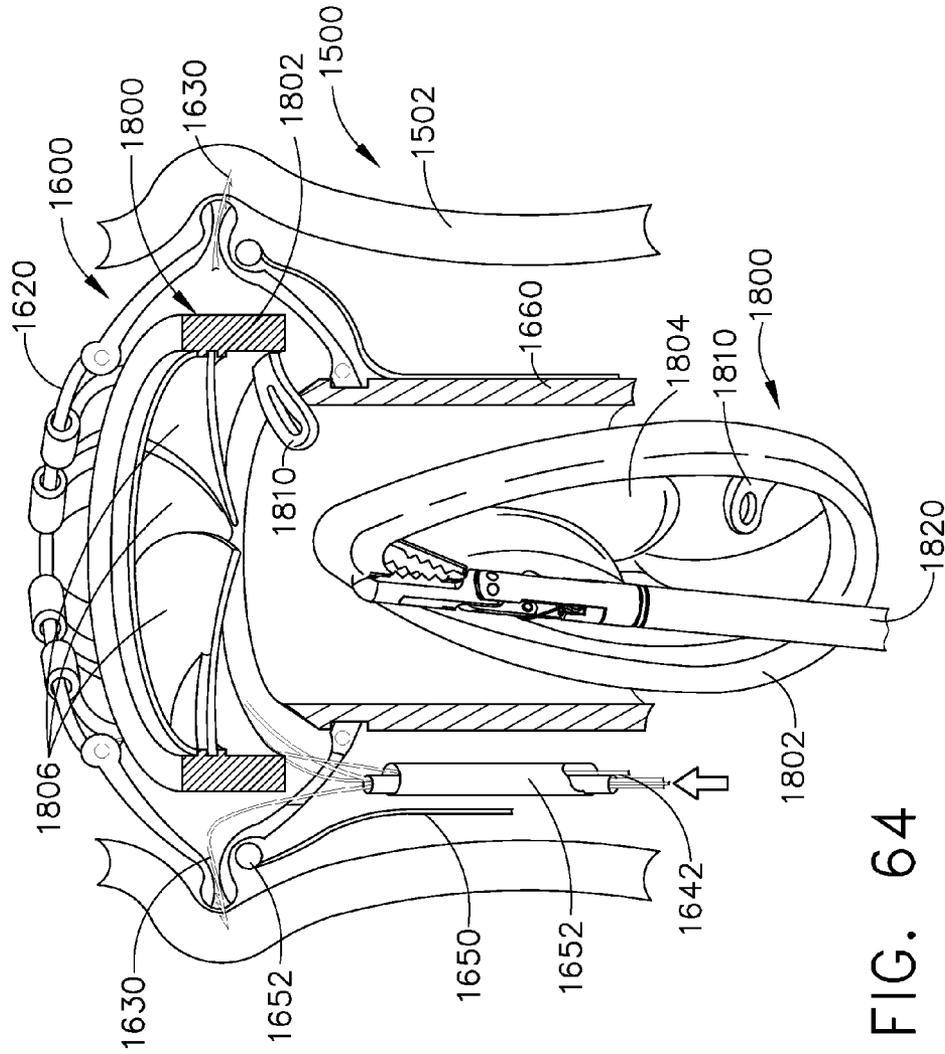
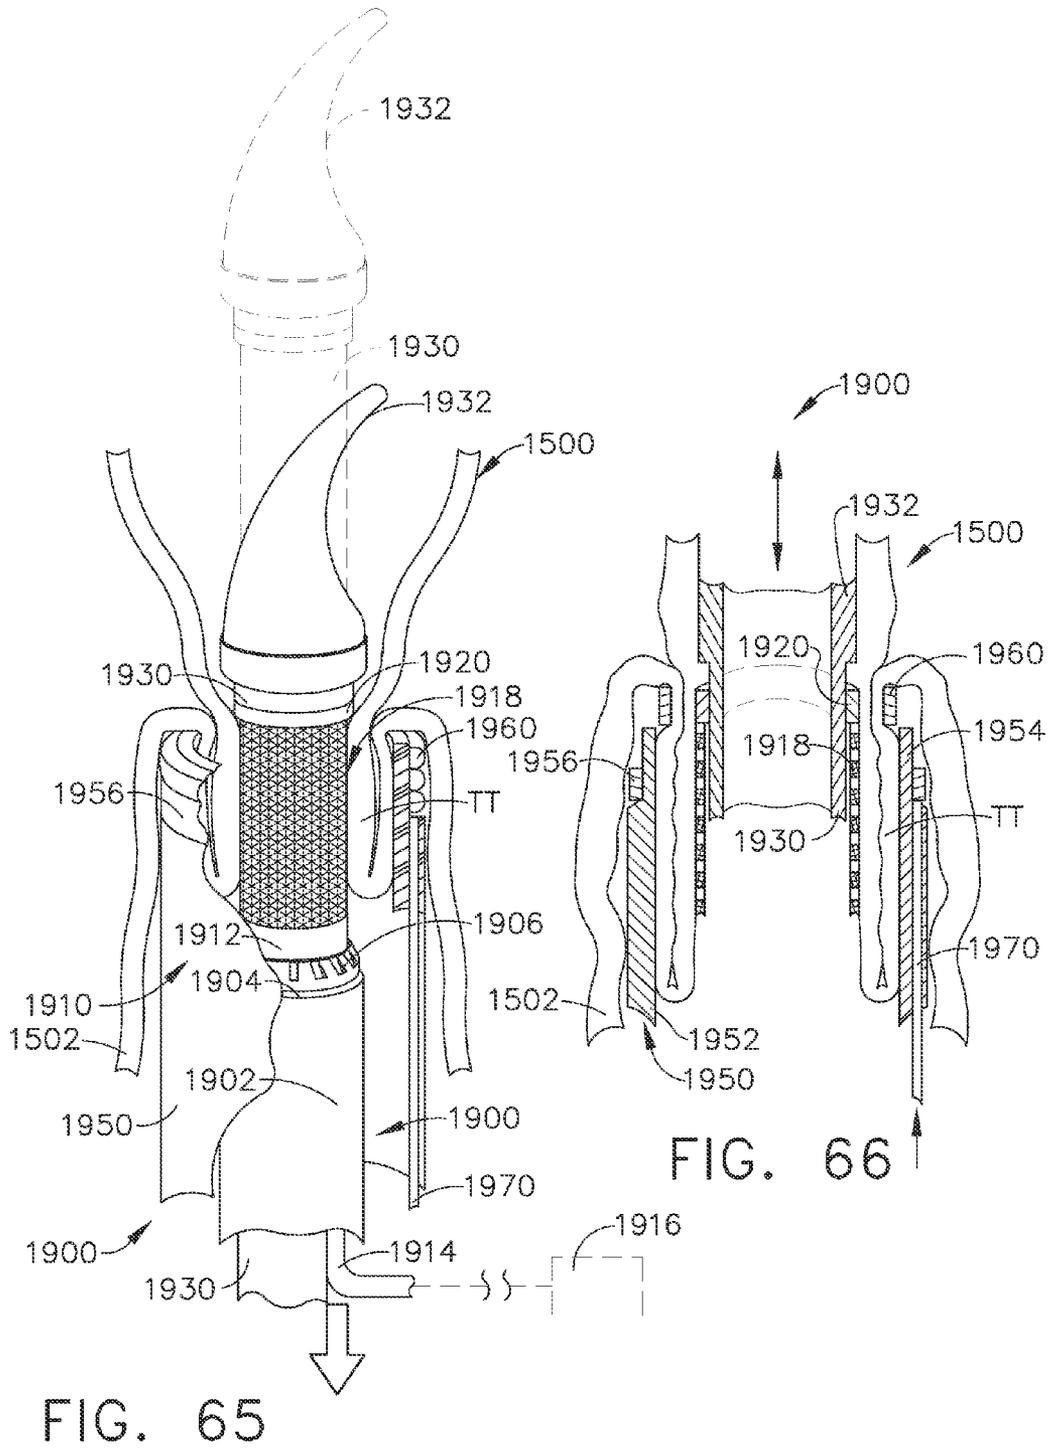


FIG. 64



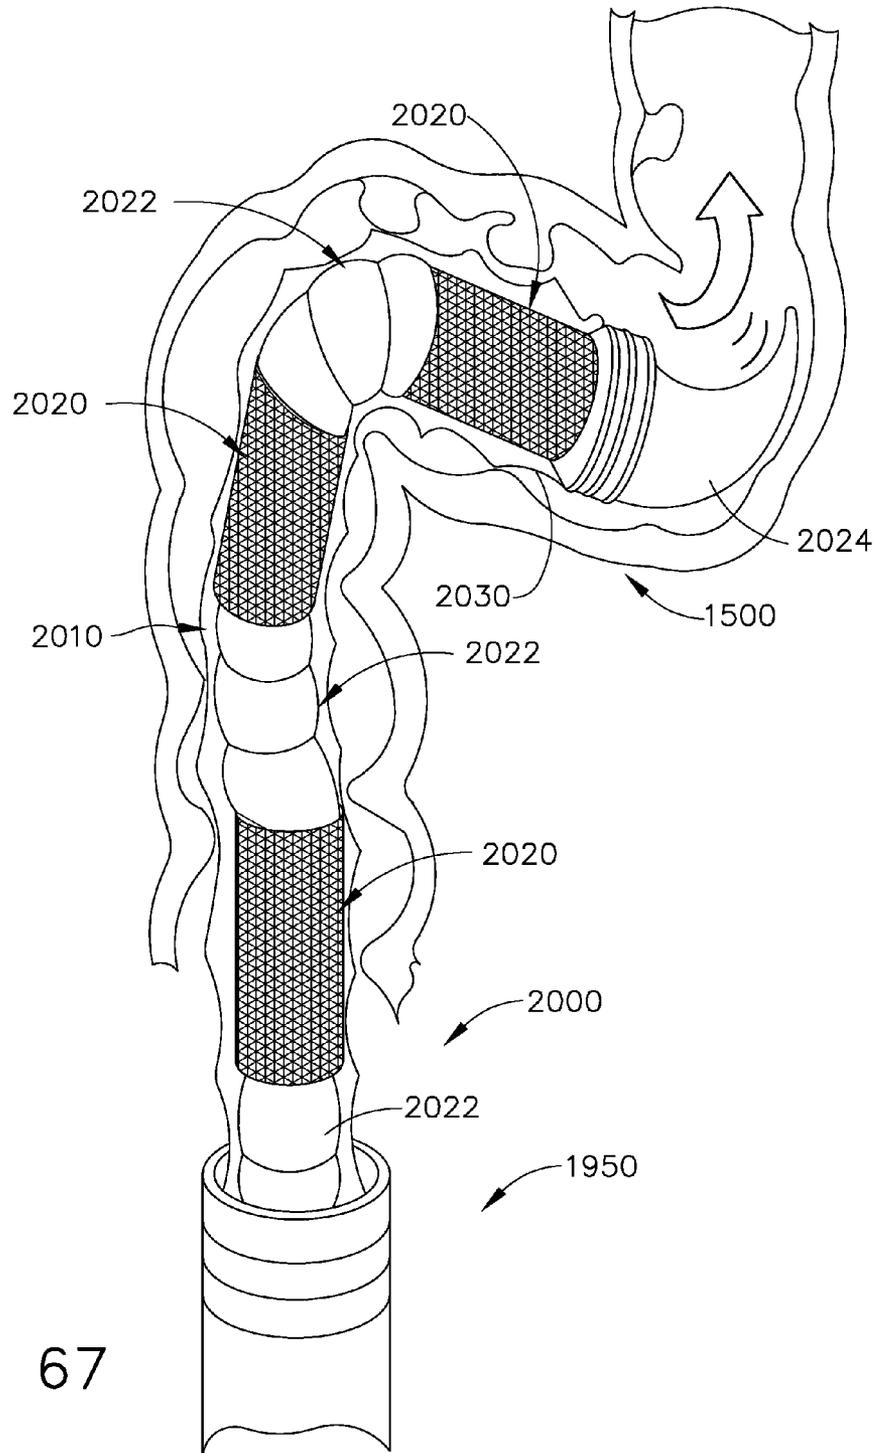


FIG. 67

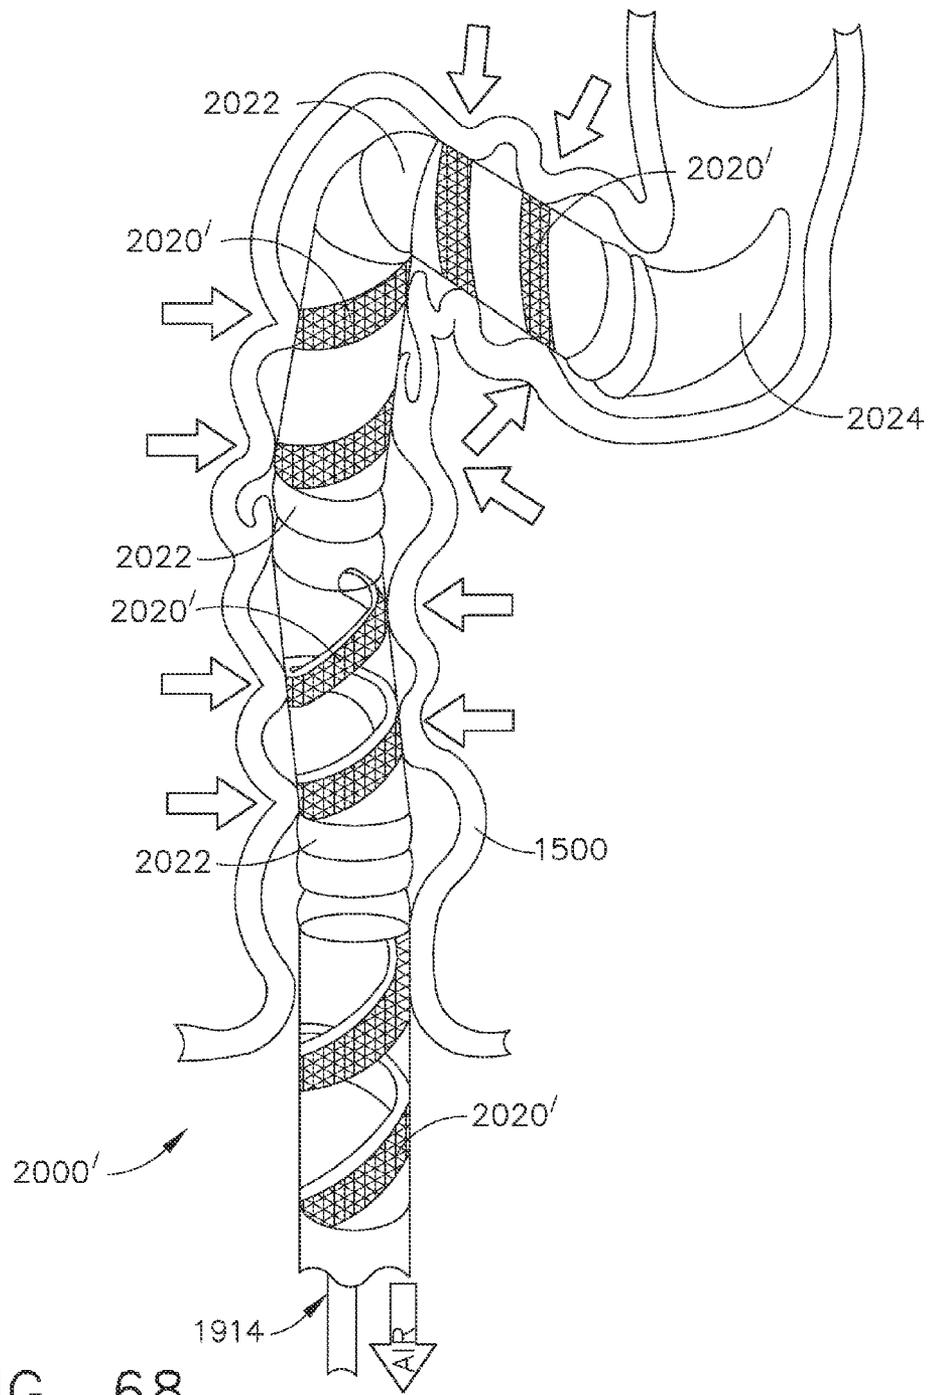


FIG. 68

MODULAR SURGICAL TOOL SYSTEMS**CROSS-REFERENCE TO RELATED APPLICATIONS**

This non-provisional patent application claims the benefit of and priority from U.S. Provisional Patent Application Ser. No. 61/452,432, filed Mar. 14, 2011, entitled "Surgical Stapling Instruments", the entire disclosure of which is hereby incorporated by reference.

FIELD OF THE INVENTION

The present invention generally relates to surgical devices for performing a variety of surgical procedures, and more particularly, to a surgical tool system that comprises a single handle assembly that can be employed with different tool attachments that are capable of performing different surgical procedures and actions.

BACKGROUND

Circular instruments are used to perform a number of surgical procedures. Such procedures often require the use of several different circular instruments that have a desired diametric size, shaft length and shaft geometry. Hospitals require storage space to inventory multiple product codes to satisfy these procedures.

One type of circular instrument that is often used in open and laparoscopic approaches is a circular stapling instrument. In general, a conventional circular stapler typically consists of an elongated shaft that has a proximal actuating mechanism and a distal stapling mechanism mounted to the elongated shaft. Various circular stapling devices are disclosed, for example, in U.S. Pat. Nos. 5,104,025; 5,205,459; 5,285,945; and 5,309,927 which are each herein incorporated by reference in their respective entireties. The distal stapling mechanism commonly consists of a fixed stapling cartridge that contains a plurality of staples configured in a concentric circular array. A round cutting knife is concentrically mounted in the cartridge interior for axial travel therein. Extending axially from the center of the cartridge is a movable trocar or attachment shaft that is adapted to have a staple anvil removably coupled thereto. The anvil is configured to form the ends of the staples as they are driven into it. The distance between a distal face of the staple cartridge and the staple anvil is commonly controlled by an adjustment mechanism that is mounted to the proximal end of the stapler shaft for controlling the axial movement of the trocar. Tissue that is clamped between the staple cartridge and the staple anvil is simultaneously stapled and cut when the actuating mechanism is activated by the surgeon.

Such circular stapling instruments are essential for creating anastomosis within the body when using open or laparoscopic methods. However, such instruments cannot perform other actions or procedures that may also be required to complete a particular operation. Such actions may comprise, for example, grasping and manipulating tissue, cutting tissue without deploying fasteners, dilating colon tissue, safely managing the removal of the transected specimens from the colon, etc. Thus, different types and sizes of instruments must be kept on hand.

Thus, the need exists for a surgical tool system that includes a single handle assembly that can be employed with different tool attachments that are capable of performing different surgical procedures and actions.

There is a further need for a universal port arrangement that can be used to dilate and/or occlude the colon and facilitate the entry and removal of surgical instruments within the colon;

5 There is a further need for a universal port arrangement that may be selectively employed to sever colon tissue.

Yet another need exists for a universal port arrangement that can facilitate the safe removal of transected colon portions.

10 The foregoing discussion is intended only to illustrate some of the shortcomings present in the field of the invention at the time, and should not be taken as a disavowal of claim scope.

BRIEF SUMMARY

In connection with general aspects of various embodiments of the present invention, there is provided a modular circular surgical instrument. In at least one form, the instrument comprises an actuator for generating an actuation motion and an actuation system that is configured to generate a plurality of discrete rotary drive motions in response to an application of the actuation motion thereto. An elongated shaft assembly operably interfaces with the actuation system and is configured to be interchangeably attached to a plurality of different surgical tool heads such that upon attachment of a first one of the surgical tool heads thereto, the elongated shaft assembly is caused to interact with the actuation system to impart a first one of the discrete rotary drive motions to the first surgical tool head when the actuation motion is applied to the actuation system. When a second one of the surgical tool heads is attached to the elongated shaft assembly, the elongated shaft assembly is caused to interact with the actuation system to impart a second one of the discrete rotary drive motions to the second surgical tool head upon when the actuation motion is applied to the actuation system.

In connection with yet another general aspect of one form of the present invention, there is provided a modular surgical instrument system that comprises a handle assembly that has a manually-actuatable actuator trigger operably supported thereon for generating an actuation motion. An actuation system is operably supported by the handle assembly and is configured to generate a plurality of discrete drive motions in response to an application of the actuation motion thereto. The instrument further comprises an elongated shaft assembly that includes an outer shaft casing that has a distal end. A rotary drive shaft is operably supported within the outer shaft casing and is oriented for selective operable interaction with the actuation system. The instrument further comprises a first surgical tool head that is configured for interchangeable attachment to the distal end of the outer shaft casing such that upon attachment thereto, the first surgical tool head moves the rotary drive shaft to a first drive position wherein upon application of the actuation motion to the actuation system, the rotary drive shaft imparts a first rotary drive motion to the first surgical tool head to cause the first surgical tool head to perform a first surgical action. A second surgical tool head is configured for interchangeable attachment to the distal end of the outer shaft casing such that upon attachment thereto, the second surgical tool head moves the rotary drive shaft to a second drive position wherein upon application of the actuation motion to the actuation system, the rotary drive shaft imparts a second rotary drive motion to the second surgical tool head to cause the second surgical tool head to perform a second surgical action that differs from the first surgical action. A third surgical tool head is configured for interchangeable attachment to the distal end of the outer shaft

casing such that upon attachment thereto, the third surgical tool head moves the rotary drive shaft to a third drive position wherein upon said application of said actuation motion to said actuation system, the rotary drive shaft imparts a third rotary drive motion to the third surgical tool head to cause the third surgical tool head to perform a third surgical action.

In accordance with still another general aspect of one form of the present invention, there is provided a method for performing colorectal surgery. The method comprises providing a modular surgical instrument that has an elongated shaft assembly that includes a distal end and is configured to generate a plurality of discrete drive motions upon application of actuation motions thereto. The method further comprises coupling a first surgical tool head that is configured to perform a first surgical procedure to the distal end of the elongated shaft assembly and inserting the surgical instrument into the colon to bring the first surgical tool head into operable engagement with a target tissue. The method further includes applying a first actuation motion to the surgical instrument to cause the first surgical tool head to perform the first surgical action on the target tissue. The method also comprises withdrawing the surgical instrument from the colon and detaching the first surgical tool head from the surgical instrument. The method further includes coupling a second surgical tool head that is configured to perform a second surgical procedure that differs from the first surgical procedure to the distal end of the elongated shaft assembly and reinserting the surgical instrument into the colon to position the second surgical tool head in a second position therein. The method further includes applying a second actuation motion to the surgical instrument to cause the second surgical tool head to perform the second surgical action and withdrawing the surgical instrument from the colon.

In accordance with general aspects of various forms of the present invention, there is provided a circular stapling head for use with a modular circular surgical instrument that has an elongated shaft assembly that is configured to apply rotary drive motions. In various embodiments, the circular stapling head comprises an outer casing that is configured for releasable attachment to the elongated shaft. The outer casing operably supports at least one circular array of surgical staples therein. A staple driver is constrained for axial movement within the outer casing and is configured for driving engagement by a rotary drive shaft portion of the elongated shaft assembly when the outer casing is attached to the elongated shaft assembly. An application of a rotary drive motion from the rotary drive shaft portion to the staple driver causes the staple driver to axially drive the surgical staples out of the outer casing.

In accordance with still other general aspects of various embodiments of the present invention, there is provided a surgical grasping device for use with a modular circular surgical instrument that has an elongated shaft assembly that is configured for generating rotary drive motions. Various forms of the surgical grasping device comprise an outer casing that is configured for releasable attachment to the elongated shaft assembly. The outer casing movably supports first and second jaws thereon that are each configured to receive rotary drive motions from the elongated shaft assembly. Upon application of the rotary drive motion in a first rotary direction, the first and second movable jaws are caused to move from a closed position to an open position. Upon application of the rotary drive motion to the first and second movable jaws in a second rotary direction, the first and second movable jaws are caused to move from the open position to the closed position.

In accordance with yet other general aspects of various forms of the present invention, there is provided a kit of

surgical tool heads for interchangeable use with a circular surgical instrument. In various forms, the kit comprises at least two of the circular tool heads selected from a group of circular surgical tool heads that includes a first circular stapling head that is configured for removable operable attachment to the circular surgical instrument for operably receiving a corresponding first drive motion therefrom. The group further includes a second circular stapling head that is configured for removable operable attachment to the circular surgical instrument for operably receiving a corresponding second drive motion therefrom. The group also includes a surgical grasping head that is configured for removable operable attachment to the circular surgical instrument for receiving corresponding third drive motion therefrom. The group also includes a universal port member that is configured for removable operable attachment to the circular surgical instrument for receiving at least one corresponding fourth drive motion therefrom.

In accordance with general aspects of various forms of the present invention, at least one embodiment comprises a universal port for insertion into a colon. In various forms, the universal port comprises a first ring stage that is configured to be selectively expanded from a collapsed insertion state to an expanded state upon application of a first rotary drive motion thereto and a second ring stage that is operably attached to the first ring stage and is configured to retainingly engage a portion of the colon upon application of a second rotary drive motion thereto.

In accordance with other general aspects of other forms of the present invention, in at least one embodiment, there is provided a universal port for insertion into a colon. In at least one form, the universal port comprises an annular port body that has a centrally-disposed port extending therethrough. A plurality of tissue-engaging barbs are operably supported within the annular port body and are configured for movement from a first insertion position within the annular port body to a second deployed position wherein a tissue-engaging portion thereof protrudes outward from the annular port body. A deployment drive assembly is operably supported within the annular port body and is configured for operable engagement with a surgical instrument. The deployment drive assembly operably interfaces with each of the tissue-engaging barbs such that upon application of a drive motion from the surgical instrument in a first direction causes the tissue-engaging barbs to move from the first insertion position to the second deployed position and upon another application of the drive motion from the surgical instrument in a second direction causes the tissue-engaging barbs to move from the deployed position to the insertion position.

In accordance with still other general aspects of other forms of the present invention, in at least one embodiment, there is provided a universal port for installation within a colon. In at least one form, the universal port comprises a first annular port body that is configured to be releasably inserted within the colon by an insertion member. A second annular port body is movably coupled to the first annular port body and is configured for releasable operable engagement with a drive member for applying drive motions thereto. The second annular port body operably supports a plurality of tissue-engaging barbs around a circumference of the second annular port body that are selectively deployable from an insertion position wherein each of the tissue-engaging barbs is supported substantially within the second annular port body and a deployed position wherein the tissue-engaging tip portions thereof protrude outward from the second annular port body.

In accordance with other general aspects of other forms of the present invention, in at least one embodiment, there is

5

provided a colon expansion port for installation within a colon. In at least one form, the colon expansion portion comprises a port body that has a proximal port end, a distal port end and a central portion that extends therebetween. The port body is selectively configurable from a collapsed insertion position and an expanded installation position. An insertion instrument is releasably attachable to the proximal end of the port body. An actuation member interfaces with the distal end of the port body to apply an actuation motion thereto for drawing the distal portion of the port body towards the proximal portion of the port body to move the port body from the insertion position to the installation position. A plurality of tissue-engaging barbs are operably supported within the port body and are movable from an un-deployed position to a deployed position when the actuation motion is applied to the distal end portion of the port body.

In accordance with other general aspects of other forms of the present invention, in at least one embodiment, there is a universal port for insertion into a colon. The universal port comprises a dilatable portion configured to be selectively expanded from a collapsed insertion state to an expanded state upon the application of a rotary drive motion thereto wherein the dilatable portion is configured to engage the colon in its expanded state. The universal port further comprises a drive portion configured to engage the dilatable portion and apply the rotary drive motion to the dilatable portion.

In accordance with other general aspects of other forms of the present invention, in at least one embodiment, there is a port for insertion into a patient's colon and use during a surgical technique using a surgical stapler, the surgical stapler including a tool head and an anvil attachable to the tool head. The port comprises a frame configured to engage the colon, an aperture extending through the frame, wherein the aperture is sized and configured to permit the anvil to be passed therethrough in a first direction and a portion of the patient's colon to be passed therethrough in a second direction. The port can further comprise a sleeve extending from the frame, wherein the sleeve is sized and configured to receive at least a portion of the tool head therein.

In accordance with other general aspects of other forms of the present invention, in at least one embodiment, there is a port for insertion into a patient's colon and use during a surgical technique using a surgical stapler, the surgical stapler including a tool head and an anvil attachable to the tool head. The port comprises a frame configured to engage the colon, means for permitting the anvil to be passed through the frame in a first direction, and means for permitting a portion of the patient's colon to be passed through the frame in a second direction.

In accordance with other general aspects of other forms of the present invention, in at least one embodiment, there is a port for insertion into a patient's colon and use during a surgical technique using a surgical stapler, the surgical stapler including a tool head and an anvil attachable to the tool head. The port comprises means for securely engaging the colon, means for permitting the anvil to be passed through the frame in a first direction, and means for permitting a portion of the patient's colon to be passed through the frame in a second direction.

BRIEF DESCRIPTION OF THE FIGURES

The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodiments of the invention, and, together with the general description of the invention given above, and the detailed description

6

of the embodiments given below, serve to explain the principles of the various forms of the present invention.

FIG. 1 is an exploded perspective view of one form of a modular surgical instrument of an embodiment of the present invention and a surgical tool head embodiment of the present invention;

FIG. 2 is a cross-sectional view of one form of a modular surgical instrument embodiment of the present invention attached to a surgical tool head embodiment of the present invention;

FIG. 3 is a partial perspective view of one embodiment of an actuation system of a modular surgical instrument embodiment of the present invention;

FIGS. 3A-3C are side views of a gear plate embodiment and rotary drive shaft embodiment of the present invention;

FIG. 4 is another cross-sectional view of the modular surgical instrument embodiment of and surgical tool head of FIG. 2 with an anvil (shown in phantom lines) attached thereto;

FIG. 5 is a cross-sectional view of the shaft assembly and surgical tool head depicted in FIGS. 2 and 4;

FIG. 5A is another cross-sectional view of the shaft assembly and surgical tool head depicted in FIG. 5 with an anvil (shown in phantom lines) attached thereto;

FIG. 6 is a partial cross-sectional view of the handle and shaft assembly of the modular surgical instrument of FIGS. 2 and 4;

FIG. 7 is another partial cross-sectional view of the handle and shaft assembly of FIG. 6 and three different surgical tool head embodiments of the present invention;

FIG. 8 is a cross-sectional view of one form of a modular surgical instrument embodiment of the present invention attached to another surgical tool head embodiment of the present invention;

FIG. 9 is a cross-sectional view of the shaft assembly and surgical tool head depicted in FIG. 8;

FIG. 10 is a partial side view of one rotary drive shaft embodiment of the present invention;

FIG. 11 is a partial cross-sectional perspective view of the surgical tool head depicted in FIGS. 8 and 9;

FIG. 12 is a cross-sectional view of the surgical tool head of FIG. 11;

FIG. 13 is a partial perspective view of a portion of the rotary drive shaft and an adapter cap embodiment of the present invention;

FIG. 14 is an exploded perspective view of a rotary drive shaft embodiment and a gear drive adapter shaft embodiment of the present invention;

FIG. 15 is an assembled view of the rotary drive shaft and gear drive adapter shaft embodiment of FIG. 14;

FIG. 16 is a partial cross-sectional view of another surgical tool head embodiment of the present invention with the movable jaws thereof in an open position;

FIG. 17 is another partial cross-sectional view of the surgical tool head embodiment of FIG. 16 with the movable jaws thereof in a closed position;

FIG. 18 is a partial cross-sectional view of another surgical tool head embodiment of the present invention with the movable jaws thereof in an open position;

FIG. 19 is another partial cross-sectional view of the surgical tool head embodiment of FIG. 18 with the movable jaws thereof in a closed position;

FIG. 20 is a partial top view of a rotary adapter employed in the surgical tool head of FIGS. 18 and 19;

FIG. 21 is a partial cross-sectional view of another surgical tool head embodiment of the present invention with various component portions thereof omitted for clarity;

FIG. 22 is a partial cross-sectional view of another surgical tool head embodiment of the present invention with various component portions thereof omitted for clarity;

FIG. 23 is a partial cross-sectional view of a modular surgical instrument embodiment wherein the surgical staples have been driven horizontally through an elastic ring supported within the colon;

FIG. 24 is another partial cross-sectional view of a modular surgical instrument embodiment wherein the surgical staples have been driven horizontally through an elastic ring supported on the distal end of a shaft assembly;

FIG. 25 is another partial cross-sectional view illustrating surgical staples that have been driven horizontally through an elastic ring supported within the colon with a metal ring removably inserted into the interior of the elastic ring to prevent the elastic ring from collapsing;

FIG. 26 illustrates a colon portion wherein the elastic rings disclosed in FIGS. 23-25 have been attached to the ends of the colon portion and are in a collapsed state;

FIG. 27 is a partial cross-sectional perspective view of a severed portion of the colon being pulled through a tube inserted through the rectum;

FIG. 28 is a partial perspective view of portions of a patient's colon after the diseased portion has been removed through a port installed in the rectum;

FIG. 29 is a partial cross-sectional view of a universal port member embodiment of the present invention;

FIG. 30A is a top cross-sectional view of a first ring stage of the universal port member of FIG. 29 taken along line 30A-30A in FIG. 29;

FIG. 30B is another top cross-sectional view of the first ring stage of FIG. 30A in an expanded orientation;

FIG. 31A is a top cross-sectional view of a second ring stage of the universal port member of FIG. 29 taken along line 31A-31A in FIG. 29;

FIG. 31B is another top cross-sectional view of the second ring stage of FIG. 31A in an expanded orientation;

FIG. 32A is a top cross-sectional view of a third ring stage of the universal port member of FIG. 29 taken along line 32A-32A in FIG. 29;

FIG. 32B is another top cross-sectional view of the third ring stage of FIG. 32A in an expanded orientation;

FIG. 33 is a cross-sectional view of another universal port embodiment of the present invention;

FIG. 33A is a diagrammatical perspective view of the universal port embodiment of FIG. 33;

FIG. 33B is another diagrammatical perspective view of another universal port embodiment of the present invention;

FIG. 34 is a top cross-sectional view of another surgical tool head embodiment of the present invention;

FIG. 35 is a partial cross-sectional elevational view of the surgical tool head embodiment of FIG. 34;

FIG. 36 is a partial cross-sectional view of another universal port embodiment of the present invention in connection with an installation tool;

FIG. 37 is a top cross-sectional view of the universal port and installation tool embodiments of FIG. 36 taken along line 37-37 in FIG. 36;

FIG. 38 is a top cross-sectional view of the universal port and installation tool embodiments of FIGS. 36 and 37 taken along line 38-38 in FIG. 36;

FIG. 39 is a top cross-sectional view of the universal port and installation tool embodiments of FIGS. 36-38 with the tissue retaining barbs in a deployed position;

FIG. 40 is a side cross-sectional view of the universal port and installation tool embodiments as depicted in FIG. 39;

FIG. 41A is a cross-sectional view of the universal port of FIGS. 36-40;

FIG. 41B is a cross-sectional view of a universal port in accordance with at least one alternative embodiment;

FIG. 42 is a partial cross-sectional view of a universal port embodiment of the present invention and insertion tube embodiment of the present invention positioned within the rectum;

FIG. 43 illustrates a universal port embodiment of the present invention installed in the rectum and wherein a diseased portion of the colon has been severed from a distal portion of the colon;

FIG. 44 illustrates use of a grasping instrument through a universal port embodiment of the present invention;

FIG. 45 is another view of the universal port and grasping instrument depicted in FIG. 44;

FIG. 46 is another view of the universal port of FIGS. 44 and 45 wherein the grasping instrument is being used to draw the diseased colon portion through the universal port;

FIG. 47 illustrates use of another universal port embodiment of the present invention within a colon wherein a diseased portion has been drawn therein and the tissue cutting members of the port have been deployed to sever the diseased portion from the rectum;

FIG. 48 is another view of a portion of a colon with a universal port embodiment of the present invention installed therein;

FIG. 49 is another view of the colon and universal port of FIG. 47 wherein a severed diseased portion has been inserted into a collection bag that is being drawn through the port with a grasping instrument;

FIG. 50 is a partial perspective view of a retrieval instrument used to retrieve an anvil from the surgical site;

FIG. 51 is a partial cross-sectional view of a universal port embodiment of the present invention and insertion tube embodiment of the present invention positioned within the rectum with a retrieval tool embodiment of the present invention inserted therein to introduce an anvil into the surgical site;

FIG. 52 is another view of the universal port, insertion tube and retrieval tool as depicted in FIG. 51 and wherein a diseased portion of the colon is being drawn into the retrieval tool by a grasping instrument inserted therethrough;

FIG. 53 is a partial cross-sectional view of another universal port embodiment of the present invention;

FIG. 54 is a partial cross-sectional view of another port embodiment of the present invention and insertion tube embodiment of the present invention positioned within the rectum;

FIG. 55 is a perspective view of a portion of the port of FIG. 54 in a collapsed state;

FIG. 56 is another perspective view of the port of FIGS. 54 and 55 in an expanded state;

FIG. 57 is another partial cross-sectional view of the port and insertion tube embodiments of FIG. 54;

FIG. 58 is another partial cross-sectional view of the port and insertion tube of FIG. 57 inserted into a portion of the colon and illustrating deployment of the tissue retaining barbs into the colon;

FIG. 59 is another partial cross-sectional view of the port and insertion tube of FIG. 57 deployed in a portion of the rectum and wherein a tissue cutting instrument is cutting a diseased portion of the colon from the rectum;

FIG. 60 is another view of the port and insertion tube of FIGS. 54-59 wherein the insertion tube has been detached from the port;

FIG. 61 is another view of the port of FIGS. 54-59 being draw into a circular stapling head embodiment of the present invention;

FIG. 62 is a partial perspective view of another universal port embodiment of the present invention installed within the colon and being engaged by a circular stapling head embodiment of the present invention;

FIG. 63 a partial cross-sectional view of the circular stapling head and universal port of FIG. 62 wherein the universal port has been drawn into the circular stapling head;

FIG. 64 is another perspective view of a port and insertion tube embodiment of the present invention installed with the colon and wherein a grasping instrument is used to introduce and insert a flexible port member embodiment therein;

FIG. 65 is a partial cross-sectional perspective view of a tissue manipulation device embodiment of the present invention inserted into the colon and engaging a portion thereof;

FIG. 66 is a cross-sectional view of a portion of the tissue manipulation device and colon of FIG. 65;

FIG. 67 is a partial perspective view of another tissue manipulation device embodiment of the present invention inserted into the colon; and

FIG. 68 is a partial perspective view of another tissue manipulation device embodiment of the present invention inserted into the colon.

DETAILED DESCRIPTION

The assignee of the present application also owns the following applications which were contemporaneously filed herewith and which are each herein incorporated by reference in their respective entireties:

U.S. patent application Ser. No. 13/181,779, entitled "Multiple Part Anvil Assemblies For Circular Surgical Stapling Devices"; now U.S. Patent Application Publication No. 2012/0234892;

U.S. patent application Ser. No. 13/181,801, entitled "Specimen Retraction Devices and Methods"; now U.S. Pat. No. 8,632,462;

U.S. patent application Ser. No. 13/181,807, entitled "Modular Occlusion and Tissue Acquisition Mechanisms For Circular Stapling Devices"; now U.S. Patent Application Publication No. 2012/0238829;

U.S. patent application Ser. No. 13/181,831, entitled "Tissue Manipulation Devices"; now U.S. Patent Application Publication No. 2012/0239082;

U.S. patent application Ser. No. 13/181,768, entitled "Collapsible Anvil Plate Assemblies For Circular Surgical Stapling Devices"; now U.S. Patent Application Publication No. 2012/0234890;

U.S. patent application Ser. No. 13/181,786, entitled "Circular Stapling Devices With Tissue-Puncturing Anvil Features"; now U.S. Patent Application Publication No. 2012/0234898;

U.S. patent application Ser. No. 13/181,774, entitled "Anvil Assemblies With Collapsible Frames For Circular Staplers"; now U.S. Patent Application Publication No. 2012/0234891;

U.S. patent application Ser. No. 13/181,842, entitled "Rectal Manipulation Devices"; now U.S. Pat. No. 8,734,478;

U.S. patent application Ser. No. 13/181,836, entitled "Surgical Access Devices With Anvil Introduction and Specimen Retrieval Structures"; now U.S. Patent Application Publication No. 2012/0238823; and

U.S. patent application Ser. No. 13/181,827, entitled "Surgical Bowel Retractor Devices"; now U.S. Patent Application Publication No. 2012/0238824.

Certain exemplary embodiments will now be described to provide an overall understanding of the principles of the structure, function, manufacture, and use of the devices and methods disclosed herein. One or more examples of these embodiments are illustrated in the accompanying drawings. Those of ordinary skill in the art will understand that the devices and methods specifically described herein and illustrated in the accompanying drawings are non-limiting exemplary embodiments and that the scope of the various embodiments of the present invention is defined solely by the claims. The features illustrated or described in connection with one exemplary embodiment may be combined with the features of other embodiments. Such modifications and variations are intended to be included within the scope of the present invention.

Reference throughout the specification to "various embodiments," "some embodiments," "one embodiment," or "an embodiment", or the like, means that a particular feature, structure, or characteristic described in connection with the embodiment is included in at least one embodiment. Thus, appearances of the phrases "in various embodiments," "in some embodiments," "in one embodiment", or "in an embodiment", or the like, in places throughout the specification are not necessarily all referring to the same embodiment. Furthermore, the particular features, structures, or characteristics may be combined in any suitable manner in one or more embodiments. Thus, the particular features, structures, or characteristics illustrated or described in connection with one embodiment may be combined, in whole or in part, with the features structures, or characteristics of one or more other embodiments without limitation. Such modifications and variations are intended to be included within the scope of the present invention.

The terms "proximal" and "distal" are used herein with reference to a clinician manipulating the handle portion of the surgical instrument. The term "proximal" referring to the portion closest to the clinician and the term "distal" referring to the portion located away from the clinician. It will be further appreciated that, for convenience and clarity, spatial terms such as "vertical", "horizontal", "up", and "down" may be used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and/or absolute.

FIG. 1 illustrates one form of a modular surgical instrument 10 of an embodiment of the present invention. In at least one embodiment, the modular surgical instrument 10 includes a universal actuator handle assembly 20 that is attached to an elongated shaft assembly 60 that is configured for operable attachment to a variety of different surgical tool heads. FIG. 1 illustrates a circular stapling head 310a, the attachment and operation of which will be discussed in further detail below. In the depicted embodiment, the handle assembly 20 operably supports an actuation system generally designated as 100 which is configured to selectively apply various forms of actuation motions to the particular-type of surgical tool head attached thereto. As the present Detailed Description proceeds, those of ordinary skill in the art will appreciate that portions of the various modular surgical instruments disclosed herein may be configured to operably interface with a robotic control system that can provide the requisite actuation motions to the instruments.

In various embodiments, the handle assembly 20 includes two handle case segments 21 that may be interconnected together by suitable fastener arrangements for ease of assembly. The shaft assembly 60 includes an outer shaft casing 70 that is substantially hollow and may be fabricated from two

11

casing segments 72 that are coupled together to form a hollow conduit. The outer shaft casing 70 has a proximal end 74 that is coupled to the handle assembly 20 and an open distal end 76.

The Rotary Drive System

Various embodiments of the modular surgical instrument 10 include a unique and novel transmission or actuation system that facilitates the selective application of a variety of different axial and rotary motions to a particular surgical tool head attached thereto. Referring to FIGS. 2 and 3, one form of actuation system 100 includes a gear plate 110 that is pivotally supported in the handle assembly 20 for selective pivotal travel about a pivot axis PA-PA that is substantially transverse to the instrument's longitudinal axis LA-LA. The gear plate 110 may be pivotally supported within the handle assembly 20 on a pivot shaft 104 that extends between the handle case segments 21. As will be discussed in further detail below, the gear plate 110 is also laterally movable on the pivot shaft 104 from a first rotary drive position to a second axial drive position by a first drive selector switch 130 that is slidably supported between the handle case segments 21. As can be seen in FIG. 3, the first drive selector switch 130 is provided with two downwardly protruding clevis arms 132 that are configured to receive a proximal end portion 112 of the gear plate 110 therebetween. The first drive selector switch 130 extends through slots 22 in the handle case members 21 and have down turned end portions 134 to enable the user to slide the first drive selector switch 130 laterally back and forth (arrow "A" in FIG. 3) within the handle assembly 20 along a selector axis SA-SA that is substantially transverse to the longitudinal axis LA-LA. An "actuator" in the form of a firing trigger 140 is attached to, or otherwise integrally formed with, the gear plate 110 such that the gear plate 110 may be selectively pivoted about the pivot axis PA-PA by squeezing the firing trigger 140 toward the handle assembly 20. The term "actuator" may also encompass a portion of a robotic system configured to apply the requisite actuation motion to the gear plate 110.

As can be further seen in FIG. 2, the gear plate 110 is configured to operably interact with a rotary drive shaft 150 that extends through the outer shaft casing 70 of the elongated shaft assembly 60 and is rotatably supported therein. In various embodiments the gear plate 110 has a first gear rack 114, a second gear rack 116, and a third gear rack 118 formed thereon. See FIGS. 3A-3C. The rotary drive shaft 150 has a first pinion gear 152 that is adapted for selective meshing engagement with the first gear rack 114 and a second pinion gear 154 that is adapted for selective meshing engagement with the second gear rack 116 and a third pinion gear 156 that is adapted for selective meshing engagement with the third gear rack 118. As will become further apparent as the present Detailed Description proceeds, each gear rack 114, 116, 118 defines a discrete amount of rotary travel that may be applied to the rotary drive shaft 150. For example, the first gear rack 114, when in meshing engagement with the first pinion gear 152, may facilitate an application of a first amount of rotary travel to the rotary drive shaft 150 upon application of an actuation motion to the firing trigger 140. For example, the first gear rack 114 may facilitate a first amount of rotary travel of approximately 0.70" when the firing trigger 140 is pivoted from a starting position to an ending position. The second gear rack 116, when in meshing engagement with the second pinion gear 154, facilitates a second range of rotary travel to the rotary drive shaft 150. For example, the second gear rack 116 may facilitate a second amount of rotary travel of approximately 1.41" when the firing trigger 140 is pivoted from a starting position to an ending or fully depressed posi-

12

tion. The third gear rack 118, when in meshing engagement with the third pinion gear 156, facilitates a third amount of rotary travel of approximately 2.11" when the firing trigger 140 is pivoted from a starting position to an ending or fully depressed position. It will be understood, however, that other numbers and lengths of gear rack and pinion gear arrangements could conceivably be employed to provide other ranges of rotary motion without departing from the spirit and scope of the present invention.

Also in various handle assembly embodiments, a torsion spring 142 is employed to bias the firing trigger 140 to the unactuated position shown in FIG. 1. Thus, in various embodiments, once the surgeon releases the firing trigger 140, the spring 142 returns the firing trigger 140 to the unactuated position and, in doing so, applies a reverse rotary motion to the rotary drive shaft 150. Various forms of known trigger safety arrangements such as those disclosed in U.S. Pat. No. 7,506,791, entitled "Surgical Stapling Instrument With Mechanical Mechanism For Limiting Maximum Tissue Compression", the disclosure of which is herein incorporated by reference in its entirety, may also be employed.

The rotary drive shaft 150 further has a proximal end 160 that is movably supported within the handle assembly for rotary and axial travel therein. In one embodiment, for example, the proximal end 160 of the rotary drive shaft 150 is configured to support a bearing assembly 162 thereon that is constrained to move in axial tracks 170 formed in the handle cases 21. See FIG. 2. The bearing assembly 162 facilitates rotation of the rotary drive shaft 150 about the longitudinal axis LA-LA while also facilitating its axial travel within the handle assembly 20 and the outer shaft casing 70 of the shaft assembly 60. As can be seen in FIG. 2, a compression spring 164 serves to axially bias the rotary drive shaft 150 in the distal direction "DD".

As can also be seen in FIGS. 2-6, the rotary drive shaft 150 is hollow and has a distal end portion 180 that is configured to operationally mate with various forms of surgical tool heads attached thereto. As will be discussed in further detail below, the distal end portion 180 has an actuator flange 182 formed thereon that is oriented for engagement by a proximal end of the particular surgical tool head or adapter arrangement coupled thereto. Thus, when a particular surgical tool head is coupled to the shaft assembly 60, its distal end contacts the actuator flange 182 to bias the rotary drive shaft 150 in the proximal direction.

Also in various embodiments, the handle assembly 20 may have a window or opening 25 therein (FIG. 1) that facilitates viewing by the surgeon of an indicator member 190. In various embodiments, the indicator member 190 may comprise a tape member that is flexible enough to axially travel back and forth within the handle assembly 20 and be viewable through the window or opening 25. The tape member 190 is attached to the bearing assembly 162 as can be seen in FIGS. 2 and 4 and has indication indicia thereon that corresponds to the gear rack 114, 116, 118 that is engaged with its corresponding pinion gear 152, 154, 156, respectively. For example, the indicator indicia may comprise a picture, drawing, diagram, model identification number, etc. of the particular surgical tool head that requires the corresponding amount of discrete rotary travel of the rotary drive shaft 150 for actuation purposes.

The Axial Drive Systems

The instrument 10 further includes axial drive arrangements for selectively applying axial actuation motions to the various surgical tool heads attached to the shaft assembly 60. As was discussed above, a first drive selector switch 130 is configured to engage the proximal end portion 112 of the gear

plate 110. Such arrangement permits the first drive selector switch 130 to be used to laterally move the gear plate 110 on the pivot shaft 104 between a first rotary drive position wherein an application of an actuation motion to the firing trigger 140 results in the application of a rotary drive motion to the rotary drive shaft 150 and a second axial drive position wherein an application of an actuation motion to the firing trigger 140 results in the application of an axial drive motion to an axial drive bar 200. More specifically and with reference to FIGS. 2-4, the axial drive bar 200 is coupled to an axial drive linkage 210 that is configured to releasably interface with the gear plate 110. As can be seen in FIG. 3, the gear plate 110 has an engagement lug 120 formed thereon that has a hole 122 that is sized to receive a first engagement pin 212 that protrudes from the axial drive linkage 210. The axial drive bar 200 is pinned to a linkage bar 214 by a pin 216 that extends through the linkage bar 214 into a slot 218 in one of the handle cases 21. As can be most particularly seen in FIG. 3, the first engagement pin 212 is also attached to the linkage bar 214 and protrudes therethrough into a second slot 220 in the handle case 21. A compression spring 222 is supported within the slot 220 to bias the pin 212 within the slot 220 to the starting position shown in FIG. 3. The axial drive bar 200 has a distal end 201 that is configured to engage a corresponding portion of the particular surgical tool head that has been coupled to the modular surgical instrument 10 to apply the requisite amount of axial drive motion thereto.

Thus, to actuate the axial drive bar 200, the surgeon laterally moves the first drive selection switch 130 in the "L" direction to bring the pin 212 into the hole 122 in the gear plate attached lug 120. This action also moves the gear plate 110 to the axial drive position wherein all of the gear racks 114, 116, 118 are out of meshing engagement with their corresponding pinion gears 152, 154, 156 on the rotary drive shaft 150 and the gear plate 110 is in driving engagement with the axial drive bar 200. Thereafter, the surgeon may depress the firing trigger 140 to drive the axial drive bar 200 distally within the outer shaft casing 70 of the shaft assembly 60. When the surgeon releases the firing trigger 140, the springs 222 and 142 bias the gear plate 110, axial drive bar 200 and firing trigger 140 back to the starting position.

As will be discussed in further detail below, various of the surgical tool head embodiments of the present invention require rotary actuation motions to be applied to various portions of the tool head that are axially displaced from each other. Such axial displacement can be relatively small and may be accomplished without completely de-meshing one of the pinion gears 152, 154, 156 from its respective rack gear 114, 116, 118 so that activation of the firing trigger 140 results in the application of rotary motion to the rotary drive shaft 150. In at least one embodiment, a second axial drive switch 230 is employed. In various forms, the second axial drive switch 230 comprises a slider switch that can be slid between multiple positions which correspond to various axial positions of the rotary drive shaft 150. The slide switch 230 may include, for example, a clevis-type arrangement that permits the rotary drive shaft 150 to rotate relative thereto and serves to apply an axial motion to the rotary drive shaft 150 to move it axially within the handle assembly 20 and outer casing 70 of the shaft assembly 60. See FIG. 1.

Tool Component Acquisition and Operational Adjustment Drive System

Various embodiments of the modular surgical instrument 10 of the present invention include a tool acquisition shaft 240 that axially extends through the rotary drive shaft 150 and is independently movable relative thereto. In various embodiments, the proximal end portion 242 of the tool acquisition

shaft 240 has a series of helical threads 244 thereon that is configured to rotatably interface with a closure nut portion 246 interfacing with an adjustment knob 248 located on the proximal end of the handle assembly 20. Such adjustment knob and closure nut arrangements are known in the art and will not be described in further detail herein. See, e.g., U.S. Pat. No. 7,506,791, the disclosure of which has been herein incorporated by reference. Thus, rotation of the adjustment knob 248 relative to the handle assembly 20 will result in the axial movement of the tool acquisition shaft 240 within the rotary drive shaft 150.

Surgical Tool Heads

As is apparent from the foregoing description, various forms of the modular surgical instrument 10 are well-suited for actuating a variety of different forms of surgical tool heads that may be required, for example, during a single surgical operation—particularly those devices/tool heads that are used to perform different surgical procedures or actions within the colon. Such surgical tool heads may be provided in a kit form wherein the kit includes at least two different surgical tool heads for use with a modular surgical instrument 10. In various embodiments, each surgical tool head has an outer casing that has an attachment stem portion that is sized to be received within the distal end 76 of the outer shaft casing 70 of the shaft assembly 60. The distance in which the attachment stem portion extends into the outer shaft casing 70 will dictate the axial position of the rotary drive shaft 150 and ultimately which pinion gear 152, 154, 156 is brought into meshing engagement with its corresponding gear rack 114, 116, 118 thereby dictating the amount of rotary drive motion applied to the rotary drive shaft 150 upon actuation of the firing trigger 140. Further understanding of this unique feature may be gleaned from reference to FIG. 7.

FIG. 7 illustrates, in general form, three different forms of surgical tool heads 310a, 310b, 310c that each require three different amounts of rotary drive motion for actuation thereof. For example, tool head 310a requires ¼ turn of rotary drive motion to actuate. Tool head 310b requires ½ turn of rotary motion to actuate. Tool head 310c requires one full turn of rotary drive motion to actuate. As can also be seen in that Figure, tool head 310a has an attachment stem 312a that is configured to be inserted into the shaft assembly 60. Thus, when the attachment stem 312a is fully seated in the distal end 76 of the outer shaft casing 70, the end 311a of the attachment stem 310a engages the actuation flange 182 on the rotary drive shaft 150 and biases the rotary drive shaft 150 in the proximal direction "PD" to bring the pinion gear 156 into meshing alignment with its corresponding gear rack 118. Likewise, tool head 310b has an attachment stem 312b that is shorter than attachment stem 312a by distance "a" which corresponds to the distance between the gear rack 118 and 116 as shown. Thus, when the attachment stem 312b is fully seated in the distal end 76 of the outer shaft casing 70, the end 311b of the attachment stem 312b engages the actuation flange 182 and biases the rotary drive shaft 150 in the proximal direction "PD" to bring the pinion gear 154 into meshing alignment with its corresponding gear rack 116. Likewise, tool head 310c has an attachment stem 312c that is shorter than attachment stem 312a by distance "c" which corresponds to the distance between gear racks 118 and 114 and is shorter than attachment stem 312b by distance "b" which corresponds to the distance between the gear racks 116 and 114 as shown. Thus, when the attachment stem 312c is fully seated in the distal end 76 of the outer shaft casing 70, the end 311c of the attachment stem 312c engages the actuation flange 182 on the rotary drive shaft 150 and biases the rotary

15

drive shaft **150** in the proximal direction “PD” to bring the pinion gear **152** into meshing alignment with gear rack **114**.

Various surgical tool head embodiments of the present invention also employ a “bayonet-type” attachment configuration to attach the surgical tool head to the shaft assembly **60**. In particular, as can be seen in FIG. 7, each of the attachment stems **312a**, **312b**, and **312c** are provided with diametrically-opposed outwardly protruding pins **316**. To attach a surgical tool head to the shaft assembly **60**, the user aligns the pins **316** with corresponding bayonet-type slots **377** provided in the distal end **76** of the outer shaft casing **70**. See FIG. 6. Once the pins **316** are aligned with their respective slots **377**, the user inserts the attachment stem portion into the distal end **76** of the outer shaft casing **70** and, when seated therein, rotates the surgical tool head slightly to seat the pins **316** into their respective bayonet slots **377**. In alternate embodiments, the pins may be provided on the outer shaft casing and the slots may be provided in the attachment stems.

Referring to FIGS. 2, 4, 5, and 5A, there is shown a surgical tool head **400** that may be effectively used in connection with the various embodiments of the surgical instruments **10** of the present invention. In this embodiment, the surgical tool head **400** comprises a circular stapler head **410** that only requires axial actuation motion for cutting and stapling tissue. As can be seen in those Figures, the circular stapler head **410** has an outer casing **412** that has an attachment stem portion **414** that is sized to be seated into the distal end **76** of the outer shaft casing **70**. Attachment pins **416** protrude from the attachment stem **414** and are configured to be received within the bayonet slots **377** in the outer shaft casing **70**. A circular staple driver **420** is movably supported within the outer casing **412**. The staple driver **420** operably supports a plurality of surgical staples **422** therein in a known fashion. A tissue cutting member **430** is concentrically supported with the staple driver **420**.

In use, the circular stapler head **410** must be used in conjunction with an anvil **440** to form the staples therein. FIGS. 2, 4, and 5A illustrate (in broken lines) a conventional circular stapler anvil **440**. Those of ordinary skill in the art will appreciate, however, that any of the various collapsible anvil arrangements disclosed in the various patent applications identified above that are presently owned by the assignee of the subject application and which have been incorporated by reference, as well as other anvil arrangements, may be employed. The depicted anvil **440** includes an anvil head **442** that is attached to an anvil stem **444**. The anvil head **442** has a staple-forming surface **446** formed thereon that is adapted for confronting relationship with the surgical staples in the staple head **410**.

Use of the surgical tool head **400** will now be described. Prior to installing the surgical tool head **400** onto the shaft assembly **60** of the modular surgical instrument **10**, the user may bias the first drive selector switch **130** to move the gear plate **110** out of driving engagement with the rotary drive shaft **150** and into driving engagement with the axial drive bar **200**. Thus, when the attachment stem **414** of the surgical tool head **400** is inserted into the distal end **76** of the outer shaft casing **70**, in at least one embodiment, the rotary drive shaft **150** may be biased axially in the proximal direction without regard to the meshing alignment between the pinion gears **152**, **154**, **156** and the gear racks **114**, **116**, **118**. In such circumstances, the stem **414** of the tool head **400** can contact the flange **182** extending from the rotary drive shaft **150** and push the drive shaft **150** axially against the biasing force applied by spring **164**, as described above. In certain other embodiments, the rotary drive shaft **150** may be biased axially in the proximal direction by the attachment stem **414** without first moving the gear plate **110** out of driving engagement

16

with the gears **152**, **154**, **156**. In at least one such embodiment, the proximal end and/or distal end of each gear **152**, **154**, **156** may each include a beveled and/or radiused surface which can facilitate the alignment and/or realignment of the gears **152**, **154**, **156** with their respective gear racks **114**, **116**, **118**, in the event that this is desirable. If the axial motion of the drive bar **200** is desired without the rotation of the rotary drive shaft **150**, the gear plate **110** can be disengaged from the drive shaft via selector switch **130** as described above. In any event, the attachment stem **414** of the surgical tool head **400** can be seated in the outer shaft casing **70** and locked in position using the bayonet-type connection arrangement described above. Furthermore, when the surgical tool head **400** is attached to the shaft assembly **60**, the distal end **201** of the axial drive bar can **200** seatingly engage the circular stapler driver **420**. See FIGS. 2, 4, 5, and 5A. Prior to or after securing the tool head **400** to the shaft assembly **60**, in certain embodiments, the user can rotate the control knob **248** at the proximal end of the handle assembly **20** to distally advance the distal end **250** of the adjustment shaft **240** and to enable the user to install a trocar shaft extension **260** thereon. In at least one embodiment, the trocar shaft extension **260** is configured to removably snap onto the distal end **250** of the adjustment shaft **240**.

In use, the anvil **440** is introduced into the portion of colon to be cut and stapled using any suitable techniques including any conventional surgical techniques, any of the techniques described in the aforementioned patent applications, or any of the techniques disclosed herein. In order to assemble the anvil **440** to the surgical instrument **10**, as described above, the user can insert the portion of the modular surgical instrument **10** supporting the surgical tool head **400** into the colon through the patient’s anus and into the portion of the colon to be resected. The surgeon can then manipulate the modular surgical instrument **10** to bring the trocar shaft extension **260** into retaining engagement with the anvil stem **444**. Once the anvil stem **444** is attached to the trocar shaft extension **260**, the user then rotates the adjustment knob **248** to move the anvil head **442** towards the staple head **410** to capture the tissue to be cut and stapled therebetween. Once the surgeon has moved the anvil head **442** into its final position, the user then squeezes the firing trigger **140** which drives the axial drive bar **200** distally. As the axial drive bar **200** is driven distally, the circular staple driver **420** is driven towards the anvil head **442** thereby driving the surgical staples **422** supported therein into forming engagement with the underside **446** of the anvil head **440** and the cutting knife **430** through the captured tissue. Once the cutting and stapling action has been completed, the user may release the firing trigger **140** to permit the springs **222** and **142** to return the axial drive bar **200** and the firing trigger **140** to the starting position. Thereafter, the surgeon may withdraw the modular surgical instrument **10** from the patient.

FIGS. 8, 9, 11, and 12 illustrate another surgical tool head **500** that may be effectively used in connection with the various embodiments of the modular surgical instrument **10** of the present invention. In this embodiment, the surgical tool head **500** comprises another form of circular stapler head **510**. This surgical tool head embodiment requires the application of a rotary drive motion thereto to cause the surgical tool head to cut and staple tissue. As can be seen in FIGS. 8, 9, 11, and 12, the circular stapler head **510** has an outer casing **512** that has an attachment stem portion **514** that is sized to be seated into the distal end **76** of the outer shaft casing **70**. Attachment pins **516** protrude from the attachment stem **514** and are configured to be received within the bayonet slots **377** in the outer shaft casing **70**. A circular staple driver **520** is movably supported within the outer casing **512**. The staple driver **520**

operably supports a plurality of surgical staples 522 therein on driver 520 or support members 523 in a known fashion. A tissue cutting member 541 is concentrically attached to the staple driver 520. As can also be seen in FIGS. 11 and 12, the staple driver 520 has a stem portion 530 that has at least one and preferably a pair of helical drive slots 532 therein. The drive slots 532 are configured to receive corresponding drive pins 542 therein that protrude from an adapter cap 540. As can be seen in FIG. 10, the distal end 180 of the rotary drive shaft 150 has a splined outer surface 181 or is fitted with fins for non-rotatably interfacing with the adapter cap 540. Thus, when the user inserts the attachment stem 514 into the distal end 76 of the outer shaft casing 70, the adapter cap 540 slides over the distal end portion 180 of the rotary drive shaft 150 such that rotation of the rotary drive shaft 150 results in rotation of the adapter cap 540. See FIG. 13.

Use of the surgical tool head 500 will now be described. Prior to installing the surgical tool head 500 onto the shaft assembly 60 of the modular surgical instrument 10, the user may bias the first drive selector switch 130 on the handle assembly 20 to move the gear plate 110 out of driving engagement with the rotary drive shaft 150. The attachment stem 514 of the surgical tool head 500 is inserted into the distal end 76 of the outer shaft casing 70 and is affixed thereto in the manner described above. Thus, when the attachment stem 514 of the surgical tool head 500 is inserted into the distal end 76 of the outer shaft casing 70, in at least one embodiment, the rotary drive shaft 150 may be biased axially in the proximal direction without regard to the meshing alignment between the pinion gears 152, 154, 156 and the gear racks 114, 116, 118. In such circumstances, the stem 514 of the tool head 500 can contact the flange 182 extending from the rotary drive shaft 150 and push the drive shaft 150 axially against the biasing force applied by spring 164, as described above. In certain other embodiments, the rotary drive shaft 150 may be biased axially in the proximal direction by the attachment stem 514 without moving the gear plate 110 out of driving engagement with the gears 152, 154, 156. In at least one such embodiment, the proximal end and/or distal end of each gear 152, 154, 156 may each include a beveled and/or radiused surface which can facilitate the alignment and/or realignment of the gears 152, 154, 156 with their respective gear racks 114, 116, 118, as appropriate, when the rotary drive shaft 150 is displaced relative to the gear plate 110. In this embodiment, the circular stapling head 510 may require a 1/2 rotary turn, for example, to cut and staple tissue. Thus, in this embodiment, the attachment stem 514 is sized to position the rotary drive shaft 150 such that the pinion gear 154 is in alignment with gear rack 116. In the event that the gear plate 110 had been previously displaced by the selector switch 130, the surgeon may move the selector switch 130 to bring the gear rack 116 into meshing engagement with the pinion gear 154. Prior to or after securing the surgical tool head 500 to the shaft assembly 60, similar to the above, the user may rotate the control knob 248 to distally advance the distal end 250 of the adjustment shaft 240 and to enable the user to install a trocar shaft extension 260 thereto. The trocar shaft extension 260 is configured to removably snap onto the distal end 250 of the adjustment shaft 240.

The anvil 440, for example, is then attached to the trocar shaft extension 260 and is brought into confronting relationship with the staple driver 520 as described above. Once the surgeon has moved the anvil head 442 into the final position, the user then squeezes the firing trigger 140 which rotates the rotary drive shaft 150 and the adapter cap 540 thereon. As the adapter cap 540 rotates, the pins 542, by virtue of their engagement with the slots 532 in the staple driver 520, drive

the staple driver 520 distally. Such axial motion causes the surgical staples 422 to be driven into forming engagement with the underside 446 of the anvil head 442 and the cutting knife 541 to be driven through the captured tissue. Once the cutting and stapling action has been completed, the user may release the firing trigger 140 to permit the springs 142, 222 to return the axial drive bar 200 and the firing trigger 140 to the starting position. Thereafter, the surgeon may withdraw the modular surgical instrument 10 and surgical tool head 500 from the patient.

FIGS. 16 and 17 illustrate another surgical tool head embodiment 600 that may be effectively used in connection with various embodiments of the modular surgical instruments 10 of the present invention. In this embodiment, the surgical tool head 600 comprises a grasper head 610. This embodiment requires the application of a rotary drive motion to actuate the two movable jaws 670, 680 thereof. As can be seen in those Figures, the grasper head 610 has an outer casing 612 that has an attachment stem portion 614 that is sized to be seated into the distal end 76 of the outer shaft casing 70. Attachment pins 616 protrude from the attachment stem 614 and are configured to be received within the bayonet slots 377 in the outer shaft casing 70. The first and second movable jaws 670, 680 are pivotally pinned to the distal end 616 of the casing 612 for pivotal travel about a common pivot axis between an open position (FIG. 16) and a closed position (FIG. 17). The first movable jaw 670 has a first gear portion 672 and the second movable jaw 680 has a second gear portion 682.

As can be seen in FIG. 14, the distal end 180 of the rotary drive shaft 150 has a plurality of (four) fins 184 protruding therefrom for attachment with a gear drive adapter shaft 650. As can be seen in FIGS. 14 and 15, the gear drive adapter shaft 650 has a body portion 652 that has two attachment arms 654 protruding therefrom. Each attachment arm 654 has a hole or dimple 656 therein that is adapted to retainingly engage a corresponding detent 186 formed on the distal end portion 180 of the rotary drive shaft 150. In addition, the distal end of the gear drive adapter shaft 650 has a drive gear 658 formed thereon adapted to meshingly engage the gear portions 672 and 682 on the first and second movable jaws 670, 680 respectively.

Use of the surgical tool head 600 will now be described. Prior to installing the surgical tool head 600 onto the shaft assembly 60 of the modular surgical instrument 10, the user may bias the first drive selector switch 130 on the handle assembly 20 to move the gear plate 110 to a neutral position out of driving engagement with the rotary drive shaft 150. The attachment stem 614 of the surgical tool head 600 is inserted into the distal end 76 of the outer shaft casing 70 and is affixed thereto in the manner described above. In this embodiment, to move the jaws 670, 680 between the open and closed positions, the gear drive adapter shaft 650 may require a 1/4 rotary turn, for example. Thus, the attachment stem 614 is sized to position the rotary drive shaft 150 such that the pinion gear 154 is in alignment with gear rack 116. Thereafter the surgeon may move the first drive selector switch 130 to bring the gear rack 116 into meshing engagement with the pinion gear 154. However, as indicated above, the rotary drive shaft 150 may also be moved axially relative to the gear plate 110 without first moving the gear plate 110 to the neutral position. Prior to securing the surgical tool head 600 to the shaft assembly 60, the user rotates the control knob 248 on the proximal end of the handle assembly 20 to proximally advance the distal end 250 of the adjustment shaft 240 to its proximal-most position. When the attachment stem 614 is inserted into the distal end 76 of the outer shaft casing 70, the gear drive adapter shaft 650

is coupled to the distal end **180** of the rotary drive shaft **150** in the above described manner. The user may then rotate the gear drive adapter shaft **650** to move the jaws **670**, **680** to the closed position by squeezing the firing trigger **140**. When the user releases the firing trigger, a reverse rotary motion will be applied to the gear drive adapter shaft **650** to pivot the jaws **670**, **680** to the open position.

FIGS. **18-20** illustrate another surgical tool head embodiment **700** that may be effectively used in connection with the various embodiments of the modular surgical instruments **10** of the present invention. In this embodiment, the surgical tool head **700** comprises a grasper head **710**. This embodiment requires the application of a rotary drive motion to actuate the two movable jaws **770**, **780** thereof. As can be seen in those Figures, the grasper head **710** has an outer casing **712** that has an attachment stem portion **714** that is sized to be seated into the distal end **76** of the outer shaft casing **70**. Attachment pins **716** protrude from the attachment stem **614** and are configured to be received within the bayonet slots **377** in the outer shaft casing **70**. The first and second movable jaws **770**, **780** are pivotally pinned to the distal end **716** of the casing **712** for pivotal travel about a common pivot axis between an open position (FIG. **18**) and a closed position (FIG. **19**). The first movable jaw **770** has a first actuator rod **772** protruding therefrom and the second movable jaw **780** has a second actuator rod **782** protruding therefrom.

This embodiment employs a rotary adapter member **790** that has a central aperture **792** shaped to non-rotatably receive the distal end portion **180** of the rotary drive shaft **150** therein. See FIG. **20**. When installed as shown in FIGS. **18** and **19**, the first actuator rod **772** extends into a first arcuate actuation slot **794** and the second actuator rod **782** extends into a second arcuate actuation slot **796** in the rotary adapter member **790**. Thus, when the user rotates the rotary drive shaft **150** in the above-described manners, the rotary adapter **790** is also rotated which drives the first and second movable jaws **770**, **780** to the closed position by virtue of the interaction between the first and second actuator rods **772**, **782** and their respective actuation slots **784**, **796**, respectively. When the user releases the firing trigger a reverse rotary motion will be applied to the rotary adapter **790** to pivot the jaws **770**, **780** to the open position.

FIG. **21** illustrates another surgical tool head embodiment **800** that may be effectively used in connection with the various embodiments of the modular surgical instruments **10** of the present invention. In this embodiment, the surgical tool head **800** comprises a circular stapler head **810** that has an outer casing **812** that supports a circular staple cartridge **820** therein. The anvil has been omitted from the Figure for clarity. However, the reader will understand that, except for the differences noted below, the circular stapler head **810** may otherwise operate in the same manner as the stapling heads described above. The circular staple cartridge **820** movably supports an outer circular array **822** of staple drivers **824** and an inner circular array **826** of staple drivers **827**. Each staple driver **824**, **827** supports one or more surgical staples **828** thereon. This embodiment requires the application of a rotary drive motion to a rotary drive assembly **830** that is rotatably supported within the circular staple cartridge **820** and non-rotatably attached to the distal end **180** of the rotary drive shaft **150** in the above-mentioned manners. The rotary drive assembly **830** includes a driver member **832** that is attached thereto that supports an outer driver wedge **834** configured to drivingly engage the drivers **824** and an inner driver wedge **836** configured to drivingly engage the drivers **826** as the rotary drive assembly **830** is rotated. Once the stapler head **810** has been attached to the shaft assembly **60** in the above-

described manner, the user may apply rotary motion to the rotary drive shaft **150** and rotary drive assembly **830**. This embodiment requires a full turn of rotary motion. Thus, the attachment stem **814** of the circular stapler head **810** is sized to move the rotary drive shaft **150** such that the pinion gear **152** is brought into meshing alignment with the gear rack **114**. Rotary motion is then applied to the rotary drive shaft **150** and rotary drive assembly **830** by depressing the firing trigger **140**. As the rotary drive assembly **830** is rotated about the longitudinal axis LA-LA, the outer drive wedge **834** sequentially contacts the outer drivers **824** to sequentially drive the surgical staples **828** supported thereon axially into forming contact with the anvil (not shown). Likewise, as the rotary drive assembly **830** is rotated about the longitudinal axis LA-LA, the inner drive wedge **836** sequentially contacts the inner drivers **826** to sequentially drive the surgical staples **828** supported thereon axially into forming engagement with the anvil. FIG. **22** illustrates a surgical tool head **800'** that comprises a circular stapler head **810'** that is substantially the same as the circular stapler head **810**, except in that embodiment, the drive wedges **834'**, **836'** are integrally formed in the rotary drive adapter **830'**.

FIG. **23** illustrates surgical staples **828** that have been driven "horizontally" through an elastomeric retainer ring **850**. In this context, the term "horizontally" means that the staples are driven in directions that are substantially transverse to the longitudinal axis LA-LA. During at least one surgical technique, the rectal tissue R can be pulled proximally into the distal end **76** of the outer shaft casing **70** and positioned along the inner sidewall thereof. In various circumstances, a grasper can be inserted upwardly through the outer shaft casing **70** and engaged with the rectal tissue R such that the rectal tissue can then be pulled downwardly into the shaft casing **70**. In certain applications, the grasper can include an expandable portion, such as those described herein, for example, which is configured to expand outwardly and engage the rectal tissue. Once engaged with the tissue, the expandable portion of the grasper can be retracted inwardly prior to and/or as the expandable portion is being pulled into the outer shaft casing **70**. Once the rectal tissue R has been suitably positioned, a tool head attached to the surgical instrument **10** can be inserted upwardly through the outer shaft casing **70** and positioned relative to the rectal tissue. In various embodiments, the tool head can comprise an annular staple cartridge including staple cavities and staple drivers which can be configured to eject the staples **828** laterally. In at least one such embodiment, the staples **828** and the staple drivers can be horizontally supported around the circumference of the staple cartridge and, likewise, the drive wedge(s) of the tool head and/or staple cartridge can be orientated horizontally to drivingly contact the staple drivers as the drive assembly is rotated.

Further to the above, in various embodiments, the staple cartridge can further comprise the elastomeric retainer ring **850** positioned around the outer surface of the staple cartridge wherein, as the staples **828** are deployed from the staple cartridge, the staples **828** can penetrate the retainer ring **850**. In various other embodiments, the ring **850** can be positioned relative to the rectal tissue R before the tool head of the surgical instrument is positioned within the outer shaft casing **70**. Once the tool head and staple cartridge are positioned, though, the staples **828** can be driven through the elastomeric retainer ring **850** into the distal end **76** of the outer shaft casing **70** and formed thereby. In at least one such embodiment, the distal end portion **76** of the outer shaft casing **70** may include a hardened anvil insert against which the staples can be deformed. In certain embodiments, the tool head and/or

staple cartridge can comprise one or more drive wedges which are rotated about an axis in order to sequentially deploy, the staples **828** from the staple cartridge. In certain other embodiments, the tool head and/or staple cartridge can include a cone shaped, or frustoconical, drive wedge which can be displaced distally along an axis and cam, or displace, the staple drivers and the staples **828** simultaneously. In any event, the arrangements described herein can deploy staples within a plane that is substantially perpendicular or substantially transverse to the longitudinal tool axis, although other embodiments are envisioned in which the staples are deployed within any other suitably-oriented plane, for example.

Further to the above, referring now to FIG. **24**, a surgical instrument configured to deploy staples horizontally, laterally, radially, or transversely relative to the instrument axis may be used with or without a retaining ring. In such embodiments, the staples **828** can be deployed directly into the rectal tissue **R**. Whether or not a retaining ring is utilized, referring now to FIG. **25**, a stiffening ring can be utilized to at least temporarily stiffen the staple rectal tissue. In various embodiments, a rigid ring **852** can be inserted through the outer shaft casing **70**, for example, and fitted within the rectal tissue adjacent to the staple line in order to hold the overall shape of the rectum. In at least one embodiment, the rigid ring **852** can be comprised of metal, for example. Once the rigid ring **852** is no longer needed, a removal tool can be inserted through the rectum to pull the rigid ring **852** out of the surgical site.

FIG. **26** depicts a diseased specimen **1508** of the colon **1500** after the elastomeric rings **850** have been stapled into each end of the specimen **1508** and the metal rings (if used) have been removed. As can be seen therein, the elastomeric rings **850** serve to bunch up the ends of the diseased specimen **1508** which can reduce the likelihood of depositing diseased cells from inside of the specimen **1508** as it is being removed through the rectum. FIG. **27** illustrates use of a grasper head **900** to pull the diseased colon specimen **1508** through a tube **902** inserted into the rectum. FIG. **28** depicts the colon segments **1502** and **1520** after the specimen or diseased portion **1508** of the colon has been removed. As can be seen in that Figure, a conventional anvil **440** has been inserted through a distal portion **1520** of the colon **1500**. The surgical instrument **10** with a horizontal stapling head of the type described above has been inserted through a port **1501** installed into the patient's anus **1504**.

Various embodiments of the modular surgical instrument **10** may be used in connection with other forms of surgical tool heads that may be employed to uniformly grip and acquire portions of the colon which facilitates better visualization of the portion of the colon to be transected. Such devices may also be used to ensure that the transection is made substantially perpendicular to the colon. In one embodiment, the surgical tool head **1000** comprises an expandable universal port **1010**. See FIGS. **29-32**. The universal port **1010** includes an outer shaft portion **1012** that has an attachment stem **1014** that is configured to be attached to the distal end **76** of the outer shaft casing **70** of a modular surgical instrument **10** of the various types and constructions described above. See FIG. **29**. However, in other embodiments, the outer shaft portion **1012** may comprise a portion of a dedicated installation tool. In one embodiment, a rotary drive shaft extension **1020** is non-rotatably attached to the distal end portion **180** of the rotary drive shaft **150** in the various manners described above. The rotary drive shaft extension **1020** has a rotary drive gear **1022** attached to its distal end. In this embodiment, only a small amount of rotation may be required to actuate the first and second ring stages

of the universal port **1010**. Thus, the attachment stem portion **1014** may be sized relative to the flange **182** on the rotary drive shaft **150** such that the pinion gear **156** and gear rack **118** may be brought into meshing alignment and remain in meshing alignment as the rotary drive shaft **150** is axially moved in the distal direction. Such axial movement brings the rotary drive gear **1022** of the rotary drive shaft extension **1020** into meshing engagement with each of the three ring stages of the universal port **1010** as will be described in further detail below.

As can be seen in FIG. **29**, the universal port **1010** has a first ring stage **1030** that is coupled to a second ring stage **1050** with an attachment feature **1032** that permits relative rotation between the first ring stage **1030** and the second ring stage **1050**. The universal port **1010** further has a third ring stage **1070** that is coupled to the second ring stage **1050** by an attachment feature **1052** that permits relative rotation of those components. In at least one embodiment, the first ring stage **1030** is intended to expand the colon. In the depicted embodiment, the first ring stage **1030** includes an expandable first hub assembly **1034** that has an elastomeric outer ring **1048** supported thereon. As can be seen in FIGS. **30A** and **30B**, the first hub assembly **1034** includes a first central gear hub **1036** that has central gear-receiving aperture **1037** therein that is configured to receive the drive gear **1022** therein. Attached to the first central gear hub **1036** are a plurality of radially extending first spring arms **1038**. Each spring arm **1038** has an inner end **1039** that is pivotally pinned to the first central gear hub **1036** and extends through a corresponding opening **1013** in the outer shaft portion **1012**. See FIG. **30B**. As can be further seen in FIG. **30B**, each spring arm **1038** has an outer end **1040** that has a spring member **1042** pivotally pinned thereto. FIG. **30A** illustrates the first hub assembly **1034** in a collapsed orientation. Upon application of a rotary motion thereto, the hub assembly **1034** opens to the deployed or expanded orientation depicted in FIG. **30B**.

As indicated above, the second ring stage **1050** is attached to the first ring stage **1030** by attachment feature **1032** that permits rotation of the second ring stage **1050** relative to the first ring stage **1030**. In the depicted embodiment, the second ring stage **1050** includes an expandable second hub assembly **1054** that has a second elastomeric Outer ring **1068** supported thereon. As can be seen in FIGS. **31A** and **31B**, the second hub assembly **1054** includes a second central gear hub **1056** that has central gear-receiving aperture **1057** therein that is configured to receive the drive gear **1022** therein. Attached to the second central gear hub **1056** is a plurality of radially extending second spring arms **1058**. Each second spring arm **1058** has an inner end **1059** that is pivotally pinned to the second central gear hub **1056** and extends through a corresponding opening **1015** in the outer shaft portion **1012**. See FIG. **31B**. As can be further seen in FIG. **31B**, each spring arm **1058** has an outer end **1060** that has a spring member **1062** pivotally pinned thereto. In addition, each spring arm **1058** has a tissue gripping barb **1064** attached thereto that, when deployed, extend through openings **1069** in the second elastomeric outer ring **1068**. FIG. **31A** illustrates the second hub assembly **1054** in a collapsed orientation. Upon application of a rotary motion thereto, the second hub assembly **1054** opens to the deployed or expanded orientation depicted in FIG. **31B**. As the spring arms **1058** move to the expanded orientation, the barbs **1064** are caused to rotate outward.

As indicated above, the third ring stage **1070** is attached to the second ring stage **1050** by attachment feature **1052** that permits rotation of the third ring stage **1070** relative to the second ring stage **1050**. In the depicted embodiment, the third ring stage **1070** includes an expandable third hub assembly

1074 that has a third elastomeric outer ring 1088 supported thereon. As can be seen in FIGS. 32A and 32B, the third hub assembly 1074 includes a third central gear hub 1076 that has central gear-receiving aperture 1077 therein that is configured to receive the drive gear 1022 therein. Attached to the third central gear hub 1076 is a plurality of radially extending third spring arms 1078. Each third spring arm 1078 has an inner end 1079 that is pivotally pinned to the second central gear hub 1076 and extends through a corresponding opening 1017 in the outer shaft portion 1012. See FIG. 32B. As can be further seen in FIG. 32B, each spring arm 1078 has an outer end 1080 that has a spring member 1082 pivotally pinned thereto. In addition, each spring arm 1078 has a tissue cutting blade 1084 attached thereto that, when deployed, extend through openings 1089 in the third elastomeric outer ring 1088. FIG. 32A illustrates the third hub assembly 1074 in a collapsed orientation. Upon application of a rotary motion thereto, the third hub assembly 1074 opens to the deployed or expanded orientation depicted in FIG. 32B. As the spring arms 1078 move to the expanded orientation, the cutting blades 1084 are caused to rotate outward through the openings 1089. The inner end 1079 of each spring arm 1078 is configured to lockingly engage the shaft 1012 through the corresponding opening 1017 when in the expanded position, such that upon application of a rotary motion thereto (in a counterclockwise direction in FIG. 32B), the spring arms 1078 lock in the extended position and do not collapse when the tissue cutting blades 1084 engage the tissue to be severed.

Operation of the universal port 1010 will now be described. When used in connection with an embodiment of the surgical instrument 10, the surgeon may rotate the control knob 248 to distally advance the distal end 250 of the adjustment shaft 240 to enable the user to install the rotary drive shaft extension 1020 thereon. The rotary drive shaft extension 1020 is configured to removably snap onto or otherwise removably engage the distal end 250 of the adjustment shaft 240. After the rotary drive shaft extension 1020 has been attached, the universal port 1010 is attached to the distal end 76 of the outer shaft casing 70. In particular, the attachment stem 1014 is seated in the outer shaft casing 70 and locked in position using the bayonet-type connection arrangement described above. Prior to inserting the attachment stem 1014 into the distal end 76 of the outer shaft casing 70, the first drive selector switch 130 is moved to disengage the gear plate 110 out of driving engagement with the rotary drive shaft 150 in the manner described above. When the attachment stem 1014 is fully seated within the shaft assembly 60, the rotary drive gear 1022 on the distal end of the rotary drive shaft extension 1020 is brought into meshing engagement with the opening 1037 in the first hub portion 1036. Once the universal port 1010 has been attached to the shaft assembly 60, the first drive selector switch 130 is actuated to bring the gear rack 118 into meshing engagement with the pinion gear 156. The universal port 1010 may then be introduced into the rectum portion 1502 of the colon 1500 through the patient's anus 1504 to the desired deployment position.

Once the universal port 1010 has been positioned in the desired location within the colon 1500, the surgeon may then expand the first ring stage 1030 by squeezing the firing trigger 140. Such action will apply a first rotary motion to the first hub assembly 1034 causing it to move to the expanded orientation shown in FIG. 30B to thereby expand the first outer ring 1048 into expanding contact with the corresponding inner wall portion of the colon 1500. Once the first ring stage 1030 has been expanded, the user may then slide the second axial drive switch 230 to move the rotary drive shaft 150 distally to bring the drive gear 1022 into meshing engagement

with the second hub portion 1056 of the second ring stage 1050. Such movement of the rotary drive shaft 150 does not disengage the pinion gear 156 from the rack gear 118. Once the drive gear 1022 has meshingly engaged the second hub portion 1056, the surgeon may once again squeeze the firing trigger 140 to impart a second rotary drive motion to the second hub portion 1056. Such action will apply a second rotary motion to the second hub assembly 1056 causing it to move to the expanded orientation shown in FIG. 31B to thereby expand the second outer ring 1068 and deploy the barbs 1064 into retaining engagement with the corresponding portion of the colon 1500 to retain the universal port 1010 in that location. Thereafter, the user may then slide the second axial drive switch 230 to move the rotary drive shaft 150 distally to bring the drive gear 1022 into meshing engagement with the third hub portion 1076 of the third ring stage 1070. Such movement of the rotary drive shaft 150 does not disengage the pinion gear 156 from the rack gear 118. Once the drive gear 1022 has meshingly engaged the third hub portion 1076, the surgeon may once again squeeze the firing trigger 140 to impart a third rotary drive motion to the third hub portion 1076. Such action will apply a third rotary motion to the third hub assembly 1076 causing it to move to the expanded orientation shown in FIG. 32B to thereby expand the third outer ring 1088 and deploy the cutting blades 1064 outwardly through the adjacent colon tissue. As the third ring stage 1070 is rotated, the cutting blades 1064 sever the colon at that location. While the above-described operation of the universal port 1010 employs the use of the modular surgical instrument 10 of various embodiments of the present invention, other embodiments may employ a dedicated tool for actuation of the ring stages of the universal port in the manners described above without departing from the spirit and scope of various embodiments of the present invention.

FIG. 33 illustrates another universal port embodiment 1110 that only employs two of the ring stages employed by universal port 1010. For example, as shown, the embodiment 1110 illustrates use of the first and second ring stages 1030, 1050 that operate in the same manner described above. However, other embodiments contemplate use of the second and third ring stages 1050, 1070. In either case, the universal port 1110 may be fitted with an occlusion cover to prevent infiltration of tissue into the portion of the colon in which the universal port 1110 has been installed. For example, in one embodiment, the distal-most ring stage (either 1050 or 1070) has a diaphragm assembly 1120 attached thereto. FIG. 33A illustrates a centrally disposed segmented diaphragm assembly 1120. In alternative embodiments, a cover or cap 1121 may be attached to the distal-most ring stage (either 1050 or 1070) as shown in FIG. 33B.

FIGS. 34 and 35 illustrate yet another universal port embodiment 1200 of the present invention that may be used in connection with the surgical instrument 10 or with another dedicated instrument capable of applying axial actuation motions thereto. In the depicted embodiment, the universal port 1200 includes an annular port body or outer casing 1212 that has a stem portion 1214 that is configured for removable attachment to the distal end 76 of the outer shaft casing 70 of an embodiment of the surgical instrument 10 in the above-described manner. A deployment drive assembly in the form of a rotary drive hub 1220 is rotatably supported within the outer casing 1212. As can be seen in FIG. 34, the rotary drive hub 1220 has an inner bore wall 1222 that has a pair of helical slots 1224 therein. The slots 1224 are configured to receive a corresponding actuator pin 1232 that is attached to a drive shaft extension 1230 that is attached to the adjustment shaft 240 employing any of the above-described or similar attach-

ment arrangements. Thus, by distally advancing the drive shaft extension **1230** by rotating the control knob **248**, the rotary drive hub **1220** is rotated about the longitudinal axis L.A-LA by virtue of the interaction between the actuator pins **1232** and helical slots **1224**.

As can be seen in FIGS. **34** and **35**, a drive gear **1228** is formed around the outer circumference **1126** of the rotary drive hub **1220**. The drive gear **1228** is supported to meshingly engage with a gear portion **1242** on a plurality of tissue barb assemblies **1240** that are each rotatably supported on an annular support ring **1250** as shown. The tissue barb assemblies **1240** have a hook portion **1246** thereon that are adapted to hookingly engage the colon when the universal port **1200** has been deployed therein. Each hook portion **1246** is configured to protrude through a corresponding opening **1213** in the outer casing **1212**. Thus, application of the axial drive motion to the adjustment shaft **240** ultimately causes the rotary drive hub **1220** to rotate and deploy the hook portions **1246** into the adjacent colon tissue.

FIGS. **36-40** illustrate another universal port embodiment **1400** of the present invention that may be used in connection with an embodiment of the modular surgical instrument **10** or with a dedicated instrument **1310** that has a hollow support shaft **1320** that rotatably supports a rotary drive shaft assembly **1330** therein. Additionally, FIGS. **36** and **40** illustrate use of the surgical instrument **1310** with a hollow support or stiffening tube **1340**, the purpose of which will be discussed in further detail below. As can be seen in FIGS. **36-40**, the hollow support shaft **1320** has a plurality of first support arms **1322** protruding therefrom. The rotary drive shaft assembly **1330** has a substantially blunt distal end **1332** and a plurality of second arms **1334** radially extending therefrom. The drive shaft assembly **1330** is rotatably supported within the support shaft **1320** and is configured to interface with a handle or other source of rotary motion.

In various embodiments, the universal port **1400** has first annular port body in the form of an outer ring portion **1410** and a second annular port body in the form of an inner ring portion **1420**. In at least one form, the inner and outer ring portions **1410**, **1420** are fabricated from a rigid polymer or other suitable material and are attached together as shown to enable the outer ring **1410** to rotate relative to the inner ring **1420**. A flexible sleeve **1412** is attached to the outer circumference of the first ring stage **1410** and extends beyond the proximal end **1413** thereof as shown and preferably is long enough to protrude out of the patient's anus. As will become further apparent as the present Detailed Description proceeds, the sleeve **1412** forms a passageway extending from the universal port **1400** which can make repeated insertions of various surgical instruments into the rectum easier and simpler and may also serve as a wound protector and shield for preventing contact between the extracted specimen and the rectum. Thus, the sleeve **1412** may minimize the likelihood of "seeding" and makes extraction of the diseased specimen easier. In various embodiments, the sleeve **1412** is fabricated from a puncture-resistant weave. In other embodiments, the sleeve has a plastic reducing spiral built therein which could provide the sleeve with "funnel-like" attributes to further the passage of large masses of tissue therethrough.

As can be seen in FIGS. **38** and **39**, the inner ring **1420** has a plurality of barbed sutures **1430** spaced equally around its outer circumference. Each tissue barb **1430** has an end portion **1432** that extends into a corresponding slot **1414** in the outer ring portion **1410**. The slots **1414** are shaped such that when the universal port **1400** is in the un-deployed or insertion state, the end portion **1432** is substantially completely contained within the slot **1414** and when the inner ring **1420**

is rotated relative to the outer ring **1410**, the suture barbs **1430** are deployed therefrom as shown in FIGS. **39** and **40**.

As indicated above, the hollow support shaft **1320** has a plurality of first support arms **1322** radially protruding therefrom and the rotary drive shaft assembly **1330** has a plurality of second support arms **1334** protruding therefrom. As can be seen in FIGS. **40** and **41A-B**, the ends of the first support arms **1322** are adapted to be received within corresponding closed end slot formations **1416** formed along the inner circumference of the outer ring **1410**. Likewise, the ends of the second support arms **1334** are adapted to be received within corresponding closed end slot formations **1426** formed along the inner circumference of the inner ring **1420**.

Use of the universal port **1400** will now be explained. Prior to insertion into the colon, the universal port **1400** is installed onto the tool **1310**. In at least one embodiment, the support shaft **1320** and rotary drive shaft assembly **1330** are axially advanced into the open center area **1402** in the universal port **1400** such that the first support arms **1322** are seated in corresponding slot formation **1416** in the outer ring **1410** and the second support arms **1334** are seated in corresponding slot formations **1426** in the inner ring **1420**. The hollow stiffening tube **1340** may be inserted over the support shaft **1320** to engage the bottom surface of the outer ring **1413**. Once the universal port **1400** has been installed onto the tool **1310** and the stiffening tube **1340** installed as shown, the surgeon may then insert the assembly into the rectum portion **1502** of the colon **1500** through the anus **1504** to bring the universal port **1400** into the desired location within the rectum portion **1502**. See FIG. **42**. Once the surgeon has determined that the universal port **1400** is located in the desired position, a rotary actuation motion is applied to the rotary drive shaft assembly **1330** which rotates the inner ring **1420** relative to the outer ring **1410** and thereby deploys the suture barbs **1430** into the adjacent colon wall to affix the universal port **1400** thereto. Thereafter, the surgeon may then withdraw the surgical tool **1310** out through the stiffening tube **1340** leaving the universal port **1400** and stiffening tube **1340** in position as shown in FIG. **42**. As can be seen in FIG. **42**, the end of the flexible sleeve **1412** extends around the stiffening tube **1340** and out through the patient's anus **1504**. The surgeon may then insert other instruments up through the stiffening tube **1340** (if retained in place) or through the flexible sleeve **1412** (if the stiffening tube **1340** has been removed) and through the opening **1402** in the universal port **1400** to gain access to the colon portions beyond. FIGS. **43** and **44** illustrate the universal port **1400** installed in the rectum **1502** after the stiffening tube **1340** has been removed. In FIG. **43**, the diseased colon portion **1508** has been cut from the distal colon portion **1520**. Both the end **1510** of the diseased portion **1508** and the end **1522** of the distal colon portion **1520** have been stapled shut. Those processes may be performed using the various surgical tools, stapling heads and anvil arrangements of various embodiments of the present invention or they could have been performed using a separate endocutter (not shown) that was inserted through additional ports or openings provided through the abdominal wall.

FIG. **44** illustrates use of a grasping instrument **900** in connection with the universal port **1400** that has been attached within the rectum **1502** of the colon **1500**. In this Figure, the diseased portion **1508** of the colon **1500** has been cut from the distal portion and wax or other suitable material **1512** has been injected over some of the lesions **1511** and a web like covering material **1514** has been placed over other lesions **1513** to prevent seeding. FIG. **45** illustrates use of the grasping device to grab the end **1510** of the diseased portion **1508** to pull it back through the universal port **1400** as shown

in FIG. 46. Thereafter, the diseased portion 1508 may be severed from the rectum 1502 by a conventional tissue cutting instrument that is inserted through another port or opening in the abdominal wall. FIG. 47 illustrates, in somewhat diagrammatic format, a similar arrangement wherein a universal port 1010 or 1110 has been used and the diseased portion 1508 has been pulled down therethrough. In that instance, the surgeon reattaches the surgical instrument 10 or installation tool to the universal port to activate the tissue cutting members 1084 thereof to sever the diseased portion 1508 from the rectum.

In FIG. 48, a conventional metal clamp 1530 has been installed between the rectum portion 1502 and the diseased portion 1508. In the depicted embodiment, the surgeon is using a cutting instrument 1540 to cut the portion 1503 of the colon 1500 located between the universal port 1400 and the clamp 1530. Once the diseased portion 1508 has been separated from the rectum portion 1502, the surgeon may withdraw the severed diseased portion 1508 through the hole 1402 in the universal port 1400. The sleeve 1412 prevents the diseased portion 1508 from contaminating the rectum portion 1502 as it is removed through the anus 1504. Once the diseased portion 1508 of the colon 1500 has been removed, the surgical tools and tool heads disclosed herein may be inserted through the anus 1504 to re-attach the colon portion 1520 to the rectum 1502. In FIG. 49, the diseased portion 1508 has been placed into a pouch 1530 that was inserted through the universal port 1400.

FIG. 50 illustrates one method of removing an anvil 440 from the surgical site after use. In this method, a retrieval instrument 1590 that has a deployable pouch portion 1592 is inserted through another opening or port provided through the abdominal wall. However, those of ordinary skill in the art will appreciate that the surgeon may introduce and remove an anvil 440 through the universal port 1400. In particular, it will be further appreciated that the various collapsible anvil arrangements disclosed in the previously incorporated patent applications are well-suited for this purpose.

Turning to FIGS. 51 and 52, the universal port 1400 and the stiffening tube 1340 are particularly well-suited for use with a retrieval tool embodiment 1560 of the present invention. In various forms, the retrieval tool 1560 comprises a handle portion 1562 that has a hollow retrieval tube 1564 protruding therefrom that defines a conduit passage 1566 extending through the tool to facilitate the passage of tools therethrough. FIGS. 51 and 52 illustrate the passage of a grasping instrument 900 therethrough. Various embodiments further include a flexible sleeve 1570 that has a cinchable distal opening 1572 that is positioned on the distal end 1565 of the retrieval tube 1564. A cinch cord 1574 is attached to around the cinchable opening and extends through a passage 1567 in the retrieval tube 1564 as shown in FIG. 51. FIG. 51 also illustrates use of the retrieval tool 1560 and universal port 1400 for introducing an anvil 440 into the surgical site with a grasping instrument 900. FIG. 52 illustrates the withdrawal of the diseased specimen 1508 into the sleeve 1570 in the retrieval tool 1560. Once the specimen 1508 has been received within the sleeve 1570, the surgeon may cinch the opening 1572 closed by pulling on the cinch cord 1574.

Referring again to FIG. 36, the outer ring portion 1410 and/or the inner ring portion 1420 of the universal port arrangement 1400 can be comprised of a rigid material. In at least one embodiment, the ring portion 1410 and/or the ring portion 1420 can be comprised of plastic, for example. FIG. 53 illustrates an alternative universal port arrangement 1400' that is substantially similar to universal port 1400, except that the inner and/or the outer ring portions 1410, 1420 are fabri-

cated from an elastic material such as, for example, rubber. In such an embodiment, a rigid ring 1470 can be positioned within the universal port 1400' to retain the port 1400' in an expanded orientation during installation. In at least one embodiment, referring now to FIG. 41B, the rigid ring 1470 can be comprised of metal, for example, and can comprise slots 1476 which are sufficiently aligned with the slots 1426 defined in the inner ring 1420 such that the second arms 1334 of the tool 1310 can extend through the slots 1476 into the slots 1426. In at least one such embodiment, the rigid ring 1470 can be sized and configured such that it is closely received within the inner ring portion 1420 in order to hold the ring portions 1410, 1420 in their configurations when the universal port arrangement 1400' is being positioned within the patient's rectum. Thereafter, the rigid ring 1470 can be removed from the port arrangement 1400. In at least one such embodiment, referring again to FIG. 41B, the rigid ring 1470 can comprise a slot 1479 which can be configured to be engaged by a withdrawal tool. In certain embodiments, the surgeon may insert a grasping instrument up through the patient's rectum and grasp the rigid ring 1470 once the tool 1310 has been disengaged and removed from the port arrangement 1400' and it is no longer desirable to pass objects through the universal port 1400'. In any event, once the rigid ring 1470 has been removed from the universal port 1400', the flexible rings 1410, 1420 can flex inwardly and assume a collapsed position, for example. See e.g., FIG. 26.

FIGS. 54-60 illustrate another port 1600 embodiment of the present invention. As can be most particularly seen in FIGS. 55 and 56, the port 1600 has a body portion 1602 that is fabricated from a plurality of flexible slat member 1604. Each slat member 1604 has a distal end 1606 that is journaled on a distal ring 1620. Likewise, each slat member 1604 has a proximal end 1608 that is journaled on a proximal ring 1622. The proximal end portions 1608 are configured to releasably engage a distal end 1662 of a stiffening tube 1660. In particular, in at least one embodiment, a collection of bayonet-type slots 1664 are formed around the outer circumference of the distal end 1662 of the stiffening tube 1660. Such bayonet-type arrangement facilitates releasable attachment of the port 1600 by aligning the proximal end portions 1608 of the slat members 1604 with the slots 1664 and inserting the end portions 1608 and twisting to seat them in the slots 1664. FIG. 55 illustrates the port 1600 in its collapsed state. When in that state, the port 1600 has an outer diameter "OD" and when in an expanded state (FIG. 56), the port 1600 has an overall outer diameter "OD1". The ends of the member have an outer diameter of OD2. In one embodiment, for example, OD may be approximately 20 mm, OD1 may be approximately 65 mm and OD2 may be approximately 40 mm. However, other sizes may be employed.

As can be seen in FIGS. 55 and 56, each slat 1604 has a central portion 1610 that has a slight radius area formed therein and which has a barb deployment hole 1612 there-through. A barbed surgical suture 1630 extends through each barb deployment hole 1612. The sutures 1630 extend through an actuator conduit 1632 as shown in FIG. 54. An actuator 1640, in the form of a tension cable 1642, is attached to the distal ring 1620. Also various embodiments employ a flexible sleeve 1650 that extends around the port body 1602 and is retained in position by an elastic band or ring 1552.

FIG. 54 illustrates use of the port 1600 and the hollow stiffening tube 1660. After the port 1600 has been attached to the distal end of the stiffening tube 1660, the sleeve 1550 is deployed to extend over the stiffening tube 1660 and the actuation conduit 1632. The entire device may then be inserted through the anus 1504 into the rectum portion 1502

of the colon **1500** and oriented in a desired position. As can be seen in FIG. **54**, the sleeve **1550** also protrudes out through the anus **1504**. Once the surgeon has located the port **1600** in the desired position, an actuation motion in the form of tension “T” is applied to the cable **1642** to expand the member **1600**. As the port **1600** expands, the relatively stiff suture barbs **1630** protrude through the holes **1612** in the slats **1604** to engage the colon wall and thereby retain the port **1600** in position.

FIG. **59** illustrates use of a tissue cutting instrument **1540** to cut through the colon portion **1503** that extends between a metal clamp (not shown) and the port **1600**. The surgeon may then sever the diseased portion in the various manners described above and remove them through the expanded port **1600** and out through the stiffening tube **1660**. Thereafter, the surgeon may detach the stiffening tube **1660** from the port **1600** by applying a twisting motion to disengage the bayonet-type connection to enable the stiffening tube to be separated therefrom and pulled out of the anus leaving the sleeve **1650** attached to the port **1600**. As can be seen in FIG. **60** the port **1600** is permitted to collapse to enable the rectum **1502** to return down to smaller diameter.

FIG. **61** illustrates one method of removing the port **1600** using the surgical tool **10** or other surgical circular stapler arrangement. In the depicted embodiment, a retraction adapter shaft **1670** is attached to the distal end **180** of the rotary drive shaft **150** using the various methods described above. The retraction adapter shaft **1670** has a plurality of distal retraction wedges **1674** radially extending from its distal end **1672**. In addition, a plurality of proximal retraction wedges **1676** radially extend therefrom as shown in FIG. **61**. Once the retraction adapter shaft **1670** has been attached as shown, the surgeon may insert the instrument into the rectum **1502** to the position shown in FIG. **61**. As can be seen in that Figure, the distal retraction wedges **1674** are in retracting engagement with the distal ring **1620** and the proximal retraction wedges **1676** engage the proximal ring **1622**. The surgeon may then use the slider switch **230** on the handle assembly **20** (FIG. **1**) and, if necessary the control knob **248** to axially pull the rotary drive shaft **150** and the retraction adapter shaft **1670** proximally. Prior to pulling the adapter shaft **1670** proximally, the surgeon may attach an anvil onto the retraction adapter shaft **1670**, such that the anvil gets pulled into position as the retraction adapter shaft **1670** pulls the port **1600** and attached colon tissue into the central area **401** in the stapling head **400** for example. Those of ordinary skill in the art will appreciate that such arrangement serves to draw the colon tissue into position for cutting and stapling. Thereafter, the stapling head **410** may be actuated as before.

FIGS. **62** and **63** illustrate an alternate port **1700** that has a body portion **1702** with a plurality of suture barbs **1704** protruding therefrom that has been attached to the rectum **1502** as shown. The port **1700** also has a flexible sleeve **1710** attached thereto. This embodiment also employs a retraction adapter shaft **1720** that has distal retraction wedges **1722** thereon. The surgical instrument **10** is otherwise used as described above to draw the port **1700** into the stapling head **400** as shown. As the port **1700** is drawn into the stapling head **400**, the surgeon pulls on the sleeve **1710** such that it disengages from the port **1700** and assumes a position around the stapling head **400**. See FIG. **63**.

FIG. **64** illustrates use of a flexible port member **1800** in connection with a port **1600**. As can be seen in that Figure, the port member **1800** has a flexible outer ring **1802** that has a plurality of overlapping spirally arranged flaps or petal-like members **1806** that serve to close the central area **1804** defined by the ring **1802**, yet permit the passage of objects

therethrough. To install the port member **1800** into the port **1600**, the surgeon may employ a grasping instrument **1820** to insert the port member **1800** into the stiffener shaft **1660** and into the central area of the expanded port **1600**. The port member **1800** may also include a retrieval tab **1810** to enable the surgeon to remove the port member **1800** with the grasping instrument **1820**.

One of the challenges facing surgeons when performing colorectal surgery is the difficulty in making the transection in tight and angulated spaces. Limited visualization, as well as the magnitudes of the forces that may generally be required to transect and seal the colon, add to those challenges. Rather than use a mechanical structure to dilate the head of a modular circular stapler, the tissue manipulation device **1900** of the present invention uses a vacuum to draw the colon down to the shaft diameter. With the colon tissue bound to the vacuum shaft, the manipulation of the shaft can then facilitate relative easy movement of the colon for dissection.

As can be seen in FIGS. **65** and **66**, the tissue manipulation device **1900**, according to at least one embodiment includes a hollow outer shaft **1902** that rotatably supports a vacuum shaft **1910** thereon. The hollow outer shaft **1902** is substantially rigid and is designed to be inserted into the rigid shaft portion **1952** of a ring installation instrument **1950** as will be discussed in further detail below. The vacuum shaft **1910** comprises a proximal attachment collar **1912** that is rotatably affixed to the distal end **1904** of the outer shaft **1902**. A seal **1906** is provided between the distal end **1904** of the outer shaft **1902** and the proximal attachment collar **1912**. The collar **1912** interfaces with a vacuum supply tube **1914** that is attached to a source of vacuum **1916**.

In various embodiments, the vacuum shaft **1910** has a screen section **1918** therein that is attached to the attachment collar **1912**. The screen mesh may comprise stainless steel, titanium, etc. mesh. In at least one embodiment, the screen mesh may be constructed of two layers of screen at a 45 degree rotation to one another in an effort minimize any likelihood of clogging with tissue. The distal end of the screen section **1918** is attached to a seal ring **1920** that is configured to establish a sliding and rotating seal with a central drive shaft member **1930**. As shown in FIGS. **65** and **66**, flexible head member **1932** is attached to the distal end **1931** of the drive shaft **1930**. The flexible head **1932** may be fabricated from rubber or other flexible material and have a slight bias as shown. Such arrangement enables the surgeon to better manipulate portions of the colon during installation and positioning of the instrument **1900**. However, other head configurations could be use. The drive shaft **1930** extends through the outer shaft **1902** and interfaces with a handle or other arrangement that enables the surgeon to apply rotary and axial motions thereto.

As indicated above, the tissue manipulation device **1900** may be used in connection with a ring installation instrument **1950**. As can be seen in FIGS. **65** and **66**, the ring installation instrument **1950** includes a shaft **1952** that has a distal end **1954** that is configured to slidably support an elastic anastomosis ring **1960** thereon. The distal end **1954** of the shaft **1952** further includes a ring deployment member **1956** that is attached to a push rod **1970** that extends through the wall of shaft **1952**.

The tissue manipulation device **1900** may be used as follows. The surgeon first inserts the ring installation instrument **1950** into the rectum through the patient’s anus. Thereafter the tissue manipulation instrument **1900** is inserted through the shaft **1952** and into the colon. The surgeon may then apply an axial motion to the drive shaft **1930** to push a portion of the drive shaft **1930** out of the screened section **1918** to manipu-

31

late the colon into a desirable position. The vacuum shaft **1910** is also advanced distally out of the shaft **1952** to enable the target tissue "TT" to be retrieved. Once the screen section **1918** is positioned adjacent to the target tissue "TT", the surgeon may then apply the vacuum thereto to draw the target tissue "TT" onto the screen section **1918**. Thereafter the vacuum shaft **1910** is drawn back into the outer shaft **1902** and the shaft **1952** of the ring installation instrument **1950**. Such action causes the target tissue "TT" to fold over between the screen section **1918** and the inner wall of the shaft **1952** as shown. Once the target tissue "TT" is positioned between the screen section **1918** the shaft **1952**, the surgeon may then apply a pushing motion to the push rod **1970** to axially advance the ring deployment member in the distal direction to push the anastomosis ring **1960** off of the distal end of the shaft **1952** as shown in FIG. 66.

FIG. 67 illustrates another vacuum shaft embodiment **2000** of the present invention. In at least one form, the vacuum shaft **2000** has a central shaft portion **2010** that has three screen sections **2020** that are interconnected by flexible joints **2022**. The distal end of the shaft portion **2010** has a flexible head portion **2024**. An outer sleeve **2030** may be employed to facilitate ease of insertion and when the shaft **2000** has been properly located the user may withdraw the sleeve **2030** from the device exposing the screen sections **2020**. The screen sections communicate with a source of vacuum as was described above to enable the portions of the colon **1500** to be drawn into engagement therewith to facilitate better manipulation of the colon **1500**.

FIG. 68 illustrates a vacuum shaft embodiment **2000'** that employs spirally arranged screen sections **2020'** that communicate with a source of vacuum. As the tissue is drawn into contact with the screen sections **2020'** the air in the colon is permitted to exit out the vacuum shaft **2000'**.

The various embodiments of the present invention represent a vast improvement over prior surgical methods and devices used to perform colorectal surgery. While several embodiments of the invention have been described, it should be apparent, however, that various modifications, alterations and adaptations to those embodiments may occur to persons skilled in the art with the attainment of some or all of the advantages of the invention. For example, according to various embodiments, a single component may be replaced by multiple components, and multiple components may be replaced by a single component, to perform a given function or functions. This application is therefore intended to cover all such modifications, alterations and adaptations without departing from the scope and spirit of the disclosed invention as defined by the appended claims.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

The invention which is intended to be protected is not to be construed as limited to the particular embodiments disclosed. The embodiments are therefore to be regarded as illustrative rather than restrictive. Variations and changes may be made by others without departing from the spirit of the present

32

invention. Accordingly, it is expressly intended that all such equivalents, variations and changes which fall within the spirit and scope of the present invention as defined in the claims be embraced thereby.

What is claimed is:

1. A modular circular surgical instrument comprising:
 - an actuator for generating an actuation motion;
 - an actuation system configured to generate a plurality of discrete rotary drive motions in response to an application of said actuation motion thereto; and
 - an elongated shaft assembly operably interfacing with said actuation system and configured to be interchangeably attached to a plurality of different surgical tool heads such that upon attachment of a first one of said surgical tool heads thereto, said elongated shaft assembly is caused to interact with said actuation system to impart a first one of said discrete rotary drive motions to said first surgical tool head upon said application of said actuation motion to said actuation system and when a second one of said surgical tool heads is attached to said elongated shaft assembly, said elongated shaft assembly is caused to interact with said actuation system to impart a second one of said discrete rotary drive motions to said second surgical tool head upon said application of said actuation motion to said actuation system, wherein said actuation system is selectively movable between a rotary drive position and an axial drive position, and wherein said elongated shaft assembly comprises:
 - a rotary drive shaft selectively interfacing with said actuation system and configured to operably interface with said first and second surgical tool heads to apply said discrete rotary motions thereto when said first and second surgical tool heads are interchangeably attached to said elongated shaft assembly; and
 - an axial drive shaft selectively interfacing with said actuation system, wherein upon attachment of a third one of said surgical tool heads to said elongated shaft assembly, said elongated shaft assembly is configured to apply an axial drive motion thereto upon said application of said actuation motion to said actuation system, wherein said actuation system comprises a gear plate having a first gear rack thereon and a second gear rack thereon and being selectively movable between said rotary drive position and said axial drive position, wherein said rotary drive shaft has first and second pinion gears thereon and is axially movable relative to said gear plate such that upon attachment of said first surgical tool head to said elongated shaft assembly, said rotary drive shaft is moved by said first surgical tool head to a first axial position, wherein said first pinion gear is in substantial meshing alignment with said first gear rack and when said second surgical tool head is attached to said elongated shaft assembly, said rotary drive shaft is moved by said second surgical tool head to a second axial position, and wherein said second pinion gear is in substantial meshing alignment with said second gear rack.
2. The modular circular surgical instrument of claim 1 wherein said gear plate further comprises a third gear rack and said rotary drive shaft further has a third pinion gear thereon which corresponds to said third gear rack such that upon attachment of said third surgical tool head to said elongated shaft assembly, said third surgical tool head moves said rotary drive shaft to a third axial position, and wherein said third pinion gear is in substantial meshing alignment with said third gear rack.

33

3. A modular circular surgical instrument comprising:
 an actuator for generating an actuation motion;
 an actuation system configured to generate a plurality of
 discrete rotary drive motions in response to an applica-
 tion of said actuation motion thereto; and
 an elongated shaft assembly operably interfacing with said
 actuation system and configured to be interchangeably
 attached to a plurality of different surgical tool heads
 such that upon attachment of a first one of said surgical
 tool heads thereto, said elongated shaft assembly is
 caused to interact with said actuation system to impart a
 first one of said discrete rotary drive motions to said first
 surgical tool head upon said application of said actuation
 motion to said actuation system and when a second one
 of said surgical tool heads is attached to said elongated
 shaft assembly, said elongated shaft assembly is caused
 to interact with said actuation system to impart a second
 one of said discrete rotary drive motions to said second
 surgical tool head upon said application of said actuation
 motion to said actuation system, wherein said elongated
 shaft assembly comprises:
 an outer shaft casing configured to be interchangeably
 coupled to said first and second surgical tool heads;
 and
 a rotary drive shaft supported within said outer shaft
 casing and being rotatably and axially movable
 therein such that when said first surgical tool head is
 coupled to said outer shaft casing, said rotary drive
 shaft is axially moved into a first driving engagement
 position with said actuation system such that upon
 said application of said actuation motion thereto, said
 rotary drive shaft imparts said first discrete rotary
 drive motion to said first surgical tool head, and
 wherein when said second surgical tool head is
 coupled to said outer shaft casing, said second surgi-
 cal tool head axially moves said rotary drive shaft into
 a second driving engagement position with said
 actuation system such that upon said application of
 said actuation motion thereto, said rotary drive shaft
 imparts said second discrete rotary drive motion to
 said second surgical tool head.
4. The modular circular surgical instrument of claim 3
 wherein said elongated shaft assembly further comprises an
 axial drive shaft supported within said outer shaft casing for
 selective axial travel therein and configured for selective driv-
 ing engagement with said actuation system such that upon
 said application of said actuation motion thereto, said axial
 drive shaft imparts an axial motion to any one of said plurality
 of surgical tool heads attached to said outer shaft casing.
5. The modular circular surgical instrument of claim 3
 wherein said outer shaft casing is configured to be inter-
 changeably coupled to any one of said plurality of surgical
 tool heads by a bayonet-type connection.
6. A modular surgical instrument system, comprising:
 a handle assembly;
 a manually-actuatable actuator trigger operably supported
 on said handle assembly and configured to generate an
 actuation motion;
 an actuation system operably supported within said handle
 assembly and configured to generate a plurality of dis-
 crete drive motions in response to an application of said
 actuation motion thereto;
 an elongated shaft assembly, comprising:
 an outer shaft casing having a distal end; and
 a rotary drive shaft operably supported within said outer
 shaft casing and

34

- oriented for selective operable interaction with said actua-
 tion system and wherein said modular surgical instru-
 ment system further comprises:
- a first surgical tool head configured for interchangeable
 attachment to said distal end of said outer shaft casing
 such that upon attachment thereto, said first surgical tool
 head moves said rotary drive shaft to a first drive position
 wherein upon said application of said actuation motion
 to said actuation system, said rotary drive shaft imparts
 a first rotary drive motion to said first surgical tool head
 to cause said first surgical tool head to perform a first
 surgical action;
- a second surgical tool head configured for interchangeable
 attachment to said distal end of said outer shaft casing
 such that upon attachment thereto, said second surgical
 tool head moves said rotary drive shaft to a second drive
 position wherein upon said application of said actuation
 motion to said actuation system, said rotary drive shaft
 imparts a second rotary drive motion to said second
 surgical tool head to cause said second surgical tool head
 to perform a second surgical action that differs from said
 first surgical action; and
- a third surgical tool head configured for interchangeable
 attachment to said distal end of said outer shaft casing
 such that upon attachment thereto, said third surgical
 tool head moves said rotary drive shaft to a third drive
 position wherein upon said application of said actuation
 motion to said actuation system, said rotary drive shaft
 imparts a third rotary drive motion to said third surgi-
 cal tool head to cause said third surgical tool head to per-
 form a third surgical action.
7. The modular surgical instrument system of claim 6
 wherein said actuation system is selectively movable between
 a rotary drive position and an axial drive position and wherein
 said elongated shaft assembly further comprises an axial
 drive shaft operably supported within said outer shaft casing
 such that when said actuation system is in said axial drive
 position and said actuation motion is applied thereto, said
 axial drive shaft applies an axial drive motion to a fourth
 surgical tool head interchangeably attached to said distal end
 of said outer shaft casing.
8. The modular surgical instrument system of claim 7
 wherein said distal end of said outer shaft casing has a pair of
 bayonet-type slots therein and wherein said first, second,
 third and fourth surgical tool heads each has an attachment
 stem portion thereon that has a pair of attachment pins pro-
 truding therefrom for coupling engagement with said bayo-
 net-type slots in said distal end of said outer shaft casing.
9. The modular surgical instrument system of claim 7
 wherein said distal end of said outer shaft casing has a pair of
 attachment pins protruding therefrom and wherein said first,
 second, third and fourth surgical tool heads each has an
 attachment stem portion thereon that has a pair of bayonet-
 type slots therein for coupling engagement with said attach-
 ment pins in said distal end of said outer shaft casing.
10. The modular surgical instrument system of claim 6
 wherein:
 said first surgical action comprises the grasping and
 manipulation of tissue;
 said second surgical action comprises installing a universal
 port within a colon; and
 said third surgical action comprises cutting and fastening
 of tissue.

35

11. A surgical instrument for use with a surgical tool, said surgical instrument comprising:
 an actuator for generating an actuation motion;
 an actuation system configured to generate a plurality of drive motions in response to an application of said actuation motion thereto; and
 an elongated shaft assembly extending distally from said actuation system, said elongated shaft assembly comprising:
 a proximal portion comprising a drive member transitionable from a first position to a second position to interface with said actuation system, wherein said drive member is biased out of engagement with said actuation system in said first position, and wherein said drive member is engaged with said actuation system in said second position; and
 a distal portion positioned distal to said proximal portion, said distal portion separably attachable to the surgical tool, wherein attachment of the surgical tool to said distal portion of said elongated shaft assembly transitions said drive member from said first position to said second position.
12. A surgical instrument, comprising:
 an actuator for generating an actuation motion;
 an actuation system configured to generate a plurality of drive motions in response to an application of said actuation motion thereto; and
 an elongated shaft assembly extending distally from said actuation system, said elongated shaft assembly comprising:
 a proximal portion movable to interface with said actuation system; and
 a distal portion positioned distal to said proximal portion, said distal portion configured to be interchangeably attached to a plurality of surgical tool heads, wherein attachment of one of the plurality of surgical tool heads to said distal portion of said elongated shaft assembly causes said proximal portion to move axially to interface with said actuation system.
13. A surgical instrument for use with a surgical tool, said surgical instrument comprising:
 an actuator for generating an actuation motion;
 an actuation system configured to generate a plurality of drive motions in response to an application of said actuation motion thereto; and

36

- an elongated shaft assembly extending distally from said actuation system, said elongated shaft assembly comprising:
 a proximal portion movable to interface with said actuation system; and
 a distal portion positioned distal to said proximal portion, said distal portion configured to be interchangeably attached to a first surgical tool head and a second surgical tool head, wherein attachment of the first surgical tool head to said distal portion of said elongated shaft assembly transitions said proximal portion a first distance to interface with said actuation system, and wherein attachment of the second surgical tool head to said distal portion of said elongated shaft assembly transitions said proximal portion a second distance to interface with said actuation system, and wherein said first distance is different than said second distance.
14. A surgical instrument, comprising:
 an actuator for generating an actuation motion;
 an actuation system configured to generate a plurality of drive motions in response to an application of said actuation motion thereto;
 an elongated shaft assembly extending distally from said actuation system, said elongated shaft assembly comprising a first drive portion movable to interface with said actuation system; and
 an interchangeable surgical tool head separably couplable to said elongated shaft assembly, wherein said interchangeable surgical tool head comprises a second drive portion movable from a first position to a second position to interface with said actuation system, wherein said second drive portion is disengaged from said actuation system in said first position, wherein said second drive portion is engaged with said actuation system in said second position, where coupling of said interchangeable surgical tool head to said elongated shaft assembly causes said first drive portion to interface with said second drive portion, and wherein said first drive portion is configured to move said second drive portion from said first position to said second position.

* * * * *