




(86) Date de dépôt PCT/PCT Filing Date: 2003/06/13
 (87) Date publication PCT/PCT Publication Date: 2004/01/08
 (45) Date de délivrance/Issue Date: 2013/08/06
 (85) Entrée phase nationale/National Entry: 2004/12/07
 (86) N° demande PCT/PCT Application No.: GB 2003/002570
 (87) N° publication PCT/PCT Publication No.: 2004/003129
 (30) Priorités/Priorities: 2002/06/27 (GB0214846.8);
 2002/11/27 (GB0227649.1)

(51) Cl.Int./Int.Cl. *G01N 1/28* (2006.01),
G01N 1/31 (2006.01), *C12M 3/00* (2006.01)
 (72) Inventeur/Inventor:
 SHARPE, JAMES ALEXANDER, GB
 (73) Propriétaire/Owner:
 MEDICAL RESEARCH COUNCIL, GB
 (74) Agent: KIRBY EADES GALE BAKER

(54) Titre : TRAITEMENT DE SPECIMENS DE TISSUS
 (54) Title: TREATMENT OF TISSUE SPECIMENS

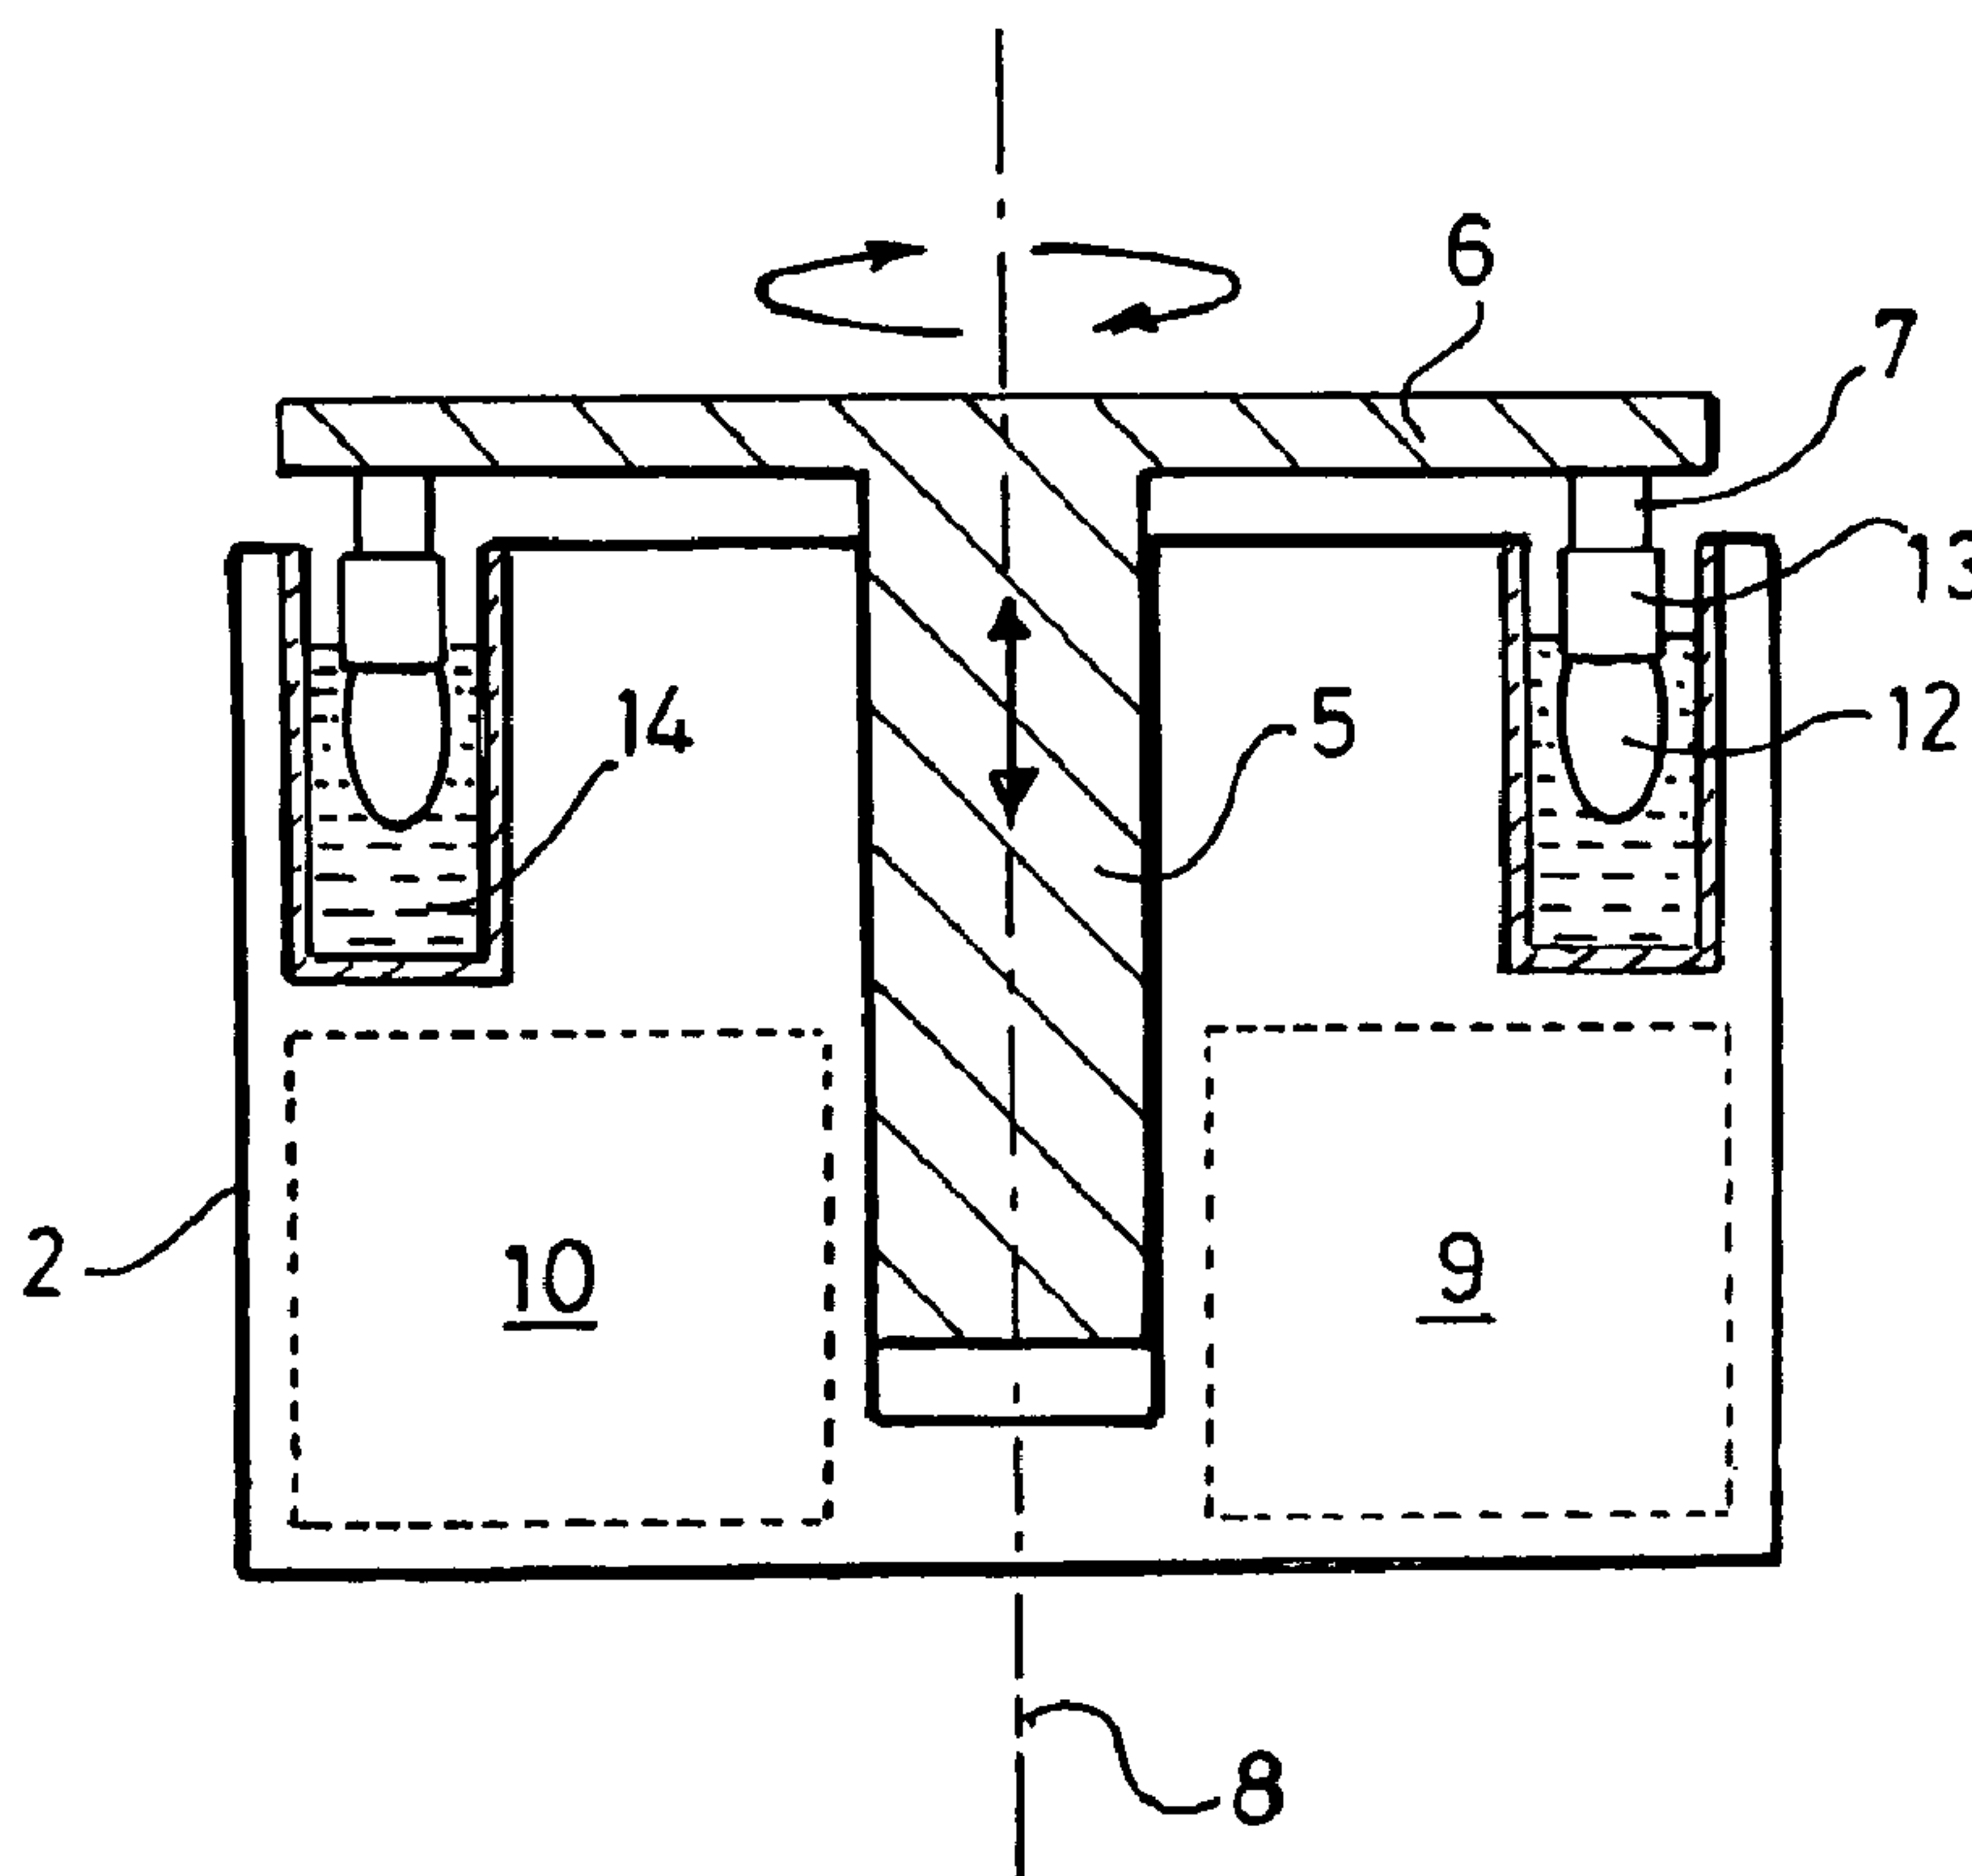

(57) Abrégé/Abstract:

Apparatus for treating tissue specimens comprises a stationary outer casing (2) in the top of which is positioned an annular trough (3) for holding a liquid. Rotatably mounted in the outer casing (2) is a central hub (5) supporting a disc-like lid (6) the underside of which carries a magnet (7). In use, the magnets hold, in a detachable manner, tissue specimens (12) and the trough (3) is filled with a liquid for treating the specimens. The hub (5) is capable of vertical translational movement with respect to the casing (2) to enable the specimens to be lowered into and subsequently lifted out of the trough (3). A method of treating tissue specimens is also provided.



(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau




(43) International Publication Date
8 January 2004 (08.01.2004)

PCT

(10) International Publication Number
WO 2004/003129 A3

- (51) International Patent Classification⁷: G01N 33/50, C12M 3/00, G01N 1/31
- (21) International Application Number: PCT/GB2003/002570
- (22) International Filing Date: 13 June 2003 (13.06.2003)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
0214846.8 27 June 2002 (27.06.2002) GB
0227649.1 27 November 2002 (27.11.2002) GB
- (71) Applicant (for all designated States except US): MEDICAL RESEARCH COUNCIL [GB/GB]; 20 Park Crescent, London W1B 1AL (GB).
- (72) Inventor; and
(75) Inventor/Applicant (for US only): SHARPE, James, Alexander [GB/GB]; 63 Comley Bank Avenue, Edinburgh EH4 1ET (GB).
- (74) Agent: KEITH W NASH & CO; 90-92 Regent Street, Cambridge CB2 1DP (GB).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:
— with international search report
— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments
- (88) Date of publication of the international search report: 26 February 2004
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: TREATMENT OF TISSUE SPECIMENS

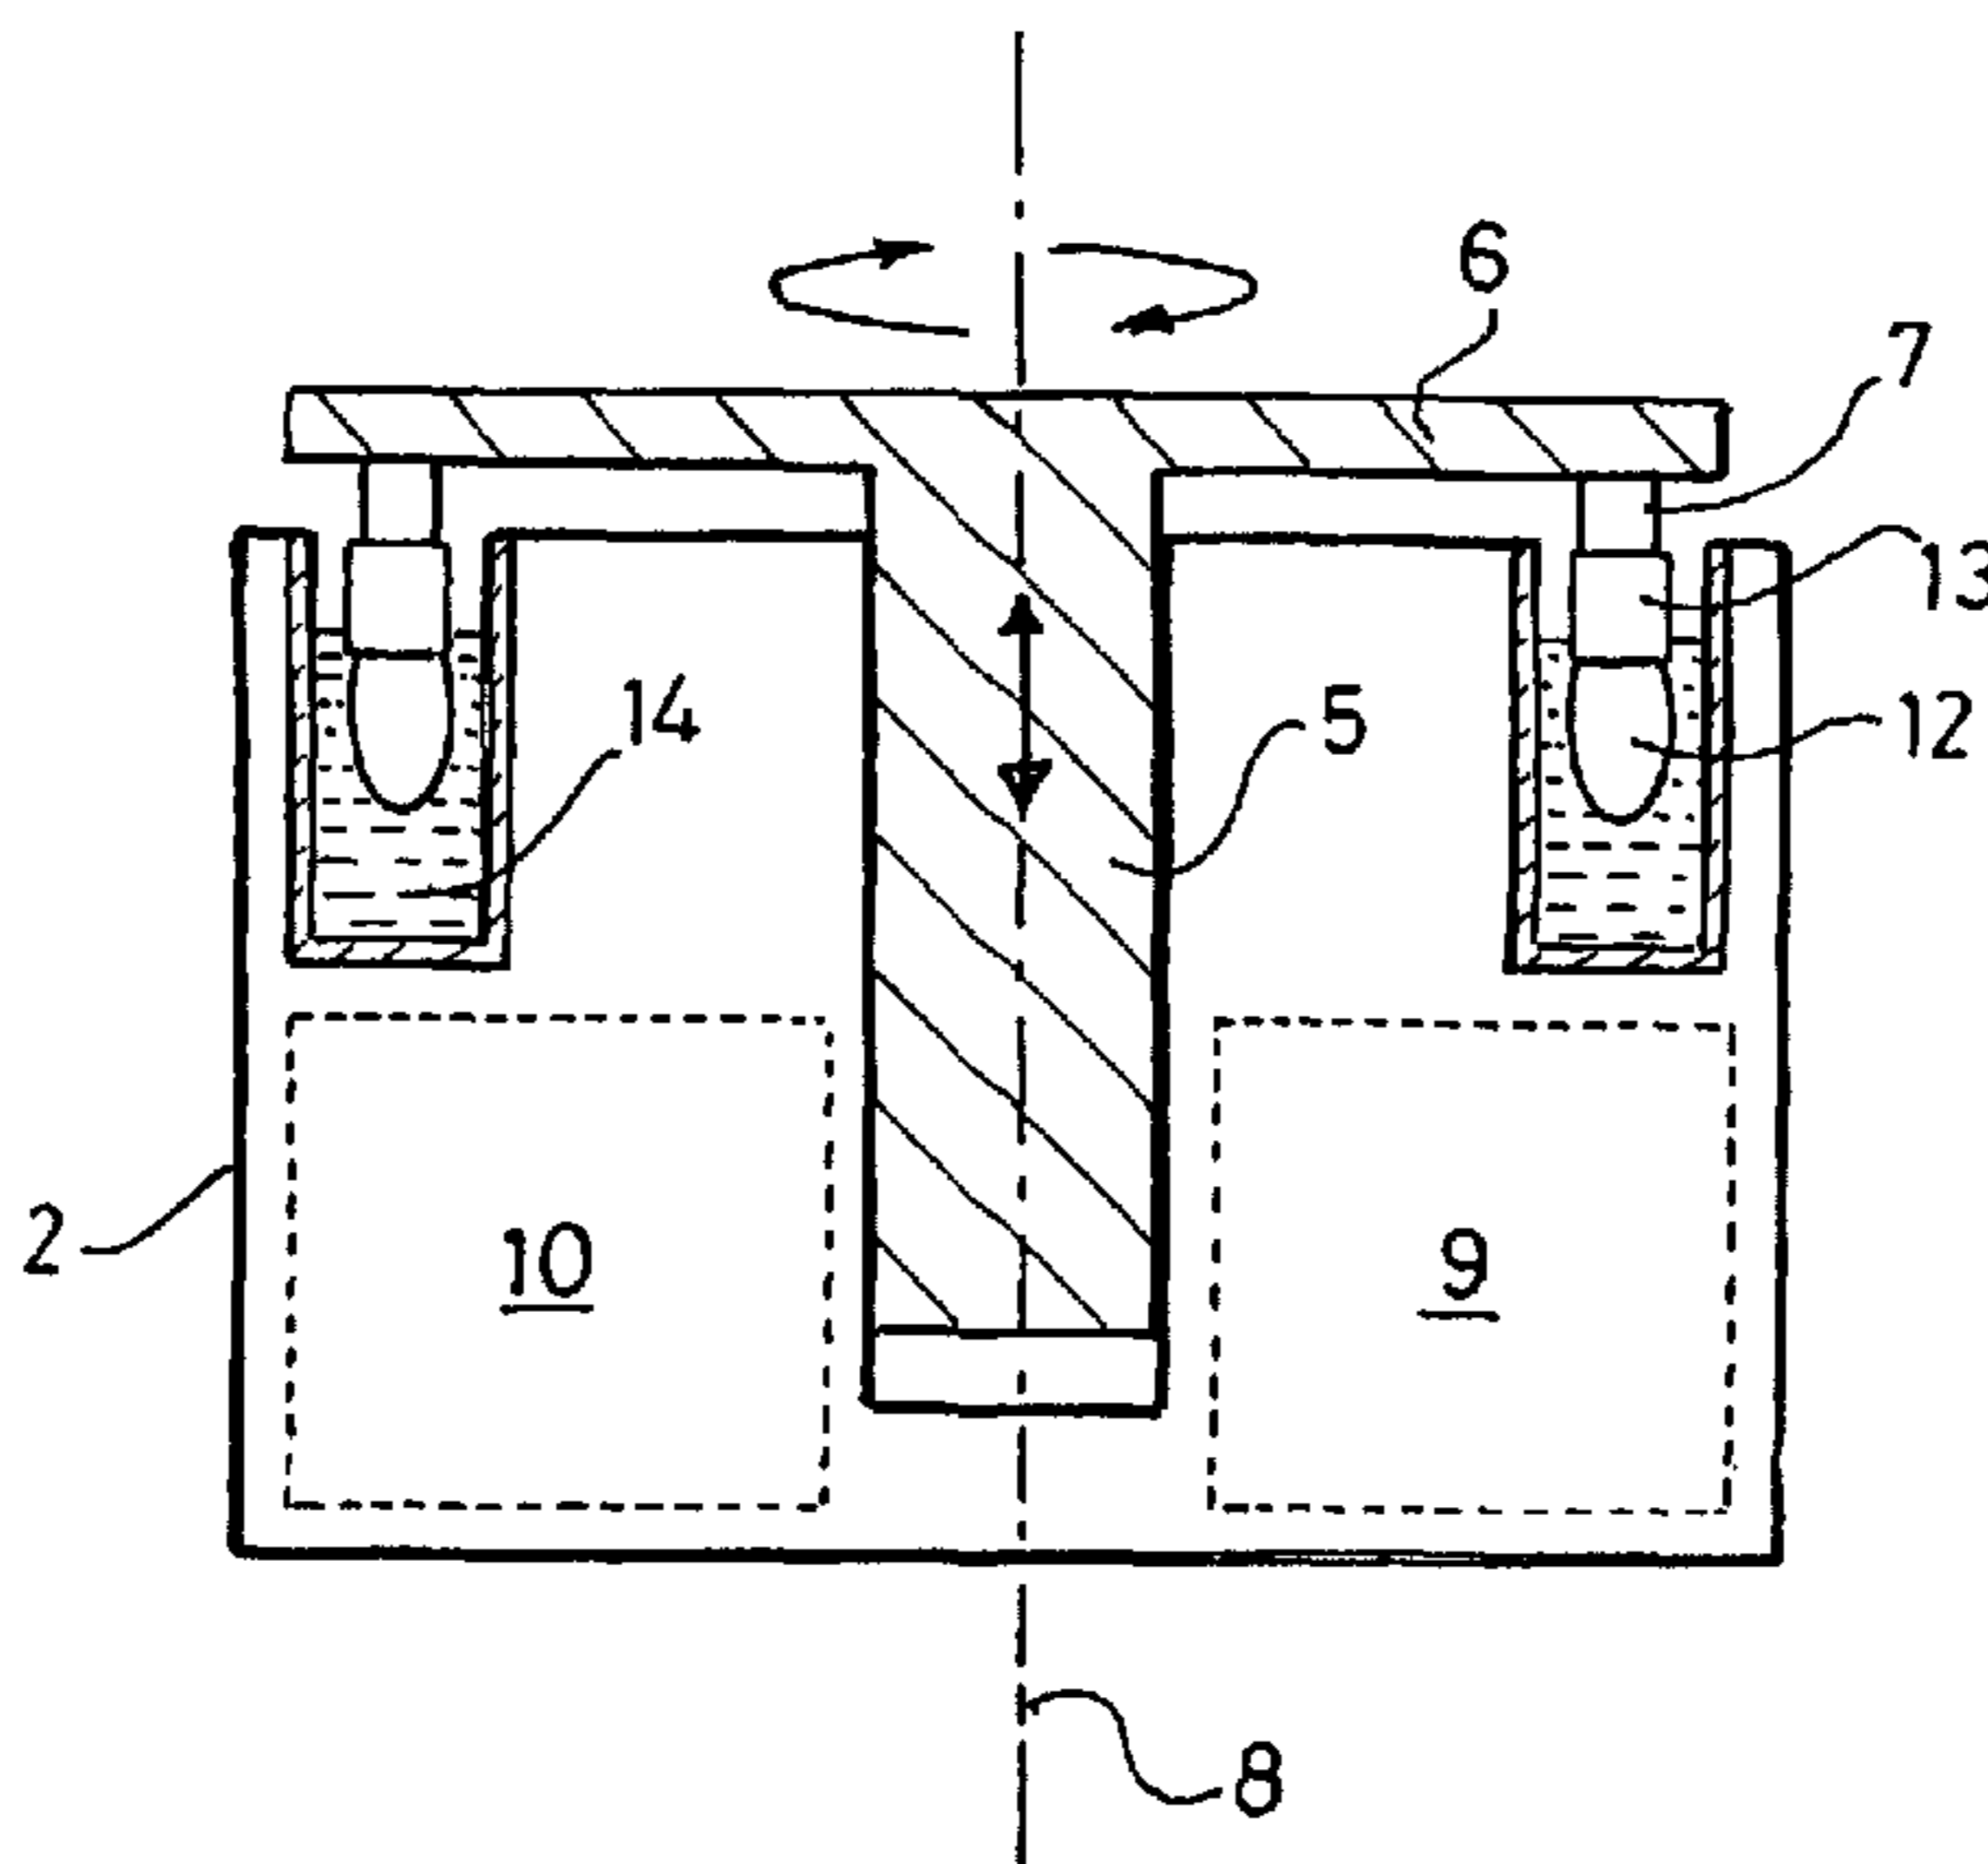

(57) Abstract: Apparatus for treating tissue specimens comprises a stationary outer casing (2) in the top of which is positioned an annular trough (3) for holding a liquid. Rotatably mounted in the outer casing (2) is a central hub (5) supporting a disc-like lid (6) the underside of which carries a magnet (7). In use, the magnets hold, in a detachable manner, tissue specimens (12) and the trough (3) is filled with a liquid for treating the specimens. The hub (5) is capable of vertical translational movement with respect to the casing (2) to enable the specimens to be lowered into and subsequently lifted out of the trough (3). A method of treating tissue specimens is also provided.

WO 2004/003129 A3

TREATMENT OF TISSUE SPECIMENS

Field of the Invention

This invention relates to the treatment of tissue specimens, particularly (but not exclusively) prior to imaging of the specimens by optical projection tomography (OPT), and to uses of optical projection tomography methods and apparatus.

Background to the Invention

Tissue specimens are normally treated by immersion in one or more liquids, before the specimens are imaged in OPT apparatus, and the invention was devised as a way of facilitating this pre-treatment of specimens.

Summary of the Invention

According to one aspect of the invention there is provided apparatus for treating tissue specimens by immersion in a liquid, the apparatus comprising a first structure providing a chamber for holding the liquid, and a second structure including holding means for releasably holding the specimens, the first and second structures being relatively moveable in a direction having a vertical component between a first position in which the holding means are relatively close to the chamber and in which the second structure closes the top of the chamber to enable the specimens to be immersed in the liquid whilst the latter is protected from the environment, and a second position in which the holding means are relatively distant from the chamber to enable the specimens to be loaded onto or unloaded from the holding means; wherein the chamber is in the form of an annular trough, the holding means hold the specimens so that the latter depend from the holding means at angularly spaced positions around a circle and wherein the second structure includes a lid which acts to close the chamber in the first position and the underside of which carries the holding means.

Preferably, the first structure is stationary and the second structure is shiftable vertically with respect to the first structure.

The holding means may include magnets to enable specimens, each provided with a metal mount, to be detachably retained on the second structure by magnetic attraction.

As noted, chamber is in the form of an annular trough in which case the holding means may hold the specimens so that the latter depend from the holding means, conveniently at angularly spaced positions around a circle such that the specimens are lowered into the trough as the second structure is lowered to its first position. In this case, the second structure includes a lid which acts to close the chamber in the first position and the underside of which carries the holding means. Lid closure helps to prevent evaporation of volatile treatment liquids.

The second structure may be rotatably moveable around a central vertical axis, enabling specimens to be loaded onto and unloaded from the second structure at a chosen position alongside the apparatus, either by a robotic arm or a human hand.

The apparatus may have the facility to change the liquid when in the first position, enabling the specimens to be treated by different liquids in a succession of treatment stages, whilst retaining the chamber closed. For example, the apparatus may have a pump to fill and empty the chamber with a succession of chosen liquids which, in the case of tissue specimens, may act to wash or otherwise treat the specimens prior to the specimens being imaged by means of optical projection tomography.

According to another aspect of the invention there is provided a method of treating tissue specimens by immersion in a liquid in a chamber in the form of an annular trough, the method comprising loading the specimens onto a holder carried on the underside of a lid so that the specimens depend from the holder at angularly spaced positions around a circle and are disposed above the liquid in the chamber, effecting relative movement between the chamber and the specimens in one direction to cause immersion of the specimens in the liquid whilst maintaining the chamber closed and protected from the environment during immersion by said lid, effecting relative movement between the chamber and the specimens in the opposite direction to bring the specimens out of the liquid, and unloading the treated specimens from the holder.

The specimens may be treated by different liquids in a plurality of treatment stages which are preferably carried out by successive emptying and filling of the chamber with the different liquids, whilst the specimens remain in the chamber and whilst the chamber remains closed and protected from the environment.

According to another aspect of the present invention, there is provided a method of performing any one or more of the analyses or procedures listed hereunder comprising use of a method or apparatus of any of the aspects set out above.

According to the present invention, samples for use in the present invention may be prepared as described in the earlier patent applications and/or employing conventional pathological and histological techniques and procedures well known to persons skilled in the art.

For example, in-situ hybridisation (particularly useful for detecting RNAs): Hammond K L, Hanson I M, Brown A G, Lettice L A, Hill R E "Mammalian and Drosophila dachsund genes are related to the Ski proto-oncogene and are expressed in eye and limb". Mech Dev. 1998 Jun;74(1-2):121-31.

Immunohistochemistry (particularly useful for detecting proteins and other molecules): Sharpe J, Ahlgren U, Perry P, Hill B, Ross A, Hecksher-Sorensen J, Baldock R, Davidson D. "Optical projection tomography as a tool for 3D microscopy and gene expression studies" Science. 2002 Apr 19;296(5567):541-5.

Brief Description of the Drawings

The invention will now be further described, by way of example, with reference to the accompanying drawings, in which:-

Figure 1 is an isometric view of apparatus according to the invention and in an open condition,

Figure 2 is an isometric view of the apparatus in a closed condition,

Figure 3 is a fragmentary view, to an enlarged scale, of part of the apparatus in an open condition, showing specimens held by the apparatus,

Figure 4 is a cross-sectional view of the apparatus,

Figure 5 shows the apparatus in combination with a robotic arm,

Figure 6 is an enlarged view of part of Figure 5, and

Figure 7 shows the robotic arm positioning a specimen onto the rotary stage of an OPT scanner.

Detailed Description

The apparatus comprises a fixed structure 1 having a cylindrical outer casing 2 in the top of which is positioned an annular trough 3 which is open at the top. Mounted in the fixed structure is a moveable structure 4 having a central hub or spindle 5 on the top of which is mounted a disc-like lid 6 the underside of which carries a number of angularly spaced and downwardly depending cylindrical magnets 7. The hub or spindle 5 is rotatably mounted in the fixed structure for rotation of the moveable structure about a central vertical axis

indicated at 8 in Figure 4. Also, the hub or spindle 5 is capable of vertical translational movement with respect to the fixed structure 1 along the vertical axis 8.

Within the casing 2 are located motors and gearing for driving the structure 4 both in rotation and translational movement, as indicated at 9 in Figure 4. The trough 3 is capable of being filled with liquids, and the structure 1 includes containers for holding these liquids and pumps for filling and emptying the trough, as indicated at 10 in Figure 4.

The magnets 7 are used to hold, in a detachable manner, tissue specimens 12 each of which has been prepared with a metal mount 13 at one end of the specimen. This allows each metal 13 mount to depend from one of the magnets 7, with the specimen 12 depending downwardly from the mount 13. When the apparatus is in the open condition (Figure 1), the magnets 7 are raised clear of the top of the trough 3 so that the specimens 12 can be attached to or removed from the magnets 7. When the apparatus is in the closed position (Figure 2), the lid 6 engages the top of the casing 2 and the specimens 12 are immersed in a liquid 14 in the trough 3.

The robotic arm 15 shown in Figures 6 and 7 is used to load untreated specimens into the apparatus and also to transfer treated specimens from the apparatus to the rotary stage 16 of an OPT scanner where the specimens are imaged.

In use, the robotic arm 15 is used to load specimens into the apparatus, each specimen being attached to the lower end of a corresponding magnet 7 by virtue of the magnetic attraction between the magnet 7 and the metal mount 13 at one end of the specimen 12, the moveable structure 4 being in the open position and being indexed in a rotational sense as the specimens are loaded. When loaded with specimens, the moveable structure is moved to its lowered or closed position, thereby immersing the specimens 12 in the liquid 14 which has been pumped into the trough 3. In this closed position, the lid 6 engages the upper rim of the outer casing 2 so that the liquid 14 is closed to the air, thereby allowing the use of a volatile liquid, unlike known apparatus which uses conveyor belts for transferring specimens through a liquid.

If it is required to treat the specimens by a succession of liquids, the first liquid is drained from the trough 3 and a second liquid pumped thereinto, without the need for the trough 3 to be opened to the air. Moreover, the attachment of the metal mounts 13 to the magnets 7 retains the specimens 12 in their hanging positions so that the specimens do not engage the bottom of the trough 3, which could damage them.

Any number of treatment stages can be carried out in this manner, the liquid being changed without the need to move the specimens and employing only a small volume of each treatment liquid.

After treatment of the specimens 12, the moveable structure 4 is raised to its upper position and the treated specimens 12 are then transferred to the rotary stage 16 by means of the robotic arm 15, the structure 4 being rotationally indexed to enable the robotic arm 15 to unload each specimen 12 in turn and to transfer the treated specimen 5 to the rotary stage 16.

Examples of liquids for treating the specimens are fixatives (such as paraformaldehyde or formalin), alcohols (in particular methanol and ethanol) and organic solvents for clearing the specimens (in particular benzyl alcohol and benzyl benzoate).

CLAIMS

1. Apparatus for treating tissue specimens by immersion in a liquid, the apparatus comprising a first structure providing a chamber for holding the liquid, and a second structure including holding means for releasably holding the specimens, the first and second structures being relatively moveable in a direction having a vertical component between a first position in which the holding means are relatively close to the chamber and in which the second structure closes the top of the chamber to enable the specimens to be immersed in the liquid whilst the latter is protected from the environment, and a second position in which the holding means are relatively distant from the chamber to enable the specimens to be loaded onto or unloaded from the holding means; wherein the chamber is in the form of an annular trough, the holding means hold the specimens so that the latter depend from the holding means at angularly spaced positions around a circle and wherein the second structure includes a lid which acts to close the chamber in the first position and the underside of which carries the holding means.
2. Apparatus according to claim 1, wherein the first structure is stationary and the second structure is shiftable vertically with respect to the first structure.
3. Apparatus according to claim 1 or 2, wherein the holding means include magnets to enable specimens, each provided with a metal mount, to be detachably retained on the second structure by magnetic attraction.
4. Apparatus according to any of claims 1 to 3, wherein the second structure is rotatably moveable around a central vertical axis, enabling specimens to be loaded onto and unloaded from the second structure at a chosen position alongside the apparatus, either by a robotic arm or a human hand.
5. Apparatus according to any of claims 1 to 4, wherein the apparatus has the facility to change the liquid when in the first position, enabling the specimens to be treated by different liquids in a succession of treatment stages, whilst retaining the chamber closed.

6. A method of treating tissue specimens by immersion in a liquid in a chamber in the form of an annular trough, the method comprising loading the specimens onto a holder carried on the underside of a lid so that the specimens depend from the holder at angularly spaced positions around a circle and are disposed above the liquid in the chamber, effecting relative movement between the chamber and the specimens in one direction to cause immersion of the specimens in the liquid whilst maintaining the chamber closed and protected from the environment during immersion by said lid, effecting relative movement between the chamber and the specimens in the opposite direction to bring the specimens out of the liquid, and unloading the treated specimens from the holder.
7. A method according to claim 6, wherein the specimens are treated by different liquids in a plurality of treatment stages.
8. A method according to claim 7, wherein the treatment stages are carried out by successive emptying and filling of the chamber with the different liquids, whilst the specimens remain in the chamber and whilst the chamber remains closed and protected from the environment.

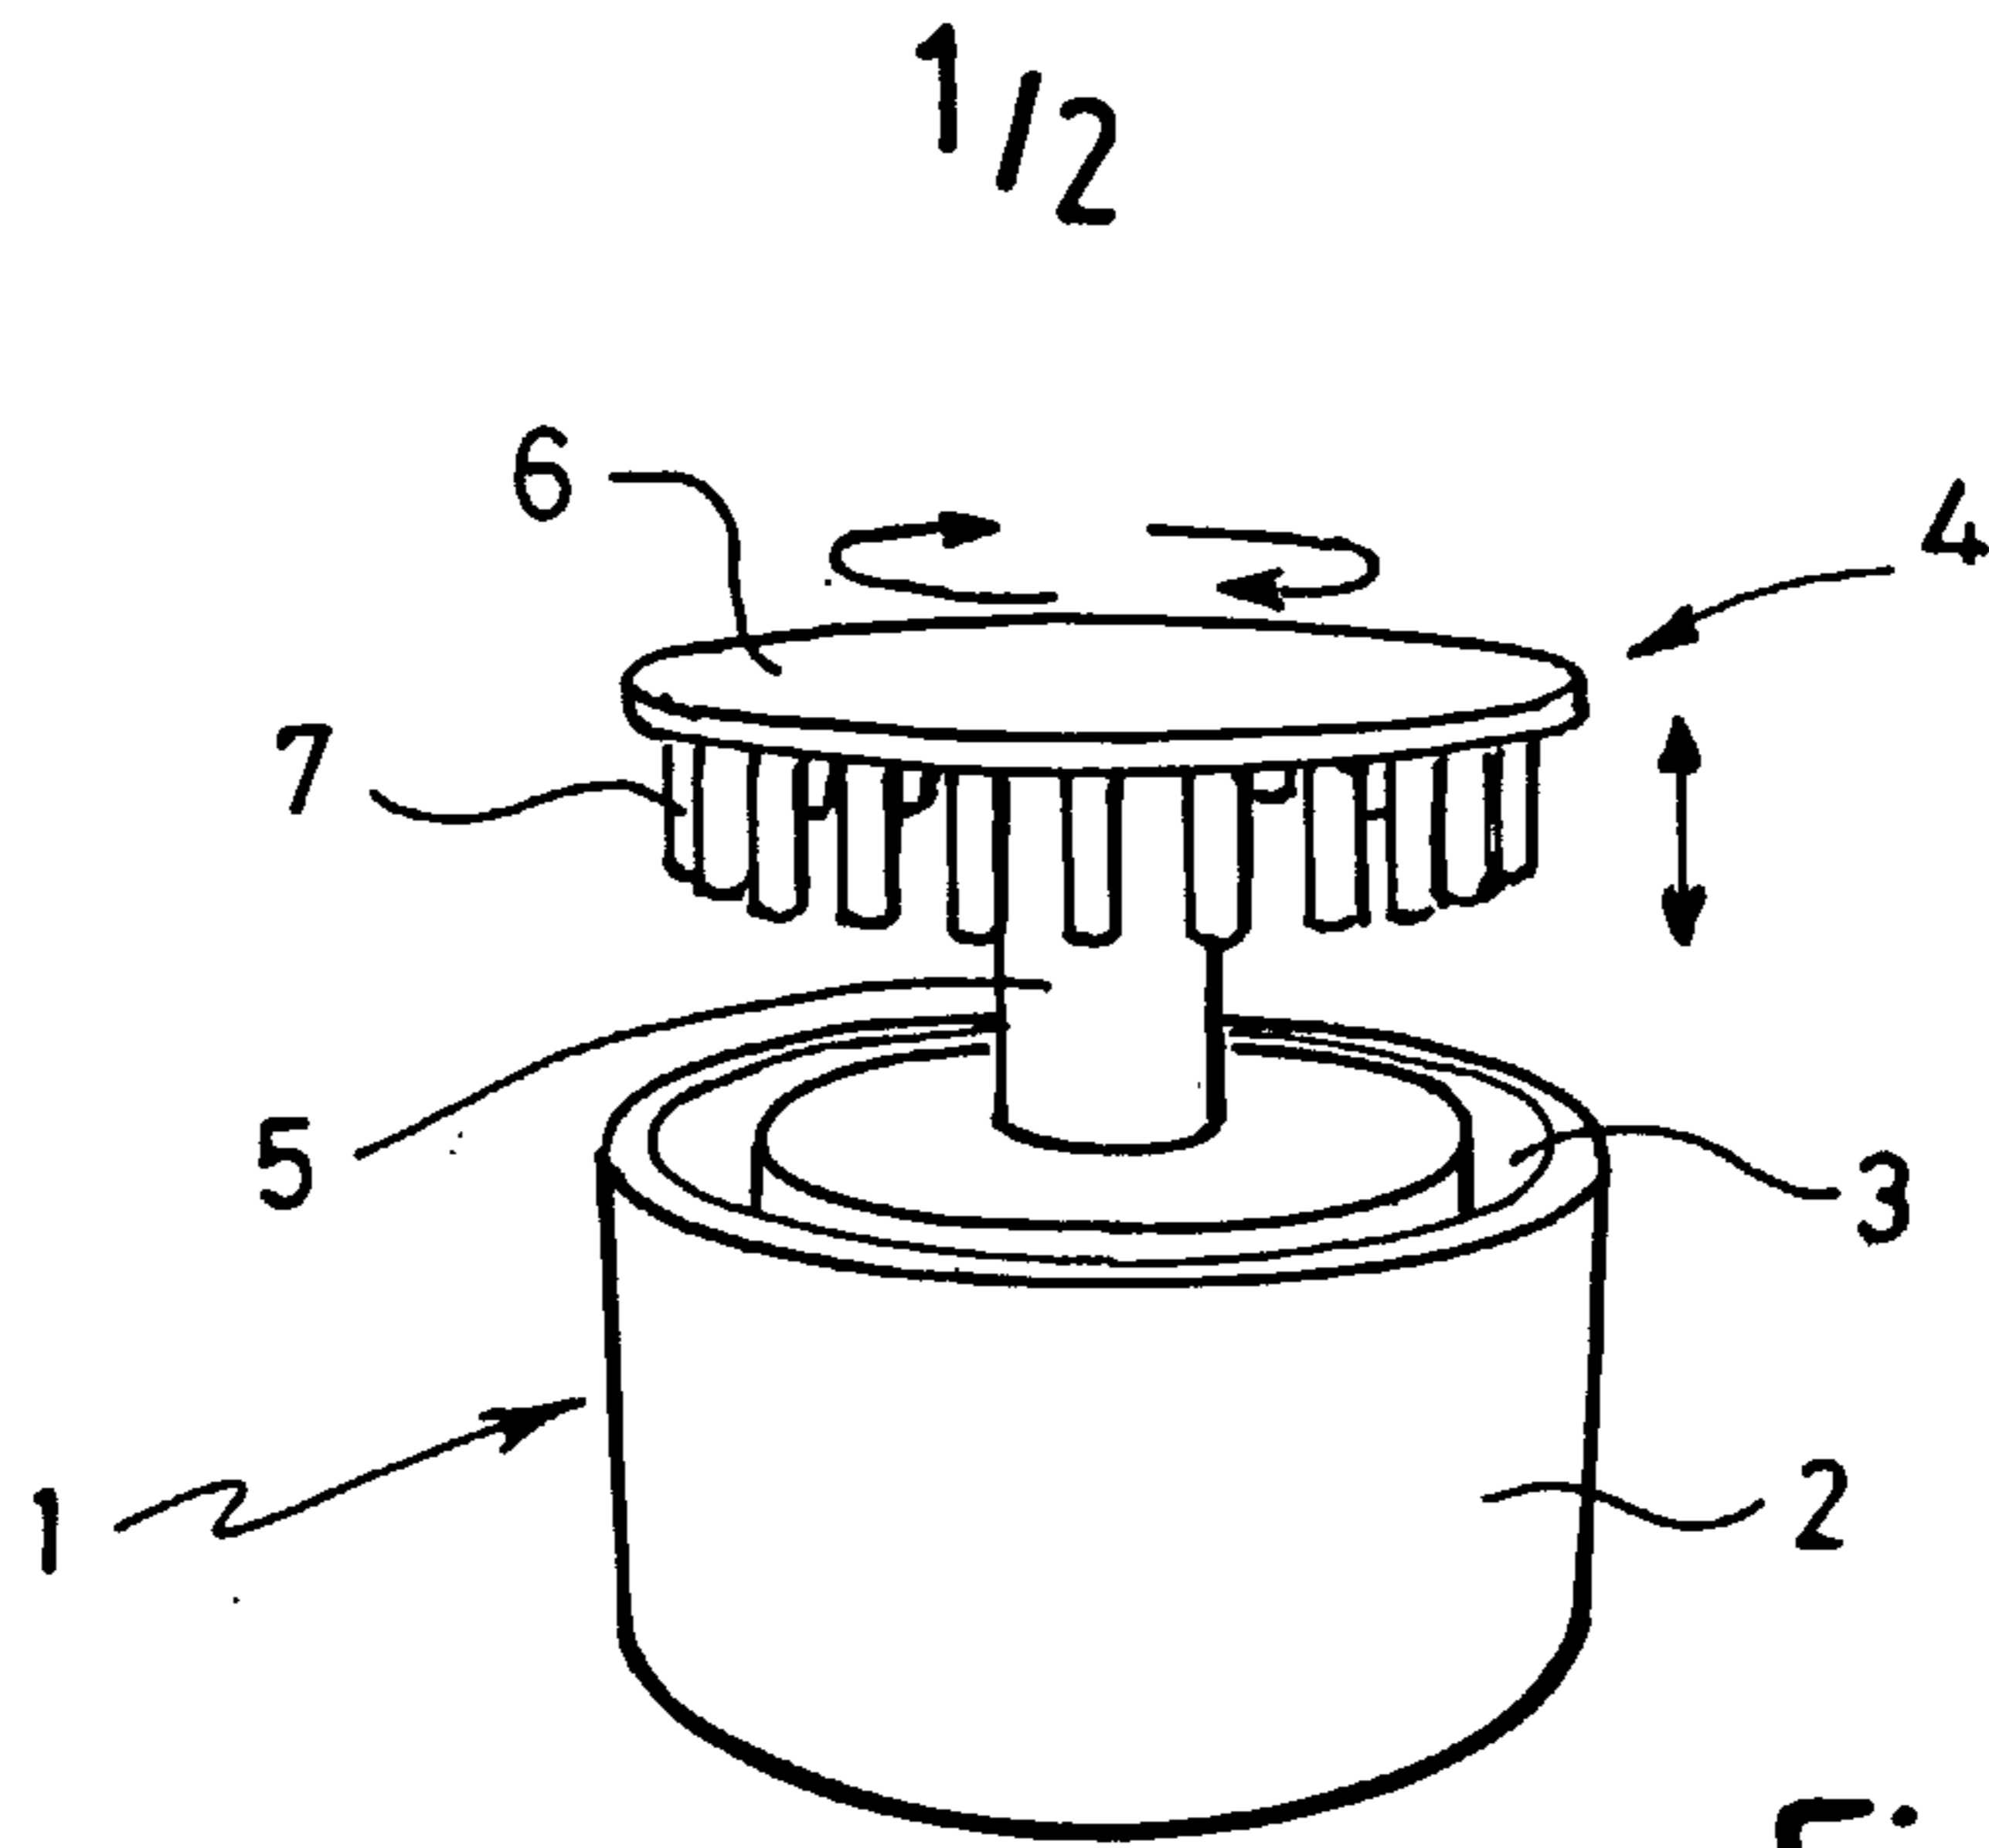


Fig. 1

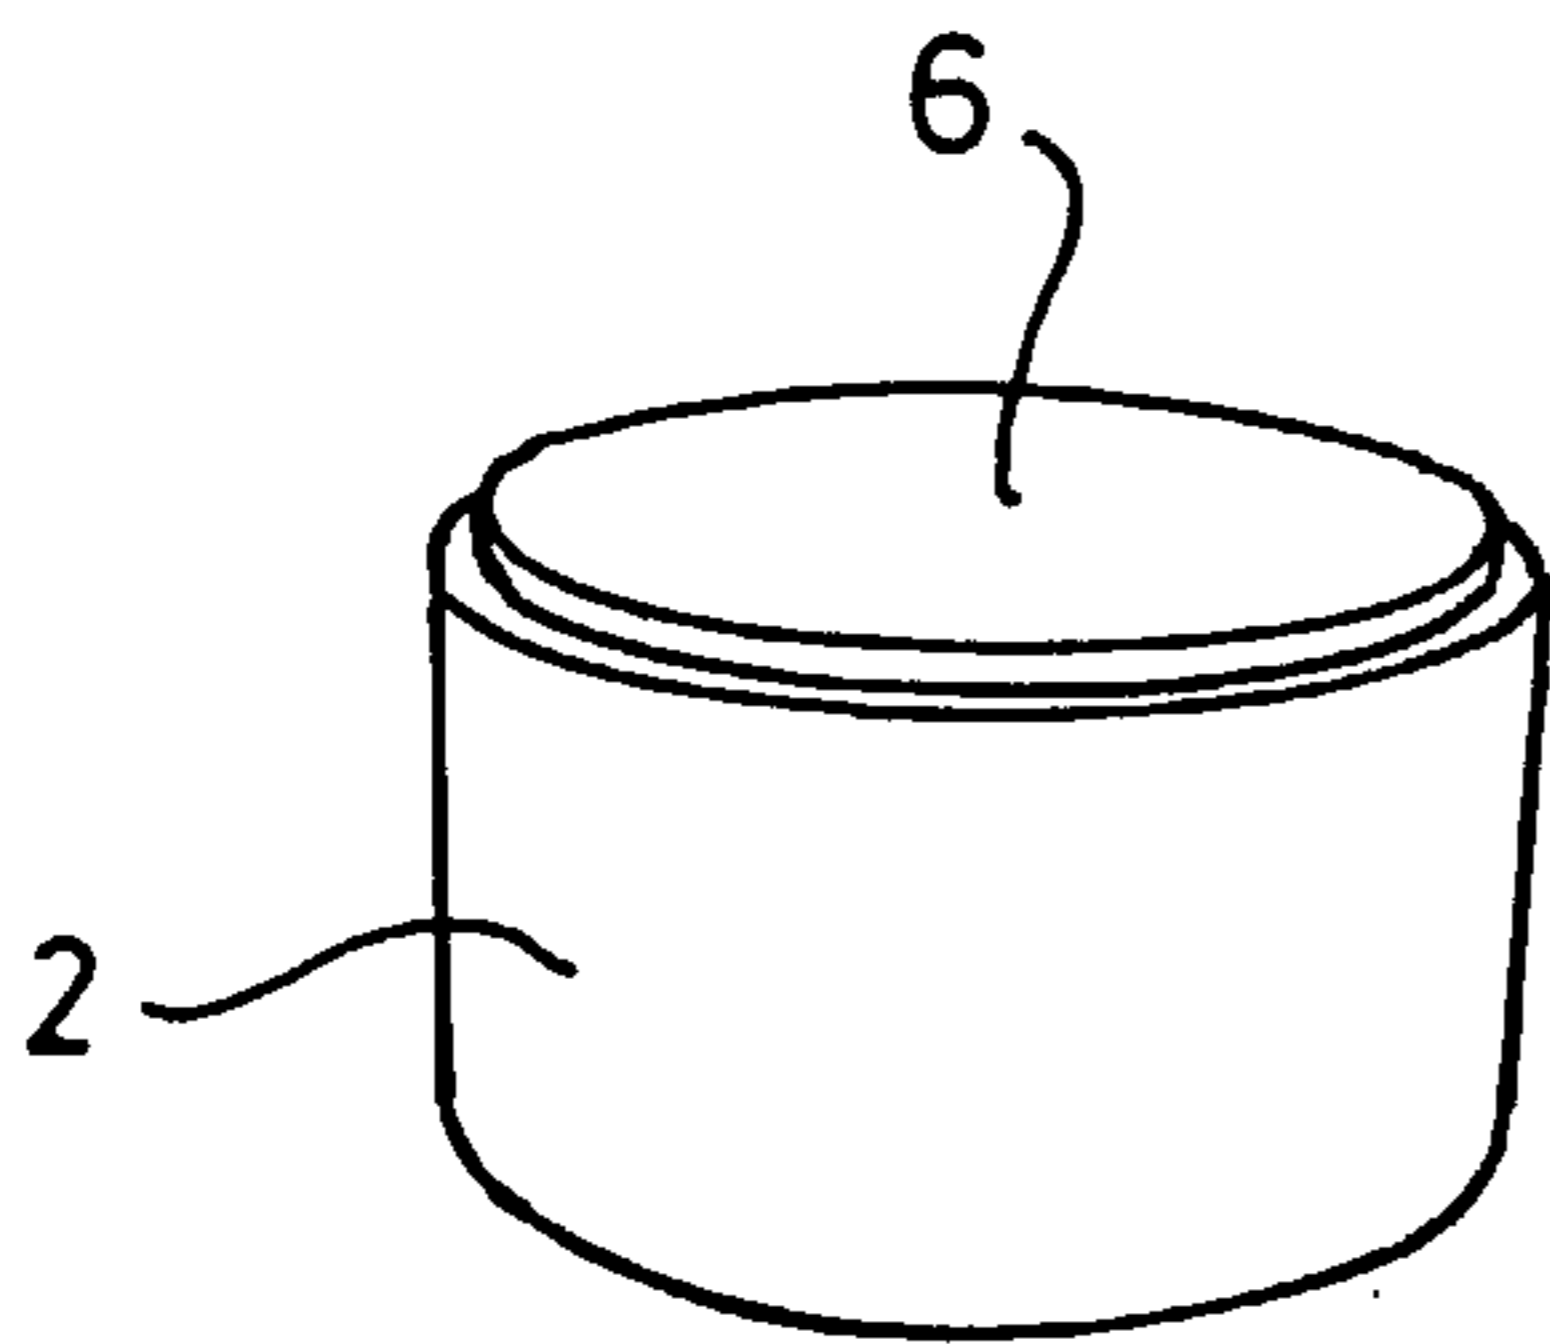


Fig. 2

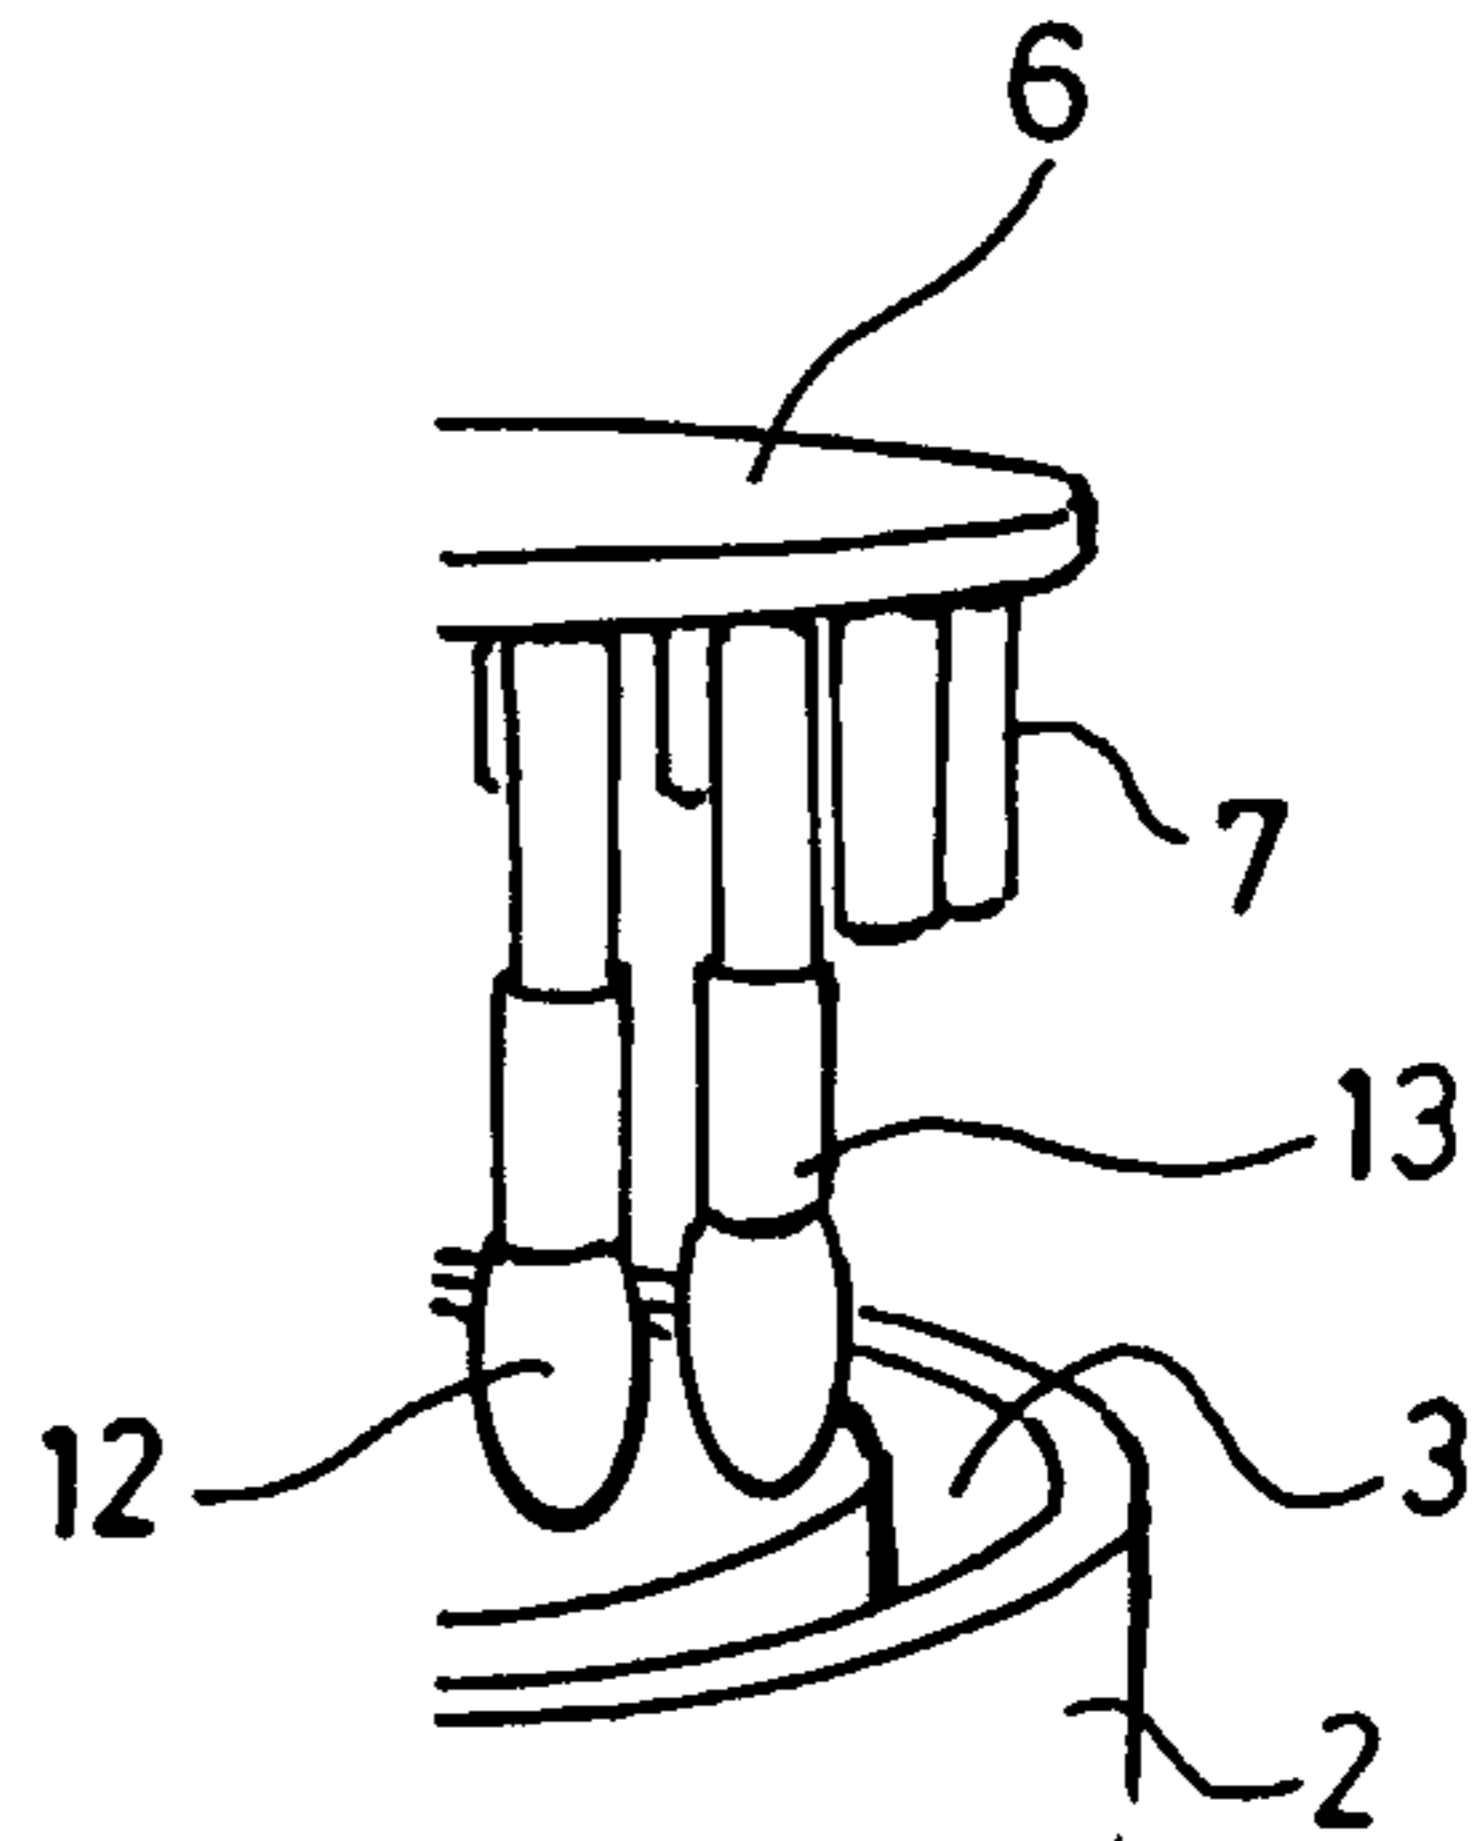


Fig. 3

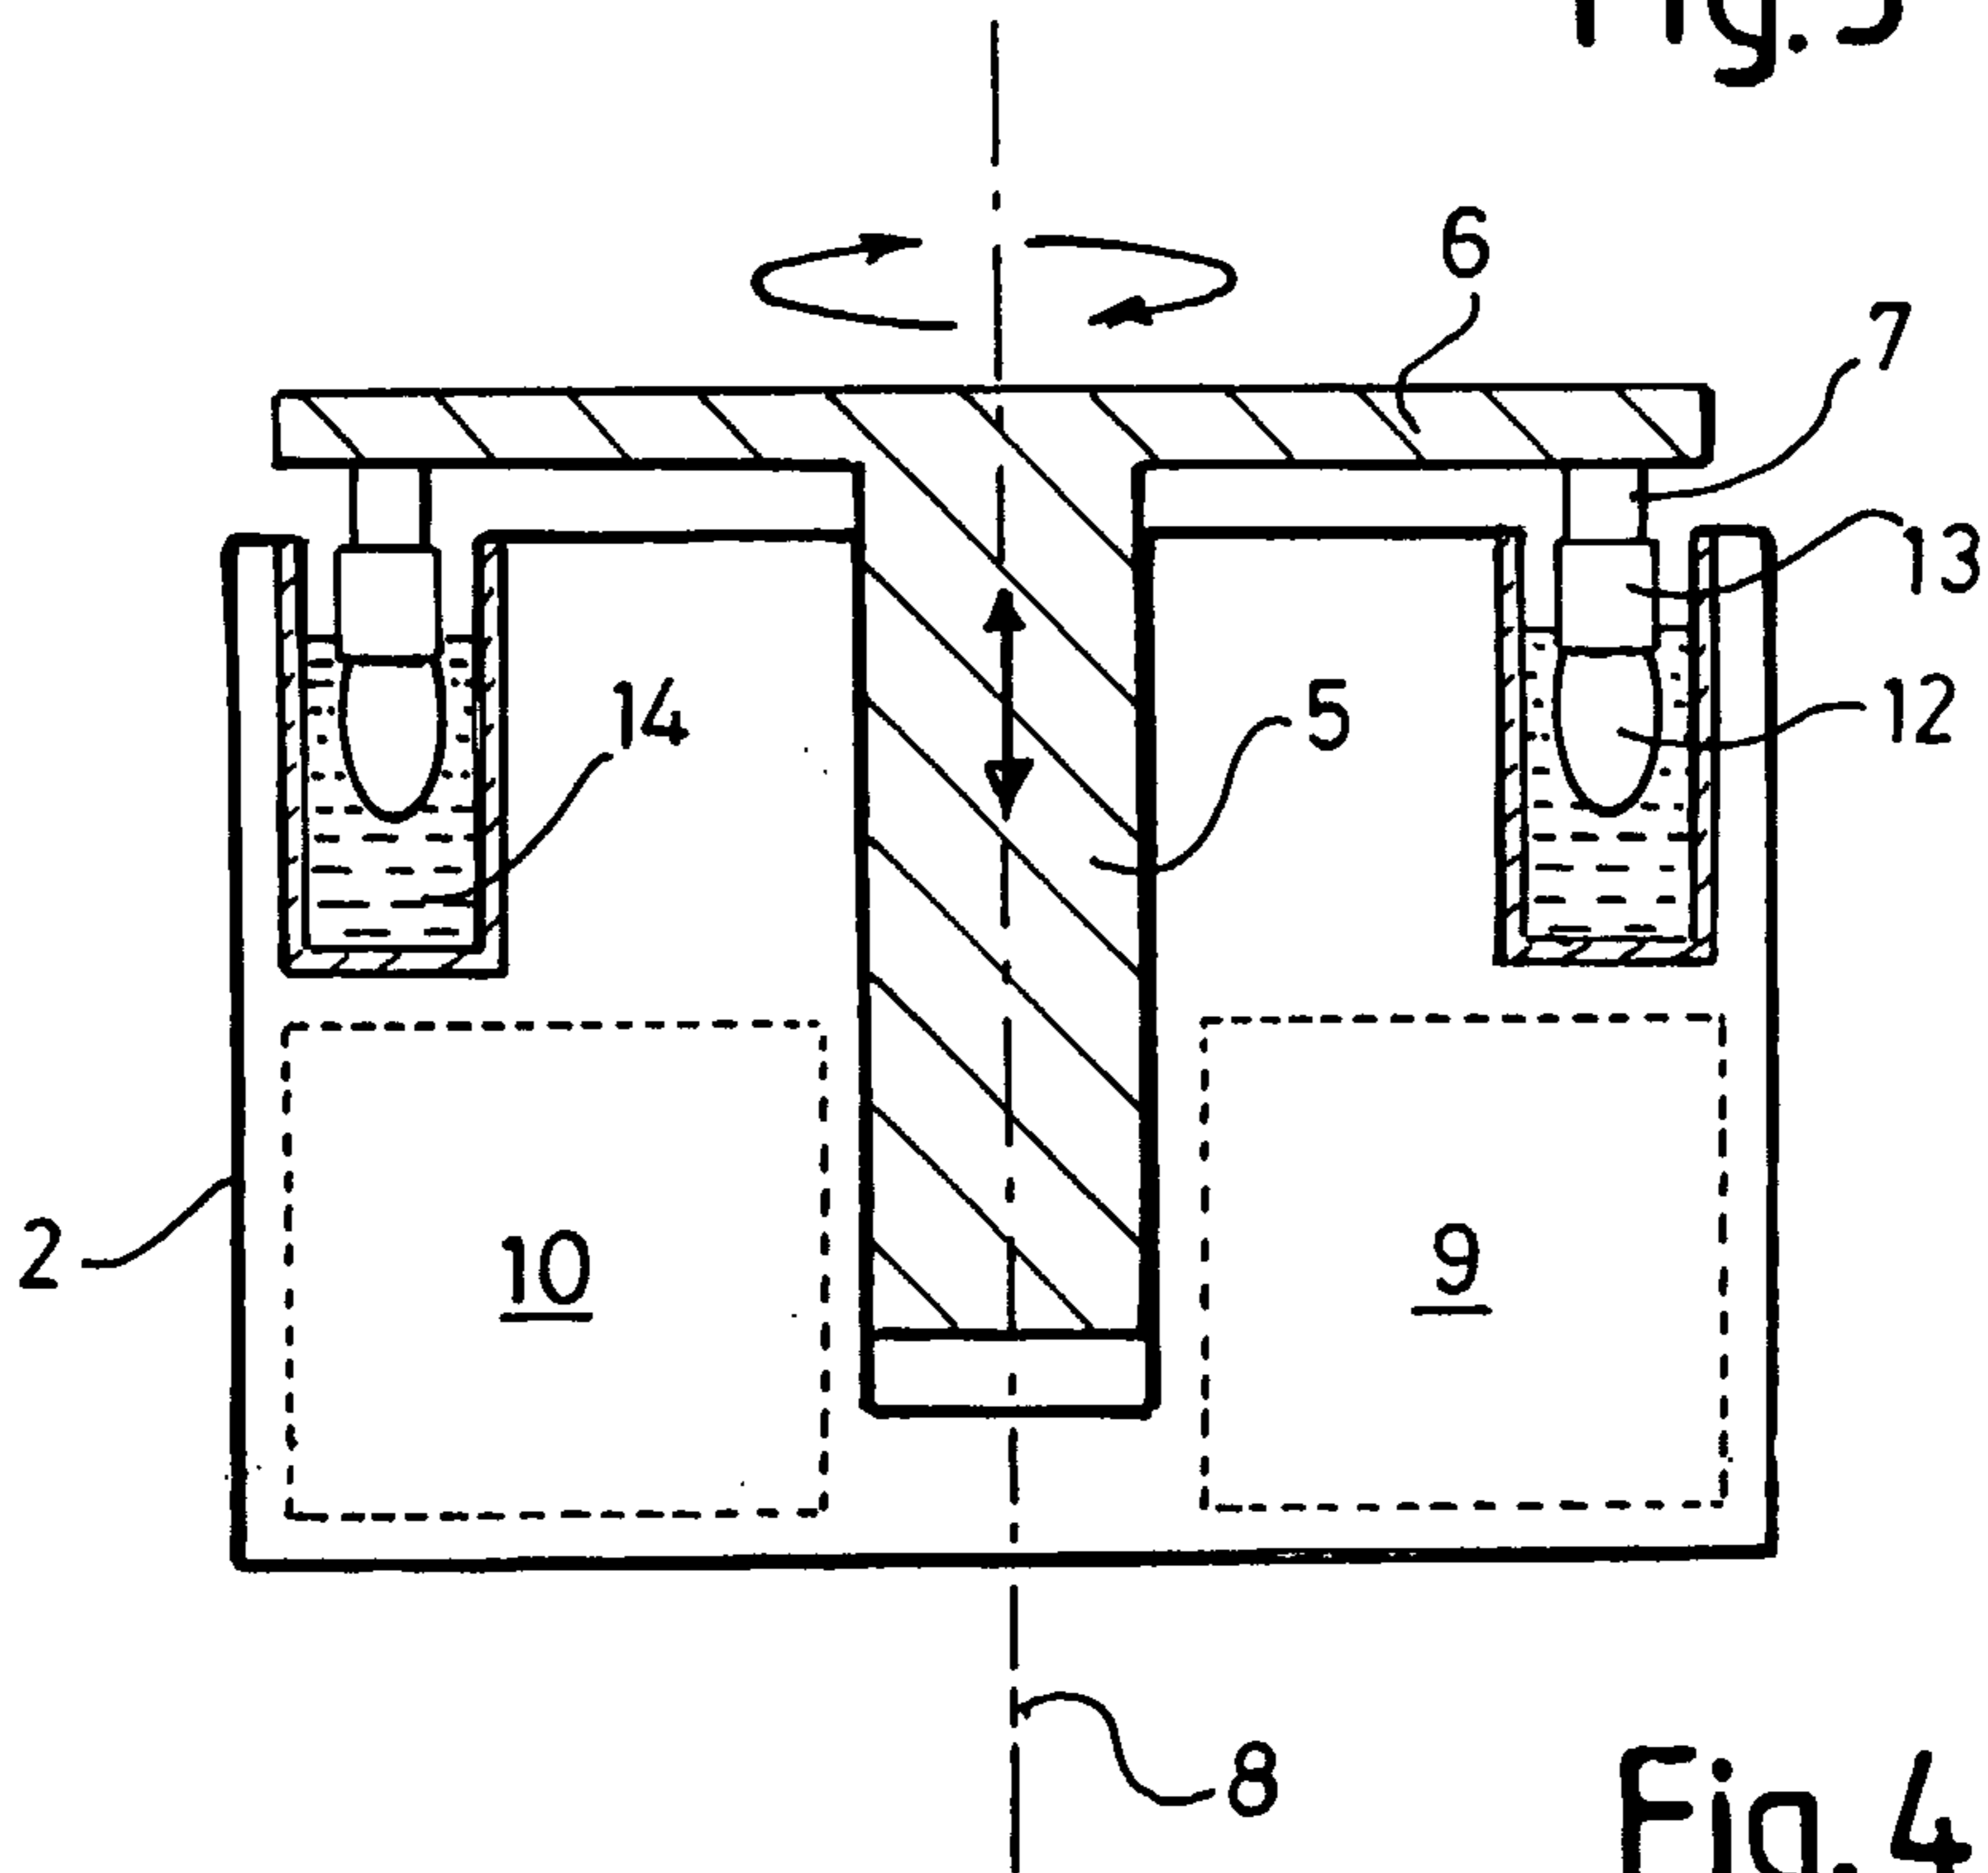


Fig. 4

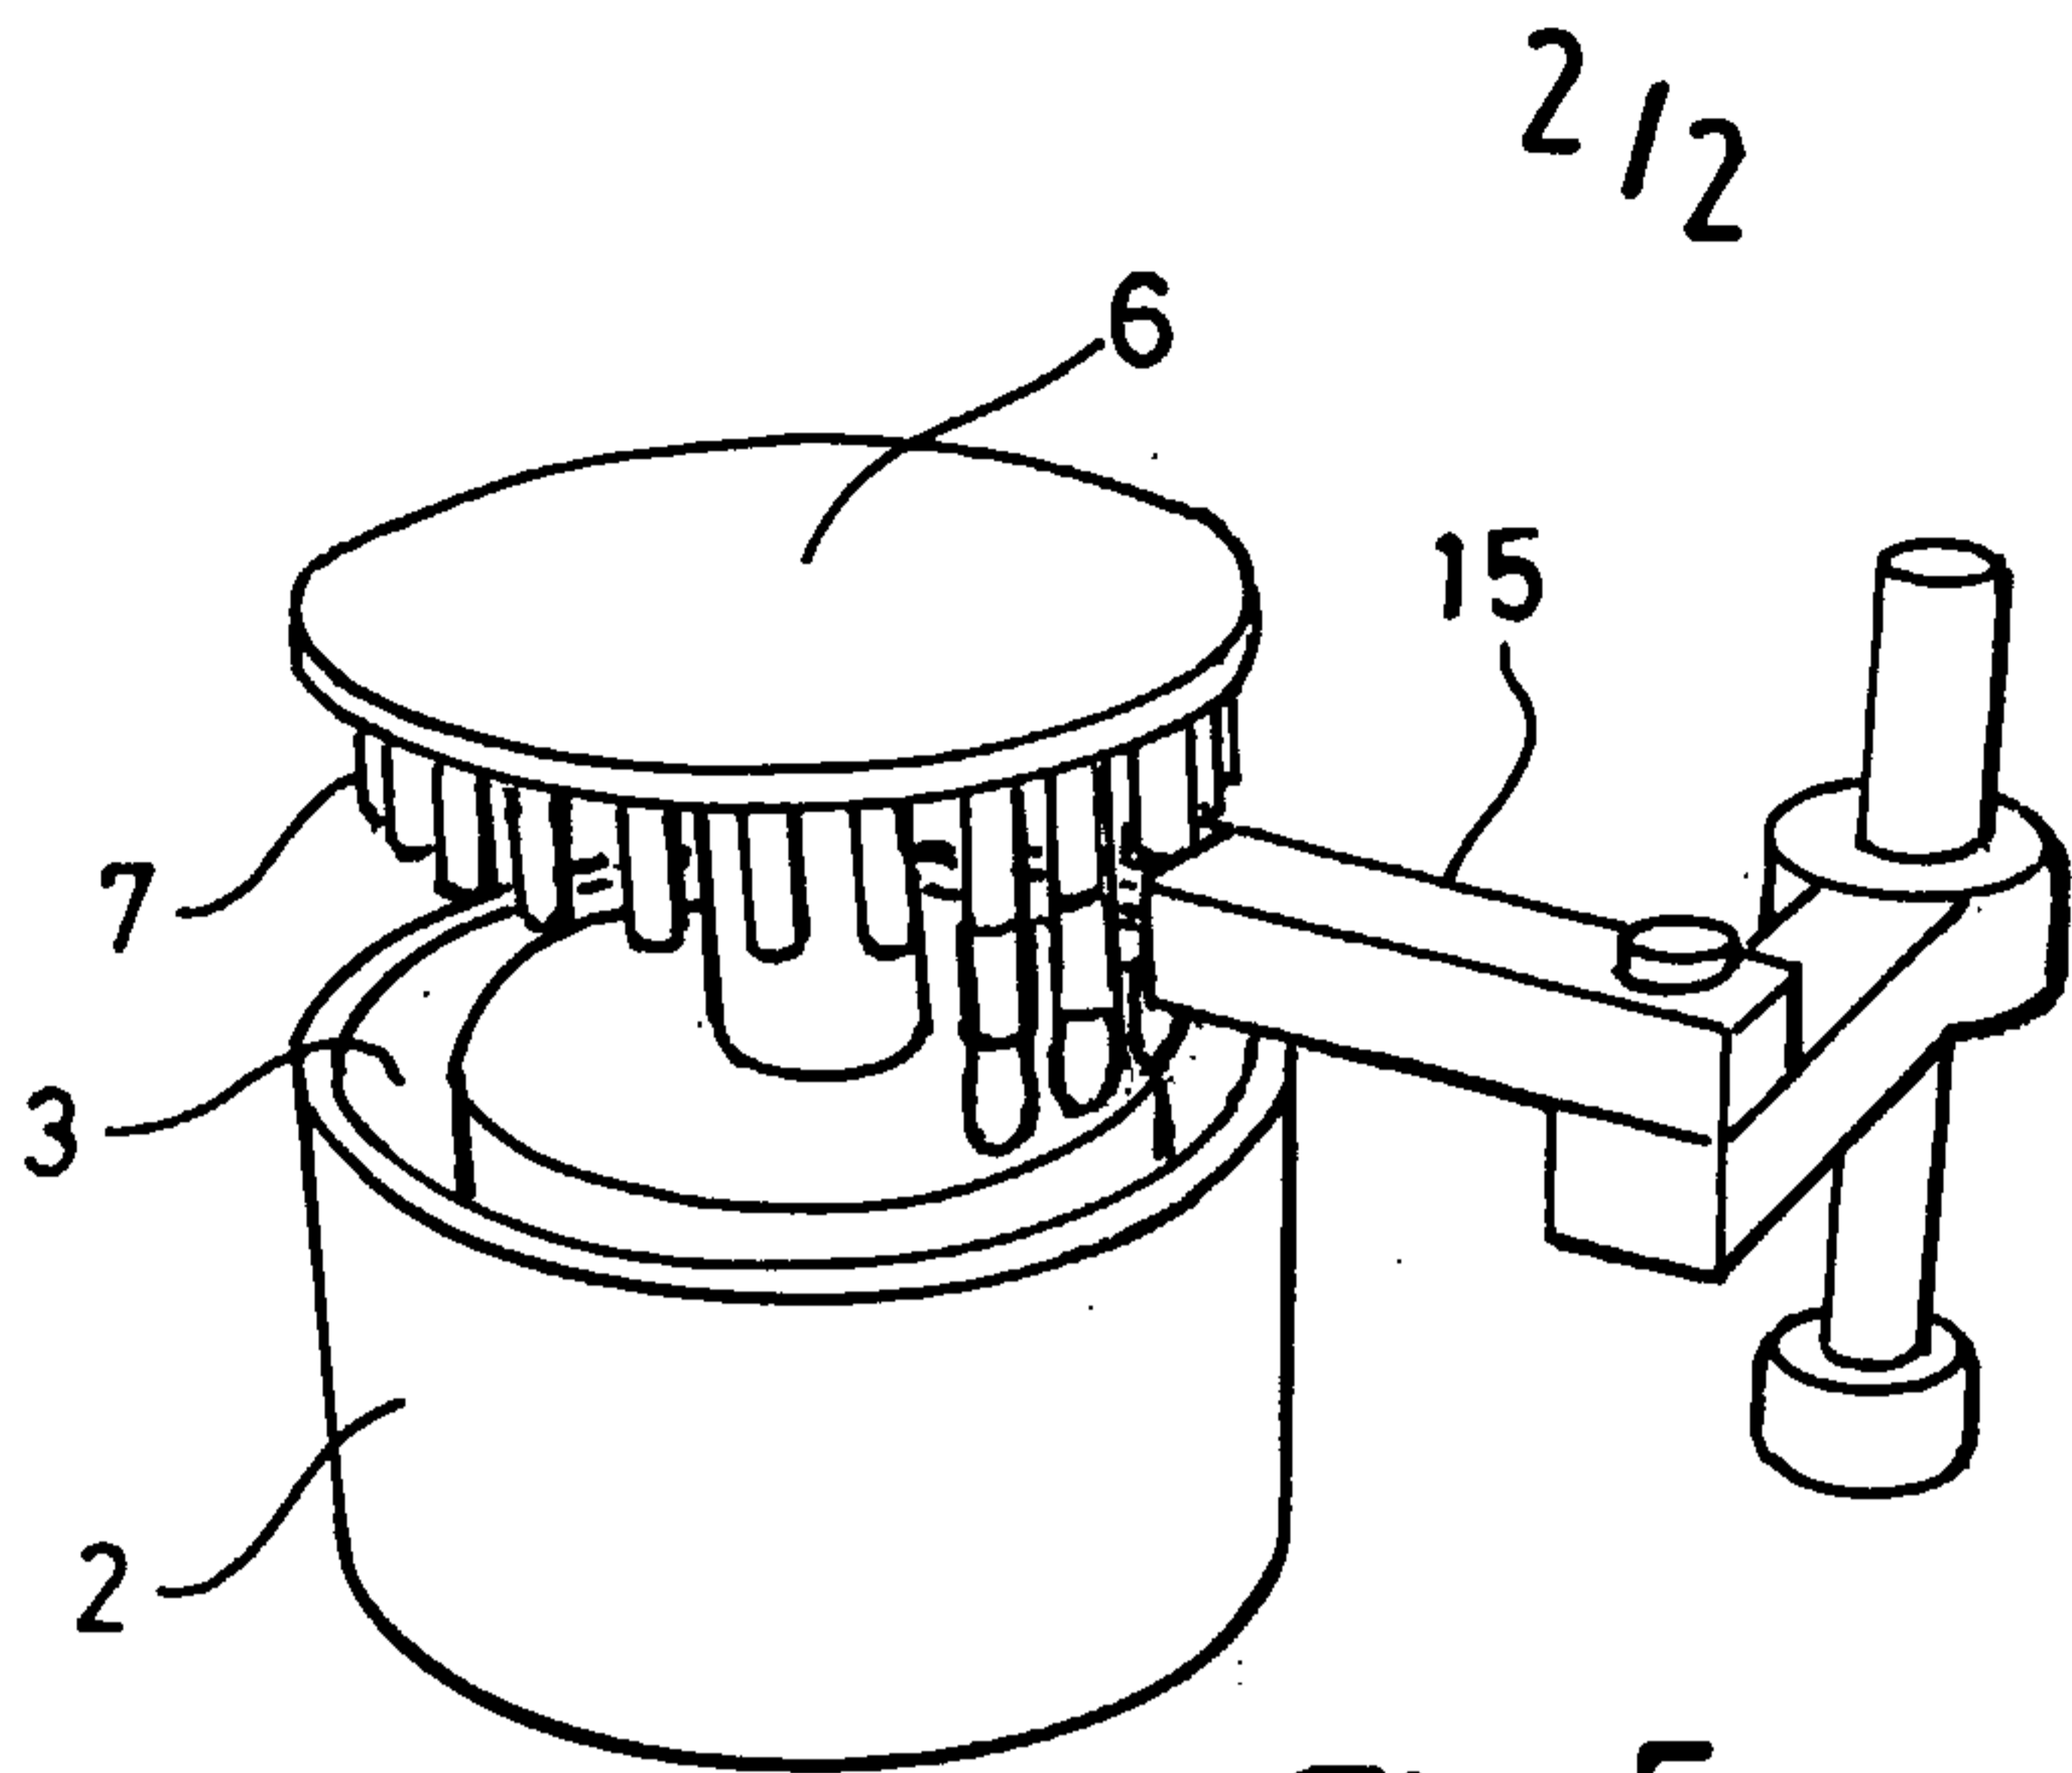


Fig. 5

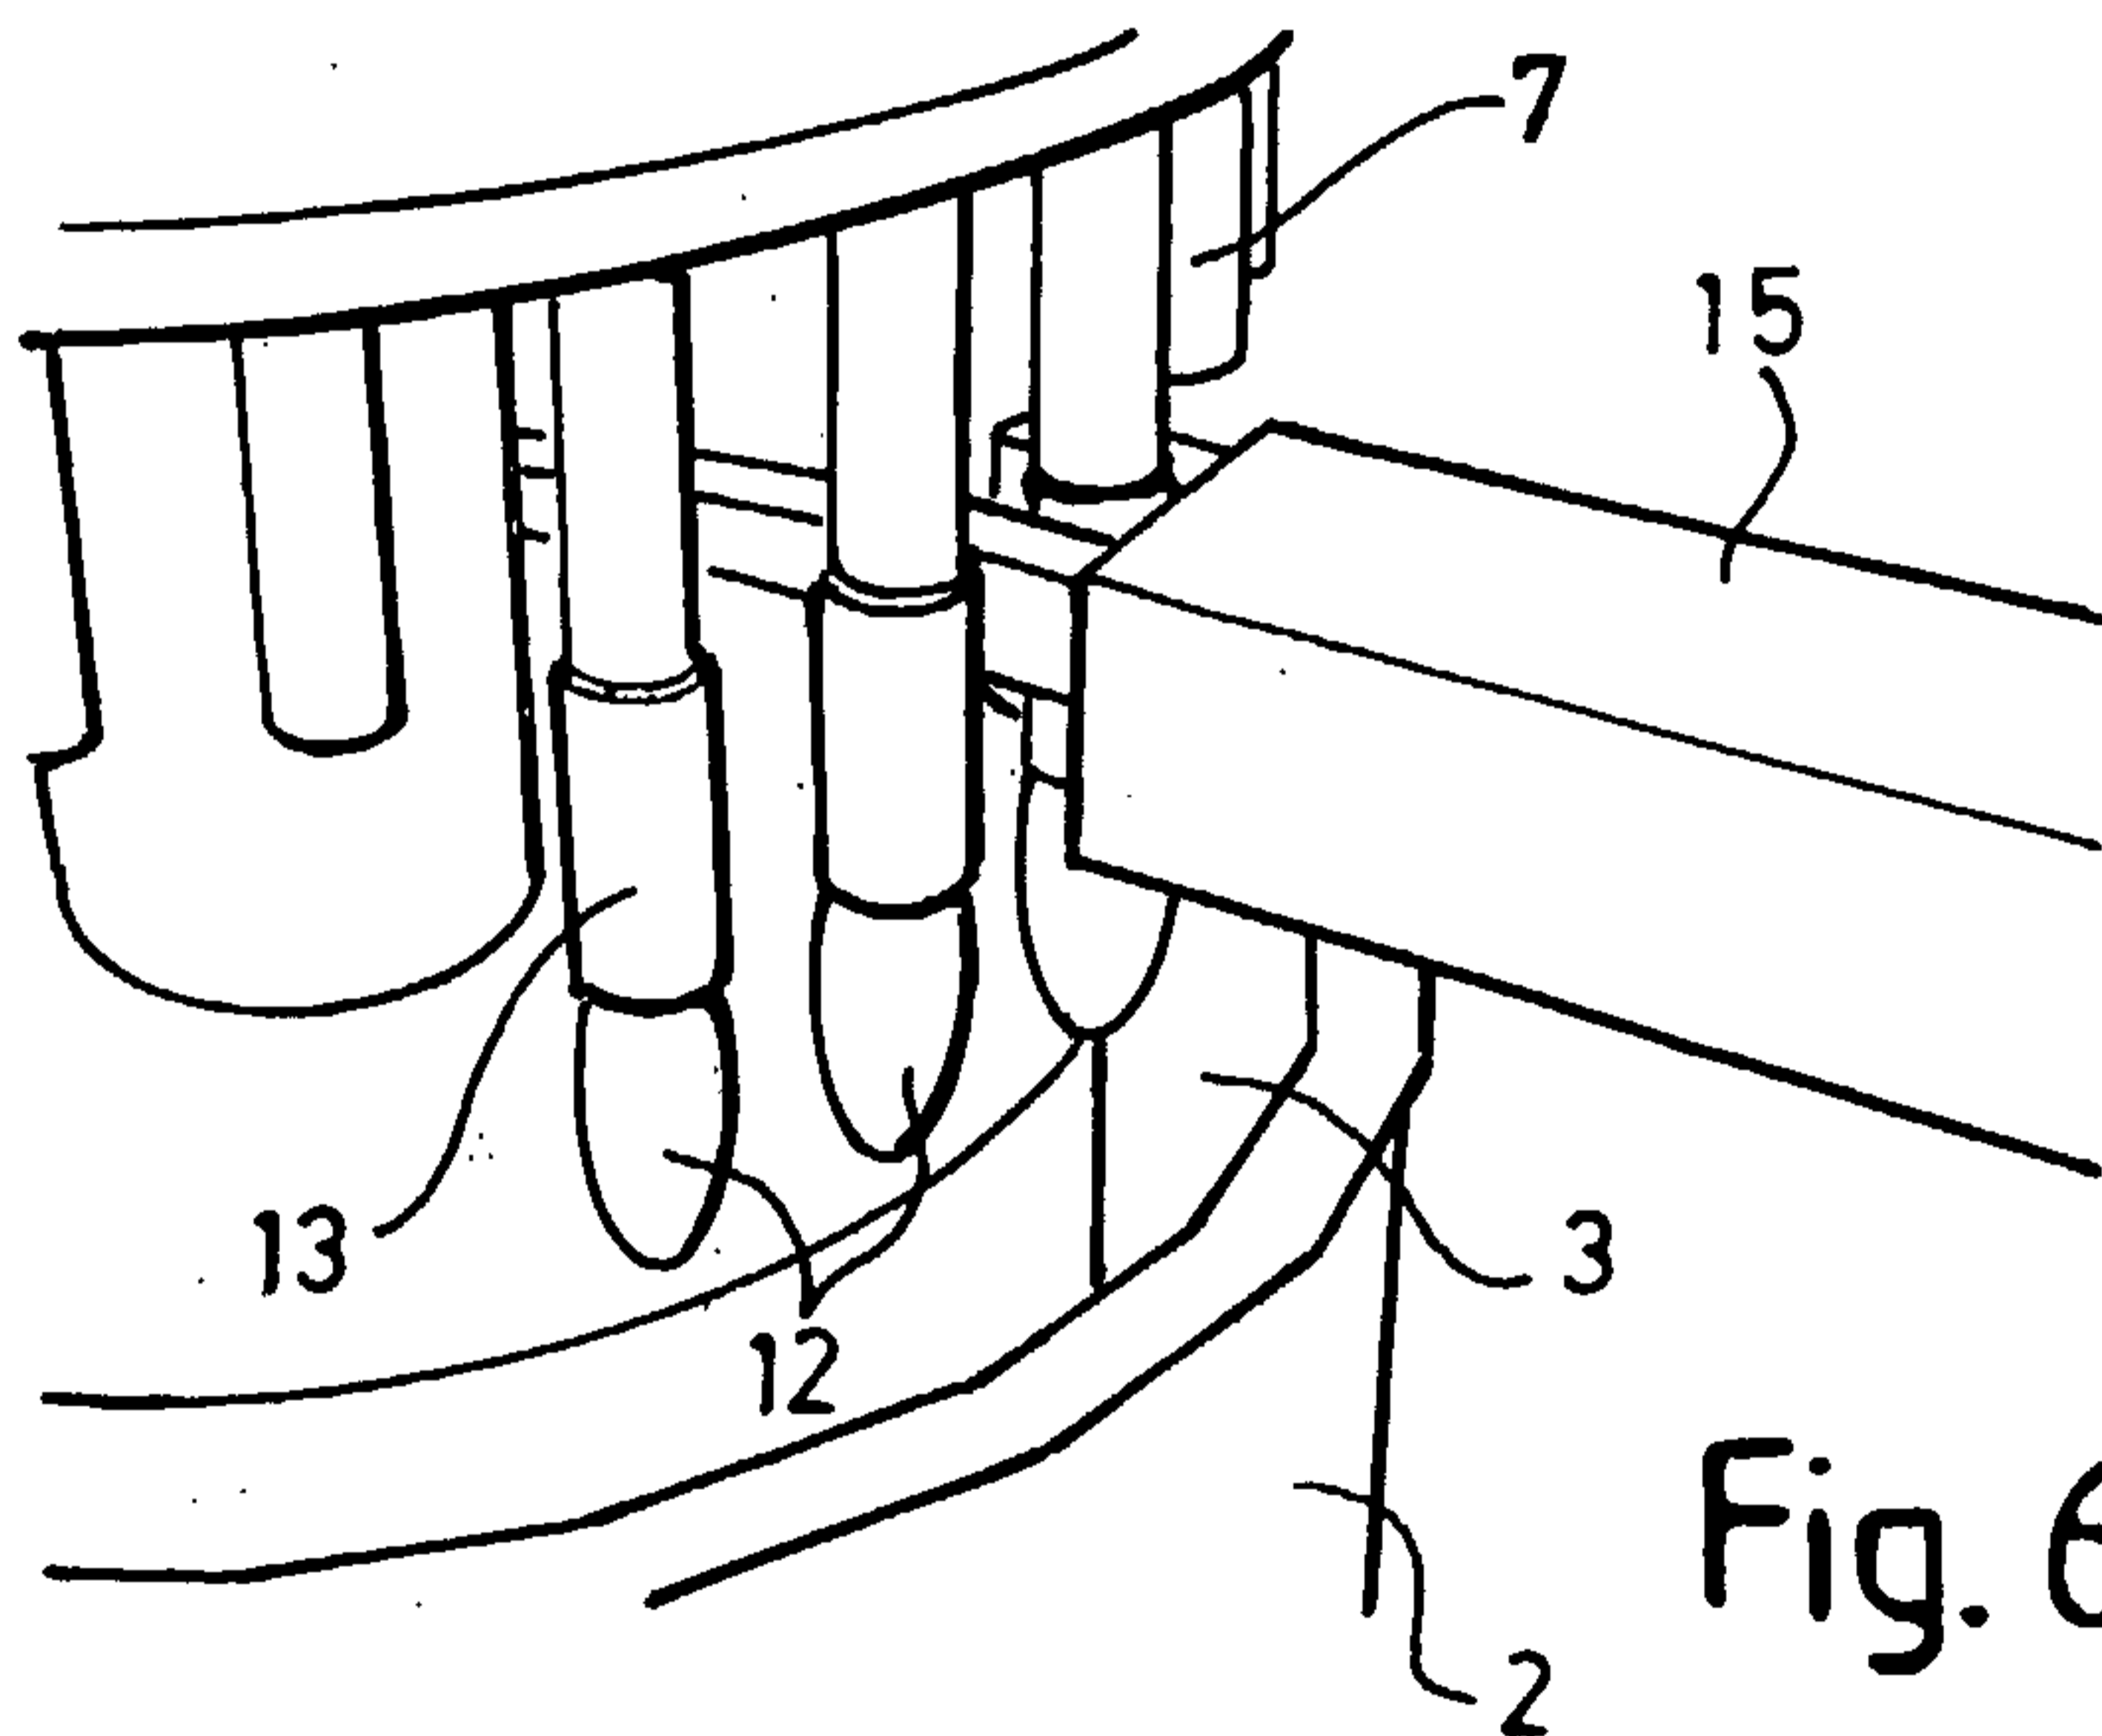


Fig. 6

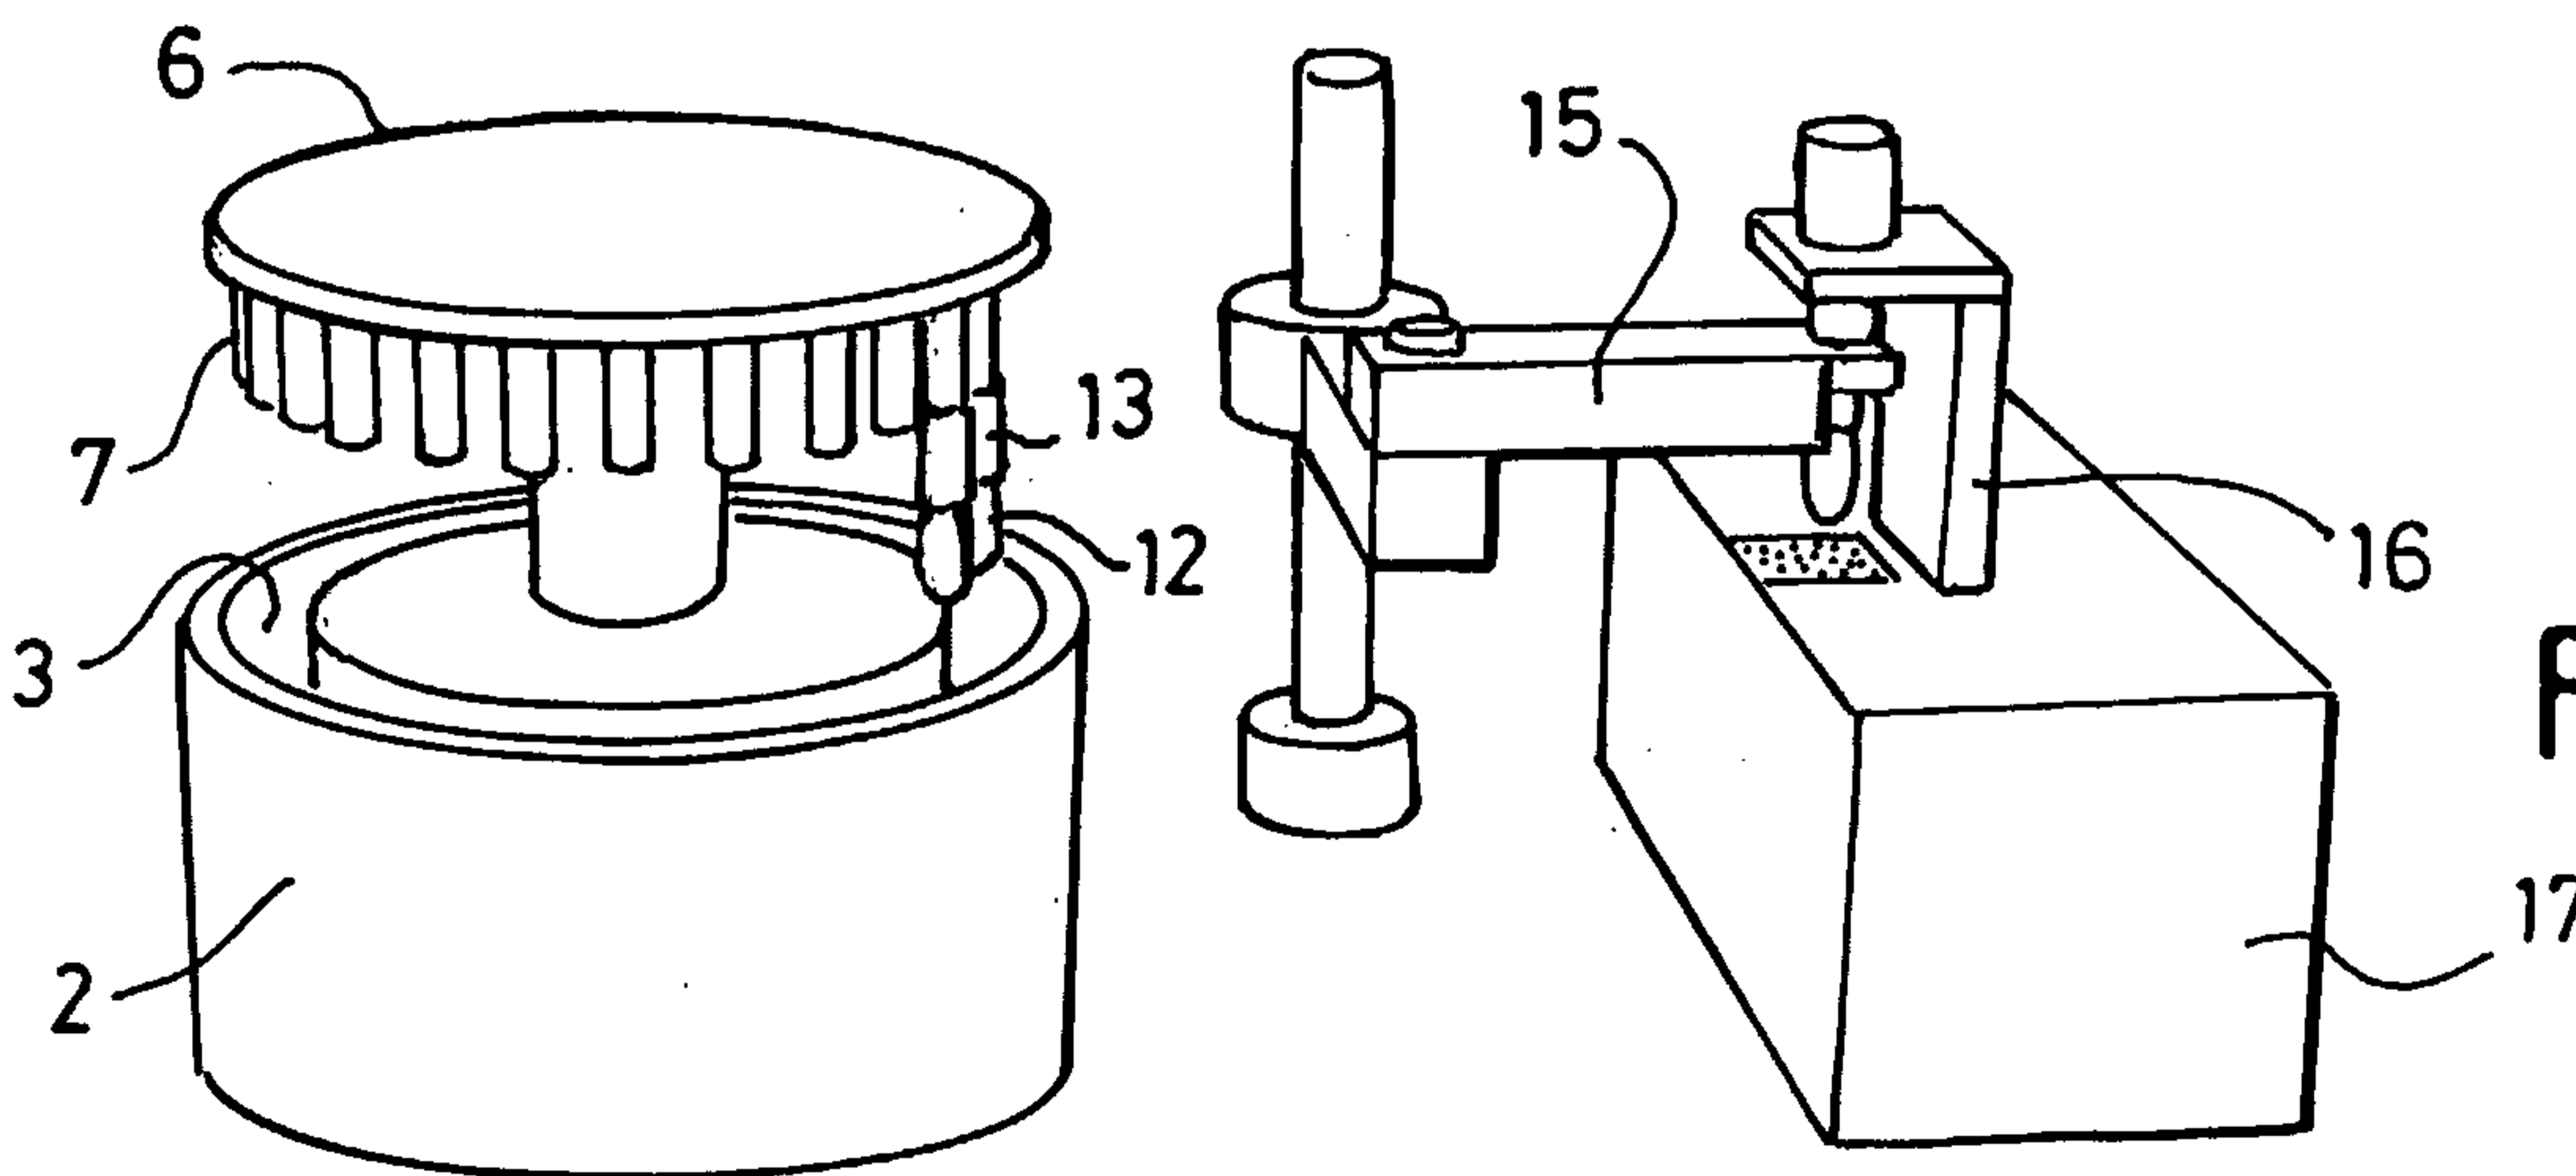


Fig. 7

