



(51) International Patent Classification:

A61B 18/12 (2006.01) A61B 6/00 (2006.01)  
A61B 18/14 (2006.01) A61B 5/055 (2006.01)  
A61B 17/3203 (2006.01)

(21) International Application Number:

PCT/US2013/053977

(22) International Filing Date:

7 August 2013 (07.08.2013)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

13/586,559 15 August 2012 (15.08.2012) US

(71) Applicant: THERMEDICAL, INC. [US/US]; 150 Bear Hill Road, Second Floor, Waltham, MA 02451 (US).

(72) Inventor: CURLEY, Michael, G.; 654 Boston Post Road, Weston, MA 02493 (US).

(74) Agents: ADAMS, Lisa et al.; Nutter McClennen & Fish Llp, Seaport West, 155 Seaport Boulevard, Boston, MA 02210-2604 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: LOW PROFILE FLUID ENHANCED ABLATION THERAPY DEVICES AND METHODS

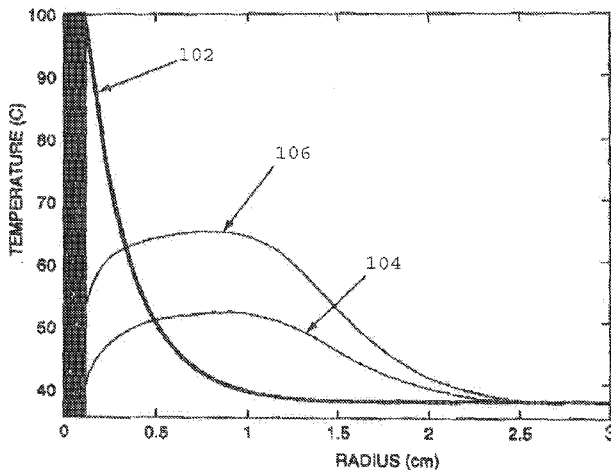


FIG. 1

(57) Abstract: Low profile devices and methods for delivering fluid enhanced ablation therapy are provided herein. In one embodiment, an ablation device is provided that includes an elongate body having proximal and distal ends, an inner lumen extending therethrough and at least one outlet port formed therein and configured to deliver fluid to surrounding tissue. The device can also include at least one ablation element disposed along a length of the body adjacent to the at least one outlet port and configured to deliver energy to surrounding tissue, as well as at least one heating element disposed within the inner lumen of the elongate body. The device further includes a handle having proximal and distal ends, the distal end of the handle being coupled to the proximal end of the elongate body. Further, a longitudinal axis of the elongate body extends at an angle to a longitudinal axis of the handle.

WO 2014/028287 A1

## LOW PROFILE FLUID ENHANCED ABLATION THERAPY DEVICES AND METHODS

### FIELD

[0001] This application relates generally to fluid enhanced ablation therapy, and more particularly, this application relates to improved low profile devices and methods for administering fluid enhanced ablation therapy.

### BACKGROUND

[0002] The use of thermal energy to destroy bodily tissue can be applied to a variety of therapeutic procedures, including the destruction of tumors. Thermal energy can be imparted to the tissue using various forms of energy, such as radio frequency electrical energy, microwave or light wave electromagnetic energy, or ultrasonic vibrational energy. Radio frequency (RF) ablation, for example, can be effected by placing one or more electrodes against or into tissue to be treated and passing high frequency electrical current into the tissue. The current can flow between closely spaced emitting electrodes or between an emitting electrode and a larger, common electrode located remotely from the tissue to be heated.

[0003] One disadvantage with these techniques is that maximum heating often occurs at or near the interface between the therapeutic tool and the tissue. In RF ablation, for example, maximum heating can occur in the tissue immediately adjacent to the emitting electrode. This can reduce the conductivity of the tissue, and in some cases, can cause water within the tissue to boil and become water vapor. As this process continues, the impedance of the tissue can increase and prevent current from entering into the surrounding tissue. Thus, conventional RF instruments are limited in the volume of tissue that can be treated.

[0004] Fluid enhanced ablation therapy, such as the SERF™ ablation technique (Saline Enhanced Radio Frequency™ ablation), can treat a greater volume of tissue than conventional RF ablation. The SERF ablation technique is described in U.S. Patent No. 6,328,735, which is hereby incorporated by reference in its entirety. Using the SERF ablation technique, saline is passed through a needle and heated, and the heated fluid is delivered to the tissue immediately surrounding the needle. The saline helps distribute the heat developed adjacent to the needle and thereby allows a greater volume of tissue to be treated with a

therapeutic dose of ablative energy. The therapy is usually completed once a target volume of tissue reaches a desired therapeutic temperature, or otherwise receives a therapeutic dose of energy.

[0005] Fluid enhanced ablation therapy can be administered to a patient in a variety of manners. For example, an RF electrode can be introduced into a patient's body percutaneously using a needle during a laparoscopic or other minimally invasive surgical procedure. In such a procedure, a surgeon, doctor, interventional radiologist, or other medical professional administering the therapy must utilize a medical imaging apparatus to guide the positioning of the RF electrode at a desired location. Such an imaging apparatus can also be utilized to monitor the effectiveness of the therapy as the procedure progresses.

[0006] Many medical imaging apparatuses, however, require a patient to be placed in a space-constrained volume within the apparatus in order to be effectively imaged. X-ray Computed Tomography (CT) scanners and Magnetic Resonance Imaging (MRI) scanners, for example, often require a patient to be moved through a small cylindrical opening in the device. Moving a patient through these devices while long needles and extended manipulating handles are protruding from their body can be difficult or impossible. Professionals administering the therapy can be forced to remove the devices from the patient and subsequently reintroduce them several times in order to successfully image and treat the targeted area of the patient's body.

[0007] Accordingly, there is a need for improved low profile fluid enhanced ablation therapy devices and methods that can be utilized by medical professionals in space-constrained environments, such as within medical imaging apparatuses.

## SUMMARY

[0008] The present invention generally provides low profile devices and methods for administering fluid enhanced ablation therapy. In particular, the devices and methods described herein permit surgeons, doctors, radiologists, or other medical professionals to administer fluid enhanced ablation therapy in space-constrained environments, such as inside medical imaging apparatuses. The low profile devices and methods of the present invention can thereby allow continuous or periodic medical imaging of the ablation therapy to determine positional accuracy and therapy effectiveness without having to remove and re-introduce any ablation devices being used.

[0009] In one aspect, an ablation device is provided that includes an elongate body having proximal and distal ends, an inner lumen extending longitudinally through the elongate body, and at least one outlet port formed in the elongate body and configured to deliver fluid to tissue surrounding the elongate body. The ablation device further includes at least one ablation element disposed along a length of the elongate body adjacent to the at least one outlet port and configured to deliver energy to tissue surrounding the elongate body. The ablation device also includes a handle having proximal and distal ends, the distal end of the handle being coupled to the proximal end of the elongate body. In addition, a longitudinal axis of the elongate body can extend at an angle to a longitudinal axis of the handle.

[0010] The devices and methods described herein can have a variety of modifications and additional features, all of which are considered within the scope of the invention. For example, in some embodiments, the angle between the longitudinal axis of the elongate body and the longitudinal axis of the handle can be about 90 degrees. In other embodiments, the angle can be acute, or less than 90 degrees, such that the handle extends at least partially back towards the distal end of the elongate body. In still other embodiments, the angle can be obtuse, or greater than 90 degrees, such that the handle extends proximally and farther away from the distal end of the elongate body. In certain embodiments, for example, the angle between the longitudinal axis of the elongate body and the longitudinal axis of the handle can be in a range of about 10 degrees to about 120 degrees. In other embodiments, the angle can be in a range of about 30 degrees to about 100 degrees, and in still other embodiments the angle can be in a range of about 45 degrees to about 90 degrees.

[0011] In certain embodiments, the handle can include an inner lumen extending therethrough that can be used to transport fluid and/or electrical power to the distal end of the elongate body. As a result, in some embodiments, the inner lumen of the handle can be in communication with the inner lumen of the elongate body.

[0012] The handle itself can have a variety of shapes and sizes. For example, in some embodiments the handle can be straight along its longitudinal length. In other embodiments, however, the handle can be contoured along its longitudinal length to better fit within a user's hand. Such contouring can also be present in other directions as well (*e.g.*, along a circumference or width of the handle) to enable a user to more comfortably and accurately manipulate the ablation device. The size of the handle can also be varied according to preference to fit a user's hand by, for example, making the handle longer, thicker, and

heavier, or smaller, thinner, and lighter, etc. In other embodiments, the handle can include a surface texture or other surface features to improve a user's grip of the device. This can be especially useful if the user is wearing surgical gloves or has come into contact with one or more bodily or cleansing fluids.

[0013] As a result of the fact that the handle is coupled to an elongate body that can be inserted percutaneously into a patient's body, the ablation device can also include an insertion stopping element slidably disposed on the elongate body to prevent over-insertion of the device.

[0014] In some embodiments, the entire ablation device can be formed from materials that are non-magnetic (*i.e.*, negligibly affected by or affecting magnetic fields). Forming the device from non-magnetic materials can allow the device to remain in a patient when imaged using, for example, Magnetic Resonance Imaging (MRI) scanners that create strong magnetic fields as part of the imaging process.

[0015] In certain embodiments, the ablation device can further include at least one heating element disposed within the inner lumen of the elongate body and configured to heat fluid passing therethrough. The introduction of therapeutically heated fluid into tissue surrounding the distal end of the elongate body can have several advantages, as is described in more detail below. The at least one heating element can have a variety of forms but, in one embodiment, a heating element can include at least one wire and at least one spacer where the at least one wire is configured to pass energy through the fluid flowing through the inner lumen of the elongate body. By passing energy through the fluid within the inner lumen of the elongate body, the fluid's temperature can be increased due to its natural resistance. The at least one spacer can be used to maintain the position of the at least one wire within the inner lumen of the elongate body.

[0016] In another aspect, a method for administering fluid enhanced ablation therapy is provided that includes percutaneously inserting a distal end of an elongate body of an ablation device into a patient. The method further includes manipulating the distal end of the elongate body within the patient using a low profile handle coupled to the proximal end of the elongate body and having a longitudinal axis that extends at an angle to a longitudinal axis of the elongate body. The method further includes delivering fluid through the elongate body of

the ablation device into tissue surrounding the distal end of the elongate body while simultaneously delivering energy into tissue surrounding the distal end of the elongate body.

[0017] In some embodiments, the method can further include imaging at least a portion of the patient using a medical imaging apparatus. Furthermore, in some embodiments, imaging can occur simultaneously with any of the manipulating step and the delivering step.

Accordingly, in some embodiments, the patient can be positioned within the medical imaging apparatus during at least a portion of the method. Indeed, in some embodiments, both the manipulating step and the delivering step can be performed inside the medical imaging apparatus.

[0018] Any of a number of medical imaging apparatuses can be utilized in the methods disclosed herein. For example, in some embodiments the imaging apparatus can be selected from the group consisting of an X-ray Computed Tomography (CT) scanner, a Magnetic Resonance Imaging (MRI) scanner, an ultrasound scanner, and an X-ray scanner. However, other imaging devices known in the prior art can also be utilized with the methods of the present invention.

[0019] In certain embodiments, the method can further include heating the fluid inside the elongate body prior to delivering the fluid into the tissue surrounding the elongate body. As mentioned above and discussed in more detail below, heating the fluid prior to delivery into tissue can be beneficial and enhance the effectiveness of the fluid enhanced ablation therapy.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0020] The aspects and embodiments of the invention described above will be more fully understood from the following detailed description taken in conjunction with the accompanying drawings, in which:

[0021] FIG. 1 is a graphical representation of simulated heating profiles for various forms of ablation;

[0022] FIG. 2 is a diagram of one embodiment of a fluid enhanced ablation system;

[0023] FIG. 3 is a perspective view of a medical device having an elongate body for use in fluid enhanced ablation therapy;

[0024] FIG. 4 is an illustration of one embodiment of a medical imaging apparatus;

[0025] FIG. 5 is a side view of one embodiment of a low profile fluid enhanced ablation device;

[0026] FIG. 6 is an alternate view of the low profile fluid enhanced ablation device of FIG. 5;

[0027] FIG. 7 is a front view of the medical imaging apparatus of FIG. 4 including the low profile fluid enhanced ablation device of FIG. 5;

[0028] FIG. 8 is a diagram of one embodiment of a heating element in an elongate body of a fluid enhanced ablation device; and

[0029] FIG. 9 is a diagram of one embodiment of an electrical circuit for driving a fluid enhanced ablation device.

#### DETAILED DESCRIPTION

[0030] Certain exemplary embodiments will now be described to provide an overall understanding of the principles of the devices and methods disclosed herein. One or more examples of these embodiments are illustrated in the accompanying drawings. Those skilled in the art will understand that the devices and methods specifically described herein and illustrated in the accompanying drawings are non-limiting exemplary embodiments and that the scope of the present invention is defined solely by the claims. The features illustrated or described in connection with one exemplary embodiment may be combined with the features of other embodiments. Such modifications and variations are intended to be included within the scope of the present invention.

[0031] The terms “a” and “an” can be used interchangeably, and are equivalent to the phrase “one or more” as utilized in the present application. The terms “comprising,” “having,” “including,” and “containing” are to be construed as open-ended terms (*i.e.*, meaning “including, but not limited to,”) unless otherwise noted. The terms “about” and “approximately” used for any numerical values or ranges indicate a suitable dimensional tolerance that allows the composition, part, or collection of elements to function for its intended purpose as described herein. These terms generally indicate a  $\pm 10\%$  variation about a central value. Components described herein as being coupled may be directly coupled, or

they may be indirectly coupled via one or more intermediate components. The recitation of any ranges of values herein is merely intended to serve as a shorthand method of referring individually to each separate value falling within the range, unless otherwise indicated herein, and each separate value is incorporated into the specification as if it were individually recited. All methods described herein can be performed in any suitable order unless otherwise indicated herein or otherwise clearly contradicted by context. The use of any and all examples, or exemplary language (*e.g.*, “such as”), provided herein is intended merely to better illuminate the invention and does not impose a limitation on the scope of the invention unless otherwise claimed. No language in the specification should be construed as indicating any non-claimed element as essential to the practice of the invention. Further, to the extent the term “saline” is used in conjunction with any embodiment herein, such embodiment is not limited to the use of “saline” as opposed to another fluid unless explicitly indicated. Other fluids can typically be used in a similar manner.

[0032] The present invention is generally directed to low profile fluid enhanced ablation devices and methods. These low profile devices and methods allow for the administration of fluid enhanced ablation therapy in space-constrained environments, such as within a medical imaging apparatus (*e.g.*, a Magnetic Resonance Imaging, or MRI, scanner, etc.). The low profile devices and methods disclosed herein generally accommodate more tightly constrained environments by including handles for manipulating the devices that extend at an angle to the needles or other elongate bodies that are inserted into a patient’s body to administer the therapy. By extending a handle in a direction that is offset from a longitudinal axis of the elongate body inserted into a patient, the required clearance space surrounding the patient’s body can be reduced.

[0033] Fluid enhanced ablation therapy, as mentioned above, is defined by passing a fluid into tissue while delivering therapeutic energy from an ablation element. The delivery of therapeutic energy into tissue causes hyperthermia in the tissue, ultimately resulting in necrosis. This temperature-induced selective destruction of tissue can be utilized to treat a variety of conditions including tumors, fibroids, cardiac dysrhythmias (*e.g.*, ventricular tachycardia, etc.), and others.

[0034] The SERF<sup>TM</sup> ablation technique (Saline Enhanced Radio Frequency<sup>TM</sup> ablation) described in U.S. Patent No. 6,328,735 and incorporated by reference above, delivers fluid heated to a therapeutic temperature into tissue along with ablative energy. Delivering heated

fluid enhances the ablation treatment because the fluid flow through the extracellular space of the treatment tissue can increase the heat transfer through the tissue significantly. The flowing heated fluid therefore convects thermal energy from the ablation energy source further into the target tissue. In addition, the fact that the fluid is heated to a therapeutic temperature increases the amount of energy that can be imparted into the tissue. Finally, the fluid can also serve to constantly hydrate the tissue and prevent any charring and associated impedance rise, as described in more detail below.

[0035] By way of illustration, ablation is often quantified in terms of an administered thermal dose level, which can be expressed as a particular time during which tissue was raised to a temperature above 41° Celsius (C) (a generally accepted threshold temperature for causing irreversible damage to tissue). A number of different methods exist for determining a therapeutic thermal dose, but Nath, S. and Haines, D. E., *Prog. Card. Dis.* 37(4):185-205 (1995) (Nath *et al.*) suggest a temperature of 50° C for one minute as therapeutic. Using this as a reference, FIG. 1 shows the performance profiles of several ablation techniques by plotting a simulated temperature profile achieved as a function of distance from an ablation element, such as an emitter electrode. The first profile 102 illustrates the performance of RF ablation without the use of fluid enhancement. As shown in the figure, the temperature of the tissue falls very sharply with distance from the electrode. This means that within 10 mm of the ablation element the temperature of the tissue is still approximately body temperature (37° C), far below the therapeutic temperature of 50° C mentioned above. Furthermore, very close to the ablation element the temperature is very high, meaning that the tissue will more quickly desiccate, or dry up, and char. Once this happens, the impedance of the tissue rises dramatically, making it difficult to pass energy to tissue farther away from the ablation element.

[0036] A second tissue temperature profile 104 is associated with a second prior art system similar to that described in U.S. Pat. No. 5,431,649. In this second system, an electrode is inserted into tissue and imparts a 400 kHz RF current flow of about 525 mA to heat the tissue. Body temperature (37° C) saline solution is simultaneously injected into the tissue at a rate of 10 ml/min. The resulting tissue temperature profile 104 is more uniform than profile 102, but the maximum temperature achieved anywhere is approximately 50° C. Thus, the temperature profile 104 exceeds the 50° C temperature threshold specified for one minute of

therapy in only a small portion of the tissue. Such a small temperature increment requires significant treatment time to achieve any therapeutically meaningful results.

[0037] A third tissue temperature profile 106 is achieved using fluid enhanced ablation therapy. In the illustrated embodiment, an electrode formed from silver/silver chloride is inserted into tissue and imparts a 480 kHz RF current flow of 525 mA to heat the tissue. Saline solution heated to 50° C is simultaneously injected into the tissue at a rate of 10 ml/min. The resulting temperature profile 106 is both uniform and significantly above the 50° C therapeutic threshold out to 15 mm from the electrode. Moreover, because the temperature is uniform within the volume, the thermal dose delivered is also uniform through the volume.

[0038] The uniform temperature profile seen in FIG. 1 can be achieved by the introduction of heated fluid into the target tissue during application of ablative energy. The fluid convects the heat deeper into the tissue, thereby reducing the charring and impedance change in tissue that occurs near the ablation element, as shown in profile 102. Further, because the fluid is heated to a therapeutic level, it does not act as a heat sink that draws down the temperature of the surrounding tissue, as seen in profile 104. Therefore, the concurrent application of RF energy and perfusion of heated saline solution into the tissue eliminates the desiccation and/or vaporization of tissue adjacent to the electrode, maintains the effective tissue impedance, and increases the thermal transport within the tissue being heated with RF energy. The total volume of tissue that can be heated to therapeutic temperatures is thereby increased. For example, experimental testing has demonstrated that a volume of tissue having a diameter of approximately 8 cm (*i.e.*, a spherical volume of approximately 156 cm<sup>3</sup>) can be treated in 5 minutes using the fluid enhanced ablation techniques described herein. By comparison, conventional RF can only treat volumes having a diameter of approximately 3 cm (*i.e.*, a spherical volume of approximately 14 cm<sup>3</sup>) in the same 5-minute timespan.

[0039] In addition, fluid enhanced ablation devices have a greater number of parameters that can be varied to adjust the shape of the treatment profile according to the tissue being treated. For example, when using the SERF ablation technique, an operator or control system can modify parameters such as saline temperature (*e.g.*, from about 40° C to about 80° C), saline flow rate (*e.g.*, from about 0 ml/min to about 20 ml/min), RF power (*e.g.*, from about 0 W to about 100 W), and duration of treatment (*e.g.*, from about 0 min to about 10 min) to adjust the temperature profile 106. Different electrode configurations can also be used to vary the

treatment. For example, an emitter electrode can be configured as a continuous cylindrical band around a needle or other elongate body, or the electrode can be formed in other geometries, such as spherical or helical. The electrode can form a continuous surface area, or it can have a plurality of discrete portions. Still further, the electrode can be adapted for a mono-polar current flow, or multiple electrodes can be configured for bipolar operation, in which one electrode (or a portion of an electrode) acts as a cathode and another electrode (or portion thereof) acts as an anode.

[0040] FIG. 2 illustrates a diagram of one embodiment of a fluid enhanced ablation system 100. The system includes an elongate body 202 configured for insertion into a target volume of tissue. The elongate body can have a variety of shapes and sizes according to the geometry of the target tissue. Further, the particular size of the elongate body can depend on a variety of factors including the type and location of tissue to be treated, the size of the tissue volume to be treated, etc. By way of example only, in one embodiment, the elongate body can be a thin-walled stainless steel needle between about 16- and about 18-gauge (*i.e.*, an outer diameter of about 1.27 mm to about 1.65 mm), and having a length L (*e.g.*, as shown in FIG. 3) that is approximately 25 cm. The elongate body 202 can include a pointed distal tip 204 configured to puncture tissue to facilitate introduction of the device into a target volume of tissue, however, in other embodiments the tip can be blunt and can have various other configurations. The elongate body 202 can be formed from a conductive material such that the elongate body can conduct electrical energy along its length to one or more ablation elements located along a distal portion of the elongate body. Emitter electrode 205 is an example of an ablation element capable of delivering RF energy from the elongate body.

[0041] In some embodiments, the emitter electrode 205 can be a portion of the elongate body 202. For example, the elongate body 202 can be coated in an insulating material along its entire length except for the portion representing the emitter electrode 205. More particularly, in one embodiment, the elongate body 202 can be coated with 1.5 mil of the fluoropolymer Xylan™ 8840. The electrode 205 can have a variety of lengths and shape configurations. In one embodiment, the electrode 205 can be a 4 mm section of a tubular elongate body that is exposed to surrounding tissue. Further, the electrode 205 can be located anywhere along the length of the elongate body 205 (and there can also be more than one electrode disposed along the length of the elongate body). In one embodiment, the electrode can be located adjacent to the distal tip 204. In other embodiments, the elongate body can be formed from

an insulating material, and the electrode can be disposed around the elongate body or between portions of the elongate body.

[0042] In other embodiments, the electrode can be formed from a variety of other materials suitable for conducting current. Any metal or metal salt may be used. Aside from stainless steel, exemplary metals include platinum, gold, or silver, and exemplary metal salts include silver/silver chloride. In one embodiment, the electrode can be formed from silver/silver chloride. It is known that metal electrodes assume a voltage potential different from that of surrounding tissue and/or liquid. Passing a current through this voltage difference can result in energy dissipation at the electrode/tissue interface, which can exacerbate excessive heating of the tissue near the electrodes. One advantage of using a metal salt such as silver/silver chloride is that it has a high exchange current density. As a result, a large amount of current can be passed through such an electrode into tissue with only a small voltage drop, thereby minimizing energy dissipation at this interface. Thus, an electrode formed from a metal salt such as silver/silver chloride can reduce excessive energy generation at the tissue interface and thereby produce a more desirable therapeutic temperature profile, even where there is no liquid flow about the electrode.

[0043] The electrode 205 or other ablation element can include one or more outlet ports 208 that are configured to deliver fluid from an inner lumen 206 extending through the elongate body 202 into surrounding tissue (as shown by arrows 209). Alternatively, the electrode 205 can be positioned near one or more outlet ports 208 formed in the elongate body 202. In many embodiments, it can be desirable to position the electrode adjacent to the one or more outlet ports to maximize the effect of the flowing fluid on the therapy. The outlet ports 208 can be formed in a variety of sizes, numbers, and pattern configurations. In addition, the outlet ports 208 can be configured to direct fluid in a variety of directions with respect to the elongate body 202. These can include the normal orientation (*i.e.*, perpendicular to the elongate body surface) shown by arrows 209 in FIG. 2, as well as orientations directed proximally and distally along a longitudinal axis of the elongate body 202, including various orientations that develop a circular or spiral flow of liquid around the elongate body. Still further, in some embodiments, the elongate body 202 can be formed with an open distal end that serves as an outlet port. By way of example, in one embodiment, twenty-four equally-spaced outlet ports 208 having a diameter of about 0.4 mm can be created around the circumference of the electrode 205 using Electrical Discharge Machining (EDM). One

skilled in the art will appreciate that additional manufacturing methods are available to create the outlet ports 208. In addition, in some embodiments, the outlet ports can be disposed along a portion of the elongate body adjacent to the electrode, rather than being disposed in the electrode itself.

[0044] The inner lumen 206 that communicates with the outlet ports 208 can also house a heating assembly 210 configured to heat fluid as it passes through the inner lumen 206 just prior to being introduced into tissue. Furthermore, the portion of the elongate body located distal to the electrode 205 or other ablation element can be solid or filled such that the inner lumen 206 terminates at the distal end of the electrode 205. In one embodiment, the inner volume of the portion of the elongate body distal to the electrode can be filled with a plastic plug that can be epoxied in place or held by an interference fit. In other embodiments, the portion of the elongate body distal to the electrode can be formed from solid metal and attached to the proximal portion of the elongate body by welding, swaging, or any other technique known in the art.

[0045] Fluid can be supplied to the inner lumen 206 and heating assembly 210 from a fluid reservoir 212. The fluid reservoir 212 can be connected to the inner lumen 206 via a fluid conduit 214. The fluid conduit 214 can be, for example, a length of flexible plastic tubing. The fluid conduit 214 can also be a rigid tube, or a combination of rigid and flexible tubing. A preferred fluid for use in the SERF ablation technique is sterile normal saline solution (defined as a salt-containing solution). However, other liquids may be used, including Ringer's solution, or concentrated saline solution. A fluid can be selected to provide the desired therapeutic and physical properties when applied to the target tissue and a sterile fluid is recommended to guard against infection of the tissue.

[0046] Fluid can be urged from the fluid reservoir 212 into the inner lumen 206 by a pump 216. The pump 216 can be a syringe-type pump that produces a fixed volume flow with advancement of a plunger (not shown). An example of such a pump is a Model 74900 sold by Cole-Palmer Corporation of Chicago, IL. Other types of pumps, such as a diaphragm pump, may also be employed.

[0047] The pump 216 can be controlled by a power supply and controller 218. The power supply and controller 218 can deliver electrical control signals to the pump 216 to cause the pump to produce a desired flow rate of fluid. The power supply and controller 218 can be

connected to the pump 216 via an electrical connection 220. The power supply and controller 218 can also be electrically connected to the elongate body 202 via connection 222, and to a collector electrode 224 via connection 226. In addition, the power supply and controller 218 can be connected to the heating assembly 210 through a similar electrical connection, as described below.

[0048] The collector electrode 224 can have a variety of forms. For example, the collector electrode 224 can be a large electrode located outside a patient's body. In other embodiments, the collector electrode 224 can be a return electrode located elsewhere along the elongate body 202, or it can be located on a second elongate body introduced into a patient's body at a different location.

[0049] In operation, the power supply and controller 218 can drive the delivery of fluid into target tissue at a desired flow rate, the heating of the fluid to a desired therapeutic temperature, and the delivery of therapeutic ablative energy via the one or more ablation elements, such as electrode 205. To do so, the power supply and controller 218 can itself comprise a number of components for generating, regulating, and delivering required electrical control and therapeutic energy signals. For example, the power supply and controller 218 can include one or more frequency generators to create one or more RF signals of a given amplitude and frequency. These signals can be amplified by one or more RF power amplifiers into relatively high-voltage, high-amperage signals, *e.g.*, 50 volts at 1 amp. These RF signals can be delivered to the ablation element via one or more electrical connections 222 and the elongate body 202 such that RF energy is passed between the emitter electrode 205 and the collector electrode 224 that can be located remotely on a patient's body. In embodiments in which the elongate body is formed from non-conductive material, the one or more electrical connections 222 can extend through the inner lumen of the elongate body or along its outer surface to deliver current to the emitter electrode 205. The passage of RF energy between the ablation element and the collector electrode 224 can heat the tissue surrounding the elongate body 202 due to the inherent electrical resistivity of the tissue. The power supply and controller 218 can also include a directional coupler to feed a portion of the one or more RF signals to, for example, a power monitor to permit adjustment of the RF signal power to a desired treatment level.

[0050] The elongate body 202 illustrated in FIG. 2 can be configured for insertion into a patient's body in a variety of manners. FIG. 3 illustrates one embodiment of a medical

device 300 having an elongate body 302 coupled to a distal end thereof and configured for laparoscopic or direct insertion into a target area of tissue. In addition to the elongate body 302, the device 300 includes a handle 304 to allow an operator to manipulate the device. The handle 304 includes one or more electrical connections 306 that connect various components of the elongate body (*e.g.*, the heating assembly and ablation element 305) to, for example, the power supply and controller 218 described above. The handle 304 also includes at least one fluid conduit 308 for connecting a fluid source to the device 300. In the device 300 shown in FIG. 3, the handle 304 extends from the elongate body 302 along a common longitudinal axis. In other words, the longitudinal axes of the elongate body 302 and the handle 304 are collinear, or at least parallel. Thus, the overall length of the device 300 is the combined longitudinal lengths of the elongate body 302 and handle 304. Furthermore, even more additional overall length may be added to the device as a result of the at least one electrical connection 306 and fluid conduit 308 that can extend along the same longitudinal axis from a proximal end of the handle 304.

[0051] The device 300 shown in FIG. 3 can be used in percutaneous or laparoscopic procedures conducted by interventional radiologists or other medical professionals. These procedures can provide fluid enhanced ablation therapy to a large number of regions within the body. However, due to the minimally invasive nature of the procedure (which does not require a large open incision, but rather a small incision for the elongate body 302 to pass through), visualizing the procedure can be difficult for the medical professional administering the therapy. As a result, fluid enhanced ablation therapy is often conducted with the aid of a medical imaging apparatus to visualize the position of the elongate body's distal end within the patient's body, as well as the effectiveness of the therapy.

[0052] While different medical facilities have access to different imaging apparatuses, common medical imaging tools employed in combination with fluid enhanced ablation therapy include, for example, X-ray Computed Tomography (CT) scanners, Magnetic Resonance Imaging (MRI) scanners, X-ray scanners, and ultrasound scanners. Several of these scanners, including, for example, CT scanners and MRI scanners, require placing or moving a patient through a space-constrained environment in order to produce an image of the targeted therapy site. FIG. 4, for example, illustrates one embodiment of a CT scanner 400. The CT scanner 400 includes a large scanner housing 402 having a small diameter cylindrical pass-through 404 that is not much larger than a patient 406. The patient 406 is

placed on a gurney or sliding tray 408 and subsequently moved back and forth through the pass-through 404. The X-ray computed tomography equipment in the scanner housing 402 rotates around the outer perimeter of the pass-through 404 and collects X-ray images of the patient from a variety of angles. Computer software then analyzes the collected images to construct a model of the patient's body.

[0053] One difficulty encountered when using a medical imaging apparatus, such as the CT scanner 400, is that the small diameter pass-through 404 is not large enough to accommodate a patient having one or more devices, such as device 300, protruding from the patient's body. This is the result of the extended length of the device 300. As mentioned above, the fact that the longitudinal axes of the handle 304 and elongate body 302 are parallel or collinear means that the overall length of the device 300 is extended. This greater overall length produces a larger required clearance space around a patient's body. In many situations, the patient cannot be moved through the pass-through 404 of the CT scanner 400 without the handle 304 of the device 300 contacting the scanner housing 402, thereby upsetting the positioning of the device 300.

[0054] This potential interference between ablation and imaging components can require the removal of any devices, such as the device 300, that may be protruding from the patient prior to conducting medical imaging. Removing the ablation devices from the patient is undesirable because it can be difficult to reposition the devices correctly and because it can be difficult to gauge the therapy progress if the devices are not visible in the images.

[0055] To solve these problems, the low profile devices and methods of the present invention include a device manipulation handle that extends at an angle to the longitudinal axis of the elongate body. One embodiment of such a device 500 is illustrated in FIG. 5. The device 500 includes an elongate body 502 and a handle 504 coupled to the elongate body for manipulating it within a patient's body. The elongate body 502 can be similar to the elongate body 202 discussed above. For example, the elongate body 502 can include a proximal end 506, a distal end 508, and an inner lumen extending longitudinally through the elongate body. Furthermore, the elongate body 502 can include at least one ablation element disposed along a length thereof adjacent to one or more outlet ports formed in the elongate body that are configured to deliver fluid into tissue surrounding the elongate body.

[0056] The handle 504 can extend between a proximal end 510 and a distal end 512. The distal end 512 of the handle 504 can be coupled to the proximal end 506 of the elongate body 502 such that manipulation of the handle results in corresponding manipulation of the elongate body. Furthermore, the longitudinal axis of the elongate body 502 can extend at an angle  $\alpha$  to the longitudinal axis of the handle 504. The angle  $\alpha$  formed between the elongate body 502 and the handle 504 can, in some embodiments, be about 90 degrees. Such an angle extends the handle away from the elongate body 502 similar to a pistol grip and minimizes the length of the device 500 along the longitudinal axis of the elongate body 502. In other embodiments, however, the angle  $\alpha$  can be acute, or less than 90 degrees, such that the handle extends partially back toward the distal end 508 of the elongate body 502. In still other embodiments, the angle  $\alpha$  can be obtuse, or greater than 90 degrees, to ease the severity of the turn that internal conduits must make in routing through the handle into the elongate body. For example, in some embodiments, the angle  $\alpha$  can be in a range of about 10 degrees to about 120 degrees, while in other embodiments the angle  $\alpha$  can be in a range of about 30 degrees to about 100 degrees. In still other embodiments, the angle  $\alpha$  can be in a range of about 45 degrees to about 90 degrees.

[0057] Similar to the elongate body 502, the handle 504 can include one or more inner lumens extending therethrough to allow electrical and fluid connections 514, 516 to pass through the handle. To this end, any inner lumens extending through the handle 504 can be in communication with the inner lumen of the elongate body 502.

[0058] In some embodiments, the device 500 can also include an insertion stopping element 518 slidably disposed on the elongate body 502. The insertion stopping element 518 can have a larger cross sectional area than the elongate body 502 and can function to prevent over-insertion of the device 500 into a patient's body. The insertion stopping element 518 can be configured to slide along the elongate body but retain its position with an interference fit. In such an embodiment, the insertion stopping element 518 can be set at a variety of adjustable depths and prevent insertion beyond the set depth during a procedure. The insertion stopping element 518 can be formed from a variety of materials, including, for example, rubber or other polymer materials. In certain embodiments, the insertion stopping element can include a flat or concave distal face configured to abut against a patient's skin surface and a sloping proximal face that couples to the distal end 512 of the handle 504.

[0059] The handle 504 can have a variety of shapes and sizes depending on the preferences of the user, the size of the elongate body, etc. For example, the handle 504 can be shaped to extend in a straight line between its proximal end 510 and distal end 512. In some embodiments, however, the handle can have a contour along a longitudinal length thereof, as shown in FIG. 5. The contoured shape of the handle can be employed to allow for more comfortable gripping and manipulation by a user's hand 520. With regard to size, the handle can be formed in a variety of sizes but, in some embodiments, can be about 12 cm long and have a width of about 2.5 cm.

[0060] In addition to various shapes and sizes, the handle 504 can also include various surface features to enhance the ability of a user to grip and manipulate the device 500. For example, the handle 504 can include a surface texture over a portion or the entirety of the handle, or can include one or more surface texturizing features to aid a user in gripping and manipulating the device 500. For example, FIG. 6 depicts the device 500 from an alternate view and shows a plurality of grooves 602 formed on the surface of the handle 504 near its distal end 512. These grooves can provide a surface that more effectively grips, for example, the thumb of a user's hand 520, as shown in FIG. 5. Such features can be especially beneficial for medical professionals wearing surgical gloves that can become covered in bodily fluids, saline, or other liquids during a procedure.

[0061] The handle 504 can be formed from a variety of materials depending on the intended use and required strength, stiffness, and other mechanical properties of the handle. For example, in some embodiments forming the handle (and all other components of the device 500) from a polymer or other non-magnetic material can be preferred so that the device can operate within the strong magnetic fields developed by an MRI scanner. Exemplary non-magnetic materials include, for example, polymers, aluminum, copper, and glass, etc.

[0062] A low profile handle according to the invention can reduce the overall length of the device 500 such that it can be used in combination with medical imaging devices, such as the CT scanner 400 shown in FIG. 4. FIG. 7 illustrates the reduced clearance space required around a patient when utilizing an ablation device having a handle that extends at an angle to the longitudinal axis of an elongate body inserted into a patient. The figure depicts a front view of the patient 406 being moved through the pass-through 404 in the scanner housing 402 on the sliding tray 408. Inserted into the patient's body is the device 500 described above. The handle 504 of the device 500 extends at an angle to the longitudinal axis of the

elongate body 502 and substantially parallel to a skin surface of the patient. As a result, the handle 504 is able to move through the pass-through 404 without interfering with the scanner housing 404, in contrast to the device 200 discussed above.

[0063] As mentioned above, the elongate body 502 coupled to the handle 504 can be similar to the elongate body 202 described above and can include, for example, one or more ablation elements disposed along a length thereof and at least one outlet port formed therein for delivering fluid from the inner lumen into tissue surrounding the elongate body. In some embodiments, however, the elongate body can also include at least one heating element disposed within the inner lumen of the elongate body and configured to heat fluid passing therethrough. Heating the fluid prior to its introduction into the tissue surrounding the elongate body can have a number of advantages including, for example, imparting a greater amount of thermal energy into the tissue and preventing the reduction in temperature of the ablation element upon contact therewith, as discussed above. The heating element can have a number of different configurations but, in some embodiments, the heating element can include at least one wire and at least one spacer where the at least one wire is configured to pass energy through the fluid flowing through the inner lumen of the elongate body. By passing energy, *e.g.*, RF electrical energy, through the fluid flowing through the inner lumen of the elongate body, the fluid can become heated due to its natural resistivity.

[0064] FIG. 8 illustrates one embodiment of a heating element including two wires and two spacers. An elongate body 802, similar to elongate body 502, having a proximal end and a pointed distal end 804 includes an inner lumen 806. The elongate body 802 can also include at least one ablation element, such as emitter electrode 805, that is configured to deliver RF energy to tissue surrounding the elongate body 802. The electrode 805 also includes one or more outlet ports 708 configured to deliver fluid from the inner lumen 806 into surrounding tissue.

[0065] Disposed within the inner lumen 806 is a heating assembly that includes two wires 810, 812 that are suspended a distance apart by one or more spacers 814, 814'. The wires 810, 812 can be connected to a power source such that electrical energy can be passed between the wires through the fluid flowing in the inner lumen 806. The passage of electrical (*e.g.*, RF) energy through the fluid in the inner lumen 806 can cause the fluid to increase in temperature due to the natural electrical resistivity of the fluid, similar to the mechanism discussed above by which tissue surrounding the elongate body can be heated using RF

energy. The wires 810, 812 can be formed from any conductive material, similar to the materials discussed above in connection with the electrode 205. In one embodiment, however, the wires 810, 812 can be formed from silver wire and can have an exposed chlorided surface between or adjacent to the spacers 814, 814'. As discussed above, these materials can participate in an ion exchange process that minimizes the voltage drop across the wire/fluid interface and prevents excessive heating of the surrounding fluid.

[0066] In order to effectively pass energy through the fluid flowing within the inner lumen 806, in an exemplary embodiment, the wires 810, 812 (or at least the exposed portion of the wires) are held in an optimum relation to one another by the spacers 814, 814'. This prevents the wires from contacting each other and producing an electrical short. In some embodiments, the wires 810, 812 are exposed for only a short distance located just proximal of the electrode 805 and outlet ports 808. As shown in FIG. 8, the wires can be exposed for a distance  $d_1$  between the two spacers 814, 814' that are positioned at a proximal and a distal end of a distal portion of the wires. The distance  $d_1$  can vary and, in one embodiment, can be about 5 mm. Proximal to the spacer 814, the wires 810, 812 can be covered in an electrically insulating material 818 to prevent the passage of electrical energy therebetween. In addition, the wires 810, 812 can also be prevented from directly contacting the elongate body 802, as an electrical short can result from both of the wires 810, 812 simultaneously contacting the electrically conductive elongate body. Accordingly, in some embodiments, the elongate body 802 can be lined with an insulating material 820, such as a plastic tube, liner, or coating disposed on the inner walls of the elongate body 802.

[0067] The inner lumen 806 can also house one or more temperature sensors to monitor and assist in controlling the heating of fluid flowing within the inner lumen. The embodiment illustrated in FIG. 8 includes a chromel-constantan fine-wire thermocouple configured to float in the fluid distal of the spacer 814' by a distance  $d_2$ . One skilled in the art will appreciate that thermocouples are just one example of temperature sensors that can be employed to measure the temperature of the flowing fluid and that a variety of sensors, including thermistors and diodes, can also be used. Further, distance  $d_2$  can vary and, in one embodiment, it can be about 10 mm. The thermocouple 822 can also be disposed a distance  $d_3$  proximal to the electrode 805 and outlet ports 808. While this distance can vary as well, in one embodiment, the distance  $d_3$  is about 2 mm. The distances  $d_1$ ,  $d_2$ , and  $d_3$  (and the corresponding positions of the spacers 814, 814') can be chosen to allow for sufficient heating

of fluid flowing in the inner lumen 806, as well as to allow sufficient mixing of the heated fluid prior to flowing through outlet ports 808 so as to assure that the fluid being injected into tissue surrounding the elongate body 802 has a uniform temperature. However, the distances  $d_2$  and  $d_3$  should be minimized such that heating of the fluid flowing within the inner lumen 806 occurs as close to the outlet ports 808 as possible. This configuration minimizes the thermal losses and unintentional environmental heating associated with transporting heated fluids from remote locations within a patient's body.

[0068] FIG. 9 illustrates an exemplary electrical circuit for delivering RF energy to both tissue surrounding the elongate body 802 and fluid flowing through the inner lumen 806 of the elongate body 802. In the illustrated embodiment, two separate power sources 902, 904 are utilized to deliver electrical energy including, for example, RF energy. The power source 902 can be connected to the two wires 810, 812 running through the inner lumen 806 of the elongate body 802. By passing electrical current through the wires, energy can be transmitted through the fluid flowing within the inner lumen 806 between the exposed portions of the wires 810, 812.

[0069] The power source 904 can be connected to both the elongate body 802 and a collector electrode 906. The collector electrode can be located remotely on a patient's body, for example, placed under a patient's back on an operating table. In other embodiments, the collector electrode 906 can be co-located on the elongate body 802 or it can be located on a second elongate body positioned nearby the elongate body 802.

[0070] The power source 904 can deliver RF energy from the electrode 805 to the collector electrode 906 by passing electrical current through the elongate body 702. The two power sources 802, 804 do not share a common electrical ground and therefore remain electrically isolated from one another. This ensures that power from the source 902 heats only saline flowing within the elongate body 802, while power from the source 904 heats only tissue surrounding the elongate body 802. The spacers and insulating materials discussed above prevent a short between the two wires 810, 812 that can result from the wires touching each other or simultaneously contacting the elongate body 802. One skilled in the art will appreciate that a variety of combinations of spacers and insulating materials covering the wires and/or the inner walls of the elongate body can be used to prevent such an electrical short circuit.

[0071] In an exemplary embodiment, as saline solution is pumped through the elongate body's inner lumen 706, the saline can be heated above body temperature by the power source 802, preferably to between about 50° C and about 70° C. This can be accomplished by delivering RF energy to the fluid within the inner lumen 706 via the wires 710, 712. For example, typical fluid enhanced ablation therapy operating parameters involve the application of 20 volts or more to the wires 710, 712. In some embodiments, the applied voltage can go as high as 120 volts and, in some embodiments, can be about 30 volts (*e.g.*, 31.25 volts in one embodiment). The heated, flowing saline solution can be subsequently injected into tissue surrounding the elongate body 702 via the outlet ports 708 at a variety of flow rates. For example, in some embodiments fluid can be ejected from the elongate body 702 at a flow rate of about 10 ml/min. The delivery of heated fluid can be done independently or in conjunction with the delivery of ablative energy from the power source 804. The operating parameters of fluid enhanced ablation therapy can vary according to a number of factors, including the desired therapeutic effect, the geometry and tissue properties of the treatment volume, etc. By way of example, in one embodiment ablation therapy conducted in a patient's liver can heat saline to 50° C using 40 watts of power and deliver the saline at 10 ml/min for about 5 minutes. By way of further example, ablation therapy using these same parameters can be delivered for only about 90 seconds when treating cardiac tissue. While the particular properties of the intended treatment site will ultimately govern the selected operating parameters, fluid enhanced ablation therapy typically involves the delivery of saline at a rate between about 0 and about 20 ml/min. The saline is typically heated to between about 50° C and 80° C using up to 80 watts of power and up to 120 volts. Fluid heated according to these exemplary operating parameters can be combined with electrical energy delivered directly to the tissue to conduct ablation therapy. In some embodiments, up to 100 watts of power can be applied to the tissue from, for example, an emitter electrode.

[0072] While the preceding discussion has described a two wire, two spacer heating element configuration, other configurations are possible as well. Further information on heating elements for use in fluid enhanced ablation therapy is available in U.S. Patent No. 6,328,735 to Curley et al. and U.S. Pat. Appl. No. 13/445,036, filed on April 12, 2012, and entitled "Methods and Devices for Heating Fluid in Fluid Enhanced Ablation Therapy." The contents of each of these references are hereby incorporated by reference in their entirety.

[0073] Methods for the administration of fluid enhanced ablation therapy using the low profile devices described herein are also provided. For example, a method for administering fluid enhanced ablation therapy can include percutaneously inserting a distal end of an elongate body of an ablation device into a patient's body. The method can further include manipulating the distal end of the elongate body within the patient's body using a low profile handle coupled to the proximal end of the elongate body and having a longitudinal axis that extends at an angle to a longitudinal axis of the elongate body. Finally, the method can include delivering fluid through the elongate body of the ablation device into tissue surrounding the distal end of the elongate body while simultaneously delivering energy into tissue surrounding the distal end of the elongate body.

[0074] Manipulating and delivering fluid and energy through a low profile device having a handle extending at an angle to the longitudinal axis of the elongate body can reduce the amount of clearance required around a patient due to the decreased overall length of the ablation therapy device. Furthermore, the decreased clearance space can allow fluid enhanced ablation therapy procedures to be carried out in conjunction with medical imaging without having to repeatedly remove and reintroduce the ablation devices being used.

[0075] For example, in some embodiments, methods for administering fluid enhanced ablation therapy can include imaging at least a portion of the patient using a medical imaging apparatus. When the low profile devices and methods of the invention are utilized, imaging can occur simultaneously with any of the method steps for manipulating the devices or delivering fluid and energy into tissue surrounding the elongate bodies inserted into tissue. Still further, in some embodiments, both the method steps for manipulating the devices and delivering fluid and energy into tissue can be conducted inside a medical imaging apparatus, such as the CT scanner 400. Other exemplary medical imaging apparatuses include, for example, an MRI scanner, an ultrasound scanner, and an X-ray scanner.

[0076] In other embodiments, the methods of the invention can also include heating the fluid inside the elongate body prior to delivering the fluid into the tissue surrounding the elongate body. This can be accomplished, for example, by passing energy through one or more wires disposed within the inner lumen of the elongate body, as discussed above.

[0077] The low profile devices disclosed herein can be designed to be disposed after a single use, or they can be designed for multiple uses. In either case, however, the devices can be

reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of a device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, a device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, a device can be reassembled for subsequent use either at a reconditioning facility or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that the reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present invention.

[0078] For example, the devices disclosed herein may be disassembled partially or completely. In particular, the elongate body portion of any device can be removed from the handle portion of the device, or the elongate body and handle can be decoupled from the electrical and fluid connections joining the device to the remainder of the fluid enhanced ablation system. In other embodiments, solely the distal portion of an elongate body (*e.g.*, on the portion that extends into a patient's body) can decouple from a proximal portion that can remain connected to the handle of the device. In yet another embodiment, the handle, elongate body, and connections can be removably coupled to a housing that contains, for example, the fluid reservoir, pump, and power supply and controller shown in FIG. 2. These are exemplary disassembly steps only, as any component of the device can be configured to separate from the device for cleaning and/or replacement.

[0079] Preferably, the devices described herein will be processed before surgery. First, a new or used instrument can be obtained and, if necessary, cleaned. The instrument can then be sterilized. In one sterilization technique, the instrument is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and its contents can then be placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation can kill bacteria on the instrument and in the container. The sterilized instrument can then be stored in the sterile container. The sealed container can keep the instrument sterile until it is opened in the medical facility.

[0080] In many embodiments, it is preferred that the device is sterilized. This can be done by any number of ways known to those skilled in the art including beta or gamma radiation, ethylene oxide, steam, and a liquid bath (*e.g.*, cold soak). In certain embodiments, the

materials selected for use in forming components such as the elongate body may not be able to withstand certain forms of sterilization, such as gamma radiation. In such a case, suitable alternative forms of sterilization can be used, such as ethylene oxide.

[0081] All papers and publications cited herein are hereby incorporated by reference in their entirety. One skilled in the art will appreciate further features and advantages of the invention based on the above-described embodiments. Accordingly, the invention is not to be limited by what has been particularly shown and described, except as indicated by the appended claims.

[0082] What is claimed is:

## CLAIMS:

1. An ablation device, comprising:
  - an elongate body having
    - proximal and distal ends,
    - an inner lumen extending longitudinally through the elongate body, and
    - at least one outlet port formed in the elongate body configured to deliver fluid to tissue surrounding the elongate body;
  - at least one ablation element disposed along a length of the elongate body adjacent to the at least one outlet port and configured to deliver energy to tissue surrounding the elongate body;
  - at least one heating element disposed within the inner lumen of the elongate body and configured to heat fluid passing therethrough; and
  - a handle having proximal and distal ends, the distal end of the handle being coupled to the proximal end of the elongate body;wherein a longitudinal axis of the elongate body extends at an angle to a longitudinal axis of the handle.
2. The ablation device of claim 1, wherein the angle between the longitudinal axis of the elongate body and the longitudinal axis of the handle is in a range of about 10 degrees to about 120 degrees.
3. The ablation device of claim 1, wherein the angle between the longitudinal axis of the elongate body and the longitudinal axis of the handle is in a range of about 30 degrees to about 100 degrees.
4. The ablation device of claim 1, wherein the angle between the longitudinal axis of the elongate body and the longitudinal axis of the handle is in a range of about 45 degrees to about 90 degrees.
5. The ablation device of claim 1, wherein the angle between the longitudinal axis of the elongate body and the longitudinal axis of the handle is about 90 degrees.
6. The ablation device of claim 1, wherein the handle includes an inner lumen extending therethrough.

7. The ablation device of claim 6, wherein the inner lumen extending through the elongate body is in communication with the inner lumen extending through the handle.
8. The ablation device of claim 1, wherein the handle is contoured along a longitudinal length thereof.
9. The ablation device of claim 1, further comprising an insertion stopping element slidably disposed on the elongate body.
10. The ablation device of claim 1, wherein the handle is formed from a non-magnetic material.
11. The ablation device of claim 1, wherein the handle includes a surface texture to improve a user's grip of the handle.
12. The ablation device of claim 1, wherein the at least one heating element comprises at least one wire and at least one spacer, the at least one wire being configured to pass energy through the fluid flowing through the inner lumen of the elongate body.
13. A method for administering fluid enhanced ablation therapy, comprising:
  - percutaneously inserting a distal end of an elongate body of an ablation device into a patient;
  - manipulating the distal end of the elongate body within the patient using a low profile handle coupled to the proximal end of the elongate body and having a longitudinal axis that extends at an angle to a longitudinal axis of the elongate body;
  - delivering fluid through the elongate body of the ablation device into tissue surrounding the distal end of the elongate body while simultaneously delivering energy into tissue surrounding the distal end of the elongate body.
14. The method of claim 13, further comprising imaging at least a portion of the patient using a medical imaging apparatus.
15. The method of claim 14, wherein imaging occurs simultaneously with any of the manipulating step and the delivering step.
16. The method of claim 14, wherein the patient is positioned within the medical imaging apparatus during at least a portion of the method.

17. The method of claim 14, wherein the manipulating step and the delivering step are conducted inside the medical imaging apparatus
18. The method of claim 14, wherein the imaging apparatus is selected from the group consisting of an X-ray Computed Tomography (CT) scanner, a Magnetic Resonance Imaging (MRI) scanner, an ultrasound scanner, and an X-ray scanner.
19. The method of claim 13, further comprising heating the fluid inside the elongate body prior to delivering the fluid into the tissue surrounding the elongate body.

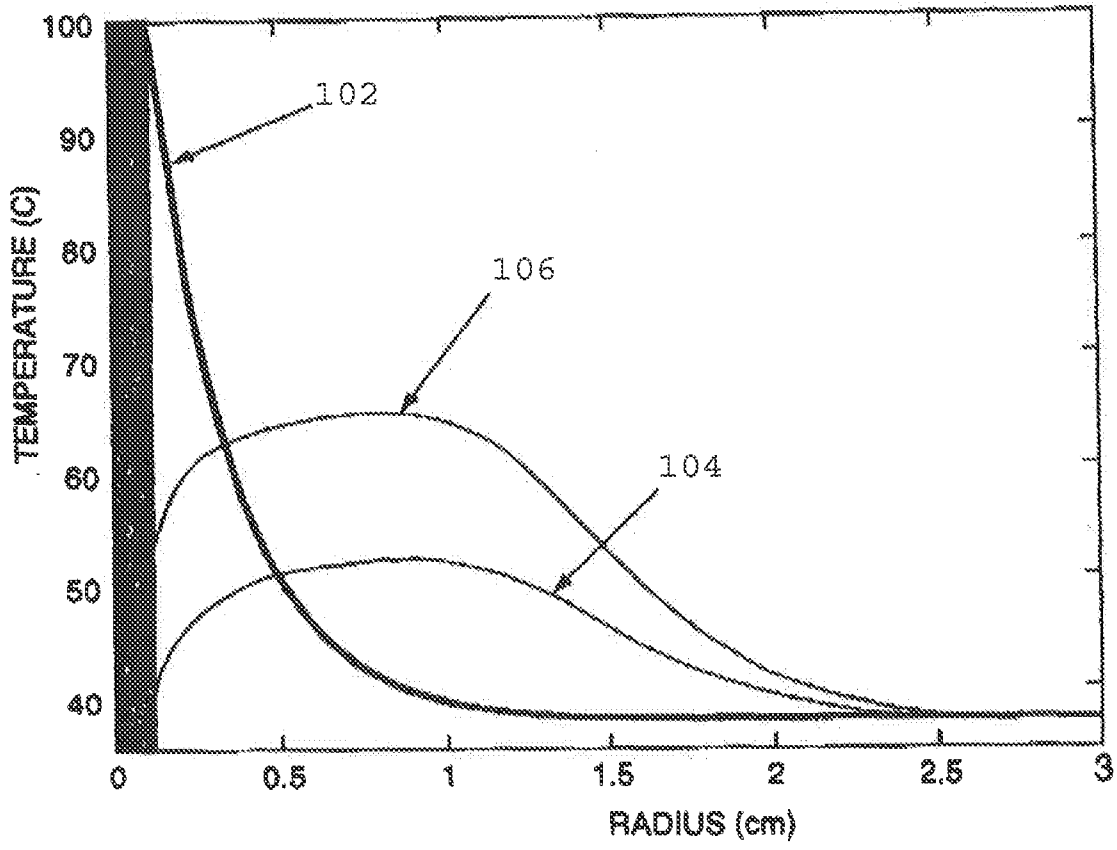


FIG. 1

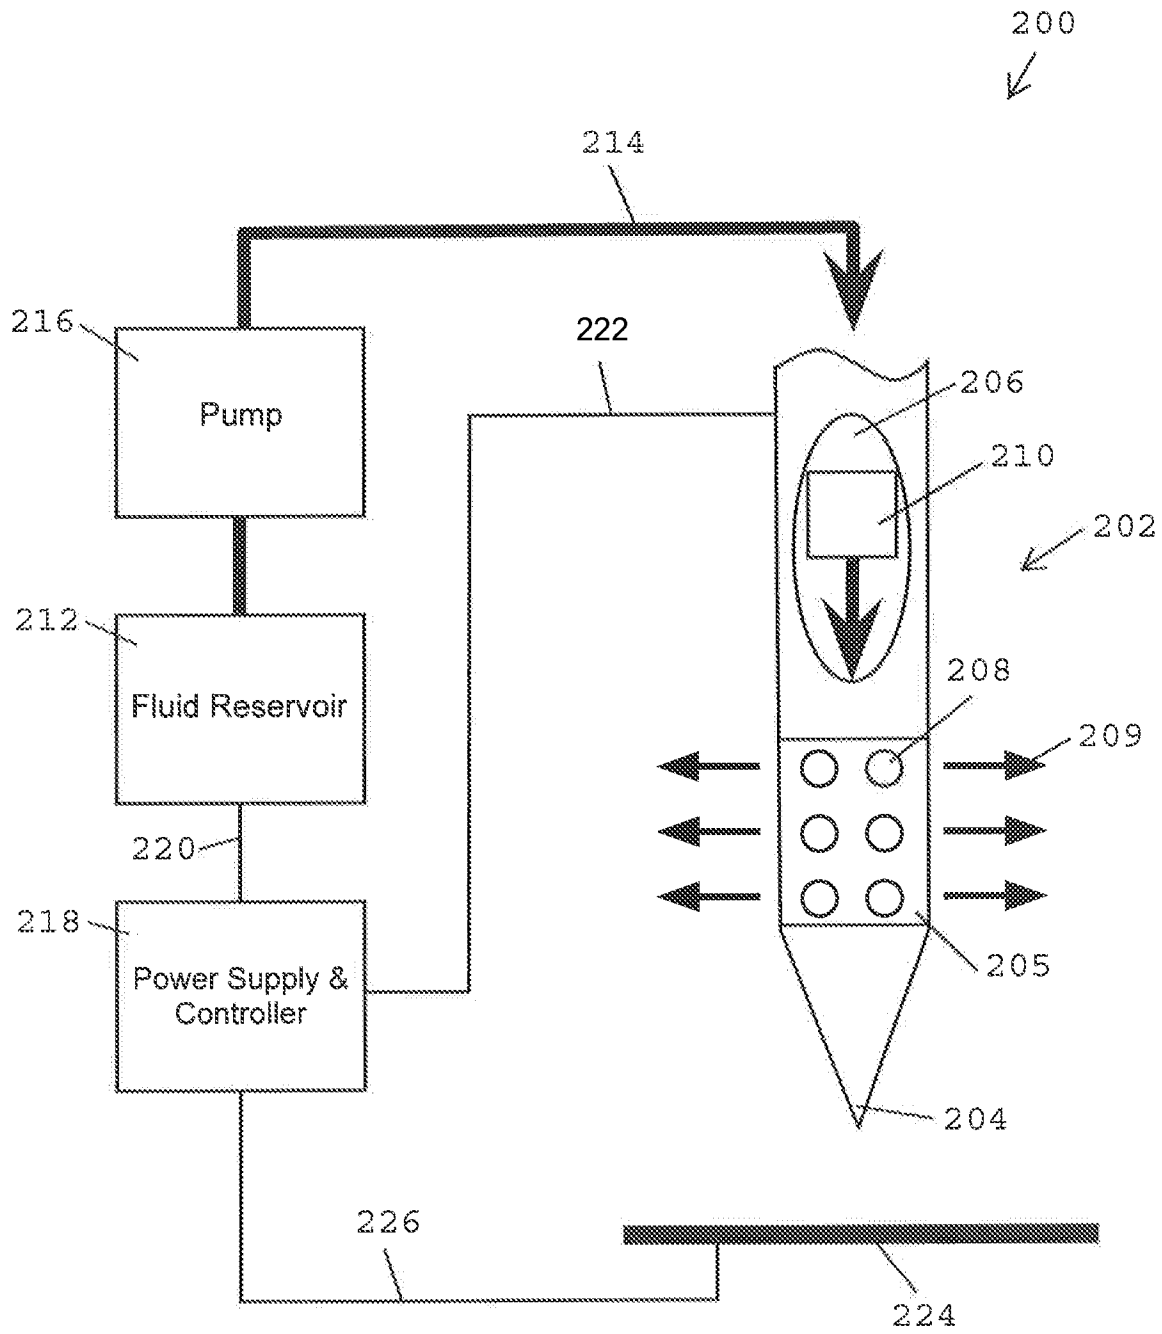


FIG. 2

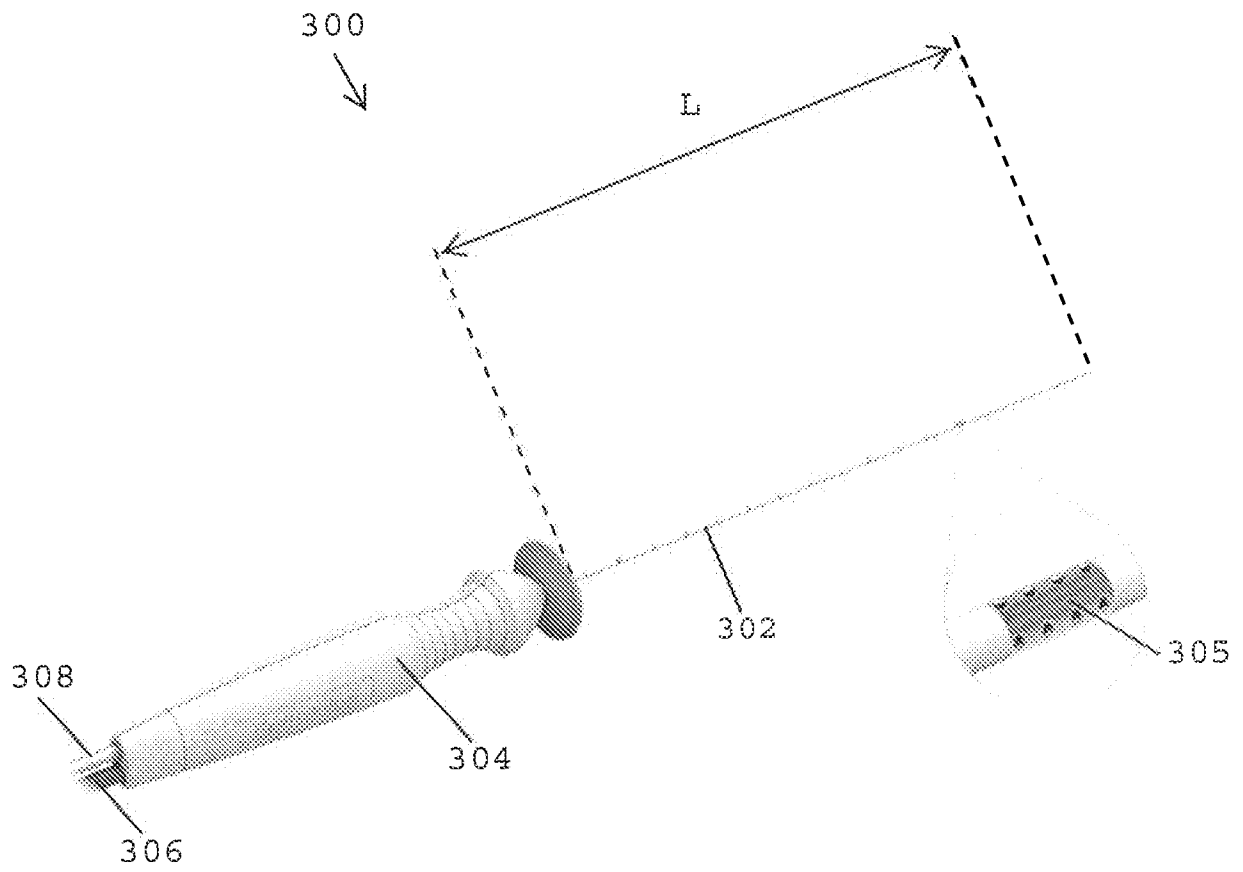


FIG. 3

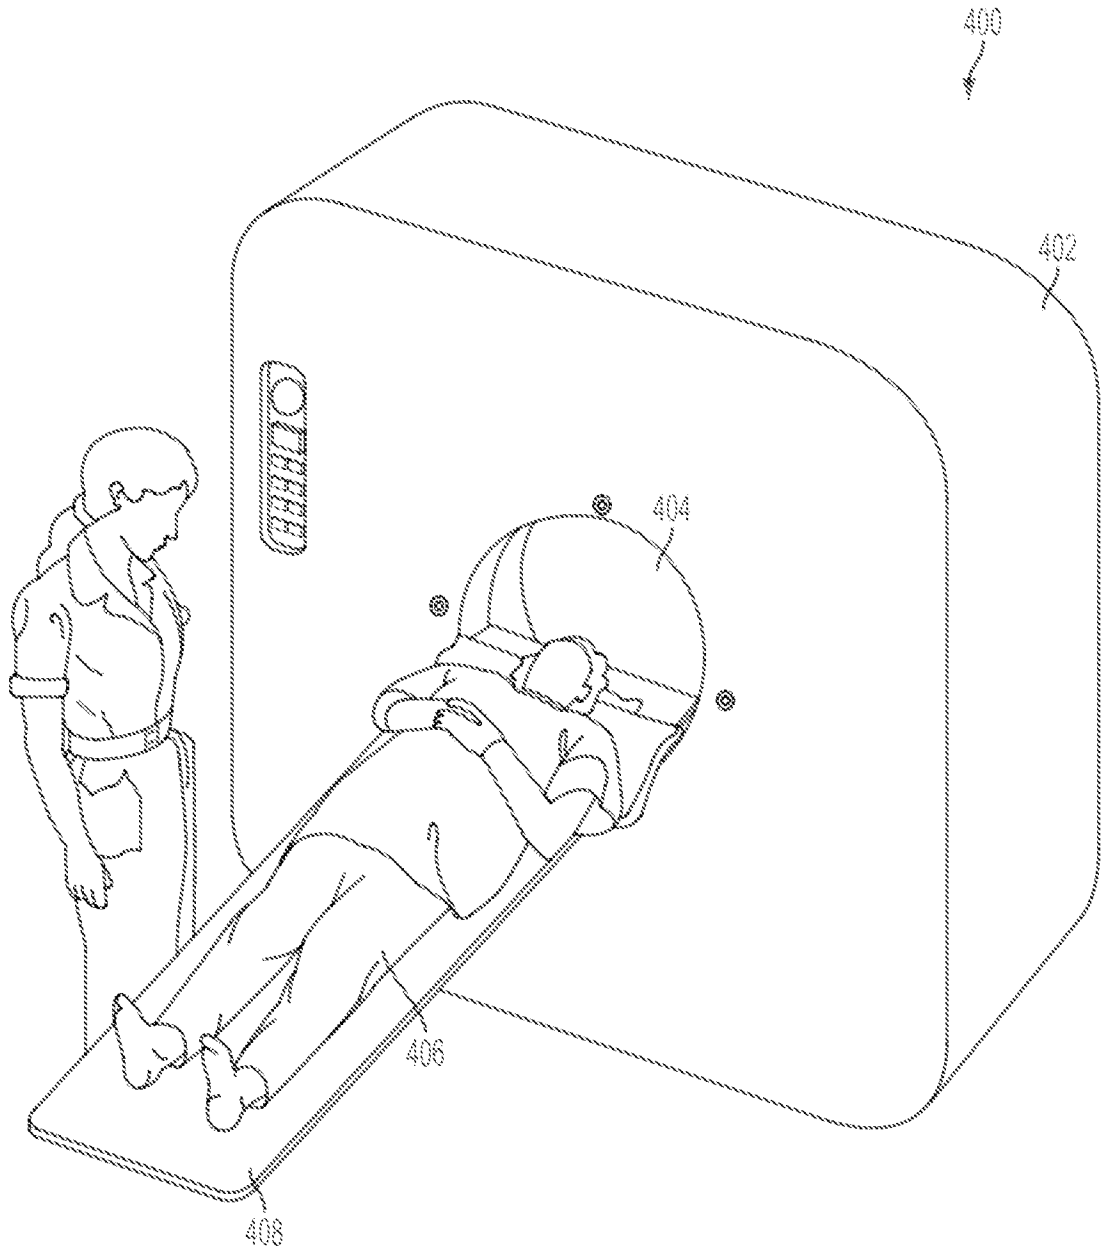


FIG. 4

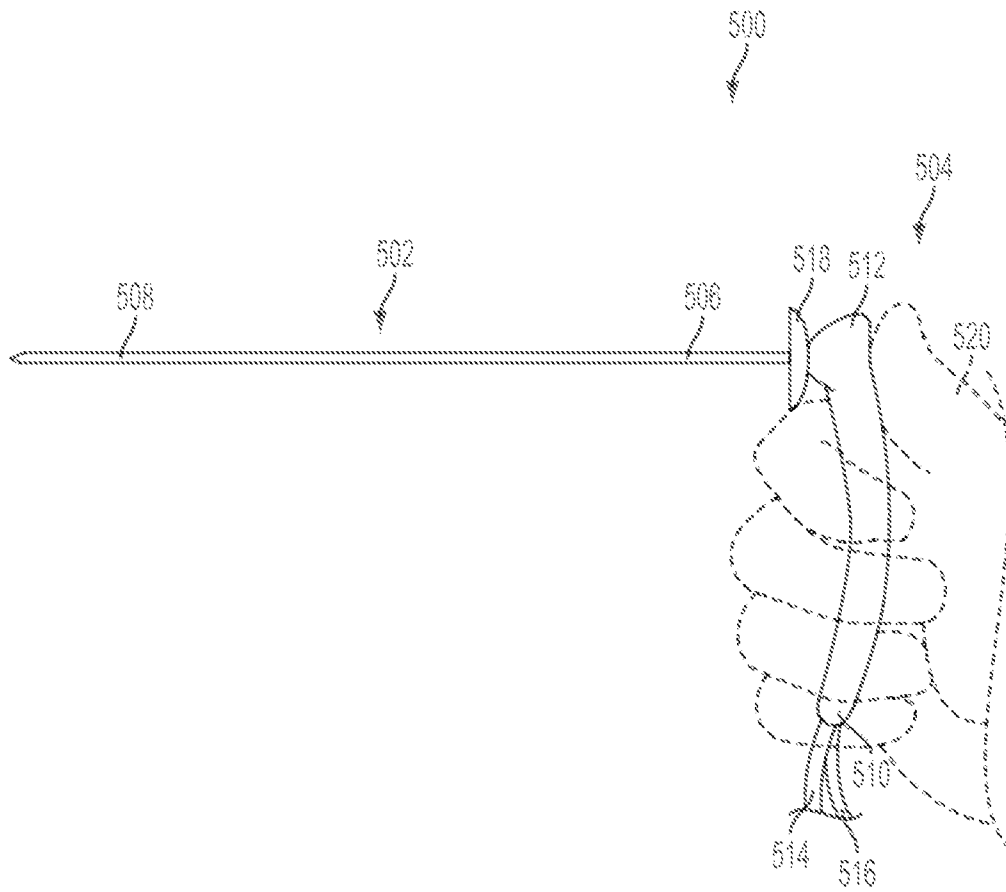


FIG. 5

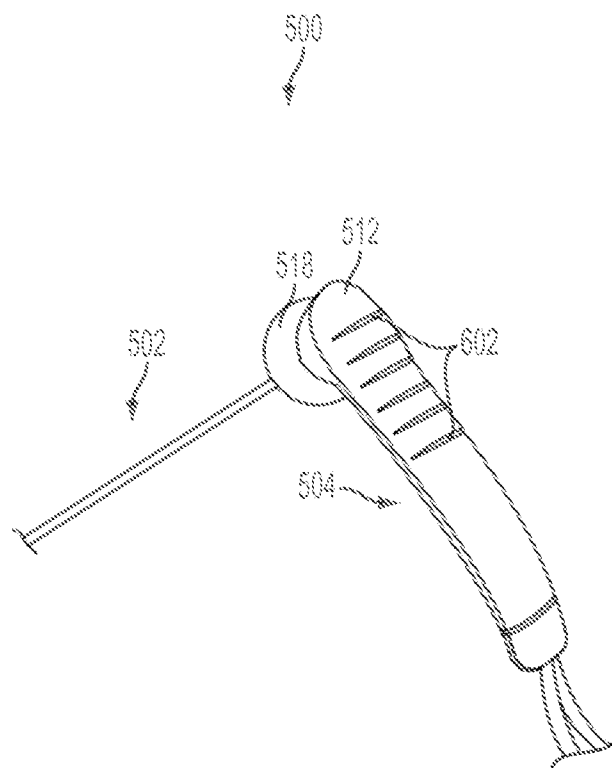


FIG. 6

7/9

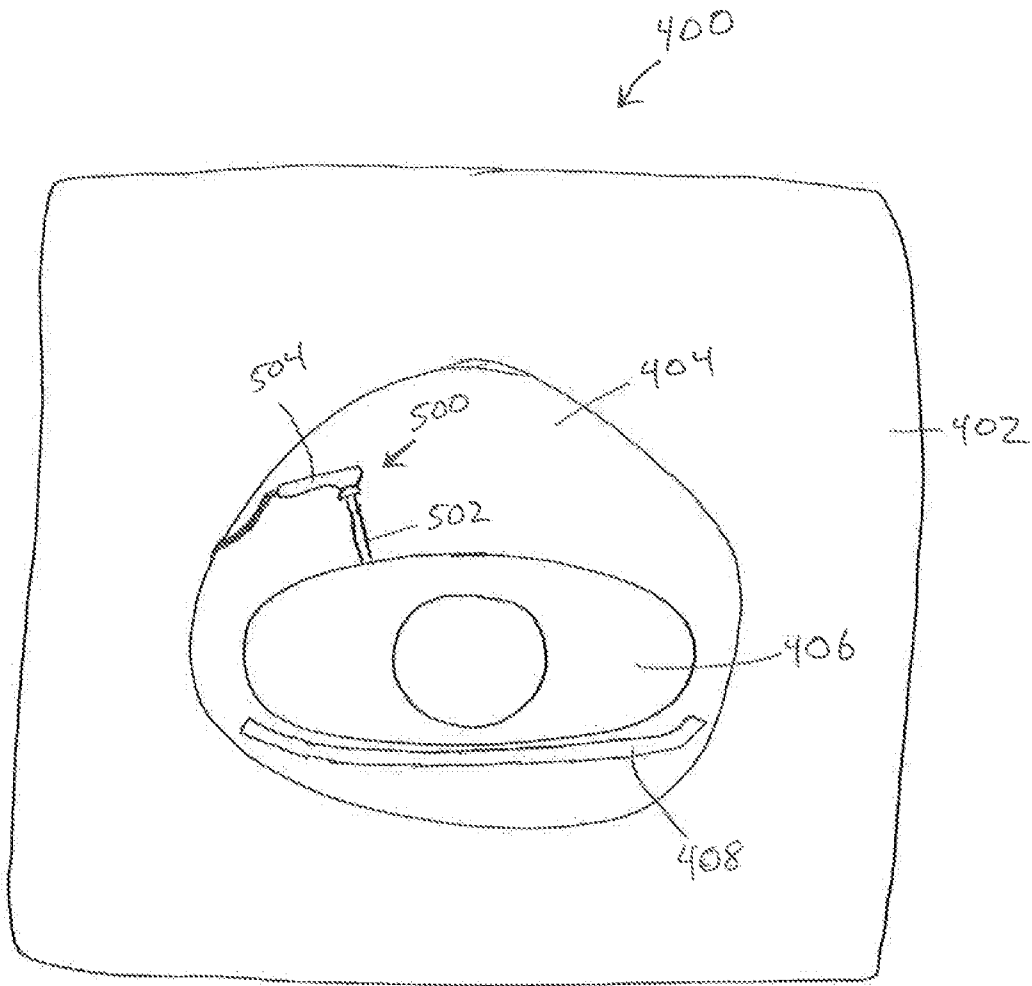


FIG. 7

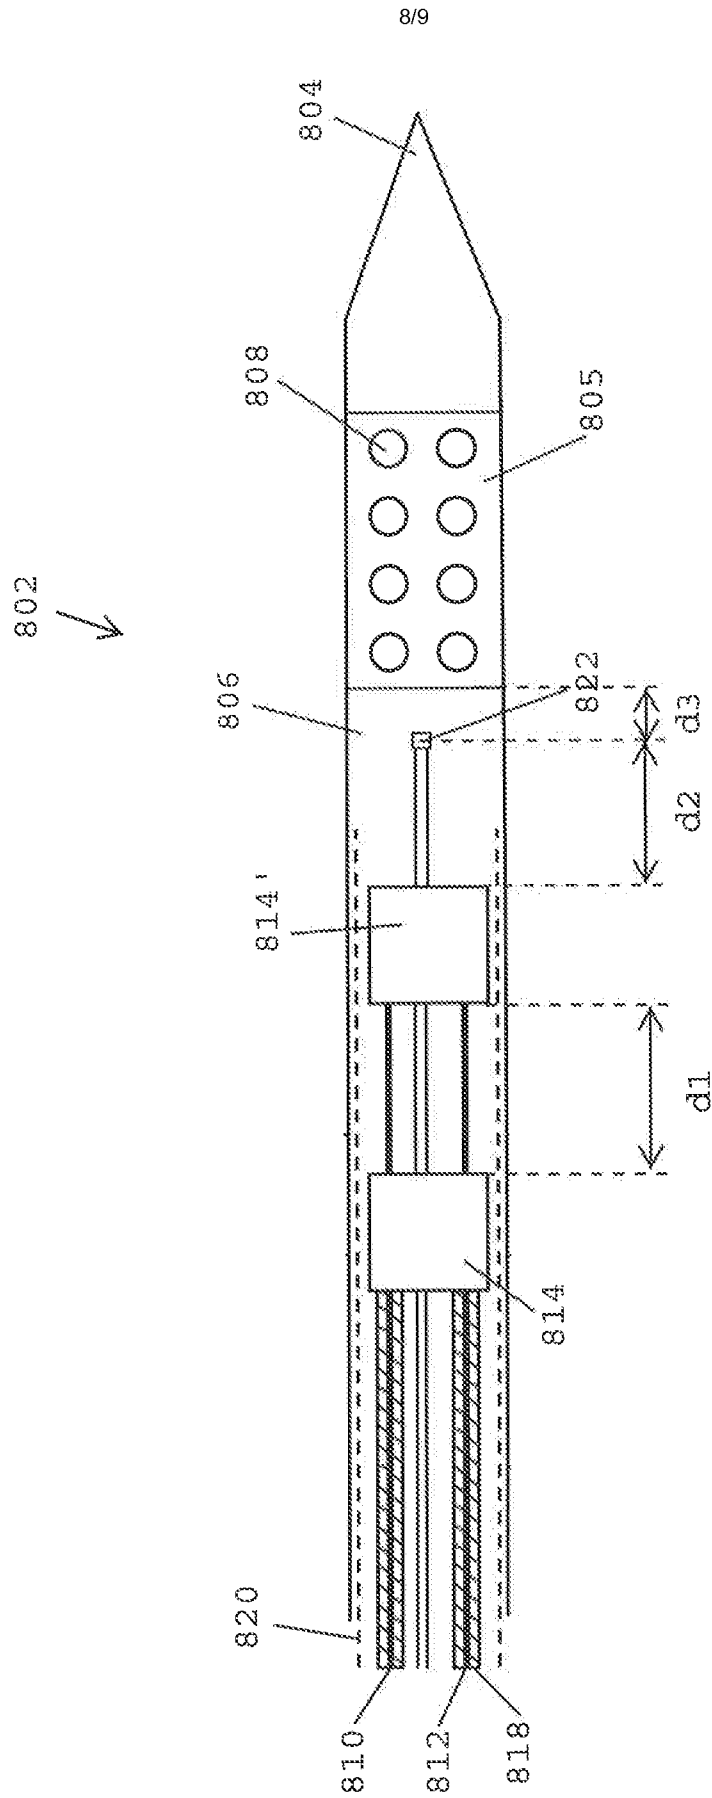


FIG. 8

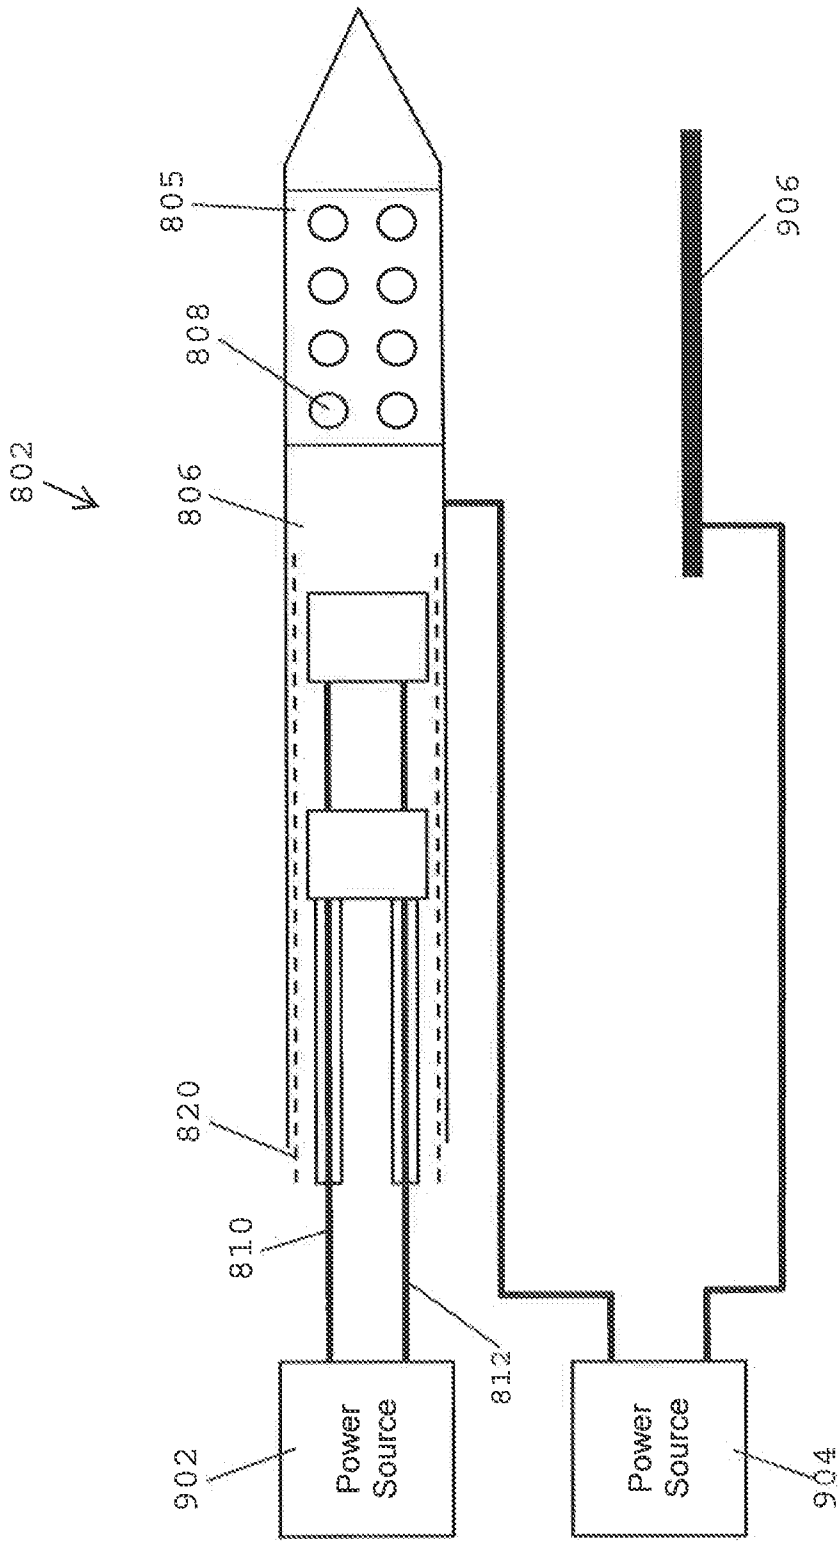


FIG. 9

**A. CLASSIFICATION OF SUBJECT MATTER**

A61B 18/12(2006.01)i, A61B 18/14(2006.01)i, A61B 17/3203(2006.01)i, A61B 6/00(2006.01)i, A61B 5/055(2006.01)i

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)

A61B 18/12; A61B 5/04; A61B 18/14; A61B 5/042; A61B 17/22; A61B 17/3203; A61B 6/00; A61B 5/055

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) &amp; Keywords: ablation, electrode, fluid, opening, angle, handle

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2002-0120259 A1 (LETTICE, J. J. et al.) 29 August 2002 See paragraphs [0125]-[0134], [0182]; figures 4-6.	1-12
Y	EP 1033107 A1 (CORDIS WEBSTER INC.) 06 September 2000 See paragraphs [0021], [0053]; figures 1, 6.	1-12
A	US 2005-0055019 A1 (SKARDA, J. R.) 10 March 2005 See claims 1-22; figures 1-7.	1-12
A	EP 0908156 B1 (RITA MEDICAL SYSTEMS, INC.) 12 November 2003 See the entire document.	1-12
A	US 2012-0108938 A1 (KAUPHUSMAN, J. V. et al.) 03 May 2012 See the entire document.	1-12



Further documents are listed in the continuation of Box C.



See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family


Date of the actual completion of the international search

14 November 2013 (14.11.2013)

Date of mailing of the international search report

**14 November 2013 (14.11.2013)**

Name and mailing address of the ISA/KR


 Korean Intellectual Property Office  
 189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City,  
 302-701, Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

Han, Inho

Telephone No. +82-42-481-3362



**Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1.  Claims Nos.: 13-19  
because they relate to subject matter not required to be searched by this Authority, namely:  
Claims 13-19 pertain to methods for treatment of human body and thus relate to a subject matter which this International Searching Authority is not required, under Article 17(2)(a)(i) of the PCT and Rule 39.1(iv) of the Regulations under the PCT, to search.
2.  Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3.  Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

**Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)**

This International Searching Authority found multiple inventions in this international application, as follows:

1.  As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2.  As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3.  As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
  
4.  No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

**Remark on Protest**

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.  
**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2002-0120259 A1	29/08/2002	AU 1996-60266 B2	10/06/1999
		AU 1997-10545 B2	04/03/1999
		AU 1997-10571 B2	09/09/1999
		AU 1997-24724 B2	07/10/1999
		AU 1998-97829 A1	27/04/1999
		AU 1999-11124 A1	10/05/1999
		AU 1999-11940 A1	10/05/1999
		AU 1999-14640 A1	15/06/1999
		AU 1999-19990 A1	05/07/1999
		AU 1999-32961 A1	06/09/1999
		AU 1999-39758 A1	23/11/1999
		AU 1999-48429 A1	17/01/2000
		AU 1999-52554 A1	28/02/2000
		AU 1999-57736 A1	06/03/2000
		AU 2000-16334 A1	19/06/2000
		AU 2000-39129 A1	09/10/2000
		AU 2000-42233 A1	02/11/2000
		AU 2000-46507 A1	02/11/2000
		AU 2000-51429 A1	12/12/2000
		AU 2001-43151 A1	27/08/2001
		AU 2001-61637 A1	18/02/2002
		AU 2001-61726 A1	24/12/2001
		AU 2003-237102 A1	10/11/2003
		AU 2003-248766 A1	19/01/2004
		CA 2129745 A1	08/07/1993
		CA 2162395 A1	24/11/1994
		CA 2221330 A1	19/12/1996
		CA 2237947 A1	29/05/1997
		CA 2287206 A1	17/12/1998
		CA 2318891 A1	26/08/1999
		EP 0624076 A1	28/10/1998
		EP 0624076 B1	02/12/1998
		EP 0820457 A1	11/08/2004
		EP 0865256 A1	12/03/2003
		EP 0865256 B1	19/03/2003
		EP 0882430 A2	09/12/1998
		EP 0882430 A3	20/01/1999
		EP 0917482 A1	05/01/2005
		EP 0917482 B1	09/09/2009
		EP 0921759 A1	07/02/2001
		EP 0921759 B1	31/08/2011
		EP 0998248 A1	10/05/2000
		EP 1009343 A1	21/06/2000
		EP 1018994 A1	19/07/2000
		EP 1018994 B1	21/09/2005
		EP 1024769 A1	09/08/2000
		EP 1024769 B1	25/02/2009
EP 1026996 A1	16/08/2000		
EP 1026996 B1	10/10/2007		

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		EP 1027020 A1	16/08/2000
		EP 1027020 B1	16/11/2005
		EP 1036547 A2	20/09/2000
		EP 1036547 A3	27/12/2000
		EP 1039862 A1	04/10/2000
		EP 1039862 B1	21/05/2008
		EP 1041933 A1	11/10/2000
		EP 1041933 B1	31/03/2004
		EP 1061857 A1	27/12/2000
		EP 1061857 B1	19/12/2007
		EP 1079746 A1	07/03/2001
		EP 1079746 B1	21/03/2007
		EP 1080680 A1	07/03/2001
		EP 1080682 A1	07/03/2001
		EP 1080682 B1	08/07/2009
		EP 1174093 A1	23/01/2002
		EP 1178757 A1	13/02/2002
		EP 1178758 A1	13/02/2002
		EP 1178758 B1	27/10/2010
		EP 1179320 A2	13/02/2002
		EP 1179320 A3	03/12/2003
		EP 1187570 A1	20/03/2002
		EP 1257221 A1	20/11/2002
		EP 1289438 A1	12/03/2003
		EP 1309282 A1	14/05/2003
		EP 1404236 A1	07/04/2004
		EP 1404236 B1	14/09/2011
		EP 1411847 A2	28/04/2004
		EP 1411847 B1	06/06/2012
		EP 1503688 A1	09/02/2005
		EP 1571969 A2	14/09/2005
		EP 1571969 A3	21/09/2005
		EP 1571969 B1	08/02/2012
		EP 1637087 A2	22/03/2006
		EP 1637087 A3	10/05/2006
		EP 1637087 B1	10/08/2011
		EP 1880686 A2	23/01/2008
		EP 1880686 A3	26/01/2011
		EP 2055253 A2	06/05/2009
		EP 2055253 A3	03/02/2010
		EP 2055254 A2	06/05/2009
		EP 2055254 A3	10/02/2010
		EP 2057954 A1	13/05/2009
		EP 2057954 B1	16/03/2011
		JP 10-510745 A	20/10/1998
		JP 11-501555 A	09/02/1999
		JP 11-502144 A	23/02/1999
		JP 11-503725 A	30/03/1999
		JP 2000-060868 A	29/02/2000
		JP 2000-515798 A	28/11/2000

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.  
**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		JP 2001-513395 A	04/09/2001
		JP 2001-518352 A	16/10/2001
		JP 2001-520081 A	30/10/2001
		JP 2001-522252 A	13/11/2001
		JP 2001-523513 A	27/11/2001
		JP 2002-503508 A	05/02/2002
		JP 2002-508214 A	19/03/2002
		JP 2002-513619 A	14/05/2002
		JP 2002-514097 A	14/05/2002
		JP 2002-541902 A	10/12/2002
		JP 2002-541904 A	10/12/2002
		JP 2003-500099 A	07/01/2003
		JP 2003-527875 A	24/09/2003
		JP 2004-505663 A	26/02/2004
		JP 2008-220988 A	25/09/2008
		JP 2008-296034 A	11/12/2008
		JP 2011-045756 A	10/03/2011
		JP 2912023 B2	28/06/1999
		JP 2931102 B2	09/08/1999
		JP 3033848 B2	17/04/2000
		JP 3215434 B2	09/10/2001
		JP 3391466 B2	31/03/2003
		JP 4261070 B2	30/04/2009
		JP 4290894 B2	08/07/2009
		JP 4713613 B2	29/06/2011
		JP 4756179 B2	24/08/2011
		JP 4986006 B2	25/07/2012
		JP 9501328 A	10/02/1997
		KR 10-1998-0703800 A	05/12/1998
		US 5366443 A	22/11/1994
		US 5419767 A	30/05/1995
		US 5681282 A	28/10/1997
		US 5683366 A	04/11/1997
		US 5697281 A	16/12/1997
		US 5697536 A	16/12/1997
		US 5697882 A	16/12/1997
		US 5697909 A	16/12/1997
		US 5766153 A	16/06/1998
		US 5810764 A	22/09/1998
		US 5843019 A	01/12/1998
		US 5860951 A	19/01/1999
		US 5871469 A	16/02/1999
		US 5873855 A	23/02/1999
		US 5888198 A	30/03/1999
		US 5891095 A	06/04/1999
		US 5902272 A	11/05/1999
		US 5925663 A	20/07/1999
		US 5941722 A	24/08/1999
		US 6024733 A	15/02/2000
		US 6032674 A	07/03/2000

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 6045532 A	04/04/2000
		US 6053172 A	25/04/2000
		US 6063079 A	16/05/2000
		US 6066134 A	23/05/2000
		US 6080776 A	27/06/2000
		US 6086585 A	11/07/2000
		US 6102046 A	15/08/2000
		US 6105581 A	22/08/2000
		US 6109268 A	29/08/2000
		US 6113597 A	05/09/2000
		US 6117109 A	12/09/2000
		US 6142992 A	07/11/2000
		US 6149620 A	21/11/2000
		US 6159194 A	12/12/2000
		US 6159208 A	12/12/2000
		US 6179824 B1	30/01/2001
		US 6179836 B1	30/01/2001
		US 6183469 B1	06/02/2001
		US 6190381 B1	20/02/2001
		US 6203542 B1	20/03/2001
		US 6210402 B1	03/04/2001
		US 6224592 B1	01/05/2001
		US 6228078 B1	08/05/2001
		US 6228082 B1	08/05/2001
		US 6235020 B1	22/05/2001
		US 6235765 B1	22/05/2001
		US 6238391 B1	29/05/2001
		US 6254600 B1	03/07/2001
		US 6264650 B1	24/07/2001
		US 6264651 B1	24/07/2001
		US 6264652 B1	24/07/2001
		US 6277112 B1	21/08/2001
		US 6283961 B1	04/09/2001
		US 6296636 B1	02/10/2001
		US 6296638 B1	02/10/2001
		US 6309387 B1	30/10/2001
		US 6312408 B1	06/11/2001
		US 6322549 B1	27/11/2001
		US 6355032 B1	12/03/2002
		US 6363937 B1	02/04/2002
		US 6379351 B1	30/04/2002
		US 6391025 B1	21/05/2002
		US 6416507 B1	09/07/2002
		US 6416508 B1	09/07/2002
		US 6432103 B1	13/08/2002
		US 6461350 B1	08/10/2002
		US 6461354 B1	08/10/2002
		US 6464695 B2	15/10/2002
		US 6468270 B1	22/10/2002
		US 6468274 B1	22/10/2002

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 6482201 B1	19/11/2002
		US 6500173 B2	31/12/2002
		US 6540741 B1	01/04/2003
		US 6544261 B2	08/04/2003
		US 6557559 B1	06/05/2003
		US 6575968 B1	10/06/2003
		US 6582423 B1	24/06/2003
		US 6589237 B2	08/07/2003
		US 6595990 B1	22/07/2003
		US 6602248 B1	05/08/2003
		US 6620155 B2	16/09/2003
		US 6623454 B1	23/09/2003
		US 6632193 B1	14/10/2003
		US 6632220 B1	14/10/2003
		US 6659106 B1	09/12/2003
		US 6712811 B2	30/03/2004
		US 6719754 B2	13/04/2004
		US 6726684 B1	27/04/2004
		US 6746447 B2	08/06/2004
		US 6749604 B1	15/06/2004
		US 6763836 B2	20/07/2004
		US 6770071 B2	03/08/2004
		US 6772012 B2	03/08/2004
		US 6773431 B2	10/08/2004
		US 6805130 B2	19/10/2004
		US 6832996 B2	21/12/2004
		US 6837887 B2	04/01/2005
		US 6837888 B2	04/01/2005
		US 6855143 B2	15/02/2005
		US 6856511 B1	15/02/2005
		US 6896672 B1	24/05/2005
		US 6896674 B1	24/05/2005
		US 6915806 B2	12/07/2005
		US 6929640 B1	16/08/2005
		US 6949096 B2	27/09/2005
		US 6960204 B2	01/11/2005
EP 1033107 A1	06/09/2000	EP 1033107 B1	16/06/2004
		JP 2000-279528 A	10/10/2000
		JP 4156169 B2	24/09/2008
		US 6203507 B1	20/03/2001
US 2005-0055019 A1	10/03/2005	US 7104989 B2	12/09/2006
EP 0908156 B1	12/11/2003	AU 1999-13720 A1	24/05/1999
		AU 1999-14526 A1	07/06/1999
		AU 1999-60247 A1	27/03/2000
		AU 1999-62419 A1	27/03/2000
		EP 0777445 B1	02/06/1999
		EP 0777445 B2	02/01/2004

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.  
**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		EP 0850024 A1	30/07/2003
		EP 0850024 B1	29/10/2003
		EP 0851743 A1	07/04/2004
		EP 0851743 B1	24/11/2010
		EP 0883379 A1	16/04/2003
		EP 0891158 A1	24/03/2004
		EP 0891158 B1	22/09/2004
		EP 0908156 A1	14/04/1999
		EP 0957988 A2	26/05/2004
		EP 0957988 B1	15/12/2004
		EP 1109504 A2	27/06/2001
		EP 1109504 B1	13/05/2009
		EP 1109505 A1	27/06/2001
		EP 1344497 A1	17/09/2003
		EP 1366725 A1	03/12/2003
		EP 1366725 B1	24/01/2007
		EP 1598025 A2	23/11/2005
		EP 1598025 A3	02/08/2006
		HK 1002098 A1	24/03/2000
		JP 10-503959 A	14/04/1998
		JP 11-511988 A	19/10/1999
		JP 11-511991 A	19/10/1999
		JP 11-511992 A	19/10/1999
		JP 2000-500033 A	11/01/2000
		JP 2000-506415 A	30/05/2000
		JP 2000-507844 A	27/06/2000
		JP 2001-231790 A	28/08/2001
		JP 2002-524129 A	06/08/2002
		JP 2002-524130 A	06/08/2002
		JP 2007-125414 A	24/05/2007
		JP 3009735 B2	14/02/2000
		JP 3560917 B2	02/09/2004
		JP 4001210 B2	31/10/2007
		JP 4191897 B2	03/12/2008
		KR 10-0243503 B1	02/03/2000
		KR 10-0243744 B1	02/03/2000
		KR 10-1997-0706864 A	01/12/1997
		KR 10-1997-0706866 A	01/12/1997
		KR 10-1999-0082587 A	25/11/1999
		KR 10-1999-0087805 A	27/12/1999
		US 2001-0001819 A1	24/05/2001
		US 2002-0026185 A1	28/02/2002
		US 2002-0035363 A1	21/03/2002
		US 2004-0181217 A1	16/09/2004
		US 2004-0260282 A1	23/12/2004
		US 2005-0033279 A1	10/02/2005
		US 2005-0101950 A1	12/05/2005
		US 2005-0203503 A1	15/09/2005
		US 2006-0247616 A1	02/11/2006
		US 2008-0154259 A1	26/06/2008

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 2008-0167649 A1	10/07/2008
		US 5458597 A	17/10/1995
		US 5472441 A	05/12/1995
		US 5507743 A	16/04/1996
		US 5536267 A	16/07/1996
		US 5599345 A	04/02/1997
		US 5599346 A	04/02/1997
		US 5672173 A	30/09/1997
		US 5672174 A	30/09/1997
		US 5683384 A	04/11/1997
		US 5728143 A	17/03/1998
		US 5735847 A	07/04/1998
		US 5782827 A	21/07/1998
		US 5800484 A	01/09/1998
		US 5810804 A	22/09/1998
		US 5863290 A	26/01/1999
		US 5913855 A	22/06/1999
		US 5925042 A	20/07/1999
		US 5928229 A	27/07/1999
		US 5935123 A	10/08/1999
		US 5951547 A	14/09/1999
		US 5980517 A	09/11/1999
		US 6053937 A	25/04/2000
		US 6059780 A	09/05/2000
		US 6071280 A	06/06/2000
		US 6080150 A	27/06/2000
		US 6090105 A	18/07/2000
		US 6132425 A	17/10/2000
		US 6235023 B1	22/05/2001
		US 6330478 B1	11/12/2001
		US 6471698 B1	29/10/2002
		US 6500175 B1	31/12/2002
		US 6551311 B2	22/04/2003
		US 6569159 B1	27/05/2003
		US 6605085 B1	12/08/2003
		US 6632221 B1	14/10/2003
		US 6632222 B1	14/10/2003
		US 6641580 B1	04/11/2003
		US 6652516 B1	25/11/2003
		US 6660002 B1	09/12/2003
		US 6663624 B2	16/12/2003
		US 6689127 B1	10/02/2004
		US 6958062 B1	25/10/2005
		US 7150744 B2	19/12/2006
		WO 00-13602 A2	16/03/2000
		WO 00-13602 A3	20/07/2000
		WO 00-13603 A1	16/03/2000
		WO 95-13113 A1	18/05/1995
		WO 96-04860 A1	22/02/1996
		WO 97-06739 A2	27/02/1997

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2013/053977**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		WO 97-06740 A2	27/02/1997
		WO 97-06855 A2	27/02/1997
		WO 97-06857 A2	27/02/1997
		WO 97-29702 A1	21/08/1997
		WO 97-33524 A1	18/09/1997
		WO 97-36548 A1	09/10/1997
		WO 99-22657 A1	14/05/1999
		WO 99-25260 A1	27/05/1999
US 2012-0108938 A1	03/05/2012	EP 2068738 A2	17/06/2009
		US 2009-254078 A1	08/10/2009
		US 2009-287210 A1	19/11/2009
		US 2010-094279 A1	15/04/2010
		WO 2008-045877 A2	17/04/2008
		WO 2008-045877 A3	09/04/2009
		WO 2008-045929 A2	17/04/2008
		WO 2008-045929 A3	14/08/2008
		WO 2008-045936 A2	17/04/2008
		WO 2008-045936 A3	09/10/2008
		WO 2008-045938 A2	17/04/2008
		WO 2008-045938 A3	26/06/2008