



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification <sup>6</sup> :</b>  <b>A61B 5/029</b>	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 99/02086</b>  <b>(43) International Publication Date:</b> 21 January 1999 (21.01.99)
<b>(21) International Application Number:</b> PCT/GB98/01972  <b>(22) International Filing Date:</b> 3 July 1998 (03.07.98)  <b>(30) Priority Data:</b> 9714550.2                      10 July 1997 (10.07.97)                      GB  <b>(71) Applicant:</b> MONITORING TECHNOLOGY LIMITED [GB/GB]; The Finance Dept., Medical School Building, Guy's Hospital, London SE1 9RT (GB).  <b>(72) Inventors; and</b> <b>(75) Inventors/Applicants (for US only):</b> BAND, David, Marston [GB/GB]; 88 Ditton Road, Surbiton, Surrey KT6 6RH (GB). LINTON, Nicholas, William, Fox [GB/GB]; 83 Deodar Road, Putney, London SW15 2NU (GB). LINTON, Robert, Anthony, Fox [GB/GB]; 83 Deodar Road, Putney, London SW15 2NU (GB). O'BRIEN, Terence, Kevin [GB/GB]; 5 Headley Gardens, Great Shelford, Cambridge CB2 5JZ (GB).  <b>(74) Agent:</b> ALLARD, Susan, Joyce; Boulton Wade Tennant, 27 Fumival Street, London EC4A 1PQ (GB).		<b>(81) Designated States:</b> AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, GW, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).  <b>Published</b> <i>With international search report.</i>
<b>(54) Title:</b> IMPROVED METHOD AND APPARATUS FOR THE MEASUREMENT OF CARDIAC OUTPUT		
<b>(57) Abstract</b>  A method for the measurement of cardiac output in a patient in which the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time is subjected to various transformations and corrections, including a Fourier analysis in order to obtain the modulus of the first harmonic. The nominal stroke volume is then determined from the first harmonic and data relating to the arterial blood pressure and heart rate. The nominal cardiac output is then obtained from the nominal stroke volume.		

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

<b>AL</b>	Albania	<b>ES</b>	Spain	<b>LS</b>	Lesotho	<b>SI</b>	Slovenia
<b>AM</b>	Armenia	<b>FI</b>	Finland	<b>LT</b>	Lithuania	<b>SK</b>	Slovakia
<b>AT</b>	Austria	<b>FR</b>	France	<b>LU</b>	Luxembourg	<b>SN</b>	Senegal
<b>AU</b>	Australia	<b>GA</b>	Gabon	<b>LV</b>	Latvia	<b>SZ</b>	Swaziland
<b>AZ</b>	Azerbaijan	<b>GB</b>	United Kingdom	<b>MC</b>	Monaco	<b>TD</b>	Chad
<b>BA</b>	Bosnia and Herzegovina	<b>GE</b>	Georgia	<b>MD</b>	Republic of Moldova	<b>TG</b>	Togo
<b>BB</b>	Barbados	<b>GH</b>	Ghana	<b>MG</b>	Madagascar	<b>TJ</b>	Tajikistan
<b>BE</b>	Belgium	<b>GN</b>	Guinea	<b>MK</b>	The former Yugoslav Republic of Macedonia	<b>TM</b>	Turkmenistan
<b>BF</b>	Burkina Faso	<b>GR</b>	Greece	<b>ML</b>	Mali	<b>TR</b>	Turkey
<b>BG</b>	Bulgaria	<b>HU</b>	Hungary	<b>MN</b>	Mongolia	<b>TT</b>	Trinidad and Tobago
<b>BJ</b>	Benin	<b>IE</b>	Ireland	<b>MR</b>	Mauritania	<b>UA</b>	Ukraine
<b>BR</b>	Brazil	<b>IL</b>	Israel	<b>MW</b>	Malawi	<b>UG</b>	Uganda
<b>BY</b>	Belarus	<b>IS</b>	Iceland	<b>MX</b>	Mexico	<b>US</b>	United States of America
<b>CA</b>	Canada	<b>IT</b>	Italy	<b>NE</b>	Niger	<b>UZ</b>	Uzbekistan
<b>CF</b>	Central African Republic	<b>JP</b>	Japan	<b>NL</b>	Netherlands	<b>VN</b>	Viet Nam
<b>CG</b>	Congo	<b>KE</b>	Kenya	<b>NO</b>	Norway	<b>YU</b>	Yugoslavia
<b>CH</b>	Switzerland	<b>KG</b>	Kyrgyzstan	<b>NZ</b>	New Zealand	<b>ZW</b>	Zimbabwe
<b>CI</b>	Côte d'Ivoire	<b>KP</b>	Democratic People's Republic of Korea	<b>PL</b>	Poland		
<b>CM</b>	Cameroon	<b>KR</b>	Republic of Korea	<b>PT</b>	Portugal		
<b>CN</b>	China	<b>KZ</b>	Kazakstan	<b>RO</b>	Romania		
<b>CU</b>	Cuba	<b>LC</b>	Saint Lucia	<b>RU</b>	Russian Federation		
<b>CZ</b>	Czech Republic	<b>LI</b>	Liechtenstein	<b>SD</b>	Sudan		
<b>DE</b>	Germany	<b>LK</b>	Sri Lanka	<b>SE</b>	Sweden		
<b>DK</b>	Denmark	<b>LR</b>	Liberia	<b>SG</b>	Singapore		
<b>EE</b>	Estonia						

- 1 -

IMPROVED METHOD AND APPARATUS FOR THE MEASUREMENT OF  
CARDIAC OUTPUT

5       The present invention relates to an improved  
method and apparatus for the measurement of cardiac  
output and in particular to an improved method and  
apparatus which has a rapid rate of response and good  
noise rejection.

10       Cardiac output is an important haemodynamic  
variable which is defined as the volume of blood that  
is pumped by the heart per minute.

15       Blood pressure was first measured in 1750. Since  
at least 1904 (Erlanger and Hooker, Bull. John Hopkins  
Hosp. 15:179) it has been suggested that the arterial  
pulse pressure could be regarded as a rough index to  
the stroke volume of the heart and, in combination  
with the heart rate, could provide the cardiac output.  
This approach was found to be simplistic and has been  
surpassed by other methods.

20       Kouchoukos et al. (Estimation of stroke volume in  
the dog by a pulse contour method, Circ. Res., vol.  
26, 5:611-23, 1970) used a method that uses the  
systolic area to determine stroke volume. The  
systolic area is the area between the blood pressure  
and end diastolic pressure during systole. Since 1970  
25       there have been many modifications to the systolic  
area technique of pulse contour analysis. For  
example, correction factors such as age, height and  
weight have been added as well as factors to allow for  
30       the changing compliance of the arteries and  
reflections of the pressure wave from the peripheral  
circulation.

35       Even after the correction factors were introduced  
the results were still not reliable. Currently, pulse  
contour analysis is not routinely used by clinicians  
despite the importance of cardiac output. One of the

- 2 -

major shortcomings of these methods is their reliance upon measuring morphological features of the blood pressure waveform. In particular, the position of the dicrotic notch, which signifies the closure of the aortic valve, must be found in order to measure the systolic area. During surgery and intensive care the dicrotic notch may not be detectable or it may be mimicked by other minor waves superimposed upon the pressure waveform.

US Patent No. 5400793 describes another method for determining the stroke volume from aortic blood pressure in a subject. The method uses a simulation model of the aorta as a transmission line, including a pressure volume relationship for the aorta that is known in the art and supplemented with a Windkessel compliance.

In essence, the pressure recorded in the aorta is used to determine the characteristic impedance of the transmission line model. The simulation is then performed and the parameters of the Windkessel are adapted until the flow calculated in the model is consistent with the pressure in the aorta. The flow is then integrated over the period of systole. Ideally, this method requires a high fidelity transducer positioned in the aorta. Although a method of correcting a pressure measurement in a peripheral artery is mentioned, this method cannot be used with the poor frequency response given by most pressure transducers now routinely in clinical use: in the presence of noise an "anti-resonance filter" cannot recover the information that is lost by the poor quality of these transducers.

None of the aforementioned methods of measuring cardiac output explicitly account for the frequency response of the transducers now in routine clinical use. Lambert et al. (Pressure measurement in

- 3 -

diagnostic and therapeutic cardiac catheterisation,  
eds. Pepine et al., Williams and Wilkins, Baltimore,  
283-97) found that with added extension tubes, the  
response of some measuring systems is accurate (to  
5 within 5%) only for frequencies less than 2 Hz.

Finally, Hamilton (The physiology of cardiac  
output, circulation 8: 527, 1953) suggested that  
cardiac output could be derived from a patient's blood  
pressure pulse height following calibration by another  
10 device.

It is now accepted in the art that all existing  
pulse contour methods require calibration for improved  
accuracy. The present invention is also intended to  
be used with a calibration device, for example a  
15 thermodilution or indicator dilution method. An  
indicator dilution method is described, for example,  
in W093/09427. The method as described in W093/09427  
is highly repeatable and only one single point  
calibration is required to give the cardiac output.  
20 It will be understood, however, that the method of the  
present invention may be used without calibration in  
order to show trends in or directions of change of the  
cardiac output of a patient.

In our co-pending application W097/24982 we have  
25 described an improved method for measuring cardiac  
output using pulse contour analysis. A non-linear  
transformation is used to correct for the changing  
characteristics of the arterial system with pressure  
and autocorrelation is then used to derive the cardiac  
30 output. Although this technique is an improvement  
over the prior art methods discussed above, there is  
still a need for a further improved method.

The method described in W097/24982 was an  
empirical finding and has given good results in  
35 patients undergoing cardiac surgery. The present  
invention gives results that are numerically similar

- 4 -

under normal conditions. However, the frequency response of the pressure measurement system is explicitly accounted for. It is also based upon a stronger theoretical framework which will allow  
5 modification to the method to be assessed more easily.

Accordingly, in a first aspect the present invention provides a method for the measurement of cardiac output in a patient, which method comprises the steps of:-

- 10 (i) recording and storing the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time;
- (ii) 15 subjecting the data obtained in step (i) to Fourier analysis in order to obtain the modulus of the first harmonic;
- (iii) 20 determining the nominal stroke volume from the modulus of the first harmonic obtained in step (ii) and data relating to the arterial blood pressure and the heart rate; and
- (iv) obtaining the nominal cardiac output and/or the systemic vascular resistance from data obtained in step (iii).

25 Step (ii) above is preferably achieved by identifying a period of the waveform obtained in step (i) that contains at least one beat.

Arteries generally have non-linear properties. The above method assumes that the compliance does not  
30 vary significantly within the range of blood pressures that occur during a single beat. The compliance at the corresponding mean arterial pressure is preferably used. Alternatively, the blood pressure may be transformed during an initial step which linearises  
35 the blood pressure with respect to the arterial compliance.

- 5 -

In a second aspect the present invention provides a method for the measurement of cardiac output in a patient, which method comprises the steps of:-

- 5 (a) recording and storing the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time;
- (b) 10 subjecting the waveform obtained in step (a) to a non-linear transformation that corrects for the variation of the characteristics of the arterial system with pressure;
- (c) 15 subjecting the data obtained in step (b) to Fourier analysis in order to obtain the modulus of the first harmonic;
- (d) determining the nominal stroke volume from the modulus of the first harmonic obtained in step (c) and data relating to the heart rate and optionally the arterial blood pressure; and
- 20 (e) obtaining the nominal cardiac output and/or the systemic vascular resistance from data obtained in step (d).

25 In step (b) the non-linear transformation preferably linearises the pressure with respect to the arterial compliance.

Step (c) is preferably achieved by identifying each beat of the waveform obtained in step (b) that contains at least one beat.

30 In both aspects of the present invention the heart rate may be determined, for example, using an autocorrelation method as described in W097/24982, Fourier analysis, filtering techniques on the pressure waveform and/or edge detection or any other suitable  
35 technique. The same data is preferably used to

- 6 -

determine the nominal stroke volume and the heart rate.

In both aspects of the present invention the nominal cardiac output is preferably obtained by multiplying the nominal stroke volume by the heart rate. If this is done beat-by-beat, then stroke volume and heart rate data are obtained for a number of beats. It will be appreciated that this data may be used in a number of ways to derive the nominal cardiac output and the systemic vascular resistance.

In carrying out either of the methods of the present invention the patient's arterial blood pressure is monitored continuously by conventional means from, for example, the aorta, the brachial artery or radial artery. Accordingly, the patient's arterial blood pressure may be monitored using an arterial catheter with a transducer system or a non-invasive method. The output from the pressure measuring device preferably provides the blood pressure for at least one beat. It is preferably an analogue or digital signal with a sample rate great enough to accurately reproduce the first harmonic of the waveform, preferably for a period of up to four seconds. The blood pressure data is generally analysed on a beat-by-beat basis.

Fourier analysis may be used to determine the harmonic components of a complex wave and is described in detail in many mathematical and physics textbooks. Fourier analysis enables a periodic function to be represented by a Fourier series of trigonometric functions, thus:

$$f(t) = a_0/2 + a_1 \cos(2\pi t/T) + a_2 \cos(4\pi t/T) + \dots \\ + b_1 \sin(2\pi t/T) + b_2 \sin(4\pi t/T) + \dots$$

where  $a_0$ ,  $a_1$ ,  $b_1$  and  $b_2$  are constants,  $t$  is the time and  $T$  is the period.

The use of Fourier analysis in the present invention assumes that the signal is periodic and that



- 7 -

the arterial system is linear. In reality, the heart may beat irregularly and there are non-linearities, for example the arteries become stiffer as arterial pressure increases. However, the errors that this introduces have been examined by other workers who found them to be small (E.O. Attinger, A. Anné and D.A. MacDonald, "Use of Fourier series for the Analysis of Biological Systems", Biophysical Journal, Volume 6, 1966).

It is possible to reduce the errors introduced by the reduction of arterial compliance with increases in arterial pressure. Accordingly, in the second aspect of the present invention a non-linear transformation of the blood pressure waveform obtained in step (a) is carried out to correct for the variation of the characteristics of the arterial system with pressure. The corrected waveform is then subjected to Fourier analysis.

As mentioned above, the pressure waveform obtained in step (i) of the first method is transformed, preferably via a 'look up' table which represents the pressure-volume relationship of the arterial system. The basic approximation to a look up table is known in the art. A series of pressure-volume curves is described in Remington et al., "Volume elasticity characteristics of the human aorta and prediction of the stroke volume from the pressure pulse", Am. J. Physiol 153: 298-308, 1948.

The nominal cardiac output may be obtained using the nominal stroke volume and heart rate. The nominal cardiac output may found, for example, by multiplying the nominal stroke volume by the heart rate. If more than one beat is used to calculate the nominal cardiac output then it may be calculated as the sum of the stroke volumes divided by the sum of the durations of each beat. It will be understood that the nominal

- 8 -

stroke volume and the nominal cardiac output are uncalibrated and may be converted into calibrated data if desired. This is performed by multiplying the nominal stroke volume by a calibration factor to give  
5 the true stroke volume, as found by another method. The cardiac output may then be calculated from the true stroke volume and heart rate. The nominal systemic vascular resistance (SVR) may be calculated by dividing the mean arterial pressure by the nominal  
10 cardiac output. A true value may also be obtained from the true cardiac output.

The present invention gives a close to real-time analysis of rapidly changing events. For example, the method of the present invention may be used to monitor  
15 changes in the cardiac output following the administration of fluids, or to set a pacemaker to an optimal rate, or to determine when administration of a vasoactive drug may be required.

In carrying out the second method of the present  
20 invention steps (a), (d) and (e) correspond generally to steps (i), (iii) and (iv) of the first method as discussed herein.

The methods of the present invention may be applied to periods of blood pressure data greater than  
25 one heart beat or to single heart beats if they can be identified separately, i.e. a beat-by-beat analysis. Methods for identifying single heart beats are known in the art.

Apparatus for carrying out the present invention  
30 may comprise any suitably programmed computer such as an IBM compatible computer or a Macintosh computer which is able to acquire data from the blood pressure measurement device or monitor. It may also be integrated with software and hardware for performing  
35 other tasks. For example, the device may be capable of carrying out the present invention as well as the

- 9 -

method used for calibration or other monitoring tasks.  
The computer programme running on the computer may  
then either display the results on a visual display  
unit or can output this information to some other  
5 device.

Accordingly, in a further aspect the present  
invention provides an apparatus for the measurement of  
cardiac output in a patient, which comprises:-

- 10 (1) means for recording and storing the  
arterial blood pressure waveform of a  
patient from a blood pressure monitoring  
device over a period of time;
- (2) means for Fourier analysis of the arterial  
blood pressure waveform to obtain the  
15 modulus of the first harmonic;
- (3) means for deriving the nominal stroke  
volume from the modulus of the first  
harmonic and data relating to the arterial  
blood pressure and the heart rate; and
- 20 (4) means for calculating the nominal cardiac  
output and/or the systemic vascular  
resistance.

Alternatively, in a still further aspect the  
present invention provides an apparatus for the  
25 measurement of cardiac output in a patient, which  
method comprises the steps of:-

- (A) means for recording and storing the  
arterial blood pressure waveform of a  
patient from a blood pressure monitoring  
30 device over a period of time;
- (B) means for transforming the arterial blood  
pressure waveform to correct for the  
variation of the characteristics of the  
arterial system with pressure;

- 10 -

(C) means for the Fourier analysis of the transformed data to obtain the modulus of the first harmonic of the waveform;

5 (D) means for determining the nominal stroke volume from the modulus of the first harmonic and data relating to the heart rate and optionally the arterial blood pressure; and

10 (E) means for calculating the nominal cardiac output and/or the systemic vascular resistance.

The present invention will be further described, by way of example, with reference to the accompanying drawings in which:

15 Figure 1 is a diagram of the physical processes which relate the ejection of blood from the left ventricle to the blood pressure reading from the measurement device;

20 Figure 2 shows a typical example of the aortic flow for one beat; and

Figure 3 illustrates the use of the method of the present invention in determining cardiac output in a patient undergoing heart surgery.

25 The current invention is based upon a model that relates the first harmonic of the measured blood pressure to the first harmonic of the flow in the aorta. A relationship between the first harmonic of the flow in the aorta and the mean flow in the aorta is assumed. The stroke volume for each beat can then  
30 be calculated by multiplying the mean flow by the duration of each beat. The cardiac output can be calculated over any required period by summing the stroke volumes over that period and dividing by the duration of the period. A period of 15 seconds is  
35 typical for this purpose.

- 11 -

Figure 1 describes the physical processes which relate the ejection of blood from the left ventricle to the blood pressure reading from the measurement device. These are described in four stages. Stage 1 - the ventricle creates a flow into the aorta, this rises to a peak during systole and is approximately zero during diastole (assuming a competent aortic valve). Stage 2 - the flow from the ventricle creates a pressure in the ascending aorta, the pressure-flow relationship is the ascending aorta input impedance. Stage 3 - the pressure in the aorta is transmitted to the peripheral arteries. Stage 4 - the peripheral artery pressure (e.g. radial artery) is measured, however, the measurement process introduces distortion. The current invention uses approximations to each stage in order to relate the first harmonic of the blood pressure to the stroke volume ejected by the heart. These approximations are described below.

Stage 1 Figure 2 shows a typical example of the aortic flow for one beat. During systole the flow increases after the left ventricle starts to contract. The flow rises to a peak and then falls. The flow then reverses for a short period which causes the aortic valve to close. This prevents blood from returning to the relaxed ventricle. The basic morphology of the flow waveform is restricted by these physical processes. Thus there is a predictable relationship between the first harmonic of the aortic flow and mean aortic flow. As the heart rate increases, the duration of systole occupies a greater proportion of the cardiac cycle. This results in the ratio of the mean flow to the first harmonic of the flow falling as the heart rate rises. Thus, the first harmonic can be related to the mean flow.

Stage 2 The aortic input impedance relates the flow to the pressure, in the frequency domain. The

- 12 -

present invention uses an approximation for the aortic impedance in the range of frequencies that may occur for the first harmonic of the pressure/flow waveform i.e. the heart rate. This is 30-150 beats per minute  
5 or 0.5-2.5 Hz. The approximation also allows for changes in impedance that occur as the systemic vascular resistance (SVR) and arterial pressure change.

The relationship between aortic input impedance  
10 and frequency has been studied *in vivo* by many other workers. In particular, O'Rourke and Aviolo found good agreement between measurements made in a man and a 128 segment numerical model (M.F. O'Rourke and A.P. Aviolo, 'Pulsatile flow and pressure in human systemic  
15 arteries: studies in man and in a multibranched model of the human systemic arterial tree', Circulation Research, vol. 43, no. 3, March 1980). This model is well approximated by impedance =  $1 \div \text{frequency}$  for the range 0.5-2.5 Hz.

20 Since the work of Aviolo and O'Rourke others have developed the model to account for changes in SVR. As the SVR increases the impedance at the frequency of the first harmonic (for normal heart rates) also increases. In addition to this the blood pressure  
25 also affects aortic input impedance; at high blood pressures the arteries are less compliant.

As well as the effects described above, arterial dilatation can also affect the aortic input impedance. This is due to a reduction in wave reflection from the  
30 peripheral circulation. In order to account for the resulting change in impedance an augmentation index may be calculated. This gives an indication of the magnitude of wave reflection and a method for doing this is reviewed in McDonald's Blood Flow in Arteries,  
35 Nichols and O'Rourke, London, Arnold 1998.

- 13 -

In order to approximate the aortic impedance (at the frequency of the first harmonic of the blood pressure waveform) a relationship is used that depends upon frequency, SVR, and mean blood pressure. The approximation may be further improved by calculation of an augmentation index.

Stage 3 As the pressure waveform is transmitted from the aorta to the peripheral arteries it is distorted. This occurs because of arterial branching, changes in the characteristic impedance of the arteries, and reflection from the periphery caused by an impedance mismatch between the arteries and the arterioles. However, reflection is more predictable at low frequencies.

Stage 4 The performance of catheter-manometer systems (which are used to measure blood pressure clinically) is described in McDonald's Blood Flow in Arteries, Nichols & O'Rourke, London, Arnold, 1998. The present invention is intended for use at heart rates of 0.5-2.5 Hz. It is important that the measurement system has a frequency response that is sufficient to reproduce the fundamental frequency of the blood pressure waveform i.e. the frequency of the heart rate. If the measurement system is only capable of reproducing frequencies up to less than 2.5 Hz then the system may still be used if the heart rate remains below the maximum frequency that can be reproduced. The formula used to relate the blood pressure data to the stroke volume is required to account for the relationships described by stages 1 & 2. No explicit correction is usually required for stages 3 and 4 because their physical effects upon frequencies less than 2.5 Hz are negligible.

- 14 -

An example of an equation which may be used is:

$$\text{nominal mean flow} = \frac{\text{modulus of first harmonic of blood pressure waveform}}{e^{+0.0092 \times \text{MAP}}}$$

$$\text{nominal stroke volume} = \frac{\text{modulus of first harmonic of blood pressure waveform}}{e^{+0.0092 \times \text{MAP}} \times \text{HR}}$$

where e is the base of natural logarithms, MAP is the mean arterial blood pressure and HR is the heart rate.

Thus, the nominal cardiac output may be calculated directly from the modulus of the first harmonic of the blood pressure waveform and the blood pressure, and optionally the heart rate. For example:

$$\text{nominal cardiac output} = \frac{\text{modulus of first harmonic of blood pressure waveform}}{e^{+0.0092 \times \text{MAP}}}$$

Referring now to Figure 3, a beat-by-beat analysis of the patient's heart rhythm during heart surgery is charted as the trace labelled HR. The mean arterial blood pressure is also charted as the trace MAP. The heart was in nodal rhythm - a condition in which abnormal electrical activity causes the heart to function inefficiently. About twenty-seven seconds into the trace the heart changed to sinus rhythm (normal). The immediate increase in the performance of the heart is indicated by the change in mean arterial pressure over the next four beats. The derived cardiac output also shows an immediate increase confirming that the cause of the increase in pressure was due to better cardiac performance (rather than an increase in peripheral resistance).



**CLAIMS:**

1. A method for the measurement of cardiac output in a patient, which method comprises the steps of:-
- 5 (i) recording and storing the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time;
- 10 (ii) subjecting the data obtained in step (i) to Fourier analysis in order to obtain the modulus of the first harmonic;
- (iii) determining the nominal stroke volume from the modulus of the first harmonic obtained in step (ii) and data relating to the
- 15 arterial blood pressure and the heart rate; and
- (iv) obtaining the nominal cardiac output and/or the systemic vascular resistance
- 20 from data obtained in step (iii).
2. A method as claimed in claim 1 wherein the arterial blood pressure is plotted in step (i) for a period of up to ten seconds.
- 25 3. A method as claimed in claim 2 wherein the arterial blood pressure is plotted in step (i) for a period of up to four seconds.
- 30 4. A method as claimed in claim 1 wherein the arterial blood pressure is analysed on a beat-by-beat basis.
5. A method as claimed in any one of the preceding claims wherein the nominal stroke volume is
- 35 obtained from the following equation:

- 16 -

$$\text{nominal stroke volume} = \frac{\text{modulus of first harmonic of blood pressure waveform}}{e^{+0.0092 \times \text{MAP}} \times \text{HR}}$$

where e is the base of natural logarithms and MAP is the mean arterial blood pressure.

6. A method as claimed in any one of claims 1 to 5, wherein an augmentation index is included in the calculation of the nominal stroke volume in step (iii).

7. A method for the measurement of cardiac output in a patient, which method comprises the steps of:-

- (a) recording and storing the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time;
- (b) subjecting the waveform obtained in step (a) to a non-linear transformation that corrects for the variation of the characteristics of the arterial system with pressure;
- (c) subjecting the data obtained in step (b) to Fourier analysis in order to obtain the modulus of the first harmonic;
- (d) determining the nominal stroke volume from the modulus of the first harmonic obtained in step (c) and data relating to the heart rate and optionally the arterial blood pressure; and
- (e) obtaining the nominal cardiac output and/or the systemic vascular resistance from data obtained in step (d).

35

- 17 -

8. A method as claimed in claim 7 wherein the arterial blood pressure is plotted in step (a) for a period of up to ten seconds.

5 9. A method as claimed in claim 8 wherein the arterial blood pressure is plotted in step (a) for a period of up to four seconds.

10 10. A method as claimed in claim 7 wherein the arterial blood pressure is analysed on a beat-by-beat basis.

15 11. A method as claimed in any one of claims 7 to 10 wherein the transformation in step (b) is effected using a look up table, with the mean of the data then being found and subtracted.

20 12. A method as claimed in any one of claims 7 to 11 wherein the nominal stroke volume is obtained from the following equation:

$$\text{nominal stroke volume} = \frac{\text{modulus of first harmonic of blood pressure waveform}}{e^{+0.0092 \times \text{MAP}} \times \text{HR}}$$

25 13. A method as claimed in any one of the preceding claims wherein the nominal cardiac output is obtained by multiplying the nominal stroke volume by the heart rate.

30 14. A method as claimed in any one of claims 7 to 13 wherein an augmentation index is included in the calculation of the nominal stroke volume in step (iii).

35 15. An apparatus for the measurement of cardiac output in a patient, which comprises:-

- 18 -

- (1) means for recording and storing the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time;
- 5 (2) means for Fourier analysis of the arterial blood pressure waveform to obtain the modulus of the first harmonic;
- (3) means for deriving the nominal stroke volume from the modulus of the first harmonic and data relating to the arterial blood pressure and the heart rate; and
- 10 (4) means for calculating the nominal cardiac output and/or the systemic vascular resistance.

15

16. An apparatus for the measurement of cardiac output in a patient, which method comprises the steps of:-


- (A) means for recording and storing the arterial blood pressure waveform of a patient from a blood pressure monitoring device over a period of time;
- 20 (B) means for transforming the arterial blood pressure waveform to correct for the variation of the characteristics of the arterial system with pressure;
- 25 (C) means for the Fourier analysis of the transformed data to obtain the modulus of the first harmonic of the waveform;
- 30 (D) means for determining the nominal stroke volume from the modulus of the first harmonic and data relating to the heart rate and optionally the arterial blood pressure; and

- 19 -

- (E) means for calculating the nominal cardiac output and/or the systemic vascular resistance.

1/3

FIG. 1.

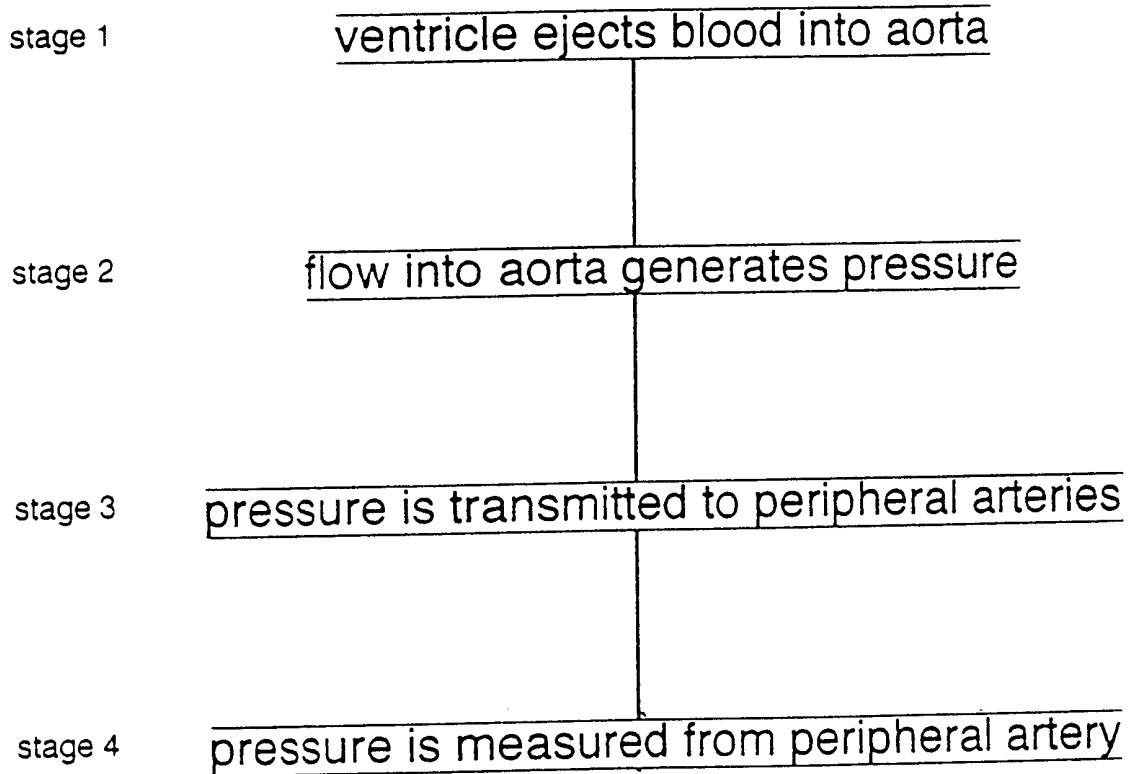

2/3


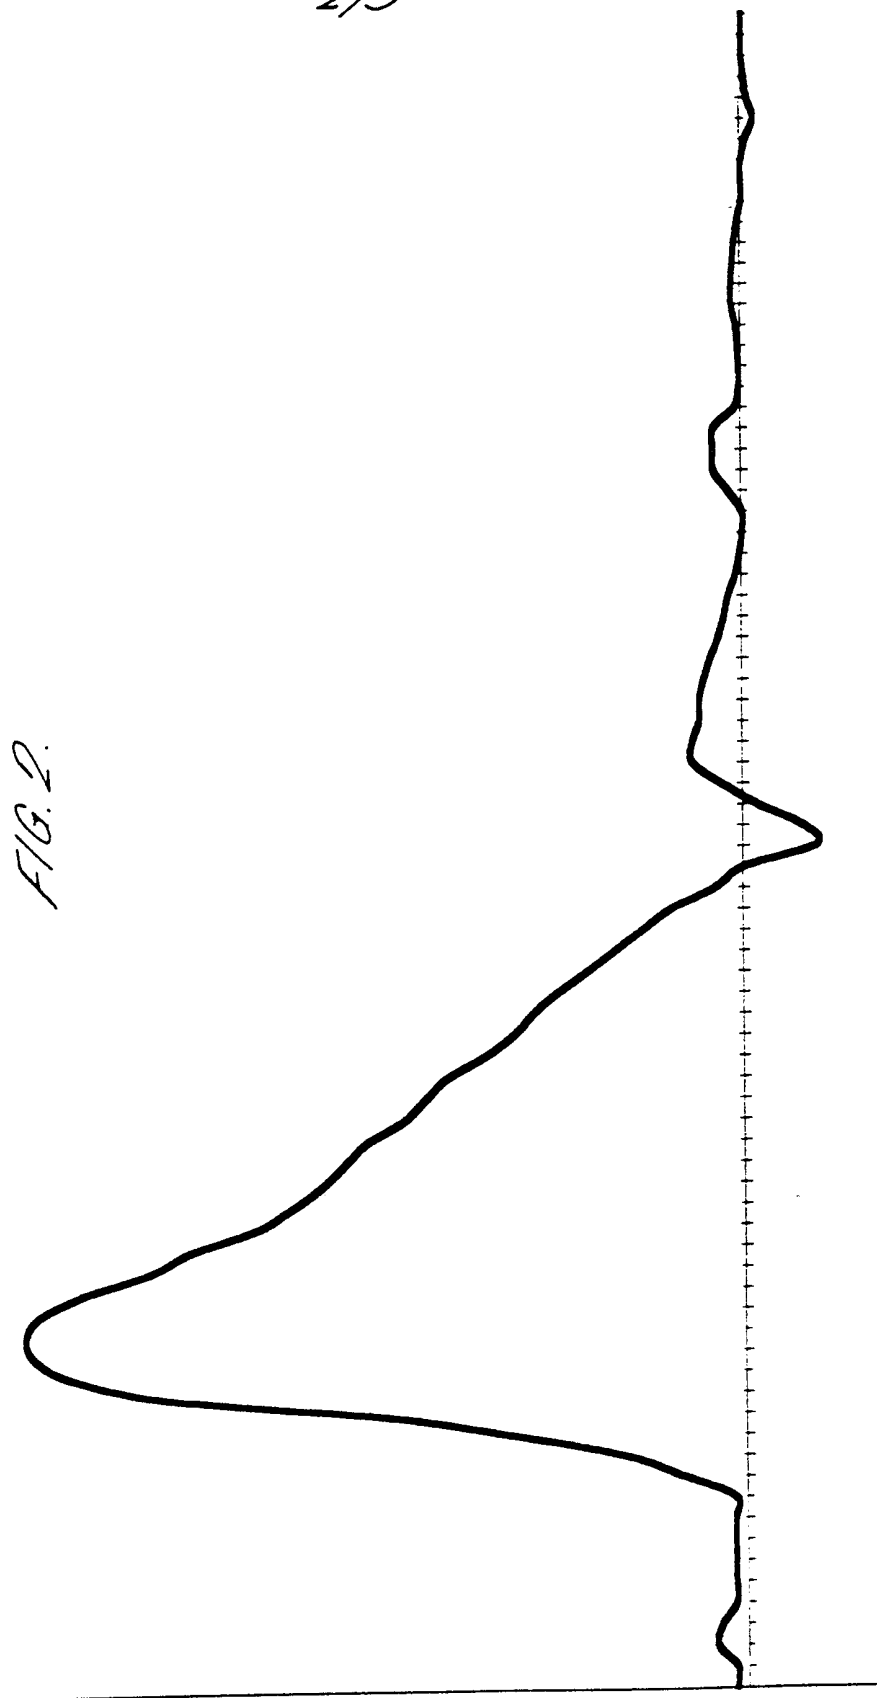


FIG. 3. BEAT-BY-BEAT ANALYSIS



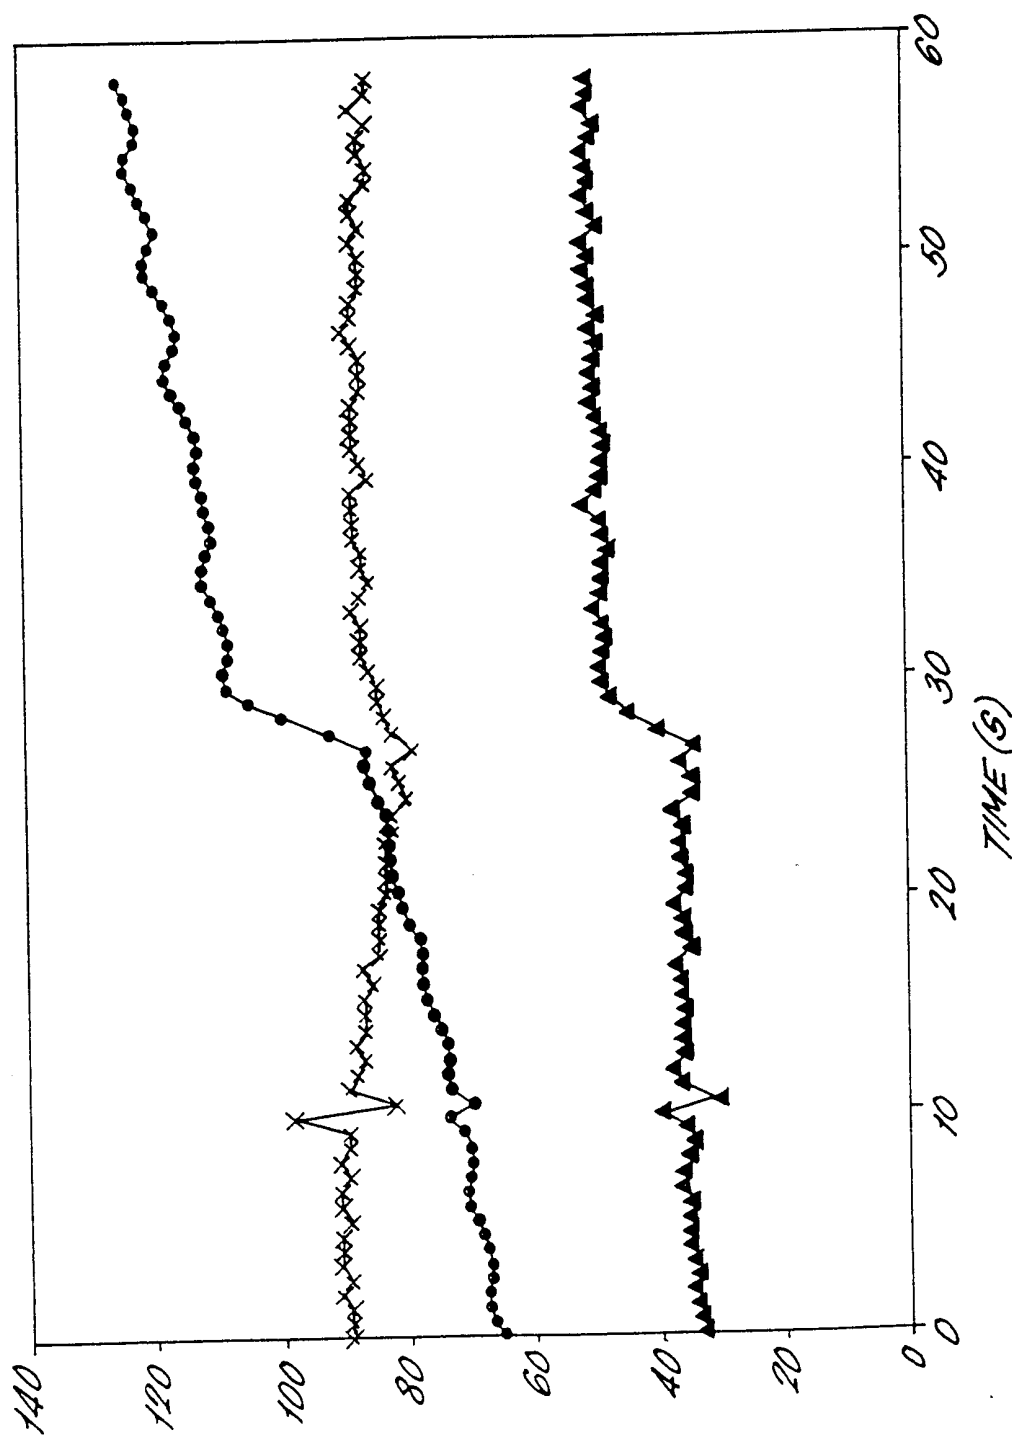

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/GB 98/01972

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61B5/029

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61B G06F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
P,A	WO 97 24982 A ( MONITORING TECHNOLOGY LIMITED ) 17 July 1997 cited in the application see the whole document ---	1-16
P,A	EP 0 818 175 A ( SEIKO EPSON CORPORATION ) 14 January 1998  see page 3, line 11 - page 4, line 14 see page 28, line 39 - page 29, line 20 ---	1-4, 7-11, 13-17
A	US 5 390 679 A ( J. F. MARTIN ) 21 February 1995 see column 1, line 8 - column 4, line 59 see column 5, line 5 - column 6, line 54 --- -/--	1,7,11, 15,16



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

° Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

21 October 1998

Date of mailing of the international search report

28/10/1998

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Geffen, N

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/GB 98/01972

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>WO 92 06633 A ( HYPERTENSION DIAGNOSTICS, INC. ) 30 April 1992  see page 2, line 30 - page 3, line 35  see page 4, line 22 - page 9, line 34  see tables 1,2</p> <p style="text-align: center;">---</p>	1,7,15, 16
A	<p>MARTIN J F ET AL: "APPLICATION OF PATTERN RECOGNITION AND IMAGE CLASSIFICATION TECHNIQUES TO DETERMINE CONTINUOUS CARDIAC OUTPUT FROM THE ARTERIAL PRESSURE WAVEFORM"  IEEE TRANSACTIONS ON BIOMEDICAL ENGINEERING,  vol. 41, no. 10, 1 October 1994, pages 913-920, XP000556740  see page 913, column 2, line 9 - page 915, column 2, line 35</p> <p style="text-align: center;">-----</p>	1,7,15, 16

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/GB 98/01972

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9724982 A	17-07-1997	AU 1386197 A	01-08-1997
EP 0818175 A	14-01-1998	CN 1175892 A	11-03-1998
		WO 9716114 A	09-05-1997
US 5390679 A	21-02-1995	US 5797395 A	25-08-1998
WO 9206633 A	30-04-1992	AU 8924491 A	20-05-1992
		US 5241966 A	07-09-1993