

(12) **United States Patent**  
**Naor**

(10) **Patent No.:** **US 9,750,604 B2**  
(45) **Date of Patent:** **\*Sep. 5, 2017**

(54) **HEART VALVE PROSTHESIS WITH COLLAPSIBLE VALVE AND METHOD OF DELIVERY THEREOF**

*A61F 2/2496* (2013.01); *A61F 2220/0008* (2013.01); *A61F 2220/0016* (2013.01)

(71) Applicant: **Mitrassist Medical Ltd.**, Caesarea (IL)

(72) Inventor: **Gil Naor**, Hofit (IL)

(73) Assignee: **Mitrassist Medical Ltd.**, Caesarea (IL)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 74 days.

This patent is subject to a terminal disclaimer.

(58) **Field of Classification Search**

CPC .... *A61F 2/2418*; *A61F 2/2442*; *A61F 2/2445*; *A61F 2/2448*; *A61F 2220/0016*  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,106,129 A 8/1978 Carpentier et al.  
6,478,819 B2 11/2002 Moe  
(Continued)

FOREIGN PATENT DOCUMENTS

JP 2005-505343 2/2005  
JP 2005-535384 11/2005  
(Continued)

OTHER PUBLICATIONS

Official Action Dated Nov. 12, 2014 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

(Continued)

*Primary Examiner* — Brian Dukert

(57) **ABSTRACT**

A valve prosthesis is adapted to operate in conjunction with native heart valve leaflets. The prosthesis includes an annulus and a skirt extending from the annulus. The skirt may be configured to be positioned through a native heart valve annulus, and the skirt may be movable between an open configuration permitting blood flow through the skirt and a closed configuration blocking blood flow through the skirt in cooperation with opening and closing of the native heart valve leaflets.

**17 Claims, 17 Drawing Sheets**

(65) **Prior Publication Data**

US 2014/0214160 A1 Jul. 31, 2014


**Related U.S. Application Data**

(63) Continuation of application No. 12/726,338, filed on Mar. 17, 2010, now Pat. No. 9,078,751.

(60) Provisional application No. 61/257,979, filed on Nov. 4, 2009, provisional application No. 61/227,193, filed on Jul. 21, 2009, provisional application No. 61/186,100, filed on Jun. 11, 2009, provisional application No. 61/215,944, filed on May 12, 2009, provisional application No. 61/212,459, filed on Apr. 13, 2009, provisional application No. 61/210,255, filed on Mar. 17, 2009.

(51) **Int. Cl.**  
*A61F 2/24* (2006.01)

(52) **U.S. Cl.**  
CPC ..... *A61F 2/2418* (2013.01); *A61F 2/2436* (2013.01); *A61F 2/2442* (2013.01); *A61F 2/2445* (2013.01); *A61F 2/2448* (2013.01);

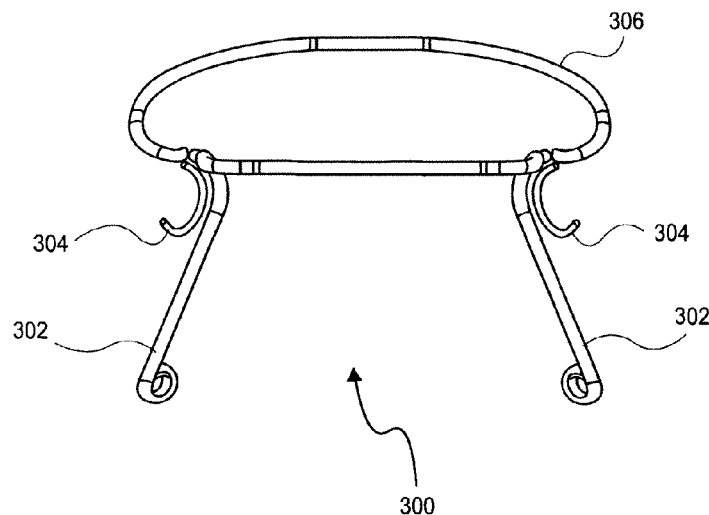

(56)

**References Cited**

**U.S. PATENT DOCUMENTS**

6,726,717	B2	4/2004	Alfieri et al.	
7,381,220	B2	6/2008	Macoviak et al.	
8,092,520	B2	1/2012	Quadri	
2001/0010017	A1	7/2001	Letac et al.	
2001/0049556	A1	12/2001	Moe	
2003/0199975	A1	10/2003	Gabbay	
2004/0127982	A1*	7/2004	Machold	A61F 2/2418
				623/2.36
2004/0243230	A1*	12/2004	Navia	A61F 2/2445
				623/2.36
2005/0010287	A1*	1/2005	Macoviak	A61F 2/2445
				623/2.36
2005/0228495	A1	10/2005	Macoviak	
2006/0058871	A1	3/2006	Zakay et al.	
2006/0195183	A1	8/2006	Navia et al.	
2007/0010877	A1	1/2007	Salahieh et al.	
2007/0067029	A1	3/2007	Gabbay	
2007/0156233	A1	7/2007	Kapadia et al.	
2007/0185571	A1	8/2007	Kapadia et al.	
2007/0270943	A1	11/2007	Solem et al.	
2008/0065204	A1	3/2008	Macoviak et al.	
2008/0071362	A1*	3/2008	Tuval	A61F 2/2418
				623/2.1
2008/0208328	A1	8/2008	Antocci et al.	
2009/0005863	A1	1/2009	Goetz et al.	
2010/0280606	A1	11/2010	Naor	
2010/0298931	A1	11/2010	Quadri et al.	
2012/0078353	A1	3/2012	Quadri et al.	
2012/0215303	A1	8/2012	Quadri et al.	
2016/0038282	A1	2/2016	Naor	

**FOREIGN PATENT DOCUMENTS**

JP	2007-536003	12/2007
WO	WO 03/030776	4/2003
WO	WO 2004/014258	2/2004
WO	WO 2004/030568	4/2004

WO	WO 2004/089250	10/2004
WO	WO 2005/027797	3/2005
WO	WO 2005/107650	11/2005
WO	WO 2010/106438	9/2010

**OTHER PUBLICATIONS**

Applicant-Initiated Interview Summary Dated Jan. 20, 2015 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

Notice of Reason for Rejection Dated Sep. 26, 2014 From the Japanese Patent Office Re. Application No. 2012-5000334 and Its Translation Into English.

International Preliminary Report on Patentability Dated Sep. 29, 2011 From the International Bureau of WIPO Re. Application No. PCT/IB2010/000833.

International Search Report and the Written Opinion Dated Sep. 1, 2010 From the International Searching Authority Re. Application No. PCT/IB2010/000833.

Notice of Reason for Rejection Dated Jan. 24, 2014 From the Japanese Patent Office Re. Application No. 2012-5000334 and Its Translation Into English.

Official Action Dated Jul. 5, 2011 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

Official Action Dated Aug. 6, 2012 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

Official Action Dated Feb. 22, 2013 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

Official Action Dated Mar. 25, 2014 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.


Official Action Dated Sep. 28, 2011 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

Official Action Dated Mar. 29, 2012 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.


Restriction Official Action Dated Dec. 19, 2013 From the US Patent and Trademark Office Re. U.S. Appl. No. 12/726,338.

Restriction Official Action Dated Jul. 12, 2016 From the US Patent and Trademark Office Re. U.S. Appl. No. 14/797,218.


\* cited by examiner

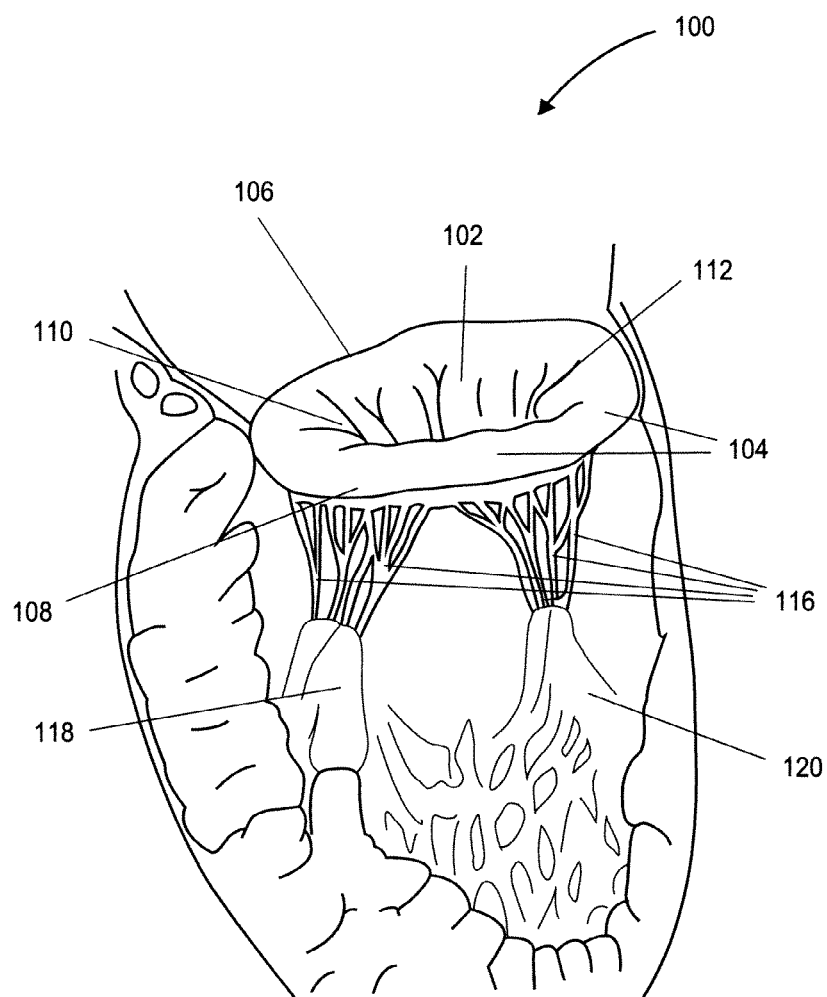


**FIG. 1**

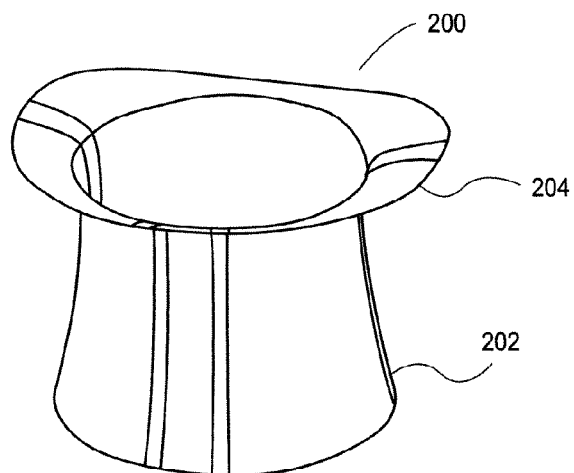


**FIG. 2A**

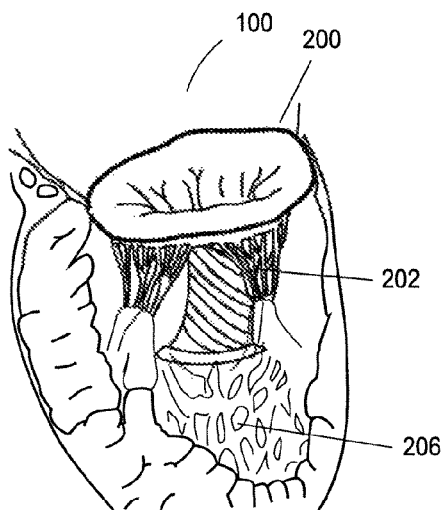


**FIG. 2B**

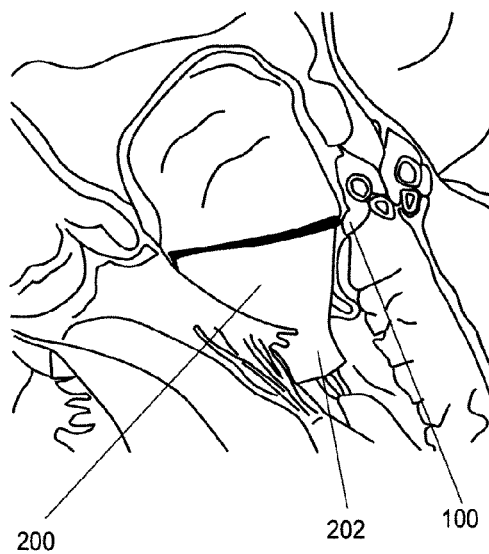


**FIG. 2C**

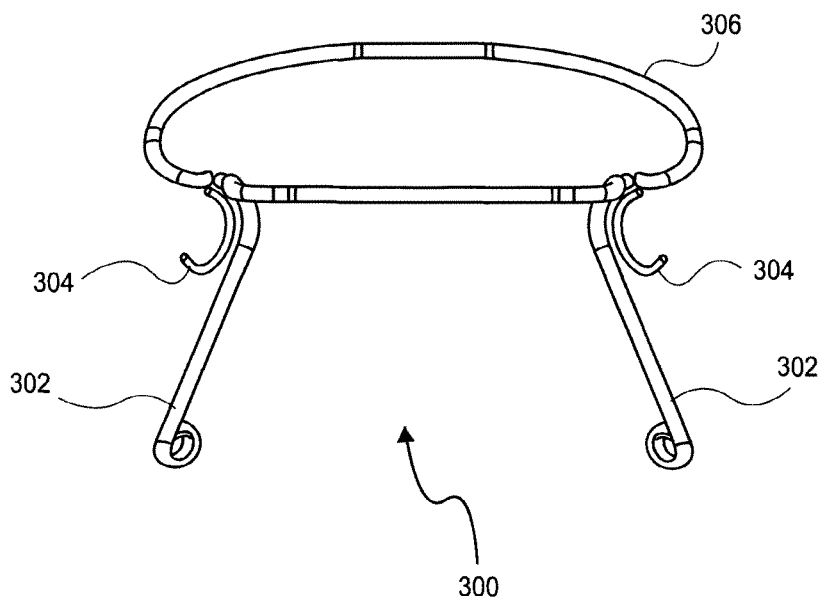


**FIG. 3**

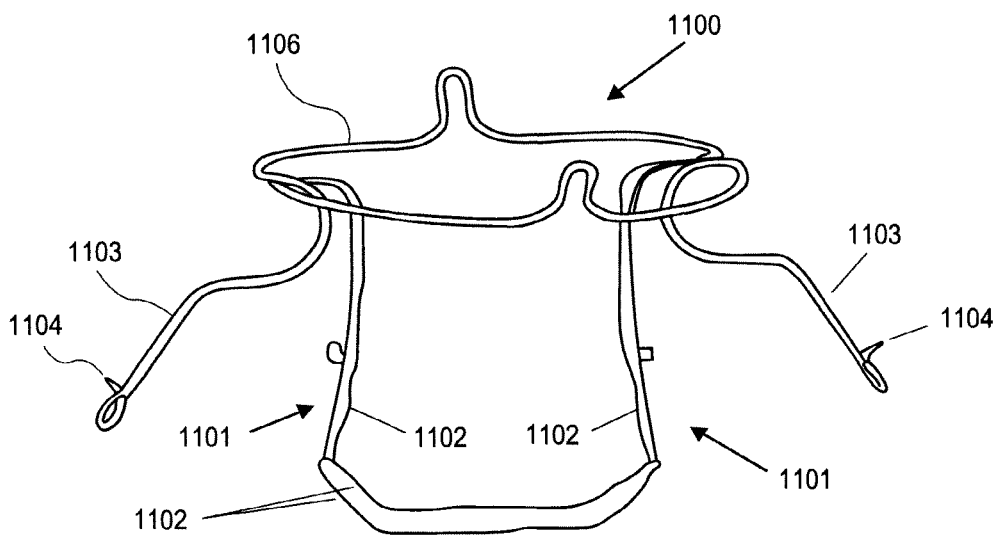


**Fig. 11**

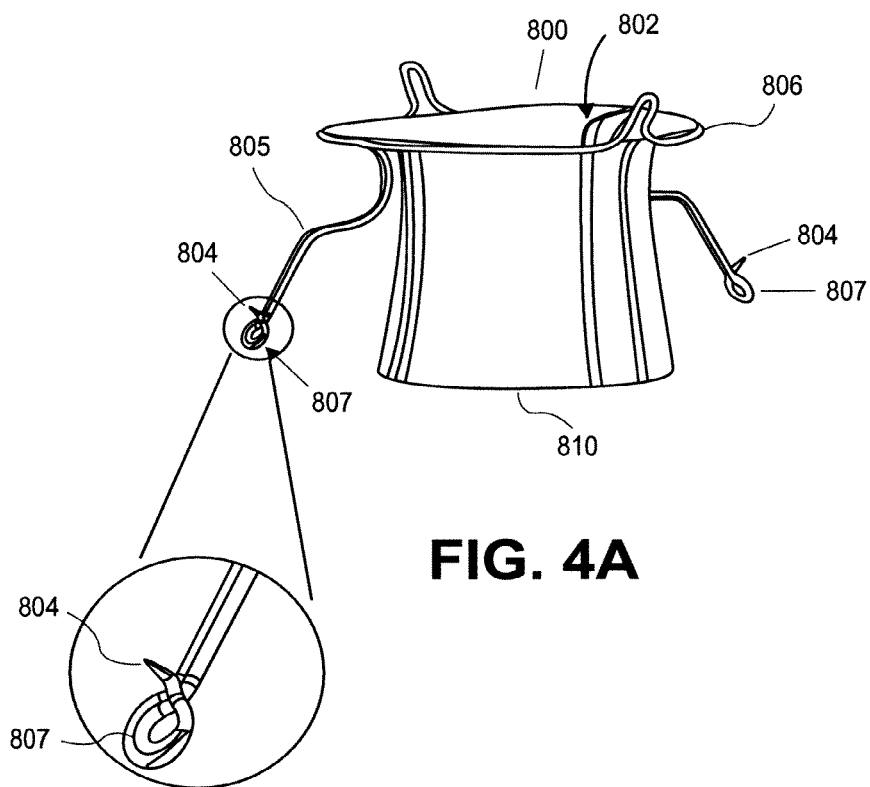


**FIG. 4A**

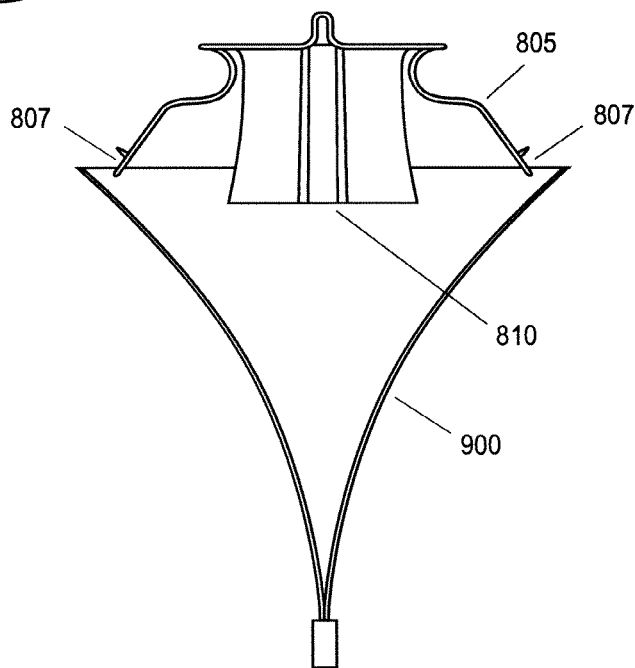


**FIG. 4B**

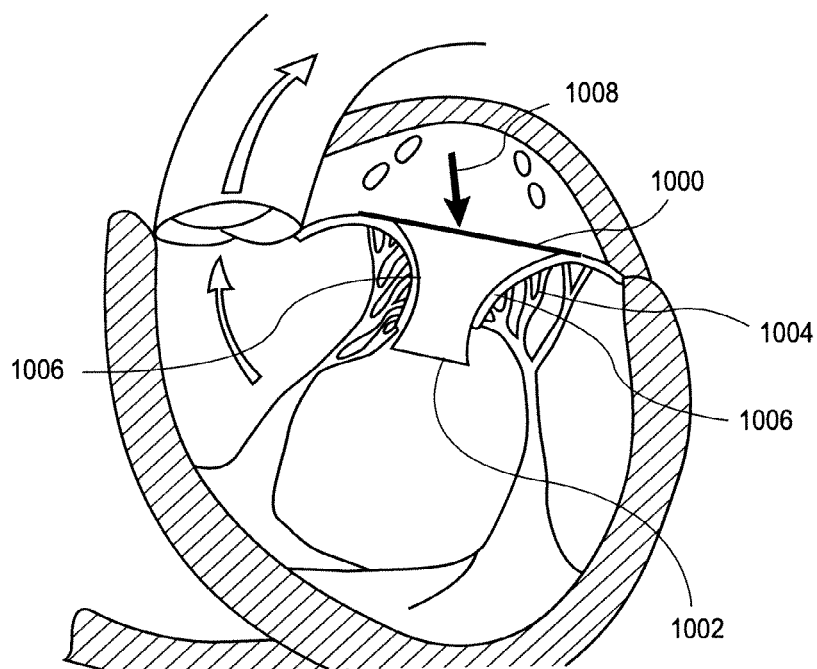


**FIG. 5**

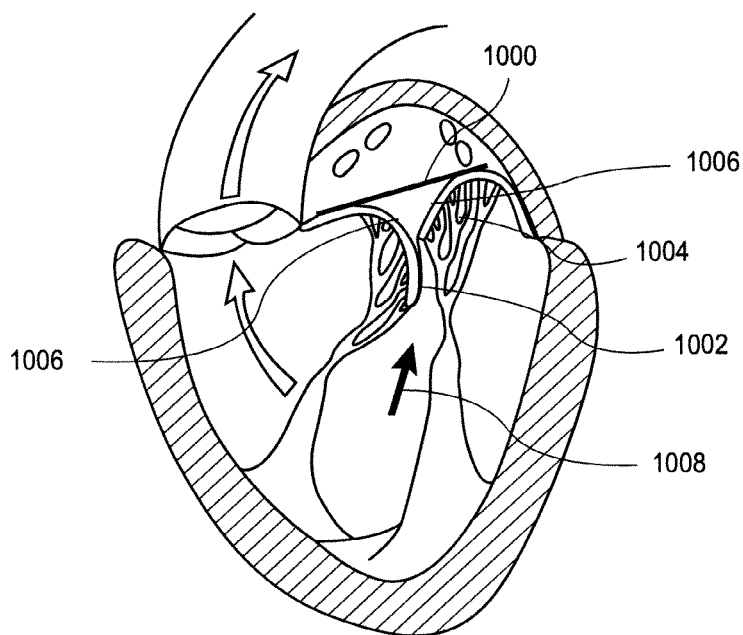


**FIG. 6**

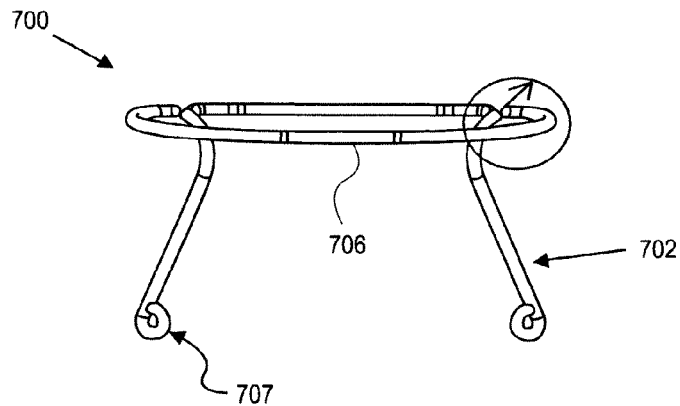


**FIG. 7**

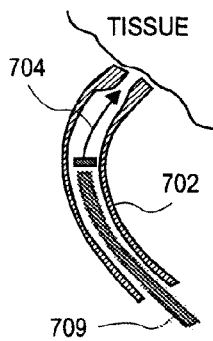


**FIG. 8A**

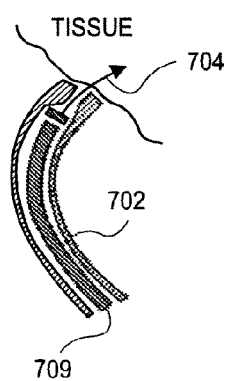

**FIG. 8B**

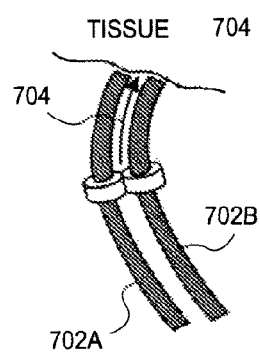


**FIG. 8C**

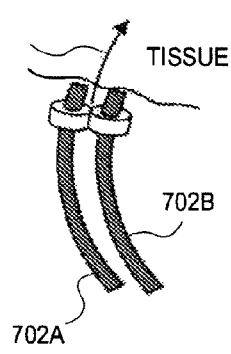

**FIG. 8D**



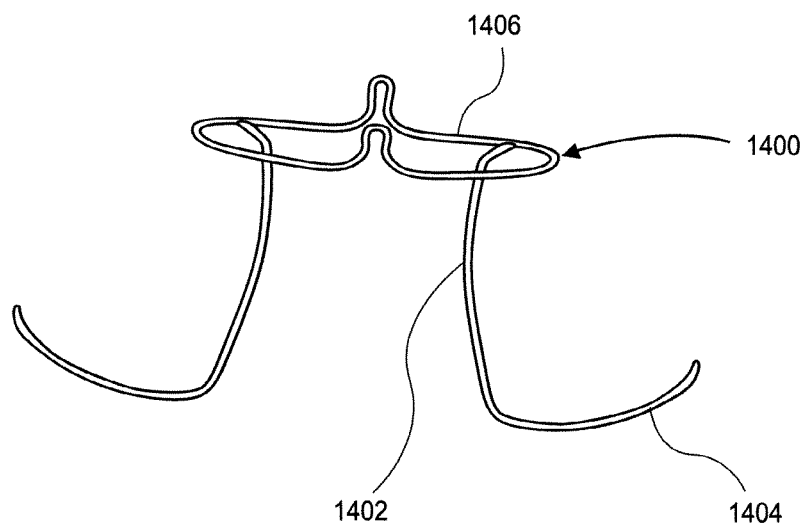

**FIG. 9**



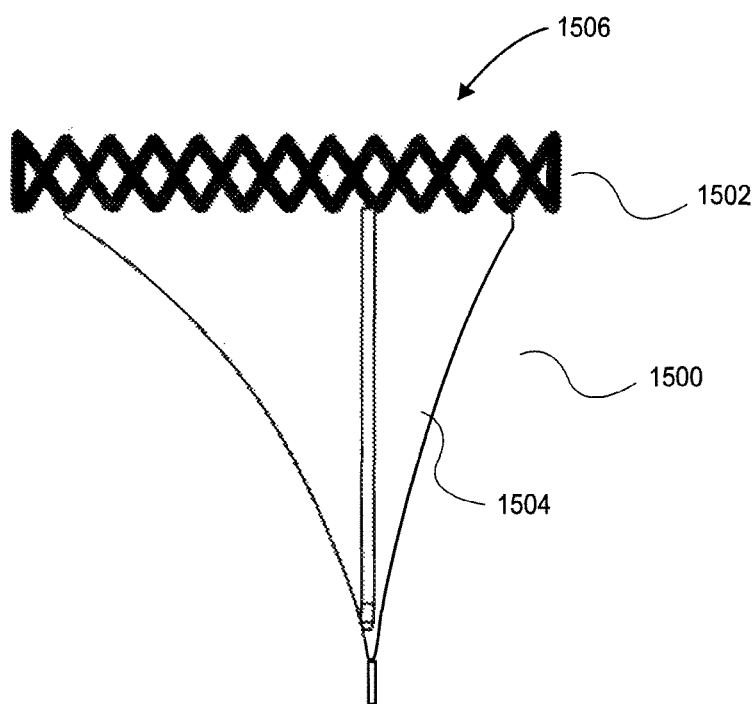



FIG. 10

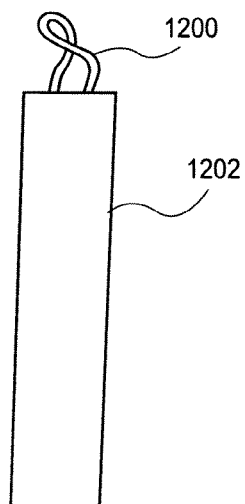


**FIG. 12A**

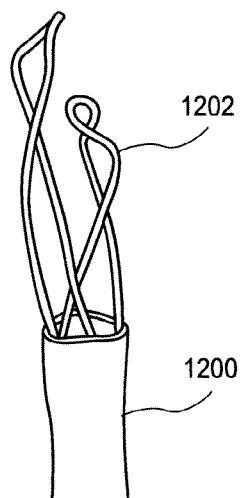

**FIG. 12B**

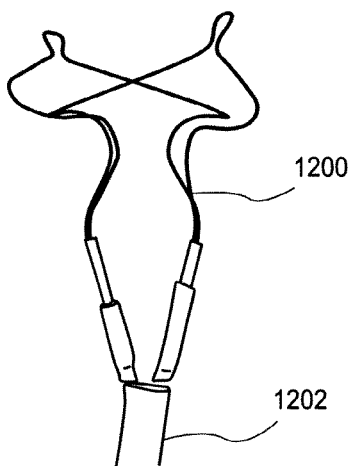

**FIG. 12C**

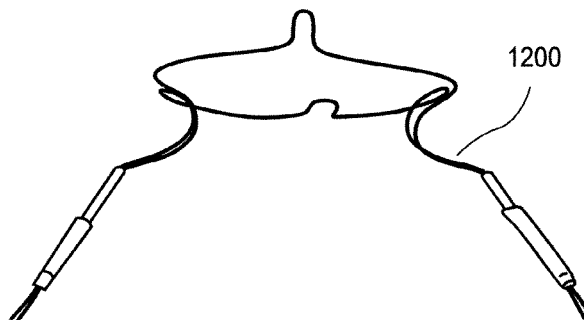

**FIG. 12D**

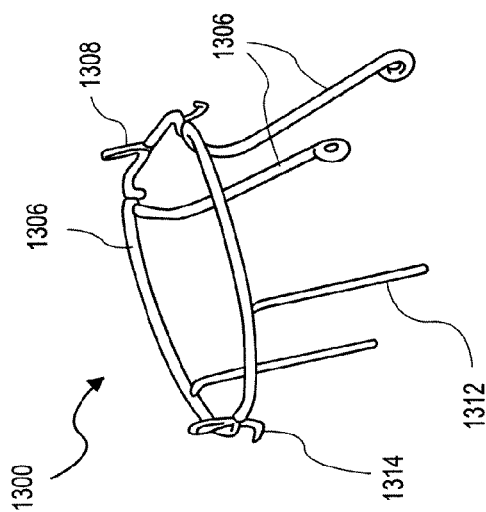


FIG. 13A

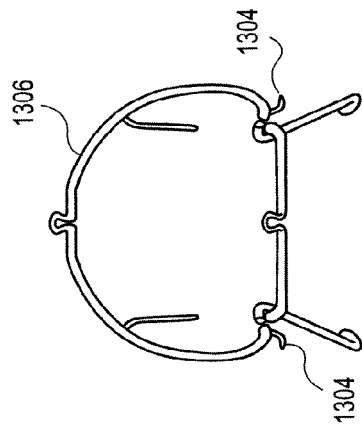


FIG. 13B

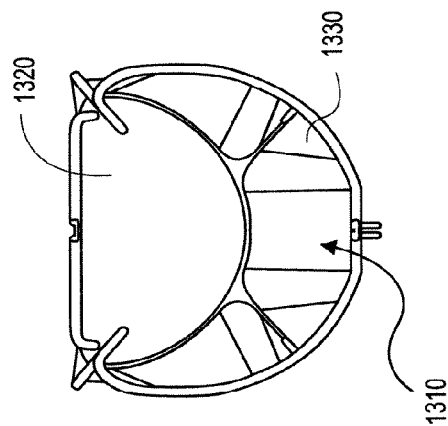


FIG. 13D

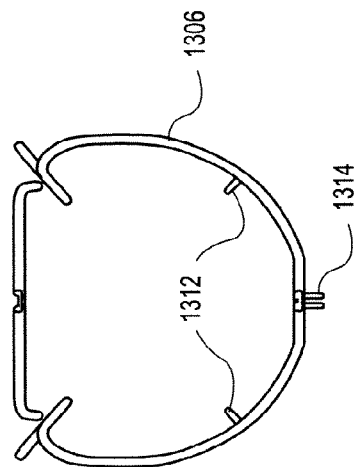


FIG. 13C

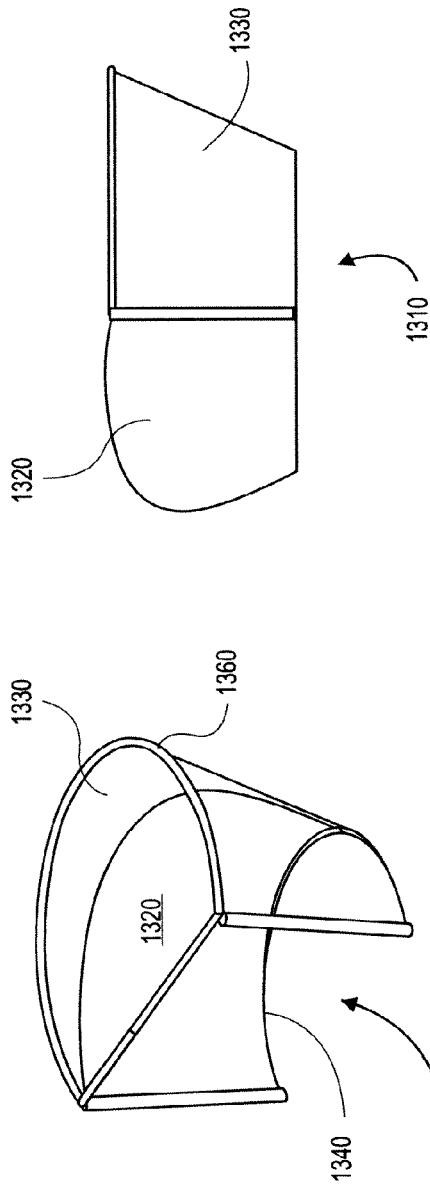


FIG. 14A

FIG. 14B

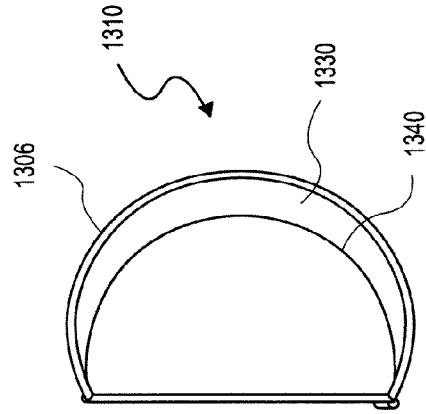


FIG. 14D



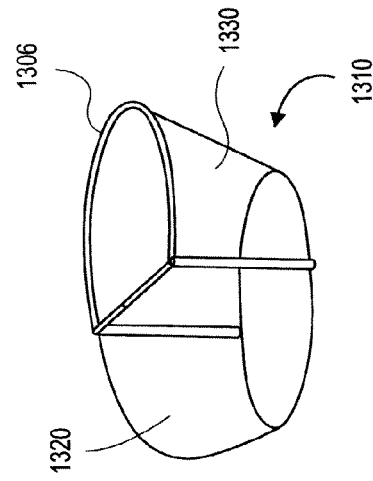



FIG. 14C

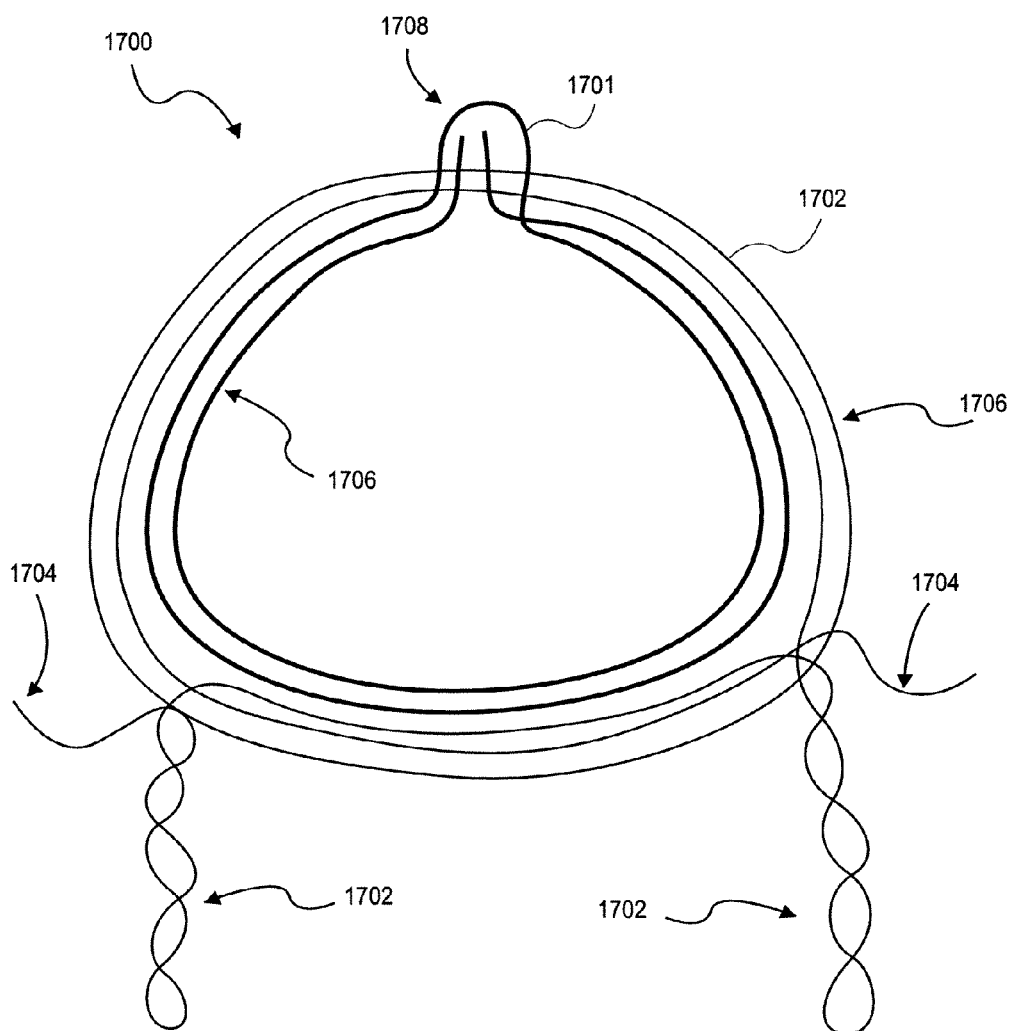

**FIG. 15**

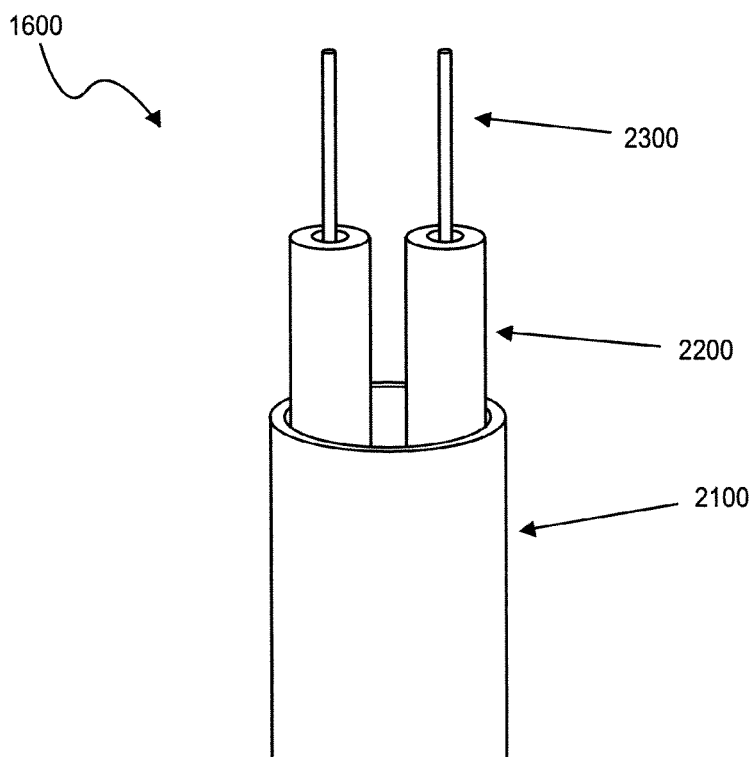


**FIG. 16**

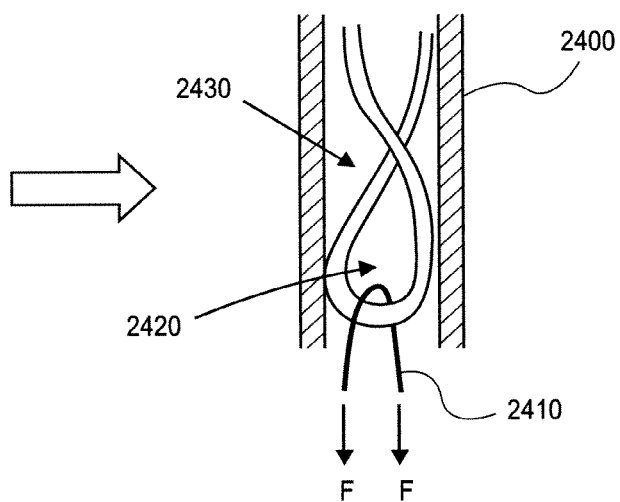



**FIG. 17**



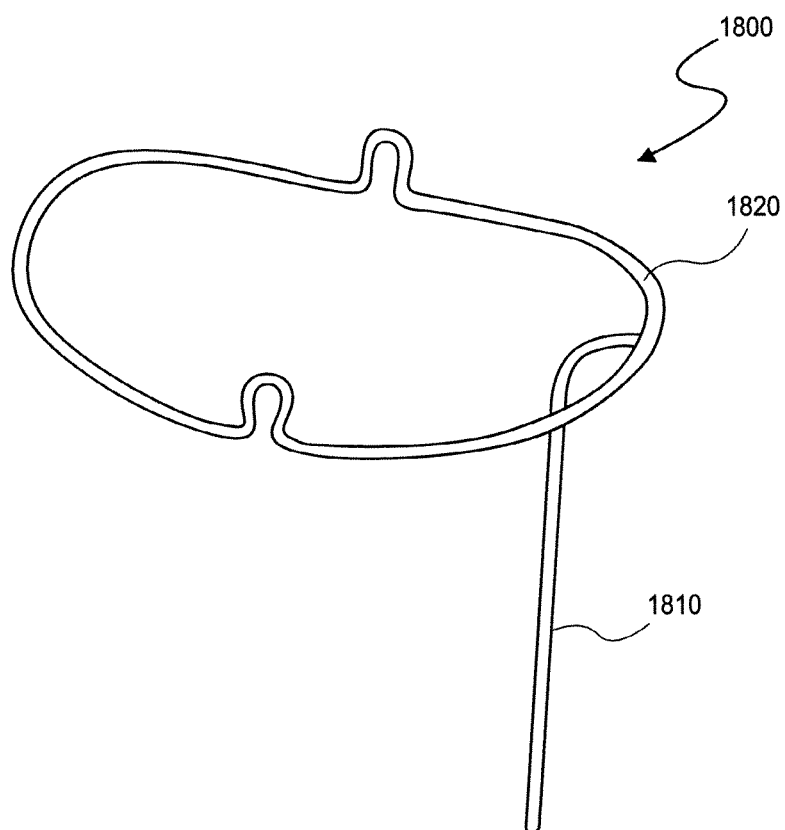

**FIG. 18**

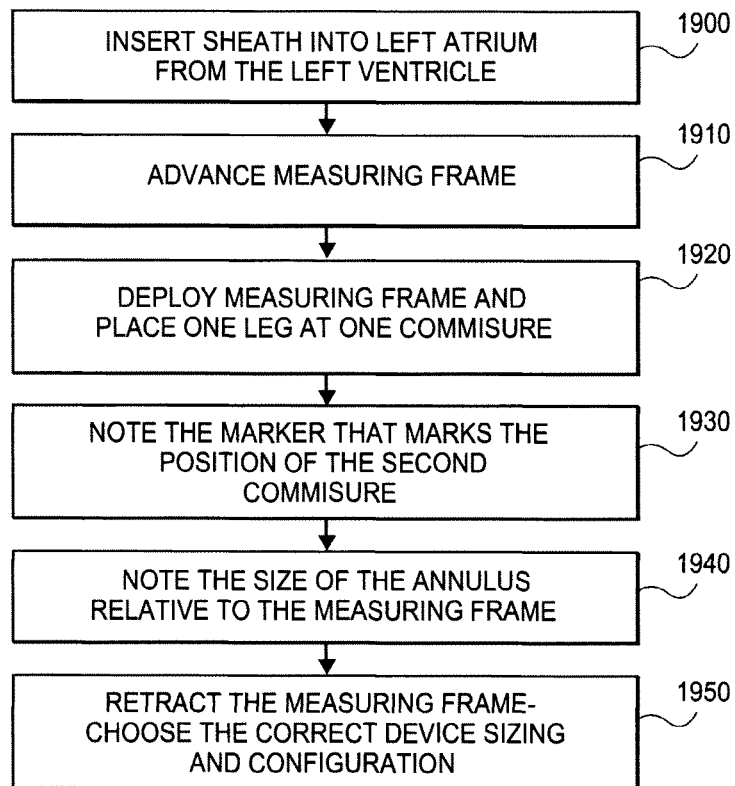**FIG. 19**

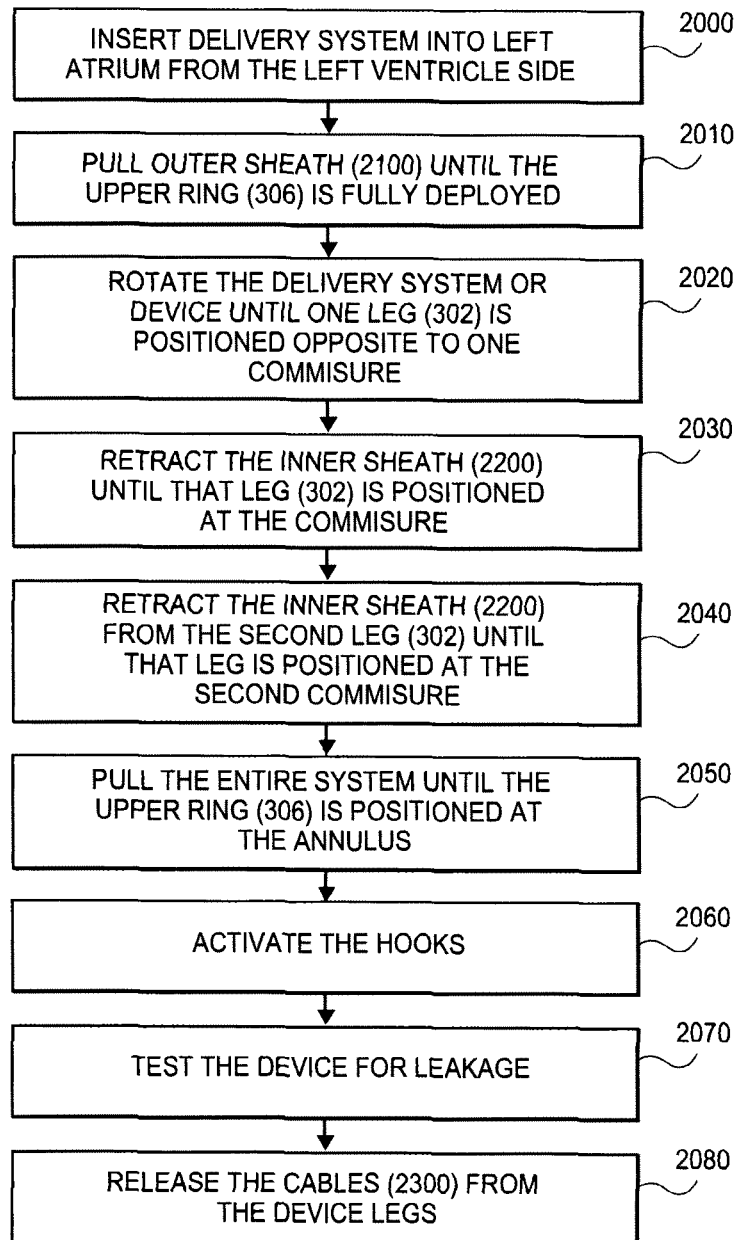**FIG. 20**

1

# HEART VALVE PROSTHESIS WITH COLLAPSIBLE VALVE AND METHOD OF DELIVERY THEREOF

## RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 12/726,338 filed on Mar. 17, 2010, which claims the benefit of priority of U.S. Provisional Patent Application Nos. 61/257,979 filed on Nov. 4, 2009, 61/227,193 filed on Jul. 21, 2009, 61/186,100 filed on Jun. 11, 2009, 61/215,944 filed on May 12, 2009, 61/212,459 filed on Apr. 13, 2009 and 61/210,255 filed on Mar. 17, 2009. The contents of the above applications are all incorporated by reference as if fully set forth herein in their entirety.

## TECHNICAL FIELD

The present disclosure relates to minimally invasive surgical or percutaneous replacement and/or repair of a valve, namely the mitral valve or the tricuspid valve. More particularly, the present disclosure relates to a heart valve prosthesis with a collapsible valve and a method of delivery of the prosthesis.

## BACKGROUND

The mitral valve and tricuspid valve are unidirectional heart valves that separate the atria left and right respectively, from the corresponding heart ventricles. These valves have a distinct anatomical and physiological structure, having two (mitral) or three (tricuspid) sail-like leaflets connected to a subvalvular mechanism of strings (chordae tendinae) and papillary muscles forming a part of the heart's ventricular shape, function and size.

The heart has four chambers: the right and left atria, and the right and left ventricles. The atria receive blood and then pump it into the ventricles, which then pump it out into the body.

The synchronous pumping actions of the left and right sides of the heart constitute the cardiac cycle. The cycle begins with a period of ventricular relaxation, called ventricular diastole. The cycle ends with a period of ventricular contraction, called ventricular systole.

The heart has four valves that ensure that blood does not flow in the wrong direction during the cardiac cycle; that is, to ensure that the blood does not back flow from the ventricles into the corresponding atria, or back flow from the arteries into the corresponding ventricles. The valve between the left atrium and the left ventricle is the mitral valve. The valve between the right atrium and the right ventricle is the tricuspid valve. The pulmonary valve is at the opening of the pulmonary artery. The aortic valve is at the opening of the aorta.

The opening and closing of heart valves occur primarily as a result of pressure differences. For example, the opening and closing of the mitral valve occurs as a result of the pressure differences between the left atrium and the left ventricle. During ventricular diastole, when ventricles are relaxed, the venous return of blood from the pulmonary veins into the left atrium causes the pressure in the atrium to exceed that in the ventricle. As a result, the mitral valve opens, allowing blood to enter the ventricle. As the ventricle contracts during ventricular systole, the intraventricular pressure rises above the pressure in the atrium and pushes the mitral valve shut.

2

As noted above, these valves feature a plurality of leaflets connected to chordae tendinae and papillary muscles, which allow the leaflets to resist the high pressure developed during contractions (pumping) of the left and right ventricles.

In a healthy heart, the chords become taut, preventing the leaflets from being forced into the left or right atria and everted. Prolapse is a term used to describe the condition wherein the coaptation edges of each leaflet initially may coapt and close, but then the leaflets rise higher and the edges separate and the valve leaks. This is normally prevented by contraction of the papillary muscles and the normal length of the chords. Contraction of the papillary muscles is simultaneous with the contraction of the ventricle and serves to keep healthy valve leaflets tightly shut at peak contraction pressures exerted by the ventricle.

Valve malfunction can result from the chords becoming stretched, and in some cases tearing. When a chord tears, the result is a flailed leaflet. Also, a normally structured valve may not function properly because of an enlargement of the valve annulus pulling the leaflets apart. This condition is referred to as a dilation of the annulus and generally results from heart muscle failure. In addition, the valve may be defective at birth or because of an acquired disease, usually infectious or inflammatory.

Diseases of the valves can cause either narrowing (stenosis) or dilatation (regurgitation, insufficiency) or a combination of those, of the valve. Surgical treatment for repair or replacement of the valves includes an open-heart procedure, extracorporeal circulation and, if replaced, a complete resection of the diseased valve.

Currently all available surgical options for valve replacement involve open heart surgery; although minimally invasive methods for valve replacement are more desirable, such methods are still in the experimental stage.

Even valves which could theoretically be provided through a non-invasive method, such as those taught by U.S. Pat. No. 7,381,220, have many drawbacks. For example, the taught valves are useful for replacement of the existing valves; however, their installation through non-invasive means is problematic. Furthermore, the valves themselves, even when installed in a manner that supports existing valve tissue, must still withstand very high pressures. Such high pressures can lead to many different types of problems, including reflux as blood returns through heart in a retrograde manner.

It may be desirable to provide a valve prosthesis that supports the mitral and/or tricuspid valve without necessarily replacing it, but instead supplements the native valve functionality by providing an adjunctive valve prosthesis, which cooperates together with the native valve for improved functionality. The background art also does not teach or suggest such a valve prosthesis which may optionally be inserted through minimally invasive surgical techniques.

## SUMMARY OF INVENTION

In accordance with various aspects of the disclosure, a valve prosthesis is adapted to operate in conjunction with native heart valve leaflets. The prosthesis includes an annulus and a skirt extending from the annulus. The skirt may be configured to be positioned through a native heart valve annulus, and the skirt may be movable between an open configuration permitting blood flow through the skirt and a

closed configuration blocking blood flow through the skirt in cooperation with opening and closing of the native heart valve leaflets

According to various aspects, a novel valve prosthesis, for example, for a tricuspid valve and/or mitral valve, may be inserted through any one or more of a minimally invasive surgical procedure, a “traditional” operative procedure (which may for example involve open heart surgery), or a trans-catheter procedure.

The valve prosthesis, in at least some embodiments, is a (optionally non-stented) bioprosthesis attached by means of suture or any other means of bonding, to an expandable, frame (platform), which may be made from a suitable metal, including without limitation an alloy, or any type of suitable composite material (optionally including those that include metal). The frame can be made of self expanding alloy such as Nitinol (nickel/titanium alloy) or made of another metal, such as a cobalt/chrome alloy, expanded by a specialized balloon, or radial expander.

The frame engages the tissue at or near or above the top margins of the native valve (annulus). The native valve is not removed, and the ventricular shape and function are preserved. Therefore, the valve prosthesis may not replace the native valve functionality but rather supports its function.

By “native valve” or “native valve annulus” it is meant the valve or valve annulus already present in the subject, as opposed to an artificial valve or valve annulus.

According to some embodiments, the valve prosthesis comprises a support structure featuring a deployable construction adapted to be initially collapsed (crimped) in a narrow configuration suitable for introduction through a small puncture or incision into the heart cavity such as the left ventricle, the left atrium, the right atrium, the right ventricle and so forth, thereby providing access to the target location. It is further adapted to be deployed by means of removing a radial constriction such as a sheath to allow the platform to self-expand to its deployed state in the target location.

In some embodiments, the valve prosthesis optionally features a flexible film made of biological tissue such as pericardia tissue but may also optionally feature one or combination of synthetic materials, additionally or alternatively. The prosthesis may have a funnel like shape that is generally tubular and may have a variable diameter that enables flow in one direction (from the atrium to the ventricle); when the ventricle contracts, the funnel shape valve collapses and blocks any return flow from the ventricle to the atrium. Such retrograde flow is quite dangerous; over a prolonged period of time, it can lead to many deleterious health effects, including on the overall health of the heart muscle.

In an exemplary, illustrative configuration, the valve platform of the prosthesis is anchored to the ventricle wall through extensions that pass through the commissures of the native valve or at the plane of the commissures and have hooks at their ends that anchor into the ventricular wall between the chordate attachment to the ventricular wall. Furthermore, in an illustrative example, these extensions have curved ends that can be in any plane (but which may be at a 90 degree angle to the plane of both extensions) that allows a wire or cable to pass through and keep the prosthesis connected to the delivery system as long as this wire or cable is not released. The delivery action of the prosthesis may be reversible. That is, the device may optionally be refolded into the catheter after having being deployed.

In an optional embodiment, these extensions should not act on the valve in any way, including not on the valve

annulus or surrounding valve tissue, nor should these extensions apply any pressure that may reshape the annulus or deform the leaflet configuration.

In an exemplary embodiment, the valve prosthesis features a “skirt” that does not restrict the motion of any of the native valve leaflets but which is situated above such leaflets, for example in the direction of the atrium (by “above” it is meant with regard to the direction of normal, not retrograde, blood flow). If the leaflets prolapse into the atrium, no blood will be able to flow into the atrium because the skirt is situated above the native valve, thus preventing retrograde blood flow into the atrium from the ventricle.

In an embodiment, the “skirt” is generally tubular in shape with a diameter that may vary and which is optionally used to complete the incompetent closure of the native valve as a whole. Thus, the skirt specifically and the valve prosthesis generally are not intended to be used as a replacement to the entire valve or in addition to only one native leaflet (in contrast to the apparatus described by Macoviak et al. in U.S. patent application publication number 2008/0065204, for example). In an exemplary embodiment, the valve skirt may be reinforced with at least one reinforcement along at least a portion of its length, for example, along the entirety of its length, in order to prevent prolapse of the skirt into the left atrium. This reinforcement is optionally an extension from the platform.

In yet another configuration, the valve “skirt” is connected to the extensions by a cable or wire in order to prevent the prolapsed of the skirt into the left atrium. These connections may optionally be an integral part of the valve platform or alternatively may be connected separately.

In an exemplary embodiment, the closing action of the native valve leaflets promotes the collapse of the prosthetic valve (skirt). Thus, during systole function, the native valve may achieve partial closure (i.e. function partially) and hence may assist the function of the valve prosthesis.

During systole, the action of the native valve leaflets is to close the passage between the left ventricle and the left atrium. In an exemplary embodiment, the leaflets, while acting as such, resist part of the pressure applied by the blood pressure in the ventricle during valve closure as well as reducing the effective area on which the pressure is applied to the valve prosthesis as a whole, thus reducing the total force applied to the prosthesis for migration into the left atrium. Depending on which valve is affected, the present invention is contemplated as a potential treatment for all forms of valvular regurgitation, such as tricuspid regurgitation, pulmonary regurgitation, mitral regurgitation, or aortic regurgitation.

#### BRIEF DESCRIPTION OF THE DRAWINGS

In the drawings:

FIG. 1 shows an exemplary anatomy of a mitral valve (for reference only);

FIGS. 2a-2c show an exemplary valve prosthesis according to some embodiments of the present disclosure; FIG. 2a shows the valve skirt alone, and FIGS. 2b and 2c show the valve skirt in place in the heart as an example only;

FIG. 3 shows an illustrative embodiment of an exemplary valve prosthesis in accordance with various aspects of the disclosure;

FIGS. 4a-4b show an illustrative configuration of an exemplary valve prosthesis according to some embodiments of the present disclosure;

FIG. 5 shows a schematic view of the prosthetic and native mitral valve leaflets during Diastole;

5

FIG. 6 shows a schematic view of the prosthetic and native mitral valve leaflets during Systole;

FIG. 7 shows an illustrative embodiment of an exemplary valve prosthesis in accordance with various aspects of the disclosure;

FIGS. 8A-8D show illustrative embodiments of various exemplary valve prostheses in accordance with various aspects of the disclosure;

FIG. 9 shows an exemplary frame for a valve prosthesis in accordance with various aspects of the disclosure;

FIG. 10 shows an exemplary valve prosthesis in accordance with various aspects of the disclosure;

FIG. 11 shows an exemplary frame for a valve prosthesis in accordance with various aspects of the disclosure;

FIGS. 12A-12D show an exemplary prosthesis in its folded state and as it unfolds from a catheter;

FIGS. 13A-13D show an exemplary valve prosthesis in accordance with various aspects of the disclosure;

FIGS. 14A to 14D show an exemplary skirt for a valve prosthesis in accordance with various aspects of the disclosure;

FIG. 15 shows an exemplary delivery system for a valve prosthesis in accordance with various aspects of the disclosure;

FIG. 16 shows a portion of an exemplary delivery system valve prosthesis in accordance with various aspects of the disclosure;

FIG. 17 shows a portion of an exemplary delivery system valve prosthesis in accordance with various aspects of the disclosure;

FIG. 18 is an exemplary measuring device for use in delivery of a valve prosthesis in accordance with various aspects of the disclosure;

FIG. 19 is a flow chart of an exemplary delivery method of a valve prosthesis in accordance with various aspects of the disclosure; and

FIG. 20 is a flow chart of an exemplary pre-delivery method of a valve prosthesis in accordance with various aspects of the disclosure.

#### DETAILED DESCRIPTION

The disclosure provides, in at least some embodiments, a valve prosthesis and method of insertion thereof which supports the mitral and/or tricuspid valve without replacing it. The valve prosthesis may operate to support the native valve leaflets to provide a functioning heart valve and to prevent retrograde motion of the blood, even if the native valve leaflets alone are unable to completely close and/or to prevent such retrograde motion of the blood.

FIG. 1 shows an exemplary anatomy of a native mitral valve (for reference only). As shown, a native valve **100** features an anterior leaflet **102** and a three lobed posterior leaflet **104**, which together comprise the leaflets of native valve **100**, as well as an anterior annulus **106** and a posterior annulus **108**, which together comprise the annulus of native valve **100**. Native valve **100** also features a posterolateral commissure **110** and an anteromedial commissure **112**, one or both of which are optionally used for installation of a valve prosthesis according to some embodiments of the present disclosure.

A plurality of chordinae tendinae **116** attach the leaflets to a lateral papillary muscle **118** or a medial papillary muscle **120**. In a healthy heart, chordinae tendinae **116** become taut to prevent retrograde blood flow back through the leaflets. In a non-healthy heart, for a variety of reasons as described above, bloods flow in a retrograde manner through the

6

leaflets. As described in greater detail below, in at least some embodiments of the present disclosure, the leaflets are assisted in their function by a valve prosthesis.

FIGS. 2a-2c show an exemplary valve prosthesis according to some embodiments of the present disclosure. As shown in FIG. 2a, a valve prosthesis **200** may comprise a valve skirt **202** and a prosthetic valve annulus **204** according to various aspects of the present disclosure. Although not clearly shown in FIG. 2a, in some aspects, the prosthetic valve annulus **204** may have a D-shape configuration. In some aspects, the annulus **204** may have an oval configuration.

According to various aspects, the skirt **202** may comprise a biological tissue, such as, for example, an animal (e.g., bovine or porcine tissue) or human pericardium. In some aspects, the skirt **202** may comprise a synthetic material, such as, for example, polyurethane. In various aspects, the skirt **202** may comprise a native mitral valve processed to be biologically compatible for a particular implantation.

According to some aspects, the skirt **202** may comprise an ultra-thin sheet of nitinol. According to various aspects of the disclosure, the skirt **202** and/or the prosthetic annulus **204** may be coated with various bioactive agents, such as anti-proliferative and/or anti-inflammatory properties or can have other properties such as antineoplastic, antiplatelet, anti-coagulant, anti-fibrin, antithrombotic, antimetabolic, anti-biotic, antiallergic, antioxidant as well as cystostatic agents, anti-inflammatory agents (e.g., steroidal anti-inflammatory agent, a nonsteroidal anti-inflammatory agent, or a combination thereof, and anti-proliferative agents (e.g., rapamycin and derivatives of rapamycin; everolimus and derivatives of everolimus; taxoids including taxols, docetaxel, paclitaxel, and related derivatives of taxoids, Biolimus A9, etc.). According to various aspects, the skirt may have a thickness of between about 0.05 mm and about 0.4 mm.

According to some aspects, the length of valve prosthesis **200** is at least as long as the native valve leaflets, but is not excessively long so as to avoid disturbing the flow through the aortic or adjacent valve. For example, in some aspects, the length of valve prosthesis **200** is no more than about 120% of the length of the native valve leaflets. According to various aspects, the diameter of the bottom of valve skirt **202** is at least about 80% of the diameter of the native valve area and no more than about 130% of the diameter of the native valve area.

FIG. 2b shows an exemplary valve prosthesis **200** in place in a mitral valve **100** as an illustrative example only of installation. Valve skirt **202** is shown as well, extending into a ventricle **206**. FIG. 2c shows the view of FIG. 2b in cross-section. Valve skirt **202** is configured and positioned to prevent retrograde flow of blood from the ventricle **206** back into the atrium (not shown) by assisting the function of the natural, native leaflets of the mitral valve **100**. It should be appreciated that the exemplary valve prosthesis **200** may also be placed in a tricuspid valve in accordance with various aspects of the disclosure.

FIG. 3 shows an exemplary valve frame, or valve platform, configured to support a valve skirt of a valve prosthesis in accordance with various aspects of the present disclosure. Valve frame **300** may comprise a valve annulus **306**, for example, a D-shaped annulus. According to various aspects, the semi-circular section of the D-shape may have a length at least about 1.1 to 2 times greater than that of the straight section.

According to various aspects, the valve frame **300** may comprise a wire having a diameter of about 0.3 mm to about 1.0 mm, although other diameters may be selected depend-

ing upon the material chosen for the wire, in order to maintain a desired tensile strength of the valve frame **300**, as well as its ability to be folded and delivered through a catheter at least in some embodiments. Any suitable material may optionally be used for the wire as long as it retains sufficient superelasticity and may also optionally be selected from any material described herein. For example, the valve frame **300** may comprise a nickel titanium alloy (i.e., nitinol).

The valve frame **300** may include a pair of reinforcement members **302** extending from the valve annulus **306**. The reinforcement members **302** are configured such that they extend along an interior surface of a valve skirt (not shown) of an exemplary valve prosthesis. The reinforcement members **302** may thus prevent the valve skirt from everting back into the atrium after deployment. The frame **300** may also include two or more hooks **304** extending from the valve annulus **306** and configured to anchor the prosthesis to the ventricle wall. In summary, the frame of valve prosthesis incorporates various anchoring members which provide stability of the valve mechanism during cardiac function, and prevent migration of the valve prosthesis over time relative to its originally deployed anatomic position. For example, the anchoring members can comprise example, hook-like members or barbs disposed at circumferentially-distributed locations along the annulus of the frame, at the distal ends of each reinforcement member. Additionally the anchoring members can also comprise expandable annulus frame designs which ensure fluid tight wall apposition along its outer periphery with the annulus of the native valve, such as by the use of a properly sized, expandable, nitinol frame, or in the alternative, the use of a radially-expandable, plastically deformable, stent-like body which cooperates with the wire frame to ensure wall apposition with the native valve annulus.

FIGS. **4a-4b** show an illustrative configuration of an exemplary valve prosthesis in accordance with various aspects of the disclosure. As shown, a valve prosthesis **800** may include a valve annulus **806** with a pair of reinforcing members **802** extending therefrom through a valve skirt **810**. The valve annulus **806** may include a plurality of folded loops **308**. The folded loops **308** may enable the valve prosthesis **800**, including the valve frame, to be folded and collapsed for delivery through a catheter, as described in greater detail below. As shown, a pair of curved, hooked extensions **805** extend from the valve annulus. The extensions **805** may include hooks **804** at its ends opposite to the valve annulus **806**. The extensions may also include eyelets **807** configured to receive a delivery cable **900** (FIG. **4b**) therethrough. The delivery cable **900** may pass through the eyelets **806**, circle at least partially around the base of the skirt **810**, and then down through the catheter (not shown), for example for adjustment of the placement of the valve prosthesis **800** at the native valve annulus, by collapsing the valve prosthesis back into the catheter for placement in a different or adjusted location. Upon installation, once the surgeon or doctor has positioned the valve prosthesis correctly, delivery cable **900** may be removed, for example, by being withdrawn through the catheter.

FIG. **5** shows a schematic view of an exemplary prosthetic valve and the native mitral valve leaflets during diastole. As shown, a schematic valve prosthesis **1000** with a valve skirt **1002** may be installed in a native valve **1004** having a plurality of native valve leaflets **1006**. The blood flow pressure gradient **1008** is also indicated by an arrow. Native valve leaflets **1006** are open, and the prosthetic valve skirt **1002** is shown as being expanded to permit blood flow.

FIG. **6** shows a schematic view of the exemplary prosthetic valve and native mitral valve leaflets during systole, when native valve **1004** should be closed. However, native valve leaflets **1006** are only partially closed due to incomplete coaptation, resulting in valve regurgitation. Blood flow pressure gradient **1008** has now reversed, which could lead to retrograde blood flow, since valve leaflets **1006** are not completely closed. However, such retrograde blood flow is prevented by the collapse of prosthetic valve skirt **1002**. The collapse of prosthetic valve skirt **1002** is assisted by the partial closure of native valve leaflets **1006**.

Referring now to FIG. **7**, an exemplary valve frame for a valve prosthesis in accordance with various aspects of the disclosure is described. As shown, a valve frame **700** may include a valve annulus **706** with a pair of reinforcing members **702** extending therefrom. The reinforcing members are configured to extend downwardly through the interior of a valve skirt (not shown) to prevent eversion of the valve skirt after deployment to a heart valve. The reinforcing members **702** may include eyelets **707** at, for example, the ends of the reinforcing members **702** opposite the valve annulus **706**. It should be appreciated that the valve annulus **706** may include a plurality of folded loops (not shown) to enable the valve prosthesis, including the valve frame **700**, to be folded and collapsed for delivery through a catheter, as described in greater detail below.

The valve frame **700** may include a pair of hooks **704** (only one shown in FIG. **7**) for anchoring the prosthesis in position relative to the native heart valve. The hooks **704** may be slidable relative to the reinforcing members **702** between an unexposed, delivery position and an exposed, anchoring position.

For example, as shown in FIGS. **8a** and **8b**, each hook **704** may be slidable within a hollow reinforcing member **702**. The hollow reinforcing member **702** has an opening sized and configured to permit passage of an anchoring portion of the hook **704** curved, while retaining a base portion of the hook **704** that has a larger diameter than the hollow lumen of the reinforcing member. The hook **704** may be pushed out of the reinforcing member **702** by a pusher **709** that is an element of a delivery system which is operable by a user.

As shown in FIGS. **8c** and **8d**, each reinforcing member **702** may comprise two reinforcing elements **702a**, **702b**. The hook **704** is coupled to a sliding member **711** coupled to both reinforcing elements **702a**, **702b**. As shown, the hook **704** may be slidable relative to the reinforcing members **702** between an unexposed, delivery position and an exposed, anchoring position. For example, as shown in FIGS. **8c** and **8d**, each hook **704** may be slidable between a pair of reinforcing members **702a**, **702b**. The reinforcing members **702a**, **702b** may include a stop member (not shown) for preventing the hook from being slid off the reinforcing members **702a**, **702b**. The hook **704** may be pushed to the exposed, anchoring position by a pusher (not shown) that is an element of a delivery system which is operable by a user.

Referring now to FIG. **9**, an exemplary valve frame for a valve prosthesis in accordance with various aspects of the disclosure is described. As shown, a valve frame **1400** may include a valve annulus **1406** with a pair of reinforcing members **1402** extending therefrom. The reinforcing members **1402** may be configured to extend downwardly through the interior of a valve skirt (not shown) to prevent eversion of the valve skirt after deployment to a heart valve. The reinforcing members **1402** may be configured such that the ends of the reinforcing members **1402** distal to the valve annulus **1406** comprise hooks **1404** for anchoring the valve

prosthesis, including the valve frame **1400**, in position relative to the native heart valve.

FIG. **10** shows an illustrative configuration of an exemplary valve prosthesis in accordance with various aspects of the disclosure. As shown, a valve prosthesis **1500** may include a valve frame annulus **1506** comprising an expandable stent **1502**. According to various aspects, the stent may be self expanding or balloon inflated (e.g., plastically expandable), for example, to hold the valve prosthesis **1500** in position relative to the native heart valve. A valve skirt **1504** may extend from the expandable stent **1502**.

Referring now to FIG. **11**, an exemplary valve frame, or valve platform, configured to support a valve skirt of a valve prosthesis in accordance with various aspects of the present disclosure is described. Valve frame **1100** may comprise a valve annulus **1106**, for example, a D-shaped or oval annulus. According to various aspects, the valve frame **1100** may comprise a wire having a diameter of about 0.3 mm to about 1.0 mm, although other diameters may be selected depending upon the material chosen for the wire, in order to maintain a desired tensile strength of the valve frame **1100**, as well as its ability to be folded and delivered through a catheter at least in some embodiments. Any suitable material may optionally be used for the wire as long as it retains sufficient superelasticity and may also optionally be selected from any material described herein. For example, the valve frame **1100** may comprise a nickel titanium alloy (i.e., nitinol).

The valve frame **1100** may include a pair of reinforcement members **1101** extending from the valve annulus **1106**. The reinforcement members **1101** comprise a wire loop **1102** that extends from the valve annulus **1106** along an interior surface of a valve skirt (not shown) to a distal end of the valve skirt opposite the annulus **1106** along the distal edge of the valve skirt and back to the valve annulus **1106** along an interior surface of the valve skirt. The wire loop **1102** then extends away from the valve annulus **1106** along an interior surface of the valve skirt in a direction toward the distal end of the valve skirt, along the distal edge of the valve skirt, and back to the valve annulus **1106** along an interior surface of the valve skirt to complete the loop. The reinforcement members **1101** may thus prevent the valve skirt from evert-ing back into the atrium after deployment.

According to various aspects, the reinforcement members of the disclosure may be secured, for example, by suturing, to the valve skirt at any or all locations coextensive between the reinforcement member and the valve skirt.

As shown, a pair of curved, hooked extensions **1103** extend from the valve annulus **1106**. The extensions **1103** may include hooks **1104** at their ends opposite to the valve annulus **1106**. The extensions **1103** may also include eyelets (unnumbered) configured to receive a delivery cable (not shown) therethrough. Alternatively or additionally, the reinforcement members **1101** may include eyelets configured to receive a delivery cable.

FIGS. **12a-12d** show the prosthesis in its folded state and as it unfolds from a catheter. As shown in FIG. **12a**, a valve prosthesis **1200** (shown as the frame only for the purpose of description and without any intention of being limiting) is shown completely folded into a catheter **1202** (it is possible that valve prosthesis **1200** could be so completely collapsed that no portion is visible; however, for a clearer illustration, a part of valve prosthesis **1200** is shown slightly protruding from catheter **1202**).

In FIG. **12b**, valve prosthesis **1200** starts to emerge from catheter **1202**; in FIG. **12c**, valve prosthesis **1200** continues to emerge from catheter **1202**.

FIG. **12d** shows valve prosthesis **1200** completely emerged from catheter **1202** and ready for installation on the native valve annulus.

Referring now to FIGS. **13a-13d**, an illustrative configuration of an exemplary valve prosthesis in accordance with various aspects of the disclosure is depicted. As shown, a valve prosthesis **1300** may include a valve annulus **1306** such as, for example, a D-shaped annulus. The valve annulus **1306** may include a plurality of folded loops **1308**. The folded loops **1308** may enable the valve prosthesis **800**, including the valve frame, to be folded and collapsed for delivery through a catheter.

A first pair of reinforcing members **1302** may extend from the annulus **1306** through an interior of a valve skirt **1310** (FIG. **13d**). According to some aspects, the reinforcing members **1302** may extend from each end of the substantially straight portion of the D-shaped annulus **1306**. The extensions may also include eyelets **1307** configured to receive a delivery cable (not shown) therethrough. In some aspects, a pair of hooks **1304** extend from the valve annulus **1306** proximate the reinforcing members **1302**. According to various aspects, a third hook **1314** may be provided at a region of the curved portion of the D-shaped annulus **1306** that is furthest from the straight portion of the annulus **1306** or at the approximate midpoint of the curved portion. The hooks **1304**, **1314** may be configured to anchor the valve prosthesis **1300** in position at the native heart valve. The extensions **805** may include hooks **804** at its ends opposite to the valve annulus **806**.

A second pair of reinforcing members **1322** may extend from the valve annulus **1306** along the inner surface of the valve skirt **1310** (FIG. **13d**). According to some aspects, the second pair of reinforcing members **1322** may extend from regions of the curved portion of the D-shaped annulus **1306** in opposition to the first pair of reinforcing members **1312**.

Referring now to FIG. **13d**, the valve skirt **1310** may comprise a first skirt portion **1320** and a second skirt portion **1330**. When the valve skirt **1310** is urged to a closed position coaptation by the normal pressure gradient between the ventricle and atrium, the second pair of reinforcing members **1322** cause the second skirt member **1330** to close around the second pair of reinforcing members **1322**, thus giving the appearance from a top view of the valve prosthesis (FIG. **13d**) that the valve skirt **1310** has four leaflets instead of two valve skirt portions.

FIGS. **14a-14d** illustrate an exemplary valve skirt **1310** of a valve prosthesis in accordance with various aspects of the disclosure. FIGS. **14a** and **14d** illustrate the valve skirt **1310** in a relaxed yet substantially closed configuration, while FIGS. **14b** and **14c** illustrate the valve skirt **1310** in an expanded ex vivo configuration. As shown, the valve skirt **1310** includes a first skirt portion **1320** and a second skirt portion **1330**. As shown in FIGS. **14a** and **14d**, the region **1340** of the valve skirt **1310** where the first and second skirt portions **1320**, **1330** meet in a relaxed yet substantially closed configuration along a curved segment to form a D-shape similar to that of the valve annulus **1306**. Further, the D-shaped annulus **1306** and D-shaped closure region **1340** are similar to those of the native heart valve.

Referring now to FIG. **15**, an exemplary valve prosthesis in accordance with various aspects of the disclosure is described. As shown, the exemplary prosthesis **1700** can be configured from two wires **1701**, **1702** twisted and wound together. As illustrated, the first wire **1701** may define a portion of the valve annulus **1706** and at least one folded loop **1708** as well as one or more hooks (**1314**) at the apex of the curved part of the D-shape. The second wire **1702** may



## 11

define a further portion of the valve annulus **1706**, one or more hooks **1704**, and one or more reinforcing members **1702**.

FIGS. **16** and **17** show portion of an exemplary delivery system for delivering and deploying a valve prosthesis in accordance with various aspects of the disclosure. FIG. **16** illustrates a delivery system **1600** including an outer sheath **2100**, two inner sheaths **2200**, and two cables or rods **2300**. The inner sheaths **2200** may be disposed in the outer sheath **2100** and may be exposed, for example, by pulling the outer sheath **2100** in a proximal direction relative to the inner sheaths **2200**. Similarly, one cable or rod **2300** may be disposed in each of the inner sheaths **2200**. The cable or rod **2300** may be exposed, for example, by pulling the inner sheath **2200** in a proximal direction relative to the cable or rod **2300**. According to various aspects, the cable or rods **2300** may be coupled to one or more reinforcing members, hooks, and/or extensions of a valve prosthesis, for example, by passing through eyelets provided on the one or more reinforcing members, hooks, and/or extensions of the valve prosthesis. The cables or rods **2300** can operate as pushers for moving hooks from a withdrawn position to an anchoring position in accordance with various aspects of the disclosure.

Referring now to FIG. **17**, any of the aforementioned hooks used for anchoring the valve prosthesis to tissue can be folded for delivery into a tubular sheath **2400**. The various hooks can be pulled into the sheath **2400** by passing a wire or cable **2410** through an eyelet **2420** of the hook **2430** and pulling the hook **2430** into the sheath **2400** with the wire or cable **2410**. The sheath **2400** can be retracted to deploy the hook **2430** upon delivery.

FIG. **18** illustrates an exemplary tool, for example, measuring frame **1800**, for use with an exemplary method for delivering a valve prosthesis in accordance with various aspects of the disclosure. The measuring frame **1800** includes a single leg **1810** extending from an annulus **1820**. The annulus **1820** may include markings (not shown) to help size the native valve annulus as described below. Use of the tool is described in connection with the method illustrated in FIG. **19** below.

Referring now to FIG. **19**, an exemplary pre-delivery procedure is described with respect to the provided flow chart. The pre-delivery process begins at step **1900** where a sheath containing the measuring frame **1800** is inserted into the left atrium from the left ventricle. The process continues to step **1910** where the measuring frame **1800** is advanced from the sheath. Then, in step **1920**, the measuring frame **1800** is deployed such that the leg **1810** is at one commissure of a heart valve. The process proceeds to step **1930**.

In step **1930**, the user observes which one of various markers, for example, radiopaque markers, on the annulus **1820** aligns with the second commissure of the heart valve. Next, in step **1940**, the user notes the size of the annulus relative to the measuring frame **1800**. The process concludes in step **1950** where the measuring frame **1800** is retracted into the sheath and the correct size and configuration for a valve prosthesis is selected.

FIG. **20** is a flow chart showing an exemplary method for delivering a valve prosthesis in accordance with various aspects of the disclosure. The method begins at step **2000** where a delivery system is inserted into the left atrium from the left ventricle. The process proceeds to step **2010** where the outer sheath **2100** is pulled proximally until a valve annulus is fully deployed. The process then goes to step **2020**.

## 12

In step **2020**, the delivery system is rotated until a first leg of the valve prosthesis is positioned opposite to one commissure of the heart valve. The process continues to step **2030** where the inner sheath **2200** associated with the first leg is retracted until the first leg is positioned at the commissure. The process then proceeds to step **2040** where the inner sheath **2200** associated with the second leg is retracted until the second leg is positioned at the second commissure. The process continues to step **2050**.

Next in step **2050**, the entire delivery system **1600** is retracted proximally until the valve annulus is positioned at the native valve annulus. Then, in step **2060**, the hooks are activated either by being pushed into an anchoring position or by retraction of a tubular sheath enclosed the hooks. The process continues to step **2070** where the device is tested for leakage by observing the flow across the valve using such means as ultrasound. For example, various pre-treatment and post-treatment diagnostic techniques are available for assessing valvular sufficiency and/or leakage, such as transthoracic, echo-Doppler based echocardiography (TTE), and transesophageal, echo-Doppler based echocardiography (TEE); cardiac catheterization with radiopaque dye; stress tests; and other known techniques. The process then concludes at step **2080** where the cables **2300** are withdrawn to release the reinforcing members.

It would be appreciated by persons skilled in the art that radiopaque markers can be incorporated into the valve prosthesis such as by the use of radiopaque material, for example, tantalum, platinum, and/or gold, which may be physically secured to the valve frame such as by collars crimped or welded on the frame at various locations along the annulus and/or the skirt and/or at the distal ends of the reinforcement members. Alternatively, radiopaque markers can be practice by use of gold thread woven into desired locations of the valve skirt.

It will be apparent to those skilled in the art that various modifications and variations can be made to the heart valve prosthesis and method of delivery of the present disclosure without departing from the scope of the invention. Other embodiments of the invention will be apparent to those skilled in the art from consideration of the specification and practice of the invention disclosed herein. It is intended that the specification and examples be considered as exemplary only.

What is claimed is:

1. A prosthetic cardiac valve support device comprising: an annular support element configured for positioning at or near a native heart valve annulus; at least two valve support extensions shaped to extend through commissures of the native heart valve for supporting a flexible valve; and at least two anchoring extensions: attached at one end to said annular support element, and extending in an opposite direction towards an unattached end; in a form of hooks shaped for anchoring said annular support element to tissue; all of the anchoring extensions being adapted to extend through commissures of a native heart valve without interfering with movement of native heart valve leaflets; and the anchoring extensions shaped to prevent said annular support element from shifting upstream relative to the native heart valve annulus.
2. The device of claim 1 in which said anchoring extensions are shaped to extend below an annulus of the native heart valve.

## 13

3. The device of claim 1 in which said anchoring extensions are attached to approximately opposing edges of the annular support element.

4. The device of claim 1 in which said anchoring extensions are attached to said annular support element at non-opposing positions around said annular support element, conforming to positions of commissures of the native heart valve.

5. The device of claim 1 in which all of said anchoring extensions are shaped to extend through commissures of a native heart valve and extend radially outward from a valve center, further than native heart valve leaflets, without interfering with closing of native heart valve leaflets.

6. The device of claim 1 in which said valve support extensions are connected to each other at tips of the valve support extensions distal from an attachment of said support extensions to said annular support element.

7. The device of claim 1 in which said anchoring extensions comprises a loop at a tip of said anchoring extensions.

8. The device of claim 1, wherein a part of said annular support element is a D-shaped annulus element conforming to a shape of a mitral valve annulus.

9. The device of claim 1, wherein said annular support element is elastically deformable.

10. The device of claim 1, in which said unattached end of said anchoring extensions are shaped to extend through the native heart valve annulus and are curved in a direction from a center of the native heart valve annulus toward heart walls.

11. A method for providing support for a cardiac valve comprising:

placing an annular support element for a cardiac valve upstream of a native heart valve annulus;

extending at least two valve support extensions shaped to extend through commissures of the native heart valve for supporting a flexible valve;

extending at least two anchoring extensions:

## 14

attached at one end to said annular support element and extending in an opposite direction towards an unattached end;

in a form of hooks shaped for anchoring said annular support element to tissue; and

all of the anchoring extensions being adapted to extend through commissures of a native heart valve without interfering with movement of native heart valve leaflets,

so as to prevent said annular support element from shifting upstream relative to the native heart valve annulus.

12. The method of claim 11 in which the anchoring extensions are anchored in tissue.

13. The method of claim 11 in which the anchoring extensions extend below an annulus of the native heart valve.

14. The method of claim 11 in which said anchoring extensions are extended through commissures of a native heart valve without interfering with movement of native heart valve leaflets.

15. The method of claim 11 in which all of said anchoring extensions are extended through commissures of a native heart valve and extended radially outward from a valve center, further than native heart valve leaflets without interfering with closing of native heart valve leaflets.

16. The method of claim 11 in which the cardiac valve comprises a flexible valve, and further comprising extending at least two valve support extensions for supporting said flexible valve through commissures of the native heart valve.

17. The method of claim 11 in which said placing said annular support element upstream of a native heart valve annulus comprises expanding said annular support element radially like a stent.

\* \* \* \* \*