



US0D1032012S

(12) **United States Design Patent**
Moriwake et al.

(10) **Patent No.:** **US D1,032,012 S**

(45) **Date of Patent:** **** Jun. 18, 2024**

- (54) **BIOCHEMICAL ANALYZER**
- (71) Applicant: **PHC Holdings Corporation**, Tokyo (JP)
- (72) Inventors: **Yuta Moriwake**, Ehime (JP); **Kouji Yukikado**, Ehime (JP)
- (73) Assignee: **PHC HOLDINGS CORPORATION**, Tokyo (JP)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/802,165**
- (22) Filed: **Aug. 3, 2021**

- D644,544 S 9/2011 Yukikado
- D644,546 S 9/2011 Yukikado
- D665,917 S * 8/2012 TerMaat D24/216
- D730,535 S 5/2015 Gutmann et al.
- D735,878 S * 8/2015 Chang D24/216
- D848,880 S * 5/2019 Smith D24/234
- D883,510 S * 5/2020 Neuman D24/216
- D888,267 S * 6/2020 Salomon D24/216

(Continued)

FOREIGN PATENT DOCUMENTS

- CA 177948 * 7/2018
- CN 3365879 * 4/2004

(Continued)

OTHER PUBLICATIONS

“BioWorld: 10x Genomics.” Found online Mar. 13, 2024 at bioworld.com. Reference dated Jul. 14, 2021. Retrieved from https://www.bioworld.com/keywords/19040-10x-genomics-inc.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton
Assistant Examiner — Elizabeth S Struble
(74) *Attorney, Agent, or Firm* — Crowell & Moring LLP

(57) **CLAIM**

The ornamental design for a biochemical analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view from front side of a biochemical analyzer showing our new design;
FIG. 2 is a perspective view from rear side thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a top plan view thereof;
FIG. 6 is a bottom plan view thereof;
FIG. 7 is a left side view thereof; and,
FIG. 8 is a right side view thereof.

1 Claim, 4 Drawing Sheets

(30) **Foreign Application Priority Data**

Apr. 21, 2021 (JP) 2021-008503 D

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**

USPC **D24/216**

(58) **Field of Classification Search**

USPC D24/107, 108, 186, 216, 223, 224, 231, D24/232



CPC A61J 1/2086; A61J 1/2096; A61J 1/2089; A61B 5/0006; A61B 5/0205; B01L 3/021; B01L 3/058; B01L 3/52; B01L 3/5085; B01L 2200/16; B01L 3/5023; G01N 21/78; G01N 1/38; G01N 21/6428; G01N 33/50; G01N 33/49; C12M 23/08; C12M 23/14; C12M 23/44; C12M 23/46; C12M 23/48; C12M 23/58

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D381,749 S * 7/1997 Lawrence D24/186
- D598,551 S * 8/2009 Miwa D24/186
- D607,569 S 1/2010 Yukikado et al.

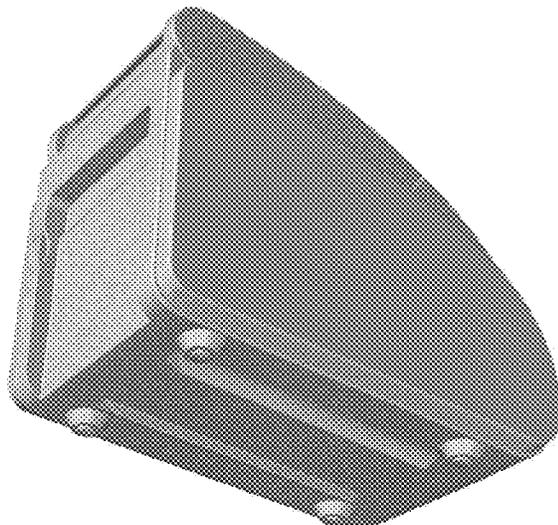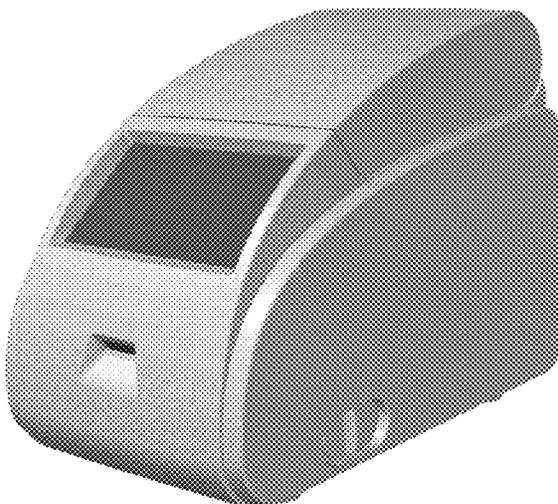

(56)

References Cited

U.S. PATENT DOCUMENTS

D927,723 S * 8/2021 Nelsen D24/216
 D932,047 S * 9/2021 Hölbl D24/216
 D985,797 S * 5/2023 André D24/232
 11,921,104 B2 * 3/2024 Barry, Jr. G01N 21/6458
 2013/0004954 A1 * 1/2013 Bianchessi G01N 21/6428
 435/6.12
 2018/0169658 A1 * 6/2018 Lei B01L 3/5085

FOREIGN PATENT DOCUMENTS

CN 306665045 * 7/2021
 CN 307758953 * 12/2022
 JP D1373600 S 11/2009
 JP 1400050 S 11/2010
 JP D1400049 S 11/2010
 JP 1549224 S 5/2016

OTHER PUBLICATIONS

“Seamaty: Comparison of Semi-auto, Auto and Dry Biochemisry Machine.” Found online Mar. 28, 2024. Reference dated Oct. 11, 2022. Retrieved from <https://en.seamaty.com/index.php?s=/sys/533.html>.*

“Bloomberg: Abbott Launces 5-minute Virus Test for Use Almost Anywhere.” Found online Oct. 30, 2023 at bloomberg.com. Reference dated Mar. 27, 2020. Retrieved from <https://www.bloomberg.com/news/articles/2020-03-27/abbott-launches-5-minute-covid-19-test-for-use-almost-anywhere#xj4y7vzkg>.*

“Fujifilm Emea: Immuno AG1.” Found online Oct. 30, 2023 at youtube.com. Reference dated Sep. 15, 2017. Retrieved from <https://www.youtube.com/watch?v=NQjgiPxALZg>.*

* cited by examiner

FIG.1

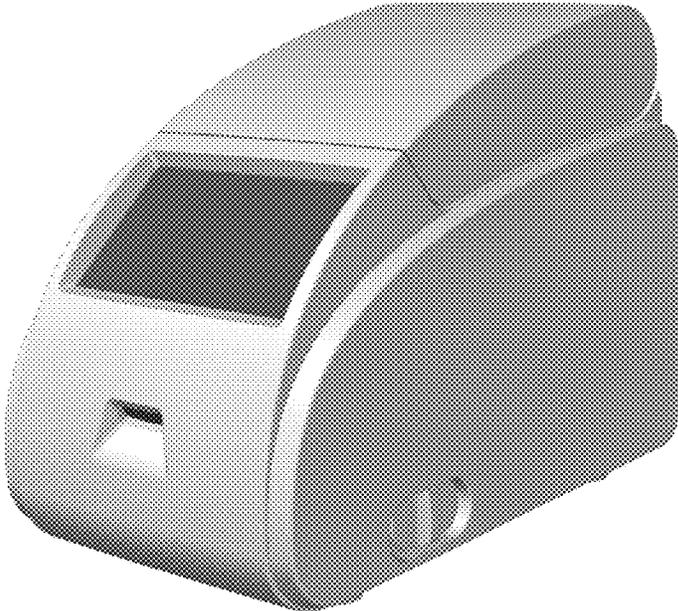


FIG.2

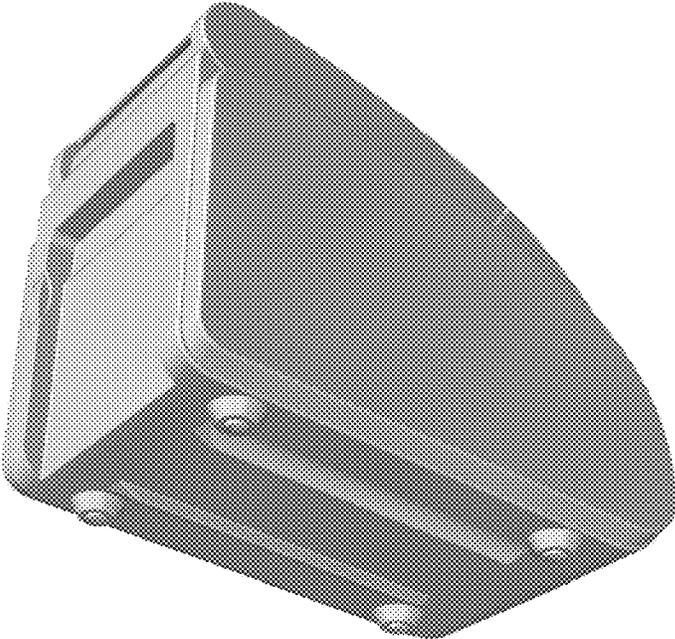


FIG.3

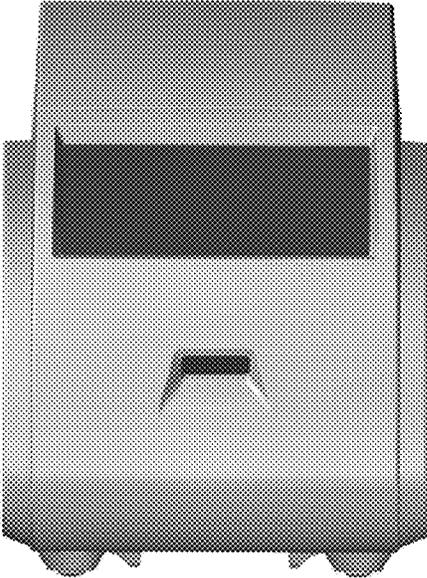


FIG.4

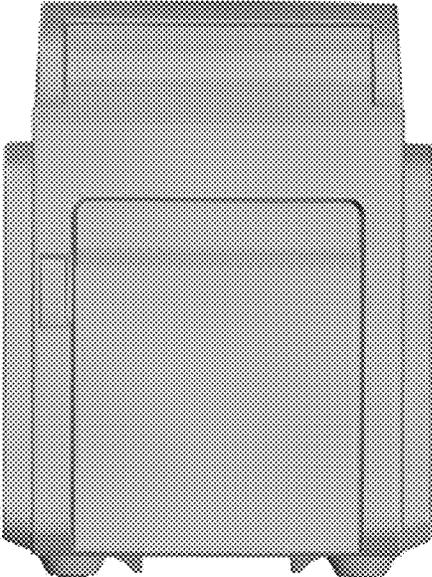


FIG.5

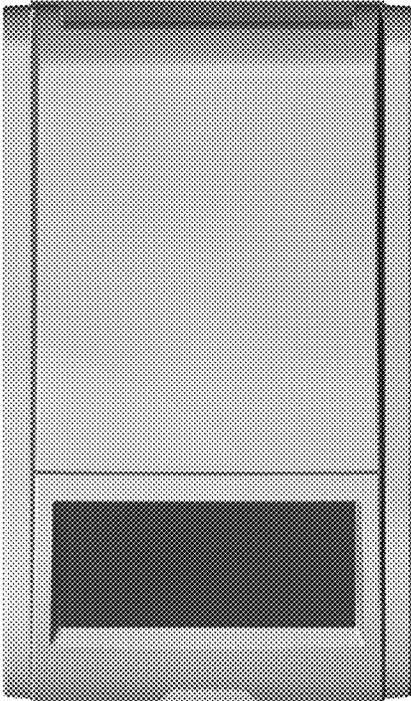


FIG.6

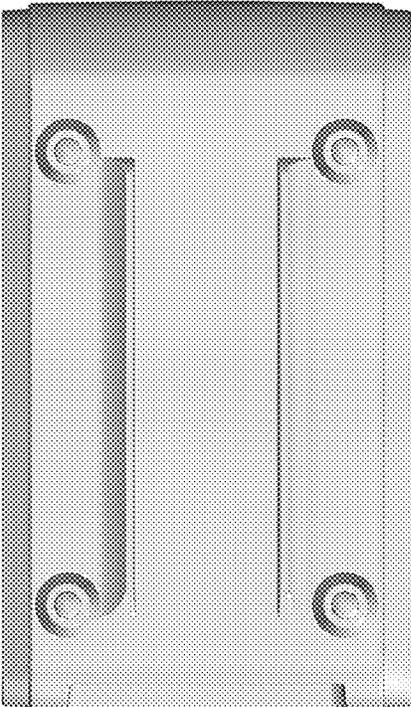


FIG.7

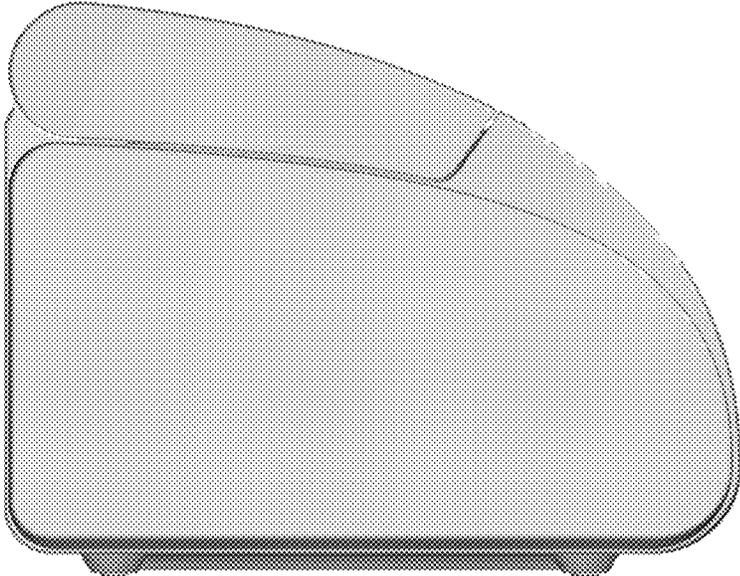


FIG.8

