



- (51) International Patent Classification:  
A61F 2/44 (2006.01) A61F 2/28 (2006.01)
- (21) International Application Number:  
PCT/US2016/014100
- (22) International Filing Date:  
20 January 2016 (20.01.2016)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
14/600,617 20 January 2015 (20.01.2015) US
- (71) Applicant: OUROBOROS MEDICAL, INC. [US/US];  
47757 Fremont Blvd., Fremont, CA 94538 (US).
- (72) Inventors; and
- (71) Applicants : TO, John [US/US]; 36514 Dijon Drive, Newark, CA 94560 (US). FLYNN, John, J. [US/US]; 136 Panoramic Way, Walnut Creek, CA 94595 (US).
- (74) Agent: BOYER, Brian, S.; Syndicated Law PC, 503 Seaport Court, Suite 102, Redwood City, CA 94063 (US).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,

BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).


**Published:**

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))



WO 2016/118608 A1

(54) Title: STABILIZED INTERVERTEBRAL SCAFFOLDING SYSTEMS

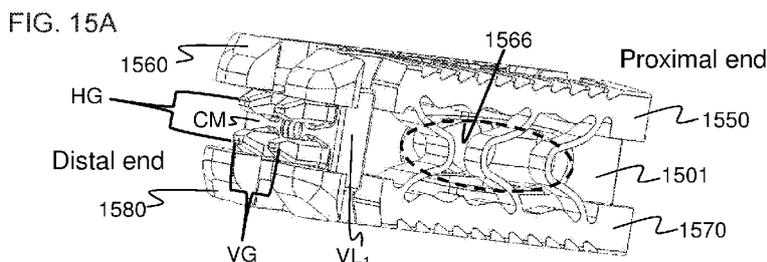

(57) Abstract: An intervertebral scaffolding system is provided having a central beam having a proximal portion having an end, a grafting portion having a top and a bottom, a distal portion having an end, a central beam axis, a graft distribution channel having an entry port at the end of the proximal portion, a top exit port at the top of the grafting portion, and a bottom exit port at the bottom of the grafting portion. These systems can also include a laterovertically-expanding frame operable for a reversible collapse from an expanded state into a collapsed state. The expanded state, for example, can be configured to have an open graft distribution window that at least substantially closes upon the reversible collapse.

## STABILIZED INTERVERTEBRAL SCAFFOLDING SYSTEMS

JOHN TO  
JOHN FLYNN

## BACKGROUND

Field of the Invention

[0002] The teachings herein are directed to intervertebral scaffolding systems having a stabilizer for stabilizing and/or retaining support beams upon expansion of the scaffolding in an intervertebral disc space.

Description of the Related Art

[0003] Bone grafts are used in spinal fusion, for example, which is a technique used to stabilize the spinal bones, or vertebrae, and a goal is to create a solid bridge of bone between two or more vertebrae. The fusion process includes “arthrodesis”, which can be thought of as the mending or welding together of two bones in a spinal joint space, much like a broken arm or leg healing in a cast. Spinal fusion may be recommended for a variety of conditions that might include, for example, a spondylolisthesis, a degenerative disc disease, a recurrent disc herniation, or perhaps to correct a prior surgery.

[0004] Bone graft material is introduced for fusion and a fusion cage can be inserted to help support the disc space during the fusion process. In fact, fusion cages are frequently used in such procedures to support and stabilize the disc space until bone graft unites the bone of the opposing vertebral endplates in the disc space. A transforaminal lumbar interbody fusion (TLIF), for example, involves placement of posterior instrumentation (screws and rods) into the spine, and the fusion cage loaded with bone graft can be inserted into the disc space. Bone graft material can be pre-packed in the disc space or packed after the cage is inserted. TLIF can be used to facilitate stability in the front and back parts of the lumbar spine promoting interbody fusion in the anterior portion of the spine. Fusion in this region

can be beneficial, because the anterior interbody space includes an increased area for bone to heal, as well as to handle increased forces that are distributed through this area.

[0005] Unfortunately, therein lies a problem solved by the teachings provided herein. Currently available systems can be problematic in that the methods of introducing the fusion cage and bone graft material leaves pockets in regions of the intervertebral space that are not filled with bone graft material, regions in which fusion is desired for structural support. These pockets can create a premature failure of the fused intervertebral space due to forces that are distributed through the regions containing the pockets, for example, when the patient stands and walks.

[0006] Traditional fusion cages, such as the Medtronic CAPSTONE cage, are designed to be oversized relative to the disc space to distract the disc space as the entire cage is inserted. However, this makes it difficult to insert and position properly. In response to the problem, the art has developed a number of new fusion cages, such as the Globus CALIBER cage which can be inserted at a low height and expanded vertically to distract the disc space. Unfortunately, these types of devices have the typical graft distribution problem discussed above, in that they do not provide a path for bone graft to be inserted and fill in the space surrounding the cage or within the cage. They have other problems as well, including that the annulotomy must be large to accommodate a large enough cage for stability, and this large opening necessitates more trauma to the patient. Moreover, they can also create the additional problem of “backout”, in that they cannot expand laterally beyond the annulotomy to increase the lateral footprint of the cage relative to lateral dimension of the annulotomy. Since it takes several months for the fusion to occur to completion in a patient, the devices have plenty of time to work their way out of the space through the large annulotomy.

[0007] Scaffolding systems may also suffer a lack of stability and/or a lack of a retention of structural components in a desired expansion configuration in the intervertebral space. As such, a multi-component scaffolding system, for example, can benefit from an improved design that adds stability through, for example, (i) enhancing the amount of contact between the scaffolding components upon expansion; and/or (ii) limiting the amount of expansion, or relative movement, that can occur between components upon expansion, or after expansion, in the intervertebral space. Such design considerations can, for example, address the problems of overexpansion of one component relative to another due to, for example, variable stresses that might occur in the intervertebral space upon expansion or

after expansion, stresses which can result in at least partial failure of the scaffolding system in the intervertebral space.

[0008] Accordingly, and for at least the above reasons, those of skill in the art will appreciate bone graft distribution systems that facilitate an improved distribution of graft material throughout the intervertebral space. Such systems are provided herein, the systems configured to (i) effectively distribute bone graft material both from the system, and around the system, to improve the strength and integrity of a fusion; (ii) reduce or eliminate the problem of failures resulting from a poor bone graft distribution; (iii) have a small maximum dimension in a collapsed state for a low-profile insertion into the annulus in a minimally-invasive manner, whether using only a unilateral approach or a bilateral approach; (iv) laterally expand within the intervertebral space to avoid backout of the system through the annulotomy; (v) vertically expand for distraction of the intervertebral space; (vi) provide an expansion in the intervertebral space without contracting the system in length to maintain a large footprint and an anterior position adjacent to the inner, anterior annulus wall, distributing load over a larger area, anteriorly, against the endplates; (vii) and, incorporate a stabilizer for stabilizing and/or retaining support beams upon expansion of the scaffolding in an intervertebral disc space..

## SUMMARY

[0009] The teachings herein are directed to intervertebral scaffolding systems having a stabilizer for stabilizing and/or retaining support beams upon expansion of the scaffolding in an intervertebral disc space. As such, the teachings herein are generally directed to an intervertebral scaffolding system.

[00010] The systems provided herein can comprise, for example, a central beam having a central beam axis; a proximal portion and a distal portion; a top surface with a first top-lateral surface and a second top-lateral surface; a bottom surface with a first bottom-lateral surface and a second bottom-lateral surface; a first side surface with a first top-side surface and a first bottom-side surface; and, a second side surface with a second top-side surface and a second bottom-side surface. The systems can also comprise a laterovertically-expanding frame configured for operably contacting the central beam to create an intervertebral scaffolding system *in vivo*. The frame can have a collapsed state and an expanded state, the expanded state operably contacting with the central beam in the

intervertebral space; a proximal portion having an end, a distal portion having an end, and a central frame axis of the expanded state.

[00011] In some embodiments, the frame can be constructed to have a first top beam including a proximal portion having an end and a distal portion having an end, the first top beam configured for contacting the first top-lateral surface of the central beam and the first top-side surface of the central beam in the expanded state, a central axis of the first top beam at least substantially on (i) a top plane containing the central axis of the first top beam and a central axis of a second top beam and (ii) a first side plane containing the central axis of the first top beam and a central axis of a first bottom beam; the second top beam including a proximal portion having an end and a distal portion having an end, the second top beam configured for contacting the second top-lateral surface of the central beam and the second top-side surface of the central beam in the expanded state, the central axis of the second top beam at least substantially on (i) the top plane and (ii) a second side plane containing the central axis of the second top beam and a central axis of a second bottom beam; the first bottom beam including a proximal portion having an end and a distal portion having an end, the first bottom beam configured for contacting the first bottom-lateral surface of the central beam and the first bottom-side surface of the central beam in the expanded state, the central axis of the first bottom beam at least substantially on (i) a bottom plane containing the central axis of the first bottom beam and the central axis of the second top beam and (ii) the first side plane; the second bottom beam including a proximal portion having an end and a distal region having an end, the second bottom beam configured for contacting the second bottom-lateral surface of the central beam and the second bottom-side surface of the central beam in the expanded state, the central axis of the second bottom beam being at least substantially on (i) the bottom plane and (ii) a second side plane containing the central axis of the second bottom beam and the central axis of the second top beam.

[00012] The frame can also be constructed, for example, to have a plurality of top connector elements configured to expandably connect the first top beam to the second top beam, the expanding consisting of a flexing at least substantially on the top plane; a plurality of bottom connector elements configured to expandably connect the first bottom beam to the second bottom beam, the expanding consisting of a flexing at least substantially on the bottom plane; a plurality of first side connector elements configured to expandably connect the first top beam to the first bottom beam, the expanding consisting of a flexing at least

substantially on the first side plane; and, a plurality of second side connector elements configured to expandably connect the second top beam to the second bottom beam, the expanding consisting of a flexing at least substantially on the second side plane

[00013] In some embodiments, the systems include a stabilizer that slidably engages with the distal region of the first top beam, the first bottom beam, the second top beam, the second bottom beam, or a combination thereof. The stabilizer can be configured for retaining the first top beam, the first bottom beam, the second top beam, the second bottom beam, or the combination thereof, from a lateral movement that exceeds the expanded state.

[00014] And, in some embodiments, the framing can be configured for engaging with the central beam *in vivo* to support the framing in the expanded state. Moreover, the connector elements can be struts configured to have a cross-sectional aspect ratio of longitudinal thickness to transverse thickness ranging from 1:2 to 1:8, adapted to maintain structural stiffness in the laterover vertically expanding frame in a direction perpendicular to the central frame axis of the expanded state of the frame.

[00015] The stabilizer can be in an X-configuration. In some embodiments, the X-configuration can have a first top leg for slidably-engaging with the first top beam at an angle  $\Theta_{1T}$  with the lateral movement of the first top beam, first bottom leg for slidably engaging with the first bottom beam at an angle  $\Theta_{1B}$  with the lateral movement of the first bottom beam, a second top leg for slidably engaging with the second top beam at an angle  $\Theta_{2T}$  with the lateral movement of the second top beam, and a second bottom leg for slidably engaging with the second bottom beam at an angle  $\Theta_{2B}$  with the lateral movement of the second bottom beam. In some embodiments, each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$ , respectively, provide a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state. In some embodiments, the stabilizer further comprises a point of attachment for releasably attaching a guidewire for guiding the central beam into the laterover vertically expanding frame. And, in some embodiments, the first top leg, the first bottom leg, the second top leg, and the second bottom leg converge to form a hub having a point of attachment for releasably attaching a guidewire for guiding the central beam into the laterover vertically expanding frame.

[00016] The stabilizer can be in an H-configuration. The H-configuration can have a first vertical leg, a second vertical leg, and a cross-member that connects the first vertical leg at

least substantially parallel to the second vertical leg, the first vertical leg including a retaining surface for engaging with the first top beam and the first bottom beam, the second vertical leg including a retaining surface for engaging with the second top beam and the second bottom beam, and the cross member providing a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state. In some embodiments, the central beam has a horizontal groove configured complementary to the cross-member of the stabilizer, and the horizontal groove of the central beam slidably connects with the cross-member in the expanded state. In some embodiments, the cross-member further comprises a vertical support member and the central beam has a vertical groove configured complementary to the vertical support member of the stabilizer, and the vertical groove of the central beam slidably connects with the vertical support member in the expanded state. In some embodiments, the stabilizer further comprises a point of attachment for releasably attaching a guidewire adapted for guiding the central beam into the laterover vertically expanding frame. And, in some embodiments, cross-member includes a first pillar and a second pillar that operably connect at a hub that has a point of attachment for releasably attaching a guidewire for guiding the central beam into the laterover vertically expanding frame.

[00017] In some embodiments, the systems are bone graft distribution systems. In these embodiments, the central beam can further comprise a grafting port. Likewise the expanding frame can open bone graft distribution windows on the top, the bottom, the sides, or a combination thereof, upon expansion.

[00018] In some embodiments, the frame can be formed monolithically. In these embodiments, each plurality connector elements can be struts; wherein, the top struts are configured monolithically integral to the first top beam and the second top beam; and, the bottom struts are configured monolithically integral to the first bottom beam and the second bottom beam. The top struts and the bottom struts of the laterover vertically-expanding frame can each be configured to open a graft distribution window upon expansion, expanding from the first top beam to the second top beam, the first top beam to the first bottom beam, the second top beam to the second bottom beam, or the first bottom beam to the second bottom beam. Likewise, in some embodiments, the top connector struts are configured monolithically integral to the first top beam and the second top beam; and, the bottom struts are configured monolithically integral to the first bottom beam and the second bottom beam; the first side struts are configured monolithically integral to the first top beam and the first

bottom beam; and, the second side struts are configured monolithically integral to the second top beam and the second bottom beam. It should be appreciated that, in such embodiments, the top, bottom, first side, and second side of the laterover vertically-expanding frame can form a monolithically integral frame.

[00019] The teachings are also directed to a method of fusing an intervertebral space. The methods can use the scaffolding systems taught herein. For example, the methods can include creating a point of entry into an intervertebral disc, the intervertebral disc having a nucleus pulposus surrounded by an annulus fibrosis; removing the nucleus pulposus from within the intervertebral disc through the point of entry, leaving the intervertebral space for expansion of the scaffolding system of claim 1 within the annulus fibrosis, the intervertebral space having a top vertebral plate and a bottom vertebral plate; inserting the laterover vertically expanding frame in the collapsed state through the point of entry into the intervertebral space; inserting the central beam into the frame to form the scaffolding system; and, adding a grafting material to the intervertebral space.

[00020] The step of creating the point of entry can comprise creating a lateral dimension of the point of entry ranging from about 5 mm to about 15 mm, and the amount of lateral expansion can be selected to exceed the lateral dimension of the point of entry. The step of expanding can include expanding the laterover vertically expanding frame laterally to a width that exceeds the width of the point of entry; and, inserting the central beam to expand the laterover vertically expanding frame vertically to support the frame in the expanded state. The step of inserting the central beam into the laterover vertically expanding frame includes engaging a means for preventing the central beam from backing out of the laterover vertically-expanding frame after the expanding.

[00021] The teachings are also directed to a kit comprising a scaffolding system taught herein. The systems can include a cannula for inserting the scaffolding system into the intervertebral space; and, a guidewire adapted for guiding the central beam into the laterover vertically expanding frame.

#### BRIEF DESCRIPTION OF THE FIGURES

[00022] FIGs. 1A-1I illustrate components of the graft distribution system, according to some embodiments.

[00023] FIGs. 2A-2F illustrate a method of using a bidirectionally-expandable cage, according to some embodiments.

[00024] FIGs. 3A-3D illustrate a bidirectionally-expandable cage for fusing an intervertebral disc space, according to some embodiments.

[00025] FIGs. 4A and 4B illustrate collapsed and expanded views of a bidirectionally-expandable cage having a bone graft window on each wall for fusing an intervertebral disc space, according to some embodiments.

[00026] FIGs. 5A-5D illustrate system for fusing an intervertebral disc space, according to some embodiments.

[00027] FIG. 6 is a diagram of a method of using a bidirectionally-expandable cage, according to some embodiments.

[00028] FIGs. 7A-7F illustrate some additional features of graft distribution systems, according to some embodiments.

[00029] FIGs. 8A-8D illustrate components of a graft distribution kit, according to some embodiments.

[00030] FIGs. 9A-9C illustrate the expansion of a laterover vertically-expandable frame in an intervertebral space, according to some embodiments.

[00031] FIGs. 10A-10C illustrate profiles of an expanded graft distribution system to highlight the exit ports and bone graft windows, according to some embodiments.

[00032] FIGs. 11A and 11B compare an illustration of the graft distribution in place to a test placement in a cadaver to show relative size, according to some embodiments.

[00033] FIGs. 12A-12C show x-rays of a placement in a cadaver, according to some embodiments.

[00034] FIGs. 13A-13D show orientations of the first top beam relative to the second top beam, first bottom beam relative to the second bottom beam, first top beam relative to the first bottom beam, and the second top beam relative to the second bottom beam, according to some embodiments.

[00035] FIGs. 14A-14D illustrate components of a system having a stabilizer, wherein the stabilizer is in an X-configuration, according to some embodiments.

[00036] FIGs. 15A-15D illustrate components of a system having a stabilizer, wherein the stabilizer is in an H-configuration, according to some embodiments.

#### DETAILED DESCRIPTION OF THE INVENTION

[00037] The teachings herein are directed to intervertebral scaffolding systems having a stabilizer for stabilizing and/or retaining support beams upon expansion of the scaffolding in an intervertebral disc space. The systems can have, for example, a central beam having a proximal portion having an end, a grafting portion having a top and a bottom, a distal portion having an end, a central beam axis, a graft distribution channel having an entry port at the end of the proximal portion, a top exit port at the top of the grafting portion, and a bottom exit port at the bottom of the grafting portion. These systems can also include a laterover vertically-expanding frame having a lumen, a first top beam, a second top beam, a first bottom beam, and a second bottom beam, each having a proximal portion and a distal portion, and each operably connected to each other at their respective proximal portions and distal portions with connector elements to form the laterover vertically-expanding frame that is operable for a reversible collapse from an expanded state into a collapsed state. The expanded state, for example, can be configured to have an open graft distribution window that at least substantially closes upon the reversible collapse. In these embodiments, the laterover vertically-expanding frame is adapted for receiving an insertion of the central beam to form the graft distribution system.

[00038] In some embodiments, the systems can also include a laterover vertically-expanding frame having a first top beam, a second top beam, a first bottom beam, and a second bottom beam; wherein, the beams are in an at least substantially parallel arrangement with each other, each having a proximal portion, a grafting portion, and a distal portion, and each operably connected to each other at their respective proximal portions and distal portions to form the laterover vertically-expanding frame in a square, cylindrical shape that is operable for a reversible collapse from an expanded state into a collapsed state. The expanded state, for example, can be configured to have an open graft distribution window that at least substantially closes upon the reversible collapse. In these embodiments, the laterover vertically-expanding frame is adapted for receiving an insertion of the central beam to form the graft distribution system.

[00039] The term "subject" and "patient" can be used interchangeably in some embodiments and refer to an animal such as a mammal including, but not limited to, non-

primates such as, for example, a cow, pig, horse, cat, dog; and primates such as, for example, a monkey or a human. As such, the terms “subject” and “patient” can also be applied to non-human biologic applications including, but not limited to, veterinary, companion animals, commercial livestock, and the like. Moreover, terms of degree are used herein to provide relative relationships between the position and/or movements of components of the systems taught herein. For example, the phrase “at least substantially parallel” is used to refer to a position of one component relative to another. An axis that is at least substantially parallel to another axis refers to an orientation that is intended, for all practical purposes to be parallel, but it is understood that this is just a convenient reference and that there can be variations due to stresses internal to the system and imperfections in the devices and systems. Likewise, the phrase “at least substantially on a...plane” refers to an orientation or movement that is intended, for all practical purposes to be on or near the plane as a convenient measure of the orientation or movement, but it is understood that this is just a convenient reference and that there can be variations due to stresses internal to the system and imperfections in the devices and systems. Likewise, the phrase “at least substantially coincident” refers to an orientation or movement that is intended, for all practical purposes to be on or near, for example, an axis or a plane as a convenient measure of the orientation or movement, but it is understood that this is just a convenient reference and that there can be variations due to stresses internal to the system and imperfections in the devices and systems.

[00040] FIGs. 1A-1I illustrate components of the system, according to some embodiments. As shown in FIG. 1A, the graft distribution systems 100 can have a central beam 101 with a central beam axis 105, a graft distribution channel with an entry port 135 in fluid communication with a top exit port 140, and a bottom exit port 141. The central beam 101 can also have a proximal portion 111 having and end with the entry port 135, a grafting portion 112 having the top exit port 140 and the bottom exit port 141, and a distal portion (not shown). The central beam 101 can also be sized to have a transverse cross-section 110 having a maximum dimension ranging from 5 mm to 15 mm for placing the central beam 101 into an intervertebral space through an annular opening having a maximum lateral dimension ranging from 5 mm to 15 mm, the intervertebral space having a top vertebral plate and a bottom vertebral plate. The central beam 101 can also have a top surface 115 with a first top-lateral surface 117 and a second top-lateral surface 119, a bottom surface 120 with a first bottom-lateral surface 122 and a second bottom-lateral surface 124, a first side surface 125 with a first top-side surface 127 and a first bottom-side surface 129, and a

second side surface 130 with a second top-side surface 132 and a second bottom-side surface 134.

[00041] In some embodiments, the central beam can have transverse cross-sectional lateral dimension ranging from about 5mm to about 15mm. In some embodiments, the vertical dimension of the central beam can range from about 4mm to about 12mm, about 5mm to about 11mm, about 6mm to about 10mm, and about 7mm to about 9mm, about 6mm to about 8mm, about 6mm, or any range or amount therein in increments of 1mm. In some embodiments, the lateral dimension of the central beam can range from about 5 mm to about 15 mm, about 6mm to about 14mm, about 7mm to about 13mm, about 8mm to about 12mm, about 10mm, or any range or amount therein in increments of 1mm. In some embodiments, transverse cross-section of the central beam has an area with an effective diameter ranging from about 2mm to about 20 mm, from about 3 mm to about 18 mm, from about 4 mm to about 16 mm, from about 5 mm to about 14 mm, from about 6 mm to about 12 mm, from about 7 mm to about 10 mm, or any range therein. In some embodiments, the low profile has an area with a diameter of 2 mm, 4 mm, 6 mm, 8 mm, 10 mm, 12 mm, 14 mm, 16 mm, 18 mm, or any range therein, including any increment of 1 mm in any such diameter or range therein. In some embodiments, the width (mm) x height (mm) of the central beam can be 9.0x5.0, 9.0x6.0, 9.0x7.0, 9.0x8.0, 9.0x9.0, and 9.0x10.0, or any deviation in dimension therein in increments of +/- 0.1mm. And, in some embodiments, the central beam can have a transverse cross-sectional lateral or vertical dimension that ranges from 6.5mm to 14.0mm.

[00042] As shown in FIGs. 1B and 1C, the system 100 can also comprise a laterovertically-expanding frame 149 configured for operably contacting the central beam 101 to create a graft distribution system 100 *in vivo*, the frame 149 having a collapsed state 149c with a transverse cross section 149ct having a maximum dimension ranging from 5 mm to 15 mm for placing the frame 149 in the intervertebral space through the annular opening for expansion. Likewise, the frame 149 can also have an expanded state 149e with a transverse cross section 149et having a maximum dimension ranging from 6.5 mm to 18 mm for retaining the frame 149 in the intervertebral space, the expanded state operably contacting with the central beam 101 in the intervertebral space. The frame 149 can be defined as including a proximal portion 111 having an end, a grafting portion 112, a distal portion (not shown) having an end, and a central frame axis 113 of the expanded state 149e.

[00043] In some embodiments, the frame can have transverse cross-sectional lateral dimension in the collapsed state ranging from about 5mm to about 15mm. In some embodiments, the vertical dimension of the frame in the collapsed state can range from about 4mm to about 12mm, about 5mm to about 11mm, about 6mm to about 10mm, and about 7mm to about 9mm, about 6mm to about 8mm, about 6mm, or any range or amount therein in increments of 1mm. In some embodiments, the lateral dimension of the frame in the collapsed state can range from about 5 mm to about 15 mm, about 6mm to about 14mm, about 7mm to about 13mm, about 8mm to about 12mm, about 10mm, or any range or amount therein in increments of 1mm. In some embodiments, transverse cross-section of the frame in the collapsed state has an area with an effective diameter ranging from about 2mm to about 20 mm, from about 3 mm to about 18 mm, from about 4 mm to about 16 mm, from about 5 mm to about 14 mm, from about 6 mm to about 12 mm, from about 7 mm to about 10 mm, or any range therein. In some embodiments, the low profile has an area with a diameter of 2 mm, 4 mm, 6 mm, 8 mm, 10 mm, 12 mm, 14 mm, 16 mm, 18 mm, or any range therein, including any increment of 1 mm in any such diameter or range therein. In some embodiments, the width (mm) x height (mm) of the frame in the collapsed state can be 9.0x5.0, 9.0x6.0, 9.0x7.0, 9.0x8.0, 9.0x9.0, and 9.0x10.0, or any deviation in dimension therein in increments of +/- 0.1mm. In some embodiments, the frame can have a transverse cross-sectional dimension, lateral or vertical in the expanded state ranging from 4.0mm to 18mm, from 5.0mm to 19.0mm, from 6.0mm to 17.5mm, from 7.0mm to 17.0mm, from 8.0mm to 16.5mm, from 9.0mm to 16.0mm, from 9.0mm to 15.5mm, from 6.5mm to 15.5 mm, or any range or amount therein in increments of +/- 0.1mm.

[00044] The term "collapsed state" can be used to refer to a configuration of the frame in which the transverse cross-sectional area, or profile, is at least substantially at its minimum, and the term "expanded state" can be used to refer to a configuration of the frame that is expanded at least substantially beyond the collapsed state. In this context, a frame is expanded at least "substantially" beyond the collapsed state when a bone graft window of the frame has opened from the closed configuration by at least a 20% increase area of the bone graft window from the collapsed state. In some embodiments, the frame is expanded at least "substantially" beyond the collapsed state when a bone graft window of the frame has opened by at least a 15%, 20%, 25%, 30%, 35%, 40%, 45%, 50%, 60%, 70%, 80%, 90%, 100%, 150%, 200%, 250%, 300%, or more when compared to the bone graft window from the collapsed state. In some embodiments, the frame is expanded at least "substantially" beyond the collapsed state when a bone graft window of the frame has

opened by at least 2x, 3x, 5x, 10x, 15x, 20x, or more when compared to the bone graft window from the collapsed state.

[00045] In some embodiments, the laterovertically expandable frames are created in an expanded state. And the expanded state can include a state that is at least 30%, at least 40%, at least 50%, at least 60%, at least 70%, at least 80%, at least 90%, or at least 95% of the full expansion. The term “full expansion” can be used to refer to an extent of expansion upon which a connector element begins to fatigue, fail, or crack; or, in some embodiments, strain beyond 10%, 20%, or 30%.

[00046] The frame 149 can be configured to have a first top beam 150 including a proximal portion 111 having an end, a grafting portion 112, and a distal portion (not shown) having an end, the first top beam 150 configured for contacting the first top-lateral surface 117 of the central beam and the first top-side surface 127 of the central beam 101 in the expanded state 149e, the central axis of the first top beam at least substantially on (i) a top plane containing the central axis of the first top beam and the central axis of a second top beam and (ii) a first side plane containing the central axis of the first top beam and the central axis of a first bottom beam. Likewise the frame 149 can be configured to have a second top beam 160 including a proximal portion 111 having an end, a grafting portion 112 having an end, and a distal portion (not shown) having an end, the second top beam 160 configured for contacting the second top-lateral surface 119 of the central beam 101 and the second top-side surface 132 of the central beam 101 in the expanded state 149e, the central axis of the second top beam at least substantially on (i) the top plane and (ii) a second side plane containing the central axis of the second top beam and the central axis of a second bottom beam. Likewise the frame 149 can be configured to have a first bottom beam 170 including a proximal portion 111 having an end, a grafting portion 112, and a distal portion (not shown) having an end, the first bottom beam 170 configured for contacting the first bottom-lateral surface 122 of the central beam 101 and the first bottom-side surface 129 of the central beam 101 in the expanded state 149e, the central axis of the first bottom beam at least substantially on (i) a bottom plane containing the central axis of the first bottom beam and the central axis of a second top beam and (ii) the first side plane. Likewise the frame 149 can be configured to have a second bottom beam 180 including a proximal portion 111 having an end, a grafting portion 112 having an end, and a distal region (not shown) having an end, the second bottom beam 160 configured for contacting the second bottom-lateral surface 124 of the central beam 101 and the second bottom-side

surface 134 of the central beam 101 in the expanded state 149e, the central axis of the second bottom beam being at least substantially on (i) the bottom plane and (ii) a second side plane containing the central axis of the second bottom beam and the second top beam.

[00047] In some embodiments, the central axis of the first top beam 150 can be at least substantially parallel to the central beam axis 105. Likewise the frame 149 can be configured to have a second top beam 160 including a proximal portion 111 having an end, a grafting portion 112 having an end, and a distal portion (not shown) having an end, the second top beam 160 configured for contacting the second top-lateral surface 119 of the central beam 101 and the second top-side surface 132 of the central beam 101 in the expanded state 149e, the central axis of the second top beam 160 being at least substantially parallel to the central beam axis 105. Likewise the frame 149 can be configured to have a first bottom beam 170 including a proximal portion 111 having an end, a grafting portion 112, and a distal portion (not shown) having an end, the first bottom beam 170 configured for contacting the first bottom-lateral surface 122 of the central beam 101 and the first bottom-side surface 129 of the central beam 101 in the expanded state 149e, the central axis of the first bottom beam 170 being at least substantially parallel to the central beam axis 105. Likewise the frame 149 can be configured to have a second bottom beam 180 including a proximal portion 111 having an end, a grafting portion 112 having an end, and a distal region (not shown) having an end, the second bottom beam 160 configured for contacting the second bottom-lateral surface 124 of the central beam 101 and the second bottom-side surface 134 of the central beam 101 in the expanded state 149e, the central axis of the second bottom beam 180 being at least substantially parallel to the central beam axis 105.

[00048] As shown in FIG. 1D, the systems provided herein have the layered effect from the frame on the central beam that provides an additive dimension, both laterally and vertically. The added dimension allows for a low profile entry of the system into the intervertebral disc space, a wide lateral profile after expansion *in vivo* to avoid backout, as well as a sleeve for safe insertion of the central beam between the top endplate and bottom endplate in the intervertebral space. In some embodiments, the first top beam, second top beam, first bottom beam, and second bottom beam can each have a transverse cross-sectional wall thickness adding to the respective central beam dimension, the thickness ranging from about 0.5mm to about 5.0mm, from about 0.75mm to about 4.75mm, from about 1.0mm to about 4.5mm, from about 1.25mm to about 4.25mm, from about 1.5mm to

about 4.0mm, from about 1.75mm to about 3.75mm, from about 2.0mm to about 3.5mm, from about 2.25mm to about 3.25mm, or any range therein in increments of 0.05mm. In some embodiments, the first top beam, second top beam, first bottom beam, and second bottom beam can each have a transverse cross-sectional wall thickness adding to the respective central beam dimension, the thickness ranging from about 1.5mm to about 2.5mm, including 1.5, 1.75, 2.0, 2.25, 2.5, or an amount therein in increments of 0.05mm.

[00049] The beams of the laterovertically-expanding frame 149 can be operably connected through connector elements. As such, the frame 149 can include a plurality of proximal top connector elements 191 configured to expandably connect the proximal portion 111 of the first top beam 150 to the proximal portion 111 of the second top beam 160, the expanding consisting of a flexing at least substantially on a top plane containing the central axis of the first top beam 150 and the central axis of the second top beam 160. Likewise the frame 149 can be configured to have a plurality of distal top connector elements (not shown) configured to expandably connect the distal portion of the first top beam 150 to the distal portion of the second top beam 160, the expanding consisting of a flexing at least substantially on the top plane.

[00050] Likewise the frame 149 can be configured to have a plurality of proximal bottom connector elements 193 configured to expandably connect the proximal portion 111 of the first bottom beam 170 to the proximal portion 111 of the second bottom beam 180, the expanding consisting of a flexing at least substantially on a bottom plane containing the central axis of the first bottom beam 170 and the central axis of the second bottom beam 180. Likewise the frame 149 can be configured to have a plurality of distal bottom connector elements (not shown) configured to expandably connect the distal portion of the first bottom beam 170 to the distal portion of the second bottom beam 180, the expanding consisting of a flexing at least substantially on the bottom plane.

[00051] Likewise the frame 149 can be configured to have a plurality of proximal first side connector elements 195 configured to expandably connect the proximal portion 111 of the first top beam 150 to the proximal portion 111 of the first bottom beam 170, the expanding consisting of a flexing at least substantially on a first side plane containing the central axis of the first top beam 150 and the central axis of the first bottom beam 170; a plurality of distal first side connector elements (not shown) configured to expandably connect the distal portion of the first top beam 150 to the distal portion of the first bottom beam 170, the expanding consisting of a flexing at least substantially on the first side plane. Likewise the

frame 149 can be configured to have a plurality of proximal second side connector elements 197 configured to expandably connect the proximal portion 111 of the second top beam 160 to the proximal portion 111 of the second bottom beam 170, the expanding consisting of a flexing at least substantially on a second side plane containing the central axis of the second top beam 160 and the central axis of the second bottom beam 180; a plurality of distal second side connector elements (not shown) configured to expandably connect the distal portion of the second top beam 160 to the distal portion of the second bottom beam 180, the expanding consisting of a flexing at least substantially on the second side plane.

[00052] In some embodiments, each plurality of proximal connector elements can be configured as proximal struts in an at least substantially parallel alignment in the expanded state and the collapsed state; and, each plurality distal connector elements are distal struts can be configured in an at least substantially parallel alignment in the expanded state and the collapsed state. As such, the proximal top struts can be configured monolithically integral to the first top beam and the second top beam and adapted to flex toward the distal top struts during collapse; and, the distal top struts can be configured monolithically integral to the first top beam and the second top beam and adapted to flex toward the proximal top struts during collapse. Likewise, the proximal bottom struts can be configured monolithically integral to the first bottom beam and the second bottom beam and adapted to flex toward the distal bottom struts during collapse; and, the distal bottom struts can be configured monolithically integral to the first bottom beam and the second bottom beam and adapted to flex toward the proximal bottom struts during collapse. Likewise, the proximal first side struts can be configured monolithically integral to the first top beam and the first bottom beam and adapted to flex toward the distal first side struts during collapse; and, the distal first side struts can be configured monolithically integral to the first top beam and the first bottom beam and adapted to flex toward the proximal first side struts during collapse. Likewise, the proximal second side struts can be configured monolithically integral to the second top beam and the second bottom beam and adapted to flex toward the distal second side struts during collapse; and, the distal second side struts can be configured monolithically integral to the second top beam and the second bottom beam and adapted to flex toward the proximal second side struts during collapse.

[00053] As shown in FIG. 1D, the frame 149 can be configured for slidably engaging with the central beam 101 *in vivo* following placement of the central beam 101 in the intervertebral space through the annular opening, the slidably engaging including translating

the central beam 101 into the frame 149 from the proximal end 11 of the frame 149 toward the distal end of the frame 149 *in vivo*; the translating including keeping the central beam axis 105 at least substantially coincident with the central frame axis 113 during the translating to create the graft distribution system 100 *in vivo* through the annular opening. The system 100 can also be configured to form a top graft-slab depth 199t between the top surface 115 of the central beam 101 and the top vertebral endplate; and, a bottom graft-slab depth 199b (not shown) between the bottom surface 120 of the central beam 101 and the bottom vertebral endplate *in vivo*. And, in some embodiments, the transverse cross-section 110 of the system 100 *in vivo* is greater than the maximum lateral dimension of the annular opening to avoid backout.

[00054] One of skill will appreciate that the central beam can have any configuration that would be operable with the teachings provided herein. In some embodiments, criteria for a suitable central beam may include a combination of a material and configuration that provides a suitable stiffness. In some embodiments, the central beam can comprise an I-beam. An example of an I-beam configuration and a complementary laterover vertically expandable cage are shown in FIGs. 1E and 1F.

[00055] One of skill will further appreciate that the central beam can have any one or any combination of graft port configurations that would be operable with the teachings provided herein. In some embodiments, criteria for a suitable graft port configuration may include a combination of port size, number of ports, and placement of ports. In some embodiments, the central beam can comprise a side graft port.

[00056] One of skill will further appreciate that the connector elements can vary in design but should meet the constraints as taught herein. In some embodiments, for example each of the connector elements 191,193,195,197 can have a cross-sectional aspect ratio of longitudinal thickness to transverse thickness ranging from 1:2 to 1:8. A section of a connector element is shown in FIG. 1G.

[00057] As such, the systems can also include an improved, low-profile, intervertebral disc cage that expands bidirectionally. Consistent with the teachings herein, the cages offer several improvements to the art that include, for example, preventing the cage from backing out of the annulus fibrosis after expansion in an intervertebral disc space. As such, the terms "cage," "scaffold" and "scaffolding", for example, can be used interchangeably with "laterover vertically expandable frame", "expandable frame", or "frame", in some embodiments. The cages have the ability to at least (i) laterally expand within the intervertebral space to

avoid backout of the device through the annulotomy, (ii) vertically expand for distraction of the intervertebral space, (iii) provide additional space within the device in the annulus for the introduction of graft materials; (iv) maintain a large footprint to distribute load over a larger area against the endplate, for example, by not contracting in length to expand in height and/or width; and, (v) insert into the annulus in a minimally-invasive manner using only a unilateral approach.

[00058] FIGs. 2A-2F illustrate a method of using a bidirectionally-expandable cage, according to some embodiments. As shown in FIGs. 2A-2B, an annulus 205 is prepared with an annulotomy serving as a single point of entry 210 and an intervertebral space 215 for insertion of a bidirectionally expandable cage system 250. As shown in FIGs. 2C-2F, the system 250 has a cage 255 having a proximal end 256, a distal end 257, and a lumen 258 that communicates with the intervertebral space 215 through an expandable/collapsible bone graft window 259; a shim core 260 having a tapered nose 262 at the distal end of the shim core 260; a releasably attachable rail beam 265; a pusher 270 that slidably translates over the shim core 260 and the rail beam 265; a trial shim 275 having a shoulder 277 and slidably translating over the rail beam 265 and shim core 260 into the lumen 258 of the cage 255, and a permanent shim 280 having a shoulder 282 and slidably translating over the rail beam 265 and shim core 260 into the lumen 258 of the cage 255.

[00059] The procedure for implanting the cage 255 begins in FIG. 2A, including inserting a cannula (not shown) with a bullet-nosed obturator through the single point of entry 210 and inside the intervertebral disc space 215 until contacting the opposing wall of the annulus 205. The cannula (not shown) depth is used to select the desired length of the cage 255. The shim core 260 is loaded with bone graft material and the rail beam 265 is releasably attached to the shim core 260. The cage 255 is loaded onto the rail beam 265 and pushed onto the shim core 260 and into the cannula (not shown) using the pusher 270 until the distal end 257 of the cage 255 contacts the back of the tapered nose 262 of the shim core 260 as shown in FIG. 2A. The assembly of the shim core 260 and the cage 255 are inserted into the intervertebral space 215, and the cannula (not shown) is removed as shown in FIG. 2B. The lumen 258 of the cage 255 is loaded with bone graft material, and the trial shim 275 is slidably translated over the rail beam 265 and the shim core 260 into the lumen 258 of the cage 255 as shown in FIG. 2C. A variety of sizes of the trial shim 275 can be tested until the largest trial shim 275 that will fit is found, or until the trial shim having the desired vertical and lateral dimensions for expansion is used, in order to laterovertically

expand the cage 255 as desired. The trial shim 275 is then removed, and the lumen 258 of the cage 255 is again filled with bone graft material with the shim core 260 remaining in place as shown in FIG. 2D. The permanent shim 280 is then slidably translated along the rail beam 265 and the shim core 260 into the intervertebral space 215 using the pusher 270 until the distal end 257 of the cage 255 contacts the back of the tapered nose 262 of the shim core 260 to maintain the desired laterovertical expansion of the cage 255 as shown in FIG. 2E. The rail beam 265 is then disconnected from the shim core 260 as shown in FIG. 2F.

[00060] It should be appreciated that the annulotomy can have nearly any dimension considered desirable to one of skill in the art. The annulotomy can have a vertical dimension, for example, that is the distance between a top vertebral plate and a bottom vertebral plate, the top vertebral plate and the bottom vertebral plate defining the upper and lower borders of the intervertebral disc space. In some embodiments, the vertical dimension can range from about 4mm to about 12mm, about 5mm to about 11mm, about 6mm to about 10mm, and about 7mm to about 9mm, about 6mm to about 8mm, about 6mm, or any range or amount therein in increments of 1mm. In some embodiments, the lateral dimension of the single point of entry can range from about 5 mm to about 15 mm, about 6mm to about 14mm, about 7mm to about 13mm, about 8mm to about 12mm, about 10mm, or any range or amount therein in increments of 1mm. In some embodiments, the single point of entry has an area with a diameter ranging from about 2mm to about 20 mm, from about 3 mm to about 18 mm, from about 4 mm to about 16 mm, from about 5 mm to about 14 mm, from about 6 mm to about 12 mm, from about 7 mm to about 10 mm, or any range therein. In some embodiments, the low profile has an area with a diameter of 2 mm, 4 mm, 6 mm, 8 mm, 10 mm, 12 mm, 14 mm, 16 mm, 18 mm, or any range therein, including any increment of 1 mm in any such diameter or range therein. The low profile dimensions of the cages taught herein are designed to fit within these dimensions.

[00061] One of skill will also appreciate that there are several methods and devices that could be used to expand the cage. In some embodiments, the expanding includes using a means for (i) laterovertically expanding the cage and (ii) creating a convex surface that at least substantially complements the concavity of a surface of a vertebral endplate that contacts the pair of top beams or the pair of bottom beams.

[00062] One of skill will also appreciate a method that distracts the intervertebral space and laterally expands the cage to avoid back-out. As such, in some embodiments, the

expanding includes introducing a lateroververtical expansion member into the intervertebral space through the single point of entry and into the cage, the lateroververtical expansion member configured to provide a vertical force through the cage and into the top vertical endplate and bottom vertical endplate to distract the intervertebral space; and, a lateral force on the first side wall and the second side wall to expand the cage to a width that is greater than the lateral dimension of the single point of entry to prevent the bidirectionally-expandable cage from backing out of the annulus fibrosis after the expanding.

[00063] One of skill will also appreciate having a method for passing bone grafting material into the intervertebral space. As such, the lateroververtical expansion member can include a port for introducing the grafting material into the intervertebral space. The methods and systems provided herein include the use of bone graft materials known to one of skill. Materials which may be placed or injected into the intervertebral space include solid or semi-solid grafting materials, bone from removed from patient's facet, an iliac crest harvest from the patient, and bone graft extenders such as hydroxyapatite, demineralized bone matrix, and bone morphogenic protein. Examples of solid or semi-solid grafting material components include solid fibrous collagen or other suitable hard hydrophilic biocompatible material. Some materials may also include swelling for further vertical expansion of the intervertebral disc space.

[00064] One of skill will also appreciate having a method for retaining the lateroververtical expansion member in the cage. As such, the introducing can include engaging a ratchet mechanism comprising a protuberance on the lateroververtical expansion member that engages with a strut of the cage to prevent the cage from backing out of the annulus fibrosis after the expanding. The ratchet mechanism can be, for example, similar to a zip-tie ratchet mechanism having a gear component and a pawl component. In some embodiments, the cage has the gear component, for example, including the struts; and, the lateroververtical expansion member is a shim device having the pawl component, for example, a projection that can angle toward the proximal end of the expansion member or away from the direction of insertion of the shim device. In some embodiments, the cage has the pawl component, for example, including the struts; and, the lateroververtical expansion member is a shim device having the gear component, for example, a series of projections. In some embodiments, a projection can angle from about 5° to about 75° toward the proximal end of the expansion member or away from the direction of insertion of the shim device.

[00065] One of skill will also appreciate having a method of designing the shape of the cage upon expansion. As such, in some embodiments, the expanding includes selecting a shim configured to create a convex surface on the top surface of the top wall to at least substantially complement the concavity of the respective top vertebral plate, and/or the bottom surface of the bottom wall to at least substantially complement the concavity of the respective bottom vertebral plate. In some embodiments, the expanding includes selecting a shim configured to vertically expand the distal end of the cage more than the proximal end of the cage. And, in some embodiments, the expanding includes selecting a shim configured to laterally expand the distal end of the cage more than the proximal end of the cage.

[00066] FIGs. 3A-3D illustrate collapsed and expanded views of a bidirectionally-expandable cage for fusing an intervertebral disc space, according to some embodiments. FIGs. 3A and 3C show an expanded configuration, and FIGs. 3B and 3D show a collapsed configuration. The cage 300 can comprise at least 4 walls 302,304,306,308 that form a cylinder having a long axis 309, the at least 4 walls 302,304,306,308 including a top wall 302 forming a top plane and having a top surface with protuberances (not shown) adapted to contact the top vertebral plate (not shown); a bottom wall 304 forming a bottom plane and having a bottom surface with protuberances (not shown) adapted to contact the bottom vertebral plate (not shown); a first side wall 306 forming a first side wall plane; and, a second side wall 308 forming a second side wall plane. In these embodiments, each of the walls 302,304,306,308 can have at least 2 longitudinal beams, such that a rectangular cylinder can have a total of 4 longitudinal beams 312,314,316,318; and, a plurality of struts 333 that (i) stack in the collapsed state of the cage 300, as shown in FIGs. 3B and 3D, to minimize void space in their respective wall for a low profile entry of the cage 300 both vertically and laterally into a single point of entry (not shown) into an intervertebral disc space (not shown) and (ii) deflect upon expansion to separate the at least 2 longitudinal beams of the total of 4 longitudinal beams 312,314,316,318 in the rectangular cylinder in their respective wall 302,304,306,308. In addition, the cage 300 can be configured to expand laterally in the intervertebral space (not shown) to a size greater than a lateral dimension of the single point of entry (not shown) to prevent the bidirectionally-expandable cage 300 from backing out of the annulus fibrosis (not shown) after the expanding shown in FIGs. 3A and 3C.

[00067] It should be appreciated that the collapsed configuration includes the design of a low profile entry through the annulus fibrosis to allow for a minimally-invasive procedure. In order to facilitate the use of a minimally-invasive procedure, the low profile entry of the collapsed configuration should be a substantially small area of entry having a diameter ranging, for example, from about 5 mm to about 12 mm for the single point of entry through the annulus fibrosis. In some embodiments, the low profile has an area with a diameter ranging from about 2mm to about 20 mm, from about 3 mm to about 18 mm, from about 4 mm to about 16 mm, from about 5 mm to about 14 mm, from about 6 mm to about 12 mm, from about 7 mm to about 10 mm, or any range therein. In some embodiments, the low profile has an area with a diameter of 2 mm, 4 mm, 6 mm, 8 mm, 10 mm, 12 mm, 14 mm, 16 mm, 18 mm, or any range therein, including any increment of 1 mm in any such diameter or range therein.

[00068] One of skill will appreciate that a variety of strut configurations may be contemplated to minimize void space for the low profile entry of the cage into the intervertebral space. In some embodiments, each wall of the cage has a series of v-shaped struts 333 that (i) stack in a closed-complementary configuration 344 in the collapsed state to minimize void space in their respective wall for the low profile entry of the cage both vertically and laterally into the intervertebral space, and (ii) deflect upon expansion in a plane that is at least substantially parallel to the plane of their respective wall to an open-complementary configuration 355 to separate the at least 2 longitudinal beams of the total of 4 longitudinal beams 312,314,316,318 in the rectangular cylinder in their respective wall and open a bone graft window 366 to pass a bone graft material into the intervertebral space in the expanded configuration. In some embodiments, the cage 300 is configured to accommodate the lateral dimension of the single point of entry ranging from about 5 mm to about 15 mm.

[00069] The v-shaped struts can be "V" shaped slots projected through each of the cage walls starting at a distance of 2mm (.5-4) from each corner of the cage to effectively render the "V" shaped struts in the mid region of the wall faces, in which the struts can be fabricated as continuous with L shaped beams on the corners. The slots can be cut such that they are projected perpendicular to the faces or angled distally from the outside of the cage to the inside of the cage. The distally angled projection can facilitate insertion of the shims taught herein. And, the proximal faces of the corners of the beams can also have inward, distally angled chamfers to facilitate insertion of the shims taught herein. The struts

can be uniform in thickness in the proximal-distal direction. In some embodiments, the struts range from about 0.2mm to about 1.0mm, from about 0.3mm to about 0.9mm, from about 0.4mm to about 0.8mm, from about 0.5mm to about 0.7mm in thickness, or any range therein in increments of about 0.1mm. The vertex of the "V" strut can trace along the center axis of the each of the side faces and can be radiused to dimension of .031" (.005-.062"), in some embodiments, to prevent stress cracking. Moreover, the shape of the strut or the slot projections can also be C, U, or W, in some embodiments. The struts can be 4 times thicker in the direction perpendicular to the long axis of the cage than in the direction of the long axis of the cage. In some embodiments, this thickness ratio can range from about 2x to about 8x, from about 3x to about 7x, from about 4x to about 6x, about 5x, or any range therein in increments of 1x. This thickness can help maintain a high structural stiffness and strength in the direction perpendicular to the proximal-distal axis so that the transverse cross section (perpendicular to the proximal-distal axis) shape is maintained during and after insertion of the cage into the intervertebral disc space.

[00070] In some embodiments, the angle of each strut can range from about 140° -170° as measured at the vertex in the non-stressed state. In these embodiments, the angle facilitates flexion of the legs of each strut towards each other upon moderate inward pressure to collapse the cage for insertion into the disc space. Furthermore the angled strut lies in a plane at least substantially parallel to the plane of it's respective wall, and in some embodiments to the long axis of the cage, so that the flexion does not alter the side wall thickness. This helps to maintain the low profile for insertion while maximizing the lumen size. This geometry combined with the solid beams on the corners helps ensure that the implant has a minimal change in length, less than 15% reduction in length as measured along the long axis, when expanded more than 20% vertically and/or horizontally. As such, the top and bottom of the cage that support the vertebra remain at least substantially constant in length regardless of expansion.

[00071] In some embodiments, the cage 300 has v-shaped struts 333 and a bone graft window 366 that (i) complements the v-shaped struts 333 in the collapsed configuration and (ii) opens upon expansion to pass a bone graft material into the intervertebral space in the open-complementary configuration 355, which can also be referred to as an expanded configuration. And, in some embodiments, the cage 300 has a proximal region 311, a proximal end 322, a distal region 388, a distal end 399, and at least one of the at least 4 walls 302,304,306,308 having a first series of v-shaped struts 333 that are configured to

stack in a closed-complementary configuration 344 in the collapsed state to minimize void space for the low profile entry of the cage 300 into the intervertebral space; and, deflect upon expansion to an open-complementary configuration 355 to separate the at least 2 longitudinal beams of the total of 4 longitudinal beams 312,314,316,318 in the rectangular cylinder in their respective wall and open a bone graft window 366 adapted to pass a bone graft material into the intervertebral space in the expanded configuration; wherein, the first series of v-shaped struts 333F is located in the proximal region of the cage, the vertices of the first series of v-shaped struts 333F pointing away from the proximal end 322 of the cage 300 and toward the distal end 399 of the cage 300. In some embodiments, the cage 300 can further comprise a second series of v-shaped struts 333S that stack in a closed-complementary configuration 344 in the collapsed state to minimize void space for the low profile entry of the cage 300 into the intervertebral space; and, deflect upon expansion to an open-complementary configuration 355 to separate the at least 2 longitudinal beams of the total of 4 longitudinal beams 312,314,316,318 in the rectangular cylinder in their respective wall and open a bone graft window 366 adapted to pass a bone graft material into the intervertebral space in the expanded configuration; wherein, the second series of v-shaped struts 333S is located in the distal region 388 of the cage 300, the vertices of the second series of v-shaped struts 333S pointing away from the distal end 399 of the cage 300 and toward the proximal end 322 of the cage 300. In such embodiments, the strut configuration can result in the expansion of the first series of v-shaped struts 333F and the second series of v-shaped struts 333S creating a bone graft window 366 that opens to the bow-tie configuration shown in FIGs. 3A and 3C.

[00072] One of skill will also appreciate that the cage design provides flexibility in the relative amounts of lateral expansion and vertical expansion, as well as the relative amounts of expansion proximally and distally across the cage in either the lateral or vertical expansions. As such, in some embodiments, the cage is configured such that the ratio of the amount of lateral expansion to the amount of vertical expansion is variable. And, in some embodiments, the cage is configured such that the ratio of the amount of proximal expansion to the amount of distal expansion is variable for lateral expansion or vertical expansion.

[00073] FIGs. 4A and 4B illustrate collapsed and expanded views of a bidirectionally-expandable cage having a bone graft window on each wall for fusing an intervertebral disc space, according to some embodiments. FIG. 4A shows the cage 400 in the collapsed

configuration for a low-profile entry 405 into to single point of entry into an intervertebral disc space, and FIG. 4B shows the cage 400 in the expanded configuration to distract the intervertebral disc space and avoid back-out of the cage through the single point of entry after the expansion. As shown, each wall contains a bone graft window 466 for passing bone graft material into the intervertebral disc space.

[00074] FIGs. 5A-5D illustrate system for fusing an intervertebral disc space, according to some embodiments. As shown, the system 550 has a cage 555 having an expandable/collapsible bone graft window 566; a shim core 560 having a tapered nose 562 at the distal end of the shim core 560 and a bone graft window 566; a releasably attachable rail beam 565; a pusher (not shown) that slidably translates over the shim core 560 and the rail beam 565; a trial shim 575 having a shoulder 577 and slidably translating over the rail beam 565 and shim core 560 into the cage 555, and a permanent shim 580 having a shoulder 582 and slidably translating over the rail beam 565 and shim core 560 into the cage 555. The system can comprise a bidirectionally-expandable cage having at least 4 walls that form a cylinder having a long axis. The at least 4 walls can include, for example, a top wall forming a top plane and having a top surface with protuberances adapted to contact the top vertebral plate; a bottom wall forming a bottom plane and having a bottom surface with protuberances adapted to contact the bottom vertebral plate; and, a first side wall forming a first side wall plane, and a second side wall forming a second side wall plane. Each of the walls can have at least 2 longitudinal beams; and, a plurality of struts that (i) stack in the collapsed state to minimize void space in their respective wall for a low profile entry of the cage both vertically and laterally into a single point of entry into an intervertebral disc; and, (ii) deflect upon expansion to separate the at least 2 longitudinal beams in their respective wall. In some embodiments, the cage can be configured to expand laterally in the intervertebral space to a size greater than a lateral dimension of the single point of entry to prevent the bidirectionally-expandable cage from backing out of the annulus fibrosis after the expanding. Moreover, the system can include a laterovertical expansion member configured to induce the laterally expanding and the vertically expanding of the cage; and, a core configured to guide the laterovertical expansion member into the cage to induce the laterally expanding and the vertically expanding of the cage.

[00075] One of skill will appreciate that the laterovertical expansion member can also be configured to slidably engage with the core to translationally enter the cage in along the long axis of the cage. In some embodiments, the lateral expansion can occur concurrent with the

vertical expansion and, in some embodiments, the lateral expansion can occur prior to the vertical expansion, for example, to reduce frictional stress on the cage during the lateral expansion. A two stage shim, for example, can be used. A first stage shim can be inserted to expand the cage laterally before inserting a second stage shim to expand the cage vertically. In some embodiments, the second stage shim can slidably translate along the first stage shim. The shim can be made of any material considered desirable to one of skill, for example, a metal or a polymer. In some embodiments, the shim can comprise a non-resorbable polymer material, an inorganic material, a metal, an alloy, or bone.

[00076] One of skill will appreciate that a system can include all or any combination of the above. As such, the teachings also include system for fusing an intervertebral disc space, the system comprising a bidirectionally-expandable cage having a proximal region, a proximal end, a distal region, a distal end, and at least 4 walls, the cage fabricated as a continuous single piece. In these embodiments, the at least 4 walls form a cylinder having a long axis and include a top wall forming a top plane and having a top surface with protuberances adapted to contact the top vertebral plate; a bottom wall forming a bottom plane and having a bottom surface with protuberances adapted to contact the bottom vertebral plate; and, a first side wall forming a first side wall plane, and a second side wall forming a second side wall plane. Each of the walls can have at least 2 longitudinal beams and a plurality of struts.

[00077] At least one of the walls can have a first series of v-shaped struts that are configured to stack in a closed-complementary configuration in the collapsed state to minimize void space for a low profile entry of the cage through a single point of entry into an intervertebral disc space; and, deflect upon expansion to an open-complementary configuration to separate the at least 2 longitudinal beams in their respective wall and open a bone graft window adapted to pass a bone graft material into the intervertebral space in the expanded configuration. The first series of v-shaped struts can be located in the proximal region of the cage, the vertices of the first series of v-shaped struts pointing away from the proximal end of the cage and toward the distal end of the cage; and, the cage can be configured to expand laterally in the intervertebral space to a size greater than a lateral dimension of the single point of entry to prevent the bidirectionally-expandable cage from backing out of the annulus fibrosis after the expanding. A laterovertical expansion member can be configured to induce the laterally expanding and the vertically expanding of the cage; and, a core can be configured to guide the laterovertical expansion member into the

proximal end of the cage, and along the long axis of the cage, to expand the cage laterally and vertically. Moreover, the laterovertical expansion member can slidably engage with the core to translationally enter the cage along the long axis of the cage.

[00078] One of skill will appreciate that the systems and system components can be manufactured using any method known to one of skill in the manufacture of such intricate metal and/or polymeric components. For example, the cage can be fabricated in a partially expanded state or a fully expanded state. Moreover, the cage can be manufactured to have no internal stress or strain in the partially or fully expanded state when no external loading is applied.

[00079] The system components can comprise any suitable material, or any combination of materials, known to one of skill. For example, all components can be metal, all components can be plastic, or the components can be a combination of metal and plastic. One of skill will appreciate that the cages can have performance characteristics that are near that of a bone structure, in some embodiments, such that the scaffoldings are not too stiff or hard, resulting in a localized loading issue in which the scaffolding puts too much pressure on native bone tissue, and likewise such that the scaffoldings are too flexible or soft, resulting in a localized loading issue in which the bone tissue puts too much pressure on the scaffolding. A radio-opaque material can be employed to facilitate identifying the location and position of the scaffolding in the spinal disc space. Examples of such materials can include, but are not limited to, platinum, tungsten, iridium, gold, or bismuth.

[00080] One of skill can select materials on the basis of desired material performance characteristics. For example, one of skill will look to performance characteristics that can include static compression loading, dynamic compression loading, static torsion loading, dynamic torsion loading, static shear testing, dynamic shear testing, expulsion testing, and subsidence testing. The parameters for upper and lower limits of performance for these characteristics can fall within the range of existing such spinal devices that bear the same or similar environmental conditions during use. For example, a desired static compression loading can be approximately 5000N. A desired dynamic compression loading can have an asymptotic load level of  $\geq 3000\text{N}$  at  $5 \times 10^6$  cycles or  $\geq 1500\text{N}$  at  $10 \times 10^6$  cycles. The desired load level can range, for example, from about 1.0x to about 2.0x, from about 1.25x to about 1.75x, or any range therein in increments of 0.1x, the vertebral body compression strength. Examples of standard procedures used to test such performance characteristics include ASTM F2077 and ASTM F2624.

[00081] Examples of suitable materials can include non-reinforced polymers, carbon-reinforced polymer composites, PEEK (polyether ketone) and PEEK composites, polyetherimide (ULTEM), polyimide, polyamide or carbon fiber. Other examples include metals and alloys comprising any one or more components including, but not limited to, shape-memory alloys, nickel, titanium, titanium alloys, cobalt chrome alloys, stainless steel, ceramics and combinations thereof. In some embodiments, the components are all titanium or titanium alloy; all PEEK; or a combination of titanium or titanium alloy and PEEK. In some embodiments, the cage comprises titanium or titanium alloy, and the shim comprises PEEK. In some embodiments, the scaffolding can comprise a metal frame and cover made of PEEK or ULTEM. Examples of titanium alloys can include alloys of titanium, aluminum, and vanadium, such as  $Ti_6Al_4V$  in some embodiments.

[00082] In some embodiments, the cage can be fabricated from strong and ductile polymers having a tensile modulus of about 400,000 psi or more, and a tensile strength of about 14,000 psi or more. Such polymers may also have the ability to strain more than 4% to break, and perhaps at least 20% to break in some embodiments. The materials can be stiffened by being filled with glass fibers or carbon fibers in some embodiments.

[00083] Bone ingrowth is desirable in many embodiments. As such, the scaffolding can comprise materials that contain holes or slots to allow for such bone ingrowth. Consistently, the scaffoldings can be coated with hydroxyapatite, or other bone conducting surface, for example, bone morphogenic protein, to facilitate bone ingrowth. Moreover, the surfaces of the scaffoldings can be formed as rough surfaces with protuberances, insets, or projections of any type known to one of skill, such as teeth or pyramids, for example, to grip vertebral endplates, avoid migration of the scaffolding, and encourage engagement with bone ingrowth.

[00084] The methods and systems provided herein include the use of bone graft materials known to one of skill. Materials which may be placed or injected into the intervertebral space include solid or semi-solid grafting materials, bone from removed from patient's facet, an iliac crest harvest from the patient, and bone graft extenders such as hydroxyapatite, demineralized bone matrix, and bone morphogenic protein. Examples of solid or semi-solid grafting material components include solid fibrous collagen or other suitable hard hydrophilic biocompatible material. Some materials may also include swelling for further vertical expansion of the intervertebral disc space.

[00085] The systems taught herein can be provided to the art in the form of kits. A kit can contain, for example, a cage, a vertical expansion member, and a bone graft material. In some embodiments, the kit will contain an instruction for use. The vertical expansion member can be any vertical expansion mechanism or means taught herein. For example, the vertical expansion member can be a shim. In some embodiments, the kit includes a graft-injection shim for temporarily distracting the intervertebral space, the graft-injection shim having a port for receiving and distributing the bone graft material in the intervertebral space. In these embodiments, the graft-injection shim can remain as a permanent shim or be removed and replaced with a permanent shim.

[00086] FIG. 6 is a flowchart of a method of using a bidirectionally-expandable cage, according to some embodiments. The methods can include creating 605 a single point of entry into an intervertebral disc, the intervertebral disc having a nucleus pulposus surrounded by an annulus fibrosis, and the single point of entry having a lateral dimension created through the annulus fibrosis. The methods can also include removing 615 the nucleus pulposus from within the intervertebral through the single point of entry, leaving an intervertebral space for expansion of a bidirectionally-expandable cage within the annulus fibrosis, the intervertebral space having a top vertebral plate and a bottom vertebral plate. The methods can also include inserting 625 a bidirectionally-expandable cage through the single point of entry into the intervertebral space. Moreover, the methods can include expanding 635 the cage in the intervertebral space both laterally and vertically, adding 645 a grafting material to the intervertebral space through the single point of entry, and inserting 665 a permanent shim into the cage.

[00087] One of skill will appreciate having the ability to control the amounts of vertical expansion and lateral expansion of the cage to accommodate a variety of applications, for example, to accommodate a variety annulotomy dimensions used for the single point of entry. As such, in some embodiments, the expanding 635 includes selecting 655 an amount of lateral expansion independent of an amount of vertical expansion. The lateral expanding of the cage can be selected, for example, to exceed the lateral dimension of the single point of entry through an annulotomy by a desired amount to avoid, or prevent, the cage from backing out of the intervertebral space after expansion.

[00088] As such, methods of fusing an intervertebral space are provided herein using any of the graft distribution systems taught herein. The methods can include creating a single point of entry into an intervertebral disc, the intervertebral disc having a nucleus pulposus

surrounded by an annulus fibrosis, and the single point of entry having the maximum lateral dimension created through the annulus fibrosis. The methods can also include removing the nucleus pulposus from within the intervertebral disc through the single point of entry, leaving the intervertebral space for expansion of the graft distribution system within the annulus fibrosis, the intervertebral space having the top vertebral plate and the bottom vertebral plate. The methods can also include inserting the laterover vertically expanding frame in the collapsed state through the single point of entry into the intervertebral space; and, inserting the central beam into the frame to form the graft distribution system. Moreover, the methods can also include adding a grafting material to the intervertebral space through the entry port.

[00089] FIGs. 7A-7F illustrate some additional features of graft distribution systems, according to some embodiments. The graft distribution systems 700 provided herein have at least a top exit port 740 and a bottom exit port 741 in the grafting portion of the central beam 701, but they can also contain side ports 742, 743, such that there are at least 4 graft distribution ports in some embodiments. In some embodiments, the central beam 701 further comprises a first side graft port 742 and a second side graft port 743, in addition to a locking clip 702 at the proximal end of the central beam. In some embodiments, the laterover vertically-expanding frame 749 can be a monolithically integral frame, optionally having a "bullet nose" 703 at the distal end of the frame for safe position of the cage against the anterior inner annulus *in vivo*, and adapted to open a graft distribution window 788 on at least the top and bottom sides, as well as the first side and second side in some embodiments containing side ports, upon expansion of the connector elements to facilitate graft distribution within the intervertebral space.

[00090] The distal end of the frame 749 can be configured to have a laterover vertically operable connection with a guide plate 707 that restricts the first top beam, the first bottom beam, the second top beam, and the second bottom beam to laterover vertical movement relative to the guide plate when converting the frame from the collapsed state to the expanded state *in vivo*. And, in some embodiments, the laterover vertically-expandable frame has a lumen, and the guide plate has a luminal side with a connector 708 for reversibly receiving a guide wire for inserting the laterover vertically-expandable frame into the intervertebral space. In some embodiments, the frame has a chamfer inside the proximal end of the frame beams to facilitate insertion of central beam. And, in many embodiments,

the frames have means for creating friction between the vertebral endplates and the frame, such as protuberances, for example cleat-type structures 704, to further avoid backout.

[00091] As can be seen in at least FIG. 7, the bone graft distribution systems provided herein include bone graft windows defined by the connector elements, the bone graft windows opening upon expansion of the laterover vertically expanding frame. In some embodiments, the method further comprises opening a bone graft window, wherein the connector elements include v-shaped struts that (i) stack either proximally or distally in a closed-complementary configuration in the collapsed state to minimize void space for a low profile entry of the system both vertically and laterally into the intervertebral space, and (ii) deflect upon expansion to open the bone graft window.

[00092] It should be appreciated that the bone graft distribution systems provided herein also allow for independent expansion laterally and vertically by expanding in steps. In some embodiments, the expanding includes selecting an amount of lateral expansion independent of an amount of vertical expansion. And, in some embodiments, the lateral expansion exceeds the width of the annular opening that is the single point of entry into the intervertebral space. For example, the lateral dimension of the single point of entry can range from about 5 mm to about 15 mm in some embodiments. As such, in some embodiments, the expanding includes expanding the laterover vertically expanding frame laterally to a width that exceeds the width of the single point of entry; and, inserting the central beam to expand the laterover vertically expanding frame vertically to create the graft distribution system.

[00093] The bone graft distribution systems provided herein also have additional means for retaining the central beam in the laterover vertically expanding frame. In some embodiments, the inserting of the central beam into the laterover vertically expanding frame includes engaging a ratchet mechanism comprising a protuberance on the central beam that engages with the laterover vertically-expanding frame to prevent the central beam from backing out of the laterover vertically-expanding frame after the expanding.

[00094] Moreover, the bone graft distribution systems provided herein can be in the form of a kit. The kits can include, for example, a graft distribution system taught herein, a cannula for inserting the graft distribution system into the intervertebral space, a guidewire adapted for guiding the central beam into the laterover vertically expanding frame, and an expansion handle for inserting the central beam into the laterover vertically expanding frame to form the graft distribution system.

[00095] FIGs. 8A-8D illustrate components of a kit, according to some embodiments. FIGs. 8A and 8B illustrate a 4-sided funnel cannula 805 as taught herein having a shaft 810 forming a channel 815, a funnel 820 for guiding a laterover vertically expandable frame into an annulus in a low-profile configuration, the cannula shown with an obturator 825 in the channel 815 of the cannula 805, the cannula 805 inserted posterolaterally through an annulotomy 877 in the annulus 888, into an intervertebral space 899, with the distal end of the cannula 805 position near the inner anterior wall of the annulus 888. FIG. 8C illustrates FIG. 8A with a guidewire used to insert the laterover vertically expandable frame 749 into the funnel 820 of the cannula 805 to guide the frame 749 into the annulus 888 in the low profile, collapsed state of the frame 749. FIG. 8D illustrates an expansion handle 855 having trigger 856 that pushes a pushrod 857 along the guidewire 866 while holding the guidewire to push on the proximal end of the central beam 701 to insert the central beam 701 into the frame 749 to expand the frame 749 by applying equal, or substantially equal forces: a proximally-directed force,  $F_P$ , at the connection 708 between the guide plate 707 and the guide wire 866 onto the distal portion of the beams of the frame 749, and a distally-directed force,  $F_D$ , at the proximal end of the central beam 701.

[00096] FIGs. 9A-9C illustrate the expansion of a laterover vertically-expandable frame in an intervertebral space, according to some embodiments. FIG. 9A shows a collapsed frame 949 receiving a central beam 901 along a guidewire 966. FIG. 9B shows the central beam 901 partially inserted into the frame 949 in an expanded state, the guidewire 966 still in place FIG. 9C shows how the expanded state may appear when inserted posterolaterally and expanded in the intervertebral space in an annulus 988. Side ports 942,943 for bone graft distribution are shown through an open bone graft window in the expanded frame 749.

[00097] FIGs. 10A-10C illustrate profiles of an expanded graft distribution system to highlight the exit ports and bone graft windows, according to some embodiments. Profiles of an expanded frame 1049, highlighting bone graft windows 1088 and graft ports 1040,1041,1042,1043 as they may appear in an intervertebral space after an implant procedure. The guidewire 1066 is shown as remaining in place.

[00098] FIGs. 11A and 11B compare an illustration of the graft distribution in place to a test placement in a cadaver to show relative size, according to some embodiments. Likewise, FIGs. 12A-12C show x-rays of a placement in a cadaver, according to some embodiments.

[00099] As described above, the frame 149 can be configured such that the central axis of the first top beam 150 is at least substantially on (i) the top plane and (ii) the first side plane; the central axis of the second top beam 160 is at least substantially on (i) the top plane and (ii) the second side plane; the central axis of the first bottom beam 170 is at least substantially on (i) the bottom plane and (ii) the first side plane; and, the central axis of the second bottom beam being at least substantially on (i) the bottom plane and (ii) the second side plane. It should be appreciated that this configuration provides a “top face” framed by the first top beam and the second top beam, a “bottom face” framed by the first bottom beam and the second bottom beam, a “first side face” framed by the first top beam and the first bottom beam, and a “second side face” framed by the second top beam and the second bottom beam.

[000100] In some embodiments, it can be desirable to have the frame expand to shape that is predesigned to fit between the top endplate and the bottom endplate of the intervertebral space in a manner that calls, for example, for opposing faces of the frames to be something other than “at least substantially parallel.” For example, it may be desired to have the two opposing sides of the frame expand such that the central axis of the first top beam is no longer at least substantially parallel to the central axis of the second top beam. Likewise, it may be desired to have the two opposing sides of the frame expand such that the central axis of the first bottom beam is no longer at least substantially parallel to the central axis of the second bottom beam. Likewise, it may be desired to have the opposing top and bottom sides of the frame expand such that the central axis of the first top beam is no longer at least substantially parallel to the central axis of the first bottom beam. Likewise, it may be desired to have the opposing top and bottom sides of the frame expand such that the central axis of the second top beam is no longer at least substantially parallel to the central axis of the second bottom beam. Or, any combination of the above may be desired. The laterovertically expandable frames taught herein enable each of these desirable configurations.

[000101] FIGs. 13A-13D show orientations of the first top beam relative to the second top beam, first bottom beam relative to the second bottom beam, first top beam relative to the first bottom beam, and the second top beam relative to the second bottom beam, according to some embodiments. FIG. 13A shows the first top beam 150 relative to the second top beam 160, in which the angle  $\Theta_T$  is formed by the two beams to shape the top face of the frame. FIG. 13B shows the first bottom beam 170 relative to the second bottom beam 180,

in which the angle  $\Theta_B$  is formed by the two beams to shape the bottom face of the frame. FIG. 13C shows the first top beam 150 relative to the first bottom beam 170, in which the angle  $\Theta_{FS}$  is formed by the two beams to shape the first side face of the frame. FIG. 13D shows the second top beam 160 relative to the second bottom beam 180, in which the angle  $\Theta_{SS}$  is formed by the two beams to shape the second side face of the frame. In some embodiments, each of  $\Theta_T$ ,  $\Theta_B$ ,  $\Theta_{FS}$ , and  $\Theta_{SS}$  can be independently selected and each can range from  $0^\circ$  to  $32^\circ$ , from  $0.5^\circ$  to  $31.5^\circ$ , from  $0.1^\circ$  to  $31.0^\circ$ , from  $1.5^\circ$  to  $30.5^\circ$ , from  $2.0^\circ$  to  $30.0^\circ$ , from  $2.5^\circ$  to  $29.5^\circ$ , from  $3.0^\circ$  to  $29.0^\circ$ , from  $3.5^\circ$  to  $28.5^\circ$ , from  $4.0^\circ$  to  $28.0^\circ$ , from  $4.5^\circ$  to  $27.5^\circ$ , from  $5.0^\circ$  to  $27^\circ$ , from  $5.5^\circ$  to  $26.5^\circ$ , from  $6.0^\circ$  to  $26.0^\circ$ , from  $6.5^\circ$  to  $25.5^\circ$ , from  $7.0^\circ$  to  $25.0^\circ$ , from  $7.5^\circ$  to  $25.5^\circ$ , from  $8.0^\circ$  to  $26.0^\circ$ , from  $8.5^\circ$  to  $26.5^\circ$ , from  $9.0^\circ$  to  $26.0^\circ$ , from  $9.5^\circ$  to  $25.5^\circ$ , from  $10.0^\circ$  to  $25.0^\circ$ , from  $10.5^\circ$  to  $24.5^\circ$ , from  $11.0^\circ$  to  $24.0^\circ$ , from  $11.5^\circ$  to  $23.5^\circ$ , from  $12.0^\circ$  to  $23.0^\circ$ , from  $12.5^\circ$  to  $22.5^\circ$ , from  $13.0^\circ$  to  $22.0^\circ$ , from  $13.5^\circ$  to  $21.5^\circ$ , from  $14.5^\circ$  to  $21.0^\circ$ , from  $15.5^\circ$  to  $20.5^\circ$ , from  $16.0^\circ$  to  $20.0^\circ$ , from  $16.5^\circ$  to  $19.5^\circ$ , from  $17.0^\circ$  to  $19.0^\circ$ , or any range therein in increments of  $0.1^\circ$ . In some embodiments, each of  $\Theta_T$ ,  $\Theta_B$ ,  $\Theta_{FS}$ , and  $\Theta_{SS}$  can be independently selected and each can be about  $1^\circ$ ,  $2^\circ$ ,  $3^\circ$ ,  $4^\circ$ ,  $5^\circ$ ,  $6^\circ$ ,  $7^\circ$ ,  $8^\circ$ ,  $9^\circ$ ,  $10^\circ$ ,  $11^\circ$ ,  $12^\circ$ ,  $13^\circ$ ,  $14^\circ$ ,  $15^\circ$ ,  $16^\circ$ ,  $17^\circ$ ,  $18^\circ$ ,  $19^\circ$ ,  $20^\circ$ ,  $21^\circ$ ,  $22^\circ$ ,  $23^\circ$ ,  $24^\circ$ ,  $25^\circ$ ,  $26^\circ$ ,  $27^\circ$ ,  $28^\circ$ ,  $29^\circ$ ,  $30^\circ$ ,  $31^\circ$ ,  $32^\circ$ ,  $33^\circ$ ,  $34^\circ$ ,  $35^\circ$ , or any angle therein in increments of  $0.1^\circ$ .

[000102] It should be appreciated that the beams can each be independently designed to have its own, independently selected curvature, whether convex or concave, and the curvatures can be the same or different between beams that share a face of the frame. And, the curvatures can be opposing for beams that form opposing faces of the frame. Moreover, the frame can have a mixture of one or more straight and one or more curved beams.

[000103] Given the above, it should be appreciated that the frames can be designed according to nearly any opening bordered by the top vertebral endplate and bottom vertebral endplate of an intervertebral space, as well as according to a given clinical treatment regardless of the opening dimensions prior to treatment. In some embodiments, the top face of the frame can be at least substantially parallel to the bottom face of the frame, whereas the first side face of the frame and the second side face of the frame can be oriented at angles  $\Theta_T$  and  $\Theta_B$ , wherein  $\Theta_T$  and  $\Theta_B$  can be independently selected to be the same or different. Likewise, in some embodiments, the first side face of the frame can be at least substantially parallel to the second side face of the frame, whereas the top face of the frame and the bottom face of the frame can be oriented at angles  $\Theta_{FS}$  and  $\Theta_{SS}$ , wherein  $\Theta_{FS}$

and  $\Theta_{SS}$  can be independently selected to be the same or different. In some embodiments, each of  $\Theta_T$ ,  $\Theta_B$ ,  $\Theta_{FS}$ , and  $\Theta_{SS}$  can be independently selected to range from about  $5^\circ$  to about  $32^\circ$ , from about  $7^\circ$  to about  $22^\circ$ , and from about  $8^\circ$  to about  $16^\circ$ , in some embodiments. As such, any of a variety of frames can be constructed from any of a variety of quadrilateral structures having the angles taught herein.

[000104] In some embodiments, the systems include a stabilizer that slidably engages with the distal region of the first top beam, the first bottom beam, the second top beam, the second bottom beam, or a combination thereof. The stabilizer serves the function of the guide plate taught herein and can also be configured for retaining the first top beam, the first bottom beam, the second top beam, the second bottom beam, or the combination thereof, from a lateral movement that exceeds the expanded state.

[000105] And, in some embodiments, the framing can be configured for engaging with the central beam *in vivo* to support the framing in the expanded state. Moreover, the connector elements can be struts configured to have a cross-sectional aspect ratio of longitudinal thickness to transverse thickness ranging from 1:2 to 1:8, adapted to maintain structural stiffness in the laterovertically expanding frame in a direction perpendicular to the central frame axis of the expanded state of the frame.

[000106] FIGs. 14A-14D illustrate components of a system having a stabilizer, wherein the stabilizer is in an X-configuration, according to some embodiments. As shown in FIG. 14A, the system 1400 can include a stabilizer 1407 that can be in an X-configuration. In some embodiments, the X-configuration can have a first top leg  $TL_1$  for slidably-engaging with the first top beam 1450 at an angle  $\Theta_{1T}$  with the intended lateral movement  $LM_{1T}$  of the first top beam 1450, first bottom leg  $BL_1$  for slidably engaging with the first bottom beam 1470 at an angle  $\Theta_{1B}$  with the intended lateral movement  $LM_{1B}$  of the first bottom beam 1470, a second top leg  $TL_2$  for slidably engaging with the second top beam 1460 at an angle  $\Theta_{2T}$  with the intended lateral movement  $LM_{2T}$  of the second top beam 1460, and a second bottom leg  $BL_2$  for slidably engaging with the second bottom beam 1480 at an angle  $\Theta_{2B}$  with the intended lateral movement  $LM_{2B}$  of the second bottom beam 1480.

[000107] In some embodiments, each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$ , respectively, provide a tensile force for resisting the first top beam 1450, the first bottom beam 1470, the second top beam 1460, and the second bottom beam 1480 from the lateral movement  $LM_{1T}$ ,  $LM_{2T}$ ,  $LM_{1B}$ ,  $LM_{2B}$  that exceeds the expanded state. In some embodiments, each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$  can be independently selected from an amount of angulation

ranging from about 15° to about 75°, from about 20° to about 75°, from about 25° to about 75°, from about 30° to about 75°, from about 35° to about 75°, from about 55° to about 75°, from about 15° to about 70°, from about 15° to about 65°, from about 15° to about 60°, from about 15° to about 55°, from about 15° to about 50°, from about 15° to about 45°, or any range therein. In some embodiments, each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$  can be independently selected from an amount of angulation that is about 10°, about 15°, about 20°, about 25°, about 30°, about 35°, about 40°, about 45°, about 50°, about 55°, about 60°, about 65°, about 70°, about 75°, about 80°, or any angulation therein in amounts of 1°.

[000108] In some embodiments, the stabilizer 1407 further comprises a point of attachment 1408 for releasably attaching a guidewire (not shown) for guiding the central beam 1401 into the laterover vertically expanding frame comprising the first top beam 1450, the second top beam 1460, the first bottom beam 1470, and the second bottom beam 1480. And, in some embodiments, the first top leg  $TL_1$ , the first bottom leg  $BL_1$ , the second top leg  $TL_2$ , and the second bottom leg  $BL_2$  converge to form a hub 1408H having a point of attachment 1408 on the posterior surface of the hub 1408H for releasably attaching a guidewire (not shown) for guiding the central beam 1401 into the laterover vertically expanding frame. The point of attachment might be, for example, a male or female threaded component, or any other releasable connector known to one of skill. And, the beams 1450, 1460, 1470, 1480 can be configured with ports  $TP_1, TP_2, BP_1, BP_2$  for passage of the respective legs  $TL_1, TL_2, BL_1, BL_2$  of the stabilizer 1407. FIGs. 14B and 14C show the system in a collapsed configuration and expanded side configuration, respectively. In some embodiments, the central beam 1401 can include one or more bone graft distribution ports 1466. And, as in other embodiments taught herein, the beams 1450, 1460, 1470, 1480 can be interconnected using flexible struts 1495.

[000109] FIGs. 15A-15D illustrate components of a system having a stabilizer, wherein the stabilizer is in an H-configuration, according to some embodiments. The H-configuration can have a first vertical leg  $VL_1$ , a second vertical leg  $VL_2$ , and a cross-member CM that connects the first vertical leg  $VL_1$  at least substantially parallel to the second vertical leg  $VL_2$ , the first vertical leg  $VL_1$  including a first retaining surface  $RS_1$  for engaging with the first top beam 1550 and the first bottom beam 1570, the second vertical leg  $VL_2$  including a second retaining surface  $RS_2$  for engaging with the second top beam 1560 and the second bottom beam 1580, and the cross member CM providing a tensile force for resisting the first top beam 1550, the first bottom beam 1570, the second top beam 1560, and the second bottom

beam 1580 from the lateral movement that exceeds the expanded state. In some embodiments, the central beam 1501 has a horizontal groove HG configured complementary to the cross-member CM of the stabilizer 1507, and the horizontal groove HG of the central beam 1501 slidably connects with the cross-member CM in the expanded state. In some embodiments, the cross-member CM further comprises a vertical support member VSM and the central beam 1501 has a vertical groove VG configured complementary to the vertical support member VSM of the stabilizer, and the vertical groove VG of the central beam 1501 slidably connects with the vertical support member VSM in the expanded state. In some embodiments, the stabilizer 1507 further comprises a point of attachment 1508 at a hub 1508H for releasably attaching a guidewire (not shown) adapted for guiding the central beam 1501 into the lateroververtically expanding frame comprising the first top beam 1550, the second top beam 1560, the first bottom beam 1570, and the second bottom beam 1580. guidewire (not shown) for guiding the central beam 1501 into the lateroververtically expanding frame. The point of attachment might be, for example, a male or female threaded component, or any other releasable connector known to one of skill. And, the beams 1550,1560,1570,1580 can be configured with slots  $S_1, S_2$  in which the vertical legs  $VL_1, VL_2$  can travel during the lateral expansion of the beams 1550,1560,1570,1580 of the expandable frame. And, in some embodiments, cross-member CM includes a first pillar  $P_1$  and a second pillar  $P_2$  that operably connect at a hub that has the point of attachment 1508 for releasably attaching the guidewire (not shown) for guiding the central beam 1501 into the lateroververtically expanding frame. In some embodiments, the central beam 1501 can include one or more bone graft distribution ports 1566. And, as in other embodiments taught herein, the beams 1550,1560,1570,1580 can be interconnected using flexible struts 1595.

[000110] One of skill will appreciate that the teachings provided herein are directed to basic concepts that can extend beyond any particular embodiment, embodiments, figure, or figures. It should be appreciated that any examples are for purposes of illustration and are not to be construed as otherwise limiting to the teachings. For example, it should be appreciated that the devices provided herein can also be used as implants in other areas of the body. The devices provided herein can be used, for example, in intravertebral body procedures to support or distract vertebral bodies in the repair of, for example, collapsed, damaged or unstable vertebral bodies suffering from disease or injury.

## WE CLAIM

1. An intervertebral scaffolding system, comprising;  
a central beam having
  - a central beam axis;
  - a proximal portion and a distal portion;
  - a top surface with a first top-lateral surface and a second top-lateral surface;
  - a bottom surface with a first bottom-lateral surface and a second bottom-lateral surface;
  - a first side surface with a first top-side surface and a first bottom-side surface; and,
  - a second side surface with a second top-side surface and a second bottom-side surface;a laterover vertically-expanding frame configured for operably contacting the central beam to create an intervertebral scaffolding system *in vivo*, the frame having
  - a collapsed state and an expanded state, the expanded state operably contacting with the central beam in the intervertebral space;
  - a proximal portion having an end, a distal portion having an end, and a central frame axis of the expanded state;
  - a first top beam including a proximal portion having an end and a distal portion having an end, the first top beam configured for contacting the first top-lateral surface of the central beam and the first top-side surface of the central beam in the expanded state, a central axis of the first top beam at least substantially on (i) a top plane containing the central axis of the first top beam and a central axis of a second top beam and (ii) a first side plane containing the central axis of the first top beam and a central axis of a first bottom beam;
  - the second top beam including a proximal portion having an end and a distal portion having an end, the second top beam configured for contacting the second top-lateral surface of the central beam and the second top-side surface of the central beam in the expanded state, the central axis of the second top beam at least substantially on (i) the top plane and (ii) a second side plane containing the central axis of the second top beam and a central axis of a second bottom beam;

the first bottom beam including a proximal portion having an end and a distal portion having an end, the first bottom beam configured for contacting the first bottom-lateral surface of the central beam and the first bottom-side surface of the central beam in the expanded state, the central axis of the first bottom beam at least substantially on (i) a bottom plane containing the central axis of the first bottom beam and the central axis of the second top beam and (ii) the first side plane;

the second bottom beam including a proximal portion having an end and a distal region having an end, the second bottom beam configured for contacting the second bottom-lateral surface of the central beam and the second bottom-side surface of the central beam in the expanded state, the central axis of the second bottom beam being at least substantially on (i) the bottom plane and (ii) a second side plane containing the central axis of the second bottom beam and the central axis of the second top beam;

a plurality of top connector elements configured to expandably connect the first top beam to the second top beam, the expanding consisting of a flexing at least substantially on the top plane;

a plurality of bottom connector elements configured to expandably connect the first bottom beam to the second bottom beam, the expanding consisting of a flexing at least substantially on the bottom plane;

a plurality of first side connector elements configured to expandably connect the first top beam to the first bottom beam, the expanding consisting of a flexing at least substantially on the first side plane;

a plurality of second side connector elements configured to expandably connect the second top beam to the second bottom beam, the expanding consisting of a flexing at least substantially on the second side plane;

and,

a stabilizer that slidably engages with the distal region of the first top beam, the first bottom beam, the second top beam, the second bottom beam, or a combination thereof, and is configured for retaining the first top beam, the first bottom beam, the second top beam, the second bottom beam, or the combination thereof, from a lateral movement that exceeds the expanded state;

wherein,

the framing is configured for engaging with the central beam *in vivo* to support the framing in the expanded state; and,

the connector elements are struts configured to have a cross-sectional aspect ratio of longitudinal thickness to transverse thickness ranging from 1:2 to 1:8, adapted to maintain structural stiffness in the laterover vertically expanding frame in a direction perpendicular to the central frame axis of the expanded state of the frame.

2. The scaffolding system of claim 1, wherein the stabilizer is in an X-configuration having a first top leg for slidably-engaging with the first top beam at an angle  $\Theta_{1T}$  with the lateral movement of the first top beam, first bottom leg for slidably engaging with the first bottom beam at an angle  $\Theta_{1B}$  with the lateral movement of the first bottom beam, a second top leg for slidably engaging with the second top beam at an angle  $\Theta_{2T}$  with the lateral movement of the second top beam, and a second bottom leg for slidably engaging with the second bottom beam at an angle  $\Theta_{2B}$  with the lateral movement of the second bottom beam, wherein each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$ , respectively, provide a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state.
3. The scaffolding system of claim 1, wherein the stabilizer is in an X-configuration having a first top leg for slidably-engaging with the first top beam at an angle  $\Theta_{1T}$  with the lateral movement of the first top beam, first bottom leg for slidably engaging with the first bottom beam at an angle  $\Theta_{1B}$  with the lateral movement of the first bottom beam, a second top leg for slidably engaging with the second top beam at an angle  $\Theta_{2T}$  with the lateral movement of the second top beam, and a second bottom leg for slidably engaging with the second bottom beam at an angle  $\Theta_{2B}$  with the lateral movement of the second bottom beam, wherein each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$ , respectively, provide a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state;

wherein the stabilizer further comprises a point of attachment for releasably attaching a guidewire for guiding the central beam into the laterover vertically expanding frame.

4. The scaffolding system of claim 1, wherein the stabilizer is in an X-configuration having a first top leg for slidably-engaging with the first top beam at an angle  $\Theta_{1T}$  with the lateral movement of the first top beam, first bottom leg for slidably engaging with the first bottom beam at an angle  $\Theta_{1B}$  with the lateral movement of the first bottom beam, a second top leg for slidably engaging with the second top beam at an angle  $\Theta_{2T}$  with the lateral movement of the second top beam, and a second bottom leg for slidably engaging with the second bottom beam at an angle  $\Theta_{2B}$  with the lateral movement of the second bottom beam, wherein each of the angles  $\Theta_{1T}$ ,  $\Theta_{1B}$ ,  $\Theta_{2T}$ ,  $\Theta_{2B}$ , respectively, provide a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state;

wherein the first top leg, the first bottom leg, the second top leg, and the second bottom leg converge to form a hub having a point of attachment for releasably attaching a guidewire for guiding the central beam into the lateroververtically expanding frame.

5. The scaffolding system of claim 1, wherein the stabilizer is in an H-configuration having a first vertical leg, a second vertical leg, and a cross-member that connects the first vertical leg at least substantially parallel to the second vertical leg, the first vertical leg including a retaining surface for engaging with the first top beam and the first bottom beam, the second vertical leg including a retaining surface for engaging with the second top beam and the second bottom beam, and the cross member providing a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state.
6. The scaffolding system of claim 1, wherein the stabilizer is in an H-configuration having a first vertical leg, a second vertical leg, and a cross-member that connects the first vertical leg at least substantially parallel to the second vertical leg, the first vertical leg including a retaining surface for engaging with the first top beam and the first bottom beam, the second vertical leg including a retaining surface for engaging with the second top beam and the second bottom beam, and the cross member providing a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state;

wherein, the central beam has a horizontal groove configured complementary to the cross-member of the stabilizer, and the horizontal groove of the central beam slidably connects with the cross-member in the expanded state.

7. The scaffolding system of claim 1, wherein the stabilizer is in an H-configuration having a first vertical leg, a second vertical leg, a cross-member that connects the first vertical leg at least substantially parallel to the second vertical leg, the first vertical leg including a retaining surface for engaging with the first top beam and the first bottom beam, the second vertical leg including a retaining surface for engaging with the second top beam and the second bottom beam, and the cross member providing a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state;

wherein, the cross-member further comprises a vertical support member and the central beam has a vertical groove configured complementary to the vertical support member of the stabilizer, and the vertical groove of the central beam slidably connects with the vertical support member in the expanded state.

8. The scaffolding system of claim 1, wherein the stabilizer is in an H-configuration having a first vertical leg, a second vertical leg, a cross-member that connects the first vertical leg at least substantially parallel to the second vertical leg, the first vertical leg including a retaining surface for engaging with the first top beam and the first bottom beam, the second vertical leg including a retaining surface for engaging with the second top beam and the second bottom beam, and the cross member providing a tensile force for resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state;

wherein, the stabilizer further comprises a point of attachment for releasably attaching a guidewire adapted for guiding the central beam into the laterover vertically expanding frame.

9. The scaffolding system of claim 1, wherein the stabilizer is in an H-configuration having a first vertical leg, a second vertical leg, a cross-member that connects the first vertical leg at least substantially parallel to the second vertical leg, the first vertical leg including a retaining surface for engaging with the first top beam and the first bottom beam, the second vertical leg including a retaining surface for engaging with the second top beam and the second bottom beam, and the cross member providing a tensile force for

resisting the first top beam, the first bottom beam, the second top beam, and the second bottom beam from the lateral movement that exceeds the expanded state;

wherein, cross-member includes a first pillar and a second pillar that operably connect at a hub that has a point of attachment for releasably attaching a guidewire for guiding the central beam into the laterover vertically expanding frame.

10. The scaffolding system of claim 1, the central beam further comprising a grafting port.

11. The scaffolding system of claim 1, wherein each plurality connector elements are struts; wherein,

the top struts are configured monolithically integral to the first top beam and the second top beam; and,

the bottom struts are configured monolithically integral to the first bottom beam and the second bottom beam;

wherein, the top struts and bottom struts of the laterover vertically-expanding frame are each configured to open a graft distribution window upon expansion, expanding from the first top beam to the second top beam, the first top beam to the first bottom beam, the second top beam to the second bottom beam, or the first bottom beam to the second bottom beam.

12. The scaffolding system of claim 1, wherein,

the top connector struts are configured monolithically integral to the first top beam and the second top beam; and,

the bottom struts are configured monolithically integral to the first bottom beam and the second bottom beam;

the first side struts are configured monolithically integral to the first top beam and the first bottom beam; and,

the second side struts are configured monolithically integral to the second top beam and the second bottom beam;

wherein, the top, bottom, first side, and second side of the laterover vertically-expanding frame form a monolithically integral frame.

13. A method of fusing an intervertebral space using the scaffolding system of claim 1, the method comprising:

creating a point of entry into an intervertebral disc, the intervertebral disc having a nucleus pulposus surrounded by an annulus fibrosis;

removing the nucleus pulposus from within the intervertebral disc through the point of entry, leaving the intervertebral space for expansion of the scaffolding system of claim 1 within the annulus fibrosis, the intervertebral space having a top vertebral plate and a bottom vertebral plate;

inserting the laterover vertically expanding frame in the collapsed state through the point of entry into the intervertebral space;

inserting the central beam into the frame to form the scaffolding system;

and,

adding a grafting material to the intervertebral space.

14. The method of claim 12, wherein the creating the point of entry comprises creating a lateral dimension of the point of entry ranging from about 5 mm to about 15 mm, and the amount of lateral expansion is selected to exceed the lateral dimension of the point of entry.

15. The method of claim 10, wherein the expanding includes

expanding the laterover vertically expanding frame laterally to a width that exceeds the width of the point of entry; and,

inserting the central beam to expand the laterover vertically expanding frame vertically to support the frame in the expanded state.

16. The method of claim 10, wherein the inserting of the central beam into the laterover vertically expanding frame includes engaging a means for preventing the central beam from backing out of the laterover vertically-expanding frame after the expanding.

17. A kit, comprising:

the scaffolding system of claim 1;

a cannula for inserting the scaffolding system into the intervertebral space; and,

a guidewire adapted for guiding the central beam into the laterover vertically expanding frame.

18. A kit, comprising:

the scaffolding system of claim 2;

a cannula for inserting the scaffolding system into the intervertebral space; and,

a guidewire adapted for guiding the central beam into the laterover vertically expanding frame.

19. A kit, comprising:

the scaffolding system of claim 4;

a cannula for inserting the scaffolding system into the intervertebral space; and,

a guidewire adapted for guiding the central beam into the laterover vertically expanding frame.

20. A kit, comprising:

the scaffolding system of claim 6;

a cannula for inserting the scaffolding system into the intervertebral space; and,

a guidewire adapted for guiding the central beam into the laterover vertically expanding frame.

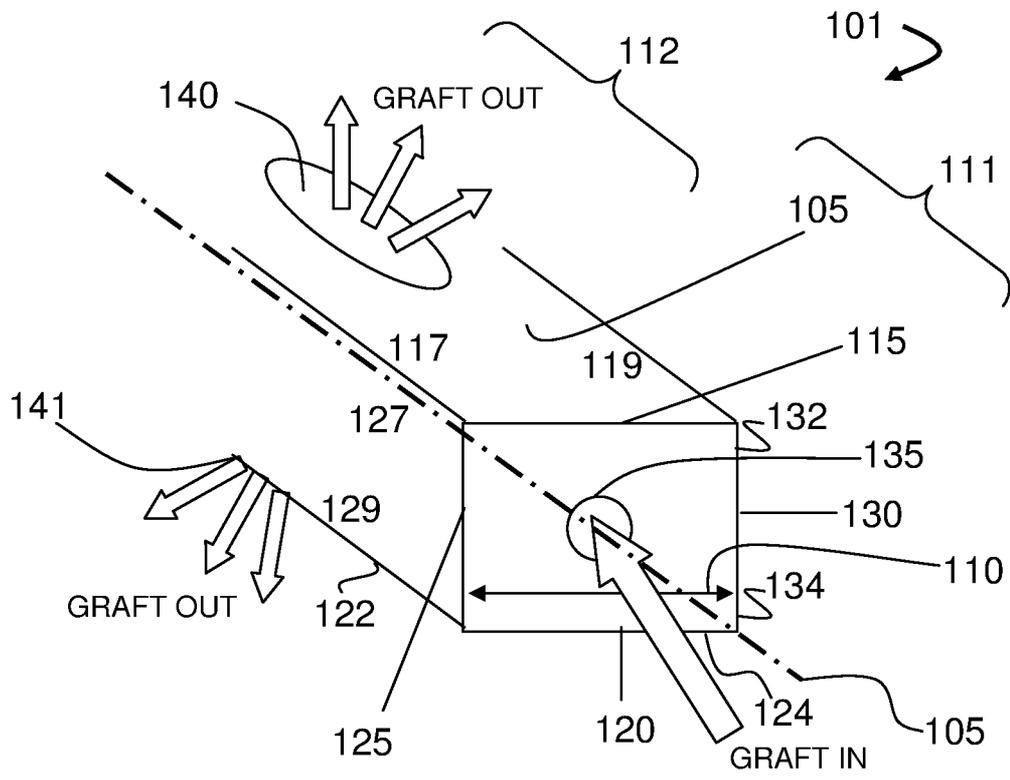


FIG. 1A

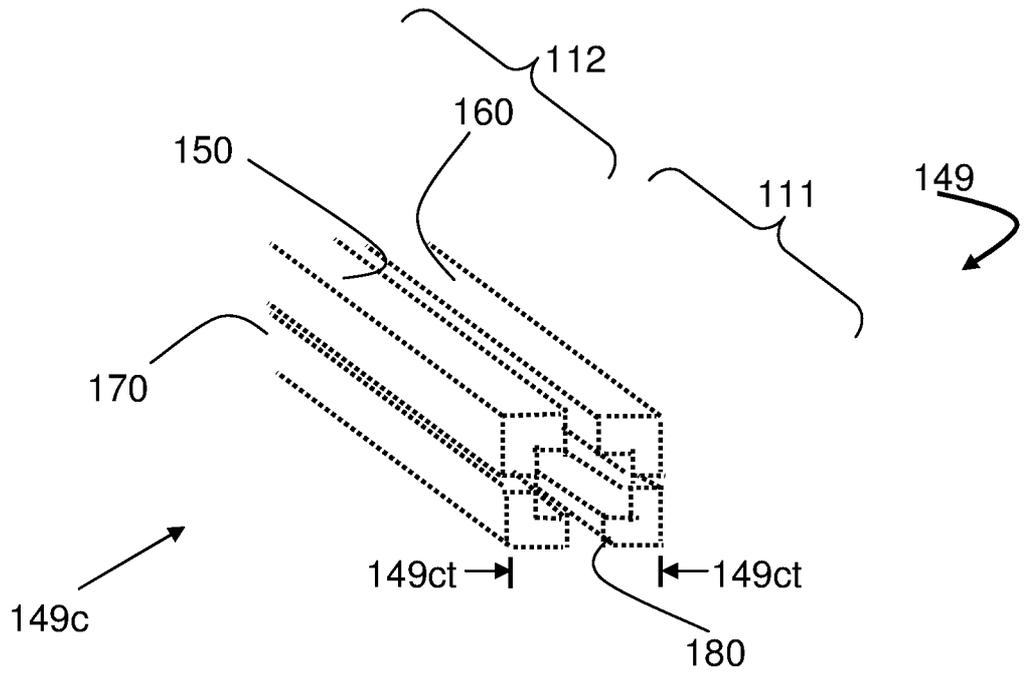


FIG. 1B

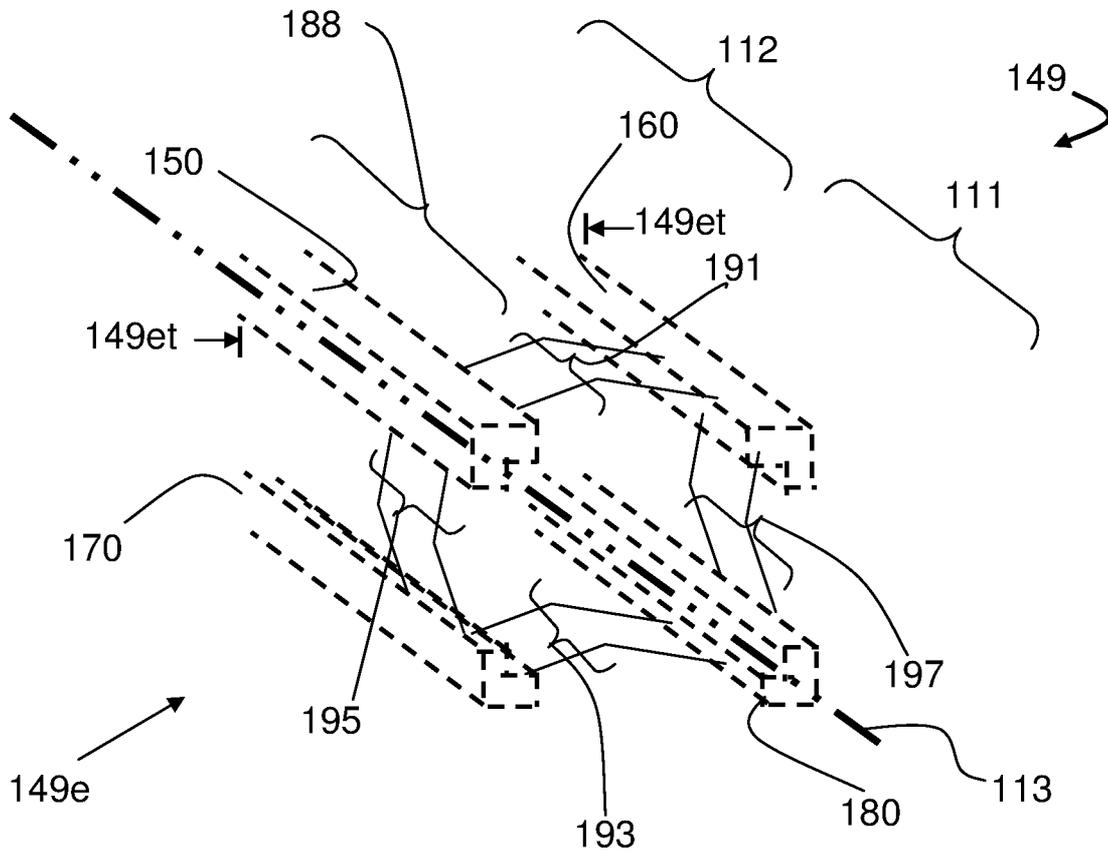


FIG. 1C

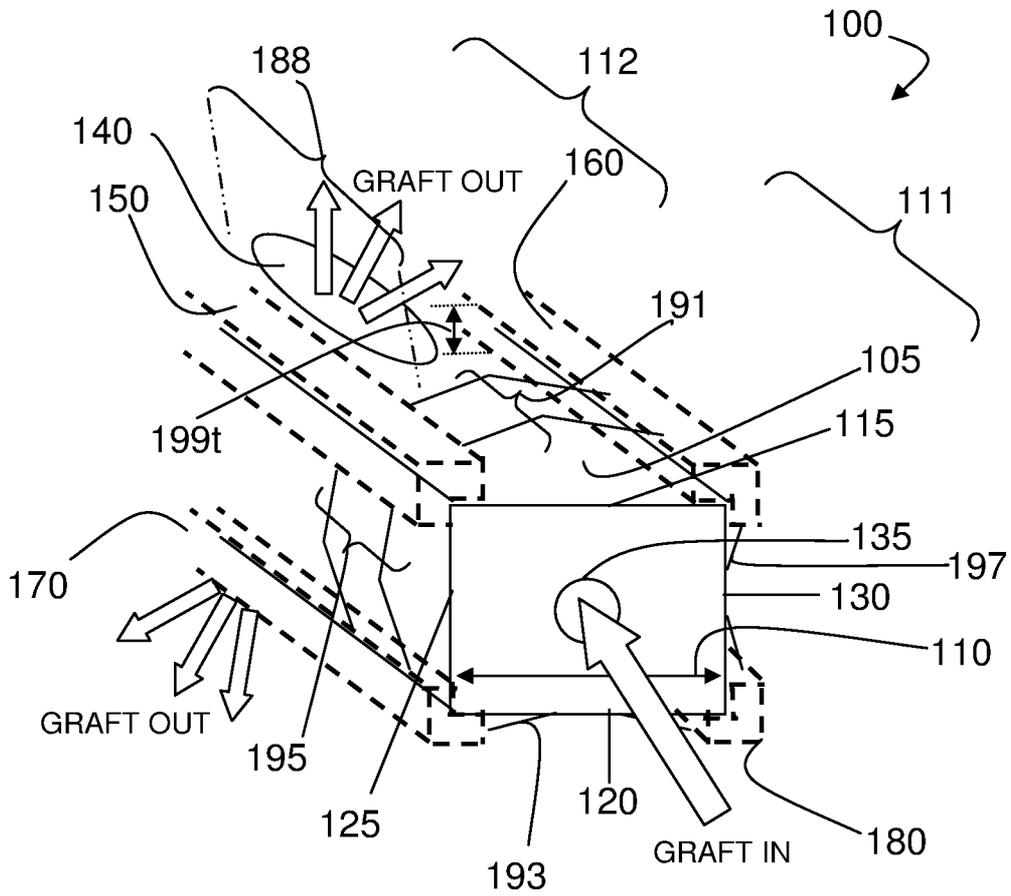


FIG. 1D

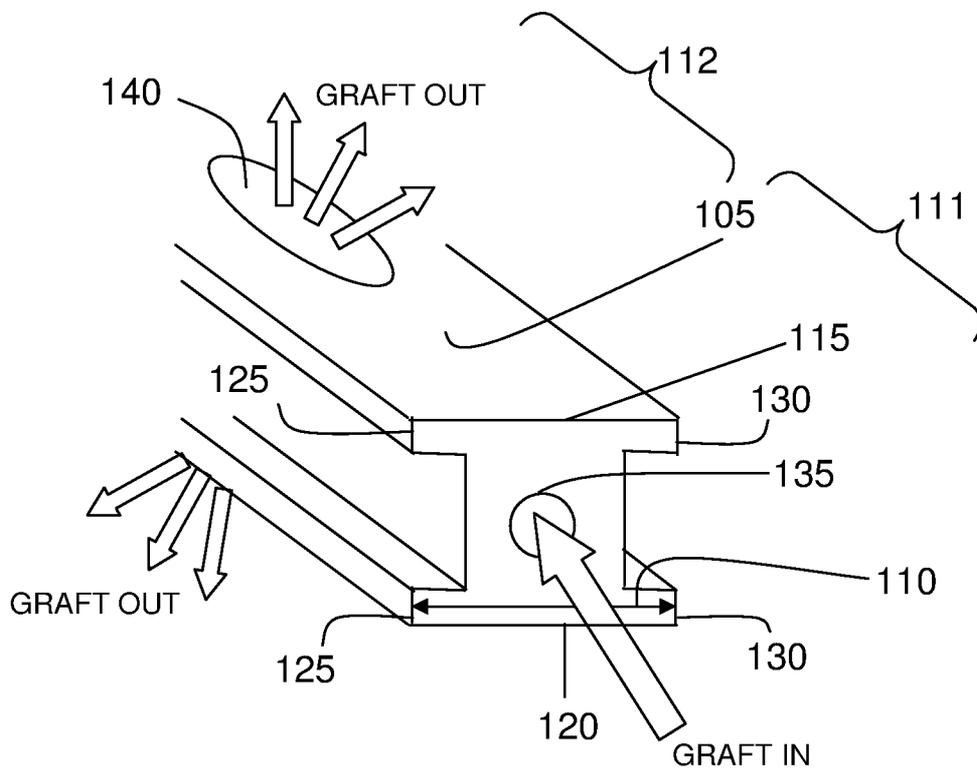


FIG. 1E

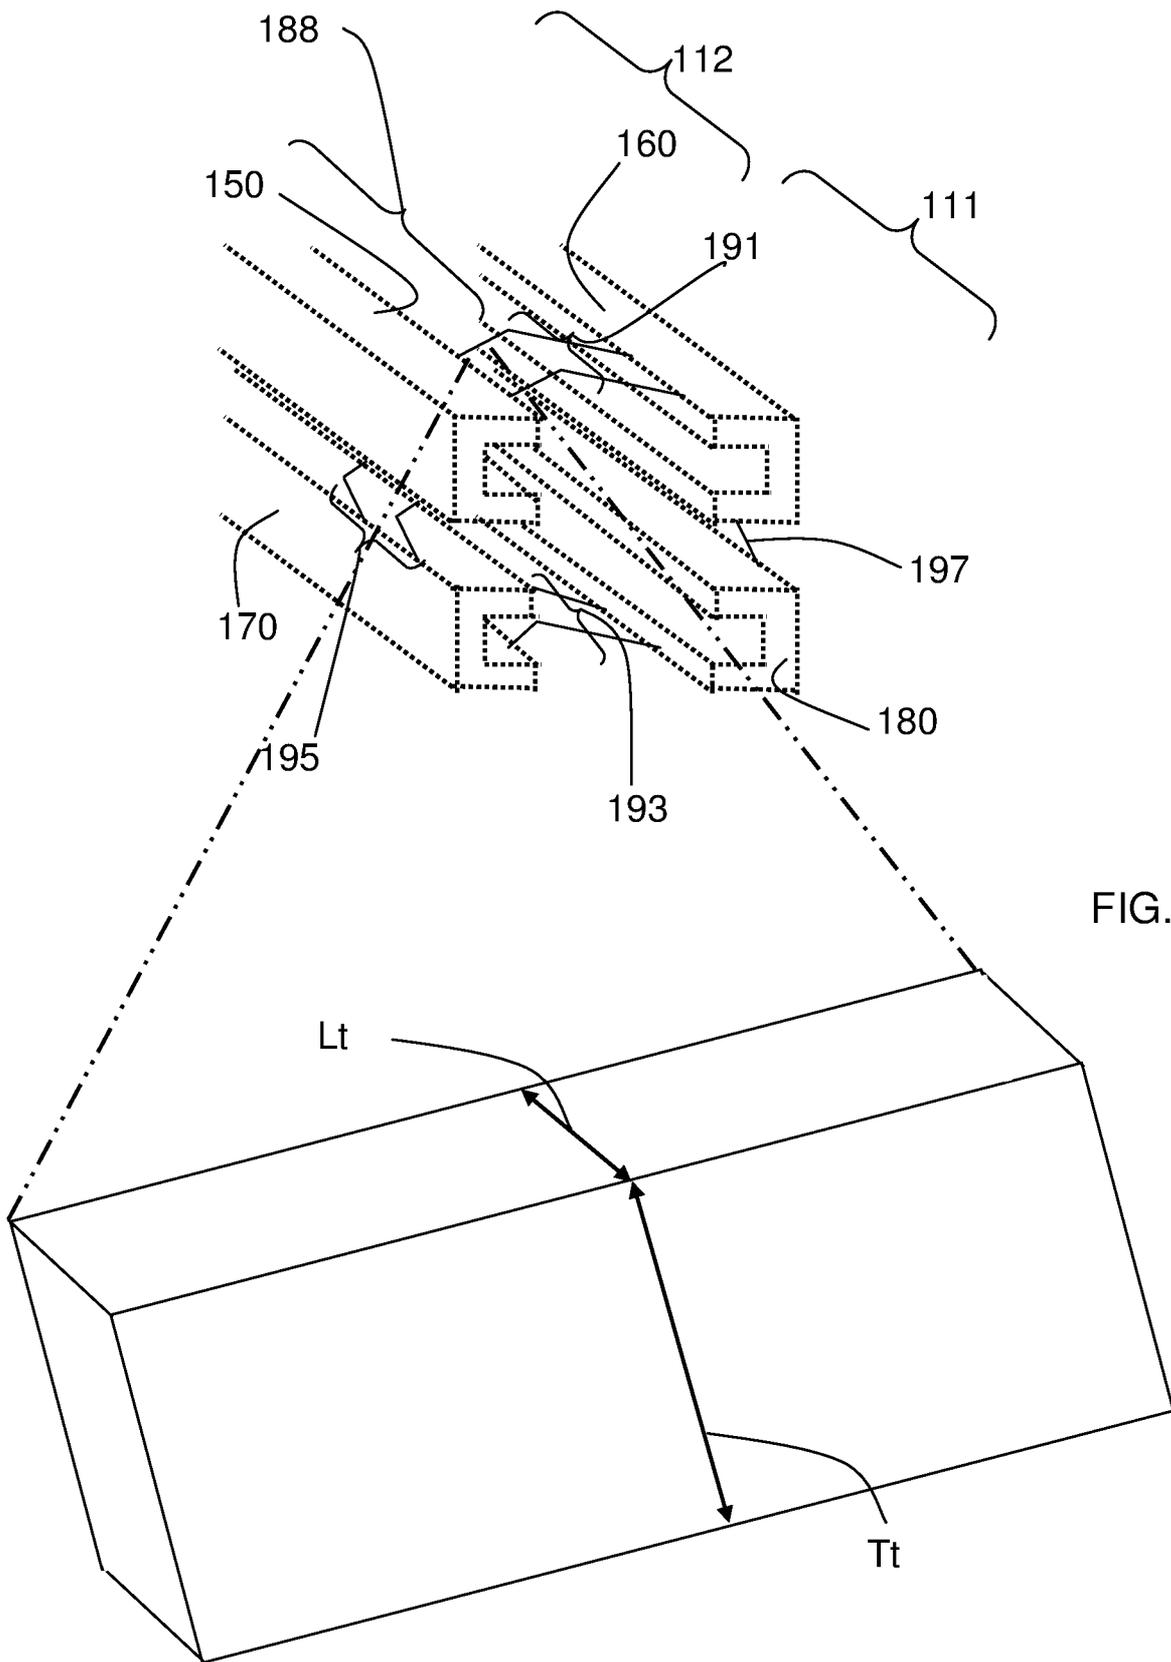


FIG. 1F

FIG. 1G

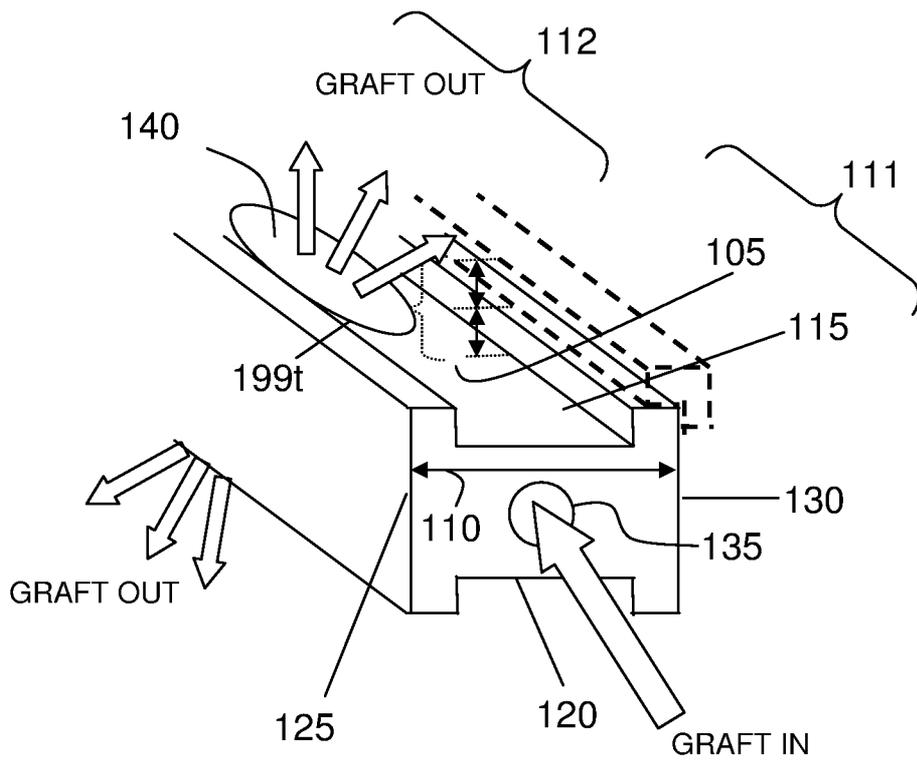


FIG. 1H

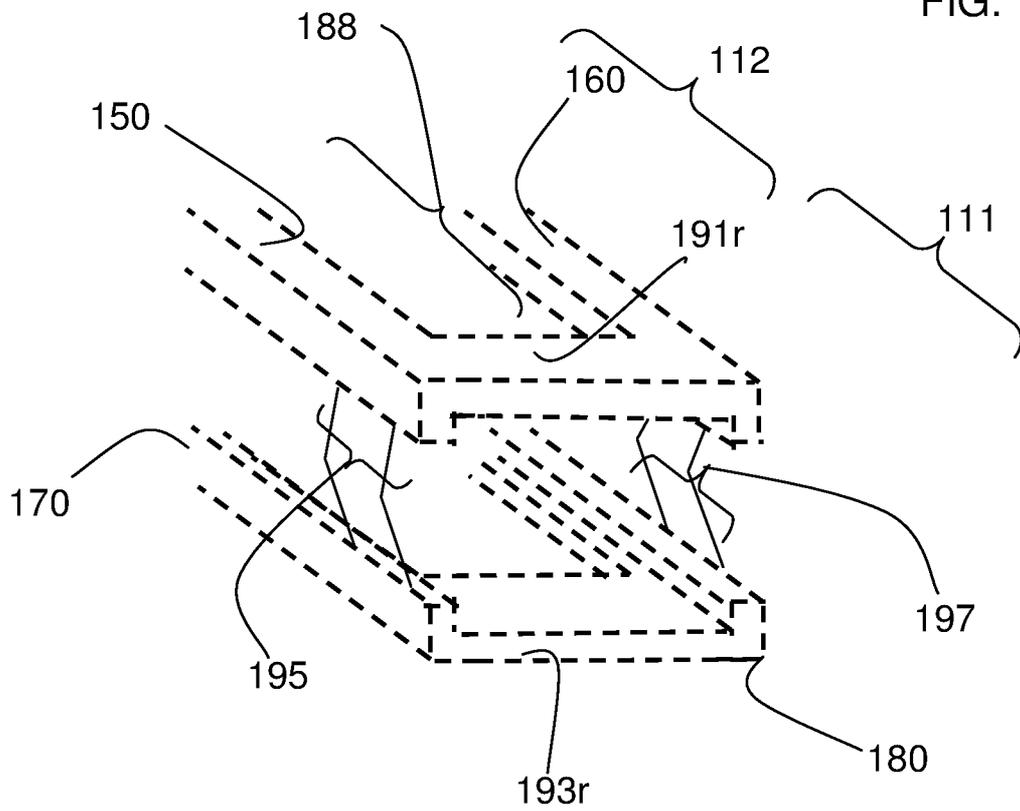


FIG. 1I

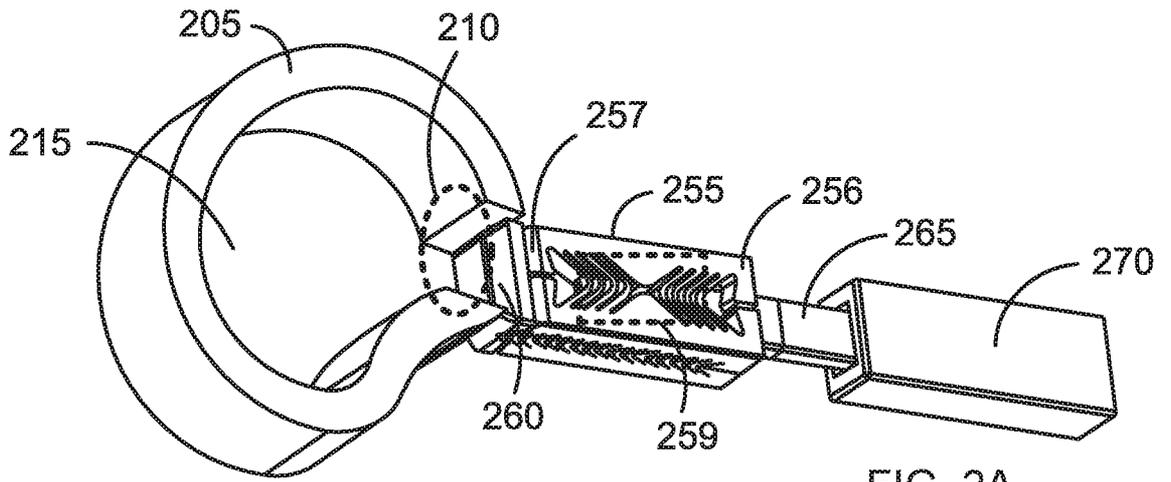


FIG. 2A

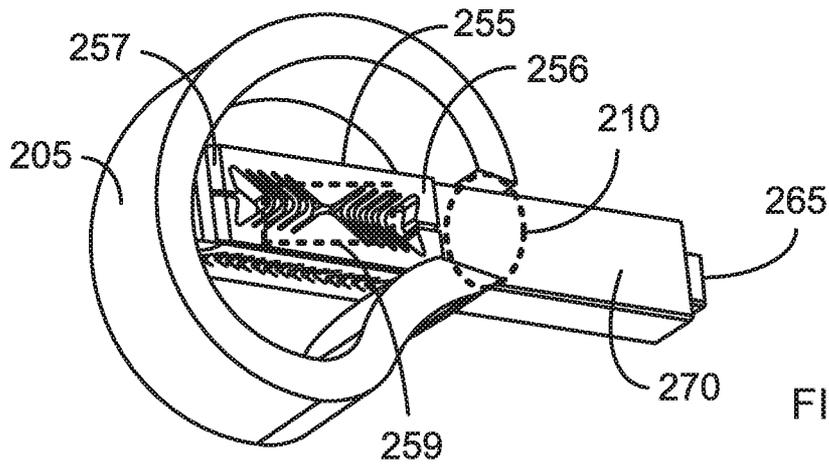


FIG. 2B

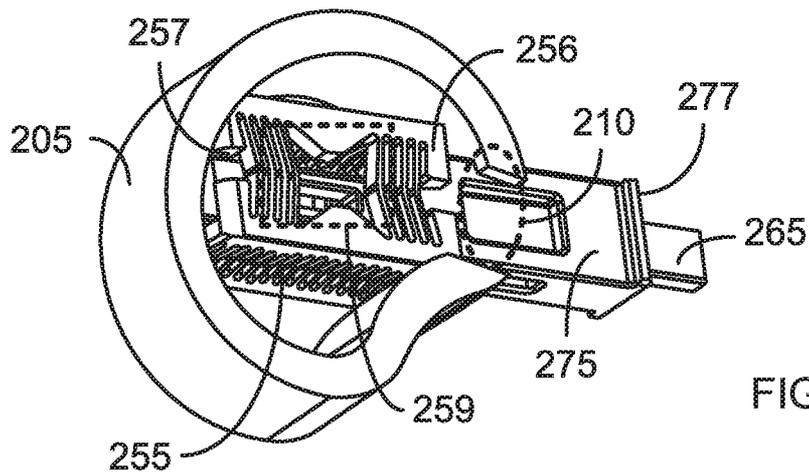


FIG. 2C

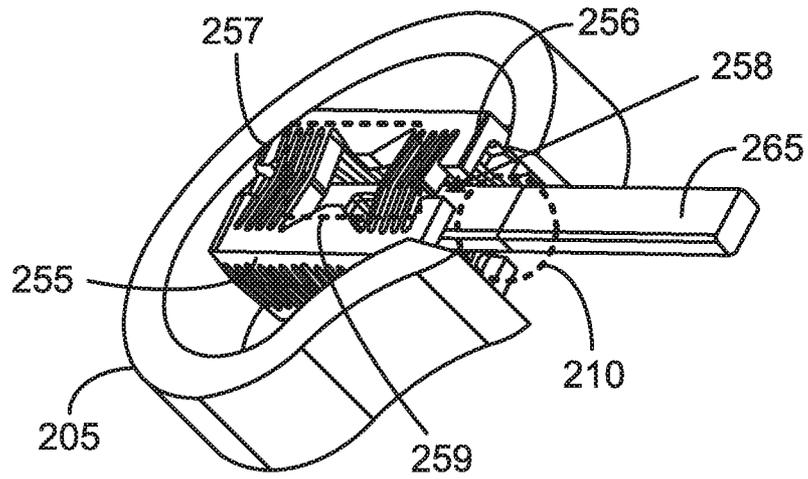


FIG. 2D

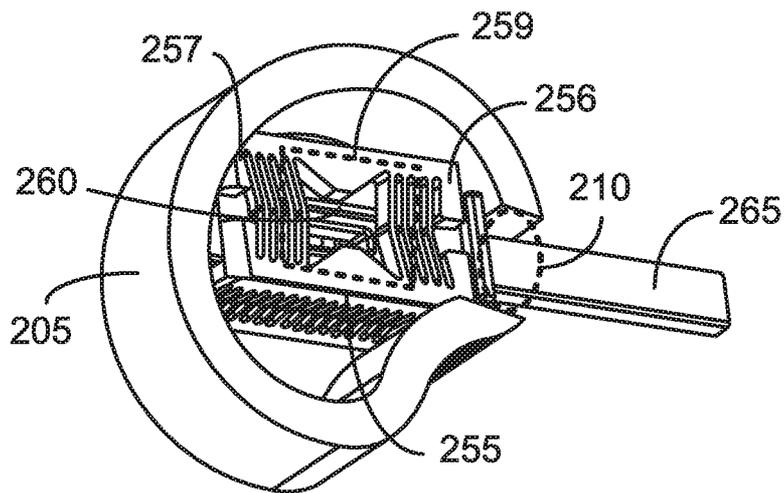


FIG. 2E

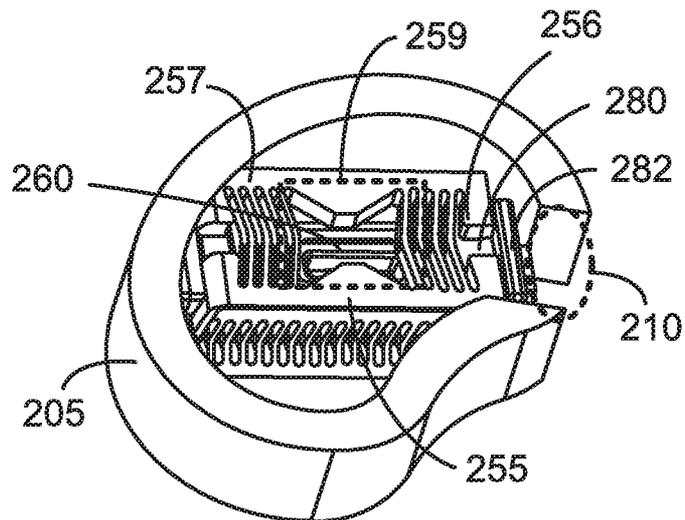


FIG. 2F

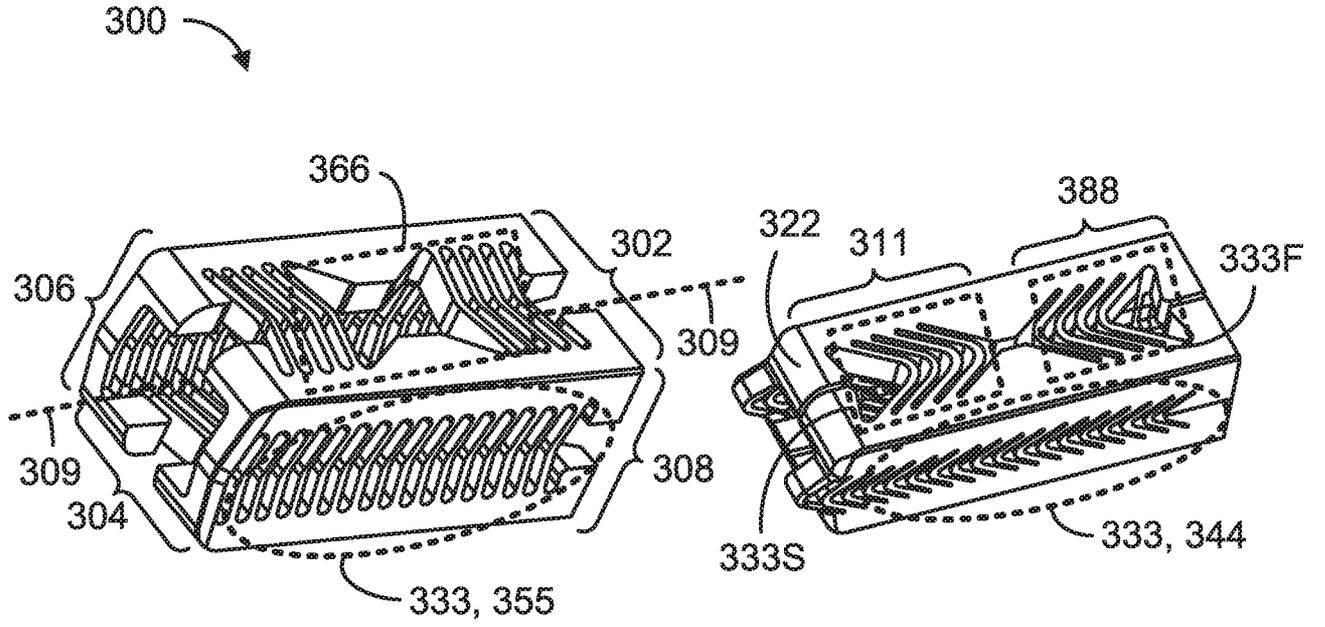


FIG. 3A

FIG. 3B

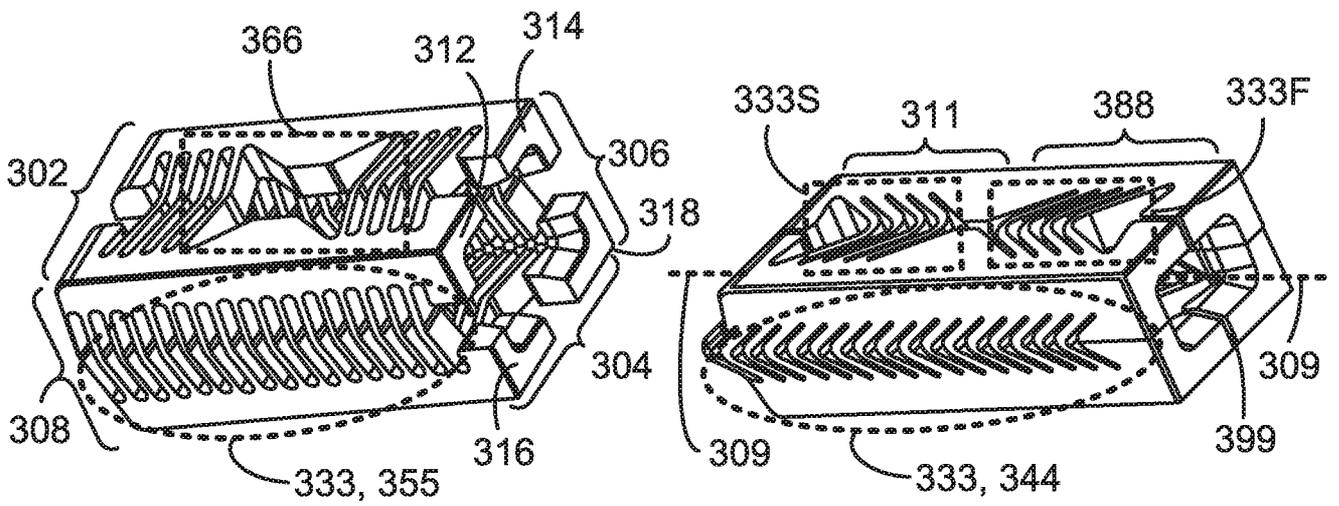


FIG. 3C

FIG. 3D

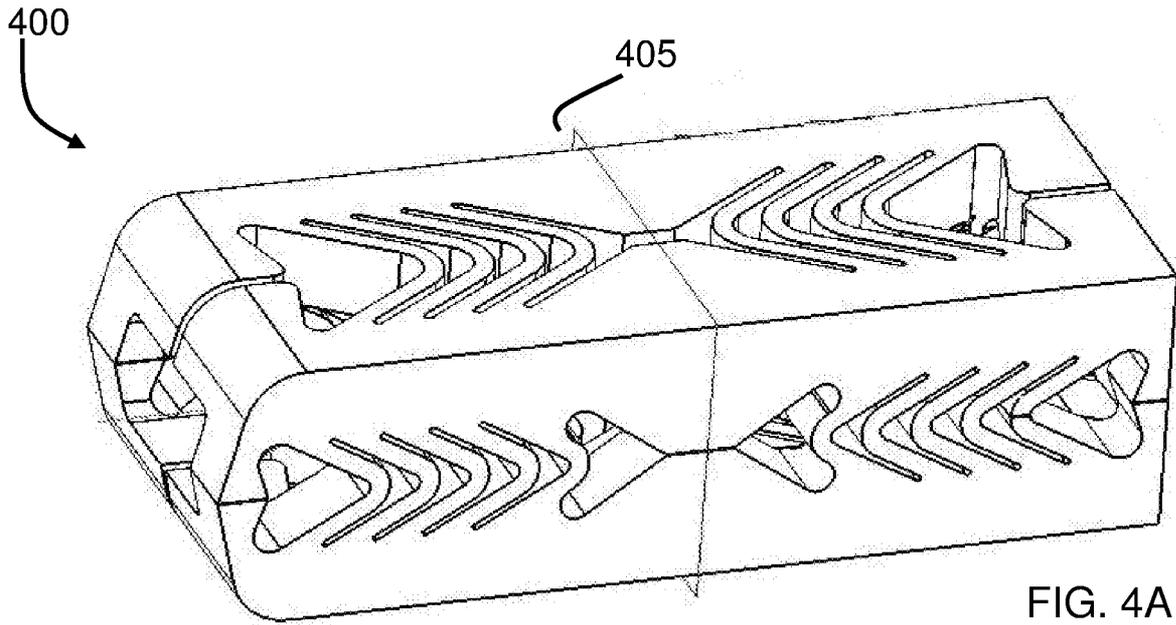


FIG. 4A

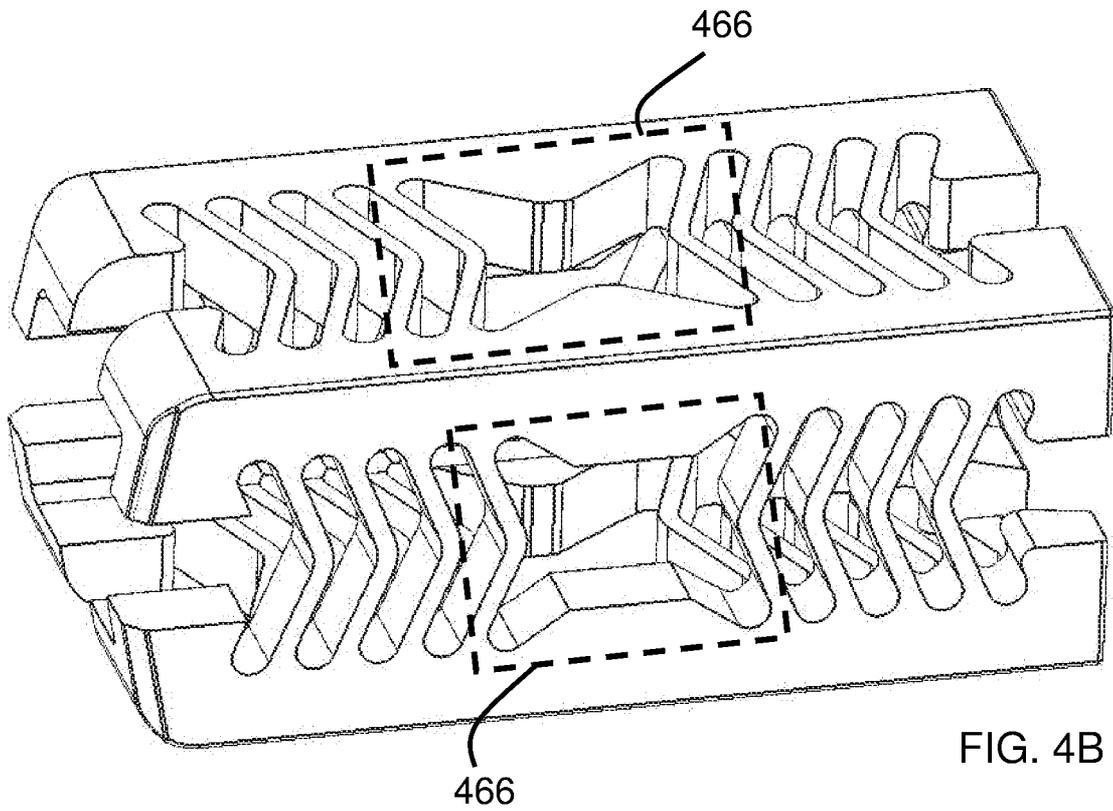
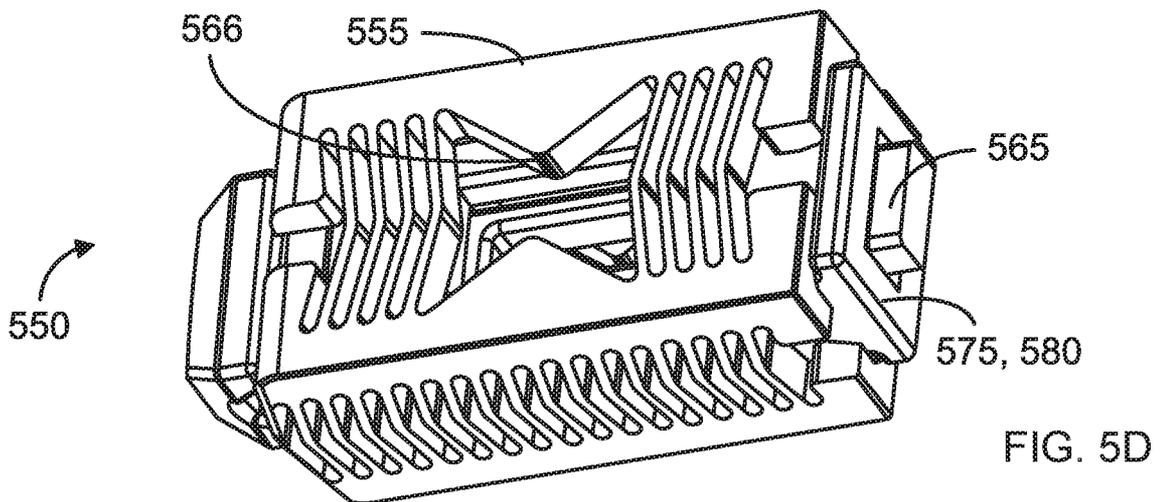
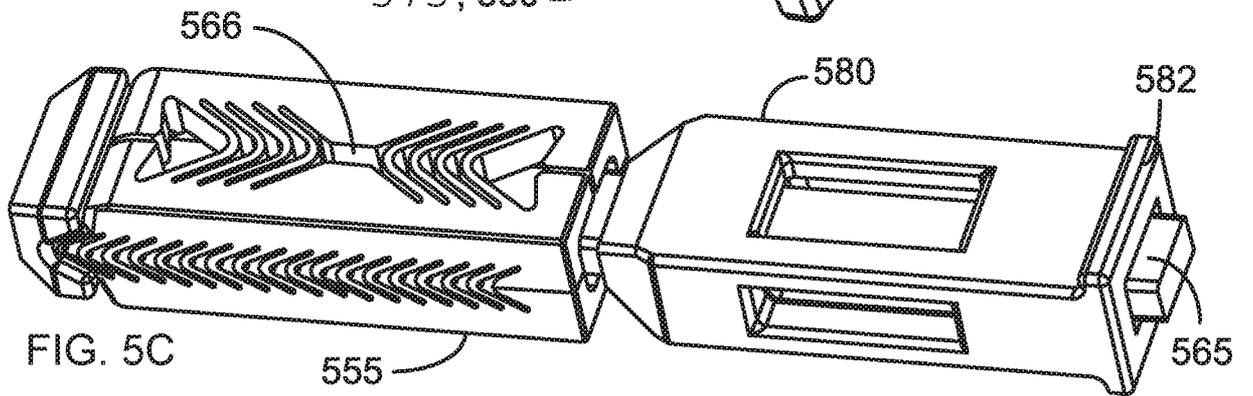
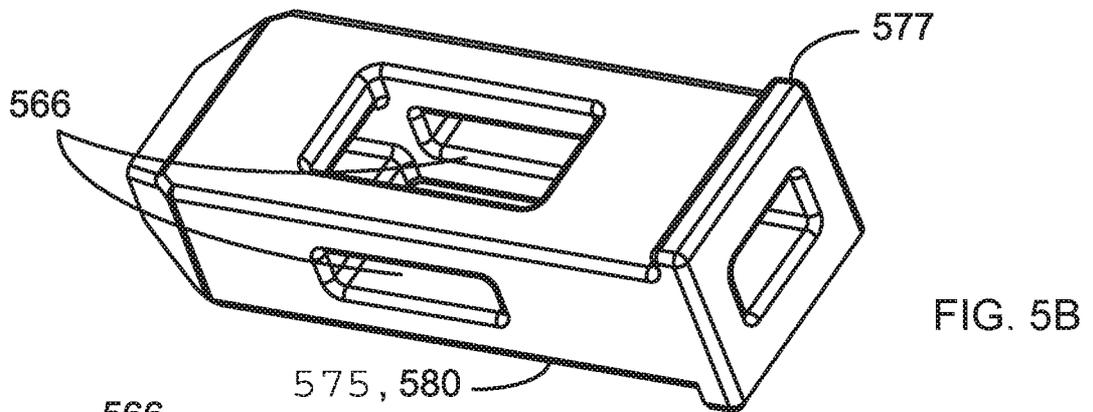
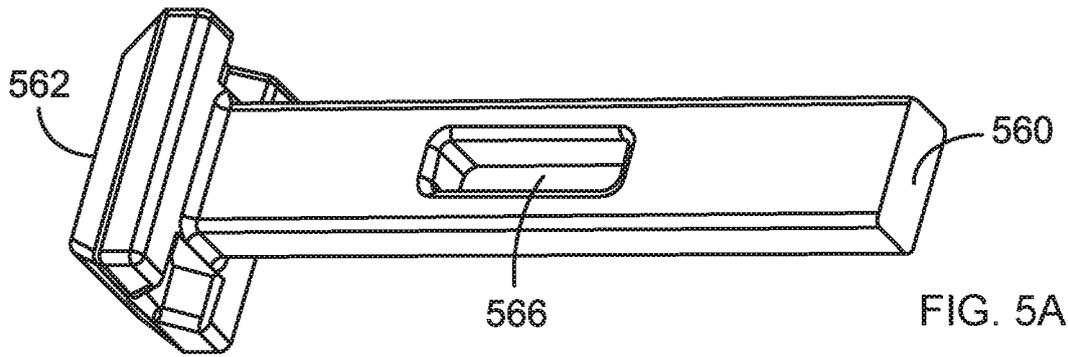


FIG. 4B



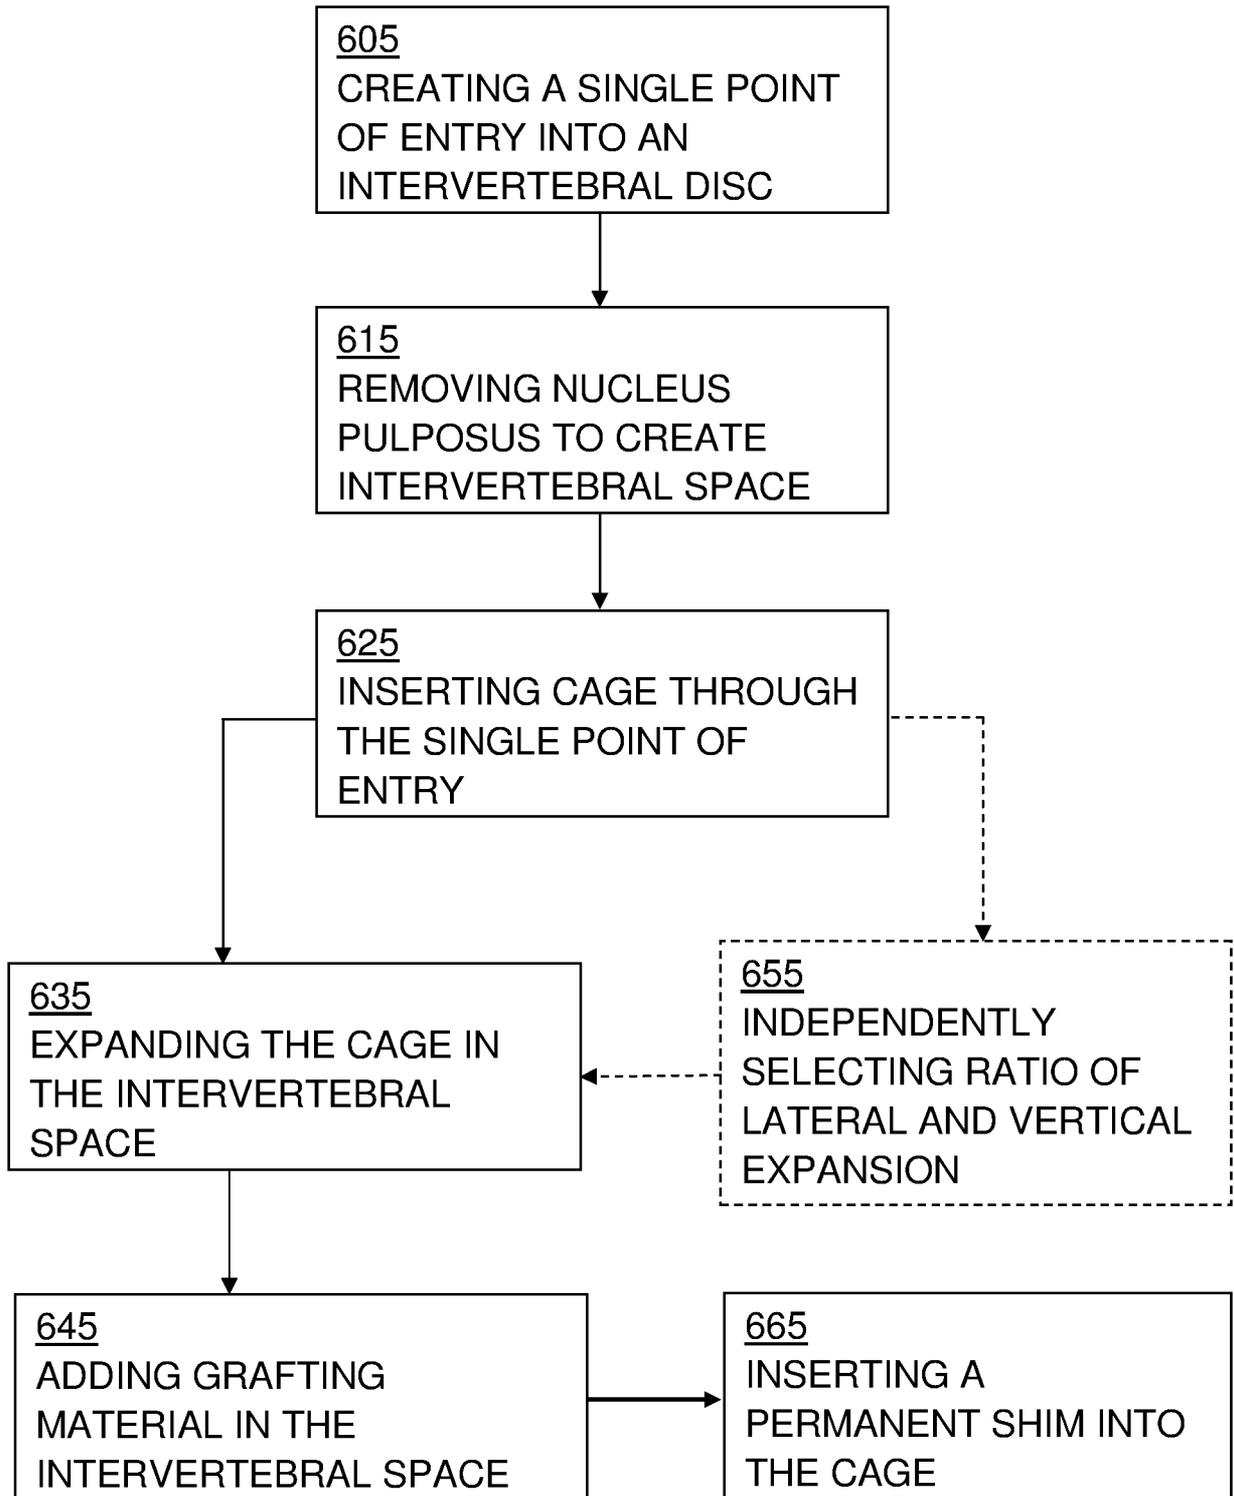


FIG. 6

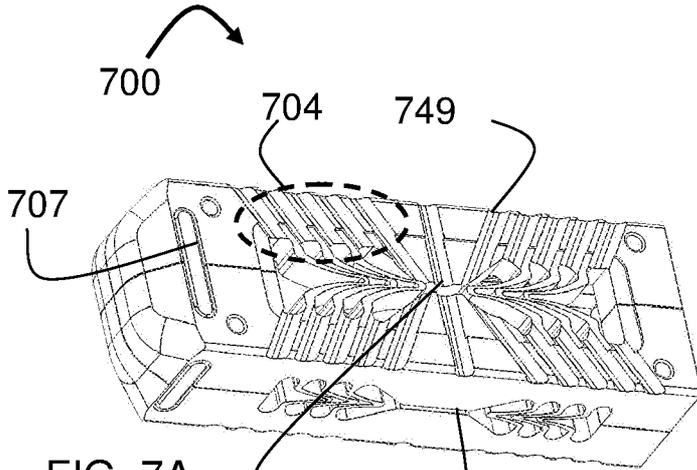


FIG. 7A

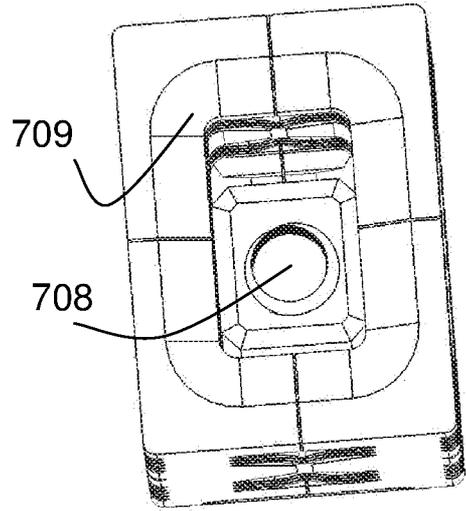


FIG. 7B

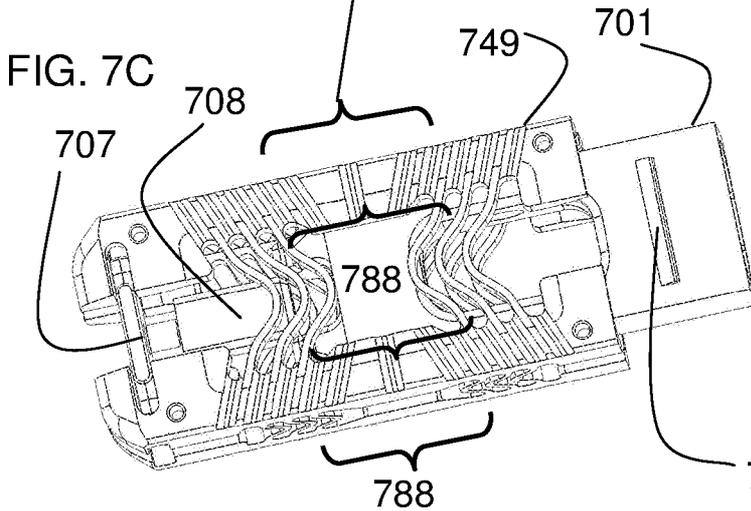


FIG. 7C

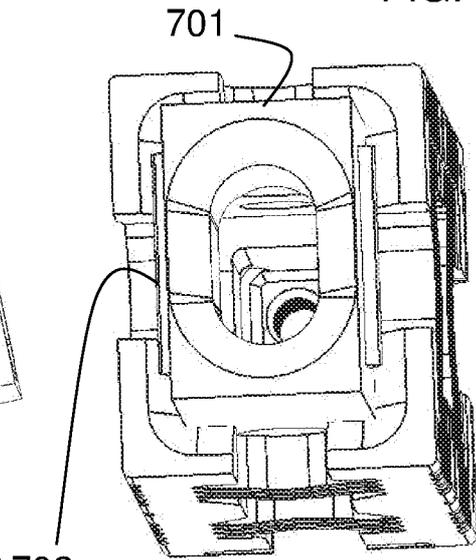


FIG. 7D

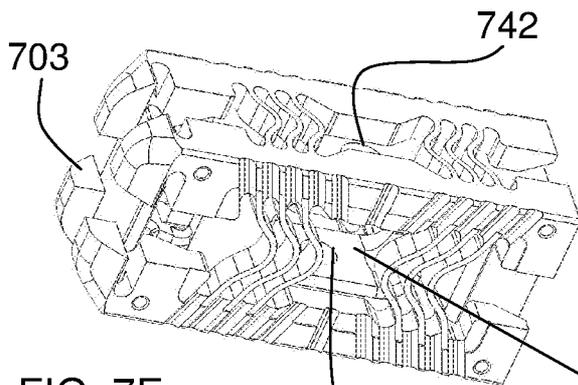


FIG. 7E

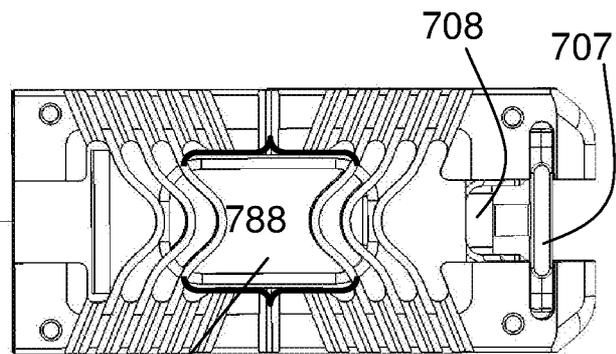
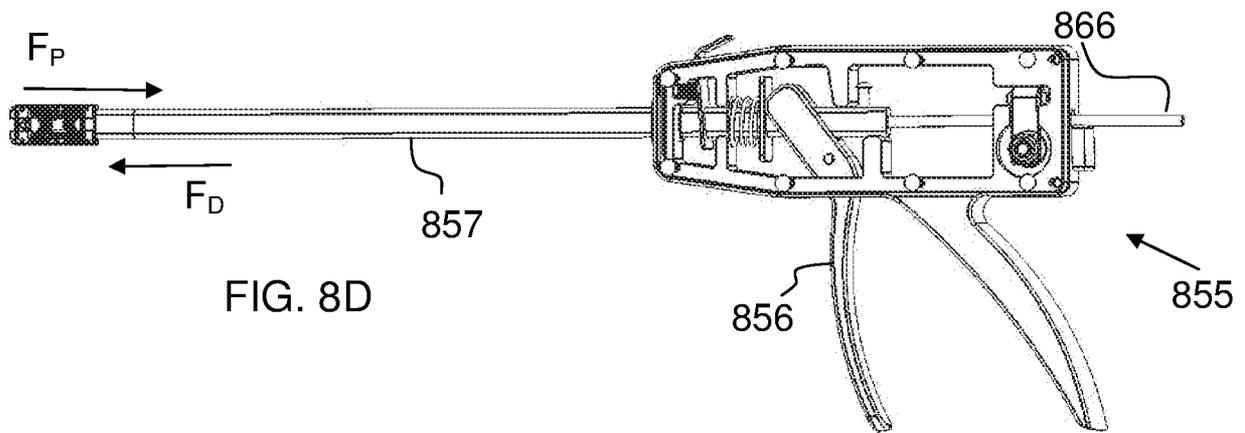
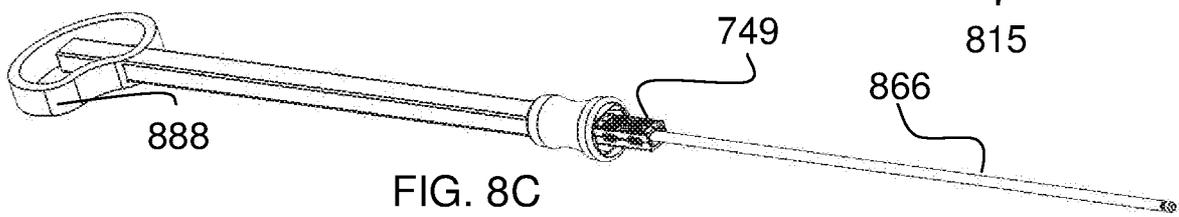
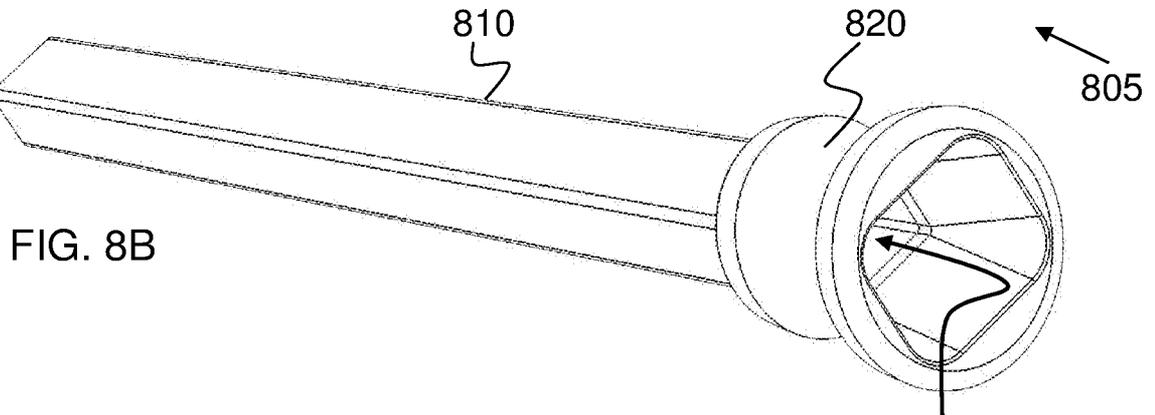
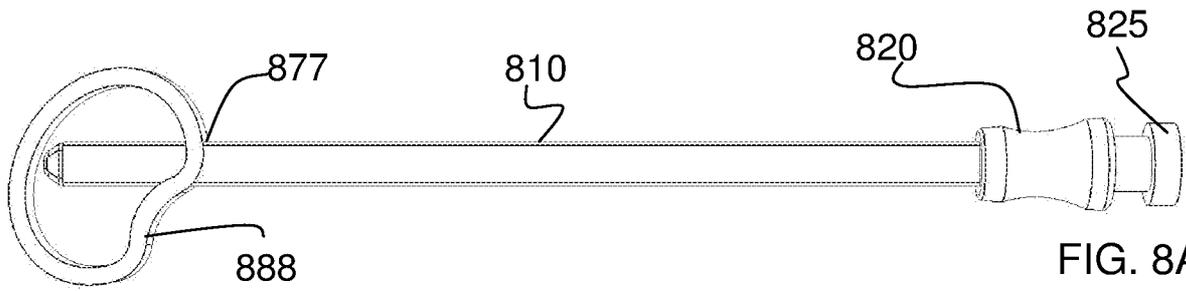


FIG. 7F



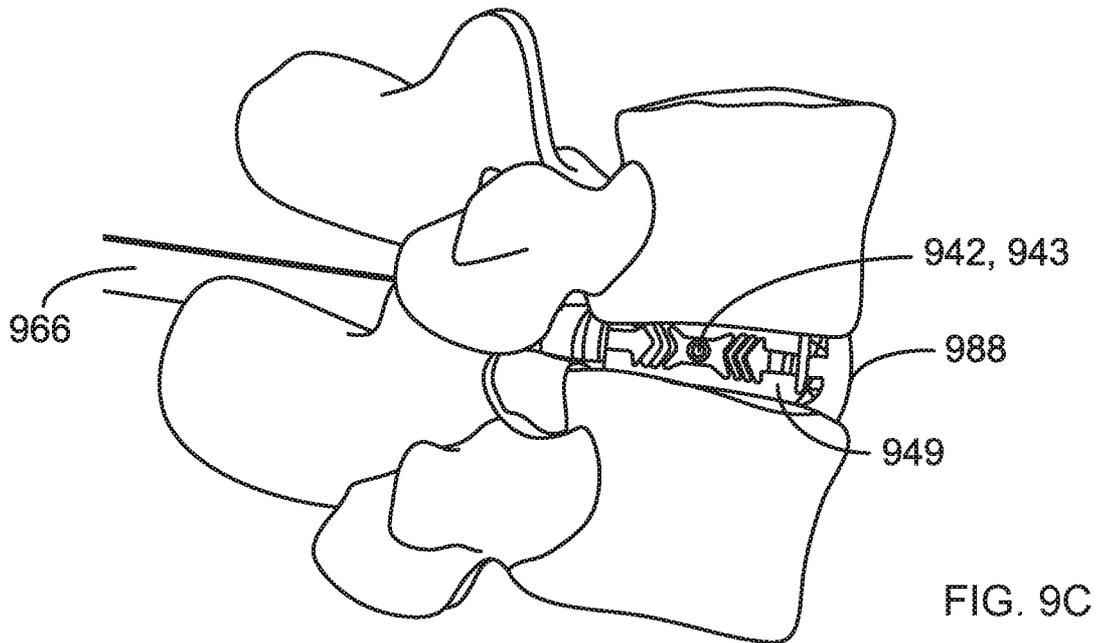
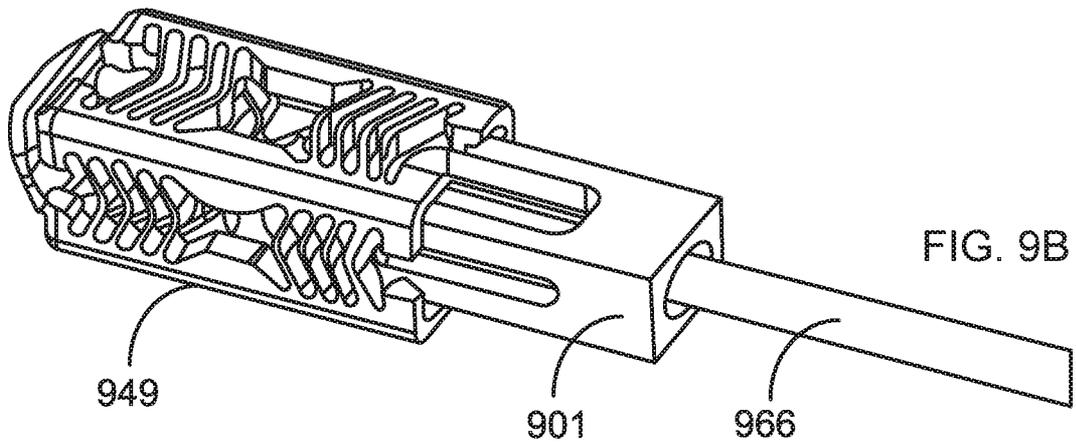
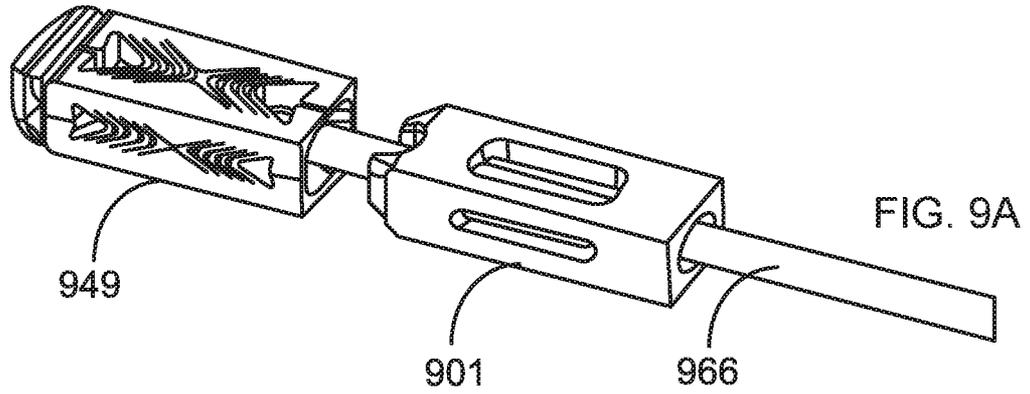
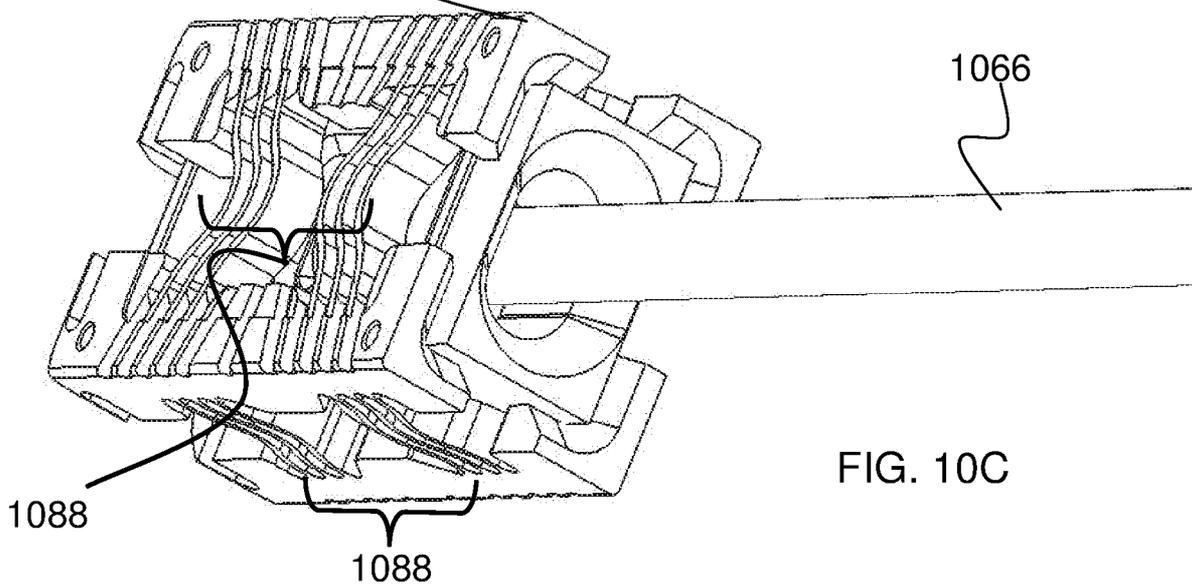
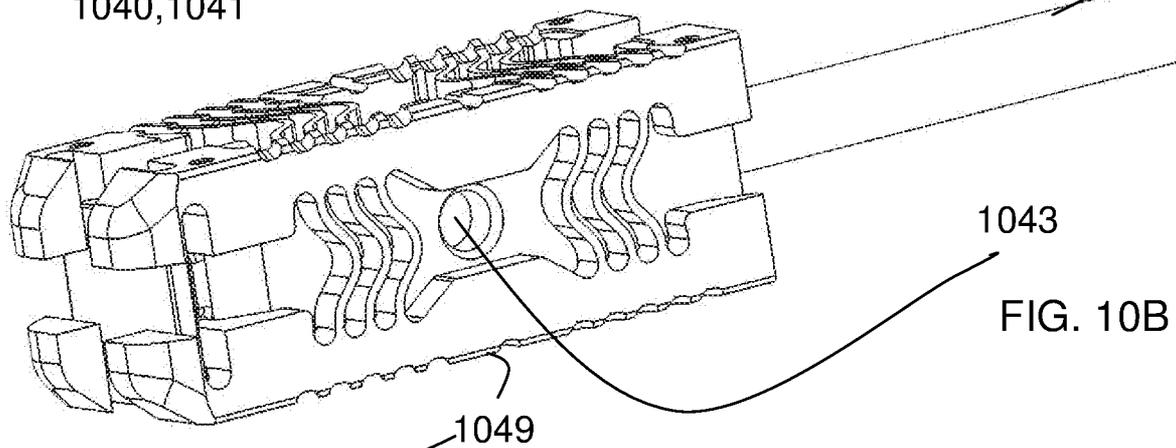
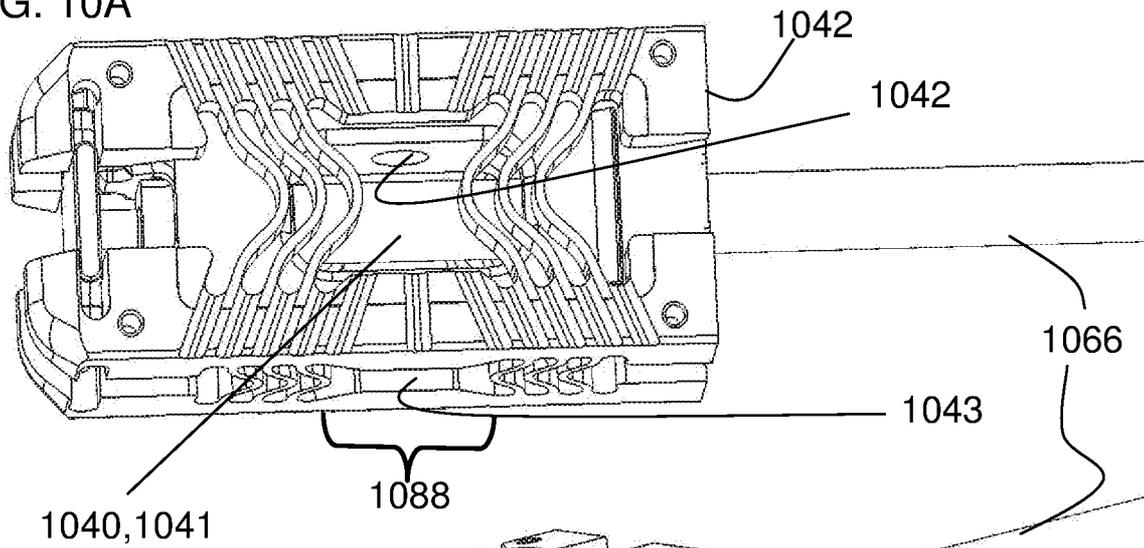


FIG. 10A



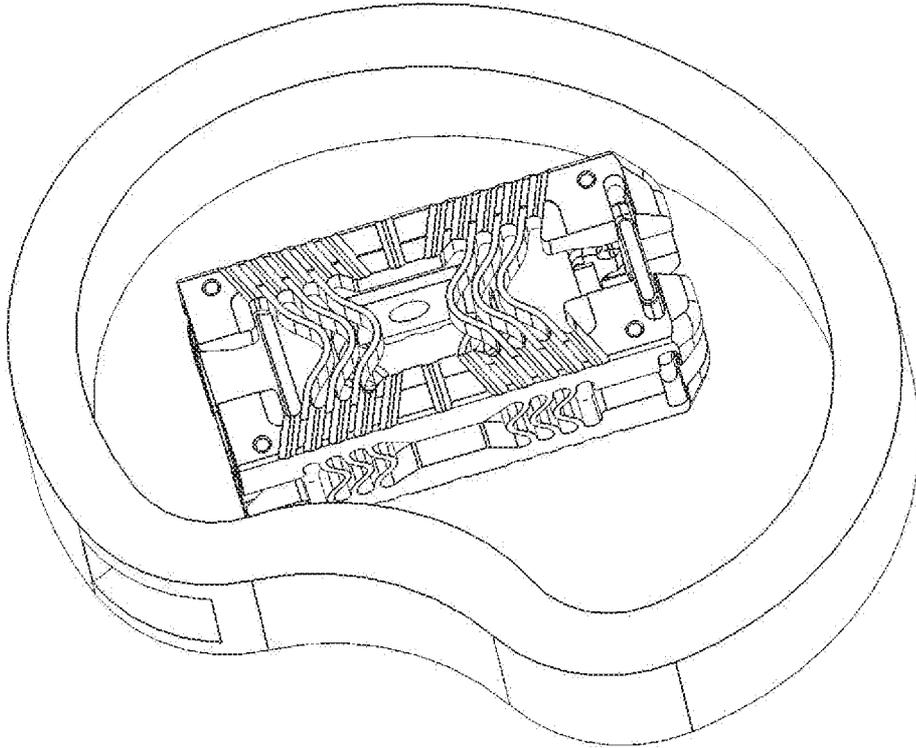


FIG. 11A

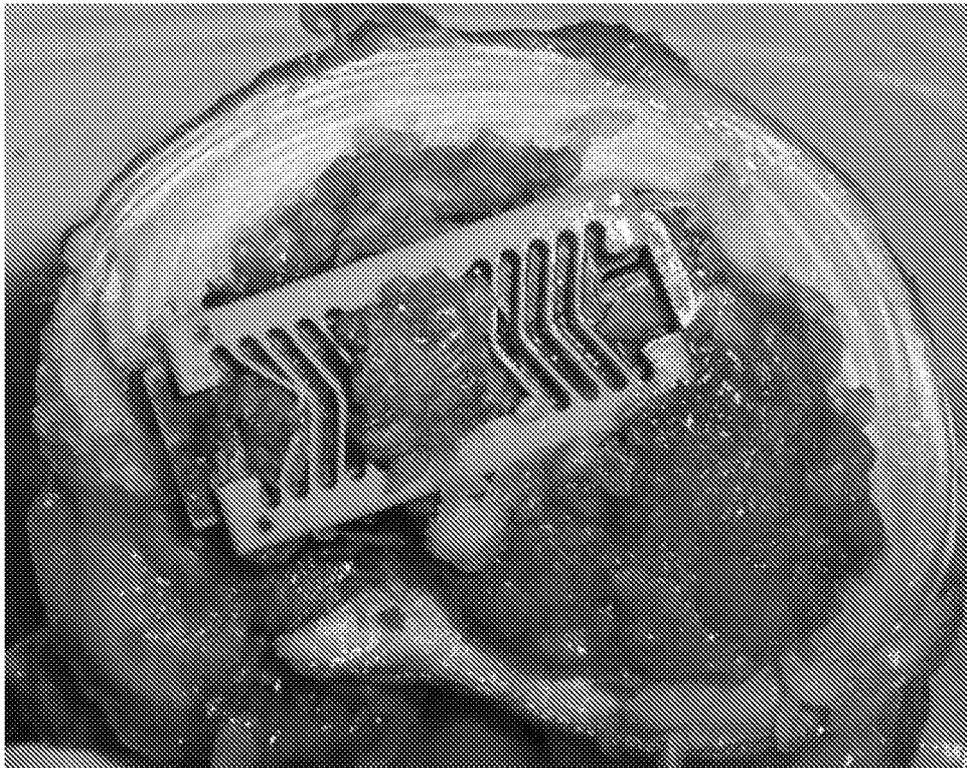


FIG. 11B

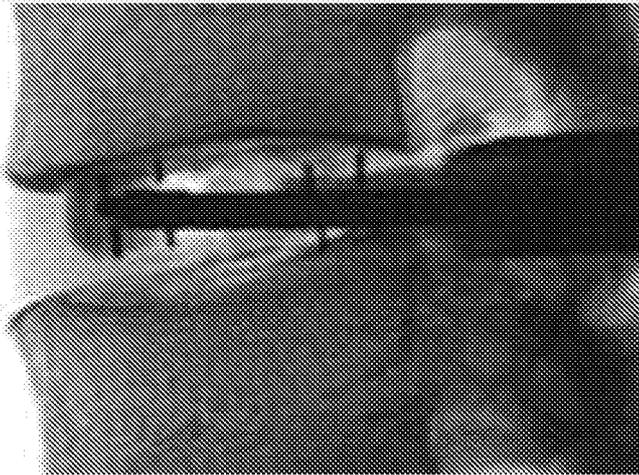


FIG. 12A

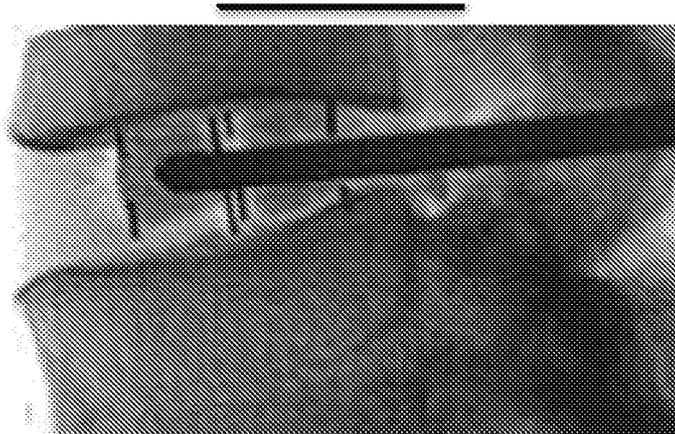


FIG. 12B

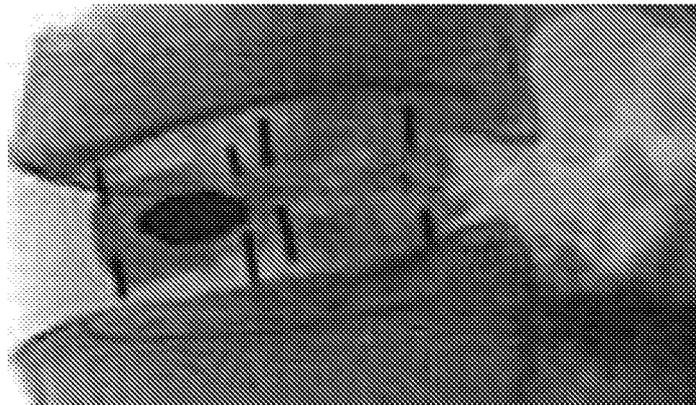


FIG. 12C

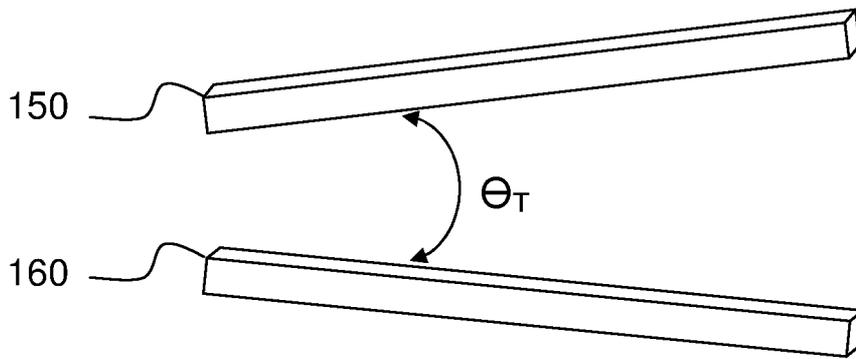


FIG. 13A

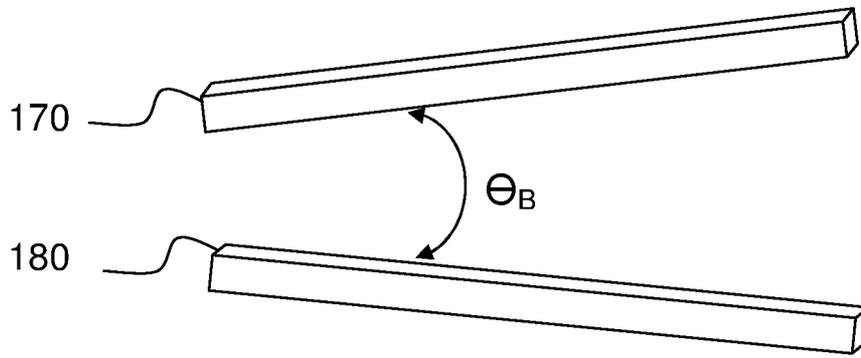


FIG. 13B

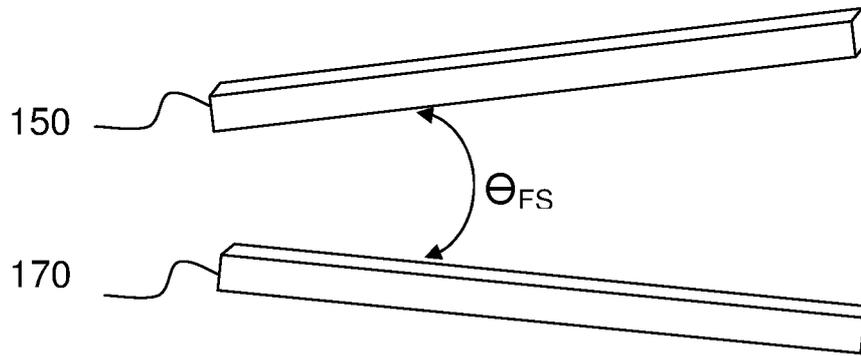


FIG. 13C





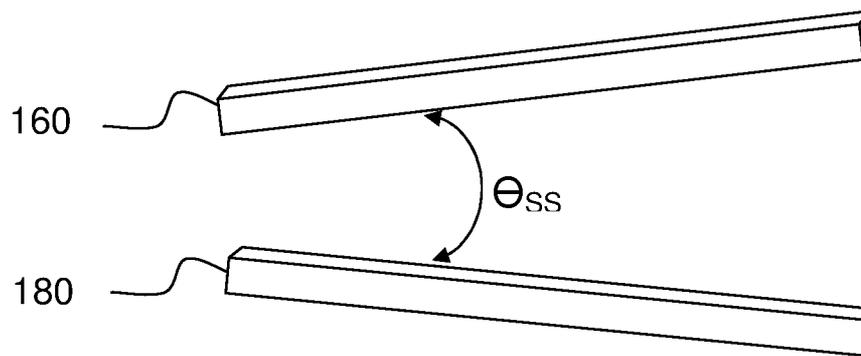


FIG. 13D

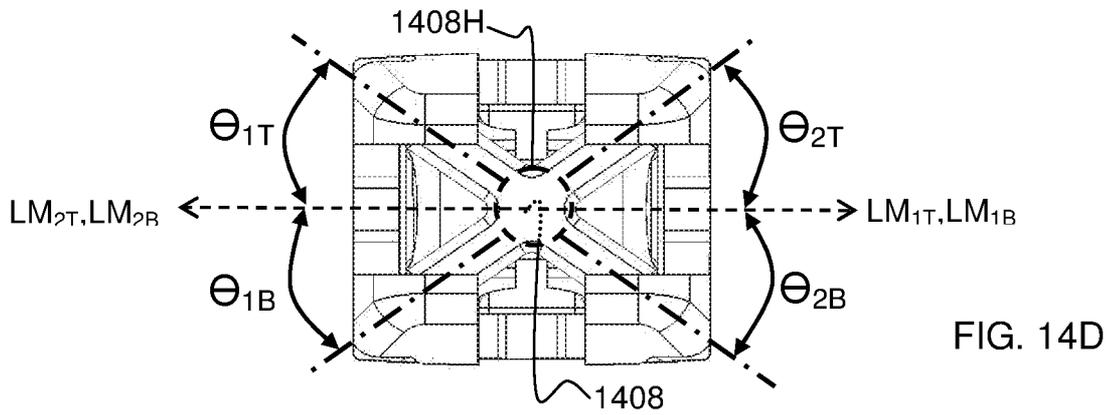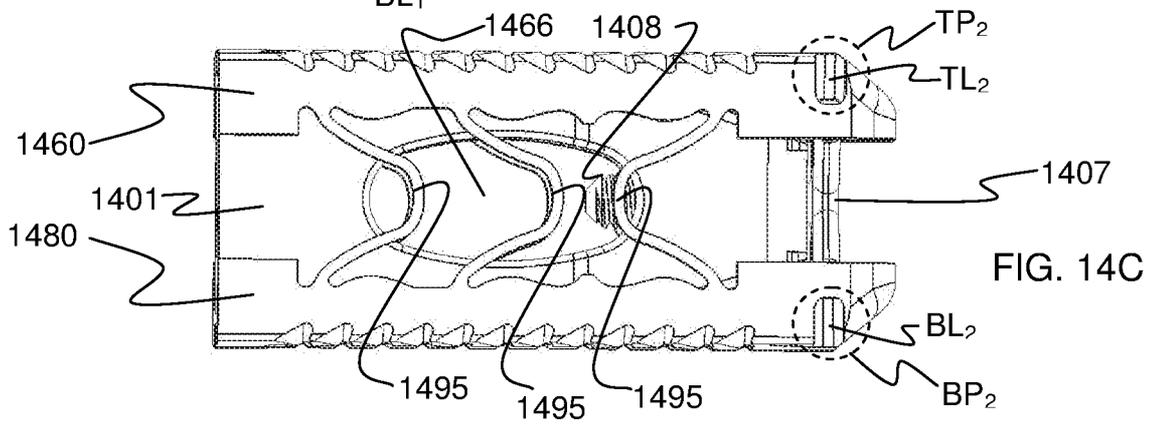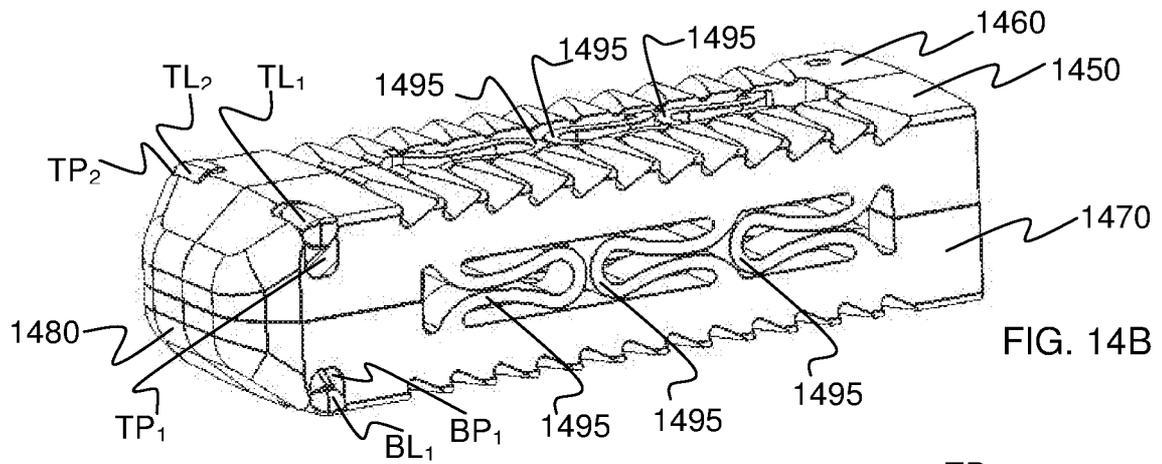

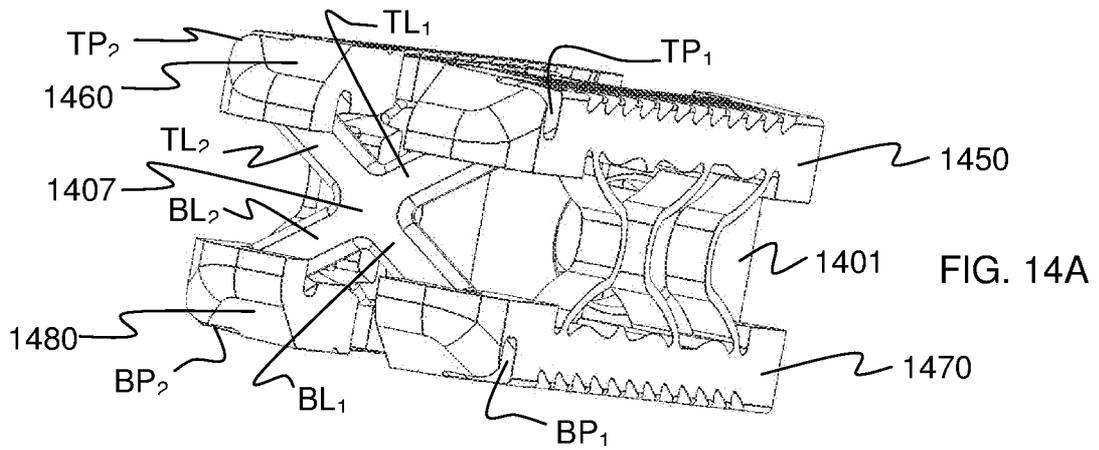

## INTERNATIONAL SEARCH REPORT

International application No.  
**PCT/US2016/014100****A. CLASSIFICATION OF SUBJECT MATTER****A61F 2/44(2006.01)i, A61F 2/28(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**Minimum documentation searched (classification system followed by classification symbols)  
A61F 2/44; B05D 3/00; A61F 2/28Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched  
Korean utility models and applications for utility models  
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)  
eKOMPASS(KIPO internal) & Keywords: intervertebral scaffolding, beam, frame, expand, connector, stabilizer, leg, sliding, tensile force, bone graft, cannula, guide wire**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2014-0172106 A1 (OUROBOROS MEDICAL, INC.) 19 June 2014 See paragraphs [0046]-[0109]; claims 1-31; figures 1A-13.	1-12, 17-20
A	US 2014-0243981 A1 (DAVENPORT, D. et al.) 28 August 2014 See entire document.	1-12, 17-20
A	US 8551173 B2 (LECHMANN, B. et al.) 08 October 2013 See entire document.	1-12, 17-20
A	US 5658336 A (PISHARODI, M.) 19 August 1997 See entire document.	1-12, 17-20
A	US 6375682 B1 (FLEISCHMANN, L. W. et al.) 23 April 2002 See entire document.	1-12, 17-20

 Further documents are listed in the continuation of Box C. See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

02 May 2016 (02.05.2016)

Date of mailing of the international search report

**17 May 2016 (17.05.2016)**

Name and mailing address of the ISA/KR

International Application Division  
Korean Intellectual Property Office  
189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea

Facsimile No. +82-42-481-8578

Authorized officer

Han, Inho

Telephone No. +82-42-481-3362



**INTERNATIONAL SEARCH REPORT**

International application No.

**PCT/US2016/014100****Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1.  Claims Nos.: 13-16  
because they relate to subject matter not required to be searched by this Authority, namely:  
Claims 13-16 pertain to a method for treatment of the human body by surgery and thus relate to a subject matter which this International Searching Authority is not required, under PCT Article 17(2)(a)(i) and PCT Rule 39.1(iv), to search.
2.  Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3.  Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

**Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)**

This International Searching Authority found multiple inventions in this international application, as follows:

1.  As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2.  As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3.  As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4.  No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

**Remark on Protest**

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

## INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

**PCT/US2016/014100**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2014-0172106 A1	19/06/2014	CN 104936554 A	23/09/2015
		EP 2931185 A1	21/10/2015
		KR 10-2015-0100731 A	02/09/2015
		US 8663332 B1	04/03/2014
		WO 2014-093136 A1	19/06/2014
US 2014-0243981 A1	28/08/2014	EP 2958525 A1	30/12/2015
		WO 2014-130989 A1	28/08/2014
US 8551173 B2	08/10/2013	AU 2009-205894 A1	23/07/2009
		AU 2009-205896 A1	23/07/2009
		CA 2710142 A1	23/07/2009
		CN 101909548 A	08/12/2010
		CN 101909548 B	30/07/2014
		EP 2237748 A1	13/10/2010
		EP 2237748 B1	05/09/2012
		EP 2471493 A1	04/07/2012
		JP 2011-509766 A	31/03/2011
		JP 5441922 B2	12/03/2014
		KR 10-1552476 B1	11/09/2015
		KR 10-2010-0113084 A	20/10/2010
		US 2009-0184213 A1	23/07/2009
		US 2010-0025969 A1	04/02/2010
		US 2010-0286783 A1	11/11/2010
		US 2014-0025169 A1	23/01/2014
		US 2015-0257892 A1	17/09/2015
		US 8140201 B2	20/03/2012
		WO 2009-092100 A1	23/07/2009
		WO 2009-092101 A2	23/07/2009
WO 2009-092101 A3	29/10/2009		
WO 2009-092102 A1	23/07/2009		
US 5658336 A	19/08/1997	CA 2185460 A1	28/09/1995
		CA 2222025 A1	19/12/1996
		CA 2298531 A1	11/02/1999
		CA 2407275 A1	08/11/2001
		CA 2560237 A1	06/10/2005
		CN 1192669 A	09/09/1998
		CN 1270501 A	18/10/2000
		EP 0750482 A1	07/04/1999
		EP 0750482 B1	05/01/2000
		EP 0755481 A1	19/03/1997
		EP 0755481 B1	07/10/1998
		EP 0830116 A2	24/10/2001
		EP 0999808 A1	17/05/2000
		EP 0999808 B1	29/12/2004
		EP 1278487 A2	29/01/2003
		EP 1278487 B1	13/09/2006
		EP 1737395 A1	03/01/2007

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2016/014100**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		EP 1737395 B1	30/09/2009
		JP 09-511806 A	25/11/1997
		JP 11-510405 A	14/09/1999
		JP 2001-511391 A	14/08/2001
		JP 2007-529286 A	25/10/2007
		US 2005-0065610 A1	24/03/2005
		US 2006-0282165 A1	14/12/2006
		US 2007-0032873 A1	08/02/2007
		US 2007-0043441 A1	22/02/2007
		US 5429089 A	04/07/1995
		US 5601556 A	11/02/1997
		US 5653761 A	05/08/1997
		US 5653762 A	05/08/1997
		US 5697977 A	16/12/1997
		US 5893890 A	13/04/1999
		US 6093207 A	25/07/2000
		US 6264655 B1	24/07/2001
		US 6309421 B1	30/10/2001
		US 7879095 B2	01/02/2011
		US 8480742 B2	09/07/2013
		WO 2005-092250 A1	06/10/2005
		WO 2007-016673 A2	08/02/2007
		WO 2007-016673 A3	21/06/2007
US 6375682 B1	23/04/2002	None	