

JS011607276B2

(12) United States Patent

Weingarten et al.

US 11,607,276 B2

Mar. 21, 2023

(54) DYNAMIC 3D LUNG MAP VIEW FOR TOOL NAVIGATION INSIDE THE LUNG

(71) Applicant: Covidien LP, Mansfield, MA (US)

(72) Inventors: **Oren P. Weingarten**, Hod-Hasharon

(IL); Ron Barak, Tel Aviv (IL)

(73) Assignee: Covidien LP, Mansfield, MA (US)

(*) Notice: Subject to any disclaimer, the term of this

patent is extended or adjusted under 35

U.S.C. 154(b) by 0 days.

(21) Appl. No.: 17/531,670

(22) Filed: Nov. 19, 2021

(65) Prior Publication Data

US 2022/0079679 A1 Mar. 17, 2022

Related U.S. Application Data

- (60) Division of application No. 17/199,433, filed on Mar.11, 2021, which is a continuation of application No.(Continued)
- (51) **Int. Cl.**A61B 34/10 (2016.01)

 G06T 19/20 (2011.01)

 (Continued)
- (58) Field of Classification Search
 CPC G06T 7/0012; G06T 19/003; G06T 19/20;
 G06T 2207/30064; G06T 2219/2016;
 (Continued)

(56) References Cited

(10) Patent No.:

(45) Date of Patent:

U.S. PATENT DOCUMENTS

5,592,939 A 1/1997 Martinelli 5,611,025 A 3/1997 Lorensen et al. (Continued)

FOREIGN PATENT DOCUMENTS

BR 0013237 A 7/2003 BR 0116004 A 6/2004 (Continued)

OTHER PUBLICATIONS

Canadian Office Action issued in Canadian Application No. 2953390 dated May 20, 2021, 6 pages.


(Continued)

Primary Examiner — Brenda C Bernardi (74) Attorney, Agent, or Firm — Weber Rosselli & Cannon LLP

(57) ABSTRACT

A method for implementing a dynamic three-dimensional lung map view for navigating a probe inside a patient's lungs includes loading a navigation plan into a navigation system, the navigation plan including a planned pathway shown in a 3D model generated from a plurality of CT images, inserting the probe into a patient's airways, registering a sensed location of the probe with the planned pathway, selecting a target in the navigation plan, presenting a view of the 3D model showing the planned pathway and indicating the sensed location of the probe, navigating the probe through the airways of the patient's lungs toward the target, iteratively adjusting the presented view of the 3D model showing the planned pathway based on the sensed location of the probe, and updating the presented view by removing at least a part of an object forming part of the 3D model.

13 Claims, 7 Drawing Sheets

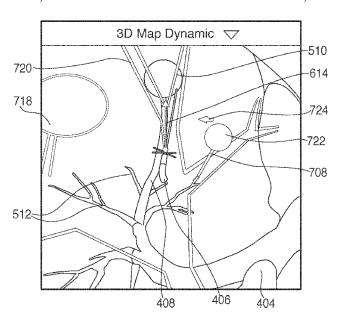

Related U.S. Application Data

17/068,820, filed on Oct. 12, 2020, which is a continuation of application No. 16/828,947, filed on Mar. 24, 2020, now Pat. No. 10,799,297, which is a continuation of application No. 16/418,495, filed on May 21, 2019, now Pat. No. 10,646,277, which is a continuation of application No. 16/148,174, filed on Oct. 1, 2018, now Pat. No. 10,660,708, which is a continuation of application No. 15/828,551, filed on Dec. 1, 2017, now Pat. No. 10,105,185, which is a continuation of application No. 15/447,472, filed on Mar. 2, 2017, now Pat. No. 9,848,953, which is a continuation of application No. 14/751,257, filed on Jun. 26, 2015, now Pat. No. 9,603,668.

(60) Provisional application No. 62/020,262, filed on Jul. 2, 2014.

```
(51) Int. Cl.
     G06T 19/00
                           (2011.01)
     A61B 90/00
                           (2016.01)
     G06T 7/00
                           (2017.01)
     A61B 17/00
                           (2006.01)
     A61B 34/00
                          (2016.01)
     A61B 34/20
                           (2016.01)
```

(52) U.S. Cl.

CPC G06T 19/003 (2013.01); G06T 19/20 (2013.01); A61B 34/25 (2016.02); A61B 2017/00809 (2013.01); A61B 2034/105 (2016.02); A61B 2034/107 (2016.02); A61B 2034/2051 (2016.02); A61B 2090/365 (2016.02); G06T 2207/30064 (2013.01); G06T 2210/41 (2013.01); G06T 2219/2016 (2013.01)

(58) Field of Classification Search

CPC G06T 2210/41; A61B 90/37; A61B 34/10; A61B 2034/2051; A61B 2034/105; A61B 2017/00809; A61B 34/25; A61B 2090/365; A61B 2034/107

See application file for complete search history.

(56)**References Cited**

U.S. PATENT DOCUMENTS

5,676,673 A	10/1997	Ferre et al.
5,697,377 A	12/1997	Wittkampf
5,699,799 A	12/1997	Xu et al.
5,715,836 A	2/1998	Kliegis et al.
5,729,129 A	3/1998	Acker
5,752,513 A	5/1998	Acker et al.
5,782,762 A	7/1998	Vining
5,881,124 A	3/1999	Giger et al.
5,891,030 A	4/1999	Johnson et al.
5,913,820 A	6/1999	Bladen et al.
5,920,319 A	7/1999	Vining et al.
5,967,980 A	10/1999	Ferre et al.
5,971,767 A	10/1999	Kaufman et al.
5,987,960 A	11/1999	Messner et al.
6,019,725 A	2/2000	Vesely et al.
6,047,080 A	4/2000	Chen et al.
6,083,162 A	7/2000	Vining
6,138,045 A	10/2000	Kupinski et al.
6,151,404 A	11/2000	Pieper
6,167,296 A	12/2000	Shahidi
6,181,348 B1	1/2001	Geiger
6,201,387 B1	3/2001	Govari
6,233,476 B1	5/2001	Strommer et al.
6,246,784 B1	6/2001	Summers et al.
6,266,551 B1	7/2001	Osadchy et al.
6,332,089 B1	12/2001	Acker et al.

6,346,940 B1 2/2002 Fukunaga 6,366,800 B1 4/2002 Vining et al. 6,381,485 B1 4/2002 Hunter et al. 6,387,092 B1 5/2002 Burnside et al. 6,466,815 B1 10/2002 Saito et al. 6,496,188 B1 12/2002 Deschamps et al. 6,501,848 B1 12/2002 Carroll et al. 6,501,981 B1 12/2002 Schweikard et al 6,505,065 B1 1/2003 Yanof et al 6,522,907 B1 2/2003 Bladen et al. 6,526,162 B2 2/2003 Asano et al. 6,535,756 B1 3/2003 Simon et al. 6,578,579 B2 6/2003 Burnside et al. 6,584,174 B2 6/2003 Schubert et al. 6,603,868 B1 8/2003 Ludwig et al. 6,611,793 B1 8/2003 Burnside et al. 6,650,927 B1 11/2003 Keidar 6,651,669 B1 11/2003 Burnside Vining 6,694,163 B1 2/2004 6,757,557 B1 6/2004 Bladen et al. 6,783,523 B2 8/2004 Qin et al. 6,792,390 B1 9/2004 Burnside et al. 6,829,379 B1 12/2004 Knoplioch et al. 6.850.794 B2 2/2005 Shahidi 6,892,090 B2 6,898,263 B2 5/2005 Verard et al. 5/2005 Avinash et al. 6,909,913 B2 Vining 6/2005 6,920,347 B2 7/2005 Simon et al. 6,925,200 B2 8/2005 Wood et al. 7,006,677 2/2006 B2 Manjeshwar et al. 7,072,501 B2 7/2006 Wood et al. 7.085.400 B1 Holsing et al. 8/2006 7,096,148 B2 8/2006 Anderson et al. 7,149,564 B2 7,167,180 B1 12/2006 Vining et al. 1/2007 Shibolet 7,174,202 B2 2/2007 Bladen et al. 7,179,220 B2 2/2007 Kukuk 7,236,558 B2 6/2007 Saito et al. 7,301,332 B2 11/2007 Govari et al. 7.315.639 B2 1/2008 Kuhnigk 7,324,104 B1 1/2008 Bitter et al. 7,336,809 B2 2/2008 Zeng et al. 7,397,937 B2 7/2008 Schneider et al. 7,428,334 B2 9/2008 Schoisswohl et al. 7,452,357 B2 11/2008 Vlegele et al. 7,505,809 B2 3/2009 Strommer et al. 7,517,320 B2 4/2009 Wibowo et al. 7.518.619 B2 4/2009 Stoval et al. 7,630,752 B2 12/2009 Viswanathan 7,630,753 B2 12/2009 Simon et al. 7,659,912 B2 2/2010 Akimoto et al. 7,702,153 B2 4/2010 Hong et al. 7,751,865 B2 7/2010 Jascob et al. 7,756,316 B2 7/2010 Odry et al. 7,788,060 B2 8/2010 Schneider 7,792,565 B2 Vining 9/2010 7,805,269 B2 9/2010 Glossop 7,809,176 B2 10/2010 Gündel 7,811,294 B2 10/2010 Strommer et al. 7,822,461 B2 10/2010 Geiger et al. 7,901,348 B2 Soper et al. 3/2011 7,907,772 B2 3/2011 Wang et al. 7,929,014 B2 4/2011 Akimoto et al. 7,951,070 B2 5/2011 Ozaki et al. 7,969,142 B2 6/2011 Krueger et al. 7,985,187 B2 Wibowo et al. 7/2011 3,009,891 A1 8/2011 Vaan 8,049,777 B2 11/2011 Akimoto et al. 8,055,323 B2 11/2011 Sawyer 8,102,416 B2 1/2012 Ito et al. 8,126,241 B2 2/2012 Zarkh et al. 8,131,344 B2 3/2012 Strommer et al 8,170,328 B2 5/2012 Masumoto et al. 8,199,981 B2 6/2012 Koptenko et al. 8,200,314 B2 6/2012 Bladen et al. 8,202,213 B2 6/2012 Ito et al. 8,208,708 B2* 6/2012 Homan A61B 90/36

8,219,179 B2

7/2012 Ganatra et al.


378/4

US 11,607,276 B2 Page 3

(56)		Referen	ces Cited	2012/0249546 A			Tschirren et al.
	U.S.	PATENT	DOCUMENTS	2012/0280135 A 2012/0287238 A		11/2012 11/2012	Onishi A61B 1/0005
8,257,346	5 B2	9/2012	Qin et al.	2013/0144124 A	11*	6/2013	348/45 Prisco A61B 1/000094
8,267,927			Dalal et al.	2013/0165854 A	. 1	6/2012	600/117
8,290,228 8,298,135			Cohen et al. Ito et al.	2013/0103834 A 2013/0231556 A			Sandhu et al. Holsing et al.
8,335,359			Fidrich et al.	2013/0236076 A			Averbuch et al.
8,391,952			Anderson	2013/0303945 A			Blumenkranz et al.
8,417,009			Mizuno	2013/0317352 A			Case et al.
8,494,612 8,509,877			Vetter et al. Mori et al.	2013/0345/18 A	41 °	12/2013	Crawford A61B 90/39 606/130
8,672,836			Higgins et al.	2014/0035798 A	4 1	2/2014	Kawada et al.
8,682,045			Vining et al.	2014/0066766 A			Stonefield et al.
8,696,549			Holsing et al.	2014/0298270 A			Wiemker et al.
8,698,806 8,700,132			Kunert et al. Ganatra et al.	2014/0343408 A 2015/0148690 A			Tolkowsky Chopra et al.
8,706,184			Mohr et al.	2015/0265368 A			Chopra et al.
8,706,193	B2	4/2014	Govari et al.	2015/0305612 A	A 1	10/2015	Hunter et al.
8,709,034			Keast et al.	2015/0313503 A			Seibel et al.
8,730,237 8,768,029			Ruijters et al. Helm et al.	2016/0000302 A 2016/0000414 A			Brown et al. Brown et al.
8,784,400			Roschak	2016/0005220 A			Weingarten et al.
8,798,227			Tsukagoshi et al.	2016/0073928 A		3/2016	Soper et al.
8,798,339			Mielekamp et al. Prisco et al.	2016/0157939 A 2016/0183841 A			Larkin et al. Duindam et al.
8,801,601 8,819,591			Wang et al.	2016/0192860 A			Allenby et al.
8,827,934	B2		Chopra et al.	2016/0287344 A			Donhowe et al.
8,862,204			Sobe et al.	2017/0112576 A			Coste-Maniere et al.
9,008,754 9,129,048			Steinberg et al. Stonefield et al.	2017/0172664 A 2017/0209071 A			Weingarten et al. Zhao et al.
9,603,668			Weingarten et al.	2017/0265952 A			Donhowe et al.
9,770,216		9/2017	Brown et al.	2017/0311844 A			Zhao et al.
9,848,953			Weingarten et al.	2017/0319165 A			Averbuch
9,918,659 9,974,525			Chopra et al. Weingarten et al.	2018/0078318 A 2018/0153621 A			Barbagli Duindam et al.
10,373,719		8/2019	Soper et al.	2018/0235709 A			Donhowe et al.
10,376,178			Chopra	2018/0240237 A			Donhowe et al.
10,405,753 10,478,162		9/2019	Sorger Barbagli	2018/0256262 A 2018/0263706 A			Duindam et al. Averbuch
10,480,926			Froggatt et al.	2018/0279852 A			Rafii-Tari et al.
10,524,866	6 B2	1/2020	Srinivasan et al.	2018/0325419 A	A 1		Zhao et al.
10,555,788			Panescu et al. Chopra	2019/0000559 A			Berman et al. Berman et al.
10,610,306 10,638,953			Duindam et al.	2019/0000560 A 2019/0008413 A			Duindam et al.
10,674,970			Averbuch et al.	2019/0038359 A			Weingarten et al.
10,682,070			Duindam	2019/0038365 A			Soper et al.
10,706,543 10,709,506			Donhowe et al. Coste-Maniere et al.	2019/0065209 A 2019/0110839 A			Mishra et al. Rafii-Tari et al.
10,743,748			Gilboa	2019/0175062 A			Rafii-Tari et al.
10,772,485			Schlesinger et al.	2019/0183318 A			Froggatt et al.
10,796,432 10,823,627			Mintz et al. Sanborn et al.	2019/0183585 A 2019/0183587 A			Rafii-Tari et al. Rafii-Tari et al.
10,823,027			Ummalaneni et al.	2019/0183387 A			Gadda et al.
10,835,153			Rafii-Tari et al.	2019/0209016 A		7/2019	Herzlinger et al.
10,885,630			Li et al.	2019/0209043 A			Zhao et al.
2003/0013972 2005/0182295		1/2003 8/2005	Soper et al.	2019/0216548 A 2019/0239723 A			Ummalaneni Duindam et al.
2005/0207630			Chan et al.	2019/0239831 A			Chopra
2008/0118135	A1*	5/2008	Averbuch G06T 7/155	2019/0250050 A			Sanborn et al.
2008/0123921	A 1 %	£/2009	382/131 Gielen G06T 7/32	2019/0254649 A 2019/0269462 A			Walters et al. Weingarten et al.
2008/0123921	AI'	3/2008	382/175	2019/0269470 A			Barbagli et al.
2008/0183073	A1	7/2008	Higgins et al.	2019/0272634 A	1 1	9/2019	Li et al.
2009/0012390			Pescatore et al.	2019/0298160 A			Ummalaneni et al.
2009/0030306 2009/0096807			Miyoshi et al. Silverstein et al.	2019/0298451 A 2019/0320878 A			Wong et al. Duindam et al.
2009/0096807			Liang A61B 34/10	2019/0320937 A			Duindam et al.
	_		434/262	2019/0336238 A			Yu et al.
2010/0030064			Averbuch	2019/0343424 A 2019/0350659 A			Blumenkranz et al. Wang et al.
2010/0290693 2010/0310146			Cohen et al. Higgins et al.	2019/03/03/03/9 A 2019/03/03/03/9 A			Zhao et al.
2010/0310140			Guttman et al.	2019/0365479 A	A 1	12/2019	Rafii-Tari
2011/0085720	A1	4/2011	Averbuch	2019/0365486 A			Srinivasan et al.
2011/0237897	A1*	9/2011	Gilboa A61B 1/00154	2019/0380787 A			Ye et al.
2011/0251607	7 A1	10/2011	600/208 Kruecker et al.	2020/0000319 A 2020/0000526 A		1/2020	Saadat et al. Zhao
2012/0203065			Higgins et al.	2020/0008655 A			Schlesinger et al.

(56) References Cited		MX 225663 B 1/2005 MX 226292 B 2/2005
U.S. PATENT	DOCUMENTS	MX 226292 B 2/2003 MX 246862 B 6/2007 MX 265247 B 3/2009
2020/0030044 A1 1/2020	Wang et al.	MX 284569 B 3/2011
	Sorger	WO 2009138871 A2 11/2009 WO 2011102012 A1 8/2011
	Kojima	WO 2011102012 A1 8/2011 WO 2013192598 A1 12/2013
	Lo et al.	WO 2013192398 A1 12/2013
	Soper et al.	
2020/0054399 A1 2/2020	Tzeisler et al. Duindam et al.	OTHER PUBLICATIONS
	Holsing et al.	Chinese Office Action dated Dec. 3, 2018 issued in corresponding
	Lo et al. Sanborn et al.	CN Appln. No. 201580035779.3.
	Dicarlo et al.	Chinese Office Action for application No. 201580035779.3 dated
	Chopra et al.	Nov. 28, 2017 with English Translation (8 pages).
	Duindam et al.	Chinese Rejection Decision issued in Chinese Patent Application
	Blumenkranz	No. 201580035779.3 dated Aug. 19, 2019, 4 pages. No English
	Pomper et al.	translation available.
	Prisco	Examination Report No. 1 for standard patent application issued in
2020/0129239 A1 4/2020	Bianchi et al.	Australian Patent Application No. 2019204469 dated Oct. 10, 2019,
	Wong	3 pages.
	Hunter et al.	Examination Report No. 1 for standard patent application issued in
	Donhowe et al.	Australian Patent Application No. 2020205248 dated Nov. 6, 2020,
	Averbuch	4 pages.
	Ummalaneni Barbagli	Extended European Search Report for application No. 15814621.7
	Donhowe et al.	dated Mar. 12, 2018 (9 pages).
	Srinivasan et al.	Japanese Office Action For application No. 2016-575425 dated Mar.
	Chopra	19, 2019 with English translation.
	Zhao et al.	Non-Final Office Action issued in U.S. Appl. No. 17/199,433 dated
2020/0229679 A1 7/2020	Zhao et al.	Jan. 6, 2022.
2020/0242767 A1 7/2020	Zhao et al.	Non-Final Office Action issued in U.S. Appl. No. 17/526,933 dated
	Duindam	Jan. 27, 2022.
	Adebar et al.	Notice of Allowance issued in U.S. Appl. No. 17/199,433 dated Jul.
	Averbuch et al.	27, 2021.
	Sawant et al.	Notification of the Fourth Office Action issued in Chinese Patent
	Deyanov	Application No. 201580035779.3 dated Jun. 21, 2019, 17 pages.
	Donhowe et al.	Office Action issued in U.S. Appl. No. 17/199,429 dated May 19, 2021.
	ENT DOCUMENTS	Rejection Decision issued in Chinese Patent Application No. 201580035779.3 dated Oct. 13, 2021, with English google transla-
CN 101877996 A	11/2010	tion.
CN 103068294 A	4/2013	Srikantha et al. "Ghost Detection and Removal for High Dynamic
CZ 486540 CZ 2709512	9/2016	Range Images: Recent Advances". Published in "Signal Processing:
CZ 2709512 CZ 2884879	8/2017 1/2020	Image Communication (2012) 10.1016/j.image.2012.02.001".
EP 3413830 A4	9/2019	DOI: 10.1016/j.image.2012.02.001 (Year: 2012).
EP 3478161 A4	2/2020	The Fifth Office Action issued in Chinese Patent Application No.
EP 3641686 A2	4/2020	201580035779.3 dated Apr. 1, 2021 with English Translation.
EP 3644885 A1	5/2020	U.S. Office Action issued in U.S. Appl. No. 16/148,174 dated Aug.
EP 3644886 A1	5/2020	8, 2019, 43 pages.
JP 2002306403 A	10/2002	U.S. Office Action issued in U.S. Appl. No. 17/068,820 dated Sep.
JP 2009018184 A	1/2009	24, 2021.
JP 2011193885 A MX PA03005028 A	10/2011 1/2004	* cited by examiner
		-

^{*} cited by examiner

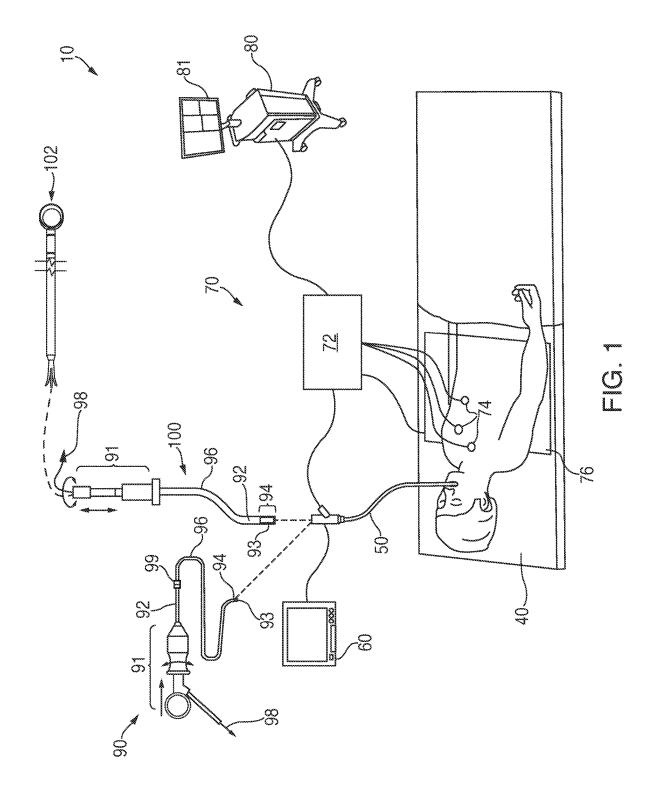

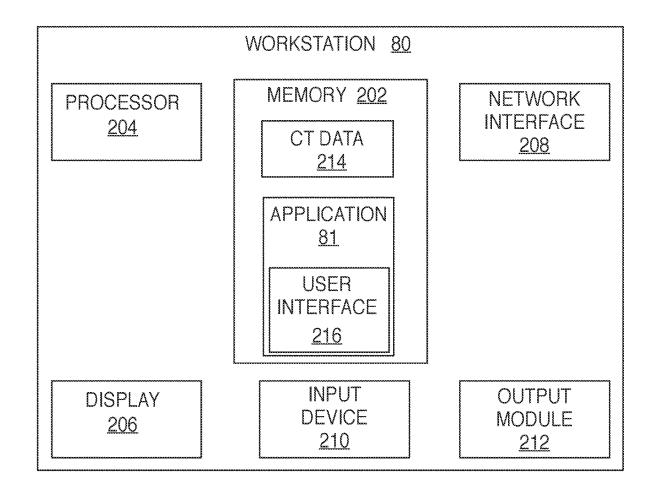
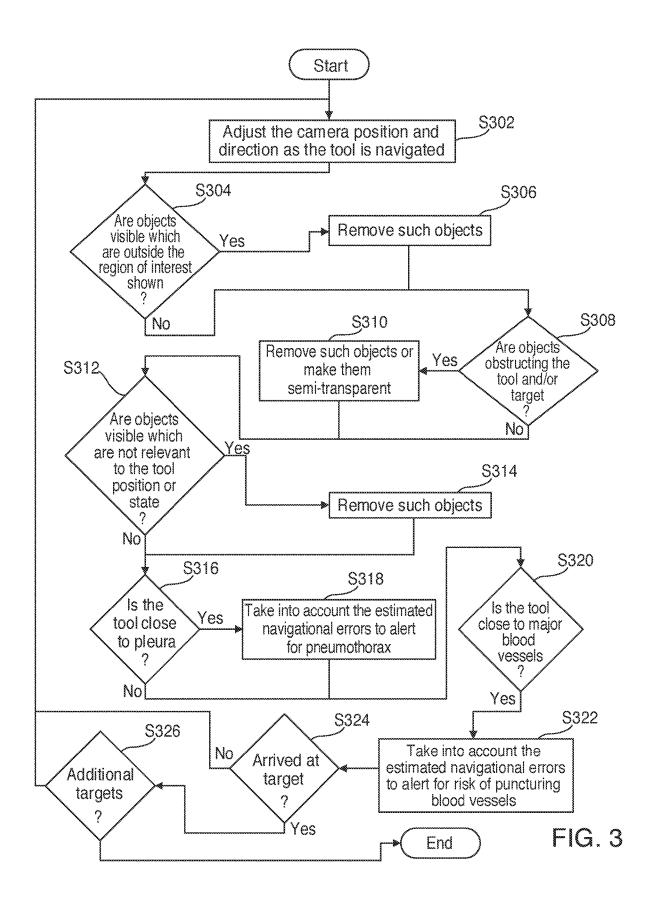


FIG. 2



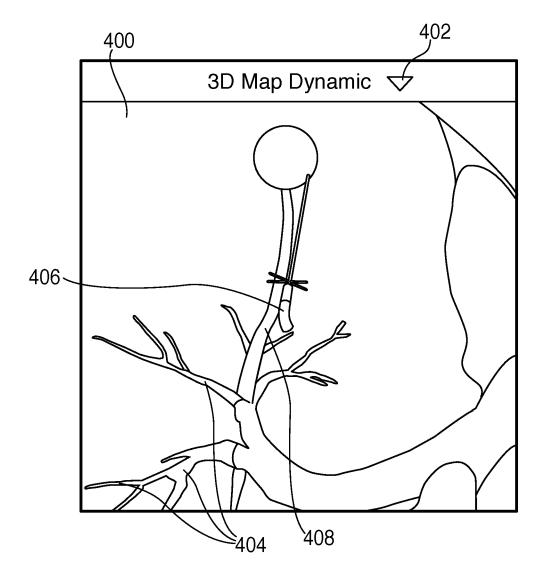


FIG. 4

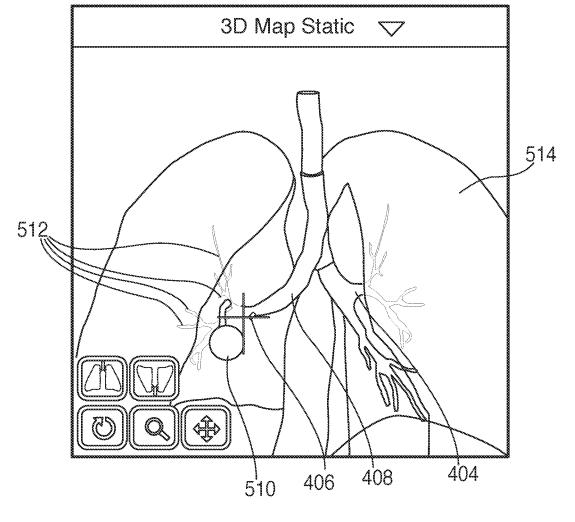


FIG. 5

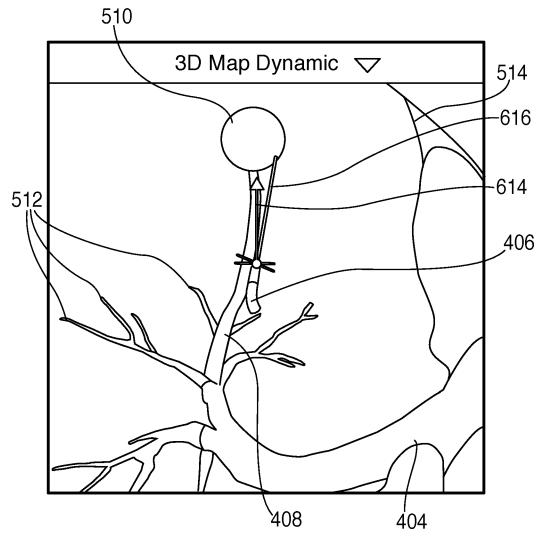


FIG. 6

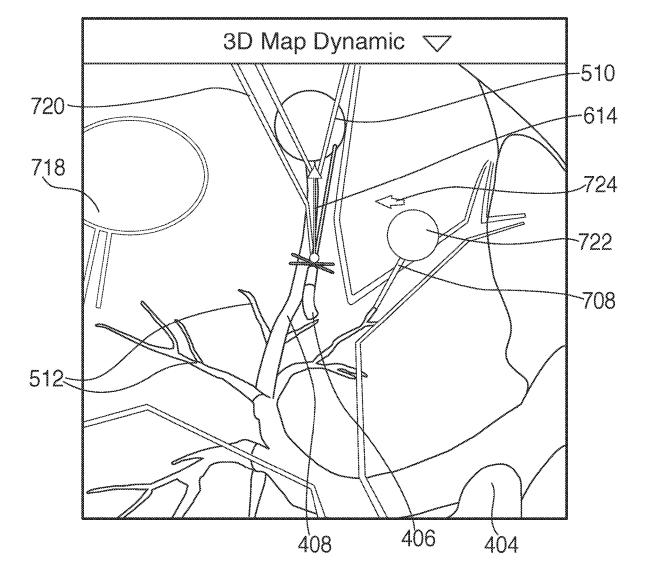


FIG. 7

DYNAMIC 3D LUNG MAP VIEW FOR TOOL NAVIGATION INSIDE THE LUNG

CROSS REFERENCE TO RELATED APPLICATIONS

This application is a division of U.S. patent application Ser. No. 17/199,433, filed Mar. 11, 2021, now U.S. Pat. No. 11,185,371, which is a continuation of U.S. patent application Ser. No. 17/068,820, filed Oct. 12, 2020, which is a continuation of U.S. patent application Ser. No. 16/828,947, filed Mar. 24, 2020, now U.S. Pat. No. 10,799,297, which is a continuation of U.S. patent application Ser. No. 16/418, 495, filed May 21, 2019, now U.S. Pat. No. 10,646,277, which is a continuation of U.S. patent application Ser. No. 16/148,174, filed Oct. 1, 2018, now U.S. Pat. No. 10,660, 708, which is a continuation of U.S. patent application Ser. No. 15/828,551, filed Dec. 1, 2017, now U.S. Pat. No. 10,105,185, which is a continuation of U.S. patent application Ser. No. 15/447,472, filed Mar. 2, 2017, now U.S. Pat. 20 No. 9,848,953, which is a continuation of U.S. patent application Ser. No. 14/751,257, filed Jun. 26, 2015, now U.S. Pat. No. 9,603,668, which claims the benefit of the filing date of provisional U.S. Patent Application No. 62/020,262, filed Jul. 2, 2014.

BACKGROUND

Technical Field

The present disclosure relates to the treatment of patients with lung diseases and, more particularly, to devices, systems, and methods for implementing a dynamic 3D lung map view for tool navigation inside a patient's lungs.

Description of Related Art

Lung cancer has an extremely high mortality rate, especially if it is not diagnosed in its early stages. The National Lung Screening Trial has demonstrated that a reduction in 40 mortality occurs if diagnostic scans such as computed tomography (CT) scans are used for early detection for those at risk of contracting the disease. While CT scans increase the possibility that small lesions and nodules in the lung can be detected, these lesions and nodules still require biopsy 45 and cytological examination before a diagnosis can be rendered and treatment can be undertaken.

To perform a biopsy, as well as many treatments, navigation of tools within the lungs to the point of biopsy or treatment is necessary. Accordingly, improvements to systems and methods of navigating are continually being sought.

SUMMARY

Provided in accordance with the present disclosure is a method for implementing a dynamic three-dimensional (3D) lung map view for navigating a probe inside a patient's lungs.

In an aspect of the present disclosure, the method includes 60 loading a navigation plan into a navigation system, the navigation plan including a planned pathway shown in a 3D model generated from a plurality of CT images, inserting the probe into a patient's airways, the probe including a location sensor in operative communication with the navigation 65 system, registering a sensed location of the probe with the planned pathway, selecting a target in the navigation plan,

2

resenting a view of the 3D model showing the planned pathway and indicating the sensed location of the probe, navigating the probe through the airways of the patient's lungs toward the target, iteratively adjusting the presented view of the 3D model showing the planned pathway based on the sensed location of the probe, and updating the presented view by removing at least a part of an object forming part of the 3D model.

In another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes zooming in when the probe approaches the target.

In yet another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes zooming in when the diameter of an airway within which the probe is sensed to be located is less than a predetermined threshold.

In another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes changing the presented view to a view wherein the airway tree bifurcation is maximally spread.

In yet another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes aligning the view with the sensed location of the probe to show where the probe is and what lies ahead of the probe.

In another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes changing the presented view to be orthogonal to a vector from the probe to the pathway.

In yet another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes changing the presented view to be perpendicular to the sensed location of the probe in relation to the 3D model to show the area around the probe.

In another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes changing the presented view to be behind the sensed location of the probe in relation to the 3D model to show the area ahead of the probe.

In yet another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes changing the presented view to be at the tip of the probe and orthogonal to the directing in which the probe is moving.

In another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes changing the presented view to be perpendicular to a vector from the probe to the target to show the alignment of the probe to the target.

In yet another aspect of the present disclosure, iteratively adjusting the presented view of the 3D model includes rotating the presented view around a focal point to improve a 3D perception of the sensed location of the probe in relation to the 3D model.

In a further aspect of the present disclosure, updating the presented view by removing at least part of an object includes removing at least part of an object which is outside of a region of interest.

In yet a further aspect of the present disclosure, updating the presented view by removing at least part of an object includes removing at least part of an object which is obstructing the probe.

In a further aspect of the present disclosure, updating the presented view by removing at least part of an object includes removing at least part of an object which is obstructing the target.

In yet a further aspect of the present disclosure, updating the presented view by removing at least part of an object

includes removing at least part of an object which is not relevant to the sensed location of the probe.

In a further aspect of the present disclosure, updating the presented view by removing at least part of an object includes removing at least part of an object which is not ⁵ relevant to a current selected state of the navigation system.

In another aspect of the present disclosure, the method further includes presenting an alert.

In a further aspect of the present disclosure, presenting an alert includes presenting an alert when the probe is ¹⁰ approaching the pleura.

In yet a further aspect of the present disclosure, presenting an alert includes presenting an alert when the tool is approaching major blood vessels.

In a further aspect of the present disclosure, presenting an ¹⁵ alert includes presenting an alert when the sensed location of the probe is off of the planned pathway.

Any of the above aspects and embodiments of the present disclosure may be combined without departing from the scope of the present disclosure.

BRIEF DESCRIPTION OF THE DRAWINGS

Various aspects and features of the present disclosure are described hereinbelow with references to the drawings, ²⁵ wherein:

FIG. 1 depicts a system diagram of an example electromagnetic navigation (EMN) system which may be used to create and display a dynamic 3D lung map view, according to an embodiment of the present disclosure;

FIG. 2 depicts a schematic diagram of an example workstation forming part of the EMN system of FIG. 1 which may be used to create and display a dynamic 3D lung map view, according to an embodiment of the present disclosure;

FIG. 3 is a flowchart illustrating an example method for 35 creating a dynamic 3D lung map view, according to an embodiment of the present disclosure;

FIG. 4 illustrates an example view of a user interface that may be presented on the workstation of FIG. 2 showing an example of a dynamic 3D lung map view, according to an 40 embodiment of the present disclosure;

FIG. 5 illustrates an example of an unadjusted 3D lung map view, according to an embodiment of the present disclosure:

FIG. 6 illustrates an example of a dynamic 3D lung map 45 view, according to an embodiment of the present disclosure; and

FIG. 7 illustrates another example of a dynamic 3D lung map view, according to an embodiment of the present disclosure.

DETAILED DESCRIPTION

Devices, systems, and methods for implementing a dynamic 3D lung map view for tool navigation inside a 55 patient's lungs are provided in accordance with the present disclosure. A location sensor may be incorporated into different types of tools and catheters to track the location and assist in navigation of the tools. The tracked location of the location sensor may be used to visually show the location of 60 a tool on the dynamic 3D lung map. The location of the location sensor within the body of a patient, with reference to a 3D map or 2D images as well as a planned pathway assists the clinician in navigating lungs of the patient. However, because of the amounts of data being presented 65 and the ability to show details of the airways, there is a desire to assist the clinician and eliminate unessential data or

4

data regarding portions of the anatomy that are unrelated to a specific navigation or a specific procedure. In addition, there is a desire to harness this detailed anatomical data and alert the clinician regarding proximity to certain anatomical features. These and other aspects of the present disclosure are detailed herein below.

The dynamic 3D lung map view, as disclosed herein, is one of a variety of views that may be presented by an electromagnetic navigation (EMN) system which may be used by a clinician to perform an ELECTROMAGNETIC NAVIGATION BRONCHOSCOPY® (ENB) procedure. Among other tasks that may be performed using the EMN system are planning a pathway to target tissue, navigating a positioning assembly to the target tissue, and navigating a variety of tools, such as a locatable guide (LG) and/or a biopsy tool to the target tissue.

An ENB procedure generally involves at least two phases: (1) planning a pathway to a target located within, or adjacent 20 to, the patient's lungs; and (2) navigating a probe to the target along the planned pathway. These phases are generally referred to as (1) "planning" and (2) "navigation." An example of the planning software described herein can be found in U.S. patent application Ser. Nos. 13/838,805, 13/838,997, and 13/839,224, all of which are filed by Covidien LP on Mar. 15, 2013 and entitled "Pathway Planning System and Method," all of which are incorporated herein by reference. An example of the planning software can be found in commonly assigned U.S. Provision Patent Application No. 62/020,240 entitled "SYSTEM AND METHOD FOR NAVIGATING WITHIN THE LUNG" the entire contents of which are incorporated herein by reference.

Prior to the planning phase, the patient's lungs are imaged by, for example, a computed tomography (CT) scan, although additional applicable methods of imaging will be known to those skilled in the art. The image data assembled during the CT scan may then be stored in, for example, the Digital Imaging and Communications in Medicine (DI-COM) format, although additional applicable formats will be known to those skilled in the art. The CT scan image data may then be loaded into a planning software application ("application") to be used during the planning phase of the ENB procedure.

The application may use the CT scan image data to generate a three-dimensional (3D) model of the patient's lungs. The 3D model may include, among other things, a model airway tree corresponding to the actual airways of the patient's lungs, and showing the various passages, branches, and bifurcations of the patient's actual airway tree. Additionally, the 3D model may include lesions, markers, blood vessels, and/or a 3D rendering of the pleura. While the CT scan image data may have gaps, omissions, and/or other imperfections included in the image data, the 3D model is a smooth representation of the patient's airways, with any such gaps, omissions, and/or imperfections in the CT scan image data filled in or corrected. As described in more detail below, the 3D model may be viewed in various orientations. For example, if a clinician desires to view a particular section of the patient's airways, the clinician may view the 3D model represented in a 3D rendering and rotate and/or zoom in on the particular section of the patient's airways. Additionally, during the navigation phase of an ENB procedure, while a tool is being navigated through the patient's airways, the clinician may want to have the presented view of the 3D model dynamically updated as the tool is navigated. Such a dynamic 3D lung map view is disclosed below.

Prior to the start of the navigation phase of an ENB procedure, the 3D model is registered with the actual lungs of the patient. One potential method of registration involves navigating a locatable guide into each lobe of the patient's lungs to at least the second bifurcation of the airways of that 5 lobe. The position of the locatable guide is tracked during this registration phase, and the 3D model is iteratively updated based on the tracked position of the locatable guide within the actual airways of the patient's lungs. This registration process is described in commonly-owned U.S. Pro- 10 visional Patent Application Ser. No. 62/020,220 entitled "Real-Time Automatic Registration Feedback", filed on Jul. 2, 2014, by Brown et al. With reference to FIG. 1, an EMN system 10 is provided in accordance with the present disclosure. One such EMN system is the ELECTROMAG- 15 NETIC NAVIGATION BRONCHOSCOPY® system currently sold by Covidien LP. As shown in FIG. 1, EMN system 10 generally includes an operating table 40 configured to support a patient; a bronchoscope 50 configured for patient's airways; monitoring equipment 60 coupled to bronchoscope 50 for displaying video images received from bronchoscope 50; a tracking system 70 including a tracking module 72, a plurality of reference sensors 74, and an electromagnetic field generator 76; a workstation 80 includ- 25 ing software and/or hardware, such as an EMN application 81, used to facilitate pathway planning, identification of target tissue, and navigation to the target tissue.

FIG. 1 also depicts two types of catheter guide assemblies 90, 100. Both catheter guide assemblies 90, 100 are usable 30 with the EMN system 10 and share a number of common components. Each catheter guide assembly 90, 100 includes a handle 91, which is connected to an extended working channel (EWC) 96. EWC 96 is sized for placement into the working channel of bronchoscope 50. In operation, a locat- 35 able guide (LG) 92, including an electromagnetic (EM) sensor 94, is inserted into EWC 96 and locked into position such that the sensor 94 extends a desired distance beyond the distal tip 93 of EWC 96. The location of EM sensor 94, and thus the distal end of EWC 96, within an electromagnetic 40 field generated by the electromagnetic field generator 76 can be derived by the tracking module 72, and the workstation 80. Catheter guide assemblies 90, 100 have different operating mechanisms, but each contain a handle 91 that can be manipulated by rotation and compression to steer the distal 45 tip 93 of LG 92 and EWC 96. Catheter guide assemblies 90 are currently marketed and sold by Covidien LP under the name SUPERDIMENSION® Procedure Kits, similarly catheter guide assemblies 100 are currently sold by Covidien LP under the name EDGETM Procedure Kits, both kits 50 include a handle 91, EWC 96, and LG 92. For a more detailed description of the catheter guide assemblies 90, 100, reference is made to commonly-owned U.S. patent application Ser. No. 13/836,203 entitled "MICROWAVE ABLA-TION CATHETER AND METHOD OF UTILIZING THE 55 SAME", filed on Mar. 15, 2013 by Ladtkow et al., the entire contents of which are hereby incorporated by reference.

As illustrated in FIG. 1, the patient is shown lying on operating table 40 with bronchoscope 50 inserted through the patient's mouth and into the patient's airways. Broncho- 60 scope 50 includes a source of illumination and a video imaging system (not explicitly shown) and is coupled to monitoring equipment 60, e.g., a video display, for displaying the video images received from the video imaging system of bronchoscope 50.

Catheter guide assemblies 90, 100 including LG 92 and EWC 96 are configured for insertion through a working

channel of bronchoscope 50 into the patient's airways (although the catheter guide assemblies 90, 100 may alternatively be used without bronchoscope 50). LG 92 and EWC 96 are selectively lockable relative to one another via a locking mechanism 99. A six degrees-of-freedom electromagnetic tracking system 70, e.g., similar to those disclosed in U.S. Pat. No. 6,188,355 and published PCT Application Nos. WO 00/10456 and WO 01/67035, entitled "Wireless six-degree-of-freedom locator", filed on Dec. 14, 1998 by Gilboa, the entire contents of each of which is incorporated herein by reference, or any other suitable positioning measuring system, is utilized for performing navigation, although other configurations are also contemplated. Tracking system 70 is configured for use with catheter guide assemblies 90, 100 to track the position of EM sensor 94 as it moves in conjunction with EWC 96 through the airways of the patient, as detailed below.

As shown in FIG. 1, electromagnetic field generator 76 is insertion through the patient's mouth and/or nose into the 20 positioned beneath the patient. Electromagnetic field generator 76 and the plurality of reference sensors 74 are interconnected with tracking module 72, which derives the location of each reference sensor 74 in six degrees of freedom. One or more of reference sensors 74 are attached to the chest of the patient. The six degrees of freedom coordinates of reference sensors 74 are sent to workstation 80, which includes EMN application 81 where sensors 74 are used to calculate a patient coordinate frame of reference.

Also shown in FIG. 1 is a biopsy tool 102 that is insertable into catheter guide assemblies 90, 100 following navigation to a target and removal of LG 92. The biopsy tool 102 is used to collect one or more tissue sample from the target tissue. As detailed below, biopsy tool 102 is further configured for use in conjunction with tracking system 70 to facilitate navigation of biopsy tool 102 to the target tissue, and tracking of a location of biopsy tool 102 as it is manipulated relative to the target tissue to obtain the tissue sample. Though shown as a biopsy tool in FIG. 1, those of skill in the art will recognize that other tools including for example microwave ablation tools and others may be similarly deployed and tracked as the biopsy tool 102 without departing from the scope of the present disclosure.

Although the EM sensor 94 is described above as being included in LG 92 it is also envisioned that EM sensor 94 may be embedded or incorporated within biopsy tool 102 where biopsy tool 102 may alternatively be utilized for navigation without need of LG 92 or the necessary tool exchanges that use of LG 92 requires. A variety of useable biopsy tools are described in U.S. Provisional Patent Application Nos. 61/906,732 and 61/906,762 both entitled "DEVICES, SYSTEMS, AND METHODS FOR NAVI-GATING A BIOPSY TOOL TO A TARGET LOCATION AND OBTAINING A TISSUE SAMPLE USING THE SAME", filed Nov. 20, 2013 and U.S. Provisional Patent Application No. 61/955,407 having the same title and filed Mar. 14, 2014, the entire contents of each of which are incorporated herein by reference and useable with the EMN system 10 as described herein.

During procedure planning, workstation 80 utilizes computed tomographic (CT) scan image data for generating and viewing a three-dimensional (3D) model of the patient's airways, enables the identification of target tissue on the 3D model (automatically, semi-automatically or manually), and allows for the selection of a pathway through the patient's airways to the target tissue. The 3D model may be presented on a display monitor associated with workstation 80, or in any other suitable fashion.

Using workstation **80**, various views of the 3D model may be presented and may be manipulated by a clinician to facilitate identification of a target and selection of a suitable pathway through the patient's airways to access the target. For example, EMN application **81** may be configured in 5 various states to display the 3D model in a variety of view modes. Some of these view modes may include a dynamic 3D lung map view, as further described below. For each view of the 3D model, the angle from which the 3D model is displayed may correspond to a view point. The view point 10 may be fixed at a predefined location and/or orientation, or may be adjusted by the clinician operating workstation **80**.

The 3D model may also show marks of the locations where previous biopsies were performed, including the dates, times, and other identifying information regarding the 15 tissue samples obtained. These marks may also be selected as the target to which a pathway can be planned. Once selected, the pathway is saved for use during the navigation procedure.

Following procedure planning, a procedure may be undertaken in which the EM sensor **94**, in conjunction with tracking system **70**, enables tracking of EM sensor **94** (and thus the distal end of the EWC or the tool **102**) as EM sensor **94** is advanced through the patient's airways following the pathway planned during the procedure planning phase.

Turning now to FIG. 2, there is shown a system diagram of workstation 80. Workstation 80 may include memory 202, processor 204, display 206, network interface 208, input device 210, and/or output module 212. Memory 202 may store EMN application 81 and/or CT data 214. EMN application 81 may, when executed by processor 204, cause display 206 to present user interface 216. The EMN application 81 provides the interface between the sensed position of the EM sensor 94 and the image and planning data developed in the planning phase.

Referring now to FIG. 3, there is shown an aspect which may be incorporated into an EMN application 81. Specifically, FIG. 3 depicts a flowchart of an exemplary method of creating a dynamic 3D lung map view. During an ENB procedure, this example method may be started when a 40 clinician selects a dynamic 3D lung map view button 402 in an EMN application 81 user interface 400. Alternatively, button 402 may be a drop down menu from which the clinician may select the dynamic 3D lung map view from among a plurality of available views. Starting at step S302, 45 the view point from which the 3D model is displayed may be automatically adjusted in relation to the tracked location of a tool, which is depicted as a probe 406 in FIGS. 4-7, inside the patient's lungs. Adjusting the view point may include moving the view point in relation to the 3D model 50 and/or zooming in on the 3D model to display a closer image of the 3D model. As shown in FIG. 6 below, an unadjusted 3D lung map view (FIG. 5) is adjusted such that the position of a probe 406 is more clearly shown in relation to the position of a target 510 and surrounding airways 512. The 55 view point may further be adjusted according to the direction in which probe 406 is being navigated and/or to be orthogonal to a vector between the tip of probe 406 and a target 510 or in relation to the pathway 408, as is shown in FIGS. 6 and 7, which depict the 3D model from a view point 60 orthogonal to vector 614 which runs from the tip of digital probe 406 to target 510. The view point may further be adjusted by zooming in when probe 406 approaches target 510 or airways having a diameter less than a predetermined threshold. In an embodiment, a preferred view point may be 65 such that the displayed view of the 3D model shows the bifurcations of the airway tree around digital probe 406 as

8

maximally spread, that is, a view point from a direction showing the airway tree with as few overlapping branches as possible. In an embodiment the view point may be moved to be above probe 406 in relation to the 3D model, or behind probe 406 in relation to the 3D model, in order to provide the clinician with a clearer understanding of the position of probe 406 in relation to surrounding objects. In such an embodiment, the dynamic 3D lung map view may show the area of the 3D model in front of and around the tool, as shown in FIG. 7. In another embodiment, the view point may be moved such that the view presented by EMN application 81 is looking ahead out of the tip of digital probe 406.

Next, at step S304, EMN application 81 determines whether any objects are visible from the current view point but are outside of a region of interest for the current navigation procedure. An example might be other targets, or portions of the patient's physiology, such as blood vessels and the heart, which lie outside of the region in which the pathway is located, such as in other lobes of the patient's lungs, or along other branches of airway tree 404 which are not used for the current procedure. If EMN application 81 determines that such objects are visible, those objects may be removed from the view at step S306, as shown below by FIG. 7.

Thereafter, or if EMN application 81 determines that there are no such objects in the view, processing proceeds to step S308, where EMN application 81 determines whether there are objects obstructing the view of digital probe 406 and/or target 510. For example, depending on the angle of the view point, the surrounding airways which do not form part of the planned pathway may lie in the line of sight and between the view point and probe 406 or target 510. If EMN application 81 determines that such objects are obstructing the view of probe 406 or target 510, those objects may be removed from the view at step S310, as shown below by FIG. 7.

Thereafter, or if EMN application 81 determines that there are no such objects in the view, processing proceeds to step S312, where EMN application 81 determines if there are any objects visible in the view which are unrelated to the position of probe 406, the type of tool being used in the current navigation procedure, or the selected state of EMN application 81. For example, markers indicating the location of previous biopsies at different target locations may be within the view angle from the view point, but are not relevant to the current procedure, as shown below by FIG. 7. Another example may be targets 722 which are part of the current navigation plan but have at least one other target 510 which must be visited first. Such targets 722 may become visible or "unhidden" once target 510 has been visited and the necessary procedures performed. If EMN application 81 determines that such objects are within the view, those objects may be removed from the view at step S314.

Thereafter, or if EMN application 81 determines that there are no such objects in the view, processing proceeds to step S316, where EMN application 81 determines whether digital probe 406, and thus sensor 94, is approaching the pleural boundaries of the patient's lungs. EMN application 81 may determine that sensor 94 is approaching the pleural boundaries of the patient's lungs based on, for example, the distance between sensor 94 and the pleura, the angle between sensor 94 and the pleura, the speed at which sensor 94 is moving, and/or any combination thereof. The determination may further be based on a known or estimated rate of navigational errors. When sensor 94 is close to the pleura, there is an increased risk of injury, such as pneumothorax, to the patient, and the clinician may want to be aware of that

to proceed with added caution. Thus, if EMN application **81** determines that sensor **94** is close to the pleura, EMN application **81** may present an alert to the clinician at step S**318**. EMN application **81** may also take known or estimated navigational errors into account when determining 5 whether sensor **94** is approaching the pleura.

9

Thereafter, or if EMN application 81 determines that sensor 94 is not approaching the pleura, processing proceeds to step S320, where EMN application 81 determines whether sensor 94 is approaching one or more major blood 10 vessels. As with the pleura, when sensor 94 is close to major blood vessels, particularly where a tool 102, such as a biopsy or microwave ablation tool, is being deployed, there is added risk of injury to the patient, and the clinician may want to be aware that sensor 94 is close to major blood vessels to 15 proceed with added caution. Thus, if EMN application 81 determines that sensor 94 is close major blood vessels, EMN application 81 may present an alert to the clinician at step S322. Additionally, as with the pleura, EMN application 81 may take known or estimated navigational errors into 20 account when determining whether sensor 94 is approaching major blood vessels.

Thereafter, or if EMN application 81 determines that sensor 94 is not approaching any major blood vessels, processing proceeds to step S324, where EMN application 25 81 determines whether probe 406 has arrived at the target. If EMN application 81 determines that probe 406 has not arrived at the target, processing returns to step S302. In this way, the dynamic 3D lung map view is continuously updated and/or adjusted during the navigation procedure. If EMN 30 application 81 determines that digital probe 406 has arrived at the target, processing proceeds to step S326, where EMN application 81 determines whether there are more targets to be visited. If EMN application 81 determines that there are no more targets to be visited, processing ends. Otherwise, 35 processing returns to step S302.

FIG. 4 illustrates an example user interface that may be presented by workstation 80 showing an example view of the 3D model. User interface (UI) 400 includes a button 402 which may be used to select and/or enable the dynamic 3D 40 lung map view. UI 400 further shows an airway tree 404, a digital probe 406, and a pathway 408.

FIG. 5 illustrates an example of an unadjusted 3D lung map view which may be presented by EMN application 81 via UI 400. The unadjusted 3D lung map view shows the 45 probe 406 within the 3D model, corresponding to the location of sensor 94 within the patient's airways. Also shown by the unadjusted 3D lung map view are the airway tree 404, the pathway 408, the target 510, the surrounding airways 512, and the pleura 514 of the lungs. The unadjusted 50 3D lung map view may be adjusted manually.

FIG. 6 illustrates an example view of a dynamic 3D lung map view which may be presented by EMN application 81. The example dynamic 3D lung map view shows the same probe 406 and target 510 as the unadjusted 3D lung map 55 view of FIG. 5. However, the dynamic 3D lung map view has been adjusted by zooming in on the 3D model to show the position of probe 406 in relation to target 510. The dynamic 3D lung map view has further been aligned with the tip of probe 406, or a vector 614 from digital probe 406 to 60 target 510, and positioned such that pathway 408 and surrounding airways 512 may clearly be seen. A line 614 indicates the line of sight from the tip of digital probe 406 intersecting with target 510.

FIG. 7 illustrates an example dynamic 3D lung map view 65 wherein objects have been hidden or "ghosted out" to more clearly show the objects and components of the 3D model

10

which are relevant to the current procedure, according to an embodiment of this disclosure. Hiding or "ghosting out" objects may involve completely removing such objects from the displayed 3D lung map, or such objects may be shown in a different way from objects which are not hidden, for example with a higher level of transparency. The example dynamic 3D lung map view includes airway tree **404**, probe **406**, pathway **408**, target **510**, surrounding airways **512**, and vector **614**, as described above with reference to FIGS. **4-6**.

The example dynamic 3D lung map view further shows additional targets 718 which have been hidden because they are located outside of the region of interest, as described above with regard to step S304 of FIG. 3. The example dynamic 3D lung map view also shows that a branch 720 of airway tree 404 which overlaps with pathway 408 and target 510, and thus obstructs the view of pathway 408 and target 510, has been hidden, as described above with regard to step S308 of FIG. 3. Additionally, the example dynamic 3D lung map view shows that a target 722 which does lie within the region of interest but is not relevant to the current procedure has been hidden, as described above with regard to step S312 of FIG. 3. Target 722 may, for example, be a subsequent target on the current pathway to which the tool will be navigated during the current procedure, but it is not yet relevant to the procedure because at least one other target 510 must first be visited. The current pathway may be divided into two or more portions: a first portion 408 representing the portion of the pathway to be navigated to the current target 510, and additional portions 708 representing the portion of the pathway leading to the next target 722 to be visited. The dynamic 3D lung map view also shows that other objects, such as markers 724, are hidden because they are not relevant to the current procedure. Markers 724 may be, for example, markers indicating the locations where previous biopsies were performed.

By using the dynamic 3D lung map view described above during an ENB procedure, the clinician may be presented with a continuously updated view of the 3D model which is adjusted as the tool, and thus sensor 94, is moved through the patient's airways. The dynamic 3D lung map view presents the clinician with a view of the 3D model from a viewpoint which clearly shows digital probe 406, and removes objects which may obscure digital probe 406, airway tree 404, target 510, and/or other objects which are relevant to the ENB procedure being performed.

Detailed embodiments of devices, systems incorporating such devices, and methods using the same as described herein. However, these detailed embodiments are merely examples of the disclosure, which may be embodied in various forms. Therefore, specific structural and functional details disclosed herein are not to be interpreted as limiting, but merely as a basis for the claims and as a representative basis for allowing one skilled in the art to variously employ the present disclosure in appropriately detailed structure. While the preceding embodiments are described in terms of bronchoscopy of a patient's airways, those skilled in the art will realize that the same or similar devices, systems, and methods may be used in other lumen networks, such as, for example, the vascular, lymphatic, and/or gastrointestinal networks as well.

With respect to memory 202 described above in connection with FIG. 2, the memory 202 may include any nontransitory computer-readable storage media for storing data and/or software that is executable by processor 204 and which controls the operation of workstation 80. In an embodiment, memory 202 may include one or more solid-state storage devices such as flash memory chips. Alterna-

tively or in addition to the one or more solid-state storage devices, memory 202 may include one or more mass storage devices connected to the processor 204 through a mass storage controller (not shown) and a communications bus (not shown). Although the description of computer-readable media contained herein refers to a solid-state storage, it should be appreciated by those skilled in the art that computer-readable storage media can be any available media that can be accessed by the processor 204. That is, computer readable storage media includes non-transitory, volatile and non-volatile, removable and non-removable media implemented in any method or technology for storage of information such as computer-readable instructions, data structures, program modules or other data. For example, 15 computer-readable storage media includes RAM, ROM, EPROM, EEPROM, flash memory or other solid state memory technology, CD-ROM, DVD, Blu-Ray or other optical storage, magnetic cassettes, magnetic tape, magnetic disk storage or other magnetic storage devices, or any other 20 medium which can be used to store the desired information and which can be accessed by workstation 80.

Network interface 208 may be configured to connect to a network such as a local area network (LAN) consisting of a wired network and/or a wireless network, a wide area 25 executed by the processor, further cause the processor to: network (WAN), a wireless mobile network, a Bluetooth network, and/or the internet. Input device 210 may be any device by means of which a user may interact with workstation 80, such as, for example, a mouse, keyboard, foot pedal, touch screen, and/or voice interface. Output module 30 212 may include any connectivity port or bus, such as, for example, parallel ports, serial ports, universal serial busses (USB), or any other similar connectivity port known to those skilled in the art.

Further aspects of image and data generation, manage- 35 ment, and manipulation useable in either the planning or navigation phases of an ENB procedure are more fully described in commonly-owned U.S. Provisional Patent Application Ser. No. 62/020,177 entitled "Methods for Marking Biopsy Location", filed on Jul. 2, 2014, by Brown.; 40 U.S. Provisional Patent Application Ser. No. 62/020,238 entitled "Intelligent Display", filed on Jul. 2, 2014, by Kehat et al.; U.S. Provisional Patent Application Ser. No. 62/020, 242 entitled "Unified Coordinate System for Multiple CT Scans of Patient Lungs", filed on Jul. 2, 2014, by Green- 45 burg.; U.S. Provisional Patent Application Ser. No. 62/020, 245 entitled "Alignment CT", filed on Jul. 2, 2014, by Klein et al.; U.S. Provisional Patent Application Ser. No. 62/020, 250 entitled "Algorithm for Fluoroscopic Pose Estimation", filed on Jul. 2, 2014, by Merlet.; U.S. Provisional Patent 50 Application Ser. No. 62/020,261 entitled "System and Method for Segmentation of Lung", filed on Jul. 2, 2014, by Markov et al.; and U.S. Provisional Patent Application Ser. No. 62/020,258 entitled "Cone View—A Method of Providing Distance and Orientation Feedback While Navigating in 55 3D", filed on Jul. 2, 2014, by Lachmanovich et al., the entire contents of all of which are hereby incorporated by refer-

While several embodiments of the disclosure have been shown in the drawings, it is not intended that the disclosure 60 be limited thereto, as it is intended that the disclosure be as broad in scope as the art will allow and that the specification be read likewise. Therefore, the above description should not be construed as limiting, but merely as exemplifications of particular embodiments. Those skilled in the art will 65 envision other modifications within the scope and spirit of the claims appended hereto.

12

What is claimed is:

- 1. A system comprising:
- a catheter:
- a processor; and
- a memory having stored thereon instructions, which, when executed by the processor, cause the processor to: determine a position of the catheter;
 - present, on a display, a three-dimensional (3D) lung map view of a 3D model showing at least one planned pathway to at least one target in a lung of a patient and the position of the catheter;

adjust the 3D lung map view; and

- show, in the 3D lung map view, at least a part of an object in a way different from a way that other objects forming a part of the 3D model are shown.
- 2. The system of claim 1, wherein the instructions, when executed by the processor, further cause the processor to display a line indicating a line of sight from a tip of the catheter in the 3D lung map view of the 3D model.
- 3. The system of claim 2, wherein the line intersects with the at least one target.
- 4. The system of claim 1, further comprising a sensor located at a tip of the catheter, the position of the catheter being determined based on information from the sensor.
- 5. The system of claim 1, wherein the instructions, when track a position of a probe as the probe is navigated within the lung of the patient; and

register the 3D model with the position of the probe tracked within the lung of the patient.

- 6. The system of claim 1, wherein the object is at least one of a branch of an airway tree overlapping with the planned pathway, a target which is not relevant to a current procedure, an additional target, or a pleura.
- 7. The system of claim 1, wherein the instructions, when executed by the processor, further cause the processor to display a vector from the catheter to the at least one target.
- **8**. The system of claim **1**, wherein showing the part of the object in the way different from the way that the other objects are shown includes hiding or ghosting out the part of the object.
- 9. The system of claim 8, wherein hiding the part of the object includes removing the part of the object from the 3D lung map view.
- 10. The system of claim 9, wherein the instructions, when executed by the processor, further cause the processor to determine that the object is not relevant to the position of the catheter or a state of the catheter, and
 - wherein the removing the part of the object is performed in response to determining that the object is not relevant to the position of the catheter or the state of the catheter.
- 11. The system of claim 9, wherein the instructions, when executed by the processor, further cause the processor to determine that the object is outside a region of interest, and wherein the removing the part of the object is performed in response to determining that the object is outside the region of interest.
- 12. The system of claim 1, wherein showing the part of the object in the way different from the way that the other objects are shown includes altering a transparency of the part of the object.
- 13. The system of claim 1, wherein the instructions, when executed by the processor, further cause the processor to determine that the part of the object is obstructing the catheter or the at least one target, and
 - wherein the showing the part of the object in the way different from the way that the other objects are shown

is performed in response to determining that the part of the object is obstructing the catheter or the at least one target.

* * * * *