



US0D1079014S

(12) **United States Design Patent**
Arakawa et al.

(10) **Patent No.:** **US D1,079,014 S**

(45) **Date of Patent:** **** Jun. 10, 2025**

(54) **PATIENT TABLE**

- (71) Applicant: **Hitachi High-Tech Corporation**,
Tokyo (JP)
- (72) Inventors: **Masayuki Arakawa**, Tokyo (JP); **Yuta Kawaguchi**, Tokyo (JP); **Junpei Hokari**, Tokyo (JP); **Yu Saitoh**, Tokyo (JP); **Takashi Ishizuka**, Tokyo (JP)
- (73) Assignee: **Hitachi High-Tech Corporation**,
Tokyo (JP)
- (**) Term: **15 Years**

- (21) Appl. No.: **29/886,401**
- (22) Filed: **Mar. 8, 2023**

(30) **Foreign Application Priority Data**

- Oct. 31, 2022 (JP) 2022-023697 D
- (51) **LOC (15) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/183**
- (58) **Field of Classification Search**
USPC D24/107, 158-161, 183, 184, 188,
D24/190-192, 200, 201, 212-214;
D6/336, 380, 382, 384, 605, 392
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D462,445 S * 9/2002 Barde D24/183
 - 6,505,364 B2 * 1/2003 Simmons F16P 3/02
108/150
- (Continued)

FOREIGN PATENT DOCUMENTS

- JP D2023-06434 * 1/2024

OTHER PUBLICATIONS

Radiotherapy Table, Online, Published date unknown, Retrieved on Jan. 8, 2025 from URL: <https://www.radiotherapy-patient-system.com/medical-physicists/impact-treatment-table/>.*

(Continued)

Primary Examiner — Justin C Dodson
Assistant Examiner — Eric Eldone Tormanen
(74) *Attorney, Agent, or Firm* — Crowell & Moring LLP

(57) **CLAIM**


The ornamental design for a patient table as shown and described.

DESCRIPTION

FIG. 1 is a front, top and left side perspective view of a patient table according to the design;
 FIG. 2 is a front, top and right side perspective view thereof;
 FIG. 3 is a front, bottom and right side perspective view thereof;
 FIG. 4 is a front view thereof;
 FIG. 5 is a rear view thereof;
 FIG. 6 is a left side view thereof;
 FIG. 7 is a right side view thereof;
 FIG. 8 is a top plan view thereof;
 FIG. 9 is a bottom plan view thereof;
 FIG. 10 is an enlarged cross-sectional view taken along line 10-10 of FIG. 4;
 FIG. 11 is an enlarged view of the portion shown in box labeled "11" in FIG. 1; and,
 FIG. 12 is an enlarged view of the portion shown in box labeled "12" in FIG. 2.

The broken lines illustrate portions of the patient table that form no part of the claimed design. The broken line box shown in FIG. 1 defines the enlarged portion view shown in FIG. 11 and forms no part of the claimed design. The broken line box shown in FIG. 2 defines the enlarged portion view shown in FIG. 12 and forms no part of the claimed design.

1 Claim, 10 Drawing Sheets

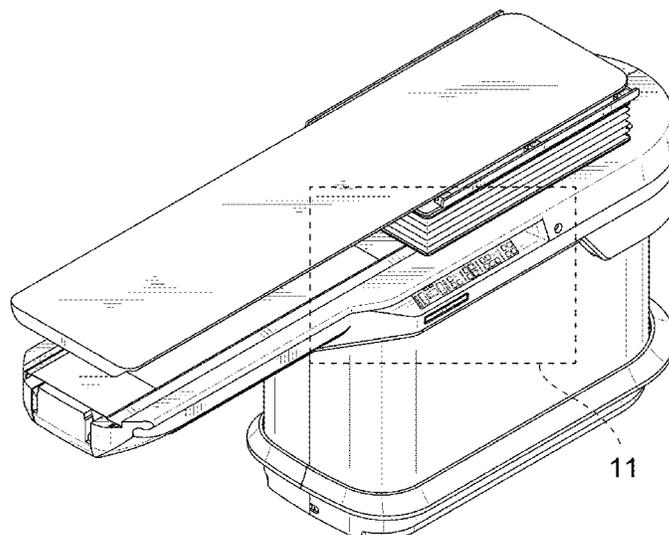

(58) **Field of Classification Search**

CPC A61M 16/101; A61H 1/00; A61G 13/10;
A61G 13/1235; A61G 2210/50

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D630,330	S	*	1/2011	Baba	D24/159
D701,605	S	*	3/2014	Ohmukai	D24/183
D726,319	S	*	4/2015	Sul	D24/159
D727,509	S	*	4/2015	Tan	D24/159
D735,864	S	*	8/2015	Doerre	D24/159
D736,934	S	*	8/2015	Kim	D24/183
D743,555	S	*	11/2015	Hasebe	D24/159
D748,804	S	*	2/2016	Eenboom	D24/183
D757,940	S	*	5/2016	Boegel	D24/159
D820,459	S	*	6/2018	Eenboom	D24/183
D843,583	S	*	3/2019	Roth	D24/159
D855,189	S	*	7/2019	Doerrfuss	D24/183
D865,971	S	*	11/2019	Doerrfuss	D24/183
D897,540	S	*	9/2020	Roth	D24/183
D978,356	S	*	2/2023	Achleitner	D24/183

OTHER PUBLICATIONS

Mitsubishi Heavy Industries, Ltd, "Radiation Therapy Device (Vero 4DRT/MHI-TM2000) Started Treatment Corresponding to the Movement of Cancer Tumor" Kyoto University Hospital, Internet URL: <https://www.mhi.com/jp/news/1109205107.html>, Publication Date Sep. 2011 (five (5) pages), with English translation.

* cited by examiner

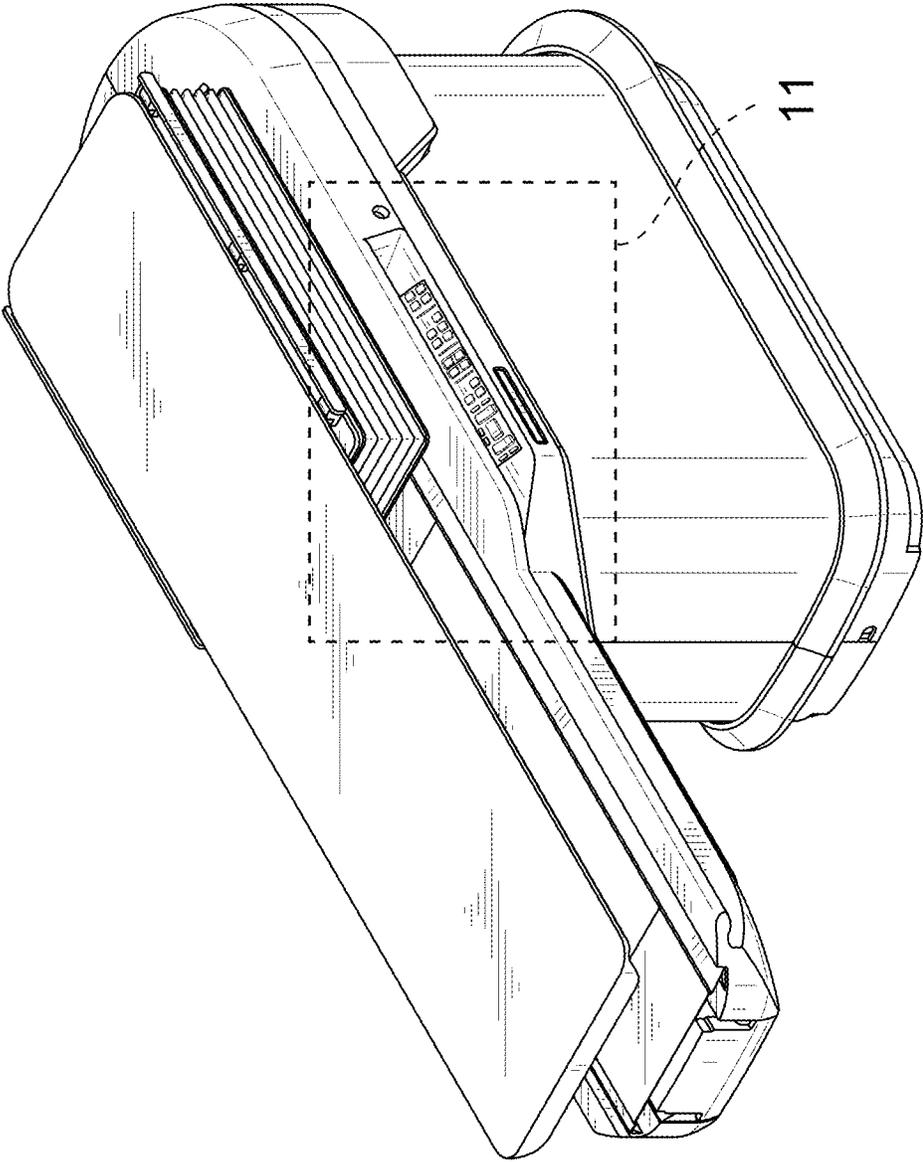


FIG. 1

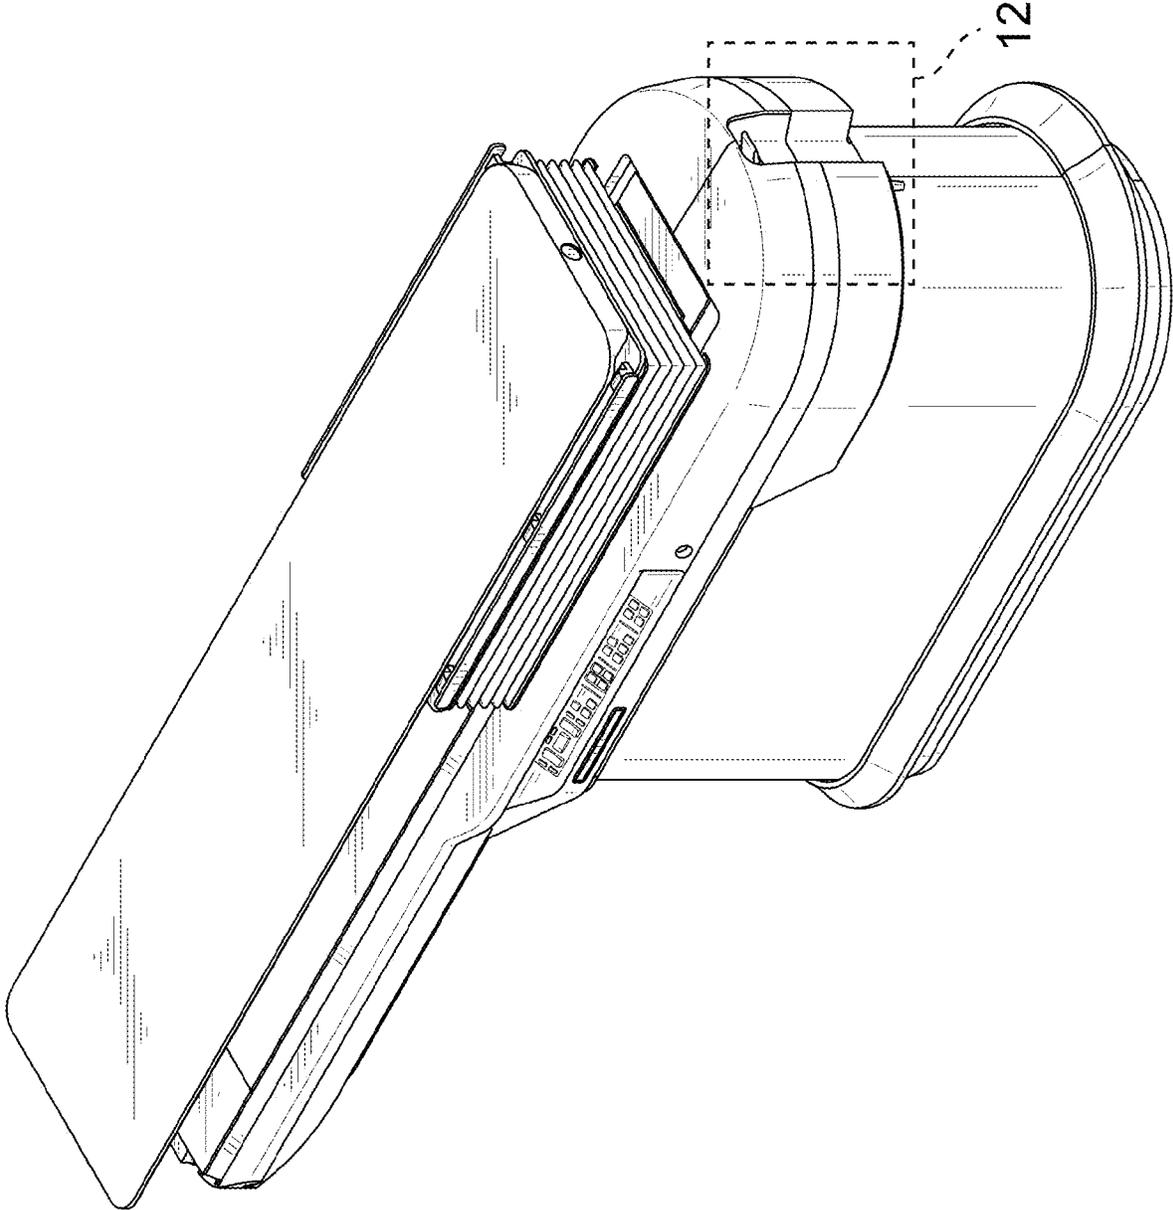


FIG. 2

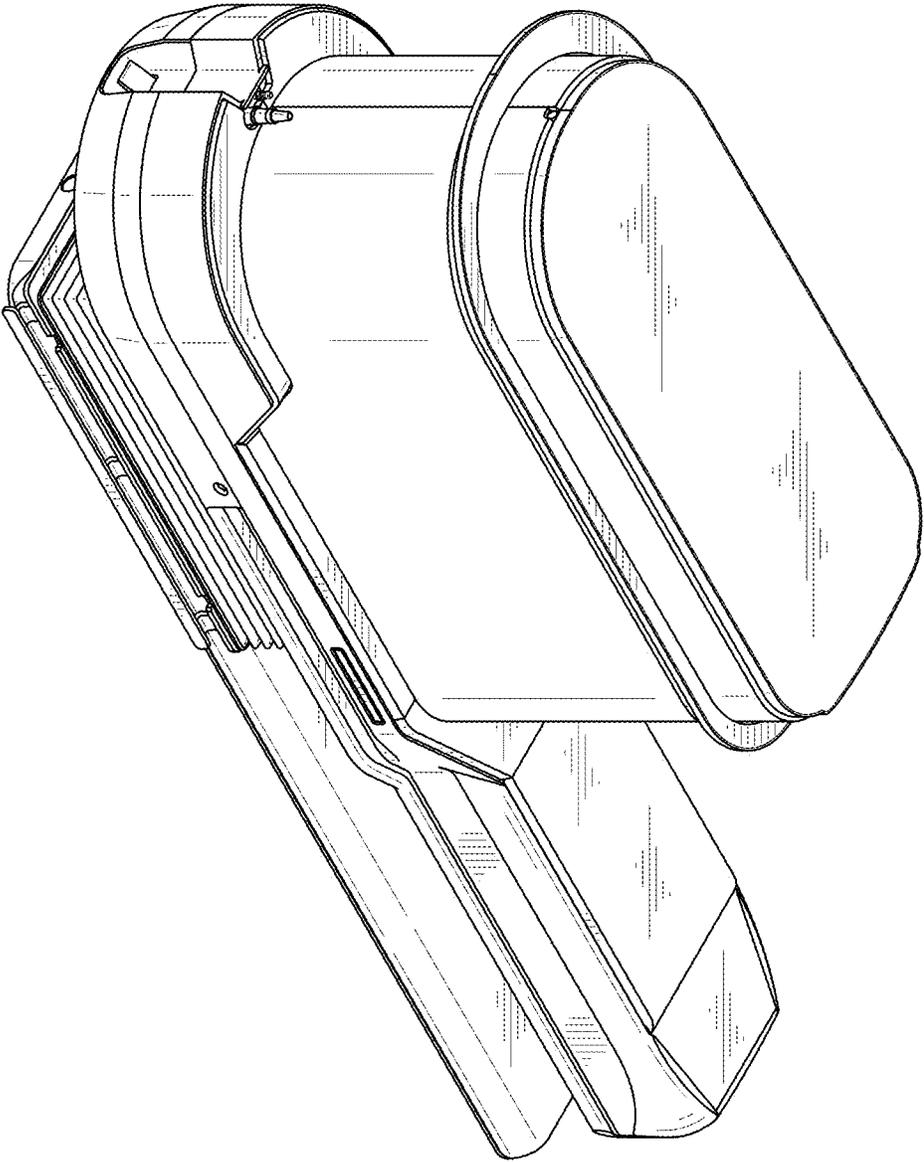


FIG. 3

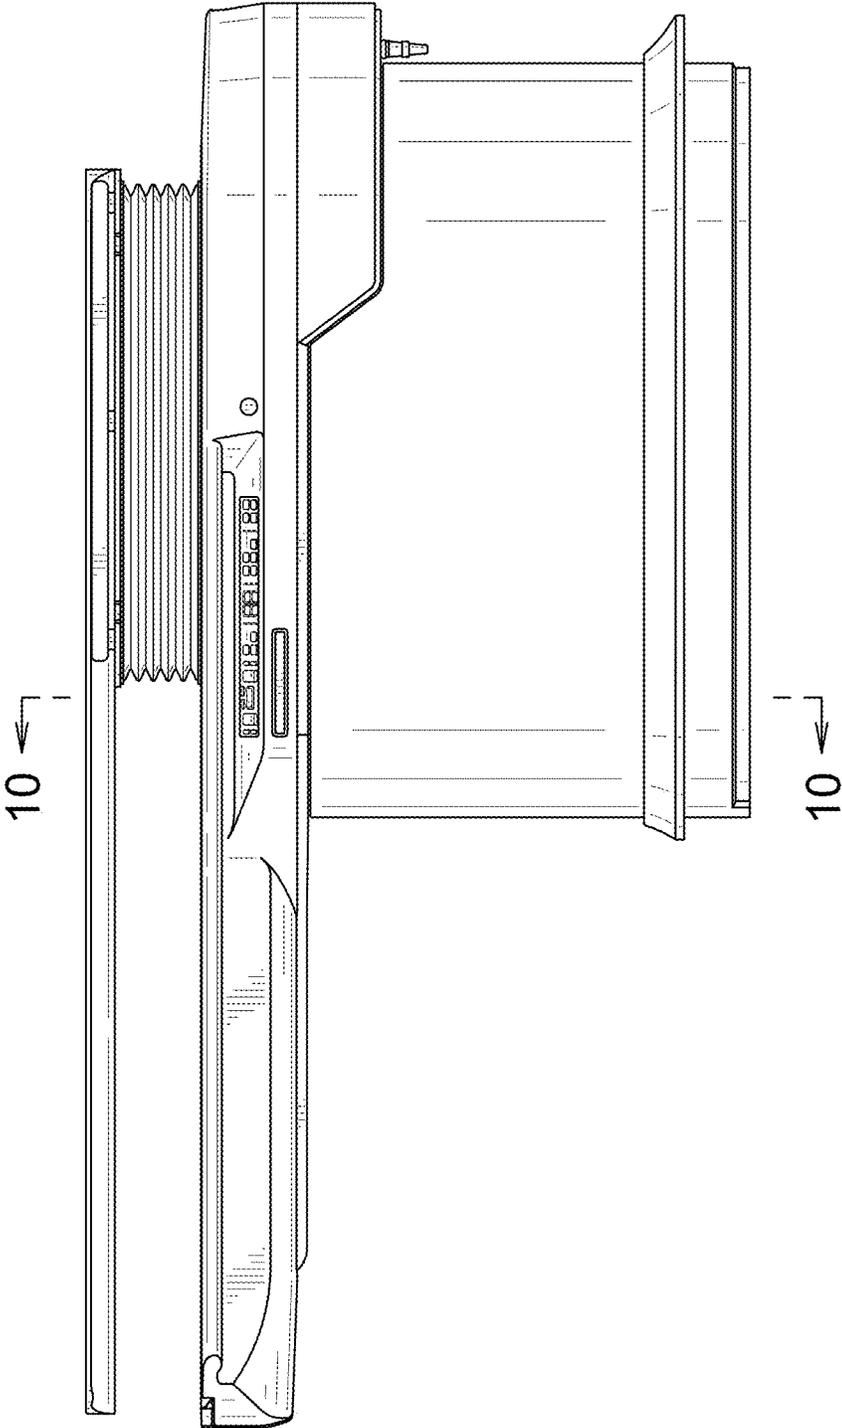


FIG. 4

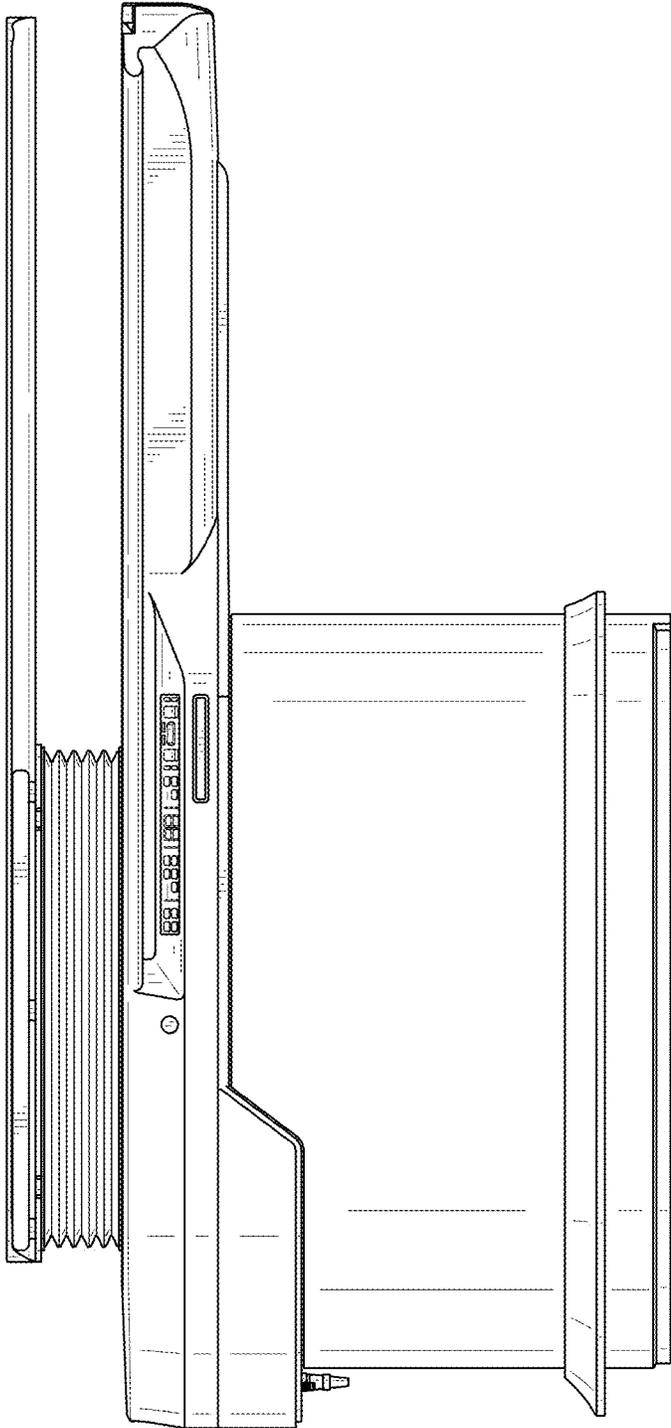


FIG. 5

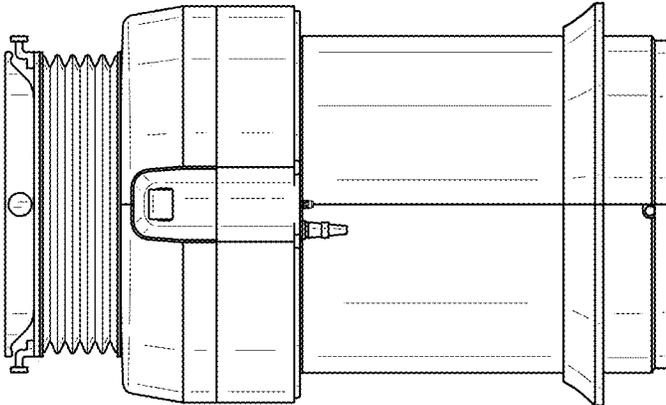


FIG. 7

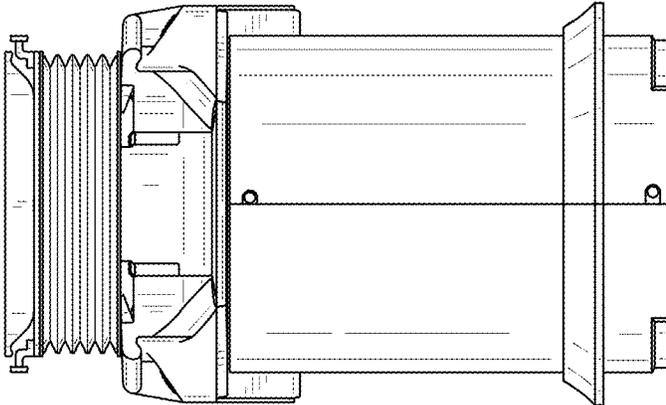


FIG. 6

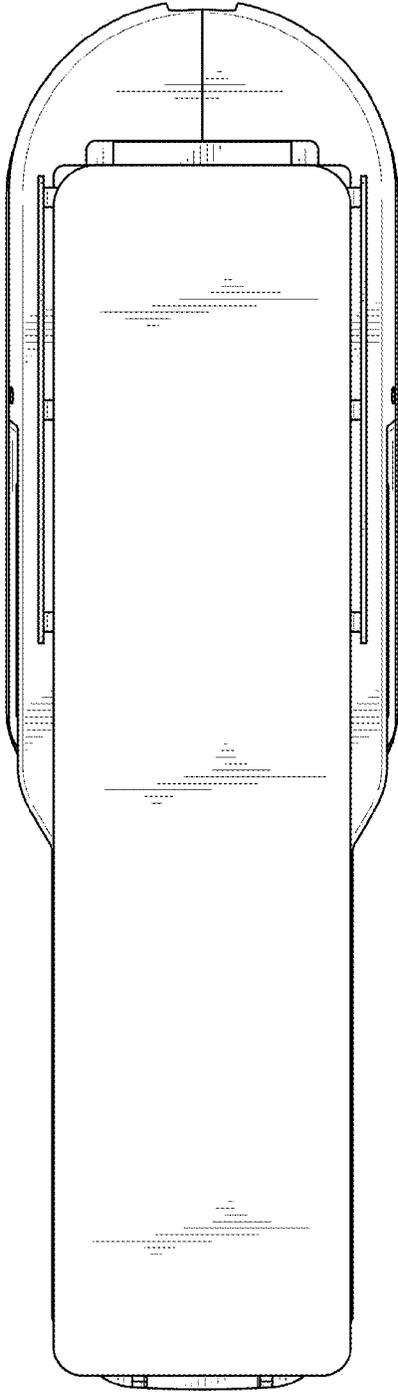


FIG. 8

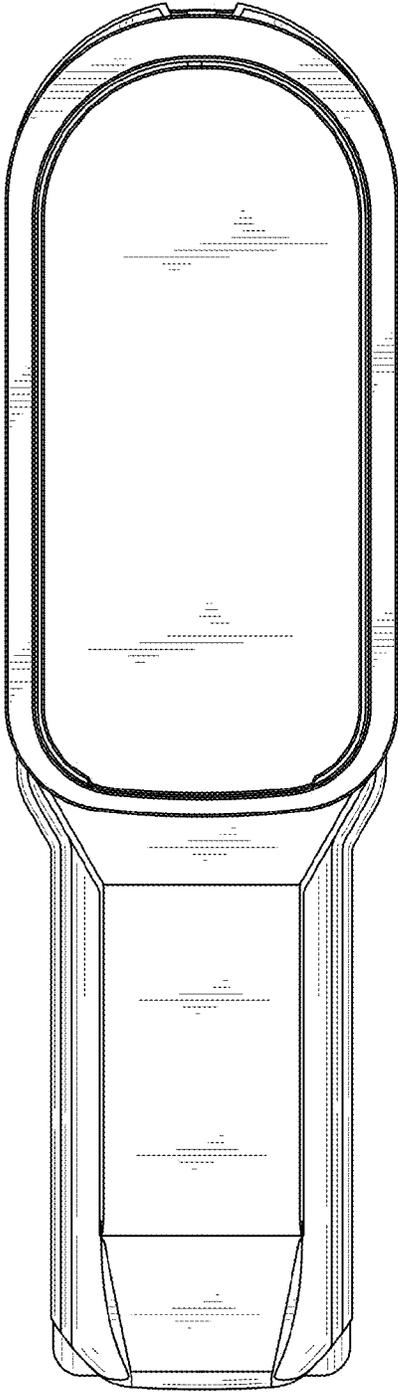


FIG. 9

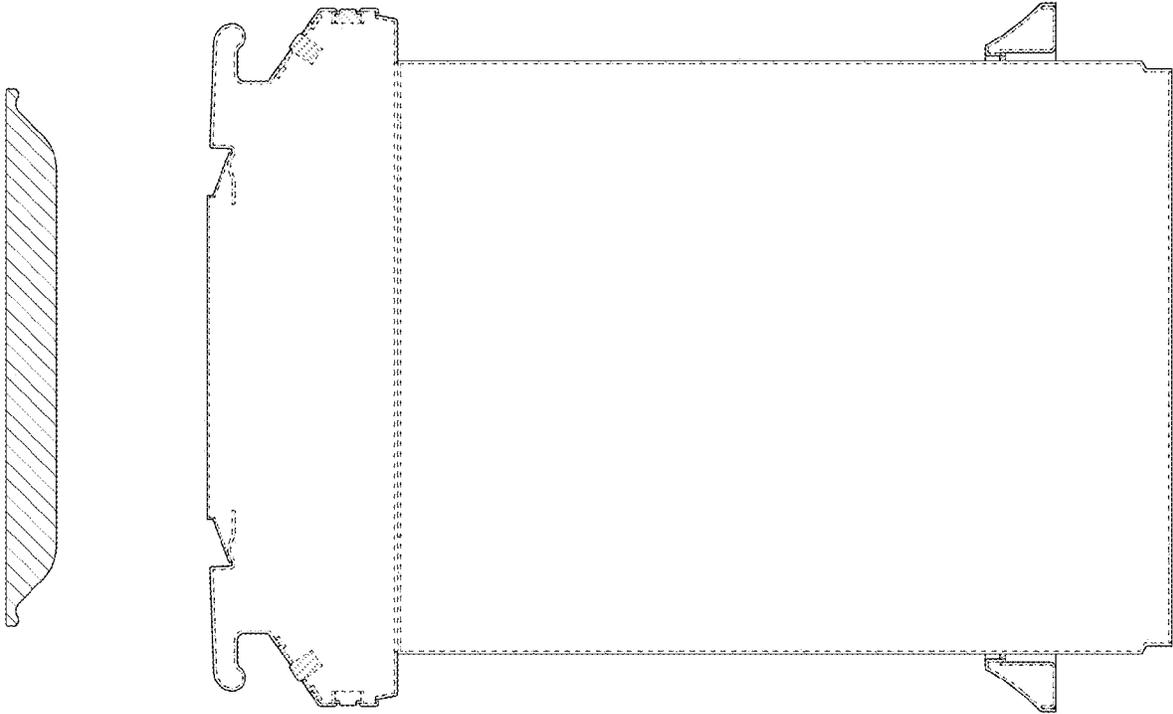


FIG. 10

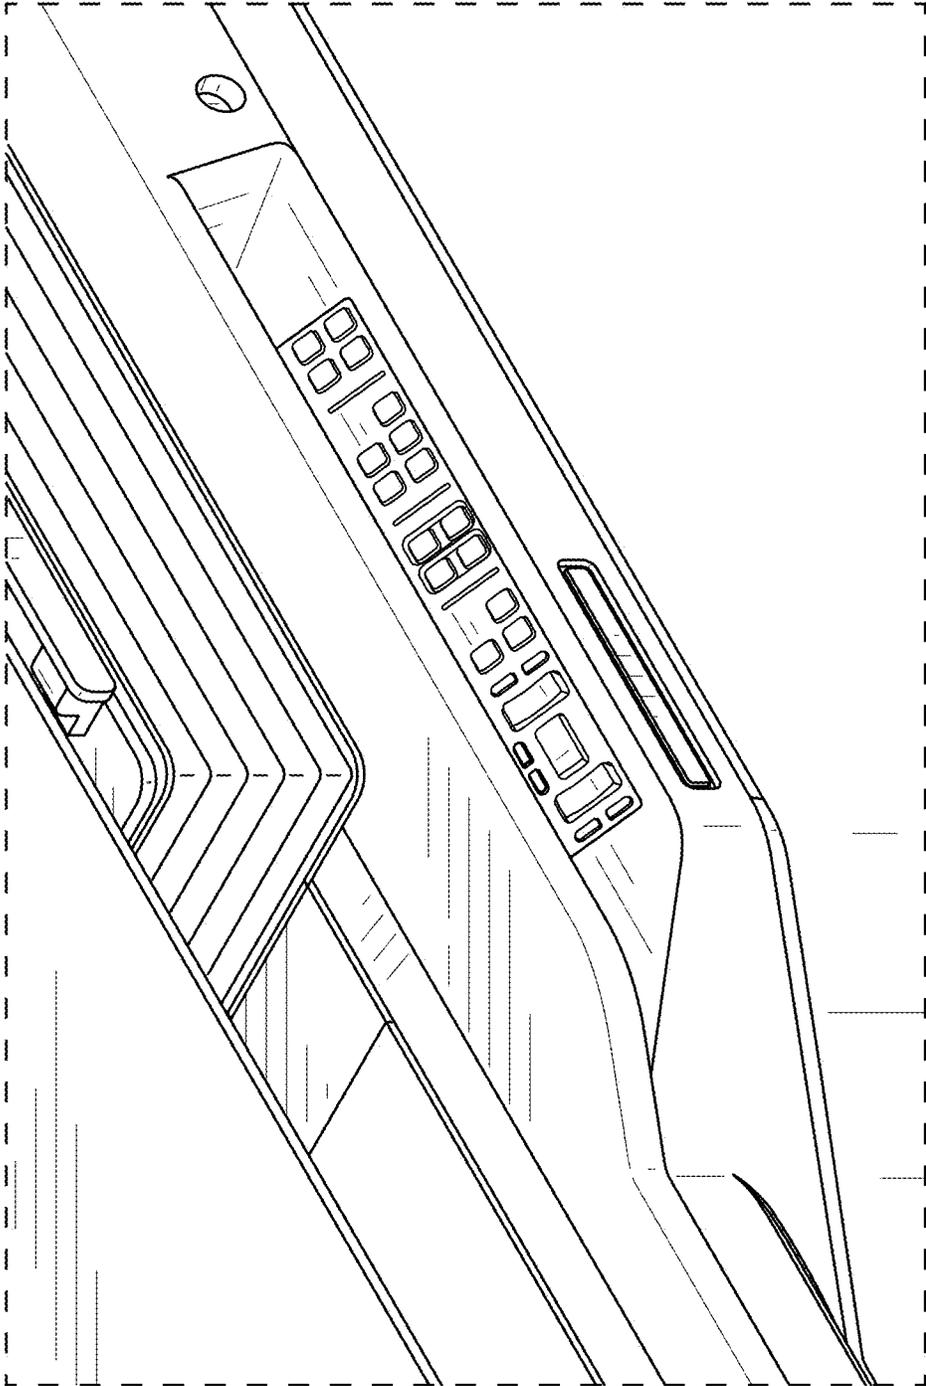


FIG. 11

FIG. 12

