

(19) **DANMARK**

(10) **DK/EP 3157270 T3**



Patent- og  
Varemærkestyrelsen

(12) **Oversættelse af  
europæisk patentskrift**

- 
- (51) Int.Cl.: **H 04 R 25/00 (2006.01)**
- (45) Oversættelsen bekendtgjort den: **2021-06-21**
- (80) Dato for Den Europæiske Patentmyndigheds bekendtgørelse om meddelelse af patentet: **2021-03-31**
- (86) Europæisk ansøgning nr.: **16193673.7**
- (86) Europæisk indleveringsdag: **2016-10-13**
- (87) Den europæiske ansøgnings publiceringsdag: **2017-04-19**
- (30) Prioritet: **2015-10-14 EP 15189769**
- (84) Designerede stater: **AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**
- (73) Patenthaver: **Sonion Nederland B.V., Taurusavenue 143, 2132 LS Hoofddorp, Holland**
- (72) Opfinder: **van Halteren, Aart Zeger, C/o Sonion Nederland B.V., Taurusavenue 143, 2132 LS Hoofddorp, Holland**  
**Taghavi, Hamidreza, C/o Sonion Nederland B.V., Taurusavenue 143, 2132 LS Hoofddorp, Holland**
- (74) Fuldmægtig i Danmark: **Inspicos P/S, Kogle Alle 2, 2970 Hørsholm, Danmark**
- (54) Benævnelse: **Høreaggregat med vibrationsfølsom transducer**
- (56) Fremdragne publikationer:  
**EP-A2- 1 519 625**  
**WO-A1-93/23944**  
**WO-A1-2015/110587**  
**US-A1- 2013 343 584**  
**US-A1- 2015 043 762**



# DESCRIPTION

## FIELD OF THE INVENTION

**[0001]** The present invention relates to a reliable power saving arrangement for hearing devices, including increased comfort for the users of the hearing devices. In particular, the present invention relates to an automatic manner of switching a hearing device on and/or off using a predetermined human voice vibration signal, or to bring the hearing device in and/or out of a power saving state using the predetermined human voice vibration signal.

## BACKGROUND OF THE INVENTION

**[0002]** Various automatic power saving arrangements for hearing devices have been suggested over the years. However, many of the suggested arrangements are unreliable in that they switch the hearing devices on and/or off at inappropriate times which is very annoying for the user of the hearing device. Thus, there seems to be a need for reliable automatic power saving arrangements for hearing devices in order for the hearing aid batteries to last longer, Moreover, there seems to be a need for reliable automatic power saving arrangements for hearing devices for increasing the comfort for the hearing device users, and for making the hearing devices more user-friendly.

**[0003]** Examples of prior art arrangements are disclosed in for example US 2013/343584 A1, EP 1 519 625 A2, US 2015/043762 A1, WO 2015/110587 A1 and WO 93/23944 A1. US 2013/343584 A1 relates to a hearing device involving speech recognition for processing signals provided by a vibration sensor positioned on an outer surface, i.e. at a vulnerable position, of the hearing device. EP 1 519 625 A2 teaches a power saving scheme for a voice controlled hearing device involving a microphone positioned in an ear canal for detecting the user's voice. In order to save power an occluded sound is gated off if the occluded sound is not detected by the microphone in a predetermined time period. US 2015/043762 A1 relates to a hearing device capable of detecting mouth movements of the user by applying a bone conduction sensor. WO 2015/110587 relates to bone conduction and teaches that the head phone housing comprises an opening for accommodating a bone conduction microphone. WO 93/23944 A1 teaches a bone conduction ear piece comprising a housing within which housing a speaker element and a microphone element is provided.

**[0004]** It may be seen as an object of embodiments of the present invention to provide a reliable power saving arrangement for hearing devices, such as hearing aids.

## DESCRIPTION OF THE INVENTION

**[0005]** The above-mentioned object is complied with by providing, in a first aspect, a hearing device according to claim 1.

**[0006]** Thus, the present invention relates to a voice controlled power saving arrangement for hearing devices. In the present context voice generated vibrations should be understood as any type of vibration being generated by the vocal cords of the user of the hearing device, including speech, growl, humming etc.

**[0007]** It is advantageous that by proper signal processing within the DSP the hearing device may only react on the voice of the user of the hearing device in that the DSP may be adapted to apply a voice recognition algorithm to determine the predetermined human voice vibration signal, in particular the voice of the user of the hearing device.

**[0008]** Voice generated vibrations may be present only in a certain frequency band. Moreover, voice generated vibrations may often be comparable to a typical background noise level. Thus, in order for the voice recognition algorithm to operate properly the vibration sensitive transducer must have low noise properties as well as a certain frequency response in terms of sensitivity, damping and low frequency roll off.

**[0009]** The DSP may be a discrete device, or it may form an integral part of the vibration sensitive transducer. In case of a discrete DSP the DSP may be applied for various signal processing within the hearing device, such as signal processing of signals from a microphone or signals to be provided to a receiver. In case of a vibration sensitive transducer comprising an integrated DSP this DSP may process only vibrations signals, and optionally control another DSP of the hearing device.

**[0010]** The DSP may be configured to switch the hearing device on when the predetermined human voice vibration signal is detected. As previously stated the predetermined human voice vibration signal is related to the voice of the user of the hearing device. The DSP is configured to switch the hearing device off when the predetermined human voice vibration signal is not detected in a predetermined time period. Again, the predetermined human voice vibration signal is related to the voice of the user of the hearing device.

**[0011]** The hearing device may further comprise a microphone unit for receiving incoming acoustical signals and a receiver unit for reproducing the incoming acoustical signals.

**[0012]** The vibration sensitive transducer is configured to detect human voice generated vibrations via the skull of the user of the hearing device. In achieve this, the hearing device comprises a shell being adapted to abut the skin of the skull of the user of the hearing device. In order to detect human voice generated vibrations the vibration sensitive transducer may be mechanically connected to said shell, either directly secured to the shell, or connected via a mechanically rigid connection.

**[0013]** In terms of positioning the vibration sensitive transducer may be positioned in the shell

at a point where the voice generated vibrations are dominant, while other types of vibrations, such as receiver generated vibrations, are essentially zero.

**[0014]** During operation the shell of the hearing device is adapted to be positioned between the vibration sensitive transducer and the skull of the user of the hearing device. Thus, the shell of the hearing device is adapted to abut the skin of the skull on one side of the shell, while the vibration sensitive transducer is secured to the opposite side of the shell.

**[0015]** The hearing device of the present invention may further comprise additional transducers, such as accelerometers, rotation sensors and/or gyroscopes. Such additional transducers may be advantageous in case the user of the hearing device has a poor bone conduction transmission through the skull bone. Moreover, additional transducers may be applied for measuring additional user-related activities, such as foot-step counting, fitness and health related indicators etc.

**[0016]** The term hearing device should be understood as any device being capable of increasing the hearing capability of a human being. Thus, the term hearing device may comprise, among other devices, hearing aids being selected from the group consisting of: behind-the-ear, in-the-ear, in-the-canal, invisible-in-canal and completely-in-canal.

**[0017]** In a second aspect the present invention relates to a method for operating a hearing device in accordance with claim 9.

**[0018]** Again, the term hearing device should be understood as any device being capable of increasing the hearing capability of a human being. This may include hearing aids being selected from the group consisting of: behind-the-ear, in-the-ear, in-the-canal, invisible-in-canal and completely-in-canal.

**[0019]** The predetermined human voice vibration signal may be determined using a voice recognition algorithm within the DSP. As mentioned in relation to the first aspect the DSP may be a discrete and multi-purpose component of the hearing device, or it may form an integral part of the vibration sensitive transducer.

**[0020]** In terms of controlling the hearing device may be switched on when the predetermined human voice vibration signal is detected. Likewise, the hearing device is switched off when the predetermined human voice vibration signal is not detected in a predetermined time period. Similar to the first aspect the predetermined human voice vibration signal is associated with the voice of the user of the hearing device. Thus, in terms of controlling, such bringing the hearing device into or out of a power saving state, the hearing device may be configured to react only on the voice of its user, i.e. the person wearing the hearing device. The predetermined human voice vibration signal is detected via the skull of the user of the hearing device by positioning the vibration sensitive transducer in mechanical contact with a shell of the hearing device as explained in relation to the first aspect of the present invention.

**BRIEF DESCRIPTION OF THE DRAWINGS**

**[0021]** The present invention will now be described in further details with reference to the accompanying figures, wherein

Fig. 1 shows part of an in-the-canal hearing aid including a vibration sensor,

Fig. 2 shows part of a behind-the-ear hearing aid including a vibration sensor, and

Fig. 3 shows a simplified electrical block diagram.

**[0022]** While the invention is susceptible to various modifications and alternative forms specific embodiments have been shown by way of examples in the drawings and will be described in details herein. It should be understood, however, that the invention is not intended to be limited to the particular forms disclosed.

**DETAILED DESCRIPTION OF THE INVENTION**

**[0023]** In its broadest aspect the present invention relates to a hearing device, such as a hearing aid, and an associated method where a human voice generated vibration signal is used to control the hearing device in a power saving manner. The human voice generated vibration signal is provided by a vibration sensitive transducer and an appropriate signal processing algorithm of a DSP within the hearing device. The processing of the vibration signal may be performed by a discrete DSP of the hearing device, or it may be performed by a DSP being integrated with for example the vibration sensitive transducer.

**[0024]** The vibration sensitive transducer, such as an electret vibration sensor, is provided for sensing voice generated vibrations via the skull of the user of the hearing device. A suitable approach for providing the human voice generated vibration signal is to apply a voice recognition algorithm to the signal from the vibration sensitive transducer. The voice recognition algorithm may apply a modulation analysis scheme in that human voice modulation is a very unique identifier. By following this approach the hearing device will only respond to voice vibrations originating from the user of the hearing device.

**[0025]** In terms of controlling, the hearing device may for example be switched on or switched off in response to vibrations being generated by the user's voice. However, other control schemes are also applicable as it will be disclosed in the following.

**[0026]** Referring now to Fig. 1 a part of an in-the-canal hearing aid 100 is depicted. As seen in Fig. 1 the vibration sensor 102 is secured directly to the shell 101 of the hearing aid. In this

way human voice generated vibrations may be detected when the shell is positioned in the ear canal. In Fig. 2 a part of a behind-the-ear hearing aid 200 is depicted. As seen the vibration sensor 202 is secured directly to the shell 201 so that vibrations may be detected via the skull when the hearing device 200 is positioned behind the ear. Additional electronic components 203 are also shown in Fig. 2. Fig. 3 shows a simplified electronic block diagram 300. The block diagram 300 shows a DSP 301 being adapted to process signals from a microphone 303 before forwarding it to the receiver 304 for reproduction. A vibration sensor 302 is provided for sensing voice generated vibrations. The vibration sensor 302 is operatively connected to the DSP 301 so that the software provided therein may be used to process the vibration signals in order to identify predetermined human voice vibration signals. Such signals may be identified using voice recognition programs, including for example modulation analysing programs. The DSP is configured to control the hearing device in response to the detection of the predetermined human voice vibration signals, cf. the description below.

**[0027]** The signal from the vibration sensitive transducer may be passed through a band- pass filter in order to remove noises and disturbances.

**[0028]** Generally, a hearing device may apply a vibration sensitive transducer for automatic on/off control as well as other ways to change the power state of the hearing device. The various vibration-based control scenarios may be divided as follows:

- 6) Basic setup
- 7) Using sleep mode
- 8) Using other sensors
- 9) Using wired or wireless recharging
- 10) Improvements

**[0029]** The basic setup has already been disclosed above, i.e. an arrangement for automatic on/off control of a hearing device. Such an arrangement can only work in a reliable manner if a characteristic being unique to a human being can be applied, in particular a parameter that has a unique range.

**[0030]** One possible approach to gain information would be to pick-up the vibrations generated by a human voice in the ear-canal using the vibration sensor, such as an electret vibration sensor which is hermetically closed. In an electret vibration sensor a moving back-plate is used to get a large moving mass and thus the required sensitivity. A MEMS-based vibration sensor may be applicable as well despite its lower sensitivity.

**The basic setup:**

**[0031]** The vibration sensor requires mechanical contact to the human skull through either the skin in the ear-canal, or the skin around the ear in case of a BTE. The vibration sensor is always switched on, but uses only very little current (down to 2  $\mu$ A). Thus, when the hearing device is positioned in a drawer, on a table or in another position where it is not in vibrational contact with a human being, only a very little amount of electrical power is used. The remaining components of the hearing device use very little power as well. For example only part of the DSP is applied to process the signal from the vibration sensor. A significant amount of power can also be saved by only processing the vibration sensor signal at a low duty cycle, and only if the vibration sensor signal is above a certain level. The total quiescent current may be as low as 20  $\mu$ A.

**[0032]** If the signal from the vibration sensor is above a certain level the DSP will determine if the signal resembles a human voice using the same software as used for classifying the acoustic scene in the hearing device. For instance the DSP software may analyze the modulation of the vibration sensor signal since the human voice has a very unique modulation. If the vibration signal does not resemble the human voice no change of the state of operation of the hearing device is provided. On the other hand if the voice of the user of the hearing device is recognized, then the hearing device will switch on, assuming that it is positioned in either 1) the ear-canal or 2) on/behind the ear. The hearing device stays in the on-state for at least a certain time of period, say for example 30 minutes. During this period of time the hearing device will at least once process the vibration signal again and act in response thereto.

**[0033]** If the user of the hearing device has been silent for a period of time the hearing device will provide a warning signal, such as a beep or a message, before eventually switching off. The beep or message informs the user that the hearing device will switch off within a certain period of time, such as within one a minute. Then the hearing device goes into a super sensitive mode to detect a swallow, scratching throat or other patterns as a special event. If the user of the hearing device reacts to the warning signal by in somehow using his/hers voice or any predetermined patterns, the hearing device will stay switched on. It should be noted however that other control schemes are applicable as well. If the user of the hearing device does not react on the warning signal, the hearing device will switch off in order to save power.

**[0034]** To make the hearing device a user-friendly device, it will provide a beep or the like when starting up since the typical startup cycle might take 10 seconds for some hearing aids. The user might get confused if he puts the hearing device in his ear-canal or on/behind his ear. The user of the hearing device must be instructed to in somehow use his voice (scratch the throat, say any word etc.). This way of controlling the hearing device is completely reliable in that if a third person talks to the user of the hearing device, and the user does not understand, the user will say at least some words which will initiate switch on of the hearing device. The hearing device will then provide a beep or the like and subsequently startup. The user of the hearing device will then be able to hear again.

**The sleep mode:**

**[0035]** In order to save power, modern microphones/vibration sensors may have a build-in sleep mode. In this sleep mode they use only very little power, i.e. a very low average current where the performance is low as well. Alternatively, the power saving mode may be provided by operating at a low duty cycle. Even in this power saving mode modern microphones/vibration sensors can wake up and are still able to process the voice identification on their own. In that case the DSP is completely switched off and all the intelligence is positioned in the modern microphone/vibration sensor for switching the hearing device on. However, the DSP still plays a role when the hearing device is to be switched off.

**[0036]** Alternatively, the DSP itself can also have a sleep mode. For example when the user of the hearing device does not use his voice above a certain level perhaps for some time, it must be assumed that the user is also in a situation where speech communication is not taking place, or at least is less important. If the user of the hearing device does not communicate, uses his/hers voice, then the user related voice level picked-up by the hearing device decreases and the acoustical signal processing can be used for switching the DSP to a sleep mode. The hearing device then goes into a power saving mode with reduced processing. For example the hearing device could switch off all advanced signal processing. The same algorithms may be applied for voice detection as well.

**[0037]** Thus, according to the present invention the vibration sensor may be used to switch the DSP into a sleep mode. The hearing device will leave the sleep mode when the user of the hearing device uses his voice above a certain sound level.

**[0038]** Another interesting possibility would be to use the same setup to open and close a valve. The following approach could be imagined in relation to anti-occlusion: If the user of the hearing device uses his voice a valve could open (and have no occlusion). When the user of the hearing device stops talking the valve is closed which enables very high gain.

**Using other types of sensors:**

**[0039]** In general, the process of putting the hearing device in a different power state could also be initiated by other types of sensors, such as for example rotation sensors, accelerometers, gyroscopes or other sensors that are capable of indicating that the hearing device in somehow moves. The overall functioning would however be the same as in the case of a vibration sensor.

**Wired or wireless charging:**

**[0040]** When using wireless or wired charging, the hearing device will know that it is in a

charging mode and can always be switched off in that situation.

**Improvements:**

[0041] During fitting of the hearing device, or after any startup of the hearing device the classification software can be calibrated to the user. For instance each hearing device user has a different spectrum for the vibration which is pretty unique. The combination of the basic resonance frequency in the low frequency end, the higher resonances due to the size and mechanical behavior of the ear canal, the mechanical transmission paths between where the user's voice is generated and where the vibration signal is picked up, defines a unique 'finger print'. This may also help in relation to the very small percentage of hearing device users that have a much lower vibration transmission. In this case, a software backup is needed, for example the user of the hearing device can tap on the hearing device to avoid sleep mode or switching off the device. There might be cases where one has to switch off the system and rely on other things.

## REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

**Patent documents cited in the description**

- [US2013343584A1 \[0003\] \[0003\]](#)
- [EP1519625A2 \[0003\] \[0003\]](#)
- [US2015043762A1 \[0003\] \[0003\]](#)
- [WO2015110587A1 \[0003\]](#)
- [WO9323944A1 \[0003\] \[0003\]](#)
- [WO2015110587A \[0003\]](#)

PATENTKRAV

1. Høreaggregat (100), der omfatter

- en vibrationsfølsom transducer (102), der er indrettet til at detektere vibrationer, der fremkaldes af en menneskelig stemme, og
- en digital signalprocessor til behandling af signaler fra den vibrationsfølsomme transducer (102) med henblik på at identificere et på forhånd fastlagt vibrationssignal fra en menneskelig stemme, der er knyttet til stemmen af brugeren af høreaggregatet (100) og styring af høreaggregatet (100) i overensstemmelse hermed

hvor den vibrationsfølsomme transducer (102) er fastgjort til en skal (101) af høreaggregatet (100), således at vibrationerne detekteres via kraniet af brugeren af høreaggregatet (100),

kendetegnet ved, at skallen (101) af høreaggregatet (100), under drift, er indrettet til at blive anbragt mellem den vibrationsfølsomme transducer (102) og kraniet af brugeren af høreaggregatet (100), ved at skallen (101) af høreaggregatet (100) er indrettet til at ligge op til huden på kraniet på den ene side af skallen (101), mens den vibrationsfølsomme transducer (102) er fastgjort til den modsatte side af skallen (101), og at

den digitale signalprocessor er konfigureret til at slukke for høreaggregatet (100), når det på forhånd fastlagte vibrationssignal fra en menneskelig stemme ikke identificeres i en på forhånd fastlagt tidsperiode.

2. Høreaggregat (100) ifølge krav 1, kendetegnet ved, at den digitale signalprocessor er indrettet til at anvende en stemmegenkendelsesalgoritme for at identificere det på forhånd fastlagte vibrationssignal fra en menneskelig stemme.
3. Høreaggregat (100) ifølge krav 1 eller 2, kendetegnet ved, at den digitale signalprocessor er en diskret anordning, eller hvor den digitale signalprocessor danner en integreret del af den vibrationsfølsomme transducer (102).
4. Høreaggregat (100) ifølge et hvilket som helst af kravene 1 til 3, kendetegnet ved, at den digitale signalprocessor er konfigureret til at tænde for høreaggregatet (100), når det på forhånd fastlagte vibrationssignal fra en menneskelig stemme identificeres.
5. Høreaggregat (100) ifølge et hvilket som helst af kravene 1 til 4, der desuden omfatter en mikrofonenhed til modtagelse af indgående akustiske signaler og en lyd giverenhed til reproduktion af de indgående akustiske signaler.
6. Høreaggregat (100) ifølge et hvilket som helst af kravene 1 til 5, kendetegnet ved, at den vibrationsfølsomme transducer (102) er fastgjort mekanisk til skallen af høreaggregatet.
7. Høreaggregat (100) ifølge et hvilket som helst af de foregående krav, der desuden omfatter yderligere transducere som f.eks. accellerometre, rotationssensorer og/eller gyroskoper.
8. Høreaggregat (100) ifølge et hvilket som helst af de foregående krav, hvilket høreaggregat (100) omfatter et

høreapparat, der udvælges fra gruppen bestående af: "bag-ved-øret", "i-øret", "i-kanalen", "usynligt-i-kanalen" og "fuldstændigt-i-kanalen".

9. Fremgangsmåde til at drive et høreaggregat (100), der omfatter en vibrationsfølsom transducer (102), der er driftsmæssigt forbundet med en digital signalprocessor, hvor den vibrationsfølsomme transducer (102) er fastgjort til en skal (101) af høreaggregatet (100), og hvor den vibrationsfølsomme transducer (102) er indrettet til at detektere vibrationer via kraniet af brugeren af høreaggregatet (100), hvilken fremgangsmåde omfatter følgende trin:

- identifikation af et på forhånd fastlagt vibrationssignal fra en menneskelig stemme ved hjælp af den vibrationsfølsomme transducer (102) og signalbehandlingsevnen af den digitale signalprocessor, hvor det på forhånd fastlagte vibrationssignal fra en menneskelig stemme er knyttet til stemmen af brugeren af høreaggregatet (100), og
- styring af høreaggregatet (100) i overensstemmelse med det identificerede på forhånd fastlagte vibrationssignal fra en menneskelig stemme

kendetegnet ved, at skallen (101) af høreaggregatet (100) er anbragt mellem den vibrationsfølsomme transducer (102) og kraniet af brugeren af høreaggregatet (100), ved at skallen (101) på høreaggregatet (100) ligger op til huden på kraniet på den ene side af skallen (101), mens den vibrationsfølsomme transducer (102) er fastgjort til den modsatte side af skallen (101), og ved at

høreaggregatet (100) slukkes, når det på forhånd fastlagte vibrationssignal fra en menneskelig stemme ikke identificeres i en på forhånd fastlagt tidsperiode.

10. Fremgangsmåde ifølge krav 9, kendetegnet ved, at vibrationssignalet fra den menneskelige stemme identificeres ved hjælp af en stemmegenkendelsesalgoritme i den digitale signalprocessor.
11. Fremgangsmåde ifølge krav 9 eller 10, kendetegnet ved, at høreaggregatet (100) tændes, når det på forhånd fastlagte vibrationssignal fra en menneskelig stemme identificeres.

# DRAWINGS

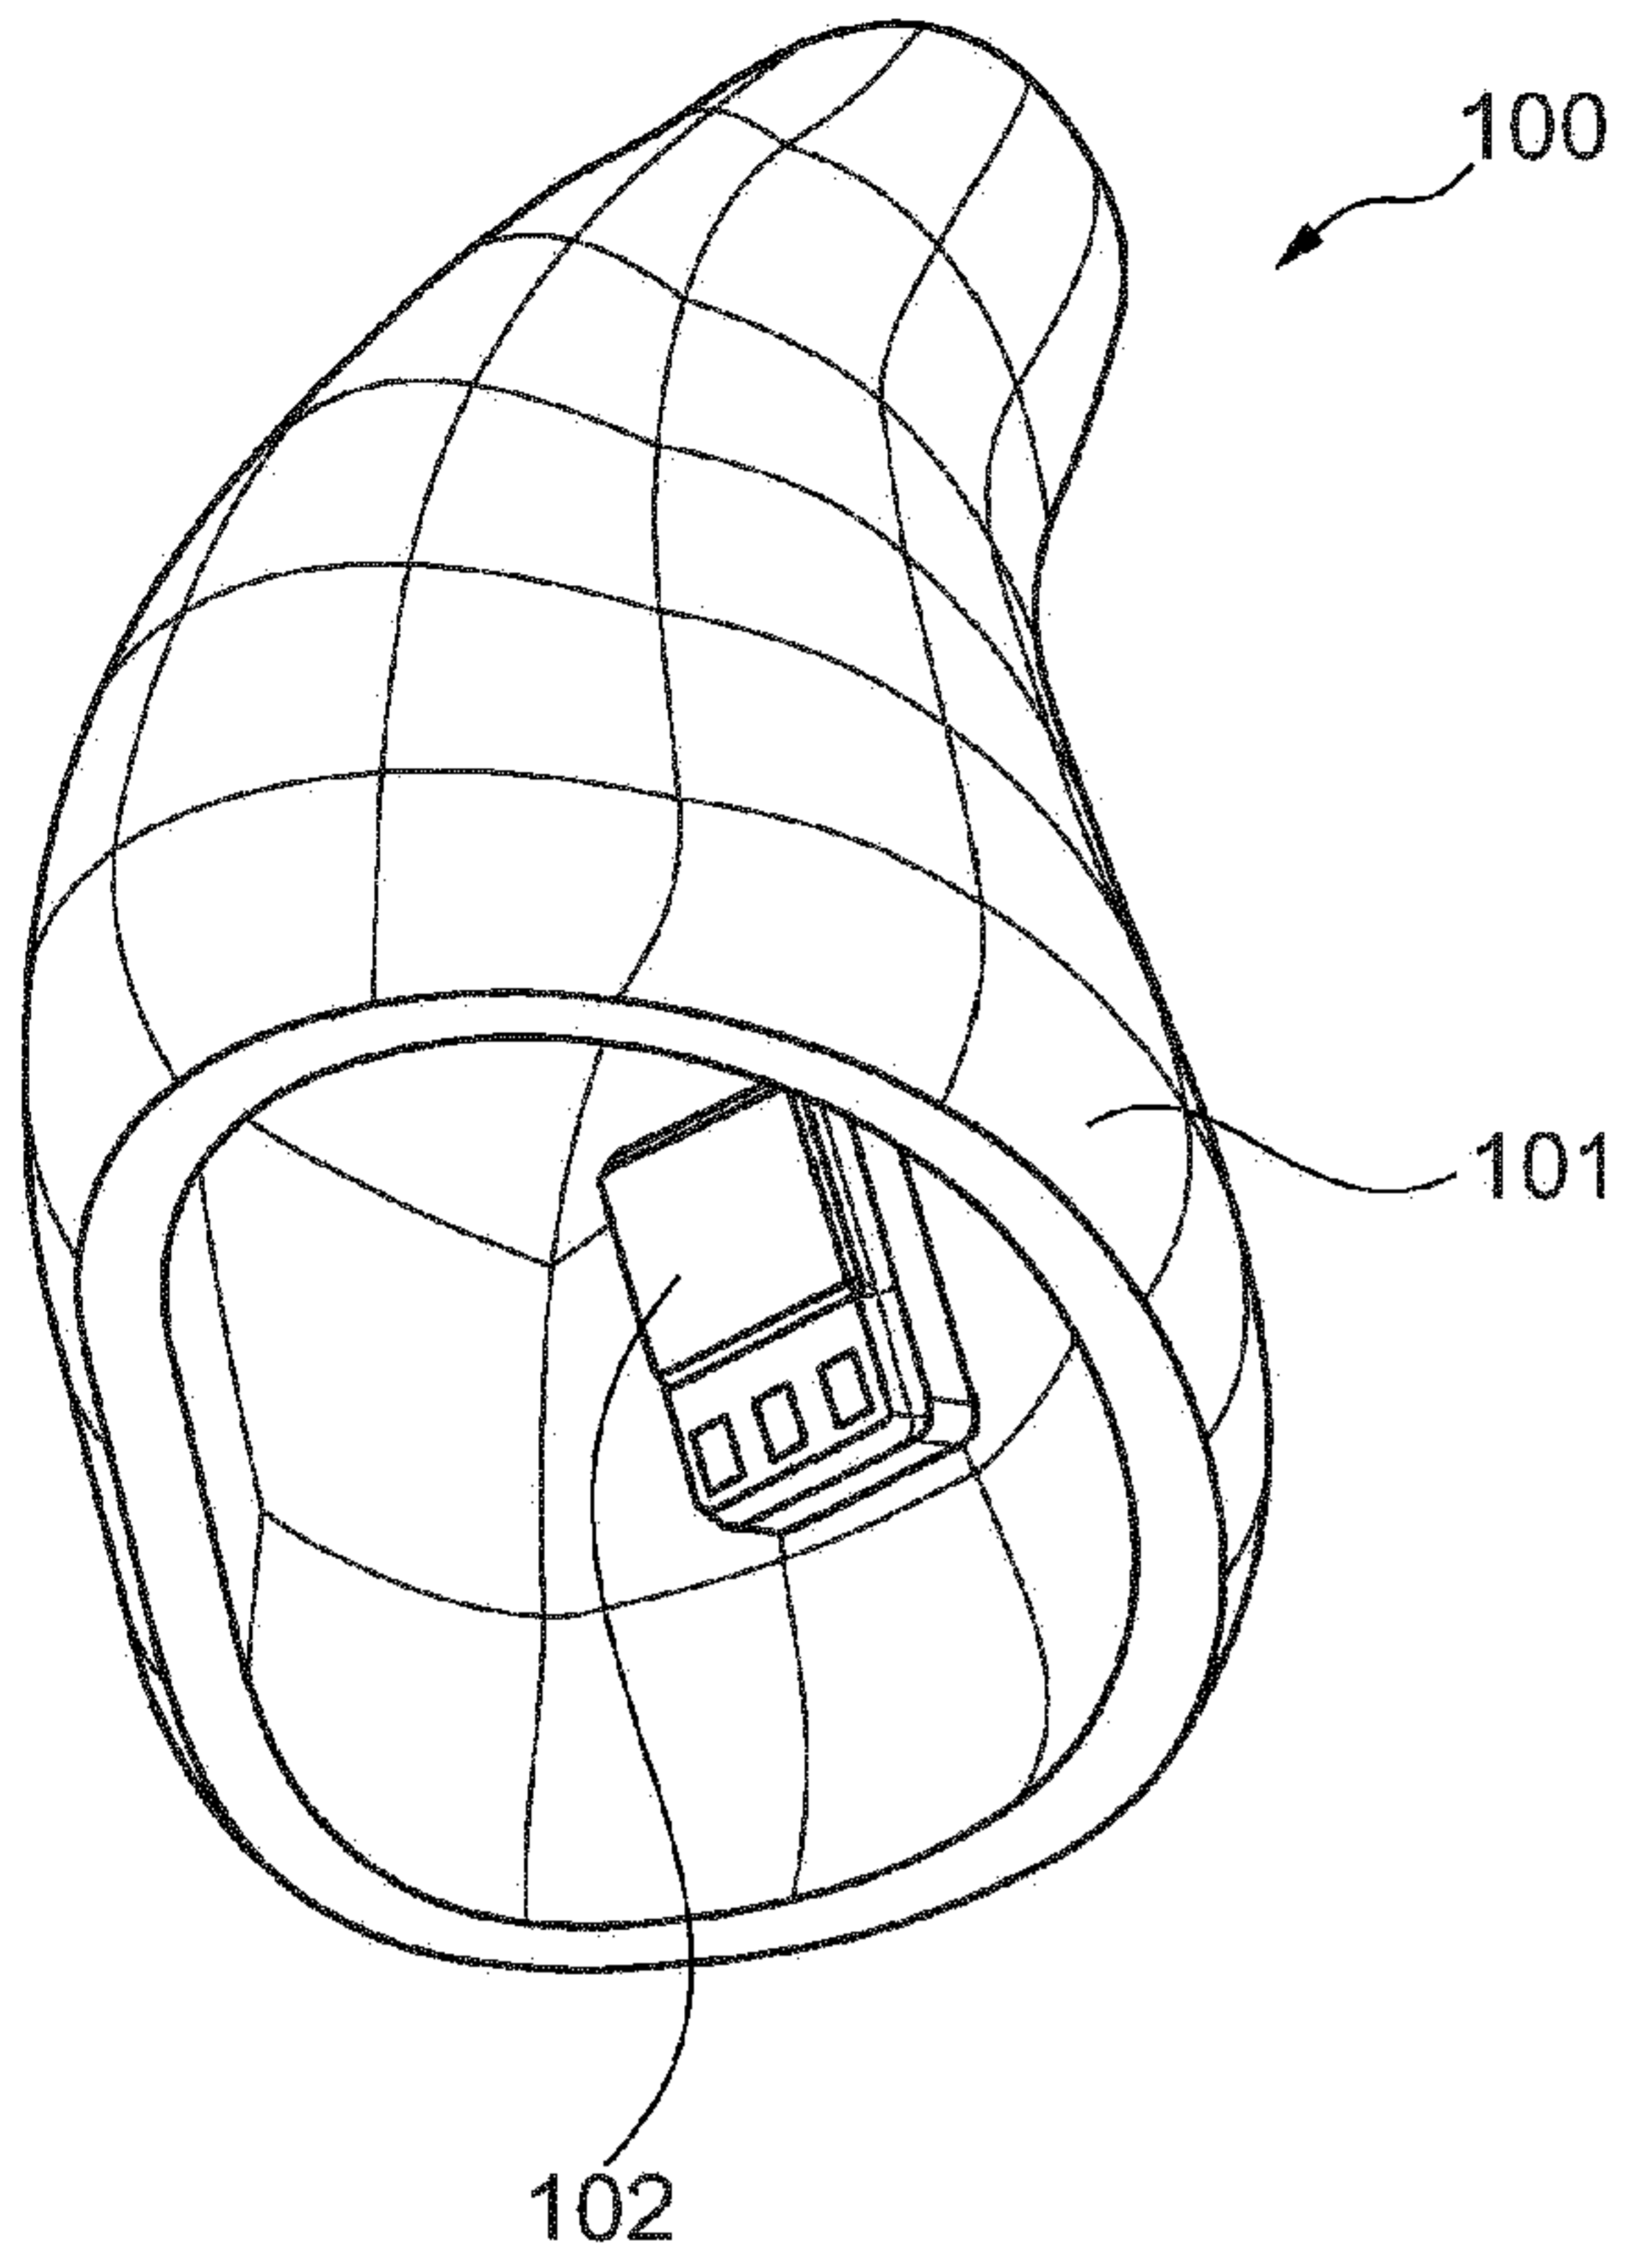


Fig. 1

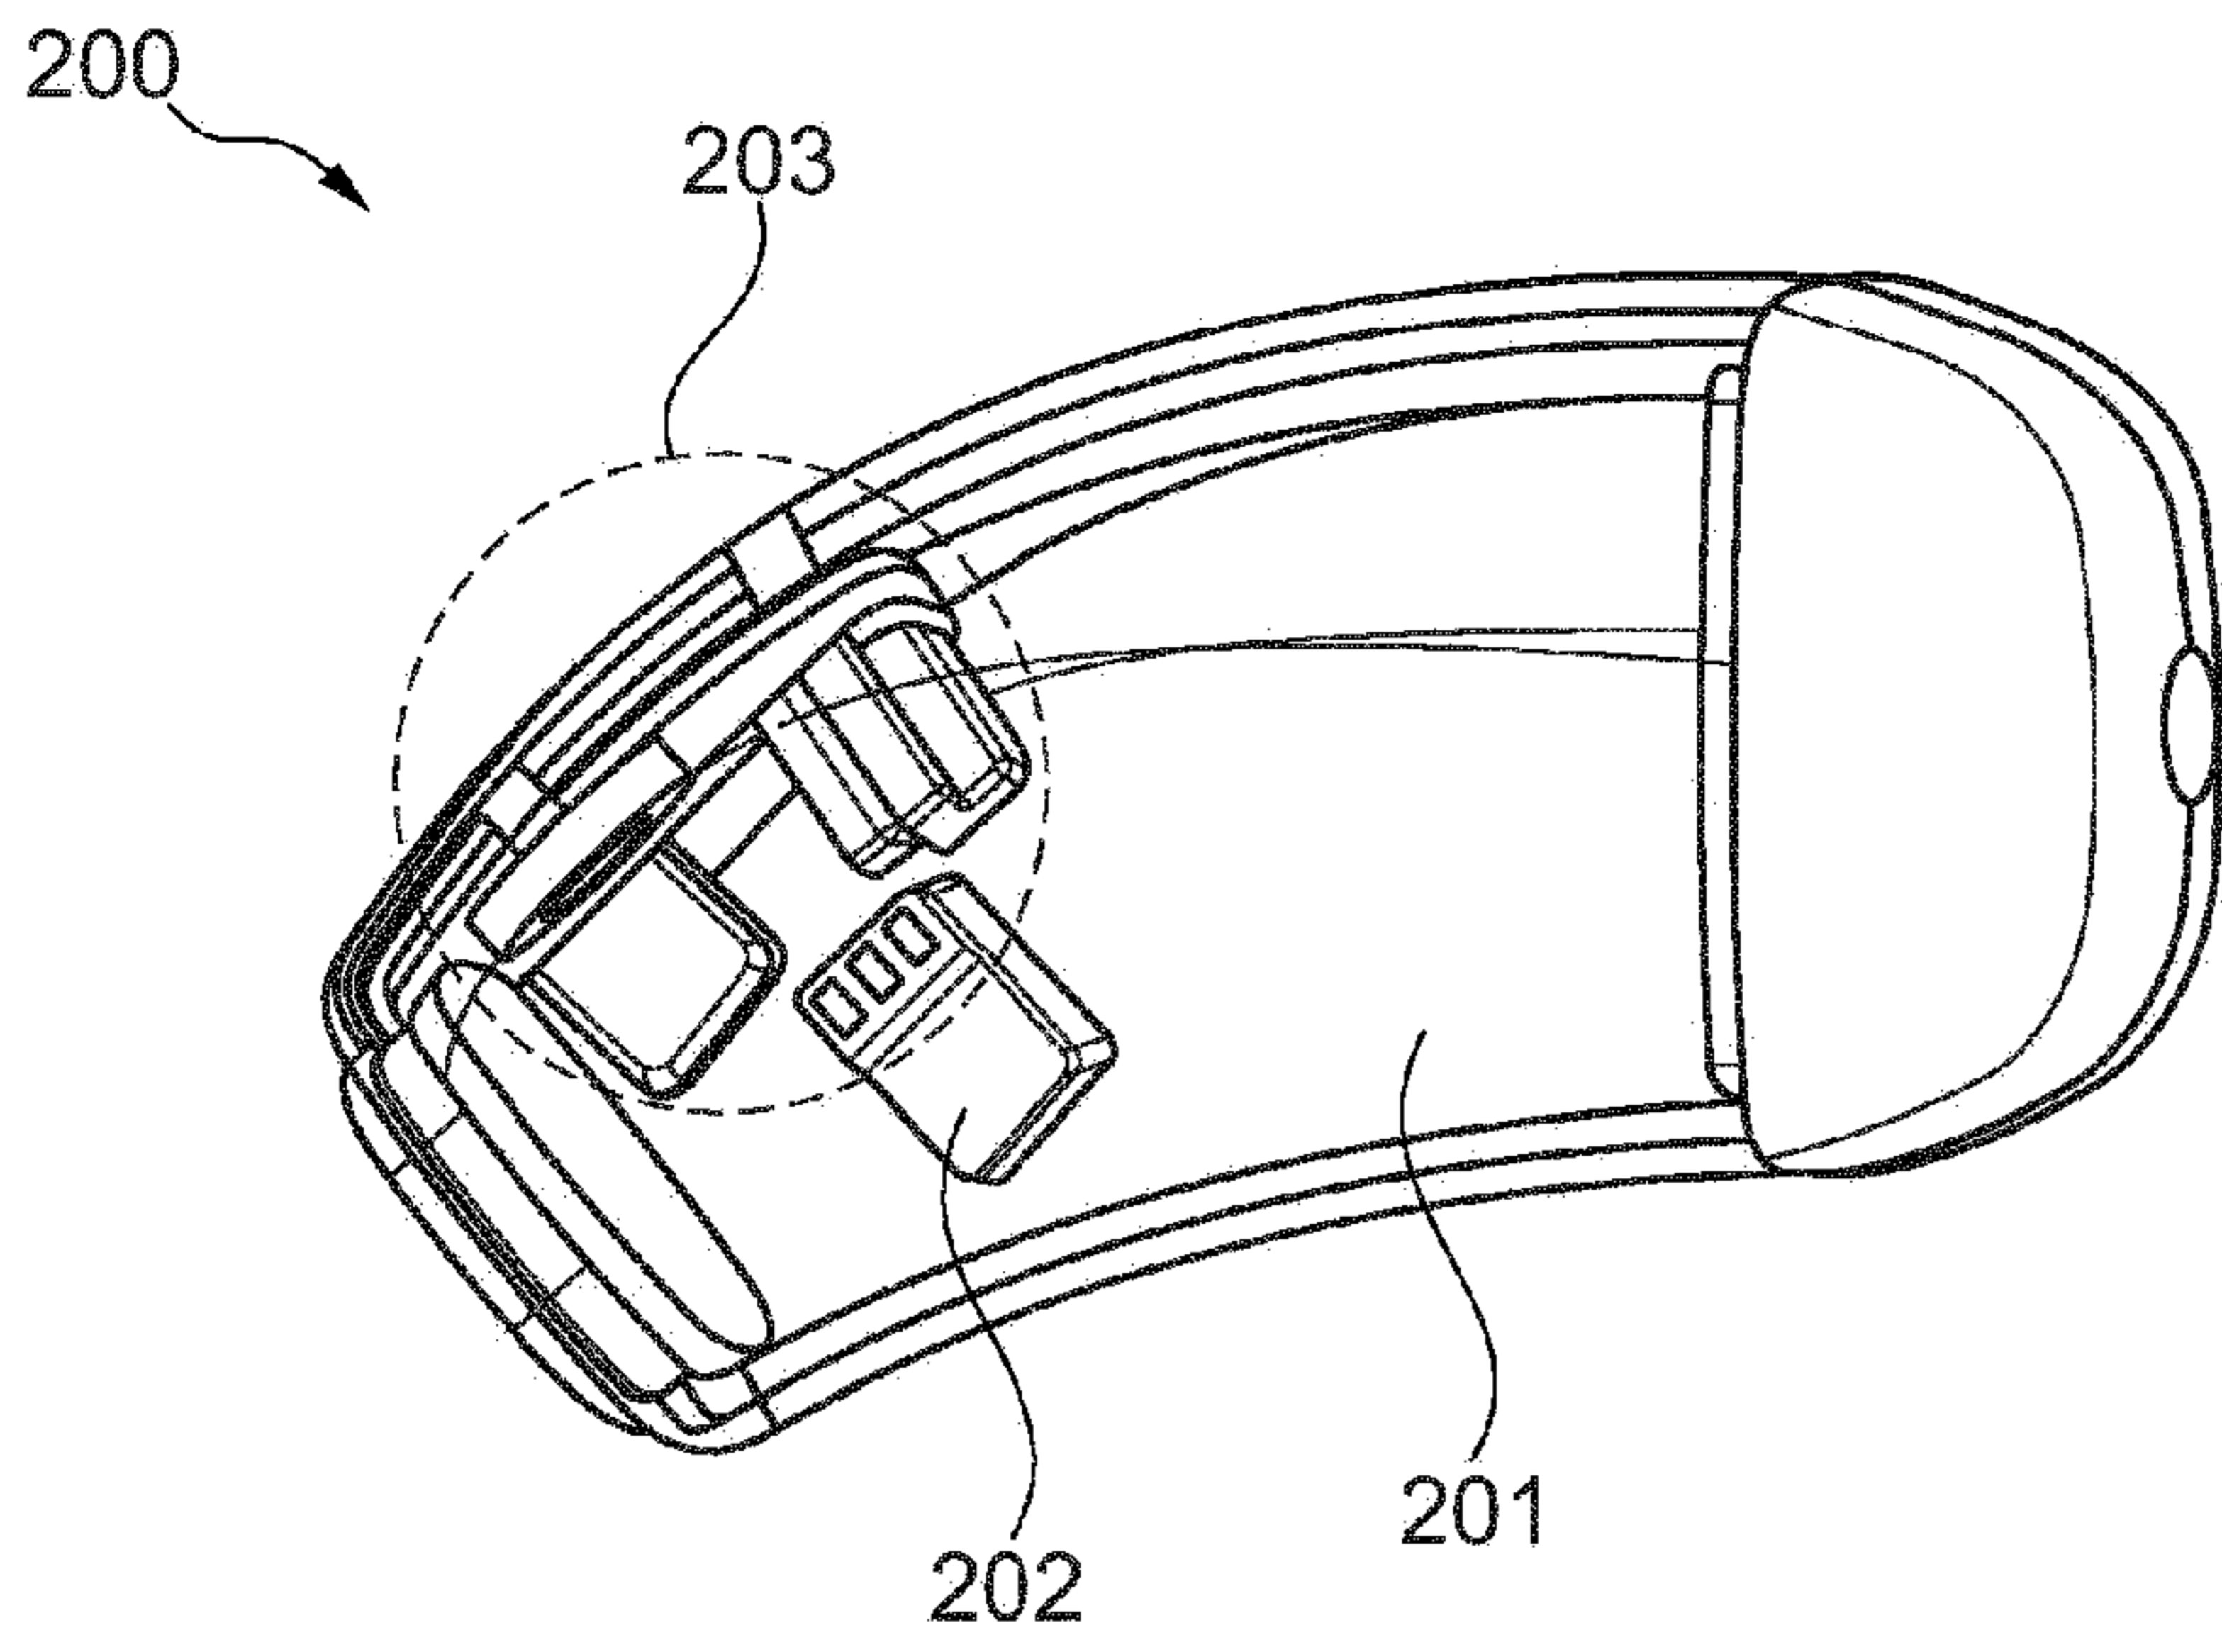


Fig. 2

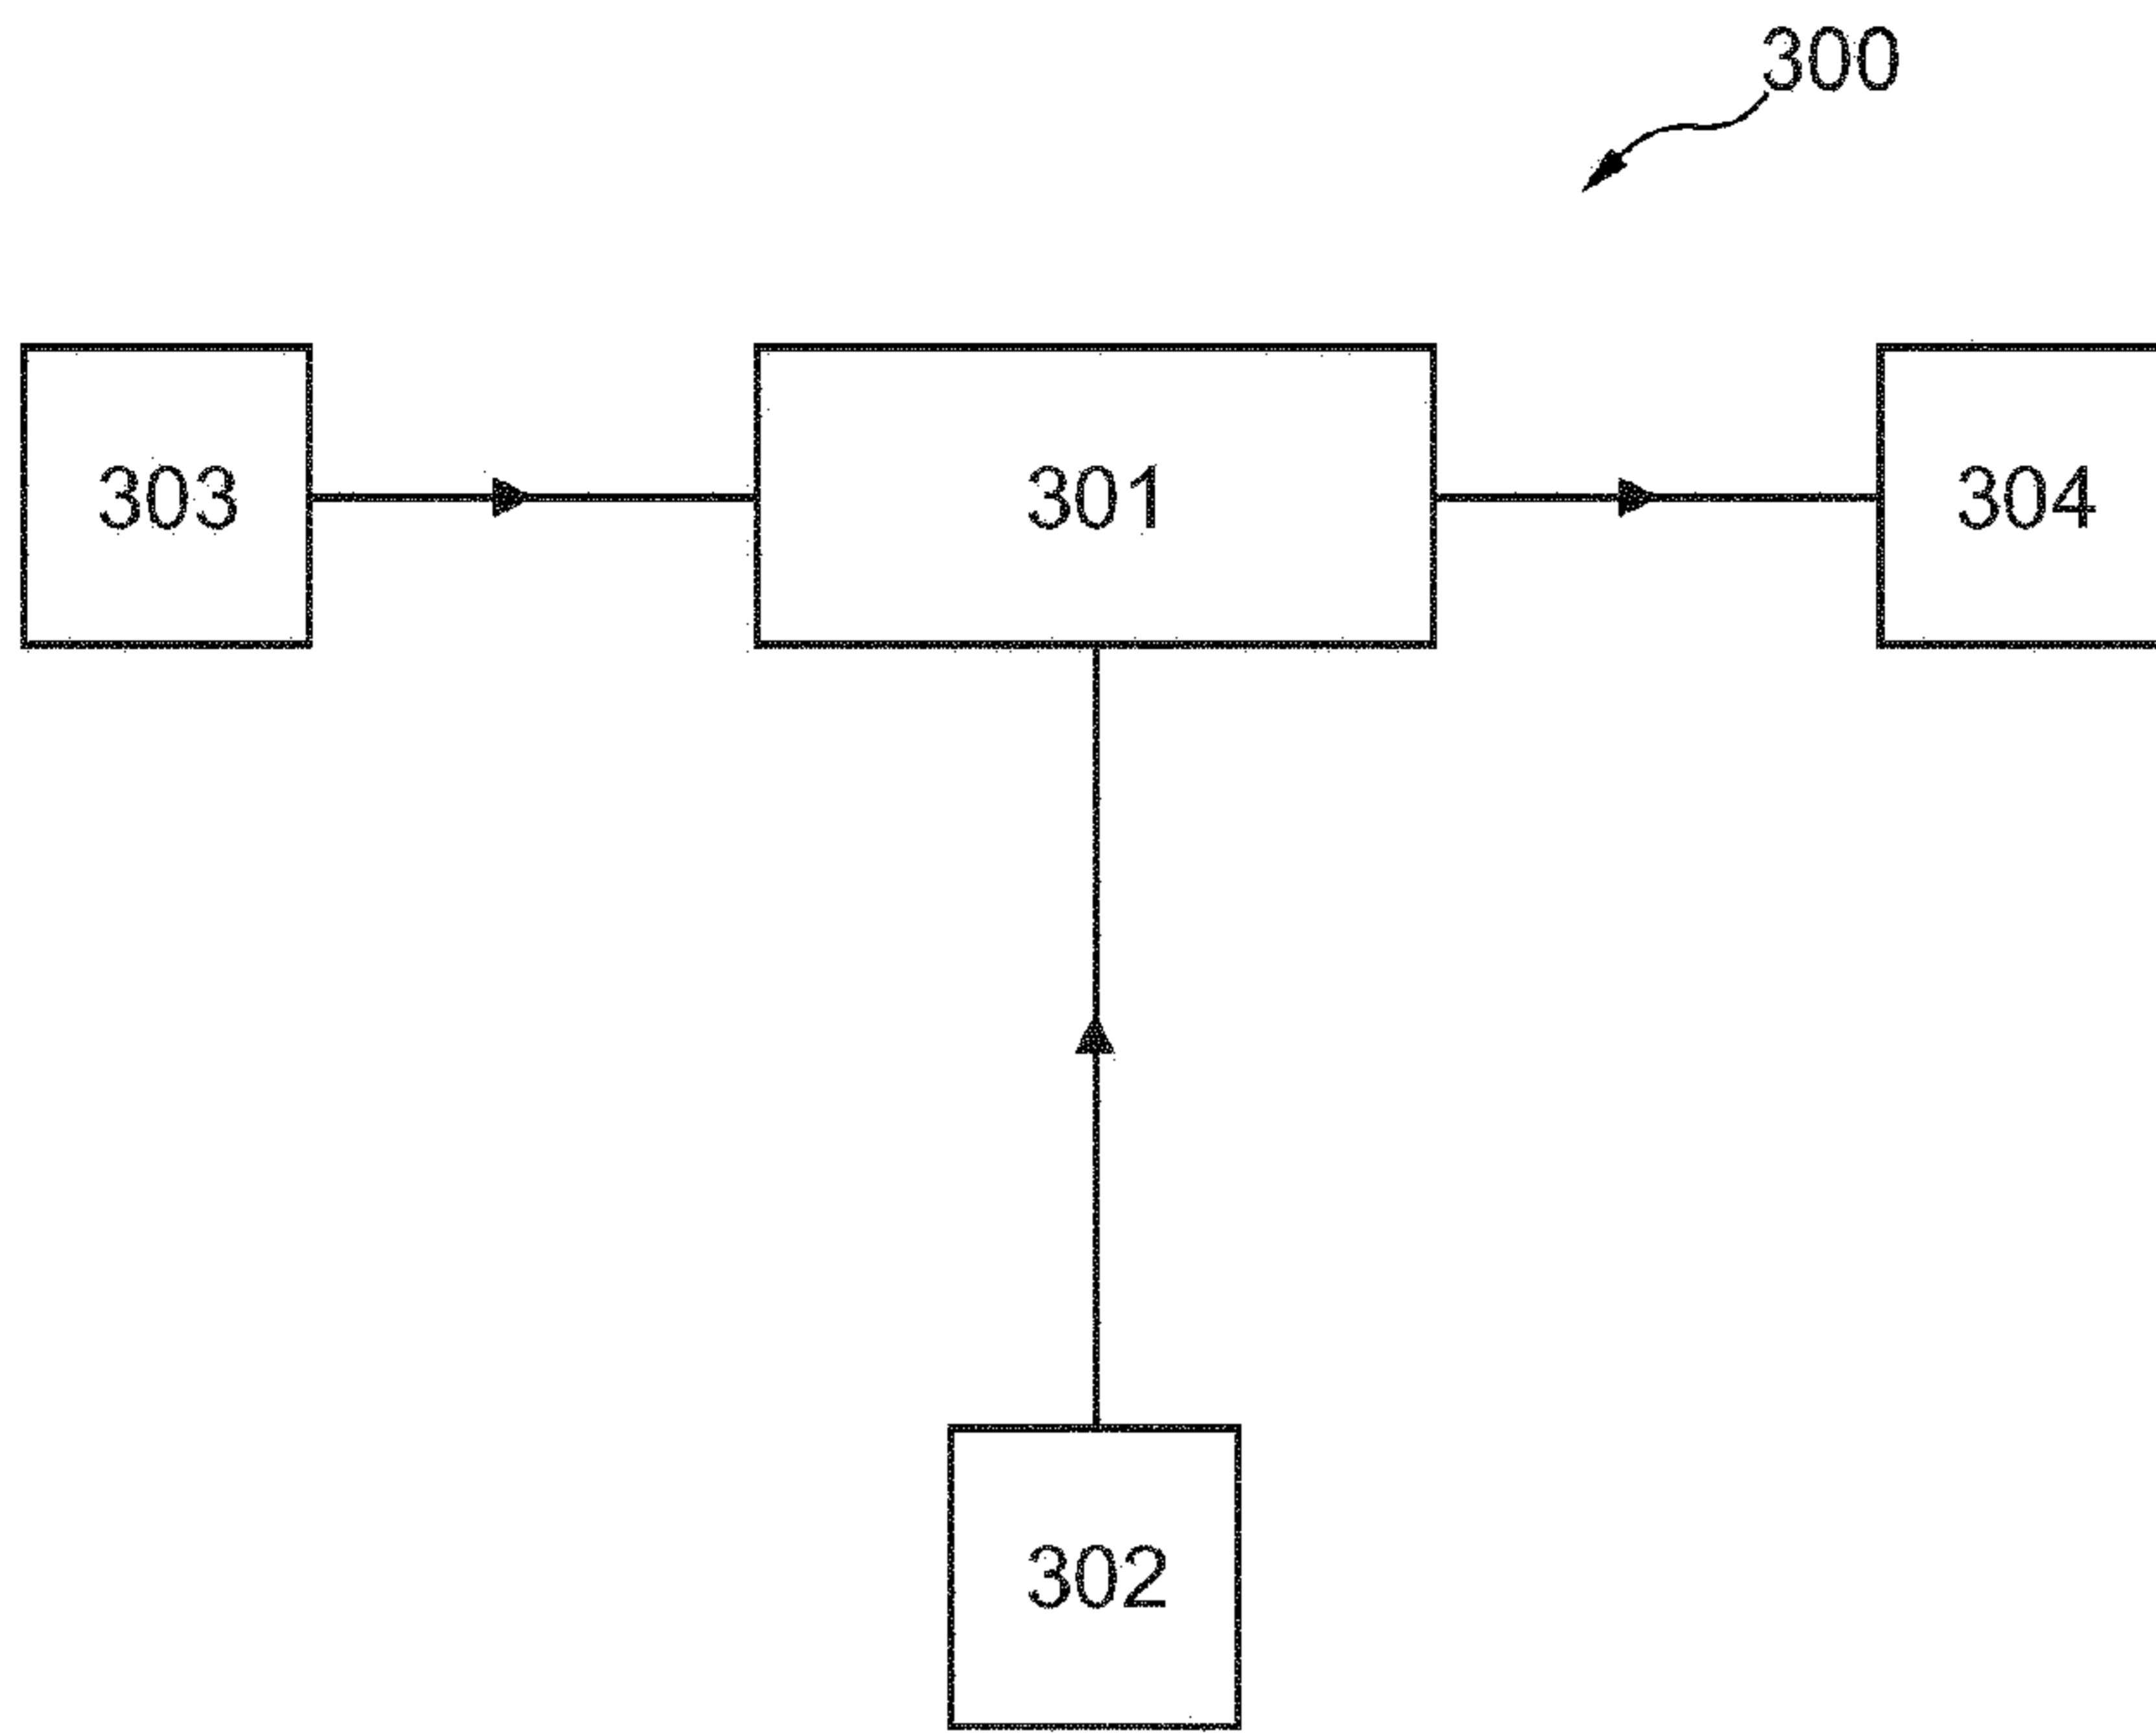


Fig. 3