

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
22 December 2005 (22.12.2005)

PCT

(10) International Publication Number
WO 2005/120332 A1

(51) International Patent Classification⁷: **A61B 5/00**

(21) International Application Number:
PCT/CH2004/000345

(22) International Filing Date: 7 June 2004 (07.06.2004)

(25) Filing Language: English

(26) Publication Language: English

(71) Applicant (for all designated States except US): **PEN-DRAGON MEDICAL LTD.** [CH/CH]; Hagenholzstrasse 81 a, CH-8050 Zürich (CH).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **CADUFF, Andreas** [CH/CH]; Klingenstrasse 21, CH-8005 Zürich (CH). **TRUFFER, Pascal** [CH/CH]; Giblenstrasse 55, CH-8049 Zürich (CH). **RYABOV, Yaroslav** [RU/RU]; Gavrilova str. 22/22, Kazan, 420133 (RU). **FELDMAN, Yuri** [IL/IL]; Moshe Kol str. 57/14, 93715 Jerusalem (IL). **PUZENKO, Alexander** [IL/IL]; Abbu Ahimeiz str. 13/17, 97350 Jerusalem (IL).

(74) Agent: **E. BLUM & CO.**; Vorderberg 11, CH-8044 Zürich (CH).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.


(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: A METHOD AND DEVICE FOR DETERMINING A PARAMETER OF LIVING TISSUE

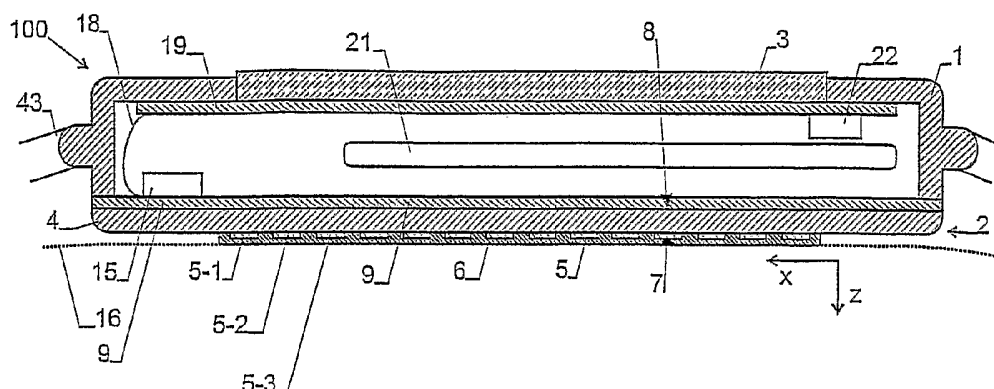

(57) Abstract: A device for measuring a glucose level or some other parameter of living tissue that affects the dielectric properties of the tissue is disclosed. The device comprises an electrode arrangement (5) having a plurality of electrodes (5-i). The signal from a signal source (31) can be applied to the electrode arrangement via a switching assembly (39). The switching assembly (39) is designed to selectively connect a first and a second pattern of the electrodes (5-i) to the signal source, thereby generating a first and a second electrical field with different spatial distribution in the tissue. By using a differential method which relies on measuring the impedance of the electrode arrangement (5) for each field and on suitable subtraction of the measured results, surface effects can be reduced and the focus of the measurement can be offset to a point deeper inside the tissue.

A method and device for determining a parameter of living tissue

5

Technical Field

The invention relates to a method and a device for determining dielectric properties of living tissue, in particular but not exclusively for the purpose of measuring the glucose level in the tissue.

15

Background Art

WO 02/069791 describes a device for measuring blood glucose in living tissue. It comprises an electrode arrangement with a ground electrode and a signal electrode. A signal source applies an electrical AC-signal of known voltage or current through a resistor to the electrodes, and a detector determines the voltage over the electrodes. This depends on the dielectric properties of the tissue, which, as it has been found, are indicative of the glucose level within the tissue.

25

Devices of this type have been found to deliver good results, but they require a substantial effort for calibration and are prone to drift, in particular when the environmental conditions change or when they are being displaced. Differential methods have been used to improve measurement accuracy in other fields of technology. Differential methods are generally based on two or more measurements, wherein one or more measurement conditions are changed between measurements. Depending on the specific application, the influence of some parameters can be eliminated or reduced by calculating the difference between the measurements.

35

Disclosure of the Invention

Hence, it is a general object of the invention to provide a method and a device of the type mentioned above that has improved accuracy.

This object is achieved by the method and device according to the independent claims.

Hence, the device according to the invention comprises an electrode arrangement, a signal source and a detector. The signal source feeds an electrical signal to the electrode arrangement. The device is adapted to generate at least two spatially different electrical fields in the tissue. The detector measures the difference of the responses of the tissue to the electrical fields. This difference depends on the spatial difference between the electrical fields, i.e. it primarily depends on the dielectric properties of those regions within the tissue where the difference between the at least two spatially different fields is strongest.

Hence, by suitably selecting the spatial distribution of the fields, it becomes possible to primarily measure the properties of regions of the tissue that cannot be selectively measured by using a single field only.

In particular, the spatially different fields can be generated with an electrode arrangement having at least three, advantageously even more, electrodes, and by first applying a first voltage pattern to the electrodes and by then applying a second voltage pattern to the electrodes, wherein said first and said second voltage patterns are different. This can e.g. be achieved by arranging a switching assembly between the signal source and the electrodes, which selectively connects at least a first and a second pattern of the electrodes to the signal source.

In an advantageous embodiment, two values s_1 and s_2 are measured, s_1 being indicative of the response

of the tissue to a first electrical field and s_2 being indicative of the response of the tissue to a second electrical field. The parameter is calculated from a weighted difference $D = k_1 \cdot s_1 - k_2 \cdot s_2$ with weights k_1 and k_2 . The weights k_1 and k_2 or the ratio $k_1:k_2$ can be calculated in a calibration procedure under the condition that the weighted difference depends only weakly on the response of the tissue near the surface of the body (i.e. in the epidermis), but primarily on the response of the tissue in a region farther away from the electrodes, i.e. deeper inside the body, such as the dermis. In other words, k_1 and k_2 are chosen such that the contribution of the tissue close to the electrode arrangement (i.e. of the contribution of the epidermis) to the weighted difference D is minimized; in this context, "minimized" is understood to imply that the contribution to D is considerably smaller than for the individual measured values s_1 , s_2 , but not necessarily zero or at an absolute minimum. This allows to minimize undesired effects (such as temperature and surface conditions) affecting the properties of the body surface. The values s_1 and s_2 may be real or complex quantities. If s_1 and s_2 are complex, k_1 and k_2 will generally be complex as well.

The device according to the invention is especially suited for measuring a glucose level of the tissue, but it can also be used for measuring any other parameter that affects the dielectric properties of the tissue, such as an electrolyte level.

30

Brief Description of the Drawings

The invention will be better understood and objects other than those set forth above will become apparent when consideration is given to the following detailed description thereof. Such description makes reference to the annexed drawings, wherein:

35

Fig. 1 is a cross section of a device for measuring a glucose level,

Fig. 2 is a block circuit diagram of the device of Fig. 1,

5 Fig. 3 is a detailed view of the electrode arrangement and the switching assembly, and

Fig. 4 shows normalized, average absolute fields as a function of depth.

10

Modes for Carrying Out the Invention

Fig. 1 shows a cross section of a device 100 for measuring a patient's glucose level or some other parameter in a patient's body, such as an electrolyte level of the tissue. It comprises a housing 1 closed on one side by an electrode plate 2. A display 3 is arranged opposite electrode plate 2. Electronic circuitry is arranged between electrode plate 2 and display 3.

20 Electrode plate 2 comprises an electrically insulating substrate 4. An electrode arrangement 5 comprising a plurality of parallel strip electrodes 5-0, 5-1, 5-2, etc. and being covered by an insulating layer 6 is arranged on an outer side 7 of insulating substrate 4. 25 An inner side 8 of insulating substrate 4 may be covered by a ground electrode 9. Suitable through-contacts (not shown) connect the strip electrodes 5-i to contact pads arranged on inner side 8.

A first temperature sensor 15 is mounted to ground electrode 9 in direct thermal contact thereto and 30 measures a first temperature T1.

Leads or springs 18 are provided to connect ground electrode 9, the contact pads and first temperature sensor 15 to the electronic circuitry arranged on a printed circuit board 19 forming an assembly of electronic components. A battery 21 for powering the circuitry is arranged between printed circuit board 19 and 35

electrode plate 2. A second temperature sensor 22 can be arranged on printed circuit board 19 and in direct thermal contact thereto for measuring a second temperature T_2 .

5 Fig. 2 shows a block circuit diagram of the circuitry of device 100. It comprises a voltage controlled oscillator (VCO) 31 as a signal source for generating a sine wave signal or another periodic signal. Instead of an oscillator, a pulse generator could be used
10 for generating substantially non-periodic signals, such as short pulses or step-like voltage transitions. The signal from the signal source is fed to two amplifiers 32, 33. The output of first amplifier 32 is connected via a resistor R1 to a first signal path 34. A resonant circuit 35 comprising an inductance L and the capacitive
15 load of the electrode arrangement 5 in series is connected between first signal path 34 and ground. A switching assembly 39 is used to selectively connect the strip electrodes 5-i to either inductance L or ground as described below, thereby defining at least two different
20 electrode patterns.

The output of second amplifier 33 is connected via a resistor R2 to a second signal path 36. Second signal path 36 can be substantially identical to
25 first signal path 34 but comprises a resistor R3 as a reference load instead of resonant circuit 35.

Both signal paths 34, 36 are fed to a measuring circuit 37, which determines the relative amplitude A of both signals and/or their mutual phase shift ϕ .
30 Relative amplitude A can e.g. be the amplitude of first signal path 34 in units of the amplitude of second signal path 36 (wherein the amplitudes are the peak values of the sine waves or, if pulses or voltage steps are used as measuring signal, the corresponding peak amplitude or
35 step voltage).

The output signal of measuring circuit 37 is fed to a microprocessor 38, which also controls the operation of VCO 31.

Microprocessor 38 further samples the first and second temperature signals T1, T2 from first and second temperature sensors 15, 22. It also controls display device 3, an input device 40 with user operable controls, and an interface 41 to an external computer. A memory 42 is provided for storing calibration parameters, measurement results, further data as well as firmware for microprocessor 38. At least part of memory 42 is non-volatile.

Inductance L of the device of Fig. 2 can be generated by a coil and/or by the leads and electrodes of electrode arrangement 5. Its value is generally known with reasonable accuracy.

Electrode arrangement 5 represents a primarily capacitive load C.

The electrodes of electrode arrangement 5 are arranged on the skin 16 of the patient as shown in Fig. 1. For a good and permanent contact with the patient's skin, the device is advantageously worn on an arm or leg and provided with a suitable holder or wrist band 43.

In summary, the device shown in Figs. 1 and 2 comprises:

- an electrode arrangement 5,
- a signal source (VCO 31) for applying an electrical signal to electrode arrangement 5 for generating an electrical field in the tissue,
- a detector for measuring a response from the tissue to the electrical field and for determining at least one parameter therefrom, the detector primarily comprising the elements 37, 38.

Fig. 3 shows switching assembly 39 and electrode arrangement 5 in detail. As shown, each strip electrode 5-i of electrode arrangement 5 is connected to an electronic switch Si for selectively connecting it either

to ground or to inductance L. A switch control unit 45 is provided for individually controlling the position of each the switches S_i . Switch control unit 45 is controlled by microprocessor 38.

5 In the present embodiment, switch control unit 45 has two modes of operation.

 In the first mode of operation (as it is shown by the switch positions of Fig. 3), switch control unit 45 sets switches S_0 , S_2 , S_4 and S_6 to connect electrodes 5-0, 5-2, 5-4 and 5-6 to inductance L and thereby to the signal from VCO 31, while switches S_1 , S_3 , S_5 , S_7 are set to connect electrodes 5-1, 5-3, 5-5 and 5-7 to ground. In this first mode of operation, the voltage pattern applied to the electrodes is therefore such that
10 each pair of neighboring electrodes carry different voltages.
15

 In the second mode of operation, switches S_0 , S_1 , S_4 and S_5 are set to connect electrodes 5-0, 5-1, 5-4 and 5-5 to inductance L and thereby to the signal from VCO 31 while switches S_2 , S_3 , S_6 and S_7 are set to connect electrodes 5-2, 5-3, 5-6 and 5-7 to ground. In this mode of operation, the voltage pattern at the electrodes of a first part of the pairs of neighboring electrodes carry equal voltages and the electrodes of a second part of the pairs of neighboring electrodes carry different
20 voltages. As will be easily understood, the electric fields generated in the two modes of operation will have different spatial distribution, as illustrated by curves e1, e2 of Fig. 4. Any measured parameter s describing the
25 response of the tissue to the applied field will depend on how the field is distributed and will have different values s_1 and s_2 in the two modes of operation.
30

 In the present context, it is of particular interest how the measured parameter s depends on the dielectric properties of the epidermis close to the surface
35 and how it depends on the dielectric properties of the dermis deeper in the tissue.

In the following, we assume that the measured parameter s is the capacitance C_i of electrode arrangement 5 for a given mode of operation i . In linear approximation, we can write

5

$$C_i(\varepsilon_{ep}, \varepsilon_{dr}) \approx C_i(\varepsilon_{ep}^0, \varepsilon_{dr}^0) + (\varepsilon_{ep}^0 - \varepsilon_{ep}) \left. \frac{\partial C_i}{\partial \varepsilon_{ep}} \right|_{\varepsilon_{ep}^0} + (\varepsilon_{dr}^0 - \varepsilon_{dr}) \left. \frac{\partial C_i}{\partial \varepsilon_{dr}} \right|_{\varepsilon_{dr}^0}, \quad (1)$$

where subscript "ep" denotes contributions from the epidermis and "dr" contributions from the dermis. Superscript "0" denotes "normal" (unperturbed) values, e.g. at the time of a calibration measurement or for a typical subject. ε is the dielectric constant of the tissue in the dermis or epidermis, respectively. The derivatives of C in view of ε can e.g. be calculated from a dielectric model of typical tissue. A similar dependence will be observed for other measured values, such as the inverse resistance $1/R$ between the electrodes versus conductivities of dermis and epidermis or the complex impedance Z as function of both dielectric constants and conductivities in dermis and epidermis. Again, the measured value will depend on the mode of operation, i.e. on the voltage pattern applied to the electrodes.

In operation, device 100 can e.g. be used to measure the capacitance C , resistance R or complex impedance Z of electrode arrangement 5 at one or more frequencies f . This impedance Z depends on the dielectric response of the tissue to the applied electric field and, as it has been found, it is indicative of the glucose concentration in the tissue.

As it is known to the person skilled in the art, capacitance C , resistance R or impedance Z can e.g. be measured by determining the relative amplitude A and phase shift ϕ provided by measuring circuit 37.

Advantageously, microprocessor 38 computes two values s_1 and s_2 indicative of the dielectric response of the tissue to the first and the second electric

field. If the capacitance C_1 and C_2 in the first and the second mode of operation are measured, we have $s_1 = C_1$ and $s_2 = C_2$.

Subsequently, the difference of the responses to the two electric fields is determined, advantageously by calculating the weighted difference

$$D^C = k_1 \cdot C_1 - k_2 \cdot C_2, \quad (2)$$

where the subscript C denotes that we are talking about constants k_1 , k_2 for the measurement of capacitance (a similar equation with different constants can be derived for the measurement of the conductance, i.e. $s = 1/R$), where the weights k_1 and k_2 are chosen such that the non-constant contributions of the dielectric properties of the epidermis to the difference D are substantially 0.

Combining Equations (1) and (2), we obtain

$$D^C \approx \left[k_1^C C_1(\varepsilon_{ep}^0, \varepsilon_{dr}^0) - k_2^C C_2(\varepsilon_{ep}^0, \varepsilon_{dr}^0) \right] + (\varepsilon_{ep}^0 - \varepsilon_{ep}) \left[k_1^C \frac{\partial C_1}{\partial \varepsilon_{ep}} \bigg|_{\varepsilon_{ep}^0} - k_2^C \frac{\partial C_2}{\partial \varepsilon_{ep}} \bigg|_{\varepsilon_{ep}^0} \right] + (\varepsilon_{dr}^0 - \varepsilon_{dr}) \left[k_1^C \frac{\partial C_1}{\partial \varepsilon_{dr}} \bigg|_{\varepsilon_{dr}^0} - k_2^C \frac{\partial C_2}{\partial \varepsilon_{dr}} \bigg|_{\varepsilon_{dr}^0} \right] \quad (3)$$

In order to minimize the non-constant epidermis contributions, the value of the second square bracket in Eq. (3) should be 0. This can e.g. be achieved by arbitrarily setting k_1^C to 1 and using $k_2^C = (\partial C_1 / \partial \varepsilon_{ep}) / (\partial C_2 / \partial \varepsilon_{ep})$.

Instead of arbitrarily setting k_1^C to 1, the constants can be chosen such that the contribution from the "normal" values in the first square bracket of Eq. (3) becomes 0 as well, thus making the difference D dependent on the dermis contributions only. In that case, setting the first and the second square bracket in Eq. (3) to 0 will yield a system of two equations that allows to determine the values of k_1^C and k_2^C . After measuring the difference D as well as the temperatures T_1 and T_2 , microprocessor 38 can e.g. use a formula of type

$$g = F(D, T_1, T_2, a_0, \dots a_M) \quad (4)$$

for determining the glucose level g (or a parameter indicative thereof) from the measured input values D , T_1 and T_2 , where the function F has $M+1$ parameters $a_0, \dots a_M$ ($M \geq 0$).

The function F can be empirical or it can be based at least partially on a model describing the physiological nature of the mechanisms involved.

Assuming that the relation between the glucose level g and the measured values s_i is linear at least in approximation, we can use

$$g = a_0 + a_1 \cdot D + a_2 \cdot T_1 + a_3 \cdot T_2 \quad (5)$$

with $M = 3$.

In order to determine the parameters $a_0, a_1, \dots a_M$, a series of at least $M+1$ calibration measurements has to be carried out, each calibration measurement comprising a determination of the input values D , T_1 and T_2 and a reference glucose level g measured by conventional means, e.g. by an invasive method.

In a most simple approach, the parameters a_i can then be obtained from a conventional least-squares fitting algorithm that varies the parameters a_i in order to find a best match of equations (4) or (5) to the calibration measurements. Suitable algorithms are known to a person skilled in the art and are e.g. described by Press, Teukolsky, Vetterling and Flannery in "Numerical Recipes in C", Cambridge University Press, 2nd edition, 1992, Chapter 15.

Once the parameters a_i are known, the glucose level g can be determined from equations (4) or (5) based on the measurement of the input values D , T_1 and T_2 .

Re-calibration of at least part of the parameters may be advisable at regular intervals or after a displacement of device 100 in respect to the specimen.

In the above example, the electrode arrangement comprises a plurality of strip-shaped electrodes arranged side by side. The number of electrodes may vary, even though a number of at least three electrodes is required in order to support at least two spatially different electrode patterns. At least four, in particular at least eight electrodes is advantageous in order to keep fringe field effects small.

The voltage pattern to be applied to the electrodes in the different modes of operation can vary as well. In the example above, the following scheme was used: In the first mode of operation, the voltage v_i at the electrode i was

$$\begin{aligned} v_i &= v_0 && \text{if } i \text{ is even} \\ &= 0 && \text{otherwise,} \end{aligned} \quad (6)$$

(where v_0 denotes the voltage at the output of inductance L) while in the second mode of operation the voltage at electrode i was

$$\begin{aligned} v_i &= v_0 && \text{if } \text{floor}(i/2) \text{ is even} \\ &= 0 && \text{otherwise,} \end{aligned} \quad (7)$$

where $\text{floor}(x)$ is equal to x if x is an integer value or the next lower integer value otherwise.

It must be noted, though, that other patterns can be used as well. For example, instead of two, three or more neighboring electrodes can be applied to the same voltage in the second mode of operation. It may also be advisable to make sure that the outermost electrodes are always connected to ground in order to have well defined boundary conditions.

Other voltage patterns can be used as well. In order to emphasize the difference of the fields far from the electrodes, i.e. the difference of the contributions from the dermis, it is also possible to use more than two possible voltage levels. For example, in the second mode of operation, the voltage at electrode v_i can be chosen to be

$$v_i = v_0 \cdot \sin(i \cdot \pi / k), \quad (8)$$

10

with $k \geq 2$. For example, for $k = 2$, the voltage at electrode 0 is 0, at electrode 1 it is v_0 , at electrode 2 it is 0, at electrode 3 it is $-v_0$, etc., which leads to an increase of the field at some distance from the electrodes as compared to the field close to the electrodes.

15

In general, any electrode arrangement can be used that is able to generate at least two spatially different alternating fields in the adjacent tissue. "Spatially different" is used to describe fields that have different shape. Fields that merely differ by a multiplicative factor are not understood to be "spatially different".

20

While there are shown and described presently preferred embodiments of the invention, it is to be distinctly understood that the invention is not limited thereto but may be otherwise variously embodied and practiced within the scope of the following claims.

25

Claims

1. A device for measuring a parameter of living tissue, in particular a glucose level, which parameter affects a response of said tissue to an electric field, comprising
- an electrode arrangement (5),
- a signal source (31) generating an electrical signal to be applied to said electrode arrangement (5)
- for generating an electrical field in said tissue, and
- a detector (37, 38) for measuring a response from said tissue to said electrical field and for determining at least one parameter therefrom,
- wherein said device is adapted to generate at least two spatially different electrical fields (E_1 , E_2) in said tissue, and wherein said detector is adapted to determine said parameter from a difference of the responses of said tissue to said spatially different electrical fields.
2. The device of claim 1 wherein said electrode arrangement (5) comprises at least three electrodes (5-i), wherein said device is adapted to generate said at least two spatially different electrical fields (E_1 , E_2) by first applying a first voltage pattern to said electrodes (5-i) and by then applying a second voltage pattern to said electrodes (5-i), wherein said first and said second voltage patterns are different.
3. The device of claim 2 further comprising a switching assembly (39) arranged between said signal source (31) and said electrodes (5-i) for selectively connecting at least a first and a second pattern of said electrodes (5-i) to said signal source (31).
4. The device of any of the preceding claims wherein said electrode arrangement (5) comprises a plurality of electrodes (5-i) arranged side by side.
5. The device of claim 4 wherein said electrode arrangement (5) comprises at least four, in par-

ticular at least eight, electrodes (5-i) arranged side by side.

6. The device of any of the claims 4 or 5, wherein said device is adapted to selectively apply

5 in a first mode of operation, a first voltage pattern to said electrodes (5-i), wherein in said first voltage pattern the electrodes of each pair of neighboring electrodes carry different voltages, and

10 in a second mode of operation, a second voltage pattern to said electrodes (5-i), wherein in said second voltage pattern a the electrodes of a first part of the pairs of neighboring electrodes carry equal voltages and the electrodes of a second part of the pairs of neighboring electrodes carry different voltages.

15 7. The device of any of the preceding claims wherein detector (37, 38) is adapted

to measure a first measured value s_1 indicative of the response of said tissue to a first electrical field and a second measured value s_2 indicative of the response of said tissue to a second electrical field, wherein said first and said second electrical field are spatially different, and

20 to calculate a weighted difference $k_1 \cdot s_1 - k_2 \cdot s_2$ with weights k_1 and k_2 , wherein the weights are chosen such that a non-constant contribution of the dielectric response of an epidermis of the tissue to the weighted difference is minimized.

8. The device of any of the preceding claims wherein said electrode arrangement (5) comprises a plurality of electrodes (5-i) and wherein said detector (37, 38) is adapted for measuring values depending on a capacitance (C), and/or resistance (R) and/or impedance (Z) of at least two different combinations of the electrodes.

9. The device of any of the preceding claims wherein said parameter is a glucose level in the tissue.

35 10. A method for measuring a parameter of living tissue, in particular a glucose level, which pa-



parameter affects a response of said tissue to an electric field, comprising the steps of

applying an electrode arrangement (5) to said tissue,

5 applying a first electrical signal to said electrode arrangement (5) for generating a first electrical field in said tissue and detecting a first response of said tissue to said first electrical field,

10 applying a second electrical signal to said electrode arrangement (5) for generating a second electrical field in said tissue and detecting a second response of said tissue to said second electrical field, wherein said first and said second electrical fields are spatially different,

15 determining said parameter from a difference of the first and the second response of said tissue.

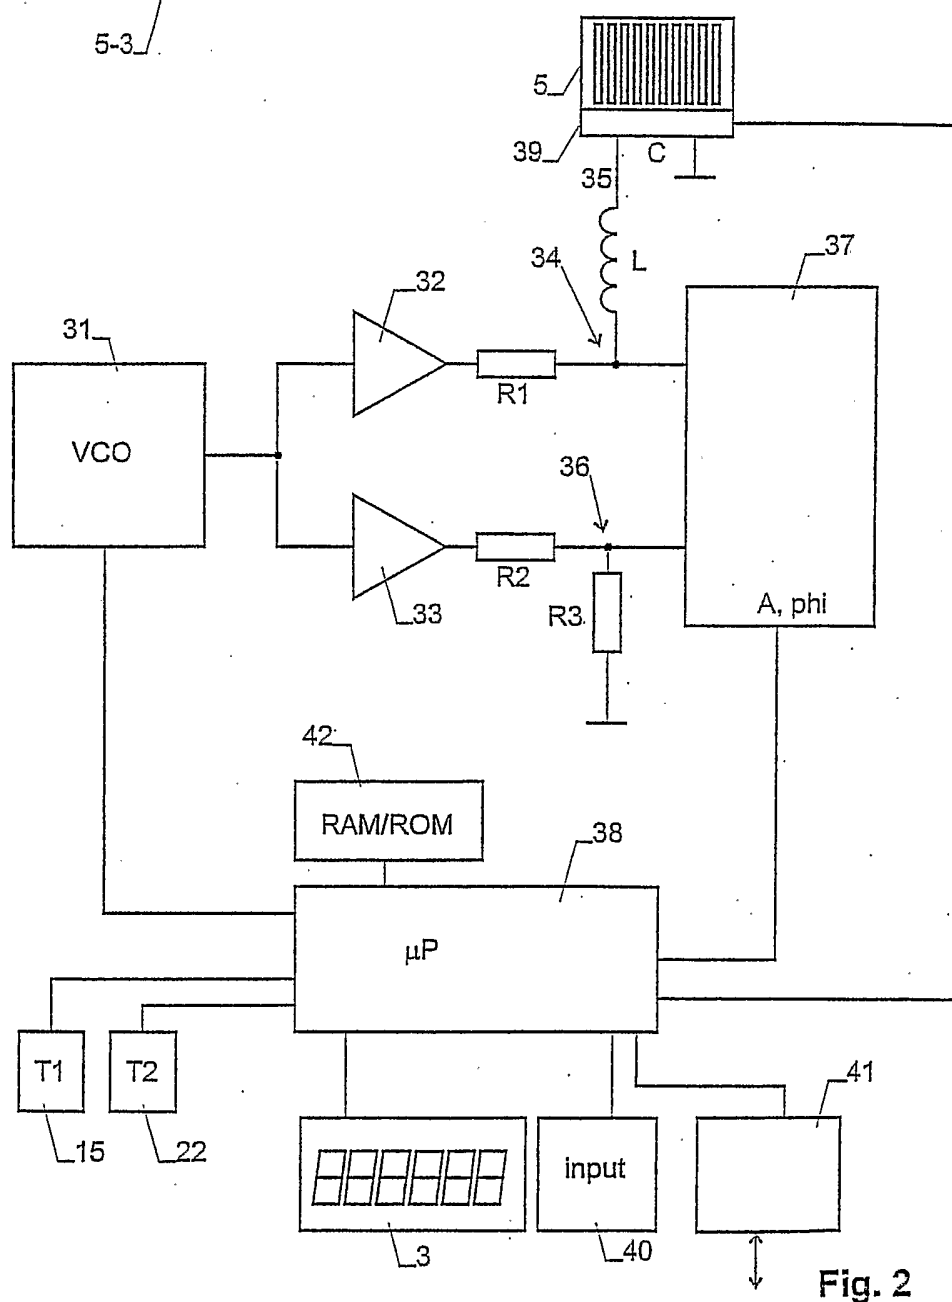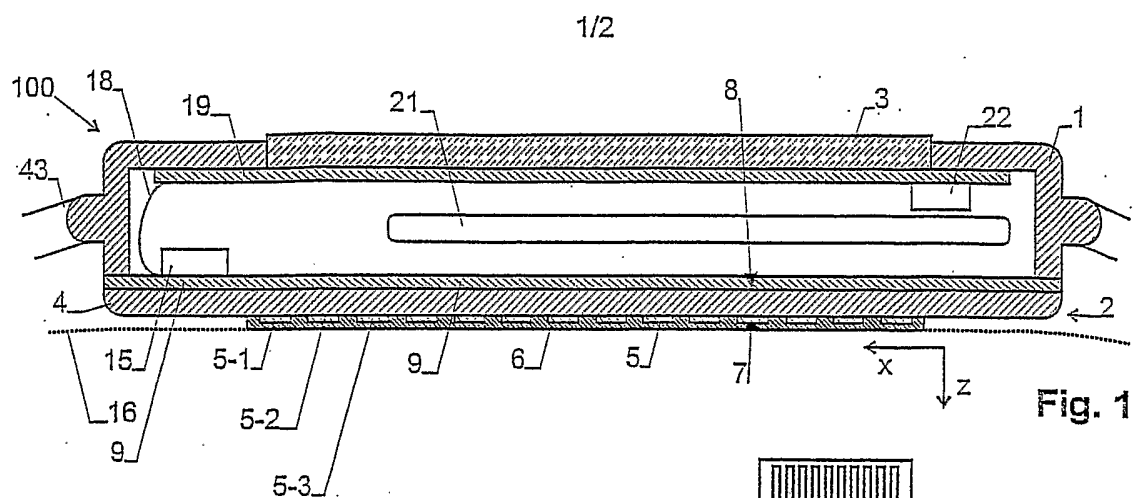

2/2

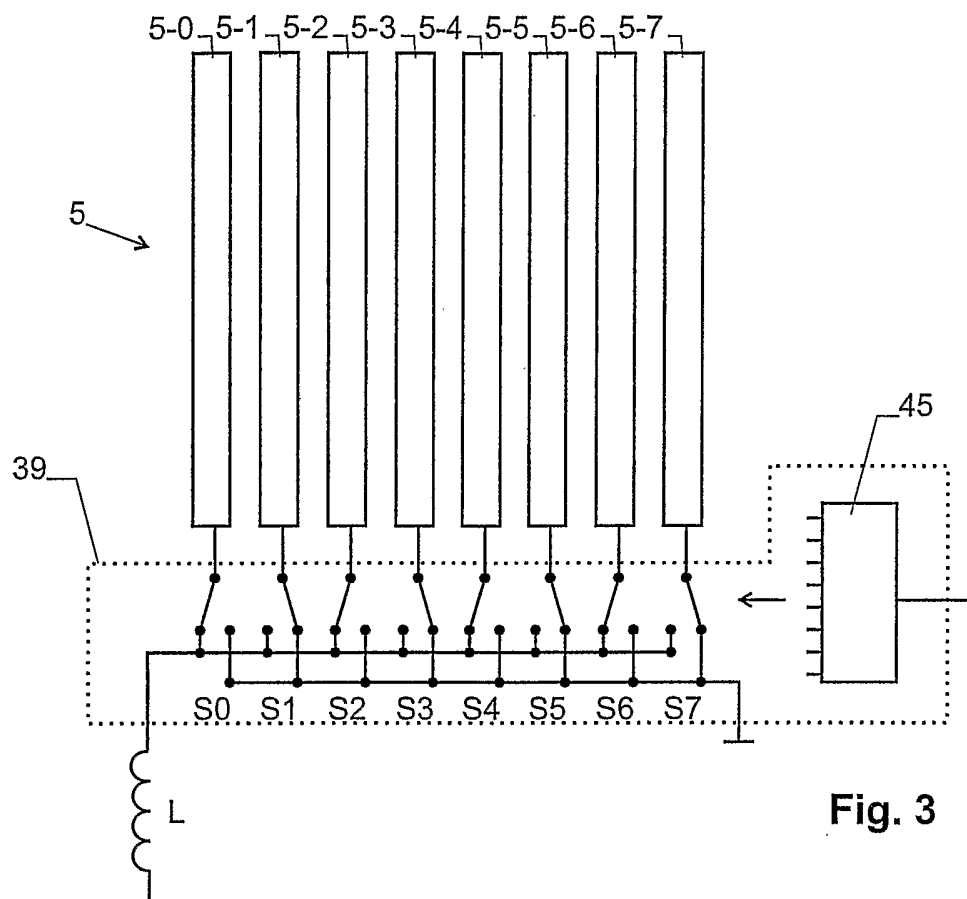


Fig. 3

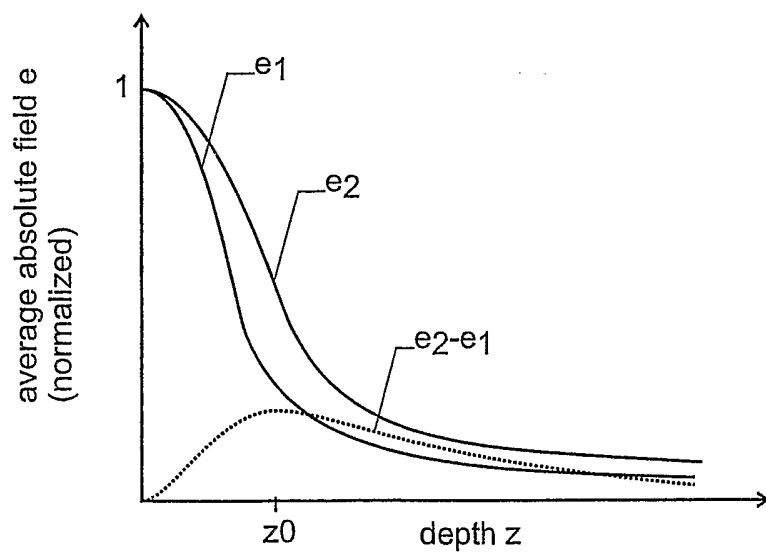


Fig. 4

INTERNATIONAL SEARCH REPORT

International Application No
PCT/CH2004/000345A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 02/069791 A (PENDRAGON MEDICAL LTD ; CADUFF ANDREAS (CH); HIRT ETIENNE (CH); SCHREP) 12 September 2002 (2002-09-12) cited in the application page 2, line 8 - page 5, line 26; claims; figure 1.3	1,7,9
Y	WO 99/39627 A (DERMAL THERAPY BARBADOS INC ; OLLMAR STIG (SE); WICKETT R RANDALL (US)) 12 August 1999 (1999-08-12) page 3, line 1 - page 5, line 22	1,7,9
A	US 5 353 802 A (OLLMAR STIG) 11 October 1994 (1994-10-11) the whole document	1-5,8

☐ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

° Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- * & * document member of the same patent family

Date of the actual completion of the international search

5 January 2005

Date of mailing of the international search report

12/01/2005

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Manschot, J

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CH2004/000345

Box II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 10
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Diagnostic method practised on the human or animal body
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/CH2004/000345

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 02069791	A	12-09-2002	WO 02069791 A1	12-09-2002
			CA 2439822 A1	12-09-2002
			CZ 20032650 A3	14-04-2004
			EP 1299029 A1	09-04-2003
			JP 2004526492 T	02-09-2004
			SK 12272003 A3	08-06-2004
			TW 524977 B	21-03-2003
			US 2004065158 A1	08-04-2004
WO 9939627	A	12-08-1999	WO 9939627 A1	12-08-1999
			AU 762922 B2	10-07-2003
			AU 6142198 A	23-08-1999
			CA 2318735 A1	12-08-1999
			EP 1052929 A1	22-11-2000
			JP 2002501802 T	22-01-2002
			US 6517482 B1	11-02-2003
US 5353802	A	11-10-1994	SE 466987 B	11-05-1992
			AT 167794 T	15-07-1998
			AU 659111 B2	11-05-1995
			AU 8849991 A	20-05-1992
			CA 2093922 A1	19-04-1992
			DE 69129698 D1	06-08-1998
			DE 69129698 T2	11-03-1999
			DK 553187 T3	28-06-1999
			EP 0553187 A1	04-08-1993
			ES 2120419 T3	01-11-1998
			FI 931730 A	16-04-1993
			HU 66173 A2	28-09-1994
			JP 3320413 B2	03-09-2002
			JP 6502323 T	17-03-1994
			KR 201178 B1	15-06-1999
			NO 931415 A	13-05-1993
			SE 9003336 A	19-04-1992
			WO 9206634 A1	30-04-1992