




(86) Date de dépôt PCT/PCT Filing Date: 2009/04/24
 (87) Date publication PCT/PCT Publication Date: 2010/01/14
 (85) Entrée phase nationale/National Entry: 2012/01/11
 (86) N° demande PCT/PCT Application No.: US 2009/041680
 (87) N° publication PCT/PCT Publication No.: 2010/005617
 (30) Priorité/Priority: 2008/07/11 (US61/080,171)

(51) Cl.Int./Int.Cl. *G01N 33/483* (2006.01),
C12Q 1/02 (2006.01), *G01N 35/08* (2006.01)
 (71) Demandeur/Applicant:
INTELLICYT CORPORATION, US
 (72) Inventeurs/Inventors:
TRINKLE, LINDA, US;
DUNLAY, R. TERRY, US;
SKLAR, LARRY, US;
EDWARDS, BRUCE, US
 (74) Agent: BERGSTEIN, COREY

(54) Titre : SYSTEME D'ANALYSE DE PARTICULES A ECHANTILLONS MULTIPLES ET PROCEDE DE CRIBLAGE A HAUT RENDEMENT

(54) Title: MULTI-SAMPLE PARTICLE ANALYZER SYSTEM AND METHOD FOR HIGH THROUGHPUT SCREENING

FIG. 1

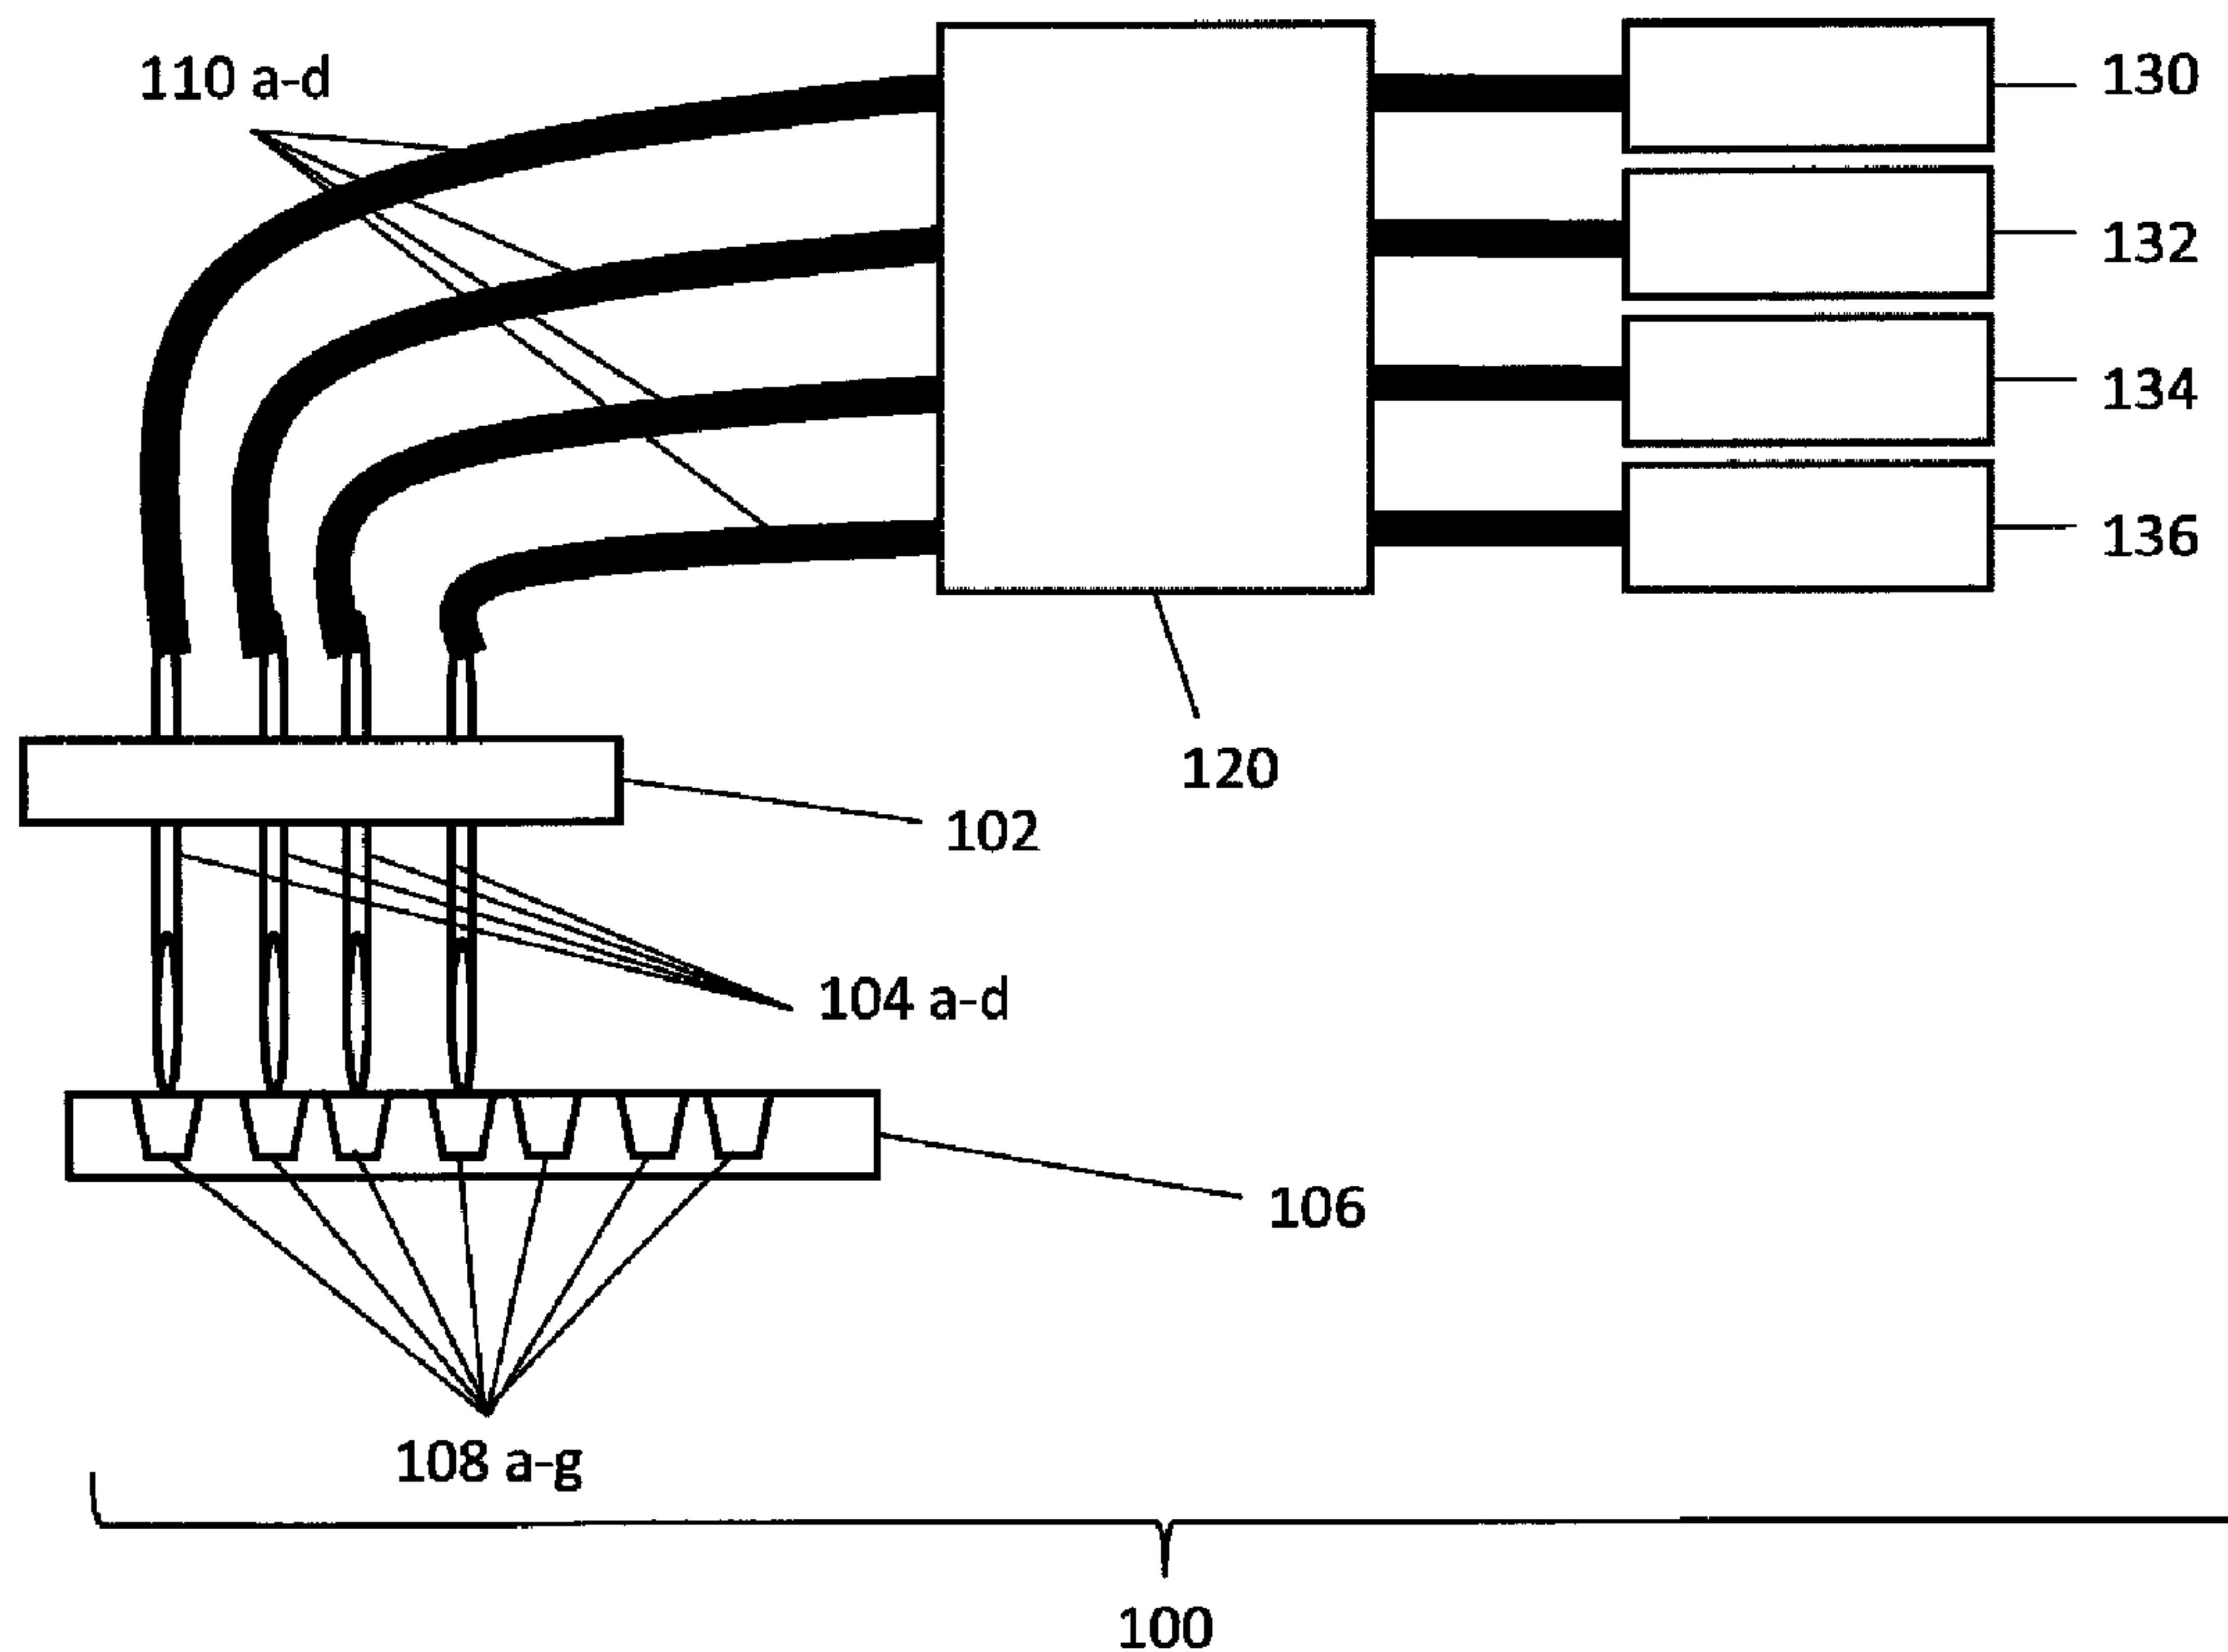

(57) **Abrégé/Abstract:**

Embodiments of the present invention provide a system and method for analyzing a plurality of samples comprising obtaining with an autoamplifier a plurality of samples from a first plate having a plurality of sample wells wherein the autosampler has a plurality of

(57) **Abrégé(suite)/Abstract(continued):**

probes for sampling a set of samples and wherein each probe of the plurality of probes is in communication with a separate flow cytometer via a separate conduit. The plurality of samples comprising particles is moved into a fluid flow stream for each separate conduit. Adjacent ones of the plurality of samples are separated from each other in the fluid flow stream by a separation gas, thereby forming a gas-separated fluid flow stream. The gas-separated fluid flow stream is independently guided to and through each separate flow cytometer.

-27-

ABSTRACT

Embodiments of the present invention provide a system and method for analyzing a plurality of samples comprising obtaining with an autoamplifier a plurality of samples from a first plate having a plurality of sample wells wherein the autosampler has a plurality of probes for sampling a set of samples and wherein each probe of the plurality of probes is in communication with a separate flow cytometer via a separate conduit. The plurality of samples comprising particles is moved into a fluid flow stream for each separate conduit. Adjacent ones of the plurality of samples are separated from each other in the fluid flow stream by a separation gas, thereby forming a gas-separated fluid flow stream. The gas-separated fluid flow stream is independently guided to and through each separate flow cytometer.

PATENT APPLICATION

MULTI-SAMPLE PARTICLE ANALYZER SYSTEM AND METHOD FOR HIGH THROUGHPUT SCREENINGCROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to and the benefit of the filing of U.S. Provisional Patent Application Serial No. 61/080,171, entitled " Multi-Sample Particle Analyzer System and Method for High-Throughput Screening ", filed on July 11, 2008, and the specification and claims thereof are incorporated herein by reference.

BACKGROUND OF THE INVENTIONField of the Invention (Technical Field):

[0002] The present invention relates to a particle analyzer and sample handling for use with particle analysis apparatus and a method for high-throughput analysis using the same.

[0003] Particle analysis using flow cytometry is used to characterize cells and particles by making measurements on each at rates up to thousands of events per second. The measurement consists of simultaneous detection of the light scatter and fluorescence associated with each event. Commonly, the fluorescence characterizes the expression of cell surface molecules or intracellular markers sensitive to cellular responses to drug molecules. The technique often permits homogeneous analysis such that cell associated fluorescence can often be measured in a background of free fluorescent indicator. The technique often permits individual particles to be sorted from one another.

[0004] However, a deficiency with conventional flow cytometry is that it does not allow for the analysis of multiple samples consisting of multiple cells or particles in a rapid manner, a fact that has limited the uses of flow cytometry in drug discovery and other high throughput screening applications. For example, the industrial standard for high throughput drug discovery is 100,000 samples per day. Because of its low throughput, flow cytometry has generally not been considered applicable to high throughput screening applications in areas such as drug discovery, antibody hybridoma screening, and systems biology.

[0005] There have been several efforts at automated sample handling in flow cytometry. For example, sample handling systems are known that use carousels to handle samples from standard sized tubes and sample injection systems which handle samples from 96-384 well

microplates. These systems treat each tube or well as a single sample. A separate data file is created for each sample. These systems typically intake samples at a rate of approximately 1 up to 5 samples per minute and require priming the sample line with each individual specimen before analysis. Therefore, a single data file exists for each well sample interrogated.

[0006] Other groups have also used valves and syringes in flow cytometry, most notably, the "flow injection" group, Lindberg et al. at University of Washington. However, the processes described above did not address throughput speed. A group at the University of New Mexico has used high throughput flow cytometry and achieved sampling rates as high as 40 samples per minute, see U.S. patents 6878556, 6890487, 7368084, the entire disclosure and contents of which is hereby incorporated by reference. However, to our knowledge, no one has reported the capability to process samples at rates higher than 40 samples per minute for flow cytometry.

[0007] The presence of uncontrolled bubbles in the flow cytometer system is one of the primary sources of corrupted experimental data. Flow cytometers may periodically experience bubbles in the sheath fluid or sample fluid lines. Precautions are taken to exclude bubbles as bubbles are known to cause anomalies in the flow within the flow cytometer system that reduce the performance of the flow cytometer. Furthermore, bubbles passing through the interrogation zone of the flow cytometer can cause spurious or false event signals that corrupt the experimental data being collected. The user can take corrective action only after the bubbles have been detected, which often occurs after experimental data has been corrupted and the user has been inconvenienced. Therefore the flow cytometry art teaches against introduction of bubbles in the flow stream.

SUMMARY OF THE INVENTION

[0008] It is an aspect of the present invention to provide a flow cytometry apparatus that meets the needs of high throughput screening for multiwell, for example, 96, 384, or 1536 well microplates.

[0009] It is an aspect of the present invention to provide a method for analyzing a plurality of samples in a single source file using high throughput screening.

[0010] It is another aspect of the present invention to separate with a gas a plurality of adjacent samples in a fluid flow stream which passes through a flow cytometer for analysis.

[0011] One embodiment of the present invention provides for a method for analyzing a plurality of samples comprising obtaining with an autoamplifier a plurality of samples from a first plate

having a plurality of sample wells wherein the autosampler has a plurality of probes for sampling a set of samples and wherein each probe of the plurality of probes is in communication with a separate flow cytometer via a separate conduit. The plurality of samples comprising particles is moved into a fluid flow stream for each separate conduit. Adjacent ones of the plurality of samples are separated from each other in the fluid flow stream by a separation gas, thereby forming a gas-separated fluid flow stream. The gas-separated fluid flow stream is independently guided to and through each separate flow cytometer.

[0012] Another embodiment of the present invention provides for a method for analyzing a plurality of samples comprising the steps of obtaining with an autoamplifier a plurality of samples from a first plate having a plurality of sample wells wherein the autosampler has a plurality of probes for sampling a set of samples and wherein each probe of the plurality of probes is in communication with a single multi-channel flow cytometer via a separate conduit attached to each of the probes in the plurality of probes. The plurality of samples comprising particles are moved into a fluid flow stream for each separate conduit. Adjacent ones of the plurality of samples are separated from each other in the fluid flow stream by a separation gas, thereby forming a gas-separated fluid flow stream. The gas separated fluid flow stream is independently guided to and through the single multi-channel flow cytometer. The multi-channel flow cytometer is operated to focus the gas-separated fluid flow stream and to selectively analyze the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through the multi-channel flow cytometer.

[0013] In a preferred embodiment, the step of moving may occur with gravity, or suction, or pumping or pushing. In another preferred embodiment, moving the plurality of samples is with a fluid moving device located before or after the cytometer. For example the fluid moving device is a multihead peristaltic pump. The conduit through which the fluid flow streams move may be tubing. The step of moving the plurality of fluid flow streams through each separate conduit is at a rate that may be independently controlled for each conduit.

[0014] In another preferred embodiment the first plate is positioned on a platform that is moveable in the xyz direction to bring the samples to the probes. Alternatively the plurality of probes are positionable and move to the samples on the first plate. In another embodiment a probe of the plurality of probes is positionable and moves to a plurality of samples located on a second plate. Further still, two or more probes may or may not occupy the same sample well at the same time.

[0015] Yet another embodiment to the present invention provides for a flow cytometry apparatus comprising an autosampler comprising a plurality of probes with each probe suitable for inserting a plurality of samples comprising particles from a plurality of respective source wells into a separate fluid flow stream. A plurality of flow cytometers in communication with the plurality of

-4-

probes of the autosampler via a separate conduit connecting one probe of the plurality of probes with one flow cytometer of the plurality of flow cytometers. Moving the plurality of samples in each separate fluid flow streams through each separate conduit to a selected cytometer of the plurality of flow cytometers, the plurality of probes introducing aliquots of a separation fluid between successive ones of the plurality of samples in each of the separate fluid flow streams to configure each of the separate fluid flow streams as a gas-separated fluid flow stream, each of the plurality of flow cytometers focusing the gas-separated fluid flow stream delivered by the separate conduit and selectively analyzing the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through each separate cytometer of the plurality of cytometers. In a preferred embodiment of the present invention the plurality of probes are positioned on a bracket. Alternatively, the plurality of probes are positionable relative to the plurality of respective source wells and/or the bracket is fixed relative to the plurality of respective source wells and/or the probes are independently positionable relative to each other and the plurality of respective source wells. In a preferred embodiment, the apparatus further comprises a fluid movement device which may be a pump such as a peristaltic pump. The pump may be positioned before or after each flow cytometer. The fluid movement device comprises a plurality of fluid movement devices each one of the plurality of fluid movement devices may be associated with a separate conduit. In a preferred embodiment the step of moving is selected from pumping, pushing, suctioning or moving with gravity.

[0016] Yet another embodiment provides for a flow cytometry apparatus comprising an autosampler comprising a plurality of probes for inserting a plurality of samples comprising particles from a plurality of respective source wells into a plurality of fluid flow streams. A multi-channel flow cytometer is in communication with the plurality of probes of the autosampler via a plurality of separate conduits connected to one each of the probes of the plurality of probes wherein each of the separate conduits of the plurality moves a separate fluid flow stream of the plurality of fluid flow streams. The plurality of samples moving in each of the separate fluid flow streams moving in each separate conduit moves to the multi-channel flow cytometer with the autosampler introducing aliquots of a separation fluid between successive ones of the plurality of samples in the fluid flow stream to configure the fluid flow stream as a gas-separated fluid flow stream. The multi-channel flow cytometer focusing the gas-separated fluid flow stream delivered by the conduit from the autosampler and selectively analyzing the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through the multi-channel flow cytometer.

[0017] Yet another embodiment to the present invention provides for a flow cytometry apparatus comprising an autosampler comprising a probe with each probe suitable for inserting a sample comprising particles from a source well into a fluid flow stream. A flow cytometer in communication with the probe of the autosampler via a conduit connecting the probe with the flow cytometer. Moving the samples in the fluid flow stream through the conduit to the cytometer, the

probe introducing aliquots of a separation fluid between successive ones of the plurality of samples in the fluid flow streams to configure the fluid flow stream as a gas-separated fluid flow stream, each of the plurality of flow cytometers focusing the gas-separated fluid flow stream delivered by the separate conduit and selectively analyzing the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through the flow cytometer. The apparatus further comprising a fluid movement device located after the cytometer such that the fluid movement device assists the autosampler with introducing aliquots of a separation fluid between successive ones of the plurality of samples. In an alternative embodiment the gas is pushed into the sample via pressurization.

[0018] Additional objects and advantages of the present invention will be apparent in the following detailed description read in conjunction with the accompanying drawing figures.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWINGS

[0019] The accompanying drawings, which are incorporated into and form a part of the specification, illustrate one or more embodiments of the present invention and, together with the description, serve to explain the principles of the invention. The drawings are only for the purpose of illustrating one or more preferred embodiments of the invention and are not to be construed as limiting the invention. In the drawings:

[0020] Fig. 1 illustrates a particle analysis apparatus according to one embodiment of the present invention.

[0021] Fig. 2 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0022] Fig. 3 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0023] Fig. 4 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0024] Fig. 5 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0025] Fig. 6 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0026] Fig. 7 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0027] Fig. 8 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0028] Fig. 9 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0029] Fig. 10 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0030] Fig. 11 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0031] Fig. 12 illustrates a particle analysis apparatus according to another embodiment of the present invention.

[0032] Fig. 13 illustrates cytometry results of forward scatter vs. side scatter with a system and method according to one embodiment of the present invention.

[0033] Fig. 14 illustrates cytometry results of fluorescence vs. time with a system and method according to one embodiment of the present invention.

[0034] Fig. 15 illustrates a particle analysis apparatus according to another embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0035] It is advantageous to define several terms before describing the invention. It should be appreciated that the following definitions are used throughout this application.

Definitions:

[0036] Where the definition of terms departs from the commonly used meaning of the term, applicant intends to utilize the definitions provided below, unless specifically indicated.

[0037] For the purposes of the present invention, the term "particles" refers to any particles that may be detected using a particle analyzer such as a cytometer where particles are focused hydrodynamically, acoustically or with capillary action.

[0038] For the purposes of the present invention, the term "source well" refers to any container that is intended to hold a fluid such as a fluid sample, for example a well on a well plate, whether or not the source well contains a sample. For the purposes of the present invention, the term "sample source well" refers to a source well containing a sample.

[0039] For the purposes of the present invention, the term "sample" refers to a fluid solution or suspension containing particles to be analyzed using a method and/or apparatus of the present invention. The particles to be analyzed in a sample may be tagged, such as with a fluorescent tag. The particles to be analyzed may also be bound to a bead, a receptor, or other useful protein or polypeptide, or may just be present as free particles, such as particles found naturally in a cell lysate, purified particles from a cell lysate, particles from a tissue culture, etc. The sample may include chemicals, either organic or inorganic, used to produce a reaction with the particles to be analyzed. When the particles to be analyzed are biomaterials, drugs may be added to the samples to cause a reaction or response in the biomaterial particles. The chemicals, drugs or other additives may be added to and mixed with the samples when the samples are in sample source wells or the chemicals, drugs or other additives may be added to the samples in the fluid flow stream after the samples have been intaken by the autosampler.

[0040] For the purposes of the present invention, the term "adjacent samples" refers to two samples in a fluid flow stream that are separated from each other by a separation gas, such as an air bubble. For the purposes of the present invention, the term "immediately adjacent samples" refers to adjacent samples that are only separated from each other by a separation gas. For the purposes of the present invention, "buffer fluid separated adjacent samples" refers to adjacent samples that are separated from each other by two separation gas bubbles and a buffer fluid, with the buffer fluid being located between the two separation gas bubbles.

[0041] For the purposes of the present invention, the term "separation gas" refers to any gas such as air, an inert gas, or fluid, etc. that can be used to form a gas bubble or immiscible fluid between adjacent samples or between a sample and a buffer fluid. An immiscible fluid is a fluid that will not substantially mix with and contaminate a sample.

[0042] For the purposes of the present invention, the term "buffer fluid" refers to a fluid that is substantially free of the particles to be detected by the apparatus and method of the present invention.

[0043] For the purposes of the present invention, the term "plurality" refers to two or more of anything, such as a plurality of samples. For the purposes of the present invention, the terms "a", "an" or "the" refers to one or more of anything, such as a sample or the sample.

[0044] For the purposes of the present invention, the term "homogenous" refers to a plurality of identical samples. The term "homogenous" also refers to a plurality of samples that are indistinguishable with respect to a particular property being measured by an apparatus or a method of the present invention.

[0045] For the purposes of the present invention, the term "heterogeneous" refers to a plurality of samples in a fluid flow stream in which there are at least two different types of samples in the fluid flow stream. One way a heterogeneous plurality of samples in a fluid flow stream of the present invention may be obtained is by intaking different samples from different source wells in a well plate. The identification of sequential samples to be analyzed in the fluid flow stream is based upon the separation of the fluid samples by one or more bubbles of a separation gas and/or one or more portions of a buffer fluid. Another way of obtaining a heterogeneous plurality of samples is by intaking different samples from identical source wells at various time points where a reaction or a series of reactions is or had been occurring.

[0046] For the purposes of the present invention, the term "fluid flow stream" refers to a stream of fluid samples, separated by one or more bubbles of a separation gas and/or one or more portions of a buffer fluid.

[0047] For the purpose of the present invention, the term "fluid flow path" refers to device such as a conduit, tube, channel, etc. through which a fluid flow stream flows. A fluid flow path may be composed of several separate devices, such as a number of connected or joined pieces of tubing or a single piece of tubing, alone or in combination with channels or other different devices.

[0048] For the purposes of the present invention, the term "high speed multi-sample tube" includes any tube that may be used with a fluid movement device such as a peristaltic pump, a syringe pump, an injector, or gravity. The tubing for use with a peristaltic pump for example may have compression characteristics that allow a peristaltic pump to move samples separated by a separation gas through the tube at a speed of at least 6 samples per minute without causing adjacent samples to mix with each other.

Detailed Description of the Invention:

[0049] An embodiment of the present invention preferably uses a separation fluid, such as air, water, bubbles, or a combination thereof to separate samples introduced from an autosampler into a conduit such as a tubing line that connects directly or indirectly the autosampler and a particle analyzer such as a flow cytometer using sheath fluid or acoustic forces or capillary action to focus particles to an interrogation zone of a flow cell. In one embodiment, the fluid is moved from the autosampler to the particle analyzer. The fluid sample is pulled or pushed through a conduit by for example by pump action, suction, syringe or by gravity. A separation fluid such as a gas, preferably air bubbles, effectively separates a sample into a plurality of samples or separates a first sample from a second sample which have previously occupied different sample source well locations on a plate. Samples separated by air bubbles are analyzed by the particle analyzer as a continuous fluid sample. Data from the optical signature of a plurality of samples in the fluid sample stream is collected in a single data file. An interrogation zone is an area within a particle analyzer where the particles are aligned or focused. A light source such as a laser and a light detector are connected to the interrogation zone such that a sample flowing through the interrogation zone can be optically analyzed through methods known in the art of flow cytometry. The particle analyzer may or may not contain a flow cell.

[0050] FIG. 1 illustrates a preferred multi-sample particle analyzer apparatus **100** of one embodiment of the present invention. Multi-sample particle analyzer apparatus **100** preferably comprises conventional autosampler, for example a gantry robot, having adjustable XYZ positioning arm **102** on which is positioned a plurality of hollow probes **104 a-d**. As arm **102** moves back and forth (left and right in FIG. 1) and side to side (into and out of the plane of FIG. 1), one or more of a plurality of probes selected from **104 a-d** are lowered into different individual source wells **108 a-g** of plate **106** to obtain a first sample. The movement of the sample probes with regards to the sample source wells is programmed by a user into a computer programmed with instructions for moving the arm in the XYZ directions in space. The first sample may have been spiked with particles of different size or tags having a fluorescent property that will be detected upon interrogation of the sample with a light source such as a laser. One or more of probes **104 a-d** uptakes a sample from a separate well **108 a-d**.

[0051] Once a sample is picked up by one or more of the plurality of probes **104 a-d**, the sample is moved through a tube **110 a-d** in communication with the corresponding probe selected from **104 a-d** such that the tube extends from autosampler XYZ arm **102** and into a multi-channel fluid movement device such as a multihead peristaltic pump or multiple injectors **120** and then into a particle analyzer **130, 132, 134, 136** in communication with the respective tube **110 a-d**. A particle analyzer **130, 132, 134, 136** may comprise one or more of the following: a flow cell, a means for focusing the particles to a desired location within the flow cell for the sample to be analyzed, a laser

interrogation device, an optical system configured to receive and focus the light from a laser source, a spectrum detector, a fiber optic transmission means, processor for collecting data from particles, and data storage. A laser interrogation device examines individual samples flowing through a flow cell located therein at a laser interrogation point. In between intaking sample material from each of source wells **108**, one or more of the plurality of probes **104 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **104 a-d** and through the respective tube **110 a-d** are communicated to a respective individual particle analyzer for example **130, 132, 134, 136**. In a preferred embodiment the fluid movement device is positioned after the particle analyzer and therefore the sample moves from the sample probe to the particle analyzer through the tube.

[0052] When a fluid sample having particles therein passes through a laser interrogation point, the particles in the fluid sample are sensed by the particle analyzer for example **130** of FIG. 1 due to, for example, a fluorescent tag on the particles or the light scattering properties of the particles themselves. In contrast, when air bubbles pass through laser interrogation point no particles are sensed. Therefore, a graph of the data points of fluorescence sensed versus time for a series of samples analyzed using the particle analyzer of the present invention will form distinct groups, each aligned with the time that a sample containing particles passes through the laser interrogation point.

[0053] In order to detect the presence of each of two or more different types of samples, in a heterogeneous plurality of samples, each of the two or more different types of samples may be tagged with different fluorescent tags, different amounts of a single tag or some combination of different tags and different amount of a single tag. In such a case, the groupings of data points will vary vertically on a fluorescence versus time graph, depending on which type of sample is being sensed. As with the case of sensing a single type of sample, each sensed sample will exhibit a group of data points aligned with the time that the sample passes through the laser interrogation point.

[0054] In one embodiment of the device, samples from selected wells in the well plate are introduced as a single specimen to a particle analyzer and data from all of the wells in the plate or a portion of a plate are collected in a single data file by the particle analyzer system. In a preferred embodiment, sample from every well having sample herein in the plate is introduced as a single specimen in a continuous manner. In the case of multiprobe sample introduction, multiple analyzers may create multiple data files that the analysis protocol will associate with the well from which the sample was taken. Multichannel sampling from a single plate into multiple particle analyzers, or multiplate data from multiple analyzers are analyzed by proprietary software that correlates the data with individual well information.

[0055] In an alternative embodiment of the present invention using the particle analyzer apparatus of FIG. 1, some of the source wells on the well plate of the apparatus illustrated in FIG. 1 may contain a buffer solution to allow for the formation of buffer fluid separated adjacent samples in a tube through which samples pass. When this is the case, after the first sample is taken up by the probe from a first well, the probe intakes air, then buffer solution, located in second well, then the probe uptakes air again, and then the probe uptakes a second sample, located in a third well. This sequence may then be repeated for additional samples located in subsequent wells, which the probe subsequently intakes.

[0056] A graph of the data points of fluorescence detected versus time for a series of samples analyzed using one embodiment of the particle analyzer of the present invention will form distinct groups, each aligned with the time that a sample containing particles passes through the laser interrogation point (see for example FIG. 14). In order to detect the presence of two or more different types of samples, each of the two or more different types of samples may be tagged with different fluorescence tags or different amounts of a single tag as compared to the particle in the sample. In such a case, the groupings of data points will vary vertically on a fluorescence versus time graph, depending on which type of sample is being sensed. As with the case of sensing a single type of sample, each sensed sample will exhibit a group of data points aligned with the time that the sample passes through the laser interrogation point.

[0057] Alternatively, buffer fluid separated adjacent samples may be formed by providing a reservoir of buffer fluid in the autosampler or attached to the autosampler to inject buffer fluid into the tube for the fluid flow stream. In this case, after each sample is taken up by the probe, the probe intakes air, then buffer fluid is injected into the tube for the fluid flow stream, then the probe intakes air again, and then the probe intakes a second sample. This sequence may then be repeated for subsequent samples to be separated by a buffer fluid.

[0058] One embodiment of the present invention is compatible with standard commercial multi-well plates for use with autosamplers from 96 well plates to 1536 well plates or greater. The source wells of one embodiment of the present invention may be all filled with samples and/or buffer fluids, or some may be left empty or some combination thereof. When there is a plurality of different types of samples in the source wells of a well plate, the sample types may be arranged in the order in which they are taken up by the probe, or the sample types may be arranged in any other convenient arrangement. For example, all of the source wells in a first row of source wells may contain one sample type and all of the source wells of a second row may contain a second sample type. Or individual wells may contain multiple specimens that are differentiated by size of particles within the sample or fluorescent probes within the sample associated with particles therein.

[0059] The source wells may be of any conventional shape used for source wells in a well plate for an autosampler. Preferably, when small amounts of sample are used in each source well, the source wells are conical in shape, to allow even the smallest amounts of sample to be withdrawn by the probe or to allow the particles to concentrate in the bottom of the well. The use of a well plate with conical source wells reduces the problems associated with the settling of particles to the bottom of the well prior to being intaken by the probe. A device which resuspends the particles before and during sampling such as an orbital shaker can be used to reduce issues associated with settling of particles and is being used in the current embodiment of the invention. FIG. 2 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **200** of the present invention. Multi-sample particle analyzer apparatus **200** preferably comprises conventional XYZ stage **202** on which is positioned a well plate **206**. The plurality of probes **204 a-d** are stationary as stage **202** moves back and forth (left and right in FIG. 2) and side to side (into and out of the plane of FIG. 2), the stage **202** raises and lowers the well plate **206** to a plurality of probes **204 a-d** so that individual samples from individual source wells **208 a-g** are obtained from well plate **206**. Alternatively, the probes may be positionable and move to the sample well. Further still, the probes and the well plate may move with respect to each other in a coordinated fashion.

[0060] Once a sample is picked up by one or more of the plurality of probes **204 a-d**, the sample is moved through a tube **210 a-d** in communication with the corresponding probe selected from **204 a-d** such that the tube extends from the respective probe **204 a-d** into a multi-channel fluid movement device **220** and then into the particle analyzers in communication with the respective tube **210 a-d**. However, the fluid movement device **220** is not required to be located between the sample probe and the particle analyzer as the fluid movement device may be located after the particle analyzer or may be absent altogether in the case of gravity moving the samples. A particle analyzer **230, 232, 234, 236** comprises a flow cell and a laser interrogation device. A laser interrogation device examines individual samples flowing through a flow cell located therein at a laser interrogation point. In between taking up sample material from each of source wells **208 a-d** for example, one or more of the plurality of probes **204 a-d** is allowed to intake (sometimes referred to herein as uptake) a fluid such as air prior to moving to a subsequent well, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **204 a-d** and through the respective tube **210 a-d** are communicated to a respective individual particle analyzer **230, 232, 234, 236**. Multichannel fluid movement device may be for example a multihead peristaltic pump or a multichannel push-pull syringe system.

[0061] FIG. 3 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **300** of the present invention. Multi-sample particle analyzer apparatus **300** preferably comprises conventional autosampler having adjustable XYZ positioning arm **302** on which is

positioned a plurality of hollow probes **304 a-d**. As arm **302** moves back and forth (left and right in FIG. 3) and side to side (into and out of the plane of FIG. 3), a plurality of probes selected from **304 a-d** are lowered into individual source wells **308** of well plate **306** to obtain a sample.

[0062] Once a sample is picked up by one or more of the plurality of probes **304 a-d**, the sample is moved through a conduit **310 a-d** in communication with the corresponding probe selected from **304 a-d** such that the conduit extends from autosampler XYZ arm **302** to the particle analyzers in communication with the respective tube **310 a-d**. A particle analyzer **330, 332, 334, 336** comprises a flow cell and a laser interrogation device. A laser interrogation device examines individual samples flowing through a flow cell located therein at a laser interrogation point. In between intaking sample material from each of source wells **308**, one or more of the plurality of probes **304 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **304 a-d** and through the respective tube **310 a-d** are communicated to a respective individual particle analyzer **330, 332, 334, 336**. The sample is moved to a particle analyzer by a fluid movement device which may be located before the probe, between the probe and the particle analyzer or after the particle analyzer.

[0063] FIG. 4 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **400** of the present invention. Multi-sample particle analyzer apparatus **400** preferably comprises conventional XYZ stage **402** on which is positioned a well plate **406**. The plurality of hollow probes **404 a-d** are stationary as stage **402** moves back and forth (left and right in FIG. 4) and side to side (into and out of the plane of FIG. 4), the stage **402** raises and lower the well plate **406** to a plurality of probes **404 a-d** so that individual samples from individual source wells **408** are obtained of well plate **406**. The probes may be positioned on one or more arms (sometimes referred to herein as a bracket) with each arm independently controlled to coordinate sampling of the sample wells. The arms may be controlled by a computer with instructions for moving the sample well plate and/or the probes.

[0064] Once a sample is picked up by one or more of the plurality of probes **404 a-d**, the sample is moved through a tube **410 a-d** in communication with the corresponding probe selected from **404 a-d** such that the tube extends from the respective probe **404 a-d** into a multi-channel fluid movement device **420** and then into the particle analyzers in communication with the respective tube **210 a-d**. However, the multi-channel fluid movement device **410 a-d** may be located after the particle analyzer or before the sample probe. A particle analyzer **430, 432, 434, 436** comprises a flow cell and a laser interrogation device. A laser interrogation device examines individual samples flowing through a flow cell located therein at a laser interrogation point. In between intaking sample material from each of source wells **408**, one or more of the plurality of probes **404 a-d** is allowed to

intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **404 a-d** and through the respective tube **410 a-d** are communicated to a respective individual particle analyzer **430, 432, 434, 436**.

[0065] FIG. 5 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **500** of the present invention. Multi-sample particle analyzer apparatus **500** preferably comprises conventional autosampler having adjustable XYZ positioning arm **502** on which is positioned one or more hollow probes **504 a-d**. As arm **502** moves back and forth (left and right in FIG. 5) and side to side (into and out of the plane of FIG. 5), a plurality of probes selected from **504 a-d** are lowered into individual source wells **508 a-g** of well plate **506** to obtain a separate sample for each probe.

[0066] Once a portion of a sample is withdrawn from a sample well by one or more of the plurality of probes **504 a-d**, the sample is moved through a conduit such as a tube **510 a-d** in communication with the corresponding probe selected from **504 a-d** such that the tube extends from autosampler XYZ arm **502** and into the particle analyzers in communication with the respective tube **510 a-d**. The particle analyzer **530, 532, 534, 536** may comprise a flow cell and a laser interrogation device. A laser interrogation device examines individual samples flowing past a laser interrogation point within the particle analyzer. In between intaking sample material from each of source wells **508**, one or more of the plurality of probes **504 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **504 a-d** and through the respective tube **510 a-d** are communicated to a respective individual particle analyzer **530, 532, 534, 536**.

[0067] FIG. 6 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **600** of the present invention. Multi-sample particle analyzer apparatus **600** preferably comprises conventional XYZ stage **602** on which is positioned a well plate **606**. The plurality of hollow probes **604 a-d** are stationary as stage **602** moves back and forth (left and right in FIG. 6) and side to side (into and out of the plane of FIG. 6), the stage **602** raises and lower the well plate **606** to a plurality of probes **604 a-d** so that individual samples from individual source wells **608** are obtained from well plate **606**. Probes **604 a-d** may be fixed in space relative to each other or may move relative to the stage **602** and relative to the other probes **604 a-d**.

[0068] Once a sample is picked up by one or more of the plurality of probes **604 a-d**, the sample is moved through a tube **610 a-d** in communication with the corresponding probe selected from **604 a-d** such that the tube extends from the respective probe **604 a-d** to the particle analyzer to deliver the sample for analysis. A particle analyzer **630, 632, 634, 636** may comprise a flow cell and a laser interrogation device. A laser interrogation device examines individual samples flowing

within the particle analyzer by focusing a beam of light at a laser interrogation point and detecting the beam of laser light or alterations at an optical detector. In between intaking sample material from each of source wells **608**, one or more of the plurality of probes **604 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **604 a-d** and through the respective tube **610 a-d** are communicated to a respective individual particle analyzer **630, 632, 634, 636**.

[0069] FIG. 7 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **700** of the present invention. Multi-sample particle analyzer apparatus **700** preferably comprises conventional autosampler having adjustable XYZ positioning arm **702** on which is positioned a plurality of hollow probes **704 a-d**. As arm **702** moves back and forth (left and right in FIG. 7) and side to side (into and out of the plane of FIG. 7), a plurality of probes selected from **704 a-d** are lowered into individual source wells **708** of well plate **706** to obtain a sample.

[0070] Once a sample is picked up by one or more of the plurality of probes **704 a-d**, the sample is moved through a tube **710 a-d** in communication with the corresponding probe selected from **704 a-d** such that the tube extends from autosampler XYZ arm **702** and into a multi-channel fluid movement device **720** and then into the particle analyzer in communication with the respective tube **710 a-d**. However, the fluid movement device may be located after the particle analyzer **730** or before the probes. A plurality of samples are communicated to a single multi-channel particle analyzer **730** which will multiplex the samples to a single laser interrogation device and analyze the samples simultaneously. A laser interrogation device examines individual samples flowing through a flow cell located within the particle analyzer at a laser interrogation point. In between uptaking sample material from each of source wells **708**, one or more of the plurality of probes **704 a-d** is allowed to uptake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **704 a-d** and through the respective tube **710 a-d** are communicated to a multi-channel particle analyzer **730**.

[0071] FIG. 8 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **800** of the present invention. Multi-sample particle analyzer apparatus **800** preferably comprises conventional XYZ stage **802** on which is positioned a well plate **806**. A plurality of probes **804 a-d** are stationary as stage **802** moves back and forth (left and right in FIG. 8) and side to side (into and out of the plane of FIG. 8), the stage **802** raises and lower the well plate **806** to the plurality of probes **804 a-d** so that individual samples from individual source wells **808** of well plate **806** are sampled. The plurality of probes have an open first end and an open second end apposite the first end. The open second end connects to a conduit. The sample flows from the sample well to the particle analyzer through the conduit. A conduit as used herein may be a channel, a tube, a groove or other structure that guides the fluid sample stream or fluid flow path to the particle analyzer.

[0072] Once a sample is picked up by one or more of the plurality of probes **804 a-d**, the sample is moved through a conduit **810 a-d** in communication with the corresponding probe selected from **804 a-d** such that the conduit extends from the respective probe **804 a-d** into a multi-channel fluid movement device **820** and then into the particle analyzers in communication with the respective conduit **810 a-d**. However, the multiple single-channel fluid movement devices **920 a-d** may be positioned after the particle analyzer or before the probes. The plurality of samples are communicated to a single multi-channel particle analyzer **830** which will multiplex the samples to a single laser interrogation device and analyze the samples simultaneously. In between uptaking sample material from each of source wells **808**, one or more of the plurality of probes **804 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **804 a-d** and through the respective tube **810 a-d** are communicated to a multi-channel particle analyzer **830**.

[0073] FIG. 9 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **900** of the present invention. Multi-sample article analyzer apparatus **900** preferably comprises conventional autosampler having adjustable XYZ positioning arm **902** on which is positioned a plurality of hollow probes **904 a-d**. As arm **902** moves back and forth (left and right in FIG. 9) and side to side (into and out of the plane of FIG. 9), a plurality of probes selected from **904 a-d** are lowered into individual source wells **908** of well plate **906** to obtain a sample.

[0074] Once a sample is picked up by one or more of the plurality of probes **904 a-d**, the sample is moved through a tube **910 a-d** in communication with the corresponding probe selected from **904 a-d** such that the tube extends from autosampler XYZ arm **902** and into multiple single-channel fluid movement devices **920 a-d** and then into the particle analyzers in communication with the respective tube **910 a-d**. However, the multiple single-channel fluid movement devices **920 a-d** may be position after the particle analyzer or before the probes. The fluid flow streams may be moved at different rates or the same rates by the fluid movement device. A plurality of samples are communicated to a single multi-channel particle analyzer **930** which will multiplex the samples to a single laser interrogation device and analyze the samples simultaneously. A laser interrogation device examines individual samples flowing through a flow cell located therein at a laser interrogation point. In between intaking sample material from each of source wells **908**, one or more of the plurality of probes **904 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **904 a-d** and through the respective tube **910 a-d** are communicated to a multi-channel particle analyzer **930**.

[0075] FIG. 10 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **1000** of the present invention. Multi-sample particle analyzer apparatus **1000** preferably comprises conventional XYZ stage **1002** on which is positioned a well plate **1006**. The plurality of hollow probes **1004 a-d** are stationary as stage **1002** moves back and forth (left and right in FIG. 10) and side to side (into and out of the plane of FIG. 10), the stage **1002** raises and lower the well plate **1006** to a plurality of probes **1004 a-d** so that individual samples from individual source wells **1008** are obtained of well plate **1006**.

[0076] Once a sample is picked up by one or more of the plurality of probes **1004 a-d**, the sample is moved through a tube **1010 a-d** in communication with the corresponding probe selected from **1004 a-d** such that the tube extends from the respective probe **1004 a-d** into a multi-channel fluid movement device **1020** and then into the particle analyzers in communication with the respective tube **210 a-d**. However, the fluid movement device **1020 a-d** may be located after the particle analyzer **1030**. The plurality of samples are communicated to a single multi-channel particle analyzer **1030** which will multiplex the samples to a single laser interrogation device and analyze the samples simultaneously. In between intaking sample material from each of source wells **1008**, one or more of the plurality of probes **1004 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **1004 a-d** and through the respective tube **1010 a-d** are communicated to a multi-channel particle analyzer **1030**.

[0077] FIG. 11 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **1100** of the present invention. Multi-sample particle analyzer apparatus **1100** preferably comprises an autosampler having adjustable XYZ positioning arm **1102** on which is positioned a plurality of hollow probes **1104 a-d**. As arm **1102** moves back and forth (left and right in FIG. 11) and side to side (into and out of the plane of FIG. 11), a plurality of probes selected from **1104 a-d** are lowered into individual source wells **1108** of well plate **1106** to obtain a sample.

[0078] Once a sample is picked up by one or more of the plurality of probes **1104 a-d**, the sample is moved through a tube **1110 a-d** in communication with the corresponding probe selected from **1104 a-d** such that the tube extends from autosampler XYZ arm **1102** and into the particle analyzers in communication with the respective tube **1110 a-d**. The plurality of samples are communicated to a single multi-channel particle analyzer **1130** which will multiplex the samples to a single laser interrogation device and analyze the samples simultaneously. A laser interrogation device interrogates a sample flowing through a flow cell located therein at a laser interrogation point. In between uptaking individual samples from a second source well **1108 a-g**, a probe **1104 a-d** introduces a fluid such as air between a first sample and a second sample, thereby forming a gas separation between the first sample and the second sample to form a continuous fluid flow stream to

be analyzed. The continuous fluid flow stream from each of the probes **1104 a-d** and through the respective tube **1110 a-d** are communicated to a multi-channel particle analyzer **1130**.

[0079] FIG. 12 illustrates an alternative embodiment of the multi-sample particle analyzer apparatus **1200** of the present invention. Multi-sample particle analyzer apparatus **1200** preferably comprises conventional XYZ stage **1202** on which is positioned a well plate **1206**. The plurality of hollow probes **1204 a-d** are stationary as stage **1202** moves back and forth (left and right in FIG. 12) and side to side (into and out of the plane of FIG. 12), the stage **1202** raises and lower the well plate **1206** to a plurality of probes **1204 a-d** so that individual samples from individual source wells **1208** are obtained of well plate **1206**.

[0080] Once a sample is withdrawn by one or more of the plurality of probes **1204 a-d**, the sample is moved through a tube **1210 a-d** in communication with the corresponding probe selected from **1204 a-d** such that the tube extends from the respective probe **1204 a-d** into the particle analyzers in communication with the respective tube **1210 a-d**. The plurality of samples are communicated to a single multi-channel particle analyzer **1230** which will multiplex the samples to a single laser interrogation device and analyze the samples simultaneously. A laser interrogation device examines individual samples flowing through a flow cell located therein at a laser interrogation point. In between intaking sample material from each of source wells **1208**, one or more of the plurality of probes **1204 a-d** is allowed to intake a fluid such as air, thereby forming a gas separation between each adjacent sample. The continuous fluid flow stream from each of the probes **1204 a-d** and through the respective tube **1210 a-d** are communicated to a multi-channel particle analyzer **1230**.

[0081] FIG. 13 illustrates cytometry results of forward scatter vs. side scatter with a gate around the particles aligned in the laser beam according to one embodiment of the present invention.

[0082] FIG. 14 illustrates flow cytometry results using a fluid means to move samples **1402, 1406, 1410, and 1414** naming particles having a first fluorochrome as a fluorescence tag and four samples **1404, 1408, 1412, and 1416** having particles having a second fluorochrome as a fluorescence tag. FIG. 14 is a graph of Fluorescence vs. Time (1024 channels=60 seconds).

[0083] FIG. 15 illustrates an embodiment of the present invention wherein multiple sample probes **1504 a-d** are positioned in a plurality of sample source wells **1508 a-d** from a plurality of plates **1506 a-d**. The samples withdrawn from the plates by the probes are moved to a particle analyzer (not shown) through conduits **1510 a-d** connected to a respective probe **1508 a-d**. The plates may be positioned on a platform that moves the plates in the XYZ dimensions in space or the

probes may move in the XYZ dimensions in space relative to the plates, relative to each other or both.

[0084] The autosampler of the present invention may be any conventional autosampler suitable for intaking samples from a well plate or other sample source container. For example, an autosampler as produced by TM the Gilson 223 liquid manager.

[0085] The XYZ stage of the present invention may be any XYZ stage suitable for positioning a well plate.

[0086] The use of automation, for example a robotic plate loader, in plate delivery and retrieval for the autosampler or XYZ stage may allow automation of the overall screening process.

[0087] One preferred probe for the present invention is a 0.01 inch ID, inch OD stainless steel needle compatible with HPLC ferrule fittings. Similar probes with reinforced tubular sheaths are suited for multiprobe sampling. The current embodiment of the invention utilizes a Gilson interface module for bidirectional communication between a computer and a probe manipulating arm or XYZ stage, and a fluid movement device. Software designed using commercial languages, such as C++, C#, Java, etc. may be used to control the speed and distance of probe motions in all 3 dimensions, the sensing of probe contact with liquid in a source well to assure reproducible sample volumes, and the speed of the fluid movement device. A computer or other known device may be used to control the autosampler or XYZ stage to regulate sample size and bubble size by varying the time that the probe is in a source well or above a source well. Also, various sample handlers, XYZ stages, and sampler handling systems that may be useful in the apparatus and method of the present invention are well known in the art.

[0088] In order to reduce sample carryover a rinsing station or device that may be attached to the autosampler to rinse the autosampler probe between intakes of sample and/or buffer solution. The rinsing fluid may be water, a mild detergent, or a solvent, such as a solvent in which each of the particles in one or more of the samples is dissolved. When the particles are merely suspended in a suspension fluid, the rinsing fluid may be the same as the suspension fluid.

[0089] Various conventional means may be employed to move the sample through the system. For example, peristaltic pumps or injection devices may be used with a particle analyzer such as a flow cytometer or an acoustic cytometry apparatus for the present invention. According to one embodiment, the peristaltic pump is a multi channel or head pump that accommodates up to 4 separate sample tubes leading to particle analyzers.

[0090] There are various types of tubing may be used for the fluid flow path of the present invention, as long as the tubing may function as high speed multi-sample tubing. When thin walled PVC (polyvinyl chloride) tubing is used as the tubing for the present invention, carryover between samples is substantially reduced compared to conventional peristaltic tubing.

[0091] Various types of flow cytometers may be used with the present invention. Commercially available flow cytometers from Becton Dickinson (FACSCalibur, FACSArray, FACSCantoII and LSRII), Beckman Coulter (CyAn) and Accuri Cytometers (C6) have all been proven compatible with embodiments of the current invention. The use of the real-time software in conjunction with flow cytometer controlling software may allow the samples from a given source well to be rapidly re-checked during sampling and data analysis to prove that "hits" from neighboring source wells do not arise from cross-contamination, or to identify hits for additional treatment or testing.

[0092] On-line data analysis may be used in the flow cytometer to compare data between well plates and facilitate overall utility of the data in conjunction with automation. Operation of the flow cytometer at higher pressure generally increases the sample flow rate and may, in some circumstances yield a higher throughput. Also, operation of the flow cytometer with increased time resolution in data software may allow resolution of samples at higher throughput rates.

[0093] Both peristaltic pumps and air bubbles have been used in a variety of detection devices with flowing samples. For example, bubbles are commonly used in clinical instruments to separate samples and the peristaltic pumps to move fluids. However, in flow cytometry there is specific teaching against air bubbles with the idea that, optimally, the bubbles should be removed from the sample prior to injection into the flow cytometer. However, in the current invention, carefully controlling the air bubble and using a temporal separation of the specimens to eliminate the air bubble from analysis, the introduction of air bubbles between samples has proven to have little or no effect on the quality of results.

[0094] Using the flow cytometry apparatus of the present invention, it has already been possible to move and analyze up to 40 samples per minute in a single channel (consisting of a probe, tube, peristaltic pump). In a preferred embodiment, utilizing multiple probes, 80 – 400 samples can be moved and analyzed per minute.

[0095] Among the advantages of the flow cytometer apparatus of the present invention is that it allows rapid sampling of small volumes of sample. For example, a sample drawn into the fluid stream tubing at a rate of about .3 ul/sec requires less than a 2 ul sample.

[0096] The throughput of the flow cytometry apparatus of the present invention tends to be more affected by the behavior of the autosampler rather than the characteristics of the fluid movement device, the tubing or the flow cytometer. Thus, to the extent that an autosampler can move more rapidly from source well to source well, higher throughputs are achieved. Improved accuracy in volume intake/delivery by the autosampler leads to smaller sample volumes and improved throughputs.

[0097] In another embodiment of the present invention, a plurality of samples are simultaneously picked up using a multichannel autosampler comprising a plurality of sampling probes and a plurality of sample delivery tubes. In this embodiment, a peristaltic pump or other sample moving device moves the plurality of samples in the delivery tubes through the pump simultaneously using a plurality of pump heads or injection devices thus providing a plurality of channels. By having a plurality of probes sampling a plurality of wells of a microplate simultaneously, each channel is delivered to a separate input port of a single particle analyzer or separate particle analyzer to enable each channel to be analyzed in parallel, thereby increasing sample throughput 100% for each channel added.

[0098] Although the invention has been described in detail with particular reference to these preferred embodiments, other embodiments can achieve the same results. Variations and modifications of the present invention will be obvious to those skilled in the art and it is intended to cover in the appended claims all such modifications and equivalents. For example, the arm **102** in figure 1 directs the movement of probe **104 a** independent of the movement of probes **104 b**, **104 c** or **104 d**. For embodiments where there are four probes illustrated, the invention is not limited thereto. For example, the invention may include two or more probes each attached to be a conduit leading to a separate particle analyzer or a multi-channel particle analyzer. A means for moving the fluid can be positioned before or after the particle analyzer or before the probes. The entire disclosures of all references, applications, patents, and publications cited above are hereby incorporated by reference.

What is claimed**1. A method for analyzing a plurality of samples, comprising:**

obtaining with an autosampler a plurality of samples from a first plate having a plurality of sample wells wherein the autosampler comprises a plurality of probes for sampling the plurality of samples and wherein each probe of the plurality of probes is in communication with a separate flow cytometer via a separate conduit;

moving the plurality of samples comprising particles into a fluid flow stream for each separate conduit;

separating adjacent ones of the plurality of samples from each other in the fluid flow stream by a separation gas, thereby forming a gas-separated fluid flow stream;

independently guiding the gas-separated fluid flow stream to and through each separate flow cytometer;

operating each separate flow cytometer to focus the gas-separated fluid flow stream and to selectively analyze the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through each separate flow cytometer.

2. The method of claim 1 wherein the first plate is positioned on a platform that is moveable in the xyz direction to bring the samples to the probes.

3. The method of claim 1 wherein the step of moving the plurality of samples are moved by a fluid moving device located before or after each separate flow cytometer.

4. The method of claim 1 wherein the fluid moving device is a multihead peristaltic pump.

5. The method of claim 1 wherein the step of moving is selected from moving with gravity, moving with suction, moving with pumping or moving with pushing.

6. The method of claim 1 wherein the separate conduit is tubing.

7. The method of claim 1 wherein the probes are positionable to the samples on the first plate.

8. The method of claim 1 wherein at least one of the probes of the plurality of probes is positionable to a sample on a second plate.

9. The method of claim 1 wherein the step of moving the plurality of fluid samples streams is at a rate that is independently controlled.

10. A method for analyzing a plurality of samples, comprising:

obtaining with an autosampler a plurality of samples from a first plate having a plurality of sample wells wherein the autosampler comprises a plurality of probes for sampling a set of samples and wherein each probe of the plurality of probes is in communication with a multi-channel flow cytometer via a separate conduit attached to each of the probes of the plurality of probes;

moving the plurality of samples comprising particles into a fluid flow stream for each separate conduit;

separating adjacent ones of the plurality of samples from each other in the fluid flow stream by a separation gas, thereby forming a gas-separated fluid flow stream;

independently guiding the gas-separated fluid flow stream to and through the multi-channel flow cytometer;

operating the multi-channel flow cytometer to focus the gas-separated fluid flow stream and to selectively analyze the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through the multi-channel flow cytometer.

11. The method of claim 10 wherein the first plate is positioned on a platform that is moveable in the xyz direction to bring the samples to the probes.

12. The method of claim 10 wherein the step of moving the plurality of samples is with a fluid moving device located before or after the multi-channel flow cytometer.

13. The method of claim 12 wherein the fluid moving device is a multihead peristaltic pump.

14. The method of claim 10 wherein the step of moving is selected from moving with gravity, moving with suction, moving with pumping or moving with pushing.

15. The method of claim 10 wherein the separate conduit is tubing.

16. The method of claim 10 wherein the first plate is positioned on a platform that is moveable in the xyz direction to bring the samples to the probes.

17. The method of claim 10 wherein the plurality of probes are positionable and move to the samples on the first plate.

18. The method of claim 10 wherein at least one of the probes of the plurality of probes is positionable and moves to a plurality of samples located on a second plate.

19. The method of claim 10 wherein the step of moving the plurality of fluid samples streams is at a rate that is independently controlled.

20. A flow cytometry apparatus comprising:

an autosampler comprising a plurality of probes with each probe suitable for inserting a plurality of samples comprising particles from a plurality of respective source wells into a separate fluid flow stream;

a plurality of flow cytometers in communication with the plurality of probes of the autosampler via a separate conduit connecting a probe of the plurality of probes with a separate flow cytometer of the plurality of flow cytometers; and

moving the plurality of samples in each separate fluid flow streams through each separate conduit to a selected flow cytometer of the plurality of flow cytometers, the plurality of probes introducing aliquots of a separation fluid between successive ones of the plurality of samples in each of the separate fluid flow stream to configure each of the separate fluid flow streams as a gas-separated fluid flow stream, each of the plurality of flow cytometers focusing the gas-separated fluid flow stream delivered by the separate conduit and selectively analyzing the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through each separate cytometer of the plurality of cytometers.

21. The apparatus of claim 20 wherein the plurality of probes are positioned on an arm.

22. The apparatus of claim 20 wherein the plurality of probes are positionable relative to the plate.

23. The apparatus of claim 21 wherein the arm is fixed relative to the position of the plate.

24. The apparatus of claim 20 wherein the probes are independently positionable relative to each other.

25. The apparatus of claim 20 further comprising a fluid movement device.

26. The apparatus of claim 25 wherein the fluid movement device is a pump.

27. The apparatus of claim 25 wherein the fluid movement device is positioned before or after a flow cytometer.

28. The apparatus of claim 26 wherein the pump is a peristaltic pump.

29. The apparatus of claim 20 wherein the step of moving is selected from pumping, pushing, suctioning or moving with gravity.

30. The apparatus of claim 29 wherein the fluid movement device comprises a plurality of fluid movement devices each associated with the separate conduit.

31. A flow cytometry apparatus comprising:

an autosampler comprising a plurality of probes for inserting a plurality of samples comprising particles from a plurality of respective source wells into a plurality of fluid flow streams;

a multi-channel flow cytometer in communication with the plurality of probes of the autosampler via a plurality of separate conduits connected to one each of the probes of the plurality of probes wherein each of the separate conduits of the plurality moves a separate fluid flow stream of the plurality of fluid flow streams; and

moving the plurality of samples in each of the separate fluid flow streams moving in each separate conduit to the multi-channel flow cytometer, the autosampler introducing aliquots of a separation fluid between successive ones of the plurality of samples in the fluid flow stream to configure the fluid flow stream as a gas-separated fluid flow stream, the multi-channel flow cytometer focusing the gas-separated fluid flow stream delivered by the conduit from the autosampler and selectively analyzing the particles in each of the plurality of samples as the gas-separated fluid flow stream passes through the multi-channel flow cytometer.

32. The apparatus of claim 31 wherein the plurality of probes are positioned on an arm.

33. The apparatus of claim 31 wherein the plurality of probes are positionable relative to the plurality of respective source wells.

34. The apparatus of claim 32 wherein the arm is fixed relative to the plurality of respective source wells.

35. The apparatus of claim 31 wherein the probes are independently positionable relative to each other and the plurality of respective source wells.
36. The apparatus of claim 31 further comprising a fluid movement device.
37. The apparatus of claim 36 wherein the fluid movement device is a pump.
38. The apparatus of claim 37 wherein the pump is positioned before or after the multi-channel flow cytometer.
39. The apparatus of claim 37 is a peristaltic pump.

FIG. 1

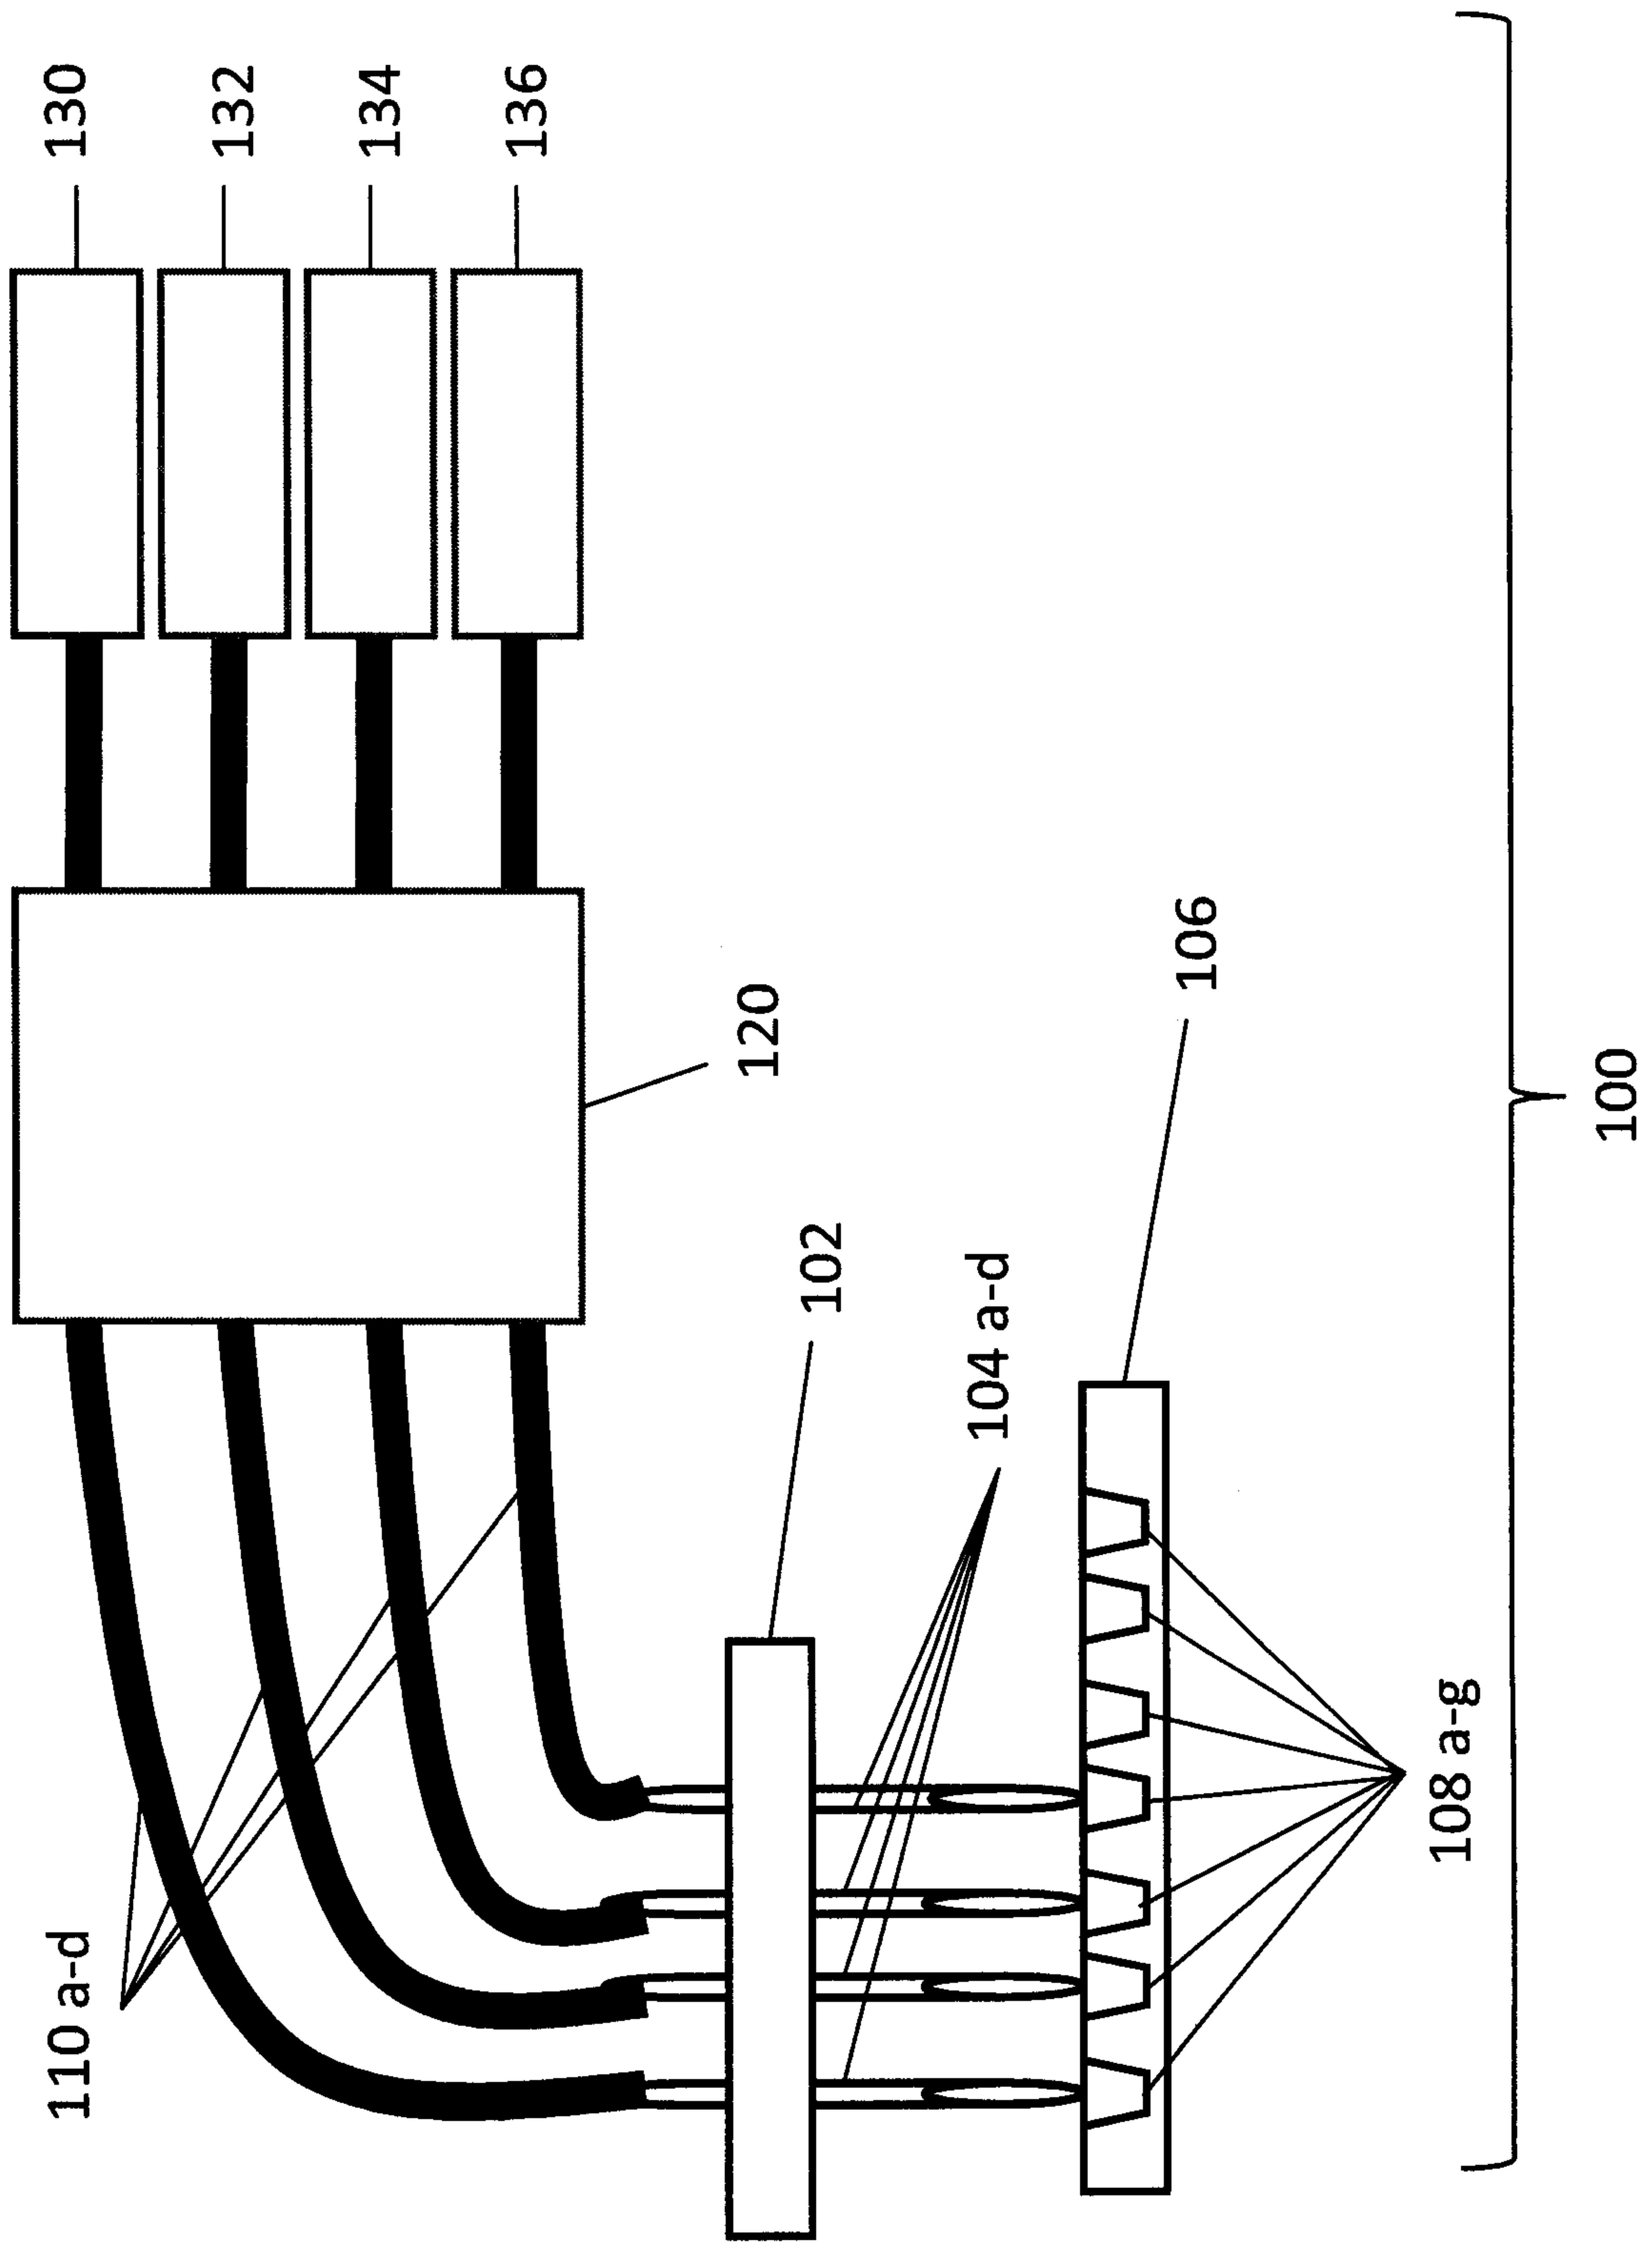


FIG. 2

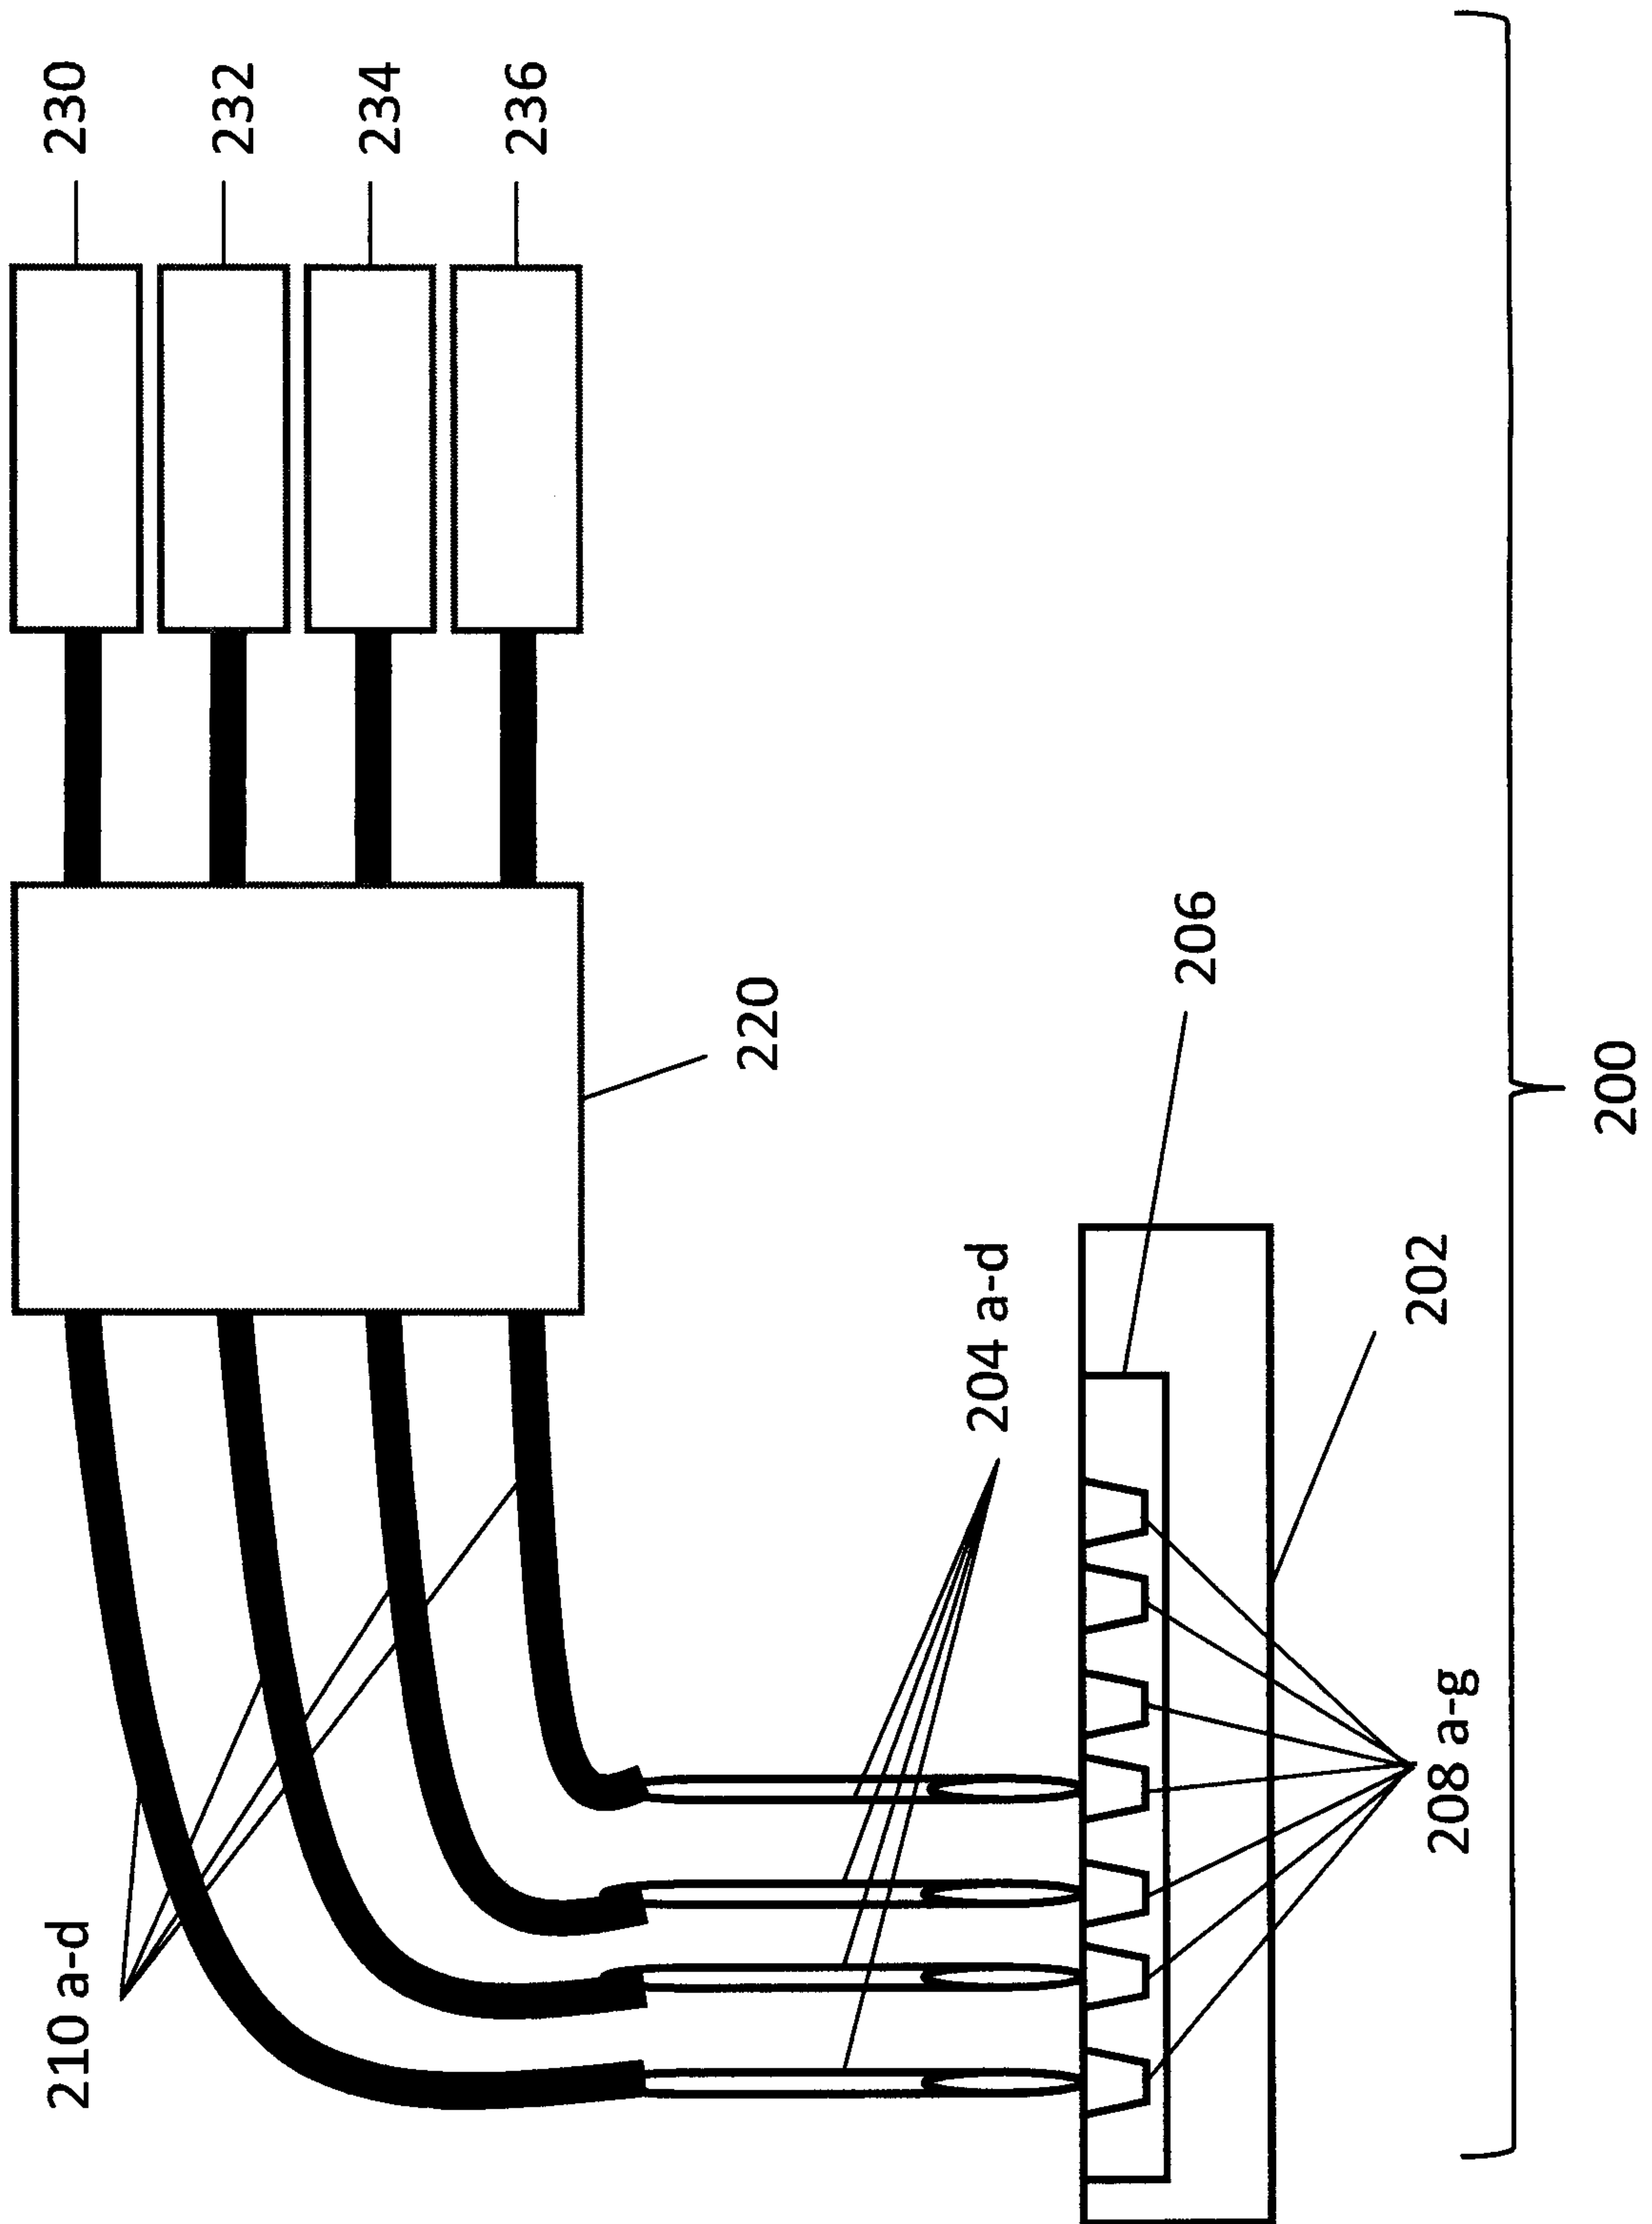
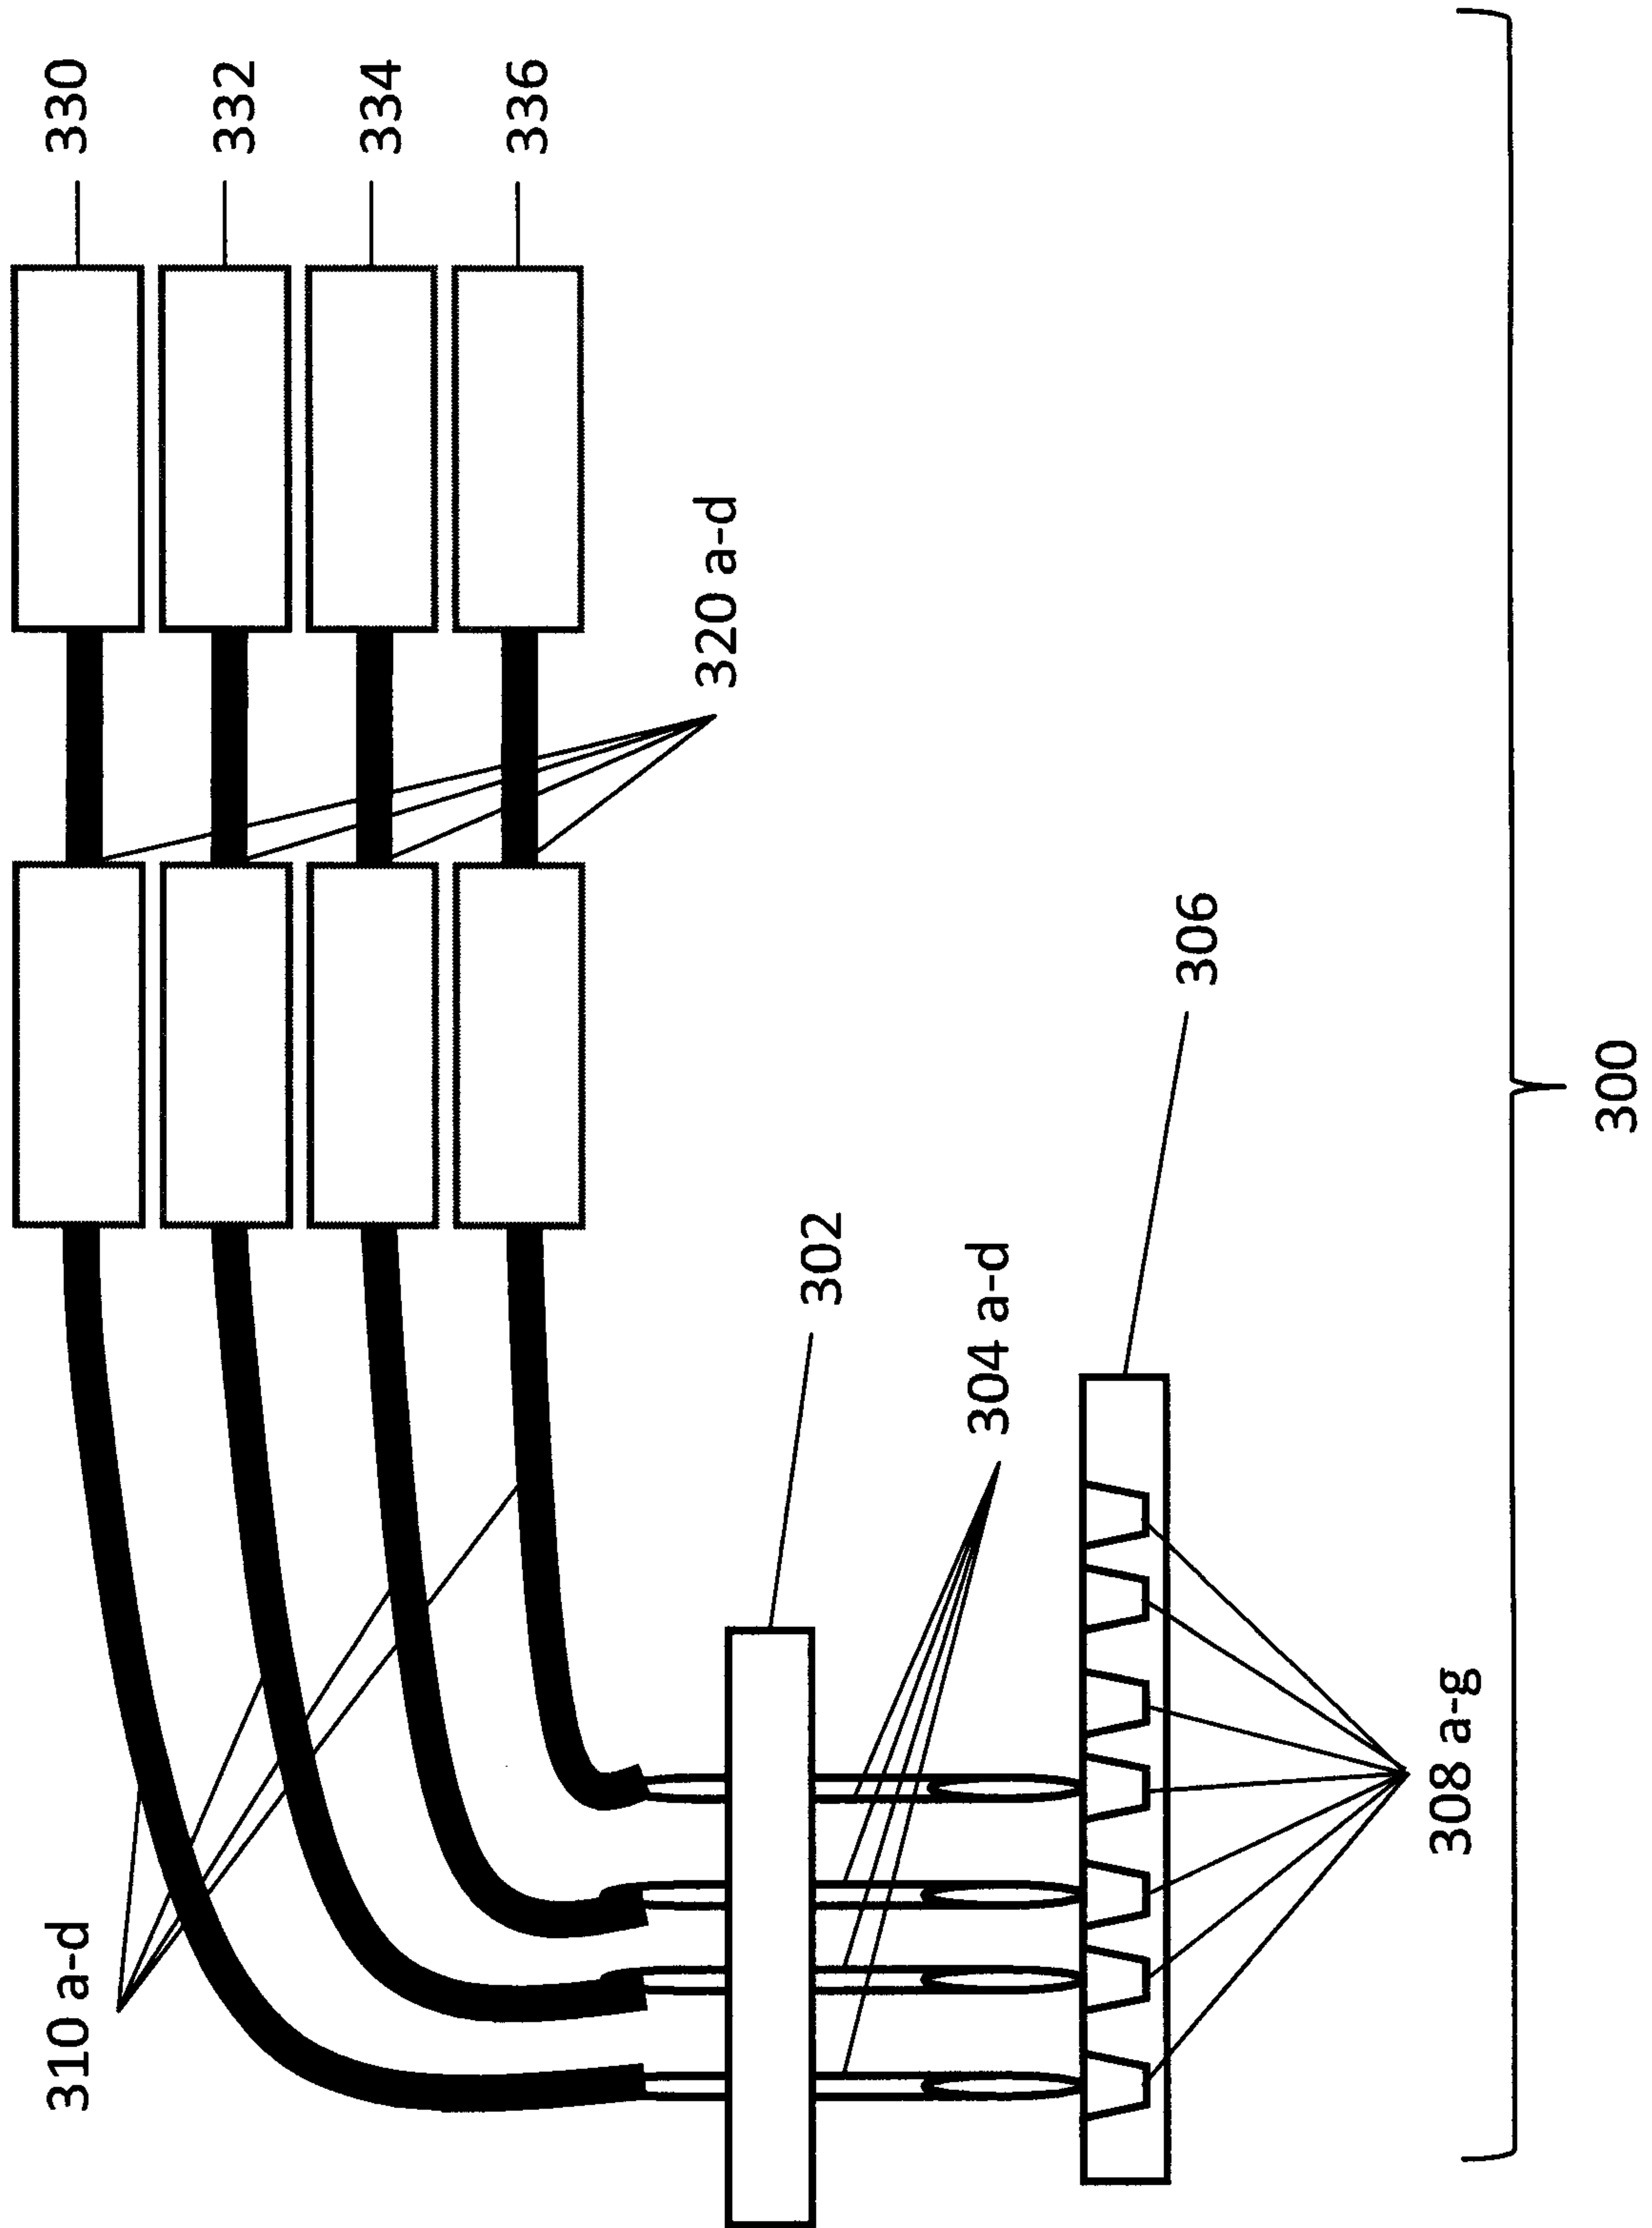


FIG. 3



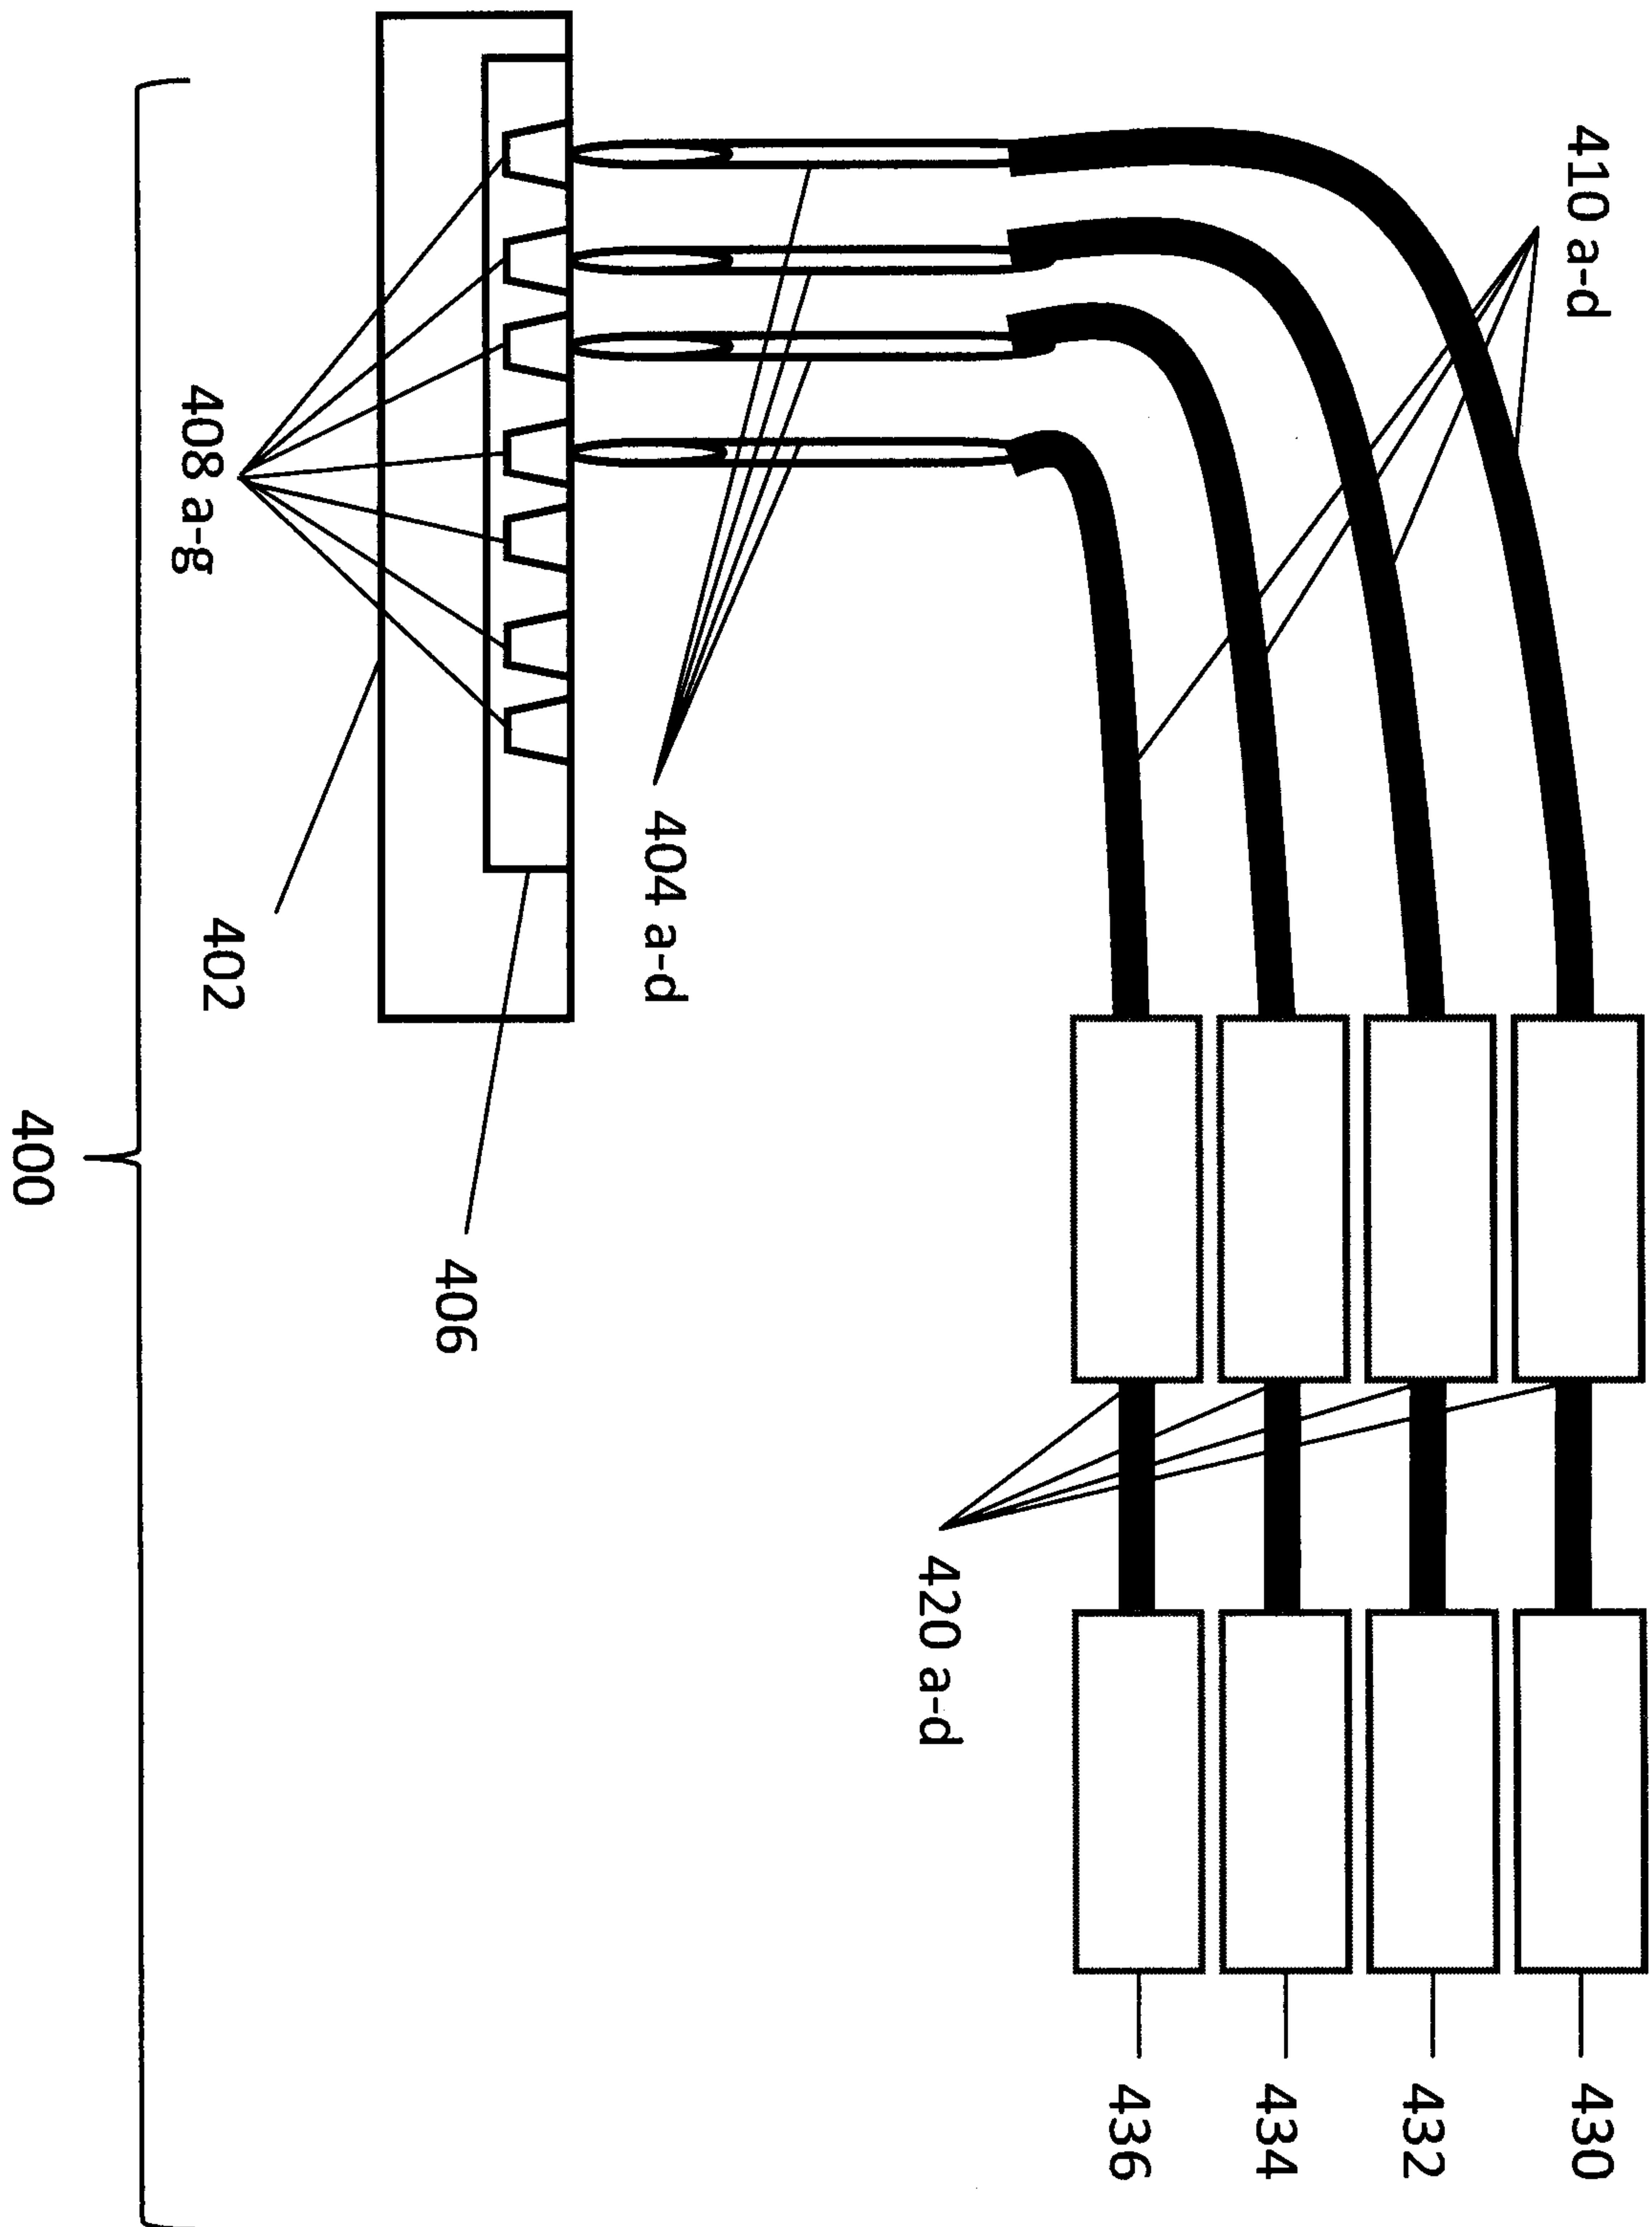


FIG. 4

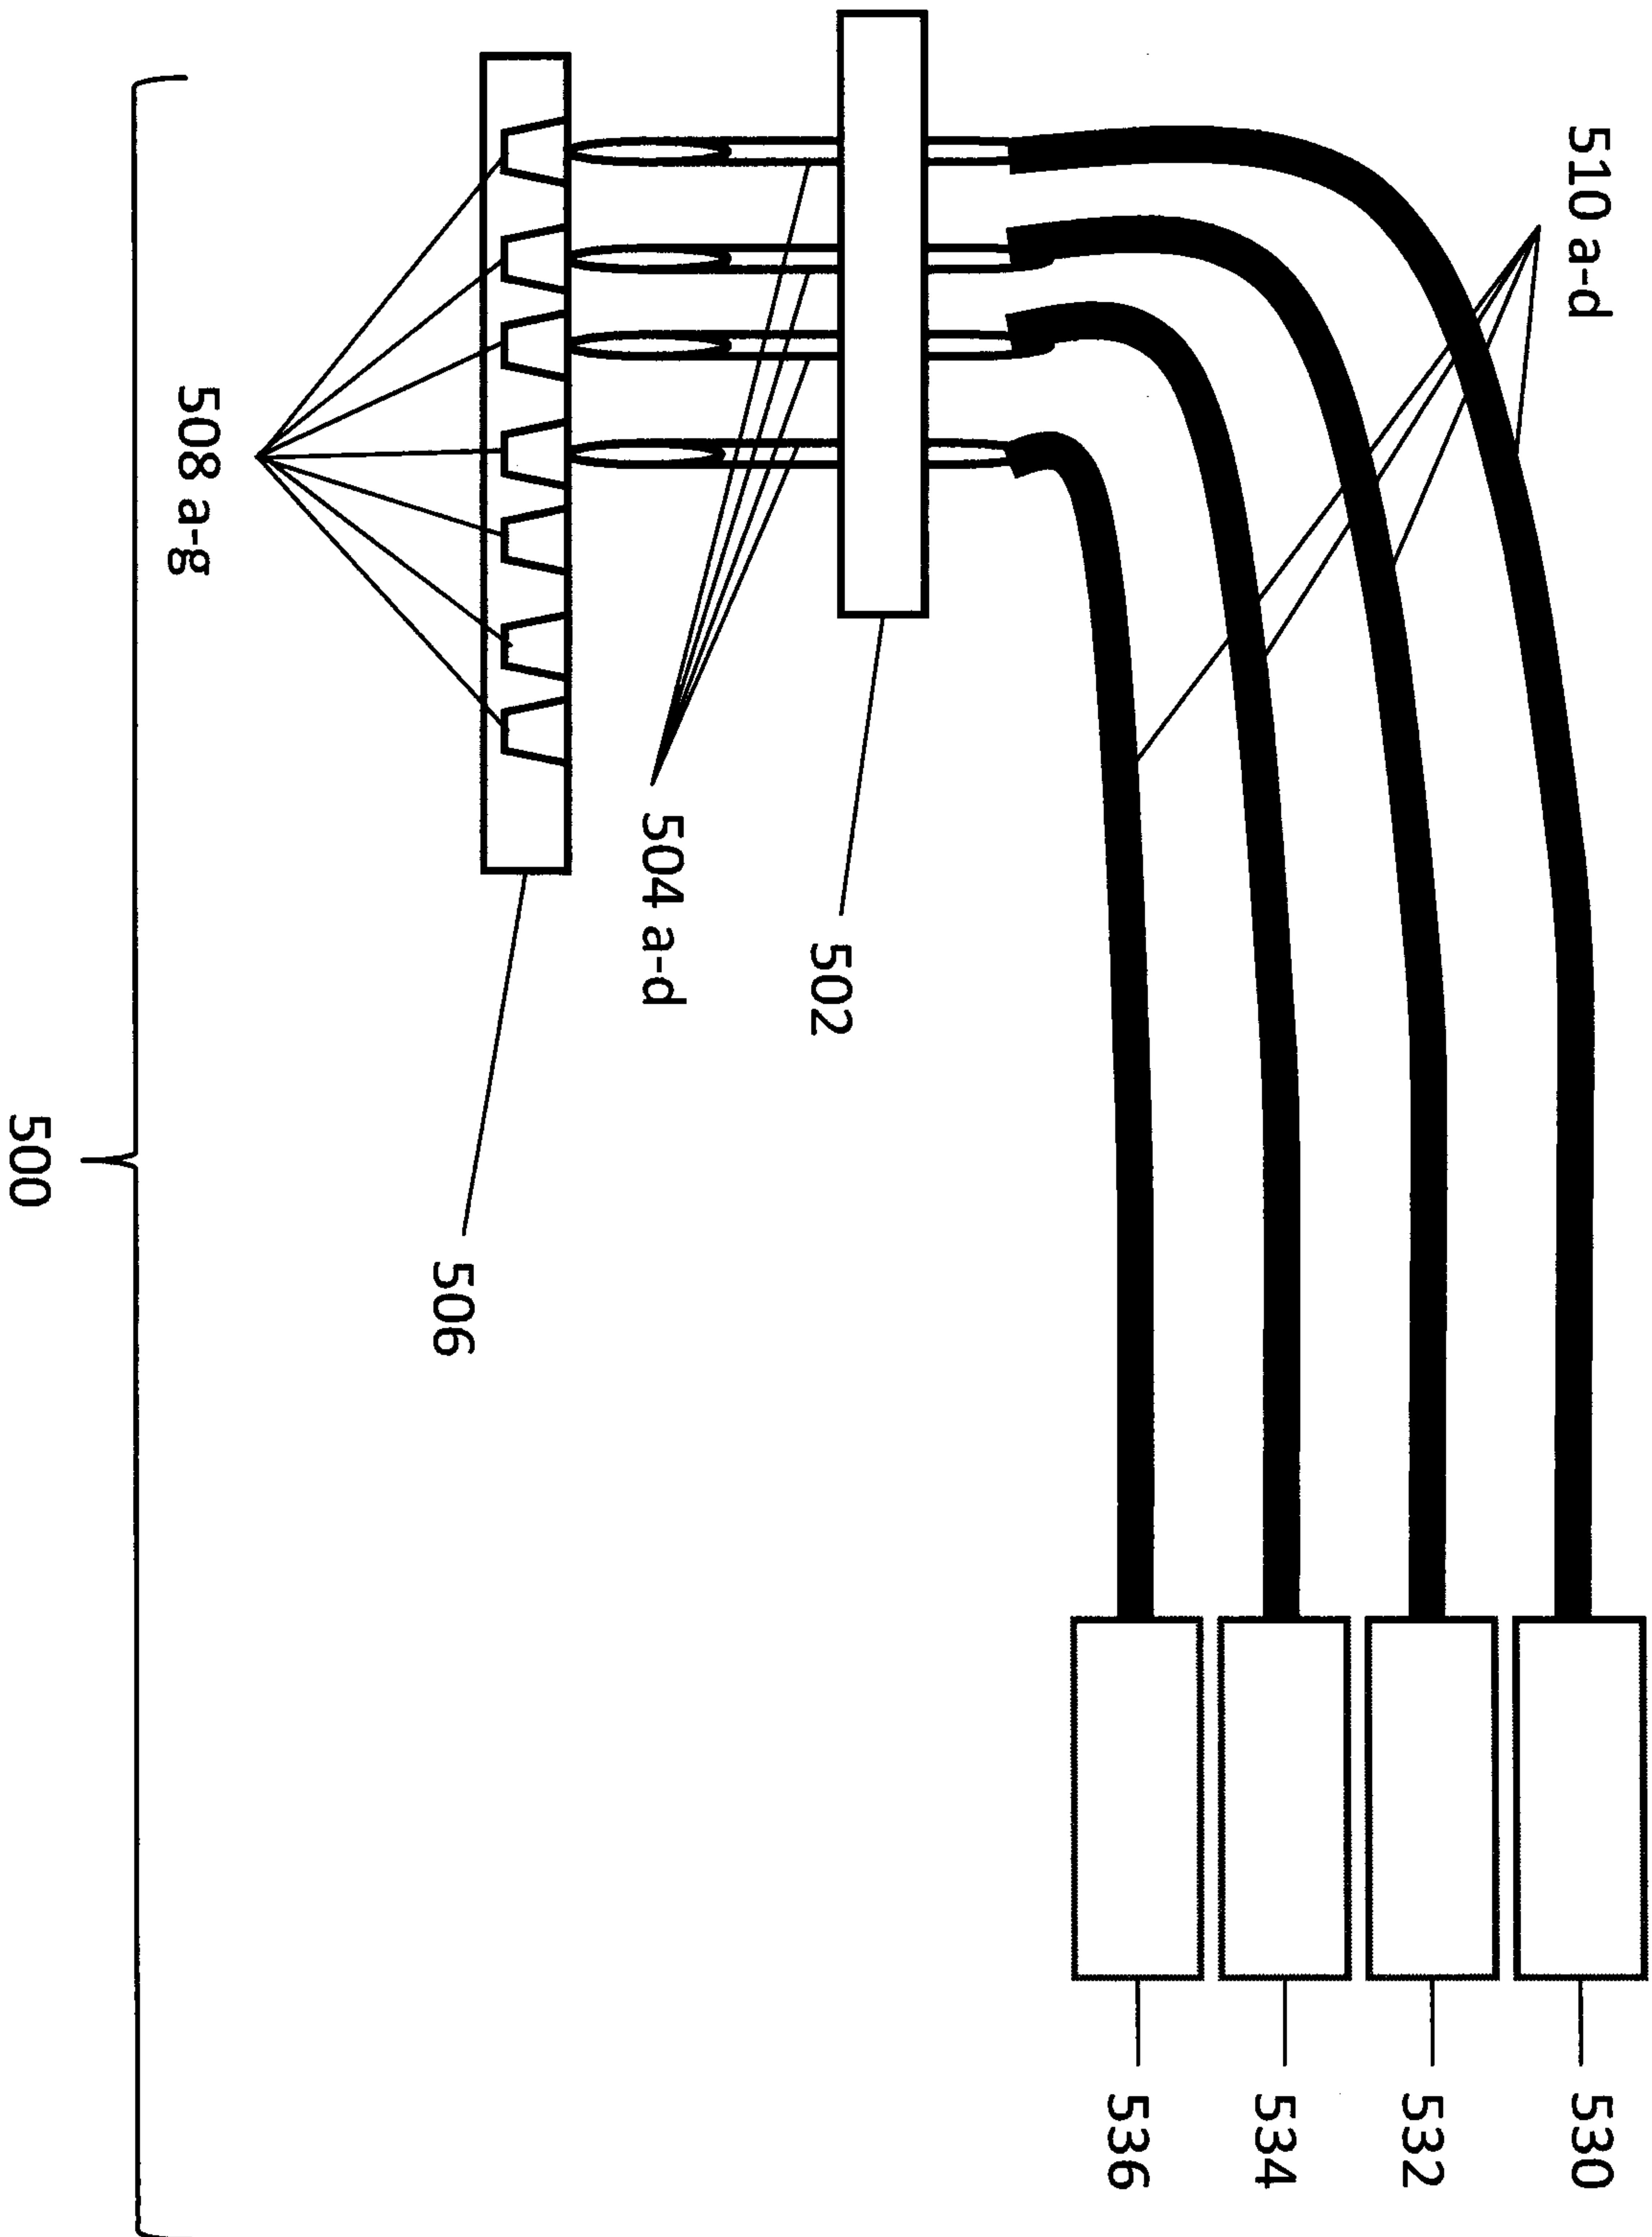


FIG. 5

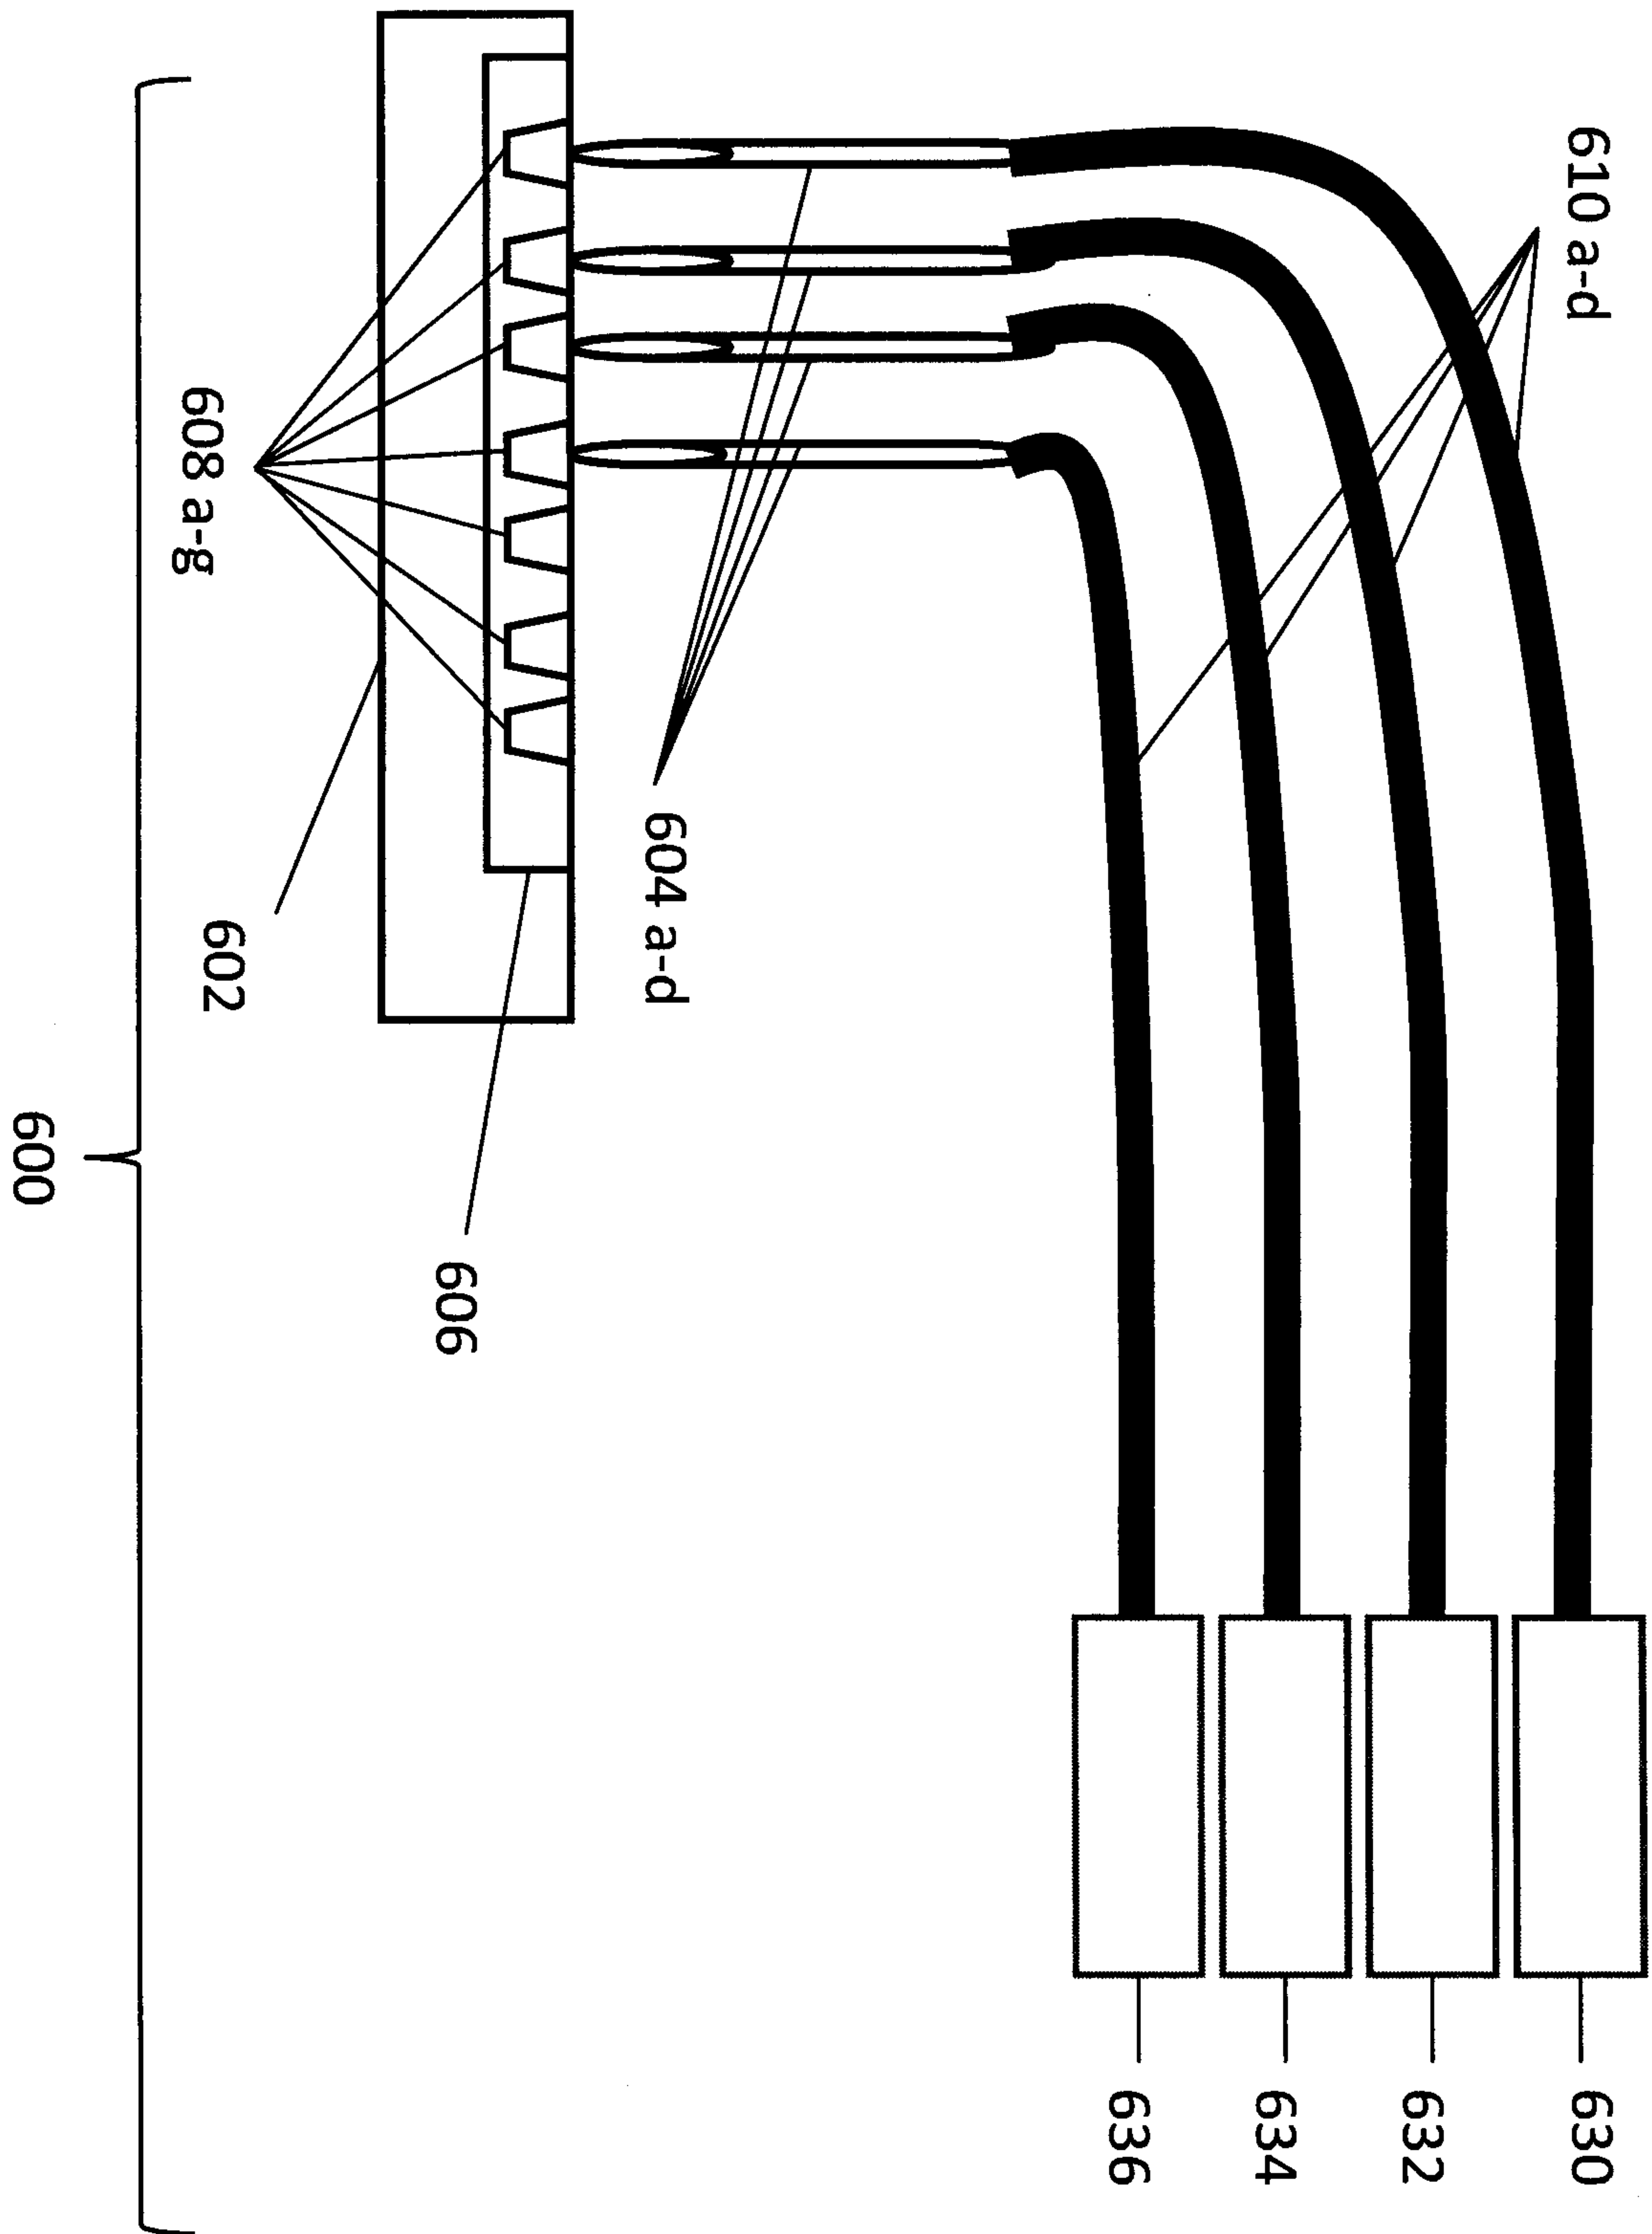
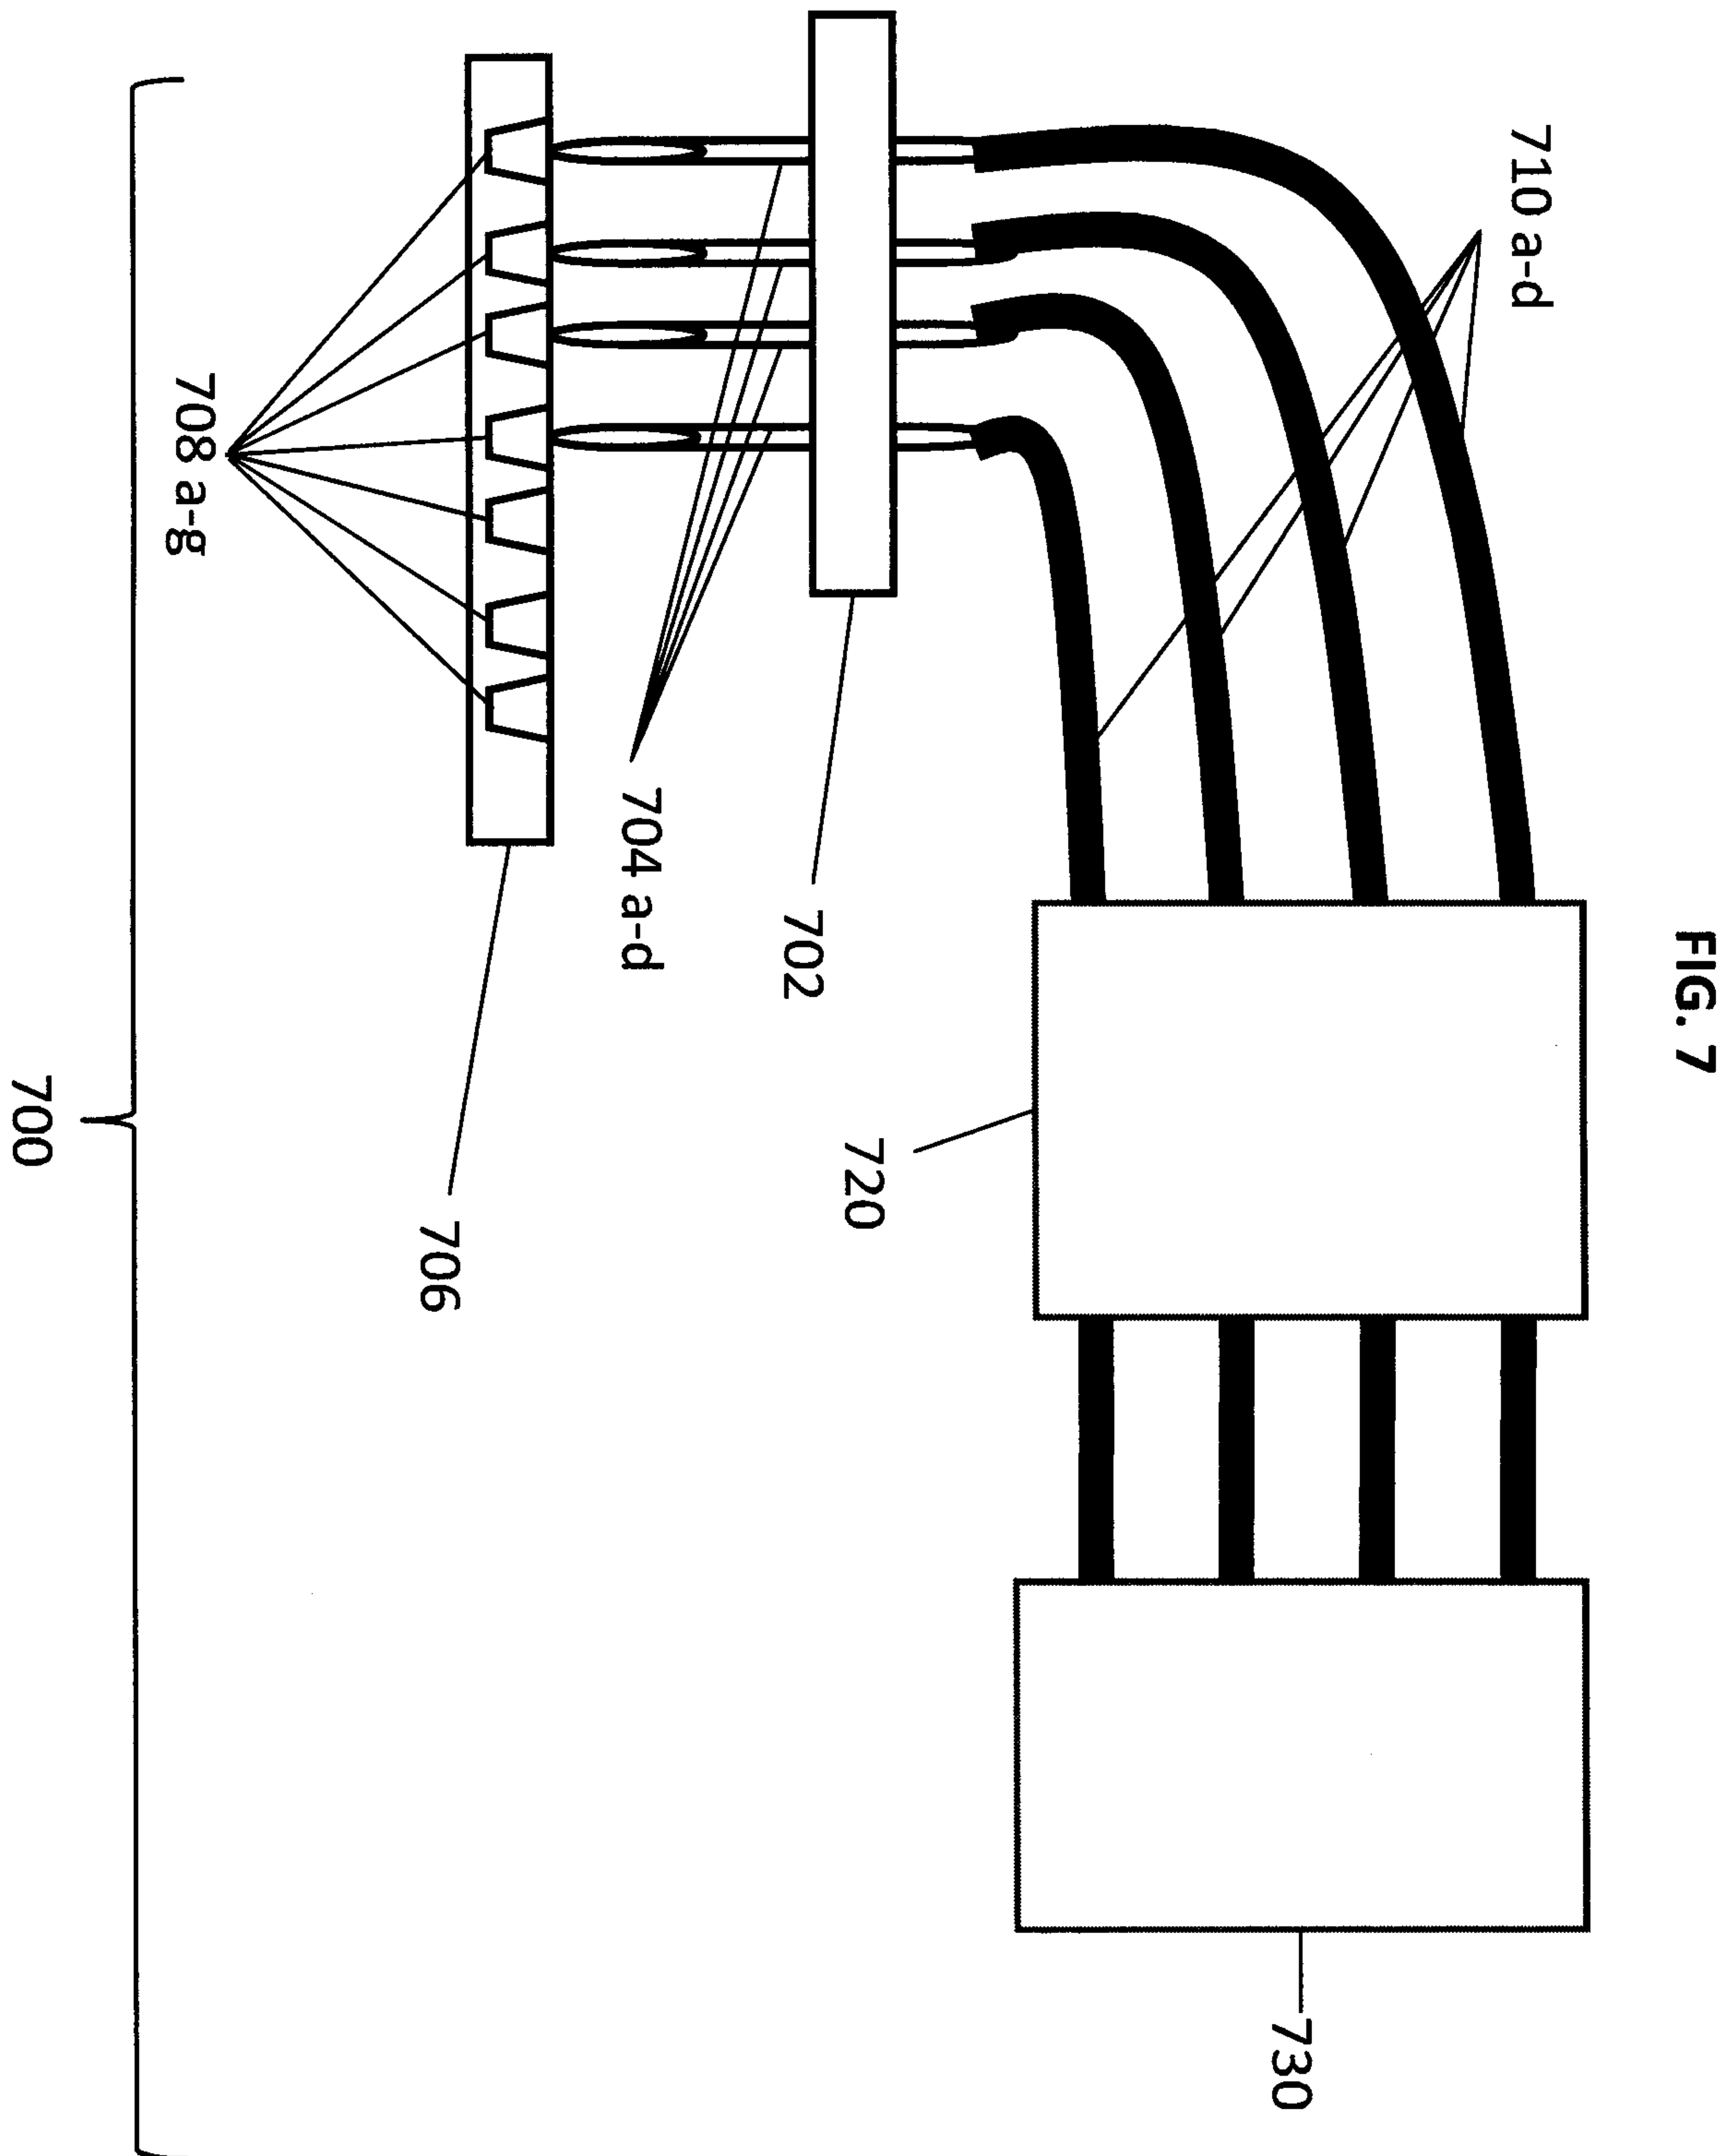
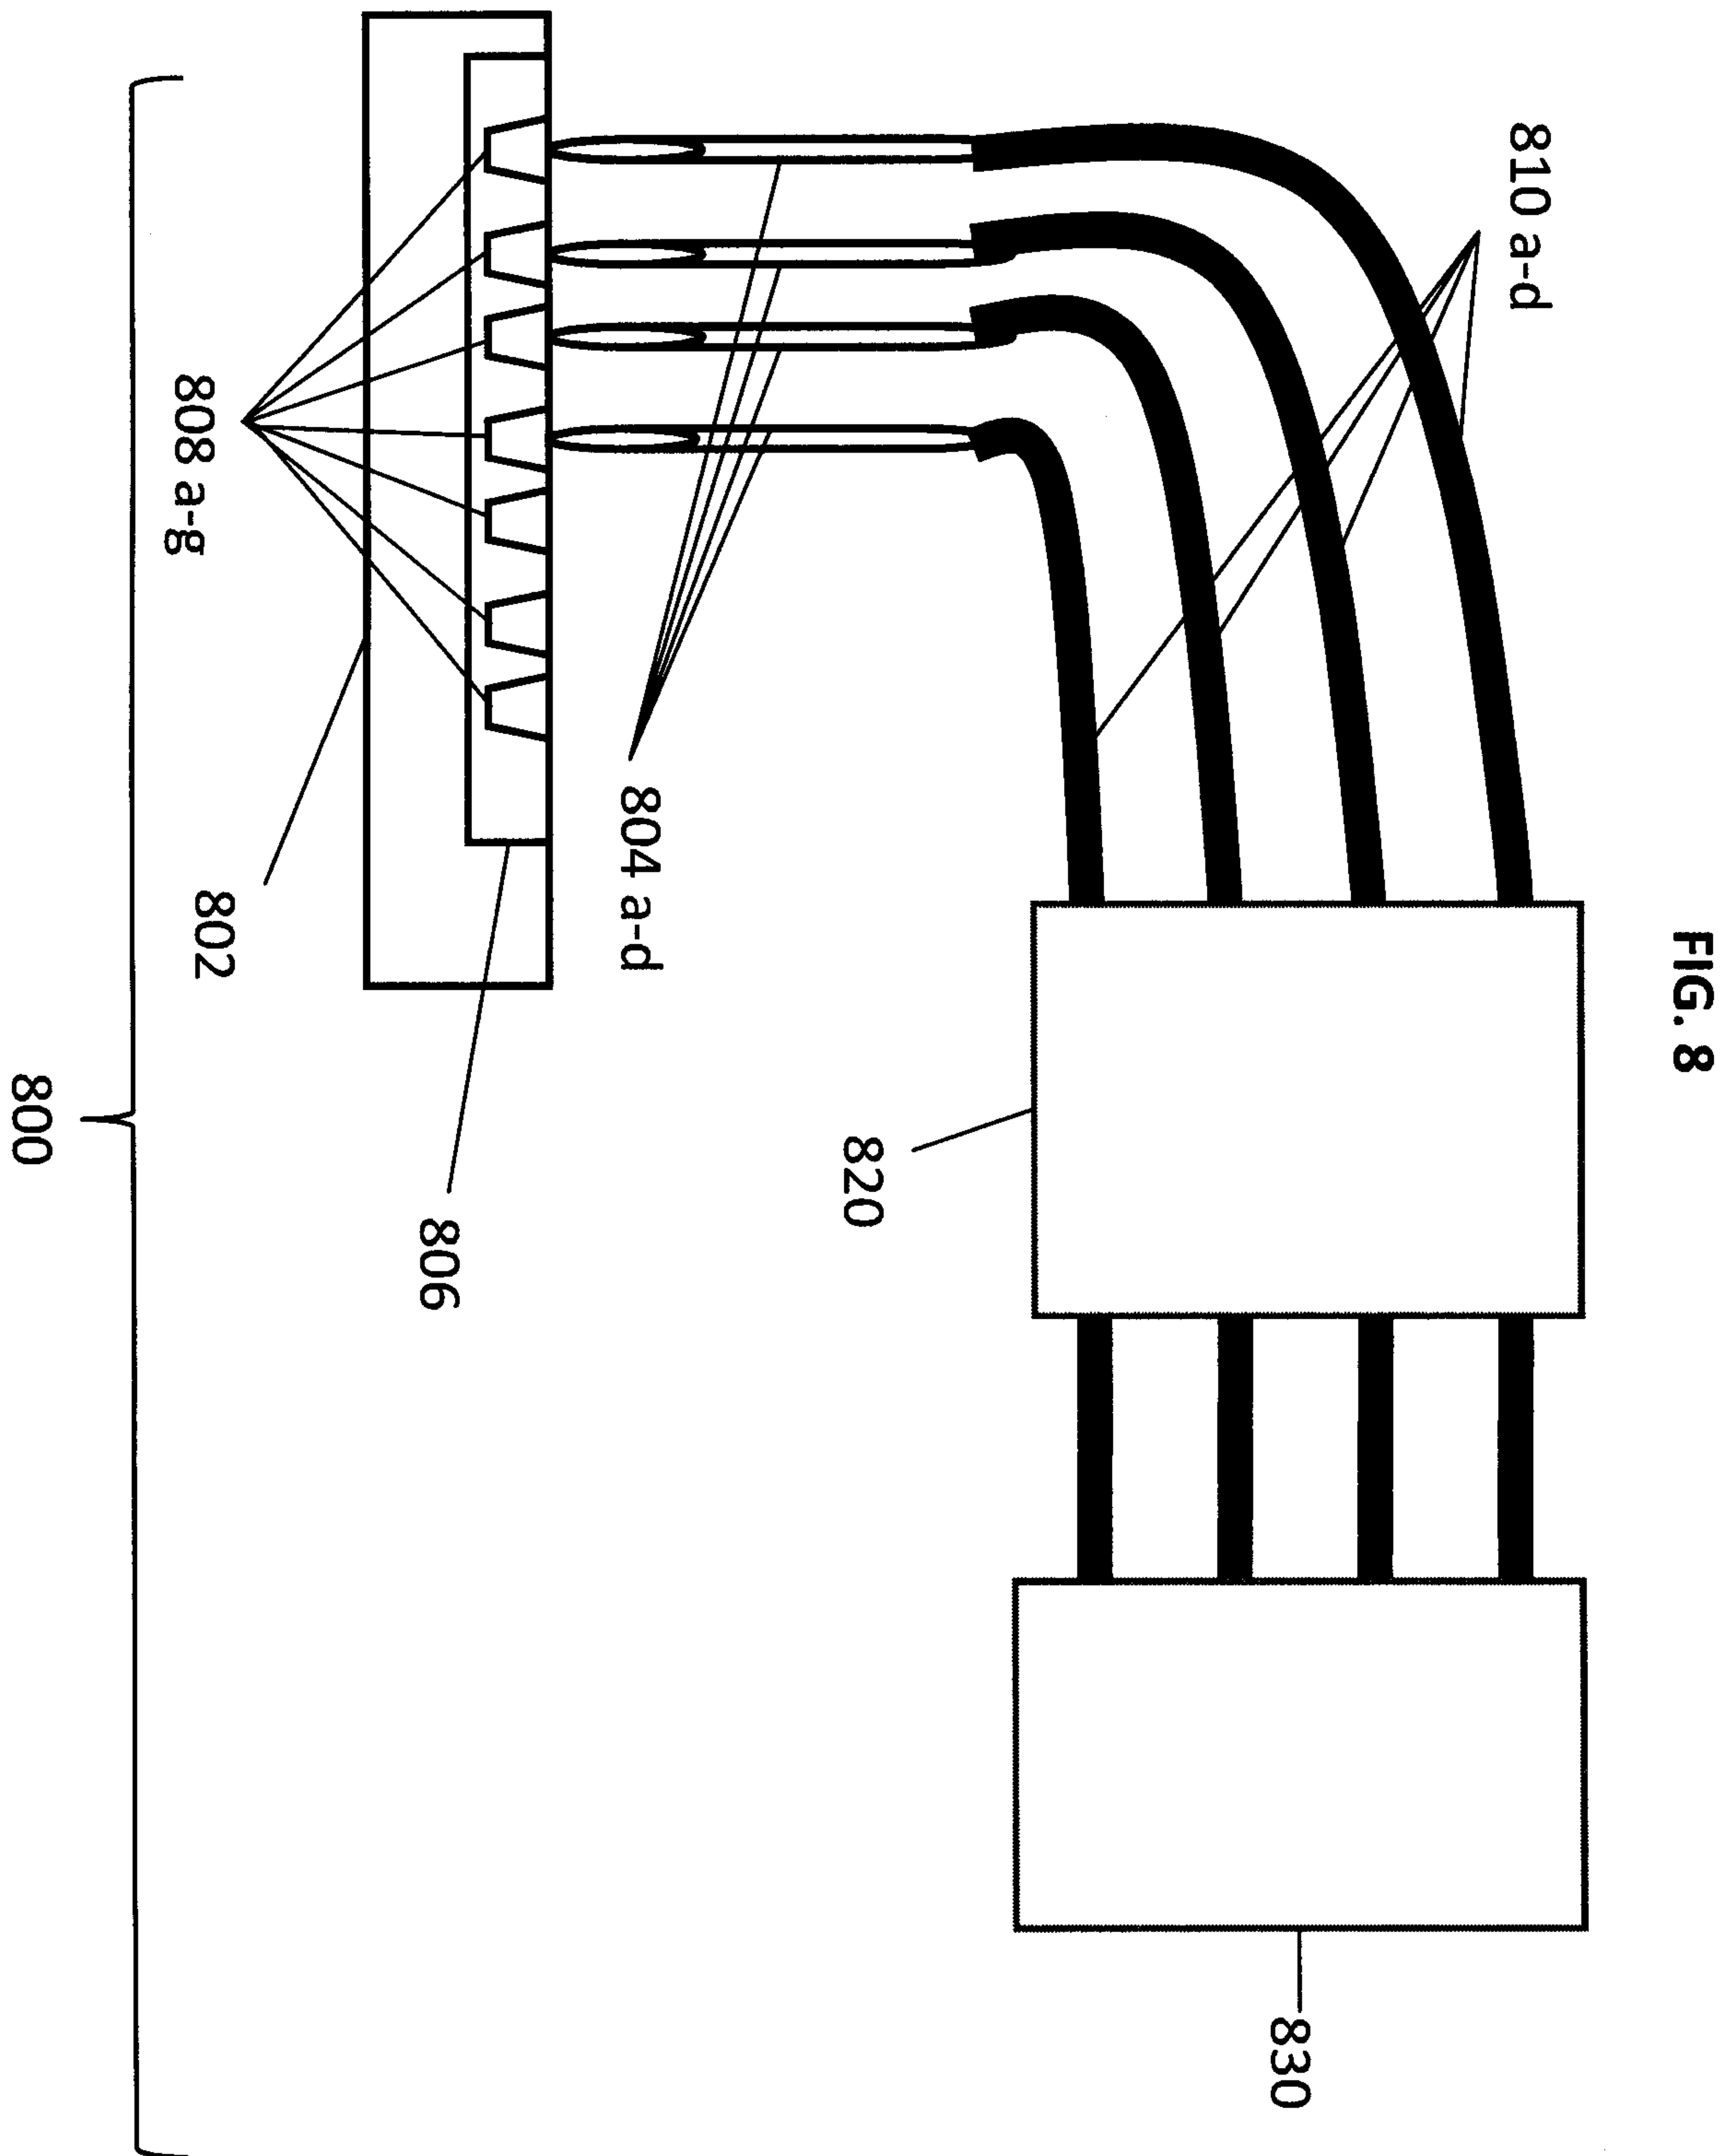


FIG. 6





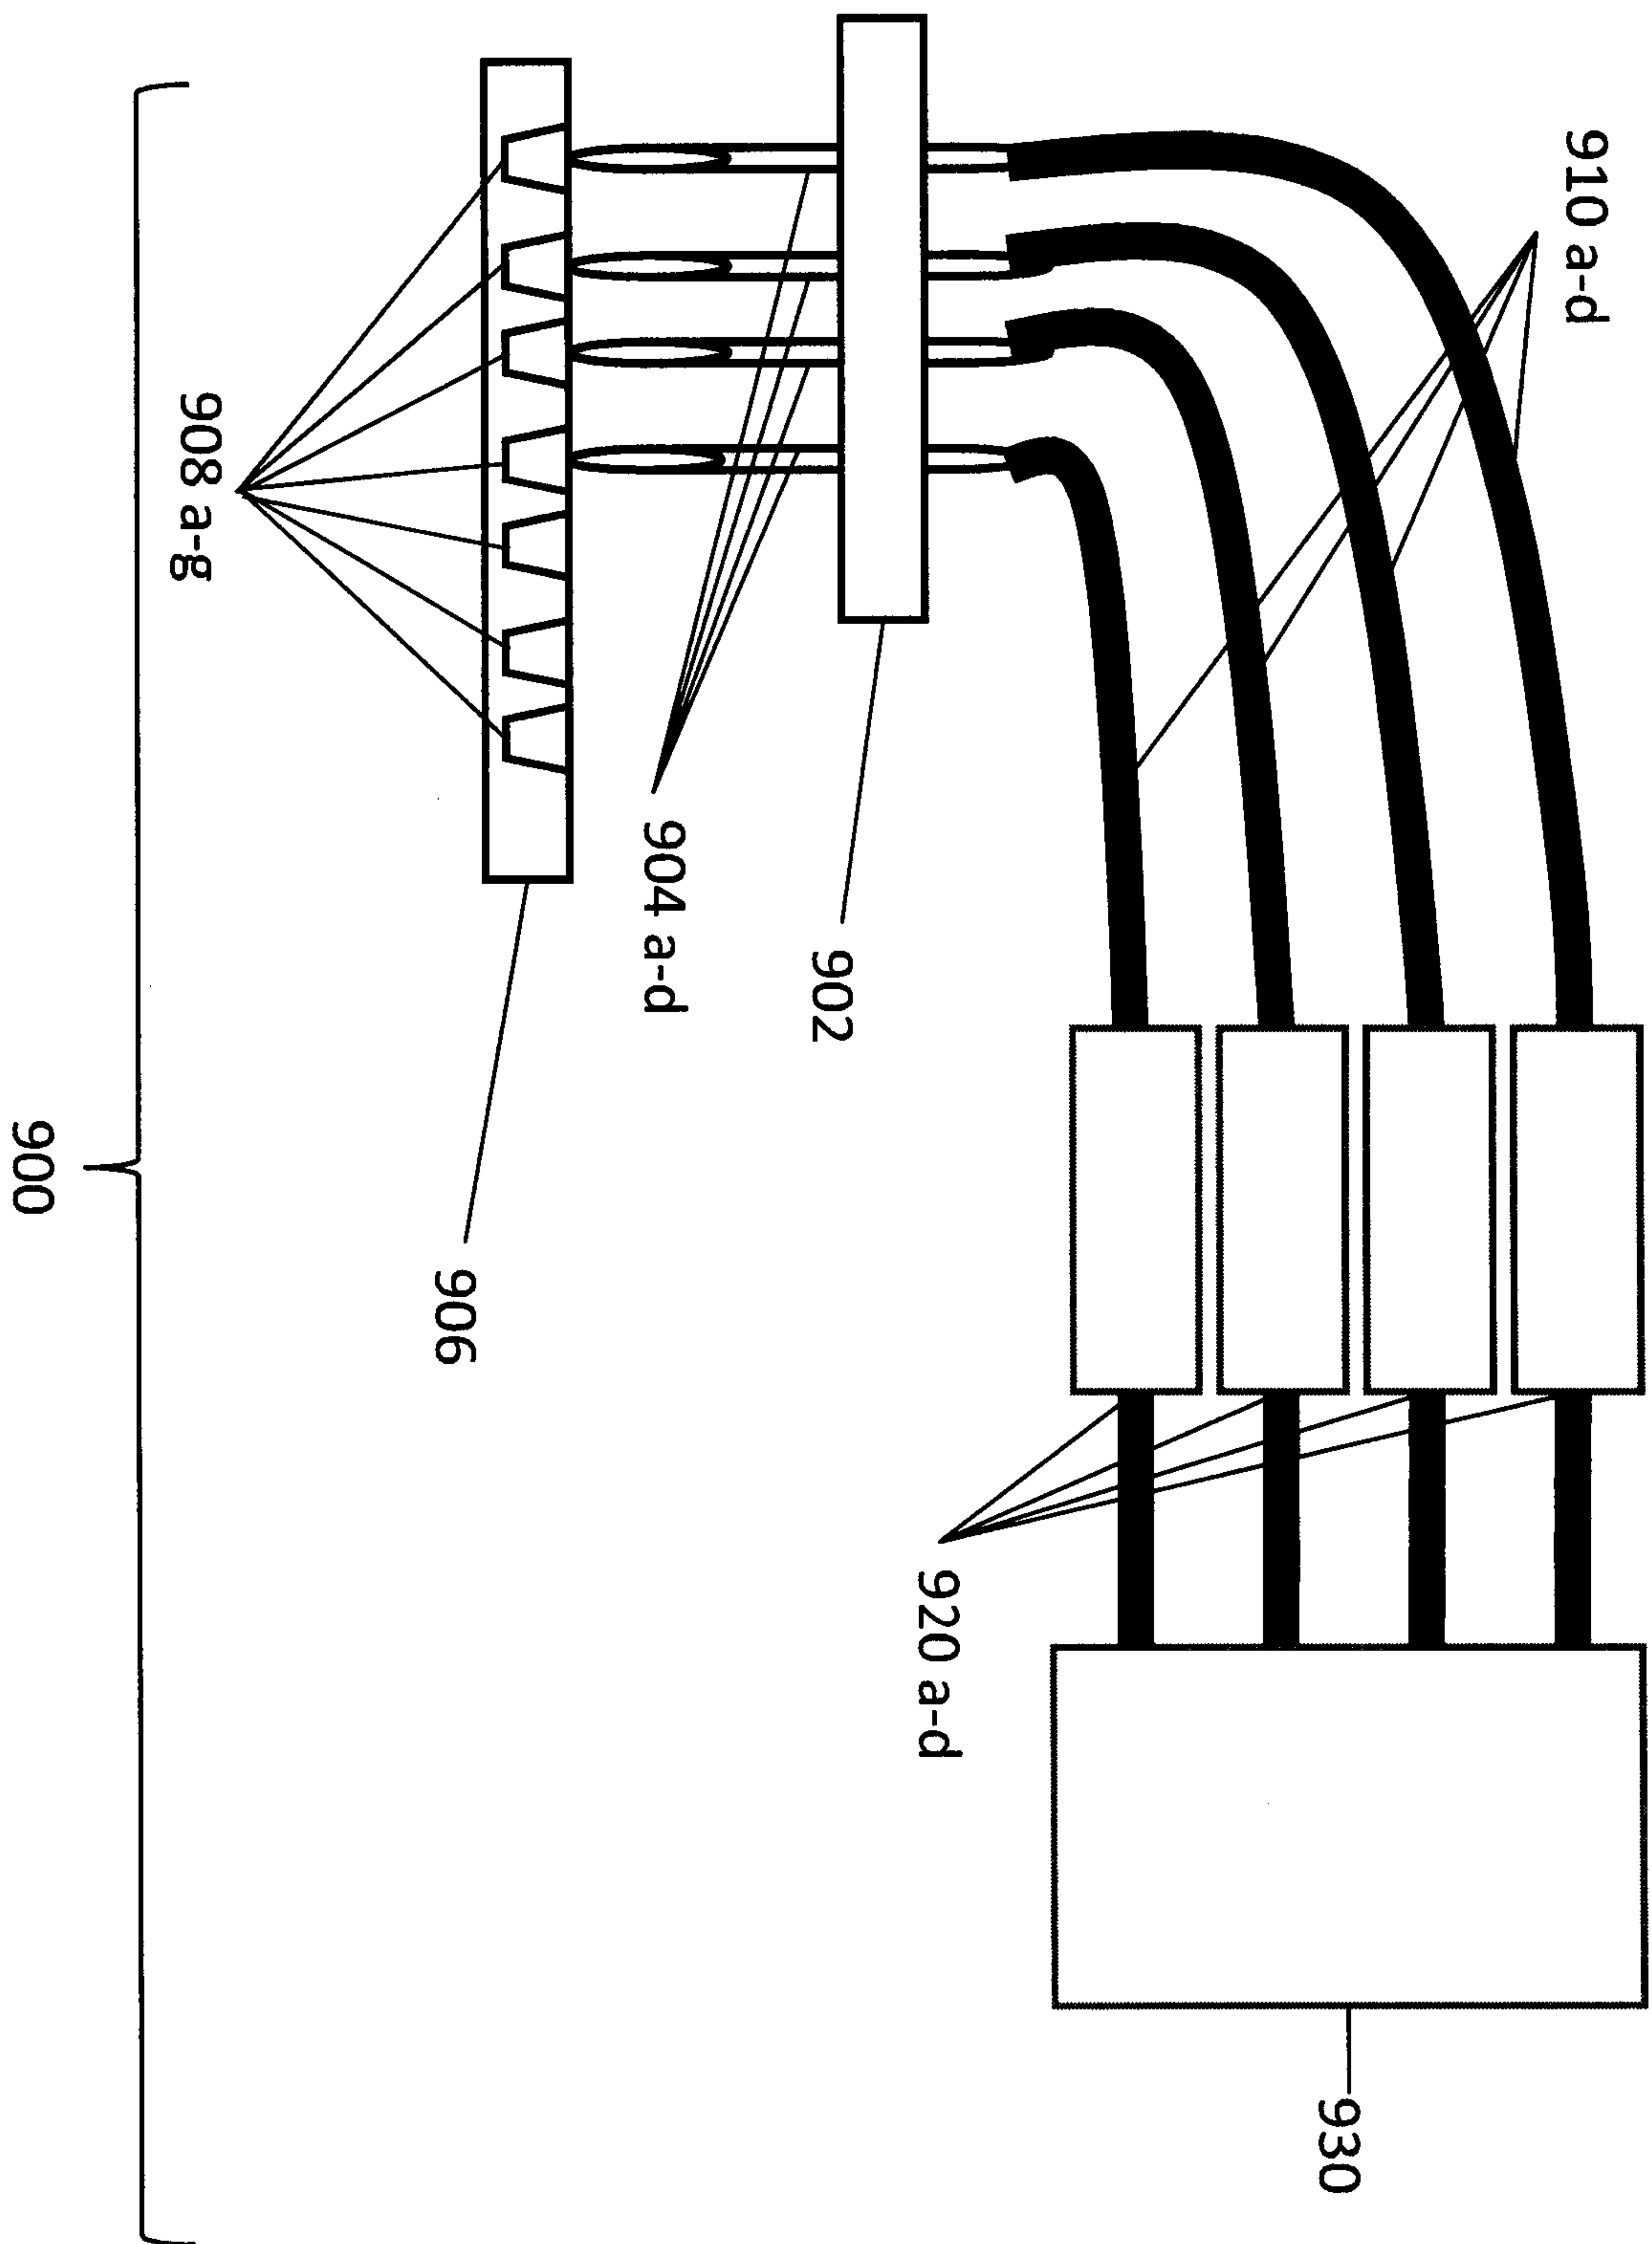


FIG. 9

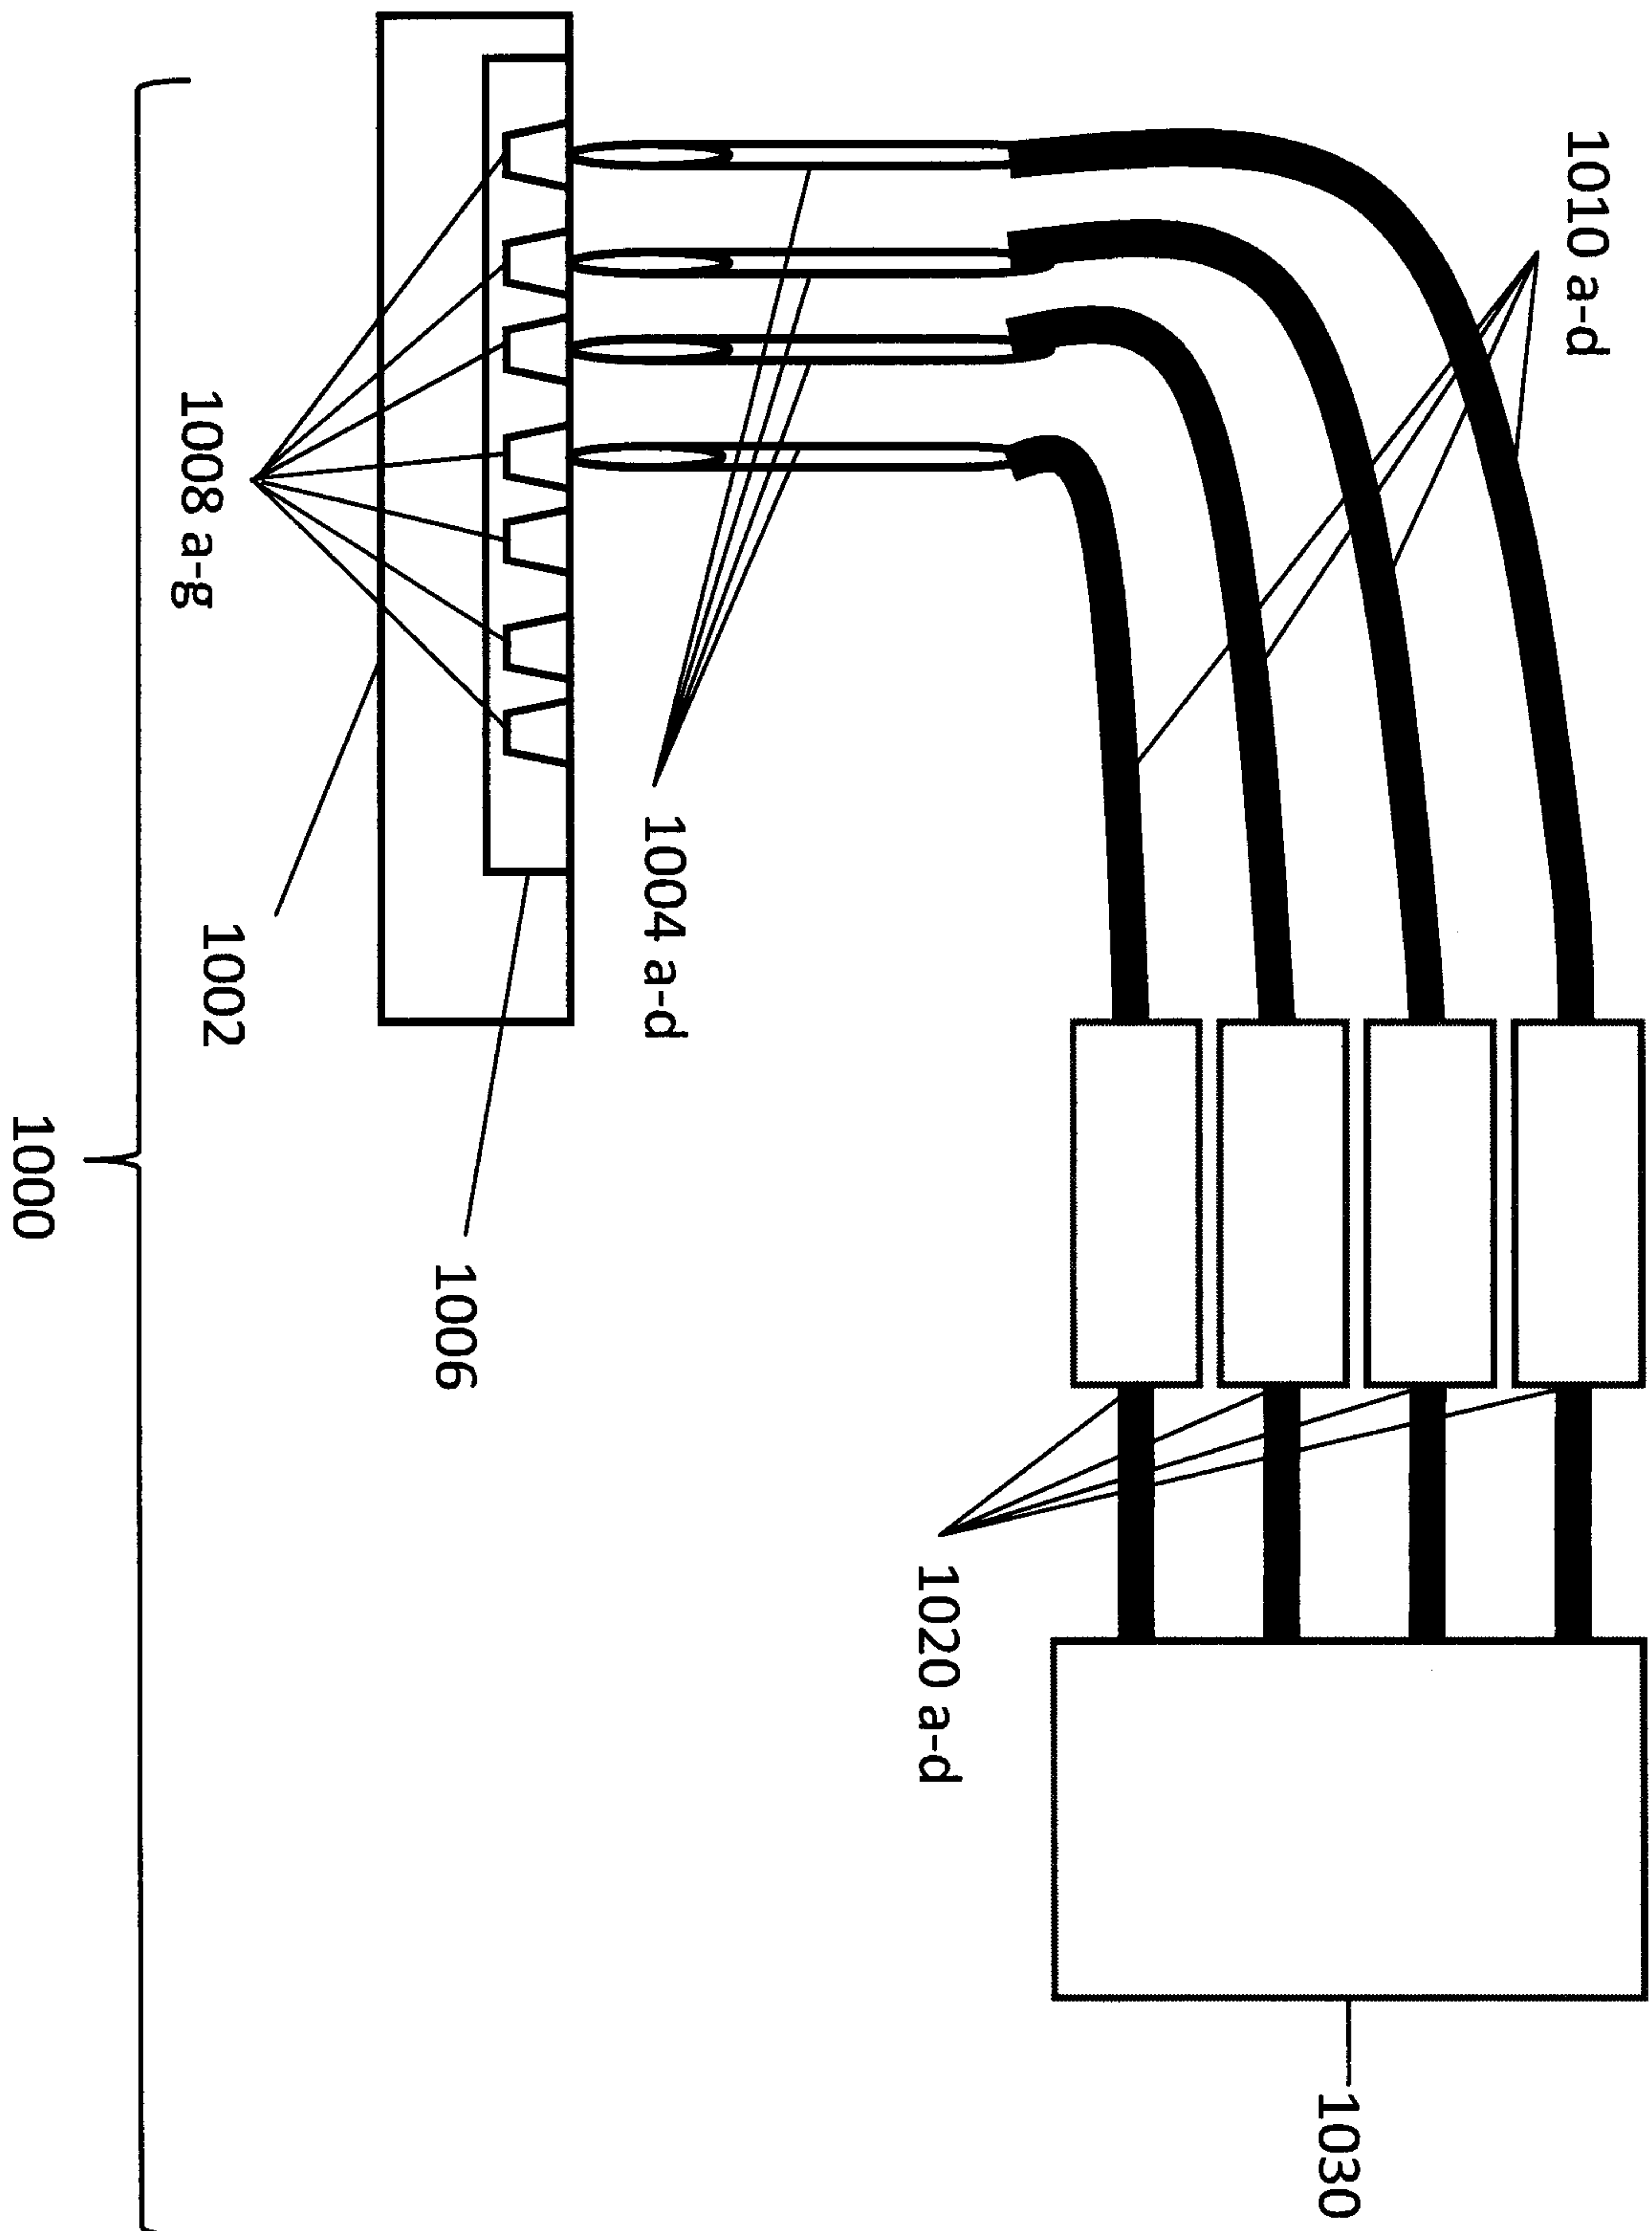


FIG. 10

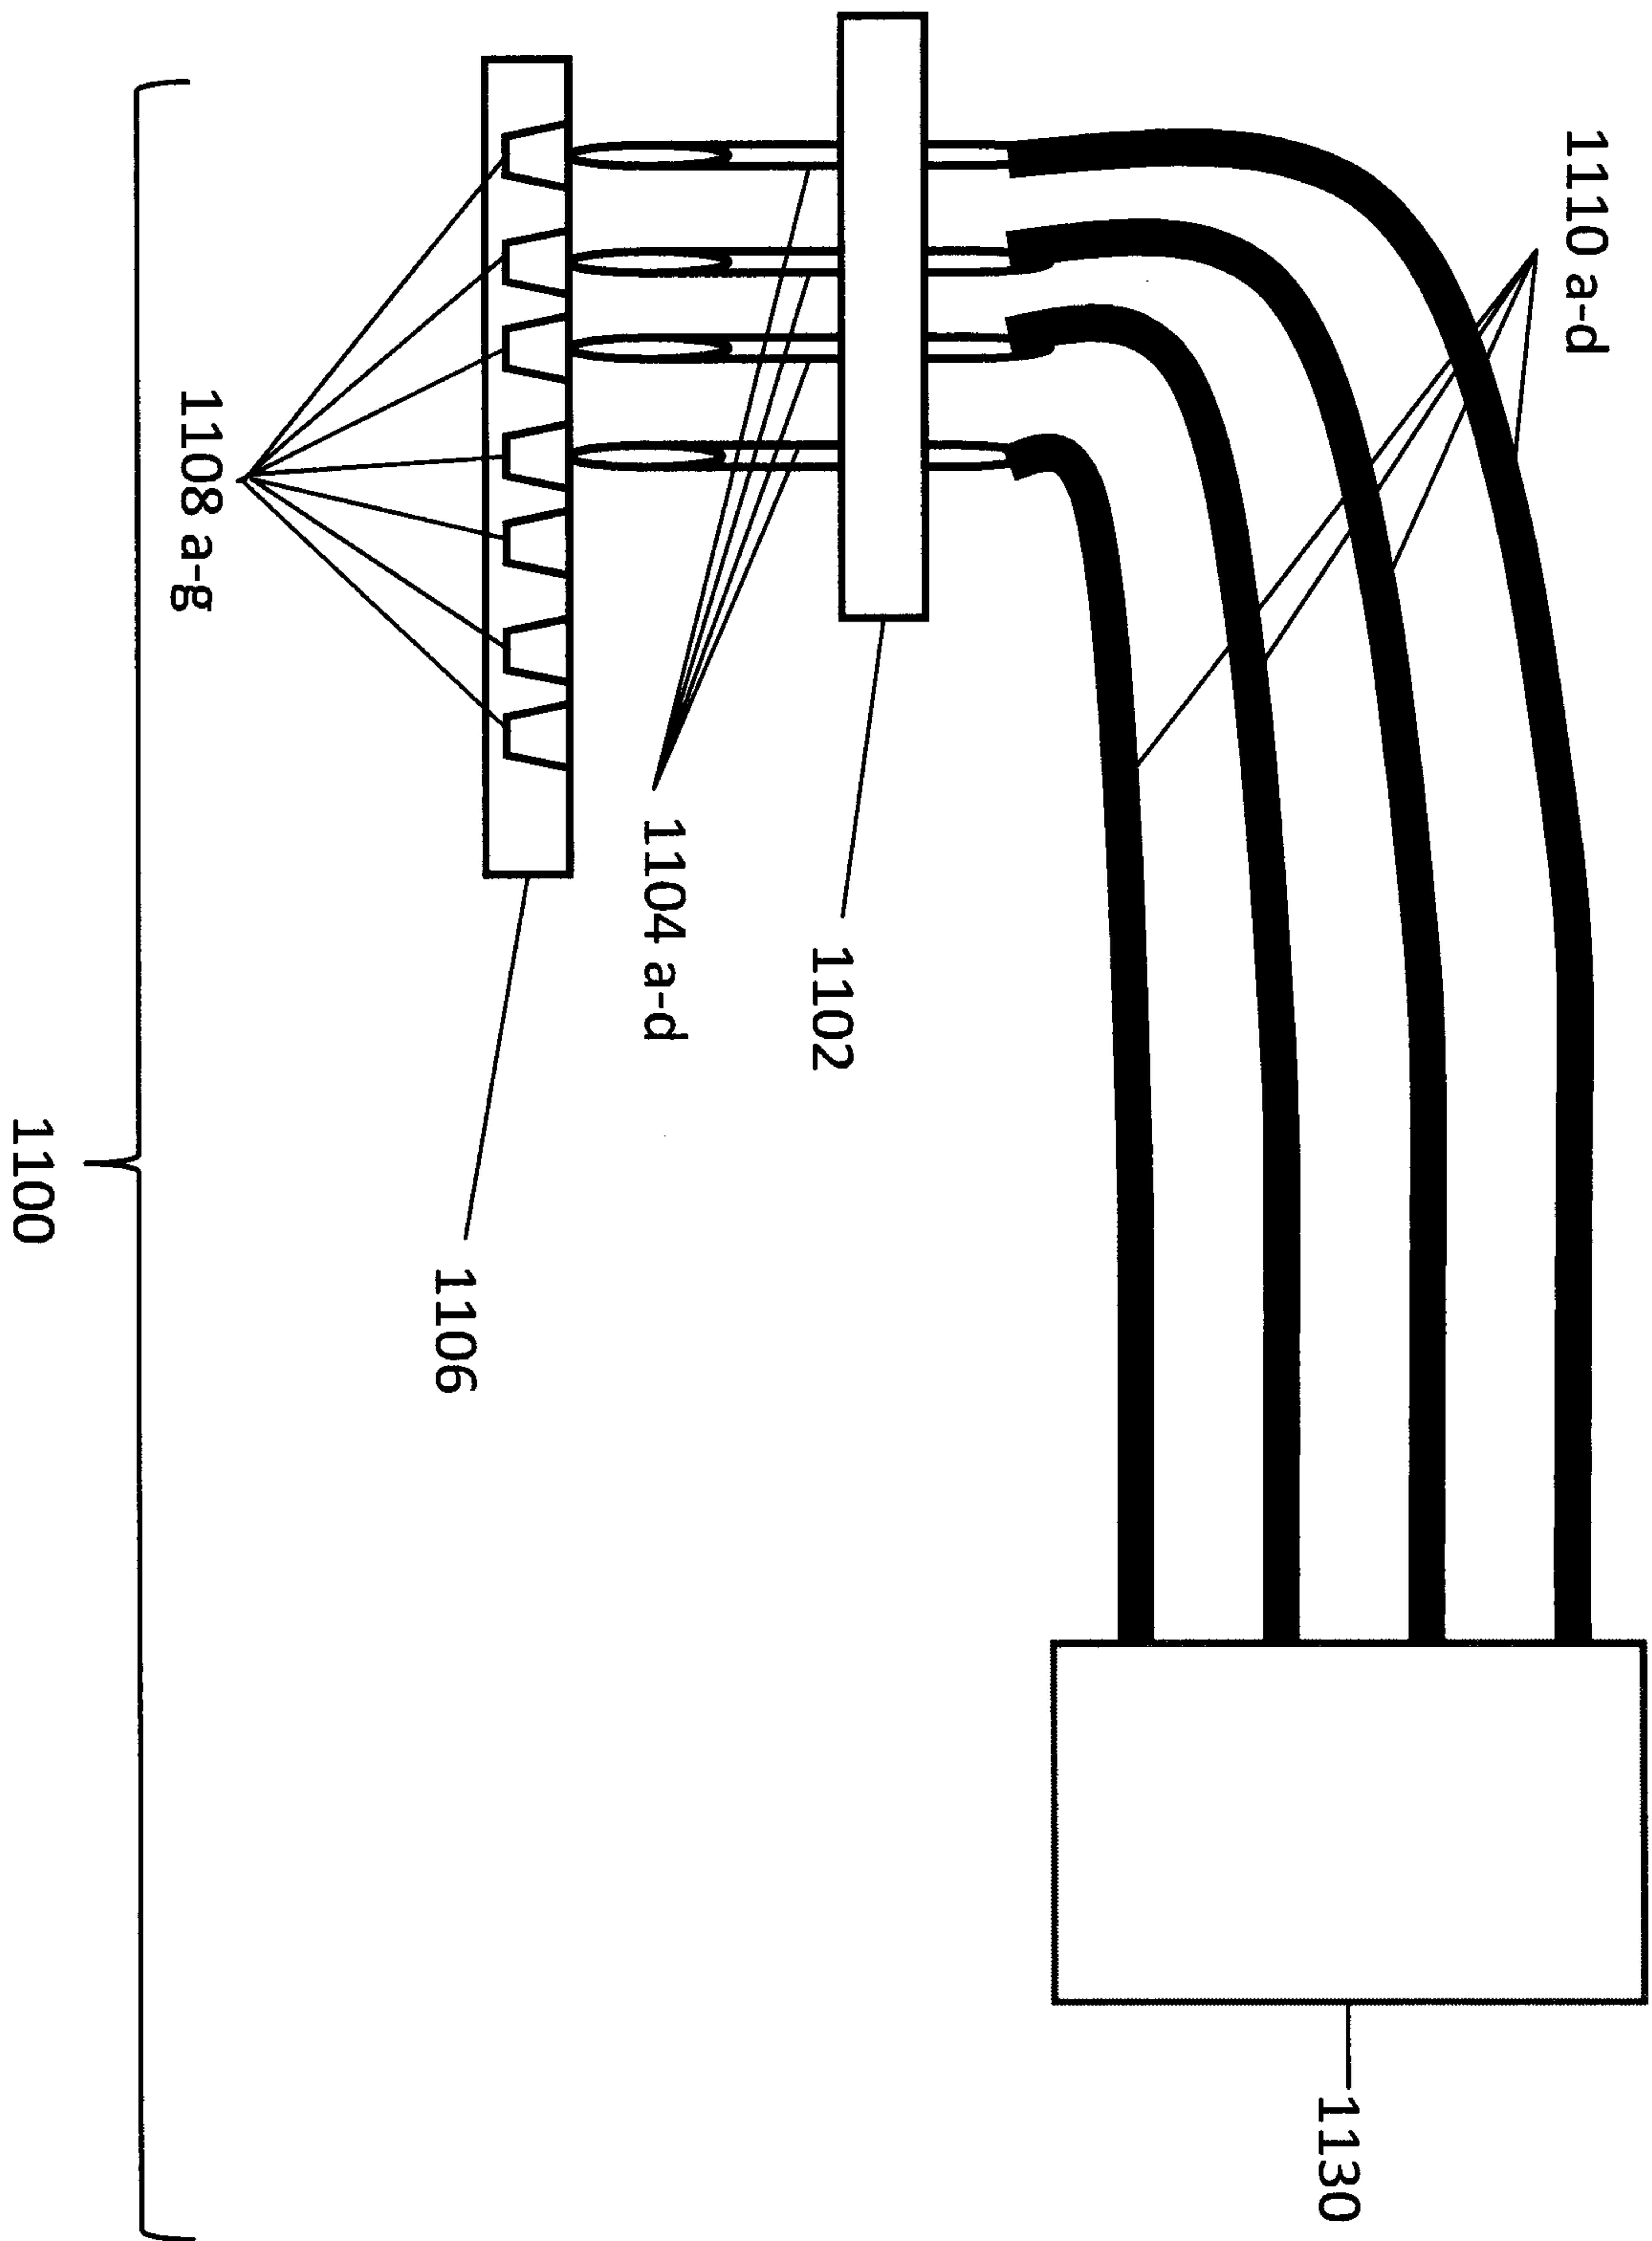
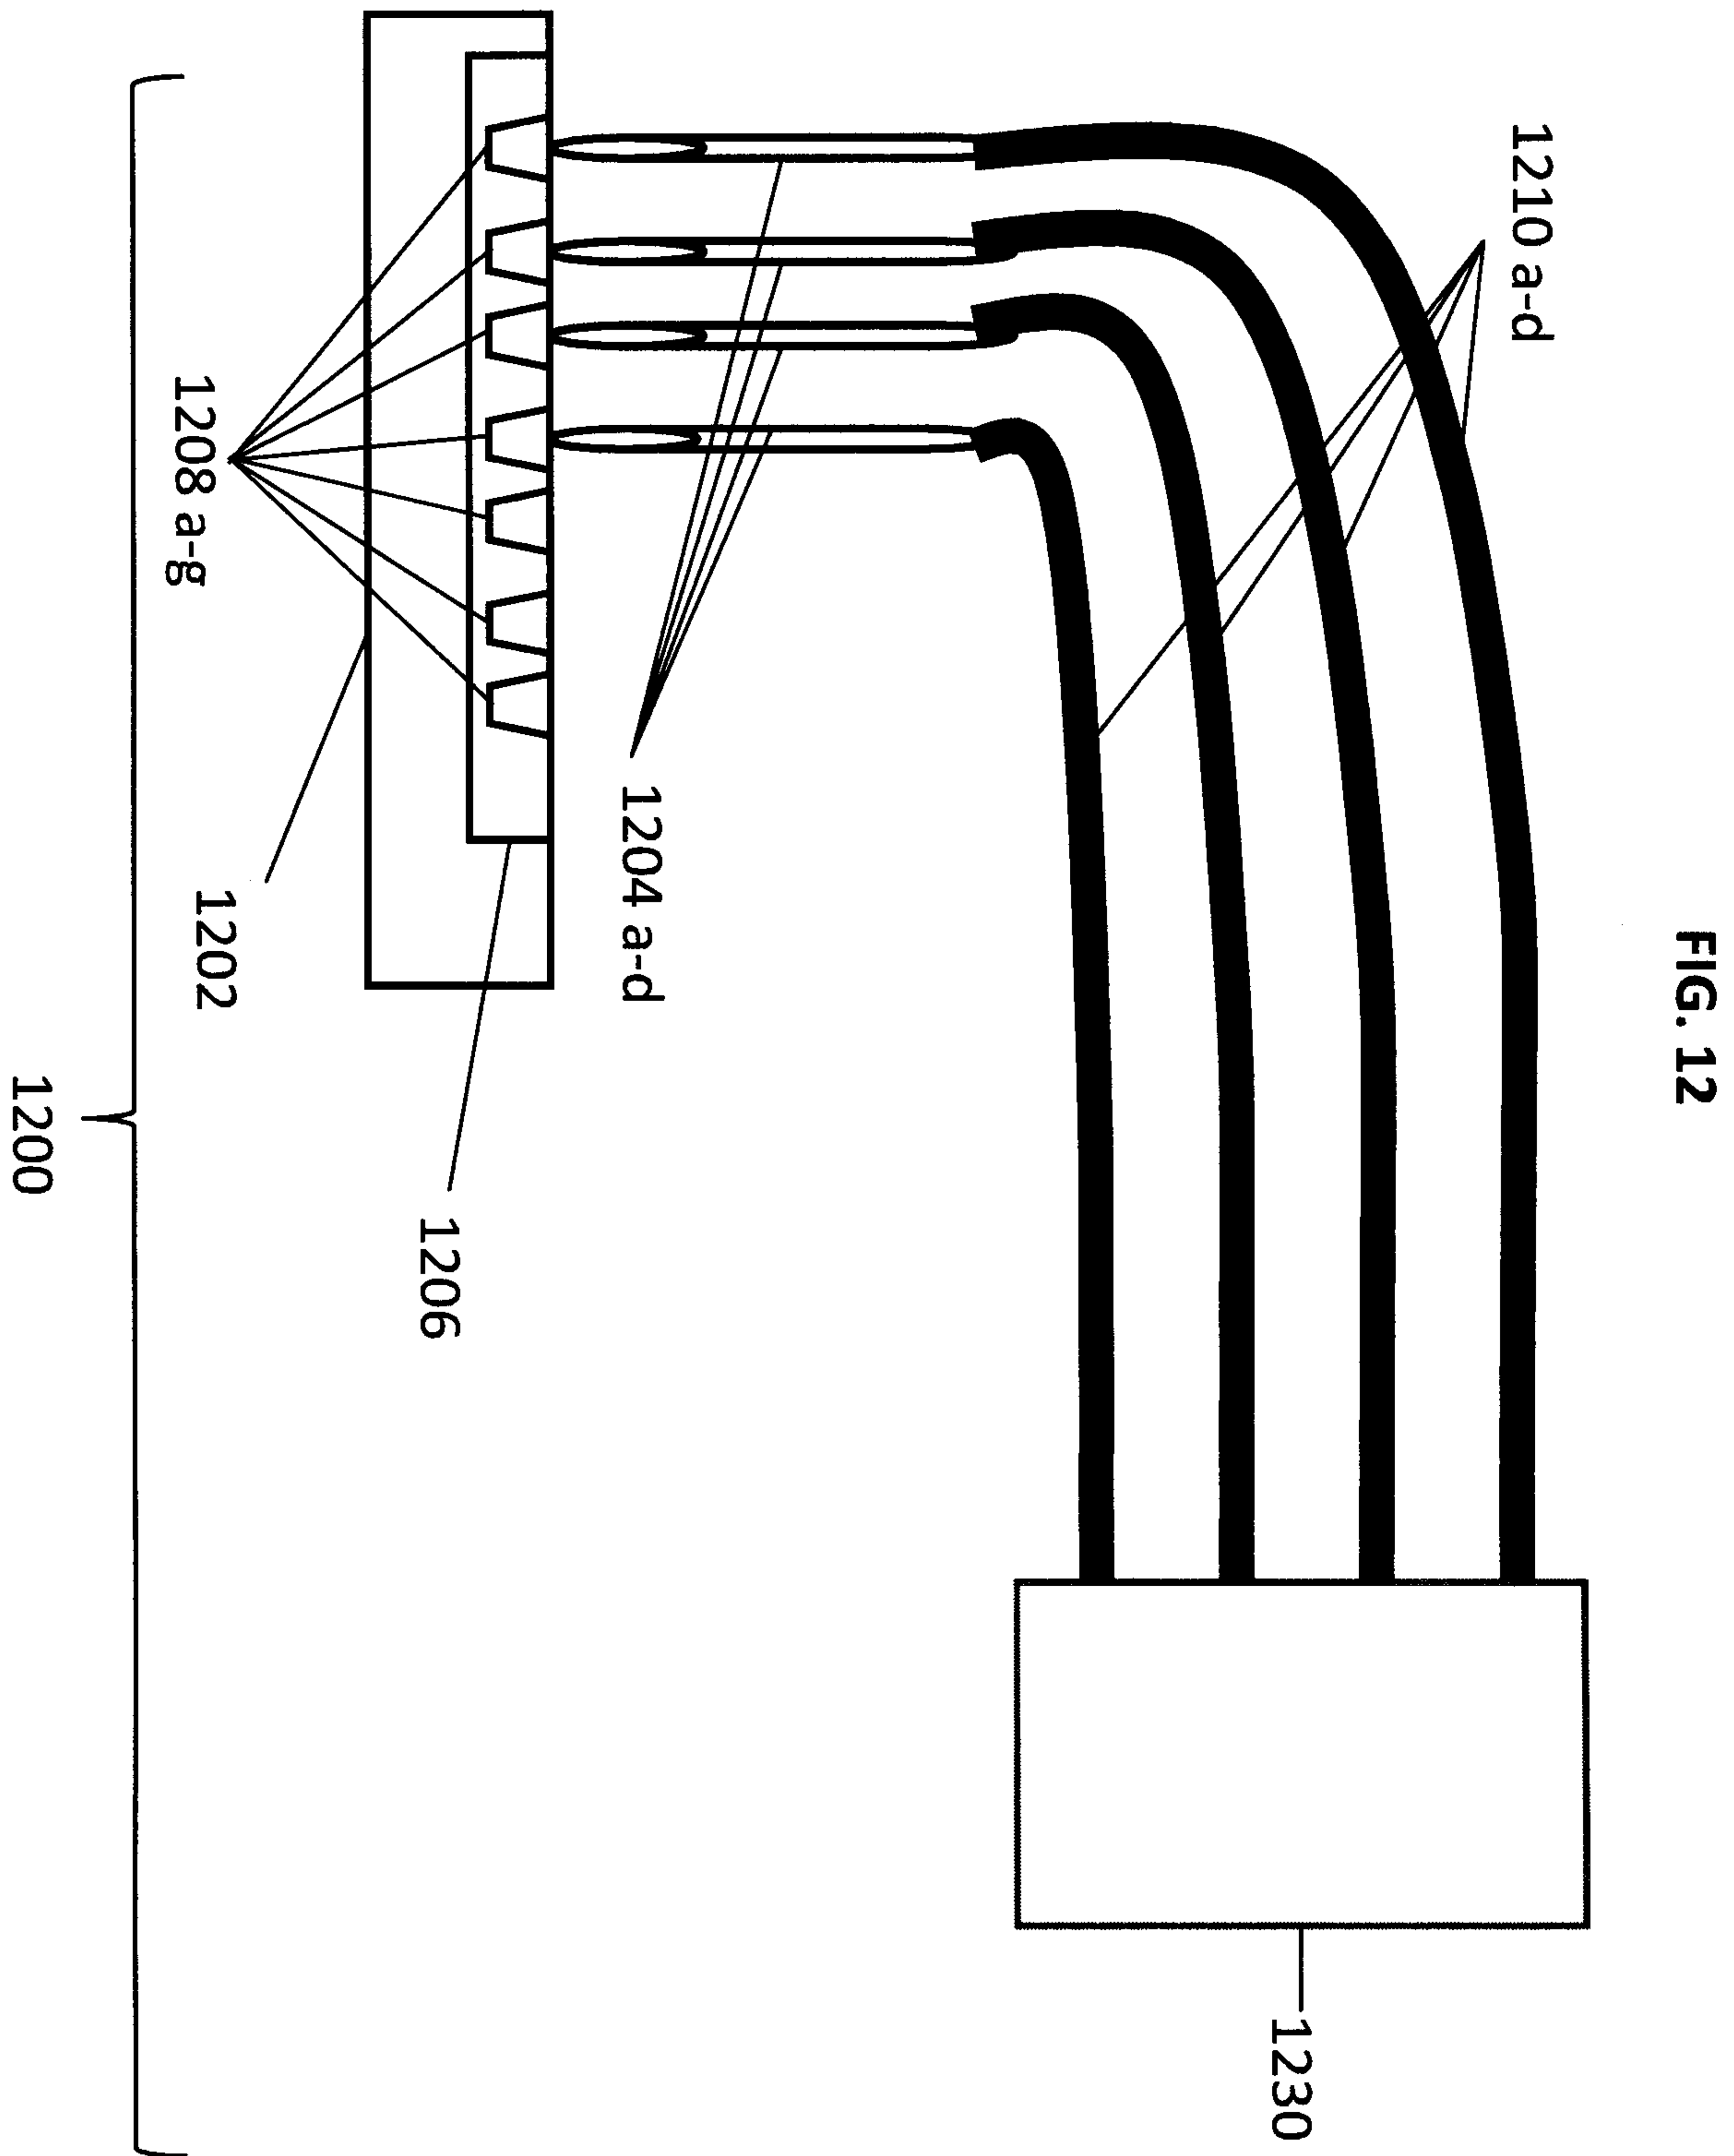


FIG. 11



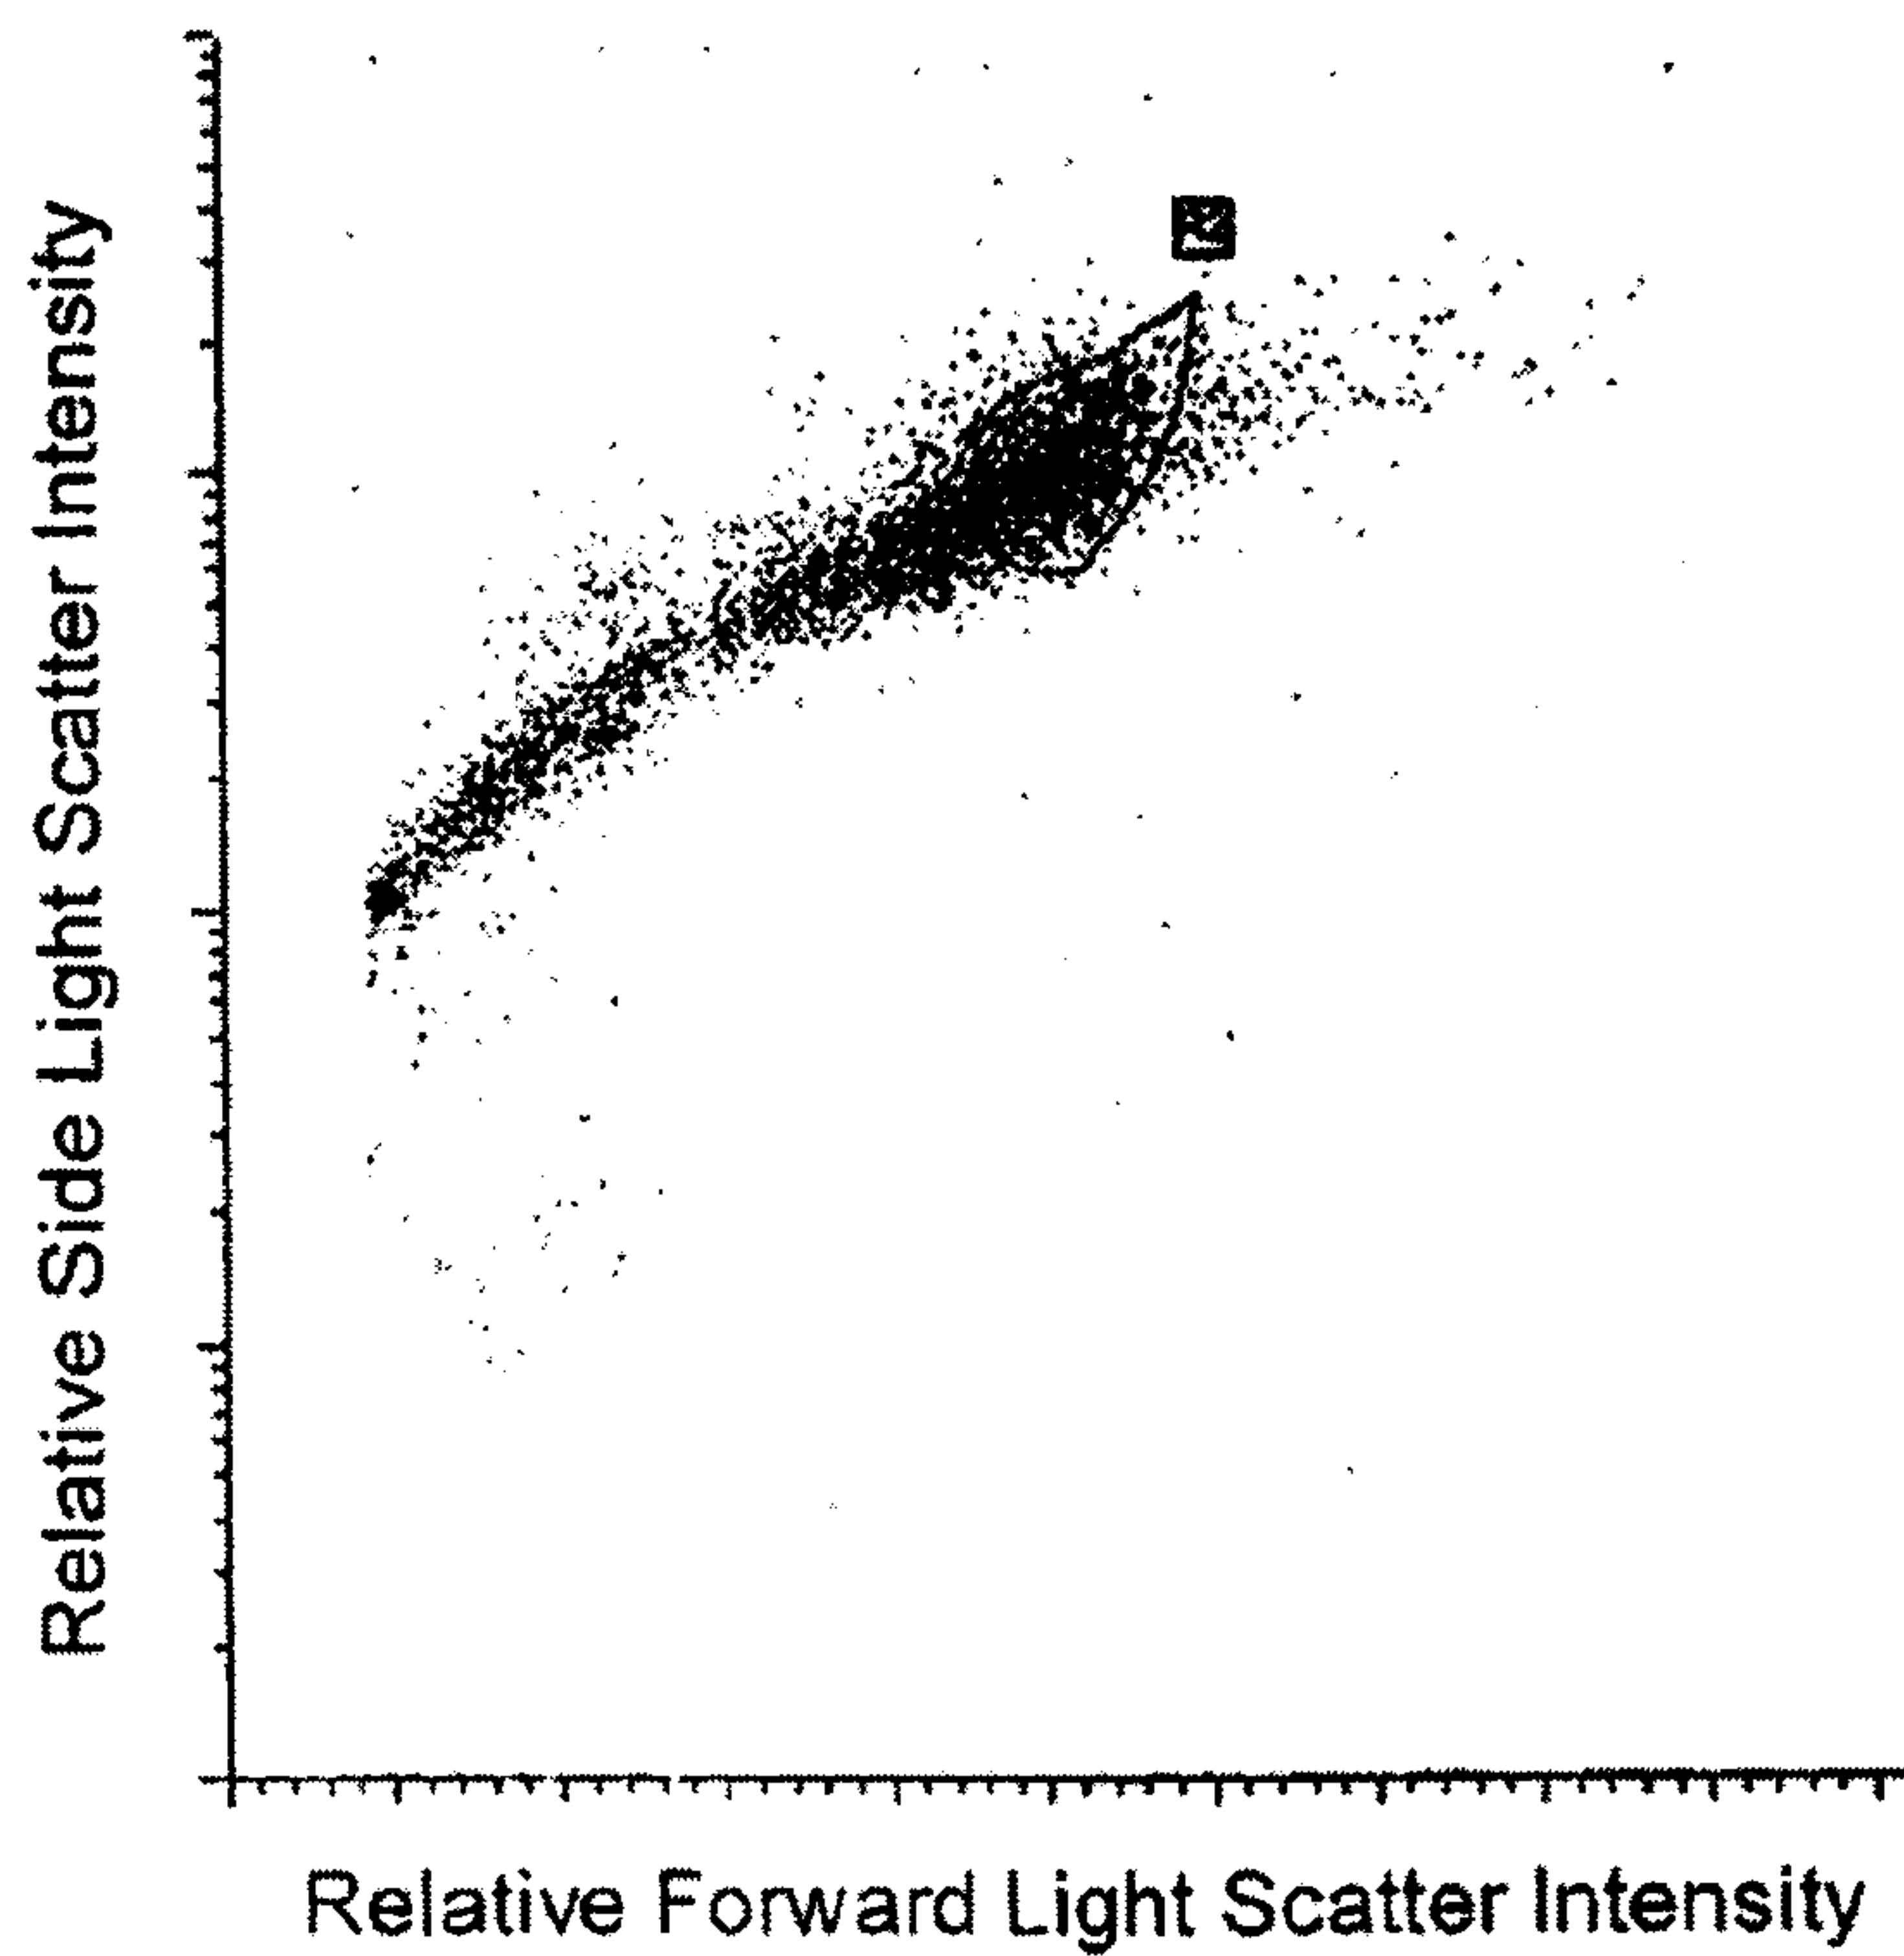


FIG. 13

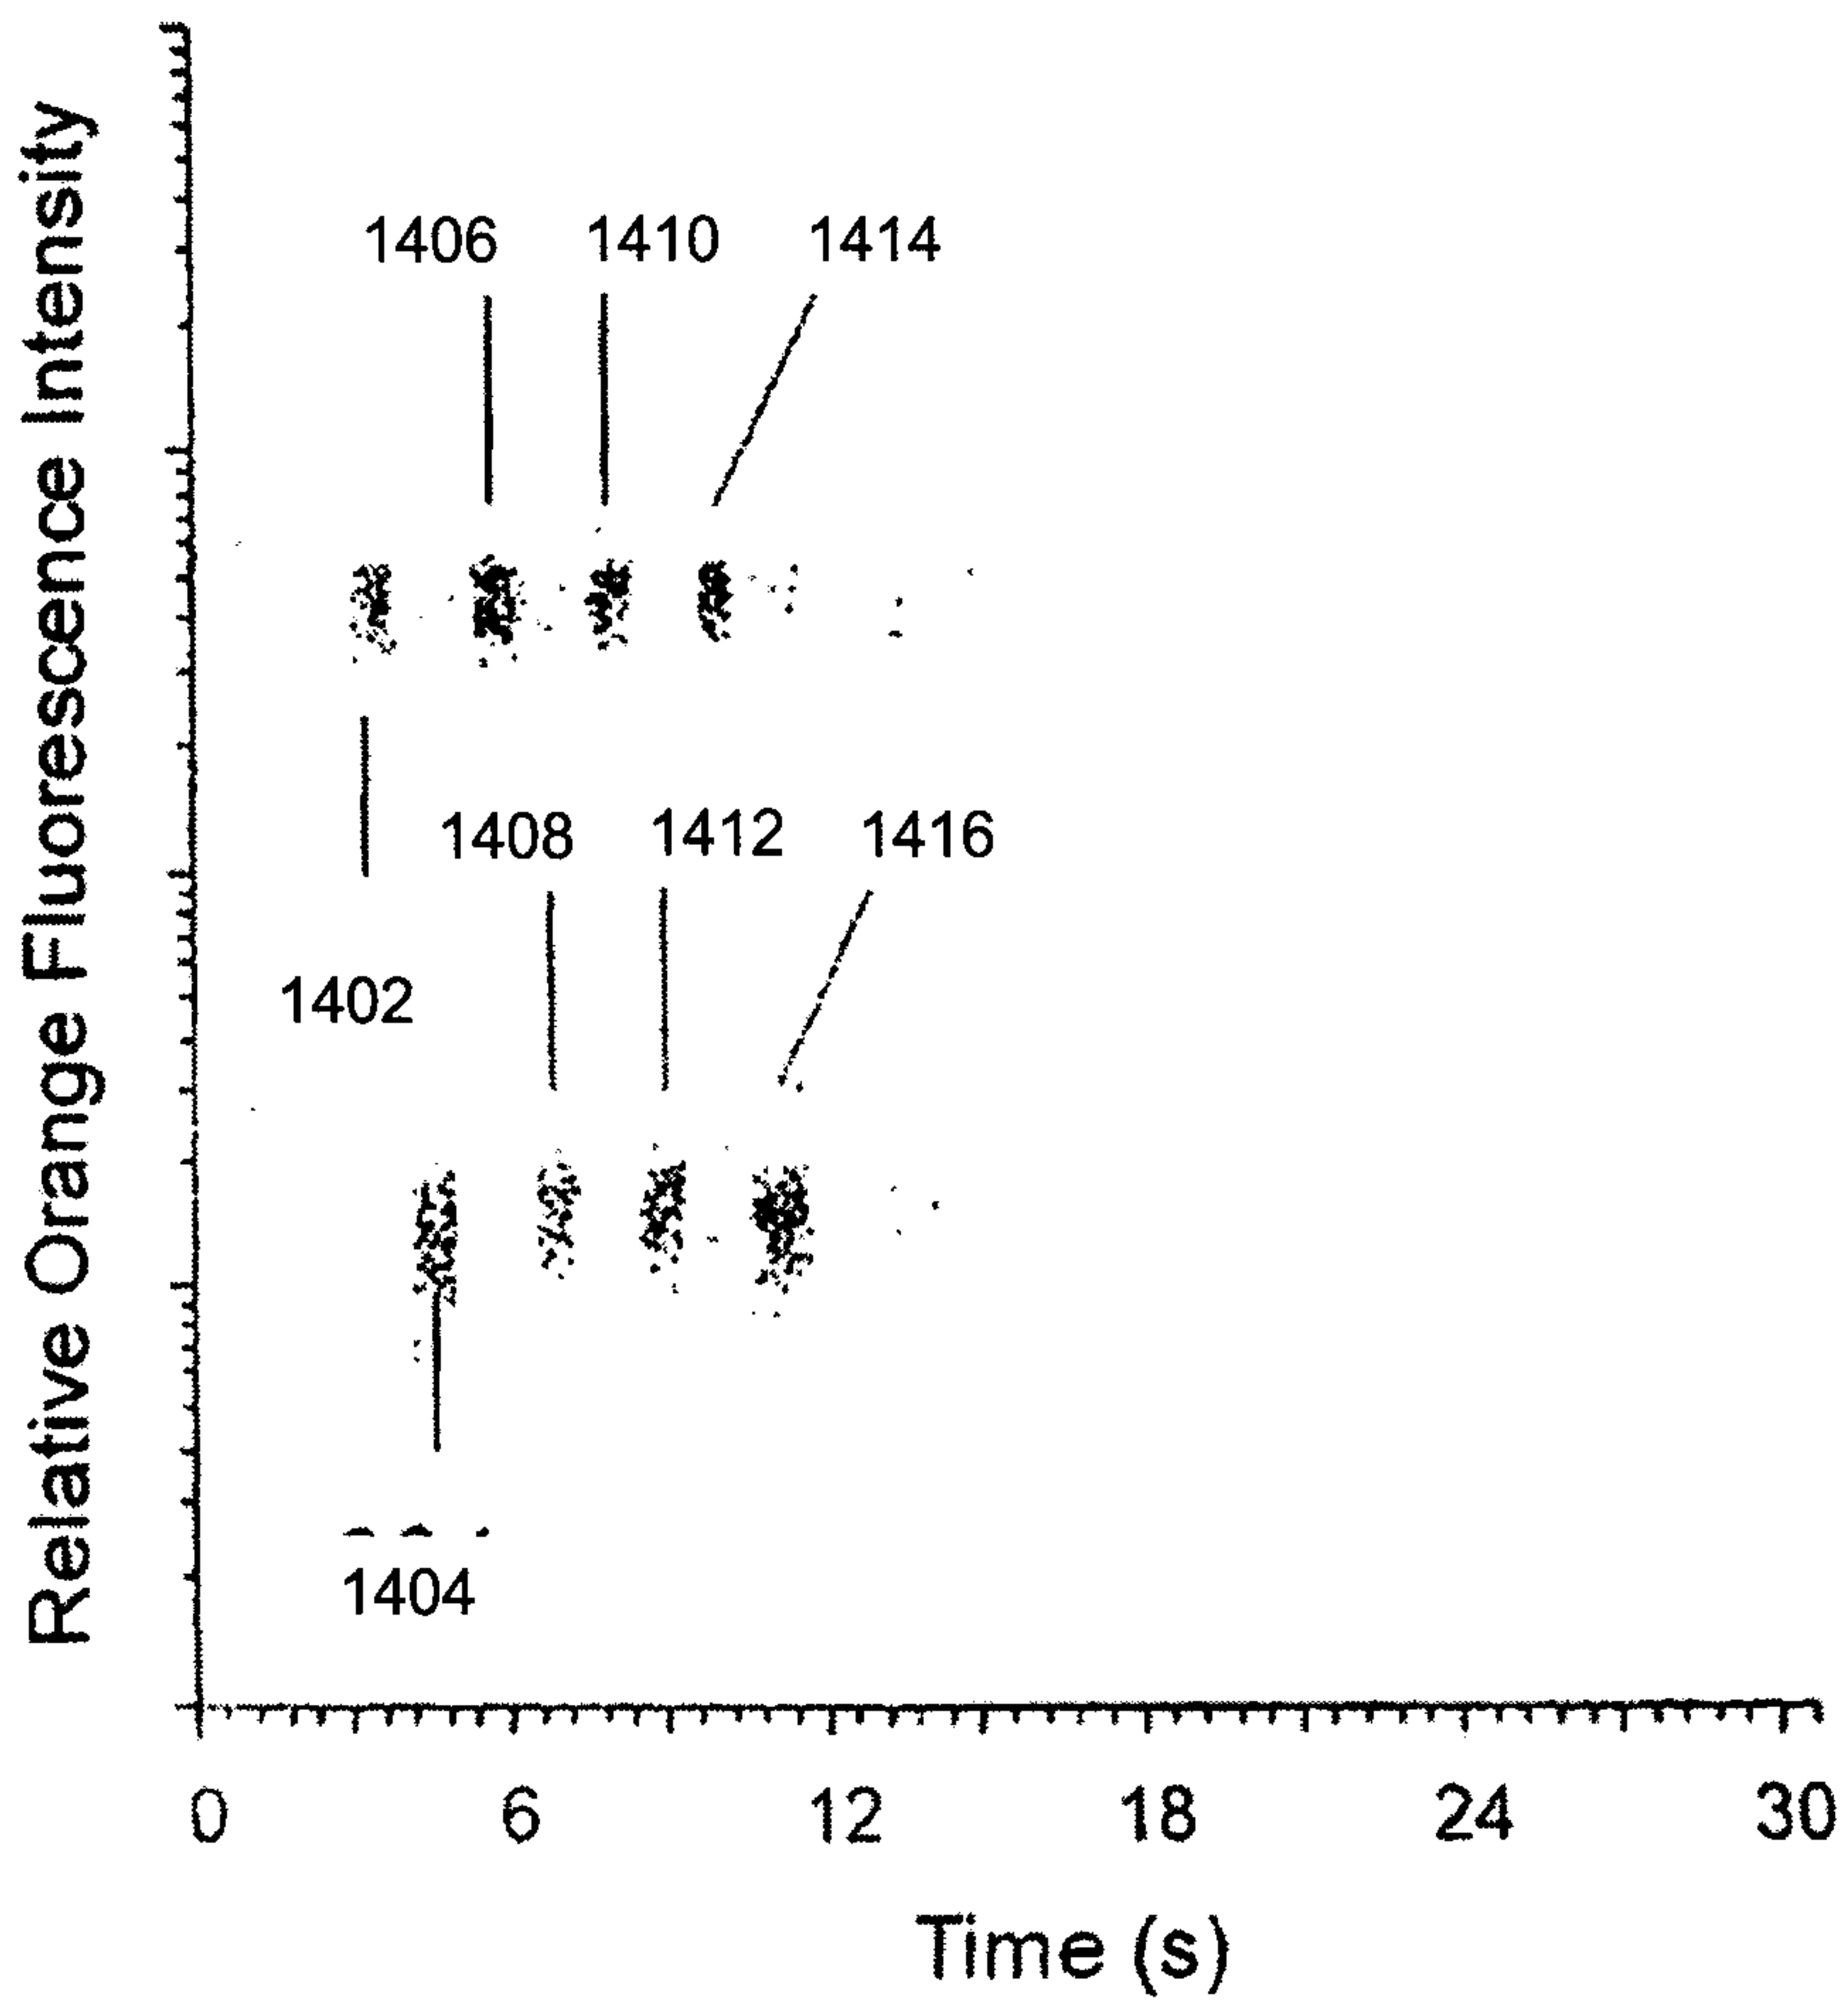


FIG. 14

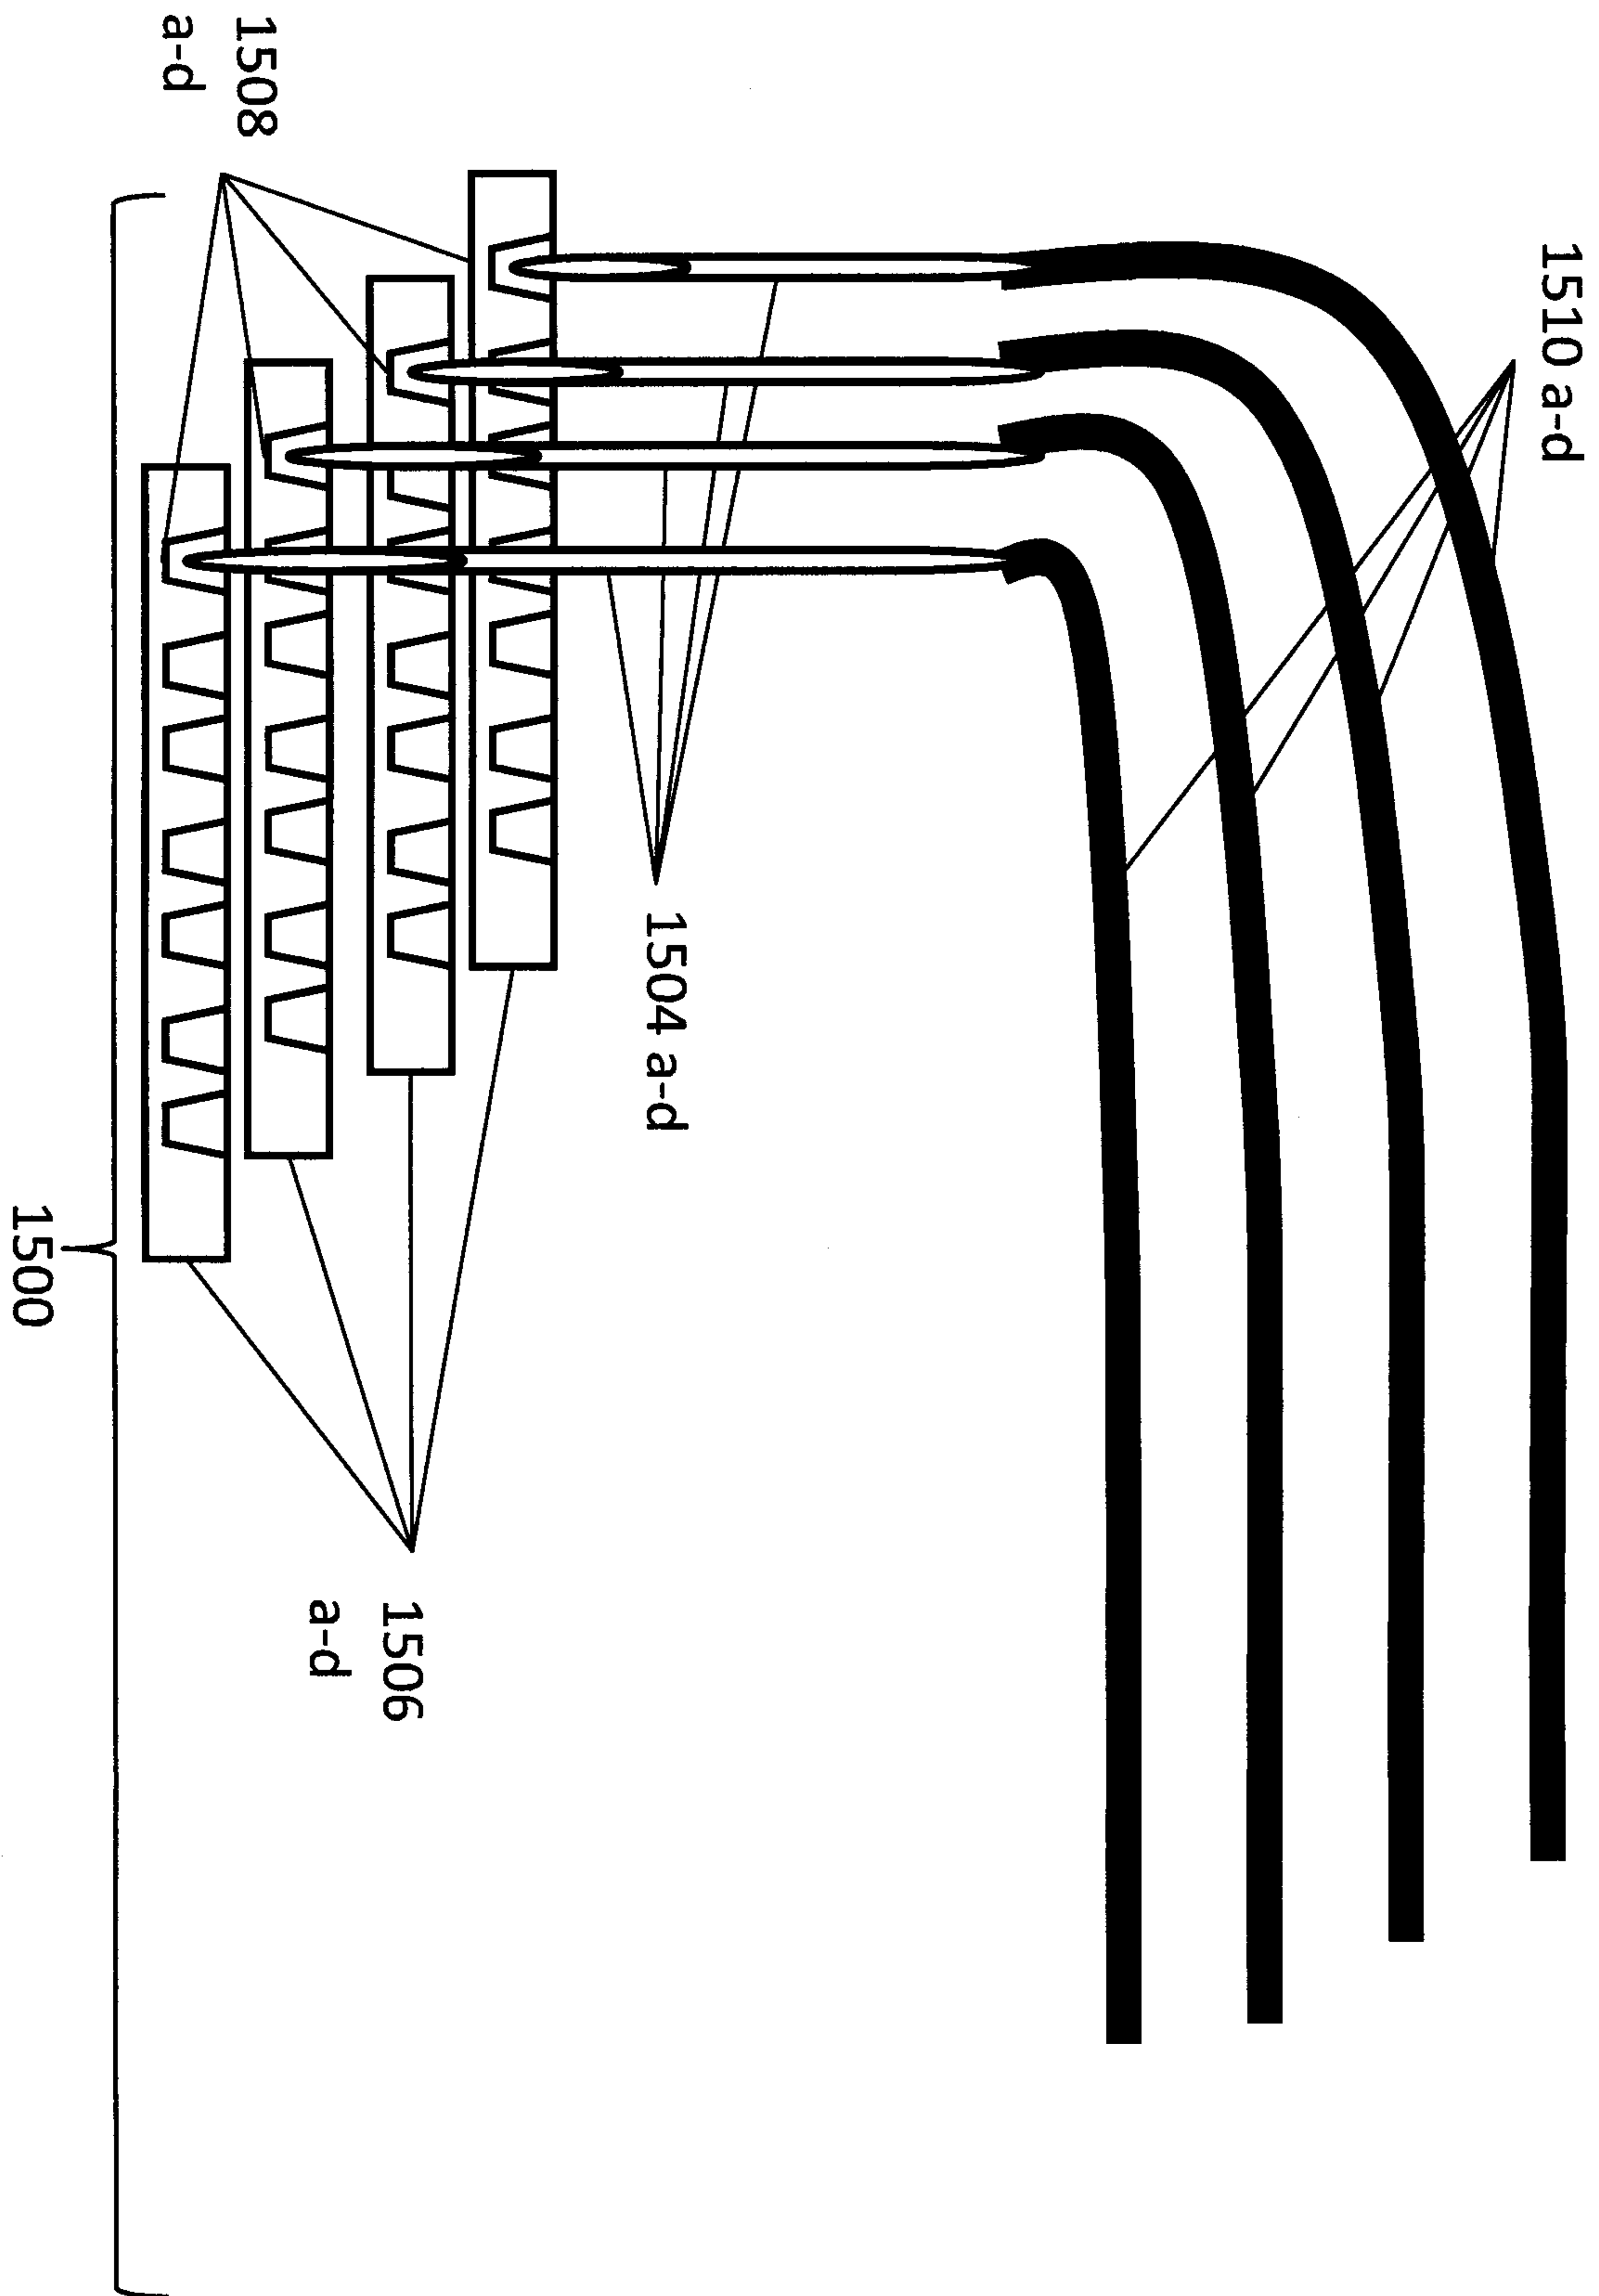


FIGURE 15

FIG. 1

