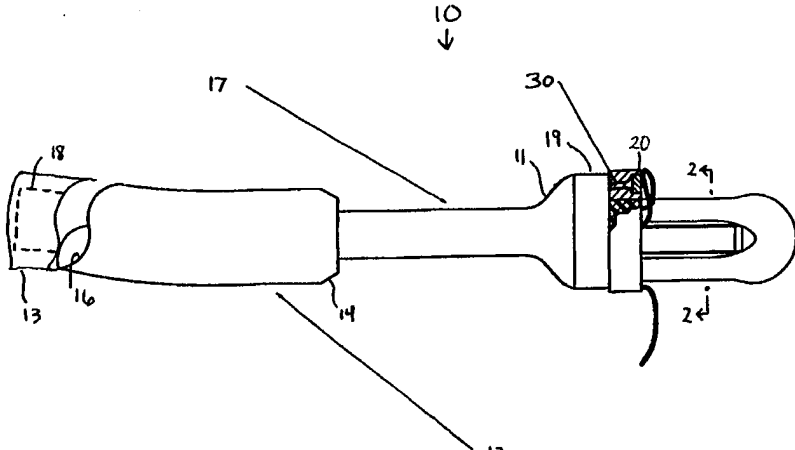


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61B 8/08	A1	(11) International Publication Number: WO 98/38916 (43) International Publication Date: 11 September 1998 (11.09.98)		
<table style="width: 100%; border: none;"> <tr> <td style="width: 50%; vertical-align: top; padding: 5px;"> (21) International Application Number: PCT/US98/04569 (22) International Filing Date: 6 March 1998 (06.03.98) (30) Priority Data: 08/812,656 7 March 1997 (07.03.97) US (71) Applicant: CARDIOGENESIS CORPORATION [US/US]; 540 Oakmead Parkway, Sunnyvale, CA 94086 (US). (72) Inventor: KESTEN, Randy, J.; 181 Ada Avenue #41, Mountain View, CA 94043 (US). (74) Agents: LYNCH, Edward, J.; Heller, Ehrman, White & McAuliffe, 525 University Avenue, Palo Alto, CA 94301-1900 (US) et al. </td> <td style="width: 50%; vertical-align: top; padding: 5px;"> (81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, GW, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i> </td> </tr> </table>			(21) International Application Number: PCT/US98/04569 (22) International Filing Date: 6 March 1998 (06.03.98) (30) Priority Data: 08/812,656 7 March 1997 (07.03.97) US (71) Applicant: CARDIOGENESIS CORPORATION [US/US]; 540 Oakmead Parkway, Sunnyvale, CA 94086 (US). (72) Inventor: KESTEN, Randy, J.; 181 Ada Avenue #41, Mountain View, CA 94043 (US). (74) Agents: LYNCH, Edward, J.; Heller, Ehrman, White & McAuliffe, 525 University Avenue, Palo Alto, CA 94301-1900 (US) et al.	(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, GW, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i>
(21) International Application Number: PCT/US98/04569 (22) International Filing Date: 6 March 1998 (06.03.98) (30) Priority Data: 08/812,656 7 March 1997 (07.03.97) US (71) Applicant: CARDIOGENESIS CORPORATION [US/US]; 540 Oakmead Parkway, Sunnyvale, CA 94086 (US). (72) Inventor: KESTEN, Randy, J.; 181 Ada Avenue #41, Mountain View, CA 94043 (US). (74) Agents: LYNCH, Edward, J.; Heller, Ehrman, White & McAuliffe, 525 University Avenue, Palo Alto, CA 94301-1900 (US) et al.	(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, GW, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i>			
(54) Title: APPARATUS AND METHOD OF MYOCARDIAL REVASCULARIZATION USING ULTRASONIC PULSE-ECHO DISTANCE RANGING				
				
(57) Abstract <p>An apparatus and method of intraoperative myocardial revascularization of the myocardium of the heart of a patient. A catheter apparatus comprising an elongated catheter, an elongated laser wave guide slidably disposed within a lumen of the catheter, and an ultrasonic transducer secured to the distal end of the elongated laser wave guide, is inserted into the patient. The distal end of the catheter apparatus is guided to the portion of the patient's heart wall in which channels will be formed, and the ultrasonic transducer is activated to create brief pulses of ultrasonic energy. The transducer receives a returned ultrasonic echo from the heart wall. The ultrasonic echo is processed by signal processing elements. The processed ultrasonic echoes are displayed to show the distance between the epicardial and endocardial surfaces of the portion of the heart wall in which the revascularization energy is to be discharged, and the distance between the operative distal end of the myocardial revascularization device and such endocardial and epicardial surfaces. After distance measurements have been performed, channels are formed in the heart wall.</p>				

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

APPARATUS AND METHOD OF MYOCARDIAL REVASCULARIZATION
USING ULTRASONIC PULSE-ECHO DISTANCE RANGING

BACKGROUND OF THE INVENTION

The invention relates to the field of medical devices, and more particularly
5 to an apparatus and method for measuring the distance between the operative
distal end of a myocardial revascularization device and the endocardial and
epicardial surfaces of the heart wall of a patient.

In the treatment of cardiovascular disease, transmyocardial
revascularization (TMR) is a well known technique in which channels are
10 formed in a patient's heart wall to supply blood flow to the ischemic heart
tissue and to treat angina. The channels extend through the heart wall
muscular surface, or myocardium, located between the epicardium and
endocardium of the heart wall. In laser transmyocardial revascularization
(LMR), a laser is used to form one or more channels in a patient's heart wall
15 defining the heart chamber. The laser energy is typically transmitted from the
laser to the heart tissue by an optical fiber, with a lens on the distal end of the
optical fiber operatively engaging the heart tissue to be revascularized. Other
energy systems, such as electrodes, may be used for myocardial
revascularization.

20 Initial revascularization procedures required the chest wall to be
opened for insertion of the revascularization device and penetration of the
entire heart wall to form a channel through the myocardium into the
endocardium. Copending application, Serial No. 08/368,409, filed on
December 30, 1994 which is incorporated herein in its entirety, describes an

intravascular system for percutaneous transmymocardial revascularization (PTMR) which eliminates the need of the prior procedures for opening the chest cavity and penetrating the entire heart wall. The PTMR system is introduced into a peripheral artery and advanced through the patient's arterial system into the left ventricle of the patient's heart, from where the revascularization channels are formed through the endocardium and into the myocardium.

Transmyocardial revascularization requires accurate measurement of the thickness of the patient's heart wall, in order for the procedure to be performed with maximum safety and effectiveness. Establishing the thickness of the heart wall at the location where TMR energy is to be discharged decreases the likelihood of injury to the patient from transmural perforation, and allows the physician to precisely control the channel formation by controlling of the depth of penetration of the discharged energy. TMR also requires establishing the distance between the operative distal end of a TMR device and the heart wall surface to determine when activation of the TMR device will effectively form channels within the patient's heart wall. Intimate contact between the operative distal end of the TMR device and the patient's heart tissue is necessary to provide sufficient transmission of the channel forming energy to the heart wall. Ranging information regarding the TMR device is therefore necessary to determine when contact between the TMR device and the heart wall surface has been achieved.

One of the difficulties with currently used PTMR devices has been the inability to accurately measure the thickness of the patient's heart wall

at the precise location where TMR channels are to be formed. Information regarding wall thickness is currently obtained through echocardiographic analysis that may be performed either before or during the TMR procedure. However, methods of measuring heart wall thickness, such as transthoracic
5 or transesophageal echocardiography, only provide information for a small sample of locations on the heart wall and do not provide information regarding the precise location in which the TMR channels are to be formed.

Current methods used in TMR for determining contact with the heart wall have proven inadequate. In typical TMR devices, the physician
10 determines the point at which the operative distal end has contacted the endocardium by observation of a fluoroscopic image of the optical assembly. However, fluoroscopic imaging requires a substantial amount of fluoroscopy time, and therefore exposes the patient to a large amount of radiation.

Alternatively, the physician may infer contact from the observation of ectopic
15 beats on the electrocardiogram, or from the observation of a reciprocating motion in the PTMR device produced when the device is in contact with the endocardial surface. However, these methods increase the expertise required to perform the procedure, and often provide ambiguous information.

What has been needed is the ability to reliably measure the thickness
20 of the heart wall to be revascularized, and the distance between the operative distal tip of a PTMR device and the heart wall surface, in order to precisely control the channels formed in the patient's heart wall during PTMR. The invention satisfies these and other needs.

SUMMARY OF THE INVENTION

The invention is directed to an apparatus and method of transmyocardial revascularization utilizing pulsed echo ultrasonic ranging. Specifically, the ultrasonic ranging provides information on the thickness of the heart wall in the precise location in which the revascularization energy is to be discharged, and the distance separating the operative distal end of the revascularization device from the heart wall.

The catheter apparatus of the invention generally has an elongated laser wave guide with an ultrasonic transducer on a distal end of the wave guide. The catheter apparatus also includes an elongated catheter having proximal and distal ends and a lumen therein which slidably receives the elongated laser wave guide.

The present invention comprises a method of intraoperative myocardial revascularization of the myocardium of the heart of a patient. A catheter apparatus comprising an elongated catheter, an elongated laser wave guide slidably disposed within a lumen of the catheter, and an ultrasonic transducer secured to the distal end of the elongated laser wave guide, is inserted into the patient. The distal end of the lasing apparatus is guided to the portion of the patient's heart wall in which channels will be formed, and the ultrasonic transducer is activated to create brief pulses of ultrasonic energy. The transducer receives a returned ultrasonic echo from the heart wall. The ultrasonic echo is used to measure the distances between the distal end of the elongated laser wave guide and the endocardial and epicardial surfaces of the desired portion of the wall of the patient's heart. After distance measurements have been performed, channels are

formed in the heart wall. The distal end of the laser wave guide is maintained against the desired portion of the heart wall while transmitting laser energy from a remote laser source through the laser wave guide and out the distal end thereof in a beam onto the heart wall with sufficient energy and for a
5 sufficient time to form a channel through the wall of the patient's heart.

When the ultrasonic transducer is activated to create brief pulses of ultrasonic energy, an echo of the pulses from the heart wall returns to the transducer. The transducer receives a first returned ultrasonic echo from the surface of the heart wall closest to the transducer, and a second returned
10 ultrasonic echo from the furthestmost surface of the heart wall. For example, in PTMR when the TMR device is within a chamber of the patient's heart, the distal end of the TMR device is positioned directly adjacent to the endocardial surface which lines the inside of the heart chamber. Because the endocardial surface is the heart wall surface closest to the ultrasonic transducer, the first
15 returned ultrasonic echo is from the endocardial surface. A second ultrasonic echo is returned from the epicardial surface on the outer side of the heart wall furthestmost from the distal end of the TMR device. Therefore, the position of the distal end of the TMR device relative to the endocardial surface is indicated by the first ultrasonic echo, and the position relative to the epicardial
20 surface is indicated by the second ultrasonic echo.

In accordance with the invention, the ultrasonic transducer is used to measure the distances between the distal end of the elongated laser wave guide and the endocardial and epicardial surfaces of the portion of the wall of the patient's heart in which the revascularization energy is to be discharged.

Measurement of such distances allows for a determination of the thickness of the heart wall to be revascularized, and whether the operative distal tip of a PTMR device is in contact with the heart wall surface.

The ultrasonic echo is processed by signal processing elements. The
5 processed ultrasonic echoes are displayed to show the distance between the epicardial and endocardial surfaces of the portion of the heart wall in which the revascularization energy is to be discharged, and the distance between the operative distal end of the myocardial revascularization device and such endocardial and epicardial surfaces.

10 The apparatus and method of the invention provides for improved transmyocardial revascularization by allowing more precise control over the channel formation. Measurement and display of the distances between the operative distal end of the TMR device and the endocardial and epicardial surfaces greatly reduces the risk of transmural perforation. Moreover,
15 because the thickness of the heart wall is known, the physician is able to control the channel formation by selecting the depth of penetration of the lasing energy. Additionally, because the position of the distal end of the TMR device relative to the heart wall is known, the premature discharge of lasing energy before the operative distal end of the TMR device has contacted the
20 heart wall is eliminated. These and other advantages of the invention will become more apparent from the following detailed description of the invention and the accompanying exemplary drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is an enlarged longitudinal cross sectional view of a catheter apparatus which embodies features of the invention.

Fig. 2 is a transverse cross sectional view of the catheter apparatus shown in Fig. 1 taken along the lines 2-2.

Fig. 3 is a longitudinal cross sectional view of a human heart with a transmyocardial revascularization catheter apparatus therein.

Fig. 4 is illustrates a display console which embodies features of the invention.

DETAILED DESCRIPTION OF THE INVENTION

As shown in Fig. 1, the catheter apparatus 10 of the invention suitable for performing myocardial revascularization on a desired portion of a wall of the patient's heart generally includes a distal end 11, an elongated catheter 12 having proximal 13 and distal 14 ends and a lumen 16 therein, and an elongated laser wave guide 17 having proximal 18 and distal 19 ends and being slidably disposed within the lumen of the elongated catheter 11. An ultrasonic transducer 20 secured to the distal end 19 of the elongated laser wave guide 17 emits bursts of ultrasonic energy. In the embodiment illustrated in Fig. 1, the ultrasonic transducer 20 is mounted on a side of the laser wave guide 17. Fig. 2 illustrates a cross section of the catheter apparatus shown in Fig. 1, taken along lines 2-2.

An apparatus suitable for implementing the method of myocardial revascularization of the present invention is embodied in the apparatus

illustrated in Fig. 1. Fig. 3 illustrates a TMR device positioned within a heart chamber. Referring to Figs. 1 and 3, the method of the present invention comprises providing a catheter apparatus 10 suitable for performing myocardial revascularization. As illustrated in Fig. 3, the patient's heart 21 includes a portion 22 at which a myocardial revascularization channel 23 is to be formed in the wall 24 of the heart, said wall comprising an endocardial surface 26, a myocardium 27, and an epicardial surface 28. The distal end 11 of the apparatus 10 is guided within the patient to the desired portion 22 of the heart wall 24 through which a channel 23 is to be formed. The ultrasonic transducer is then activated to create a pulse of ultrasonic energy. An ultrasonic echo retrieved by the ultrasonic transducer is monitored to measure distances between the distal end 19 of the elongated laser wave guide 17 and the endocardial 26 and epicardial 28 surfaces of the desired portion 22 of the wall 24 of the patient's heart 21.

In one aspect of the invention, fine wire leads 30 operably connect the ultrasonic transducer 20 to signal processing elements 32 located externally to the laser wave guide 17. The fine wire leads 30 may be contained within the lumen 16 of the elongated catheter or within a catheter wall defining the lumen 16. The fine wire leads 30 connect to a suitable cable 31 on the proximal end of the catheter 12 which connects to the signal processing elements 32 and a display console 33. The signal processing elements 32 process the ultrasonic echo for display of distances measured thereby. The signal processing elements 32 generate and amplify an ultrasonic pulse emitted from the ultrasonic transducer 20, and amplify and process for

display the echo signal received by the transducer 20. Typical pulse echo techniques are used to create a clock driven pulse generator and to demodulate and amplify the returned echo signal.

Fig. 4 illustrates a display console 33 for displaying the processes
5 echo signal. The display console 33 indicates the distance between the distal end 19 of the laser wave guide 17 and the endocardial surface 26, as well as the thickness of the myocardium 27 directly in front of the laser wave guide distal end 19. The display console 33 may be a cathode ray tube (CRT) monitor, a liquid crystal display (LCD) screen, or other similar suitable
10 devices. In the embodiment illustrated in Fig. 4, the display console 33 has a permanently imprinted representation of the distal end 19 of the laser wave guide 17. Displayed on the console are two dashed lines; the lower line 36 represents the location of the endocardial surface as determined by the initial echo of the ultrasonic pulse during a PTMR procedure, and the upper line 37
15 represents the location of the epicardial surface 28 as determined by the second echo. A scale 38 is shown on the display console 33 to provide distance measurements. However, other suitable display systems exist, including a linear series of light emitting diodes (LEDs) or LCD segments displaying the positions of the endocardial 26 and epicardial 28 surfaces
20 relative to the laser wave guide 17 distal end 19 (not shown).

In one aspect of the invention, the frequency of the ultrasonic transducer 20 is selected to provide a desired depth of penetration into the wall 24 of the patient's heart 21. In one embodiment, the frequency of the ultrasonic transducer 20 is about 2 to about 9 MHz. The catheter apparatus

10 components are chosen so that the desired frequency coincides with the resonant frequency of the ultrasonic transducer 20.

In a presently preferred embodiment, the ultrasonic transducer 20 is a piezoelectric crystal, such as lead zirconium titanate (PZT) transducers.

- 5 However, one skilled in the art will recognize that many suitable transducers exists. In the embodiment illustrated in Figs. 1 and 2, the ultrasonic transducer 20 is a rectangular shape. However, alternatively shaped transducers are also suitable, including an annular transducer positioned coaxially around the distal end 19 of the laser wave guide 17 (not shown).
- 10 Mechanical mounting of the transducer is performed in such a way as to provide moderate acoustic damping behind the ultrasonic transducer 20 and efficient acoustic coupling in front of the transducer. The ultrasonic transducer 20 may be mounted on the laser wave guide 17 using suitable materials, such a conductive epoxies (not shown), and coatings (not shown),
- 15 such as polystyrene, may be applied to the transducer 20.

While the present invention has been described herein in terms of certain preferred embodiments, modifications and improvements may be made to the invention without departing from the scope thereof.

WHAT IS CLAIMED IS:

1. A catheter apparatus suitable for performing myocardial revascularization on a desired portion of a wall of a patient's heart, comprising:

- 5 a) an elongated catheter having proximal and distal ends and a lumen therein;
- b) an elongated laser wave guide having proximal and distal ends slidably disposed within the lumen of the elongated catheter; and
- 10 c) an ultrasonic transducer secured to the distal end of the elongated laser wave guide for measuring distances between the distal end of the elongated laser wave guide and the endocardial and epicardial surfaces of the desired portion of the wall of the patient's heart.

15 2. The catheter apparatus of claim 1 wherein the ultrasonic transducer is a piezoelectric crystal.

 3. The catheter apparatus of claim 1 wherein fine wire leads operably attached to the ultrasonic transducer connect the ultrasonic transducer to external signal processing elements.

20 4. The catheter apparatus of claim 1 wherein the ultrasonic transducer operates at a frequency of about 2 to about 9 MHz.

 5. A method of forming a channel in a desired portion of a wall of a patient's heart, comprising the steps of:

a) providing a catheter apparatus having a distal end, comprising an elongated catheter having proximal and distal ends and a lumen therein; an elongated laser wave guide having proximal and distal ends slidably disposed within the lumen of the elongated catheter; and an ultrasonic transducer secured to the distal end of the elongated laser wave guide for measuring distances between the distal end of the elongated laser wave guide and the endocardial and epicardial surfaces of the desired portion of the wall of the patient's heart;

b) guiding the distal end of the catheter apparatus within the patient to the desired portion of the patient's heart wall through which a channel is to be formed; and

c) activating the ultrasonic transducer to create pulses of ultrasonic energy;

d) receiving an ultrasonic echo from the heart wall at the ultrasonic transducer;

e) monitoring the ultrasonic echo to measure the distances between the distal end of the elongated laser wave guide and the endocardial and epicardial surfaces of the desired portion of the wall of the patient's heart; and

e) maintaining the distal end of the laser wave guide against the desired portion of the heart wall while transmitting laser energy from a remote laser source through the laser wave guide and out the distal end thereof in a beam onto the heart wall with sufficient energy and for a sufficient time to form a channel through the wall of the patient's heart.

6. The method of claim 5 further including the step of processing the ultrasonic echo using signal processing elements operably connected to the ultrasonic transducer.

7. The method of claim 6 further including the step of displaying the
5 ultrasonic echo to show the distance between the epicardial and endocardial surfaces of the portion of the heart wall, and the distance between the distal end of the elongated laser wave guide and such endocardial and epicardial surfaces.

8. The method of claim 5 wherein a frequency of the ultrasonic
10 transducer is selected to provide a desired depth of penetration into the wall of the patient's heart.

9. The method of claim 5 wherein the frequency of the ultrasonic transducer is about 2 to about 9 MHz.



10. A method of measuring a distance between a distal end of a
15 catheter apparatus suitable for performing myocardial revascularization and an endocardial surface and epicardial surface of a portion of a patient's heart wall in which myocardial revascularization channels are to be formed, comprising creating pulses of ultrasonic energy from an ultrasonic transducer secured to a distal end of the apparatus, receiving ultrasonic echoes from the
20 heart wall, determining from the ultrasonic echoes the distance between the distal end of the apparatus and the endocardial and epicardial surfaces of the portion of the heart wall.

11. The method of claim 10 wherein a frequency of the ultrasonic transducer is selected to provide a desired depth of penetration into the wall of the patient's heart.

12. The method of claim 11 wherein the frequency of the ultrasonic
5 transducer is about 2 to about 9 MHz.

13. The method of claim 10 further including the step of processing the ultrasonic echoes using signal processing elements operably connected to the ultrasonic transducer.

14. The method of claim 10 further including the step of displaying
10 the ultrasonic echoes to show the distance between the epicardial and endocardial surfaces of the portion of the heart wall, and the distance between the distal end of the catheter apparatus and such endocardial and epicardial surfaces.

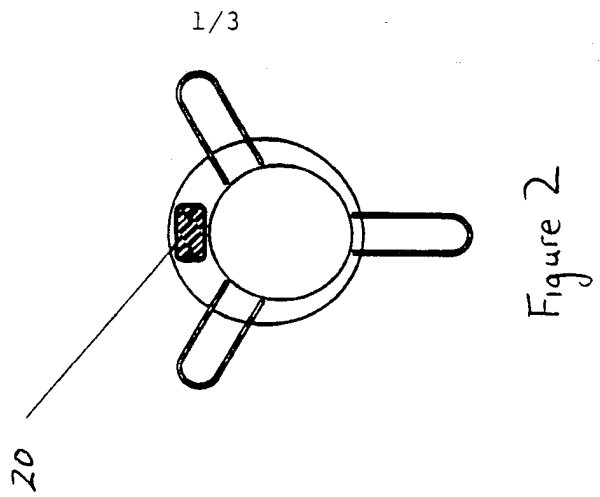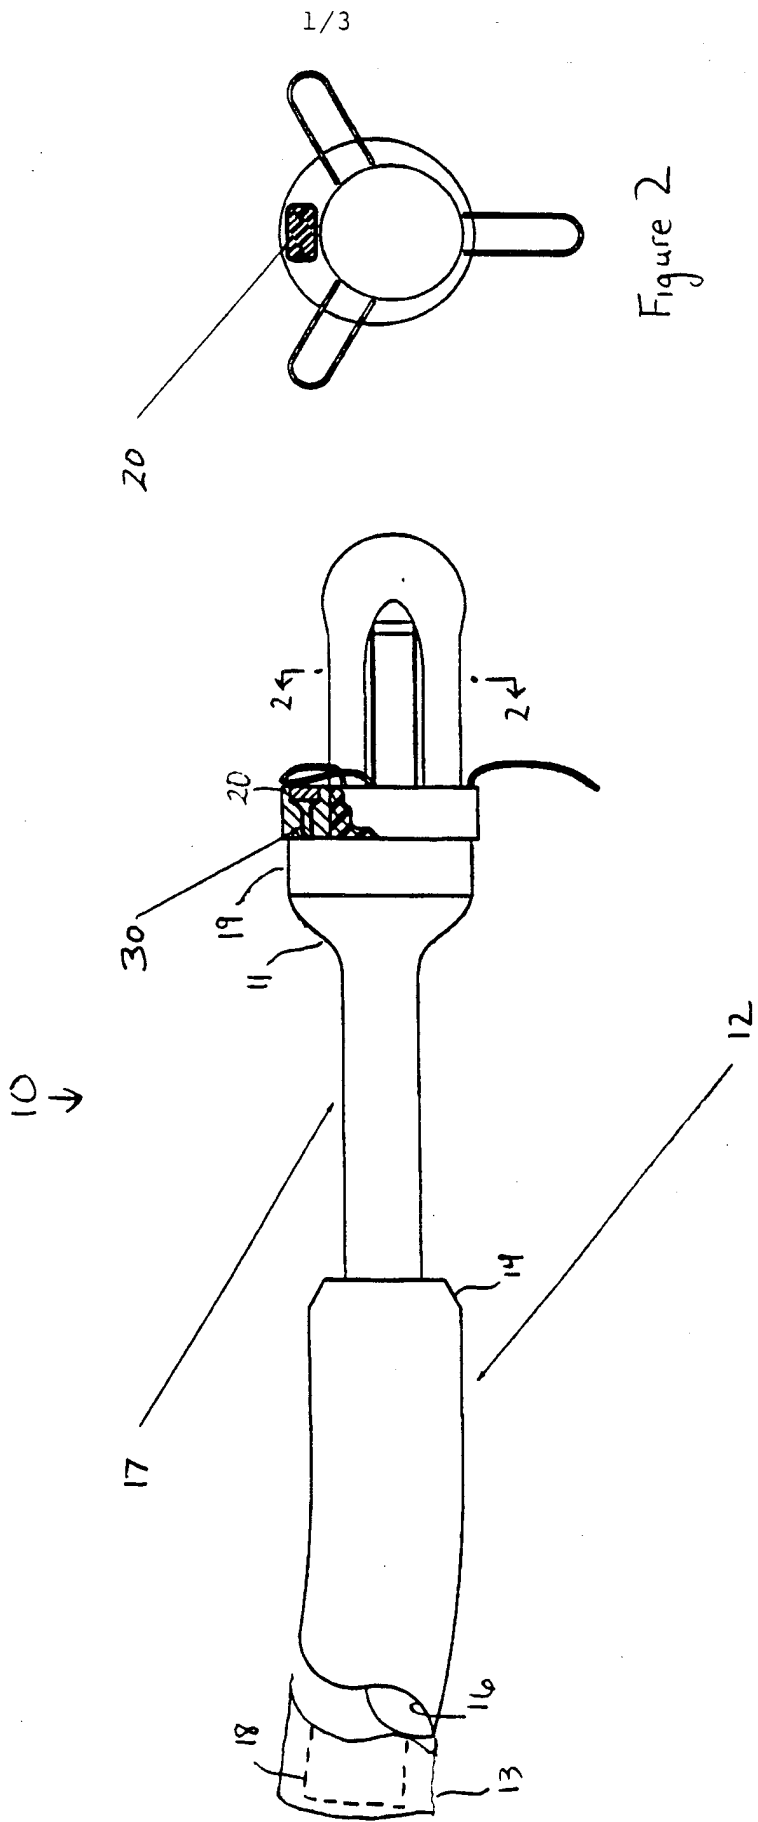

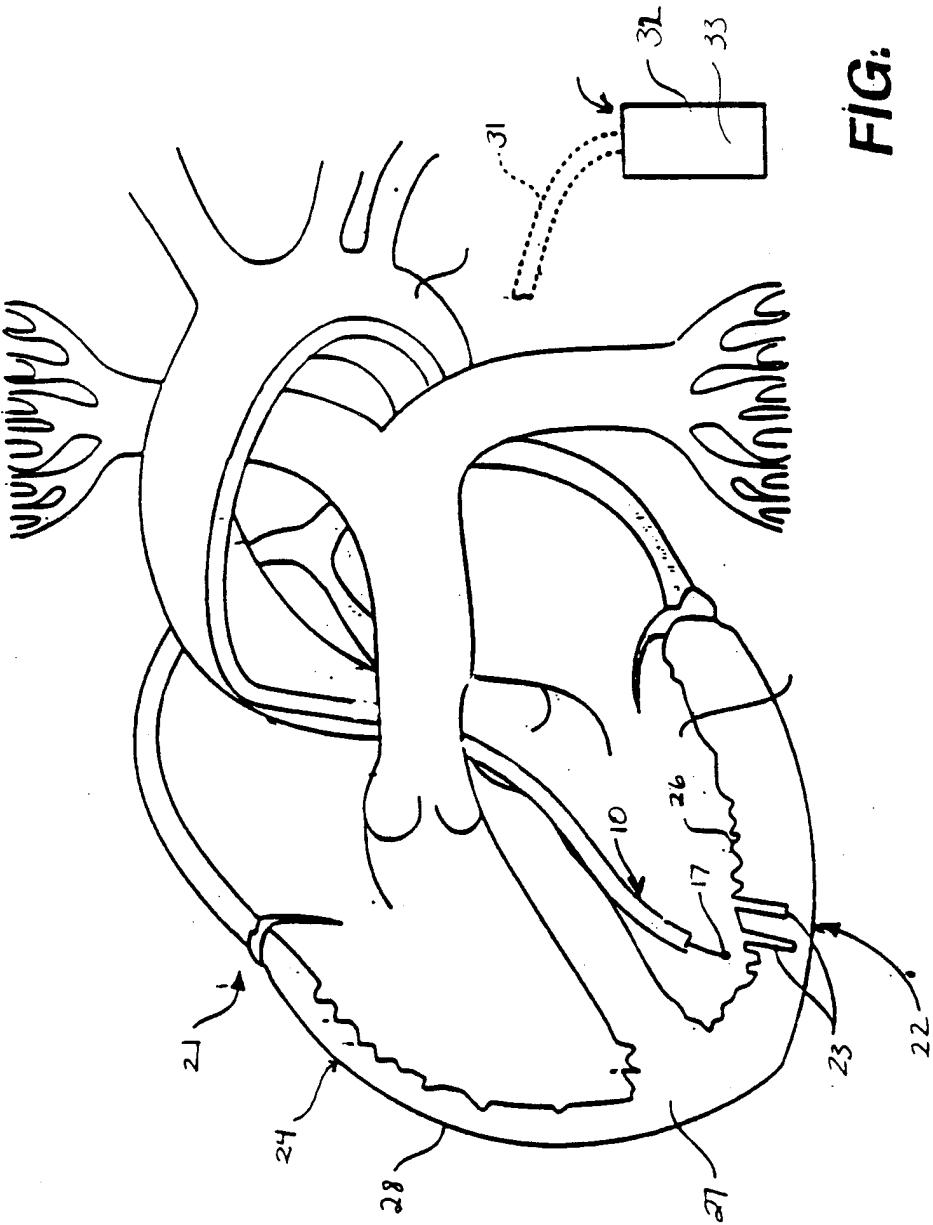


FIG. 3

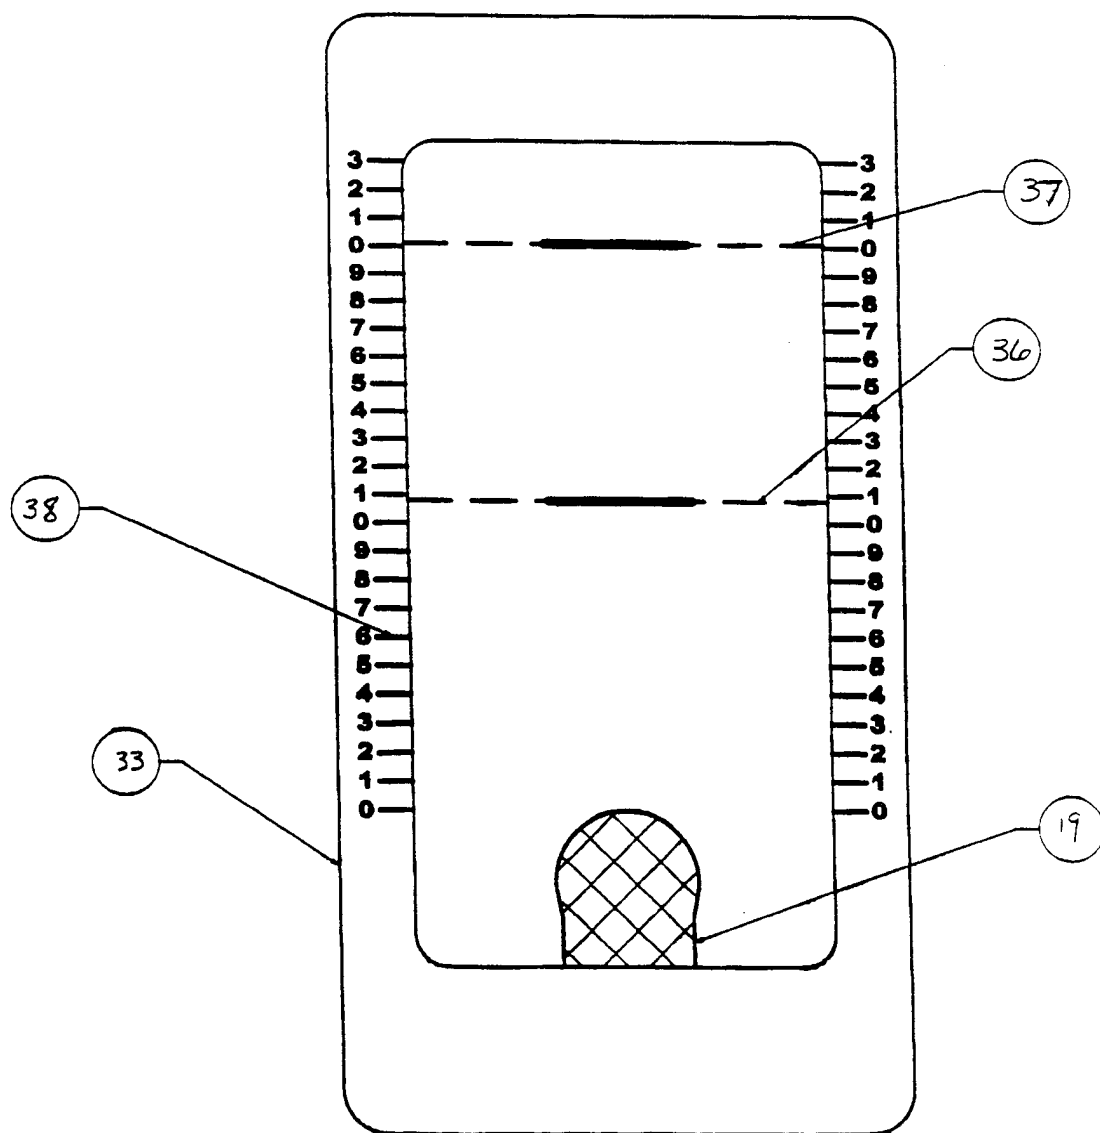


Figure 4

INTERNATIONAL SEARCH REPORT

Intern. Application No

PCT/US 98/04569

A. CLASSIFICATION OF SUBJECT MATTER
IPC 6 A61B8/08

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 6 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 96 35469 A (CARDIOGENESIS CORP) 14 November 1996 see page 12, line 1 - page 14, line 7; figures 1-4	1
Y	US 5 601 084 A (JIN HUAICHUAN ET AL) 11 February 1997 see abstract see column 7, line 38 - column 8, line 15; figure 2A	1
A	US 5 196 006 A (KLOPOTEK PETER J ET AL) 23 March 1993 see abstract; claims 1,4; figure 1	1-3
A	US 5 242 386 A (HOLZER ERIC) 7 September 1993 see column 4, line 14 - line 47; figure 1	1-4



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

° Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

15 June 1998

Date of mailing of the international search report

25.06.98

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Hansen, S

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/US 98/04569

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 345 940 A (SEWARD JAMES B ET AL) 13 September 1994 see column 4, line 25 - column 5, line 16; figures 1-3 ---	1-4
A	US 5 389 096 A (AITA MICHAEL ET AL) 14 February 1995 see column 3, line 27 - line 63; figures 1,2 -----	1

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 98/04569

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 5-13
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 98/04569

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9635469 A	14-11-1996	NONE	
US 5601084 A	11-02-1997	US 5435310 A	25-07-1995
US 5196006 A	23-03-1993	NONE	
US 5242386 A	07-09-1993	WO 9405343 A	17-03-1994
US 5345940 A	13-09-1994	US 5325860 A	05-07-1994
		US 5713363 A	03-02-1998
		US 5704361 A	06-01-1998
		CA 2121353 A	13-05-1993
		EP 0611292 A	24-08-1994
		JP 7505791 T	29-06-1995
		WO 9308738 A	13-05-1993
US 5389096 A	14-02-1995	NONE	