



US008324900B2

(12) **United States Patent**
Helvoort et al.

(10) **Patent No.:** **US 8,324,900 B2**
(45) **Date of Patent:** **Dec. 4, 2012**

(54) **MAGNETIC RESONANCE
INTEGRATED-CIRCUIT LOW-NOISE
AMPLIFIER**

(75) Inventors: **Marinus Johannes Adrianus Maria
Helvoort**, Eindhoven (NL); **Paulus
Cornelius Hendrikus Adrianus Haans**,
Eindhoven (NL); **Leo De Vreede**,
Eindhoven (NL)

(73) Assignee: **Koninklijke Philips Electronic N.V.**,
Eindhoven (NL)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 259 days.

(21) Appl. No.: **12/601,532**

(22) PCT Filed: **May 30, 2008**

(86) PCT No.: **PCT/IB2008/052113**

§ 371 (c)(1),
(2), (4) Date: **Nov. 24, 2009**

(87) PCT Pub. No.: **WO2008/146256**

PCT Pub. Date: **Dec. 4, 2008**

(65) **Prior Publication Data**

US 2010/0164498 A1 Jul. 1, 2010

(30) **Foreign Application Priority Data**

May 31, 2007 (EP) 07109257

(51) **Int. Cl.**
G01V 3/00 (2006.01)

(52) **U.S. Cl.** **324/322**; 324/318; 324/313; 324/310;
324/307; 324/314

(58) **Field of Classification Search** 324/300–322;
330/310, 295, 85, 110; 600/407–435; 382/128–131
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,996,658 A * 8/1961 Jimerson, Jr. et al. 324/310
2,999,976 A * 9/1961 Francis et al. 324/307
3,099,793 A * 7/1963 Pinkley 324/313

(Continued)

FOREIGN PATENT DOCUMENTS

DE 4037294 A1 7/1991

(Continued)

OTHER PUBLICATIONS

Cherifi, T., et al.; A CMOS Microcoil-associated Preamplifier for
NMR Spectroscopy; 2005; IEEE Trans. on Circuits and systems;
52(12)2576-2583.

(Continued)



Primary Examiner — Melissa Koval

Assistant Examiner — Tiffany Fetzner

(57) **ABSTRACT**

It is proposed herein to improve the specifications of a low-
noise amplifier (LNA) by integrating it in a chip. In order to
cover a range of operating frequencies using a single chip, the
integrated-circuit amplifier proposed herein comprises an
input port configured to receive a magnetic resonance (MR)
signal from a radio-frequency (RF) coil, one or more LNAs
configured to amplify the received MR signal, and an output
port configured to output the amplified MR signal from the
one or more LNAs. The operating frequency of the RF coil
depends on the field strength. The matching circuit, if present,
needs to be tuned to operate at the operating frequency of the
RF coil, and depends on the component values in the loop,
thus on loop size. In contrast, the proposed integrated-circuit
amplifier is capable of directly connecting to RF coils with
different loop sizes, without the need for a matching circuit.

18 Claims, 4 Drawing Sheets

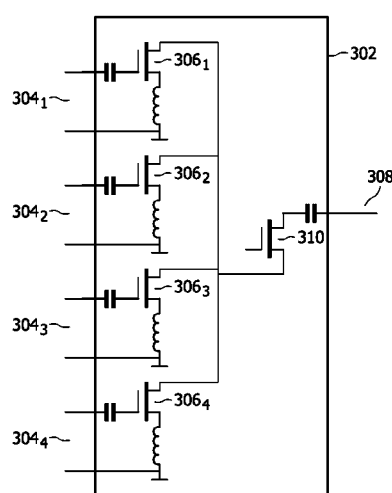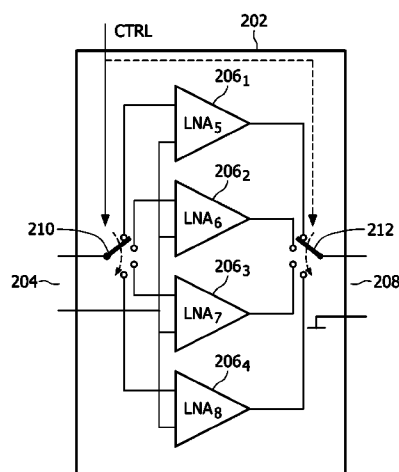

U.S. PATENT DOCUMENTS

3,122,702	A *	2/1964	Franken	324/304
3,174,099	A *	3/1965	Larson	324/310
3,418,564	A *	12/1968	Nelson	324/310
3,588,678	A *	6/1971	Ernst	324/310
3,860,818	A *	1/1975	Stalder et al.	250/343
4,629,987	A *	12/1986	King et al.	324/306
4,631,495	A *	12/1986	Mueller et al.	330/310
4,731,585	A *	3/1988	Fox	324/322
5,296,813	A	3/1994	Holmes et al.	
6,838,936	B2 *	1/2005	Oppelt	330/110
7,378,851	B1 *	5/2008	de Rooij et al.	324/322
7,646,249	B2 *	1/2010	Hajimiri et al.	330/297
7,652,476	B2 *	1/2010	de Rooij et al.	324/322
7,710,197	B2 *	5/2010	Aoki et al.	330/252
7,999,621	B2 *	8/2011	Hajimiri et al.	330/297
2003/0234684	A1 *	12/2003	Oppelt	330/85
2005/0001680	A1	1/2005	Ratzel	
2006/0033499	A1 *	2/2006	Flexman et al.	324/322
2006/0202699	A1 *	9/2006	Reiderman	324/339
2008/0136414	A1 *	6/2008	de Rooij et al.	324/322
2008/0136415	A1 *	6/2008	de Rooij et al.	324/322
2008/0211584	A1 *	9/2008	Hajimiri et al.	330/297

2009/0015328	A1 *	1/2009	Aoki et al.	330/252
2010/0164498	A1 *	7/2010	Helvoort et al.	324/322
2011/0091987	A1 *	4/2011	Weissleder et al.	436/173

FOREIGN PATENT DOCUMENTS

EP	0344293	B1	3/1995
EP	1521094	A1	4/2005
JP	08191813	A	7/1996
JP	09024036	A	1/1997
RU	2417745	C1 *	5/2011
WO	2006048816	A1	5/2006
WO	2007043009	A2	4/2007
WO	WO 2008146256	A2 *	12/2008

OTHER PUBLICATIONS

Girlando, G., et al.; Noise Figure and Impedance Matching in RF Cascode Amplifiers; 1999; IEEE Trans. on circuits and Systems; 46(11)1388-1396.
Texas Instruments; Information for Medical Applications; downloaded Jul. 11, 2006 <http://focus.ti.com/lit/ml/slyb108a/slyb108a.pdf> see p. 3 and 4.

* cited by examiner

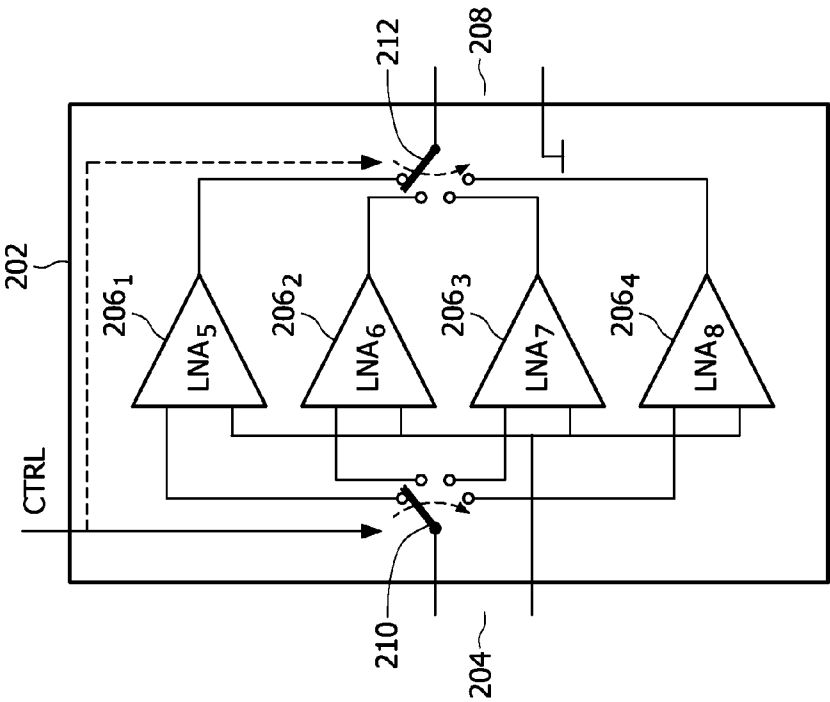


FIG. 1

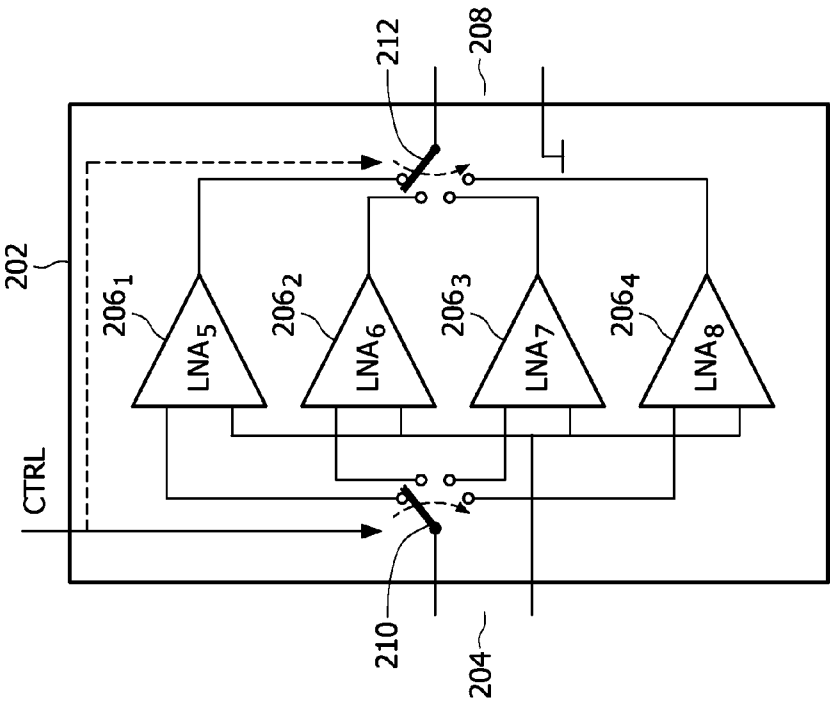


FIG. 2

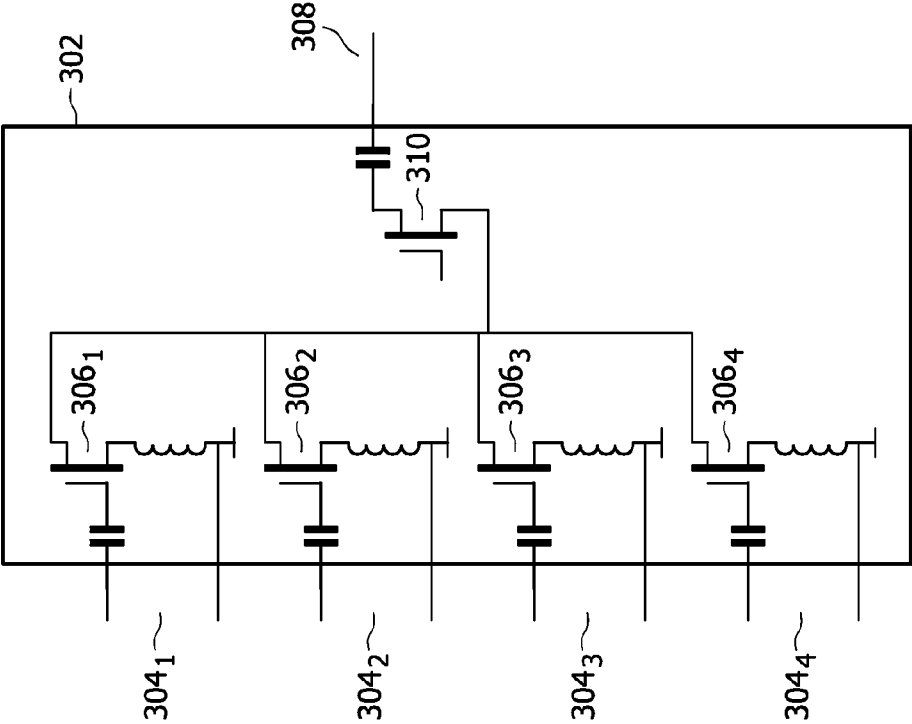


FIG. 3

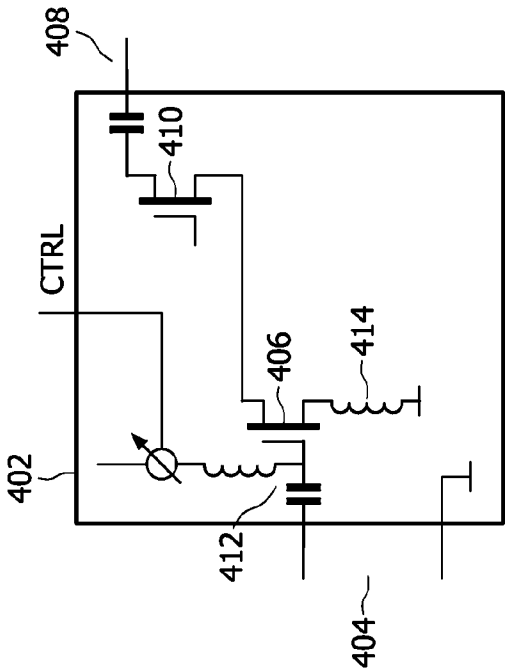


FIG. 4

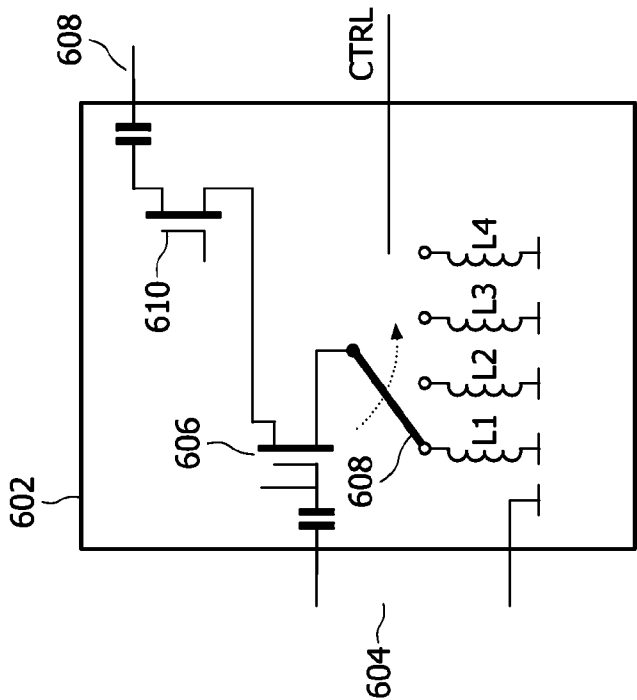


FIG. 5

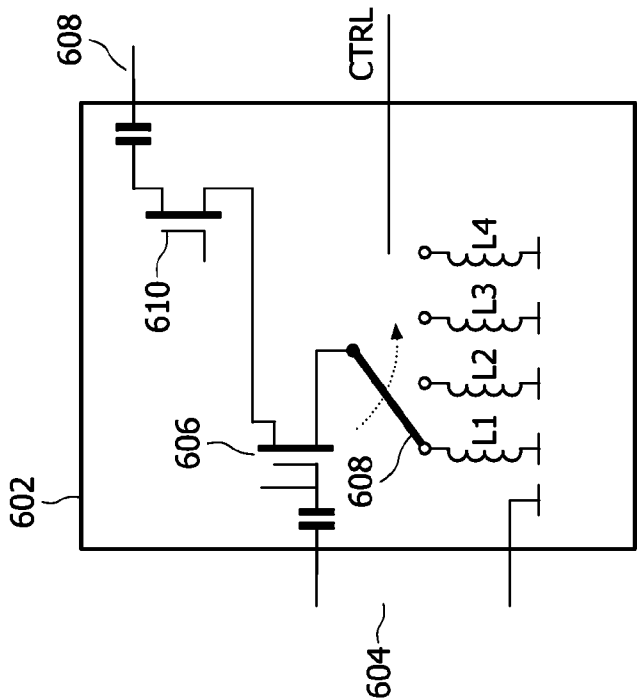


FIG. 6

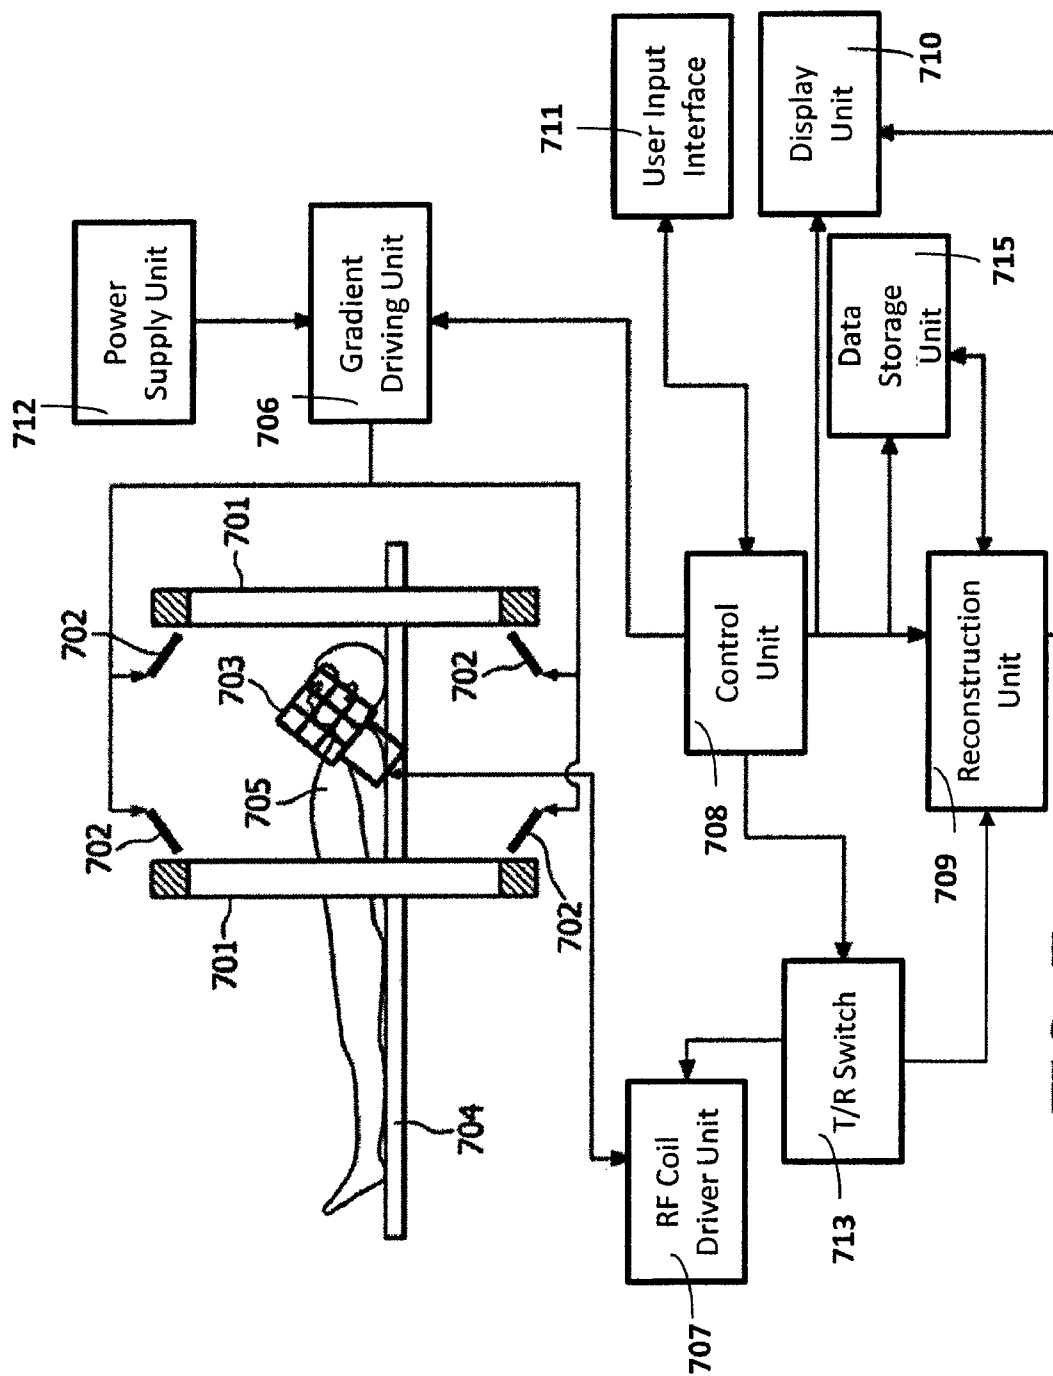


FIG. 7

1

MAGNETIC RESONANCE INTEGRATED-CIRCUIT LOW-NOISE AMPLIFIER

FIELD OF THE INVENTION

The invention relates to the field of low-noise amplifiers (LNA) for radio-frequency (RF) applications, and particularly to LNA devices for RF coils in a magnetic resonance (MR) system.

BACKGROUND OF THE INVENTION

The European patent application EP0344293B1 discusses a nuclear magnetic resonance signal acquisition apparatus that includes a coil, a matching means and a preamplifier. The coil has a source impedance (designated R_s in the aforementioned European patent application), while the preamplifier has an optimum source impedance R_{opt} and an input impedance R_{in} , with R_{in} being less than R_{opt} . The matching means connects the coil to the preamplifier such that the source impedance of the coil R_s is transformed by the matching means to be approximately equal to the optimum source impedance R_{opt} at the point of connection between the matching means and the preamplifier. At the same time, the low input impedance of the preamplifier is transformed by the matching means to be a value higher than the optimum source impedance R_{opt} at the point of connection between the matching means and the coil.

SUMMARY OF THE INVENTION

A matching means as described above could have fairly large dimensions which could add to the size of the integrated-circuit amplifier device. It could also add unwanted noise to the signal received by the coil itself. In addition, in the case of coils with multiple transmitting or receiving loops, e.g., phased-array coils, the matching means of one loop might couple with the B_1 transmit fields of other loops, and could also result in an increased number of parasitic loops.

It is therefore proposed herein to improve the specifications of the LNA by integrating it in a chip. In order to cover a range of operating frequencies using a single chip, the integrated-circuit amplifier proposed herein comprises an input port configured to receive an MR signal from an RF coil, one or more LNAs configured to amplify the received MR signal, and an output port configured to output the amplified MR signal from the one or more LNAs. The operating frequency of the RF coil is dependent on the field strength of the main magnetic field. The matching circuit, as mentioned in the prior art, needs to be tuned to operate at the operating frequency of the RF coil. The component values in the matching circuit depend on the loop size. In contrast, the proposed integrated-circuit amplifier is capable of directly connecting to RF coils with different loop sizes, without the need for a matching circuit.

BRIEF DESCRIPTION OF THE DRAWINGS

These and other aspects will be described in detail hereinafter, by way of example, on the basis of the following embodiments, with reference to the accompanying drawings, wherein:

FIG. 1 shows an embodiment of the integrated-circuit amplifier disclosed herein, wherein multiple LNAs are provided on a single chip with individual inputs and outputs for each LNA;

2

FIG. 2 shows a second embodiment of the integrated-circuit amplifier with multiple LNAs that are selectable based on a control signal;

FIG. 3 shows a third embodiment having multiple input ports and a single output port;

FIG. 4 shows a fourth embodiment wherein the LNA is formed from a field-effect transistor device, and wherein an additional bias voltage is applied;

FIG. 5 shows a fifth embodiment in which a feedback loop is added to the LNA;

FIG. 6 shows a sixth embodiment wherein a particular degenerating inductor is selected by a switch; and

FIG. 7 shows a magnetic resonance system utilizing an integrated-circuit amplifier as disclosed herein.

Corresponding reference numerals when used in the various figures represent corresponding elements in the figures.

DETAILED DESCRIPTION OF EMBODIMENTS

Phased-array coils, sometimes also referred to as "Synergy" coils, employ multiple receive loops simultaneously to receive MR signals from a subject under examination. Due to the proximity of the coil loops to one another, noise currents in one loop could couple to other loops. If each of the loops were connected to a high impedance, the flow of potentially problematic noise currents could be blocked.

Since the MR signals received by the loops are very weak, the signals need to be amplified in order to obtain reasonable image quality. LNAs are often used for amplifying the MR signals. However, currently known LNA topologies generate low noise only within a specific, small range of input impedances (optimal impedance Z_{opt}); in other words, outside of this range of input impedances, the noise levels generated by the LNA are high.

In general, there will be a mismatch between the requirements on the impedance seen by the loop and the optimal impedance at the input of the LNA. This problem is generally solved in phased-array or synergy coils by adding a transformer network (also known as a matching network) between the receive loop and the LNA. The disadvantage of adding a matching network is that it might add additional noise and could also take up significant space, which prevents miniaturization of the complete preamplifier assembly. In addition, the matching circuits themselves might mutually couple to each other, due to the high quality, core-less inductors needed in their construction.

FIG. 1 shows an embodiment in which the integrated-circuit amplifier 102 is formed on a single chip having several LNAs on-board. Four LNAs 106₁, 106₂, 106₃ and 106₄ are shown integrated on a single integrated-circuit amplifier chip 102. Each LNA 106₁, 106₂, 106₃ and 106₄ has its own input port 104₁, 104₂, 104₃ and 104₄, and its own output port 108₁, 108₂, 108₃ and 108₄, respectively.

As each LNA has its own separate input and output, it is possible to select the appropriate LNA by connecting a receive coil to the appropriate input port 104₁, 104₂, 104₃ or 104₄ of the integrated-circuit amplifier 102. In the exemplary embodiment shown in FIG. 1, the four different LNAs 106₁, 106₂, 106₃ and 106₄, have four different optimal input impedances, for example 20 Ohm, 54 Ohm, 9 Ohm and 22 Ohm, respectively. The operational frequency of the first two LNAs 106₁, 106₂ is 128 MHz, while that of the last two LNAs 106₃, 106₄ is 64 MHz. It is possible to have more LNAs on the same chip, operating at the above or other operational frequencies. It is also possible to have LNAs with other optimal input impedances as well.

3

The above design of the integrated-circuit amplifier permits an end-user, for example an imaging technician at a healthcare facility, to connect RF coils having various loop sizes (and therefore, operating at different resonance frequencies) to the same integrated-circuit amplifier by simply connecting the coil to the appropriate input **104**₁, **104**₂, **104**₃ or **104**₄, thereby selecting the appropriate LNA within the integrated-circuit amplifier chip **102**. Though this would be a useful item for clinical research sites, in the normal product these items are preassembled into a coil. The real customer value is improved image quality (as there is no noise added by the matching circuit), more compact coil design and less weight on the patient. For example, a cascode amplifier with a shunt inductor, manufactured using PHILIPS' CMOS 250 nm technology, makes it feasible to directly couple the RF receive loop to the LNA, without a matching network.

FIG. 2 shows an embodiment of the integrated-circuit amplifier disclosed herein, wherein the integrated-circuit amplifier **202** is configured as a single chip have multiple LNAs **206**₁, **206**₂, **206**₃ and **206**₄ on-board and with a single input **204** and single output **208**. The input stage of a particular LNA **206**₁, **206**₂, **206**₃ or **206**₄ is chosen by a low-loss multiplex or switching device **210**, for example a micro-electromechanical switch (MEMS). A similar switching device **212** could be used to connect the output stage of an LNA **206**₁, **206**₂, **206**₃ or **206**₄ to the output port **208** of the integrated-circuit amplifier **202**, if different output stages are beneficial. The MEMS or other switching or selector devices **210**, **212** are operated based on a control signal CTRL. It is also conceivable that different control signals are used to trigger the operation of the switching devices **210**, **212** at the input and output ports **204**, **208**, respectively.

As in the embodiment discussed above, the four different LNAs **206**₁, **206**₂, **206**₃ and **206**₄, have four different optimal input impedances, for example 20 Ohm, 54 Ohm, 9 Ohm and 22 Ohm, respectively. The operational frequency of the first two LNAs **206**₁, **206**₂ is 128 MHz, while that of the last two LNAs **206**₃, **206**₄ is 64 MHz. As in the above-mentioned embodiment, it is possible to have fewer or more than four LNAs on the same chip, operating at the above or other operational frequencies. It is also possible to have LNAs with other optimal input impedances as well.

FIG. 3 shows a single chip integrated-circuit amplifier **302** with a single output port **308** and multiple input ports **304**₁, **304**₂, **304**₃, **304**₄. Each input port connects to a different first stage amplifier **306**₁, **306**₂, **306**₃, **306**₄ such that each input (or combination of inputs) has a different optimal impedance. The various first stage amplifiers **306**₁, **306**₂, **306**₃, **306**₄ connect to a second stage amplifier **310**. Though only one second stage amplifier **310** is shown in this embodiment, it is possible to have multiple second stage amplifiers as well.

Both the first and second-stage amplifiers shown in this embodiment utilize field-effect transistors (FETs), though other implementations are also possible, such as one utilizing bipolar-junction transistors (BJTs). The advantage of using multiple input stages with different optimal impedances is that RF coils having different loop sizes can be connected directly to the same integrated-circuit amplifier **302**, by connecting the coil to the appropriate external pins. The inputs of the unused FETs are grounded externally and do not play a role in the circuit anymore. This implementation using FETs has the additional advantage that it requires less space and has fewer external pins than some of the other embodiments. It may be noted that the unused FETs may be left unbiased in order to attain improved power dissipation in the circuit.

FIG. 4 shows a single integrated-circuit amplifier chip **402**, with a single input port **404** and a single output port **408**. A

4

first-stage FET amplifier **406** has its source grounded internally via a degenerating inductor **414**, while its drain is connected to the source of a second-stage amplifier **410**. This "grounded-gate" configuration results in a low input impedance of the second-stage amplifier. Another way of achieving low input impedance is to use grounded-base bi-polar transistor amplifiers. The second-stage amplifier **410** converts an input current into an amplified output voltage at the output port **408**. A control signal CTRL supplied to the gate of the first stage FET amplifier **406** determines the input impedance of the integrated-circuit amplifier **402**. The input impedance may be controlled via adjustments in biasing (external controls) or with active and externally controlled feedback. In this embodiment the bias voltage supplied to the gate of the first-stage FET amplifier **406** is made adjustable via an external control signal CTRL, which results in the ability to control the input impedance of the LNA circuit over a limited range. This in turn, makes it possible to connect RF coils of various loop sizes (within a limited range) to the LNA. By incorporating multiple such LNAs in a single chip, the range of RF coils (i.e., loop sizes) that may be connected to the integrated-circuit amplifier may be increased.

FIG. 5 shows an integrated-circuit amplifier **502** having a single input port **504** and a single output port **508**. The source of the first-stage FET amplifier **506** is grounded internally via a degenerating inductor **514**, while its drain is connected to the source of a second-stage FET amplifier **510**. A feedback signal is added to the first-stage FET amplifier **506** by connecting its source to the drain of the second-stage FET amplifier **508** via a feedback amplifier **512**. The feedback response curve may be controlled externally via the control signal CTRL, and may be used to control the optimal frequency.

FIG. 6 shows an integrated-circuit amplifier **602** with a single input **604** and a single output **608**. The drain of a first-stage FET amplifier **606** is connected to the source of a second-stage FET amplifier **610**, while the source of the first-stage FET amplifier **606** is connected to one of a number of degenerating inductors **L1**, **L2**, **L3**, **L4**, via a switching mechanism **608**. This embodiment differs from the embodiment of FIG. 4 in that the inductor connected to the source of the first-stage FET is selectable. The switching mechanism may be a low-noise switch like a MEMS. The switching mechanism is controlled by a control signal CTRL which may be supplied externally.

Some of the advantages of integrating an LNA on a chip include less power consumption, which may be important especially for wireless coils, and less requirements for board-space, which may be especially important for the RF coils used in massive parallel imaging schemes. Several chip technologies exist that might be used for integrating the LNA as disclosed herein, like metal-oxide semiconductor (MOS) using either N-channel or P-channel FETs, complementary metal-oxide semiconductor (CMOS) using either N-channel or P-channel FETs, bipolar junction transistors (BJT) using bipolar devices, etc.

Though the embodiments of FIGS. 3, 4, 5 and 6 have been depicted as utilizing FETs, it is possible to replace the FETs with BJTs to arrive at alternate configurations having the same functionality. In such cases, the configurations utilizing BJTs may be directly derived from the FET configurations by replacing the words "drain, gate and source" for the FET with the words "collector, base and emitter", respectively for the BJT.

FIG. 7 shows a possible embodiment of an MR system capable of utilizing the integrated-circuit amplifier as disclosed herein. The MR system comprises a set of main coils **701**, multiple gradient coils **702** connected to a gradient driver

5

unit **706**, and RF coils **703** connected to an RF coil driver unit **707**. The function of the RF coils **703**, which may be integrated into the magnet in the form of a body coil, or may be separate surface coils, is further controlled by a transmit/receive (T/R) switch **713**. The multiple gradient coils **702** and the RF coils are powered by a power supply unit **712**. A transport system **704**, for example a patient table, is used to position a subject **705**, for example a patient, within the MR imaging system. A control unit **708** controls the RF coils **703** and the gradient coils **702**. The control unit **708**, though shown as a single unit, may be implemented as multiple units as well. The control unit **708** further controls the operation of a reconstruction unit **709**. The control unit **708** also controls a display unit **710**, for example a monitor screen or a projector, a data storage unit **715**, and a user input interface unit **711**, for example, a keyboard, a mouse, a trackball, etc.

The main coils **701** generate a steady and uniform static magnetic field, for example, of field strength 1T, 1.5T or 3T; the embodiments disclosed herein may be used at other field strengths as well. The main coils **701** are arranged in such a way that they typically enclose a tunnel-shaped examination space, into which the subject **705** may be introduced. Another common configuration comprises opposing pole faces with an air gap in between them into which the subject **705** may be introduced by using the transport system **704**. To enable MR imaging, temporally variable magnetic field gradients superimposed on the static magnetic field are generated by the multiple gradient coils **702** in response to currents supplied by the gradient driver unit **706**. The power supply unit **712**, fitted with electronic gradient amplification circuits, supplies currents to the multiple gradient coils **702**, as a result of which gradient pulses (also called gradient pulse waveforms) are generated. The control unit **708** controls the characteristics of the currents, notably their strengths, durations and directions, flowing through the gradient coils to create the appropriate gradient waveforms. The RF coils **703** generate RF excitation pulses in the subject **705** and receive MR signals generated by the subject **705** in response to the RF excitation pulses. The RF coil driver unit **707** supplies current to the RF coil **703** to transmit the RF excitation pulse, and amplifies the MR signals received by the RF coil **703**. The transmitting and receiving functions of the RF coil **703** or set of RF coils are controlled by the control unit **708** via the T/R switch **713**. The T/R switch **713** is provided with electronic circuitry that switches the RF coil **703** between transmit and receive modes, and protects the RF coil **703** and other associated electronic circuitry against breakthrough or other overloads, etc. The characteristics of the transmitted RF excitation pulses, notably their strength and duration, are controlled by the control unit **708**.

It is to be noted that though the transmitting and receiving coil are shown as one unit in this embodiment, it is also possible to have separate coils for transmission and reception, respectively. It is further possible to have multiple RF coils **703** for transmitting or receiving or both. The RF coils **703** may be integrated into the magnet in the form of a body coil, or may be separate surface coils. They may have different geometries, for example, a birdcage configuration or a simple loop configuration, etc. The control unit **708** is preferably in the form of a computer that includes a processor, for example a microprocessor. The control unit **708** controls, via the T/R switch **713**, the application of RF pulse excitations and the reception of MR signals comprising echoes, free induction decays, etc. User input interface devices **711** like a keyboard, mouse, touch-sensitive screen, trackball, etc., enable an operator to interact with the MR system.

6

The MR signal received with the RF coils **703** contains the actual information concerning the local spin densities in a region of interest of the subject **705** being imaged. The received signals are reconstructed by the reconstruction unit **709**, and displayed on the display unit **710** as an MR image or an MR spectrum. It is alternatively possible to store the signal from the reconstruction unit **709** in a storage unit **715**, while awaiting further processing. The reconstruction unit **709** is constructed advantageously as a digital image-processing unit that is programmed to derive the MR signals received from the RF coils **703**.

The various embodiments of the integrated-circuit amplifier disclosed herein are suitable for phased-array RF coils that employ multiple receive loops or elements. They are also suitable for other types of coils including one- or two-element coils, though in this case, the requirements regarding isolation of loops from one another are less strict.

It should be noted that the above-mentioned embodiments illustrate rather than limit the invention, and that those skilled in the art will be able to design many alternative embodiments without departing from the scope of the appended claims. In the claims, any reference signs placed between parentheses shall not be construed as limiting the claim. The word "comprising" does not exclude the presence of elements or steps other than those listed in a claim. The word "a" or "an" preceding an element does not exclude the presence of a plurality of such elements. The disclosed embodiments can be implemented by means of hardware comprising several distinct elements, or by means of a combination of hardware and software. In the system claims enumerating several means, several of these means can be embodied by one and the same item of computer readable software or hardware. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage.

The invention claimed is:

1. A magnetic resonance system comprising:
 - a radio-frequency coil; and
 - an integrated-circuit amplifier including:
 - a plurality of radio-frequency coils, each of the plurality of radio-frequency coils operating at a different impedance that requires different amplification;
 - a plurality of input ports, each of the plurality of input ports configured to receive the magnetic resonance signal from a corresponding radio-frequency coil;
 - one or more low-noise amplifiers configured to amplify the received magnetic resonance signal, wherein each of the one or more low-noise amplifiers correspond to one of the plurality of input ports and one of the plurality of radio-frequency coils; and
 - an output port configured to output the amplified magnetic resonance signal from the one or more low-noise amplifiers.
2. An integrated-circuit amplifier configured for amplifying a magnetic resonance signal received from a radio-frequency coil, the integrated-circuit amplifier comprising:
 - an input port configured to receive the magnetic resonance signal from the radio-frequency coil;
 - one or more low-noise amplifiers configured to amplify the magnetic resonance signal received from the input port;
 - a control port and a switch capable of connecting selectively to the one or more low-noise amplifiers, wherein a particular low-noise amplifier is selectable by activating the switch in response to a control signal supplied via the control port; and

7

an output port configured to output the amplified magnetic resonance signal from the one or more low-noise amplifiers.

3. The integrated-circuit amplifier of claim 2, including multiple input and output ports and a switching device configured to connect each of the one or more low-noise amplifiers to the output port,

wherein each low-noise amplifier is connected to a respective input port and output port, and wherein a particular low-noise amplifier is selectable by connecting to the respective input and output ports.

4. The integrated-circuit amplifier of claim 2, including multiple input ports and a single output port, wherein each low-noise amplifier is connected to a respective input port and to the single output port, and wherein a particular low-noise amplifier is selectable by connecting the radio-frequency coil to the respective input port.

5. The integrated-circuit amplifier of claim 2, wherein the low-noise amplifier is a field effect transistor device including:

a drain connected to the output port;
a gate connected to the input port; and
a source;

wherein at least one of an additional adjustable bias voltage is applied to the gate in order to control a gain of the low-noise amplifier within a limited range and the low-noise amplifier includes a feedback circuit connected from the drain to the source.

6. The integrated-circuit amplifier of claim 2, including a control port and two or more degenerating inductors selectable by a switch, wherein the low-noise amplifier is a bipolar junction transistor device including:

a collector connected to the output port;
a base connected to the input port; and an emitter; and
wherein the switch is configured to connect the emitter to a particular degenerating inductor based on a control signal applied to the control port.

7. The integrated-circuit amplifier of claim 2, including a control port and two or more degenerating inductors selectable by a switch, wherein the low-noise amplifier is a field effect transistor device including:

a drain connected to the output port;
a gate connected to the input port; and a source; and
wherein the switch is configured to connect the source to a particular degenerating inductor based on a control signal applied to the control port.

8. The integrated-circuit amplifier of claim 2, wherein the low-noise amplifier is a bipolar junction transistor device including:

a collector connected to the output port;

8

a base connected to the input port; and
an emitter

wherein at least one of an additional adjustable bias voltage is applied to the base in order to control a gain of the low-noise amplifier within a limited range and the low-noise amplifier includes a feedback circuit connected from the collector to the emitter.

9. The integrated-circuit amplifier of claim 2, wherein the one or more low-noise amplifiers are first stage amplifiers and further including:

a second stage amplifier connected to the one or more low-noise amplifiers.

10. An integrated-circuit amplifier configured for amplifying a magnetic resonance signal received from a radio-frequency coil, the integrated-circuit amplifier comprising:

an input port configured to receive the magnetic resonance signal from the radio-frequency coil;

one or more low-noise amplifiers configured to amplify the magnetic resonance signal received from the input port;

a switching device configured to connect each of the one or more low-noise amplifiers to an output port; and

an output port configured to output the amplified magnetic resonance signal from the one or more low-noise amplifiers.

11. The integrated-circuit amplifier of claim 10, wherein each of low-noise amplifiers have different optimal input impedances.

12. The integrated-circuit amplifier of claim 10, wherein the switching device includes a micro-electromechanical switch (MEMS).

13. The integrated-circuit amplifier of claim 12, wherein the MEMS is operated by a control signal.

14. The integrated-circuit amplifier of claim 10, wherein the one or more low-noise amplifiers are first stage amplifiers and further including:

a second stage amplifier connected to the one or more low-noise amplifiers.

15. The integrated-circuit amplifier of claim 14, wherein a drain of the one or more first stage amplifiers are connected to a source of the second stage amplifier.

16. The integrated-circuit amplifier of claim 14, wherein a bias voltage supplied to a gate of the one or more first stage amplifiers are adjustable via a control signal.

17. The integrated-circuit amplifier of claim 10, wherein each of the one or more first stage amplifiers are connected to a degenerating inductor via the switching device.

18. The integrated-circuit amplifier of claim 17, wherein each of the degenerating inductors are connected to a source of a corresponding first state amplifier.

* * * * *