

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
2 June 2005 (02.06.2005)

PCT

(10) International Publication Number  
**WO 2005/048887 A1**

(51) International Patent Classification<sup>7</sup>: **A61F 2/66**,  
2/68, 2/76

(21) International Application Number:  
PCT/CA2003/001802

(22) International Filing Date:  
18 November 2003 (18.11.2003)

(25) Filing Language: English

(26) Publication Language: English

(71) Applicant (for all designated States except US): **VIC-  
THOM HUMAN BIONICS INC.** [CA/CA]; 4780, rue  
Saint-Félix, Bureau 105, Saint-Augustin-de-Desmaures,  
Québec G3A 2J9 (CA).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **BEDARD, Stéphane**

[CA/CA]; 256, rue du Tonnelier, Saint-Augustin-de-Des-  
maures, Québec G3A 2K5 (CA). **ROY, Pierre-Olivier**  
[CA/CA]; 1242, rue Allard, Sainte-Foy, Québec G1W 3G1  
(CA).


(74) Agent: **BRITT, Katherine**; McCarthy Tétrault LLP,  
Patent Agent, 1170 Peel Street, Montréal, Québec H3B  
4S8 (CA).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU,  
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,  
CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE,  
GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR,  
KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK,  
MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT,  
RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR,  
TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (BW, GH,  
GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),  
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),

[Continued on next page]

(54) Title: INSTRUMENTED PROSTHETIC FOOT

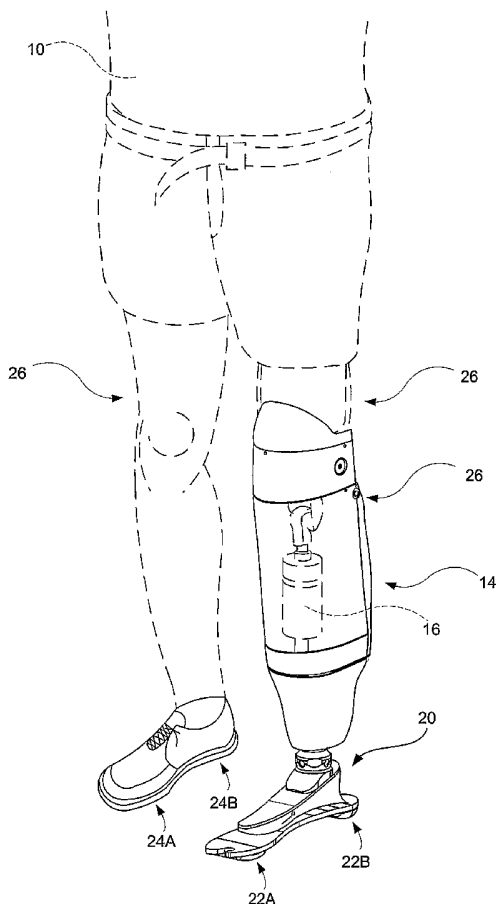

(57) Abstract: The present application discloses an instrument prosthetic foot (20) for use with an actuated leg prosthesis (14) controlled by a controller, the instrumented prosthetic foot (20) comprising a connector to connect the instrumented prosthetic foot (20) to the leg prosthesis (14), an ankle structure connected to the connector, a ground engaging member connected to the ankle, at least one sensor (22a, 22b, 24a, 24b, 26) for detecting changes in weight distribution along the foot, and an interface for transmitting signals from the sensor to the controller.



European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

**Published:**

— *with international search report*

## INSTRUMENTED PROSTHETIC FOOT

### BACKGROUND

As is well known to control engineers, the automation of complex mechanical systems is not something easy to achieve. Among such systems, conventional  
5 powered artificial limbs are notorious for having control problems. These conventional prostheses are equipped with basic controllers that artificially mobilize the joints without any interaction from the amputee and are only capable of generating basic motions. Such basic controllers do not take into consideration the dynamic conditions of the working environment, regardless the fact that the  
10 prosthesis is required to generate appropriate control within a practical application. They are generally lacking in predictive control strategies necessary to anticipate the artificial limb's response as well as lacking in adaptive regulation enabling the adjustment of the control parameters to the dynamics of the prosthesis. Because human limb mobility is a complex process including voluntary, reflex and random  
15 events at the same time, conventional prostheses do not have the capability to interact simultaneously with the human body and the external environment in order to have minimal appropriate functioning.

Accordingly, it is an object of the present application to obviate or mitigate some or all of the above disadvantages.

### SUMMARY

According to the present invention, there is provided an instrumented prosthetic foot for use with an actuated leg prosthesis controlled by a controller, the instrumented prosthetic foot comprising a connector to connect the instrumented  
20 prosthetic foot to the leg prosthesis, an ankle structure connected to the connector, a ground engaging member connected to the ankle, at least one  
25 sensor for detecting changes in weight distribution along the foot, and an interface for transmitting signals from the sensor to the controller.

## BRIEF DESCRIPTION OF THE FIGURES

Embodiments of the invention will be described by way of example only with reference to the accompanying drawings, in which:

FIG. 1 shows the lower body of an individual provided with a prosthesis and an instrumented prosthetic foot on one side and having a healthy leg on the other side.

FIG. 2 is a block diagram showing a control system for a prosthesis having an actuating mechanism.

FIG. 3 is a perspective view, from the front and slightly above, of a instrumented prosthetic foot.

FIG. 4 is an exploded perspective view of the instrumented prosthetic foot of FIG. 3.

FIG. 5 is a perspective view, from the front and slightly above, of an alternative embodiment of the instrumented prosthetic foot of FIG. 3.

FIG. 6 is an exploded perspective view of the instrumented prosthetic foot of FIG. 5.

FIG. 7 is a perspective view, from the front and slightly above, of another alternative embodiment of the instrumented prosthetic foot of FIG. 3

FIG. 8 is an exploded perspective view of the instrumented prosthetic foot of FIG. 7.

FIG. 9 is schematic view of forces exerted on a foot.

FIG. 10 is a perspective view, from the front and slightly above, of a further still alternative embodiment of the instrumented prosthetic foot of FIG. 3

FIG. 11 is an exploded perspective view of the instrumented prosthetic foot of FIG. 10.

FIG. 12 is a perspective view, from the front and slightly above, of a yet further still alternative embodiment of the instrumented prosthetic foot of FIG. 3

FIG. 13 is an exploded perspective view of the instrumented prosthetic foot of FIG. 12.

5 FIG. 14 is a perspective view, from the front and slightly above, of a further alternative embodiment of the instrumented prosthetic foot of FIG. 3

FIG. 15 is an exploded perspective view of the instrumented prosthetic foot of FIG. 14.

#### DETAILED DESCRIPTION

10 The appended figures show a instrumented prosthetic foot (20) having sensors (22A, 22B) for use, in cooperation with possible additional sensors (24A, 24B, 26), with a control system (100) for controlling a prosthesis (14) having an actuating mechanism (16). It should be understood that the present invention is not limited to the illustrated implementation since various changes and modifications may be  
15 effected herein without departing from the scope of the appended claims.

Referring therefore to FIG. 1 an individual (10) has a pair of legs (26) and (28), one of which, (26), is amputated above the knee. A prosthesis (14) is attached to the leg (26) and includes an actuating mechanism (16), which may be either passive or active. An instrumented prosthetic foot (20) is attached to the  
20 prosthesis (14) and includes sensors (22A, 22B). Additional sensors (24A, 24B) are located on the healthy foot and additional sensors (26) located on the individual (10) and/or the prosthesis (14). A passive actuating mechanism may be generally defined as an electro-mechanical component that only absorbs mechanical energy in order to modify dynamics of mechanical joints of the  
25 prosthesis, while an active actuating mechanism may be generally defined as an electro-mechanical component that absorbs and supplies mechanical energy in order to set dynamics of mechanical joints of the prosthesis.

An example of a passive actuating mechanism is described in U.S. patent application No. 09/767,367, filed January 22, 2001, entitled "ELECTRONICALLY CONTROLLED PROSTHETIC KNEE". Examples of active actuating mechanisms are described in U.S. patent application No. 10/463,495 filed June 17, 2003, entitled "ACTUATED PROSTHESIS FOR ABOVE-KNEE AMPUTEES", by Stéphane Bédard et al., the entire disclosure of which is hereby incorporated by reference herein.

The prosthesis (14) is controlled, as shown schematically in FIG. 2, by a basic control system (100) comprising sensors (22A, 22B, 24A, 24B, 26), connected through an interface (30) to a controller (40). The controller (40) provides signals to an actuating mechanism (16) in the prosthesis (14), such as shown in FIG. 1. The purpose of the control system (100) is to provide the required signals for controlling the actuating mechanism (16). To do so, the control system (100) is interfaced with the amputee (10) using sensors (22A, 22B, 24A, 24B, 26) to ensure proper coordination between the amputee (10) and the movements of the prosthesis (14). The sensors (22A, 22B, 24A, 24B, 26) capture information, in real time, about the dynamics of the amputee's movement and provide that information to the controller (40) via the interface (30). The controller (40) then uses the information to determine the resistance to be applied to a joint, in the case of a passive actuating mechanism, or the joint trajectories and the required angular force or torque that must be applied by a joint, in the case of an active actuating mechanism, in order to provide coordinated movements.

The sensors (22A, 22B, 24A, 24B, 26) may include myoelectric sensors, neuro-sensors, kinematic sensors, kinetic sensors, strain gauges or plantar pressure sensors. Myoelectric sensors are electrodes used to measure the internal or the external myoelectrical activity of skeletal muscles. Neuro-sensors are electrodes used to measure the summation of one or more action potentials of peripheral nerves. Kinematic sensors are used to measure the position of articulated joints, the mobility speed or acceleration of lower extremities. Kinetic sensors are used to measure angular forces at articulated joints or reaction forces of lower extremities. Strain gages are used to measure the strain forces at a specific

underfoot area. Plantar pressure sensors are used to measure the vertical plantar pressure of a specific underfoot area. Of course, additional types of sensors which provide various information about dynamics of human locomotion may be used. For a given application, the use of sensors (22A, 22B, 24A, 24B, 26) is not  
5 restricted to a specific type of sensor, multiple types of sensors in various combinations may be used.

As illustrated in FIG. 1, the sensors (22A, 22B, ) may comprise localized plantar pressure sensors located at spaced locations on the prosthetic foot (20) to measure the vertical plantar pressure of a specific underfoot area. Similarly, the  
10 plantar pressure sensors (24A, 24B) located on the side of the healthy foot may be provided at spaced locations in a custom-made insole, preferably in the form of a standard orthopaedic insole, that is modified to embed the two sensors (24A, 24B) for the measurement of two localized plantar pressures. The sensors (22A, 22B, 24A, 24B) are operable to measure the weight transfer along the foot as the  
15 individual moves which may be combined with other sensors (26) such as kinematic sensors to measure the angular speed of body segments of the lower extremities and kinematic sensors to measure the angle of the prosthesis (14) knee joint.

Each sensor (22A, 22B, 24A, 24B) may comprise a thin Force-Sensing Resistor  
20 (FSR) polymer cell directly connected to the interface (30) of the control system (100) or indirectly using an intermediary system (not shown), for instance a wireless emitter. Of course, other types of communication link technologies may be used, such as, for example, optical. The FSR cell has a decreasing electrical resistance in response to an increasing force applied perpendicularly to the  
25 surface thereof. Each cell outputs a time variable electrical signal for which the intensity is proportional to the total vertical plantar pressure over its surface area. The size and position of the plantar pressure sensors (22A, 22B, 24A, 24B) may be defined in accordance with the stability and the richness (intensity) of the localized plantar pressure signals provided by certain underfoot areas during  
30 locomotion. For example, it was found by experimentation that the heel and the toe regions are two regions of the foot sole where the Plantar Pressure Maximum

Variation (PPMV) may be considered as providing a signal that is both stable and rich in information.

Accordingly, the controller (40) may use the data signals from the four localized plantar pressure sensors (22A, 22B, 24A, 24B), as well as the information gathered from the data signals of the other sensors (26) such as kinematic sensors, in order to decompose the locomotion of the individual (10) into a finite number of states, and generate the appropriate control signals for controlling the actuating mechanism (16) according to the locomotion. Of course, the controller (40) is not limited to the use of the preceding data signals.

10 An example of a controller (40) and control system (100) using sensors comprising plantar pressure sensors as well as kinematic sensors is described in U.S. patent application No. 10/600,725 filed June 20, 2003, entitled "CONTROL SYSTEM AND METHOD FOR CONTROLLING AN ACTUATED PROSTHESIS", by Stéphane Bédard, the entire disclosure of which is hereby incorporated by reference herein.

To facilitate the acquisition of the data in a repeatable and dependable manner, the sensors (22A, 22B) are incorporated in to the structure of the foot (20). An embodiment of the instrumented prosthetic foot (20) is shown in more detail in FIGS 3 and 4. The instrumented prosthetic foot (20) includes a foot plate (53), forming an elongated body, with a connector (51) at one end, a toe plate (55A) and a heel plate (55B) that is cantilevered from the foot plate (53). Such an arrangement is provided by, for example, a Vari-Flex® prosthetic foot from Össur. Pressure sensors (22A, 22B) are located at longitudinally spaced locations on the underside of the foot plate (53) and heel plate (55) respectively. The sensors (22A, 22B) are covered by rigid plates (52A, 52B) and resilient pads (54A, 54B). The pressure sensors (22A, 22B) are located so as to be responsive to loads imposed on the instrumented prosthetic foot (20) at the regions corresponding to the toe area and the heel area respectively.

The rigid plates (52A, 52B) covering the sensors (22A, 22B), although not essential, help to optimize the pressure distribution on the entire surface of the

sensors (22A, 22B) as well as inhibiting any shearing and may be made of 85A durometer polyurethane. Of course, other type of material may be used as well.

The pads (54A, 54B) wrap up the rigid plates (52A, 52B) and the sensors (22A, 22B), forming a ground engaging member, in order to optimize the contact  
5 between the instrumented prosthetic foot (20) and the ground. The pads (54A, 54B) may be made of 40A durometer polyurethane. Of course, other type of material may be used as well.

In operation, therefore, as the foot (20) traverses the ground, the force applied to the heel plate (55B) is measured by the sensor (22B) and a corresponding signal  
10 forwarded to the controller (40). The force applied to the toe plate (55A) is also measured by the sensor (22A) and the relative loading between the two locations is measured. As the foot (20) continues to traverse the ground, the force applied to the toe area increases and that at the heel decreases to provide a pair of signals from which the disposition of the leg may be determined and the  
15 appropriate control provided to the actuator (16).

An alternative embodiment of the instrumented prosthetic foot (20) is shown in FIGS 5 and 6. The instrumented prosthetic foot (20) includes connector (61), foot plate (63), toe plate (64A) and heel plate (64B), such as provided by, for example, a Vari-Flex® prosthetic foot from Össur. Pressure sensors (22A, 22B) are located  
20 between the foot plate (63) and rigid plates (62A, 62B). The pressure sensors (22A, 22B) are located so as to be responsive to load imposed on the instrumented prosthetic foot (20) at the regions corresponding to the toe area and the heel area respectively. More specifically, pressure sensor (22A) is sandwiched between a pair of rigid plates (62A), which in turn are positioned  
25 between the heel plate (64B) and the foot plate (63). Pressure sensor (22B) is sandwiched between a pair of rigid plates (62B), which in turn are positioned between the foot plate (63) and the connector (61).

As for the previous embodiment, rigid plates (62A, 62B) covering the sensors (22A, 22B), although not essential, help to optimize the pressure distribution on  
30 the entire surface of the sensors (22A, 22B) as well as inhibiting any shearing and

may be made of 85A durometer polyurethane. Of course, other type of material may be used as well.

Another alternative embodiment of the instrumented prosthetic foot (20) is shown in FIGS 7 and 8. The instrumented prosthetic foot (20) includes connector (71),  
5 top foot plate (75), foam cushion core (73) and bottom foot plate (74), such as provided by, for example, a LP Talux® prosthetic foot from Össur. Pressure sensors (22A, 22B) are sandwiched between pairs of rigid plates (72A, 72B). The pressure sensors (22A, 22B) are located so as to be responsive to load imposed on the instrumented prosthetic foot (20) at the regions corresponding to the toe  
10 area and the heel area respectively. More specifically, pressure sensor (22A) is sandwiched between a pair of rigid plates (72A), which in turn are positioned within gap (76A), which is located between a bottom foot plate (74) and a foam cushion core (73). Pressure sensor (22B) is sandwiched between a pair of rigid plates (72B), which in turn are positioned within gap (76B), which is located within  
15 the foam cushion core (73).

Again, as for the previous embodiments, rigid plates (72A, 72B) covering the sensors (22A, 22B), although not essential, help to optimize the pressure distribution on the entire surface of the sensors (22A, 22B) as well as preventing any shearing and may be made of 85A durometer polyurethane. Of course, other  
20 type of material may be used as well.

In the previous embodiments, the force (or pressure) at the toe and heel areas,  $F_{\text{toe}}$  and  $F_{\text{heel}}$  respectively, was obtained by positioning pressure sensors (22A, 22B) directly at those areas. More specifically, referring to FIG. 9,  $F_{\text{toe}}$  and  $F_{\text{heel}}$  were obtained as follows:

$$25 \quad F_{\text{toe}} = F_{\text{toe\_meas}} \quad \text{Equation 1}$$

$$F_{\text{heel}} = F_{\text{heel\_meas}} \quad \text{Equation 2}$$

In other possible embodiments of the instrumented prosthetic foot (20), sensors (22A, 22B) may not be restricted to being positioned directly at the toe and heel

areas, the equivalent information may be obtained by measuring the equivalent torque at the ankle and the axial force at the connector of the instrumented prosthetic foot (20).  $F_{\text{toe}}$  and  $F_{\text{heel}}$  may be defined in terms of the torque measured at the ankle,  $M_{\text{ankle\_meas}}$ , and the force measured at the connector,

5  $F_{\text{conn\_meas}}$ , using the following equations:

$$F_{\text{toe}} = \frac{M_{\text{ankle\_meas}} + (F_{\text{conn\_meas}} \cdot l_{\text{heel}})}{(l_{\text{heel}} + l_{\text{toe}})} \quad \text{Equation 3}$$

$$F_{\text{heel}} = \frac{-M_{\text{ankle\_meas}} + (F_{\text{conn\_meas}} \cdot l_{\text{toe}})}{(l_{\text{heel}} + l_{\text{toe}})} \quad \text{Equation 4}$$

where

10  $l_{\text{heel}}$  is the distance between the center of the connector and the center of the heel area;

$l_{\text{toe}}$  is the distance between the center of the connector and the center of the toe area.

Following the previous discussion about the locations of sensors (22A, 22B), a further alternative embodiment of the instrumented prosthetic foot (20) is shown in  
 15 FIGS 10 and 11. The instrumented prosthetic foot (20) includes connector (81), foot plate (83), toe plate (84A) and heel plate (84B), such as provided by, for example, a Vari-Flex® prosthetic foot from Össur, and load cells (22A, 22B). Load cells (22A, 22B) are located below connector (91), load cell (22A) being slightly biased towards the toe area of the foot and load cell (22B) being slightly biased  
 20 towards the heel area. Since the sensors (22A, 22B) are not located directly at the toe and heel areas, **Equation 3** and **Equation 4** may be used, for example by controller (40), to compute the equivalent pressures at the toe and heel areas by defining the equivalent torque at the ankle and the axial force at connector (81) as follows:

$$25 \quad F_{\text{conn\_meas}} = F_{\text{22B}} + F_{\text{22A}} \quad \text{Equation 5}$$

$$M\_ankle\_meas = F\_22B \cdot l\_22B - F\_22A \cdot l\_22A \quad \text{Equation 6}$$

where

$F\_22B$  is the force measured at sensor 22B;

$F\_22A$  is the force measured at sensor 22A;

5  $l\_22B$  is the distance between the center of the connector (81) and the center of sensor 22B;

$l\_22A$  is the distance between the center of the connector (81) and the center of sensor 22A.

In the previous embodiments of the instrumented prosthetic foot (20), the force (or pressure) at the toe and heel areas,  $F\_toe$  and  $F\_heel$  respectively, was obtained  
 10 either by positioning pressure sensors (22A, 22B) directly at those areas or by positioning pressure sensors or load cells (22A, 22B) in other areas and obtaining the equivalent information by computing the equivalent torque at the ankle and the axial force at the connector. Other types of sensors may also be used to obtain  
 15 the equivalent torque at the ankle and the axial force at the connector. Such an example is illustrated by a further still embodiment of the instrumented prosthetic foot (20), which is shown in FIGS 12 and 13. The instrumented prosthetic foot (20) includes connector (91), mounted on pivoting ankle (93). Bumpers (92A, 92B) are positioned between the pivoting ankle (93) and rocker plate (95) located  
 20 on a foot plate (94). The pivoting ankle (93) is connected to the rocker plate (95) by a pivot pin (96). Such an arrangement is provided by, for example, an Elation® prosthetic foot from Össur. A load cell (22A) and an optical encoder (22B). are incorporated into the foot (20) to provide measurement of the distribution of forces along the foot (20). Load cell (22A) is positioned between connector (91) and  
 25 pivoting ankle (93). Optical encoder (22B) comprises reader (221) and disk (223). Reader (221) is located on pivoting ankle (93) while disk (223) is located on rocker plate (95) and encircles pivot pin (96). Once again, **Equation 3** and **Equation 4** may be used, for example by controller (40), to compute the equivalent pressures

at the toe and heel areas by defining the equivalent torque at the ankle and the axial force at connector (91) as follows:

$$F_{\text{conn\_meas}} = F_{22A} \quad \text{Equation 7}$$

$$M_{\text{ankle\_meas}} = R_{\text{ankle\_meas}} \cdot R_{\text{const}} \quad \text{Equation 8}$$

5 where

$F_{22A}$  is the force measured at sensor 22A;

$R_{\text{ankle\_meas}}$  is the rotation measurement of pivoting ankle (93) about pivot pin (96) as measured by optical encoder (22B);

10  $R_{\text{const}}$  is a constant associated with the resistance of bumpers (92A, 92B) to compression, which constant varies depending in the material used.

A yet further alternative embodiment of the instrumented prosthetic foot (20) is shown in FIGS 14 and 15. The instrumented prosthetic foot (20) includes connector (101), mounted on pivoting ankle (103). Bumpers (102A, 102B) are positioned between the pivoting ankle (103) and rocker plate (105) located on a foot plate (104). The pivoting ankle (103) is connected to the rocker plate (105) by a pivot pin (106). Such an arrangement is provided by, for example, an Elation® prosthetic foot from Össur. Pressure sensors (22A, 22B) and load cell (22C) are incorporated into the foot (20) to provide measurement of the distribution of forces along the foot (20). Pressure sensor (22A) is positioned between rocker plate (85) and bumper (82A) while pressure sensor (22B) is positioned between rocker plate (85) and bumper (82B). A load cell (22C) is positioned between connector (91) and pivoting ankle (93).

25 In this embodiment, **Equation 6** is used to compute the equivalent torque at the ankle, while the axial force at connector (101) is computed using the following equation:

$$F_{\text{conn\_meas}} = F_{\text{22C}}$$

**Equation 9**

Load cell (22C) is required to compute the axial force at connector (101) since when there is no torque at the ankle, i.e. the wearer of the prosthesis is standing still, the axial force is being exerted in its entirety onto pivot pin (96).

- 5 In all of the described embodiments, the sensors (22A, 22B) may be directly connected to interface (30) of control system (100) or indirectly using an intermediary system (not shown), for instance a wireless emitter. Of course, other types of communication link technologies may be used, such as, for example, optical.
- 10 Other types of non-articulated or articulated prosthetic foot may be used as well as long as the selected prosthetic foot provides approximately the same dynamical response as the ones mentioned here above. Nevertheless, an articulated foot offers the best performances. The instrumented prosthetic foot (20) may further have an exposed metal or composite structure or it may have a cosmetic covering
- 15 that gives it the appearance of a human ankle and foot.

It should be noted that the present invention is not limited to its use with the mechanical configuration illustrated in FIG. 1 or the control system (100) illustrated in FIG. 2. It may be used with a leg prosthesis having more than one joint. For instance, it may be used with a prosthesis having an ankle joint, a

- 20 metatarsophalangeal joint or a hip joint in addition to a knee joint. Moreover, instead of a conventional socket a osseo-integrated devices could also be used, ensuring a direct attachment between the mechanical component of the prosthesis and the amputee skeleton. Other kinds of prostheses may be used as well.

## WHAT IS CLAIMED IS:

1. An instrumented prosthetic foot for use with an actuated leg prosthesis controlled by a controller, the instrumented prosthetic foot comprising:  
  
an elongated body having a top and a bottom part;  
  
a connector to connect the instrumented prosthetic foot to the leg prosthesis, the connector being attached to the top part of the elongated body;  
  
a ground engaging member attached to the bottom part of the elongated body;  
  
at least one sensor for detecting changes in weight distribution along the foot; and  
  
an interface for transmitting signals from the sensor to the controller.
2. An instrumented prosthetic foot according to claim 1, wherein:  
  
the ground engaging member includes a pair of basic underfoot locations, the first region corresponding to the heel area of the human foot and second region corresponding to the toe area of the human foot.
3. An instrumented prosthetic foot according to claim 2, wherein:  
  
at least two sensors are provided, one of the sensors being associated with each basic underfoot locations of the ground engaging member.
4. An instrumented prosthetic foot according to claim 3, wherein:  
  
the sensors include a strain sensor to measure the strain applied at a corresponding basic underfoot location of the ground engaging member.
5. An instrumented prosthetic foot according to claim 3, wherein:

the sensors include a pressure sensor to measure the pressure applied at a corresponding basic underfoot location of the ground engaging member.

6. An instrumented prosthetic foot according to claim 3, wherein:

the sensors include a load cell to measure the pressure applied at a corresponding basic underfoot location of the ground engaging member.

7. An instrumented prosthetic foot according to claim 3, wherein:

the sensors are positioned under the ground engaging member.

8. An instrumented prosthetic foot according to claim 3, wherein:

the sensors are positioned between the ground engaging member and the elongated body.

9. An instrumented prosthetic foot according to claim 3, wherein:

the sensors are positioned between the elongated body and the connector.

10. An instrumented prosthetic foot according to claim 5, wherein:

the pressure sensor is a force-sensing resistor.

11. An instrumented prosthetic foot according to claim 5, further comprising:

a rigid plate placed on at least one side of the sensor.

12. An instrumented prosthetic foot according to claim 11, further comprising:

a resilient pad covering the rigid plate and the sensor.

13. An instrumented prosthetic foot according to claim 1, further comprising:

an ankle structure pivotally connecting the elongated body to the connector.

14. An instrumented prosthetic foot according to claim 13, wherein:  
  
at least two sensors are provided, the sensors including two load cells positioned between the connector and the ankle structure.
15. An instrumented prosthetic foot according to claim 13, wherein:  
  
at least two sensors are provided, the sensors including an optical encoder and a load cell, the optical encoder being positioned on the ankle structure about its pivot axis with the elongated body and the load cell being positioned between the ankle structure and the connector.
16. An instrumented prosthetic foot according to claim 1, wherein:  
  
the interface for transmitting signals from the sensor to the controller is a wired connection.
17. An instrumented prosthetic foot according to claim 1, wherein:  
  
the interface for transmitting signals from the sensor to the controller is a wireless connection.
18. An instrumented prosthetic foot according to claim 1, further comprising:  
  
means for removably connecting the instrumented prosthetic foot to the leg prosthesis.

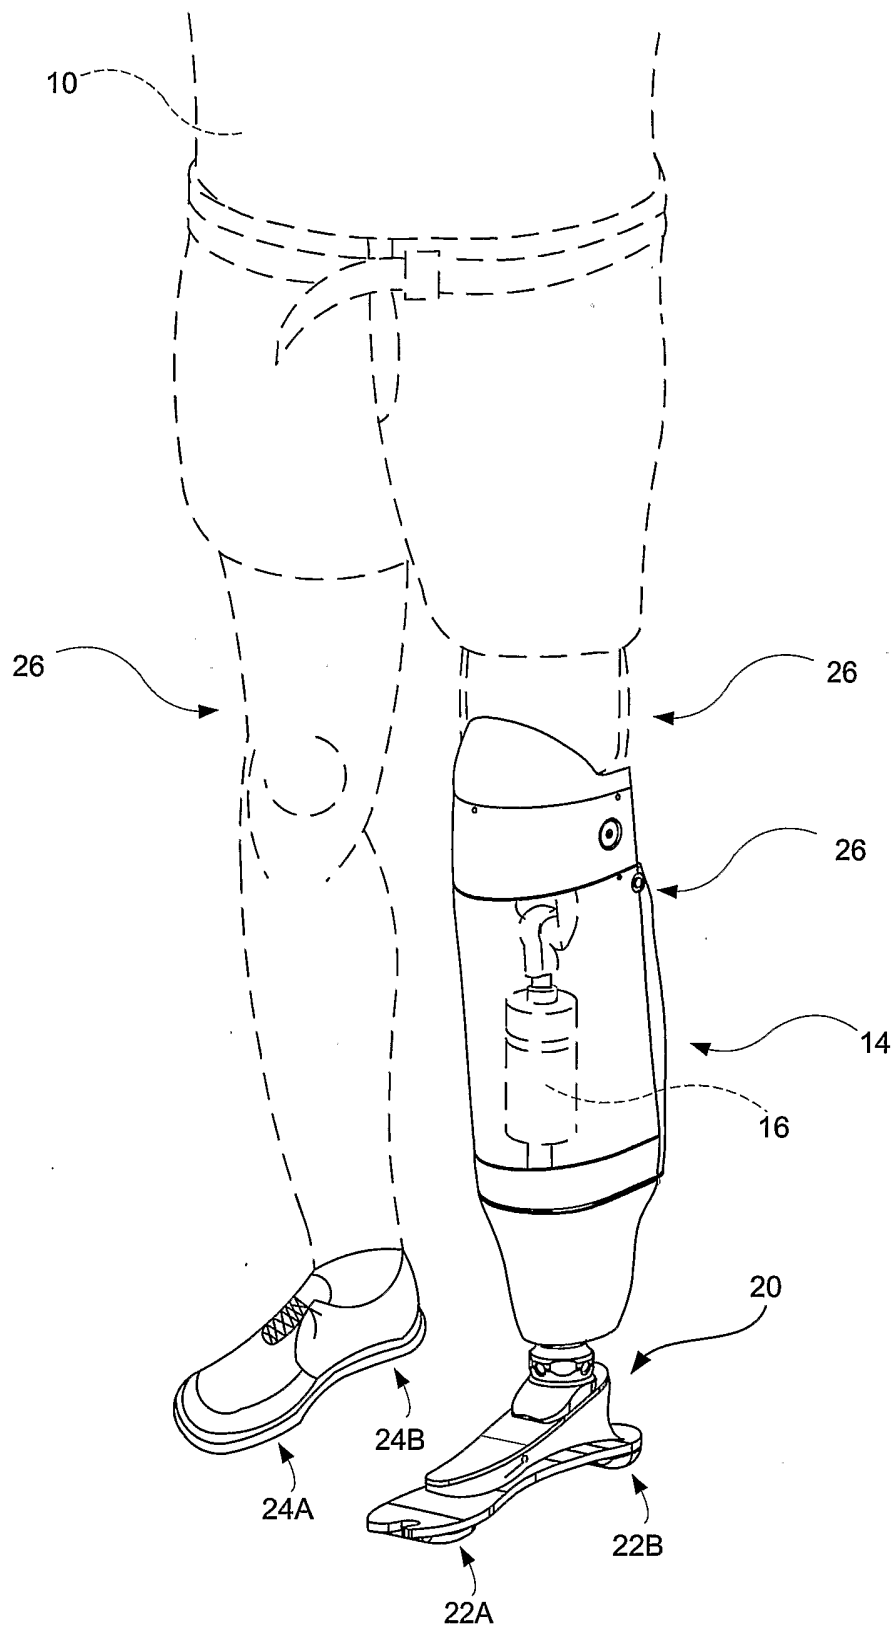


FIG. 1

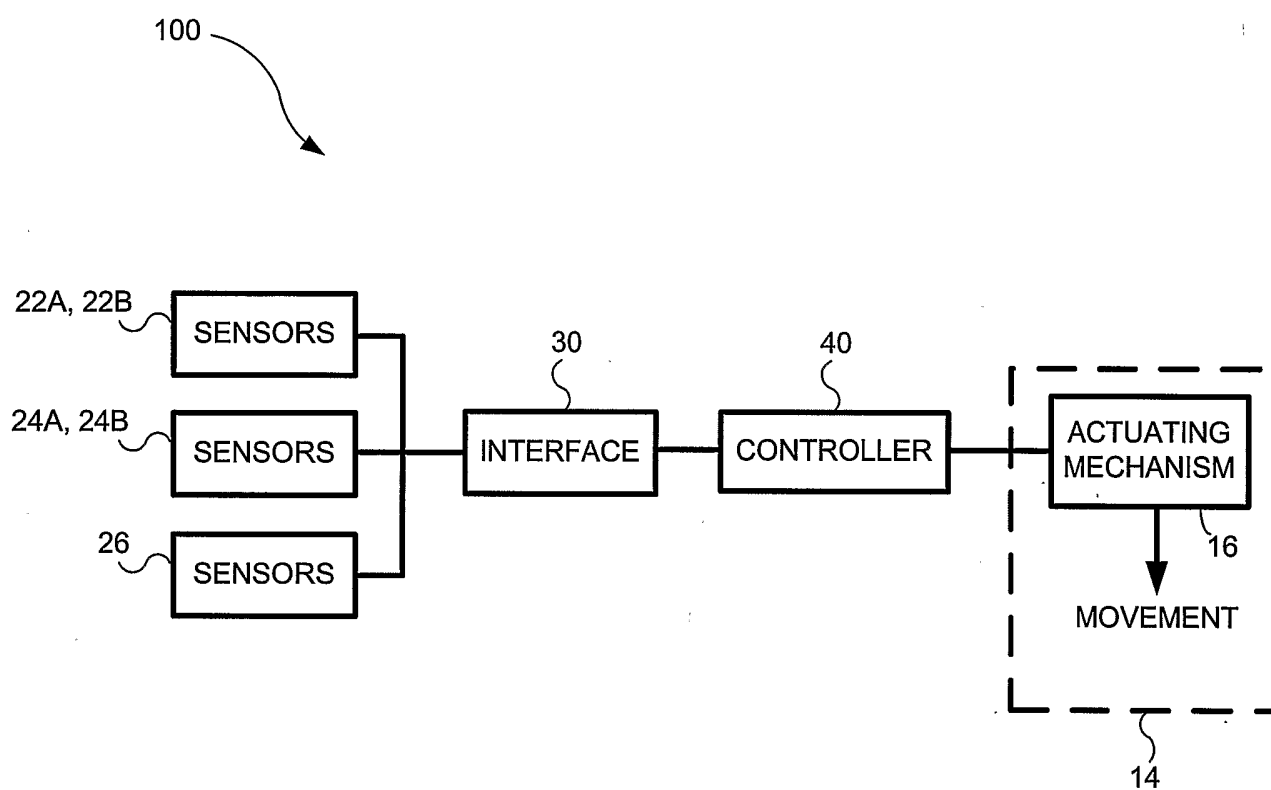


FIG. 2

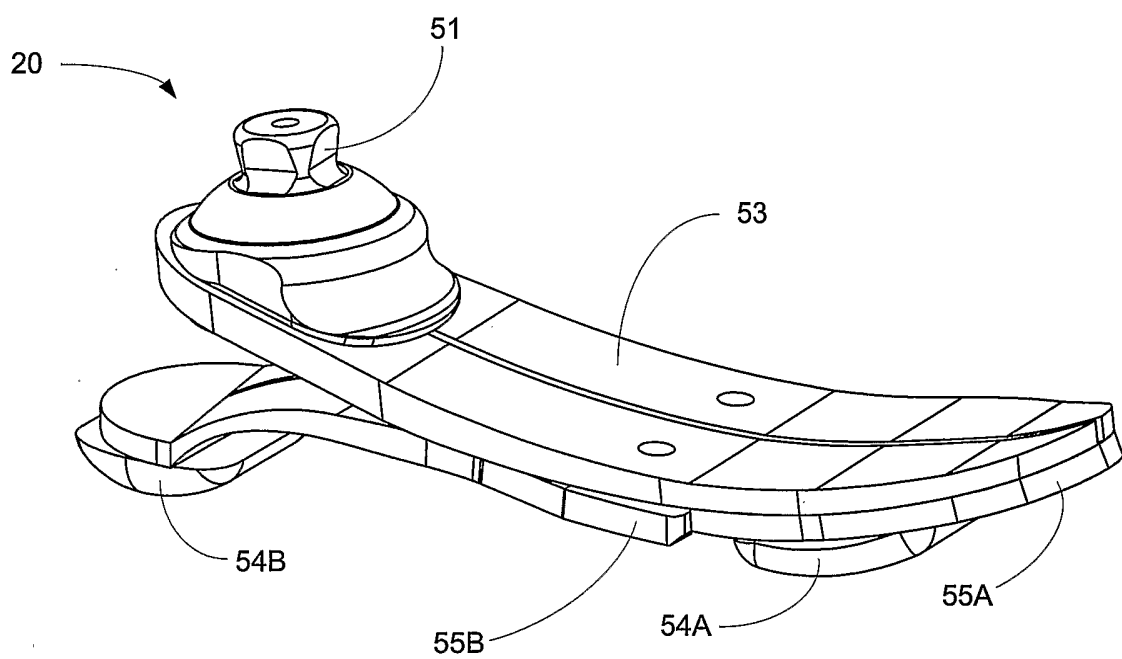


FIG. 3

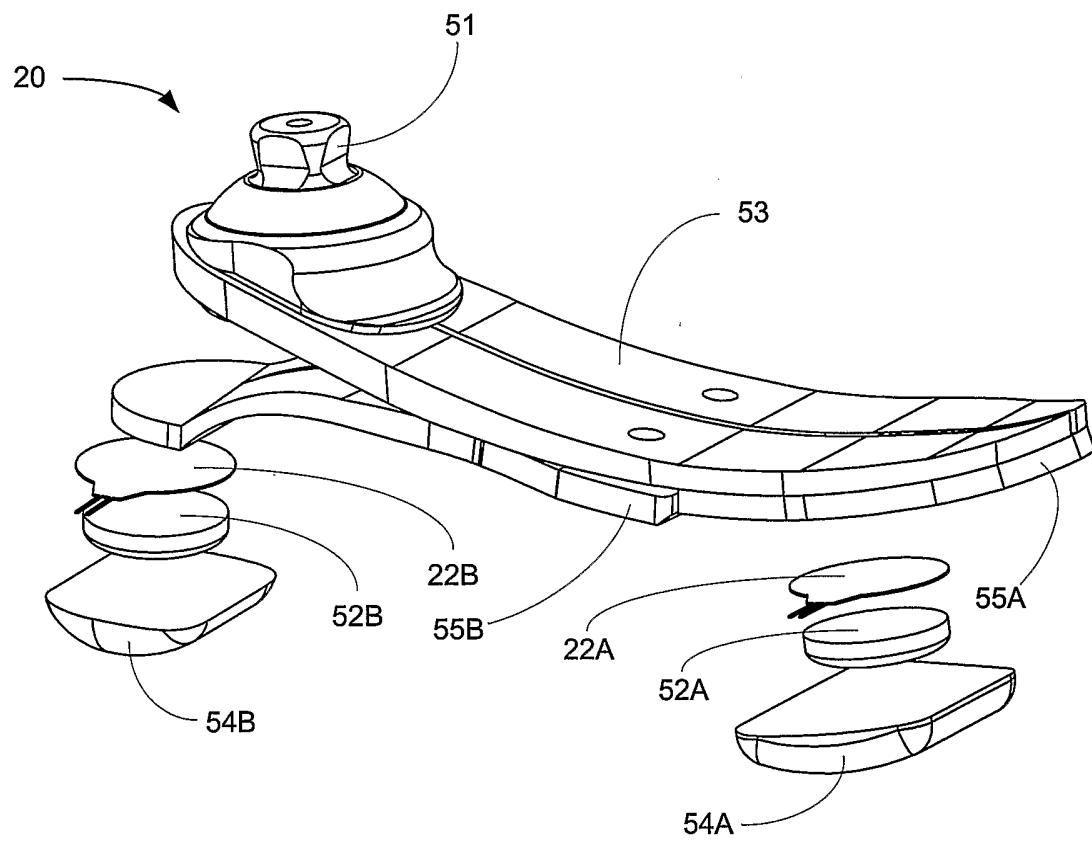


FIG. 4

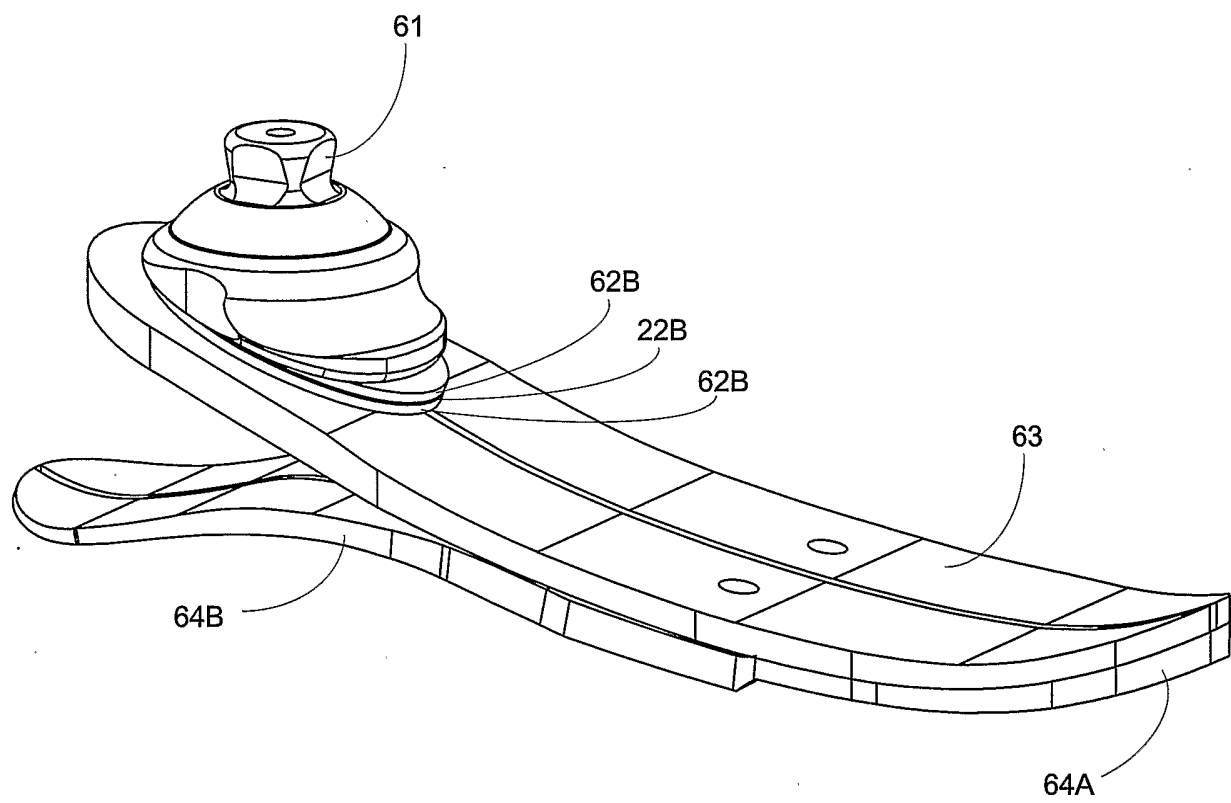


FIG. 5

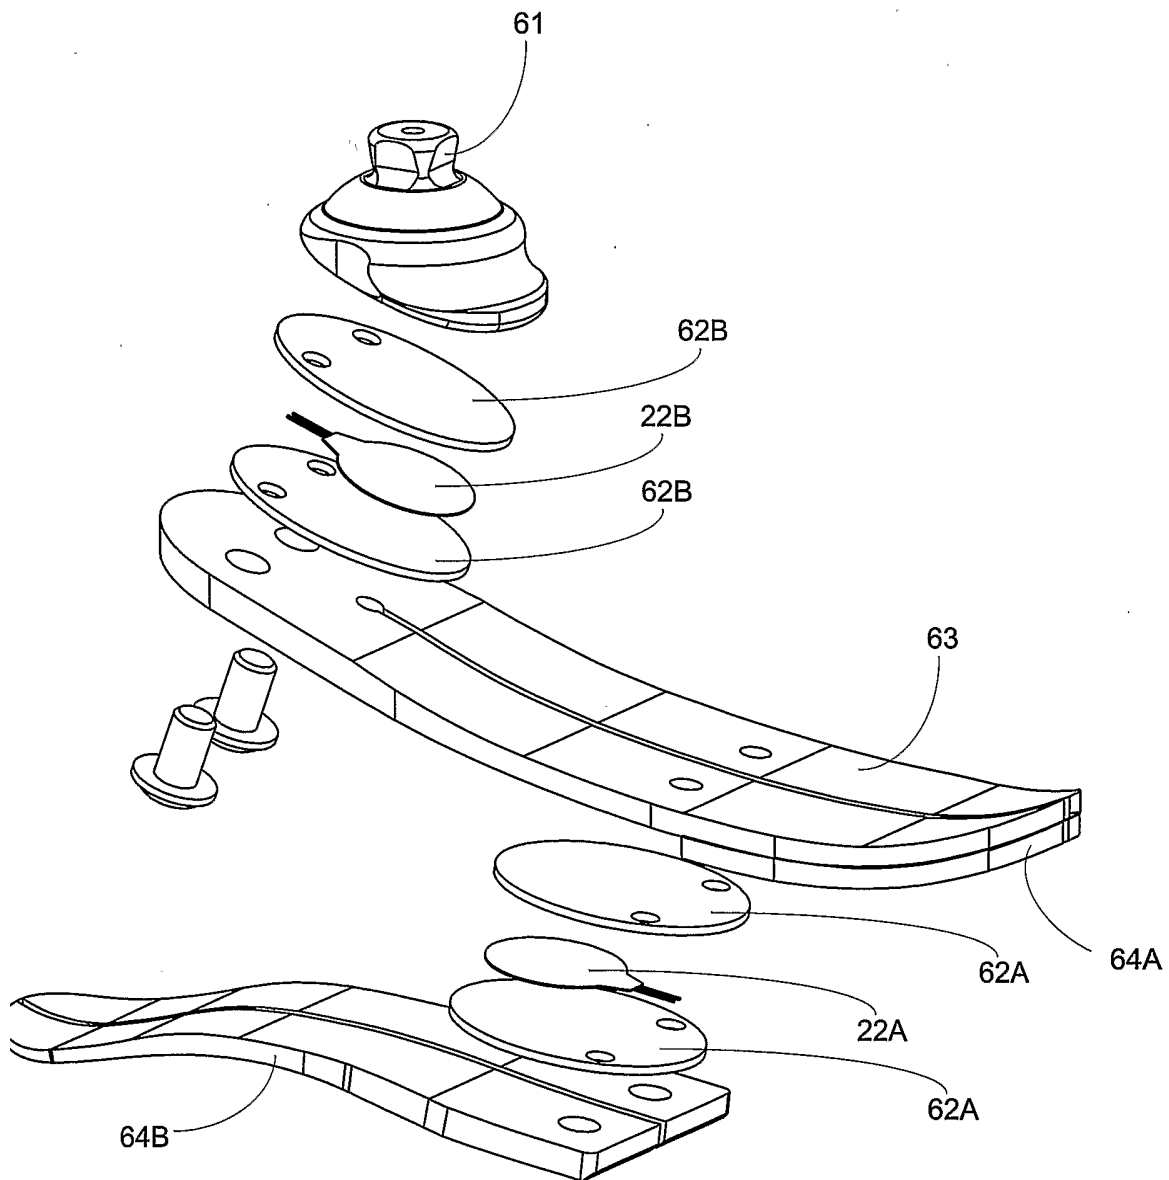


FIG. 6

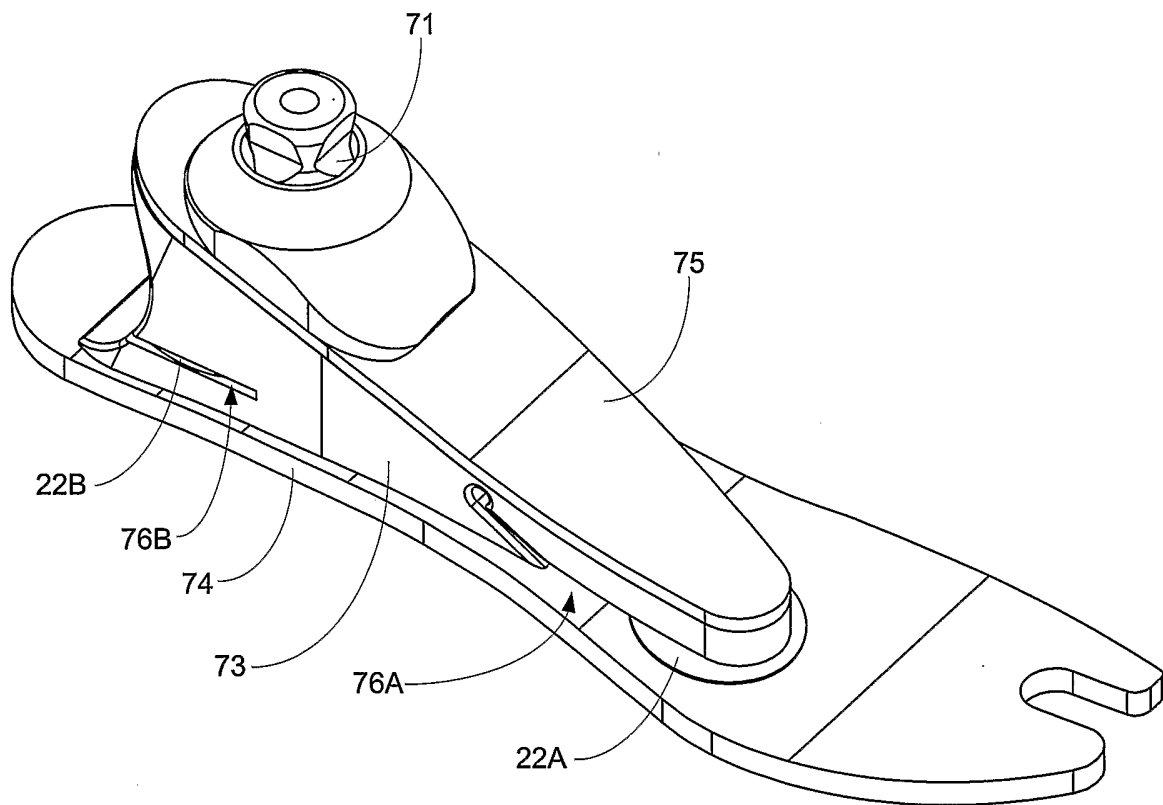


FIG. 7

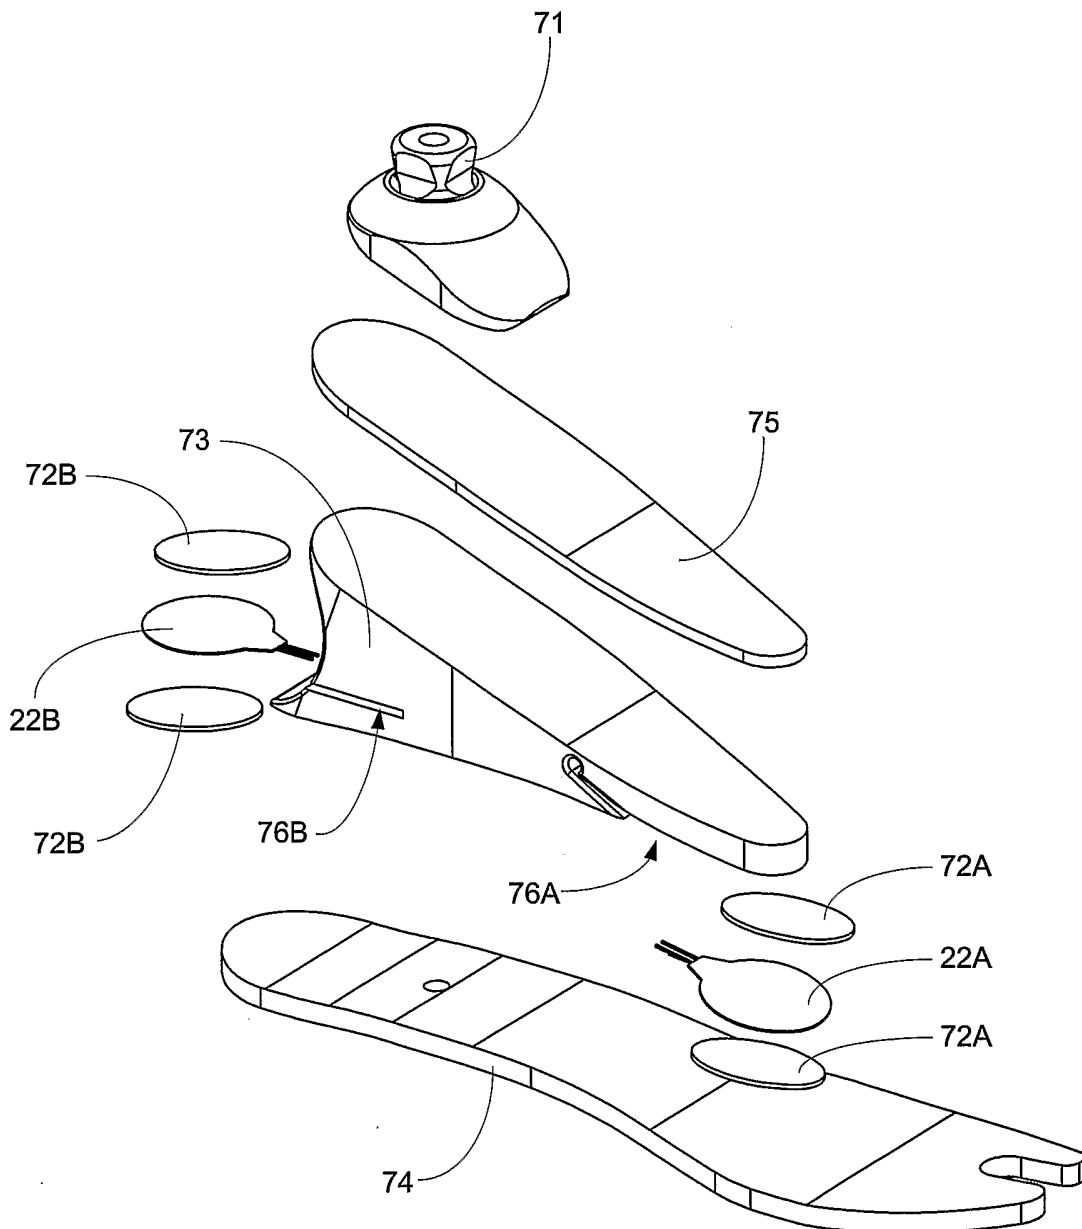


FIG. 8

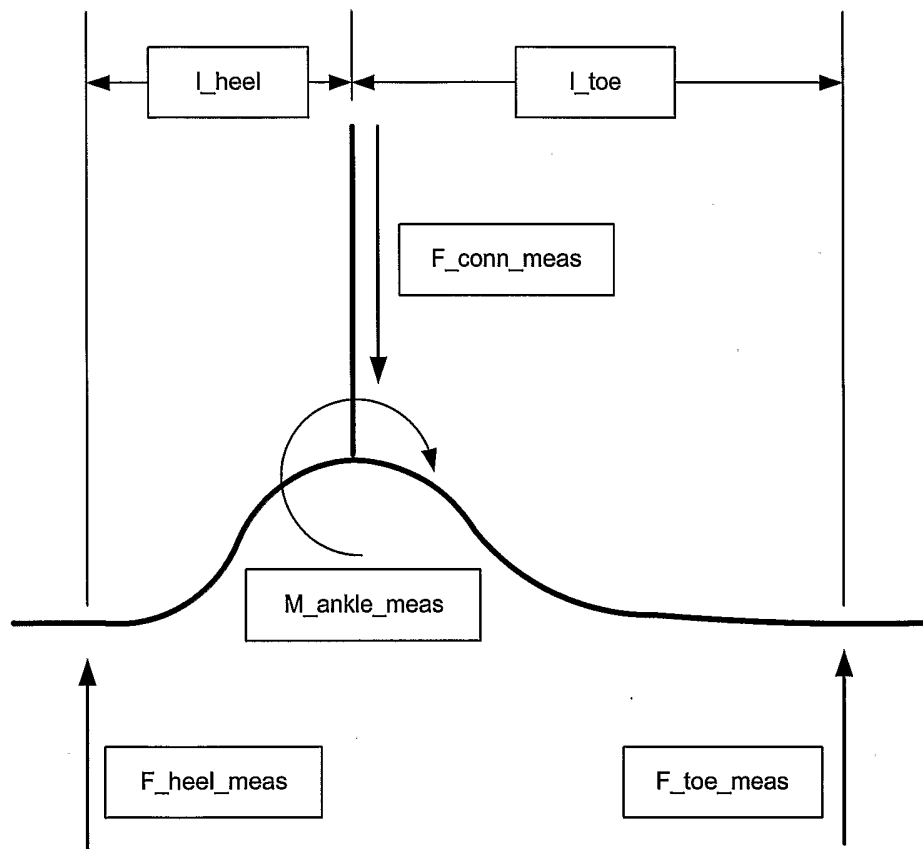


FIG. 9

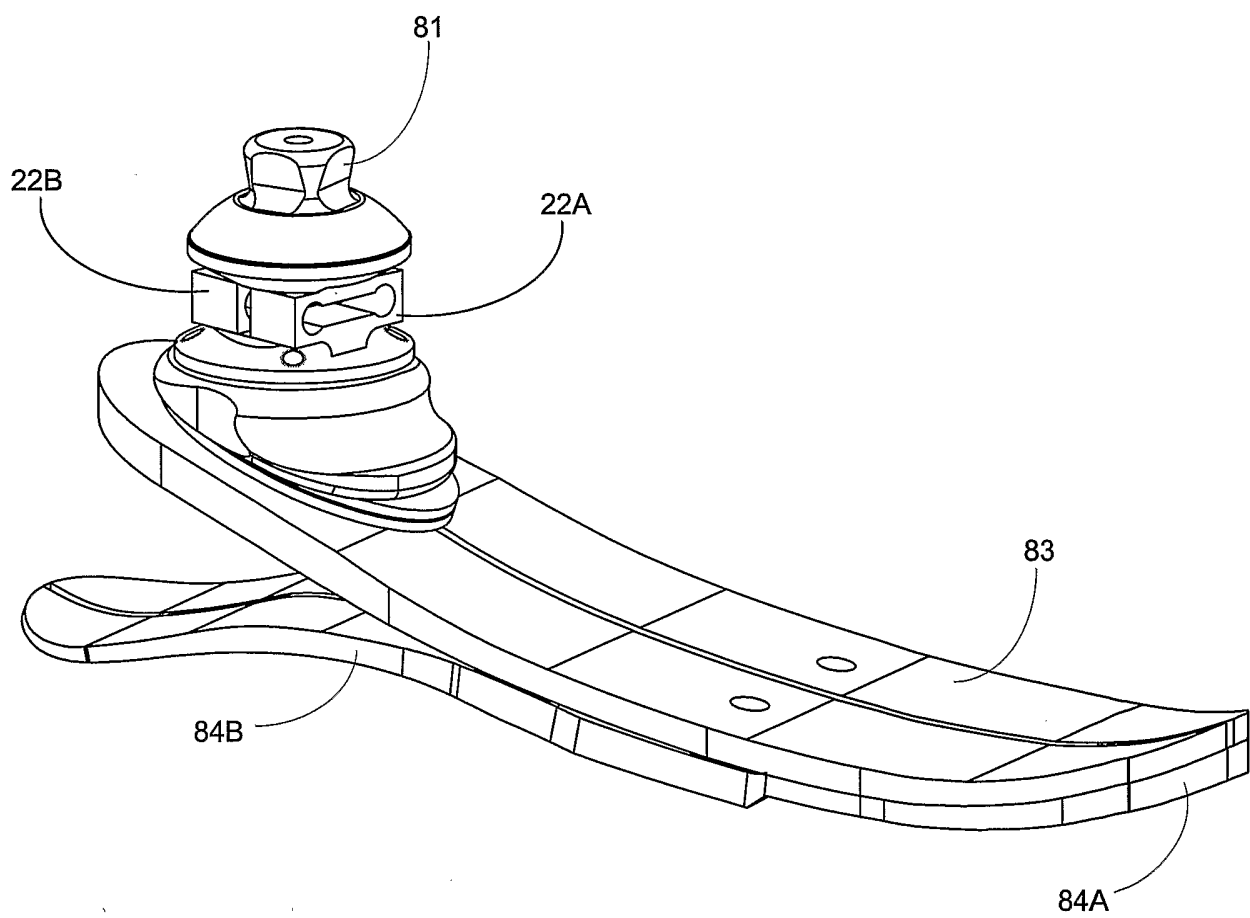


FIG. 10

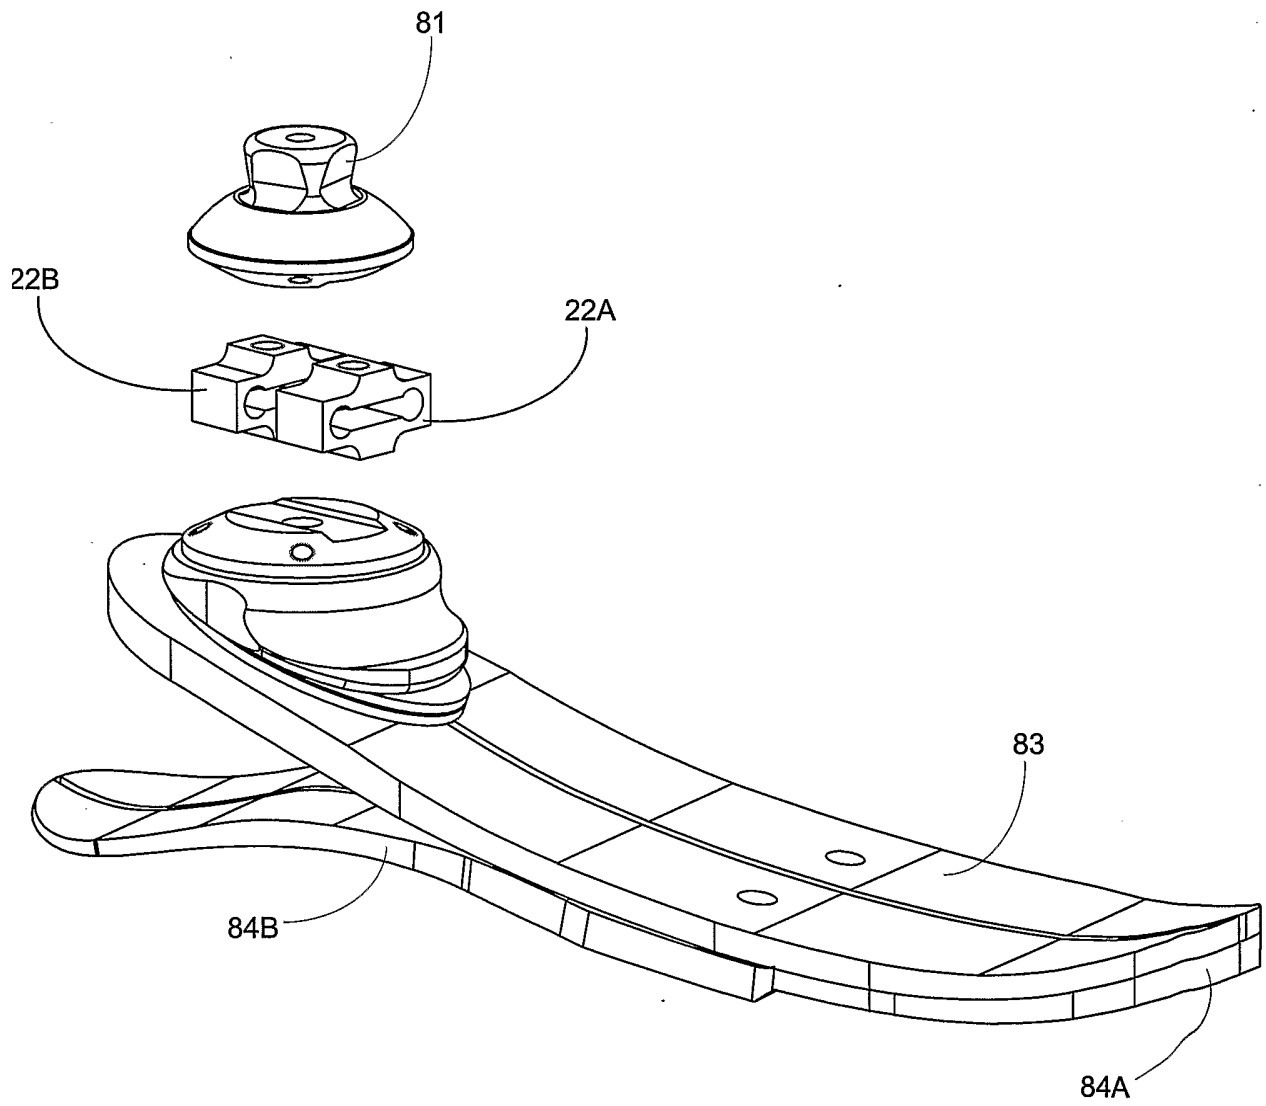


FIG. 11

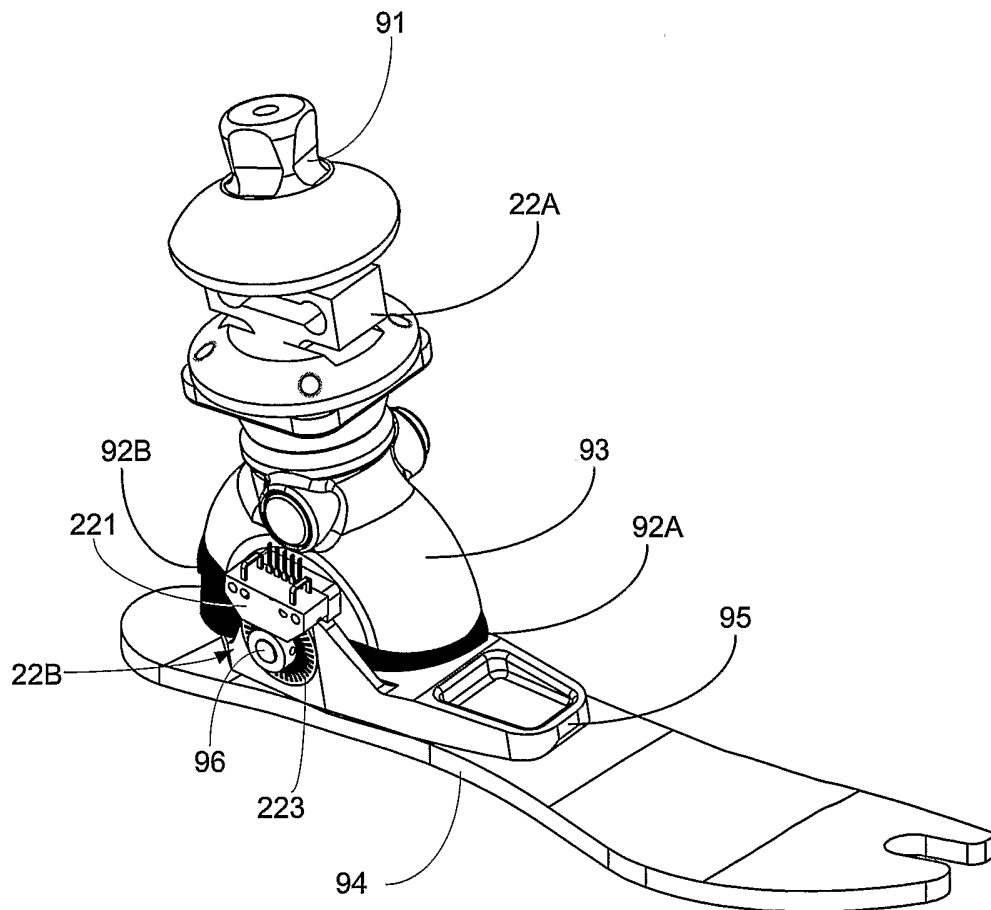


FIG. 12

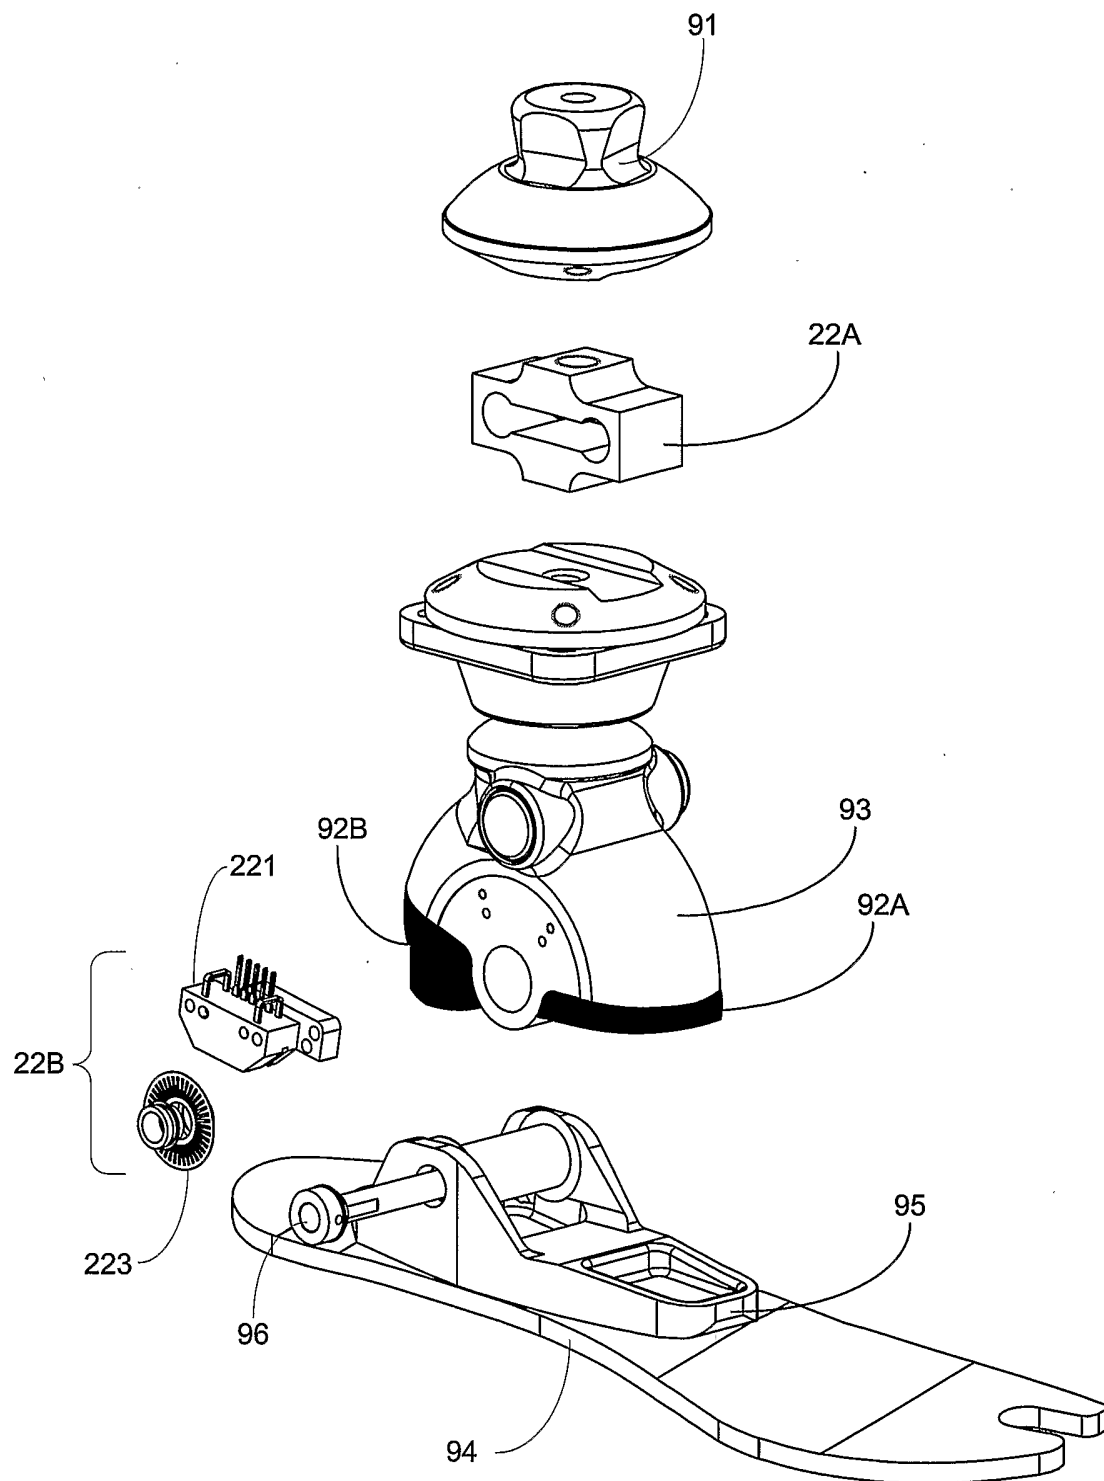


FIG. 13

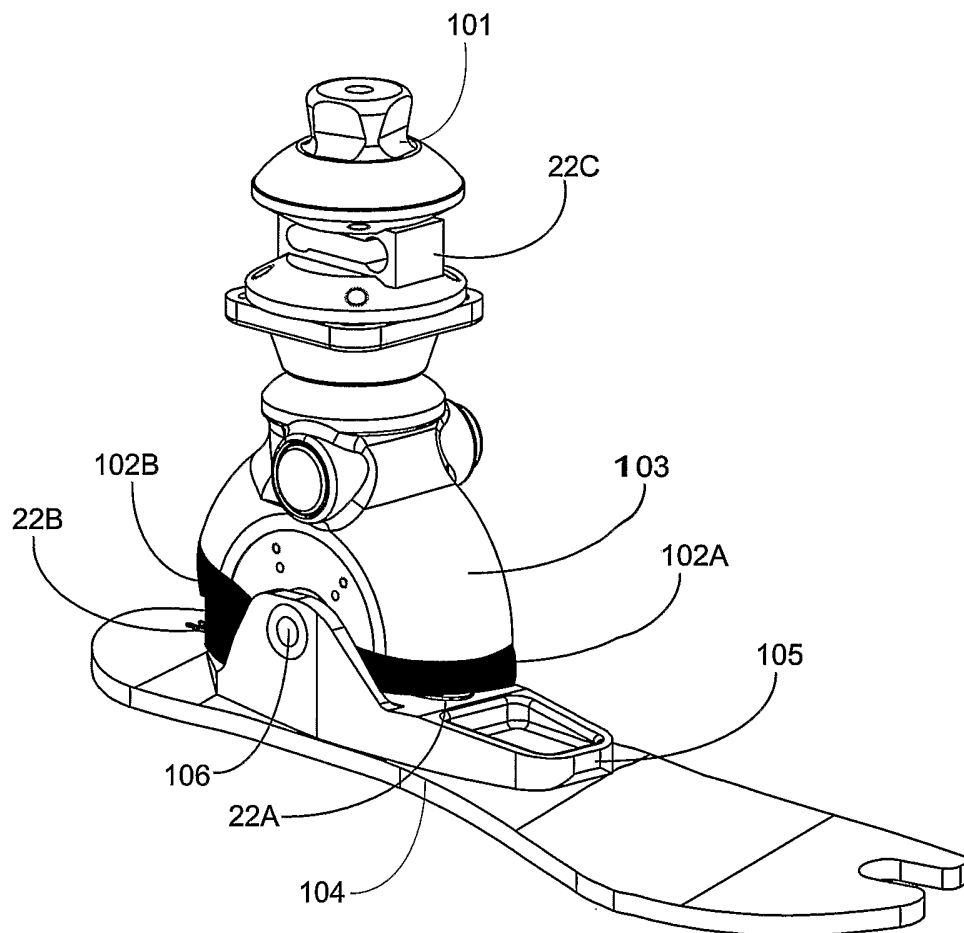


FIG. 14

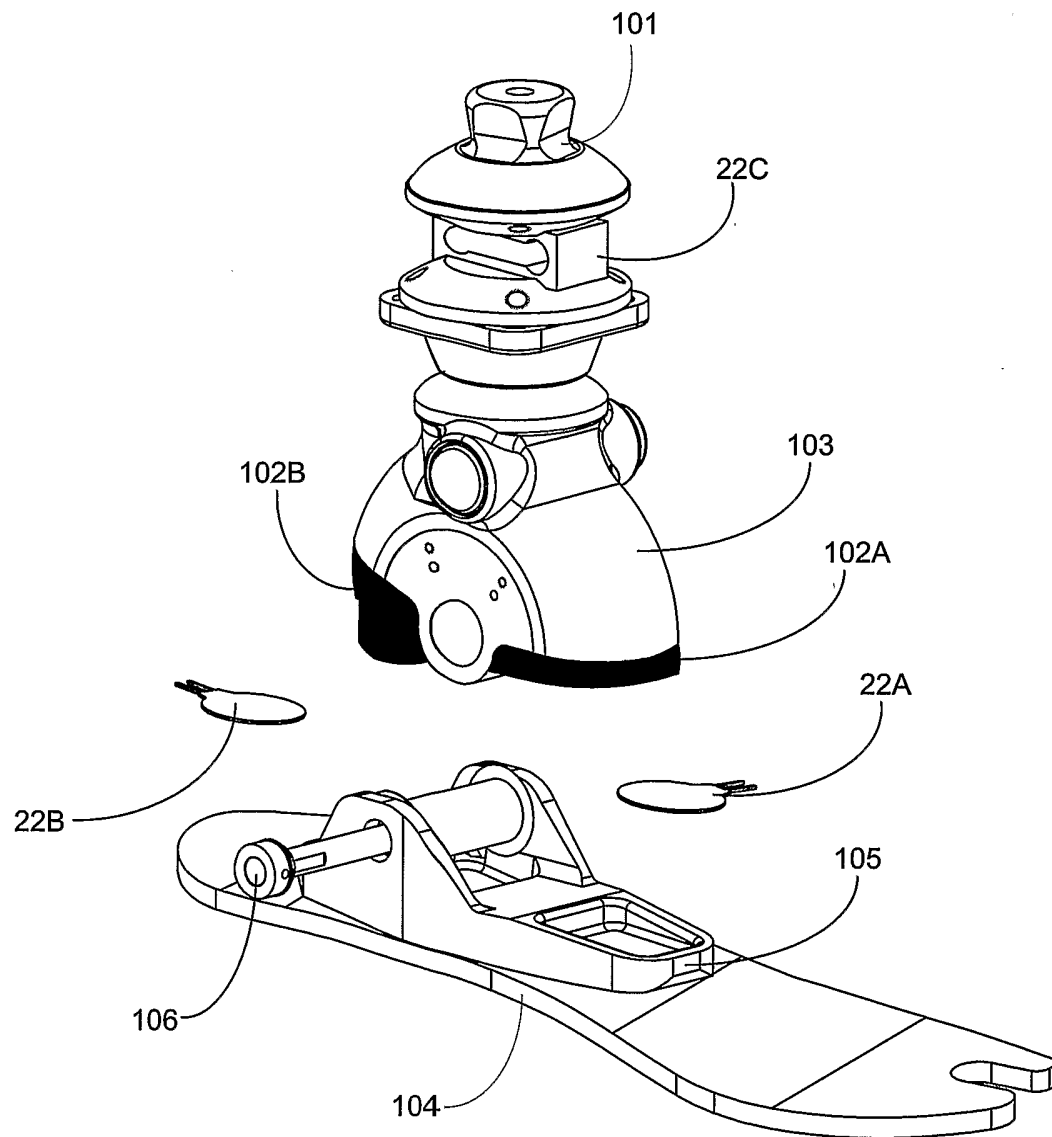


FIG. 15

## INTERNATIONAL SEARCH REPORT

International Application No

PCT/CA 03/01802

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61F2/66 A61F2/68 A61F2/76

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
E	WO 2004/017871 A (VICTHOM HUMAN BIONICS INC) 4 March 2004 (2004-03-04) page 4 - page 6, line 20; claims 25-72; figures 1-4; example 1 -----	1-10,13, 16,17
X	DE 195 21 464 A (BOCK ORTHOPAED IND) 20 March 1997 (1997-03-20) column 6, line 30; figures 1,4 column 8, line 56 - line 65; claims 1,10,11,17,18,28 -----	1-7, 10-12,16
X	WO 99/29272 A (BIEDERMANN MOTECH GMBH) 17 June 1999 (1999-06-17) page 3, paragraph 3 - page 4, paragraph 2; claims; figure 1 ----- -/--	1-5,7, 10,16

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

## \* Special categories of cited documents:

\*A\* document defining the general state of the art which is not considered to be of particular relevance

\*E\* earlier document but published on or after the international filing date

\*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

\*O\* document referring to an oral disclosure, use, exhibition or other means

\*P\* document published prior to the international filing date but later than the priority date claimed

\*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

\*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

\*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

\*&amp;\* document member of the same patent family

Date of the actual completion of the international search

26 July 2004

Date of mailing of the international search report

02/08/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Kuehne, H-C

## INTERNATIONAL SEARCH REPORT

International Application No

PCT/CA 03/01802

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 387 472 A (WILSON MICHAEL T) 14 June 1983 (1983-06-14) column 2, line 37 - column 4, line 24; claims; figures -----	1,16
X	WO 98/25552 A (NOVACARE ORTHOTICS AND PROSTHETICS EAST INC) 18 June 1998 (1998-06-18) page 6, line 5 - line 12; claims 8-28; figures -----	1-5
A	US 2003/029247 A1 (BIEDERMANN LUTZ ET AL) 13 February 2003 (2003-02-13) claims; figures -----	1-18
A	WO 00/38599 A (BIEDERMANN MOTECH GMBH) 6 July 2000 (2000-07-06) claims; figures -----	1-18

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/CA 03/01802

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 2004017871	A	04-03-2004	WO 2004017872 A1	04-03-2004
			WO 2004017873 A1	04-03-2004
			WO 2004017871 A2	04-03-2004
			US 2004111163 A1	10-06-2004
			US 2004049290 A1	11-03-2004
			US 2004088057 A1	06-05-2004
DE 19521464	A	20-03-1997	DE 19521464 A1	20-03-1997
			WO 9641599 A1	27-12-1996
WO 9929272	A	17-06-1999	DE 19754690 A1	01-07-1999
			AT 195240 T	15-08-2000
			DE 59800232 D1	14-09-2000
			WO 9929272 A1	17-06-1999
			EP 0957838 A1	24-11-1999
			ES 2151320 T3	16-12-2000
			JP 2001511052 T	07-08-2001
			US 6423098 B1	23-07-2002
US 4387472	A	14-06-1983	NONE	
WO 9825552	A	18-06-1998	US 6500210 B1	31-12-2002
			AU 5372398 A	03-07-1998
			EP 0964661 A1	22-12-1999
			WO 9825552 A1	18-06-1998
US 2003029247	A1	13-02-2003	DE 10139333 A1	06-03-2003
			EP 1285640 A2	26-02-2003
			JP 2003070817 A	11-03-2003
WO 0038599	A	06-07-2000	DE 19859931 A1	06-07-2000
			WO 0038599 A1	06-07-2000
			EP 1058524 A1	13-12-2000
			JP 2002533161 T	08-10-2002
			US 6755870 B1	29-06-2004