



US00D937409S

(12) **United States Design Patent** (10) **Patent No.:** **US D937,409 S**
Ooshima et al. (45) **Date of Patent:** **** Nov. 30, 2021**

(54) **HOLDER FOR AN X-RAY TOMOGRAPHY DIAGNOSIS APPARATUS**
(71) Applicant: **Canon Medical Systems Corporation**, Otawara (JP)
(72) Inventors: **Jun Ooshima**, Nasushiobara (JP); **Kana Nishimura**, Tokyo (JP); **Rika Harada**, Tokyo (JP)
(73) Assignee: **Canon Medical Systems Corporation**, Otawara (JP)
(**) Term: **15 Years**

D669,990 S * 10/2012 Degruytere D24/158
D683,024 S * 5/2013 Baba D24/158
D695,405 S * 12/2013 Moon D24/158
D715,941 S * 10/2014 Li D24/158
D725,779 S * 3/2015 Braswell, Jr. D24/158
D766,440 S * 9/2016 Kim D24/158
D797,945 S * 9/2017 Kim D24/191
D799,052 S 10/2017 Rossouw
D800,911 S * 10/2017 Diemer D24/192
D828,551 S * 9/2018 Zou D24/130
D829,913 S * 10/2018 Kitayama D24/159
D835,783 S * 12/2018 Smith D24/140
D837,385 S 1/2019 He et al.
D890,344 S * 7/2020 Wells D24/158
D905,234 S * 12/2020 Nock D24/127
D908,229 S * 1/2021 Wagner D24/191

(Continued)

(21) Appl. No.: **29/714,905**

(22) Filed: **Nov. 26, 2019**

(30) **Foreign Application Priority Data**

Jun. 14, 2019 (JP) 2019-013097

(51) **LOC (13) CL.** **24-02**

(52) **U.S. CL.**
USPC **D24/128; D24/158**

(58) **Field of Classification Search**
USPC D24/128, 127, 189-192, 158; 604/179, 604/180; 600/391, 392; 128/DIG. 26
CPC A61M 25/02; A61M 16/0666; A61M 2210/0618; A61M 2025/0253; A61M 2025/0226

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D527,822 S 9/2006 Trevino
D554,257 S * 10/2007 Ogiwara D24/158
D601,261 S 9/2009 Levan
D642,278 S 7/2011 Sharps et al.
D663,798 S * 7/2012 Duncan D21/789

FOREIGN PATENT DOCUMENTS

CN 303128501 3/2015
CN 303980459 12/2016
JP 1091161 11/2000

(Continued)

Primary Examiner — David G Muller

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson, Farabow, Garrett & Dunner, L.L.P.


(57) **CLAIM**

The ornamental design for a holder for an X-ray tomography diagnosis apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a holder for an X-ray tomography diagnosis apparatus showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a top plan view thereof; FIG. 5 is a bottom plan view thereof; and, FIG. 6 is a left side elevational view thereof.

1 Claim, 6 Drawing Sheets

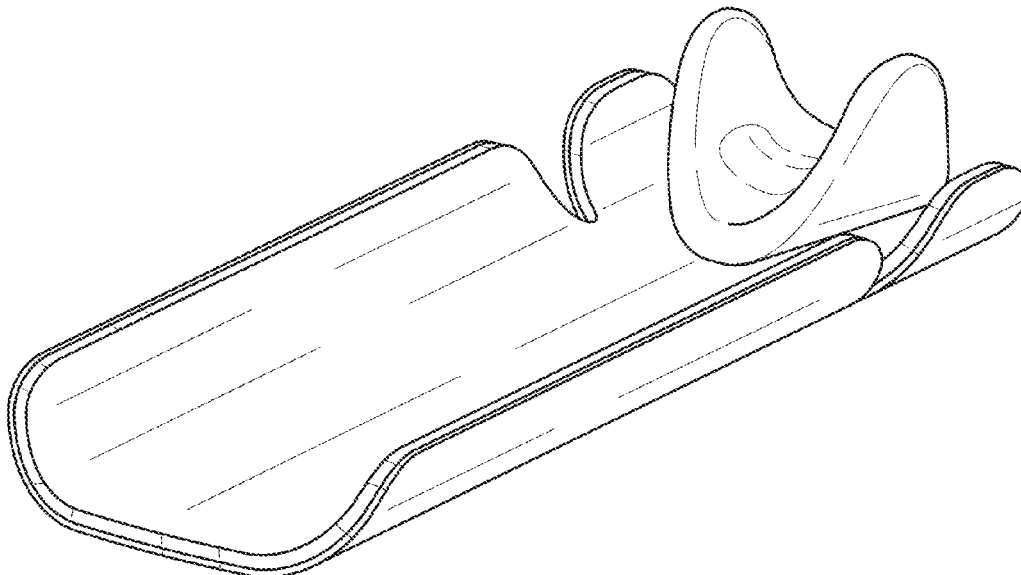

(56)

References Cited

U.S. PATENT DOCUMENTS

D919,100 S * 5/2021 Al-Ali D24/186

FOREIGN PATENT DOCUMENTS

JP	1161361	12/2002
JP	1161362	12/2002
JP	1187079	10/2003
JP	1390819	6/2010
JP	1617186	11/2018

* cited by examiner

Fig. 1

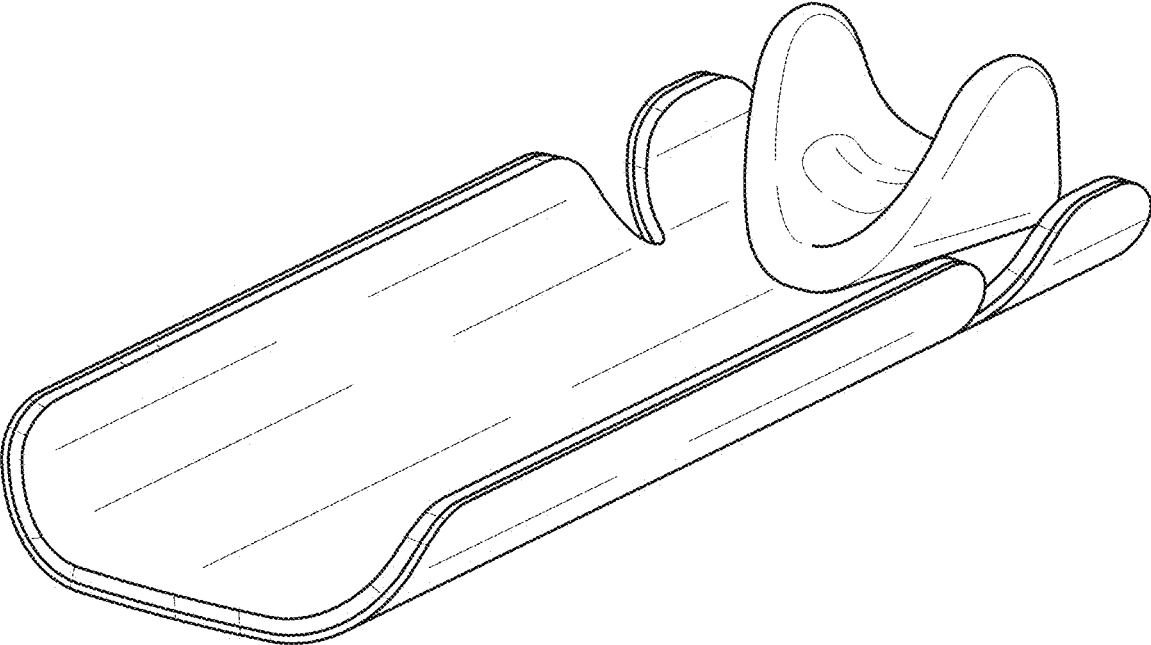


Fig. 2

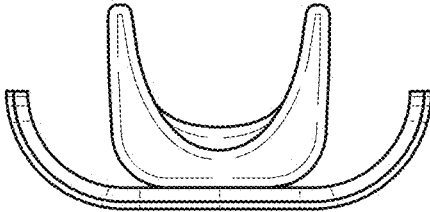


Fig. 3

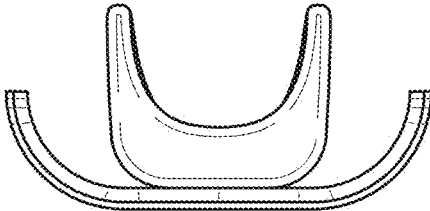


Fig. 4

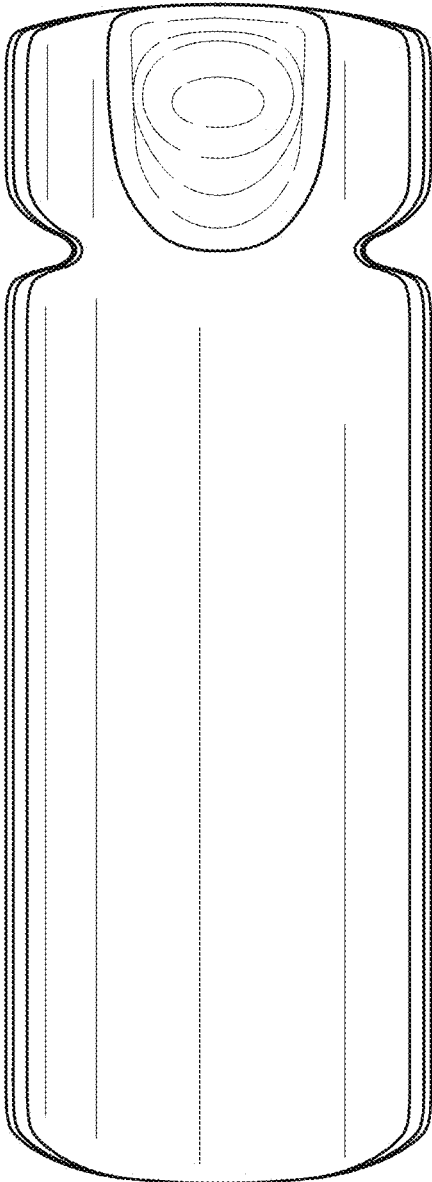


Fig. 5

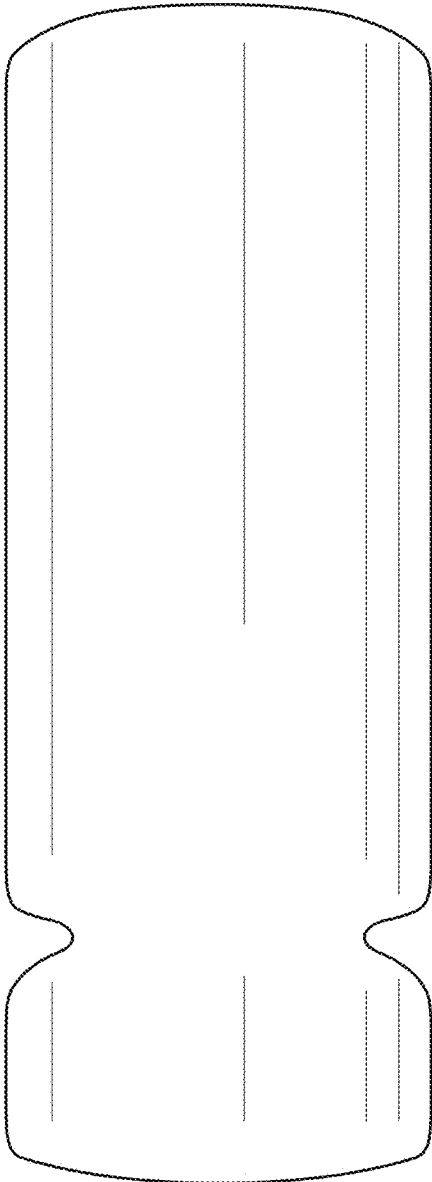


Fig. 6

