



(43) International Publication Date
24 October 2013 (24.10.2013)

- (51) International Patent Classification:
A61B 5/1455 (2006.01) *A61B 5/1459* (2006.01)
- (21) International Application Number:
PCT/US2013/031236
- (22) International Filing Date:
14 March 2013 (14.03.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/636,299 20 April 2012 (20.04.2012) US
- (71) Applicant: UNIVERSITY OF ROCHESTER [US/US];
601 Elmwood Avenue, Box OTT, Rochester, NY 14642 (US).
- (72) Inventors: HUANG, Jason; 7857 Royal Woods, Pittsford, New York 14534 (US). DAYAWANSA, Samantha; 517 Richardson Road, Rochester, NY 14623 (US).
- (74) Agent: GREENBAUM, Michael, C.; Blank Rome LLP, 600 New Hampshire Ave., NW, Washington, DC 20037 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.


(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: IMPLANTABLE REAL-TIME OXIMETER TO DETERMINE POTENTIAL STROKES AND POST-TRAUMATIC BRAIN-INJURY COMPLICATION

Figure 2A

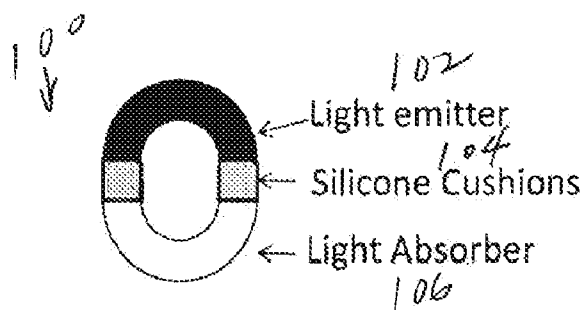

Coronal section of the sensor

(57) Abstract: A first embodiment of an oximetry probe is attached around a blood vessel near the site of a likely stroke. That will be useful to monitor large and medium size cerebral arteries. Another type of pulse oximeter can be passed within cerebral blood vessels to monitor the oxygenation status of the surrounding cerebral tissues. In that version, the emitter and detector are coplanar and contained in a small area, e.g., 50-12 μm .

IMPLANTABLE REAL-TIME OXIMETER TO DETERMINE POTENTIAL STROKES AND POST-TRAUMATIC BRAIN-INJURY COMPLICATIONS

Reference to Related Application

[0001] The present application claims the benefit of U.S. Provisional Patent Application No. 61/636,299, filed April 20, 2012, whose disclosure is hereby incorporated by reference in its entirety into the present disclosure.

Field of the Invention

[0002] The present invention is directed to a pulse oximeter and more particularly to a pulse oximeter that can be implanted onto a large or medium sized blood vessel in which its occlusion would give rise to a stroke or that can be inserted into a medium or a small cerebral blood vessel non-invasively to measure cerebral tissue oxygenation.

Description of Related Art

[0003] Pulse oximetry is a technique for monitoring the oxygenation of a patient's hemoglobin. A sensor is placed on a thin part of the patient's body, usually a fingertip or earlobe, or in the case of an infant, across a foot. Light of two different wavelengths, typically red and infrared, is passed through or reflected by the patient's blood to a photo detector. The changing absorbance at each of the wavelengths is measured, allowing determination of the absorbances due to the pulsing arterial blood alone, excluding venous blood, skin, bone, muscle, and fat. From the absorbances, the ratio of oxygenated to deoxygenated hemoglobin can be determined.

[0004] Above skin, pulse oximetry has long been used to detect hypoxic situations. Such above skin versions cannot be used on moving patients.

[0005] Available versions cannot be used to measure the oxygenation status of cerebral tissues.

[0006] An implantable pulse oximeter is taught in Reichelt et al, "Development of an Implantable Pulse Oximeter," *Transactions in Biomedical Engineering*, Vol. 55, No. 2, February 2008, pp. 581-588. That article also suggests the use of telemetry to transmit the signal from the detector to an external unit. However, there is no teaching to use the oximeter for stroke or other brain conditions and the oximeter taught therein cannot be miniaturized enough for use on blood vessels near the likely location of a potential stroke. They have not tested the device *in vivo*.

[0007] Hickey et al., 2011, *Journal of Clinical Monitoring and Computing* (2011) 25:245–255 describes a single plane oximeter.

[0008] In cardiology, there are devices as Holter monitoring to detect rhythm differences. There is no device to monitor cerebral perfusion.

Summary of the Invention

[0009] It is thus an object of the invention to provide an implantable pulse oximeter for implantation in the blood vessels which can give rise to a stroke (as exemplified by the first preferred embodiment, or Oximeter A) and another (as exemplified by the second preferred embodiment, or Oximeter B) which will have the ability to be passed within a cerebral blood vessel to measure oxygenation of deep brain areas.

[0010] Oximeter A, which will embrace a large rodent vessel, will be developed. That will have a diameter of 1-3mm. That design will be miniaturized in stages to embrace human carotid or major cerebral arteries or major cerebral artery branches.

[0011] At the same time, oximeter B, a single plane oximeter, in which the light emitter and the acceptor are in the same plane, will also be developed.

[0012] That second device will be used to measure tissue oxygenation levels by measuring capillary oxy/deoxy Hemoglobin levels.

[0013] Oximeter B will be attempted to be miniaturized to a size 125-50 μm . Since oxygen measuring probes as small as 125 μm are known, the target size is deemed to be feasible. The light source and the detector are coplanar, so that the oximeter works by reflection. The oximeter is made of biocompatible materials to avoid immunorejection and will have a design that will allow direct attachment to an inner wall of a blood vessel. The output signal of that will note the oxygenation status of the surrounding brain tissues.

[0014] Signals from both of the above devices can be output to a telemetry unit. That will allow remote detection of the condition of a moving patient.

[0015] The oximeter device A can be implanted to monitor a potential stroke. It can be used for high-risk populations and can be used to determine the need for preemptive treatment.

[0016] The principle involved is the same as that of the present pulse oximeter which is in research/clinical use now. The proposed device will also use the ratio of red and infrared absorption of oxy and deoxy hemoglobin to measure the hemoglobin saturation of oxygen. The present method is non-invasive, and there are no known side effects of that mechanism for the past decades.

[0017] During phase 1 of the project, a semicircular red and infrared light emitter and a semicircular light receptor will be used to make the oximeter A. They will face each other embracing the blood vessel. Considering the biconcave shape of the red blood cell, such an assembly will be able get a better reading.

[0018] The design of Oximeter B is as follows. Infrared and red light sources will be used along with a single light receptor, in which all three will be in the same plane. That sensor will be designed to be passaged through cerebral vessels with or without CT (computer tomography) guidance. The reason for having such an assembly is to measure the oxygen saturation of the hemoglobin in capillaries of adjoining cerebral tissues, none invasive to the cerebral tissues' parse. Our final aim is to build a 50 μm diameter sensor to reach deep brain areas angiographically. We will be using fiber optic light sources and absorption fibers as material. Such an application is described in the manuscript Hickey et al., 2011.

[0019] During phase 3, both devices following phases 1, 2, will be made wireless using telemetry. That will allow patients as well as the hospital to monitor those patients and intervene as soon as the need arises.

[0020] Applications include:

- [0021] 1) Monitor patients for complications following traumatic brain injury.
- [0022] 2) Post stroke monitoring of the patient to prevent recurrent strokes.
- [0023] 3) Diagnose stroke
- [0024] 4) Monitor patients with vascular insufficiencies (Transient ischemic attack, carotid stenosis, basilar artery insufficiency, peripheral arterial diseases, mesenteric ischemia, etc),
- [0025] 5) Monitor patients with pulmonary insufficiencies (Pulmonary embolism, Asthma, pulmonary edema),
- [0026] 6) Monitor patients with cardiac insufficiencies
- [0027] 7) Monitoring fetuses and mothers with high risk pregnancies.
- [0028] 8) Measurement of intraoperative organ specific blood oxygen saturation
- [0029] 9) Presently there aren't any "implantable" pulse oximeters or blood gas measurement devices. Even the external oximeters are unable to measure from moving subjects. That compromises the ability to get a real time recording from moving patients or chronic monitoring patients.
- [0030] 10) Identification of ischemic areas of brain. Unlike CT angiography, the present method will not need contrast material.
- [0031] 11) Acute, on nidus, monitoring of patients following stroke. That will prevent subsequent strokes.
- [0032] During the first phase of our study, we will be developing an implantable pulse oximeter (oximeter A) that can be used to record hemoglobin saturation of oxygen in moving subjects. Such a device will be able to do all of the immediate applications listed under applications (numbers 1-9) above and will be located outside a major blood vessel, embracing it.

[0033] A single plane fiber-optic sensor will be tested and attempted to be miniaturized (Oximeter B). Such an application will be able to reach inner brain areas through an angiocatheter and identify would be ischemic areas. Presently there aren't any devices to measure potential stroke areas or to do intracerebral post stroke monitoring. That will serve functions 8-11. There is an overlap of functions of oximeter A, B. According to the area of measurement either A or B will be selected by the clinician.

[0034] Although implantable on a blood vessel (Oximeter A) or within a blood vessel (Oximeter B), the device will still be non invasive to the cerebral tissues.

[0035] Oximeter B will be useful to identify ischemic deep brain areas. Presently for that purpose, CT perfusion scans are used. A CT perfusion scan finds out the areas of under perfusion. However, areas of under perfusion are not always ischemic due to collateral blood supply. Also, areas which are perfused may still be ischemic due to edema, collected material, etc. Therefore, a CT perfusion scan reading can be inaccurate. Use of contrast material can be harmful for some patients, another shortcoming of CT perfusion scans. Above all, the CT perfusion scan method cannot be used for continuous post stroke measurements.

[0036] Another available option to measure cerebral oxygenation is the "Licox" probe. Due to its size (2-3mm diameter), that cannot be passed via an interventional radiology route. Also it takes 20min-2hrs for the Licox probe to stabilize to give a reading. Therefore, it may not be the ideal solution for an acute stroke patient who has only 2-4 hrs time window for intervention. A Licox probe should be physically located within the brain area which will cause invasion of healthy tissue and more traumas.

[0037] On the other hand, an intravascular pulse oximeter (B) can be sent through the angiographic route to its desired destination. The sensor we are proposing will be devoid of the shortcomings of CT perfusion scan and the Licox probe method. It will still meet the expectations of present stroke treatment regimens.

[0038] Our oximeter B will also have the light emitter as well as the receiver in the same plane.

[0039] Oximeters A and B will be able to monitor the oxygenation status of any organ of the body either during surgery or chronically. Those will also be helpful as diagnostic devices to identify ischemic areas. Therefore, although they are made to monitor stroke, they will be able to be applied to monitor other organs, too.

[0040] The two proposed devices can be implanted either on a blood vessel (oximeter A) or within a blood vessel (oximeter B), to monitor tissue oxygenation levels.

[0041] The probe according to the present invention is preferably autoclavable. The emitter and sensor can be made overlapping to allow adjustment for the size of the blood vessel.

[0042] Monitoring blood oxygenation in the blood vessel, using the probe on top of a vessel, will allow quick diagnosis of an impending stroke. If the blood oxygen levels of a distal artery are low, that favors a proximal obstruction.

[0043] The present invention can be used to measure simultaneous major cerebral artery and vein oxygenation. The difference will be less if there is cerebral swelling (edema, stroke, bleeding). The present method is an alternative method to diagnose complications following traumatic brain injury. Presently, interventions are made in the presence of signs and symptoms only.

[0044] A pulse oximeter (A) is attached to a blood vessel near the site of a likely stroke. That will be useful to monitor large and medium size cerebral arteries. Aim of that is to monitor

large areas of cerebral tissues supplied by those arteries. Simultaneous application to an artery and a vein will allow quick diagnosis of cerebral swelling, bleeding, stroke, among many common complications following traumatic brain injury.

[0045] Another type (B) pulse oximeter will be developed which will be able to be passed within cerebral blood vessels to monitor the oxygenation status of the surrounding cerebral tissues. In that version, the emitter and detector are coplanar and contained in a small area, e.g., 50-12 μm . Aim of that is to measure small areas of cerebral tissues located deep within the brain.

[0046] Both applications (A, B) can be useful to monitor any organ in the body either during surgery or chronically.

[0047] The output can be analyzed through suitable software.

[0048] Both versions (A, B) will be converted to send wireless signals in order to allow for chronic monitoring. Presently there is no device to measure cerebral oxygenation, chronically.

Brief Description of the Drawings

[0049] Preferred embodiments will be set forth in detail with reference to the drawings, in which:

[0050] Figure 1 is a diagram showing the basic circuitry of the oximeter according to the first preferred embodiment;

[0051] Figures 2A and 2B are diagrams showing cross-sectional views of the oximeter probe according to the first preferred embodiment;

[0052] Figure 3 is a diagram showing the manner in which the oximeter probe according to the first preferred embodiment surrounds the blood vessel;

[0053] Figure 4 is an image showing the emitter and sensor in an un-assembled state;

[0054] Figure 5 is an image showing the emitter and sensor in an assembled state in a variation of the first preferred embodiment;

[0055] Figure 6 is an image showing the probe of Figure 5 attached to a blood vessel;

[0056] Figures 7A and 7B are diagrams showing the probe according to the second preferred embodiment;

[0057] Figure 8 is a diagram showing a fiber optic sensor pathway for use with the probe of Figures 7A and 7B;

[0058] Figure 9 is a diagram showing four probes according to the second preferred embodiment within a lumen of a blood vessel; and

[0059] Figure 10 is a screen shot showing measurement.

Detailed Description of the Preferred Embodiments

[0060] Preferred embodiments of the invention will now be set forth in detail with reference to the drawings, in which like reference numerals refer to like elements throughout.

[0061] Figures 1-6 show the first preferred embodiment, or the oximeter A design.

[0062] Figure 1 shows the basic circuitry of the extravascular oximeter 100. The oximeter 100 includes a light emitter 102, silicone cushions 104, and a photo receiving sensor 106 configured in a cylindrical shape to surround a vessel (not shown in Figure 1). The emitter 102 operates under the control of an emitter driver 108 to emit light at two wavelengths, e.g., in the red and infrared ranges. An output of the photo receiving sensor 106 is made incident via fiber optics onto a photo diode 110, whose output signal goes to amplification and filtering circuitry 112 and recording circuitry 114.

[0063] Figures 2A and 2B show the oximeter A cross section. A waterproof semicircular light emitter 102 and a light sensor 106 will be made. An outer rubber or Teflon covering 116 will embrace both to keep them in place and protect them from moisture. Nylon hooks 118 will receive sutures, which will be used to attach the assembly to the body wall. That sensor will be tested initially while it is embracing the aorta as well as the inferior vena cava of 400-600g Sprague Dawley rats.

[0064] Figure 3 shows the sensor 100 wrapped around an aorta or inferior vena cava A.

[0065] Figure 4 shows the emitter 102 and the sensor 106 in an un-assembled state.

[0066] As shown in Figure 5, the emitter 102 and the sensor 106 can be attached to a plastic tube 120, in which case the silicone cushions 104 are unnecessary. The plastic tube 120 has an opening 122 so that it can be clipped onto a blood vessel A, as shown in Figure 6.

[0067] The emitter 102 has the ability to adjust to the light level automatically. Various intensities of light can be used, depending on the environment light intensity.

[0068] Figures 7A-9 show the design of the oximeter B.

[0069] Figures 7A and 7B show the second preferred embodiment, namely, the intravascular pulse oximeter (B) 200. The diameter of the sensor 200 will be 600 μm at the initial stage. At the final stages, the aim is to miniaturize its size to 50 μm . That will be feasible, as there are 125 μm fiber-optic oxygen sensors commercially available in the \$100-300 range (<http://www.instechlabs.com/Oxygen/fiberoptic/125.php>). In that design, the light emitter 202 and the receptor 206 will be in the same plane. A rubber sleeve 216 will encase them both. A touch sensor 226 in the periphery will note the sensor contact with the vessel wall. Biodegradable fibrin glue will be applied to the rubber sleeve, which will allow the sensor to be chronically placed. A ball and socket joint 228 allows the oximeter 200 to adhere to the vessel contour while providing a connection to a connecting cable 230.

[0070] Figure 8 shows the basic fiber optic sensor pathway that will be used to record during phase 2 of the project. It was excerpted from Hickey, M et al., Journal of Clinical monitoring and computing (2011) 25:245-255; while it was not originally designed for an oximeter according to the present invention, it can easily be adapted for the oximeter B 200. An emitter driver 208 controls a red emitter 232 and an infrared emitter 234 to emit red and infrared light, respectively. Their outputs are combined by a Y piece 236 and input via a single transmitting fiber 238 into the oximeter 200. Light from the sensed area goes through a single receiving fiber 240 into a photodiode 210, whose output goes to a 1V amplifier 242 and a demux 244. The above components communicate via isolation 246 with filtering and

amplifying circuitry 248 and a computing device 250. Of course, similar circuitry can be used for the oximeter A 100 of the first preferred embodiment.

[0071] Figure 9 shows four oximeters (B) 200 in action within a lumen L of a cerebral vessel V . Each sensor 200 will be able to get readings from tissues around the periphery of the blood vessel in an area of measurement M . That will allow isolating the area of ischemia. A few sensors can be arranged to monitor a larger brain area, as shown in the figure.

[0072] The oximeter can be incorporated into a MERCI catheter or a Penumbra catheter to evacuate the thrombus at the same time. A common transmission line 252 can be used. The output of the sensor can be sent to a computing device to analyze the output to achieve any of the above ends. The computing device will be programmed with a suitable algorithm. The device will measure real time oximetry, heart rate, breath rate, breath distension and pulse pressure. Since the sensor and the light emitter is directly attached to a major blood vessel, the measurements will be very accurate and should not have artifacts when getting readings from above skin versions of the oximetry set up presently used in clinical settings.

[0073] The following discussion can apply to either of the preferred embodiments or to any other embodiment.

[0074] Figure 10 shows a screen shot taken while recording.

[0075] The physiological parameters measured and their scientific basis are as follows. The oximeter provides real-time percent oxygen saturation of functional arterial hemoglobin.

[0076] Real-time cardiac pulse rate is given in bpm (beats per minute).

[0077] A real-time breath rate measurement is updated every few seconds. Note that that parameter is actually derived from respiratory effort, not airflow, and will be present even if

the patient is experiencing an obstructive apnea, as long as breathing effort is present. Breath rate is given in breaths per minute or brpm.

[0078] Pulse distention is a measurement of the change in distention of the arterial blood vessels residing between the sensor pads due to a cardiac output pulse. It is a direct measurement of changes in local blood volume that accompany each cardiac pulse. Since the preferred embodiment records from the aorta, the readings are very accurate. For a given vascular compliance, pulse distention can also provide a surrogate for pulse pressure.

[0079] Pulse oximetry measures the oxygen content of arterial blood. The blood is identified as being arterial because of its pulsatile nature. That pulsation is identifiable because it causes a cyclic change in the absorption of light energy from the red and infrared LEDs (Light Emitting Diodes) as it passes through the vessel, due to the presence of changing quantities of blood that occur with every heart beat. Because the blood is arterial, it possesses systemic arterial oxygen content, which is what is measured. Pulse distention is simply a measurement of the change in the effective path length of the light that passes through only the arterial or pulsating blood, and it has true linear distance units of m.

[0080] One could picture that by thinking of placing all of the arterial blood residing in the light path between the sensor pads into a cylinder that has a cross-sectional area equal to the cross-sectional area of the column of the light beam passing from the LEDs to the photodiode. If the cylinder had one inlet and one outlet for the blood to enter and exit, then the level of blood in the cylindrical chamber would rise with each cardiac ejection stroke, and lower during each subsequent cardiac filling phase. The change in height of the blood in that cylinder between ejection and filling, or systole and diastole (Systolic BP-Diastolic BP), would then be measured directly as pulse distention.

[0081] The larger the pulse distention value, the more arterial blood will be available to make oximetry, as well as heart rate and breath rate, measurements.

[0082] Breath distention is a measurement of the change in distention of the arterial blood vessel residing between the sensor pads due to breathing effort. For a given vascular compliance, the breath distention provides a surrogate for intrapleural pressure.

[0083] While two preferred embodiments have been set forth above, those skilled in the art who have reviewed the present disclosure will readily appreciate that other embodiments can be realized within the scope of the invention. For example, recitations of numerical values, specific technologies, and specific materials are illustrative rather than limiting. Therefore, the invention should be construed as limited only by the appended claims.

We claim:

1. An implantable pulse oximetry probe comprising:
an emitter for emitting light;
a detector for detecting the light; and
an attachment for attaching the emitter and the detector around a blood vessel such that the emitter and the detector are on opposite sides of the blood vessel.
2. The probe of claim 1, wherein the emitter emits the light at at least two wavelengths.
3. The probe of claim 2, wherein the at least two wavelengths are in the red and infrared ranges.
4. The probe of claim 1, wherein the probe is configured such that the probe completely surrounds the blood vessel.
5. The probe of claim 4, further comprising cushions for separating the emitter from the detector.
6. The probe of claim 4, further comprising a covering around the emitter and the detector.
7. The probe of claim 6, further comprising a hook attached to the cover for suturing the probe to tissue.
8. The probe of claim 1, wherein the probe is configured such that the probe partially surrounds the blood vessel.
9. The probe of claim 8, further comprising a tube to which the emitter and the detector are attached, the tube having an opening for allowing the tube to be clipped onto the blood vessel.
10. The probe of claim 1, wherein the emitter and the detector are concave.

11. An implantable pulse oximetry probe comprising:
an emitter for emitting light;
a detector for detecting the light; and
an attachment for attaching the emitter and the detector within a lumen of a blood vessel.
12. The probe of claim 11, wherein the emitter emits the light at at least two wavelengths.
13. The probe of claim 12, wherein the at least two wavelengths are in the red and infrared ranges.
14. The probe of claim 11, wherein the attachment is configured to attach the emitter and the detector within the lumen such that the emitter and the detector are coplanar.
15. The probe of claim 11, wherein the attachment is configured to attach the emitter and the detector to a side of the blood vessel.
16. The probe of claim 15, wherein the attachment is configured to attach the emitter and the detector to the side of the blood vessel such that the emitter emits the light out of the blood vessel into surrounding tissue and such that the detector detects the light from the surrounding tissue.
17. The probe of claim 15, wherein the attachment comprises a sleeve for the emitter and the detector.
18. The probe of claim 17, wherein the attachment further comprises a touch sensor for detecting that the probe is attached to the side of the blood vessel.

Figure 1



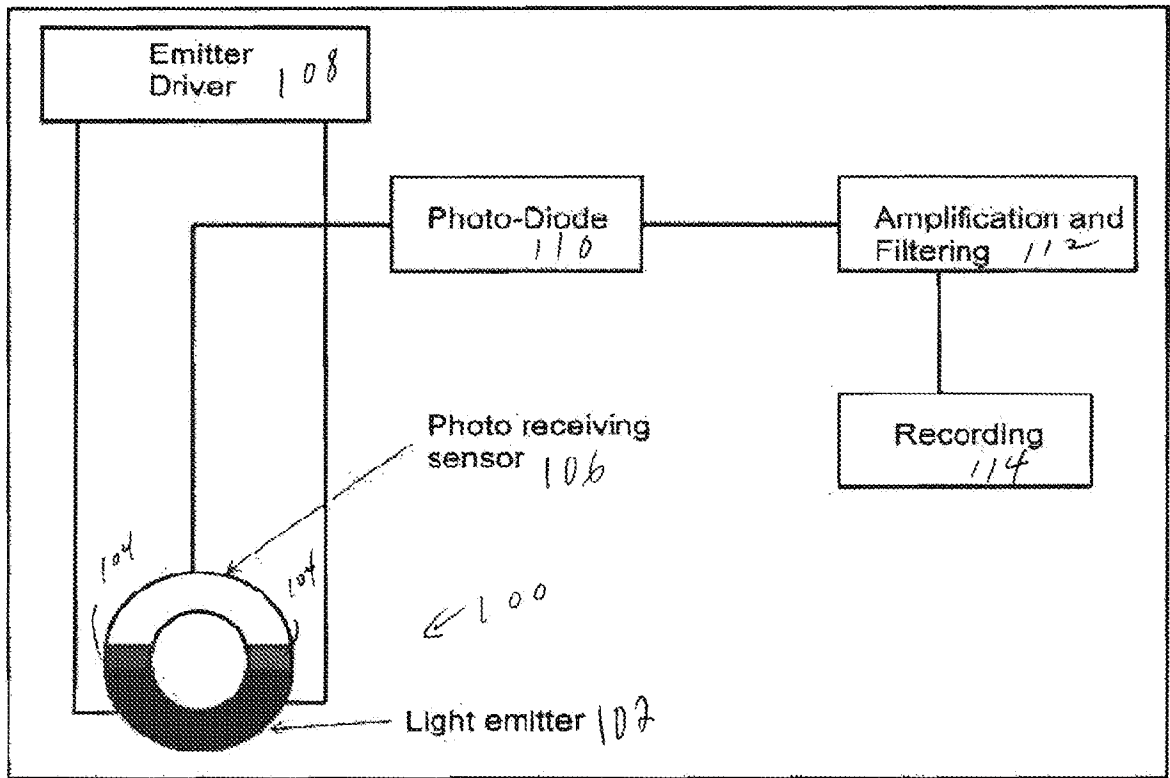


Figure 2A

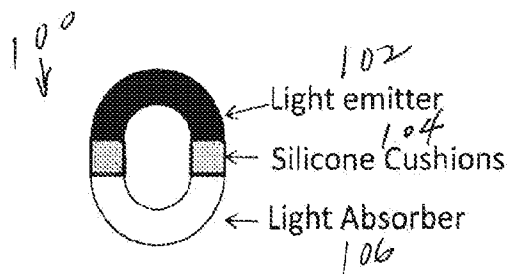

Coronal section of the sensor

Figure 2B

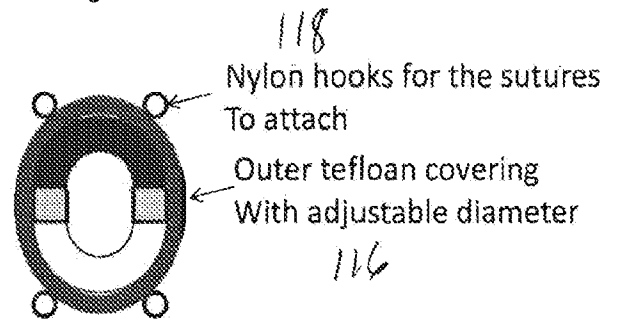

Coronal section of the sensor with outer covering

Figure 3

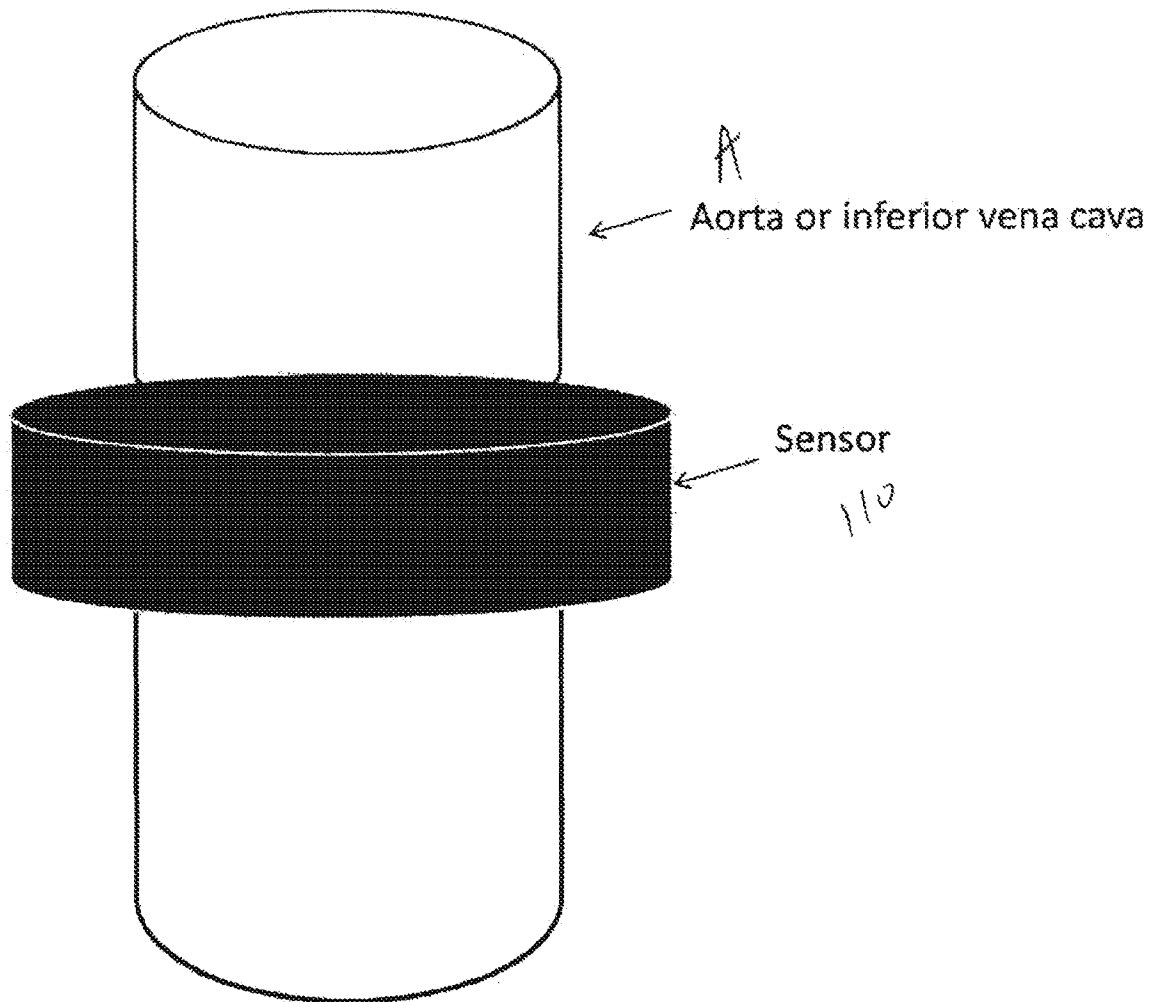


Figure 4

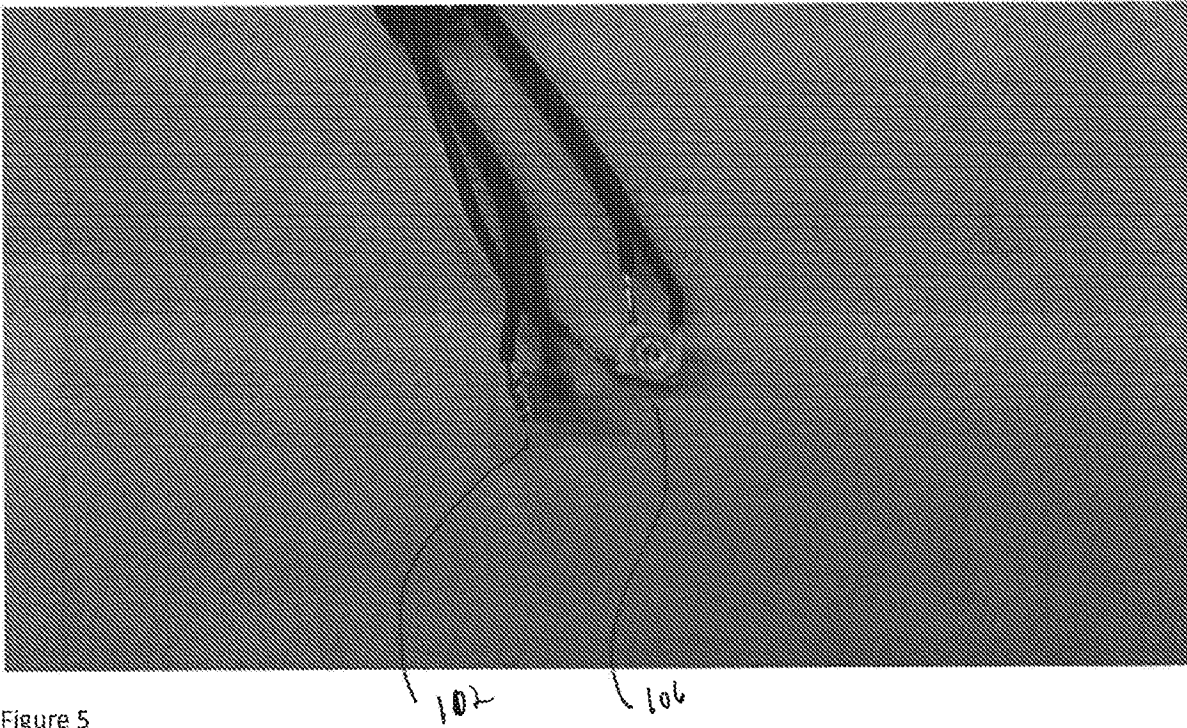


Figure 5

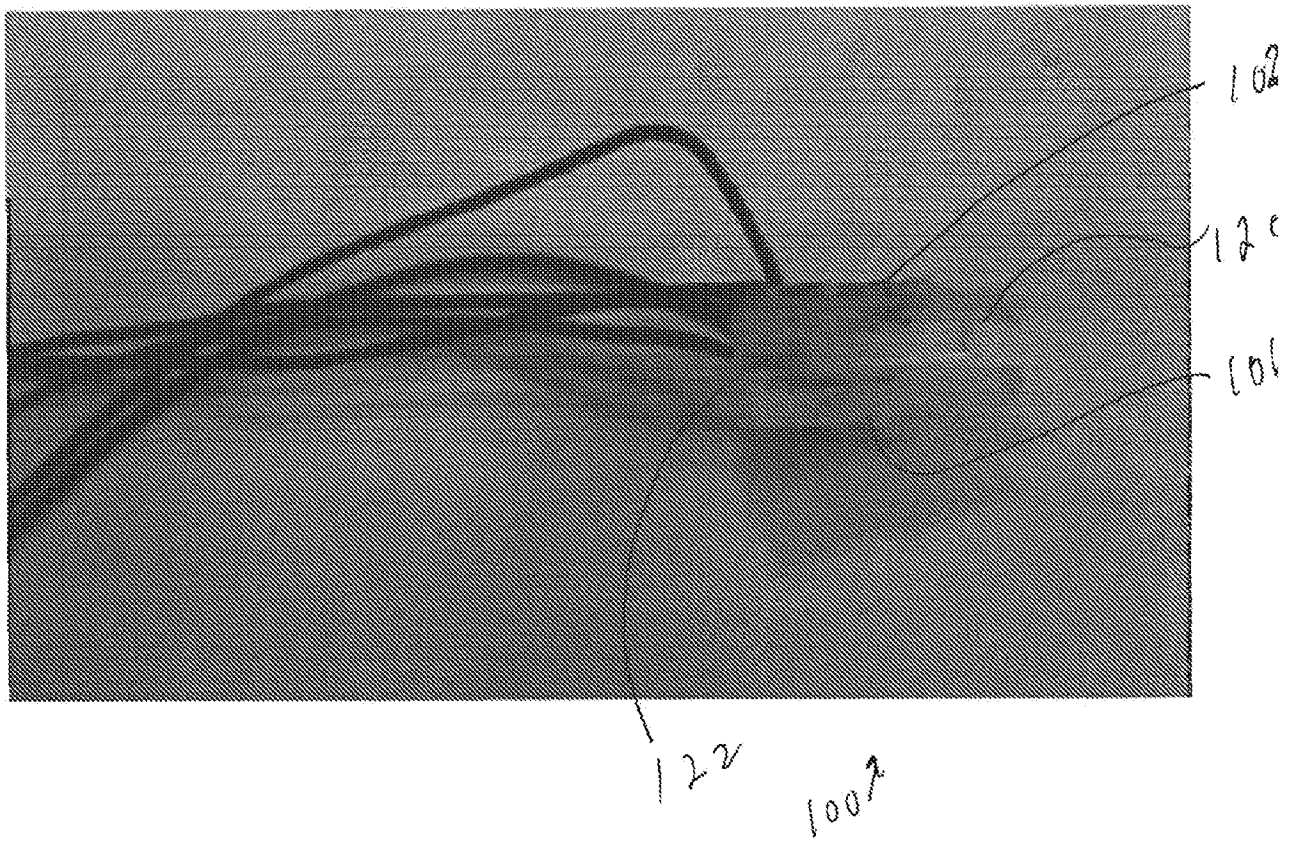


Figure 6

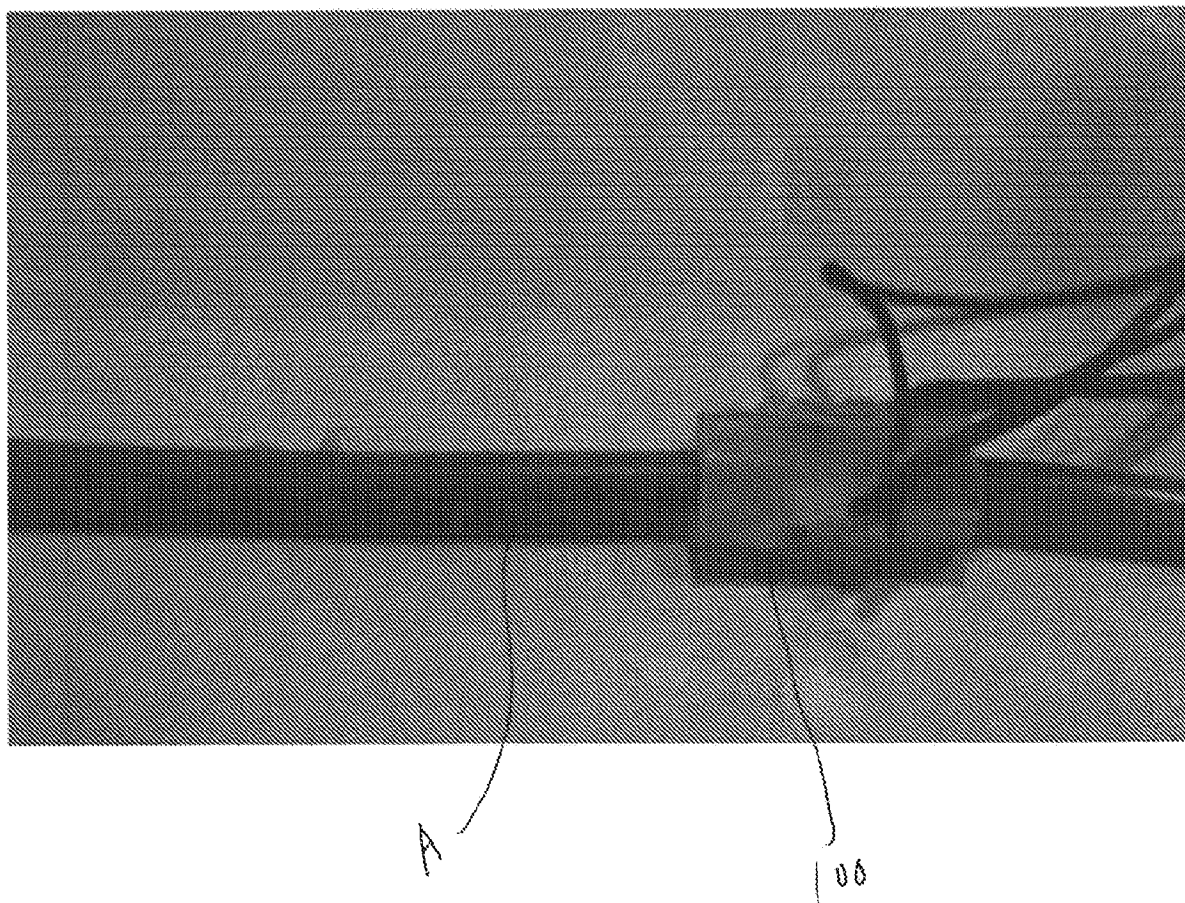


Figure 7A

Figure 7B

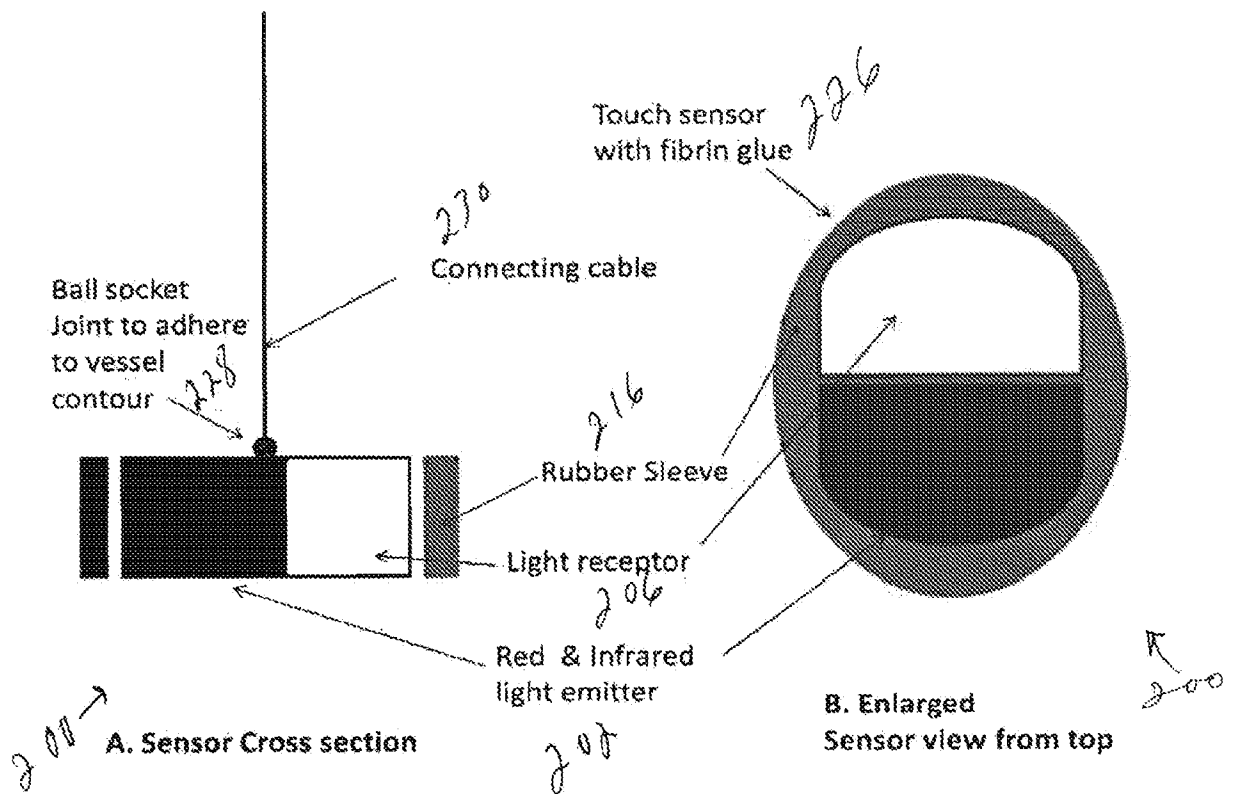


Figure 8

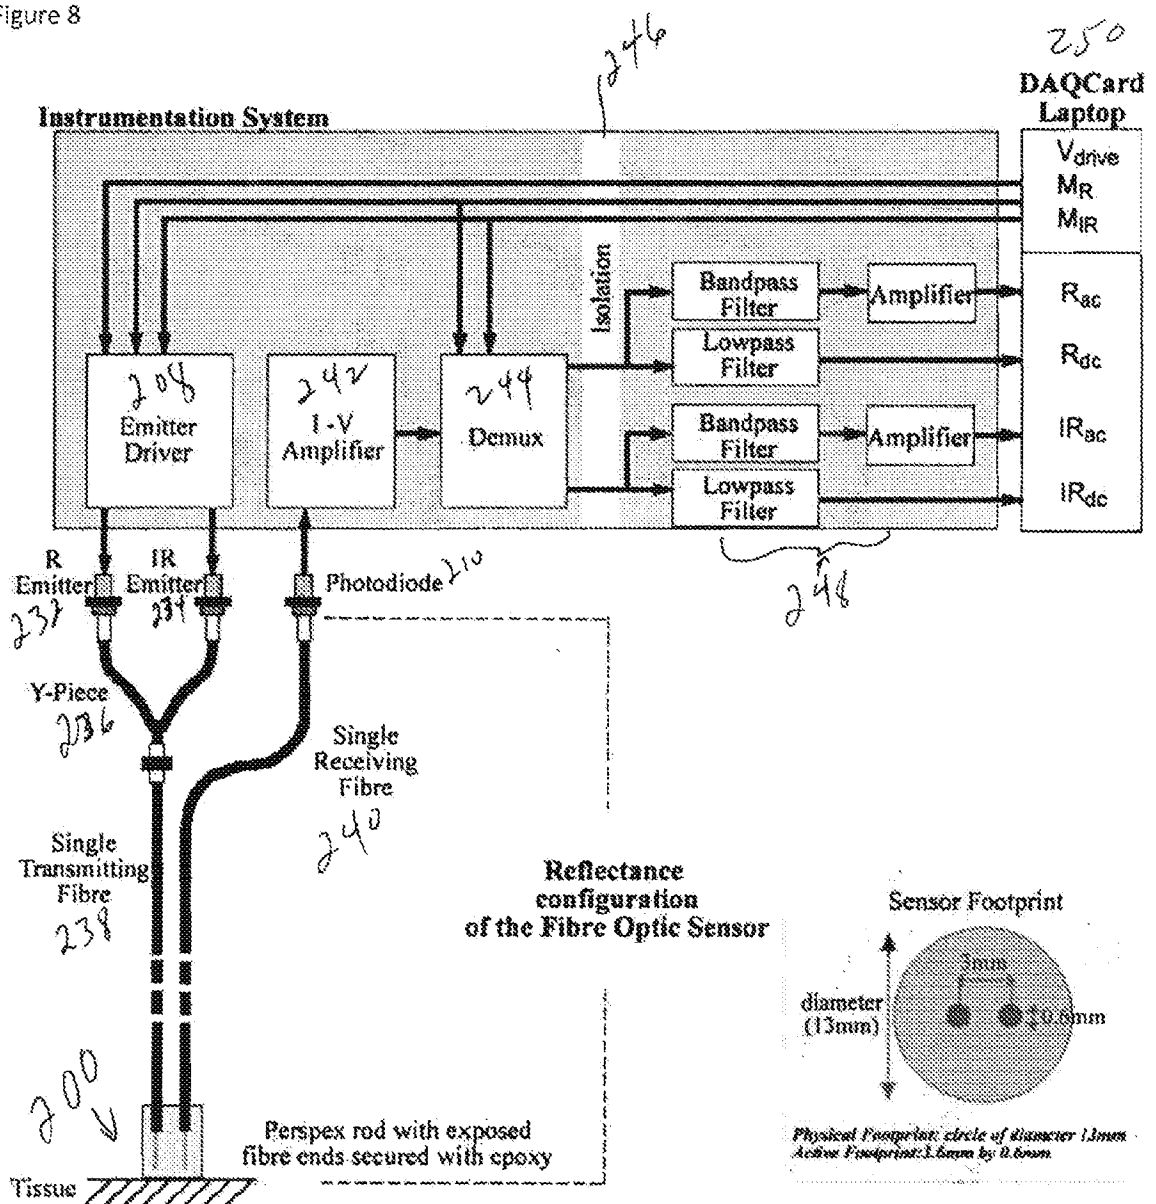


Figure 9


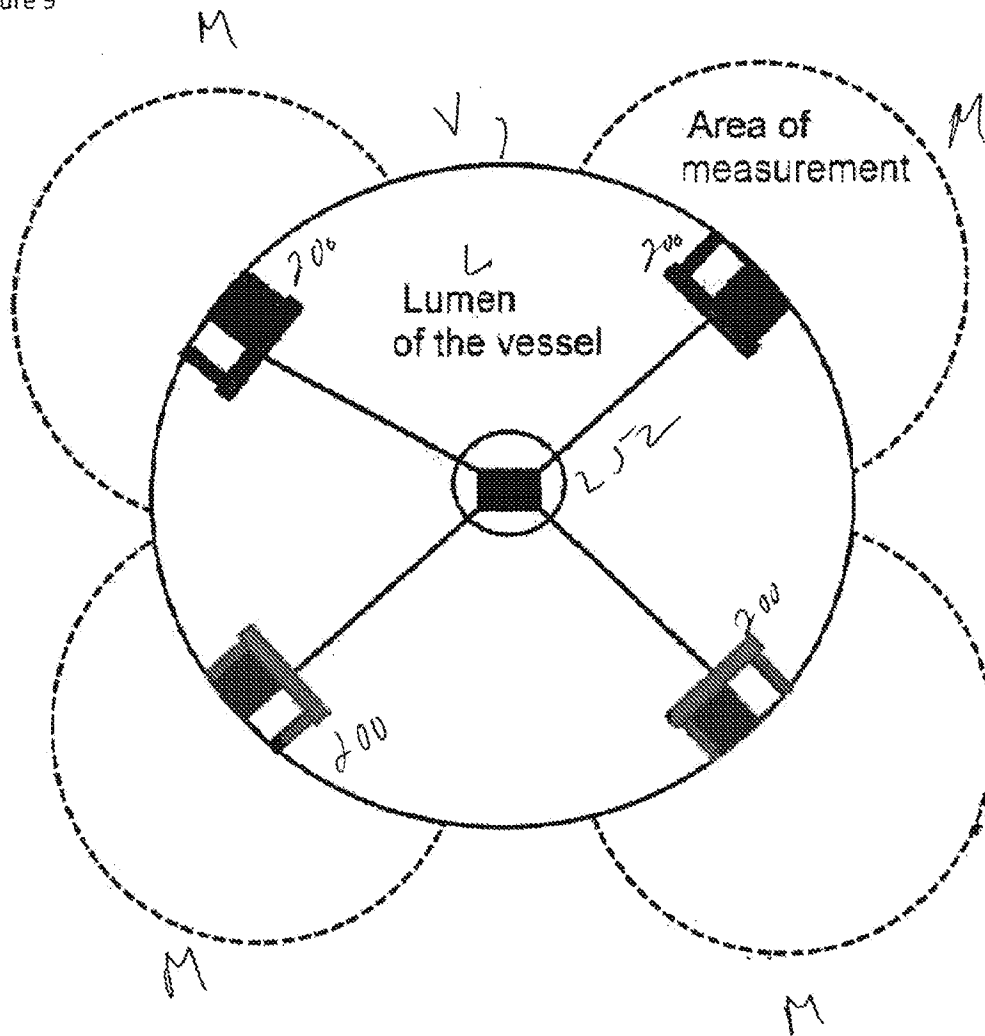


Figure 10

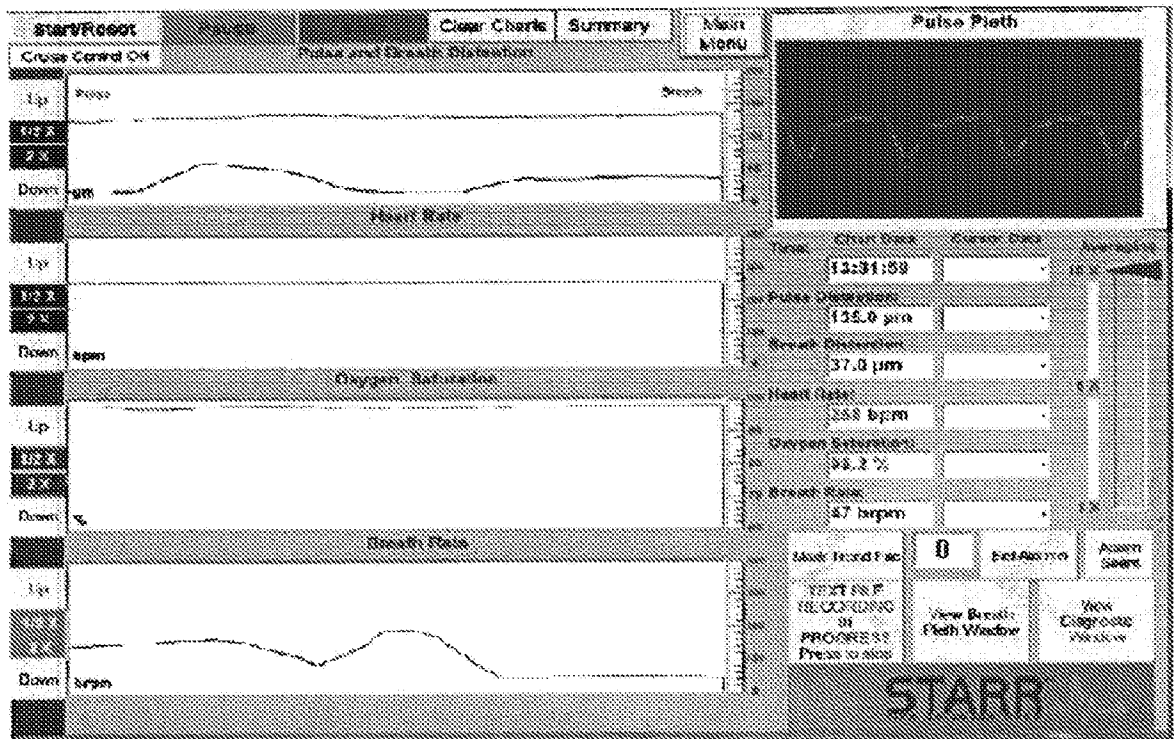

A. CLASSIFICATION OF SUBJECT MATTER**A61B 5/1455(2006.01)i, A61B 5/1459(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 5/1455; A61B 8/12; A61B 5/145; A61B 5/02; A61B 5/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: oximeter, vessel, emitter, detector

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2009-0240125 A1 (SUCH OLAF et al.) 24 September 2009 See abstract, paragraphs [0027]-[0031], claim 1 and figures 1-2.	1-17
A		18
Y	US 5205292 A (CZAR, CARL T. et al.) 27 April 1993 See abstract, column 2, line 63 - column 4, line 32, claim 1 and figures 1-4.	1-10
Y	US 2006-0129050 A1 (MARTINSON JAMES B. et al.) 15 June 2006 See abstract, paragraphs [0126]-[0132], claim 1 and figures 13,18A-18B.	11-17
A	US 2003-0139656 A1 (KIANI MASSI E. et al.) 24 June 2003 See abstract, paragraphs [0025]-[0030], claim 1 and figures 1-3.	1-18
A	JP 2004-329607 A (NIPPON KODEN CORP.) 25 November 2004 See abstract, paragraphs [0026]-[0034], claim 1 and figures 1-4.	1-18



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

24 June 2013 (24.06.2013)

Date of mailing of the international search report

24 June 2013 (24.06.2013)

Name and mailing address of the ISA/KR

Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City,
302-701, Republic of Korea

Facsimile No. 82-42-472-7140

Authorized officer

KIM, Tae Hoon

Telephone No. 82-42-481-8407



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/031236

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2009-0240125 A1	24.09.2009	AT535184 T CN101080192 A0 CN101080192 B EP 1830695 A2 EP 1830695 B1 US 8315682 B2 WO 2006-064399 A2 WO 2006-064399 A3	15.12.2011 28.11.2007 08.09.2010 12.09.2007 30.11.2011 20.11.2012 22.06.2006 31.08.2006
US 05205292 A	27.04.1993	CA 2103237 A1 CA 2103237 C EP 0602048 A1 EP 0602048 B1 US 05284146 A WO 92-21284 A1	04.12.1992 10.06.2003 18.06.1997 22.03.2000 08.02.1994 10.12.1992
US 2006-0129050 A1	15.06.2006	EP 1816951 A2 EP 1819278 A2 US 2006-0271112 A1 US 2012-271200 A1 US 8308794 B2 WO 2006-055443 A2 WO 2006-055443 A3 WO 2006-055547 A2	15.08.2007 22.08.2007 30.11.2006 25.10.2012 13.11.2012 26.05.2006 03.05.2007 26.05.2006
US 2003-0139656 A1	24.07.2003	US 6526300 B1 US 6771994 B2	25.02.2003 03.08.2004
JP 2004-329607 A	25.11.2004	JP 4131434 B2	13.08.2008