

## (12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
08 March 2018 (08.03.2018)

(10) International Publication Number  
WO 2018/041963 A1

(51) International Patent Classification:  
*A61M 1/10* (2006.01)      *A61M 1/36* (2006.01)

DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(21) International Application Number:  
PCT/EP2017/071890

(22) International Filing Date:  
31 August 2017 (31.08.2017)

(25) Filing Language: English

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

(26) Publication Language: English

(30) Priority Data:  
16186860.9      01 September 2016 (01.09.2016) EP

(71) Applicant: ABIOMED EUROPE GMBH [DE/DE];  
Neuenhofer Weg 3, 52074 Aachen (DE).

(72) Inventors: SIESS, Thorsten; c/o Abiomed Europe GmbH, Neuenhofer Weg 3, 52074 Aachen (DE). SPANIER, Gerd; c/o Abiomed Europe GmbH, Neuenhofer Weg 3, 52074 Aachen (DE). ABOULHOSN, Walid; c/o Abiomed Europe GmbH, Neuenhofer Weg 3, 52074 Aachen (DE).

(74) Agent: KLUNKER IP PATENTANWÄLTE PARTG  
MBB; Destouchesstraße 68, 80796 München (DE).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,

## Declarations under Rule 4.17:


— of inventorship (Rule 4.17(iv))

## Published:

— with international search report (Art. 21(3))

## (54) Title: BLOOD PUMP WITH FLOW CANNULA

FIG 1

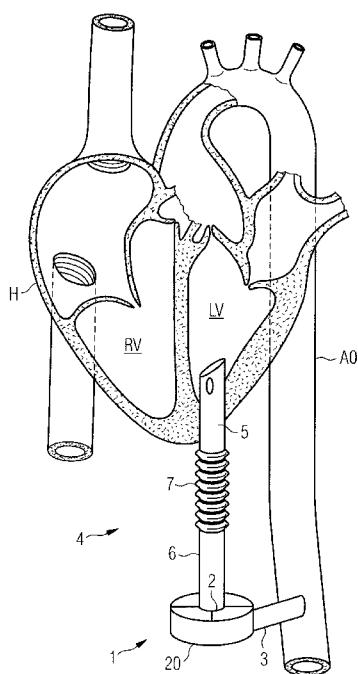

(57) Abstract: A blood pump (1) for supporting a patient's heart comprises a flow cannula (4) having a distal end (10) and a proximal end (11) opposite the distal end (10), wherein the distal end (10) of the flow cannula (4) is configured to be connected to the patient's heart or a blood vessel in order to establish a fluid communication between the blood pump (1) and the patient's heart and blood vessel, respectively. The flow cannula (4) comprises a distal portion (5) having said distal end (10) and a proximal portion (6) having said proximal end (11). The flow cannula (4) further comprises an intermediate portion (7) attached to the distal portion (5) and the proximal portion (6), wherein the intermediate portion (7) allows twisting thereof with a lower force than the distal portion (5) and the proximal portion (6). The intermediate portion (7) is configured to be fully occluded by twisting it. At least a portion of the intermediate portion (7) either alone or in combination with the distal portion (5) is adapted to be permanently attached to the patient's heart or a blood vessel.

## BLOOD PUMP WITH FLOW CANNULA

## BACKGROUND

**[0001]** This invention relates to a flow cannula for a blood pump for supporting a patient's heart. The flow cannula is configured for connecting the blood pump to the patient's heart or a blood vessel. The flow cannula can be separated such that a part connected to the heart or blood vessel remains inside the patient's thorax after removing the blood pump. The invention further relates to a method of removing a blood pump from a patient.

**[0002]** Blood pumps may be inserted into a patient's vessel such as the aorta by means of a catheter, or may be placed in the thoracic cavity or even outside the patient's body. In some applications, and in particular in those cases in which the blood pump is not placed intravascularly, it may be necessary to establish a direct connection to a blood vessel or the heart, e.g. the left ventricle. The flow cannula of the blood pump is inserted into an opening of the heart and secured to the wall of the heart to establish a fluid communication between the blood pump and the patient's heart. An outflow of the blood pump may then be connected to the aorta to pump blood from the left ventricle directly into the aorta.

**[0003]** If the blood pump is no longer needed, e.g. because the heart has recovered, the blood pump is removed. However, complete removal of the flow cannula from the heart would usually require an open thorax surgery and would involve a high risk of severe bleeding, and the opening in the heart would have to be closed. Therefore, the flow cannula is usually separated, e.g. cut, such that the part connected to the heart remains inside the patient's thorax. A clip, clamp or the like is used to close the remaining part of the flow cannula. However, the flow cannula is usually cut close below the patient's skin to facilitate handling if complications occur. Thus, the remaining part of the flow cannula is usually relatively long and the clamp may be bulky. This may affect the surrounding tissue and may cause irritations or even inflammations. Apart from that, there may be a risk that the flow cannula, which may be relatively stiff and may have a relatively large diameter, cannot be clamped tightly such that blood leaks into the patient's thorax.

## SUMMARY OF THE INVENTION

**[0004]** It is therefore an object of the present invention to provide a flow cannula for a blood pump, and a blood pump with such a flow cannula, wherein the flow cannula can be easily occluded to stop the blood flow and subsequently separated, both 5 preferably by a minimally invasive procedure, wherein further preferably interference of a part of the flow cannula that remains inside the patient with surrounding tissue can be reduced.

**[0005]** This object is achieved according to the present invention by a flow cannula and a method having the features of the independent claims. Preferred 10 embodiments and further developments of the invention are specified in the claims dependent thereon.

**[0006]** According to the invention, a flow cannula for a blood pump for supporting a patient's heart comprises a distal end and a proximal end opposite the distal end along a longitudinal axis of the flow cannula. The distal end of the flow 15 cannula is configured to be connected to the patient's heart or a blood vessel in order to establish a fluid communication between the blood pump and the patient's heart and blood vessel, respectively. The flow cannula comprises a distal portion having said distal end, a proximal portion having said proximal end. The flow cannula further comprises an intermediate portion attached to at least one of the distal portion and the 20 proximal portion. The intermediate portion allows at least one of clamping and twisting, in particular twisting, thereof with a lower force than at least one of the distal portion and the proximal portion. The intermediate portion is configured to be fully occluded by twisting thereof. Throughout this disclosure, the term "distal" refers to directions away from a user, e.g. a surgeon, and towards the heart, whereas the term "proximal" refers to 25 directions towards a user.

**[0007]** At least a portion of the intermediate portion either alone or in combination with the distal portion is adapted to be permanently attached to the patient's heart or a blood vessel. In other words, said portion of the intermediate portion either alone or in combination with the distal portion is adapted to remain inside the 30 patient's body after removal of the blood pump. Vice versa, preferably at least the

proximal portion, possibly the proximal portion and the distal portion, in combination with the remaining part of the intermediate portion is adapted to be removed from the patient's body. Since only a small part of the flow cannula is left behind in the patient, fewer irritations and inflammations occur.

5   **[0008]**       The flow cannula, which is designed in multiple portions, in particular a proximal portion, a distal portion and an intermediate portion allows for improved separation of the flow cannula during removal of the blood pump, wherein the portion that will remain in the patient's body causes less interference with surrounding tissue. The flow cannula can be easily occluded in a minimally invasive surgery by twisting the

10   intermediate portion. In particular, the intermediate portion is configured to be twisted such it is fully occluded and a blood flow through the flow cannula is stopped. Twisting of the intermediate portion can be caused by twisting the proximal portion relative to the distal portions because twisting of the intermediate portion requires less force than twisting of at least the distal portion, preferably both of the distal and proximal portions.

15   **[0009]**       Since the intermediate portion requires less force for twisting or clamping or both clamping and twisting, it can be easily and securely occluded. A smaller clamp or clip compared to a clamp or clip that would be necessary to occlude the distal portion is sufficient to occlude the intermediate portion of the flow cannula. Twisting of the intermediate portion allows for provisional occlusion of the flow

20   cannula which may then be finally closed by a clamp or clip or other suitable means, such as a cable, wire or the like. Since lower forces are required to manipulate the intermediate portion, the procedure of occluding the flow cannula and removing the proximal portion can be done minimally invasive, which bears less risk for the patient. Moreover, alternatively or in addition to twisting the intermediate portion, a loop or

25   cutting wire can be used that is looped around the intermediate portion to clamp it by pulling tight the loop or cutting wire. The term "clip" or "clamp" refers to a piece that is placed around the flow cannula, in particular the twisted portion of the intermediate portion, to securely and finally close it such that the flow cannula can be cut or otherwise separated. The clip or clamp can be applied in a minimally invasive procedure. In contrast to that, known cannulas may require bulky instruments, like a

scissor-like surgical clamp, to stop the blood flow. This can be done only in an open thorax surgery.

[0010] The distal and proximal portions of the flow cannula may be releasably connected to each other, e.g. by a releasable connector, such as a male/female connector, threads, bayonet mount, quick coupling, magnets or the like. Alternatively, the distal and proximal portions of the flow cannula may be connected via a predetermined breaking line, e.g. a circumferential notch. Thus, the proximal and distal portions can be separated by a low force while the intermediate portion remains attached to both the proximal portion and the distal portion.

10 [0011] Although releasably connected, however, inadvertent separation of the proximal and distal portions should be avoided. Therefore, in case a predetermined breaking line is provided, the predetermined breaking line should have a minimum resistance to withstand low breaking forces. In particular, it may be advantageous to design the predetermined breaking line such that an instrument, such as a hemostat or 15 other clamp or cutting tool, is necessary to separate the proximal and distal portions. It may also be possible to protect the predetermined breaking line, e.g. by a cover, or a tear strip or the like may be provided. One or more, such as two, three, four, five or six, security filaments may be provided attached to the proximal and distal portion, respectively, in order to keep the proximal and distal portions together. The security 20 filaments may be arranged outside the intermediate portion, e.g. evenly spaced about the circumference of the flow cannula. They may be cut or otherwise separated in order to allow separating the proximal and distal portions from each other.

[0012] When separated from each other, the proximal and distal portions may be axially movable with respect to each other, which may be achieved by axially 25 compressing or stretching the intermediate portion or by twisting the intermediate portion, which causes the proximal and distal portions to get closer to each other. Alternatively, the distal and proximal portions may be integrally formed and intended not to be separated. For example, the distal and proximal portions may form a single 30 tubular member, wherein the intermediate portion is placed over the tubular member like a jacket.

[0013] More specifically, the intermediate portion of the flow cannula may have a distal end and a proximal end, the distal end of the intermediate portion being attached to the distal portion of the flow cannula and the proximal end of the intermediate portion being attached to the proximal portion of the flow cannula. Consequently, while 5 the flow cannula is being prepared for complete separation no blood leaks from the flow cannula because the intermediate portion bridges the gap between the proximal and distal portions even when the proximal and distal portions have been separated. It will thus be appreciated that the intermediate portion is preferably attached to at least the distal portion, preferably both the proximal and distal portions, in a fluid tight manner in 10 order to conduct a blood flow between the distal portion and the proximal portion. For example, it may be glued, welded, clamped, bonded or otherwise attached. In embodiments, in which not both ends of the intermediate portion are attached, i.e. fixedly secured, to the proximal portion and distal portion, respectively, the respective free end may be at least disposed on or about the respective end portion.

[0014] In an embodiment the intermediate portion is attached to the distal and proximal portions of the flow cannula such that it at least partially overlaps at least one of, preferably each of, the distal and proximal portions of the flow cannula. That means that during operation of the blood pump, when the proximal and distal portions of the flow cannula are connected to each other, the intermediate portion does not have contact 15 with the blood flowing through the flow cannula if it completely overlaps the proximal and distal portions. Thus, the intermediate portion can be made of a variety of materials that would not be suitable for long term blood exposure. Further, the intermediate portion can be made of a very thin material, which could bear the risk of tearing if it had to conduct the blood flow during the entire operation of the blood pump. Only during 20 separation of the flow cannula, the intermediate portion will have direct contact with the blood flow as described in more detail below. Thus, in particular but not exclusively in this embodiment, the intermediate portion may have a wall thickness of less than about 150 $\mu$ m, preferably about 30 $\mu$ m, and may comprise a tubular polymer film, such as polyethylene terephthalate (e.g. Dacron $\circledR$ ), polyurethane or ePTFE. For instance, the 25 wall thickness may range from about 5  $\mu$ m to about 100  $\mu$ m for polyurethane and from 30

about 300 µm to about 1,000 µm for ePTFE. The thin polymer film is particularly suitable for twisting and thereby fully occluding the flow cannula as described above.

5 [0015] The intermediate portion may be gathered, in particular axially gathered, when the distal and the proximal portions of the flow cannula are connected to each other. The intermediate portion may behave in a bellows-like manner, i.e. it may fold in a zig-zag manner, or it may simply be compressed in an axial direction. If the intermediate portion is gathered or compressed when the proximal and distal portions are connected, the intermediate portion can unfold or decompress when the proximal and distal portions are moved away from each other without stretching it. In other words, there is no tension on the intermediate portion when the proximal and distal portions are spaced apart. This allows for easy clamping and if necessary twisting of the intermediate portion without having to hold a tension on the intermediate portion, which is advantageous for a minimally invasive procedure. However, in any embodiment, the intermediate portion may be stretchable in a direction of the longitudinal axis.

10 15 [0016] Apart from that, in any embodiment the intermediate portion is sized and dimensioned not to interfere with an axial movement of the proximal and distal portions, i.e. the intermediate portion is not too tight about the proximal and distal portions. For instance, a slight gap may be provided between the intermediate portion and at least one of, preferably both of, the proximal and distal portions. Since the 20 intermediate portion may be attached to the proximal and distal portions, the intermediate portion may be slightly tapered, i.e. have a slightly larger diameter in the middle compared to its ends.

25 [0017] In another embodiment, in particular where the distal and proximal portions are integrally formed, the intermediate portion may comprise an attachment member, such as a disc at its distal end, which is configured to be attached to the patient's heart, e.g. by suturing, in particular permanently. Preferably, the proximal end of the intermediate portion is attached to the proximal portion. In this embodiment, the proximal and distal portions of the flow cannula will not be separated but pulled out of the heart as a single piece. By pulling the proximal and distal portions, the intermediate 30 portion will be stretched or unfolded as described above such that it can be twisted and

clamped. The intermediate portion will be cut, such that only the attachment member along with a part of the intermediate portion is left behind in the patient to close the opening in the patient's heart. The proximal and distal portions are completely removed. In order to avoid inadvertent retraction of the proximal and distal portions, security 5 filaments similar to those mentioned above can be provided, which are secured to the attachment member and the proximal portion.

**[0018]** The attachment member is preferably made of a material that allows suturing of the attachment member to the tissue of the heart, such as a felt or the like. In one embodiment the attachment member may comprise radially extending sections, 10 such as three, four, five or six, with gaps between the sections. Upon twisting the intermediate portion, the sections will get closer to each other in a circumferential direction, such that the underlying heart tissue will be twisted and compressed in a circumferential direction about the opening to thereby narrow the opening in the heart tissue, in particular when the proximal and distal portions have been retracted from the 15 heart. This reduces the wound size after the flow cannula has been removed. The wound is then closed by means of the compressed attachment member and the part of the intermediate portion that remains inside the patient.

**[0019]** In still another embodiment the intermediate portion may be attached to the distal and proximal portions such that the distal and proximal portions are axially 20 spaced from each other and the intermediate portion is disposed between the distal and proximal portions. In other words, the proximal and distal portions are not directly connected to each other but are connected via the intermediate portion. In this embodiment, the intermediate portion conducts the blood flow during operation of the blood pump between the proximal and distal portions. Thus, in particular in this 25 embodiment, the intermediate portion may comprise a polymer tube, preferably silicone tube or polyurethane tube, which is suitable for long term blood exposure.

**[0020]** In any of the above described embodiments, the intermediate portion is preferably a flexible tubular member. The proximal and distal portions of the flow cannula preferably are tubular members, too. Advantageously, the distal portion of the 30 flow cannula is as short as possible, in either case shorter than the proximal portion of

the flow cannula in a longitudinal direction, wherein a length of the distal portion is preferably less than 50%, more preferably less than 25%, most preferably less than 15% of a length of the proximal portion. For example, the distal portion may have a length of 0.5 cm to 3 cm, e.g. 1 cm, and the proximal portion may have a length of 5 cm to 9 cm, 5 e.g. 7 cm. The flow cannula may have a diameter of about 2 to 15 mm, preferably about 6 to 8 mm.

**[0021]** Preferably, the blood pump is sized and configured to be placed in the patient's thoracic cavity. This allows an application in which the blood pump is fully implanted in a patient's body, e.g. connected to the patient's heart and aorta. In other 10 embodiments the blood pump may include a pumping device that is configured to be placed extracorporeal, wherein the flow cannula extends through the patient's skin.

**[0022]** A system may comprise a blood pump as described above and at least one clip or clamp that is sized and configured to be placed around the intermediate portion in order to fully occlude the flow cannula. In particular, the clip or clamp may 15 be sized and shaped to be placed around the intermediate portion when the proximal and distal portions are spaced from each other. After the clip or clamp has been placed around the intermediate portion, the proximal portion of the flow cannula can be removed, e.g. by cutting the intermediate portion as described in more detail below.

**[0023]** An exemplary method of using the blood pump as described above, in 20 particular removing the blood pump from a patient, includes the following steps. If the proximal and distal portions of the flow cannula are connected, e.g. by means of a releasable connector or predetermined breaking line, the proximal and distal portions are separated and axially moved apart from each other. The intermediate portion may then unfold or stretch but remains connected to the proximal and distal portions. The 25 intermediate portion is then occluded in order to occlude the flow cannula and stop the blood flow through the flow cannula. If necessary or indicated by the application, the intermediate portion may first be twisted in order to obtain a provisional occlusion. At the same time, by twisting the intermediate portion its diameter is reduced, which makes it possible to use a small clip. The twisted or untwisted intermediate portion is then 30 clamped by a clamp, clip or the like in order to fully and definitely occlude the flow

cannula. The proximal portion of the flow cannula can then be removed, e.g. by cutting the intermediate portion at a location proximal with respect to the clip. The distal portion along with part of the intermediate portion and the clip remains inside the patient. This procedure can be performed minimally invasively. The parts remaining 5 inside the patient are small and not bulky in order to reduce or avoid interference with surrounding tissue. Irritations and inflammations can be reduced or avoided.

**[0024]** In another exemplary embodiment, the proximal and distal portions form a single piece and will not be separated. The intermediate portion has an attachment member at its distal end that is securely attached to the patient's heart, while the 10 proximal end of the intermediate portion is attached to the proximal portion of the flow cannula. Once the flow cannula is to be removed, the single piece comprising the proximal and distal portions is pulled out of the heart, such that the intermediate portions unfolds and/or stretches. It is pulled far enough out of the heart to be able to twist and clamp and subsequently cut the intermediate portion. Only a distal part of the 15 intermediate portion along with the attachment member remains inside the patient. This can further reduce the size of material that is left behind in the patient and improve healing of the punch hole in the heart muscle.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0025]** The foregoing summary, as well as the following detailed description of 20 preferred embodiments, will be better understood when read in conjunction with the appended drawings. For the purpose of illustrating the present disclosure, reference is made to the drawings. The scope of the disclosure is not limited, however, to the specific embodiments disclosed in the drawings. In the drawings:

Fig. 1 shows a patient's heart with a blood pump attached thereto.

25 Figs. 2a and 2b show an embodiment of a flow cannula.

Figs. 3a to 3e show the flow cannula of Figs. 2a, 2b during use.

Figs. 4a to 4d show a flow cannula according to another embodiment during use.

Figs. 5a to 5e show a flow cannula according to another embodiment during use.

Fig. 6 shows an intermediate portion according to one embodiment.

30 Fig. 7 shows an intermediate portion according to another embodiment.

Figs. 8a and 8b schematically show an attachment member during use.

#### DETAILED DESCRIPTION

**[0026]** Referring to Fig. 1 a blood pump 1 is illustrated inserted into a patient's heart H. The blood pump 1 is placed in the thoracic cavity and is directly connected to the left ventricle LV of the heart H by means of a flow cannula 4, which in this application is an inflow cannula because blood is drawn into the flow cannula 4, conveyed into a pump casing 20 through an inlet 2 by means of an impeller (not shown) in the pump casing 20, and further conveyed out of the blood pump 1 through an outflow cannula 3 that is attached to the aorta AO. The flow cannula 4 has a distal portion 5 secured to the wall of the heart H, a proximal portion 6 connected to the inlet 2 of the pump casing 20 and an intermediate portion 7 attached to the distal portion 5 and proximal portion 6 as described in more detail below. The blood pump 1 supports the patient's heart H. Once the blood pump 1 is to be removed, the flow cannula 4 is separated and the remaining distal part of the flow cannula 4 is closed and left behind in the thoracic cavity.

**[0027]** The flow cannula 4 is illustrated in more detail in Figs. 2a and 2b. Fig. 2a shows an unassembled view in order to illustrate the connection 12 between the proximal and distal portions 5, 6. The proximal and distal portions 5, 6 are releasably connected to each other, e.g. by means of a predetermined breaking line, which may be formed e.g. by a circumferential notch (see enlarged cutout), or by any other releasable connector, such as threads, male/female connector, bayonet mount or the like. The flow cannula 4 has a distal end 10 that is inserted into the patient's heart H as illustrated in Fig. 1 and an opposing proximal end 11 that is attached to the pump casing 20. The distal end 10 may be sloped or tapered to facilitate insertion into the heart H.

**[0028]** The intermediate portion 7 has a distal end 8 that is attached to the distal portion 5 and a proximal end 9 that is attached to the proximal portion 6 as shown in Fig. 2b. Thus, the intermediate portion 7 overlaps both the distal portion 5 and the proximal portion 6. It will be appreciated that the intermediate portion 7 may be attached to the distal and proximal portions 5, 6 such that it overlaps only one of them.

The intermediate portion 7 is gathered on the distal and proximal portion 5, 6. Since the distal and proximal portions 5, 6 are connected as shown in Fig. 2a, the intermediate portion 7 does not have contact to the blood flowing through the flow cannula 4 during operation of the blood pump 1.

5 [0029] With reference to Figs. 3a to 3e an exemplary method of removing a flow cannula from a patient's body, e.g. during removal of the blood pump 1 of Fig. 1, including the flow cannula 4 of Fig. 2b, is described. While the blood pump 1 is shown as a centrifugal blood pump, it will be appreciated that the flow cannula 4 can be used in combination with another medical device, in particular another type of blood pump, 10 such as an axial blood pump or a mixed-type (centrifugal/axial) blood pump. Fig. 3a is substantially the same view as Fig. 2b and shows the flow cannula 4 during operation of the blood pump 1. After operation of the blood pump 1 has been stopped, the flow cannula 4 has to be separated to remove the proximal portion 6 from the patient. As 15 illustrated in Fig. 3b, the proximal portion 6 is separated from the distal portion 5 by disconnecting the releasable connector 12, which may be done e.g. by breaking the flow cannula 4 at a predetermined breaking line. Other connection mechanisms, such as a threaded connection may be used but are not shown in Fig. 3b for the sake of simplicity. While the distal portion 5 remains attached to the patient's heart H, the proximal portion 6 is axially moved away from the distal portion 5. The intermediate portion 7 unfolds or 20 stretches and bridges the created gap between the distal and proximal portions 5, 6. Therefore, the intermediate portion 7 is attached to the proximal and distal portions 5, 6 in a fluid tight manner.

25 [0030] Since the intermediate portion 7 is made of a thin polymer film, it can be easily twisted to provisionally fully occlude the flow cannula 4 as shown in Fig. 3c to stop the blood flow through the flow cannula 4. A clip 13 is then placed around the twisted intermediate portion 7 (Fig. 3d) for final occlusion and the intermediate portion 7 is separated, e.g. by cutting (Fig. 3e). The remaining parts do not require much space in the thoracic cavity and can remain in the thoracic cavity without causing severe irritations or inflammations.

**[0031]** With reference to Figs. 4a to 4d an exemplary method during removal of a blood pump according to another embodiment is described. In contrast to the embodiment of Figs. 3a to 3e, the flow cannula 14 comprises an intermediate portion 17 that does not overlap the distal and proximal portions 15, 16 but is disposed between them and connected to the proximal portion 15 with its proximal end 18 and to the distal portion 16 with its distal end 19. Thus, the intermediate portion 17 is in contact with the blood flowing through the flow cannula 14 and is preferably made of a material suitable for long term blood exposure, such as silicone or polyurethane. The intermediate portion 17 is not as thin as the intermediate portion 7 of the previous embodiment, but is softer than the distal and proximal portions 15, 16 to allow clamping and if applicable twisting thereof with a lower force than at least the distal portion 15.

**[0032]** As shown in Fig. 4b, the intermediate portion 17 is twisted to create a provisional full occlusion of the flow cannula 14 to stop the blood flow through the flow cannula 14. It will be appreciated that this step may be omitted and that the clip 13 (Fig. 4c) can be placed over the twisted or untwisted intermediate portion 17 to create a full occlusion of the flow cannula 14. As in the previous embodiment, the intermediate portion 17 is then separated to remove the proximal portion 16 from the patient, while the distal portion 15 remains attached to the patient's heart H (Fig. 4d).

**[0033]** With reference to Figs. 5a to 5e an exemplary method during removal of a blood pump according to yet another embodiment is described. The flow cannula 24 includes a jacket-like intermediate portion 27 that comprises an attachment member 30, which may be in the form of a disc, plate or sheet, at its distal end 29 opposite the proximal end 28, which is shown in more detail in Figs. 6 and 7. The attachment member 30 is directly attached to the patient's heart H, e.g. sutured, and is configured to stay attached to the heart H permanently. Except for the attachment member 30, the intermediate portion 27 is substantially similar to the intermediate portion 7 of the embodiment of Figs. 3a to 3e, e.g. with respect to the material and rigidity characteristics. The flow cannula 24 comprises a tube having a proximal portion 26 and a distal portion 25 that are integrally formed. In contrast to the previous embodiments, the proximal portion 26 and distal portion 25 will not be separated but are formed as a single piece. The intermediate portion 27 is placed over the tube and may be connected

to particularly the proximal portion 26 with the proximal end 28. It may be sufficient if the intermediate portion 27 is attached to the proximal portion 26 by friction fit but a secure and fluid tight attachment may be preferred.

5 [0034] During operation of the blood pump, the attachment member 30, which may be made of a felt material or the like, is fixed to the heart H, e.g. sutured, and the distal portion 25 extends into the heart H (Fig. 5a). When the blood pump is to be removed, the tube including the proximal portion 26 and the distal portion 25 is pulled out of the heart H as shown in Fig. 5b. Since the disc 30 is securely fixed to the heart H and the proximal end 28 of the intermediate portion 27 is attached to the proximal portion 26, the intermediate portion 27 will unfold or stretch as shown in Fig. 5b. It will be appreciated that any fixation between the intermediate portion 27 and the proximal portion 26 would be appropriate that allows for this action, e.g. permanent fixation or sufficiently strong friction fit. It may be possible that the proximal end 28 of the intermediate portion 27 slides along the proximal portion 26.

15 [0035] In order to prevent the tube from being pulled out of the heart accidentally, security filaments 31 are provided that attach to the tube and the attachment member 30 as shown in Fig. 5a. They are cut or otherwise separated in order to be able to retract the tube as shown in Fig. 5b. The part of the security filaments 31 that remains inside the patient's body is kept as short as possible. More than one, such 20 as two, three, four, five or six security filament 31 may be provided.

25 [0036] As in the previous embodiments, the intermediate portion 27 is twisted to provisionally close it (Fig. 5c) to stop the blood flow through the flow cannula 24. This is done by twisting the proximal portion 26, which requires sufficient fixation of the intermediate portion 27 on the proximal portion 26. The intermediate portion 27 is then clamped by clip 13 (Fig. 5d). Finally, the intermediate portion 27 is cut, such that the entire tube including the distal portion 25 and the proximal portion 26 along with the cut part of the intermediate portion 27 are removed from the patient. Only the attachment member 30 with a distal part of the intermediate portion 27 remains inside the patient attached to the heart H to close the opening in the heart H. Since only a small part of the

flow cannula 24 remains inside the patient, irritations of the surrounding tissue and the risk of inflammations can be reduced.

5 [0037] As shown in Figs. 6 and 7 the attachment member 30 may be designed in accordance with different embodiments. Preferably, the attachment member is made of or comprises a material that allows suturing the attachment member to the patient's heart. A suitable material may be a felt or the like. The attachment member 30 may be a disc, sheet or the like as shown in Fig. 6 and may assume any appropriate shape, such as rounded, circular, rectangular, polygonal or the like. For instance, a surgeon may adapt the size and shape by cutting the edges of the attachment member 30.

10 [0038] In another embodiment as shown in Fig. 7, the attachment member 30 may comprise a plurality of, such as three, four, five or six, sections 32 separated by respective gaps 33. The sections 32 extend radially from the intermediate portion 27. Referring again to Figs. 5c to 5e and to Figs. 8a and 8b, providing sections 32 instead of a continuous disc or sheet has the advantage that during twisting of the intermediate 15 portion 27, the sections 32 get closer to each other and thereby twist and narrow the punch hole in the heart tissue as indicated by arrows in Fig. 8b, which reduces the wound size.

## CLAIMS

1. A flow cannula (4; 14; 24) for a blood pump (1) for supporting a patient's heart, the flow cannula (4; 14; 24) comprising a distal end (10) and a proximal end (11) opposite the distal end (10) along a longitudinal axis of the flow cannula (4; 14; 24), the distal end (10) of the flow cannula (4; 14; 24) configured to be connected to the patient's heart or a blood vessel in order to establish a fluid communication between the blood pump (1) and the patient's heart and blood vessel, respectively, the flow cannula (4; 14; 24) comprising a distal portion (5; 15; 25) having said distal end (10) and a proximal portion (6; 16; 26) having said proximal end (11), the flow cannula (4; 14; 24) further comprising an intermediate portion (7; 17; 27) attached to at least one of the distal portion (5; 15; 25) and the proximal portion (6; 16; 26), wherein the intermediate portion (7; 17; 27) allows twisting thereof with a lower force than at least one of the distal portion (5; 15; 25) and the proximal portion (6; 16; 26), wherein the intermediate portion (7; 17; 27) is configured to be fully occluded by twisting thereof, wherein at least a portion of the intermediate portion (7; 17; 27) either alone or in combination with the distal portion (5; 15; 25) is adapted to be permanently attached to the patient's heart or a blood vessel.
2. The flow cannula of claim 1, wherein the intermediate portion (7; 17; 27) of the flow cannula (4; 14; 24) has a distal end (8; 18; 28) and a proximal end (9; 19; 29), the distal end (8; 18; 28) of the intermediate portion (7; 17; 27) being attached to or arranged on the distal portion (5; 15; 25) of the flow cannula (4; 14; 24) and the proximal end (9; 19; 29) of the intermediate portion (7; 17; 27) being attached to or arranged on the proximal portion (6; 16; 26) of the flow cannula (4; 14; 24).
3. The flow cannula of claim 1 or 2, wherein the intermediate portion (7; 17; 27) is attached to at least one of the distal portion (5; 15; 25) and the proximal portion (6; 16; 26), preferably both the distal and proximal portions (5, 6; 15, 16; 25, 26), of the flow cannula (4; 14; 24) in a fluid tight manner in order to conduct a blood flow between the distal portion (5; 15; 25) and the proximal portion (6; 16; 26).
4. The flow cannula of any one of claims 1 to 3, wherein the intermediate portion (7; 27) is attached to or arranged on the distal and proximal portions (5, 6; 25; 26) of the

flow cannula (4; 24) such that it at least partially overlaps at least one of, preferably each of, the distal and proximal portions (5, 6; 25; 26) of the flow cannula (4; 24).

5. The flow cannula of any one of claims 1 to 4, wherein the distal portion (5) and the proximal portion (6) of the flow cannula (4) are releasably connected to each other.

5 6. The flow cannula of claim 5, wherein the intermediate portion (7) is axially gathered when the distal and the proximal portions (5, 6) of the flow cannula (4) are connected to each other.

7. The flow cannula of any one of claims 1 to 4, wherein the intermediate portion (27) comprises an attachment member (30) at a distal end (28) thereof, the attachment member (30) being configured to be attached to the patient's heart, wherein preferably a proximal end (29) of the intermediate portion (27) is attached to the proximal portion (26), wherein further preferably the distal portion (25) and the proximal portion (26) are integrally formed.

8. The flow cannula of any one of claims 1 to 3, wherein the intermediate portion (17) is attached to the distal portion (15) and the proximal portion (16) of the flow cannula (14) such that the distal portion (15) and the proximal portion (16) are axially spaced from each other and the intermediate portion (17) is disposed between the distal portion (15) and the proximal portion (16).

9. The flow cannula of any one of claims 1 to 8, wherein the intermediate portion (7; 17; 27) is a flexible tubular member.

10. The flow cannula of any one of claims 1 to 9, wherein the intermediate portion (7; 17; 27) is stretchable in a direction of the longitudinal axis.

11. The flow cannula of any one of claims 1 to 10, wherein the intermediate portion (7; 27) has a wall thickness of about 5  $\mu\text{m}$  to about 1,000  $\mu\text{m}$ , preferably less than about 150  $\mu\text{m}$ , more preferably less than about 50  $\mu\text{m}$ , still more preferably about 30  $\mu\text{m}$ .

12. The flow cannula of any one of claims 1 to 11, wherein the intermediate portion (7; 27) comprises a tubular polymer film, preferably a polymer material that induces

tissue ingrowth, more preferably polyethylene terephthalate, or wherein the intermediate portion (17) comprises a polymer tube, preferably silicone tube or polyurethane tube.

13. A blood pump (1) for supporting a patient's heart, comprising a flow cannula (4; 14; 24) of any one of claims 1 to 12.

5 14. The blood pump claim 13, wherein the blood pump is sized and configured to be placed in the patient's thoracic cavity.

15. A system, comprising a flow cannula (4; 14; 24) of any one of claims 1 to 12 or a blood pump of claim 13 or 14, and at least one clip (13) that is sized and configured to be placed around the intermediate portion (7; 17; 27) of the flow cannula (4; 14; 24) in 10 order to fully occlude the flow cannula (4; 14; 24).

16. A method for removing a blood pump (1) from a patient, wherein the blood pump (1) is in fluid communication with the patient's heart or a blood vessel via a flow cannula (4; 14; 24), the flow cannula (4; 14; 24) comprising a distal end (10) and a proximal end (11) opposite the distal end (10) along a longitudinal axis of the flow 15 cannula (4; 14; 24), the distal end (10) of the flow cannula (4; 14; 24) connected to the patient's heart or blood vessel in order to establish the fluid communication between the blood pump (1) and the patient's heart and blood vessel, respectively, the flow cannula (4; 14; 24) comprising a distal portion (5; 15; 25) having said distal end (10) and a proximal portion (6; 16; 26) having said proximal end (11), the flow cannula (4; 14; 24) 20 further comprising an intermediate portion (7; 17; 27) attached to at least one of the distal portion (5; 15; 25) and the proximal portion (6; 16; 26),

the method comprising the step of twisting the intermediate portion (7; 17; 27) such that it is fully occluded to stop a blood flow through the flow cannula (4; 14; 24).

25 17. The method of claim 16, further comprising the step of attaching a clip (13) around the twisted intermediate portion (7; 17; 27) in order to definitely occlude the flow cannula (4; 14; 24).

18. The method of claim 16 or 17, further comprising the step of removing the proximal portion (6; 16; 26) of the flow cannula (4; 14; 24) by separating the

intermediate portion (7; 17; 27) at a location proximal with respect to the clip (13), wherein at least a portion of the intermediate portion (7; 17; 27) either alone or in combination with the distal portion (5; 15; 25) remains permanently attached to the patient's heart or blood vessel.

- 5 19. The method of any one of claims 16 to 18, further comprising the step of separating the proximal and distal portions and axially moving the proximal and distal portions apart from each other before twisting the intermediate portion.
20. The method of any one of claims 16 to 19, further comprising the step of unfolding or stretching the intermediate portion (7; 17; 27) before twisting it.
- 10 21. The method of any one of claims 16 to 20, performed in a minimally invasive surgery.

FIG 1

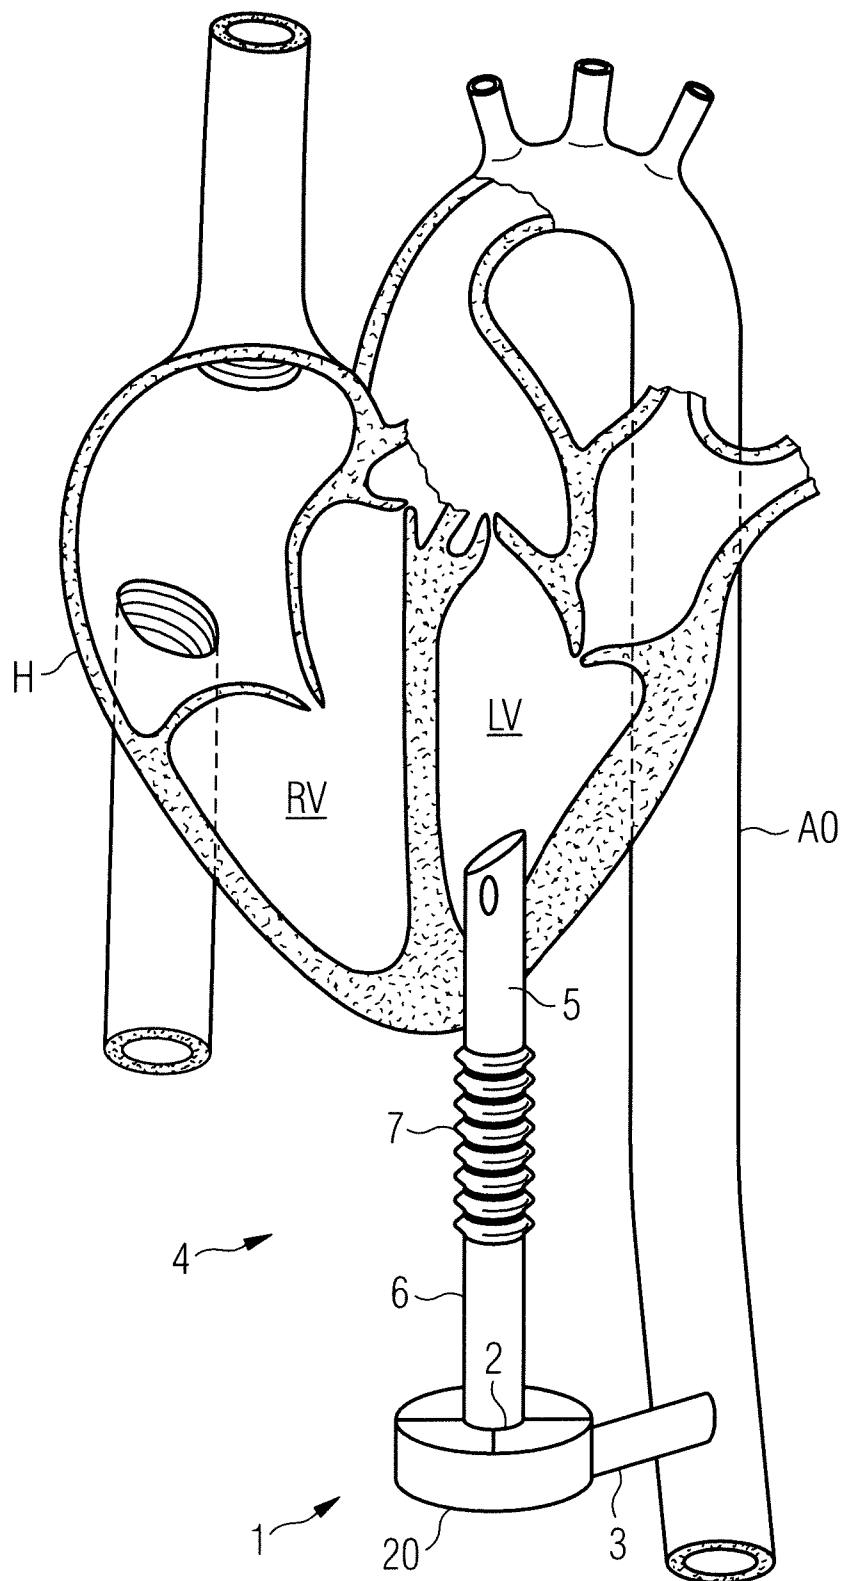


FIG 2a

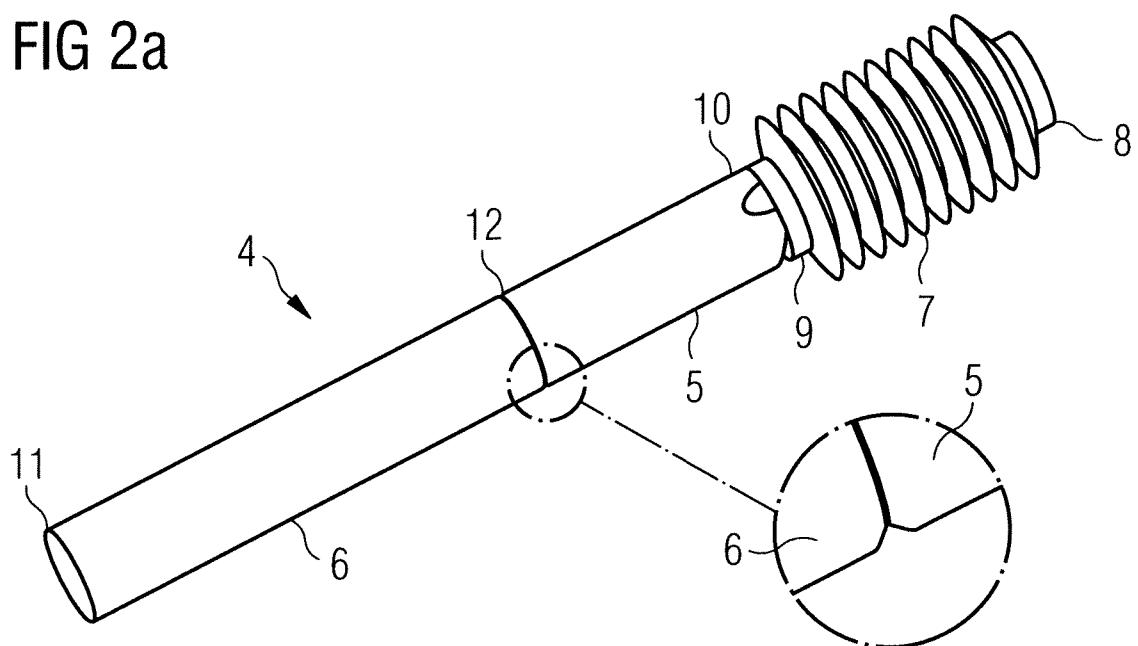


FIG 2b

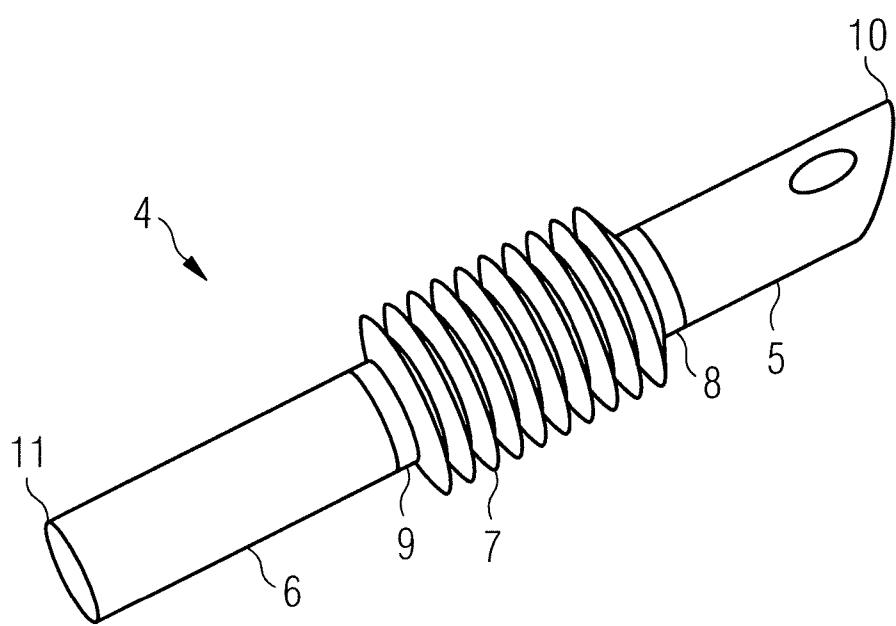


FIG 3a

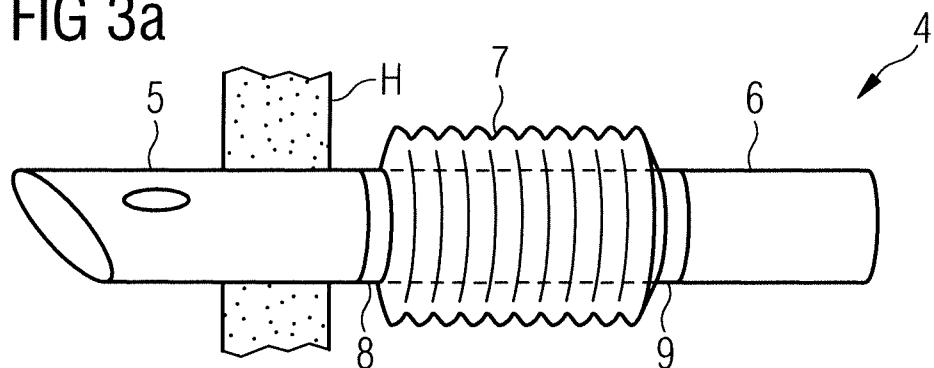


FIG 3b

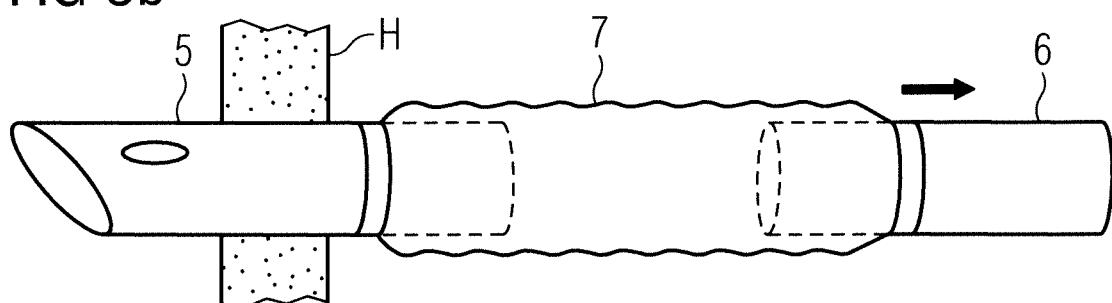


FIG 3c

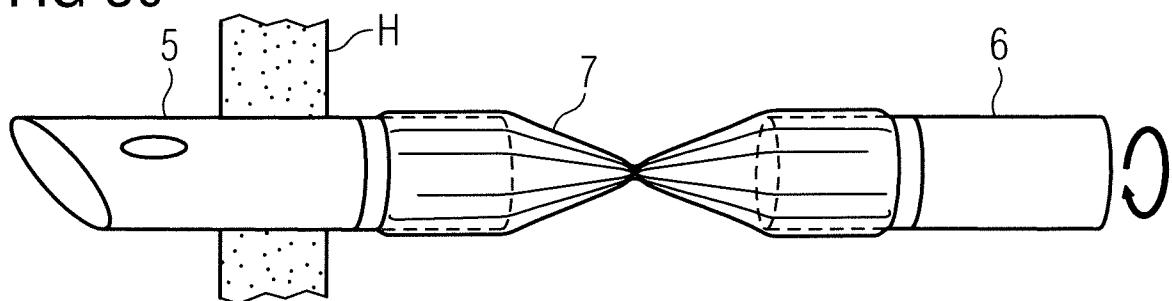


FIG 3d

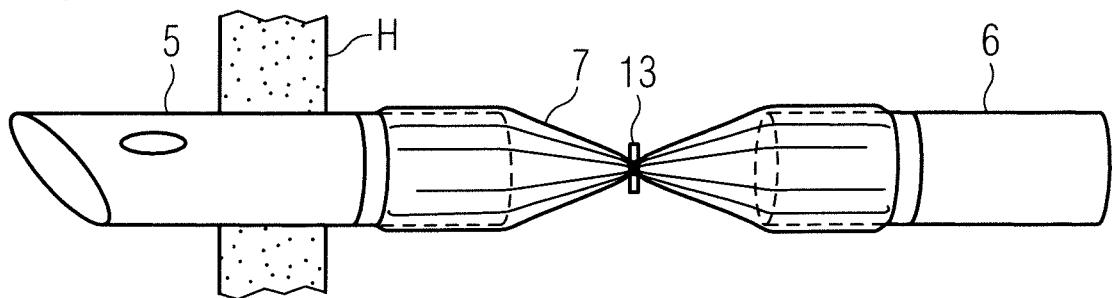


FIG 3e

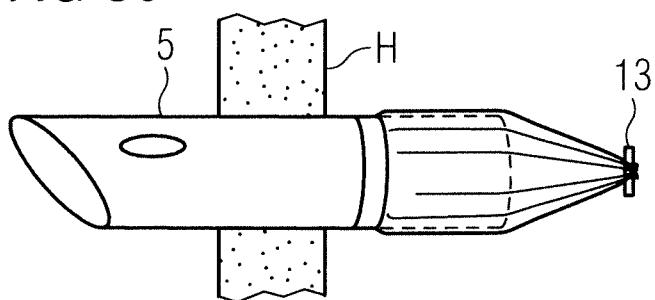


FIG 4a

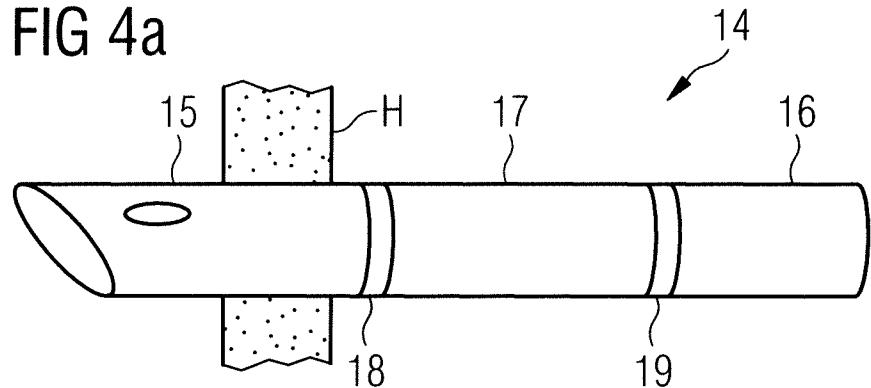


FIG 4b

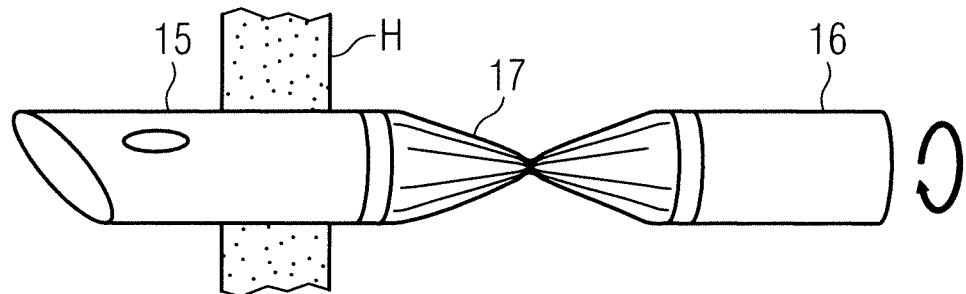


FIG 4c

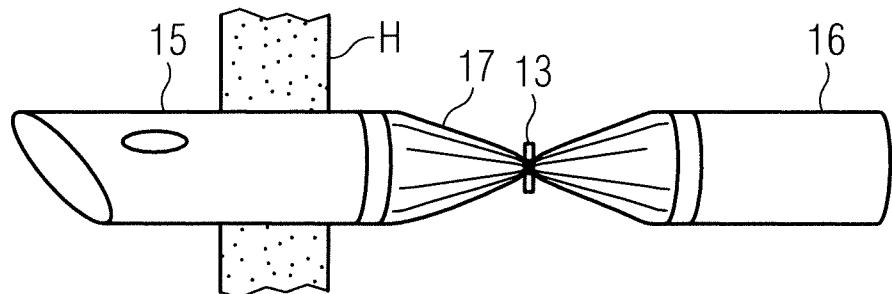


FIG 4d

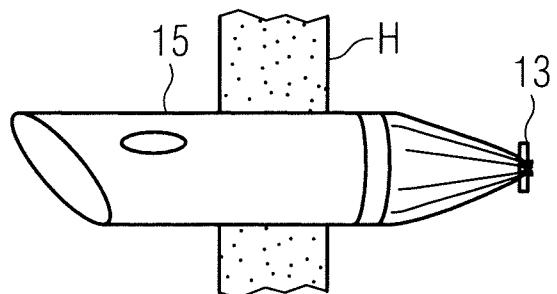


FIG 5a

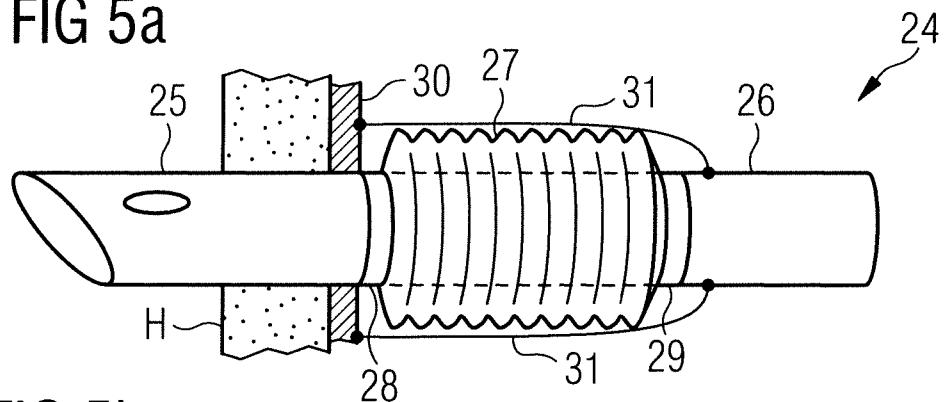


FIG 5b

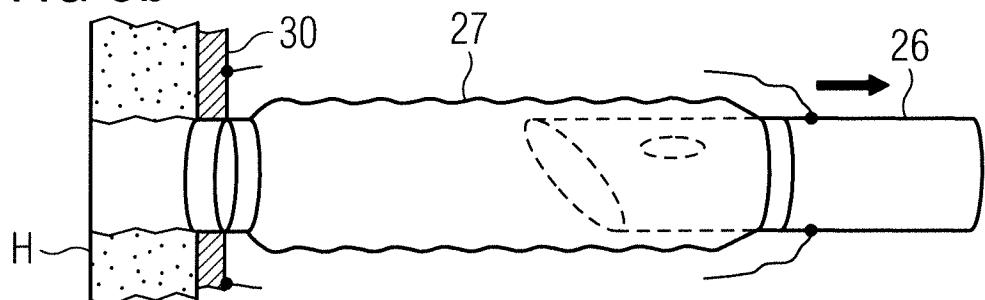


FIG 5c

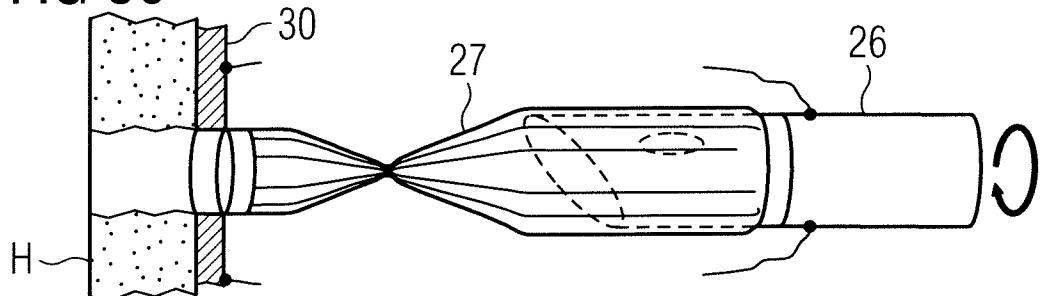


FIG 5d

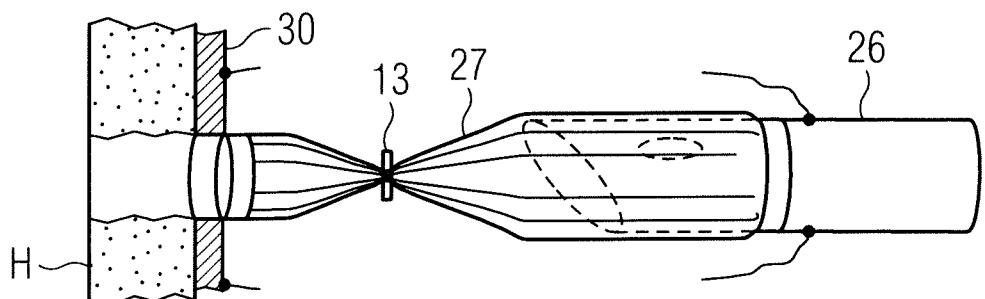


FIG 5e

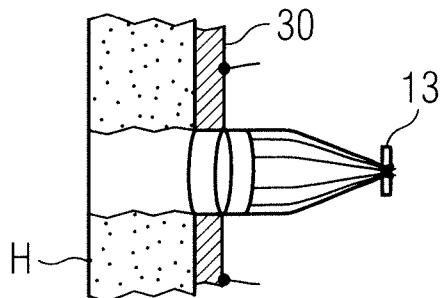


FIG 6

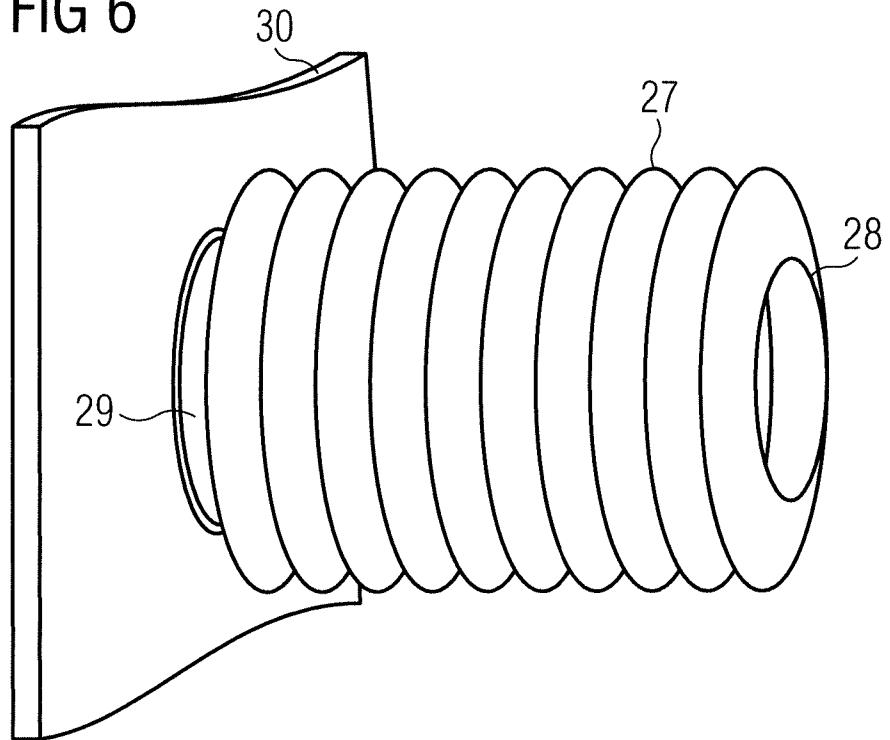


FIG 7

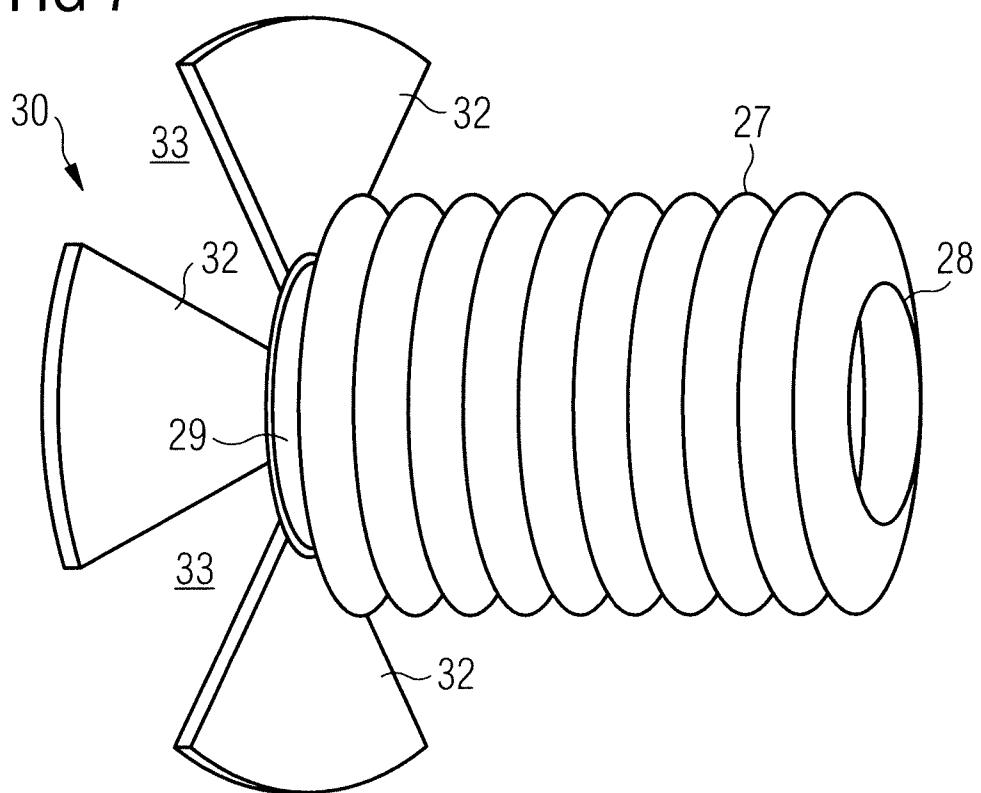


FIG 8a


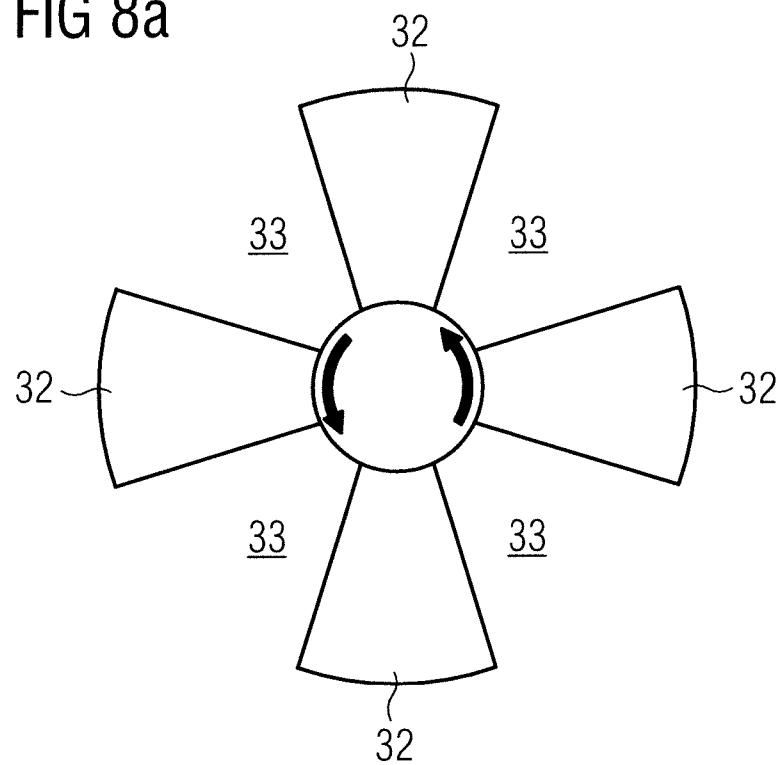


FIG 8b

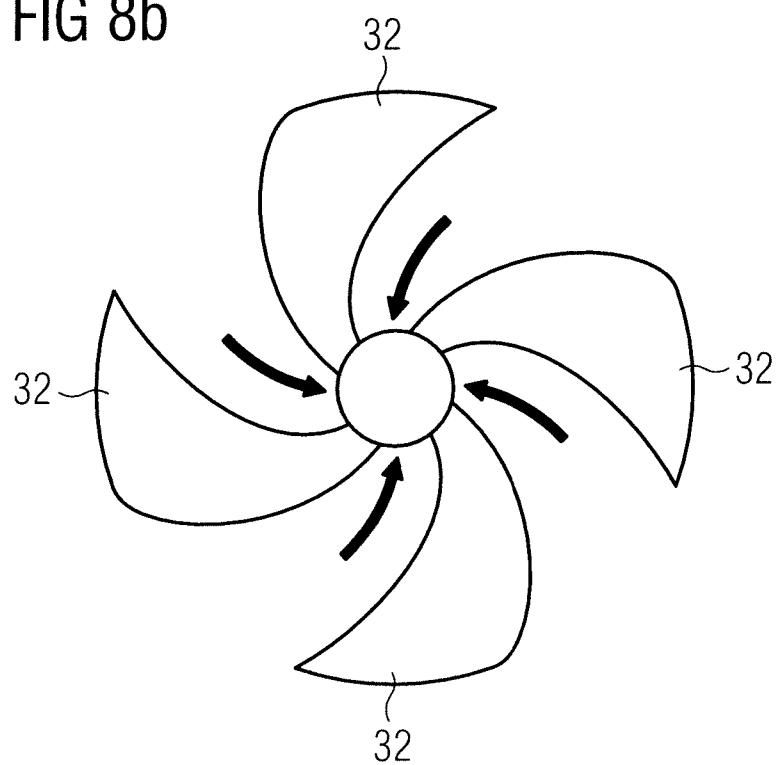

# INTERNATIONAL SEARCH REPORT

International application No  
PCT/EP2017/071890

**A. CLASSIFICATION OF SUBJECT MATTER**  
INV. A61M1/10 A61M1/36  
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)

A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>US 2004/059178 A1 (MCCARTHY PATRICK M [US] ET AL) 25 March 2004 (2004-03-25) flexible conduit 60 ; surgical clamp 100 [0071] The apparatus 10 thus provides the ability to temporarily occlude blood flow through the inflow cannula 12 to the VAD 14. This ability to occlude blood flow through the inflow cannula 12 can be useful in cases where the VAD 14 has allowed the heart to heal itself and the VAD is to be removed, as well as cases where the VAD remains implanted but requires service or replacement of certain parts; paragraphs [0070] - [0071]; figures 7,8 the whole document</p> <p style="text-align: center;">-----</p> <p style="text-align: center;">-/-</p>	1-15

Further documents are listed in the continuation of Box C.

See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

Date of mailing of the international search report

4 December 2017

20/12/2017

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040,  
Fax: (+31-70) 340-3016

Authorized officer

Van Veen, Jennifer

**INTERNATIONAL SEARCH REPORT**International application No  
PCT/EP2017/071890

## C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6 186 999 B1 (CHEN JI-FENG [US]) 13 February 2001 (2001-02-13) flexible tube (18); clamp (44); cuff (32); figures 1,2 -----	1-15
A	US 2014/303427 A1 (KERKHOFFS WOLFGANG [DE] ET AL) 9 October 2014 (2014-10-09) clamp (209;309a,b); paragraphs [0076], [0078], [0079]; figure 1 -----	1-15

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/EP2017/071890

### Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1.  Claims Nos.: **16-21**  
because they relate to subject matter not required to be searched by this Authority, namely:  
see FURTHER INFORMATION sheet PCT/ISA/210
2.  Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3.  Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

### Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1.  As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2.  As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3.  As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4.  No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

#### Remark on Protest

The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.

The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.

No protest accompanied the payment of additional search fees.

**FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210**

Continuation of Box II.1

Claims Nos.: 16-21

Claims 16-21 refer to a method for treatment of the human or animal body by therapy and/or surgery, which is against Rule 39.1 (iv) pCT and Rule 67.1 (iv) PCT. The reason is that they include the step of removing a blood pump from a patient, wherein the blood pump is in fluid communication with the patient's heart or a blood vessel. This Authority is not required to search the present application with respect to the aforementioned claim/s (Article 17(2)(b) PCT and Rule 39.1(iv) PCT). Consequently, no International Search Report and no Written Opinion (Rule 67.1 PTC in combination with Rule 43bis.1(b) PCT) have been established with respect to it/them.

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No

PCT/EP2017/071890

Patent document cited in search report	Publication date	Patent family member(s)			Publication date
US 2004059178	A1	25-03-2004	AU	2003277167 A1	08-04-2004
			US	2004059178 A1	25-03-2004
			WO	2004026124 A2	01-04-2004
-----					
US 6186999	B1	13-02-2001	CA	2350793 A1	09-03-2000
			EP	1107811 A1	20-06-2001
			US	6186999 B1	13-02-2001
			WO	0012164 A1	09-03-2000
-----					
US 2014303427	A1	09-10-2014	US	2014303427 A1	09-10-2014
			WO	2014169023 A2	16-10-2014
-----					