



US011752262B2

(12) **United States Patent**
Al-Ali et al.

(10) **Patent No.:** **US 11,752,262 B2**
(45) **Date of Patent:** **Sep. 12, 2023**

(54) **HEMOGLOBIN DISPLAY AND PATIENT TREATMENT**

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(72) Inventors: **Ammar Al-Ali**, San Juan Capistrano, CA (US); **Massi Joe E. Kiani**, Laguna Niguel, CA (US); **Michael O'Reilly**, Dana Point, CA (US)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 45 days.

(21) Appl. No.: **17/208,734**

(22) Filed: **Mar. 22, 2021**

(65) **Prior Publication Data**

US 2021/0316071 A1 Oct. 14, 2021

Related U.S. Application Data

(63) Continuation of application No. 16/571,591, filed on Sep. 16, 2019, now Pat. No. 10,953,156, which is a (Continued)

(51) **Int. Cl.**
A61M 5/172 (2006.01)
A61B 5/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61M 5/1723** (2013.01); **A61B 5/1455** (2013.01); **A61B 5/14546** (2013.01);
(Continued)

(58) **Field of Classification Search**

CPC .. A61M 5/1723; A61M 1/1603; A61M 1/024; A61B 5/14546; A61B 5/1455;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,567,926 A 9/1951 Dunkelberger
3,103,214 A 9/1963 Smith

(Continued)

FOREIGN PATENT DOCUMENTS

CA 2052650 4/1992
DE 3619442 12/1987

(Continued)

OTHER PUBLICATIONS

US 9,579,050 B2, 02/2017, Al-Ali (withdrawn)

(Continued)

Primary Examiner — Clayton E. LaBalle


Assistant Examiner — Kevin C Butler

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

The present disclosure describes embodiments of a patient monitoring system and methods that include the measure and display of hemoglobin statistics. In an embodiment, total hemoglobin trending is displayed over a period of time. Statistics can include frequency domain analysis, which may be unique for each patient monitored. The total hemoglobin trending and/or statistics can further be used to help control the treatment of a patient, such as being used to control IV administration.

16 Claims, 7 Drawing Sheets

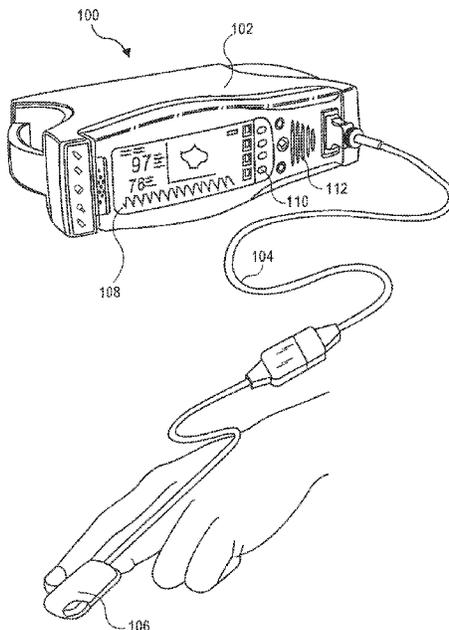

Related U.S. Application Data

continuation of application No. 15/789,357, filed on Oct. 20, 2017, now Pat. No. 10,413,666, which is a continuation of application No. 15/184,950, filed on Jun. 16, 2016, now Pat. No. 9,795,739, which is a continuation of application No. 14/714,691, filed on May 18, 2015, now Pat. No. 9,370,325, which is a continuation of application No. 14/064,026, filed on Oct. 25, 2013, now Pat. No. 9,037,207, which is a continuation of application No. 12/783,436, filed on May 19, 2010, now Pat. No. 8,571,619.

(60) Provisional application No. 61/221,435, filed on Jun. 29, 2009, provisional application No. 61/180,018, filed on May 20, 2009.

(51) **Int. Cl.**

A61B 5/1455 (2006.01)
A61B 5/145 (2006.01)
A61M 1/16 (2006.01)
A61M 1/02 (2006.01)
A61M 37/00 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/14551* (2013.01); *A61B 5/416* (2013.01); *A61B 5/4836* (2013.01); *A61B 5/6826* (2013.01); *A61B 5/7257* (2013.01); *A61B 5/742* (2013.01); *A61M 1/024* (2013.01); *A61M 1/1603* (2014.02); *A61B 5/14532* (2013.01); *A61B 5/14552* (2013.01); *A61M 37/00* (2013.01); *A61M 2230/20* (2013.01)

(58) **Field of Classification Search**

CPC ... *A61B 5/14551*; *A61B 5/416*; *A61B 5/4836*; *A61B 5/6826*; *A61B 5/7257*; *A61B 5/742*
 USPC 600/4.01
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,313,290 A 4/1967 Chance et al.
 3,319,216 A 5/1967 McCullough
 3,463,142 A 8/1969 Harte et al.
 3,482,565 A 12/1969 Gowen
 3,543,310 A 10/1970 Pelissier
 3,647,299 A 3/1972 Lavallee
 3,704,706 A 12/1972 Herczfeld et al.
 3,710,303 A 1/1973 Gallagher, Jr.
 3,711,272 A 1/1973 Randall et al.
 3,740,570 A 6/1973 Kaelin et al.
 3,799,672 A 3/1974 Vurek
 3,802,776 A 4/1974 Tchang
 3,970,353 A 7/1976 Kaufman
 3,995,209 A 11/1976 Weston
 4,051,522 A 9/1977 Healy et al.
 4,086,915 A 5/1978 Kofsky et al.
 4,129,124 A 12/1978 Thalmann
 4,169,976 A 10/1979 Cirri
 4,182,977 A 1/1980 Stricklin, Jr.
 4,216,462 A 8/1980 McGrath et al.
 4,237,344 A 12/1980 Moore
 4,305,401 A 12/1981 Reissmueller et al.
 4,308,456 A 12/1981 Van Der Gaag et al.
 4,321,930 A 3/1982 Jobsis et al.
 4,334,544 A 6/1982 Hill et al.
 4,346,590 A 8/1982 Brown
 4,350,165 A 9/1982 Striese
 4,356,475 A 10/1982 Neumann et al.
 4,380,240 A 4/1983 Jöbsis et al.
 4,406,289 A 9/1983 Wesseling et al.

4,407,290 A 10/1983 Wilber
 4,414,980 A 11/1983 Mott
 4,449,821 A 5/1984 Lee
 4,451,694 A 5/1984 Harper et al.
 4,480,886 A 11/1984 Bergamin
 4,481,804 A 11/1984 Eberhard et al.
 4,490,003 A 12/1984 Robinson
 4,498,722 A 2/1985 Fedder et al.
 4,505,848 A 3/1985 Kobayashi
 4,528,986 A 7/1985 Arundel et al.
 4,531,795 A 7/1985 Sinclair
 4,580,867 A 4/1986 Wright et al.
 4,621,643 A 11/1986 New, Jr. et al.
 4,636,786 A 1/1987 Haertling
 4,642,627 A 2/1987 Hodsdon
 4,648,028 A 3/1987 DeKlotz
 4,653,498 A 3/1987 New, Jr. et al.
 4,674,085 A 6/1987 Aranguren et al.
 4,684,245 A 8/1987 Goldring
 4,684,246 A 8/1987 Downing et al.
 4,685,464 A 8/1987 Goldberger et al.
 4,690,492 A 9/1987 Beard
 4,695,258 A 9/1987 Hanson et al.
 4,700,708 A 10/1987 New, Jr. et al.
 4,770,179 A 9/1988 New, Jr. et al.
 4,797,125 A 1/1989 Malana
 4,815,469 A 3/1989 Cohen et al.
 4,824,242 A 4/1989 Frick et al.
 4,825,872 A 5/1989 Tan et al.
 4,825,879 A 5/1989 Tan et al.
 4,830,014 A 5/1989 Goodman et al.
 4,834,532 A 5/1989 Yount
 4,838,808 A 6/1989 Fujiura
 4,843,013 A 6/1989 Chiang
 4,844,784 A 7/1989 Suzuki et al.
 4,848,901 A 7/1989 Hood, Jr.
 4,858,615 A 8/1989 Meinema
 4,859,057 A 8/1989 Taylor et al.
 4,865,038 A 9/1989 Rich et al.
 4,867,165 A 9/1989 Noller et al.
 4,877,322 A 10/1989 Hill
 4,880,304 A 11/1989 Jaeb et al.
 4,887,260 A 12/1989 Carden et al.
 4,900,904 A 2/1990 Wright et al.
 4,907,594 A 3/1990 Muz
 4,913,150 A 4/1990 Cheung et al.
 4,916,444 A 4/1990 King
 4,920,339 A 4/1990 Friend et al.
 4,927,264 A 5/1990 Shiga
 4,938,218 A 7/1990 Goodman et al.
 4,942,877 A 7/1990 Sakai et al.
 4,952,177 A 8/1990 Drake et al.
 4,960,128 A 10/1990 Gordon et al.
 4,961,711 A 10/1990 Fujiura et al.
 4,964,408 A 10/1990 Hink et al.
 4,974,591 A 12/1990 Awazu et al.
 4,996,975 A 3/1991 Nakamura
 5,007,704 A 4/1991 McCartney
 RE33,643 E 7/1991 Isaacson et al.
 5,031,608 A 7/1991 Weinstein
 5,038,800 A 8/1991 Oba
 5,041,187 A 8/1991 Hink et al.
 5,058,098 A 10/1991 Sakaue et al.
 5,058,588 A 10/1991 Kaestle
 5,061,916 A 10/1991 French et al.
 5,066,859 A 11/1991 Karkar et al.
 5,069,213 A 12/1991 Hink et al.
 5,080,098 A 1/1992 Willett et al.
 5,086,229 A 2/1992 Rosenthal et al.
 5,087,242 A 2/1992 Petelenz et al.
 5,090,410 A 2/1992 Saper et al.
 5,099,842 A 3/1992 Mannheim et al.
 5,108,298 A 4/1992 Simmel
 5,109,848 A 5/1992 Thomas et al.
 5,109,849 A 5/1992 Goodman et al.
 5,113,862 A 5/1992 Mortazavi
 5,125,403 A 6/1992 Culp
 5,126,648 A 6/1992 Jacobs
 5,140,228 A 8/1992 Biegel

(56)

References Cited

U.S. PATENT DOCUMENTS

5,158,323	A	10/1992	Yamamoto et al.	5,588,427	A	12/1996	Tien
5,163,438	A	11/1992	Gordon et al.	5,590,649	A	1/1997	Caro et al.
5,170,786	A	12/1992	Thomas et al.	5,602,924	A	2/1997	Durand et al.
5,188,098	A	2/1993	Hoffman et al.	5,617,857	A	4/1997	Chader et al.
5,193,543	A	3/1993	Yelderman	5,632,272	A	5/1997	Diab et al.
5,209,230	A	5/1993	Swedlow et al.	5,638,816	A	6/1997	Kiani-Azarbayjany et al.
5,217,013	A	6/1993	Lewis et al.	5,638,818	A	6/1997	Diab et al.
5,224,478	A	7/1993	Sakai et al.	5,645,440	A	7/1997	Tobler et al.
5,224,882	A	7/1993	Olms	5,660,567	A	8/1997	Nierlich et al.
5,246,003	A	9/1993	DeLonzor	5,671,914	A	9/1997	Kalkhoran et al.
5,247,931	A	9/1993	Norwood	5,673,693	A	10/1997	Solenberger
5,249,576	A	10/1993	Goldberger et al.	5,678,544	A	10/1997	DeLonzor et al.
5,259,381	A	11/1993	Cheung et al.	5,682,803	A	11/1997	Boianjiu
5,266,792	A	11/1993	Crowne et al.	5,685,299	A	11/1997	Diab et al.
5,267,562	A	12/1993	Ukawa et al.	5,687,734	A	11/1997	Dempsey et al.
5,287,853	A	2/1994	Vester et al.	5,692,503	A	12/1997	Kuenstner
5,295,852	A	3/1994	Renn et al.	5,715,390	A	2/1998	Hoffman
5,295,872	A	3/1994	Christensson	5,720,293	A	2/1998	Quinn et al.
5,297,548	A	3/1994	Pologe	5,726,440	A	3/1998	Kalkhoran et al.
5,302,133	A	4/1994	Tondreault	D393,830	S	4/1998	Tobler et al.
5,308,919	A	5/1994	Minnich	5,742,512	A	4/1998	Edge
5,309,908	A	5/1994	Friedman et al.	5,743,262	A	4/1998	Lepper, Jr. et al.
5,313,940	A	5/1994	Fuse et al.	5,747,806	A	5/1998	Khalil et al.
5,317,269	A	5/1994	Mills et al.	5,748,103	A	5/1998	Flach et al.
5,319,355	A	6/1994	Russek	5,750,994	A	5/1998	Schlager
5,319,363	A	6/1994	Welch et al.	5,758,644	A	6/1998	Diab et al.
5,337,744	A	8/1994	Branigan	5,760,910	A	6/1998	Lepper, Jr. et al.
5,339,810	A	8/1994	Ivers et al.	5,767,791	A	6/1998	Stoop et al.
5,341,805	A	8/1994	Stavridi et al.	5,769,785	A	6/1998	Diab et al.
5,365,937	A	11/1994	Reeves et al.	5,770,028	A	6/1998	Maley et al.
D353,195	S	12/1994	Savage et al.	5,779,630	A	7/1998	Fein et al.
D353,196	S	12/1994	Savage et al.	5,782,757	A	7/1998	Diab et al.
5,377,676	A	1/1995	Vari et al.	5,785,644	A	7/1998	Diab et al.
5,380,213	A	1/1995	Piorunneck et al.	5,785,659	A	7/1998	Caro et al.
5,387,122	A	2/1995	Goldberger et al.	5,790,432	A	8/1998	Morys
5,390,670	A	2/1995	Centa et al.	5,791,347	A	8/1998	Flaherty et al.
5,397,247	A	3/1995	Aoki et al.	5,803,909	A	9/1998	Maki et al.
5,400,267	A	3/1995	Denen et al.	5,807,247	A	9/1998	Mechant et al.
5,407,368	A	4/1995	Strand et al.	5,807,248	A	9/1998	Mills
5,415,629	A	5/1995	Henley	5,810,724	A	9/1998	Gronvall
D359,546	S	6/1995	Savage et al.	5,810,734	A	9/1998	Caro et al.
5,422,632	A	6/1995	Bucholtz et al.	5,817,010	A	10/1998	Hibl
5,425,375	A	6/1995	Chin et al.	5,818,985	A	10/1998	Merchant et al.
5,431,170	A	7/1995	Mathews	5,823,950	A	10/1998	Diab et al.
5,436,499	A	7/1995	Namavar et al.	5,830,129	A	11/1998	Baer et al.
D361,840	S	8/1995	Savage et al.	5,830,131	A	11/1998	Caro et al.
5,438,986	A	8/1995	Disch et al.	5,833,618	A	11/1998	Caro et al.
D362,063	S	9/1995	Savage et al.	5,841,435	A	11/1998	Dauerer et al.
5,452,717	A	9/1995	Branigan et al.	5,860,919	A	1/1999	Kiani-Azarbayjany et al.
D363,120	S	10/1995	Savage et al.	5,890,929	A	4/1999	Mills et al.
5,456,252	A	10/1995	Vari et al.	5,895,369	A	4/1999	Flower
5,460,182	A	10/1995	Goodman et al.	5,904,654	A	5/1999	Wohlmann et al.
5,469,845	A	11/1995	DeLonzor et al.	5,919,133	A	7/1999	Taylor et al.
5,479,934	A	1/1996	Imran	5,919,134	A	7/1999	Diab
5,482,036	A	1/1996	Diab et al.	5,934,925	A	8/1999	Tobler et al.
5,490,505	A	2/1996	Diab et al.	5,939,609	A	8/1999	Knapp et al.
5,490,523	A	2/1996	Isaacson et al.	5,940,182	A	8/1999	Lepper, Jr. et al.
5,494,043	A	2/1996	O'Sullivan et al.	5,957,885	A	9/1999	Bollish et al.
5,498,235	A	3/1996	Flower	5,970,353	A	10/1999	Sultan
5,509,823	A	4/1996	Harting et al.	5,987,343	A	11/1999	Kinast
5,515,169	A	5/1996	Cargill et al.	5,991,355	A	11/1999	Dahlke
5,520,177	A	5/1996	Ogawa et al.	5,995,855	A	11/1999	Kiani et al.
5,521,997	A	5/1996	Rovenolt et al.	5,997,343	A	12/1999	Mills et al.
5,533,509	A	7/1996	Koashi et al.	5,999,834	A	12/1999	Wang et al.
5,533,511	A	7/1996	Kaspari et al.	6,002,952	A	12/1999	Diab et al.
5,534,851	A	7/1996	Russek	6,010,937	A	1/2000	Karam et al.
5,561,275	A	10/1996	Savage et al.	6,011,985	A	1/2000	Athan et al.
5,564,108	A	10/1996	Hunsaker et al.	6,011,986	A	1/2000	Diab et al.
5,564,417	A	10/1996	Chance	6,014,576	A	1/2000	Raley
5,569,823	A	10/1996	Schreier et al.	6,027,452	A	2/2000	Flaherty et al.
5,570,002	A	10/1996	Castleman	6,036,642	A	3/2000	Diab et al.
5,575,284	A	11/1996	Athan et al.	6,040,578	A	3/2000	Malin et al.
5,579,001	A	11/1996	Dempsey et al.	6,045,509	A	4/2000	Caro et al.
5,579,775	A	12/1996	Dempsey et al.	6,061,584	A	5/2000	Lovejoy
5,584,296	A	12/1996	Cui et al.	6,066,204	A	5/2000	Haven
				6,067,462	A	5/2000	Diab et al.
				6,074,345	A	6/2000	Van Oostrom et al.
				6,081,735	A	6/2000	Diab et al.
				6,088,607	A	7/2000	Diab et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,110,522	A	8/2000	Lepper, Jr. et al.	6,597,932	B2	7/2003	Tian et al.
6,115,673	A	9/2000	Malin et al.	6,597,933	B2	7/2003	Kiani et al.
6,124,597	A	9/2000	Shehada et al.	6,600,940	B1	7/2003	Fien et al.
6,128,521	A	10/2000	Marro et al.	6,606,511	B1	8/2003	Ali et al.
6,129,675	A	10/2000	Jay	6,611,320	B1	8/2003	Lindberg et al.
6,144,868	A	11/2000	Parker	6,632,181	B2	10/2003	Flaherty et al.
6,151,516	A	11/2000	Kiani-Azarbayjany et al.	6,635,559	B2	10/2003	Greenwald et al.
6,152,754	A	11/2000	Gerhardt et al.	6,639,668	B1	10/2003	Trepagnier
6,157,850	A	12/2000	Diab et al.	6,640,116	B2	10/2003	Diab
6,165,005	A	12/2000	Mills et al.	6,640,117	B2	10/2003	Makarewicz et al.
6,174,283	B1	1/2001	Nevo	6,643,530	B2	11/2003	Diab et al.
6,184,521	B1	2/2001	Coffin, IV et al.	6,650,917	B2	11/2003	Diab et al.
6,206,830	B1	3/2001	Diab et al.	6,654,624	B2	11/2003	Diab et al.
6,223,064	B1*	4/2001	Lynn A61B 5/14551 600/324	6,658,276	B2	12/2003	Kiani et al.
6,229,856	B1	5/2001	Diab et al.	6,661,161	B1	12/2003	Lanzo et al.
6,232,609	B1	5/2001	Snyder et al.	6,671,531	B2	12/2003	Al-Ali
6,236,872	B1	5/2001	Diab et al.	6,678,543	B2	1/2004	Diab et al.
6,241,683	B1	6/2001	Macklem et al.	6,684,090	B2	1/2004	Ali et al.
6,255,708	B1	7/2001	Sudharsanan et al.	6,684,091	B2	1/2004	Parker
6,256,523	B1	7/2001	Diab et al.	6,697,656	B1	2/2004	Al-Ali
6,263,222	B1	7/2001	Diab et al.	6,697,657	B1	2/2004	Shehada et al.
6,268,283	B1	7/2001	Huang et al.	6,697,658	B2	2/2004	Al-Ali
6,275,717	B1	8/2001	Gross et al.	RE38,476	E	3/2004	Diab et al.
6,278,522	B1	8/2001	Lepper, Jr. et al.	6,699,194	B1	3/2004	Diab et al.
6,280,213	B1	8/2001	Tobler et al.	6,714,804	B2	3/2004	Al-Ali et al.
6,280,381	B1	8/2001	Malin et al.	RE38,492	E	4/2004	Diab et al.
6,282,438	B1	8/2001	Maki et al.	6,721,582	B2	4/2004	Trepagnier et al.
6,285,896	B1	9/2001	Tobler et al.	6,721,585	B1	4/2004	Parker
6,301,493	B1	10/2001	Marro et al.	6,725,075	B2	4/2004	Al-Ali
6,308,089	B1	10/2001	von der Ruhr et al.	6,728,560	B2	4/2004	Kollias et al.
6,317,627	B1	11/2001	Ennen et al.	6,728,561	B2	4/2004	Smith et al.
6,321,100	B1	11/2001	Parker	6,735,459	B2	5/2004	Parker
6,325,761	B1	12/2001	Jay	6,738,652	B2	5/2004	Mattu et al.
6,330,468	B1	12/2001	Scharf	6,745,060	B2	6/2004	Diab et al.
6,334,065	B1	12/2001	Al-Ali et al.	6,760,607	B2	7/2004	Al-Ali
6,343,224	B1	1/2002	Parker	6,763,256	B2	7/2004	Kimball et al.
6,349,228	B1	2/2002	Kiani et al.	6,770,028	B1	8/2004	Ali et al.
6,360,114	B1	3/2002	Diab et al.	6,771,994	B2	8/2004	Kiani et al.
6,368,283	B1	4/2002	Xu et al.	6,788,965	B2	9/2004	Ruchti et al.
6,371,921	B1	4/2002	Caro et al.	6,790,178	B1	9/2004	Mault et al.
6,377,829	B1	4/2002	Al-Ali	6,792,300	B1	9/2004	Diab et al.
6,388,240	B2	5/2002	Schulz et al.	6,813,511	B2	11/2004	Diab et al.
6,397,091	B2	5/2002	Diab et al.	6,816,241	B2	11/2004	Grubisic
6,411,373	B1	6/2002	Garside et al.	6,816,741	B2	11/2004	Diab
6,415,167	B1	7/2002	Blank et al.	6,822,564	B2	11/2004	Al-Ali
6,430,437	B1	8/2002	Marro	6,826,419	B2	11/2004	Diab et al.
6,430,525	B1	8/2002	Weber et al.	6,830,711	B2	12/2004	Mills et al.
6,433,696	B1	8/2002	Deiterman et al.	6,850,787	B2	2/2005	Weber et al.
6,440,067	B1	8/2002	DeLuca et al.	6,850,788	B2	2/2005	Al-Ali
6,463,142	B1	10/2002	Kilp	6,852,083	B2	2/2005	Caro et al.
6,463,311	B1	10/2002	Diab	6,861,639	B2	3/2005	Al-Ali
6,470,199	B1	10/2002	Kopotic et al.	6,876,931	B2	4/2005	Lorenz et al.
6,473,632	B1	10/2002	Myers	6,879,850	B2	4/2005	Kimball
6,487,429	B2	11/2002	Hockersmith et al.	6,898,452	B2	5/2005	Al-Ali et al.
6,496,711	B1	12/2002	Athan et al.	6,920,345	B2	7/2005	Al-Ali et al.
6,501,975	B2	12/2002	Diab et al.	6,928,370	B2	8/2005	Anuzis et al.
6,505,059	B1	1/2003	Kollias et al.	6,931,268	B1	8/2005	Kiani-Azarbayjany et al.
6,515,273	B2	2/2003	Al-Ali	6,934,570	B2	8/2005	Kiani et al.
6,519,487	B1	2/2003	Parker	6,939,305	B2	9/2005	Flaherty et al.
6,525,386	B1	2/2003	Mills et al.	6,943,348	B1	9/2005	Coffin IV
6,526,300	B1	2/2003	Kiani et al.	6,950,687	B2	9/2005	Al-Ali
6,534,012	B1	3/2003	Hazen et al.	6,956,649	B2	10/2005	Acosta et al.
6,541,756	B2	4/2003	Schulz et al.	6,961,598	B2	11/2005	Diab
6,542,764	B1	4/2003	Al-Ali et al.	6,970,792	B1	11/2005	Diab
6,544,173	B2	4/2003	West et al.	6,979,812	B2	12/2005	Al-Ali
6,544,174	B2	4/2003	West et al.	6,985,763	B2	1/2006	Boas et al.
6,553,241	B2	4/2003	Mannheimer et al.	6,985,764	B2	1/2006	Mason et al.
6,558,276	B1	5/2003	Yokota et al.	6,990,364	B2	1/2006	Ruchti et al.
6,571,113	B1	5/2003	Fein et al.	6,993,371	B2	1/2006	Kiani et al.
6,580,086	B1	6/2003	Schulz et al.	6,996,427	B2	2/2006	Ali et al.
6,584,336	B1	6/2003	Ali et al.	6,997,879	B1	2/2006	Turcott
6,587,196	B1	7/2003	Stippick et al.	6,998,247	B2	2/2006	Monfre et al.
6,587,199	B1	7/2003	Luu	6,999,904	B2	2/2006	Weber et al.
6,595,316	B2	7/2003	Cybulski et al.	7,003,338	B2	2/2006	Weber et al.
				7,003,339	B2	2/2006	Diab et al.
				7,015,451	B2	3/2006	Dalke et al.
				7,024,233	B2	4/2006	Ali et al.
				7,027,849	B2	4/2006	Al-Ali
				7,030,749	B2	4/2006	Al-Ali

(56)

References Cited

U.S. PATENT DOCUMENTS

7,039,449	B2	5/2006	Al-Ali	7,509,154	B2	3/2009	Diab et al.
7,041,060	B2	5/2006	Flaherty et al.	7,509,494	B2	3/2009	Al-Ali
7,044,918	B2	5/2006	Diab	7,510,849	B2	3/2009	Schurman et al.
7,048,687	B1	5/2006	Reuss et al.	7,514,725	B2	4/2009	Wojtczuk et al.
7,067,893	B2	6/2006	Mills et al.	7,519,406	B2	4/2009	Blank et al.
D526,719	S	8/2006	Richie, Jr. et al.	7,526,328	B2	4/2009	Diab et al.
7,096,052	B2	8/2006	Mason et al.	D592,507	S	5/2009	Wachman et al.
7,096,054	B2	8/2006	Abdul-Hafiz et al.	7,530,942	B1	5/2009	Diab
D529,616	S	10/2006	Deros et al.	7,530,949	B2	5/2009	Al Ali et al.
7,132,641	B2	11/2006	Schulz et al.	7,530,955	B2	5/2009	Diab et al.
7,133,710	B2	11/2006	Acosta et al.	7,532,919	B2	5/2009	Soyemi et al.
7,142,901	B2	11/2006	Kiani et al.	7,563,110	B2	7/2009	Al-Ali et al.
7,142,902	B2	11/2006	Eda et al.	7,593,230	B2	9/2009	Abul-Haj et al.
7,149,561	B2	12/2006	Diab	7,596,398	B2	9/2009	Al-Ali et al.
7,186,966	B2	3/2007	Al-Ali	7,606,608	B2	10/2009	Blank et al.
7,190,261	B2	3/2007	Al-Ali	7,618,375	B2	11/2009	Flaherty et al.
7,215,984	B2	5/2007	Diab et al.	7,620,674	B2	11/2009	Ruchti et al.
7,215,986	B2	5/2007	Diab et al.	D606,659	S	12/2009	Kiani et al.
7,216,108	B2	5/2007	Hastings	7,629,039	B2	12/2009	Eckerbom et al.
7,221,971	B2	5/2007	Diab et al.	7,640,140	B2	12/2009	Ruchti et al.
7,225,006	B2	5/2007	Al-Ali et al.	7,647,083	B2	1/2010	Al-Ali et al.
7,225,007	B2	5/2007	Al-Ali et al.	D609,193	S	2/2010	Al-Ali et al.
RE39,672	E	6/2007	Shehada et al.	7,660,616	B1	2/2010	Poore
7,239,905	B2	7/2007	Kiani-Azarbayjany et al.	D614,305	S	4/2010	Al-Ali et al.
7,241,270	B2	7/2007	Horzewski et al.	7,697,966	B2	4/2010	Monfre et al.
7,245,953	B1	7/2007	Parker	7,698,105	B2	4/2010	Ruchti et al.
7,248,910	B2	7/2007	Li et al.	RE41,317	E	5/2010	Parker
7,254,429	B2	8/2007	Schurman et al.	RE41,333	E	5/2010	Blank et al.
7,254,431	B2	8/2007	Al-Ali et al.	7,725,007	B2	5/2010	Moon et al.
7,254,433	B2	8/2007	Diab et al.	7,729,733	B2	6/2010	Al-Ali et al.
7,254,434	B2	8/2007	Schulz et al.	7,734,320	B2	6/2010	Al-Ali
7,272,425	B2	9/2007	Al-Ali	7,761,127	B2	7/2010	Al-Ali et al.
7,274,955	B2	9/2007	Kiani et al.	7,761,128	B2	7/2010	Al-Ali et al.
D554,263	S	10/2007	Al-Ali et al.	7,764,982	B2	7/2010	Dalke et al.
7,280,858	B2	10/2007	Al-Ali et al.	D621,516	S	8/2010	Kiani et al.
7,289,835	B2	10/2007	Mansfield et al.	7,791,155	B2	9/2010	Diab
7,292,883	B2	11/2007	De Felice et al.	7,801,581	B2	9/2010	Diab
7,295,866	B2	11/2007	Al-Ali	7,822,452	B2	10/2010	Schurman et al.
7,319,894	B2	1/2008	Higgins	RE41,912	E	11/2010	Parker
7,328,053	B1	2/2008	Diab et al.	7,844,313	B2	11/2010	Kiani et al.
7,332,784	B2	2/2008	Mills et al.	7,844,314	B2	11/2010	Al-Ali
7,340,287	B2	3/2008	Mason et al.	7,844,315	B2	11/2010	Al-Ali
7,341,559	B2	3/2008	Schulz et al.	7,848,798	B2	12/2010	Martinsen et al.
7,343,186	B2	3/2008	Lamego et al.	7,865,222	B2	1/2011	Weber et al.
D566,282	S	4/2008	Al-Ali et al.	7,873,497	B2	1/2011	Weber et al.
7,355,512	B1	4/2008	Al-Ali	7,880,606	B2	2/2011	Al-Ali
7,356,365	B2	4/2008	Schurman	7,880,626	B2	2/2011	Al-Ali et al.
7,371,981	B2	5/2008	Abdul-Hafiz	7,891,355	B2	2/2011	Al-Ali et al.
7,373,193	B2	5/2008	Al-Ali et al.	7,894,868	B2	2/2011	Al-Ali et al.
7,373,194	B2	5/2008	Weber et al.	7,899,507	B2	3/2011	Al-Ali et al.
7,376,453	B1	5/2008	Diab et al.	7,904,132	B2	3/2011	Weber et al.
7,377,794	B2	5/2008	Al-Ali et al.	7,909,772	B2	3/2011	Popov et al.
7,377,899	B2	5/2008	Weber et al.	7,910,875	B2	3/2011	Al-Ali
7,383,070	B2	6/2008	Diab et al.	7,919,713	B2	4/2011	Al-Ali et al.
7,395,158	B2	7/2008	Monfre et al.	7,937,128	B2	5/2011	Al-Ali
7,415,297	B2	8/2008	Al-Ali et al.	7,937,129	B2	5/2011	Mason et al.
7,426,407	B2	9/2008	Higgins	7,937,130	B2	5/2011	Diab et al.
7,428,432	B2	9/2008	Ali et al.	7,941,199	B2	5/2011	Kiani
7,438,683	B2	10/2008	Al-Ali et al.	7,949,380	B2	5/2011	Fein et al.
7,440,787	B2	10/2008	Diab	7,951,086	B2	5/2011	Flaherty et al.
7,454,240	B2	11/2008	Diab et al.	7,957,780	B2	6/2011	Lamego et al.
7,467,002	B2	12/2008	Weber et al.	7,962,188	B2	6/2011	Kiani et al.
7,469,157	B2	12/2008	Diab et al.	7,962,190	B1	6/2011	Diab et al.
7,471,969	B2	12/2008	Diab et al.	7,976,472	B2	7/2011	Kiani
7,471,971	B2	12/2008	Diab et al.	7,988,637	B2	8/2011	Diab
7,483,729	B2	1/2009	Al-Ali et al.	7,990,382	B2	8/2011	Kiani
7,483,730	B2	1/2009	Diab et al.	7,991,446	B2	8/2011	Ali et al.
7,483,731	B2	1/2009	Hoarau et al.	8,000,761	B2	8/2011	Al-Ali
7,489,958	B2	2/2009	Diab et al.	8,008,088	B2	8/2011	Bellott et al.
7,496,391	B2	2/2009	Diab et al.	RE42,753	E	9/2011	Kiani-Azarbayjany et al.
7,496,393	B2	2/2009	Diab et al.	8,019,400	B2	9/2011	Diab et al.
D587,657	S	3/2009	Al-Ali et al.	8,028,701	B2	10/2011	Al-Ali et al.
7,499,741	B2	3/2009	Diab et al.	8,029,765	B2	10/2011	Bellott et al.
7,499,835	B2	3/2009	Weber et al.	8,036,727	B2	10/2011	Schurman et al.
7,500,950	B2	3/2009	Al-Ali et al.	8,036,728	B2	10/2011	Diab et al.
				8,046,040	B2	10/2011	Ali et al.
				8,046,041	B2	10/2011	Diab et al.
				8,046,042	B2	10/2011	Diab et al.
				8,048,040	B2	11/2011	Kiani

(56)

References Cited

U.S. PATENT DOCUMENTS

8,050,728 B2	11/2011	Al-Ali et al.	8,548,548 B2	10/2013	Al-Ali
RE43,169 E	2/2012	Parker	8,548,549 B2	10/2013	Schurman et al.
8,118,620 B2	2/2012	Al-Ali et al.	8,548,550 B2	10/2013	Al-Ali et al.
8,126,528 B2	2/2012	Diab et al.	8,560,032 B2	10/2013	Al-Ali et al.
8,128,572 B2	3/2012	Diab et al.	8,560,034 B1	10/2013	Diab et al.
8,130,105 B2	3/2012	Al-Ali et al.	8,570,167 B2	10/2013	Al-Ali
8,145,287 B2	3/2012	Diab et al.	8,570,503 B2	10/2013	Vo et al.
8,150,487 B2	4/2012	Diab et al.	8,571,617 B2	10/2013	Reichgott et al.
8,175,672 B2	5/2012	Parker	8,571,618 B1	10/2013	Lamego et al.
8,180,420 B2	5/2012	Diab et al.	8,571,619 B2	10/2013	Al-Ali et al.
8,182,443 B1	5/2012	Kiani	8,577,431 B2	11/2013	Lamego et al.
8,185,180 B2	5/2012	Diab et al.	8,581,732 B2	11/2013	Al-Ali et al.
8,190,223 B2	5/2012	Al-Ali et al.	8,584,345 B2	11/2013	Al-Ali et al.
8,190,227 B2	5/2012	Diab et al.	8,588,880 B2	11/2013	Abdul-Hafiz et al.
8,203,438 B2	6/2012	Kiani et al.	8,600,467 B2	12/2013	Al-Ali et al.
8,203,704 B2	6/2012	Merritt et al.	8,606,342 B2	12/2013	Diab
8,204,566 B2	6/2012	Schurman et al.	8,626,255 B2	1/2014	Al-Ali et al.
8,219,172 B2	7/2012	Schurman et al.	8,630,691 B2	1/2014	Lamego et al.
8,224,411 B2	7/2012	Al-Ali et al.	8,634,889 B2	1/2014	Al-Ali et al.
8,228,181 B2	7/2012	Al-Ali	8,641,631 B2	2/2014	Sierra et al.
8,229,532 B2	7/2012	Davis	8,652,060 B2	2/2014	Al-Ali
8,229,533 B2	7/2012	Diab et al.	8,663,107 B2	3/2014	Kiani
8,233,955 B2	7/2012	Al-Ali et al.	8,666,468 B1	3/2014	Al-Ali
8,244,325 B2	8/2012	Al-Ali et al.	8,667,967 B2	3/2014	Al-Ali et al.
8,255,026 B1	8/2012	Al-Ali	8,670,811 B2	3/2014	O'Reilly
8,255,027 B2	8/2012	Al-Ali et al.	8,670,814 B2	3/2014	Diab et al.
8,255,028 B2	8/2012	Al-Ali et al.	8,676,286 B2	3/2014	Weber et al.
8,260,577 B2	9/2012	Weber et al.	8,682,407 B2	3/2014	Al-Ali
8,265,723 B1	9/2012	McHale et al.	RE44,823 E	4/2014	Parker
8,274,360 B2	9/2012	Sampath et al.	RE44,875 E	4/2014	Kiani et al.
8,280,473 B2	10/2012	Al-Ali	8,688,183 B2	4/2014	Bruinsma et al.
8,301,217 B2	10/2012	Al-Ali et al.	8,690,799 B2	4/2014	Telfort et al.
8,306,596 B2	11/2012	Schurman et al.	8,700,112 B2	4/2014	Kiani
8,310,336 B2	11/2012	Muhsin et al.	8,702,627 B2	4/2014	Telfort et al.
8,315,683 B2	11/2012	Al-Ali et al.	8,706,179 B2	4/2014	Parker
RE43,860 E	12/2012	Parker	8,712,494 B1	4/2014	MacNeish, III et al.
8,337,403 B2	12/2012	Al-Ali et al.	8,715,206 B2	5/2014	Telfort et al.
8,346,330 B2	1/2013	Lamego	8,718,735 B2	5/2014	Lamego et al.
8,353,842 B2	1/2013	Al-Ali et al.	8,718,737 B2	5/2014	Diab et al.
8,355,766 B2	1/2013	MacNeish, III et al.	8,718,738 B2	5/2014	Blank et al.
8,359,080 B2	1/2013	Diab et al.	8,720,249 B2	5/2014	Al-Ali
8,364,223 B2	1/2013	Al-Ali et al.	8,721,541 B2	5/2014	Al-Ali et al.
8,364,226 B2	1/2013	Diab et al.	8,721,542 B2	5/2014	Al-Ali et al.
8,374,665 B2	2/2013	Lamego	8,723,677 B1	5/2014	Kiani
8,385,995 B2	2/2013	Al-Ali et al.	8,740,792 B1	6/2014	Kiani et al.
8,385,996 B2	2/2013	Smith et al.	8,754,776 B2	6/2014	Poeze et al.
8,388,353 B2	3/2013	Kiani et al.	8,755,535 B2	6/2014	Telfort et al.
8,399,822 B2	3/2013	Al-Ali	8,755,856 B2	6/2014	Diab et al.
8,401,602 B2	3/2013	Kiani	8,755,872 B1	6/2014	Marinow
8,405,608 B2	3/2013	Al-Ali et al.	8,761,850 B2	6/2014	Lamego
8,414,499 B2	4/2013	Al-Ali et al.	8,764,671 B2	7/2014	Kiani
8,418,524 B2	4/2013	Al-Ali	8,768,423 B2	7/2014	Shakespeare et al.
8,423,106 B2	4/2013	Lamego et al.	8,771,204 B2	7/2014	Telfort et al.
8,428,967 B2	4/2013	Olsen et al.	8,777,634 B2	7/2014	Kiani et al.
8,430,817 B1	4/2013	Al-Ali et al.	8,781,543 B2	7/2014	Diab et al.
8,437,825 B2	5/2013	Dalvi et al.	8,781,544 B2	7/2014	Al-Ali et al.
8,455,290 B2	6/2013	Siskavich	8,781,549 B2	7/2014	Al-Ali et al.
8,457,703 B2	6/2013	Al-Ali	8,788,003 B2	7/2014	Schurman et al.
8,457,707 B2	6/2013	Kiani	8,790,268 B2	7/2014	Al-Ali
8,463,349 B2	6/2013	Diab et al.	8,801,613 B2	8/2014	Al-Ali et al.
8,466,286 B2	6/2013	Bellott et al.	8,821,397 B2	9/2014	Al-Ali et al.
8,471,713 B2	6/2013	Poeze et al.	8,821,415 B2	9/2014	Al-Ali et al.
8,473,020 B2	6/2013	Kiani et al.	8,830,449 B1	9/2014	Lamego et al.
8,483,787 B2	7/2013	Al-Ali et al.	8,831,700 B2	9/2014	Schurman et al.
8,489,364 B2	7/2013	Weber et al.	8,840,549 B2	9/2014	Al-Ali et al.
8,498,684 B2	7/2013	Weber et al.	8,847,740 B2	9/2014	Kiani et al.
8,504,128 B2	8/2013	Blank et al.	8,849,365 B2	9/2014	Smith et al.
8,509,867 B2	8/2013	Workman et al.	8,852,094 B2	10/2014	Al-Ali et al.
8,515,509 B2	8/2013	Bruinsma et al.	8,852,994 B2	10/2014	Wojtczuk et al.
8,523,781 B2	9/2013	Al-Ali	8,868,147 B2	10/2014	Stippick et al.
8,529,301 B2	9/2013	Al-Ali et al.	8,868,150 B2	10/2014	Al-Ali et al.
8,532,727 B2	9/2013	Ali et al.	8,870,792 B2	10/2014	Al-Ali et al.
8,532,728 B2	9/2013	Diab et al.	8,886,271 B2	11/2014	Kiani et al.
D692,145 S	10/2013	Al-Ali et al.	8,888,539 B2	11/2014	Al-Ali et al.
8,547,209 B2	10/2013	Kiani et al.	8,888,708 B2	11/2014	Diab et al.
			8,892,180 B2	11/2014	Weber et al.
			8,897,847 B2	11/2014	Al-Ali
			8,909,310 B2	12/2014	Lamego et al.
			8,911,377 B2	12/2014	Al-Ali

(56)

References Cited

U.S. PATENT DOCUMENTS

8,912,909 B2	12/2014	Al-Ali et al.	9,392,945 B2	7/2016	Al-Ali et al.
8,920,317 B2	12/2014	Al-Ali et al.	9,397,448 B2	7/2016	Al-Ali et al.
8,921,699 B2	12/2014	Al-Ali et al.	9,408,542 B1	8/2016	Kinast et al.
8,922,382 B2	12/2014	Al-Ali et al.	9,436,645 B2	9/2016	Al-Ali et al.
8,929,964 B2	1/2015	Al-Ali et al.	9,445,759 B1	9/2016	Lamego et al.
8,942,777 B2	1/2015	Diab et al.	9,466,919 B2	10/2016	Kiani et al.
8,948,834 B2	2/2015	Diab et al.	9,474,474 B2	10/2016	Lamego et al.
8,948,835 B2	2/2015	Diab	9,480,422 B2	11/2016	Al-Ali
8,965,471 B2	2/2015	Lamego	9,480,435 B2	11/2016	Olsen
8,983,564 B2	3/2015	Al-Ali	9,492,110 B2	11/2016	Al-Ali et al.
8,989,831 B2	3/2015	Al-Ali et al.	9,510,779 B2	12/2016	Poeze et al.
8,996,085 B2	3/2015	Kiani et al.	9,517,024 B2	12/2016	Kiani et al.
8,998,809 B2	4/2015	Kiani	9,532,722 B2	1/2017	Lamego et al.
9,028,429 B2	5/2015	Telfort et al.	9,538,949 B2	1/2017	Al-Ali et al.
9,037,207 B2	5/2015	Al-Ali et al.	9,538,980 B2	1/2017	Telfort et al.
9,060,721 B2	6/2015	Reichgott et al.	9,549,696 B2	1/2017	Lamego et al.
9,066,666 B2	6/2015	Kiani	9,554,737 B2	1/2017	Schurman et al.
9,066,680 B1	6/2015	Al-Ali et al.	9,560,996 B2	2/2017	Kiani
9,072,474 B2	7/2015	Al-Ali et al.	9,560,998 B2	2/2017	Al-Ali et al.
9,078,560 B2	7/2015	Schurman et al.	9,566,019 B2	2/2017	Al-Ali et al.
9,084,569 B2	7/2015	Weber et al.	9,579,039 B2	2/2017	Jansen et al.
9,095,316 B2	8/2015	Welch et al.	9,591,975 B2	3/2017	Dalvi et al.
9,106,038 B2	8/2015	Telfort et al.	9,622,692 B2	4/2017	Lamego et al.
9,107,625 B2	8/2015	Telfort et al.	9,622,693 B2	4/2017	Diab
9,107,626 B2	8/2015	Al-Ali et al.	D788,312 S	5/2017	Al-Ali et al.
9,113,831 B2	8/2015	Al-Ali	9,636,055 B2	5/2017	Al-Ali et al.
9,113,832 B2	8/2015	Al-Ali	9,636,056 B2	5/2017	Al-Ali
9,119,595 B2	9/2015	Lamego	9,649,054 B2	5/2017	Lamego et al.
9,131,881 B2	9/2015	Diab et al.	9,662,052 B2	5/2017	Al-Ali et al.
9,131,882 B2	9/2015	Al-Ali et al.	9,668,679 B2	6/2017	Schurman et al.
9,131,883 B2	9/2015	Al-Ali	9,668,680 B2	6/2017	Bruinsma et al.
9,131,917 B2	9/2015	Telfort et al.	9,668,703 B2	6/2017	Al-Ali
9,138,180 B1	9/2015	Coverston et al.	9,675,286 B2	6/2017	Diab
9,138,182 B2	9/2015	Al-Ali et al.	9,687,160 B2	6/2017	Kiani
9,138,192 B2	9/2015	Weber et al.	9,693,719 B2	7/2017	Al-Ali et al.
9,142,117 B2	9/2015	Muhsin et al.	9,693,737 B2	7/2017	Al-Ali
9,153,112 B1	10/2015	Kiani et al.	9,697,928 B2	7/2017	Al-Ali et al.
9,153,121 B2	10/2015	Kiani et al.	9,717,425 B2	8/2017	Kiani et al.
9,161,696 B2	10/2015	Al-Ali et al.	9,717,458 B2	8/2017	Lamego et al.
9,161,713 B2	10/2015	Al-Ali et al.	9,724,016 B1	8/2017	Al-Ali et al.
9,167,995 B2	10/2015	Lamego et al.	9,724,024 B2	8/2017	Al-Ali
9,176,141 B2	11/2015	Al-Ali et al.	9,724,025 B1	8/2017	Kiani et al.
9,186,102 B2	11/2015	Bruinsma et al.	9,730,640 B2	8/2017	Diab et al.
9,192,312 B2	11/2015	Al-Ali	9,743,887 B2	8/2017	Al-Ali et al.
9,192,329 B2	11/2015	Al-Ali	9,749,232 B2	8/2017	Sampath et al.
9,192,351 B1	11/2015	Telfort et al.	9,750,442 B2	9/2017	Olsen
9,195,385 B2	11/2015	Al-Ali et al.	9,750,443 B2	9/2017	Smith et al.
9,211,072 B2	12/2015	Kiani	9,750,461 B1	9/2017	Telfort
9,211,095 B1	12/2015	Al-Ali	9,775,545 B2	10/2017	Al-Ali et al.
9,218,454 B2	12/2015	Kiani et al.	9,775,546 B2	10/2017	Diab et al.
9,226,696 B2	1/2016	Kiani	9,775,570 B2	10/2017	Al-Ali
9,241,662 B2	1/2016	Al-Ali et al.	9,778,079 B1	10/2017	Al-Ali et al.
9,245,668 B1	1/2016	Vo et al.	9,782,077 B2	10/2017	Lamego et al.
9,259,185 B2	2/2016	Abdul-Hafiz et al.	9,782,110 B2	10/2017	Kiani
9,267,572 B2	2/2016	Barker et al.	9,787,568 B2	10/2017	Lamego et al.
9,277,880 B2	3/2016	Poeze et al.	9,788,735 B2	10/2017	Al-Ali
9,289,167 B2	3/2016	Diab et al.	9,788,768 B2	10/2017	Al-Ali et al.
9,295,421 B2	3/2016	Kiani et al.	9,795,300 B2	10/2017	Al-Ali
9,307,928 B1	4/2016	Al-Ali et al.	9,795,310 B2	10/2017	Al-Ali
9,323,894 B2	4/2016	Kiani	9,795,358 B2	10/2017	Telfort et al.
D755,392 S	5/2016	Hwang et al.	9,795,739 B2	10/2017	Al-Ali et al.
9,326,712 B1	5/2016	Kiani	9,801,556 B2	10/2017	Kiani
9,333,316 B2	5/2016	Kiani	9,801,588 B2	10/2017	Weber et al.
9,339,220 B2	5/2016	Lamego et al.	9,808,188 B1	11/2017	Perea et al.
9,341,565 B2	5/2016	Lamego et al.	9,814,418 B2	11/2017	Weber et al.
9,351,673 B2	5/2016	Diab et al.	9,820,691 B2	11/2017	Kiani
9,351,675 B2	5/2016	Al-Ali et al.	9,833,152 B2	12/2017	Kiani et al.
9,364,181 B2	6/2016	Kiani et al.	9,833,180 B2	12/2017	Shakespeare et al.
9,368,671 B2	6/2016	Wojtczuk et al.	9,839,379 B2	12/2017	Al-Ali et al.
9,370,325 B2	6/2016	Al-Ali et al.	9,839,381 B1	12/2017	Weber et al.
9,370,326 B2	6/2016	McHale et al.	9,847,002 B2	12/2017	Kiani et al.
9,370,335 B2	6/2016	Al-Ali et al.	9,847,749 B2	12/2017	Kiani et al.
9,375,185 B2	6/2016	Ali et al.	9,848,800 B1	12/2017	Lee et al.
9,386,953 B2	7/2016	Al-Ali	9,848,806 B2	12/2017	Al-Ali
9,386,961 B2	7/2016	Al-Ali et al.	9,848,807 B2	12/2017	Lamego
			9,861,298 B2	1/2018	Eckerbom et al.
			9,861,304 B2	1/2018	Al-Ali et al.
			9,861,305 B1	1/2018	Weber et al.
			9,867,578 B2	1/2018	Al-Ali et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,872,623 B2	1/2018	Al-Ali	10,456,038 B2	10/2019	Lamego et al.
9,876,320 B2	1/2018	Coverston et al.	10,463,340 B2	11/2019	Telfort et al.
9,877,650 B2	1/2018	Muhsin et al.	10,471,159 B1	11/2019	Lapotko et al.
9,877,686 B2	1/2018	Al-Ali et al.	10,505,311 B2	12/2019	Al-Ali et al.
9,891,079 B2	2/2018	Dalvi	10,524,738 B2	1/2020	Olsen
9,895,107 B2	2/2018	Al-Ali et al.	10,532,174 B2	1/2020	Al-Ali
9,913,617 B2	3/2018	Al-Ali et al.	10,537,285 B2	1/2020	Shreim et al.
9,924,893 B2	3/2018	Schurman et al.	10,542,903 B2	1/2020	Al-Ali et al.
9,924,897 B1	3/2018	Abdul-Hafiz	10,555,678 B2	2/2020	Dalvi et al.
9,936,917 B2	4/2018	Poeze et al.	10,568,553 B2	2/2020	O'Neil et al.
9,943,269 B2	4/2018	Muhsin et al.	10,608,817 B2	3/2020	Haider et al.
9,949,676 B2	4/2018	Al-Ali	D880,477 S	4/2020	Forrest et al.
9,955,937 B2	5/2018	Telfort	10,617,302 B2	4/2020	Al-Ali et al.
9,965,946 B2	5/2018	Al-Ali et al.	10,617,335 B2	4/2020	Al-Ali et al.
9,980,667 B2	5/2018	Kiani et al.	10,637,181 B2	4/2020	Al-Ali et al.
D820,865 S	6/2018	Muhsin et al.	D886,849 S	6/2020	Muhsin et al.
9,986,919 B2	6/2018	Lamego et al.	D887,548 S	6/2020	Abdul-Hafiz et al.
9,986,952 B2	6/2018	Dalvi et al.	D887,549 S	6/2020	Abdul-Hafiz et al.
9,989,560 B2	6/2018	Poeze et al.	10,667,764 B2	6/2020	Ahmed et al.
9,993,207 B2	6/2018	Al-Ali et al.	D890,708 S	7/2020	Forrest et al.
10,007,758 B2	6/2018	Al-Ali et al.	10,721,785 B2	7/2020	Al-Ali
D822,215 S	7/2018	Al-Ali et al.	10,736,518 B2	8/2020	Al-Ali et al.
D822,216 S	7/2018	Barker et al.	10,750,984 B2	8/2020	Pauley et al.
10,010,276 B2	7/2018	Al-Ali et al.	D897,098 S	9/2020	Al-Ali
10,032,002 B2	7/2018	Kiani et al.	10,779,098 B2	9/2020	Iswanto et al.
10,039,482 B2	8/2018	Al-Ali et al.	10,827,961 B1	11/2020	Iyengar et al.
10,052,037 B2	8/2018	Kinast et al.	10,828,007 B1	11/2020	Telfort et al.
10,058,275 B2	8/2018	Al-Ali et al.	10,832,818 B2	11/2020	Muhsin et al.
10,064,562 B2	9/2018	Al-Ali	10,849,554 B2	12/2020	Shreim et al.
10,086,138 B1	10/2018	Novak, Jr.	10,856,750 B2	12/2020	Indorf
10,092,200 B2	10/2018	Al-Ali et al.	D906,970 S	1/2021	Forrest et al.
10,092,249 B2	10/2018	Kiani et al.	D908,213 S	1/2021	Abdul-Hafiz et al.
10,098,550 B2	10/2018	Al-Ali et al.	10,918,281 B2	2/2021	Al-Ali et al.
10,098,591 B2	10/2018	Al-Ali et al.	10,932,705 B2	3/2021	Muhsin et al.
10,098,610 B2	10/2018	Al-Ali et al.	10,932,729 B2	3/2021	Kiani et al.
10,111,591 B2	10/2018	Dyell et al.	10,939,878 B2	3/2021	Kiani et al.
D833,624 S	11/2018	DeJong et al.	10,953,156 B2	3/2021	Al-Ali et al.
10,123,726 B2	11/2018	Al-Ali et al.	10,956,950 B2	3/2021	Al-Ali et al.
10,123,729 B2	11/2018	Dyell et al.	D916,135 S	4/2021	Indorf et al.
10,130,289 B2	11/2018	Al-Ali et al.	D917,046 S	4/2021	Abdul-Hafiz et al.
10,130,291 B2	11/2018	Schurman et al.	D917,550 S	4/2021	Indorf et al.
D835,282 S	12/2018	Barker et al.	D917,564 S	4/2021	Indorf et al.
D835,283 S	12/2018	Barker et al.	D917,704 S	4/2021	Al-Ali et al.
D835,284 S	12/2018	Barker et al.	10,987,066 B2	4/2021	Chandran et al.
D835,285 S	12/2018	Barker et al.	10,991,135 B2	4/2021	Al-Ali et al.
10,149,616 B2	12/2018	Al-Ali et al.	D919,094 S	5/2021	Al-Ali et al.
10,154,815 B2	12/2018	Al-Ali et al.	D919,100 S	5/2021	Al-Ali et al.
10,159,412 B2	12/2018	Lamego et al.	11,006,867 B2	5/2021	Al-Ali
10,188,296 B2	1/2019	Al-Ali et al.	D921,202 S	6/2021	Al-Ali et al.
10,188,331 B1	1/2019	Kiani et al.	11,024,064 B2	6/2021	Muhsin et al.
10,188,348 B2	1/2019	Al-Ali et al.	11,026,604 B2	6/2021	Chen et al.
RE47,218 E	2/2019	Al-Ali	D925,597 S	7/2021	Chandran et al.
RE47,244 E	2/2019	Kiani et al.	D927,699 S	8/2021	Al-Ali et al.
RE47,249 E	2/2019	Kiani et al.	11,076,777 B2	8/2021	Lee et al.
10,194,847 B2	2/2019	Al-Ali	11,114,188 B2	9/2021	Poeze et al.
10,194,848 B1	2/2019	Kiani et al.	D933,232 S	10/2021	Al-Ali et al.
10,205,291 B2	2/2019	Scruggs et al.	D933,233 S	10/2021	Al-Ali et al.
10,226,187 B2	3/2019	Al-Ali et al.	D933,234 S	10/2021	Al-Ali et al.
10,231,657 B2	3/2019	Al-Ali et al.	11,145,408 B2	10/2021	Sampath et al.
10,231,670 B2	3/2019	Blank et al.	11,147,518 B1	10/2021	Al-Ali et al.
RE47,353 E	4/2019	Kiani et al.	11,185,262 B2	11/2021	Al-Ali et al.
10,279,247 B2	5/2019	Kiani	11,191,484 B2	12/2021	Kiani et al.
10,292,664 B2	5/2019	Al-Ali	D946,596 S	3/2022	Ahmed
10,299,720 B2	5/2019	Brown et al.	D946,597 S	3/2022	Ahmed
10,327,337 B2	6/2019	Schmidt et al.	D946,598 S	3/2022	Ahmed
10,327,713 B2	6/2019	Barker et al.	D946,617 S	3/2022	Ahmed
10,332,630 B2	6/2019	Al-Ali	11,272,839 B2	3/2022	Al-Ali et al.
10,383,520 B2	8/2019	Wojtczuk et al.	11,289,199 B2	3/2022	Al-Ali
10,383,527 B2	8/2019	Al-Ali	RE49,034 E	4/2022	Al-Ali
10,388,120 B2	8/2019	Muhsin et al.	11,298,021 B2	4/2022	Muhsin et al.
D864,120 S	10/2019	Forrest et al.	D950,580 S	5/2022	Ahmed
10,441,181 B1	10/2019	Telfort et al.	D950,599 S	5/2022	Ahmed
10,441,196 B2	10/2019	Eckerbom et al.	D950,738 S	5/2022	Al-Ali et al.
10,448,844 B2	10/2019	Al-Ali et al.	D957,648 S	7/2022	Al-Ali
10,448,871 B2	10/2019	Al-Ali et al.	11,389,093 B2	7/2022	Triman et al.
			11,406,286 B2	8/2022	Al-Ali et al.
			11,417,426 B2	8/2022	Muhsin et al.
			11,439,329 B2	9/2022	Lamego
			11,445,948 B2	9/2022	Scruggs et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0331670	A1	12/2013	Kiani	2015/0099955	A1	4/2015	Al-Ali et al.
2013/0345921	A1	12/2013	Al-Ali et al.	2015/0101844	A1	4/2015	Al-Ali et al.
2014/0012100	A1	1/2014	Al-Ali et al.	2015/0106121	A1	4/2015	Muhsin et al.
2014/0034353	A1	2/2014	Al-Ali et al.	2015/0112151	A1	4/2015	Muhsin et al.
2014/0051953	A1	2/2014	Lamego et al.	2015/0116076	A1	4/2015	Al-Ali et al.
2014/0051954	A1*	2/2014	Al-Ali	2015/0126830	A1	5/2015	Schurman et al.
			A61B 5/14551	2015/0133755	A1	5/2015	Smith et al.
			604/66	2015/0140863	A1	5/2015	Al-Ali et al.
2014/0066783	A1	3/2014	Kiani et al.	2015/0141781	A1	5/2015	Weber et al.
2014/0077956	A1	3/2014	Sampath et al.	2015/0157245	A1	6/2015	Al-Ali et al.
2014/0081100	A1	3/2014	Muhsin et al.	2015/0165312	A1	6/2015	Kiani
2014/0081175	A1	3/2014	Telfort	2015/0196237	A1	7/2015	Lamego
2014/0094666	A1*	4/2014	Fine	2015/0196249	A1	7/2015	Brown et al.
			A61B 5/7278	2015/0201874	A1	7/2015	Diab
			600/324	2015/0208966	A1	7/2015	Al-Ali
2014/0094667	A1	4/2014	Schurman et al.	2015/0216459	A1	8/2015	Al-Ali et al.
2014/0100434	A1	4/2014	Diab et al.	2015/0230755	A1	8/2015	Al-Ali et al.
2014/0114199	A1	4/2014	Lamego et al.	2015/0238722	A1	8/2015	Al-Ali
2014/0120564	A1	5/2014	Workman et al.	2015/0245773	A1	9/2015	Lamego et al.
2014/0121482	A1	5/2014	Merritt et al.	2015/0245793	A1*	9/2015	Al-Ali
2014/0121483	A1	5/2014	Kiani				A61B 5/6826
2014/0127137	A1	5/2014	Bellott et al.	2015/0245794	A1	9/2015	600/322
2014/0129702	A1	5/2014	Lamego et al.	2015/0257689	A1	9/2015	Al-Ali
2014/0135588	A1	5/2014	Al-Ali et al.	2015/0272514	A1	10/2015	Al-Ali et al.
2014/0142401	A1	5/2014	Al-Ali et al.	2015/0351697	A1	12/2015	Kiani et al.
2014/0163344	A1	6/2014	Al-Ali	2015/0351704	A1	12/2015	Weber et al.
2014/0163402	A1	6/2014	Lamego et al.	2015/0359429	A1	12/2015	Kiani et al.
2014/0166076	A1	6/2014	Kiani et al.	2015/0366472	A1	12/2015	Al-Ali et al.
2014/0171763	A1	6/2014	Diab	2015/0366507	A1	12/2015	Kiani
2014/0180038	A1	6/2014	Kiani	2015/0374298	A1	12/2015	Blank et al.
2014/0180154	A1	6/2014	Sierra et al.	2015/0380875	A1	12/2015	Al-Ali et al.
2014/0180160	A1	6/2014	Brown et al.	2016/0000362	A1	1/2016	Coverston et al.
2014/0187973	A1	7/2014	Brown et al.	2016/0007930	A1	1/2016	Diab et al.
2014/0194766	A1	7/2014	Al-Ali et al.	2016/0029932	A1	2/2016	Weber et al.
2014/0206963	A1	7/2014	Al-Ali	2016/0029933	A1	2/2016	Al-Ali
2014/0213864	A1	7/2014	Abdul-Hafiz et al.	2016/0045118	A1	2/2016	Al-Ali et al.
2014/0266790	A1	9/2014	Al-Ali et al.	2016/0051205	A1	2/2016	Kiani
2014/0275808	A1	9/2014	Poeze et al.	2016/0058338	A1	2/2016	Al-Ali et al.
2014/0275835	A1	9/2014	Lamego et al.	2016/0058347	A1	3/2016	Schurman et al.
2014/0275871	A1	9/2014	Lamego et al.	2016/0058347	A1	3/2016	Reichgott et al.
2014/0275872	A1	9/2014	Merritt et al.	2016/0066823	A1	3/2016	Al-Ali et al.
2014/0275881	A1	9/2014	Lamego et al.	2016/0066824	A1	3/2016	Al-Ali et al.
2014/0276115	A1	9/2014	Dalvi et al.	2016/0066879	A1	3/2016	Al-Ali et al.
2014/0288400	A1	9/2014	Diab et al.	2016/0072429	A1	3/2016	Telfort et al.
2014/0303520	A1	10/2014	Telfort et al.	2016/0073967	A1	3/2016	Kiani et al.
2014/0316217	A1	10/2014	Purdon et al.	2016/0073967	A1	3/2016	Lamego et al.
2014/0316218	A1	10/2014	Purdon et al.	2016/0081552	A1	3/2016	Wojtczuk et al.
2014/0316228	A1	10/2014	Blank et al.	2016/0095543	A1	3/2016	Telfort et al.
2014/0323825	A1	10/2014	Al-Ali et al.	2016/0095548	A1	4/2016	Al-Ali et al.
2014/0323897	A1	10/2014	Brown et al.	2016/0103598	A1	4/2016	Telfort et al.
2014/0323898	A1	10/2014	Purdon et al.	2016/0113527	A1	4/2016	Al-Ali et al.
2014/0330092	A1	11/2014	Al-Ali et al.	2016/0143548	A1	5/2016	Al-Ali
2014/0330098	A1	11/2014	Merritt et al.	2016/0166182	A1	6/2016	Al-Ali et al.
2014/0330099	A1	11/2014	Al-Ali et al.	2016/0166183	A1	6/2016	Al-Ali et al.
2014/0336481	A1	11/2014	Shakespeare et al.	2016/0166188	A1	6/2016	Poeze et al.
2014/0357966	A1	12/2014	Al-Ali et al.	2016/0166188	A1	6/2016	Bruinsma et al.
2014/0371548	A1	12/2014	Al-Ali et al.	2016/0166210	A1	6/2016	Al-Ali
2014/0371632	A1	12/2014	Al-Ali et al.	2016/0192869	A1	7/2016	Al-Ali et al.
2014/0378784	A1	12/2014	Kiani et al.	2016/0196388	A1	7/2016	Kiani et al.
2015/0005600	A1	1/2015	Blank et al.	2016/0197436	A1	7/2016	Lamego
2015/0011907	A1	1/2015	Purdon et al.	2016/0213281	A1	7/2016	Barker et al.
2015/0012231	A1	1/2015	Poeze et al.	2016/0228043	A1	7/2016	Eckerbom et al.
2015/0018650	A1	1/2015	Al-Ali et al.	2016/0228043	A1	8/2016	O'Neil et al.
2015/0025406	A1	1/2015	Al-Ali	2016/0233632	A1	8/2016	Scruggs et al.
2015/0032029	A1	1/2015	Al-Ali et al.	2016/0234944	A1	8/2016	Schmidt et al.
2015/0038859	A1	2/2015	Dalvi et al.	2016/0270735	A1	9/2016	Diab et al.
2015/0045637	A1	2/2015	Dalvi	2016/0283665	A1	9/2016	Sampath et al.
2015/0045685	A1	2/2015	Al-Ali et al.	2016/0287090	A1	10/2016	Al-Ali et al.
2015/0051462	A1	2/2015	Olsen	2016/0287786	A1	10/2016	Kiani
2015/0073241	A1	3/2015	Lamego	2016/0296169	A1	10/2016	McHale et al.
2015/0080754	A1	3/2015	Purdon et al.	2016/0310052	A1	10/2016	Al-Ali et al.
2015/0087936	A1	3/2015	Al-Ali et al.	2016/0314260	A1	10/2016	Kiani
2015/0094546	A1	4/2015	Al-Ali	2016/0324486	A1	11/2016	Al-Ali et al.
2015/0097701	A1	4/2015	Muhsin et al.	2016/0324488	A1	11/2016	Olsen
2015/0099324	A1	4/2015	Wojtczuk et al.	2016/0327984	A1	11/2016	Al-Ali et al.
2015/0099950	A1	4/2015	Al-Ali et al.	2016/0328528	A1	11/2016	Al-Ali et al.
2015/0099951	A1	4/2015	Al-Ali et al.	2016/0331332	A1	11/2016	Al-Ali
				2016/0367173	A1	12/2016	Dalvi et al.
				2017/0007134	A1	1/2017	Al-Ali et al.
				2017/0007190	A1	1/2017	Al-Ali et al.
				2017/0007198	A1	1/2017	Al-Ali et al.
				2017/0014083	A1	1/2017	Diab et al.
				2017/0014084	A1	1/2017	Al-Ali et al.

(56)		References Cited					
U.S. PATENT DOCUMENTS							
2017/0021099	A1*	1/2017	Al-Ali	A61B 5/1455	2018/0214090 A1	8/2018	Al-Ali et al.
2017/0024748	A1	1/2017	Haider		2018/0218792 A1	8/2018	Muhsin et al.
2017/0027456	A1	2/2017	Kinast et al.		2018/0225960 A1	8/2018	Al-Ali et al.
2017/0042488	A1	2/2017	Muhsin		2018/0238718 A1	8/2018	Dalvi
2017/0055847	A1	3/2017	Kiani et al.		2018/0242853 A1	8/2018	Al-Ali
2017/0055851	A1	3/2017	Al-Ali		2018/0242921 A1	8/2018	Muhsin et al.
2017/0055882	A1	3/2017	Al-Ali et al.		2018/0242923 A1	8/2018	Al-Ali et al.
2017/0055887	A1	3/2017	Al-Ali		2018/0242924 A1	8/2018	Barker et al.
2017/0055896	A1	3/2017	Al-Ali		2018/0242926 A1	8/2018	Muhsin et al.
2017/0079594	A1	3/2017	Telfort et al.		2018/0247353 A1	8/2018	Al-Ali et al.
2017/0086723	A1	3/2017	Al-Ali et al.		2018/0247712 A1	8/2018	Muhsin et al.
2017/0143281	A1	5/2017	Olsen		2018/0249933 A1	9/2018	Schurman et al.
2017/0147774	A1	5/2017	Kiani		2018/0253947 A1	9/2018	Muhsin et al.
2017/0156620	A1	6/2017	Al-Ali et al.		2018/0256087 A1	9/2018	Al-Ali et al.
2017/0173632	A1	6/2017	Al-Ali		2018/0256113 A1	9/2018	Weber et al.
2017/0187146	A1	6/2017	Kiani et al.		2018/0285094 A1	10/2018	Housel et al.
2017/0188919	A1	7/2017	Al-Ali et al.		2018/0289325 A1	10/2018	Poeze et al.
2017/0196464	A1	7/2017	Jansen et al.		2018/0289337 A1	10/2018	Al-Ali et al.
2017/0196470	A1	7/2017	Lamego et al.		2018/0296161 A1	10/2018	Shreim et al.
2017/0224262	A1	8/2017	Al-Ali		2018/0300919 A1	10/2018	Muhsin et al.
2017/0228516	A1	8/2017	Sampath et al.		2018/0310822 A1	11/2018	Indorf et al.
2017/0245790	A1	8/2017	Al-Ali et al.		2018/0310823 A1	11/2018	Al-Ali et al.
2017/0251974	A1	9/2017	Shreim et al.		2018/0317826 A1	11/2018	Muhsin et al.
2017/0251975	A1	9/2017	Shreim et al.		2018/0317841 A1	11/2018	Novak, Jr.
2017/0258403	A1	9/2017	Abdul-Hafiz et al.		2018/0333055 A1	11/2018	Lamego et al.
2017/0311891	A1	11/2017	Kiani et al.		2018/0333087 A1	11/2018	Al-Ali
2017/0332976	A1	11/2017	Al-Ali		2019/0000317 A1	1/2019	Muhsin et al.
2017/0340293	A1	11/2017	Al-Ali et al.		2019/0000362 A1	1/2019	Kiani et al.
2017/0360310	A1	12/2017	Kiani		2019/0015023 A1	1/2019	Monfre
2017/0367632	A1	12/2017	Al-Ali et al.		2019/0209060 A1*	7/2019	Katra
2018/0008146	A1	1/2018	Al-Ali et al.		2019/0239787 A1	8/2019	Pauley et al.
2018/0013562	A1	1/2018	Haider et al.		2019/0320906 A1	10/2019	Olsen
2018/0014752	A1	1/2018	Al-Ali et al.		2019/0374713 A1	12/2019	Kiani et al.
2018/0028124	A1	2/2018	Al-Ali et al.		2020/0060869 A1	2/2020	Telfort et al.
2018/0055385	A1	3/2018	Al-Ali		2020/0111552 A1	4/2020	Ahmed
2018/0055390	A1	3/2018	Kiani et al.		2020/0113520 A1	4/2020	Abdul-Hafiz et al.
2018/0055430	A1	3/2018	Diab et al.		2020/0138368 A1	5/2020	Kiani et al.
2018/0064381	A1	3/2018	Shakespeare et al.		2020/0163597 A1	5/2020	Dalvi et al.
2018/0069776	A1	3/2018	Lamego et al.		2020/0196877 A1	6/2020	Vo et al.
2018/0070831	A1*	3/2018	Sutin	A61B 5/031	2020/0246544 A1*	8/2020	Al-Ali
2018/0070867	A1	3/2018	Smith et al.		2020/0253474 A1	8/2020	Muhsin et al.
2018/0082767	A1	3/2018	Al-Ali et al.		2020/0253544 A1	8/2020	Belur Nagaraj et al.
2018/0085068	A1	3/2018	Telfort		2020/0275841 A1	9/2020	Telfort et al.
2018/0087937	A1	3/2018	Al-Ali et al.		2020/0288983 A1	9/2020	Telfort et al.
2018/0103874	A1	4/2018	Lee et al.		2020/0321793 A1	10/2020	Al-Ali et al.
2018/0103905	A1	4/2018	Kiani		2020/0329983 A1	10/2020	Al-Ali et al.
2018/0110478	A1	4/2018	Al-Ali		2020/0329984 A1	10/2020	Al-Ali et al.
2018/0116575	A1	5/2018	Perea et al.		2020/0329993 A1	10/2020	Al-Ali et al.
2018/0125368	A1	5/2018	Lamego et al.		2020/0330037 A1	10/2020	Al-Ali et al.
2018/0125430	A1	5/2018	Al-Ali et al.		2021/0022628 A1	1/2021	Telfort et al.
2018/0125445	A1	5/2018	Telfort et al.		2021/0104173 A1	4/2021	Pauley et al.
2018/0130325	A1	5/2018	Kiani et al.		2021/0113121 A1	4/2021	Diab et al.
2018/0132769	A1	5/2018	Weber et al.		2021/0117525 A1	4/2021	Kiani et al.
2018/0132770	A1	5/2018	Lamego		2021/0118581 A1	4/2021	Kiani et al.
2018/0146901	A1	5/2018	Al-Ali et al.		2021/0121582 A1	4/2021	Krishnamani et al.
2018/0146902	A1	5/2018	Kiani et al.		2021/0161465 A1	6/2021	Barker et al.
2018/0153442	A1	6/2018	Eckerbom et al.		2021/0236729 A1	8/2021	Kiani et al.
2018/0153446	A1	6/2018	Kiani		2021/0256267 A1	8/2021	Ranasinghe et al.
2018/0153447	A1	6/2018	Al-Ali et al.		2021/0256835 A1	8/2021	Ranasinghe et al.
2018/0153448	A1	6/2018	Weber et al.		2021/0275101 A1	9/2021	Vo et al.
2018/0153455	A1*	6/2018	Guazzi	A61B 5/02416	2021/0290060 A1	9/2021	Ahmed
2018/0161499	A1*	6/2018	Al-Ali	A61B 5/4836	2021/0290072 A1	9/2021	Forrest
2018/0168491	A1	6/2018	Al-Ali et al.		2021/0290080 A1	9/2021	Ahmed
2018/0174679	A1	6/2018	Sampath et al.		2021/0290120 A1	9/2021	Al-Ali
2018/0174680	A1	6/2018	Sampath et al.		2021/0290177 A1	9/2021	Novak, Jr.
2018/0182484	A1	6/2018	Sampath et al.		2021/0290184 A1	9/2021	Ahmed
2018/0184917	A1	7/2018	Kiani		2021/0296008 A1	9/2021	Novak, Jr.
2018/0192924	A1	7/2018	Al-Ali		2021/0307661 A1*	10/2021	Katra
2018/0192953	A1	7/2018	Shreim et al.		2021/0316071 A1*	10/2021	Al-Ali
2018/0192955	A1	7/2018	Al-Ali et al.		2021/0330228 A1	10/2021	Olsen et al.
2018/0199871	A1	7/2018	Pauley et al.		2021/0386382 A1	12/2021	Olsen et al.
2018/0206795	A1	7/2018	Al-Ali		2021/0402110 A1	12/2021	Pauley et al.
2018/0206815	A1	7/2018	Telfort		2022/0026355 A1	1/2022	Normand et al.
2018/0213583	A1	7/2018	Al-Ali		2022/0039707 A1	2/2022	Sharma et al.
2018/0214031	A1	8/2018	Kiani et al.		2022/0053892 A1	2/2022	Al-Ali et al.
					2022/0071562 A1	3/2022	Kiani
					2022/0096603 A1	3/2022	Kiani et al.
					2022/0151521 A1	5/2022	Krishnamani et al.
					2022/0218244 A1	7/2022	Kiani et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2022/0287574 A1 9/2022 Telfort et al.
 2022/0296161 A1 9/2022 Al-Ali et al.
 2022/0361819 A1 11/2022 Al-Ali et al.
 2022/0379059 A1 12/2022 Yu et al.
 2022/0392610 A1 12/2022 Kiani et al.
 2023/0028745 A1 1/2023 Al-Ali

FOREIGN PATENT DOCUMENTS

DE 3711272 5/1989
 DE 19531520 1/1997
 EP 0 013 278 7/1980
 EP 0 019 278 11/1980
 EP 0 019 478 11/1980
 EP 0 074 428 3/1983
 EP 0 262 779 4/1988
 EP 0 313 238 10/1988
 EP 0 329 196 8/1989
 EP 0 104 772 3/1990
 EP 0 404 562 12/1990
 EP 0 481 612 4/1992
 EP 0 538 631 4/1993
 EP 0 640 978 3/1995
 EP 0 745 348 12/1996
 EP 0 832 598 4/1998
 EP 0 576 560 5/2000
 EP 0 790 800 8/2000
 EP 1 281 353 2/2003
 EP 1 424 036 6/2004
 JP 52-031736 3/1977
 JP 62-217938 9/1987
 JP 63-065844 3/1988
 JP 63-050694 4/1988
 JP 02-017462 1/1990
 JP 02-191434 7/1990
 JP 03-245042 10/1991
 JP 04-138342 5/1992
 JP 04-250140 9/1992
 JP 04-306725 10/1992
 JP 04-312447 11/1992
 JP 05-207993 8/1993
 JP 05-275746 10/1993
 JP 05-334458 12/1993
 JP 06-003890 1/1994
 JP 06-237013 8/1994
 JP 08-015023 1/1996
 JP 08-315919 11/1996
 JP 09-187442 7/1997
 JP 10-165420 6/1998
 JP 10-314149 12/1998
 JP 11-053662 2/1999
 JP 11-156657 6/1999
 JP 11-170568 6/1999
 JP 11-185193 7/1999
 JP 3135765 2/2001
 JP 2003-506778 2/2003
 JP 2003-521985 7/2003
 JP 2006-512948 4/2006
 RU 2096985 11/1997
 WO 88/010462 12/1988
 WO 92/001894 2/1992
 WO 92/016142 10/1992
 WO 96/013208 5/1996
 WO 97/023159 7/1997
 WO 97/029678 8/1997
 WO 00/042911 7/2000
 WO 01/009733 2/2001
 WO 01/013790 3/2001
 WO 01/030414 5/2001

WO 01/041634 6/2001
 WO 01/058347 8/2001
 WO 02/015781 2/2002
 WO 02/017779 3/2002
 WO 03/073927 9/2003
 WO 2004/060155 7/2004
 WO 2005/011488 2/2005
 WO 2005/040793 5/2005
 WO 2006/023721 3/2006
 WO 2006/048840 5/2006
 WO 2008/054976 5/2008

OTHER PUBLICATIONS

US 2022/0192529 A1, 06/2022, Al-Ali et al. (withdrawn)
 Ruckman, Jared S., "A Comparative Study of Total Hemoglobin Measurement Technology: Noninvasive Pulse Coximetry and Conventional Methods", University of Connecticut Graduate School, Master's Theses, May 7, 2011, pp. 55.
 Scharf, MD, John E., "Optimization of Portable Pulse Oximetry Through Fourier Analysis", USD Department of Anesthesiology; USF Department of Electrical Engineering, 1993, pp. 233-235.
 Wolf et al., "Correlation of Functional and Resting State Connectivity of Cerebral oxy-, deoxy-, and Total Hemoglobin Concentration Changes Measured by Near-Infrared Spectrophotometry", Journal of Biomedical Optics, Aug. 2011, vol. 16, No. 8, pp. 13.
 De Kock, J.P. et al., "The Effect of Varying LED Intensity on Pulse Oximeter Accuracy", Journal of Medical Engineering & Technology, vol. 15, No. 3, May/Jun. 1991, pp. 111-116.
<http://www.masimo.com/adt.htm>, "Inop adt—Adult Disposable Digit Sensor," 1 page, reviewed on Sep. 17, 1999.
<http://www.masimo.com/cables.htm>, "Patient Cables", 1 page, reviewed on Sep. 17, 1999.
<http://www.masimo.com/pndt.htm>, "Products & Technology", 1 page, reviewed on Sep. 17, 1999.
<http://www.masimo.com/systemo.htm>, "System Overview & Performance", 2 pages, reviewed on Sep. 17, 1999.
http://www.mrequipment.com/products/oximetry_patient_mntrg.htm, "MR Equipment Magnetic Resonance Equipment Corporation, MR-Compatible High-Performance Optical Fiber Sensors, Pulse Oximetry Sensors for MRI Fiber Optic Sensors for use with MR-Compatible Pulse Oximeter", 2 pages, reviewed on Sep. 17, 1999.
 Masimo Corporation, "Discrete Saturation Transforms Example", reviewed on Sep. 17, 1999.
 MSP Industry Alert, Masimo to Introduce NR7 at ASA, pp. 18, 19, and the front and back cover, vol. 3, No. 3, Fall 2001.
 Reynolds, K.J., et al., "Temperature Dependence of LED and its Theoretical Effect on Pulse Oximetry", British Journal & Anesthesia, 1991, vol. 67, pp. 638-643.
 Schmitt, Joseph M., "Simple Photon Diffusion Analysis of the Effects of Multiple Scattering on Pulse Oximetry", IEEE Transactions on Biomedical Engineering, vol. 38, No. 12, Dec. 1991, pp. 1194-1203.
 International Search Report and Written Opinion received in PCT Application No. PCT/US2007/081146, dated May 21, 2008 in 10 pages.
 International Preliminary Report on Patentability dated Nov. 26, 2008 for International Application No. PCT/US2007/081146, filed Oct. 11, 2007, 12 pages.
 Office Action dated Jan. 31, 2013 issued in Japanese Application No. 2009-532585, along with its English Translation, 6 pages.
 Office Action dated Oct. 25, 2013 issued in Japanese Application No. 2009-532585, along with its English Translation, 10 pages.
 Final Office Action dated Apr. 1, 2014 issued in Japanese Application No. 2009-532585, along with its English Translation, 6 pages.

* cited by examiner

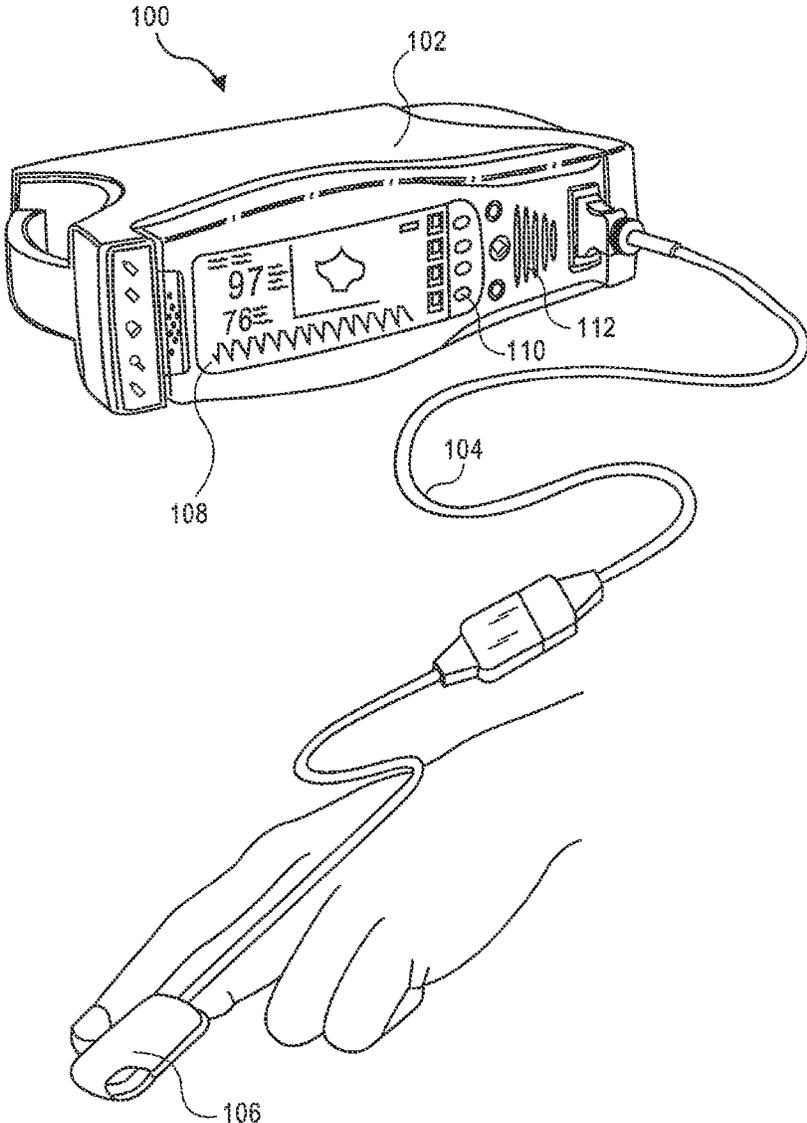


FIG. 1

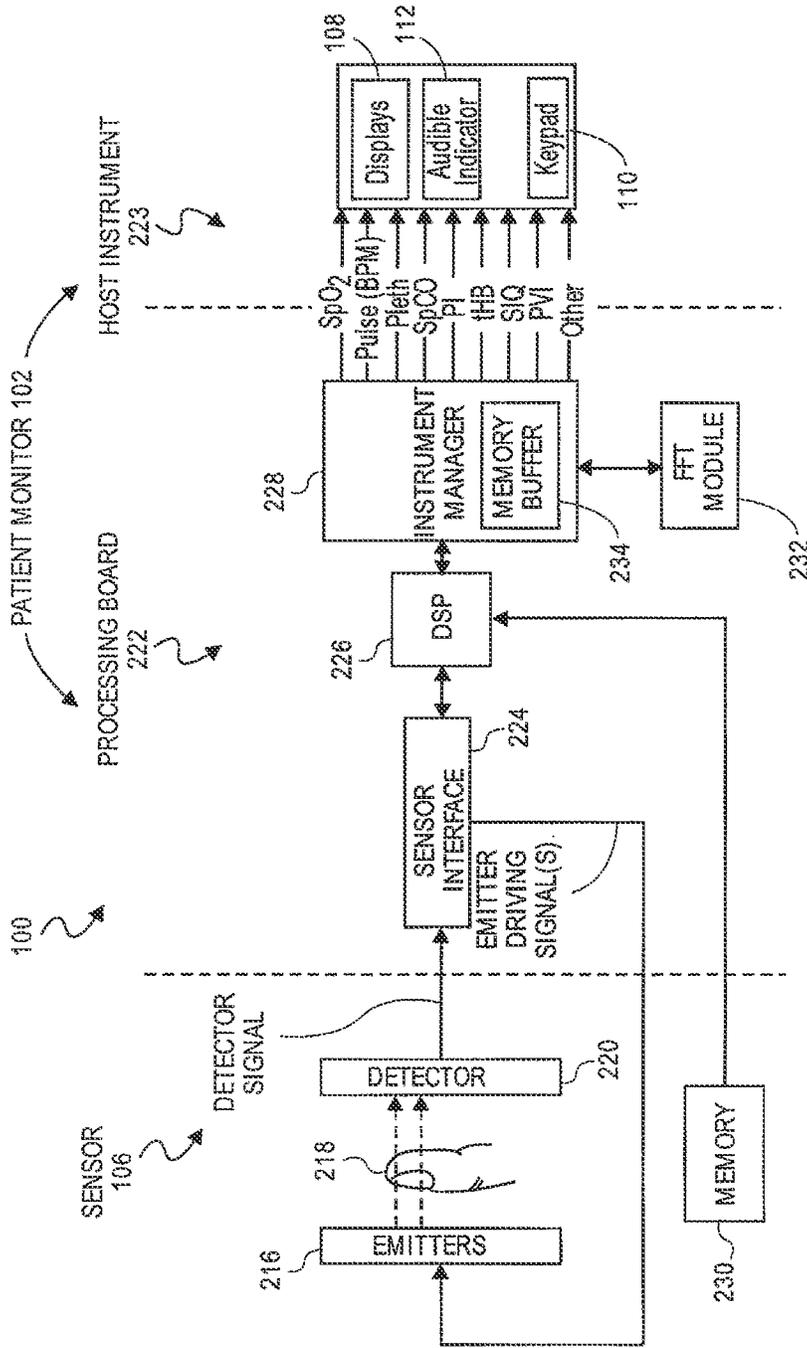


FIG. 2

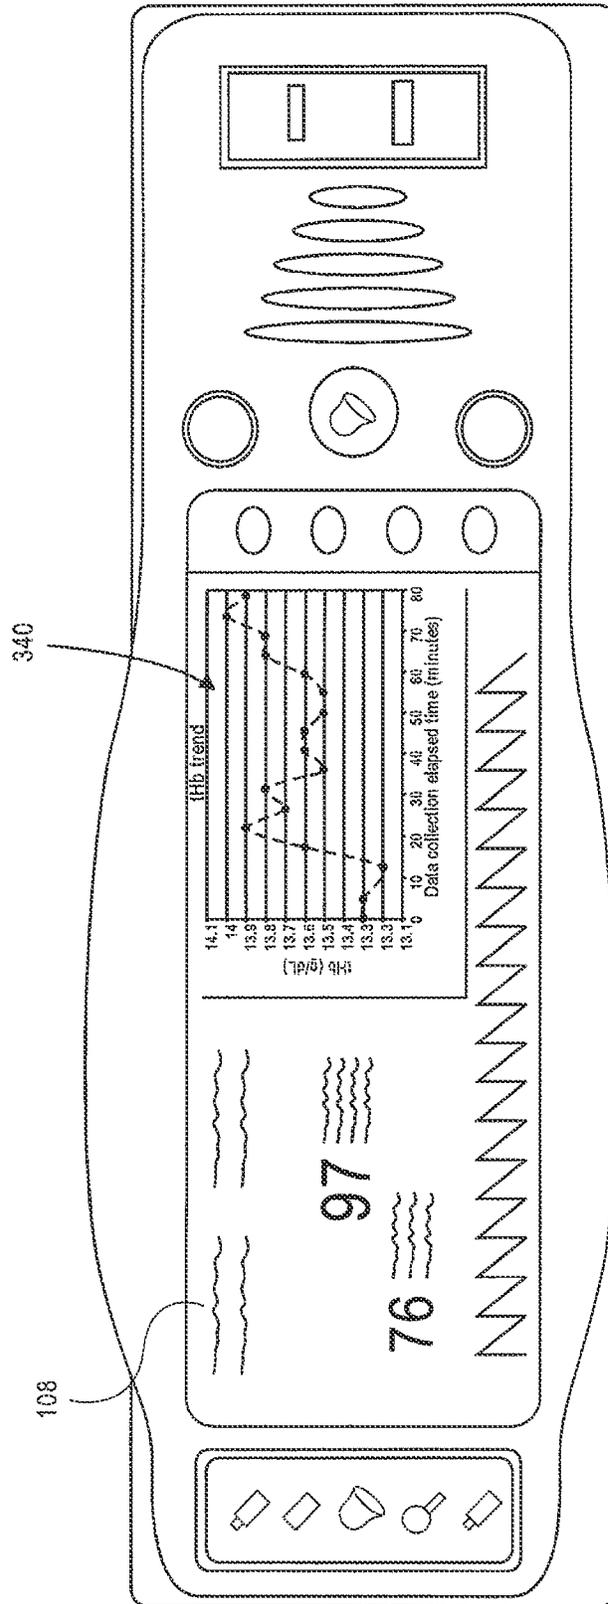
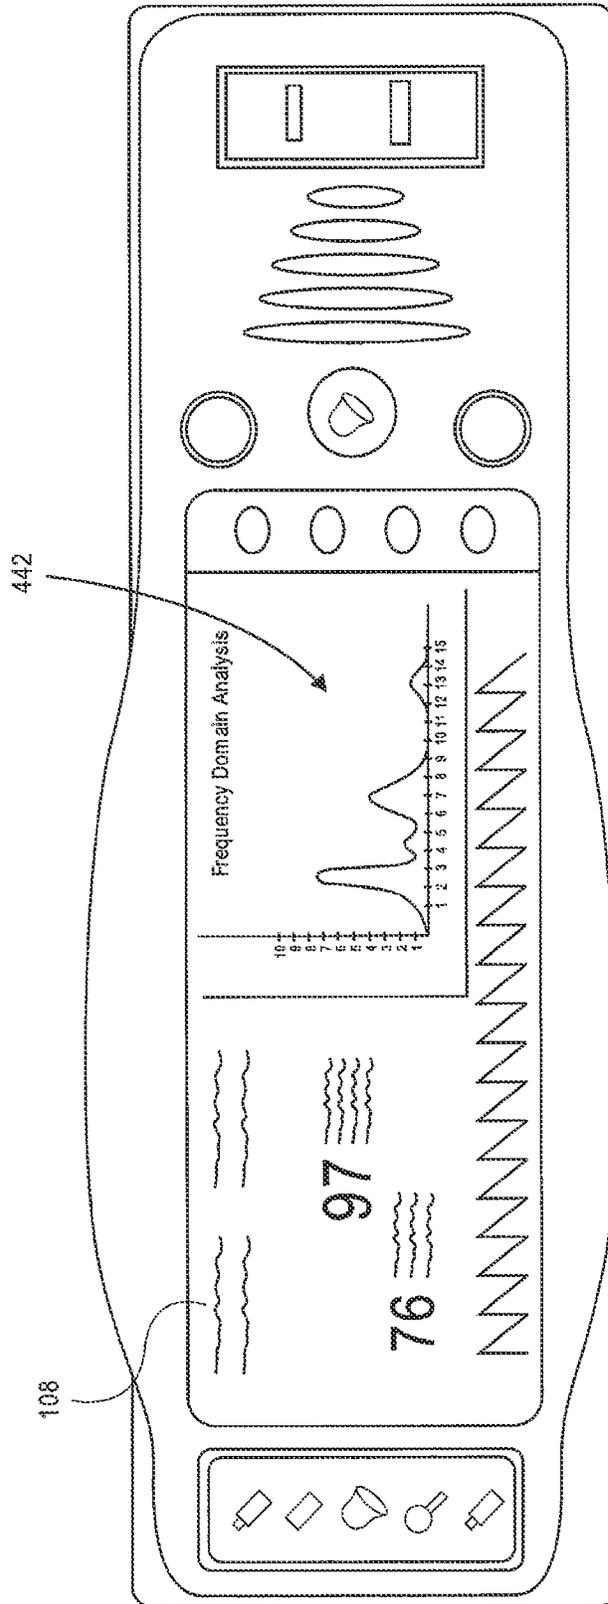


FIG. 3



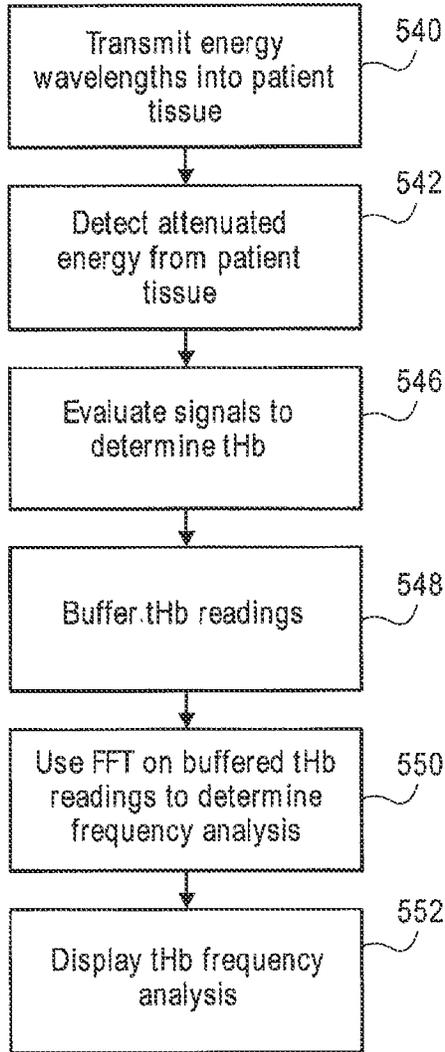


FIG. 5

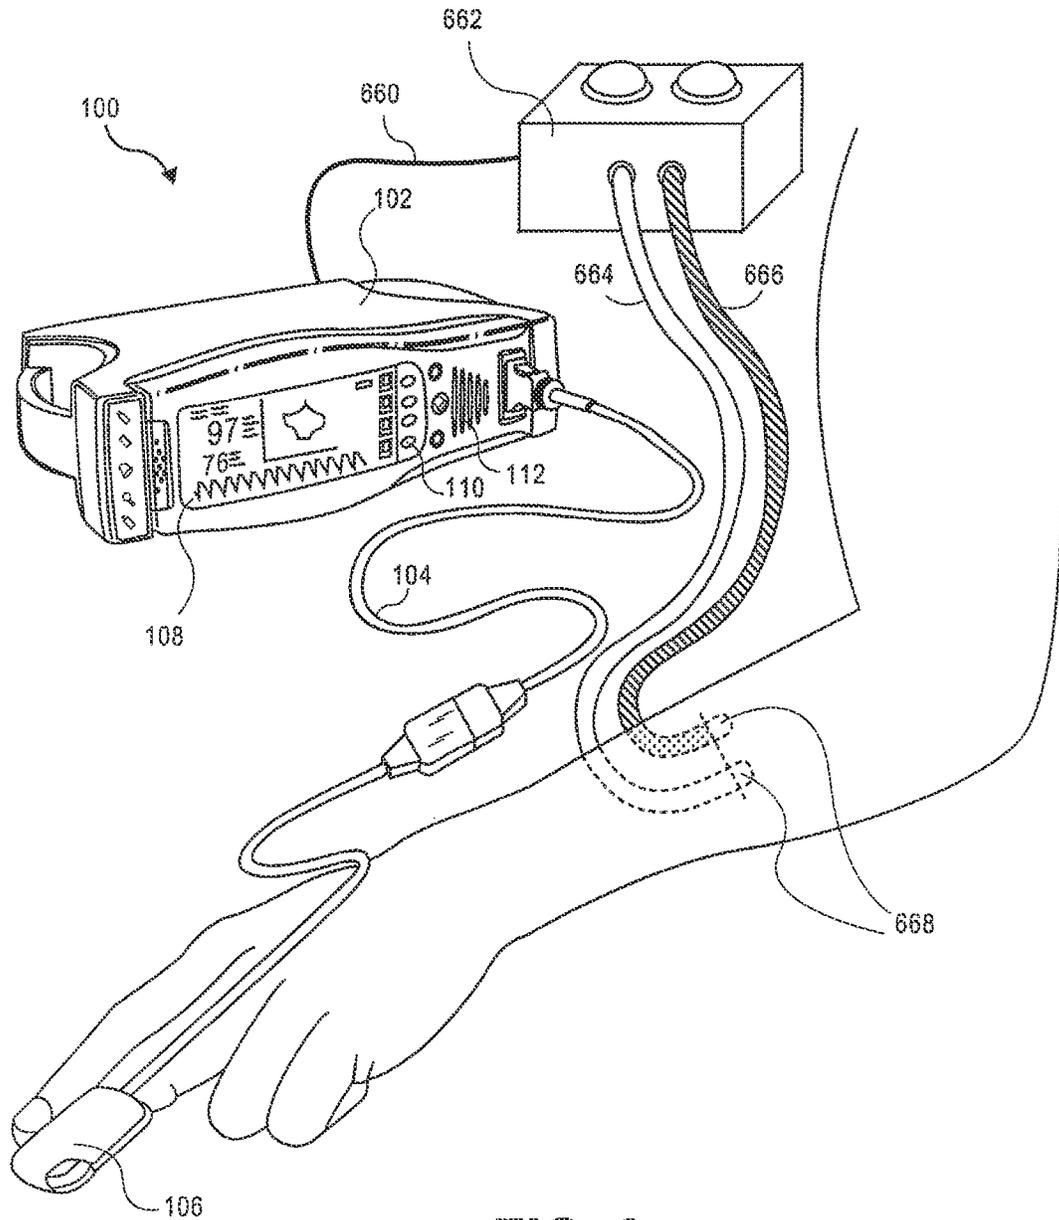


FIG. 6

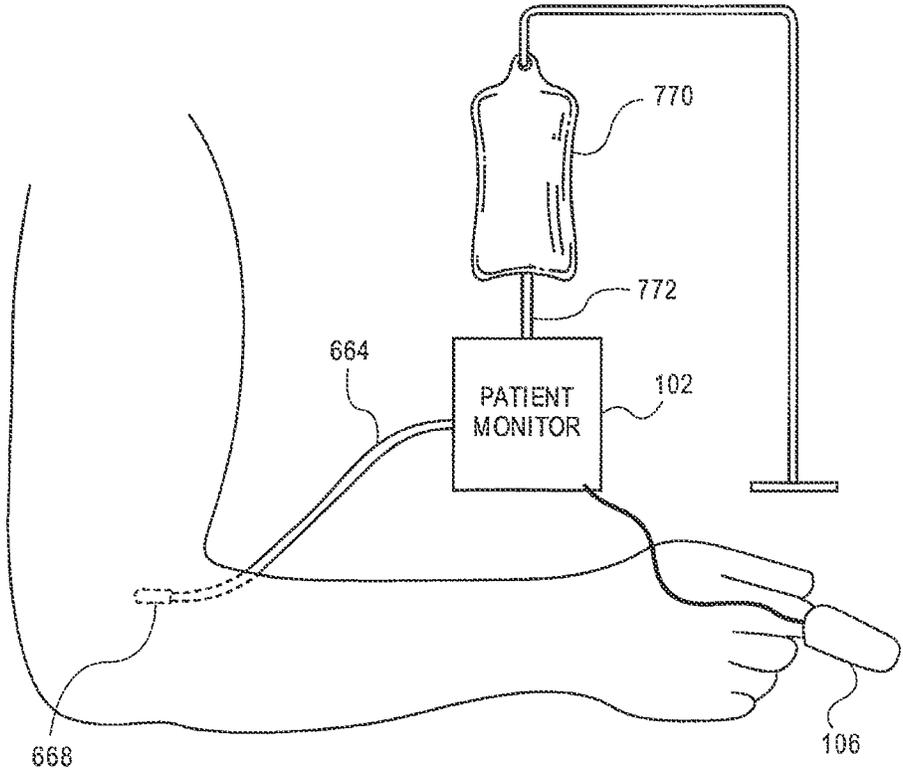


FIG. 7

HEMOGLOBIN DISPLAY AND PATIENT TREATMENT

REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 16/571,591, filed Sep. 16, 2019, entitled "HEMOGLOBIN DISPLAY AND PATIENT TREATMENT," which is a continuation of U.S. application Ser. No. 15/789,357, filed Oct. 20, 2017, entitled "HEMOGLOBIN DISPLAY AND PATIENT TREATMENT," which is a continuation of U.S. patent application Ser. No. 15/184,950, filed Jun. 16, 2016, entitled "HEMOGLOBIN DISPLAY AND PATIENT TREATMENT," which is a continuation of U.S. patent Ser. No. 14/714,691, filed May 18, 2015, now U.S. Pat. No. 9,370,325, entitled "HEMOGLOBIN DISPLAY AND PATIENT TREATMENT," which is a continuation of U.S. patent application Ser. No. 14/064,026, filed Oct. 25, 2013, now U.S. Pat. No. 9,037,207, entitled "Hemoglobin Display and Patient Treatment," which is a continuation of U.S. patent application Ser. No. 12/783,436, filed May 19, 2010, now U.S. Pat. No. 8,571,619, entitled "Hemoglobin Display and Patient Treatment," which claims priority benefit under 35 U.S.C. § 119(e) of U.S. Provisional Application Nos. 61/180,018 filed May 20, 2009, entitled "Hemoglobin Display," and 61/221,435 entitled "Hemoglobin Display and Patient Treatment," filed Jun. 29, 2009. The present application incorporates the disclosures of the foregoing applications herein by reference in their entireties.

FIELD OF THE INVENTION

The present disclosure relates to the processing and display of a hemoglobin measurement.

BACKGROUND

During patient care, it is important to know the composition of the patient's blood. Knowing the composition of the patient's blood can provide an indication of the patient's condition, assist in patient diagnosis, and assist in determining a course of treatment. One blood component in particular, hemoglobin, is very important. Hemoglobin is responsible for the transport of oxygen from the lungs to the rest of the body. If there is insufficient total hemoglobin or if the hemoglobin is unable to bind with or carry enough oxygen, then the patient can suffocate. In addition to oxygen, other molecules can bind to hemoglobin. For example, hemoglobin can bind with carbon monoxide to form carboxyhemoglobin. When other molecules bind to hemoglobin, the hemoglobin is unable to carry oxygen molecules, and thus the patient is deprived of oxygen. Also, hemoglobin can change its molecular form and become unable to carry oxygen, this type of hemoglobin is called methemoglobin.

Pulse oximetry systems for measuring constituents of circulating blood have gained rapid acceptance in a wide variety of medical applications including surgical wards, intensive care and neonatal units, general wards, home care, physical training, and virtually all types of monitoring scenarios. A pulse oximetry system generally includes an optical sensor applied to a patient, a monitor for processing sensor signals and displaying results and a patient cable electrically interconnecting the sensor and the monitor. A pulse oximetry sensor has light emitting diodes (LEDs), typically at least one emitting a red wavelength and one emitting an infrared (IR) wavelength, and a photodiode detector. The emitters and detector are attached to a patient

tissue site, such as a finger. The patient cable transmits drive signals to these emitters from the monitor, and the emitters respond to the drive signals to transmit light into the tissue site. The detector generates a signal responsive to the emitted light after attenuation by pulsatile blood flow within the tissue site. The patient cable transmits the detector signal to the monitor, which processes the signal to provide a numerical readout of physiological parameters such as oxygen saturation (SpO₂) and pulse rate.

Standard pulse oximeters, however, are unable to provide an indication of how much hemoglobin is in a patient's blood or whether other molecules were binding to hemoglobin and preventing the hemoglobin from binding with oxygen. Care givers had no alternative but to measure most hemoglobin parameters, such as total hemoglobin, methemoglobin and carboxyhemoglobin by drawing blood and analyzing it in a lab. Given the nature of non-continuous blood analysis in a lab, it was widely believed that total hemoglobin did not change rapidly.

Advanced physiological monitoring systems utilize multiple wavelength sensors and multiple parameter monitors to provide enhanced measurement capabilities including, for example, the measurement of carboxyhemoglobin (HbCO), methemoglobin (HbMet) and total hemoglobin (Hbt or tHb). Physiological monitors and corresponding multiple wavelength optical sensors are described in at least U.S. patent application Ser. No. 11/367,013, filed Mar. 1, 2006 and titled Multiple Wavelength Sensor Emitters and U.S. patent application Ser. No. 11/366,208, filed Mar. 1, 2006 and titled Noninvasive Multi-Parameter Patient Monitor, both assigned to Masimo Laboratories, Irvine, Calif. ("Masimo Labs") and both incorporated by reference herein. Pulse oximeters capable of reading through motion induced noise are disclosed in at least U.S. Pat. Nos. 6,770,028, 6,658,276, 6,650,917, 6,157,850, 6,002,952, 5,769,785, and 5,758,644; low noise pulse oximetry sensors are disclosed in at least U.S. Pat. Nos. 6,088,607 and 5,782,757; all of which are assigned to Masimo Corporation, Irvine, Calif. ("Masimo") and are incorporated by reference herein.

Further, physiological monitoring systems that include low noise optical sensors and pulse oximetry monitors, such as any of LNOP® adhesive or reusable sensors, SofTouch™ sensors, Hi-Fi Trauma™ or Blue™ sensors; and any of Radical®, SatShare™, Rad-9™, Rad-S™, Rad-5v™ or PPO+™ Masimo SET® pulse oximeters, are all available from Masimo. Physiological monitoring systems including multiple wavelength sensors and corresponding noninvasive blood parameter monitors, such as Rainbow™ adhesive and reusable sensors and Rad-57™, Rad-87™ and Radical-7™ monitors for measuring SpO₂, pulse rate, perfusion index, signal quality, HbCO and HbMet among other parameters are also available from Masimo.

SUMMARY

The present disclosure provides for the measurement, display and analysis of hemoglobin content in living patients. It has been discovered that, contrary to the widely held understanding that total hemoglobin does not change rapidly, total hemoglobin fluctuates over time. In an embodiment, the trend of a patient's continuous total hemoglobin (tHb or Hbt) measurement is displayed on a display. In an embodiment, the trend of the total hemoglobin is analyzed through, for example, a frequency domain analysis to determine patterns in the patient hemoglobin fluctuation. In an embodiment, a frequency domain analysis is used to determine a specific signature of the hemoglobin variability

specific to a particular patient. In some embodiments, the specific elements of a patient's hemoglobin variability may provide information useful for the diagnosis of specific diseases, including, for example, diseases that affect hemoglobin and red blood cell function such as sickle cell anemia.

Additionally, exemplary uses of these hemoglobin readings are illustrated in conjunction with dialysis treatment and blood transfusions.

BRIEF DESCRIPTION OF THE DRAWINGS

The drawings and following associated descriptions are provided to illustrate embodiments of the present disclosure and do not limit the scope of the claims. Corresponding numerals indicate corresponding parts, and the leading digit of each numbered item indicates the first figure in which an item is found.

FIG. 1 illustrates a perspective view of a patient monitoring system in accordance with an embodiment of the disclosure.

FIG. 2 illustrates a block drawing of a patient monitoring system in accordance with an embodiment of the disclosure.

FIG. 3 illustrates a planar view of a patient monitor displaying a sample graph of total hemoglobin versus time as may be displayed by a patient monitoring system in accordance with an embodiment of the disclosure.

FIG. 4 illustrates a planar view of a patient monitor displaying a graph of a frequency domain analysis.

FIG. 5 illustrates a block diagram of a method of monitoring and analyzing a patient's total hemoglobin levels.

FIG. 6 illustrates a perspective view of a patient monitoring system and blood manipulation device, such as a dialysis machine, in accordance with an embodiment of the disclosure.

FIG. 7 illustrates a block diagram of a patient monitoring system, including transfusion capabilities in accordance with an embodiment of the disclosure.

DETAILED DESCRIPTION

Aspects of the disclosure will now be set forth in detail with respect to the figures and various embodiments. One of skill in the art will appreciate, however, that other embodiments and configurations of the devices and methods disclosed herein will still fall within the scope of this disclosure even if not described in the same detail as some other embodiments. Aspects of various embodiments discussed do not limit the scope of the disclosure herein, which is instead defined by the claims following this description.

Turning to FIG. 1, an embodiment of a patient monitoring system 100 is illustrated. The patient monitoring system 100 includes a patient monitor 102 attached to a sensor 106 by a cable 104. The sensor monitors various physiological data of a patient and sends signals indicative of the parameters to the patient monitor 102 for processing. The patient monitor 102 generally includes a display 108, control buttons 110, and a speaker 112 for audible alerts. The display 108 is capable of displaying readings of various monitored patient parameters, which may include numerical readouts, graphical readouts, and the like. Display 108 may be a liquid crystal display (LCD), a cathode ray tube (CRT), a plasma screen, a Light Emitting Diode (LED) screen, Organic Light Emitting Diode (OLED) screen, or any other suitable display. A patient monitoring system 102 may monitor oxygen saturation (SpO₂), perfusion index (PI), pulse rate (PR), hemoglobin count, and/or other parameters. An embodiment of a patient monitoring system according to the present

disclosure is capable of measuring and displaying total hemoglobin trending data and preferably is capable of conducting data analysis as to the total hemoglobin trending.

FIG. 2 illustrates details of an embodiment of a patient monitoring system 100 in a schematic form. Typically a sensor 106 includes energy emitters 216 located on one side of a patient monitoring site 218 and one or more detectors 220 located generally opposite. The patient monitoring site 218 is usually a patient's finger (as pictured), toe, ear lobe, or the like. Energy emitters 216, such as LEDs, emit particular wavelengths of energy through the flesh of a patient at the monitoring site 218, which attenuates the energy. The detector(s) 220 then detect the attenuated energy and send representative signals to the patient monitor 102.

Specifically, an embodiment of the patient monitor 102 includes processing board 222 and a host instrument 223. The processing board 222 includes a sensor interface 224, a digital signal processor (DSP) 226, and an instrument manager 228. In an embodiment of the disclosure, the processing board also includes a fast Fourier transform (FFT) module 232. In an embodiment, the FFT module 232 can comprise a special-purpose processing board or chip, a general purpose processor running appropriate software, or the like. The FFT module 232 may further be incorporated within the instrument manager 228 or be maintained as a separate component (as illustrated in FIG. 2).

The host instrument typically includes one or more displays 108, control buttons 110, a speaker 112 for audio messages, and a wireless signal broadcaster 234. Control buttons 110 may comprise a keypad, a full keyboard, a track wheel, and the like. Additionally embodiments of a patient monitor 102 can include buttons, switches, toggles, check boxes, and the like implemented in software and actuated by a mouse, trackball, touch screen, or other input device.

The sensor interface 224 receives the signals from the sensor 106 detector(s) 220 and passes the signals to the DSP 226 for processing into representations of physiological parameters. These are then passed to the instrument manager 228, which may further process the parameters for display by the host instrument 223. In some embodiments, the DSP 226 also communicates with a memory 230 located on the sensor 106; such memory typically contains information related to the properties of the sensor that may be useful in processing the signals, such as, for example, emitter 216 energy wavelengths. The elements of processing board 222 provide processing of the sensor 106 signals. Tracking medical signals is difficult because the signals may include various anomalies that do not reflect an actual changing patient parameter. Strictly displaying raw signals or even translations of raw signals could lead to inaccurate readings or unwarranted alarm states. The processing board 222 processing generally helps to detect truly changing conditions from limited duration anomalies. The host instrument 223 then is able to display one or more physiological parameters according to instructions from the instrument manager 228, and caregivers can be more confident in the reliability of the readings.

In an embodiment, the patient monitor 102 keeps track of total hemoglobin data over a period of time, such as a few minutes, a few hours, a day or two, or the like. It is important to monitor total hemoglobin over a range of time because it has been discovered that hemoglobin fluctuates over time. In an embodiment, the instrument manager may include a memory buffer 234 to maintain this data for processing throughout a period of time. Memory buffer 234 may include RAM, Flash or other solid state memory, magnetic or optical disk-based memories, combinations of the same or

the like. The data for total hemoglobin over a period of time can then be passed to host instrument 223 and displayed on display 108. In an embodiment, such a display may include a graph such as that illustrated by FIG. 3. FIG. 3 illustrates a sample tHb trend graph measuring tHb in g/dL over a period of approximately 80 minutes. In an embodiment, a patient monitor 102 may periodically or continuously update the total hemoglobin display to show the previous hour, previous 90 minutes, or some other desirable time period.

Displaying a current total hemoglobin count, as well as data for a prior time period helps allow a caregiver to determine if the current count is within a normal range experienced by the individual patient. It has also been found that the variations in total hemoglobin count are generally cyclic. It is preferable to display a time period that encompasses at least one complete tHb cycle. As such, a caregiver will be quickly able to see if a total hemoglobin count has fallen above or below the patient's general cyclic range. Additionally, the caregiver may also be able to see if the patient's total hemoglobin count is rising or falling abnormally.

In an embodiment, the trending of the total hemoglobin is additionally or alternatively analyzed through, for example, a frequency domain analysis to determine patterns in the patient hemoglobin fluctuation. Total hemoglobin data from the instrument manager 228 or its memory buffer 234 is passed to the FFT module 232, in an embodiment, to accomplish such an analysis. The FFT module uses one of a number of fast Fourier transform algorithms to obtain the frequencies of various total hemoglobin readings. The resulting data can be graphed and displayed by the host instrument 223's display(s) 108, as shown by example in FIG. 4.

In an embodiment, both total hemoglobin graphs and frequency domain analysis can be displayed on a single patient monitor display 108. In an embodiment, a button 110 or other control allows switching between two such display states. In other embodiments, the display 108 may change automatically, such as periodically or based on a specific event, such as an abnormal change in a patient's total hemoglobin count.

The frequency domain analysis can determine a specific patient signature for a patient, in an embodiment, because the frequency variations have been found to be unique or semi-unique between different patients. As such, a portion of the memory buffer 234 may maintain a baseline total hemoglobin frequency data set for comparison to later data readings from the sensor 106. Changes in the frequency analysis may indicate a change in a monitored patient's status. In such an embodiment, a baseline reference graph and a more current frequency domain analysis may be graphed together on a single graph display, on multiple proximate graph displays or display windows, or the like to allow caregivers to recognize changes in the patient's hemoglobin levels over time. For example, in an embodiment, a single graph may include both sets of data graphed in different colors, such as a blue baseline reading and a green more current reading frequency analysis. Variations between the two may, in an embodiment, trigger an alert or an alarm if they reach a certain threshold. Such an alert or alarm may be audible and output through audible indicator 112 and/or may alter the display 108. The alarm or alert may incorporate changing colors, flashing portions of a screen, text or audible messages, audible tones, combinations of the same or the like.

FIG. 5 illustrates an embodiment of a method of obtaining, analyzing, and displaying total hemoglobin data for

patient status and analysis as generally described herein. Starting with block 540, energy is transmitted through patient tissue at a measurement site, generally by a sensor 106. The patient tissue attenuates the energy which is then detected at block 542. The detected signals are evaluated to determine a current total hemoglobin count (block 546). This step may include, in an embodiment, filtering noise from the signals, filtering errant readings, and the like. In an embodiment, a buffer stores the total hemoglobin readings for a period of time in (block 548). This allows the patient monitor to display trending data, display the total hemoglobin readings for a period of time, rather than just relatively instantaneous readings, and the like. In an embodiment, the patient monitor analyzes the set of buffered total hemoglobin readings using a Fourier transform, such as a discrete Fourier transform, or more preferably one of many suitable fast Fourier transform algorithms (block 550). This analysis decomposes the sequence of total hemoglobin readings into components of different frequencies. Displaying this frequency analysis (block 552) can help caregivers identify changing conditions for a patient that may indicate worsening or improving health conditions.

The display of trending total hemoglobin data and caregiver understanding of a patient's condition that comes with understanding such a display are important uses. The automatic interpretation of this data into patient care is another. FIGS. 6 and 7 illustrate exemplary systems incorporating uses for patient monitoring of a patient's total hemoglobin in treating the patient for various ailments or injuries. For example, studies have shown that one of the most recurrent problems of hemodialysis is anemia—a condition in which a patient's blood lacks sufficient red blood cells. Dialysis-dependent patients can improve their quality of life by maintaining an adequate hemoglobin level. To this end, it may be advantageous to link the patient monitoring of hemoglobin levels to a dialysis machine to provide hemoglobin level feedback, allowing the dialysis machine to act intelligently and help regulate hemoglobin levels during dialysis. An embodiment of such a system is illustrated in FIG. 6.

As illustrated, an embodiment of the patient monitor 102 is set up in much the same way as described above, with a cable 104 attaching to a noninvasive sensor 106 located proximal to a patient measurement site, such as the finger shown in FIG. 6. An additional cable 660 connects dialysis machine 662 to the patient monitor 102. The dialysis machine 662 generally includes an arterial line 664 and a venous line 664, each of which end in needles 668 for insertion into a patient's artery and vein, respectively. Dialysis machine 662 may then operate at least in part based on hemoglobin levels of the patient as determined by the patient monitor 102. As the hemoglobin levels naturally change, in an embodiment, patient monitor 102 may simply signal the dialysis machine when hemoglobin levels are approaching or have fallen outside of maximum and minimum ranges. Alternatively, the patient monitor 102 may pass hemoglobin level readings to the dialysis machine 662 continuously, at generally periodic intervals, upon changes in hemoglobin level readings, or the like. The dialysis machine 662 can then alter its processing of the blood, inject appropriate amounts of drugs, turn off or on, or otherwise change states or processes based in whole or in part on the hemoglobin levels detected.

FIG. 7 illustrates another exemplary use for patient monitoring of a patient's total hemoglobin in treating the patient for various ailments or injuries. In the embodiment shown, an IV fluid bag is connected to the patient monitor by tubing

772. The patient monitor **102** then incorporates a venous line **664** ending in a needle **668** for insertion into a patient's vein. IVs are often used to administer nutrition, drugs, blood, plasma, and other transfusions, and the like. The patient monitor **102** may thus incorporate a device to control the rate or amount of IV fluid administered to a patient. In the embodiment illustrated, the patient monitor controls the administration, at least in part, based on the hemoglobin levels detected.

As one example, erythropoiesis-stimulating agents (ESAs) are drugs that can help encourage the production of red blood cells. The patient monitor **102** can use the hemoglobin readings of a monitored patient to control the administration of such a drug through an IV. Similarly, the patient monitor can increase the transfusion of blood to a patient if, for example, hemoglobin levels fall below the normal range of hemoglobin. Monitoring the hemoglobin levels with knowledge of the natural fluctuation of those levels in the patient can help reduce the amounts of drugs administered, blood or other fluids transfused, and the like. For example, the patient monitor can help keep the hemoglobin levels in a normal range rather than trying to maintain an exact level, which may lead to less efficient treatment. For example, a falling hemoglobin level may still be within natural limits and may rise without additional treatment. In an embodiment, the patient monitor **102** can withhold treatment in such a situation and provide additional treatment if the hemoglobin is predicted to fall outside or is outside normal limits. This can help reduce the usage of costly treatments and/or conserve those in short supply. Additionally, it may be important to limit usage of a drug due to increased risks of side effects, drug dependency, or the like.

Of course, the foregoing are exemplary only and any IV administered drug, blood, plasma, nutrition, other fluid, or the like that has a tendency to affect hemoglobin levels can be administered and controlled in this manner. One of skill in the art will also understand that the patient monitor and administration devices can be incorporated in a single unit (such as illustrated in FIG. 7) or occur in wired or wirelessly communicating separate units (such as illustrated in FIG. 6) in various embodiments. Administration devices can include not only IV controlling units and dialysis machines as discussed, but other devices designed to aid in providing something of need to a patient. Similarly, other patient parameters detected by sensor **106** and calculated by patient monitor **102** may also be passed to administration devices or used internally to affect the administration of drugs, blood, nutrition, other fluid, or the like.

Hemoglobin concentration can be affected by a variety of different physiological factors, including abnormalities of the hemoglobin or the red blood cells that carry the hemoglobin, vessel fluid volume changes or other physiological factors. For example, fluid volume in the vessel is constantly changing as fluid can enter or exit the blood cell through the arteries. As concentration of hemoglobin is generally determined by the amount of hemoglobin divided by the amount of volume of fluid in the blood cells, changes in the vessel volume will directly affect the hemoglobin concentration. For example, standing up or changing position can alter the hydrostatic affect of blood pressure on the arteries, potentially changing the concentration of total hemoglobin in the blood.

Another exemplary use for patient monitoring of a patient's total hemoglobin involves monitoring these various physiological factors that can affect the total hemoglobin concentration and determining when variations are normal or can indicate physiological problems or abnormalities. For

example, in some embodiments differences in the fluid volume based on permeability or other factors that affect the vessel fluid volume can have an effect on the total hemoglobin concentration in the blood. In one embodiment, fluctuations in the permeability of the blood vessels and ion balance can cause the influx our excretion of fluid from the blood vessels causing changes in the hemoglobin concentration. These changes can be normal or periodic changes that can be identified as such through specific algorithms or can be abnormal changes in the permeability that can trigger an alarm during patient monitoring. Also, changes in the rate of hemoglobin production over time can have an effect on the hemoglobin concentration that can be monitored or taken into account. Further, changes in the spleen function, including in its capacity to remove dead or damages red blood cells from the blood stream, can produce changes in the total hemoglobin concentration.

Another exemplary use for patient monitoring of a patient's total hemoglobin related to physiological processes or abnormalities involves determining an abnormality or type of hemoglobin that can be present in the blood. For example, in some embodiments, certain types or deformations of the hemoglobin or red blood cells may cause the total hemoglobin value in a patient's arteries to vary with time or vary locally in certain parts of the arteries. For example, sickle cell anemia, a condition characterized by sickle shaped red blood cells, may cause red blood cells to clump together. This or other abnormalities in the cells may cause local or global variation in the amount of hemoglobin, as a clump of red blood cells may be more dense than a dispersed group of red blood cells, or alter the permeability or ability of the red blood cells to enter the micro circulation. Sometimes, the red blood cells of a person with sickle cell anemia can have difficulty deforming and therefore fitting through vessels in the micro circulation. This can cause them to bunch up near the smaller blood vessels in the micro circulation and change the concentration of hemoglobin. Therefore, this abnormality may exhibit a somewhat normal or predictable cyclical change or frequency of variation in the hemoglobin of the blood and therefore monitoring the total hemoglobin may aid in the diagnosis of these types of conditions. Also, it can cause the hemoglobin concentration to be abnormally low or high in some cases. In other embodiments, various other red blood cell or hemoglobin abnormalities may cause regular variation in the total hemoglobin that may be used to assist in the diagnosis of these ailments, including for example, Thalassemia.

Various data can be collected from patients with hemoglobin and red blood cell abnormalities to determine or identify any potential signatures or unique or predictable fluctuations in the hemoglobin levels. This data can be used to diagnose patients by comparing a patient's hemoglobin variability to that of data from normal patients and from patients with certain abnormalities. This can provide a non-invasive method of screening for certain abnormalities that may otherwise require invasive blood testing by drawing blood and testing it in the lab or other time consuming and costly methods of analysis. Also, knowledge about the physiological processes that cause normal variation in the hemoglobin concentration can increase the ability to screen normal from abnormal variation in the hemoglobin by analyzing total hemoglobin data over time.

For example, in an embodiment, a caregiver can set up the patient monitor **102** to obtain signals from a patient representative of the total hemoglobin of the patient over time. The patient monitor **102** can then send the signals to the processing board **222** to be analyzed and processed to

determine whether or not the signals or data from the patient is representative of a patient with a hemoglobin abnormality such as sickle cell anemia or are indicative of normal variation in the hemoglobin concentration. In an embodiment, the signals can be compared to existing data from patients that have been confirmed to have sickle cell anemia to determine if the condition likely exists in the current patient based on similarity of hemoglobin variability. In another embodiment, the signals can be filtered and processed to look for certain signal components that may be indicative of an abnormality such as sickle cell anemia.

Although the foregoing has been described in terms of certain specific embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. Moreover, the described embodiments have been presented by way of example only, and are not intended to limit the scope of the disclosure. Indeed, the novel methods and systems described herein may be embodied in a variety of other forms without departing from the spirit thereof. Accordingly, other combinations, omissions, substitutions, and modifications will be apparent to the skilled artisan in view of the disclosure herein. For example, various functions described as occurring in FFT module 232 may be incorporated within other portions of the processing board 222. Similarly, a patient monitor 102 may not have a distinct processing board 222 and host instrument 223; instead, the various functions described herein may be accomplished by different components within a patient monitor 102 without departing from the spirit of the disclosure. Thus, the present disclosure is not limited by the preferred embodiments, but is defined by reference to the appended claims. The accompanying claims and their equivalents are intended to cover forms or modifications as would fall within the scope and spirit of the disclosure.

What is claimed is:

- 1. A patient monitoring system comprising:
 - a light emitter configured to emit energy into a tissue site of a patient;
 - a detector configured to detect a response from the tissue site responsive to the emission of energy into the tissue site of the patient; and
 - one or more hardware processors configured to:
 - determine a plurality of hemoglobin concentration measurements over time for the tissue site based on the detected response;
 - perform a frequency transform on the plurality of hemoglobin concentration measurements; and
 - display a plurality of frequency components on a display screen of a patient monitor based on the performed frequency transform of the plurality of hemoglobin concentration measurements.
- 2. The patient monitoring system of claim 1, wherein the one or more hardware processors are further configured to determine an oxygen saturation of blood flow into the tissue site based on the detected response.
- 3. The patient monitoring system of claim 2, wherein the oxygen saturation is displayed on the display screen.

4. The patient monitoring system of claim 1, wherein the one or more hardware processors are further configured to determine a trend in total hemoglobin based on the frequency transform.

5. The patient monitoring system of claim 4, wherein the one or more hardware processors are further configured to provide an indication of the trend to a dialysis management system.

6. The patient monitoring system of claim 4, wherein the one or more hardware processors are further configured to provide an indication of the trend to an infusion management system.

7. The patient monitoring system of claim 4, wherein the one or more hardware processors are further configured to determine hemoglobin abnormalities based on the trend in total hemoglobin.

8. The patient monitoring system of claim 1, wherein the one or more hardware processors are further configured to determine signal components from the frequency transformed hemoglobin measurements and identify a patient physiological condition based on the determined signal components.

9. A patient monitoring method comprising:
 emitting energy into a tissue site of a patient;
 detecting a response from the tissue site responsive to the emission of energy into the tissue site of the patient;
 determining a plurality of hemoglobin concentration measurements over time for the tissue site based on the detected response;
 performing a frequency transform on the plurality of hemoglobin concentration measurements; and
 displaying a plurality of frequency components on a display screen of a patient monitor based on the performed frequency transform of the plurality of hemoglobin concentration measurements.

10. The patient monitoring method of claim 9, further comprising determining an oxygen saturation of blood flow into the tissue site based on the detected response.

11. The patient monitoring method of claim 10, wherein the oxygen saturation is displayed on the display screen.

12. The patient monitoring method of claim 9, further comprising determining a trend in total hemoglobin based on the frequency transform.

13. The patient monitoring method of claim 12, further comprising providing an indication of the trend to a dialysis management system.

14. The patient monitoring method of claim 12, further comprising providing an indication of the trend to an infusion management system.

15. The patient monitoring method of claim 12, further comprising determining hemoglobin abnormalities based on the trend in total hemoglobin.

16. The patient monitoring method of claim 12, further comprising determining signal components from the frequency transformed hemoglobin measurements and identify a patient physiological condition based on the determined signal components.

* * * * *