



(86) Date de dépôt PCT/PCT Filing Date: 1998/12/04

(87) Date publication PCT/PCT Publication Date: 1999/06/10

(45) Date de délivrance/Issue Date: 2003/12/02

(85) Entrée phase nationale/National Entry: 2000/05/11

(86) N° demande PCT/PCT Application No.: US 1998/025850

(87) N° publication PCT/PCT Publication No.: 1999/027849

(30) Priorité/Priority: 1997/12/04 (60/067,499) US

(51) Cl.Int.⁶/Int.Cl.⁶ A61B 5/00

(72) Inventeurs/Inventors:

BATMAN, CAROL JANE, US;

BYRD, NANCY KENNEDY, US;

DISHOP, TIMOTHY J., US;

HENDERSON, LES G., US;

HOPKINSON, PATRICIA A., US;

MOAK, STEPHEN E., US;

PARKER, JAMES R., US;

...


(73) Propriétaire/Owner:

ROCHE DIAGNOSTICS CORPORATION, US

(74) Agent: OGILVY RENAULT


(54) Titre : METHODE DE CONFIGURATION D'UN INSTRUMENT MANUEL

(54) Title: METHOD OF CONFIGURING A HAND-HELD INSTRUMENT

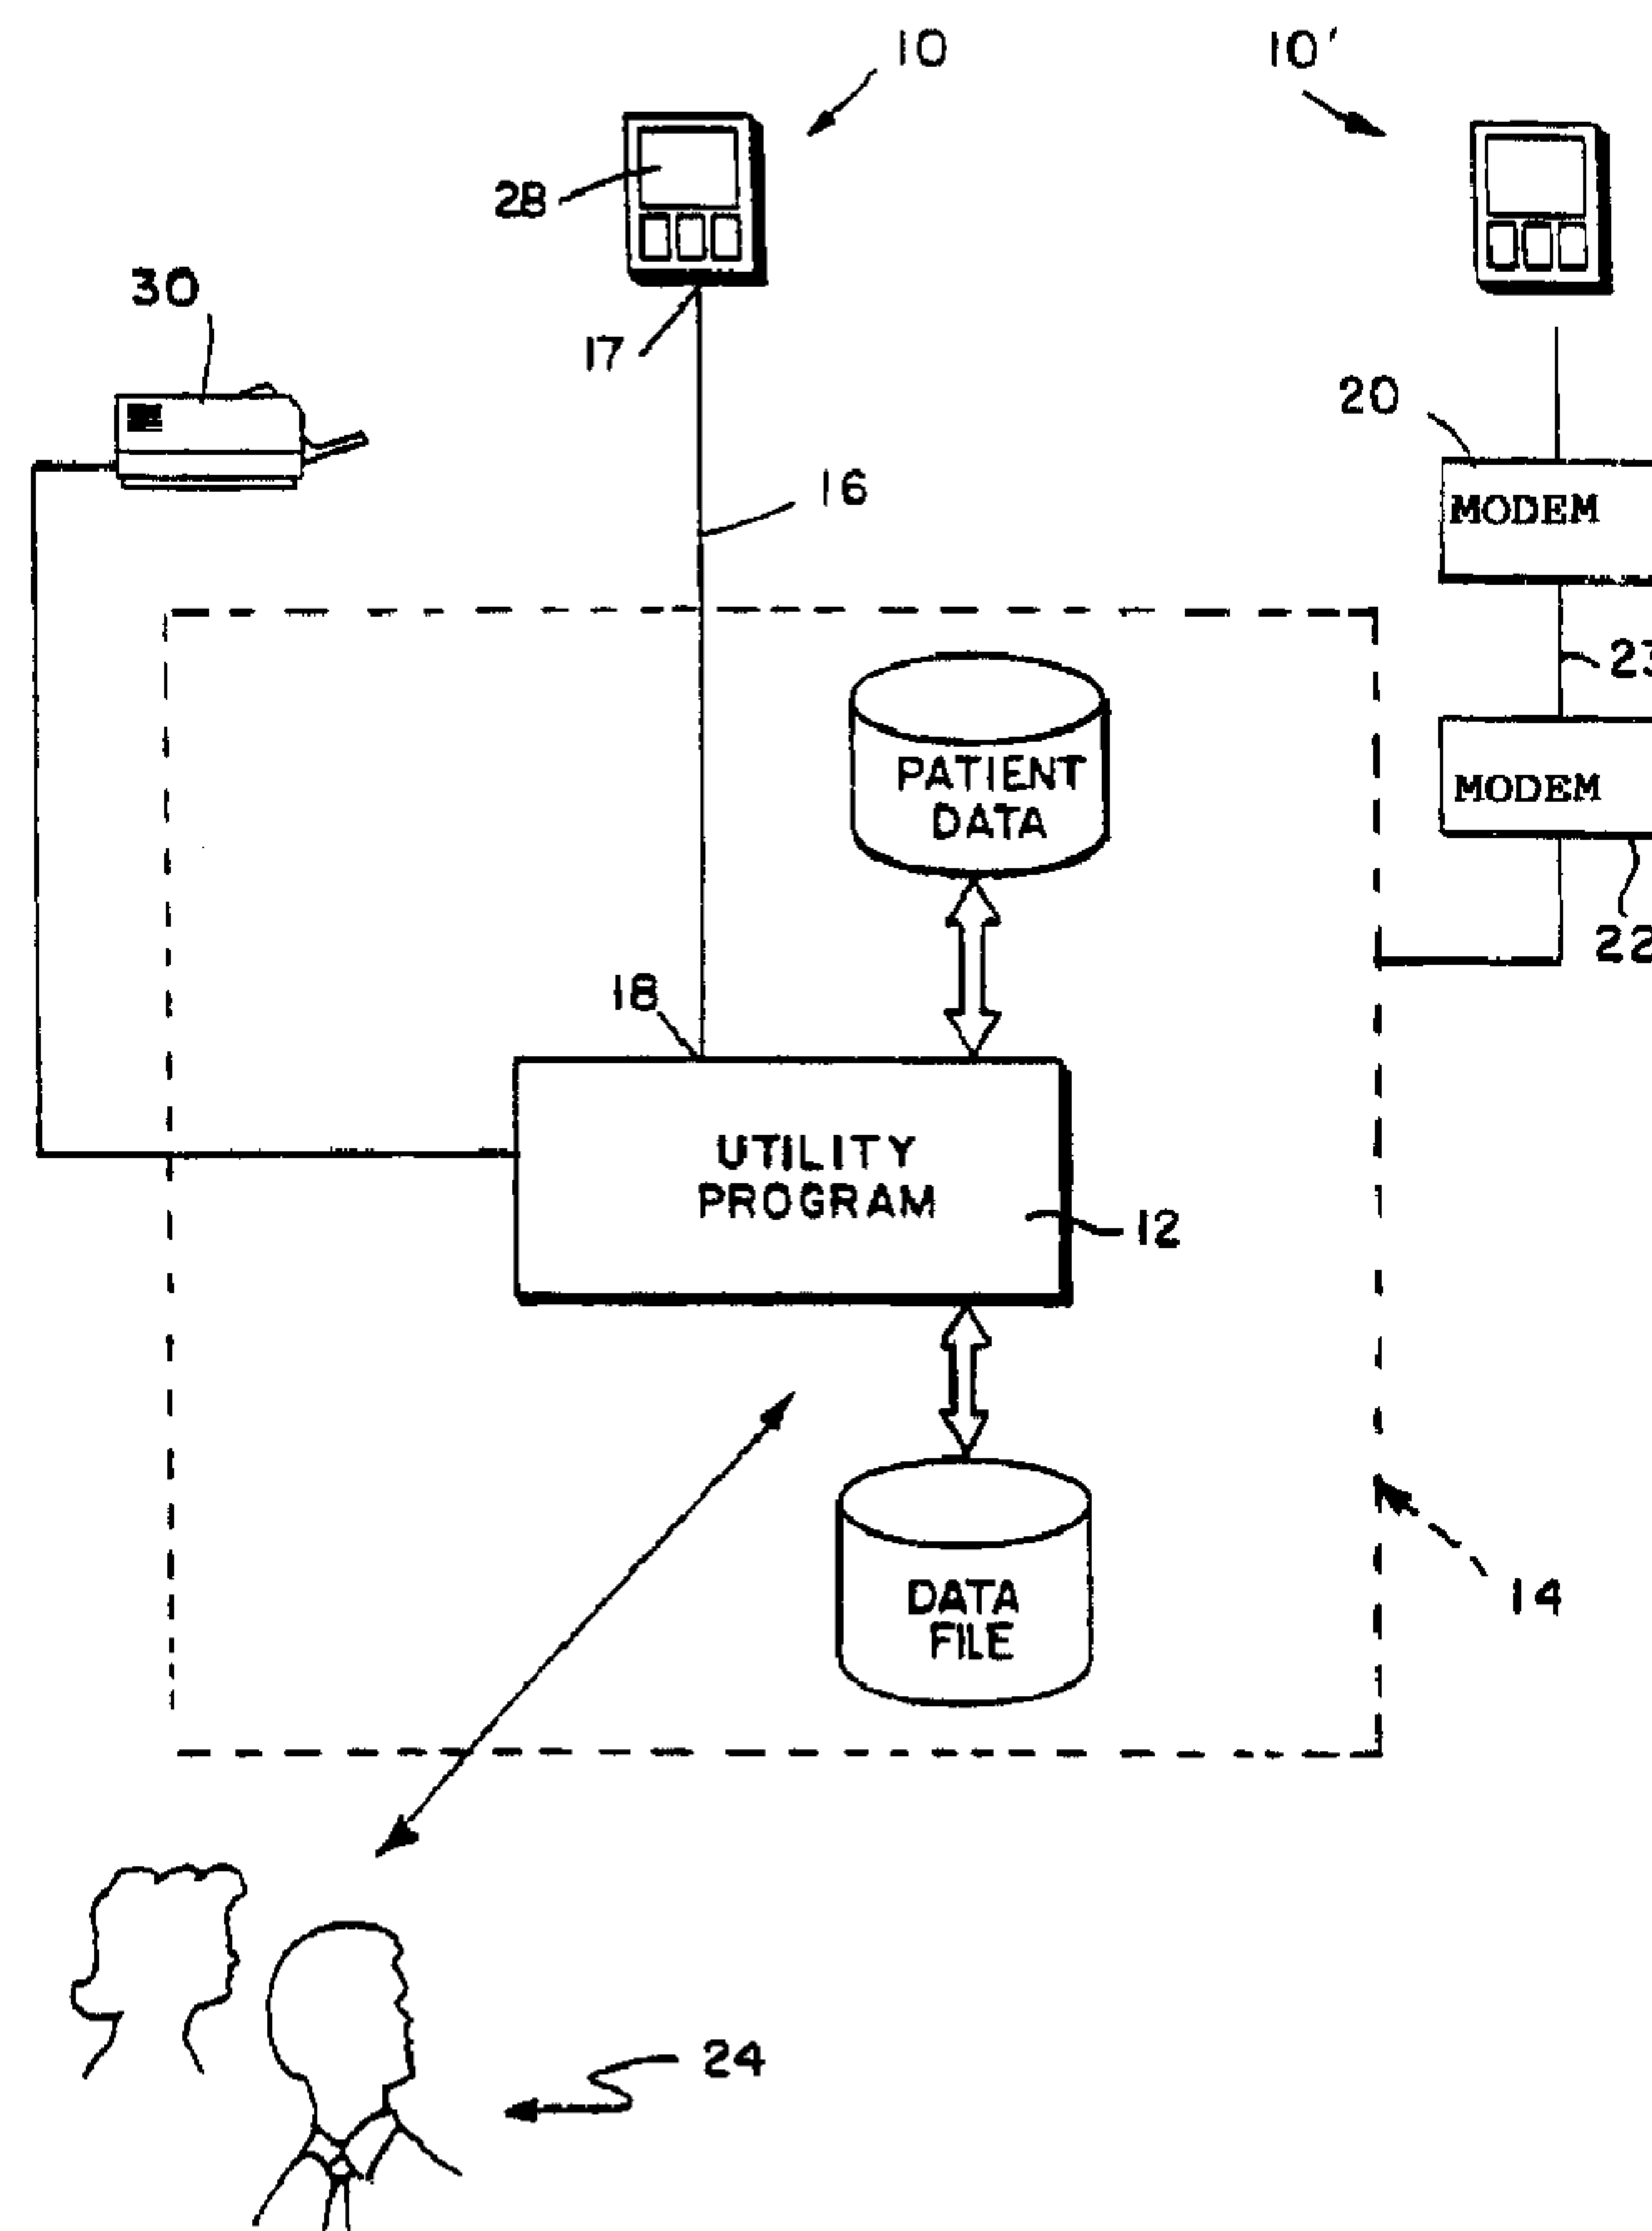

(57) Abrégé/Abstract:

A method of configuring a hand-held instrument (10) for determining the concentration of a medically significant component of a body fluid or a control comprises providing a configuring computer (14) having a first port (18) for transmitting instructions and

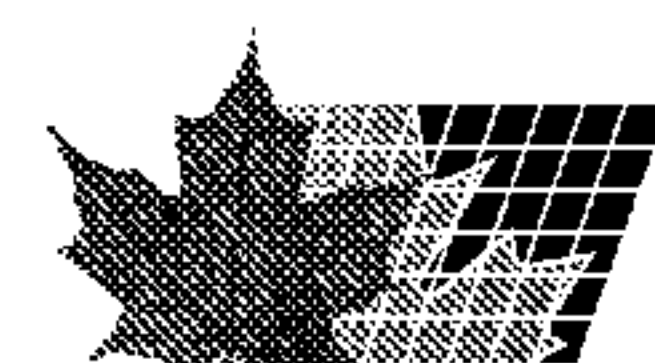

(72) **Inventeurs(suite)/Inventors(continued):** POLASKI, FRANK M., US; SHEARER, ATWELL R., US; TETZLAFF, TRACY L., US; SLY, LYNNE DENISE, US; KLEM, KURT GERARD, US

(57) **Abrégé(suite)/Abstract(continued):**

data for configuring the instrument (10), providing on the instrument (10) a second port (17) for receiving the instructions and data from the configuring computer (14), coupling the first port (18) to the second port (17), transmitting instructions and data to configure the instrument (10) from the first port (18), receiving the instructions and data at the second port (17), and configuring the instrument (10) according to the instructions and data transmitted from the first port (10) and received at the second port (17).

**PCT**WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61B 5/00		A1	(11) International Publication Number: WO 99/27849
			(43) International Publication Date: 10 June 1999 (10.06.99)
(21) International Application Number: PCT/US98/25850		(74) Agent: CONARD, Richard, D.; Barnes & Thornburg, 11 South Meridian Street, Indianapolis, IN 46204 (US).	
(22) International Filing Date: 4 December 1998 (04.12.98)			
(30) Priority Data: 60/067,499 4 December 1997 (04.12.97) US		(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).	
(71)(72) Applicants and Inventors: BATMAN, Carol, Jane [US/US]; 5318 Ochs Avenue, Indianapolis, IN 46254 (US). BYRD, Nancy, Kennedy [US/US]; 9758 Chaldean Circle, Fishers, IN 46038 (US). DISHOP, Timothy, J. [US/US]; 4924 Long Canon Place, Fort Wayne, IN 46804 (US). DZADO, Michael, Daniel [US/US]; 1754 CR 60, Garrett, IN 46738 (US). HENDERSON, Les, G. [US/US]; 6345 East 226th Street, Cicero, IN 46034 (US). HOPKINSON, Patricia, A. [US/US]; HRC #1, Box 11, Lake Placid, NY 12946 (US). MOAK, Stephen, E. [US/US]; 411 Inwood Drive, Fort Wayne, IN 46815 (US). PARKER, James, R. [US/US]; 10807 Weston Drive, Carmel, IN 46032-9321 (US). POLASKI, Frank, M. [US/US]; 10732 Current Cove, Fort Wayne, IN 46845 (US). SHEARER, Atwell, R. [US/US]; P.O. Box 165, Rome City, IN 46784 (US). TETZLAFF, Tracy, L. [US/US]; Apartment 106, 5607 Elmer Street, Pittsburgh, PA 15232 (US).		Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>	

(54) Title: INSTRUMENT SETUP UTILITY PROGRAM

(57) Abstract

A method of configuring a hand-held instrument (10) for determining the concentration of a medically significant component of a body fluid or a control comprises providing a configuring computer (14) having a first port (18) for transmitting instructions and data for configuring the instrument (10), providing on the instrument (10) a second port (17) for receiving the instructions and data from the configuring computer (14), coupling the first port (18) to the second port (17), transmitting instructions and data to configure the instrument (10) from the first port (18), receiving the instructions and data at the second port (17), and configuring the instrument (10) according to the instructions and data transmitted from the first port (10) and received at the second port (17).

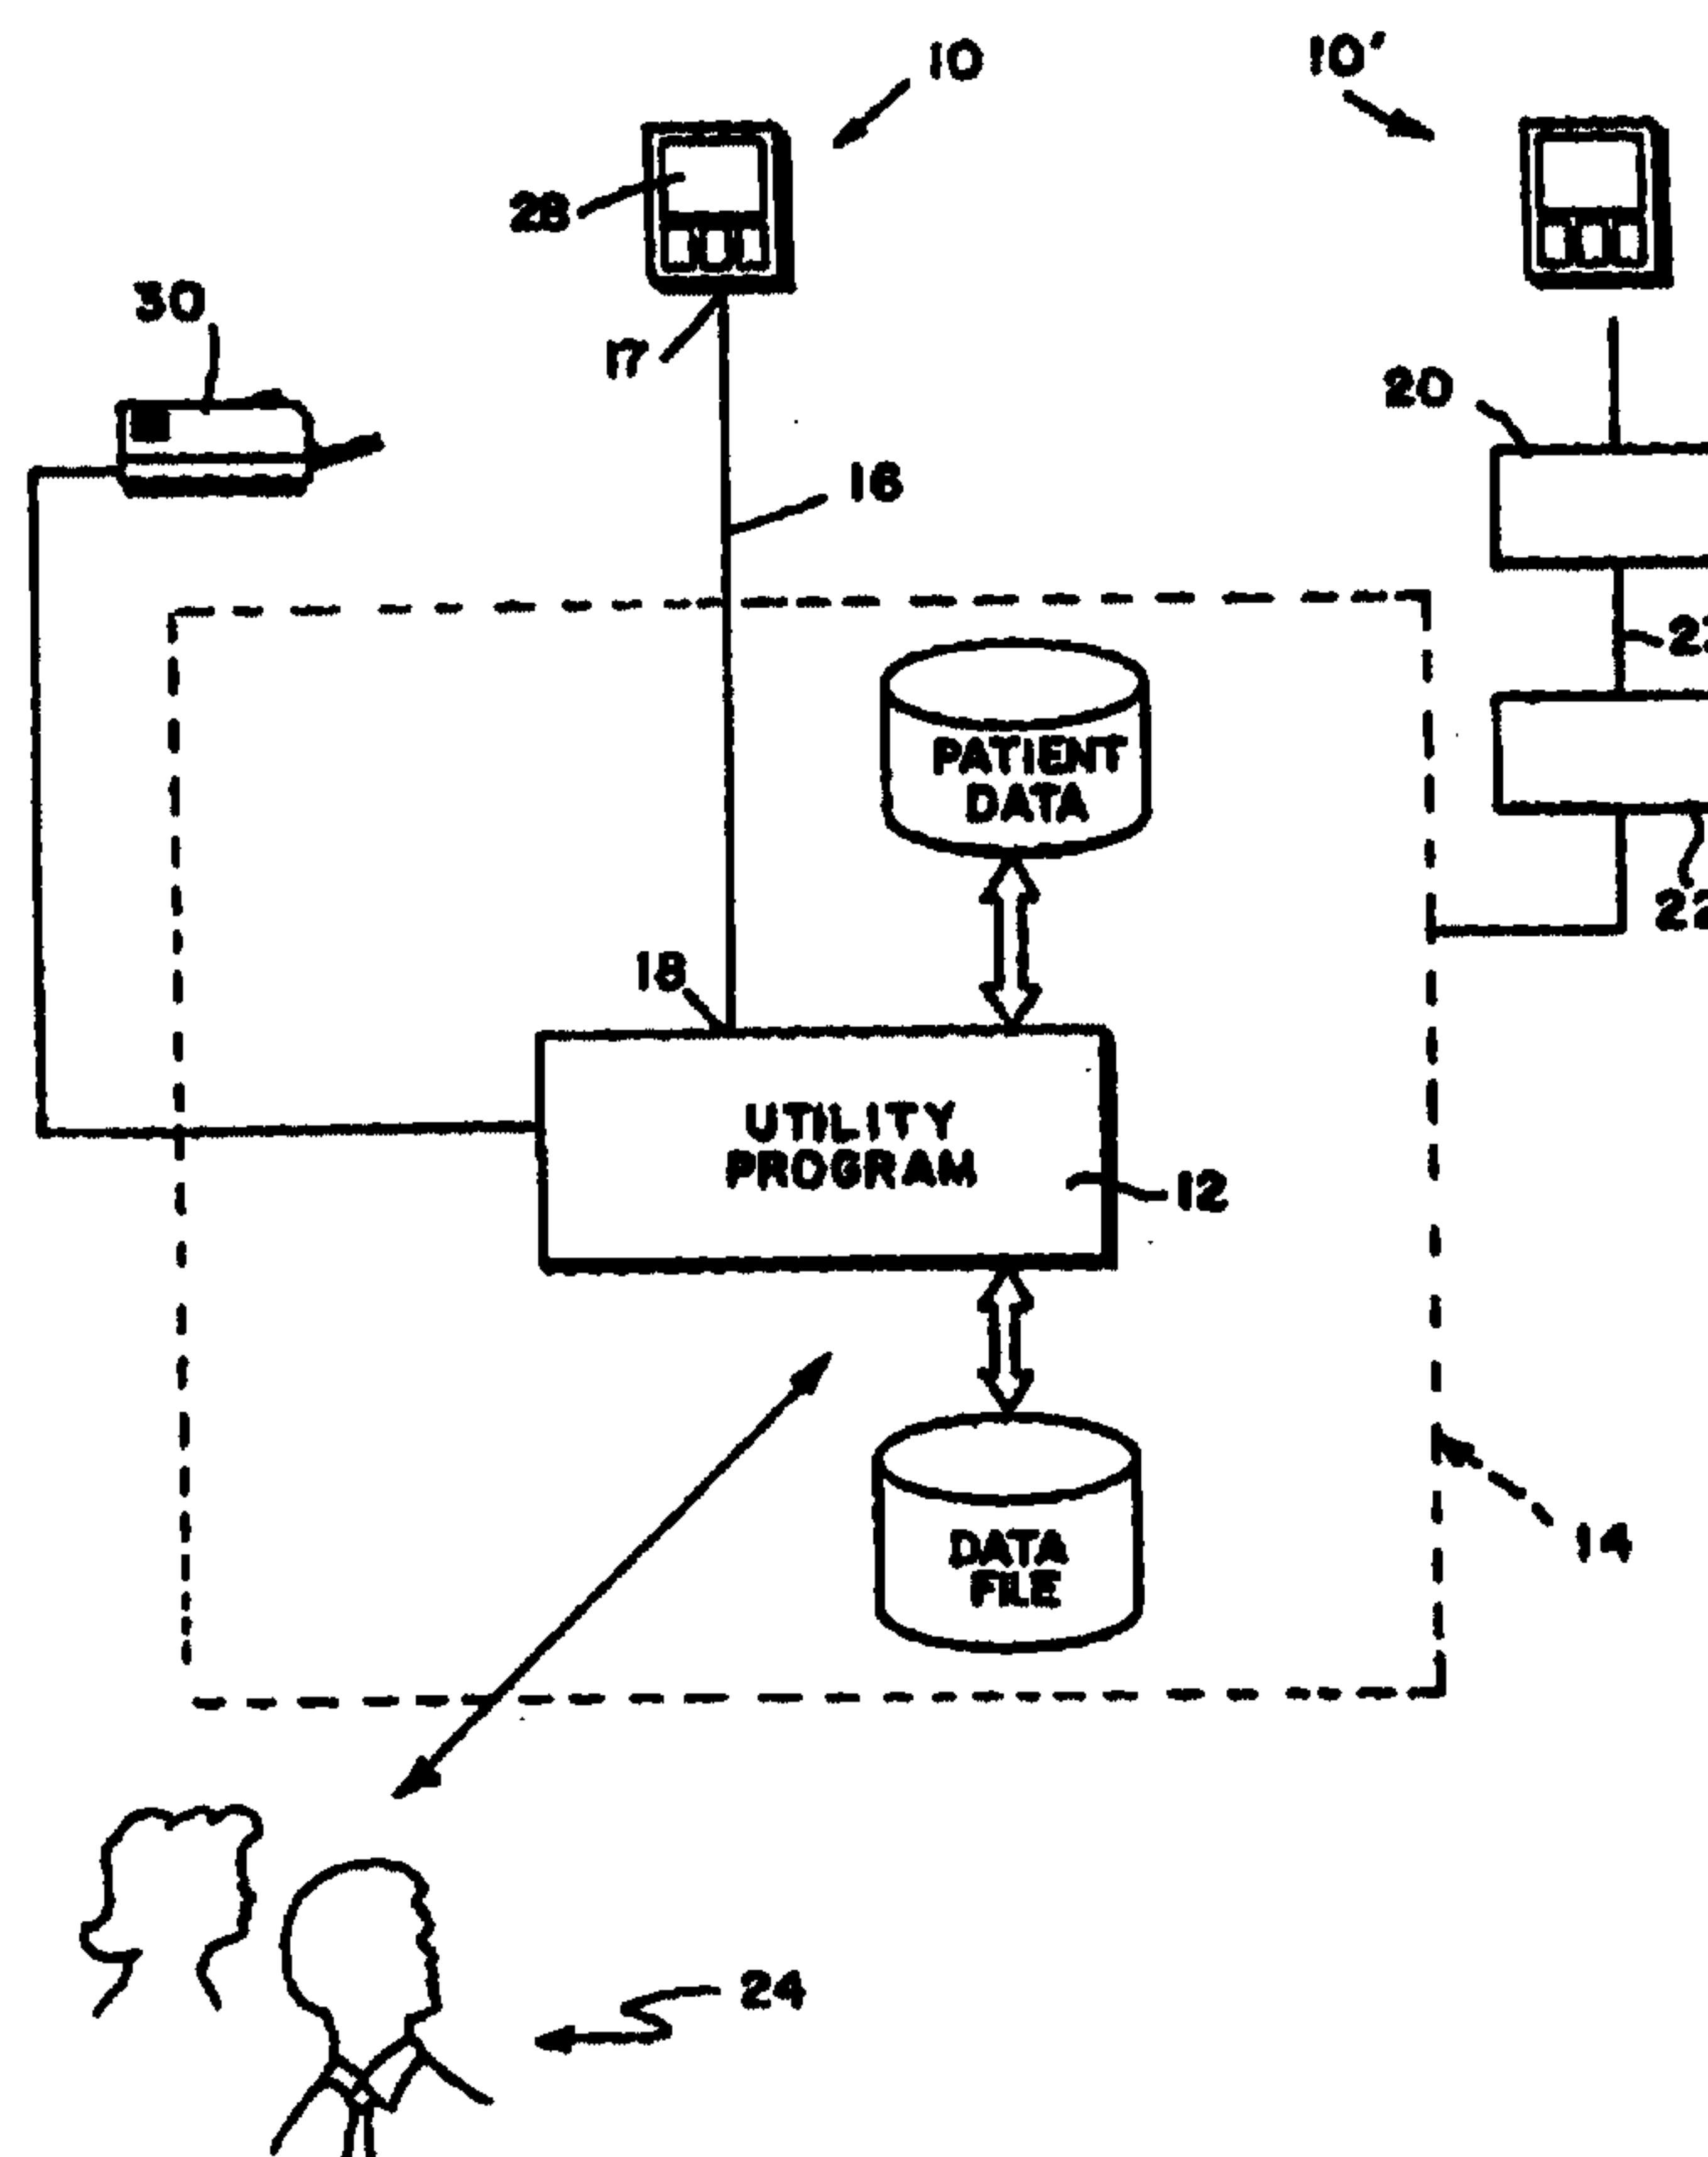

METHOD OF CONFIGURING A HAND-HELD INSTRUMENT**Field of the Invention**

This invention relates to a utility program useful in, for example, the setup of, and the communication with, instruments of the general type described in

5 WO 99/28736.

Disclosure of the Invention

A method of configuring a hand-held instrument for determining the concentration of a medically significant component of a body fluid or a control comprises the steps of providing a configuring computer having a first port for
10 transmitting at least one of instructions and data for configuring the instrument, providing on the instrument a second port for receiving said at least one of instructions and data from the configuring computer, coupling said first port to said second port, transmitting said one of instructions and data to configure said instrument from said first port, receiving said one of instructions and data at said
15 second port, and configuring said instrument according to said one of instructions and data transmitted from said first port and received at said second port.

Illustratively according to the invention, the step of providing a configuring computer having a first port for transmitting at least one of instructions and data for configuring the instrument comprises the step of providing a configuring computer
20 having a first port for transmitting instructions for configuring the instrument.

Further illustratively according to the invention, the step of providing a

-2-

configuring computer having a first port for transmitting at least one of instructions and data for configuring the instrument comprises the step of providing a configuring computer having a first port for transmitting data for configuring the instrument.

Additionally illustratively according to the invention, the hand-held
5 instrument further comprises a display for displaying information related to the determined concentration. The step of transmitting said one of instructions and data to configure said instrument from said first port comprises the step of transmitting said one of instructions and data from said first port to configure said display.

Illustratively according to the invention, the method further comprises
10 the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

Further illustratively according to the invention, the step of transmitting one of instructions and data concerning determined concentration of a medically
15 significant component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

Additionally illustratively according to the invention, the method further comprises updating a file in the computer with the transmitted data.

20 Illustratively according to the invention, the steps of transmitting said one of instructions and data to configure said instrument from said first port and receiving said one of instructions and data at said second port comprise transmitting said one of instructions and data through a fiber optic coupler from said first port to said second port.

25 Further illustratively according to the invention, the instrument comprises an instrument for determining the glucose concentration of blood, a blood fraction or a control.

Additionally illustratively according to the invention, the step of transmitting said one of instructions and data concerning determined concentration of a
30 medically significant component of a body fluid from the second port to the first port comprises the step of transmitting said one of instructions and data concerning determined concentration of a medically significant component of a body fluid via a

- 3 -

modem from the second port to the first port.

Brief Description of the Drawings

The invention may best be understood by referring to the following detailed descriptions of illustrative embodiments and the accompanying drawings. In the drawings:

5 Fig. 1 illustrates a diagram of a system implementing a utility program according to the present invention;

 Fig. 2 illustrates installation of a utility program according to the present invention where the program is distributed on one or more disks containing the program in one or more languages; and,

10 Figs. 3-60 illustrate various screens displayed during the running of a utility program according to the invention.

Detailed Descriptions of Illustrative Embodiments

 This invention relates to a utility program useful in, for example, the setup of, and communication with, instruments of the general type described in WO 99/28736. Fig. 1
15 illustrates diagrammatically a system implementing the utility program 12 of the present invention. Setup of such an instrument 10 is handled by a portion of the program 12 sometimes referred to hereinafter as a Meter Setup Manager through a docking station provided for the instrument 10 on a personal computer (PC) 14. Communication between the docked instrument 10 and the PC 14 is coupled through a serial cable 16 such as, for example,
20 a fiber optic connector, from a port 17 on instrument 10 to a port 18 on the PC 14. Communication with a remote instrument 10', such as for the downloading of test results from storage on board the instrument 10' to the PC 14, is handled by a portion of the program sometimes referred to hereinafter as a Phone-In Manager. Phone-In Manager is conducted via telephone modems 20, 22 at the remote instrument 10' site and the PC 14.

25 Installation of the program 12, where the program is distributed on one or more disks containing the program in one or more languages, for example, is achieved as illustrated in Fig. 2. The user 24 may be asked to enter certain security information, for example, to verify the user 24's access to the PC 14 on which the

-4-

program 12 is loaded. A program 12 screen displays a list of utility languages from which the user 24 selects one. Illustratively, the user 24 will have to reinitialize the program 12 if, after selection of a utility language, the user 24 decides to select a different utility language.

5 Meter Setup Manager

Certain functions of the program can be performed only while an instrument of the general type discussed above is connected through, for example, a serial cable 16 rather than through modems 20, 22 and phone line 23, to the PC 14. A Meter Setup Manager icon, for example, an illustration of the instrument 10, will
10 appear on one of the early screens. Once the user 24 clicks on the Meter Setup Manager icon, a copyright screen will appear briefly and will be followed by a "Welcome" screen illustrated in Fig. 3. The "Welcome" screen includes a list of tasks the Meter Setup Manager is capable of performing at the user 24's option. This "Welcome" screen can be deselected at the user 24's option. If the user 24 has
15 deselected this screen, the default task will be initialized. If the user 24 has selected the "Create a Meter Setup" option, a standard Microsoft® Windows® development tool, known as the Wizard™, is launched.

Each screen in the meter setup routine is based on the template illustrated in Fig. 4. As an example of the screens based upon this template, Fig. 5
20 illustrates the "Enter personal information" screen. This screen displays three fields into which the user 24 is directed to enter information pertinent to the patient whose instrument 10 is being set up. The fields are patient name, patient identification, such as, for example, patient number, patient social security number, and so on, and health care provider computer 14 phone number. The next screen, illustrated in Fig. 6, is the
25 "Glucose units/glucose ranges" screen. With this screen, the user 24 sets up the patient's instrument 10's glucose upper limit, glucose lower limit, hypoglycemic limit, and units of glucose measurement, for example, millimoles per liter (mmol/L) or milligrams per deciliter (mg/dL). The next screen, illustrated in Fig. 7, prompts the user 24 to set up the patient's instrument 10 for the type(s) of insulin the patient is to
30 take, for example, REGular, NPH or 90/10, and the dosage increments, for example, tenths of a unit, half units, or whole units.

With the next screen, illustrated with sample data in Fig. 8, the user 24

-5-

is prompted to load into the patient's instrument 10 certain events which the patient is then capable of entering into the patient's diary, which the instrument 10 is equipped to keep. From a library of, for example, 255 events, fifteen are chosen from which the patient may select to enter one in his or her diary with each glucose test result. Some
5 one or more of these may be customized for the patient whose instrument 10 is being set up.

The next screen, illustrated with sample data in Fig. 9, permits the user 24 to load into the patient's instrument 10 schedule control over any twenty-four hour period. A glucose test entry regimen dividing the twenty-four hour day into eight two-
10 to five-hour intervals is the default regimen. This default regimen will be displayed on the screen, and the user 24 will be permitted to edit away from the default settings for the individual patient. Editing is done by clicking on the "Edit" button or by double clicking on any of the time block entries. Once the time block to be edited has been highlighted, its entries are available for edit. The program requires that every minute
15 of the twenty-four hour period be accounted for, and does not permit any minute to be in two different time blocks. As a result, adjusting an entry will typically result in an automatic adjustment of another entry.

Advancing to the next screen, illustrated with sample data in Fig. 10, the information just entered is combined in the "Time block information" screen. The
20 insulin types that were selected in the screen illustrated in Fig. 7 are the ones displayed on the screen illustrated in Fig. 10. If insulin type "None" was selected in connection with the setup illustrated in Fig. 7, no dosage can be selected in connection with the setup illustrated in Fig. 10. If the user 24 does not select an exercise type, he may not enter an exercise duration. The events list contains events which were selected in the
25 events screen. The program does not permit the user 24 to list an event on the screen illustrated in Fig. 10 which was not one of the selected events in Fig. 8.

The screen illustrated in Fig. 11 is the meter setup "Insulin pump profile" screen. This screen contains a schedule list box similar to the time blocks schedule list box illustrated in Fig. 9. The user 24 selects an insulin type, and a start
30 date and time for the insulin pump profile. The profile can contain no less than one time block and no more than twelve. The user 24 can insert or edit a time block from the screen. The user 24 can only delete a time block when the profile contains more

-6-

than one time block.

With reference to Fig. 12, the user 24 may insert a new time block by selecting a time block from the list and selecting the "Insert" button. The user 24 is presented with the option to insert the new time block either before or after the
5 selected time block. The new time block, with a duration of one half hour, is inserted into the schedule list box. The user 24 can edit the start time of the newly added time block by double clicking on its entry in the list box, or by selecting the "Edit" button.

The user 24 can edit a specific insulin pump profile time block by double clicking on its entry in the profile time block list box. See Fig. 13. When this is
10 done, the start time and insulin pump rate for the selected time block can be edited. The user 24 can also edit a time block by highlighting its entry in the time block list box and selecting the "Edit" button. All times must be part of some time block, so the user interface does not permit gaps between time blocks. Nor can time blocks overlap. Setting the start time of one block automatically adjusts the end time of the previous
15 time block to end one minute before. The user 24 can also delete a specific profile time block by highlighting its entry in the profile list box and selecting the "Delete" button. Unless the selected time block is the first time block, the preceding time block's end time will be adjusted appropriately so that there are no gaps in the profile schedule. If the selected time block is the first time block, then the following time
20 block's start time will be adjusted appropriately.

Referring to Fig. 14, a number of miscellaneous options relating primarily to the display of information on the instrument 10 are also user 24 selectable. For example, the format in which decimals are displayed (X.X or X,X), whether a 24 hour clock or a twelve hour one (with AM and PM), the date format (month, day, year
25 or day, month, year), whether the instrument 10 display 28 is to be backlit or not, and whether the instrument 10's audio beeper is to be activated or not, are displayed for selection.

With the next screen, illustrated in Fig. 15, the user 24 selects from among a number, for example, eight, of languages in which instruments 10 can be
30 programmed to display information, a number, for example, four, in which the particular instrument 10 being set up can display information at the patient's option. The "Tip Messages" screen, illustrated in Fig. 16, enables a list control that permits the

-7-

user 24 to select a number, for example, ten, of tip messages for display on the instrument 10 being set up. If the user 24 does not want tip messages displayed on the patient's instrument 10, the user 24 may deselect the "Tip Messages Enabled for Meter Setup" box. If this box is not checked, the user 24 must select individual messages
5 which the user 24 wants to appear on the patient's instrument 10 at appropriate times.

The user 24 may add custom tip messages to an instrument 10 being set up for a patient. To do this, the user 24 selects the "Custom" button. The screen illustrated in Fig. 17 is displayed. If the user 24 then selects the "Add" button, the screen illustrated in Fig. 18 is displayed. If the user 24 selects the "Edit" button, the
10 screen illustrated in Fig. 19 is displayed. If the user 24 selects the "Remove" button, the tip message highlighted in the screen illustrated in Fig. 17 is deleted. Once these screens have been completed, the instrument 10 setup is complete. The user 24 is presented with a dialog and given instructions on how to view and save the completed setup. This screen is illustrated in Fig. 20.

15 Returning briefly to Fig. 3, if the user 24 selects the "Retrieve an Existing Meter Setup from a Meter" option, and no instrument 10 is connected to the PC 14, the user 24 is asked to connect the instrument 10 to the PC 14. If the user 24 selects "OK" and no instrument 10 is yet connected to the PC 14, the user 24 is again asked to connect the instrument 10 to the PC 14. If the user 24 selects "Cancel," the
20 "Welcome" screen of Fig. 3 again appears. If the user 24 selects "Help," the help facility is launched with troubleshooting information regarding connecting an instrument 10 to the PC 14. If the user 24 selects the "Open an Existing Meter Setup File" from the "Welcome" screen, a Microsoft® Windows® file opening common dialog is launched. The user 24 may then select an instrument 10 setup file to edit or
25 cancel back to the "Welcome" screen.

If the user 24 has selected either the "Open an Existing Meter Setup File" option or the "Retrieve an Existing Meter Setup from a Meter" option, ultimately a summary screen of the general configuration illustrated in Fig. 21 will be displayed. This screen displays the instrument 10 setup. The user 24 may edit this setup by
30 selecting the highlighted text on the screen. The user 24 is then presented with the appropriate instrument 10 setup tab to edit instrument 10 setup options. The basic elements of the summary screen as they appear on the Microsoft® Windows® 95

-8-

platform are illustrated in Fig. 21. The title bar contains a descriptor for the data contained in the client area followed by the name of the software. This descriptor may be "New Meter," a filename, or a designation such as "John Smith's Meter." Below the title bar is a menu bar. The menu bar is described later.

5 Below the menu bar, in the client area of the window, is a summary screen. This summary screen contains the current instrument 10 setup settings. The user 24 may edit the information contained on this screen by clicking on the underlined text. This activates the instrument 10 setup tabs, similarly to the screen illustrated in Fig. 22, "Instrument setup manager-tab template screen." The tab control contains
10 screens that are nearly identical to the ones available via the instrument 10 setup Wizard™, with the difference being that the Wizard™ provides a simple, step-by-step approach to entering data, whereas the tab control gives the user 24 one-click access to any screen. The tabs can also be used to set up instruments 10. They provide a somewhat more powerful tool for doing this. However, it is suggested that, for the
15 first few times at least, the user 24 perform instrument 10 setup using the Wizard™ as a learning tool.

 With reference to Fig. 23, the contents of the "Personal" tab are illustrated. As will be appreciated, the contents of this tab, and the appropriate user 24 interactions, are generally as described in connection with the screen illustrated in Fig.
20 5. Referring to Fig. 24, the contents of the "Glucose units/ranges" tab and the appropriate user interactions are generally as described in connection with the screen illustrated in Fig. 6. Turning to Fig. 25, the contents of the "Insulin type" tab are illustrated. These contents and the associated user 24 interactions are generally as described in connection with the screen illustrated in Fig. 7. Referring to Fig. 26, the
25 contents of the "Event markers" tab and the related user 24 interactions are generally as described in connection with the screen illustrated in Fig. 8.

 Turning to Fig. 27, the contents of the "Time blocks" tab are illustrated. These contents and the associated user 24 interactions are generally as described in connection with the screen illustrated in Fig. 9. With reference to Fig. 28, the contents
30 of the "Time blocks" tab and user 24 interactions are generally as described in connection with the screen illustrated in Fig. 10. Referring to Fig. 29, the contents of the "Insulin pump profile" tab and the related user 24 interactions are generally as

-9-

described in connection with the screen illustrated in Fig. 11. Turning to Fig. 30, the contents of the "Miscellaneous options" tab and user 24 interactions associated with it are generally as described in connection with the screen illustrated in Fig. 14. With reference to Fig. 31, the contents of the "Language" tab and user 24 interactions associated with it are generally as described in connection with the screen illustrated in Fig. 15. Referring to Fig. 32, the contents of the "Tip messages" tab and user 24 interactions associated with it are generally as described in connection with the screen illustrated in Fig. 16.

The user 24 may press a function key, F1 in the illustrated example, to open the help facility and obtain context sensitive help. All dialogs also have associated help buttons which access the help facility. The instrument 10 setup manager also has a help menu. The user 24 may cancel from the "Welcome" screen by selecting the "Cancel" button on that screen. When that action is taken, the welcome dialog box illustrated in Fig. 3 is dismissed and the main screen is displayed.

The user may select "Retrieve Patient Data from a Meter" connected to the computer 14 from the "Welcome" screen. If the user 24 then selects "OK," a sequence to retrieve patient data from a connected instrument 10 is initiated. This is exactly equivalent to selecting the "Retrieve Patient Data" option from the Meter menu. The Meter Setup Manager functions are divided into "File," "Meter," "View" and "Help" menus. See, for example, Fig. 21. The options under the "File" menu include "New," "Open . . . , " "Close," "Save," "Save As . . . , " "Print," "View Patient Report . . . , " "Print Patient Report . . . , " "Edit Patient Database . . . , " "Recent File List" and "Exit." The options under the "Meter" menu include "Retrieve Patient Data," "Retrieve Meter Setup," "Send Meter Setup," "Clear Patient Diary" and "COMmunication Port Settings " The options under the "View" menu include "Toolbar," "Status Bar" and "Options " The options under the "Help" menu include "Help topics" and "About "

The "File" menu contains commands that operate on Meter Setup Data and Patient Data. "New" returns all fields to their default states and initially opens a new instrument 10 setup with the Meter Setup Wizard. The user 24 may change this setting to Meter Setup Tabs by selecting "Options" under the "View" menu. If there is any unsaved data in the fields, the user 24 is prompted to save it. "Open" prompts the

-10-

user 24 to name a file to open and opens a Meter Setup File. If the selected file is not an instrument 10 setup file, an error message is displayed and the Summary Screen is blank. If the selected file is an instrument 10 setup file, then the data is initially displayed with the Summary Screen. The user 24 may edit the open document with the Meter Setup Tabs by clicking on the underlined text, or may edit the open document with the Meter Setup Wizard™ by selecting the Wizard™ toolbar button.

“Close” closes the currently open instrument 10 setup file. If the currently open instrument 10 setup file has not been saved, the user 24 will be prompted to save it. “Save” saves the currently open file. If the file has not yet been assigned a name, the user 24 will be prompted to assign it a name and location. “Save As” saves the current file under the assigned name. The user 24 is prompted to assign it a name and location. “Print” prints the current instrument 10 setup data. “View Patient Report . . .” prompts the user 24 to identify a patient data file to view using the patient name, instrument 10 serial number and the date received or the actual file name to select the file for viewing. “View Patient Report . . .” causes the selected report to be displayed in the format specified by the user 24. See Fig. 33. The user 24 selects the report format by selecting “Options” from the “View” menu. “View Patient Report Browser,” Fig. 34, is accessed by the user 24 clicking on the “Browse . . .” button on the screen illustrated in Fig. 33. “View Patient Report Browser” permits the user 24 to scroll through the patient reports saved in the database for one the user wishes to view. “Print Patient Report . . .” causes the selected report to be printed. The user 24 selects the report to be printed in response to a prompt from this routine. See Fig. 35. “Print Patient Report Browser,” Fig. 36, is accessed by the user 24 clicking on the “Browse . . .” button on the screen illustrated in Fig. 35. “Print Patient Report Browser” permits the user 24 to scroll through the patient reports saved in the database for one the user 24 wishes to print. “Edit Patient Database . . .” permits the user 24 to add, delete and edit patient name-to-instrument 10 serial number associations. See Figs. 37 and 38. “Recent File List” causes the four most recently opened files from the Patient Data and Meter Setup databases to be displayed, and permits the user 24 to open one of these files by selecting it from the list. “Exit” causes the computer 14 to exit from the Meter Setup Manager routine.

The “Meter” menu contains commands that act upon the instrument 10

-11-

that is connected to the computer 14. "Retrieve Patient Data" prompts the user 24 to enter a filename and a location to save the patient data to, and then retrieves the patient data from the instrument 10 connected to the computer 14. If no instrument 10 is connected to the computer 14, the user 24 is prompted to connect one. Once the data transfer is complete, the patient data is displayed in the format selected by the user 24. An "Options" screen illustrated in Fig. 39 permits the user 24 to select various Meter Setup Manager application options. For example, under the "Report settings" tab, the user 24 is prompted to select from among the various report formats: "Diary," "Glucose values," Trend," "Glucose graph," "Average trend," Glucose ranges," and "Hypoglycemic events." The user 24 is also prompted to select the time range for average trend, glucose ranges and hypoglycemic events reports. The user 24 is further prompted to select the glucose units, for example, mg/dL or mmol/L, for the reports. Under the "New meter setup" tab, the user 24 is prompted to select how new instrument 10 setup will be performed, permitting the user 24 to select the Meter Setup Wizard™, or use the tabs, or instructing the Meter Setup Manager always to ask how instrument 10 setup is to be performed. See Fig. 40 and the discussion of Fig. 22 above. Under the "Meter COM port" tab, the user 24 is prompted to select the computer 14 port 18 through which communication with the instrument 10 will be conducted. See Fig. 41. Referring to Fig. 42, under the "Startup" tab, the user 24 is prompted to indicate whether the "Welcome" screen, Fig. 3, should be displayed at startup.

"Retrieve Meter Setup" retrieves the Meter Setup Data from an instrument 10 and displays the instrument 10 setup data using the Summary Screen. If no instrument 10 is connected to the computer 14, the user 24 is prompted to connect one. Fig. 43 illustrates the screen which is displayed when instrument 10 setup status data is being transferred. When the instrument 10 setup data transfer is complete, if the instrument 10 serial number does not have associated with it a patient name, the "Enter Patient Name" prompt appears, Fig. 44, prompting the user 24 to enter the patient's name. The entered patient's name then appears on the summary screen.

"Send Meter Setup" sends instrument 10 setup data to an instrument 10 connected to the computer 14. If no instrument 10 is connected to the computer 14, the user 24 will be prompted to connect one. Before the instrument 10 setup data is

-12-

sent to the instrument 10, the user 24 is prompted to set the date and time on the instrument 10. The user 24 has the option of not changing the instrument 10's date and time, synchronizing the instrument 10's date and time to the computer 14's or manually setting the instrument 10's date and time. See Fig. 45. As the instrument 10
5 setup data is being sent to the instrument 10, the screen illustrated in Fig. 46 is displayed.

"Clear Patient Diary" clears the patient diary data of an instrument 10 connected to the computer 14. To prevent accidental clearing of diary, the user 24 is prompted to save patient data to files before proceeding with clearing of patient diary
10 from an instrument 10. If no instrument 10 is connected to the computer 14, the user 24 will be prompted to connect one. "COM Port Settings" causes the screen illustrated in Fig. 47 to be displayed. The user 24 is prompted to select the computer 14 port 18 through which communication with the instrument 10 will be conducted.

The "View" menu contains items that adjust the settings for the Meter
15 Setup Manager. The "Toolbar" command permits the user 24 to select whether the toolbar is displayed. The "Status Bar" command permits the user 24 to select whether the status bar, which is located at the bottom of the Meter Setup Manager application screen, is displayed. "Options" creates a display which permits the user 24 to choose various Meter Setup Manager application options. This multi-page display is
20 illustrated in Figs. 48-51. See the above discussion of Figs. 39-42.

The "Help" menu contains items that provide the user 24 with access to information about the Meter Setup Manager. "Help Topics" displays the table of contents of a help file. The user 24 may navigate via hyperlinks from the table of contents to the contents of the various help file entries. The "About" entry causes the
25 version of the software and copyright notice information to be displayed.

The toolbar for the Meter Setup Manager contains command buttons for commonly accessed features, such as "File-New," "File-Open," "File-Save," "File-Print," "Meter Setup Wizard," "Meter Communication-Retrieve Meter Setup," "Meter Communication-Send Meter Setup" and "Meter Communication-Retrieve Patient
30 Data."

Phone-In Manager

All functions related to telephone modem 20, 22-based communication

-13-

between a patient's instrument 10' and the user 24's computer 14 fall within the control of the Phone-In Manager routine. Consequently, the Phone-In Manager routine illustratively runs all of the time. Installation of the utility program 12 places a link to the Phone-In Manager routine's executable in the Microsoft® Windows® startup folder, so that the Phone-In Manager routine launches automatically whenever Microsoft® Windows® launches. In rare cases, the user 24 may need to launch the Phone-In Manager routine by double clicking on its icon, for example, an illustration of a telephone, or by other Microsoft® Windows® convention.

After the Phone-In Manager routine is launched, a copyright screen will appear briefly. After launch, Phone-In Manager is generally minimized. This waiting state is generally referred to herein as "Wait for New Calls." The user 24 may also "Review Calls" or "Perform Administrative Tasks." From the perspective of a patient who is using an instrument 10', the patient's data may be sent to the health care professional's office prior to a scheduled appointment. The patient may also phone the patient data in to the health care professional's office at any time, as necessary, to permit the health care professional to review it. From the perspective of the health care professional, such a connection is completely automatic. The patient performs all necessary interactions to achieve the data transfer.

As previously noted, Phone-In Manager is always running, at least as a background task. It will be active only when a phone call comes in to the health care professional's office computer 14 or when a user 24 restores it to display status on the computer 14 monitor. A user 24 restores Phone-In Manager, for example, to review calls or to change any of the Phone-In Manager configuration options. Fig. 52 illustrates the Phone-In Manager main screen restored. When patients phone their data in via modems 20, 22 to the health care professional's computer 14, the Phone-In Manager keeps track of each call and the data that was received.

All calls are logged in order from most recent to oldest. Each logged call is displayed in the list with the instrument 10' serial number, patient's name if available, and the time and date of the phone call. The user 24 of the computer 14 may view or print patient data by highlighting the desired patient's instrument 10' serial number and selecting the "View" or "Print" button, respectively. The user 24 may also select the "Auto Print" option, in which case incoming patient data is automatically

-14-

printed. The user 24 may also view or print patient data which has expired from the Recent Calls list displayed in the screen illustrated in Fig. 52. Selecting the "View" button results in the display of the selected patient's data in the format illustrated in Fig. 53. The user 24 can then choose to print or close this file. The user 24 can also
5 view this screen by selecting old files to view from the menu. The files can be selected by the serial number of the instrument 10', patient name and data transfer date, or by file name. Selecting the "Print" button results in the printing of the selected patient's data in the report format illustrated in Fig. 53. The user 24 can also print files which have expired from the Recent Calls list by selecting old files to print from the menu.
10 Again, the files to be printed can be selected by the serial number of the instrument 10', patient name and data transfer date, or by file name. If the "Auto Print" check box is checked, patient reports will be printed upon receipt.

In Phone-In Manager as in Meter Setup Manager, features that are accessed on a routine basis are located in the client area of the window. These
15 features and their data are easily accessible and reviewable. Other features which are used less frequently are located in a standard Microsoft® Windows® menu bar. These include the "File," "View" and "Help" menus. The "File" menu contains commands which operate on patient data. "View Patient Reports" permits the user 24 to view older patient files by selecting the instrument 10' serial number, patient name and date
20 of receipt of data, or the actual file name. "Print Patient Reports" permits the user 24 to print older patient files by selecting the instrument 10' serial number, patient name and date of receipt of data, or the actual file name. "Edit Patient Database" permits the user 24 to add, delete and edit patient name to instrument 10' serial number associations. "Print Setup" is the standard Microsoft® Windows® printer 30 setup
25 routine. "Exit" results in the Phone-In Manager routine being exited.

The "View" menu contains menu items that permit the user 24 to view and modify various Phone-In Manager data stores. The "Status Bar" permits the user 24 to turn the status bar at the bottom of the main window on or off. "Phone Line Status" displays a dialog, illustrated in Fig. 54, containing the states of all phone lines.
30 This permits the user 24 to enable or disable one or more of the phone lines 23 connected to the computer 14. When the utility program 12 is running in Windows® 95 and the user 24 clicks on the "Add" button or the "Properties" button on the screen

-15-

illustrated in Fig. 54, the screen illustrated in Fig. 55 is displayed. This screen permits the user 24 to select from modems 20, 22 configured using the control panel. When the utility program 12 is running in Windows® 3.1 and the user 24 clicks on the "Add" button or the "Properties" button on the screen illustrated in Fig. 54, the screen
5 illustrated in Fig. 56 is displayed. This screen prompts the user 24 to set the serial port and baud rate for the modems 20, 22. When the utility program 12 is running in Windows® 3.1 and the user 24 clicks on the "Advanced Modem Settings" button on the screen illustrated in Fig. 54, the screen illustrated in Fig. 57 is displayed. This screen permits the user 24 to modify modem 20, 22 strings.

10 "Call Statistics" causes a screen illustrated in Fig. 58 to be displayed. Statistics for each phone line connected to the computer 14 are displayed. Statistics include the number of calls made to the line, the number of patient data transfers attempted, and the number of patient data transfers which succeeded. This screen also permits the user 24 to reset the statistics. "Options" permits the user 24 to modify the
15 Phone-In Manager options. There are two tabs under "Options." One tab, "Report Settings," is illustrated in Fig. 59. This page permits the user 24 to select the type of Patient Data Report to view. The other tab, "Miscellaneous Options," is illustrated in Fig. 60. This page permits the user 24 to select how many files are kept for each patient, and how many days' calls are kept in the Recent Calls list. It also permits the
20 user 24 to select to have patient reports printed automatically.

The "Help" menu contains items that provide the user 24 with access to information about the Phone-In Manager. "Help Topics" displays the table of contents of a help file. The user 24 may navigate via hyperlinks from the table of contents to the contents of the various help file entries. The "About" entry causes the version of
25 the utility program 12 and copyright notice information to be displayed.

CLAIMS

1. A method of configuring a hand-held instrument for determining the concentration of a medically significant component of a body fluid or a control, the method comprising the steps of providing a configuring computer having a first port for transmitting at least one of instructions and data for configuring the instrument, providing on the instrument a second port for receiving said at least one of instructions and data from the configuring computer, coupling said first port to said second port, transmitting said one of instructions and data to configure said instrument from said first port, receiving said one of instructions and data at said second port, and configuring said instrument according to said one of instructions and data transmitted from said first port and received at said second port characterized in that at least said one of instructions and data include certain events, which a user of the hand-held instrument is then capable of entering with a test result into a user's diary which is maintained in the hand-held instrument, said events being chosen from a library of events.

2. The method of claim 1 wherein the step of providing a configuring computer having a first port for transmitting at least one of instructions and data for configuring the instrument comprises the step of providing a configuring computer having a first port for transmitting instructions for configuring the instrument.

3. The method of claim 2 wherein the step of providing a configuring computer having a first port for transmitting at least one of instructions and data for configuring the instrument comprises the step of providing a configuring computer having a first port for transmitting data for configuring the instrument.

4. The method of claim 1 wherein the step of providing a configuring computer having a first port for transmitting at least one of instructions and data for configuring the instrument comprises the step of providing a configuring computer having a first port for transmitting data for configuring the instrument.

5. The method of claim 1 wherein the hand-held instrument further comprises a display for displaying information related to the determined concentration, the step of transmitting said one of instructions and data to configure said instrument from said first port comprising the step of transmitting said one of instructions and data from said first port to configure said display.

6. The method of claim 2 wherein the hand-held instrument further comprises a display for displaying information related to the determined concentration,

-17-

the step of transmitting instructions from said first port to configure said instrument comprising the step of transmitting instructions to configure said display.

7. The method of claim 3 wherein the hand-held instrument further comprises a display for displaying information related to the determined concentration, the step of transmitting said one of instructions and data to configure said instrument from said first port comprising the step of transmitting data to configure said instrument display.

8. The method of claim 1 further comprising the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

9. The method of claim 8 wherein the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

10. The method of claim 9 and further comprising updating a file in the computer with the transmitted data.

11. The method of claim 2 further comprising the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

12. The method of claim 11 wherein the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

13. The method of claim 12 and further comprising updating a file in the computer with the transmitted data.

14. The method of claim 3 further comprising the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

15. The method of claim 14 wherein the step of transmitting one of instructions and data concerning determined concentration of a medically significant

-18-

component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

16. The method of claim 15 and further comprising updating a file
5 in the computer with the transmitted data.

17. The method of claim 4 further comprising the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

18. The method of claim 17 wherein the step of transmitting one of
10 instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

19. The method of claim 18 and further comprising updating a file
15 in the computer with the transmitted data.

20. The method of claim 5 further comprising the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

21. The method of claim 20 wherein the step of transmitting one of
20 instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

22. The method of claim 21 and further comprising updating a file
25 in the computer with the transmitted data.

23. The method of claim 6 further comprising the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

24. The method of claim 23 wherein the step of transmitting one of
30 instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port comprises the step of transmitting data concerning determined concentration of a medically significant

-19-

component of a body fluid from the instrument to the computer.

25. The method of claim 24 and further comprising updating a file in the computer with the transmitted data.

26. The method of claim 7 further comprising the step of
5 transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port.

27. The method of claim 26 wherein the step of transmitting one of instructions and data concerning determined concentration of a medically significant component of a body fluid from the second port to the first port comprises the step of
10 transmitting data concerning determined concentration of a medically significant component of a body fluid from the instrument to the computer.

28. The method of claim 27 and further comprising updating a file in the computer with the transmitted data.

29. The method of claim 1, 2, 3, 4, 5, 6 or 7 wherein the steps of
15 transmitting said one of instructions and data to configure said instrument from said first port and receiving said one of instructions and data at said second port comprise transmitting said one of instructions and data through a fiber optic coupler from said first port to said second port.

30. The method of claim 29 wherein the instrument comprises an
20 instrument for determining the glucose concentration of blood, a blood fraction or a control.


31. The method of claim 8, 9, 10, 11, 12, 13, 14, 15, 16, 17, 18, 19,
20, 21, 22, 23, 24, 25, 26, 27 or 28 wherein the step of transmitting said one of instructions and data concerning determined concentration of a medically significant
25 component of a body fluid from the second port to the first port comprises the step of transmitting said one of instructions and data concerning determined concentration of a medically significant component of a body fluid via a modem from the second port to the first port.

32. The method of claim 31 wherein the instrument comprises an
30 instrument for determining the glucose concentration of blood, a blood fraction or a control.


WO 99/27849


PCT/US98/25850

1/44

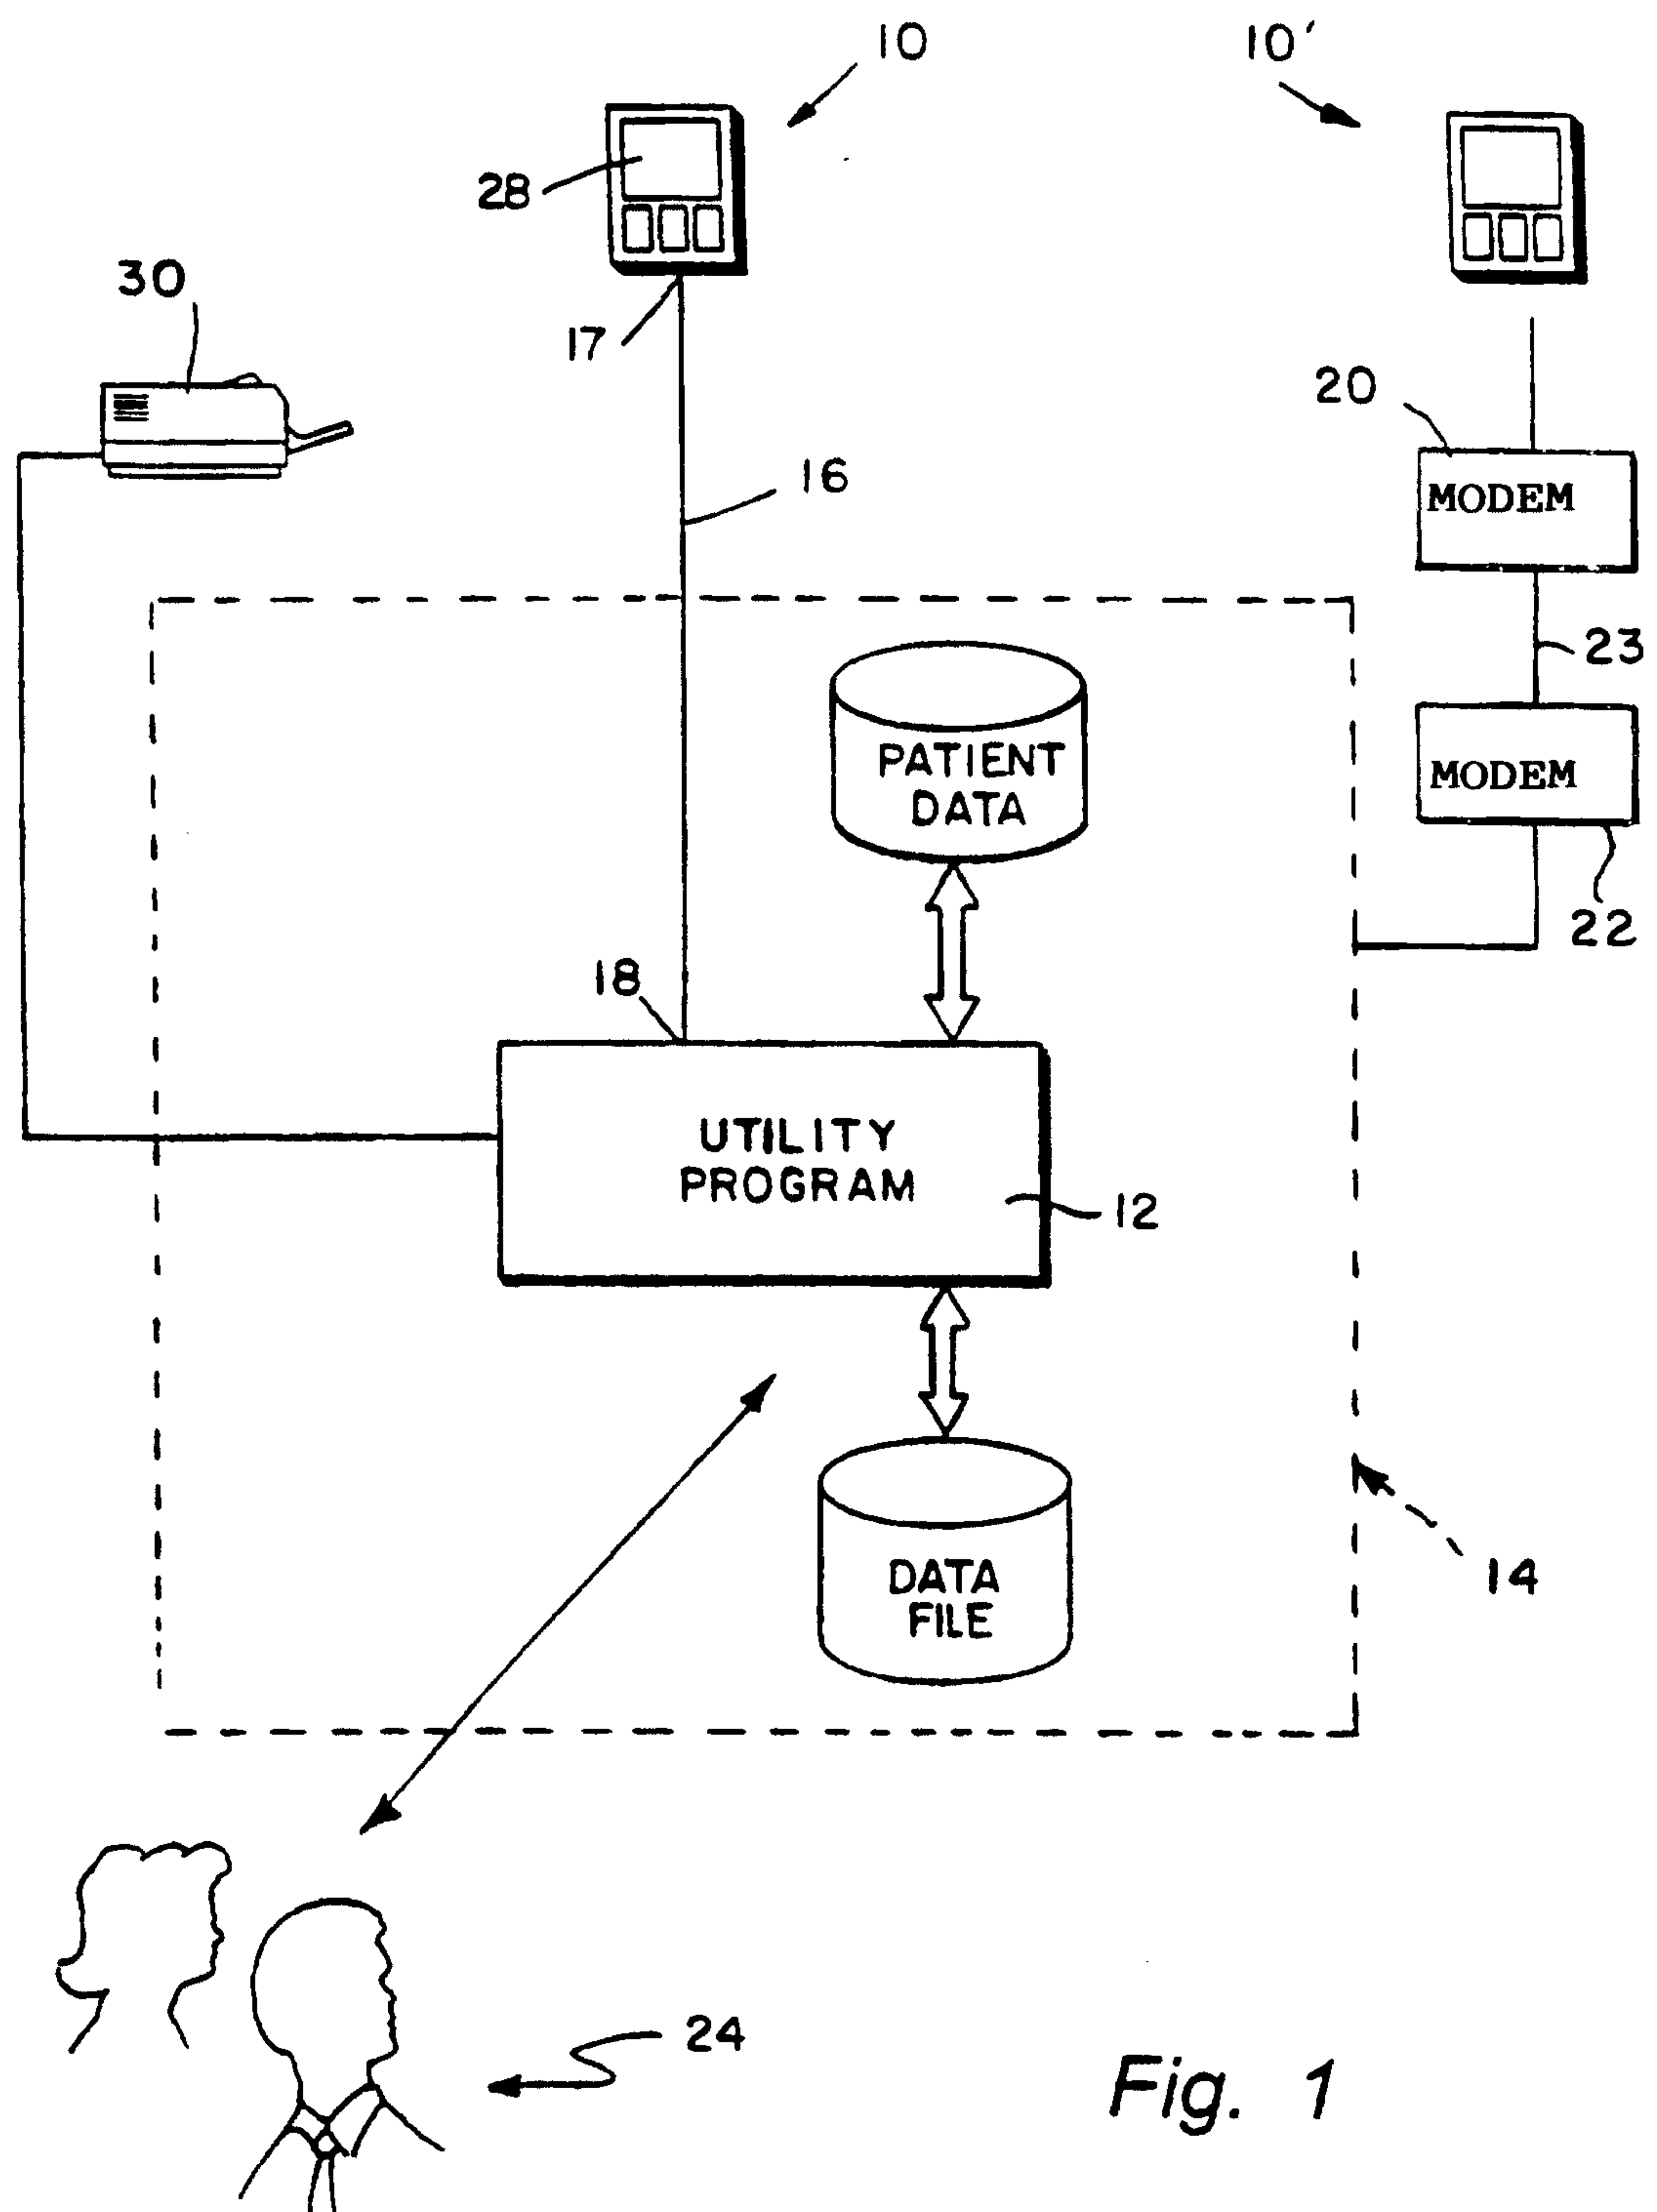

2/44

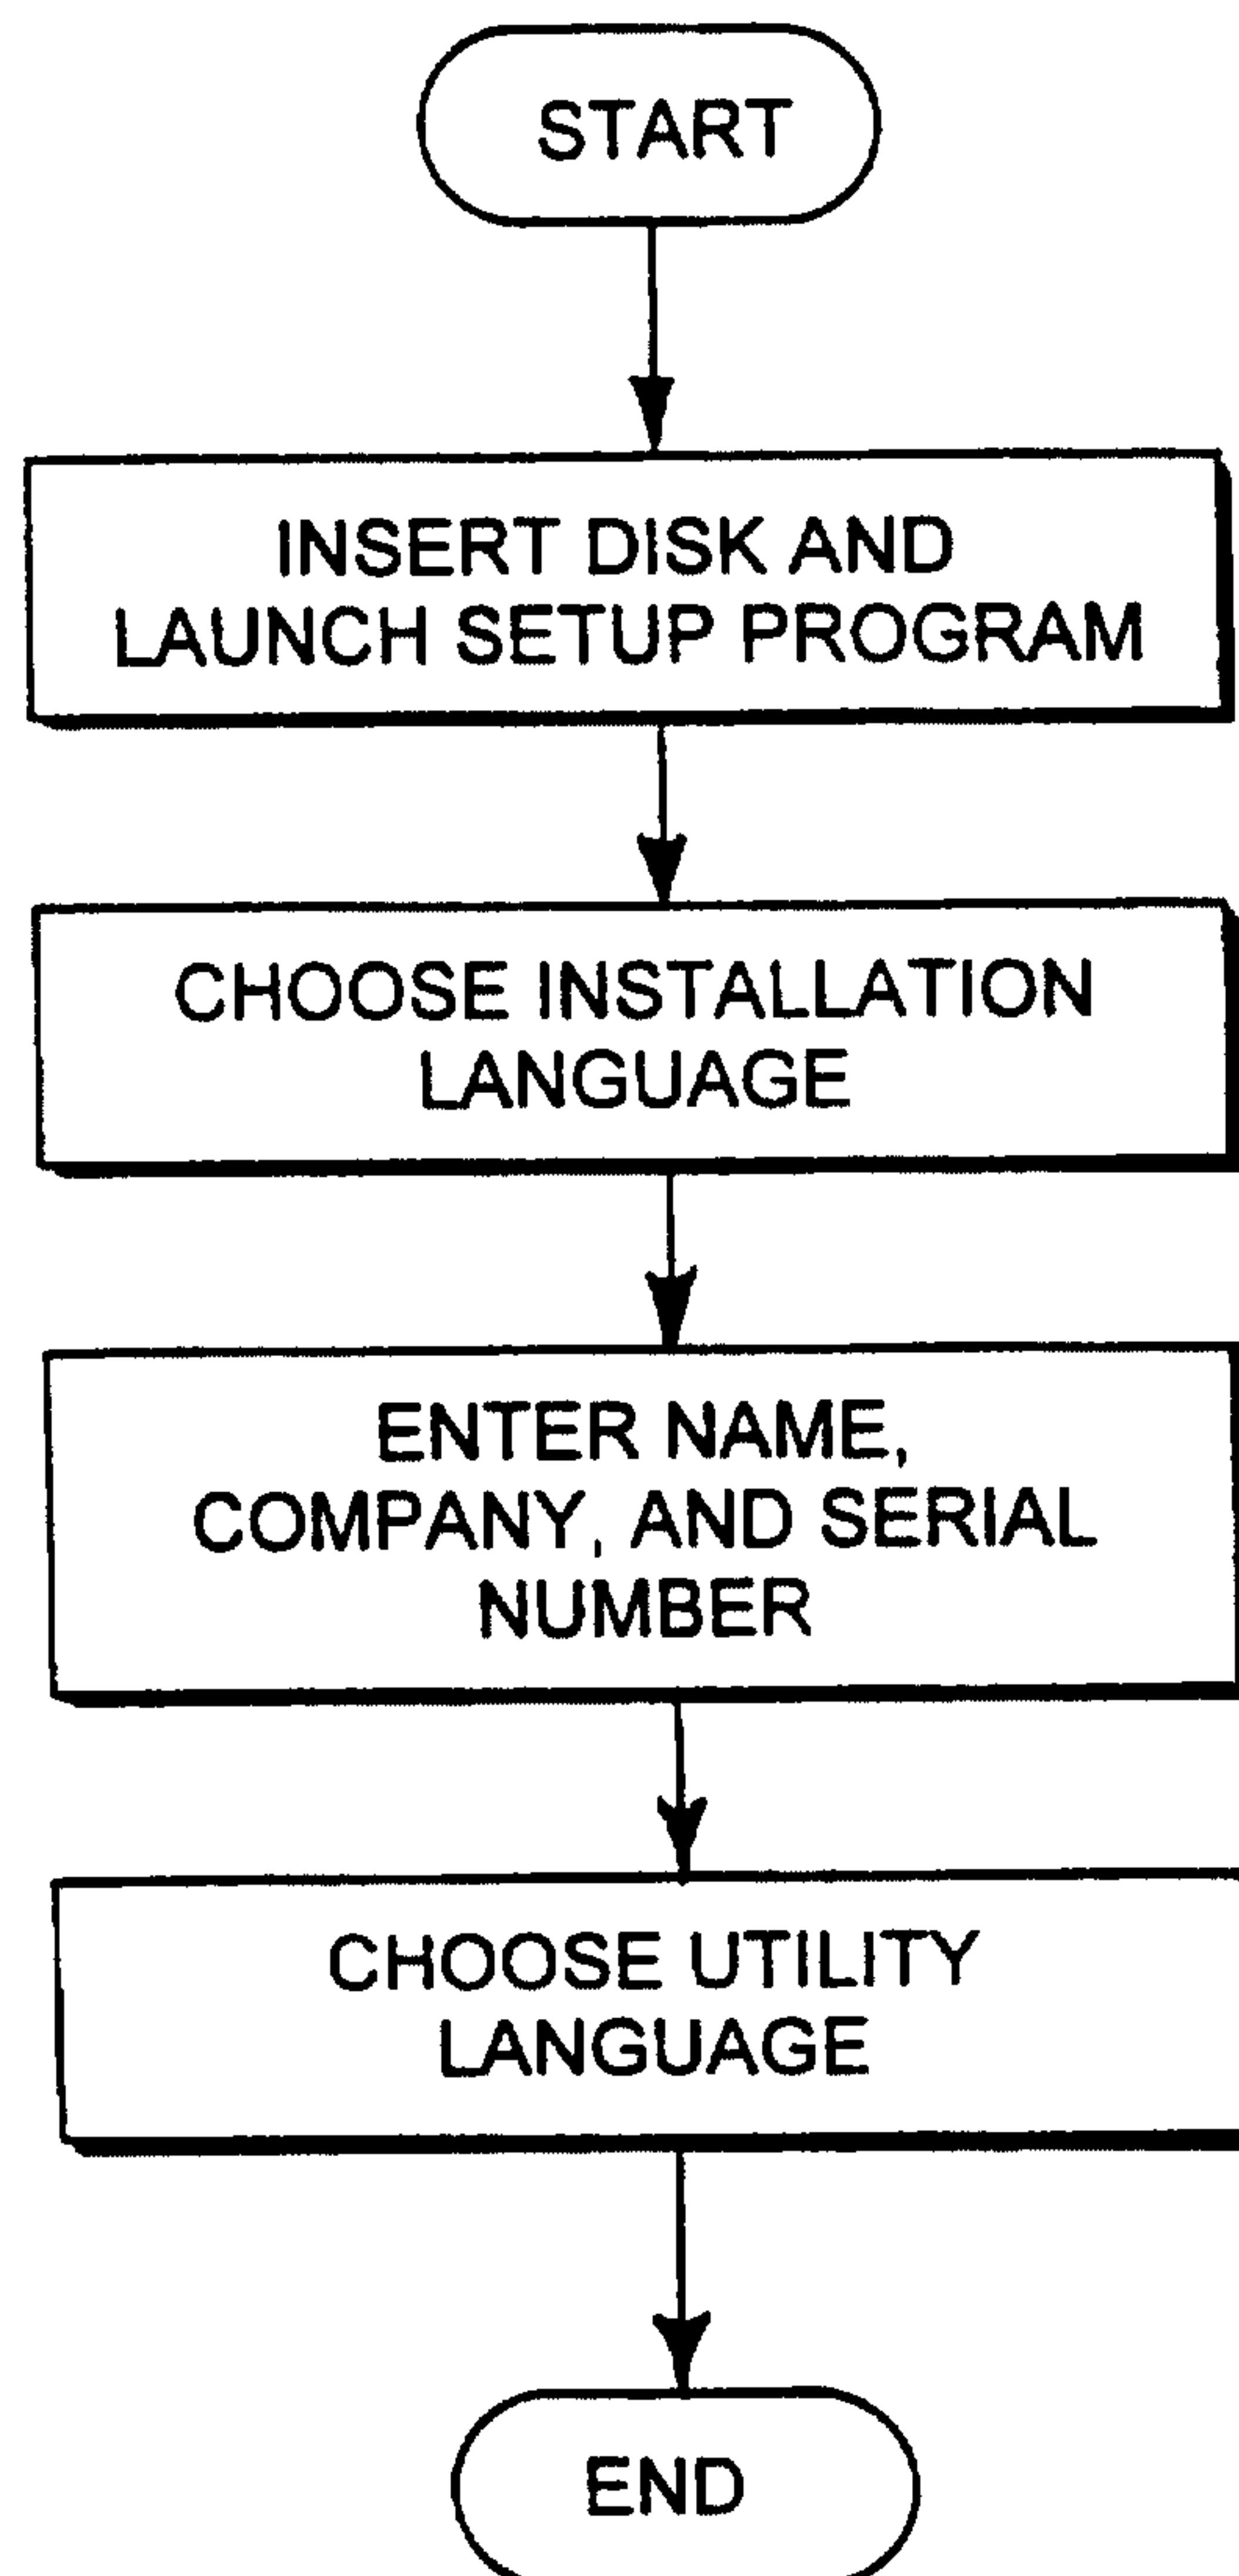*Fig. 2*

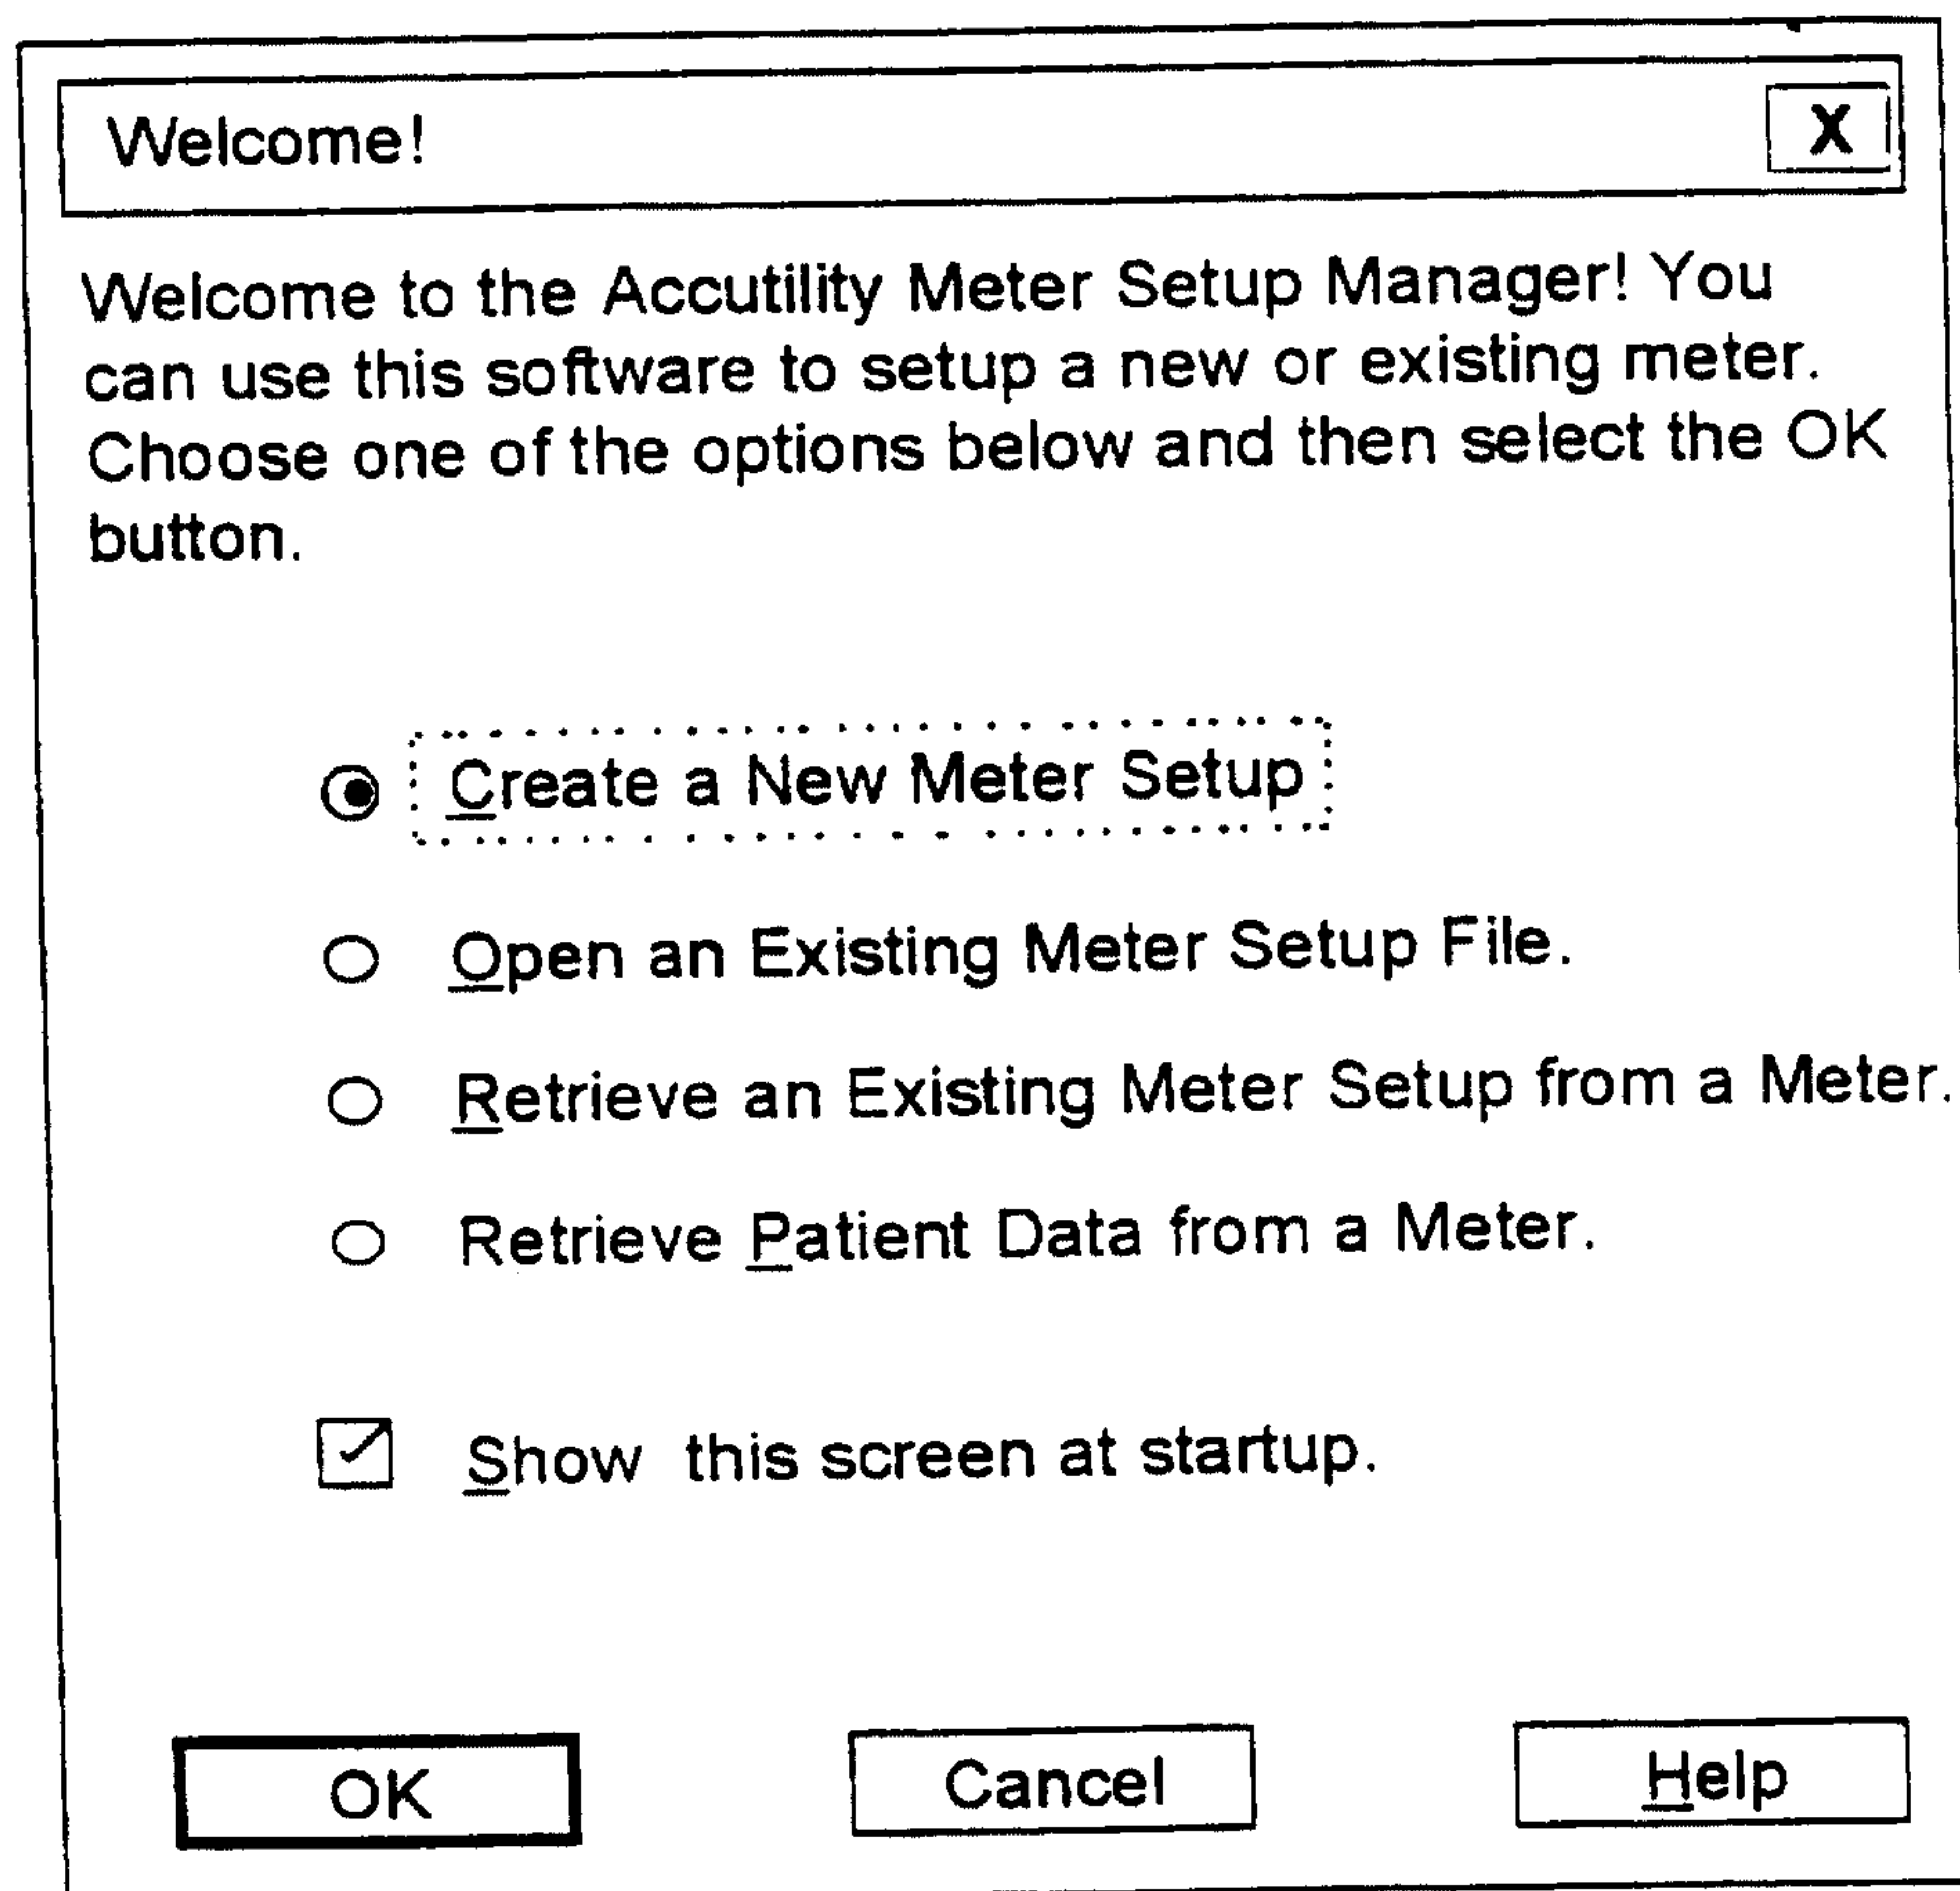*Fig. 3*

4/44

Fig. 4

Meter Setup Wizard -

Instructions on what to do on each screen appear here.

Interaction

< Back Next > Cancel Help

Fig. 5

Meter Setup Wizard - Personal Information

Enter the Patient and Healthcare Provider Information below.

The Patient ID may be a number or a name that is up to 20 characters in length.

Patient Information

Name:

ID:

Healthcare Provider Information:

Healthcare Computer Phone Number:

< Back Next > Cancel Help

5/44

Fig. 6

Meter Setup Wizard - Glucose Units/Ranges	
Units of Measure	
Glucose:	☒ mg/dL ☐ mmol/L
Glucose Limits	
Upper Limit:	0 mg/dL
Lower Limit:	0 mg/dL
Hypo:	0 mg/dL
< Back <input checked="" style="border: 1px solid black;" type="button" value=" Next > "/> Cancel Help	

Fig. 7

Meter Setup Wizard - Insulin Type	
Select up to three Insulin Types. These will be the only types available in the meter. Check the Insulin Logging box if you want to record insulin information in your meter.	
☐ Insulin Logging Enabled for Meter Setup	
Insulin Types	
Insulin Type 1:	Insulin Type 2:
Insulin Type 3:	
<None> ▼	<None> ▼
<None> ▼	
Insulin Increment:	
☒ Tenth Unit ☐ Half Unit ☐ Whole Unit	
< Back <input checked="" style="border: 1px solid black;" type="button" value=" Next > "/> Cancel Help	

Meter Setup Wizard - Time Blocks

Time Block information is contained in the list below.

The minimum time span for a Time Block is 1/2 hour. Editing the start time of a Time Block automatically adjusts the end time of the previous Time Block. No Time gaps are allowed between Time Blocks.

To edit an existing Time Block, select the Time Block and press the Edit button, or double click on the Time Block entry in the list.

Time Block	Name	3 Letter Name	Start Time	End Time	Duration
Breakfast		Brk	6:00 AM	8:59 AM	3.0
Midmorning		Mmo	9:00 AM	11:59 AM	3.0
Lunch		Lun	12:00 PM	2:59 PM	3.0
Midafternoon		Maf	3:00 PM	5:59 PM	3.0
Dinner		Din	6:00 PM	7:59 PM	2.0
Evening		Eve	8:00 PM	9:59 PM	2.0
Bed time		Bed	10:00 PM	2:59 AM	5.0
Night time		Ngt	3:00 AM	5:59 AM	3.0

Edit...

< Back

Next >

Cancel

Help

Fig. 9

Meter Setup Wizard - Event Markers

Select up to 15 Event Markers to add to the Meter Setup

The Events will appear in the meter in the order they appear in the 'Events To Load Into Meter' list.

You have selected 15 Events

S Available Events ▲

Active

After Breakfast

After Dinner

✓ After Exercise

Alter Lunch

✓ After Meal

Bed Time

Before Brekfast

Before Dinner

✓ Before Exercise

Before Lunch

✓ Before Meal

Cold Outdoors

Different Food

Drank Alcohol

Add >

< Remove

Events to Load into Meter

Before Meal

After Meal

Fasting

Snack

Feel Hypo.

Before Exercise

After Exercise

Illness

Invalid Test

Other's Result

User Defined

Stress

L1 Control

L2 Control

Oral Medication

S = Selected Event Markers

< Back

Next >

Cancel

Help

Fig. 8

7/44

Fig. 10

Time Block Information X

Three Letter Name: Brk

Start time: 6:00 AM End Time: 8:59 AM

Customize Time Block

Insulin Type 1: <None> Dose 0.0

Insulin Type 2: <None> Dose 0.0

Insulin Type 3: <None> Dose 0.0

Exercise Type: <None> Duration: 0.00

Carbohydrates: 0 grams

Event 1: No Event Event 3: No Event

Event 2: No Event Event 4: No Event

Fig. 11

Meter Setup Wizard - Insulin Pump Profile

Check the Insulin Pump Logging box if you want to record Insulin Pump Information in your meter:


☐ Insulin Pump Logging Enabled in Meter Setup

Type of Insulin: <None>

Profile Start Date: 11/09/98 Profile Start Time: 2:50 PM

Time Block Name	Start Time	End Time	Pump Rate
Time Block #1	12:00 AM	11:59 PM	0.0

8/44

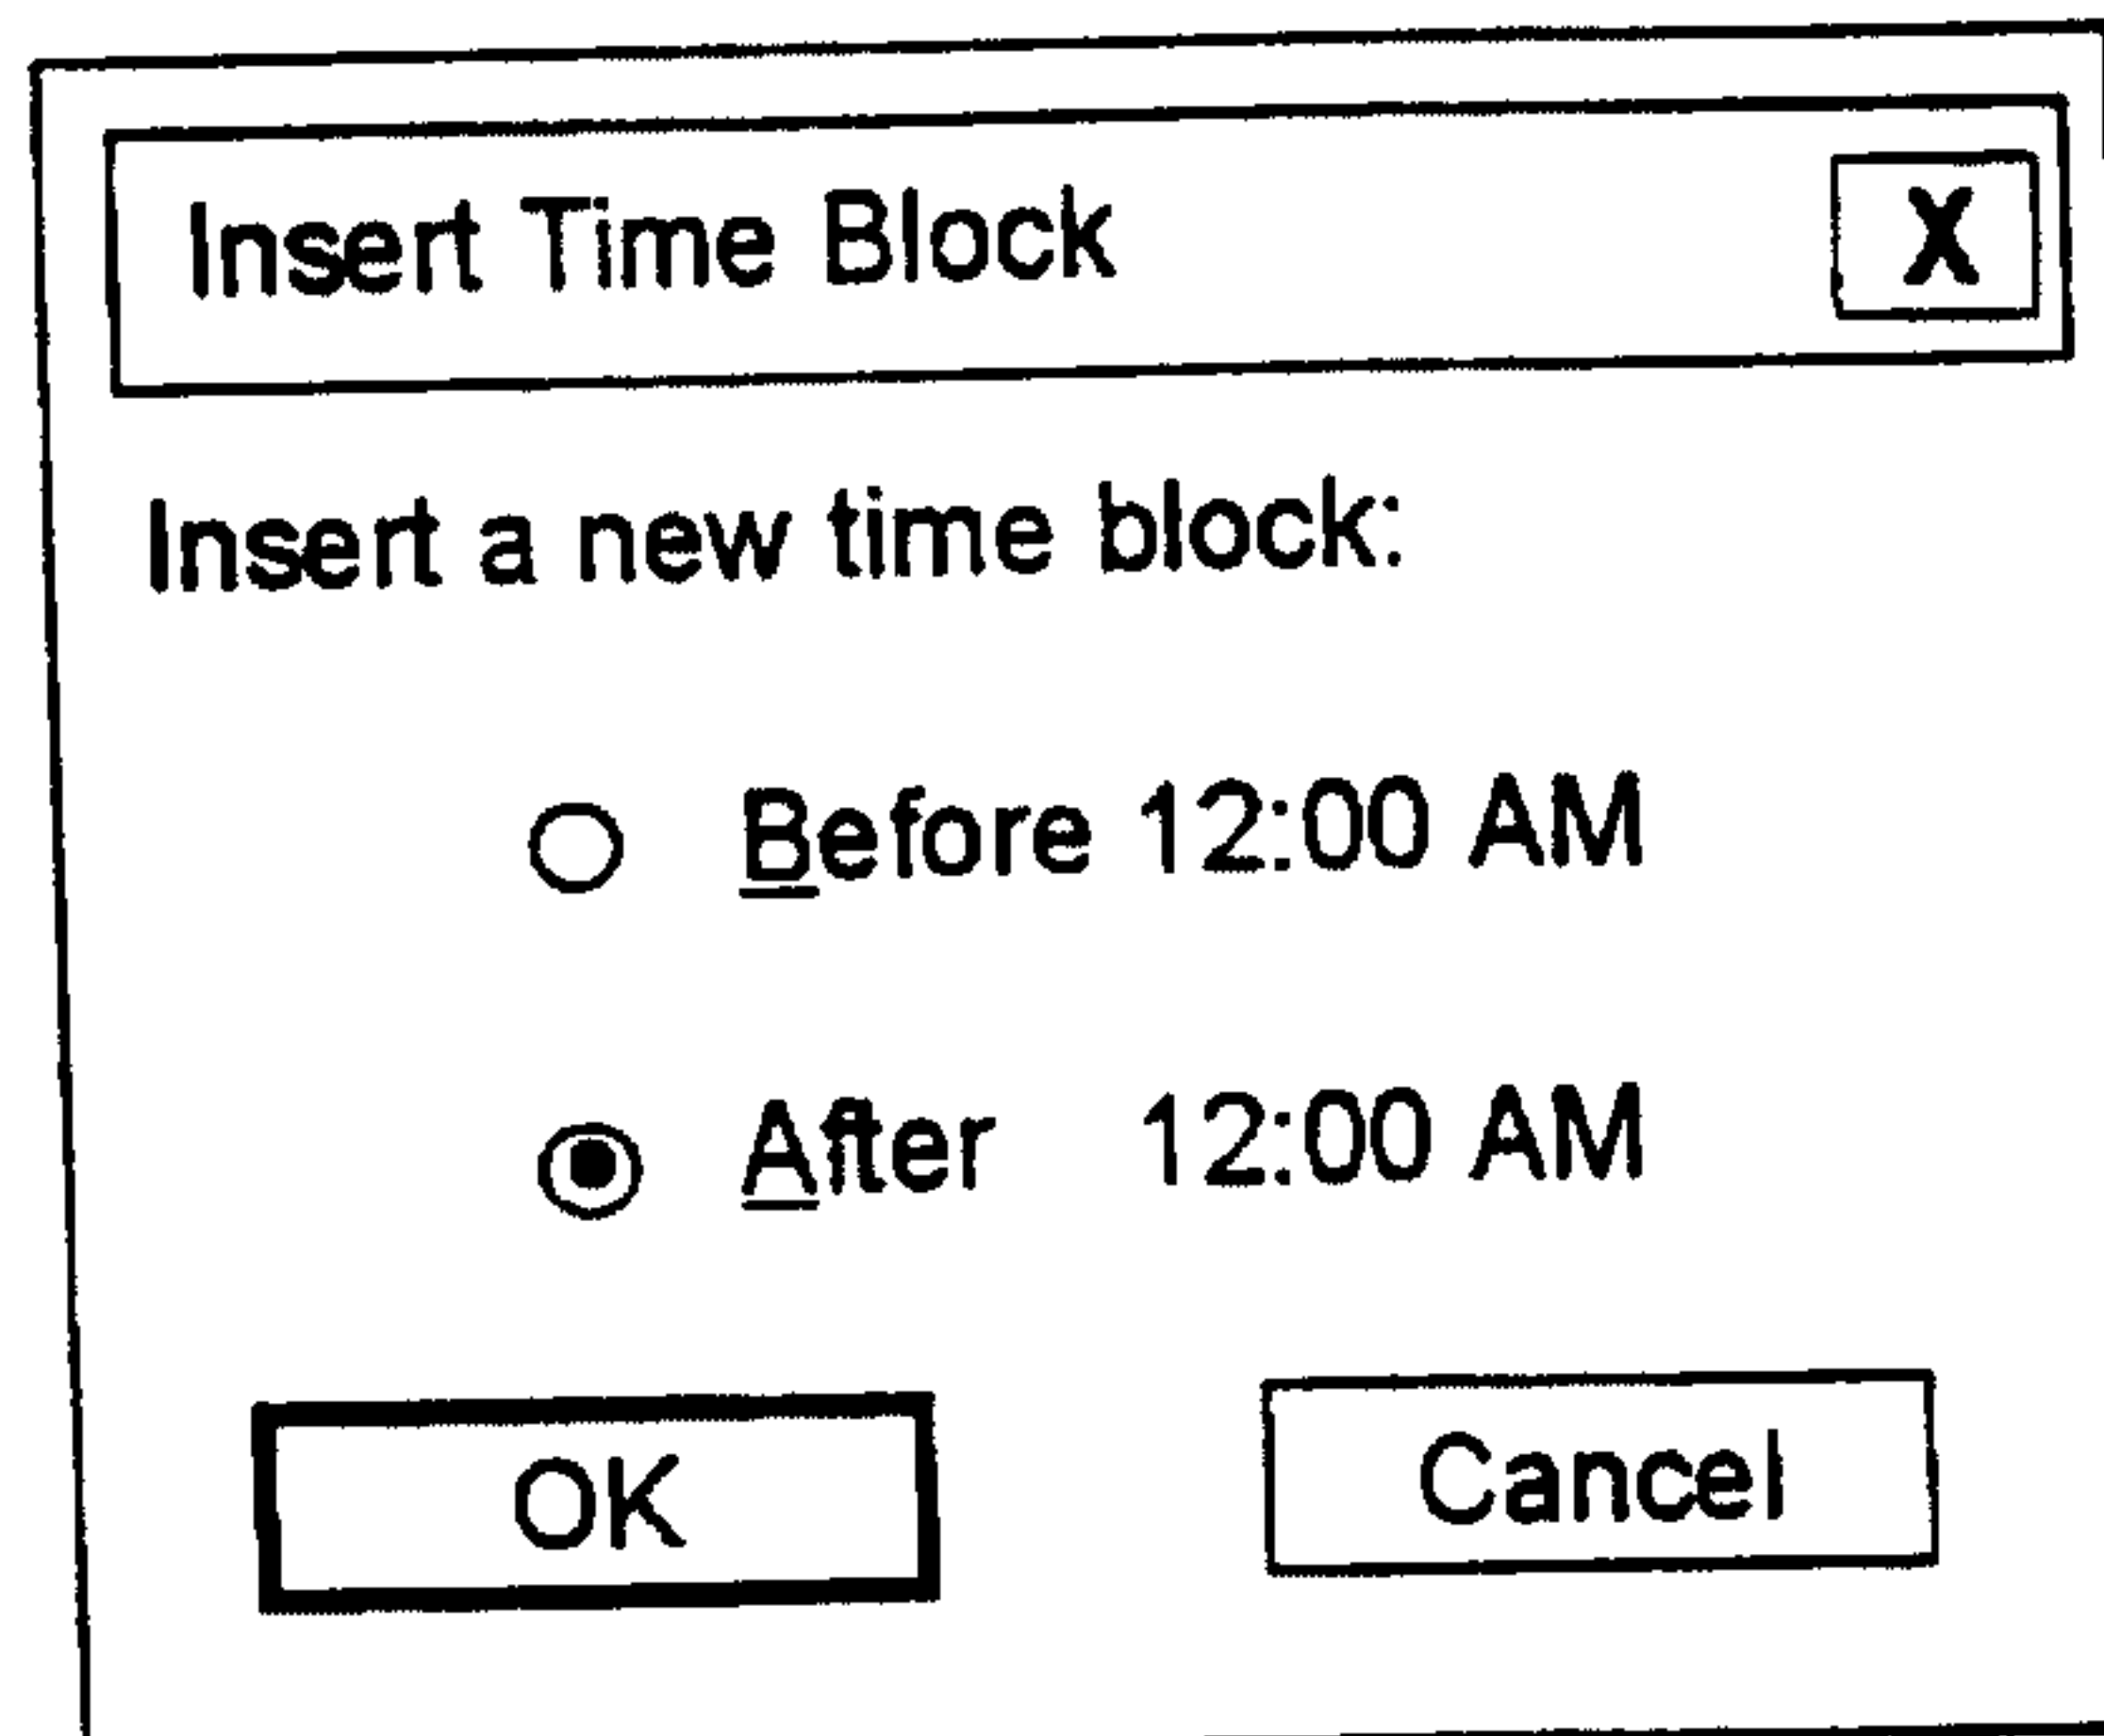

A dialog box titled "Insert Time Block" with a close button (X) in the top right corner. The text "Insert a new time block:" is followed by two radio button options: "Before 12:00 AM" and "After 12:00 AM". The "After 12:00 AM" option is selected. At the bottom are "OK" and "Cancel" buttons.


Insert Time Block [X]

Insert a new time block:

☐ Before 12:00 AM

☒ After 12:00 AM

OK Cancel

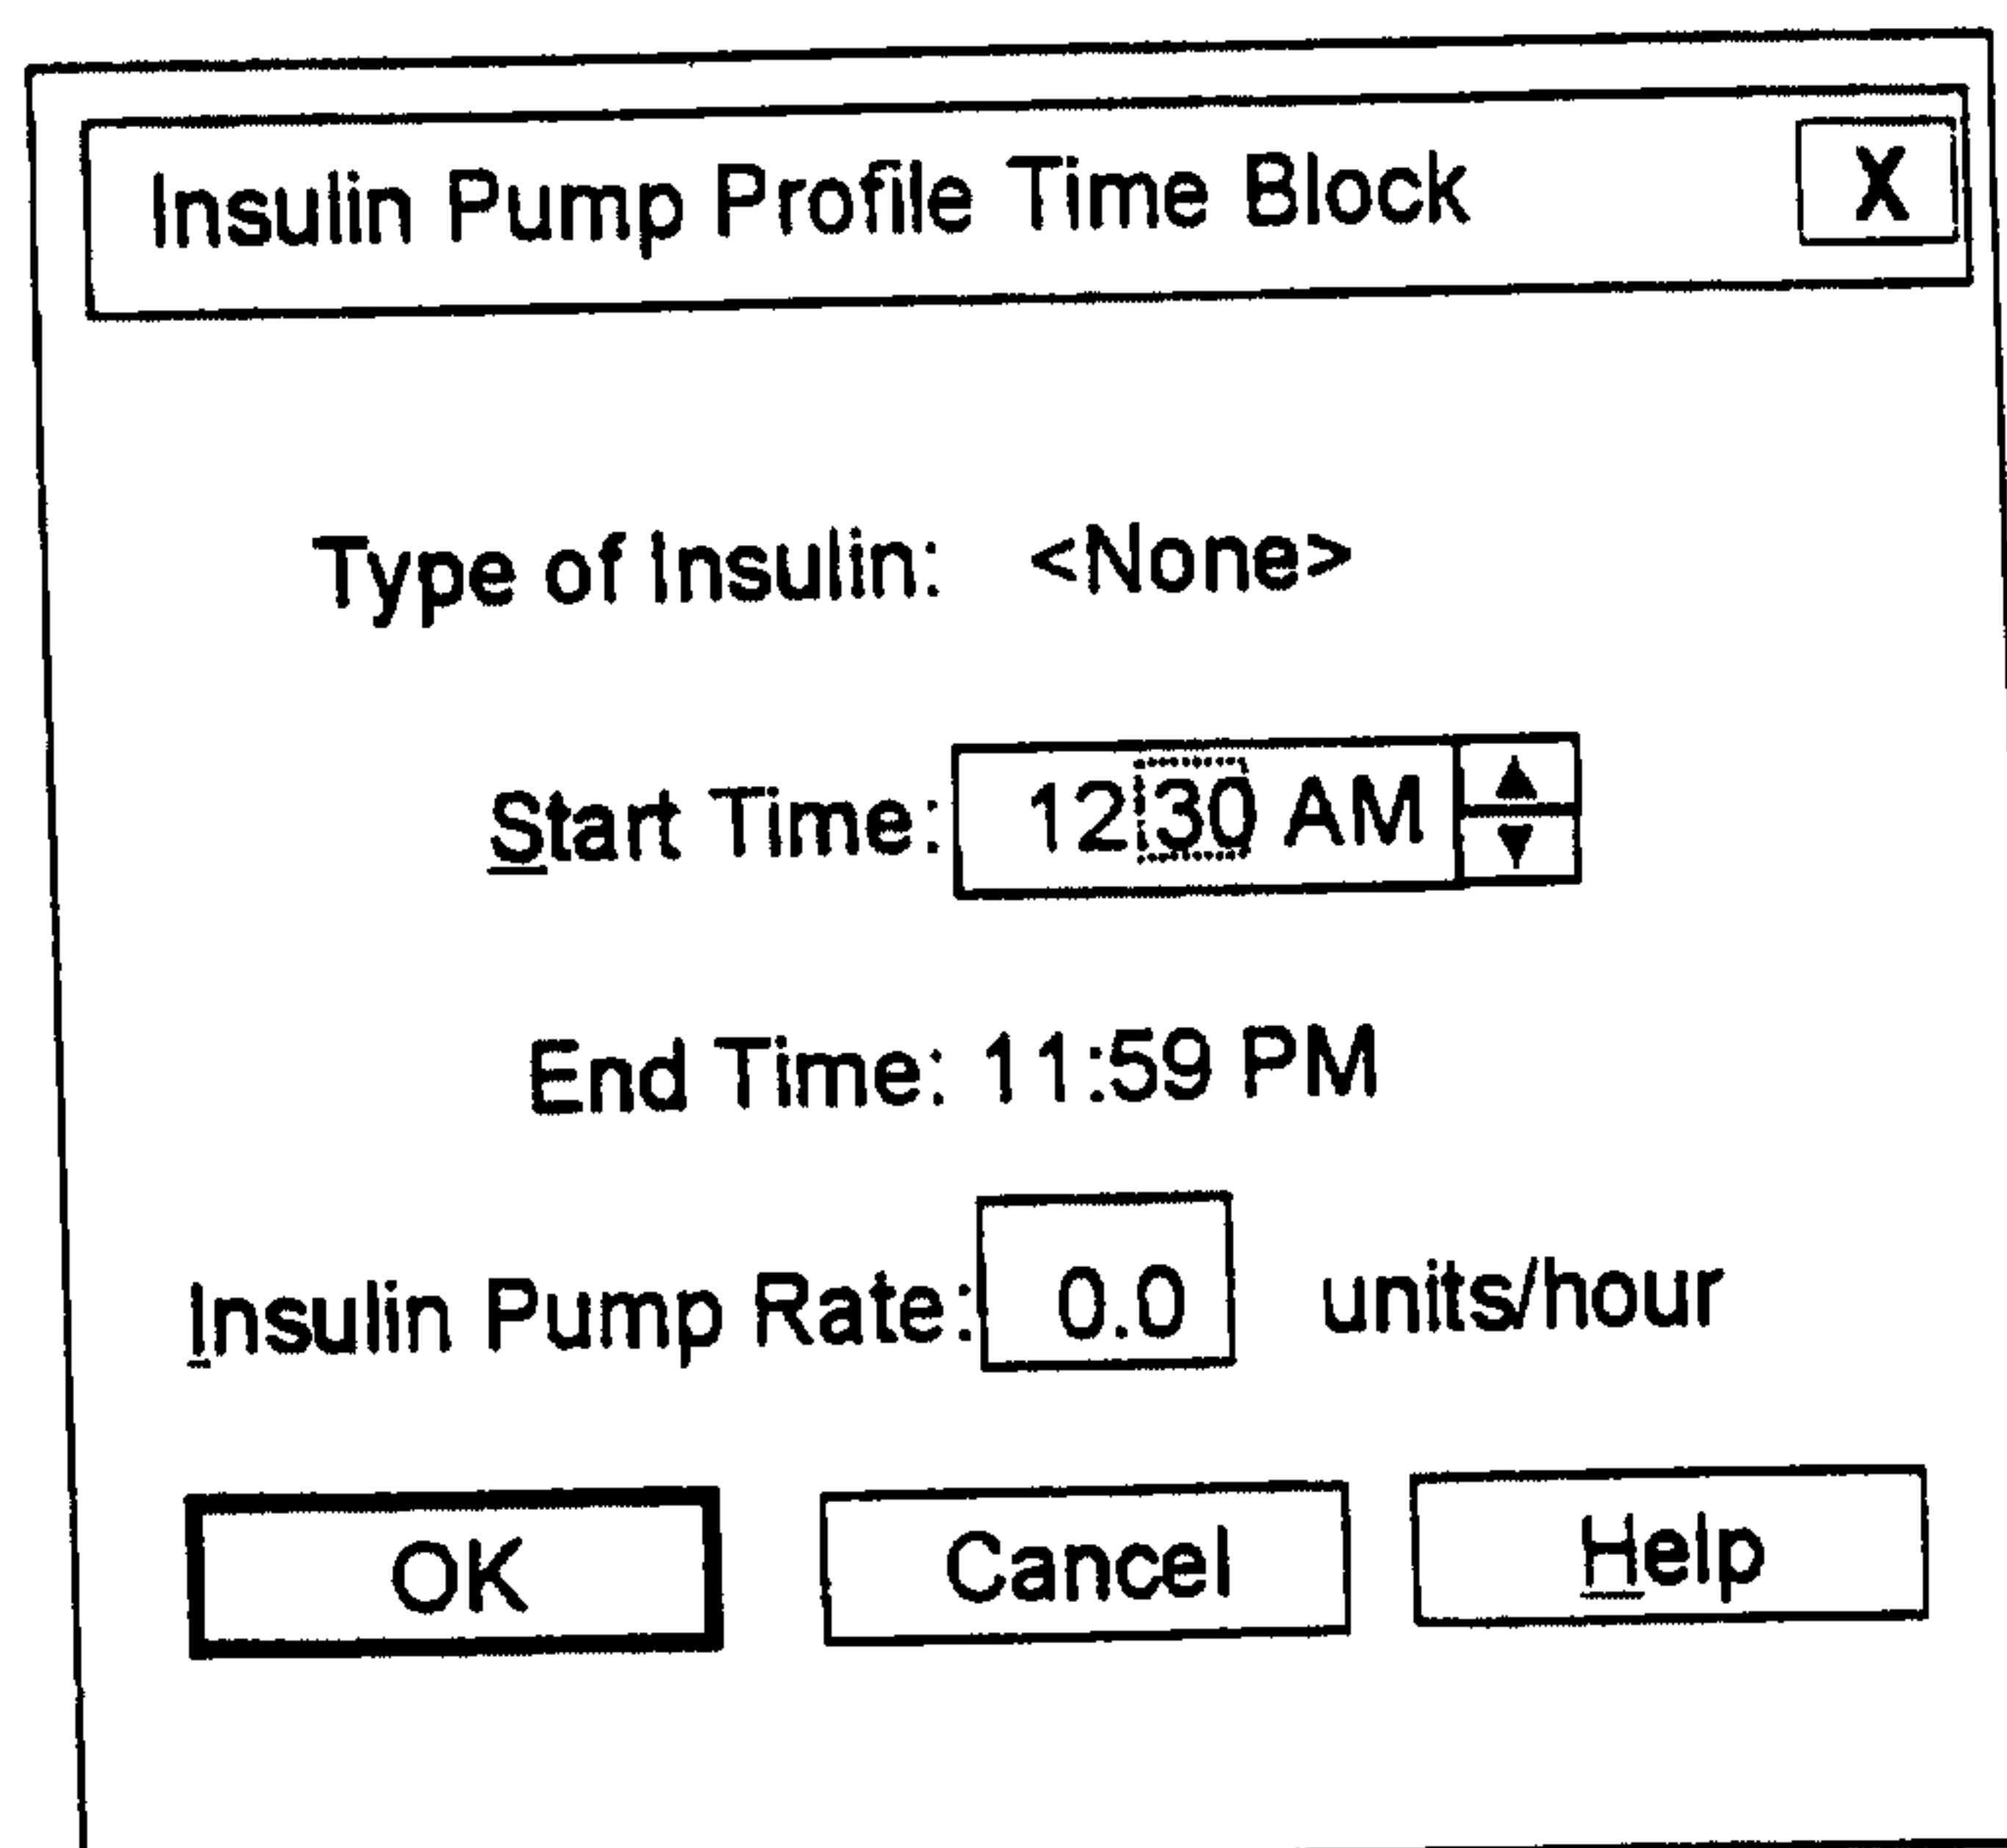Fig. 12

A dialog box titled "Insulin Pump Profile Time Block" with a close button (X) in the top right corner. It contains fields for "Type of Insulin" (set to "<None>"), "Start Time" (12:30 AM with a time picker), "End Time" (11:59 PM), and "Insulin Pump Rate" (0.0 units/hour). At the bottom are "OK", "Cancel", and "Help" buttons.

Insulin Pump Profile Time Block [X]

Type of Insulin: <None>

Start Time: 12:30 AM [time picker]

End Time: 11:59 PM

Insulin Pump Rate: 0.0 units/hour

OK Cancel Help

Fig. 13

9/44

Fig. 14

Meter Setup Wizard - Misc. Options

Select the appropriate Meter Customization Options

Decimal Format —

☐ Comma [,] ☒ Period [.]

Time Format —

☐ 24 Hour ☒ 12 Hour

Date Format —

☐ dd-mm-yy ☒ mm-dd-yy

Meter Back Light —

☐ Off ☒ On

Beeper —

☐ Off ☒ On

< Back Next > Cancel Help

Fig. 15

Meter Setup Wizard - Languages

Select four Languages for the Meter Setup.

Languages

☐ Dutch

☒ English

☒ French

☒ German

☐ Italian

☒ Spanish

☐ Swedish

< Back Next > Cancel Help

Fig. 16

Fig. 17

Custom Tip Messages

Custom Tip Messages List:

- new tip message
- new tip message ddd

Add...


Edit...

Remove


Close

Help

11/44

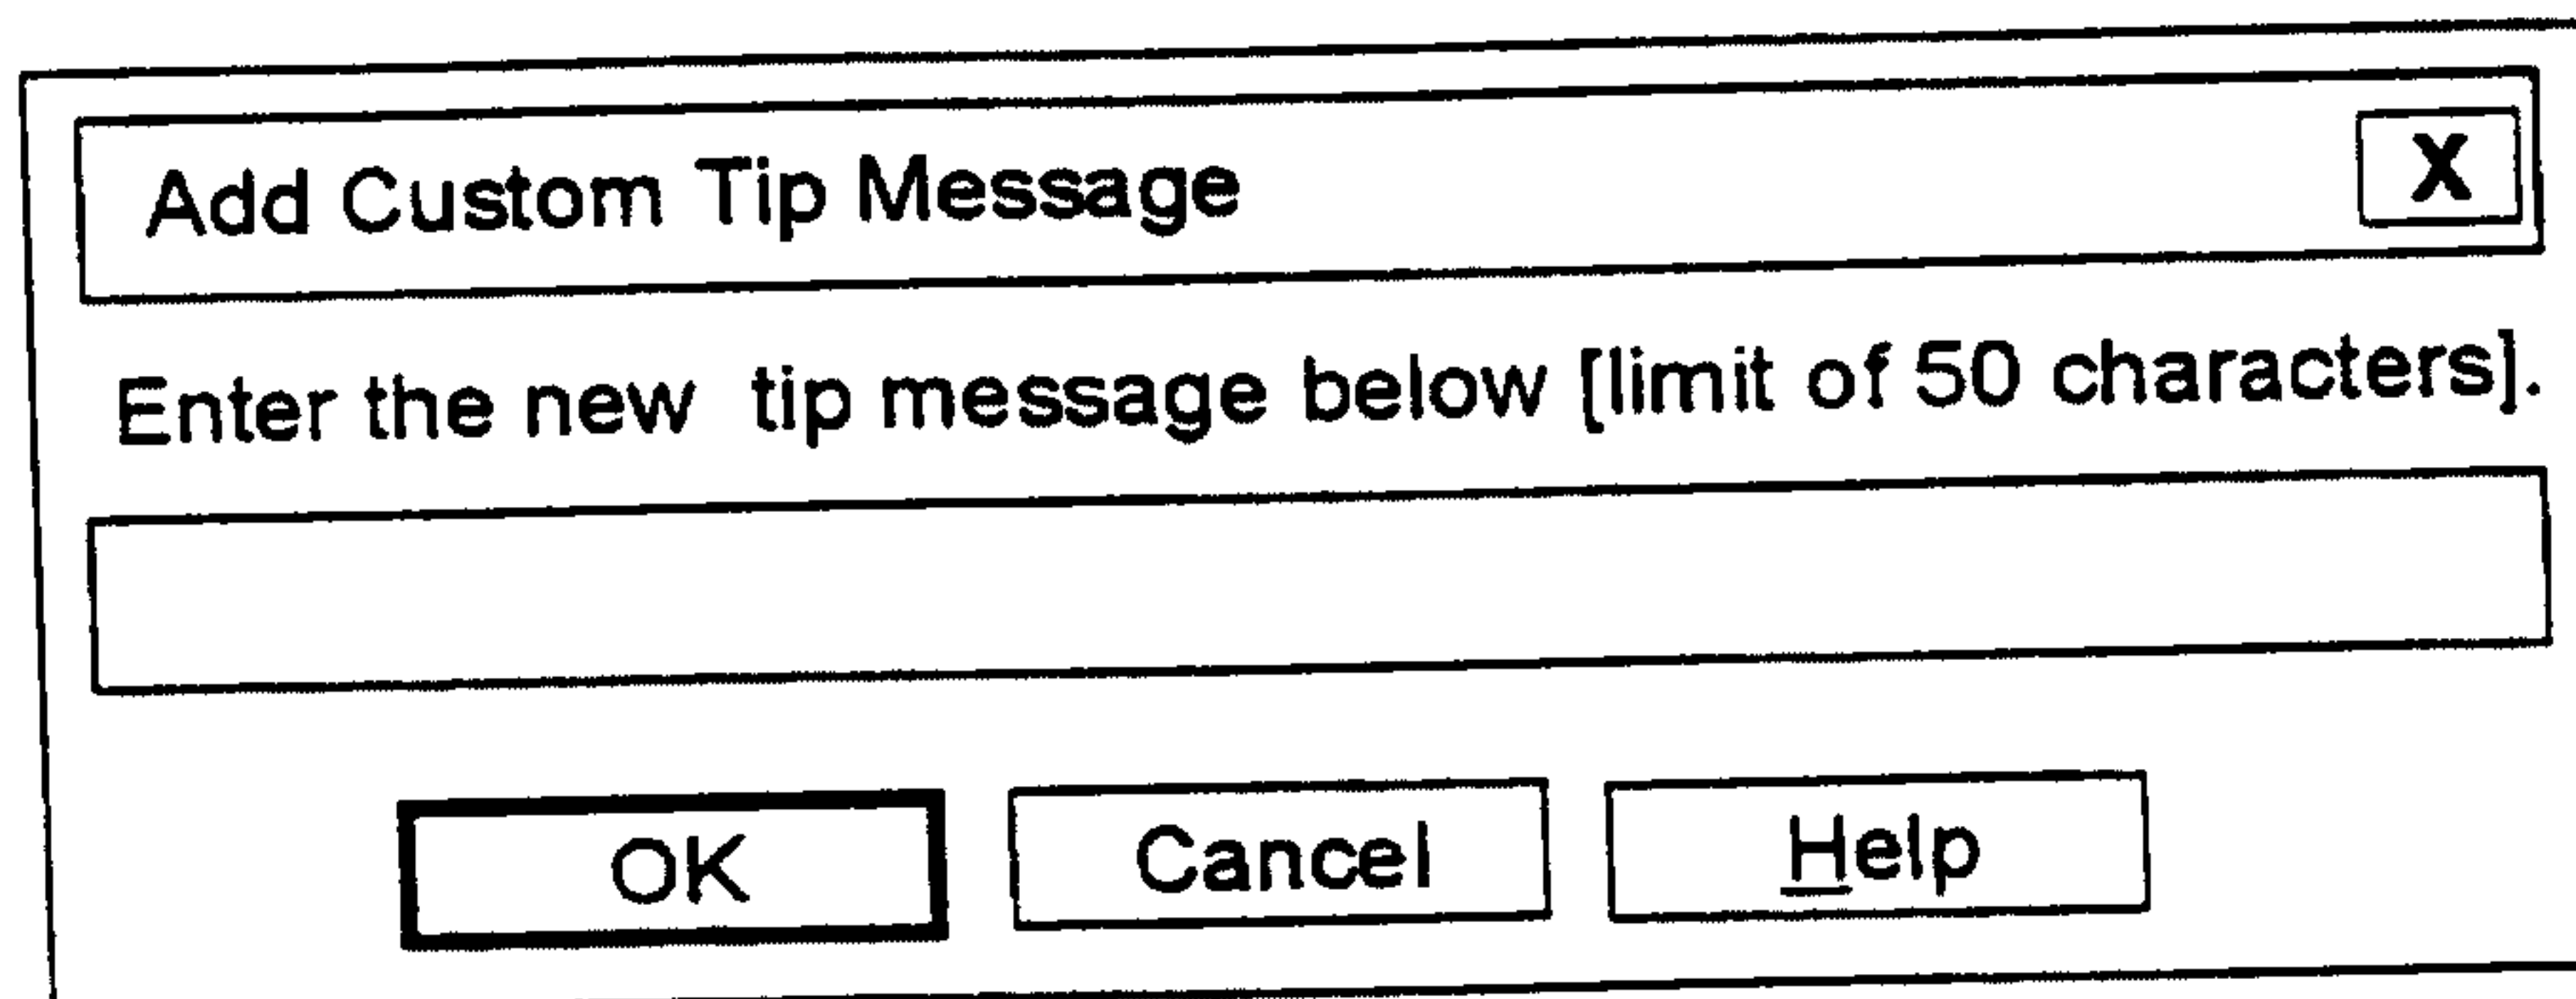

A dialog box titled "Add Custom Tip Message" with a close button (X) in the top right corner. Below the title bar, the text "Enter the new tip message below [limit of 50 characters]." is displayed. Underneath this text is a single-line text input field. At the bottom of the dialog box are three buttons: "OK", "Cancel", and "Help".

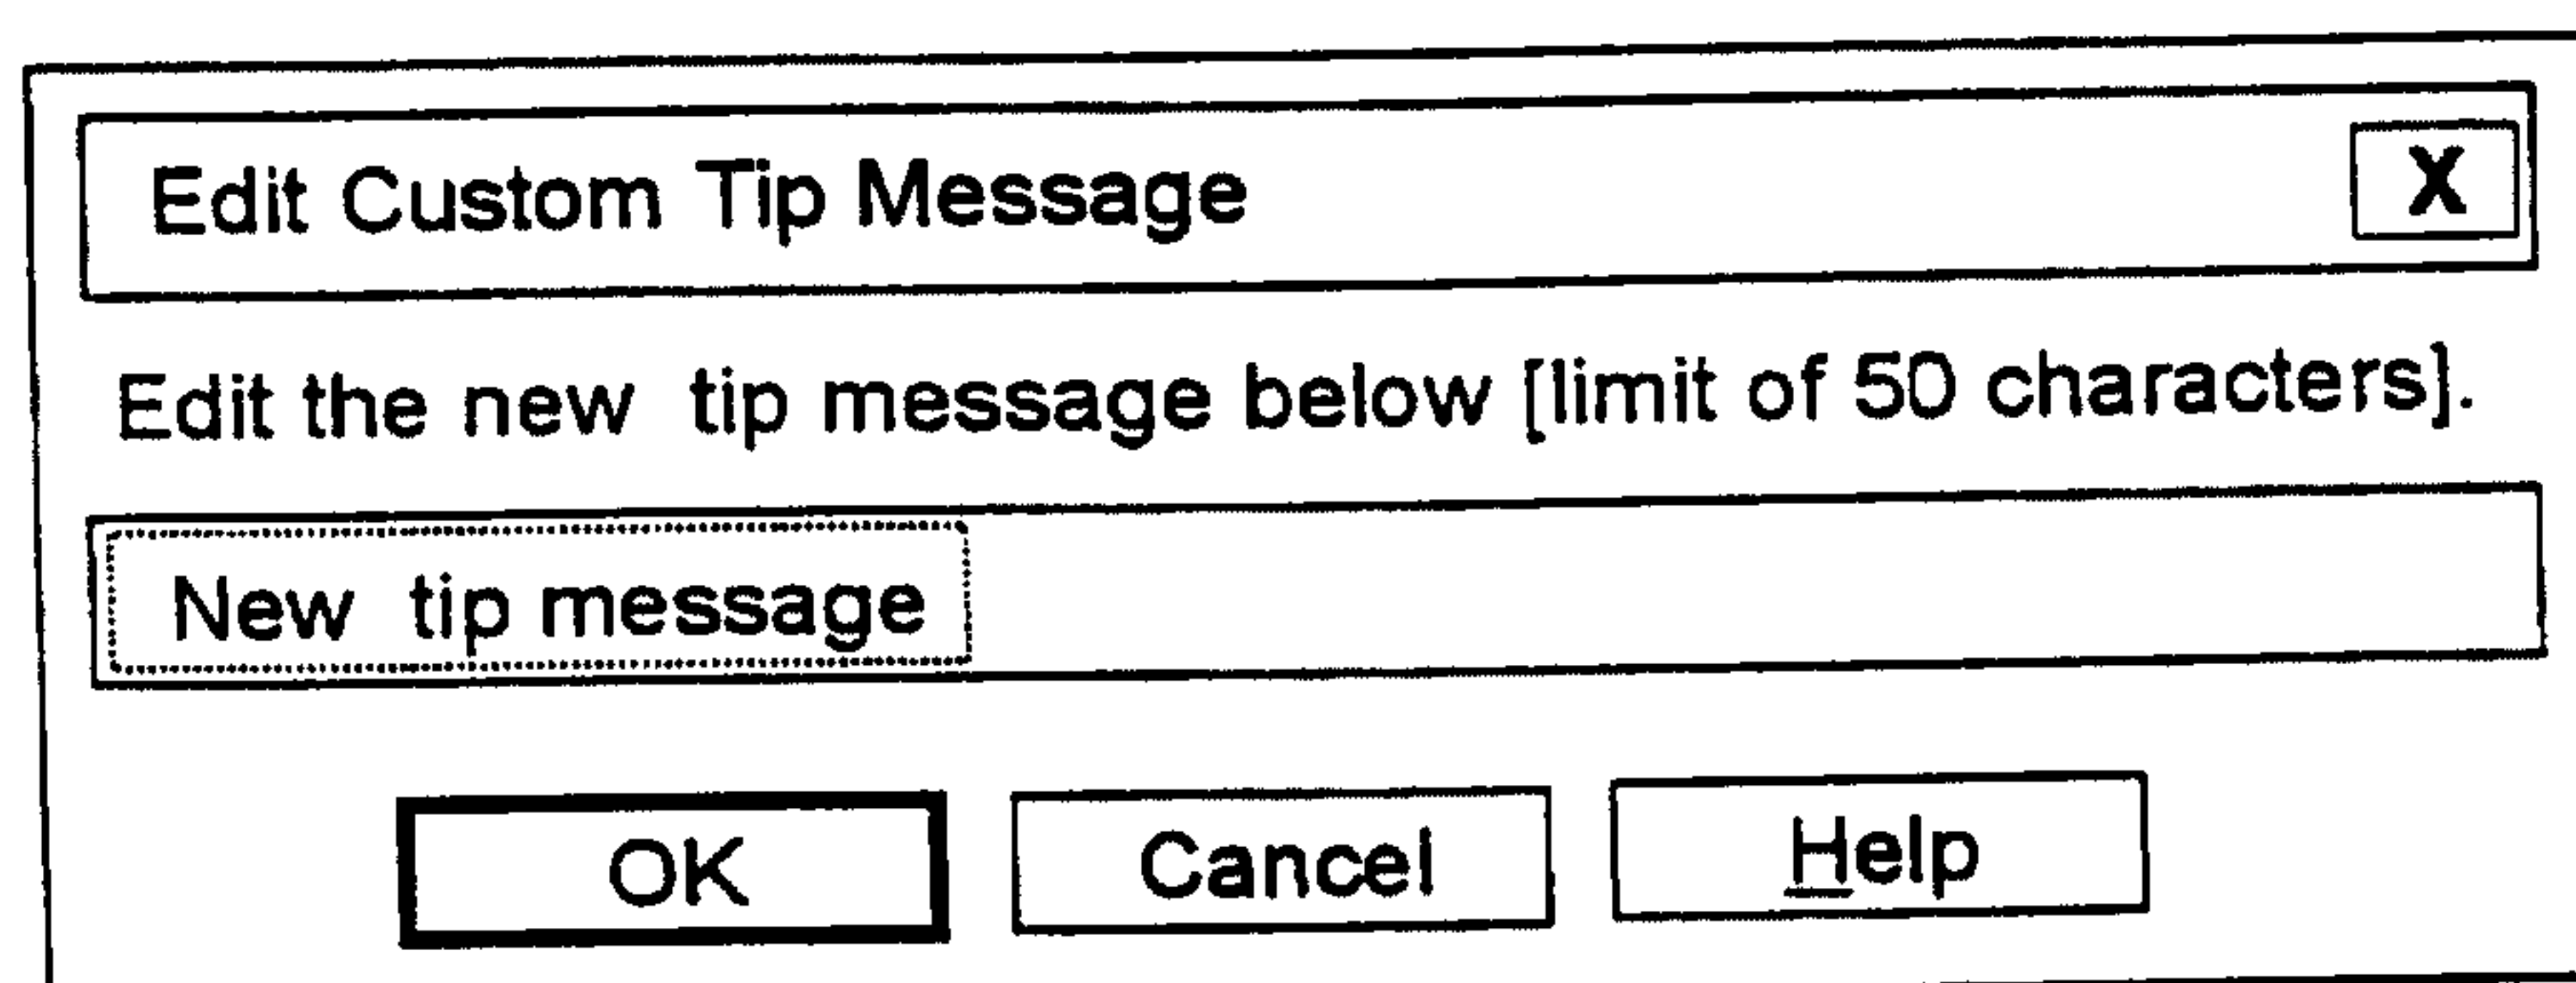Fig. 18

A dialog box titled "Edit Custom Tip Message" with a close button (X) in the top right corner. Below the title bar, the text "Edit the new tip message below [limit of 50 characters]." is displayed. Underneath this text is a single-line text input field containing the text "New tip message". At the bottom of the dialog box are three buttons: "OK", "Cancel", and "Help".

Fig. 19

12/44

Meter Setup Wizard - Complete Meter Setup

You have finished selecting the Meter Options.

Select the "Finish" button to view the options selected.

To save the options selected [after viewing]:

From the File menu select 'Save' to save to a file.

From the Meter menu, select 'Send Meter Setup' to send the options to a meter that is connected to the computer.

Fig. 20

13/44

-Accutivity Meter Setup Manager

File Meter View Help

Summary of Meter Setup
(Select underlined text to make changes)

Personal:

Patient Name	John Smith
Patient ID	default
Healthcare Computer	
Phone Number	default

Glucose Units/Ranges:

Units of Measure	mg/dL
Upper Limit	0
Lower Limit	0
Hypo	0

Insulin Type:

Insulin Logging	Disabled
Insulin Type 1	< None >
Insulin Type 2	< None >
Insulin Type 3	< None >
Insulin Increments	0.1 units

Event Markers:

Before Meal	
After Meal	
Fasting	

For Help, press F1

NUM

Fig. 21

14/44

Fig. 22

Instructions on what to do on each screen appear here.

Interaction

OK Cancel Apply Help

Fig. 23

Accutivity Meter Setup Manager

Time Block Insulin Pump Profile Misc Options Language Tip Messages

Personal Glucose Units/Ranges Insulin Type Event Markers

Enter the Patient and Healthcare Provider Information below.

The Patient ID may be a number or a name that is up to 20 characters in length.

Patient Information

Name: John Smith

ID: default

Healthcare Provider Information:

Healthcare Computer Phone Number: default

OK Cancel Help

15/44

Fig. 24

Accutivity Meter Setup Manager [X]

Time Block | Insulin Pump Profile | Misc Options | Language | Tip Messages

Personal | **Glucose Units/Ranges** | Insulin Type | Event Markers

Units of Measure

Glucose: ☒ mg/dL ☐ mmol/L

Glucose Limits

Upper Limit: mg/dL

Lower Limit: mg/dL

Hypo: mg/dL

OK Cancel Help

Fig. 25

Accutivity Meter Setup Manager [X]

Time Block | Insulin Pump Profile | Misc Options | Language | Tip Messages

Personal | Glucose Units/Ranges | **Insulin Type** | Event Markers

Select up to three Insulin Types. These will be the only types available in the meter.

Check the Insulin Logging box if you want to record insulin information in your meter.

☐ Insulin Logging Enabled for Meter Setup

Insulin Types

Insulin Type 1: Insulin Type 2: Insulin Type 3:

Insulin Increment:

☒ Tenth Unit ☐ Half Unit ☐ Whole Unit

OK Cancel Help

16/44

Accutivity Meter Setup Manager [X]

Time Block | Insulin Pump Profile | Misc Options | Language | Tip Messages

Personal | Glucose Units/Ranges | Insulin Type | Event Markers

Select up to 15 Event Markers to add to the Meter Setup

The Events will appear in the meter in the order they appear in the 'Events To Load Into Meter' list.

You have selected 15 Events

S	Available Events ▲		Events to Load into Meter
	Active		Before Meal
	After Breakfast		After Meal
	After Dinner		Fasting
✓	After Exercise	Add >	Snack
	After Lunch		Feel Hypo.
✓	After Meal	<Remove	Before Exercise
	Bed Time		After Exercise
	Before Brekfast		Illness
	Before Dinner		Invalid Test
✓	Before Exercise		Other's Result
	Before Lunch		User Defined
✓	Before Meal		Stress
	Cold Outdoors		L1 Control
	Different Food		L2 Control
	Drank Alcohol		Oral Medication

S = Selected Event Markers

OK Cancel Help

Fig. 26

17/44

Accutivity Meter Setup Manager
X

Personal
Glucose Units/Ranges
Insulin Type
Event Markers

Time Block
Insulin Pump Profile
Misc Options
Language
Tip Messages

Time Block information is contained in the list below.

The minimum time span for a Time Block is 1/2 hour.

Editing the start time of a Time Block automatically adjusts the end time of the previous Time Block. No Time gaps are allowed between Time Blocks.

To edit an existing Time Block, select the Time Block and press the Edit button, or double click on the Time Block entry in the list.

Time Block Name	3 Letter Name	Start Time	End Time	Duration
Breakfast	Brk	6:00 AM	8:59 AM	3.0
Midmorning	Mmo	9:00 AM	11:59 AM	3.0
Lunch	Lun	12:00 PM	2:59 PM	3.0
Midafternoon	Maf	3:00 PM	5:59 PM	3.0
Dinner	Din	6:00 PM	7:59 PM	2.0
Evening	Eve	8:00 PM	9:59 PM	2.0
Bed time	Bed	10:00 PM	2:59 AM	5.0
Night time	Ngt	3:00 AM	5:59 AM	3.0

Edit...

OK
Cancel
Help

Fig. 27

18/44

Time Block Information X

Three Letter Name: Brk

Start time: 6:00 AM ▲▼ End Time: 8:59 AM

Customize Time Block

Insulin Type 1: <None>	Dose	0.0
Insulin Type 2: <None>	Dose	0.0
Insulin Type 3: <None>	Dose	0.0

Exercise Type: <None> ▼ Duration: 0:00 ▲▼

Carbohydrates: 0 grams

Event 1: No Event ▼ Event 3: No Event ▼

Event 2: No Event ▼ Event 4: No Event ▼

OK Cancel Help

Fig. 28

19/44

Accutivity Meter Setup Manager X

Personal
Glucose Units/Ranges
Insulin Type
Event Markers

Time Block
Insulin Pump Profile
Misc Options
Language
Tip Messages

Check the Insulin Pump Logging box is you want to record Insulin Pump Information in your meter:

☒ Insulin Pump Logging Enabled in Meter Setup

Type of Insulin: 10/90 ▼

Profile Start Date: 11/09/97 ▲▼ Profile Start Date: 2:50 PM ▲▼

Time Block Name	Start Time	End Time	Pump Rate
Time Block #1	12:00 AM	12:29 AM	0.0
Time Block #2	12:30 AM	11:59 PM	0.0

Insert
Edit...
Delete

OK
Cancel
Help

Fig. 29

20/44

Accutivity Meter Setup Manager X

Personal Glucose Units/Ranges Insulin Type Event Markers
Time Block Insulin Pump Profile Misc Options Language Tip Messages

Select the appropriate Meter Customization Options

Decimal Format ☐ Comma [.] ☒ Period [.]

Time Format ☐ 24 Hour ☒ 12 Hour

Date Format ☐ dd-mm-yy ☒ mm-dd-yy

Meter Back Light ☐ Off ☒ On

Beeper ☐ Off ☒ On

OK Cancel Help

Fig. 30

21/44

Accutivity Meter Setup Manager

Personal Glucose Units/Ranges Insulin Type Event Markers

Time Block Insulin Pump Profile Misc Options Language Tip Messages

Select four Languages for the Meter Setup.

Languages

- ☐ Dutch
- ☒ English
- ☒ French
- ☒ German
- ☐ Italian
- ☒ Spanish
- ☐ Swedish

OK Cancel Help

Fig. 31

22/44

Accutility Meter Setup Manager [X]

Personal | Glucose Units/Ranges | Insulin Type | Event Markers
 Time Block | Insulin Pump Profile | Misc Options | Language | **Tip Messages**

Select 10 Tip Messages to add to the Meter Setup from the list below.
 To add Custom Tip Messages to the list below, select the 'Custom' button

☒ Tip Messages Enabled for Meter Setup

You have selected 10 Tip Messages.

S	C	Available Events
✓		Check your feet daily
✓		Choose a nutrition goal you can already do
✓		Choose an exercise goal you can already do
		Exercise helps keep your blood sugars in range
✓		Exercise is important for good diabetes management
✓		Exercise makes you more fit
		Ketones provide you with important information
		See your dentist every six months
✓		See your diabetes educator regularly
✓		See your doctor regularly
✓		See your eye doctor annually
✓		Tailor goals to fit your own lifestyle

S = Selected Tip Messages
 C = Custom Tip Messages


[Custom...]

[OK] [Cancel] [Help]

Fig. 32

View Patient Report		X
Patient Name	Serial number	Received
John Smith	0005040225	
File Path:		
		View
		Cancel
Browse...		Help

Fig. 33

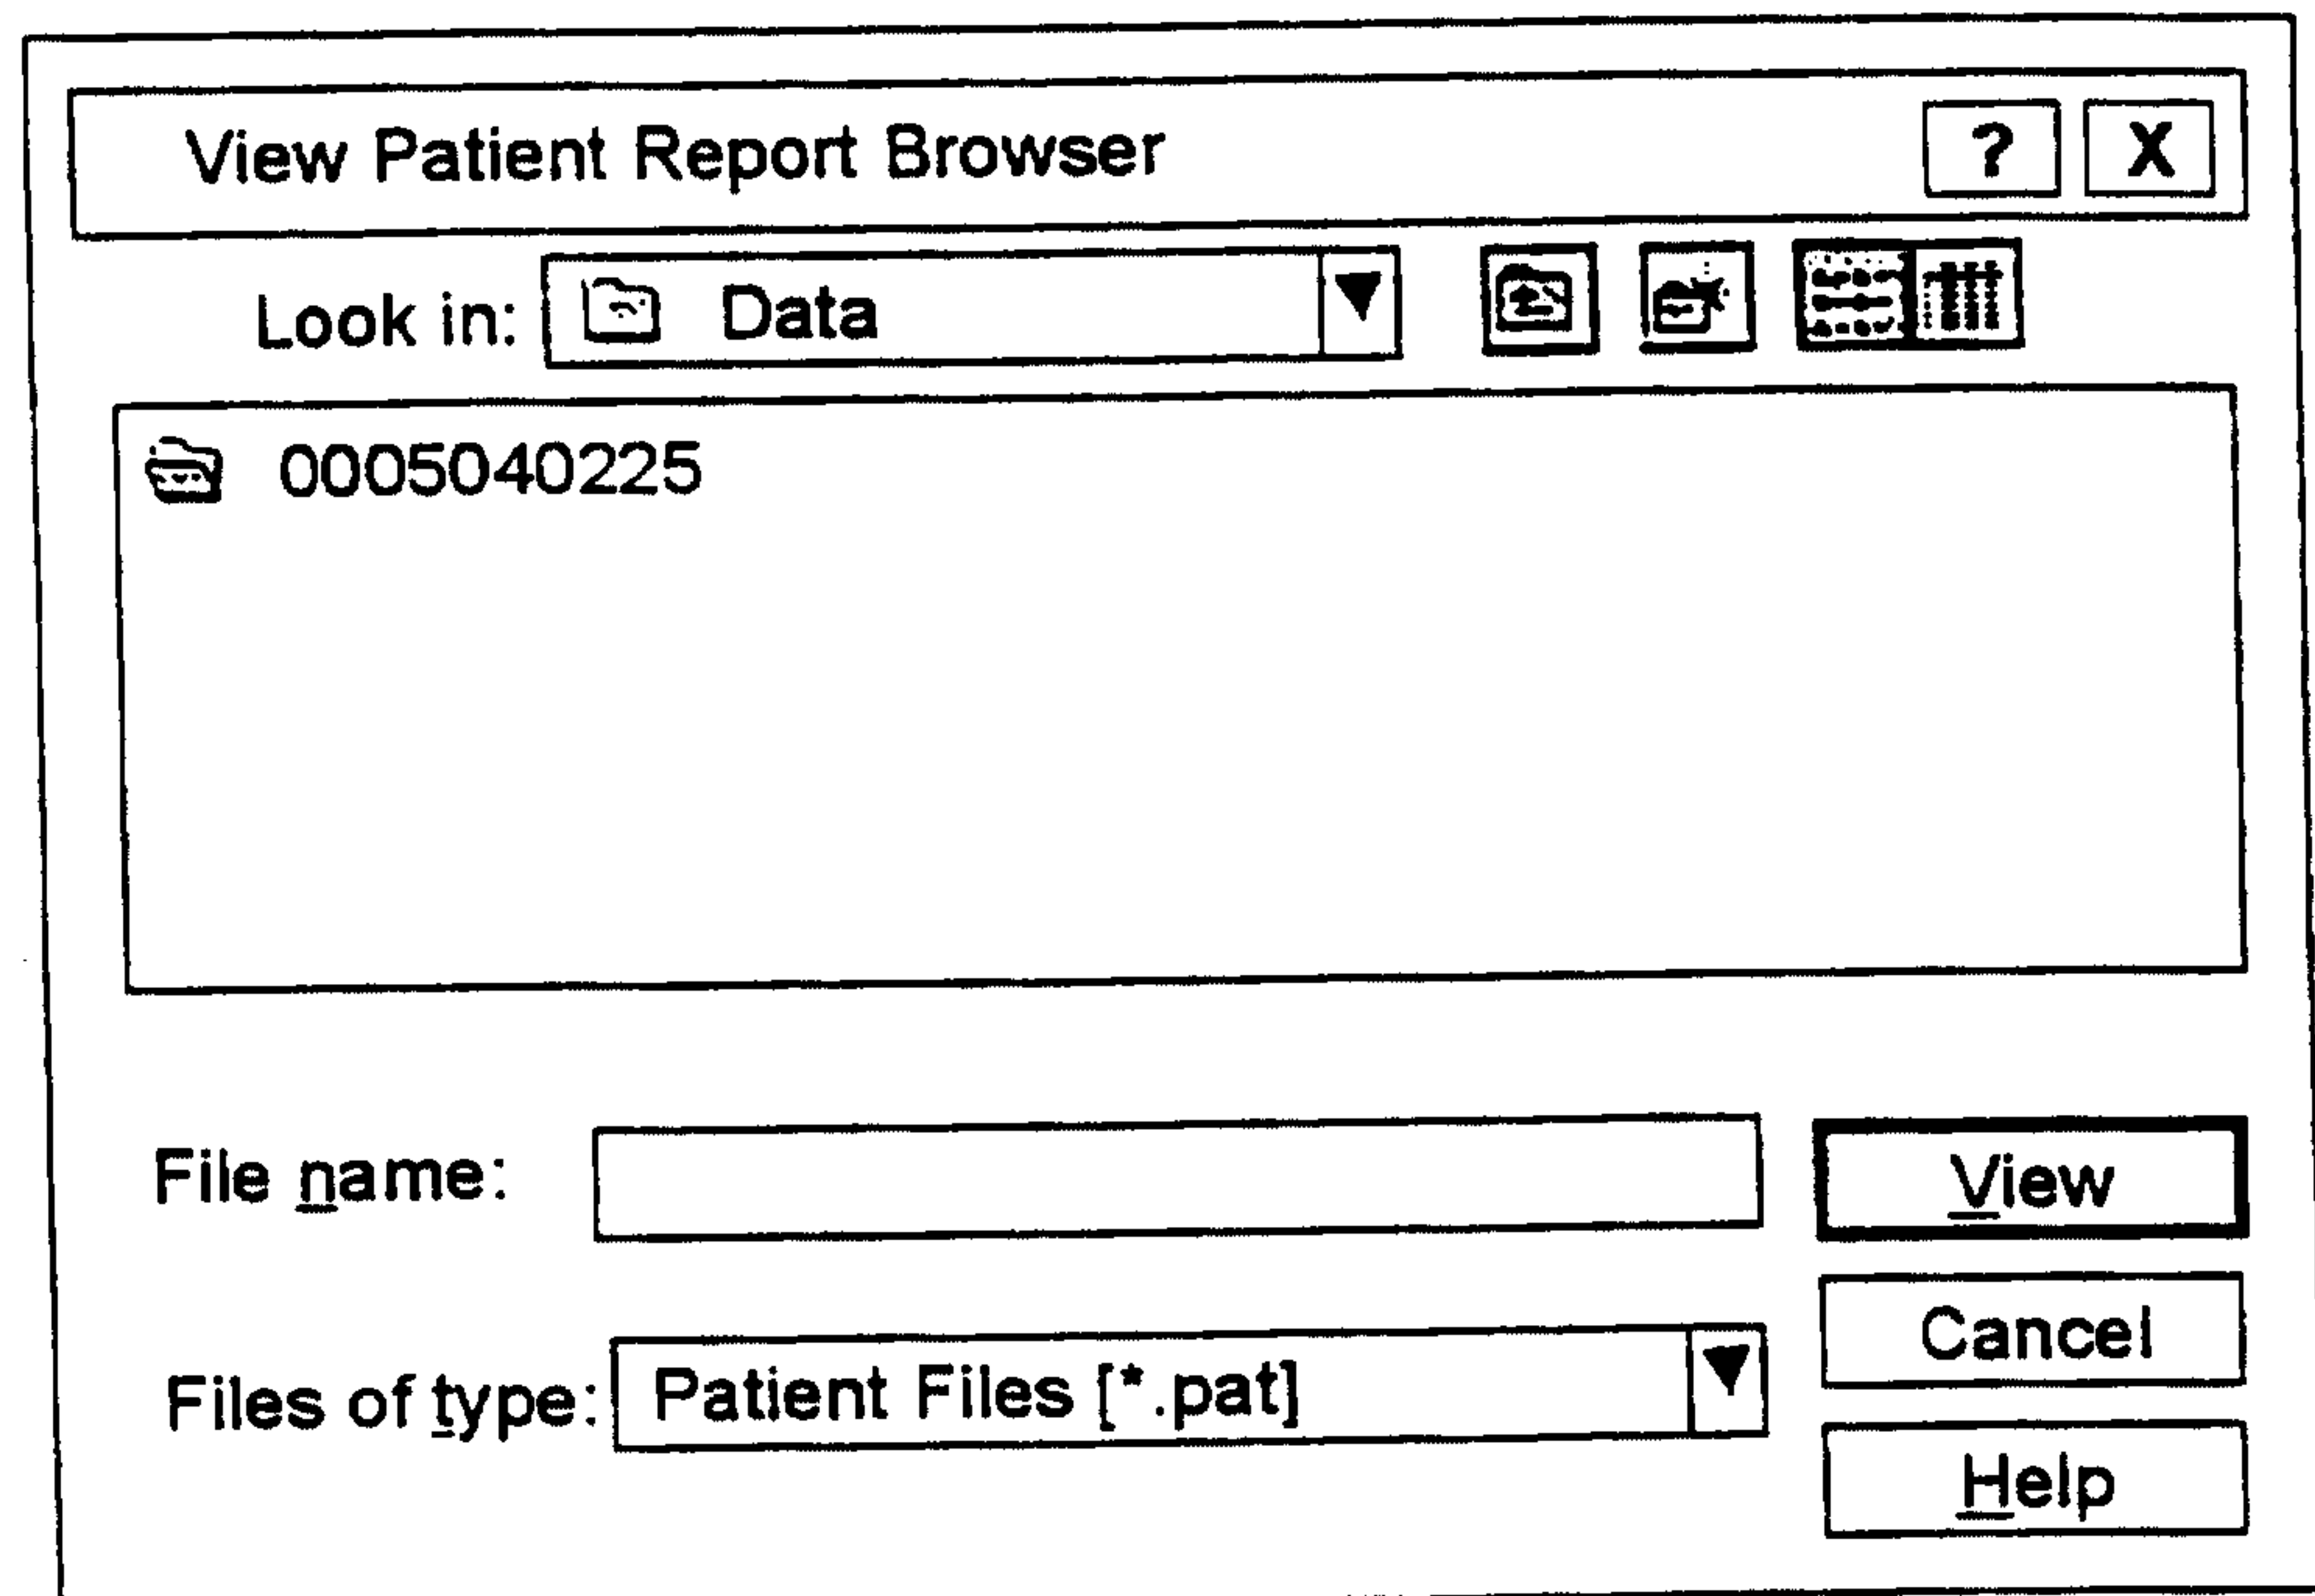*Fig. 34*

25/44

Print Patient Report		X
Patient Name	Serial number	Received
John Smith	0005040225	
File Path:		
		Print
		Cancel
Browse...		Help

Fig. 35

Print Patient Report Browser

Look in: Data

0005040225

File name:

Files of type: Patient Files (*.pat)

Print

Cancel

Help

Fig. 36

27/44

The dialog box titled "Edit Patient Name Database" contains a table with two columns: "Patient Name" and "Serial number". The first row of the table contains the text "tracy" and "1230123456". To the right of the table are three buttons: "Add...", "Edit...", and "Remove". Below these buttons are two more buttons: "Close" and "Help". A close button with an "X" icon is located in the top right corner of the dialog box.

Patient Name	Serial number
tracy	1230123456

Buttons: Add..., Edit..., Remove, Close, Help

Fig. 37

The dialog box titled "Add/Edit Patient Name" contains two input fields. The first field is labeled "Patient Name:" and the second field is labeled "Meter Serial Number:". Below the input fields are three buttons: "OK", "Cancel", and "Help". A close button with an "X" icon is located in the top right corner of the dialog box.

Labels: Patient Name:, Meter Serial Number:

Buttons: OK, Cancel, Help

Fig. 38

28/44

Options [X]

Report Settings New Meter Setup Meter COM Port Startup

Report Formats

- ☒ Diary
- ☐ Glucose Values
- ☐ Trend
- ☐ Glucose Graph
- ☐ Average Trend
- ☐ Glucose Ranges
- ☐ Hypoglycemic Events

Range for Average Trend. Glucose Ranges and Hypo Events reports

48 hours ▼


Glucose Units

- ☒ mg/dL
- ☐ mmol/L

OK Cancel Help

Fig. 39

29/44

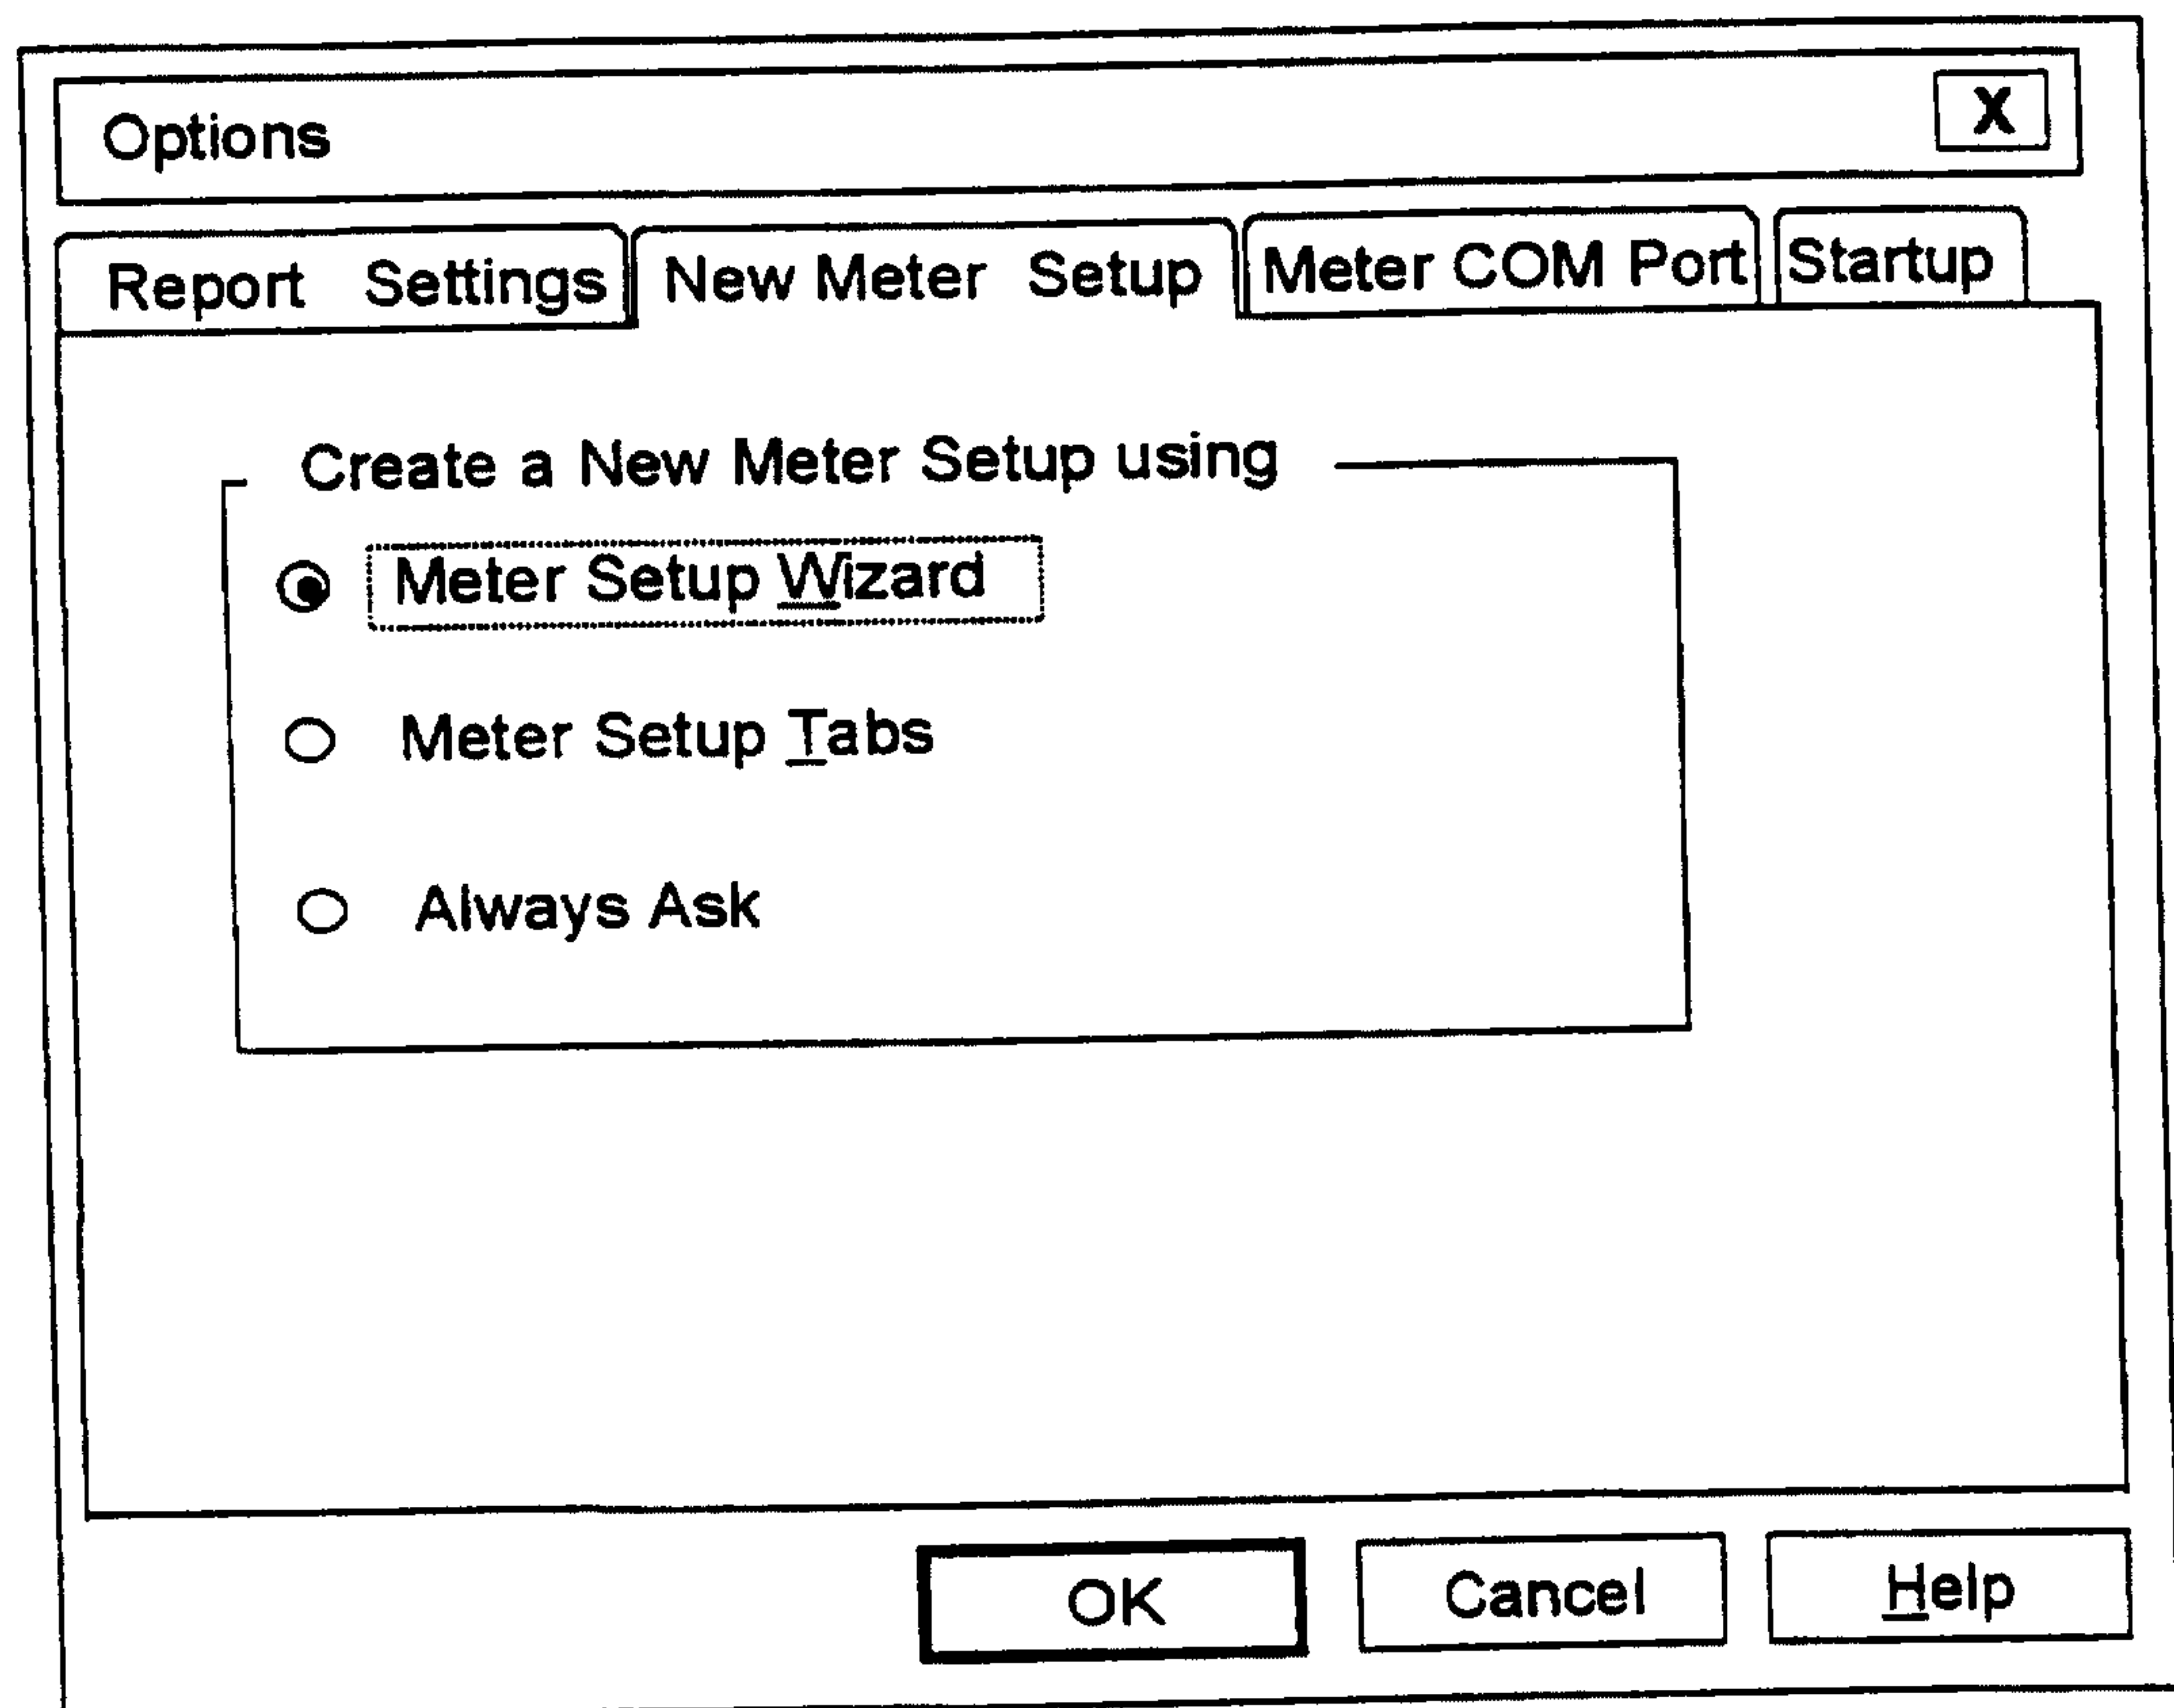*Fig. 40*

30/44

Options [X]

Report Settings New Meter Setup Meter COM Port Startup

COM Port



☒ COM1 ☐ COM3

☐ COM2 ☐ COM4

OK Cancel Help

Fig. 41

31/44

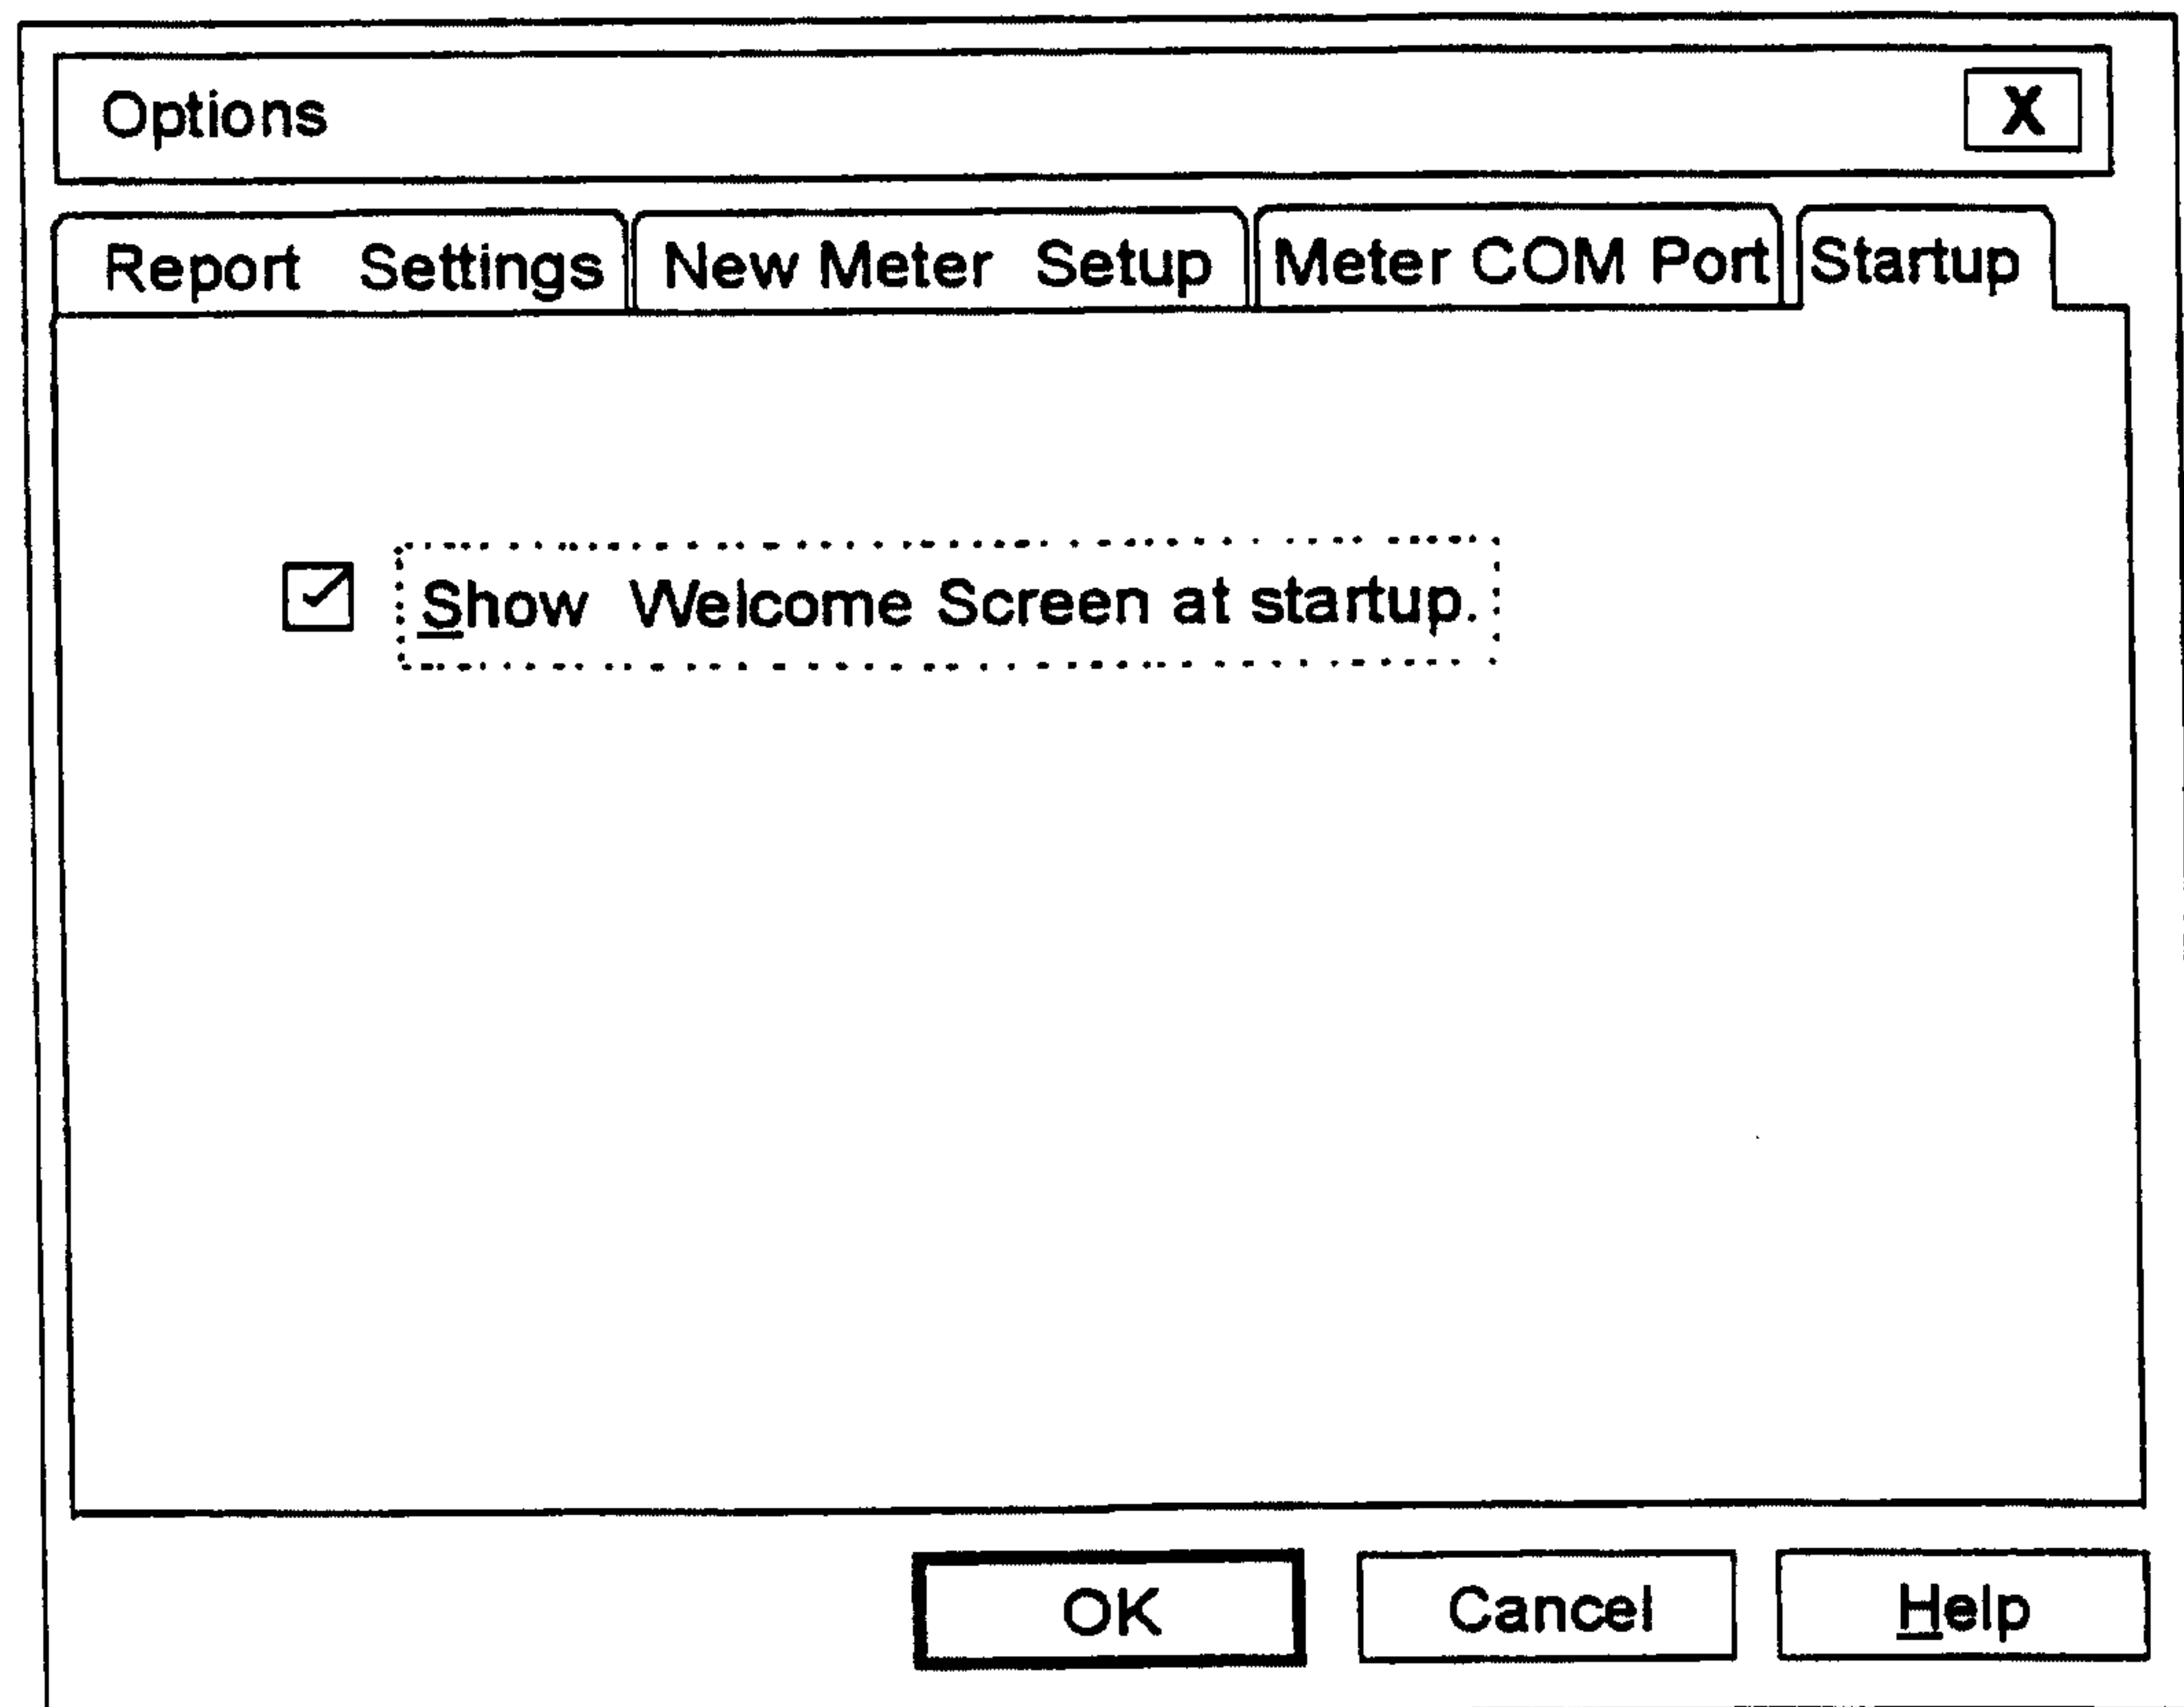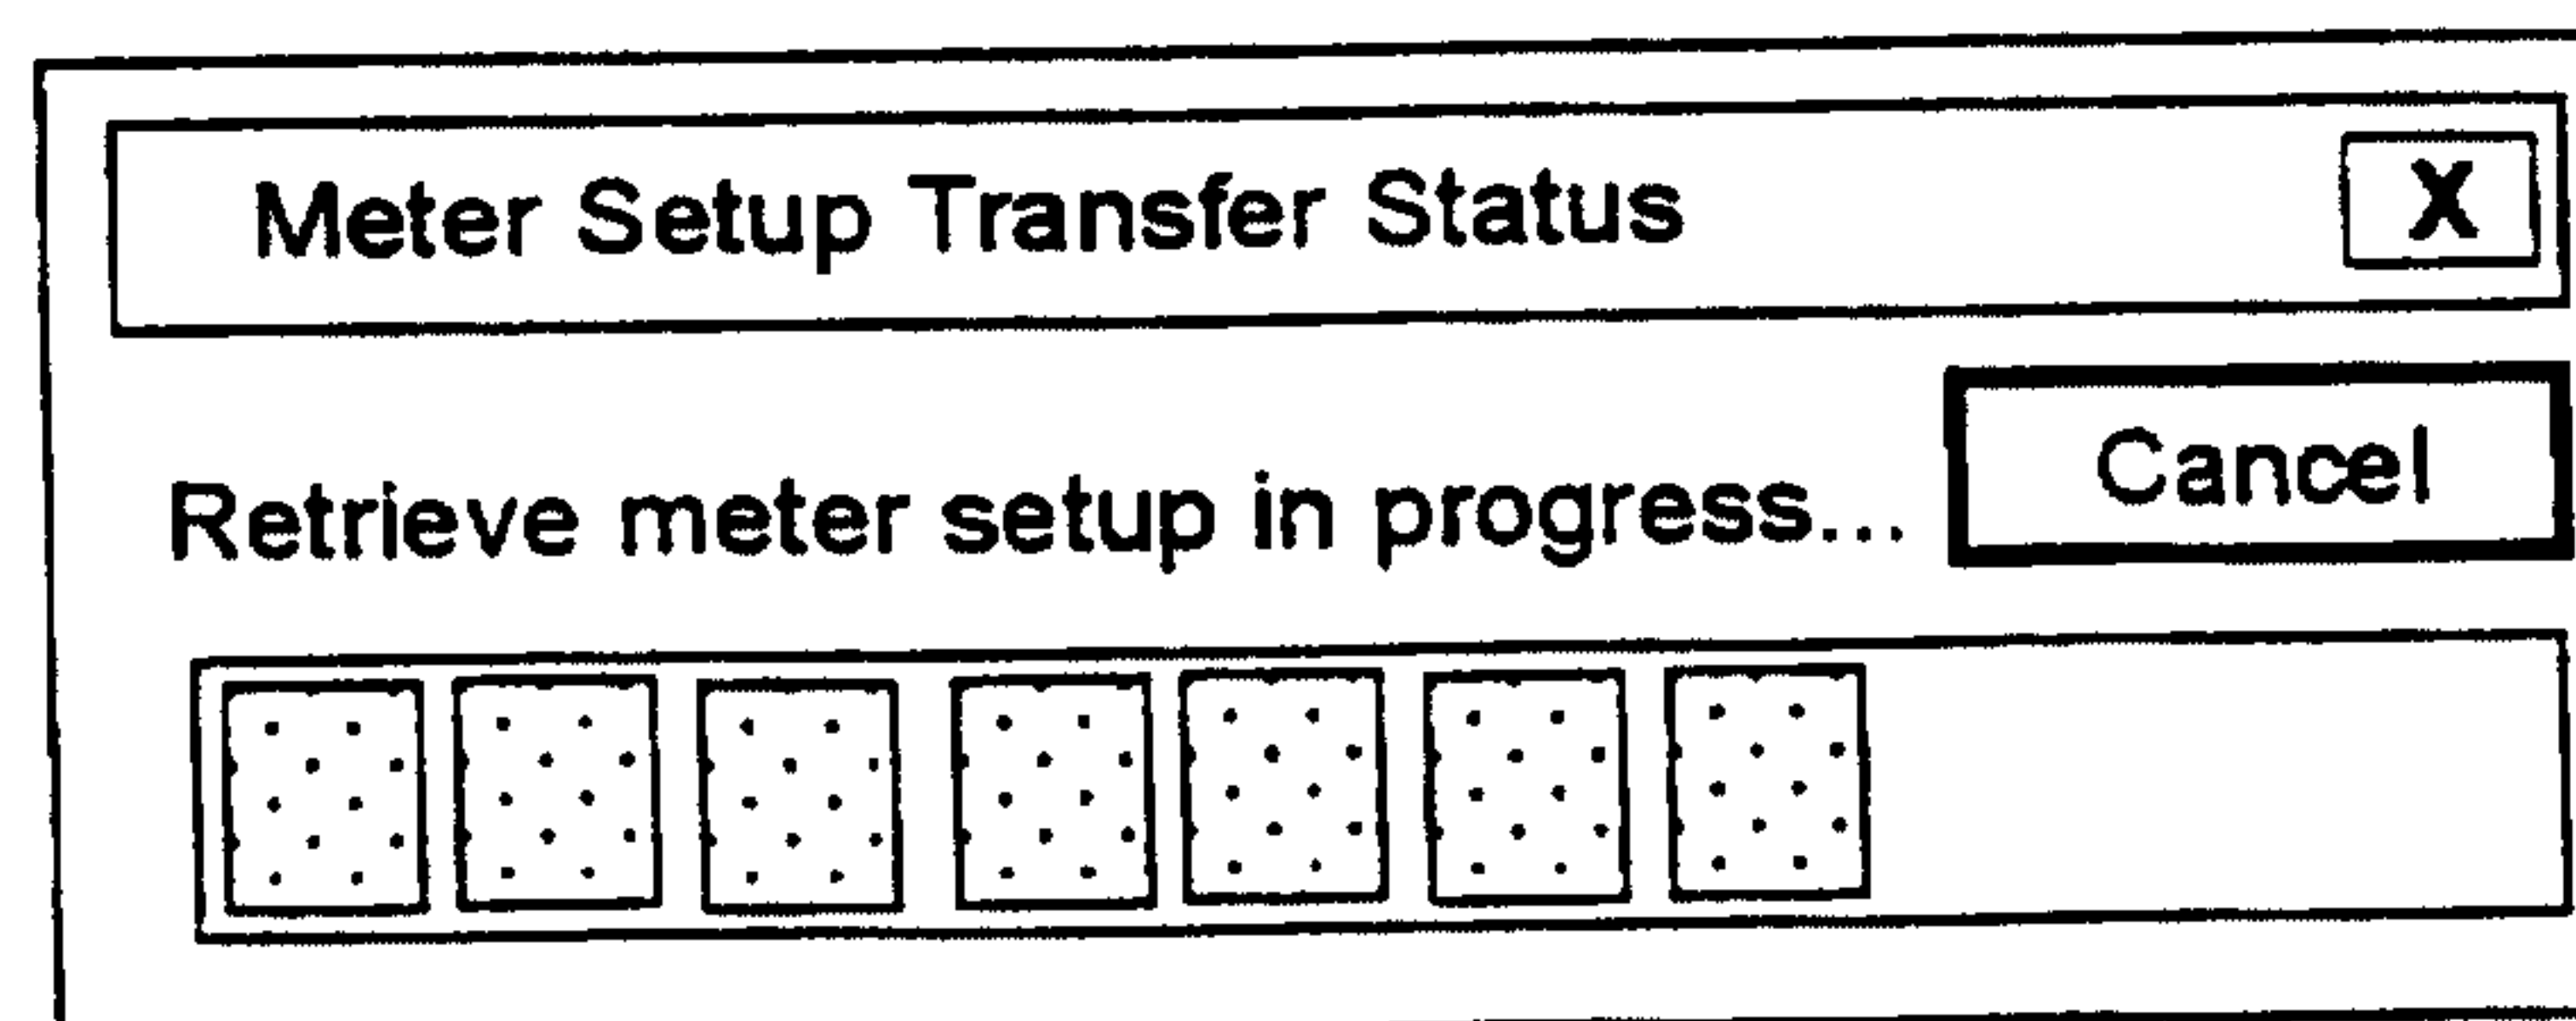*Fig. 42**Fig. 43*

32/44

Enter Patient Name X

The meter serial number has no corresponding patient name. Please enter the patient's name.

Meter Serial Number: 0005040225

Patient Name:

OK Cancel Help

Fig. 44

Meter Date and Time [X]

Computer Settings

Date: 11/9/98
Time: 3:45 PM

Meter Settings

Date: 11/9/98
Time: 3:46 PM

Set Date and Time

☒ Do not change Meter Settings

☐ Synchronize Meter Settings with Computer Settings

☐ Set new Meter Date and Time:


Date: 11/09/98 [▲▼]

Time: 3:45 PM [▲▼]


OK Cancel Help

Fig. 45

34/44

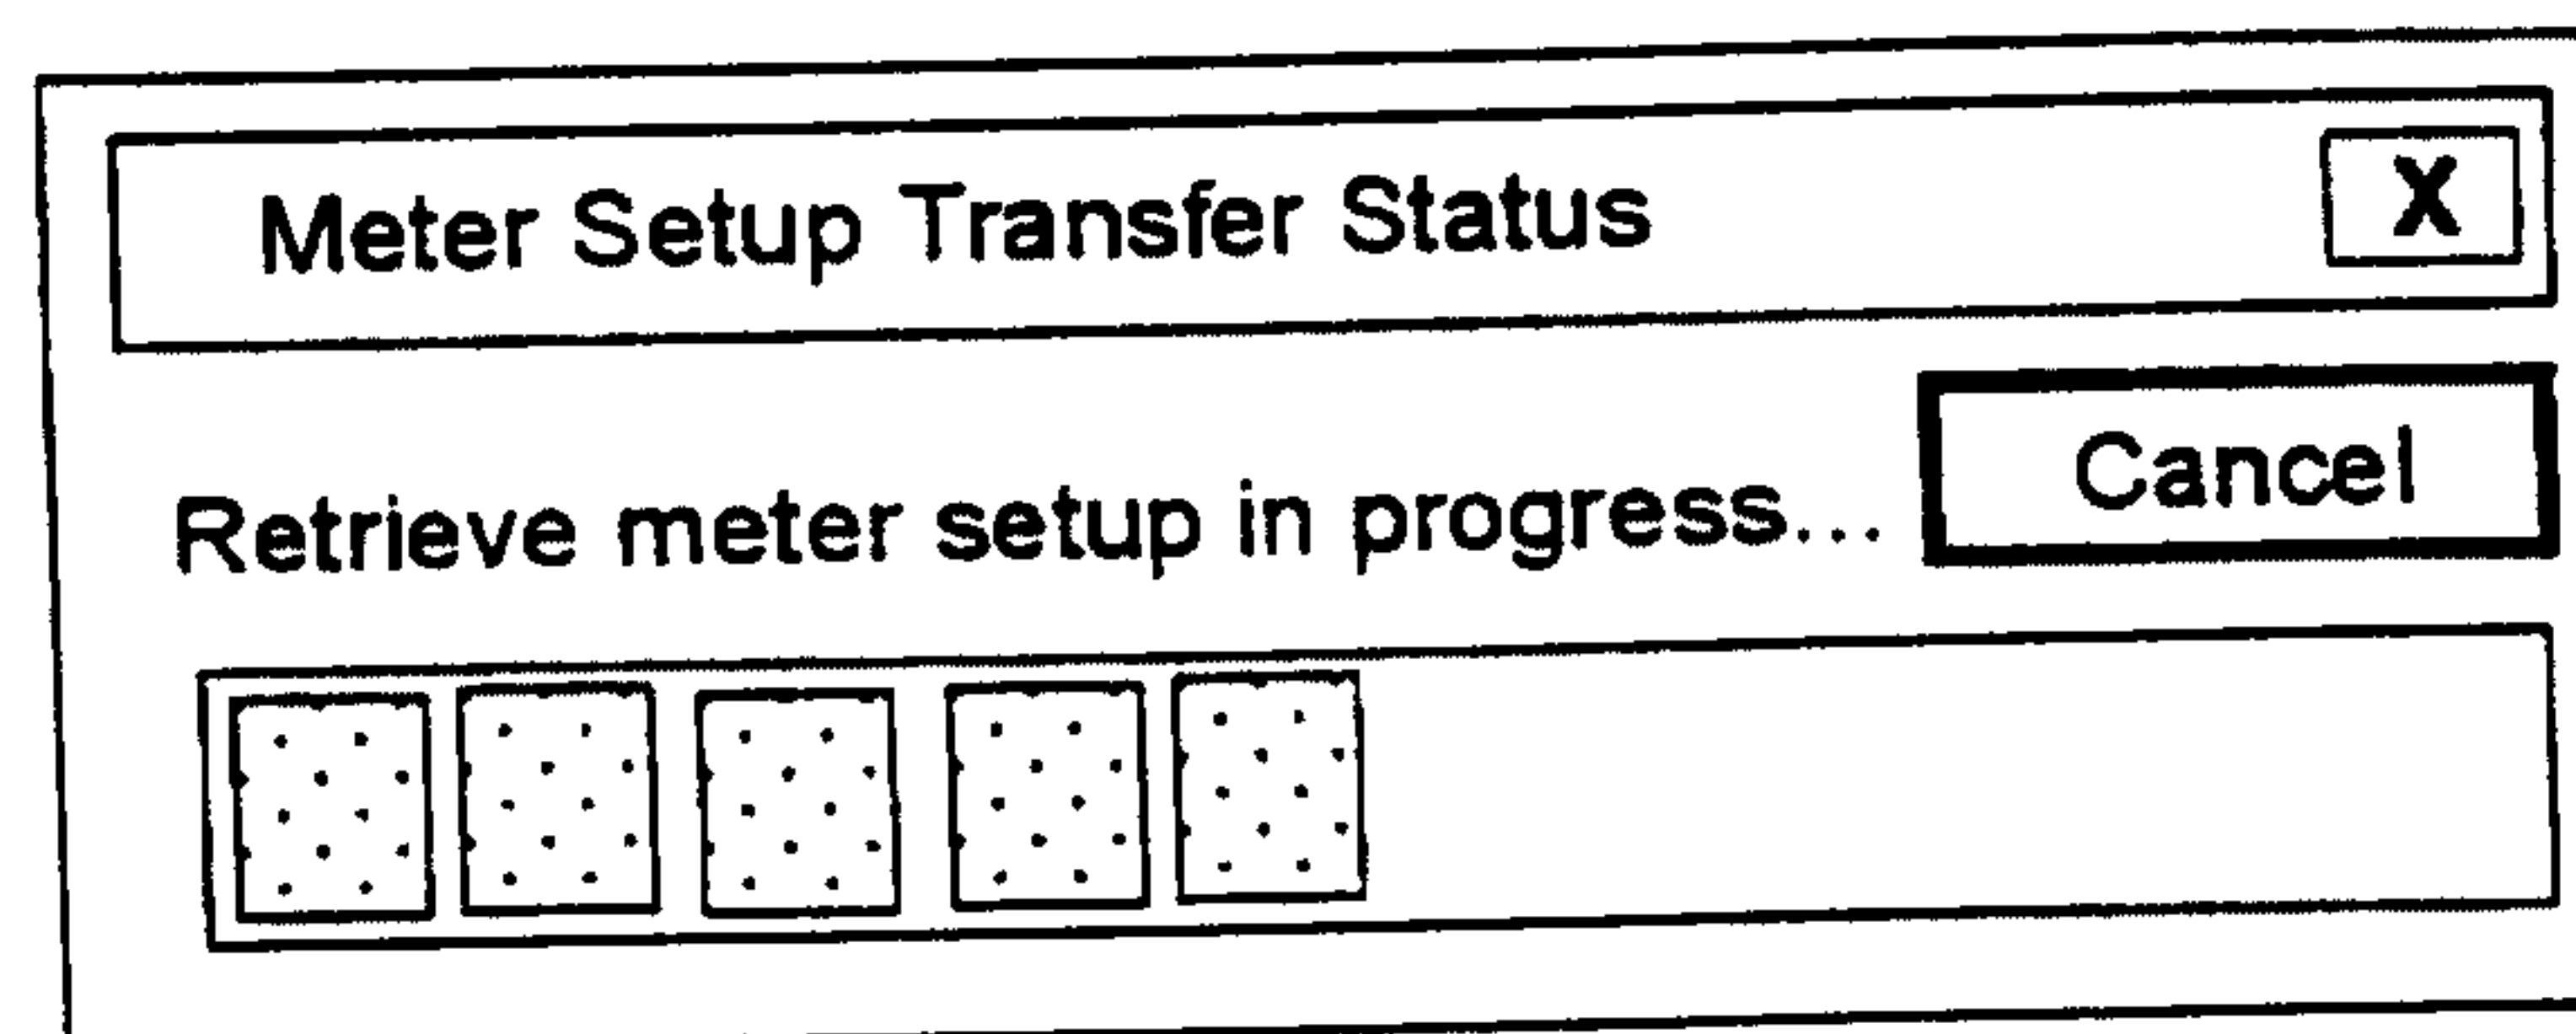*Fig. 46*

35/44

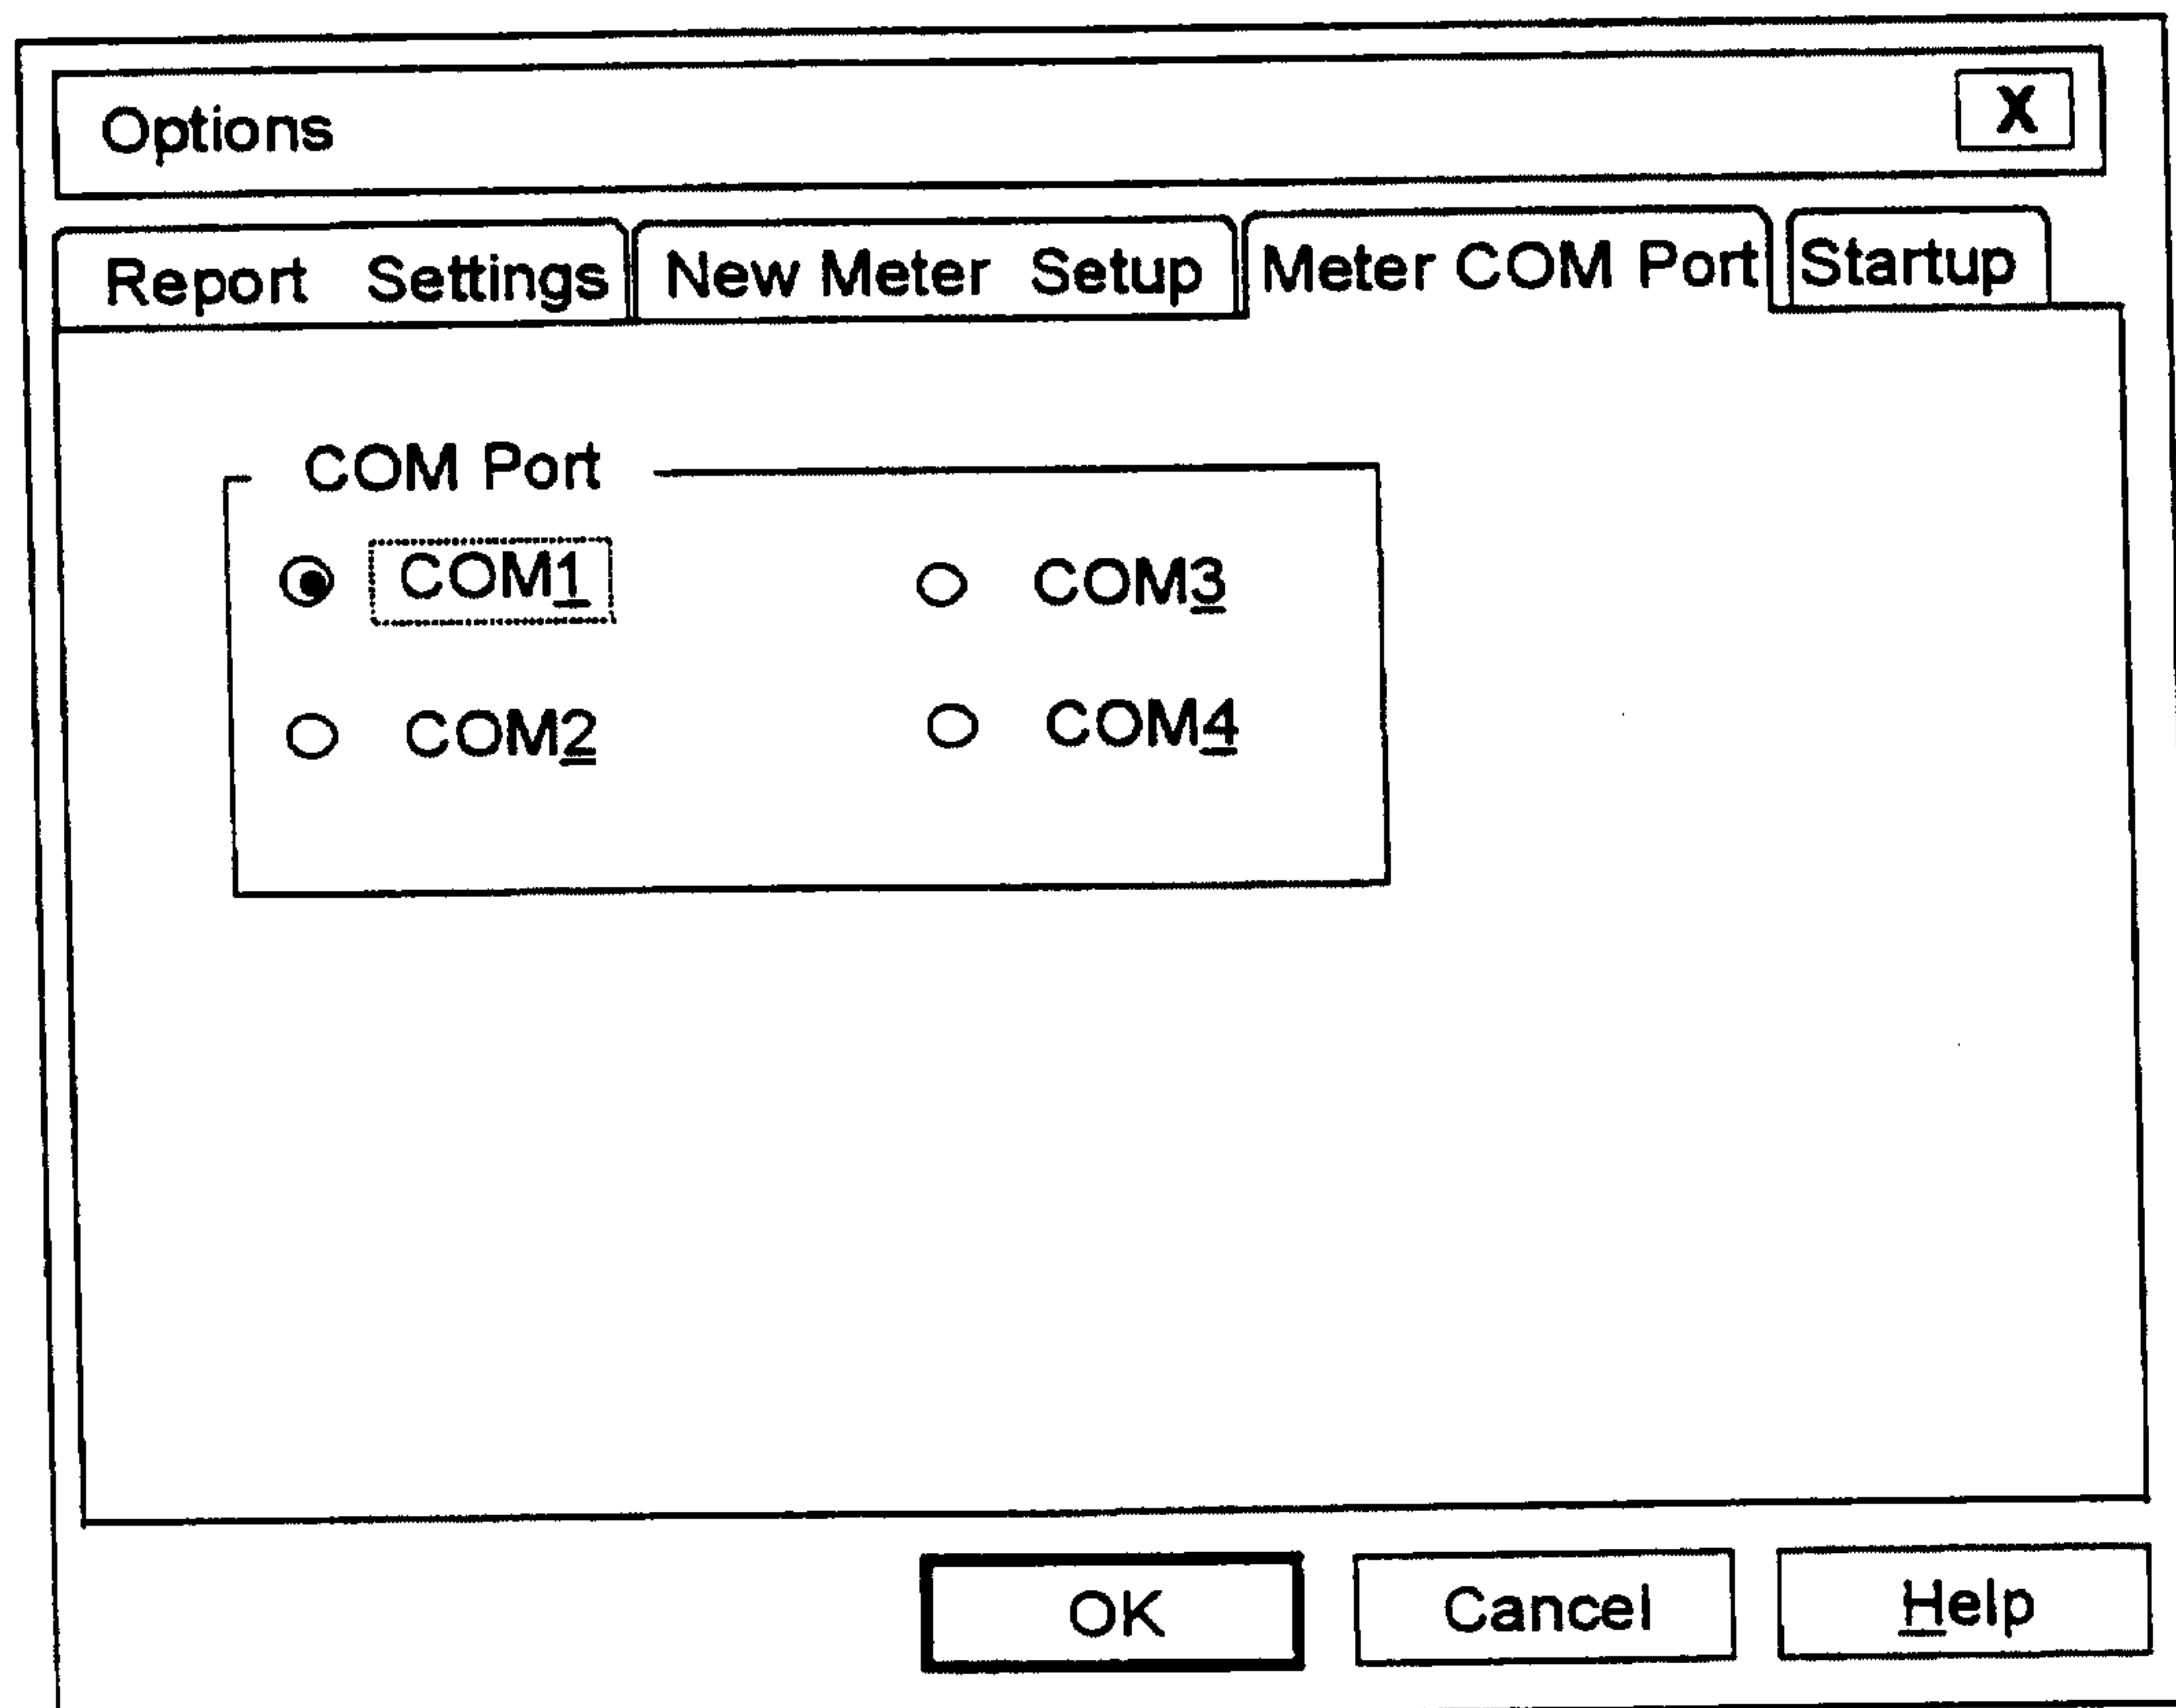*Fig. 47*

36/44

Options

Report Settings New Meter Setup Meter COM Port Startup

Report Formats

- ☒ Diary
- ☐ Glucose Values
- ☐ Trend
- ☐ Glucose Graph
- ☐ Average Trend
- ☐ Glucose Ranges
- ☐ Hypoglycemic Events

Range for Average Trend. Glucose Ranges and Hypo Events reports

48 hours ▼


Glucose Units

- ☒ mg/dL
- ☐ mmol/L


OK Cancel Help

Fig. 48


37/44

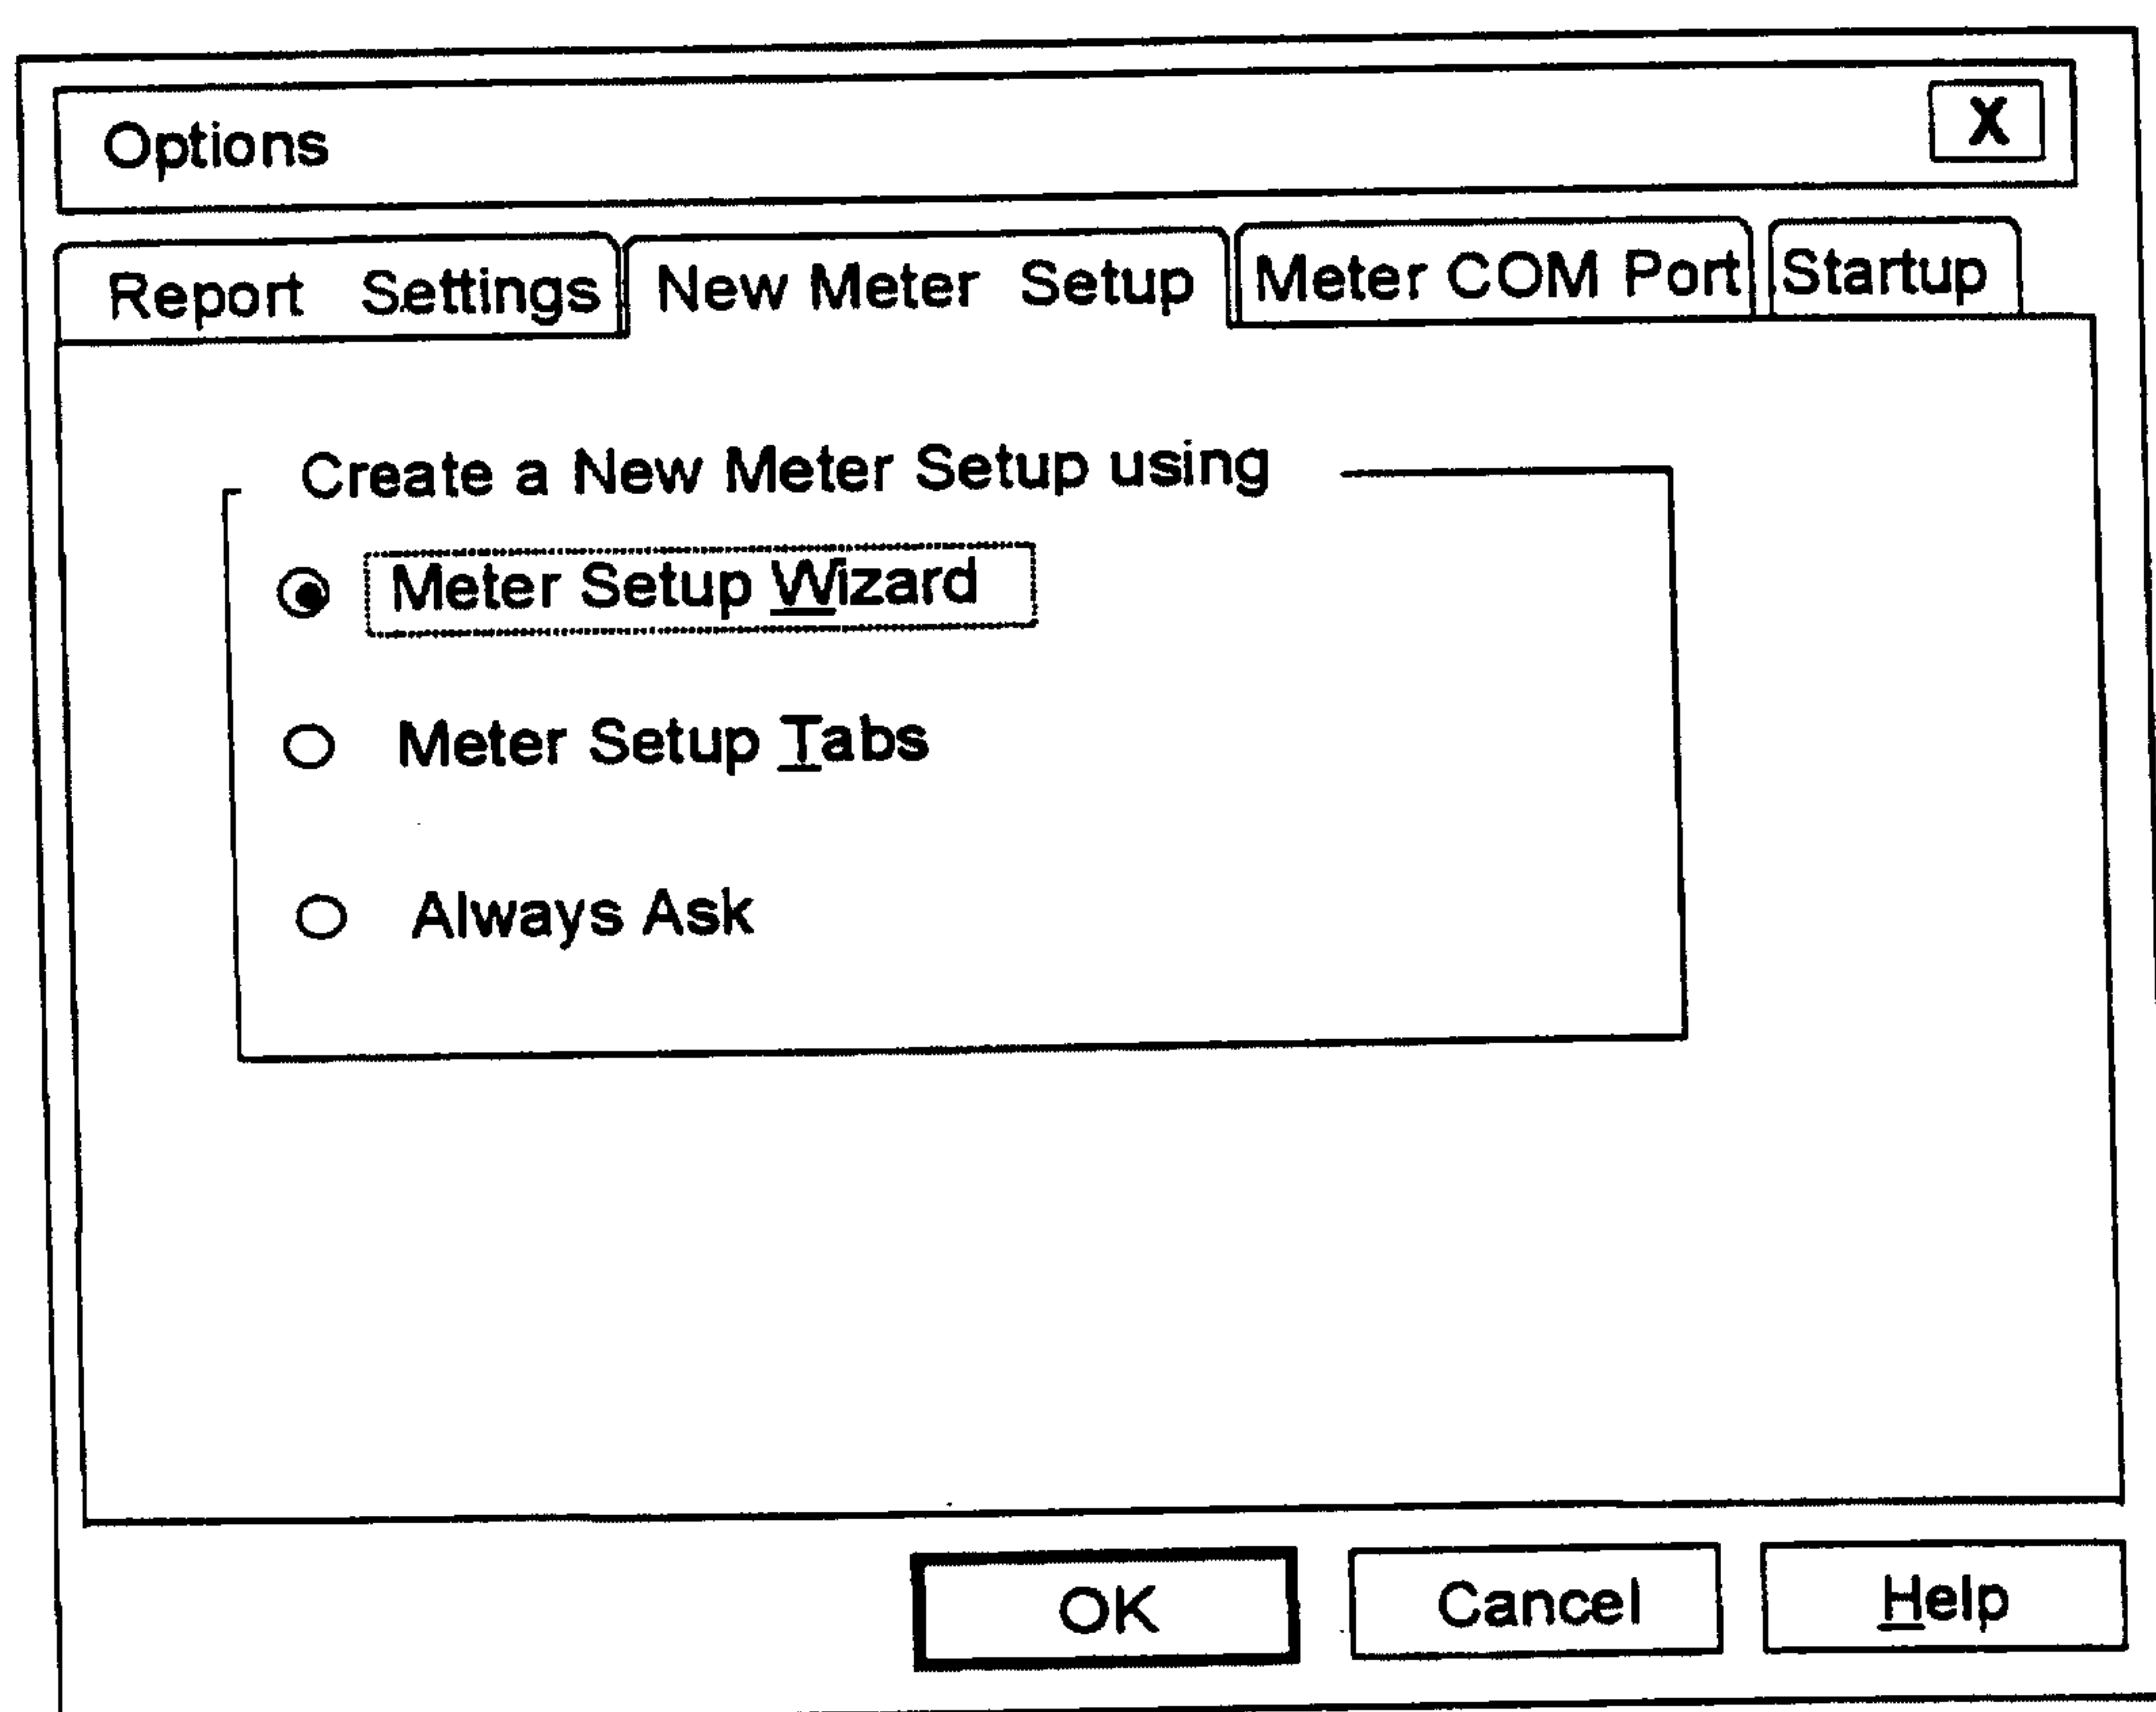*Fig. 49*

38/44

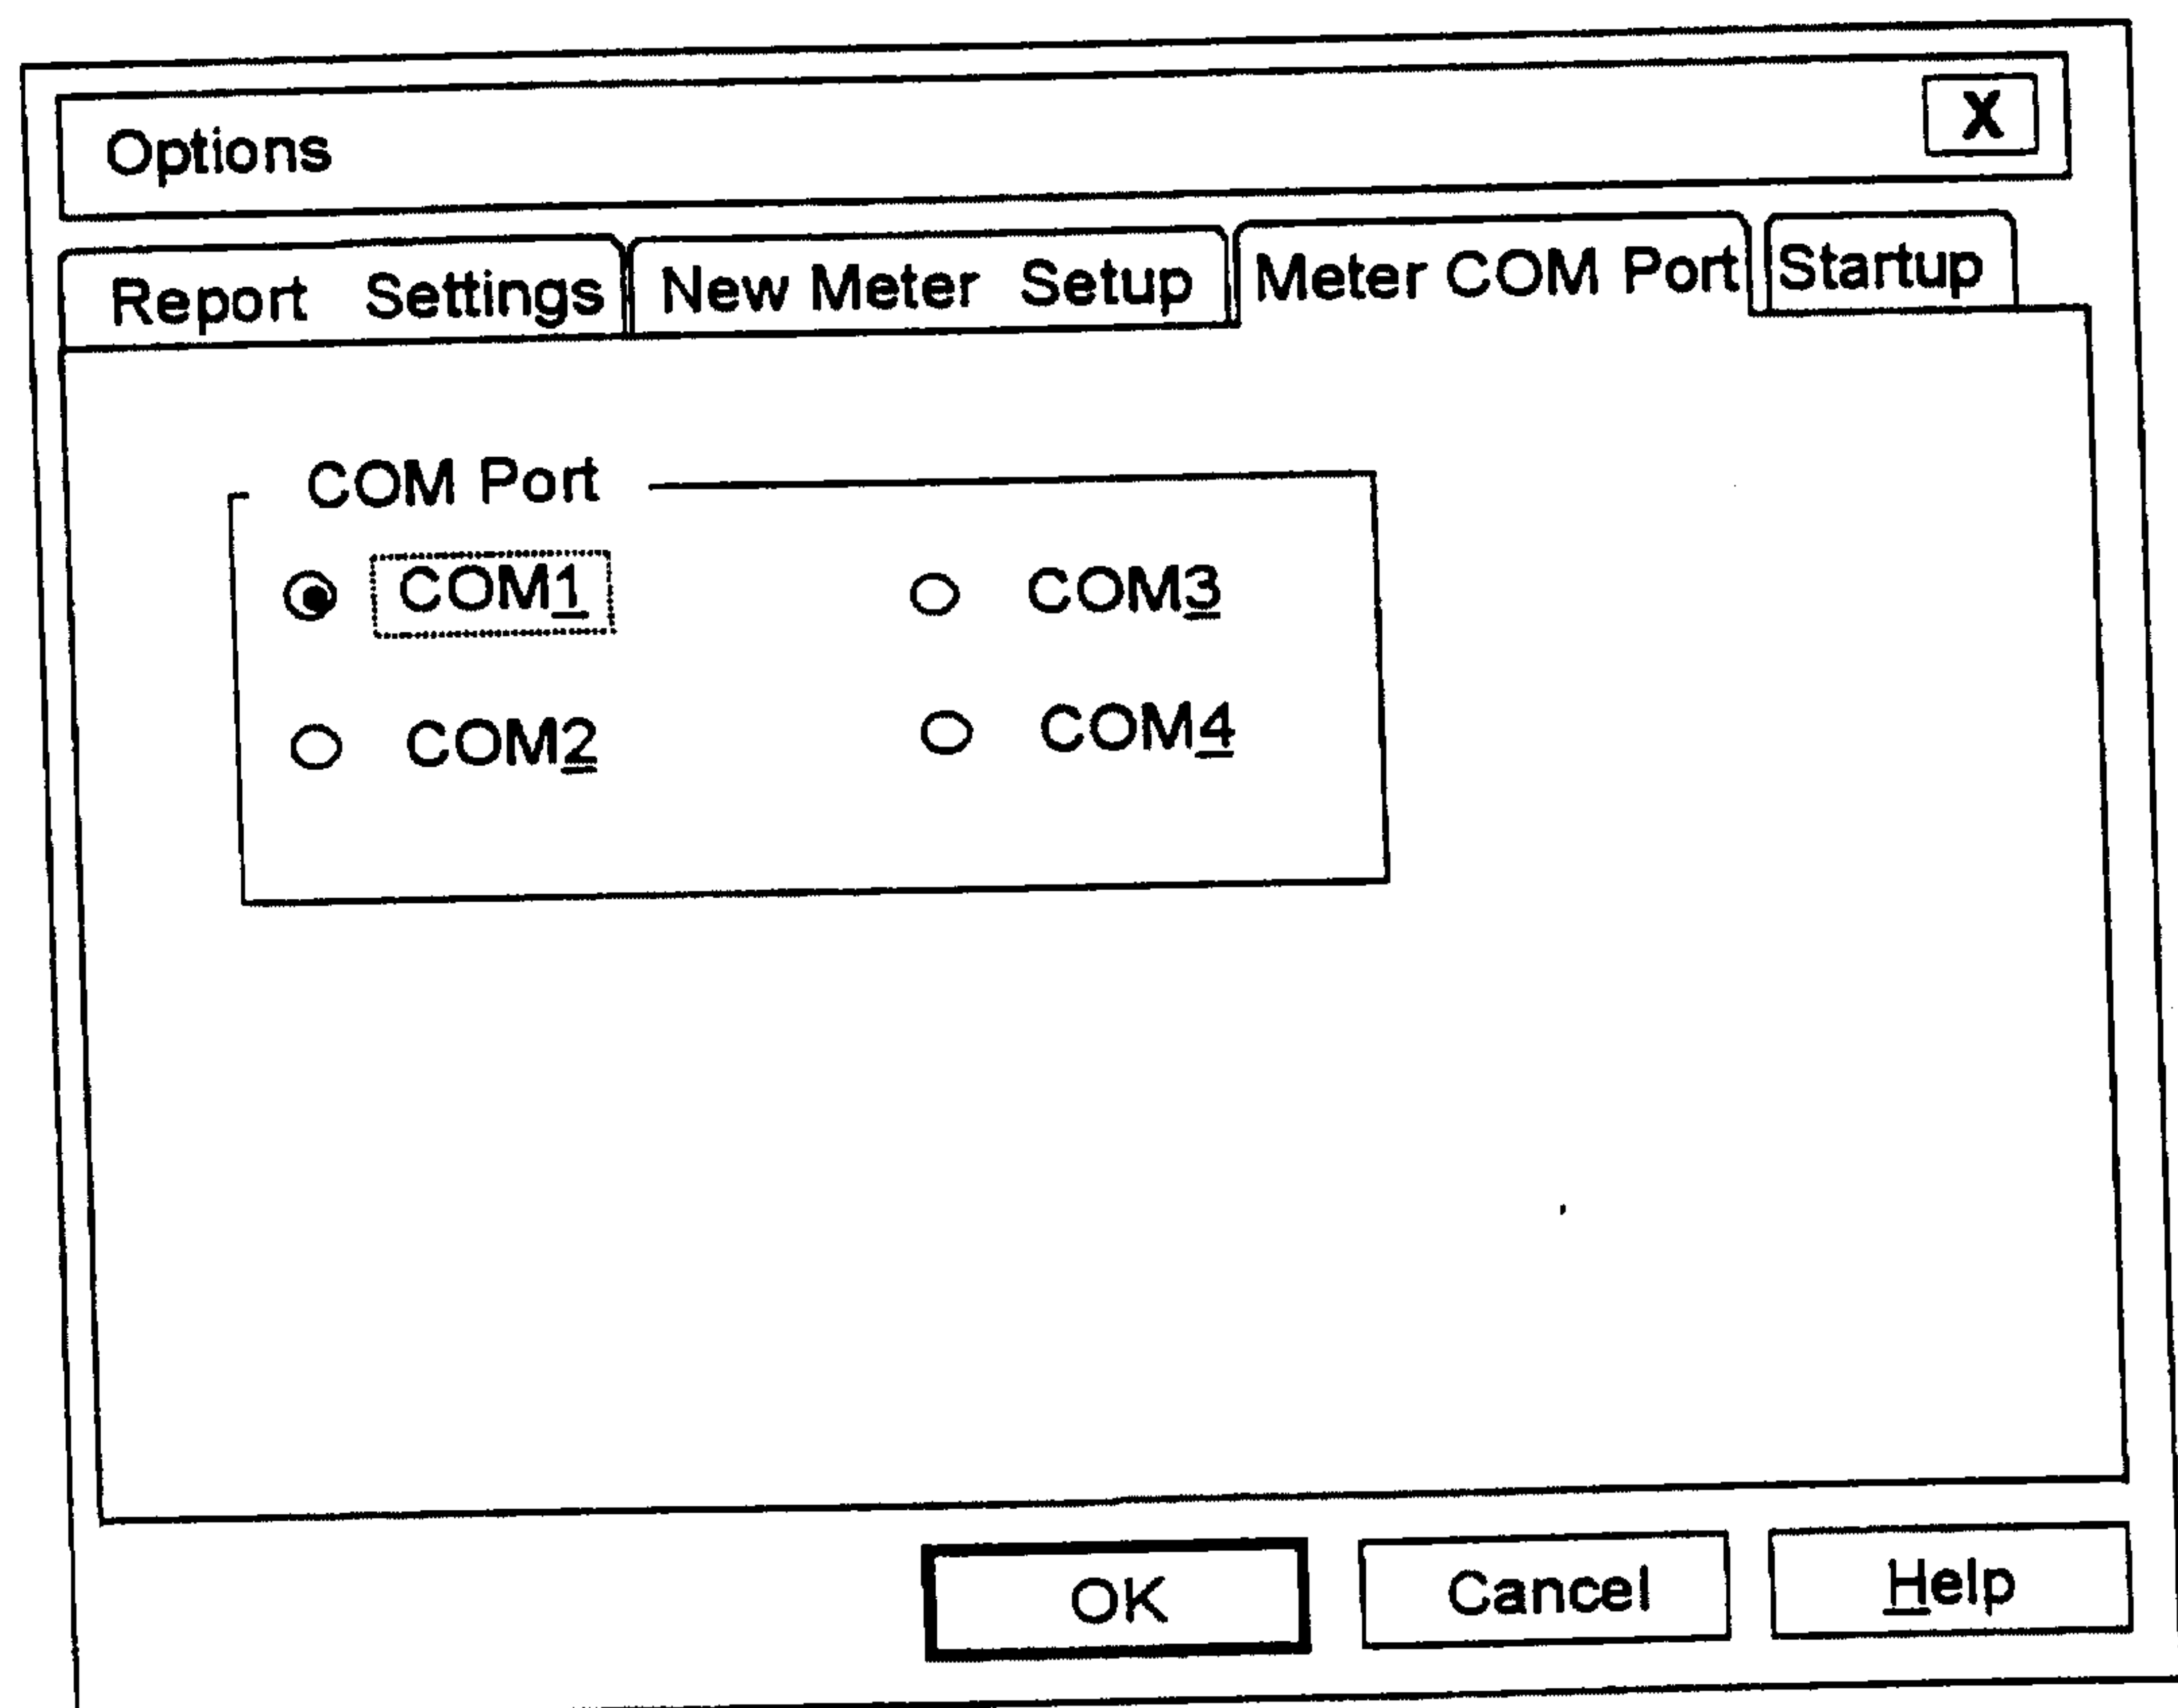*Fig. 50*

39/44

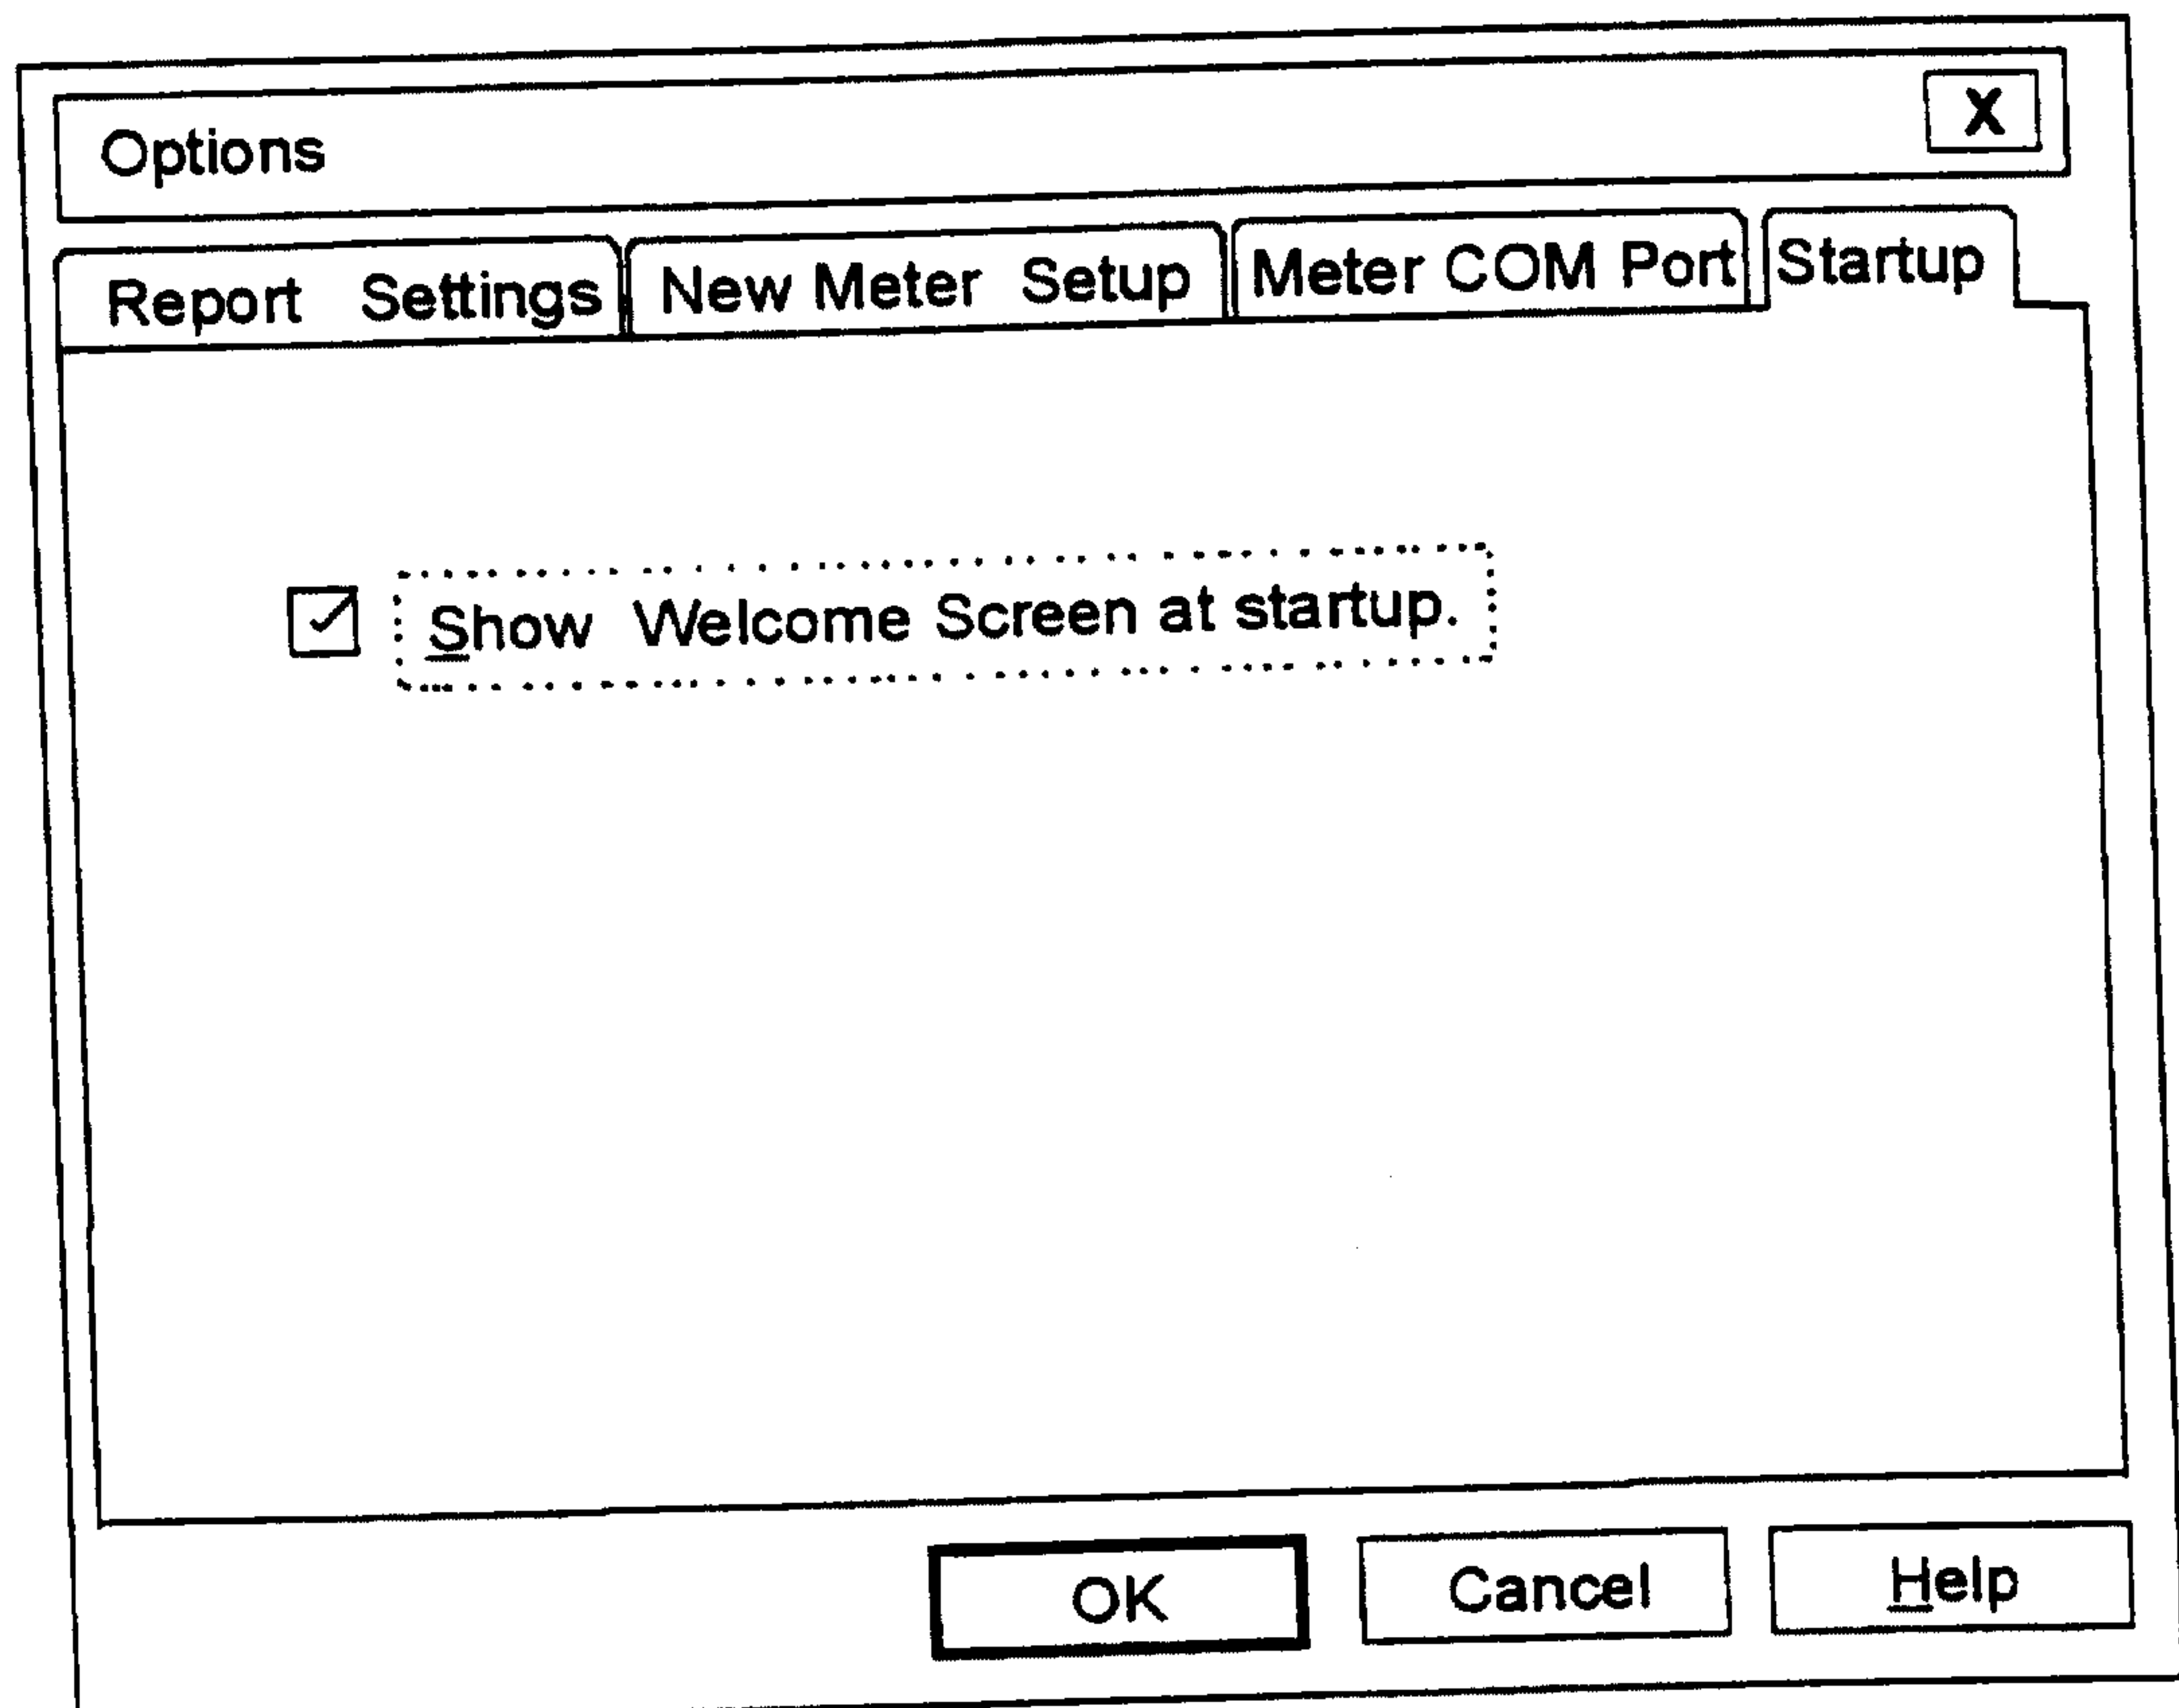*Fig. 51*

40/44

Phone In Manager

File View Help

Recent Phone-ins

111111112	Tim Dishop	12/6/96	4:19 PM
111111111	Steve Moak	12/6/96	11:06 AM
111111111	Steve Moak	12/6/96	10:56 AM
111111111	Steve Moak	12/6/96	10:55 AM
1234567890	John Smith	12/5/96	10:45 AM

Print

View

☒ Auto Print

Phone Line Status

Line 1 Line 2 Line 3 Line 4

Details...

For Help, press F1

NUM

Fig. 52

- [] [X]

-Patient Data Report

Transfer Date/Time: 11/10/98 7:28 AM
Meter Serial Number: 0005040225
Patient Name: John Smith
Patient ID: default

Diary Report

Date	Time	Glucose (mg/dL)	Insulin Type	Insulin Dosage	Events	Other
1/16/98	7:30 AM	236	70/30	22.0	Before Meal	bG=high, Carbs=60g
1/16/98	12:28 PM	85			Before Meal	Carbs=60g
1/16/98	2:45 PM	179			After Meal	Carbs=30g
1/16/98	5:20 PM	314	Reg 70/30	2.0 8.0	Before Meal	bG=high, Carbs=60g
1/16/98	8:00 PM	250				bG=high
1/17/98	12:15 AM	275				bG=high
1/17/98	7:58 AM	151	70/30	22.0	Before Meal	Carbs=45g
1/17/98	10:00 AM	180			After Meal	Carbs=15g

◀ [] ▶

Fig. 53

42/44



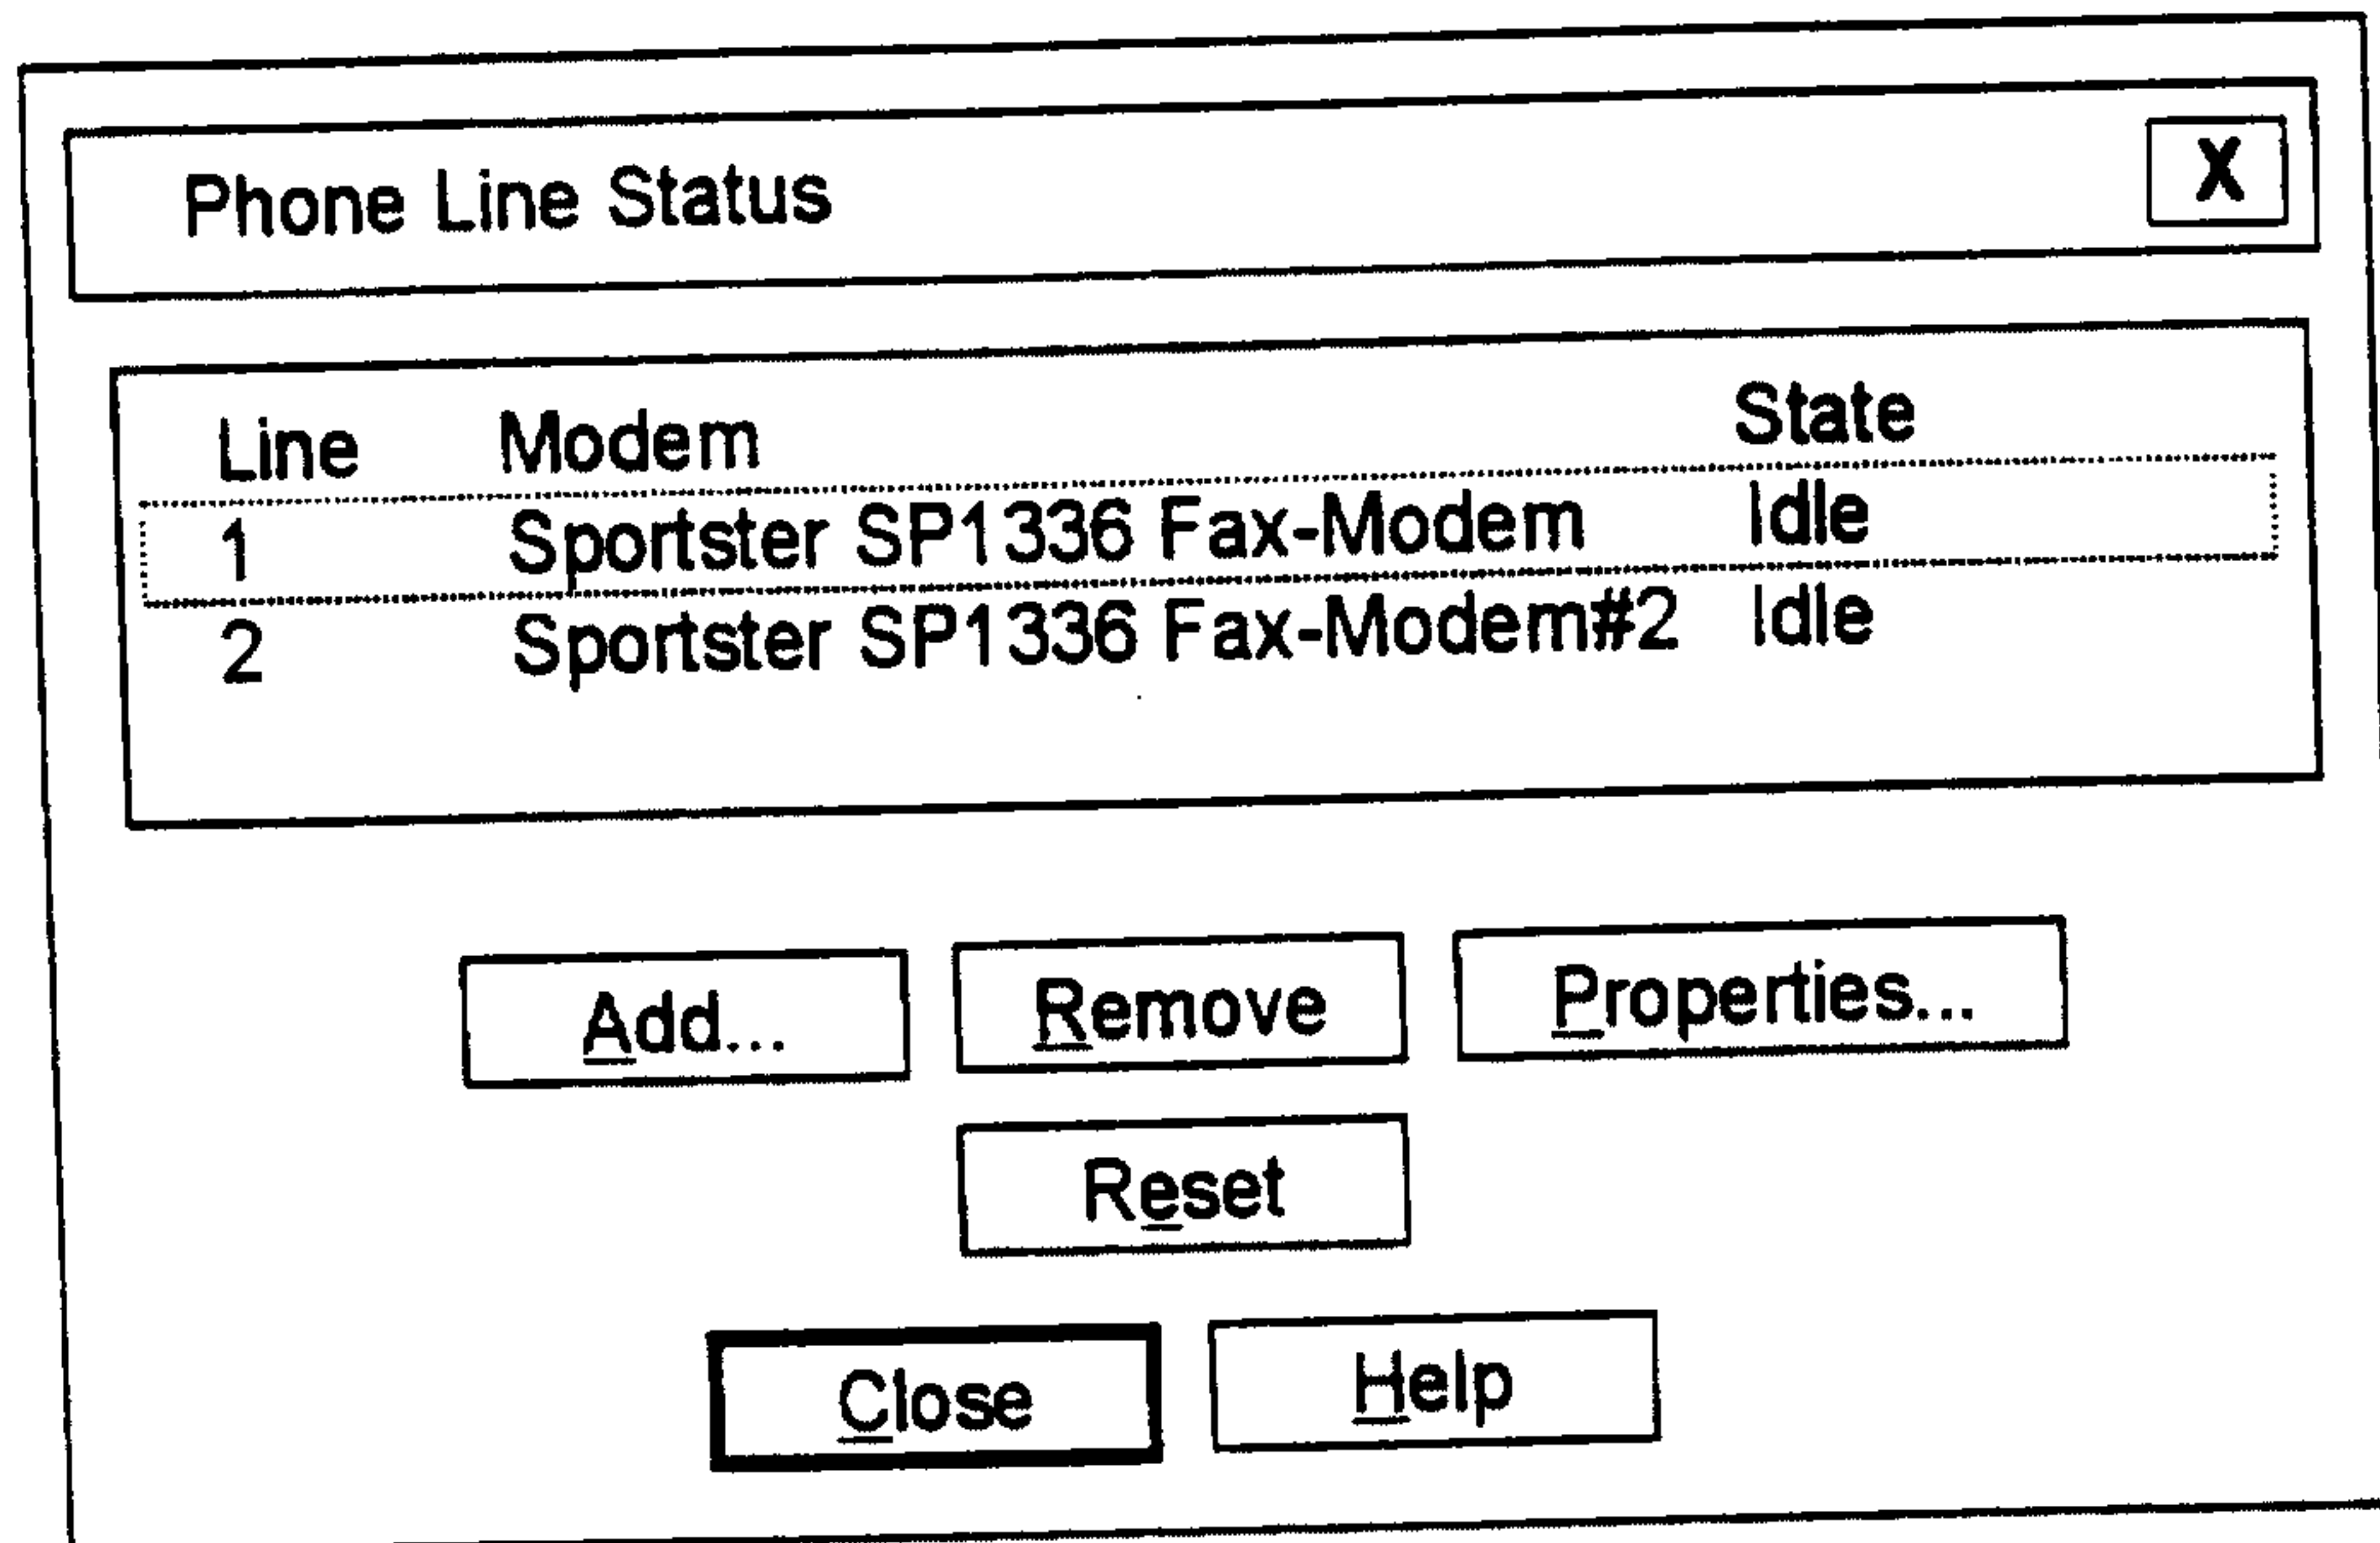
*Fig. 54**Fig. 55*

Fig. 56

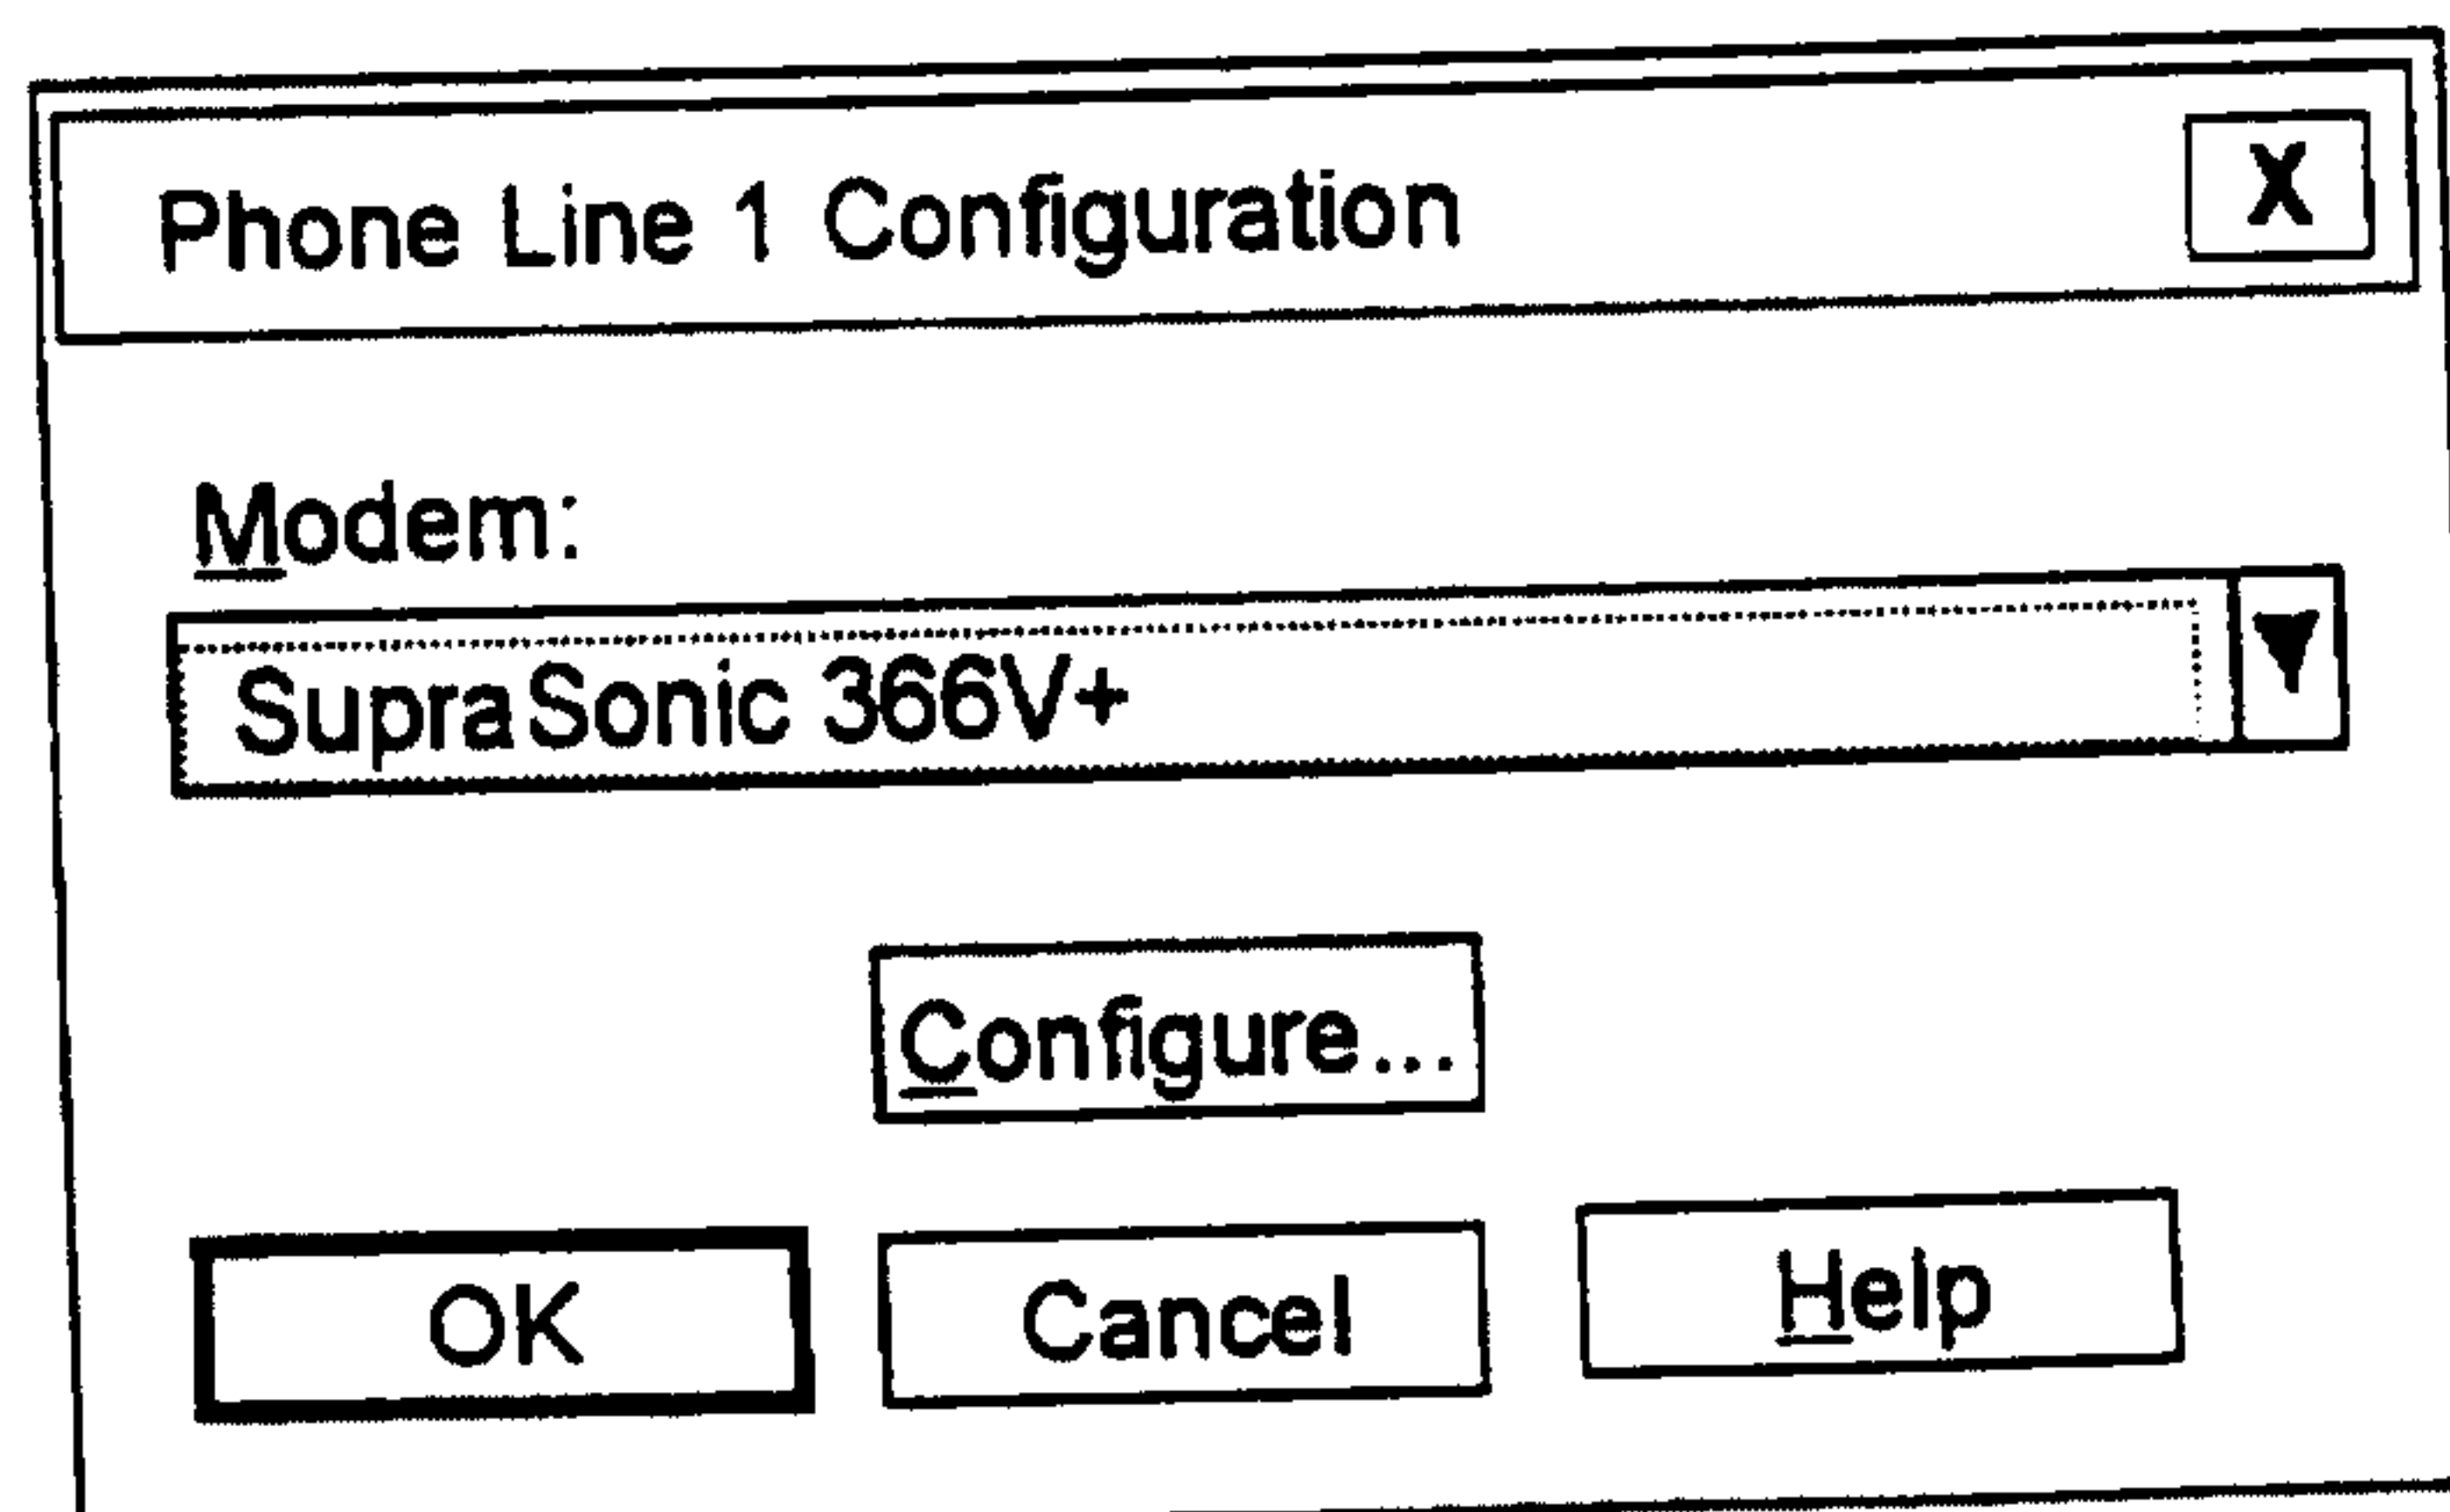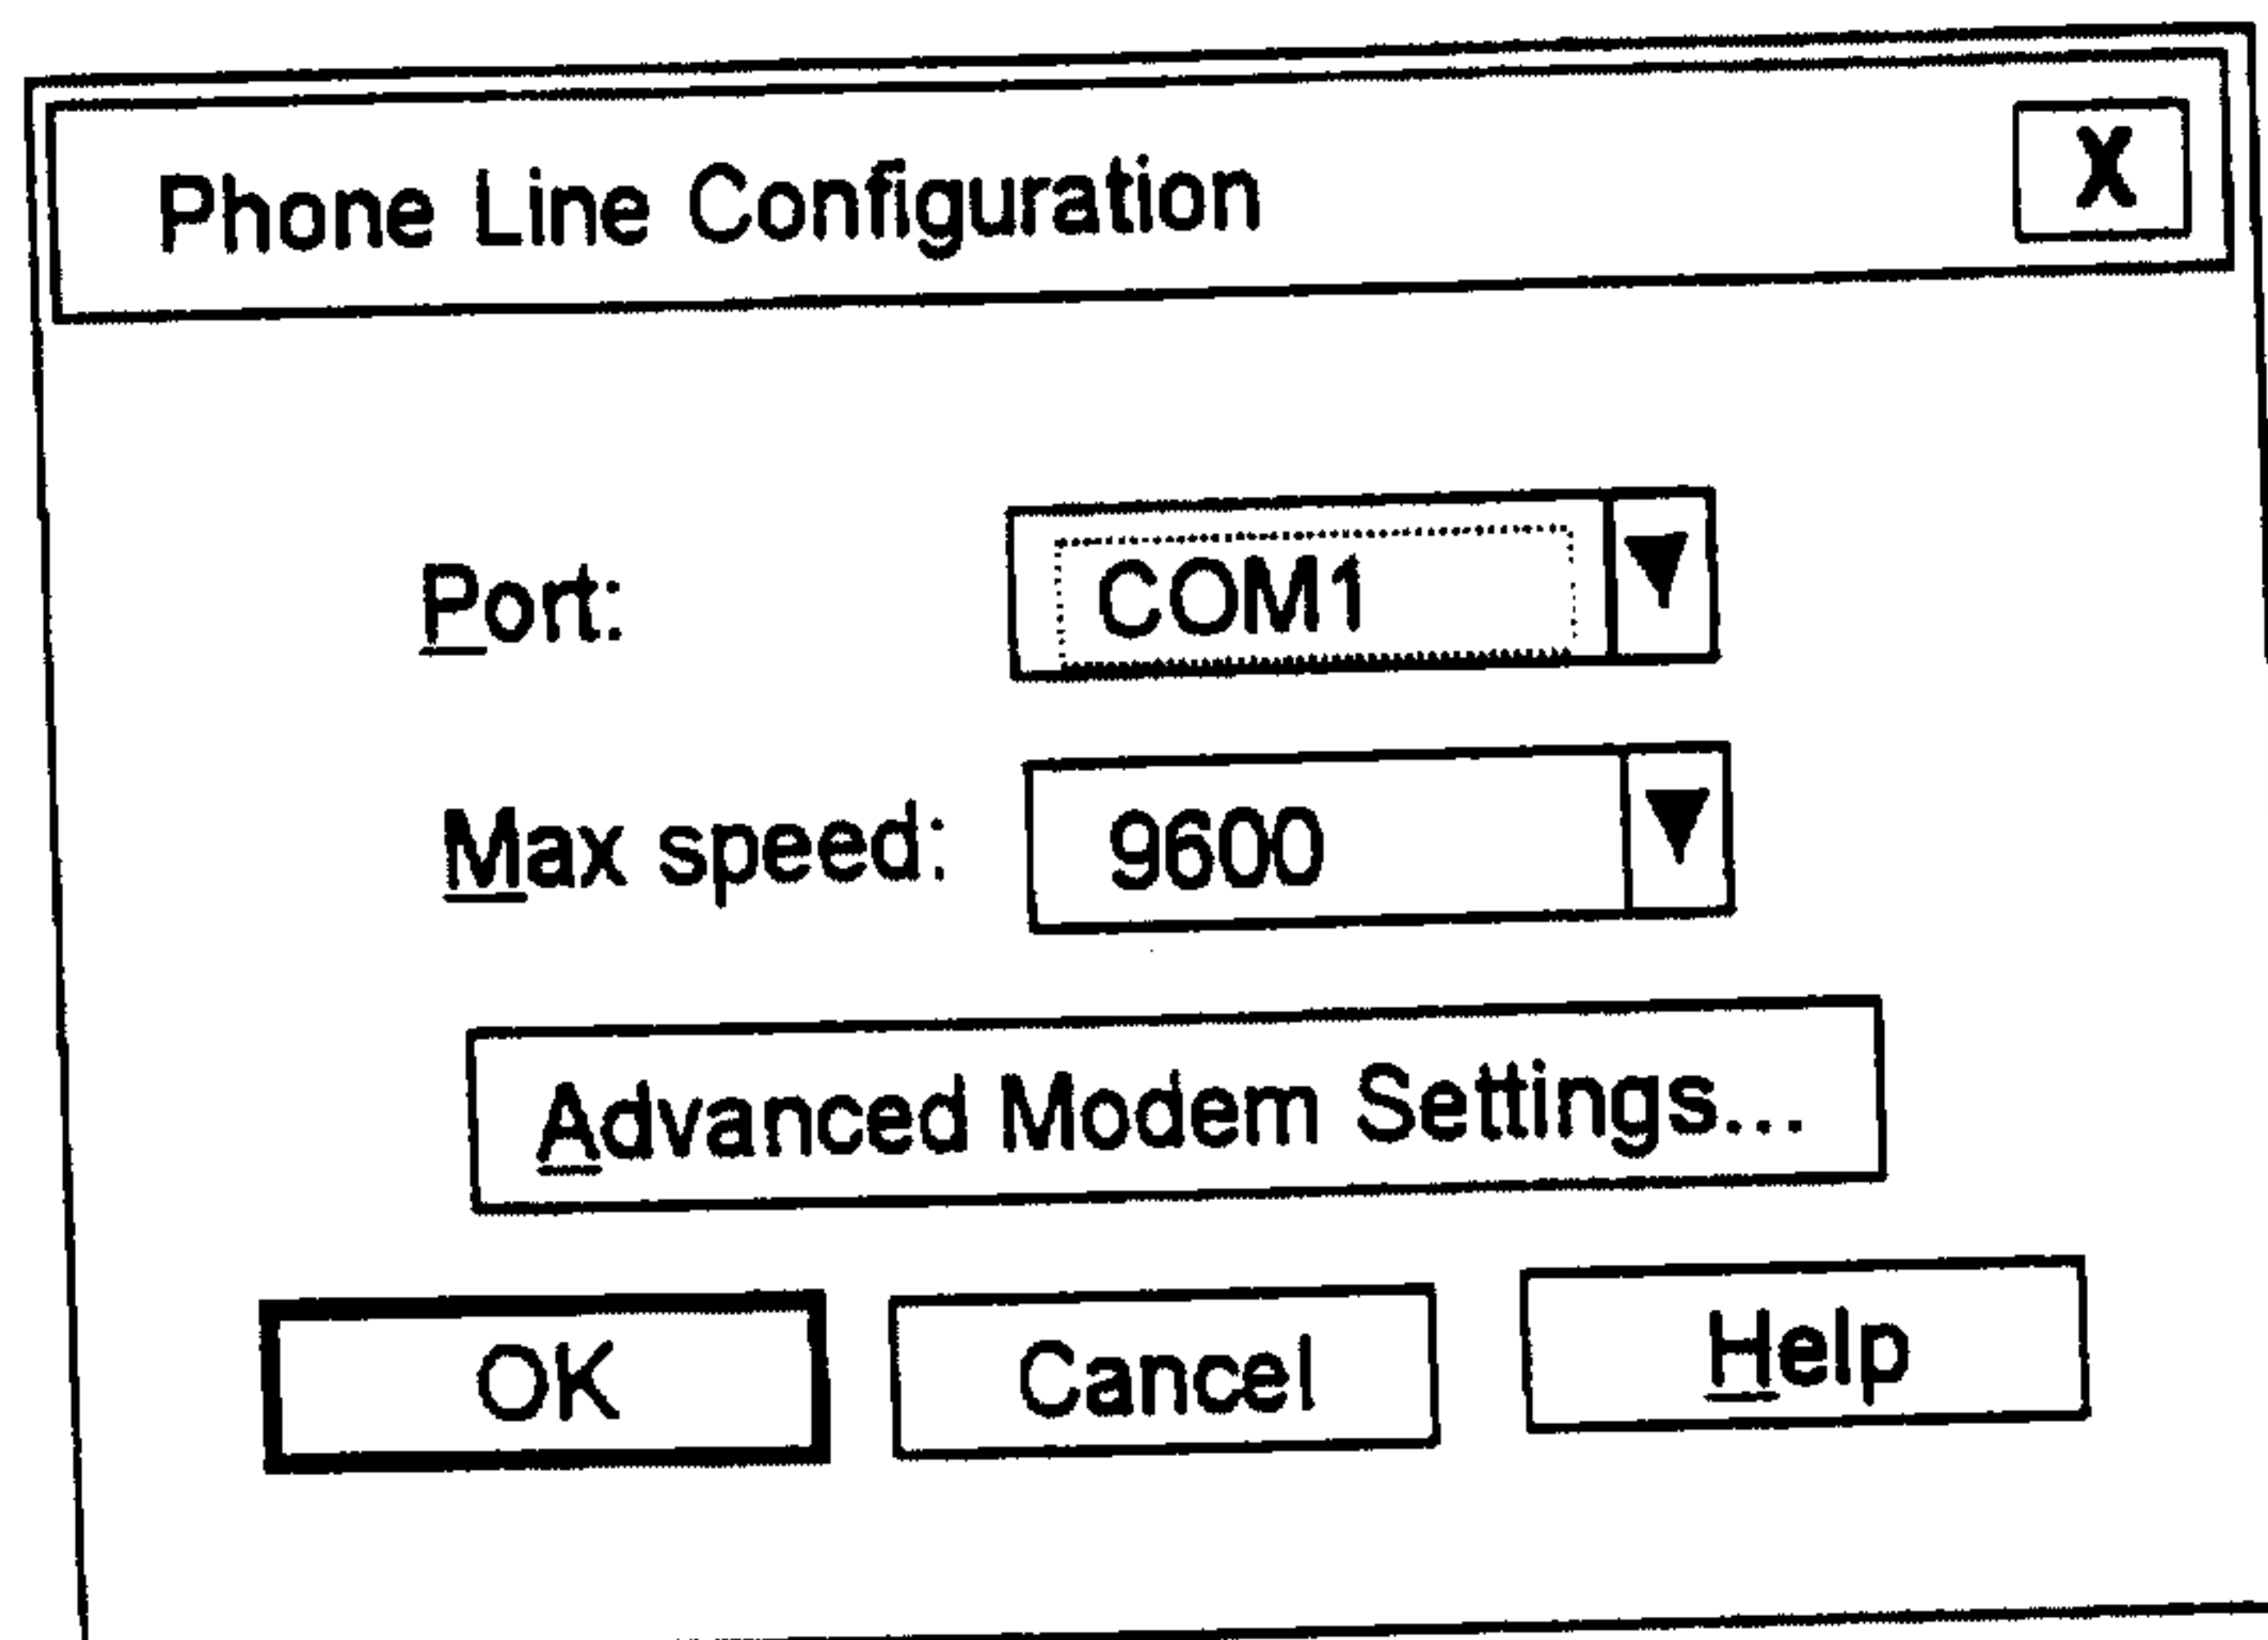

Phone Line Configuration


Port: COM1 ▼

Max speed: 9600 ▼

Advanced Modem Settings...

OK Cancel Help

Fig. 57

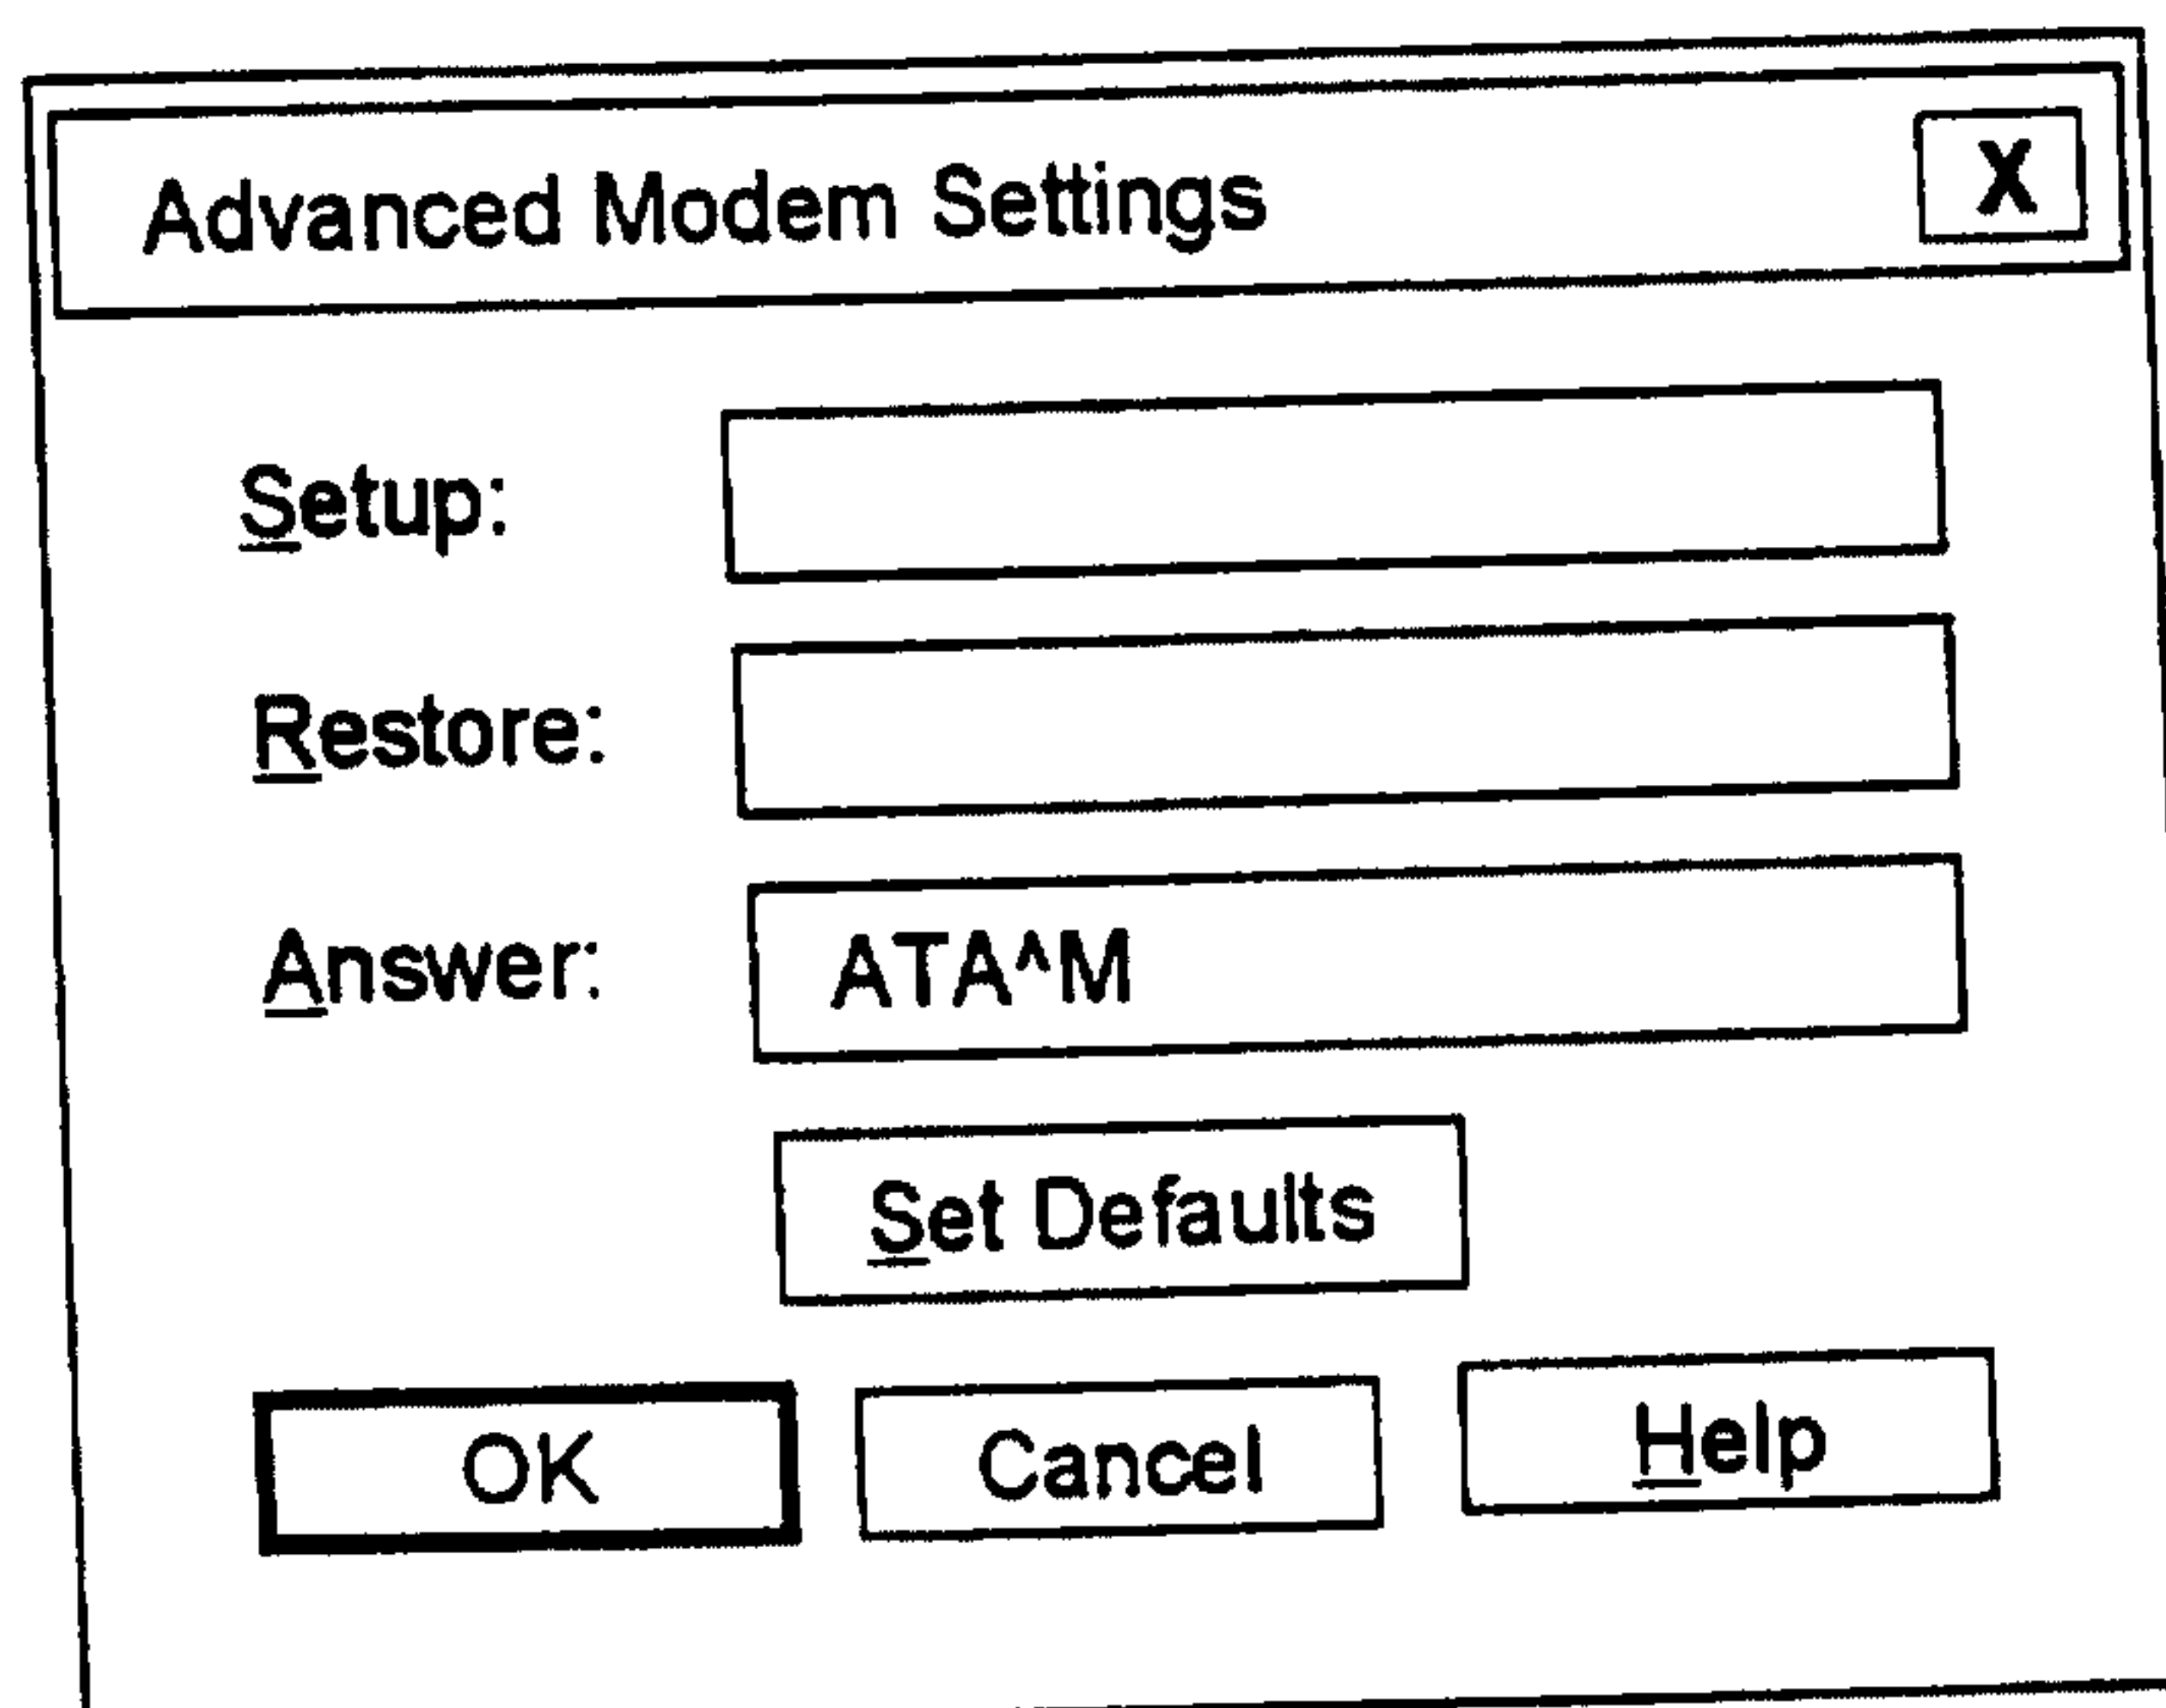

Advanced Modem Settings

Setup:


Restore:

Answer: ATA^M

Set Defaults

OK Cancel Help

Fig. 58

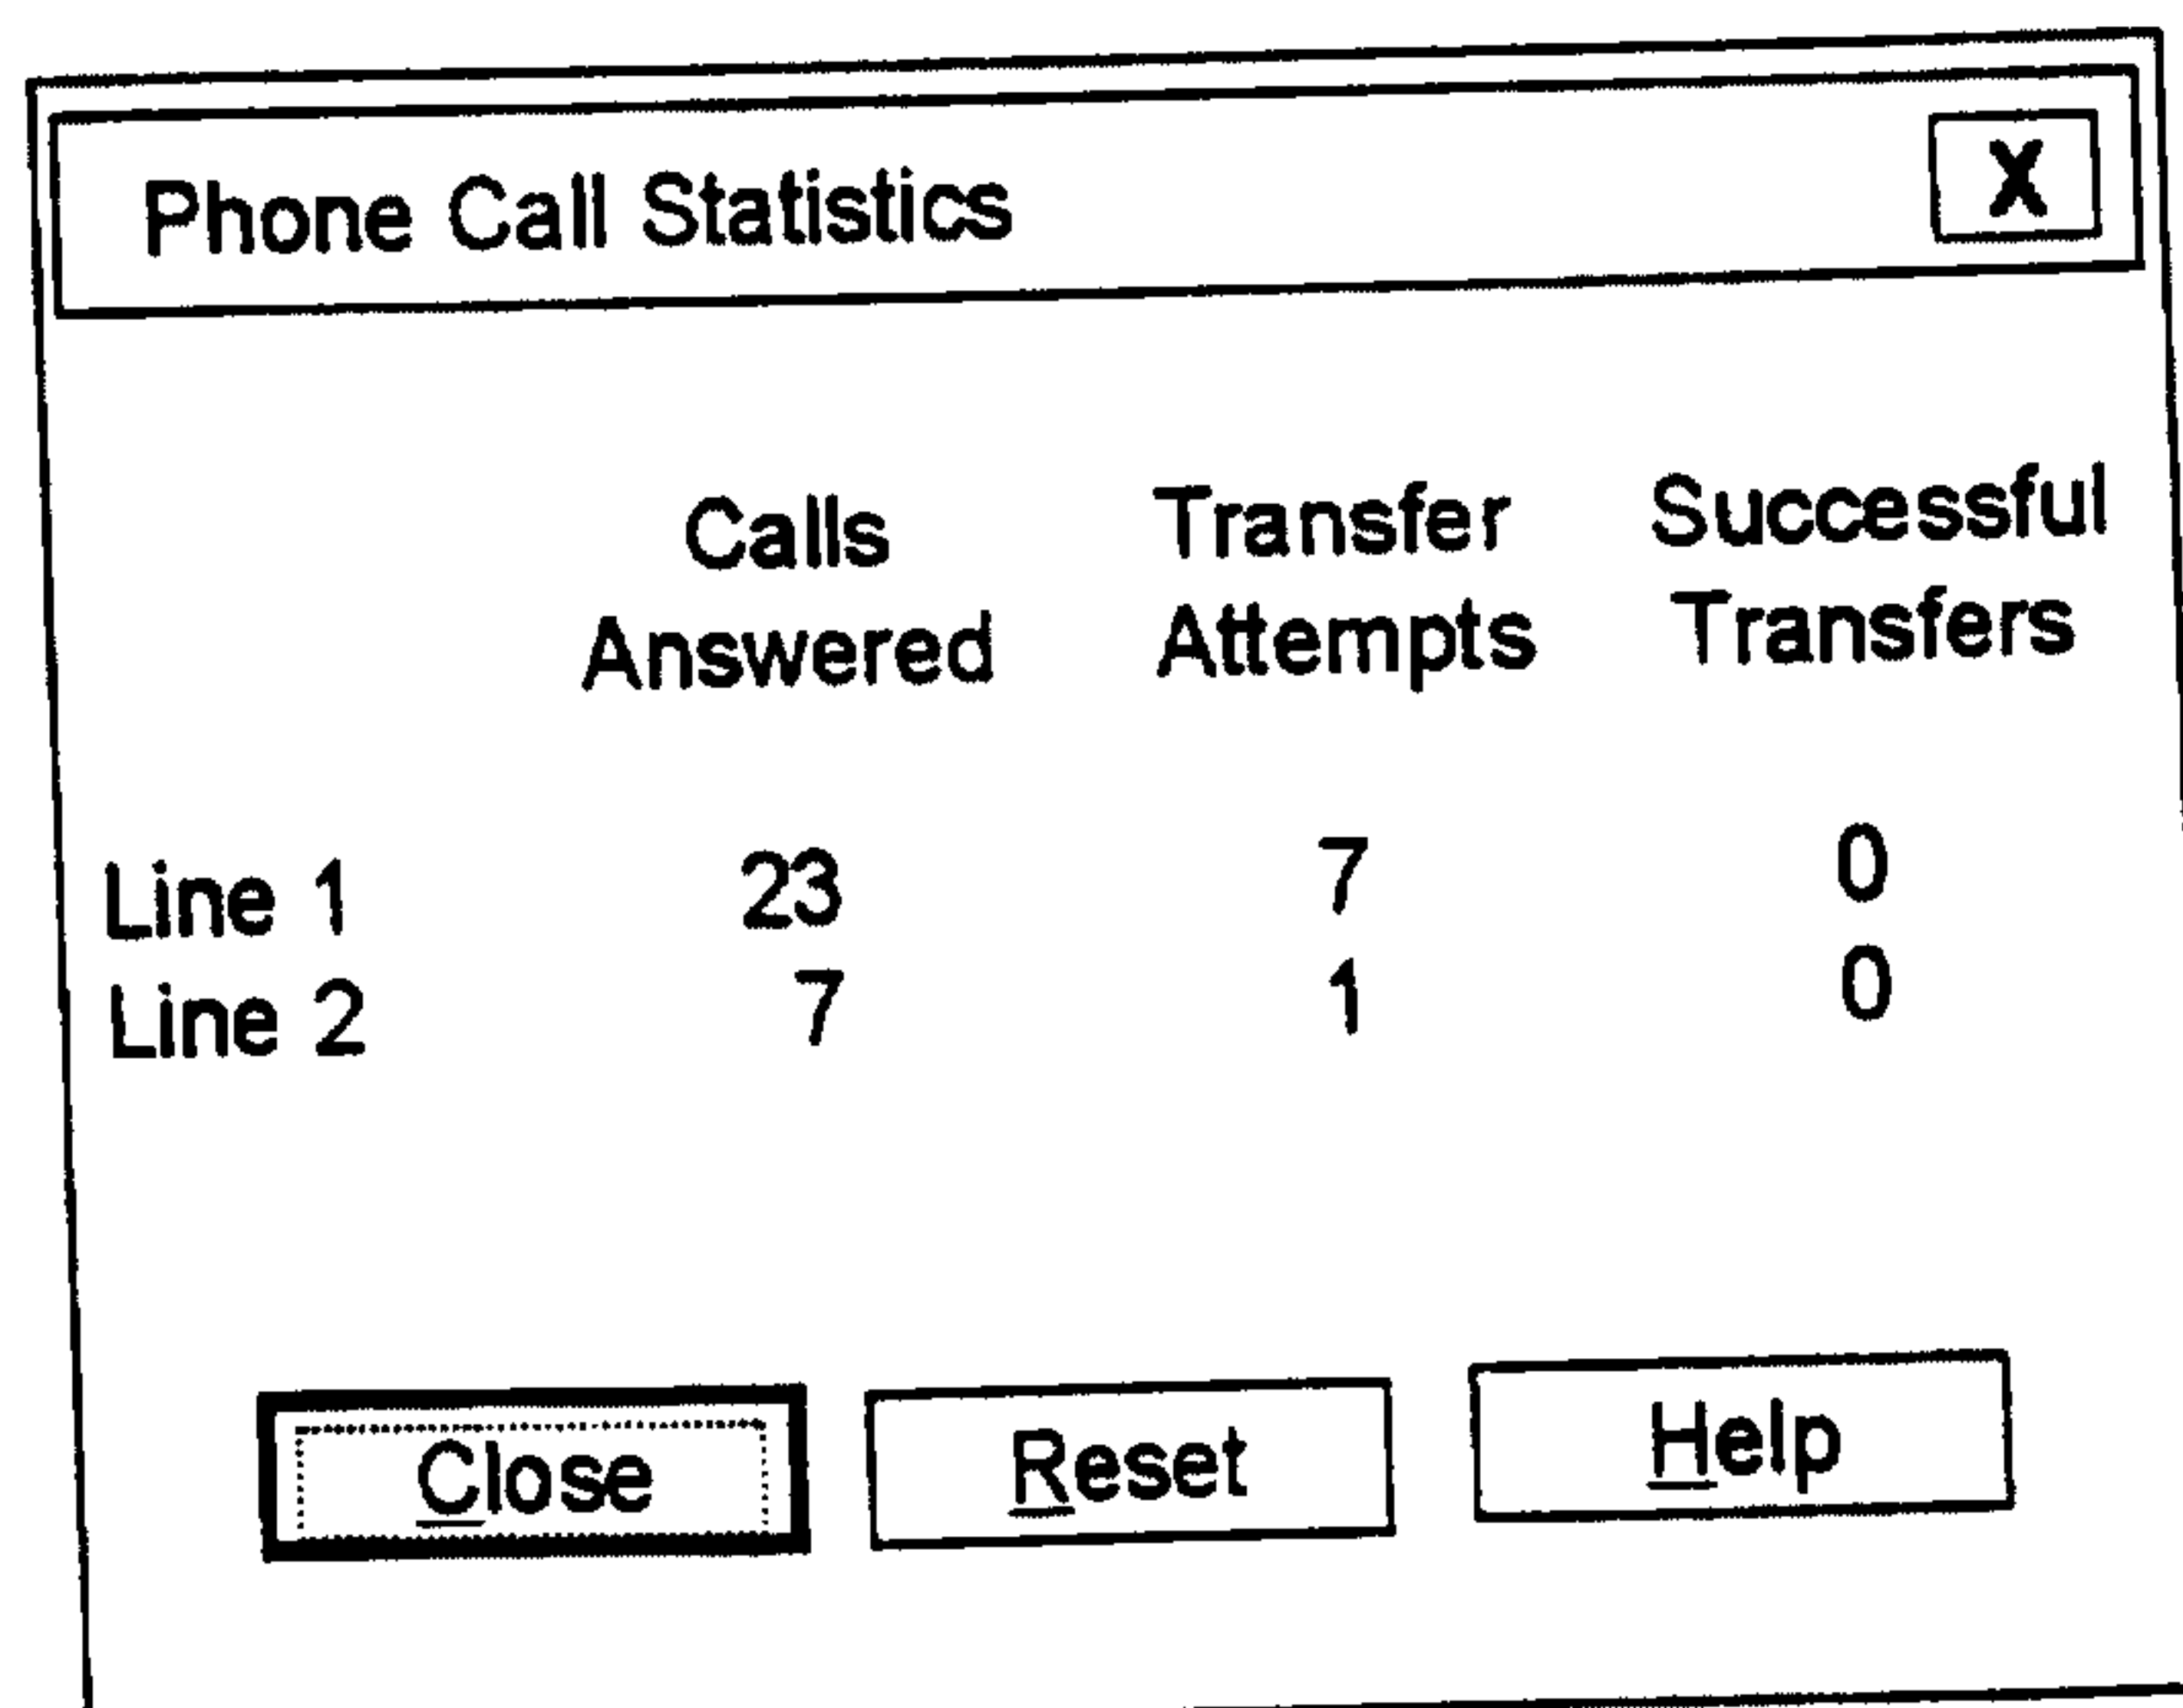


Phone Call Statistics

	Calls Answered	Transfer Attempts	Successful Transfers
Line 1	23	7	0
Line 2	7	1	0

Close Reset Help

44/44

Fig. 59

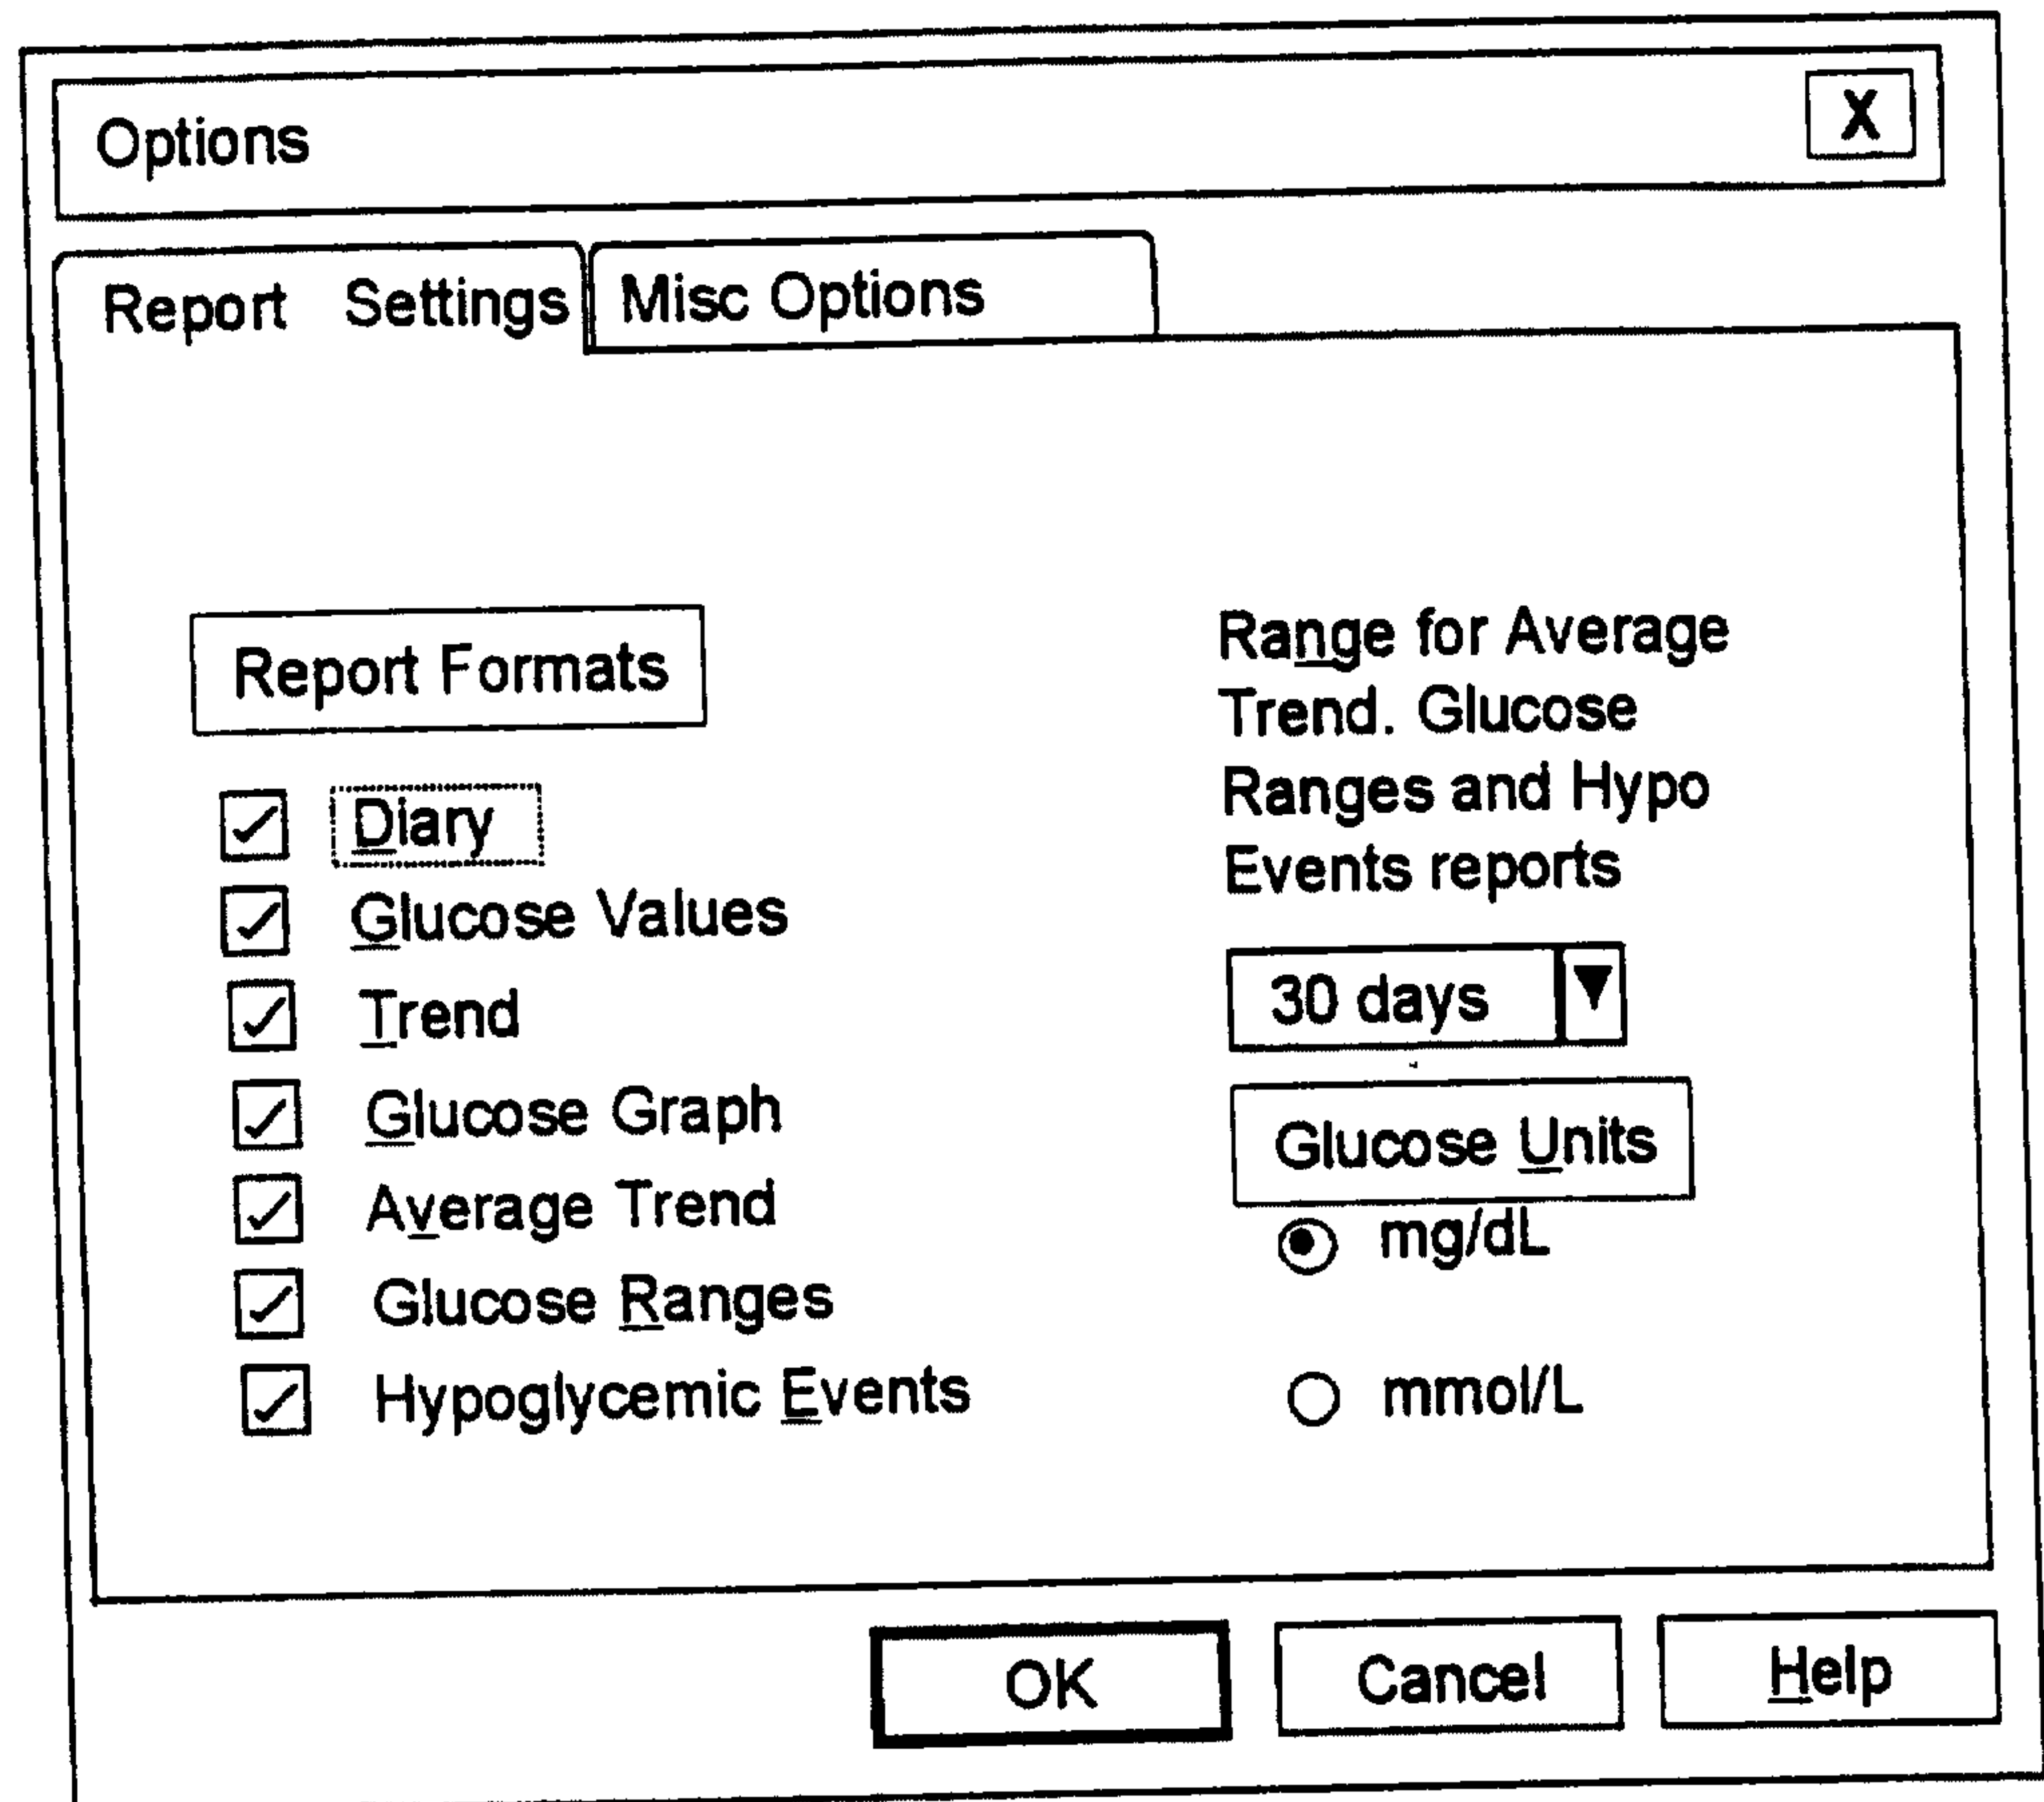

Options [X]

Report Settings Misc Options

Report Formats

- ☒ Diary
- ☒ Glucose Values
- ☒ Trend
- ☒ Glucose Graph
- ☒ Average Trend
- ☒ Glucose Ranges
- ☒ Hypoglycemic Events

Range for Average Trend. Glucose Ranges and Hypo Events reports

30 days ▼


Glucose Units

☒ mg/dL

☐ mmol/L

OK Cancel Help

Fig. 60

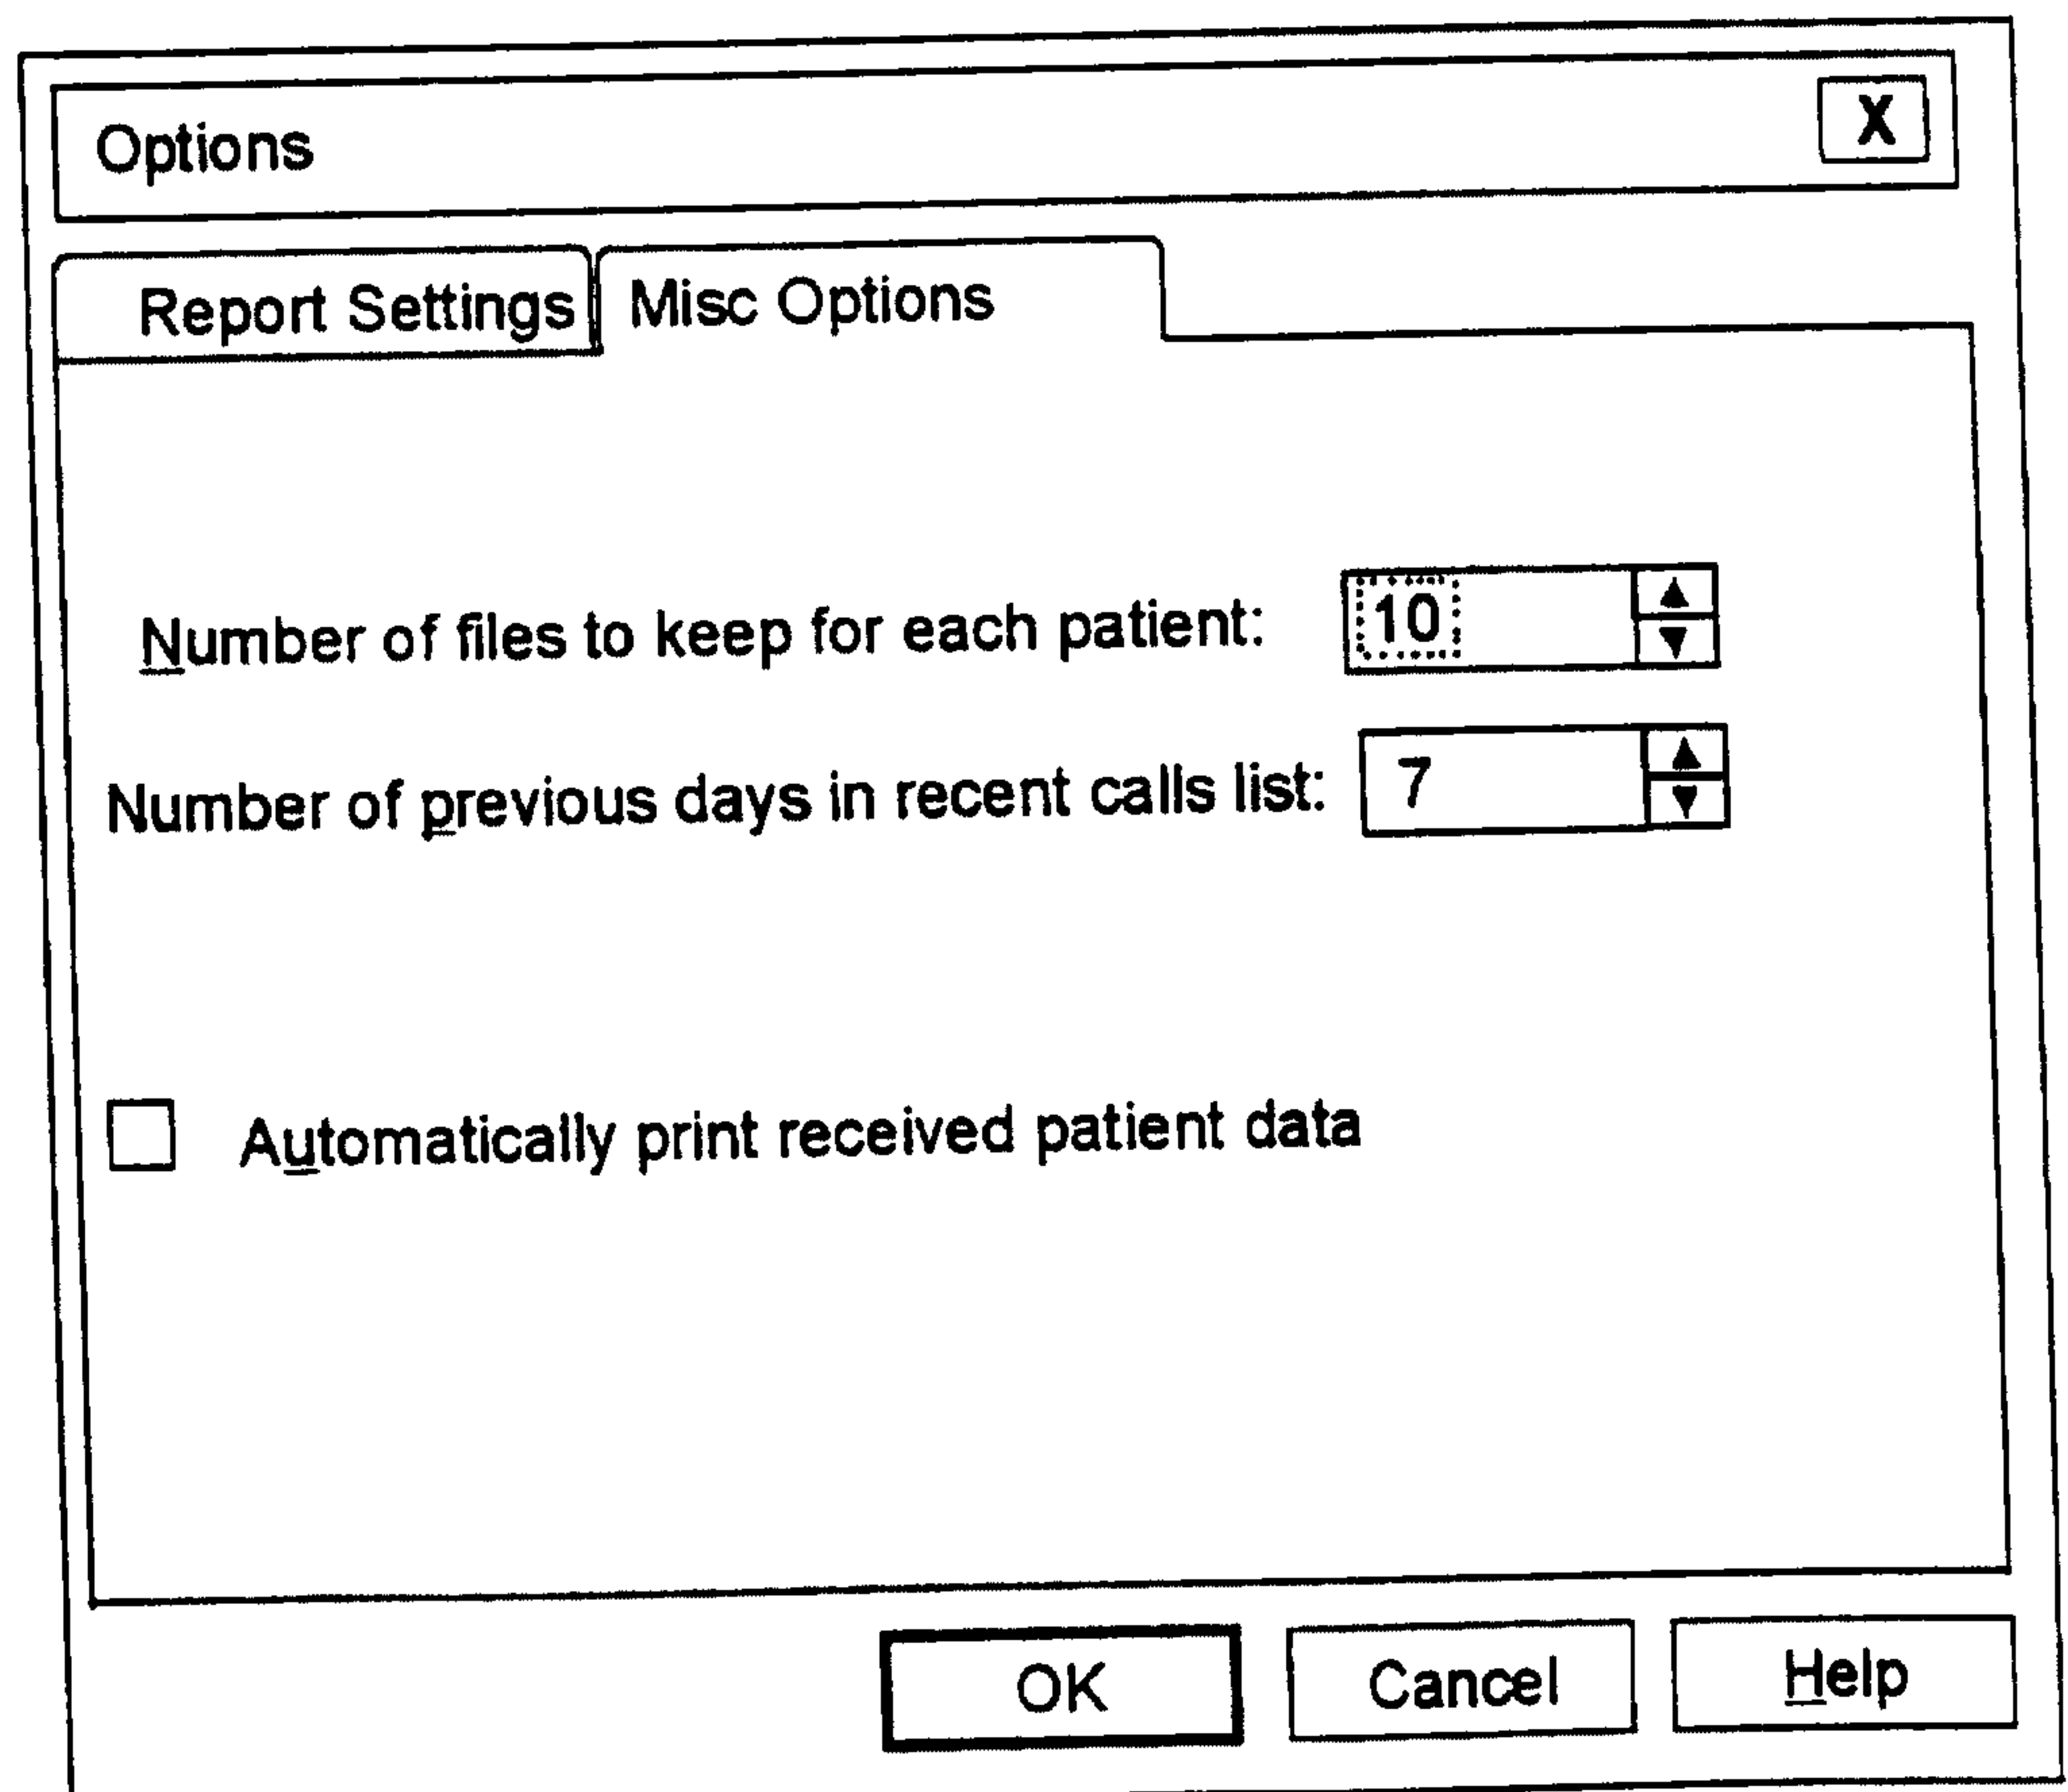

Options [X]

Report Settings Misc Options

Number of files to keep for each patient: 10 ▲▼

Number of previous days in recent calls list: 7 ▲▼

☐ Automatically print received patient data

OK Cancel Help

