




(86) Date de dépôt PCT/PCT Filing Date: 2009/04/03
(87) Date publication PCT/PCT Publication Date: 2009/10/15
(45) Date de délivrance/Issue Date: 2014/10/28
(85) Entrée phase nationale/National Entry: 2010/10/08
(86) N° demande PCT/PCT Application No.: EP 2009/002483
(87) N° publication PCT/PCT Publication No.: 2009/124695
(30) Priorité/Priority: 2008/04/11 (EP08007250.7)

(51) Cl.Int./Int.Cl. *A61F 9/01* (2006.01)
(72) Inventeur/Inventor:
VOGLER, KLAUS, DE
(73) Propriétaire/Owner:
WAVELIGHT GMBH, DE
(74) Agent: RIDOUT & MAYBEE LLP

(54) Titre : SYSTEME DE CHIRURGIE OPHTHALMOLOGIQUE PAR REFRACTION
(54) Title: SYSTEM FOR REFRACTIVE OPHTHALMOLOGICAL SURGERY

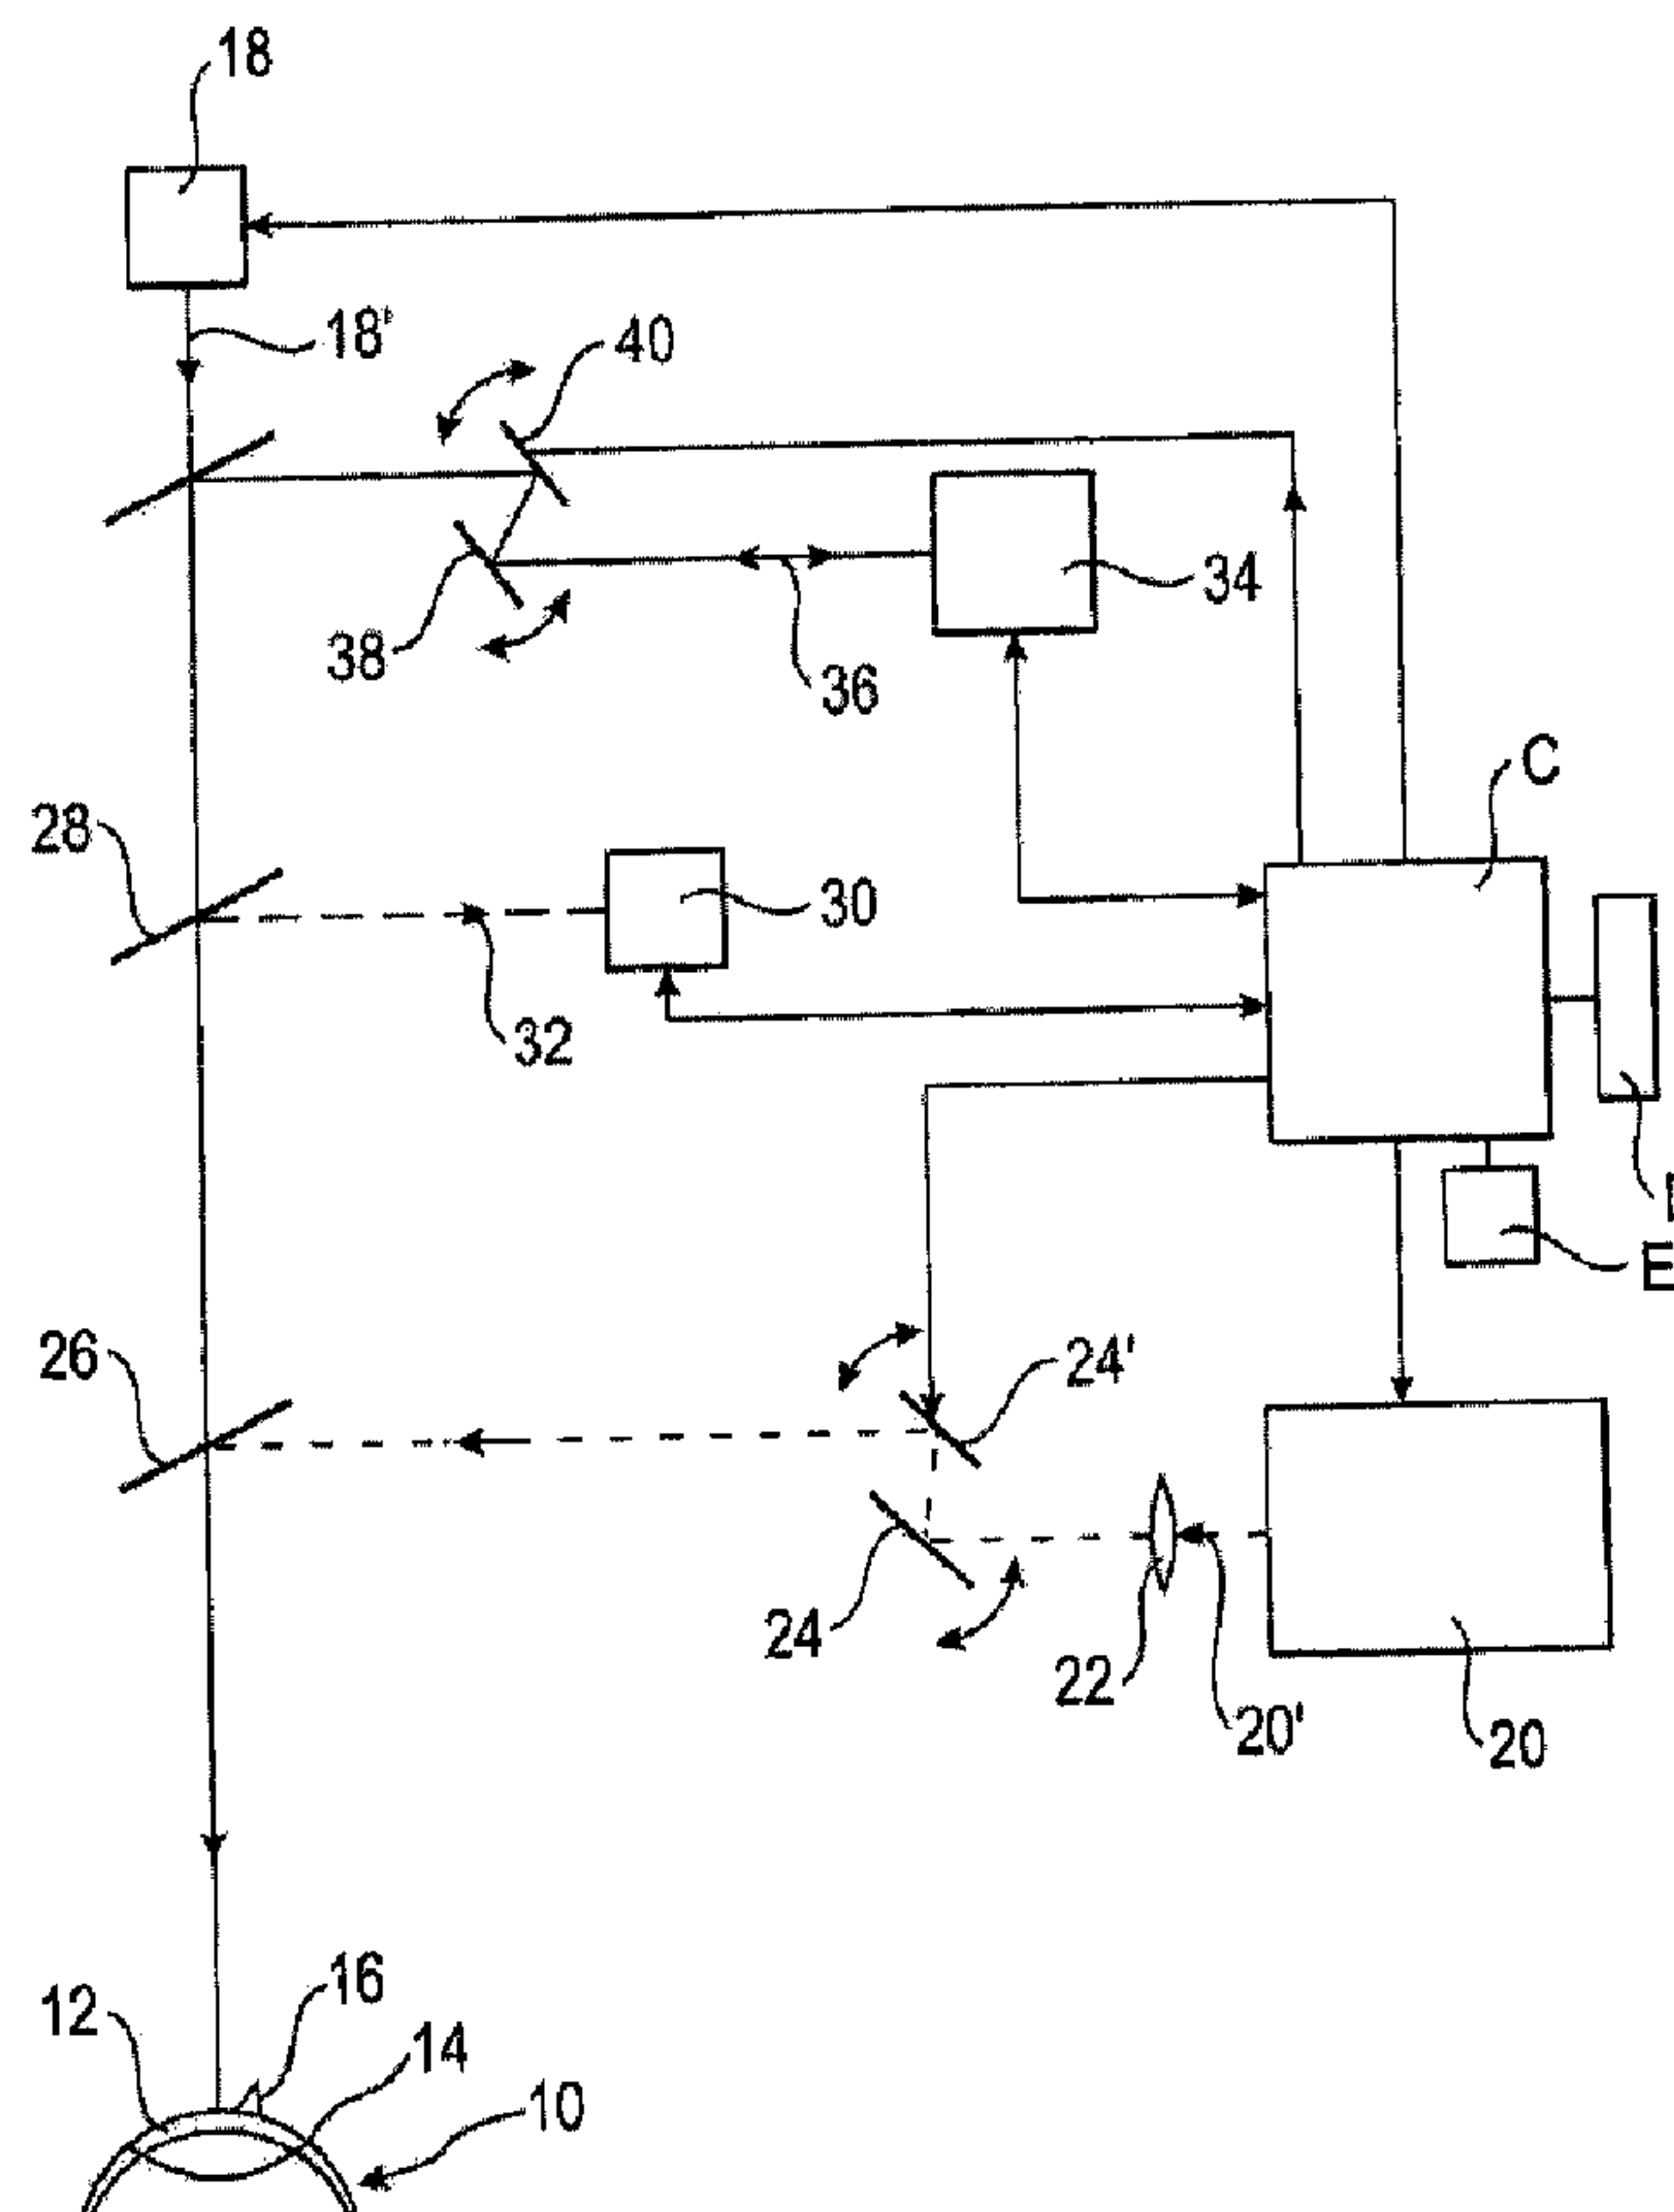

(57) Abrégé/Abstract:

A system for refractive ophthalmologic surgery, particularly for LASIK, in addition to the ablation laser and optionally further optical guiding means (18, 30), comprises a device (34) for optical coherence tomography as an integrated component in order to enable measurement results obtained with said device to either be displayed on a display device and/or to be used for controlling the ablation.



(12) NACH DEM VERTRAG ÜBER DIE INTERNATIONALE ZUSAMMENARBEIT AUF DEM GEBIET DES
PATENTWESENS (PCT) VERÖFFENTLICHTE INTERNATIONALE ANMELDUNG(19) Weltorganisation für geistiges Eigentum
Internationales Büro(43) Internationales Veröffentlichungsdatum
15. Oktober 2009 (15.10.2009)(10) Internationale Veröffentlichungsnummer
WO 2009/124695 A1(51) Internationale Patentklassifikation:
A61F 9/01 (2006.01)

(21) Internationales Aktenzeichen: PCT/EP2009/002483

(22) Internationales Anmeldedatum:
3. April 2009 (03.04.2009)

(25) Einreichungssprache: Deutsch

(26) Veröffentlichungssprache: Deutsch

(30) Angaben zur Priorität:
08007250.7 11. April 2008 (11.04.2008) EP(71) Anmelder (für alle Bestimmungsstaaten mit Ausnahme von US): **WAVELIGHT AG** [DE/DE]; Am Wolfsmantel 5, 91058 Erlangen (DE).

(72) Erfinder; und

(75) Erfinder/Anmelder (nur für US): **VOGLER, Klaus** [DE/DE]; Goethestrasse 13, 90542 Eckental (DE).(74) Anwalt: **VON HELLFELD, Axel**; Wuesthoff & Wuesthoff, Schweigerstr. 2, 81541 München (DE).

(81) Bestimmungsstaaten (soweit nicht anders angegeben, für jede verfügbare nationale Schutzrechtsart): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO,

DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Bestimmungsstaaten (soweit nicht anders angegeben, für jede verfügbare regionale Schutzrechtsart): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), eurasisches (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), europäisches (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Veröffentlicht:


— mit internationalem Recherchenbericht (Artikel 21 Absatz 3)

— vor Ablauf der für Änderungen der Ansprüche geltenden Frist; Veröffentlichung wird wiederholt, falls Änderungen eingehen (Regel 48 Absatz 2 Buchstabe h)

(54) Title: SYSTEM FOR REFRACTIVE OPHTHALMOLOGIC SURGERY

(54) Bezeichnung: SYSTEM FÜR DIE REFRAKTIVE OPHTHALMOLOGISCHE CHIRURGIE

Fig. 1

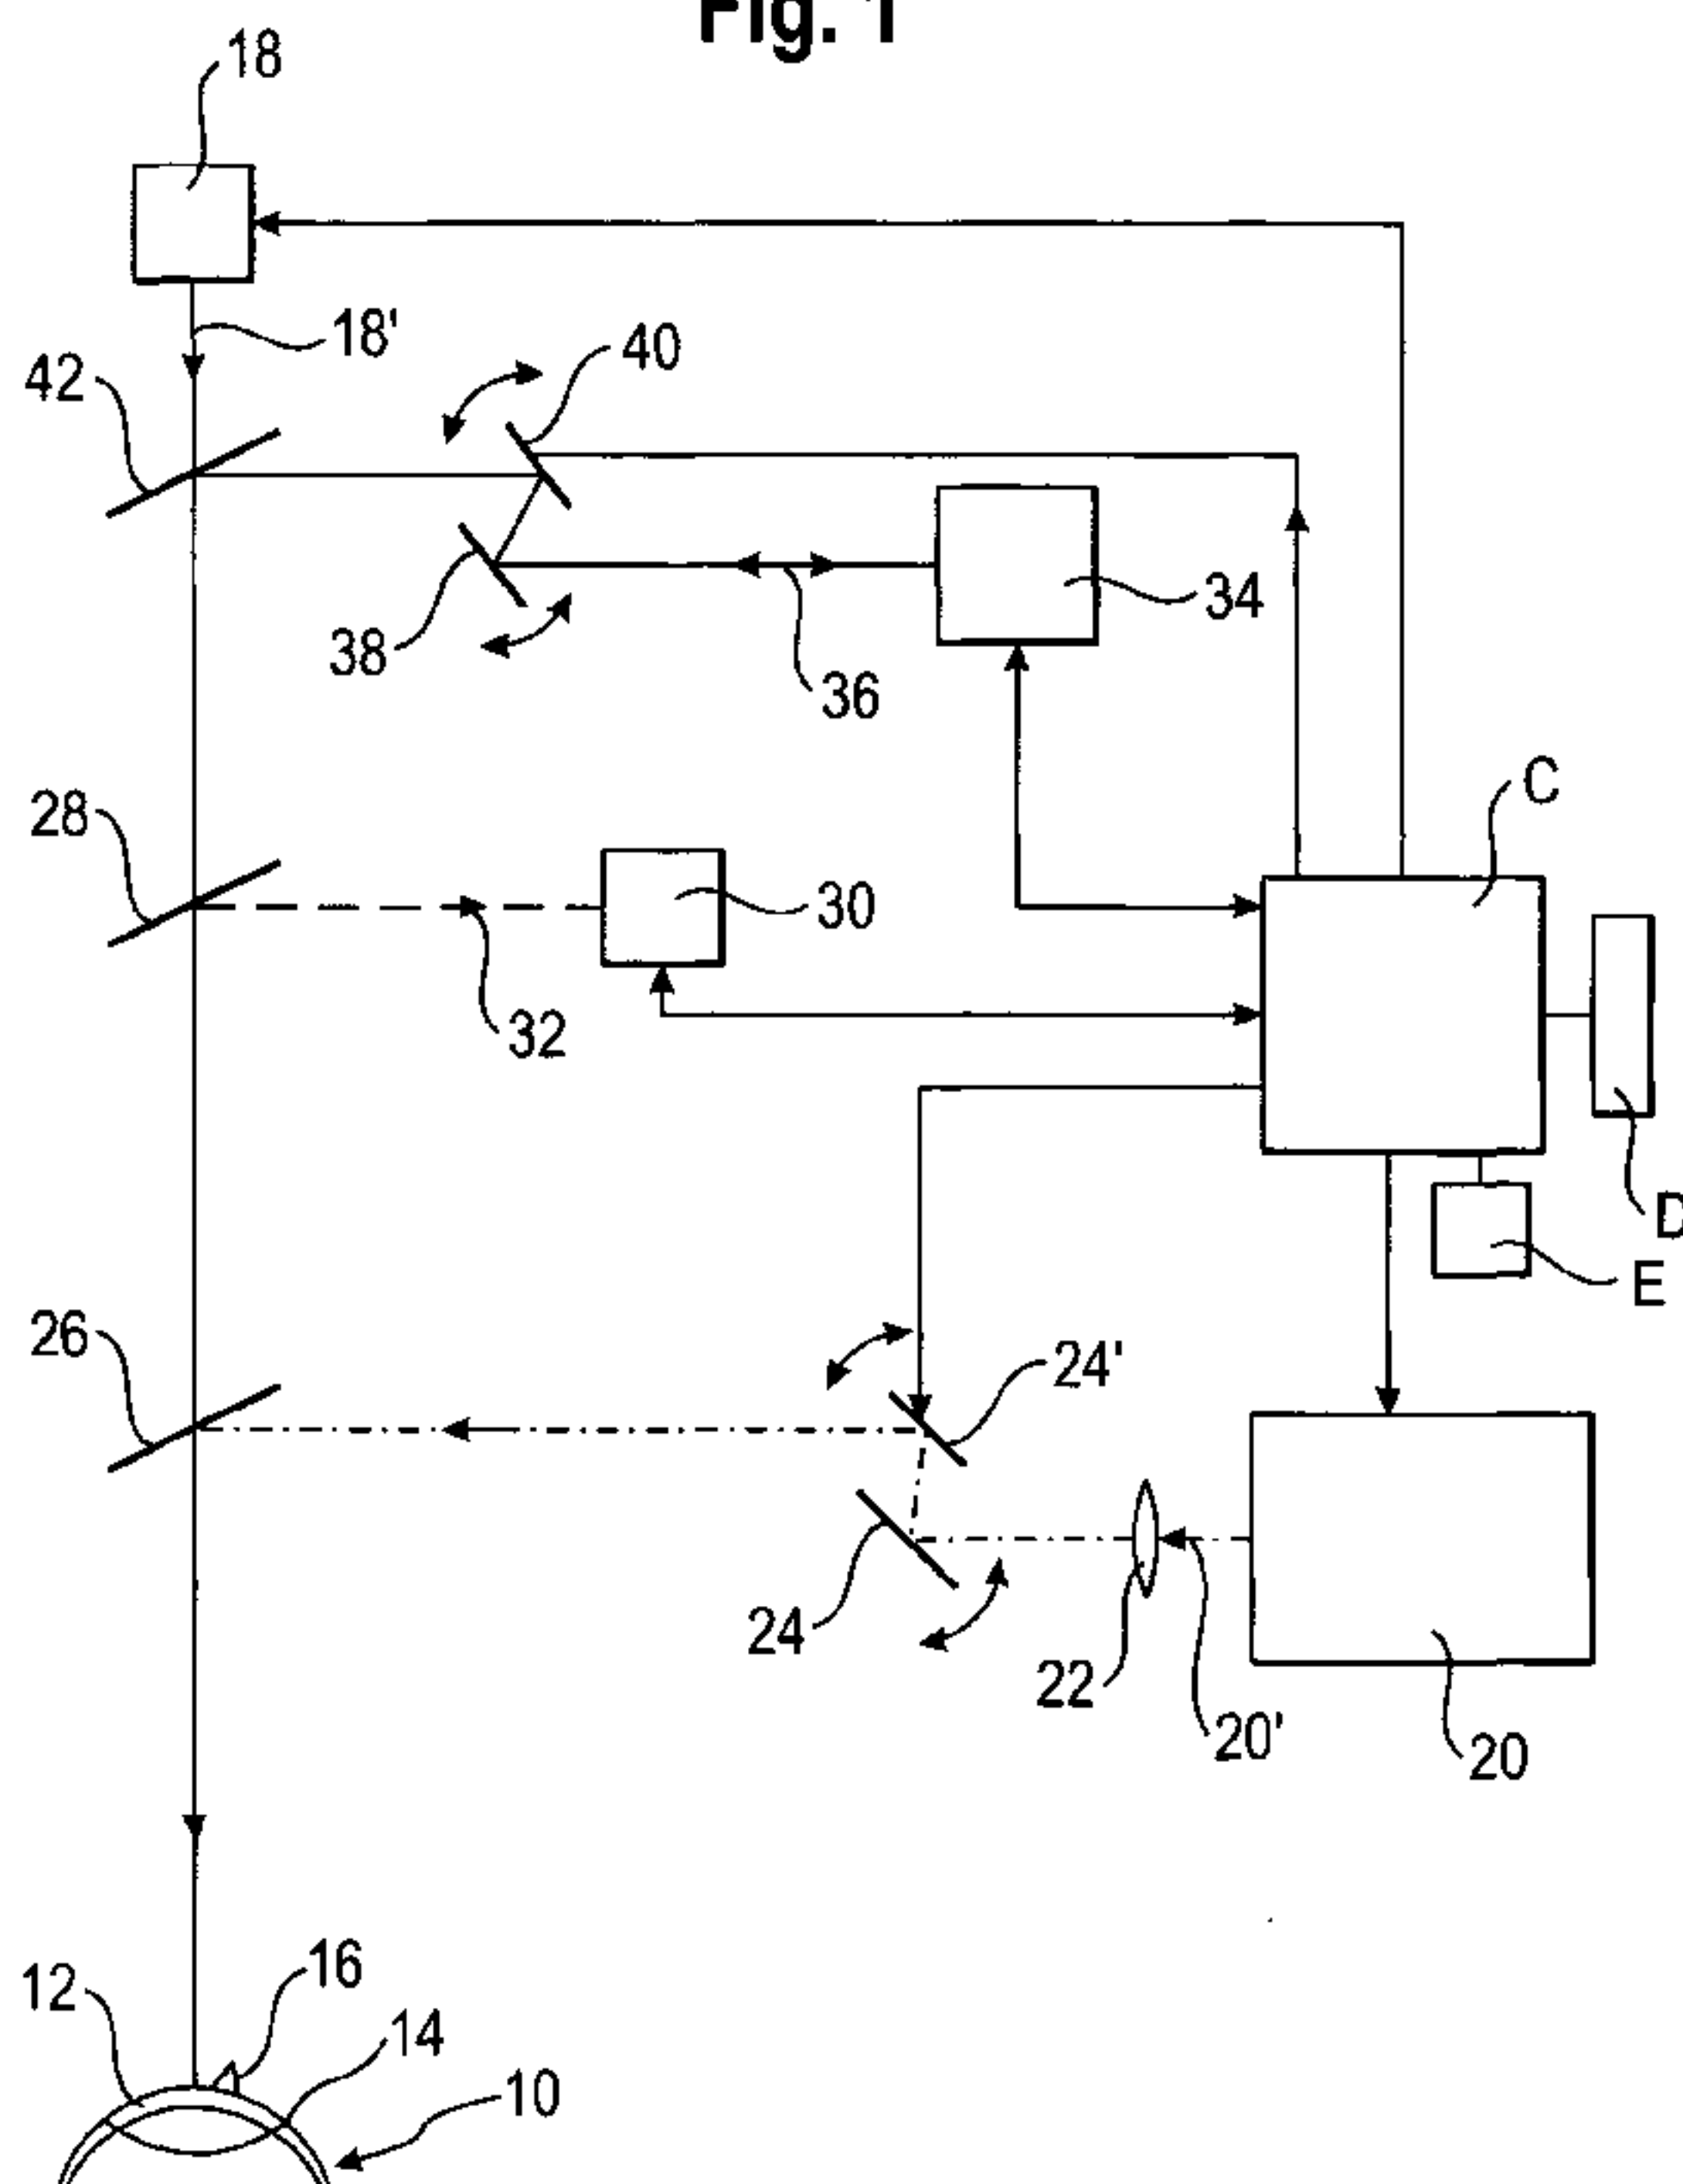

(57) Abstract: A system for refractive ophthalmologic surgery, particularly for LASIK, in addition to the ablation laser and optionally further optical guiding means (18, 30), comprises a device (34) for optical coherence tomography as an integrated component in order to enable measurement results obtained with said device to either be displayed on a display device and/or to be used for controlling the ablation.

(57) Zusammenfassung: Ein System für die refraktive ophthalmologische Chirurgie, insbesondere die LASIK, hat zusätzlich zum Ablationslaser und gegebenenfalls weiteren optischen Führungsmitteln (18, 30) als integrierten Bestandteil eine Einrichtung (34) für die optische Kohärenztomographie, um mit dieser Einrichtung gewonnene Messergebnisse entweder zur Darstellung auf einer Anzeigeeinrichtung und/oder zur Steuerung der Ablation zu ermöglichen.

- 1 -

System for refractive ophthalmological surgery

The invention relates to a system for refractive ophthalmological surgery.

5

In refractive ophthalmological surgery the optical refractive properties of the eye, particularly of the cornea, are changed by using laser radiation in order to correct or at least alleviate visual deficiencies. A prominent example of refractive ophthalmological surgery is LASIK, in which corneal tissue is resected (ablated) in order to reshape the cornea for the purpose of correcting sight defects. For the purpose of resecting corneal tissue, as a rule an excimer laser in the UV region (typically 193 nm) is employed. The laser radiation is guided over the eye in such a way with respect to time and location that a certain amount of tissue is resected at selected points in the cornea. This resection is described by the so-called ablation profile, i.e. the ablation profile specifies the resection (ablation) to be performed at each point in the cornea.

10
15

The present invention relates, in particular, to LASIK.

20

The ablation profile is calculated, as a rule, prior to implementation of the surgical intervention in respect of the eye to be corrected. The basis of this calculation is a surveying of the eye in its actual state. For this surveying of the eye, the state of the art is familiar with a variety of techniques, in particular topography-measuring instruments (so-called topolyzers), wavefront analysers, Scheimpflug instruments and also pachymeters.

25

30

Refractive ophthalmological surgery with a wavefront analyser or with a topography-measuring instrument is hardly capable of resolving small local structures of the cornea within the millimetre range effectively, let alone of assigning them in defined and locally exact manner, in order to enable a locationally faithful treatment. With topolyzers it is also hardly possible to detect so-called central islands within the millimetre range – that is to say, prominences on the cornea which often originate from preceding, not entirely perfect, operations from the early days of PRK.

35

- 2 -

At present, attempts are being made to track deviations from the desired ablation process in online manner during the ablation, in particular deviations that are based on a so-called cyclotorsion or on a so-called pupil center shift.

5 But with these processes that are known at present it is, as a rule, not possible to detect local corneal irregularities precisely and to put the laser beam into effect in the course of such a detection in precisely local manner only at this point, and in the process also to track the outcome of the ablation.

10 So-called optical coherence tomography has been available for some time as a measuring process for non-contacting surveying of biological tissues, cf. for example B. Wolfgang Drexler, Journal of Biomedical Optics, 9(1), 42-74, 2004. With optical coherence tomography, in particular using broadband irradiators, it is possible to survey very fine biological structures, in particular with resolutions
15 in the region of 1 μm and finer.

EP 1 231 496 A2 describes the application of optical coherence tomography (OCT) for the controlled alteration of tissue in the eye, the treatment laser being controlled as regards power, exposure-time and spot-size. Treated ocular tissue
20 is distinguished therein from untreated ocular tissue by means of OCT and a threshold value. The region of the ocular tissue that has been successfully treated with the laser is determined with OCT.

US 2007/0282313 A1 (Huang et al.) describes the use of OCT only for the purpose of topographical surveying in refractive surgery. No reference is to be
25 found therein to an online-controlled photoablation by means of OCT. In this state of the art the topographical data acquired with OCT are utilised merely for the advance calculation of an ablation program.

30 EP 0 697 611 A2 describes a system similar to that of EP 1 231 496 A2, discussed above, with an autofocus system for an ophthalmological surgical microscope. Topographical measurements in respect of the cornea are effected therein, but no online control of a resection of tissue with OCT.

- 3 -

US 2007/0073905 A1 does not use OCT but describes generally the state of the art of a surgical intervention in respect of the eye using previous model calculations.

WO 2006/087180 A2 describes a process for ablation, though without using OCT.

DE 103 23 422 A1 also does not describe a use of OCT, but only the detection of an optical pressure range in the tissue.

The object underlying the invention is to provide a system of the type stated in the introduction that enables improved surgical outcomes.

To this end, the invention teaches a system for refractive ophthalmological surgery with

- a) a first laser adapted to resect corneal tissue for changing the optical refractive properties of the eye,
- b) means for time-controlled and location-controlled guidance of the radiation of the first laser onto the eye,
- c) a device for optical coherence tomography with a second laser for implementing optical coherence tomography in respect of the eye,
- d) means for time-controlled and location-controlled guidance of the radiation of the second laser onto the eye, and with
- e) a computer which
 - e1) in the course of the resection of corneal tissue in accordance with a program controls the first laser and the stated means for time-controlled and location-controlled guidance of the radiation of the first laser onto the eye for the purpose of achieving a reshaping of the cornea,
 - e2) controls the device for optical coherence tomography and is programmed in such a way that during the resection of corneal tissue measurements in respect of the cornea (12) are carried out, wherein the computer is programmed in such a way that also before the start of and after conclusion of the resection of corneal tissue measurements in respect of the cornea are carried out, the computer under specifiable conditions, controls the program flow for the resection of corneal tissue subsequent to a measurement by means of optical coherence tomography depending on the result of the measurement.

- 4 -

The invention accordingly integrates a module for optical coherence tomography (OCT) into a system for refractive ophthalmological surgery in such a manner that the results of measurement acquired thereby have an influence, in virtually online manner, on the process of the surgical intervention. In particular, high-resolution and high-speed OCT (HHS-OCT) enables the ascertainment and representation of the corneal structures with resolutions within the μm range at very high speed by virtue of scanning-rates within the range from a few MHz up to several GHz, in particular up to 10 GHz and even up to 100 GHz, and with measuring-times distinctly shorter than one second. Hence it is possible not only to survey the initial structure prior to the resection of corneal tissue and the final structure of the cornea after the resection, but also to track the entire progress of the treatment in between and to control the treatment in a manner depending on results of OCT measurement that are acquired during the treatment.

According to the present invention, a resection of tissue, guided by OCT, is, in particular, effected with a UV laser (typically an excimer laser), in the course of which certain areas of the cornea are targeted and then corneal tissue is resected via a number of shots which are controlled in real time (online) until the OCT measurement in virtually real time (online) yields the desired result of measurement.

By reason of the integration of the OCT module into the system for refractive surgery, it is moreover possible to recognise certain irregularities of the cornea, in particular the so-called central islands, and to take them into account in the treatment. Such central islands – that is to say, irregular prominences on the corneal surface – have dimensions in the region of a few millimetres and less and were therefore barely capable, or not capable, of being registered by conventional measuring methods in the course of refractive surgery. Such irregularities were also not discoverable, or barely discoverable, before or during the treatment, or accurately addressable for the laser control. Corresponding remarks apply in respect of extremely fine irregularities in the form of scars which likewise sometimes arise on the corneal surface.

With broadband optical coherence tomography such irregularities are recognisable, and correspondingly the ablation profile can be formed in such a way that,

- 5 -

for example, in the region of central islands (that is to say, prominences on the cornea) locally more corneal tissue is resected in targeted manner than in other regions of the cornea, so that a smooth surface arises overall, whereas in the case of the aforementioned scars the resection in the region of these scars is so greatly reduced that, as a result, a substantially smooth corneal surface likewise arises. If in the state of the art such irregularities were not recognised in the result of measurement and taken in account in the ablation, they were substantially preserved in the course of the ablation and resulted in corresponding irregularities also on or in the treated cornea.

With the integration, according to the invention, of OCT into the system for refractive ophthalmological surgery, it is possible to detect the exact corneal structure as regards cross-section, thickness, anterior surface and posterior surface, and to track it momentarily (instantaneously) during the treatment. Therefore a special configuration of the invention teaches to calculate during the ablation process (that is to say, during the refractive surgery) virtually in real time (online) the respective momentary imaging properties of the cornea such as obtain momentarily by reason of the ablation stage that has been reached, and to conclude the ablation precisely when the imaging properties of the eye that have been calculated online in this way correspond to a desired, specifiable objective. This makes parallel topographical measurements or even wavefront measurements no longer absolutely necessary.

A preferred configuration of the system according to the invention for refractive ophthalmological surgery provides that the computer is programmed in order to represent on a display device results of measurement acquired in the course of optical coherence tomography before and/or during the resection of corneal tissue. In this way the treating physician can inspect virtually in online manner - that is to say, practically in real time - the progress of the ablation, represented graphically. For example, the initial shape of the cornea (before the start of the intervention) can be presented to the physician on the display screen by means of a line (in the case of two-dimensional representation) or by means of a surface (in the case of three-dimensional representation), and then, below that, correspondingly the momentary corneal structure by means of a, for example, colour-contrasted line or surface successively during the intervention. In this connection, in addition the surface of the cornea on the inside of the eye, which

- 6 -

is also capable of being surveyed with coherence tomography, can also be optionally indicated to the physician. This helps, in particular, to avoid excessively thin residual thicknesses of the cornea. Further structures of the eye being treated that are of interest, such as the lens and/or the pupil, can also be surveyed with OCT and represented on the display device.

If the aforementioned process is employed in the course of LASIK and if in this case the so-called flap incision is carried out with a femtosecond laser, for example, then the incision arising can be tracked with OCT and represented on the display device, and in the course of the subsequent ablation of corneal tissue the aforementioned lines or surfaces in the graphical representation can be ascertained by computation in such a way that the situation after folding the flap back and after the assumed healing process can be calculated and represented.

Another preferred configuration of the invention provides that an input device is provided, with which a user can cause the computer to bring about an additional resection of corneal tissue with the first laser within a selected range of the represented results of measurement of optical coherence topography, or to reduce the resection of corneal tissue within a selected range.

The invention also teaches the use of extremely fast devices for OCT using femtosecond radiation-sources, preferably with repetition-rates in the region of 10 GHz and preferably in the region of 100 GHz or more, in particular the use of so-called VECSELs or VCSELs (Vertical External Cavity Surface Emitting Lasers). Such semiconductor laser diodes can be pumped electrically or optically and attain very high outputs and efficiencies, despite a physical size within the centimetre range. Femtosecond fibre lasers may also be employed for the invention. The invention also teaches the use of such radiation-sources with generation of fs supercontinua with bandwidths greater than 100 nm up to 1000 nm and with repetition-rates greater than 100 GHz, so that an extremely high measuring-rate can be attained – that is to say, the generation of images of structures of the cornea on, for example, a display screen with an extremely short time-delay in comparison with the state of the cornea actually achieved momentarily in the course of an ablation procedure, i.e. the actual state of the cornea is represented graphically virtually in real time (without time-delay) and may also be processed by computation without time-delay.

- 7 -

An exemplary embodiment of the invention will be described in more detail in the following on the basis of the drawings. Shown are:

Fig. 1 schematically, a system for refractive ophthalmological surgery;
5 and

Fig. 2 schematically, a display device for displaying data acquired with optical coherence tomography.

Figure 1 shows an eye 10 to be treated by refractive ophthalmological surgery, schematically the cornea 12 thereof, the pupillary margin 14 and a so-called irregularity 16 of the cornea, here in the form of a so-called central island – that is to say, a prominence on the cornea having dimensions within the mm range to μm range.

15 In known manner the system exhibits a fixation laser 18 which emits a (weak) laser beam 18' and is sighted by the patient for the purpose of fixing the eye.

In a manner known as such, the system exhibits - as in the case of a LASIK apparatus - a UV laser 20, for example an excimer laser, which emits radiation 20' with a wavelength of 193 nm which is directed onto scanner mirrors 24, 24' via a lens 22 and is deflected onto the eye 10 via a deflecting mirror 26. A computer C controls the laser 20 and the scanner mirrors 24, 24', in a manner conventional as such, in accordance with a previously calculated ablation profile. With the system that has been presented, a LASIK, for example, is carried out in
25 known manner.

The system exhibits moreover a so-called eye-tracker. The eye-tracker includes a camera 30 with which images from the eye 10 in the direction of the arrow 32 are recorded via a deflecting mirror 28, which are then subjected to image processing in a manner known as such, in order to track movements of the eye
30 which the patient frequently cannot avoid, despite the fixation laser 18, and to track the control of the scanner mirrors 24, 24' for the laser beam 20' in a man-

- 8 -

ner corresponding to the movements of the eye, so that the ablation profile is resected in a manner that is as locationally faithful as possible.

5 The digitally acquired recordings of the camera 30 are processed in the computer C, and the computer C then controls the scanner mirrors 24, 24' correspondingly with respect to the ablation beam 20'.

10 Integrated into the system for LASIK is a device 34 for optical coherence tomography, which in a manner known as such includes an appropriate laser. The device 34 for optical coherence tomography emits radiation and receives radiation in accordance with the double-headed arrow 36. The scanning is effected via scanner mirrors 38, 40. The interaction of the computer C with the individual components is indicated in Figure 1 by lines and arrows. Correspondingly, the computer C controls the device 34 for optical coherence tomography and the scanner mirrors 38, 40 pertaining thereto.

15 The device 34 for optical coherence tomography operates with scanning-rates in the region of a few MHz up to scanning-rates within the GHz range, depending on the radiation-source being used, so that measuring-times for an entire surface to be surveyed (that is to say, corresponding roughly to the ablation region of the cornea) are attained that are distinctly shorter than 1 second.

20 The radiation-source of the device 34 for optical coherence tomography - for example, a laser - is an extreme broadband radiation-source with a broadband measure distinctly greater than 100 nm and with very high repetition-rates greater than 10 MHz up to more than 100 GHz. This enables a high three-dimensional resolution in the region of 10 μm and better. In this case, an image of interest of a surface of the cornea - for example, the momentary surface during the successive ablation - can be surveyed in less than 1 second and can be represented on a display device D via the computer C. The broadband radiation with $\Delta\lambda \gg 100$ nm has centre wavelengths λ in the region of about 800 nm to 1300 nm. Hence, according to the exemplary embodiment that is shown, the topography of the cornea, the thickness thereof, the extent of the anterior chamber of the eye and the local position of the adjoining structures - such as iris and crystalline lens - are surveyed, and corresponding geometrical images of

- 9 -

these structures are represented, alternatively and in desired combination, on the display device D via the computer C.

The resolution in depth (ordinarily designated as the z-direction) in this case lies within the μm range, for example better than $3\ \mu\text{m}$, whereas in the transverse direction (ordinarily designated as the xy-direction) resolutions distinctly better than $10\ \mu\text{m}$ are likewise attained. Hence substructures of the cornea - such as the epithelium, Bowman's membrane, or the position of the microkeratome incision in the case of LASIK - can be recognised well.

Figure 2 shows schematically a representation with OCT-surveyed structures on the display device D in accordance with a control by the computer C. Shown is the surface K1 of the cornea obtaining before the start of the ablation, with a first irregularity I in the form of a central island – that is to say, a prominence. The prominence has dimensions within the mm range to μm range (is accordingly extremely enlarged in the Figure in comparison with the dimensions of the cornea). The two flanks of the prominence have gradients G1, G2, i.e. slopes in relation to the adjoining surface K1 of the cornea 12. Moreover, in the example that is represented the surface K1 of the cornea 12 has scars N which likewise have dimensions within the mm range to μm range.

Moreover, Figure 2 shows the set surface K2 of the cornea to be striven for on the basis of the calculated resection of the ablation profile – that is to say, the outcome of the operation to be striven for. Figure 2 also shows the inner surface K3 of the cornea schematically.

With the device 34 for optical coherence tomography and with the computer C which processes the results of measurement of said device, the curve K1 according to Figure 2 can be generated and can be represented on the display device D. In this connection the computer C is programmed in such a way that it recognises the stated irregularities having dimensions within the μm range and, according to an option of the user, represents them in emphasised manner, for example in colour or by means of thick lines. With processes of image processing that are known as such, the computer can 'recognise' the irregularities on the basis of the gradients G1, G2 by comparison with specifiable threshold values and can represent them. In the course of image processing, for example,

- 10 -

by comparison of contiguous measuring-point ranges a gradient G1, G2 can be recognised that lies above a specified threshold value and indicates that an irregularity is possibly present at this point. According to a preferred configuration, the option can then be made available to the user to call up and represent
5 an enlarged representation of the momentary state of the cornea in this critical region. This representation can be continually repeated online during the implementation of the ablation – that is to say, during the stepwise resection of corneal tissue, layer by layer - so that the physician can track the progress of the treatment - i.e. the temporal procedure of the successive resection of corneal
10 tissue, layer by layer - on the display device D on the basis of the measurements by coherence tomography. If on the basis of the irregularities the physician detects certain problem regions in which a stronger ablation or even a weaker ablation than originally stipulated in accordance with the ablation profile is required, then according to a preferred configuration he/she can intervene in the
15 process directly. If, for example, the physician detects on the representation an irregularity corresponding to the prominence I (central island), then he/she can place markers M1 M2, between which in this case an increased resection of corneal tissue in comparison with the surrounding regions of the cornea is required, and he/she can set the markers M1, M2 corresponding to the delimita-
20 tion of this region via an input device E. It will be understood that these markers are to be placed three-dimensionally – that is to say, also in the downward direction from the plane of the drawing they have roughly the dimension that is given in the plane of the representation. The physician can then specify via the input device E how strong the additional resection of tissue is to be in the
25 region of the irregularity.

Corresponding remarks apply to the region of the scars N, in which the ablation then has to be diminished where appropriate, in order, as a result, in cases of all irregularities then to obtain a relatively smooth corneal surface as designated by
30 K2 in Figure 2.

- 11 -

List of Reference Symbols

	10	eye
5	12	cornea
	14	pupillary margin
	16	scar or central island
	18	fixation laser
	18'	fixation laser beam
10	20	UV laser
	22	lens
	24	scanner mirror
	24'	scanner mirror
	26	deflecting mirror
15	28	deflecting mirror
	30	camera
	32	arrow
	34	OCT system
	36	double-headed arrow
20	38	scanner mirror
	40	scanner mirror
	C	computer
	D	display
	E	input
25	I	central island
	N	scar(s)
	M1,M2	markers
	G1,G2	gradients
	K1,K2,K3,K4	surfaces

- 12 -


Claims

1. System for refractive ophthalmological surgery with
 - a) a first laser adapted to resect corneal tissue for changing the optical refractive properties of the eye,
 - b) means for time-controlled and location-controlled guidance of the radiation of the first laser onto the eye,
 - c) a device for optical coherence tomography with a second laser for implementing optical coherence tomography in respect of the eye,
 - d) means for time-controlled and location-controlled guidance of the radiation of the second laser onto the eye, and with
 - e) a computer which
 - e1) in the course of the resection of corneal tissue in accordance with a program controls the first laser and the stated means for time-controlled and location-controlled guidance of the radiation of the first laser onto the eye for the purpose of achieving a reshaping of the cornea,
 - e2) controls the device for optical coherence tomography and is programmed in such a way that during the resection of corneal tissue measurements in respect of the cornea are carried out,
 - e3) controls, under specifiable conditions, the program flow for the resection of corneal tissue subsequent to a measurement by means of optical coherence tomography depending on the result of the measurement, and
 - e4) is programmed in order to represent results of measurement acquired in the course of optical coherence tomography on a display device before and/or during the resection of corneal tissue; and
 - f) an input device with which a user can cause the computer to bring about an additional resection of corneal tissue with the first laser within a first selected range of represented results of measurement of optical coherence topography or to reduce the resection of corneal tissue within a second selected range.

- 13 -

2. System for refractive ophthalmological surgery according to claim 1, wherein the representation of the results of measurement acquired with optical coherence tomography includes an at least two-dimensional image of a curve which reproduces, before and/or during the resection of corneal tissue, the respectively current state of a corneal surface to be treated or being treated.
3. System for refractive ophthalmological surgery according to claim 1, wherein:
an input device is provided, with which a user can cause the computer to
bring about an additional resection of corneal tissue with the first laser within a first selected range of the represented results of measurement of optical coherence topography or to reduce the resection of corneal tissue within a second selected range;
the representation of the results of measurement acquired with optical coherence tomography includes an at least two-dimensional image of a curve which reproduces, before and/or during the resection of corneal tissue, the respectively current state of a corneal surface to be treated or being treated; and
the computer is programmed in such a way that the first selected range is capable of being marked by the user in relation to the image.
4. System for refractive ophthalmological surgery according to any one of claims 1 to 3, wherein the computer is programmed in such a way that the results of measurement acquired with optical coherence tomography are analysed as to whether a corneal surface to be ablated exhibits an irregularity.
5. System for refractive ophthalmological surgery according to claim 4, wherein the stated analysis includes the ascertainment of gradients of the corneal surface.

1/2

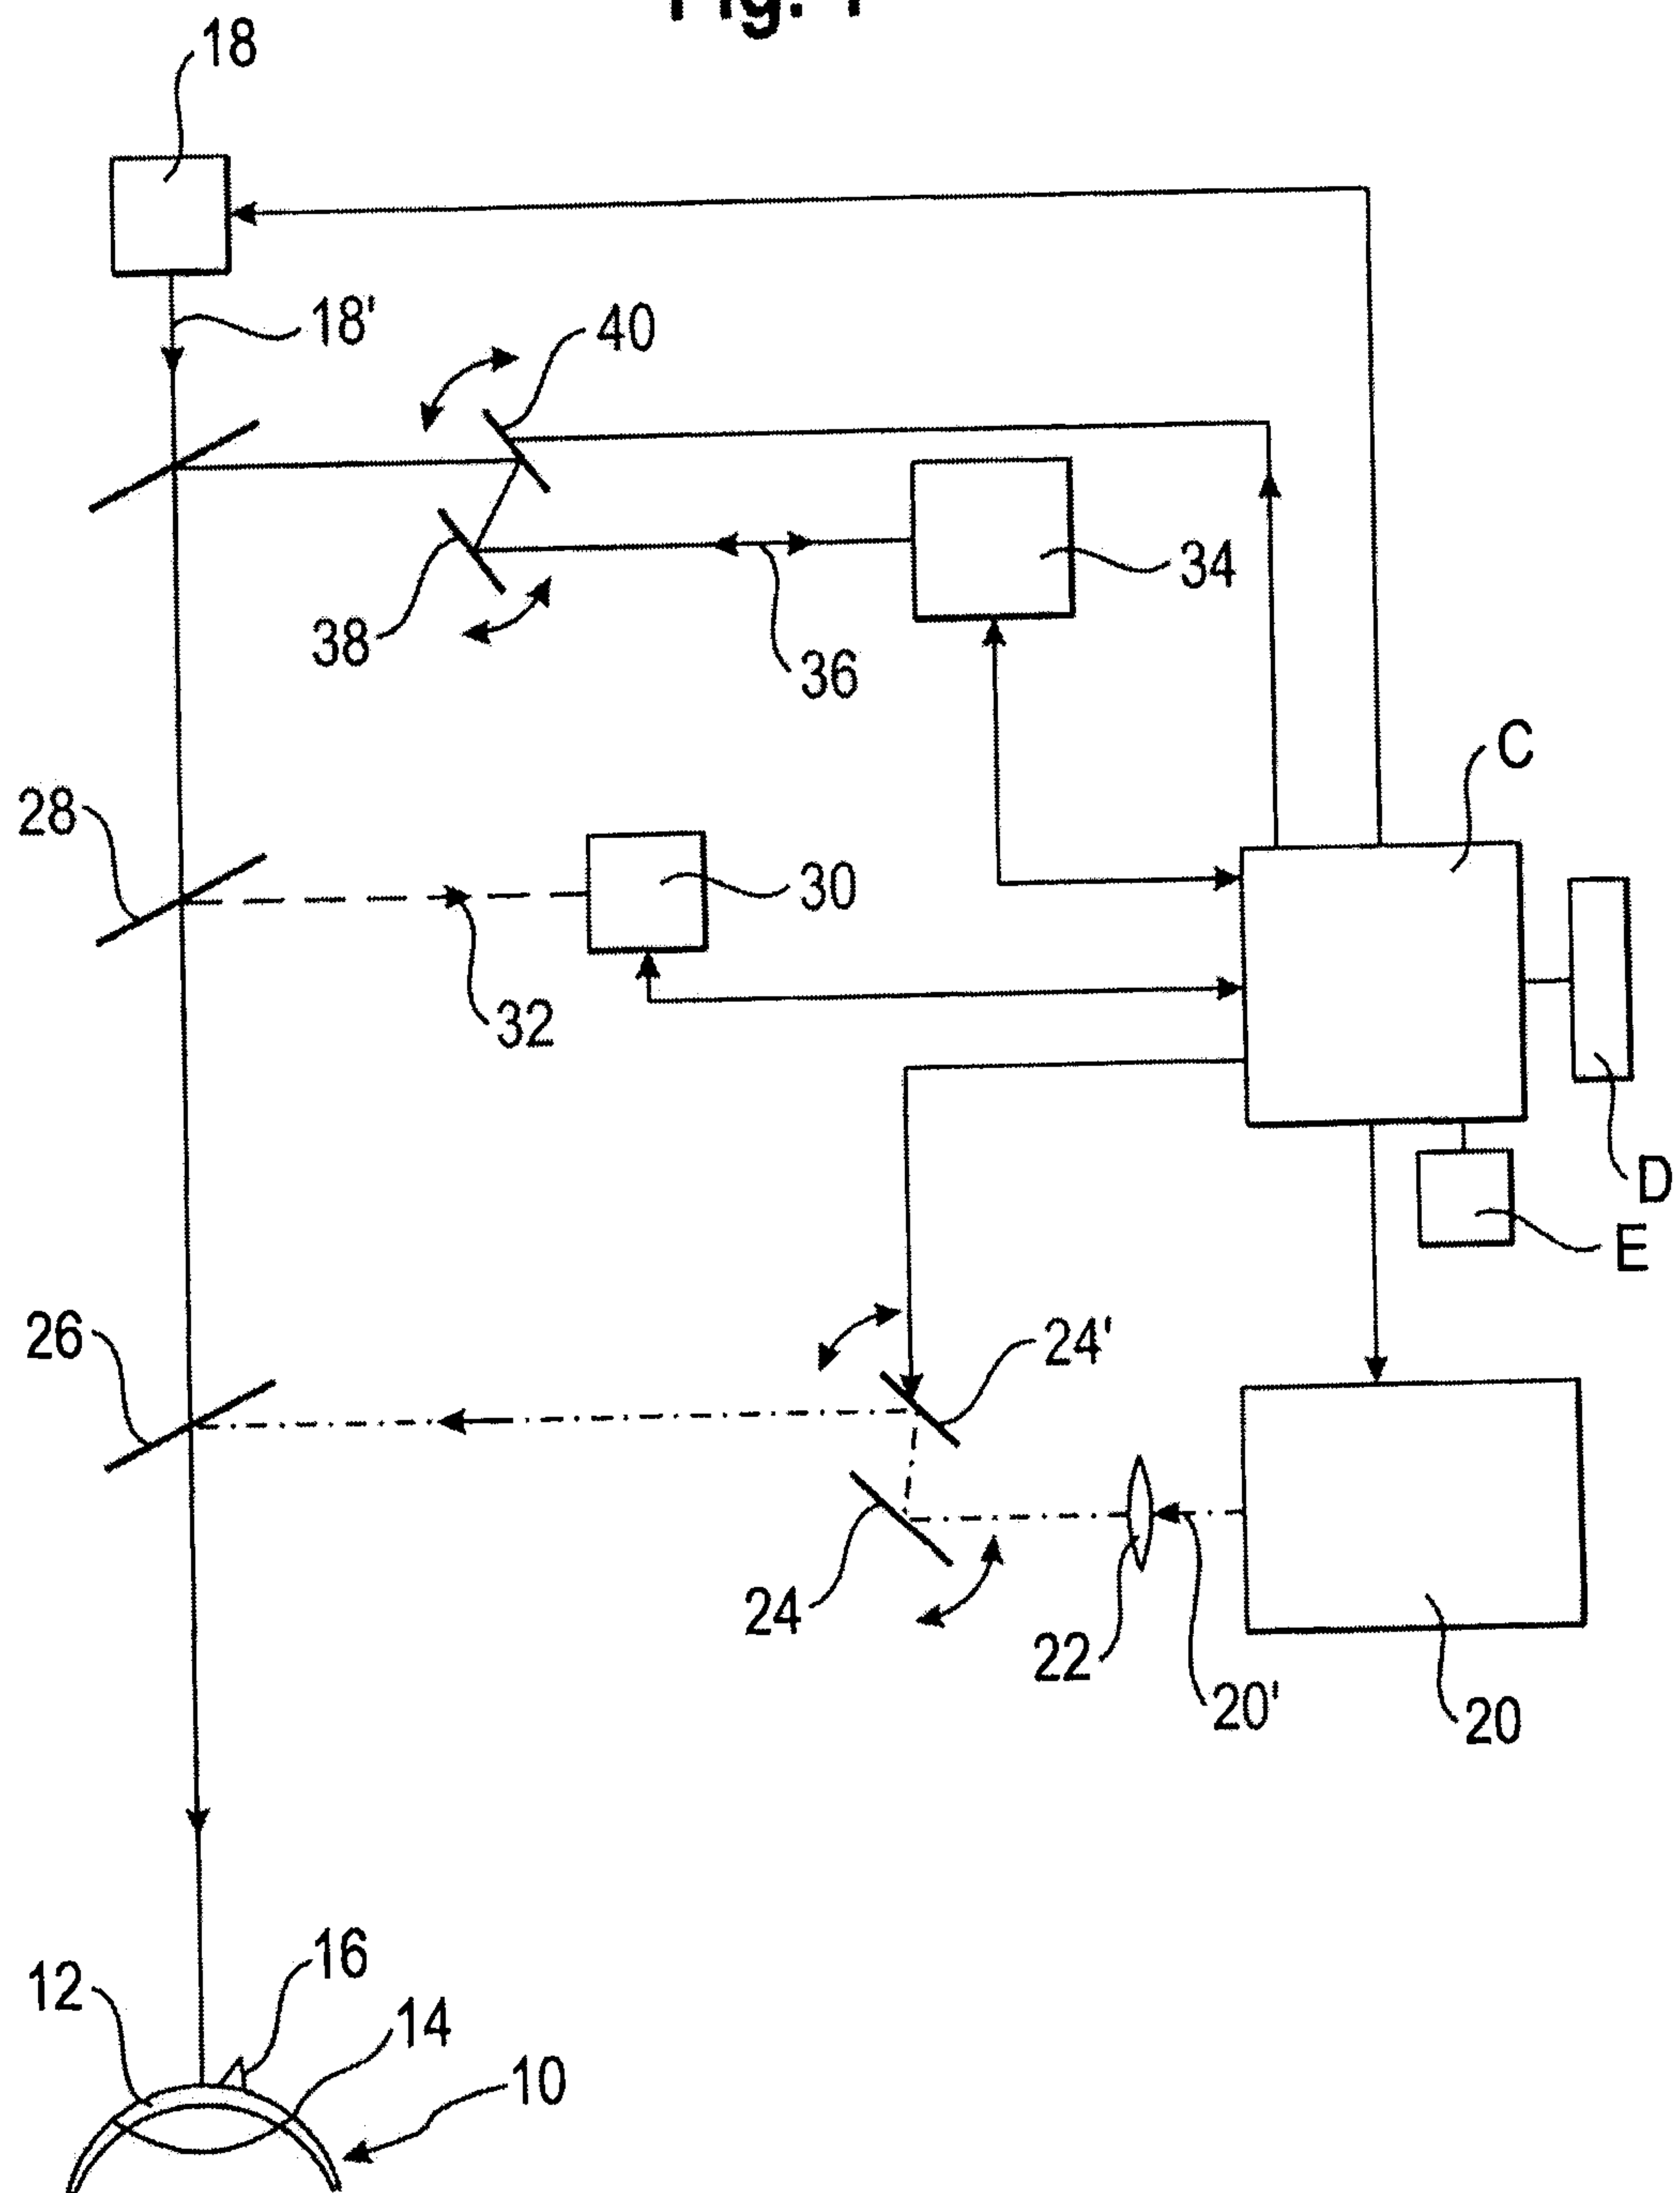Fig. 1

2/2

Fig. 2