



(86) Date de dépôt PCT/PCT Filing Date: 2003/07/02
(87) Date publication PCT/PCT Publication Date: 2004/01/15
(45) Date de délivrance/Issue Date: 2013/06/11
(85) Entrée phase nationale/National Entry: 2004/12/31
(86) N° demande PCT/PCT Application No.: NL 2003/000485
(87) N° publication PCT/PCT Publication No.: 2004/004786
(30) Priorité/Priority: 2002/07/02 (EP02077626.6)

(51) Cl.Int./Int.Cl. *A61K 49/18* (2006.01),
A61K 51/12 (2006.01), *A61P 35/00* (2006.01)
(72) Inventeurs/Inventors:
NIJSEN, JOHANNES FRANCISCUS WILHELMUS, NL;
VAN HET SCHIP, ALFRED DIRK, NL;
ZONNENBERG, BERNARD ANTONI, NL
(73) Propriétaires/Owners:
UNIVERSITAIR MEDISCH CENTRUM UTRECHT, NL;
UNIVERSITEIT UTRECHT HOLDING B.V., NL
(74) Agent: BORDEN LADNER GERVAIS LLP

(54) Titre : SUSPENSION DE BALAYAGE COMPRENANT UNE PARTICULE DONT LE DIAMETRE S'ELEVE A AU
MOINS 1 MICROMETRE
(54) Title: SCANNING SUSPENSION COMPRISING A PARTICLE WITH A DIAMETER OF AT LEAST 1 MICROMETER

(57) **Abrégé/Abstract:**

The invention provides a scanning suspension comprising a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of at least 1 μm , and use thereof for obtaining a scanning image. Preferably, said particle comprises holmium and a composition capable of essentially maintaining its structure during irradiation. A particle of the invention is suitable for preparing a kit of parts, comprising a diagnostic and a therapeutic composition which both comprise particles of the invention with essentially the same chemical structure, wherein said therapeutic composition is more radioactive than said diagnostic composition. Said kit of parts is especially suitable for treatment of a tumour. Firstly, the distribution of a particle of the invention within an individual can be determined with a scanning image obtained with said scanning composition. Subsequently, a radioactive therapeutic composition can be administered, wherein a suitable dose of said therapeutic composition is derived from said scanning image.



(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
15 January 2004 (15.01.2004)

PCT

(10) International Publication Number
WO 2004/004786 A1

(51) International Patent Classification⁷: **A61K 49/18,**
A61P 35/00

(74) Agent: **PRINS, A.W.;** Nieuwe Parklaan 97, NL-2587 BN
Den Haag (NL).

(21) International Application Number:
PCT/NL2003/000485

(81) Designated States (*national*): AE, AG, AL, AM, AT (utility model), AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ (utility model), CZ, DE (utility model), DE, DK (utility model), DK, DM, DZ, EC, EE (utility model), EE, ES, FI (utility model), FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK (utility model), SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(22) International Filing Date: 2 July 2003 (02.07.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
02077626.6 2 July 2002 (02.07.2002) EP

(71) Applicants (*for all designated States except US*): **UNIVERSITAIR MEDISCH CENTRUM UTRECHT** [NL/NL]; Heidelberglaan 100, NL-3584 CX Utrecht (NL). **UNIVERSITEIT UTRECHT HOLDING B.V.** [NL/NL]; Jenalaan 18a, NL-3584 CK Utrecht (NL).

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(72) Inventors; and

(75) Inventors/Applicants (*for US only*): **NIJSEN, Johannes, Franciscus, Wilhelmus** [NL/NL]; Stauntonstraat 28, NL-3554 EX Utrecht (NL). **VAN HET SCHIP, Alfred, Dirk** [NL/NL]; Pauwoogweide 39, NL-3437 VW Nieuwegein (NL). **ZONNENBERG, Bernard, Antoni** [NL/NL]; Fazantenkamp 464, NL-3607 DA Maarssen (NL).

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: SCANNING SUSPENSION COMPRISING A PARTICLE WITH A DIAMETER OF AT LEAST 1 MICROMETER

(57) Abstract: The invention provides a scanning suspension comprising a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of at least 1 μm , and use thereof for obtaining a scanning image. Preferably, said particle comprises holmium and a composition capable of essentially maintaining its structure during irradiation. A particle of the invention is suitable for preparing a kit of parts, comprising a diagnostic and a therapeutic composition which both comprise particles of the invention with essentially the same chemical structure, wherein said therapeutic composition is more radioactive than said diagnostic composition. Said kit of parts is especially suitable for treatment of a tumour. Firstly, the distribution of a particle of the invention within an individual can be determined with a scanning image obtained with said scanning composition. Subsequently, a radioactive therapeutic composition can be administered, wherein a suitable dose of said therapeutic composition is derived from said scanning image.

WO 2004/004786 A1

Title: SCANNING SUSPENSION COMPRISING A PARTICLE WITH A DIAMETER OF AT LEAST 1 MICROMETER

The invention relates to the field of medicine. More specifically, the invention relates to the field of diagnostics and radiotherapy.

Reliable, detailed diagnostics is often a key prerequisite for efficient treatment of a disorder. Especially disorders which display a significant
5 different pattern in each individual patient involve the need for very careful and accurate diagnosis. Such disorders for instance comprise tumour-related diseases. If a patient has been found to suffer from a tumour, it is important to obtain reliable insight into the status of the disease. For instance the growth and position of the tumour should be established, and it should be determined
10 whether there are metastases in other parts of the body, etc. Additionally, adequate information about targeting of a drug to a tumour can increase a treatment efficacy.

Many scanning techniques are known, such as magnetic resonance imaging (MRI) which provide information of the internal status of an
15 individual. A contrast agent is often used in order to be capable of obtaining a scanning image. For instance ferrite particles and gadolinium-DTPA (diethylaminetriaminepentaacetic acid) complexes are often used in contrast agents for MR scanning. This way, a good impression can be obtained of internal disorders, like the presence of (a) tumour(s).

20 After diagnosis, a treatment is often started involving administration of a pharmaceutical composition to a patient. It is often important to monitor the status of a patient during treatment as well. For instance the course of a treatment and targeting of a drug can be monitored, as well as possible side effects which may imply a need for terminating, or temporarily interrupting, a
25 certain treatment.

Sometimes local treatment in only a specific part of the body is preferred. For instance, tumour growth can sometimes be counteracted by internal radiotherapy comprising administration of radioactive particles to an

individual. If said radioactive particles accumulate inside and/or around the tumour, specific local treatment is possible. However, to prevent radiation-induced gastritis and/or radiation pneumonitis, especially in case of liver tumours, patients with significant shunting to the gastroduodenum and the lungs must be excluded from therapy. Therefore, the exact distribution of the radioactive particles is determined by firstly administering a tracer dose comprising said radioactive particles. This involves extra exposure of radioactivity, both for the patient and the medical staff, which is unwanted. Furthermore, some kind of radioactive particles, such as radioactive yttrium, can hardly be detected with a gamma camera. If such yttrium particles are to be used for therapy, other radioactive particles (for example: technetium labelled albumin particles) which can be detected with a gamma camera and which are expected to target and distribute approximately similar as said yttrium particles are administered before treatment. A distribution of said other radioactive particles is then determined. Because said distribution of said other radioactive particles is considered to be approximately similar to a distribution of yttrium, it can approximately be estimated whether significant shunting of yttrium to the gastroduodenum and/or the lungs will occur.

It is thus very complicated to determine how such particles should be used, and what the distribution pattern will be. These problems cannot be solved with current non-radioactive scanning techniques, for instance because the distribution of MRI contrast agents is not the same as the distribution of radioactive therapeutic compounds.

After the radioactive therapeutic compound has become non- (or barely) radioactive, its distribution cannot be followed anymore. This is inconvenient, because it would be desirable to monitor how said compound is removed from the body. Information about the biodistribution of said compound gives an indication about the course of a disease and/or treatment, and about the status of a patient.

It is an object of the present invention to provide an alternative scanning suspension. A scanning suspension of the invention can be used for existing applications. New applications with a suspension of the invention are also herewith provided.

5 The invention provides a scanning suspension comprising a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of at least 1 μm . Said particle can be detected by a non-radioactive scanning method such as MRI. Preferably said scanning suspension comprises an MRI scanning suspension. More preferably, said
10 particle comprises holmium.

A use of a particle which is capable of at least in part disturbing a magnetic field for the preparation of a scanning suspension, wherein said particle comprises a diameter of at least 1 μm is also herewith provided. Methods to generate a scanning suspension, such as an MRI scanning
15 suspension, are known in the art and need no further description here. With a scanning suspension of the invention a scanning image can be obtained. Thus, the invention provides a use of a scanning suspension comprising a particle which is capable of at least in part disturbing a magnetic field for obtaining a scanning image, wherein said particle comprises a diameter of at least 1 μm .
20 Preferably said scanning image comprises an MR scanning image. In this application the meaning of the word suspension has to be understood as at least including dispersions.

A scanning suspension of the invention is suitable for determining a flowing behaviour of a particle. Since a scanning suspension of the invention
25 comprises a particle of at least 1 μm , it can simulate the flowing pattern of such relatively large particles. A use of a scanning suspension comprising a particle with a diameter of at least 1 μm which is capable of at least in part disturbing a magnetic field for determining the flowing behaviour of said particle is therefore also herewith provided.

A scanning suspension of the invention, comprising a particle with a diameter of at least 1 μm which is capable of at least in part disturbing a magnetic field, is also very suitable for detecting a site of angiogenesis. A site of angiogenesis can be detected by determining the flowing behaviour of said particle.

- 5 Preferably said particle comprises holmium. The size of said particle can be chosen such to enable said particle to get stuck in a blood vessel. Typically said size comprises a diameter of about 3-5 μm . A site of angiogenesis can be detected after administration of said particles to an individual. At a site with many (developing) blood vessels, the concentration of stuck particles will be
- 10 high compared to other parts of the body. Detection of said site is thus possible, for instance by MRI scanning. One embodiment of the invention therefore provides a use of the invention for detecting a site of angiogenesis.

- A scanning suspension of the invention is also very suitable for detecting a tumour. This can for instance be performed by determining the flowing
- 15 behaviour of a particle of the invention, and/or by detecting a site of angiogenesis, with a use according to the invention. A presence of a tumour often involves a site of angiogenesis, because a tumour often needs much oxygen and nutrients for a high metabolism rate. Therefore new blood vessels are generated around said tumour. Hence, a site of angiogenesis can be
- 20 indicative for a presence of a tumour. Said tumour can be detected without the need of using radioactive material. Alternatively, particles with low radioactivity can be used. After a tumour has been detected, said tumour can be treated with a therapeutic composition comprising the same kind of particles as said scanning suspension. In said therapeutic composition,
- 25 however, said particles are preferably rendered (more) radioactive. Despite the difference in radioactivity, the particles of said diagnostic composition and the particles of said therapeutic composition are chemically the same. Therefore, the distribution of the radioactive particles of said therapeutic composition can be adequately predicted by determining the distribution of the particles of a
- 30 scanning suspension of the invention. The size of the particles are preferably

sufficiently large to avoid an equal distribution throughout the whole body. In one embodiment said therapeutic composition comprises a particle of the invention which is provided with at least one therapeutically active compound, for instance capable of treating a tumour.

5 The invention therefore provides a use of the invention for detecting a tumour. Preferably, said tumour comprises a liver metastasis.

In a preferred embodiment a use of the invention is provided wherein said scanning suspension comprises an MRI scanning suspension.

10 In yet another preferred embodiment a use of the invention is provided wherein said particle comprises a diameter sufficiently large to enable said particle to be stuck within a tumour. Such particle is very suitable for detecting a tumour. More preferably, said particle is at least in part capable of flowing through non-tumorous vessels. Such particle can stick in a tumour vessel while less sticking in normal vessels. This is possible because of the fact
15 that tumour vessels are mostly somewhat smaller and more irregularly formed than normal vessels. This way, tumour tissue can be very adequately distinguished from normal tissue, because a higher concentration of particles of the invention will be present in tumour tissue. Said particle of the invention preferably comprises a diameter of approximately 1-10 μm . More preferably,
20 such particle comprises a diameter of about 2-8 μm , most preferably about 3-5 μm .

 To distinguish tumorous from non-tumorous tissue, it is preferred to firstly administer a scanning suspension of the invention comprising particles, which are capable of at least in part disturbing a magnetic field, with a small
25 diameter, for instance about 3 μm . Then it can be determined whether those particles stick within tumorous vessels. If they do not stick within said tumorous vessels yet (the size of tumorous vessels will vary to some extent) one can administer a second dose of scanning suspension comprising particles of the invention with a somewhat larger diameter, for instance about 4 μm . If
30 these particles still do not stick within said tumorous vessels, a scanning

suspension comprising particles of the invention with an even larger diameter can be administered, etc. This way the minimal diameter can be determined allowing a particle of the invention to stick within a certain tumour while still being capable of flowing through non-tumorous vessels. Said minimal diameter
5 can vary between different tumours, and between different patients. Said minimal diameter is often between 3-5 μm . This way it is possible to detect a tumour with a scanning suspension of the invention comprising particles of the invention which stick within tumorous vessels while still being capable of flowing through non-tumorous vessels.

10 In one aspect the invention provides a method for detecting a tumour, comprising

- administering to an individual a scanning suspension comprising a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of at least 1 μm ;
- 15 - obtaining a scanning image; and
- determining whether said image reveals the presence of a tumour.

Preferably, said particle comprises a diameter of approximately 3-5 μm . As outlined above, a method of the invention can comprise administering to an individual different scanning suspensions, comprising particles of the
20 invention with different size. Preferably, each different scanning suspension is administered separately, with a time interval between administration of each suspension. Alternatively, different scanning suspensions can be administered simultaneously, or shortly after one another.

In another preferred embodiment, a particle of the invention comprises a
25 diameter of approximately 10-200 μm or 15-200 μm , more specifically 15-100 μm , even more specifically 20-100 μm , more preferably 20 to 50 or 80-100 μm . A particle of this size is very suitable for radiotherapeutic purposes. Said particle comprises a diameter sufficiently large to enable said particle to be lodged within arterioles. Hence, said particle is suitable for embolizing a blood vessel, preferably embolizing
30 an arteriole. A tumour can be deprived from blood, and

therefore be deprived from oxygen and nutrients, by lodging at least one blood vessel near said tumour with a particle of the invention. This is possible because of the fact that a tumour receives an increased blood flow as compared to normal tissue. Therefore an increased amount of particles of the invention will lodge in and around a tumour as compared to normal tissue. For instance, tumours in the liver receive their blood for the greater part from the hepatic artery while normal liver tissue receives its blood mainly from the portal vein. This results in an increased amount of particles of the invention in and around the tumour after administration of said particles in the hepatic artery. Said particles can for instance be administered to the hepatic artery with a catheter. Embolizing a blood vessel with a particle of the invention is also particularly suitable for treating a tumour present in the throat and/or head of an individual. The invention thus provides a use of a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of approximately 20-100 μm , for embolizing a blood vessel. In using relatively large particles, for example between 50-200 μm , embolisation of tumours, for example bone cancer and tumours due to Tuber Sclerosis, is possible. This latter disease results in very large benign kidney tumours which are very painful and may lead to rupture of blood vessels and death of a patient. Using particles of said size according to the invention embolisation of the vessels leading to said tumour may lead to retardation of tumour growth and prevent excessive exposure to radiation for patients and staff.

In yet another embodiment, a particle of the invention is administered to a particle or complex of interest. Preferably said particle or complex of interest comprises a particle or complex with a desired function which it can perform within an organism. More preferably, said particle or complex of interest comprises an organelle or cell of an organism. Most preferably, said particle or complex of interest comprises a liposome or a white blood cell. After administration of a particle of the invention to a particle or complex of interest, said particle or complex of interest can be detected by a scanning method such

as MRI. This way a presence and/or migration of said particle or complex of interest can be detected. For instance, a liposome is useful for delivering a nucleic acid of interest to a suitable site for gene therapy. If such liposome has been provided with a particle of the invention it can be determined where said
5 liposome is present inside an organism. It can then be estimated whether a nucleic acid of interest is delivered to a desired site. As another example, after administration of a particle of the invention to a white blood cell, migration of said white blood cell to a site of inflammation, or to a tumour, can be detected using a scanning method such as MRI. The invention thus provides a use of a
10 particle of the invention for detecting a presence and/or migration of a particle or complex of interest.

In one embodiment, a suspension comprising a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of at least 1 μm is used for the preparation of a kit of parts. Said
15 suspension can be used as such as a diagnostic composition. Alternatively, said suspension can be used for the preparation of a diagnostic composition. Preferably said suspension is essentially non-radioactive. Another aliquot of said suspension can be made (more) radioactive. Said other aliquot is very useful for radiotherapy. Such radioactive suspension of the invention can thus
20 be used as a therapeutic composition. Additionally, a composition comprising such radioactive suspension of the invention can be used as a therapeutic composition. In one embodiment a radioactive therapeutic composition of the invention comprises a particle of the invention which is provided with at least one therapeutically active compound, for instance capable of treating a
25 tumour. Said therapeutic composition is for instance capable of treating a tumour simultaneously by radiotherapy and with a therapeutic action of said compound. In an alternative embodiment a non-radioactive therapeutic composition of the invention comprises a particle of the invention which is provided with at least one therapeutically active compound, for instance
30 capable of treating a tumour. Said therapeutic composition is capable of

treating a tumour by a therapeutic action of said compound. Of course, a particle of the invention can be provided with any therapeutic compound. Such particle is suitable for treatment of any disease against which said therapeutic compound can perform its therapeutic action.

5 Said diagnostic composition and said therapeutic composition are suitable for the preparation of a kit of parts. A use of a particle of the invention for the preparation of a kit of parts is therefore also herewith provided.

 The invention provides a kit of parts comprising a diagnostic composition and a therapeutic composition, said diagnostic composition and
10 said therapeutic composition comprising particles of the invention with essentially the same chemical structure, said therapeutic composition being more radioactive than said diagnostic composition. Preferably, said diagnostic composition is essentially non-radioactive. In one embodiment, said particles comprise holmium. Said diagnostic composition can be used to determine a
15 distribution of said particles inside an individual. This can for instance be determined by MRI. Hence, there is now no more need for a radioactive tracer dose. This is both beneficial for the patient and for the medical staff. No special precautionary measures have to be taken against (too much) exposure to radioactive radiation. Moreover, if a radioactive tracer dose is used, a
20 distribution pattern has to be determined within limited time, before radioactivity has decayed. However, if a diagnostic composition of the invention is essentially non-radioactive, a distribution pattern of said particles does not have to be determined within limited time. Said distribution can now be determined during the whole time that said particles are present within an
25 individual. Hence, more time is available now for determining a distribution pattern.

 Subsequently, it can be decided whether said individual is capable of undergoing radioactive therapy with said therapeutic composition. This is for instance dependent on the degree of shunting of said particles to the lungs and
30 the gastrointestinal tract. Also, the optimal amount of radioactive therapeutic

composition to be administered to said individual can be determined, by interpretation of the obtained distribution pattern of said diagnostic composition. It can be determined how many particles accumulate in a tumour, if they are distributed inside said tumour, etc. Because said (more radioactive) particles of said therapeutic composition are chemically the same as said particles of said diagnostic composition, the distribution of said therapeutic composition will be the same as the distribution of said diagnostic composition in said individual.

10 Hence, in a preferred embodiment, a therapeutic composition of the invention is provided comprising a radioactive particle of the invention. Said particle of the invention can be directly generated using a radioactive component, such as radioactive holmium. Preferably however, a non-radioactive particle of the invention is firstly generated, followed by irradiation
15 of said particle. This avoids the use of high doses of radioactive components, the need for specially equipped (expensive) facilities, etcetera. For instance, after a scanning image has been obtained with a diagnostic composition of the invention, the optimal dosage of a particle of the invention for radiotherapy can be estimated. Such dose of non-radioactive particles of the invention can be
20 provided. Said particles can subsequently be irradiated. The present inventors used the high neutron flux facilities in Petten, The Netherlands. Irradiation (neutron flux $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$) took place for at least 0.5 hour, preferably about 1 hour. Of course, other facilities and other irradiation times can be used as well, provided that the particles of the invention essentially maintain their
25 structure during irradiation. With the term "essentially maintaining their structure" is meant herein that said particles maintain at least 50 %, more preferably 75 %, more preferably 90 %, most preferably 95 % of their content, shape, and/or density. Preferably, a scanning suspension of the invention is provided, wherein said particle comprises a composition capable of essentially
30 maintaining its structure during irradiation for at least 0.5 hour with a

neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$. More preferably, said composition is capable of essentially maintaining its structure during irradiation for about 0.5-2 hours with a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$. Most preferably, said composition is capable of essentially maintaining its structure during irradiation for about 1
5 hour with a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$.

In another preferred embodiment, said composition essentially does not comprise water, either bound and/or unbound, since the presence of water has appeared to have a destructive effect during irradiation.

In yet another preferred embodiment, said particle is biodegradable,
10 allowing for degradation in an animal body after it has been used, for instance for MRI and/or (radio)therapy.

In one embodiment a kit of parts is provided wherein said diagnostic composition comprises a suspension of the invention.

15 In yet another embodiment a kit of parts is provided comprising a diagnostic composition and a therapeutic composition, said diagnostic composition and said therapeutic composition comprising particles with essentially the same chemical structure which are capable of at least in part disturbing a magnetic field, wherein said particles comprise a diameter of at
20 least $1 \mu\text{m}$, wherein said therapeutic composition comprises a particle of the invention which is provided with at least one therapeutically active compound. The distribution of said therapeutic composition can be followed over time using a scanning method such as MRI. In one embodiment said therapeutic composition is essentially non-radioactive.

25 In one embodiment, a particle of the invention comprises a microsphere. Preferably, said microsphere comprises holmium. In another preferred embodiment, said particle comprises poly(L)-lactic acid. As shown in reference [14], poly(L)-lactic acid microspheres are capable of essentially maintaining their structure during irradiation for at least about 1 hour with a neutron flux of 5×10^{13}
30 $\text{cm}^{-2} \cdot \text{s}^{-1}$.

A particle of the invention comprising holmium preferably releases less than 10%, more preferably less than 5%, most preferably less than 1% holmium after and/or during irradiation, because released holmium results in a scanning image that may not be completely indicative for the distribution of said particles of the invention. Moreover, released radioactive holmium might harm (parts of) tissues which said particles are unable to reach. In yet another preferred embodiment, a scanning suspension of the invention is provided, wherein said composition comprises holmium chemically bound to a compound capable of essentially maintaining its structure during irradiation for 1 hour with a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$. Chemical linkage of holmium is favourable for at least in part avoiding holmium release. Irradiated holmium-loaded poly-(L)-lactic acid microspheres are capable of retaining >99.3% of ^{166}Ho activity after incubation for 288 h, 37°C, in PBS and pig liver homogenate [14]. Holmium is chemically linked to said microspheres [34]. A particle of the invention, a scanning suspension of the invention, and/or a kit of parts of the invention therefore preferably comprises said microspheres.

In one embodiment, biodegradable poly (L-lactic acid) microspheres (PLLA-MS) were manufactured in a glass beaker with four baffles, Holmiumacetylacetonate (Ho-AcAc) complex (10 g) and PLLA (6 g) were added to continuously stirred 186 g chloroform. PVA (20 gram) was dissolved in 1000 gram continuously stirred water of 40°C and poured into the glass beaker after cooling. The solutions and the beaker were kept at 25°C. The chloroform solution was added to the PVA solution and continuously stirred (500 rpm) until the chloroform was completely evaporated. To remove residual PVA and unincorporated Ho-AcAc, the formed microspheres were washed sequentially with water, 0.1 N HCl and water. The microspheres were graded and collected according to size on stainless steel sieves of 20 and 50 micrometer (20 micrometer sieve, S/Steel, NEN 2560, Endecotts, London; 50 micrometer sieve, S/Steel, ASIM E 11-87; B.V. metaalgaasweverij, Twente, The Netherlands) under sprinkled water, and dried under nitrogen. Characterisation of non-

irradiated and irradiated microspheres was carried out by scanning electron microscopy (SEM), laser particle size analysis and gamma-spectrometry of ^{166}Ho , after neutron activation of the ^{165}Ho incorporated in the PLLA-MS. For determination of PLLA molecular weight, microspheres were dissolved in
5 chloroform and analysed by high-performance liquid chromatography (HPLC) using a gel permeation chromatography column (Shodex™KD 800) from Showa Benco, Japan. Samples were irradiated individually and within 1 day, in order to create reactor conditions as closely comparable as possible. It appeared that well-defined irradiation conditions were necessary to produce therapeutic
10 dosages of ^{166}Ho -PLLA-MS while maintaining their integrity and suitability for therapy. Non-irradiated ^{165}Ho -PLLA-MS show a smooth, spherical appearance. After irradiation in the PRS facility (neutron flux $5 \times 10^{13} \text{cm}^{-2} \cdot \text{s}^{-1}$) for 1 h in polyethylene vials, minor surface changes were seen with SEM, giving rise to small PLLA fragments. These led to a larger number of particles,
15 <20 micrometer. While overall structural integrity was maintained in terms of form and size, the microspheres showed a minimal tendency towards aggregation; they could, however, be easily suspended in PBS and should be suitable for intra-arterial therapy.

The present inventor has developed holmium loaded poly(L-lactic acid)
20 microspheres (also called herein "holmium microspheres"), which can be detected by MRI. These microspheres can be used to generate an essentially non-radioactive diagnostic composition. With this diagnostic composition, the flowing behaviour of a particle of the invention, a site of angiogenesis, the presence of one or more tumours, and/or the distribution of said composition
25 inside and around a tumour can for instance be determined. Additionally, it can be estimated whether significant shunting to the gastroduodenum and the lungs occurs. In one aspect the invention thus provides a use of a particle of the invention for the preparation of a diagnostic composition.

Once the distribution of said composition inside a patient is known, another
30 sample of holmium loaded poly(L-lactic acid) microspheres can be rendered

radioactive, for instance by neutron activation. These radioactive holmium microspheres can be used to generate a therapeutic composition. The distribution of said therapeutic composition inside said patient will be the same as the distribution of said diagnostic non- (or low-) radioactive composition, because said microspheres are chemically the same. Thus, from the acquired (MRI-)information about the distribution of the diagnostic composition the optimal amount of therapeutic composition can be determined. Alternatively, the administered essentially non-radioactive microsphere can be made radioactive *in vivo*. This can for instance be done by neutron activation.

However, it is possible that the administered amount of diagnostic composition appears not to be the optimal amount for the patient involved, since different patients can display different distribution patterns. Therefore, preferably an optimal amount of a radioactive therapeutic composition is administered after the distribution of said non-radioactive diagnostic composition is determined.

It is also possible, in intervention MRI, to follow the administration and dosing of microspheres according to the present invention.

In terms of the invention, an individual means an animal, preferably a human.

By a particle of the invention is meant herein a particle which is capable of at least in part disturbing a magnetic field, wherein said particle comprises a diameter of at least 1 μm . Preferably said particle is paramagnetic, for instance comprising holmium, gadolinium and/or dysprosium. A particle of the invention has a different susceptibility to a magnetic field as compared to the environment. A particle of the invention for instance comprises a molecule bound to an element capable of at least in part disturbing a magnetic field. Said molecule may form a cage wherein said element is present. For instance, said particle comprises a microsphere. However, any particle comprising said element falls within the scope of a particle of the invention. A particle only containing said element also falls within the scope of a particle of the

invention. Preferably said element comprises holmium. By a suspension of the invention is meant a suspension comprising a particle of the invention.

By a composition or a particle which is more radioactive than another composition or particle is meant that the amount of radioactivity per mole is
5 higher. This amount of radioactivity is normally expressed in becquerel. By essentially non-radioactive is meant that the radioactivity is essentially the same as the normal background values generally present.

In terms of the invention, chemically the same means that the chemical formula is essentially the same, or that a particle comprises an essentially
10 similar shape while comprising essentially the same kind of sub-particle(s). Such sub-particle for instance comprises a particle of the invention. However, elements or compounds which are chemically the same may comprise different isotopes. A certain isotope of an element is considered to have essentially the same chemical properties compared to another isotope of the same compound.

15 By the expression "a particle with a diameter of 1 μm " is meant that a batch of said particles comprises particles with a mean value of approximately 1 μm . For instance, if said batch comprises microspheres, the size of each individual microsphere can vary between approximately 0.5 and 2 μm . The same applies for other diameter sizes described in this application.

20 By "treating a tumour" is meant herein that said tumour is counteracted. This can result in decreased growth of said tumour. In some cases growth can be stopped. Said tumour may be killed, although this is not necessarily the case.

The invention further provides a method for treating an individual
25 suffering from a tumour, comprising:

- administering to said individual a scanning suspension comprising a particle which is capable of at least in part disturbing a magnetic field;
- obtaining a scanning image of said individual;
- determining the distribution of said particle within said individual;
- 30 - administering to said individual a therapeutic composition comprising said

particle. Said particle in said therapeutic composition is more radioactive than said particle in said diagnostic composition, and/or is provided with at least one therapeutically active compound.

Preferably, said particle comprises holmium. More preferably, said
5 particle comprises a diameter of at least 1 μm . Most preferably, the optimal amount of said therapeutic composition is derived from the distribution of said particle of said scanning suspension. In one embodiment, said scanning suspension comprises a scanning suspension of the invention.

A method of the invention is particularly suitable for treatment of a
10 liver tumour, for instance a liver metastasis.

Liver metastases frequently occur during the progression of various solid tumours, especially colorectal cancers, and are the cause of 25–50% of all cancer deaths. The median survival of patients with liver metastases ranges from 2–12 months depending on volume of the metastases and histology of the
15 original tumour. Surgical resection is presently the only approach that offers patients with liver metastases substantial chance of cure. However this is an option for only 10-20 % of the patients.

External beam radiotherapy in the treatment of hepatic malignancies is limited by the tolerance of the hepatic parenchyma, which can tolerate doses of
20 only up to 30 Gy for whole liver irradiation; this treatment modality is therefore ineffective. With a method of the invention treatment of liver malignancies is improved.

A particularly useful mode of therapy is the use of intra-arterially injected radioactive particles of the invention of a size sufficient to lodge in
25 endarterioles. The basis for such therapy is that tumours are usually rich in vasculature and that liver metastases are almost exclusively dependent on arterial blood supply. This contrasts with normal liver, which receives most of its flow from the portal vein. This selectivity can also be increased by the use of vasoactive drugs, which cause vasoconstriction of the normal liver arterioles,
30 but to which tumour vessels, lacking smooth muscle, are insensitive. Of course,

other kind of tumours can also be treated by lodging of a blood vessel by a particle of the invention.

In another aspect the invention provides a use of a particle which is
5 capable of at least in part disturbing a magnetic field as a medicament,
wherein the dosage of said particle has been derived from a scanning image
obtained with particles with essentially the same chemical structure.
Preferably, said medicament is capable of, at least in part, treating a tumour,
more preferably a liver metastasis. A use of a particle which is capable of at
10 least in part disturbing a magnetic field for the preparation of a medicament
for the treatment of a tumour, wherein the dosage of said particle has been
derived from a scanning image obtained with particles with essentially the
same chemical structure, is therefore also herewith provided. Preferably, said
particle comprises a diameter of at least 1 μm , more preferably about 3-5 μm ,
15 enabling said particle to get stuck in a blood vessel. Since a particle of the
invention is preferably used for obtaining a scanning image as well as for
radiotherapy, a method or use of the invention is preferably provided wherein
said particle comprises a composition capable of essentially maintaining its
structure during irradiation for at least 0.5 hour, preferably about 1 hour, with
20 a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$. More preferably said particle comprises a
microsphere, most preferably a poly(L-lactic acid) microsphere. In yet another
preferred embodiment said composition comprises holmium chemically bound
to a compound capable of essentially maintaining its structure during
irradiation for 1 hour with a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$. As explained
25 above, chemical linkage improves stability of said particle and at least partly
avoids release of holmium from said particle.

The invention furthermore provides a method for preparing a
therapeutic composition for treatment of a tumour, comprising the steps of:
30 - in a first step obtaining a scanning image, more specifically an MRI

image of a person provided with a scanning suspension of the invention;

in a second step preparing a therapeutic suspension for treatment of a tumour, using particles with essentially the same chemical structure as said particles in said scanning suspension, which particles are made more
5 radioactive than said particles in said scanning suspension.

In one embodiment an amount of particles is prepared prior to obtaining said scanning image, wherein a first part of said amount of particles is used for preparing said scanning suspension and a second part of said amount of particles is used for preparing said therapeutic suspension. Using the same
10 source of particles of the invention for both said scanning suspension and said therapeutic suspension is favourable, especially when the dosage of said particles in said therapeutic suspension is derived from the scanning image obtained, because variables in distribution patterns of different batches of particles is avoided.

15 In yet another embodiment a method for preparing a therapeutic composition is provided, wherein a dose of radiation for rendering said particles for use in said therapeutic suspension radioactive, and/or the amount of particles to be used in said therapeutic suspension, is at least partly based on said scanning image obtained.

20

In one embodiment, a method of the invention is provided wherein said particle comprises a microsphere, for instance a poly(L-lactic acid) microsphere.

Preferably, said particle comprises holmium.

25 For example, neutron activated radioactive holmium loaded poly(L-lactic acid) microspheres (Ho-PLLA-MS) emit gamma rays which can be used for imaging with a gamma-camera and beta particles for treatment of a patient. Animal studies showed that these microspheres can be targeted to the tumour and that they can be easily imaged with a gamma camera. Since holmium is
30 paramagnetic it can also be viewed by non-radioactive scanning methods such

as MRI. It is therefore possible to image non-radioactive holmium loaded microspheres. Imaging of non-radioactive holmium loaded microspheres before treatment with radioactive microspheres results in a radiation reduction for the patient and medical personnel. In that case no special precautionary
5 measures have to be taken against (too much) exposure to ionizing radiation, as has been explained above. Moreover, more time is now available for determining a distribution pattern. Said distribution can now be determined during the whole time that said particles are present within an individual, whereas a radioactive tracer dose should be detected before radioactivity has
10 decayed.

Furthermore, the distribution of holmium loaded microspheres can be also followed over time.

In yet another embodiment the invention provides a method for obtaining a scanning image, comprising administering a scanning suspension
15 to an individual and subsequently generating a scanning image of said individual, wherein said scanning suspension comprises a scanning suspension of the invention.

In one aspect, there is provided a kit of parts comprising a diagnostic composition; a therapeutic composition; and instructions for use in treating a
20 tumour, wherein said diagnostic composition and said therapeutic composition comprise particles with essentially the same chemical structure for at least in part disturbing a magnetic field, said therapeutic composition being more radioactive than said diagnostic composition, said particles having a diameter of at least 1 μm .

In another aspect, there is provided a use of a particle for at least in part
25 disturbing a magnetic field as a medicament, wherein the dosage of said particle is derived from a scanning image obtained with particles with essentially the same chemical structure, based on the distribution of said particles in said scanning image inside a patient, wherein said particle comprises holmium and has a diameter of between 20 and 100 μm , and wherein said particle is more
30 radioactive than said particles used for obtaining said scanning image.

19a

In another aspect, there is provided a use of a particle for at least in part disturbing a magnetic field for the preparation of a medicament for the treatment of a tumour, wherein the dosage of said particle is derived from a scanning image obtained with particles with essentially the same chemical structure, based on the distribution of said particles in said scanning image inside a patient, wherein said particle comprises holmium and has a diameter of between 20 and 100 μm , and wherein said particle is more radioactive than said particles used for obtaining said scanning image.

In another aspect, there is provided a method for preparing a therapeutic composition for treatment of a tumour, comprising the steps of: generating paramagnetic particles which are capable of at least in part disturbing a magnetic field, wherein said particles comprises a diameter of at least 1 μm ; rendering said paramagnetic particles radioactive; preparing a therapeutic composition for treatment of a tumour comprising an optimal therapeutic dosage of said paramagnetic particles, wherein said optimal dosage of said therapeutic composition is determined based on the distribution inside a patient of paramagnetic particles of a scanning suspension which are capable of at least in part disturbing a magnetic field and which have essentially the same chemical structure as said paramagnetic particles in said therapeutic composition, and wherein said paramagnetic particles of said therapeutic composition are more radioactive than said paramagnetic particles of said scanning suspension.

In one aspect, there is provided a kit of parts comprising a diagnostic composition; a therapeutic composition; and instructions for use in treating a tumour, wherein said diagnostic composition and said therapeutic composition comprise paramagnetic particles comprising holmium, gadolinium and/or dysprosium with essentially the same chemical structure for at least in part disturbing a magnetic field, said therapeutic composition being more radioactive than said diagnostic composition, said particles having a diameter of 1-200 μm .

In another aspect, there is provided use of a paramagnetic particle for at least in part disturbing a magnetic field as a medicament, wherein the dosage of said particle is derived from a scanning image obtained with particles with essentially the same chemical structure, based on the distribution of said particles

19b

in said scanning image inside a patient, wherein said particle comprises holmium, gadolinium and/or dysprosium and has a diameter of between 20 and 100 μm , and wherein said particle is more radioactive than said particles used for obtaining said scanning image.

5 In another aspect, there is provided use of a paramagnetic particle for at least in part disturbing a magnetic field for the preparation of a medicament for the treatment of a tumour, wherein the dosage of said particle is derived from a scanning image obtained with particles with essentially the same chemical structure, based on the distribution of said particles in said scanning image inside
10 a patient, wherein said particle comprises holmium, gadolinium and/or dysprosium and has a diameter of between 20 and 100 μm , and wherein said particle is more radioactive than said particles used for obtaining said scanning image.

In another aspect, there is provided a method for preparing a therapeutic
15 composition for treatment of a tumour, comprising the steps of: generating paramagnetic particles which are capable of at least in part disturbing a magnetic field, wherein said particles comprise holmium, gadolinium and/or dysprosium and have a diameter of 1-200 μm ; rendering said paramagnetic particles radioactive; preparing a therapeutic composition for treatment of a tumour
20 comprising an optimal therapeutic dosage of said paramagnetic particles, wherein said optimal dosage of said therapeutic composition is determined based on the distribution inside a patient of paramagnetic particles of a scanning suspension which are capable of at least in part disturbing a magnetic field and which have essentially the same chemical structure as said paramagnetic particles in said
25 therapeutic composition, and wherein said paramagnetic particles of said therapeutic composition are more radioactive than said paramagnetic particles of said scanning suspension.

In another aspect, there is provided a scanning suspension comprising paramagnetic particles for at least in part disturbing a magnetic field, wherein said
30 particles comprise holmium, gadolinium and/or dysprosium and have a diameter of 1-200 μm and have been irradiated for use in a method as described herein.

The following examples are meant to illustrate the present invention. They do not limit the scope of the invention in any way.

Examples

The purpose of this study was to investigate the possibility of measuring the biodistribution of holmium loaded microspheres with MRI. Measurements
5 were done in phantoms, in ex-vivo rabbit livers and in rabbits. MR images of the rabbits were compared with gamma scintigraphic images.

Methods and materials

10

Preparation of microspheres. Radioactive holmium loaded microspheres were prepared as previously described [14]. Briefly, holmium acetylacetonate [20] is incorporated into poly(L-lactic acid) by solvent evaporation, resulting in microspheres of 20-50 µm after sieving. Neutron activation of the microspheres
15 was performed by irradiation for 1h in the PRS facility of the high-flux nuclear reactor in Petten, The Netherlands. Prior to administration during the in-vivo and ex-vivo experiments the microspheres were sonicated for 10 min in an ultrasonic cleaner and suspended in Gelofusine® (Vifor Medical SA, Switzerland).

20

Phantoms. For preparation of the agar gel matrix dry agar powder (20g; Life technologies GIBCO BRL, Paisley, Scotland) was mixed in cold deionized water (1000g) with manganese(II) chloride tetrahydrate (900 mg; Merck, Darmstadt, Germany). The manganese-chloride was used to simulate liver
25 NMR properties. Holmium or yttrium loaded poly(L-lactic acid) microspheres (Ho-PLLA-MS or Y-PLLA-MS) were suspended in the agar solution under stirring. The microspheres suspension and agar suspension were heated till 100 °C for 10 minutes resulting in transparent fluid gels. The gels were added in different proportions to each other which resulted in a rising Ho-PLLA-MS
30 and Y-PLLA-MS concentration. The mixed gels were sonicated during cooling.

Once cooled to room temperature, the gel is optically transparent with visible homogeneously distributed microspheres.

In a perfusion phantom of the abdominal region, the detection of A-V shunting across the liver was examined. A tube with an inner diameter of 12 mm was
5 chosen as a scaled model of the human inferior vena cava, which has a diameter of around 24 mm. The tube was placed in a Plexiglas container, filled with manganese-doped water as a background, mimicking muscle tissue. An air-pressure-driven flow pump generating a constant flow of 17 ml/s was connected to the phantom, yielding a flow velocity of 15 cm/s, which is a
10 velocity expected for an average human vena cava. The circulating and background fluid consisted of water with manganese-chloride (19.2 mg/l $\text{MnCl}_2 \cdot 4\text{H}_2\text{O}$). The manganese solution was used to approximate the relaxation times of human blood. For detection of the passage of holmium-loaded microspheres, a holmium-sensitive dynamic sequence (as described in the MR
15 imaging section) was used. After acquisition of a base-line value, a short injection of microspheres was given via a 5F injection catheter, and this was subsequently flushed with approximately 4 ml of the blood mimicking fluid. The injected doses of microspheres ranged from 4.4 to 31 mg. The shunting experiment was also carried out for larger and slowly injected doses
20 (respectively 40, 48 and 53 mg).

Rabbits. All experiments were performed in agreement with The Netherlands Experiments on Animals Act (1977) and the European Convention guidelines
25 (86/609/EC). Approval was obtained from the University Animal Experiments Committee. The experiments were performed using four female pathogen-free New Zealand White inbred hsdIF rabbits of 3000-4000 g (Harlan, Horst, The Netherlands). The rabbits were housed individually in steel cages and provided daily with approximately 100 g "complete diet" pellets for rabbits.
30 Water was provided ad libitum. The three tumour bearing rabbits were

sacrificed after three or four weeks. The Rabbit without tumour was sacrificed direct after the SPECT and MRI images were taken.

Analgesia, sedation and euthanasia. Analgesia and sedation during
5 laparatomies were achieved with 0.5 ml methadone (10mg/ml; Veterinary Pharmacy, University of Utrecht, The Netherlands) and 0.5 ml Ventrtranquil[®] (acepromazine, 10 mg/ml; Sanofi Sante Animale Benelux BV, Maassluis, The Netherlands). Subsequently, the rabbits were anaesthetized by an intravenous
10 injection of Hypnomidate[®] (2mg/ml; B. Braun Melsungen AG, Melsungen, Germany) and N₂O and halothane (Albic BV, Maassluis, The Netherlands) as inhalation anasteticum. Rabbits were sacrificed with 3 ml Euthesate (pentobarbital, 200mg/ml; Apharmo b.v., Arnhem The Netherlands).

Tumour cells. The VX2 cell line [21] was obtained from the Department of Oral
15 and Maxillofacial Surgery of the University Medical Center, Utrecht, The Netherlands [22]. The VX2 tumour was propagated by subcutaneous passage in the hip region of the rabbit. After the tumour was dissected small parts (2 mm in diameter) were chosen for implantation.

20 *Tumour implantation.* Tumour parts (two or three) were injected in the left lateral lobe with an Abbocath[®] 18G (Abbocath Ltd., Ireland). The injection wound was sealed with tissue glue (Histoacryl, B. Braun Melsungen AG, Melsungen, Germany). After approximately 12 days the first ultrasound investigation (HDI 3000 ATL, Entos[™] CL10-5 transducer) was performed to
25 check tumour growth.

Administration of the microspheres. When the tumour had reached a diameter of ≥ 20 mm, a second laparotomy was performed in order to administer the holmium loaded microspheres. The gastroduodenal artery was cannulated
30 with an Abbocath[®] 24G (Abbott Ltd., Ireland). Back flow was checked with

0.1% methylene blue in 5% glucose. A pre-flushed administration system similar as described by Herba et al. [23] was connected to the Abbocath®. The suspended microspheres were administered and the syringe was measured for activity pre- and post injection, in order to calculate the injected dosage. The
5 gastroduodenal artery was ligated or if possible sealed with tissue glue (Histoacryl, B. Braun Melsungen AG, Melsungen, Germany). MR images were taken before, three days after and 17 days after administration of the radioactive microspheres. SPECT images were taken three days after administration. In order to verify presence of microspheres liver was embedded
10 in paraffin and histologically evaluated after staining with haematoxylin-eosin.

Ex-vivo liver. The liver was derived from a rabbit used in a terminal animal experiment. No extra rabbits were killed for performing these ex-vivo
15 experiments. A needle was jabbed in the left ventricle of the heart and the right auricle was cut away. The rabbit was flushed with saline and heparine; 500 ml with 1ml heparine (Leo Pharma BV, Weesp, 5000 IE /1ML). The liver was removed and the hepatic artery was cannulated with a Abbocath® 24 G. Again the liver was flushed with saline and heparine via the hepatic artery.
20 The livers were stored in saline by 5 °C during a maximum of 30 hours. The suspended microspheres were administered via the hepatic artery during the dynamic MR-imaging experiments.

Magnetic resonance imaging. All MR investigations were performed on a whole
25 body system operating at 1.5T (Gyrosan ACS-NT 15, Philips Medical Systems). The imaging protocol included T₁- weighted SE imaging and T₂-weighted SE imaging. Measurement of the relaxation properties of the holmium and yttrium microspheres for different concentrations was performed using a multi-echo spin echo (SE) measurement, combined with an inversion
30 recovery sequence. Longitudinal relaxation ($R_1=1/T_1$) and transversal

relaxation ($R2=1/T2$) rates were determined by least square fits of the obtained signals. The transversal relaxation rate ($R2^*=1/T2^*$) for gradient echo (FFE) imaging was determined using a multi-gradient echo sequence, acquiring 25 echoes with an echo spacing of 0.91 ms.

- 5 In order to detect injected boluses of microspheres, passing the modelled vena cava, a dynamic transversal $T2^*$ -weighted FFE (resolution 2 mm, slice 30 mm, echo-time (TE) 15 ms, 0.352 s/dynamic) was performed. The increase of transversal relaxation rate ($\Delta R2^*$) due to passing microspheres was calculated by means of observed signal change, relative to an acquired base-line value.
- 10 The imaging protocol for both ex vivo and in vivo MR measurements before and after administration of the holmium-loaded microspheres included anatomical $T1$ -weighted SE (TE 9.5 ms) imaging, tumour sensitive $T2$ -weighted SE imaging (TE 90 ms) and holmium-sensitive $T2^*$ -weighted FFE imaging (TE 4.6, 9.2 ms). For the ex vivo experiments, a dynamic $T2^*$ -
- 15 weighted FFE (resolution 2 mm, TE 9.2 ms, slice thickness 4 or 10 mm, 1 s per slice) sequence was also used to depict the administration of the microspheres.

Scintigraphic imaging. After administration of the radioactive microspheres imaging of the total rabbit and the abdominal region was performed using a

20 dual-head camera (Vertex-MCD, ADAC, Milpitas, CA). A planar and SPECT image was generated. SPECT acquisition involved a rotation of each detector of 180° with 32 stops at 30 s per stop.

Results

- 25 *Microspheres* Microspheres prepared by solvent evaporation resulted after sieving in 3-5 grams spherical particles with a diameter of 20-50 μm (Fig. 1) and a holmium content of 15-17% (w/w).

Phantoms R1 and R2 as measured by the multi spin-echo with inversion

30 recovery experiment were largely independent of the concentration of holmium

microspheres, Figure 2. The least squares fit suggests $\Delta R_2 = 1.93 \times [\text{HoMS}] \text{ s}^{-1}$,
[HoMS] in mg/g. This is to be expected for stationary paramagnetic perturbors
of this size, because the perturbing particles are large compared to the
diffusion length of the protons [24]. Figure 3 shows the R_2^* dependence on
5 HoMS concentration. The transverse relaxivity corresponds to that predicted
for the static dephasing regime [25], where the susceptibility of the HoMS is
calculated using the Curie law from the magnetic moment of uncoupled Ho
ions (10.4 Bohr magnetons) and the Ho content of the microspheres.
Detection of passing holmium-loaded microspheres in order to estimate lung
10 shunting in a scaled model of an average human vena cava showed the ability
of dynamic MRI to detect all injected single doses (Table 1), which is
illustrated in Figure 9 for a dose of 6.7 mg and 48 mg. The latter dose was
injected slowly to simulate shunting of microspheres over time. This figure
shows that after acquisition of a base-line value, a dose of a few mg is easily
15 detected. For all other injected doses, measured changes in relaxation rates
were linearly proportional to the amount of administrated microspheres.

Tumour implantation and administration of ^{166}Ho microspheres Implantation
20 of the tumour resulted in a 100% "take"-rate. After 16 days the tumours
reached a diameter of approximately 23 mm. The tumours were well
vascularized as was seen with ultrasound. Tumour size varied from 10 to 17
 cm^3 ($12.7 \pm 4.1 \text{ cm}^3$) in volume measured with a ruler (Fig. 4).
25 Approximately 6% of the activity was adhered in the administration system
after administration. An amount of 48-50 mg radioactive holmium
microspheres was effectively administrated to the liver with tumour
corresponding with 560-640 MBq of activity.

Biodistribution in liver tumour bearing rabbits On scintigraphic images radioactivity was especially seen in the tumour and the liver (Fig. 5). The activity in the liver was heterogeneously distributed. Increased accumulation of microspheres was seen in and around the tumour.

5

MRI of the rabbit before administration of holmium loaded microspheres resulted in an ideal diagnostic tool for the visualisation of the VX2-tumours (Fig. 6a). The tumours appear as an homogeneous, round sharply margined lesion. On T1-weighted images the tumours are hypointense and on T2-weighted images they appear as hyperintense lesions compared with liver tissue. After administration of holmium loaded microspheres field disturbances were seen in the tumour and in the liver caused by accumulation of holmium loaded microspheres (Fig. 6b-c). The T2-weighted image is more sensitive for holmium as is shown by the increased black areas in the liver and especially around the tumour. No holmium accumulation was seen in the nucleus of the tumour (Fig.6d).

The follow-up MR scans were obtained 17 days after administration of the microspheres. No progression was seen of the tumour. No substantial redistribution of holmium loaded microspheres was seen. In two rabbits MR images showed that the right lateral lobe was increased to 2-4 times the original volume. In the right and left medial lobe and the left lateral lobe damage of the liver tissue was observed. These lobes showed large necrotic and yellow coloured areas caused by accumulation of bile. No apparent lesions were found in the stomach and duodenum. The tumour was totally necrotic. MR images were very helpful in identifying the accumulation of the holmium loaded microspheres and thus the tumour. Histology confirmed the accumulation in and around the necrotic tumour.

Ex-vivo liver Processing of the administration of the microspheres was done in three ex-vivo rabbit livers. The accumulation in the arteries was observed by using dynamic MR. First the smaller vessels till the brim of the liver were filled with microspheres (Fig. 8c 1-4). Thereafter accumulation of the
5 microspheres appeared in the larger blood vessels and the centre of the liver (Fig. 8c 4-8). During these experiments 0-100 mg microspheres were used. After image 5 in figure 8 almost no new vessels were embolised (at that moment approximately 40 mg microspheres were administered).

10

Discussion

In this study the feasibility of using MRI for imaging radioactive and non-radioactive holmium loaded microspheres was investigated. During *in-vivo* and *ex-vivo* experiments the biodistribution in the liver was examined, after intra-
15 arterial administration into the hepatic artery of rabbits with implanted VX2 tumours.

Phantom experiments with holmium loaded poly(L-lactic acid) microspheres suspended in agar show a susceptibility of the HoMS which can be described by the Curie law, indicating no magnetic interactions between the Ho-ions.
20 The magnetic susceptibility for Ho is comparable of that of Dy [17].

MR imaging is very useful to identify the anatomical structure of the abdominal region. The tumour is visible as a spherical tissue mass in the left lateral lobe. Sizes of the tumour measured with echo and with a ruler are comparable to the measurements with MRI. After administration of the
25 radioactive holmium loaded microspheres accumulation was seen in and especially around the tumour. This can be explained by the tumour angiogenesis of liver metastases. Liver tumours have often a hypervascular brim and derive their blood supply almost exclusively from the hepatic artery [32]. Microspheres injected into the hepatic artery therefore accumulate
30 around the tumour.

On both scintigraphic and MR images an inhomogeneous distribution of the holmium microspheres in the liver was observed. This heterogeneous distribution is described also for human patients and can explain the toleration of the liver for high doses of activity [32;33]. Large parts of the liver
5 will receive less activity than would be expected for a uniform distribution of activity resulting in survival of most of the liver tissue.

MR and scintigraphic images show both the holmium accumulation in the animal. However MRI combines this image with detailed information about the morphology of the animal which result in straightforward proof where in
10 the body holmium microspheres are accumulated. It is shown that quantitative MR of holmium microspheres in a target organ with tumour provides in easy and accurate dosimetric studies.

In the *ex-vivo* liver experiments the feasibility of real-time MR images during
15 administration was demonstrated. Clearly was observed that at a well-defined point no further vessels were provided of microspheres and that first the smaller vessels were filled-up with spheres. This shows that vascular tissue is limited in the capacity of gathering spheres and that administering of extra microspheres will only result in fill-up of the larger vessels. Generally, these
20 larger vessels are non-tumour vessels and therefore will not join in tumour treatment after accumulation of spheres. The possibility of real-time controlling and changing the administration position, flow and quantity of microspheres on the basis of the MR images will result in optimisation of therapeutic properties of radioactive holmium loaded microspheres.

25 Customizing a treatment for each individual patient effects in better treatment resulting in decrease of liver damage and increase of the tumour to liver ratio. Tumour to liver ratio is to be understood as the ratio between the activity of and/or the number of particles in the tumour relative to the activity of and/or the number of particles in the liver. A higher ratio is therefore more effective.

Follow-up of a patient is desirable for further research and clinical explanation of observed effects. Holmium microspheres can be imaged after treatment as long as they accumulate in the body. Information about redistribution and tissue reaction on such particles can be observed with MR. The animal
5 experiments in rabbits show that redistribution is not seen during the first 17 days.

In conclusion, this study has demonstrated that holmium loaded PLLA microspheres which can be used for internal radionuclide therapy can be imaged *in-vivo*. The possibility of imaging non-radioactive and radioactive
10 holmium loaded spheres with MR opens the way for accurate administration and follow-up of a treatment.

Table 1.

Comparison of detection of Ho-PLLA-MS with SPECT and MRI

	SPECT	MRI
Imaging therapeutic microspheres	+	+
Quantification of therapeutic microspheres	+	+
Radioactive trace dose to estimate lung-shunting	+	+
Non-radioactive trace dose to estimate lung-shunting	-	+
Direct anatomical reference	-	+
High resolution	-	+
Soft tissue contrast (tumours)	-	+
Long term post-treatment imaging	-	+
Highly selective administration	-	+
Possibility to interfere during administration	-	+

Brief description of the drawings

Figure 1a-b. a) Scanning electron micrograph of holmium loaded PLLA
5 microspheres. b) Volume weight distribution of sieved microspheres. The used
microspheres for the experiments had a mean diameter of 30 μm and 96% of
the volume of the particles had a diameter between 20 and 40 μm .

Figure 2a-b. a) R_1 and b) R_2 versus HoMS concentration. The solid line is a
10 least squares fit to the data points.

Figure 3. R_2^* versus HoMS concentration. The solid line represents the
theoretical result in the static dephasing regime (Eq. 11 in Ref. 25) as
calculated from the holmium content of the spheres.

15

Fig.4a-b. a) Picture of the tumour on the left lateral liver lobe. b) Liver
overview of the rabbit. In the left lateral liver lobe (I) the tumour is implanted
10 mm from the brim of the lobe (white dot). This liver lobe which is laying on
the stomach can be easily attained for implantation. Left medial lobe (II) and
20 right medial lobe (III) are partly fused to each other and are laying on the
stomach. The gall bladder is positioned on the back of the right medial lobe.
The right lateral lobe (IV) is laying next to the stomach close to the backbone
which is also seen on figure 6.

25 **Figure 5a-d.** MR and scintigraphic images of one of the tumour-bearing
rabbits. a) T1-weighted SE image after administration of the microspheres.
Field disturbances caused by holmium accumulation are seen as black areas.
b) T2-weighted FFE (TE=4.6 and 9.2 msec) image after administration of the
microspheres. Clearly is seen that the T2-weighted image is more sensitive for
30 holmium as is shown by the increased black areas. Increased accumulation of

holmium ~thus microspheres~ is indicated with small arrows. The larger arrow indicates the microspheres in and around the tumour. c) Schematic drawing of MR image "a" which shows the organs and tumour in the rabbit. d) Whole body scintigraphic image of the rabbit 3 days after injection of

5 radioactive microspheres (48 mg; 560 MBq) into the hepatic artery. The small scintigraphic image in the right upper corner shows the contours of the rabbit obtained by using a "flood source". Contour of the rabbit was obtained using the "flood source". Increased accumulation of radioactivity ~thus holmium loaded microspheres~ is indicated with small arrows. The larger arrow

10 indicates the activity in and around the tumour.

Figure 6a-d. Magnetic resonance images of the transverse plane of the rabbit. b) Schematic drawing shows the organs which are seen in the images. The colour and position of the organs corresponds with the small drawings in each

15 MRI image. a) Representative T1-weighted SE image before administration of the holmium loaded microspheres. c) T1-weighted SE image after administration of the microspheres. Field disturbances caused by holmium accumulation are seen as black areas indicated with small arrows. In and around the tumour indicated with the large arrow is an increased holmium

20 accumulation seen. d) T2-weighted FFE (TE=4.6 and 9.2 msec) image after administration of the microspheres.

Figure 7a-c. Magnetic resonance images of the tumour bearing rabbit liver 4 weeks after treatment. a) T1-weighted SE image. b) T2-weighted FFE image

25 with field disturbances caused by holmium accumulation. White arrow indicate the tumour side. c) Ex-vivo liver with tumour (black arrow). The right lateral lobe is increased while the other lobes and the tumour are growth to each other.

Figure 8a-c. Dynamic magnetic resonance images (c) of the administration of holmium loaded microspheres in an ex-vivo liver (without tumour) of a rabbit (a-b). The administration was mainly selective for the medial lobes. T2* weighted FFE images shows the flow of the microspheres in the normal liver.

- 5 Images 8c 1-3 (Dyn-T2* FFE, 4 mm thickness, time resolution= 5s/slice, TE=9.2) and images 8c 4-8 (Dyn-T2* FFE, 10 mm thickness, time resolution= 1s/slice, TE=9.2).

- Figure 9.** Detection of holmium-loaded microspheres passing a scaled model of a human vena cava. Dashed lines denote the base line values before injection of the boluses. For the small dose (5.5 mg), a rapid injection was given at point A, whereas the large dose was injected from points B to C. Point D is a rapid flushing of the injection catheter with the circulating fluid. The areas between the base-lines and the curves are proportional to the injected doses. a.u.:
- 10
15 arbitrary units.

References

- (14) Nijsen JFW, Zonnenberg BA, Woittiez JR, Rook DW, Swildens-van
5 Woudenberg IA, van Rijk PP, van het Schip AD. Holmium-166 poly lactic acid microspheres applicable for intra-arterial radionuclide therapy of hepatic malignancies: effects of preparation and neutron activation techniques. Eur J Nucl Med 1999; 26(7):699-704.
- (17) Fossheim S, Johansson C, Fahlvik AK, Grace D, Klaveness J.
10 Lanthanide-based susceptibility contrast agents: assessment of the magnetic properties. Magn Reson Med 1996; 35(2):201-206.
- (20) Kooijman H, Nijsen F, Spek AL, van het Schip F. Diaquatrakis(pentane-2,4-dionato-O,O')holmium(III) monohydrate and diaquatrakis(pentane-2,4-dionato-O,O')holmium(III) 4-hydroxypentan-2-one solvate dihydrate. Acta
15 Crystallogr C 2000; 56(Pt 2):156-158.
- (21) Kidd JG, Rous P. A transplantable rabbit carcinoma originating in a virus-induced papilloma and containing the virus in masked or altered form. J.Exp.Med. 71[469], 813-837. 1940.
- 20 (22) van Es RJ, Franssen O, Dullens HF, Bernsen MR, Bosman F, Hennink WE, Slootweg PJ. The VX2 carcinoma in the rabbit auricle as an experimental model for intra-arterial embolization of head and neck squamous cell carcinoma with dextran microspheres. Lab Anim 1999; 33(2):175-184.
- 25 (23) Herba MJ, Illescas FF, Thirlwell MP, Boos GJ, Rosenthal L, Atri M, Bret PM. Hepatic malignancies: improved treatment with intraarterial Y-90. Radiology 1988; 169(2):311-314.

- (24) Weisskoff RM, Zuo CS, Boxerman JL, Rosen BR. Microscopic susceptibility variation and transverse relaxation: theory and experiment. Magn Reson Med 1994; 31(6):601-610.
- (25) Yablonskiy DA, Haacke EM. Theory of NMR signal behavior in magnetically inhomogeneous tissues: the static dephasing regime. Magn Reson Med 1994; 32(6):749-763.
- (32) Fox RA, Klemp PF, Egan G, Mina LL, Burton MA, Gray BN. Dose distribution following selective internal radiation therapy. Int J Radiat Oncol Biol Phys 1991; 21(2):463-467.
- (33) Yorke ED, Jackson A, Fox RA, Wessels BW, Gray BN. Can current models explain the lack of liver complications in Y-90 microsphere therapy? Clin Cancer Res 1999; 5(10 Suppl):3024s-3030s.
- (34) Nijssen JFW, Van Steenbergen MJ, Kooijman H, Talsma H, Kroon-Batenburg LMJ, Van de Weert M, Van Rijk PP, De Witte A, Van het Schip AD, Hennink WE. Characterization of poly(L-lactic acid) microspheres loaded with holmium acetylacetonate. Biomaterials 22 (2001): 3073-3081

CLAIMS:

1. A method for preparing a therapeutic composition for treatment of a tumour, comprising the steps of:

- generating paramagnetic particles which are capable of at least in part disturbing a magnetic field, wherein said particles comprise holmium, gadolinium and/or dysprosium and have a diameter of 1-200 μm ;

- rendering said paramagnetic particles radioactive;

- preparing a therapeutic composition for treatment of a tumour comprising an optimal therapeutic dosage of said paramagnetic particles,

wherein said optimal dosage of said therapeutic composition is determined based on the distribution inside a patient of paramagnetic particles of a scanning suspension which are capable of at least in part disturbing a magnetic field and which have essentially the same chemical structure as said paramagnetic particles in said therapeutic composition, wherein a scanning image is obtained using a non-radioactive scanning method.

2. A method according to claim 1 wherein said scanning image is an MRI image.

3. A method according to claim 1 or 2, wherein an amount of particles is prepared prior to obtaining said scanning image, wherein a first part of said amount of particles is used for preparing said scanning suspension and a second part of said amount of particles is used for preparing said therapeutic suspension.

4. A method according to any one of claims 1 to 3, wherein a dose of radiation for rendering said particles for use in said therapeutic suspension radioactive, and/or the amount of particles to be used in said therapeutic suspension, is at least partly based on said scanning image obtained.

5. A method according to any one of claims 1 to 4, further comprising imaging said paramagnetic particles using a gamma-camera.

6. A kit of parts when used in a method according to any one of claims 1 to 5, comprising a diagnostic composition; a therapeutic composition; and instructions for use in treating a tumour, wherein said diagnostic composition and said therapeutic composition comprise paramagnetic particles comprising holmium, gadolinium and/or dysprosium with essentially the same chemical structure for at least in part disturbing a magnetic field, said therapeutic composition being more radioactive than said diagnostic composition, said particles having a diameter of 1-200 μm .
7. A kit of parts according to claim 6, wherein said diagnostic composition is essentially non-radioactive.
8. A kit of parts according to claim 6 or 7, wherein said particles comprise holmium.
9. Use of a paramagnetic particle for at least in part disturbing a magnetic field as a medicament, wherein the dosage of said particle is derived from a scanning image obtained with particles with essentially the same chemical structure, said scanning image obtained using a non-radioactive scanning method, based on the distribution of said particles in said scanning image inside a patient, wherein said particle comprises holmium, gadolinium and/or dysprosium and has a diameter of between 20 and 100 μm , and wherein said particle is more radioactive than said particles used for obtaining said scanning image.
10. Use of a paramagnetic particle for at least in part disturbing a magnetic field for the preparation of a medicament for the treatment of a tumour, wherein the dosage of said particle is derived from a scanning image obtained with particles with essentially the same chemical structure, said scanning image obtained using a non-radioactive scanning method, based on the distribution of said particles in said scanning image inside a patient, wherein said particle comprises holmium, gadolinium and/or dysprosium and has a diameter of between 20 and 100 μm , and wherein said particle is more radioactive than said particles used for obtaining said scanning image.
11. A use according to claim 10, wherein said tumour comprises a liver metastasis.

12. A use according to claim 10 or 11, wherein said particle comprises a composition which essentially maintains its structure during irradiation for 1 hour with a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$.
13. A use according to any one of claims 10 to 12, wherein said particle comprises a microsphere.
14. A use according to any one of claims 10 to 13, wherein said particle comprises a poly(L-lactic acid) microsphere.
15. A use according to claim 12 or any one of claims 13 to 14 when dependent on claim 12, wherein said composition comprises holmium chemically bound to a compound which essentially maintains its structure during irradiation for 1 hour with a neutron flux of $5 \times 10^{13} \text{ cm}^{-2} \cdot \text{s}^{-1}$.
16. A scanning suspension comprising paramagnetic particles for at least in part disturbing a magnetic field, wherein said particles comprise holmium, gadolinium and/or dysprosium and have a diameter of 1-200 μm and have been irradiated when used in a method according to any one of claims 1-5.
17. A scanning suspension according to claim 16, said particles having been irradiated by a neutron flux.
18. A kit of parts comprising a diagnostic composition; a therapeutic composition; and instructions for use in treating a tumour, wherein said diagnostic composition and said therapeutic composition comprise paramagnetic particles comprising holmium, gadolinium and/or dysprosium with essentially the same chemical structure for at least in part disturbing a magnetic field, said therapeutic composition being radioactive and said diagnostic composition being non-radioactive, said particles having a diameter of 1-200 μm .

19. Use of a particle for at least in part disturbing a magnetic field for the preparation of a kit of parts according to claim 18.

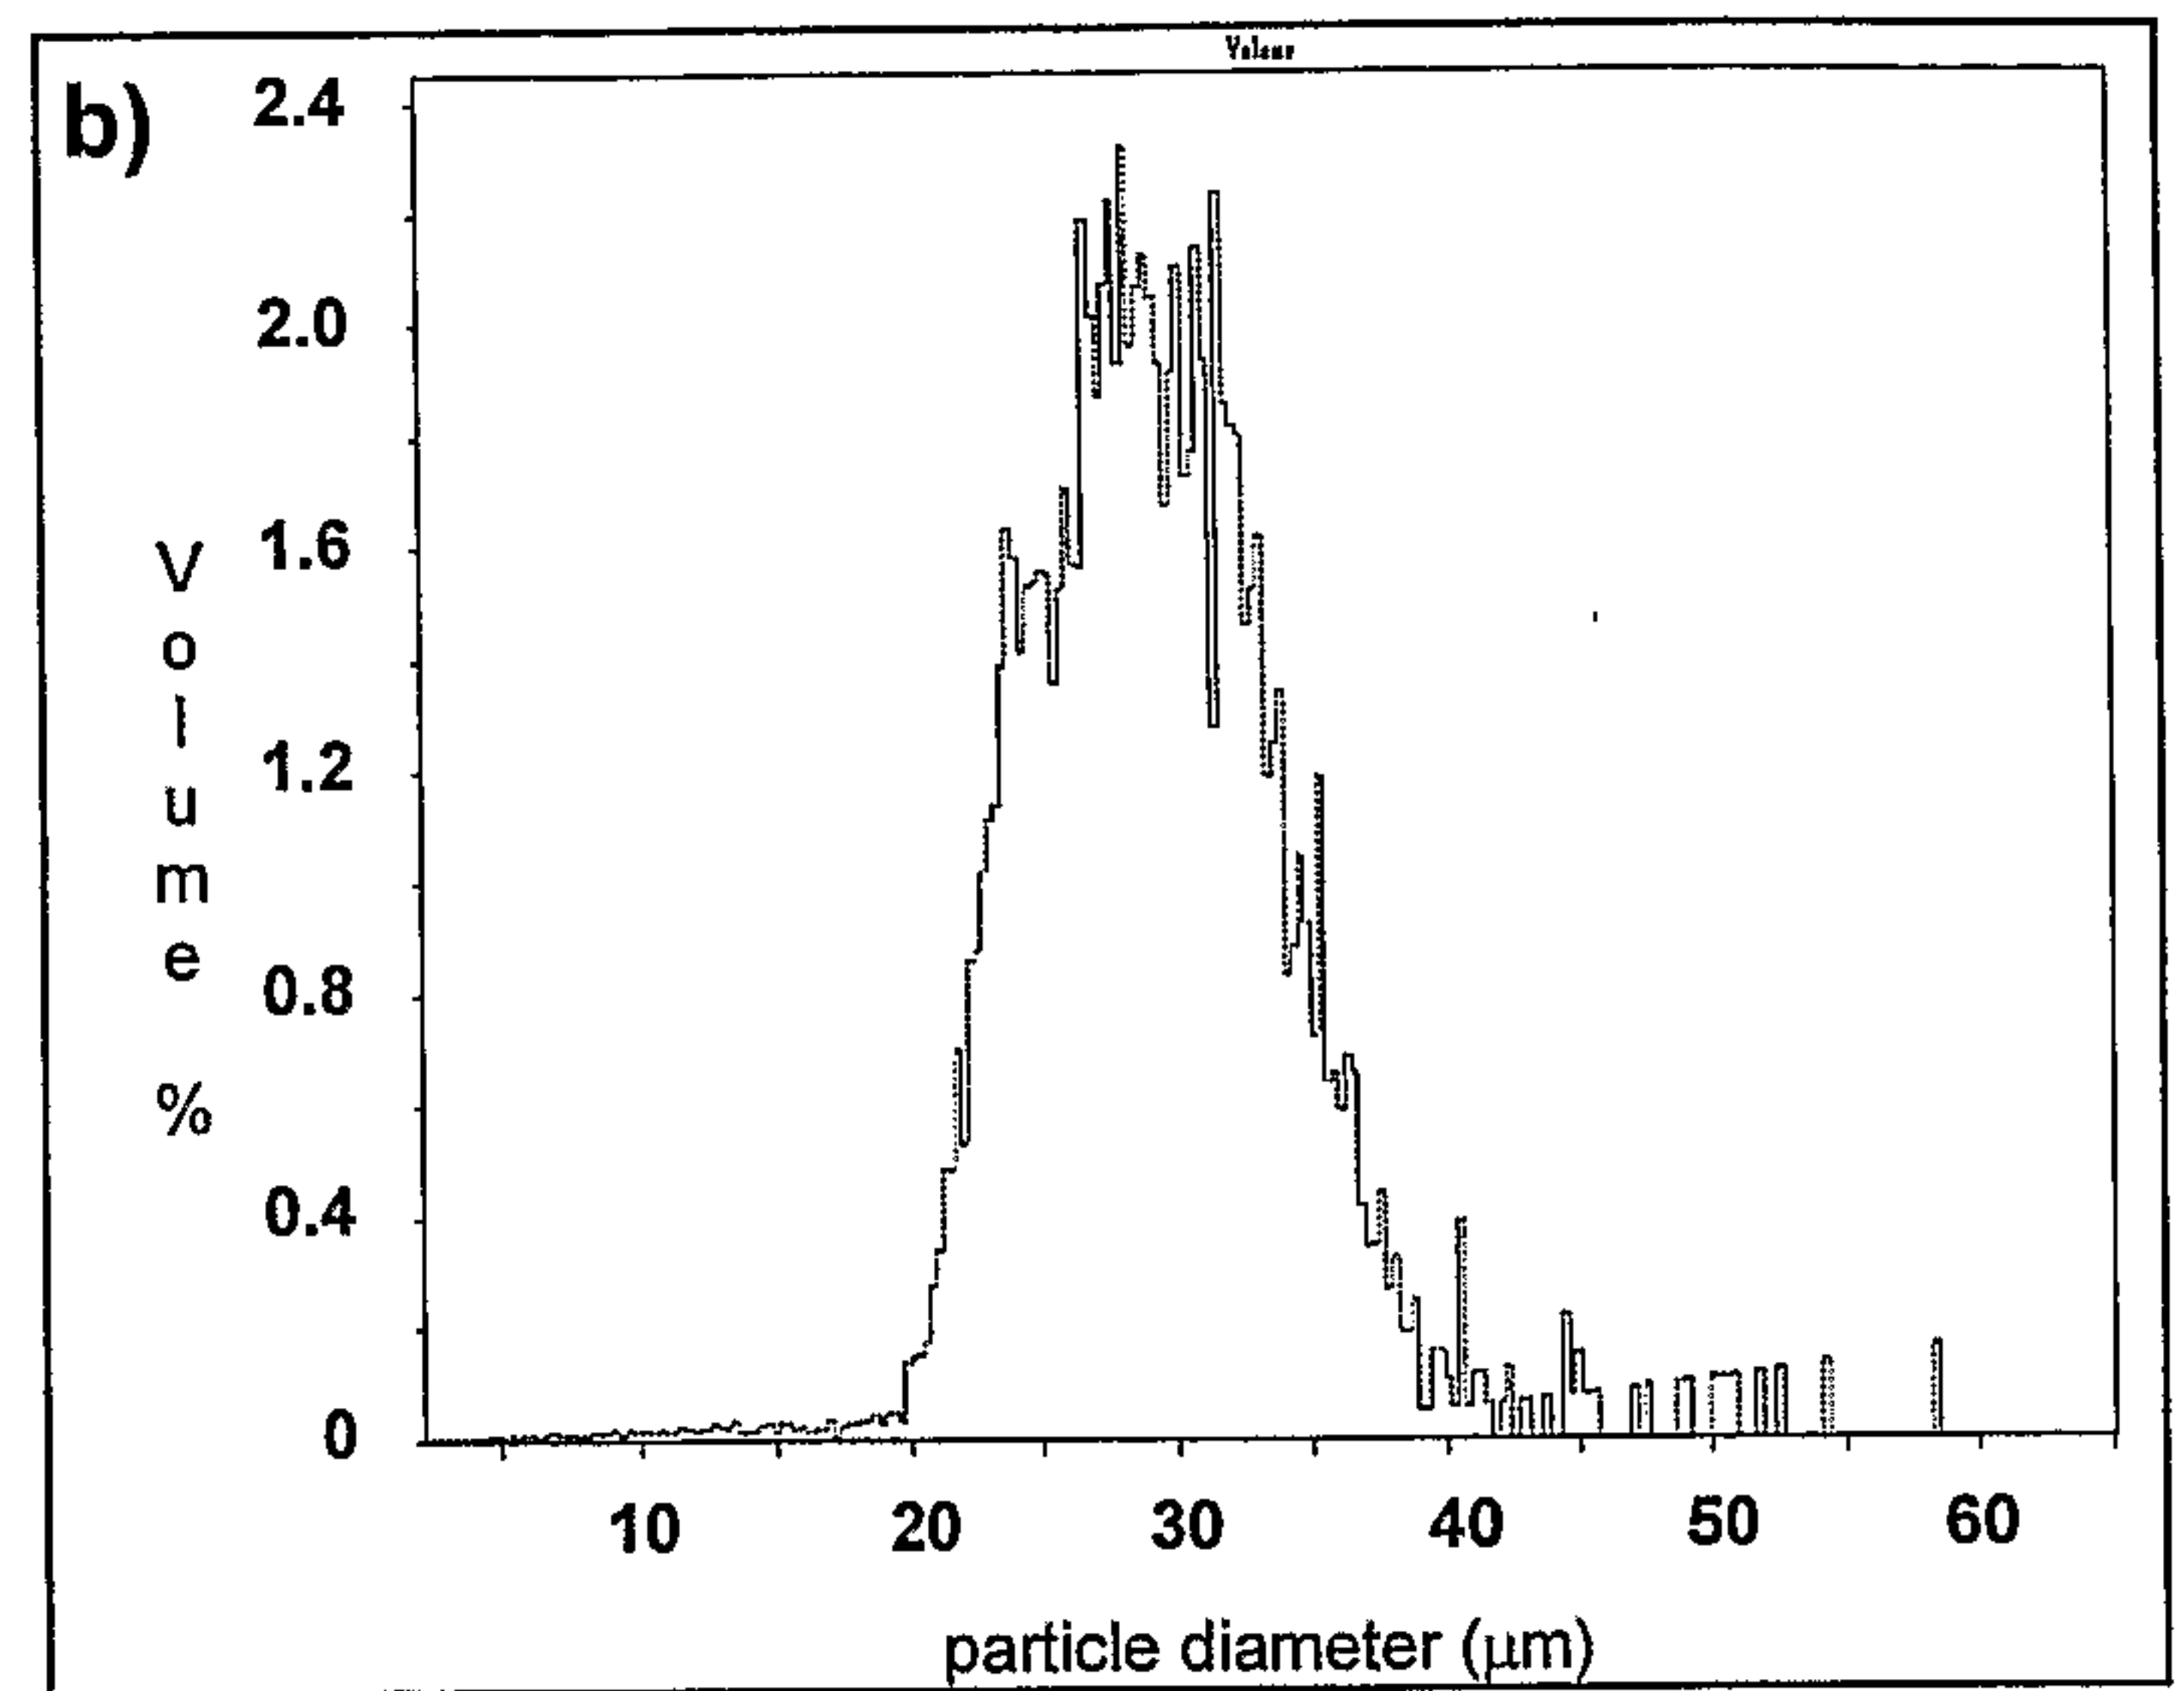
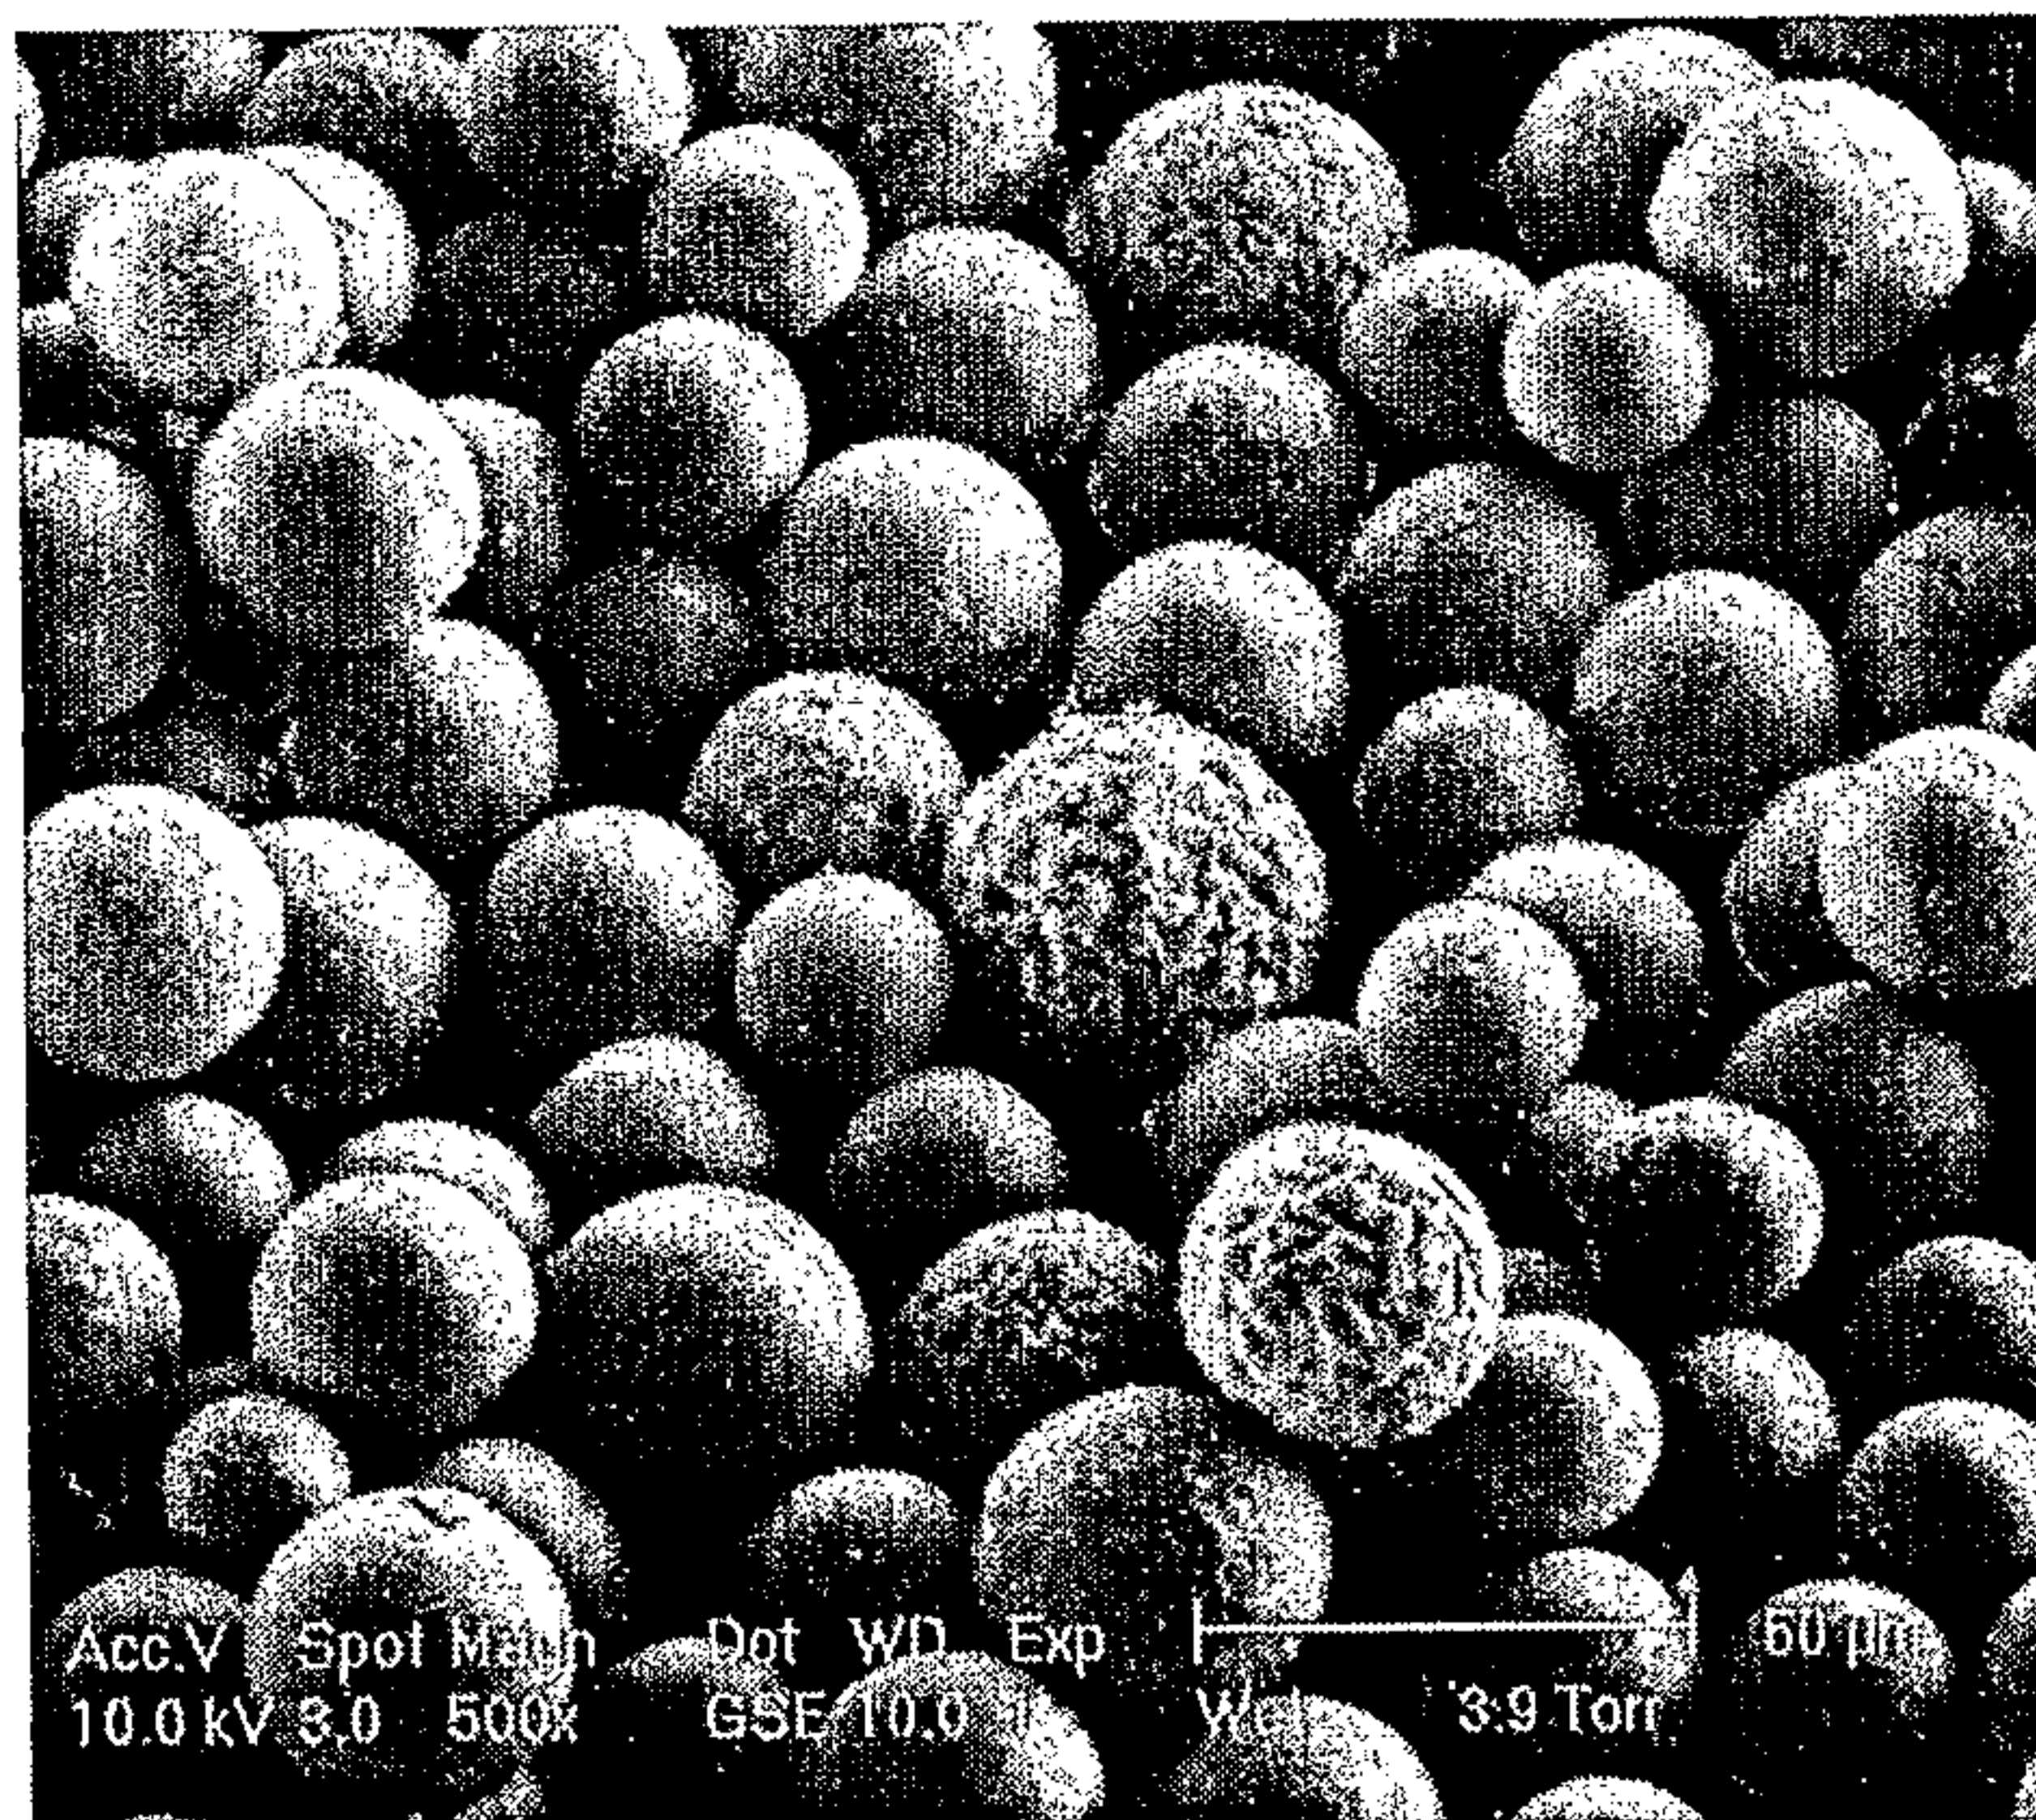
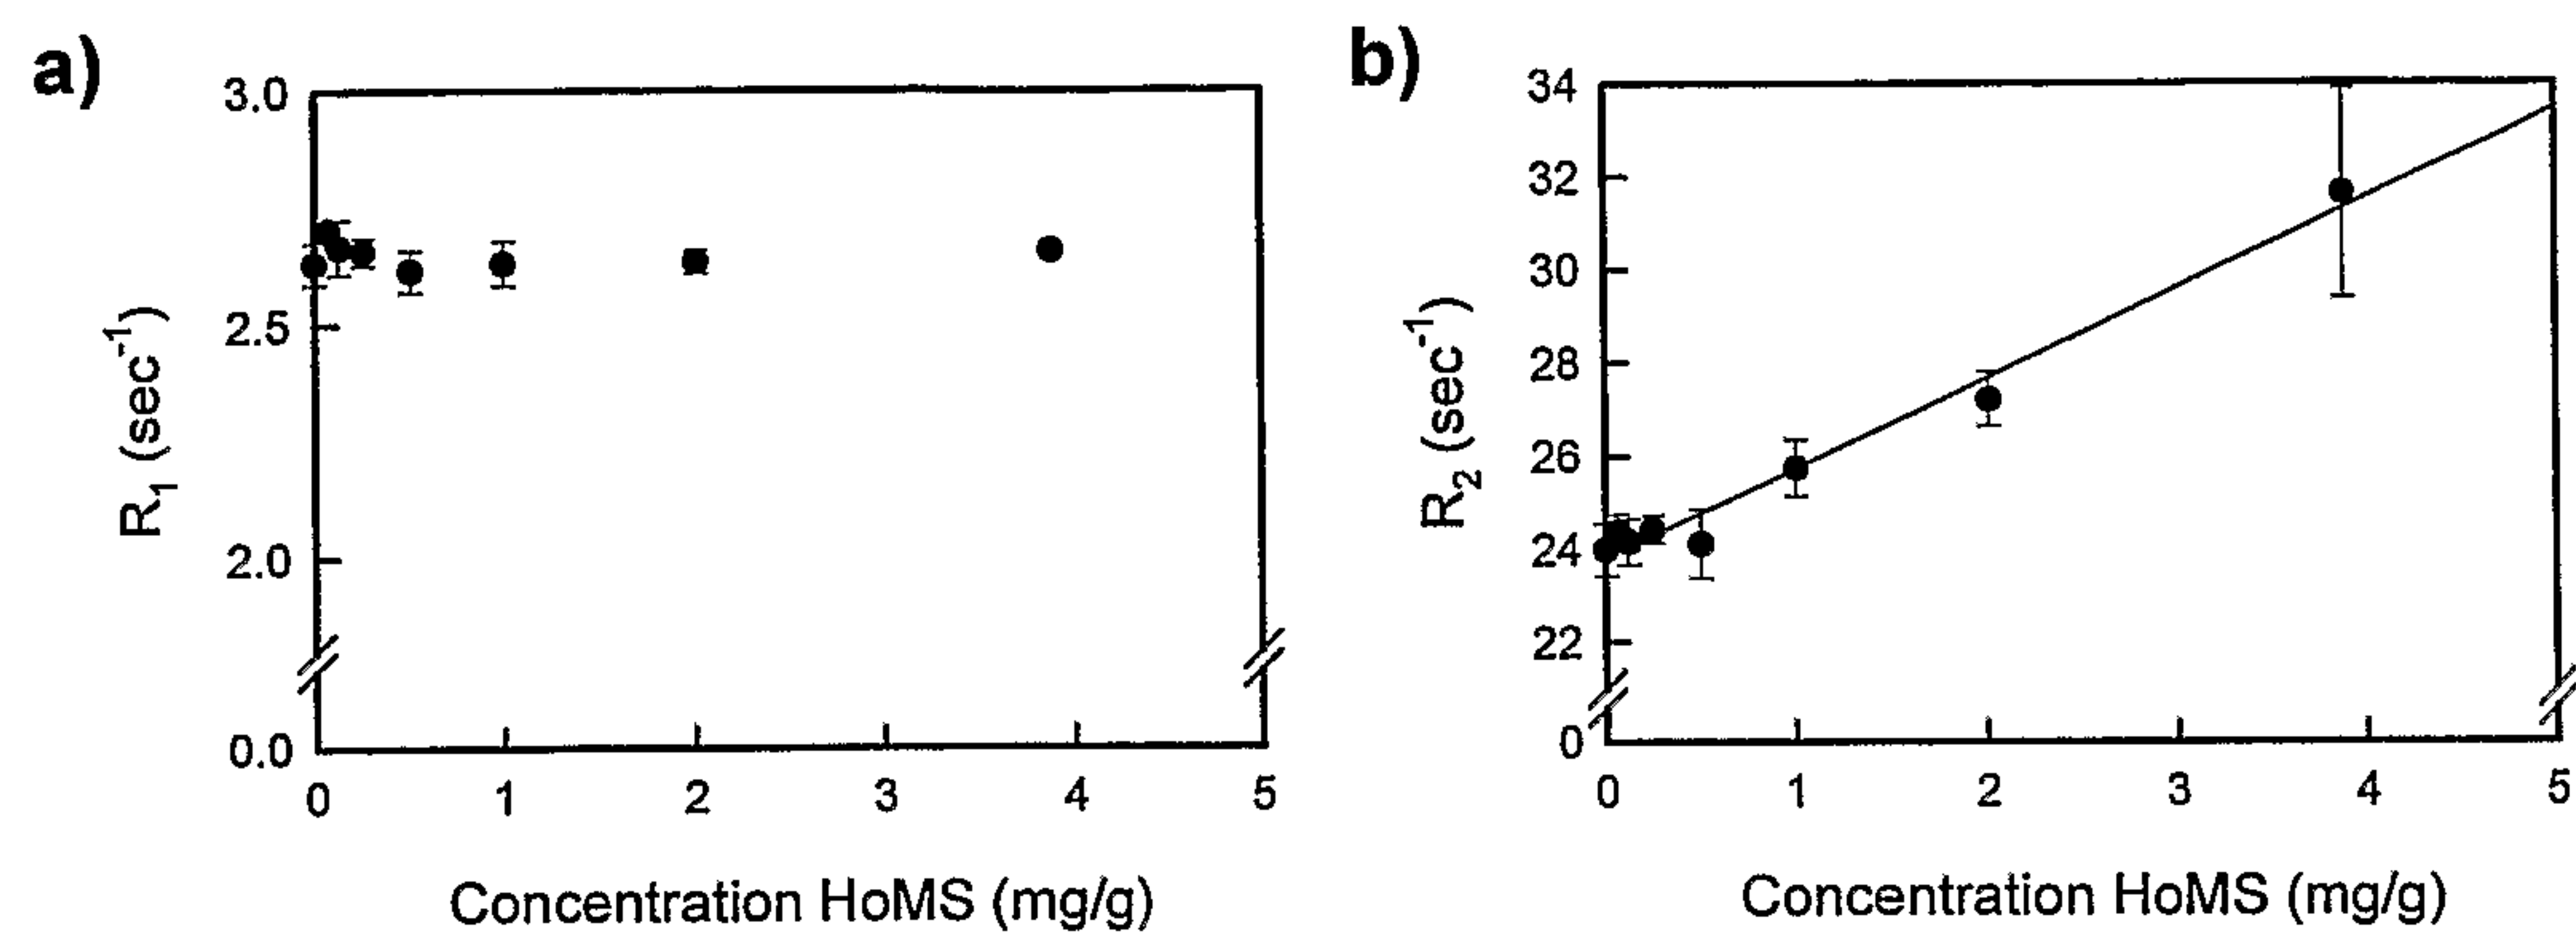
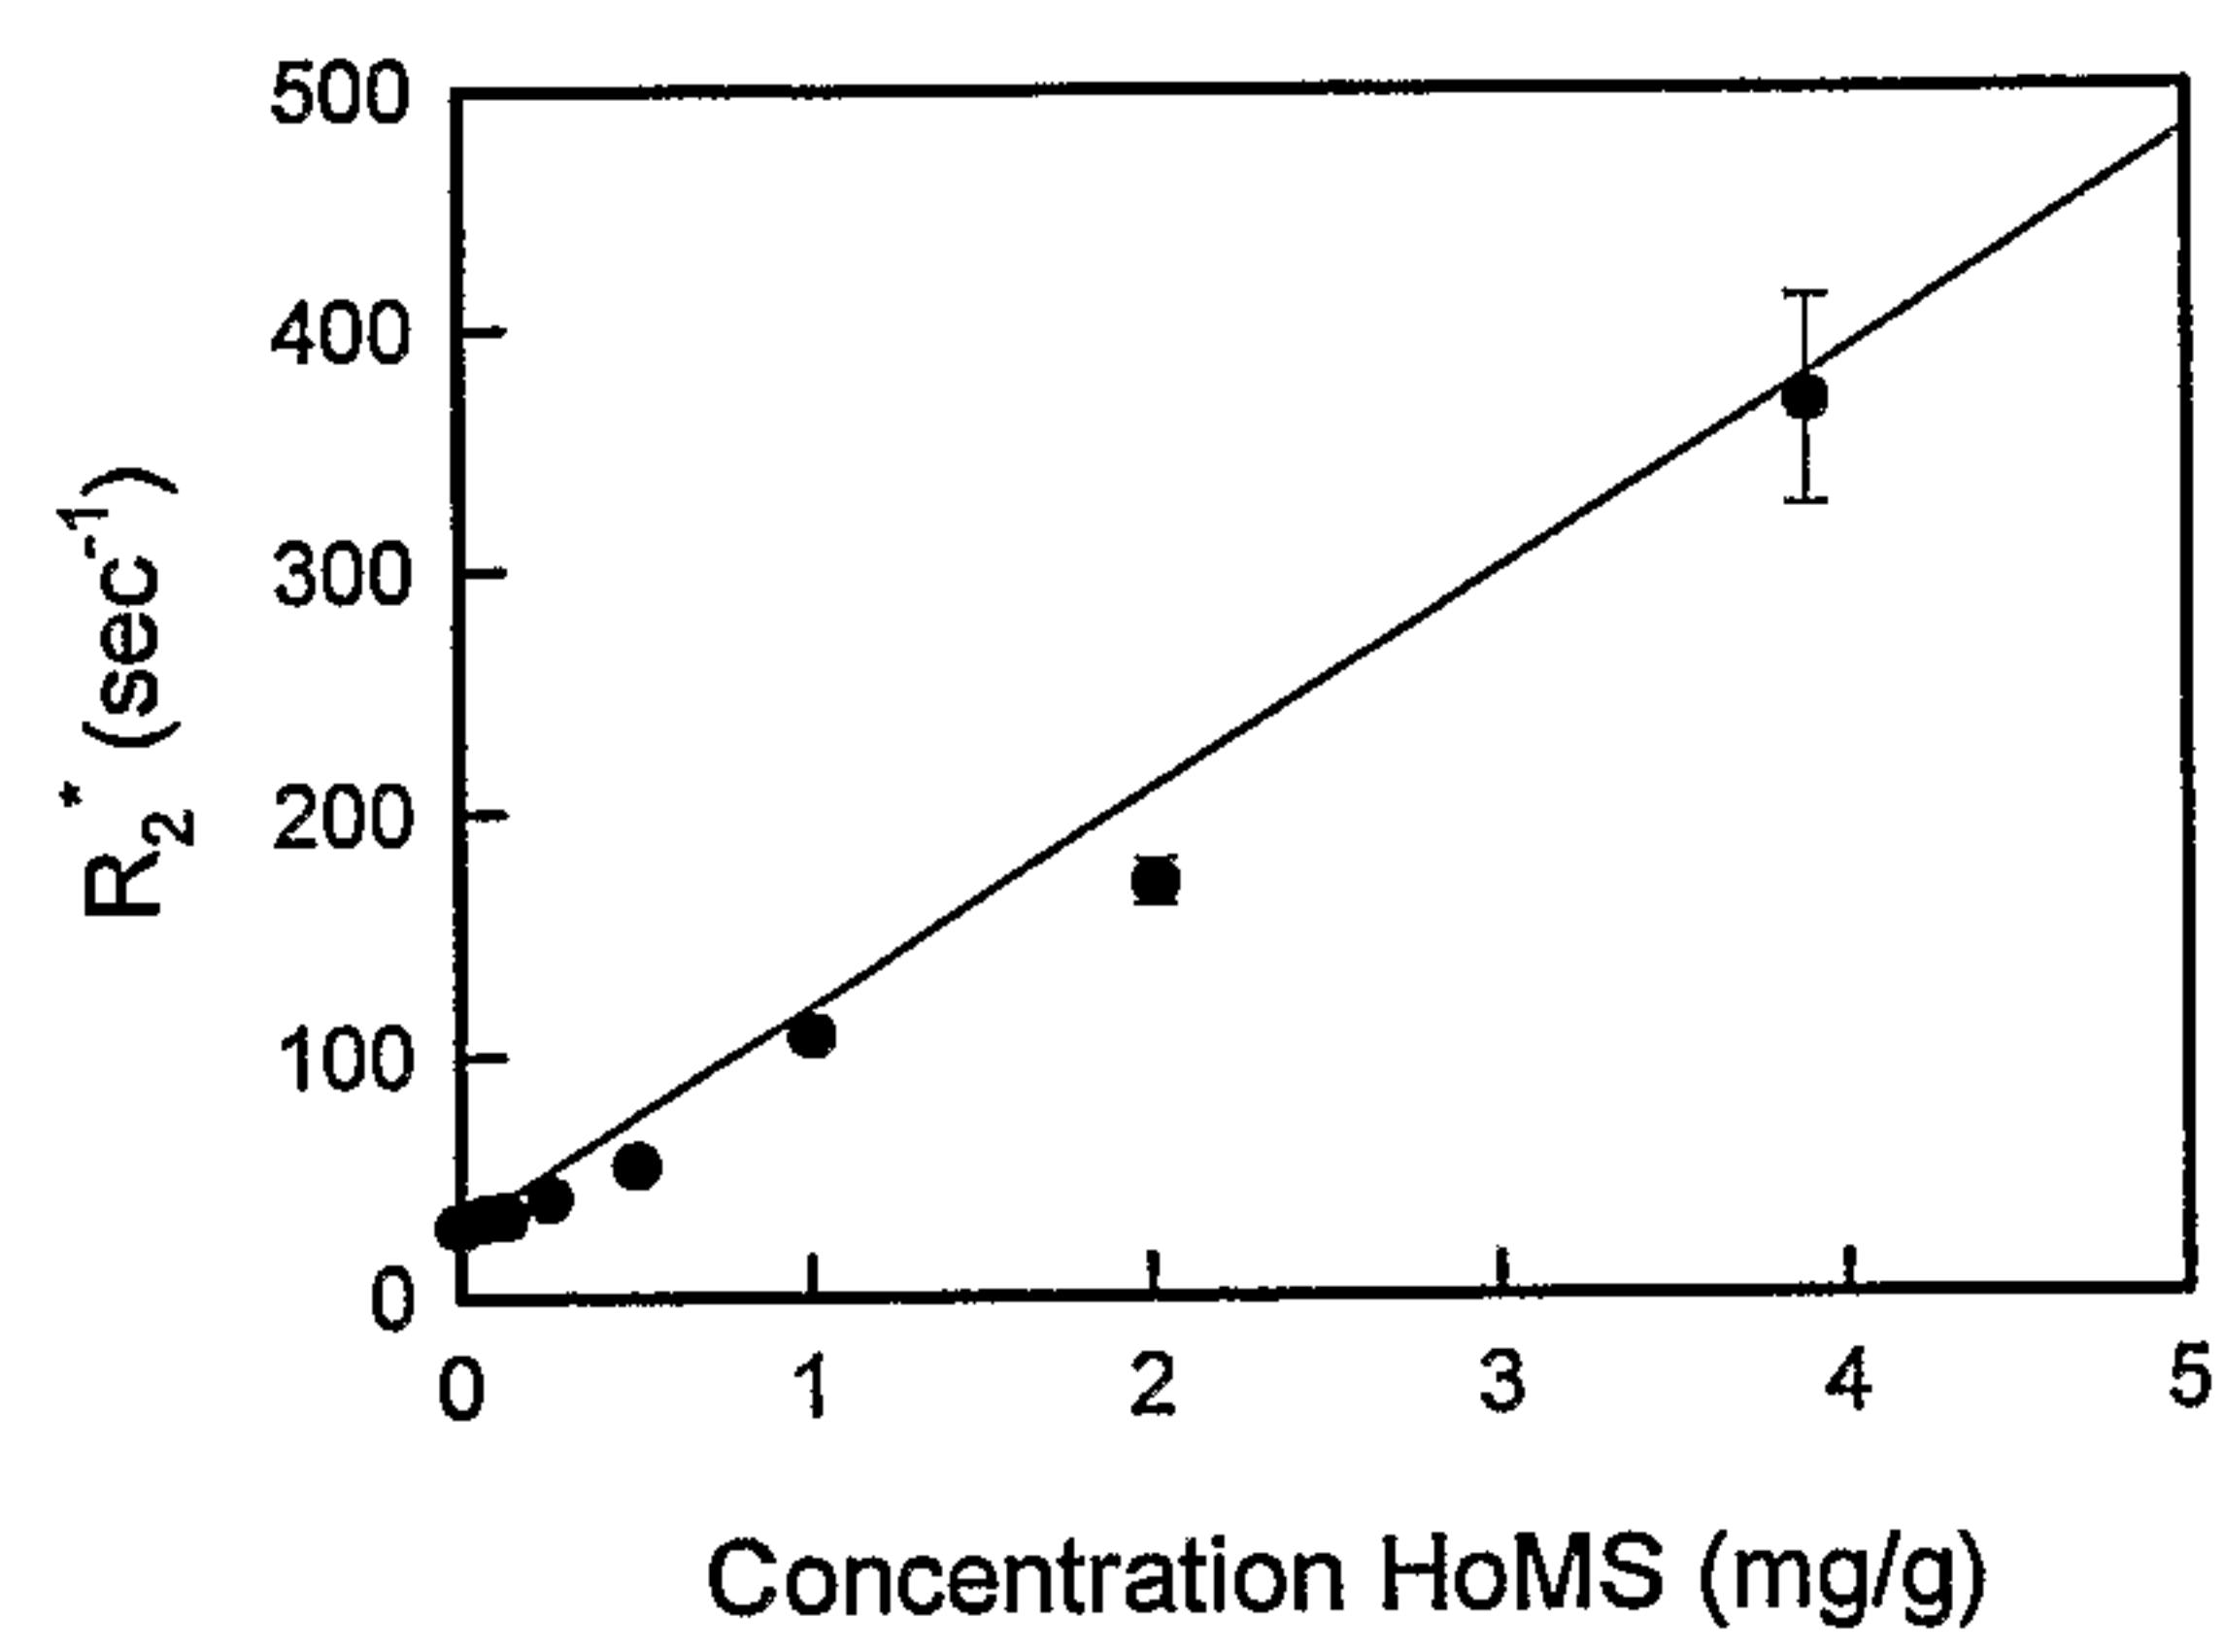


Figure 1a-b.

**Figure 2a-b.**

**Figure 3.**

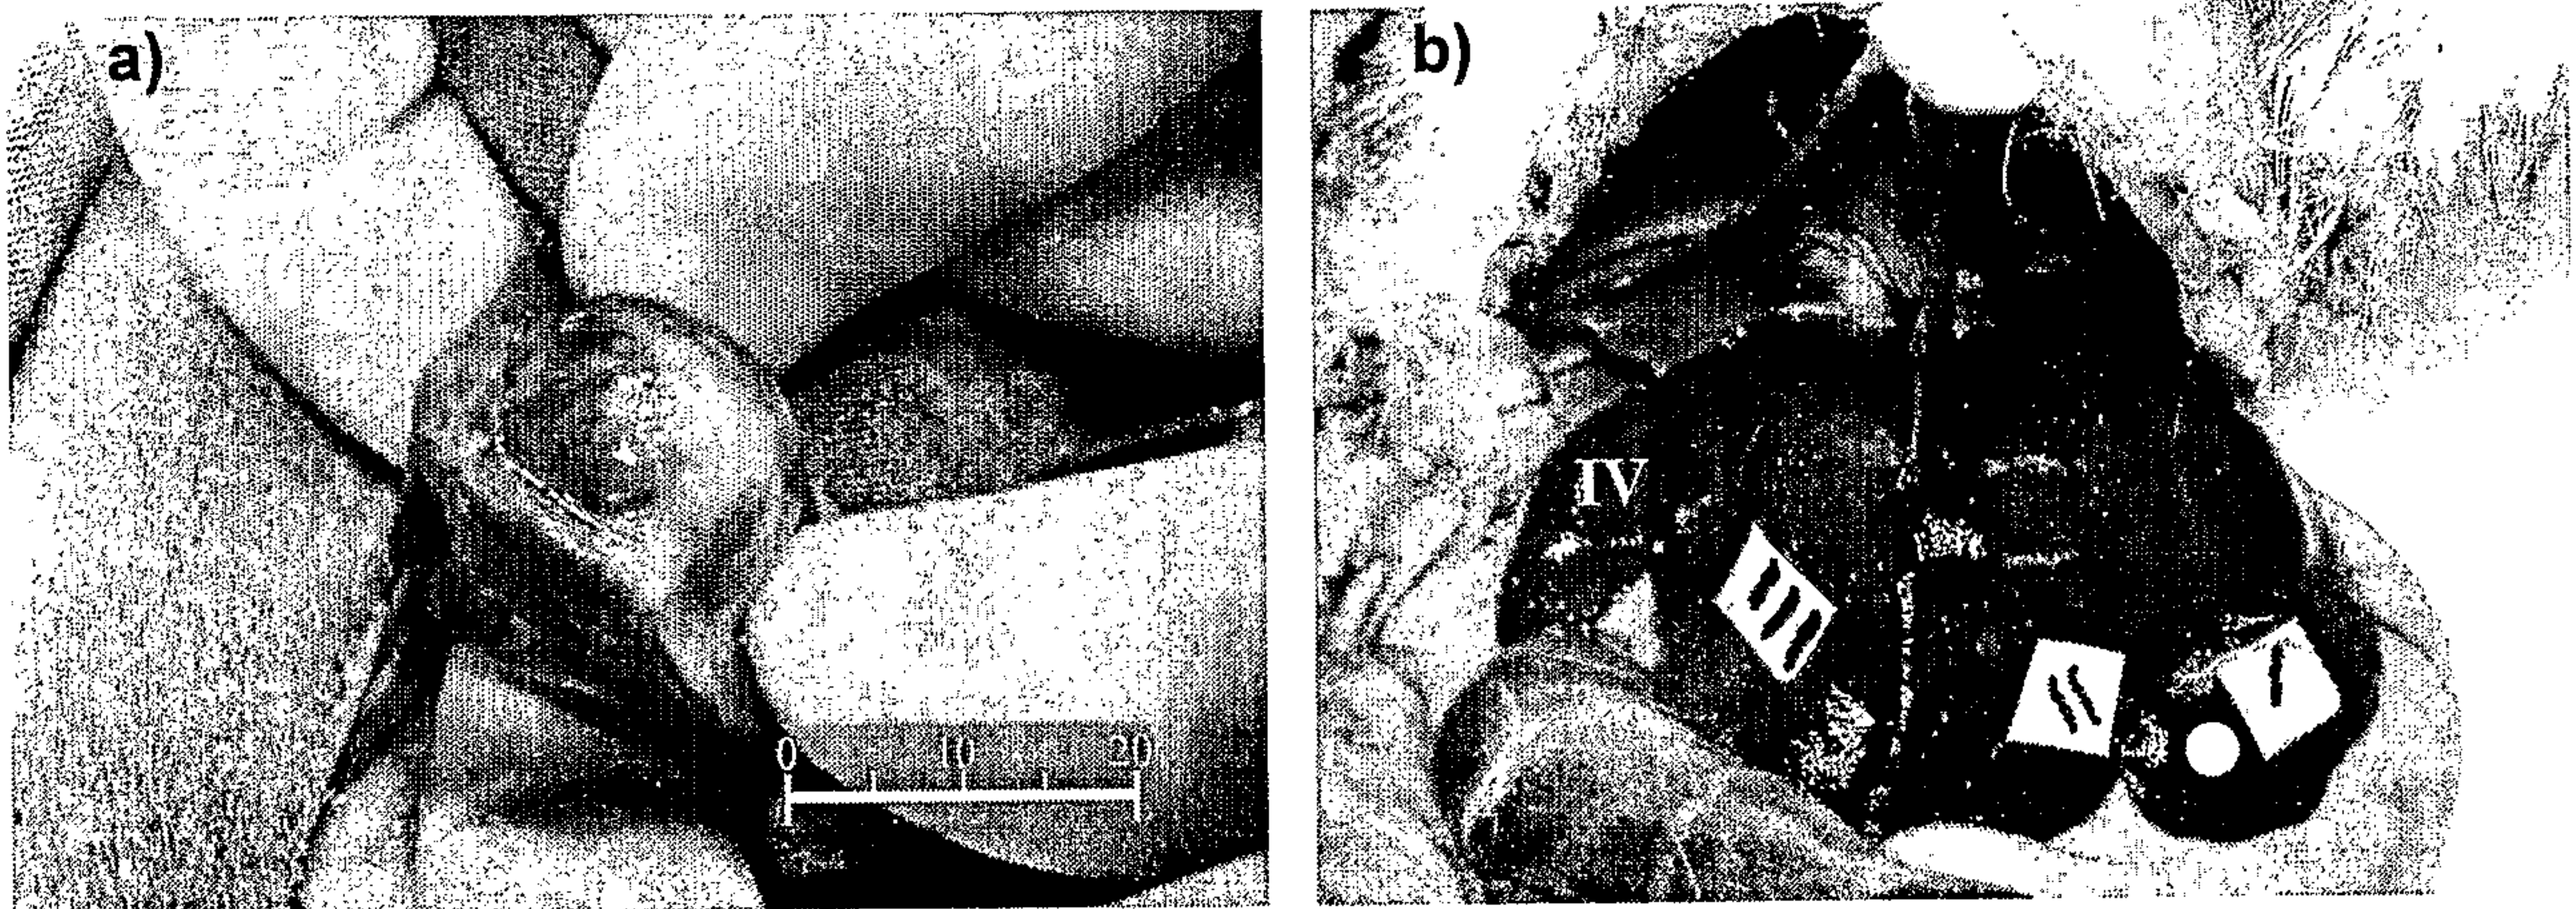
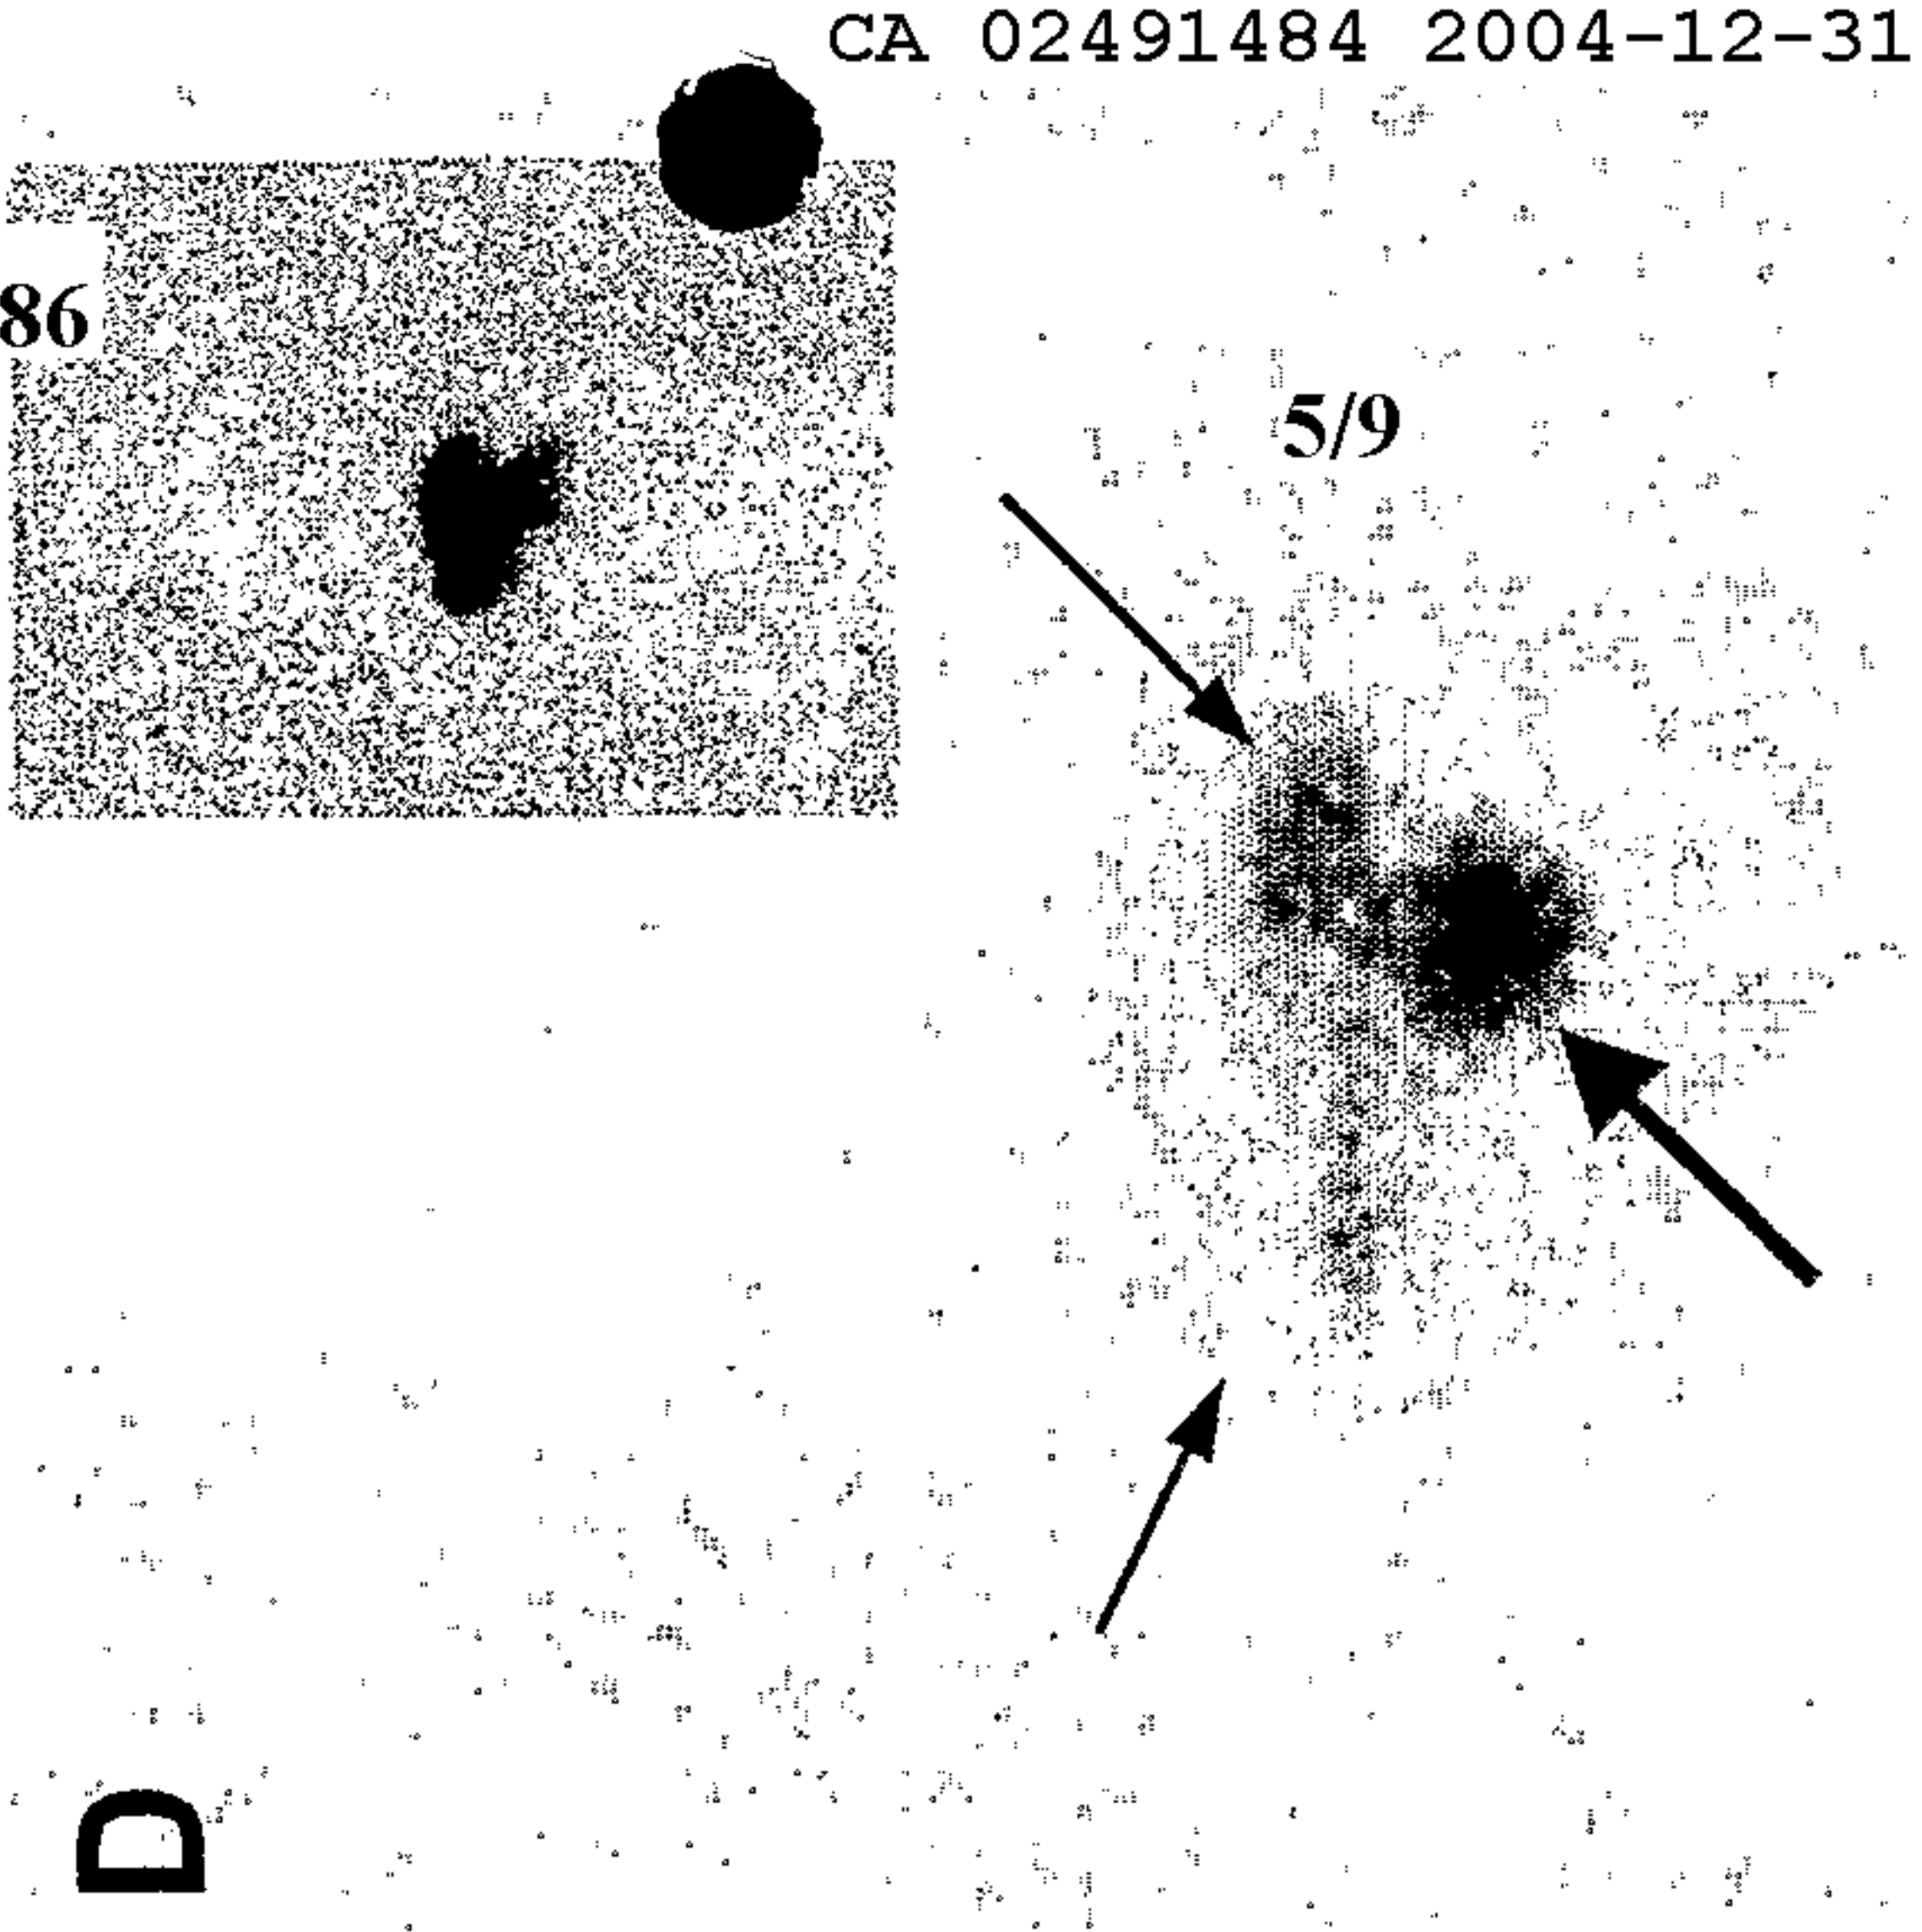
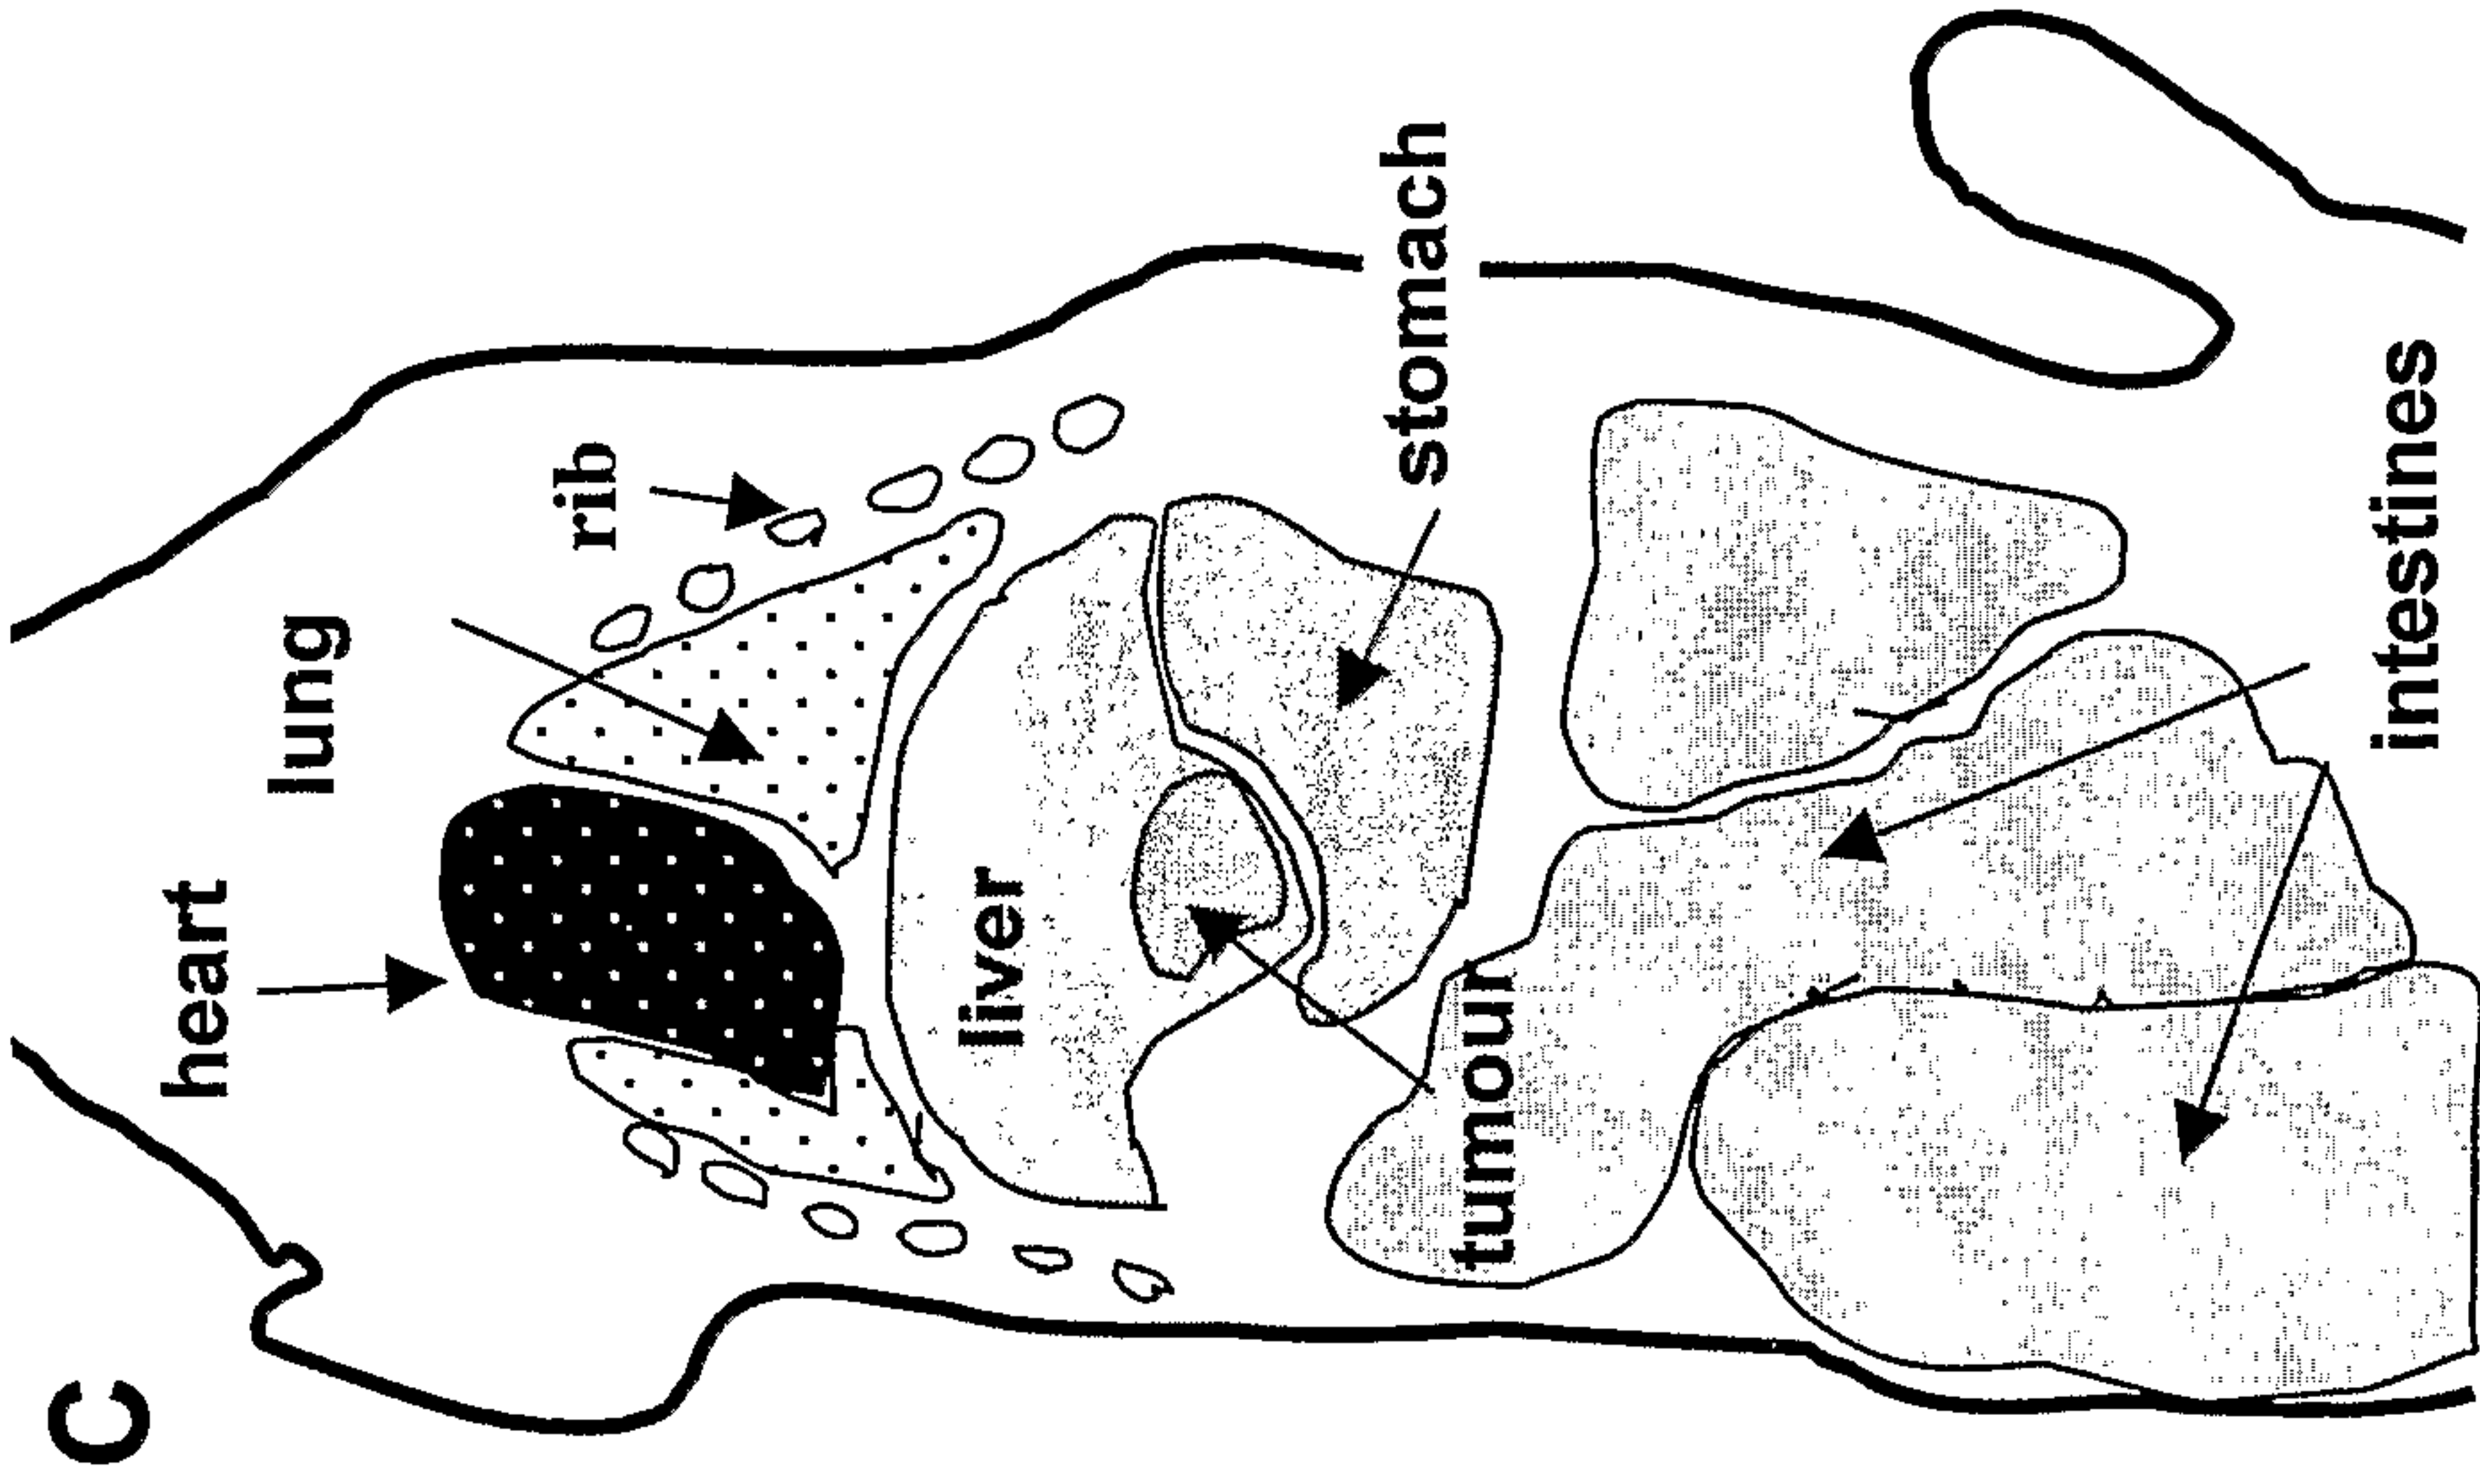
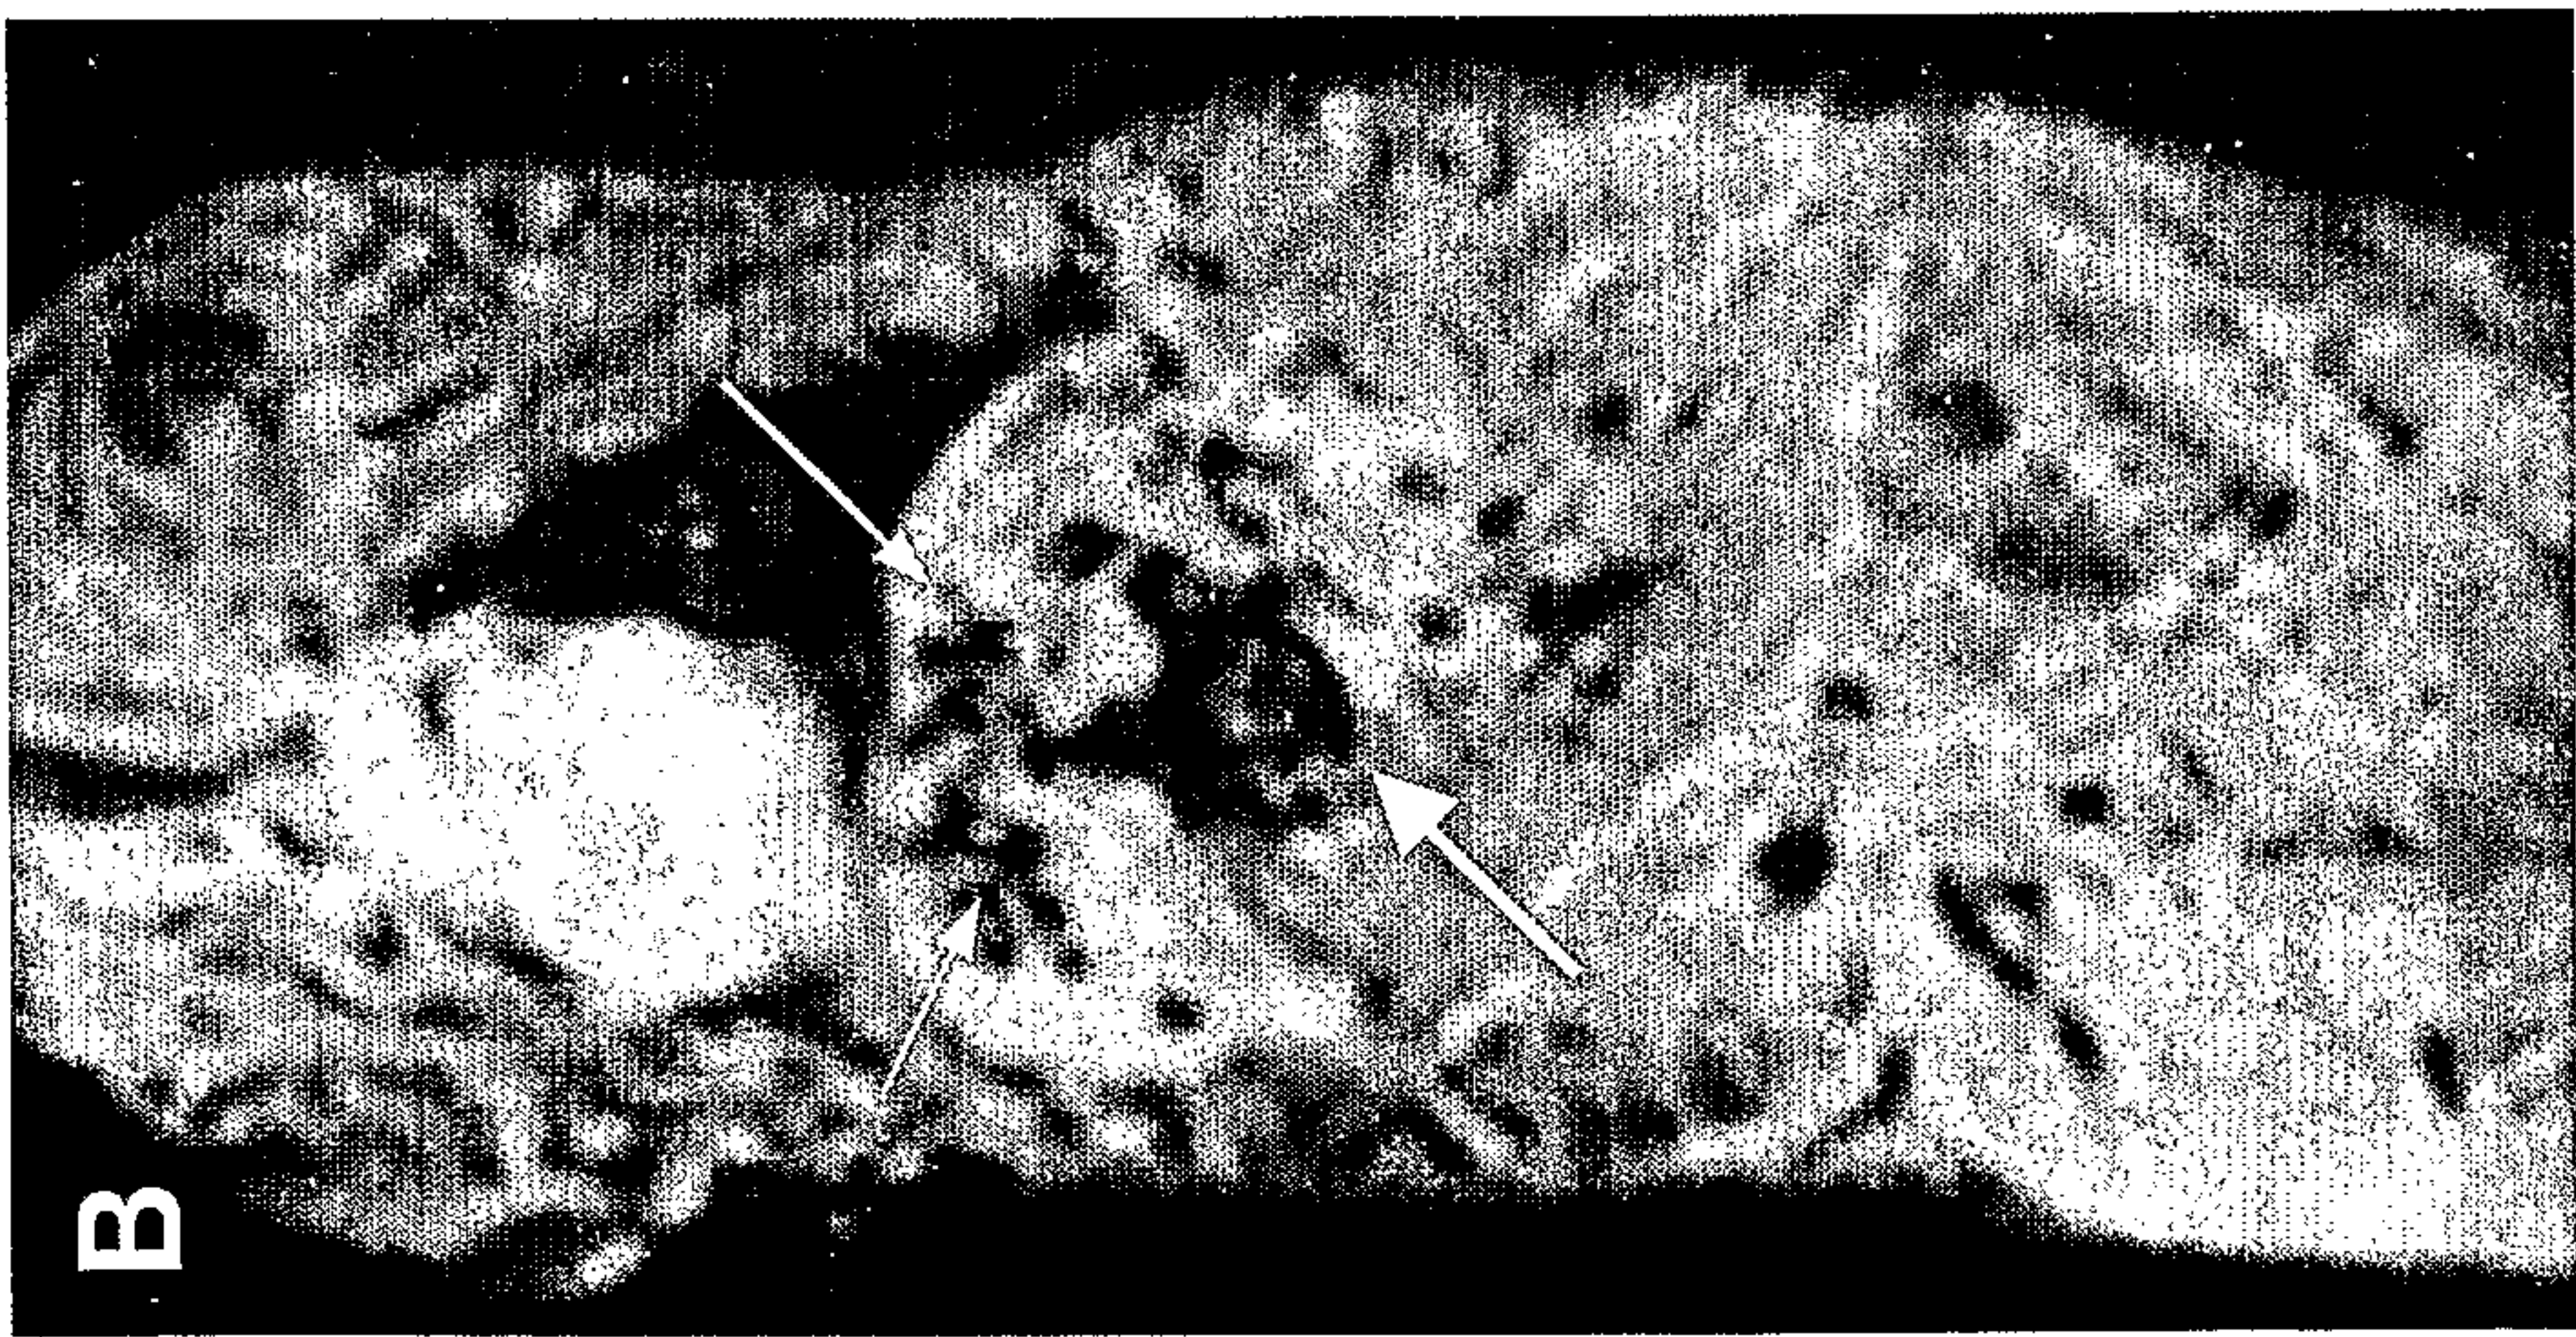
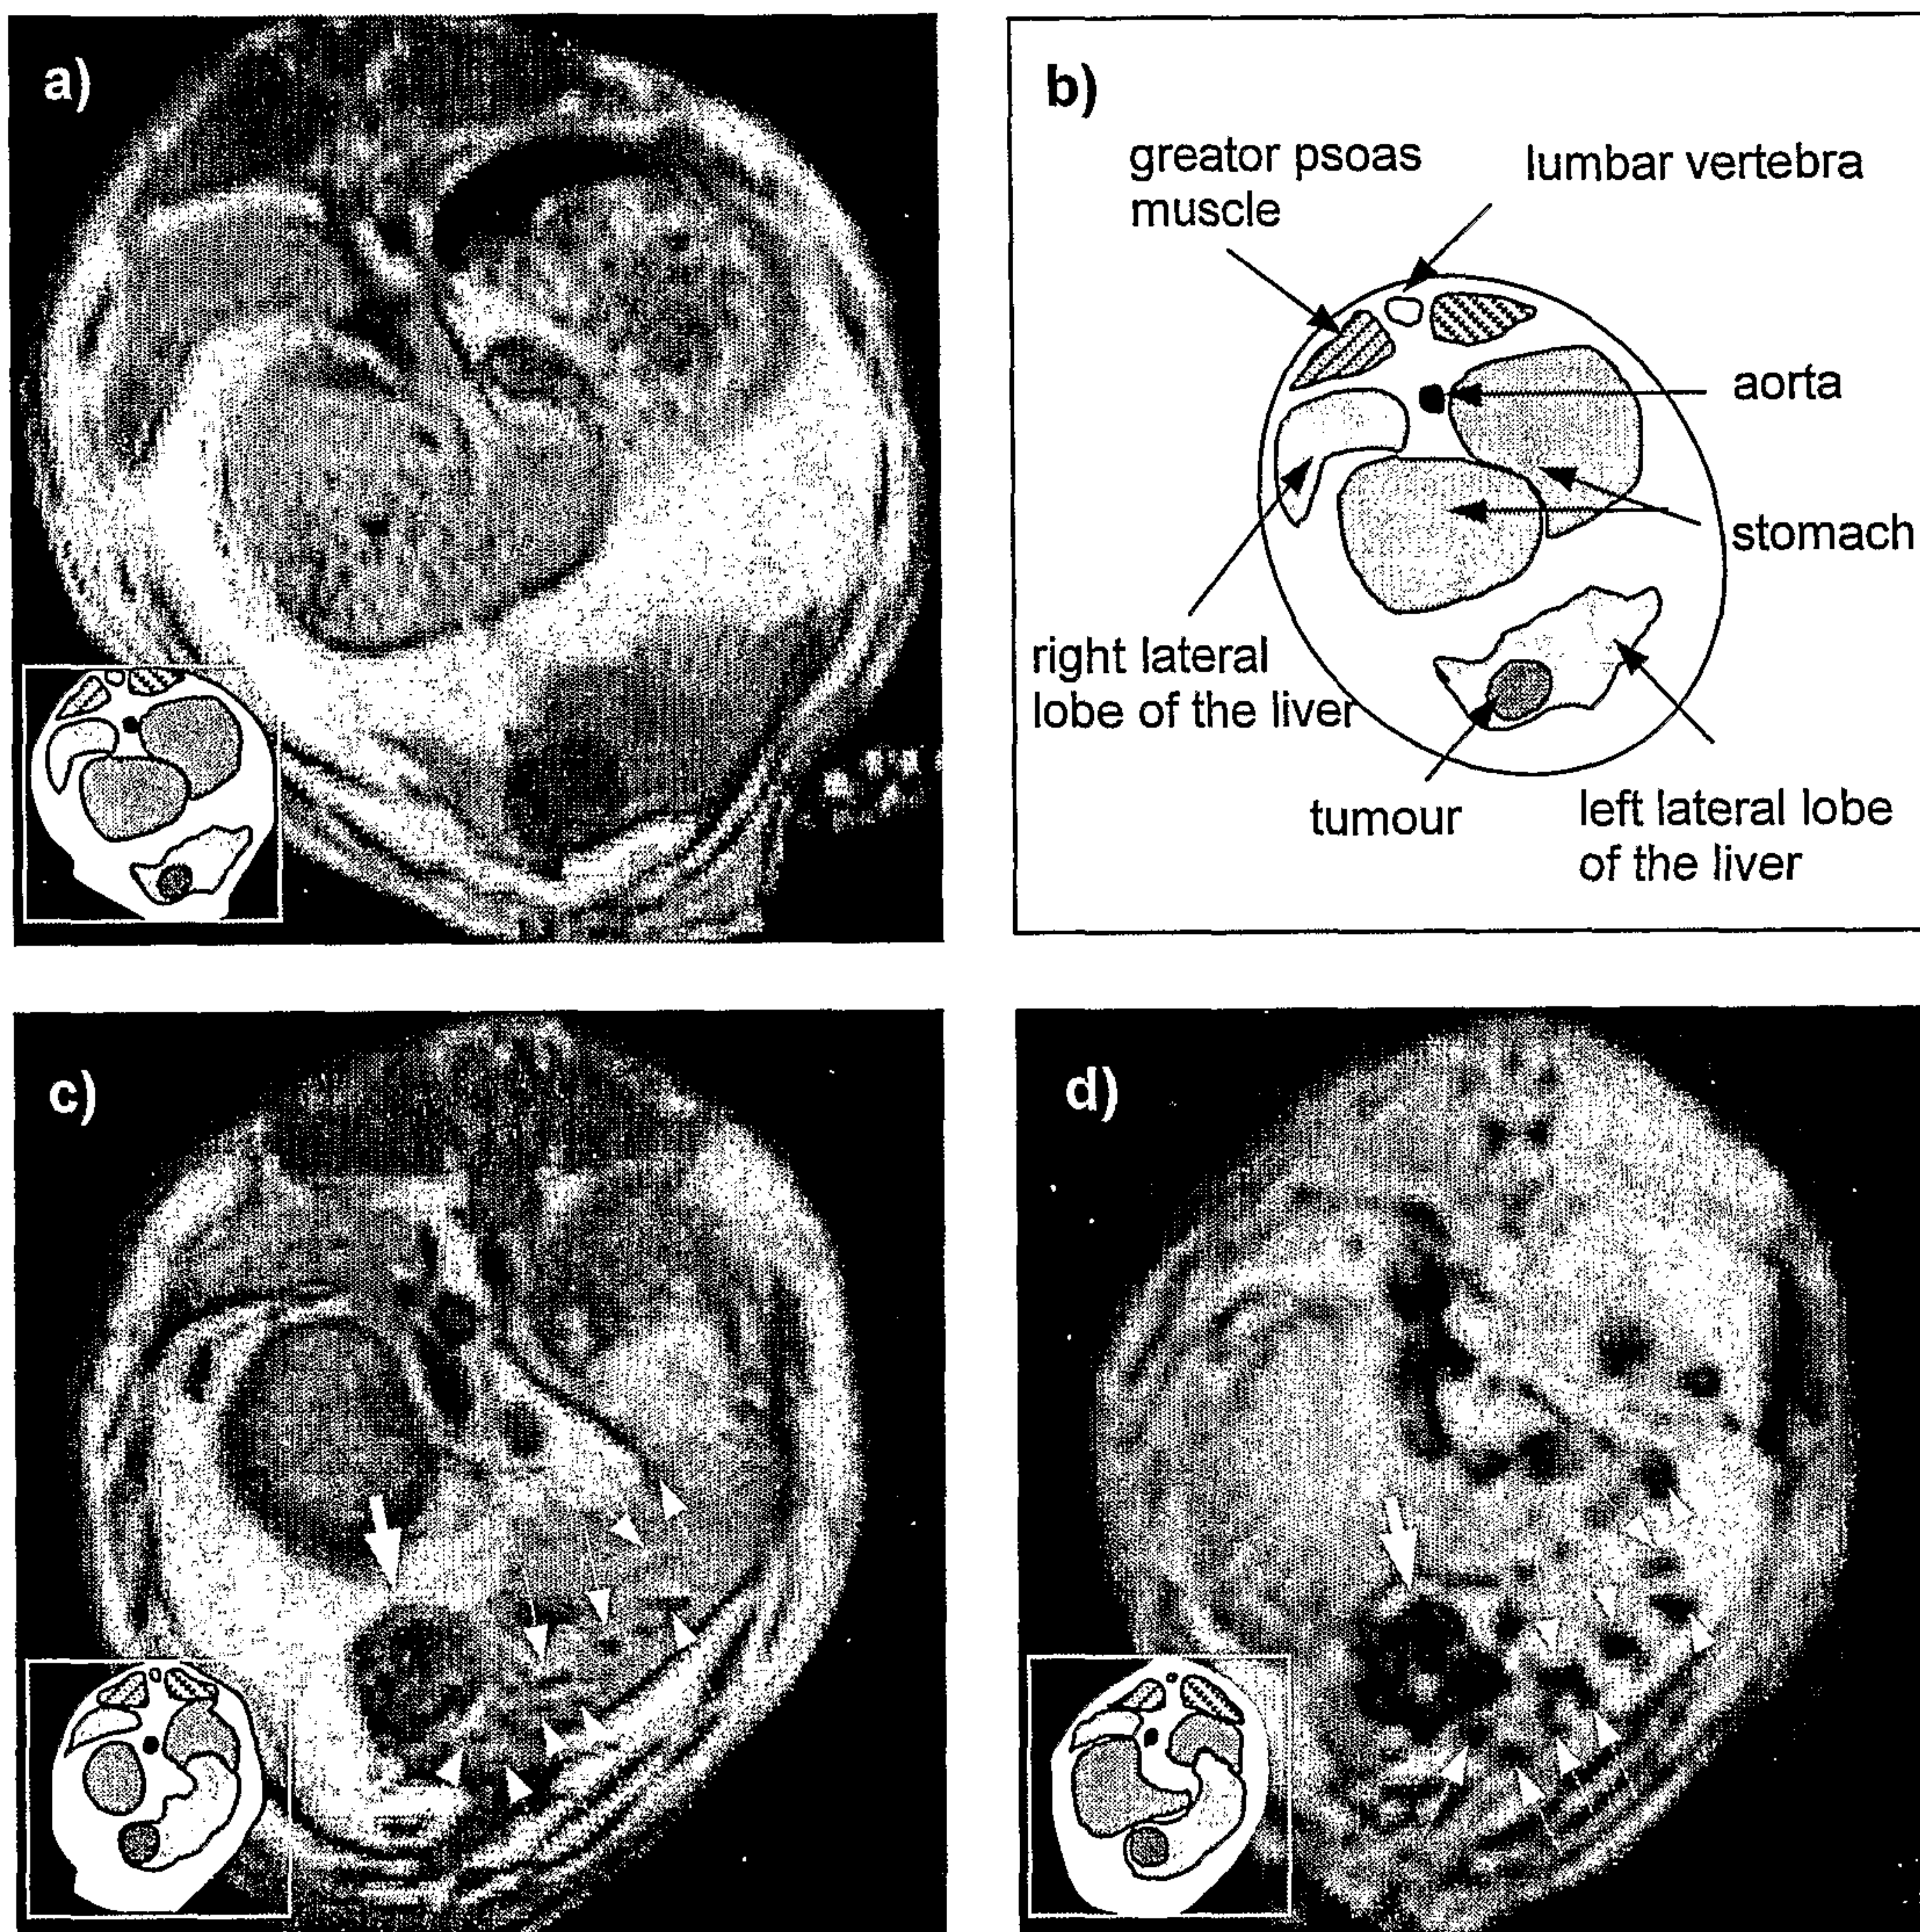


Fig.4a-b.

Figure 5



**Figure 6a-d.**

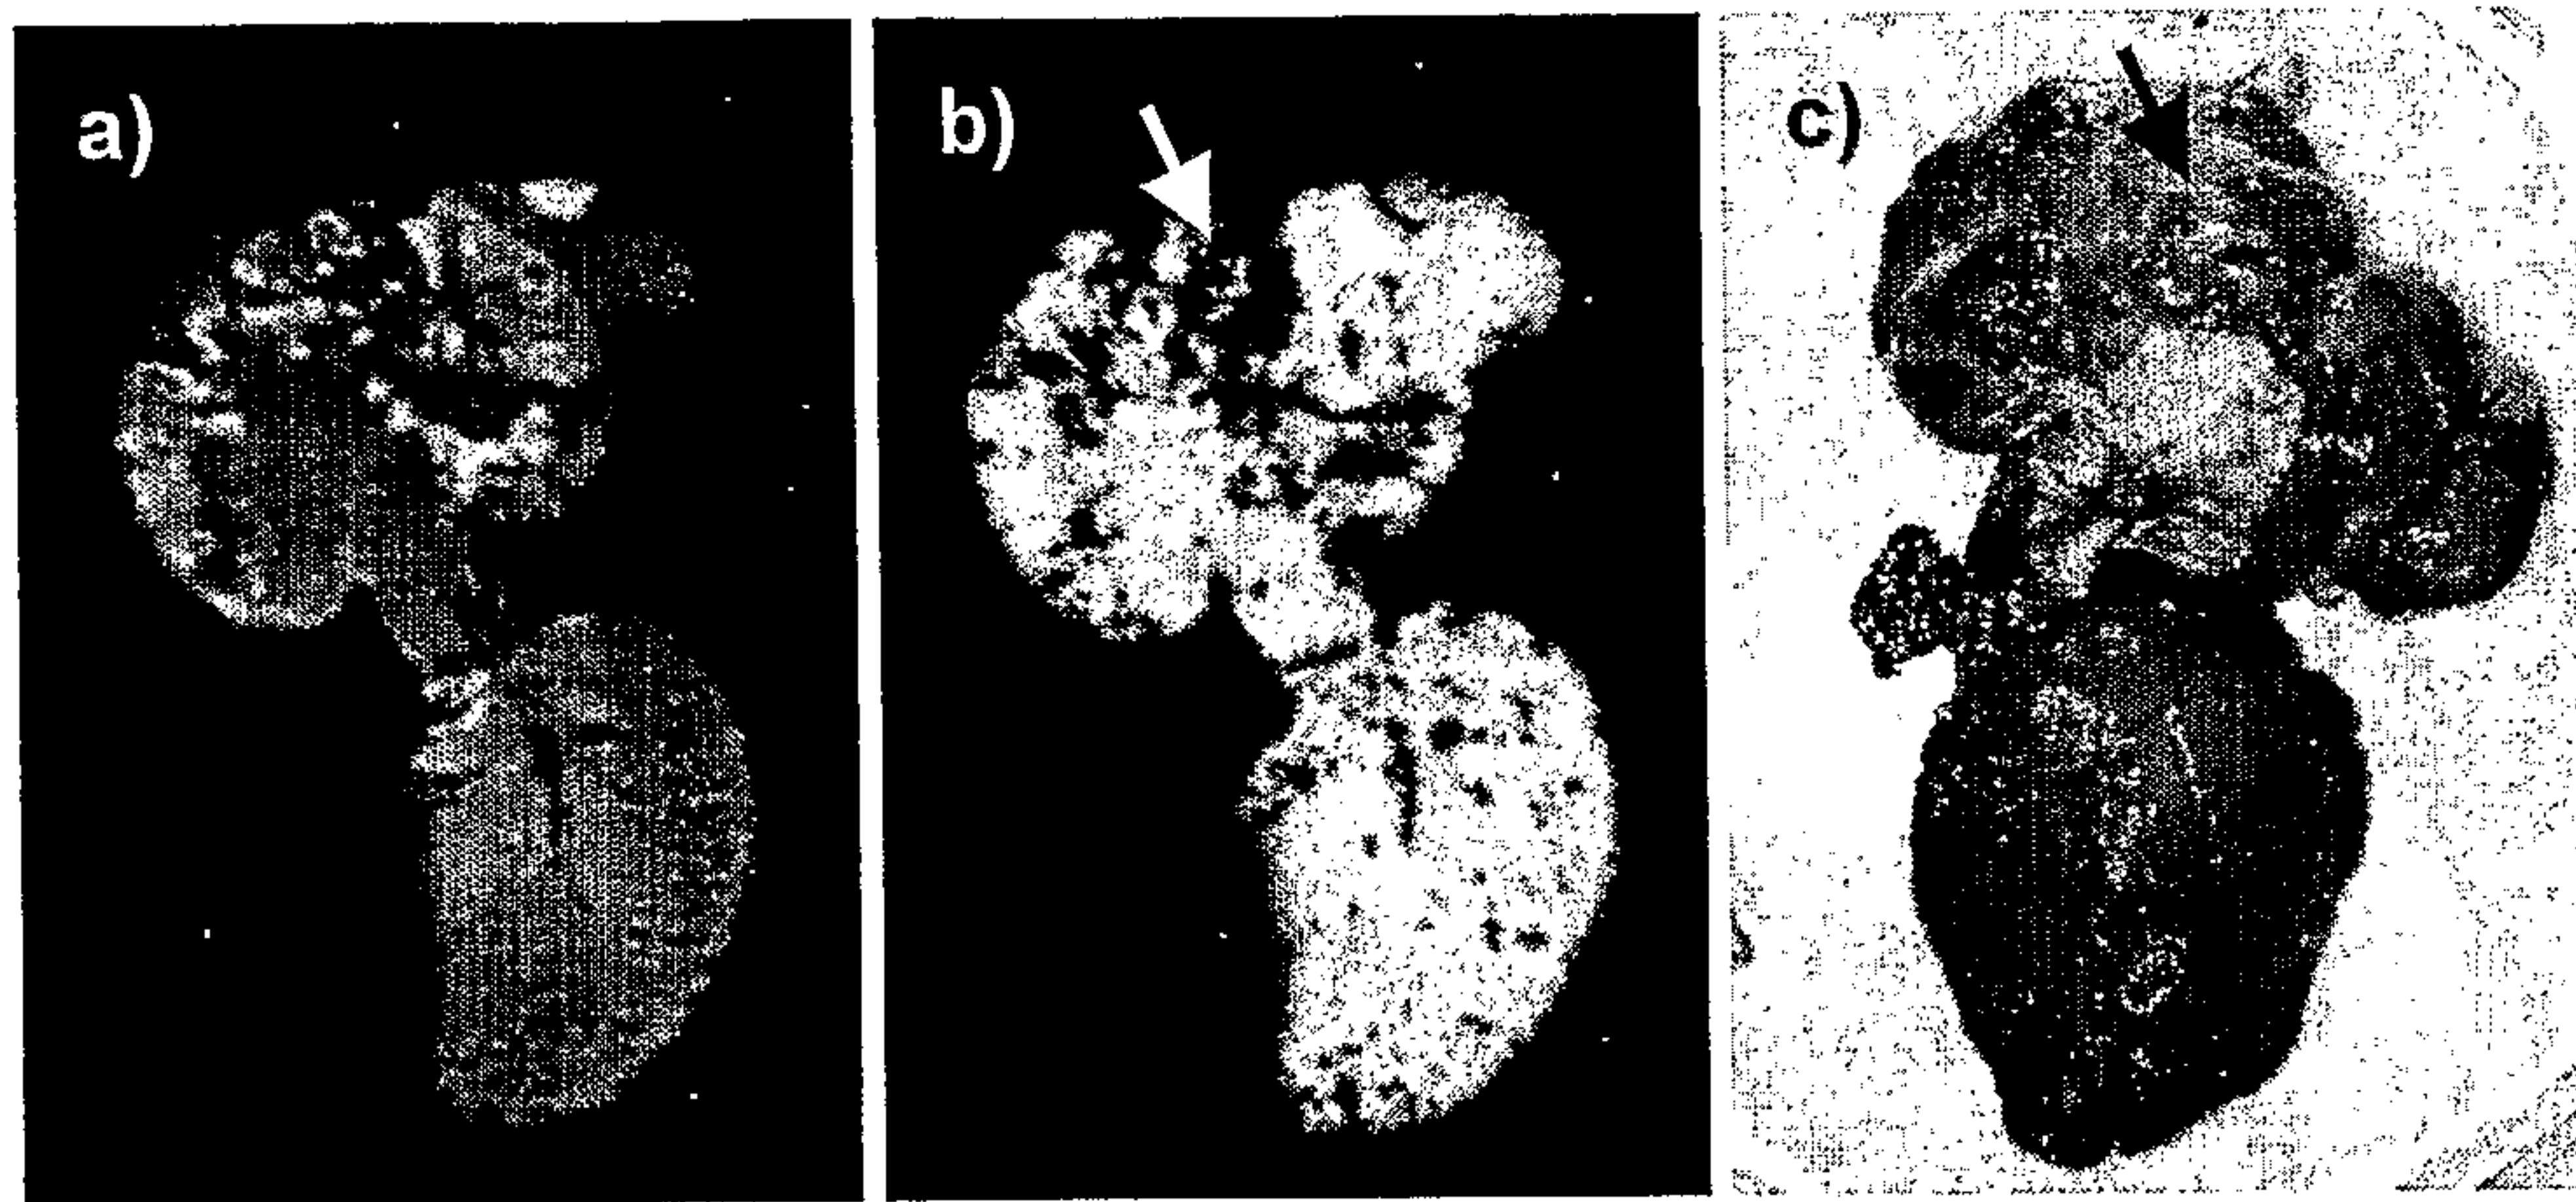
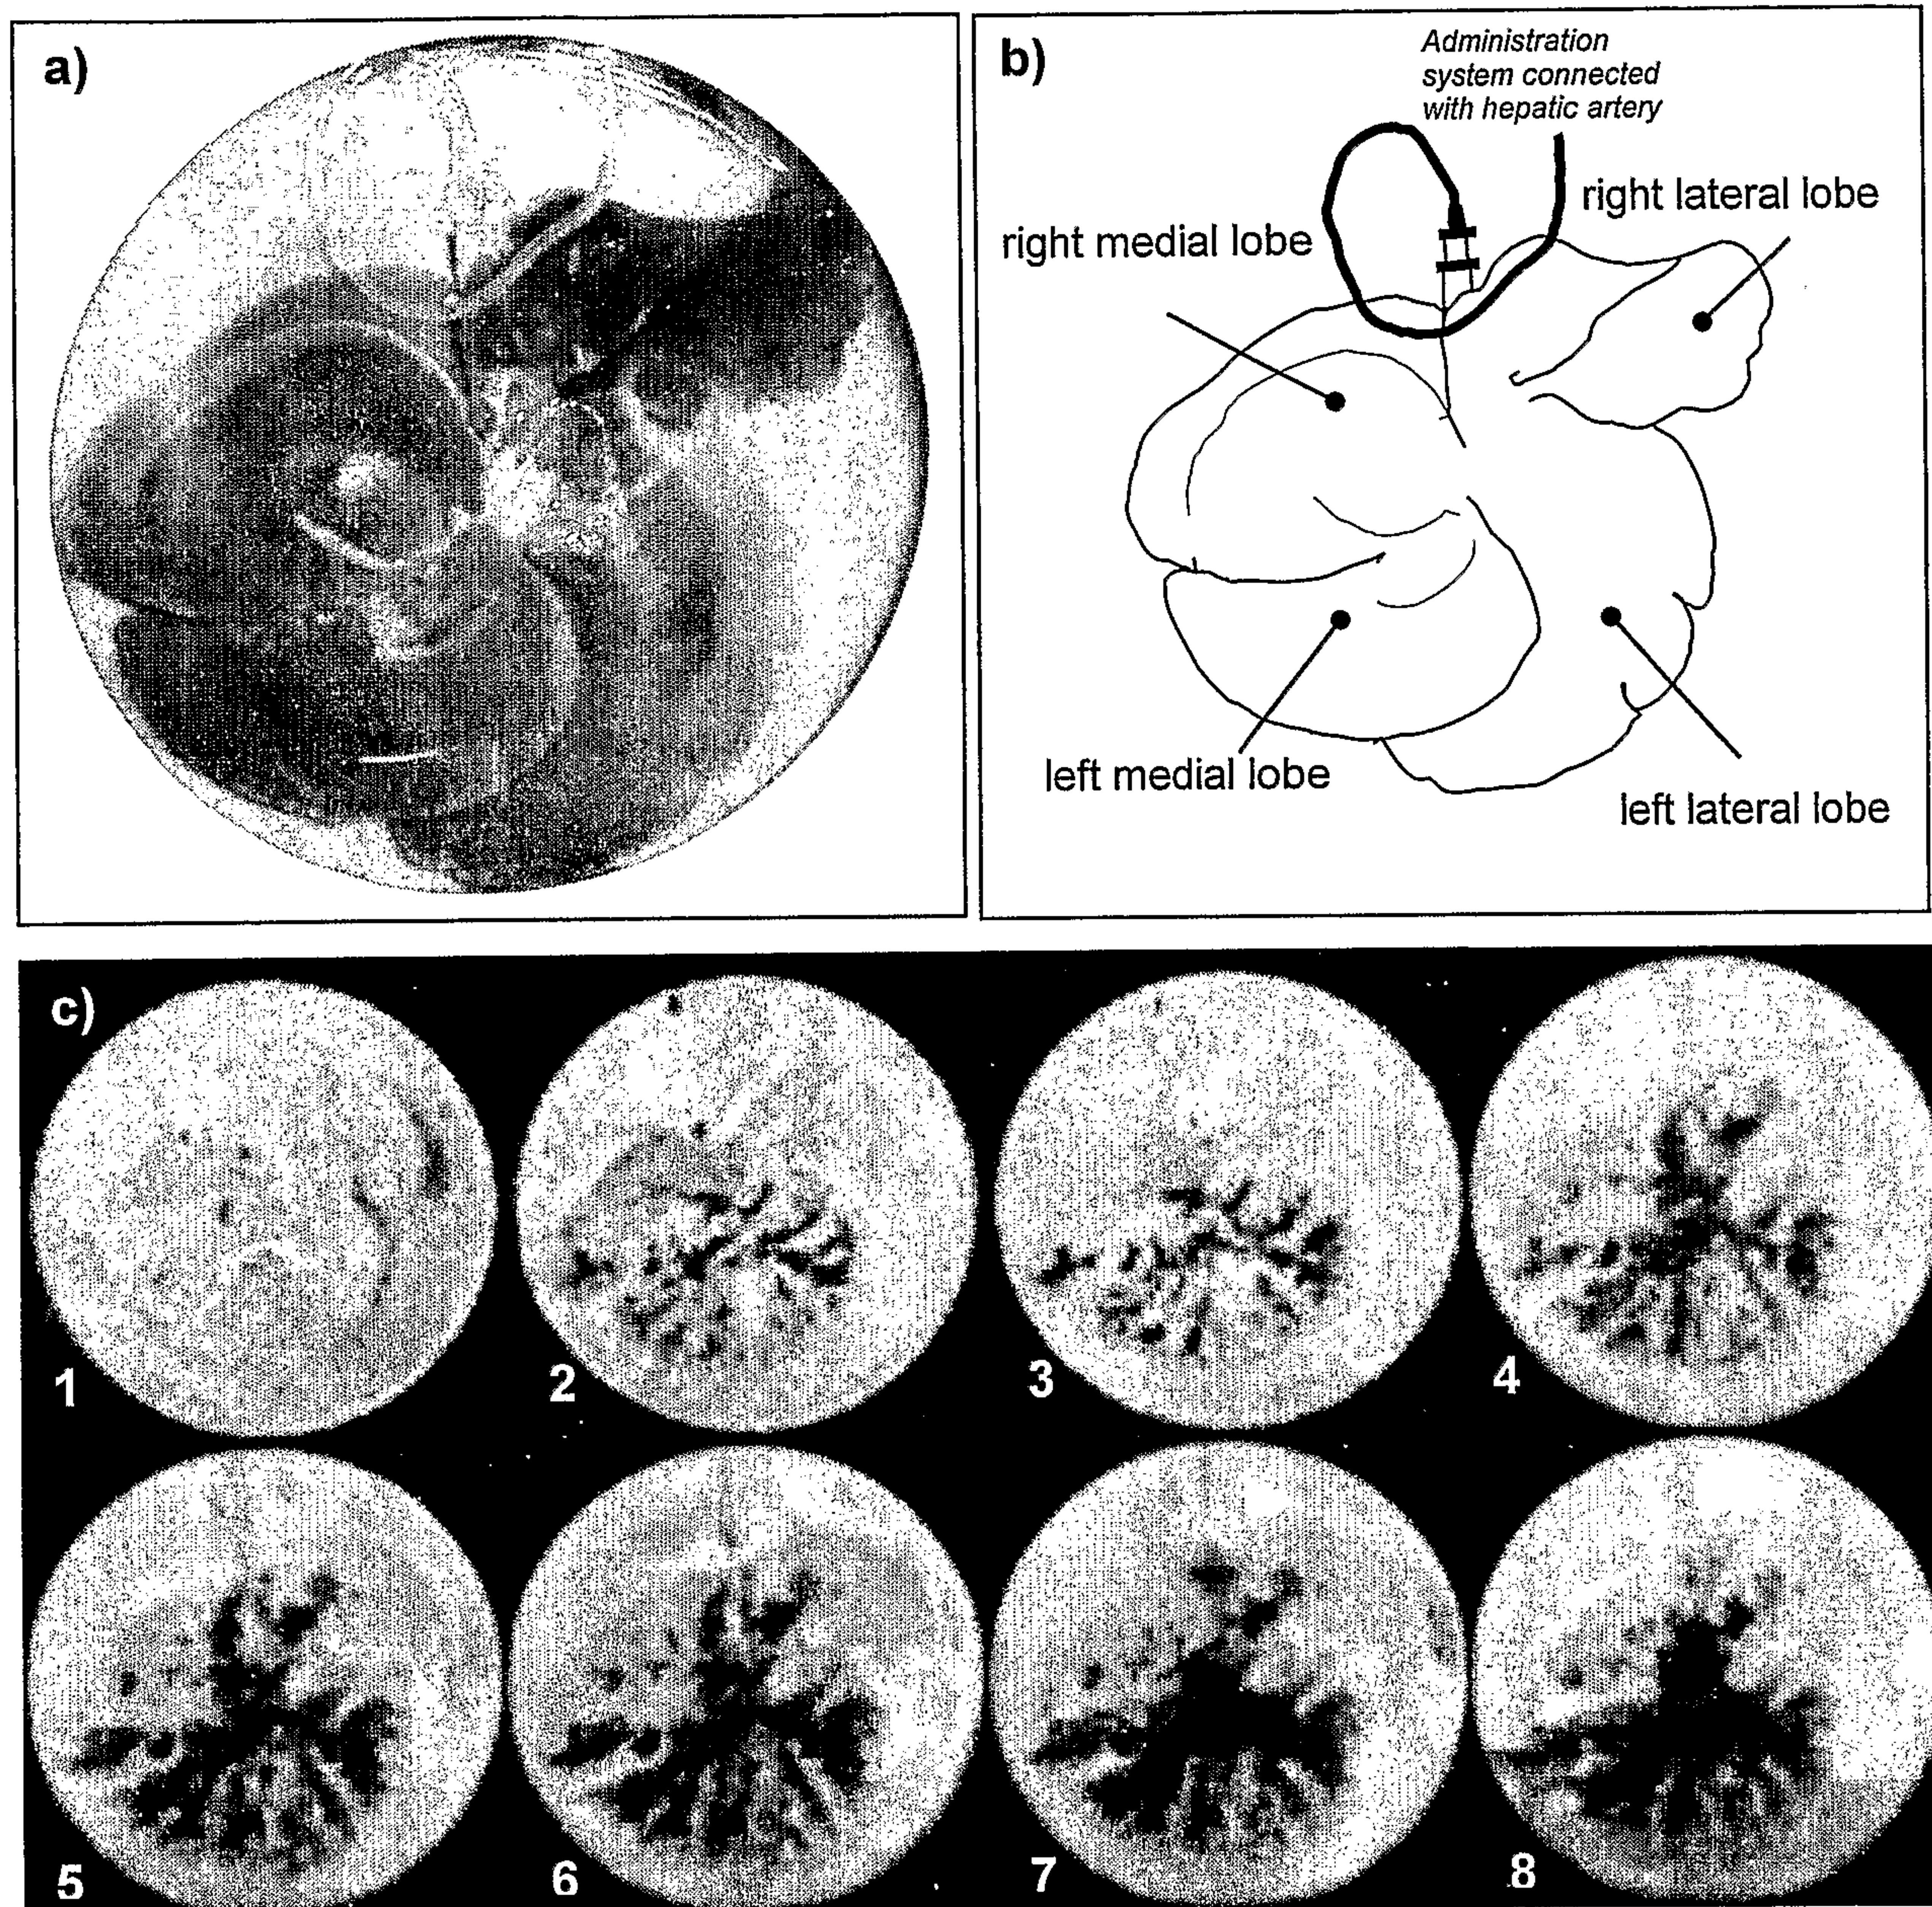


Figure 7a-c.

**Figure 8a-c.**

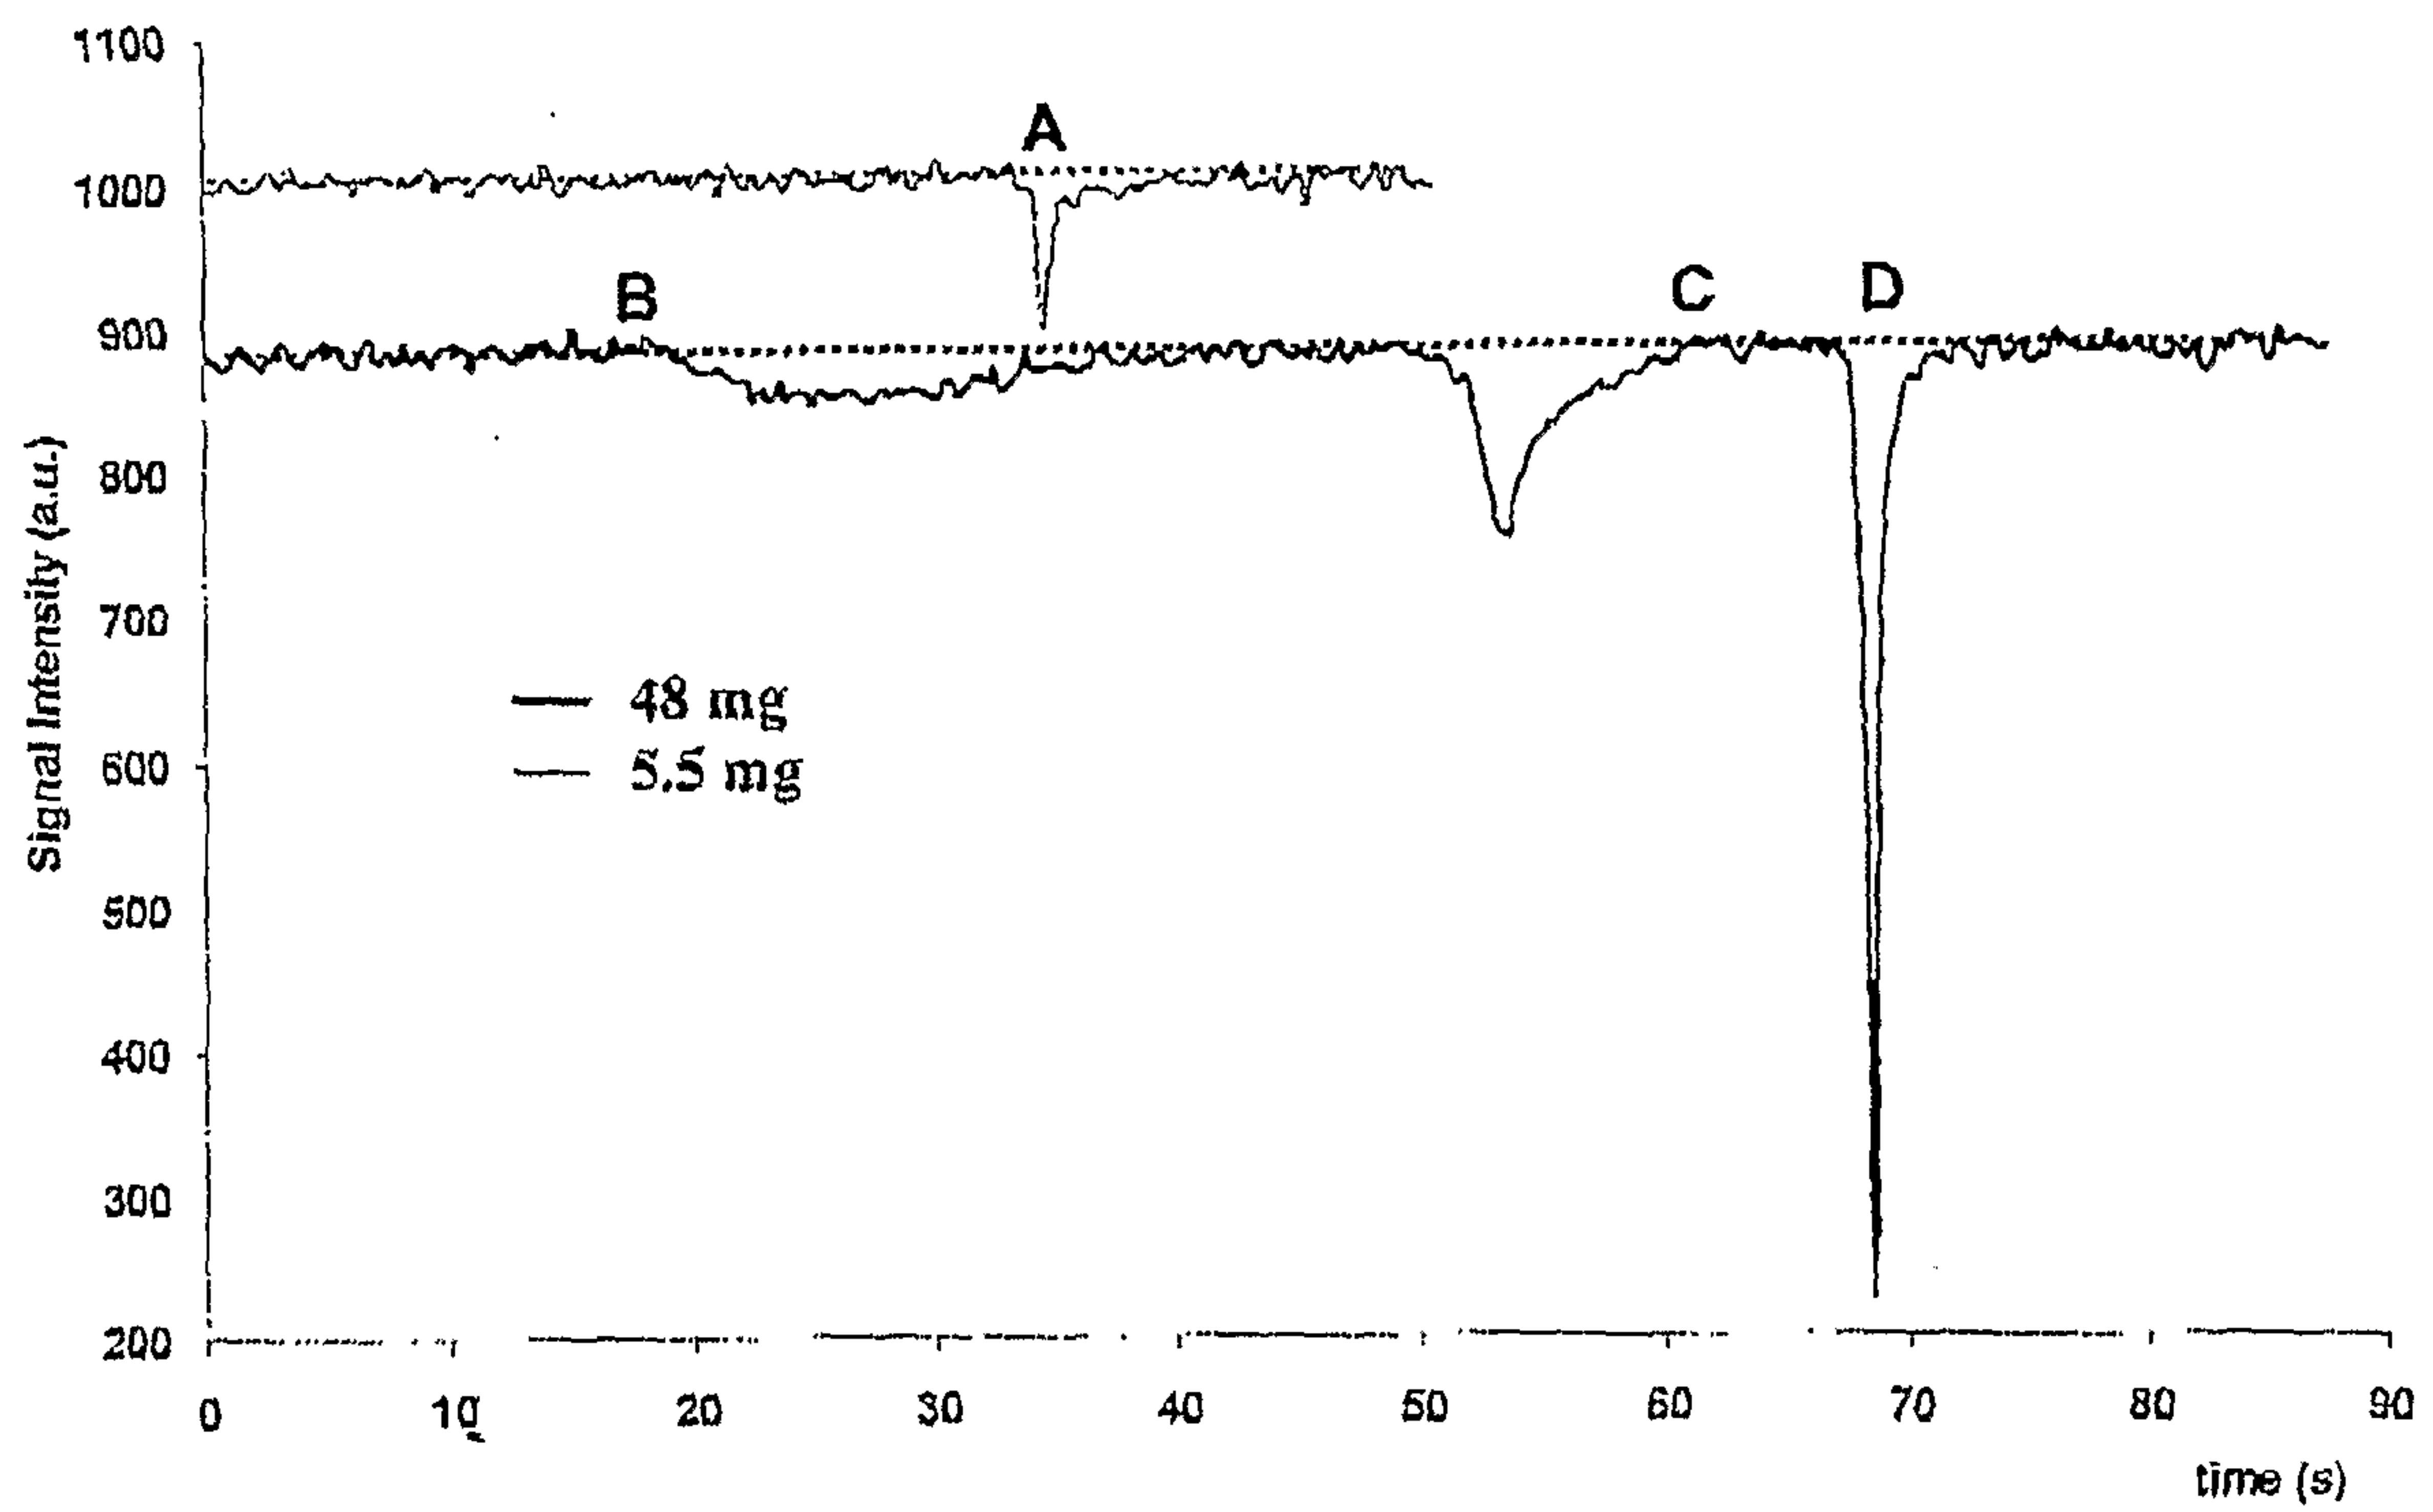


Figure 9.