



(19) **United States**

(12) **Patent Application Publication**

**Franck et al.**

(10) **Pub. No.: US 2001/0027271 A1**

(43) **Pub. Date: Oct. 4, 2001**

(54) **INSTRUMENT GUIDANCE FOR STEREOTACTIC SURGERY**

**Related U.S. Application Data**

(63) Continuation of application No. 09/063,658, filed on Apr. 21, 1998, now abandoned.

(76) Inventors: **Joel I. Franck**, Durham, ME (US); **Frederick C. Haer**, Brunswick, ME (US); **Ronald J. Franklin**, Bowdoinham, ME (US); **Kevin J. Frank**, Lafayette, CO (US); **John B. Clayton**, Superior, CO (US); **Jaimie Henderson**, St. Louis, MO (US); **Richard D. Bucholz**, St. Louis, MO (US); **Kurt R. Smith**, Eldorado Spring, CO (US); **Catalina J. Carroll**, Memphis, TN (US)

**Publication Classification**

(51) **Int. Cl.<sup>7</sup>** ..... **A61B 6/00**  
(52) **U.S. Cl.** ..... **600/426; 606/130**

**ABSTRACT**


A method and apparatus for positioning a surgical instrument during stereotactic surgery using a guidance fixture. The guidance fixture includes an upper portion, which includes an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion, and includes an adjustable base supporting the upper portion, which includes a mounting base and an adjustment mechanism. The adjustable base can include a rotating collar attached to the mounting base and a pivoting collar coupling the rotating collar to the upper portion. A remote sensing device, such as a camera array sensing LEDs on the fixture, is used to determine the orientation of the upper portion of the guidance assembly in relation to the body.


Correspondence Address:

**G. ROGER LEE**  
**Fish & Richardson P.C.**  
**225 Franklin Street**  
**Boston, MA 02110-2804 (US)**

(21) Appl. No.: **09/846,640**


(22) Filed: **May 1, 2001**

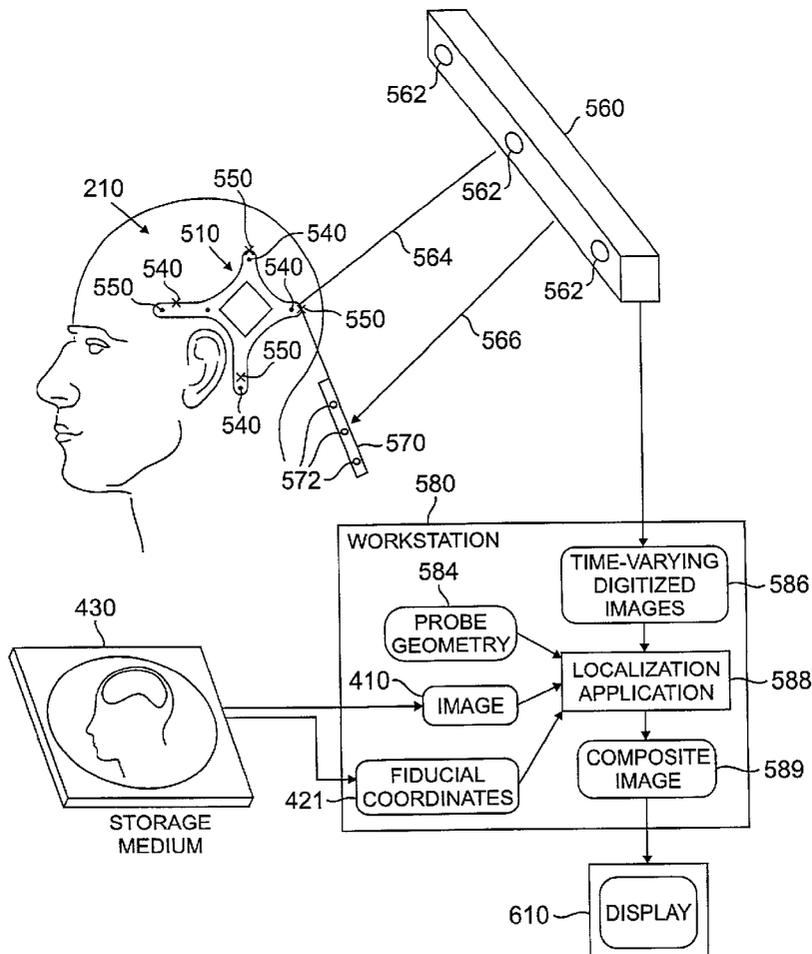

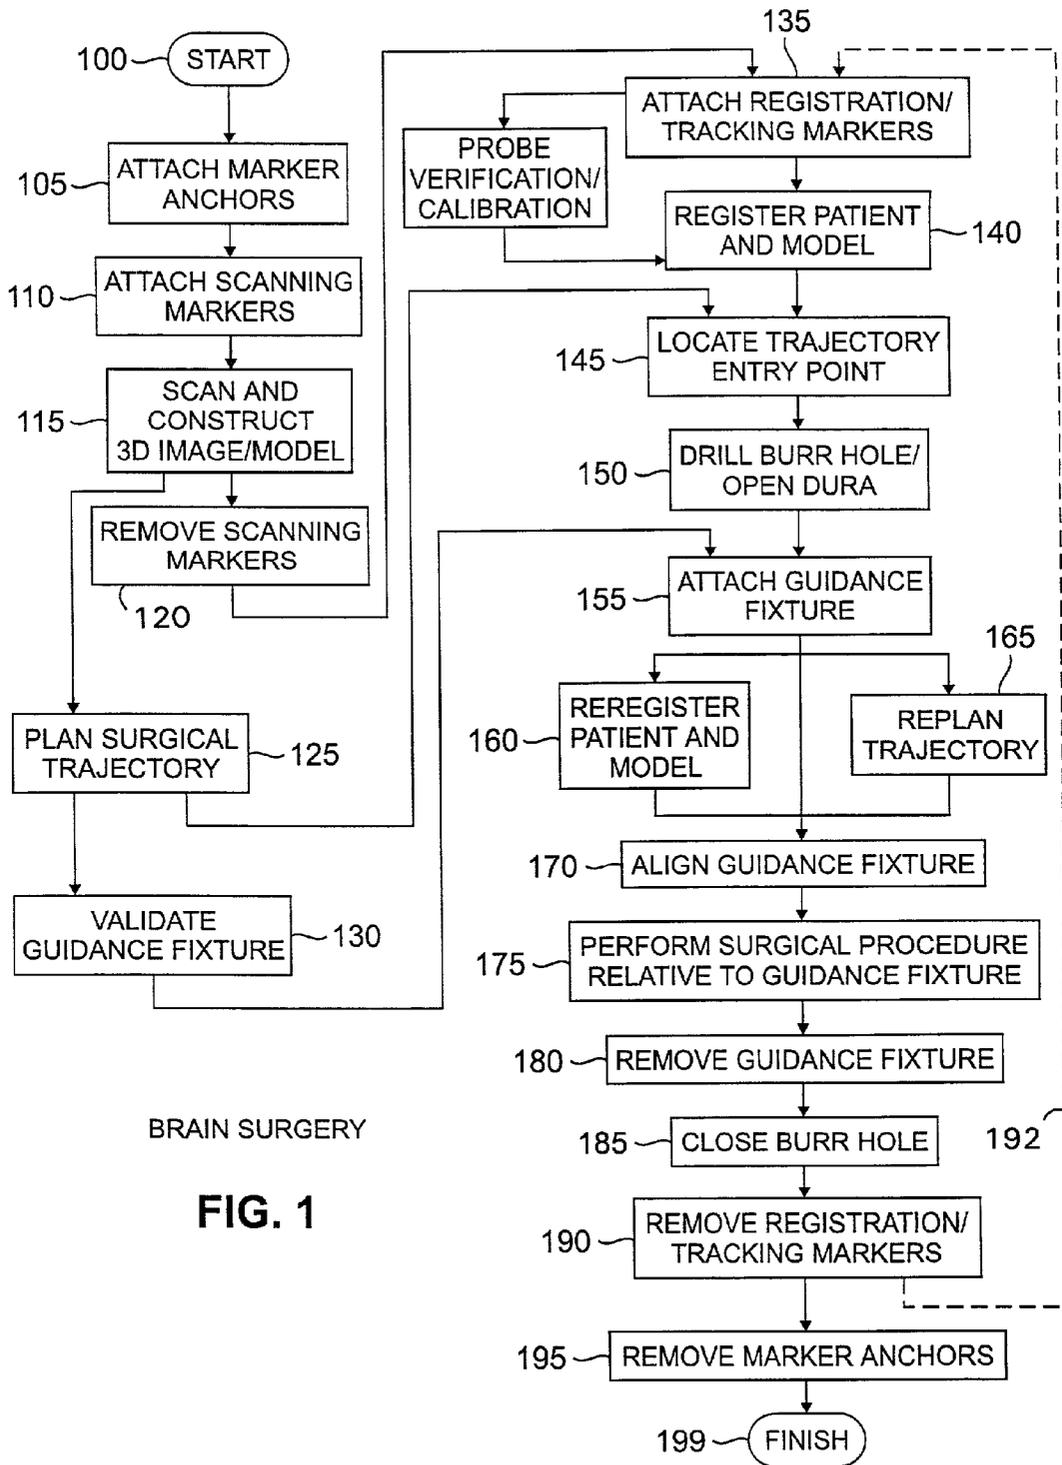

BRAIN SURGERY

FIG. 1

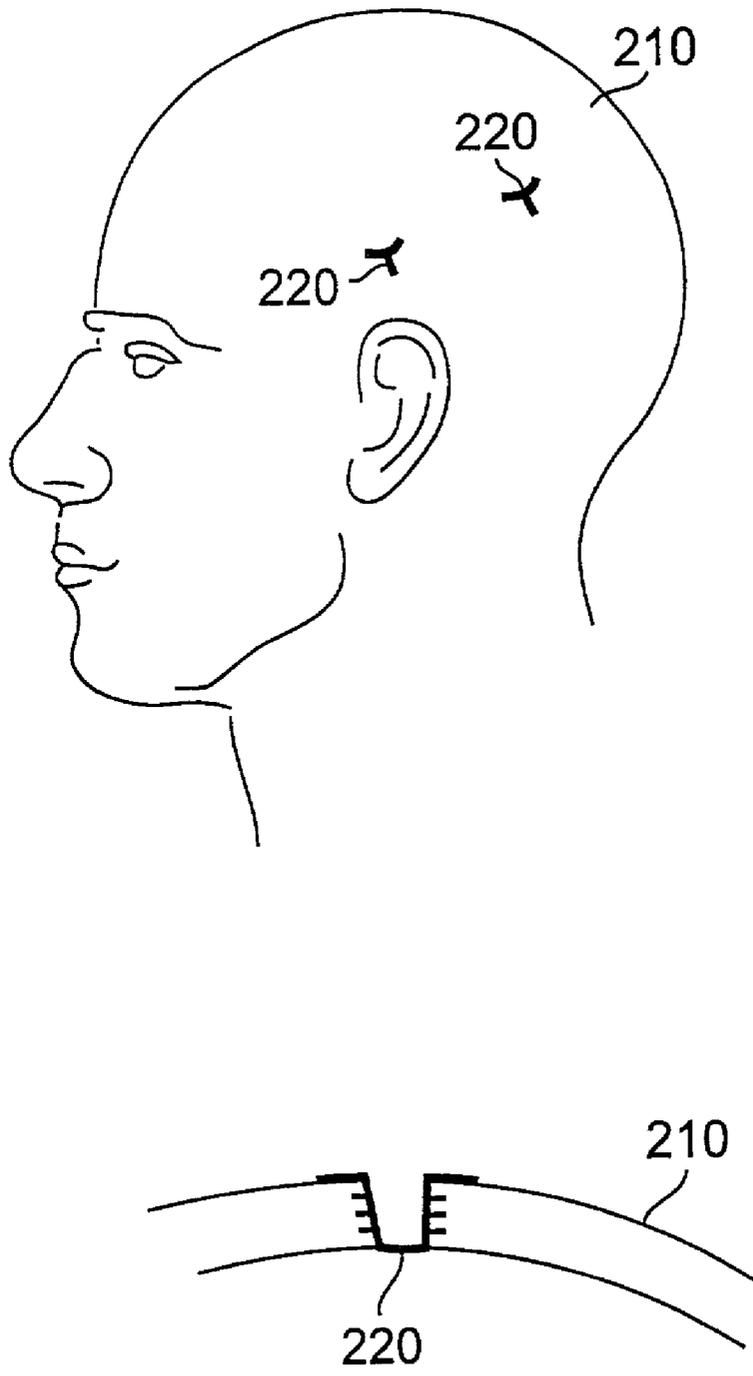

**FIG. 2**

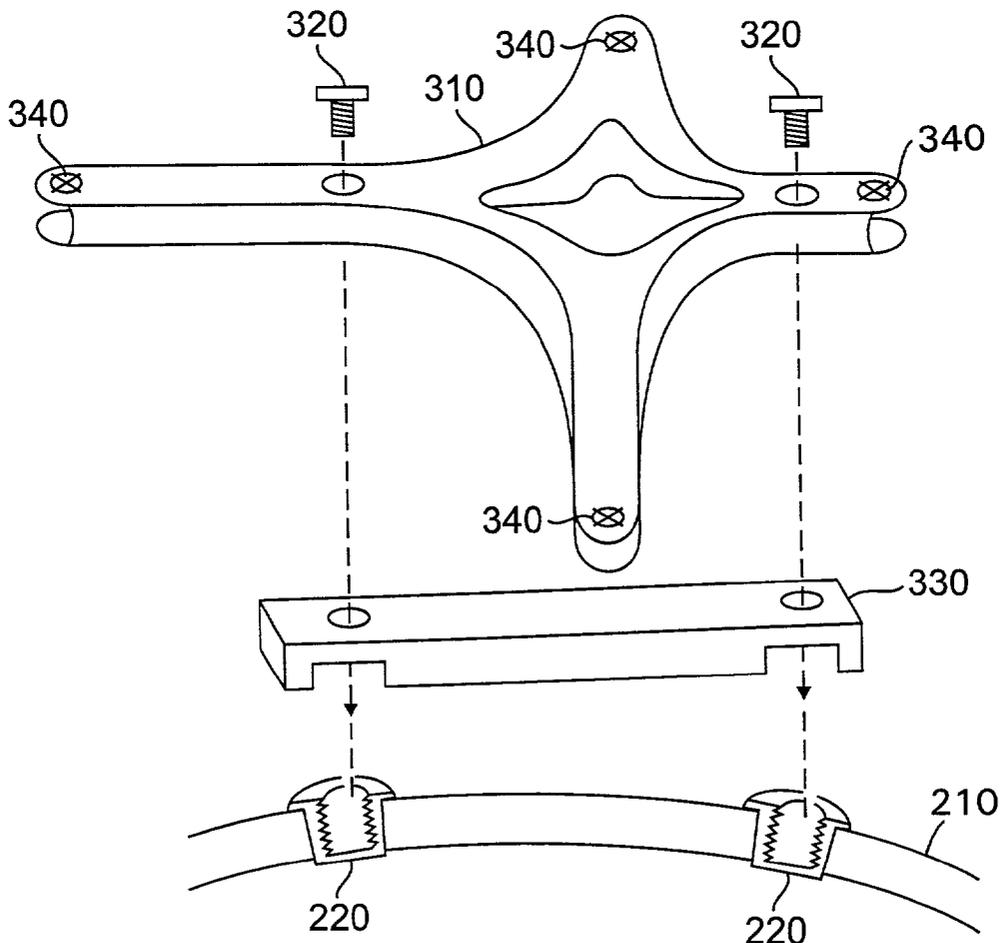
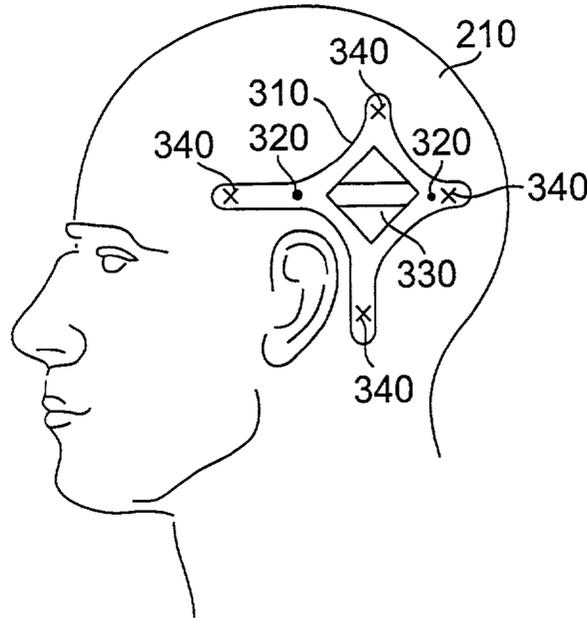


FIG. 3

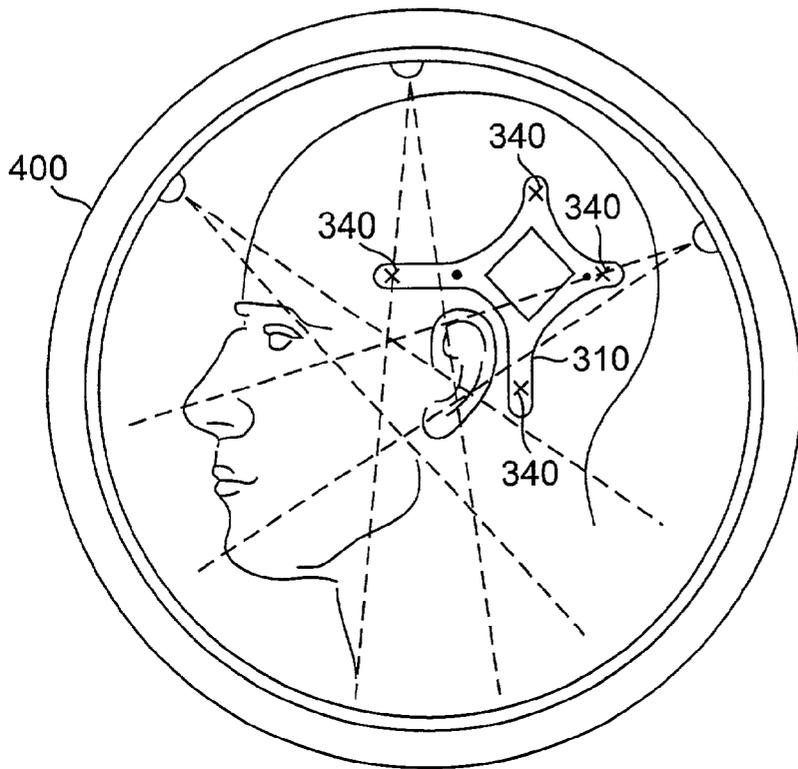
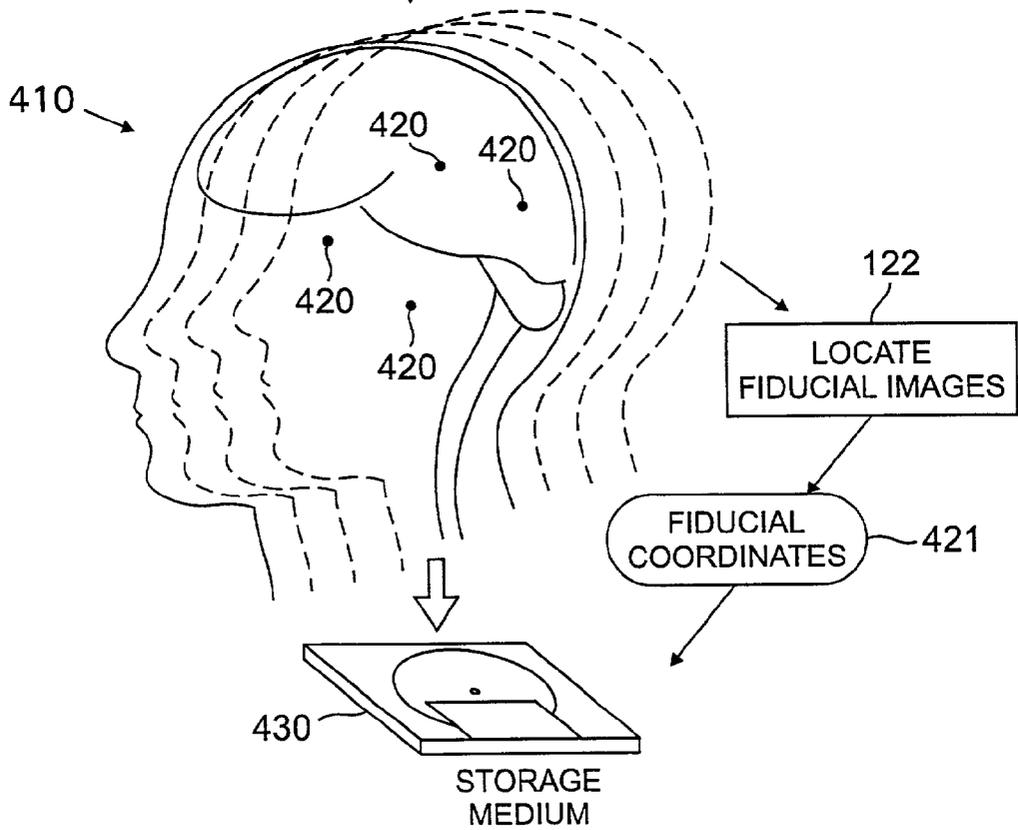


FIG. 4



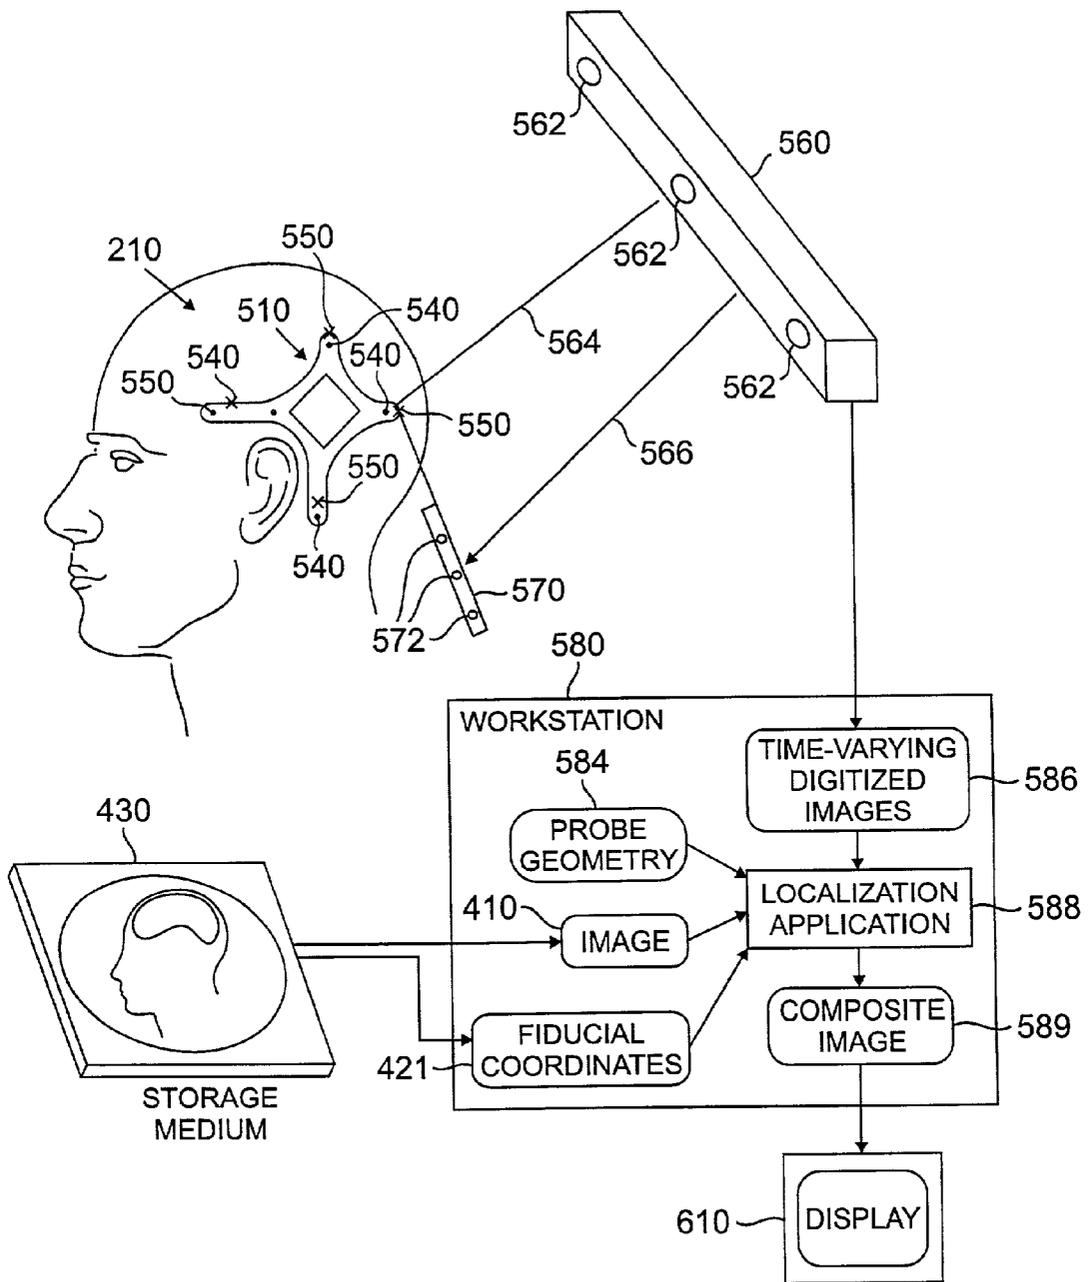


FIG. 5

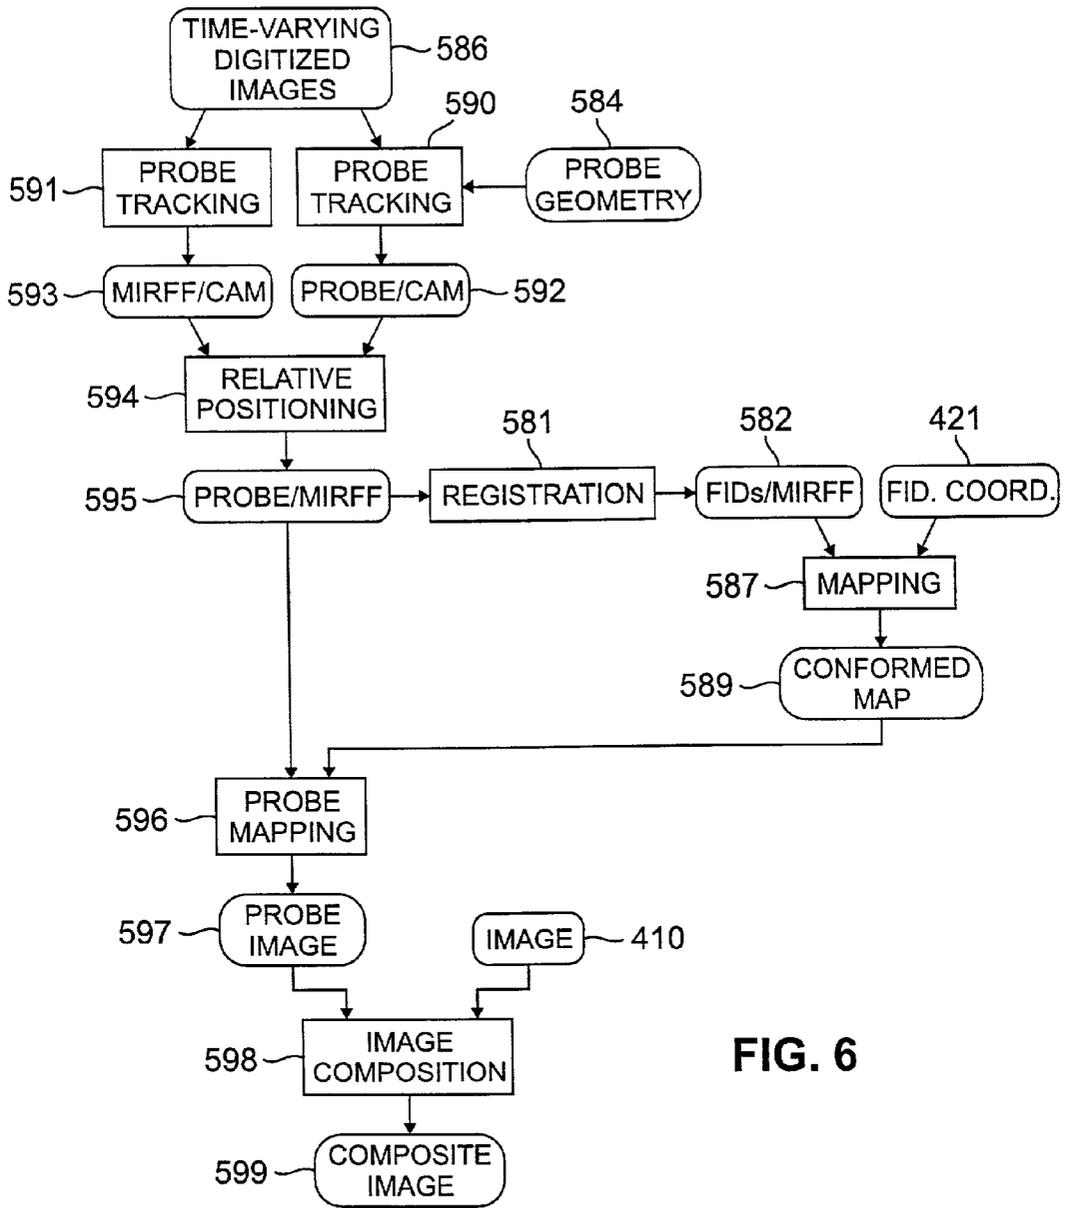


FIG. 6


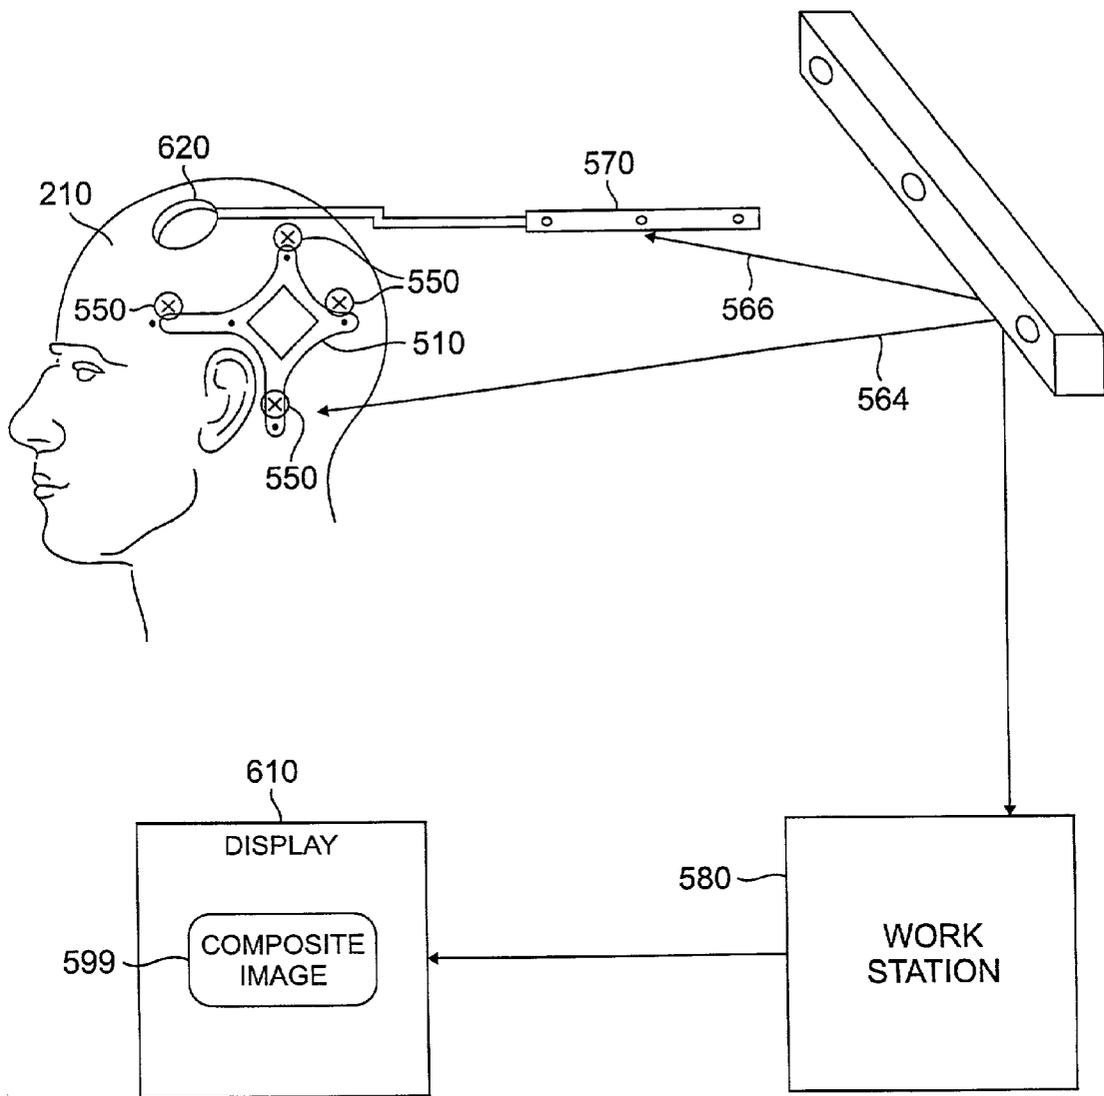


FIG. 7

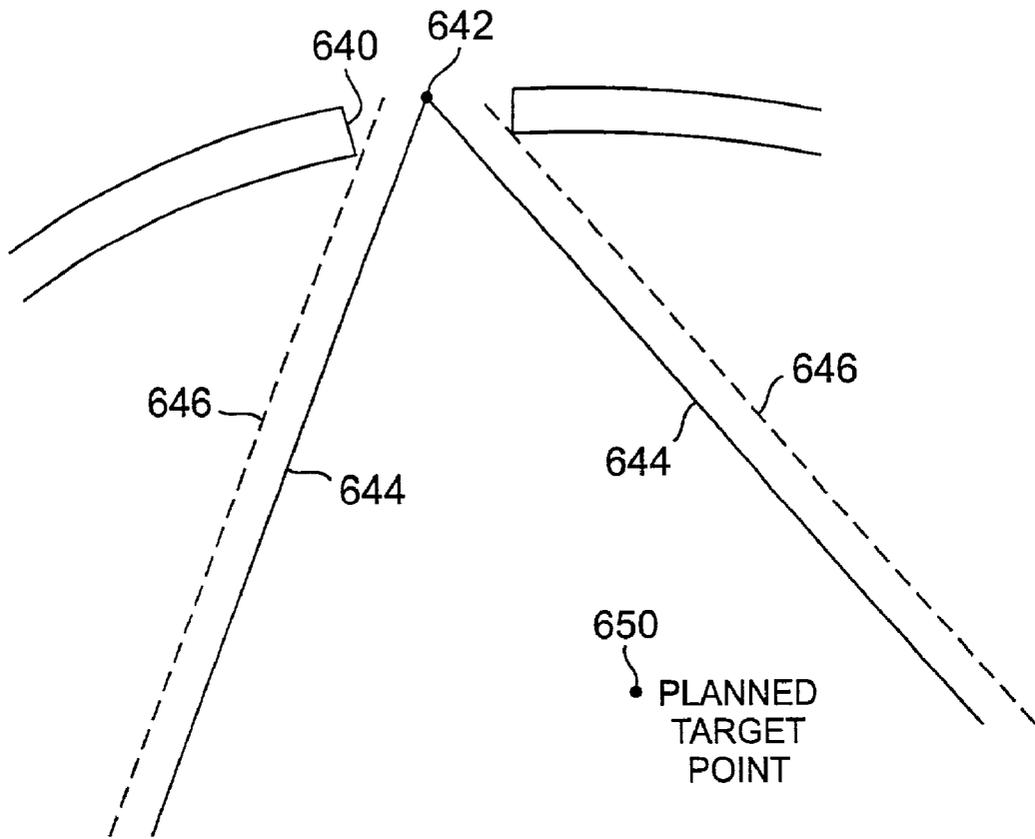

**FIG. 8**

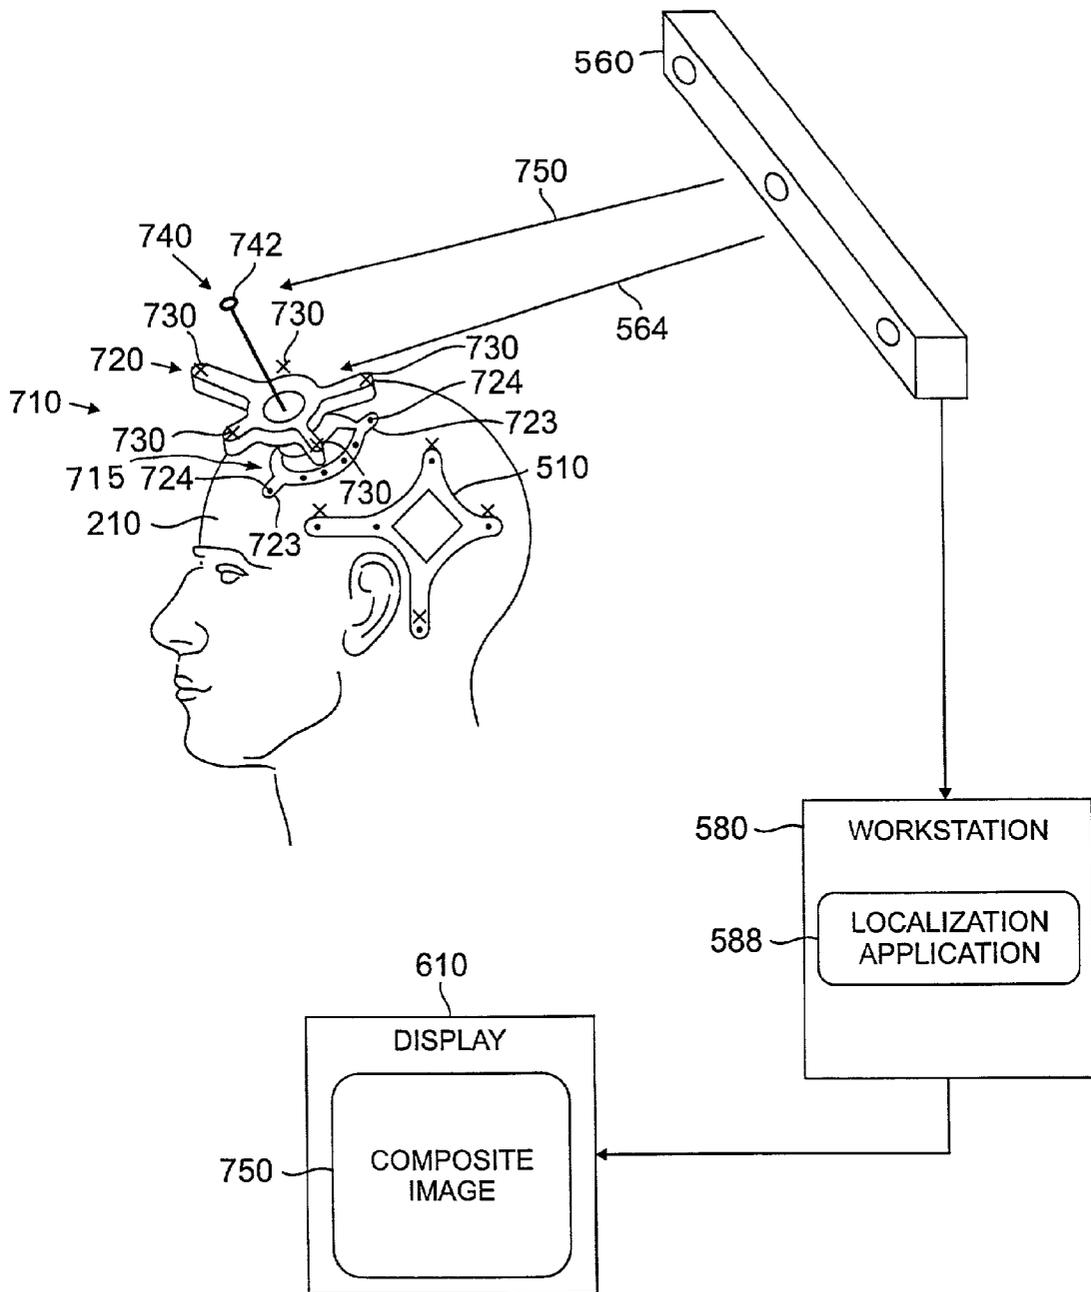


FIG. 9

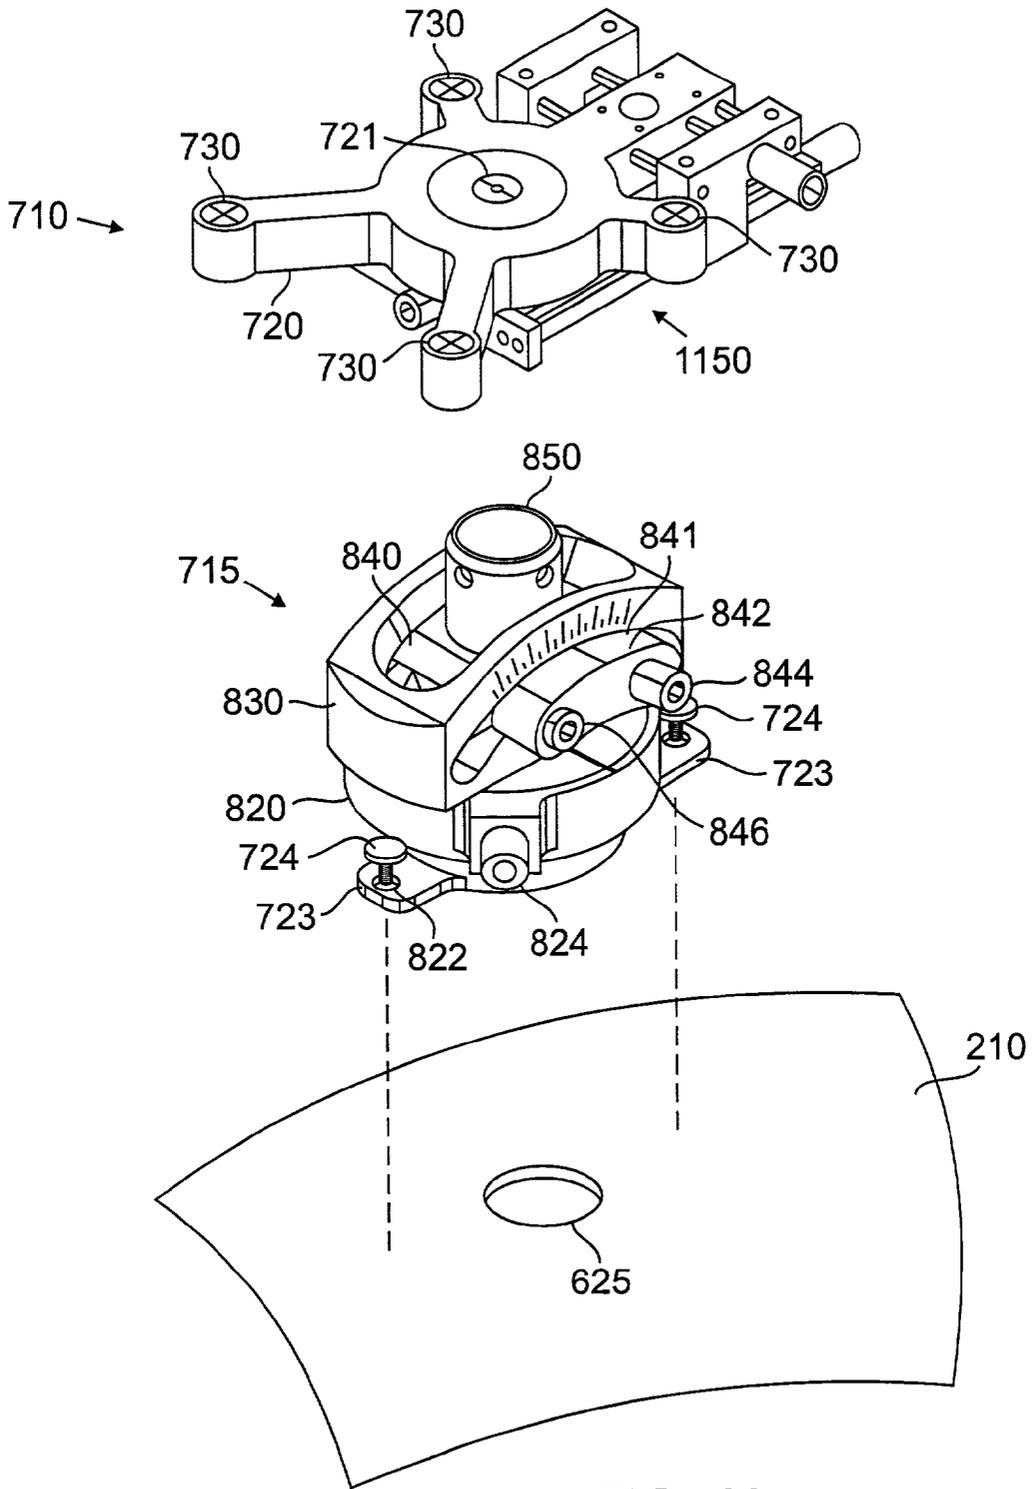


FIG. 10

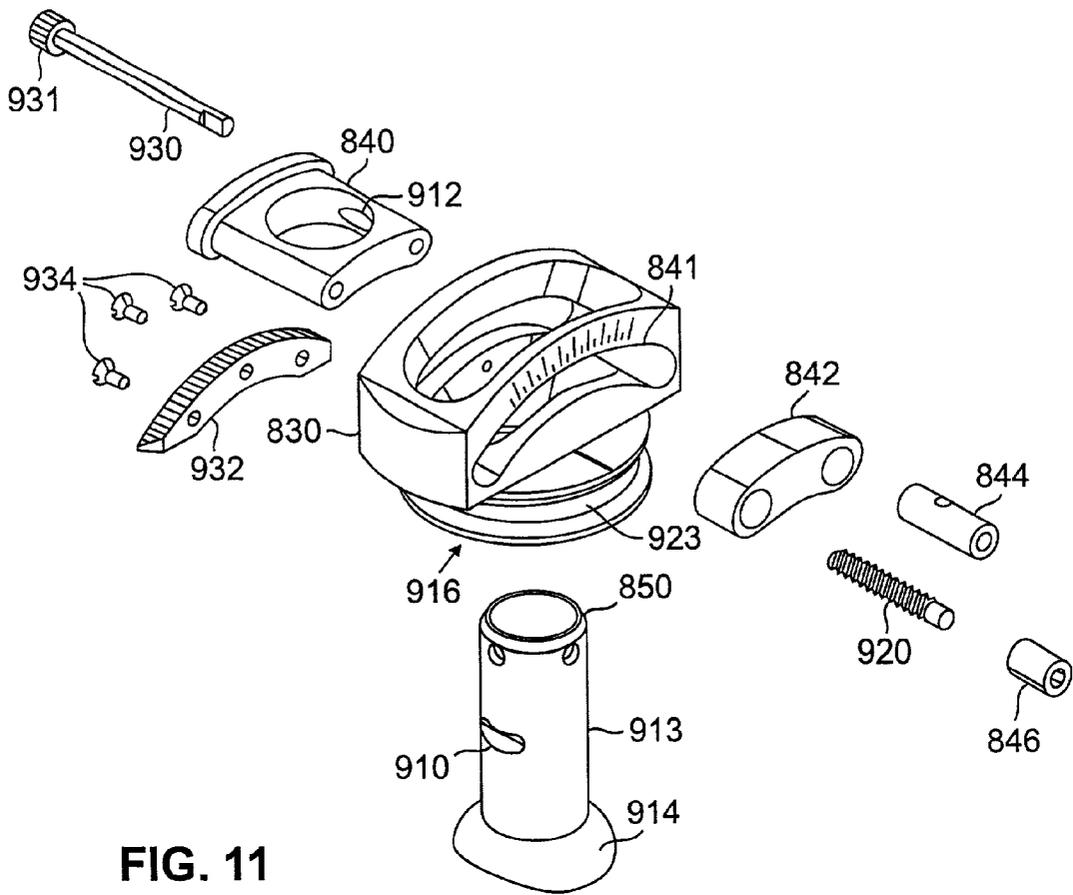
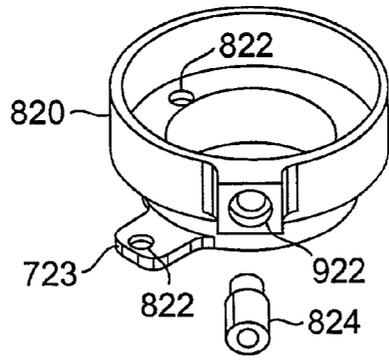


FIG. 11




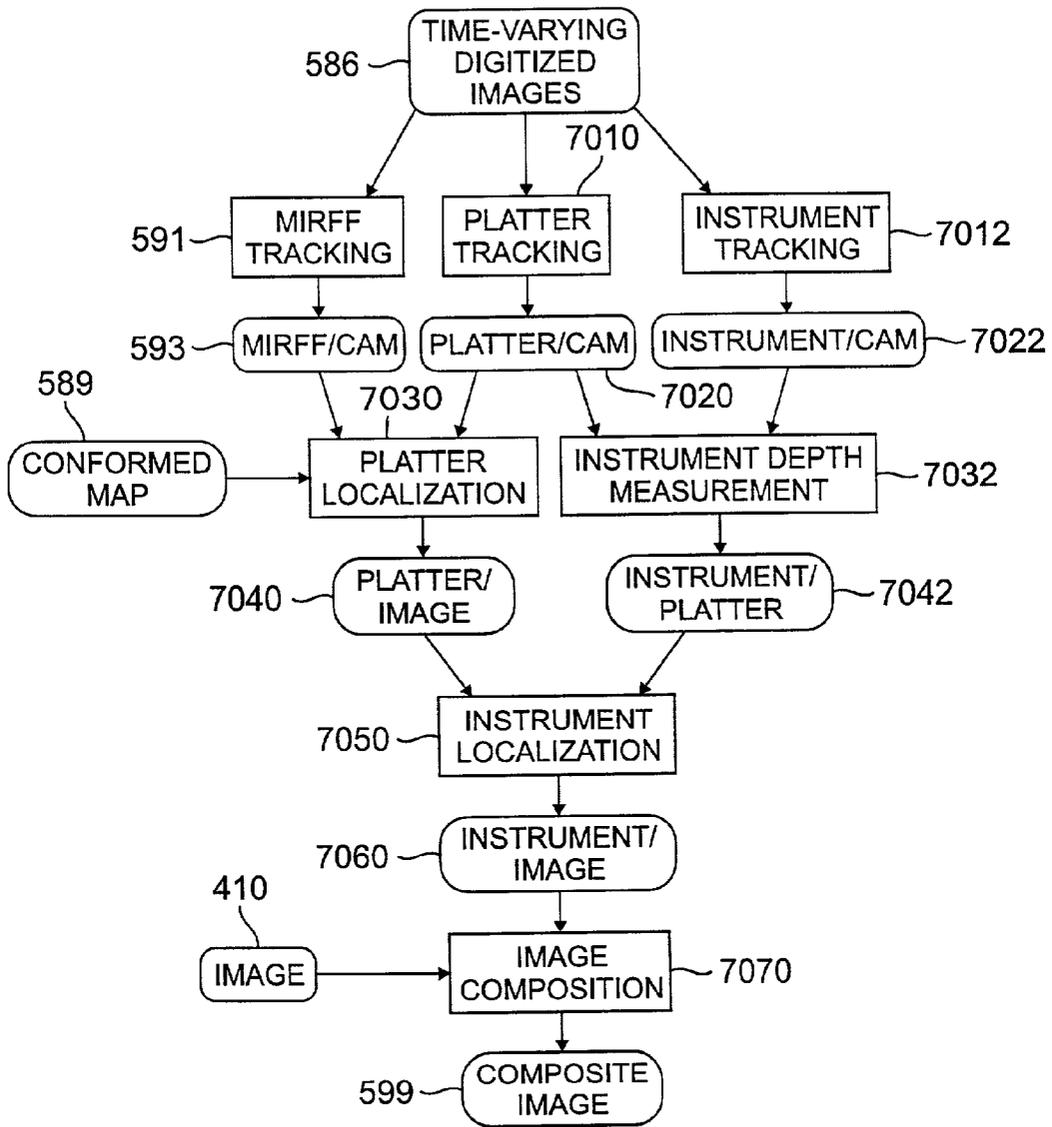


FIG. 12

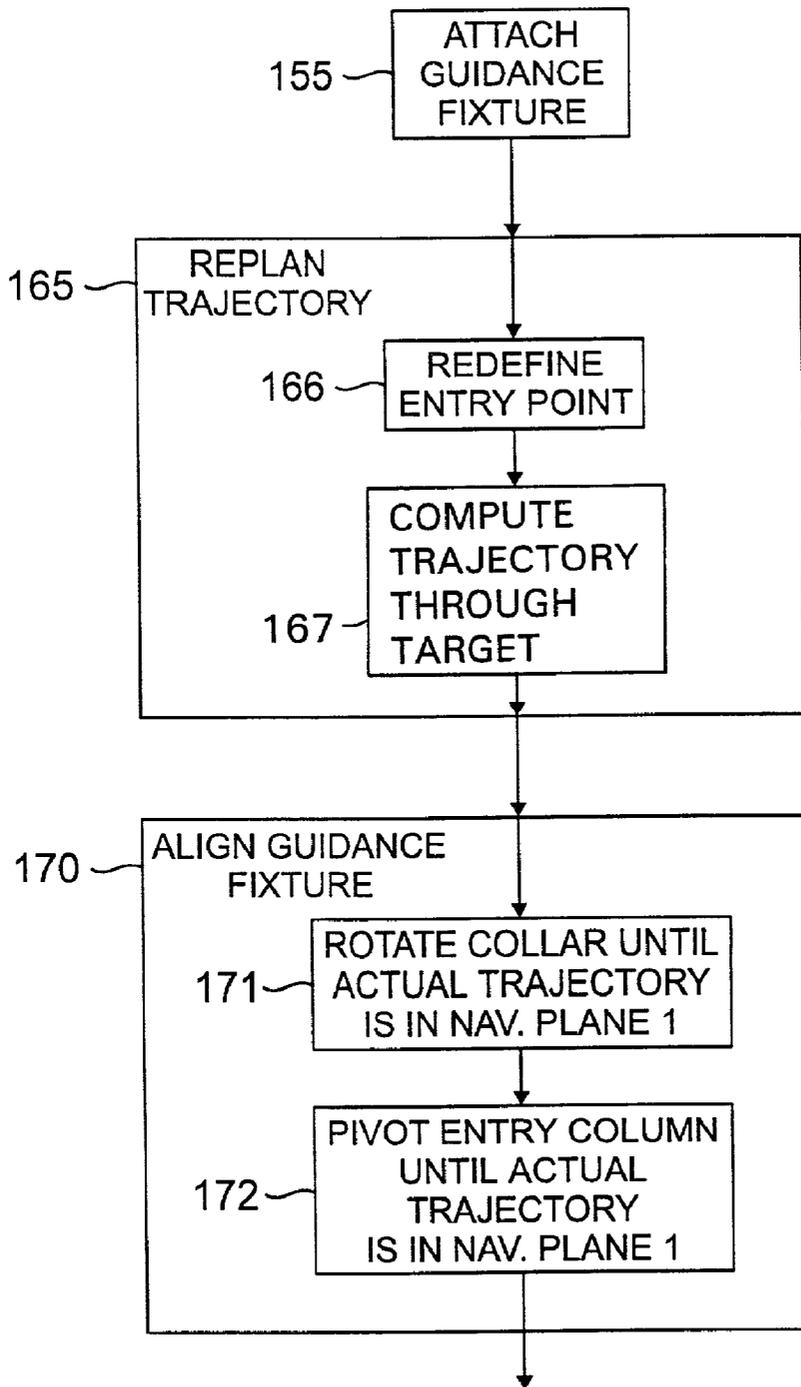

**FIG. 13**

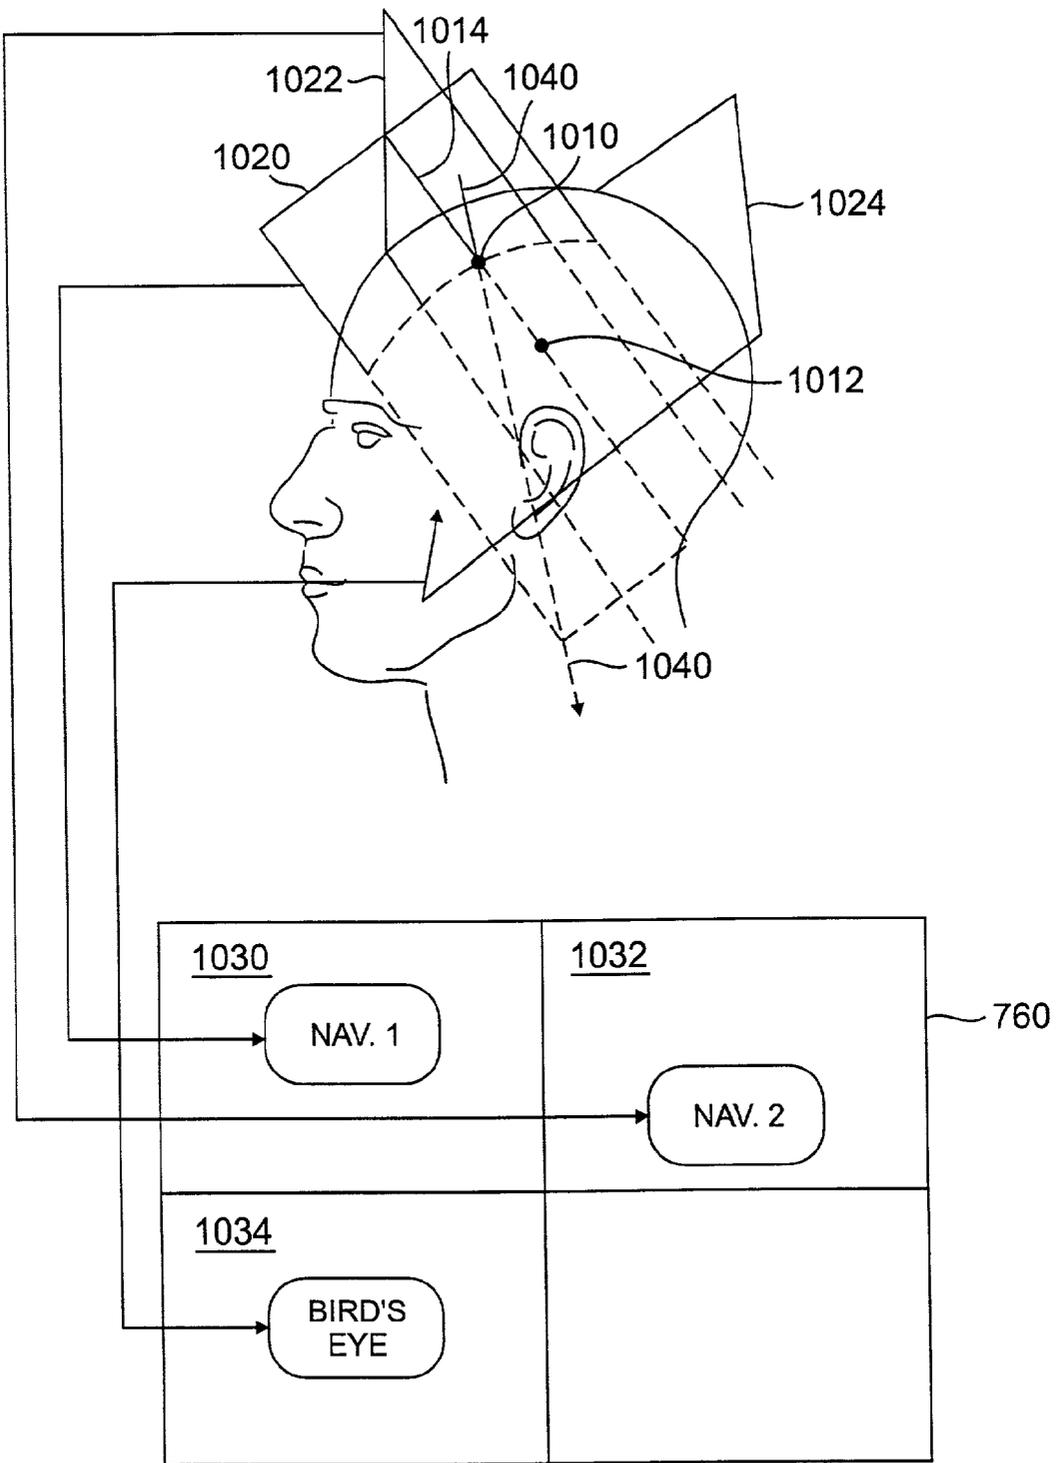


FIG. 14a

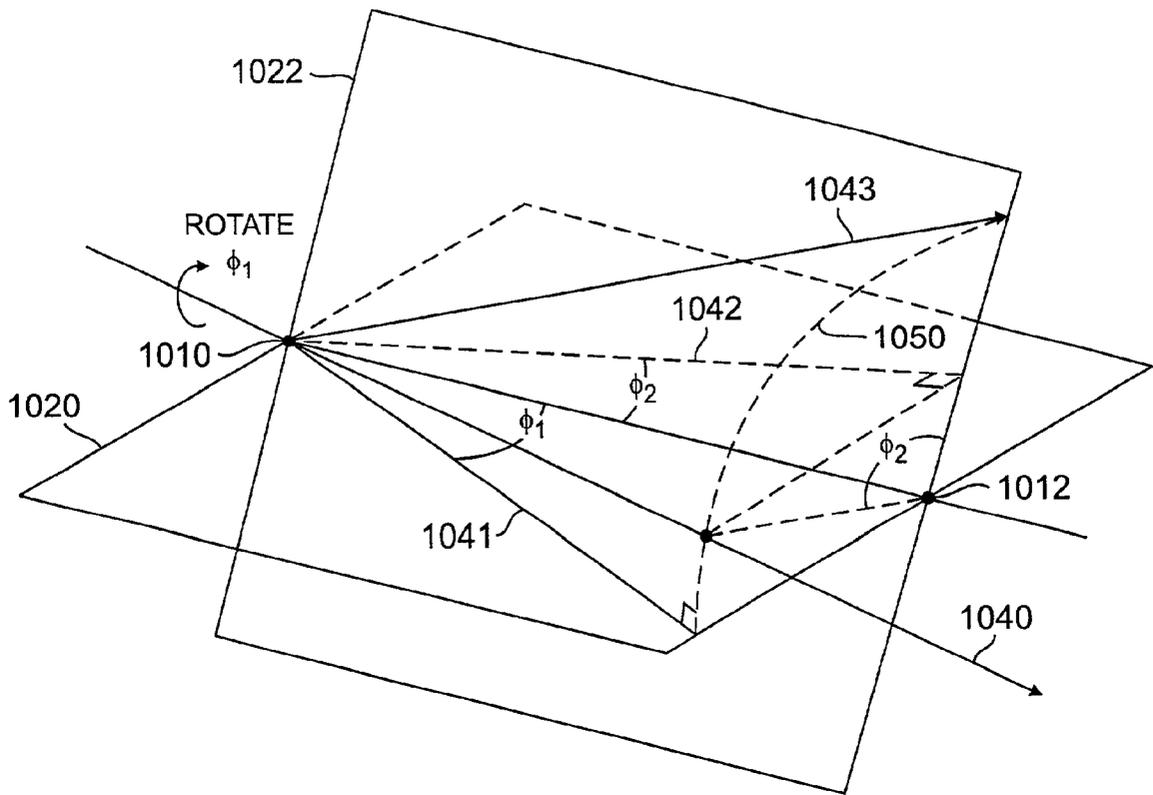


FIG. 14b









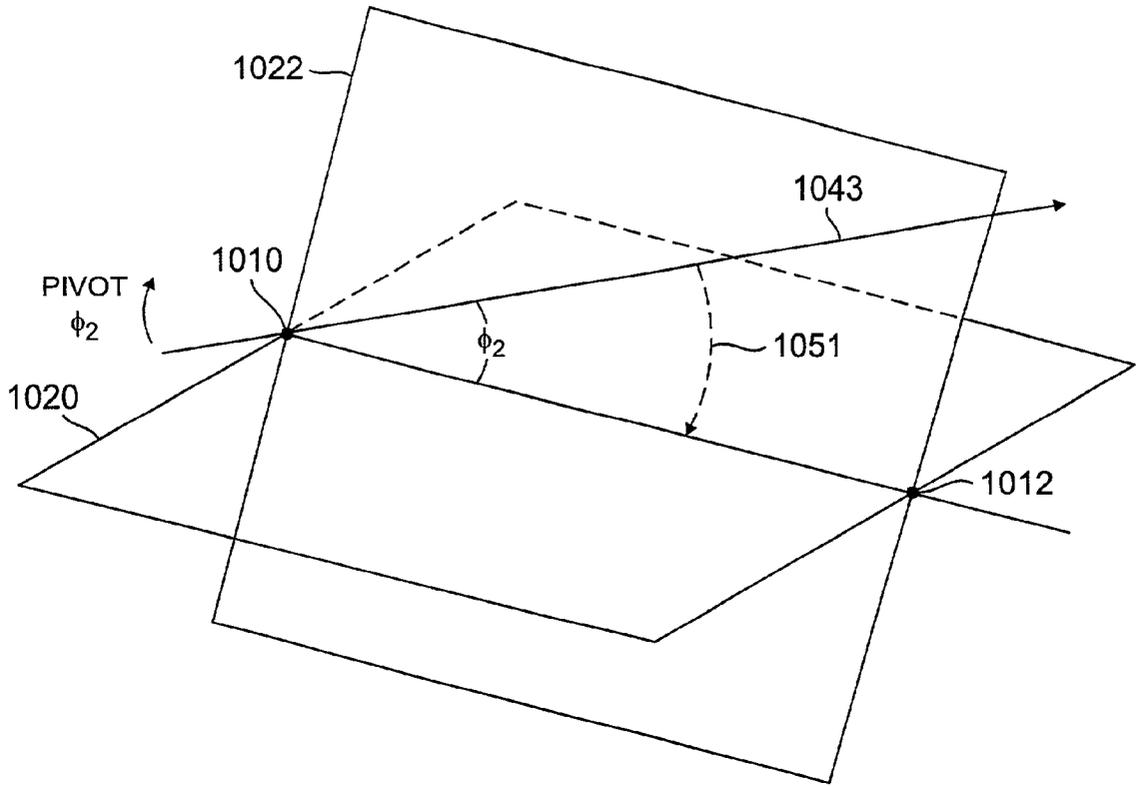


FIG. 14c

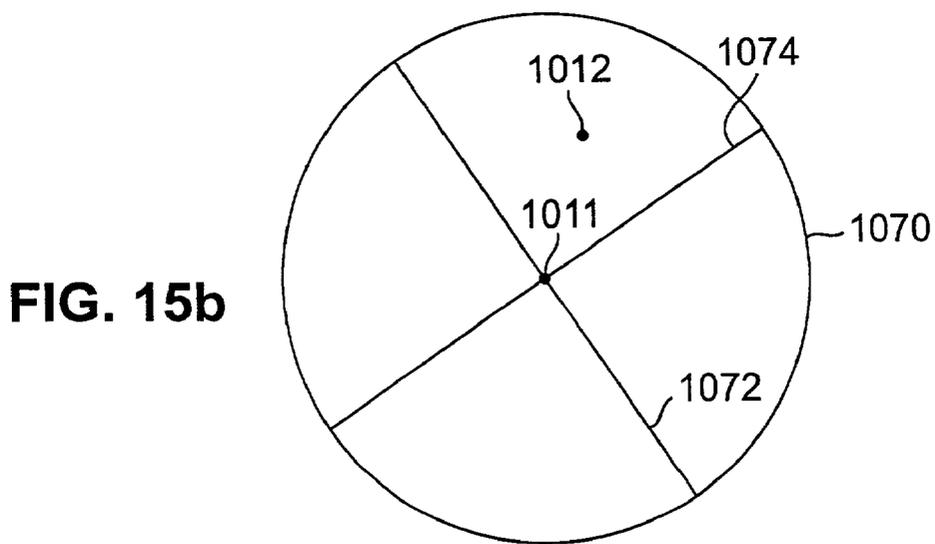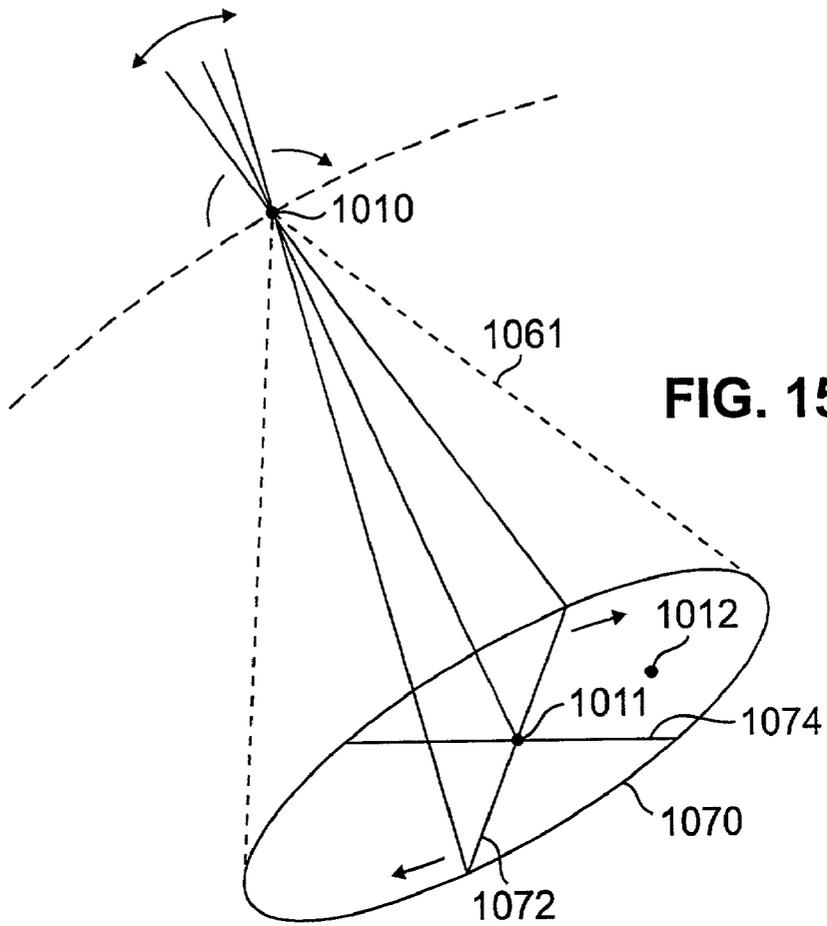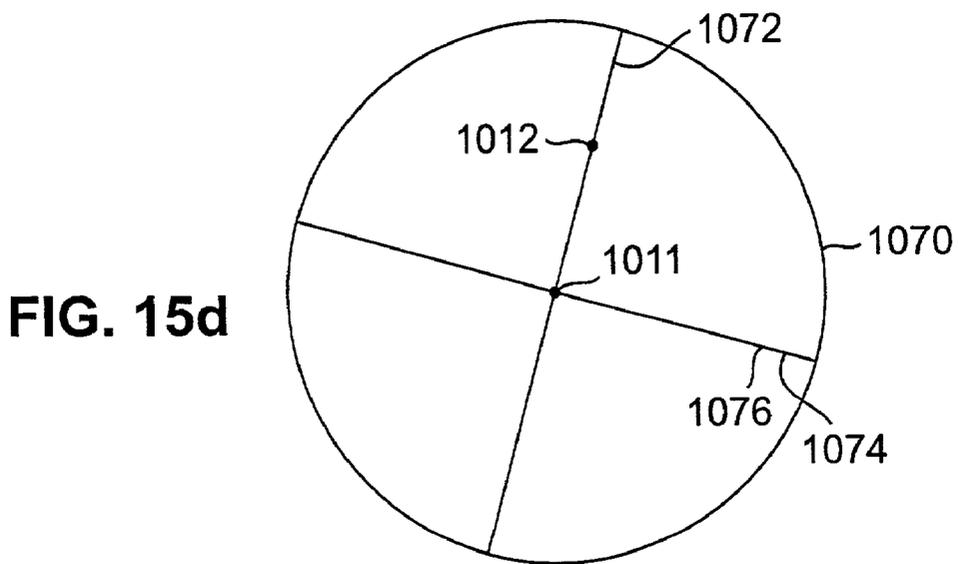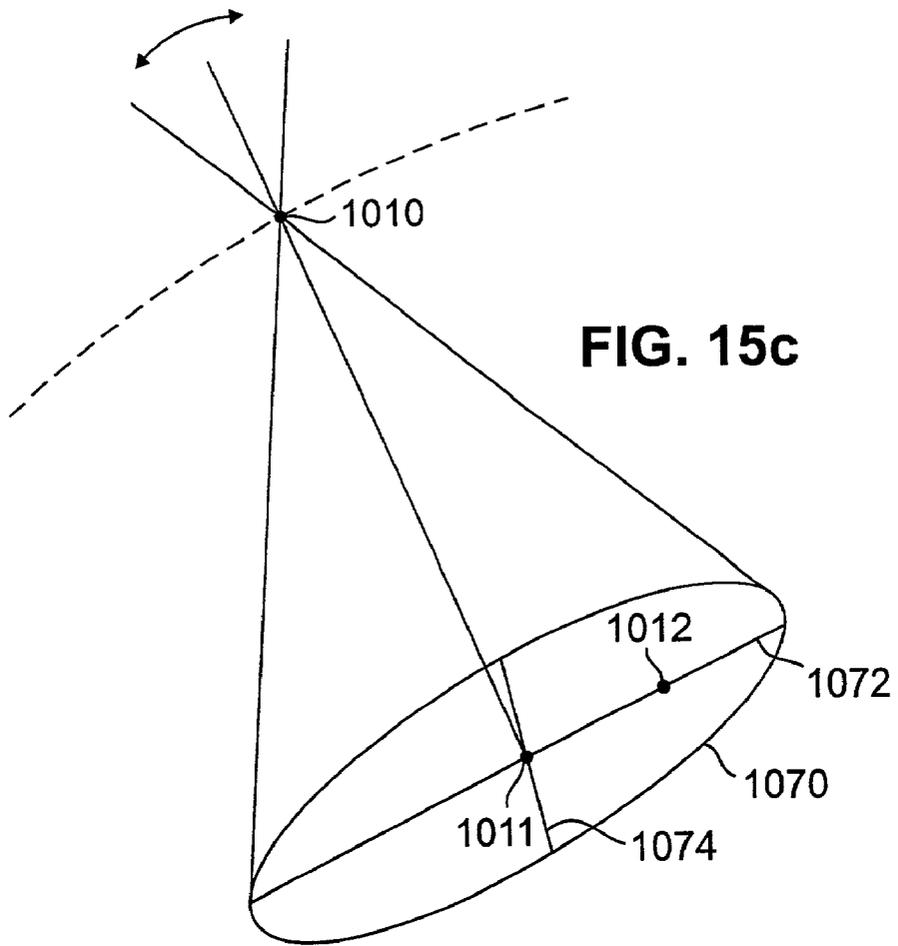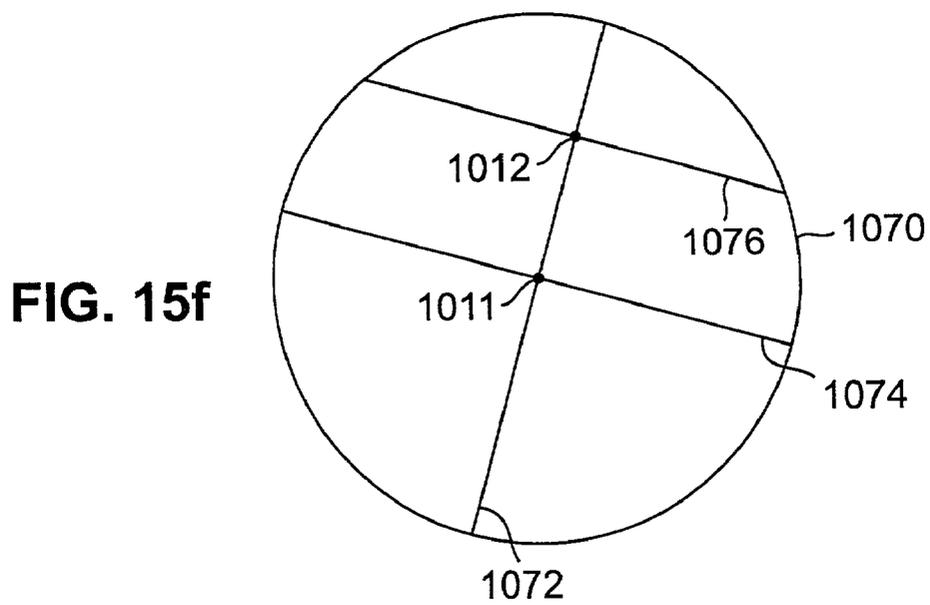


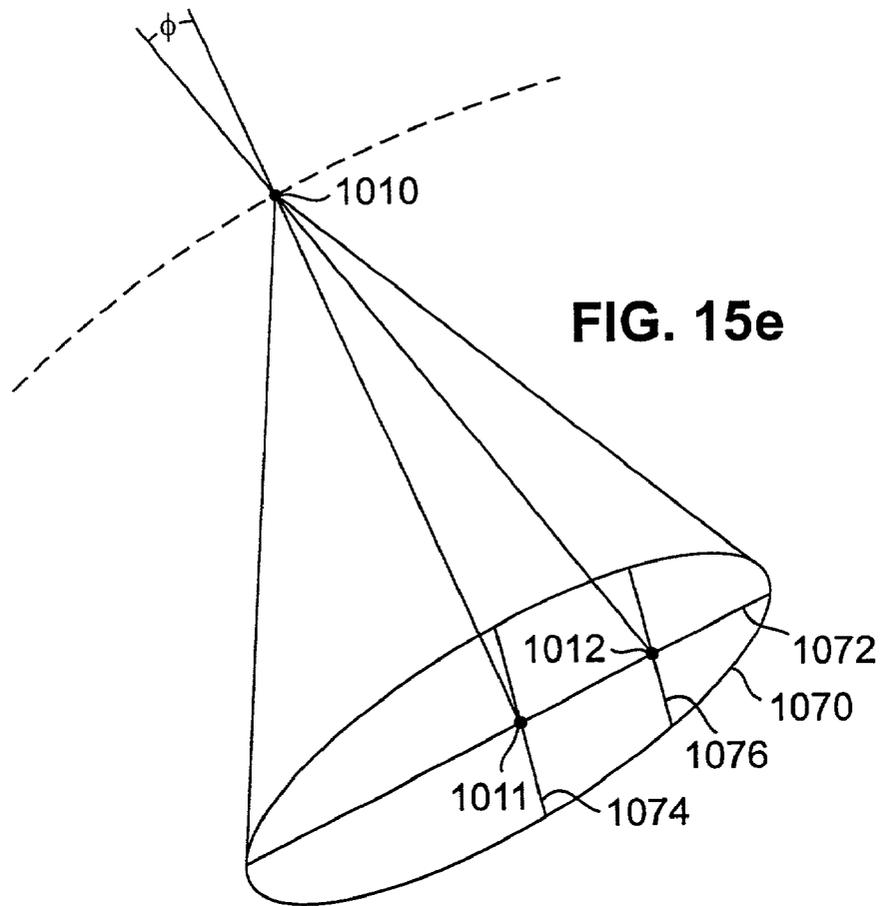

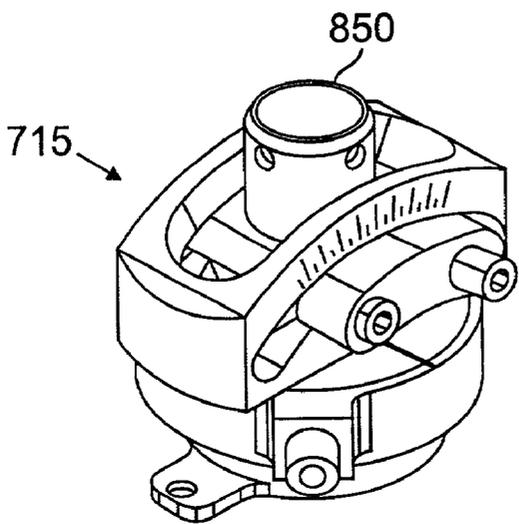


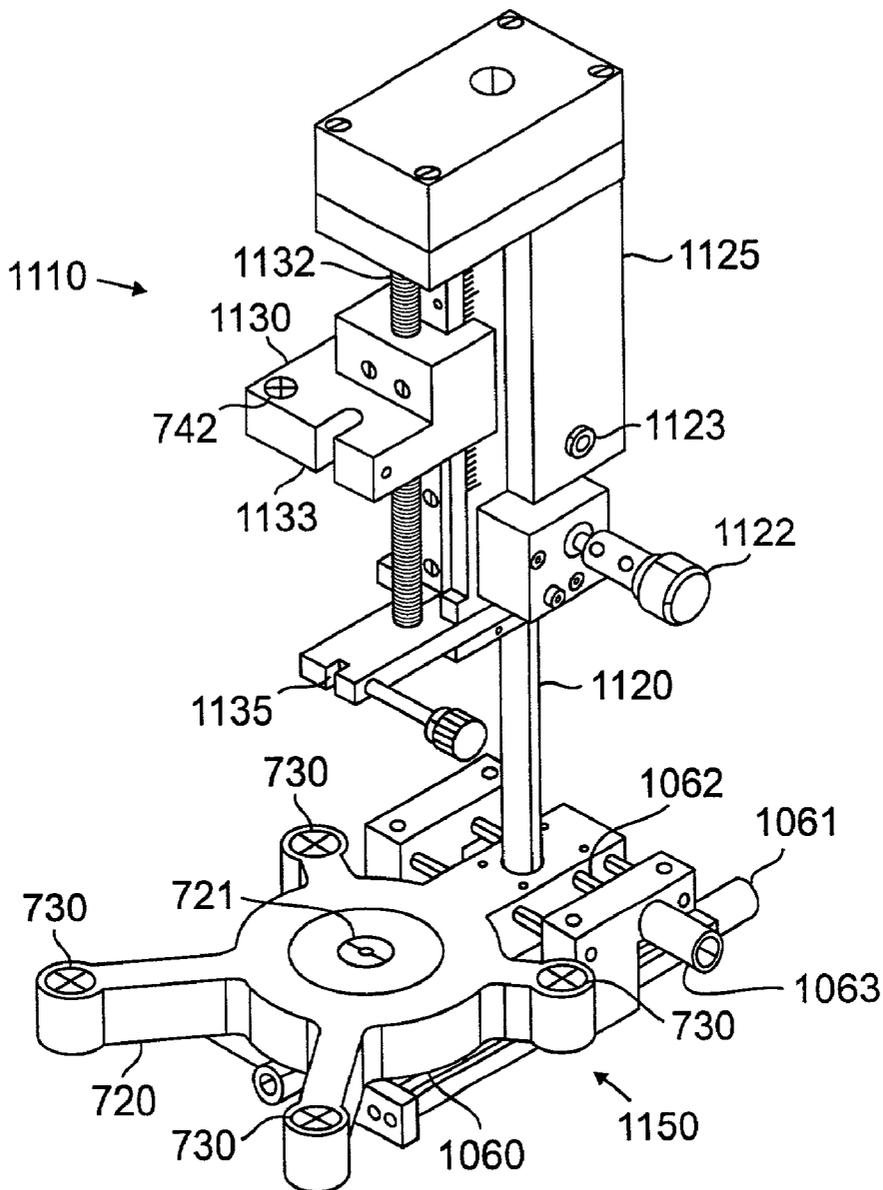


**FIG. 16**

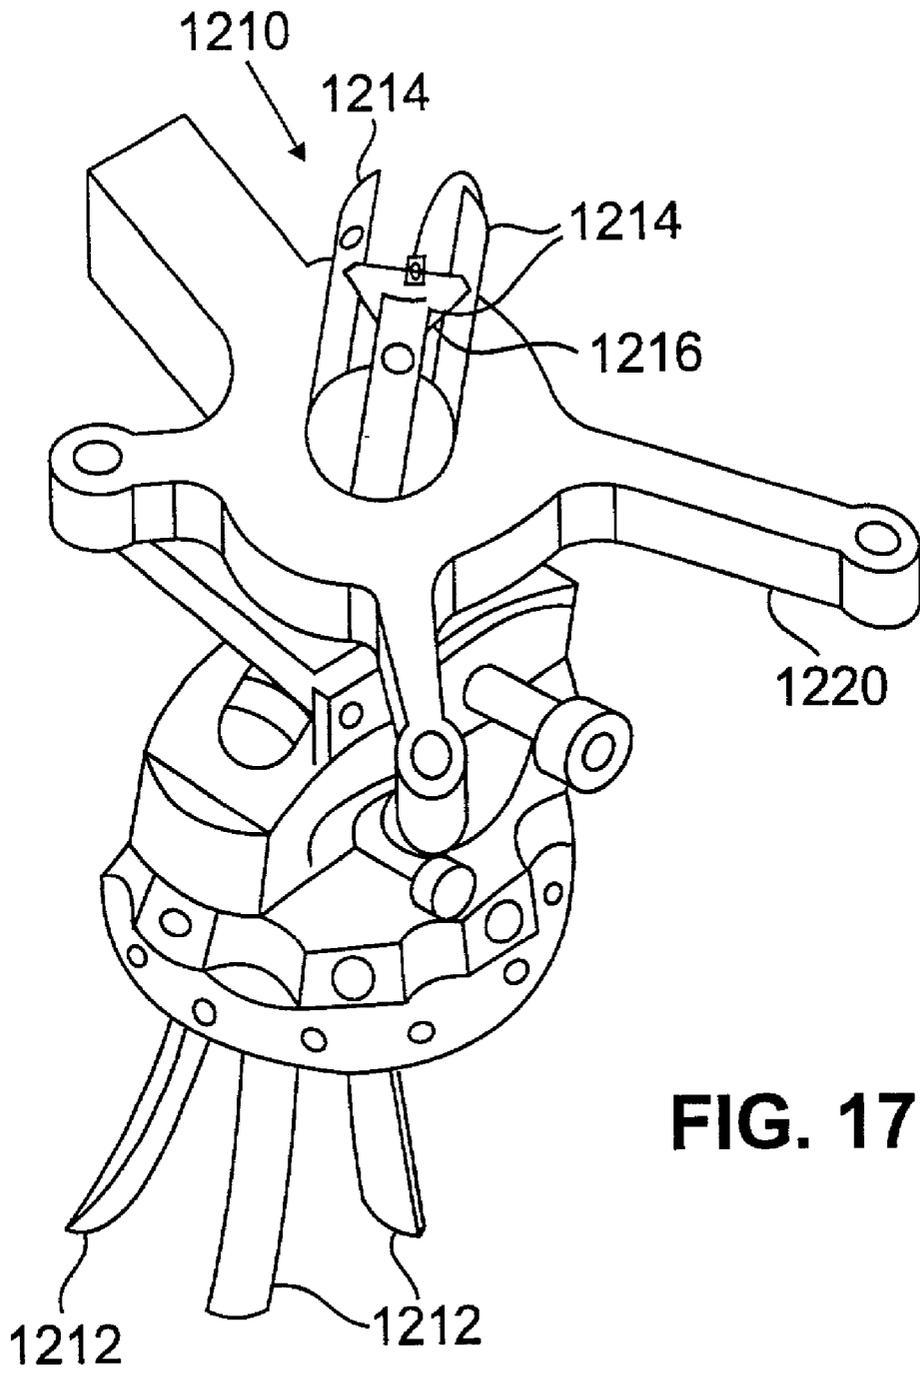


**FIG. 17**

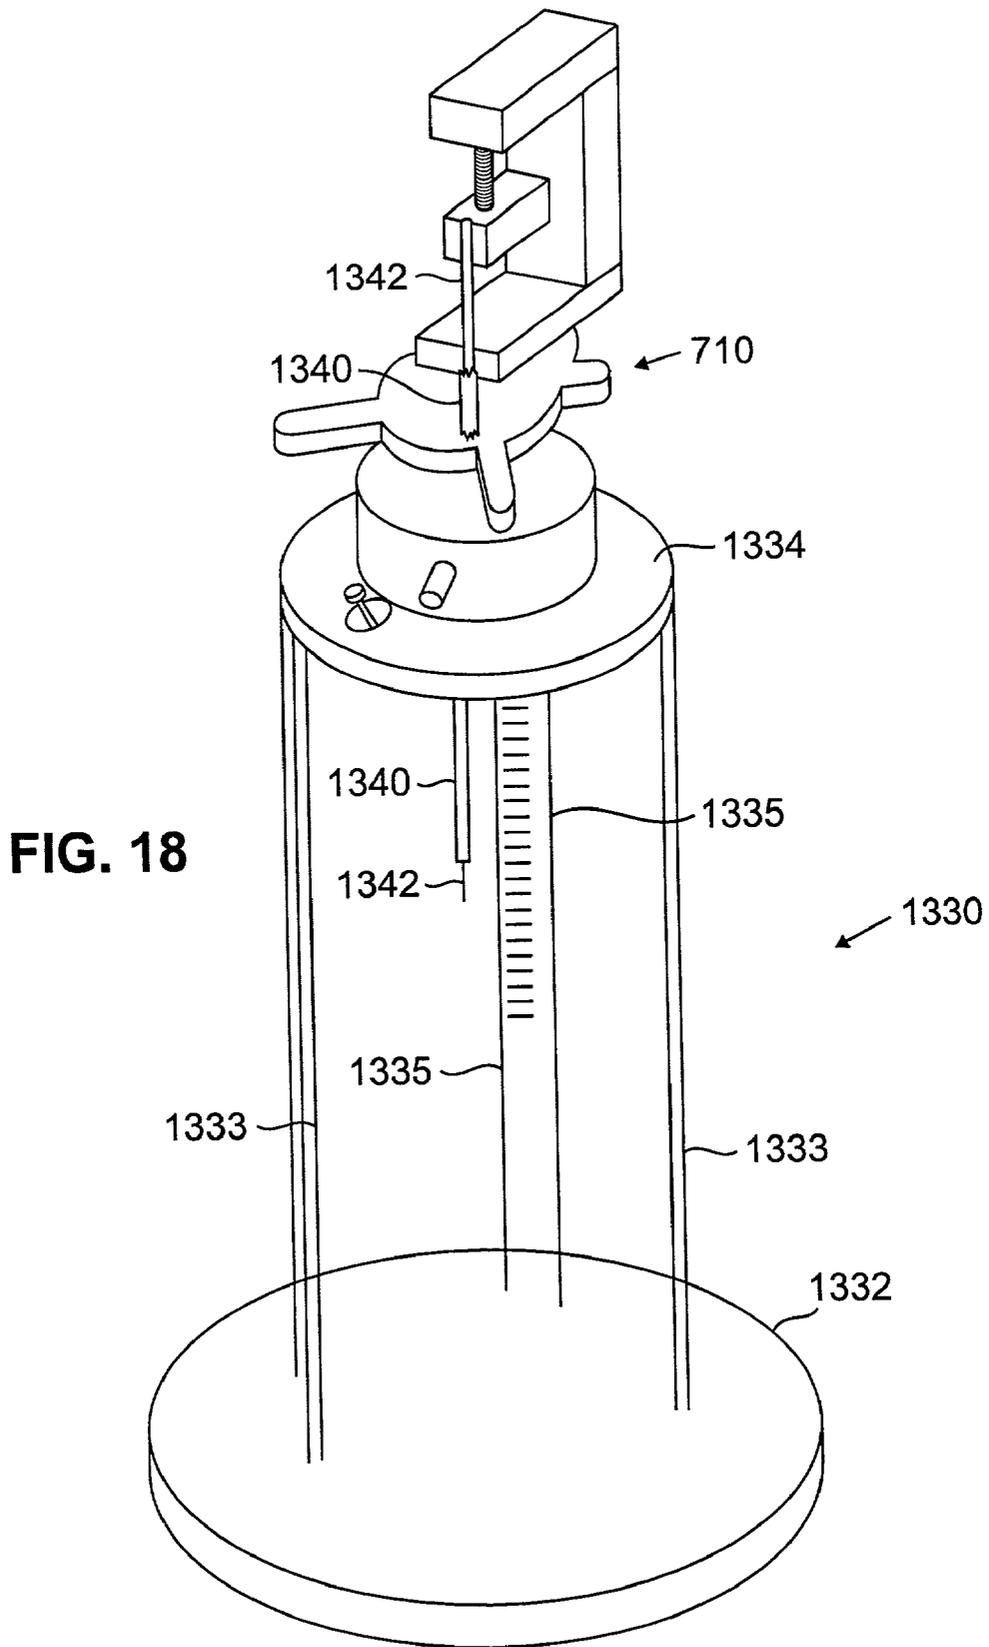


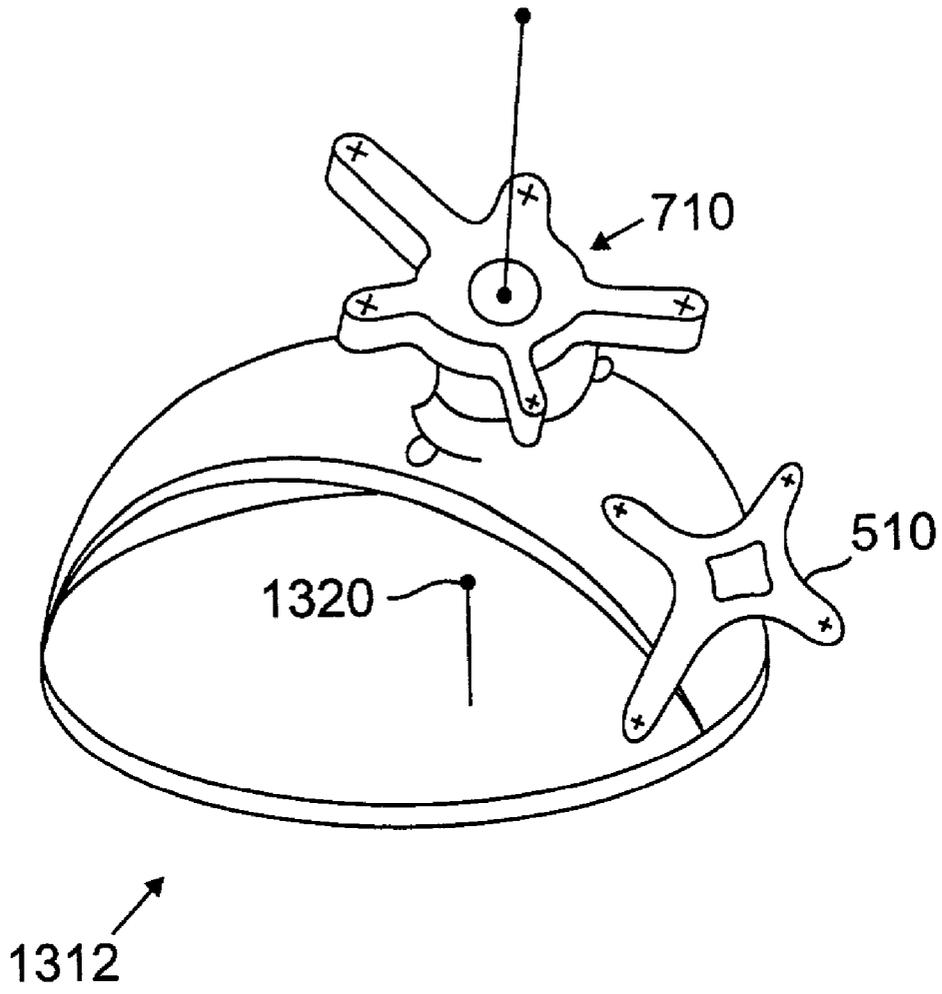


**FIG. 19**

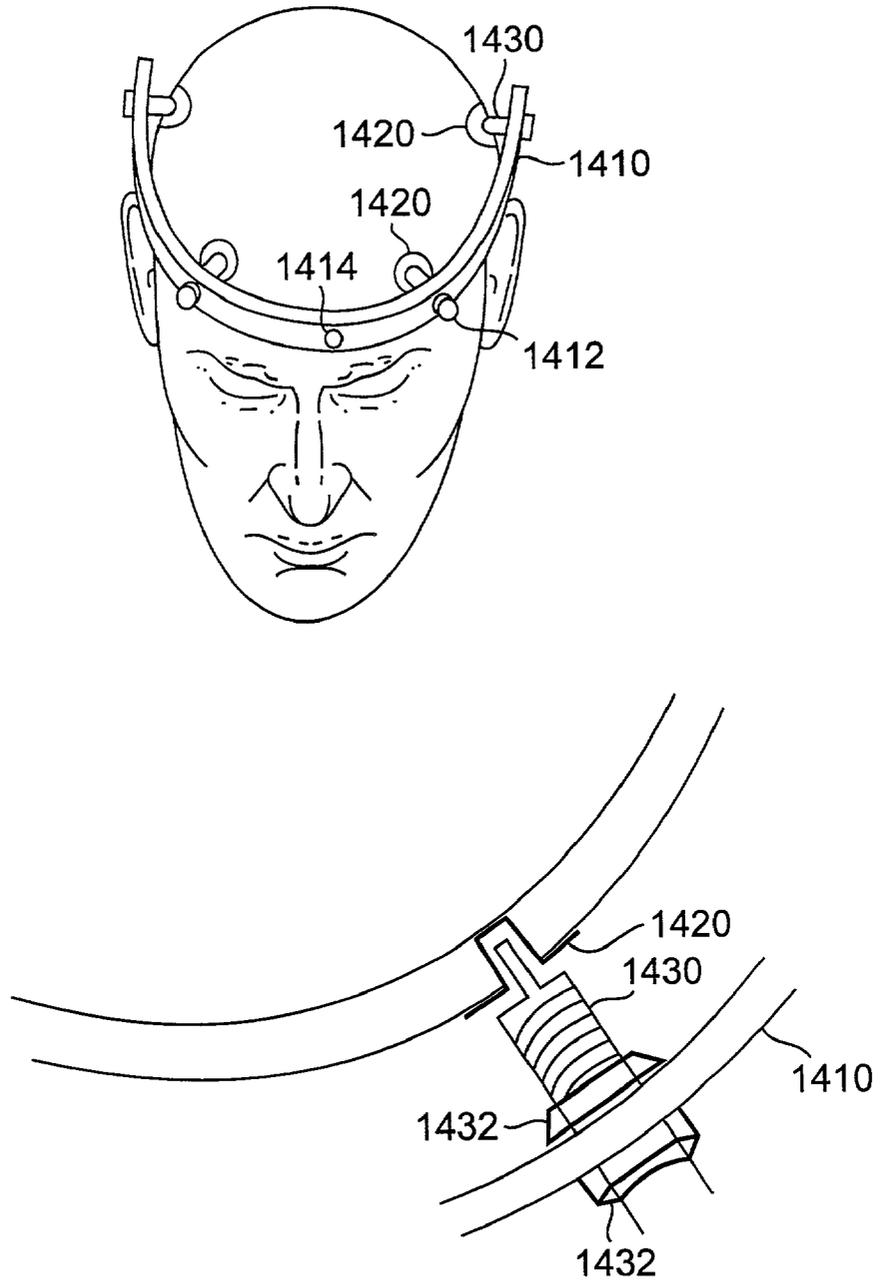


**FIG. 20**

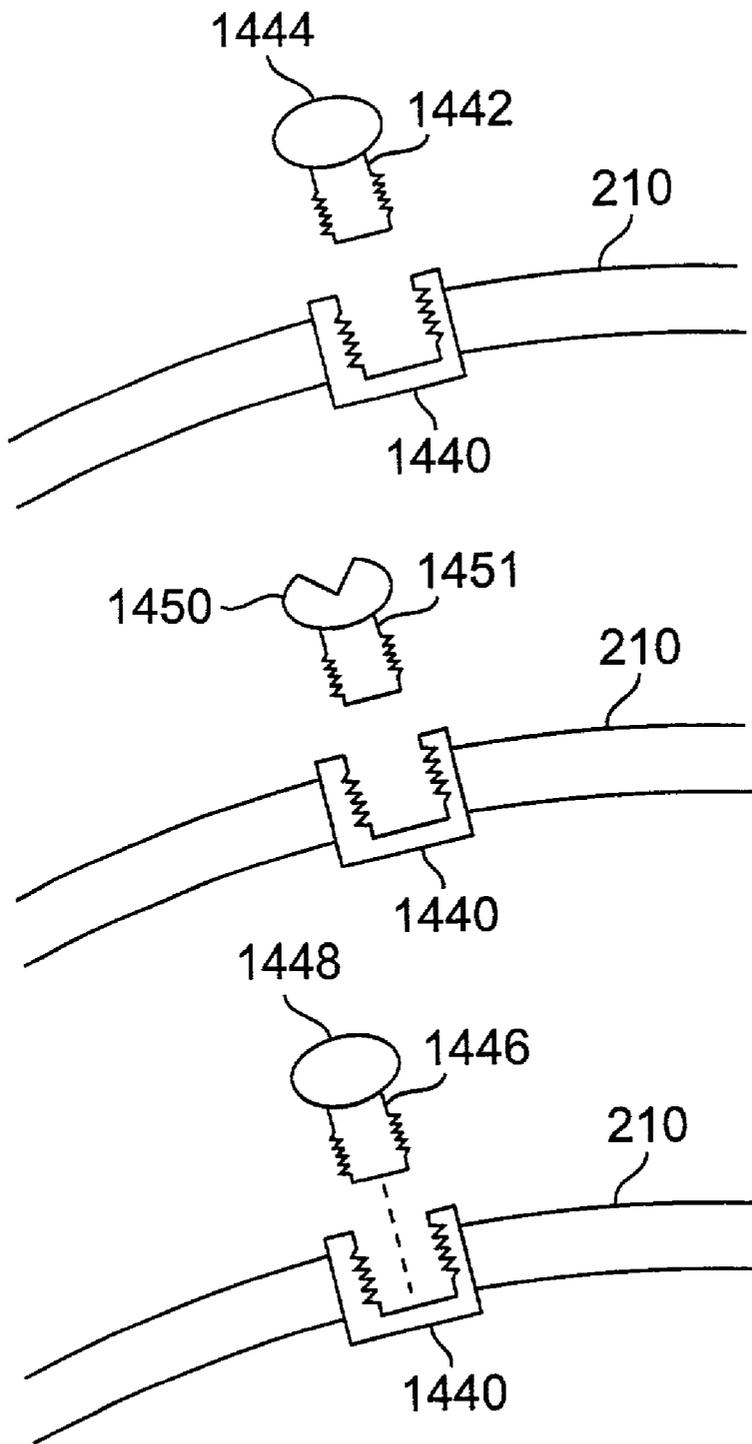

**FIG. 21**

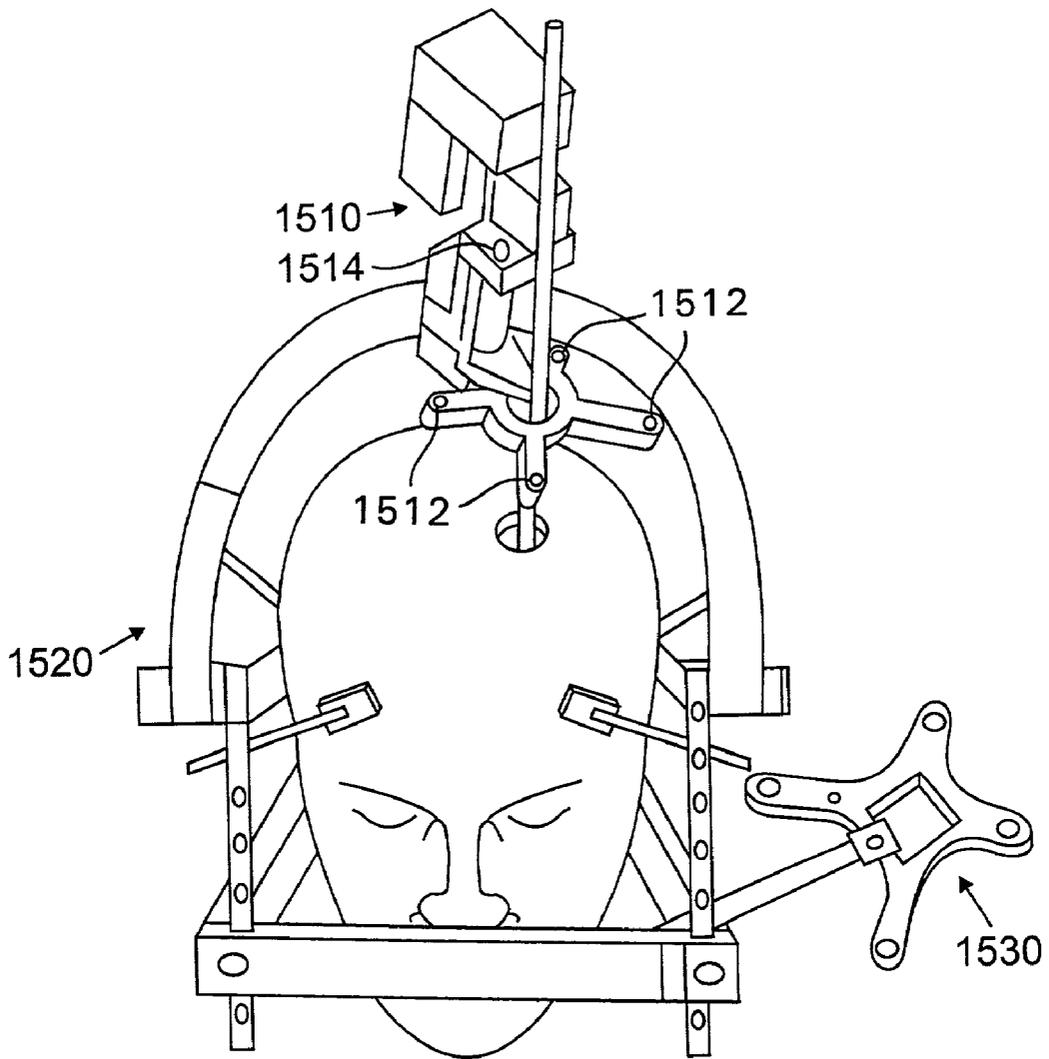

**FIG. 22**

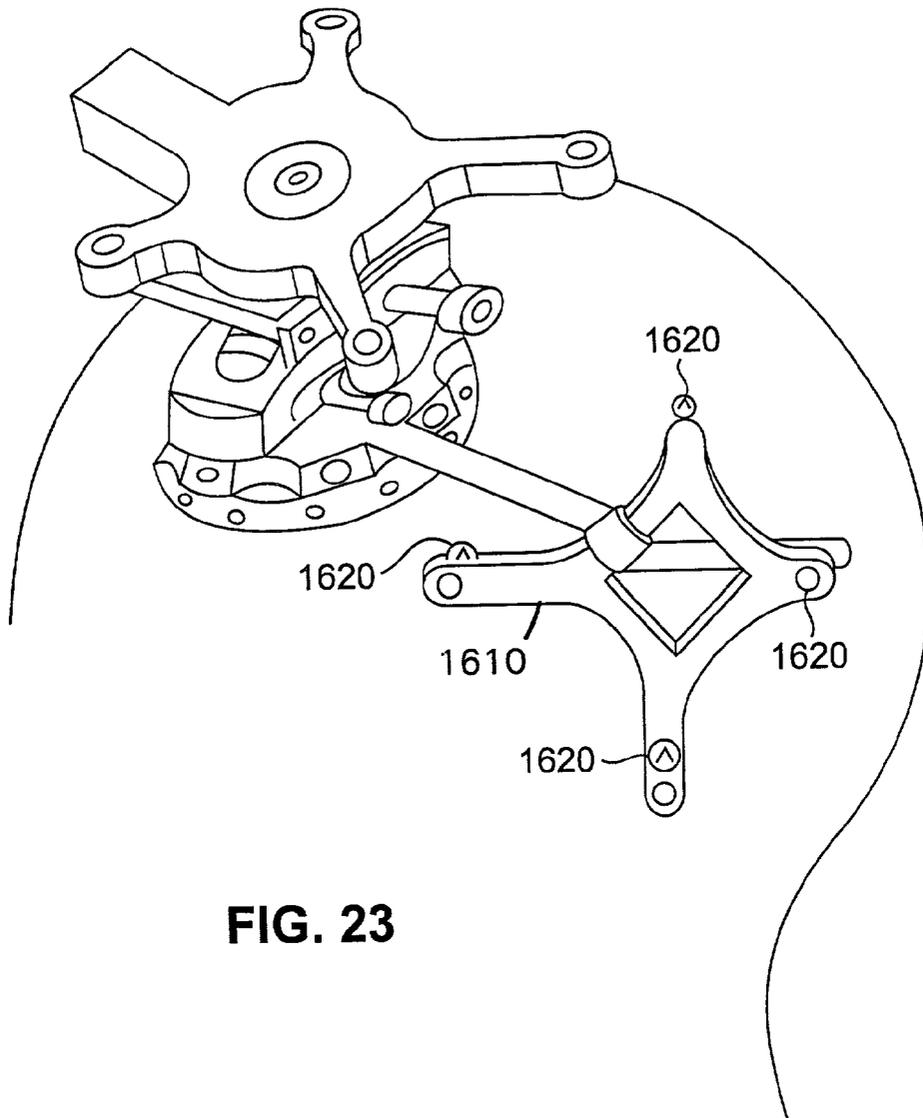

**FIG. 23**

## INSTRUMENT GUIDANCE FOR STEREOTACTIC SURGERY

### RELATED APPLICATION

[0001] This application is a continuation and claims the benefit of priority under 35 USC 120 of U.S. application Ser. No. 09/063,658, filed Apr. 21, 1998. The disclosure of the prior application is considered part of (and is incorporated by reference in) the disclosure of this application.

### BACKGROUND

[0002] This invention relates to guidance of surgical instruments using stereotactic localization.

[0003] Stereotactic localization is a method for locating a target within a three-dimensional object. This method is used in the medical arts and sciences to locate a target in the human body, in particular in the brain or spine, for medical and surgical treatment. Stereotactic surgery has a history dating back to the turn of the century, when the Horsely-Clark Apparatus was described as a mechanical frame system in which an animal was immobilized. This frame system permitted reproducible targeting within the animal's brain for physiological experiments. This and similar technology found application in 1948 in the work of Wycis and Spiegel. In their work, a frame was attached to a human skull. The frame permitted targeting of sites within the human brain for neurosurgical treatment. A detailed survey of the field of stereotactic surgery can be found in *Textbook of Stereotactic and Functional Neurosurgery*, P. L. Gildenberg and R. R. Tasker (eds.), McGraw-Hill, June 1997 (ISBN: 0070236046).

[0004] One approach to stereotactic surgery involves the following steps. Fiducial scanning markers are attached to the body in one of a variety of manners, including using an attachable frame or attaching the markers to the skin with an adhesive. A scan is then taken of a body, for example of the head, to produce a three-dimensional image of the body.

[0005] Scanning can be done using a variety of techniques including CT, MRI, PET, and SPECT. Images of the fiducial scanning markers that are located around the body are then located in the three-dimensional image at fiducial image points. Points of interest, such as the location of a tumor, are located in the three-dimensional image with reference to these fiducial image points. The body and the image are registered by matching the locations of the scanning markers and the coordinates of the fiducial image points. In an approach to stereotactic brain surgery, a three-dimensional frame is screwed to the patient's skull prior to scanning the head. This frame serves as a mechanical reference mechanism that supports scanning fiducial markers at fiducial points around the body. The frame remains attached to the patient's skull from before scanning until after surgery is complete. Prior to surgery, a mechanical guide assembly is attached to the frame. The relative location in the image of the point of interest with respect to the fiducial image points is determined, and this relationship is used to adjust the mechanical guide assembly with respect to the fiducial points on the frame. Using the adjusted mechanical guide assembly, a surgical instrument is then guided to a location in the body that corresponds to the point of interest in the image.

[0006] In another form of stereotactic surgery, known generally as "image-guided" stereotactic surgery, rather than relying on mechanical adjustment of a guide assembly, visual feedback is provided to a surgeon by displaying a composite image formed from the scanned three-dimensional image and a synthesized image of a hand-held surgical instrument. The surgeon guides the hand-held instrument into the body using the visual feedback. In this form of surgery, a frame is attached to the patient and a scan is taken as described above. After scanning, the head and frame are secured in a fixed position, for example, fixed to an operating table. In order to display the image of the surgical instrument in a proper relationship to the scanned image, the position and orientation of the instrument is sensed using a localization apparatus that remains in a fixed position relative to the body. The localization apparatus can be coupled to the surgical instrument using an articulated mechanical arm on which the surgical instrument is attached. Sensors in the joints of the arm provide signals that are used to determine the location and orientation of the instrument relative to a fixed base of the mechanical arm. Some more recent systems do not use mechanical coupling between the surgical instrument and the localization apparatus and instead rely on remote sensing of small localized energy emitters (e.g., sources or transducers of energy) fixed to the instrument. For example, a camera array is used to locate light-emitting diodes (LEDs) that are attached to the instrument. The locations of the LED images in the camera images are used to determine the three-dimensional physical locations of the LEDs relative to the camera array. The locations of multiple LEDs attached to the instrument are then used to determine the location and orientation of the instrument. Another example of remote sensing uses sound generators and a microphone array and relies on the relative time of arrival of acoustical signals to determine the three-dimensional locations of the sound generators.

[0007] Before a synthesized image of the instrument can be combined with the scanned image in a proper relationship, some form of registration is required. For example, the tip of the surgical instrument can be placed at each of several fiducial markers for which corresponding images have been located in the three-dimensional scanned image. Registration of the synthesized image of the instrument and the scanned image can thereby be established.

[0008] In a variant of image-guided stereotactic surgery, generally known as "dynamic referencing," the head and frame are secured in a fixed position, as in the image-guided approach. However, unlike other image-guided techniques, the sensors (e.g., cameras) of the localization apparatus are not at a fixed location. In order to compensate for the motion of the sensors, energy emitters are fixed to the frame as well as to the instrument. At any point in time, the location and orientation of the frame relative to the sensors as well as the location and orientation of the instrument relative to the sensors are both determined, and the differences in their locations and orientations are used to compute the location and orientation of the instrument relative to the frame. This computed location of the instrument is then used to display the synthesized image of the surgical instrument in an appropriate relationship to the scanned image.

[0009] Still another approach to stereotactic surgery, generally known as "frameless image-guided" stereotactic surgery, does not rely on attaching a frame to the body before

scanning. Instead, adhesive fiducial scanning markers are applied to the scalp, or small screws are inserted into the skull, and the patient is scanned as in the techniques described above. During surgery, the patient is immobilized and locked in place using a head clamp or a frame. The image-guided stereotactic approach described above is then followed, including the registration procedure described above to establish the locations of the fiducial scanning markers relative to the instrument.

[0010] In image-guided techniques, a surgeon can rely on a variety of views of a three dimensional scanned image. These views can include a three-dimensional surface view with an adjustable point of view (e.g., a perspective view with surface shading). In addition, planar (i.e., two-dimensional) views of the image can be displayed. In particular, three two-dimension "slices" through orthogonal planes of the image are typically displayed, with the orientations of the planes being sagittal (dividing a head into a left and a right part), coronal (dividing a head into a front and a back part), and axial (dividing a head into an upper and lower part). As the orientations of the planes are predetermined, the particular planes that are displayed can be determined by the point of intersection of the three planes. A point, such as the tip of a probe, can be displayed in a three-dimensional surface view as a point in a appropriate geometric relationship. The point can be displayed in a planer view by orthogonally projecting the point onto the associated plane. A line can be displayed in a planar view as an orthogonal projection onto the associated plane, or as the point of intersection of the line and the associated plane. Note that if a first point, such as a surgical entry point is used to determine which planes are displayed, a second point, such as a surgical target point, does not in general fall in any of the displayed planes.

[0011] Planar views of a three-dimensional scan can also use alternative orientations than the standard sagittal, coronal, and axial orientations described above, allowing two points to lie in two orthogonal planes, and one of the two points to additionally lie in a third orthogonal plane.

[0012] In particular, a "navigational" view can be determined according to two points in an image, such as an entry point at the surface of a body and a target point within the body.

[0013] The line joining the entry point and the target point is chosen as the intersection of two orthogonal planes, navigation planes **1** and **2**. The orientation of navigational planes **1** and **2** is arbitrary (that is, the two planes can be rotated together around their intersecting line). A third plane, orthogonal to navigation planes **1** and **2**, provides a "bird's eye" view looking from the entry point to the target point. This bird's eye plane is typically chosen to pass through the target point. (Such a navigational view is shown in **FIG. 14a**). Using a navigational view, the orientation of a surgical instrument is typically shown as a line projected orthogonally onto the two navigational planes, and as the point of intersection of the line and the bird's eye plane. Manipulating an instrument using such a navigational view for feedback requires considerable practice and is not intuitive for many people.

[0014] Image-guided frameless stereotaxy has also been applied to spine surgery. A reference frame is attached to an exposed spinous process during open spine surgery, and a

probe is used to register the patient's spine with scanned image of the spine. Anatomical landmarks are used as fiducial points which are located in the scanned image. Visual feedback is provided to manually guide placement of instruments, such as insertion of pedicle screws into the spinal structures.

#### SUMMARY

[0015] In one aspect, in general, the invention is a method for positioning a surgical instrument during stereotactic surgery by providing a guidance fixture that includes an upper portion, including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion, and also includes an adjustable base supporting the upper portion, including a mounting base and an adjustment mechanism. The method includes attaching the guidance fixture to a body, including attaching the mounting base to the body. The method also includes determining, using a remote sensing device, the orientation of the upper portion of the guidance assembly in relation to the body, and displaying a representation of a relationship of the constrained trajectory and a target point in the body. The method also includes aligning the guidance fixture, including aligning the orientation of the upper portion to achieve a desired relation between the constrained trajectory and the target point.

[0016] The invention can include one or more of the following features.

[0017] Aligning the orientation of the upper portion includes rotating the upper portion about a central axis of the mounting base and pivoting the upper portion to adjust an angle between the upper portion and the central axis.

[0018] Determining the orientation of the upper portion includes determining the locations of a first set of tracking markers affixed to the upper portion, determining the locations of a second set of tracking markers affixed to the body, and computing the orientation using the locations of the first and the second sets of tracking markers.

[0019] The method can include locking the adjustment mechanism to fix the orientation of the upper portion in relation to the body, and then determining a displacement of the surgical instrument along the constrained trajectory. For example, a remote sensing device can be used to locate a tracking marker affixed in a fixed relationship to the surgical instrument, and used to locate a set of tracking markers affixed to the guidance assembly. The displacement can then be computed using the location of the marker affixed in a fixed relationship to the surgical instrument and the locations of the set of tracking markers affixed to the guidance assembly. The method can also include displaying a representation of a location of the surgical instrument in relation to the body, and guiding the surgical instrument into the body along the constrained trajectory.

[0020] The method can also include attaching to the body a scanning frame that includes a set of scanning markers and then scanning a three-dimensional image of the body, including locating images of the scanning markers in the three-dimensional image. The method then includes attaching to the body a tracking frame that includes a set of tracking markers, and registering the body and the three-dimensional image, including tracking the tracking markers

in the tracking frame and locating points on the body corresponding to the scanning markers. The tracking frame can be attached in a predetermined location in relation to the attachment location of the scanning frame. Locating points on the body can be done by tracking the location of a point on a probe using the remote sensing device, and positioning the point on the probe at each of the points on the body corresponding to the scanning markers.

[0021] Aligning the orientation of the upper portion can include rotating the upper portion about a central axis of the mounting base, and pivoting the upper portion to adjust an angle between the upper portion and the central axis. Displaying the representation of the relationship of the constrained trajectory and the target point then includes displaying a representation of the target point, displaying a representation of the range of possible orientations of the guidance fixture, displaying a first line segment corresponding to possible orientations of the guidance fixture that could result from pivoting the upper portion at a current degree of rotation of the upper portion, and displaying an indication of a current degree of pivoting of the upper portion.

[0022] In another aspect, in general, the invention is a guidance fixture for guiding a surgical instrument into a body during stereotactic surgery. The fixture includes an upper portion including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion, and an adjustable base supporting the upper portion, including a mounting base for attaching the guidance fixture to a body, the mounting base having central opening and a central axis passing through the central opening, and an orientation adjustment mechanism coupled between the mounting base and the upper portion, configuration of the adjustment mechanism determine the orientation of the upper portion relative to the mounting base. The guidance fixture can include a set of tracking markers, such as light emitting diodes, that can be located by a remote sensing device, such as an array of camera.

[0023] The orientation adjustment mechanism of the guidance fixture can include a rotation adjustment mechanism and a pivoting adjustment mechanism, wherein adjustment of the rotation adjustment mechanism rotates the upper portion about the central axis, and adjustment of the pivoting adjustment mechanism adjusts an angle between the upper portion and the central axis. The rotation adjustment mechanism can include a rotating collar attached to the mounting base and the pivoting adjustment mechanism includes a pivoting collar coupling the rotating collar to the upper portion. The adjustable base can further include a rotation locking screw for preventing rotation of the rotating collar and a pivoting locking screw for preventing pivoting of the pivoting collar.

[0024] The upper portion of the guidance fixture can include an x-y table adjustment of which displaces the constrained trajectory.

[0025] The instrument guide of the guidance fixture can include a driving mechanism for positioning the instrument along the constrained trajectory, such as a linear trajectory.

[0026] In another aspect, in general, the invention is a system for stereotactic surgery on a body, which includes a remote sensing device, a tracking frame, including a plurality of tracking markers for tracking a location and an

orientation of the body by the remote sensing device, and a guidance fixture. The system also includes a tracking system for accepting the locations of the tracking markers on the tracking frame and the locations of the tracking markers on the guidance fixture, and computing a relationship between the constrained trajectory and the body, and a display system for presenting an image of the body and the relationship between the constrained trajectory and the body.

[0027] The invention provides several advantages. A highly accurate and reproducible way of guiding a surgical instrument deep into a body is provided without requiring a frame to be fixed to the body for the entire interval from scanning through subsequent surgery. Not requiring the frame to be fixed for this time avoids the inconvenience, discomfort, and inefficiency of placement of a fiducial frame on a patient. Inaccuracy imparted to an MRI scan by electromagnetic interaction with a reference frame or to a CT scan by x-ray interaction with the frame is also improved. Furthermore, by providing a compact and relatively lightweight guidance fixture, the patient is not required to be immobilized during surgery and therefore may not require general anesthesia or heavy sedation. This can allow immediate determination of the response to a surgical intervention in behavioral or physiological terms without interference of general anesthesia or heavy sedation. In addition, both the patient and the sensors used to locate a patient and a surgical instrument can be mobile providing further flexibility in operating procedures.

[0028] An additional advantage is that the invention does not require immobilizing (i.e., clamping in a fixed position) the patient. This contributes to patient comfort which can extend the time a surgical procedure can be carried out. Furthermore, since a guidance fixture is not attached until a scan has been made, surgical time is further extended as discomfort generally relates to having a guidance fixture attached. Also, alignment of the guidance fixture is made easier with this invention, and therefore, less time can be spent on alignment, thereby leaving more time for the actual surgical procedure.

[0029] Another advantage of the invention is that alignment of the guidance fixture is performed using motions, each of which is constrained to one degree of freedom (e.g., rotation or pivoting). When the two motions are clamped in position, this arrangement provides a relatively stable alignment compared to alternative arrangements in which a two degree of freedom motion (such as alignment of a ball and socket arrangement) is clamped.

[0030] Yet another advantage of the invention is that the constrained motions of the guidance fixture, that is, the rotation and pivoting motions, are directly reflected in the computer displayed navigational view, thereby greatly simplifying targeting.

[0031] Other features and advantages of the invention will be apparent from the following description, and from the claims.

#### DESCRIPTION OF THE DRAWING

[0032] FIG. 1 is a flowchart of a stereotactic brain surgery procedure;

[0033] FIG. 2 is a head with threaded inserts implanted including a cross-sectional view of the skull and a threaded insert;

[0034] FIG. 3 is a head with a scanning MIRRF attached including a detailed exploded view of the attachment of the MIRRF to the implanted threaded inserts;

[0035] FIG. 4 illustrates scanning of a head on which a scanning MIRRF is attached;

[0036] FIG. 5 is a head with a tracking MIRRF attached and a cranial probe being tracked using a camera array;

[0037] FIG. 6 is a dataflow diagram for computation of a composite image including a synthesized image of a probe;

[0038] FIG. 7 illustrates locating a planned entry point using the tracked cranial probe and a computer display;

[0039] FIG. 8 is a display of a virtual burr hole and accessible cone of orientations;

[0040] FIG. 9 is a head with a tracking MIRRF and a guidance fixture attached being tracked using a camera array;

[0041] FIG. 10 is a view of a base platter and an adjustable base of a guidance fixture;

[0042] FIG. 11 is an exploded view of the adjustable base of a guidance fixture;

[0043] FIG. 12 is a dataflow diagram for computation of a composite image including a synthesized image of a surgical instrument;

[0044] FIG. 13 is a detailed flowchart of trajectory replanning and fixture alignment;

[0045] FIGS. 14a-c illustrate a navigational view display and corresponding planar segments through a body;

[0046] FIGS. 15a-f illustrate a "field of view" display and corresponding conical section through a body;

[0047] FIG. 16 is a guidance fixture including an adjustable base and an instrument drive attached to a base platter;

[0048] FIG. 17 is a retractor in a guidance fixture;

[0049] FIG. 18 is a calibration jig;

[0050] FIG. 19 is a phantom jig and a guidance fixture and a tracking MIRRF attached to the jig;

[0051] FIG. 20 is an arc shaped MIRRF attached to a head including a view of a threaded insert and mounting bolt;

[0052] FIG. 21 is a scanning marker and a tracking marker attached to a threaded insert;

[0053] FIG. 22 is a guidance fixture and a tracking MIRRF attached to a conventional stereotactic frame; and

[0054] FIG. 23 is a tracking MIRRF attached directly to a guidance fixture.

#### DESCRIPTION

[0055] Referring to FIG. 1, an aspect of the invention relates to stereotactic brain surgery. This approach to brain surgery involves a series of steps, shown in FIG. 1, from start 100 prior to scanning through finish 199 after the surgical phase of a procedure is completed. There are generally two phases to the approach. The first phase involves creating a three-dimensional image of the head (steps 105, 110, 115, 120), planning a surgical trajectory based on the image (step 125), and validating the guidance

fixture (step 130) that will be used during the surgical procedure. The second phase involves the remaining steps (steps 135 through 195) that are used to carry out the actual surgical procedure. The steps of the first phase can be carried out quite some time before those of the second phase. For example, creating the three-dimensional image of the head can be done on one day, and the steps used to carry out the actual surgery can be done on a subsequent day. Also, the steps of the second phase may be repeated, for example on several different days, illustrated by transition 192 between steps 195 and 135.

[0056] One to three days prior to surgery, the patient is seen in a post anesthesia care unit (PACU) or other suitable location. Referring to FIG. 1, the first step of the procedure is to attach anchors to which scanning, registration, and tracking markers will be subsequently attached (step 105). Referring to FIG. 2, the anchors include two threaded inserts 220 that are surgically implanted into the patient's skull 210 using a template (described below). The template precisely determines the separation and parallel orientation of inserts 220.

[0057] Referring to FIG. 3, a rigid cross-shaped device, a scanning "miniature removable reference frame" (scanning MIRRF) 310, is next attached to threaded inserts 220 using screws 320 (FIG. 1, step 110). A retention plate 330 is used to aid precise reattachment of scanning MIRRF 310 to the skull. Retention plate 330 is also used as the template during insertion of threaded inserts 220. Scanning MIRRF 310 includes four fiducial scanning markers 340 that will be visible in the scanned image. Scanning MIRRF 310 is made from a material that is chosen to interfere as little as possible with the type of scan that will be performed. For example, for MRI and CT scans, the chosen material can be polycarbonate, which results in scanning MIRRF 310 being almost invisible in the scanned image. Fiducial scanning markers 340 are mounted in spherical cavities in scanning MIRRF 310. The design of the cavities is such that the "press-in" marker inserts can be removed for cleaning. The star-shaped design of scanning MIRRF 310 is such that, when attached, the elongated part of the star extends behind or in front of the ear so that mounting screws 320 are located toward the top of the skull where soft tissue thickness is minimal and skull thickness is maximal. This minimal tissue thickness allows threaded inserts 220 to be implanted easily under local anesthetic by making a small incision. As an alternative to attaching a single MIRRF as shown in FIG. 3, multiple MIRRFs can be attached in a similar manner to increase the number or separation of the scanning markers.

[0058] Referring to FIG. 4, MRI or CT scanner 400 is used to obtain a three-dimensional digitized image 410 of the head, for example, as a series of two-dimensional "slices" (step 115 in FIG. 1). In addition, a model or map of the surface of the skull can be made allowing, for instance, subsequent three-dimensional surface display of the skull. The fiducial scanning markers 340 produce fiducial images 420 at in image 410. Fiducial coordinates 421 of fiducial images 420 in the coordinate system of image 410 are determined, for example, by manually positioning a cursor at fiducial images 420 on a computer display. Image 410, along with the fiducial coordinates 421, are stored on a computer readable storage medium 430 for use during the subsequent surgical phase of the approach. Typically the

image is stored as a series of two-dimensional images, each corresponding to a horizontal "slice" of the head.

[0059] After scanning, scanning MIRRFF 310 is removed (FIG. 1, step 120), and threaded inserts 220 are left in place. Antibiotic ointment can be applied and the patient is either discharged or sent to the operating room.

[0060] Also after scanning, a surgeon determines the location of a target point within the brain and an entry point through the skull (FIG. 1, step 125). A planned surgical trajectory is then determined as the line joining the entry point and the target point. The surgeon plans the trajectory using a computer display of image 410 which provides, for example, a three-dimensional surface view, and sagittal, coronal, and axial planar views. This allows the surgeon, for example, to plan a trajectory that avoids critical structures in the brain. The target and entry points, and the trajectory are stored along with the image on storage medium 430.

[0061] Other than an optional fixture validation (FIG. 1, step 130), all the preoperative steps are complete at this point.

[0062] Referring to FIG. 5, the surgical phase of the procedure begins by attaching a tracking MIRRFF 510 to threaded inserts 220 (not shown) that remained implanted in the patient's skull after scanning MIRRFF 310 was previously removed. Tracking MIRRFF 510 has a very similar structure to scanning MIRRFF 310. Tracking MIRRFF 510 includes fiducial divots 540 at the centers of locations corresponding to fiducial markers 340 (shown in FIGS. 3 and 4). Four tracking LEDs 550 are also attached to tracking MIRRFF 510. Since tracking MIRRFF 510 is rigid, the geometric relationship between tracking LEDs 550 and fiducial divots 540 is fixed and can be determined beforehand and verified in a subsequent verification step, or can be unknown and determined in a subsequent registration step. Preferably, tracking MIRRFF 510 is made of a material that is lightweight and can be autoclaved, such as Radel.

[0063] After attaching tracking MIRRFF 510 to the patient's skull, the patient can be comfortably placed in an awake, possibly lightly sedated, state in an operating room chair, which is similar to a dental chair. The patient is allowed to recline in an essentially unrestrained manner in the operating room chair in a semi-sitting position. Alternatively, at the surgeon's prerogative and if appropriate, general anesthesia can be administered to the patient.

[0064] Referring still to FIG. 5, a camera array 560 provides time-varying digitized images 586 to a localization application 588 executing on a computer workstation 580. The patient can be free to move relative to camera array 560 and relative to the operating room chair, and camera array 560 can be free to move relative to the patient and relative to the operating room chair. Camera array 560 includes three CCD cameras 562 positioned in a fixed configuration relative to one another. Alternatively, two cameras, which are sufficient for three dimensional localization, or more than three cameras, which may provide greater accuracy, can be used. Each camera 562 in camera array 560 produces one time-varying image. Each tracking LED 550 on tracking MIRRFF 510 is powered and emits infra-red illumination which is seen as a bright point in each of time-varying digitized images 586. Based on the relative coordinates of the bright points in images 586 from each camera 562 of

camera array 560 localization application 588 computes the position (i.e., the coordinates) of tracking LEDs 550 in the coordinate system of camera array 560. Using the positions of multiple tracking LEDs 550, the location and orientation of tracking MIRRFF 510 can be computed by localization application 588. Tracking of MIRRFF coordinates 510 is illustrated schematically by line 564.

[0065] A cranial probe 570, including three probe LEDs 572 attached along its length, is also tracked using camera array 560 and localization application 588. Based on the coordinates of the images of probe LEDs 572 in images 586 and probe geometry 584, localization application 588 computes the position and orientation of probe 570 in the coordinate system of camera array 560.

[0066] Using cranial probe 570, the surgeon then carries out a registration step (FIG. 1, step 140). In this registration step, the surgeon first locates the fiducial points in the image. Then he touches the tip of probe 570 to each of fiducial divots 540 in tracking MIRRFF 510 in turn, indicating to localization application 588 when he is touching each of the divots. Localization application 588 then computes a three-dimensional conformal registration (map) between image 410 and the coordinate system of tracking MIRRFF 510.

[0067] Note that if the geometric relationship of tracking LEDs 550 and fiducial divots 540 is known to localization application 588, for example using a previously calibrated MIRRFF, the coordinates of the fiducial divots can be computed from the coordinates of the tracking LEDs, which in turn can be computed from the locations of the fiducial images in the camera images. The step of touching the divots can be omitted in this case, or used to verify the computed coordinates of fiducial divots.

[0068] Having computed the conformal mapping, localization application 588 continuously combines image 410 and a synthesized image of probe 570 to form a composite image 599 that combines the scanned image with the synthesized image of the probe. Composite image 599 is shown on a computer display 610 which includes a three-dimensional surface display.

[0069] Referring to FIG. 6, the registration and image composition functions performed by localization application 588 involves a series of data processing stages. As shown in FIG. 5, time-varying digitized images 586 are provided to localization application 588 from camera array 560. Referring to FIG. 6, time-varying digitized images 586 are input to MIRRFF tracking 591, a processing stage of localization application 588, which tracks tracking LEDs 550 on tracking MIRRFF 510 and produces "MIRRFF/cam" 593, an orientation and location of tracking MIRRFF 510 in the coordinate system of camera array 560. At the same time, probe tracking 590 tracks probe 570 and produces "probe/cam" 592, an orientation and location of probe 570 in the coordinate system of camera array 560. Probe tracking 590 makes use of probe geometry 584 which specifies the geometric relationship between the tip of the probe 570 and probe LEDs 572. The next stage of localization application 588, relative positioning 594 inputs MIRRFF/cam 593 and probe/cam 592 and produces "probe/MIRRFF" 595, the position and orientation of probe 570 in the coordinate system of tracking MIRRFF 510. When the surgeon touches fiducial divots 540, registration 581 takes the location information from probe/MIRRFF 595 and records it in "fids/MIRRFF" 582,

the coordinates of fiducial divots **540** in the coordinate system of tracking MIRROR **510**. Fiducial coordinates **421**, the coordinates of fiducial images **420** in the coordinate system of image **410**, are provided to localization application **588**, along with image **410**, from storage medium **430**. Mapping **587** includes matching of corresponding coordinates in fids/MIRROR **582** and fiducial coordinates **421** and forming a conformal map **589** between the coordinate system of image **410** and the coordinate system of tracking MIRROR **510**. Conformal map **589** includes the quantities required to transform any three-dimensional coordinate in the coordinate system of tracking MIRROR **510** into a three-dimensional coordinate in the coordinate system of image **410**. These quantities correspond, in general, to a rotation, scaling, and translation of points in the coordinate system of tracking MIRROR **510** to determine the corresponding points in the coordinate system of image **410**.

[**0070**] Referring still to **FIG. 6**, the next stage of localization application **588**, probe mapping **596**, takes the continually updated probe coordinates, probe/MIRROR **595**, and conformal map **589**, and computes probe/image **597**, the coordinates of probe **570** in the coordinate system of image **410**. Then, image composition **598** combines image **410** and a synthesized image of probe **570** to form composite image **599**.

[**0071**] Composite image **599** typically includes a three-dimensional surface view and three orthogonal planar views.

[**0072**] The orthogonal planar views can correspond to the three standard orientations, sagittal, coronal, and axial planes, for instance passing through the planned target point. More typically, three planar views of a navigational view that is determined by the planned entry and target points are included in composite image **599**. The tip of the probe is displayed as an orthogonal projection onto the planes of the planar views, and as a point in an appropriate geometric relationship in the three-dimensional surface view. The orientation of the probe can be displayed using a line passing through the tip of the probe and displayed as an orthogonal projection onto navigational planes **1** and **2** of the navigational view, and as a point of intersection on the bird's eye view of the navigational view.

[**0073**] If the geometric relationships of the fiducial points, fids/MIRROR **582**, the coordinates of fiducial divots **540** does not match the geometric relationships of fiducial coordinates **421**, then an error in placing probe **570** during the registration procedure may have occurred. If such an error is detected, conformal mapping **589** is not computed, a warning is provided to the surgeon, and the surgeon must perform the registration procedure again. Furthermore, if the geometric relationships between fiducial divots **540** is known through prior measurement or calibration, registration errors and errors locating fiducial points **420** in image **410** can also be detected.

[**0074**] Referring to **FIG. 7**, a cranial probe **570** is used to determine an actual entry point. A computer display **610** shows composite image **599**, which includes a three-dimensional surface view and three planar views of a navigational view determined by the planned entry and target points.

[**0075**] Referring to **FIG. 8**, a virtual burr hole **640** is displayed in the planar views of navigational view at the probe location **642** of cranial probe **570**. In addition, the

range of adjustable orientations of a guidance fixture that would be attached at probe location **642** is displayed as a cone **644**, and the extent of effects of x-y adjustment of the guidance fixture is displayed as a second cone **646**. Display of cones **644** and **646** allows the surgeon to verify that planned target point **650** is accessible in the range of adjustments of a guidance fixture attached at probe location **642**.

[**0076**] When the surgeon has located an entry point **620** on the skull, he marks the entry point as the desired center point of attachment of a guidance fixture that will be used during the surgical phase of the procedure.

[**0077**] The patient then has a small area of the head shaved and draped off. A 2 to 4 cm linear incision is made over entry point **620** after local anesthesia is administered. The location of entry point **620** is then reconfirmed using cranial probe **570** after the incision is made. An approximately 1 cm burr hole (not shown in **FIG. 7**) is then drilled through the skull at entry point **620** (**FIG. 1**, step **150**). The surgeon opens the dura under the burr hole and visually inspects the area to determine that no critical structures, such as a blood vessel, are located directly under the burr hole. If the location of the burr hole is found to be unacceptable, a new entry point can be planned and return to the step of locating the entry point (**FIG. 1**, step **145**).

[**0078**] Referring to **FIG. 9**, having drilled the burr hole, the surgeon next attaches a guidance fixture **710** to the skull (**FIG. 1**, step **155**). (Note that an optional instrument drive can also be included in the guidance fixture but is not shown in **FIG. 9**.) As is described more fully below, guidance fixture **710** includes a base platter **720** on which platter LEDs **730** are attached. Base platter **720** is attached to an adjustable base **715**, which is in turn attached to the skull. The orientation of a line normal to base platter **720** is adjustable within a cone forming a solid angle of approximately 45 degrees. After attaching guidance fixture **710** the surgeon adjusts the orientation of base platter **720** (**FIG. 1**, step **170**; note that optional steps **160** and **165** are described below). A surgical instrument **740**, including an instrument LED **742** fixed relative to the instrument, passes through guidance fixture **710**. Surgical instrument **740** is constrained to follow a fixed trajectory perpendicular to and through a central opening through adjusted base platter **720**. Workstation **580** tracks the location and orientation of base platter **720**, and the displacement of surgical instrument **740**, indicated schematically by lines **564** and **750** respectively, and computes the position of surgical instrument **740** in the coordinate system of image **410**. Workstation **580** continually displays on display **610** a composite image **750** including a navigational view of image **410** showing the position and orientation of surgical instrument **740**. The surgeon uses the visual feedback on display **610** to position surgical instrument **740** along the constrained trajectory. Note that during this time, the patient is not necessarily immobilized. Both the patient and camera array **560** can move and, as long as platter LEDs **730** and instrument LED **742** are visible to camera array **560** at an appropriate distance and orientation, workstation **580** can maintain a continuously updated display.

[**0079**] Referring to **FIG. 10**, guidance fixture **710** includes base platter **720** and adjustable base **715**. In use, base platter **720** is attached to an entry column **850** (through an x-y

positioning table **1150**, described fully below) which is held in adjustable base **715**. The orientation of entry column **850** can be adjusted relative to skull **210** using separate rotation and pivoting motions, as described below.

[0080] Referring also to the exploded view of adjustable base **715** shown in FIG. 11, guidance base **715** includes a mounting base **820**, which is rigidly attached to the skull during an operation using screws through mounting holes **822**. Mounting holes **822** pass through mounting tabs **723** as well as through the inside of the mounting base **820**. Mounting tabs **823** are pliable to allow them to conform to the skull. As mounting base **820** may be distorted in being mounted to the skull, it can be designed to be disposable. Mounting base **820** has a cylindrical opening which accepts a rotating collar **830**. A rotation locking screw **824** in mounting base **820**, when tightened, locks rotating collar **830** in place and prevents its movement within the mounting base. Entry column **850** is held within rotating collar **830** by a pivoting collar **840**. Pivoting collar **840** slides in an arc-shaped pivoting guide **841** within rotating collar **830**. When rotated, a pivoting locking knob **846** prevents pivoting collar **840** from sliding by drawing a collar clamp **842** against pivoting collar **840** using a threaded rod **920**. When rotated, a pivoting adjustment knob **844** slides pivoting collar **840** along pivoting guide **841**.

[0081] Referring again to FIG. 11, mounting base **820** includes mounting holes **822** drilled through mounting tabs **723** (one tab is not visible on the side opposite the visible one), as well as through the inside of mounting base **820**. Mounting base **820** includes a threaded hole **922** within which rotation locking screw **824** turns. Rotation locking screw **824** mates with a recessed channel **923** in rotating collar **830**, thereby preventing rotation of rotating collar **830** and also preventing rotating collar **830** from lifting off mounting base **820**.

[0082] Entry column **850** includes a cylindrical portion **913** and a spherical portion **914** at one end. Spherical portion **914** mates with a spherical socket **916** in the bottom of rotating collar **830**. When mated, entry column **850** can pivot within rotating collar **830**. Entry column **850** also has opposing groves **910** which mate with protrusions **912** on the inside of the circular opening in pivoting collar **840**. Entry column **850** passes through the circular opening, and protrusions **912** mate with groves **910**. When assembled, the mated groves and protrusions hold the spherical portion **914** of entry column **850** against spherical socket **916** in the bottom of rotating collar **830**.

[0083] The position of pivoting collar **840** within pivoting guide **841** is adjusted by turning pivoting adjustment knob **844** and tightened in place by rotating pivoting tightening knob **846**. Pivoting adjustment knob **844** attaches to a pivoting adjustment rod **930** which passes through collar clamp **842** and the main portion of pivoting collar **840** to a rack and pinion mechanism. A pinion **931** is attached to the end pivoting adjustment rod **930**. Pinion **931** mates with an arc-shaped rack **932** which attaches to rotating collar **830** using three screws **934**. Rotation of pivoting adjustment knob **844** rotates pivoting adjustment rod **930** and pinion **931**, which then slides pivoting collar **840** in pivoting guide **841**.

[0084] Rotating pivoting locking knob **846** locks pivoting collar **840** rigidly to rotating collar **830**. Tightening both

rotation locking screw **824** and pivoting locking knob **846** fixes the orientation of entry column **850** relative to mounting base **820**.

[0085] Referring to FIG. 10, the procedure for attaching and adjusting guidance fixture **710** (FIG. 1, steps **155** through **170**) is carried out as follows. Mounting base **820** is attached in a temporary fashion over burr hole **625**. While attaching the base, mounting tabs **723** are conformed to the shape of the skull **210** and secured to the skull an orientation generally directed towards the target using three or more titanium bone screws **724** passing through mounting holes **822** through mounting tabs **723** and through the interior of the mounting base.

[0086] After mounting base **820** is attached to skull **210**, the remainder of guidance base **715** is attached to mounting base **820**. In particular, rotating collar **830**, with entry column **850** already attached, and adjusted to be centered (oriented along the central axis of guidance base **715**) is inserted in mounting base **820** and rotation locking screw **824** is tightened to mate with recessed channel **923**.

[0087] After guidance base **715** is attached to skull **210**, the remainder of guidance fixture **710** is attached to guidance base **715**. In FIG. 10, the drive assembly, which is already attached to base platter **720** at the time base platter **720** is attached to guidance base **715** is not shown. Base platter **720** is attached to entry column **850** via an x-y positioning table **1150** (described below). During the alignment phase in which the orientation of guidance base **715** is adjusted, x-y positioning table **1150** remains centered.

[0088] During a surgical procedure, surgical instrument **740** is passed through a central opening **721** of base platter **720** and through entry column **850** into the brain. During the alignment phase in which x-y table **1150** is centered, a line along the trajectory surgical instrument **740** would follow passes along the central axis of entry column **850**. Adjusting the orientation of guidance base **715** adjusts this trajectory. In all orientations, the trajectory passes through a single point on the central axis of guidance base **715** near the surface of the skull. If the guidance base is exactly mounted over the planned entry point, this single point is the planned entry point. More typically, the point is slightly displaced from the planned entry point due to mounting inaccuracies.

[0089] Referring again to FIG. 9, platter LEDs **730** on base platter **720** are sensed by camera array **560**, and the location and orientation of base platter **720** in the coordinate system of image **410** is computed by localization application **588** executing on computer workstation **580**. Localization application **588** computes the location and orientation of base platter **720** using the known geometry of the base platter relative to platter LEDs **730**.

[0090] Referring to FIG. 12, localization application **588** computes composite image **750** (FIG. 9) in a series of data transformations. Time-varying digitized images **586** are passed to MIRRFF tracking **591** as well as platter tracking **7010** and instrument tracking **7012**. MIRRFF tracking **591** produces "MIRRFF/cam"**592**, the position and orientation of tracking MIRRFF **510** in the coordinate system of camera array **560**. Platter tracking **7010** produces "platter/cam"**7020**, the position and orientation of base platter **720**. The instrument trajectory is at a known location and orientation relative to platter LEDs **730** on base platter **720**,

therefore the location and orientation of the instrument trajectory in the coordinate system of camera array 560 is also known. Instrument tracking 7012 produces instrument/cam 7022, the location of instrument LED 742 in the coordinate system of camera array 560. Platter localization 7030 uses conformal map 589, MIRRF/cam 593, and platter/cam 7020 to compute platter/image 7040, the location and orientation of base platter 720 in the coordinate system of image 410. Note that once guidance fixture 710 is attached and aligned, then base platter 720 no longer moves relative to the skull (other than due to adjustment of x-y table 1150) and therefore, platter/image 7040 can be fixed rather than continuously recomputed. Instrument depth measurement 7032 combines platter/cam 7020 and instrument/cam 7022 to compute instrument/platter 7042, the depth of penetration of the surgical instrument relative to the plane of base platter 720. Instrument depth measurement 7032 makes use of the known displacement of the tip of the instrument from instrument LED 742. Instrument localization 7050 takes platter/image 7040 and instrument/platter 7042 and computes instrument/image 7060, the location and orientation of the surgical instrument in the coordinate system of image 410. Finally, image composition 7070 combines image 410 with a synthesized image of the surgical instrument to generate a composite image 750.

[0091] Referring to FIG. 13, before aligning guidance fixture 710, the surgical trajectory is optionally replanned to go through the center of the actual mounted position of the guidance fixture, rather than the planned entry point (FIG. 1, step 165).

[0092] The surgeon aligns guidance fixture 710 using visual feedback. Referring to FIGS. 14a-c, a navigational view indicating the trajectory of the surgical instrument is used. Referring to FIG. 14a, navigational planes 1020 and 1022 correspond to navigational planar views 1030 and 1032 respectively. Navigational planes 1020 and 1022 are orthogonal and their intersection forms a line passing through an entry point 1010 and a target point 1012. Bird's eye plane 1024, the third plane of the navigational view, is orthogonal to planes 1020 and 1024 and passes through target point 1012.

[0093] Referring to FIG. 14b-c, navigational planes 1020 and 1024 are shown schematically, along with a line 1040 corresponding to the orientation of guidance fixture 710. The goal of the alignment procedure is to make line 1040 coincident with the intersection of planes 1020 and 1022. The alignment procedure is carried out in a series of two motions each of which is constrained to one degree of freedom. Initially, line 1040 is not generally coincident with either navigational plane. Prior to beginning the alignment procedure, the orientation of line 1040 is displayed as orthogonal projections, lines 1041 and 1042, on planes 1020 and 1022, respectively.

[0094] In the first alignment motion, rotating collar 830 is rotated within mounting base 820 (FIGS. 10 and 11). Referring to FIG. 14b, this rotation causes line 1040 to sweep out a portion of a cone, indicated diagrammatically by dashed arrow 1050. After rotation through an angle  $\delta_1$ , orientation line 1040 is in the direction of line 1043, which is coincident with plane 1022. During the rotation, the orthogonal projection line 1041 of line 1040 in plane 1020 forms a smaller and smaller angle  $\epsilon_1$  with the

desired orientation in plane 1020, while the angle  $\epsilon_2$  between the orthogonal projection line 1042 in plane 1022 and the desired orientation in plane 1022 increases, ultimately to  $\delta_2$  when line 1040 is coincident with plane 1022.

[0095] Referring to FIG. 14c, the second alignment motion reduces the angle  $\delta_2$  while maintaining the coincidence of the orientation line and plane 1022. This motion corresponds to sliding pivoting collar 840 within rotating collar 830 (FIGS. 8 and 9). Alignment is achieved when angle  $\delta_2$  is zero, that is, the orientation line 1040 is coincident with the intersection of planes 1020 and 1022.

[0096] At this point, after tightening the locking knobs on guidance fixture 710, base platter 720 is firmly fixed to the skull, in an orientation and location that constrains a surgical instrument passing through it to pass along the replanned trajectory to the planned target point in the head.

[0097] In addition to, or as an alternative to, using a navigational view to provide visual feedback during the alignment procedure, a "field of view" display can be provided. Referring to FIGS. 15a-f, the field of view display uses a representation of a cross-section of a cone extending below the entry point. Referring to FIG. 15a, the central axis of a cone 1061 is coincident with the central axis of the mounting base of a guidance fixture mounted at an entry point 1010. That is, the central axis of the cone is generally perpendicular to the surface of the skull at the entry point. The angle of the cone corresponds to the range of possible alignments of a guidance fixture mounted at the entry point. In this embodiment, this is a 45 degree angle. The cross-section is normal to the central axis of the cone, and passes through a target point 1012. Referring to FIG. 15b, the corresponding display shows a circular section 1070 of the scanned image. The center 1011 and the target point 1012 are indicated. Also indicated are two orthogonal axes. An axis 1072 corresponds to the achievable orientations of the guidance fixture as its pivoting collar is moved in the rotating collar. Another axis 1074 is orthogonal to axis 1072. Motion of the rotating collar rotates the orientation of axes 1072 and 1074. These axes can be thought of as intersections of the navigational planes with the bird's eye plane of a navigational view, although here, the intersecting lines rotate with the rotation of the guidance fixture while in the navigational view, the navigation planes remain fixed as the guidance fixture is rotated. Referring to FIG. 15c, after an appropriate rotation, axis 1072 passes through target point 1012. FIG. 15d shows the display after this rotation. Motion of the pivoting collar is indicated by a line 1076, parallel to axis 1074. If the pivoting collar is centered, then line 1076 is aligned with axis 1074, as is shown in FIG. 15d. When the guidance fixture is aligned with the target point, line 1076 passes through target point 1064, as does axis 1072. FIG. 15f, corresponding to FIG. 15e, shows the display after alignment is achieved. This circular field of view display provides intuitive visual feedback to the surgeon who is aligning the guidance fixture. Furthermore, displacement of the x-y table can also be shown in such a field of view display, by indicating the intersection of the resulting instrument trajectory on the circular display.

[0098] Referring to FIG. 16, an instrument drive 1110 is attached to base platter 720 prior to attaching the combination of instrument drive 1110, base platter 720, and x-y table 1150 to guidance base 715. In FIG. 16, instrument drive

**1110** is shown partially mounted onto a drive post **1120**. Prior to attachment to guidance base **715**, drive post **1120** is fully inserted into instrument drive **1110** so that instrument drive **1110** is in contact with base platter **720**. Base platter **720** can be displaced relative to guidance base **715** in a plane orthogonal to entry column **850** using two perpendicular adjustment screws **1060**, and **1062** turned by x-y table adjustment knobs **1061**, and **1063**. Note that prior to alignment (**FIG. 1**, step **170**) the x-y table is adjusted so that central opening **721** in base platter **720** is centered over entry column **850**.

[**0099**] Instrument drive **1110** includes a drive platform **1130** that moves within a drive mechanism **1125** along a threaded rod **1132**. Threaded rod **1132** is oriented parallel to drive post **1120** and perpendicular to base platter **720**. In this embodiment, rotation of threaded rod **1132**, which causes displacement of drive platform **1130**, is manual using a mechanism that is not shown. Alternative embodiments can use an electronic stepper motor or a manual hydraulic drive to rotate threaded rod **1132** and thereby displace drive platform **1130**.

[**0100**] In operation, a surgical instrument, such as a micro-electrode, is passed into the brain through a guidance tube. After alignment of guidance fixture **710**, the guidance tube is manually inserted into the brain through central opening **721** in base platter **720**. The guidance tube is then secured in clamp **1135** that is fixed relative to drive mechanism **1125**. The instrument is passed into the guidance tube and is secured in a clamp **1133**, which is fixed relative to drive platform **1130**.

[**0101**] Instrument LED **742** is attached to drive platform **1130**. The displacement of the end of the surgical instrument from instrument LED **742** is known to localization application **588** which executes on workstation **580**. By tracking the position of instrument LED **742**, as well as platter LEDs **730**, the position of the end of a surgical instrument on workstation **580** and displayed on display **610** (**FIG. 9**) to the surgeon. The surgeon then uses this visual feedback in adjusting the depth of the instrument.

[**0102**] Various types of surgical probes or instruments can be attached to drive mechanism **1110** shown in **FIG. 16**. One type of instrument is an electrode, such as a recording micro-electrode or a stimulating electrode or lesioning electrode. The electrode is introduced into a rigid insertion (guidance) tube that is attached to drive mechanism **1110**. Another type of instrument is a hypothermia cold probe.

[**0103**] In cases of movement disorder or pain surgery, a chronically implanted stimulating electrode can be placed utilizing an insertion tube. The lead, being of a smaller diameter than the insertion tube, can be slipped through the insertion tube upon removal of the drive and guide assembly, to allow fixation of the chronically implanted electrode into the brain. The electrode is secured to the skull using a compression-fitting. A chronically implanted recording electrode can similarly be placed during epilepsy surgery to monitor abnormal activity within the deep brain utilizing similar techniques.

[**0104**] In cases of hydrocephalus or other situations where chronic drainage of intracranial cavities is necessary, a shunt tube, such as a ventricular shunt, can be applied through the insertion tube into the target such as the ventricles of the brain. The shunt tube will have a stylet and be slipped into the insertion tube.

[**0105**] The insertion tube structure and its retention ring will have varying diameters, depending on the diameters of the various objects that can be placed in the insertion tube, such as the shunt tube, in this application, or micro-electrodes, in the prior application. The insertion tube, therefore, will be connected to the drive mechanism using varying sized retention rings. The shunt will be directed towards the target established by the software mechanism alluded to above. The shunt tube will then be secured to the skull via mechanisms described in prior art, or via a compression fitting described above.

[**0106**] Alternatively, a biopsy probe can be inserted into the insertion tube by first placing a biopsy tube with a trocar/obturator through the insertion tube. The mechanism would then be directed down towards the appropriate target using the drive mechanism. The obturator would be removed, and a cutting blade will then be inserted into the biopsy tube.

[**0107**] In applications in which a radioactive seed for brachytherapy, a targeting nodule with a radio sensitizing, chemotherapeutic agent for external beam radiation, or a sustained release polymer drug or microdialysis capsule for local drug administration, are required for placement in a deep brain target, a different insertion tube can be connected to the drive mechanism **1110**. A delivery catheter can be placed through the insertion tube. The whole mechanism can be directed towards the deep target using the software system as alluded to above. An insertion plunger can be used to insert the object of delivery and the system is then be removed after insertion of the object. A micro-endoscope can also be inserted through the insertion tube mechanism described above and deep brain structures can be visualized prior to excision or lesioning.

[**0108**] In certain surgical procedures, it is desirable to drive a surgical instrument along several parallel tracks. This is facilitated using x-y table **1150**. Before an instrument is driven toward the target, an offset is adjusted using adjustment knobs **1061**, and **1063**. These knobs include markings that allow precise adjustment.

[**0109**] An example of a procedure using penetration of an instrument along parallel tracks involves mapping the electrical activity of a region of the brain. The surgical instrument in this case is a thin electrode that is repeatedly inserted to points on a two- or three-dimensional grid. At each point, electrical activity is monitored.

[**0110**] Referring to **FIG. 17**, when larger masses within the brain, such as brain tumors, have to be removed with precision, the drive mechanism has a localizing surgical retractor **1210** mounted in place of the insertion tube, and base platter **1220** has a large central opening through which the retractor passes. Retractor **1210** includes three or more spatulas **1212** inserted through base platter **1220** and the entry column. Each spatula **1212** includes a tracking LED **1214** attached to it. The relationship of the spatulas is controlled by a screw assembly **1216** that allows the relative distance between the spatulas to be modified. Relatively small movement at the screw assembly results in a larger movement at the other ends of the spatulas due to the pivoting of the spatulas within the retractor. Tracking LEDs **1214** are tracked by the camera array and the localization application computes the depth of spatulas **1212** and their displacement from the central axis. Using the tracking

approach described above, surgical localizing retractor **1210** is directed towards the brain target. Upon acquiring the target, screw assembly **1216** is adjusted to expand localizing retractor **1210** to allow visualization of the underlying brain. A variety of surgical instruments can be attached to retractor **1210** in addition to using the retractor with more conventional manual techniques. These instruments can include an endoscope, an ultrasonic aspirator, an electronic coagulation/evaporator/ablator, or a laser.

[0111] An optional fixture validation step (**FIG. 1**, step **130**) can be used to confirm that the position of the tip of the surgical instrument is accurately tracked. Two types of validation can be performed. Referring to **FIG. 18**, guidance fixture **710** is attached to an upper mounting plate **1334** of a calibration jig **1330**. Prior to attaching guidance fixture **710** to calibration jig **1330**, pivoting locking knob **846** (**FIG. 10**) is loosened allowing pivoting collar **840** to pivot. After guidance fixture **710** is attached, pivoting collar **840** is centered and pivoting locking knob **846** is tightened. A guidance tube **1340** is clamped into the guidance fixture, and a surgical instrument **1342** is passed through the guidance tube. Guidance tube **1340** protrudes below upper mounting plate **1334**. A ruler **1335** can then be used to measure the depth of penetration of the guidance tube. Similarly, ruler **1335** can be used to measure the penetration of surgical instrument **1342**.

[0112] Referring to **FIG. 19**, a validation (or “phantom”) jig **1312** can also be used. Tracking MIRROR **510** is attached to validation jig **1312**. Guidance fixture **710** is mounted on validation jig **1312**. A phantom target point **1320** at a known position relative to validation jig **1312**, and therefore at a known position relative to the fiducial points on tracking MIRROR **510**, is chosen. The localization application **588** is programmed with the phantom target position. Using the procedure that will be used during the surgical phase, the surgeon performs the registration and alignment steps and then drives the instrument through guidance fixture **710**. If the tip of the instrument is coincident with the phantom target point, then guidance fixture **710** is validated. If for some reason the instrument is not coincident with the phantom target point, for example, due to improper attachment of the instrument to the drive assembly resulting in an incorrect depth calibration, the surgeon readjusts the instrument and attempts the validation step again.

[0113] Other embodiments of the invention use alternative scanning, registration, and tracking markers, and methods of scanning and registration.

[0114] In the first embodiment, scanning MIRROR **310** and tracking MIRROR **510** are star-shaped. Other alternative shapes of MIRRFS can be used. Referring to **FIG. 20**, an arc-shaped MIRROR **1410** is attached to threaded inserts **1420** using bolts **1430**, and marking and locking nuts **1432**. Arc-shaped MIRROR **1410** includes scanning fiducial markers **1412**. The fiducial markers are more widely spaced than in star-shaped MIRRFS **310**, and **510**, resulting in a more accurate tracing of the MIRROR. During insertion of threaded inserts **1420**, arc-shaped MIRROR **1410** acts as a template for accurate positioning of the threaded inserts.

[0115] In embodiments described above, threaded inserts are inserted into the skull to provide the fixed points of attachment for MIRRFS. Alternative embodiments use other types of anchors or forms of mechanical attachment. Pro-

truding posts can be attached to the skull. A MIRROR is then attached to the posts. Also, inserts can be implanted in the skull which provide precisely positioned “divots.” These divots are used to mate clamping posts on a MIRROR, which hold the MIRROR in place. Such implanted divots can be covered by the skin and remain in place for an extended period of time.

[0116] An alternative to use of a MIRROR is to attach markers directly to anchors in the skull. Referring to **FIG. 21**, each such anchor, shown as threaded insert **1440**, can support a single scanning marker **1444** on a post **1442**, subsequently support a single registration divot **1450** on a second post **1451**, and then support a single tracking marker, LED **1448**, on a third post **1446**. The geometric relationship of the anchor to the scanning marker is the same as the geometric relationship of the anchor to the tracking marker thereby allowing a localization application to directly track the fiducial points by tracking the location of the tracking marker.

[0117] Using any of the MIRROR structures described, multiple MIRRFS can be used to provide increased accuracy in registration and tracking. For example, two star-shaped MIRRFS can be used, one on each side of the head.

[0118] In other embodiments, alternative attachment methods can be used to secure a guidance fixture to the skull. For instance, the mounting base can be relatively small and have extended “legs” extending radically and secured to the skin or skull with sharp points. These legs provide stabilization that may not be achievable using mounting screws through the smaller mounting base. The mounting base can alternatively include an insert that fits into the burr hole. This insert can also be threaded to allow direct attachment of the mounting base to the burr hole.

[0119] In other embodiments, threaded inserts are used to attach, and subsequently accurately reattach, conventional stereotactic frames. This allows the conventional stereotactic frame to be removed and then accurately reattached to the skull. Procedures, such as fractionated multi-day stereotactic radiation treatments could then be performed with the stereotactic frame being reattached for each treatment.

[0120] Referring to **FIG. 22**, a modified guidance fixture **1510** is used in combination with a conventional stereotactic frame **1520**. Guidance fixture **1510** includes an x-y positioning table with LEDs **1512** and an instrument drive with an LED **1514** for tracking the depth of the surgical instrument. The guidance assembly is positioned on frame **1520** to align with the planned surgical trajectory. A tracking MIRROR **1530** is attached to frame **1520** to allow dynamic tracking.

[0121] Rather than using a scanning MIRROR with scanning fiducial markers, or scanning fiducial markers attached directly to anchors embedded in the skull, alternative embodiments can use other features for registration. In one alternative embodiment, paste-on scanning markers are attached to the skin. During the registration phase, the cranial probe is positioned at each of the paste-on markers in turn, rather than at the fiducial points on a MIRROR. Tracking LEDs are attached in a fixed position relative to the skull in some other way than using a MIRROR, for example, using an elastic headband. Rather than using pasted on fiducial markers, another alternative embodiment uses accessible anatomical features. These features are located in

the scanned image, and the probe is positioned at these features during the registration phase. Still another alternative does not use discrete fiducial points, but rather makes use of the surface shape of the skull in a "surface merge" approach. The surface of the skull is located in the three-dimensional image. During registration, the cranial probe touches a large number of points on the skull. The locations of these points is matched to the shape of the skull to determine the conformal mapping from the physical coordinate system to the image coordinate system.

[0122] In yet another embodiment, referring to FIG. 23, a tracking MIRROR 1610 can be attached directly to the base of a guidance fixture 710. Tracking MIRROR 1610 is only useful for tracking after guidance fixture 710 has been attached to the skull. In this approach, registration is based on fiducial points elsewhere on the skull than tracking MIRROR 1610.

[0123] Locating the entry point, over which guidance fixture 710 is attached can be accomplished using one of a variety of alternative techniques. For example, the entry point may be known-for some standardized procedures. Alternatively, the entry point may be determined by registration of the skull and the three-dimensional image based on fiducial markers attached to the head, for example using adhesive pads, anatomical markers, or a "surface merge" technique as described above.

[0124] Once the guidance fixture and tracking MIRROR 1610 are attached to the skull, LEDs 1620 on tracking MIRROR 1610 are used to track the location of the skull, and thereby track the location of the surgical instrument. A reregistration step (FIG. 1, step 160) can be performed to determine the relative position of the fiducial points to LEDs 1620.

[0125] Various mechanical adjustments of guidance fixture 710, if performed when an guidance tube is inserted in the brain, would potentially damage the brain tissue. The guidance fixture optionally includes a feature that the various locking knobs and x-y adjustment knobs are rotated using a removable knob (or key). When not in use, this knob is stowed on the drive assembly. Whenever the removable knob is removed from its stowed position, the signal from an electrical sensor on the drive assembly that is connected to the workstation causes a warning, for example on the computer display, to be provided to the surgeon.

[0126] Alternative related embodiments can make use of known geometric relationships of points on various devices.

[0127] For instance, the relationship between the tip of a probe and the location of tracking LEDs can be calibrated and used by a localization application to compute the location of tip using the computed location the LEDs. Similarly, the relationship between the location of fiducial points on a MIRROR and tracking LEDs can be calibrated, thereby allowing a localization application to compute the coordinates of fiducial points from the coordinates of the tracking LEDs without using the registration procedure described above.

[0128] In the above embodiments, tracking LEDs are tracked using a camera. Other alternative embodiments can use other three-dimensional sensing and tracking approaches. Rather than LEDs, other tracking markers that are active emitters of electromagnetic-or mechanical energy such as electronic sparks, heat, magnetic energy, or sound

can be used. Appropriate three-dimensional tracking approaches, for example, using imaging or triangulation techniques determine the three-dimensional coordinates of the emitters. Alternatively, tracking markers that are passive reflectors or transducers of externally applied localizing energy, such as infrared light, sound, magnetism, can be used.

[0129] The devices described above can be made of a variety of materials. One alternative is to use a material, such as carbon fiber, which does not interfere with MRI scanning. This allows use of the devices during intraoperative MRI scanning. Also, use of hydraulic drive mechanisms rather than electrical motors avoids interference with MRI scanning.

[0130] In the surgical procedures described above, the patient is not necessary immobilized. It may be desirable, however, to immobilize the patient, for example by clamping the guidance fixture to an operating table, at some times during the surgery.

[0131] It is to be understood that the foregoing description is intended to illustrate and not limit the scope of the invention, which is defined by the scope of the appended claims. Other aspects, advantages, and modifications are within the scope of the following claims.

What is claimed is:

1. A method for positioning a surgical instrument during stereotactic surgery, comprising:

providing a guidance fixture that includes an upper portion, including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion, and includes an adjustable base supporting the upper portion, including a mounting base and an adjustment mechanism;

attaching the guidance fixture to a body, including attaching the mounting base to the body;

determining using a remote sensing device the orientation of the upper portion of the guidance fixture in relation to the body;

displaying a representation of a relationship of the constrained trajectory and a target point in the body; and

aligning the guidance fixture, including aligning the orientation of the upper portion to achieve a desired relation between the constrained trajectory and the target point, including rotating the upper portion about a central axis of the mounting base and pivoting the upper portion to adjust an angle between the upper portion and the central axis.

2. The method of claim 1 wherein determining the orientation of the upper portion includes:

determining the locations of a first plurality of tracking markers affixed to the upper portion;

determining the locations of a second plurality of tracking markers affixed to the body; and

computing the orientation using the locations of the first and the second pluralities of tracking markers.

3. The method of claim 1 further comprising:

locking the adjustment mechanism to fix the orientation of the upper portion in relation to the body;

- determining a displacement of the surgical instrument along the constrained trajectory;
- displaying a representation of a location of the surgical instrument in relation to the body;
- guiding the surgical instrument into the body along the constrained trajectory.
- 4.** The method of claim 3 wherein determining the displacement of the surgical instrument includes:
- determining using a remote sensing device a location of a tracking marker affixed in a fixed relationship to the surgical instrument;
- determining the locations of a plurality of tracking markers affixed to the guidance assembly; and
- computing the displacement using the location of the marker affixed in a fixed relationship to the surgical instrument and the locations of the plurality of tracking markers affixed to the guidance assembly.
- 5.** A method for positioning a surgical instrument during stereotactic surgery comprising:
- providing a guidance fixture that includes an upper portion, including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion, and includes an adjustable base supporting the upper portion, including a mounting base and an adjustment mechanism;
- attaching the guidance fixture to a body, including attaching the mounting base to the body;
- determining using a remote sensing device the orientation of the upper portion of the guidance assembly in relation to the body;
- displaying a representation of a relationship of the constrained trajectory and a target point in the body; and aligning the guidance fixture, including aligning the orientation of the upper portion to achieve a desired relation between the constrained trajectory and the target point;
- attaching at an attachment location on the body a scanning frame that includes a plurality of scanning markers;
- scanning a three-dimensional image of the body, including locating images of the scanning markers in the three-dimensional image;
- attaching to the body a tracking frame that includes a plurality of tracking markers; and
- registering the body and the three-dimensional image, including tracking the tracking markers in the tracking frame, and locating points relative to the body which correspond to the locations of the scanning markers.
- 6.** The method of claim 5 wherein attaching the tracking frame includes attaching the tracking frame in a predetermined location in relation to the attachment location of the scanning frame.
- 7.** The method of claim 5 wherein locating points relative to the body which correspond to the locations of the scanning markers includes:
- tracking the location of a point on a probe using the remote sensing device;
- positioning the point on the probe at each of the points on the body corresponding to the scanning markers.
- 8.** The method of claim 5 wherein locating points on the body includes computing the locations of points relative to the body which correspond to the locations of the scanning markers using a known geometry relationship of the locations of the scanning markers on the attached scanning frame and the locations of the tracking markers on the attached tracking frame.
- 9.** The method of claim 1 wherein displaying the representation of the relationship of the constrained trajectory and the target point includes
- displaying a representation of the target point,
- displaying a representation of the range of possible orientations of the guidance fixture,
- displaying a first line segment corresponding to possible orientations of the guidance fixture that could result from pivoting the upper portion at a current degree of rotation of the upper portion, and
- displaying an indication of a current degree of pivoting of the upper portion.
- 10.** A guidance fixture for guiding a surgical instrument into a body during stereotactic surgery, comprising:
- an upper portion including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion;
- an adjustable base supporting the upper portion, including a mounting base for attaching the guidance fixture to a body, the mounting base having central opening and a central axis passing through the central opening, and an orientation adjustment mechanism coupled between the mounting base and the upper portion, a configuration of the adjustment mechanism determining the orientation of the upper portion relative to the mounting base; and
- a plurality of tracking markers for tracking with a remote sensing device.
- 11.** The guidance fixture of claim 10 wherein the plurality of tracking markers includes a plurality of light emitting diodes and the remote sensing device includes a plurality of cameras.
- 12.** A guidance fixture for guiding a surgical instrument into a body during stereotactic surgery, comprising:
- an upper portion including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion;
- an adjustable base supporting the upper portion, including a mounting base for attaching the guidance fixture to a body, the mounting base having central opening and a central axis passing through the central opening, and an orientation adjustment mechanism coupled between the mounting base and the upper portion, a configuration of the adjustment mechanism determining the orientation of the upper portion relative to the mounting base;
- wherein the orientation adjustment mechanism includes a rotation adjustment mechanism and a pivoting adjustment mechanism, wherein adjustment of the rotation adjustment mechanism rotates the upper portion about the central axis, and adjustment of the pivoting adjust-

ment mechanism adjusts an angle between the upper portion and the central axis.

**13.** The guidance fixture of claim 12 wherein the rotation adjustment mechanism includes a rotating collar attached to the mounting base and the pivoting adjustment mechanism includes a pivoting collar coupling the rotating collar to the upper portion.

**14.** The guidance fixture of claim 13 wherein the adjustable base further includes a rotation locking screw for preventing rotation of the rotating collar and a pivoting locking screw for preventing pivoting of the pivoting collar.

**15.** The guidance fixture of claim 14 wherein the upper portion includes an x-y table adjustment of which displaces the constrained trajectory.

**16.** A guidance fixture for guiding a surgical instrument into a body during stereotactic surgery, comprising:

an upper portion including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion wherein the instrument guide includes a driving mechanism for positioning the instrument along the constrained trajectory; and

an adjustable base supporting the upper portion, including a mounting base for attaching the guidance fixture to a body, the mounting base having central opening and a central axis passing through the central opening, and an orientation adjustment mechanism coupled between the mounting base and the upper portion, a configuration of the adjustment mechanism determining the orientation of the upper portion relative to the mounting base.

**17.** The guidance fixture of claim 16 wherein the constrained trajectory is a linear trajectory.

**18.** The guidance fixture of claim 16 wherein the upper portion includes a plurality of tracking markers and the driving mechanism includes an instrument tracking marker for tracking a location of the instrument using a remote sensing device.

**19.** A system for stereotactic surgery on a body, comprising:

a remote sensing device;

a tracking frame for attachment to the body, including a plurality of tracking markers for tracking a location and an orientation of the body by using the remote sensing device;

a guidance fixture including

an upper portion including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion,

an adjustable base supporting the upper portion, including a mounting base for attaching the guidance fixture to a body, the mounting base having central opening and a central axis passing through the central opening, and an orientation adjustment mechanism coupled between the mounting base and the upper portion, configuration of the adjustment mechanism determine the orientation of the upper portion relative to the mounting base, and

a plurality of tracking markers for tracking a location of the upper portion of the guidance fixture; a tracking system for accepting the locations of the tracking markers on the tracking frame and the locations of the

tracking markers on the guidance fixture, and computing a geometric relationship between the constrained trajectory and the body; and

a display system for presenting an image of the body and the geometric relationship between the constrained trajectory and the body.

**20.** The system of claim 19 wherein the remote sensing device includes a plurality of cameras, and the tracking markers are light emitting diodes.

**21.** A method for positioning a surgical instrument during stereotactic surgery, comprising:

providing a guidance fixture that includes an upper portion, including an instrument guide for moving the surgical instrument along a constrained trajectory relative to the upper portion, and includes an adjustable base supporting the upper portion, including a mounting base and an adjustment mechanism;

attaching the guidance fixture to a body, including attaching the mounting base to the body;

sensing using a remote sensing device locations of a plurality of tracking markers affixed to the upper portion of the guidance fixture;

determining a location and an orientation of the upper portion using the plurality of sensed locations of the tracking markers;

sensing using the remote sensing device a location of a tracking marker affixed to the instrument guide; determining a location of the instrument using the determined location and orientation of the upper portion and the sensed location of the tracking marker affixed to the instrument guide.

**22.** An adjustable guidance fixture for stereotactic surgery comprising:

an upper portion including an instrument guide for moving a surgical instrument along a constrained trajectory relative to the upper portion;

an adjustable base, including a mounting base for attaching the guidance fixture to a body, and an orientation adjustment mechanism coupled between the mounting base and the upper portion;

a plurality of tracking markers affixed to the upper portion for tracking a location and an orientation of the upper portion using a remote sensing device; and

a tracking marker affixed to the instrument guide for tracking a motion of the surgical instrument using the remote sensing device.

**23.** A method for adjusting a guidance fixture for stereotactic surgery, comprising:

attaching the guidance fixture to the body at an entry point to the body, the guidance fixture having an adjustable orientation;

displaying a planar section of a three-dimensional image of the body, including displaying a representation of the orientation of the guidance fixture, the planar section containing a target point within the body;

adjusting the orientation of the guidance fixture using a first constrained motion of the guidance fixture until the orientation lies in a plane corresponding to the displayed planar section;

adjusting the orientation of the guidance fixture using a second constrained motion of the guidance fixture, such that the orientation continues to lie in the plane corresponding to the displayed planar section, until the orientation passes through the target point.

**24.** A guidance fixture for stereotactic surgery on a body, comprising:

an instrument guide for moving a surgical instrument along a constrained trajectory relative to the instrument guide;

an adjustable base supporting the instrument guide, including a mounting base having a central axis and an adjustment mechanism coupled between the mounting base and the instrument guide, wherein a configuration of the adjustment mechanism determines an orientation of the instrument guide relative to the central axis of the mounting base; and

a signaling device for providing a signal representation of the configuration of the adjustment mechanism;

wherein the adjustment mechanism includes a rotation adjustment mechanism and a pivoting adjustment mechanism, adjustment of the rotation adjustment mechanism rotates the instrument guide about the central axis, and adjustment of the pivoting adjustment mechanism adjusts an angle between the instrument guide and the central axis.

**25.** The guidance fixture of claim 24 wherein the mounting base includes a portion for mating directly with the body.

**26.** A guidance fixture for stereotactic surgery on a body, comprising:

an instrument guide for moving a surgical instrument along a constrained trajectory relative to the instrument guide;

an adjustable base supporting the instrument guide, including a mounting base having a central axis and an adjustment mechanism coupled between the mounting base and the instrument guide, wherein a configuration of the adjustment mechanism determines an orientation of the instrument guide relative to the central axis of the mounting base; and

a signaling device for providing a signal representation of the configuration of the adjustment mechanism wherein the signaling device includes a plurality of tracking markers and the signal representation of the configuration includes a plurality of signals propagating from corresponding tracking markers.

**27.** The guidance fixture of claim 26 wherein at least some of the plurality of tracking markers are in fixed locations relative to the instrument guide.

**28.** The guidance fixture of claim 26 wherein the signals propagating from the tracking markers are electromagnetic signals.

**29.** The guidance fixture of claim 26 wherein the tracking markers are light emitting diodes and the signals propagating from the tracking markers are optical signals.

**30.** The guidance fixture of claim 26 wherein the signals propagating from the tracking markers are acoustic signals.

**31.** The guidance fixture of claim 10 wherein the tracking markers emit signals to the remote sensing device.

**32.** The guidance fixture of claim 10 wherein the tracking markers reflect signals to the remote sensing device.

\* \* \* \* \*