



(51) International Patent Classification:

A61B 1/00 (2006.01) A61B 1/04 (2006.01)

(21) International Application Number:

PCT/US2017/044401

(22) International Filing Date:

28 July 2017 (28.07.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/368,582 29 July 2016 (29.07.2016) US

(71) Applicant: UNIVERSITY OF FLORIDA RESEARCH FOUNDATION, INCORPORATED [US/US]; 223 Grinter Hall, Gainesville, FL 32611 (US).

(72) Inventors: XIE, Huikai; 1124 S.W. 90th Terrace, Gainesville, FL 32607 (US). KOPPAL, Sanjeev, Jagannatha; 621 NE Boulevard, Gainesville, FL 32601 (US). ZHANG, Xiaoyang; 332 University Village Apartment, Gainesville, FL 32611 (US). ZHOU, Liang; 4000 SW 37th

Blvd Apt. 518, Gainesville, FL 32608 (US). DUAN, Can; 10131 Brentridge Ct., Dallas, TX 75243 (US).

(74) Agent: FRANK, Louis, C. et al.; Saliwanchik, Lloyd & Eisenschenk, P.O. Box 142950, Gainesville, FL 32614-2950 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,

(54) Title: ENDOSCOPIC OCT PROBES WITH IMMERSED MEMS MIRRORS

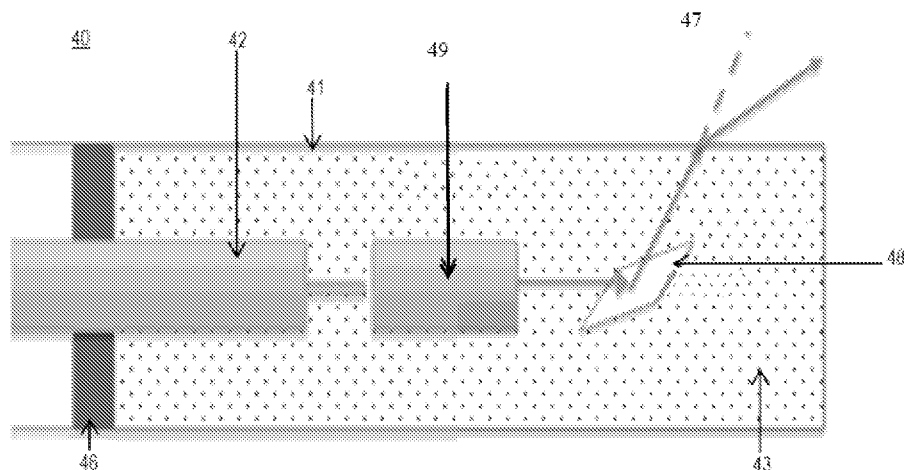


Figure 7

(57) Abstract: Methods and apparatuses for enlarging the optical scan angle of imaging probes are provided. The optical scan angle of endoscopic probes can be increased by employing the "Snell's Window" effect. An endoscopic probe can include an endoscope shell, a means for capturing electromagnetic radiation, and a liquid or gel provided between the means for capturing electromagnetic radiation and the endoscope shell. The endoscope probe can further include a first mirror placed such that electromagnetic radiation entering through the endoscope shell can bounce off the first mirror and enter the means for capturing electromagnetic radiation. The first mirror can be a microelectromechanical systems (MEMS) mirror.

EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

DESCRIPTION

ENDOSCOPIC OCT PROBES WITH IMMERSED MEMS MIRRORS

5

CROSS-REFERENCE TO RELATED APPLICATION

This application claims the benefit of U.S. Provisional Patent Application Serial No. 62/368,582, filed July 29, 2016, which is incorporated herein by reference in its entirety, including any figures, tables, and drawings.

10

STATEMENT OF GOVERNMENT SUPPORT

This invention was made with government support under 1514154 and 1512531 awarded by the National Science Foundation. The government has certain rights in the invention.

15

BACKGROUND OF THE INVENTION

Optical coherence tomography (OCT) is an established biomedical imaging technique which is able to obtain *in vivo*, real-time cross-sectional information of biological tissues with high resolution. Electrothermal microelectromechanical systems (MEMS) mirrors have been extensively used in endoscopic OCT imaging probes due to their small size, large linear range, low voltage and high fill factor. As one featured application, endoscopic OCT can be employed for internal organ imaging to aid in early stage cancer detection. Although OCT has proven to be a useful tool, one of the major challenges is assembling optical scan components into an endoscopic imaging probe that is less than a few millimeters in size. In addition, due to the relatively small mechanical rotation angle of MEMS mirrors as well as the size constraints of endoscopic imaging probes, the optical scan angle is limited. Therefore, there is always a need for methods and apparatuses to enhance the optical scan angle of imaging probes while still maintaining their compact size.

20

25

30

BRIEF SUMMARY

Embodiments of the present invention include methods and apparatuses for enlarging the optical scan angle of imaging probes. Embodiments of the present invention

can increase the optical scan angle of imaging probes with electrothermal MEMS mirrors by employing the “Snell’s Window” effect and reduce the number of insertions required for an imaging probe to completely capture the full-circumferential image of a tubular organ like an esophagus or a bronchia. Embodiments of the present invention include an MEMS OCT imaging probe that can produce a full scan of a lumen in one insertion. In addition, by immersing an MEMS mirrors in liquid, shock resistance can also be increased.

According to embodiments of the present invention, the field of view (FOV) of an endoscope probe can be increased by utilizing a liquid within an endoscopic shell. The scan range can be enlarged by harnessing the advantages of Snell’s window effect. Embodiments of the present invention can be used in OCT imaging systems.

According to an embodiment of the present invention, an endoscopic probe can include an endoscope shell, a means for capturing electromagnetic radiation, and a liquid or gel provided between the means for capturing electromagnetic radiation and the endoscope shell. The liquid or gel may completely or partially immerse the means for capturing electromagnetic radiation. The endoscopic probe can further include a first mirror placed such that electromagnetic radiation entering through the endoscope shell can bounce off the first mirror and enter the means for capturing electromagnetic radiation, and the first mirror can be a microelectromechanical systems mirror. A lens can be included between the means for capturing electromagnetic radiation and the first mirror, and the lens can be a gradient-index (GRIN) lens. The means for capturing electromagnetic radiation can be a fiber (e.g., a single mode fiber (SMF)), a camera, or some other means. The endoscopic probe can be configured to be side-viewing and forward-viewing. The first mirror can tilt in one direction, two directions, and can be raised and lowered. A means for tilting or raising the first mirror can be bimorph actuator(s) and piezo electric crystal(s). For a specific example, the means for tilting or raising the first mirror can be inverted-series-connected (ISC) Al/SiO₂ bimorph actuators. A second mirror can also be included that is positioned to reflect electromagnetic radiation coming from the first mirror and to the means for capturing electromagnetic radiation. In some embodiments, a prism can be used as the first mirror.

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a scanning electron microscope (SEM) image of an inverted-series-connected (ISC) two-axis electrothermal MEMS mirror according to an embodiment of the present invention.

Figure 2a and **Figure 2b** show the principles of the “Snell window” effect.

Figure 3 is a graph showing the static response of an MEMS mirror in both air and mineral oil.

Figure 4a shows an experimental setup of an imaging probe according to an embodiment of the present invention.

Figure 4b is an image showing a laser used to visualize the enlarged optical scan angle in an imaging probe according to an embodiment of the present invention.

Figure 5a is a 2D optical coherence tomography (OCT) image of a piece of paper captured using an imaging probe according to an embodiment of the present invention.

Figure 5b is a 3D optical coherence tomography (OCT) image of a piece of paper captured using an imaging probe according to an embodiment of the present invention.

Figure 6a and **Figure 6b** show side-viewing OCT imaging probes.

Figure 7 is a schematic diagram of a side-viewing imaging probe according to an embodiment of the present invention.

Figure 8 illustrates basic concepts of the present invention, with an MEMS mirror directing a light beam through a liquid and toward an optical window, resulting in an amplified scan angle for both axes.

Figure 9 is forward-viewing probe with an MEMS mirror and a fixed mirror in liquid, according to an embodiment of the present invention.

Figure 10 is a forward-viewing probe with an MEMS mirror and a fixed mirror in liquid, according to an embodiment of the present invention.

DETAILED DESCRIPTION

According to an embodiment of the present invention, an endoscopic probe can include an endoscope shell, a means for capturing electromagnetic radiation, and a liquid or gel provided between the means for capturing electromagnetic radiation and the endoscope shell. The endoscopic probe can further include a first mirror placed such that electromagnetic radiation entering through the endoscope shell can bounce off the first

mirror and enter the means for capturing electromagnetic radiation, and the first mirror can be a microelectromechanical systems mirror. A lens can be included between the means for capturing electromagnetic radiation and the first mirror, and the lens can be a gradient-index (GRIN) lens. The means for capturing electromagnetic radiation can be a fiber (e.g., a single mode fiber (SMF)) or a camera. The endoscopic probe can be configured to be side-viewing and forward-viewing. The first mirror can tilt in one direction, two directions, and can be raised and lowered. A means for tilting or raising the first mirror can be bimorph actuator(s) and piezo electric crystal(s). In a specific example, the means for tilting or raising the first mirror is are inverted-series-connected (ISC) Al/SiO₂ bimorph actuators. A second mirror can also be included that is positioned to reflect electromagnetic radiation coming from the first mirror and to the means for capturing electromagnetic radiation. The second mirror can also be configured to tilt and rise. Examples of the electromagnetic radiation that can be captured include visible light, ultraviolet (UV) light, infrared red, and near infrared light. In different embodiments, the first mirror and the second mirror can both tilt and rise, only one of the first or second mirrors can tilt or raise, or both mirrors can be fixed. The endoscope shell can be made of any materials known in the art including plastics, metals, glass, and ceramics, and the endoscopic shell can have a cross section that is oval or round. The endoscopic probe can further have a flattened optical window as well as a means of delivering electromagnetic radiation. The means for delivering electromagnetic radiation can include a fiber bundle that can both deliver and capture electromagnetic radiation. For instance, the fiber bundle can have a center fiber delivering light and surrounding fibers that capture the image, or vice versa. In some embodiments, a prism can be used as the first mirror, the second mirror, or for both the first and second mirror.

According to another embodiment of the present invention, an endoscopic probe can include an endoscope shell, an optical window, a fiber module, and a liquid or gel provided between the optical window and the endoscope shell. The endoscopic probe can further include a first mirror placed such that electromagnetic radiation, e.g., near infrared light, entering the endoscope shell through the fiber module can bounce off the first mirror, and the first mirror can be a microelectromechanical systems (MEMS) mirror. The fiber module consists of an optical fiber and a lens, and the lens can be a gradient-index (GRIN) lens. The fiber can be a single mode fiber (SMF)). The endoscopic probe can be

configured to be side-viewing and forward-viewing. The first mirror can tilt in one direction, two directions, and can be raised and lowered. A second mirror can also be included that is positioned to reflect electromagnetic radiation coming from the first mirror and to the optical window. The second mirror can also be configured to tilt and rise. Examples of the electromagnetic radiation that can be captured include visible light, ultraviolet (UV) light, infrared red, and near infrared light. In different embodiments, the first mirror and the second mirror can both tilt and rise, only one of the first or second mirrors can tilt or raise, or both mirrors can be fixed. The endoscope shell can be made of any materials known in the art including plastics, metals, glass, and ceramics, and the endoscopic shell can have a cross section that is oval or round. The endoscopic probe can further have a flattened optical window.

Electrothermal bimorph MEMS mirrors according to the present invention can have a gap **11** between the mirror plate **10** and the substrate **12**, as shown by a two-axis electrothermal bimorph MEMS mirror in Figure 1. In Figure 1, it can be seen that the mirror plate **10** is elevated above the silicon substrate **12**, leaving a gap **11** underneath the mirror plate **10**. The gap **11** allows a space for liquid to fill-in and reduces the squeeze-film damping. The gap **11** also allows the mirror plate **10** to rotate in liquid without serious stiction problems, which can also be alleviated by having an appropriately sized gap.

In Figure 1, four inverted-series-connected (ISC) Al/SiO₂ bimorph actuators **13** are connected at the middle points of the four sides of the mirror plate **10** to provide out-of-plane displacement. The four actuators **13** can be separately controlled to realize tip and tilt of the mirror plate **10**. Other types of actuators may also be used in the embodiments of the present invention (e.g., piezo electric actuators or electromagnetic actuators).

A liquid may be used to cover the mirror plate **10** and expand the field of view (FOV) of the mirror via the Snell's Window effect. For example, a mineral oil may be used to immerse the MEMS mirror as it is transparent and also has an effective refractive index of 1.5. Mineral oil has shown to work well in the 1,300 nm wavelength range, but other liquids can be applied and selected for their suitability depending on what wavelength range is desired to be captured. That is, instead of mineral oil, other types of liquids with varying refractive indexes can be applied in the embodiments of the present invention (e.g., water, ethylene glycol, glycerin, vegetable oils, propylene glycol, etc.). In addition, more than one liquid may be combined to form a mixture. Preferably, any liquids used would be

non-toxic in case they were to leak while the device was in operation. A liquid used in the present invention can have refractive indices of, for example, any of the following values, about any of the following values, at least any of the following values, at least about any of the following values, not more than any of the following values, not more than about any of the following values, or within any range having any of the following values as endpoints (with or without “about” in front of one or both of the endpoints), though embodiments are not limited thereto: 1.05, 1.10, 1.15, 1.20, 1.25, 1.30, 1.35, 1.40, 1.45, 1.50, 1.55, 1.60, 1.65, 1.70, 1.75, 1.80, 1.85, 1.90, 1.95, and 2.00 . For example, a liquid used in the present invention can have a refractive index of 1.30, about 1.30, at least 1.30, no more than 1.30, or from 1.20 to 1.40 (inclusive).

A schematic diagram of the physical principles embodied in the present invention can be seen in Figure 2a. When the mirror plate has a mechanical tilt angle θ_M , the output optical angle θ_R becomes $\arcsin[n \times \sin(2\theta_M)]$. When θ_M reaches the critical angle, which is 20.9° for mineral oil, θ_R becomes 90° and is more than twice as much as the optical scan angle of 41.8° in air.

For the inverted-series-connected (ISC) MEMS mirror shown in Figure 1, its maximum mechanical tilt angle range is $\pm 8^\circ$. Therefore, the mirror has a total mechanical tilt of 16° , which is smaller than the critical angle. As can be seen in Figure 2a, angle amplification increases when θ_M approaches the critical angle. Thus, in order to maximize the FOV, an oblique incidence is used. As shown in Figure 2b, the light is incident on the mirror plate at 25.8° . In this arrangement, the output optical beam scans the liquid/air boundary from 9.8° to 41.8° when the mirror tilts from -8° to $+8^\circ$. Thus, the theoretical maximum output FOV reaches 75° , which is about 2.3 times the FOV for the mirror in air.

The static angular tilt angle response of an MEMS mirror in air and mineral oil is shown in Figure 3, where only one of the four actuators was excited. The maximum optical scan angle on a single side reached 16.6° at 5.6 V in air and 25.4° at 9 V in oil. The corresponding maximum mechanical tilt angle of the mirror is 8.3° in both air and mineral oil.

Although specific tilt angles, tilting mechanisms, and voltages are given for the working prototype embodiment of Figure 1, these figures are only examples and are not intended to limit the present invention. That is, the tilt angles, tilting mechanisms, and voltages applied can be selected depending on the application of each embodiment.

In general, there are two different types of endoscopic imaging probes, side-viewing and forward-viewing, both of which can be implemented in embodiments of the present invention. Two exemplified side-viewing probes are illustrated in Figures 6a and 6b. The embodiment in Figure 6a has an MEMS mirror **101** placed on a 45° slope and is electrically connected through a flexible printed circuit board (FPCB) **102** while the embodiment in Figure 6b has an MEMS mirror **201** with the mirror plate tilted 45° and integrated on a silicon optical bench **202**. Both embodiments can have internal electrical wiring, **103** and **203**, for control of the mirrors, **101** and **201**, and a support framework **104** for supporting the mirrors, substrate, fiber (and/or camera), and lens (the support framework is not shown in Figure 6b). In either the embodiment of Figure 6a or Figure 6b, a liquid can be filled and sealed in the endoscope shells, **105** and **205**, as shown in Figure 7.

Figure 7 is a schematic diagram of a side-viewing imaging probe **40** (or endoscope) according to an embodiment of the present invention. Figure 7 shows an endoscope shell **41**, a lens **49** (which can be a GRIN lens), a fiber **42** or a camera to collect incoming electromagnetic radiation, a liquid **43** within the endoscope shell **41**, and a seal ring **46** that forms a barrier to keep the liquid **43** in place and separated from the rest of the endoscope **40**. The outside perimeter of the endoscope shell **41** can take a multitude of shapes, including but not limited to a circle, an oval, a square or a rectangle, and its edges can be smoothed. If the perimeter of the endoscope shell **41** is an oval or a circle, there can be a flattened window where light can pass through the endoscopic shell and lands on the articulating mirror **48**, which may be an MEMS mirror. Examples of electromagnetic radiation that can be utilized in the embodiments of the present invention include but are not limited to ultra-violet radiation, infrared radiation, near infrared radiation and visible light.

Endoscope shells used in the present invention can have an outside diameter of, for example, any of the following values, about any of the following values, at least any of the following values, at least about any of the following values, not more than any of the following values, not more than about any of the following values, or within any range having any of the following values as endpoints (with or without “about” in front of one or both of the endpoints), though embodiments are not limited thereto (all measurements are in millimeters): 0.50, 1.0, 2.0, 3.0, 4.0, 5.0, 6.0, 7.0, 8.0, 9.0, 10.0, 11.0, 12.0, 13.0, 14.0, and 15.0. For example, an endoscope shell according to the present invention can have an

outside diameter of 10.0 mm, about 10.0 mm, at least 10.0 mm, no more than 10.0, or from 8.0 mm to 10.0 mm (inclusive).

In order to improve the scan angle amplification effect, a flat optical window can be incorporated into the endoscope shell. This is especially true when the tubing is not transparent. For example, the endoscope shell can be made of circular stainless steel tubing with a glass or plastic flat viewing window. When a flat window is placed in front of a mirror plate and a liquid is filled in between the window and the mirror plate, the Snell refraction angle amplification occurs for both scan directions, as illustrated in Figure 8.

There are various forward-viewing probe designs that can be applied to the embodiments of the present invention, one of which is illustrated in Figure 9. The incident light is reflected on a fixed mirror **20**, before landing on the MEMS mirror **21**, which then directs the light beam to scan forward. The endoscope shell **24** may be made of glass, metal, or metal with a glass window through which light can pass. Once the optical beam reaches the liquid/glass/air interface **22**, the scan angle can be increased. This embodiment can also include a camera or a fiber to collect electromagnetic radiation bouncing off the fixed mirror **20**. The embodiments of the present invention may also use the fiber or another fiber to deliver electromagnetic radiation (e.g., visible light) to the end of the endoscope.

Another design with a slightly slanted optical window is shown in Figure 10, including a fixed mirror **30**. The fixed mirror **30** can consist of a highly-reflective plate attached in front of the optical window. An endoscope shell **31** can be provided and can be made of glass, plastic, metal, or some combination of glass plastic and metal or other materials known in the art. For example, the sides of the probe may be made of metal while the tip of the probe can have a window **38**, which can be made of glass or plastic. A liquid **32** can be filled inside the endoscope shell **31** and can submerge the maneuverable mirror **34** (which can be an MEMS mirror, for example). Electrical wires **35** can be run through the probe to control the movement of the maneuverable mirror **34** in all of the embodiments of the present invention, as shown in Figure 10. A camera or a fiber **36** can be used to collect the electromagnetic radiation being reflected off of the fixed mirror **30**. A lens **37** can be provided in front of or attached to the fiber **36**,

and the lens **37** can be a gradient-index lens. A ferule **39** may also be provided as a support structure.

A greater understanding of the present invention and of its many advantages may be had from the following example, given by way of illustration. The following example is illustrative of some of the methods, applications, embodiments and variants of the present invention. It is, of course, not to be considered as limiting the invention. Numerous changes and modifications can be made with respect to the invention.

EXAMPLE 1

A proof of concept experiment was conducted including the fabrication of a prototype according to an embodiment of the present invention. The setup of an immersed two-axis MEMS mirror for OCT imaging experiment is shown in Figure 4a, where a single mode fiber (SMF) with a gradient-index (GRIN) lens glued on its tip was inserted in mineral oil and pointed to a mirror with a maximum FOV angle of 25.8° , as illustrated in Figure 2b. Figure 4b shows a picture in which a red laser is used to visualize the enlarged optical scan angle. Note that the incident laser beam approaches the experimental setup from a medium of air. The immersed MEMS mirror was then employed in an OCT system to perform a lateral scan for imaging a piece of paper. The details of the optics for the OCT are reported in Reference [2].

The 2D and 3D OCT images shown in Figure 5 were acquired with two differential ramp voltages (0-8 V) applied to four actuators with the frequencies of 1.25 Hz and 450 mHz, respectively. The width of the 2D OCT image is 3.3 mm and the height is 2.5 mm. The 3D image was achieved by stacking 100 frames of 2D OCT images with dimensions of 3.3mm by 3.3mm by 2.5 mm. The obtained FOV was about 62° .

The subject invention includes, but is not limited to, the following exemplified embodiments.

Embodiment 1. An endoscopic probe comprising:
an endoscope shell;
a means for capturing electromagnetic radiation; and

a liquid or gel (or both) provided between the means for capturing electromagnetic radiation and the endoscope shell.

Embodiment 2. The endoscopic probe of embodiment 1, further comprising a first mirror placed such that electromagnetic radiation entering through the endoscope shell can
5 bounce off the first mirror and enter the means for capturing electromagnetic radiation.

Embodiment 3. The endoscopic probe of embodiment 2, wherein the first mirror is a microelectromechanical systems (MEMS) mirror.

Embodiment 4. The endoscopic probe of any of embodiments 1 to 3, further comprising a lens between the means for capturing electromagnetic radiation and the first
10 mirror.

Embodiment 5. The endoscopic probe of embodiment 4, wherein the lens is a gradient-index (GRIN) lens.

Embodiment 6. The endoscopic probe of any of embodiments 1 to 5, wherein the means for capturing electromagnetic radiation is a fiber.

15 Embodiment 7. The endoscopic probe of embodiment 6, wherein the fiber is a single mode fiber (SMF).

Embodiment 8. The endoscopic probe of any of embodiments 1 to 7, wherein the endoscopic probe is configured to be side-viewing.

20 Embodiment 9. The endoscopic probe of any of embodiments 1 to 7, wherein the endoscopic probe is configured to be forward-viewing.

Embodiment 10. The endoscopic probe of any of embodiments 2 to 9, wherein the first mirror is configured to tilt in one direction.

Embodiment 11. The endoscopic probe of any of embodiments 2 to 9, wherein the first mirror is configured to tilt in two directions.

Embodiment 12. The endoscopic probe of any of embodiments 2 to 11, wherein the first mirror can be raised and lowered.

Embodiment 13. The endoscopic probe of any of embodiments 2 to 12, wherein a means for tilting or raising the first mirror is bimorph actuator(s).

5 Embodiment 14. The endoscopic probe of any of embodiments 2 to 12, wherein a means for tilting or raising the first mirror is piezo electric crystal(s).

Embodiment 15. The endoscopic probe of any of embodiments 2 to 12, wherein a means for tilting or raising the first mirror is inverted-series-connected (ISC) Al/SiO₂ bimorph actuator(s).

10 Embodiment 16. The endoscopic probe of any of embodiments 2 to 15, wherein the means for capturing electromagnetic radiation is a camera.

Embodiment 17. The endoscopic probe of any of embodiments 1 to 16, further comprising a second mirror positioned to reflect electromagnetic radiation coming from the first mirror and to the means for capturing electromagnetic radiation.

15 Embodiment 18. The endoscopic probe of any of embodiments 1 to 17, wherein the second mirror is configured to tilt.

Embodiment 19. The endoscopic probe of any of embodiments 1 to 18, wherein the electromagnetic radiation is visible light.

20 Embodiment 20. The endoscopic probe of any of embodiments 1 to 18, wherein the electromagnetic radiation is in the infrared range.

Embodiment 21. The endoscopic probe of any of embodiments 1 to 20, wherein both of the first and the second mirror are fixed.

Embodiment 22. The endoscopic probe of any of embodiments 1 to 21, wherein the endoscope shell is made of plastic, metal, or glass.

Embodiment 23. The endoscopic probe of any of embodiments 1 to 22, wherein a cross section of the endoscope shell is oval or round.

Embodiment 24. The endoscopic probe of any of embodiments 1 to 23, wherein the endoscope shell has a flattened optical window.

5 Embodiment 25. The endoscopic probe of any of embodiments 1 to 24, wherein the first mirror is fixed.

Embodiment 26. The endoscopic probe of any of embodiments 1 to 25, wherein the second mirror is fixed.

10 Embodiment 27. The endoscopic probe of any of embodiments 1 to 26, wherein the electromagnetic radiation is in the UV range.

Embodiment 28. The endoscopic probe of any of embodiments 1 to 27, further comprising a seal ring.

15 Embodiment 29. The endoscopic probe of any of embodiments 1 to 28, further comprising one or more optical fibers suitable for delivering electromagnetic radiation to the endoscopic probe.

Embodiment 30. The endoscopic probe of any of embodiments 1 to 29, wherein the camera has a means for tilting and raising and the means for tilting and raising can be piezoelectric and electromagnetic actuators.

20 Embodiment 31. The endoscopic probe of any of embodiments 1 to 30, further comprising a means for delivering electromagnetic radiation to the endoscopic shell.

Embodiment 31. The endoscopic probe of any of embodiments 1 to 30, wherein the means for delivering electromagnetic radiation to the endoscopic shell is an LED or an electromagnetic radiation transmitting fiber.

Embodiment 101. A method for capturing images using an endoscopic probe comprising:

providing a means for capturing electromagnetic radiation within an endoscope shell; and using the Snell's window effect to expand the field of view captured by the means
5 for capturing electromagnetic radiation.

Embodiment 102. The method for capturing images using an endoscopic probe of embodiment 101, further comprising providing a mirror placed such that electromagnetic radiation entering through the endoscope shell can bounce off the mirror and enter the means for capturing electromagnetic radiation.

10 Embodiment 103. The method for capturing images using an endoscopic probe of any of embodiments 101 to 102, wherein the mirror is a microelectromechanical systems mirror.

Embodiment 104. The method for capturing images using an endoscopic probe of any of embodiments 101 to 103, further comprising providing a lens between the means for
15 capturing electromagnetic radiation and the mirror.

Embodiment 105. The method for capturing images using an endoscopic probe of embodiment 104, wherein the lens is a gradient-index (GRIN) lens.

Embodiment 106. The method for capturing images using an endoscopic probe of any of embodiments 101 to 105, wherein the means for capturing electromagnetic radiation
20 is a fiber.

Embodiment 107. The method for capturing images using an endoscopic probe of any of embodiments 101 to 106, wherein the fiber is a single mode fiber (SMF).

Embodiment 108. The method for capturing images using an endoscopic probe of any of embodiments 101 to 107, wherein the endoscopic probe is configured to be side-viewing.

Embodiment 109. The method for capturing images using an endoscopic probe of any of embodiments 101 to 107, wherein the endoscopic probe is configured to be forward-viewing.

Embodiment 110. The method for capturing images using an endoscopic probe of any of embodiments 102 to 109, wherein the mirror is configured to tilt in one direction.

Embodiment 111. The method for capturing images using an endoscopic probe of any of embodiments 102 to 109, wherein the mirror is configured to tilt in two directions.

Embodiment 112. The method for capturing images using an endoscopic probe of any of embodiments 102 to 111, wherein the mirror can be raised in lowered.

Embodiment 113. The method for capturing images using an endoscopic probe of any of embodiments 102 to 111, wherein a means for tilting or raising the mirror is bimorph actuator(s).

Embodiment 114. The method for capturing images using an endoscopic probe of any of embodiments 102 to 112, wherein a means for tilting or raising the mirror is piezo electric crystal(s).

Embodiment 115. The method for capturing images using an endoscopic probe of any of embodiments 102 to 112, wherein a means for tilting or raising the mirror is inverted-series-connected (ISC) Al/SiO₂ bimorph actuator(s).

Embodiment 116. The method for capturing images using an endoscopic probe of any of embodiments 101 to 115, wherein the means for capturing electromagnetic radiation is a camera.

Embodiment 117. The method for capturing images using an endoscopic probe of any of embodiments 102 to 116, further comprising providing a second mirror positioned to reflect electromagnetic radiation coming from the first mirror and to the means for capturing electromagnetic radiation.

5 Embodiment 118. The method for capturing images using an endoscopic probe of any of embodiments 101 to 117, wherein the second mirror is configured to tilt using actuators or piezoelectric crystals.

Embodiment 119. The method for capturing images using an endoscopic probe of any of embodiments 101 to 118, wherein the electromagnetic radiation is visible light.

10 Embodiment 120. The method for capturing images using an endoscopic probe of any of embodiments 101 to 118, wherein the electromagnetic radiation is in the infrared range.

Embodiment 121. The method for capturing images using an endoscopic probe of any of embodiments 101 to 120, wherein both of the first and the second mirror are fixed.

15 Embodiment 122. The method for capturing images using an endoscopic probe of any of embodiments 101 to 121, wherein the endoscope shell is made of plastic, metal, or glass.

Embodiment 123. The method for capturing images using an endoscopic probe of any of embodiments 101 to 122, wherein a cross section of the endoscope shell is oval or
20 round.

Embodiment 124. The method for capturing images using an endoscopic probe of any of embodiments 101 to 123, wherein the endoscope shell has a flattened optical window.

Embodiment 125. The method for capturing images using an endoscopic probe of any of embodiments 101 to 124, wherein the first mirror is fixed.

Embodiment 126. The method for capturing images using an endoscopic probe of any of embodiments 101 to 125, wherein the second mirror is fixed.

5 Embodiment 127. The method for capturing images using an endoscopic probe of any of embodiments 101 to 125, wherein the electromagnetic radiation is in the UV range.

10 It should be understood that the examples and embodiments described herein are for illustrative purposes only and that various modifications or changes in light thereof will be suggested to persons skilled in the art and are to be included within the spirit and purview of this application.

15 All patents, patent applications, provisional applications, and publications referred to or cited herein (including those in the “References” section) are incorporated by reference in their entirety, including all figures and tables, to the extent they are not inconsistent with the explicit teachings of this specification.

REFERENCES

- [1] D. Huang, E. A. Swanson, C. P. Lin, J. S. Schuman, W. G. Stinson, W. Chang, M. R. Hee, T. Flotte, K. Gregory, and C. A. Puliafito, "Optical coherence tomography.," *Science*, vol. 254, no. 5035, pp. 1178–81, 1991.
- [2] J. Sun, S. Guang, L. Wu, L. Liu, S. W. Choe, B. S. Sorg, and H. Xie, "3D in vivo optical coherence tomography based on a low-voltage, large-scan-range 2D MEMS mirror", *Opt. Express*, vol. 18, no. 12, pp. 12065-12075, 2010.
- [3] X. Zhang, S. J. Koppal, R. Zhang, L. Zhou, E. Butler, and H. Xie, "Wide-angle structured light with a scanning MEMS mirror in liquid," *Opt. Express*, vol. 24, no. 4, p. 3479, 2016.
- [4] K. Jia, S. Pal, and H. Xie, "An electrothermal tip-tilt-piston micromirror based on folded dual s-shaped bimorphs," *J. Microelectromechanical Syst.*, vol. 18, no. 5, pp. 1004–1015, 2009.

CLAIMS

What is claimed is:

1. An endoscopic probe, comprising:
an endoscope shell;
a means for capturing electromagnetic radiation; and
an intermediate layer provided between the means for capturing electromagnetic radiation and the endoscope shell, wherein the intermediate layer comprises at least one of a liquid and a gel.
2. The endoscopic probe according to claim 1, further comprising a first mirror disposed such that electromagnetic radiation entering through the endoscope shell bounces off the first mirror and enters the means for capturing electromagnetic radiation.
3. The endoscopic probe according to claim 2, wherein the first mirror is a microelectromechanical systems (MEMS) mirror.
4. The endoscopic probe according to any of claims 2-3, wherein the first mirror is configured to tilt in at least one direction,
wherein the first mirror is configured to be raised and lowered, and
wherein the first mirror comprises at least one of the following: a first bimorph actuator for tilting the first mirror, raising the first mirror, or both; a piezo electric crystal for tilting the first mirror, raising the first mirror, or both; and second bimorph actuator that is an inverted-series-connected (ISC) Al/SiO₂ bimorph actuator for tilting the first mirror, raising the first mirror, or both.
5. The endoscopic probe according to any of claims 1-4, wherein the means for capturing electromagnetic radiation is a fiber or a camera.

6. The endoscopic probe according to any of claims 1-4, wherein the means for capturing electromagnetic radiation is a single mode fiber (SMF).

7. The endoscopic probe according to any of claims 2-6, further comprising a lens between the means for capturing electromagnetic radiation and the first mirror.

8. The endoscopic probe according to claim 7, wherein the lens is a gradient-index (GRIN) lens.

9. The endoscopic probe according to any of claims 2-8, further comprising a second mirror positioned to reflect electromagnetic radiation coming from the first mirror and to the means for capturing electromagnetic radiation.

10. The endoscopic probe according to any of claims 1-9, wherein the electromagnetic radiation comprises visible light.

11. The endoscopic probe according to any of claims 1-10, wherein the electromagnetic radiation comprises infrared light.

12. The endoscopic probe according to any of claims 1-11, wherein the electromagnetic radiation comprises ultraviolet (UV) light.

13. The endoscopic probe according to any of claims 1-12, wherein a cross section of the endoscope shell is oval or circular.

14. The endoscopic probe according to any of claims 1-13, wherein the endoscope shell comprises a flattened optical window.

15. The endoscopic probe according to any of claims 1-14, further comprising a seal ring.

16. The endoscopic probe according to any of claims 1-15, further comprising a means for delivering electromagnetic radiation to the endoscopic probe,

wherein means for delivering electromagnetic radiation comprises at least one of the following: an optical fiber; a light-emitting diode (LED); and an electromagnetic radiation transmitting fiber.

17. A method for capturing images using an endoscopic probe comprising an endoscope shell, the method comprising:

providing a means for capturing electromagnetic radiation within the endoscope shell; and

using Snell's window effect to expand a field of view captured by the means for capturing electromagnetic radiation.

18. The method according to claim 17, further comprising providing a mirror placed such that electromagnetic radiation entering through the endoscope shell can bounce off the mirror and enter the means for capturing electromagnetic radiation.

19. The method for capturing images using an endoscopic probe according to claim 18, wherein the mirror is a MEMS mirror.

20. The method according to any of claims 18-19, wherein the first mirror is configured to tilt in at least one direction,

wherein the first mirror is configured to be raised and lowered, and

wherein the first mirror comprises at least one of the following: a first bimorph actuator for tilting the first mirror, raising the first mirror, or both; a piezo electric crystal for tilting the first mirror, raising the first mirror, or both; and second bimorph actuator that is an inverted-

series-connected (ISC) Al/SiO₂ bimorph actuator for tilting the first mirror, raising the first mirror, or both.

21. The method according to any of claims 17-20, wherein the means for capturing electromagnetic radiation is a fiber or a camera.

22. The method according to any of claims 17-20, wherein the means for capturing electromagnetic radiation is a single mode fiber (SMF).

23. The method according to any of claims 18-22, further comprising providing a lens between the means for capturing electromagnetic radiation and the mirror.

24. The method according to claim 23, wherein the lens is a GRIN lens.

25. The method according to any of claims 18-24, further comprising providing a second mirror positioned to reflect electromagnetic radiation coming from the first mirror and to the means for capturing electromagnetic radiation.



26. The method according to any of claims 17-25, wherein the electromagnetic radiation comprises visible light.



27. The method according to any of claims 17-26, wherein the electromagnetic radiation comprises infrared light.



28. The method according to any of claims 17-27, wherein the electromagnetic radiation comprises ultraviolet (UV) light.

29. The method according to any of claims 17-28, wherein a cross section of the endoscope shell is oval or circular.

30. The method according to any of claims 17-29, wherein the endoscope shell has a flattened optical window.

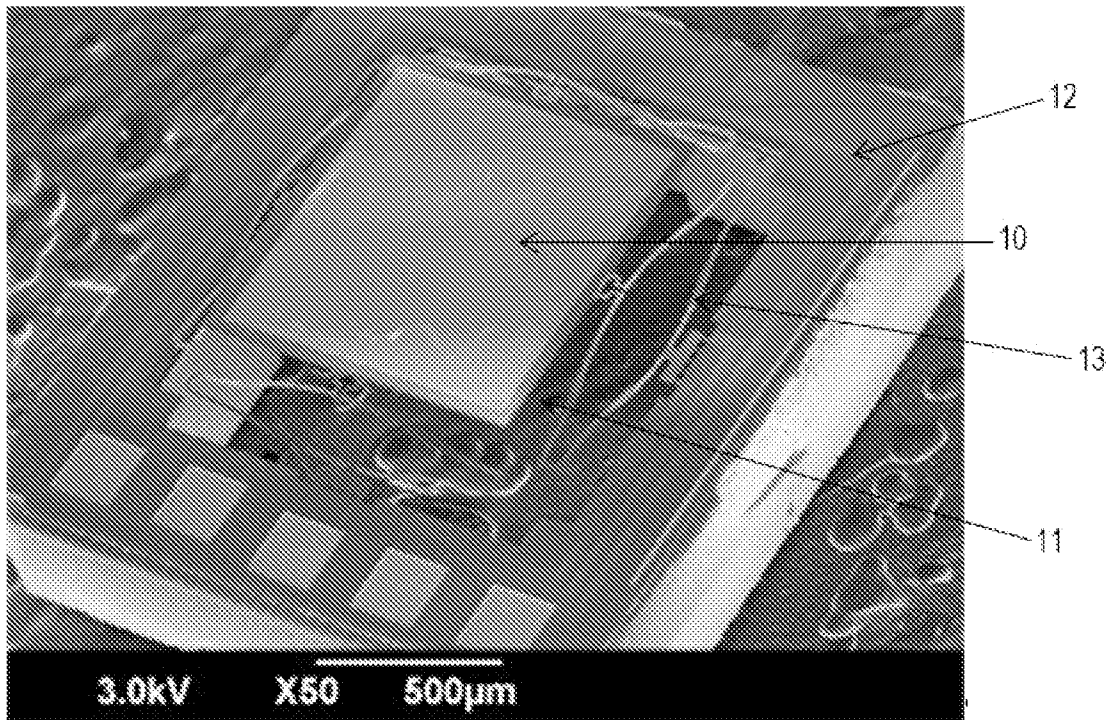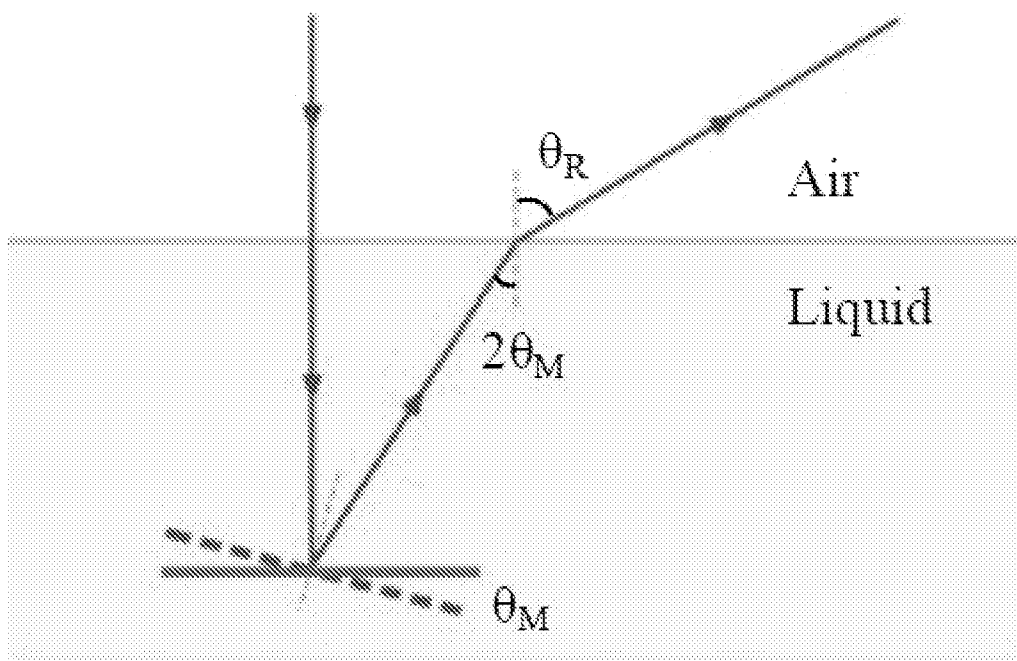**Figure 1****Figure 2a**

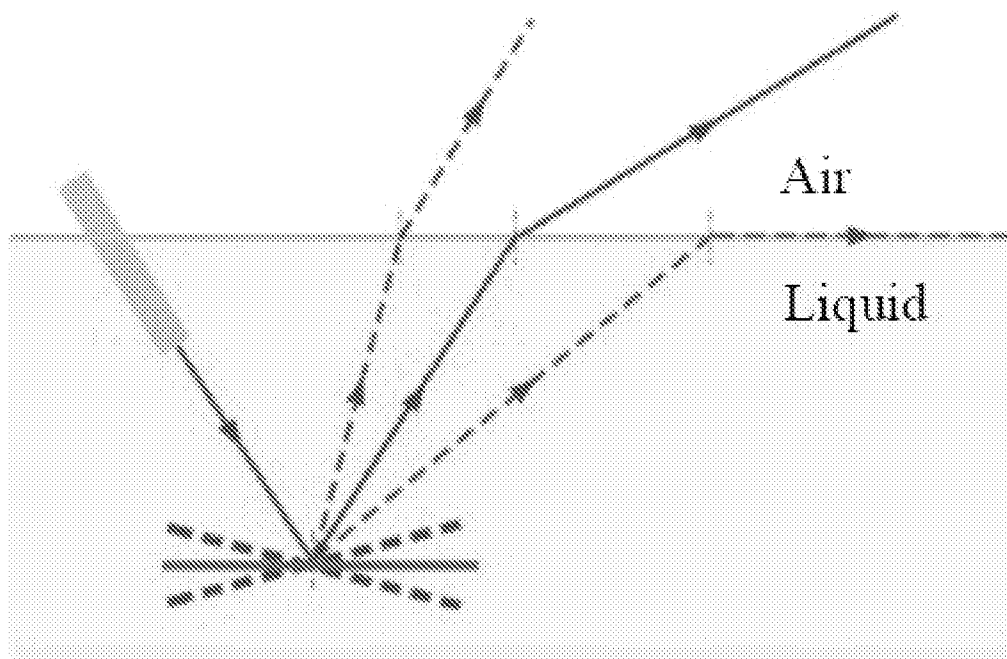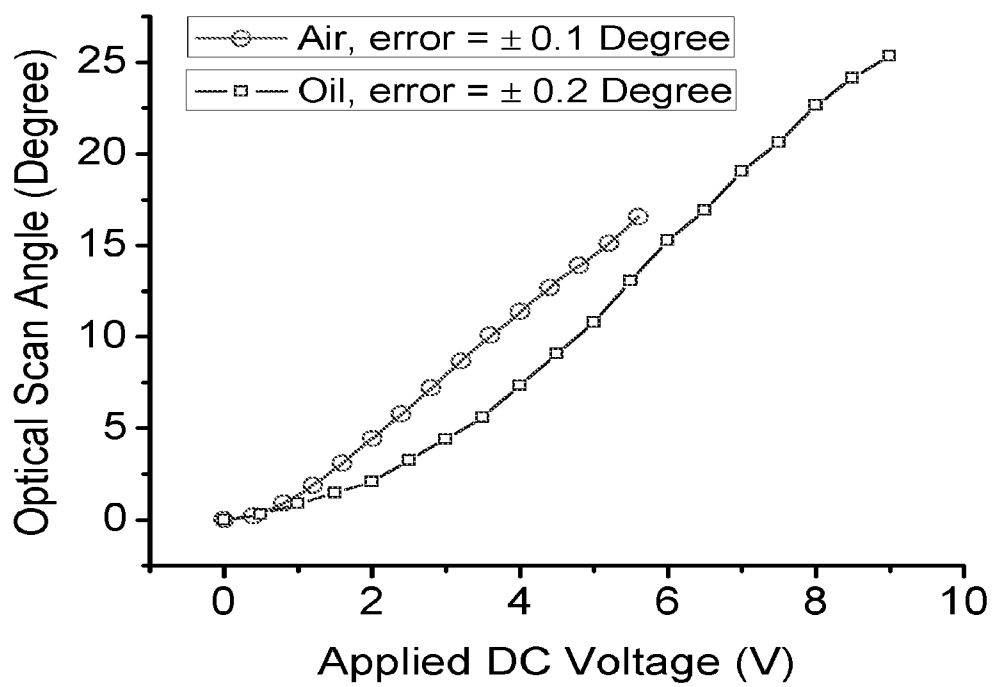**Figure 2b****Figure 3**

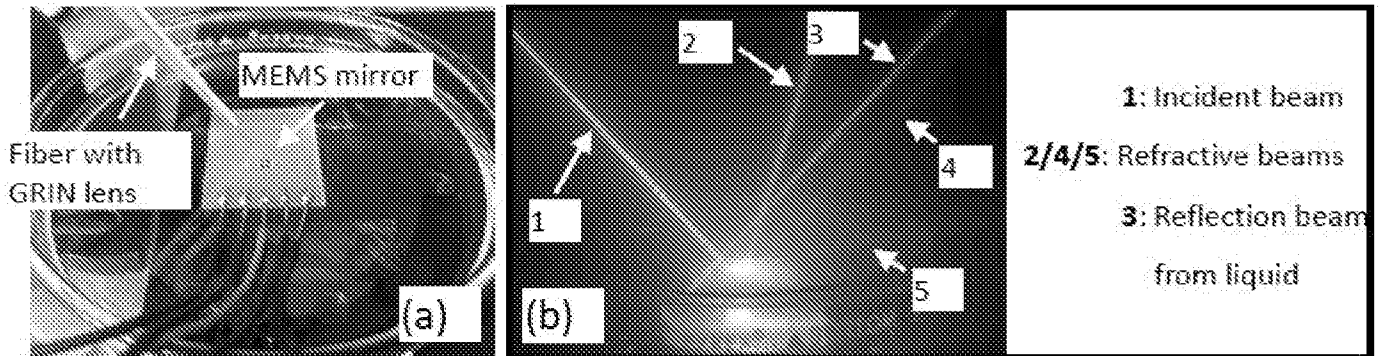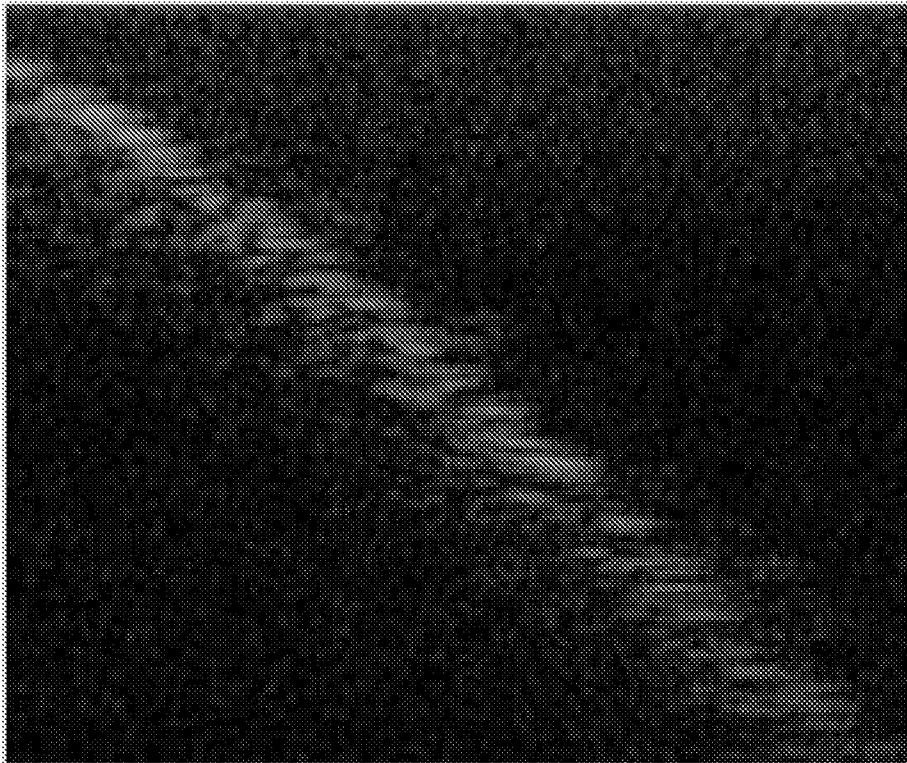**Figure 4****Figure 5a**

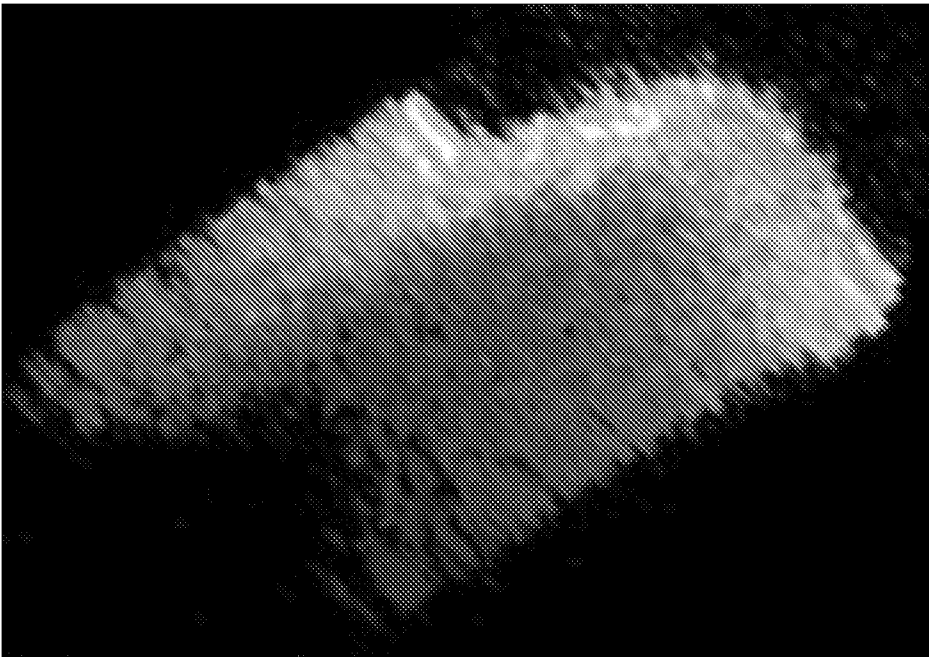


Figure 5b

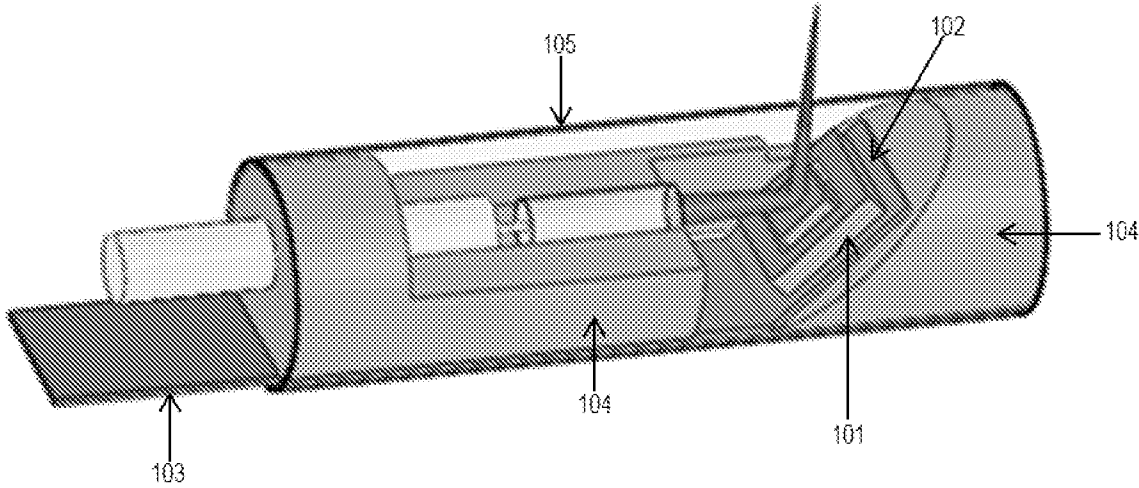


Figure 6a

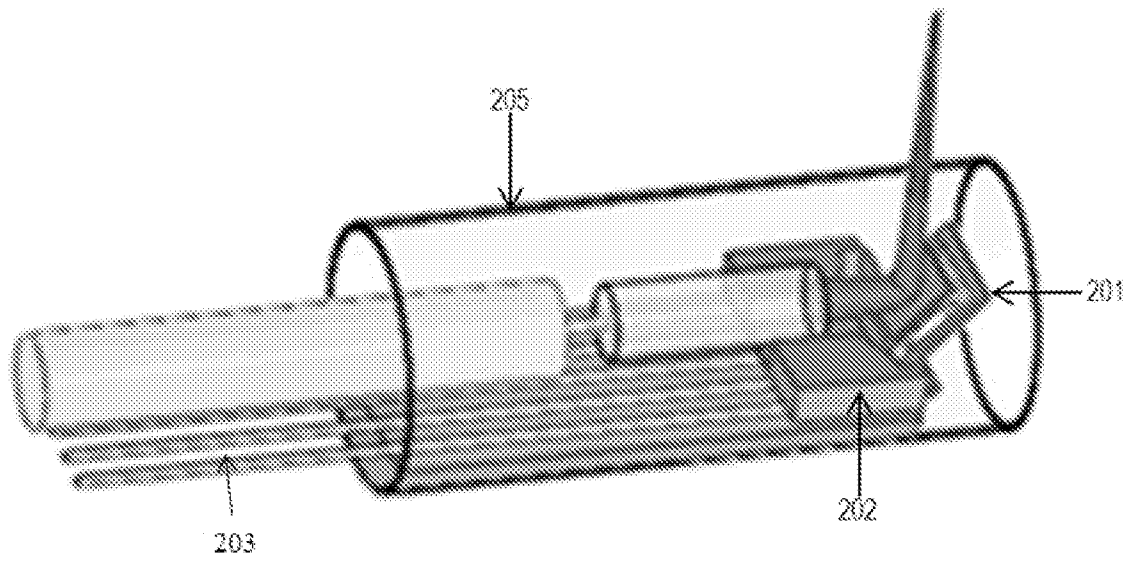


Figure 6b

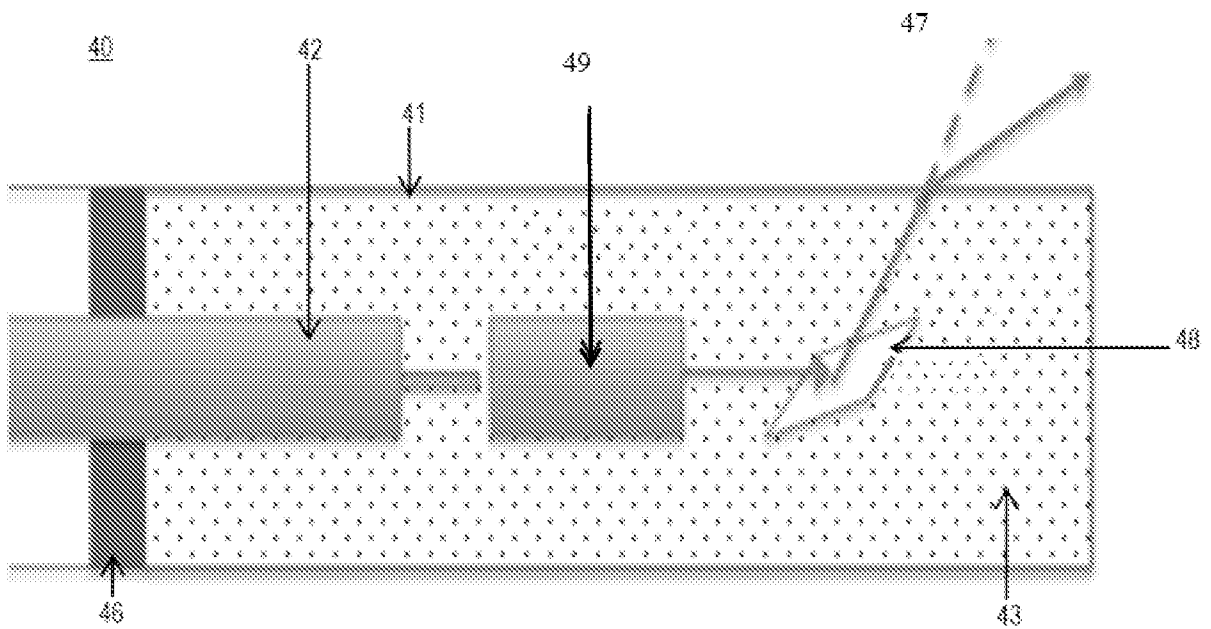


Figure 7

6/7

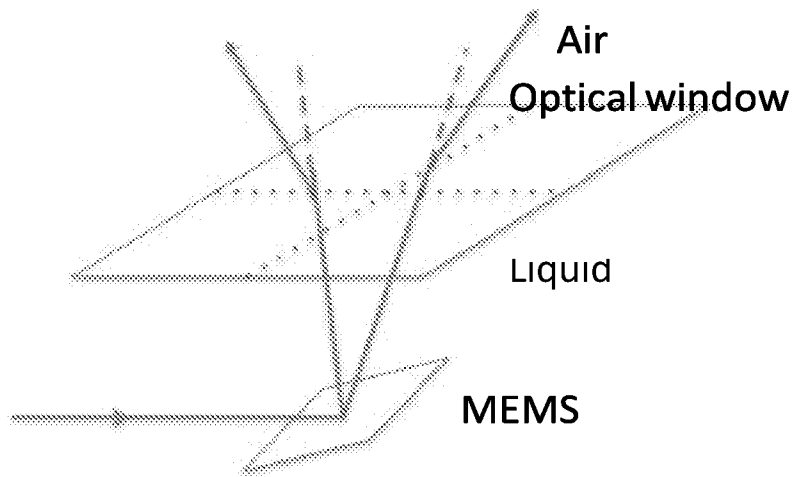


Figure 8

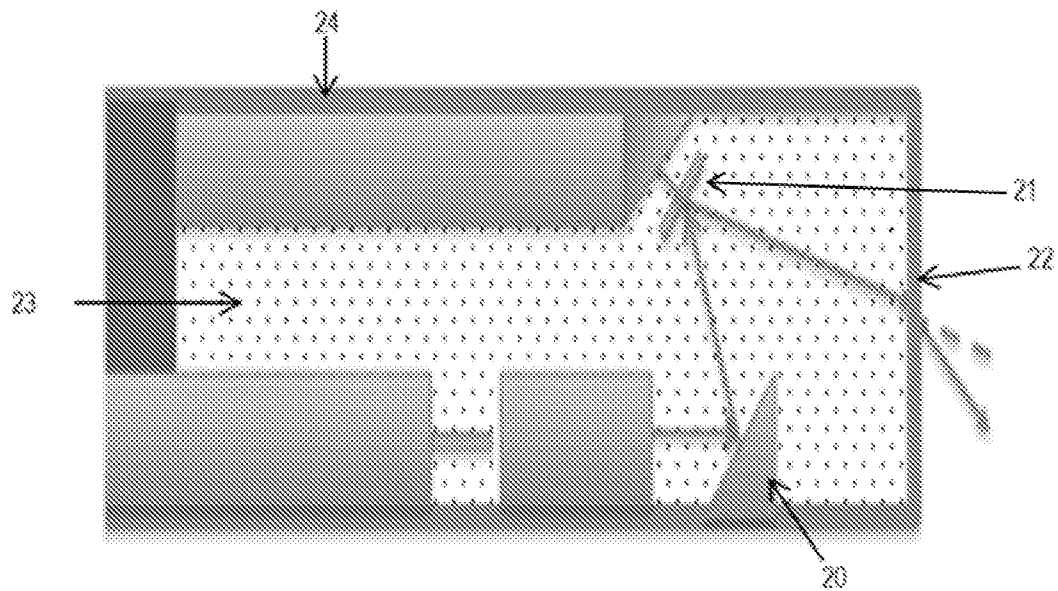


Figure 9

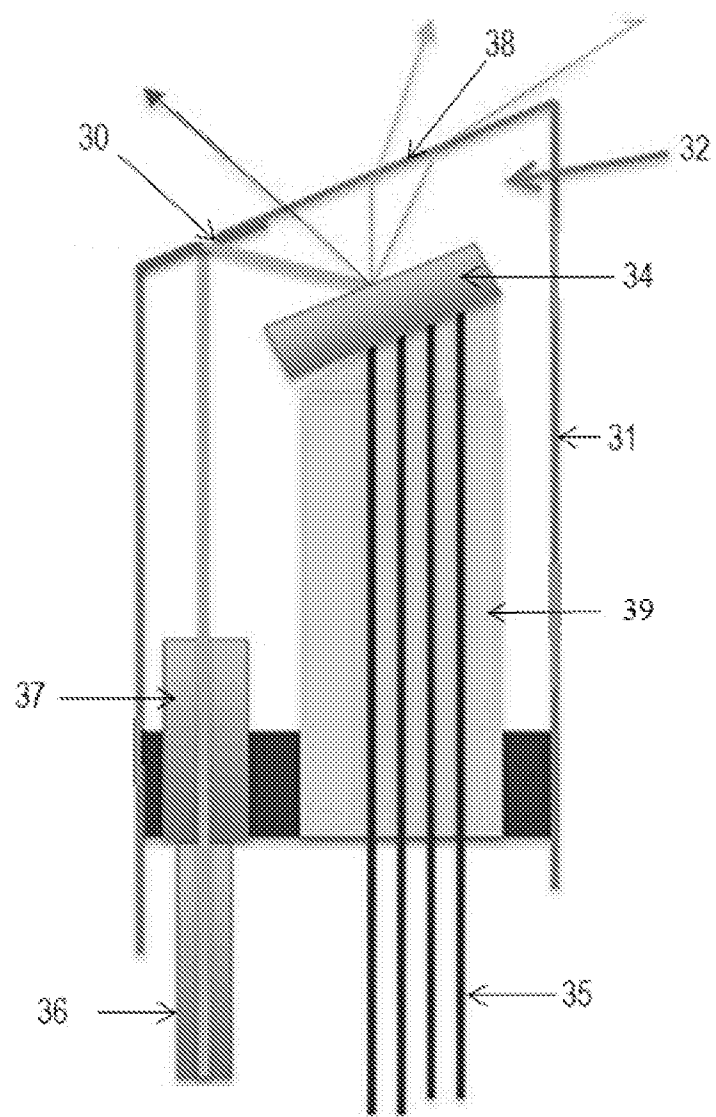


Figure 10

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2017/044401**A. CLASSIFICATION OF SUBJECT MATTER****A61B 1/00(2006.01)i, A61B 1/04(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 1/00; A61B 5/027; A61B 6/00; G01N 21/17; A61B 1/06; G01B 9/02; A61B 1/04

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: endoscopic, probe, capture, MEMS mirror, liquid

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 2014-157645 A1 (SONY CORPORATION) 02 October 2014	1-3, 17-19
Y	See paragraphs [66]-[68], [87], [89], [152], claim 19 and figures 2, 3, 7A, 7B.	4, 20
Y	US 2010-0157308 A1 (XIE) 24 June 2010	4, 20
	See claims 3, 4 and figure 3.	
A	US 8060187 B2 (MARSHIK-GEURTS et al.) 15 November 2011	1-4, 17-20
	See claim 1 and figure 1.	
A	JP 2013-507189 A (THE GENERAL HOSPITAL CORPORATION) 04 March 2013	1-4, 17-20
	See paragraph [61] and figure 17.	
A	WO 2009-137704 A1 (VOLCANO CORPORATION et al.) 12 November 2009	1-4, 17-20
	See claims 1-9 and figure 1A.	



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

22 September 2017 (22.09.2017)

Date of mailing of the international search report

22 September 2017 (22.09.2017)

Name and mailing address of the ISA/KR

International Application Division

Korean Intellectual Property Office

189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea



Facsimile No. +82-42-481-8578

Authorized officer

KIM, Yeon Kyung

Telephone No. +82-42-481-3325



INTERNATIONAL SEARCH REPORTInternational application No.
PCT/US2017/044401**Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☒ Claims Nos.: 8,24
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
Claims 8,24 are unclear, because these claims refer to multiple dependent claims which do not comply with PCT Rule 6.4(a).
3. ☒ Claims Nos.: 5-7,9-16,21-23,25-30
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2017/044401

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2014-157645 A1	02/10/2014	CN 105050475 A US 2016-0299170 A1	11/11/2015 13/10/2016
US 2010-0157308 A1	24/06/2010	US 7944566 B2 WO 2006-084279 A2 WO 2006-084279 A3	17/05/2011 10/08/2006 12/10/2006
US 8060187 B2	15/11/2011	AU 2003-256954 A1 AU 2003-258062 A1 EP 1538968 A1 EP 1538968 B1 EP 1551299 A2 JP 2005-534415 A JP 2005-534428 A JP 4602765 B2 US 2004-0024298 A1 US 2004-0024321 A1 US 2004-0077950 A1 US 2008-0221455 A1 US 7376456 B2 US 7486985 B2 US 7689268 B2 WO 2004-012586 A2 WO 2004-012586 A3 WO 2004-012594 A1	23/02/2004 23/02/2004 15/06/2005 04/06/2008 13/07/2005 17/11/2005 17/11/2005 22/12/2010 05/02/2004 05/02/2004 22/04/2004 11/09/2008 20/05/2008 03/02/2009 30/03/2010 12/02/2004 29/04/2004 12/02/2004
JP 2013-507189 A	04/03/2013	EP 2485641 A2 EP 2485641 A4 JP 2016-027903 A JP 5856061 B2 US 2011-0137178 A1 WO 2011-044301 A2 WO 2011-044301 A3	15/08/2012 14/10/2015 25/02/2016 09/02/2016 09/06/2011 14/04/2011 30/06/2011
WO 2009-137704 A1	12/11/2009	EP 2178442 A1 EP 2278915 A1 EP 2278915 A4 JP 2010-533049 A JP 2011-519692 A JP 5524835 B2 US 2009-0018393 A1 US 2011-0137124 A1 US 9622706 B2 WO 2009-009799 A1	28/04/2010 02/02/2011 14/11/2012 21/10/2010 14/07/2011 18/06/2014 15/01/2009 09/06/2011 18/04/2017 15/01/2009