



- (51) **International Patent Classification:**
A61B 5/107 (2006.01) *A61B 5/00* (2006.01)
- (21) **International Application Number:**
PCT/US2016/017902
- (22) **International Filing Date:**
12 February 2016 (12.02.2016)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
62/115,435 12 February 2015 (12.02.2015) US
62/157,331 5 May 2015 (05.05.2015) US
62/172,516 8 June 2015 (08.06.2015) US
- (71) **Applicant: FOUNDRY INNOVATION & RESEARCH 1, LTD.** [IE/IE]; Arthur Cox Building, Earlsfort Centre, Earlsfort Terrace, Dublin 2 (IE).
- (72) **Inventors: GIFFORD, Hanson, S., III;** 199 Jefferson Drive, Menlo Park, CA 94025 (US). **DEEM, Mark, E.;** 199 Jefferson Drive, Menlo Park, CA 94025 (US). **MORRISS, John;** 199 Jefferson Drive, Menlo Park, CA 94025 (US). **SUTTON, Douglas, S.;** 199 Jefferson Drive, Menlo Park, CA 94025 (US). **GRAINGER, Jeffrey, J.;** 199 Jefferson Drive, Menlo Park, CA 94025 (US). **RAJASEKHAR, Vijaykumar;** 199 Jefferson Drive, Menlo Park, CA 94025 (US).
- (74) **Agent: KOHLER, Thomas, D.;** Downs Rachlin Martin PLLC, 199 Main Street, P.O. Box 190, Burlington, VT 05402-0190 (US).

(81) **Designated States** (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) **Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) **Title:** IMPLANTABLE DEVICES AND RELATED METHODS FOR HEART FAILURE MONITORING

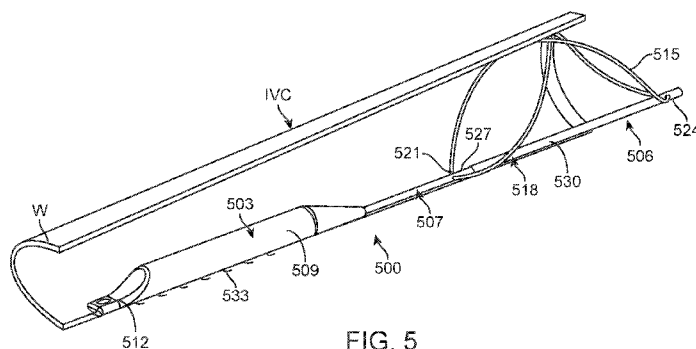


FIG. 5

(57) **Abstract:** Implantable devices for continuously monitoring vascular lumen dimensions, in particular in the inferior vena cava (IVC) for determining heart failure status of a patient. Related therapy systems as well as monitoring and therapy methods are also disclosed. Devices include active or passive marker elements placed in contact with, adhered to or injected into the vessel wall to generate or reflect signals from which lumen diameter may be determined. Disclosed devices may be fully implantable and self-contained including capabilities for wirelessly communication monitored parameters.

IMPLANTABLE DEVICES AND RELATED METHODS FOR HEART FAILURE MONITORING

RELATED APPLICATION DATA

[0001] This application claims the benefit of priority of U.S. Provisional Patent Application Serial No. 62/115,435, filed February 12, 2015, and titled “Implantable Device and Related Methods for Heart Failure Monitoring”, this application also claims the benefit of priority of U.S. Provisional Patent Application Serial No. 62/157,331, filed May 5, 2015, and titled “Heart Failure Monitoring System and Method”, and also claims the benefit of priority of U.S. Provisional Patent Application No. 62/172,516, filed June 8, 2015, and titled “Methods and Apparatus for Monitoring Patient Physiological Status Based On Inferior Vena Cava Volume”. Each of these applications is incorporated by reference herein in their entirety.

FIELD OF THE INVENTION

[0002] The present invention generally relates to the field of medical devices and methods for monitoring heart health. In particular, the present invention is directed to an implantable device for heart failure monitoring, and more particularly for detecting early warning signs of acutely decompensated heart failure.

BACKGROUND

[0003] Heart failure is one of the most significant chronic conditions afflicting adult populations. In the United States, 5.7 million Americans have heart failure, with 870,000 new cases annually. As the population ages, this population is growing, as approximately 10% of the population over 80 suffers from heart failure. It is estimated that by 2030 8 million Americans will have heart failure. The costs of caring for heart failure are over thirty billion dollars per year. Twenty billion of this cost is direct medical costs. This expense is expected to more than double over the next fifteen years.

[0004] In patients with chronic heart failure, a significant portion of these costs is due to hospitalization to manage acutely decompensated heart failure (ADHF). Each re-hospitalization can last up to a week, and costs approximately \$10,000. ADHF is very often a result of some combination of a downturn in the heart’s performance and excessive intake of fluids and/or salt. This leads to a buildup of fluid in the vascular system. Increased blood volume in the left atrium

at higher pressure means higher blood pressure in the lungs, which eventually leads to fluid filling the lungs and an inability to breathe. At this stage it is imperative to hospitalize the patient to carefully manage them while drugs are delivered to remove the excess fluids.

[0005] Managing these patients to prevent the need for re-hospitalization is extremely challenging. Many non-invasive approaches to monitoring patients have been tried, such as weighing patients daily to detect fluid weight gain, having a nurse call them daily to assess their health status, and so on. More recently, various implantable monitoring devices have been tested. One example is the “CardioMEMS” device of St. Jude Medical, Inc., which is a wireless pressure monitor implanted in the pulmonary artery (PA). An external power supply and receiver is placed on the patient’s chest to charge the implanted sensor and receive pressure data measured by it. Other companies are developing their own versions of such PA pressure monitors. The money saved by avoiding re-hospitalization can more than pay for the cost of such devices.

[0006] It is important to measure the onset of ADHF early enough to give the patient and/or caregiver enough time to adjust their behavior, medication, or other factors to prevent the patient from ending up with frank congestion and the need for hospitalization. FIG. 47, adapted from the CardioMEMS website, shows the timeline of physiologic changes leading up to ADHF requiring hospitalization. There is clinical evidence that IVC volume variation changes occur up to several weeks prior to decompensation.

[0007] In addition to heart failure patients, hemodialysis patients have a chronic need for careful volume management. Large volumes of fluid are involved in the hemodialysis process, and managing patients so that they don’t end up hypovolemic or overloaded with fluid requires careful management. A monitor which provided immediate feedback on these patient’s volume status before, during and after hemodialysis would be very helpful.

[0008] There are other groups of patients who might benefit from such a monitor. For example, patients in septic shock or occult shock due to trauma are subject to hypoperfusion which can be identified by measuring the degree of collapse of the IVC. While it may or may not make sense to implant a device permanently to manage these acute events, if the patient has

recurrent episodes of these events or already has such a monitor implanted for other reasons, the IVC monitor may be helpful in managing these patients.

[0009] Congestive heart failure is so-named because additional blood volume backing up into the lungs causes fluid to seep out of the pulmonary circulation into the airway passages of the lungs, causing congestion of the lungs. The patients become short of breath, and typically need to be hospitalized and carefully managed while the excess fluid is removed by a combination of fluid management and aggressive use of diuretic medications.

[0010] This happens because the left ventricle is not able to pump all of the volume of blood returning to the heart from the lungs. Although measurement of left atrial pressure, typically by measuring pulmonary artery wedge pressure, is commonly considered the most direct way to measure congestion in heart failure, there are other areas where congestion can be detected. When additional blood volume is added to the circulatory system, the IVC is one of the first places for that added volume to collect. To quote a paper, “In patients with advanced heart failure, left ventricular systolic dysfunction causes increased left atrial pressure. The pressure is transmitted back through the pulmonary circulation to cause pulmonary artery hypertension. The pulmonary artery hypertension can worsen pre-existing right ventricular dysfunction and exacerbate tricuspid valve regurgitation, leading to systemic venous congestion. If venous congestion and elevated central venous pressure are the hallmarks of heart failure, then distention of the inferior vena cava [measured by echocardiography] may be a good prognostic marker in patients with decompensated heart failure.” (Lee et al, “Prognostic significance of dilated inferior vena cava in advanced decompensated heart failure,” *International Journal of Cardiovascular Imaging* (2014) 30:1289-1295).

[0011] The diameter of the IVC has also demonstrated correlation with right atrial pressure, and it may correlate with renal function and renal sodium retention, which are also very important prognostic factors of heart failure. Therefore, increasing IVC volume and/or pressure may be a very effective early indicator of worsening heart failure condition.

[0012] However, recent studies have indicated that the variation in IVC volume over the respiratory cycle is a more sensitive measurement of fluid overload and/or heart failure than simple measurement of average IVC volume, diameter, or pressure. During inspiration,

intrathoracic pressure decreases, thereby increasing venous return and causing collapse of the IVC. During expiration, intrathoracic pressure increases, decreasing venous return and causing an increase in the volume of the IVC.

[0013] Since the IVC typically collapses in the anterior-posterior direction, some studies have suggested that the most accurate technique for measuring IVC volume changes with ultrasound is to measure the distance from the anterior wall of the IVC to the posterior wall.

[0014] In applying this measurement to heart failure, at least one study has suggested that a variation of less than 15% (measured as maximum anterior-posterior dimension minus minimum A-P dimension, divided by the maximum A-P dimension) is indicative of impending or present ADHF.

[0015] While vessel dimensions may be measurable using external ultrasound, magnetic resonance imaging, computerized axial tomography, or other technologies, these imaging procedures must be administered in a hospital or other specialized facility, do not permit continuous monitoring, and do not allow for monitoring of the patient at their home or other remote location. As a result, the condition of a heart failure patient can worsen into a critical state before care providers become aware of it, dramatically increasing the mortality risk and cost of treatment for the patient.

[0016] Prior studies of IVC dimensions without implantable devices have been conducted using ultrasound imaging. This typically requires a highly trained physician or ultrasound technician to manage the ultrasound machine, ensure an appropriate connection of the transducer to the skin, position the ultrasound transducer in the appropriate location, identify the IVC, and take accurate measurements. This is not something that heart failure patients or their caregivers could typically be trained to do predictably and accurately with existing equipment. Moreover, these systems typically include large, complex, and expensive pieces of equipment which are not suitable for use outside of a specialized medical facility.

[0017] As is understood in the art, there is a long history of implantable vena cava filters to catch clots which embolize from the leg veins, catching them and holding them in the vena cava until they dissolve in the blood flowing past. The widespread clinical use of such IVC filters

demonstrates the safety and feasibility of anchoring an implant in the IVC and provides useful teachings as to how aggressively IVC anchors may be shaped, how much radial force a device should exert, how strong the elements should be, etc. However, in spite of the widespread use of IVC filters over many years, heretofore it has not been suggested that an implant in the IVC could be utilized for purposes of monitoring fluid volume or IVC dimensions. Moreover, even if a suggestion were made to equip an IVC filter with a sensor for monitoring vascular dimensions, such filters would be unsuited to the purpose. The anchoring structures used to secure IVC filters constrain the vessel from natural size and shape changes in response to changes in fluid volume and would thus limit the usefulness or accuracy of such a device.

SUMMARY OF DISCLOSURE

[0018] Embodiments disclosed herein include an implantable device for monitoring vascular lumen diameter, comprising means for detecting lumen diameter at a monitoring location; an anchor element configured to securely anchor the device to the vascular lumen at an anchoring location with the detecting means positioned at the monitoring location; and an anchor isolation structure extending between the detecting means and anchor element, the anchor isolation structure having a shape and length specifically configured to substantially isolate the detecting means at the sensing location from distortions of the vessel caused by the anchoring element at the anchoring location.

[0019] In one alternative embodiment, the detecting means comprises an active marker element coupled to an end of the anchor isolation structure opposite the anchor element; the anchor element comprises a resilient member moveable between a first, collapsed configuration and a second, deployed configuration, wherein the first collapsed configuration has an overall diameter sufficiently less than the vascular lumen diameter to permit deployment of the device through the vasculature, and the second expanded deployed condition has an overall diameter sufficient to securely engage the vessel lumen at the anchoring location; and the anchor isolation structure comprises a member having sufficient stiffness to maintain the active marker element substantially in contact with the lumen wall without eroding the lumen wall and with the active marker element oriented substantially in the direction of the lumen wall opposite the transducer.

[0020] In another alternative embodiment of claim 1, wherein: the detecting means comprises an electronics capsule having an ultrasound transducer disposed at an end opposite the anchor element, the electronics capsule containing at least power and communications modules controlled by a control modules to receive and wirelessly transmit signals based on inputs from the ultrasound transducer; the anchor element comprises a looped anchor wire secured to a telescoping deployment member moveable between a first collapsed configuration and a second deployed configuration, wherein the looped wire in the second deployed configuration expands sufficiently to place the electronics capsule against one wall of the lumen while in contact with a substantial portion of an internal diameter of the lumen at the anchoring location; and the anchor isolation structure comprise a flexible member disposed between the anchor element deployment member and the electronics capsule, wherein the anchor isolation structure has sufficient stiffness to maintain the electronics capsule against the one wall of the lumen and a length equal to approximately 1 to 4 times the undistorted diameter of the lumen at the anchor location.

[0021] A further alternative embodiment disclosed is a cardiac therapy system comprising the implantable monitoring device described above in combination with an implantable cardiac therapy device including an implantable housing containing at least power and control modules; at least one lead connecting the detecting means with the implantable housing and modules contained therein; at least one cardiac therapy delivery element; and at least one lead connecting the at least one therapy delivery element to the implantable housing and modules contained therein. The control module is configured to execute instructions for generating a signal with the detecting means, receiving a signal responsive to the generated signal with the detecting means, the received signal being indicative of vessel diameter at the monitoring location; determining vena cava diameter at the monitoring location based on the signal; comparing the determined diameter to a reference diameter to determine a change in vena cava diameter, evaluating heart condition based on the determined change in vena cava diameter; and modulating cardiac therapy delivered by the at least one therapeutic device passed on the evaluated heart condition

[0022] In another disclosed embodiment an implantable device for monitoring vascular lumen diameter comprises an electronics capsule having an ultrasound transducer disposed at one end, the electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from

the ultrasound transducer, the ultrasound transducer configured substantially in contact with a lumen wall and to detect lumen diameter at a monitoring location by echo reflection off an opposite lumen wall; a looped anchor wire secured to a telescoping deployment member moveable between a first collapsed configuration and a second deployed configuration, wherein the looped anchor wire in the second deployed configuration expands sufficiently to place the electronics capsule against one wall of the lumen while in contact with a substantial portion of an internal diameter of the lumen at an anchoring location; and a flexible anchor isolation member disposed between the tubular deployment member and the electronics capsule, wherein the anchor isolation structure has sufficient stiffness to maintain the electronics capsule against the one wall of the lumen, the anchor isolation member having a shape and length specifically configured to at least substantially isolate the electronics capsule from distortions of the vessel lumen caused by the anchoring looped anchor wire at the anchoring location.

[0023] In a further disclosed embodiment a system for monitoring vascular lumen diameter comprises at least two implantable passive marker elements configured to be implanted in or through a vascular lumen wall at a monitoring location; an intravascular delivery device for delivering and implanting the passive marker elements at the monitoring location; and detecting means configured to be positioned outside a patient's body for sensing position and movement of the implanted passive marker elements relative to each other.

[0024] Another disclosed embodiment is An implantable device for monitoring vascular lumen diameter, comprising an ultrasound transducer configured to be positioned substantially in contact with a lumen wall and to detect lumen diameter at a monitoring location by echo reflection off an opposite lumen wall; an, electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from the ultrasound transducer; an anchoring member configured to rotationally and longitudinally immobilize the implantable device at an anchoring location in the vascular lumen ; and a flexible anchor isolation member disposed between the anchoring member and the ultrasound transducer, wherein the anchor isolation structure has a shape and stiffness selected to maintain the ultrasound transducer against the one wall of the lumen, the anchor isolation member having a shape and length specifically configured to at least

substantially isolate the ultrasound transducer from distortions of the vessel lumen caused by the anchoring member at the anchoring location.

[0025] An implantable device for monitoring vascular lumen diameter according to another disclosure comprises an ultrasound transducer configured to be positioned substantially in contact with a lumen wall and to detect lumen diameter at a monitoring location by echo reflection off an opposite lumen wall; an electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from the ultrasound transducer; and an anchoring member configured to rotationally and longitudinally immobilize the implantable device at an anchoring location in the vascular lumen and having a shape and stiffness selected to maintain the ultrasound transducer against the one wall of the lumen. The electronics capsule may be mounted directly to the anchor element.

[0026] In another aspect of the present disclosure, a method of continuously monitoring a diameter of a vascular lumen with an implanted device, comprises implanting at least one marker element on a wall of the lumen at a monitoring location; anchoring the marker element to the lumen wall at an anchoring location, wherein the anchoring location is spaced from the monitoring location by a distance sufficient to isolate the marker element from distortions of the lumen wall due to the anchoring; generating a signal in cooperation with the at least one marker element indicative of vessel diameter at the monitoring location; receiving the signal; and determining vessel diameter based on the signal.

[0027] In a further embodiment of the method aspects of the present disclosure, a method of treating a cardiac condition in a patient comprises implanting a monitoring device in a vena cava wall such that at least one active marker element of the monitoring device is positioned against the wall at a monitoring location; anchoring the monitoring device to the vena cava wall at an anchoring location, wherein the anchoring location is spaced from the monitoring location by a distance sufficient to isolate the at least one active marker element from distortions of the lumen wall due to the anchoring; implanting at least one therapeutic device configured to deliver a cardiac therapy; generating a signal with the at least one active marker element indicative of vessel diameter at the monitoring location; receiving the signal; determining vena cava diameter

at the monitoring location based on the signal; comparing the determined diameter to a reference diameter to determine a change in vena cava diameter, evaluating heart condition based on the determined change in vena cava diameter; and modulating cardiac therapy delivered by the at least one therapeutic device passed on the evaluated heart condition.

[0028] Another method disclosed herein is a method of monitoring a cardiac condition of a patient, comprising implanting an intravascular device in a vena cava with an anchor element at an anchoring location, the intravascular device further having a pair of markers or sensors, the pair of markers or sensors being positioned in engagement with opposing walls of the vena cava at a monitoring location; receiving a signal from the pair of markers or sensors; and determining a diameter of the vena cava based on the signal; wherein the implanting comprises positioning the anchor element at the anchoring location sufficiently distant from the monitoring location such that diameter determinations based on the signal are not substantially affected by distortion of the vena cava wall by the anchor element at the anchor location.

[0029] In another disclosed embodiment, a monitoring system comprises an intravascular device configured for implantation in a vessel in a body cavity and having first and second markers biased or secured against opposing interior walls of the vessel; at least one anchor element configured to secure and position the intravascular device on the body cavity wall; an anchor isolation structure disposed between the at least one anchor element and the first and second markers, the anchor isolation structure having a length specifically configured to position the first and second markers sufficiently distant from the monitoring location such that diameter calculations derived from the markers are not substantially affected by distortion of the vena cava wall by the anchor element at; and an external device adapted to receive a first signal from the intravascular device and to calculate a distance between the first and second markers based on the signal.

[0030] In a further embodiment an intravascular device comprises an anchoring structure for anchoring within the vessel; and first and second arms extending longitudinally from the anchoring structure, wherein the first and second markers are coupled to the first and second arms, respectively. The first and second arms are configured to bias the first and second markers

against the vessel wall and to allow the first and second markers to move inwardly and outwardly with physiologic movement of the vessel wall.

[0031] Yet another embodiment is a therapeutic system for treating a patient comprising a monitoring system including an intravascular implant for implantation in a vena cava configured to monitor a dimension of the vena cava; a transmission device to transmit data based on the dimension; and a therapeutic device implanted in the patient and configured to receive the data transmitted from the monitoring system, the therapeutic device adapted to deliver therapy to the patient based upon the data received.

BRIEF DESCRIPTION OF THE DRAWINGS

[0032] For the purpose of illustrating and exemplifying the claimed invention, the drawings show aspects of embodiments of the present disclosure. However, it should be understood that the claimed invention is not limited to the precise arrangements and instrumentalities of the exemplifying embodiments shown in the drawings, wherein:

FIG. 1 is a schematic illustration of one embodiment of an implantable device deployed in the inferior vena cava (IVC) in accordance with the present disclosure.

FIGS. 2A, 2B, 2C and 2D show schematic cross-sections of the IVC and relative electrode positioning in embodiments described in the present disclosure.

FIG. 3 is a schematic illustration of one disclosed embodiment of an implantable device, showing its placement in the vasculature.

FIG. 4 is a schematic illustration of another disclosed embodiment of an implantable device, showing its placement in the vasculature.

FIG. 5 is a perspective view of a further alternative embodiment positioned in a partially cross-sectioned portion of the IVC.

FIG. 6 is side view of the embodiment shown in FIG. 5 and the partially cross-sectioned IVC.

FIG. 7 is an end view of the embodiment of FIG. 5 as viewed in the IVC from the superior aspect.

FIG. 8 is an end view of the embodiment of FIG. 5 as viewed in the IVC from the inferior aspect.

FIG. 9 is a detail of the anchor element of the embodiment of FIG. 5 in a collapsed configuration.

FIG. 10 is a detail of the anchor element of the embodiment of FIG. 5 in an expanded or deployed condition, shown outside the IVC.

FIGS. 11 and 12 are perspective views illustrating a further alternative embodiment of anchoring elements, in deployed and collapsed configurations, respectively.

FIG. 13 is a perspective view illustrating the embodiment of FIGS. 11 and 12 as it may appear deployed within the IVC (note that for illustration purposes the orientation is not intended to be anatomically accurate in this or similar figures).

FIGS. 14 and 15 are perspective views illustrating yet another alternative embodiment of an anchor element, in the collapsed and deployed configurations, respectively.

FIG. 16 is a perspective view illustrating the embodiment of FIGS. 14 and 15 as it may appear deployed within the IVC.

FIG. 17 is a side view illustrating another alternative embodiment of an implantable IVC monitor with a stent-like anchor element and electronics capsule.

FIGS. 18 and 19 are perspective views illustrating a further embodiment of an anchor element shown in the collapsed and expanded/deployed configurations, respectively.

FIG. 20 and 21 are perspective views illustrating the embodiment of FIGS. 18 and 19 as it may appear deployed within in IVCs of different dimensions.

FIG. 22 is a schematic illustration of a further embodiment of implantable device positioned in the IVC according to the present disclosure.

FIG. 23 is a schematic illustration of yet another embodiment of implantable device positioned in the IVC according to the present disclosure.

FIG. 24 is a schematic illustration of a further embodiment of implantable device according to the present disclosure.

FIG. 25 is a schematic illustration of a further embodiment of implantable device positioned in the IVC according to the present disclosure.

FIG. 26 is a schematic illustration of another embodiment of implantable device positioned in the IVC according to the present disclosure.

FIGS. 27A and 27B are schematic illustrations of a further embodiment of implantable device according to the present disclosure.

FIGS. 28A, 28B and 28C are a series of schematic illustrations showing delivery and placement of an embodiment of a device configured for external placement on the IVC according to an alternative of present disclosure.

FIG. 29 illustrates another alternative device embodiment deployed in the IVC [1A-005].

FIG. 30 schematically depicts an alternative embodiment of a system described in the present disclosure.

FIG. 31 schematically depicts an embodiment for detection of markers in a deployed device using ultrasound.

FIG. 32 schematically depicts an arrangement of markers and two sensors on a transverse cross-section of the body in a system according to one disclosed embodiment.

FIG. 33 schematically depicts another alternative embodiment of a system described in the present disclosure.

FIG. 34A illustrates placement or injection of a marker between the medial and adventitial layers of the wall of the IVC according to one exemplary embodiment disclosed herein.

FIG. 34B illustrates delivery and adherence of a marker to the outer surface of the wall of the IVC in another exemplary embodiment disclosed herein.

FIG. 35 illustrates another exemplary embodiment in which a marker is deployed through a delivery catheter that holds the marker between two jaws until it reaches the distal end of the delivery catheter, at which point the jaws separate to release the marker.

FIG. 36A illustrates an embodiment of a guidewire coil.

FIG. 36B illustrates a guidewire coil coated with a polymer to permanently entrap air to provide echo-reflective characteristics.

FIG. 36C is a close-up or enlarged view of a section of a coiled ribbon marker with surface texture configured to increase echo-reflectivity.

FIG. 36D illustrates another embodiment of a marker, which may comprise a simple echo-reflective tube such as a sealed tube of air.

FIG. 36E illustrates another embodiment of a marker, in this case a tube of cast polymer such as silicone with echo-reflective gas bubbles embedded in the tube wall.

FIGS. 37A, 37B and 37C illustrate various embodiments of markers formed as particles in accordance with alternative embodiments disclosed herein.

FIG. 38 is an enlarged view of a further exemplary embodiment of a marker as disclosed herein comprising a gel mixed with marker particles injected into the wall of the IVC.

FIG. 39A is a cross-sectional view of a particle/marker containing patch endothelialized into the IVC wall.

FIG. 39B is a cross-sectional view of an alternative marker patch utilizing a “Velcro-like” texture of microneedles or microhooks to adhere to and embed into the IVC wall.

FIG. 40A illustrates balloon delivery of one or more markers in accordance with a further alternative embodiment disclosed herein.

FIG. 40B illustrates another alternative embodiment in which a two-balloon catheter is used such that blood flow may be maintained during marker delivery and placement.

FIG. 41 illustrates an exemplary embodiment of an external transmitter/receiver configured to provide more consistent and precise measurements of relative distance between IVC two markers as described herein.

FIG. 42 schematically depicts another alternative system employing communicating monitoring and therapeutic devices.

FIG. 43 schematically depicts a further alternative system employing direct communication through the IVC wall.

FIG. 44 schematically depicts yet another alternative system employing intravascular leads for direct communication.

FIG. 45 illustrates one exemplary embodiment of a pulmonary artery sensor being implanted by a delivery catheter in the pulmonary artery following implantation of an IVC monitoring device in the IVC.

FIG. 46 is a block diagram illustrating embodiments for communication and computerized implementation of various embodiments described herein.

FIG. 47 illustrates a typical timeline of symptoms leading to hospitalization for ADHF.

DISCLOSURE OF EMBODIMENTS

[0033] Various embodiments disclosed herein are intended to monitor for and detect variations in volume and/or pressure of the inferior vena cava (IVC) as an early warning signal of the acute severity of heart failure. Implantable IVC monitors, markers and related systems, devices and methods as described herein may enable the patient and physician to take proactive

steps in time to prevent acute decompensation requiring hospitalization. Such devices and methods also may be helpful in managing hemodialysis patients, in whom volume management is a chronic challenge. The present disclosure thus describes methods and devices for measuring IVC volume and/or pressure more or less continuously, depending on clinical need, using various forms of implantable devices.

[0034] In order to measure changes in IVC dimension or volume accurately, the devices of the invention must be configured to be secured at the desired location in or on the vessel without affecting the natural dilation and constriction of the vessel, or by affecting it in a way which is known and predictable so that it can be accounted for. In many of the embodiments disclosed herein, implantable monitoring devices include an anchoring member which secures the device to the vessel and immobilizes the device both longitudinally and rotationally, and a sensing or marking element which responds to vessel expansion and contraction to allow monitoring of changes in vessel dimension. It is critical in such embodiments that the anchoring element not distort the vessel dimensions being measured by the sensing/marketing element. In preferred embodiments, the sensing or marking element is isolated from the anchoring member such that the vessel can naturally expand and contract at the site of measurement without significant constraint. In some embodiments, this isolation comprises a longitudinal separation of the sensing/marketing element from the anchor member a distance sufficient to minimize the effects of the anchor on the vessel motion at the measurement site. In such embodiments the sensing/marketing element will be coupled to the anchor member by an elongated connecting element which has a length and flexibility sufficient to provide the necessary isolation, which has sufficient rigidity to maintain the position of the sensing/marketing element at the measurement site, and which, in many embodiments, has the appropriate shape and resilience to bias the sensing/marketing element against the wall of the vessel as it moves inward and outward. Such connecting elements will also have a length selected to allow the anchor member to be implanted in the desired location in the IVC, in preferred embodiments just inferior to the hepatic veins, with the sensing/marketing element positioned in the IVC between the anchor member and the right atrium. In certain exemplary embodiments, such connecting elements will have a length in the range of 1 to 4 times the vessel diameter (e.g. 1-8 cm), more desirably 1 to 3 times the vessel diameter (e.g. 2-6 cm), and preferably 1 to 2 times the vessel diameter (e.g. 2-4 cm). In some embodiments it will be desirable to provide a longitudinal separation between the anchor element

and the marker elements of about 3-5 cm. Also, it may be desirable to position the anchor elements somewhat inferior to the renal arteries so that the marker elements fall between the renal and hepatic veins. In one preferred embodiment, the marker elements are positioned at a monitoring location falling in a region from approximately 2 cm below the hepatic veins down to, but not below the renal veins. In other embodiments, instead or in addition to spatial separation of the anchor and sensor/marker, isolation may be achieved by a mechanical coupling between the anchor and the sensing/marketing element which mechanically isolates movement of the sensing/marketing element from the anchor, such as a spring, hinge, flexible link, or other type of isolating coupling.

[0035] Because heart failure patients often receive catheters for monitoring and treatment which are inserted through the IVC, preferred embodiments of the invention will be configured to allow the placement of catheters and other devices past the location of the implanted monitoring device without risk of displacement or compromising its function. In some embodiments, the devices of the invention are configured to be anchored to the vessel wall without jailing (i.e. extending across) or substantially occluding the vessel lumen.

[0036] In certain embodiments described herein the monitoring devices of the invention are configured to measure vascular dimension in a predetermined direction or along a predetermined axis. Such embodiments are configured to facilitate implantation within the vessel in a position which enables such directional measurement. In exemplary embodiments, the devices of the invention are configured to measure IVC diameter in the anterior-posterior direction. In such embodiments the devices are configured to preferentially position and maintain the sensing or marking elements against the posterior and/or anterior wall of the IVC throughout the respiratory cycle. Exemplary embodiments may further include anchoring elements that deploy in such a way as to preferentially position the device in the desired rotational position in the vessel. For example, such anchoring elements may have a shape or include features which take advantage of the oval cross-sectional shape of the IVC and naturally seat themselves in the desired rotational orientation.

[0037] One type of device disclosed herein, as shown, for example, by the embodiment in FIG. 1, may have flexible marker elements, such as flexible electrodes, that lay unobtrusively

against the wall of the IVC. Various embodiments of this type of device are described in more detail below. As the marker element positions change relative to one another based on changes in shape/volume of the IVC, the change may be determined through signals or feedback exchanged between the marker elements. For example, as the IVC decreases in volume, it may go from being fully inflated with a round shape to a flatter shape. In a design with a number of marker elements deployed circumferentially around a cross-section of the IVC, this means that certain marker elements may become closer together as the IVC collapses, and some may move farther apart. FIGS. 2A, 2B, 2C and 2D schematically illustrate how this change may occur. As is seen, the variation in proximity of the marker elements with IVC collapse depends upon the orientation of the device relative to the axis of collapse of the IVC. In FIGS. 2A and 2B, it is seen that marker elements a and c become closer as the IVC collapses, while marker elements b and d move farther apart. In FIGS. 2C and 2D, marker elements a and b and c and d become closer as the IVC collapses. Alternatively, a single marker element may be provided with a signal type that may be reflected off of the opposite IVC wall. The same principals apply when a single marker element is used with a signal reflected off the opposite IVC wall. In one such example, the single marker element may be positioned at location a in FIGS. 2A and 2B, with the reflected wall being generally at location c, directly across from a.

[0038] In general, marker elements used in embodiments disclosed herein may be active marker elements or passive elements. Examples of active marker elements include ultrasound transducers, electrodes and inductance coils. Passive marker elements are generally signal reflective, such as echo-reflective, which can reflect an ultrasound signal directed at the marker elements from outside the body. In an embodiment where the market elements are comprised of electrodes, it may be most effective to determine which electrodes are positioned most directly on the anterior and posterior walls, and to measure the variation in impedance between those electrodes. Alternatively, the system could measure the impedance from each electrode to each of the others, and to use the variation in impedances to estimate the change in shape. Or it may be equally effective to combine the impedances of all of the opposing electrode pairs in parallel, and look at the variation in that single overall impedance reading.

[0039] In certain situations it may alternatively or also be effective to measure the longitudinal impedance along the length of the IVC or the superior vena cava (SVC), or both. As

the IVC and/or SVC collapses, the cross-sectional area of the IVC and SVC decreases, which may lead to a meaningful change in impedance along its length. One exemplary embodiment employing this alternative is illustrated in FIG. 35 as described below.

[0040] In addition to simply measuring impedance across the IVC by use of implantable, flexible electrodes, there are a number of other ways by which an implantable device may measure the variation in shape of the IVC. Such further alternatives include elements such as strain gauges or displacement sensors attached to a radial or circumferential element of the device, proximity sensors, *etc.* One exemplary embodiment in this regard is illustrated in FIG. 24 as described below.

[0041] Fluid pressure sensors may also be useful in measuring variations in IVC status. Alternatively, the flow rate through the IVC might be measured using a Doppler ultrasound sensor or other sensor. As the volume and cross-sectional area of the IVC change, the speed of blood flow through the IVC might change inversely and proportionately, although blood volume and flow will also change with changes in posture, exercise level, and so on. In this approach, it might be helpful to measure heart rate as well as an indicator of cardiac output, to normalize flow rates or to make certain that measurements are only being taken when the patient is at rest. Inertial sensors might also be included, to measure posture and motion. MEMS inertial sensors have been developed which are tiny and consume very little battery power. It might also be helpful to implant a reference pressure sensor or inertial sensor elsewhere in the body or vascular system, such as in the leg, to detect posture changes and activity level.

[0042] A further alternative measurement means is to use sonomicrometry. This involves tiny piezoelectric crystal sensors which emit tiny sonic signals, which are then detected by other sensors and converted to an electrical signal. By analyzing the time between the transmission and reception of these signals, the distance between the crystals can be accurately measured. A further alternative measurement means is to transmit a sonic vibration into the IVC, and by measuring the reflection or resonance of that signal, the overall volume or dimensions of the IVC might be determined.

[0043] The choice between these different methods will depend in part on determining which ones measure the variation in IVC volume and pressure most consistently and precisely.

Minimizing energy consumption is also an essential factor for implantable devices which are intended to function for years, unless external power sources are used to power or re-charge the device.

[0044] In alternative embodiments, one or more devices may be implanted on an external surface of the IVC to detect changes in vascular dimensions. For example, a single device having two spaced-apart electrodes, or two separate devices each with its own electrode, may be anchored to the outer IVC wall and used to measure impedance between the electrodes. Alternatively, a device having a strain gauge may be anchored to the outer wall to measure stress, strain, or displacement between two points on the wall. In another embodiment, a wire loop or band incorporating a force or displacement sensor may be placed around the IVC to detect changes in IVC circumference based upon the change in size or tension in the loop or band. Such devices may be miniaturized so as to be delivered using a large-bore needle or other low-profile delivery instrument that can be placed through a small puncture in the thoracic or abdominal wall and delivered to the desired location on the IVC.

[0045] This monitoring may be performed continuously or intermittently, depending upon the desired tradeoff between data intensity and battery life. It might be most efficient to take measurements only at night, when the patient is lying down and at rest. It might be desirable to intermittently measure IVC dimensions at random, or at specific time intervals. Although these intermittent measurements might result in measuring the IVC distention at random points in the cardiac and respiratory cycle, over a period of minutes, hours, or days an effective picture of the IVC variation may become clear. Alternatively, the device may intermittently take continuous measurements over one or more entire cardiac and/or respiratory cycles, to get an effective measurement of the maximum and minimum IVC volumes. The difference between those minimum and maximum volumes may be an important prognostic indicator. If there is only a small variation between minimum and maximum IVC volumes, that may be an indicator of congestion.

[0046] Exemplary embodiments shown in the figures will now be described in more detail to further illustrate various configurations and designs of the disclosure. As will be apparent to persons of ordinary skill in the art based on the teachings herein contained, different features of

the various disclosed embodiments may be employed with embodiments other than those with which they are specifically shown in the drawings for purposes of illustration. Given the number of possible combinations, it is not possible within a concise disclosure to separately illustrate each combination of features as would be understood by those skilled in the art. As non-limiting examples, each of the different **anchor elements** shown in FIGS. 5-21, and the **marker elements** shown in FIGS. 1, **3-5**, 22-30 may be used together in different combinations or individually with each different implant herein.

[0047] As shown in FIG. 1, monitoring device 100 may have several flexible, insulated arms 103 that lay passively against the wall W of the IVC. Marker elements 106 (referred to hereinafter generically as marker elements or by specific marker element type, such as electrode, coil or ultrasound element, *etc.*) may be mounted on arms 103, preferably at an end spaced from the body of device 100. In one exemplary embodiment, marker element 106 comprise electrodes 106 mounted on arms 103, and the impedance between the electrodes may be monitored via suitable monitoring devices and means as described further below. There may be as few as two, three, or four electrodes 106, or there may be many. There also may be more than two arms 103. If there are just two arms 103, they may generate the most effective measurements if positioned against the anterior and posterior walls of the IVC. Electrodes 106, or other marker element, may be arrayed circumferentially around the IVC at one specific cross-section, or there may be electrodes at two or more specific cross-sections, or they may be arranged over the length of the IVC. Impedances may be measured in a matrix between all of the different electrodes, or the system may focus on measuring impedances just between electrodes on opposing walls, to measure any collapse of the IVC most efficiently.

[0048] Alternatively, instead of measuring impedance between electrodes, marker elements 106 may comprise inductance coils that may be located at the ends of arms 103 of device 100 in FIG. 1. A small current could be delivered to one coil, and the induced current in the other coil could be measured to determine the distance between the coils.

[0049] A further alternative embodiment comprises positioning two ultrasound crystals as marker elements 106 on opposing arms 103 of device 100. An ultrasonic signal from one crystal could then be detected by the opposing crystal, and the diameter of the IVC could then be

determined by measuring the time-of-travel between the two crystals. Alternatively, and as described further below, a single ultrasound crystal could be positioned on a single arm of the device with the crystal acting as both emitter and receiver of an ultrasound signal such that vessel diameter could be determined by reflecting a signal against the opposing wall of the vessel and measuring time of travel back and forth from the crystal.

[0050] Device 100 may be located entirely within the IVC as shown in FIG. 1. In this exemplary embodiment, device 100 is held in place by anchor element 109, comprising a radially expanding stent, which has hooks 112 that engage the IVC wall W. Multiple arms 103 extend superiorly along the IVC, and are biased gently outwards to hold themselves against the IVC wall W. At the end of arms 103 are marker elements 106, which may be electrodes as described above. Device 100 senses changes in impedance between the marker element electrodes to measure the degree of distention or collapse of the IVC. Alternatively or in addition, device 100 may also include arms 103 extending inferiorly, holding another set of marker elements 106 against the IVC wall W in a more inferior position, which can also be used to determine the variation in IVC size. Anchor element 109, such as the illustrated radially expanding stent, may be made gentle enough so as to not prevent the distention or collapse of the IVC. In that case, marker elements 106 (here illustrated as electrodes) may be mounted directly on the anchoring element itself. Various similar embodiments disclosed herein, may be important to encapsulate the structure and arms of the device in an electrically insulative material, so that it doesn't prevent the measurement of IVC cross-section via impedance measurements.

[0051] In a further alternative, anchor element 109 (such as, for example, the stent shown in FIG. 1 or in FIG. 23) and/or arms 103 may be made of a bioerodable material which softens over time, to minimize any effect the structure might have on the natural motion of the IVC. The structure of arms 103 (or anchor element 109) may also be designed to aggressively heal into the walls of the IVC, to minimize the risk of migration or embolization over time. Such alternatives may also be combined, for example, by making the anchor element or arms out of a bioerodable material such as poly-L-lactide (PLLA) and covering the struts of the device with a woven or braided polyester sleeve or open-cell expanded polytetrafluorethylene (ePTFE). As the struts erode over time, they will stimulate a somewhat inflammatory response which will encourage the

fabric to heal into the wall, so that by the time the PLLA structure is gone, the device will be well-healed into the wall.

[0052] The IVC is large enough that a low-profile electronics control housing, such as capsule 118 in FIG. 1, can be located on an implantable device such as device 100 without meaningfully occluding blood flow through the IVC. Such an electronics capsule also may be configured and dimensioned to be entirely positioned against the walls of the IVC, so that the central channel of the IVC remains open and unimpeded for the introduction of any other catheter in the future. Electronics capsule 118 may have either a battery or inductive coil or both to power the device. Alternatively, or additionally, the device may be designed to harvest energy from local environmental sources by including, for example, a piezoelectric generator to produce power from the pulsation of the heart. In addition, the electronics capsule will have connections to the marker elements and a telemetry circuit to communicate information to a controller unit (not shown) outside the patient's body. Preferably the device includes a wireless transmitter to transmit sensor data to an external receiver and controller. The device may be configured to transmit continuously or at programmed intervals, or to transmit data upon interrogation by an external device. It may also have a memory circuit to store historical sensor measurements, and a calculation circuit to convert the various sensor measurements to an estimate of IVC distention or collapse. Additionally or alternatively, the device may be configured to communicate with a wireless-enabled cellular device such as a smartphone, which may include software to transmit data via cellular or wireless network to a remote computer. In this way, the measured IVC parameters may be automatically transmitted to healthcare providers to allow monitoring of the patient's condition. More details of related control and networking embodiments are discussed below.

[0053] Device 100, as illustrated in FIG. 1, is shown positioned largely superior to the renal veins within the IVC. However, implantable devices as disclosed herein also may be positioned partially or entirely inferior to the renal veins, or even within the right atrium or the superior vena cava (SVC). Alternatively the devices may have multiple components implantable in different locations, such as one component in the IVC, and a second component in the SVC or elsewhere.

[0054] In an alternative embodiment, device 300 may have a secondary element 321 that deploys portions of the device within the vascular system much closer to a point of insertion, or at another location more easily accessed (for physical access or energy transfer), as shown in FIG. 3. In this embodiment, device 300 includes IVC sensing unit 323 (which may be generally configured including anchor element(s) and marker element(s) as described with respect to other embodiments disclosed herein), with secondary element 321 located remotely from the sensing unit 323, and lead 329 connecting and providing communication between the two units. For example, an antenna element for telemetry and/or an inductive coil may be placed in secondary unit 321 in the subclavian vein or jugular vein. This would make it much easier to accurately position an external power source and/or controller antenna 332 close to the antenna or inductive coil contained within secondary unit 321. The secondary unit 321 may be held in place, for example, using a self-expanding stent or other intraluminal anchor element as described herein.

[0055] Alternatively, an implantable device according to the present disclosure may have an implantable battery and circuitry that can be implanted within the body, but outside of the vascular system as shown in FIG. 4. Device 400 comprises IVC sensing unit 423 (which also may be generally configured as described with respect to other embodiments disclosed herein) and implantable controller/battery unit 426 connected to sensing unit 423 by lead 429 providing communication there between. There are similarities between placement of device 400 and the common placement of pacemakers and defibrillators in an infra-clavicular pocket. However, unlike those common devices, lead 429 between the IVC sensing unit 423 and placement location of controller/battery unit 426 would not need to traverse any heart valves, which may make it a relatively safe and simple connection. Alternatively, IVC sensor 423 may be adapted to connect to a pacemaker or defibrillator, including additional leads providing sensing and stimulation of the heart, for example, as described below in connection with the embodiment of FIG. 45.

[0056] A further exemplary embodiment is shown in FIGS. 5-10. As shown therein, device 500 comprises three major components or assemblies, electronics capsule 503, anchor element 506 and anchor isolation structure 507 connecting the electronics capsule and anchor element. Electronics capsule 503 comprises a sealed housing 509 for containing control, power and other alternative functional modules as elsewhere described herein to provide a self-

contained, sealed device. Capsule 503 also provides support for marker element 512, which in the case of device 500 is a single ultrasound marker element positioned at the inferior end of the device. Such a marker element may utilize one or more ultrasound crystals to measure IVC diameter by emitting an ultrasound pulse, and then detecting the reflection of that pulse from the opposing wall of the IVC. Other modes of detection with ultrasound receivers and/or other marker element types as described herein may be alternatively employed by persons of ordinary skill without departing from the teachings of this disclosure. Electronics capsule 503 generally will be provided with the lowest possible profile so as to minimize obstruction of the lumen when positioned in the IVC.

[0057] Electronics capsule 503 is connected to anchor element 506 at the superior end of the capsule. Anchor element 506 as depicted in this embodiment includes a single anchor wire 515 configured in a generally figure-eight or double helix shape. Alternatively, the same configuration can be provided with two or more wires. Anchor wire 515 is pinned to telescoping deployment member 518 at both its inferior end 521 and superior end 524. Telescoping deployment member 518 includes inner member 527, which is secured to electronics capsule 503, through anchor isolation structure 507 and outer member 530. Relative motion between inner member 527 and outer member 530 moves anchor wire 515 from a collapsed position, shown in FIG. 9, to a deployed or anchoring position, shown in FIG. 10.

[0058] Various actuation mechanisms may be utilized for deploying and securing anchor element 506. In one alternative, anchor wire 515 is resilient, with shape-memory properties configured to provide a rest state in the deployed configuration. In this alternative, device 500 may be delivered to the desired location in the IVC via a conventional guide catheter or other suitable sheath type delivery device. When position is confirmed as described below, device 500 is ejected from the delivery catheter or sheath with anchor element 506 self-deploying upon ejection.

[0059] In another alternative deployment mechanism, an actuating wire (not shown) is removably connected to deployment member 518 at superior end 524 using a mechanical release mechanism, for example a screw threaded connection, spring release, hooks or other such means known in the art. The actuating wire may be a single or double wire, which may be coaxial or

parallel, depending on the mode of actuation. In this alternative, movement of the actuating wire effects relative movement of the inner and outer deployment members 527, 530 to deploy anchor wire 515 from the collapsed configuration to the expanded, deployed configuration as explained above. After deployment of the anchor element, the actuating wire is released from device 500 according to its mode of connection and released to leave the device secured in the IVC via anchor element 506.

[0060] As mentioned above, a further feature of this and other embodiments disclosed herein is the spacing between the marker element position relative to the anchor element, provided by anchor isolation structure 507. In general, it is preferred if the anchor element is positioned sufficiently distant from the marker elements so as to not have an effect upon the IVC size or shape at or close to the location of measurement due to the anchoring force imparted to the IVC wall. Anchor isolation structure 507 ensures the desired positioning, which may be approximately 1 to 4 times the IVC diameter as indicated above. In general, the IVC has a somewhat oval cross section with a minor axis of the oval extending in the anterior-posterior direction and a major axis extending in the lateral-medial direction. It is thus desirable to minimize any effect of the device on this natural oval shape at or close to the point of measurement.

[0061] The shape of the IVC and possible effect of the anchor element on the IVC shape is illustrated, in one possible configuration, in FIGS. 5-8. As shown therein, at the more inferior portion of the IVC, proximate marker element 512, the IVC assumes its more natural oval shape as best seen in FIG. 7. However, at the superior portion where subjected to the force of anchor wire 515 of anchor element 506, the IVC is forced into a more circular shape as best seen in FIG. 8. Thus, not only does the anchor element potentially distort the shape of the IVC, it may also stiffen the IVC so as not to be as responsive to varying fluid volumes which may indicate heart failure risk. Anchor isolation structure reduces or eliminates such problems as might otherwise be associated within sensing devices positioned in the IVC.

[0062] In order to achieve accurate measurement with marker element 512 using an anchor configuration of the type shown in FIGS. 5-10, the entire device, from deployment member 518 through anchor isolation structure 507 into electronics capsule 503 should be provided with a

stiffness sufficient to maintain the electronics capsule (and marker element) against the wall of the IVC at one side and yet provide sufficient flexibility (and smoothness) to avoid damage or erosion of the IVC wall by contact with device 500 over the remaining lifetime of the patient.

[0063] As also shown in FIGS. 5-8, it may be most advantageous if the device, such as device 500, or other device disclosed herein, is positioned with the electronics capsule 503, and more specifically the active marker element (*e.g.*, ultrasound marker element 512), against the posterior wall of the IVC so as to measure the distance to the anterior wall. This arrangement may offer advantages in accuracy and sensitivity in measurements by measuring along the minor anterior-posterior axis of the oval IVC shape, and by measuring from the posterior wall, bony structures lying behind the posterior wall, which may create artifacts or other interference with ultrasound measurements may be avoided. Such positioning may provide for the greatest accuracy in measurement of diameter over the respiratory cycle (*e.g.*, measurement of diameter variability vs. static measurement). While a single ultrasound marker element 512 is shown for device 500, a similar device with more than one ultrasound crystal may be positioned elsewhere in the IVC, for example in the center of the IVC, with two crystals measuring the distance to the anterior and posterior walls simultaneously. Specific requirements for positioning and measurements may be clinically determined based on patient anatomy as determined by the procedure provider, and the device to be implanted may be modified according to the teachings contained herein to suit those specific patient requirements.

[0064] In general, devices as disclosed herein may be positioned at any suitable position in the IVC based on clinical assessment. In one example, the marker element of the device, such as an ultrasound crystal, may be disposed at the cranial end of the device, with the cranial end then positioned in the IVC between the renal veins and the hepatic veins. In this case, the anchor element may be disposed at the opposite, caudal end of the devices and thus positioned in the IVC inferior to the renal veins. Also, when positioning the device on the posterior wall of the IVC, it may be desirable to ensure that the device is centrally located on the posterior wall and oriented at least substantially straight across the minor axis for most accurate measurements. Positioning of the device in the IVC may be controlled using convention catheterization techniques with observation under fluoroscopy. However, in a device such as device 500, marker element 512 may be used to assist in confirming placement by slightly rotating

electronics capsule 503 so as to effectively scan the opposite IVC walls with the ultrasound sensor to detect placement position relative to the oval IVC cross-sectional shape.

[0065] In a further alternative embodiment in FIG. 5, additional anchor elements may be provided on electronics capsule 503, such as barbs 533. It is to be noted, however, that while barbs 533 are shown in FIG. 5, they are an optional feature. Basic operation of anchor element 506 is described above. As anchor element 506 opens, it shortens and tends to pull back on electronics capsule 503. Through a linkage between barbs 533 and deployment member 518, the relative movement of those two parts during deployment of anchor element 506 may be used to deploy barbs 533 from the back of electronics capsule 503. Anchor element 506 and barbs 533 may be positioned to engage the IVC wall in opposition to one another to reinforce the anchoring force and security. However, as previously indicated, substantially the same device may be alternatively provided without anchor barbs 533, held in place only by the collapsible/expandable double helix anchor wire 515 of anchor element 506. These anchor structures, as well as further alternative anchor structures described below, are configured to achieve secure fixation against both longitudinal and rotational movement while preferentially maintaining at least the marker element in the posterior aspect of the IVC, most preferably against the posterior IVC wall. The anchor elements described also can be deployed and redeployed multiple times during a placement procedure in order to ensure the most optimum placement of the device. The shape or configuration of the anchoring wire also may be adapted for IVC size and shape using different anchor element configurations as exemplified by the following additional alternatives.

[0066] The anchoring elements exemplified herein may take a wide variety of alternative shapes, as shown generally in FIGS 11-21. Such alternatives may or may not utilize one or more aspects of the “double helix” anchor wire design discussed above

[0067] Alternative anchor element 1100 is shown in FIGS. 11 and 12. Anchor element 1100 includes two separate wire loops 1103 and 1106 secured to deployment member 1109, which is comprised of an inner member 1112 and concentric telescoping members 1115 and 1118, which are in turn covered by outer telescoping member 1121. Wire loop 1103 is secured to inner member 1112 and covered directly by inner concentric telescoping

member 115. Second wire loop 1106 is also secured to inner member 1112, either by access through an opening in the concentric telescoping members or by an attachment wire that extends along the inside of telescoping member 1118 and is secured at the remote end to inner member 1112. Alternatively, second wire loop 1106 may be secured directly to the second concentric telescoping member 1118. In the collapsed configuration each wire loop is covered at least in part by one of the telescoping members. To deploy the anchor element, the telescoping members are pulled back, either by self-deployment forces generated by the wire loops or by actuation with external means as previously described. FIG. 12 shows anchor element 1100 in its fully collapsed state with the anchor wires and concentric telescoping members 1115, 1118 covered by outer telescoping member 1121. Also shown in FIGS. 11 and 12 is a further alternative electronics capsule 1124, which is joined to anchor element 1100 by anchor isolation structure 1127.

[0068] FIG. 13 illustrates anchor element 1100 and electronics capsule 1124 as it may appear when deployed within the IVC. Anchor wire loops 1103 and 1106 are released to extend outwardly to contact the IVC wall while leaving the central portion of the IVC unobstructed to allow access for other procedures and to minimize restriction of blood flow.

[0069] FIGS. 14-16 illustrate another alternative anchor element 1400. In this embodiment, mesh sleeve 1403, secured at one end to anchor wire 1405 is deployed over inner member 1408 to which anchor wire 1405 is secured. Once again, relative movement between inner member 1408 and mesh sleeve 1403 controls deployment or collapse of the anchor wire 1405. Anchor element 1400 is depicted in FIG. 16 as deployed within the IVC with wire anchor 1405 engaging the IVC wall.

[0070] FIG. 17 illustrates a collapsible, tubular, stent-like alternative anchor element 1700. Anchor element 1700 may be formed of braided wires, welded wires, spiral wound wire, or laser-cut tube, and is preferably a resilient self-expanding metal or polymer. Electronics capsule 1701 is depicted as attached to one end of the anchor element. Weld or cold bond 1703 with biocompatible materials may be used to attach the electronics capsule to the anchor element. Anchor element 1700 may be deployed through a guide catheter in a manner similar to conventional stent deployment. Advantageously, such a tubular anchor element provides secure

anchoring in the vessel while leaving the vessel lumen patent to allow introduction of catheters and other devices without disruption of the monitoring device.

[0071] FIGS. 18-21 illustrate yet another alternative anchor element 1800 coupled with electronics capsule 1801. In this embodiment, anchor wire loops 1803 and 1806 in this embodiment are secured at opposite ends to inner member 1809 and outer member 1812. In this manner, relative movement between inner member 1809 and outer member 1812 permits deployment of the anchor wires without a covering sheath. The anchor wires may be again collapsed by an opposite relative movement between the inner member and outer member. FIGS. 20 and 21 show how anchor element 1800 may be deployed in different sized IVCs. In this embodiment, anchor wire loops 1803 and 1806 are relatively longer such that they may cross multiple times when less than fully expanded to accommodate smaller size IVCs, as is apparent from a comparison of FIGS. 20 and 21.

[0072] As should be apparent to those of ordinary skill in the art, each of the anchor element configurations described above includes common features of secure anchoring with a virtually unobstructed IVC, even when the anchor elements are fully deployed. By minimizing or eliminating obstruction of the IVC, combined with positioning of the anchor elements remote from sensing elements and location, embodiments of the present disclosure may remain positioned in the IVC over longer periods of time without affecting the natural tendency of the IVC to collapse or expand when venous pressure or volume is changed.

[0073] While it is anticipated that in most cases it will be desirable to maintain an unobstructed pathway through the IVC as provided by exemplary anchor elements described above, in some cases it may be desirable to integrate a monitoring device as described herein with an IVC filter, as shown for example in FIG. 22. In addition to monitoring IVC distention, device 2200 would trap any clots embolizing from the legs and prevent them from reaching the lungs as is understood with respect to IVC filters as stand-alone devices. Device 2200 includes electronic capsule 2203 with battery, connections to the sensor, memory, telemetry, etc., stent-like anchor element 2206 with anchor members 2209, and flexible arms 2212 supporting marker element 2215. In this embodiment, marker element 2215 are depicted as electrodes, which may be substantially the same as the electrodes described above in connection with the embodiment

of FIG. 1. In addition, arms 2218 at the superior end of device 2200 extend across the lumen of the IVC and intersect to form a basket to retain any clots which embolize from the legs.

[0074] FIGS. 23 and 24 show devices 2300 and 2400, respectively, configured to measure the longitudinal impedance along the length of the IVC or the superior vena cava (SVC), or both. Device 2300 includes anchors 2303 to engage the IVC and secure electronics capsule 2306. One electrode 2309 is provided relatively closer to electronics capsule 2306, and an insulated straight or spiral wire 2312, which lays against the IVC wall, leads to second electrode 2315 located more superiorly in the IVC, right atrium, or SVC. Rather than applying a simple direct current voltage between these two electrodes to measure the impedance, it may be more effective to apply a particular alternating-current frequency that exhibits a lower impedance through blood and a higher impedance across the IVC wall and through other tissues. This would allow such a device to measure the variation in IVC volume even more effectively. Alternatively, a device may measure a combination of the change in both longitudinal and radial impedance, to gather an even more effective measurement of the change in IVC volume.

[0075] FIG. 24 further shows device 2400, shaped similarly to a standard IVC filter, which uses the variation in bending of struts 2403 to apply pressure to pressure sensors 2406 on central body 2409 of the device. Struts 2403 extend radially outward from body 2409 and have distal tips 2412 configured to engage and anchor to the wall of the IVC. Struts 2403 have flexibility and resilience so as to move with the wall as the vessel contracts and expands, thereby changing the forces exerted by the struts on sensors 2406. Electronics capsule 2415 is contained within body 2409 providing power, control and communication for sensors 2406.

[0076] FIG. 25 shows another embodiment, device 2500, configured similarly to an IVC filter. However, in this embodiment, device 2500 is provided with lateral struts 2503, which are intended to anchor the device in the IVC, and anterior-posterior struts 2506, which are intended to flex with the movement of the anterior and posterior walls of the IVC. Therefore, the distance between marker elements 2509, such as sensors or electrodes, on the anterior and posterior struts can be measured. As with other embodiments, device 2500 includes electronics capsule 2512, which provides structural support for the struts and contains necessary power and control functions as elsewhere described.

[0077] FIG. 26 shows a further alternative embodiment in which device 2600 is comprised as a stent 2603 on which marker element 2606 are disposed at two different cross-sections (lateral-medial and anterior-posterior) of the IVC. Stent 2603 has a resilient, self-expanding configuration which will expand and contract with the IVC. Stent 2603 may be a mesh or woven structure, a simple wire-form having a zig-zag or sinusoid shape, or a series of closed or open cells cut from a tube. Power and control may be provided by integrated power and data transmission components in an electronics capsule as previously described, or marker element sensors directly powered via external energy delivery means, and transmitting information directly to an external module may be provided.

[0078] FIGS. 27A and 27B show another embodiment in which device 2700 is provided with two pairs of arms 2703 held in place by a stent structure 2706. Marker element 2709 (such as electrodes, ultra sound crystals or other sensors as previously described) are positioned at the apex of each pair of arms. These may be oriented in the patient such that one side of each pair extends from the anterior wall of the IVC, and one from the posterior wall. As the IVC collapses as shown in FIG. 27B, the arms tend to scissor together and the apices holding marker elements 2709 move closer together. This change in position may be detected. Alternatively, strain gage type sensors or other angle detection may be used to detect the change in angle from compression alone or in combination with the change in distance sensors. Embodiments such as device 2700 can be configured such that the sensors move relative to each other a distance greater than the actual movement of the IVC wall, thereby magnifying the change in the distance from the anterior to posterior walls.

[0079] Device embodiments as described herein may be delivered into the IVC from a variety of locations. The subclavian or cephalic vein is the normal route of introduction of pacemaker and defibrillator leads, so that these leads can be attached to the pacemaker itself, which is placed in an infra-clavicular pocket just below the subclavian vein. Embodiments disclosed herein may be similarly delivered from the subclavian vein, cephalic vein or the jugular vein, or the femoral vein. Other access points to the venous circulation may also be used.

[0080] One exemplary delivery method for certain embodiments disclosed herein is to have the device to be delivered compressed into a catheter, with a cover sleeve over the device. A

guidewire lumen within the catheter would allow a guidewire to be positioned under fluoroscopy or ultrasound guidance into the IVC, and then the delivery catheter would be advanced over that guidewire into the appropriate location. Once appropriate location is confirmed, the cover sleeve would be retracted, allowing the device to self-expand against the walls of the IVC. Under appropriate clinical indications, disclosed devices may be delivered at the bedside under ultrasound imaging guidance, without the need for fluoroscopy.

[0081] If the device has an electronic lead, the lead may take advantage of all of the designs, materials, and techniques that have been used to optimize pacemaker leads. This lead may extend to a secondary fixation element within the circulatory system, as shown in FIG. 3, or it may extend out of the circulatory system to an implantable element as shown in FIG. 4.

[0082] As a source of power, embodiments described herein may include an inductance coil to power the sensors on the device using a power source from outside the body. Externally powered devices may also include a small battery or capacitor to maintain steady power to the sensors. An external power source could be in the form of a pendant which hangs from a necklace around the patient's neck, or a module which is kept in a shirt pocket, strapped around the patient's chest or abdomen, clipped to the patient's belt, or other locations proximate to the implanted device. It could also be kept at the patient's bedside or under their mattress or pillow, so it can deliver power, take measurements, download data, etc. each evening while the patient is sleeping.

[0083] Given the available cross-sectional area of the IVC and the low power requirements of current implantable device circuitry, embodiments of devices described herein, including a long-term battery and circuitry, may be safely implanted in the IVC without disrupting blood flow. The diameter of the delivery catheter for such a device may be as large as 24-30 French size (8-10mm) if delivered via the femoral vein. The overall implanted device or structural elements also may be used as an antenna to enhance transmission of this data outside of the body, especially, for example, if the device has a stent-like body or multiple metal arms.

[0084] In yet another alternative embodiment, a sensing device may be implanted on the outside of the IVC as shown, for example, in FIGS. 28A-C. In this embodiment, device 2800 is configured to be implanted around the outside of the IVC and thus includes two resilient arms

2803 extending from electronics capsule 2806. Marker elements 2809 are disposed at the ends or elsewhere along resilient arms 2803. Arms 2803 may be, for example, a coated, resilient flexible material or a tubular insulator with a wire inside. Device 2800 may be placed via an otherwise conventional laparoscopic procedure. A right posterolateral access to the abdomen, just inferior and/or posterior to the liver, should allow the surgeon to advance to the IVC. In this manner a resilient loop device such as device 2800 could be wrapped around the IVC, as shown in FIG. 28B. FIG. 28C shows one embodiment of delivery device 2815 containing straightened device 2800. Delivery device 2815 may comprise a tubular member such as a catheter or trocar with a pushing element for delivery and position of device 2800 around the IVC.

[0085] In a further alternative embodiment, a marker element as elsewhere described herein may be implanted against one side of the external wall of the IVC, held in place by sutures, clips, adhesives, or other mechanical attachment means. Such an external sensor type element could measure IVC cross-sectional area via mechanical, sonic, impedance, or other means.

Marker Element Embodiments with External Activation

[0086] Embodiments described above focus on implantable systems with electronics to measure IVC dimensions as well as other physiologically important data, and then transmit that information to a receiver located outside the patient's body. Embodiments described hereinafter include devices, systems, and methods for measuring the IVC employing external instruments to measure IVC dimensions in communication with implanted marker devices, potentially without a need for more complex implants, or implanted active measurement devices and/or the need to transmit measurement data out of the body. Such devices, systems and methods may include passive elements, which are used in conjunction with external instruments for calculating and communicating IVC dimensions. More specifically, disclosed systems may have one, two or more markers that would allow an instrument outside the body to easily measure IVC dimensions without the need for sophisticated training or human analysis. Such systems may use portable, and relatively inexpensive instruments to take the measurements.

[0087] In one disclosed embodiment, shown in FIG. 29, device 2900, including two or more passive elements 2903, is configured to be implanted in the IVC. Passive elements 2903 are themselves configured to reflect a signal directed towards them from outside the body. Such

passive element reflectors may be made of a metal such as Nitinol, or they may be made from any other echoreflective material (or other suitable biocompatible material reflective of the signal employed). Passive elements 2903 are connected by anchor isolation structures 2906 to anchor structure 2909, exemplified here as a stent-like structure, which may be made of Nitinol or other resilient material biased into engagement with the IVC wall. Other anchor elements as described herein may be alternatively employed.

[0088] It will be appreciated by persons skilled in the art that the depiction in FIG. 29, as in other figures presented in this disclosure, is not at a particular scale. Connecting elements 2906 may be suitably elongated to allow the anchoring structure to be placed in a position spaced upstream or downstream from the location of the markers so that the anchoring structure does not affect the natural geometry and movement of the IVC where it is measured by the passive elements as previously described. Passive elements 2903 may be gently biased outwardly against the anterior and posterior walls of the IVC to maintain contact therewith.

[0089] In other embodiments employing passive marker elements, the passive elements may be mounted directly to an anchoring structure such as a stent, and not separated therefrom by connecting elements. Alternatively the marker elements may be stapled, screwed, sutured, or otherwise fastened to the IVC wall. Passive elements such as shown in FIG. 29 may be fenestrated, including grooves, channels, holes, depressions or the like to accelerate the ingrowth of IVC wall tissue over them. The passive elements may also have a surface texture or coating to enhance reflection of the signals. For example, the surface may have a series of grooves or depressions whose walls were at right angles or other selected angles relative to each other to more effectively reflect those signals. Alternatively, such grooves, channels or other features may be arranged on each passive element in unique patterns which make them more clearly identifiable and differentiable from each other and from surrounding structures by an external detection instrument. In other embodiments, the passive elements may be of known size, but oriented at different known angles relative to each other, such as in orthogonal directions (e.g. at least one in circumferential direction and one in the axial direction), so calculating the length and orientation of the reflected signal can determine the location of each passive element in three dimensions.

[0090] It is anticipated that within a few months of their implantation, the passive elements as of the types described herein would be fully healed into the IVC wall. The posterior passive element may be somewhat larger than or offset from the anterior passive element, so that one does not shield the other regardless of where the reading/detecting instrument is held against the anterior abdomen.

[0091] A reading instrument for use with passive elements as described above may comprise a generally conventional ultrasound signal generator and receiver which would be held against the anterior abdomen or thorax outside the body to detect the device in the IVC, as schematically depicted in FIGS. 30 and 31. In this exemplary embodiment, ultrasound system 3000 includes handheld probe 3003 connected to table top control console 3006 and display 3009. Advantageously, ultrasound system 3000 would not need to image the IVC, although optionally may do so. Thus, ultrasound probe 3003 could be provided as a single crystal, intermittently delivering a pulse and measuring the time-of-travel until the reflected echo is detected by the same crystal. Ultrasound probe 3003 transmits a sonic signal, as shown, for example, in FIG. 31, through the body wall BW and the receiver records the reflection of that signal from the two passive elements 2903 elements on device 2900 implanted within the IVC. System 3000 may differentiate the two passive elements in any of various ways, including through differences in their relative distance away, size, shape, patterns of fenestrations, echo-reflective coatings or other features. By a time-of-travel calculation, for example, the relative spacing of the two passive elements could be calculated. By measuring this distance many times per second, an accurate assessment of the variation in IVC dimensions could be made.

[0092] System 3000 may be programmed to look for the appropriate number of signals from the passive elements within the appropriate time period after it transmits a signal. This would minimize the risk of it tracking inappropriate signal reflections from other sources or anatomical structures such as the spine. In use, probe 3003 is held against the anterior abdomen and gently reoriented until it receives an effective echo from all of the passive elements. At this point system 3000 emits an audible signal, shows a green light, or uses other indicator means to confirm to the patient that the instrument is appropriately positioned. System 3000 may also include a strap around the patient's body that could be tightened to hold the device in place, or

the patient could hold it in place manually, or use tape, adhesive, or other means to hold it in place while readings are taken.

[0093] In further alternative embodiments, instead of or accompanying passive elements, more active elements may be included with an implantable device such as device 2900. Such more active elements may comprise piezoelectric or other crystals which absorb incoming sonic signals and re-transmit these signals back to the receiver. Such embodiments may further comprise active elements powered by an externally delivered magnetic, electrical, or ultrasonic field. In such active embodiments, active marker elements, which may be also be schematically depicted by elements 2903 in FIG. 29, could then emit a signal that allows the external instrument to determine position more exactly. In further examples, each active marker element may include an inductance coil or other means to gather energy from a variable external electric or magnetic field; a capacitor or other means to store that energy; and then a piezoelectric crystal to emit an ultrasound signal, along with the appropriate circuitry to manage these elements. Such externally powered active marker elements need not be overly complex, firing an ultrasound signal whenever they are sufficiently charged or excited. Alternatively, the external system may send a triggering signal to tell each marker element when to fire, or to make them all fire simultaneously.

[0094] In embodiments employing active, ultrasound-emitting marker elements, one or more external ultrasound receivers may be arrayed on the body surface to detect the emitted signals. Again using time-of-travel calculations as will be appreciated by persons skilled in the art, the precise location of the active marker elements within the body could be determined. If the active marker elements fired simultaneously, then one ultrasound receiver located on the anterior abdominal wall could be enough to accurately measure the anterior-posterior dimension of the IVC. If they did not fire simultaneously, then more than one receiver may be necessary. The external sensors may be arrayed in a way that maximizes the precision of the anterior-posterior measurement. FIG. 32 shows a transverse cross-section of the body, and one arrangement of two external sensors 3203. The distance from implanted active marker elements 2903, within the IVC, to sensor 3203A on the patient's anterior abdomen will vary directly as the anterior-posterior (A-P) IVC dimensions change, while the distance from implanted active marker elements 2903 to sensor 3203B on the patient's side will change little. By analyzing the

difference in the time it takes for ultrasound signal from each active marker element to reach sensor A versus sensor B, the A-P dimensions of the IVC can be calculated. As long as at least two sensors are used (for example, one on the anterior wall of the IVC and one on the posterior wall), their relative motion could be measured quite accurately, cancelling out other motions such as the rise and fall of the abdominal wall during respiration. Note that elements 2903 may also be implanted on an external surface of the IVC as depicted in the embodiment of FIGS. 28A-C, or may be passive elements if transducers are used instead of sensors 3203.

[0095] Other methods of determining position from passive or active marker elements also may be employed. For example, in one embodiment, the marker elements may comprise one or more small magnets implanted against the IVC wall using device embodiments described herein above, and a sensitive magnetometer could be used to detect the position and motion of the magnet(s). A SQUID magnetometer (Superconducting Quantum Interference Device) could be used to very sensitively measure the variation in location of an implanted magnet, although this device may require a cooling apparatus to bring even a high-temperature SQUID to a temperature where it becomes superconducting. Other types of magnetometers could also be used.

[0096] A further alternative embodiment may comprise the implantation of marker elements, such as containing ultrasound crystals, that show up very brightly on an ultrasound image. Automated image analysis software within the ultrasound system can then automatically detect marker element positions and record them. One embodiment of this approach would be to implant a stent with Nitinol arms that can be easily identified by an ultrasound imaging system using automated software. An implanted device similar to that shown in FIG. 29 could include a stent implanted caudal to the renal veins, and two or more metal arms that extend cranial to the renal veins. For example, one arm could be positioned along the anterior wall of the IVC and another along the posterior wall. A transverse cross-sectional ultrasound image of the IVC cranial to the renal veins will cross these arms, and they will show up as clear marks on the ultrasound image. Image-analysis software could then identify those marks, track them, and measure the variation in IVC dimensions automatically. To make these measurements consistent, the patient or caregiver could be trained to hold an ultrasound imaging transducer on the patient's abdomen in a specific location. Tattoos or other markings on the skin could be used

to identify a consistent location from which measurements are to be taken. In one embodiment, as shown in FIG. 33, a wearable detection system 3300 includes ultrasound probe 3303 that may be fastened in place on the patient via strap 3306 and buckle 3309. Ultrasound probe 3303 may also include windows 3312 mounted on body contacting tabs 3315, or other indicators, that would be placed over or adjacent the location mark on the body to ensure proper location of probe 3303. Ultrasound probe 3303 may communicate wirelessly with an external device 3318, such as a cell phone, which controls the probe, displays the measured data, and transmits it to other systems or cell phones. Alternatively the ultrasound transducer could be shaped so that the transducer is reliably positioned a certain distance from various anatomical points, such as a distance from the bottom of the rib cage.

[0097] A further embodiment is a system that monitors IVC dimensions without implanted elements. For example, a portable, external ultrasound system could comprise a processor and software that analyzes a reasonably consistent ultrasound image of the abdomen to automatically identify the IVC. This software then automatically identifies the anterior and posterior walls of the IVC within that image, and continuously or periodically measures and records the variation in IVC dimensions over time. In such an embodiment, the system would include an emitter and receiver that can be secured to the patient, or that can be positioned at one or more marked locations on the patient's skin, so that measurements are taken from a consistent location. Preferably such a system is contained in a lightweight, compact housing, battery-powered, and small enough to be worn by the patient or easily held by the patient during measurements. System 3300 as shown in FIG. 33 may also be used in this embodiment.

[0098] As a further method of simplifying the identification of the IVC and appropriate positioning of the probe, a three-dimensional ultrasound map of most of the patient's abdomen can be stored in the ultrasound system's memory when the patient first begins using the system. From that point, optimal positioning of the probe and its two-dimensional slice within that three-dimensional volume can be defined. Then, when the patient is imaged in a subsequent measurement, the ultrasound system can compare the image to the three-dimensional map, determine where the image is relative to the desired slice, and indicate to the person doing the image to move the probe cranially, caudally, medially, or laterally to reach the optimal position.

[0099] In all of the above-mentioned marker element-based embodiments, external components of such systems are preferably configured to report the IVC dimensions to the patient, as well as wirelessly transmit that information to the patient's doctor or other people monitoring the patient's health. Since they are external to the body, size is less critical, and such components could have more significant batteries to allow communication with the physician or other monitors via a Bluetooth®, WiFi®, cellphone, or other communications modality as described in more detail later in this disclosure. The ultrasound receiving/transmitting element of any of these less-invasive IVC monitoring systems could be configured to be worn continuously by the patient, or it could be used for a period of minutes once or more per day. All of the external components may be contained in a single housing, or could be broken up into two or more separate units. For example, in system 3000, shown in FIG. 30, ultrasound receiver/transmitter probe 3003 may be connected either wirelessly or by cable to console 3006 adapted to provide user control functions, perform calculations, store and display information, and communicate with cell phones or the Internet via wireless networks. Console 3006 may include a CPU, memory device, and other components for input, communication and storage as described in further detail below in connection with FIG. 46. In this way, a transmitter/receiver probe may be compact, lightweight and wearable (as in FIG. 33), while the control console could be a larger tabletop unit.

Injectable and other Passive Marker Embodiments

[00100] Embodiments discussed above primarily encompass active marker element-based embodiments and more passive marker elements that may be fastened to the IVC wall by various embodiments of anchor elements or other similar suitable means. In further alternative embodiments, as described herein below, marker elements are placed or injected into or within the IVC wall. In some clinical situations, instead of a marker element that is fastened to the inner or outer wall of the IVC, such placement may be easier or preferable.

[00101] In one such injectable-type embodiment, as shown in FIGS. 34A and 34B, a relatively small guiding catheter 3403 may be introduced into the IVC, and through that catheter a needle or blade 3406 may be introduced. Under ultrasound or fluoroscopic guidance, needle 3406 may be directed towards the appropriate wall of the IVC, and inserted into the wall.

Needle/blade/catheter 3406 may have a shoulder or hilt a selected distance from its distal tip to engage the wall surface so as to limit the depth of penetration of the needle or blade. The needle or blade 3406 may be configured to create a pocket or flap in the IVC wall into which biocompatible or resorbable substance 3409 containing marker elements 3412 may be placed or injected. System 3400 may be further configured to deliver marker elements 3412 into the middle of the IVC wall, such as between the medial and adventitial layers of the IVC, or between the intimal and medial layers. System 3400 may also be configured to deliver marker elements 3412 through the thickness of the IVC wall to the exterior so that marker elements 3412 would adhere against the outer surface of the IVC as shown, for example, in FIG. 34B.

[00102] Injectable marker elements may be, for example, a flexible wire, ribbon, or guidewire segment, which could be advanced easily through a catheter or needle into or against the IVC wall. Such a marker element could be attached to a delivery wire or catheter, and removed or repositioned as needed. The marker element would only be detached from the delivery system once appropriate positioning had been confirmed. System 3500, shown in FIG. 35, uses coiled wire marker element 3503, which is deployed using delivery catheter 3506. Delivery catheter 3506 holds marker element 3503 with two jaws 3509 until the marker element reaches the distal end of the delivery catheter 3506, at which point the jaws separate to release the marker element. Marker element 3503 also may be released via a threaded connection, an interlocking mechanism, an electrolytic or other soluble connection, or other such release mechanisms as are known in the art.

[00103] Examples of embodiments of guidewire segments for use in such injectable marker element embodiments are shown in FIGS. 36A-E. Such segments may have a surface texture optimized to reflect the ultrasound or other signal and may be metallic, such as platinum, titanium, gold, or other material, or it may be a polymer. A polymer embodiment may be molded with appropriate echo-reflective surfaces and radiopaque markings. Alternatively, such a guidewire marker element may comprise a section of hollow wire, sealed on each end and filled with air or echo-reflective fluid. A wire or ribbon may include barbs, scales, or other features to inhibit it from backing out of the IVC wall or migrating completely through the IVC wall. FIG. 36A shows a simple guidewire coil 3603. FIG. 36B shows a guidewire coil 3606 coated with polymer 3607 to permanently entrap air creating a highly echo-reflective marker. FIG. 36C

shows a close-up of a coiled ribbon marker element 3609 with surface texture 3612 to enhance its echo-reflectivity. FIG. 36D shows marker element 3615 formed as a sealed tube of air. FIG. 36E shows marker element 3618, formed as a tube of cast polymer such as silicone which has been emulsified prior to curing, entrapping many tiny echo-reflective gas bubbles 3621. Gas bubbles 3621 can be of a particular gas to minimize any absorption through the walls of the polymer over time. Tubular or coil devices delivered through a catheter may be provided with a selectively releasable retention mechanism such that placement may first be confirmed before the device is released from the catheter. One such mechanism is illustrated in FIG. 36E, which includes threaded connector 3624 at one end, configured to cooperate with a threaded release mechanism in the delivery catheter. Once appropriate positioning has been confirmed, the delivery catheter may be unscrewed, leaving the polymer tube permanently in place.

[00104] Alternatively, injectable marker elements may comprise a number of small echo-reflective beads or particles, as shown in FIGS. 37A-C, which may be injected into the wall of the IVC or into the peri-adventitial space against the outside of the IVC. Such injectable marker particles may comprise spheres of gas similar to commonly used air bubbles for temporary ultrasound imaging, except they would be encased in surrounding shells of a permanent or semi-permanent material such as silicone or other polymers. These bubbles form spherical reflectors for ultrasound signals. The injectable marker particles may alternatively be shaped with pyramidal indentations with 90 degree angles which will reflect signals very effectively, similar to radar reflectors used on sailboats. Injectable marker particles may be metallic, such as titanium, or they could be a polymer such as PEEK (polyetheretherketone).

[00105] FIG. 37A shows injectable marker particles 3703 with random jagged echo-reflective shapes. FIG. 37B shows hollow spherical injectable particles 3706. FIG. 37C shows alternative injectable marker particles 3709 with molded or shaped configurations having echo-reflective indentations 3712. Such injectable marker particles may be of any size from a few microns, to hundreds of microns, or the maximum size which will pass through the delivery catheter. The size might be particularly selected to maximize the reflection of signals of specific frequencies. Nanoparticle-based technologies also may be employed to provide such particles.

[00106] During delivery, injectable marker particles as described above may be suspended in a fluid such as saline, or a gel such as certain formulations of polyethylene glycol (PEG). PEG is already used in vessel walls for vascular closure applications, such as the MYNXtm device from Access Closure. Depending upon their formulation, materials such as PEG can be resorbed over the course of weeks or months, leaving the marker particles permanently in place. Alternatively, a permanent polymer could be injected which can be injected as a liquid, but then hardens in place. This polymer may have marker particles suspended within it, or the polymer itself could be the marker. One example of a biocompatible polymer which could be used for this is urethane methacrylate. FIG. 38 shows a close-up of a urethane methacrylate gel 3803 mixed with marker particles 3806 injected into the wall W of the IVC.

[00107] Another alternative embodiment may comprise securing or sticking marker particles 3903 to the inner walls of the IVC with a material 3906 or texture that encourages the marker elements to grow into the IVC wall as shown, for example in FIGS. 39A and 39B. Fibrin is one example of a biocompatible material that is known to adhere to blood vessel walls, and to endothelialize in place. Other biocompatible, bioabsorbable adhesives could be used. Marker particles 3903 may be mixed into a fibrin patch and placed as desired in or against the IVC wall. After the patch is endothelialized and the fibrin absorbed, the marker particles remain in the vessel wall. FIG. 39A shows a cross-sectional view of patch 3906, containing marker particles 3903, which has endothelialized into the vessel wall, but patch 3906 itself has not yet been resorbed. Alternatively, a marker patch could be designed with a “Velcro-like” texture of microneedles or microhooks 3909 as shown in FIG. 39B, which embed into the IVC wall and may remain in place permanently.

[00108] Marker elements 4003 designed to be applied to an inner surface of the IVC wall may be delivered to the IVC wall by mounting them on the outside of an inflatable balloon 4006, introducing that balloon into the IVC, and inflating it to press the marker elements against the IVC wall as shown in FIG. 40A. Marker elements 4003 may be relatively long and slender, to minimize the overall diameter of the combined marker elements and delivery system. Various marker elements described herein for adherence to or embedding in the IVC wall may be applied using this technique, such as, e.g., as shown in FIG. 39A or 39B. Before or during delivery, it will be important to confirm that marker elements 4003 are aligned with the anterior and

posterior walls of the IVC, which may be accomplished, for example, by using radiopaque markers and fluoroscopy. Delivery balloon 4006 may have wings 4009 to cover marker elements 4003 during delivery, but which unfold or retract to expose the marker elements as the balloon is inflated. Alternatively, a cover sheath may be provided over the markers to hold them in place on the balloon during introduction. This cover sheath would then be withdrawn shortly before expansion of the balloon to deploy the markers. In a further alternative, two-balloon catheter 4012 may be used as shown in FIG. 40B, to permit blood flow through space 4015 so that blood flow would not be interrupted during the delivery process.

[00109] Sensing and position/measurement detection using injectable-type marker elements as described in the embodiments above may be accomplished by a variety of means or systems. For example, injectable marker elements may be designed to reflect ultrasound energy. Since the ultrasound signal is being used to measure distance rather than imaging, the signal may be provided at a relatively low power. Since the IVC is located deep in the abdomen, and higher-frequency signals attenuate rapidly in human tissue, it may be preferable to use a relatively low frequency, perhaps in the range of 200KHz-2MHz, although the frequency might be higher or lower in practice. The anterior-posterior dimension of the IVC could be measured simply by measuring the additional time it takes the signal to reflect off the posterior marker element and return to the system monitor, compared to the time it takes to reflect off the anterior marker element. Since the speed of sound in human soft tissue is approximately 1540 meters/second, if the A-P dimension of the IVC is approximately 20mm in an average human patient, the posterior reflection will return to the monitor approximately 26 microseconds after the anterior reflection. Each additional millimeter of dimension will add approximately 1.3 microseconds to the differential.

[00110] It should be noted that one important measurement may be the percentage variation in that anterior-posterior dimension. Even if the absolute dimensional measurement is not accurate, the percentage variation should still be accurate. For example, if the monitor is 15 degrees to one side of the anterior-posterior alignment of the marker elements, the maximum measured absolute A-P dimension may be reduced by [one minus the cosine of 15 degrees], or 3.4%. But the minimum measured A-P dimension should be similarly reduced, so the overall percentage change should be minimal. Similarly, any movement of the abdominal wall, for

instance with respiration, should not affect the differential in the time it takes for the two reflected signals to return to the system monitor.

[00111] Given the relatively low power needed for such a simple distance measurement, the monitor device may be of simple design and obtain a good signal even with a very low-power signal, which should maximize both the safety and battery life of the device. However, if more accurate distance measurements are desired, an external transmitter/ receiver can be configured to provide consistent, precise measurement of the relative distance of the two marker elements. In one exemplary embodiment, shown in FIG. 41, external handset 4103 comprises two emitter/receiver pairs 4106 mounted a fixed distance apart on handle 4109. Each emitter/receiver pair 4106 is mounted on a contact pad 4712 configured to engage the patient's skin. Each emitter transmits a signal toward the implanted IVC markers, which reflect the signals back toward the handset for reception by the receivers. In this way the distance to each IVC marker may be calculated by triangulation to obtain a very precise measurement. Optionally, the two emitters can transmit signals at different frequencies to eliminate interference.

Multi-Sensor Monitoring Systems

[00112] While pulmonary artery (PA) pressure measurement mentioned in the Background above holds some promise as an approach to heart failure monitoring, it is believed that IVC volume measurement may present a more accurate and early indication of heart failure. However, the combination of IVC volume measurement with PA pressure monitoring may provide an even more comprehensive picture of disease progression.

[00113] The systems of the present disclosure may therefore include both an IVC volume monitor along with a PA pressure monitor, and/or other sensors for measuring symptoms related to heart failure. The multiple monitors/sensors may be coupled together by either a wired or wireless connections to allow data transmission between them, or they could operate completely independently. In preferred embodiments, the IVC monitor and the PA monitor will both communicate with a single data receiver outside the patient's body. Alternatively one of the monitors could transmit data to the other, from which it could be transmitted to an external receiver. Additionally, a power supply integrated into one of the two monitors could deliver

power to the other of the monitors, or a separately implanted power supply could be connected to each monitor. The system could also include a controller/data analyzer that analyzed the data received from each monitor and used the combined data to determine the extent of or change in the patient's disease, and whether to set off an alarm or transmit a notification to the patient or health professional.

[00114] One exemplary embodiment of such a system is system 4200, shown in FIG. 42. System 4200 may include a first delivery catheter (not shown) for implanting IVC volume monitoring device 4203 in the IVC, and second delivery catheter 4206 for implanting pressure sensor 4209 in the pulmonary artery. Each of these catheters could be introduced through a single introducer 4212 positioned in a peripheral vein such as a femoral or iliac vein. Alternatively, system 4200 may utilize a single delivery catheter carrying both IVC monitor 4203 and PA pressure monitor 4209. A single catheter arrangement allows monitoring of implants to be delivered serially (either PA first or IVC first) from a single catheter in a single intervention. Other sensors that could be included in a multi-sensor system such as system 4200, to provide additional data related to heart failure include a respiratory rate monitor, cardiac rhythm monitor, arterial or venous blood pressure monitor, blood oxygen saturation sensor, or cardiac output monitor.

Closed-Loop Therapy System Embodiments

[00115] This disclosure has heretofore described various embodiments, devices and methods for using the size, relative size, and variation in size of the IVC to detect the early onset of acute decompensation in heart failure. With the information provided by these devices and methods, various actions may be taken by patients, caregivers and physicians to diagnose or treat the disease. In still further embodiments, the IVC monitoring system may be expanded to provide for closed-loop control of a number of different therapeutic interventional systems. By sensing the onset of an event of acute heart failure decompensation and then triggering an intervention that may reverse, minimize or eliminate the episode of decompensation, significant suffering or death of the patient potentially may be avoided, and the health care system will save significant financial and human resources.

[00116] It is common practice to use intravenous (IV) diuretics to increase fluid output for patients who are admitted to the hospital for acute heart failure decompensation. Many patients in heart failure take oral diuretics, but as their heart failure status deteriorates, diuretics can become less and less effective when delivered orally. Intravenous or intramuscular diuretic delivery remains more effective in these situations. The output from the sensor/monitor contemplated herein could be coupled with IV pumps, for example, to control the dosage of IV diuretics in the in-patient setting. In this example, the sensor/monitor would communicate to an external module, increasing or decreasing dosage of the IV diuretics as necessary to maintain a desired IVC status. The external communication module could be a separate module, which in turn communicates to the IV pump, or it could be incorporated into the IV pump directly. Even if the physician preferred to manually set the initial infusion rate for the drug, the feedback system here could serve as an additional safety shut-off, interrupting delivery of diuretics once the IVC status reaches the appropriate level.

[00117] Also in clinical practice or in development are wearable or fully implantable pumps that can deliver IV or subcutaneous diuretics. To date these have been open-loop or uncontrolled systems. For example, Zatarain-Nicolas et al. reported a series of patients who were implanted with simple, passive constant-flow elastomeric subcutaneous pumps to deliver furosemide (a common diuretic) over time. The sensors discussed herein could be configured to communicate

with a valved version of this type of pump to create a simple closed-loop system and to deliver subcutaneous diuretics.

[00118] Alternatively, fully implantable, refillable drug pumps, for example the Medtronic SynchroMed pump, are currently used to deliver pain medications. A fully implantable pump could be configured to communicate with the IVC sensors and deliver IV or subcutaneous diuretics. In one configuration, an implantable pump could be implanted in an infraclavicular pouch and the IVC sensor could be introduced into the IVC from the subclavian vein adjacent to the pouch. A lead could connect the two elements of the system, so that the pump uses the data from the IVC sensor to help determine whether to infuse the drug, and how much drug to deliver. The pump could deliver the drug into the infraclavicular pouch, into nearby muscle tissue, or it could deliver the drug directly into the vascular system. If it were delivering the drug directly into the vascular system, the infusion lumen from the pump to the vascular system might be integral with the lead from the IVC sensor, or it might be introduced parallel to it. The infusion lumen might be designed with a valve at the distal tip, to minimize the incidence of clotting or clogging that might block drug delivery.

[00119] Another class of drugs commonly used to treat heart failure are inotropes. Inotropes change the force of muscular contractions. In each of the embodiments described herein, diuretics could be exchanged for, or used in conjunction with, inotropic drugs. For example, dual chamber drug pumps configured to deliver both diuretic drugs and inotropic drugs could be configured to act upon the data generated by and communicated from the sensors described herein.

[00120] In addition to directly administering diuretics to the body, drug pumps and electrical neuromodulation systems have been contemplated for the control of heart failure by directly modulating the activity of the renal nerves. The renal nerves directly influence the renin angiotensin system and modulate fluid retention or excretion. The IVC sensors herein could be configured to communicate with drug pumps or neuromodulation systems to up- or down-regulate the activity of the renal nerves, thus increasing or decreasing the actions of the renin angiotensin system.

[00121] It should be noted that the renin angiotensin system also has regulatory effects on other aspects of heart failure decompensation. Notably, the peripheral vascular system, specifically vascular tone, is involved in heart failure status. The modulatory effects of the closed-loop systems described herein may also act directly on the systems that control vascular tone, such as the renin angiotensin system.

[00122] It was described above that the IVC sensor could be configured to communicate with an external IV pump. Similarly, the sensor data can be used to control other external devices to effect a therapeutic outcome. For example, the external data collection systems described in earlier open-loop IVC sensor systems could be configured to contain as part of that external system an automatic drug injection device similar to an EpiPen. In one embodiment the external data reader can be held in contact with the body while the data from the IVC sensor is transmitted. If the data shows that an intervention is required, the external system containing one or more automatic injection systems could deploy as a result of the collected data, injecting for example subcutaneous furosemide.

[00123] FIG. 43 presents a high-level schematic of such closed-loop system embodiments, which may include an IVC monitoring device (passive or active as described above) and at least one interventional treatment device, wherein the devices are configured to communicate with one another. The IVC monitor and the therapeutic device may communicate as necessary to coordinate sensed physiologic data and required intervention in a number of ways. Any of the typically used communication protocols may be used, including but not limited to Bluetooth protocol, RF communication link, microwave communication link, ultrasound communication or the like as further described below.

[00124] In one embodiment, a direct communication can be made through the wall of the IVC proximate to, or posterior to the main body of the IVC sensor as shown in FIG. 44. This direct communication through the wall of the IVC may, for example, take the form of a mechanical grommet 4403 extending laterally from a side wall of anchor element 4406 of monitoring device 4409. Grommet 4404 is configured to pass through a penetration in the IVC wall. The grommet attachment can serve a dual purpose of helping anchor the sensor to the IVC and providing a wired communication port to the therapeutic device 4412. Grommet 4403 may

be configured to seal with the IVC wall around its periphery, either mechanically and/or via an induced healing response, and may include a flange on its outer end to seal against the exterior surface of the IVC. Alternatively, a purse-string suture can be used to seal the vessel wall around the leads. A further alternative would be to locate the IVC sensor(s) on the outside of the IVC, for example as in the embodiment shown in FIG. 28B. If the therapeutic device is also outside the vascular system, then no transmural link is necessary. Note that monitoring device 4409 utilizes marker elements 4415 connected to anchor element 4406 via anchor isolation structure 4418.

[00125] In another alternative, exemplified by the embodiment shown in FIG. 45, wired communication occurs via leads which run intravascularly to allow the IVC sensor to connect directly to the therapeutic device. For example, leads 4503 from IVC monitor 4506 can connect directly to dedicated ports 4509 of the therapeutic device 4512 (for example a pacing device such as a biventricular pacemaker). Inputs from IVC monitor 4506 can be programmed into the algorithm of the therapeutic device. For example, the inputs can be programmed into the biventricular pacing algorithm of a biventricular pacemaker to fine tune the coordination of the pacing of the heart. Since biventricular pacers are typically placed in an infraclavicular pouch with pacing leads 4515 introduced into the subclavian vein and advanced into the heart, the IVC monitor(s) could also be introduced into the subclavian vein on a delivery catheter and advanced into the IVC using techniques described above. This example could be incorporated to modulate the action of any of the therapeutic devices described below.

[00126] As an alternative to working directly with the therapeutic device by feeding the IVC sensor data into the device to modify a treatment algorithm, a separate lead (or a wireless signal) emanating from the sensor to modify the actions of a therapeutic device may be used. For example, the leads emanating from an IVC sensor could be placed in a position in which the signal from the sensor device can interact with the signal of a therapeutic device such that the signal from the sensor modifies the action of the therapeutic device. More specifically, a lead from a sensor can be placed in proximity to a lead from a pacing device such that a signal from the sensor causes a signal to emit from the sensor leads to interfere with or to augment the signal from the therapeutic device.

[00127] Embodiments of the interference mode of action described above may include placing a lead from the sensor alongside a lead from a pacemaker or biventricular pacemaker such that the signal from the sensor cancels out the signal from the pacer, or conversely augments the signal from the pacer to modify or modulate the therapy delivered. This example could be incorporated to modulate the action of any of the therapeutic devices described below. The integration of sensor data into a closed-loop system may be accomplished with many different therapeutic devices and methods currently marketed or in development for the treatment of heart failure and its associated comorbidities.

Closed-Loop Systems With Spinal Cord Stimulation

[00128] Spinal Cord Stimulation (SCS) has been tested to treat heart failure by modulating the balance of sympathetic and parasympathetic activity in the body. This typically involves the surgical implantation of an implantable pulse generator (IPG) or neurostimulator, with electrodes which are placed near the spinal cord to deliver a series of low-energy electrical impulses. The IPG is typically implanted in the abdomen near the spine.

[00129] It may be appropriate to adjust the delivery, frequency, or intensity of these electrical impulses to match the severity of the patient's heart failure status. Therefore, it may be appropriate to link the IVC monitor and the SCS into a closed-loop system. Since the IPG is very close to the IVC near the posterior wall of the abdomen, it may be appropriate to surgically implant sensors in the IVC which are connected via leads directly to the IPG. Alternatively, wireless markers could be implanted in the IVC and the IPG could wirelessly sense the distance of the markers to determine the volume status of the patient, similar to the previously described external monitoring device.

[00130] The healthcare provider could then program this closed-loop system based on an algorithm which might have the SCS impulses turned down or completely off when the patient's status is relatively healthy, with increasing intensity of SCS impulses if the patient's condition deteriorated. This system could also integrate additional physiologic information such as heart rate, respiration rate, physical activity, etc. into its calculations. It could also wirelessly communicate with external devices, which communicate the patient's and system's status to the patient, a physician, or other caregiver.

[00131] One exemplary application of this device would be to monitor the heart failure status of patients with chronic heart failure. It may very sensitively measure a patient's trend toward fluid overload, and may do so well in advance of an episode of acute decompensated heart failure. This would give the patient, physician, nurse, or other caregiver time to adjust fluid intake, increase diuretic medications or take other steps to reduce the patient's fluid status. The external module might include an alarm which tells the patient to get out of bed and sleep more upright or to go directly to the hospital, if the perceived risk of fluid overload is extremely high.

[00132] Another exemplary application of disclosed devices is to manage a patient during an episode of hospitalization for acute decompensated heart failure. Even though a patient may spend several days in the hospital receiving intravenous diuretics, reduced fluid intake, and even aquapheresis (dialysis to reduce fluid volume), it is quite possible that the patient leaves the hospital with excess fluid. In these situations, embodiments described may be usefully applied to titrate the diuresis process and to assess when the patient should be discharged. Further, as this new parameter of IVC distention and variability is studied more extensively based on the teachings of the present disclosure, it may prove to be an important prognostic indicator for a number of other conditions and situations other than management of heart failure, dialysis, and patients in shock.

[00133] As noted in connection with various embodiments described herein, one or more aspects and embodiments may be conveniently implemented using one or more machines (*e.g.*, one or more computing devices that are utilized as a user computing device for electronic medical information or documents, one or more server devices, etc.) programmed according to the teachings of the present disclosure, as will be apparent to those of ordinary skill in the art.

[00134] This device may have electronic circuitry that stores data which may then be communicated to an outside monitor via a telemetry system. This information could then be further processed for presentation to the patient, giving a simple indication of their risk level or recommended level of drug intake, or diet and activity recommendations. This information could also be forwarded to the patient's physician, so that they can monitor the patient's condition and communicate with the patient as appropriate.

[00135] This information could also be forwarded via the internet or other means to the company which manufactures or sells the device, so that the company can continue to optimize the algorithms which use the raw data to determine the patient's risk level. It may be most effective to have the external monitor forward all of the raw data to the company, since the company will have the most up-to-date and optimized algorithms for analyzing data, and then send the processed information back to the patient and their physician. The company might also have the most secure data storage means for storing all historical information for each specific patient, so that the data analysis algorithm can be further optimized for each specific patient.

[00136] Embodiments disclosed herein may also be used for measuring dimensions of other body elements besides the IVC. Sensors could be placed in the heart, for example placing them in the left ventricle via catheter-based delivery. They could also be placed on the surface of the heart, within the pericardium via a subxyphoid access. These sensors could be used to directly monitor the heart's activity. As another example, sensors could be placed on or in the bladder to monitor bladder conditions. In patients who need to self-catheterize to drain their bladders, it may be useful to have an automated warning of when the bladder was full.

[00137] For all of the above-mentioned embodiments that have markers or sensors implanted into the IVC, these markers or sensors may heal into the IVC wall over time. Therefore, the stent, anchor, or other elements that hold the markers in place may not need to be permanent. Therefore, it may be desirable to make the stent or anchor bioerodable, so that after a period of time, there is no longer a stent in the IVC. The specific duration of the anchoring elements can be varied from weeks to years through material selection, formulation, and processing. This would eliminate a foreign body, and it would also render the IVC more flexible, allowing it to more naturally collapse or expand. Other bioabsorbable vascular elements have already been made from materials such as Poly-L-Lactide. These materials have less springiness than Nitinol, so the stent design may need to be modified. For example, the stent could be made with circumferential elements that ratchet open to apply pressure to the IVC to hold the stent in place. The delivery catheter for this bioabsorbable stent might include a balloon to actively expand the stent against the IVC.

[00138] Embodiments described in this disclosure so far have focused primarily on volume changes in the IVC. As the patient inhales, thoracic pressure drops slightly, increasing the flow of blood from the IVC into the right atrium (RA). As the patient exhales, thoracic pressure increases slightly, decreasing the flow of blood into the right atrium. This leads to a variation in blood volume in the IVC over the respiratory cycle. This variation in blood volume is necessarily correlated with a slight variation in the relative pressure between the IVC and the RA. As an alternative or adjunct to IVC volume measurement, a measurement of the relative variation in fluid pressure between the IVC and right atrium may provide a useful indication of blood volume. An implant with two pressure sensors arrayed along a single lead could be implanted from the femoral vein, jugular vein, or subclavian vein and anchored in position so that one pressure sensor is in the RA and one in the IVC. Embodiments described above having different configurations for IVC monitors (wireless, externally powered, powered by electronics deployed within the IVC or RA, powered from an infraclavicular implant, *etc.*) may alternatively or additionally employ such a measurement of relative variation in fluid pressure.

System and, Control and Communication Hardware and Software Aspects of Disclosed Embodiments

[00139] Appropriate software coding can readily be prepared by skilled programmers based on the teachings of the present disclosure, as will be apparent to those of ordinary skill in the software arts. Aspects and implementations discussed above employing software and/or software modules may also include appropriate hardware for assisting in the implementation of the machine executable instructions of the software and/or software module.

[00140] Such software may be a computer program product that employs a machine-readable storage medium. A machine-readable storage medium may be any medium that is capable of storing and/or encoding a sequence of instructions for execution by a machine (*e.g.*, a computing device) and that causes the machine to perform any one of the methodologies and/or embodiments described herein. Examples of a machine-readable storage medium include, but are not limited to, a magnetic disk, an optical disc (*e.g.*, CD, CD-R, DVD, DVD-R, *etc.*), a magneto-optical disk, a read-only memory “ROM” device, a random access memory “RAM” device, a magnetic card, an optical card, a solid-state memory device, an EPROM, an EEPROM,

and any combinations thereof. A machine-readable medium, as used herein, is intended to include a single medium as well as a collection of physically separate media, such as, for example, a collection of compact discs or one or more hard disk drives in combination with a computer memory. As used herein, a machine-readable storage medium does not include transitory forms of signal transmission.

[00141] Such software may also include information (*e.g.*, data) carried as a data signal on a data carrier, such as a carrier wave. For example, machine-executable information may be included as a data-carrying signal embodied in a data carrier in which the signal encodes a sequence of instruction, or portion thereof, for execution by a machine (*e.g.*, a computing device) and any related information (*e.g.*, data structures and data) that causes the machine to perform any one of the methodologies and/or embodiments described herein.

[00142] Examples of a computing device include, but are not limited to, an electronic book reading device, a computer workstation, a terminal computer, a server computer, a handheld device (*e.g.*, a tablet computer, a smartphone, etc.), a web appliance, a network router, a network switch, a network bridge, any machine capable of executing a sequence of instructions that specify an action to be taken by that machine, and any combinations thereof. In one example, a computing device may include and/or be included in a kiosk.

[00143] FIG. 46 shows a diagrammatic representation of one embodiment of a computing device in the exemplary form of a computer system 4600 within which a set of instructions for causing a control system to perform any one or more of the aspects and/or methodologies of the present disclosure may be executed, such as a control system that may be embodied by or implemented in accordance with one or more components of: any one or more of the IVC sensors and/or monitors and/or associated components disclosed herein; electronics capsule 118 of FIG. 1; electronics capsule 503 of FIG. 5; electronics capsule 1124 of FIG. 11; electronics capsule 1701 of FIG. 17; electronics capsule 1801 of FIG. 18; electronics capsule 2306 of FIG. 23; electronics capsule 2512 of FIG. 25; electronics capsule 2806 of FIG. 28A-C; console 3006 and/or ultrasound receiver/transmitter probe 3003 of FIG. 30; wearable detection system 3300 and/or external device 3318 of FIG. 33; external handset 4103 of FIG. 41; system 4200 of FIG. 42; one or more components of the systems of FIGS. 43 and/or 44; and/or

IVC monitor 4506 of FIG. 45, among others. It is also contemplated that multiple computing devices may be utilized to implement a specially configured set of instructions for causing one or more of the devices to perform any one or more of the aspects and/or methodologies of the present disclosure. Computer system 4600 includes a processor 4604 and a memory 4608 that communicate with each other, and with other components, via a bus 4612. Bus 4612 may include any of several types of bus structures including, but not limited to, a memory bus, a memory controller, a peripheral bus, a local bus, and any combinations thereof, using any of a variety of bus architectures.

[00144] Memory 4608 may include various components (*e.g.*, machine-readable media) including, but not limited to, a random access memory component, a read only component, and any combinations thereof. In one example, a basic input/output system 4616 (BIOS), including basic routines that help to transfer information between elements within computer system 4600, such as during start-up, may be stored in memory 4608. Memory 4608 may also include (*e.g.*, stored on one or more machine-readable media) instructions (*e.g.*, software) 4620 embodying any one or more of the aspects and/or methodologies of the present disclosure. In another example, memory 4608 may further include any number of program modules including, but not limited to, an operating system, one or more application programs, other program modules, program data, and any combinations thereof.

[00145] Computer system 4600 may also include a storage device 4624. Examples of a storage device (*e.g.*, storage device 4624) include, but are not limited to, a hard disk drive, a magnetic disk drive, an optical disc drive in combination with an optical medium, a solid-state memory device, and any combinations thereof. Storage device 4624 may be connected to bus 4612 by an appropriate interface (not shown). Example interfaces include, but are not limited to, SCSI, advanced technology attachment (ATA), serial ATA, universal serial bus (USB), IEEE 1394 (FIREWIRE), and any combinations thereof. In one example, storage device 4624 (or one or more components thereof) may be removably interfaced with computer system 4600 (*e.g.*, via an external port connector (not shown)). Particularly, storage device 4624 and an associated machine-readable medium 4628 may provide nonvolatile and/or volatile storage of machine-readable instructions, data structures, program modules, and/or other data for computer system 4600. In one example, software 4620 may reside, completely or partially,

within machine-readable medium 4628. In another example, software 4620 may reside, completely or partially, within processor 4604.

[00146] Computer system 4600 may also include an input device 4632. In one example, a user of computer system 4600 may enter commands and/or other information into computer system 4600 via input device 4632. Examples of an input device 4632 include, but are not limited to, an alpha-numeric input device (*e.g.*, a keyboard), a pointing device, a joystick, a gamepad, an audio input device (*e.g.*, a microphone, a voice response system, etc.), a cursor control device (*e.g.*, a mouse), a touchpad, an optical scanner, a video capture device (*e.g.*, a still camera, a video camera), a touchscreen, and any combinations thereof. Input device 4632 may be interfaced to bus 4612 via any of a variety of interfaces (not shown) including, but not limited to, a serial interface, a parallel interface, a game port, a USB interface, a FIREWIRE interface, a direct interface to bus 4612, and any combinations thereof. Input device 4632 may include a touch screen interface that may be a part of or separate from display 4636, discussed further below. Input device 4632 may be utilized as a user selection device for selecting one or more graphical representations in a graphical interface as described above.

[00147] A user may also input commands and/or other information to computer system 4600 via storage device 4624 (*e.g.*, a removable disk drive, a flash drive, etc.) and/or network interface device 4640. A network interface device, such as network interface device 4640, may be utilized for connecting computer system 4600 to one or more of a variety of networks, such as network 4644, and one or more remote devices 4648 connected thereto. Examples of a network interface device include, but are not limited to, a network interface card (*e.g.*, a mobile network interface card, a LAN card), a modem, and any combination thereof. Examples of a network include, but are not limited to, a wide area network (*e.g.*, the Internet, an enterprise network), a local area network (*e.g.*, a network associated with an office, a building, a campus or other relatively small geographic space), a telephone network, a data network associated with a telephone/voice provider (*e.g.*, a mobile communications provider data and/or voice network), a direct connection between two computing devices, and any combinations thereof. A network, such as network 4644, may employ a wired and/or a wireless mode of communication. In general, any network topology may be used. Information (*e.g.*, data, software 4620, etc.) may be communicated to and/or from computer system 4600 via network interface device 4640. In

some embodiments, one or more cloud computing services, “software as a service” services, “storage as a service” services, and/or distributed networks or components, among others, may be used to receive, store, and/or provide data and/or execute software in accordance with aspects of the present disclosure, as will be understood by those of ordinary skill in the relevant art after reading this disclosure in its entirety.

[00148] Computer system 4600 may further include a video display adapter 4652 for communicating a displayable image to a display device, such as display device 4636. Examples of a display device include, but are not limited to, a liquid crystal display (LCD), a cathode ray tube (CRT), a plasma display, a light emitting diode (LED) display, and any combinations thereof. Display adapter 4652 and display device 4636 may be utilized in combination with processor 4604 to provide graphical representations of aspects of the present disclosure. In addition to a display device, computer system 4600 may include one or more other peripheral output devices including, but not limited to, an audio speaker, a printer, and any combinations thereof. Such peripheral output devices may be connected to bus 4612 via a peripheral interface 4656. Examples of a peripheral interface include, but are not limited to, a serial port, a USB connection, a FIREWIRE connection, a parallel connection, and any combinations thereof.

[00149] Device embodiments disclosed herein also may measure other physiologic data, and integrate that data in its reporting and analysis. It might be used at different times to treat different conditions. For example, the IVC diameter and its variation will be significantly different while the patient is standing in comparison to when the patient is sitting, prone, or supine. Therefore, the IVC monitor can also be used to track patient activity. Also, electrodes can be placed on the IVC element itself and/or on the leads leading to the device, in order to monitor, record, and communicate the heart’s electrical activity.

[00150] Although a primary indication described for embodiments disclosed herein is the management of heart failure, embodiments and information collected thereby may be used for management of other conditions as well. For example, it could also be simultaneously used to manage blood volume in patients undergoing dialysis, providing direct feedback to dialysis machines to modulate total fluid volume delivered or removed. It could similarly be used to

communicate with IV pumps to manage re-hydration for patients who have acute episodes of shock.

[00151] As described above, embodiments may be connected to a drug pump or stimulator to modulate the renal nerves, due to the multiple indirect effects the renal nerves have on heart failure. If a device of such embodiments is also monitoring heart rhythm status as well and detected an episode of atrial fibrillation, it could be programmed to modulate the renal nerves in that situation as well. Afferent renal nerves are known to increase systemic sympathetic tone, and increased systemic sympathetic tone increases the risk of atrial fibrillation, so temporary denervation of the renal nerves might cause the episode of atrial fibrillation to terminate.

Use of IVC volume measurement in dialysis patients

[00152] Volume management in dialysis patients can be particularly challenging, since the kidneys are not providing normal volume homeostasis. Dialysis patients typically increase their fluid volume between dialysis sessions. Since the kidneys are not making urine, excess volume needs to be removed during dialysis, along with the other waste products which dialysis filters out. However, most of the excess volume is in the cells and interstitial volume, not in the circulatory system. It takes time, typically more than an hour, for that volume to re-enter the circulatory system as other fluid is removed from the blood. The excess volume should not be removed too quickly, as that would lead to excessive hemoconcentration and potentially dangerously low blood pressure. Excessive hemoconcentration can cause myocardial stunning and other significant dangers. Moreover, it may be difficult and impractical for the care provider managing the dialysis process to track the patient's blood volume continuously during the dialysis session. Therefore, excess fluid is typically removed very gradually over the course of a dialysis session. This reduces the rate at which intracellular and extracellular fluid returns to the vascular system, and makes the overall dialysis session less efficient. An efficient and effective method to measure circulating blood volume real-time during dialysis is needed.

[00153] Secondly, it is important to remove as much volume as is safely possible over the course of the complete dialysis session. As mentioned, fluid volume builds up in patients between dialysis sessions. This leads to many potential clinical issues, including high blood pressure, fluid in the lungs, fibrosis, and heart failure. If the patients leave each dialysis session

with a minimum of fluid in their systems, that increases the chances that they will not be overloaded with fluid by the time they return for their next session. However, determining whether the patient is euvolemic (has the right fluid volume) or is hyper- or hypo-volemic is challenging with current techniques. An effective method to measure final blood volume in dialysis patients at the end of dialysis sessions is therefore also an important need.

[00154] At present, blood concentration during dialysis is often measured using devices such as Fresenius' Critline or Intelomedics' CVinsight. These systems measure the patient's hematocrit and blood oxygenation to calculate the fluid volume removed from the patient. Assessing euvolemia at the end of dialysis may be done using 'BioImpedance measurement', which gives an indication of extracellular and intracellular fluid volume in the patient. These measurements are imperfect, but are the best available at this time.

[00155] Measurement of a dialysis patient's volume status using ultrasound imaging of the IVC has been studied. It gives an important physiologic reading of the patient's volume status, one which relates directly to whether the patient is truly euvolemic. However, it is user-dependent, technology-sensitive, and difficult. It also gives only a single-point measurement, and is completely impractical as a method of continuously measuring volume status.

[00156] For all of these reasons, IVC volume measurement systems embodied in the present disclosure provide an improved method of managing the dialysis patient's volume status. Described systems provide for continuous monitoring and give a true measurement of whether the patient is hyper-, hypo-, or euvolemic, and can be used to guide therapy. The IVC markers described herein, when implanted on or in the IVC wall, allow a patient's fluid volume to be monitored before, during or after a dialysis session. Because dialysis is typically conducted in a specialized facility staffed by healthcare providers, readings could be taken by trained professionals to ensure accuracy. In addition, with the patient being immobile in a chair or bed during dialysis, an ultrasound probe may be attached to the patient's skin to provide continuous monitoring of the IVC markers during the dialysis session. The IVC volume monitor may be connected directly to the dialysis machine, for closed-loop volume management. For example, an appropriate minimum blood volume may be established by the healthcare provider; for example, as an average 40% variation in IVC dimension over the respiratory cycle. The dialysis machine

could then be programmed to reduce the blood volume at a measured, but relatively rapid pace until that volume is reached, and then to maintain that volume over the rest of the dialysis session. This approach would maximize the intracellular and extracellular fluid that is removed from the patient, while preventing the patient from risk of myocardial stunning, lightheadedness, or the other dangers of hypovolemia. It may be possible to shorten the dialysis session slightly as a result. At the end of the dialysis session, the IVC monitor would reconfirm that the patient was appropriately euvolemic before ending the session.

[00157] All of this discussion of volume management in dialysis patients applies equally to the management of heart failure patients who are having volume removed using an aquapheresis system such as the CHF Solutions Aquadex, or when using aggressive diuretics. It is desirable to remove the excess volume as quickly as possible, but also to allow time for the excess volume in tissue to gradually return to the bloodstream, so that overall blood volume does not drop too low, nor the blood become too concentrated.

Measurement of volume status in other vessels besides the IVC

[00158] The discussion of the various alternative embodiments above is generally made in the context of measurement of volume in the IVC. However, these embodiments also apply to and may be used for similar measurements in the superior vena cava (SVC), right atrium, or other vessels. The variation in IVC volume over the respiratory cycle has been well documented in studies using ultrasound imaging. The mild valsalva effect of respiration causes a slight variation in thoracic pressure, which modulates the flow of blood from the IVC (in the abdomen) into the right atrium (in the thorax). Therefore, this variation may be more pronounced in the IVC than in other vessels. IVC variation may also be more sensitive to variations in right atrial pressure, which may vary less in patients with marked volume overload causing tricuspid regurgitation or reduced right ventricular filling volume. However, very sensitive measurement systems might measure similar variations in vessels that are more accessible for the placement of markers and/or for placement of a measurement device. The subclavian veins, jugular veins, and femoral veins, among others, are all potential vessels for measurement of volume and volume variation that could provide similar information about a patient's blood volume and/or heart failure status. However, the teachings of this disclosure are not so limited and may be applied by

persons of ordinary skill to any vein in the body, using the sensitive measurement techniques described herein. Further features, considerations and embodiments are described below, which may be incorporated singly or multiply into one or more embodiments described above. For example, discussed above is the use of the sensor/monitor input to modify the action of cardiac pacemakers to better control the heart and circulatory system. Another embodiment or method of treating heart failure, and more specifically the fluid overload associated with heart failure, is through chemical, neural, hormonal, or electrical manipulation of the renin-angiotensin system and the degree to which the kidneys excrete or retain water.

[00159] Exemplary embodiments have been disclosed above and illustrated in the accompanying drawings. It will be understood by those skilled in the art that various changes, omissions and additions may be made to that which is specifically disclosed herein without departing from the spirit and scope of the present disclosure.

1. An implantable device for monitoring vascular lumen diameter, comprising:
 - means for detecting lumen diameter at a monitoring location;
 - an anchor element configured to securely anchor the device to the vascular lumen at an anchoring location with the detecting means positioned at the monitoring location;
 - and
 - an anchor isolation structure extending between the detecting means and anchor element, the anchor isolation structure having a shape and length specifically configured to substantially isolate the detecting means at the sensing location from distortions of the vessel caused by the anchoring element at the anchoring location.
2. The implantable device of claim 1, wherein:
 - said detecting means comprises an active marker element coupled to an end of said anchor isolation structure opposite the anchor element;
 - the anchor element comprises a resilient member moveable between a first, collapsed configuration and a second, deployed configuration, wherein the first collapsed configuration has an overall diameter sufficiently less than the vascular lumen diameter to permit deployment of the device through the vasculature, and the second expanded deployed condition has an overall diameter sufficient to securely engage the vessel lumen at the anchoring location; and
 - the anchor isolation structure comprises a member having sufficient stiffness to maintain the active marker element substantially in contact with the lumen wall without eroding the lumen wall and with the active marker element oriented substantially in the direction of the lumen wall opposite said transducer.
3. The implantable device of claim 2, wherein the detecting means comprises an ultra sound transducer positioned on an electronics capsule further containing power control and wireless communications modules to communicate outputs from the ultrasound transducer under control of the control module.
4. The implantable device of claim 2, wherein:
 - the anchor element further comprises a deployment member moveable between the first collapsed position and the second, deployed position;

said resilient member comprises a looped anchor wire secured to the telescoping deployment member; and

the looped anchor wire in the second deployed configuration expands sufficiently to place the electronics capsule against one wall of the lumen in which it is to be positioned while in contact with a substantial portion of an internal diameter of the lumen at the anchoring location.

5. The implantable device of claim 4, wherein the telescoping deployment member comprises inner and outer members each connected to the looped anchor wire at opposite ends.
6. The implantable device of claim 5, wherein the anchor isolation member is attached to one of said inner and outer members of the telescoping deployment member.
7. The implantable device of claim 5, wherein the anchor isolation member is integrally formed with one of said inner and outer members of the telescoping deployment member.
8. The implantable device of claim 2, wherein said anchor element comprises a stent and the anchor isolation member is attached at one end of the stent.
9. The implantable device of claim 1, wherein:

said detecting means comprises an electronics capsule having an ultrasound transducer disposed at an end opposite the anchor element, the electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from the ultrasound transducer;

said anchor element comprises a looped anchor wire secured to a telescoping deployment member moveable between a first collapsed configuration and a second deployed configuration, wherein the looped wire in the second deployed configuration expands sufficiently to place the electronics capsule against one wall of the lumen while in contact with a substantial portion of an internal diameter of the lumen at the anchoring location; and

the anchor isolation structure comprises a flexible member disposed between the anchor element deployment member and the electronics capsule, wherein said anchor isolation structure has sufficient stiffness to maintain the electronics capsule against said one wall of the lumen and a length equal to approximately 1 to 4 times the undistorted diameter of the lumen at the anchor location.

10. The implantable device of claim 1, wherein said detecting means comprises at least one active marker element.
11. The implantable device of claim 10, wherein said at least one active marker element comprises a single ultrasound transducer communicating with power, wireless communication and control modules contained in a sealed electronics capsule attached to the anchor isolation structure opposite the anchor element.
12. The implantable device of claim 10, wherein said at least one active marker element comprises at least two ultrasound transducers with power, wireless communication and control modules contained in a sealed electronics capsule attached to the anchor isolation structure opposite the anchor element.
13. The implantable device of claim 10, wherein said at least one active marker element comprises at least two electrodes with power, wireless communication and control modules contained in an electronics capsule attached to the anchor isolation structure opposite the anchor element.
14. The implantable device of claim 10, wherein said at least one active marker element comprises at least two coils with power, wireless communication and control modules contained in a sealed electronics capsule attached to the anchor isolation structure opposite the anchor element.
15. The implantable device of claim 10, wherein said detecting means further comprises a lead extending from said at least one active marker element to a sensor control unit positionable remotely from said at least one active marker element.
16. The implantable device of claim 15, wherein said sensor control unit includes power, communications and control modules communicating through said lead with said at least one marker element to receive signals therefrom and to generate an output based on said signals delivered through said communications module.
17. The implantable device of claim 16, wherein said detecting means further comprises at least a second communications module configured to be positioned outside the body and to communicate with the communications module in the sensor control unit.

18. The implantable device of claim 1, wherein said detecting means comprises at least two passive marker elements.
19. The implantable device of claim 18, wherein said at least two passive marker elements comprise at least two echo-reflective members.
20. The implantable device of claim 18, wherein said at least two passive marker elements comprise at least two passive coils.
21. The implantable device of claim 1, wherein said anchor element comprises at least one looped anchor wire mounted on at least two telescoping members having a first position relative to one another corresponding to a collapsed configuration of the at least one looped anchor wire and a second position corresponding to an expanded, deployed configuration of the at least one looped anchor wire.
22. The implantable device of claim 1, wherein said anchor element comprises an expandable and collapsible stent-like structure.
23. The implantable device of claim 22, wherein said stent-like structure is self-expanding.
24. The implantable device of claim 22, wherein said stent-like structure includes an embolic filter portion.
25. The implantable device of claim 22, wherein said stent-like structure includes outer anchoring hooks configured to engage the lumen wall.
26. The implantable device of claim 1, wherein said anchor element comprises plural flexible, resilient struts with distal tips configured to engage the lumen wall extending outward the device.
27. The implantable device of claim 1, wherein said anchor isolation structure comprises a flexible elongate member.
28. The implantable device of claim 27, wherein said flexible elongate member has sufficient stiffness to maintain said detecting means against a wall of the lumen.
29. The implantable device of claim 28, wherein said flexible elongate member has a length equal to approximately one half to four times the undistorted lumen diameter at the anchoring location.

30. The implantable device of claim 1, wherein said anchor isolation comprises at least first and second flexible arms spaced apart and extending from one end of the anchor element.
31. The implantable device of claim 30, wherein each said flexible arm has shape and stiffness selected to maintain said detecting means against the lumen wall.
32. The implantable device of claim 30, wherein each said flexible are is resiliently biased to maintain said detecting means against the lumen wall.
33. The implantable device of claim 1, wherein said anchor isolation structure comprises plural flexible arms with at least two said flexible arms extending from each end of the anchor element.
34. The implantable device of claim 1, wherein said each said flexible arm has sufficient stiffness to maintain detecting means against the wall of the lumen.
35. The implantable device of claim 1, wherein detecting means means comprises at least two marker elements positioned at one end of the anchor element, each with a respective anchor isolation structure connecting to the anchor element, said markers, anchor element and anchor isolation structures being specifically configured and dimensioned together to position a first said marker element on the posterior wall of the IVC and a second said marker element on the anterior wall of the IVC in opposition to the first said marker element when the device is positioned in the IVC between the renal and hepatic veins.
36. The implantable device of claim 35 wherein the detecting means comprises two marker elements and the anchor element has a shape specifically configured and dimensioned to preferentially position the two marker elements in opposition on the anterior and posterior walls of the IVC when implanted therein.
37. The implantable device of claim 1, wherein the detecting means is configured for ingrowth into the lumen wall and the anchor isolation structure is at least partially bioerodable to separate the detecting means from the anchor element after a selected time.
38. The implantable device of claim 10, wherein said at least one marker element comprises a single ultrasound transducer.
39. The implantable device of claim 10, wherein said at least one active marker element comprises at least two ultrasound transducers Stents with sensors right on them.

40. The implantable device of claim 10, wherein said at least one active marker element comprises at least two electrodes.
41. The implantable device of claim 10, wherein said at least one active marker element comprises at least two coils.
42. A cardiac therapy system comprising the implantable monitoring device of claim 1 and further comprising:
- an implantable cardiac therapy device including an implantable housing containing at least power and control modules;
 - at least one lead connecting said detecting means with the implantable housing and modules contained therein;
 - at least one cardiac therapy delivery element; and
 - at least one lead connecting said at least one therapy delivery element to the implantable housing and modules contained therein;
- wherein said control module executes instructions for
- generating a signal with said detecting means,
 - receiving a signal responsive to the generated signal with said detecting means, the received signal being indicative of vessel diameter at the monitoring location;
 - determining vena cava diameter at the monitoring location based on said signal;
 - comparing the determined diameter to a reference diameter to determine a change in vena cava diameter,
 - evaluating heart condition based on the determined change in vena cava diameter; and
 - modulating cardiac therapy delivered by said at least one therapeutic device passed on the evaluated heart condition.
43. The cardiac therapy system of claim 42, wherein said cardiac therapy device comprises a pacemaker and said at least one cardiac therapy delivery element comprises at least one pacing lead.
44. An implantable device for monitoring vascular lumen diameter, comprising:
- an electronics capsule having an ultrasound transducer disposed at one end, the electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from

- the ultrasound transducer, the ultrasound transducer configured substantially in contact with a lumen wall and to detect lumen diameter at a monitoring location by echo reflection off an opposite lumen wall;
- a looped anchor wire secured to a telescoping deployment member moveable between a first collapsed configuration and a second deployed configuration, wherein the looped anchor wire in the second deployed configuration expands sufficiently to place the electronics capsule against one wall of the lumen while in contact with a substantial portion of an internal diameter of the lumen at an anchoring location; and
- a flexible anchor isolation member disposed between the tubular deployment member and the electronics capsule, wherein said anchor isolation structure has sufficient stiffness to maintain the electronics capsule against said one wall of the lumen, the anchor isolation member having a shape and length specifically configured to at least substantially isolate the electronics capsule from distortions of the vessel lumen caused by the anchoring looped anchor wire at the anchoring location.
45. The implantable device of claim 44, wherein the anchor isolation member length is equal to approximately 1 to 4 times the undistorted diameter of the lumen at the anchoring location.
46. A system for monitoring vascular lumen diameter, comprising:
- at least two implantable passive marker elements configured to be implanted in or through a vascular lumen wall at a monitoring location;
 - an intravascular delivery device for delivering and implanting said passive marker elements at the monitoring location; and
 - detecting means configured to be positioned outside a patient's body for sensing position and movement of the implanted passive marker elements relative to each other.
47. The system of claim 46, wherein said passive marker elements comprise echo-reflective particles.
48. The system of claim 47, wherein said echo-reflective particles comprise jagged particles.
49. The system of claim 47, wherein said echo-reflective particles comprise hollow spherical particles.
50. The system of claim 47, wherein said echo-reflective particles comprise particles shaped with

echo-reflective indentations.

51. The system of claim 50, wherein said echo-reflective particles are contained within a bioresorbable fluid or gel.
52. The system of claim 46, wherein said passive marker elements comprise strips or patches of eco-reflective material configured for tissue ingrowth on the lumen wall.
53. The system of claim 46, wherein said passive marker elements comprise flexible, echo-reflective elongate members.
54. The system of claim 53, wherein said flexible, echo-reflective elongate members comprise guide wire coil segments.
55. The system of claim 53, wherein said flexible, echo-reflective elongate members comprise guide wire coil segments coated with polymer surrounding entrapped air.
56. The system of claim 53, wherein said flexible, echo-reflective elongate members comprise coiled ribbon with eco-reflective surface textures.
57. The system of claim 53, wherein said flexible, echo-reflective elongate members comprise sealed tubes of air.
58. The system of claim 53 wherein said flexible, echo-reflective elongate members comprise tubes of cast polymer.
59. The system of claim 53, wherein said flexible, echo-reflective elongate members include attachment means for attachment to said delivery device.
60. The system of claim 46, wherein said delivery device comprises a guide catheter containing a hollow cutting element for penetrating and implanting the passive marker elements in or through the lumen wall.
61. The system of claim 60, wherein said deliver device further includes jaw member for gripping and releasing passive marker elements.
62. The system of claim 46, wherein said delivery device comprises a balloon catheter for applying passive marker elements to the lumen wall.
63. The system of claim 62, wherein said balloon catheter is a double balloon catheter with a

central passage to permit blood flow there through during passive marker deployment.

64. The system of claim 46, wherein said detecting means comprises a signal emitting/receiving probe configured to scan for said passive marker elements.

65. The system of claim 64, wherein said signal emitting receiving probe comprises an ultrasound probe.

66. The system of claim 65, wherein the ultrasound probe is configured to be secured to the patient.

67. The system of claim 66, wherein the ultra sound probe includes position means for alignment with markers provided externally on the patient.

68. An implantable device for monitoring vascular lumen diameter, comprising:

- an ultrasound transducer configured to be positioned substantially in contact with a lumen wall and to detect lumen diameter at a monitoring location by echo reflection off an opposite lumen wall;

- an, electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from the ultrasound transducer;

- an anchoring member configured to rotationally and longitudinally immobilize the implantable device at an anchoring location in the vascular lumen; and

- a flexible anchor isolation member disposed between the anchoring member and the ultrasound transducer, wherein said anchor isolation structure has a shape and stiffness selected to maintain the ultrasound transducer against said one wall of the lumen, the anchor isolation member having a shape and length specifically configured to at least substantially isolate the ultrasound transducer from distortions of the vessel lumen caused by the anchoring member at the anchoring location.

69. The implantable device of claim 68, wherein the ultrasound transducer is mounted to the electronics capsule and the electronics capsule is disposed at a distal end of the anchor isolation member opposite the anchoring member.

70. An implantable device for monitoring vascular lumen diameter, comprising:

- an ultrasound transducer configured to be positioned substantially in contact with a lumen

- wall and to detect lumen diameter at a monitoring location by echo reflection off an opposite lumen wall;
- an electronics capsule containing at least power and communications modules controlled by a control module to receive and wirelessly transmit signals based on inputs from the ultrasound transducer; and
- an anchoring member configured to rotationally and longitudinally immobilize the implantable device at an anchoring location in the vascular lumen and having a shape and stiffness selected to maintain the ultrasound transducer against said one wall of the lumen;
- wherein the electronics capsule is mounted directly to the anchor element.
71. A method of continuously monitoring a diameter of a vascular lumen with an implanted device, comprising:
- implanting at least one marker element on a wall of the lumen at a monitoring location;
 - anchoring the marker element to the lumen wall at an anchoring location, wherein said anchoring location is spaced from said monitoring location by a distance sufficient to isolate the marker element from distortions of the lumen wall due to said anchoring;
 - generating a signal in cooperation with said at least one marker element indicative of vessel diameter at the monitoring location;
 - receiving said signal; and
 - determining vessel diameter based on said signal.
72. The method of claim 71, wherein said marker element comprises a single ultrasound transducer directed at an opposite lumen wall.
73. The method of claim 72, wherein said generating and receiving a signal comprises said ultrasound transducer sending ultrasound signals at the opposite lumen wall and receiving a reflected signal therefrom.
74. The method of claim 73 wherein said generating, receiving and determining steps are executed within an electronics capsule implanted in the vascular lumen, and said method further comprises wirelessly communicating vessel diameter based on said determining to an extracorporeal receiver.
75. The method of claim 74, wherein said ultrasound transducer is provided on the electronics

capsule.

76. The method of claim of claim 75, wherein said method further comprises positioning the electronics module within the vasculature remote from the ultrasound sensor and providing communication between the ultrasound sensor and electronics module by a wired connection through the lumen.
77. The method of claim 72, wherein said at least one marker element comprises at least two passive marker elements.
78. The method of claim 77, wherein:
said generating and receiving steps comprise directing an externally generated signal at said at least two markers and detecting a reflected signal therefrom; and
said determining step comprising analyzing change in relative position of said at least two markers based on the reflected signal.
79. The method of claim 78, wherein said receiving comprises wirelessly transmitting to and receiving said signals at an external analysis system.
80. The method of claim 77, wherein said at least two passive markers comprise echo-reflective markers and said signal comprises an ultrasound signal.
81. The method of claim 71, wherein said at least one marker element is active marker element.
82. The method of claim 81 wherein said at least one active marker element comprises an ultrasound transducer.
83. The method of claim 82, wherein generating and receiving the signal comprises sending an ultrasound signal and receiving a reflected signal.
84. The method of claim 81, wherein said at least one active marker element comprises at least two inductance coils.
85. The method of claim 84, wherein:
said generating and receiving comprises providing a current in one said coil and receiving an induced current in an opposite coil; and
said determining comprises determining the distance between the inductance coils based on measurement of current induced in the opposite coil.

86. The method of claim 81, wherein said at least one active marker element comprises at least two electrodes.

87. The method of claim 86, wherein:

said generating and receiving comprises delivering a current at one electrode and receiving the current at an opposite electrode; and

said determining comprises calculating changes in distance between said electrodes based on measured changes in impedance between the electrodes.

88. A method of treating a cardiac condition in a patient, comprising

implanting a monitoring device in a vena cava wall such that at least one active marker element of the monitoring device is positioned against the wall at a monitoring location;

anchoring the monitoring device to the vena cava wall at an anchoring location, wherein said anchoring location is spaced from said monitoring location by a distance sufficient to isolate the at least one active marker element from distortions of the lumen wall due to said anchoring;

implanting at least one therapeutic device configured to deliver a cardiac therapy;

generating a signal with said at least one active marker element indicative of vessel diameter at the monitoring location;

receiving said signal;

determining vena cava diameter at the monitoring location based on said signal;

comparing the determined diameter to a reference diameter to determine a change in vena cava diameter,

evaluating heart condition based on the determined change in vena cava diameter; and

modulating cardiac therapy delivered by said at least one therapeutic device passed on the evaluated heart condition.

89. The method of claim 88, wherein said at least one active marker element is supported by on an intravascular device including an electronics capsule containing power, communications and control modules and said generating, receiving, determining comparing evaluating and modulating steps are executed by said intravascular device in communication with said at least one therapeutic device without extracorporeal intervention.

90. A method of monitoring a cardiac condition of a patient, comprising:
implanting an intravascular device in a vena cava with an anchor element at an anchoring location, the intravascular device further having a pair of markers or sensors, the pair of markers or sensors being positioned in engagement with opposing walls of the vena cava at a monitoring location;
receiving a signal from the pair of markers or sensors; and
determining a diameter of the vena cava based on the signal;
wherein said implanting comprises positioning the anchor element at the anchoring location sufficiently distant from the monitoring location such that diameter determinations based on said signal are not substantially affected by distortion of the vena cava wall by the anchor element at the anchor location.
91. The method of claim 90, wherein the signal is delivered from outside the body and reflected by the pair of markers or sensors.
92. The method of claim 90, wherein the signal generated by the intravascular device.
93. The method of claim 90, further comprising:
comparing the determined diameter to a reference diameter to determine a change in the diameter, and
evaluating the heart condition based on the change.
94. The method of claim 93, wherein the heart condition includes heart failure.
95. The method of claim 93, wherein the signal includes an ultrasound signal.
96. The method of claim 93, further comprising positioning the intravascular device by fluoroscopic visualization.
97. The method of claim 96, wherein said positioning further comprises receiving signals from said markers or sensors to confirm position.
98. A monitoring system, comprising:
an intravascular device configured for implantation in a vessel in a body cavity and
having first and second markers biased or secured against opposing interior walls of the vessel;
at least one anchor element configured to secure and position the intravascular device on

- the body cavity wall;
- an anchor isolation structure disposed between said at least one anchor element and said first and second markers, the anchor isolation structure having a length specifically configured to position said first and second markers sufficiently distant from the monitoring location such that diameter calculations derived from said markers are not substantially affected by distortion of the vena cava wall by the anchor element at; and
- an external device adapted to receive a first signal from the intravascular device and to calculate a distance between the first and second markers based on the signal.
99. The monitoring system of claim 98, further comprising a measurement device further adapted to transmit a second signal to the intravascular device.
100. The monitoring system of claim 98, wherein a second signal reflected by the first and second markers creates a reflected signal, and wherein the first signal includes the reflected signal.
101. The monitoring system of claim 100, further wherein a second signal is reflected by the first marker to create a first reflected signal and by the second marker to create a second reflected signal, and wherein the measurement device calculates the distance based on differences in the first and second reflected signals.
102. The monitoring system of claim 100, wherein the first and second markers are electrically charged by a second signal.
103. The monitoring system of claim 98, wherein the external measurement device includes an ultrasound system.
104. The monitoring system of claim 98, wherein the first and second markers include passive markers or reflectors.
105. The monitoring system of claim 104, wherein the first and second markers include active sensors.
106. An intravascular device, comprising:
an anchoring structure for anchoring within the vessel; and
first and second arms extending longitudinally from the anchoring structure, wherein the

first and second markers are coupled to the first and second arms, respectively, wherein the first and second arms are configured to bias the first and second markers against the vessel wall and to allow the first and second markers to move inwardly and outwardly with physiologic movement of the vessel wall.

107. A therapeutic system for treating a patient, comprising
a monitoring system including an intravascular implant for implantation in a vena cava configured to monitor a dimension of the vena cava;
a transmission device to transmit data based on the dimension; and
a therapeutic device implanted in the patient and configured to receive the data transmitted from the monitoring system, the therapeutic device adapted to deliver therapy to the patient based upon the data received.
108. The system of claim 107, wherein the therapeutic device is a pacemaker.
109. The system of claim 107, wherein the therapeutic device includes an infusion pump.
110. The system of claim 107, further comprising a lead connecting the intravascular implant to the therapeutic device, wherein the lead may be intravascular and/or configured to extend through a penetration in a wall of the vena cava.

1 / 39

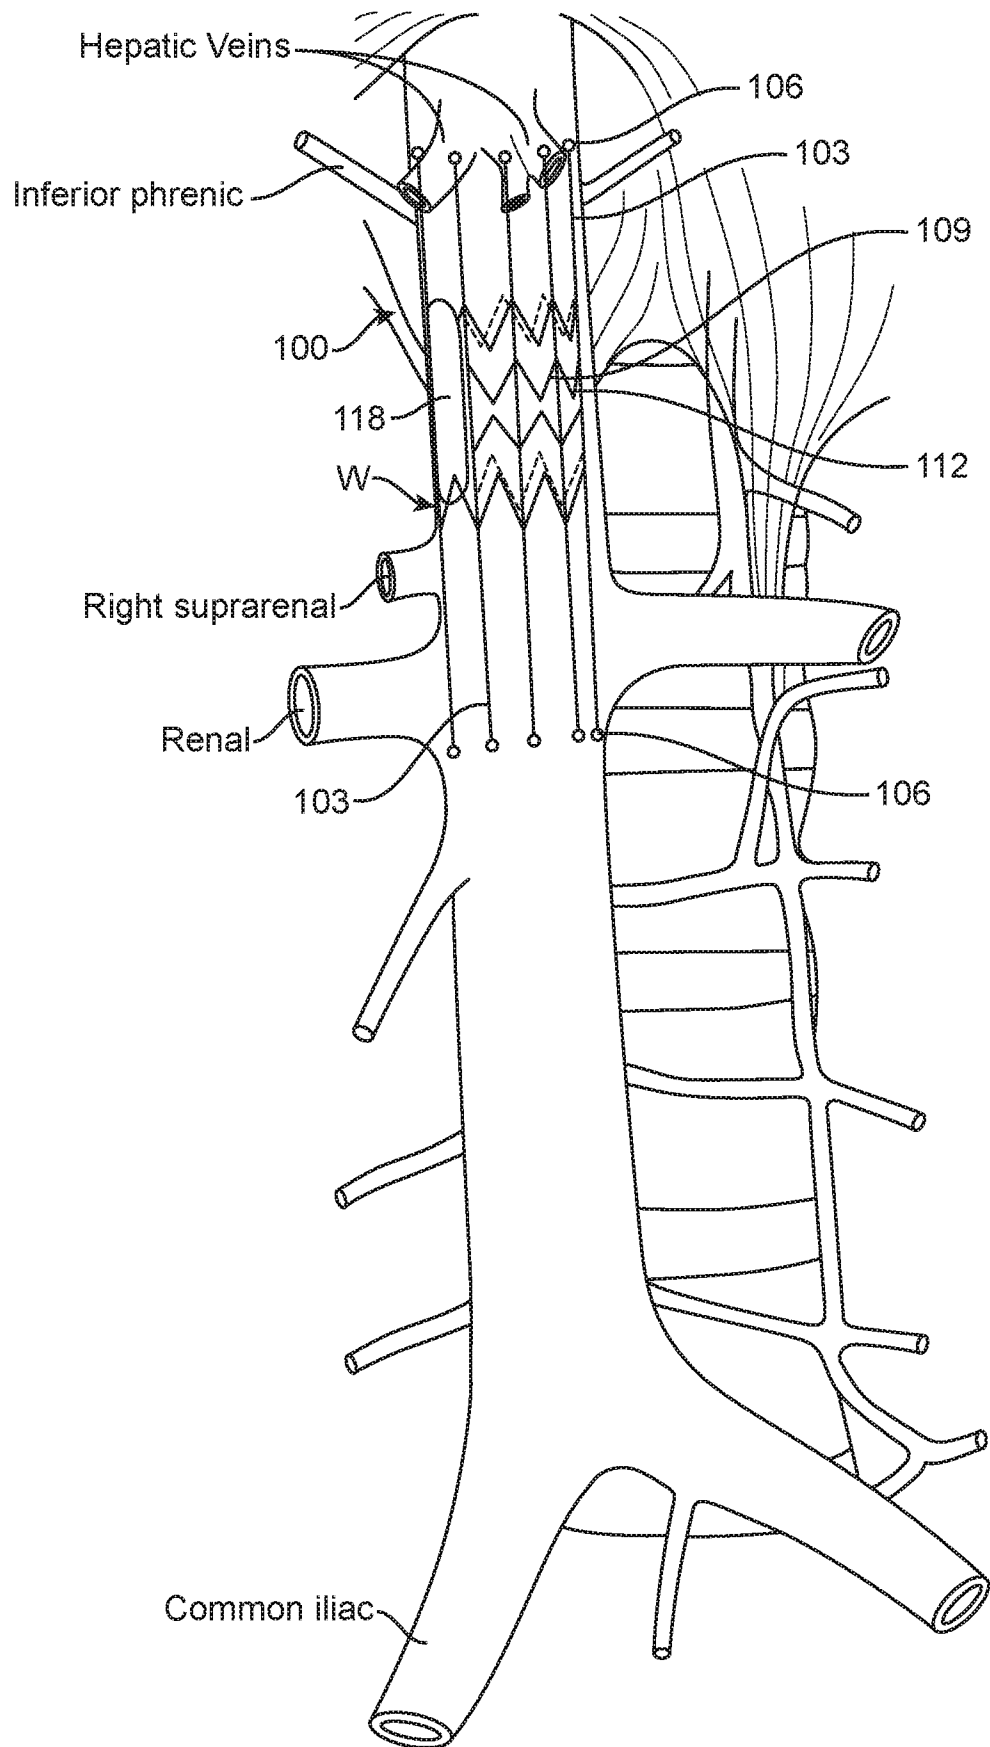


FIG. 1

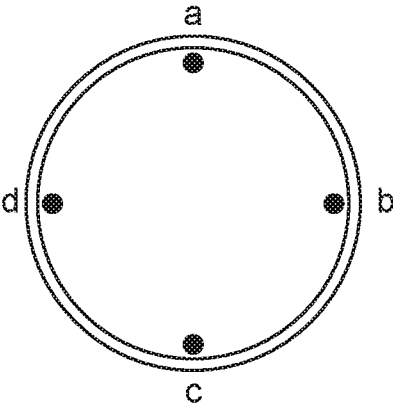


FIG. 2A

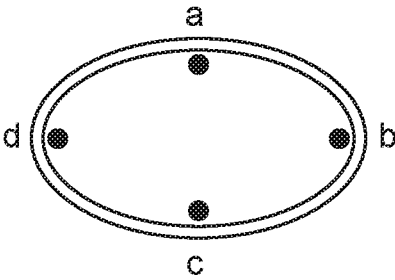


FIG. 2B

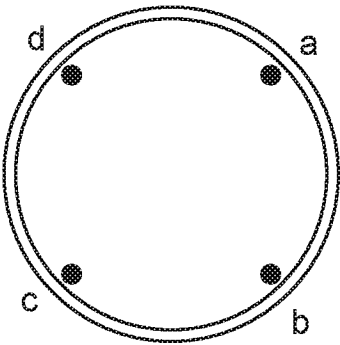


FIG. 2C

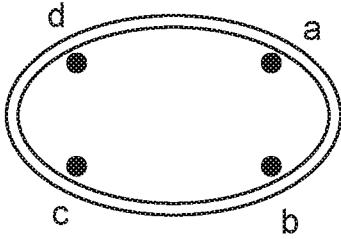


FIG. 2D

3 / 39

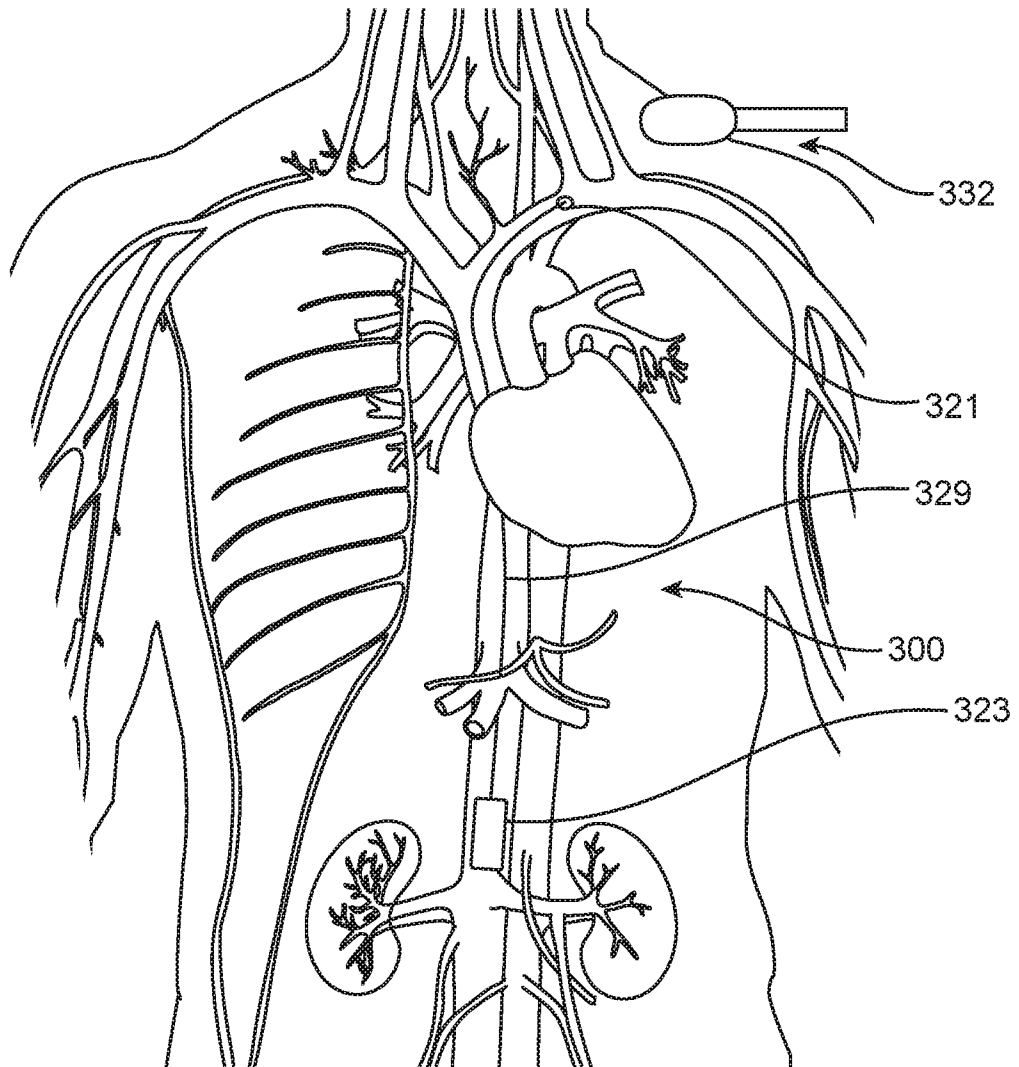


FIG. 3

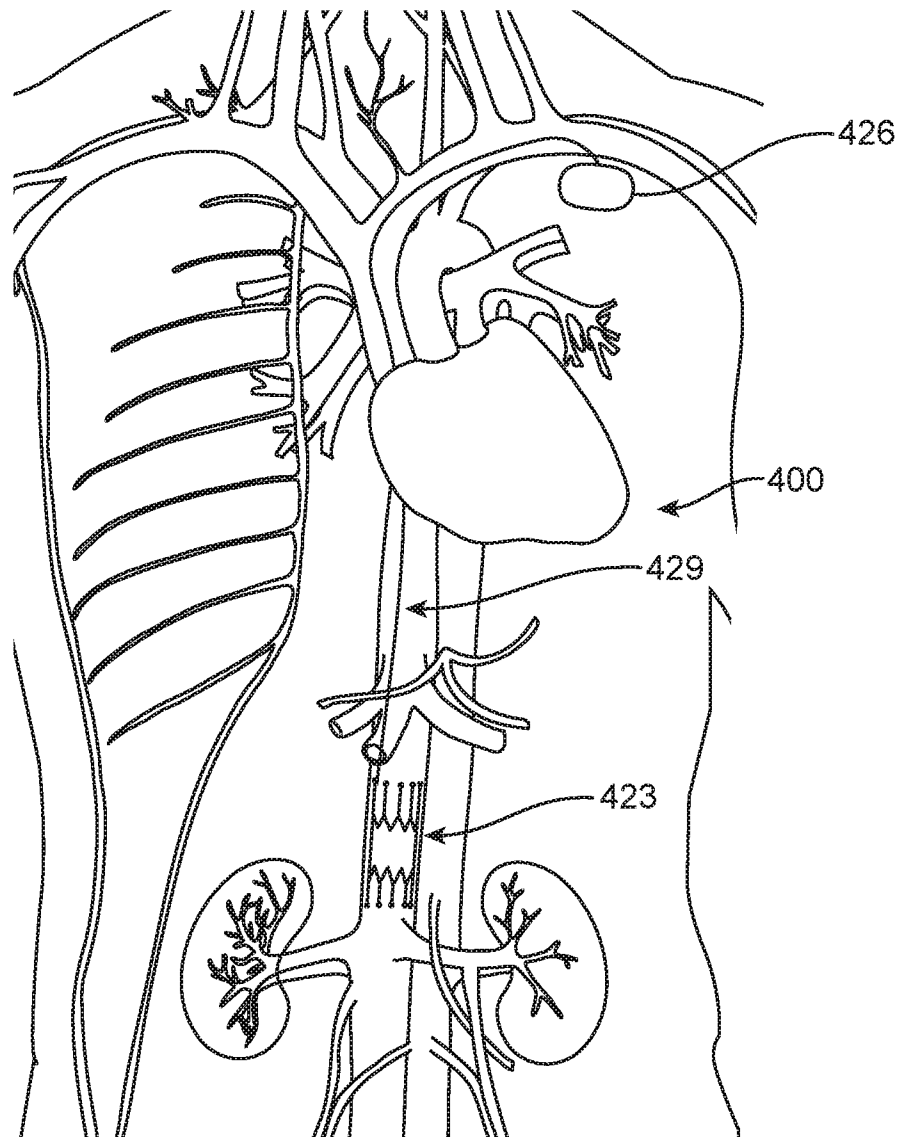


FIG. 4


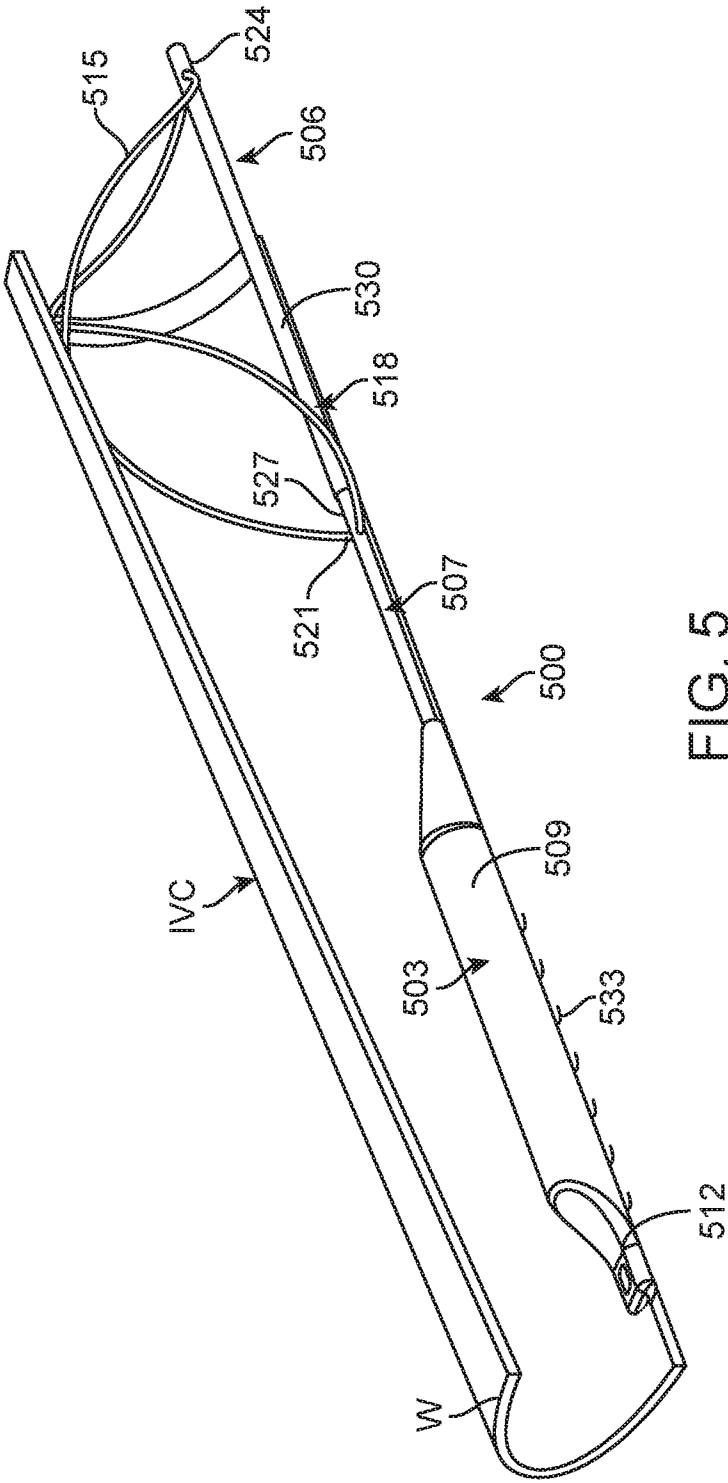


FIG. 5

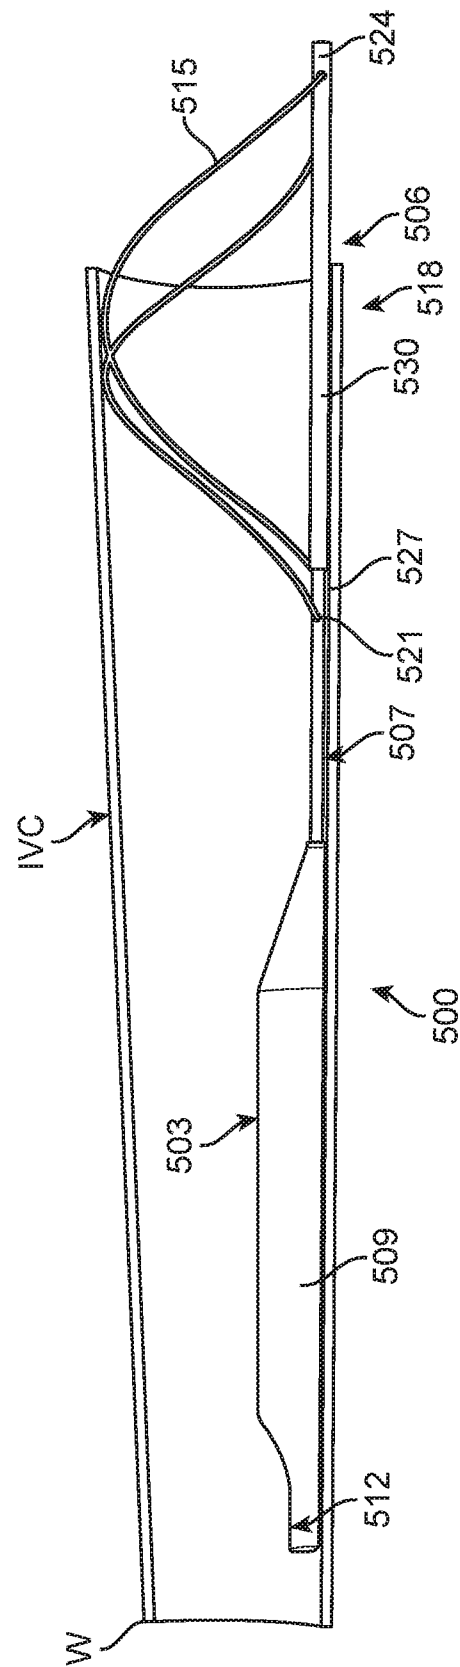

6
7
8
9

7 / 39

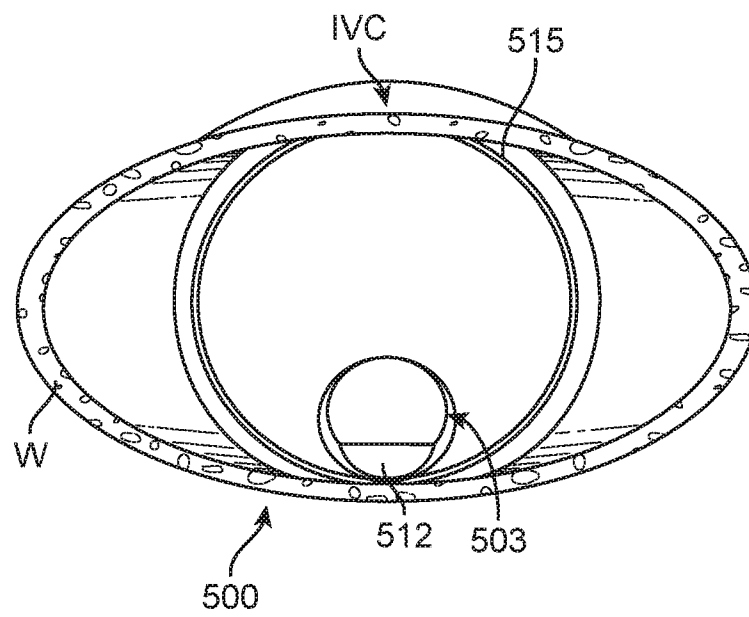


FIG. 7

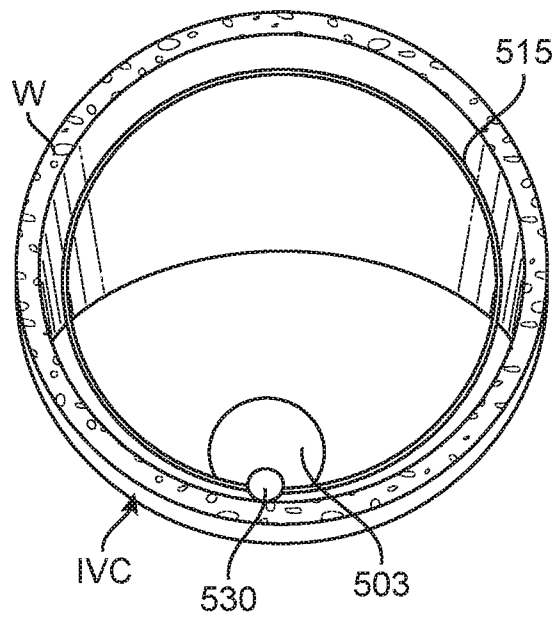


FIG. 8

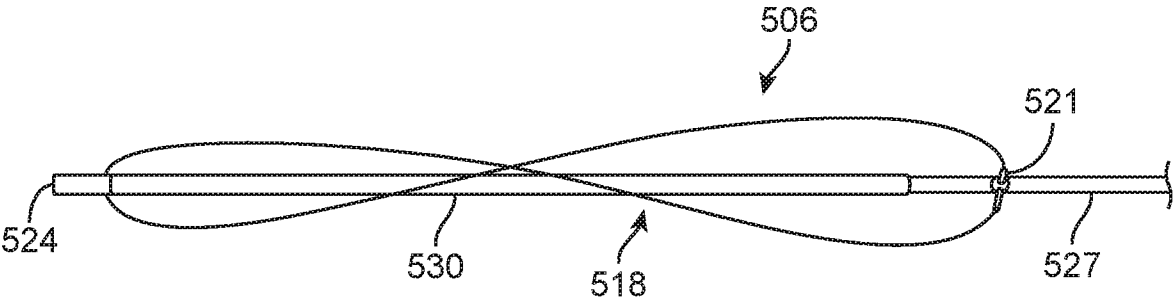


FIG. 9

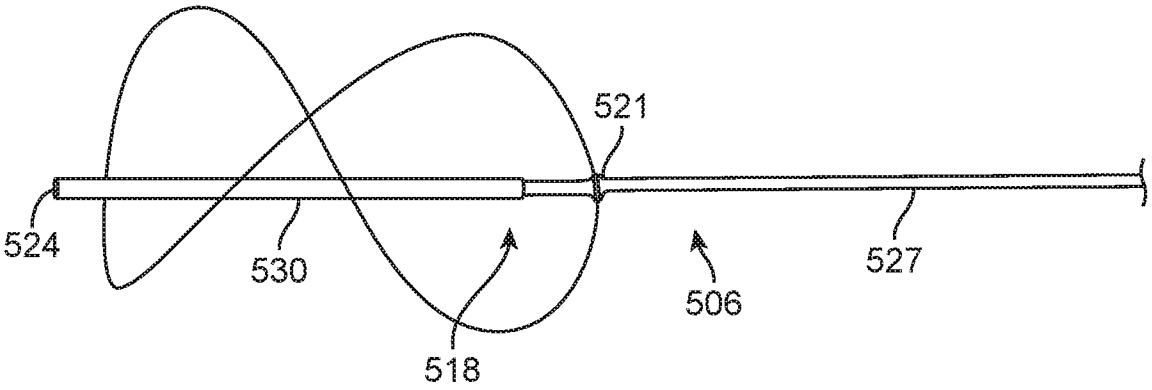


FIG. 10

10 / 39

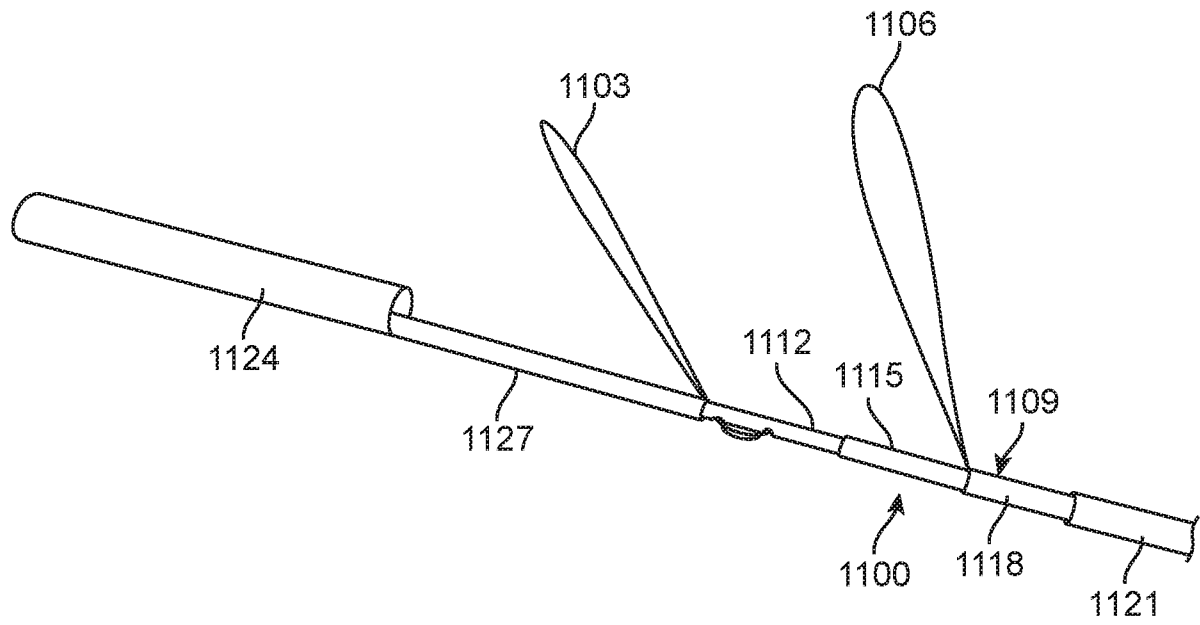


FIG. 11


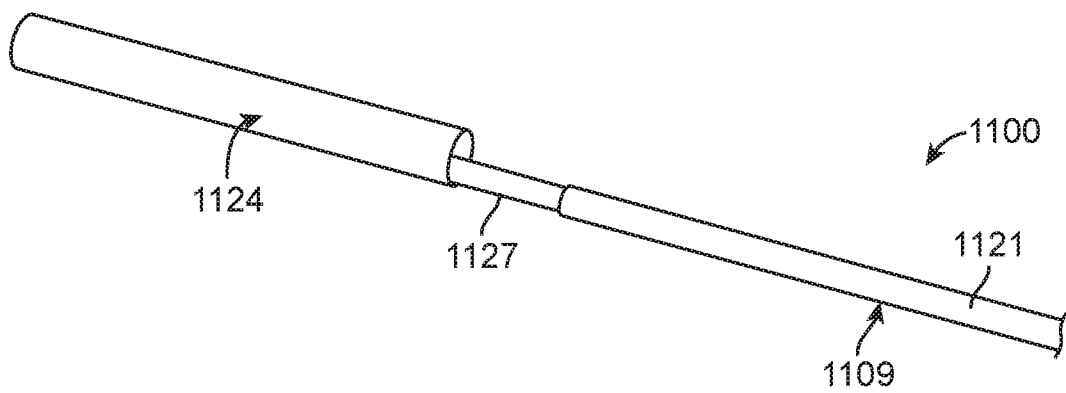


FIG. 12

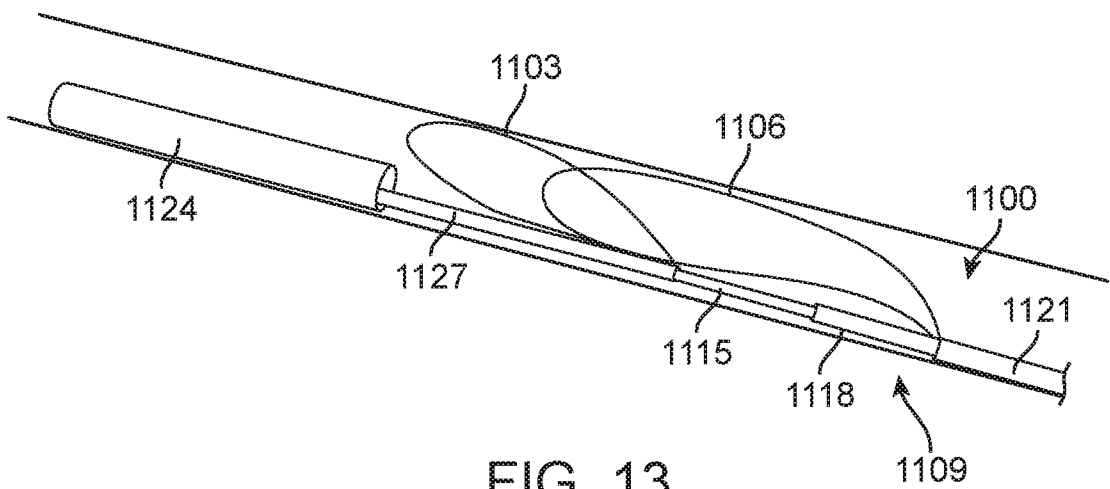

12 / 39

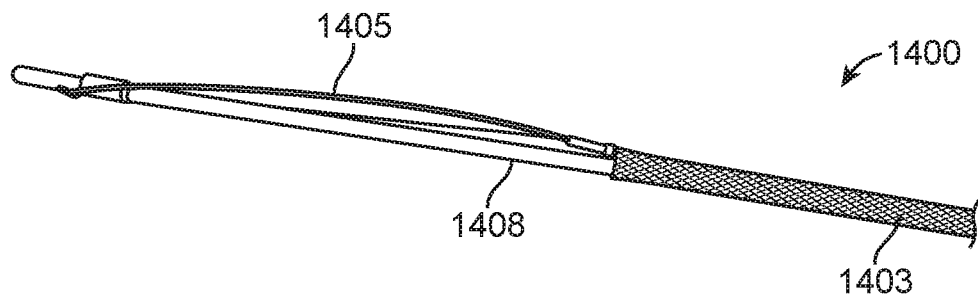


FIG. 14

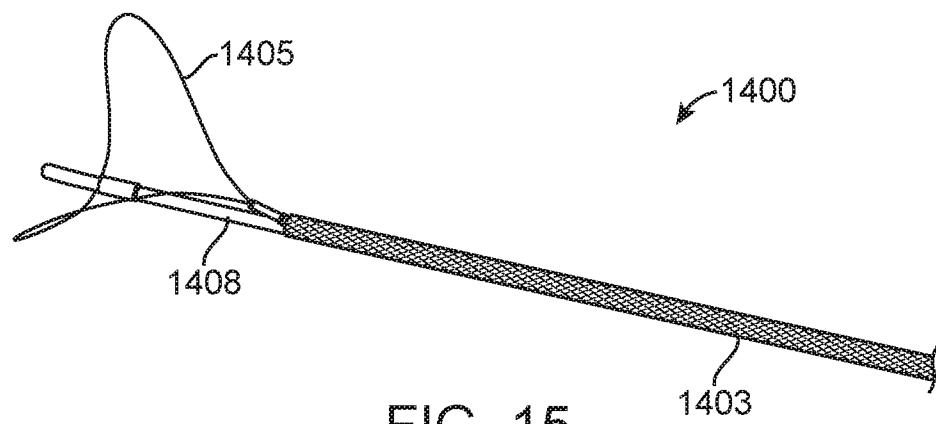


FIG. 15

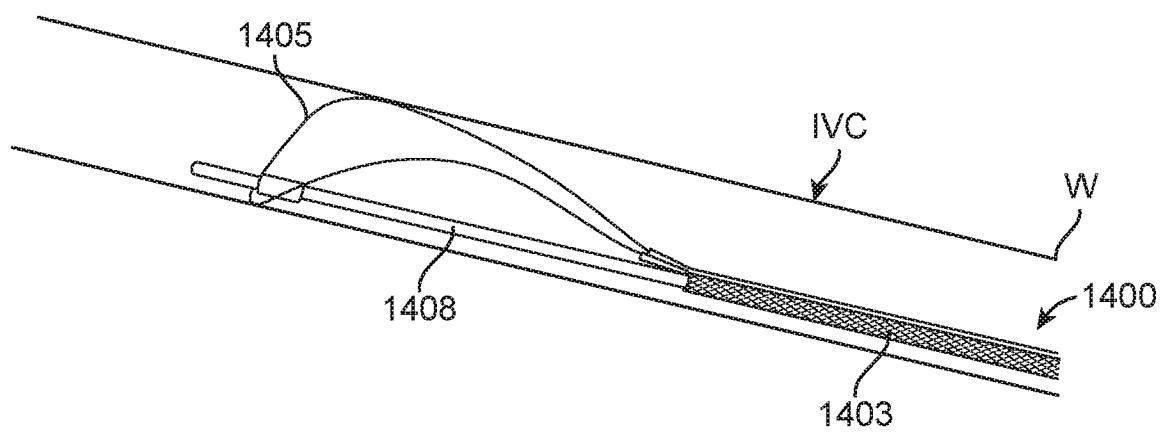


FIG. 16

13 / 39

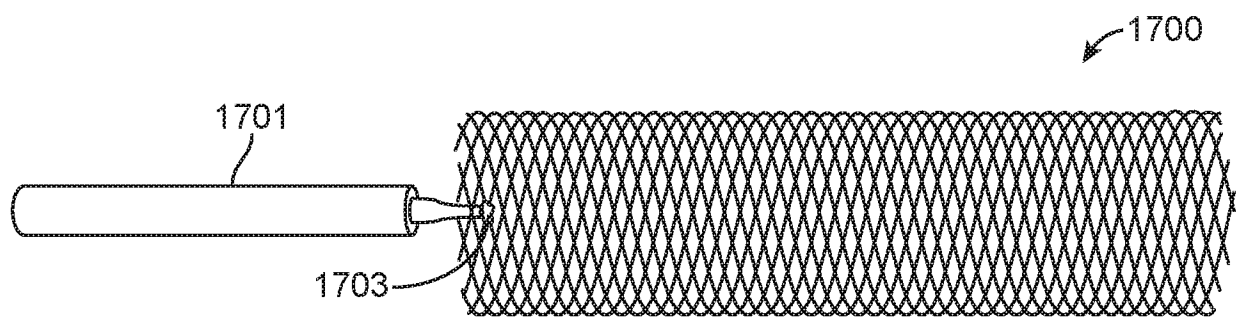


FIG. 17

14 / 39

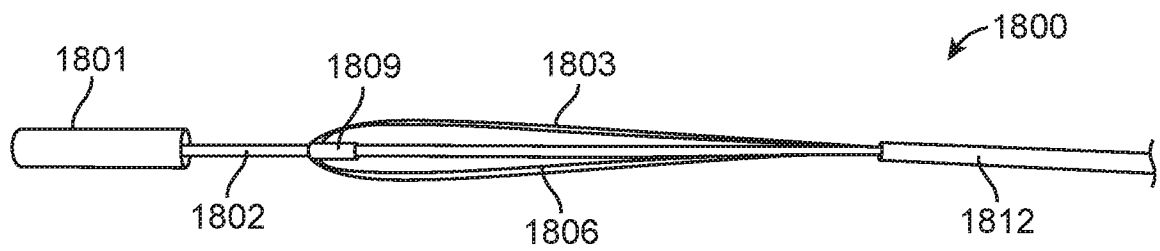


FIG. 18

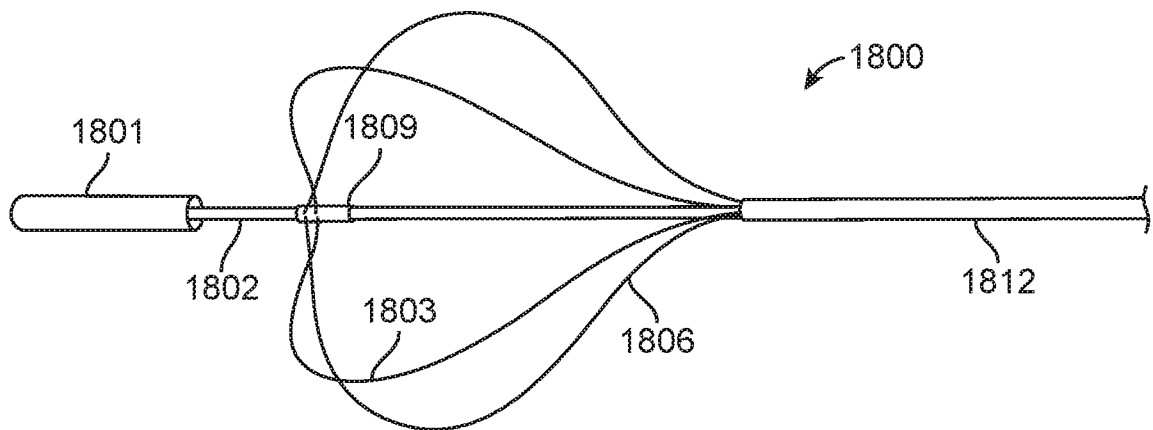


FIG. 19

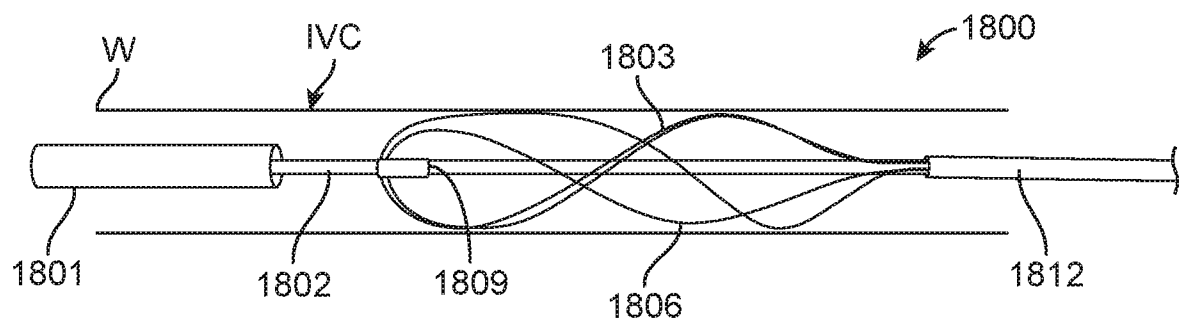


FIG. 20

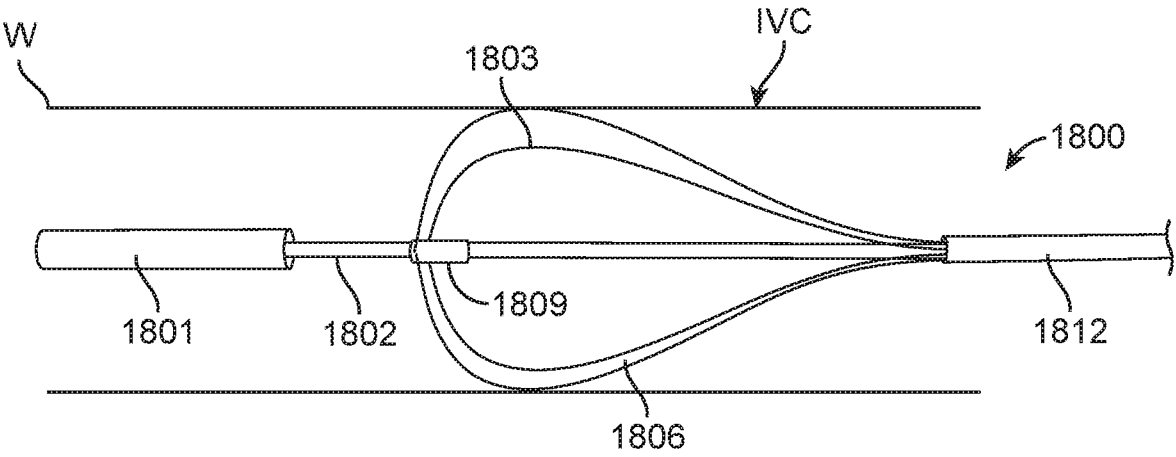


FIG. 21

16 / 39

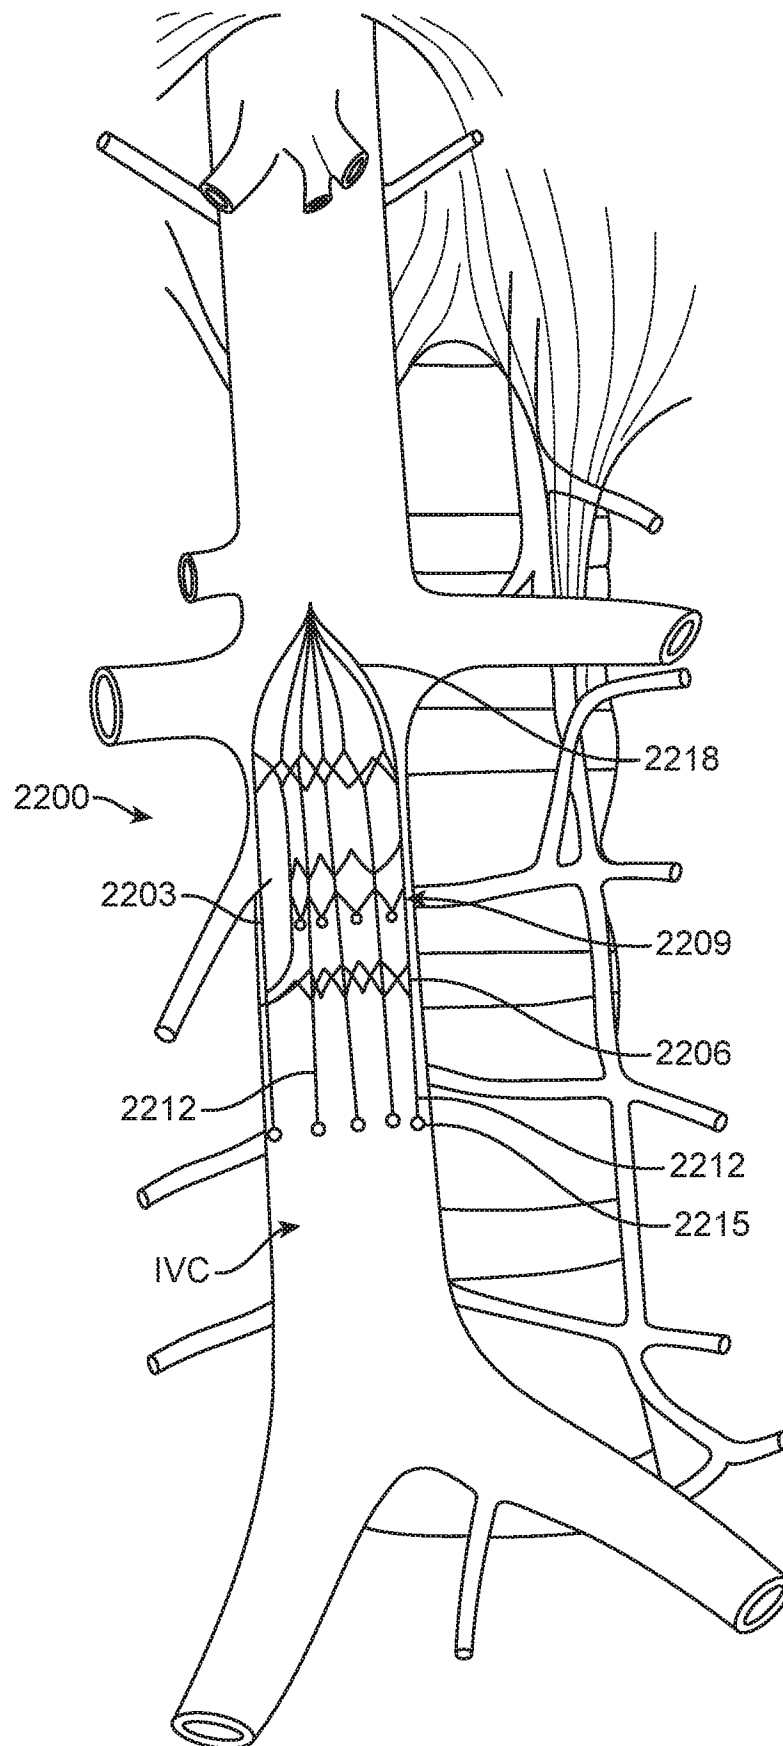


FIG. 22

17 / 39

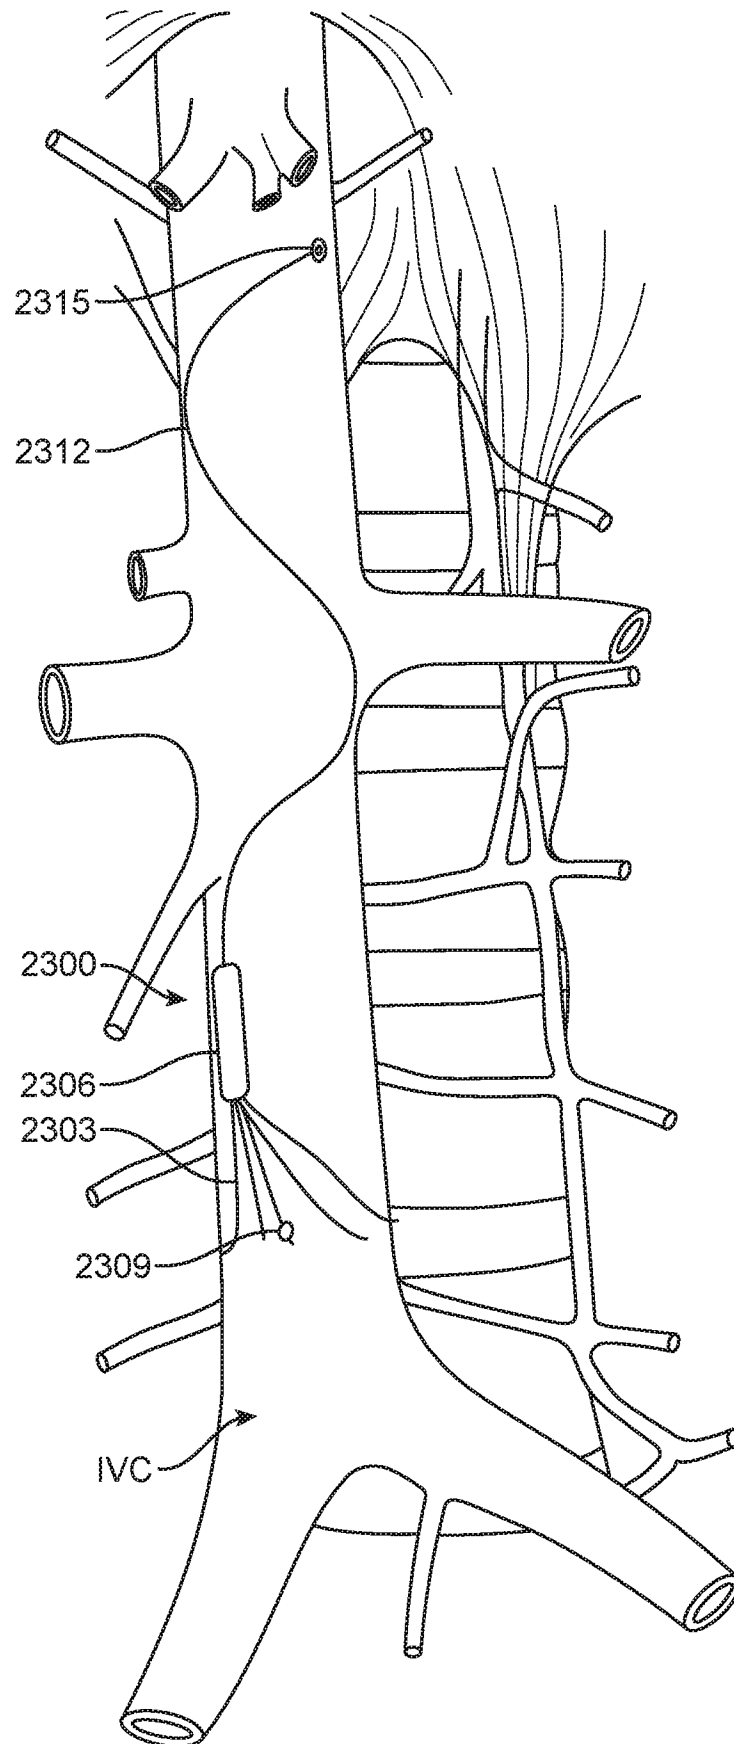


FIG. 23

18 / 39

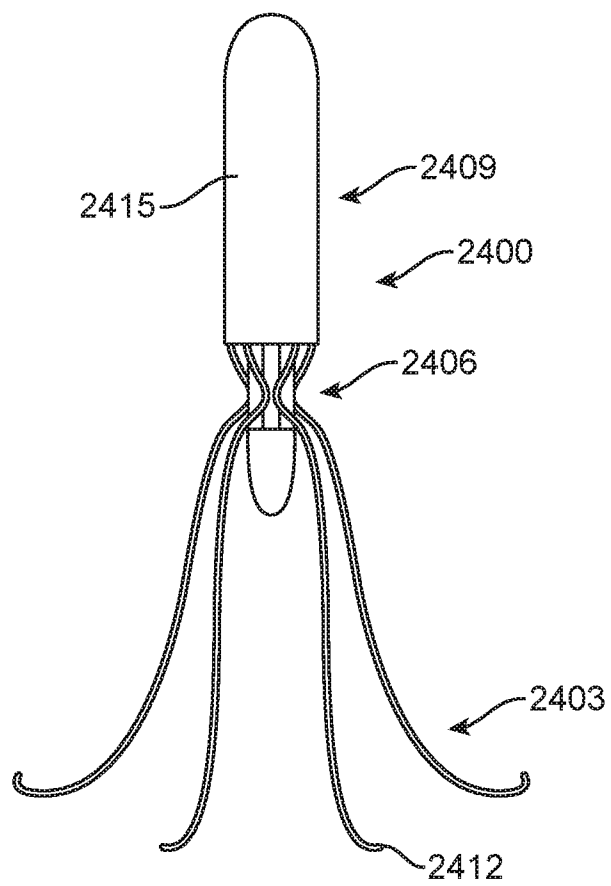


FIG. 24

19 / 39

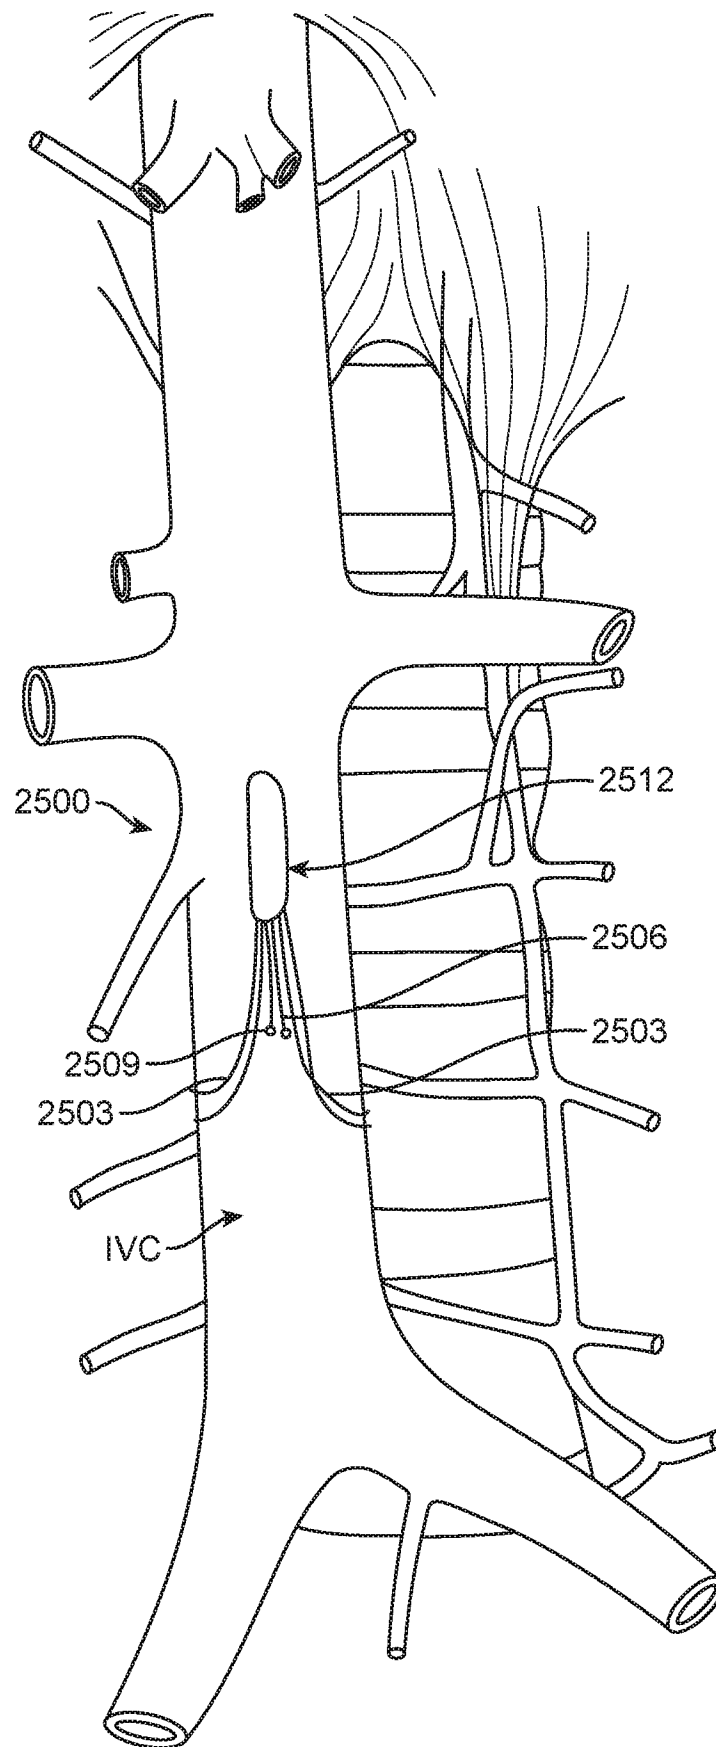


FIG. 25

20 / 39

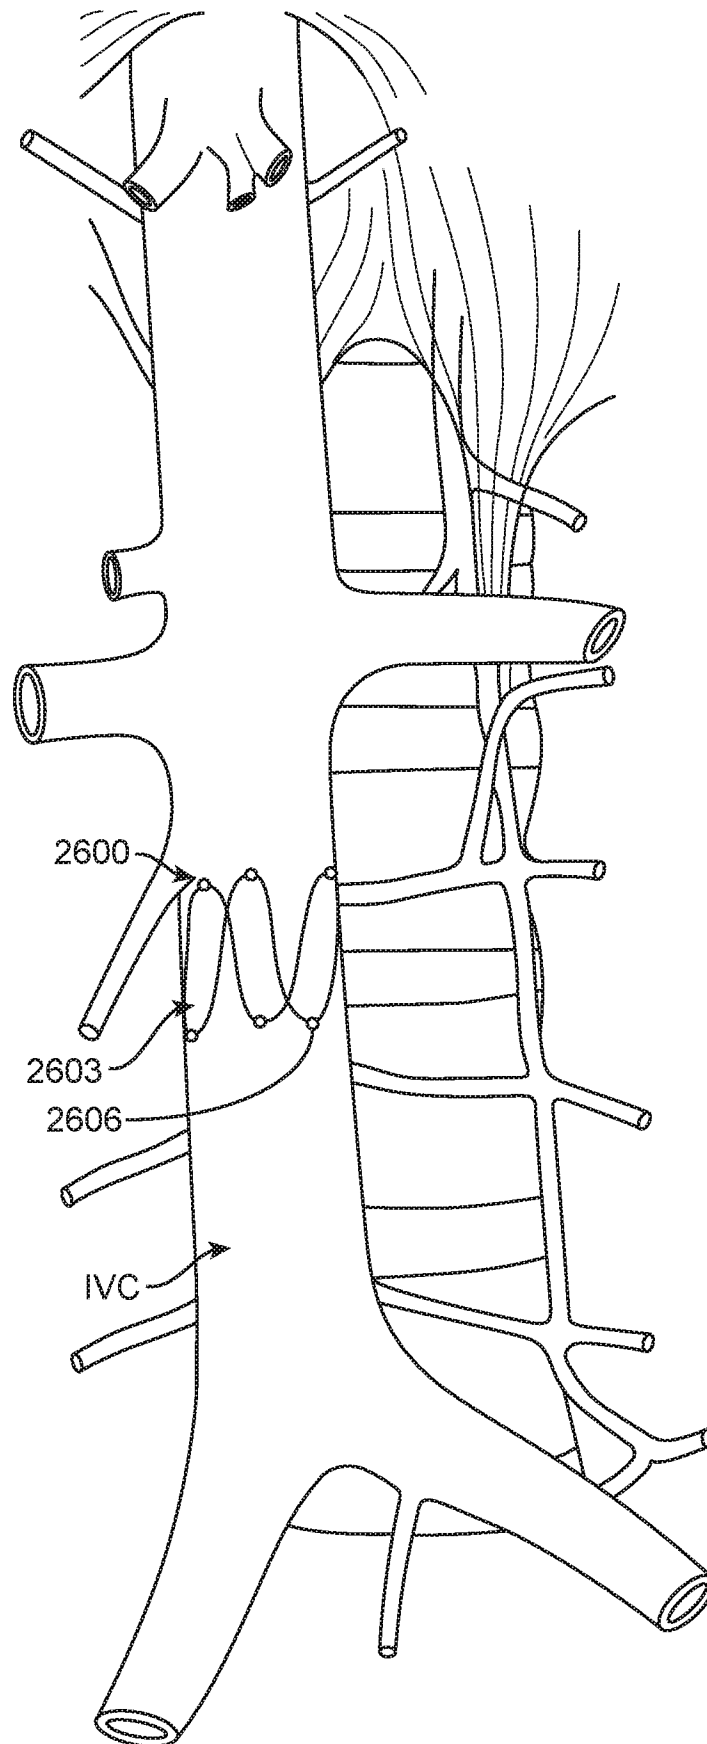


FIG. 26

21 / 39

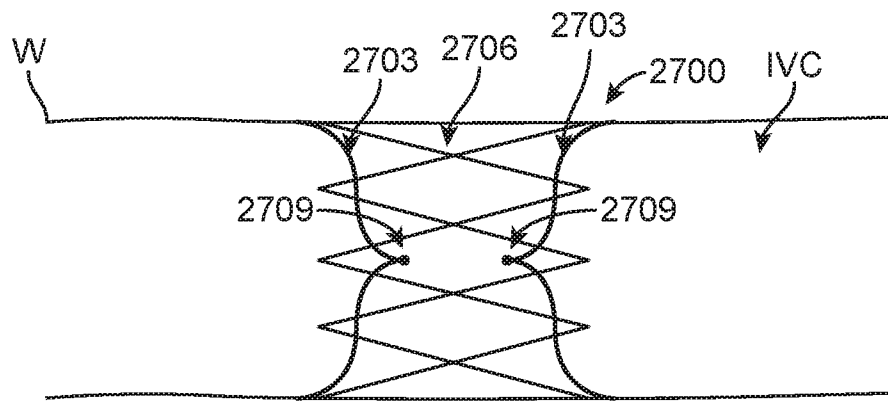


FIG. 27A

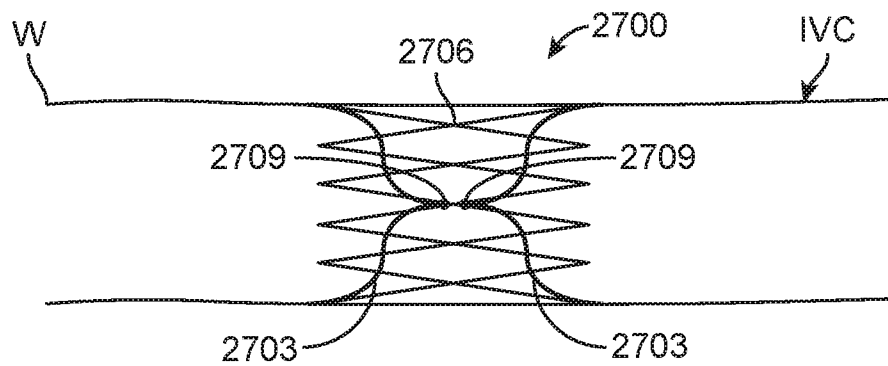


FIG. 27B

22 / 39

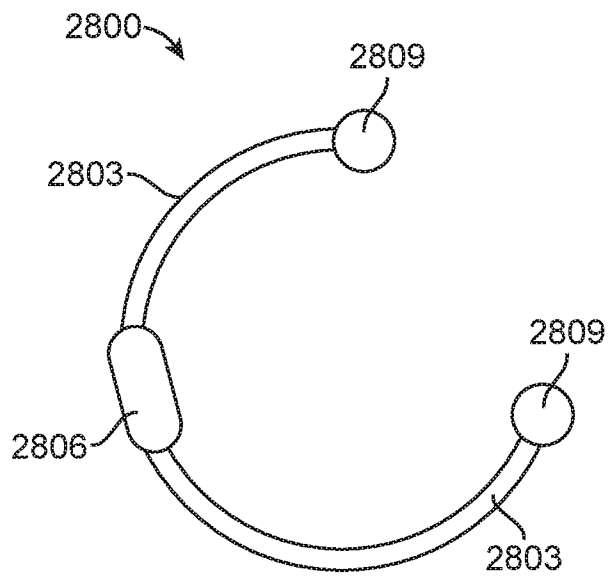


FIG. 28A

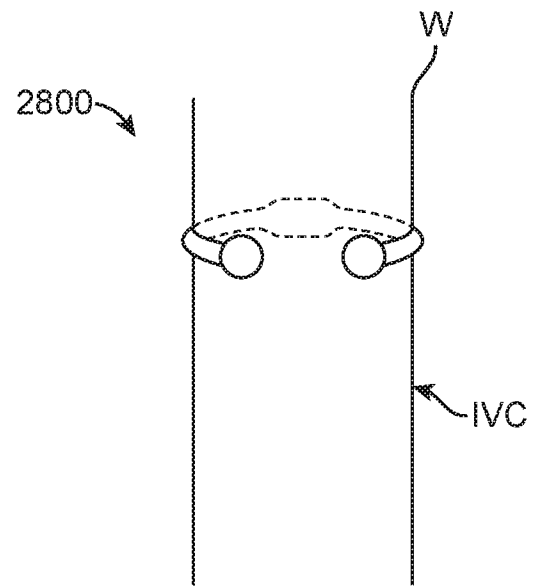


FIG. 28B

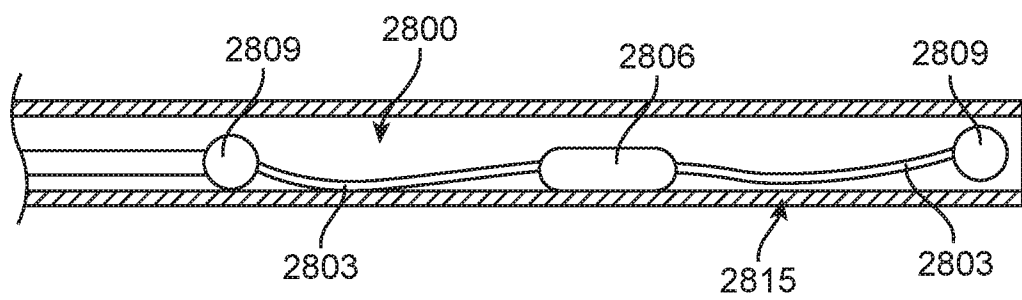


FIG. 28C

23 / 39



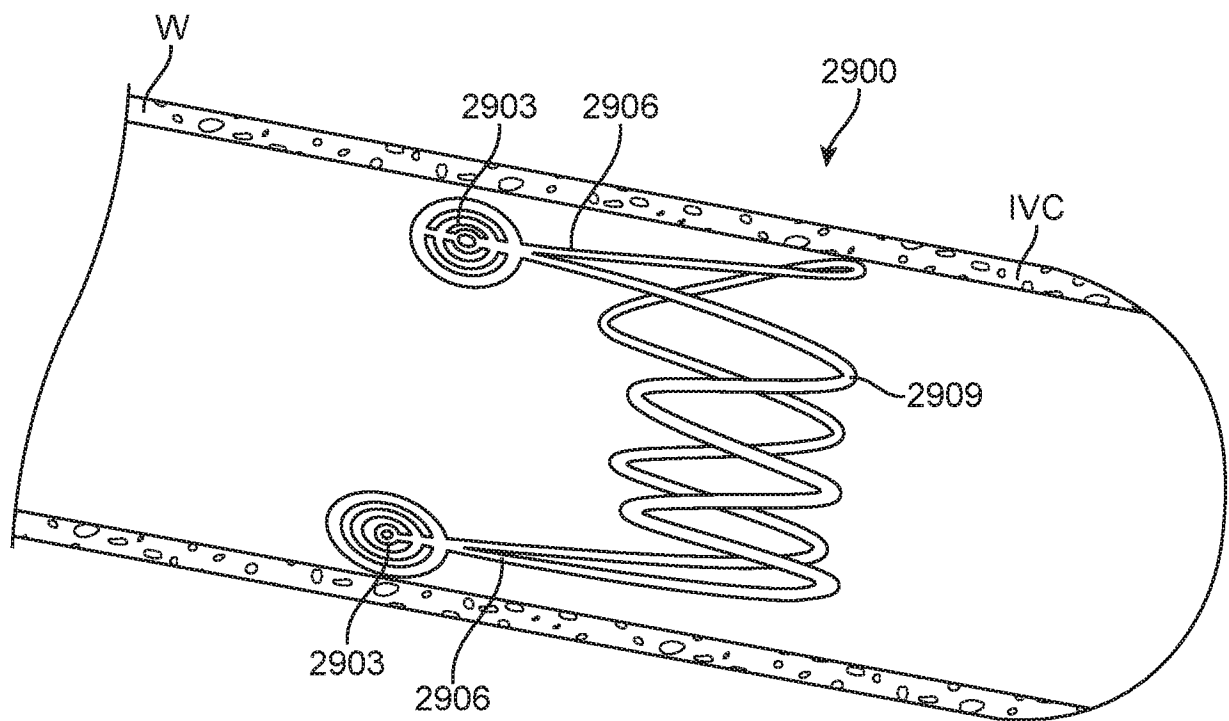


FIG. 29

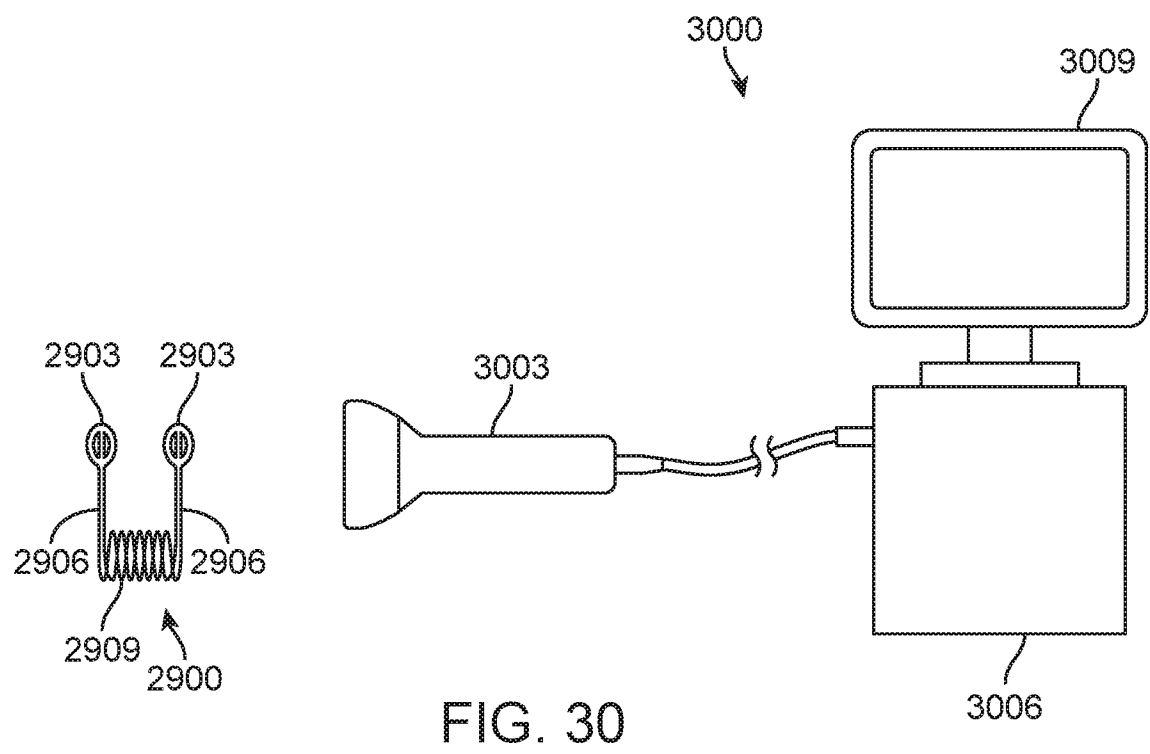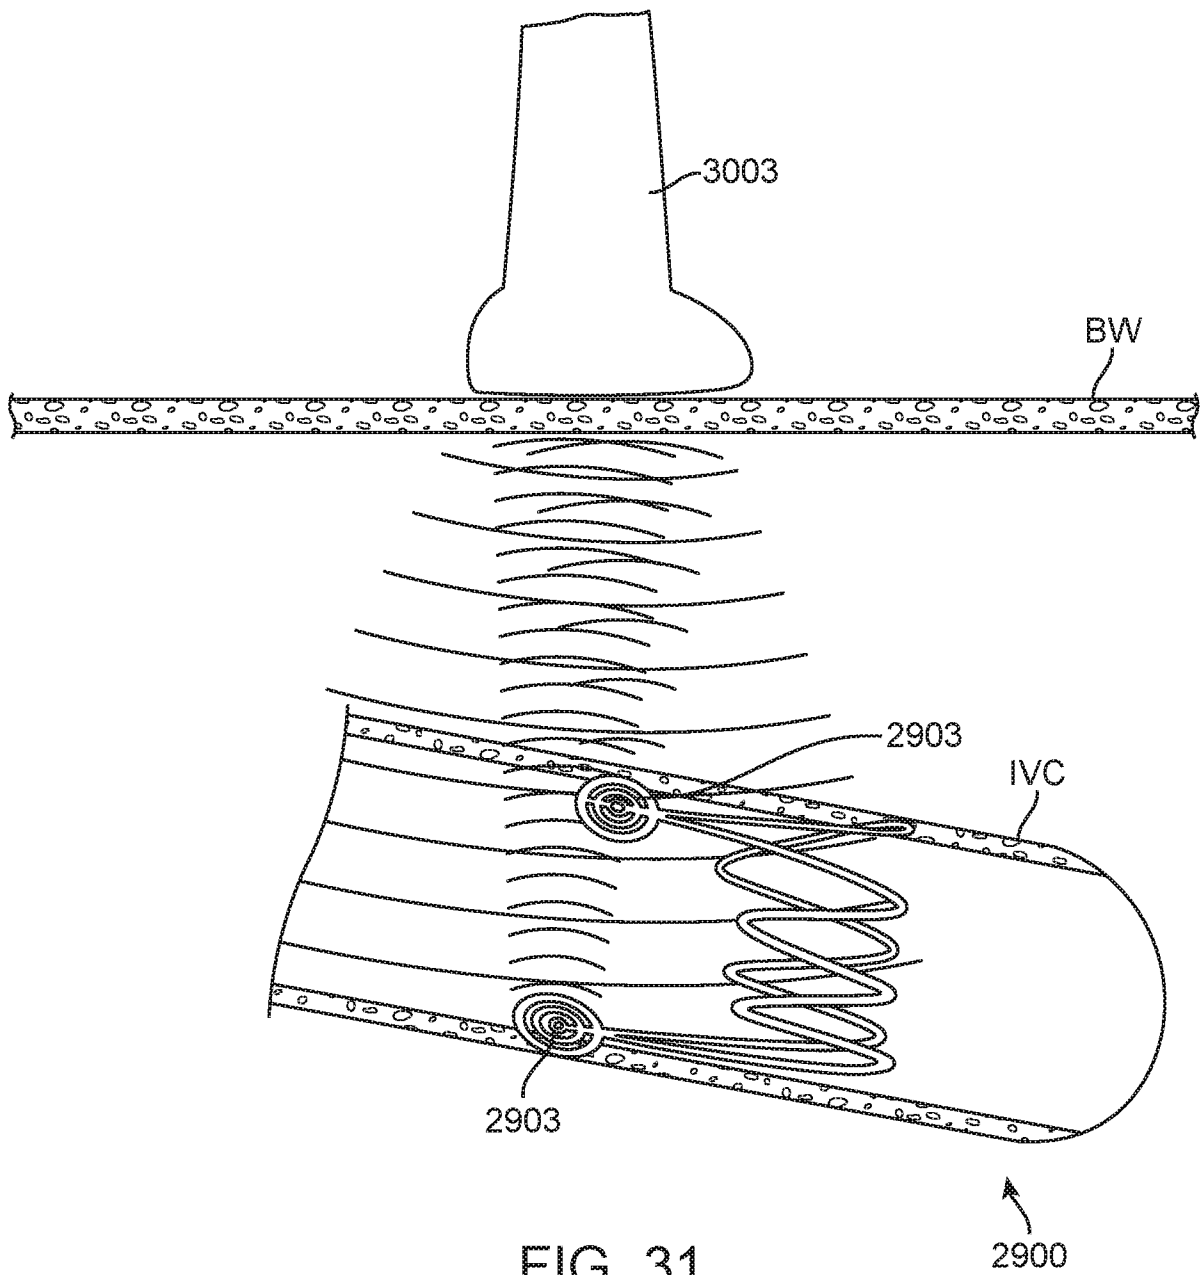

25 / 39



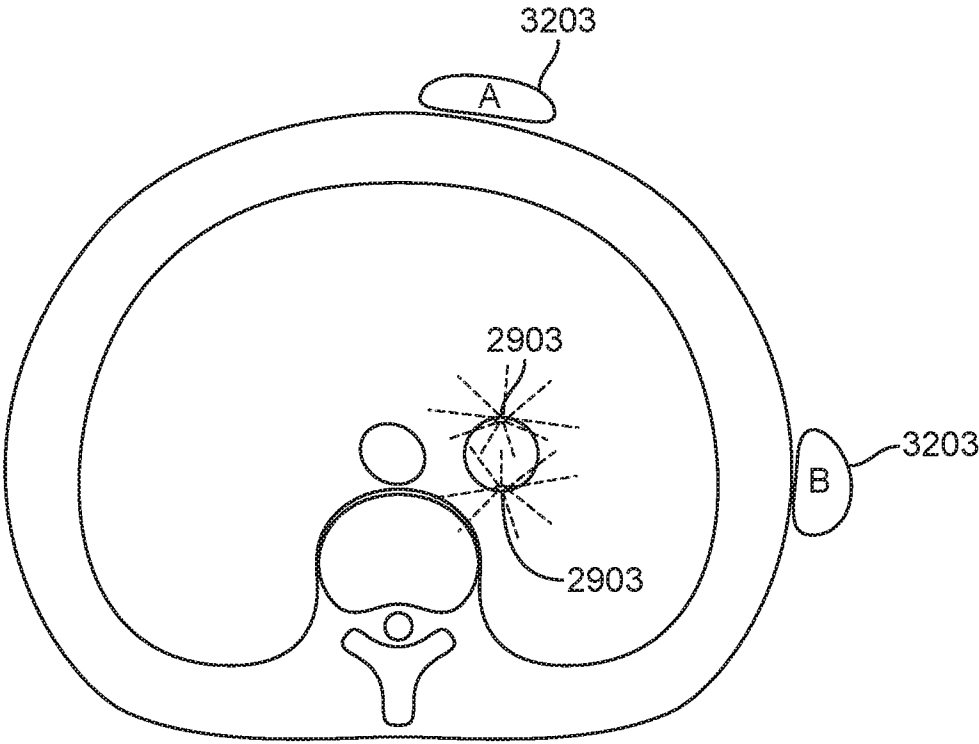


FIG. 32

27 / 39

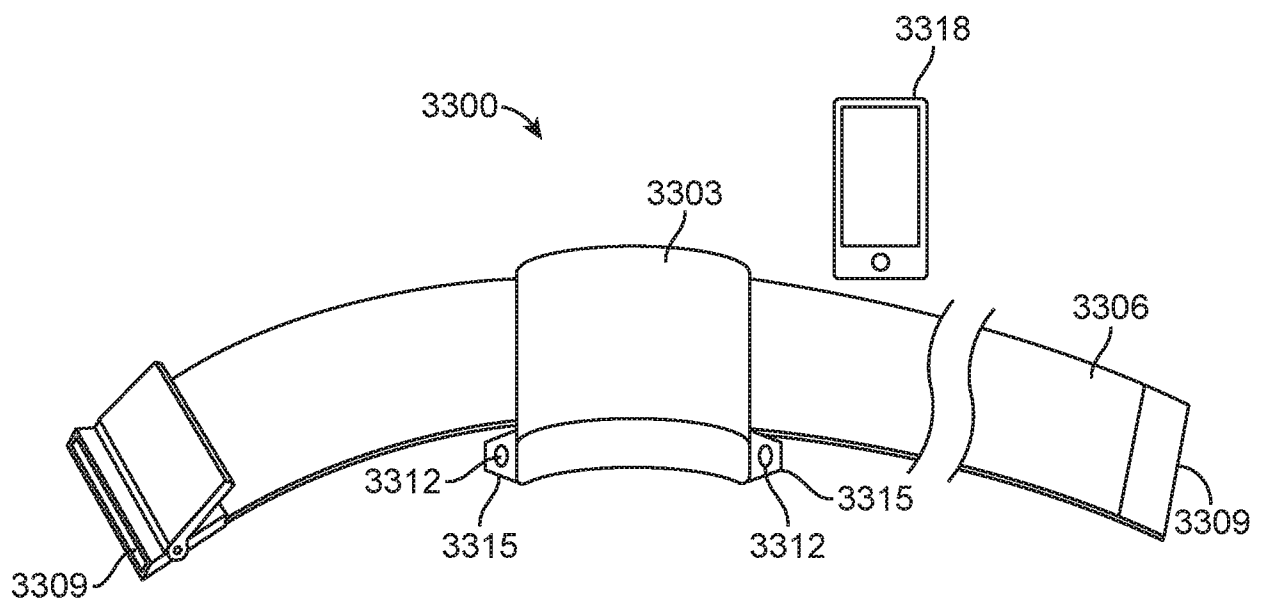


FIG. 33

28 / 39

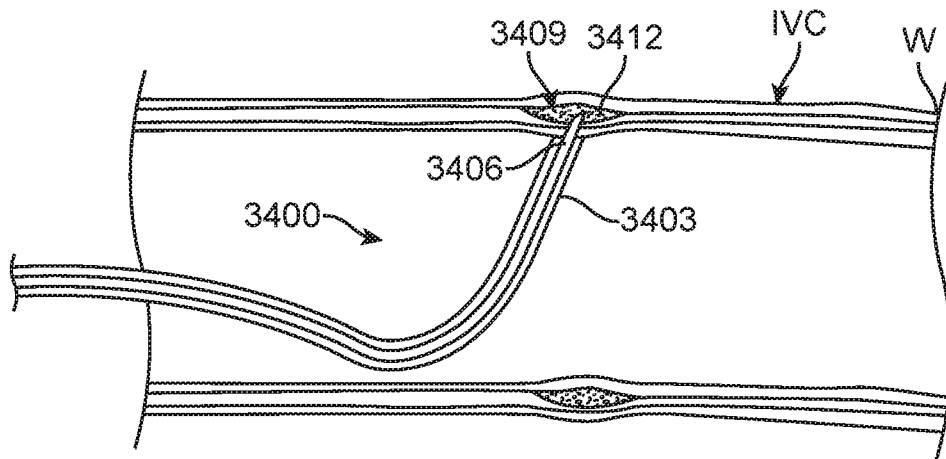


FIG. 34A

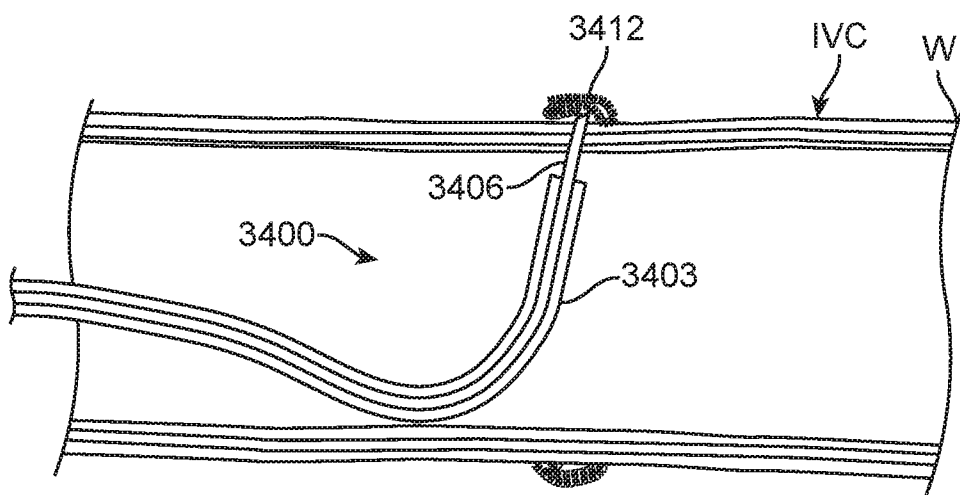


FIG. 34B

29 / 39

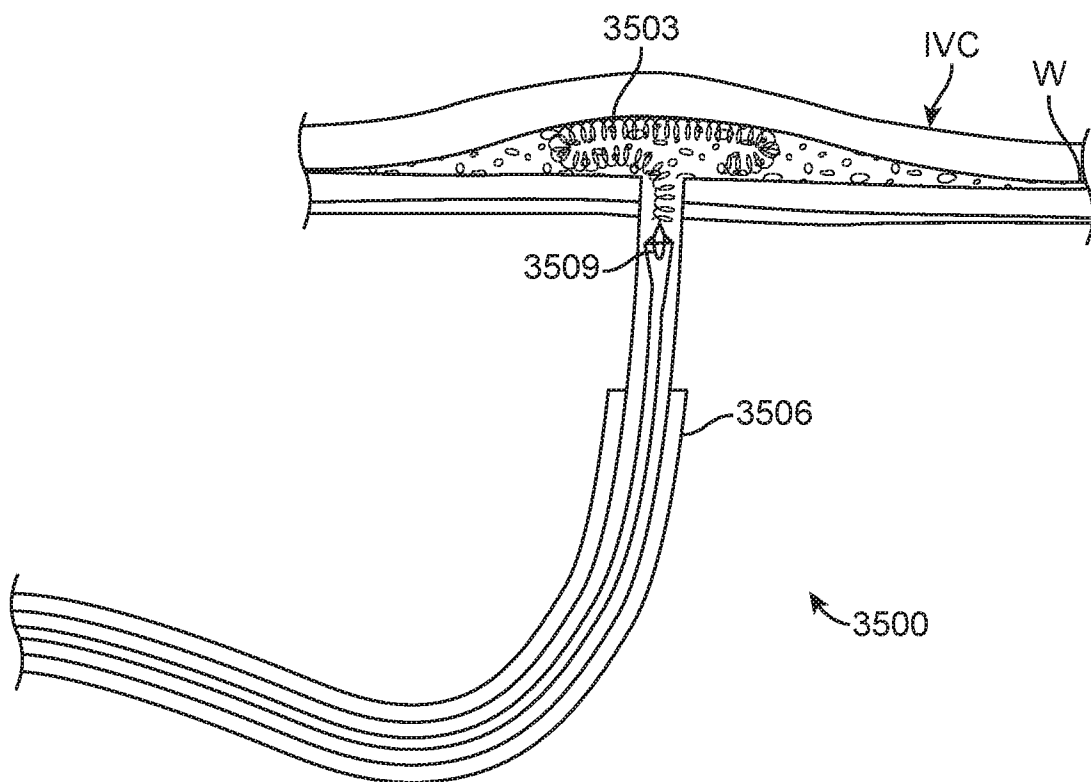


FIG. 35

30 / 39

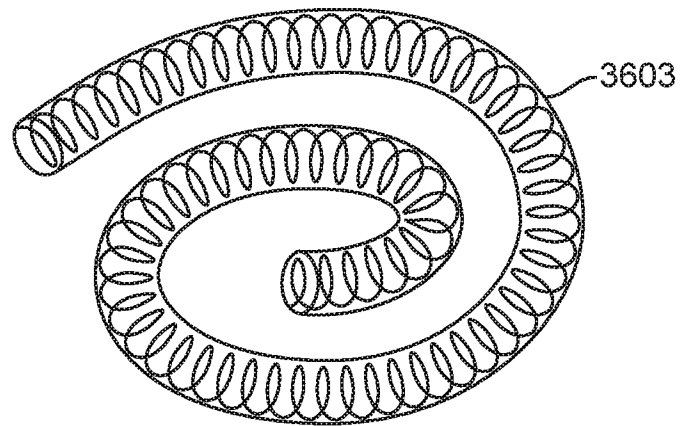


FIG. 36A

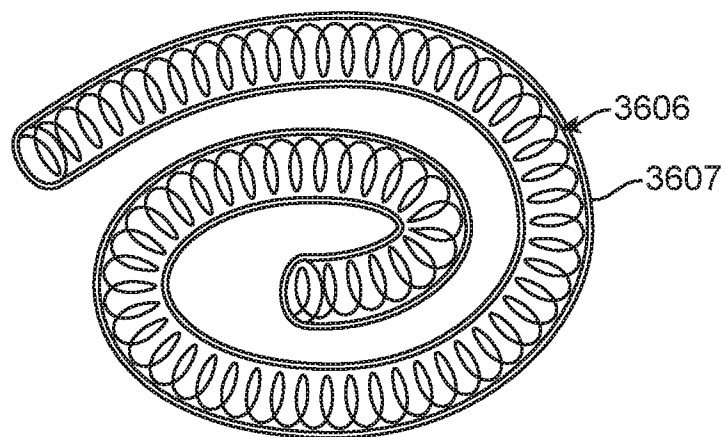


FIG. 36B

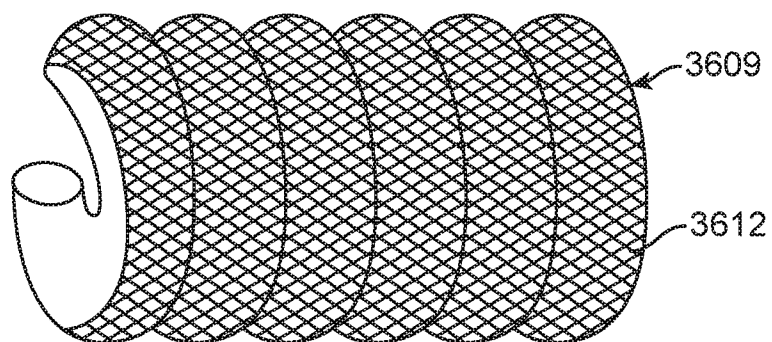


FIG. 36C

31 / 39

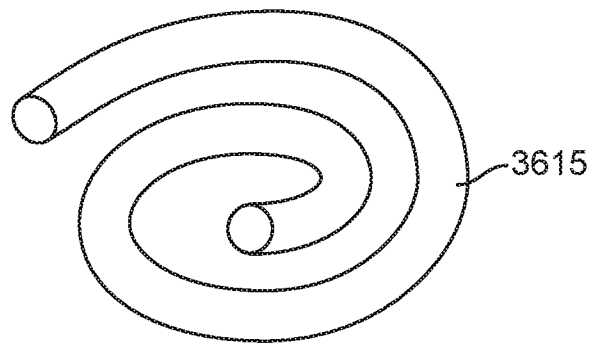


FIG. 36D

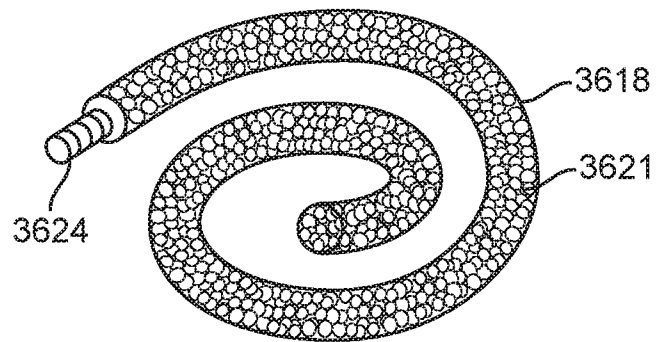


FIG. 36E

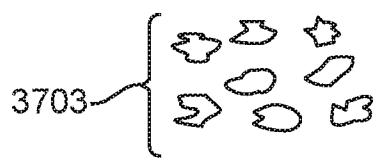


FIG. 37A

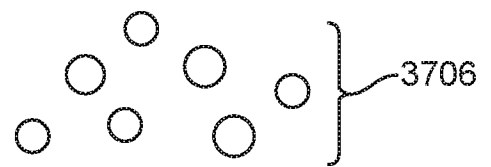


FIG. 37B

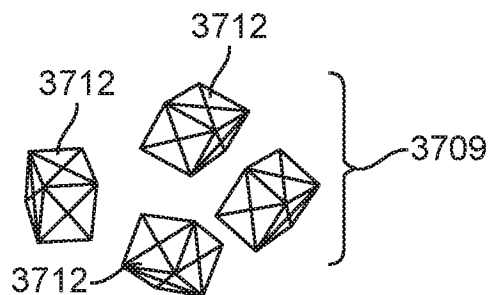


FIG. 37C

32 / 39

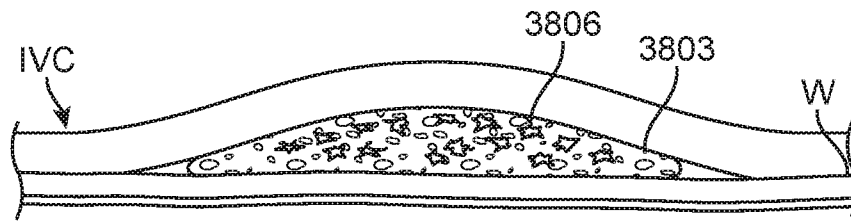


FIG. 38

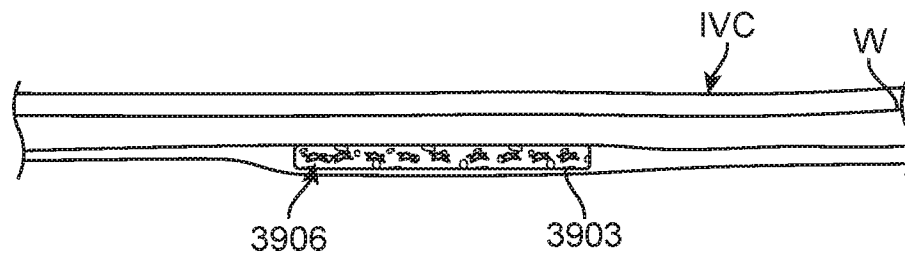


FIG. 39A

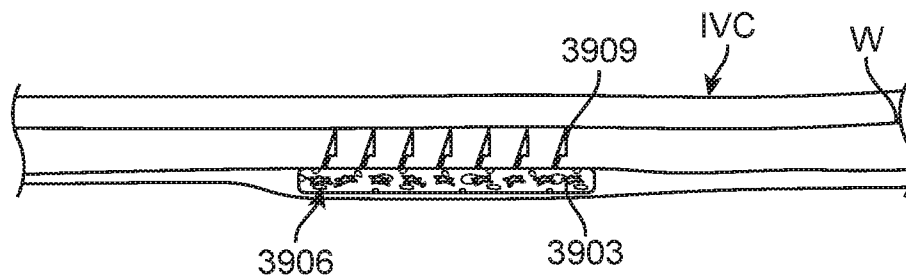


FIG. 39B

33 / 39

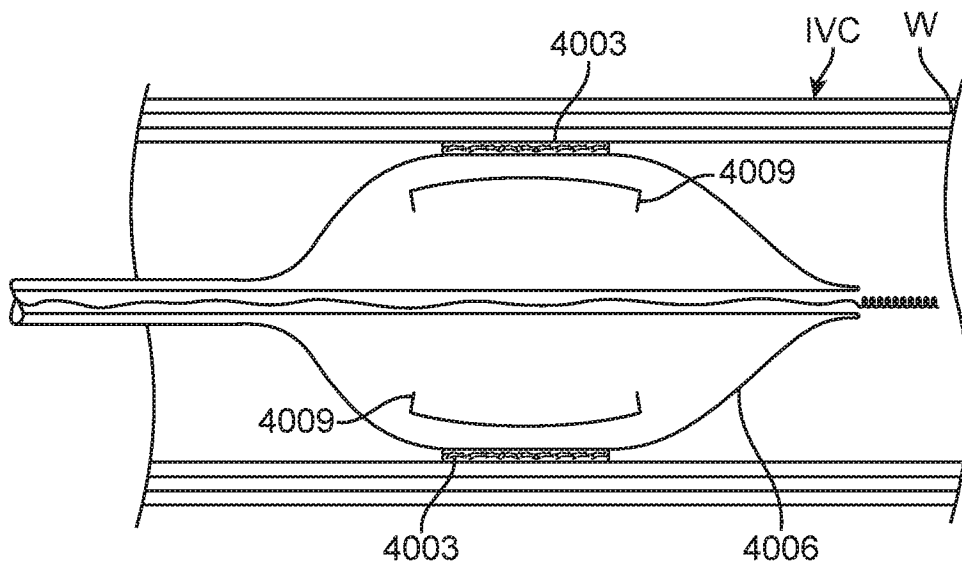


FIG. 40A

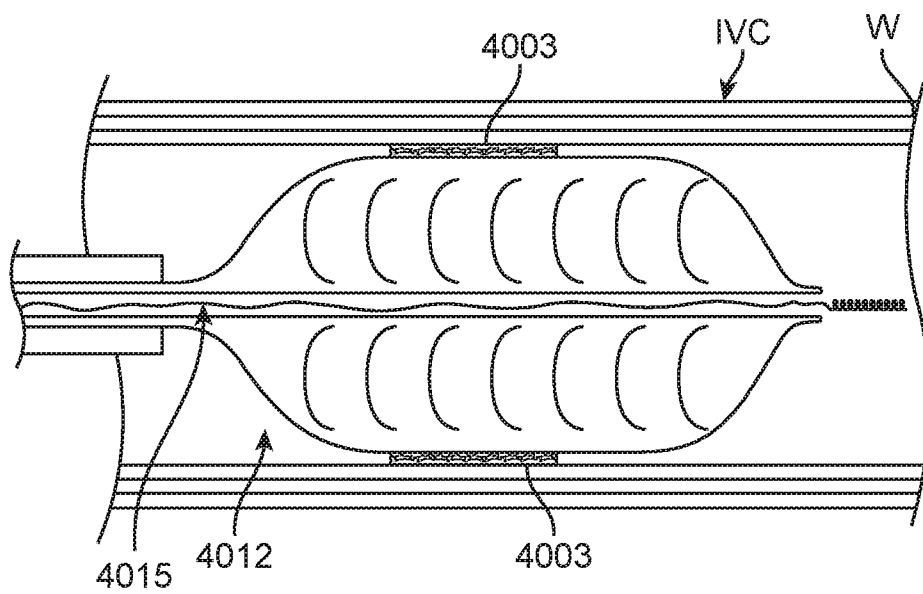


FIG. 40B

34 / 39

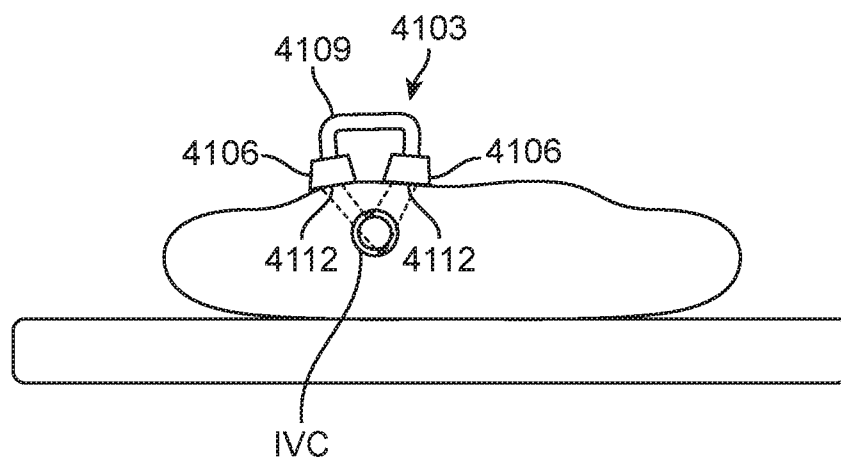


FIG. 41

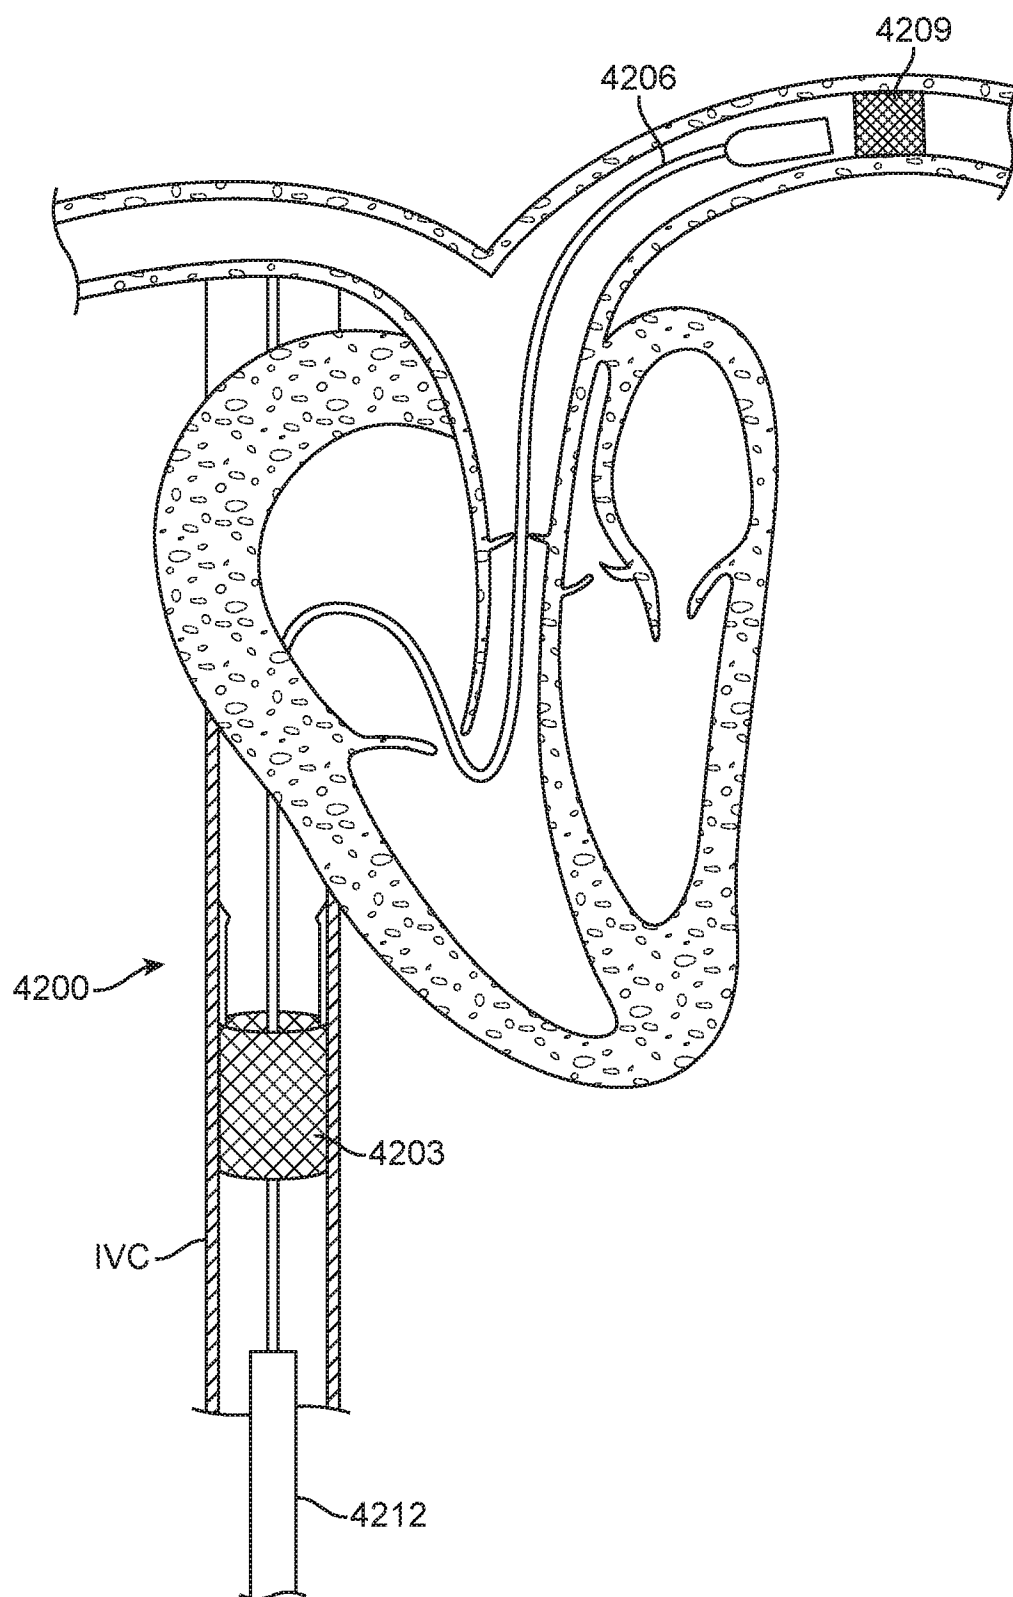


FIG. 42

36 / 39

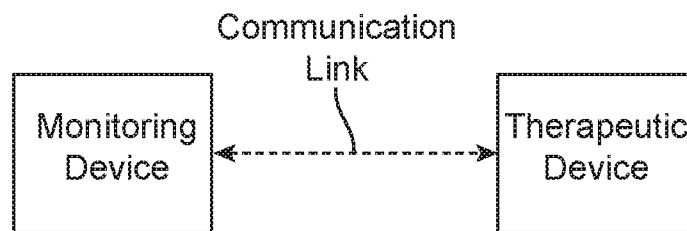


FIG. 43

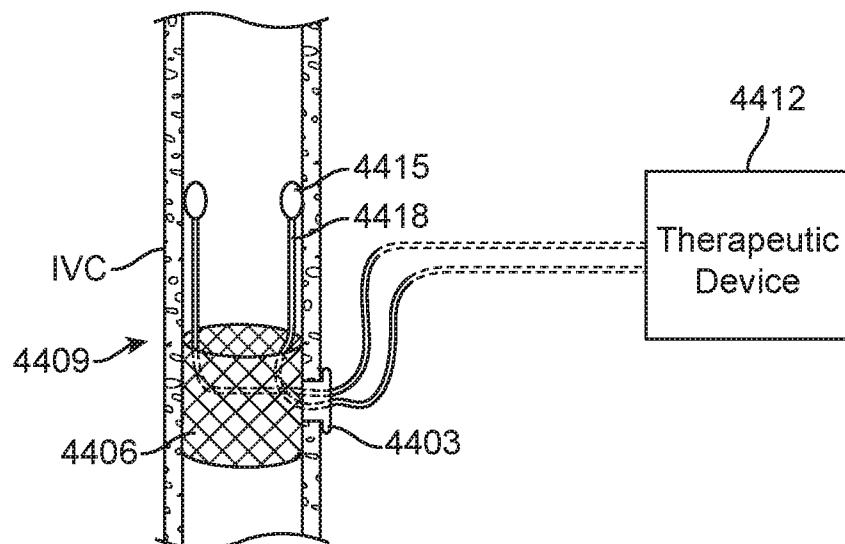


FIG. 44

37 / 39

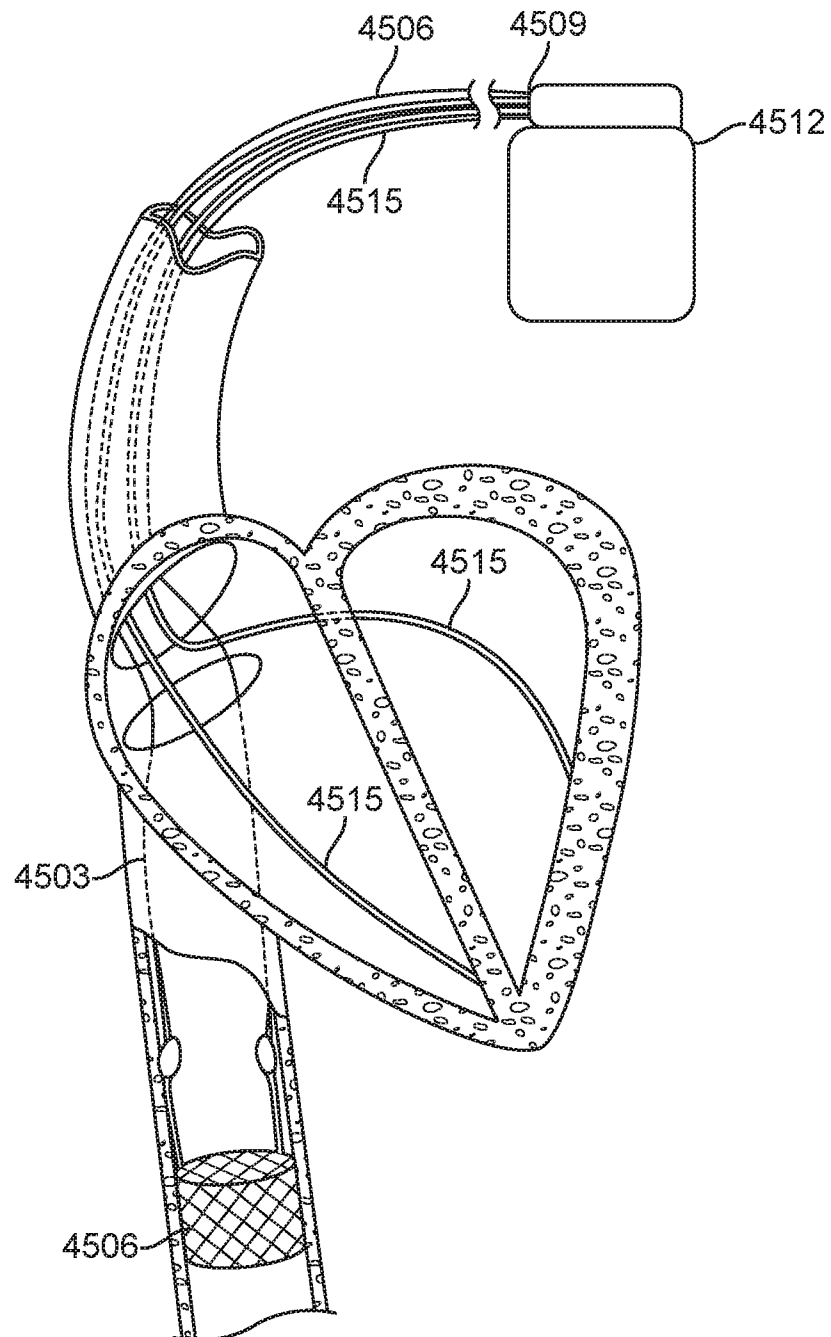
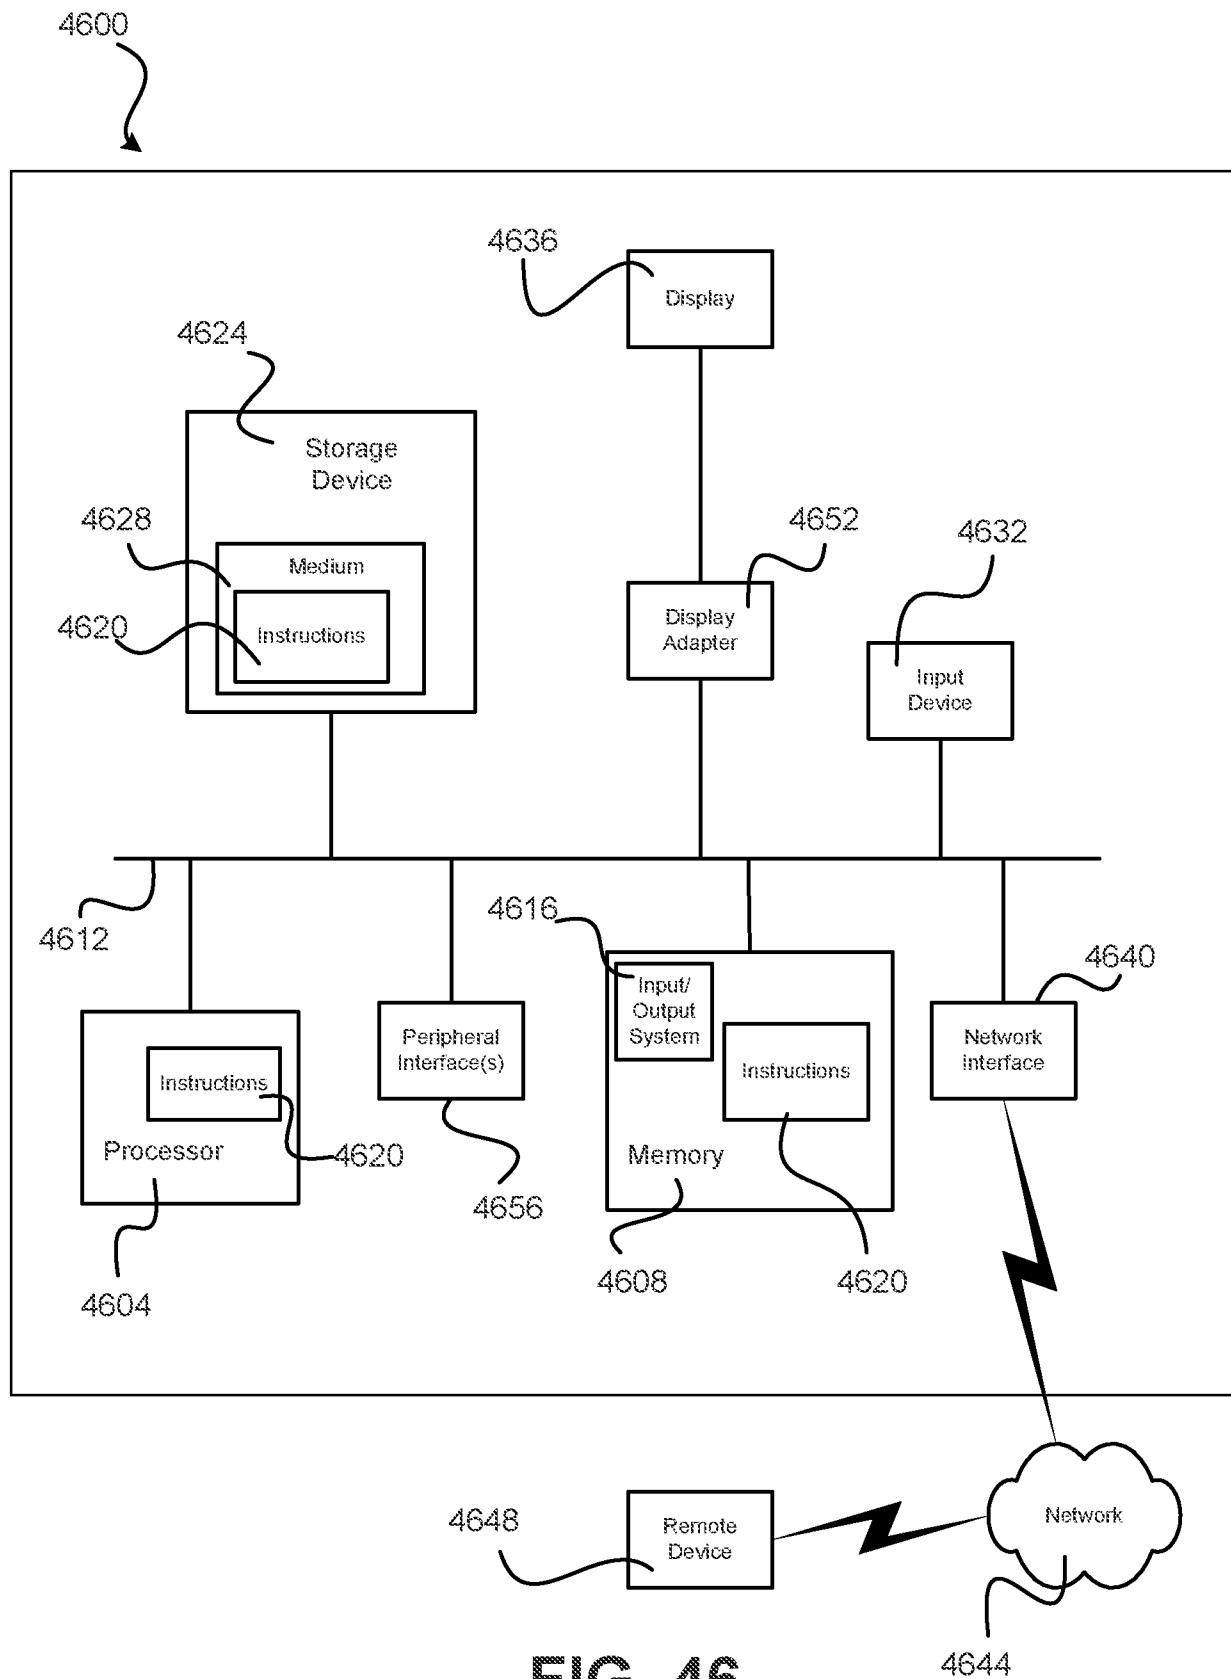


FIG. 45

38/39



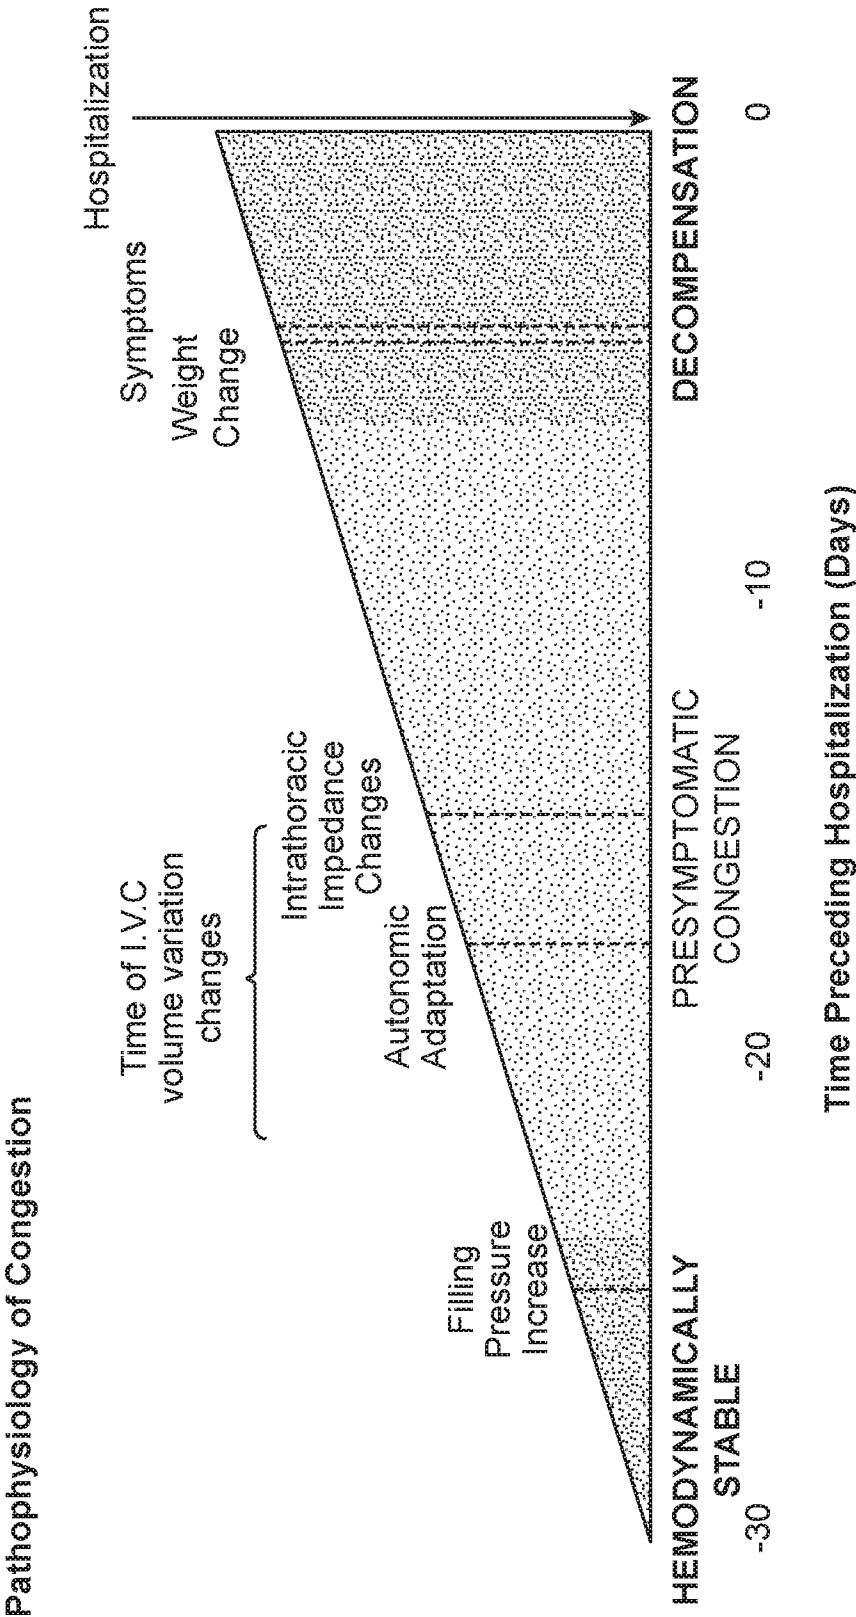


FIG. 47

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2016/017902

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61B5/107 A61B5/00
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 205 292 A (CZAR CARL T [US] ET AL) 27 April 1993 (1993-04-27) column 3, line 31 - line 34; figures 3,6 -----	1,10-43
X	US 5 339 816 A (AKAMATSU SHIGERU [JP] ET AL) 23 August 1994 (1994-08-23) column 9, line 56 - column 10, line 17; figure 8 -----	1
A	US 2010/324432 A1 (BJOERLING ANDERS [SE] ET AL) 23 December 2010 (2010-12-23) paragraph [0027] -----	1-43
A	DE 10 2005 035022 A1 (UNIVERSITAETSKLINIKUM FREIBURG [DE]) 23 November 2006 (2006-11-23) paragraphs [0011], [0012], [0013], [0014], [0015], [0021] -----	1-43



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

9 May 2016

Date of mailing of the international search report

27/07/2016

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Knüpling, Moritz

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2016/017902

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 71-97
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:
1-43

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International Application No. PCT/ US2016/ 017902

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-43

Implantable device

2. claims: 44, 45, 68-70

Implantable device comprising wireless transmitting and receiving feature

3. claims: 46-67, 98-105

Implantable device having delivery device and external detecting means

4. claim: 106

Implantable device having first and second arms

5. claims: 107-110

Therapeutic system based on vena cava dimension measurements

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2016/017902

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5205292	A	27-04-1993	AU 2177892 A 08-01-1993
		CA 2103237 A1 04-12-1992	
		DE 69230826 D1 27-04-2000	
		DE 69230826 T2 19-10-2000	
		EP 0602048 A1 22-06-1994	
		JP H06510443 A 24-11-1994	
		US 5205292 A 27-04-1993	
		US 5284146 A 08-02-1994	
		WO 9221284 A1 10-12-1992	

US 5339816	A	23-08-1994	DE 69228974 D1 27-05-1999
		DE 69228974 T2 26-08-1999	
		DE 69229802 D1 16-09-1999	
		DE 69229802 T2 20-01-2000	
		EP 0538885 A1 28-04-1993	
		EP 0670146 A1 06-09-1995	
		US 5339816 A 23-08-1994	

US 2010324432	A1	23-12-2010	EP 2117639 A1 18-11-2009
		US 2010324432 A1 23-12-2010	
		WO 2008103077 A1 28-08-2008	

DE 102005035022	A1	23-11-2006	DE 102005035022 A1 23-11-2006
		WO 2006122750 A1 23-11-2006	
