



US0D1082007S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,082,007 S**  
**Prutchi et al.** (45) **Date of Patent:** **\*\* Jul. 1, 2025**

(54) **CHARGER FOR IMPLANTABLE CARDIAC DEVICE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Impulse Dynamics NV**, Willemstad (CW)

CN	304159820	*	6/2017
CN	307626015	*	10/2022
EM	008874259-0001	*	3/2022
KR	301182885.0000	*	9/2022

(72) Inventors: **David Prutchi**, Voorhees, NJ (US);  
**Jason Meyers**, Haddonfield, NJ (US)

OTHER PUBLICATIONS

(73) Assignee: **Impulse Dynamics NV**, Willemstad (CW)

Patient Manual for the AIM HIGHER Clinical Trial, posted Aug. 8, 2021 [retrieved online Dec. 6, 2023]. Retrieved from internet, <https://tinyurl.com/OPTIMIZER-smart-system> (Year: 2021).\*  
CCM Information—Global—Impulse Dynamics, posted date unavailable [retrieved online Dec. 6, 2023]. Retrieved from internet, <https://impulse-dynamics.com/global/ccm-information/> (Year: 2023).\*

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/828,978**

(Continued)

(22) Filed: **Mar. 2, 2022**

*Primary Examiner* — Justin M Jonaitis

(51) **LOC (15) Cl.** ..... **24-02**

*Assistant Examiner* — Samantha K Pollack

(52) **U.S. Cl.**

USPC ..... **D24/167**

(58) **Field of Classification Search**

USPC ..... D24/112, 127–129, 164, 166, 167, 169,  
D24/170, 184, 186, 216, 231; D10/75

CPC ..... A61N 1/046; A61N 1/05; A61N 1/37512;  
A61N 1/39; A61N 1/3937; A61N 1/3956

See application file for complete search history.

(57) **CLAIM**

The ornamental design for a charger for implantable cardiac device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a charger for implantable cardiac device, showing our new design;

FIG. 2 is a rear view thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof;

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

The broken lines in the drawing illustrate portions of the charger for implantable cardiac device that form no part of the claimed design.

The oblique lines in the drawings indicate transparency.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D479,877	S *	9/2003	Lee	.....	D24/186
D484,246	S *	12/2003	Lee	.....	D24/186
D609,813	S *	2/2010	Molden	.....	D24/167
D718,867	S *	12/2014	Schroderus	.....	D24/167
8,929,986	B2 *	1/2015	Parker	.....	H02J 7/0042 607/36
D782,682	S *	3/2017	Jung	.....	D24/167
D783,832	S *	4/2017	Dascoli	.....	D24/167
D811,598	S *	2/2018	Baek	.....	D24/167
11,011,801	B2 *	5/2021	Deininger	.....	H01M 50/50

**1 Claim, 7 Drawing Sheets**



(56)

**References Cited**

OTHER PUBLICATIONS

Resonant Link Wireless Charging, posted Jun. 9, 2021 [retrieved online Dec. 6, 2023]. Retrieved from internet, <https://www.resonant-link.com/newsroom/resonant-link-brings-efficient-wireless-charging-to-the-medical-device-industry> (Year: 2021).\*

How to charge your system—Boston Scientific, posted date unavailable [retrieved online Jun. 9, 2023]. Retrieved from internet, <https://www.bostonscientific.com/en-US/patients-caregivers/device-support/scs/system-charging.html> (Year: 2023).\*

Impulse Dynamics Vesta Charging System User Guide, posted date unavailable [retrieved online Dec. 6, 2023]. Retrieved from internet, <https://device.report/manual/4397606> (Year: 2023).\*

\* cited by examiner

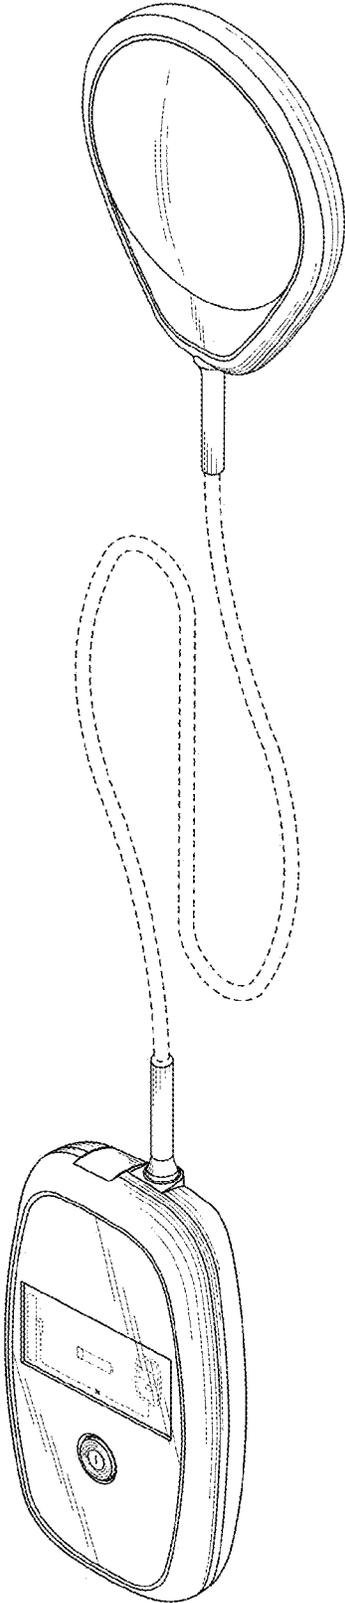


FIG. 1

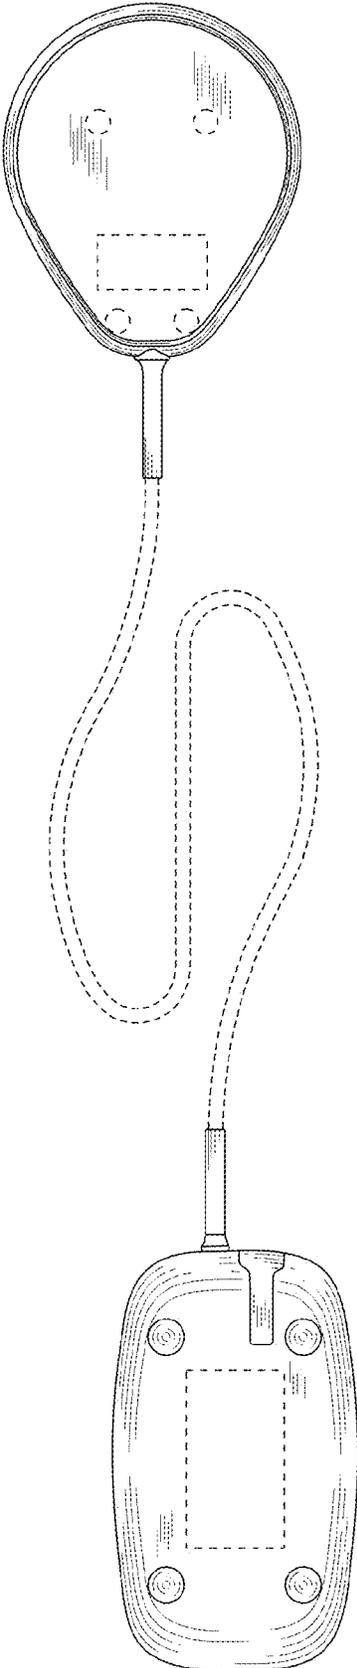


FIG. 2

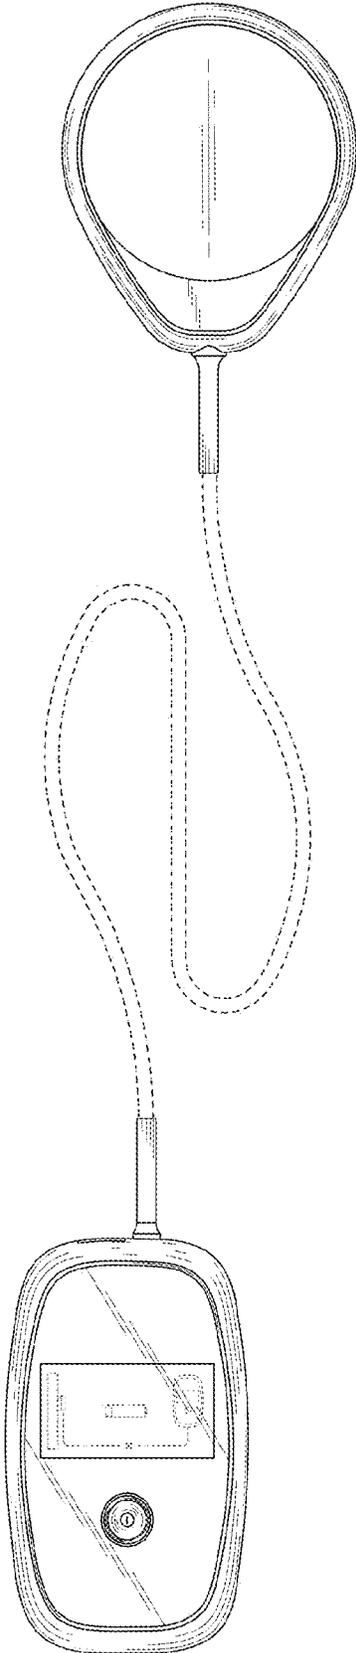


FIG. 3



FIG. 4




FIG. 5



FIG. 6




FIG. 7