



(51) International Patent Classification:

B01D 21/28 (2006.01) *G01N 29/22* (2006.01)
B03B 1/04 (2006.01) *G01N 15/14* (2006.01)
A61M 1/36 (2006.01) *B01L 3/00* (2006.01)

(21) International Application Number:

PCT/US2016/037104

(22) International Filing Date:

11 June 2016 (11.06.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/174,512 11 June 2015 (11.06.2015) US

(71) Applicant: **FLODESIGN SONICS, INC.** [US/US]; 380 Main Street, Wilbraham, MA 01095 (US).

(72) Inventors: **GILMANSHIN, Rudolf**; 380 Main Street, Wilbraham, MA 01095 (US). **LIPKENS, Bart**; 380 Main Street, Wilbraham, MA 01095 (US).

(74) Agent: **KLEIN, Richard, M.**; Fay Sharpe LLP, 1228 Euclid Avenue, 5th Floor, Cleveland, OH 44115-1843 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— without international search report and to be republished upon receipt of that report (Rule 48.2(g))

(54) Title: ACOUSTIC METHODS FOR SEPARATION CELLS AND PATHOGENS

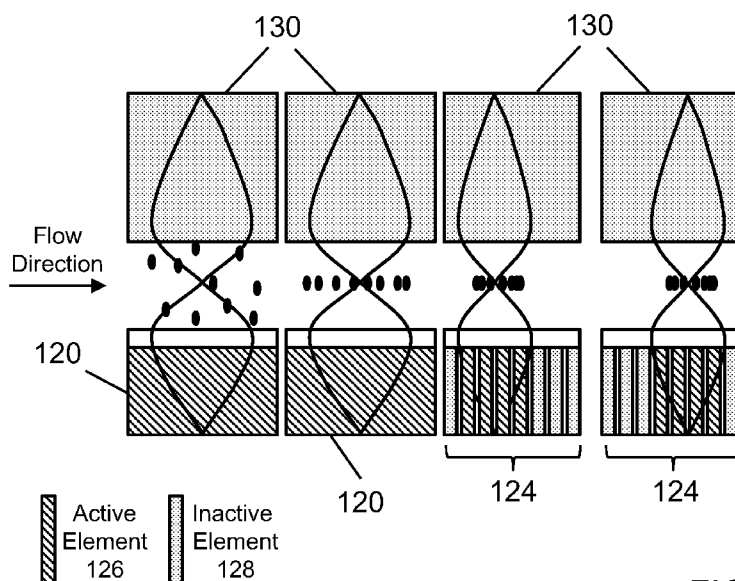


FIG. 2

(57) Abstract: Devices and methods for inspecting, detecting, isolating, monitoring, characterizing, or separating pathogens in blood containing blood cells are disclosed. The devices include a flow chamber having a solvent inlet, at least one host-fluid inlet, a particulate outlet, at least one residual outlet, and a reflector. The methods include trapping the pathogens in the acoustic standing wave, introducing a solvent into the flow chamber, and removing the pathogens from the device. Devices and methods for inspecting, detecting, isolating, monitoring, characterizing, or separating specialized circulating cells in blood containing blood cells are also disclosed. The devices include a flow chamber having at least one inlet and at least one outlet, and a microscope objective and a cover glass. The methods include driving the transducer to create an acoustic standing wave in the flow chamber and micro-bubbles in the blood.

ACOUSTIC METHODS FOR SEPARATION OF CELLS AND PATHOGENS

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to U.S. Provisional Patent Application Serial No. 62/174,512, filed on June 11, 2015, the disclosure of which is hereby fully incorporated by reference in its entirety.

BACKGROUND

[0002] The identification and separation of specialized circulating cells, such as circulating tumor cells (CTCs) or pathogenic cells such as *Escherichia coli* (*E. coli*) is very desirable for advancing the knowledge of cancer types, for diagnostics, and for monitoring the progress of cancer treatments.

[0003] One conventional method of identifying and separating specialized circulating cells utilizes different fluorescent materials to tag different cells based on their specific surface chemistry. The cells are then sorted based on their different fluorescent colors. This method, however, attaches secondary molecules to the cell of interest and may modify the surface characteristics of the cells, which is undesirable. Other methods of locating rare cells in circulation involve video or microscopy techniques, which are painstaking and very time-consuming processes.

[0004] Diagnostic applications for specialized circulating cells typically require the ability to be used with small analysis volumes. In addition, reagents for such applications are very expensive. Because only a small number of target cells are contained in the specimen and they are at low concentrations, high sensitivity (i.e. the ability to correctly identify the target cells) and high specificity (i.e. the ability to correctly identify cells that are not the target cells) are desirable.

[0005] It would therefore be desirable to provide methods for both identification and segmentation or separation of rare cell types for both diagnostic and treatment purposes. A ready-to-operate system for both identification and segmentation or separation of rare cell types for both diagnostic and treatment purposes is likewise desirable. Diagnostic systems and methods that enhance sensitivity are desirable, in

addition to systems and method with high specificity, as incorrect identification causes incorrect or unnecessary treatment.

BRIEF DESCRIPTION

[0006] The present disclosure relates, in various embodiments, to systems and methods of identification and separation of target cells such as specialized circulating cells and/or rare cell types, such as pathogenic cells, utilizing acoustic manipulation via acoustic standing waves. These systems and methods are useful for various diagnostic and treatment purposes, including pathogen detection in blood, and trapping and characterization of specialized circulating cells, such as CTCs. Briefly, the use of an acoustic standing allows for contact-free manipulation of cells, thereby increasing sensitivity because of the elimination of contact with surfaces, which are the main channel of losses of cells and reagents. Additionally, acoustic manipulation allows for high local concentrations of analytes at large microfluidic volumes, which enhances sensitivity, lowers costs, and simplifies the design. Finally, the acoustic manipulation systems and methods described herein advantageously possess the potential for automation of the manipulation of particles or cells through the combination of fluid flows and acoustic pressure using an acoustic standing wave.

[0007] In accordance with the present disclosure, methods are disclosed for inspecting, detecting, isolating, monitoring, characterizing, or separating pathogens from a fluid (e.g. in blood or its derivatives, containing blood cells). The method comprises flowing the fluid containing the pathogens through an acoustic manipulation device. The fluid may be diluted, such as up to ten times its original concentration. The fluid may also be stratified through the use of a centrifuge and then separated prior to introduction into the acoustic separation device. The stratified layers may be treated separately. For example, in blood, one typically stratified layer is known as the “buffy coat” and contains the white cells and platelets in the blood sample. The white cells are neutrophils, eosinophils, basophils, lymphocytes, and monocytes. The lymphocytes can contain T cells, B cells and NK cells. The acoustic manipulation device comprises a flow chamber having a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and a particulate outlet and at least one residual outlet at a second end of the flow

chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis; at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and a reflector located on a wall on the opposite side of the flow chamber from the at least one ultrasonic transducer. The flow chamber may alternatively be shaped to form a resonant chamber. The method further comprises sending a voltage signal to drive the at least one ultrasonic transducer to create the acoustic standing wave in the flow chamber to drive the pathogens toward the longitudinal axis where the pathogens become trapped in the acoustic standing wave; introducing a solvent into the flow chamber through the solvent inlet; and removing the pathogens from the device through the particulate outlet.

[0008] In particular embodiments, the acoustic manipulation device further comprises at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet. The method may further comprise introducing a buffer into the flow chamber through the at least one buffer inlet, the buffer creating a buffer layer that permits the pathogens to pass therethrough but destroys other cells as they pass therethrough. The buffer can be a selective lytic buffer (e.g., mild detergents). Alternatively, an osmotic shock can be employed to create the buffer layer. If cells (e.g., mammalian cells) are passed through a solvent having a low salt concentration, the cells are generally caused to explode while the bacteria survives due to its cellular walls. Note that for acoustical purposes, the change of the density due to the decrease of salt concentration could be compensated with agents that can increase the solvent density without changing its osmolality (e.g., Ficoll, Histodenz).

[0009] The method may further comprise removing the solvent from the device through the residual outlet. The solvent may be a bacteria-friendly solvent (e.g., saline, culture broth).

[0010] In certain constructions, the piezoelectric material can include a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements operated between active and inactive modes such that the pathogens are trapped

above the piezoelectric elements in the active mode. The method may further comprise switching the piezoelectric elements between the active and inactive modes to move the pathogens trapped in the acoustic standing wave along the longitudinal axis from the first end to the second end of the flow chamber to the particulate outlet.

[0011] According to the present disclosure, another method is disclosed for inspecting, detecting, isolating, or characterizing specialized circulating cells (e.g., CTCs, stem cells, CAR T cells) in a host fluid containing the targeted cells (e.g. blood containing blood cells). The method comprises flowing the host fluid containing the targeted cells through an acoustic manipulation device. The acoustic manipulation device comprises a flow chamber having at least one inlet and at least one outlet; at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and a transparent wall forming a wall of the flow chamber opposite the at least one ultrasonic transducer. In certain embodiments, a cover glass may be required for high-resolution, high-sensitivity detection employing oil-immersed objectives. In other embodiments, objectives with lower magnification and long working distance may not require a cover glass. The method further comprises sending a voltage signal to drive the at least one ultrasonic transducer to create the acoustic standing wave in the flow chamber, and attaching acoustically active particles (e.g., microbubbles or paramagnetic particles having an affinity ligand attached) to the specialized circulating cells, the acoustically active particles being driven by the acoustic standing wave toward the transparent wall where the specialized circulating cells and attached microbubbles become trapped in the acoustic standing wave. A microscope objective is used to examine the cells through the transparent wall.

[0012] In particular embodiments, the at least one inlet includes a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and the at least one outlet includes a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis.

[0013] The acoustic manipulation device may further comprise at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet. The method may further comprise introducing a dividing buffer into the flow chamber through the at least one buffer inlet. A substantially acoustically transparent layer may be present between the cover glass and the flow chamber. The substantially acoustically transparent layer can include one or more wells therein.

[0014] The piezoelectric material may include a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements configured to operate between active and inactive modes such that the targeted cells are trapped above the piezoelectric elements in the active mode. The method may further comprise switching the piezoelectric elements between the active and inactive modes to position the targeted cells trapped in the acoustic standing wave in alignment with the microscope objective. The substantially acoustically transparent layer can include one or more wells therein. The method may further comprise switching the piezoelectric elements between the active and inactive modes to position the targeted cells trapped in the acoustic standing wave in the wells of the substantially acoustically transparent layer.

[0015] The targeted cells can be specialized circulating cells, such as circulating tumor cells.

[0016] Acoustophoretic devices are also disclosed. In one embodiment, an acoustophoretic device comprises a flow chamber having a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis; at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and a reflector located on a wall on the opposite side of the flow chamber from the at least one ultrasonic transducer.

[0017] In particular embodiments, the acoustophoretic device further comprises at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet.

[0018] The piezoelectric material may include a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements configured to operate between active and inactive modes.

[0019] The flow chamber can be disposable.

[0020] In certain constructions, the at least one ultrasonic transducer comprises a housing having a top end, a bottom end, and an interior volume; and a piezoelectric crystal at the bottom end of the housing having an exposed exterior surface and an interior surface, the crystal being able to vibrate when driven by a voltage signal. In some embodiments, no backing layer is present within the housing of the at least one ultrasonic transducer, and an air gap is present in the interior volume between the crystal and a top plate at the top end of the housing. In other embodiments, the at least one ultrasonic transducer further comprises a backing layer contacting the interior surface of the crystal, the backing layer being made of a substantially acoustically transparent material.

[0021] In a second embodiment, an acoustophoretic device comprises a flow chamber having at least one inlet and at least one outlet; at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and a transparent wall forming a portion of the flow chamber opposite the at least one ultrasonic transducer. The flow chamber may also or alternatively include a transducer and a resonant chamber, with no specific reflector component opposite the transducer.

[0022] In particular embodiments, the at least one inlet includes a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and the at least one outlet includes a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis.

[0023] The acoustophoretic device may further comprise at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet. A substantially acoustically transparent layer may be present between the transparent wall and the interior volume of the flow chamber.

[0024] The piezoelectric material may include a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements configured to operate between active and inactive modes.

[0025] The flow chamber can be disposable.

[0026] In certain constructions, the at least one ultrasonic transducer comprises a housing having a top end, a bottom end, and an interior volume; and a piezoelectric crystal at the bottom end of the housing having an exposed exterior surface and an interior surface, the crystal being able to vibrate when driven by a voltage signal. In some embodiments, no backing layer is present within the housing of the at least one ultrasonic transducer, and an air gap is present in the interior volume between the crystal and a top plate at the top end of the housing. In other embodiments, the at least one ultrasonic transducer further comprises a backing layer contacting the interior surface of the crystal, the backing layer being made of a substantially acoustically transparent material.

[0027] In particular embodiments of the methods and devices according to the present disclosure, the acoustic standing wave may be a multi-dimensional acoustic standing wave. Examples of such multi-dimensional acoustic standing waves can be found in commonly owned U.S. Patent No. 9,228,183, the entire contents being hereby fully incorporated by reference. In other embodiments of the methods and devices according to the present disclosure, the acoustic standing wave can be a planar acoustic standing wave. Further yet, in particular embodiments, the acoustic standing wave may be a combination of a planar acoustic standing wave and a multi-dimensional acoustic standing wave, where the planar acoustic standing wave and multidimensional acoustic standing wave are super positioned on each other.

[0028] These and other non-limiting characteristics are more particularly described below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0029] The following is a brief description of the drawings, which are presented for the purposes of illustrating the exemplary embodiments disclosed herein and not for the purposes of limiting the same.

[0030] **FIG. 1** is a plan view of a first exemplary embodiment of an acoustophoretic device according to the present disclosure. The device includes a flow chamber having a solvent inlet, at least one host-fluid inlet, a particulate outlet, at least one residual outlet, and at least one buffer inlet.

[0031] **FIG. 2** illustrates several exemplary transducer-reflector arrangements according to the present disclosure.

[0032] **FIG. 3** illustrates an acoustic concentrator according to the present disclosure.

[0033] **FIG. 4** is a plan view of a second exemplary embodiment of an acoustophoretic device according to the present disclosure. The device includes a transducer located opposite an acoustically transparent layer and an optically transparent wall. A microscope objective can examine cells within the flow chamber of the device through the optically transparent wall.

[0034] **FIG. 5** is a plan view of the acoustophoretic device of **FIG. 4**. The transducer includes a plurality of piezoelectric elements arranged in an array and configured to operate between active and inactive modes.

[0035] **FIG. 6** is a plan view of the acoustophoretic device of **FIG. 5**. The acoustically transparent layer includes several wells therein, and the piezoelectric elements are switched between active and inactive modes to position targeted cells in the wells.

[0036] **FIG. 7** is a plan view showing one method of the present disclosure. Here, a host fluid is flowed into the flow chamber. Acoustically active particles are attached to target cells. Acoustic standing waves are used to separate the particle-cell complex from the host fluid and other cells, and the particle-cell complex exits from the desired particulate outlet.

[0037] **FIG. 8** is a cross-sectional diagram of a conventional ultrasonic transducer.

[0038] FIG. 9 is a cross-sectional diagram of an ultrasonic transducer according to the present disclosure. An air gap is present within the transducer, and no backing layer or wear plate is present.

[0039] FIG. 10 is a cross-sectional diagram of an ultrasonic transducer according to the present disclosure. An air gap is present within the transducer, and a backing layer and wear plate are present.

DETAILED DESCRIPTION

[0040] The present disclosure may be understood more readily by reference to the following detailed description of desired embodiments and the examples included therein. In the following specification and the claims which follow, reference will be made to a number of terms which shall be defined to have the following meanings.

[0041] Although specific terms are used in the following description for the sake of clarity, these terms are intended to refer only to the particular structure of the embodiments selected for illustration in the drawings, and are not intended to define or limit the scope of the disclosure. In the drawings and the following description below, it is to be understood that like numeric designations refer to components of like function.

[0042] The singular forms "a," "an," and "the" include plural referents unless the context clearly dictates otherwise.

[0043] The term "comprising" is used herein as requiring the presence of the named component and allowing the presence of other components. The term "comprising" should be construed to include the term "consisting of", which allows the presence of only the named component, along with any impurities that might result from the manufacture of the named component.

[0044] Numerical values should be understood to include numerical values which are the same when reduced to the same number of significant figures and numerical values which differ from the stated value by less than the experimental error of conventional measurement technique of the type described in the present application to determine the value.

[0045] All ranges disclosed herein are inclusive of the recited endpoint and independently combinable (for example, the range of "from 2 grams to 10 grams" is

inclusive of the endpoints, 2 grams and 10 grams, and all the intermediate values). The endpoints of the ranges and any values disclosed herein are not limited to the precise range or value; they are sufficiently imprecise to include values approximating these ranges and/or values.

[0046] The modifier “about” used in connection with a quantity is inclusive of the stated value and has the meaning dictated by the context. When used in the context of a range, the modifier “about” should also be considered as disclosing the range defined by the absolute values of the two endpoints. For example, the range of “from about 2 to about 10” also discloses the range “from 2 to 10.” The term “about” may refer to plus or minus 10% of the indicated number. For example, “about 10%” may indicate a range of 9% to 11%, and “about 1” may mean from 0.9-1.1.

[0047] It should be noted that many of the terms used herein are relative terms. For example, the terms “upper” and “lower” are relative to each other in location, i.e. an upper component is located at a higher elevation than a lower component in a given orientation, but these terms can change if the device is flipped. The terms “inlet” and “outlet” are relative to a fluid flowing through them with respect to a given structure, e.g. a fluid flows through the inlet into the structure and flows through the outlet out of the structure. The terms “upstream” and “downstream” are relative to the direction in which a fluid flows through various components, i.e. the flow fluids through an upstream component prior to flowing through the downstream component. It should be noted that in a loop, a first component can be described as being both upstream of and downstream of a second component.

[0048] The terms “horizontal” and “vertical” are used to indicate direction relative to an absolute reference, i.e. ground level. However, these terms should not be construed to require structures to be absolutely parallel or absolutely perpendicular to each other. For example, a first vertical structure and a second vertical structure are not necessarily parallel to each other. The terms “top” and “bottom” or “base” are used to refer to surfaces where the top is always higher than the bottom/base relative to an absolute reference, i.e. the surface of the earth. The terms “upwards” and “downwards” are also relative to an absolute reference; upwards is always against the gravity of the earth.

[0049] The term “parallel” should be construed in its lay sense of two surfaces that maintain a generally constant distance between them, and not in the strict mathematical sense that such surfaces will never intersect when extended to infinity.

[0050] The present application refers to “the same order of magnitude.” Two numbers are of the same order of magnitude if the quotient of the larger number divided by the smaller number is a value of at least 1 and less than 10.

[0051] Acoustophoresis is the separation of particles and secondary fluids from a primary or host fluid using high intensity acoustic standing waves, and without the use of membranes or physical size exclusion filters. It has been known that high intensity standing waves of sound can exert forces on particles in a fluid when there is a differential in both density and/or compressibility, otherwise known as the acoustic contrast factor. The pressure profile in a standing wave contains areas of local minimum pressure amplitudes at its nodes and local maxima at its anti-nodes. Depending on the density and compressibility of the particles, they will be trapped at the nodes or anti-nodes of the standing wave. Generally, the higher the frequency of the standing wave, the smaller the particles that can be trapped due the pressure of the standing wave.

[0052] When acoustic standing waves propagate in liquids, the fast oscillations may generate a non-oscillating force on particles suspended in the liquid or on an interface between liquids. This force is known as the acoustic radiation force. The force originates from the non-linearity of the propagating wave. As a result of the non-linearity, the wave is distorted as it propagates and the time-averages are nonzero. By serial expansion (according to perturbation theory), the first non-zero term will be the second-order term, which accounts for the acoustic radiation force. The acoustic radiation force on a particle, or a cell, in a fluid suspension is a function of the difference in radiation pressure on either side of the particle or cell. The physical description of the radiation force is a superposition of the incident wave and a scattered wave, in addition to the effect of the non-rigid particle oscillating with a different speed compared to the surrounding medium thereby radiating a wave. The following equation presents an analytical expression for the acoustic radiation force on a particle, or cell, in a fluid suspension in a planar standing wave.

$$F_R = \frac{3\pi P_0^2 V_p \beta_m}{2\lambda} \varphi(\beta, \rho) \sin(2kx) \quad (1)$$

where β_m is the compressibility of the fluid medium, ρ is density, φ is acoustic contrast factor, V_p is particle volume, λ is wavelength, k is $2\pi/\lambda$, P_0 is acoustic pressure amplitude, x is the axial distance along the standing wave (i.e., perpendicular to the wave front), and

$$\varphi(\beta, \rho) = \frac{5\rho_p - 2\rho_m}{2\rho_p + \rho_m} - \frac{\beta_p}{\beta_m}$$

where ρ_p is the particle density, ρ_m is the fluid medium density, β_p is the compressibility of the particle, and β_m is the compressibility of the fluid medium.

[0053] For a multi-dimensional standing wave, the acoustic radiation force is a three-dimensional force field, and one method to calculate the force is Gor'kov's method, where the primary acoustic radiation force F_R is defined as a function of a field potential U , $F_V = -\nabla(U)$, where the field potential U is defined as

$$U = V_0 \left[\frac{\langle p^2(x, y, t) \rangle}{2\rho_f c_f^2} f_1 - \frac{3\rho_f \langle v^2(x, y, t) \rangle}{4} f_2 \right]$$

and f_1 and f_2 are the monopole and dipole contributions defined by

$$f_1 = 1 - \frac{1}{\Lambda \sigma^2} \quad f_2 = \frac{2(\Lambda - 1)}{2\Lambda + 1},$$

where

$$\sigma = \frac{c_p}{c_f} \quad \Lambda = \frac{\rho_p}{\rho_f} \quad \beta_f = \frac{1}{\rho_f c_f^2}$$

where p is the acoustic pressure, u is the fluid particle velocity, Λ is the ratio of cell density ρ_p to fluid density ρ_f , σ is the ratio of cell sound speed c_p to fluid sound speed c_f ,

V_0 is the volume of the cell, and $\langle \rangle$ indicates time averaging over the period of the wave.

[0054] The present disclosure relates to acoustophoretic devices and methods that employ multi-dimensional ultrasonic acoustic standing waves, planar acoustic standing waves or combinations of planar and multidimensional acoustic standing waves (collectively referred to herein simple as acoustic standing waves) to separate cells and/or other particles from the fluid surrounding them. This can be useful for diagnostic applications.

[0055] The acoustophoretic or acoustically active devices of the present disclosure can be used for the extraction of bacteria from a mixture of bacteria and cells (e.g., mammalian cells). Examples of other applications of the acoustophoretic devices of the present disclosure include detecting contamination of cell cultures or for separation of impurities from fluids in the food and beverage industry. The acoustophoretic or acoustically active devices of the present disclosure can also be used to diagnose and treat blood infections. For example, a volume of blood (e.g., 10 milliliters) drained from a patient can be split into two separate samples for bacteria and yeast detection. Half of the blood is then injected into an appropriate culture bottle and submitted to a blood culturing system (e.g., BACTEC) for growth. Once the pathogens in the blood grow to sufficient concentration, a sample aliquot is then analyzed by a matrix-assisted laser desorption / ionization time-of-flight mass spectrometer (MALDI-TOF MS). The typical pathogen concentration is about one to two pathogens per milliliter. Thus, for a five milliliter blood sample in a 50 milliliter bottle, the sample begins with about five to ten pathogens. Growth in the blood culturing system is generally complete at about 10^6 to about 10^7 pathogens per milliliter, which takes about 20 to 24 generations, or about 10 to 12 hours. Generally, the volume of sample required for mass spectrometry is about 1 microliter. Time-to-answer is critical in blood infections, because the more developed sepsis becomes, the more difficult it is to treat the infection, and the progressing bacteremia can induce septic shock.

[0056] **FIGS. 1-5** illustrate various embodiments of acoustophoretic devices according to the present disclosure.

[0057] In particular, **FIG. 1** illustrates a first exemplary embodiment of an acoustophoretic device **100**. The device **100** includes a flow chamber **110**, at least one ultrasonic transducer **120**, and a reflector **130**.

[0058] The flow chamber **110** is the region of the device **100** through which is flowed the fluid sample, containing both mammalian and bacterial cells (e.g., blood containing blood cells and bacteria, yeast, or specialized circulating cells), or more generally, the host fluid contains both target cells (to be separated from the host fluid) and non-target cells (which are to remain with the host fluid). The flow chamber **110** includes a solvent inlet **112**, at least one host-fluid inlet **114**, a particulate outlet **116**, at least one residual outlet **118**, and at least one buffer inlet **119**.

[0059] The solvent inlet **112**, the at least one host-fluid inlet **114**, and the at least one buffer inlet **119** are located at a first end **111** of the flow chamber **110**. The at least one buffer inlet **119** is located between the solvent inlet **112** and the at least one host-fluid inlet **114**. The particulate outlet **116** and the at least one residual outlet **118** are located at a second end **113** of the flow chamber **110**. As seen in **FIG. 1**, the first end **111** of the flow chamber **110** is opposite the second end **113** of the flow chamber **110**. As can also be seen from **FIG. 1**, the solvent inlet **112** and the particulate outlet **116** are aligned with a longitudinal axis **115** of the flow chamber **110**, and the at least one host-fluid inlet **114**, the at least one buffer inlet **119**, and the at least one residual outlet **118** are spaced apart from the longitudinal axis **115**.

[0060] In the embodiment of **FIG. 1**, the device **100** includes one solvent inlet **112**, two host-fluid inlets **114**, a particulate outlet **116**, two residual outlets **118**, and two buffer inlets **119**. In this regard, it is noted that the flow chamber **110** of device **100** is reflectionally symmetrical about the longitudinal axis **115**.

[0061] The ultrasonic transducer **120** of the device **100** is located on wall **122** of the flow chamber **110**. The reflector **130** of the device **100** is located on wall **132** of the flow chamber **110**. As seen in **FIG. 1**, wall **132** is located on the opposite side of the flow chamber **110** from wall **122**, such that the reflector **130** is located on an opposite side of the flow chamber **110** from the ultrasonic transducer **120**. In this way, one or more acoustic standing waves are created in the flow chamber between the ultrasonic transducer and the reflector. Each node of the acoustic standing wave(s) is generally

sheathed with layers of the solvent, such that the number of acoustic standing waves created in the flow chamber may correspond to the number of outlets of the device.

[0062] Prior to discussing further optimization of the systems, it is helpful to provide an explanation now of how multi-dimensional acoustic standing waves are generated. The multi-dimensional acoustic standing wave is obtained by driving an ultrasonic transducer at a frequency that both generates the acoustic standing wave and excites a fundamental 3D vibration mode of the transducer piezoelectric element. Perturbation of the piezoelectric element in an ultrasonic transducer in a multimode fashion allows for generation of a multidimensional acoustic standing wave. A piezoelectric element can be specifically designed to deform in a multimode fashion at designed frequencies, allowing for generation of a multi-dimensional acoustic standing wave. The multi-dimensional acoustic standing wave may be generated by distinct modes of the piezoelectric element such as a 3x3 mode that would generate multidimensional acoustic standing waves. A multitude of multidimensional acoustic standing waves may also be generated by allowing the piezoelectric element to vibrate through many different mode shapes. Thus, the element would excite multiple modes such as a 0x0 mode (i.e. a piston mode) to a 1x1, 2x2, 1x3, 3x1, 3x3, and other higher order modes and then cycle back through the lower modes of the element (not necessarily in straight order). This switching or dithering of the element between modes allows for various multi-dimensional wave shapes, along with a single piston mode shape, to be generated over a designated time.

[0063] It is also possible to excite or choose a frequency of excitation that excites multiple modes at the same time, each mode with a varying degree of displacement amplitude. Through this combination of multiple modes excited at the same time with varying displacement amplitude, it is possible to generate a superposition of multi-dimensional standing waves desirable for trapping, clustering, and separation of a secondary fluid or particle from a host fluid.

[0064] The scattering of the acoustic field off the particles results in a three dimensional acoustic radiation force, which acts as a three-dimensional trapping field. The acoustic radiation force is proportional to the particle volume (e.g. the cube of the radius) when the particle is small relative to the wavelength. It is proportional to

frequency and the acoustic contrast factor. It also scales with acoustic energy (e.g. the square of the acoustic pressure amplitude). When the acoustic radiation force exerted on the particles is stronger than the combined effect of fluid drag force and buoyancy and gravitational force, the particles are trapped within the acoustic standing wave field. This can result in the concentration, agglomeration and/or coalescence of the trapped particles depending on the type of acoustic standing wave that is utilized. Relatively large solids of one material can thus be separated from smaller particles of a different material, the same material, and/or the host fluid through enhanced gravitational separation.

[0065] The multi-dimensional standing wave generates acoustic radiation forces in both the axial direction (i.e., in the direction of the standing wave, between the transducer and the reflector, perpendicular to the flow direction) and the lateral direction (i.e., in the flow direction). As the mixture flows through the acoustic chamber, particles in suspension experience a strong axial force component in the direction of the standing wave. Since this acoustic force is perpendicular to the flow direction and the drag force, it quickly moves the particles to pressure nodal planes or anti-nodal planes, depending on the contrast factor of the particle. The lateral acoustic radiation force then acts to move the concentrated particles towards the center of each planar node, resulting in agglomeration or clumping. The lateral acoustic radiation force component has to overcome fluid drag for such clumps of particles to continually grow. Therefore, both the drop in drag per particle as the particle cluster increases in size, as well as the drop in acoustic radiation force per particle as the particle cluster grows in size, must be considered for the acoustic separator device to work effectively. In the present disclosure, the lateral force component and the axial force component of the multi-dimensional acoustic standing wave are of the same order of magnitude. In this regard, it is noted that in a multi-dimensional acoustic standing wave, the axial force is stronger than the lateral force, but the lateral force of a multi-dimensional acoustic standing wave is much higher than the lateral force of a planar standing wave, usually by two orders of magnitude or more.

[0066] **FIG. 2** illustrates several exemplary transducer-reflector arrangements. Beginning on the left side of **FIG. 2**, particles or cells are shown scattered between a

transducer **120** and reflector **130**. As seen in the second illustration from the left, the transducer can be driven so as to cause the particles or cells to collect, agglomerate, aggregate, clump, or coalesce at the nodes or anti-nodes of the acoustic standing wave, depending on the particles' or secondary fluid's acoustic contrast factor relative to the host fluid. Turning now to the third and fourth illustrations from the left in **FIG. 2**, the ultrasonic transducer **120** is shown as including a plurality of piezoelectric elements **124** arranged in an array. The plurality of piezoelectric elements are configured to operate in active or inactive modes, as depicted. Piezoelectric elements in the active mode are generally considered to be "on," such that particles or cells are trapped above those elements, while elements in the inactive mode are generally considered to be "off," with no particle trapping occurring above those elements. The individual piezoelectric elements may be of any suitable size and shape. In certain embodiments, the piezoelectric elements may be smaller than the size of the objects to be trapped or moved between the active piezoelectric elements. The piezoelectric elements can be individually switched between the active and inactive modes as desired. For example, in the third illustration from the left in **FIG. 2**, elements 1 and 6-8 are operated in the inactive mode and elements 2-5 are operated in the active mode, such that the particles or cells are trapped above elements 2-5 (i.e., towards the left end of the flow chamber). In comparison, in the rightmost illustration in **FIG. 2**, elements 1-3 and 8 are operated in the inactive mode and elements 4-7 are operated in the active mode, such that the particles or cells are trapped above elements 4-7 (i.e., towards the right end of the flow chamber). In this way, switching between which elements are active/inactive can be used to move the trapped particles or cells from one end of the flow chamber to another (i.e., sweeping the trapped particles or cells) or to align the trapped particles or cells in desired locations within the flow chamber.

[0067] The acoustophoretic devices of the present disclosure are operable to perform acoustics-driven selective lysis with microfluidic separation, thereby concentrating pathogens and holding them for growth. The acoustophoretic devices, such as that depicted in **FIG. 1**, can be further used for elution, monitoring pathogen growth, and / or inspecting, detecting, isolating, monitoring, characterizing, or separating pathogens (e.g., bacteria, yeast, *E. coli*, lymphocytes) in blood containing blood cells.

The blood containing pathogens and blood cells is flowed through the acoustophoretic device. As explained above, a voltage signal is sent to drive the at least one ultrasonic transducer to create the acoustic standing wave in the flow chamber. As explained above and depicted in the transducer-reflector arrangements in **FIG. 2**, the acoustic standing wave drives the pathogens toward the longitudinal axis where the bacteria become trapped in the acoustic standing wave and can be walked towards the particulate outlet. A solvent (e.g., a bacteria-friendly solvent) is then introduced into the flow chamber through the solvent inlet. Finally, the pathogens are removed from the device through the particulate outlet.

[0068] When the acoustophoretic device is provided with a buffer inlet, a buffer (e.g., a dividing buffer or a selective lytic buffer) can be introduced into the flow chamber through the at least one buffer inlet. The buffer generally creates a buffer layer in the flow chamber that permits the pathogens to pass therethrough but destroys the specimen (e.g., blood cells) as it passes therethrough. This may also be called differential lysis. In **FIG. 1**, the buffer layer is depicted in the flow chamber **110** by gray shading. As can be further seen in **FIG. 1**, the blood cells in the blood (depicted as large white circles) become destroyed upon interfacing with the buffer layer, while the pathogens in the blood (depicted as smaller black circles) pass into the buffer layer and are driven toward the longitudinal axis by the acoustic standing wave. The pathogens may be eventually removed from the device via the particulate outlet. By selecting flow pressures and channel cross-sections, a concentrating factor of 10 or higher can be achieved. The fluid compression generates a concentrating factor of 10, while the acoustic compression generates a concentrating factor of 10^3 , through use of an acoustic concentrator, such as the acoustic concentrator described below and shown in **FIG. 3**. As shown in **FIG. 3**, three consecutive acoustic ten-fold compressions along three axes normal to each other provide the 10^3 concentrating factor. Constructing the acoustic concentrator with piezoelectric elements arranged in an array allows for concentrated cells in elution to be transported out of the concentrator. In certain embodiments, the acoustic concentrator can be operated with all of the piezoelectric elements in the active mode (i.e., “on” as shown in the bottom half of **FIG. 3**), which is useful for retaining the cells in the concentrator during culture broth circulation. This

construction further permits the injection of larger volumes than the resonator volume, thereby providing an additional concentrating factor. Due to this combined 10^4 concentrating factor, all cells from a five millimeter sample can be compressed into a 0.5 microliter sample, which is sufficient for mass spectrometry. Further concentration is also possible by injecting larger volumes into the system, while acoustically retaining the cells using the acoustic standing wave. In comparison to currently-employed processes, the presently disclosed methods require less than 10 division cycles due to the smaller total volume and less than 0-4 division cycles due to growth monitoring, with division cycles of 0.5 hours or more, which may be shortened relative to the blood culturing system due to the circulating culture broth.

[0069] Turning now to **FIG. 4**, a second exemplary embodiment of an acoustophoretic device **200** is depicted.

[0070] The device **200** includes a flow chamber **210**, at least one ultrasonic transducer **220**, a transparent wall **250**, and an optional acoustically transparent layer **260**. A microscope objective **240** is illustrated here, which can be used to characterize the cells within the flow chamber.

[0071] The flow chamber **210** is the region of the device **200** through which is flowed a host fluid containing target cells. The flow chamber **210** includes at least one inlet **212** and at least one outlet **214**. The at least one inlet **210** may include a solvent inlet, at least one host-fluid inlet, and optionally include at least one buffer inlet as shown and described above with respect to device **100**. Likewise, the at least one outlet **214** may include a particulate outlet and at least one residual outlet as shown and described above with respect to device **100**.

[0072] The ultrasonic transducer **220** of the device **200** is located on wall **222** of the flow chamber **210**. The microscope objective **240** of the device **200** is located on the opposite side of the flow chamber **210** from the ultrasonic transducer **220**. The optically transparent wall **250** is located between the microscope objective **240** and the flow chamber **210** volume, and forms wall **252** of the flow chamber **210**. As seen in **FIG. 4**, wall **252** is located on the opposite side of the flow chamber **210** from wall **222** (i.e., on the same side as the microscope objective **240**), such that the microscope objective **240** and the transparent wall **250** are located on the same side of the flow chamber **210**.

opposite from the ultrasonic transducer **220**. In this way, one or more acoustic standing waves are created in the flow chamber between the ultrasonic transducer **220** and the transparent wall **250**. The use of an ultrasonic transducer without an opposite reflector may be herein referred to as a “one-piece acoustic radiator.” It is noted that walls **222**, **252** of the flow chamber can be made from the same material, or can be made from different materials. The wall **252** should be optically transparent (i.e. can see through it), but wall **222** does not have to be transparent.

[0073] Generally, the microscope objective **240** is used to inspect or monitor the target cells trapped within the flow chamber **210**. In certain embodiments, such as that shown in **FIG. 4**, an immersion oil layer **270** may be provided between the microscope objective **240** and the optically transparent wall **250**. Further yet, an acoustically transparent layer **260** may be present between the cover glass **250** and the flow chamber **210**. The acoustically transparent layer (ATL) prevents the cells from being pressed against the glass surface. The ATL may be a hydrogel. This surface may be advantageous for certain stem cells that can be studied with the system described in **FIG. 4**.

[0074] In accordance with the present disclosure, the acoustophoretic devices described herein, such as that depicted in **FIGS. 4-6**, can be used for inspecting, detecting, isolating, monitoring, characterizing, or separating various target cells (e.g., specialized circulating cells, such as CTCs, in blood containing blood cells), including their development or interaction with chemicals (e.g., drug candidates).

[0075] In the present devices, to isolate specialized circulating cells, paramagnetic particles or hollow microbubbles can be used. The paramagnetic particles / microbubbles generally pull the specialized circulating cells out of the blood because they move in an opposite direction to the blood cells when subjected to acoustophoresis (due to the negative acoustic contrast factor of the paramagnetic particles / microbubbles, which moves towards pressure antinodes of an acoustic standing wave). In this way, microfluidics with sheathing flows and acoustic standing wave(s) can be used to extract and concentrate specialized circulating cells from blood. This provides a distinct advantage over currently-employed systems and methods, which required

incubation with immunomagnetic beads to capture magnetically labeled cells by flotation as they passed through isolation zones of known microfluidic devices.

[0076] This is illustrated in **FIG. 7**. The system here is similar to that depicted in **FIG. 1**. As illustrated here, the fluid flowing in through host-fluid inlet **114** contains, for example, cells **140** and **141**, the target cells **143**, and acoustically active particles **142**. The acoustically active particles attach to the target cells. For example, the particles **142** may be coated with an affinity ligand to bind to the target cells **142**. The acoustic standing wave generated by transducer **120** and reflector **130** then operate upon the particles **142**, resulting in the target cells **143** being separated from the other cells **140**, **141**. The target cells **143** then exit through the particulate outlet **116**, while the other cells **140**, **141** exit through the residual outlet **118**.

[0077] In the presently disclosed acoustophoretic devices, acoustophoresis and acoustically active particles (e.g. microbubbles or paramagnetic particles) can be utilized instead of immunomagnetic beads. For example, device **200** can be operated by flowing blood containing specialized circulating cells and blood cells therethrough and sending a voltage signal to drive the at least one ultrasonic transducer to create the acoustic standing wave in the flow chamber and microbubbles in the blood. Because the device **200** is a one-piece acoustic radiator, the specialized circulating cells with attached microbubbles are driven by the acoustic standing wave toward the acoustically transparent wall where the specialized circulating cells and attached microbubbles become trapped in the acoustic standing wave, such as is depicted in **FIG. 3**.

[0078] With reference to **FIG. 5**, the piezoelectric material of the ultrasonic transducer **220** may include a plurality of piezoelectric elements **224** arranged in an array. The plurality of piezoelectric elements are configured to operate in active or inactive modes. As explained above, piezoelectric elements in the active mode are generally considered to be “on,” such that the specialized circulating cells are trapped above those elements, while elements in the inactive mode are generally considered to be “off,” with no trapping of the specialized circulating cells occurring above those elements.

[0079] The piezoelectric elements **124** can be individually switched between the active and inactive modes as desired. For example, in **FIG. 5**, the piezoelectric

elements toward the center of the flow chamber **210** are operated in the active mode, and the remaining piezoelectric elements (toward the inlet / outlet of the flow chamber) are operated in the inactive mode. Operating the piezoelectric elements in this way positions the specialized circulating cells trapped in the acoustic standing wave in alignment with the microscope objective **240**, which is depicted as being located at or near the center of the flow chamber **210**.

[0080] Another operation of the piezoelectric elements **124** is depicted in **FIG. 6**. In **FIG. 6**, the piezoelectric elements nearest the inlet / outlet of the flow chamber are operated in the inactive mode, and the remaining piezoelectric elements are operated in alternating active / inactive modes. Operating the piezoelectric elements **124** in this way positions the specialized circulating cells trapped in the acoustic standing wave in one or more wells **262** in the acoustically transparent layer **260**.

[0081] In biological applications, many parts of the device in contact with the sample, e.g. the flow chamber, may all be disposable, with only the transducer and reflector to be cleaned for reuse.

[0082] Some further explanation of the ultrasonic transducers used in the devices, systems, and methods of the present disclosure may be helpful as well. In this regard, the transducers use a piezoelectric element, usually made of PZT-8 (lead zirconate titanate). Such elements may have a 1 inch cross-section and a nominal 2 MHz resonance frequency, and may also be of a larger size. Each ultrasonic transducer module can have only one element, or can have multiple elements that each act as a separate ultrasonic transducer and are either controlled by one or multiple amplifiers. The piezoelectric element(s) can be crystalline, semi-crystalline, or non-crystalline. The piezoelectric element(s) can be square, rectangular, irregular polygon, or generally of any arbitrary shape. The transducer(s) is/are used to create a pressure field that generates forces of the same order of magnitude both orthogonal to the standing wave direction (lateral) and in the standing wave direction (axial).

[0083] **FIG. 8** is a cross-sectional diagram of a conventional ultrasonic transducer. This transducer has a wear plate **50** at a bottom end, epoxy layer **52**, piezoelectric element **54** (e.g. a ceramic crystal made of, e.g. PZT), an epoxy layer **56**, and a backing layer **58**. On either side of the piezoelectric element, there is an electrode: a positive

electrode **61** and a negative electrode **63**. The epoxy layer **56** attaches backing layer **58** to the piezoelectric element **54**. The entire assembly is contained in a housing **60** which may be made out of, for example, aluminum. An electrical adapter **62** provides connection for wires to pass through the housing and connect to leads (not shown) which attach to the piezoelectric element **54**. Typically, backing layers are designed to add damping and to create a broadband transducer with uniform displacement across a wide range of frequency and are designed to suppress excitation at particular vibrational eigen-modes. Wear plates are usually designed as impedance transformers to better match the characteristic impedance of the medium into which the transducer radiates.

[0084] FIG. 9 is a cross-sectional view of an ultrasonic transducer **81** of the present disclosure. Transducer **81** is shaped as a disc or a plate, and has an aluminum housing **82**. The piezoelectric element can be, e.g., a mass of perovskite ceramic crystals, each consisting of a small, tetravalent metal ion, usually titanium or zirconium, in a lattice of larger, divalent metal ions, usually lead or barium, and O²⁻ ions. As an example, in the embodiment shown in FIG. 9, a PZT (lead zirconate titanate) crystal **86** defines the bottom end of the transducer, and is exposed from the exterior of the housing. The crystal is supported on its perimeter by a small elastic layer **98**, e.g. silicone or similar material, located between the crystal and the housing. Put another way, no wear layer is present. In particular embodiments, the crystal is an irregular polygon, and in further embodiments is an asymmetrical irregular polygon.

[0085] Screws **88** attach an aluminum top plate **82a** of the housing to the body **82b** of the housing via threads. The top plate includes a connector **84** for powering the transducer. The top surface of the PZT crystal **86** is connected to a positive electrode **90** and a negative electrode **92**, which are separated by an insulating material **94**. The electrodes can be made from any conductive material, such as silver or nickel. Electrical power is provided to the PZT crystal **86** through the electrodes on the crystal. Note that the crystal **86** has no backing layer or epoxy layer. Put another way, there is an air gap **87** in the transducer between aluminum top plate **82a** and the crystal **86** (i.e. the air gap is completely empty). A minimal backing **58** and/or wear plate **50** may be provided in some embodiments, as seen in FIG. 10.

[0086] The transducer design can affect performance of the system. A typical transducer is a layered structure with the piezoelectric element bonded to a backing layer and a wear plate. Because the transducer is loaded with the high mechanical impedance presented by the standing wave, the traditional design guidelines for wear plates, e.g., half wavelength thickness for standing wave applications or quarter wavelength thickness for radiation applications, and manufacturing methods may not be appropriate. Rather, in one embodiment of the present disclosure the transducers, there is no wear plate or backing, allowing the piezoelectric element to vibrate in one of its eigenmodes (i.e. near eigenfrequency) with a high Q-factor. The vibrating piezoelectric element, such as, e.g., a ceramic crystal/disk, is directly exposed to the fluid flowing through the acoustic chamber.

[0087] Removing the backing (e.g. making the piezoelectric element air backed) also permits the element to vibrate at higher order modes of vibration with little damping (e.g. higher order modal displacement). In a transducer having a piezoelectric element with a backing, the element vibrates with a more uniform displacement, like a piston. Removing the backing allows the element to vibrate in a non-uniform displacement mode. The higher order the mode shape of the piezoelectric element, the more nodal lines the element has. The higher order modal displacement of the element creates more trapping lines, although the correlation of trapping line to node is not necessarily one to one, and driving the element at a higher frequency will not necessarily produce more trapping lines.

[0088] In some embodiments, the piezoelectric element may have a backing that minimally affects the Q-factor of the crystal (e.g. less than 5%). The backing may be made of a substantially acoustically transparent material such as balsa wood, foam, or cork which allows the element to vibrate in a higher order mode shape and maintains a high Q-factor while still providing some mechanical support for the element. The backing layer may be a solid, or may be a lattice having holes through the layer, such that the lattice follows the nodes of the vibrating element in a particular higher order vibration mode, providing support at node locations while allowing the rest of the element to vibrate freely. The goal of the lattice work or acoustically transparent material

is to provide support without lowering the Q-factor of the piezoelectric element or interfering with the excitation of a particular mode shape.

[0089] Placing the piezoelectric element in direct contact with the fluid also contributes to the high Q-factor by avoiding the dampening and energy absorption effects of the epoxy layer and the wear plate. Other embodiments may have wear plates or a wear surface to prevent the PZT, which contains lead, contacting the host fluid. This may be desirable in, for example, biological applications such as separating blood. Such applications might use a wear layer such as chrome, electrolytic nickel, or electroless nickel. Chemical vapor deposition could also be used to apply a layer of poly(p-xylylene) (e.g. Parylene) or other polymers or polymer films. Organic and biocompatible coatings such as silicone or polyurethane are also usable as a wear surface.

[0090] Certain embodiments of the acoustophoretic devices and methods described herein are useful for preparing a sample for subsequent downstream processing. In this regard, the sample may be subsequently processed by any known filtration or processing, such as by using a portable flow cytometer. Other embodiments of the acoustophoretic devices and methods described herein are useful for inspecting, detecting, isolating, or characterizing bacteria or specialized circulating cells in blood containing blood cells. In this regard, the bacteria or specialized circulating cells may be subsequently processed or filtered by any known filtration or processing, such as by collecting the bacteria or specialized circulating cells from the device and feeding the same to another filtration process.

[0091] Avoiding centrifuges and physical filters allows better separation of cells without lowering the viability of the cells. The form factor of the acoustophoretic device is also smaller than a physical filtration system, allowing cell separation to be miniaturized. The transducers may also be driven to create rapid pressure changes to prevent or clear blockages due to agglomeration of cells. The frequency of the transducers may also be varied to obtain optimal effectiveness for a given power.

[0092] The present disclosure has been described with reference to exemplary embodiments. Obviously, modifications and alterations will occur to others upon reading and understanding the preceding detailed description. It is intended that the

present disclosure be construed as including all such modifications and alterations insofar as they come within the scope of the appended claims or the equivalents thereof.

CLAIMS:

1. A method for inspecting, detecting, isolating, monitoring, characterizing, or separating target cells in a host fluid also containing non-target cells, the method comprising:

flowing the host fluid containing the target cells and the non-target cells through an acoustophoretic device, the acoustophoretic device comprising:

a flow chamber having a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis;

at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and

a reflector located on a wall on the opposite side of the flow chamber from the at least one ultrasonic transducer;

sending a voltage signal to drive the at least one ultrasonic transducer to create the acoustic standing wave in the flow chamber to drive the target cells toward the longitudinal axis where the target cells become trapped in the acoustic standing wave;

introducing a solvent into the flow chamber through the solvent inlet; and
removing the target cells from the device through the particulate outlet.

2. The method of claim 1, wherein the acoustophoretic device further comprises at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet.

3. The method of claim 2, further comprising introducing a buffer into the flow chamber through the at least one buffer inlet, the buffer creating a buffer layer that permits the target cells to pass therethrough but destroys the non-target cells as they pass therethrough.

4. The method of claim 3, wherein the buffer is a selective lytic buffer.

5. The method of claim 1, further comprising removing a portion of the solvent from the device through the residual outlet.

6. The method of claim 1, wherein the piezoelectric material includes a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements operated between active and inactive modes such that the target cells are trapped above the piezoelectric elements in the active mode.

7. The method of claim 6, further comprising switching the piezoelectric elements between the active and inactive modes to move the target cells trapped in the acoustic standing wave along the longitudinal axis from the first end to the second end of the flow chamber to the particulate outlet.

8. The method of claim 1, wherein the solvent is a bacteria-friendly solvent.

9. The method of claim 1, wherein the acoustic standing wave is a multi-dimensional acoustic standing wave.

10. The method of claim 1, wherein acoustically active particles are attached to the target cells.

11. An acoustophoretic device, comprising:
 - a flow chamber having a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis;
 - at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and
 - a reflector located on a wall on the opposite side of the flow chamber from the at least one ultrasonic transducer.
12. The acoustophoretic device of claim 11, further comprising at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet.
13. The acoustophoretic device of claim 11, wherein the piezoelectric material includes a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements configured to operate between active and inactive modes.
14. The acoustophoretic device of claim 11, wherein the flow chamber is disposable.
15. The acoustophoretic device of claim 11, wherein the at least one ultrasonic transducer comprises:
 - a housing having a top end, a bottom end, and an interior volume; and
 - a piezoelectric crystal at the bottom end of the housing having an exposed exterior surface and an interior surface, the crystal being able to vibrate when driven by a voltage signal.

16. The acoustophoretic device of claim 15, wherein no backing layer is present within the housing of the at least one ultrasonic transducer, and an air gap is present in the interior volume between the crystal and a top plate at the top end of the housing; or

wherein the at least one ultrasonic transducer further comprises a backing layer contacting the interior surface of the crystal, the backing layer being made of a substantially acoustically transparent material.

17. A method for inspecting, detecting, isolating, monitoring, characterizing, or separating specialized circulating cells in blood containing blood cells, the method comprising:

flowing the blood containing specialized circulating cells and blood cells through an acoustophoretic device, the acoustophoretic device comprising:

a flow chamber having at least one inlet and at least one outlet;

at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and

a cover glass forming a wall of the flow chamber opposite the at least one ultrasonic transducer;

sending a voltage signal to drive the at least one ultrasonic transducer to create the acoustic standing wave in the flow chamber and microbubbles in the blood, the microbubbles attaching to the specialized circulating cells and being driven by the acoustic standing wave toward the cover glass where the specialized circulating cells and attached microbubbles become trapped in the acoustic standing wave; and

examining the specialized circulating cells using a microscope objective.

18. The method of claim 17, wherein the at least one inlet includes a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and the at least one outlet includes a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis.

19. The method of claim 18, wherein the acoustophoretic device further comprises at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet.

20. The method of claim 19, further comprising introducing a dividing buffer into the flow chamber through the at least one buffer inlet.

21. The method of claim 17, wherein the acoustophoretic device further comprises a substantially acoustically transparent layer between the cover glass and the flow chamber.

22. The method of claim 21, wherein the piezoelectric material includes a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements operated between active and inactive modes such that the specialized circulating cells are trapped above the piezoelectric elements in the active mode.

23. The method of claim 22, further comprising switching the piezoelectric elements between the active and inactive modes to position the specialized circulating cells trapped in the acoustic standing wave in alignment with the microscope objective.

24. The method of claim 22, wherein the substantially acoustically transparent layer includes one or more wells therein.

25. The method of claim 24, further comprising switching the piezoelectric elements between the active and inactive modes to position the specialized circulating cells trapped in the acoustic standing wave in in the one or more wells.

26. The method of claim 17 wherein the specialized circulating cells are circulating tumor cells.

27. The method of claim 17, wherein the acoustic standing wave is a multi-dimensional acoustic standing wave.

28. An acoustophoretic device, comprising:
a flow chamber having at least one inlet and at least one outlet;
at least one ultrasonic transducer located on a wall of the flow chamber, the at least one ultrasonic transducer including a piezoelectric material driven by a voltage signal to create an acoustic standing wave in the flow chamber; and
the flow chamber having an optically transparent wall opposite the at least one ultrasonic transducer.

29. The acoustophoretic device of claim 28, wherein the at least one inlet includes a solvent inlet and at least one host-fluid inlet at a first end of the flow chamber, and the at least one outlet includes a particulate outlet and at least one residual outlet at a second end of the flow chamber opposite the first end thereof, wherein the solvent inlet and the particulate outlet are aligned with a longitudinal axis of the flow chamber and the at least one host-fluid inlet and the at least one residual outlet are spaced apart from the longitudinal axis.

30. The acoustophoretic device of claim 29, further comprising at least one buffer inlet located between the solvent inlet and the at least one host-fluid inlet.

31. The acoustophoretic device of claim 29, further comprising an acoustic concentrator fluidly connected to the particulate outlet.

32. The acoustophoretic device of claim 28, further comprising a substantially acoustically transparent layer between the optically transparent wall and the flow chamber.

33. The acoustophoretic device of claim 32, wherein the substantially acoustically transparent layer includes one or more wells therein.

34. The acoustophoretic device of claim 32, wherein the piezoelectric material includes a plurality of piezoelectric elements arranged in an array, the plurality of piezoelectric elements configured to operate between active and inactive modes.


35. The acoustophoretic device of claim 28, wherein the flow chamber is disposable.

36. The acoustophoretic device of claim 28, wherein the at least one ultrasonic transducer comprises:

- a housing having a top end, a bottom end, and an interior volume; and
- a piezoelectric crystal at the bottom end of the housing having an exposed exterior surface and an interior surface, the crystal being able to vibrate when driven by a voltage signal.

37. The acoustophoretic device of claim 36, wherein no backing layer is present within the housing of the at least one ultrasonic transducer, and an air gap is present in the interior volume between the crystal and a top plate at the top end of the housing.

38. The acoustophoretic device of claim 36, wherein the at least one ultrasonic transducer further comprises a backing layer contacting the interior surface of the crystal, the backing layer being made of a substantially acoustically transparent material.

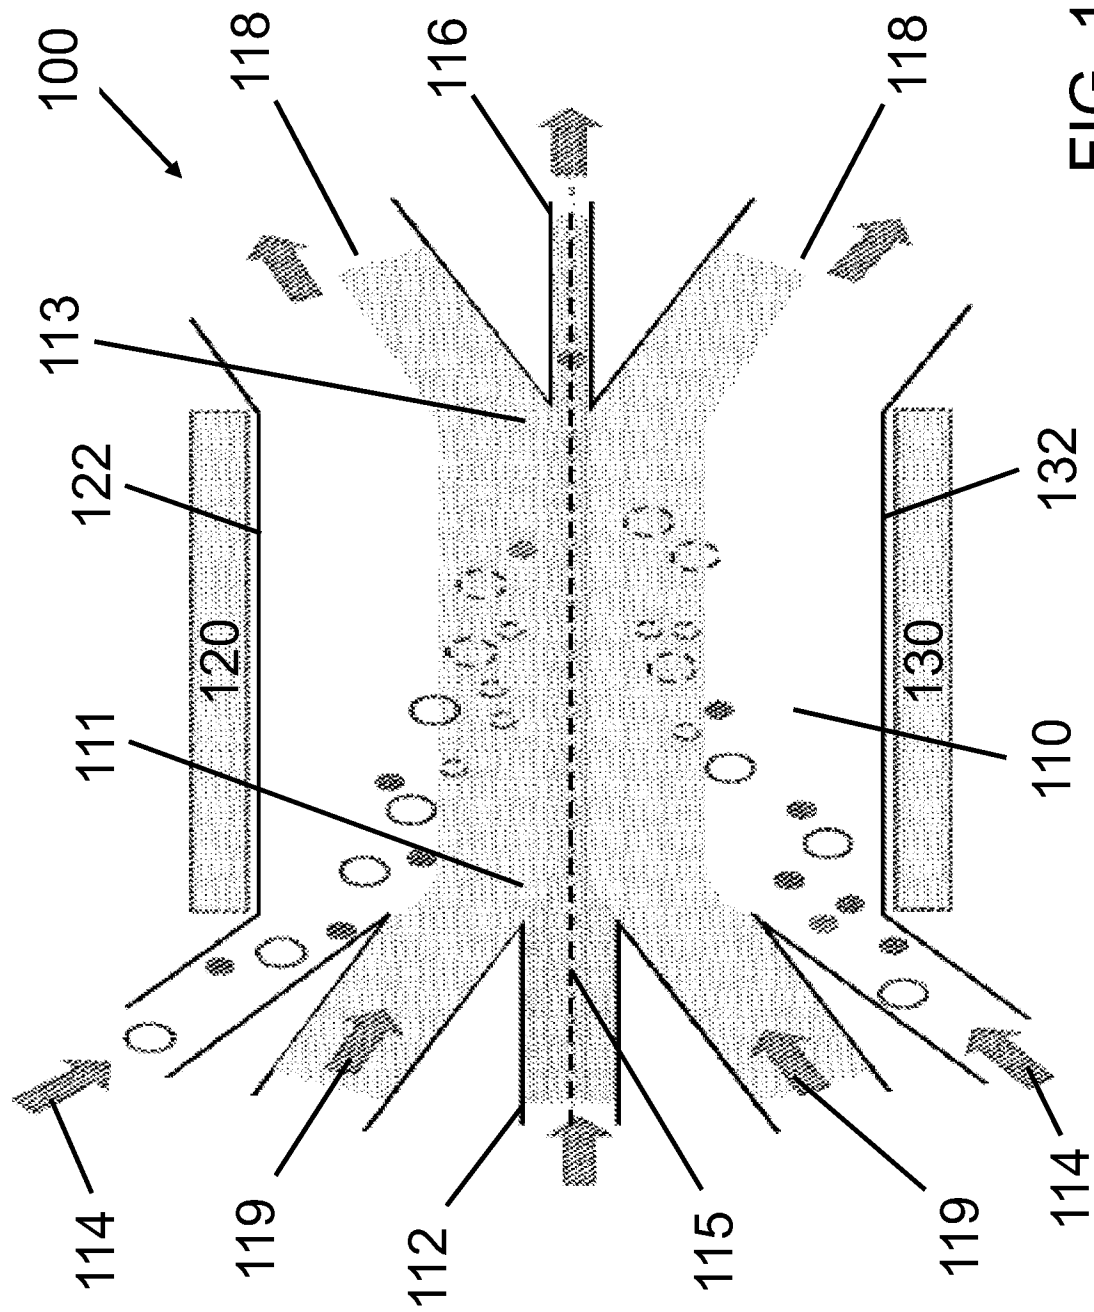

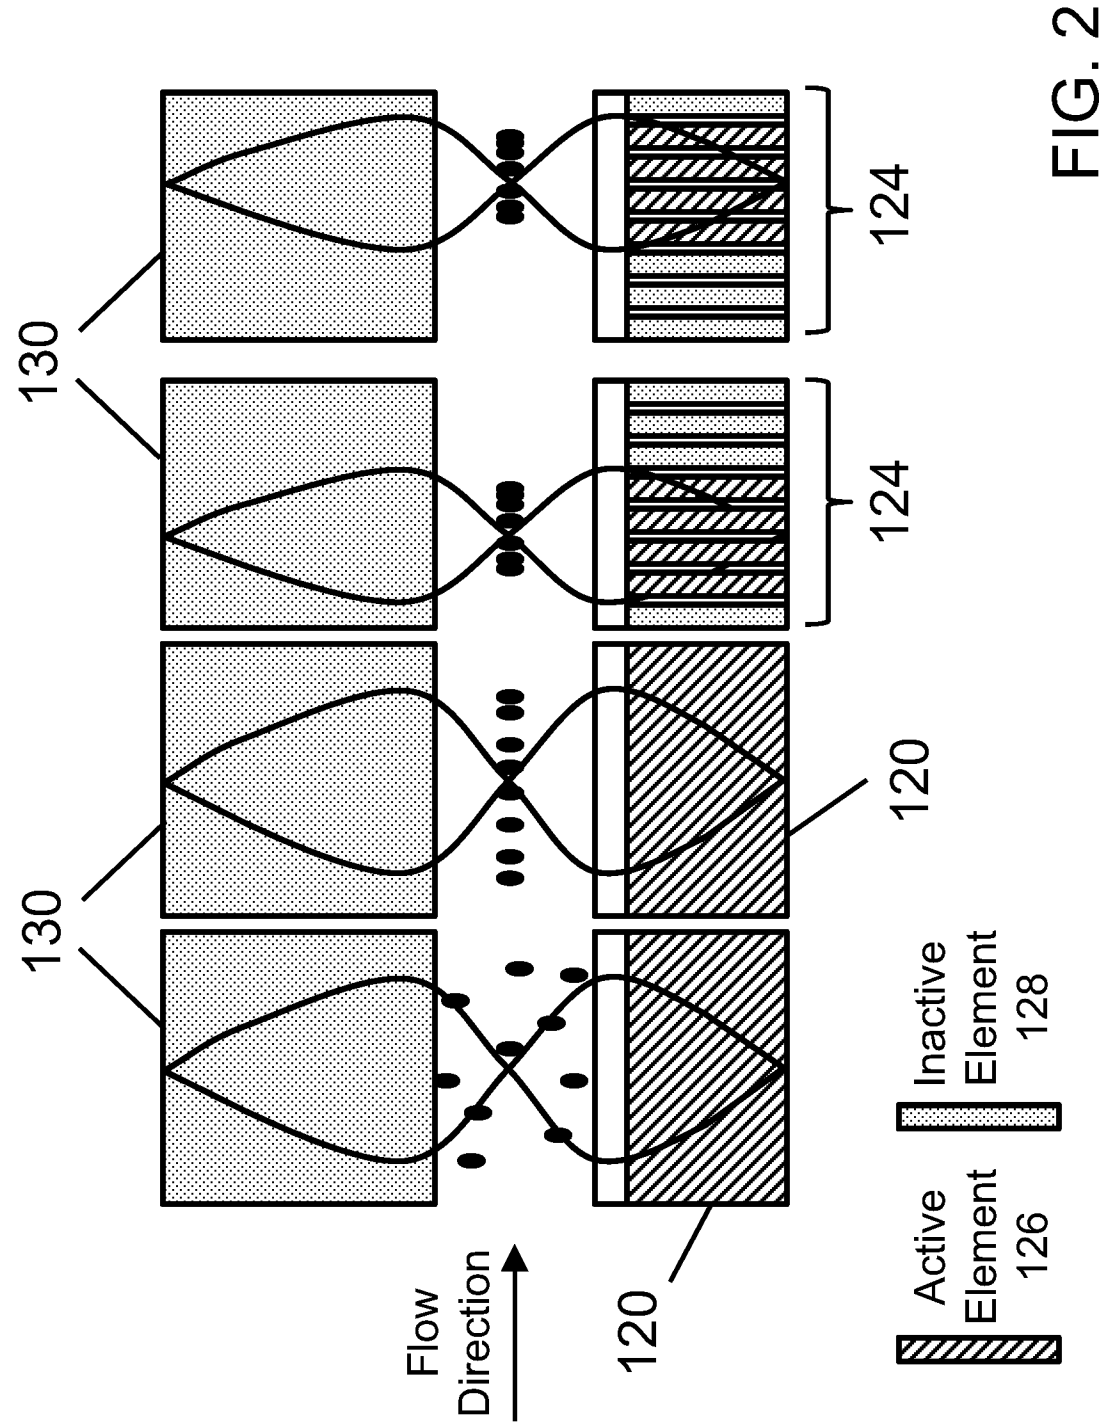


FIG. 2

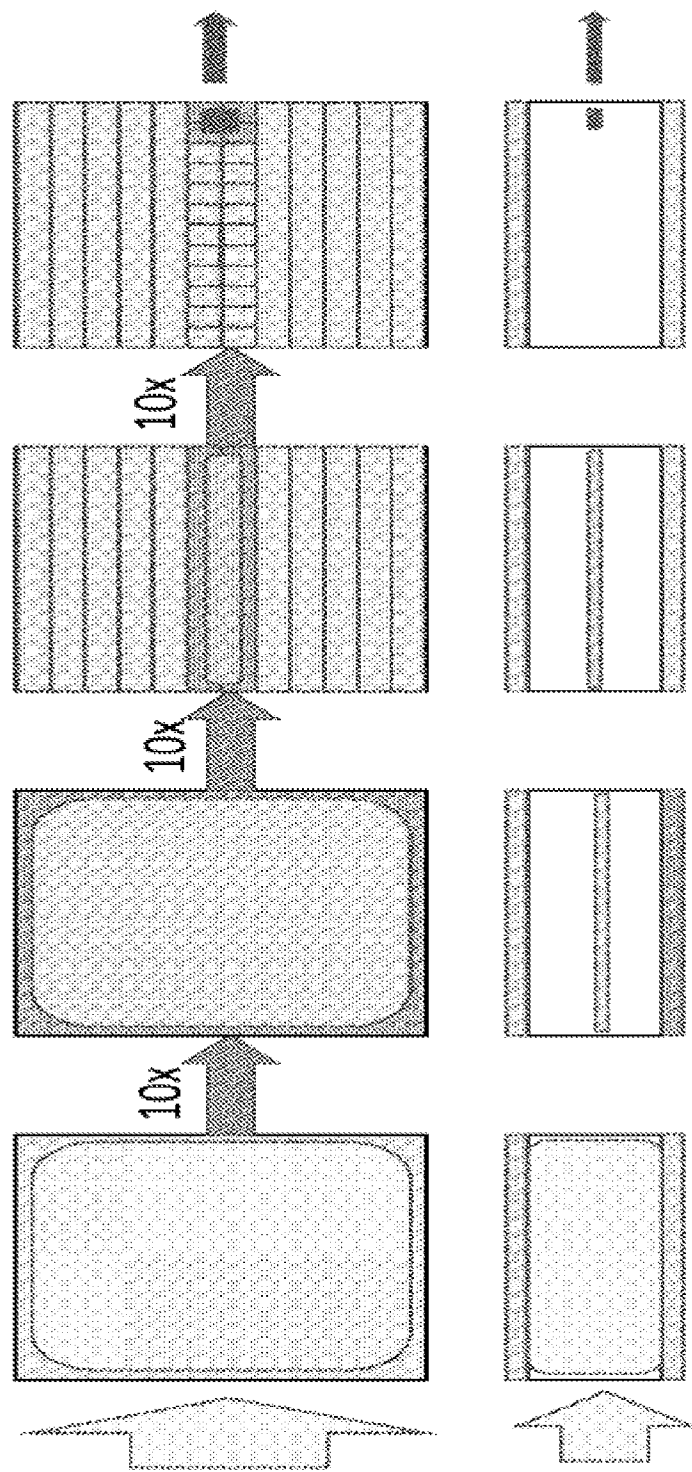


FIG. 3

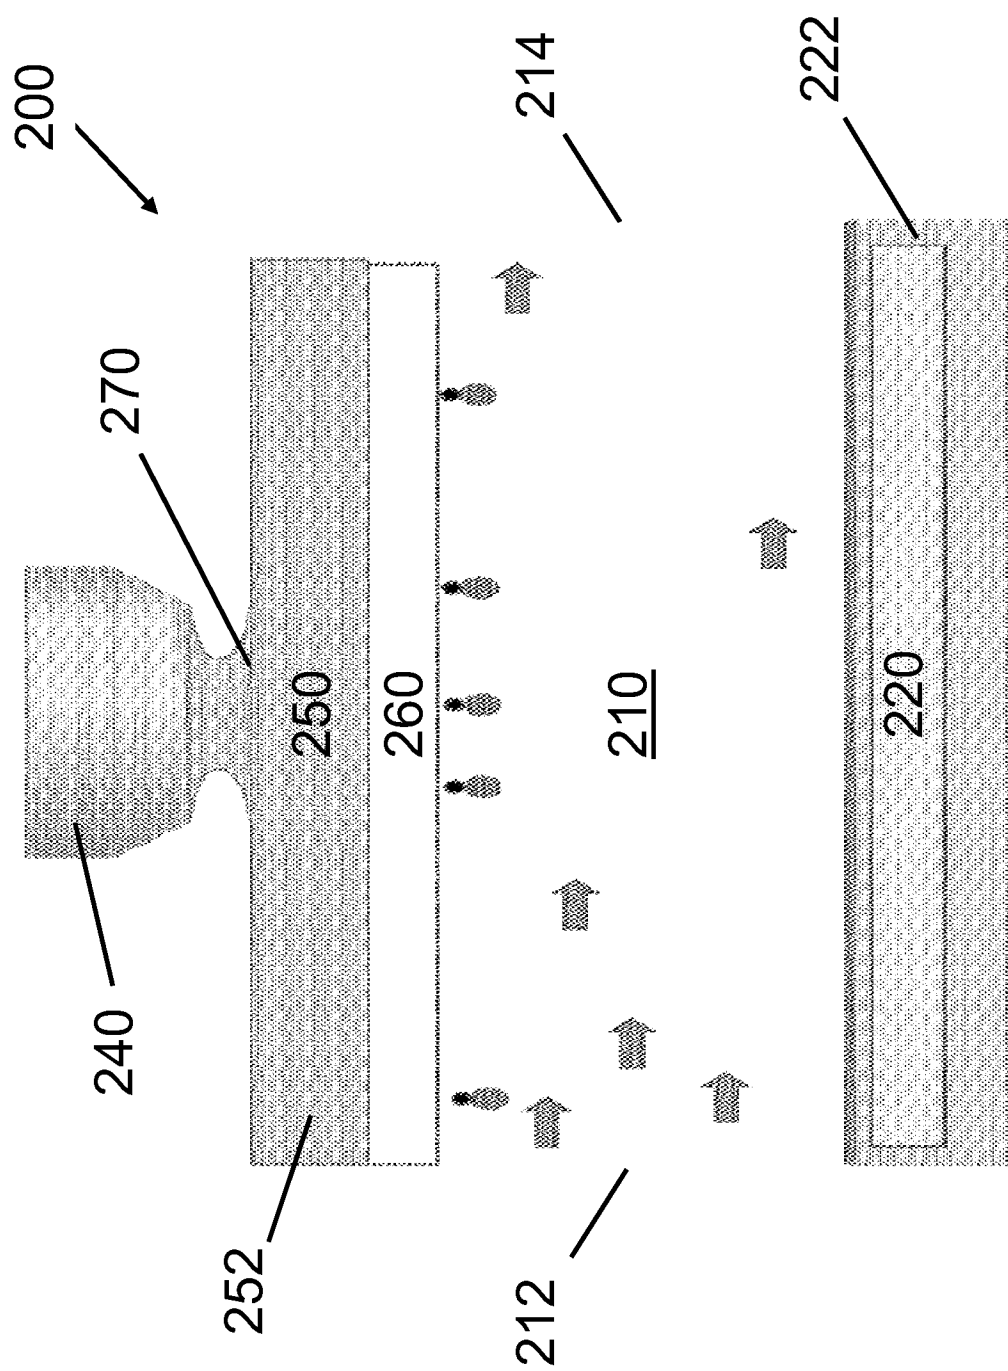


FIG. 4

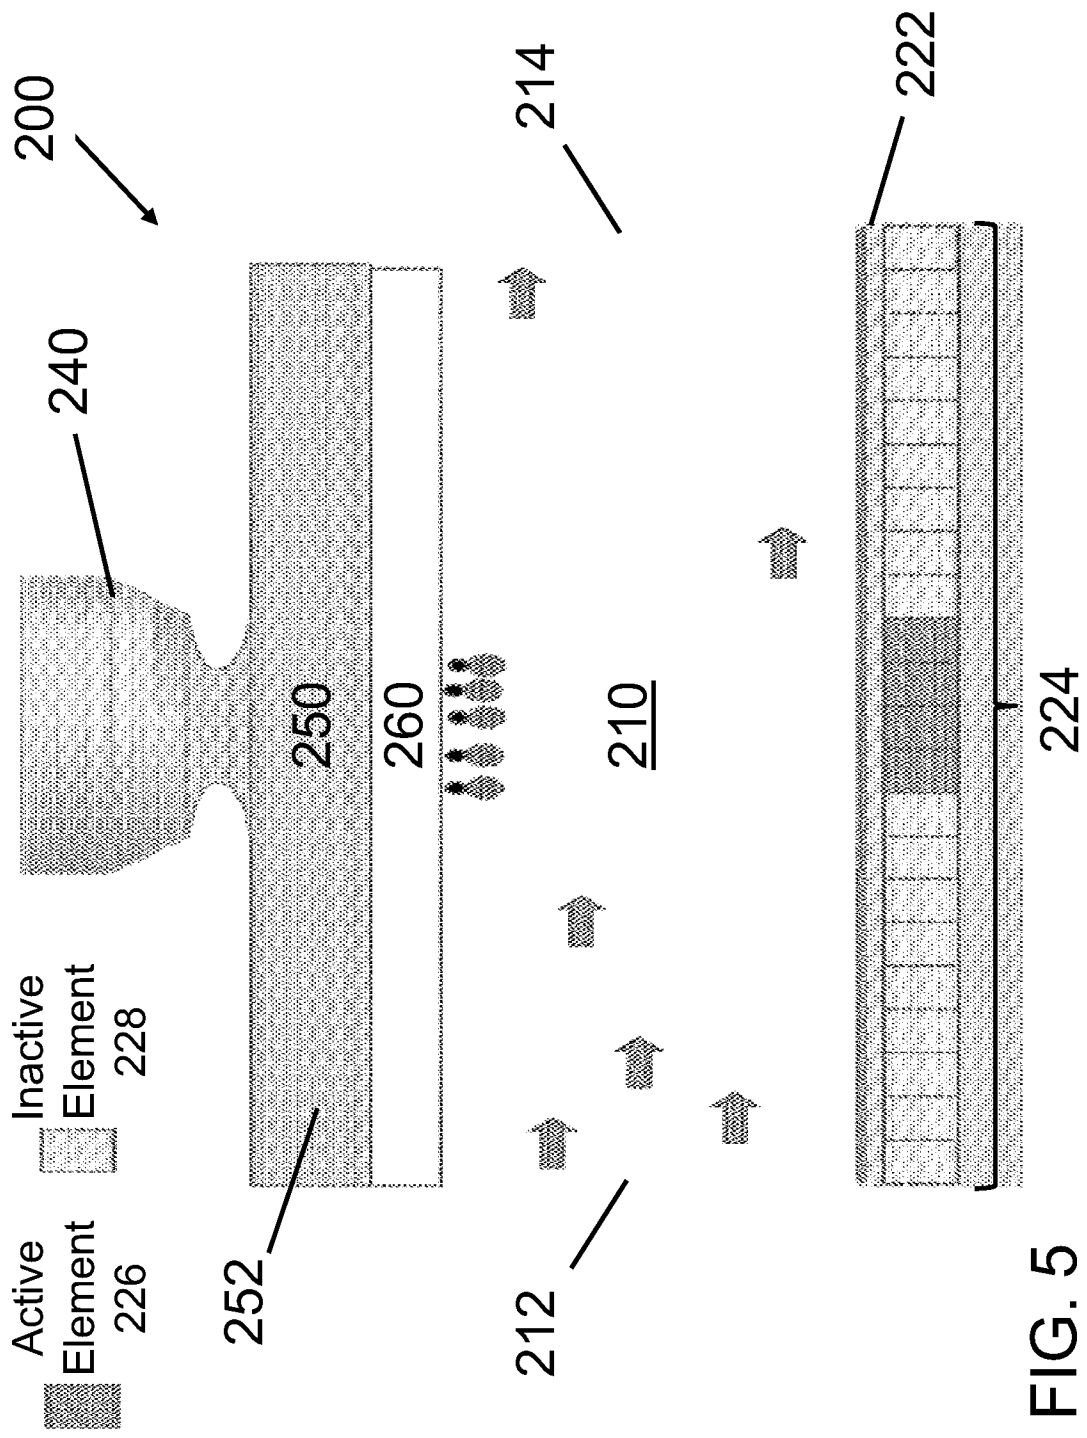


FIG. 5

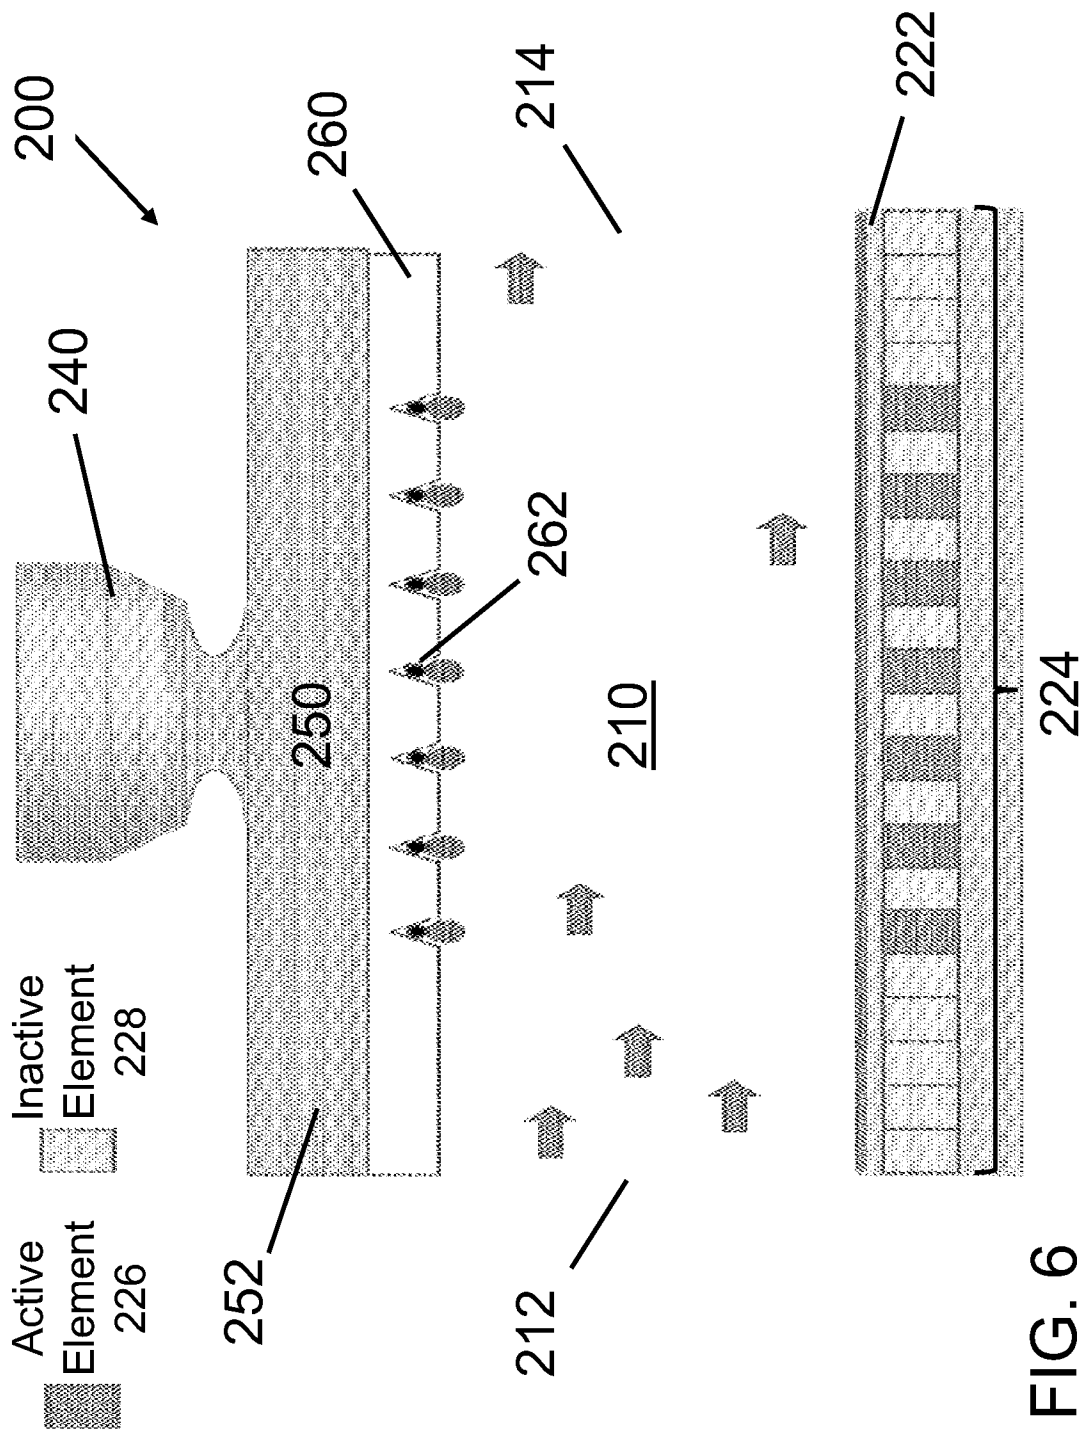


FIG. 6

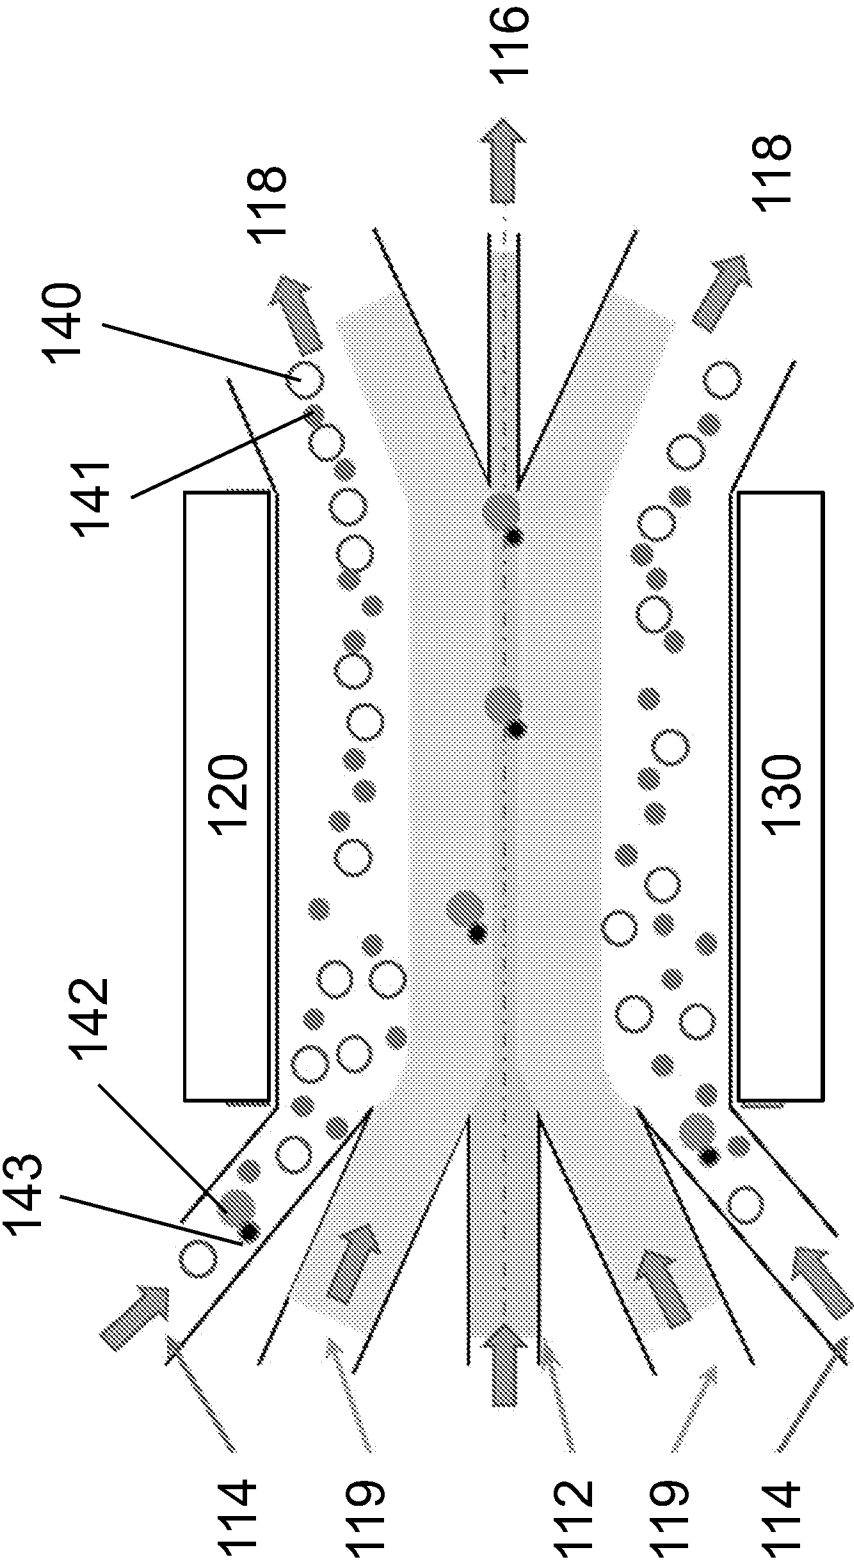


FIG. 7

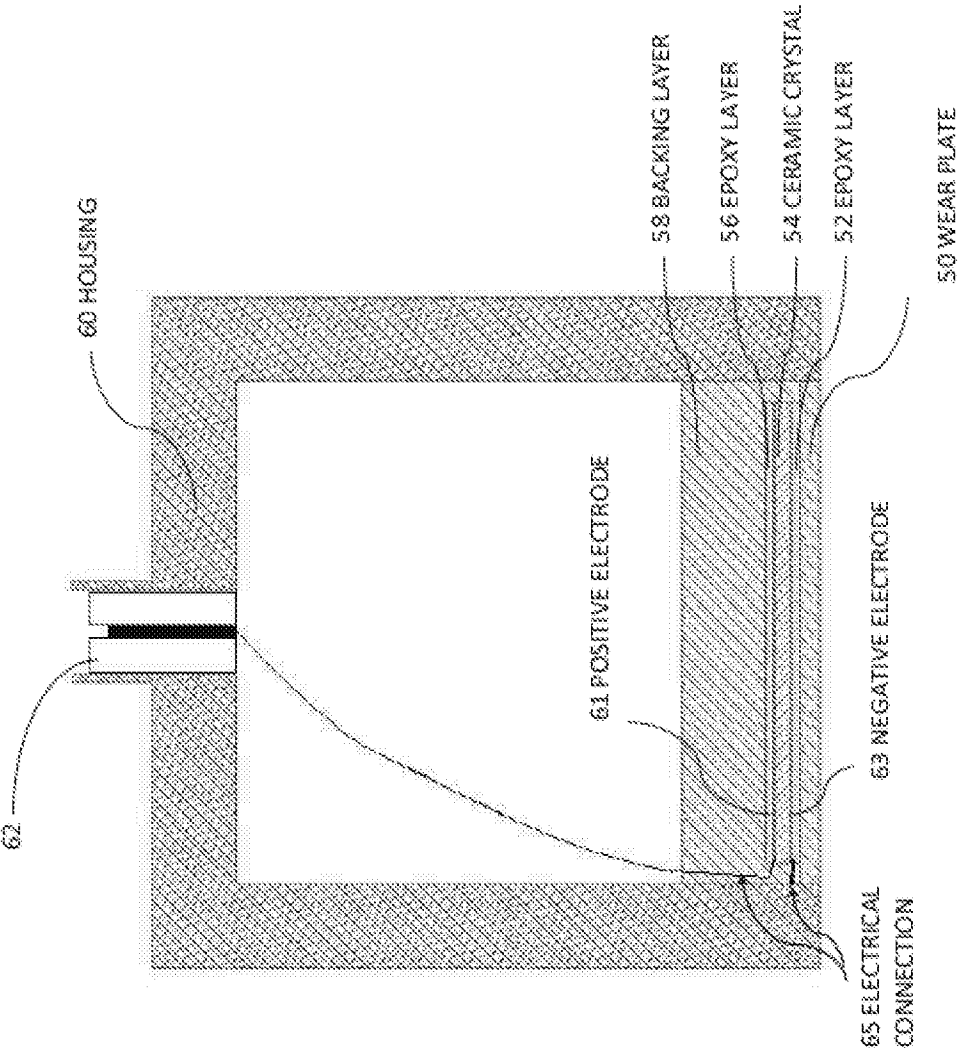


FIG. 8

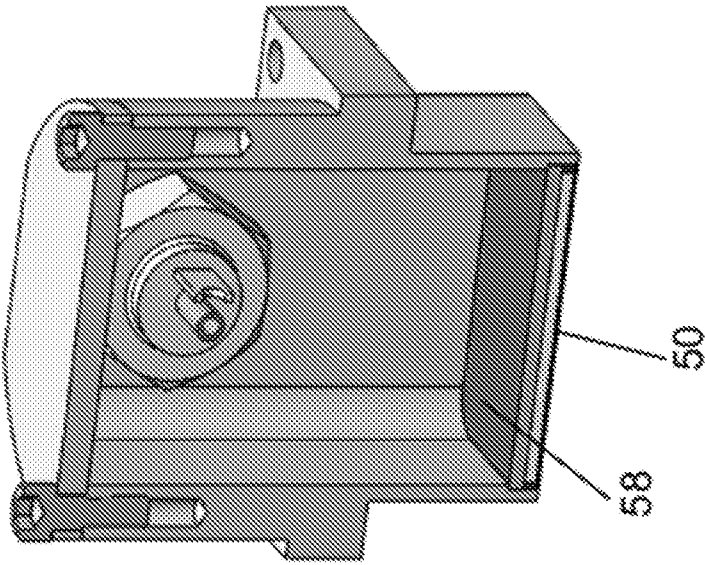


FIG. 10

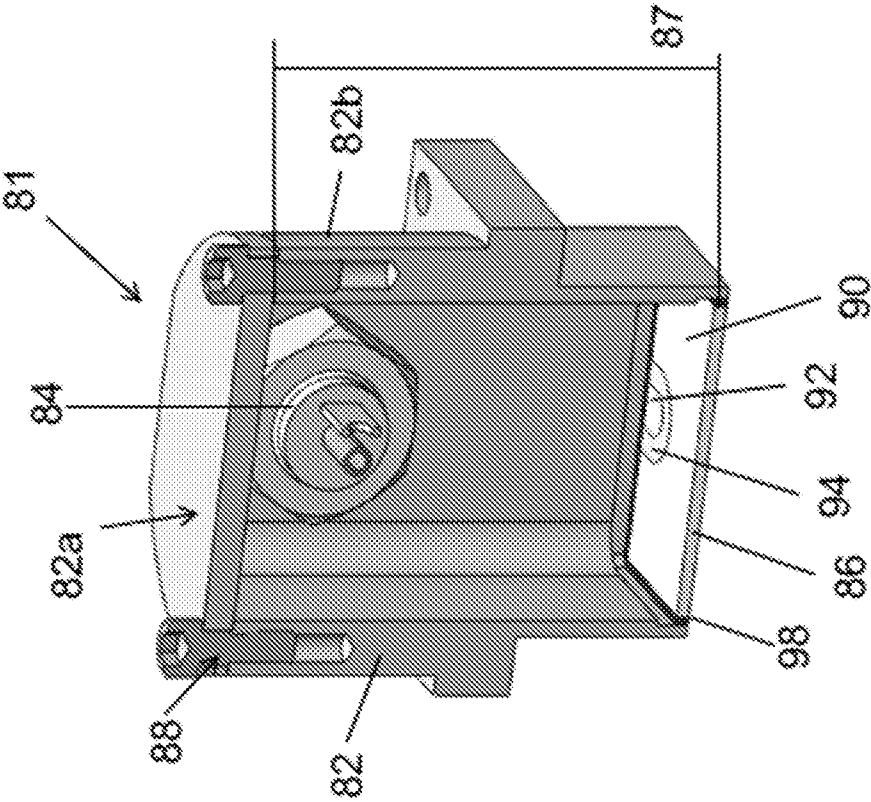


FIG. 9