



(51) International Patent Classification:

A61N 1/32 (2006.01) A61N 1/04 (2006.01)
A61N 1/40 (2006.01) A61B 18/00 (2006.01)

(21) International Application Number:

PCT/EP20 15/0623 13

(22) International Filing Date:

3 June 2015 (03.06.2015)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

1417 1193.7 4 June 2014 (04.06.2014) EP

(71) Applicant: **KONINKLIJKE PHILIPS N.V.** [NL/NL]; High Tech Campus 5, NL-5656 AE Eindhoven (NL).

(72) Inventors: **JURNA, Martin**; c/o High Tech Campus 5, NL-5656 AE Eindhoven (NL). **PALERO, Jonathan Alambra**; c/o High Tech Campus 5, NL-5656 AE Eindhoven (NL). **BARAGONA, Marco**; c/o High Tech Campus 5, NL-5656 AE Eindhoven (NL). **HORTON, Margaret Ruth**; c/o High Tech Campus 5, NL-5656 AE Eindhoven (NL). **VARGHESE, Babu**; c/o High Tech Campus 5, NL-5656 AE Eindhoven (NL).

(74) Agents: **WOLFS, Marc Johannes Maria** et al; High Tech Campus 5, 5656 AE Eindhoven (NL).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on nextpage]

(54) Title: CENTROSYMMETRIC RADIO FREQUENCY ELECTRODE CONFIGURATION FOR SKIN TREATMENT

Fig. 1A

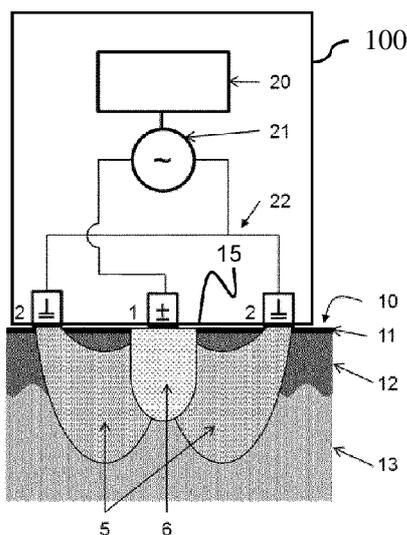

(57) Abstract: The invention relates to a device (100) for RF skin treatment comprising an outer electrode (2) arranged on an operational side (15) of the device. The outer electrode has an annular or equilateral polygonal shape. An inner electrode (1) is arranged at a center of the outer electrode and is surrounded by the outer electrode. An RF generator (21) is arranged to supply an RF treatment voltage between the inner electrode (1) and the outer electrode (2). A skin contact surface of the inner electrode has a largest cross-sectional dimension in a range of 200 -500 μm , and the RF treatment voltage is less than 50 V. The invention provides a device with improved safety in that it enables the creation of non-ablative fractionated skin lesions, particularly using a relatively low RF treatment voltage for treating the skin as compared to known devices and without the necessity of a feedback or monitoring system.



Declarations under Rule 4.17:

— *as to applicant's entitlement to apply for and be granted a patent (Rule 4.1 7(H))*

Published:

— *with international search report (Art. 21(3))*

Centrosymmetric radio frequency electrode configuration for skin treatment

FIELD OF THE INVENTION

The invention relates a device for skin treatment, in particular for radio frequency (RF) treatment of human skin. The device is primarily suitable for skin tightening and/or skin rejuvenation, in particular for fractional RF skin treatment. The invention also
5 relates to the use of such a device for skin treatment.

BACKGROUND OF THE INVENTION

Radio frequency (RF) is conventionally used in both the professional and home-use aesthetic market for skin tightening. The ability to heat a large volume at dermal
10 skin level has made the radio frequency technology the standard for skin tightening and for treating skin laxity. Compared to laser treatments, RF devices have a relatively lower cost price and can provide larger-volume and deeper tissue contraction. Additionally, RF energy dissipation does not rely on absorption of light by chromophores, so that tissue pigmentation or the vascular network does not interfere with the delivery of energy.

15 The basic principle of RF energy delivery at the skin surface and from there to tissue is that an alternating current is applied in a closed circuit with the skin. Tissue impedance directly affects the extent of the heating: RF propagates more easily through tissues with high conductivity (low electrical resistance), while tissues with high electrical resistance (high impedance, low conductance) are poor conductors of RF energy. RF energy
20 takes the path of least resistance through skin tissue and is dissipated as thermal energy primarily due to molecular vibrations.

A growing application for RF beyond skin tightening is skin rejuvenation. In most RF skin rejuvenation devices, fractional thermal lesions in the skin are created simultaneously using small electrodes. Recently different professional devices have been
25 launched onto the aesthetic market to address skin rejuvenation with a radio frequency device. Skin rejuvenation is a combination of different consumer benefits such as: even skin tone, reduction of pigmentation spots, improved radiance and texture and reduction of fine lines. Here the energy is used primarily to damage the stratum corneum and the epidermis (including the dermal-epidermal junction) and possibly the top part of the dermis.

Traditionally, skin rejuvenation treatments are done by ablative or non-ablative settings of a laser wavelength highly absorbed by water, whereby the ablative treatments vaporize the skin and create hollow pillars in the skin and the non-ablative treatments heat the skin to 65-100°C to initiate cell necrosis, collagen denaturation and contraction, and eventually collagen remodeling.

To date, fractional skin treatments using RF are limited to professional use. One possible reason is the safety of the treatment to ensure that the RF heating does not result in ablative damage to the skin tissue. This is particularly challenging since the amount of RF energy deposited in the tissue depends on local tissue impedance, and skin tissues have inhomogeneous impedance distribution. This uncertainty in impedance combined with the use of high current densities and voltages results in uncertainty in achieved temperatures in skin tissues during treatment, resulting in the occurrence of both non-ablative thermal lesions and the undesirable ablative tissue damages.

Patent application WO 2012/023129 describes an apparatus for personal aesthetic skin treatment by RF voltage. The apparatus includes an assembly of individual electrodes operative to contact fractions of the skin and deliver RF treatment voltage to each fraction. In a test mode of the apparatus, a test voltage is applied to the electrodes enabling determination of the quality of the contact between each of the electrodes and the skin. In the test mode no thermal lesions are generated in the skin. In a treatment mode, following the test mode, a treatment voltage is applied to generate thermal lesions in the skin. The test voltage does not exceed 50 Volt. The applied treatment voltage has higher values which lie between 50 Volt and 400 Volt.

SUMMARY OF THE INVENTION

It is an object of the invention to provide a device for RF skin treatment with improved safety in that it enables the generation of non-ablative fractionated skin lesions particularly by using a lower RF treatment voltage as compared to known devices, so that a feedback or monitoring system to detect proper contact between the electrodes and the skin is not required. For this purpose, according to a first aspect of the invention, a device for RF skin treatment is provided comprising an outer electrode arranged on an operational side of the device and having an annular or equilateral polygonal shape. The device comprises an inner electrode arranged on the operational side of the device at a center of the outer electrode and surrounded by the outer electrode. An RF generator is arranged to supply an RF treatment voltage between the inner electrode and the outer electrode. A skin contact surface

of the inner electrode has a largest cross-sectional dimension in a range of 200 - 500 μm , and the RF treatment voltage is less than 50 V. In an embodiment, the skin contact surface of the inner electrode is circular. In this embodiment, the largest cross-sectional dimension of the skin contact surface corresponds to a diameter of the skin contact surface and is in said range of 200 - 500 μm . The circular inner electrode may be annular (i.e. ring shaped) or disc shaped (i.e. having the shape of a filled circle). The inner electrode may also be non-circular, for example square-shaped, having a largest cross-sectional dimension within the range as mentioned above.

The proposed range of the largest cross-sectional dimension of the skin contact surface of the inner electrode of 200-500 μm enables, in combination with a relatively low treatment voltage of below 50 Volts, the generation of thermal lesions that are large enough for effective skin rejuvenation and small enough to enable fast recovery of the skin.

The inner and outer electrodes are configured to simultaneously make contact to the skin. The actual skin contact surface of the inner electrode does not need to be flat. It may be curved. This also applies to the actual skin contact surface of the outer electrode. In this respect, when the skin contact surface is flat, the expression "a largest cross-sectional dimension of the skin contact surface" refers to a largest dimension of the skin contact surface measured in the plane of the skin contact surface. When the skin contact surface is not flat, in particular when it is curved, the expression "a largest cross-sectional dimension of the skin contact surface" refers to a largest dimension measured in a cross-section of the inner electrode containing the outer circumference of the skin contact surface.

In an embodiment, the largest cross-sectional dimension of the skin contact surface of the inner electrode is in a range of 200-400 μm . Values for the largest cross-sectional dimension of the skin contact surface of the inner electrode within this preferred range have shown good results in ex-vivo skin tests.

In an embodiment, the RF treatment voltage is 40 V or less, such as 39 V. The above mentioned values for the largest cross-sectional dimension of the skin contact surface of the inner electrode enable sufficient warming of the skin, even with relatively low treatment voltages. It should be noted that the treatment voltage should not be too low, because in order to create lesions a sufficient amount of energy is required. Preferably the RF treatment voltage should not be lower than 20 volts when the RF exposure is less than 1s.

In an embodiment, a ratio between a skin contact surface of the outer electrode and the skin contact surface of the inner electrode is greater than 2 and preferably greater

than 10. In this way, there will be no discomfort by undesired heating in portions of the skin present beneath the outer electrode.

In an embodiment, a minimum distance between an outer edge of the inner electrode and an inner edge of the outer electrode is greater than 0.1 mm, more preferably greater than 0.2 mm. In a further embodiment, said minimum distance between the outer edge of the inner electrode and the inner edge of the outer electrode is smaller than 3 mm. There is no strict technical upper limit to said minimum distance (also referred to as gap between the inner and the outer electrodes), but for practical reasons to enable sufficient density of lesions from a grid of electrodes, for skin rejuvenation applications the gap should be smaller than 3 mm.

In an embodiment, the device comprises a plurality of inner electrodes and a plurality of outer electrodes, each of the plurality of outer electrodes surrounding a respective one of the plurality of inner electrodes. In this embodiment, at least some of the plurality of outer electrodes may be electrically connected to each other. In a preferred embodiment, the at least some of the plurality of outer electrodes may border each other so as to form a lattice structure. These embodiments require less wiring from the RF generator to the outer electrodes. Furthermore, more electrodes can be arranged on the same surface as compared to separate outer electrodes.

According to a second aspect, the invention relates to the use of the device as described above in the treatment of skin. The device may be used for therapeutic or non-therapeutic (e.g. cosmetic) treatment. The device is especially useful for rejuvenation of the skin, but may also be used for skin tightening.

Further preferred embodiments of the device and method according to the invention are described in the appended claims, disclosure of which is incorporated herein by reference.

BRIEF DESCRIPTION OF THE DRAWINGS

These and other aspects of the invention will be apparent from and elucidated further with reference to the embodiments described by way of example in the following description and with reference to the accompanying drawings, in which

Fig. 1A is a schematic cross section of a device for skin treatment according to an embodiment of the present invention;

Fig. 1B shows a view of an operational side of the electrode configuration of the device of Fig. 1A;

Figs. 2A-2C show examples of possible alternative embodiments of the inner electrode and the outer electrode;

Figs. 3A-3E show embodiments wherein the device comprises a plurality of inner electrodes and a plurality of surrounding outer electrodes;

5 Fig. 4 schematically shows a device for skin treatment according to an embodiment of the present invention, and

Figs. 5A-5C show three examples of histological sections of lesions created in ex-vivo skin samples.

The figures are purely diagrammatic and not drawn to scale. In the Figures, elements which
10 correspond to elements already described may have the same reference numerals.

DETAILED DESCRIPTION OF EMBODIMENTS

Fig. 1A is a schematic cross section of a device 100 for skin treatment according to an embodiment of the present invention. In this exemplary embodiment, the
15 device 100 comprises an inner electrode 1 and an annular (ring-shaped) outer electrode 2 surrounding the inner electrode 1. The device 100 also comprises an electronic controller 20, and a radio frequency (RF) generator 21 connected by wiring 22 to the electrodes 1 and 2. In this Figure, the electrodes 1, 2 are shown in a position on a skin surface 10 consisting of the stratum corneum 11, epidermis 12 and dermis 13. When powered, the electrodes 1, 2 create
20 electric field lines 5 within the skin and, due to the applied voltage in combination with the skin impedance, heat is deposited within the skin, thereby creating a non-ablative lesion 6, when the local skin temperature reaches a level above 65°C and stays under 100°C. The electronic controller 20 maybe arranged to control the RF generator 21. The RF generator 21 will provide a treatment voltage lower than 50 V. In some embodiments, the treatment
25 voltage may even be lower than 40 V. The electronic controller 20 may comprise an impedance detection system to measure skin impedance between the electrodes 1, 2, and a feedback controller based on the measured skin impedance. The electronic controller 20 may further comprise a feedback adjuster for adjusting the applied voltage or applied pulse duration.

30 Fig. 1B shows a top view of the electrode configuration of the device 100 shown in Fig. 1A, which is arranged on an operational side 15 of the device 100. The electrode configuration comprises the inner electrode 1 which is surrounded by the annular (ring-shaped) outer electrode 2. The inner electrode 1 is arranged at the center of the outer electrode 2. The specific electrode configuration of Fig. 1B comprising the inner electrode 1

and the surrounding annular outer electrode 2 is called a centrosymmetric electrode configuration. A skin contact surface of the inner electrode 1 is flat and has a diameter d_i in a range of 200 - 500 μm . A minimum distance between an outer edge of the inner electrode and an inner edge of the outer electrode is referred to as gap g_i . More particularly, the gap g_i is defined as the minimum distance between a point on the outer edge of the inner electrode 1 and a point on the inner edge of the outer electrode 2. In an embodiment, the gap g_i is greater than 0.1 mm, preferably greater than 0.2 mm. Practical values for the gap g_i lie below 3 mm.

Figs. 2A-2C show examples of alternative embodiments of the inner electrode 1 and the outer electrode 2. Fig. 2A shows an equilateral triangular-shaped outer electrode 2. Fig. 2B shows a square-shaped outer electrode 2. Fig. 2C shows an equilateral polygonal outer electrode 2 having a honeycomb shape.

It is noted that in most embodiments the inner electrode 1 will be the active electrode (i.e. the electrode connected to the live wire), while the outer electrode 2 is the return electrode, but this could be the other way round.

To create multiple lesions concurrently, the device may comprise a plurality of inner electrodes, wherein each inner electrode is surrounded by a respective one of a plurality of outer electrodes. Figs. 3A-3E show embodiments wherein the device comprises a plurality of inner electrodes 31 and a plurality of surrounding outer electrodes 32. Each of the plurality of outer electrodes 32 surrounds a respective one of the plurality of inner electrodes 31. The outer electrodes 32 may border each other so as to form a lattice structure as shown in the examples of Figs. 3A and 3C-3E, or they may just be electrically coupled as shown in the example of Fig. 3B. This will require less wiring from the RF generator to the outer electrodes. Furthermore, more electrodes can be arranged on the same surface as compared to separate outer electrodes.

Fig. 3A shows a linear array of coupled centrosymmetric round electrode pairs. Fig. 3B shows a linear array of non-coupled centrosymmetric round electrode pairs. Fig. 3C shows a two-dimensional array of coupled centrosymmetric round electrode pairs. Fig. 3D shows a linear array of coupled centrosymmetric equilateral triangular electrode pairs, and Fig. 3E shows a two-dimensional array of coupled centrosymmetric honeycomb electrode pairs.

By arranging a plurality of inner electrodes 31 on the operational side 15 of the device 100 and surrounding each by an outer electrode 32, a larger skin surface can be treated at one time as compared to devices that comprise only one electrode pair.

Fig. 4 schematically shows a device for skin treatment 40 according to another embodiment of the invention. The device 40 comprises a housing 41, a battery 42 and an electronic module 43. The electronic module 43 may comprise a PCB containing sensors, an RF generator, a feedback controller, and a function generator.

5 At the bottom, the device 40 comprises an inner electrode 46 and an outer electrode 47 provided on an operational side of the device 40. The inner electrode 46 and the outer electrode 47 may be configured as described above. The device 40 also comprises a button 44 that can be activated in order to provide pulses of RF energy between the inner and outer electrodes 46, 47.

10 The device 40 has an elongated shape which, when suitably dimensioned, can be used like a pen which can be brought into contact with the skin. This embodiment is especially useful as a home-use handheld skin treatment device for skin rejuvenation.

In an embodiment, a ratio between the skin contact surface of the outer electrode 47 and the skin contact surface of the inner electrode 46 is greater than 2, and preferably greater than 10.

15 The device described above was tested by performing ex-vivo experiments. These ex-vivo experiments have shown robust lesion creation at voltages of 40V or less, and the impedance variations within both ex-vivo and in-vivo skin models investigated are within the +/-25% range.

20 Figs. 5A-5C show three examples of histological sections of lesions created in an ex-vivo skin sample by NTBC (Nitro blue tetrazolium chloride) staining, demonstrating the area of cell damage within the epidermis and collagen coagulation within the dermis of the skin. The treatment RF voltage was set to 39V and the application time of the treatment RF voltage was 50 ms. A diameter of the inner electrode was 0.2 mm, while the annular outer electrode had an inner diameter of 1.5 mm. The gap between the outer edge of the inner electrode and the inner edge of the outer electrode was equal to 0.65 mm. The thickness of the outer electrode was 2 mm.

25 The invention also relates to the use of the device according to the embodiments described above for RF treatment of skin. The device is especially useful for rejuvenation of the skin.

30 When using the device for RF skin treatment, a contact gel may be used, preferably a conductive gel, to improve the local skin impedance and the electrical contact between the skin and the device.

It is noted that in this document the word 'comprising' does not exclude the presence of elements or steps other than those listed, and the word 'a' or 'an' preceding an element does not exclude the presence of a plurality of such elements, and it is also noted that any reference signs do not limit the scope of the claims. Further, the invention is not limited to the embodiments, and the invention lies in each and every novel feature or combination of features described above or recited in mutually different dependent claims.

CLAIMS:

1. A device (100) for RF skin treatment comprising:
 - an outer electrode (2) arranged on an operational side (15) of the device and having an annular or equilateral polygonal shape;
 - an inner electrode (1) arranged on the operational side (15) of the device at a center of the outer electrode and surrounded by the outer electrode (2);
 - an RF generator (21) arranged to supply an RF treatment voltage between the inner electrode (1) and the outer electrode (2);wherein a skin contact surface of the inner electrode has a largest cross-sectional dimension in a range of 200 - 500 μm , and wherein the RF treatment voltage is less than 50 V.
2. Device according to claim 1, wherein the largest cross-sectional dimension of the skin contact surface of the inner electrode is in a range of 200-400 μm .
3. Device according to any one of the preceding claims, wherein the RF treatment voltage is 40 V or less.
4. Device according to any one of the preceding claims, wherein a ratio between a skin contact surface of the outer electrode and the skin contact surface of the inner electrode is greater than 2, and preferably greater than 10.
5. Device according to any one of the preceding claims, wherein a minimum distance between an outer edge of the inner electrode and an inner edge of the outer electrode is greater than 0.1 mm, more preferably greater than 0.2 mm.
6. Device according to claim 4, wherein the minimum distance between the outer edge of the inner electrode and the inner edge of the outer electrode is smaller than 3 mm.
7. Device according to any one of the preceding claims, wherein the skin contact surface of the inner electrode (1) is disc-shaped.

8. Device according to any one of the claims 1 to 6, wherein the skin contact surface of the inner electrode (1) is annular.

9. Device according to any one of the preceding claims, wherein the device
5 comprises a plurality of inner electrodes and a plurality of outer electrodes, each of the plurality of outer electrodes surrounding a respective one of the plurality of inner electrodes.

10. Device according to claim 9, wherein at least some of the plurality of outer electrodes are electrically connected to each other.

10

11. Device according to claim 10, wherein the at least some of the plurality of outer electrodes border each other so as to form a lattice structure.

12. Use of the device according to any one of the preceding claims in the
15 treatment of skin, such as skin rejuvenation.

Fig. 1A

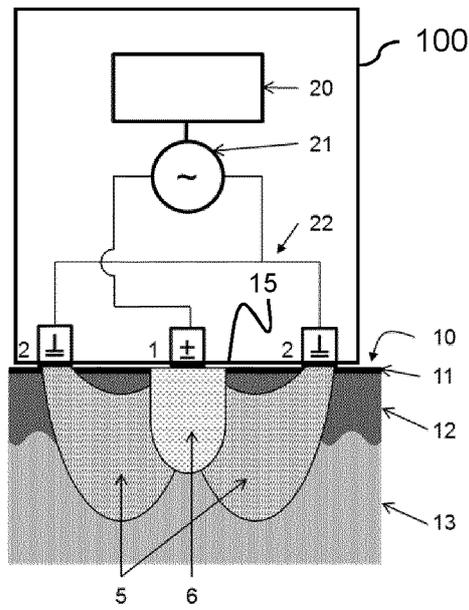


Fig. 1B

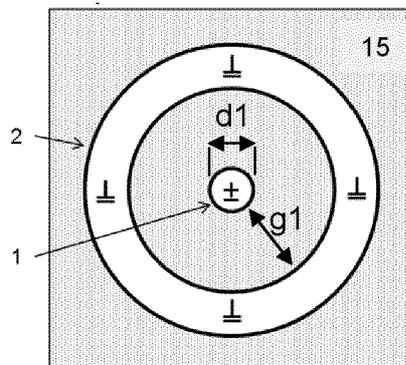


Fig. 2A




Fig. 2B

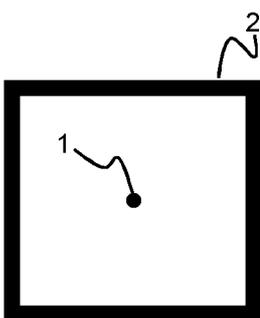



Fig. 2C



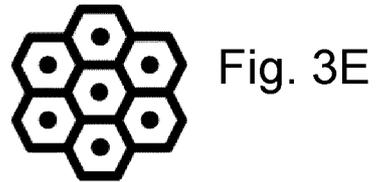
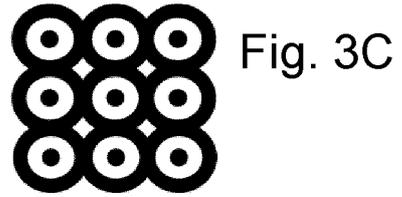
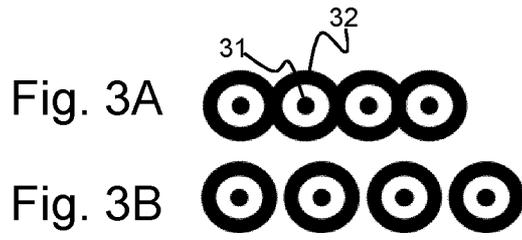


Fig. 4

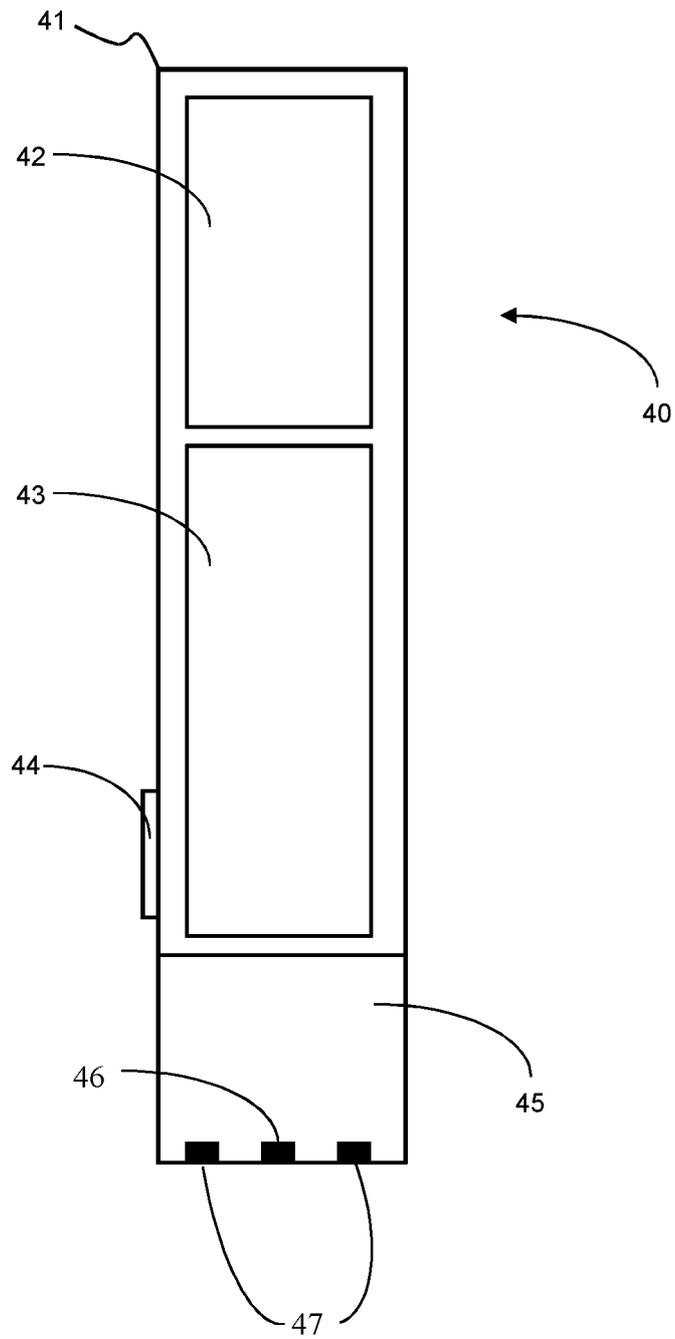


Fig. 5A

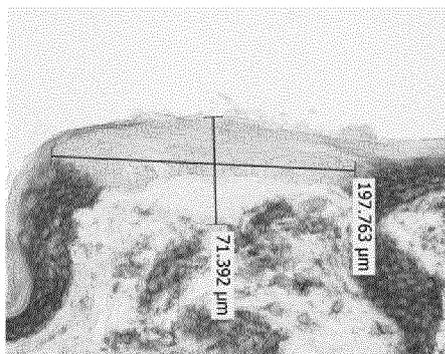


Fig. 5B


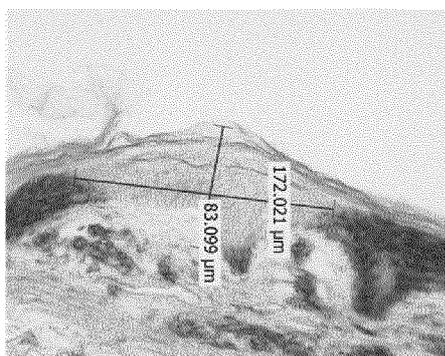


Fig. 5C

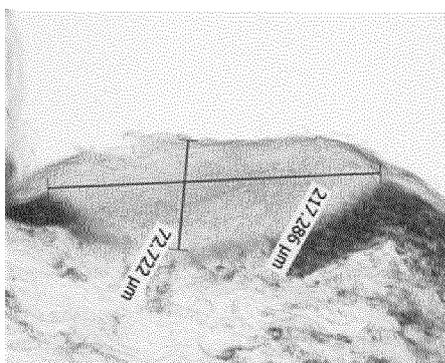

INTERNATIONAL SEARCH REPORT

International application No
PCT/EP2015/062313

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61N1/32 A61N1/40 A61N1/04
ADD. A61B18/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61N A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
EPO-Internal , WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	wo 2012/023129 AI (SYNERON MEDICAL LTD [IL]; ECKHOUSE SHIMON [IL]; FLYASH LION [IL]; VAYN) 23 February 2012 (2012-02-23) cited in the application	1,2,4-12
Y	abstract; figures 1-7 paragraphs [0027] - [0033] , [0041] - [0042]	3
Y	-----	
Y	US 2012/185029 AI (FLYASH LION [IL] ET AL) 19 July 2012 (2012-07-19)	3
A	abstract; figures 1A-C, 5 paragraphs [0029] - [0032] , [0042] - [0045]	1,2,4-12
A	-----	
A	DE 10 2011 053731 AI (GARBARTSCHUK WASSI LI [DE]) 21 March 2013 (2013-03-21) the whole document	1-12

	-/-	

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search 17 August 2015	Date of mailing of the international search report 28/08/2015
--	---

Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer Lahorte, Philippe
--	--

INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2015/062313

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2013/226269 A1 (ECKHOUSE SHIMON [IL] ET AL) 29 August 2013 (2013-08-29) abstract; figures 2C-3 paragraphs [0024] - [0034] -----	1-12

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/EP2015/062313
--

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
wo 2012023129	AI	23-02-2012	AU 2011292747 AI 14-03-2013
			EP 2605718 AI 26-06-2013
			JP 2013534167 A 02-09-2013
			KR 20140005124 A 14-01-2014
			US 2013289679 AI 31-10-2013
			Wo 2012023129 AI 23-02-2012

US 2012185029	AI	19-07-2012	AU 2008332738 AI 11-06 -2009
			CN 101969873 A 09-02 -2011
			CN 102688089 A 26-09 -2012
			EP 2219544 A2 25-08 -2010
			EP 2394594 AI 14-12 -2011
			ES 2455196 T3 14-04 -2014
			JP 2011505899 A 03-03 -2011
			KR 20100106306 A 01-10 -2010
			KR 20120035236 A 13-04 -2012
			KR 20120135429 A 13-12 -2012
			US 2009299361 AI 03-12 -2009
			US 2012185029 AI 19-07 -2012
			US 2014171934 AI 19-06 -2014
			wo 2009072108 A2 11-06 -2009

DE 102011053731	AI	21-03 -2013	NONE

US 2013226269	AI	29-08 -2013	JP 2014508542 A 10-04 -2014
			KR 20130122948 A 11-11 -2013
			US 2013226269 AI 29-08 -2013
