



(86) Date de dépôt PCT/PCT Filing Date: 2005/05/23

(87) Date publication PCT/PCT Publication Date: 2005/12/01

(85) Entrée phase nationale/National Entry: 2006/11/20

(86) N° demande PCT/PCT Application No.: US 2005/018087

(87) N° publication PCT/PCT Publication No.: 2005/113035

(30) Priorité/Priority: 2004/05/21 (US60/573,710)

(51) Cl.Int./Int.Cl. **A61B 17/12** (2006.01),
A61L 31/16 (2006.01)


(71) Demandeur/Applicant:
MICRO THERAPEUTICS, INC., US

(72) Inventeurs/Inventors:
PATTERSON, WILLIAM R., US;
SLEE, EARL H., US;
WILDER, TOM, US;
MCCARTHY, THOMAS, US;
STRAUSS, BRIAN, US;
MONSTADT, HERMANN, DE;
HENKES, HANS, DE

(74) Agent: OGILVY RENAULT LLP/S.E.N.C.R.L.,S.R.L.

(54) Titre : SPIRES METALLIQUES ENTRELACEES DE POLYMERES OU FIBRES BIOLOGIQUES OU
BIODEGRADABLES OU SYNTHETIQUES, DESTINEES A L'EMBOLISATION D'UNE CAVITE CORPORELLE

(54) Title: METALLIC COILS ENLACED WITH BIOLOGICAL OR BIODEGRADABLE OR SYNTHETIC POLYMERS OR
FIBERS FOR EMBOLIZATION OF A BODY CAVITY

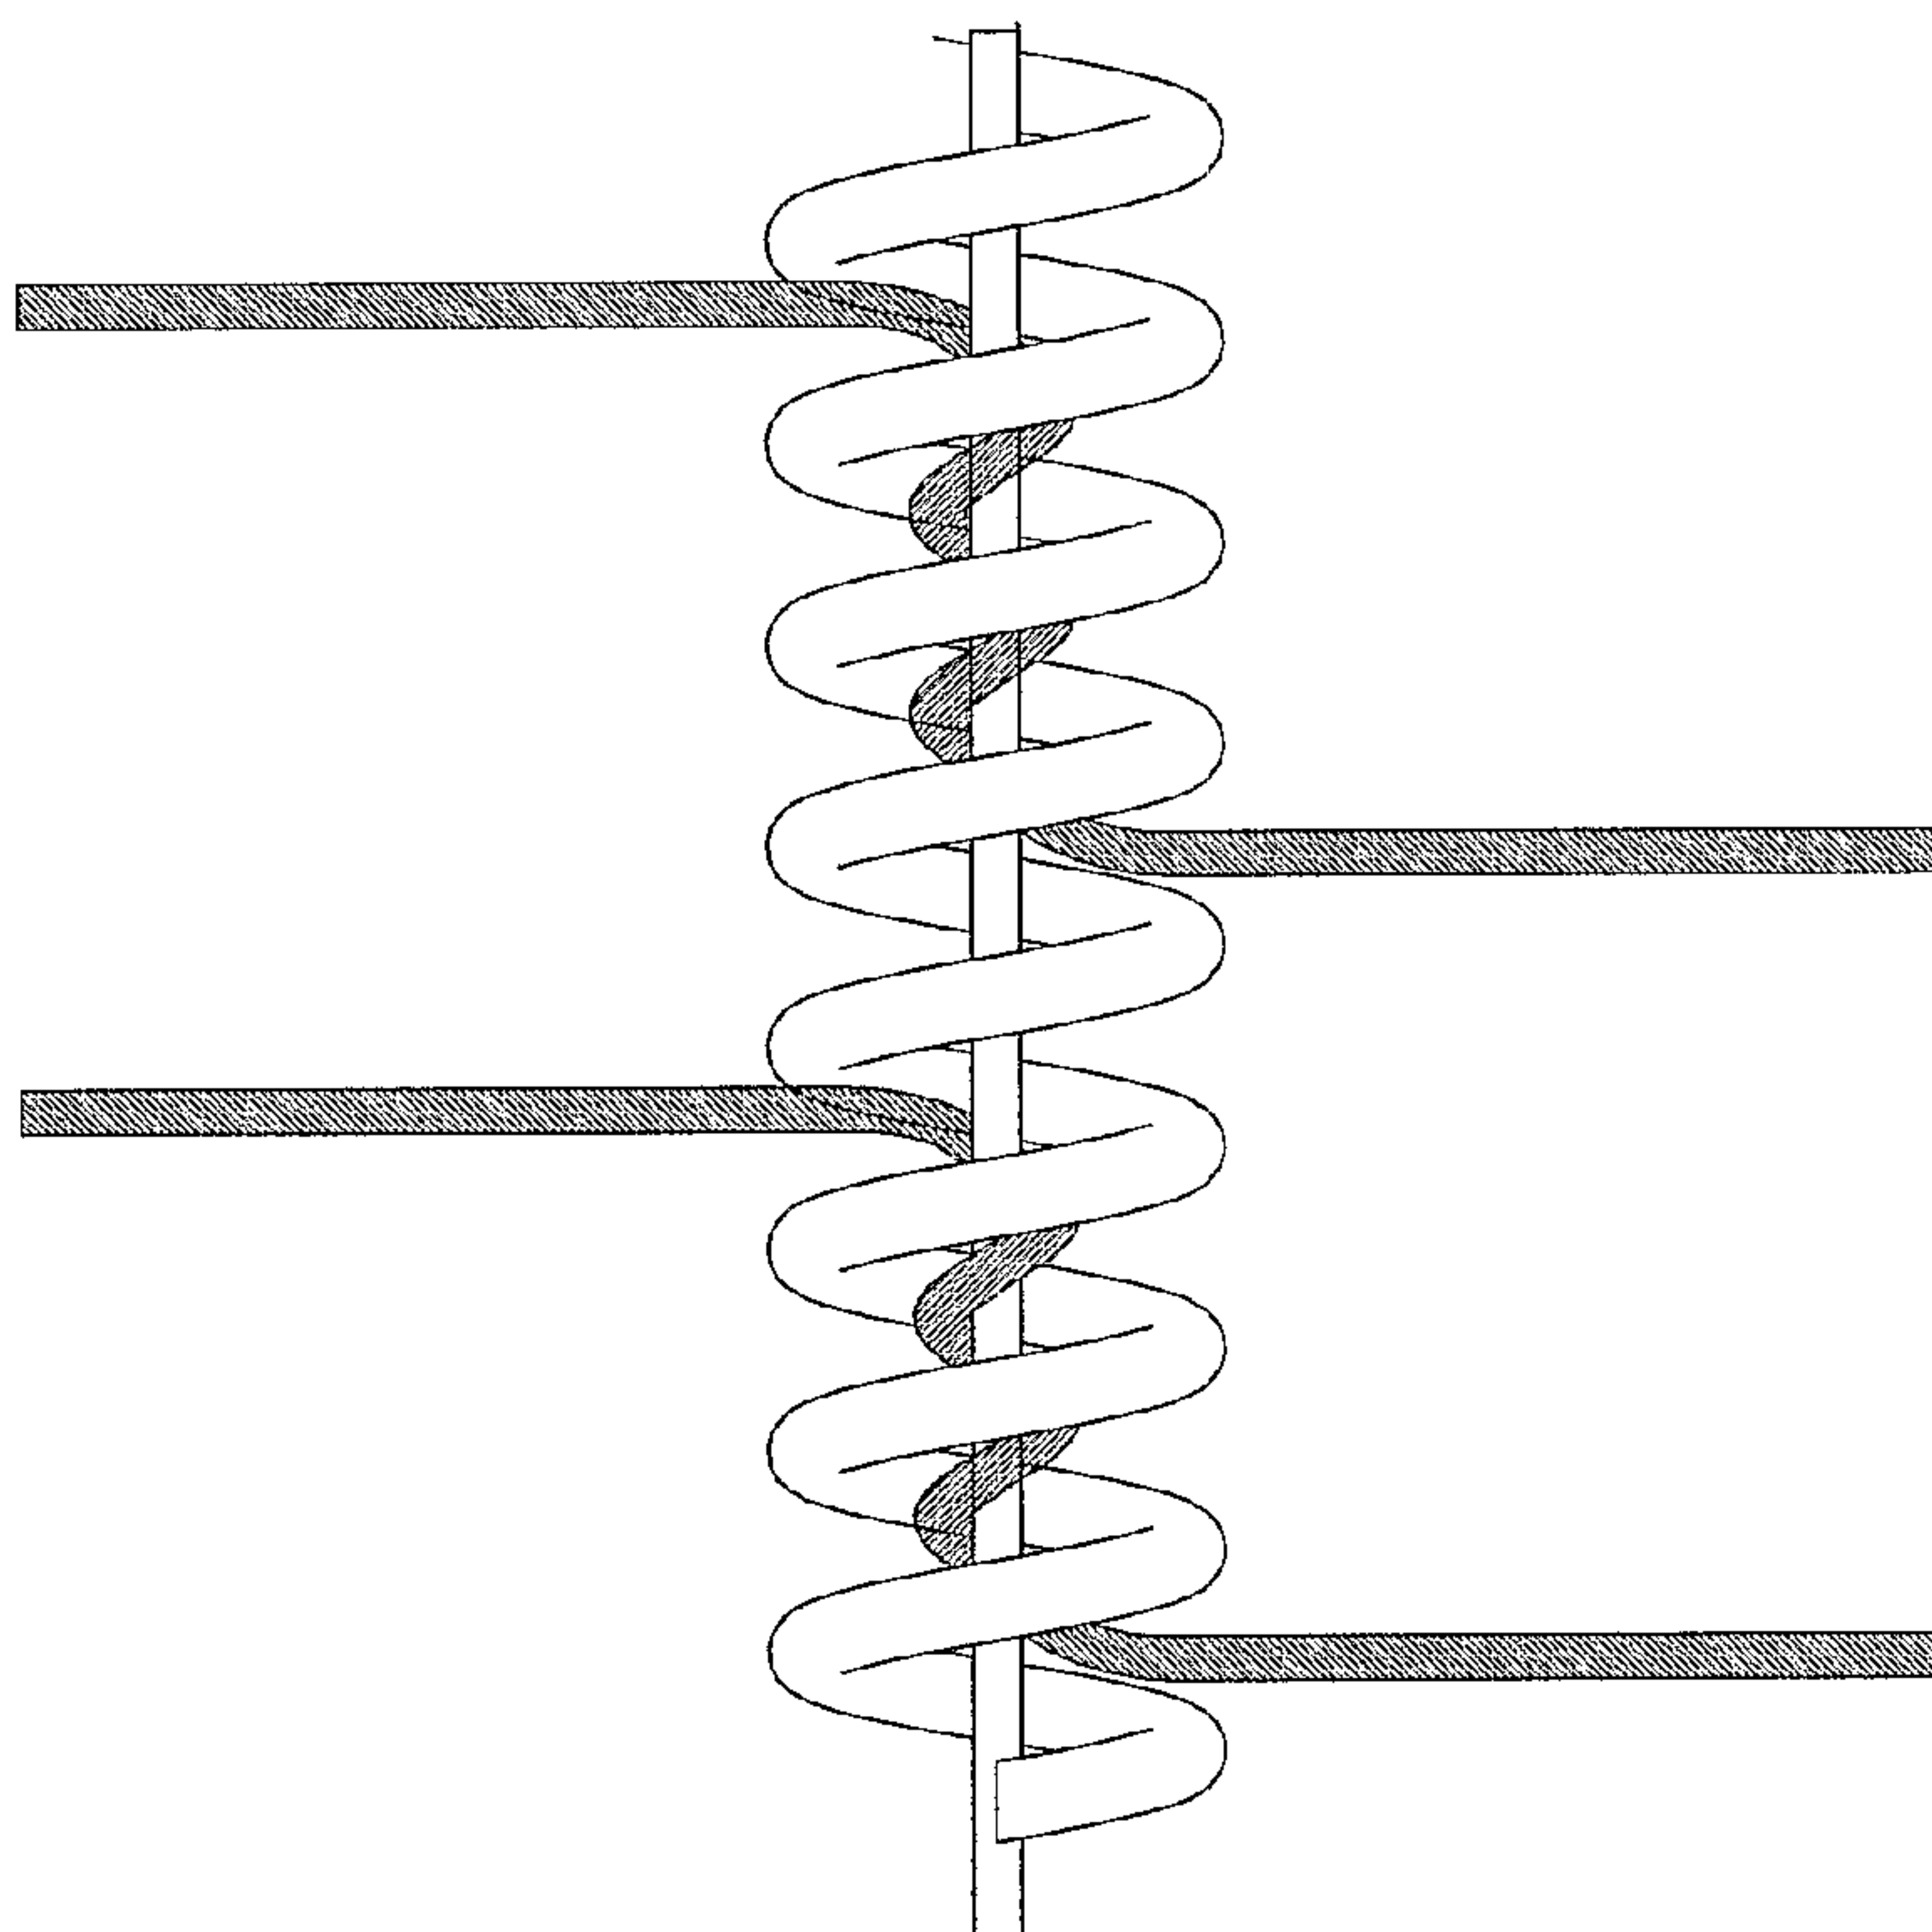

(57) **Abrégé/Abstract:**

Vaso-occlusive coils comprising fibers. The vaso-occlusive coil (12) can be a helical coil or a double helix made of biocompatible metal wire whereas the fibers (14, 16, 18, 28) are enlaced between at least a winding of the coil (12) and are made of polymeric materials like copolymers of glycolic/lactic acid. The fibers (14, 16, 18, 28) or the coil (12) can be coated with a bioactive material. The device (10) can comprise a stretch-resistant member and can be radio-opaque.



(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
1 December 2005 (01.12.2005)

PCT

(10) International Publication Number
WO 2005/113035 A3

(51) International Patent Classification⁷: **A61B 17/12**,
A61L 31/16

MONSTADT, Hermann [DE/DE]; Haarstrasse 61, 11797
Bochum (DE). **HENKES, Hans** [DE/DE]; Im Mailand
10, 44797 Bochum (DE).

(21) International Application Number:
PCT/US2005/018087

(74) Agent: **MITTLER, E., Stewart**; Kudirka & Jobse, LLP,
One State Street, Suite 800, Boston, MA 02109 (US).

(22) International Filing Date: 23 May 2005 (23.05.2005)

(25) Filing Language: English

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KM, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA,
MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO, NZ,
OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL,
SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC,
VN, YU, ZA, ZM, ZW.

(26) Publication Language: English

(30) Priority Data:
60/573,710 21 May 2004 (21.05.2004) US

(71) Applicant (*for all designated States except US*): **MICRO
THERAPEUTICS, INC.** [US/US]; 2 Goodyear, Irvine,
CA 92618 (US).


(72) Inventors; and

(84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO,
SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN,
GQ, GW, ML, MR, NE, SN, TD, TG).

(75) Inventors/Applicants (*for US only*): **PATTERSON,
William, R.** [US/US]; 90 Windjammer, Irvine, CA 92614
(US). **SLEE, Earl, H.** [US/US]; 7 White Sail, Laguna
Niguel, CA 92677 (US). **WILDER, Tom** [US/US]; 1841
Port Sheffield Place, Newport Beach, CA 02660 (US).
MCCARTHY, Thomas [US/US]; 2850 Calle Guadala-
jara, San Clemente, CA (US). **STRAUSS, Brian** [US/US];
20592 Porter Ranch Road, Trabuco Canyon, CA (US).

[Continued on next page]

(54) Title: METALLIC COILS ENLACED WITH BIOLOGICAL OR BIODEGRADABLE OR SYNTHETIC POLYMERS OR
FIBERS FOR EMBOLIZATION OF A BODY CAVITY

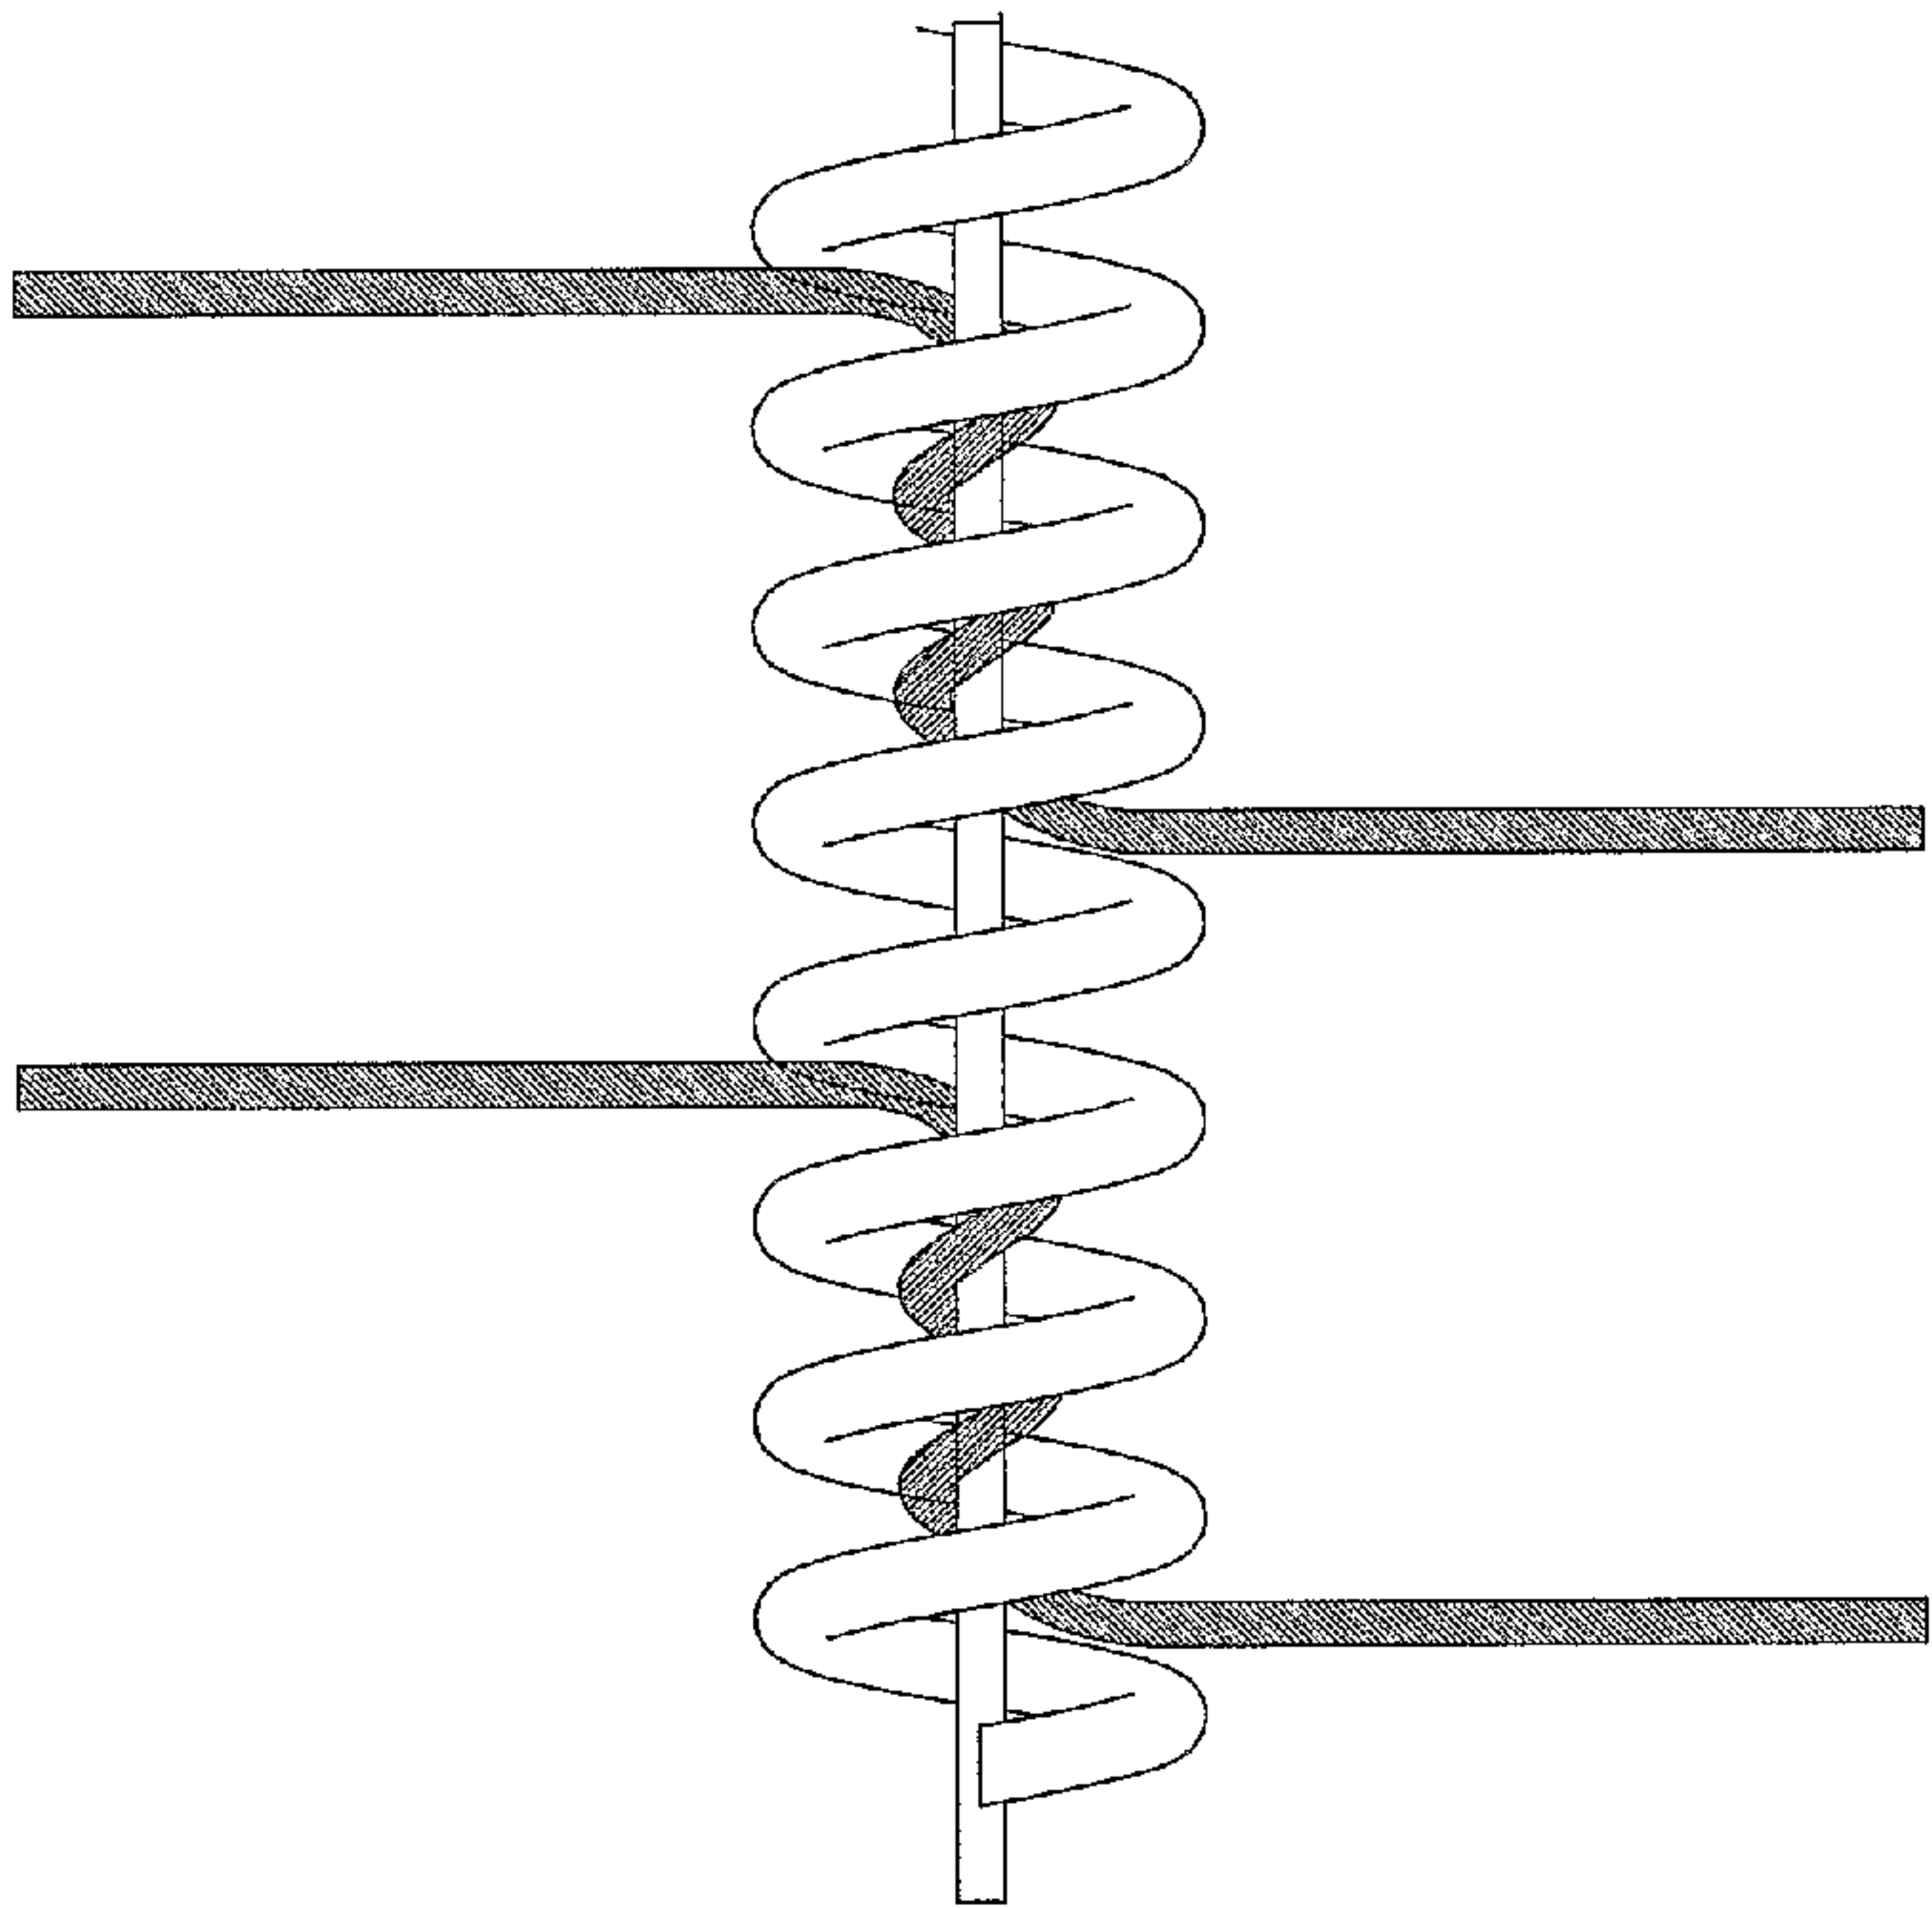

(57) Abstract: Vaso-occlusive coils comprising fibers. The vaso-occlusive coil (12) can be a helical coil or a double helix made of biocompatible metal wire whereas the fibers (14, 16, 18, 28) are enlaced between at least a winding of the coil (12) and are made of polymeric materials like copolymers of glycolic/lactic acid. The fibers (14, 16, 18, 28) or the coil (12) can be coated with a bioactive material. The device (10) can comprise a stretch-resistant member and can be radio-opaque.

WO 2005/113035 A3

WO 2005/113035 A3



Published:

- *with international search report*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(88) Date of publication of the international search report:

23 February 2006

**METALLIC COILS ENLACED WITH BIOLOGICAL OR
BIODEGRADABLE OR SYNTHETIC POLYMERS OR
FIBERS FOR EMBOLIZATION OF A BODY CAVITY**

Field of the Invention

[001] This invention relates to vaso-occlusion devices for forming an occlusion (embolism) at a desired vascular location, in particular at the site of an aneurism. The devices are helical wire coils preferably with enlaced fibrous materials providing an increased surface area to facilitate high rates of desired bioactions such as bioactive material release or embolic interactions between the device's surface and the patient's bloodstream. The coils may be coated with at least a single layer including a bioactive material.

Background

[002] Body cavity embolism (e.g. brain blood vessel aneurysm occlusion by detachable coils, liquid embolism, particle embolism, balloon embolism) is a treatment that may have a high incidence of recurrence. Due to insufficient healing at the aneurysm/parent artery interface, mechanical and biological forces, incompletely understood, create a new expansion of aneurysm. That is the aneurysm reforms or recurs after endovascular, embolic treatment.

[003] In one treatment Pt/Ir coils are packed in aneurysms so that they occupy ~ 20% to 30% of the aneurysm volume and reduce the inflow of blood into the aneurysm. Aneurismal blood, at 70% to 80% by volume, clots by

stagnation. Preferably, the clotted blood organizes and proceeds through a series of steps similar to those occurring at any wound in the body: (1) hemostasis, (2) inflammation, (3) tissue formation, and (4) remodeling. An aneurysm so treated is excluded from the arterial circulation. On the other hand, for partially understood reasons, the clotted blood may not organize, the coil mass compacts and/or new blood flow—coupled with the diseased arterial tissue—allows expansion of the aneurysm. Thus the aneurysm recurs and remains susceptible to rupture and hemorrhagic stroke.

[004] With the pursuit of tissue engineering, devices were created that attempt to direct or enhance the healing of the aneurysm/artery interface rather than rely on each patient's individual reaction to the embolism of the aneurysm cavity. Embolic devices, such as electrolytically-detached Pt/Ir coils, have been designed with coatings that swell in aqueous solution or that provoke a mild inflammatory response.

[005] One form of device contains a polyacrylamide hydrogel attached to the Pt/Ir detachable coil. As the coil resides in blood, the hydrogel swells and occupies more space than bare metal coils, leading to higher packing densities (~40% to 50%).

[006] Other coils use the biodegradable polymer PGLA (poly glycolic/lactic acid—the same material used in absorbable sutures) as a bioactive coil coating to provoke a mild inflammatory response in the aneurysm that triggers aneurismal organization per the above wound healing steps.

[007] Both approaches suffer from the same problem: they are limited by the small size of these coils and the fact that the coils must be delivered through a microcatheter with the smallest ID of ~0.015". Coils may have a minimum of 0.09 cm of surface area (0.01 1" OD, over a 1 cm length). Placing a coating, hydrogel or bioactive coating, and ensuring that the treated coil can move through a 0.015" ID catheter places a finite limit on the amount of hydrogel or bioactive coating applied to the coil. In general, the amount of material is limited by the surface of the coil and the delivery catheter. Limited to no efficacy data exist for the coated coils. However, physician feedback indicates that the results are no better than bare-metal coils.

[008] Helical coils are one form of device that has been extensively employed. Hans Henkes, et al., NEUROSURGERY 54, No. 2, 268 (2004) describe the results of over 1800 procedures involving helical coils and conclude that such devices are safe and efficacious for occlusion for patients with intracranial aneurysms.

[009] A number of variations on helical coils have been proposed heretofore. For example, United States Patent Number 5,226,911 issued to Chee and Narient describes looping 5 to 100 biocompatible polymer fibers through the helical coils. Dacron, polyglycolic acid, polylactic acid, fluoropolymers, nylon and silk are among the polymers suggested for these fibers. United States Patent Number 5,382,259 issued to Phelps and Van describes braided or woven fibrous tubular coverings with and without tassels for helical coils. United States Patent Number 5,549,624 issued to Mirigian and Van describes a helical coil device with added fibrous loops which are

described as increasing the device's thrombogenicity. United States Patent Number 5,658,308 issued to Snyder describes a helical metal device with from one to several hundred axial fibrous strands passing through its center and optionally filaments attached to the windings of the coil. These filaments are recited to be bioactive or nonbioactive and to enhance the ability of the coil to occlude the site at which it is placed. United States Patent Number 5,935,145 issued to Villar and Aganon describes helical coils two fibrous members, each of a different material, attached. One of the materials is preferably biodegradable. The other is preferably not biodegradable. United States Patent Number 6,299,627 issued to Eder et al. describes devices with coils or braids and two coatings including an inner coating and another coating selected to affect the solubility of the inner coating.

[0010] All of this work suggests that although helical coil inserts are attractive vasoocclusive devices there are opportunities to improve their performance to achieve optimal performance in terms of ease of delivery to and placement at the treatment site and in terms of the degree and rate of vaso-occlusion achieved.

SUMMARY OF THE INVENTION

Statement of the Invention

[0011] We have now discovered improvements to vaso-occlusion devices comprised of a coil, e.g., a metallic coil enlaced with biological, biodegradable or synthetic polymer fibers.

[0012] A need exists for an embolic device that can increase the effective surface area so that higher levels of biological, biodegradable, or synthetic agents can be present to embolize a body cavity and direct or provoke a healing response.

[0013] We sought to provide more surface area to an embolic coil device by adding fibers. By increasing initial blood contact surface area between aneurismal blood and tissue, bioactive agents (biological, biodegradable, or synthetic) can be used at higher concentrations or in greater amounts than previously used. The same concentration or amount can be spread over a larger contact surface area.

[0014] More particularly, we have discovered that providing a large but controlled additional surface area to a helical coil device in the form of fibers enlaced into the coil provides an improved device. The amount of additional surface area provided by the enlaced fibers should be at least 0.1 times the surface area provided by the metallic coil itself, to as much as 10 or greater times the surface area provided by the metallic coil itself.

[0015] Thus, this invention provides a vaso-occlusion device comprising:

(a) a helical coil of 0.025 mm or larger metal wire, the coil sized for insertion to a point of use in the vascular network of a patient for occluding blood flow and having a plurality of windings and having a first surface area and

(b) a plurality of fibrous elements enlaced through the helical coil and having outwardly extending ends, said fibrous elements presenting a bioactive outer surface and collectively having a second surface area with the second surface area being at least 0.1 times the first surface area.

[0016] In one embodiment the majority of the fibrous elements each enlace a single winding of the helical coil. In additional embodiments the majority of the fibrous elements each enlace two or more windings of the helical coil.

[0017] The fibrous elements can be made of a bioactive material or a nonbioactive material. They can be stable in the conditions of use or they can undergo biodegradation in that setting. They can include a coating of bioactive material on a core of nonbioactive material or on a core of bioactive material. They may include a coating comprised at least partially of a nonbioactive material. The bioactive material can be a naturally-occurring material or a synthetic material. Synthetic material may include any material made by the human hand including, but not limited to engineered versions of naturally occurring material, e.g., molecules.

[0018] An exemplary family of materials for forming the fibers or for coating the fibers include copolymers of glycolic acid with lactic acid copolymers.

[0019] In other embodiments this invention provides methods of producing these devices by enlacing fibers, before or after coating, into the

helical coils as well as methods for treating a patient to embolize a body site by placing a device of this invention at the site in need of embolization.

BRIEF DESCRIPTION OF THE DRAWINGS

[0020] This invention will be further described with reference being made to the accompanying drawings in which:

[0021] Figure 1 is a not-to-scale side view of a vaso-occlusive coil showing three representative embodiments of the fibers which are present enlaced into it. Three areas are identified in Fig. 1. Area 2-2' shows an embodiment where the fibers are enlaced around a single loop of the coil. Area 3-3' shows an embodiment where the fibers are enlaced through a single loop of the coil. Area 4-4' shows an embodiment where the fibers are enlaced through a plurality of loops of the coil.

[0022] Figure 2 is an expanded scale view of the 2-2' area of Fig 1 which shows an embodiment where the fibers are enlaced around a single loop of the coil.

[0023] Figure 3 is an expanded scale view of the 3-3' area of Fig 1 which shows an embodiment where the fibers are enlaced through a single loop of the coil.

[0024] Figure 3' is an expanded scale view of the 3-3' area of Fig 1 which shows an embodiment where the fibers are enlaced through a pair of loops of the coil.

[0025] Figure 4 is an expanded scale view of the 4-4' area of Fig 1 which shows an embodiment where the fibers are enlaced in an "S" pattern through a plurality of loops of the coil.

[0026] Figure 5 is an expanded scale view similar to Fig 4 with a variation in the way the fibers are enlaced. In this embodiment two sets of fibers are enlaced adjacent to each other in "S" patterns on the coil.

[0027] Figure 6 is a not-to-scale partial cross section of a type of fiber or a type of coil useful in the present invention having a core and an outer coating.

[0028] Figure 7a is a not-to-scale side view of an example of one embodiment of the invention comprising a vaso-occlusive coil which includes a stretch resistant member fixedly attached to the coil and a plurality of fibers, where each fiber is wrapped around the stretch resistant member at least twice.

[0029] Figure 7b is a not-to-scale top view of the embodiment of the invention shown in Figure 7a.

Detailed Description of the Invention

[0030] This detailed description is broken down into the following sections.

Metal Coils and Device Configurations

Stretch Resistant Members

Fiber Materials

Bioactive Materials

Applications

Metal Coils and Device Configurations

[0031] The vaso-occlusion devices of this invention are made up of a coil, e.g. a metal coil preferably with enlaced fibers pendant therefrom. In certain embodiments the devices are in the form of a helix and may be comprised of a simple single helix. In other embodiments, however, the coils are coils on coils having a primary helical coil wound into a secondary helix or other secondary shape with fibers enlaced through the primary coil such as shown in Figure 1. In Figure 1 a device 10 is shown having a metal coil 12 having a large or secondary helix having a diameter D_s and a small or primary helix having a diameter D_p . A plurality of fibers 14, 16, and 18 are shown enlaced through the coils of the primary helix in configurations captured in lines 2-2', 3-3' and 4-4' and thereafter depicted in expanded scale in Figures 2, 3, 3' and 4 respectively. It will be appreciated that these four enlacing configurations are merely representative and that equivalent configurations which suitably associate the fibers with the coils are also contemplated within the scope of this invention.

[0032] The wire making up the coil 12 may be a biocompatible metal, that is a metal that does not react adversely with the tissues and fluids it comes in contact with when used in the body. The metals may also be radio opaque so that the position and location of the coils in the body can be monitored with radiological techniques. Suitable metals include, but are not

limited to the noble metals such as the platinum group metals which include platinum, palladium, rhodium and rhenium as well as iridium, gold, silver, tungsten, and tantalum and alloys of these metals with one another. Additional useful metals may include the super elastic metals such as "Nitinol" and the like. These materials are described in the art such as in United States Patents Number 3,174,851 and 3,753,700 and can include nickel-titanium alloys having about 0.4 to about 0.5 molar fraction nickel and 0.5 to 0.6 molar fraction titanium; aluminum-nickel alloys having about 0.35 to 0.4 molar fraction aluminum; and the like. Platinum-iridium and platinum-tungsten alloys having predominant fractions of platinum are most preferred metals.

[0033] The metal component may be comprised of a wire. In certain embodiments the wire commonly has a diameter of from about 0.025 to about 0.09 mm, from about 0.03 to about 0.08 mm from about 0.04 to about 0.06 mm. In certain specific embodiments the wire has a diameter of about 0.05 mm. In some embodiments the wire may be comprised only of a primary shape e.g., a simple single helix. In some embodiments the wire component may comprise a primary shape e.g., helical coil and a secondary shape. The secondary shape may comprise a complicated three dimensional shape. In other embodiments the wire can comprise a coil of coils or double helix. When it is a coil of coils, the outer or secondary diameter of the outer helix may be from about 1 to about 25 mm in some embodiments and from about 2 to 20 mm in certain other embodiments. The primary (inner) helix may typically have an outside diameter of from about 0.1 to about 0.8 mm in some

embodiments, and from about 0.15 to about 0.6 mm in other embodiments and from about 0.2 to about 0.4 mm in yet other embodiments. Certain specific embodiments provide for coils having a primary diameter of about 0.28 mm sized to pass through a correspondingly dimensioned catheter. Yet other embodiments provide for coils having a primary diameter of about 0.24mm sized to pass through a correspondingly dimensioned catheter.

[0034] The secondary helix may have from about 0.5 to about 20 windings per cm in some embodiments and from about 1 to about 10 windings per cm in other embodiments. The inner or primary coil may have from about 2 to about 50 windings per mm in some embodiments and from about 5 to about 40 windings per mm in other embodiments. These primary coil winding values are determined on the primary coil without added fibers. As fibers are added they typically expand the primary helix to some degree as they enlace through the primary helical coils. Thus, in Figures 1, 2, 3 and 4 the primary helix coils are depicted with a pitch that allows for free space between adjacent coils. As shown in Figures 2 and 3, for example, this extra spacing between the coils is shown to make up to about 60% of the overall secondary helix length. While this configuration is certainly acceptable in many settings, in other settings it may be desirable to have the spacing between the coils small enough (or nonexistent) so as to permit the fibers, when added, to distort the coil and permit the coil to apply pressure to grip the fibers and hold them in place. This latter situation is referred to as a "fiber gripping" configuration for the primary coil. Accordingly, in certain embodiments the extra spacing between adjacent primary coil windings can range from about 0

% to about 80% of the overall unstretched primary helix length. A fiber-gripping configuration may be achieved when the extra spacing between adjacent coils is in the range of from about 0% to about 25% of the total length.

[0035] The unstretched overall axial length of the devices of this invention ranges from about 5 to about 400 mm in some embodiments and from about 10 to about 300 mm in other embodiments. This length may be selected depending upon the particular application of use and may be longer than 400 mm in some embodiments.

[0036] As can be seen in Figures 1 through 7, there are many possible configurations for the fibers which are present in the devices of the invention. The materials making up these fibers will be described in the section entitled Fiber Materials. The configuration of the fibers is set forth below.

[0037] In certain embodiments, the fibers that comprise part of the devices of the invention are enlaced through the primary coils of the helices. In other embodiments the fibers that comprise part of the devices of the invention are wrapped at least twice around a stretch resistant member disposed within the central lumen of the coil, typically attached at each end thereof. In some embodiments the fiber may be tied to the coil or the stretch resistant member, e.g., via a knot. The fiber may be tied and laced around the coil or the stretch resistant member or both. In other embodiments the fiber is not tied or knotted, but is laced or wound around the coil or the stretch

resistant member or both. The fibers may be flexible and may be cut to shorter lengths to accommodate coil delivery through a microcatheter.

[0038] As shown in Figure 2, one suitable lacing configuration may include fibers laced around a single coil 20 of the primary helix with both ends of a single fiber 14 extending radially from the coil 12 in the same general direction. This can occur with a single fiber such as 14c-14c' or with a plurality of fibers 14e-14e'. The fibers may be comprised of monofilaments or yarns. The fibers may be comprised of single fibers or bundles of associated fibers. The bundles of fibers may range from two fibers to about 50 fibers or more. The fibers are not drawn to scale in any of these drawings. In certain embodiments, they may extend from the secondary coil at least about 0.05 mm. In other embodiments they may extend from the secondary coil about 0.05 to about 5 mm. In yet other embodiments they may extend from the secondary coil about 0.5 mm to about 4 mm. As will be apparent, these dimensions are relatively small as compared to D_s shown in Figure 1, but comparable to or larger than D_p . The fibers may have diameters ranging from about 0.01 mm to about 0.60 mm in some embodiments. In other embodiments the fibers may have diameters ranging from about 0.02 mm to about 0.05 mm. In the case of yarns, the overall yarn diameter will typically be in these ranges with the individual filaments making up the yarn being smaller in diameter.

[0039] As noted previously, it is often advantageous for the diameter of the fiber or bundle of fibers to exceed the space between windings of the primary helix so that the space is a fiber-gripping distance.

[0040] As shown in Figure 3, one embodiment of the invention contemplates enlacing the fibers 16 such that they extend out of opposite sides of the primary winding 12. In this embodiment a single fiber 16a-16a' can enlace and pass by a single coil 22 of helix 12. Similarly a bundle of fibers 16b-16b' can enlace and pass by a single coil 22'. In this configuration it is advantageous to have the spacing between adjacent windings of the primary coils to be a fiber-gripping distance. The fibers in this embodiment may be of similar dimensions to those set forth in Figure 2.

[0041] As shown in Figure 3', variations on the lacing pattern of Figure 3 are contemplated. Thus, a bundle of fibers 16c-16c' or an individual fiber 16d-16d' may be laced through a pair of adjacent coils 24 and 24' in the primary helix. This configuration may advantageously provide a fiber-gripping spacing between adjacent coils.

[0042] As shown in Figures 4 and 5, the fibers that are enlaced through the primary helix of the coil may be enlaced back and forth across the coil in an "S" configuration to facilitate gripping of the fibers by the coil and minimize the likelihood that they are dislodged in use. In Figure 4, a bundle of fibers 28 first laces through windings 32 and 34 of coil 12 leaving a tail 30 extending a suitable distance as set forth above. Next the bundle 28 forms loop 38 spanning a number of windings 36. This number may be as small as one winding or may be as large as 10-12 windings. In certain embodiments the number of windings may be substantially larger than 12. Thus certain embodiments of the invention provide at least one winding looped by a fiber, e.g. 38 in Figure 4. Then the fibers may be enlaced through windings 40 and

42 and out the other side of coil 12 to form a corresponding opposite loop 46 which spans a number of windings 44 which may be about the same as the number of windings described for 38. The fibers may then be enlaced through windings 48 and 50 and end at 28' to form a tail 52 similar to tail 28.

[0043] Figure 5 shows that multiple bundles forming the double looped "S" configuration 28 and 28A through 28' and 28A' are also contemplated. These multiple loops may be arrayed parallel to one another and enlace adjacent windings as depicted in Figure 5 but may also vary from one another and be more random, if desired.

Stretch Resistant Members

[0044] The device of the invention may be comprised of a stretch resistant member. The stretch resistant member may prevent movement or elongation or deformation of the device e.g., during retrieval or repositioning. The stretch resistant member may be fixedly attached to at least one end of the device. In certain embodiments it may be fixedly attached to both ends of the device. In some embodiments, the stretch resistant member may axially traverse the interior region or lumen of the coil.

[0045] The stretch resistant member may be made from a wide variety of materials. These include any of the materials, e.g., metals, described as suitable for making the coil. The stretch resistant member may be comprised of a radiopaque material. It may also be comprised of a polymer.

[0046] In certain embodiments at least one fiber is wrapped at least two times round the stretch resistant member. In certain embodiments the invention provides for a plurality of fibers, e.g. at least one bundle or a plurality of bundles wrapped at least two times round the stretch resistant member. Wrapping the fiber around the stretch resistant member at least twice advantageously provides a means of securing at least one fiber to the device. In certain embodiments the fiber may not be tied or knotted to the device thereby avoiding potentially obstructive bundles which might hinder deployment of the device or might mechanically damage the device.

Fiber Materials

[0047] In certain embodiments, the fibers may be comprised of polymeric materials. The polymeric materials may include materials approved for use as implants in the body or which could be so approved. They may be nonbiodegradable polymers such as polyethylene, polyacrylics, polypropylene, polyvinylchloride, polyamides such as nylon, e.g., Nylon 6.6, polyurethanes, polyvinylpyrrolidone, polyvinyl alcohols, polyvinylacetate, cellulose acetate, polystyrene, polytetrafluoroethylene, polyesters such as polyethylene terephthalate (Dacron), silk, cotton, and the like. In certain specific embodiments the nonbiodegradable materials for the polymer component may comprise polyesters, polyethers, polyamides and polyfluorocarbons.

[0048] The polymers can be biodegradable as well. Representative biodegradable polymers include:

polyglycolic acid/polylactic acid (PGLA),
polycaprolactone (PCL),
polyhydroxybutyrate valerate (PHBV),
polyorthoester (POE),
polyethyleneoxide/polybutylene terephthalate (PEO/PBTP),
polylactic acid (PLA),
polyglycolic acid (PGA),
poly (p-dioxanone),
poly (valetolactone),
poly (tartronic acid),
poly (β malonic acid),
poly (propylene fumarate),
poly (anhydrides); and
tyrosine-based polycarbonates.

[0049] Other equivalent materials, including but not limited to stereoisomers of any of the aforementioned, may be used as well.

[0050] In certain embodiments the biodegradable polymer may be comprised of copolymers of lactic acid and glycolic acid. The copolymer may be comprised of glycolic/lactic acid in the ratio of 90:10. In certain embodiments the ratio of glycolic to lactic acid is chosen from 99:1; 90:10; 95:5; 50:50; 10:90; 5:95; 1:99. In one embodiment the fibers may be comprised of Nylon 6.6

[0051] Using polyglycolide and poly(L-lactide) as base materials it is possible to copolymerize the two monomers to extend the range of homopolymer properties. Copolymers of glycolide with both L-lactide and DL-lactide have been developed for both device and drug delivery applications. It is noteworthy that there is not a linear relationship between the copolymer

composition and the mechanical properties of the materials. For example a copolymer of 50% glycolide and 50% DL-lactide degrades faster than either homopolymer. (See, Middleton and Tipton, 2000, *Biomaterials* 21:2335, which is incorporated herein by reference).

[0052] The fibers may be coated with at least a single coating of bioactive material (e.g. growth factors, genes, collagen, peptides, oligonucleotides, marine biopolymers such as chitosan, various mono-, di-, and poly-saccharides such as hyaluronic acid and the like or combinations thereof). In some embodiments a plurality of coatings is contemplated. The fibers may be coated with a non-bioactive material, or a combination of bioactive and non-bioactive material applied as a single layer or a plurality of layers.

Bioactive Materials

[0053] In some embodiments, the fibers can include within their body a bioactive material. In other embodiments, the bioactive material can be present in a coating applied to the coil, the stretch resistant member, or to the fibers or to any combination of the three. In one embodiment of this invention, the bioactive coating may be applied to the coil as a single layer and the fibers with or without bioactive coating can be omitted. In other embodiments, however, the bioactive material is dispersed in the fiber or coated on the fiber. As shown in Figure 6 this configuration involves a core of metal coil or fiber 30 with single outer coating comprising bioactive material 32.

[0054] The bioactive material, e.g., coatings may be proteinaceous e.g., a collageneous coating. Collageneous coatings may be of a wide variety of types, including natural or synthetic. In specific embodiments the bioactive material comprises a photo polymerizable collagen coating which will bind both with the metal with or without added bioactive agents. Examples of suitable collageneous materials include those having the same surface functional groups as do Type I and Type IV natural collagens.

[0055] The bioactive material or agent present in the polymer itself or the coating if present may have one or more functions, including, but not limited to, reducing friction, providing a therapeutic for local or blood borne delivery, or reducing thrombosis, coagulation or platelet activity. The bioactive material may be hydrophilic, e.g. a lubricious hydrophilic material such as hyaluronic acid. Examples of suitable hydrophilic compounds include polyvinyl alcohol (PVA), polyvinylpyrrolidone (PVP), polyacrylamide and the like. The bioactive material may be hydrophobic. Hydrophobic compounds include membrane lipids such as phosphatidyl choline, fatty acid esters and the like. The bioactive material may include water soluble therapeutics. Examples of water-soluble therapeutics include thrombolytics such as tissue plasminogen activator (TPA), streptokinase, urokinase, hirudin and growth factors such as vEGF. The bioactive material may include fat soluble therapeutics, e.g., fat soluble vitamins.

[0056] The bioactive coating or material may also promote cell attachment. It may also be thrombogenic. Non-limiting examples of bioactive coatings or materials which increase cell attachment and/or thrombogenicity

include both natural and synthetic compounds, e.g. collagen, fibrinogen, vitronectin, other plasma proteins, growth factors (e.g. vascular endothelial growth factor, "vEGF"), synthetic peptides of these and other proteins or peptides having attached RGD (arginine glycine-aspartic acid) residues, generally at one of both termini or other cell adhesion peptides, i.e., GRGDY, oligonucleotides, full or partial DNA constructs, natural or synthetic phospholipids or polymers with phosphorylcholine functionality.

Applications

[0057] The devices of this invention may be introduced to a selected site and thus the device of the invention may be used in treating a variety of maladies. For instance, in treatment of an aneurysm, the aneurysm itself may be filled with a plurality of devices. Alternatively, only one device may be administered. Shortly after the devices are placed within the aneurysm, an emboli may begin to form optionally under the influence of the bioactive material.

[0058] A selected site may be reached through the vascular system using a collection of specifically chosen catheters and guide wires. First of all, a large catheter is introduced through an entry site in the vasculature. Typically, this would be through a femoral artery in the groin. Other entry sites sometimes chosen are found in the neck and are in general well known by physicians who practice this type of medicine. Once the introducer is in place, a guiding catheter is then used to provide a safe passageway from the entry site to a region near the site to be treated. For instance, in treating a

site in the human brain, a guiding catheter would be chosen which would extend from the entry site at the femoral artery, up through the large arteries extending to the heart, around the heart through the aortic arch, and downstream through one of the arteries extending from the upper side of the aorta. A guidewire and neurovascular catheter are then placed through the guiding catheter as a unit. Once the tip of the guidewire reaches the end of the guiding catheter, it is then extended by the physician, with the aid of fluoroscopy to the site to be treated using the vaso-occlusive devices of this invention. The guidewire is advanced first from the guide catheter tip to the treatment site, followed by the neurovascular catheter. Once both the distal tip of the neurovascular catheter and the guidewire have reached the treatment site, and the distal tip of that catheter is approximately situated, e.g. within the mouth of an aneurysm to be treated, the guidewire is then withdrawn. The neurovascular catheter then has an open lumen to the outside of the body. The device of the invention is then pushed through the lumen to the treatment site and detached from the catheter. The device may be held in place because of its shape, size or volume.

EXAMPLES

Example 1 — Adding Fibers

[0059] A T- 10 platinum coil is obtained and fastened to a flat surface at its ends. It has a primary helix diameter of 0.028 mm. A plurality of Vicryl 90/100 PGLA sutures with diameters of from 0.099 mm to 0.029 mm are obtained. These sutures are made up of a bundle of 6-7 small microfibers

about 12 μm in diameter. A single monofilament of similar size could also be employed. The fibers are cut into about 2 cm lengths and physically enlaced in between windings of the T-10 coil in the configurations shown in Figures 2-5. This is done until a total of about 10-20 fibers per cm extend away from the coils. The fibers are trimmed to have 2-4 cm lengths extending from the coils.

[0060] If the fibers are coated with bioactive material or if they contain bioactive material, the surface area provided by the fibers would enhance delivery and activity.

Example 2— Coating

[0061] 1. Fill an ice container with cold water and add ice as needed to reach a temperature of 4-6°C.

2. Submerge a 15 ml centrifuge tube rack into the container/bucket.

3. Place 15 ml centrifuge tubes (filled with collagen solution at pH 7.4 $\pm$ 2) into the centrifuge rack

4. Pass a platinum coil through a drilled centrifuge cap into the solution.

5. Allow the coil to remain in the solution for 20 minutes.

6. Remove the coil and tube (ensure that the coil remains in the collagen solution) from the ice container/bucket.

7. Place the coil(s) in a 37°C oven for 4 hours.

8. Remove the coil from the collagen solution and rinse the coil 3x in PBS and 3x in distilled water.

9. Allow the coated coil to dry overnight.

What is claimed is:

- 1 1. A vaso-occlusive device for occluding blood flow in a patient comprising
2 a) a coil sized for insertion to a point of use in a vascular network of the
3 patient, where the coil is comprised of a first surface area; and
4 b) a plurality of enlaced fibers where the enlaced fibers are comprised of a
5 second surface area where the second surface area is at least 0.1 times the
6 surface area of the first surface area.
- 1 2. The device of claim 1, wherein the coil is a helical coil.
- 1 3. The device of claim 1, wherein the fibers are enlaced through the coil.
- 1 4. The device of claim 1, wherein the coil is comprised of metal wire.
- 1 5. The device of claim 4, wherein the metal wire is a biocompatible metal
2 wire.
- 1 6. The device of claim 4, wherein the metal wire is at least 5 mm in length.
- 1 7. The device of claim 4, wherein the metal wire is radio-opaque.

1 8. The device of claim 4, wherein the metal wire is comprised of a metal
2 chosen from platinum, palladium, rhodium, rhenium, iridium, gold, silver, tungsten
3 and tantalum or an alloy of these metals.

1 9. The device of claim 8, wherein the metal wire is comprised of a platinum
2 iridium alloy.

1 10. The device of claim 8, wherein the metal wire is comprised of a platinum
2 tungsten alloy.

1 11. The device of claim 4, wherein the metal wire is comprised of a super-
2 elastic metal.

1 12. The device of claim 11, wherein the super-elastic metal is nitinol.

1 13. The device of claim 4, wherein the metal wire has a diameter of about
2 0.025 mm to about 0.09 mm.

1 14. The device of claim 4, wherein the metal wire has a diameter of about
2 0.04 mm to about 0.06 mm.

1 15. The device of claim 1, wherein the coil is comprised of a primary helix
2 which is itself wound into a secondary shape.

1 16. The device of claim 15, wherein the secondary shape is a complicated
2 three dimensional structure.

1 17. The device of claim 15, wherein the secondary shape is another helix.

1 18. The device of claim 17, wherein the secondary shape is a double helix.

1 19. The device of claim 15, wherein the primary helix has a diameter of about
2 0.1 millimeters to about 0.8 millimeters.

1 20. The device of claim 15, wherein the primary helix has a diameter of about
2 0.28 millimeters.

1 21. The device of claim 15, wherein the primary helix has a diameter of about
2 0.24 millimeters.

1 22. The device of claim 15, wherein the primary helix has about 2 to about 50
2 windings per millimeter.

1 23. The device of claim 15, wherein the primary helix is comprised of a pitch
2 that provides for free space between adjacent coils.

1 24. The device of claim 23, wherein up to about 60% of the length of
2 secondary shape is comprised of the free space.

1 25. The device of claim 23, wherein about 0% to about 25% of the length of
2 secondary shape is comprised of the free space.

1 26. The device of claim 25, wherein the free space is small enough to permit
2 the adjacent coils to grip the fibers.

1 27. The device of claim 1, wherein a majority of fibers each enlase a single
2 winding of the helical coil.

1 28. The device of claim 1, wherein a majority of fibers each enlase two or
2 more windings of the helical coil.

1 29. The device of claim 1, wherein the fibers are comprised of a bioactive
2 material.

1 30. The device of claim 1, wherein the fibers are comprised of a non-bioactive
2 material.

1 31. The device of claim 1, wherein the fibers are comprised of a copolymer of
2 glycolic acid and lactic acid.

1 32. The device of claim 1, further comprising a bioactive coating.

1 33. The device of claim 32, wherein the bioactive coating is a lubricious
2 hydrophilic coating.

1 34. The device of claim 32, wherein the bioactive coating is a hydrophobic
2 coating.

1 35. The device of claim 32, wherein the bioactive coating is applied to the
2 fiber.

1 36. The device of claim 32, wherein the bioactive coating is a copolymer.

1 37. The device of claim 36, wherein the copolymer is comprised of lactic acid
2 and glycolic acid.

1 38. The device of claim 1, wherein the fibers are comprised of non-
2 biodegradable polymer.

1 39. The device of claim 38, wherein the non-biodegradable polymer is chosen
2 from a polyethylene, a polyacrylic, a polypropylene, a polyvinylchloride, a
3 polyamide, a polyurethane, a polyvinylpyrrolidone, a polyvinyl alcohol, a
4 polyvinylacetate, a cellulose acetate, a polystyrene, a polytetrafluoroethylene, a
5 polyester, silk or cotton.

1 40. The device of claim 38, wherein the non-biodegradable polymer is nylon.

1 41. The device of claim 38, wherein the non-biodegradable polymer is
2 polyethylene terephthalate.

1 42. The device of claim 1, wherein the fibers are comprised of biodegradable
2 polymer.

1 43. The device of claim 42, wherein the biodegradable polymer is chosen from
2 polyglycolic acid, polycaprolactone, polyhydroxybutyrate valerate, polyorthoester,
3 polylactic acid, poly (p-dioxanone), poly (valetolactone), poly (tartronic acid), poly
4 (β -malonic acid), poly (propylene fumarate), a tyrosine based polycarbonate, and
5 a copolymer of polyethylene oxide and polybutylene terephthalate.

1 44. The device of claim 31, wherein the ratio of glycolic acid to lactic acid is
2 99:1.

1 45. The device of claim 31, wherein the ratio of glycolic acid to lactic acid is
2 1:99.

1 46. The device of claim 31, wherein the ratio of glycolic acid to lactic acid is
2 95:5.

1 47. The device of claim 31, wherein the ratio of glycolic acid to lactic acid is
2 5:95.

1 48 The device of claim 31, wherein the ratio of glycolic acid to lactic acid is
2 50:50.

1 49. The device of claim 31, wherein the ratio of glycolic acid to lactic acid is
2 90:10.

1 50. The device of claim 32, wherein the coating material is chosen from a
2 growth factor, a gene, an oligonucleotide, a peptide, a marine biopolymer, a
3 mono-saccharide,

4 a di-saccharide, a poly-saccharide, collagen and combinations of any of the
5 aforementioned.

1 51. The device of claim 32, wherein the coating is applied to the coil.

1 52. The device of claim 35, wherein the coating is applied to the fiber as a
2 single layer.

1 53. The device of claim 43, wherein the bioactive coating is applied to the coil
2 as a single layer.

1 54. The device of claim 32, wherein the bioactive coating is dispersed
2 throughout the fiber.

1 55. The device of claim 32, wherein the coating promotes cell attachment and
2 is thrombogenic.

1 56 The device of claim 55, wherein the coating material is chosen from
2 collagen, fibrinogen, vitronectin, vascular endothelial growth factor, a peptide
3 comprising the sequence arginine-glycine-aspartic acid (RGD).

- 1 57. A method of treating an aneurysm in a patient comprising introducing a
2 vaso-occlusive device into the patient thereby treating the aneurysm, wherein the
3 vaso-occlusive device comprises
- 4 a) a coil sized for insertion to a point of use in a vascular network of the
5 patient, where the coil is comprised of a first surface area; and
- 6 b) a plurality of enlaced fibers where the enlaced fibers are comprised of a
7 second surface area where the second surface area is at least 0.1 times the
8 surface area of the first surface area.
- 1 58. The method of claim 57, wherein the coil has a complicated 3 dimensional
2 structure.
- 1 59. The method of claim 57, wherein the coil is a helix.
- 1 60. The method of claim 57, wherein the vaso-occlusive device is introduced
2 using a catheter.
- 1 61. The method of claim 57, wherein the vaso-occlusive device is introduced
2 through an entry site in the vasculature.
- 1 62. The method of claim 61, wherein the entry site is in the femoral artery.

1 63. A method of making a vaso-occlusive device comprising the steps of
2 a) obtaining a helically coiled wire core having a fiber gripping spacing
3 between adjacent windings when not under tension;
4 b) extending the wire core into an extended condition;
5 c) enlacing between adjacent windings of said core a plurality of fibers,
6 thereby increasing the surface area of the coil by at least a factor of 0.1; and
7 d) relaxing the coil thereby causing the adjacent windings of the coil to grip
8 the enlaced fibers.

1 64. The method of claim 63, wherein the fibers are comprised of a copolymer
2 of polyglycolic acid and lactic acid.

1 65. The method of claim 63, wherein the enlacing is around a single winding.

1 66. The method of claim 63, wherein the enlacing is through a single winding.

1 67. The method of claim 63, wherein the enlacing is through multiple
2 windings.

1 68. The method of claim 63, wherein the enlacing forms an "S" configuration.

1 69. A vaso-occlusive device for occluding blood flow in a patient comprising

2 a) a coil sized for insertion to a point of use in a vascular network of the
3 patient; and

4 b) a plurality of enlaced fibers where the enlaced fibers are comprised of a
5 copolymer of lactic acid and glycolic acid.

1 70. The device of claim 69, wherein the coil is a helical coil.

1 71. The device of claim 69, wherein the fibers are enlaced through the coil.

1 72. The device of claim 69, wherein the coil is comprised of metal wire.

1 73. The device of claim 72, wherein the metal wire is a biocompatible metal
2 wire.

1 74. The device of claim 72, wherein the metal wire is at least 5 mm in length.

1 75. The device of claim 72, wherein the metal wire is radio-opaque.

1 76. The device of claim 72 wherein the metal wire is comprised of a metal
2 chosen from platinum, palladium, rhodium, rhenium, iridium, gold, silver, tungsten
3 and tantalum or an alloy of these metals.

1 77. The device of claim 76, wherein the metal wire is comprised of a platinum
2 iridium alloy.

1 78. The device of claim 76, wherein the metal wire is comprised of a platinum
2 tungsten alloy.

1 79. The device of claim 72, wherein the metal wire is comprised of a super-
2 elastic metal.

1 80. The device of claim 79, wherein the super-elastic metal is nitinol.

1 81. The device of claim 72, wherein the metal wire has a diameter of about
2 0.025 mm to about 0.09 mm.

1 82. The device of claim 72, wherein the metal wire has a diameter of about
2 0.04 mm to about 0.06 mm.

1 83. The device of claim 69, wherein the coil is comprised of a primary helix
2 which is itself wound into a secondary shape.

1 84. The device of claim 83, wherein the secondary shape is a complicated
2 three dimensional structure.

1 85. The device of claim 83, wherein the secondary shape is another helix.

1 86. The device of claim 85, wherein the secondary shape is a double helix.

1 87. The device of claim 83, wherein the primary helix has a diameter of about
2 0.1 millimeters to about 0.8 millimeters.

1 88. The device of claim 83, wherein the primary helix has a diameter of about
2 0.28 millimeters.

1 89. The device of claim 83, wherein the primary helix has a diameter of about
2 0.24 millimeters.

1 90. The device of claim 83, wherein the primary helix has about 2 to about 50
2 windings per millimeter.

1 91. The device of claim 83, wherein the primary helix is comprised of a pitch
2 that provides for free space between adjacent coils.

1 92. The device of claim 91, wherein up to about 60% of the length of
2 secondary shape is comprised of the free space.

1 93. The device of claim 91 wherein about 0% to about 25% of the length of
2 secondary shape is comprised of the free space.

1 94. The device of claim 93, wherein the free space is small enough to permit
2 the adjacent coils to grip the fibers.

1 95. The device of claim 69, wherein a majority of fibers each enlase a single
2 winding of the helical coil.

1 96. The device of claim 69, wherein a majority of fibers each enlase two or
2 more windings of the helical coil.

1 97. The device of claim 69, wherein the fibers are comprised of a bioactive
2 material.

1 98. The device of claim 69, wherein the fibers are comprised of a non-
2 bioactive material.

1 99. The device of claim 69, wherein the fibers are comprised of a copolymer
2 of glycolic acid and lactic acid.

- 1 100. The device of claim 69, further comprising a bioactive coating.
- 1 101. The device of claim 100, wherein the bioactive coating is a lubricious
2 hydrophilic coating.
- 1 102. The device of claim 100, wherein the bioactive coating is a hydrophobic
2 coating.
- 1 103 The device of claim 100, wherein the bioactive coating is a copolymer.
- 1 104. The device of claim 103, wherein the copolymer is comprised of lactic acid
2 and glycolic acid.
- 1 105. The device of claim 69, wherein the fibers are comprised of non-
2 biodegradable polymer.
- 1 106. The device of claim 105, wherein the non-biodegradable polymer is
2 chosen from a polyethylene, a polyacrylic, a polypropylene, a polyvinylchloride, a
3 polyamide, a polyurethane, a polyvinylpyrrolidone, a polyvinyl alcohol, a
4 polyvinylacetate, a cellulose acetate, a polystyrene, a polytetrafluoroethylene, a
5 polyester, silk or cotton.

1 107. The device of claim 105, wherein the non-biodegradable polymer is nylon.

1 108. The device of claim 105, wherein the non-biodegradable polymer is
2 polyethylene terephthalate.

1 109. The device of claim 69, wherein the fibers are comprised of biodegradable
2 polymer.

110. The device of claim 109, wherein the biodegradable polymer is chosen from polyglycolic acid, polycaprolactone, polyhydroxybutyrate valerate, polyorthoester, polylactic acid, poly (p-dioxanone), poly (valetolactone), poly (tartronic acid), poly (β -malonic acid), poly (propylene fumarate), a tyrosine based polycarbonate, and a copolymer of polyethylene oxide and polybutylene terephthalate.

1 111. The device of claim 99, wherein the ratio of glycolic acid to lactic acid is
2 99:1.

1 112. The device of claim 99, wherein the ratio of glycolic acid to lactic acid is
2 1:99.

1 113. The device of claim 99, wherein the ratio of glycolic acid to lactic acid is
2 95:5.

1 114. The device of claim 99, wherein the ratio of glycolic acid to lactic acid is
2 5:95.

1 115. The device of claim 99, wherein the ratio of glycolic acid to lactic acid is
2 50:50.

1 116. The device of claim 99, wherein the ratio of glycolic acid to lactic acid is
2 90:10.

1 117. The device of claim 100, wherein the coating is chosen from a growth
2 factor, a gene, an oligonucleotide, a peptide, a marine biopolymer, a mono-
3 saccahride,
4 a di-saccahride, a poly-saccahride, collagen and combinations of any of the
5 aforementioned.

1 118. The device of claim 100, wherein the coating is applied to the coil.

1 119. The device of claim 100, wherein the coating is applied to the fibers as a
2 single layer.

1 120. The device of claim 118, wherein the bioactive coating is applied to the
2 coil as a single layer.

1 121. The device of claim 100, wherein the bioactive coating is dispersed
2 throughout the fiber.

1 122. The device of claim 100, wherein the coating promotes cell attachment
2 and is thrombogenic.

1 123. The device of claim 122, wherein the coating material is chosen from
2 collagen, fibrinogen, vitronectin, vascular endothelial growth factor, a peptide
3 comprising the sequence arginine-glycine-aspartic acid (RGD).

1 124. The device of claim 100, wherein the bioactive coating is applied to the
2 fiber.

1 125. A method of treating an aneurysm in a patient comprising introducing a
2 vaso-occlusive device into the patient thereby treating the aneurysm, wherein the
3 vaso-occlusive device comprises
4 a) a coil sized for insertion to a point of use in a vascular network of the
5 patient, where the coil is comprised of a first surface area; and

6 b) a plurality of enlaced fibers where the enlaced fibers are comprised of a
7 copolymer of lactic acid and glycolic acid.

1 126. The method of claim 125, wherein the coil has a complicated 3
2 dimensional structure.

1 127. The method of claim 125, wherein the coil is a helix.

1 128. The method of claim 125, wherein the vaso-occlusive device is introduced
2 using a catheter.

1 129. The method of claim 125, wherein the vaso-occlusive device is introduced
2 through an entry site in the vasculature.

1 130. The method of claim 129, wherein the entry site is in the femoral artery.

1 131. A method of making a vaso-occlusive device comprising the steps of
2 a) obtaining a helically coiled wire core having a fiber gripping spacing
3 between adjacent windings when not under tension;
4 b) extending the wire core into an extended condition;
5 c) enlacing between adjacent windings of said core a plurality of fibers
6 comprised of a copolymer comprised of lactic acid and glycolic acid; and

7 d) relaxing the coil thereby causing the adjacent windings of the coil to grip
8 the enlaced fibers.

1 132. The method of claim 131, wherein the enlacing is around a single winding.

1 133. The method of claim 131, wherein the enlacing is through a single
2 winding.

1 134. The method of claim 131, wherein the enlacing is through multiple
2 windings.

1 135. The method of claim 131, wherein the enlacing forms an "S" configuration.

1 136. A vaso-occlusive device for occluding blood flow in a patient comprising
2

3 a) a coil, comprising a lumen and a first and a second end, and sized for
4 insertion to a point of use in a vascular network of the patient;

5

6 b) a stretch resistant member fixedly attached to at least one end of the
7 coil; and

8

9 c) a plurality of enlaced fibers where each of the enlaced fibers is enlaced
10 around the stretch resistant member at least two times.

1 137. The device of 136, wherein the stretch resistant member axially traverses
2 the lumen of the coil.

1 138. The device of 136, wherein the stretch resistant member is fixedly
2 attached to both the first and second ends of the coil.

1 139. The device of 136, wherein the plurality of fibers are not tied in a knot.

1 140. The device of claim 136, wherein the stretch resistant member is
2 comprised of a metal wire.

1 141. The device of claim 140, wherein the metal wire is radio-opaque.

1 142. The device of claim 140, wherein the metal wire is comprised of a metal
2 chosen from platinum, palladium, rhodium, rhenium, iridium, gold, silver, tungsten
3 and tantalum or an alloy of these metals.

1 143. The device of claim 140, wherein the metal wire is comprised of a
2 platinum iridium alloy.

1 144. The device of claim 140, wherein the metal wire is comprised of a
2 platinum tungsten alloy.

1 145. The device of claim 140, wherein the metal wire is comprised of a super-
2 elastic metal.

1 146. The device of claim 145, wherein the super-elastic metal is nitinol.

1 147. The device of claim 136, wherein the stretch resistant member is
2 comprised of a polymer.

1 148. The device of claim 147, wherein the polymer is non-biodegradable.

1 149. The device of claim 147, wherein the polymer is biodegradable.

1 150. The device of claim 136, wherein the stretch resistant member is further
2 comprised of a bioactive coating.

1 151. The device of claim 150, wherein the coating is chosen from a growth
2 factor, a gene, an oligonucleotide, a peptide, a marine biopolymer, a mono-
3 saccharide,

4 a di-saccharide, a poly-saccharide, collagen and combinations of any of the
5 aforementioned.

1 152. The device of claim 150, wherein the coating is a polymer.

1 153. The device of claim 136, wherein the coil is a helical coil.

1 154. The device of claim 136, wherein the fibers are enlaced through the coil.

1 155. The device of claim 136, wherein the coil is comprised of metal wire.

1 156. The device of claim 155, wherein the metal wire is a biocompatible metal
2 wire.

1 157. The device of claim 155, wherein the metal wire is at least 5 mm in length.

1 158. The device of claim 155, wherein the metal wire is radio-opaque.

1 159. The device of claim 155, wherein the metal wire is comprised of a metal
2 chosen from platinum, palladium, rhodium, rhenium, iridium, gold, silver, tungsten
3 and tantalum or an alloy of these metals.

1 160. The device of claim 155, wherein the metal wire is comprised of a
2 platinum iridium alloy.

1 161. The device of claim 155, wherein the metal wire is comprised of a
2 platinum tungsten alloy.

1 162. The device of claim 155, wherein the metal wire is comprised of a super-
2 elastic metal.

1 163. The device of claim 162, wherein the super-elastic metal is nitinol.

1 164. The device of claim 155, wherein the metal wire has a diameter of about
2 0.025 mm to about 0.09 mm.

1 165. The device of claim 155, wherein the metal wire has a diameter of about
2 0.04 mm to about 0.06 mm.

1 166. The device of claim 136, wherein the coil is comprised of a primary helix
2 which is itself wound into a secondary shape.

1 167. The device of claim 166, wherein the secondary shape is a complicated
2 three dimensional structure.

1 168. The device of claim 166, wherein the secondary shape is another helix.

1 169. The device of claim 166, wherein the secondary shape is a double helix.

1 170. The device of claim 166, wherein the primary helix has a diameter of
2 about 0.1 millimeters to about 0.8 millimeters.

1 171. The device of claim 166, wherein the primary helix has a diameter of
2 about 0.28 millimeters.

1 172. The device of claim 166, wherein the primary helix has a diameter of
2 about 0.24 millimeters.

1 173. The device of claim 166, wherein the primary helix has about 2 to about
2 50 windings per millimeter.

1 174. The device of claim 166, wherein the primary helix is comprised of a pitch
2 that provides for free space between adjacent coils.

1 175. The device of claim 174, wherein up to about 60% of the length of
2 secondary shape is comprised of the free space.

1 176. The device of claim 174, wherein about 0% to about 25% of the length of
2 secondary shape is comprised of the free space.

1 177. The device of claim 174, wherein the free space is small enough to permit
2 the adjacent coils to grip the fibers.

1 178. The device of claim 136, wherein the fibers are comprised of a bioactive
2 material.

1 179. The device of claim 136, wherein the fibers are comprised of a non-
2 bioactive material.

1 180. The device of claim 136, wherein the fibers are comprised of a copolymer
2 of glycolic acid and lactic acid.

1 181. The device of claim 136, further comprising a bioactive coating.

1 182. The device of claim 181, wherein the bioactive coating is a lubricious
2 hydrophilic coating.

1 183. The device of claim 181, wherein the bioactive coating is a hydrophobic
2 coating.

1 184. The device of claim 181, wherein the bioactive coating is applied to the
2 fiber.

1 185. The device of claim 181, wherein the bioactive coating is a copolymer.

1 186. The device of claim 185, wherein the copolymer is comprised of lactic acid
2 and glycolic acid.

1 187. The device of claim 136, wherein the fibers are comprised of non-
2 biodegradable polymer.

1 188. The device of claim 187, wherein the non-biodegradable polymer is
2 chosen from a polyethylene, a polyacrylic, a polypropylene, a polyvinylchloride, a
3 polyamide, a polyurethane, a polyvinylpyrrolidone, a polyvinyl alcohol, a
4 polyvinylacetate, a cellulose acetate, a polystyrene, a polytetrafluoroethylene, a
5 polyester, silk or cotton.

1 189. The device of claim 187, wherein the non-biodegradable polymer is nylon.

1 190. The device of claim 187, wherein the non-biodegradable polymer is
2 polyethylene terephthalate.

1 191. The device of claim 136, wherein the fibers are comprised of
2 biodegradable polymer.

1 192. The device of claim 191, wherein the biodegradable polymer is chosen
2 from polyglycolic acid, polycaprolactone, polyhydroxybutyrate valerate,
3 polyorthoester, polylactic acid, poly (p-dioxanone), poly (valerolactone), poly
4 (tartronic acid), poly (β -malonic acid), poly (propylene fumarate), a tyrosine
5 based polycarbonate, and a copolymer of polyethylene oxide and polybutylene
6 terephthalate.

193. The device of claim 186, wherein the ratio of glycolic acid to lactic acid is
99:1.

1 194. The device of claim 186, wherein the ratio of glycolic acid to lactic acid is
2 1:99.

1 195. The device of claim 186, wherein the ratio of glycolic acid to lactic acid is
2 95:5.

1 196. The device of claim 186, wherein the ratio of glycolic acid to lactic acid is
2 5:95.

1 197. The device of claim 186, wherein the ratio of glycolic acid to lactic acid is
2 50:50.

1 198. The device of claim 186, wherein the ratio of glycolic acid to lactic acid is
2 90:10.

1 199. The device of claim 181, wherein the coating material is chosen from a
2 growth factor, a gene, an oligonucleotide, a peptide, a marine biopolymer, a
3 mono-saccharide,
4 a di-saccharide, a poly-saccharide, collagen and combinations of any of the
5 aforementioned.

1 200. The device of claim 181, wherein the coating is applied to the coil and the
2 stretch resistant member.

1 201. The device of claim 181, wherein the coating is applied to the fiber as a
2 single layer.

1 202. The device of claim 200, wherein the bioactive coating is applied to the
2 coil and the stretch resistant member as a single layer.

1 203. The device of claim 181, wherein the bioactive coating is dispersed
2 throughout the fiber.

1 204. The device of claim 181, wherein the coating promotes cell attachment
2 and is thrombogenic.

1 205. The device of claim 181, wherein the coating material is chosen from
2 collagen, fibrinogen, vitronectin, vascular endothelial growth factor, a peptide
3 comprising the sequence arginine-glycine-aspartic acid (RGD).

1 206. A method of treating an aneurysm in a patient comprising introducing a
2 vaso-occlusive device into the patient thereby treating the aneurysm, wherein the
3 vaso-occlusive device comprises

4 a) a coil sized for insertion to a point of use in a vascular network of the
5 patient, where the coil is comprised of a first surface area;

6 b) a stretch resistant member fixedly attached to at least one end of the
7 coil; and

8 c) a plurality of enlaced fibers where each of the enlaced fibers is enlaced
9 around the stretch resistant member at least two times.

1 207. The method of claim 206, wherein the coil has a complicated 3
2 dimensional structure.

1 208. The method of claim 206, wherein the coil is a helix.

1 209. The method of claim 206, wherein the vaso-occlusive device is introduced
2 using a catheter.

1 210. The method of claim 206, wherein the vaso-occlusive device is introduced
2 through an entry site in the vasculature.

1 211. The method of claim 206, wherein the entry site is in the femoral artery.

1 212. A method of making a vaso-occlusive device comprising the steps of
2 a) obtaining a helically coiled wire core comprising a lumen, a first and
3 second end and a fiber gripping spacing between adjacent windings when not
4 under tension;
5 b) extending the wire core into an extended condition;
6 c) inserting a stretch resistant member into the lumen of the helically
7 coiled wire and fixedly attaching the stretch resistant member to at least one end
8 of the helically coiled wire

- 9 d) enlacing a plurality of fibers around the stretch resistant member at
10 least two times; and
11 e) relaxing the coil thereby causing the adjacent windings of the coil to grip
12 the enlaced fibers.

1 213. The method of claim 212, wherein stretch resistant member is fixedly
2 attached to the first and second end of the helically coiled wire.

1 214. The method of claim 212, wherein the enlacing is through multiple
2 windings.

1 215. The method of claim 212, wherein the enlacing forms an "S" configuration.

1 216. The method of claim 63, wherein the enlacing is around multiple windings.

1 217. The method of claim 131, wherein the enlacing is around multiple
2 windings.

1/4

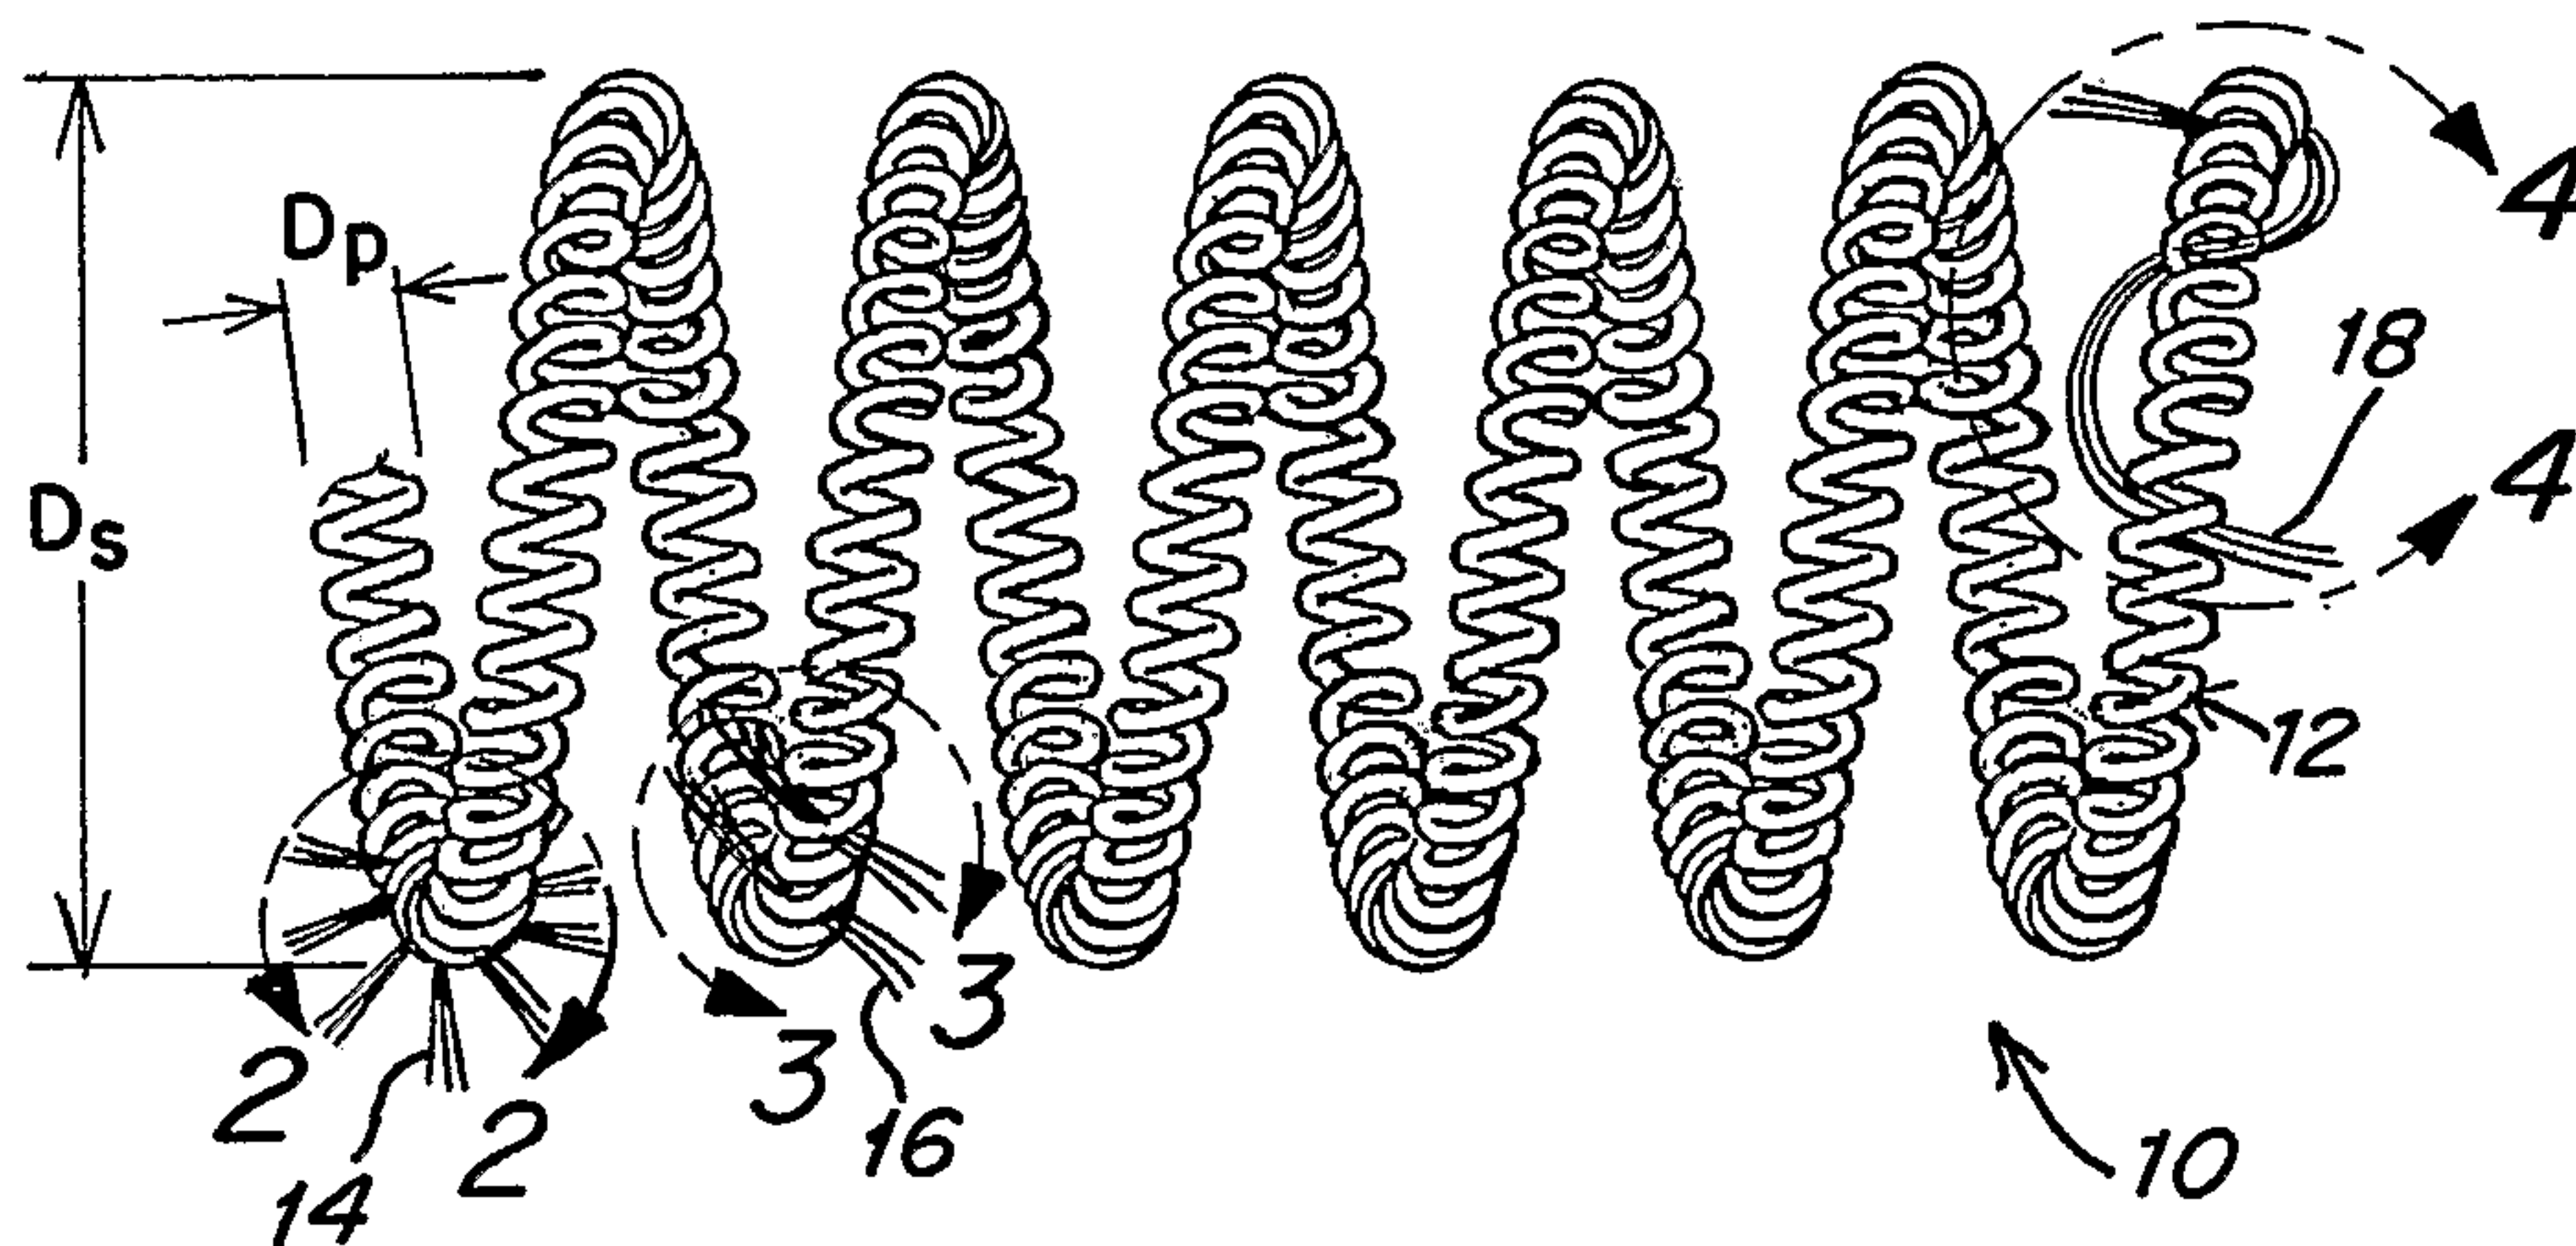


Fig. 1

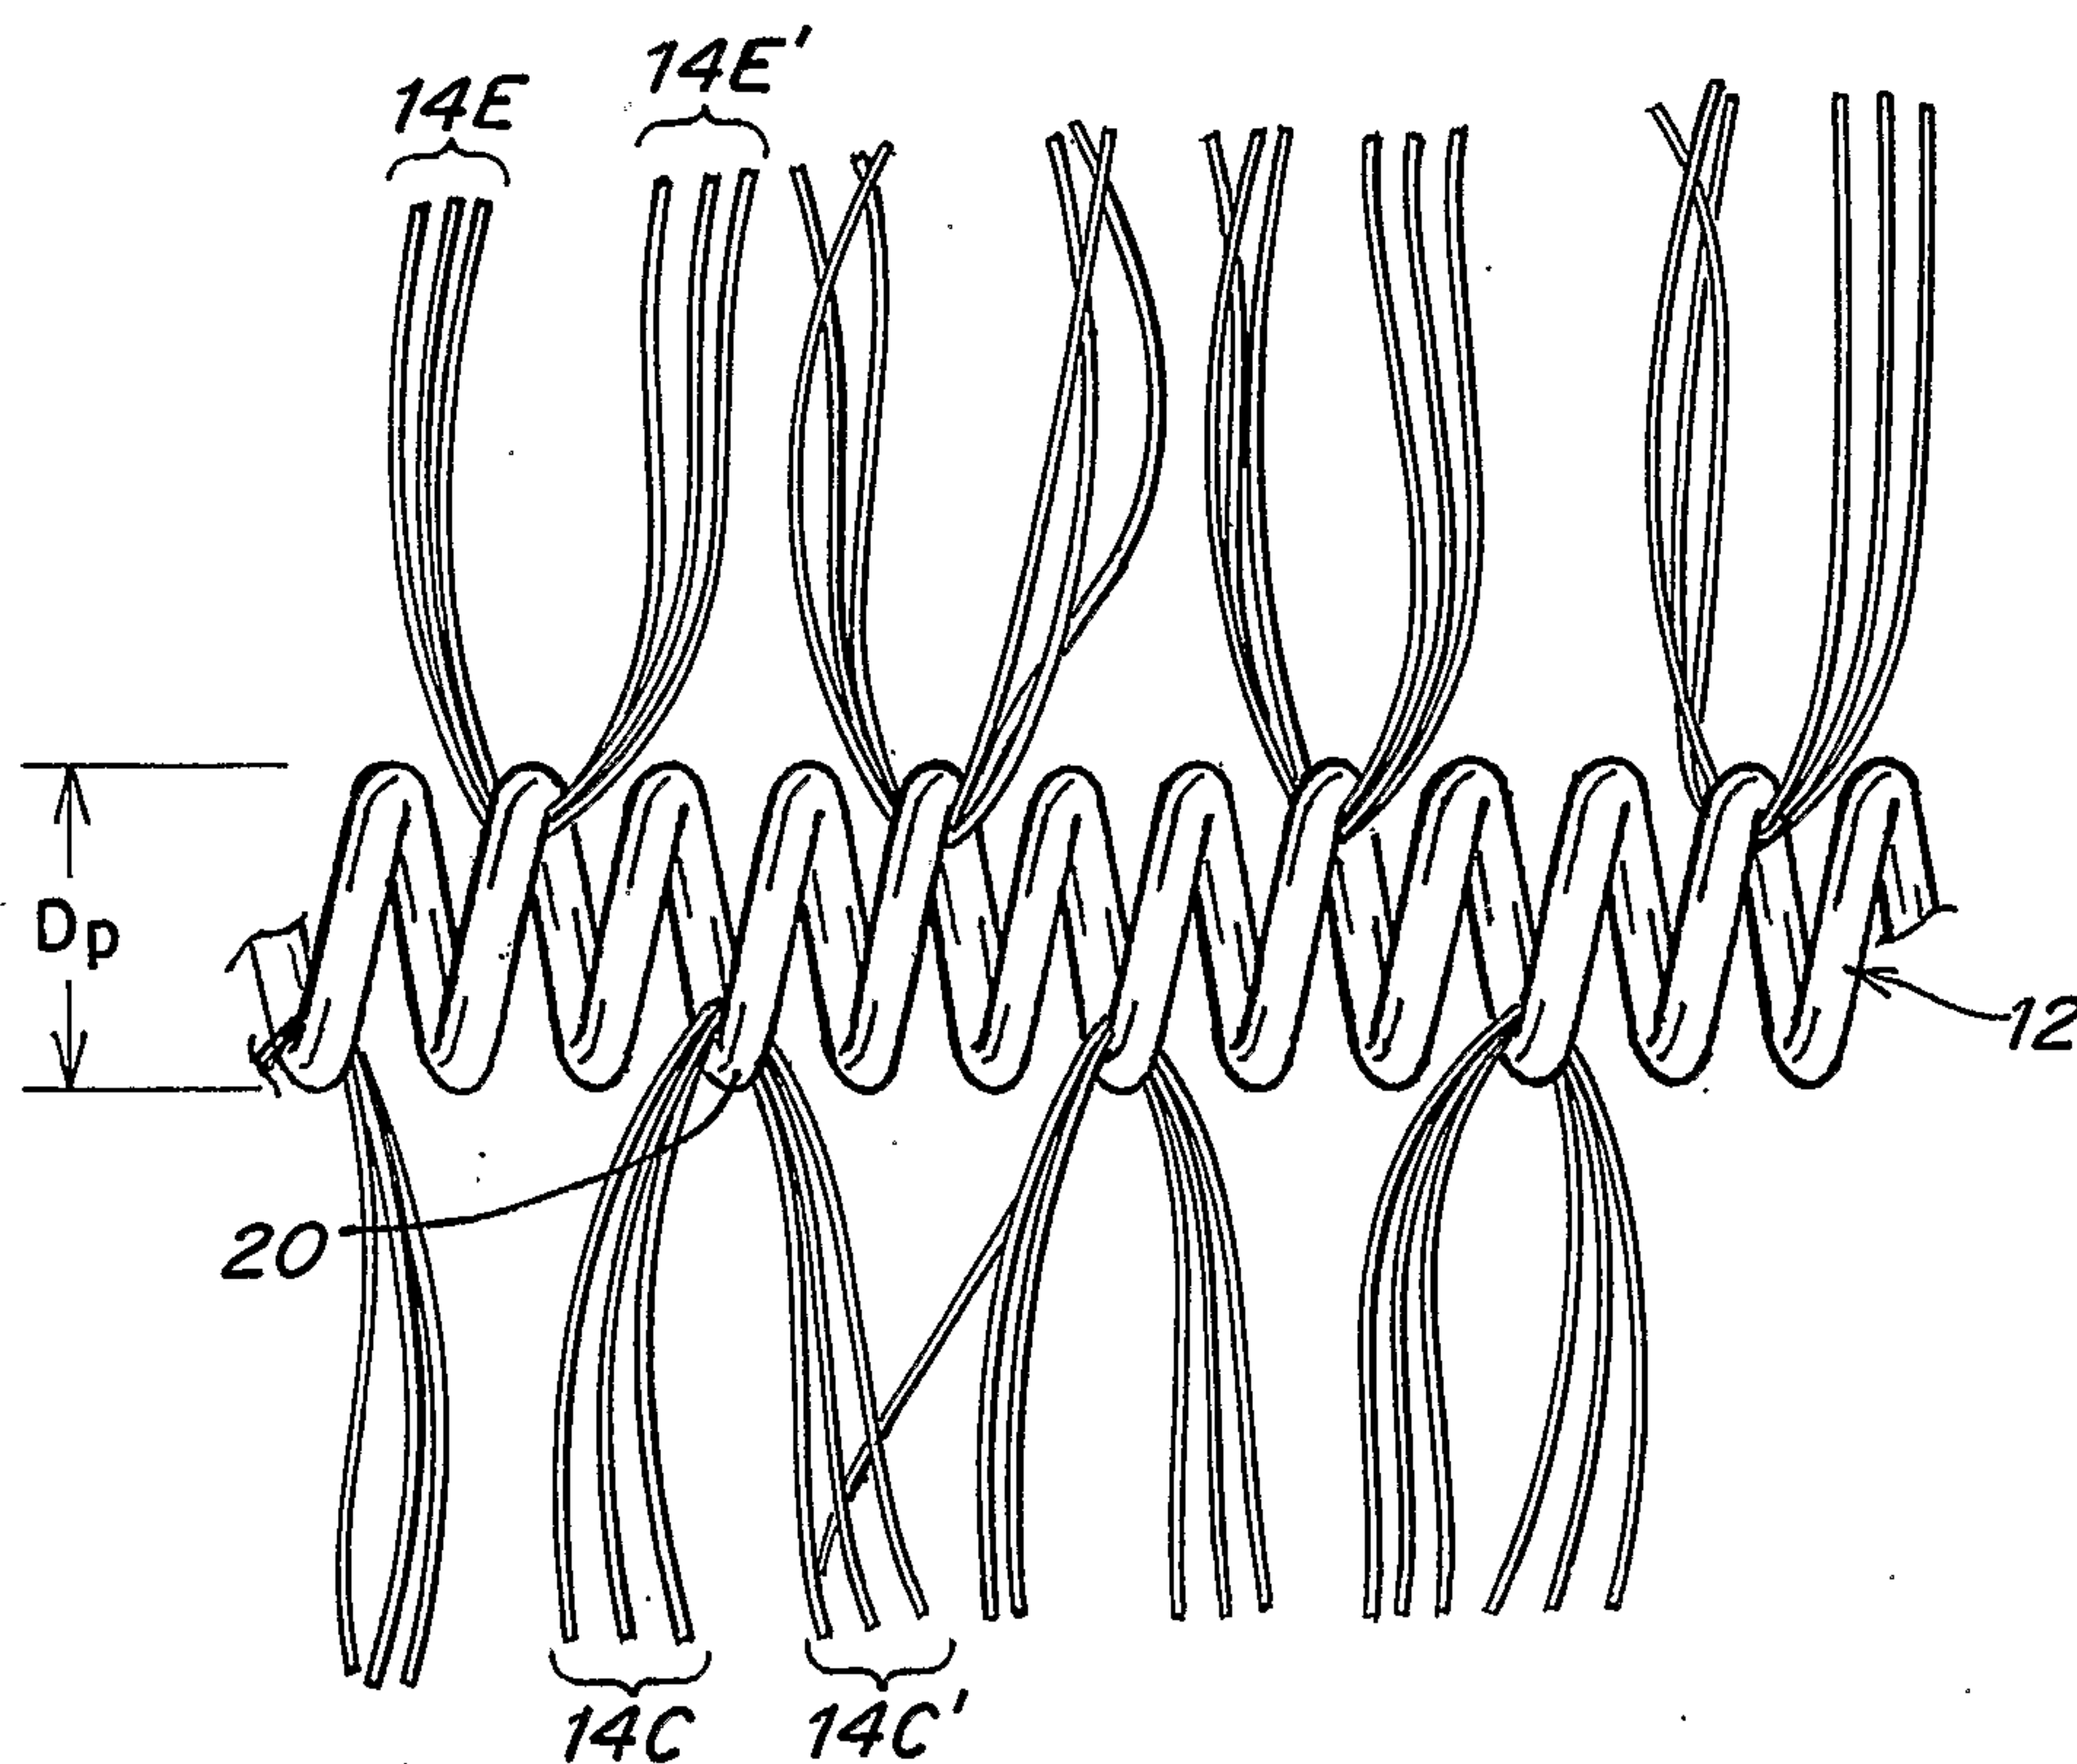
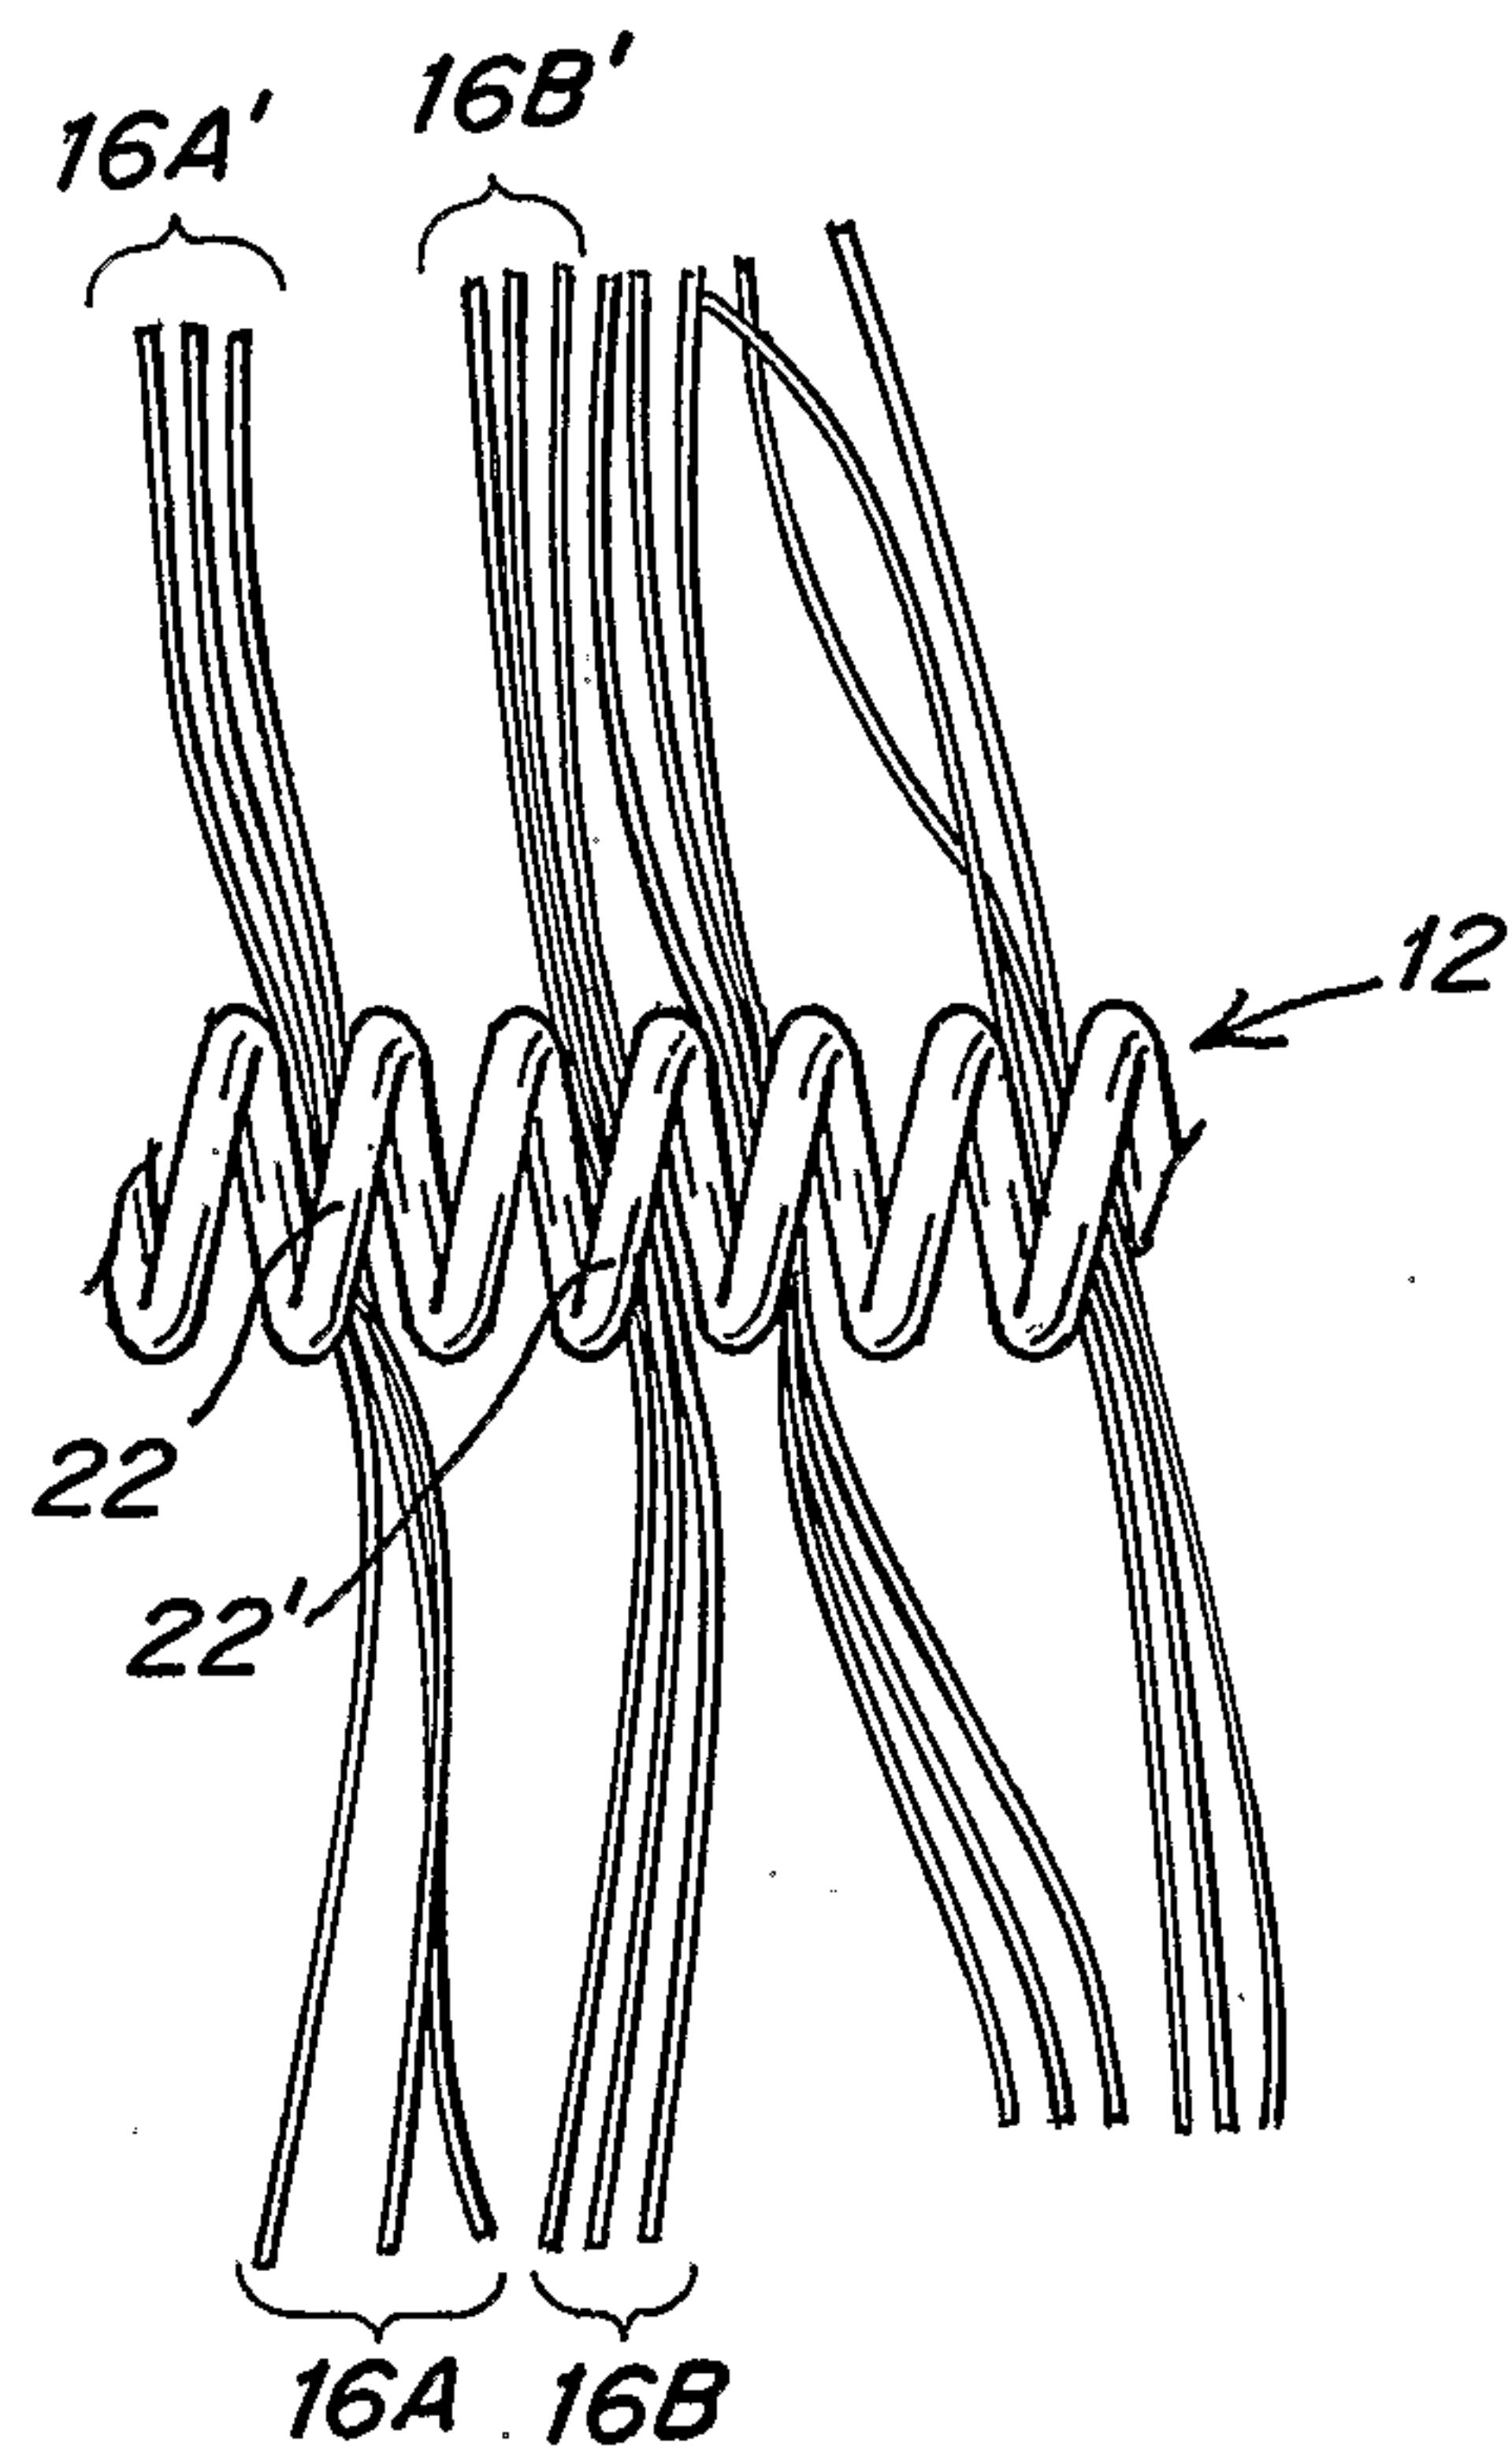
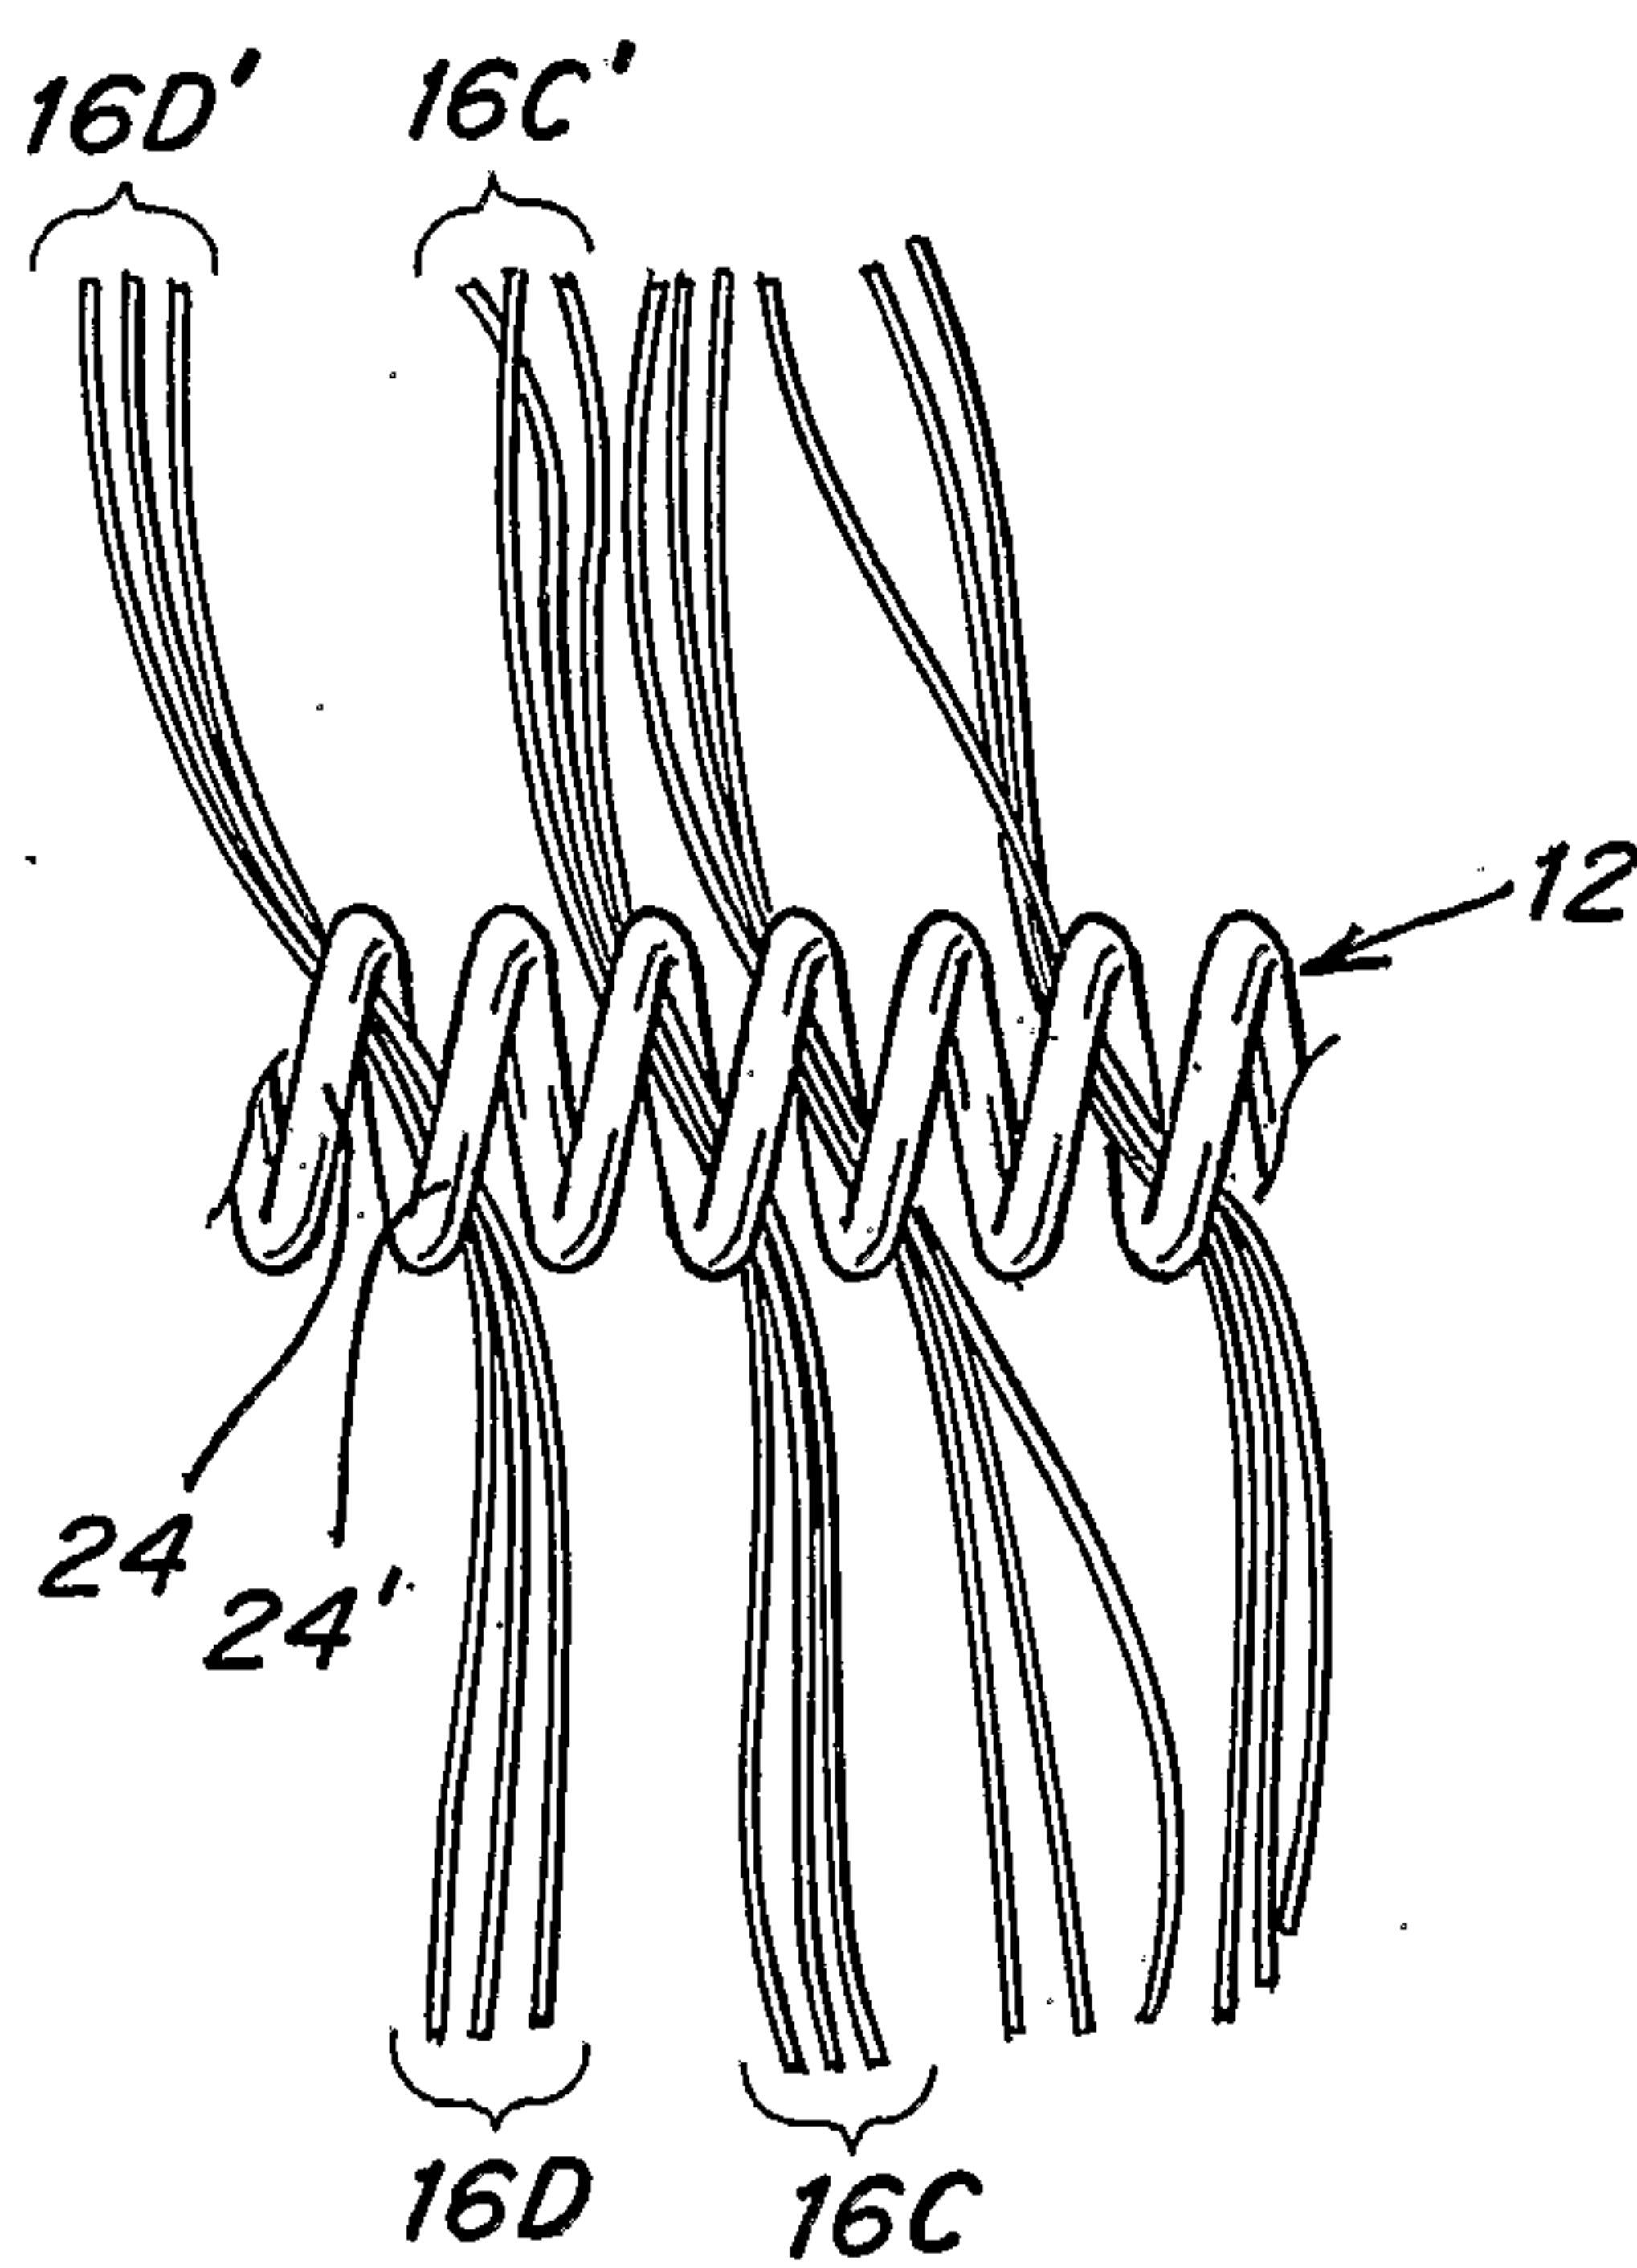


Fig. 2

2/4

*Fig. 3**Fig. 3A*

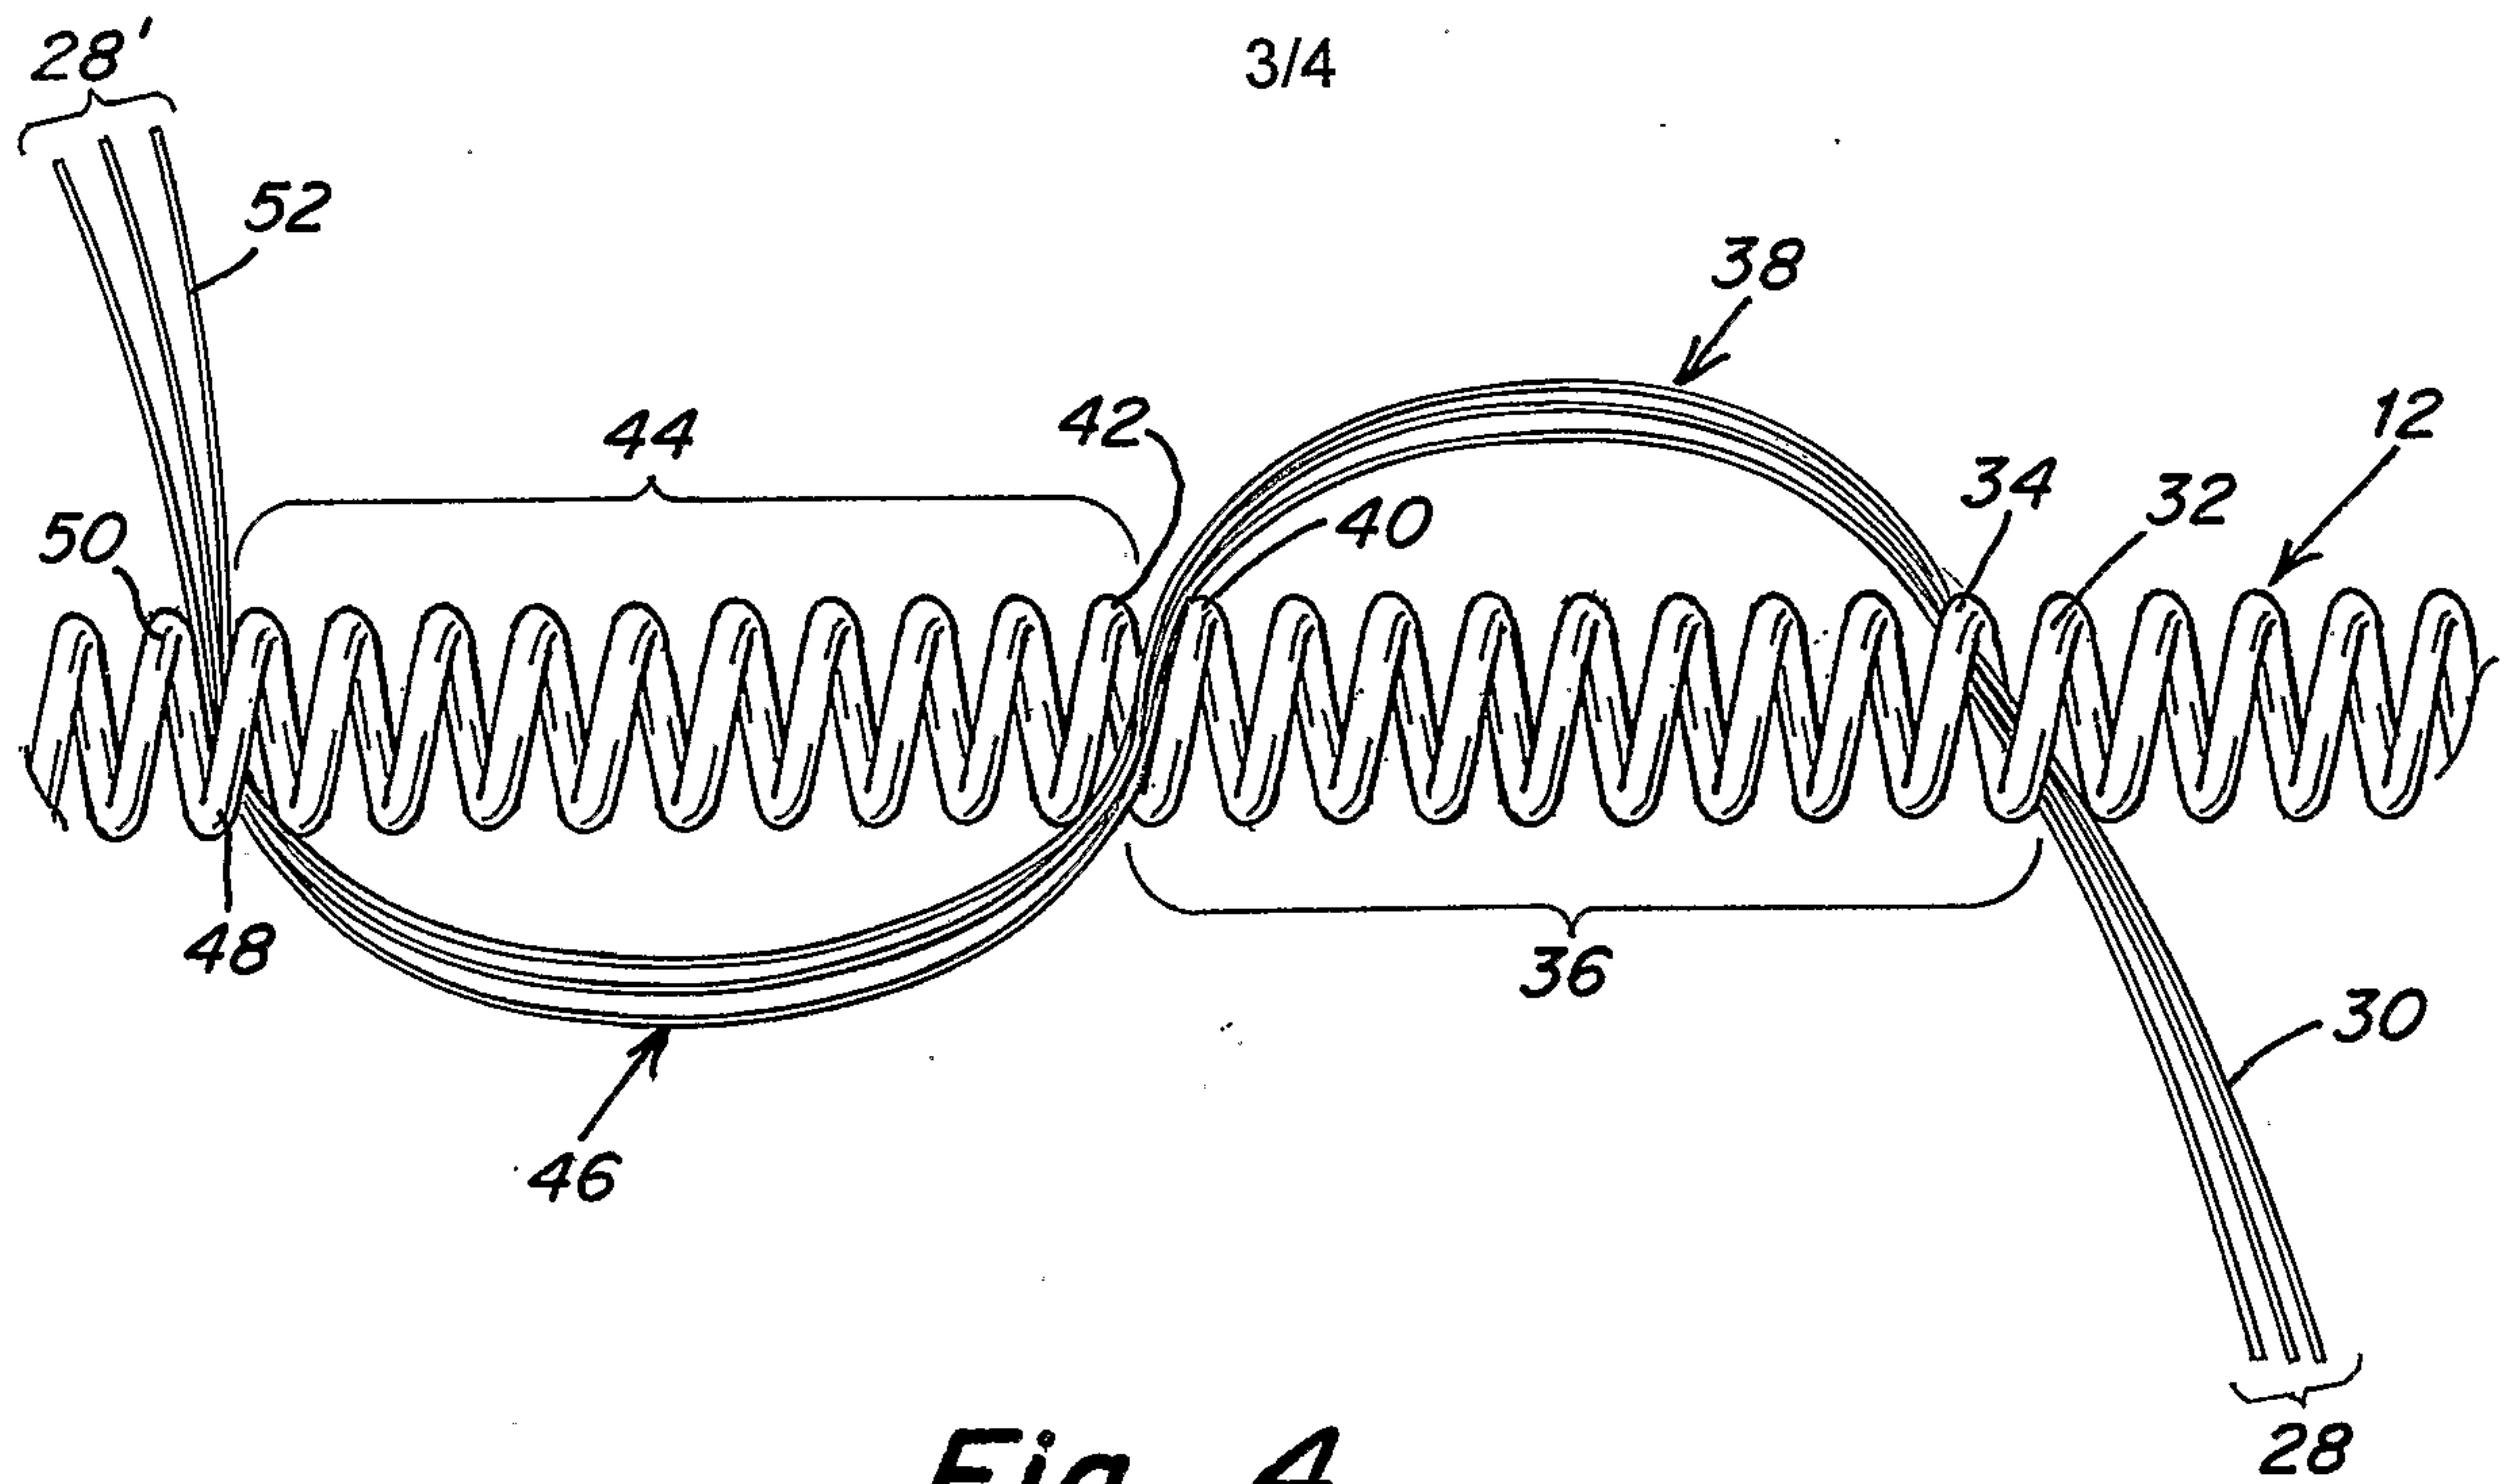


Fig. 4

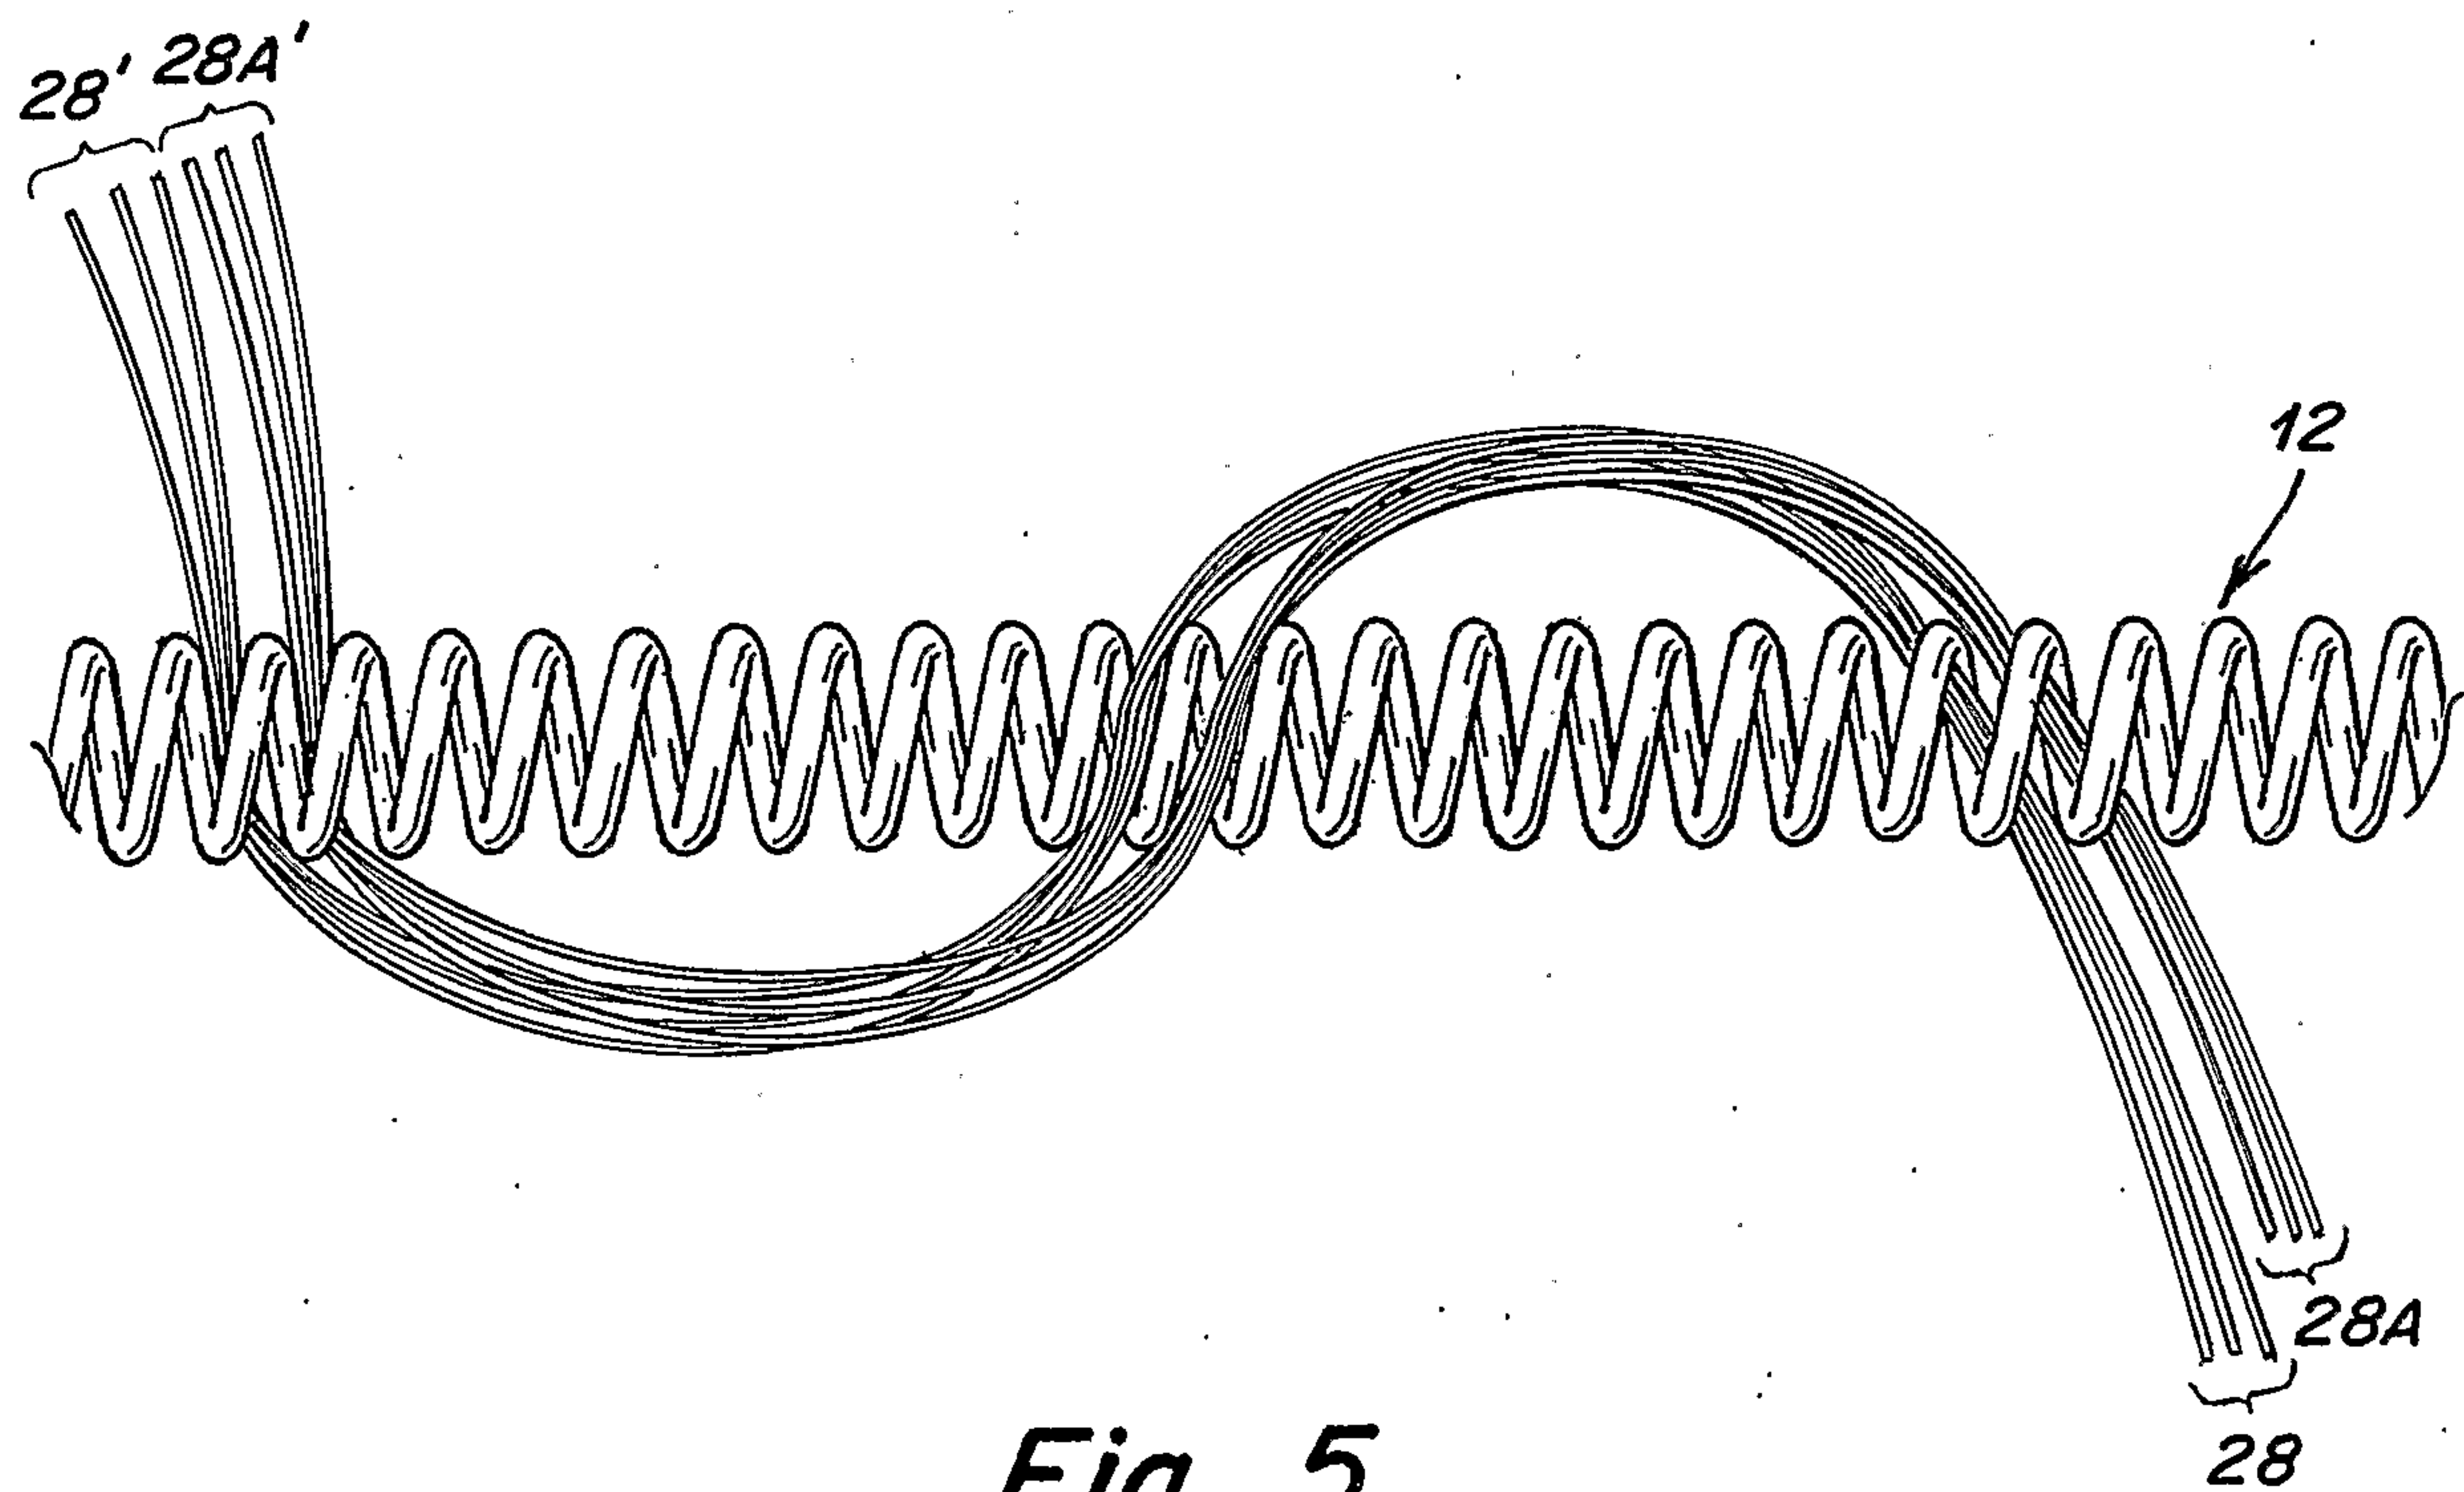


Fig. 5

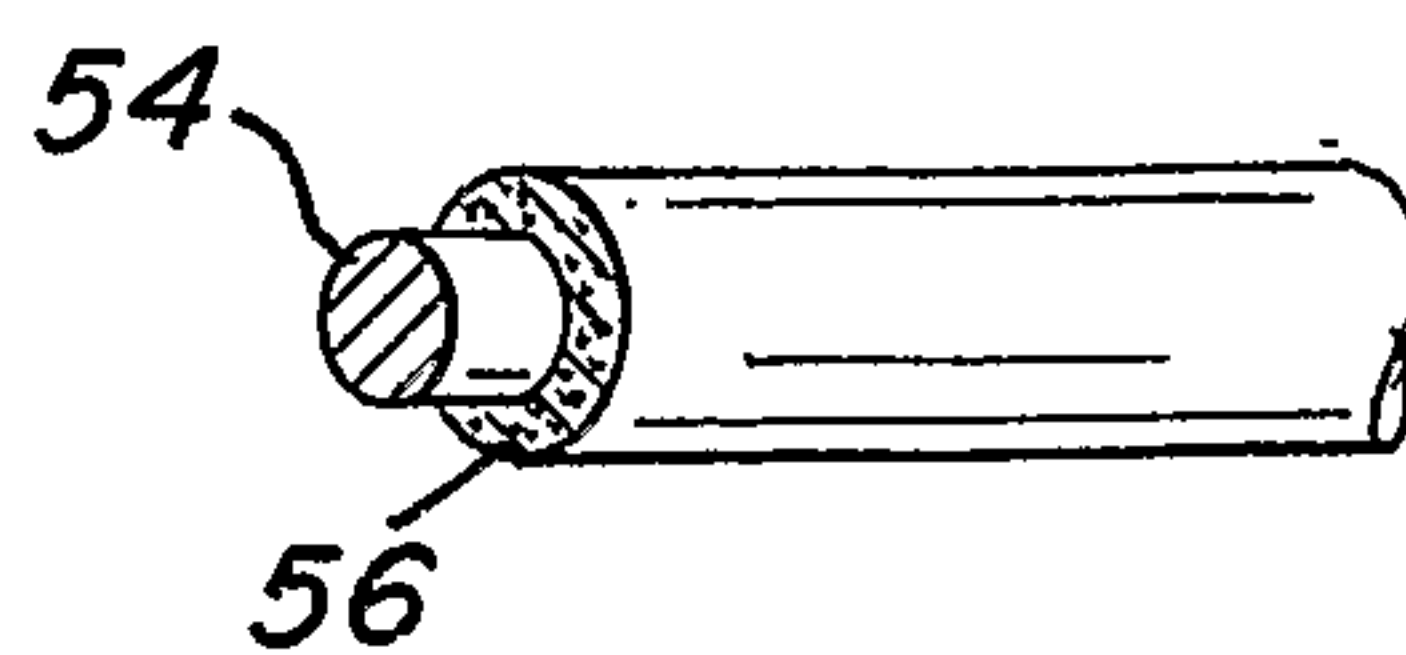


Fig. 6

4/4

Figure 7a & 7b

