



US 20160183843A1

(19) **United States**
(12) **Patent Application Publication**
Conklin et al.

(10) **Pub. No.: US 2016/0183843 A1**
(43) **Pub. Date: Jun. 30, 2016**

(54) **CATHETER-BASED CLUTCHED HEART VALVE SIZER**
(71) Applicant: **Edwards Lifesciences Corporation**, Irvine, CA (US)
(72) Inventors: **Brian S. Conklin**, Orange, CA (US); **Da-Yu Chang**, Irvine, CA (US)

A61B 5/00 (2006.01)
A61F 2/24 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 5/1076* (2013.01); *A61F 2/2496* (2013.01); *A61B 5/02028* (2013.01); *A61B 5/6859* (2013.01); *A61B 2090/065* (2016.02)

(21) Appl. No.: **15/063,353**
(22) Filed: **Mar. 7, 2016**

(57) **ABSTRACT**


Related U.S. Application Data

(63) Continuation of application No. 14/011,602, filed on Aug. 27, 2013, now Pat. No. 9,277,996, which is a continuation-in-part of application No. 13/707,395, filed on Dec. 6, 2012.
(60) Provisional application No. 61/568,913, filed on Dec. 9, 2011.

Publication Classification

(51) **Int. Cl.**
A61B 5/107 (2006.01)
A61B 5/02 (2006.01)

A valve sizer for determining an appropriate replacement valve size when performing a heart valve replacement procedure is provided. In one version the valve sizer has a hollow shaft with proximal and distal ends. A movable sizing element couples to the distal end of the shaft and is radially expandable between first, contracted and second, expanded positions. An actuator assembly on a handle includes an actuator coupled to a clutch member via a ball-spring-detent clutch. A rod extends through the shaft and maintains a fixed distance between the handle and a distal hub in the sizing element. Movement of the actuator causes axial movement of the shaft, thereby causing radial expansion of sizing petals relative to the hub. The clutch slips when a predetermined reaction force from the surrounding valve annulus is met by the petals.

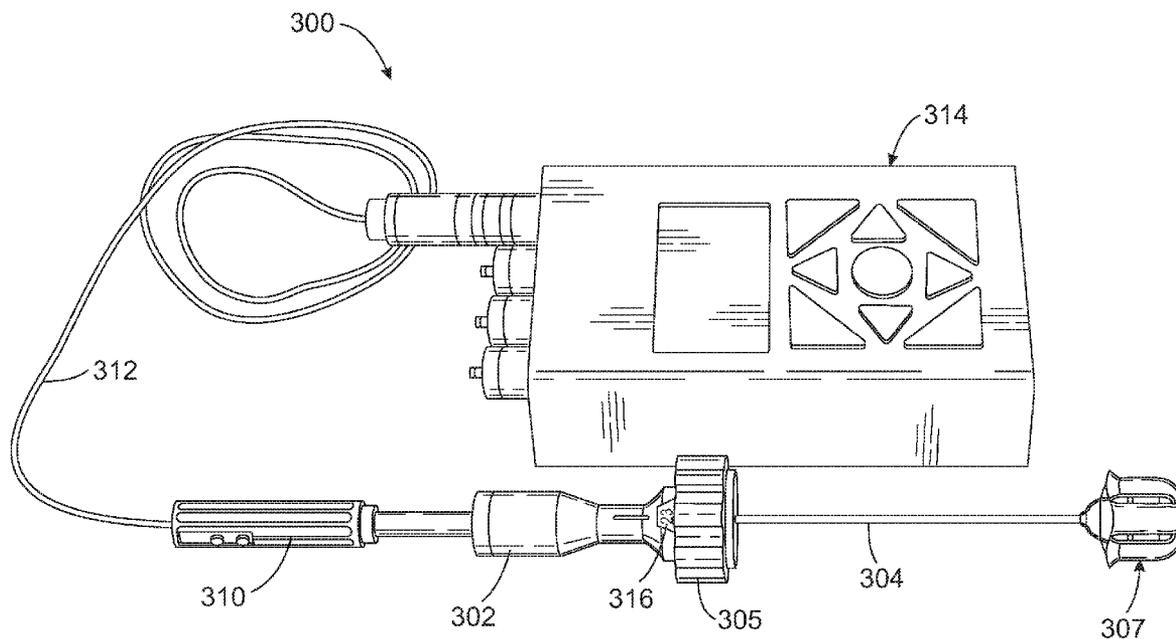

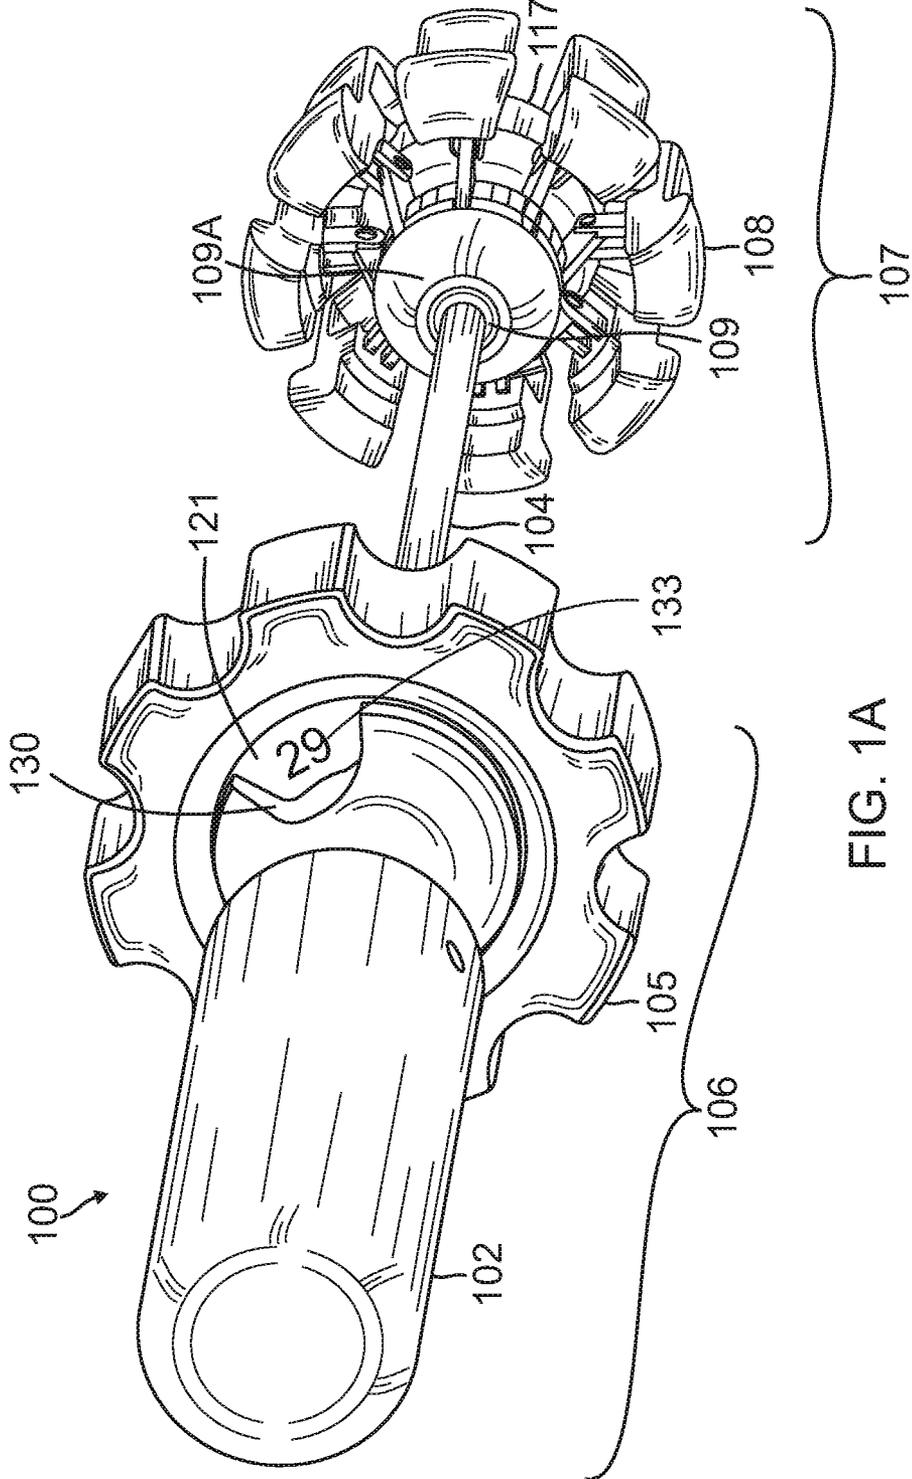
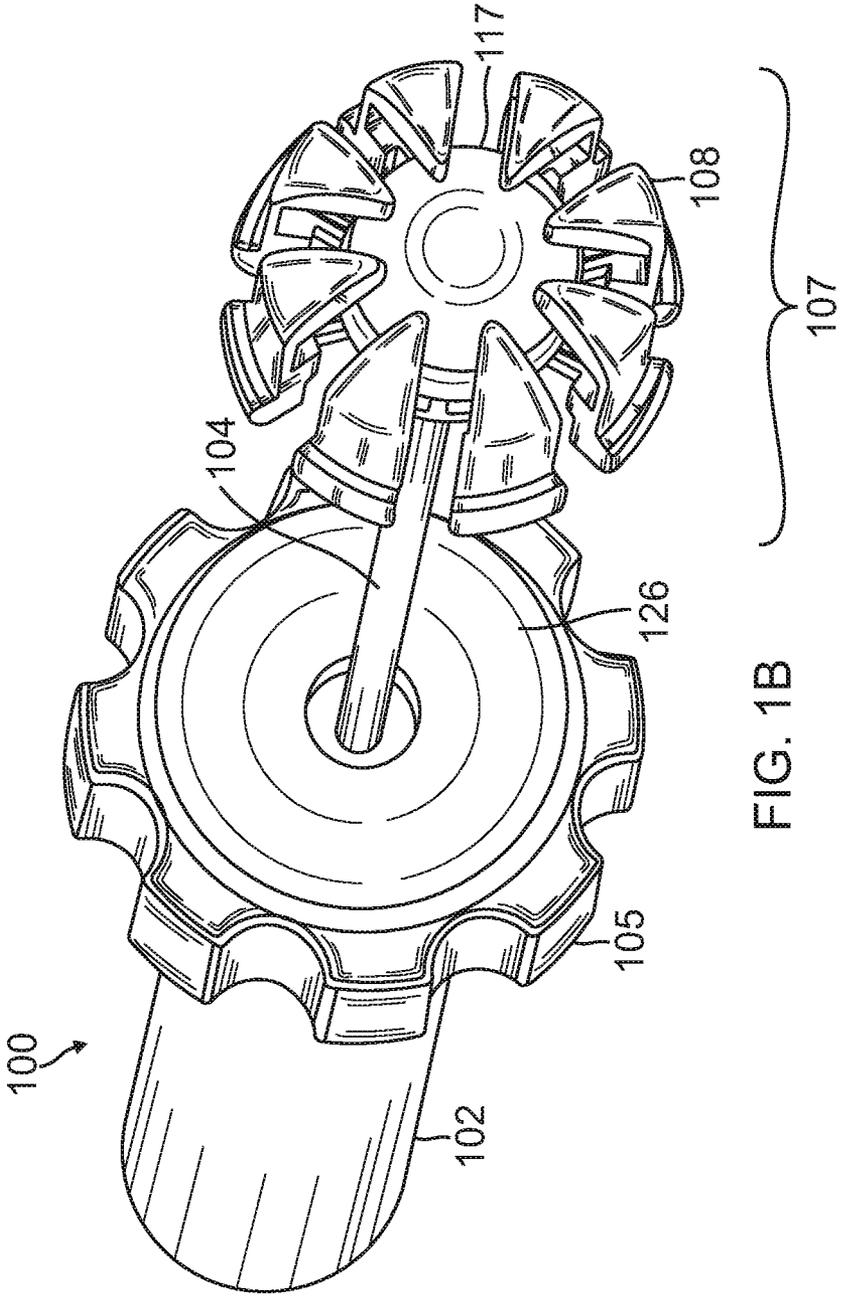


FIG. 1A



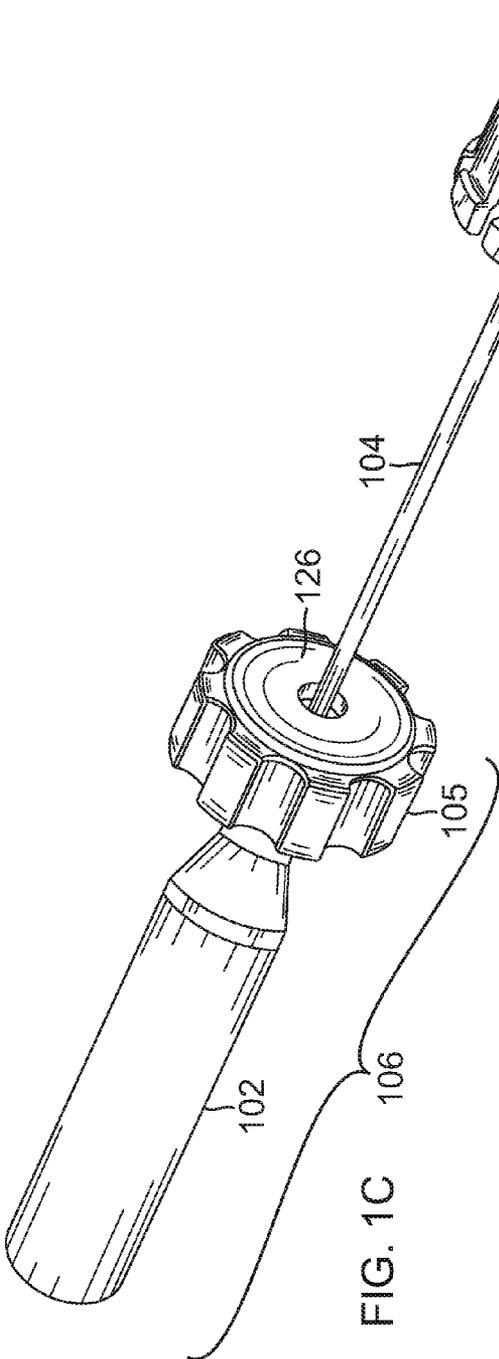


FIG. 1C

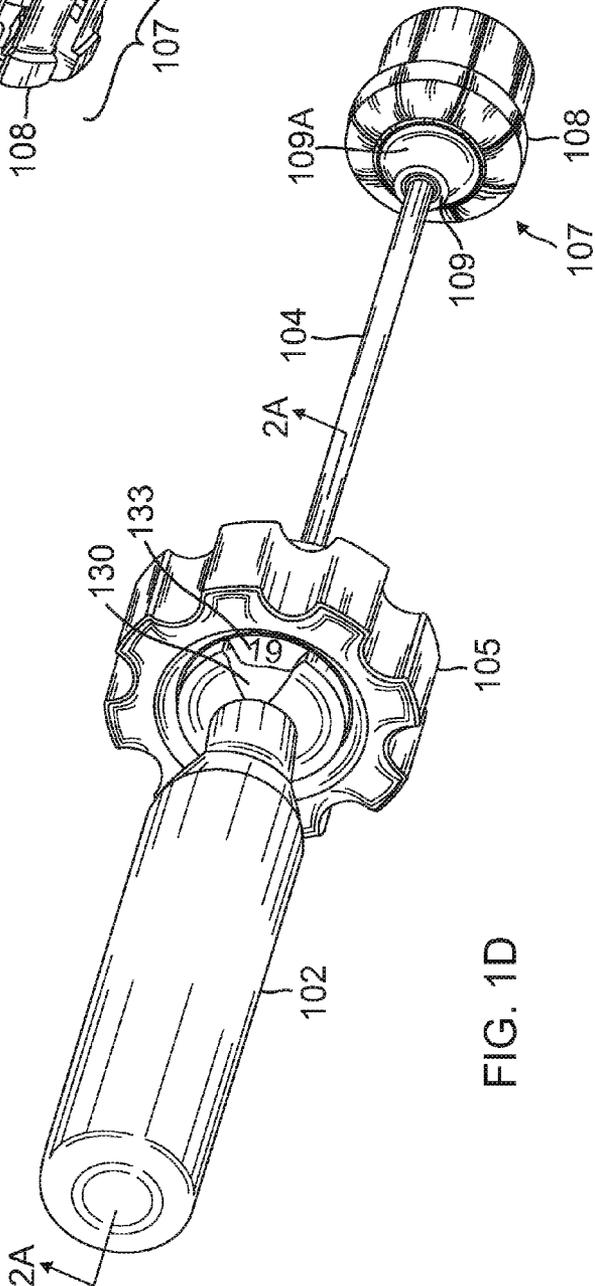


FIG. 1D

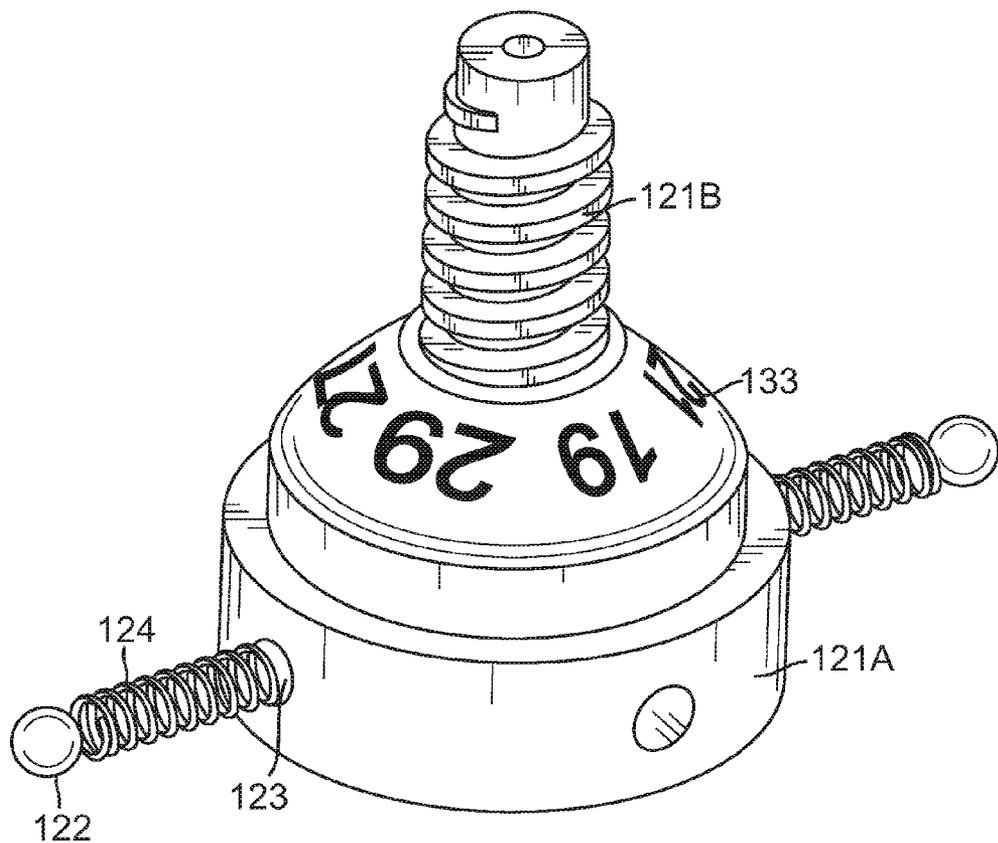


FIG. 3A

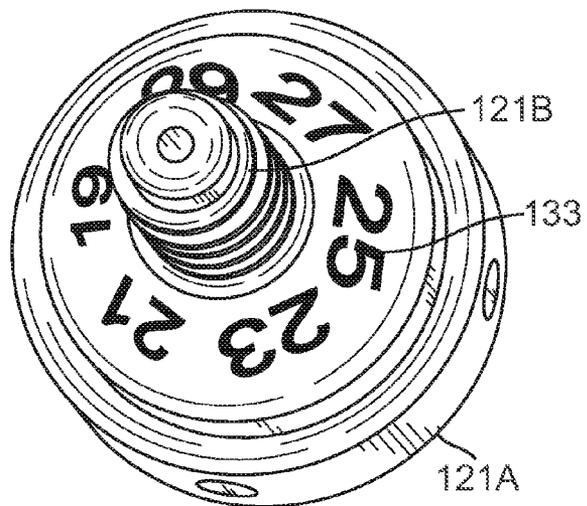


FIG. 3B

FIG. 3C

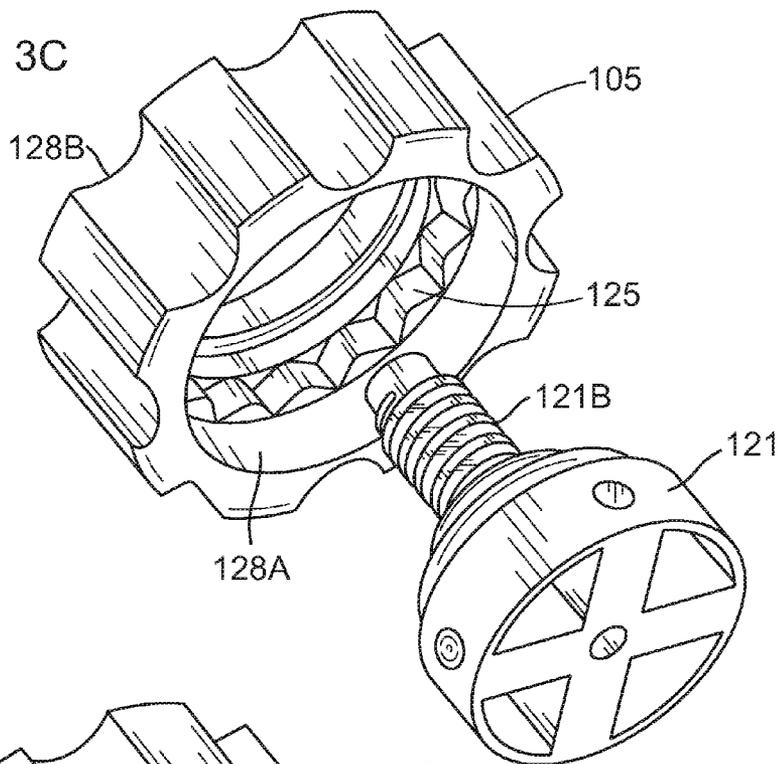


FIG. 3D

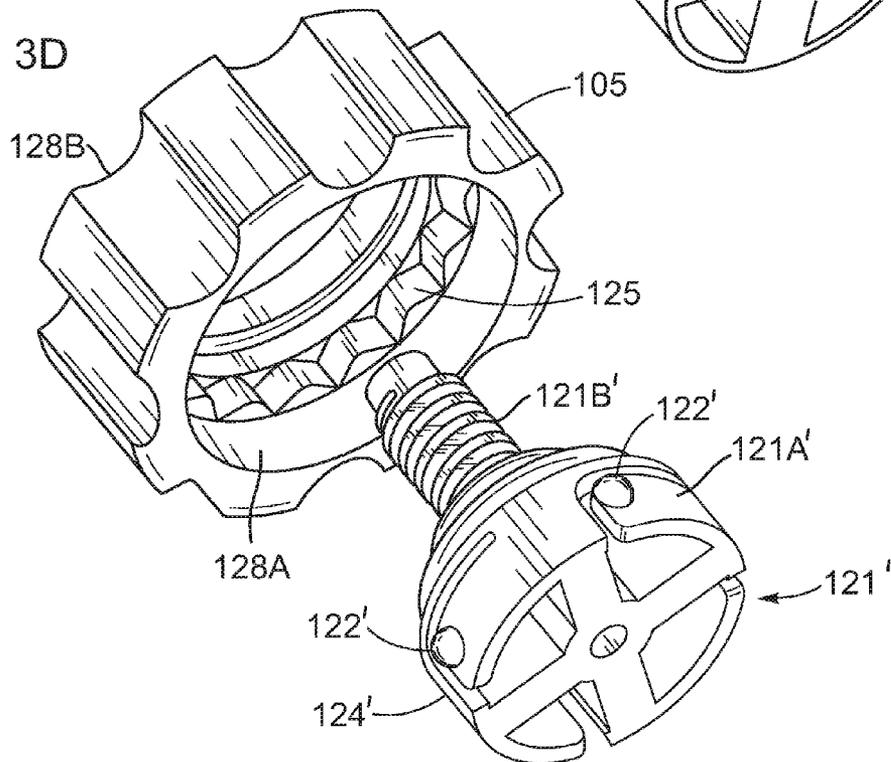


FIG. 3E

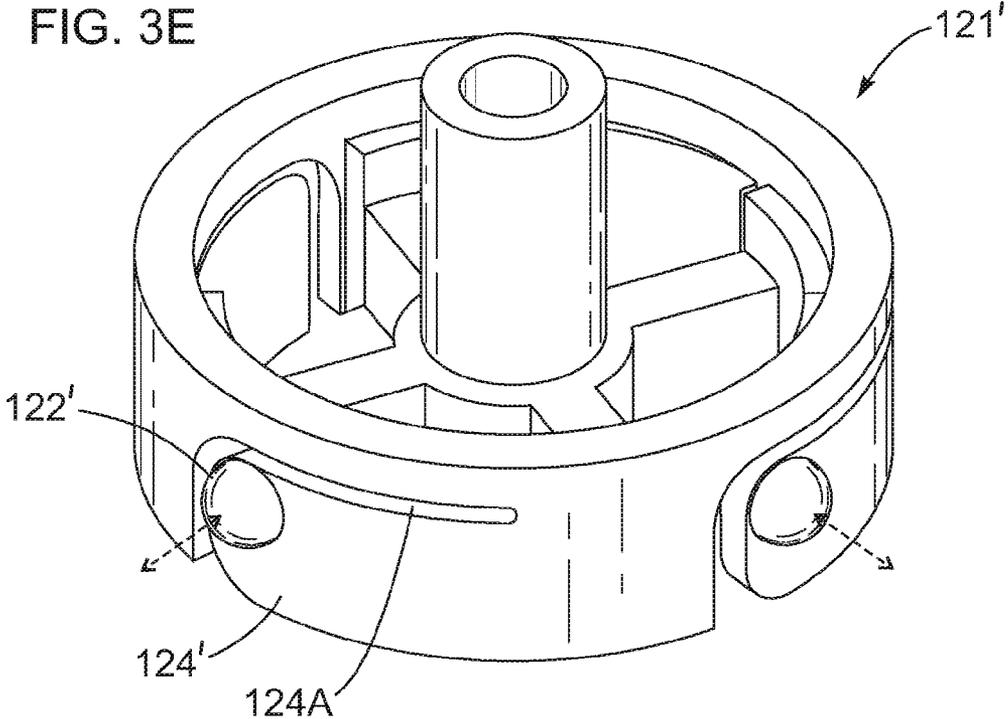
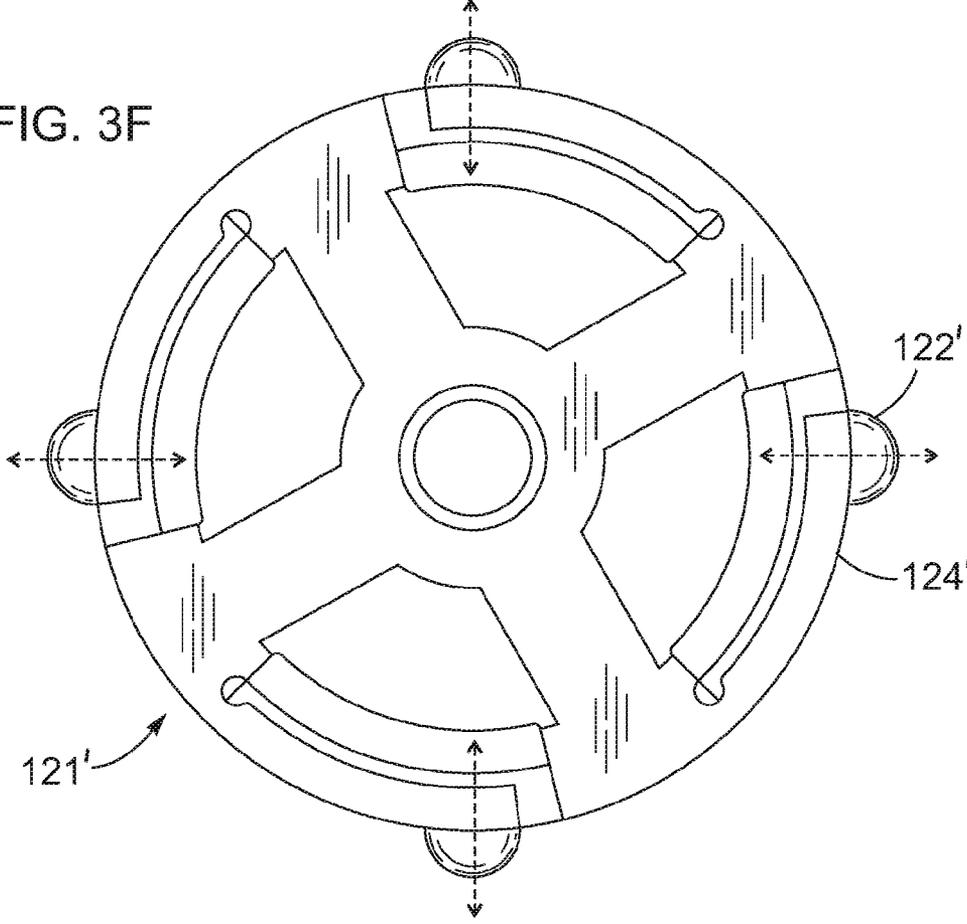
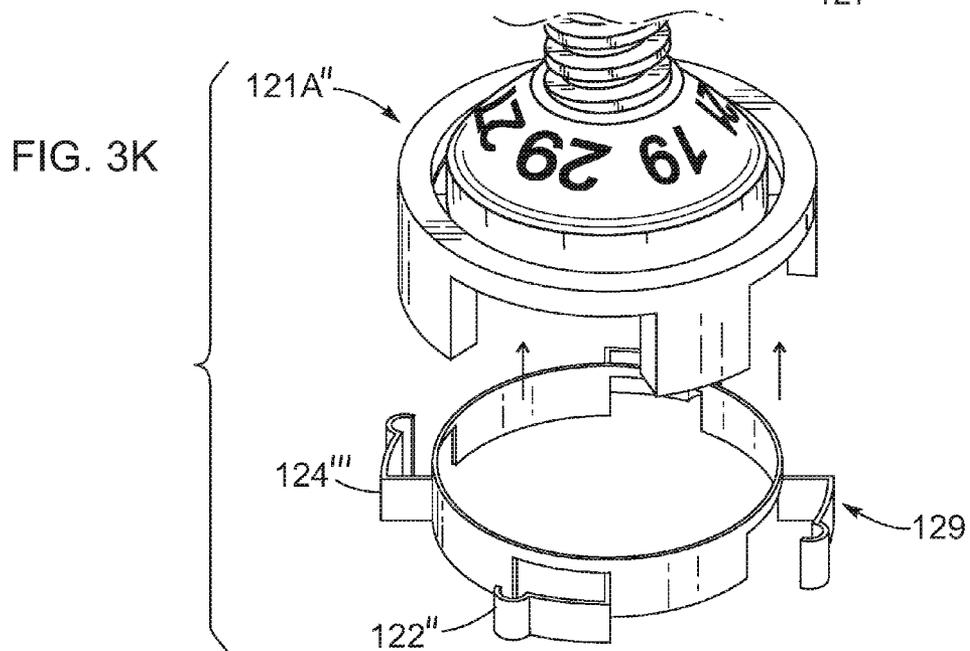
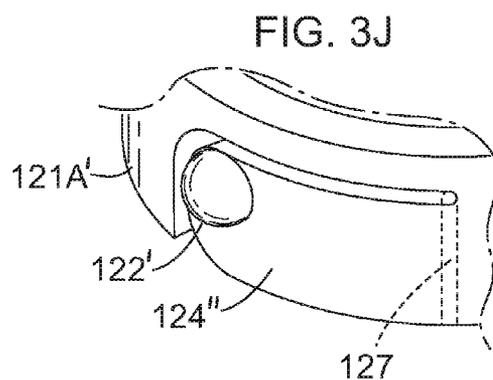
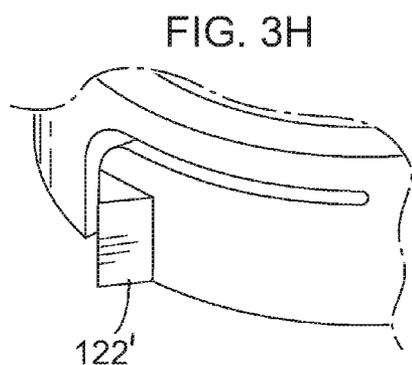
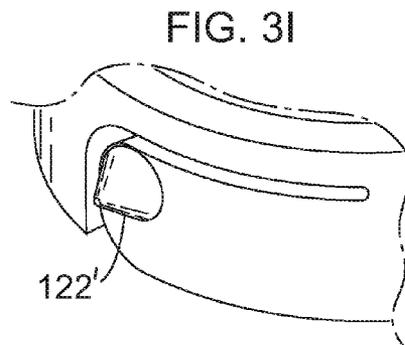
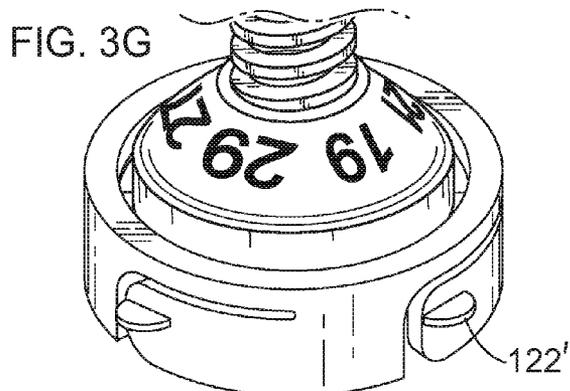
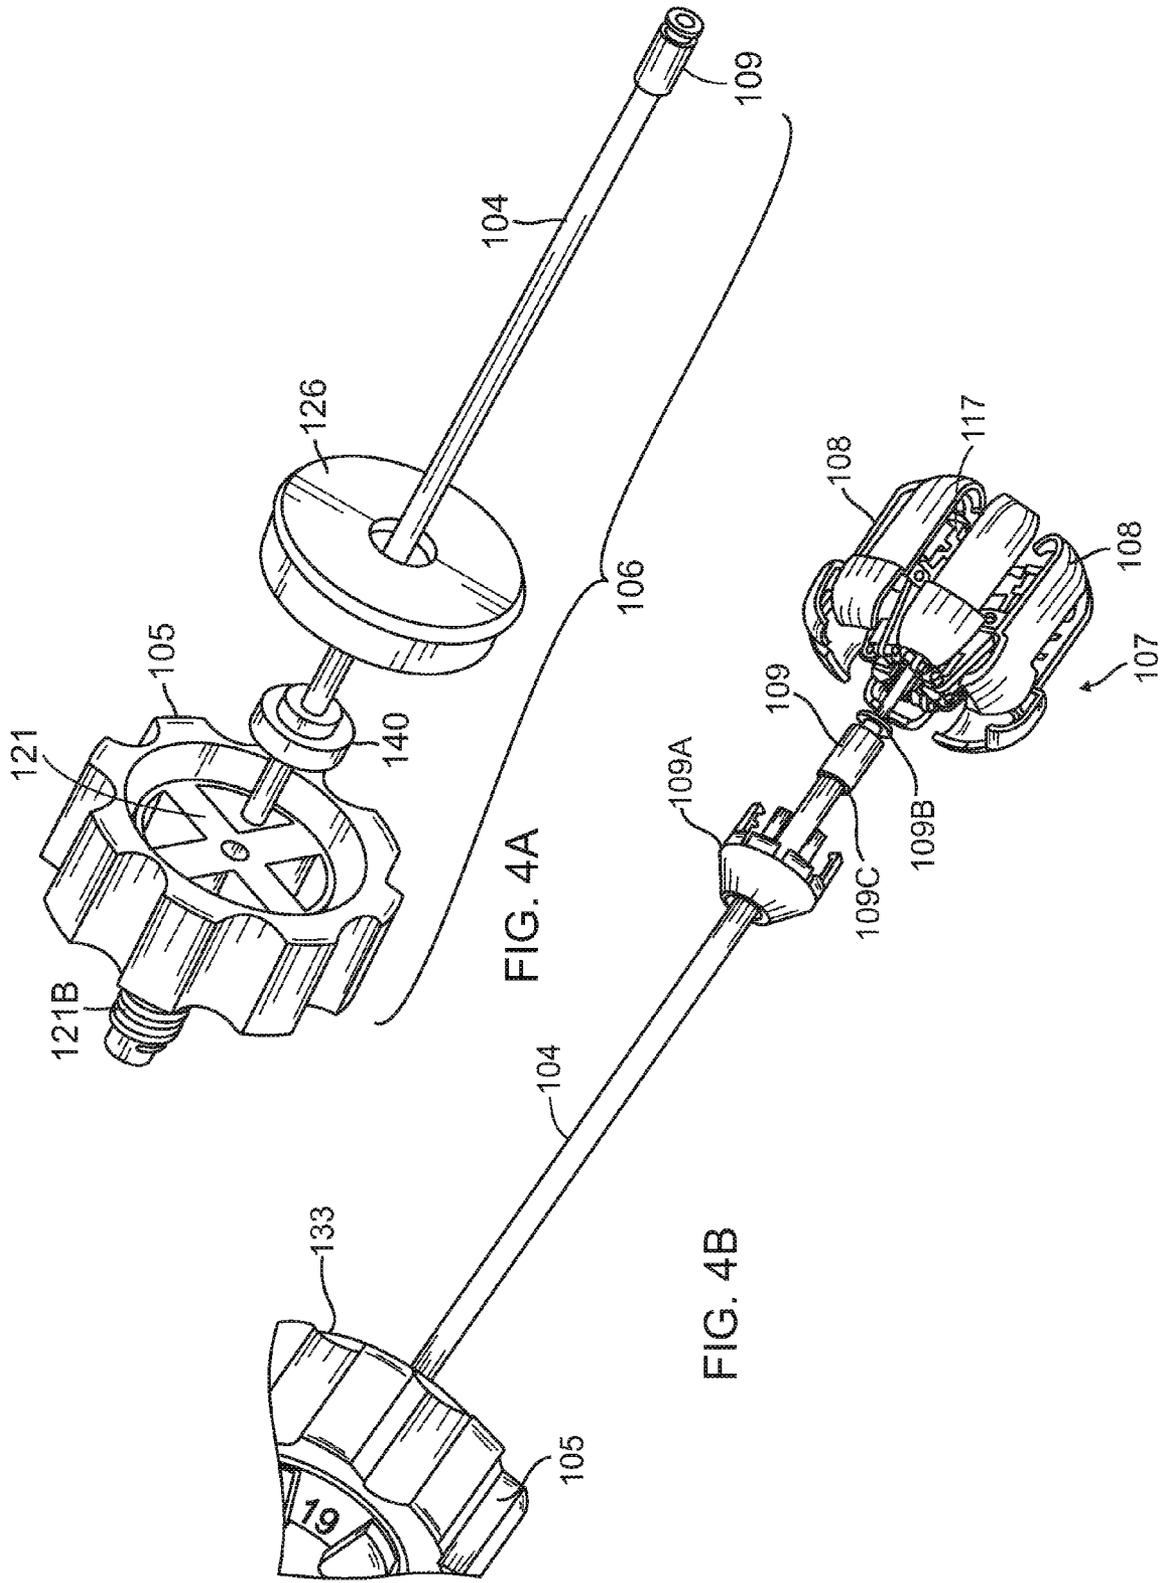


FIG. 3F







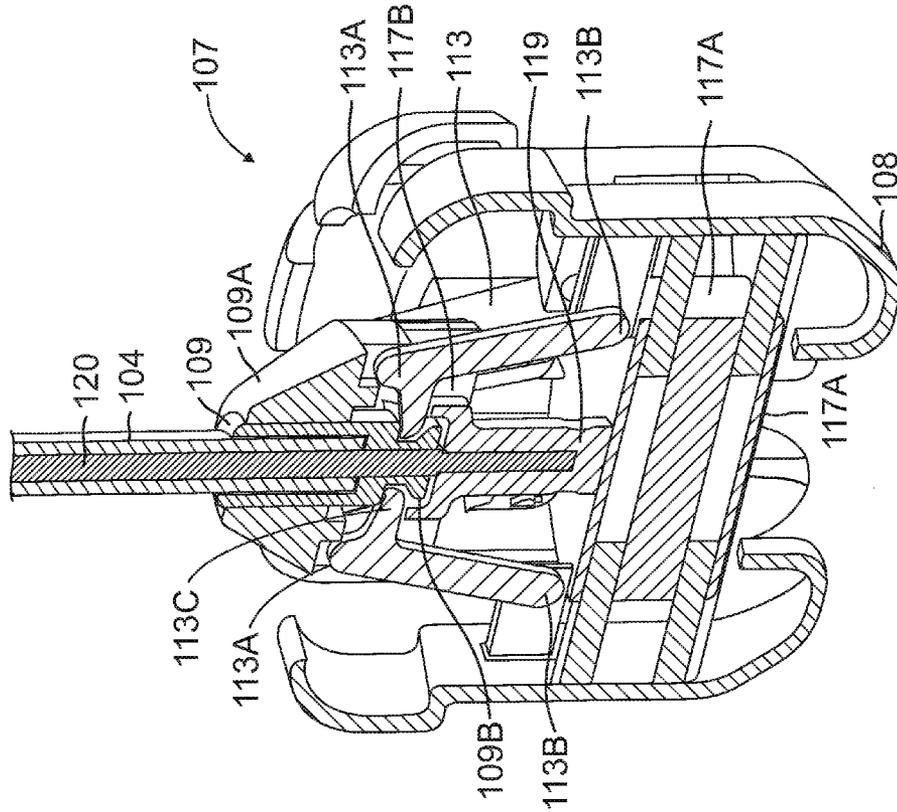


FIG. 5B

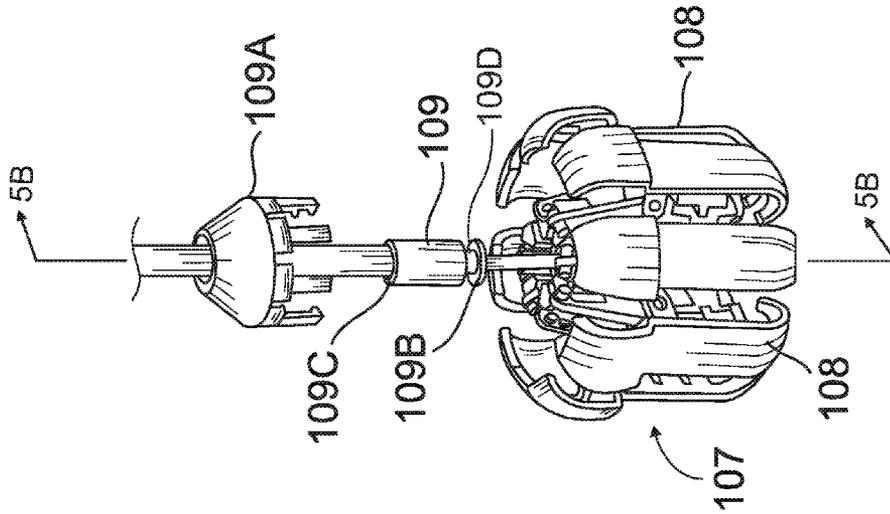


FIG. 5A

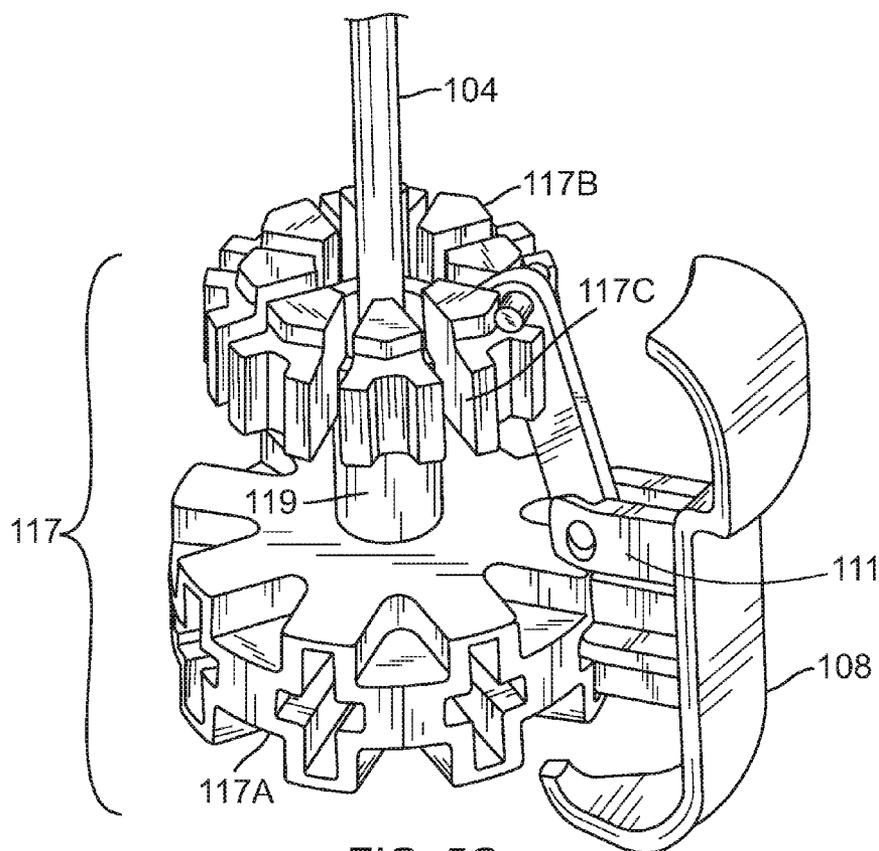


FIG. 5C

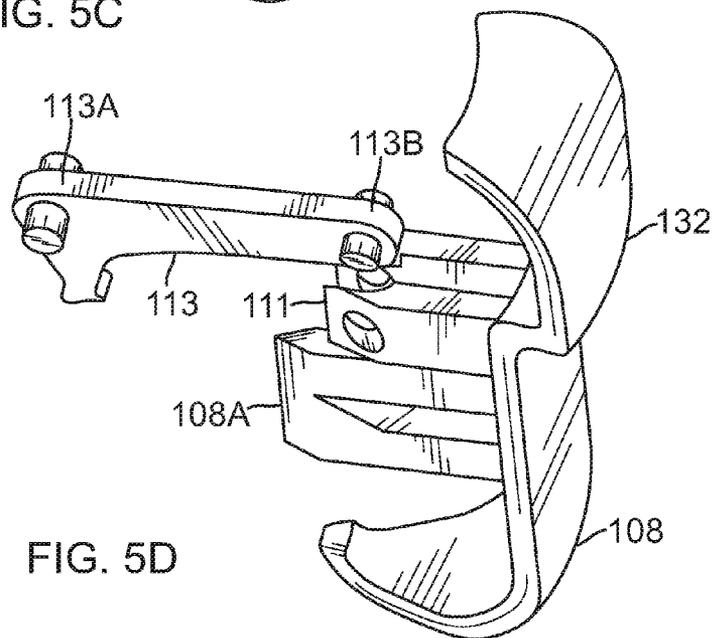


FIG. 5D

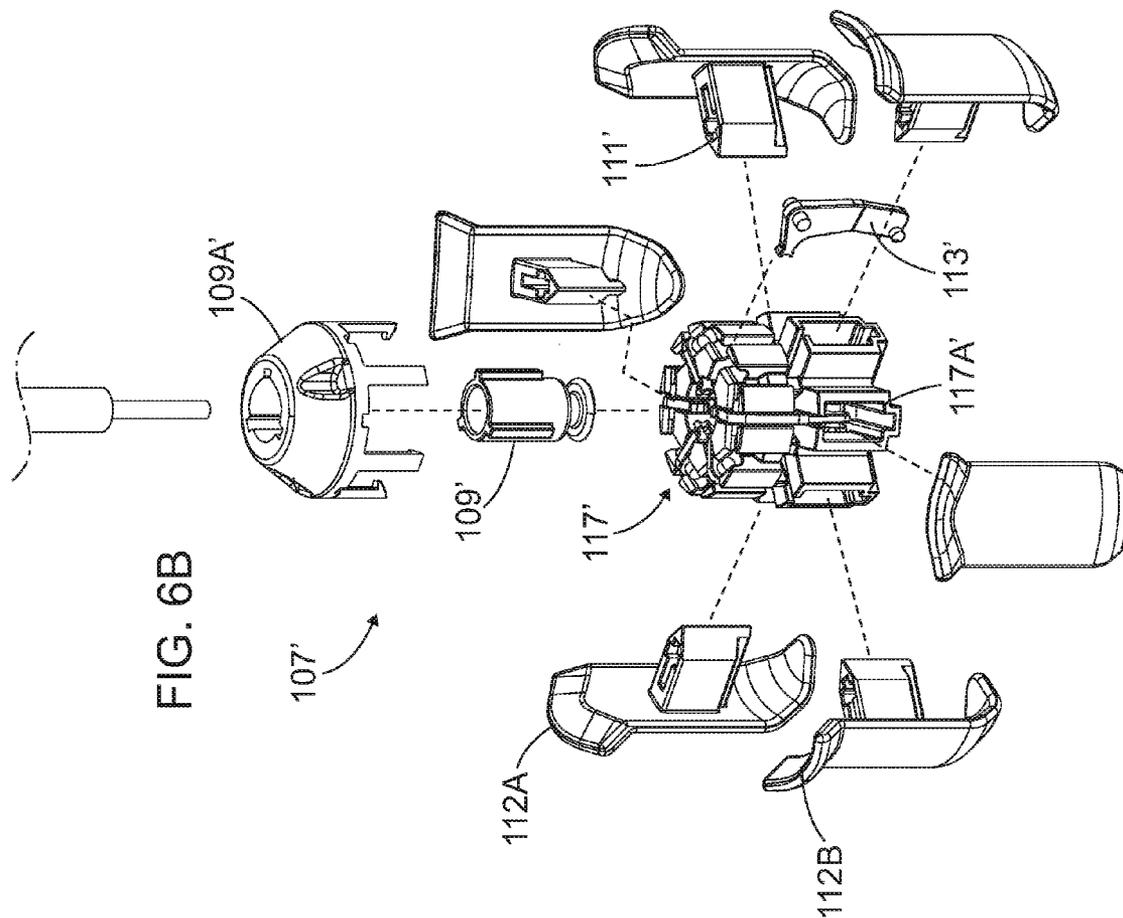
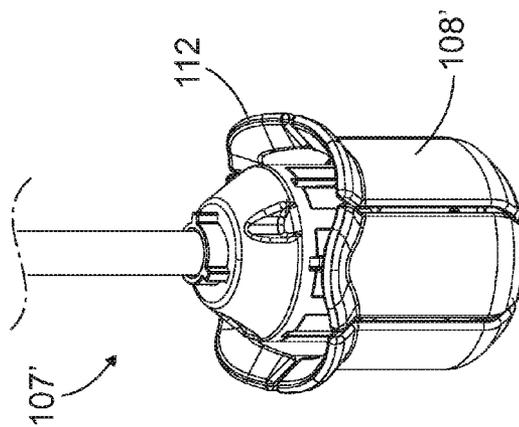


FIG. 6B

FIG. 6A



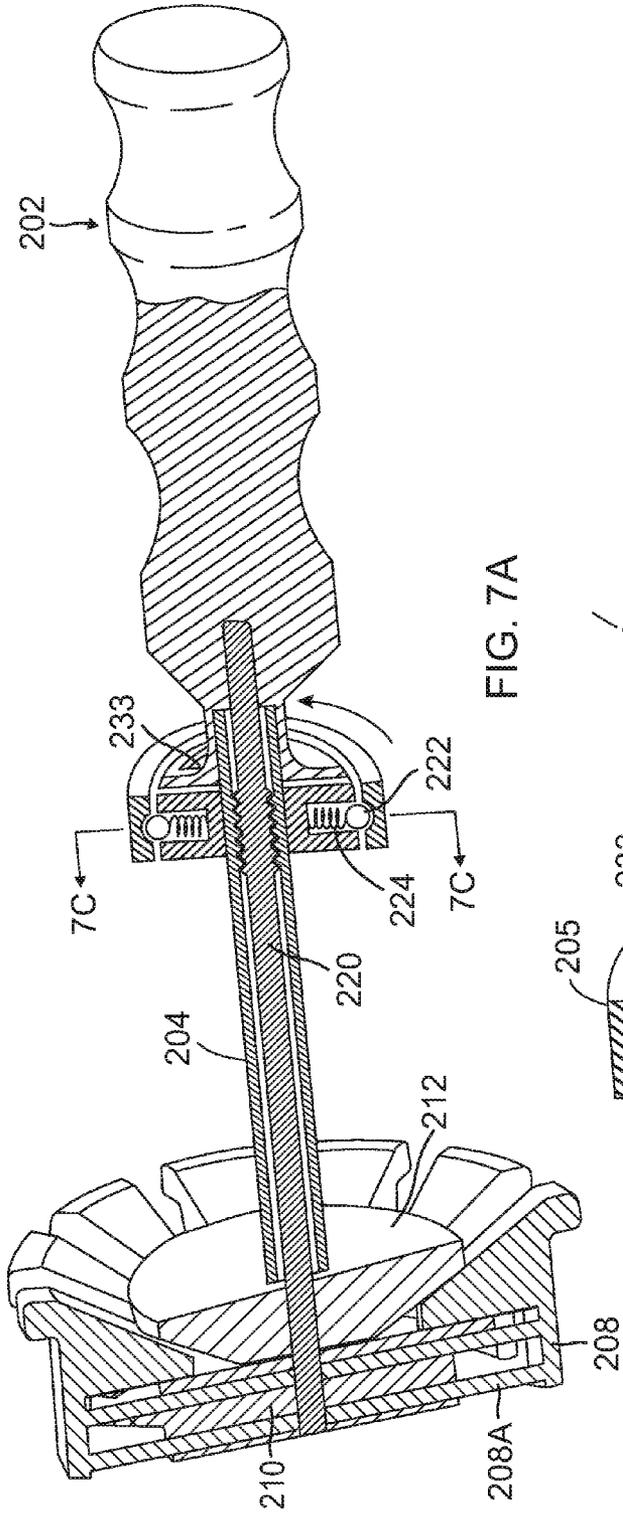


FIG. 7A

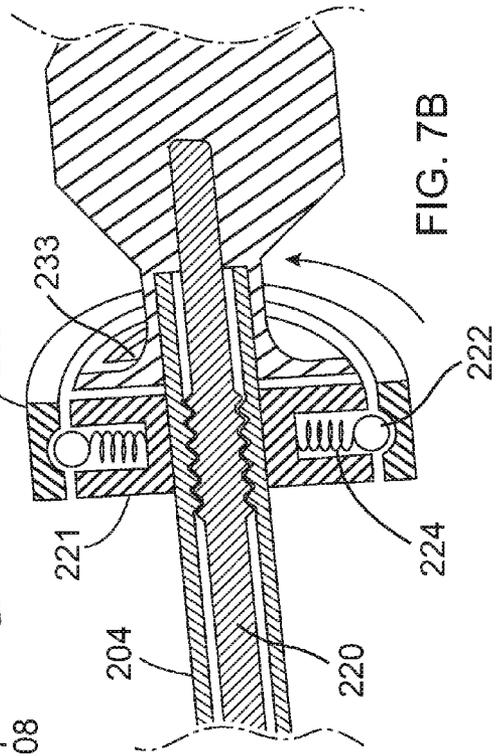


FIG. 7B

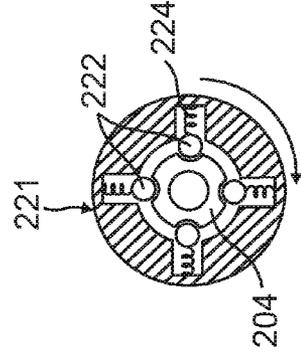


FIG. 7C

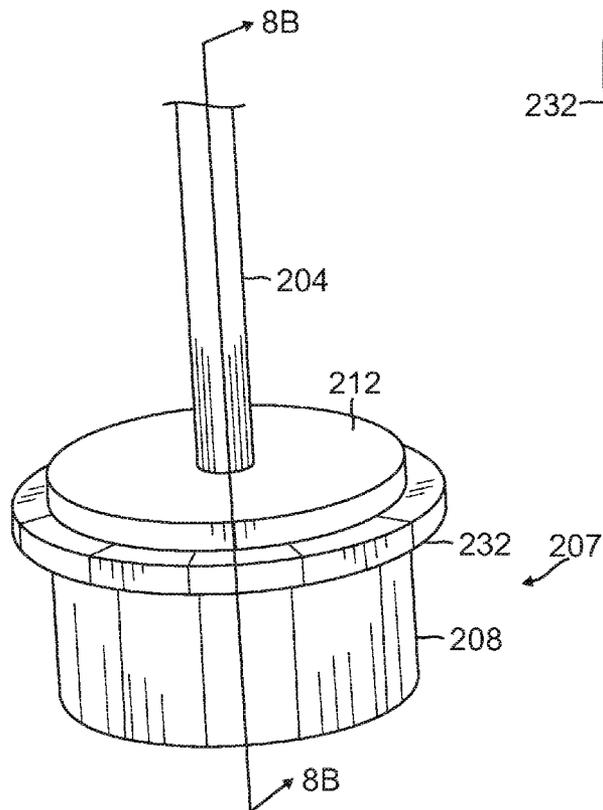


FIG. 8A

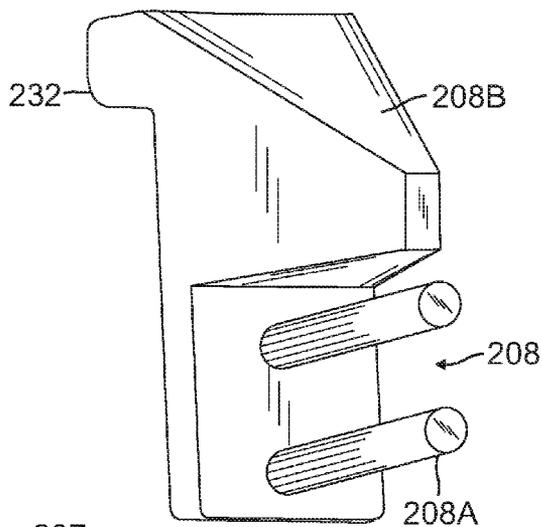


FIG. 8C

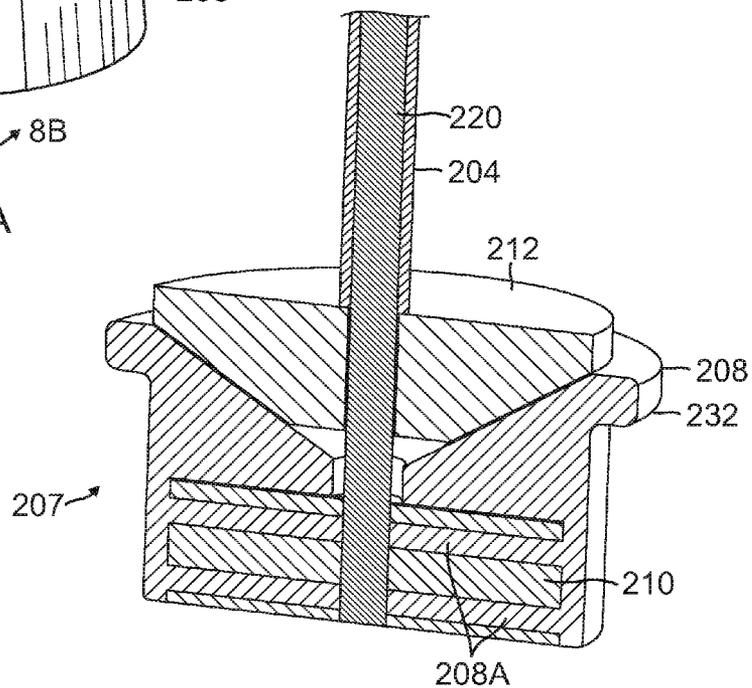


FIG. 8B

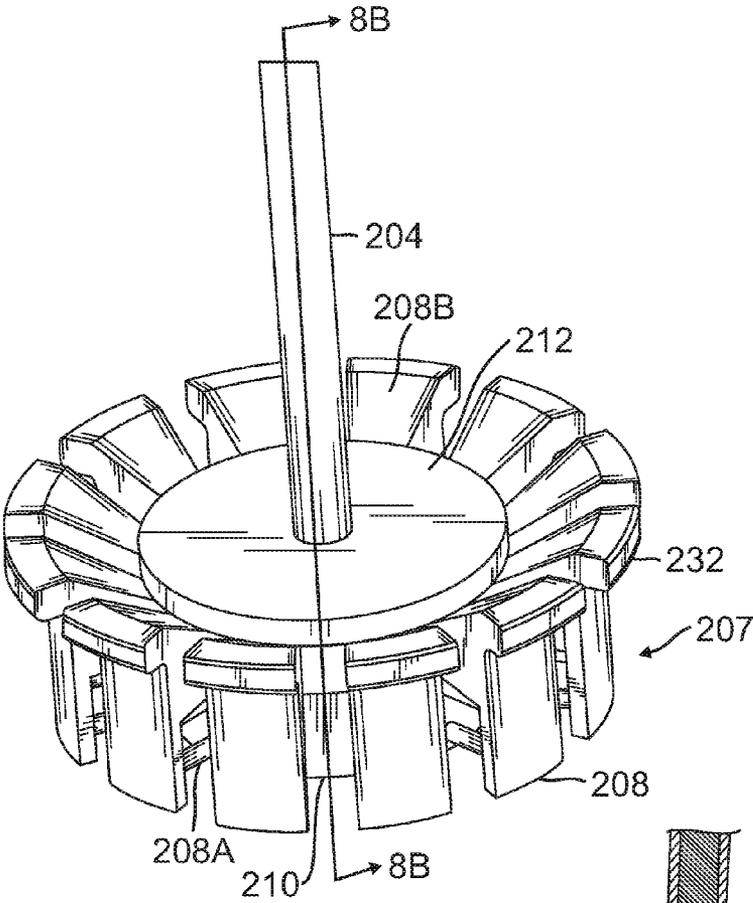


FIG. 9A

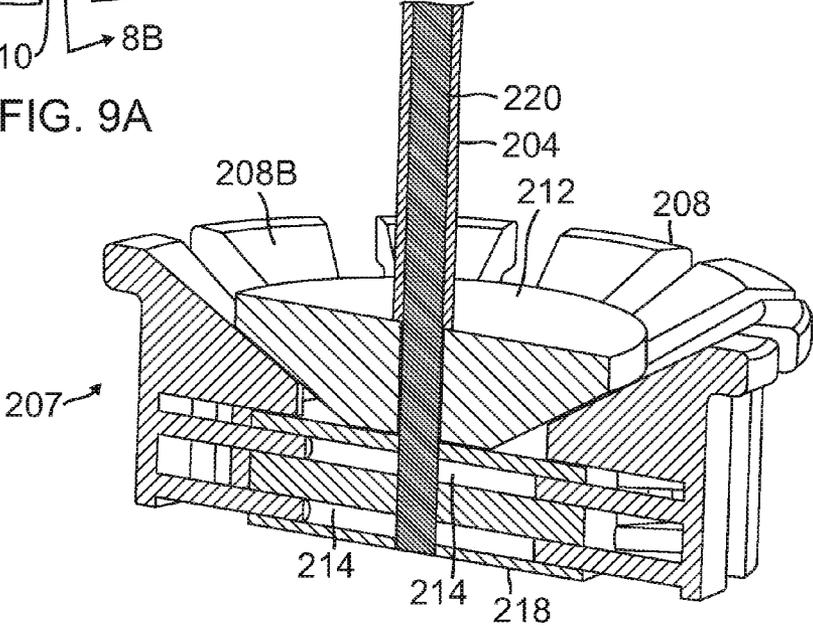


FIG. 9B

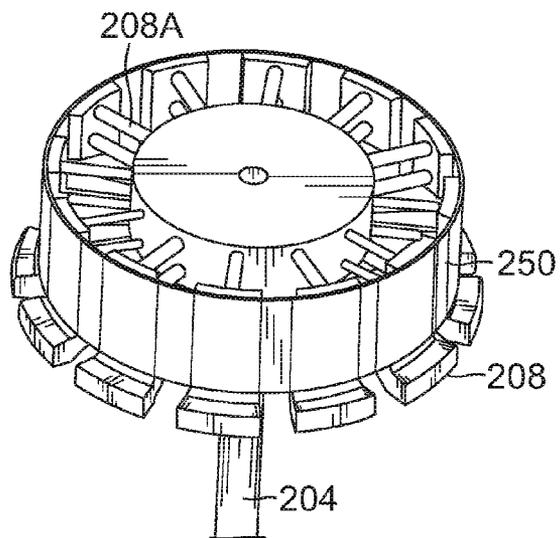


FIG. 12

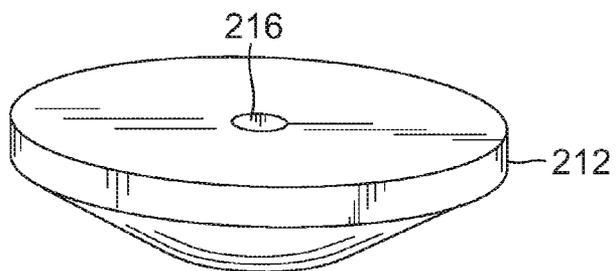


FIG. 10

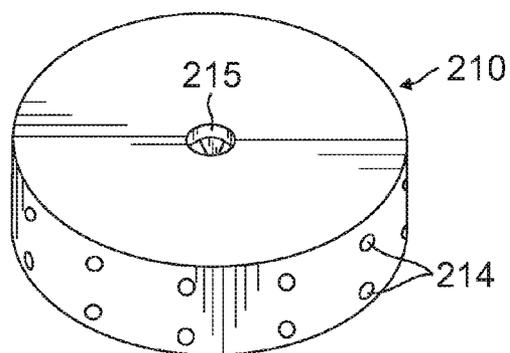


FIG. 11

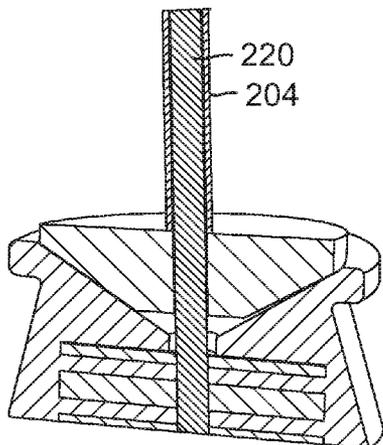


FIG. 13A

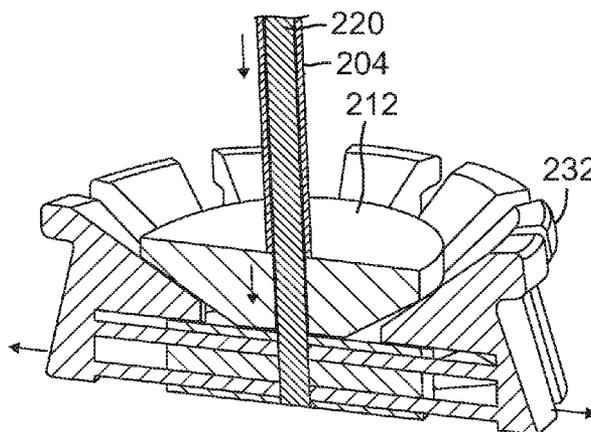


FIG. 13B

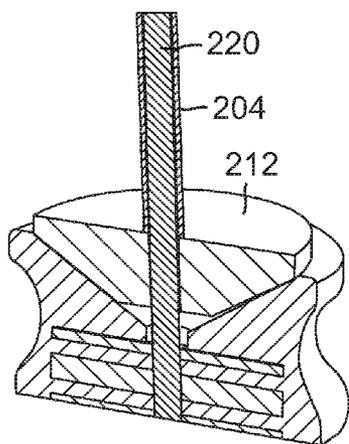


FIG. 14A

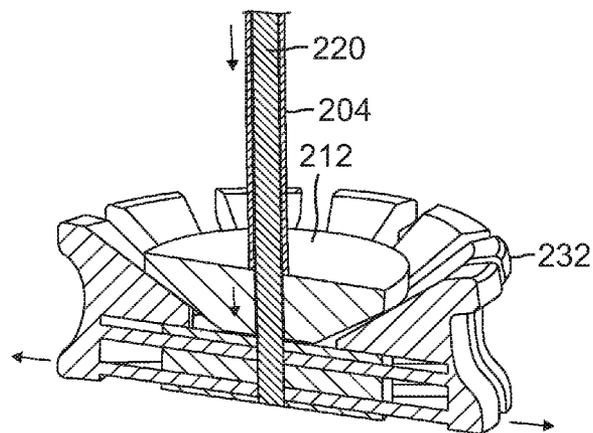
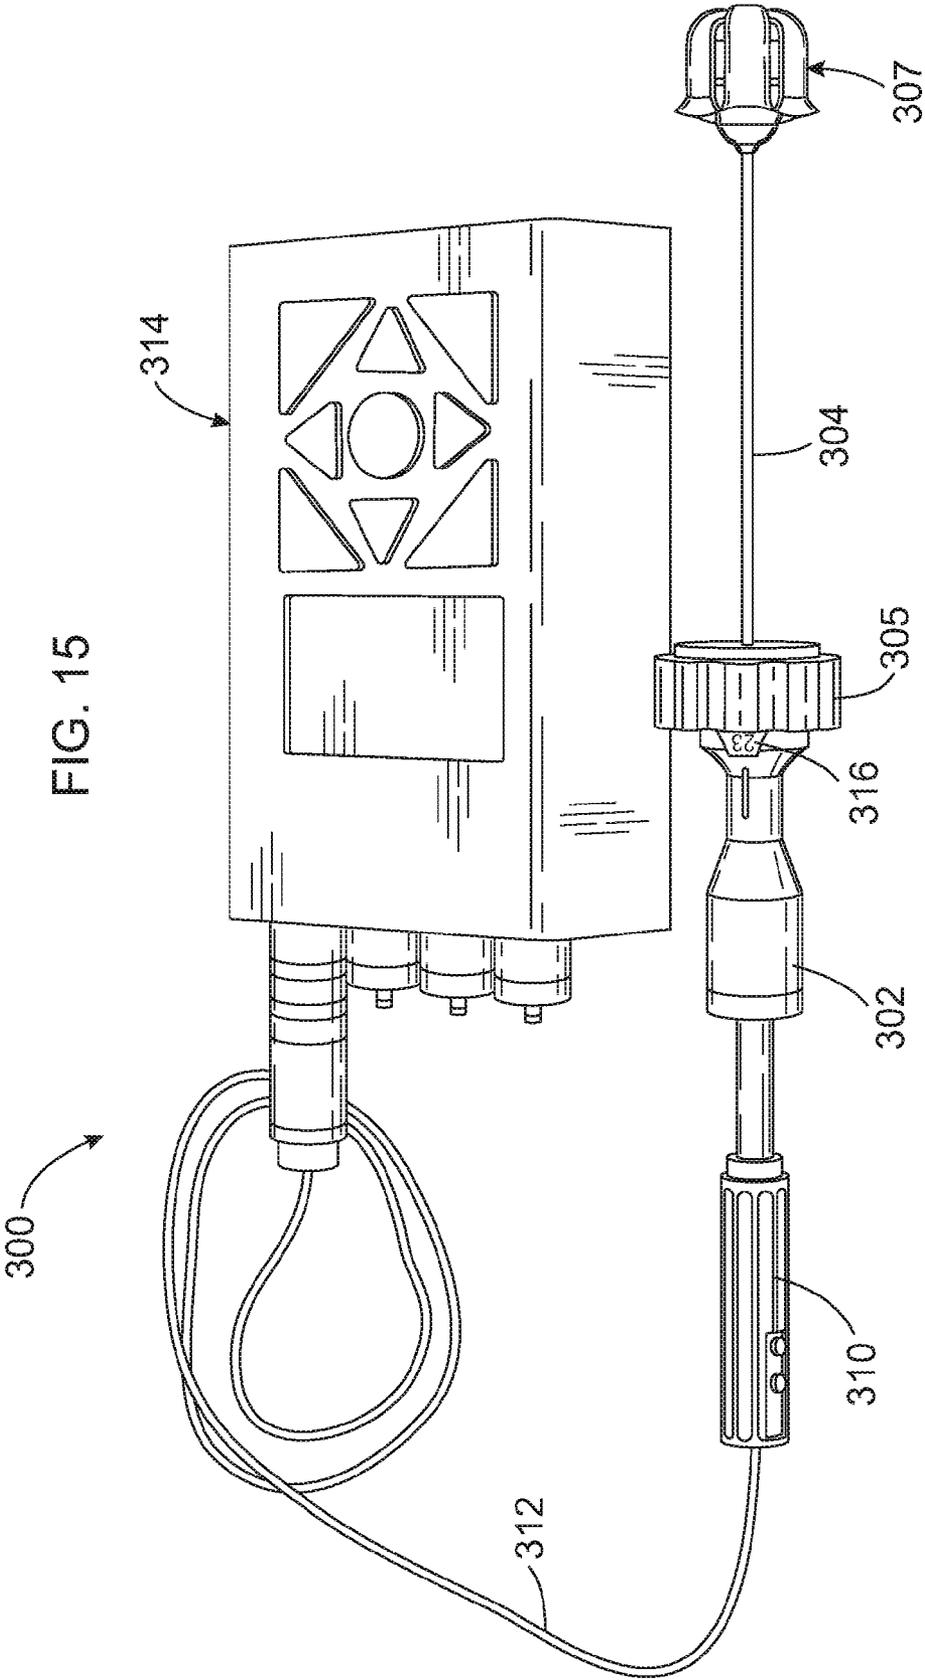
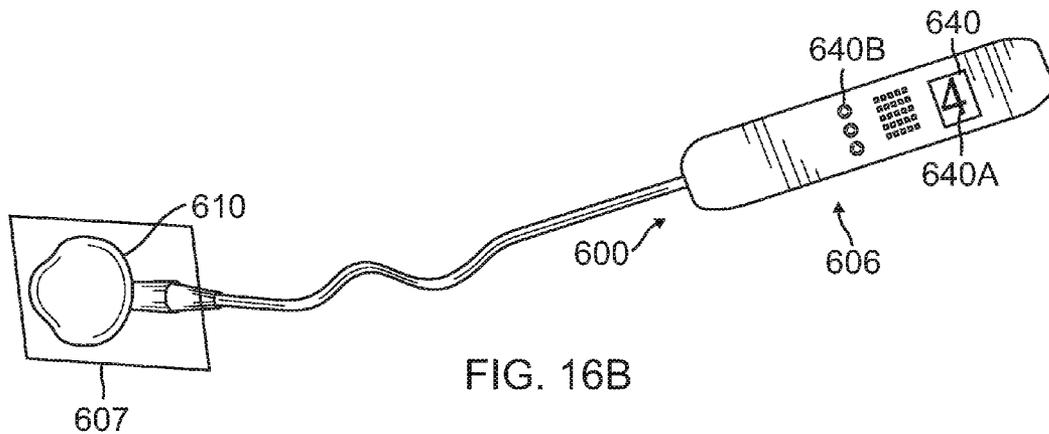
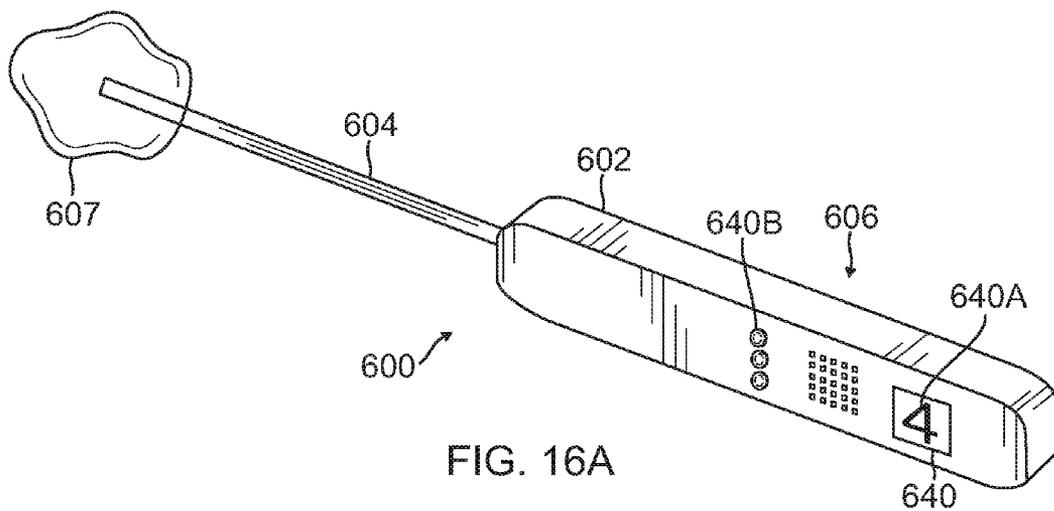


FIG. 14B





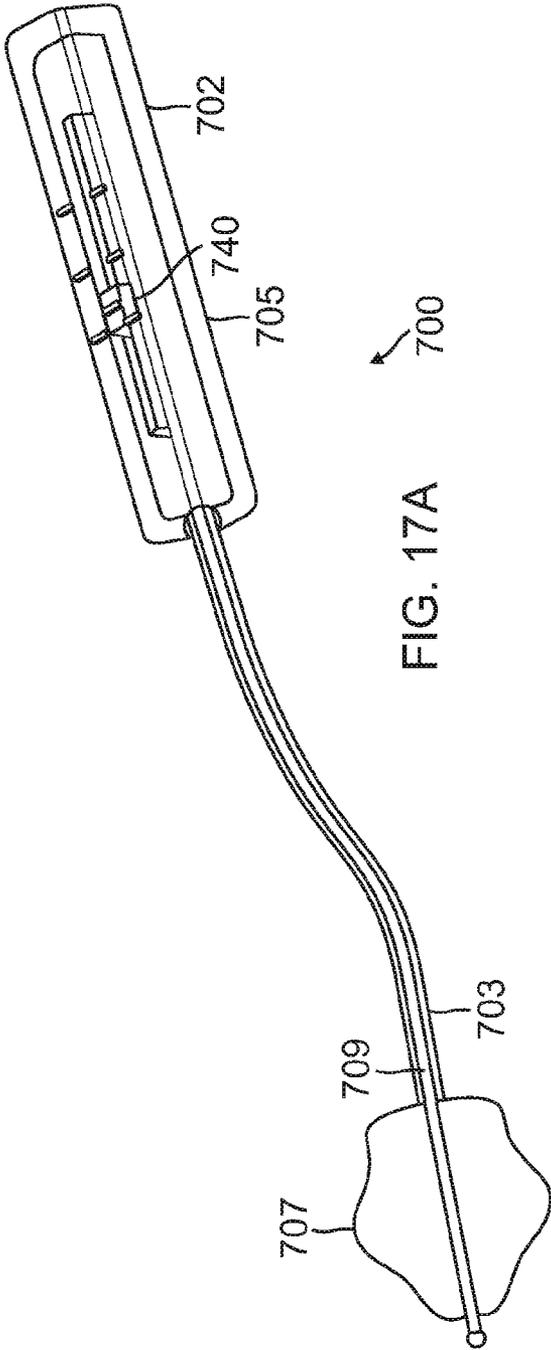


FIG. 17A

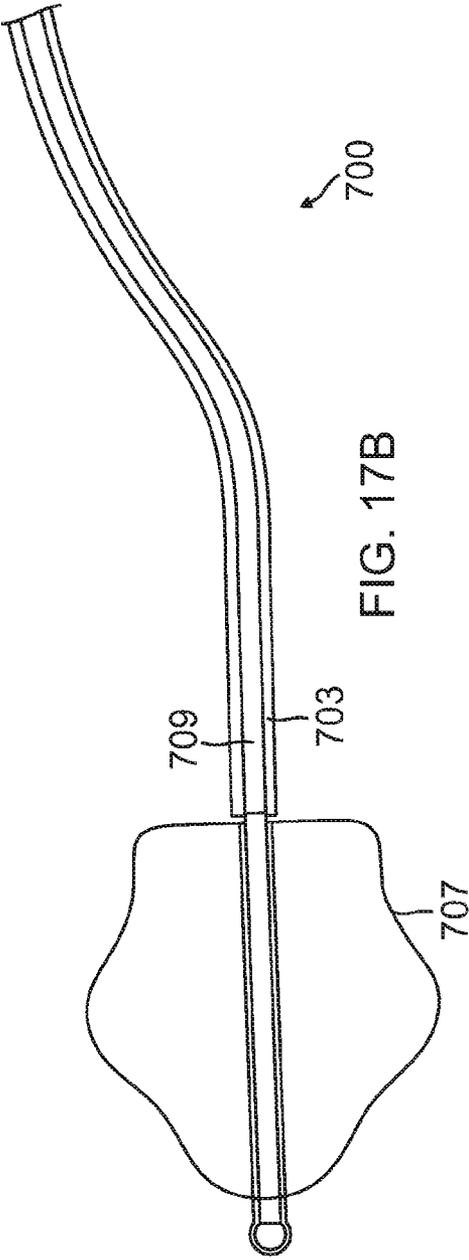


FIG. 17B

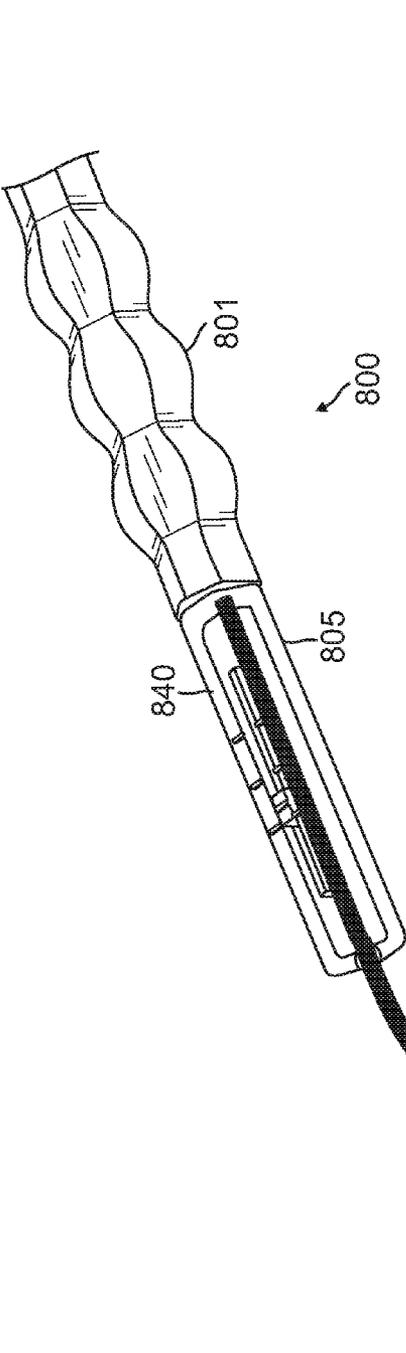


FIG. 18A

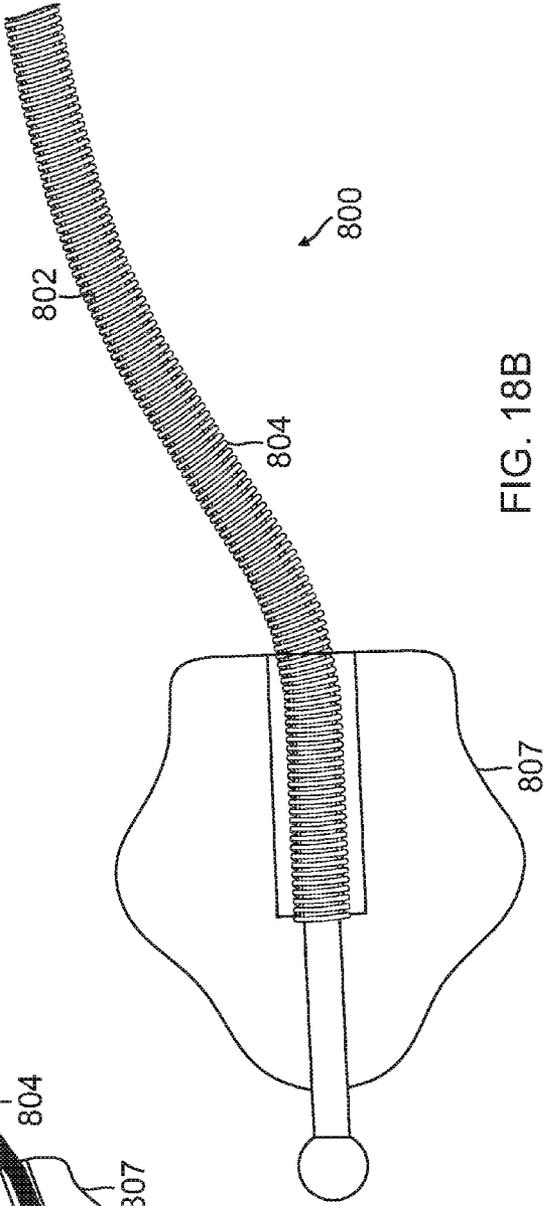


FIG. 18B

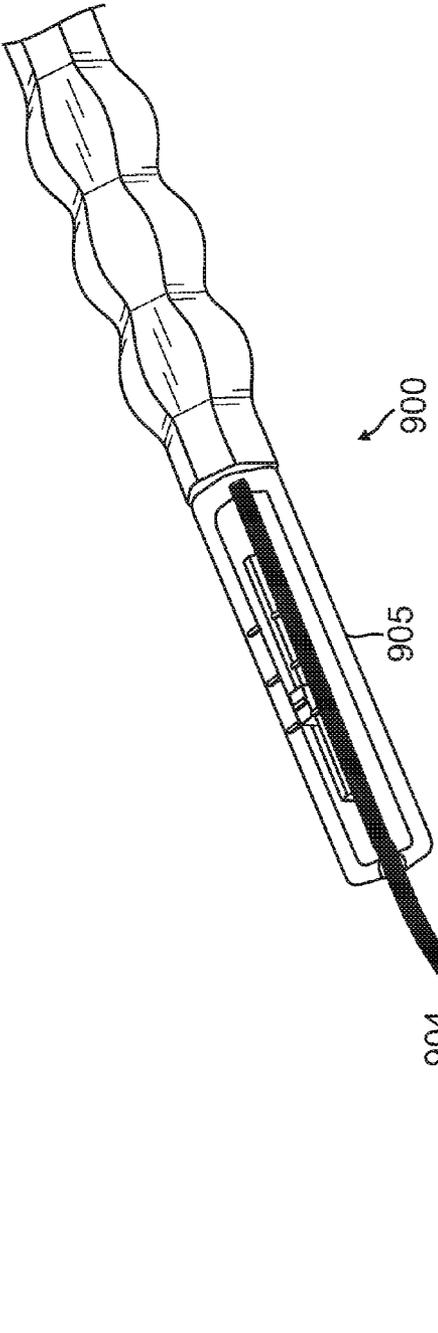


FIG. 19A

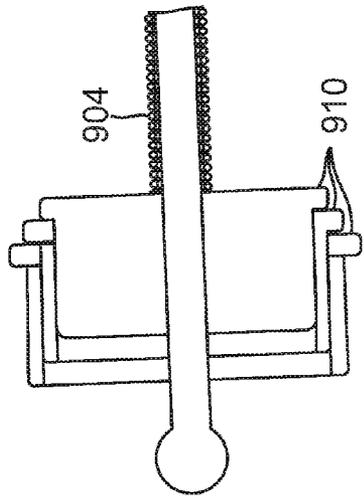


FIG. 19B

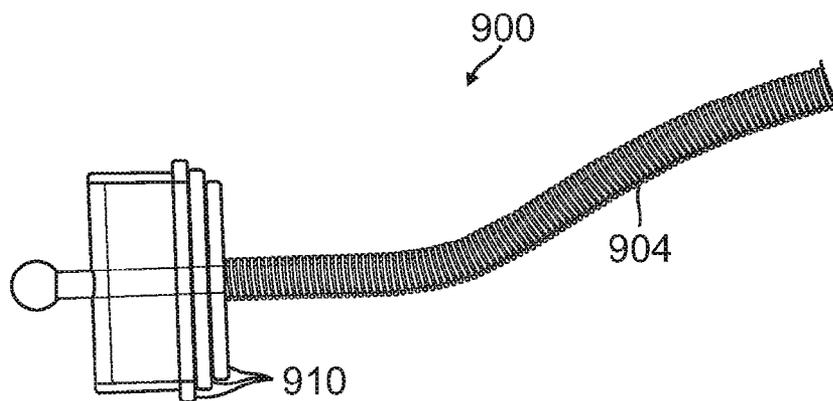


FIG. 19C

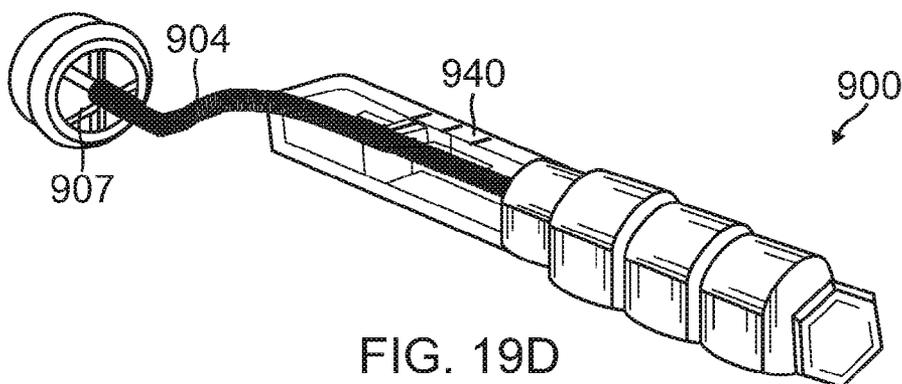


FIG. 19D

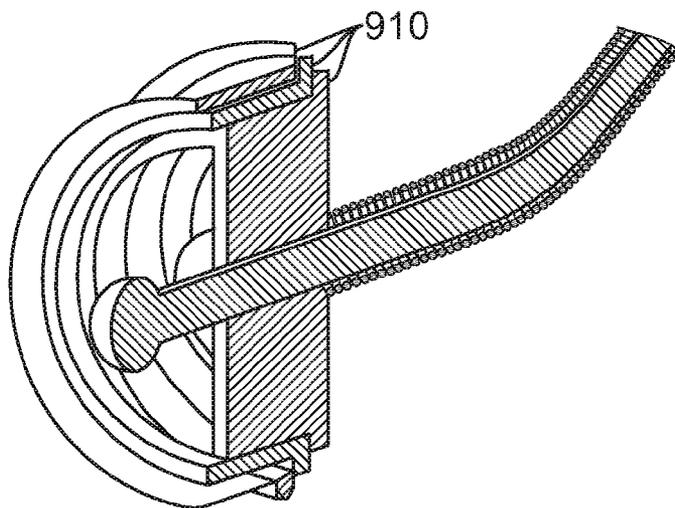


FIG. 19E

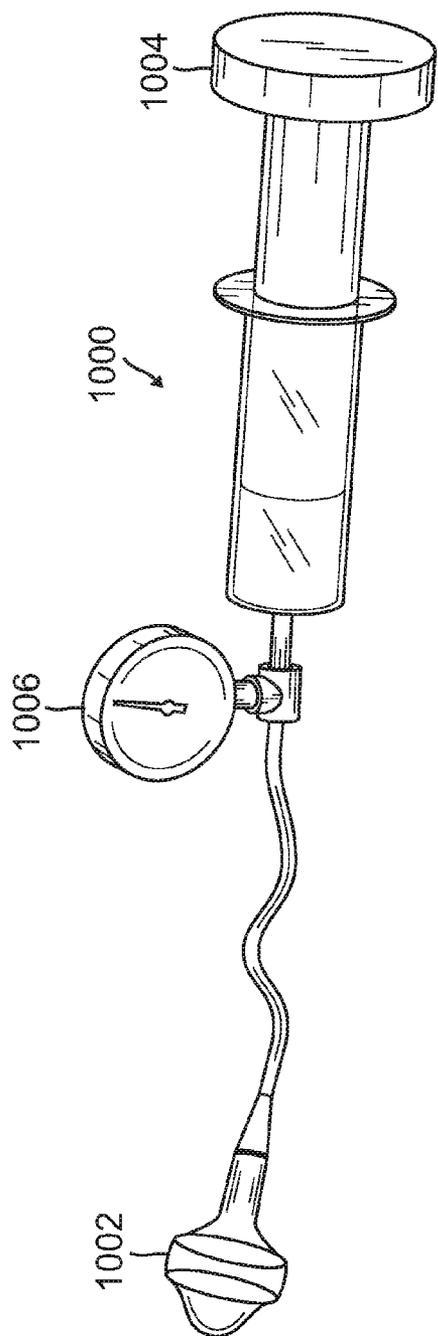


FIG. 20

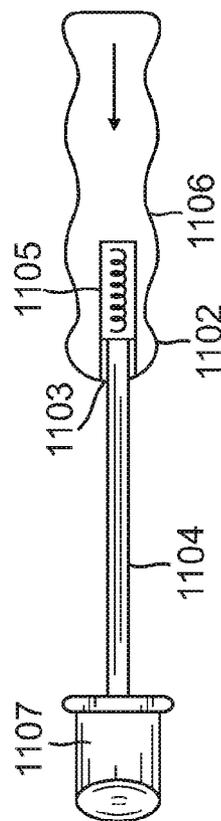


FIG. 21

FIG. 22A

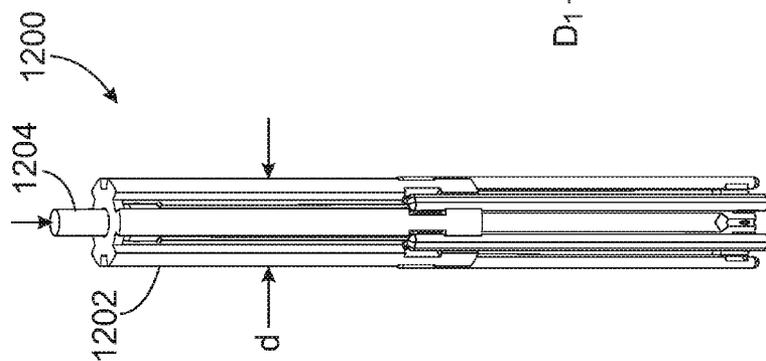


FIG. 22B

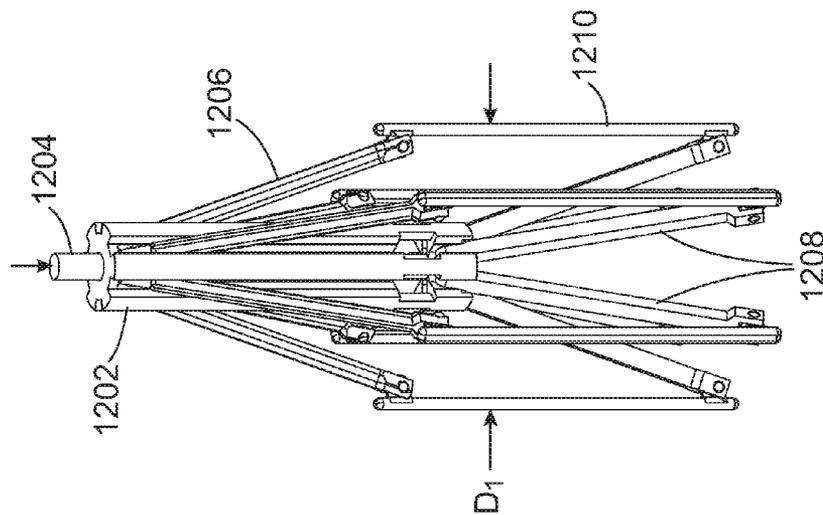
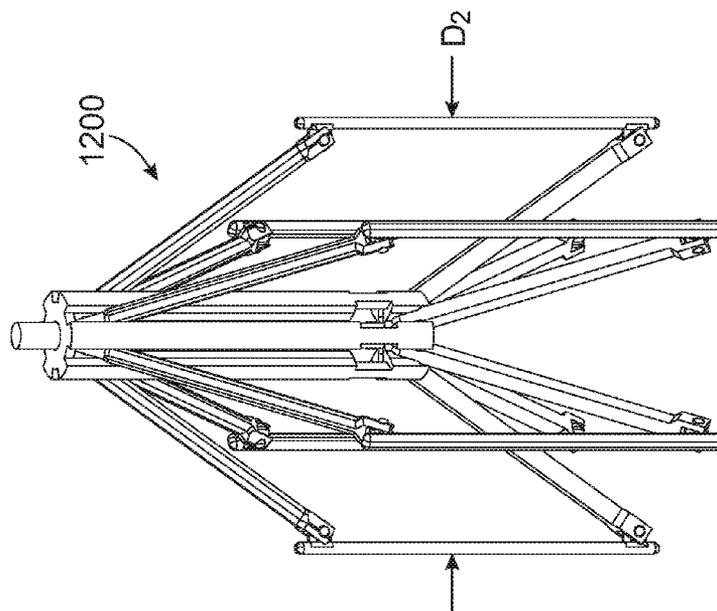


FIG. 22C



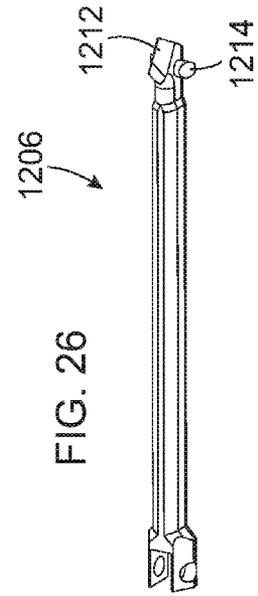
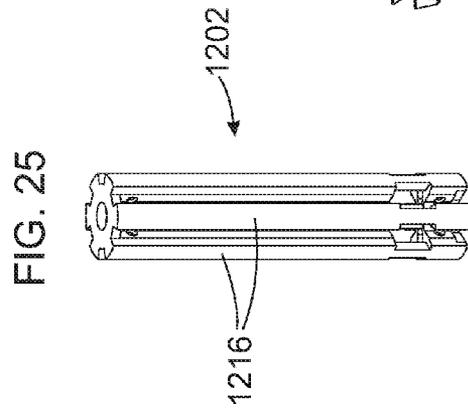
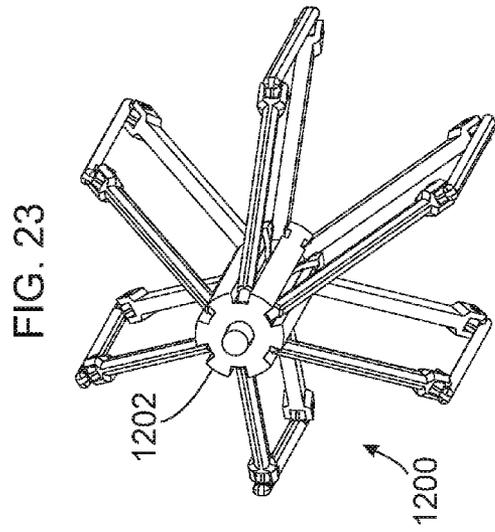
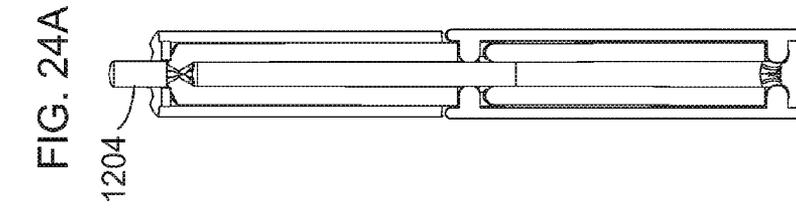
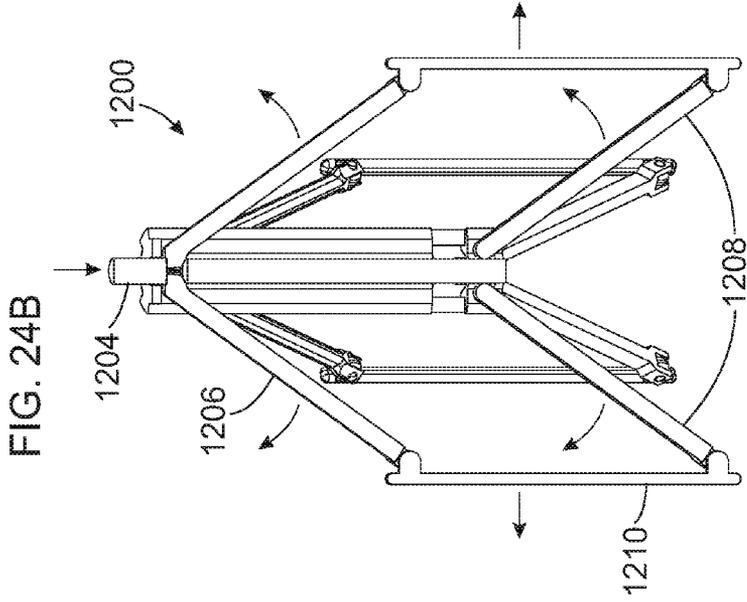


FIG. 27A

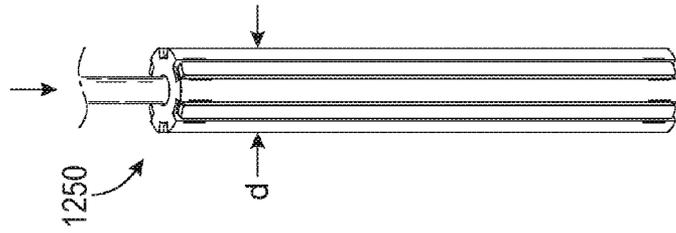


FIG. 27B

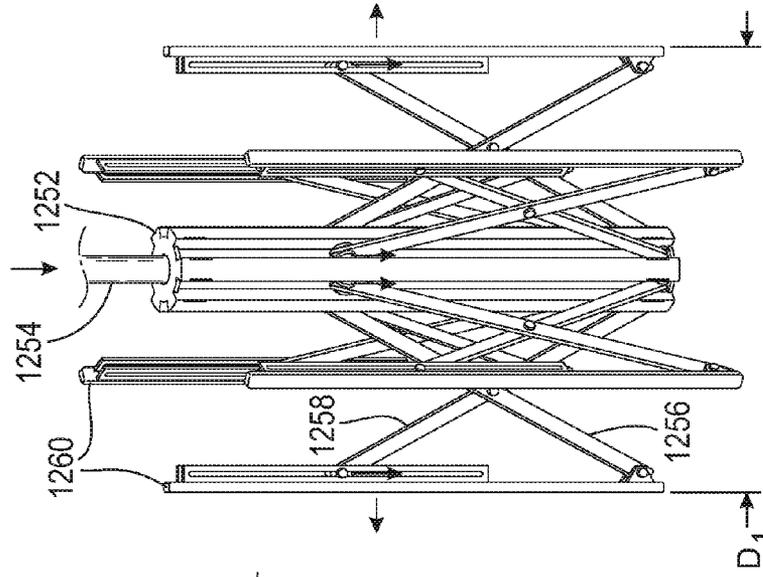


FIG. 27C

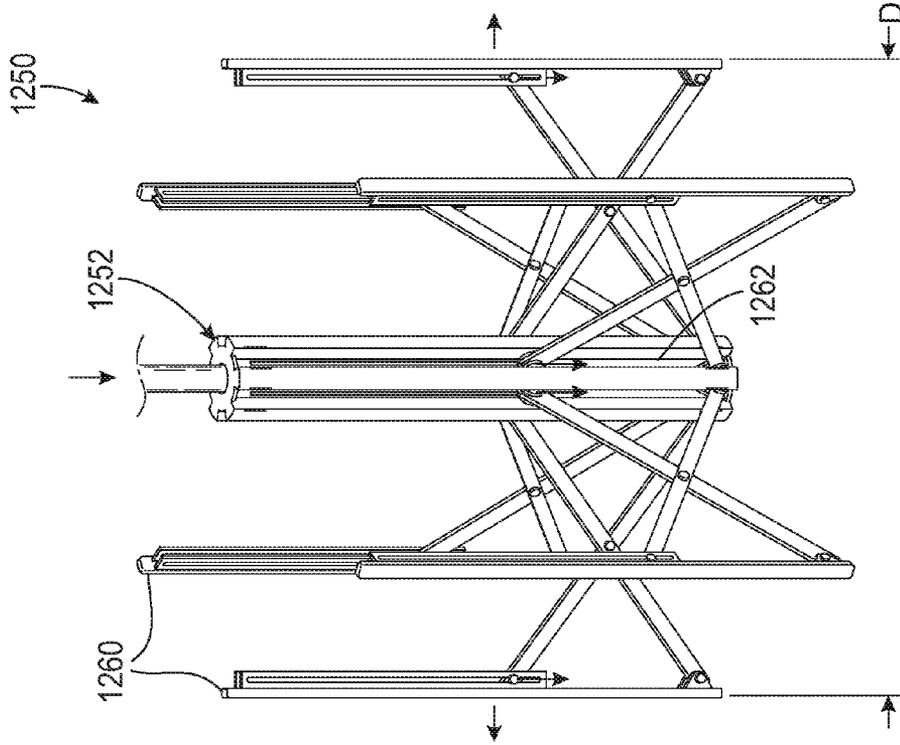


FIG. 27D

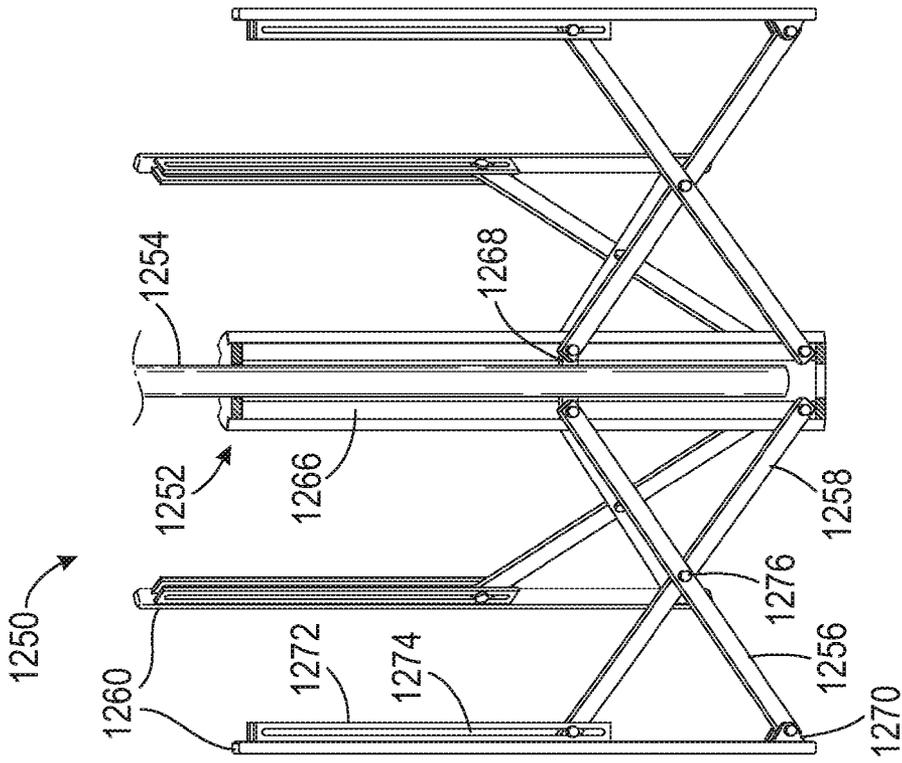


FIG. 28

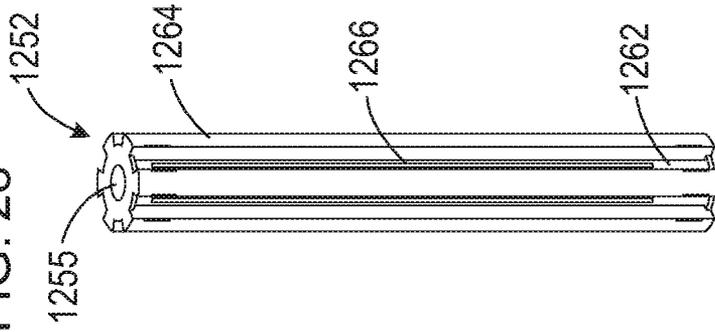


FIG. 29




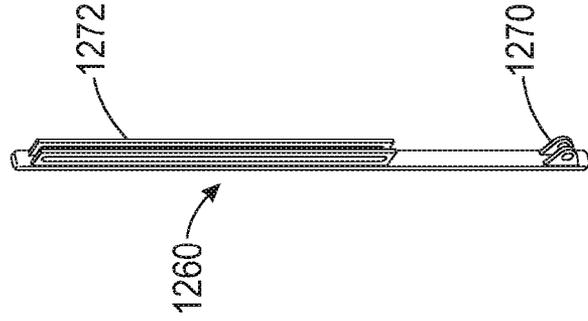


FIG. 30

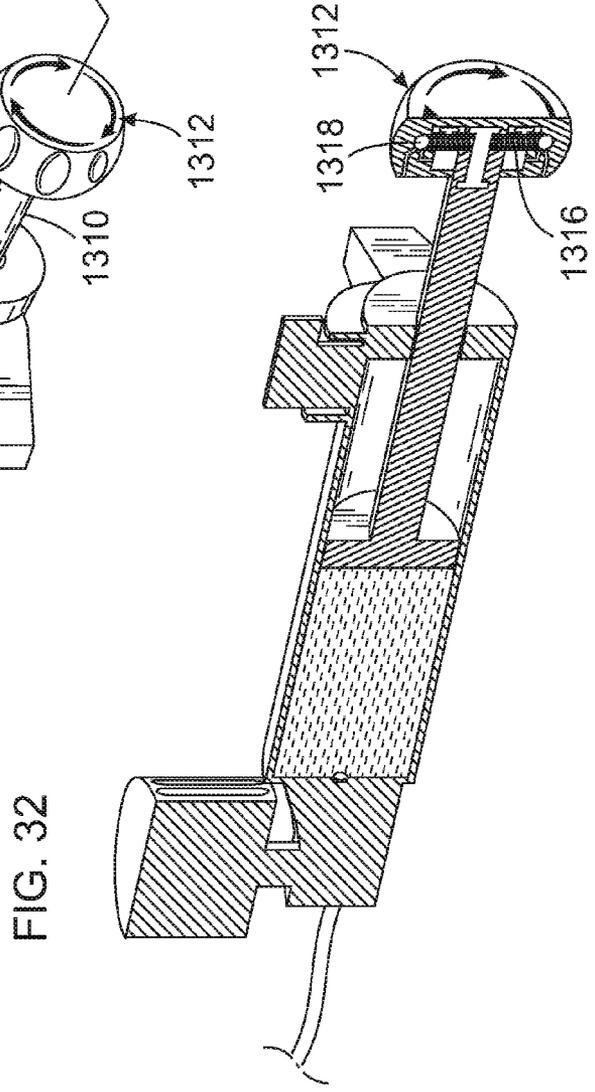

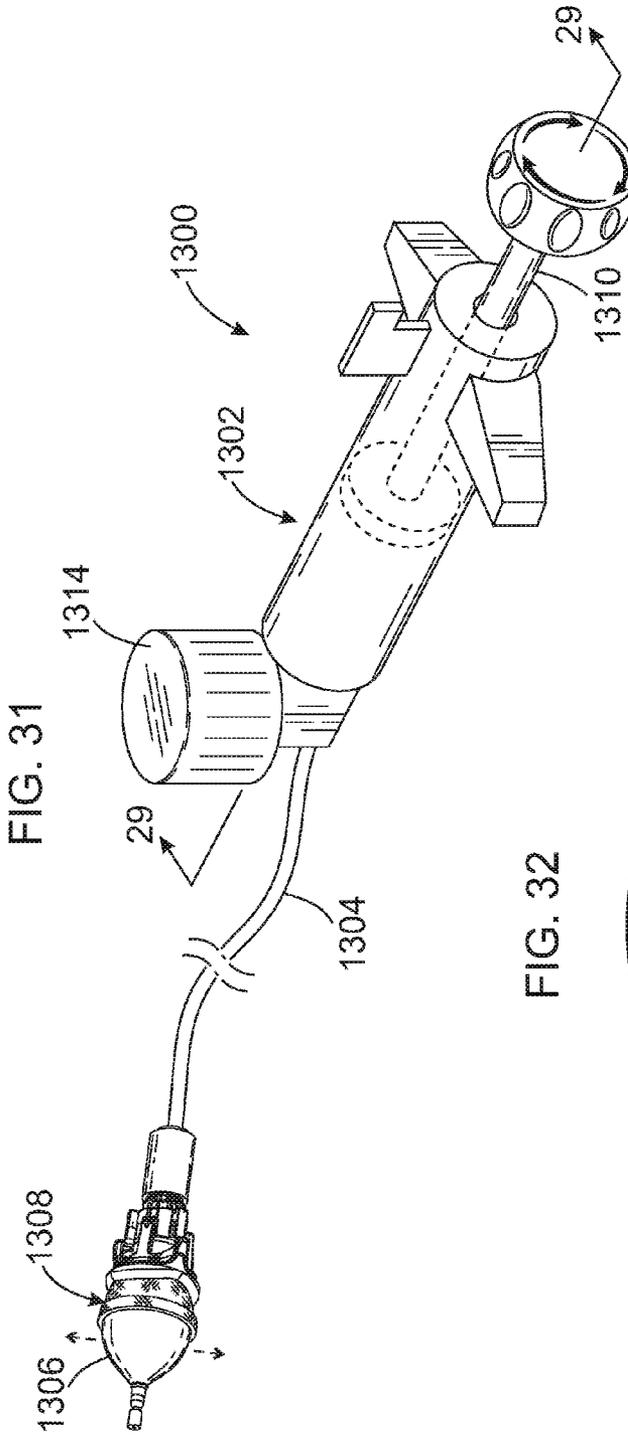

CATHETER-BASED CLUTCHED HEART VALVE SIZER

RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 14/011,602, filed Aug. 27, 2013, now U.S. Pat. No. 9,277,996, which is a continuation-in-part of U.S. patent application Ser. No. 13/707,395, filed Dec. 6, 2012, which claims the benefit of U.S. Application No. 61/568,913, filed Dec. 9, 2011, the disclosures all of which are incorporated by reference.

FIELD

[0002] The present disclosure is directed to methods and apparatus for determining a size of a valve annulus. More particularly, the present disclosure relates to a heart valve sizer.

BACKGROUND

[0003] Replacement of a diseased or malfunctioning cardiac valve requires accurate sizing of the valve annulus. After the diseased or malfunctioning cardiac valve has been removed, the surgeon measures the patient's valve annulus to determine the appropriate replacement valve size.

[0004] A conventional system for measuring a patient's valve annulus includes a number of varying size discs, which can be removably or fixedly attached to a rod. The size of each of the discs corresponds to an available valve size. The surgeon inserts the disc into the patient's valve annulus and checks the fit of the disc within the valve annulus. If the surgeon is not satisfied with the fit, the surgeon removes the disc from the body and inserts a new disc into the valve annulus. The size of a patient's native heart valve annulus is determined by inserting sizers of various diameters until the surgeon determines which one feels correct. This is a time-consuming method since for each valve size the surgeon inserts, the surgeon must remove one of the discs and try another one. This procedure increases the overall surgery time which increases the risk to the patient and also increases the cost of the procedure. Further, the determination of the appropriate size is based on the feeling of the surgeon rather than any mechanical feature. This determination based on the feeling of the surgeon may not be accurate. Thus there is a need for a sizer that is accurate in determining the size of the annulus of a valve.

[0005] Alternatively, a heart valve sizer may be used which is introduced into the patient only once, and the same sizer is capable of gauging a number of appropriate valve sizes. However, these sizers are dimensionally the same as the valves they represent. Due to size constraints, insertion of the heart valve sizers may be a hindrance for certain procedures, especially for minimally invasive surgical incisions such as thoracotomies. With minimally invasive surgical (MIS) type procedures performed through small surgical incisions, the surgeon may not have a good approach angle to the native annulus, thus hindering an accurate tactile feedback to the surgeon when the sizer is in place.

[0006] Additionally, it is essential for the replacement heart valve to be of the right fit. In determining the optimal replacement device for a diseased heart valve, a surgeon generally exerts some level of force to determine a tight fit size. Each surgeon may have a different definition of a tight fit and what is the optimal force that may be exerted. Also, excessive force

if applied may result in inaccurate sizing of the annulus, or even tissue damage. Also, traditional valves involve parachuting the valve down to the annulus with 12 to 14 sutures, and thus sizing is somewhat less sensitive. However, newer valves sometimes employ only three or in some cases no sutures making sizing accuracy more challenging. It is more difficult to avoid paravalvular leaks and risk of embolization if three of no sutures are used and there is a sizing mistake.

[0007] Given the above limitations, it is desirable to have a single, one-size-fits-all sizer which could be used to quickly and accurately determine the appropriate valve size for a patient's heart through a minimal sized incision. It is desirable to have a sizer that does not rely entirely on the surgeon's feel, but on a mechanism that consistently and more accurately determines the patient's annulus size.

SUMMARY

[0008] The embodiments of the present disclosure have several features, no single one of which is solely responsible for their desirable attributes. Without limiting the scope of the present embodiments as expressed by the claims that follow, their more prominent features will now be discussed briefly. After considering this discussion, and particularly after reading the section entitled "Detailed Description", one will understand how the features of the present embodiments provide advantages, which include providing an adjustable force-based heart valve sizer system that can be used to determine the size of patient's heart valve annulus using a single sizer through minimal size incision.

[0009] In one embodiment, an adjustable valve sizer is provided. The valve sizer includes an elongate shaft having a proximal end and a distal end with a movable sizing element coupled to the distal end of the shaft. A valve sizing portion has an outer dimension which is at least partially defined by the movable sizing element. An actuator assembly is provided at the proximal end for moving the movable sizing element so that the valve sizing portion corresponds to the various valve sizes.

[0010] In a preferred device, a heart valve sizer for determining an appropriate replacement prosthetic heart valve size when performing a valve replacement procedure comprises a proximal actuator, a shaft extending distally from the actuator and having a movable member and a stationary member, and a sizing element coupled to the distal end of the shaft. The sizing element has a hub and a plurality of petals each radially movable between a first retracted position and a second expanded position. The hub is fixed to the stationary member in the shaft and the petals are connected to expand radially upon displacement of the movable member in the shaft. A clutch mechanism connected between the actuator and the movable member in the shaft transmits movement forces therebetween, wherein movement of the actuator causes displacement of the movable member and consequently outward radial expansion of the petals in the sizing element into contact with a surrounding heart valve annulus. The clutch mechanism slips at a predetermined reaction force imparted by the heart valve annulus against further outward radial expansion of the petals.

[0011] A preferred method of sizing a patient's cardiac valve annulus disclosed herein comprises the steps of:

[0012] providing a valve sizer having a shaft with a proximal end and a distal end and an expandable sizing element coupled to the distal end of the shaft, the sizing element being radially expandable between a first retracted position and a

second expanded position, the valve sizer further having an actuator assembly comprising an actuator that moves relative to a handle, a clutch ring mounted at the proximal end of the shaft and coupled for rotation to the actuator via a clutch mechanism, and a stationary rod extending through at least a portion of the shaft, wherein the shaft is connected to the clutch ring so that movement of the actuator transmits through the clutch mechanism to the clutch ring and shaft and causes axial movement of the shaft, wherein the axial movement of the shaft causes radial expansion of the sizing element;

[0013] inserting the valve sizer in the first retracted position into the patient so that the movable element is positioned within the valve annulus; and

[0014] rotating the handle until the clutch mechanism of the actuator assembly begins to slip indicating that the sizer has fully engaged the annulus.

[0015] In both the preferred device and method, shaft preferably comprises a rod extending through a hollow shaft and the actuator comprises an actuator ring, where the rod is the stationary member fixed with respect to both the handle and the hub, and the hollow shaft is fixed with respect to a clutch ring that is coupled for rotation to the actuator ring via the clutch mechanism. In this configuration, the clutch ring is connected via a screw thread to the stationary handle so that rotation of the clutch ring causes axial movement of the hollow shaft. The clutch mechanism may comprise a plurality of bearings biased by springs into detents. The plurality of bearings and the springs are desirably held within the clutch ring and the detents are formed on an inner surface of the actuator ring. The bearings and springs may be separate elements held within channels in the clutch mechanism, or may be cantilevered fingers formed in a sidewall of the clutch ring.

[0016] In one version, the plurality of sizer petals move in a plane substantially perpendicular to a longitudinal axis defined by the shaft. The movable member may move axially along the shaft and contact and pivot a lever for each of the petals, wherein pivoting of the levers causes radial expansion of the petals. Or, the movable member may move axially along the shaft and connect to a camming member that directly contacts and causes radial expansion of the petals. The plurality of petals may define a cylindrical annulus portion and an outwardly-extending flange on a proximal end of the cylindrical annulus portion, and the outwardly-extending flange may have an axially undulating peripheral shape.

[0017] In a percutaneous version, the sizer is configured for delivery through a catheter and the petals in their first retracted position limit the diameter of the sizing element to be small enough to enable passage through the catheter, and the petals remain parallel to an axis of the hub while being displaced outward. Desirably, the sizing petals comprise axial bars that retract within recesses within a central hub so as to form a flush cylindrical shape for passing through the catheter. An actuation rod moves within a central bore within the hub and acts on a plurality of struts or levers connected to displace the sizing petals radially outward. In one embodiment, the sizing petals are displaced directly radially outward without axial movement. For example, the levers may be connected to move in a scissor-like fashion with one having a distal end fixed at a pivot point on the central hub so that the proximal end of the levers move axially in concert.

[0018] In another embodiment, a force feedback-based heart valve sizer is provided. A force feedback-based sizer provides a calibrated force indication that allows the surgeon

to apply the optimal (or at least a known) level of force. The force feedback-based sizer provides tactile and visual feedback to the surgeon that a desired force has been reached. The force feedback-based sizer may additionally measure the force applied and display the value. It may further comprise a force limiter, or clutch, that prevents forces above a predetermined level from being transmitted through to the sizer. **[0019]** These and other features will become apparent with the following description of the preferred embodiments.

BRIEF DESCRIPTION OF THE DRAWINGS

[0020] The embodiments of the present disclosure will now be discussed in detail with an emphasis on highlighting the advantageous features. These embodiments depict the novel and non-obvious features shown in the accompanying drawings, which are for illustrative purposes only. These drawings include the following figures, in which like numerals indicate like parts:

[0021] FIGS. 1A-1C show a perspective view of a heart valve sizer with a sizing element having sizing petals in radially expanded positions, according to one embodiment;

[0022] FIG. 1D shows the heart valve sizer with the sizing element, and the sizing petals in radially retracted positions;

[0023] FIGS. 2A-2C show cross sectional views of an actuator assembly for the various sizing elements disclosed herein;

[0024] FIGS. 3A-3B show an alternative clutch ring with valve size markings according to one embodiment for use in the actuator assemblies disclosed herein;

[0025] FIG. 3C shows an exploded view of an actuator assembly including an actuator ring and the clutch ring of FIGS. 3A-3B;

[0026] FIG. 3D shows an exploded view of an actuator assembly similar to that in FIG. 3C and showing an alternative clutch ring with bearings and springs integrated into the clutch ring as cantilevered fingers;

[0027] FIGS. 3E and 3F are perspective and plan views of the alternative clutch ring of FIG. 3D;

[0028] FIGS. 3G-3I are alternative bearing shapes for the integrated springs;

[0029] FIG. 3J is a still further clutch ring where the springs are cantilevered fingers coupled to the clutch ring via an elastomeric interface;

[0030] FIG. 3K shows a clutch ring assembly with a housing that receives a sheet metal ring that forms cantilevered bearings and springs;

[0031] FIGS. 4A and 4B show an alternative actuator assembly exploded and assembled with a sizing element having a hub cover;

[0032] FIG. 5A shows the sizing element with sizing petals in a semi-expanded position, and FIG. 5B is a cross section thereof;

[0033] FIG. 5C shows a petal and a hub assembly from the sizing element of FIG. 5A, while FIG. 5D shows a single petal and a lever that links the petal to the hub;

[0034] FIGS. 6A and 6B are assembled and exploded views of an alternative sizing element of the present application;

[0035] FIGS. 7A and 7B are sectional views through an alternative actuator assembly and sizing element having a conical camming hub;

[0036] FIG. 7C shows a ratchet mechanism for use in the actuator assembly of FIG. 7A;

[0037] FIG. 8A shows the sizing element coupled at the distal end of a shaft with sizing petals in a retracted position;

[0038] FIG. 8B shows a cross-section along lines A-A' of the sizing element of FIG. 8A;

[0039] FIG. 8C shows an individual sizing petal;

[0040] FIG. 9A shows the sizing element with sizing petals in an expanded position;

[0041] FIG. 9B shows a cross-section along lines B-B' of the sizing element of FIG. 9A;

[0042] FIG. 10 shows the disc that cooperates with the hub in the sizers of FIGS. 8A-9B and 13A-14B;

[0043] FIG. 11 shows one embodiment of the hub;

[0044] FIG. 12 shows a cylindrical sizing element with expanded petals covered with an extendable membrane;

[0045] FIGS. 13A-13B show a tapered conical sizing element with petals in retracted and expanded positions, respectively, according to another embodiment;

[0046] FIGS. 14A-14B show a concave shaped sizing element with petals in retracted and expanded positions, according to yet another embodiment;

[0047] FIG. 15 is a schematic view of a feedback-based heart valve sizer that utilizes a torque sensor and display in conjunction with a sizing element to determine the valve orifice size;

[0048] FIG. 16A-16B show a force feedback-based heart valve sizer, according to another embodiment;

[0049] FIG. 17A-17B show a force feedback-based heart valve sizer, according to yet another embodiment;

[0050] FIGS. 18A-18B show a heart valve sizer with a flexible coil;

[0051] FIGS. 19A-19E show a heart valve sizer with stackable valve hubs;

[0052] FIG. 20 shows a heart valve sizer with a pressure gauge.

[0053] FIG. 21 shows a cross-sectional view of a force feedback-based heart valve sizer, according to yet another embodiment;

[0054] FIGS. 22A-22C show a catheter-based sizing element in accordance with the present application in several stages of expansion;

[0055] FIGS. 23 and 24A-24B are further views of the catheter-based sizing element;

[0056] FIGS. 25 and 26 are enlarged views of two components of the catheter-based sizing element;

[0057] FIGS. 27A-27D are perspective and sectional views of an alternative catheter-based sizing element;

[0058] FIGS. 28-30 are enlarged views of components of the alternative catheter-based sizing element; and

[0059] FIGS. 31 and 32 are schematic views of a balloon catheter inflation system that utilizes a clutch-limiter as described herein to limit the maximum inflation pressure.

DETAILED DESCRIPTION

[0060] Referring to FIGS. 1A-1D, a first valve sizer 100 is shown. The valve sizer 100 includes an elongate hollow shaft 104 extending along the length of the sizer. An actuator assembly 106 is coupled to the proximal end of the shaft 104, while a radially expandable sizing element 107 is coupled to the distal end. The shaft 104 is preferably malleable ensuring that it is flexible enough to allow the sizer 100 access to the annulus from different angles, or through curved or bent access passages. The handle 102 is preferably static and is used for keeping the valve sizer steady in the hands of the operator.

[0061] With reference to FIGS. 1C and 2A-2C, the actuator assembly 106 includes an actuator 105, a handle 102, a clutch

ring 121 (also referred to as ring 121), and a clutch cover 126 mounted within the actuator 105. The handle 102 threadingly engages a tubular threaded portion 121B ending axially up from the ring 121 which, in turn, is mounted to the shaft 104. Rotation of the clutch ring 121 relative to the handle 102 causes axial displacement therebetween. The handle 102 is used for positioning the radially expandable sizing element 107 on the end of the shaft 104 within the annulus. As will be seen, rotation of the actuator 105 and clutch ring 121 expands and retracts the radially expandable sizing element 107 so that the valve sizing portion corresponds to various valve sizes, as will be discussed in detail below.

[0062] The radially expandable sizing element 107 defines an outer dimension of the valve sizing portion. The sizing element 107 has a hub 117 with a number of sizing petals 108 that extend radially outward from the hub 117 and are mounted to move radially in and out. FIGS. 1A-1C illustrate the sizing petals 108 in radially expanded positions while FIG. 1D illustrates the sizing petals 108 in radially retracted positions. Rotation of the actuator 105 controls the radial expansion of the sizing petals 108 from the retracted position to the expanded position as will be described below.

[0063] As best seen in FIG. 1A and also in FIG. 1D, the distal end of the handle 102 has a window 130 which shows a number of numerical markings 133 on the ring 121 indicating the size of the valve sizer. The ring 121 has a circular base 121A with markings 133 (see FIGS. 3A and 3B) for indicating the valve size, and the tubular threaded portion 121B extending laterally in the handle. Rotation of the actuator 105 rotates the clutch ring 121 and markings 133 thereon past the window 130 until a predetermined torque limit is reached, at which point a clutch mechanism slips, as will be explained, and further rotation of the actuator 105 is decoupled from the ring 121. The valve size corresponding to the torque limit is displayed in the window 130. In other words, the actuator 105 continues to expand the sizing element 107 outward until it contacts the surrounding annulus, at which point the resistance imparted to the sizing element 107 transmits back through the clutch mechanism, decoupling rotation of the actuator 105 from the clutch ring 121.

[0064] FIGS. 2A-2C show various cross-sectional views of the actuator assembly 106. FIG. 3C shows an exploded view of the actuator 105 and the ring 121. Ring 121 is inserted in the actuator 105 where the tubular threaded section 121B extends from the top recess 128A towards the bottom recess 128B. FIG. 4A shows an exploded view of the actuator assembly 106 mounted on the shaft 104. A clutch cover 126 snap fits on the actuator 105 over the clutch ring 121.

[0065] With reference again to FIGS. 1C and 2A-2C, the actuator assembly 106 comprises the actuator 105 having a top recess 128A and a bottom recess 128B. The handle 102 engages the tubular threaded portion 121B on the clutch ring 121 within the actuator top recess 128A. The clutch ring 121 is fixed with respect to the hollow shaft 104, while the handle 102 mounts to a fixed length cable or rod 120 extending laterally through the shaft 104. The length of the cable or rod 120 extending between the hub 117 and the handle 102 is fixed, and in this sense the rod 120 forms a stationary member between the handle 102 and the hub 117.

[0066] As seen in FIG. 2C, a stepped washer 140 abuts the lower end of the clutch ring 121 towards the bottom recess 128B of the actuator 105 and mounts such as with adhesive to the shaft 104. A clutch cover 126 snap fits over the clutch ring 121, and threads within the actuator 105, and therefore locks

the washer **140** and the ring **121** within the actuator **105** at the bottom recess **128B** of the actuator. The washer **140** is captured between the lower cover **126** and the lower surface of the clutch **121A**, and along with the shaft **104** moves distally and proximally with the actuator mechanism.

[0067] FIG. 2B shows the ratchet mechanism for the ring **121** according to one embodiment. As will be described below, the shaft **104** attaches to a mechanism that expands the sizer **100** and is coupled to the clutch actuator **105** by a ratcheting mechanism. As seen also in FIG. 3A, a cylindrical base **121A** of the ring **121** has springs **124** inserted into or extending across at least one diametric hole **123**. Spring-loaded bearings **122** seat into a series of cutouts or detents **125** formed on an inner surface of the surrounding actuator ring **105**. Rotation of the actuator ring **105** thus rotates the clutch ring **121** until the bearings **122** slip from the detents **125** against the force of the springs **124**.

[0068] The clutch ring **121** and the actuator **105** function as a ratcheting mechanism such that when a predetermined amount of torque is applied, the actuator **105** ratchets and does not drive the shaft **104** any further. Therefore, the size of the annulus is determined by rotating the actuator **105** until the ring **121** begins to ratchet. The actuator **105** is coupled to the ring **121** such that the rotation of the actuator **105** causes the shaft **104** to move. The force needed to overcome the ratchet mechanism is set to correspond to the reaction force being applied to the sizing petals by the annulus being sized. That is, the reaction force imparted by the annulus to the sizer as the sizer expands gradually increases until the sizing petals fully engage the annulus. The reaction force creates a reaction torque in the shaft **104** which will eventually overcome the springs **124** in the ratchet mechanism such that the clutch slips. The markings **133** indicate an outer diameter of the annulus. The torque at which the clutch slips may be calibrated to match a particular reaction force experienced by the sizing element **107**, such as by varying the spring force or number or character of the bearings **122**, springs **124**, and detents **125**.

[0069] Also, although it is preferred to use the rotating actuator **105** to move the sizing petals **108**, any other actuation mechanism may be used including a trigger, sliding lever, or scissors-type actuator **106**. The hollow shaft **104** forms a movable member between the handle **102** and hub **117**, and transmits the force needed to operate the petals **108**. Other movable members are possible, and the movement need not be linear but could also be rotational. Essentially, there is a stationary member (e.g., rod **120**) that holds the hub **117** from moving relative to the handle, **102**, and a movable member (e.g., the shaft **104**) that transmits the driving force from the handle to the hub to operate the petals **108**, and a variety of such mechanisms are within the scope of the present application.

[0070] The ball-spring-detent type of clutch mechanism is preferred in the heart valve sizing context as sensitivity to environmental factors is relatively low. That is, the accuracy of the torque limit is known with a high degree of accuracy and is not affected by temperature, fluids such as blood, etc. Repeatable results in the operating room make such a clutch system preferable to one which relies on frictional forces, as the coefficient of friction of the contact surfaces may change when subjected to a wet environment, temperature fluctuations, or after being sterilized.

[0071] FIG. 3D shows another ball-spring-detent type of clutch mechanism similar to that in FIGS. 2-3 but with an

alternative clutch ring **121'**, while FIGS. 3E and 3F are perspective and plan views of the alternative clutch ring.

[0072] As in the earlier embodiment, the ratchet mechanism for the clutch ring **121'** spring-loaded bearings **122'** seat into a series of cutouts or detents **125** formed on an inner surface of the surrounding actuator ring **105**. Rotation of the actuator ring **105** thus rotates the clutch ring **121'** until the bearings **122'** slip from the detents **125** against the force of the springs. Instead of separate springs and ball bearings, as described above, the clutch ring **121'** has cantilevered springs **124'** formed into the sidewall of the cylindrical base **121A'**. The finger-like springs **124'** are defined by L-shaped slits **124A** cut into the sidewall, first axially and then circumferentially. The bearings **122'** comprise outward dome-shaped bumps or protrusions integral with and located at the terminal end of the finger-like springs **124'**.

[0073] In addition to the dome-shaped bearings **122'** shown in FIGS. 3D-3F, the bearings **122'** can be formed in other shapes. For instance, FIG. 3G shows the bearings **122'** as semi-circular disks, FIG. 3H as prisms, and FIG. 3I as cones. FIG. 3J illustrates a cantilevered spring **124''** configured as a solid cantilevered beam terminating in the bearing **122'** that is coupled to the larger cylindrical base **121A'** via an elastomeric interface. For instance, the beam may be coupled using elastomeric polymer adhesive, or be overmolded or two-shot molded with an elastomer. In other words, the cantilevered spring **124''** is a separate element from the surrounding base **121A'**.

[0074] Still further, FIG. 3K illustrates a plurality of cantilevered springs **124'''** formed from a continuous sheet metal ring **129**, with the bearings **122''** bent outward at the end of each spring. The ring **129** then assembles into mating slots and recesses formed on the underside of an alternative cylindrical base **121A''** to form the clutch ring. The sheet metal ring **129** may be formed from thin-walled tubing, or first formed flat and then rolled. Techniques of fabrication may include stamping, forging and electroplating. The bearings **122''** are shown as rounded bends, but any of the previously mentioned shapes, and others, could be utilized.

[0075] The function of the separate ball bearings and springs has thus been consolidated into the cantilevered springs **124'** and bearings **122'**. This consolidation helps reduce the cost and assembly time of the device. Further, the cantilevered springs **124'** offer low dimensional variation between parts which ensures consistency in the torque-slip force between units. Calibration of the length, shape and material spring rate of the springs **124'** allows the designer to control the torque at which the clutch will slip, as with the ball bearing/spring mechanism. Indeed, there are a number of ways to provide the clutch mechanism, the illustrated embodiments merely being representative.

[0076] Details of the components and function of an exemplary sizing element **107** will now be described. FIG. 4A shows the actuator assembly **106** mounted on the shaft **104**, which terminates in an actuation bearing **109**. FIG. 4B shows the shaft **104** and actuation bearing **109** positioned just proximal to the sizing element **107**. As will be explained, axial displacement of the actuation bearing **109** within the sizing element **107** causes radial movement of the petals **108** via a camming and linkage system shown best in FIGS. 5A-5D.

[0077] As seen in FIGS. 5B and 5C, the hub **117** includes a top portion **117B** and a bottom portion **117A** connected through a shaft stub **119**, which extends through the top portion **117B** to the bottom portion **117A** of the hub. As

shown in FIG. 5B, the fixed length cable or rod 120 extends into and is fastened within the shaft stub 119, and thus the hub 117. In this way, the distance between the handle 102 and hub 117 remains constant. The top portion 117B and the bottom portion 117A include a plurality of features, such as slots 117C in the top portion 117B, splaying outward around a central axis for interacting with the linkages for moving the petals 108.

[0078] The camming assembly further comprises a hub cover 109A that snap fits to the hub 117, and the actuation bearing 109 extends through the hub cover 109A and fits within a bore in the top portion of the hub 117B. As seen in FIGS. 4B and 5B, the actuation bearing 109 has a distal end 109B and a proximal end 109C. The hub cover 109A rests over the proximal end 109C of the actuation bearing 109. The distal end 109B of the actuation bearing 109 is shaped like a disc. Actuation bearing 109 is coaxially placed around and fastened to the hollow shaft 104, and is aligned with the shaft stub 119 of the hub 117. Both the hollow shaft 104 and actuation bearing 109 slide over the rod 120, which again is anchored in the hub 117. Displacement of the hollow shaft 104 thus displaces the actuation bearing 109 relative to the hub 117.

[0079] The camming assembly includes a number of levers 113 for coupling the petals 108 with the hub 117, seen for one petal in FIG. 5D. The number of levers 113 corresponds to the number of petals 108. Proximal ends 113A of the tapered lever 113 extend through the slots 117C of the hub 117. As seen in FIG. 5B, a finger 113C of the lever 113 extends into an annular groove 109D (FIG. 5A) between the distal end 109B and proximal end 109C of the actuation bearing 109. An outer end 113B of each lever 113 is connected, such as via a journal pin, to a bifurcated pair of inwardly-extending arms 111 on the sizing petal 108, as seen in FIG. 5C. FIG. 5D shows the coupling of the lever 113 with the petal 108, where the distal end 113B of the lever 113 couples with the inwardly-extending arms 111. Rotation of the actuator 105 ultimately leads to axial movement of the shaft 104 and actuation bearing 109. Axial movement of the actuation bearing 109 causes movement of the lever 113 by virtue of the camming interaction between the annular groove 109D and the lever finger 113C. The distal end of the 113B pivots outward from distal movement of the actuation bearing 109, thus causing radial expansion and retraction of the petals 108. The converse is true also, wherein proximal retraction of the shaft 104 and actuation bearing 109 constricts the petals 108 radially inward, thus reducing the profile of the sizing element 107 to facilitate removal from the native annulus after a sizing procedure.

[0080] FIGS. 6A and 6B illustrate a modified sizing element 107' much like the previously-described element 107, and as such like parts will be given like numbers with a prime designation. The sizing element 107' has a plurality of petals 108' that constrict about a hub 117' into a first, reduced diameter configuration as seen in FIG. 6A. In contrast to the earlier petals 108, each modified petal 108' has a proximal flange that in aggregate defines an undulating or scalloped peripheral flange 112. More particularly, adjacent petals 108' have either a convex up flange 112A or a concave up flange 112B, as seen best in the exploded view of FIG. 6B. Preferably, there are six (6) petals 108' with three having a convex up flange 112A and three having a concave up flange 112B. The aggregate flange 112 therefore defines an undulating peripheral shape with three peaks and three valleys, mimicking the natural contours of an aortic annulus and the shape of the sewing ring of a

prosthetic heart valve, where the peaks correspond to the commissures and the valleys to the cusps in between. Provision of the scalloped peripheral flange 112 helps the surgeon properly seat the sizer down into the aortic annulus so that the cylindrical body formed by the petals extends fully within and accurately reflects the size of the annulus orifice.

[0081] The petals 108' also have slightly modified inwardly-extending arms 111' which have pointed inner ends for ease of assembly with the distal ends of the levers 113' and into the receiving channels formed in the bottom portion 117A' of the hub 117'. The pointed inner ends also provide maximum overlap between the internal radial channels in the hub 117' and the petals 108', which is especially important at full expansion for larger annuluses (e.g., 29 mm). Additionally, the actuation bearing 109' has axial ribs that mate with axial grooves in the hub cover 109A' to prevent relative rotation therebetween. Aside from the aforementioned modifications, the sizing element 107' functions in the same way as the earlier-described element 107, and thus will not be further described.

[0082] A method of selecting an appropriate valve size is now described with reference to the aforementioned figures. In a minimally invasive procedure, the valve sizer 100 is preferably introduced into the patient between adjacent ribs in the patient without cutting or significantly deflecting the ribs. At least one dimension of the delivery profile of the retracted valve sizer 100 is such that it is no more than 19 mm, and more preferably no more than 17 mm, so that the valve sizer 100 can be easily introduced between adjacent ribs in the patient. The surgeon then positions the sizing petals 108 in the valve annulus and rotates the actuator 105 until the sizing petals 108 contact the valve annulus. The actuator 105 is rotated until the ratchet begins to slip thus indicating that the sizer has fully engaged the annulus and that a predetermined amount of force is being applied. When in the expanded position, the outer surfaces of opposing sizing petals 108 preferably have a maximum outer dimension of at least 29 mm and more preferably at least 33 mm. The surgeon then reads the appropriate valve size using the markings 133 that appear in the window 130 of the actuator. Following the sizing of the annulus, the actuator 105 is then rotated again so that the sizing petals 108 moves into the retracted position (as shown in FIG. 1D) for removing the valve sizer 100 from the patient.

[0083] When in the retracted position, the maximum outer dimension of the valve sizer 100 is preferably no more than 17 mm, more preferably no more than 18 mm, and most preferably no more than 19 mm. The preferred dimensions of the valve sizer 100 in the retracted position permits insertion of the valve sizer 107 between adjacent ribs in a patient when performing a minimally invasive valve procedure. For minimally invasive surgery approaches, the valve sizer could be made to collapse smaller than 17 mm, as described below with respect to FIGS. 22-26.

[0084] In another embodiment shown in FIG. 7-14, a disc that directly cams the sizer petals outward is provided instead of a lever arm assembly. FIGS. 7A and 7B show a proximal handle 202 that is rigidly connected to a distal hub 210 via a fixed-length cable or rod 220. An actuator assembly including an actuator ring 205 causes axial displacement of a hollow shaft 204 surrounding the rod 220, a distal end of the hollow shaft being fixed to a camming disc 212. More particularly, the hollow shaft 204 has a series of inner threads that cooperate with external threads on the rod 220 such that rotation of

the shaft **204** relative to the handle **202** and rod **220** displaces the shaft and attached camming disc **212**. The camming disc **212**, in turn, directly acts on a plurality of sizing petals **208** of a sizing element **207** to convert them from a first, reduced diameter configuration as seen in FIG. **8A** to a second, expanded configuration as seen in FIG. **9A**.

[**0085**] FIG. **7B** shows a ratchet mechanism that interposes a clutch between rotation of the actuator ring **205** and the hollow shaft **204**, according to one embodiment. As mentioned, the shaft **204** is attached to the disc **212** that expands the sizing element **207**. The ratcheting mechanism uses bearings **222** biased outward by springs **224** held in bores in a clutch ring **221**. The clutch ring **221**, in turn, is fixed around the hollow shaft **204**. The bearings **222** seat into detents on the inner surface of the actuator ring **205**, much like the clutch embodiment described above. The force needed to overcome the ratchet mechanism is set to correspond to the force being applied to the petals by the annulus being sized. That is, the reaction force applied by the annulus to the sizer as the sizer expands is transmitted to a reaction torque against rotation of the hollow shaft **204** and clutch ring **221**, and the force needed to overcome the ratchet mechanism is set to the force needed to size the annulus.

[**0086**] FIG. **7C** shows a slight variation on the clutch mechanism, wherein the bearings **222** are biased inward by the springs **224** into detents formed in an outer surface of the hollow shaft **204**. In this version, there is no need for a separate actuator ring **205** as the user manually rotates the clutch ring **221** directly.

[**0087**] Referring to FIGS. **8A-9B**, according to one embodiment, the radially expandable sizing element **207** is shown. The hub **210** includes radial slots (or holes) **214** shown in FIG. **9B** which guide radial in and out movement of the sizing petals **208** between the retracted and expanded positions. The shaft **204** is coupled to the actuator **205** via the clutch mechanism described above so that rotation of the actuator **205** rotates the shaft **204** and the disc **212** with respect to the rod **220**. Rotation of the shaft **204** causes radial movement of the sizing petals **208** in the slots **214** of the hub **210** between the expanded and retracted positions. That is, distal axial displacement of the shaft **204** and affixed disc **212** forces the distal conical surface of the disc directly against the conical proximal faces **208B** of the petals **208**, thus camming them outward. The taper the proximal face **208B** of each sizing petal, its shape and its dimensions conforms to the shape and dimensions of the disc **212**.

[**0088**] In one embodiment, the disc **212** is conical in shape (FIGS. **8B** and **9B**), with the taper of the disc **212** matching the taper of the sizing petals **208**. The disc **212** is shown by itself in FIG. **10** having an internally threaded axial hole **216** that the threaded shaft **204** engages. The disc **212** moves axially up and down with the threaded hollow shaft **204** to which it is mounted. The axial movement of the disk **212** provides a camming action to force the sizing petals to move due to their matching tapers on the disc **212** and the inner surfaces **108B** of the sizing petals.

[**0089**] FIG. **11** shows the hub **210** by itself. The hub **210** has the radial holes **214** that correspond to pins **208A** on the sizing petals **208**, as seen in FIG. **8C**. The central, axial hole **215** is to receive the threaded shaft **204**. Each sizing petal **208** has at least one pin **208A** that slides radially in the matching holes **214** in the hub **210**. Preferably, each sizing petal **208** has at least two pins **208A** that slide in the matching holes **214** of the hub **210** for better alignment. The number of pins **208A** in

each sizing petal **208** corresponds to the number of holes in that sector of the hub **210**. The sizing petals **208** preferably have a curved outer surface **232** that together generally form a cylindrical peripheral shape when in the retracted and expanded positions. Taken together, the outer surfaces **232** of the sizing petals **208** define a valve sizing portion which engages the patient's valve annulus when sizing the replacement valve.

[**0090**] The device disclosed here shows a sizer with 8 sizer petals **208** which form a cylindrical sizer. More or fewer sizer petals could be used in the same way if it were deemed advantageous. Likewise, the shape of the sizer petals could be such that they form a sizer with a non-cylindrical shape.

[**0091**] In one embodiment, as shown in FIG. **12**, the outside of the distal end of the sizer is covered by an extendible membrane **250** made out of a material such as silicone rubber. This would make the outside of the sizer smoother when expanded.

[**0092**] For instance, their shape could form a tapered conical shape. FIGS. **13A-13B** show tapered conical petals **208** forming a tapered sizer. FIGS. **14A** and **14B** show a concave shaped sizer formed by petals **208** having concave outer surfaces. The concave shape of the sizer ensures that the sizer is properly engaged with the annulus. This may be especially beneficial in MIS procedures where visibility of the annulus is limited.

[**0093**] Up to now, clutch-based sizers have been described using a clutch mechanism with a pre-calibrated torque threshold. This is believed to provide excellent accuracy for a majority of patients and sizing procedures, especially using the relatively robust ball-detent clutch mechanism. However, certain sizing tasks may involve a high degree of variability or require a relatively fine force threshold determination which may not be satisfied by a pre-calibrated clutch having a single torque threshold. Consequently, the present application contemplates a number of force feedback-based sizing systems that supply information to the user on the actual force magnitude experienced by the sizing element. Such systems can be used in actual sizing procedures, or for analysis of different orifice characteristics to provide empirical information for use in calibrating the ball-detent clutch-based sizers described above.

[**0094**] For example, FIG. **15** shows a first embodiment of a force feedback-based sizing system **300** having a handle **302**, a shaft **304**, an actuator dial **305**, and a sizing element **307** such as described above. A torque sensor **310** connected to a proximal end of the handle **302** is connected to sense the torque imparted to the actuator dial **305**, for example, which expands the sizing element **307** against the surrounding orifice. The torque sensor **310** connects via a wire **312** to a display/data recording unit **314** to monitor and collect torque readings.

[**0095**] In use, the sizing element **307** is inserted into the annulus, orifice or structure whose diameter is being measured. While holding the torque sensor **310**, the actuator dial **305** is rotated slowly until the next size increment is displayed in the window **316**. The peak torque shown on the display/data recording unit **314** is then noted/recorded along with the diameter of the sizing element **307**. The process is repeated for greater size increments. Ultimately, the torque data is converted to outward radial force or pressure data exerted by the sizing element **307** on the surrounding annulus. This information can be useful in calibrating a ball-detent clutch system as described above, such as by identifying the proper

springs to use for a particular type of tissue or type of patient. More directly, the force feedback based sizer system 300 can be used to size a valve annulus, with the surgeon identifying the appropriate size not based on when the clutch slips but instead when a particular torque is reached. In that case, the clutch system may be set to have a relatively high torque threshold before it slips, though not too high to cause any tissue damage.

[0096] It should be noted that instead of the torque sensor 310 connected to sense the torque applied, a linear force sensor may be coupled to measure the tension in one or the other of the elements described previously for actuating the sizing elements. For example, in the embodiment of FIGS. 1-6 (e.g., FIG. 5B) the hollow shaft 104 is driven distally while the cable or rod 120 is placed in tension between the handle 102 and the hub 117. A force sensor in the handle 102 could be attached to the proximal end of the cable 120 to measure the tension, which can be used to determine the level of the reaction force of the annulus against the petals 108. Sensing the force in the cable 120 would actually be a more direct method than sensing torque, though either method is suitable. For the purpose of definition of terms, both the torque sensor and linear force sensor methods will be termed force-feedback sensors.

[0097] In another embodiment, a force feedback-based sizer 600 is provided. As shown in FIG. 16A, the sizer 600 has a hollow shaft 604 extending along the length of the sizer. A movable sizing element 607 is provided at the distal end of the shaft 604 and an actuation assembly 606 is provided at the proximal end of the shaft 604. The actuation assembly 606 includes an actuator 602 with a handle, and a force gauge disposed in the handle. The force gauge measures the force applied for operating the sizer.

[0098] The force gauge may provide a digital readout 640a of the force applied on a screen 640. In one embodiment, the force gauge may use varying colors (or colored lights) 640b to indicate if the applied pressure varies from a predetermined target range for the sizer. For example, if the force applied is within a predetermined target range the light may indicate green color. If the force applied is below the target range the color may be yellow, or red if the force applied is above the target range.

[0099] In one embodiment, as shown in FIG. 16B, the movable sizing element 607 includes a compliant spacer 610 that is filled with fluid and deforms with force. As force is applied, pressure within the spacer increases and is measured by a pressure gauge integrated into the handle.

[0100] FIGS. 17A and 17B show a heart valve sizer 700 where the electronic (light or digital readout) system of sizer 600 is replaced with a mechanical system. The system 700 features a malleable outer tube 703 with a flexible inner shaft 709 extending along the length of the sizer 700. The outer tube 703 is malleable and can be bent to any desired shape depending on the surgeon's preference and patient anatomy. The malleable outer tube 703 has a valve sizer 707 disposed at the distal end, and an actuation assembly 705 with a handle 702 disposed at its proximal end. A shaft marker (not shown) is attached to the shaft (not shown) that indicates an optimal force range of the force that may be applied to the heart valve sizer 700. A window 740 on the handle 702 of the actuator assembly 706 allows the surgeon to see the position of a marker attached to the shaft. Markings on the handle 702 indicate that the force level is optimal when aligned with the shaft marker (not shown). The spacer 707 is attached to a

flexible inner shaft 709 which is inside the malleable outer tube 703. The flexible shaft 709 can move longitudinally within the outer tube 703 with minimal resistance. When in use, the sizer 700 is introduced between adjacent ribs in the patient. The surgeon then positions the spacer 707 in the valve annulus. The annulus exerts axial forces on the spacer 707. These axial forces from the spacer 707 are transmitted along the flexible inner shaft 705 to the spring system within the handle 702, and markings on the handle provide the feedback to the surgeon.

[0101] In yet another embodiment, as shown in FIGS. 18A and 18B, a sizer 800 is provided where the electronic (light or digital readout) system 600 is replaced with a mechanical system. The system 800 features a flexible outer helical coil 804 and malleable inner shaft 802 extending along the length of the system 800. The malleable inner shaft 802 can be bent to any desired shape depending on surgeon's preference and patient's anatomy. A valve sizer 807 is disposed at the distal end of the helical coil 804, while an actuation assembly 805 is disposed at the proximal end of the helical coil 804. A handle 801 operates the actuation assembly 805. A shaft marker (not shown) is attached to the shaft 802 that indicates an optimal force range of the force that may be applied to the heart valve sizer. A window 840 is provided which allows the user to see the position of a marker attached to the shaft. Markings on the handle 801 indicate that the force level is optimal when aligned with the shaft marker. The sizer 807 can slide over the malleable inner shaft 802 which is inside a flexible outer helical coil 804. The flexible outer helical coil 804 pushed by the spacer 807 can move longitudinally over the malleable inner shaft 802 with minimal resistance. When in use, the sizer 800 is introduced between adjacent ribs in the patient. The surgeon then positions the spacer 807 in the valve annulus. The annulus exerts axial forces on the spacer 807. These axial forces from the spacer 807 are transmitted along the flexible coil 804 to the spring system within the handle 801, and markings on the handle provide the feedback to the surgeon.

[0102] FIGS. 19A-19E show a heart valve sizer 900 with stackable hubs sliding over the same flexible outer helical coil and malleable inner shaft mechanism. The valve sizer 900 has a tube 904 extending along the length of the system. A valve sizer 907 is disposed at its distal end, while an actuation assembly 905 is disposed at the proximal end of the tube 904. The hubs 910 of varying diameters may be used to measure the annulus by stacking a next size hub onto existing smaller hubs. These hubs with incremental diameters mounted against the distal end of the outer spiral coil slide over a malleable inner shaft till an optimal fit is attained. If the sizer hub seems undersized when being pushed through the annulus, a bigger hub head can be moved down the tube 904 and attached to the initial hub either by a snapping connection or a luer-like quick connection. FIGS. 19B-19D show three hubs 910 stacked onto the distal end of the tube 904, while FIG. 19E shows a cross-sectional view of the distal end of the sizer 900 with three hubs 910 stacked on the coil 904.

[0103] FIG. 20 shows an alternate embodiment of a force-based heart valve sizer 1000 with a syringe 1004 and a pressure gauge 1006. The compliant hub 1002 is inflated with fluid pressurized by the syringe 1004. The pressure applied to the hub 1002 to size the valve annulus is measured by the pressure gauge 1006.

[0104] FIG. 21 shows a cross-sectional view of a force-based sizer 1100. The hub 1107 is attached to the distal end of

the shaft **1104**. The handle **1102** of the actuator assembly **1106** has an actuation mechanism comprising at least a spring **1105**. As the hub **1107** moves towards the handle **1102**, the shaft **1104** moves into the handle cavity **1103**. Interfering features on the shaft **1104** and handle cavity **1103** eventually come into contact. As this interference is overcome, a tactile and/or audible ‘click’ is experienced. By adjusting the amount of interference, the device can be calibrated to a target force level. If no spring is present, then the device would provide minimal feedback to the operator until the interfering features came into contact. A spring **1105** that presents less force than the target force level would provide increasing tactile resistance to the operator as force was applied. Once actuated, the shaft **1104** would remain positioned proximally within the handle **1102**. If a spring **1105** that is strong enough to overcome the target force level is used, then the device would return to its expanded length after the operator stops applying force to the device.

[0105] A force feedback-based heart valve sizer enables limiting, controlling and measuring axial forces at the sizer’s distal end being inserted into the heart. The force feedback-based heart valve sizer enables sizing the heart valve annulus in a controlled manner, thereby limiting the maximum force applied and minimizing the risk of tissue damage.

[0106] The force feedback-based valve sizer disclosed here has several advantages over the currently used valve sizers. The first advantage is its adjustability, which allows a single sizer to cover the entire range of valve sizes. The use of a single one-size-fits-all sizer instead of multiple static sizers reduces clutter in the operating field and makes sizing the patient’s annulus quicker, thereby potentially reducing bypass time during the procedure. Another advantage of the device over existing valve sizers is its ability to collapse radially. This feature has the potential to facilitate MIS surgical procedures which are performed through small surgical incisions. A static sizer may be too large to fit through an MIS incision, particularly if the procedure takes advantage of a collapsible MIS surgical valve. A further advantage of this device is the use of force-based sizing. The mechanism used to expand the sizer contains a ratchet mechanism that limits the amount of force the sizer applies to the annulus. The force limit can be set to achieve proper sizing of the annulus while eliminating the potential for over-expanding and damaging the annulus. This may be particularly important in MIS valve replacement procedures where visualization is poor and the surgeon may not be able to use their sense of “feel” to determine the proper annulus size.

[0107] Heart valve sizers, as well as other body cavity sizers, may be reduced in profile (diameter) to be used in minimally-invasive or percutaneous contexts. For instance, currently there is a great deal of ongoing work to develop systems for replacing heart valves percutaneously through a patient’s vasculature without the need to stop the heart and place the patient on cardiopulmonary bypass. Currently, sizing for such procedures is done using fluoroscopy, which aside from exposing the patient and operating room staff to radiation is not as accurate as desirable. Accurate sizing of the heart valve annulus remains an issue, and the present application provides a clutch-based sizer in FIGS. **22-26** that may be used percutaneously.

[0108] FIGS. **22A-22C** show a catheter-based sizing element **1200** in several stages of expansion. The sizing element **1200** includes a central hub **1202** that receives an actuation rod **1204** through a central bore at a proximal end thereof. As

will be shown, the actuation rod **1204** acts on a plurality of proximal levers **1206** that move outward in conjunction with a plurality of distal levers **1208** to radially displace axial sizing petals **1210**. Because the lengths of the proximal and distal levers **1206**, **1208** are the same, the sizing petals **1210** remain parallel to the hub **1202** axis while being displaced outward.

[0109] In a collapsed, delivery configuration, shown in FIG. **22A**, the sizing element **1200** may have an outer diameter d of about 6 mm, sufficiently small to enable passage through an 18Fr percutaneous catheter (not shown) advanced through the femoral artery to one of the heart valve annuluses, as is known. The profile of the sizing element **1200** could be further reduced to pass through even smaller catheters. A partially expanded sizing element **1200** in FIG. **22B** has an outer diameter D_1 of about 19 mm, while a fully expanded sizing element **1200** in FIG. **22C** has an outer diameter D_2 of about 29 mm. As with the various sizers discussed previously, the petals **1210** expand outward into contact with the valve annulus until a reaction force causes the clutched drive (not shown) to slip. As before, the clutch drive preferably has a size indicator (as with size indicators **133** on the clutch ring **121** in FIG. **3A**) that displays the diameter of the sizing element **1200** at all times, such that when the clutch slips the user is aware of the valve annulus size, and thus the proper prosthetic heart valve size needed.

[0110] FIGS. **23** and **24A-24B** are further views of the catheter-based sizing element **1200**, and in particular FIG. **24B** shows the outward movement of the connected levers **1206**, **1208** and sizing petals **1210**. Distal movement of the actuation rod **1204** acts on a plurality of small fingers **1212** on each proximal lever **1206** to cause the levers to pivot outward about pivot pins **1214** journaled in bores in the hub **1202**, as seen in FIGS. **25** and **26**. In this regard, the hub **1202** comprises a generally cylindrical body having a series of radially-projecting axial ribs **1216** between which each movable “segment” of the sizing element **1200** initially resides. Each movable segment includes one each of the levers **1206**, **1208** and sizing petals **1210** connected together at hinges. Both the proximal and distal levers **1206**, **1208** rotate about pins journaled in the sides of adjacent axial ribs **1216**, and are each connected to rotate about opposite ends of a sizing petal **1210**. Although not shown, the actuation rod **1204** desirably continues the length of the hub **1202** so that it can also act on similar fingers formed on the distal levers **1208**, and thus produce an outward force on both levers.

[0111] The actuation rod **1204** could be driven by a clutch-based actuator, such as is shown above with respect to FIGS. **2A-2C** or **7A-7C**. In particular, a ball-spring-detent mechanism that drives a lead screw is preferred as the sensitivity to environmental factors is relatively low.

[0112] If the sizing element **1200** is used in a beating heart procedure when the heart is pressurized, the force limit of the sizer will be set relatively low. The sizing element **1200** will essentially act as a touch probe and begin to slip when all of the petals (**6** in the illustrated embodiment) contact the annulus with a minimum amount of force.

[0113] FIGS. **27A-27C** illustrate an alternative catheter-based sizing element **1250** in several stages of expansion. The sizing element **1250** includes a central hub **1252** that receives an actuation rod **1254** through a central bore **1255** (see FIG. **28**) at a proximal end thereof. In this description, proximal is synonymous with the upper end of the sizing element **1250** in the figures, while distal is synonymous with the lower end. As

will be shown, the actuation rod **1254** acts on a plurality of first levers **1256** that move outward in conjunction with a plurality of second levers **1258** in a scissor-like fashion to radially displace axial sizing petals **1260**. Because the lengths of the first and second levers **1256**, **1258** are the same, the sizing petals **1260** remain parallel to the hub **1252** axis while being displaced outward.

[0114] With reference to the sectional view of FIG. 27D as well as the detailed views of the components in FIGS. 28-30, the central hub **1252** comprises a generally cylindrical member having the central bore **1255** that receives the actuation rod **1254**, and further includes a plurality of axial recesses **1262** between axial ribs **1264** on its outer surface that receive and accommodate the folded up levers **1256**, **1258** as well as the sizing petals **1260**. As seen in FIG. 27A, the collapsed configuration of the sizing element **1250** substantially forms a cylinder, with the outer surfaces of the sizing petals **1260** lying essentially flush with the ribs **1264**. As seen in FIGS. 27D and 28, the central hub **1252** also has a plurality of axial slots **1266** extending between the recesses **1262** and the central bore **1255**, which will be explained below.

[0115] Still with reference to FIG. 27D, a proximal end of each of the first levers **1256** connects via a pivot pin between a pair of movement tabs **1268** projecting outward through the vertical slots **1266** from the actuation rod **1254**. A distal end of each of the first levers **1256** connects via a pivot pin between a pair of flanges **1270** extending inward at the distal end of the corresponding sizing petal **1260**. Conversely, a distal end of each of the second levers **1258** connects via a pivot pin to a fixed point at a distal end of the central hub **1252**, while a proximal end of each of the second levers connects via a pivot between a pair of elongated flanges **1272** extending inward along a proximal section of the corresponding sizing petal **1260**. The elongated flanges **1272** include axial guide slots **1274** which receive the pivot pin at the proximal end of each of the second levers **1258**, thus permitting axial movement therebetween. Finally, each pair of first and second levers **1256**, **1258** are connected where they cross each other at their midpoints by a fulcrum pin **1276**. It will thus be understood that distal displacement of the actuation rod **1254** causes distal displacement of the proximal end of the first levers **1256**, each in turn causing corresponding distal displacement of the proximal end of the second levers **1258** through the scissor-like cooperation therebetween. Because the first and second levers **1256**, **1258** are of equal length, and since the distal ends of the second levers **1258** are axially fixed with respect to the central hub **1252**, the distal ends of both levers remain at a fixed axial location with respect to the central hub while the proximal ends move together. This ensures that the sizing petals **1260** remain oriented axially, and also move only radially outward, not axially.

[0116] In a collapsed, delivery configuration, shown in FIG. 27A, the sizing element **1250** may have an outer diameter d of about 6 mm, sufficiently small to enable passage through an 18Fr percutaneous catheter (not shown) advanced through the femoral artery to one of the heart valve annulus, as is known. The profile of the sizing element **1250** could be further reduced to pass through even smaller catheters. A partially expanded sizing element **1250** in FIG. 27B has an outer diameter D_1 of about 19 mm, while a fully expanded sizing element **1250** in FIG. 27C has an outer diameter D_2 of about 29 mm. As with the various sizers discussed previously, the petals **1260** expand outward into contact with the valve annulus until a reaction force caused the clutched drive (not

shown) to slip. As before, the clutch drive preferably has a size indicator (as with size indicators **133** on the clutch ring **121** in FIG. 3A) that displays the diameter of the sizing element **1250** at all times, such that when the clutch slips the user is aware of the valve annulus size, and thus the proper prosthetic heart valve size needed.

[0117] FIGS. 31 and 32 are schematic views of a balloon catheter inflation system **1300** that utilizes a clutch-limiter as described herein to limit the maximum inflation pressure. Inflation systems **1300** such as the illustrated embodiment are used for a variety of purposes, such as angioplasties, valvuloplasties, and for expanding arterial stents and more recently heart valves. The system **1300** includes a piston/cylinder chamber **1302** having a fluid outlet line **1304** that ultimately supplies pressurized saline or other inert fluid to a distal balloon **1306**. In the illustrated embodiment, the balloon **1306** is being used to expand an anchoring frame of a hybrid-type of prosthetic heart valve which has a non-expandable valve portion as well; however the applications of the balloon inflation system **1300** should not be considered limited.

[0118] The actuator of the system **1300** includes a piston shaft **1310** that may be threaded within a bore in the piston/cylinder chamber **1302** so as to advance axially upon rotation of a clutch-limited actuator **1312**. As the piston shaft **1310** advances, fluid is forced through the line **1304** to inflate the balloon **1306**. A gauge **1314** displays the pressure within the fluid, and thus the pressure within the balloon **1306**.

[0119] As seen in FIG. 32, the actuator **1312** preferably includes a series of springs **1316** that bias bearing **1318** outward into detents (not shown) formed on an inner surface of the handle of the actuator **1312**. As with the embodiment of FIGS. 2A-2C, the springs **1316** and bearings **1318** are retained within an inner clutch member that is rigid with the shaft **1310**. The actuator **1312** may be turned until the reaction torque from displacing the shaft **1310** exceeds a threshold value, at which point the bearings **1318** are forced inward against the springs **1316** and the clutch slips. Also, the alternative clutch ring shown in FIGS. 3A-3B may also be used.

[0120] The system **1300** is a relatively simple, inexpensive solution to percutaneous inflation of heart valves and other devices. The clutch mechanism limits the maximum inflation pressure, which can be calibrated to induce a predetermined amount of device expansion. The system **1300** can be retrofitted to existing inflation devices, and acts as a safety feature to prevent over-inflation and possibly rupture of the balloon. There is a linear, predictable relationship between the amount of torque applied by the actuator **1312** and the fluid pressure generated by the advancing piston shaft **1310**, and the relatively robust and precise action of the ball-spring-detent clutch makes limiting the pressure in the operating room environment highly repeatable and accurate.

[0121] The above description merely describes the preferred embodiments and it is understood that variations of the preferred embodiment are within the scope of the invention which is defined by the claims. For example, although it is preferred to use the valve sizers when performing a minimally invasive valve replacement procedure, the valve sizer may also be used in a conventional open-chest procedure.

We claim:

1. A percutaneously delivered heart valve sizer for determining an appropriate replacement prosthetic heart valve size when performing a valve replacement procedure, the replacement prosthetic heart valves having a range of specific sizes, comprising:

- a proximal handle having an actuator mounted for movement thereon;
 - a shaft extending distally from the actuator and housing an actuation rod axially displaceable by the actuator;
 - a sizing element coupled to a distal end of the shaft, the sizing element having a central hub with a central bore along a central axis that receives the actuation rod and a plurality of petals each radially movable between a radially retracted first position and a radially expanded second position, the petals being connected to transition between the first and second positions upon displacement of the actuation rod in the shaft, wherein the petals remain parallel to the axis of the hub while being displaced between the first and second positions;
 - a catheter configured for percutaneous delivery that receives the sizer with the petals in their first position and through which the sizer may be advanced to a heart valve annulus and expelled for sizing a surrounding heart valve annulus; and
 - a clutch mechanism connected between the actuator and the actuation rod in the shaft so as to transmit movement forces therebetween, wherein movement of the actuator causes displacement of the actuation rod and consequently outward radial expansion of the petals in the sizing element from their first to their second positions and into contact with the heart valve annulus, wherein the clutch mechanism slips at a predetermined reaction force imparted by the heart valve annulus against further outward radial expansion of the petals.
2. The valve sizer of claim 1, wherein the actuation rod acts on a plurality of first levers pivotally connected to the central hub that move outward in conjunction with a plurality of second levers pivotally connected to the central hub to radially displace the petals, and the lengths of the first and second levers are the same.
3. The valve sizer of claim 2, wherein the central hub comprises a generally cylindrical body having a series of radially-projecting axial ribs, and the first and second levers rotate about pins journaled in the sides of adjacent axial ribs.
4. The valve sizer of claim 2, wherein the actuation rod acts on small fingers on both the first and second levers so as to produce an outward force on both levers.
5. The valve sizer of claim 2, wherein the first and second levers are connected together and move outward in a scissor-like fashion.
6. The valve sizer of claim 5, wherein the actuation rod has a plurality of movement tabs projecting outward through axial slots in the central hub to which a proximal end of each of the first levers connects via a pivot pin, and a distal end of each of the first levers connects via a pivot pin to a distal end of a sizing petal, and wherein a distal end of each of the second levers connects via a pivot pin to a fixed point at a distal end of the central hub, while a proximal end of each of the second levers connects via a pivot to a proximal section of the corresponding sizing petal, and wherein each pair of first and second levers are connected where they cross each other at their midpoints by a fulcrum pin.
7. The valve sizer of claim 2, wherein the central hub comprises a generally cylindrical member having a plurality of axial recesses between axial ribs on its outer surface that receive and accommodate the first and second levers as well as the petals in their radially retracted first positions so as to form a cylinder, with the outer surfaces of the petals lying flush with the ribs.

8. The valve sizer of claim 1, wherein the actuator comprises an actuator ring mounted for rotation on the handle, and the actuation rod is fixed with respect to a clutch ring that is coupled for rotation to the actuator ring via the clutch mechanism, and wherein the clutch ring is connected via a screw thread to the handle so that rotation of the clutch ring causes axial movement of the actuation rod.

9. The valve sizer of claim 8, wherein the clutch ring is coupled for rotation to the actuator via a plurality of bearings biased by springs into detents.

10. The valve sizer of claim 1, wherein the actuator comprises an actuator ring mounted for rotation on the handle, and the actuation rod is fixed with respect to a clutch ring that is coupled for rotation to the actuator ring via the clutch mechanism, and wherein the handle also includes a window at one circumferential location and the clutch ring has a number of numerical markings thereon indicating different sizes of replacement prosthetic heart valves, the numerical markings being sized and aligned to show one at a time through the window on the handle upon rotation of the clutch ring relative to the handle such that a desired valve size shows through the window when the clutch mechanism slips.

11. The surgical sizer of claim 1, wherein the sizing element has a diameter of less than about 6 mm when the petals are in their radially retracted first positions, and the sizing element has a diameter of about 29 mm when the petals are in their radially expanded second positions.

12. A percutaneously delivered heart valve sizer for determining an appropriate replacement prosthetic heart valve size when performing a valve replacement procedure, the replacement prosthetic heart valves having a range of specific sizes, comprising:

- a proximal handle having an actuator mounted for movement thereon;
- a shaft extending distally from the actuator and housing an actuation rod axially displaceable by the actuator;
- a sizing element coupled to a distal end of the shaft, the sizing element having a plurality of petals each radially movable between a radially retracted first position and a radially expanded second position upon displacement of the actuation rod in the shaft, wherein the sizing element has a diameter of less than about 6 mm when the petals are in their radially retracted first positions;
- a catheter configured for percutaneous delivery that receives the sizer with the petals in their first position and through which the sizer may be advanced to a heart valve annulus and expelled for sizing a surrounding heart valve annulus; and
- a clutch mechanism connected between the actuator and the actuation rod in the shaft so as to transmit movement forces therebetween, wherein movement of the actuator causes displacement of the actuation rod and consequently outward radial expansion of the petals in the sizing element from their first to their second positions and into contact with the heart valve annulus, wherein the clutch mechanism slips at a predetermined reaction force imparted by the heart valve annulus against further outward radial expansion of the petals.

13. The valve sizer of claim 11, wherein the sizing element has a central hub with a central bore along a central axis that receives the actuation rod, and the actuation rod acts on a plurality of first levers pivotally connected to the central hub that move outward in conjunction with a plurality of second

levers pivotally connected to the central hub to radially displace the petals, and the lengths of the first and second levers are the same.

14. The valve sizer of claim **12**, wherein the central hub comprises a generally cylindrical body having a series of radially-projecting axial ribs, and the first and second levers rotate about pins journaled in the sides of adjacent axial ribs.

15. The valve sizer of claim **12**, wherein the actuation rod acts on small fingers on both the first and second levers so as to produce an outward force on both levers.

16. The valve sizer of claim **12**, wherein the first and second levers are connected together and move outward in a scissor-like fashion.

17. The valve sizer of claim **15**, wherein the actuation rod has a plurality of movement tabs projecting outward through axial slots in the central hub to which a proximal end of each of the first levers connects via a pivot pin, and a distal end of each of the first levers connects via a pivot pin to a distal end of a sizing petal, and wherein a distal end of each of the second levers connects via a pivot pin to a fixed point at a distal end of the central hub, while a proximal end of each of the second levers connects via a pivot to a proximal section of the corresponding sizing petal, and wherein each pair of first and second levers are connected where they cross each other at their midpoints by a fulcrum pin.

18. The valve sizer of claim **12**, wherein the central hub comprises a generally cylindrical member having a plurality of axial recesses between axial ribs on its outer surface that receive and accommodate the first and second levers as well

as the petals in their radially retracted first positions so as to form a cylinder, with the outer surfaces of the petals lying flush with the ribs.

19. The valve sizer of claim **11**, wherein the actuator comprises an actuator ring mounted for rotation on the handle, and the actuation rod is fixed with respect to a clutch ring that is coupled for rotation to the actuator ring via the clutch mechanism, and wherein the clutch ring is connected via a screw thread to the handle so that rotation of the clutch ring causes axial movement of the actuation rod.

20. The valve sizer of claim **18**, wherein the clutch ring is coupled for rotation to the actuator via a plurality of bearings biased by springs into detents.

21. The valve sizer of claim **11**, wherein the actuator comprises an actuator ring mounted for rotation on the handle, and the actuation rod is fixed with respect to a clutch ring that is coupled for rotation to the actuator ring via the clutch mechanism, and wherein the handle also includes a window at one circumferential location and the clutch ring has a number of numerical markings thereon indicating different sizes of replacement prosthetic heart valves, the numerical markings being sized and aligned to show one at a time through the window on the handle upon rotation of the clutch ring relative to the handle such that a desired valve size shows through the window when the clutch mechanism slips.

22. The surgical sizer of claim **11**, wherein the sizing element has a diameter of about 29 mm when the petals are in their radially expanded second positions.

* * * * *