

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
16 March 2006 (16.03.2006)

PCT

(10) International Publication Number
WO 2006/028575 A2

(51) International Patent Classification:

G06F 19/00 (2006.01) **A61N 1/365** (2006.01)
A61B 5/08 (2006.01)

(21) International Application Number:

PCT/US2005/025235

(22) International Filing Date: 15 July 2005 (15.07.2005)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:

10/897,856 23 July 2004 (23.07.2004) US

(71) Applicant (for all designated States except US): **CARDIAC PACEMAKERS, INC.** [US/US]; 4100 Hamline Avenue North, St. Paul, MN 55112-5798 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **BROCKWAY, Marina** [US/US]; 4339 Nancy Place, Shoreview, MN 55126 (US). **HOPPER, Donald** [US/US]; 11761 99th Avenue North, Maple Grove, MN 55369 (US). **CARLSON,**

Gerrard, M. [US/US]; 11653 Nevada Lane, Champlin, MN 55316 (US). **KADHIRESAN, Veerichetty** [IN/US]; 1668 Hunter Tr., Centerville, MN 55038 (US). **BECK, Kenneth** [US/US]; 1908 Bluestem Lane, Shoreview, MN 55126 (US).


(74) Agents: **STEFFEY, Charles, E.** et al.; Schwegman, Lundberg, Woessner & Kluth, P.A., P.O. Box 2938, Minneapolis, MN 55402 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,

[Continued on next page]

(54) Title: METHOD AND APPARATUS FOR DETECTING CARDIOPULMONARY COMORBIDITIES

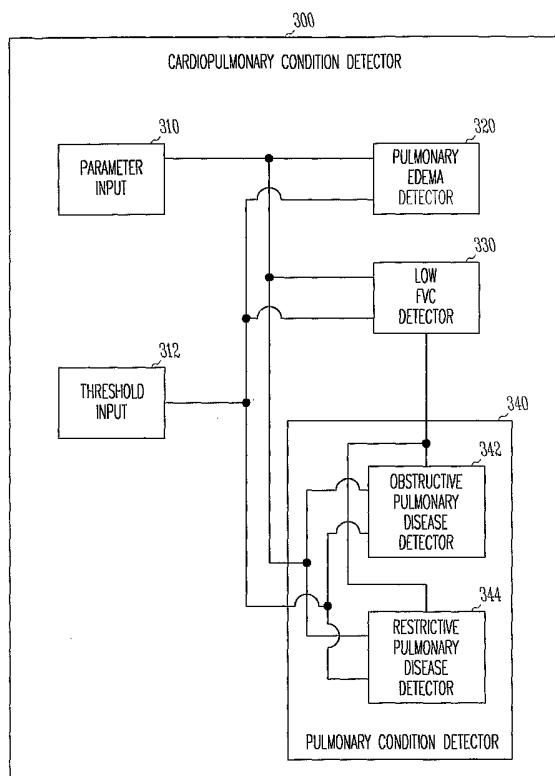

(57) Abstract: A system receives signals indicative of cardiopulmonary conditions sensed by a plurality of sensors and provides for monitoring and automated differential diagnosis of the cardiopulmonary conditions based on the signals. Cardiogenic pulmonary edema is detected based on one or more signals sensed by implantable sensors. If the cardiogenic pulmonary edema is not detected, obstructive pulmonary disease and restrictive pulmonary disease are each detected based on a forced vital capacity (FVC) parameter and a forced expiratory volume (FEV) parameter measured from a respiratory signal sensed by an implantable or non-implantable sensor. In one embodiment, an implantable medical device senses signals indicative of the cardiopulmonary conditions, and an external system detects the cardiopulmonary conditions based on these signals by executing an automatic detection algorithm.



ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

- *without international search report and to be republished upon receipt of that report*

METHOD AND APPARATUS FOR DETECTING CARDIOPULMONARY COMORBIDITIES

Claim of Priority

5 Benefit of priority is hereby claimed to U.S. Patent Application Serial
Number 10/897,856, filed on July 23, 2004, which application is herein
incorporated by reference.

Cross-Reference to Related Applications

10 This application is related to co-pending, commonly assigned, U.S.
Patent Application Serial No. 10/612,387, "IMPLANTABLE DEVICES AND
METHODS USING FREQUENCY-DOMAIN ANALYSIS OF THORACIC
SIGNAL," filed July 2, 2003, U.S. Patent Application Serial No. 10/703,175,
"DUAL-USE SENSOR FOR RATE RESPONSIVE PACING AND HEART
15 SOUND MONITORING," filed November 6, 2003, U.S. Patent Application
Serial No. 10/746,853, "METHOD AND APPARATUS FOR THIRD HEART
SOUND DETECTION," filed on December 24, 2003, and U.S. Patent
Application Serial No. 10/746,874, "A THIRD HEART SOUND ACTIVITY
INDEX FOR HEART FAILURE MONITORING," filed on December 24, 2003,
20 which are hereby incorporated by reference in their entirety.

Field of the Invention

 This document generally relates to patient monitoring systems and
particularly, but not by way of limitation, to such systems monitoring treatment
25 of heart failure patients with cardiopulmonary comorbidities.

Background

 The heart is the center of a person's circulatory system. It includes an
electro-mechanical system performing two major pumping functions. The left
30 portions of the heart draw oxygenated blood from the lungs and pump it to the
organs of the body to provide the organs with their metabolic needs for oxygen.
The right portions of the heart draw deoxygenated blood from the organs and
pump it into the lungs where the blood gets oxygenated. In a normal heart, the
sinoatrial node, the heart's natural pacemaker, generates electrical impulses,

known as action potentials, that propagate through an electrical conduction system to various regions of the heart to excite myocardial tissues in these regions. Coordinated delays in the propagations of the electrical impulses in a normal electrical conduction system cause the various regions of the heart to contract in synchrony such that the pumping functions are performed efficiently.

A blocked or otherwise damaged electrical conduction system causes irregular contractions of the myocardium, a condition generally known as arrhythmia. Arrhythmia reduces the heart's pumping efficiency and hence, diminishes the blood flow to the body. A weakened myocardium has decreased contractility, also resulting in diminished blood flow. A heart failure patient usually suffers from both a damaged electrical conduction system and a weakened myocardium. The diminished blood flow results in insufficient blood supply to various body organs, preventing these organs to function properly and causing various symptoms. For example, in a patient suffering decompensated heart failure, an insufficient blood supply to the kidneys results in abnormal fluid retention and increased central vascular pressure, and hence, cardiogenic pulmonary edema as well as edema in other organs.

Cardiogenic pulmonary edema shares common symptoms with pulmonary diseases such as obstructive pulmonary diseases including asthma and chronic obstructive pulmonary disease (COPD). Such common symptoms include difficulty of breathing, wheezing, and shortness of breathing. Safe and effective treatment for heart failure patients with cardiopulmonary comorbidities depends on differentiation of cardiogenic pulmonary edema from pulmonary diseases such as asthma and COPD. For example, beta-blockers (or beta-adrenergic blockers, pharmaceutical agents) are used to treat heart failure by reducing myocardial oxygen demand, resulting in improved cardiac functional status. However, beta-blockers are also known for their side effects including potential worsening of pulmonary conditions. Thus, heart failure patients who also suffer from asthma or COPD should be monitored while taking beta-blockers. While patient examinations in a doctor's office provide for the diagnosis of whether a heart failure patient also suffers asthma, biweekly titration of beta-blockers presents a challenge to an efficient and effective treatment.

For these and other reasons, there is a need for an efficient method and system to monitor the treatment of heart failure patients with cardiopulmonary comorbidities.

5

Summary

A system receives signals indicative of cardiopulmonary conditions sensed by a plurality of sensors and provides for monitoring and automated differential diagnosis of the cardiopulmonary conditions based on the signals. The cardiopulmonary conditions include cardiogenic pulmonary edema and various pulmonary diseases.

10

In one embodiment, a system for detecting cardiopulmonary conditions includes a parameter input, a pulmonary edema detector, a low forced vital capacity (FVC) detector, and a pulmonary condition detector. The parameter input receives parameters indicative of a plurality of cardiopulmonary conditions. The parameters include an FVC parameter, a forced expiratory volume (FEV) parameter, and one or more edema-indicating parameters. The pulmonary edema detector detects cardiogenic pulmonary edema based on the one or more edema-indicating parameters. If the cardiogenic pulmonary edema is not detected, the low FVC detector detects a low FVC when the FVC parameter is below a predetermined threshold FVC parameter value. If the low FVC is detected, the pulmonary condition detector detects at least obstructive pulmonary disease and restrictive pulmonary disease based on the FVC parameter and the FEV parameter.

15

20

In one embodiment, a system includes an implantable medical device and an external system communicating with the implantable medical device via telemetry. The implantable medical device includes one or more sensors, an implant processor, and an implant telemetry module. The one or more sensors sense one or more signals indicative of a plurality of cardiopulmonary conditions. The implant processor processes the one or more signals. The implant telemetry module transmits the processed one or more signals to the external system. The external system includes an external telemetry module and an external processor. The external telemetry module receives the processed one or more signals. An external processor includes a cardiopulmonary condition detector that detects the plurality of cardiopulmonary conditions based on the

25

30

processed one or more signals. The cardiopulmonary condition detector includes at least a cardiogenic pulmonary edema detector, an obstructive pulmonary disease detector, and a restrictive pulmonary disease detector.

5 In one embodiment, cardiopulmonary conditions are detected by executing an automatic detection algorithm using signals indicative of the cardiopulmonary conditions as inputs. According to the algorithm, cardiogenic pulmonary edema is detected based on at least one edema-indicating signal. An FVC parameter and an FEV parameter are measured from a respiratory signal. If the cardiogenic pulmonary edema is not detected, obstructive pulmonary
10 disease and restrictive pulmonary disease are detected based on the measured FVC parameter and the measured FEV parameter.

In one embodiment, a method for monitoring cardiopulmonary conditions is provided. According to the method, signals indicative of a plurality of cardiopulmonary conditions are sensed using implantable sensors. Parameters
15 are produced based on the signals. The plurality of cardiopulmonary conditions is detected based on the parameters. The plurality of cardiopulmonary conditions includes at least cardiogenic pulmonary edema, obstructive pulmonary disease, and restrictive pulmonary disease.

This Summary is an overview of some of the teachings of the present
20 application and not intended to be an exclusive or exhaustive treatment of the present subject matter. Further details about the present subject matter are found in the detailed description and appended claims. Other aspects of the invention will be apparent to persons skilled in the art upon reading and understanding the following detailed description and viewing the drawings that form a part thereof,
25 each of which are not to be taken in a limiting sense. The scope of the present invention is defined by the appended claims and their equivalents.

Brief Description of the Drawings

The drawings illustrate generally, by way of example, but not by way of
30 limitation, various embodiments discussed in the present document. The drawing are for illustrative purposes only and not to scale nor anatomically accurate.

FIG. 1 is a flow chart illustrating one embodiment of a method for detecting cardiopulmonary conditions, including FIGS. 1A – C each showing portions of the flow chart.

FIG. 2A is a graph illustrating a respiratory signal indicative of normal pulmonary function.

FIG. 2B is a graph illustrating a respiratory signal indicative of obstructive pulmonary diseases.

FIG. 2C is a graph illustrating a respiratory signal indicative of restrictive pulmonary diseases.

FIG. 3 is a block diagram illustrating one embodiment of a cardiopulmonary condition detector.

FIG. 4 is a block diagram illustrating one embodiment of a pulmonary edema detector being part of the cardiopulmonary condition detector.

FIG. 5 is a block diagram illustrating one embodiment of a cardiopulmonary condition detection system including the cardiopulmonary condition detector.

FIG. 6 is an illustration of one embodiment of a system for monitoring heart failure patients with cardiopulmonary comorbidities and portions of the environment in which the system is used.

FIG. 7 is a block diagram illustrating one embodiment of a circuit of the system of FIG. 6.

FIG. 8 is a flow chart illustrating one embodiment of a method for monitoring heart failure patients with cardiopulmonary comorbidities.

Detailed Description

In the following detailed description, reference is made to the accompanying drawings which form a part hereof, and in which is shown by way of illustration specific embodiments in which the invention may be practiced. These embodiments are described in sufficient detail to enable those skilled in the art to practice the invention, and it is to be understood that the embodiments may be combined, or that other embodiments may be utilized and that structural, logical and electrical changes may be made without departing from the spirit and scope of the present invention. The following detailed

description provides examples, and the scope of the present invention is defined by the appended claims and their equivalents.

It should be noted that references to “an”, “one”, or “various” embodiments in this disclosure are not necessarily to the same embodiment, and
5 such references contemplate more than one embodiment.

This document discusses, among other things, a method and system for monitoring a heart failure patient with cardiopulmonary comorbidities using one or more implantable sensors incorporated into, or coupled to, an implantable medical device. The monitoring includes detection of the cardiopulmonary
10 disorders by differential diagnoses based on sensed signals on a continuous or periodic basis. The result of the detection serves as a basis for making therapeutic decisions, such as starting, stopping, adjusting, and optimizing a therapy.

In this document, “cardiogenic pulmonary edema” refers to pulmonary edema resulted from heart failure and includes cardiogenic pulmonary edema or
15 an indication of cardiogenic pulmonary edema.

In this document, a “user” includes a physician or other caregiver who examines and/or treats a patient using one or more of the methods and apparatuses discussed in the present document.

20 In this document, a “forced vital capacity (FVC) parameter” includes a parameter being a measure of the FVC, and a “forced expiratory volume (FEV) parameter” includes a parameter being a measure of the FEV. In one embodiment, the FVC parameter is a direct measure of the FVC, and the FEV parameter is a direct measure of the FEV. Such direct measures are obtained, for
25 example, by measuring respiratory volumes using a spirometer. In another embodiment, the FVC parameter is an estimate of the FVC, and the FEV parameter is an estimate of the FEV. Such estimates are obtained, for example, by measurements performed on a thoracic impedance signal indicative of respiratory pattern and activities. In this embodiment, the FVC parameter is
30 used to represent or indicate the FVC, and the FEV parameter is used to represent or indicate the FEV. In another embodiment, the FVC parameter and the FEV parameter are measured parameters providing for a calculation or estimation of an FVC-to-FEV ratio or an FEV-to-FVC ratio. In the description below, “FVC” includes an FVC or an FVC parameter, and “FEV” includes an

FEV or an FEV parameter. The term “threshold FVC” includes a threshold FVC parameter value.

FIGS. 1A – C show a flow chart illustrating one embodiment of a method for detecting cardiopulmonary conditions. The method provides for detection of cardiogenic pulmonary edema, obstructive pulmonary disease, and restrictive pulmonary disease by a differential diagnostic process. In one embodiment, the method of FIGS. 1A – C is implemented as an automatic detection algorithm. In one specific embodiment, the automatic detection algorithm is executed by a combination of hardware and software of a computer-based system. In another specific embodiment, the automatic detection algorithm is implemented as a program executable by a computer or other computerized device. In one embodiment, the program is stored in a computer-readable medium to allow installation in computerized medical device systems. In one embodiment, the result of the execution of the automatic detection algorithm serves as a basis for making therapeutic decisions, such as to start, stop, adjust, and optimize a therapy. In a further embodiment, the therapy is optimized based on the result of the execution of the automatic detection algorithm on a continuous basis. In another further embodiment, the therapy is optimized based on the result of the execution of the automatic detection algorithm on a predetermined schedule, such as on a periodic basis. The therapy includes any therapy or combination of therapies treating one or more of the detected cardiopulmonary conditions, such as a drug therapy, an electrical therapy, a biological therapy, or any combination of these.

Signals and/or parameters indicative of the cardiopulmonary conditions are received at 100. In one embodiment, the signals are sensed by implantable sensors. In one further embodiment, the implantable sensors are connected to or included in an implantable medical device. The parameters are derived from the signals for the detection of the cardiopulmonary conditions.

Dyspnea is to be detected at 102. In one embodiment, dyspnea is detected based on a respiratory signal and an activity signal. The respiratory signal, such as an impedance signal sensed by an implantable impedance sensor, indicates a patient’s lung volume, which changes cyclically with respiratory cycles (breaths) and hence the respiratory pattern. In one embodiment, the respiratory signal is a minute-ventilation (MV) impedance signal that is a

processed thoracic impedance signal indicative tidal volume and respiratory rate. MV is the product of the tidal volume (air expired during each respiratory cycle) and respiratory rate (number of respiratory cycles per minute). The thoracic impedance signal is sensed by the implantable impedance sensor. The activity
5 signal, such as an acceleration signal sensed by an implantable accelerometer, indicates the patient's gross physical activity level. Dyspnea is detected when the respiratory signal indicates rapid and shallow breath and the activity signal indicates that the rapid and shallow breath is substantially unrelated to the patient's physical activity. In one embodiment, to detect dyspnea, one or more
10 of a low tidal-volume/respiratory-rate ratio, a high inspiratory-time/total-respiratory-time ratio, and a high respiratory rate are detected at 105. The tidal volume is measured from the respiratory signal as the volume of the air expired during each respiratory cycle. The respiratory rate is calculated from the number of respiratory cycles per minute, as shown in the respiratory signal. The low
15 tidal-volume/respiratory-rate ratio is detected when a measured tidal-volume/respiratory-rate ratio is below a predetermined threshold ratio. The inspiratory time is measured from the respiratory signal as the time interval of the inspiratory phase of the respiratory cycle. The expiratory time is measured from the respiratory signal as the time interval of the expiratory phase of the
20 respiratory cycle. The high inspiratory-time/total-respiratory-time ratio, also referred to as the high inspiration/expiration ratio, is detected when the inspiratory-time/total-respiratory-time ratio exceeds a predetermined threshold ratio. The high respiratory rate is detected when the measured respiratory rate exceeds a predetermined threshold rate. If a detection of at least one of these
25 conditions is indicated at 105, a low tidal volume is to be detected at 106 by comparing the measured tidal volume to a predetermined threshold tidal volume. If a detection of the low tidal volume is indicated at 106, a detection of dyspnea is indicated at 108. If no detection of the low tidal volume is indicated at 106, a low activity level is to be detected at 107. The low activity level is detected
30 when the patient's gross physical activity level, as indicated by the activity signal, is below a predetermined threshold level representing a resting state. If a detection of the low activity level is indicated at 107, which indicates that the patient is substantially inactive, a detection of dyspnea is indicated at 108.

In another embodiment, dyspnea is detected by receiving a command triggering the process of detecting the cardiopulmonary conditions. For example, the command is entered by the patient based on his/her physical feeling or by another person observing or examining the patient. In one embodiment, 5 dyspnea is detected either automatically based on the respiratory signal and/or the activity signal, as discussed above, or by a person based on feeling or observation.

If the detection of dyspnea is indicated at 108, cardiogenic pulmonary edema is to be detected at 110. In one embodiment, cardiogenic pulmonary 10 edema is detected based on one or more signals sensed by the implantable sensors. The one or more signals each indicate one or more cardiopulmonary conditions. In a further embodiment, cardiogenic pulmonary edema is detected based on one or more parameters each produced based on the one or more signals sensed by the implantable sensors. In one specific embodiment, 15 cardiogenic pulmonary edema is detected by detecting a low heart rate variability (HRV), i.e., when a measured HRV is lower than a predetermined threshold HRV, or when a decrease in the measured HRV exceeds a predetermined margin, at 115. In another specific embodiment, cardiogenic pulmonary edema is detected by detecting a high very-low-frequency (VLF) 20 HRV, i.e., when a measured VLF HRV is higher than a predetermined threshold VLF HRV, at 115. The VLF HRV includes components of the HRV having frequencies between about 0.0033 Hz and 0.04 Hz. A high VLF HRV is suggestive of periodic breathing. In another specific embodiment, cardiogenic pulmonary edema is detected by detecting a high ratio of low-frequency (LF) 25 HRV to high-frequency (HF) HRV, i.e., when the LF-HRV/HF-HRV ratio exceeds a predetermined threshold ratio, at 115. The LF HRV includes components of the HRV having frequencies between about 0.04 Hz and 0.15 Hz. The HF HRV includes components of the HRV having frequencies between about 0.15 Hz and 0.40 Hz. The LF-HRV/HF-HRV ratio is used to track trends 30 in shifts of autonomic balance. A substantial change in the LF-HRV/HF-HRV ratio indicates a change in systemic stress that indicates the degree to which the sympathetic nervous system is over-stimulated. In another specific embodiment, cardiogenic pulmonary edema is detected by detecting a high very-low-frequency (VLF) impedance, i.e., when a VLF impedance exceeds a

predetermined threshold VLF impedance, at 115. The VLF impedance includes VLF components of a thoracic impedance signal sensed by an implantable impedance sensor and suggests periodic breathing. The VLF components are within a frequency range of about 0.0033 Hz to 0.016 Hz. In another specific embodiment, cardiogenic pulmonary edema is detected by detecting a high third heart sound (S3) amplitude, i.e., when the S3 amplitude exceeds a predetermined threshold amplitude, at 115. A substantial presence of S3 indicates heart failure. In another specific embodiment, cardiogenic pulmonary edema is detected by detecting an S3 index, i.e., when the S3 index exceeds a predetermined threshold level, at 115. The S3 index is a ratio, or an estimate of the ratio, of the number of S3 beats to the number of all heart beats, where the S3 beats are each a heart beat during which an occurrence of S3 is detected. It is a measure of a frequency of S3 presence used to indicate heart failure. In another specific embodiment, cardiogenic pulmonary edema is detected by detecting a direct-current (DC) impedance, i.e., when the DC impedance is below a predetermined threshold DC impedance, at 115. The DC impedance includes DC (and/or ultra-low-frequency) components of the thoracic impedance signal sensed by the implantable impedance sensor and indicates a lung fluid status. In one embodiment, cardiogenic pulmonary edema is detected by detecting one of the low HRV, the high VLF HRV, the high LF-HRV/HF-HRV ratio, the high VLF impedance, the high S3 amplitude, the high S3 index, and the low DC impedance. A detection of cardiogenic pulmonary edema is indicated at 116 after the one of these conditions is detected at 115. In another embodiment, cardiogenic pulmonary edema is detected by detecting two or more of the low HRV, the high VLF HRV, the high LF-HRV/HF-HRV ratio, the high VLF impedance, the high S3 amplitude, the high S3 index, and the low DC impedance at 115. In one specific embodiment, a unanimous or majority voting determines whether to indicate a detection of cardiogenic pulmonary edema at 116. In one specific embodiment, a weighted voting determines whether to indicate a detection of cardiogenic pulmonary edema at 116. A weighing coefficient is assigned to each of the conditions including the low HRV, the high VLF HRV, the high LF-HRV/HF-HRV ratio, the high VLF impedance, the high S3 amplitude, the high S3 index, and the low DC impedance. The detection of each of these conditions is given a predetermined weight in the voting.

If cardiogenic pulmonary edema is not detected at 115, a low FVC is to be detected at 120. The low FVC is detected when a measured FVC is less than a predetermined threshold FVC. In one embodiment, the FVC is measured from a spirometry signal. In another embodiment, the FVC is measured from a
5 respiratory signal sensed by an implantable sensor, such as the MV impedance signal.

If the low FVC is detected at 125, obstructive pulmonary disease is to be detected at 130, and restrictive pulmonary disease is to be detected at 140. Obstructive pulmonary disease is detected by detecting a low FEV_N/FVC ratio,
10 i.e., when the ratio of the measured FEV_N (where N denotes that the FEV is measured at N seconds after the expiration phase of a respiratory cycle starts) to the measured FVC falls below a predetermined obstructive pulmonary disease threshold ratio at 135. In one embodiment, the FVC and the FEV_N are both
15 measured from the spirometry signal. In another embodiment, the FVC and the FEV_N are both measured from the respiratory signal sensed by the implantable sensor, such as the MV impedance signal. If the low FEV_N/FVC ratio is detected at 135, a detection of obstructive disease is indicated at 136. In
one embodiment, the restrictive pulmonary disease is detected by detecting a high FEV_N/FVC ratio, i.e., when the ratio of the measured FEV_N to the measured
20 FVC exceeds a predetermined restrictive pulmonary disease threshold ratio at 145. If the high FEV_N/FVC ratio is detected at 145, a detection of restrictive pulmonary disease is indicated at 146.

One or more of the thresholds used in the detection of dyspnea, cardiogenic pulmonary edema, low FVC, obstructive pulmonary disease, and
25 restrictive pulmonary disease as described above with reference to steps 105, 106, 107, 115, 125, 135, and 145 are individually established and adjusted for each patient. In one embodiment, all the thresholds are established based on baseline data collected when the system is initially used with a patient and when
the patient is in a stable condition. The baseline data represent the patient's
30 baseline condition, which is used as a reference for future progress of the conditions. In one embodiment, one or more of the thresholds are verified periodically when a patient is known to be in a stable condition and adjusted when appropriate.

FIGS. 2A – C illustrate the measurement of the FVC and FEV_N . FIG. 2A is a graph illustrating a respiratory signal 200A indicative of normal pulmonary function. FIG. 2B is a graph illustrating a respiratory signal 200B indicative of a respiratory pattern seen in an obstructive pulmonary disease. FIG. 2C is a graph illustrating a respiratory signal 200C indicative of a respiratory pattern seen in a restrictive pulmonary disease. In FIGS. 2A – C, the respiratory signals are each a signal indicative of lung volume, which changes cyclically with the respiration cycles and shows the respiratory pattern. In one embodiment, respiratory signals 200A – C are spirometry signals sensed by a spirometer. In another embodiment, respiratory signals 200A – C are respiratory signals sensed by an implantable sensor, such as the MV impedance signal sensed by the implantable impedance sensor. The FVC is measured as the change of the lung volume from the beginning of the expiratory phase to the beginning of the inspiratory phase in a respiratory cycle. As illustrated in FIGS. 2A – C, the FVC for respiratory signal 200A is measured as the change in lung volume between points 202A and 204A; the FVC for respiratory signal 200B is measured as the change in the lung volume between points 202B and 204B; and the FVC for respiratory signal 200C is measured as the change in the lung volume between points 202C and 204C. The FEV_N is measured as the change in the lung volume over a predetermined time interval (N seconds) starting with the beginning of the expiratory phase. In one specific embodiment, as illustrated in FIGS. 2A – C, the predetermined time interval is 1.0 second, and FEV_1 is measured. The FEV_1 for respiratory signal 200A is measured as the change in the lung volume between points 202A and 206A; the FEV_1 for respiratory signal 200B is measured as the change in the lung volume between points 202B and 206B; and the FEV_1 for respiratory signal 200C is measured as the change in the lung volume between points 202C and 206C. In other embodiments, the FEV_N are measured at other times such as 3 or 6 seconds after the beginning of the respiratory cycle (i.e., FEV_3 or FEV_6), and the thresholds for detecting the high FEV_N/FVC ratio and the low FEV_N/FVC ratio are adjusted accordingly.

FIG. 3 is a block diagram illustrating one embodiment of a cardiopulmonary condition detector 300 for detecting cardiopulmonary conditions. Cardiopulmonary condition detector 300 includes a parameter input 310, a threshold input 312, a pulmonary edema detector 320, a low FVC detector

330, and a pulmonary condition detector 340. Pulmonary condition detector 340 includes an obstructive pulmonary disease detector 342 and a restrictive pulmonary disease detector 344. In one embodiment, cardiopulmonary condition detector 300 includes a computerized circuit executing the automatic
5 detection algorithm discussed above with reference to FIGS. 1A – C.

Parameter input 310 receives parameters indicative the cardiopulmonary conditions. The parameters are used for the detections performed by cardiopulmonary condition detector 300. In one embodiment, the parameters are produced based on signals sensed by implantable sensors. In another
10 embodiment, the parameters are sensed by a combination of implantable and external sensors.

Threshold input 312 receives threshold values used by detectors 320, 330, 342, and 344. In one embodiment, one or more of these threshold values are programmable and adjusted for each individual patient.

15 Pulmonary edema detector 320 receives a parameter indicative of pulmonary fluid status and detects cardiogenic pulmonary edema by comparing the signal to a predetermined threshold. FIG. 4 is a block diagram illustrating a circuit of pulmonary edema detector 420 as one embodiment of pulmonary edema detector 320. Pulmonary edema detector 420 includes a low HRV
20 detector 421, a high VLF HRV detector 422, a high LF-HRV/HF-HRV ratio detector 423, a high VLF impedance detector 424, a high S3 amplitude detector 425, a high S3 index detector 426, a low DC impedance detector 427, and a cardiogenic pulmonary edema indicator 429. Low HRV detector 421 includes a comparator having a first input receiving the HRV, a second input representing a
25 predetermined threshold HRV, and an output indicating a detection of cardiogenic pulmonary edema when the HRV is lower than the predetermined threshold HRV or when the decrease in the HRV exceeds the predetermined margin. High VLF HRV detector 422 includes a comparator having a first input receiving the VLF HRV, a second input representing a predetermined threshold
30 VLF HRV, and an output indicating a detection of cardiogenic pulmonary edema when the VLF HRV exceeds the predetermined threshold VLF HRV. High LF-HRV/HF-HRV ratio detector 423 includes a comparator having a first input receiving the LF-HRV/HF-HRV ratio, a second input representing a predetermined threshold ratio, and an output indicating a detection of

cardiogenic pulmonary edema when the LF-HRV/HF-HRV ratio exceeds the predetermined threshold ratio. High VLF impedance detector 424 includes a comparator having a first input receiving the VLF impedance signal, a second input representing a predetermined threshold VLF impedance, and an output

5 indicating a detection of cardiogenic pulmonary edema when the VLF impedance exceeds the predetermined threshold VLF impedance. High S3 amplitude detector 425 includes a comparator having a first input receiving the signal indicative of the S3 amplitude, a second input representing a predetermined threshold amplitude, and an output indicating a detection of

10 cardiogenic pulmonary edema when the S3 amplitude exceeds the predetermined threshold amplitude. High S3 index detector 426 includes a comparator having a first input receiving the signal indicative of the S3 index, a second input representing a predetermined threshold index level, and an output indicating a detection of cardiogenic pulmonary edema when the S3 index exceeds the

15 predetermined threshold index level. Low DC impedance detector 427 includes a comparator having a first input receiving the DC impedance signal, a second input representing a predetermined threshold DC impedance, and an output indicating a detection of cardiogenic pulmonary edema when the DC impedance is below the predetermined threshold DC impedance. Cardiogenic pulmonary

20 edema indicator 429 indicates a detection of cardiogenic pulmonary edema based on results of detection by the one or more of detectors 421 – 427. When two or more of the detectors 421 – 427 produce results of detection, in one embodiment, cardiogenic pulmonary edema indicator 429 indicates a detection of cardiogenic pulmonary edema if detected by any of detectors cardiogenic. In

25 another embodiment, cardiogenic pulmonary edema indicator 429 indicates a detection of cardiogenic pulmonary edema based on a unanimous or majority voting. In another embodiment, cardiogenic pulmonary edema indicator 429 indicates a detection of cardiogenic pulmonary edema based on a weighted voting, for which predetermined weighing coefficients are assigned to each of

30 the low HRV, high VLF HRV, high LF-HRV/HF-HRV ratio, high VLF impedance, high S3 amplitude, high S3 index, and low DC impedance detections. In one embodiment, pulmonary edema detector 420 is programmable for selective activation of one or more of detectors 421 – 427. The selection is based on the availability of the parameters (the HRV, VLF HRV, LF-HRV/HF-

HRV ratio, VLF impedance, S3 amplitude, S3 index, and DC impedance) and/or a medical judgment on the reliability of detection. In other embodiments, pulmonary edema detector 420 includes any subset of detectors 421 – 427 and cardiogenic pulmonary edema indicator 429.

5 Low FVC detector 330 detects a low FVC if pulmonary edema detector 320 does not indicate a detection of cardiogenic pulmonary edema. Low FVC detector 330 includes a comparator having a first input receiving a measured FVC, a second input representing a predetermined threshold FVC, and an output indicating a low FVC when the measured FVC is less than the predetermined
10 threshold FVC.

 If low FVC detector 330 indicates a detection of the low FVC, obstructive pulmonary disease detector 342 detects an obstructive pulmonary disease, and restrictive pulmonary disease detector 344 detects a restrictive
15 pulmonary disease, both based on a ratio of the FEV_N/FVC ratio. Obstructive pulmonary disease detector 342 includes a comparator having a first input receiving the FEV_N/FVC ratio, a second input representing a predetermined obstructive pulmonary disease threshold ratio, and an output indicating a detection of obstructive pulmonary disease when the FEV_N/FVC ratio is below the predetermined obstructive pulmonary disease threshold ratio. Restrictive
20 pulmonary disease detector 344 includes a comparator having a first input receiving the FEV_N/FVC ratio, a second input representing a predetermined restrictive pulmonary disease threshold ratio, and an output indicating a detection of restrictive pulmonary disease when the FEV_N/FVC ratio exceeds the predetermined restrictive pulmonary disease threshold ratio.

25 In one embodiment, cardiopulmonary condition detector 300 includes a command receiver to receive a command triggering the process of detecting cardiogenic pulmonary edema, low FVC, obstructive pulmonary disease, and restrictive pulmonary disease. In one embodiment, the command is entered by a person such as the patient or a physician or other caregiver. In another
30 embodiment, cardiopulmonary condition detector 300 includes a dyspnea detector to produce the command upon a detection of dyspnea. In one embodiment, the dyspnea detector receives a respiratory parameter and an activity level parameter to detect rapid and shallow breath when the patient is at a substantially resting state. In one specific embodiment, the respiratory

parameter is the MV impedance sensed by the implantable impedance sensor, and the activity level parameter is derived from the acceleration signal sensed by the implantable accelerometer.

FIG. 5 is a block diagram illustrating one embodiment of a
5 cardiopulmonary condition detection system 500 including cardiopulmonary condition detector 300. System 500 includes a signal input 502 that receives signals sensed by one or more sensors and a signal processor 504 that produces the parameters used by cardiopulmonary condition detector 300 based on the received signals. A threshold circuit 506 provides cardiopulmonary condition
10 detector 300 with the thresholds used in the detection of the cardiopulmonary conditions. In one embodiment, signal input 502 receives signals from the implantable sensors. In one specific embodiment, the implantable sensors are included in, and/or connected to, one implantable medical device. In another embodiment, signal input 502 receives signals from both implantable and
15 external sensors.

In one embodiment, system 500 operates by executing an automatic detection algorithm that includes signal processing and parameter production, in addition to the functions of the automatic detection algorithm discussed above with reference to FIGS. 1A – C. System 500 receives signals indicative of
20 cardiopulmonary conditions and detects the cardiopulmonary conditions by executing the automatic detection algorithm using the received signals as inputs. The cardiopulmonary conditions include at least cardiogenic pulmonary edema, obstructive pulmonary disease, and restrictive pulmonary disease.

Signal input 502 includes, but is not limited to, one or more of a cardiac
25 signal input, an impedance signal input, a heart sound signal input, an activity signal input, and a spirometry signal input, depending on which parameters are used for the detections performed by cardiopulmonary condition detector 300. The cardiac signal input receives one or more signals indicative of HRV. In one embodiment, the cardiac signals include one or more electrograms sensed by an
30 implantable medical device having an electrogram sensing circuit. In another embodiment, the cardiac signals include event markers representing cardiac depolarizations detected from the one or more electrograms. The impedance signal input receives one or more impedance signals each indicative of one or more of minute ventilation (lung volume, respiratory pattern), periodic

breathing, and pulmonary fluid status. In one embodiment, the one or more impedance signals include a thoracic impedance signal sensed by an implantable impedance sensor. The heart sound input receives one or more heart sound signals indicative of at least S3. In one embodiment, the one or more heart
5 sound signals include an acceleration signal indicative of cardiac mechanical activities sensed by an implantable accelerometer. In another embodiment, the one or more heart sound signals include an acoustic signal sensed by an implantable microphone. The activity signal input receives an activity signal indicative of the patient's gross physical activity level. In one embodiment, the
10 activity signal includes an acceleration signal sensed by an implantable accelerometer. The spirometry signal input receives a spirometry signal indicative of the lung volume sensed by an external spirometer.

Signal processor 504 produces the parameters selected for the detections performed by cardiopulmonary condition detector 300 by processing the signals
15 received by signal input 502. Signal processor 504 includes one or more of an HRV processor, an impedance processor, a heart sound processor, an activity signal processor, and a respiratory signal processor.

The HRV processor produces one or more of the HRV, the VLF HRV, and the LF-HRV/HF-HRV ratio. In one embodiment, the HRV processor
20 includes an HRV measurement module, a VLF HRV generator, an LF HRV generator, an HF HRV generator, and an LF-HRV/HF-HRV ratio calculator. The HRV measurement module measures the HRV based on the one or more electrograms. The VLF HRV generator produces the VLF HRV by extracting the components of the HRV within a VLF frequency band of about 0.0033 –
25 0.04 Hz. In one embodiment, the VLF HRV generator includes a filter to produce the VLF HRV as a time-domain signal. In another embodiment, the VLF HRV generator includes a spectral analyzer to produce the VLF HRV as the power distributed in the VLF frequency band. The LF HRV generator produces the LF HRV by extracting the components of the HRV within an LF
30 frequency band of about 0.04 – 0.15 Hz. In one embodiment, the LF HRV generator includes a filter to produce the LF HRV as a time-domain signal. In another embodiment, the LF HRV generator includes a spectral analyzer to produce the LF HRV as the power distributed in the LF frequency band. The HF HRV generator produces the HF HRV by extracting the components of the HRV

within an HF frequency band of about 0.15 – 0.40 Hz. In one embodiment, the HF HRV generator includes a filter to produce the HF HRV as a time-domain signal. In another embodiment, the HF HRV generator includes a spectral analyzer to produce the HF HRV as the power distributed in the HF frequency band. The LF-HRV/HF-HRV ratio calculator calculates the LF-HRV/HF-HRV ratio by dividing the LF HRV by the HF HRV.

The impedance processor produces the MV impedance, DC impedance, and VLF impedance based on the one or more impedance signals. In one embodiment, the impedance processor includes an MV impedance generator to produce an MV impedance indicative of minute ventilation, a VLF impedance signal generator to produce a VLF impedance suggestive of periodic breathing, and an DC impedance generator to produce an DC impedance indicative of pulmonary fluid status, all from a thoracic impedance signal sensed by the implantable impedance sensor. The VLF impedance generator produces the VLF impedance by extracting the components of the thoracic impedance signal within a VLF frequency band of about 0.0033 – 0.016 Hz. In one embodiment, the VLF impedance generator includes a filter to produce the VLF impedance as a time-domain signal. In another embodiment, the VLF impedance generator includes a spectral analyzer to produce the VLF impedance as the power distributed in the VLF frequency band. The DC impedance generator produces the DC impedance by extracting the DC (or ultra-low-frequency) components of the thoracic impedance signal. In one embodiment, the VLF impedance generator includes a filter to produce the VLF impedance as a time-domain signal. In another embodiment, the VLF impedance generator includes a spectral analyzer to produce the VLF impedance as the power distributed in the VLF frequency band.

The heart sound processor includes an S3 detector and an S3 analyzer. The S3 detector detects S3 from the one or more heart sound signals. An example of an S3 detector is discussed in U.S. Patent Application Serial No. 10/746,853, "METHOD AND APPARATUS FOR THIRD HEART SOUND DETECTION," filed on December 24, 2003, assigned to Cardiac Pacemakers, Inc., which is incorporated herein by reference in its entirety. The S3 analyzer includes one or more of an S3 amplitude measurement module and an S3 index trending module. The S3 amplitude measurement module measures the S3

amplitude based on detected occurrences of S3. In one embodiment, the S3 amplitude measurement module measures amplitudes of a predetermined number of S3 and calculates the S3 amplitude as an average S3 amplitude. In another embodiment, the S3 amplitude measurement module measures
5 amplitudes of S3 over a predetermined time interval and calculates the S3 amplitude as an average S3 amplitude. The S3 index trending module produce the S3 index as a ratio, or an estimate of the ratio, of the number of S3 beats to the number of all heart beats, where the S3 beats are each a heart beat during which an occurrence of S3 is detected. An example of a system trending S3
10 index is discussed in U.S. Patent Application Serial No. 10/746,874, "A THIRD HEART SOUND ACTIVITY INDEX FOR HEART FAILURE MONITORING," filed on December 24, 2003, assigned to Cardiac Pacemakers, Inc., which is incorporated herein by reference in its entirety.

The activity signal processor derives the activity level from the activity
15 signal. In one embodiment, a dual-use sensor senses both the heart sound signal and the activity signal using a single accelerometer. One example of such a dual-use sensor that includes a single accelerometer is discussed in U.S. Patent Application Serial No. 10/703,175, "DUAL-USE SENSOR FOR RATE RESPONSIVE PACING AND HEART SOUND MONITORING," filed
20 November 6, 2003, assigned to Cardiac Pacemakers, Inc., which is incorporated herein by reference in its entirety.

The respiratory parameter generator includes an FVC measurement module, an FEV measurement module, and a respiratory ratio calculator. The FVC measurement module measures the FVC, and the FEV measurement
25 module measures the FEV_N , both from a respiratory signal being at least one of the MV impedance signal and the spirometry signal. The FEV measurement module is programmable for measuring the FEV_N in a predetermined time (N) referenced to the beginning of an expiratory phase. In one embodiment, the FVC measurement module and the FEV measurement module receive the
30 activity level from the activity signal processor and perform the measurements when the activity level is below a predetermined threshold level representing a substantially resting state. The respiratory ratio calculator calculates the FEV_N/FVC ratio.

Threshold circuit 506 provides the threshold values used by cardiopulmonary condition detector 300. In one embodiment, threshold circuit 506 includes an initial threshold storage circuit, a threshold receiver, and a current threshold register. The initial threshold storage circuit stores a complete set of default values for all thresholds required for the detections performed by cardiopulmonary condition detector 300. The threshold receiver receives threshold values entered for each individual patient. The current threshold register is initialized with the complete set of default values and updated with the threshold values received by the threshold receiver for the individual patient.

10 The threshold values for each individual patient are entered by the user and/or an automated threshold evaluation system. In one embodiment, the automated threshold evaluation system dynamically adjusts one or more thresholds when such a need is detected or otherwise indicated.

FIG. 6 is an illustration of one embodiment of a system 600 for monitoring heart failure patients with cardiopulmonary comorbidities and portions of the environment in which system 600 is used. System 600 includes an implantable system 605, an external system 655, and a telemetry link 640 providing for communication between implantable system 605 and external system 655.

20 Implantable system 605 includes, among other things, implantable medical device 610 and lead system 608. In various embodiments, implantable medical device 610 is an implantable cardiac rhythm management (CRM) device including one or more of a pacemaker, a cardioverter/defibrillator, a cardiac resynchronization therapy (CRT) device, a cardiac remodeling control therapy (RCT) device, a drug delivery device or a drug delivery controller, and a biological therapy device. In one embodiment, implantable medical device 610 includes implantable sensors for sensing the signals used in the detections performed by cardiopulmonary condition detector 300. In another embodiment, implantable medical device 610 and lead system 608 each include one or more of the implantable sensors. As shown in FIG. 6, implantable medical device 610 is implanted in a body 602. Lead system 608 provides connections between implantable medical device 610 and a heart 601. In various embodiments, lead system 608 includes leads for sensing physiological signals and delivering pacing pulses, cardioversion/defibrillation shocks, and/or pharmaceutical or

other substances. In one embodiment, at least one implantable sensor is incorporated into a lead of lead system 608 for placement in or about heart 601.

In one embodiment, external system 655 is a patient management system including external device 650, network 660, and remote device 670. External
5 device 650 is within the vicinity of implantable medical device 610 and communicates with implantable medical device 610 bi-directionally via telemetry link 640. Remote device 670 is in a remote location and communicates with external device 650 bi-directionally via network 660, thus allowing a user to monitor and treat a patient from a distant location. In another
10 embodiment, external system includes a programmer communicating with implantable medical device 610 bi-directionally via telemetry link 640.

System 600 includes cardiopulmonary condition detection system 500 for monitoring the heart failure patients with cardiopulmonary comorbidities. The treatment includes, but is not limited to, one or more of a drug therapy, an
15 electrical therapy (such as pacing, CRT, and RCT), and a biological therapy. The distribution of system 500 in system 600 depends on design and patient management considerations, such as the size and power consumption of each system component and the ability of monitoring the patient in various settings from various locations. In one embodiment, implantable medical device 610
20 includes the entire system 500. In another embodiment, external system 655 includes the entire system 500. In another embodiment, implantable medical device 610 includes signal input 502, and external system 655 includes signal processor 504, threshold circuit 506, and cardiopulmonary condition detector 300. In another embodiment, implantable medical device 610 includes signal
25 input 502 and signal processor 504, and external system 655 includes threshold circuit 506 and cardiopulmonary condition detector 300. In another embodiment, implantable medical device 610 includes signal input 502 and portions of signal processor 504, and external system 655 includes the other portions of signal processor 504, threshold circuit 506, and cardiopulmonary
30 condition detector 300. In another embodiment, implantable medical device 610 includes signal includes portions of signal input 502 and signal processor 504, and external system 655 includes the other portions of signal input 502 and signal processor 504, threshold circuit 506, and cardiopulmonary condition detector 300. In one specific embodiment, in which external system 655 is the

patient management system, remote device 650 includes the cardiopulmonary condition detector 300.

FIG. 7 is a block diagram illustrating one embodiment of a circuit of system 600. The circuit includes various embodiments of system 500.

5 Implantable system 605 includes sensors 720, implant processor 730, and implant telemetry module 742. In one embodiment, sensors 720, implant processor 730, and implant telemetry module 742 are included in implantable medical device 610. In another embodiment, at least one sensor of sensors 720 is external to implantable medical device 610. External system 780 includes
10 external telemetry module 744 and external processor 780. External processor 780 includes cardiopulmonary condition detector 300. In one embodiment, in which the spirometry signal is used as the respiratory signal, system 600 further includes an external spirometer to sense the spirometry signal. In one
15 embodiment, the external spirometer is electrically connected to external processor 780. In another embodiment, the external spirometer is wirelessly connected to external processor 780 via telemetry.

 Sensors 720 include one or more of a sensing circuit, an impedance sensor, a heart sound sensor, and an activity sensor. The sensing circuit senses one or more electrograms indicative of HRV. The impedance sensor senses
20 thoracic impedance. The heart sound sensor detects a heart sound signal indicative of at least S3. In one embodiment, the heart sound sensor includes an accelerometer. In another embodiment, the heart sound sensor includes a microphone. In one embodiment, the heart sound sensor is included in implantable medical device 610. In another embodiment, the heart sound sensor
25 is incorporated into a lead of lead system 608. The activity sensor senses an activity signal indicative of the patient's gross physical activity level. In one embodiment, the activity sensor includes an accelerometer. In another embodiment, a single accelerometer functions as a dual-use sensor that senses both the heart sound signal and the activity signal.

30 Implant processor 730 and external processor 780 include system 500. The specific distribution of the component of system 500 in implant processor 730 and external processor 780 depends on specific design and patient management considerations. In one embodiment, implant processor 730 includes signal input 502 and signal processor 504, and external processor 780

includes threshold circuit 506 and cardiopulmonary condition detector 300. In another embodiment, implant processor 730 includes signal input 502, and external processor 780 includes signal processor 504, threshold circuit 506, and cardiopulmonary condition detector 300. In another embodiment, implant processor 730 includes signal input 502 and portions of signal processor 504, and external processor 780 includes the other portions of signal processor 504, threshold circuit 506, and cardiopulmonary condition detector 300. In another embodiment, implant processor 730 includes portions of signal input 502 and signal processor 504, and external processor 780 includes the other portions of signal input 502 and signal processor 504, threshold circuit 506, and cardiopulmonary condition detector 300. In one specific embodiment in which both implant processor 730 and external processor 780 both include portions of signal processor 504, implant processor 730 includes one or more of the HRV measurement module, the impedance processor, the heart sound processor, and the activity signal processor; external processor includes one or more of the S3 analyzer and the respiratory parameter generator.

Implant telemetry module 742 and external telemetry module 744 supports telemetry link 640. Telemetry link 640 is a wireless bi-directional data transmission link. In one embodiment, telemetry link 640 is an inductive couple formed when two coils—one connected to implant telemetry module 742 and the other connected to external telemetry module 744—are placed near each other. In this embodiment, the patient or the user places the coil connected to external device 650 on body 602 over implantable medical device 610. In another embodiment, telemetry link 640 is a far-field radio-frequency telemetry link allowing implantable medical device 610 and external device 650 to communicate over a telemetry range that is at least ten feet. In one embodiment, implant telemetry module 742 transmits one or more signals and/or parameters indicative of cardiopulmonary conditions, and external telemetry module 744 receives these signals and/or parameters.

FIG. 8 is a flow chart illustrating one embodiment of a method for monitoring heart failure patients with cardiopulmonary comorbidities. In one embodiment, the method is performed by system 600.

Signals indicative of a plurality of cardiopulmonary conditions are sensed at 800. Based on the sensed signals, parameters indicative of the plurality of

cardiopulmonary conditions are produced at 810. An automatic detection algorithm is executed to detect the plurality of cardiopulmonary conditions based on the parameters at 820. The plurality of cardiopulmonary conditions includes at least cardiogenic pulmonary edema, obstructive pulmonary disease, and restrictive pulmonary disease. In one embodiment, the automatic detection algorithm performs the method discussed above with reference to FIGS. 1A – C.

In one specific embodiment using system 600, sensors 720 senses the signals at 800. Implant processor 730 and/or external processor 780 produce the parameters at 810. Cardiopulmonary condition detector 300 executes the automatic detection algorithm to detect cardiogenic pulmonary edema, obstructive pulmonary disease, and restrictive pulmonary disease based on the parameters.

It is to be understood that the above detailed description is intended to be illustrative, and not restrictive. For example, the method for detecting the cardiopulmonary conditions including cardiogenic pulmonary edema, obstructive pulmonary disease, and restrictive pulmonary disease may be implemented without using implantable sensors. The method of using a combination of implantable and external systems for differential diagnostic purposes is not limited to diagnosis of cardiopulmonary conditions. Other embodiments, including any possible permutation of the system components discussed in this document, will be apparent to those of skill in the art upon reading and understanding the above description. The scope of the invention should, therefore, be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled.

25

What is claimed is:

1. A system for detecting cardiopulmonary conditions, comprising:
a parameter input to receive parameters indicative of a plurality of
5 cardiopulmonary conditions, the parameters including a forced vital capacity (FVC) parameter, a forced expiratory volume (FEV) parameter, and one or more edema-indicating parameters indicative of cardiogenic pulmonary edema;
a pulmonary edema detector coupled to the parameter input, the
pulmonary edema detector adapted to detect the cardiogenic pulmonary edema
10 based on the one or more edema-indicating parameters;
a low FVC detector coupled to the pulmonary edema detector, the low
FVC detector adapted to detect a low FVC when the FVC parameter is below a
predetermined threshold FVC parameter value if the cardiogenic pulmonary
edema is not detected; and
15 a pulmonary condition detector coupled to the low FVC detector, the
pulmonary condition detector adapted to detect at least an obstructive pulmonary
disease and a restrictive pulmonary disease based on the FVC parameter and the
FEV parameter if the low FVC is detected.
- 20 2. The system according to claim 1, wherein the pulmonary condition
detector comprises an obstructive pulmonary disease detector adapted to detect
the obstructive pulmonary disease when a ratio of the FEV parameter to the FVC
parameter is below a predetermined obstructive pulmonary disease threshold
ratio.
25
3. The system according to any of the preceding claims, wherein the
pulmonary condition detector further comprises a restrictive pulmonary disease
detector adapted to detect the restrictive pulmonary disease when the ratio of the
FEV parameter to the FVC parameter exceeds a predetermined restrictive
30 pulmonary disease threshold ratio.
4. The system according to according to any of the preceding claims,
further comprising a respiratory parameter generator coupled to the parameter
input, the respiratory parameter generator including:

an FVC measurement module to measure the FVC parameter from a respiratory signal; and

an FEV measurement module to measure the FEV parameter from the respiratory signal.

5

5. The system according to claim 4, wherein the respiratory signal comprises a spirometry signal, and further comprising a spirometry signal input, coupled to the respiratory parameter generator, to receive the respiratory signal from a spirometer.

10

6. The system according to claim 4, wherein the respiratory signal comprises an impedance signal, and further comprising an impedance signal input, coupled to the respiratory parameter generator, to receive the impedance signal from an implantable impedance sensor.

15

7. The system according to any of claims 4 to 6, further comprising an activity signal input, coupled to the respiratory parameter generator, to receive an activity signal indicative of a physical activity level from an implantable activity sensor, and wherein the FVC measurement module is adapted to measure the FVC parameter when the activity level is below a predetermined threshold level representing a substantially resting state, and the FEV measurement module is adapted to measure the FEV parameter when the activity level is below the predetermined threshold level representing the substantially resting state.

25

8. The system according to any of the preceding claims, further comprising: a cardiac signal input to receive one or more electrograms from an implantable sensing circuit; and

a heart rate variability (HRV) processor, coupled to the cardiac signal input and the parameter input, to produce one or more parameters of the one or more edema-indicating parameters based on the one or more electrograms, the HRV processor including an HRV measurement module to measure the HRV based on the one or more electrograms.

30

9. The system according to claim 8, wherein the pulmonary edema detector comprises a low HRV detector adapted to indicate a detection of the cardiogenic pulmonary edema when the HRV is lower than a predetermined threshold HRV.

5 10. The system according to claim 8, wherein the pulmonary edema detector comprises a low HRV detector adapted to indicate a detection of the cardiogenic pulmonary edema when a decrease in the HRV exceeds a predetermined margin.

11. The system according to claim 8, wherein the HRV processor further
10 comprises a very-low-frequency (VLF) HRV generator to produce a VLF HRV having a frequency band of about 0.0033 Hz to 0.04 Hz based on the HRV, and wherein the pulmonary edema detector comprises a high VLF HRV detector adapted to indicate a detection of the cardiogenic pulmonary edema when the VLF HRV exceeds a predetermined threshold VLF HRV.

15

12. The system according to claim 8, wherein the HRV processor further comprises:

a low-frequency (LF) HRV generator to produce an LF HRV having a frequency band of about 0.04 Hz to 0.15 Hz based on the HRV;

20 a high-frequency (HF) HRV generator to produce an HF HRV having a frequency band of about 0.15 Hz to 0.40 Hz based on the HRV; and

a LF-HRV/HF-HRV ratio calculator to calculate a ratio of the LF HRV to the HF HRV,

25 wherein the pulmonary edema detector comprises a high LF-HRV/HF-HRV ratio detector adapted to indicate a detection of the cardiogenic pulmonary edema when the ratio of the LF HRV to the HF HRV exceeds a predetermined threshold ratio.

13. The system according to any of claims 1 to 7, further comprising:

30 an impedance signal input to receive at least one impedance signal from an implantable impedance sensor; and

an impedance processor, coupled to the impedance signal input and the parameter input, to produce one or more parameters of the one or more edema-indicating parameters based on the at least one impedance signal.

14. The system according to claim 13, wherein the impedance processor comprises a very-low-frequency (VLF) impedance signal generator to produce a VLF impedance having a frequency band of about 0.0033 Hz to 0.016 Hz based on the impedance signal, and wherein the pulmonary edema detector comprises a high VLF impedance detector adapted to indicate a detection of the cardiogenic pulmonary edema when the VLF impedance exceeds a predetermined threshold VLF impedance.

15. The system according to claim 13, wherein the impedance processor comprises a direct current (DC) impedance signal generator to produce a DC impedance from the impedance signal, and wherein the pulmonary edema detector comprises a low DC impedance detector adapted to indicate a detection of the cardiogenic pulmonary edema when the DC impedance is below a predetermined threshold DC impedance.

15

16. The system according to any of claims 1 to 7, further comprising:
a heart sound input to receive a heart sound signal from an implantable heart sound sensor; and

a third heart sound (S3) processor coupled to the heart sound input and the parameter input, the S3 processor including an S3 detector to detect occurrences of S3 and an S3 analyzer to produce one or more parameters of the one or more edema-indicating parameters based on the detected occurrences of S3.

17. The system according to claim 16, wherein the S3 analyzer comprises an S3 amplitude measurement module to measure an S3 amplitude, and wherein the pulmonary edema detector comprises a high S3 amplitude detector adapted to indicate a detection of the cardiogenic pulmonary edema when the S3 amplitude exceeds a predetermined threshold amplitude.

30

18. The system according to claim 16, wherein the S3 analyzer comprises an S3 index trending module to produce an S3 index being a ratio, or an estimate of the ratio, of a number of S3 beats to a number of all heart beats over a predetermined time interval, where the S3 beats are each a heart beat during

which an occurrence of S3 is detected, and wherein the pulmonary edema detector comprises a high S3 index detector adapted to indicate a detection of the cardiogenic pulmonary edema when the S3 index exceeds a predetermined threshold index level.

5

19. The system according to any of claims 1 to 7, wherein the one or more edema-indicating parameters comprise two or more of:

a heart rate variability (HRV);

a very-low-frequency (VLF) HRV suggestive of periodic breathing;

10

a ratio of low-frequency (LF) HRV to high-frequency (HF) HRV;

a very-low-frequency (VLF) impedance suggestive of periodic breathing;

a third heart sound (S3) amplitude;

an S3 index being a ratio, or an estimate of the ratio, of a number of S3 beats to a number of all heart beats over a predetermined time interval, where the

15

S3 beats are each a heart beat during which an occurrence of S3 is detected; and

a DC impedance indicative of pulmonary fluid status,

wherein the pulmonary edema detector comprises two or more of:

a low HRV detector adapted to indicate a detection of the cardiogenic pulmonary edema when a measured HRV is lower than a predetermined

20

threshold HRV;

a high VLF HRV detector adapted to indicate a detection of the cardiogenic pulmonary edema when the VLF HRV exceeds a predetermined threshold VLF HRV;

25

a high LF-HRV/HF-HRV ratio detector adapted to indicate a detection of the cardiogenic pulmonary edema when the ratio of the LF HRV to the HF HRV exceeds a predetermined threshold ratio;

a high VLF impedance detector adapted to indicate a detection of the cardiogenic pulmonary edema when the VLF impedance exceeds a predetermined threshold VLF impedance;

30

a high S3 amplitude detector adapted to indicate a detection of the cardiogenic pulmonary edema when the S3 amplitude exceeds a predetermined amplitude;

a high S3 index detector adapted to indicate a detection of the cardiogenic pulmonary edema when the S3 index exceeds a predetermined amplitude; and

- 5 a low DC impedance detector adapted to indicate a detection of the cardiogenic pulmonary edema when the DC impedance is below a predetermined threshold DC impedance.

20. The system according to claim 19, wherein the pulmonary edema detector further comprises a cardiogenic pulmonary edema indicator coupled to
10 the two or more of the low HRV detector, the high VLF HRV detector, the high LF-HRV/HF-HRV ratio detector, the high VLF impedance detector, the high S3 amplitude detector, the high S3 index detector, and the a low DC impedance detector, the cardiogenic pulmonary edema indicator adapted to indicate a detection of the cardiogenic pulmonary edema based on one or more detections
15 of the cardiogenic pulmonary edema indicated by the two or more of the low HRV detector, the high VLF HRV detector, the high LF-HRV/HF-HRV ratio detector, the high VLF impedance detector, the high S3 amplitude detector, the high S3 index detector, and the low DC impedance detector.

20 21. The system according to any of the preceding claims, further comprising a dyspnea detector coupled to the pulmonary edema detector, the dyspnea detector adapted to receive at least one dyspnea-indicating signal and detect dyspnea based on the at least one dyspnea-indicating signal, and wherein the pulmonary edema detector is adapted to detect the cardiogenic pulmonary edema
25 after each detection of the dyspnea.

22. A system, comprising:
an implantable medical device including:
one or more sensors adapted to sense one or more signals
30 indicative of a plurality of cardiopulmonary conditions;
an implant processor, coupled to the one or more sensors, to process the one or more signals; and
an implant telemetry module, coupled to the implant processor, to transmit the processed one or more signals; and

an external system communicatively coupled to the implantable medical device via telemetry, the external system including:

an external telemetry module to receive the processed one or more signals; and

5 an external processor coupled to the external telemetry module, the external processor including a cardiopulmonary condition detector adapted to detect the plurality of cardiopulmonary conditions based on the processed one or more signals, the cardiopulmonary condition detector including at least a cardiogenic pulmonary edema detector, an
10 obstructive pulmonary disease detector, and a restrictive pulmonary disease detector.

23. The system according to claim 22, wherein the implantable medical device comprises an implantable cardiac rhythm management (CRM) device.

15

24. The system according to any of claims 22 and 23, wherein the external system comprises a programmer.

25. The system according any of claims 22 and 23, wherein the external
20 system comprises a patient management system including:

an external device communicatively coupled to the implantable medical device;

a telecommunication network coupled to the external device; and

a remote device, coupled to the telecommunication network, to allow

25 access to the implantable medical device from a remote location.

26. The system according to claim 25, wherein the remote device comprises the cardiopulmonary condition detector.

30 27. The system according to any of claims 22 to 26, wherein the cardiopulmonary condition detector comprises a dyspnea detector adapted to detect dyspnea based on at least one dyspnea-indicating signal of the processed one or more signals, and wherein the pulmonary edema detector is adapted to detect a cardiogenic pulmonary edema after the dyspnea is detected.

28. The system according to any of claims 22 to 27, wherein the one or more sensors comprise a sensing circuit to sense one or more electrograms, and the implant processor comprises a heart rate variability (HRV) processor adapted to measure an HRV from the one or more electrograms and adapted to produce one
5 or more parameters indicative of cardiogenic pulmonary edema based on the HRV.

29. The system according to any of claims 22 to 27, wherein the one or more sensors comprise an impedance sensor to sense a thoracic impedance, and the
10 implant processor comprises a impedance processor adapted to produce one or more parameters indicative of cardiogenic pulmonary edema based on the thoracic impedance.

30. The system according to any of claims 22 to 27, wherein the one or more
15 sensors comprise a heart sound sensor to sense a heart sound signal indicative of at least third heart sounds (S3), and the implant processor comprises an S3 processor adapted to detect occurrences of S3 and adapted to produce one or more parameters indicative of cardiogenic pulmonary edema based on the detected occurrences of S3.

20 31. The system according to any of claims 22 to 30, wherein the obstructive pulmonary disease detector is adapted to detect an obstructive pulmonary disease based on a forced vital capacity (FVC) parameter and a forced expiratory volume (FEV) parameter, and the restrictive pulmonary disease detector is
25 adapted to detect a restrictive pulmonary disease based on the FVC parameter and the FEV parameter.

32. The system according to claim 31, wherein the cardiopulmonary condition detector further comprises a low FVC detector, coupled to the
30 cardiogenic pulmonary edema detector, to detect a low FVC when the FVC parameter is less than a predetermined threshold FVC parameter value if the cardiogenic pulmonary edema is not detected, and wherein the obstructive pulmonary disease detector is adapted to detect the obstructive pulmonary

disease if the low FVC is detected, and the restrictive pulmonary disease detector is adapted to detect the restrictive pulmonary disease if the low FVC is detected.

33. The system according to any of claims 31 and 32, further comprising an external spirometer, coupled to the external system, to sense a spirometry signal indicative of lung volume, and wherein the external processor comprises:

an FVC measurement module adapted to measure the FVC parameter from the spirometry signal; and

an FEV measurement module adapted to measure the FEV parameter from the spirometry signal.

34. The system according to any of claims 31 and 32, wherein the one or more sensors comprise an impedance sensor to sense an impedance signal indicative of minute ventilation, and the external processor comprises:

an FVC measurement module adapted to measure the FVC parameter from the impedance signal; and

an FEV measurement module adapted to measure the FEV parameter from the impedance signal.

35. The system according to claim 34, wherein the one or more sensors further comprise an activity sensor to sense an activity signal indicative of a physical activity level, and wherein:

the FVC measurement module is adapted to measure the FVC parameter from the MV impedance signal when the activity signal indicates a substantially resting state; and

the FEV measurement module is adapted to measure the FEV parameter from the MV impedance signal when the activity signal indicates a substantially resting state.

36. A method for detecting cardiopulmonary conditions, comprising: receiving signals indicative of a plurality of cardiopulmonary conditions; executing an automatic detection algorithm, the executing including:

detecting cardiogenic pulmonary edema based on at least one edema-indicating signal of the received signals;

measuring a forced vital capacity (FVC) parameter and a forced expiratory volume (FEV) parameter from at least one signal of the received signals;

5 detecting an obstructive pulmonary disease based on the measured FVC parameter and the measured FEV parameter if the cardiogenic pulmonary edema is not detected; and

detecting a restrictive pulmonary disease based on the measured FVC parameter and the measured FEV parameter if the cardiogenic pulmonary edema is not detected.

10

37. The method according to claim 36, wherein executing the automatic detection algorithm further comprises detecting a low FVC if the cardiogenic pulmonary edema is not detected, and wherein detecting the obstructive pulmonary disease comprises detecting the obstructive pulmonary disease if the low FVC is detected, and detecting the restrictive pulmonary disease comprises detecting the restrictive pulmonary disease if the low FVC is detected.

38. The method according to any of claims 36 and 37, further comprising detecting dyspnea based on at least one dyspnea-indicating signal of the received signals, and wherein detecting the cardiogenic pulmonary edema comprises detecting the cardiogenic pulmonary edema after the dyspnea is detected.

39. The method according to claim 38, wherein receiving the signals comprises receiving a respiratory signal and an activity signal, and wherein detecting the dyspnea comprises detecting dyspnea when the respiratory signal indicates rapid and shallow breath and the activity signal indicates that the rapid and shallow breath is substantially unrelated to physical activity.

40. The method according to any of claims 36 to 39, wherein receiving the signals comprises receiving at least one signal indicative of heart rate variability (HRV), and wherein detecting the cardiogenic pulmonary edema comprises detecting the cardiogenic pulmonary edema based on the HRV.

41. The method according to claim 40, further comprising:
sensing one or more electrograms indicative of the HRV; and
measuring the HRV from the one or more electrograms,
wherein detecting the cardiogenic pulmonary edema based on the HRV
5 comprises detecting the cardiogenic pulmonary edema when the HRV is lower
than a predetermined threshold HRV.
42. The method according to any of claims 36 to 39, wherein receiving the
signals comprises receiving a signal indicative of a very-low-frequency heart
10 rate variability (VLF HRV), and wherein detecting the cardiogenic pulmonary
edema comprises detecting the cardiogenic pulmonary edema based on the VLF
HRV.
43. The method according to claim 42, further comprising:
15 sensing one or more electrograms indicative of HRV; and
producing the VLF HRV including components of the HRV in a
frequency band of about 0.0033 Hz to 0.04 Hz,
wherein detecting the cardiogenic pulmonary edema based on the VLF
HRV comprises detecting the cardiogenic pulmonary edema when the VLF
20 HRV exceeds a predetermined threshold VLF HRV.
44. The method according to any of claims 36 to 39, wherein receiving the
signals comprises receiving a signal indicative of a ratio of low-frequency heart
rate variability (LF HRV) to a high-frequency heart rate variability (HF HRV),
25 and wherein detecting the cardiogenic pulmonary edema comprises detecting the
cardiogenic pulmonary edema based on the ratio of the LF HRV to the HF HRV.
45. The method according to claim 44, further comprising:
sensing one or more electrograms indicative of HRV;
30 producing a low-frequency (LF) HRV including components of the HRV
in a frequency band of about 0.05 Hz to 0.15 Hz;
producing a high-frequency (HF) HRV including components of the
HRV in a frequency band of about 0.15 Hz to 0.40 Hz; and
calculating a ratio of the LF HRV to the HF HRV,

wherein detecting the cardiogenic pulmonary edema based on the ratio of the LF HRV to the HF HRV comprises detecting the cardiogenic pulmonary edema when the ratio of the LF HRV to the HF HRV exceeds a predetermined threshold ratio.

5

46. The method according to any of claims 36 to 39, wherein receiving the signals comprises receiving a signal indicative of a very-low-frequency (VLF) impedance suggestive of periodic breathing, and wherein detecting the cardiogenic pulmonary edema comprises detecting the cardiogenic pulmonary edema based on the VLF impedance.

10

47. The method according to claim 46, further comprising:
sensing a thoracic impedance; and
producing the VLF impedance based on the thoracic impedance,
wherein detecting the cardiogenic pulmonary edema based on the VLF impedance comprises detecting the cardiogenic pulmonary edema when the VLF impedance exceeds a predetermined threshold VLF impedance.

15

48. The method according to claim 47, wherein producing the VLF impedance comprises extracting VLF components of the thoracic impedance signal, the VLF components having a frequency band of about 0.0033 Hz to 0.016 Hz.

20

49. The method according to any of claims 36 to 39, wherein receiving the signals comprises receiving a signal indicative of a direct current (DC) impedance indicative of pulmonary fluid status, and wherein detecting the cardiogenic pulmonary edema comprises detecting the cardiogenic pulmonary edema based on the DC impedance.

25

50. The method according to claim 49, further comprising:
sensing a thoracic impedance; and
producing the DC impedance based on the thoracic impedance,

30

wherein detecting the cardiogenic pulmonary edema based on the DC impedance comprises detecting the cardiogenic pulmonary edema when the DC impedance exceeds a predetermined threshold DC impedance.

- 5 51. The method according to any of claims 36 to 39, wherein receiving the signals comprises receiving a signal indicative of a third heart sound (S3) amplitude, and wherein detecting the cardiogenic pulmonary edema comprises detecting the cardiogenic pulmonary edema based on the S3 amplitude.
- 10 52. The method according to claim 51, further comprising:
 sensing a heart sound signal indicative of at least S3;
 detecting occurrences of S3 from the heart sound signal; and
 producing the S3 amplitude based on the detected occurrences of S3,
 wherein detecting the cardiogenic pulmonary edema based on the S3
15 amplitude comprises detecting the cardiogenic pulmonary edema when the S3 amplitude exceeds a predetermined threshold amplitude.
53. The method according to any of claims 36 to 39, wherein receiving the signals comprises receiving a signal indicative of a third heart sound (S3) index
20 being a ratio, or an estimate of the ratio, of the number of S3 beats to the number of all heart beats detected during a predetermined period of time, the S3 beats each being a heart beat during which an occurrence of S3 is detected, and
 wherein detecting the cardiogenic pulmonary edema comprises detecting the cardiogenic pulmonary edema based on the S3 index.
- 25 54. The method according to claim 53, further comprising:
 sensing a heart sound signal indicative of at least S3;
 detecting occurrences of S3 from the heart sound signal; and
 producing the S3 index based on the detected occurrences of S3,
30 wherein detecting the cardiogenic pulmonary edema based on the S3 index comprises detecting the cardiogenic pulmonary edema when the S3 index exceeds a predetermined threshold index level.

55. The method according to any of claims 52 and 54, wherein sensing the heart sound signal comprises sensing an acceleration signal.

56. The method according to any of claims 36 to 39, wherein receiving the
5 signals comprises receiving an impedance signal indicative of minute ventilation from an implantable impedance sensor, and wherein measuring the FVC parameter and the FEV parameter comprises measuring the FVC parameter and the FEV parameter from the impedance signal.

10 57. The method according to claim 56, further comprising:
sensing a thoracic impedance; and
producing a minute ventilation (MV) impedance signal based on the thoracic impedance, the MV impedance signal indicative of minute ventilation;
wherein measuring the FVC parameter and the FEV parameter from the
15 impedance signal comprises measuring the FVC parameter and the FEV parameter from the MV impedance signal.

58. The method according to any of claims 56 and 57, wherein receiving the signals comprises receiving an activity level signal indicative of a physical
20 activity level, and wherein measuring the FVC parameter and the FEV parameter comprises measuring the FVC parameter and the FEV parameter when the activity level is below a predetermined threshold level.

59. The method according to claim 58, wherein the activity level signal is an
25 acceleration signal, and further comprising sensing the acceleration signal.

60. The method according to any of claims 36 to 39, wherein receiving the signals comprises receiving a spirometry signal indicative of respiratory volumes from a spirometer, and wherein measuring the FVC parameter and the FEV
30 parameter comprises measuring the FVC parameter and the FEV parameter from the spirometry signal.

61. The method according to any of claims 36 to 60, wherein executing the automatic detection algorithm further comprises calculating a ratio of the FEV

parameter to the FVC parameter, and wherein detecting the obstructive pulmonary disease comprises detecting the obstructive pulmonary disease when the ratio of the FEV parameter to the FVC parameter is below a predetermined obstructive pulmonary disease threshold ratio, and detecting the restrictive pulmonary disease comprises detecting the restrictive pulmonary disease when the ratio of the FEV parameter to the FVC parameter exceeds a predetermined restrictive pulmonary disease threshold ratio.

62. The method according to any of claims 36 to 61, wherein measuring the FEV parameter comprises measuring the FEV parameter at about 1.0 second after the beginning of an expiratory phase of a respiratory cycle.

63. The method according to any of claims 36 to 62, further comprising starting, stopping, or adjusting a therapy based on a result of the executing the automatic detection algorithm.

64. The method according to claim 63, further comprising optimizing the therapy based on the result of the executing the automatic detection algorithm on a continuous basis.

65. The method according to claim 63, further comprising optimizing the therapy based on the result of the executing the automatic detection algorithm on a periodic basis.

66. The method according to claim 63, wherein the therapy comprises one or more of a drug therapy, an electrical therapy, and a biological therapy.

67. The method according to any of claims 36 to 66, further comprising sensing one or more of the signals indicative of the plurality of cardiopulmonary conditions using one or more implantable sensors.

1/10

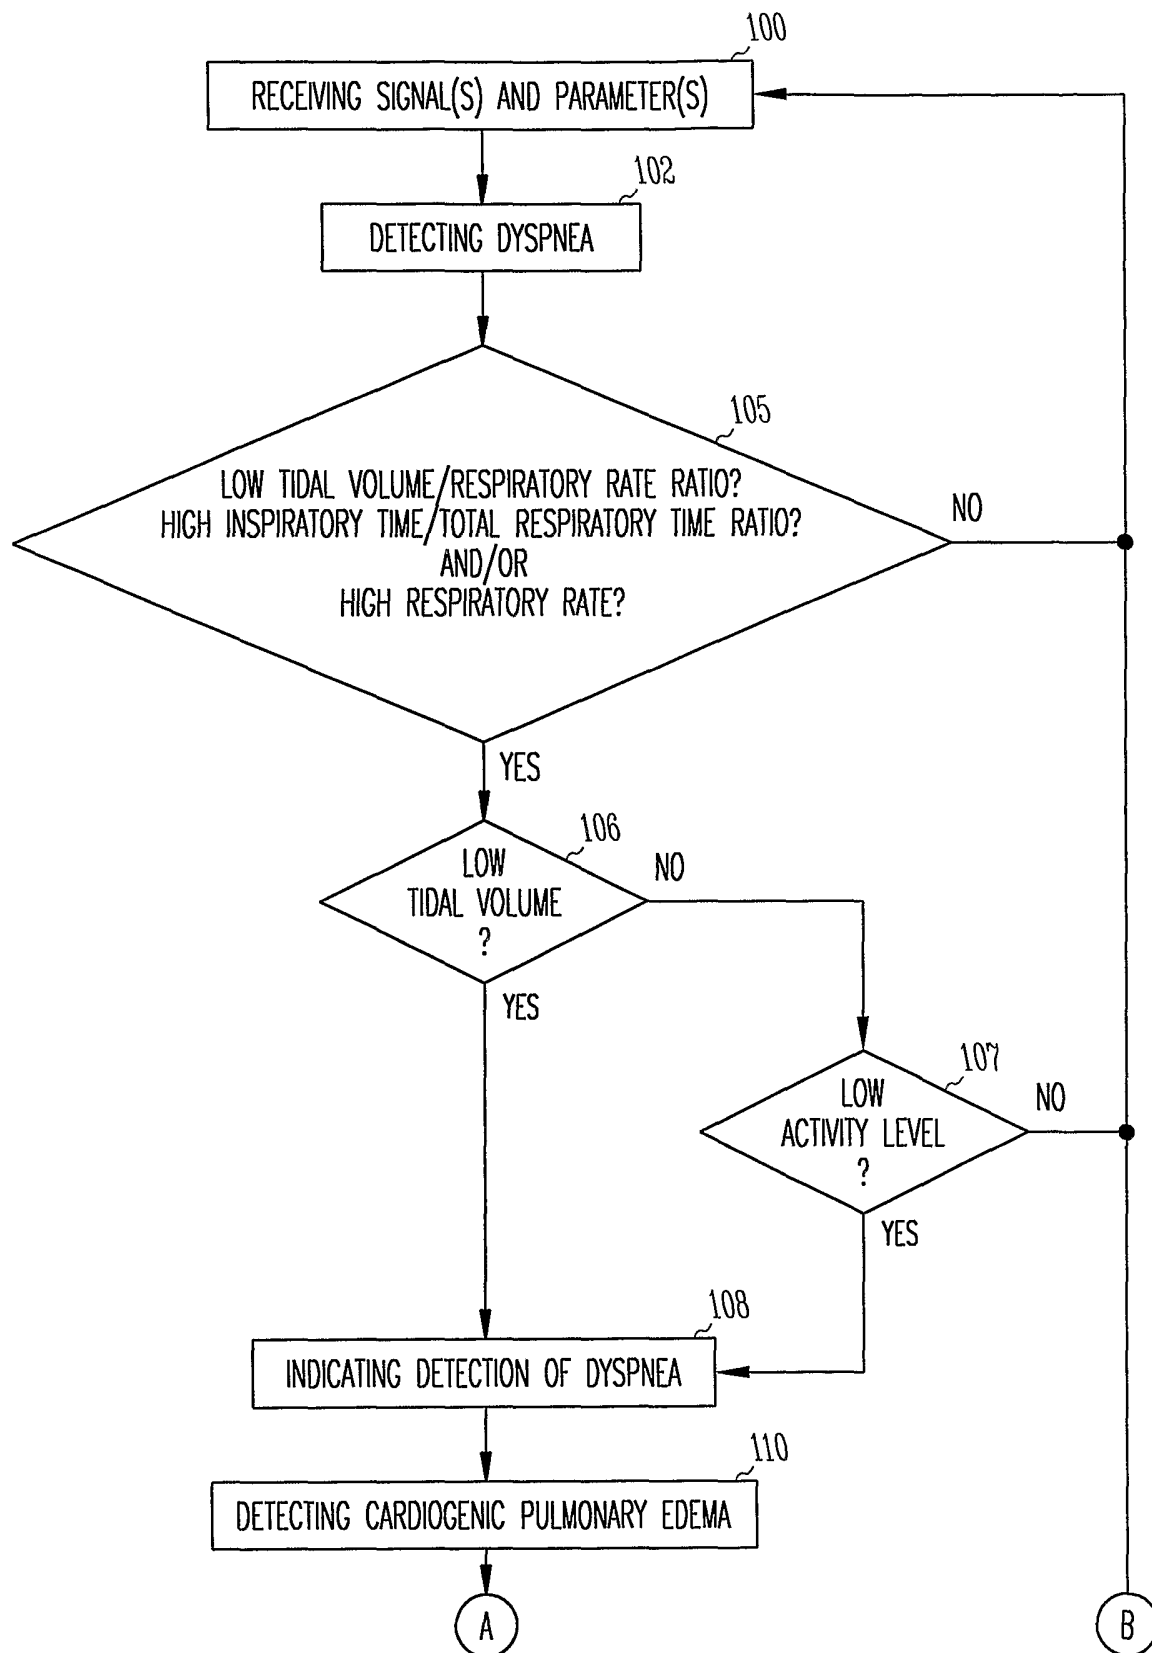


Fig.1A

2/10

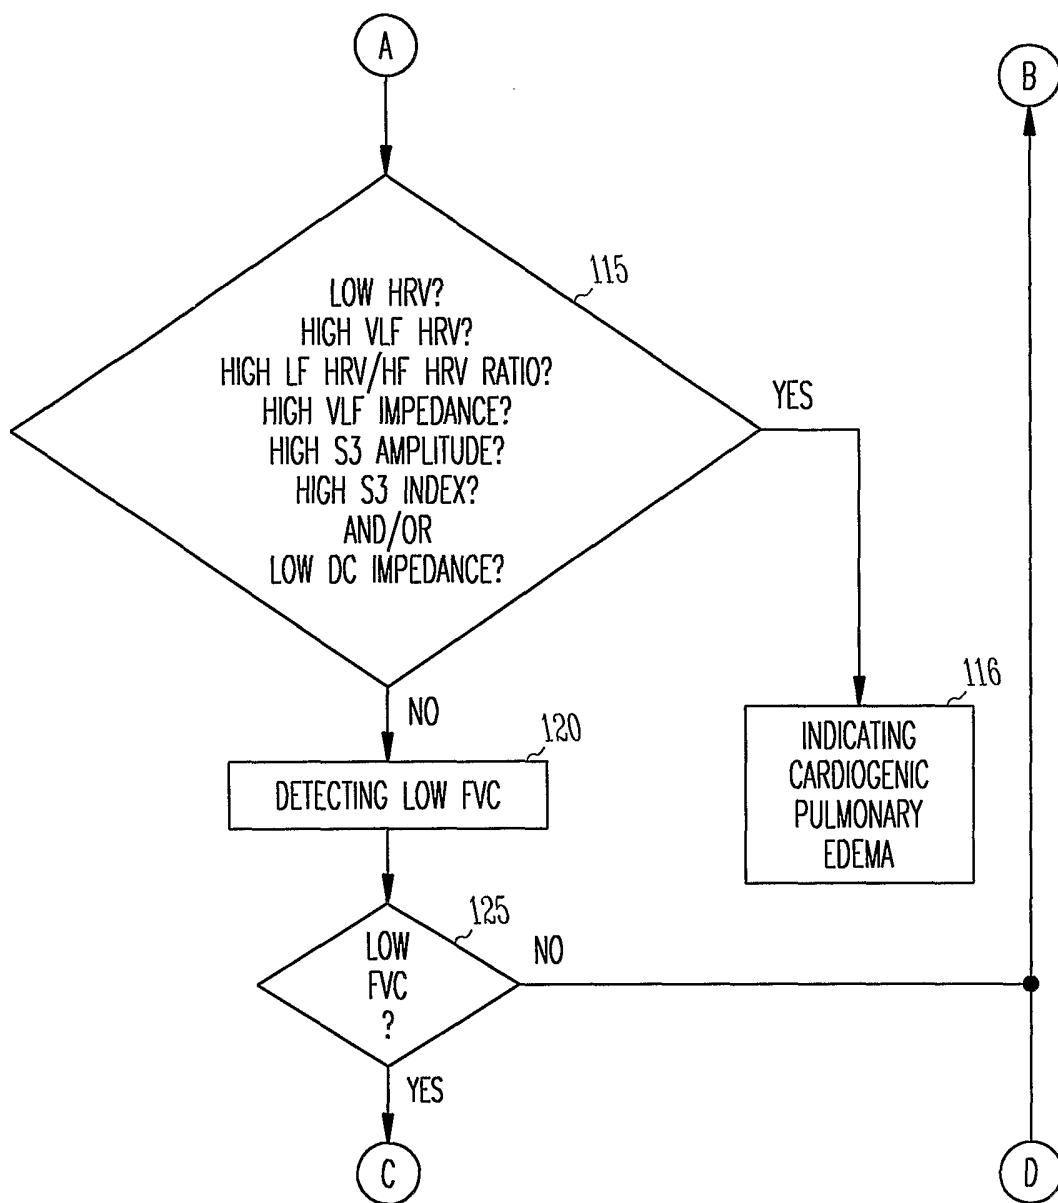


Fig.1B

3/10

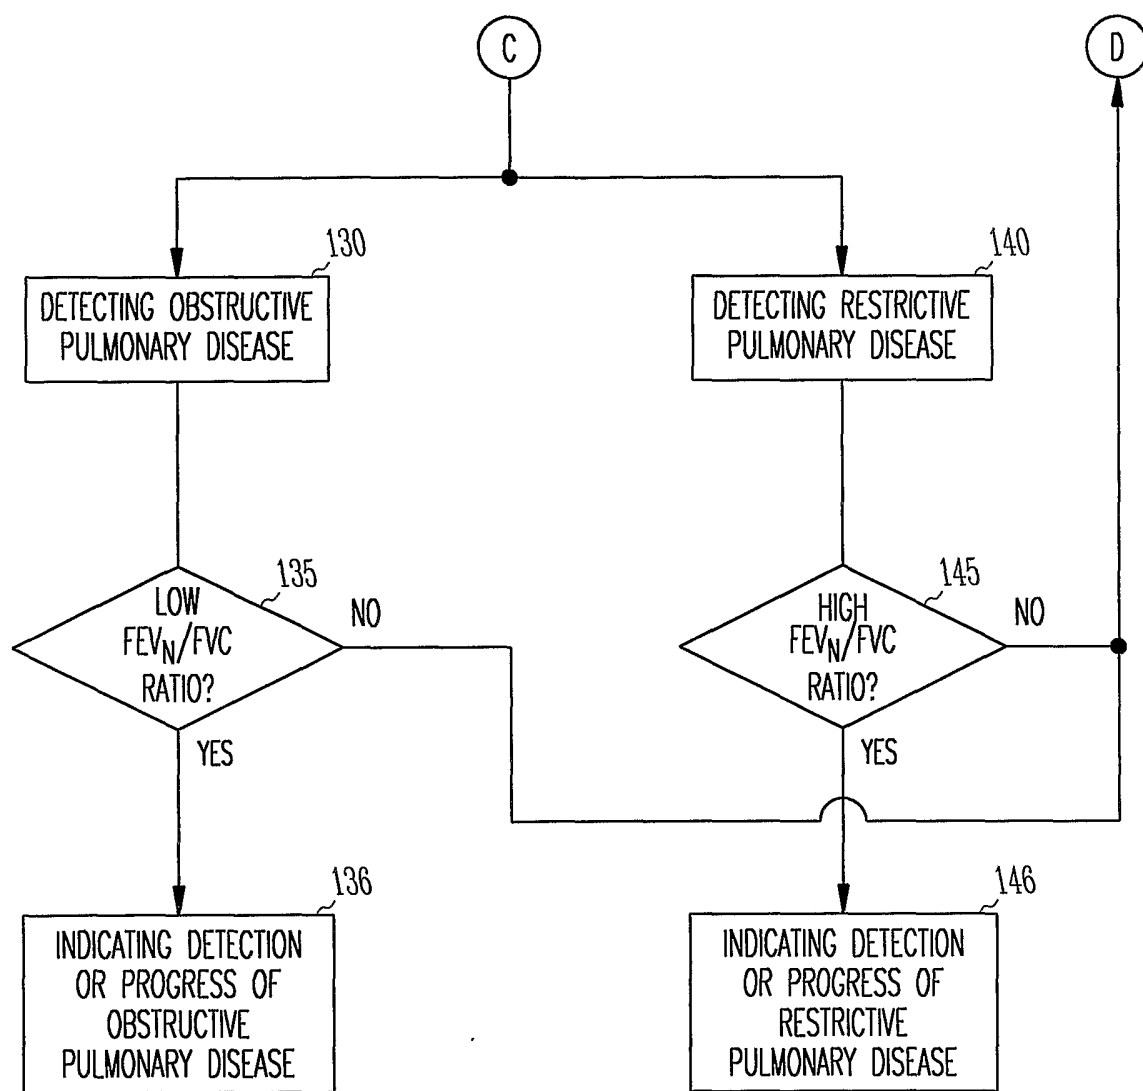


Fig.1C

4/10

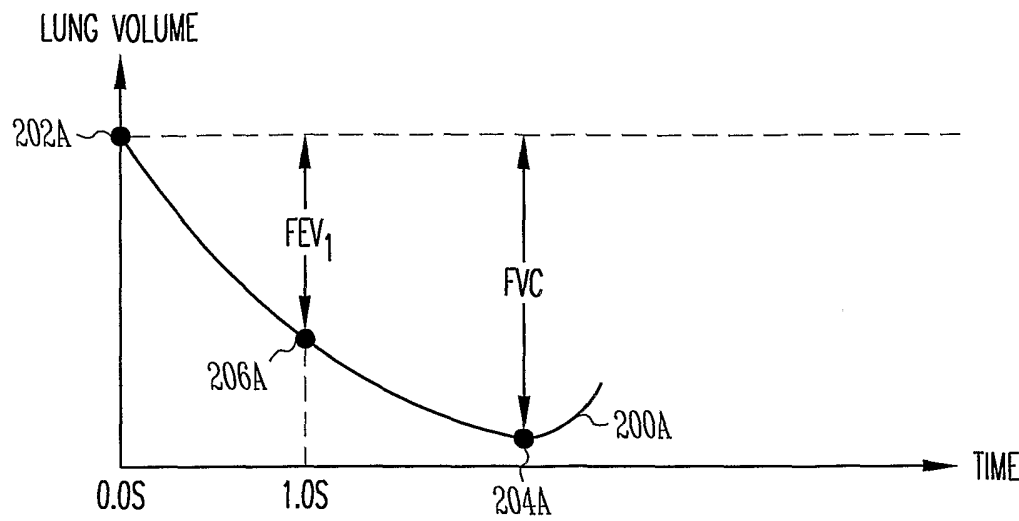


Fig.2A

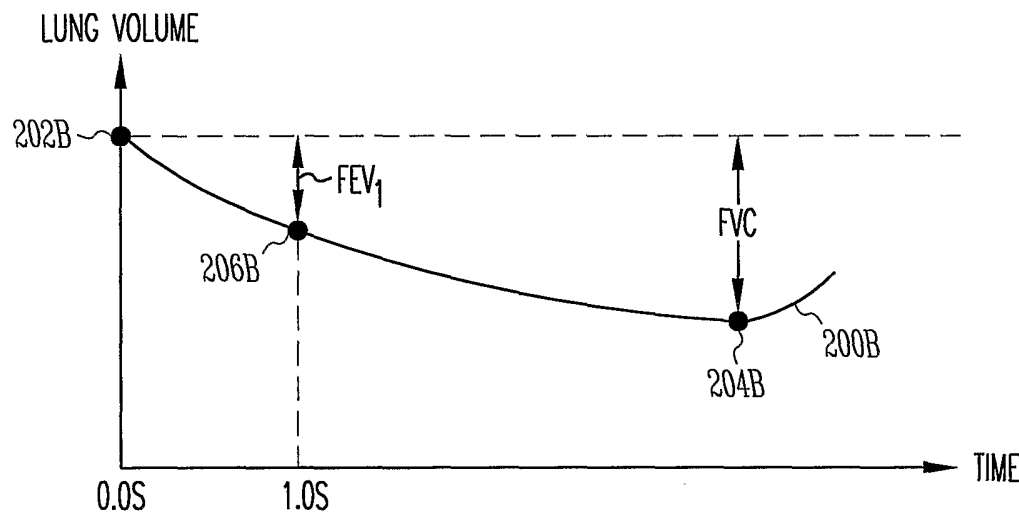


Fig.2B

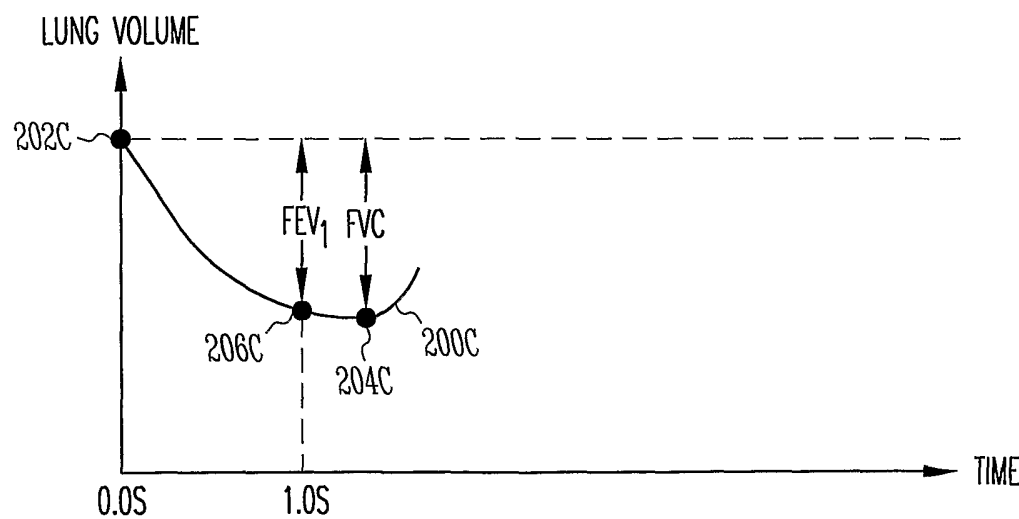


Fig. 2C

5/10

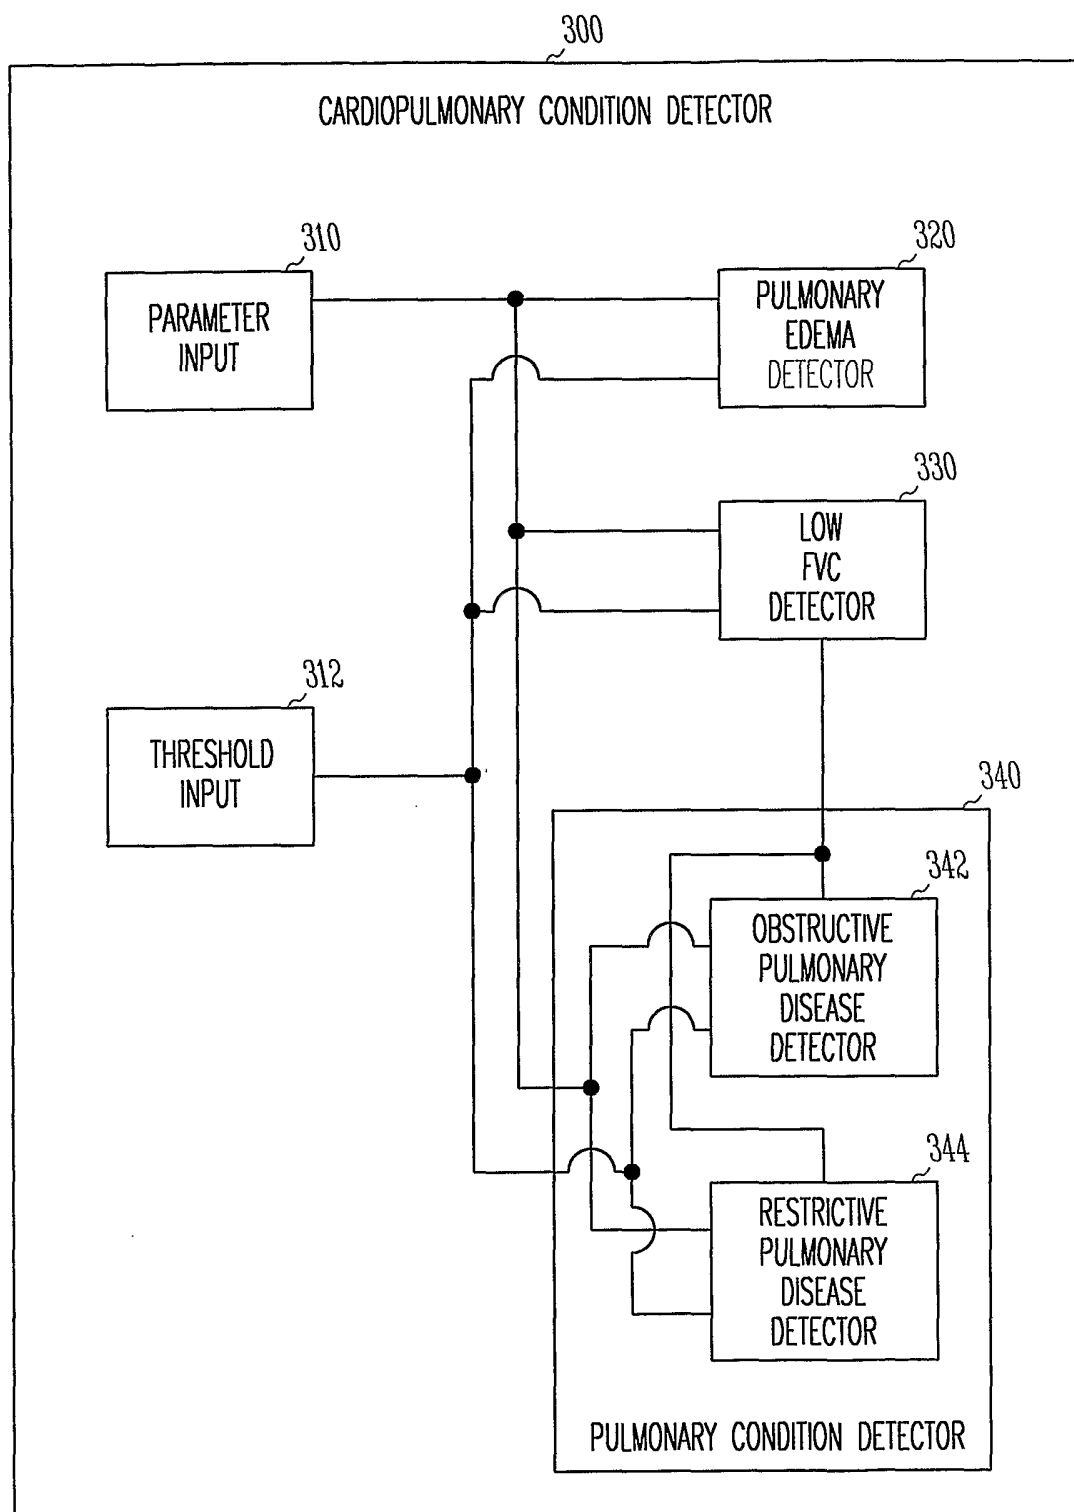


Fig.3

6/10

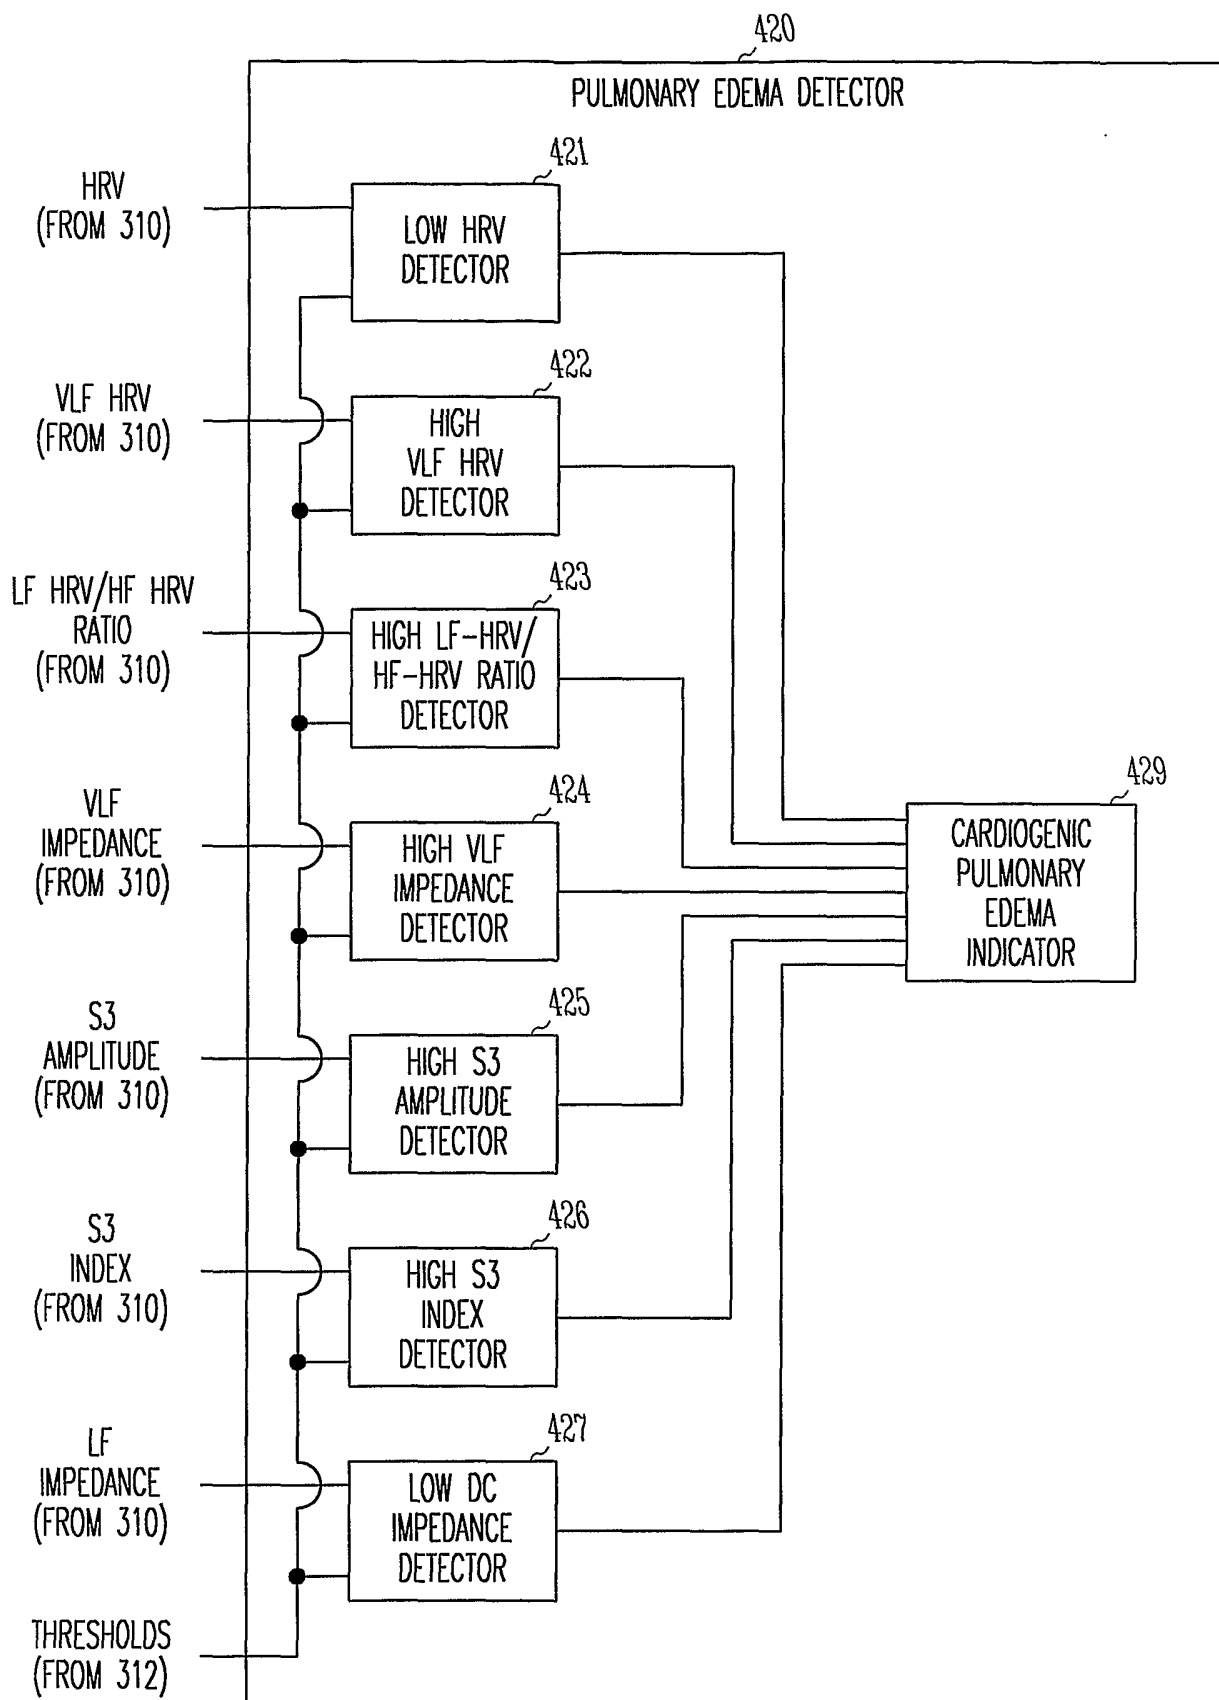


Fig.4

7/10

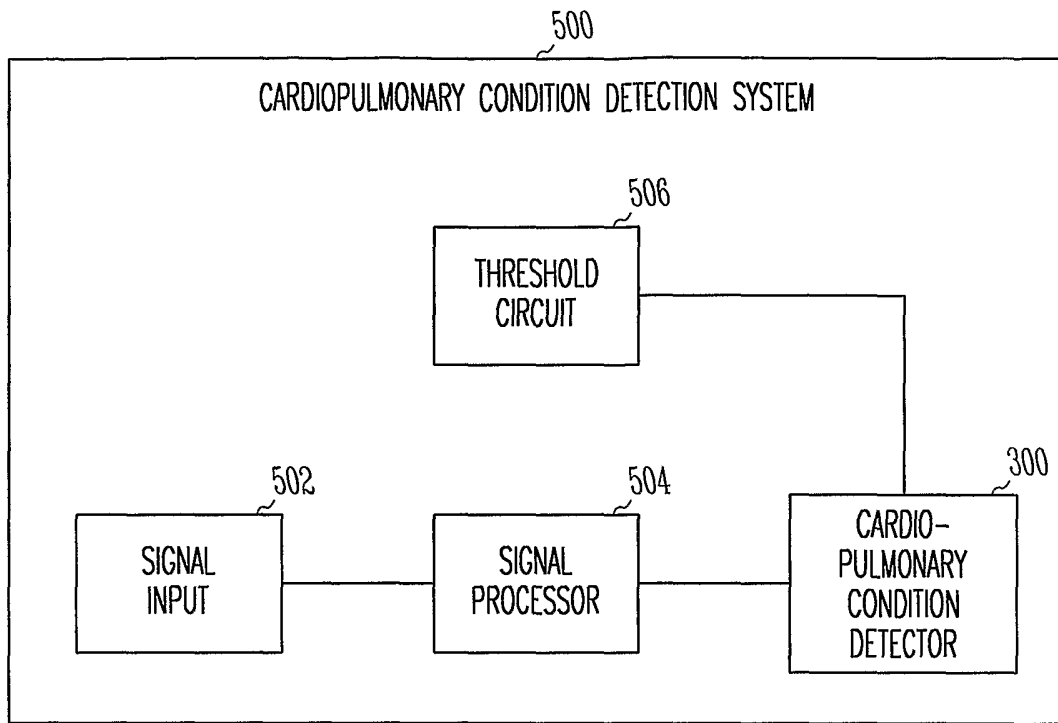


Fig.5

8/10

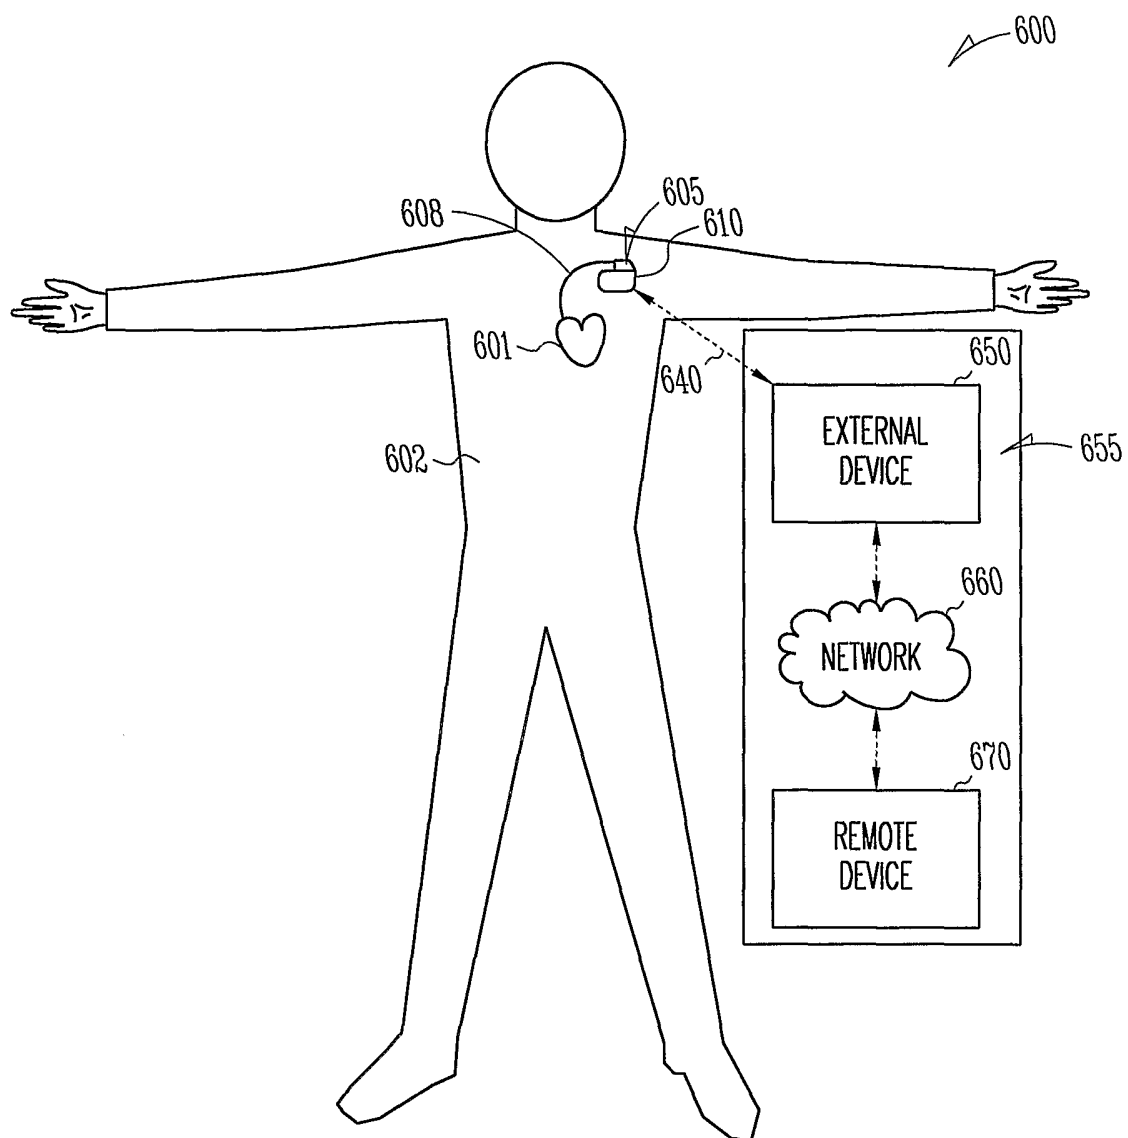


Fig.6

9/10

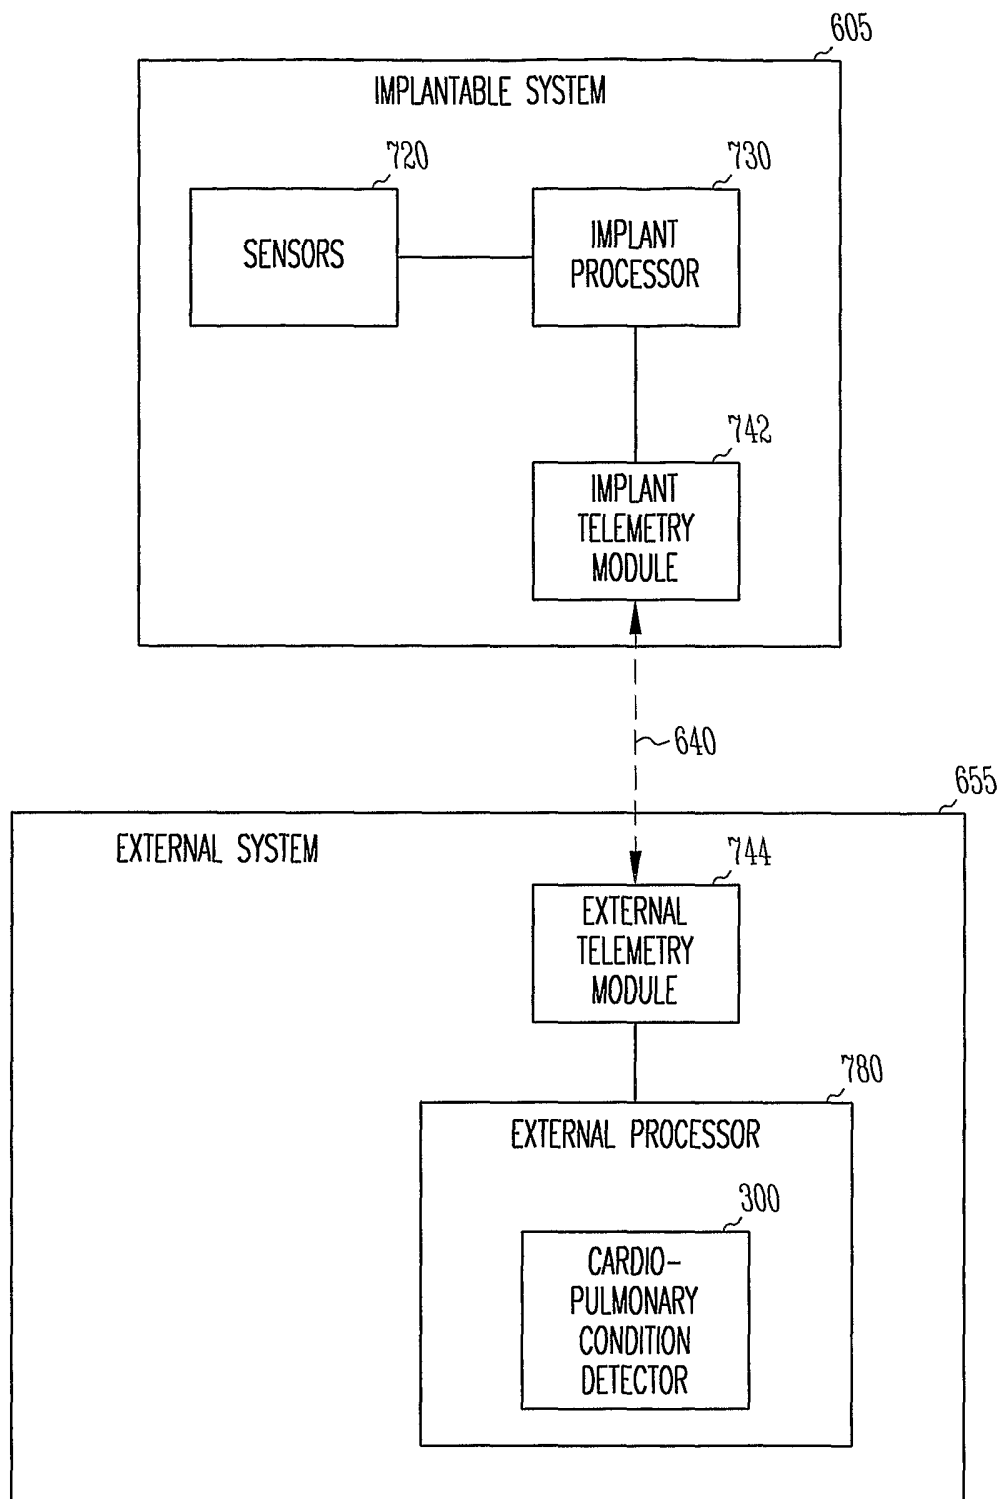


Fig.7

10/10

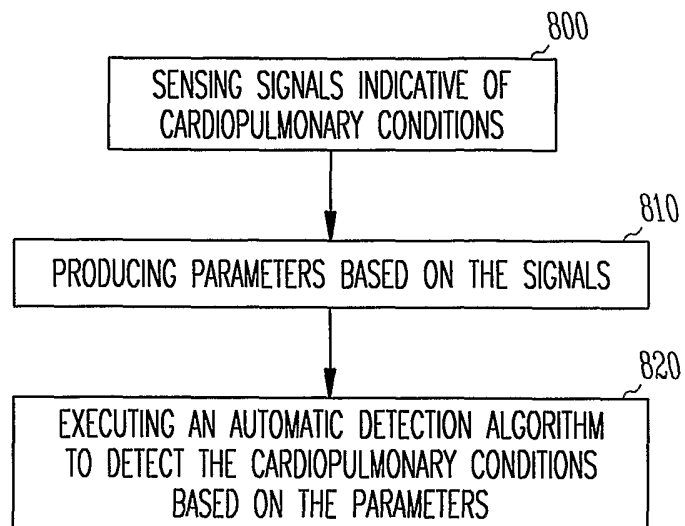


Fig.8